

## Certificate of Calibration

**Certificate No. :** 63-400281-1

**Page : 1 of 2**

**Submitted by :** Special Lab Envi and Consultant Co., Ltd.  
47/91 Moo 3, Tambol Tha-it, Pakkret, Nonthaburi 11120

**Equipment :** Digital Thermometer with TC probe  
Temperature Indicator  
Manufacturer : Thermo Scientific Model : TEMP 10K  
Range : -250 °C to 1372 °C Resolution : 0.1 °C  
Serial No. : 4008958 ID No. : SL-38

**Environment :** Ambient Temperature :  $(23 \pm 2)$  °C  
Relative Humidity :  $(50 \pm 15)$  %  
Line Voltage :  $(220 \pm 22)$  VAC

**Date of Received :** 30 May 2020

**Date of Calibration :** 04 June 2020

**Date of Issue :** 04 June 2020

**Calibrated by :** Bunjerd Masri

**Calibration Method :** This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units

### 1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0016-20	04 Mar 2022	National Institute of Metrology Thailand (NIMT)
400016	TT-0058-19	07 May 2021	National Institute of Metrology Thailand (NIMT)

### 2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	19E134	06 Jun 2021	National Institute of Metrology Thailand (NIMT)
400004	19E134	06 Jun 2021	National Institute of Metrology Thailand (NIMT)

Approved by :



( Surachai Promthong )  
Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

## Certificate of Calibration

**Certificate No. : 63-400281-1****Page : 2 of 2****Result of Calibration :** Without Adjustment**UUC Condition As-Received :** Good**Function :** Temperature measurement with Thermocouple probe Type K

Model : Type K                      Sheath Material : Teflon  
Diameter : 2 mm.                      Length : 1500 mm.  
Serial No. : N/A                      ID No. : SL-39

Immersion Depth ( mm. )	Standard Reading ( °C )	UUC Reading ( °C )	Correction ( °C )	Uncertainty ( ± °C )
130	4.0024	4.6	-0.6	0.18
130	104.0005	104.2	-0.2	0.45
130	150.0033	150.0	0.0	0.58
130	180.0009	179.8	0.2	0.65

Model : AD-1218-230                      Sheath Material : Stainless  
Diameter : 3.5 mm.                      Length : 230 mm.  
Serial No. : N/A                      ID No. : SL-40

Immersion Depth ( mm. )	Standard Reading ( °C )	UUC Reading ( °C )	Correction ( °C )	Uncertainty ( ± °C )
124	250.0027	250.3	-0.3	1.2
124	380.0030	379.0	1.0	1.5

**Remark**

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ ,  
providing a level of confidence of approximately 95%

- 000 -



## Certificate of Calibration

**Certificate No. :** 63-200136-1

**Page : 1 of 2**

**Submitted by :** Special Lab Envi and Consultant Co., Ltd.  
47/91 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

**Equipment :** Electronic Balance  
Manufacturer : AND Model : GR-200  
Serial No. : 14245322  
Capacity : 210 g Resolution : 0.0001 g

**Environment :** On site calibration was carried out at the Laboratory,  
Special Lab Envi and Consultant Co., Ltd.

Ambient Temperature : (27.0 to 27.4) °C  
Relative Humidity : (51.1 to 53.0) %  
Air Pressure : 1011.0 mbar

**Date of Received :** 04 May 2020

**Date of Calibration :** 04 May 2020

**Date of Issue :** 15 May 2020

**Calibrated by :** Akaradath Thippichai

**Calibration Method :** In-house method CAL-M2001 based on UKAS Publication ref : LAB 14  
Edition 5, July 2015

**Reference Standard Instruments :** This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02192873	14 Nov 2020	National Institute of Metrology (Thailand), (NIMT)

Approved by :



( Surachai Promthong )

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



## Certificate of Calibration

**Certificate No. : 63-200136-1**

**Page : 2 of 2**

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty $\pm$ (g)
0.001	0.0001	0.00011
0.01	0.0001	0.00011
0.1	0.0001	0.00011
0.5	-0.0001	0.00011
2	0.0000	0.00011
5	-0.0001	0.00012
10	0.0000	0.00012
50	0.0000	0.00014
100	0.0000	0.00020
200	-0.0001	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2.11$ , providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A	B	C	D	E
-0.0005	0.0001	0.0004	-0.0002	0.0000

g



Repeatability

Load test : 200 g

Stdev. : 0.00005 g

- oOo -

## Certificate of Calibration

**Certificate No. :** 63-400218-3

**Page : 1 of 2**

**Submitted by :** Special Lab Envi and Consultant Co., Ltd.  
47/91 Moo 3 Thambol Tha-it, Pakkret, Nonthaburi 11120

**Equipment :** Air Chamber (Incubator)  
Manufacturer : Lovibond Model : FKU 1800  
Range : N/A °C Resolution : 0.1 °C  
Serial No. : 0914643-01 ID No. : N/A

**Environment :** On site calibration was carried out at the Laboratory,  
Special Lab Envi and Consultant Co., Ltd.  
Ambient Temperature : (27.4 to 28.0) °C  
Relative Humidity : (45 to 55) %  
Line Voltage : (226.0 to 226.5) V

**Date of Received :** 04 May 2020

**Date of Calibration :** 04 May 2020

**Date of Issue :** 04 May 2020

**Calibrated by :** Bunjerd Masri

**Calibration Method :** CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400022 & 400028	63-400107-1	29 Aug 2020	National Institute of Metrology Thailand (NIMT)

Approved by :



( Bunjerd Masri )

Supervisor

## Certificate of Calibration

**Certificate No. : 63-400218-3**


**Page : 2 of 2**

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

This instrument was setting air ventilation at position 0 (close)

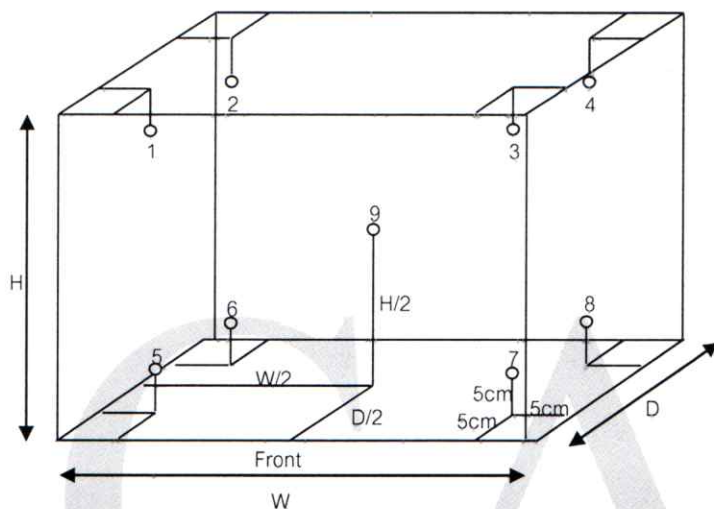

Inside of Chamber

W = 0.55 m

D = 0.73 m

H = 0.50 m

Capacity = 0.20 m<sup>3</sup>

Test Point ( ° C )	Setting Temperature ( ° C )	Indicating Temperature ( ° C )	Measured Temperature ( ° C ) @ Sensor No.									Uncertainty ( ± ° C )
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	20.0	19.8	20.0	20.0	20.0	19.9	20.2	20.2	20.1	0.77

Test Point ( ° C )	Setting Temperature ( ° C )	Indicating Temperature ( ° C )	Measured Uniformity ( ° C )	Measured Stability ( ° C )	Overall Variation ( ° C )
20.0	20.0	20.0	0.5	0.5	1.3

**Remark** The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- o0o -





MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkac Bangkok 10160  
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



## CALIBRATION CERTIFICATE

Certificate No. : AD2006-146-0001

Date Issued : 15-Jun-20

**Customer** : SPECIAL LAB ENVI AND CONSULTANT CO.,LTD.  
47/91 Moo 3, Tha-It, Pak Kret, Nonthaburi 11120

**Equipment** : Hot Air Oven

**Manufacturer** : Memmert

**Model** : UN30

**Serial No.** : B120.0284

**ID No./Tag No.** : -

**Date Received** : 12-Jun-20

**Date Calibrated** : 13-Jun-20

**Calibrated by** : Mr. Surat Aumarb

### Calibration Method or Calibration Procedure Used

Standard method : CP-05 TLAS G-20.


This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

### Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Technical Manager, Miracle International Technology Company Limited.

Approved by :

  
( Mr. Tassanai Suksukon )  
Technical Manager



Page 1 of 2

Certificate No. : AD2006-146-0001

Environment : Ambient Temperature : (25 ± 2)°C  
Relative Humidity : (50 ± 15)%RH


Calibration Temperature (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Stability <sup>1</sup> (°C)	Measured Uniformity <sup>2</sup> (°C)	Overall Variation <sup>3</sup> (°C)
104	104.0	104.0	0.18	0.42	0.92
150	150.0	150.0	0.35	0.45	1.11
180	180.0	180.0	0.44	0.47	0.88

Without adjustment

Calibration Temperature (°C)	STD No. 1 (°C)	STD No. 2 (°C)	STD No. 3 (°C)	STD No. 4 (°C)	STD No. 5 (°C)	STD No. 6 (°C)	STD No. 7 (°C)	STD No. 8 (°C)	STD No. 9 (°C)	Uncertainty <sup>4</sup> ±°C
104	104.32	104.12	103.80	104.33	103.98	103.93	104.01	104.42	104.13	0.95
150	149.93	149.62	149.49	149.80	149.63	149.41	149.48	149.91	149.71	1.0
180	179.45	179.35	179.45	179.18	179.42	179.44	179.32	179.32	179.35	1.1

Note : Probe No. 9 is Reference Probe

Setting Air Fresh No. 0

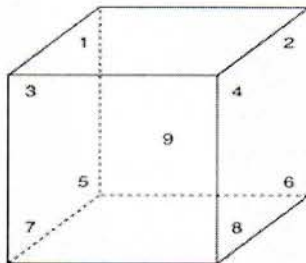

#### Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L2002-197 for Digital Thermometer with Probe (Agilent) Module 2 (08) TC Serial No. MY44000197,  
Due 26-Sep-20

Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.

2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.

3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The uncertainty of measurement is included temperature stability.

5. The temperature uniformity, stability, overall variation and indicating temperature is applicable to all air or gas filled temperature controlled enclosures at atmospheric pressure.

End of Certificate

*[Signature]*

Page 2 of 2






TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 20CH776

Page.: 1 of 3

## Certificate of Calibration

**Equipment :** pH Meter  
**Manufacturer :** Horiba  
**Model :** LAQUAact-PH130  
**Serial No. :** D08C0004  
**ID No. :** -  
**Condition As-Received:** Used Item  
**Received Date :** 01 June 2020  
**Calibration Date :** 02 June 2020  
**Reference :** 2006-0059WN-1  
**Submitted by :** Special Lab Envi And Consultant Co.,Ltd  
47/91 Moo 3, Thambon Tha-it, Pakkret  
Nonthaburi 11120  
  
**Ambient Temperature :** (25 ± 2.5) °C  
**Relative Humidity :** (50 ± 15) %  
**Calibration Procedure :** In - house method :  
- CP-CH5 : based on direct measurement by  
using standard voltage calibrator and  
certified reference material (CRM)  
- CP-CH8 : based on comparison technique by  
comparison with reference standard thermometer  
  
**Calibrated by :** Uthen Kankawi  
  
**Approved by :**   
Approved Signatory  
  
( ) Pornthippa Tameyakul  
( ☒ ) Malee Butkruea  
( ) Saithip Meangmai  
  
**Issue Date :** 9 June 2020

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0015301



Cert.No.: 20CH776

Page.: 2 of 3

**Condition of this calibration result**

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	753	43160066	130RC092	20E1369	15 Apr 2021
2) Ref. Standard Thermometer	1523	2188080	130RC044	19I1510	27 Nov 2020

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	677227	12 Mar 2022
pH 6.866	CPA chem	679462	12 Mar 2022
pH 9.176	CPA chem	670695	20 Dec 2020

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results****Function : mV Measurement****Performing standard curve by Fluke at pH (4,7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( ±mV )	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: D08C0004	4.00	177.48	177	4.00	0.58	2.00
	6.86	8.28	8	6.86	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	9.18	-128.97	-129	9.18	0.58	2.00
	10.00	-177.48	-178	10.00	0.58	2.00

Maku



Cert.No.: 20CH776

Page.: 3 of 3

### Calibration Results

#### Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,9)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading ( mV )	Uncertainty of pH measurement ( $\pm$ )	Coverage factor $k$
pH Electrode S/N.: 988E0098	4.008	4.01	150	0.0085	2.05
	6.866	6.87	-18	0.011	2.09
	9.176	9.18	-145	0.013	2.05

#### Function : Temperature Measurement

##### ( \* ) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9651  
- Serial No. : 988E0098

Dimension of probe;

- Length : 18 mm.  
- Diameter : 102 mm.  
- Immersion Depth : 90 mm.

Calibration Point ( $^{\circ}\text{C}$ )	Standard Temperature ( $^{\circ}\text{C}$ )	UUC* Reading ( $^{\circ}\text{C}$ )	Error ( $^{\circ}\text{C}$ )	Uncertainty of measurement ( $\pm$ $^{\circ}\text{C}$ )	Coverage factor $k$
25.0	25.015	25.0	-0.015	0.20	2.00
30.0	30.004	30.0	-0.004	0.20	2.00
40.0	40.016	40.0	-0.016	0.20	2.00

Remark : - UUC\* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

malu.





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 20CH1254

Page.: 1 of 3

## Certificate of Calibration

Equipment : pH Meter  
Manufacturer : Eutech  
Model : pH 700  
Serial No. : 2858459  
ID No. : SL-33  
Condition As-Received: Used Item  
Received Date : 25 August 2020  
Calibration Date : 26 August 2020  
Reference : 2008-0964WN-1  
Submitted by : Special Lab Envi And Consultant Co.,Ltd  
47/91 Moo 3, Thambon Tha-it,  
Pakkret, Nonthaburi 11120  
Ambient Temperature : (25 ± 2.5) °C  
Relative Humidity : (50 ± 15) %  
Calibration Procedure : In - house method :  
- CP-CH5 : based on direct measurement by  
using standard voltage calibrator and  
certified reference material (CRM)

Calibrated by : Walalak Sirithean

Approved by :

Approved Signatory

- ( ) Pornthippa Tameyakul  
( ☒ ) Malee Butkruea  
( ) Saithip Meangmai

Issue Date : 28 August 2020

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0018380



Cert. No.: 20CH1254

Page.: 2 of 3

**Condition of this calibration result**

## 1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	753	46530031	130RC098	19E3994	10 Oct 2020

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through Merck Ltd.,  
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15185-01-00

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	Merck	HC99078000	31 May 2022
pH 6.866	Merck	HC99138402	31 May 2022
pH 9.183	Merck	HC99627703	31 May 2021

## 3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results****Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7,9)

<u>Unit Under Calibration</u>	<u>Standard pH Buffer Solution</u>	<u>Actual pH Reading</u>	<u>Actual mV Reading ( mV )</u>	<u>Uncertainty of pH measurement (±)</u>	<u>Coverage factor k</u>
pH Electrode S/N.: 2863304	4.007	4.01	173.3	0.011	2.00
	6.866	6.86	5.1	0.010	2.00
	9.183	9.18	-129.8	0.045	2.00

make





Cert.No.: 20CH1254

Page.: 3 of 3

**Calibration Results****Function : mV Measurement****Performing standard curve by Fluke at pH (4,7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( ±mV )	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: 2858459	0.00	414.12	414	0.02	0.58	2.00
	1.00	354.96	355	1.02	0.58	2.00
	2.00	295.80	296	2.02	0.58	2.00
	3.00	236.64	237	3.01	0.58	2.00
	4.00	177.48	177.4	4.01	0.058	2.00
	5.00	118.32	118.2	5.01	0.11	2.52
	6.00	59.16	59.1	6.00	0.058	2.00
	6.86	8.28	8.2	6.86	0.058	2.00
	7.00	0.00	0.0	7.00	0.058	2.00
	8.00	-59.16	-59.2	8.00	0.058	2.00
	9.00	-118.32	-118.3	9.01	0.058	2.00
	9.18	-128.97	-129.0	9.19	0.058	2.00
	10.00	-177.48	-177.5	10.01	0.058	2.00
	11.00	-236.64	-237	11.01	0.58	2.00
	12.00	-295.80	-296	12.02	0.58	2.00
	13.00	-354.96	-355	13.02	0.58	2.00
	14.00	-414.12	-414	14.02	0.58	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

Maku

a 1013829





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 20T1897

Page : 1 of 2

Equipment : pH Meter With Sensor

Manufacturer: Eutech

Model : pH 700

Serial No.: 2858459

ID No.: SL-33

Condition As-Received: Used Item

Received Date: 25 August 2020

Calibration Date: 27 August 2020  
to 28 August 2020

Reference: 2008-0964WN

Ambient Temperature: ( 25 ± 3 ) °C

Relative Humidity: ( 50 ± 20 ) %

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: Special Lab Envi And Consultant Co.,Ltd

47/91 Moo 3 Thambon Tha-it, Pakkret Nonthaburi 11120

Procedure used: Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with  
Platinum Resistance Thermometer (PRT) into liquid bath temperature controller.  
The temperature scale used was based on ITS-90.

### Condition of this result of calibration

1. Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Digital Thermometer	1529	A66176	1911397	01 Nov 2020
2) Platinum Resistanc Temperature	162 P	3683	1911397	01 Nov 2020


2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Theerapong Ameen

Issue Date : 01 September 2020

Approved Signatory : 

[ ] Phalinee Prabpaipal

[✓] Chatchawan Khunpiluek

[ ] Wanlop Larpkurn

B 0241421



Cert. No.: 20T1897

Page.: 2 of 2

**Result of Calibration:-**

Without Adjustment

**Function:**

Temperature measurement

This equipment was connected with Temperature Sensor ID No. SL-33/1

Dimension of probe : Diameter 3.5 mm., Length 115 mm. Sheath material : Stainless Steel

Immersion <u>Depth</u> ( mm.)	Standard <u>Temperature</u> ( °C )	UUC* <u>Reading</u> ( °C )	<u>Error</u> ( °C )	Uncertainty <u>of Measurement</u> ( ±°C )
100	25.0097	25.0	-0.0097	0.12

UUC\* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

-o0o-



## Certificate of Calibration

**Certificate No. :** 63-400218-4

**Page : 1 of 2**

**Submitted by :** Special Lab Envi and Consultant Co., Ltd.  
47/91 Moo 3 Thambol Tha-it Pakkret Nonthaburi 11120

**Equipment :** Air Chamber (Refrigerator)  
Manufacturer : Frozen Model : CC-280C  
Range : N/A °C Resolution : 0.1 °C  
Serial No. : 2081307016 ID No. : N/A

**Environment :** On site calibration was carried out at the Laboratory,  
Special Lab Envi and Consultant Co., Ltd.  
Ambient Temperature : (30.0 to 31.3) °C  
Relative Humidity : (50 to 55) %  
Line Voltage : (226.0 to 226.5) V

**Date of Received :** 04 May 2020

**Date of Calibration :** 04 May 2020

**Date of Issue :** 04 May 2020

**Calibrated by :** Bunjerd Masri

**Calibration Method :** CAL-M4004, TLAS G-20  
The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400022 & 400023	63-400104-1	29 Aug 2020	National Institute of Metrology Thailand (NIMT)

Approved by :



( Bunjerd Masri )

Supervisor



## Certificate of Calibration

**Certificate No. : 63-400218-4**


**Page : 2 of 2**

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

This instrument was setting air ventilation at position 0 (close)

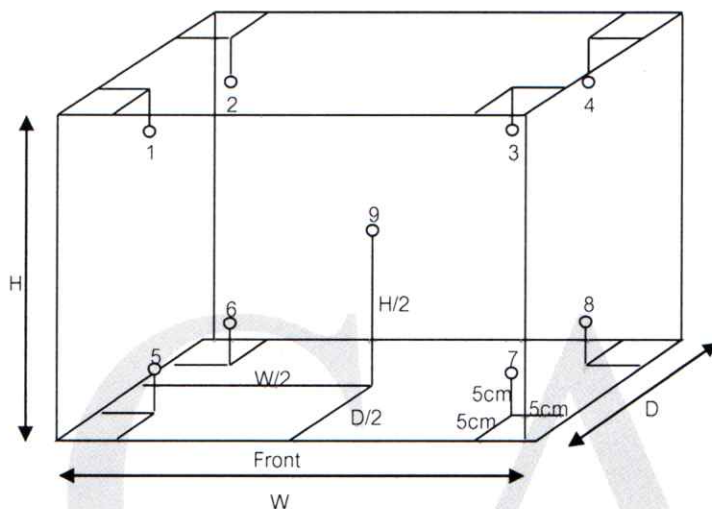

Inside of Chamber

W = 1.02 m

D = 0.47 m

H = 1.48 m

Capacity = 0.71 m<sup>3</sup>

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
4.0	4.0	4.0	3.9	4.3	3.7	3.6	4.2	4.6	3.6	3.5	3.9	0.63

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
4.0	4.0	4.0	0.8	0.3	1.5

**Remark** The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- o0o -



**BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.**  
**CALIBRATION LABORATORY**

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1  
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-20-293

Page : 1 of 3

## CERTIFICATE OF CALIBRATION

Equipment	:	Spectrophotometer
Manufacturer	:	Thermo Scientific
Model	:	Genesys 20
Serial No.	:	3SGT041007
ID No.	:	SL-34
Customer	:	Special Lab Envi And Consultant Co.,Ltd.
	:	47/91 Moo 3, Tambol Tait , Amphur Pakrad,
	:	Nonthaburi, 11120.
Location	:	Becthai Laboratory
Date of Receipt	:	15 May 2020
Date of Calibration	:	15 May 2020
Date of Issue	:	15 May 2020
Ambient Temperature	:	(25±10) °C
Relative Humidity	:	(60±20) %
Condition As-Received	:	Used Item

Calibrated by

( Ms. Alisa Lamor )

Calibration Engineer

Approved by

( Ms. Jintana Sangthaijaroenlap )

Calibration Manager

The reported expended uncertainty of measurement was based on a combined standard uncertainty multiplied by a coverage factor  $k=2.00$ , providing a level of confidence of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Indicated values are valid for the state of the Spectrophotometer at the time of calibration only.



**BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.**  
**CALIBRATION LABORATORY**

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1  
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-20-293

Page : 2 of 3

## CALIBRATION REPORT

### Conditions of this result of calibration

#### 1. Reference Standard Material :

<u>Material</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert.No.</u>	<u>Due date</u>
Holmium Glass Filter	RM-HG	12705	81255	16 Jan 22
Neutral Density Filter	RM-1N2N3N	8323	81257	16 Jan 22

#### 2. Traceability : This certification is traceable to the International System of Unit maintained at;

The Starna Scientific Ltd. Accredited Calibration Laboratory No. 0659.

#### 3. Method of calibration :

The calibration procedure was carried out according to the Guide to CPM-CAL-02 based on ASTM E275-08 (2013) and-  
ASTM E925-09 (2014).

#### 4. Result of calibration :

( ☒ ) without adjustment

( ☐ ) after adjustment

#### 5. Equipment Specifications:

Spectral Bandwidth :	8	nm
Data Interval :	1	nm
Scan Speed :	N/A	nm/min





**BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.**  
**CALIBRATION LABORATORY**

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1  
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-20-293

Page : 3 of 3

## CALIBRATION REPORT

### Wavelength Calibration

Certified Values of Reference Material (nm)	Nominal Value (nm)	UUC*Reading (nm)	Error (nm)	Uncertainty of Measurement ( $\pm$ nm)
418.40	418	418	-0.40	0.59
537.00	537	537	0.00	0.59
638.00	638	639	1.00	0.59

### Photometric Calibration for Visible

Wavelength (nm)	Certified Values of Reference Material (A)	UUC* Reading (A)	Error (A)	Uncertainty of Measurement ( $\pm$ A)
420.0	Zero	0.000	0.0000	0.0028
	0.5717	0.575	0.0033	0.0033
	0.7341	0.736	0.0019	0.0036
	1.0726	1.077	0.0044	0.0032
440.0	Zero	0.000	0.0000	0.0028
	0.5611	0.562	0.0009	0.0032
	0.7168	0.716	-0.0008	0.0036
	1.0473	1.046	-0.0013	0.0032
465.0	Zero	0.000	0.0000	0.0028
	0.5114	0.515	0.0036	0.0032
	0.6610	0.664	0.0030	0.0035
	0.9651	0.968	0.0029	0.0032
546.1 (546.0)	Zero	0.000	0.0000	0.0028
	0.5233	0.522	-0.0013	0.0034
	0.6693	0.667	-0.0023	0.0032
	0.9796	0.977	-0.0026	0.0031
590.0	Zero	0.000	0.0000	0.0028
	0.5553	0.557	0.0017	0.0033
	0.6987	0.699	0.0003	0.0032
	1.0236	1.023	-0.0006	0.0030
635.0	Zero	0.000	0.0000	0.0028
	0.5411	0.541	-0.0001	0.0033
	0.6673	0.666	-0.0013	0.0032
	0.9771	0.976	-0.0011	0.0031

Remark : Each individual filter is measured against the empty filter holder (blank) used to zero the Spectrophotometer.

Note:

UUC\* : Unit Under Calibration

- End of Report -

## Certificate of Calibration

**Certificate No. :** 63-210407-2

**Page :** 1 of 2

**Submitted by :** Special Lab Envi and Consultant Co.,Ltd.  
47/91 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

**Equipment :** Weight  
Manufacturer : LS Material : Stainless Steel  
Weight size : 100 g  
ID No. : 60-210017-2  
Assumed density of weight : 7950 kg / m<sup>3</sup>  
Assumed Air density : 1.2 kg / m<sup>3</sup>

**Environment :** Ambient Temperature : ( 20 ± 2 ) °C  
Relative Humidity : ( 50 ± 10 ) %  
Air Pressure : 1004.2 mbar

**Date of Received :** 22 August 2020

**Date of Calibration :** 27 August 2020

**Date of Issue :** 27 August 2020

**Calibrated by :** Chanakan Pongsuwan

**Calibration Method :** In-house method CAL-M2101 based on OIML R 111-1 : 2004(E)

**Reference Standard Instruments :** This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E2413-E2425	MM-0060-19	27 Mar 2022	National Institute of Metrology (Thailand), (NIMT)

Approved by :



( Surachai Promthong )

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.





## Certificate of Calibration

**Certificate No. :** 63-210407-2

**Page :** 2 of 2

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

No.	Nominal Value	Id.Mark	Conventional mass Value		Measuring Uncertainty
1	100 g	none	100 g	-0.20 mg	$\pm$ 0.11 mg

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- oOo -

