

ภาคผนวกที่ 4

เอกสารการสอบเทียบความถูกต้องของเครื่องมือตรวจวัด
ผลกระทบสิ่งแวดล้อม



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3095

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B35	B35	06/08/2021	$y = 1.248x - 7.308$	0.996
B36	B36	06/08/2021	$y = 1.152x - 3.289$	0.995
B37	B37	06/08/2021	$y = 1.222x - 6.513$	0.998
B38	B38	09/08/2021	$y = 1.077x + 1.166$	0.995
B39	B39	09/08/2021	$y = 1.191x - 4.066$	0.997
B40	B40	09/08/2021	$y = 1.163x - 2.019$	0.998
B41	B41	09/08/2021	$y = 1.232x - 6.522$	1.000
B42	B42	09/08/2021	$y = 1.160x - 3.393$	0.997
B43	B43	09/08/2021	$y = 1.147x - 2.446$	1.000
B44	B44	09/08/2021	$y = 1.104x + 0.039$	0.999
R01	R01	02/08/2021	$y = 1.167x - 3.057$	0.995
R02	R02	02/08/2021	$y = 1.260x - 7.471$	0.999
R03	R03	02/08/2021	$y = 1.137x - 2.420$	0.996
R04	R04	02/08/2021	$y = 1.088x - 0.128$	0.998
R05	R05	02/08/2021	$y = 1.280x - 9.691$	0.999
R06	R06	02/08/2021	$y = 1.126x - 1.876$	0.997
R07	R07	03/08/2021	$y = 1.168x - 3.672$	0.996
R08	R08	03/08/2021	$y = 1.127x - 2.139$	0.999
R09	R09	03/08/2021	$y = 1.165x - 2.521$	0.998
R10	R10	03/08/2021	$y = 1.190x - 5.059$	0.995
R11	R11	03/08/2021	$y = 1.124x - 0.805$	0.996
R12	R12	03/08/2021	$y = 1.155x - 2.793$	1.000
R13	R13	03/08/2021	$y = 1.216x - 5.035$	0.995
R14	R14	04/08/2021	$y = 1.159x - 2.966$	0.997
R15	R15	04/08/2021	$y = 1.116x - 1.989$	0.997
R16	R16	04/08/2021	$y = 1.203x - 6.021$	0.997
R17	R17	04/08/2021	$y = 1.194x - 5.299$	0.999
R18	R18	05/08/2021	$y = 1.173x - 3.570$	0.997
R19	R19	05/08/2021	$y = 1.135x - 1.276$	1.000
R20	R20	05/08/2021	$y = 1.145x - 3.531$	0.997

Calibrated by :

Phakhinai Khongkomnerd

(Mr. Phakhinai Khongkomnerd)

Approved by :

Peera Detudom

(Mr. Peera Detudom)

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.comNSC-TISI-TISI7025
CALIBRATION 0049

CERTIFICATE No : 21M3169

REFERENCE No : 60627-5

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 19-Mar-21

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 20-Mar-21

RECEIVED DATE : 19-Mar-21

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 21M3169

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 19-Mar-21
AIR PRESSURE : 1009mbar \pm 1mbar CALIBRATION DATE : 19-Mar-21
AMBIENT TEMPERATURE : 24°C \pm 1°C RELATIVE HUMIDITY : 52 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING WEIGHT OF QUALITY CALIBRATION TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23
2) STANDARD WEIGHT	E2	15843	C02210419	10-Feb-23
3) STANDARD WEIGHT	E2	QK-I-349	M2103235S	26-Mar-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT


1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 100 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000066
0.02	0.01998	0.00002	0.000066
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000067
0.50	0.49996	0.00004	0.000065
1.00	0.99997	0.00003	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00003	-0.00003	0.000070
20.00	20.00000	0.00000	0.000075
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0001	-0.0001	0.00022

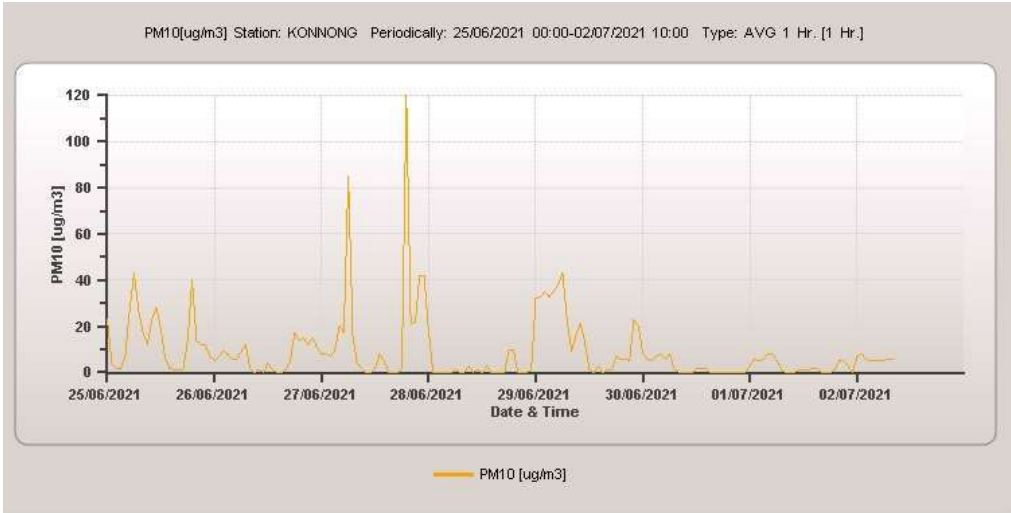
5. OFF CENTER LOADING ERROR

POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

Daily Check on 01/07/21 'Morning (01/07/21 00.00am. to 02/07/21 08.00am.)	
Station	Data & Calibration
Housing	<ul style="list-style-type: none"> - PM10 ค่า Reading drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (5 ชม.) - Off Auto-Cal.
Pluak Gate	<ul style="list-style-type: none"> - ข้อมูลโดยรวมอยู่ในเกณฑ์ปกติ - Rain : ฝนตก 01/07/21 ช่วงเวลา 23.00น. ถึง 02/07/21 เวลา 08.00น. - 01/07/21 (23.00น.) Auto-cal. ปกติทุกเครื่อง
Techno	<ul style="list-style-type: none"> - VOC : ทำงานปกติ (เฉพาะพารามิเตอร์ที่เปิดใช้งาน) - Rain 'Down' - 01/07/21 (20.00น.) Auto-cal. ปกติทุกเครื่อง
Ban Lang	<ul style="list-style-type: none"> - ข้อมูลโดยรวมอยู่ในเกณฑ์ปกติ - Rain 'Down' - 01/07/21 (20.00น.) Auto-cal. ปกติทุกเครื่อง
Ban Konnong ติดตั้ง EDM (PM10) 24/03/21 *ตรวจเช็ค/แก้ไข*	<ul style="list-style-type: none"> - PM10 ค่า Reading ต่ำผิดปกติ ค่าอยู่ 0-8 ug/m3  <ul style="list-style-type: none"> - WS โข้ว Flag <Samp ในบางชั่วโมง (4 ชม.) - SRAD ค่า Reading ช่วงกลางคืน อยู่ที่ (-4) – (-2) watt/m2 - Rain : ฝนตก 01/07/21 ช่วงเวลา 23.00น. ถึง 02/07/21 เวลา 08.00น. - 01/07/21 (21.00น.) Auto-cal. ปกติทุกเครื่อง
Bus AQMs	ปิดระบบฯ / CSR
Micro1	- ปิดระบบฯ 29/06/21 เวลา 10.00น. จอดอยู่ที่ CSR
Micro 2	- <u>ปิดระบบฯ</u> อยู่ที่ CSR
Micro 3 (CSR)	<ul style="list-style-type: none"> - <u>เริ่มตรวจวัดฯ 29/06/21 เวลา 10.00น.</u> - PM10 ค่า Reading drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (3 ชม.) - WS/WD โข้ว Flag <Samp เป็นช่วงๆ (6 ชม.)

Daily Check on 04/07/21 `Morning (04/07/21 00.00am. to 05/07/21 08.00am.)	
Station	Data & Calibration
Housing <i>*ตรวจเช็ค/แก้ไข*</i>	- PM10 ค่า Reading swing และค่า Drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (6 ชม.)
	- Off Auto-Cal.
Pluak Gate	- NO-NO2-NOx, SO2 ค่า Reading ค่อนข้างสูง
	- 05/07/21 (02.00น.) Auto-cal. ปกติทุกเครื่อง
Techno <i>*ตรวจเช็ค/แก้ไข*</i>	- NO-NO2-NOx ค่า Reading สูง 04/07/21 เวลา 18.00-22.00น.
	- NMHC ค่า Reading อยู่ที่ 0.0 ในบางชั่วโมง
	- PM10 ค่า Reading อยู่ที่ 0 ug/m3 & Over range ตั้งแต่ 04/07/21 เวลา 13.00น.ถึงปัจจุบัน
	- PM2.5 ค่า Reading swing และ Drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (3 ชม.)
	- VOC : ทำงานปกติ (เฉพาะพารามิเตอร์ที่เปิดใช้งาน)
	- Rain 'Down'
	- 04/07/21 (11.00น.) Auto-cal. ปกติทุกเครื่อง
Ban Lang	- PM10 ค่า Reading swing และค่า Drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (3 ชม.)
	- Rain 'Down'
	- 04/07/21 (23.00น.) Auto-cal. ปกติทุกเครื่อง
Ban Konnong ติดตั้ง EDM (PM10) 24/03/21 <i>*ตรวจเช็ค/แก้ไข*</i>	- PM10 ค่า Reading swing และ Drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (6 ชม.)
	- WS โชนว Flag <Samp ในบางชั่วโมง (8 ชม.)
	- SRAD ค่า Reading ช่วงกลางคืน อยู่ที่ (-5) – (-2) watt/m2
	- 05/07/21 (21.00น.) Auto-cal. ปกติทุกเครื่อง
Bus AQMs	ปิดระบบฯ / CSR
Micro1	- ปิดระบบฯ 29/06/21 เวลา 10.00น. จอดอยู่ที่ CSR
Micro 2	- ปิดระบบฯ อยู่ที่ CSR
Micro 3 (CSR)	- เริ่มตรวจวัดฯ 29/06/21 เวลา 10.00น.
	- PM10 ค่า Reading swing และค่า Drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (3 ชม.)

Daily Check on 05/07/21 'Morning (05/07/21 00.00am. to 06/07/21 08.00am.)	
Station	Data & Calibration
Housing	- PM10 ค่า Reading swing และค่า Drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (3 ชม.)
	- Off Auto-Cal.
Pluak Gate	- NO-NO2-NOx, SO2 ค่า Reading สูง ในบางชั่วโมง
	- Rain : ฝนตก ช่วงเช้า 06/07/21
	- 06/07/21 (16.00น.) Auto-cal. ปกติทุกเครื่อง
Techno	- PM10, PM2.5 : จนท. ซ่อมแซมฯ เรียบร้อย
	- VOC : ทำงานปกติ (เฉพาะพารามิเตอร์ที่เปิดใช้งาน)
	- Rain 'Down'
	- 06/07/21 (10.00น.) Auto-cal. ปกติทุกเครื่อง
Ban Lang	- ข้อมูลโดยรวมอยู่ในเกณฑ์ปกติ
	- Rain 'Down'
	- 05/07/21 (12.00น.) Auto-cal. ปกติทุกเครื่อง
Ban Konnong ติดตั้ง EDM (PM10) 24/03/21	- WS โഴว์ Flag <Samp ในบางชั่วโมง (3 ชม.)
	- SRAD ค่า Reading ช่วงกลางวัน อยู่ที่ (-5) – (0) watt/m2
	- Rain : ฝนตกช่วงเช้า 06/07/21
	- 06/07/21 (01.00น.) Auto-cal. ปกติทุกเครื่อง
Bus AQMs	ปิดระบบฯ / CSR
Micro1	- ปิดระบบฯ 29/06/21 เวลา 10.00น. จอดอยู่ที่ CSR
Micro 2	- ปิดระบบฯ อยู่ที่ CSR
Micro 3 (CSR)	- เริ่มตรวจวัดฯ 29/06/21 เวลา 10.00น.
	- PM10 ค่า Reading swing
	- WS/WD โ Zhou Flag <Samp ในบางชั่วโมง (6 ชม.)

Daily Check on 06/07/21 'Morning (06/07/21 00.00am. to 07/07/21 08.00am.)	
Station	Data & Calibration
Housing	- PM10 ค่า Reading swing และค่า Drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (2 ชม.)
	- Off Auto-Cal.
Pluak Gate	- NO-NO2-NOx, SO2 ค่า Reading สูง ในบางชั่วโมง
	- Rain : ฝนตก ในช่วง 6-7/07/21
	- 06/07/21 (15.00น.) Auto-cal. ปกติทุกเครื่อง
Techno	- VOC : ทำงานปกติ (เฉพาะพารามิเตอร์ที่เปิดใช้งาน)
	- Rain 'Down'
	- 06/07/21 (11.00น.) Cal. O3 zero = 5 span = 0.4
Ban Lang	- ข้อมูลโดยรวมอยู่ในเกณฑ์ปกติ
	- Rain 'Down'
	- 06/07/21 (12.00น.) Auto-cal. ปกติทุกเครื่อง
Ban Konnong ติดตั้ง EDM (PM10) 24/03/21 *ตรวจเช็ค/แก้ไข*	- PM10 ค่า Reading swing และค่า Drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (5ชม.)
	- WS ค่า Reading ค้าง อยู่ที่ 0.3 m/s ตั้งแต่ 06/07/21 – ถึงปัจจุบัน
	- SRAD ค่า Reading ช่วงกลางคืน อยู่ที่ (-5) – (0) watt/m2
	- Rain : ฝนตกช่วงเช้า 06/07/21
	- 07/07/21 (02.00น.) Auto-cal. ปกติทุกเครื่อง
Bus AQMs	ปิดระบบฯ / CSR
Micro1	- ปิดระบบฯ 29/06/21 เวลา 10.00น. จอดอยู่ที่ CSR
Micro 2	- ปิดระบบฯ อยู่ที่ CSR
Micro 3 (CSR)	- <u>เริ่มตรวจวัดฯ 29/06/21 เวลา 10.00น.</u>
	- PM10 ค่า Reading swing และ Drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (3 ชม.)
	- WS/WD โชน์ Flag <Samp ในบางชั่วโมง (4 ชม.)

Daily Check on 07/07/21 'Morning (07/07/21 00.00am. to 08/07/21 08.00am.)	
Station	Data & Calibration
Housing	- PM10 ค่า Reading Drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (3 ชม.)
	- Off Auto-Cal.
Pluak Gate	- NO-NO2-NOx, SO2 ค่า Reading สูง ในบางชั่วโมง
	- Rain : ฝนตก 07/07/21 เวลา 00.00-01.00น.
	- 07/07/21 (16.00น.) Auto-cal. ปกติทุกเครื่อง
Techno	- CO ค่า Reading ค้างอยู่ที่ 0.3 ppm ตลอด 24 ชม.
	- VOC : ทำงานปกติ (เฉพาะพารามิเตอร์ที่เปิดใช้งาน)
	- Rain 'Down'
	- 07/07/21 (12.00น.) Auto-cal. ปกติทุกเครื่อง
Ban Lang	- PM10 ค่า Reading swing และค่า Drop อยู่ที่ 0,1 ug/m3 ในบางชั่วโมง (4 ชม.)
	- Rain 'Down'
	- 07/07/21 (12.00น.) Cal. CO zero = 0.3 span=0.3
Ban Konnong ติดตั้ง EDM (PM10) 24/03/21	- PM10 ค่า Reading swing drop อยู่ที่ 0 ug/m3 07/07/21 เวลา 13.00-15.00น.
	- PM2.5 เริ่มตรวจวัด 07/07/21 เวลา 13.00น. ค่า Reading อยู่ 0-8 ug/m3 **เฝ้าระวัง หลังติดตั้ง*
	- WS : จนท. เข้าแก้ไขเรียบร้อยแล้ว
	- SRAD ค่า Reading ช่วงกลางคืน อยู่ที่ (-4) – (-1) watt/m2
	- Rain : ฝนตกช่วงเช้า 06/07/21
	- 08/07/21 (03.00น.) Auto-cal. ปกติทุกเครื่อง
Bus AQMs	ปิดระบบฯ / CSR
Micro1	- ปิดระบบฯ 29/06/21 เวลา 10.00น. จอดอยู่ที่ CSR
Micro 2	- <u>ปิดระบบฯ</u> อยู่ที่ CSR
Micro 3 (CSR)	- <u>เริ่มตรวจวัดฯ 29/06/21 เวลา 10.00น.</u>
	- PM10 ค่า Reading swing
	- WS/WD โฆว์ Flag <Samp ในบางชั่วโมง (2 ชม.)

Daily Check on 08/07/21 `Morning (08/07/21 00.00am. to 09/07/21 08.00am.)	
Station	Data & Calibration
Housing	<ul style="list-style-type: none"> - PM10 ค่า Reading Drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง (4 ชม.) - Off Auto-Cal.
Pluak Gate	<ul style="list-style-type: none"> - PM10 ค่า Reading swing. - Rain : ฝนตก 08/07/21 เวลา 20.00น. – 09/07/21 เวลา 05.00น. - 08/07/21 (17.00น.) Auto-cal. ปกติทุกเครื่องฯ
Techno	<ul style="list-style-type: none"> - ข้อมูลโดยรวมอยู่ในเกณฑ์ปกติ - VOC : ทำงานปกติ (เฉพาะพารามิเตอร์ที่เปิดใช้งาน) - 08/07/21 (12.00น.) Auto-cal. ปกติทุกเครื่องฯ
Ban Lang	<ul style="list-style-type: none"> - PM10 ค่า Reading swing - 87/07/21 (13.00น.) Auto-cal. ปกติทุกเครื่องฯ
Ban Konnong ติดตั้ง EDM (PM10) 24/03/21	<ul style="list-style-type: none"> - PM10 ค่า Reading swing. - PM2.5 ค่า Reading drop อยู่ที่ 0 ในบางชั่วโมง (2 ชม.) <div data-bbox="424 655 1469 1138"> <p>Station: KONNONG Periodically: 04/07/2021 00:00-09/07/2021 10:00 Type: AVG 1 Hr. [1 Hr.]</p> <p>Value</p> <p>50 40 30 20 10 0</p> <p>04/07/2021 05/07/2021 06/07/2021 07/07/2021 08/07/2021 09/07/2021</p> <p>Date & Time</p> <p>PM10 [ug/m3] PM2.5 [ug/m3]</p> </div> <ul style="list-style-type: none"> - SRAD ค่า Reading ช่วงกลางคืน อยู่ที่ (-3) – (-1) watt/m2 - Rain : ฝนตก 08/07/21 เวลา 22.00น. – 09/07/21 เวลา 03.00น. - 09/07/21 (04.00น.) Auto-cal. ปกติทุกเครื่อง
Bus AQMs	ปิดระบบฯ / CSR
Micro1	- ปิดระบบฯ 29/06/21 เวลา 10.00น. จอดอยู่ที่ CSR
Micro 2	- <u>ปิดระบบฯ</u> อยู่ที่ CSR
Micro 3 (CSR)	<ul style="list-style-type: none"> - เริ่มตรวจวัดฯ 29/06/21 เวลา 10.00น. - NO2 ค่า Reading ค้างอยู่ที่ 2 ppb ตลอด 24 ชม. - WS/WD โข้ว Flag <Samp 09/07/21 เวลา 02.00-05.00น.

Daily Check on 11/07/21 `Morning (11/07/21 00.00am. to 12/07/21 08.00am.)	
Station	Data & Calibration
Housing <i>*ตรวจเช็ค/แก้ไข*</i>	- เช็ค RH/Temp เนื่องจาก RH อยู่ที่ 0,1% ตั้งแต่ 10/07/21 ถึงปัจจุบัน
	- Off Auto-Cal.
Pluak Gate	- NO-NO2-NOx, SO2 ค่า Reading สูง 12/07/21 ช่วงเช้า
	- Rain : ฝนตก 11/07/21 ช่วงเช้า
Techno	- 11/07/21 (20.00น.) Auto-cal. ปกติทุกเครื่องฯ
	- ข้อมูลโดยรวมอยู่ในเกณฑ์ปกติ
Ban Lang	- VOC : ทำงานปกติ (เฉพาะพารามิเตอร์ที่เปิดใช้งาน)
	- 11/07/21 (16.00น.) Auto-cal. ปกติทุกเครื่องฯ
Ban Konnong ติดตั้ง EDM (PM10) 24/03/21	- ข้อมูลโดยรวมอยู่ในเกณฑ์ปกติ
	- 11/07/21 (16.00น.) Auto-cal. ปกติทุกเครื่องฯ
Ban Konnong	- WS โขว์ Flag <Samp ในบางชั่วโมง (8 ชม.)
	- SRAD ค่า Reading ช่วงกลางวัน อยู่ที่ (-4) – (-1) watt/m2
Ban Konnong	- Rain : ฝนตกไม่ตก
	- 11/07/21 (09.00น.) Auto-cal. ปกติทุกเครื่อง
Bus AQMs	ปิดระบบฯ / CSR
Micro1	- ปิดระบบฯ 29/06/21 เวลา 10.00น. จอดอยู่ที่ CSR
Micro 2	- ปิดระบบฯ อยู่ที่ CSR
Micro 3 (CSR)	- เริ่มตรวจวัดฯ 29/06/21 เวลา 10.00น.
	- SO2 ค่า Reading ค้างอยู่ที่ 5 ppb ตลอด 24 ชม.
	- PM10 ค่า Reading swing และ Drop อยู่ที่ 0 ug/m3 ในบางชั่วโมง



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	$\Delta H_{@}$ (mmH ₂ O)
B01	1563	01/09/2021	0.996	50.32
B02	8002514	03/09/2021	1.002	49.46
B03	1503016	03/09/2021	0.997	49.69
B04	2883	03/09/2021	1.003	50.73
B05	1609067	01/09/2021	1.004	48.96
R01	1561	02/09/2021	0.998	49.33
R02	8002513	02/09/2021	1.003	49.80
R03	1570	01/09/2021	0.995	50.28
R04	8002519	01/09/2021	0.997	50.11
R05	1503015	13/09/2021	1.005	49.57

Remark : Accept Value of y (test) is $0.97 < y < 1.03$

Accept Value of $\Delta H_{@}$ (test) is 46.7 ± 6.4 (mmH₂O)

Calibrated by :

Phakhinai Khongkomnerd
(Mr. Phakhinai Khongkomnerd)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B03	S	0.99	02/08/2021	0.84	0.84
B04	S	0.99	02/08/2021	0.84	0.84
B05	S	0.99	02/08/2021	0.83	0.84
B07	S	0.99	02/08/2021	0.84	0.84
B08	S	0.99	02/08/2021	0.83	0.84
B09	S	0.99	02/08/2021	0.84	0.84
B11	S	0.99	02/08/2021	0.84	0.85
B16	S	0.99	02/08/2021	0.83	0.84
B18	S	0.99	03/08/2021	0.84	0.84
B19	S	0.99	03/08/2021	0.85	0.84
B21	S	0.99	03/08/2021	0.84	0.84
B24	S	0.99	02/08/2021	0.84	0.85
B27	S	0.99	03/08/2021	0.84	0.83
B30	S	0.99	03/08/2021	0.84	0.84
B31	S	0.99	03/08/2021	0.84	0.85
B33	S	0.99	03/08/2021	0.83	0.84
B35	S	0.99	03/08/2021	0.85	0.84

Remark : Accept value of Cp (test) is 0.84 ± 0.01

Calibrated by :

Phakhinai Khongkomnerd
(Mr. Phakhinai Khongkomnerd)

Approved by :

Peerat Detudom
(Mr. Peera Detudom)

Certificate of Calibration

Certificate No. : 64-220066-1

Page : 1 of 2

Submitted by : S. P. S Consulting Service Co.,Ltd.

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Equipment : Vacuum Gauge

Manufacturer : HI-LIGHT **Model :** N/A

ID No. : 1/60

Range : 0 in Hg to -30 in Hg **Resolution :** 1 in Hg

Environment : Ambient Temperature : $(20 \pm 2) ^\circ \text{C}$

Relative Humidity : $(50 \pm 10) \%$

Date of Received : 02 July 2021

Date of Calibration : 05 July 2021

Date of Issue : 05 July 2021

Calibrated by : Satja Sangkhum

Calibration Method : In-house method CAL-M2201 based on BS EN 837-1:2016 with Pressure Calibrator

Reference Standard Instruments : This certification is traceable to the International System of Units

Pressure Calibrator & Pressure Sensors Modules

ID No.	Cert. No.	Due Date	Traceability
220007	MP-0036-20	11 Mar 2022	National Institute of Metrology (Thailand), (NIMT)
220001	MP-0036-20	11 Mar 2022	National Institute of Metrology (Thailand), (NIMT)

Approved by :



(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 64-220066-1

Page : 2 of 2

Result of Calibration : Without Adjustment

Function : Vacuum measurement

Condition of calibration :

- 1 Scale and conversion factor is 1 kPa = 0.295 in Hg
- 2 Angle of mounting from horizontal at 90 °
- 3 UUC reading after lightly tapped
- 4 Reference plane of UUC at center of Gauge
- 5 UUC calibrated by using clean air as pressure media
6. UUC Condition As-Received : Good

Standard Reading (in Hg)	UUC Reading (in Hg)	Correction (in Hg)
0.00	0	0.0
-4.69	-5	0.3
-9.57	-10	0.4
-14.67	-15	0.3
-19.71	-20	0.3
-29.93	-30	0.1
-29.92	-30	0.1
-19.69	-20	0.3
-14.69	-15	0.3
-9.58	-10	0.4
-4.69	-5	0.3
0.00	0	0.0

Remark

UUC : Unit Under Calibration

The uncertainty is combined hysteresis

The uncertainty of measurement was with in ± 0.39 in Hg

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

[Signature]





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R²
R01	SKC	224-PCXR4	602467	04/10/2021	1,000	1,500	2,000	993	1,495	1,991	0.996x + 1.128	1.000
R02	SKC	224-PCXR4	626450	01/10/2021	1,000	2,000	3,000	1,002	1,500	2,002	1.012x – 22.958	0.999
R03	SKC	224-PCXR4	691592	01/10/2021	1,000	1,500	2,000	994	1,503	2,000	1.014x – 31.464	0.999
R04	SKC	224-PCXR4	691672	01/10/2021	1,000	1,500	2,000	1,002	1,499	2,002	1.011x – 21.643	0.999
R05	SKC	224-PCXR4	798470	01/10/2021	1,000	1,500	2,000	993	1,494	1,995	1.001x – 7.868	1.000
R06	SKC	224-PCXR4	798456	04/10/2021	1,000	1,500	2,000	995	1,505	2,001	1.013x – 28.068	0.999
R07	SKC	224-PCXR4	798480	04/10/2021	1,000	1,500	2,000	991	1,494	1,991	0.998x – 3.810	1.000
R08	SKC	224-PCXR4	883215	04/10/2021	1,000	1,500	2,000	993	1,502	1,999	1.014x – 30.678	0.999
R09	SKC	224-PCXR4	034650	04/10/2021	1,000	1,500	2,000	1,000	1,501	2,001	1.013x – 24.580	0.999
R10	SKC	224-PCXR4	091765	04/10/2021	1,000	1,500	2,000	994	1,497	1,990	0.996x + 1.379	1.000
R11	SKC	224-PCXR4	091763	04/10/2021	1,000	1,500	2,000	997	1,494	1,986	0.990x + 7.306	1.000
R12	SKC	224-PCXR4	091568	01/10/2021	1,000	1,500	2,000	1,002	1,502	2,003	1.012x – 22.870	0.999
R13	SKC	224-PCXR4	091638	01/10/2021	1,000	1,500	2,000	997	1,492	1,995	0.998x – 2.097	1.000
R14	SKC	224-PCXR4	091764	01/10/2021	1,000	1,500	2,000	994	1,503	2,000	1.013x – 28.725	0.999
R15	SKC	224-PCXR8	529457	04/10/2021	1,000	1,500	2,000	997	1,504	1,999	1.012x – 26.422	0.999
R16	SKC	224-PCXR8	529643	04/10/2021	1,000	1,500	2,000	1,000	1,500	2,004	1.013x – 25.485	0.999
R17	SKC	224-PCXR8	529645	05/10/2021	1,000	1,500	2,000	994	1,495	1,991	0.997x – 2.467	1.000
R18	SKC	224-PCXR8	566756	05/10/2021	1,000	1,500	2,000	993	1,492	1,990	0.995x + 0.929	1.000
R19	SKC	224-PCXR8	566802	05/10/2021	1,000	1,500	2,000	1,001	1,500	2,002	1.013x – 25.601	0.999
R20	SKC	224-PCXR8	529089	05/10/2021	1,000	1,500	2,000	995	1,490	1,992	1.000x – 7.370	1.000
R21	SKC	224-PCXR8	665728	05/10/2021	1,000	1,500	2,000	1,003	1,500	2,001	1.010x – 20.957	0.999
R22	SKC	224-PCXR8	707444	05/10/2021	1,000	1,500	2,000	1,000	1,499	2,002	1.014x – 27.526	0.999
R23	SKC	224-PCXR8	761067	05/10/2021	1,000	1,500	2,000	994	1,496	1,992	0.999x – 4.926	1.000
R24	SKC	224-PCXR8	707893	01/10/2021	1,000	1,500	2,000	1,002	1,500	2,000	1.010x – 21.798	0.999
R25	SKC	224-PCXR8	761052	01/10/2021	1,000	1,500	2,000	1,001	1,501	2,002	1.013x – 24.198	0.999
R26	SKC	224-PCXR8	707956	01/10/2021	1,000	1,500	2,000	996	1,494	1,992	0.999x – 3.715	1.000
R27	SKC	224-PCXR8	707398	01/10/2021	1,000	1,500	2,000	999	1,500	1,992	0.994x + 4.612	1.000
R28	SKC	224-PCXR8	707481	04/10/2021	1,000	1,500	2,000	1,001	1,501	2,003	1.012x – 23.843	0.999
R29	SKC	224-PCXR8	707402	04/10/2021	1,000	1,500	2,000	995	1,493	1,992	0.996x + 2.559	1.000
R30	SKC	224-PCXR8	093811	04/10/2021	1,000	1,500	2,000	1,004	1,498	2,003	1.010x – 19.989	0.999
R31	SKC	224-PCXR8	093183	07/10/2021	1,000	1,500	2,000	1,001	1,499	2,003	1.013x – 24.122	0.999
R32	SKC	224-PCXR8	671950	07/10/2021	1,000	1,500	2,000	992	1,504	1,999	1.017x – 34.672	0.999
R33	SKC	224-PCXR4	626254	04/10/2021	1,000	1,500	2,000	996	1,494	1,994	0.996x + 0.012	1.000
R34	SKC	224-PCXR4	626131	04/10/2021	1,000	1,500	2,000	1,001	1,502	2,002	1.013x – 24.616	0.999
R35	SKC	224-PCXR8	707460	07/10/2021	1,000	1,500	2,000	995	1,500	2,001	1.012x – 27.621	0.999
R36	SKC	224-PCXR8	707446	06/10/2021	1,000	1,500	2,000	997	1,490	1,990	0.992x + 6.230	1.000
R37	SKC	224-PCXR8	707432	06/10/2021	1,000	1,500	2,000	995	1,494	1,996	1.002x – 8.928	1.000
R38	SKC	224-PCXR8	707349	06/10/2021	1,000	1,500	2,000	996	1,491	1,993	0.999x – 5.484	1.000
R39	SKC	224-PCXR8	761095	01/10/2021	1,000	1,500	2,000	989	1,504	1,999	1.017x – 35.278	0.999

Calibrated by :

Phakhinai Khongkomerd
(Mr. Phakhinai Khongkomerd)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
 Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
 Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R²
R40	SKC	224-PCXR4	612753	01/10/2021	1,000	1,500	2,000	1,000	1,488	1,995	0.994x + 2.710	1.000
R41	SKC	224-PCXR4	626140	01/10/2021	1,000	1,500	2,000	1,002	1,500	2,002	1.012x - 24.473	0.999
R42	SKC	224-PCXR4	626463	01/10/2021	1,000	1,500	2,000	1,001	1,494	2,000	0.999x - 2.575	1.000
R43	SKC	224-PCXR4	626129	04/10/2021	1,000	1,500	2,000	992	1,504	1,999	1.013x - 30.639	0.999
R44	SKC	224-PCXR4	602753	04/10/2021	1,000	1,500	2,000	998	1,497	1,993	0.996x + 1.291	1.000
R45	SKC	224-PCXR4	626137	07/10/2021	1,000	1,500	2,000	1,002	1,500	2,001	1.012x - 23.229	0.999

Calibrated by :

Phakhinai Khongkomnerd
 (Mr.Phakhinai Khongkomnerd)

Approved by :

Peera Detudom
 (Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-R01	Dwyer	VFB-65	02/07/2021	500	1,000	2,000	498.4	987.7	1990.8	1.002x – 5.855	1.000
H-R02	Dwyer	VFB-65	01/07/2021	500	1,000	2,000	499.0	996.4	1991.8	0.991x + 4.947	1.000
H-R03	Dwyer	VFB-65	01/07/2021	500	1,000	2,000	501.0	995.0	2005.4	0.996x + 3.848	1.000
H-R04	Dwyer	VFB-65	02/07/2021	500	1,000	2,000	494.6	997.2	2007.9	1.004x – 8.811	1.000
H-R05	Dwyer	VFB-65	02/07/2021	500	1,000	2,000	498.2	1000.6	1984.9	0.997x + 1.804	1.000
H-R06	Dwyer	VFB-65	01/07/2021	500	1,000	2,000	497.4	998.3	2001.5	0.999x – 1.055	1.000

Calibrated by :

Phakhinai Khongkomnerd
(Mr. Phakhinai Khongkomnerd)

Approved by :

Peera Detudom
(Mr. Peera Detudom)

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.comNSC-TISI-TISI7025
CALIBRATION 0049

CERTIFICATE No : 21M3169

REFERENCE No : 60627-5

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 19-Mar-21

APPROVED BY :  PONGSAK J.

ISSUED DATE : 20-Mar-21

RECEIVED DATE : 19-Mar-21

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 21M3169

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 19-Mar-21
AIR PRESSURE : 1009mbar \pm 1mbar CALIBRATION DATE : 19-Mar-21
AMBIENT TEMPERATURE : 24°C \pm 1°C RELATIVE HUMIDITY : 52 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING WEIGHT OF QUALITY CALIBRATION TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23
2) STANDARD WEIGHT	E2	15843	C02210419	10-Feb-23
3) STANDARD WEIGHT	E2	QK-I-349	M2103235S	26-Mar-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT


1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 100 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000066
0.02	0.01998	0.00002	0.000066
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000067
0.50	0.49996	0.00004	0.000065
1.00	0.99997	0.00003	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00003	-0.00003	0.000070
20.00	20.00000	0.00000	0.000075
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0001	-0.0001	0.00022

5. OFF CENTER LOADING ERROR

POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000


NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

Lambda UV Preventive Maintenance (PM)

Company Name:	S.P.S. CONSULTING SERVICE CO., LTD.		
Address:	7, Soi Phaholyothin24, Ladyao, Jatujak, Bangkok		
User Name:	K. Benjawan	WO Number:	WO-01338285
Telephone Number:	086-141-2523	PM Number:	6 of 6 P
Customer Support Engineer:	K. Anon	Certificate Number:	UV2043-2021
Date PM Performed: (DD-MMM-YYYY)	27-Jul-2021	Next PM Due Date: (DD-MMM-YYYY)	27-Jan-2022

Part Number	Release	Publication Date	
09370504	B	March 2013	

Scope

The purpose of this PM is to ensure the continued functionality of the PerkinElmer Lambda UV/Vis Spectrophotometer by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. Copyright © 2009 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose. PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component Specific Model	Serial #	Software Version		Configuration Notes
Lambda 25	501S14123010	6.2.0.0741	STD	1.27
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

Parts Lists

Parts Included with the PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot/SN #	Expiration Date (MM/YY)
B250 0999	Stray Light standard			
	Nal cell	1	11200	Oct-21
	NaNO2 cell	1	21175	
	KCl cell	1	31873	
	H2O	1	72075	
B050 7805	Secondary Standards for calibration of wavelength and photometric accuracy or use NBS/NIST 390 standards			
	Gray Glass G1	1	4660	Oct-21
	Gray Glass G2	1	4575	
	Gray Glass G3	1	4525	
	Holmium Glass	1	5499	

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Perform general inspection of system for cleanliness.

2. Optical checks:

- ☒ Lamp Alignment/Energy
- ☒ Sample Compartment Windows/Monochromator
- ☒ Mirror and Grating Alignment
- ☒ Cell Holder Alignment

3. Mechanical:

- ☒ Physical inspection – Please write any comments in the additional comments section.
- ☒ Grating Drive Mechanism.
- ☒ Lamp Change Mechanism.
- ☐ Slit Drive Manual Servo.

4. Test:

Refer to Appendix A for the specifications of the instrument being tested.

- ☒ D2 Wavelength accuracy

	Actual Value	Specification
Accuracy at 656.1 nm	656.09	± 0.1

☒ Holmium Oxide wavelength accuracy

Filter ID #		5499		
Test	Calibration Value	Actual Value	Deviation	Specification
279.3 nm	279.3	279.37	-0.07	± 0.5
360.8 nm	360.9	360.92	-0.02	± 0.5
459.9 nm	459.9	460.00	-0.10	± 0.5
536.4 nm	536.2	536.33	-0.13	± 0.5

☒ Scattered Light.

Test	Filter ID #	Result	Specification
NaI @ 220 nm	11200	-0.1294	< 0.02 %T
NaNO ₂ @ 340 nm	21175	0.0034	< 0.02 %T
NaNO ₂ @ 370 nm	21175	0.0027	< 0.02 %T
KCl @ 200 nm	31873	2.2355	≥ 2 A

☒ Baseline Flatness.

Corrected Baseline	Specification
0.000316	± 0.001 A

☒ Noise Test @ 500 nm.

Actual Value	Specification
0.0000250	± 0.00008 A

☒ Photometric Accuracy.

Filter 1 ID #		4660		
Test	Calibrated Value	Actual Value	Deviation	Specification
440 nm	0.3208	0.3240	-0.0032	± 0.006 A
546 nm	0.3029	0.3049	-0.0020	± 0.006 A
635 nm	0.3572	0.3584	-0.0012	± 0.006 A
Filter 2 ID #		4575		
Test	Calibrated Value	Actual Value	Deviation	Specification
440 nm	1.06	1.0627	-0.0027	± 0.006 A
546 nm	0.9835	0.9851	-0.0016	± 0.006 A
635 nm	1.007	1.0087	-0.0017	± 0.006 A
Filter 3 ID #		4525		
Test	Calibrated Value	Actual Value	Deviation	Specification
440 nm	0.4981	0.4998	-0.0017	± 0.006 A
546 nm	0.4739	0.4751	-0.0012	± 0.006 A
635 nm	0.5274	0.5286	-0.0012	± 0.006 A

5. Accessory (where applicable):

- ☐ Integrating Sphere
- ☐ Reflecting Attachment
- ☐ Cell Changer
- ☐ Sipper
- ☐ Auto Sampler


6. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☒ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<i>The preventive maintenance checks and if applicable performance tests for Lambda UV have been completed.</i>	
<i>This Lambda UV Passes <input checked="" type="checkbox"/> Fails <input type="checkbox"/> the preventive maintenance.</i>	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: 	Date: 9-Aug-21 (DD-MM-YYYY)
Authorized Customer Representative:	Date: 9-Aug-21 (DD-MM-YYYY)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	04 October 2021	Brand :	API	Model :	300E
No.	CO-B01			Serial No.	782
Calibrator (Dilution System)					
Brand : API			Model : 700		
Last Cal. Date : 05 August 2021			Serial No. : 911		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D824478		
Certified Date : 15 April 2020		Expired Date : 14 April 2022		Cylinder Conc. : 4,740 ppm	
Calibrating Condition					
Pressure : 1011 mmbar		Temp. : 24.6 °C		% RH : 49	
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response		%Dif	
Zero	0	0.11		-	
CO Span	40.00	40.06		0.150	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4015.2	mV	2500-4800 mV		
CO Reference	3947.8	mV	2500-4800 mV		
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.4	In-Hg-A	~2" < Ambient Absolute Pressure		
Sample Flow	808	CC/Min	800 ± 10%		
Sample Temperature	48.3	°C	48 ± 4		
Bench Temperature	48.1	°C	48 ± 2		
Wheel Temperature	68.4	°C	68 ± 2		
Box Temperature	30.7	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3021.9	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		

Calibrated by :

Phakhinai Khongkomnerd

(Mr.Phakhinai Khongkomnerd)

Approved by :

Peera Detudom

(Mr. Peera Detudom)

Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID: GC/MS
Organization Name: S.P.S. Consulting service
Organization Location: 7 Soi Phaholyothin Road, Ladyao, Khet Jatujak, Bangkok, 10900
Date: March 22, 2021 10:41:18 AM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.51, GCMS.02.51
Overall Qualification Status: Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Setpoint Status: Pass

	Setpoint		Actual
Inlet Pressure:	25.0	psi	24.9

Accuracy: 0.1 psi

Agilent Recommended: <= 1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Inlet Pressure Decay

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Name: 7890
Back SSL

Setpoint Status:

Pass

Pressure:

25.0 psi

Pressure Change:

-0.1 psi /5 minutes

Agilent Recommended:

>= -2.0 and <= 0.5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 7890
Back SSL

Setpoint Status:

Pass

Setpoint

Actual

Inlet Pressure: 25.0 psi

24.9 psi

Accuracy:

0.1 psi

Agilent Recommended:

<= 1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Detector Flow Accuracy

Name: 7890
Front FID

Setpoint Status:

Pass

Flow Type:

Fuel

Setpoint:

30.0 mL/min

Measured Flow:

29.9 mL/min

Accuracy:

0.1 mL/min

Agilent Recommended:

<= 10.0 % setpoint

(3.0 mL/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Setpoint Status:

Pass

Flow Type:

Oxidizer

Setpoint:

400.0

mL/min

Measured Flow:

399.8

mL/min

Accuracy:

0.2

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

40.0

ml/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status:

Pass

Flow Type:

Makeup

Setpoint:

25.0

mL/min

Measured Flow:

24.9

mL/min

Accuracy:

0.1

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

2.5

ml/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name:

7890

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

230.0

230.0

°C

Accuracy:

0.0

°C

Agilent Recommended:

>=

-1.0

% setpoint in K

(

-5.0

°C

)

<=

1.0

% setpoint in K

(

5.0

°C

)

Date:

March 22, 2021 10:41:18 AM

System ID:

GC/MS

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

100.0

100.0

°C

Accuracy:

0.0

°C

Agilent Recommended:

>=

-1.0

% setpoint in K

(

-3.7

°C

)

<=

1.0

% setpoint in K

(

3.7

°C

)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:

7890

Setpoint Status:

Pass

Setpoint/Average

Temperature:

100.0

100.05

°C

Stability:

0.1

°C

Agilent Recommended:

<=

0.5

Overall GC Oven Temperature Stability Test Status

Pass

Scouting Run

Tested Combination2

Back

SSL

/ Front

FID

Manual Injection

Name:

Not applicable

Setpoint Status:

Completed

Injection Volume on Column:

1.0

uL

Overall Scouting Run Status

Completed

Signal to Noise

Tested Combination2

Back

SSL

/ Front

FID

Date:

March 22, 2021 10:41:18 AM

System ID:

GC/MS

Manual Injection

Name: 7890

Setpoint Status:

Pass

Signal to Noise:

1711991

Agilent Recommended:

>=

300000

Overall Signal to Noise Test Status

Pass

Noise and Drift

Tested Combination2

Back

SSL

/ Front

FID

Name: 7890

Setpoint Status:

Pass

Base Signal:

14.0

pA

ASTM Noise

counts

384.56

Agilent Recommended:

<=

768.00

Drift

counts/Hr

178.79

Status:

Pass

<=

19200.00

Pass

Overall Noise and Drift Test Status

Pass

Log Amp

Tested Combination1

Front

SSL

/ External

SQ

Name: 5975C inert XL with TAD

Setpoint Status:

Pass

Overall Log Amp Test Status

Pass

RFPA

Date:

March 22, 2021 10:41:18 AM

System ID:

GC/MS

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			
Setpoint Status:	Pass			
Amu:	1050	m/z	Drift After Five Minutes:	RFPA Voltage:
			4	485
			mV	mV
Agilent Recommended:	>=	-100	and	<= 100
				<= 1100

Overall RFPA Test Status

Pass

Tune EI

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			
Setpoint Status:	Pass			
Filament:	1			
Setpoint Status:	Pass			
Filament:	2			

Overall Tune EI Test Status

Pass

Signal to Noise EI

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			
Source:	EI - Standard (Stainless Steel)		Filament:	1
Setpoint Status:	Pass			
Signal to Noise:	925			
Agilent Recommended:	>= 320			

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Source: EI - Standard (Stainless Steel) Filament: 2

Setpoint Status: Pass

Signal to Noise: 672

Agilent Recommended: \geq 320

Overall Signal to Noise EI Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GC/MS
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Manual Injection
Sampler Identifier	Sampler 1
Inlet	Front
Detector	External
LTM Included?	No

Tested Combination2

Injection Technique	Manual Injection
Sampler Identifier	Sampler 2
Inlet	Back
Detector	Front
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN10925120
Firmware Revision	A.01.10.3
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Detector 2

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5975C inert XL with TAD
Serial Number	US91732743
Firmware Revision	Not applicable
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Standard (Stainless Steel)
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Nattapat Hengcharoen
Logged On User Name:	nattapat.hengcharoen@agilent.com
Signature Creation Date:	March 22, 2021
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Date:	March 22, 2021 10:41:18 AM
System ID:	GC/MS

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 12:15:46 PM	Audit	SessionCreated	Session	None
March 19, 2021 12:15:46 PM	Start	Configuration	Session	None
March 19, 2021 12:15:46 PM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
March 19, 2021 12:21:07 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.51/Gc.02.51.eqp], EQP File Name: [Gc.02.51.eqp], EQP Name: [AgilentRecommended] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.51/GcMs.02.51.eqp], EQP File Name: [GcMs.02.51.eqp], EQP Name: [AgilentRecommended]
March 19, 2021 12:21:16 PM	End	Configuration	Session	None
March 19, 2021 12:21:22 PM	Start	Qualification	Session	OQ
March 19, 2021 12:21:22 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890; - Qualitative Test - No setpoints associated	None

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 1:38:58 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
March 19, 2021 1:39:56 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
March 19, 2021 1:40:12 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
March 19, 2021 1:40:14 PM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
March 19, 2021 1:40:21 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
March 19, 2021 1:40:24 PM	Start	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
March 19, 2021 1:40:34 PM	End	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
March 19, 2021 1:40:36 PM	Start	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
March 19, 2021 1:40:41 PM	End	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1

Page 2 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 1:40:42 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
March 19, 2021 1:41:20 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
March 19, 2021 1:41:22 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
March 19, 2021 1:41:24 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
March 19, 2021 1:41:37 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
March 19, 2021 1:41:40 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
March 19, 2021 1:41:42 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
March 19, 2021 1:41:55 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
March 19, 2021 1:41:56 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
March 19, 2021 1:41:59 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None

Page 3 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

Page 14 / 20

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 1:42:27 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
March 19, 2021 1:43:21 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over.
March 19, 2021 1:43:55 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
March 19, 2021 1:43:57 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
March 19, 2021 1:43:59 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
March 19, 2021 1:44:12 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
March 19, 2021 1:44:14 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
March 19, 2021 1:44:17 PM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
March 19, 2021 1:45:12 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry

Page 4 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 1:45:19 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
March 19, 2021 1:54:29 PM	Start	Execution	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	None
March 19, 2021 2:33:24 PM	Start	Execution	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	None
March 19, 2021 2:35:01 PM	Audit	AceClosed	Session	None
March 19, 2021 2:35:37 PM	Audit	AceRestarted	Session	None
March 19, 2021 2:35:38 PM	Audit	SessionReloaded	Session	None
March 19, 2021 2:35:41 PM	Start	Qualification	Session	OQ
March 19, 2021 2:35:41 PM	Start	Execution	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	None
March 19, 2021 2:36:12 PM	Audit	Data	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	Data files Path : E:\SPS\SCOUNT_FID.D\FID 1A.ch
March 19, 2021 2:36:32 PM	End	Execution	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	Run Count : 1
March 19, 2021 2:36:36 PM	Start	Execution	Signal to Noise - Manual Injection, Back SSL, Front FID: - Detector FID - L: >= 300000	None

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 2:36:46 PM	Audit	Data	Signal to Noise - Manual Injection, Back SSL, Front FID: - Detector FID - L: >= 300000	Data files Path : E:\SPS\SN_FID.D\FID1A.ch
March 19, 2021 2:37:00 PM	End	Execution	Signal to Noise - Manual Injection, Back SSL, Front FID: - Detector FID - L: >= 300000	Run Count : 1
March 19, 2021 2:37:06 PM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
March 19, 2021 3:46:48 PM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
March 19, 2021 3:47:08 PM	Audit	Data	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : E:\SPS\ND_FID.D\FID1A.ch
March 19, 2021 3:47:30 PM	End	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
March 19, 2021 3:47:32 PM	Start	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	None
March 19, 2021 3:49:54 PM	Start	Execution	RFP A - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	None
March 19, 2021 3:52:45 PM	Start	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	None

Page 6 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 3:53:16 PM	End	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	Run Count : 1
March 19, 2021 3:53:19 PM	Start	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	None
March 19, 2021 3:58:14 PM	End	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	Run Count : 1
March 19, 2021 3:59:01 PM	Start	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Standard (Stainless Steel) Filament 1 (Qualitative - No setpoints associated)	None
March 19, 2021 3:59:37 PM	End	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Standard (Stainless Steel) Filament 1 (Qualitative - No setpoints associated)	Run Count : 1
March 19, 2021 3:59:39 PM	Start	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Standard (Stainless Steel) Filament 2 (Qualitative - No setpoints associated)	None
March 19, 2021 4:00:01 PM	End	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Standard (Stainless Steel) Filament 2 (Qualitative - No setpoints associated)	Run Count : 1
March 19, 2021 4:00:05 PM	Audit	AcceClosed	Session	None
March 22, 2021 9:39:45 AM	Audit	AcceRestarted	Session	None
March 22, 2021 9:39:49 AM	Audit	SessionReloaded	Session	None
March 22, 2021 9:40:02 AM	Start	Qualification	Session	OQ

Page 7 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: naitapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 22, 2021 9:40:26 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 1 - L: >= 320	None
March 22, 2021 9:41:14 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 1 - L: >= 320	None
March 22, 2021 9:41:58 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 1 - L: >= 320	Data files Path : E:\SPS\SN_F1.D\DATA.MS
March 22, 2021 9:43:36 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 1 - L: >= 320	Run Count : 1
March 22, 2021 9:43:44 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 2 - L: >= 320	None
March 22, 2021 9:44:03 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 2 - L: >= 320	Data files Path : E:\SPS\SN_F2.D\DATA.MS
March 22, 2021 9:44:34 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 2 - L: >= 320	Run Count : 1

Page 8 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: nattapat.hengcharoen
Hostname: 5GG70212Y1

System Id: GC/MS
Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 22, 2021 9:44:37 AM	End	Qualification	Session	OQ
March 22, 2021 9:44:37 AM	Start	Reporting	Session	None
March 22, 2021 10:40:26 AM	Audit	Reporting	Session	Report Generated : Certificate

Certificate No.: CP20210011EA

Operation No.: CP2021090015

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: RION

Model/Type: NL-52 (Meter), UC-59 (Microphone), NH-25 (Preamplifier)

Serial No.: 00632063 (Meter), 05230 (Microphone), 32091 (Preamplifier)

ID No.: -

Customer: IRPC Public Company Limited.

Address: 299 Moo 5, Sukhumvit Rd., Tumbon Chungnern,
Amphor Muang, Rayong 21000

Received Date: 23 September 2021

Calibrated Date: 29 September 2021 - 5 October 2021

Issued Date: 6 October 2021

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: 

(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20210011EA

Calibration Report

Equipment: Sound Level Meter
Manufacturer: RION
Model/Type: NL-52 (Meter), UC-59 (Microphone), NH-25 (Preamplifier)
Serial No.: 00632063 (Meter), 05230 (Microphone), 32091 (Preamplifier)
ID No.: -
Ambient Temperature: $(23 \pm 2) ^\circ\text{C}$
Relative Humidity: $(50 \pm 15) \%$
Pressure: $(101.3 \pm 1.5) \text{ kPa}$

Method of Calibration :-

IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1001-21	12 January 2022
2) Arbitrary Function Generator	AFG2021	C010063	0145RF21	17 June 2022
3) Programmable Attenuator	PA5	2913	EF-0017-21	1 April 2022
4) 6.5 Digit precision multimeter	8846A	9609027	0478EL21	16 August 2022
5) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P210047 0255TE21	16 June 2022 7 July 2022
6) Pressure humidity and Temperature Transmitter	PTU301	F0640003	CL1-P210048 0256TE21	17 June 2022 7 July 2022
7) Performance Audio Analyzer	U8903B	MY56510003	0145EL21 0172RF21	11 February 2022 9 September 2022

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; ONSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
94.1	94.1	0.0	± 0.7

Note : Absolute sensitivity was established by the use of the Sound Calibrator RION Type NC-74 S/N : 34536115.

Certificate No.: CP20210011EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
14.2

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	9.9
C-weighting	14.9
Z-weighting	20.5

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.3	0.2	0.3	±1.0
1000	0.0	0.0	0.0	±0.7
8000	-0.7	-0.7	-0.8	+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.1	-0.1	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.1	0.0	±1.0
1000	0.0	0.0	0.0	±0.7
2000	0.0	0.2	0.0	±1.0
4000	0.0	0.1	0.0	±1.0
8000	0.2	0.2	0.0	+1.5; -2.5
16000	-1.2	-1.1	0.2	+2.5; -16.0

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

Certificate No.: CP20210011EA

Calibration Report

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
130.0	130.0	0.0	±0.8
131.0	131.0	0.0	±0.8
132.0	132.0	0.0	±0.8
133.0	133.0	0.0	±0.8
134.0	134.0	0.0	±0.8
135.0	135.0	0.0	±0.8
136.0	136.0	0.0	±0.8
137.0	137.0	0.0	±0.8

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8

Certificate No.: CP20210011EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower (Cont.)

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	33.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	126.0	0.0	±0.5
	2	108.9	-0.1	+1.0 ; -1.5
	0.25	99.9	-0.1	+1.0 ; -3.0
Slow	200	119.6	0.0	±0.5
	2	100.0	0.0	+1.0 ; -3.0
LAE	200	120.0	0.0	±0.5
	2	100.0	0.0	+1.0 ; -1.5
	0.25	90.8	-0.2	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	125.4	125.3	-0.1	±2.0
Positive half cycle	124.4	124.1	-0.3	±1.0
Negative half cycle	124.4	124.1	-0.3	±1.0

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
139.4	139.4	0.0	±1.5

Certificate No.: CP20210011EA

Calibration Report

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	129.0	129.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks: 1. The acceptance limit is for the deviated value.
2. Acceptance limits was IEC61672-3:2013 Class 1.

- - End of Report - -



บริษัท เพทโร-อินสตรูเมนต์ จำกัด
PETRO-INSTRUMENTS CORP., LTD.

7/409 ซ.วิภาวดีรังสิต 36 ถ.วิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak, Bangkok 10900, Thailand.

TEL : (662) 9395711 (12 Lines), 5132333 (12 Lines), 5139575-9 FAX : (662) 9394207, 9394208

http://www.pico.co.th E-mail-address : pico@pico.co.th

TEST REPORT OF CALIBRATION

We hereby certify that the equipment mentioned below have been maintained and have duly performed in accordance with HORIBA specifications.

Equipment	:	Multi Water Quality Checker
Model	:	U-5000G
Manufacture	:	HORIBA
Serial No.	:	RAAGSEN3
Job No.	:	JID2100311-001
Customer	:	IRPC Public Company Limited
Calibration date	:	April 27, 2021
Calibration due	:	April 27, 2022

Petro-Instruments Corp., Ltd.

Calibrated by 

(Ms.Chamaiporn Vongchalee)

Chemist

Approved by 

(Mr. Athitphong Kanchanasathian)

Assistant Section Manager

Scientific Product Business Unit



บริษัท เพทโร-อินสตรูเมนต์ จำกัด
PETRO-INSTRUMENTS CORP., LTD.

7/409 ซ.วิภาวดีรังสิต 36 ถ.วิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak, Bangkok 10900, Thailand.

TEL : (662) 9395711 (12 Lines), 5132333 (12 Lines), 5139575-9 FAX : (662) 9394207, 9394208

<http://www.pico.co.th> E-mail-address : pico@pico.co.th

CALIBRATION REPORT

Equipment : Multi Water Quality Checker
Manufacturer : HORIBA
Model : U-53
Serial No. : V39CGM6U
Date of Calibration : April 27, 2021
Customer Name : IRPC Public Company Limited

HORIBA, Multi Water Quality Checker model U-53 was tested according to service manual.

Auto Calibration (1- point)

Check function	Calibration	Before Calibrate	After Calibrate
pH	1- point auto (Zero) (4.01 pH)	4.02 pH	4.01 pH
TURBIDITY	1- point auto (Zero) (0.0 NTU)	0.0 NTU	0.0 NTU
CONDUCTIVITY	1- point auto (Span) (4.49 mS/cm)	4.48 mS/cm	4.49 mS/cm
DO	1- point auto (Span) (8.92 mg/L)	8.77 mg/L	8.92 mg/L
Depth	(0 m)	0 m	0 m

Reference Standard

- Standard Solution of HORIBA, pH 4 Lot No. S3316/03



บริษัท เพทโร-อินสตรูเมนต์ จำกัด
PETRO-INSTRUMENTS CORP., LTD.

7/409 ซ.วิภาวดีรังสิต 36 ถ.วิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak, Bangkok 10900, Thailand.

TEL : (662) 9395711 (12 Lines), 5132333 (12 Lines), 5139575-9 FAX : (662) 9394207, 9394208

http://www.pico.co.th E-mail-address : pico@pico.co.th

Manual Calibration (2- point)

A. pH Measurement.

Check item	pH Standard Solution	Before Calibrate	After Calibrate	Error	Judgment
Zero Calibration	6.86	6.86	6.86	0.00	PASS
Span Calibration	4.01	4.02	4.01	0.01	PASS

Measure at temperature 25 °C Within ± 0.1 pH

B. Conductivity Measurement.

Check item	Conductivity Standard Solution	Before Calibrate	After Calibrate	Error	Judgment
Zero Calibration	0.00 mS/cm	0.000 mS/cm	0.00 mS/cm	0.000 mS/cm	PASS
Span Calibration	Range 1 (0.100-0.999 S/m) 0.718 mS/cm	0.728 mS/cm	0.718 mS/cm	0.01 mS/cm	PASS
	Range 2 (1.00-10.00 S/m) 6.67 mS/cm	6.67 mS/cm	6.67 mS/cm	0.000 mS/cm	PASS
	Range 3 (0.0-99.9 mS/m) 58.7 mS/cm	58.1 mS/cm	58.7 mS/cm	0.6 mS/cm	PASS

Measure at temperature 25 °C Within $\pm 1\%$ /F.S.



บริษัท เพทโร-อินสตรูเมนต์ จำกัด
PETRO-INSTRUMENTS CORP., LTD.

7/409 ซ.วิภาวดีรังสิต 36 ถ.วิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak, Bangkok 10900, Thailand.

TEL : (662) 9395711 (12 Lines), 5132333 (12 Lines), 5139575-9 FAX : (662) 9394207, 9394208

http://www.pico.co.th E-mail-address : pico@pico.co.th

C. Turbidity Measurement.

Check item	Turbidity	Before Calibrate	After Calibrate	Judgment
	Standard Solution			
Zero Calibration	0.00 NTU	0.00 NTU	0.00 NTU	PASS
Span Calibration	8.00 NTU	8.00 NTU	8.00 NTU	PASS
	80.0 NTU	80.0 NTU	80.0 NTU	PASS
	800 NTU	800 NTU	800 NTU	PASS

Measure at temperature 25 °C With in $\pm 5\%$ (Reading) or ± 1 NTU whichever is greater

D. DO Measurement.

Check item	DO Standard Solution	Before Calibrate	After Calibrate	Error	Judgment
Zero Calibration	(Solution of NaSO_3) 0.00 mg/l	0.00 mg/l	0.00 mg/l	0.00 mg/l	PASS
Span Calibration	(Saturated with oxygen in air) 8.11 mg/l	8.00 mg/l	8.11 mg/l	0.11 mg/l	PASS

Measure at temperature 25 °C ,With in 0 to 20 mg/L : ± 0.2 mg/l, 20 to 50 mg/L : ± 0.5 mg/l

Calibrated by : Chamaiporn Vongchalee

Approved by : Athitphong Kanchanasathian

Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID: GC/MS
Organization Name: S.P.S. Consulting service
Organization Location: 7 Soi Phaholyothin Road, Ladyao, Khet Jatujak, Bangkok, 10900
Date: March 22, 2021 10:41:18 AM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.51, GCMS.02.51
Overall Qualification Status: Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Setpoint Status: Pass

	Setpoint		Actual
Inlet Pressure:	25.0	psi	24.9

Accuracy: 0.1 psi

Agilent Recommended: <= 1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Inlet Pressure Decay

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Name: 7890
Back SSL

Setpoint Status:

Pass

Pressure: 25.0 psi

Pressure Change: -0.1 psi /5 minutes

Agilent Recommended: ≥ -2.0 and ≤ 0.5 **Overall Inlet Pressure Decay Test Status**

Pass

Inlet Pressure Accuracy

Name: 7890
Back SSL

Setpoint Status:

Pass

	Setpoint		Actual
Inlet Pressure:	25.0 psi		24.9 psi

Accuracy: 0.1 psi

Agilent Recommended: ≤ 1.2 **Overall Inlet Pressure Accuracy Test Status**

Pass

Detector Flow Accuracy

Name: 7890
Front FID

Setpoint Status:

Pass

Flow Type: Fuel

Setpoint: 30.0 mL/min Measured Flow: 29.9 mL/min

Accuracy: 0.1 mL/min

Agilent Recommended: ≤ 10.0 % setpoint (3.0 mL/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Setpoint Status:

Pass

Flow Type:

Oxidizer

Setpoint:

400.0

mL/min

Measured Flow:

399.8

mL/min

Accuracy:

0.2

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

40.0

ml/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status:

Pass

Flow Type:

Makeup

Setpoint:

25.0

mL/min

Measured Flow:

24.9

mL/min

Accuracy:

0.1

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

2.5

ml/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name:

7890

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

230.0

230.0

°C

Accuracy:

0.0

°C

Agilent Recommended:

>=

-1.0

% setpoint in K

(

-5.0

°C

)

<=

1.0

% setpoint in K

(

5.0

°C

)

Date:

March 22, 2021 10:41:18 AM

System ID:

GC/MS

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

100.0 100.0 °C

Accuracy:

0.0 °C

Agilent Recommended:

>= -1.0 % setpoint in K

(-3.7 °C)

<= 1.0 % setpoint in K

(3.7 °C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:

7890

Setpoint Status:

Pass

Setpoint/Average

Temperature:

100.0 100.05 °C

Stability:

0.1 °C

Agilent Recommended:

<= 0.5

Overall GC Oven Temperature Stability Test Status

Pass

Scouting Run

Tested Combination2

Back

SSL

/ Front

FID

Manual Injection

Name:

Not applicable

Setpoint Status:

Completed

Injection Volume on Column:

1.0 uL

Overall Scouting Run Status

Completed

Signal to Noise

Tested Combination2

Back

SSL

/ Front

FID

Date:

March 22, 2021 10:41:18 AM

System ID:

GC/MS

Manual Injection

Name: 7890

Setpoint Status: Pass

Signal to Noise: 1711991

Agilent Recommended: \geq 300000

Overall Signal to Noise Test Status

Pass

Noise and Drift

Tested Combination2	Back	SSL	/ Front	FID
Name:	7890			

Setpoint Status: Pass

Base Signal: 14.0 pA

	ASTM Noise counts	Drift counts/Hr
	384.56	178.79
Agilent Recommended:	\leq 768.00	\leq 19200.00
Status:	Pass	Pass

Overall Noise and Drift Test Status

Pass

Log Amp

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			

Setpoint Status: Pass

Overall Log Amp Test Status

Pass

RFPA

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Tested Combination1	Front	SSL	/ External	SQ			
Name:	5975C inert XL with TAD						
Setpoint Status:	Pass						
Amu:	1050	m/z	Drift After Five Minutes:	RFPV Voltage:			
			4	485			
			mV	mV			
Agilent Recommended:	>=	-100	and	<=	100	<=	1100

Overall RFPV Test Status

Pass

Tune EI

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			
Setpoint Status:	Pass			
Filament:	1			
Setpoint Status:	Pass			
Filament:	2			

Overall Tune EI Test Status

Pass

Signal to Noise EI

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			
Source:	EI - Standard (Stainless Steel)		Filament:	1
Setpoint Status:	Pass			
Signal to Noise:	925			
Agilent Recommended:	>=		320	

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Source:	El - Standard (Stainless Steel)	Filament:	2
Setpoint Status:	Pass		
Signal to Noise:	672		
Agilent Recommended:	>=	320	

Overall Signal to Noise EI Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GC/MS
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Manual Injection
Sampler Identifier	Sampler 1
Inlet	Front
Detector	External
LTM Included?	No

Tested Combination2

Injection Technique	Manual Injection
Sampler Identifier	Sampler 2
Inlet	Back
Detector	Front
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN10925120
Firmware Revision	A.01.10.3
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Detector 2

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5975C inert XL with TAD
Serial Number	US91732743
Firmware Revision	Not applicable
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Standard (Stainless Steel)
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Nattapat Hengcharoen
Logged On User Name:	nattapat.hengcharoen@agilent.com
Signature Creation Date:	March 22, 2021
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Date:	March 22, 2021 10:41:18 AM
System ID:	GC/MS

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 12:15:46 PM	Audit	SessionCreated	Session	None
March 19, 2021 12:15:46 PM	Start	Configuration	Session	None
March 19, 2021 12:15:46 PM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
March 19, 2021 12:21:07 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.51/Gc.02.51.eqp], EQP File Name: [Gc.02.51.eqp], EQP Name: [AgilentRecommended] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.51/GcMs.02.51.eqp], EQP File Name: [GcMs.02.51.eqp], EQP Name: [AgilentRecommended]
March 19, 2021 12:21:16 PM	End	Configuration	Session	None
March 19, 2021 12:21:22 PM	Start	Qualification	Session	OQ
March 19, 2021 12:21:22 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890; - Qualitative Test - No setpoints associated	None

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 1:38:58 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
March 19, 2021 1:39:56 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
March 19, 2021 1:40:12 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
March 19, 2021 1:40:14 PM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
March 19, 2021 1:40:21 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
March 19, 2021 1:40:24 PM	Start	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
March 19, 2021 1:40:34 PM	End	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
March 19, 2021 1:40:36 PM	Start	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
March 19, 2021 1:40:41 PM	End	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1

Page 2 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 1:40:42 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
March 19, 2021 1:41:20 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
March 19, 2021 1:41:22 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
March 19, 2021 1:41:24 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
March 19, 2021 1:41:37 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
March 19, 2021 1:41:40 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
March 19, 2021 1:41:42 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
March 19, 2021 1:41:55 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
March 19, 2021 1:41:56 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
March 19, 2021 1:41:59 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None

Page 3 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

Page 14 / 20

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 1:42:27 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
March 19, 2021 1:43:21 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over.
March 19, 2021 1:43:55 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
March 19, 2021 1:43:57 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
March 19, 2021 1:43:59 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
March 19, 2021 1:44:12 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
March 19, 2021 1:44:14 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
March 19, 2021 1:44:17 PM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
March 19, 2021 1:45:12 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry

Page 4 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 1:45:19 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
March 19, 2021 1:54:29 PM	Start	Execution	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	None
March 19, 2021 2:33:24 PM	Start	Execution	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	None
March 19, 2021 2:35:01 PM	Audit	AceClosed	Session	None
March 19, 2021 2:35:37 PM	Audit	AceRestarted	Session	None
March 19, 2021 2:35:38 PM	Audit	SessionReloaded	Session	None
March 19, 2021 2:35:41 PM	Start	Qualification	Session	OQ
March 19, 2021 2:35:41 PM	Start	Execution	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	None
March 19, 2021 2:36:12 PM	Audit	Data	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	Data files Path : E:\SPS\SCOUNT_FID.D\FID 1A.ch
March 19, 2021 2:36:32 PM	End	Execution	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	Run Count : 1
March 19, 2021 2:36:36 PM	Start	Execution	Signal to Noise - Manual Injection, Back SSL, Front FID: - Detector FID - L: >= 300000	None

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 2:36:46 PM	Audit	Data	Signal to Noise - Manual Injection, Back SSL, Front FID: - Detector FID - L: >= 300000	Data files Path : E:\SPS\SN_FID.D\FID1A.ch
March 19, 2021 2:37:00 PM	End	Execution	Signal to Noise - Manual Injection, Back SSL, Front FID: - Detector FID - L: >= 300000	Run Count : 1
March 19, 2021 2:37:06 PM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
March 19, 2021 3:46:48 PM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
March 19, 2021 3:47:08 PM	Audit	Data	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : E:\SPS\ND_FID.D\FID1A.ch
March 19, 2021 3:47:30 PM	End	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
March 19, 2021 3:47:32 PM	Start	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	None
March 19, 2021 3:49:54 PM	Start	Execution	RFP A - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	None
March 19, 2021 3:52:45 PM	Start	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	None

Page 6 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 3:53:16 PM	End	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	Run Count : 1
March 19, 2021 3:53:19 PM	Start	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	None
March 19, 2021 3:58:14 PM	End	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	Run Count : 1
March 19, 2021 3:59:01 PM	Start	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Standard (Stainless Steel) Filament 1 (Qualitative - No setpoints associated)	None
March 19, 2021 3:59:37 PM	End	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Standard (Stainless Steel) Filament 1 (Qualitative - No setpoints associated)	Run Count : 1
March 19, 2021 3:59:39 PM	Start	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Standard (Stainless Steel) Filament 2 (Qualitative - No setpoints associated)	None
March 19, 2021 4:00:01 PM	End	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Standard (Stainless Steel) Filament 2 (Qualitative - No setpoints associated)	Run Count : 1
March 19, 2021 4:00:05 PM	Audit	AceClosed	Session	None
March 22, 2021 9:39:45 AM	Audit	AceRestarted	Session	None
March 22, 2021 9:39:49 AM	Audit	SessionReloaded	Session	None
March 22, 2021 9:40:02 AM	Start	Qualification	Session	OQ

Page 7 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: naitapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 22, 2021 9:40:26 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 1 - L: >= 320	None
March 22, 2021 9:41:14 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 1 - L: >= 320	None
March 22, 2021 9:41:58 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 1 - L: >= 320	Data files Path : E:\SPS\SN_F1.D\DATA.MS
March 22, 2021 9:43:36 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 1 - L: >= 320	Run Count : 1
March 22, 2021 9:43:44 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 2 - L: >= 320	None
March 22, 2021 9:44:03 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 2 - L: >= 320	Data files Path : E:\SPS\SN_F2.D\DATA.MS
March 22, 2021 9:44:34 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 2 - L: >= 320	Run Count : 1

Page 8 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: nattapat.hengcharoen
Hostname: 5GG70212Y1

System Id: GC/MS
Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 22, 2021 9:44:37 AM	End	Qualification	Session	OQ
March 22, 2021 9:44:37 AM	Start	Reporting	Session	None
March 22, 2021 10:40:26 AM	Audit	Reporting	Session	Report Generated : Certificate

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.comNSC-TISI-TISI7025
CALIBRATION 0049

CERTIFICATE No : 21M3169

REFERENCE No : 60627-5

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 19-Mar-21

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 20-Mar-21

RECEIVED DATE : 19-Mar-21

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 21M3169

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 19-Mar-21
AIR PRESSURE : 1009mbar \pm 1mbar CALIBRATION DATE : 19-Mar-21
AMBIENT TEMPERATURE : 24°C \pm 1°C RELATIVE HUMIDITY : 52 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING WEIGHT OF QUALITY CALIBRATION TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23
2) STANDARD WEIGHT	E2	15843	C02210419	10-Feb-23
3) STANDARD WEIGHT	E2	QK-I-349	M2103235S	26-Mar-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT


1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 100 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000066
0.02	0.01998	0.00002	0.000066
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000067
0.50	0.49996	0.00004	0.000065
1.00	0.99997	0.00003	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00003	-0.00003	0.000070
20.00	20.00000	0.00000	0.000075
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0001	-0.0001	0.00022

5. OFF CENTER LOADING ERROR

POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID: GC/MS
Organization Name: S.P.S. Consulting service
Organization Location: 7 Soi Phaholyothin Road, Ladyao, Khet Jatujak, Bangkok, 10900
Date: March 22, 2021 10:41:18 AM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.51, GCMS.02.51
Overall Qualification Status: Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Setpoint Status: Pass

	Setpoint		Actual
Inlet Pressure:	25.0	psi	24.9

Accuracy: 0.1 psi

Agilent Recommended: <= 1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Inlet Pressure Decay

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Name: 7890
Back SSL

Setpoint Status:

Pass

Pressure:

25.0 psi

Pressure Change:

-0.1 psi /5 minutes

Agilent Recommended:

>= -2.0 and <= 0.5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 7890
Back SSL

Setpoint Status:

Pass

Setpoint

Actual

Inlet Pressure:

25.0 psi

24.9 psi

Accuracy:

0.1 psi

Agilent Recommended:

<= 1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Detector Flow Accuracy

Name: 7890
Front FID

Setpoint Status:

Pass

Flow Type:

Fuel

Setpoint:

30.0 mL/min

Measured Flow:

29.9 mL/min

Accuracy:

0.1 mL/min

Agilent Recommended:

<= 10.0 % setpoint

(3.0 mL/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Setpoint Status:

Pass

Flow Type:

Oxidizer

Setpoint:

400.0

mL/min

Measured Flow:

399.8

mL/min

Accuracy:

0.2

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

40.0

ml/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status:

Pass

Flow Type:

Makeup

Setpoint:

25.0

mL/min

Measured Flow:

24.9

mL/min

Accuracy:

0.1

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

2.5

ml/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name:

7890

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

230.0

230.0

°C

Accuracy:

0.0

°C

Agilent Recommended:

>=

-1.0

% setpoint in K

(

-5.0

°C

)

<=

1.0

% setpoint in K

(

5.0

°C

)

Date:

March 22, 2021 10:41:18 AM

System ID:

GC/MS

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

100.0

100.0

°C

Accuracy:

0.0

°C

Agilent Recommended:

>=

-1.0

% setpoint in K

(

-3.7

°C

)

<=

1.0

% setpoint in K

(

3.7

°C

)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:

7890

Setpoint Status:

Pass

Setpoint/Average

Temperature:

100.0

100.05

°C

Stability:

0.1

°C

Agilent Recommended:

<=

0.5

Overall GC Oven Temperature Stability Test Status

Pass

Scouting Run

Tested Combination2

Back

SSL

/ Front

FID

Manual Injection

Name:

Not applicable

Setpoint Status:

Completed

Injection Volume on Column:

1.0

uL

Overall Scouting Run Status

Completed

Signal to Noise

Tested Combination2

Back

SSL

/ Front

FID

Date:

March 22, 2021 10:41:18 AM

System ID:

GC/MS

Manual Injection

Name: 7890

Setpoint Status: Pass

Signal to Noise: 1711991

Agilent Recommended: \geq 300000

Overall Signal to Noise Test Status

Pass

Noise and Drift

Tested Combination2	Back	SSL	/ Front	FID
Name:	7890			

Setpoint Status: Pass

Base Signal: 14.0 pA

	ASTM Noise counts	Drift counts/Hr
	384.56	178.79
Agilent Recommended:	\leq 768.00	\leq 19200.00
Status:	Pass	Pass

Overall Noise and Drift Test Status

Pass

Log Amp

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			

Setpoint Status: Pass

Overall Log Amp Test Status

Pass

RFPA

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Tested Combination1	Front	SSL	/ External	SQ			
Name:	5975C inert XL with TAD						
Setpoint Status:	Pass						
Amu:	1050	m/z	Drift After Five Minutes:	RFPV Voltage:			
			4	485			
			mV	mV			
Agilent Recommended:	>=	-100	and	<=	100	<=	1100

Overall RFPV Test Status

Pass

Tune EI

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			
Setpoint Status:	Pass			
Filament:	1			
Setpoint Status:	Pass			
Filament:	2			

Overall Tune EI Test Status

Pass

Signal to Noise EI

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			
Source:	EI - Standard (Stainless Steel)		Filament:	1
Setpoint Status:	Pass			
Signal to Noise:	925			
Agilent Recommended:	>= 320			

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Source: EI - Standard (Stainless Steel) Filament: 2

Setpoint Status: Pass

Signal to Noise: 672

Agilent Recommended: \geq 320

Overall Signal to Noise EI Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GC/MS
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Manual Injection
Sampler Identifier	Sampler 1
Inlet	Front
Detector	External
LTM Included?	No

Tested Combination2

Injection Technique	Manual Injection
Sampler Identifier	Sampler 2
Inlet	Back
Detector	Front
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Date: March 22, 2021 10:41:18 AM
System ID: GC/MS

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN10925120
Firmware Revision	A.01.10.3
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Detector 2

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5975C inert XL with TAD
Serial Number	US91732743
Firmware Revision	Not applicable
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Standard (Stainless Steel)
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Nattapat Hengcharoen
Logged On User Name:	nattapat.hengcharoen@agilent.com
Signature Creation Date:	March 22, 2021
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Date:	March 22, 2021 10:41:18 AM
System ID:	GC/MS

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 12:15:46 PM	Audit	SessionCreated	Session	None
March 19, 2021 12:15:46 PM	Start	Configuration	Session	None
March 19, 2021 12:15:46 PM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
March 19, 2021 12:21:07 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.51/Gc.02.51.eqp], EQP File Name: [Gc.02.51.eqp], EQP Name: [AgilentRecommended] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.51/GcMs.02.51.eqp], EQP File Name: [GcMs.02.51.eqp], EQP Name: [AgilentRecommended]
March 19, 2021 12:21:16 PM	End	Configuration	Session	None
March 19, 2021 12:21:22 PM	Start	Qualification	Session	OQ
March 19, 2021 12:21:22 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890; - Qualitative Test - No setpoints associated	None

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 1:38:58 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
March 19, 2021 1:39:56 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
March 19, 2021 1:40:12 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
March 19, 2021 1:40:14 PM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
March 19, 2021 1:40:21 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
March 19, 2021 1:40:24 PM	Start	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
March 19, 2021 1:40:34 PM	End	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
March 19, 2021 1:40:36 PM	Start	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
March 19, 2021 1:40:41 PM	End	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1

Page 2 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 1:40:42 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
March 19, 2021 1:41:20 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
March 19, 2021 1:41:22 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
March 19, 2021 1:41:24 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
March 19, 2021 1:41:37 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
March 19, 2021 1:41:40 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
March 19, 2021 1:41:42 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
March 19, 2021 1:41:55 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
March 19, 2021 1:41:56 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
March 19, 2021 1:41:59 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None

Page 3 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

Page 14 / 20

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 1:42:27 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
March 19, 2021 1:43:21 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over.
March 19, 2021 1:43:55 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
March 19, 2021 1:43:57 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
March 19, 2021 1:43:59 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
March 19, 2021 1:44:12 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
March 19, 2021 1:44:14 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
March 19, 2021 1:44:17 PM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
March 19, 2021 1:45:12 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry

Page 4 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 1:45:19 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
March 19, 2021 1:54:29 PM	Start	Execution	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	None
March 19, 2021 2:33:24 PM	Start	Execution	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	None
March 19, 2021 2:35:01 PM	Audit	AceClosed	Session	None
March 19, 2021 2:35:37 PM	Audit	AceRestarted	Session	None
March 19, 2021 2:35:38 PM	Audit	SessionReloaded	Session	None
March 19, 2021 2:35:41 PM	Start	Qualification	Session	OQ
March 19, 2021 2:35:41 PM	Start	Execution	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	None
March 19, 2021 2:36:12 PM	Audit	Data	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	Data files Path : E:\SPS\SCOUNT_FID.D\FID 1A.ch
March 19, 2021 2:36:32 PM	End	Execution	GC Scouting Run - Manual Injection, Back SSL, Front FID: - Part of System Preparation - No limits associated	Run Count : 1
March 19, 2021 2:36:36 PM	Start	Execution	Signal to Noise - Manual Injection, Back SSL, Front FID: - Detector FID - L: >= 300000	None

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 2:36:46 PM	Audit	Data	Signal to Noise - Manual Injection, Back SSL, Front FID: - Detector FID - L: >= 300000	Data files Path : E:\SPS\SN_FID.D\FID1A.ch
March 19, 2021 2:37:00 PM	End	Execution	Signal to Noise - Manual Injection, Back SSL, Front FID: - Detector FID - L: >= 300000	Run Count : 1
March 19, 2021 2:37:06 PM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
March 19, 2021 3:46:48 PM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
March 19, 2021 3:47:08 PM	Audit	Data	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : E:\SPS\ND_FID.D\FID1A.ch
March 19, 2021 3:47:30 PM	End	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
March 19, 2021 3:47:32 PM	Start	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	None
March 19, 2021 3:49:54 PM	Start	Execution	RFP A - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	None
March 19, 2021 3:52:45 PM	Start	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	None

Page 6 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: nattapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 19, 2021 3:53:16 PM	End	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	Run Count : 1
March 19, 2021 3:53:19 PM	Start	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	None
March 19, 2021 3:58:14 PM	End	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Standard (Stainless Steel)	Run Count : 1
March 19, 2021 3:59:01 PM	Start	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Standard (Stainless Steel) Filament 1 (Qualitative - No setpoints associated)	None
March 19, 2021 3:59:37 PM	End	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Standard (Stainless Steel) Filament 1 (Qualitative - No setpoints associated)	Run Count : 1
March 19, 2021 3:59:39 PM	Start	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Standard (Stainless Steel) Filament 2 (Qualitative - No setpoints associated)	None
March 19, 2021 4:00:01 PM	End	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Standard (Stainless Steel) Filament 2 (Qualitative - No setpoints associated)	Run Count : 1
March 19, 2021 4:00:05 PM	Audit	AcceClosed	Session	None
March 22, 2021 9:39:45 AM	Audit	AcceRestarted	Session	None
March 22, 2021 9:39:49 AM	Audit	SessionReloaded	Session	None
March 22, 2021 9:40:02 AM	Start	Qualification	Session	OQ

Page 7 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: naitapat.hengcharoen
 Hostname: 5CG70212Y1

System Id: GC/MS
 Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 22, 2021 9:40:26 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 1 - L: >= 320	None
March 22, 2021 9:41:14 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 1 - L: >= 320	None
March 22, 2021 9:41:58 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 1 - L: >= 320	Data files Path : E:\SPS\SN_F1.D\DATA.MS
March 22, 2021 9:43:36 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 1 - L: >= 320	Run Count : 1
March 22, 2021 9:43:44 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 2 - L: >= 320	None
March 22, 2021 9:44:03 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 2 - L: >= 320	Data files Path : E:\SPS\SN_F2.D\DATA.MS
March 22, 2021 9:44:34 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Standard (Stainless Steel) using Filament 2 - L: >= 320	Run Count : 1

Page 8 / 9

Date: March 22, 2021 10:41:18 AM
 System ID: GC/MS

User Name: nattapat.hengcharoen
Hostname: 5GG70212Y1

System Id: GC/MS
Print Date: March 22, 2021 10:41:24 AM

OQ_SPS_GC-MS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 22, 2021 9:44:37 AM	End	Qualification	Session	OQ
March 22, 2021 9:44:37 AM	Start	Reporting	Session	None
March 22, 2021 10:40:26 AM	Audit	Reporting	Session	Report Generated : Certificate



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Calibration Report Total Hydrocarbon Analyzer			
Date :	02 September 2021	Brand :	HORIBA
		Model :	APHA-360CE
No.	B01	Serial No.	4211954001
Calibrator (Dilution System)			
Brand :	API	Model :	700
Last Cal. Date :	05 August 2021	Serial No.	911
Reference Standard Gas			
Standard Gas :	Methane (CH ₄)	Cylinder No. :	D595075
Certified Date :	17 March 2015	Expired Date :	17 March 2023
		Cylinder Conc. :	456 ppm
Calibrating Condition			
Pressure	1011 mmbar	Temp.	24.5 °C
		% RH	48
		Start Time :	10:00 AM
Pre-Calibration Checks			
Change Particulate Filter	Yes	Station Temp :	25.0 °C
Leak Test	Yes		
Calibration Setting			
Span Set Point	Initial Reading (Before Adj)		Final Reading (After Adj)
	Expected Concentration (PPM)	Analyzer Response (PPM)	Analyzer Response (PPM)
Zero	0	0.11	0
Span	10	10.02	10
Calibration Setting (Final)			
Span Instrument Gain:	0.997	Finish Time:	11:00 AM
APHA-360 Total Hydrocarbon Analyzer			
Test Values	Observed Value	Units	Nominal Range
Signal (CH ₄)	910.9	mV	800-1,350
Signal (THC)	915.3	mV	800-1,350
Detector	77.8	kPa	((Pressure Air/1013)x100)-20 ± 4 kPa
Purifier	19.3	kPa	8 - 25
NMC	259.2	°C	260 ± 10
Bypass	0.9	L / min	0.9 ± 0.3
Over Flow	0.8	L / Min	0.8

Calibrated by :

Phakhinai Khongkomnerd
(Mr. Phakhinai Khongkomnerd)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



**ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT**

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860-8 Fax: +66 2324 0917-8



Certificate No.: 0229SV20
Operation No.: CP2020060015

Certificate of Calibration

Equipment: Sound Calibrator
Manufacturer: ACO
Model/Type: 2127
Serial No.: 130006
ID No.: 03
Customer: S.P.S. Consunting Co., Ltd.
Address: 7 Soi Phaholyothin 24, Phaholyothin Road,
Jompol, Chatuchak, Bangkok 10900
Received Date: 12 June 2020
Calibrated Date: 15 June 2020
Issued Date: 16 June 2020
Calibrated by: Ms. Juntaporn Kunhakom

Approved by:

(Mr. Sittichai Swaksuriyawong)

Group Manager

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: 0229SV20

Calibration Report

Equipment: Sound Calibrator
Manufacturer: ACO
Model/Type: 2127
Serial No.: 130006
ID No.: 03
Ambient Temperature: $(23 \pm 2) ^\circ\text{C}$
Relative Humidity: $(50 \pm 15) \%$
Pressure: $(101.3 \pm 1.5) \text{ kPa}$

Method of Calibration :-

IEC 60942:2017

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1007-19	30 October 2020
2) Waveform Generator	33511B	MY52302264	551220083074940	17 June 2020
3) Audio Analyzing DMM	2015-P	000136E	551220083255908	3 October 2020
4) Pressure humidity and Temperature Transmitter	PTU301	L3950483	CL1-P200020 0177TE20	12 March 2021 21 April 2021

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards Instrument for Electrical function

- Micro Precision Calibration Laboratory (Thailand); A2LA Accredited Calibration No.935.06

Result of Calibration:-

1. Function : Sound pressure level

Normal Frequency (Hz)	Specified Sound Pressure level (dB)	Measured value (dB)	Deviated value ^[1] (dB)	Acceptance limit ^[3] (dB)
1000	94	93.92	-0.08	± 0.25

2. Function : Frequency

Normal Sound Pressure level (dB)	Specified Frequency (Hz)	Measured value (Hz)	Deviated value ^[2] (%)	Acceptance limit ^[3] (%)
94	1000	999.9	0.0	± 0.7

Certificate No.: 0229SV20

Calibration Report

3. Function : Total distortion + noise

Normal Sound Pressure level (dB)	Normal Frequency (Hz)	Measured value ^[4] (%)	Acceptance limit ^[5] (%)
94	1000	1.1	2.5

Uncertainty of measurement

Function	Uncertainty	Maximum-permitted uncertainty of measurement
Sound pressure level	0.10 dB	0.15 dB
Frequency	0.10 %	0.20 %
Total distortion + noise	0.40 %	0.50 %

- Note:
- [1] The deviated value is the absolute value of the difference between the measured value and the corresponding specified sound pressure level.
 - [2] The deviated value is the absolute value of the difference in percent between the measured value and the corresponding specified frequency.
 - [3] The acceptance limit is for the deviated value.
 - [4] The measured value is the total distortion + noise, measured over the frequency range from 20 Hz to 20 kHz.
 - [5] The acceptance limit is for the Measured value.

Remarks: 1. Acceptance limit was IEC 60942:2017 Class 1.

-- End of Report --



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_072/21

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	15 June 2020
		Due Date	15 June 2021

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R01	ACO	6236	00122005	22 February 2021	94.1	94.0
ACO-R11	ACO	6236	00172038	22 February 2021	94.1	94.0
ACO-R33	ACO	6236	00192045	22 February 2021	94.0	94.0
ACO-R42	ACO	6236	00192054	22 February 2021	94.0	94.0
Acoustic Certified Value : Electrical and Electronics Institute Foundation for Industrial Development					93.92 ± 0.25 dB	

Calibrated by :

Phakhinai Khongkomnerd
(Mr. Phakhinai Khongkomnerd)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 930-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_370/21

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	15 May 2021
		Due Date	15 May 2022

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B14	ACO	6236	00172034	15 August 2021	94.0	94.0
ACO-B17	ACO	6236	00172042	15 August 2021	94.1	94.0
ACO-B35	ACO	6236	00192026	15 August 2021	94.0	94.0
ACO-R35	ACO	6236	00192047	15 August 2021	94.1	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.96 ± 0.40 dB	

Calibrated by :

Phakhinai Khongkomnerd
(Mr. Phakhinai Khongkomnerd)

Approved by :

Peera Detudom
(Mr. Peera Detudom)