

ภาคผนวก ข-3

---

เอกสารขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน และ  
เอกสารรับรองการสอบเทียบของเครื่องมือตรวจวัด

### List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
<b>Stack</b>									
1	Pre-Test Console	Total Suspended Particulate Copper Total Hydrocarbons	Apex Instruments, USA.	XC-572-V 0807048	Envi Equipment Service Co., Ltd.	E21-0821	2 Sep 21	1 Sep 22	-
2	Flue gas Analyzer	Sulphur Dioxide Oxide of Nitrogen as Nitrogen Dioxide Carbon Monoxide	Testo	Testo 350 60899456	Entech Industrial Solution Co., Ltd.	G 640441	5 Aug 21	4 Aug 22	-

### List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
<b>Ambient</b>									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Tisch Environmental, Inc.	TE-5025A 3383	Tisch Environmental, Inc.	27072020	27 Jul 20	26 Jul 22	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	22P800	12 Mar 22	11 Mar 23	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	21P2500	21 Jul 21	20 Jul 22	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	22H771	5 Apr 22	4 Apr 23	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1201778108	UAE Consultant Co., Ltd.	08122021	8 Dec 21	7 Dec 22	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1201778109	UAE Consultant Co., Ltd.	08122021	8 Dec 21	7 Dec 22	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1201778105	UAE Consultant Co., Ltd.	17112021	17 Nov 21	16 Nov 22	-
8	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	CC159599 2015PSIG	Airgas an Air Liquide company	E04N99E15A01QC	30 Jul 19	30 Jul 22	-
9	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1201497730	UAE Consultant Co., Ltd.	30112021	30 Nov 21	29 Nov 22	-
10	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1201497732	UAE Consultant Co., Ltd.	30112021	30 Nov 21	29 Nov 22	-
11	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1201497733	UAE Consultant Co., Ltd.	30112021	30 Nov 21	29 Nov 22	-
12	Standard Gases (Mixture)	Carbon Monoxide	Airgas	CC159599 2015PSIG	Airgas an Air Liquide company	160-401526192-1	30 Jul 19	30 Jul 22	-

**List of Instruments Certification for Air & Noise Quality Analysis**

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
<b>Ambient</b>									
13	Wind Speed/Wind Direction	WS/WD	LSI LASTEM	E-LOG305 19040308	Thai Meteorological Department	385/21	16 Aug 21	15 Aug 22	-
14	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6171	Innovative Instrument Co.,Ltd.	21-ACT-327	24 Aug 21	23 Aug 22	-
15	Sound Level Meter	$L_{Aeq\ 24\ hr}$ , $L_{A90}$ , $L_{Adiv}$ , $L_{Amax}$	Larson Davis	LxT2 0005286	Sithiporn Associates Co., Ltd.	ACL22081	25 Jan 22	24 Jan 23	-
16	Sound Level Meter	$L_{Aeq\ 24\ hr}$ , $L_{A90}$ , $L_{Adiv}$ , $L_{Amax}$	Larson Davis	LxT2 0005394	Innovative Instrument Co.,Ltd.	22-ACT-034	21 Jan 22	20 Jan 23	-
17	Sound Level Meter	$L_{Aeq\ 24\ hr}$ , $L_{A90}$ , $L_{Adiv}$ , $L_{Amax}$	Larson Davis	LxT2 0005286	Sithiporn Associates Co., Ltd.	ACL22081	25 Jan 22	24 Jan 23	-
18	Sound Level Meter	$L_{Aeq\ 24\ hours}$ , $L_{Adiv}$ , $L_{A90}$ , $L_{Amax}$	Larson Davis	LxT2 0006614	Innovative Instrument Co.,Ltd.	22-ACT-104	11 Feb 22	10 Feb 23	-
19	Sound Level Meter	$L_{Aeq\ 24\ hr}$ , $L_{A90}$ , $L_{Adiv}$ , $L_{Amax}$	Larson Davis	LxT2 0005396	Innovative Instrument Co.,Ltd.	22-ACT-105	11 Feb 22	10 Feb 23	-

**List of Instruments Certification for Water Quality Analysis**

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
<b>Water</b>									
1	pH Meter	pH	Horiba	LAQUA-PH210 HA1F0002	Technology Promotion Association (Thailand-Japan)	21CH1607	19 Nov 21	18 Nov 22	-

## CERTIFICATE OF CALIBRATION

**Customer** : United Analyst and Engineering Consultant Co., Ltd.  
**Address** : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhamong, Bangkok 10260  
**Description of Equipment** : Console meter  
**Manufacturer** : Apex Instrument  
**Model Number** : XC-572-V  
**Serial Number** : 0807048  
**ID./Control No.** : -  
**Environment Conditions** : Temperature (25 ± 2) °C  
 : Humidity (50 ± 15) % RH  
**Cal. Date** : 02/09/2021  
**Issue Date** : 02/09/2021

### Calibration Method or Calibration Procedure Used

US EPA Method (United State Environmental Protection Agency)

This certificate is traceable to national standard, which realize the units of measurement according to the International System of Units (SI).

### Result of Calibration

This certificate may not be reproduced other than in full except with prior Written approval of the Technical Manager, Envi Equipment Service Company Limited.

These reported uncertainties of measurement are expanded by a coverage factor of k=2, providing a 95% confidence level

Calibrated by : 

Approved by

(Mr. Manu Fuekthong)  
 Technical Manager

เอกสารไม่ควบคุม

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
<b>Workplace</b>									
1	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Svantek	SV35A 73249	Innovative Instrument Co.,Ltd.	21-ACT-187	28 May 21	27 May 22	-
2	Sound Level Meter	$L_{Aeq}$ 8 hours $L_{Amax}$	Rion, Japan	NL-42 00409050	Innovative Instrument Co.,Ltd.	22-ACT-067	3 Feb 22	2 Feb 23	-
3	Sound Level Meter	$L_{Aeq}$ 8 hours $L_{Amax}$	Rion, Japan	NL-42 00709682	Sithiporn Associates Co., Ltd.	ACL22075	25 Jan 22	24 Jan 23	-
4	Sound Level Meter	$L_{Aeq}$ 8 hours $L_{Amax}$	Larson Davis	LxT2 0005400	Innovative Instrument Co.,Ltd.	22-ACT-036	21 Jan 22	20 Jan 23	-
5	Sound Level Meter	$L_{Aeq}$ 8 hours $L_{Amax}$	Larson Davis	LxT2 0005402	Innovative Instrument Co.,Ltd.	22-ACT-103	11 Feb 22	10 Feb 23	-
6	Sound Level Meter	$L_{Aeq}$ 8 hours $L_{Amax}$	Larson Davis	LxT2 0006614	Innovative Instrument Co.,Ltd.	22-ACT-104	11 Feb 22	10 Feb 23	-
7	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104IS 67627	Innovative Instrument Co.,Ltd.	21-ACT-361	20 Sep 21	19 Sep 22	-
8	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104 91923	Innovative Instrument Co.,Ltd.	22-ACT-114	17 Feb 22	16 Feb 23	-
9	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104 91925	Innovative Instrument Co.,Ltd.	22-ACT-033	21 Jan 22	20 Jan 23	-
10	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Svantek	SV36 107224	Innovative Instrument Co.,Ltd.	21-ACT-326	24 Aug 21	23 Aug 22	-




METHOD 5 CONSOLE CALIBRATION  
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425  
5-POINT METRIC UNIT


Meter Console Information		Calibration Conditions		Factors/Conversions	
Console Model Number	XC-572-V	Date	Time	Std Temp	293 K
Console Serial Number	0807048	Calibration Reference No.	-	Std Press	760 mm Hg
DGM Model Number	SK25EX	Barometric Pressure	761.00	K <sub>i</sub>	0.386
DGM Serial Number	00003811	Calibration Meter Gamma	0.999	Console Leak Check PASS	

Calibration Data												
Run Time		Metering Console					Calibration Meter					
Elapsed (Q)	DGM Orifice DH (P <sub>m</sub> )	Volume		Outlet Temp Initial (t <sub>m</sub> )	Outlet Temp Final (t <sub>m</sub> )	Volume	Volume		Outlet Temp Initial (t <sub>m</sub> )	Outlet Temp Final (t <sub>m</sub> )	Volume	Final (V <sub>ref</sub> )
		Initial (V <sub>m</sub> )	Final (V <sub>m</sub> )				Initial (V <sub>ref</sub> )	Final (V <sub>ref</sub> )				
min	mm H <sub>2</sub> O	m <sup>3</sup>	m <sup>3</sup>	°C	°C	m <sup>3</sup>	m <sup>3</sup>	m <sup>3</sup>	°C	°C	m <sup>3</sup>	m <sup>3</sup>
12.27	13.0	544.3460	544.4860	25	25	32.17136	32.30750	24	24	24	24	24
12.40	13.0	544.4860	544.6260	24	24	32.30750	32.44346	24	24	24	24	24
8.77	26.0	544.6320	544.7720	24	24	32.44932	32.58574	24	24	24	24	24
8.58	26.0	544.7720	544.9120	24	24	32.58574	32.72218	24	24	24	24	24
14.17	40.0	544.9100	545.1000	24	24	32.72886	33.00206	23	23	23	23	23
14.17	40.0	545.1900	545.4790	24	24	33.00296	33.27582	23	23	23	23	23
10.45	70.0	545.4860	545.7670	25	25	33.28250	33.55462	23	23	23	23	23
10.42	70.0	545.7670	546.0470	26	26	33.55462	33.82500	23	23	23	23	23
9.18	90.0	546.0500	546.3390	26	26	33.83612	34.10576	23	23	23	23	23
9.15	90.0	546.3390	546.6190	27	27	34.10576	34.37388	23	23	23	23	23

**Note:** For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is  $\pm 0.02$ .  
For  $\Delta H_{H_2O}$ , orifice pressure differential that equates to 0.75 cfm (0.0212 m<sup>3</sup>/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is  $\pm 0.2$  inches (5.1 mm) H<sub>2</sub>O.

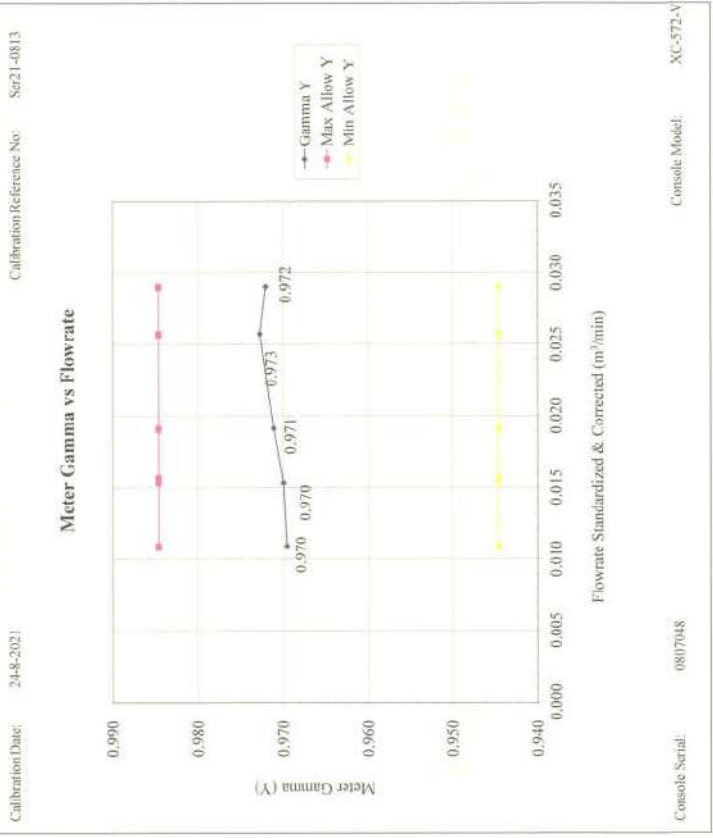

เอกสารไม่ควบคุม

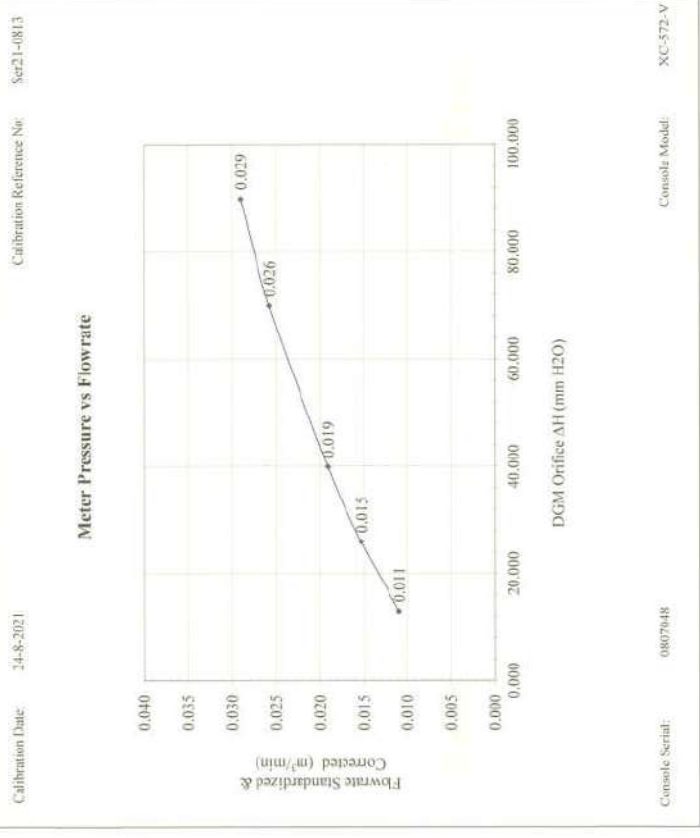

เอกสารไม่ควบคุม

## THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information		Calibration Conditions	
Console Model Number	XC-572-V	Date	07/07/2021 03:30 PM
Console Serial Number	0807048	Calibration Reference No.	
DGM Model Number	SK25EX	Reference Thermometer	DIGICON
DGM Serial Number	00003811	Serial Number	183169105
Meter Box Model Number	JENCO 765 KF		
Meter Box Serial Number	JC 08944		

Results										
Console Thermocouple Simulator										
Channel and test point	Meter Box Channel Temperature Reading (°C)									
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	816.0 1038.0
Stack	-17.0	26.0	39.0	94.0	150.0	261.0	372.0	482.0	593.0	816.0 1039.0
Aux	-17.0	26.0	39.0	94.0	150.0					
Probe	-17.0	26.0	39.0	94.0	150.0					
Filter	-17.0	26.0	39.0	94.0	150.0					
Oven	-	-	-	-	-					
Exit	-17.0	26.0	39.0							

Tolerance Range			Meter	
Stack	± 1.50%	Absolute	Enter	± 3.0 °C
Probe	± 3.0 °C		Exit	± 2.0 °C
Filter	± 3.0 °C			

เอกสารไม่ควบคุม

Instrument description : Flue gas Analyzer  
Instrument model : Teso 350 New  
Instrument serial no. : 60839456  
ID no. or control no. : UAE.EFM.003/2560  
Manufacturer : testb SE  
Probe description : -  
Probe model : -  
Probe serial : -  
Customer name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Customer address : 81 SOI UDOMSUK41, SUKHUMVIT ROAD, BANGCHAK PRAKANONG  
BANGKOK 10260

Total pages of certificate : 2 Pages  
Receiving no. : L-211963  
Receiving date. : 14-Jul-21

Parameter of calibration : Gas Calibration (Oxygen 2.501, 10.00, 21.00 %vol, Carbon Monoxide 80.23, 209.9, 1003 ppm, Nitric Oxide 10.08, 150.9, 320.6 ppm, Sulphur Dioxide 50.04, 100.9, 601.1 ppm, Nitrogen Dioxide 10.20, 80.62, 202.2 ppm)

Condition of UUC. : Used  
Ambient condition : All of the Measurement were carried out the stabilized laboratory  
Temperature : 23 ± 5 °C  
Humidity : 55 ± 15 %RH

Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Lakse, Bangkok 10210

Calibration procedure no. : WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.  
This certificate is applied only to item under test Environmental condition.  
This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory.  
Calibration certificates without signature and seal not valid.  
This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 04-Aug-21



Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O <sub>2</sub> ) 2.501 % Vol	2431/19	Linde	16-Jul-23
Oxygen (O <sub>2</sub> ) 10.00 % Vol	2453/19	Linde	18-Jul-23
Oxygen (O <sub>2</sub> ) 21.00 % Vol	2426/19	Linde	16-Jul-23
Carbon monoxide (CO) 80.97 ppm	2643/21	Linde	24-Jun-23
Carbon monoxide (CO) 309.9 ppm	2603/21	Linde	22-Jun-23
Carbon monoxide (CO) 1003 ppm	2629/21	Linde	23-Apr-23
Nitric Oxide (NO) 10.08 ppm	3241/21	Linde	25-Jul-23
Nitric Oxide (NO) 150.9 ppm	2657/21	Linde	27-Jun-23
Nitric Oxide (NO) 320.6 ppm	2944/21	Linde	02-Jul-23
Sulphur Dioxide (SO <sub>2</sub> ) 50.04 ppm	3205/21	Linde	25-Jul-23
Sulphur Dioxide (SO <sub>2</sub> ) 100.9 ppm	4942/20	Linde	20-Nov-22
Sulphur Dioxide (SO <sub>2</sub> ) 601.1 ppm	3204/21	Linde	20-Jul-23
Nitrogen Dioxide (NO <sub>2</sub> ) 10.20 ppm	2929/19	Linde	27-Aug-21
Nitrogen Dioxide (NO <sub>2</sub> ) 80.62 ppm	3240/21	Linde	25-Jul-23
Nitrogen Dioxide (NO <sub>2</sub> ) 202.2 ppm	3239/21	Linde	20-Jul-23

Measured room conditions

Temperature : 23.2 °C Humidity : 53.8 %RH Pressure : 1015.3 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,100 ml/min Gas pressure : 1021.6 mbar

Calibration Results (without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O <sub>2</sub> (%Vol)	2.501	2.47	-0.031	0.20
O <sub>2</sub> (%Vol)	10.00	9.86	-0.14	0.40
O <sub>2</sub> (%Vol)	21.00	21.14	0.14	0.80
CO (ppm)	80.97	82	1.03	2.8
CO (ppm)	309.9	310	0.1	11
CO (ppm)	1003	999	-4	34
NO (ppm)	10.08	9	-1.08	3.0
NO (ppm)	150.9	151	0.1	5.0
NO (ppm)	320.6	322	1.4	10
SO <sub>2</sub> (ppm)	50.04	49	-1.04	5.0
SO <sub>2</sub> (ppm)	100.9	101	0.1	5.0
SO <sub>2</sub> (ppm)	601.1	599	-2.1	14
NO <sub>2</sub> (ppm)	10.20	9.9	-0.30	1.5
NO <sub>2</sub> (ppm)	80.62	80.3	-0.32	5.0
NO <sub>2</sub> (ppm)	202.2	198.9	-3.3	5.0

Remark : 1 cm<sup>3</sup>/mol = 1 %vol., 1 µmol/mol = 1 ppm.

End of Report



RECALIBRATION  
DUE DATE:  
July 27, 2021

Certificate of Calibration

Cal. Date: July 27, 2020	Rootsmeier S/N: 438320	Ta: 298
Operator: Jim Tisch		Pa: 749.3
Calibration Model #: TE-5025A	Calibrator S/N: 3383	°K mm Hg

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H <sub>2</sub> O)
1	1	2	1	1.4020	3.2	2.00
2	3	4	1	1.0000	6.3	4.00
3	5	6	1	0.8920	7.8	5.00
4	7	8	1	0.8430	8.7	5.50
5	9	10	1	0.7010	12.7	8.00

Data Tabulation

Vstd (m3)	Qstd (k-axis)	$\sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (k-axis)	$\sqrt{\Delta H \left( \frac{Pa}{Pa} \right)}$ (y-axis)
0.9817	0.7002	1.4042	0.9957	0.7102	0.8919
0.9776	0.9776	1.9859	0.9916	0.9916	1.2613
0.9757	1.0938	2.2203	0.9896	1.1094	1.4101
0.9745	1.1560	2.3286	0.9884	1.1725	1.4796
0.9692	1.3826	2.8084	0.9831	1.4024	1.7837
<b>QSTD</b>	<b>m= 2.04993</b>	<b>b= -0.02762</b>	<b>QA</b>	<b>m= 1.28363</b>	<b>b= -0.01754</b>
	<b>r= 0.99985</b>			<b>r= 0.99985</b>	

Calculations

Vstd = $\Delta Vol((Pa \cdot \Delta P) / Pstd) / (Tstd / Ta)$	Va = $\Delta Vol((Pa \cdot \Delta P) / Pa)$
Qstd = Vstd / ΔTime	Qa = Va / ΔTime
For subsequent flow rate calculations:	
Qstd = $1/m \left( \sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)} - b \right)$	
Qa = $1/m \left( \sqrt{\Delta H \left( \frac{Pa}{Pa} \right)} - b \right)$	

Standard Conditions

Tstd: 298.15 °K	Key
Pstd: 760 mm Hg	
ΔH: calibrator manometer reading (in H <sub>2</sub> O)	
ΔP: rootsmeier manometer reading (mm Hg)	
Ta: actual absolute temperature (°K)	
Pa: actual barometric pressure (mm Hg)	
b: intercept	
m: slope	

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30

Tisch Environmental, Inc.  
145 South Miami Avenue  
Village of Cleves, OH 45002

www.tisch-env.com

เอกสารไม่ควบคุม  
Tel: (513) 467-9009  
Fax: (513) 467-9009



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
53/44 PATANAKARN ROAD SOI 18, SUANILANG, SUANILANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484

## Certificate of Calibration

Certificate No.: 22P800  
Page: 1 of 2

Equipment: U-Tube Manometer  
Manufacturer: Dwyer  
Model: 1221-36-WM  
Serial No.:  
ID No.: UAE EFM 022/2580  
Condition As-Received: Used Item  
Received Date: 03 March 2022  
Calibration Date: 12 March 2022

Submitted by: United Analyst and Engineering Consultant Co., Ltd.  
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,  
Phrakhanong, Bangkok 10260

Reference: 2203-0131WSC  
Ambient Temperature: ( 23 ± 2 ) °C  
Relative Humidity: ( 50 ± 15 ) %  
Atmospheric Pressure: 1010 mbar  
Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

### Condition of this result of calibration

1. Reference standards instruments :
- | Instrument          | Model  | Serial No. | Certificate No. | Due Date    |
|---------------------|--------|------------|-----------------|-------------|
| Pressure Calibrator | PC106P | 1189       | MP-0110-21      | 09 Aug 2022 |
2. This result of calibration was made on requested at the point specified by customer.  
3. Scale and conversion factor is 1 kPa = 4.0146293 inH<sub>2</sub>O  
4. This instrument was used clean air as pressure media.  
5. This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.  
6. This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.  
7. The certificate is valid only to the item calibrated on date and place of calibration.  
8. This Certification is traceable to the International System of Unit maintained at:-  
-National Institute of Metrology Thailand (NIMT)

Calibrated by: Suwit Aussanee  
Issue Date: 14 March 2022

Approved Signatory

Atatapol Panurach

เอกสารไม่ควบคุม

B 0282413



Cert.No.: 22P800  
Page: 2 of 2

Result of calibration:- Without adjustment  
Function:- Pressure Measurement  
Increasing Pressure  
Range: 0 inH<sub>2</sub>O to 36 inH<sub>2</sub>O  
Scale Interval: 0.1 inH<sub>2</sub>O ( The Fifth Estimate )

UUC Indication		ΔP (inH <sub>2</sub> O)	Error (inH <sub>2</sub> O)
Applied Pressure (inH <sub>2</sub> O)	High-port side (inH <sub>2</sub> O)		
0.00	0.00	0.00	0.00
2.00	1.00	-1.00	0.00
4.00	2.00	-2.00	0.00
6.00	3.00	-3.00	0.00
8.00	4.00	-4.00	0.00
10.00	5.00	-5.02	0.02
12.00	6.00	-6.02	0.02
14.00	7.00	-7.04	0.04
16.00	8.00	-8.04	0.04
18.00	9.00	-9.04	0.04
20.00	10.00	-10.04	0.04
22.00	11.00	-11.02	0.02
24.00	12.00	-12.02	0.02
26.00	13.00	-13.02	0.02
28.00	14.00	-14.04	0.04
30.00	15.00	-15.04	0.04
32.00	16.00	-16.04	0.04
34.00	16.98	-17.06	0.04
36.80	17.98	-18.00	0.18

The uncertainty of measurement was ± 0.11 inH<sub>2</sub>O

\* UUC = Unit Under Calibration

\* ΔP = High-port side - Low-port side

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม  
B 1099526





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES  
5344 PATTANAKARN ROAD SOI 18, SUANLIANG, BANGKOK 10250  
TEL. 0-2717-3090-24 FAX. 0-2719-9484



NSC-T8-T81713  
CALIBRATION 0018

## Certificate of Calibration

Certificate No. : 21P2500  
Page : 1 of 2

Equipment: Aneroid Barometer  
Manufacturer: Barigo  
Model: -  
Serial No.: -  
ID No.: UAE/ANV/123/2550  
Condition As-Received: Used Item  
Received Date: 20 July 2021  
Calibration Date: 21 July 2021

Reference: 2107-0570WSC  
Ambient Temperature: ( 23 ± 2 ) °C  
Relative Humidity: ( 50 ± 15 ) %  
Atmospheric Pressure: 1009 mbar  
Submitted by: United Analyst and Engineering Consultant Co., Ltd.  
81 Soi Udomsuk 41 Sukhumvit Road, Bangkok,  
Prakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

### Condition of this result of calibration

1. Reference standards instruments :

- 1) Standard Barometer  
Instrument: DP142 Model: 1422505046 Certificate No. MP-0053-21 Due Date 08 Apr 2022
2. This instrument was installed in vertical orientation and center of the dial was used as the reference level.
3. This result of calibration was made on requested at the point specified by customer.
4. This instrument was used clean air as pressure media.
5. The certificate is valid only to the item calibrated on date and place of calibration.
6. This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology (NIMT)

Calibrated by : Suwit Aussanee  
Issue Date : 22 July 2021

Approved Signatory

Atsapol Panurach

เอกสารไม่ควบคุม

0264463



Cert.No.: 21P2500  
Page: 2 of 2

Result of calibration:- Without adjustment  
Function:- Absolute Pressure Measurement  
Scale Interval: 1 hPa (The Fifth Estimate )  
Range: 900 hPa to 1030 hPa

Increasing Pressure									
Applied Pressure (hPa)	956.36	968.61	979.40	990.51	1000.62	1010.72	1020.79	1031.19	
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0	
Error (hPa)	3.64	1.39	0.60	-0.51	-0.62	-0.72	-0.76	-1.19	

Decreasing Pressure									
Applied Pressure (hPa)	1031.28	1020.72	1010.67	1000.58	990.42	979.33	968.54	956.29	
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0	
Error (hPa)	-1.28	-0.72	-0.67	-0.58	-0.42	0.67	1.46	3.71	

The uncertainty of measurement was ± 0.30 hPa

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม  
Atsapol P.  
0262244



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SCI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL: 0-2717-3000-24 FAX: 0-2719-9484



## Certificate of Calibration

Certificate No. : 22H1771  
Page : 1 of 2

Equipment : Dial Thermo-Hygrometer  
Manufacturer: Baribo  
Model :  
Serial No.:  
ID No.: UAE.ANY.003/2548  
Condition As-Received: Used Item  
Received Date: 30 March 2022  
Calibration Date: 01 April 2022  
to 05 April 2022  
Reference: 2203-1124WSC  
Ambient Temperature: ( 25 ± 3 ) °C  
Relative Humidity: ( 50 ± 20 ) %

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udornasuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260

**Procedure used:** Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

### Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Chilled Mirror Hygrometer Sensor	Dew Prime II	31863	19714	17 Sep 2022
2) Standard Humidity/Temperature Meter	400	10203027	TH-0063-21	01 Jul 2022

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Standards and Technology (NIST), The United States of America  
-National Institute of Metrology Thailand (NIMT)

Calibrated by : Somchai Dumwor  
Issue Date : 08 April 2022

Approved Signatory :

[ / ] Chaitit Weerawat  
[ / ] Pombhippa Tamayakul  
[ / ] Viporn Tantiyawutti

เอกสารไม่ควบคุม

B 0285423



Cert. No.: 22H1771  
Page.: 2 of 2

Result of Calibration:-

Function: Humidity measurement.

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	42	1.9	1.6
25.0	60.0	61	1.0	1.3
25.0	80.0	78	-2.0	2.0

Result of Calibration:-

Function: Temperature measurement.

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
20.02	20.0	-0.02	0.72
29.98	30.0	0.02	0.72
35.02	35.0	-0.02	0.72
40.03	40.0	-0.03	0.72

UUC\* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-000-

เอกสารไม่ควบคุม

a 1104141



**MULTI-POINT GAS TEST REPORT**


Test Date : Dec 8, 2021

Equipment : Gas Analyzer (NO<sub>2</sub>)  
Manufacturer : Thermo Scientific Model : 42i  
Serial Number : 1201778108

**Standard Gas Concentration**  
Sulphur Dioxide (SO<sub>2</sub>) 44.75 PPM Manufacturer : Thermo Scientific  
Nitric Oxide (NO) 45.35 PPM Model : 146i  
Methane (CH<sub>4</sub>) - PPM Serial Number : 1180540071  
Carbon Monoxide (CO) 1007  
Cylinder No. : CCL59599  
Expiration Date : Jul 30, 2022

**Multi-point gas test data**

Level	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error (ppb)	Percent Error	[% Error]
Level 1	Zero	0.0	1.2	1.20	1.20
Level 2	20.00%	100.0	101.4	1.40	1.38
Level 3	40.00%	200.0	201.3	1.30	0.65
Level 4	60.00%	300.0	301.3	1.30	0.43
Level 5	80.00%	400.0	400.7	0.70	0.17
Remark : Measuring Range 500.0 ppb					0.77
Acceptable Limit $\pm 5\%$					
Average Difference (%)					0.77

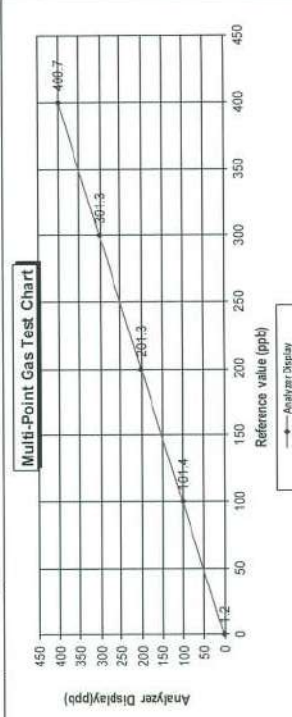

Signature: [Signature]  
Date: Dec 2021

**MULTI-POINT GAS TEST REPORT**


Test Date : Dec 8, 2021

Equipment : Gas Analyzer (NO<sub>2</sub>)  
Manufacturer : Thermo Scientific Model : 42i  
Serial Number : 1201778109

**Standard Gas Concentration**  
Sulphur Dioxide (SO<sub>2</sub>) 44.75 PPM Manufacturer : Thermo Scientific  
Nitric Oxide (NO) 45.35 PPM Model : 146i  
Methane (CH<sub>4</sub>) - PPM Serial Number : 1180540071  
Carbon Monoxide (CO) 1007  
Cylinder No. : CCL59599  
Expiration Date : Jul 30, 2022

**Multi-point gas test data**

Level	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error (ppb)	Percent Error	[% Error]
Level 1	Zero	0.0	1.1	1.10	1.10
Level 2	20.00%	100.0	100.7	0.70	0.70
Level 3	40.00%	200.0	200.5	0.50	0.25
Level 4	60.00%	300.0	300.3	0.30	0.10
Level 5	80.00%	400.0	400.7	0.70	0.17
Remark : Measuring Range 500.0 ppb					0.46
Acceptable Limit $\pm 5\%$					
Average Difference (%)					0.46

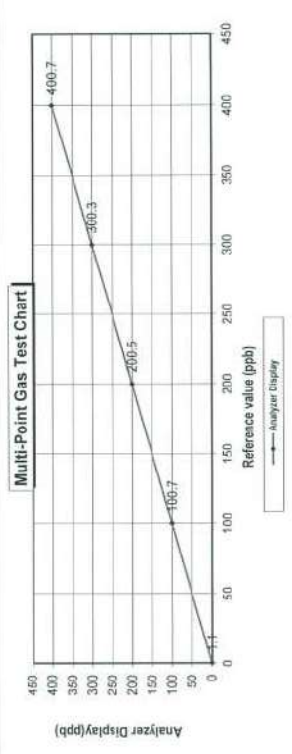

Signature: [Signature]  
Date: Dec 2021



MULTI-POINT GAS TEST REPORT

Test Date : Nov 17/2021


Equipment : Gas Analyzer (NO<sub>x</sub>) Model : 42i  
Manufacturer : Thermo Scientific Serial Number : 1201778105

Standard Gas Concentration  
Sulphur Dioxide (SO<sub>2</sub>) 44.75 PPM Manufacturer : Thermo Scientific  
Nitric Oxide (NO) 45.35 PPM Model : 146i  
Methane (CH<sub>4</sub>) - PPM Serial Number : 1180540071  
Carbon Monoxide (CO) 1007 PPM  
Cylinder No. : CC159599  
Expiration Date : Jul 30, 2022

Multi-point gas test data

Level	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	% Error
Level 1	Zero	0.0	0.90	0.90	0.90
Level 2	20.00%	100.6	0.60	0.60	0.60
Level 3	40.00%	201.3	1.30	0.65	0.65
Level 4	60.00%	301.2	1.20	0.40	0.40
Level 5	80.00%	400.5	0.50	0.12	0.12

Remark : Measuring Range: 500.0 ppb  
Acceptable Limit  $\pm$  5%

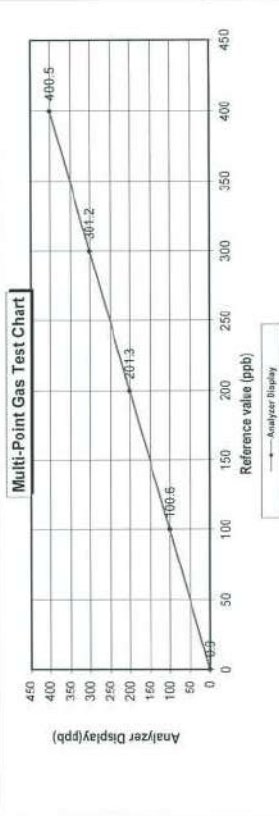

CERTIFICATE OF ANALYSIS  
Grade of Product: EPA Protocol

Part Number: E04NI99E15A01QC Reference Number: 160-401526192-1  
Cylinder Number: CC159599 Cylinder Volume: 144.4 CF  
Laboratory: 124 - Plumsteadville - PA Cylinder Pressure: 2015 PSIG  
PGVP Number: A12019 Valve Outlet: 660  
Gas Code: CO,NO,NOX,SO<sub>2</sub>,BALN Certification Date: Jul 30, 2019  
Expiration Date: Jul 30, 2022

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/351, using the assay procedure listed. Analytical Methodology used: Gravimetric. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. The volume of gas is significant unless otherwise noted. All concentrations are on a volume/volume basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	44.76 PPM	G1	$\pm$ 0.8% NIST Traceable	07/23/2019, 07/30/2019
NITRIC OXIDE	45.00 PPM	44.76 PPM	G1	$\pm$ 0.8% NIST Traceable	07/23/2019, 07/30/2019
SULFUR DIOXIDE	45.00 PPM	45.35 PPM	G1	$\pm$ 1% NIST Traceable	07/23/2019, 07/30/2019
CARBON MONOXIDE	1000 PPM	1007 PPM	G1	$\pm$ 0.4% NIST Traceable	07/23/2019
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	18060121	KAL004215	249.9 PPM NITRIC OXIDE/NITROGEN	$\pm$ 0.4%	Nov 08, 2023
NTRM	052411	KAL004307	50.03 PPM NITRIC OXIDE/NITROGEN	$\pm$ 0.80%	Mar 12, 2024
NTRM	18060121	KAL004215	250.0 PPM NOX/NITROGEN	$\pm$ 0.4%	Nov 08, 2023
NTRM	052411	KAL004307-NOX	50.03 PPM NOX/NITROGEN	$\pm$ 0.80%	Mar 12, 2024
NTRM	0141709	KAL003190	49.67 PPM SULFUR DIOXIDE/NITROGEN	$\pm$ 1.0%	Jun 20, 2022
NTRM	072508	KAL004570	970.0 PPM CARBON MONOXIDE/NITROGEN	$\pm$ 0.4%	May 14, 2021

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
CO MKS FTIR 000929062	FTIR	Jul 19, 2019
NO MKS FTIR 000929062	FTIR	Jul 22, 2019
NO MKS FTIR 000929062	FTIR	Jul 22, 2019
SO2 MKS FTIR 000929062	FTIR	Jul 22, 2019

Triad Data Available Upon Request

NOTES: RAN# 51319-CM03  
PO# 5219002210  
GROSS WEIGHT: 28.6 KG  
NET WEIGHT: 4.1 KG



Signature on file

Approved for Release

# MULTI-POINT GAS TEST REPORT


Test Date : Nov 30, 2021

Equipment : Gas Analyzer (CO) Model : 48i  
Manufacturer : Thermo Scientific Serial Number : 1201497730

**Standard Gas Concentration**  
Sulphur Dioxide (SO<sub>2</sub>) 44.75 PPM Manufacturer : Thermo Scientific  
Nitric Oxide (NO) 45.35 PPM Model : 146i  
Methane (CH<sub>4</sub>) - PPM Serial Number : 1180540071  
Carbon Monoxide (CO) 1007 PPM  
Cylinder No. : CC159599  
Expiration Date : Jul 30, 2022

## Multi-point gas test data

Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error ]
Level 1 Zero	0.0	0.6	0.6	0.6
Level 2 20.00%	10.3	0.3	2.9	2.9
Level 3 40.00%	20.6	0.6	2.9	2.9
Level 4 60.00%	30.5	0.5	1.6	1.6
Level 5 80.00%	40.4	0.4	1.0	1.0
Remark : Measuring Range 50.0 ppm				1.81
:Acceptable Limit $\pm$ 5%				
Average Difference (%)				

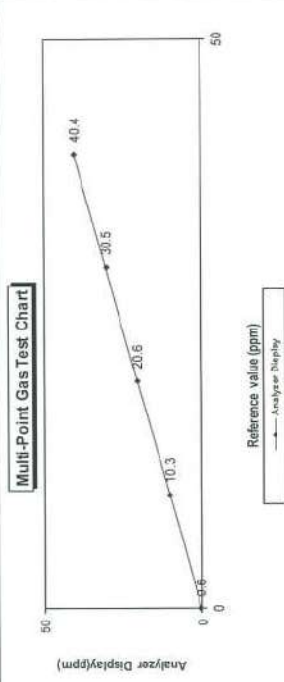

20/11/2021 14:08

# MULTI-POINT GAS TEST REPORT


Test Date : Nov 30, 2021

Equipment : Gas Analyzer (CO) Model : 48i  
Manufacturer : Thermo Scientific Serial Number : 1201497732

**Standard Gas Concentration**  
Sulphur Dioxide (SO<sub>2</sub>) 44.75 PPM Manufacturer : Thermo Scientific  
Nitric Oxide (NO) 45.35 PPM Model : 146i  
Methane (CH<sub>4</sub>) - PPM Serial Number : 1180540071  
Carbon Monoxide (CO) 1007 PPM  
Cylinder No. : CC159599  
Expiration Date : Jul 30, 2022

## Multi-point gas test data

Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error ]
Level 1 Zero	0.0	1.2	1.2	1.2
Level 2 20.00%	10.0	11.2	10.7	10.7
Level 3 40.00%	20.0	20.9	4.3	4.3
Level 4 60.00%	30.0	30.7	2.3	2.3
Level 5 80.00%	40.0	40.6	1.5	1.5
Remark : Measuring Range 50.0 ppm				4.00
:Acceptable Limit $\pm$ 5%				
Average Difference (%)				

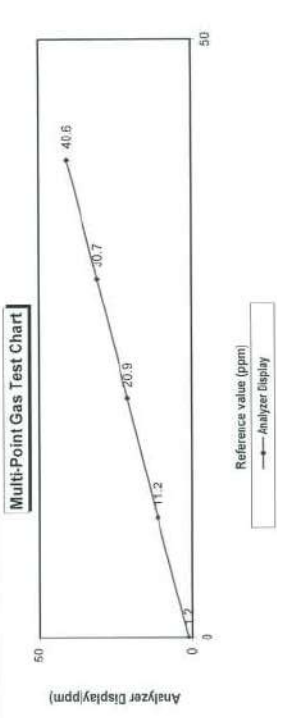

20/11/2021 14:08

MULTI-POINT GAS TEST REPORT

Test Date : Nov 30, 2021


Equipment : Gas Analyzer (CO) Model : 481  
Manufacturer : Thermo Scientific Serial Number : 1201497733

Standard Gas Concentration  
Sulphur Dioxide (SO<sub>2</sub>) 44.75 PPM Manufacturer : Thermo Scientific  
Nitric Oxide (NO) 45.35 PPM Model : 1461  
Methane (CH<sub>4</sub>) - PPM Serial Number : 1180540071  
Carbon Monoxide (CO) 1007 PPM  
Cylinder No. : CC159599  
Expiration Date : Jul 30, 2022

Multi-point gas test data

Level	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	1.5	1.5	1.5
Level 2	20.00%	10.9	0.9	8.3	8.3
Level 3	40.00%	20.7	0.7	3.4	3.4
Level 4	60.00%	31.2	1.2	3.8	3.8
Level 5	80.00%	40.5	0.5	1.2	1.2
Remark : Measuring Range 50.0 ppm			Average Difference (%)		
Acceptable Limit $\pm 5\%$			3.64		

Multi-Point Gas Test Chart

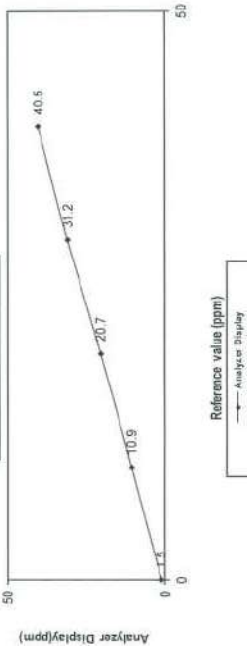

Airgas Specialty Gases  
Airgas USA, LLC  
6144 Easton Road  
Bldg 1  
Plumsteadville, PA 18949  
airgas.com

CERTIFICATE OF ANALYSIS  
Grade of Product: EPA Protocol

Part Number: EQ4HID0E15A01CC  
Cylinder Number: CC159599  
Laboratory: 124 - Plumsteadville - PA  
PGVP Number: A12019  
Gas Code: CO, NO, NO<sub>2</sub>, SO<sub>2</sub>, BALN  
References Number: 160-401528192-1  
Cylinder Volume: 144.4 CF  
Cylinder Pressure: 2015 PSIG  
Valve Outlet: 660  
Certification Date: Jul 30, 2019  
Expiration Date: Jul 30, 2022

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/031, using the assay procedure listed. Analytical Methodology does not require correction for analytical interference. The use of PPM calibration mixture. All concentrations are on a volumetric basis with a confidence level of 95%. These are not to be used for any other purpose. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	44.75 PPM	G1	+/- 0.8% NIST Traceable	07/23/2019, 07/30/2019
NITRIC OXIDE	45.00 PPM	44.75 PPM	G1	+/- 0.8% NIST Traceable	07/23/2019, 07/30/2019
SULFUR DIOXIDE	45.00 PPM	45.35 PPM	G1	+/- 1% NIST Traceable	07/23/2019, 07/30/2019
CARBON MONOXIDE	1000 PPM	1007 PPM	G1	+/- 0.4% NIST Traceable	07/23/2019
NITROGEN	Balance				
CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	18066121	KAL004215	249.9 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Nov 08, 2023
NTRM	052411	KAL004307	50.03 PPM NITRIC OXIDE/NITROGEN	+/- 0.80%	Mar 12, 2024
NTRM	18066121	KAL004215	250.0 PPM NOx/NITROGEN	+/- 0.4%	Nov 08, 2023
NTRM	052411	KAL004307-NOX	30.03 PPM NOx/NITROGEN	+/- 0.80%	Mar 12, 2024
NTRM	0141709	KAL003190	49.67 PPM SULFUR DIOXIDE/NITROGEN	+/- 1.0%	Jun 20, 2022
NTRM	072596	KAL004670	870.0 PPM CARBON MONOXIDE/NITROGEN	+/- 0.4%	May 14, 2021
ANALYTICAL EQUIPMENT					
Instrument/Make/Model			Analytical Principle		
CO MKS FTR 00925062			FTR		
NO MKS FTR 00925062			FTR		
NO MKS FTR 00925062			FTR		
SO2 MKS FTR 00925062			FTR		
Last Multipoint Calibration					
			Jul 19, 2019		
			Jul 22, 2019		
			Jul 22, 2019		
			Jul 22, 2019		

Triad Data Available Upon Request

NOTES: RAN# 51319-CM03

PO# 521902210

GROSS WEIGHT: 28.6 KG

NET WEIGHT: 4.1 KG



Signature on file

Approved for Release



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## Calibration Certificate



Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue : 16 August, 2021

Certification No. 38571

Page : 1 of 7

Object : เครื่องมือวัดความเร็วลมทิศทาง

Manufacturer : LSI

Type : Data Logger E-LOG 305 wind speed and wind direction DNA 827

Thermohygrometers DMA875 Barometer DQA 801

Mfg Code : Data Logger 19040308 wind speed and wind direction 19020211

Thermohygrometers 19010167 Barometer 19040219

Customer : United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsak 41, Sukhumvit Road,

Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1011.2 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: Istdo, Istdo 645 Serial No. 02848057 : Thermoschneider No.918802

STANDARD BAROMETER

: Digital Barometer Vaisala Type PTB330 No. 14320015

Barometer Vaisala Type PTB330 No. 14320011

(Authorised Signatory)

เอกสารไมควบคุม

Sub-Standard Instrument

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration & Test Section

Mr. Wacharapol Subwat

Mechanical Engineer

เอกสารไมควบคุม

Calibration &amp

## Certificate of Calibration

**Customer**  
 Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.LTD.  
 Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
 Prakanong Bangkok 10260

**Unit Under Calibration Details**  
 Measurement item : Acoustic Calibrator  
 Manufacturer : LARSON DAVIS  
 Model : CAL150  
 Serial Number : 6171  
 ID : UAE.EFM.1172562

**Calibration Environment and Details**  
 Temperature : ( 23 ± 2 °C )  
 Humidity : ( 50 ± 20 %RH )  
 Barometric Pressure : ( 1013 ± 10.0 hPa )  
 Received Date : 22 July 2021  
 Calibration Date : 24 August 2021  
 Location of Calibration : LAB 1 Acoustic  
 Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEL	14 May 2022
THD Multimeter	2015	1047765	NIMT	21 January 2022

**Traceability** : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By :

Signature  
 Service Calibration Engineer

Approved By :

Signature  
 Service Calibration Engineer

Issue Date : 24 August 2021

Certificate No : 21-ACT-327

Request No : Req-2021-0995

Calibration Results : Without Adjustment

Sound pressure level Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty ( ± dB )	Acceptance limit Class 2 ( ± dB )
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	94.10	0.10	-	-	0.12	0.40
114 dB / 1000 Hz	114.12	0.12	-	-	0.11	0.40

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( ± % )	Acceptance limit Class 2 ( ± % )
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.10	1.7
114 dB / 1000 Hz	1000.00	0.00	-	-	0.10	1.7

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( ± % )	Acceptance limit Class 2 ( ± % )
	Measured (%)	Error (%)	Measured (%)	Error (%)		
94 dB / 1000 Hz	0.04	-	-	-	0.40	3.0
114 dB / 1000 Hz	0.21	-	-	-	0.40	3.0

### Note :

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration



NSC-TS1-17025  
CALIBRATION 0394

Cert. No. : ACL22081  
Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** LARSON DAVIS  
**Model :** LxT2/ Microphone 375B02 / Preamplifier PRML x T2B  
**Serial No.:** 0005286 / 011740 / 056087  
**ID No.:** -

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0 ± 3 ) °C  
**Pressure :** ( 101.3 ± 3 ) kPa  
**Relative Humidity :** ( 50.0 ± 20 ) %

**Received Date :** 18 JANUARY 2022  
**Calibration Date :** 26 JANUARY 2022  
**Date of Issue :** 28 JANUARY 2022

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 2 of 8

**Calibration Procedure :** CP-AC-02

### Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL-BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL-BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.  
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).



Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

เอกสารไม่ควบคุม

7. Rth.

Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 4 of 8

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal (dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	94.0	0.0	±0.3

**2. Self-generated noise**

**2.1 Normal test**

Measured Value ( dB )
31.0

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	30.8
C - weight	30.6
Flat	36.8

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	-0.1	0.1	0.0
1000	-0.2	-0.2	-0.2
8000	3.1	3.2	3.2
			Acceptance Limits
			± 1.5
			± 1.0
			±5.0

เอกสารไม่ควบคุม

7. Rth.

Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
63	0.0	0.0	±2.0
125	0.0	0.0	±1.5
250	0.0	0.0	±1.5
500	0.0	0.0	±1.5
1000	0.0	0.0	±1.0
2000	0.0	0.1	±2.0
4000	0.0	0.0	±3.0
8000	0.0	0.0	±5.0
16000	-0.1	0.0	±5.0(+∞)

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	±0.2
Flat	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	±0.1
Leq	94.0	0.0	±0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	±0.3

Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.1	0.1	± 1.1
132.0	132.1	0.1	± 1.1
131.0	131.1	0.1	± 1.1
129.0	129.1	0.1	± 1.1
124.0	124.1	0.1	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.1	0.1	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.1	0.1	± 1.1
44.0	44.2	0.2	± 1.1
39.0	39.6	0.6	± 1.1



Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
140	94.0	94.0	0.0	±0.5

9. Tone burst response

Time Weighting	Tone burst duration, Th ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.8	-0.2	1.5 ; -5.0
	2	8	117.0	116.7	-0.3	1.0 ; -2.5
	200	800	134.0	133.9	-0.1	±1.0
Slow	2	8	108.0	107.8	-0.2	1.5 ; -5.0
	200	800	127.6	127.5	-0.1	±1.0
	0.25	1	N/A	N/A	N/A	1.5 ; -5.0
SEL	2	8	N/A	N/A	N/A	1.0 ; -2.5
	200	800	N/A	N/A	N/A	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	135.7	-0.7	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

เอกสารไม่ควบคุม

Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 8 of 8

11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle	0.2	±1.5
89.2	89.4		

12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
Address : 81 Soi Udommak 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260  
Certificate No : 22-ACT-034  
Request No : Req-2022-0092

### Unit Under Calibration Details

Measurement item : Sound Level Meter  
Manufacturer : LARSON DAVIS  
Model : LxT2  
Serial Number : 0005394  
ID : UAE.FRM.031/2564  
Resolution : 0.1 dB  
Microphone Class : 2  
Microphone Model : 375A04  
Microphone SN : 329361  
Preamplifier Model : PEMLxT2C  
Preamplifier SN : 073810  
Instrument Status : Used

### Calibration Environment and Details

Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 14 January 2022  
Calibrated Date : 21 January 2022  
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests  
Location of Calibration : Lab Acoustic

### Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188271	15 September 2022	GRAS
Multi-frequency Calibrator	Quest	Quest-cal	EFA000234	14 June 2022	TSI
Audio Generator	Svank	Svan401	131	18 October 2022	W.K. Electric

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :

Approved By :

Calibration Engineer Supervisor

Issue Date : 21 January 2022

Certificate No : 22-ACT-034  
Request No : Req-2022-0092

### 1. Indication at the calibration check frequency

UUC Setting	Nominal Level (dB)	Before Adjust		Adjust		Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)	
FAST / A / 37-139						
Calibrator Setting						
1000 Hz (14.00 dB)	113.85	113.9	+0.05	113.9	0.05	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTER, Model SV 35A, SN.58079

### 2. Self-generated noise, Microphone installed

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	27.8	0.10

### 3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	27.5	0.10
C	27.0	0.10
Z	31.8	0.10

### 4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency weighting Response curve			Acceptance Limit (± dB)
	A (dB)	C (dB)	Z (dB)	
FAST / 37-139				
STD Setting				
125 Hz	0.0	0.1	0.0	0.50
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	0.2	0.3	0.2	0.60
8000 Hz	-0.3	-0.3	-0.3	0.70

Certificate No : 22-ACT-034  
Request No : Req-2022-0092

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency				UNCERTAINTY ( ± dB)	Acceptance Limits ( ± dB)
	Weighting Response curve					
FAST / 37-130	A (dB)	C (dB)	Z (dB)			
STD Setting						
63 Hz	-0.2	-0.1	0.0			2.0
125 Hz	-0.1	0.0	0.0			1.5
250 Hz	-0.1	0.0	0.0			1.5
500 Hz	-0.1	0.0	0.0			1.5
1000 Hz	0.0	0.0	0.0		0.2	1.0
2000 Hz	0.0	0.0	0.0			2.0
4000 Hz	0.0	0.0	0.0			3.0
8000 Hz	-0.1	-0.1	0.0			5
16000 Hz	-0.1	-0.1	-0.1			+5,-INF.

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		Acceptance Limit ( $\pm$ dB)
		REF (dB)	ERR (dB)	
FAST / 37-139				
UUC Weighting				
A	114.00	114.0	0.0	0.2
C	114.00	114.0	0.0	0.2
Z	114.00	114.0	0.0	0.2
UUC Setting	STD	Measured		Acceptance Limit ( $\pm$ dB)
37-139 / A	REF (dB)	UUC (dB)	ERR (dB)	
UUC Time Response				
Fast	114.00	114.0	0.0	0.1
Slow	114.00	114.0	0.0	0.1
Leq	114.00	114.0	0.0	0.1

Certificate No : 22-ACT-034  
Request No : Req-2022-0092

7. Long Term Stability

UUC Setting	Measured		Acceptance Limit ( $\pm$ dB)
	FAST / A / 37-139	UUC (dB)	
STD Setting			
Initial		114.0	
Final		114.0	
Deviated		0.0	0.1
			0.3

8. Level linearity on the reference level range

UUC Setting	FAST / A / 37-139	STD dB	Anticipated		Deviation		Acceptance Limit ( $\pm$ dB)
			REF (dB)	ERR (dB)	UUC (dB)	ERR (dB)	
139.00			139		139.0	0.0	1.1
134.00			134		134.0	0.0	1.1
129.00			129		129.0	0.0	1.1
124.00			124		124.0	0.0	1.1
119.00			119		119.0	0.0	1.1
114.00			114		114.0	0.0	1.1
109.00			109		109.0	0.0	1.1
104.00			104		104.0	0.0	1.1
99.00			99		99.0	0.0	1.1
94.00			94		93.9	-0.1	1.1
89.00			89		88.9	-0.1	1.1
84.00			84		83.9	-0.1	1.1
79.00			79		78.9	-0.1	1.1
74.00			74		73.9	-0.1	1.1
69.00			69		69.0	0.0	1.1
64.00			64		63.9	-0.1	1.1
59.00			59		59.0	0.0	1.1
54.00			54		54.0	0.0	1.1
49.00			49		49.0	0.0	0.8
44.00			44		44.1	0.1	1.1
39.00			39		39.3	0.3	1.1
34.00			34		34.3	0.3	1.1
37.00			37		37.5	0.5	1.1



Certificate No : 22-ACT-034  
Request No : Req-2022-0092

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
		UUC (dB)	ERR (dB)		
FAST / A	REF (dB)				
UUC Range					
37-139	114	42.8	43.0	0.2	1.1
		114.0	0.0	0.3	1.1

10. Tone burst response

UUC Setting	STD	Anticipated Toneburst (ms)	Measured		UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
			Ref (dB)	UUC (dB)	ERR (dB)	
A / 37-139						
UUC Time Response						
Fast	200	135.0	135.0	0.0		1
	2	118.6	117.7	-0.3		+1.0, -2.5
	0.25	109.0	108.8	-0.2		+1.5, -5.0
Slow	200	128.6	128.5	-0.1		1
	2	109.0	108.9	-0.1		+1.0, -5.0
SEL	200	129.0	129.0	0.0		1
	2	109.0	109.1	+0.1		+1.0, -2.5
	0.25	100.0	100.0	0.0		+1.5, -5.0

11. Peak C sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
		UUC (dB)	ERR (dB)		
FAST / C / 95-142	REF (dB)				
STD Setting					
Complete cycle	137.4	136.8	-0.60		3.0
Positive half cycle	136.4	136.1	-0.30	0.2	2.0
Negative half cycle	136.4	136.2	-0.20		2.0

Certificate No : 22-ACT-034  
Request No : Req-2022-0092

12. Overload indication

UUC Setting	Measured UUC (dB)	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
FAST / A / 37-139			
STD Setting			
Positive one-half cycle	141.7		
Negative one-half cycle	141.8		
Deviated	-0.1	0.2	1.5

13. High Level Stability

UUC Setting	Measured UUC (dB)	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
FAST / A / 37-139			
STD Setting			
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate



## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** LARSON DAVIS  
**Model :** LxT2/ Microphone 375B02 / Preamplifier PRML x T2B  
**Serial No.:** 0005286 / 011740 / 056087  
**ID No.:** -

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0 ± 3 ) °C  
**Pressure :** ( 101.3 ± 3 ) kPa  
**Relative Humidity :** ( 50.0 ± 20 ) %

**Received Date :** 18 JANUARY 2022  
**Calibration Date :** 26 JANUARY 2022  
**Date of Issue :** 28 JANUARY 2022

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

**Calibration Procedure :** CP-AC-02

### Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL-BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL-BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.  
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

เอกสารไม่ควบคุม

Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value ( dB )
31.0

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	30.8
C - weight	30.6
Flat	36.8

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	-0.1	0.1	0.0
1000	-0.2	-0.2	-0.2
8000	3.1	3.2	3.2
			Acceptance Limits
			± 1.5
			± 1.0
			±5.0

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
63	0.0	0.0	±2.0
125	0.0	0.0	±1.5
250	0.0	0.0	±1.5
500	0.0	0.0	±1.5
1000	0.0	0.0	±1.0
2000	0.0	0.1	±2.0
4000	0.0	0.0	±3.0
8000	0.0	0.0	±5.0
16000	-0.1	0.0	±5.0(+∞)

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	±0.2
Flat	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	±0.1
Leq	94.0	0.0	±0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	±0.3

เอกสารไม่ควบคุม

Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.1	0.1	± 1.1
132.0	132.1	0.1	± 1.1
131.0	131.1	0.1	± 1.1
129.0	129.1	0.1	± 1.1
124.0	124.1	0.1	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.1	0.1	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.1	0.1	± 1.1
44.0	44.2	0.2	± 1.1
39.0	39.6	0.6	± 1.1

เอกสารไม่ควบคุม

Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
140	94.0	94.0	0.0	±0.5

9. Tone burst response

Time Weighting	Tone burst duration, Th ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.8	-0.2	1.5 ; -5.0
	2	8	117.0	116.7	-0.3	1.0 ; -2.5
	200	800	134.0	133.9	-0.1	±1.0
Slow	2	8	108.0	107.8	-0.2	1.5 ; -5.0
	200	800	127.6	127.5	-0.1	±1.0
	0.25	1	N/A	N/A	N/A	1.5 ; -5.0
SEL	2	8	N/A	N/A	N/A	1.0 ; -2.5
	200	800	N/A	N/A	N/A	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	135.7	-0.7	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22081  
Job No. : VC65AC0044  
Pages : 8 of 8

11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle	0.2	±1.5
89.2	89.4		

12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate



## Certificate of Calibration

**Customer**  
Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD  
Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangkok, Bangkok  
10260

Certificate No : 22-ACT-104  
Request No : Req-2022-0232

### Unit Under Calibration Details

Measurement item : Sound Level Meter  
Manufacturer : LARSON DAVIS  
Model : LxT  
Serial Number : 0006614  
ID : UAE.EFM.045/2564  
Resolution : 0.1 dB  
Microphone Class : 2  
Microphone Model : 375A04  
Microphone SN : 329353  
Preamplifier Model : PRMLxT2C  
Preamplifier SN : 071534  
Instrument Status : Used

### Calibration Environment and Details

Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 31 January 2022  
Calibrated Date : 11 February 2022  
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests  
Location of Calibration : Lab Acoustic

### Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188271	15 September 2022	GRAS
Multi-frequency Calibrator	Quest	Quest-cal	EFA000234	14 June 2022	TSI
Audio Generator	Svanick	Svan401	131	18 October 2022	W.K Electric

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :

[Signature]

Approved By :

[Signature]

Supervisor

Issue Date : 11 February 2022

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd  
PM-SLM-01 Rev.0 Issue date 01/07/16

เอกสารไม่ควบคุม

Certificate No : 22-ACT-104  
Request No : Req-2022-0232

### 1. Indication at the calibration check frequency

UUC Setting	Nominal Level (dB)	Before Adjust UUC (dB)	Before Adjust ERR (dB)	Adjust UUC (dB)	Adjust ERR (dB)	UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139							
Calibrator Setting 1000 Hz 114.00 dB	113.85	114.0	+0.15	113.9	0.05	0.20	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN:58079

### 2. Self-generated noise, Microphone installed

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting A	28.7	0.10

### 3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting A	28.6	0.10
C	28.8	0.10
Z	34.7	0.10

### 4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve	UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / 37-139	A C Z	(dB) (dB) (dB)	(± dB)
STD Setting 125 Hz	0.0 0.1 0.1	0.50	2.0
1000 Hz	0.0 0.0 0.0	0.60	1.0
4000 Hz	0.7 0.7 0.7	0.60	3.0
8000 Hz	1.0 0.9 0.8	0.70	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd  
PM-SLM-01 Rev.0 Issue date 01/07/16

เอกสารไม่ควบคุม

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency				UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
	A (dB)	C' (dB)	Z (dB)			
FAST / 37-139						
STD Setting						
63 Hz	-0.2	0.0	0.0			2.0
125 Hz	-0.1	0.0	0.0			1.5
250 Hz	-0.1	0.0	0.0			1.5
500 Hz	-0.1	0.0	0.0			1.5
1000 Hz	0.0	0.0	0.0	0.2		1.0
2000 Hz	0.0	0.1	0.0			2.0
4000 Hz	0.0	0.0	0.0			3.0
8000 Hz	0.0	0.0	0.0			5.0
10000 Hz	-0.1	-0.1	-0.1			+5, -INF.

## 6. Frequency and time weightings at 1kHz

UUC Setting	STD REF (dB)	Measured		UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
		UUC (dB)	ERR (dB)		
FAST / 37-139					
UUC Weighting					
A	114.00	114.0	0.0		0.2
C	114.00	114.0	0.0	0.2	0.2
Z	114.00	114.0	0.0		0.2

UUC Setting	STD REF (dB)	Measured		UNCERTAINTY (+/- dB)	Acceptance Limit (+/- dB)
		UUC (dB)	ERR (dB)		
37-139 / A					
UUC Time Response					
Fast	114.00	114.0	0.0		0.1
Slow	114.00	114.0	0.0	0.2	0.1
Loss	114.00	114.0	0.0		0.1

The results related only to the items calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

# เอกสารไม่ควบคุม

## 7. Long Term Stability

UUC Setting	Measured		UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
	FAST / A / 37/139	UUC (dB)		
STD Setting	Initial	114.0	0.1	0.3
	Final	114.0		
	Deviated	0.0		

## 8. Level linearity on the reference level range

UUC Setting			Anticipated	Deviation		UNCERTAINTY ( ± dB)	Acceptance Limit ( ± dB)
FAST / A / 37/139		REF (dB)		U/C (dB)	ERR (dB)		
STD dB							
140.00		140	140	140.0	0.0		1.1
139.00		139	139	139.0	0.0		1.1
134.00		134	134	134.0	0.0		1.1
129.00		129	129	129.0	0.0		1.1
124.00		124	124	124.0	0.0		1.1
119.00		119	119	119.0	0.0		1.1
114.00		114	114	114.0	0.0		1.1
109.00		109	109	109.0	0.0		1.1
104.00		104	104	104.0	0.0		1.1
99.00		99	99	99.0	0.0		1.1
94.00		94	94	94.0	0.0	0.3	1.1
89.00		89	89	89.0	0.0		1.1
84.00		84	84	84.0	0.0		1.1
79.00		79	79	79.0	0.0		1.1
74.00		74	74	74.0	0.0		1.1
69.00		69	69	69.0	0.0		1.1
64.00		64	64	64.0	0.0		1.1
59.00		59	59	59.0	0.0		1.1
54.00		54	54	54.0	0.0		1.1
49.00		49	49	49.0	0.0		1.1
44.00		44	44	44.1	0.1		1.1
39.00		39	39	39.3	0.3		1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

PM-708-SLM-01 Rev. 0 Issue date 01/07/16

# เอกสารไม่ควบคุม

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 37+139	UUC (dB)	(± dB)	(± dB)
STD Setting			
Positive one half cycle	142.7		
Negative one-half cycle	142.6		
Deviated	0.1	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 37+139	UUC (dB)	(± dB)	(± dB)
STD Setting			
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

เอกสารไม่ควบคุม

9. Level linearity including the level range control

UUC Setting	STD	Measured	UNCERTAINTY	Acceptance Limit
FAST / A	REF (dB)	UUC (dB)	(± dB)	(± dB)
UUC Range		ERR (dB)		
	44.1	-0.4		1.1
37-139	114	114.0	0.3	1.1

10. Tone burst response

UUC Setting	STD	Anticipated	Measured	UNCERTAINTY	Acceptance Limit
A / 37-139	Toneburst (ms)	Ref (dB)	UUC (dB)	(± dB)	(± dB)
UUC Time Response			ERR (dB)		
Fast	200	135.0	135.0	0.0	1.0
	2	118.0	117.9	-0.1	+1.0, -2.5
	0.25	109.0	108.7	-0.3	+1.5, -5.0
Slow	200	128.6	128.5	-0.1	1.0
	2	109.0	108.8	-0.2	+1.0, -5.0
	200	129.0	129.0	0.0	1.0
SEL	2	109.0	109.1	+0.1	+1.0, -2.5
	0.25	100.0	99.7	-0.3	+1.5, -5.0

11. Peak C Sound level

UUC Setting	Anticipated	Measured	UNCERTAINTY	Acceptance Limit
FAST / C / 95-142	REF (dB)	UUC (dB)	(± dB)	(± dB)
STD Setting		ERR (dB)		
Complete cycle	137.4	136.7	-0.70	3.0
Positive half cycle	136.4	136.2	-0.20	2.0
Negative half cycle	136.4	136.2	-0.20	2.0

เอกสารไม่ควบคุม



## Certificate of Calibration

**Customer**  
Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
Address : 81 Soi Udonasuk 41, Sukhumvit Road, Bangkok, Prakanong, Bangkok 10260

Certificate No : 22-ACT-105  
Request No : Req-2022-0229

### Unit Under Calibration Details

Measurement item : Sound Level Meter  
Manufacturer : LARSON DAVIS  
Model : LxT2  
Serial Number : 0005396  
ID : UAE.EFM.033/2564  
Resolution : 0.1 dB

Microphone Class : 2  
Microphone Model : 375A04  
Microphone SN : 329350  
Preamplifier Model : PRMLxT2C  
Preamplifier SN : 073812  
Instrument Status : Used

### Calibration Environment and Details

Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 31 January 2022  
Calibrated Date : 11 February 2022  
Calibration Procedure : In-house method (P-SLM-01) based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests  
Location of Calibration : Lab Acoustic

### Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188271	15 September 2022	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	14 June 2022	TSI
Audio Generator	Svaneck	Svan401	131	18 October 2022	W.K Electric

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :

  
Calibration Officer

Approved By :

  
Calibration Engineer Supervisor

Issue Date :

11 February 2022

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

PM-700-SLM-01 Rev.0 Issue date 01/07/16

เอกสารไม่ควบคุม

### 1. Indication at the calibration check frequency

UUC Setting	Nominal Level (dB)	Before Adjust		Adjust		Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)	
FAST / A / 37-139						
Calibrator Setting						
1000 Hz 114.00 dB	113.85	113.9	+0.05	113.9	0.05	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN:58079

### 2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting		
A	27.8	(± dB) 0.10

### 3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting		
A	27.8	(± dB) 0.10
C	27.3	0.10
Z	33.1	0.10

### 4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve				Acceptance Limit (± dB)
	A (dB)	C (dB)	Z (dB)	UNCERTAINTY (± dB)	
FAST / 37-139					
STD Setting					
125 Hz	0.1	0.1	0.2	0.50	2.0
1000 Hz	0.0	0.0	0.0	0.60	1.0
4000 Hz	0.6	0.5	0.6	0.60	3.0
8000 Hz	0.1	0.0	0.2	0.70	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

PM-700-SLM-01 Rev.0 Issue date 01/07/16

เอกสารไม่ควบคุม









TECHNOLOGICAL PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES  
5343 PATTANAKARN ROAD KVI 15, SATHUANG SIANGSIANG, BANGKOK 10250

TEL: 0-2710-3000-2 FAX: 02-19-4846



NTL-TB-17617025  
CALIBRATION 1000

Cert.No.: 21CH1607  
Page: 1 of 3

## Certificate of Calibration

Equipment : pH Meter  
Manufacturer : Horiba  
Model : LAQUA-PH-210  
Serial No. : HA1F0002  
ID No. : UAE EFM 200/2564(EFM pH 08164)  
Condition As-Received: Used Item  
Received Date : 18 November 2021  
Calibration Date : 19 November 2021  
Reference : 2111-0736WSC-1  
Submitted by : United Analyst and Engineering Consultant Co., Ltd.  
3 Soi Udonasuk 41, Sukhumvit Road  
Bangkok, Phrakhanong, Bangkok 10260  
(25 ± 2.5) °C  
(50 ± 15) %  
In - house method  
Calibration Procedure :  
- CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)  
- CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lertgagrakul

Approved by :

( ) Malee Bulkruea  
( ) Saithip Meangmai  
( ) Warakorn Lertgagrakul

Issue Date : 25 November 2021

The Uncertainties are for a confidence probability of approximately 95 %

This certificate may not be reproduced fully or in part without the prior written

Approval of the head of Corporate Services 3 - Treatment, Calibration and Training Services

เอกสารไม่ควบคุม



Cert.No.: 21CH1607  
Page: 2 of 3

### Condition of this calibration result

1. Reference Standard Instrument :  
Instrument :  
Serial No. : 54030049 ID No. : 130RC116 Cert. No. : 21E2682 Due Date : 25 Aug 2022  
2) Ref. Standard Thermometer : 4962054 ID No. : 110RC044 Cert. No. : 2111201 Due Date : 26 Oct 2022  
This certifier is traceable to the International System of Unit maintained at:  
- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials :  
The measurement results are traceable to SI through CPA chem Ltd.  
ANSI-ASQ National Accreditation Board Accredited No. AR-1835

Buffer Solution :  
pH 4.008  
pH 6.982  
pH 10.015  
Manufacturer : CPA chem  
Lot No. : 761016  
761017  
761018  
Exp. date : 02 Aug 2023  
02 Aug 2022  
02 Aug 2022

3. This certificate is valid only to the item calibrated on date and place of calibration.

### Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4.7, 7, 10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( mV )	Coverage factor k
			mV	pH		
pH Meter SN: HA1F0002	4.00	177.48	177.4	4.01	0.058	2.00
	7.00	0.00	-0.2	7.02	0.058	2.00
	10.00	-177.48	-177.6	10.01	0.058	2.00

เอกสารไม่ควบคุม



Cert.No.: 21CH1807  
Page: 3 of 3

#### Calibration Results

##### Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4.7, 7.10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor k
pH Electrode S/N: 991E0471	4.008	4.01	172	0.0071	2.00
	6.982	6.98	-4	0.011	2.00
	6.982	6.98	-4	0.011	2.00
	10.015	10.01	-181	0.011	2.05

##### Function : Temperature Measurement

(\*) Without adjustment

This equipment was connected with Temperature Probe,

- Probe : 9652
- Serial No. : 991E0471
- Dimension of probe:
  - Length : 103 mm.
  - Diameter : 16 mm.
  - Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
25.0	25.002	25.0	-0.002	0.13	2.00
30.0	30.004	30.0	-0.004	0.13	2.00
35.0	35.003	35.0	-0.003	0.13	2.00

Remark : - UUC\* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-oüo-

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB  
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE  
719 MOO 13, SOI SUTSAKORN 11 TAMBON BANG KAEU,  
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND  
TEL: (06) 921 10 2800-1 FAX: (06) 921 10 7140



ANAB  
ASSOCIATION OF NATIONAL ACCREDITATION BODIES  
ACCREDITED  
CALIBRATION LABORATORY  
No. 21CH1807

Page 1 of 2

#### Certificate of Calibration

##### Customer

Name : UNITED ANALYST AND ENGINEERING  
Address : CONSULTANT CO., LTD.  
: 81 Soi Udomsak 41, Sukhumvit Road, Bangchak, Prakanong,  
Bangkok 10260

Certificate No : 21-ACT-187

Request No : Req-2021-0523

##### Unit Under Calibration Details

Measurement item : Acoustic Calibrator  
Manufacturer : SVANTEK  
Model : SV 35A  
Serial Number : 73249  
ID : UAE.EFM.105/2561  
Class : I  
Range : 94, 114 dB / 100 Hz  
Instrument Status : Used

##### Calibration Environment and Details

Temperature : (23 ± 2 °C)  
Humidity : (50 ± 20 %RH)  
Barometric Pressure : (1013 ± 10.0 hPa)  
Received Date : 27 April 2021  
Calibration Date : 28 May 2021  
Location of Calibration : LAB 1 Acoustic  
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEL	14 May 2022
THD Multimeter	2015	1047765	NIMT	22 January 2022

**Traceability** : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

##### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By :

Mr. Pichat Muthavorn  
Service Calibration Engineer

Approved By :

Mr. Pichat Muthavorn  
Calibration Engineer Supervisor

Issue Date : 28 May 2021

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the issuing body.  
ANAB-ACCREDITED CALIBRATION LABORATORY No. 21CH1807

เอกสารไม่ควบคุม



## Certificate of Calibration

**Customer**  
Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangkok, Prakanung, Bangkok 10260  
Certificate No : 25-ACT-067  
Request No : Req-2022-0223

### Unit Under Calibration Details

Measurement Item : Sound Level Meter  
Manufacturer : RION  
Model : NL-42  
Serial Number : 00499059  
ID : UAE.EFM.0122564  
Resolution : 0.1 dB  
Microphone Class : 2  
Microphone Model : UC-52  
Microphone SN : 189887  
Preampifier Model : NH24  
Preampifier SN : 90495  
Instrument Status : Used

### Calibration Environment and Details

Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 31 January 2022  
Calibrated Date : 3 February 2022  
Calibration Procedure : In-house method CIP-SL M-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic testing

### Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	15 September 2022	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000214	14 Jun 2022	TSI
Audio Generator	Svantek	Svan401	131	18 October 2022	WK Electric

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :

Mr. Noppadol Luangrat  
Calibration Officer

Approved By :

Mr. Patch Mathayavan  
Calibration Engineer Supervisor  
Issue Date : 3 February 2022

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-7187-SL-J4-01 Rev.0 Issue date 01/07/11

เอกสารไม่ควบคุม

Certificate No : 21-ACT-187

Request No : Req-2021-0523

### Calibration Results : Without Adjustment

### Sound pressure level

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	93.81	-0.19	-	-	0.11	0.25
114 dB / 1000 Hz	113.83	-0.17	-	-	0.11	0.25

### Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	999.97	0.003	-	-	0.02	0.70
114 dB / 1000 Hz	999.98	0.002	-	-	0.02	0.70

### Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)
	Measured (%)	Error (%)	Measured (%)	Error (%)		
94 dB / 1000 Hz	0.18	-	-	-	0.17	2.5
114 dB / 1000 Hz	0.04	-	-	-	0.17	2.5

### Note :

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration

เอกสารไม่ควบคุม

1. Indication at the calibration check frequency

UUC Setting	Nominal		Before Adjust		Adjust		Acceptance Limit (± dB)
	FAST / 25 - 138	Level (dB)	UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)	
Calibrator Setting							
1000 Hz 114.00 dB		93.95	93.9	-0.05	93.9	-0.05	0.3

Note: Absolute sensitivity was established by the use of Sound Calibrator Brand Svanick, Model SV 35A, SN: 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 25 - 138		
UUC Weighting		
A	14.3	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 25 - 138		
UUC Weighting		
A	11.3	0.10
C	16.7	0.10
Z	22.8	0.10

4. Acoustic signal test of frequency weightings: (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve				Acceptance Limit (± dB)
	A	C	Z	UNCERTAINTY (± dB)	
FAST / 25 - 138					
STD Setting					
125 Hz	0.2	0.4	0.3	0.50	1.5
1000 Hz	0.0	0.0	0.0	0.60	1.0
4000 Hz	-0.5	-0.5	-0.5	0.60	3.0
8000 Hz	-2.5	-2.4	-1.5	0.70	5.0

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve				UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	A (dB)	C (dB)	Z (dB)	ERR (dB)		
FAST / 25 - 138						
STD Setting						
63 Hz	-0.2	-0.1	-0.1	-0.1		2.0
125 Hz	-0.1	0.0	0.0	0.0		1.5
250 Hz	-0.1	0.0	0.0	0.0		1.5
500 Hz	0.0	0.1	0.0	0.0		1.5
1000 Hz	0.0	0.0	0.0	0.0	0.2	1.0
2000 Hz	0.0	0.1	0.0	0.0		2.0
4000 Hz	0.0	0.0	0.0	0.0		3.0
8000 Hz	0.1	0.1	0.0	0.0		5
16000 Hz	-1.3	-1.3	-1.3	0.0		+5, -INF.

6. Frequency and time weightings at 1kHz

UUC Setting	STD REF	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)		
FAST / 25 - 138					
UUC Weighting					
A	94.00	94.0	0.0		0.2
C	94.00	94.0	0.0	0.2	0.2
Z	94.00	94.0	0.0		0.2

UUC Setting	STD REF	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)		
25 - 138 / A					
UUC Time Response					
Fast	94.00	94.0	0.0		0.1
Slow	94.00	94.0	0.0		0.1
Leq	94.00	94.0	0.0	0.2	0.1

Certificate No : 22-ACT-067  
Request No : Req-2022-0223

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 25 - 138	UUC (dB)	( $\pm$ dB)	( $\pm$ dB)
STD Setting			
Initial	94.0		
Final	94.0		
Deviated	0.0	0.1	0.3

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation	UNCERTAINTY	Acceptance Limit
FAST / A / 25 - 138	REF (dB)	UUC (dB) ERR (dB)	( $\pm$ dB)	( $\pm$ dB)
STD dB				
137.00	137	137.0 0.0		0.8
136.00	136	136.0 0.0		0.8
135.00	135	135.0 0.0		1.1
134.00	134	134.0 0.0		1.1
129.00	129	129.0 0.0		1.1
124.00	124	124.0 0.0		1.1
119.00	119	119.0 0.0		1.1
114.00	114	114.0 0.0		1.1
109.00	109	109.0 0.0		1.1
104.00	104	104.0 0.0		1.1
99.00	99	99.0 0.0		1.1
94.00	94	94.0 0.0		1.1
89.00	89	89.0 0.0		1.1
84.00	84	84.0 0.0		1.1
79.00	79	79.0 0.0		1.1
74.00	74	74.0 0.0		1.1
69.00	69	69.0 0.0		1.1
64.00	64	64.0 0.0		1.1
59.00	59	59.0 0.0		1.1
54.00	54	54.0 0.0		1.1
49.00	49	49.0 0.0		1.1
44.00	44	44.0 0.0		1.1
39.00	39	39.0 0.0		1.1
34.00	34	34.0 0.0		1.1
29.00	29	29.0 0.0		1.1
24.00	24	24.0 0.0		1.1
20.00	20	20.0 0.0		1.1
16.00	16	16.0 0.0		1.1
12.00	12	12.0 0.0		1.1
8.00	8	8.0 0.0		1.1
4.00	4	4.0 0.0		1.1
0.00	0	0.0 0.0		1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.  
P/4-738-SL-4-01 Item 0 Issue date 01/07/11

เอกสารไม่ควบคุม

Certificate No : 22-ACT-067  
Request No : Req-2022-0223

9. Level linearity including the level range control

UUC Setting	STD	Measured	UNCERTAINTY	Acceptance Limit
FAST / A	REF (dB)	UUC (dB) ERR (dB)	( $\pm$ dB)	( $\pm$ dB)
UUC Range				
25 - 138	94	94.0 0.0	0.3	1.1

10. Tone burst response

UUC Setting	Anticipated	Measured	UNCERTAINTY	Acceptance Limit
A / 25 - 138	Toneburst (ms)	Ref (dB) UUC (dB) ERR (dB)	( $\pm$ dB)	( $\pm$ dB)
UUC Time Response				
Fast	200	134.0 134.0 0.0		1.0
	2	117.0 117.0 0.0		+1.0, -2.5
	0.25	108.0 107.9 -0.1		+1.5, -5.0
Slow	200	127.6 127.6 0.0		1.0
	2	108.0 108.0 0.0		+1.0, -5.0
	200	128.0 128.0 0.0		1.0
SEL	2	108.0 108.0 0.0		+1.0, -2.5
	0.25	99.0 98.9 -0.1		+1.5, -5.0

11. Peak C Sound level

UUC Setting	Anticipated	Measured	UNCERTAINTY	Acceptance Limit
FAST / C / 25 - 138	REF (dB)	UUC (dB) ERR (dB)	( $\pm$ dB)	( $\pm$ dB)
STD Setting				
Complete cycle	133.4	132.9 -0.50		3.0
Positive half cycle	132.4	132.2 -0.20		2.0
Negative half cycle	132.4	132.2 -0.20		2.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.  
P/4-738-SL-4-01 Item 0 Issue date 01/07/11

เอกสารไม่ควบคุม



Certificate No : 22-ACT-067  
Request No : Req-2022-0223

#### 12. Overload Indication

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 25 - 138	UUC (dB)	( $\pm$ dB)	( $\pm$ dB)
STD Setting			
Positive one-half cycle	139.4		
Negative one-half cycle	139.4		
Deviated	0.0	0.2	1.5

#### 13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 25 - 138	UUC (dB)	( $\pm$ dB)	( $\pm$ dB)
STD Setting			
Initial	137.0		
Final	137.0		
Deviated	0.0	0.1	0.3

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.  
ISO 17025:2017

เอกสารไม่ควบคุม

## SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Srimthom Rd, Bangbunmu, Bangkok 10700 THAILAND  
Tel: 0 2435-8800 Fax: 0 2433 1679 e-mail: cal-center@itiphom.com http://www.itiphom.com



REC-758-TS 27023  
CALIBRATION 0386

Cert. No. : ACL22075  
Pages : 1 of 8

### Calibration Certificate

Equipment : SOUND LEVEL METER  
Manufacturer : RICON  
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24  
Serial No. : 00709682 / 187256 / 01233  
ID No. : -

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (U/AE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHIAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

Location : -  
Ambient Temperature : ( 23.0  $\pm$  3 ) °C  
Pressure : ( 101.3  $\pm$  3 ) kPa  
Relative Humidity : ( 50.0  $\pm$  20 ) %

Received Date : 18 JANUARY 2022  
Calibration Date : 21-25 JANUARY 2022  
Date of Issue : 28 JANUARY 2022

Calibrated by : Nathakorn Phurpaikan

Approved by :

( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-02/0664

เอกสารไม่ควบคุม

## Continuation of Calibration Certificate

Cert. No. : ACL22075  
Job No. : VC65AC0044  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL-BP-05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL-BP-03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-1S180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	29775900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KA1	34560495	AA-3103-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is receivable to the international system of unit maintained at :

1. National Institute of Metrology (Thailand).
2. Thailand Institute of Scientific and Technological Research (TISTR).

## Continuation of Calibration Certificate

Cert. No. : ACL22075  
Job No. : VC65AC0044  
Pages : 3 of 8

## Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long-term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

## Continuation of Calibration Certificate

Cert. No. : ACL22075  
Job No. : VC65AC0044  
Pages : 4 of 8

## Result of calibration :

## 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	93.9	0.0	±0.3

## 2. Self-generated noise

## 2.1 Normal test

Measured Value ( dB )
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	10.8
C - weight	16.7
Flat	22.5

## 3. Acoustical signal tests of frequency weightings

Meter free field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.1	0.1	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	0.8	0.9	0.9	±5.0

## Continuation of Calibration Certificate

Cert. No. : ACL22075  
Job No. : VC65AC0044  
Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

## 5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A-weight	94.0	0.0	-
C-weight	94.0	0.0	±0.2
Flat	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	±0.1
Leq	94.0	0.0	±0.1

## 6. Long-term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A-weight	94.0	94.0	0.0	±0.3



## Continuation of Calibration Certificate

Cert. No. : ACL22075  
Job No. : VC65AC0044  
Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	132.9	-0.1	$\pm 1.1$
132.0	131.9	-0.1	$\pm 1.1$
131.0	130.9	-0.1	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	30.0	0.0	$\pm 1.1$
29.0	29.1	0.1	$\pm 1.1$
28.0	28.1	0.1	$\pm 1.1$
27.0	27.1	0.1	$\pm 1.1$
26.0	26.0	0.0	$\pm 1.1$
25.0	25.1	0.1	$\pm 1.1$

เอกสารไม่ควบคุม

## Continuation of Calibration Certificate

Cert. No. : ACL22075  
Job No. : VC65AC0044  
Pages : 7 of 8

## 8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	$\pm 1.1$

## 9. Tone burst response

Time Weighting	Tone burst duration, T <sub>b</sub> (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 - 5.0
	2	8	117.0	117.0	0.0	1.0 - 2.5
	200	800	134.0	134.0	0.0	$\pm 1.0$
Slow	2	8	108.0	108.0	0.0	1.5 - 5.0
	200	800	127.6	127.6	0.0	$\pm 1.0$
	0.25	1	99.0	98.9	-0.1	1.5 - 5.0
SEL	2	8	108.0	108.0	0.0	1.0 - 2.5
	200	800	128.0	128.0	0.0	$\pm 1.0$

## 10. Peak C' sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L <sub>peak</sub> (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.2	-0.2	$\pm 3.0$

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	$\pm 2.0$
Negative half cycle	135.4	135.1	-0.3	12.0

เอกสารไม่ควบคุม

Cert. No. : ACL22075  
Job No. : VC65AC0044  
Pages : 8 of 8

# 11. Overload indication

Measured value ( dB )	Deviated Value ( dB )		Acceptance Limits ( dB )
	Positive one-half cycle	Negative one-half cycle	
89.5	89.5	0.0	±1.5

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.2

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB  
INNOVATIVE INSTRUMENT CO.,LTD. HEAD OFFICE  
7139 MOO 13, SOI SUTINSAKORN 11 TAMBON BANG KAEO,  
AMPHOE BANG PHEI SAMUT PRAKAN PROVINCE 10540 THAILAND  
TEL: (66)0-116-5869-1 FAX: (66)0-116-7140



## Certificate of Calibration

**Customer**  
Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsak 41, Subhuvit Road, Bangchak, Pratuang, Bangkok  
10260  
Certificate No : 22-ACT-026  
Request No : Req-2022-0095

### Unit Under Calibration Details

Measurement item : Sound Level Meter  
Manufacturer : LARSON DAVIS  
Model : LxT2  
Serial Number : 0005400  
ID : UAL-ETM-0372564  
Resolution : 0.1 dB  
Microphone Class : 2  
Microphone Model : 375A04  
Microphone SN : 328676  
Preamplifier Model : P8MLAT2C  
Preamplifier SN : 073803  
Instrument Status : Used

### Calibration Environment and Details

Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 14 January 2022  
Calibrated Date : 21 January 2022

Calibration Procedure : In-house method (P-SLM-01) based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests  
Location of Calibration : Lab Acoustic

### Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	15 September 2022	GRAS
Multi-frequency Calibrator	Quest	Quest-cal	EFA000234	14 June 2022	TSI
Audio Generator	Svante	Svan401	131	18 October 2022	WK Electric

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :

Mr. Noppadon Luangart  
Calibration Officer

Approved By :

Calibration Engineer Supervisor

Issue Date :

21 January 2022

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the issuing body.  
เอกสารไม่ควบคุม  
Date 01/07/19

Certificate No : 22-ACT-036

Certificate No : 22-ACT-036

Request No : Req-2022-0095

Request No : Req-2022-0095

1. Indication at the calibration check frequency

UUC Setting	Nominal		Before Adjust		Adjust		UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
	FAST / A / 37+39 Calibrator Setting	Level (dB)	UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)		
1000 Hz 114.00 dB		113.85	113.9	-0.05	113.9	0.05	0.1	0.3

Note: Absolute sensitivity was established by the use of Sound Calibrator Brand SV 35A, SN 58079

2. Self-generated noise. Microphone installed

UUC Setting	Measured (dB)	UNCERTAINTY ( $\pm$ dB)
FAST / 37.139		
UUC Weighting		
A	29.0	0.10

3. Self-generated noise: Microphone replaced by the electrical input signal device

UUC Setting	Measured (dB)	UNCERTAINTY ( $\pm$ dB)
FAST /37-139		
UUC Weighting		
A	28.8	0.10
C	28.2	0.10
Z	32.9	0.10

## 4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve				UNCERTAINTY	Acceptance Limit
	Weighting Response curve					
	A (dB)	C (dB)	Z (dB)			
FAST / 37-139						
STD Setting						
125 Hz	-0.1	0.1	0.0		0.50	2.0
1000 Hz	0.0	0.0	0.0		0.60	1.0
4000 Hz	0.5	0.5	0.6		0.60	3.0
8000 Hz	0.4	0.4	0.5		0.70	5.0

The results related only to the item calligraphed. The certificate shall not be reproduced except in full, without written approval of the Library of Congress.

เอกสารไม่ควบคุม

date 01/07/79

# เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the issuing laboratory.

วันที่ 01/07/19

**เอกสารไม่ควบคุม**

Accession 01.007/19



Certificate No : 22-ACT-436  
Request No : Req-2022-0095

#### 7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
FAST / A / 37-139	UUC (dB)		
STD Setting			
Initial	114.0		
Final	114.0		
Deviated	0.0	0.1	0.3

#### 8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
FAST / A / 37-139	REF (dB)	UUC (dB)	ERR (dB)	
STD dB				
139.00	139	139.0	0.0	1.1
134.00	134	134.0	0.0	1.1
129.00	129	129.0	0.0	1.1
124.00	124	124.0	0.0	1.1
119.00	119	119.0	0.0	1.1
114.00	114	114.0	0.0	1.1
109.00	109	109.0	0.0	1.1
104.00	104	104.0	0.0	1.1
99.00	99	99.0	0.0	1.1
94.00	94	93.9	-0.1	1.1
89.00	89	88.9	-0.1	1.1
84.00	84	83.9	-0.1	1.1
79.00	79	78.9	-0.1	1.1
74.00	74	73.9	-0.1	1.1
69.00	69	68.0	0.0	1.1
64.00	64	63.9	-0.1	1.1
59.00	59	59.0	0.0	1.1
54.00	54	54.0	0.0	1.1
49.00	49	49.0	0.0	0.9
44.00	44	44.1	0.1	1.1
39.00	39	39.3	0.3	1.1
34.00	34	34.3	0.3	1.1
37.00	37	37.5	0.5	1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory. Issue date 01/07/19

เอกสารไม่ควบคุม

Certificate No : 22-ACT-086  
Request No : Req-2022-0095

#### 9. Level linearity including the level range control

UUC Setting	STD	Measured	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
FAST / A	REF (dB)	UUC (dB)	ERR (dB)	
UUC Range				
	42.9	43.2	0.3	1.1
37-139	114	114.0	0.0	1.1

#### 10. Tone burst response

UUC Setting	Anticipated	Measured	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
A / 37-139	STD Toneburst (ms)	Ref (dB)	ERR (dB)	
UUC Time Response				
	200	135.0	0.0	1
	2	118.0	-0.2	+1.0, -2.5
	0.25	109.0	-0.2	+1.5, -5.0
Fast				
	200	128.6	-0.1	1
	2	109.0	-0.2	+1.0, -5.0
Slow				
	200	129.0	0.0	1
	2	109.0	0.0	+1.0, -2.5
SEL				
	0.25	100.0	-0.1	+1.5, -5.0

#### 11. Peak C Sound level

UUC Setting	Anticipated	Measured	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
FAST / C / 95-142	REF (dB)	UUC (dB)	ERR (dB)	
STD Setting				
Complete cycle	137.4	136.9	-0.50	3.0
Positive half cycle	136.4	136.2	-0.20	2.0
Negative half cycle	136.4	136.2	-0.20	2.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory. Issue date 01/07/19

เอกสารไม่ควบคุม

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 22-ACT-103  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok Request No : Req-2022-0230  
10260

### Unit Under Calibration Details

Measurement Item : Sound Level Meter Microphone Class : 2  
Manufacturer : LARSON DAVIS Microphone Model : 375A04  
Model : LX72 Microphone SN : 328668  
Serial Number : 0005402 Preampifier Model : FRMLxT2C  
ID : UAEFPM/038/2564 Preampifier SN : 071540  
Resolution : 0.1 dB Intrument Status : Used

### Calibration Environment and Details

Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 31 January 2022  
Calibrated Date : 11 February 2022

Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests

Location of Calibration : Lab Acoustic

### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	15 September 2022	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	14 June 2022	TSI
Audio Generator	Svaneck	Svan401	131	18 October 2022	WK Electric

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :

Mr. [REDACTED] angart

Calibration Officer

Approved By :

Calibration Engineer Supervisor

Issue Date : 11 February 2022

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.0 June due 01/07/19

เอกสารไม่ควบคุม

Certificate No : 22-ACT-036

Request No : Req-2022-0095

### 12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 37-139	UUC		
STD Setting	(dB)	( ± dB)	( ± dB)
Positive one-half cycle	142.1		
Negative one-half cycle	141.9		
Deviated	0.2	0.2	1.5

### 13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 37-139	UUC		
STD Setting	(dB)	( ± dB)	( ± dB)
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.0 June due 01/07/19

เอกสารไม่ควบคุม





Certificate No : 22-ACT-103  
Request No : Req-2022-0239

#### 7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
FAST / A / 37-139	UUC (dB)		
STD Setting			
Initial	114.0		
Final	114.0		
Deviated	0.0	0.1	0.3

#### 8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
FAST / A / 37-139	REF (dB)	UUC (dB)	ERR (dB)	
STD dB				
139.00	139	139.0	0.0	1.1
134.00	134	134.0	0.0	1.1
129.00	129	129.0	0.0	1.1
124.00	124	124.0	0.0	1.1
119.00	119	119.0	0.0	1.1
114.00	114	114.0	0.0	1.1
109.00	109	109.0	0.0	1.1
104.00	104	104.0	0.0	1.1
99.00	99	99.0	0.0	1.1
94.00	94	94.0	0.0	1.1
89.00	89	89.0	0.0	1.1
84.00	84	84.0	0.0	1.1
79.00	79	79.0	0.0	1.1
74.00	74	74.0	0.0	1.1
69.00	69	69.0	0.0	1.1
64.00	64	64.0	0.0	1.1
59.00	59	59.0	0.0	1.1
54.00	54	54.0	0.0	1.1
49.00	49	49.0	0.0	1.1
44.00	44	44.0	0.0	1.1
39.00	39	39.3	0.3	1.1
38.00	38	38.3	0.3	1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd  
FM-708-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม

Certificate No : 22-ACT-103  
Request No : Req-2022-0230

#### 9. Level linearity including the level range control

UUC Setting	STD	Measured	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
FAST / A	REF (dB)	UUC (dB)	ERR (dB)	
UUC Range				
37-139	43.2	42.9	-0.3	1.1
	114	114.0	0.0	1.1

#### 10. Tone burst response

UUC Setting	STD	Anticipated	Measured	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
A / 37-139	Toneburst (ms)	Ref (dB)	UUC (dB)	ERR (dB)	
UUC Time Response					
Fast	200	135.0	135.0	0.0	1.0
	2	118.0	117.7	-0.3	+1.0, -2.5
	0.25	109.0	108.7	-0.3	+1.5, -5.0
Slow	200	128.6	128.5	-0.1	1.0
	2	109.0	108.9	-0.1	+1.0, -5.0
	200	129.0	129.0	0.0	1.0
SEL	2	109.0	109.0	0.0	+1.0, -2.5
	0.25	100.0	99.9	-0.1	+1.5, -5.0

#### 11. Peak C Sound level

UUC Setting	Anticipated	Measured	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
FAST / C / 95-142	REF (dB)	UUC (dB)	ERR (dB)	
STD Setting				
Complete cycle	137.4	136.7	-0.70	3.0
Positive half cycle	136.4	136.1	-0.30	2.0
Negative half cycle	136.4	136.2	-0.20	2.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd  
FM-708-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม

Certificate No : 22-ACT-103  
Request No : Req-2022-0230

12. Overload Indication

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 37-139	UUC	( ± dB)	( ± dB)
STD Setting	(dB)		
Positive one-half cycle	142.2		
Negative one-half cycle	142.3		
Deviated	-0.1	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 37-139	UUC	( ± dB)	( ± dB)
STD Setting	(dB)		
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

Certificate No : 22-ACT-104  
Request No : Req-2022-0232

1. Indication at the calibration check frequency

UUC Setting	Nominal Level (dB)	Before Adjust		Adjust		Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)	
FAST / A / 37-139						
Calibrator Setting						
1000 Hz 114.09 dB	113.83	114.0	+0.13	113.9	0.05	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN.58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	28.7	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	28.6	0.10
C	28.8	0.10
Z	34.7	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve				UNCERTAINTY ( ± dB)	Acceptance Limit ( ± dB)
	A (dB)	C (dB)	Z (dB)			
FAST / 37-139						
STD Setting						
125 Hz	0.0	0.1	0.1		0.50	2.0
1000 Hz	0.0	0.0	0.0		0.60	1.0
4000 Hz	0.7	0.7	0.7		0.60	3.0
8000 Hz	1.0	0.9	0.8		0.70	5.0

Certificate No : 22-ACT-104  
Request No : Req-2022-0232

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Responce curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	A (dB)	C (dB)	Z (dB)		
FAST / 37-139					
STD Setting					
63 Hz	-0.2	0.0	0.0		2.0
125 Hz	-0.1	0.0	0.0		1.5
250 Hz	-0.1	0.0	0.0		1.5
500 Hz	-0.1	0.0	0.0		1.5
1000 Hz	0.0	0.0	0.0	0.2	1.0
2000 Hz	0.0	0.1	0.0		2.0
4000 Hz	0.0	0.0	0.0		3.0
8000 Hz	0.0	0.0	0.0		5.0
16000 Hz	-0.1	-0.1	-0.1		+5, -INF.

6. Frequency and time weightings at 1kHz

UUC Setting	STD		Measured		Acceptance Limit (± dB)
	REF (dB)		UUC (dB)	ERR (dB)	
FAST / 37-139					
UUC Weighting					
A	114.00		114.0	0.0	0.2
C	114.00		114.0	0.0	0.2
Z	114.00		114.0	0.0	0.2

UUC Setting	STD		Measured		Acceptance Limit (± dB)
	REF (dB)		UUC (dB)	ERR (dB)	
37-139 / A					
UUC Time Response					
Fast	114.00		114.0	0.0	0.1
Slow	114.00		114.0	0.0	0.1
Leq	114.00		114.0	0.0	0.1



Certificate No : 22-ACT-104  
Request No : Req-2022-0232

7. Long term stability

UUC Setting	Measured		Acceptance Limit ( $\pm$ dB)
	FAST / A	UUC (dB)	
STD Setting	Initial	114.0	0.3
	Final	114.0	
Deviated	0.0	0.1	0.3

8. Level linearity on the reference level range

UUC Setting	Anticipated		Deviation	UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
	REF (dB)	UUC (dB)	ERR (dB)		
FAST / A / 37-139	140	140.0	0.0	0.3	1.1
	139	139.0	0.0		1.1
	134	134.0	0.0		1.1
	129	129.0	0.0		1.1
	124	124.0	0.0		1.1
	119	119.0	0.0		1.1
	114	114.0	0.0		1.1
	109	109.0	0.0		1.1
	104	104.0	0.0		1.1
	99	99.0	0.0		1.1
	94	94.0	0.0		1.1
	89	89.0	0.0		1.1
STD Setting	84	84.0	0.0		1.1
	79	79.0	0.0		1.1
	74	74.0	0.0		1.1
	69	69.0	0.0		1.1
	64	64.0	0.0		1.1
	59	59.0	0.0		1.1
	54	54.0	0.0		1.1
	49	49.0	0.0		1.1
	44	44.1	0.1		1.1
	39	39.3	0.3		1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd  
PIN-709-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม

Certificate No : 22-ACT-104  
Request No : Req-2022-0232

9. Level linearity including the level range control

UUC Setting	STD		Measured		UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
	FAST / A	REF (dB)	UUC (dB)	ERR (dB)		
UUC Range	44.1	43.7	-0.4	0.3	1.1	1.1
	114	114.0	0.0			

10. Tone burst response

UUC Setting	Anticipated		Measured		UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
	Toneburst (ms)	Ref (dB)	UUC (dB)	ERR (dB)		
UUC Time Response	200	135.0	135.0	0.0	0.3	1.0
	2	118.0	117.9	-0.1		+1.0, -2.5
	0.25	109.0	108.7	-0.3		+1.5, -5.0
Fast	200	128.6	128.5	-0.1	0.3	1.0
	2	109.0	108.8	-0.2		+1.0, -5.0
Slow	200	129.0	129.0	0.0	1.0	1.0
	2	109.0	109.1	+0.1		+1.0, -2.5
SEL	0.25	100.0	99.7	-0.3	+1.5, -5.0	+1.5, -5.0

11. Peak C Sound level

UUC Setting	Anticipated		Measured		UNCERTAINTY ( $\pm$ dB)	Acceptance Limit ( $\pm$ dB)
	FAST / C / 95-142	REF (dB)	UUC (dB)	ERR (dB)		
STD Setting	137.4	136.7	-0.70	6.2	3.0	2.0
	136.4	136.2	-0.20			
Complete cycle	136.4	136.2	-0.20	2.0	2.0	2.0
Positive half cycle	136.4	136.2	-0.20			
Negative half cycle	136.4	136.2	-0.20			

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd  
PIN-709-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม

Certificate No : 22-ACT-104  
 Request No : Req-2022-0232

12. Overload indication			
UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 37-139	UUC (dB)	( $\pm$ dB)	( $\pm$ dB)
STD Setting			
Positive one-half cycle	142.7		
Negative one-half cycle	142.6		
Deviated	0.1	0.2	1.5

13. High Level Stability			
UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 37-139	UUC (dB)	( $\pm$ dB)	( $\pm$ dB)
STD Setting			
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

เอกสารไม่ควบคุม

## Certificate of Calibration

**Customer**  
 Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.LTD.  
 Address : 81 Soi Udamsook 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 21-ACT-361  
 Request No : Req-2021-1241

### Unit Under Calibration Details

Measurement item : Noise dosimeter  
 Manufacturer : SVANTEK  
 Model : SV 104IS  
 Serial Number : 67627  
 ID : UAE.FPM.1062561  
 Resolution : 0.1 dB  
 Calibration Environment and Details  
 Temperature : 23°C  $\pm$  2°C  
 Humidity : 50%RH  $\pm$  20 %RH  
 Barometric Pressure : 1013 hPa  $\pm$  10 hPa  
 Received Date : 10 September 2021  
 Calibrated Date : 20 September 2021  
 Calibration Procedure : In-house method (CP-NDM-01) based on IEC 61252: 2017  
 Location of Calibration : Lab Acoustic

Microphone Class : 2  
 Microphone Model : SV 27IS  
 Microphone S/N : 68647  
 Preamplifier Model : -  
 Preamplifier S/N : -  
 Instrument Status : Used

### Reference Standard

Instrument	Brand	Model	S/N	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	18872	14 June 2022	TSI
Standard Microphone	GRAS	46AN	18873	29 October 2021	GRAS
Sine Generator	Svanick	Svan401	131	30 September 2021	WK Electric
Timer	EXTECH	-	05-ACT	29 March 2022	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :

Approved By :

Signature  
 Calibration Officer

Signature  
 Calibration Engineer Supervisor

Issue Date :

20 September 2021

เอกสารไม่ควบคุม

Certificate No : 21-ACT-361  
 Request No : Req-2021-1241

### 1. Absolute acoustical sensitivity

UUC Setting	Time	Exposure Measurement	UNCERTAINTY	Tolerances Limit (%)
FAST / A / 60-140	Ref (s)	UUC (Pa <sup>2</sup> /h)	Error (%)	
Calibrator Setting				
1000 Hz 114 dB	120.00	3.23	3.20	-0.93
				3.0
				-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SYANTER, Model SV 35A, SN: 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting	UNCERTAINTY	Tolerances Limit
FAST / 60-140	A C	(± dB)	(± dB)
STD Setting			
*63 Hz	-1.0	0.40	2.0
125 Hz	-0.4	0.40	1.5
250 Hz	-0.1	0.40	1.5
500 Hz	-0.1	0.40	1.5
1000 Hz	0.0	0.40	-
2000 Hz	0.0	0.40	2.0
4000 Hz	-0.8	0.40	3.0
8000 Hz	-2.1	0.40	5.0

### 3. Linearity of response to steady signals

a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting	Ref (dB)	60.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0
1000 Hz	Level A	80.3	80.3	90.0	100.0	110.0	114.0	120.0	130.0	140.0
	Error	0.6	0.3	0.0	0.0	0.0	0.0	0.0	0.0	0.0
8000 Hz	Ref (dB)	88.9	98.9	108.9	112.9	118.9	128.9	138.9		
	Level A	88.9	98.9	108.9	112.9	118.9	128.9	138.9		
	Error	0.0	0.0	0.0	0.0	0.0	0.0	-0.1	-0.1	0.0
63 Hz	Ref (dB)	87.8	93.8	103.8	113.8					
	Level A	87.8	93.8	103.8	113.8					
	Error	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0
Tolerances Limit										
UNCERTAINTY										

b. Sound exposure meter linearity of error

UUC Setting	Time	Exposure Measurement	UNCERTAINTY	Tolerances Limit (%)
FAST / A / 60-140	Ref (s)	UUC (Pa <sup>2</sup> /h)	Error (%)	
Calibrator Setting				
1000 Hz 110 dB	27	0.30	0.30	0.00
1000 Hz 110 dB	45	0.50	0.50	0.00
1000 Hz 110 dB	90	1.00	0.99	-1.00
1000 Hz 110 dB	180	2.00	1.98	-1.00
1000 Hz 120 dB	36	4.00	4.03	+0.75
1000 Hz 120 dB	72	8.00	8.05	+0.63
1000 Hz 120 dB	90	10.00	10.13	+1.30
1000 Hz 120 dB	180	20.00	20.22	+1.10
1000 Hz 120 dB	360	40.00	40.34	+0.85
1000 Hz 120 dB	720	80.00	80.40	+0.61
			4.3	-21, +26
			3.8	



Certificate No : 21-ACT-361  
Request No : Req-2021-1241

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement		Tolerances Limit
	Ref (s)	UUC (s)	UUC (Pa <sup>1</sup> h)	Error (Pa <sup>1</sup> h)	
FAST / A / 60-140 Calibrator Setting 4000 Hz 95 dB	2846	2846	1.00	-0.01	-0.29 - 0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement		Tolerances Limit
	Ref (s)	UUC (s)	UUC (Pa <sup>1</sup> h)	Error (%)	
FAST / A / 60-140 Calibrator Setting Burst 1 ms 95 dB	2846	2846	1.00	0.99	-21 - +26
Burst 1 ms 100 dB	900	900	1.00	0.99	-21 - +41
Burst 1 ms 108 dB	143	143	1.00	0.99	-21 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time		Exposure Measurement		Tolerances Limit
	Ref (s)	UUC (s)	UUC (Pa <sup>1</sup> h)	Different (%)	
FAST / A / 60-140 Calibrator Setting Continuous Rectangle + Continuous Rectangle -	7	7	10.61	0.00	-21 - +26

End of Certificate

#### Certificate of Calibration

**Customer**  
Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260  
Certificate No : 22-ACT-114  
Request No : Req-2022-0331

##### Unit Under Calibration Details

Measurement Item : Noise dosimeter  
Manufacturer : SVANTEK  
Model : SV104  
Serial Number : 91923  
ID : -  
Resolution : 0.1 dB  
Microphone Class : 2  
Microphone Model : SV27  
Microphone S/N : 96604  
Preamplifier Model : -  
Preamplifier S/N : -  
Instrument Status : Used

##### Calibration Environment and Details

Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 14 February 2022  
Calibrated Date : 17 February 2022  
Calibration Procedure : In-house method CP-NIDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic

##### Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Multi-frequency Calibrator	Quest	Quest-cal	188272	14 June 2022	TSL
Standard Microphone	GRAS	40AN	188273	15 September 2022	GRAS
Sine Generator	Svantek	Svm401	131	18 October 2022	WK Electric
Timer	EXTECH	-	05-ACT	29 March 2022	TPA

##### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By : [Signature]

Approved By : [Signature]

Calibration Officer

Calibration Engineer Supervisor

Issue Date : 17 February 2022

Certificate No : 22-ACT-114  
Request No : Req-2022-0331

1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement		Tolerances Limit (%)
	Ref (s)	UUC (s)	Ref (Pa <sup>2</sup> /h)	Error (%)	
FAST / A / 55-140					
Calibrator Setting					
1000 Hz 114 dB	120.00	120	3.23	-0.93	3.0

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN: 38079

2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting			Tolerances Limit (± dB)
	A (dB)	C (dB)	UUC (Pa <sup>2</sup> /h)	
FAST / 55-140				
STD Setting				
*63 Hz	-0.3	-0.3	0.40	2.0
125 Hz	-0.1	-0.2	0.40	1.5
250 Hz	-0.2	-0.3	0.40	1.5
500 Hz	-0.2	-0.2	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	0.0	0.0	0.40	2.0
4000 Hz	1.2	1.2	0.40	3.0
8000 Hz	-1.4	-1.3	0.40	5.0

Certificate No : 22-ACT-114  
Request No : Req-2022-0331

3. Linearity of response to steady signals

a. Sound exposure meter linearity of response for changes of input sinusoidal signal level

UUC Setting	Ref (dB)	FAST / A / High									
		55.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0	
1000 Hz	Level A	34.5	79.9	90.1	100.0	110.0	114.0	120.0	130.0	140.0	
	Error	-0.5	0.1	0.0	0.0	0.0	0.0	0.0	0.0	0.0	
	Ref	88.9	98.9	108.9	112.9	118.9	128.9	138.9			
8000 Hz	Level A	88.9	98.9	108.9	112.9	118.9	128.9	138.8			
	Error	0.0	0.0	0.0	0.0	0.0	0.0	0.0	-0.1		
	Ref	87.8	93.8	103.8	113.8						
63 Hz	Level A	87.8	93.8	103.8	113.8						
	Error	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	
	Ref	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	
Tolerances Limit		1.0									
UNCERTAINTY		0.27									

b. Sound exposure meter linearity of error

UUC Setting	Ref (s)	Time		Exposure Measurement			Tolerances Limit (%)
		Ref (s)	UUC (s)	Ref (Pa <sup>2</sup> /h)	UUC (Pa <sup>2</sup> /h)	Error (%)	
FAST / A / 55-140							
Calibrator Setting							
1000 Hz 110 dB	27	27	27	0.30	0.30	0.00	
1000 Hz 110 dB	45	45	45	0.50	0.51	+2.00	
1000 Hz 110 dB	90	90	90	1.00	1.01	+1.00	
1000 Hz 110 dB	180	180	180	2.00	2.02	+1.00	
1000 Hz 120 dB	36	36	36	4.00	3.94	-1.50	
1000 Hz 120 dB	72	72	72	8.00	7.87	-1.63	
1000 Hz 120 dB	90	90	90	10.00	9.90	-1.00	
1000 Hz 120 dB	180	180	180	20.00	19.76	-1.20	
1000 Hz 120 dB	360	360	360	40.00	39.42	-1.45	
1000 Hz 120 dB	720	720	720	80.00	78.66	-1.68	

Certificate No : 22-ACT-114  
Request No : Req-2022-0331

4. Response to short duration

a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement		Tolerances
	Ref	UUC	UUC	Error	
FAST / A / 35-140	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)
Calibrator Setting					
4000 Hz 95 dB	2846	2846	0.99	-0.01	0.01
					-0.29 ~ -0.41

b. Sound exposure meter response for series of tonburst impulses

UUC Setting	Time		Exposure Measurement		Tolerances
	Ref	UUC	UUC	Error	
FAST / A / 35-140	(s)	(s)	(Pa <sup>2</sup> h)	(%)	(%)
Calibrator Setting					
Burst 1 ms, 95 dB	2846	2846	1.00	-1.00	-21 ~ +26
Burst 1 ms, 100 dB	900	900	0.99	-1.00	-21 ~ -41
Burst 1 ms, 108 dB	143	143	1.01	+1.00	-21 ~ -41

5. Response to unipolar pulse

UUC Setting	Time		Exposure Measurement		Tolerances
	Ref	UUC	UUC	Different	
FAST / A / 35-140	(s)	(s)	(Pa <sup>2</sup> h)	(%)	(%)
Calibrator Setting					
Continuous Rectangle +			10.61	0.00	2.4
Continuous Rectangle -			10.61		-21 ~ +26

\* Indicates non accredited

End of Certificate

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangkok, Prakanong, Bangkok 10260  
Certificate No : 22-ACT-033  
Request No : Req-2022-0091

Unit Under Calibration Details

Measurement item : Noise dosimeter  
Manufacturer : SVANTEK  
Model : SV104  
Serial Number : 9925  
ID : UAE.FIM.165/2564  
Resolution : 0.1 dB  
Calibration Environment and Details  
Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 14 January 2022  
Calibrated Date : 21 January 2022  
Calibration Procedure : In-house method (CP-NDM-01) based on IEC 61332 : 2017  
Location of Calibration : Lab Acoustic  
Microphone Class : 2  
Microphone Model : SV27  
Microphone SN : 96602  
Preamplifier Model : -  
Preamplifier SN : -  
Instrument Status : Used

Reference Standard	Brand	Model	SN	Due calibration	Traceability
Instrument					
Multifrequency Calibrator	Quest	Quest-cal	188272	14 June 2022	TSI
Standard Microphone	GRAS	40AN	188273	15 September 2022	GRAS
Sine Generator	SvanteK	Svan401	131	18 October 2022	WK Electric
Timer	EXTECH	-	05-6CT	29 March 2022	TPA

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :

M: [Redacted]  
[Redacted]  
Calibration Officer

Approved By :

[Redacted]  
Calibration Engineer Supervisor

Issue Date :

21 January 2022

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.  
เอกสารไม่ควบคุม  
date 01/07/19



Certificate No : 22-ACT-033  
Request No : Req-2022-0091

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement		Tolerances Limit (%)
	Ref (s)	UUC (s)	Ref (Pa <sup>2</sup> h)	Error (%)	
FAST / A / 55-140					
Calibrator Setting					
1000 Hz 114 dB	120.00	120	3.23	-0.93	3.0

Note: Absolute sensitivity was established by the use of Sound Calibrator Brand SYVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequencies Weighting			Tolerances Limit (± dB)
	A (dB)	C (dB)	UNCERTAINTY (± dB)	
FAST / 55-140				
STD Setting				
*63 Hz	-0.3	-0.3	0.40	2.0
125 Hz	-0.2	-0.2	0.40	1.5
250 Hz	-0.2	-0.1	0.40	1.5
500 Hz	-0.2	-0.2	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	0.4	0.5	0.40	2.0
4000 Hz	0.2	0.3	0.40	3.0
8000 Hz	-1.8	-1.9	0.40	5.0

Certificate No : 22-ACT-033  
Request No : Req-2022-0091

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting	Ref (dB)	FAST / A / High									
		55.0	60.0	65.0	70.0	75.0	80.0	85.0	90.0	95.0	100.0
1000 Hz	Level A	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)
	Error	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)
		-0.8	0.1	0.1	0.1	0.1	0.0	0.0	0.0	0.0	0.0
8000 Hz	Ref	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)
	Level A	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)
	Error	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)
63 Hz	Ref	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)
	Level A	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)
	Error	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)	(dB)
Tolerances Limit		1.0									
UNCERTAINTY		0.27									

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			Tolerances Limit (%)
	Ref (s)	UUC (s)	Ref (Pa <sup>2</sup> h)	UUC (Pa <sup>2</sup> h)	Error (%)	
FAST / A / 55-140						
Calibrator Setting						
1000 Hz 110 dB	27	27	0.30	0.30	0.00	
1600 Hz 110 dB	45	45	0.50	0.50	0.00	
1000 Hz 110 dB	90	90	1.00	1.01	+1.00	
1000 Hz 110 dB	180	180	2.00	2.02	+1.00	
1000 Hz 120 dB	36	36	4.00	4.03	+0.75	
1000 Hz 120 dB	72	72	8.00	8.05	+0.63	
1000 Hz 120 dB	90	90	10.00	10.13	+1.30	
1000 Hz 120 dB	180	180	20.00	20.22	+1.10	
1000 Hz 120 dB	360	360	40.00	40.34	+0.85	
1000 Hz 120 dB	720	720	80.00	80.49	+0.61	

Certificate No : 22-ACT-033  
Request No : Req-2022-0091

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement		Tolerances
	Ref	UUC	UUC	Error	
FAST / A / 55-140	(s)	2846	(Pa h)	(Pa <sup>2</sup> h)	Limit
Calibrator Setting					(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846		0.99	-0.01	0.01 -0.29 - 0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement		Tolerances
	Ref	UUC	Ref	Error	
FAST / A / 55-140	(s)	2846	(Pa h)	(%)	Limit
Calibrator Setting					(%)
Burst 1 ms, 95 dB	2846		1.00	-1.00	-21 - +26
Burst 1 ms, 100 dB	900		1.00	0.00	3.0 -21 - +41
Burst 1 ms, 108 dB	143		1.00	0.00	-21 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time		Exposure Measurement		Tolerances
	Ref	UUC	UUC	Different	
FAST / A / 55-140	(s)	2846	(Pa h)	(%)	Limit
Calibrator Setting					(%)
Continuous Rectangle +	7		10.86	0.00	2.4 -21 - +26
Continuous Rectangle -			10.86		

\* Indicates non accredited

End of Certificate

### Certificate of Calibration

#### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.LTD. Certificate No : 21-ACT-326  
Address : 81 Soi Udeniauk 41, Sukhumvit Road, Bangchak, Request No : Req-2021-0994  
Prakanong, Bangkok 10260

#### Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1  
Manufacturer : SVANTEK Range : 94 , 114 dB / 1000 Hz  
Model : SV36 Instrument Status : Used  
Serial Number : 107224  
ID : UAE.EFM.171.2564

#### Calibration Environment and Details

Temperature : ( 23 ±2 °C )  
Humidity : ( 50 ± 20 %RH )  
Barometric Pressure : ( 1013 ±10.0 hPa )  
Received Date : 22 July 2021  
Calibration Date : 24 August 2021  
Location of Calibration : LAB 1 Acoustic  
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEL	14 May 2022
THD Multimeter	2015	1047765	NIMT	21 January 2022

#### Traceability

This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

#### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By :

Mr. Suphassakorn Kongsakul

Approved By :

Mr. Paet Mahavorn

Service Calibration Engineer

Calibration Engineer Supervisor

Issue Date : 24 August 2021



Certificate No : 21-ACT-326

Request No : Req-2021-0994

Calibration Results : Without Adjustment

Sound pressure level

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty ( $\pm$ dB)	Acceptance limit Class 1 ( $\pm$ dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	94.08	0.08	-	-	0.11	0.25
114 dB / 1000 Hz	114.13	0.13	-	-	0.11	0.25

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( $\pm$ %)	Acceptance limit Class 1 ( $\pm$ %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	999.96	0.004	-	-	0.10	0.70
114 dB / 1000 Hz	999.98	0.002	-	-	0.10	0.70

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( $\pm$ %)	Acceptance limit Class 1 ( $\pm$ %)
	Measured (%)	Error (%)	Measured (%)	Error (%)		
94 dB / 1000 Hz	0.43	-	-	-	0.40	2.5
114 dB / 1000 Hz	0.35	-	-	-	0.40	2.5

Note :

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibration pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration



Accuracy Calibration Certificate

Customer


Company:  
United Analyst and Engineering Consultant Co., Ltd.

Address:  
3 Soi Udom Suk 41, Sukhumvit Rd., Bang Chak

City:  
Phra Khanong

Zip / Postal:  
10260

State / Province:  
Bangkok

Order Number:  
  
\* 0 1 3 2 4 2 9 8 0 \*

Contact:  
Suwit Chotnok

Weighing Device

Manufacturer:  
Mettler Toledo

Model:  
AB204-S

Serial No.:  
1128312528

Building:  
N/A

Floor:  
2

Room:  
Balance Room 2 (206)

Weighing Instrument  
Type:  
UAE, AIE 010/2550

Asset Number:  
N/A

Terminal Model:  
N/A

Terminal Serial No.:  
N/A

Terminal Asset No.:  
N/A

Range	Max. Capacity	Readability (d)
1	220 g	0.001 g

Procedure

Calibration Guideline:  
EURAMET cg-18 v. 4.0 (11/2015)  
CP/W002/20


METTLER TOLEDO Work Instruction:  
This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.  
The sensitivity span of the weighing instrument was adjusted before calibration with a built-in weight.  
In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

Temperature		Humidity		
As Found	Start: 22.5 °C	End: 21.4 °C	Start: 56.1 %	End: 63.2 %

As Found Calibration Date:  
07-Apr-2022

As Left Calibration Date:  
N/A

Issue Date:  
06-Apr-2022

Calibrator:  


Approved Signatory:  
☒ Kassaikom Tassanachaisakul  
☐ Santi Jimjorn  
☐ Surachet Sukkate

เอกสารไม่ควบคุม


No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	No.	Certification	Date of Calibration	Due date of Remark
1	Analytical Balance (Readability 0.1 mg) PM10	น้ำหนักของ (TSP)	Mettler-Toledo	AB204-S / 1128312528	Mettler-Toledo (Thailand) Ltd. ACC-TH	TH2058-097-040722-	7 Apr 22	7 Apr 23	-
2	Analytical Balance (Readability 0.1 mg)	น้ำหนักของ (TSP)	Mettler-Toledo	AB204-S/FACT / B108115858	Mettler-Toledo (Thailand) Ltd. ACC-TH	TH2058-098-040722-	7 Apr 22	6 Apr 23	-
3	UV-VIS Spectrophotometer (Readability 0.1 mg) (Nox as NO2)	ค่าการดูดกลืนแสงในรูปไนโตรเจนไดออกไซด์	Agilent Technologies	Cary60 66860A / M15410009	DOE Services Co.,Ltd.	SP22-016	31 May 22	30 May 23	-
4	UV-VIS Spectrophotometer (Nox as NO2)	ค่าการดูดกลืนแสงในรูปไนโตรเจนไดออกไซด์	Hitech	U-1900 / 2021-064	DOE Services Co.,Ltd.	SP22-007	20 Jan 22	19 Jan 23	-
5	pH Meter	ค่าความเป็นกรด-ด่าง	Mettler-Toledo	Seven Easy 520 / 1231155210	National Food Institute, Ministry of Industry, Thailand	2201793-001-01	1 Mar 22	28 Feb 23	-
6	pH Meter	ค่าความเป็นกรด-ด่าง	Mettler-Toledo	Seven Easy 520 / 1230525212	National Food Institute, Ministry of Industry, Thailand	2202093-001-01	16 Mar 22	15 Mar 23	-
7	Analytical Balance (Readability 0.01 mg)	น้ำหนักของ	Mettler-Toledo	XSR205DU / C210685394	Mettler-Toledo (Thailand) Ltd.	2058-043-050622-ACC-	9 May 22	8 May 23	-
8	Hot Air Oven	ค่าการอบแห้ง	Mement	UF55 / B216.1666	Technology Promotion Association (Thailand-Japan)	21TM1876	29 Oct 21	28 Oct 22	-
9	BOD Incubator	ค่าการหมัก	Arco	UC4-1320 / UAE.WAO.015/2561	Technology Promotion Association (Thailand-Japan)	22TM90	17 Feb 22	16 Feb 23	-
10	Analytical Balance (Readability 0.1 mg)	น้ำหนักและน้ำหนัก	Mettler-Toledo	AB-204S/FACT / 1129361010	National Food Institute, Ministry of Industry, Thailand	2203120-001-01	1 Jun 22	31 May 23	-

รายการรับรองสอบเทียบความสามารถของเครื่องมือหลักประจำห้องปฏิบัติการ

ผลการรับรองความสามารถสอบเทียบความสามารถของเครื่องมือหลักประจำห้องปฏิบัติการได้รับการประเมินและประกาศตามข้อกำหนด  
ในการรับฟังข้อสงสัยภายใน 30 วันทำการ (see the plan) บริษัท บัณฑิตสหวิทยา จำกัด  
ประเทศไต้หวัน - กรุงเทพฯ 2565

## Measurement Results

### Repeatability

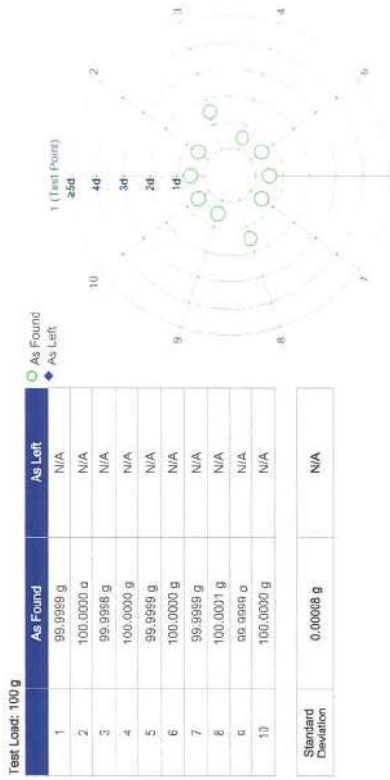

The 'g' in the graph represents the readability of the range interval in which the test was performed.  
The results of this graph are based upon the absolute values of the differences from the mean value.


### Eccentricity



The 'd' in the graph represents the readability of the range interval in which the test was performed.

## Error of Indication

As Found	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.0000 g	0.0000 g	0.0000 g	0.13 mg	2
2	0.1000 g	0.1000 g	0.0000 g	0.13 mg	2
3	1.0000 g	0.9998 g	-0.0001 g	0.13 mg	2
4	5.0000 g	5.0000 g	0.0000 g	0.13 mg	2
5	10.0000 g	9.9998 g	-0.0001 g	0.20 mg	2
6	20.0000 g	20.0000 g	0.0000 g	0.21 mg	2
7	50.0000 g	50.0000 g	0.0000 g	0.23 mg	2
8	70.0001 g	70.0000 g	-0.0001 g	0.23 mg	2
9	100.0000 g	100.0000 g	0.0000 g	0.23 mg	2
10	150.0000 g	150.0002 g	0.0002 g	0.40 mg	2
11	200.0001 g	200.0003 g	0.0002 g	0.43 mg	2

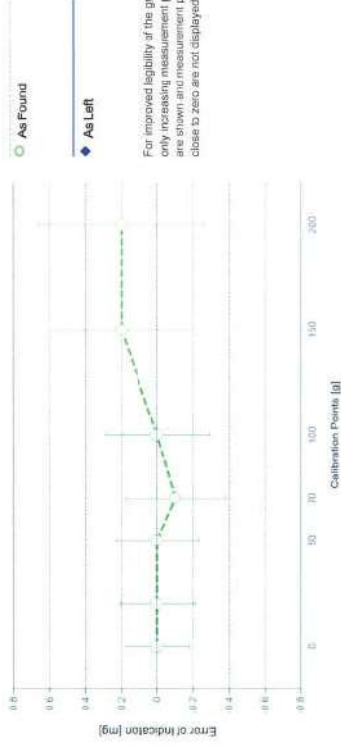

For improved legibility of the graphics only increasing measurement points are shown and measurement points close to zero are not displayed.

The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor k – which can be larger than 2 according to EURAMET cg-18. The value of the measurement lies within the assigned range of values with a probability of approximately 95%.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.

## Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

### Weight Set 1: OIML E2

Weight Set No.	WES0	Date of Issue:	23 Feb-2022
Certificate Number:	C208581031	Calibration Due Date:	14-Aug-2023

### Thermo Hygrometer

Equipment No.	IN161	Date of Issue:	14-Jun-2021
Certificate Number:	21H1220	Calibration Due Date:	01-Jun-2022

Remarks

Equipment condition: Good  
Next calibration according to customer's procedure  
Calibration data not decide by calibration laboratory  
Test weight by Filer pan : 1 g = 0.9999g , 5 g = 3.0000 g , 5 g = 5.0000 g

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with k=2 in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use:

$3.0 \cdot 10^{-6} / K$

Temperature range in use for the evaluation of the measurement uncertainty in use:

3 K


Uncertainty of Uncertainty Equation

	Range		As Found	As Left
	d	Max		
1	0.0001 g	220 g	$U_1 = 0.19 \text{ mg} + 0.00817 \text{ mg/g} \cdot R$	N/A

To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)


Net Indication	As Found	As Left
0.0220 g	0.19 mg	N/A
0.2200 g	0.19 mg	N/A
2.2000 g	0.21 mg	N/A
22.0000 g	0.37 mg	N/A
220.0000 g	2.9 mg	N/A

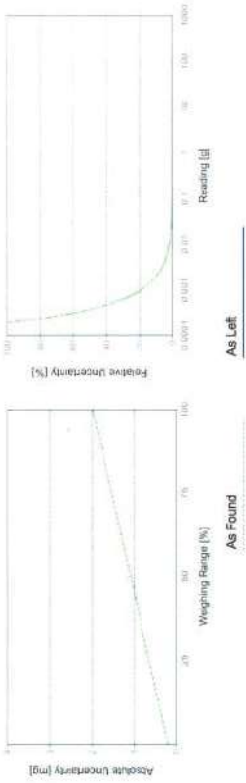



## Accuracy Calibration Certificate

Customer

Company:  
United Analyst and Engineering Consultant Co., Ltd.  
Address:  
3 Soi Udom Suk 41, Sukhumvit Rd., Bang Chak  
City:  
Phra Khanong  
Zip / Postal:  
10260  
State / Province:  
Bangkok  
Order Number:  


Contact:  
Suvit Chotirok

### Weighing Device

Manufacturer:	Mettler Toledo	Instrument Type:	Weighing Instrument
Model:	AB204-S/FACT	Asset Number:	UAE.AIR.01672555
Serial No.:	B108115858	Terminal Model:	N/A
Building:	N/A	Terminal Serial No.:	N/A
Floor:	2	Terminal Asset No.:	N/A
Room:	Balance Room 2 (206)		

Range	Max. Capacity	Readability (d)
1	220 g	0.0001 g

### Procedure

Calibration Guideline:  
METTLER TOLEDO Work Instruction:  
EURAMET cg-18 v.4.0 (11/2015)  
CP/W0102/20

This calibration certificate contains measurements for As Found and As Left calibrations.

The sensitivity/span of the weighing instrument was adjusted before As Found and As Left calibrations with a built-in weight.

In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

	Temperature	Humidity
As Found	Start: 22.6 °C    End: 22.1 °C	Start: 56.0 %    End: 51.9 %
As Left	Start: 22.3 °C    End: 22.4 °C	Start: 46.2 %    End: 55.8 %

As Found Calibration Date:	07-Apr-2022	Calibrator:	
As Left Calibration Date:	07-Apr-2022		
Issue Date:	08-Apr-2022	Approved Signatory:	



☐ Santi Jirinyon  
☐ Surachai Sukkate

### Measurement Results

#### Repeatability




#### Eccentricity



Error of Indication

As Found				
Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1 0.0000 g	0.0000 g	0.0000 g	0.15 mg	2
2 0.1000 g	0.1001 g	0.0001 g	0.15 mg	2
3 1.0000 g	0.9996 g	-0.0001 g	0.15 mg	2
4 5.0000 g	5.0006 g	0.0006 g	0.15 mg	2
5 10.0000 g	10.0001 g	0.0001 g	0.17 mg	2
6 20.0000 g	20.0001 g	0.0001 g	0.15 mg	2
7 50.0000 g	50.0003 g	0.0003 g	0.20 mg	2
8 70.0001 g	70.0005 g	0.0004 g	0.23 mg	2
9 100.0000 g	100.0005 g	0.0005 g	0.27 mg	2
10 150.0000 g	150.0007 g	0.0007 g	0.38 mg	2
11 200.0001 g	200.0008 g	0.0007 g	0.44 mg	2

As Left				
Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1 0.0000 g	0.0000 g	0.0000 g	0.15 mg	2
2 0.1000 g	0.1000 g	0.0000 g	0.15 mg	2
3 1.0000 g	0.9996 g	-0.0001 g	0.17 mg	2
4 5.0000 g	5.0000 g	0.0000 g	0.17 mg	2
5 10.0000 g	10.0000 g	0.0000 g	0.17 mg	2
6 20.0000 g	20.0000 g	0.0000 g	0.18 mg	2
7 50.0000 g	50.0000 g	0.0000 g	0.21 mg	2
8 70.0001 g	70.0001 g	0.0000 g	0.25 mg	2
9 100.0000 g	100.0000 g	0.0000 g	0.28 mg	2
10 150.0000 g	150.0001 g	0.0001 g	0.39 mg	2
11 200.0001 g	200.0001 g	0.0000 g	0.45 mg	2

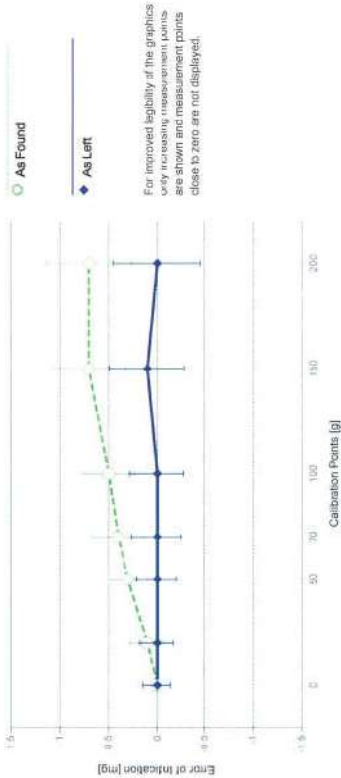

The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor  $k = 2$  - which can be larger than 2 according to EURAMET cg-18. The value of the measurand lies within the assigned range of values with a probability of approximately 95%.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2			
Weight Set No.:	WS80	Date of Issue:	23-Feb-2022
Certificate Number:	C208581631	Calibration Due Date:	14-Aug-2023
Thermo Hygrometer			
Equipment No.:	IM161	Date of Issue:	14-Jun-2021
Certificate Number:	Z1H1220	Calibration Due Date:	01-Jun-2022

Remarks

FACT adjustment functionality activated  
Value of the built-in weight adjusted

Equipment condition: Good  
Next calibration according to customer's procedure  
Calibration data not decide by calibration laboratory

Test weight by Filter pan : 1 g = 1.0000 g, 3 g = 3.0000 g, 5 g = 5.0000 g

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with  $k=2$  in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value  $R$  represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use:

2.5 · 10<sup>-6</sup> / K

Temperature range on site for the evaluation of the measurement uncertainty in use:

3 K



Linearity of Linearity Equation

Range	As Found		As Left
	d	Max	
1	0.0001 g	220 g	$U_1 = 0.16 \text{ mg} \pm 0.00932 \text{ mg/g} \cdot R$

To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a least load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication	As Found		As Left	
0.0220 g	0.16 mg	0.73%	0.16 mg	0.73%
	0.16 mg	0.074%	0.16 mg	0.073%
2.2000 g	0.16 mg	0.0064%	0.17 mg	0.0070%
	0.40 mg	0.0018%	0.29 mg	0.0013%
22.0000 g	2.4 mg	0.0012%	1.5 mg	0.00066%

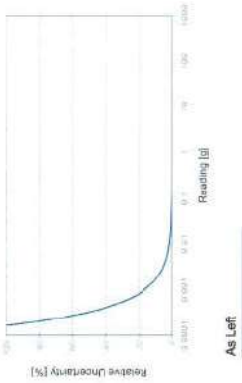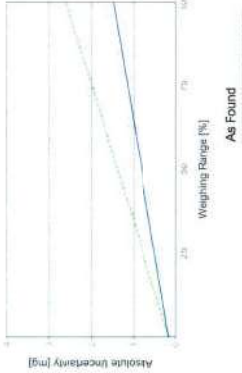

CERTIFICATE OF CALIBRATION

Certificate No. : SP22-016

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co., Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong,

Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009

ID No. : N/A

Received Date : 23 May 2022

Calibration Date : 23 May 2022

Issue Date : 26 May 2022

Condition Instrument : Good

Calibrated by :

( Mr. Tanawat Rittdach )  
Technical Manager

Approved by :

( Ms. Chuenmea Sangngern )  
Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม







# CERTIFICATE OF CALIBRATION

Certificate No.: SP22-007

Page 1 of 5

**Customer :** United Analyst and Engineering Consultant Co., Ltd. (Head Office)

**Address :** 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong,

Bangkok 10260

Location of calibration: Laboratory 315

**Equipment:** UV-Vis Spectrophotometer

**Manufacturer :** Hitachi

Model : U-1900

Serial No.: 2021-064

ID No.: UAE.WAS.006/2552

Received Date : 20 January 2022

Calibration Date: 20 January 2022

Issue Date : 24 January 2022

Condition Instrument: Good

Calibrated by: [REDACTED]  
Approved by: [REDACTED]

Approved by :

ridach)

### Technical Manager

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DOE Services Co., Ltd.

## REPORT OF CALIBRATION

Certificate No.: SP22-007

Page 2 of 5

Environment Condition: Ambient Temperature  $25 \pm 5$  °C

Relative humidity  $55 \pm 70\%$  RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

**Certified Reference Materials :**

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	95935	22 October 2023
Absorbance Standard set	25757	95929	22 October 2023
Wavelength Standard set	25806	95916	22 October 2023
Wavelength Standard set	25758	95915	22 October 2023

**Traceability** This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC: 4.0 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC: 0.1 nm.

Resolution of UUC: Photometric 0.001 Abs.

Wavelength 0.1 nm.



## REPORT OF CALIBRATION

Certificate No. : SP22-007

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5787	0.577	0.0017	0.0031	2.00
	1.0490	1.050	-0.0010	0.0029	2.00
440	2.1900	2.183	0.0070	0.0080	2.00
	0.0000	0.000	0.0000	0.0028	2.00
	0.5607	0.560	0.0007	0.0034	2.00
465	1.0247	1.023	0.0017	0.0035	2.00
	2.1229	2.118	0.0049	0.0079	2.00
	0.0000	0.000	0.0000	0.0028	2.00
546.1	0.5236	0.521	0.0026	0.0030	2.00
	0.9634	0.963	0.0004	0.0029	2.00
	1.9763	1.974	0.0023	0.0070	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5191	0.518	0.0011	0.0031	2.00
	1.0003	1.000	0.0003	0.0033	2.00
635	1.9987	1.996	0.0027	0.0084	2.00
	0.0000	0.000	0.0000	0.0028	2.00
	0.5523	0.552	0.0003	0.0030	2.00
635	1.0809	1.082	-0.0011	0.0030	2.00
	2.0391	2.033	0.0061	0.0079	2.00
	0.0000	0.000	0.0000	0.0028	2.00
635	0.5601	0.562	-0.0019	0.0031	2.00
	1.0512	1.052	-0.0008	0.0030	2.00
	1.9294	1.925	0.0044	0.0079	2.00

FM-708-02 R01 1/11/2021

เอกสารไม่ควบคุม

## REPORT OF CALIBRATION

Certificate No. : SP22-007

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7478	0.746	0.0018	0.0057	2.00
	0.0000	0.000	0.0000	0.0050	2.00
257	0.8686	0.861	0.0076	0.0059	2.00
	0.0000	0.000	0.0000	0.0050	2.00
	0.2912	0.291	0.0002	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6448	0.638	0.0068	0.0055	2.00
	0.0000	0.000	0.0000	0.0050	2.00

FM-708-02 R01 1/11/2021

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Page 5 of 5

Certificate No. : SP22-007

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.54	240.8	0.74	0.18	2.00
279.40	278.5	0.90	0.18	2.00
288.70	288.0	0.70	0.18	2.00
334.22	333.5	0.72	0.18	2.00
361.26	360.5	0.76	0.18	2.00
418.48	418.0	0.48	0.18	2.00
446.70	446.0	0.70	0.18	2.00
453.20	453.0	0.20	0.18	2.00
460.06	459.5	0.56	0.18	2.00
536.90	536.0	0.90	0.18	2.00
637.94	637.2	0.74	0.18	2.00
440.74	440.0	0.74	0.18	2.00
472.22	471.6	0.62	0.18	2.00
513.70	513.0	0.70	0.18	2.00
528.72	528.0	0.72	0.18	2.00
574.60	573.8	0.80	0.18	2.00
585.48	584.6	0.88	0.20	2.00
684.63	684.0	0.63	0.18	2.00
740.27	739.8	0.47	0.20	2.00
748.28	747.8	0.48	0.18	2.00
807.16	806.4	0.76	0.18	2.00
879.70	878.8	0.90	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k.
- which for a normal distribution corresponds to a coverage probability of approximately 95%

- \* Indicates non TISI accredited

- End of Certificate -

FM-708-02 R01 1/1/2021

เอกสารไม่ควบคุม



Request No. 25-65 / 0398

MTC. ACL No. 486 / 65

CALIBRATION CERTIFICATE

NOMENCLATURE : 1. Atomic Absorption Spectrophotometer "Agilent Technologies"

Model M240FS, Serial No. MY13160001

2. Working standard solution "Inorganic Ventures"

Multi Analyte Custom Grade Solution, Lot No. P2-MEB675610

SUBMITTED BY : United Analyst and Engineering Consultant Co., Ltd.

3. Soi Udomsuk41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10240

CALIBRATION PROCEDURE : 1. Performance Verification of Atomic Absorption Spectrophotometer (WI-500-02-30)

2. Estimation Uncertainty of Measurement in Analytical Chemistry (OP-513)

REFERENCE MATERIAL : Traceable to NIST "Agilent Technologies", "Carlo Erba"

Cadmium Lot No. 0108047046, Chromium Lot No. 0105315418, Copper Lot No. 0107480530, Iron Lot No. 0104697366,

Lead Lot No. 0104659473, Manganese Lot No. T109228A, Nickel Lot No. 0104978094, Zinc Lot No. 0100792297

CALIBRATION RANGE: 0.020.10.0.30.0.50.0.70 mg/l at 228.8 nm.Cd, 0.10.0.20.0.30.0.50.0.70 mg/l at 357.9 nm.Cr, 0.05.0.10.0.30.0.50.0.70 mg/l at 324.7 nm.Cu, 0.10.0.30.0.50.0.70.1.00 mg/l at 248.3 nm.Fe, 0.20.0.50.0.70.1.00.1.50 mg/l at 217.0 nm.Pb, 0.05.0.10.0.30.0.50.0.70 mg/l at 279.5 nm.Mn, 0.10.0.30.0.50.0.70.1.00 mg/l at 232.0 nm.Ni, 0.05.0.10.0.30.0.50.0.70 mg/l at 213.9 nm.Zn

AMBIENT CONDITIONS : Temperature 22 °C Relative humidity 60 %

The Atomic Absorption Spectrophotometer set has been calibrated against Reference Material traceable to National Institute of Standards and Technology ( NIST ) by The Analytical Chemistry Laboratory. The results are attached herewith.



Calibrated by  
( Mr. Danal Srithongkum )

Approved by  
( Mr. [Redacted] )

Director of Analytical Chemistry Laboratory

Ref. 2025265020400522001

Calibration Date : 3 February 2022

The results relate only to the items tested/calibrated or value assigned

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.DL.VTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Nong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
Email : rumpl@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2223 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9145  
E-mail : mtg@tistr.or.th

Office  
199 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2377 8832  
Fax. (66) 0 2377 8832  
Email : sumalee@tistr.or.th





Request No. 25-65 / 0398

1 / 5

MTC. ACL. No. 486 / 65

## CALIBRATION DATA

## 1. Noise Level in term of standard deviation

Element	Cd	Cr	Cu	Fe	Pb	Mn	Ni	Zn
Absorbance	-0.0004	0.0002	0.0007	0.0002	-0.0016	-0.0001	-0.0004	-0.0001
	0.0002	-0.0005	0.0010	0.0007	0.0000	-0.0003	0.0007	-0.0014
	-0.0002	0.0001	0.0008	0.0000	-0.0001	-0.0003	-0.0012	-0.0006
	0.0000	-0.0007	0.0007	0.0000	-0.0005	-0.0004	-0.0004	-0.0012
	0.0001	0.0004	0.0013	0.0014	-0.0001	-0.0001	0.0003	-0.0008
	0.0000	-0.0004	0.0003	-0.0012	-0.0005	-0.0007	-0.0004	-0.0008
	0.0000	-0.0009	0.0009	-0.0002	-0.0010	-0.0008	0.0007	-0.0003
	-0.0004	-0.0003	0.0015	0.0010	-0.0005	-0.0003	-0.0002	-0.0004
	0.0004	0.0008	0.0014	-0.0004	0.0014	0.0005	-0.0006	-0.0003
	-0.0006	-0.0013	0.0012	-0.0006	-0.0006	-0.0006	-0.0007	-0.0007
	0.0005	-0.0003	0.0014	-0.0004	-0.0008	-0.0003	-0.0006	-0.0011
	-0.0007	-0.0014	0.0004	-0.0001	-0.0001	0.0000	0.0000	-0.0003
	0.0008	0.0004	0.0005	-0.0006	-0.0008	0.0000	-0.0005	-0.0009
	0.0011	0.0002	0.0005	0.0017	-0.0016	-0.0008	0.0004	-0.0005
	0.0002	0.0010	0.0014	-0.0002	-0.0010	-0.0010	0.0002	-0.0001
	0.0001	-0.0011	0.0011	-0.0003	-0.0011	-0.0003	-0.0008	-0.0012
	0.0000	-0.0015	0.0009	-0.0010	-0.0011	-0.0013	0.0000	-0.0004
	0.0015	-0.0012	0.0005	0.0002	-0.0017	-0.0001	0.0005	-0.0002
	0.0006	0.0014	0.0010	0.0002	-0.0003	0.0001	-0.0006	-0.0010
	0.0001	0.0003	0.0003	-0.0001	-0.0004	-0.0002	-0.0001	-0.0001
Average Absorbance	0.0001	0.0000	0.0001	0.0000	-0.0001	0.0000	0.0000	-0.0001
Standard Deviation	0.0005	0.0008	0.0004	0.0007	0.0005	0.0004	0.0005	0.0004

Continue 2 / 5

## INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governing authority.

## Head Office

35 Mu. 3 Tambon Khlong Luang, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpat@isttr.or.th Website: www.isttr.or.th

## Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@isttr.or.th

## Office

199 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : sumit@isttr.or.th

IMT/MTC-002 Rev.4

เอกสารไม่ควบคุม



Request No. 25-65 / 0398

2 / 5

MTC. ACL. No. 486 / 65

## 2. Precision

Element	Conc. (mg/l)	Absorbance										Ave. Abs.	SD	%RSD
Cd	0.02	0.0074	0.0062	0.0065	0.0062	0.0070	0.0068	0.0070	0.0065	0.0065	0.0069	0.007	0.0004	5.76
	0.30	0.0952	0.0959	0.0951	0.0957	0.0952	0.0950	0.0952	0.0948	0.0956	0.0943	0.095	0.0005	0.49
	0.70	0.2213	0.2180	0.2203	0.2208	0.2234	0.2211	0.2196	0.2219	0.2194	0.221	0.221	0.0015	0.67
Cr	0.10	0.0096	0.0098	0.0097	0.0102	0.0106	0.0097	0.0098	0.0099	0.0103	0.0093	0.010	0.0004	3.83
	0.30	0.0309	0.0302	0.0300	0.0316	0.0306	0.0299	0.0309	0.0297	0.0311	0.0296	0.030	0.0007	2.20
	0.70	0.0659	0.0667	0.0664	0.0649	0.0656	0.0662	0.0658	0.0638	0.0663	0.0669	0.066	0.0011	1.70
Cu	0.05	0.0080	0.0075	0.0078	0.0075	0.0077	0.0081	0.0080	0.0075	0.0074	0.0076	0.008	0.0003	3.26
	0.30	0.0417	0.0419	0.0412	0.0421	0.0424	0.0420	0.0423	0.0403	0.0418	0.0415	0.042	0.0006	1.47
	0.70	0.0969	0.0965	0.0972	0.0957	0.0961	0.0958	0.0961	0.0963	0.0959	0.0972	0.096	0.0006	0.58
Fe	0.10	0.0090	0.0105	0.0078	0.0099	0.0091	0.0093	0.0096	0.0094	0.0093	0.0084	0.009	0.0007	8.11
	0.50	0.0462	0.0470	0.0464	0.0464	0.0467	0.0462	0.0467	0.0460	0.0468	0.0466	0.047	0.0003	0.67
	1.30	0.0867	0.0886	0.0910	0.0892	0.0897	0.0873	0.0892	0.0885	0.0888	0.0874	0.089	0.0013	1.43
Pb	0.20	0.0091	0.0095	0.0088	0.0087	0.0082	0.0094	0.0090	0.0087	0.0082	0.0090	0.009	0.0004	4.94
	0.70	0.0322	0.0321	0.0324	0.0318	0.0335	0.0326	0.0327	0.0315	0.0336	0.0321	0.032	0.0007	2.09
	1.50	0.0653	0.0645	0.0663	0.0664	0.0652	0.0671	0.0662	0.0666	0.0657	0.0648	0.066	0.0008	1.28
Mn	0.05	0.0092	0.0092	0.0097	0.0087	0.0085	0.0079	0.0096	0.0085	0.0084	0.0099	0.009	0.0007	7.33
	0.30	0.0616	0.0630	0.0632	0.0633	0.0634	0.0628	0.0640	0.0633	0.0640	0.0629	0.063	0.0007	1.08
	0.70	0.1396	0.1366	0.1386	0.1377	0.1386	0.1386	0.1396	0.1380	0.1374	0.1383	0.138	0.0009	0.67
Ni	0.10	0.0102	0.0092	0.0097	0.0104	0.0091	0.0105	0.0105	0.0096	0.0098	0.0102	0.010	0.0005	5.22
	0.50	0.0488	0.0489	0.0489	0.0495	0.0404	0.0490	0.0481	0.0492	0.0495	0.0492	0.049	0.0004	0.91
	1.00	0.0976	0.0979	0.0975	0.0992	0.0977	0.0973	0.0986	0.0962	0.0985	0.0982	0.098	0.0008	0.85
Zn	0.05	0.0340	0.0349	0.0340	0.0352	0.0337	0.0351	0.0344	0.0346	0.0349	0.0343	0.035	0.0005	1.49
	0.30	0.1669	0.1653	0.1628	0.1642	0.1657	0.1637	0.1659	0.1652	0.1654	0.1657	0.165	0.0012	0.72
	0.70	0.3456	0.3467	0.3465	0.3430	0.3422	0.3404	0.3437	0.3438	0.3435	0.3438	0.344	0.0013	0.37

Continue 3 / 5

## INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governing authority.

## Head Office

35 Mu. 3 Tambon Khlong Luang, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpat@isttr.or.th Website: www.isttr.or.th

## Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@isttr.or.th

## Office

199 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : sumit@isttr.or.th

IMT/MTC-002 Rev.4

เอกสารไม่ควบคุม





Request No. 25-65 / 0398

3 / 5

MTC. ACL. No. 486 / 65

### 3. Trueness

#### 3.1 Reading on wavelength- Cadmium (Cd) at 228.8 nm.

Element	Standard value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cd	0.02034	0.019	-0.001	5.19	± 0.004
	0.30060	0.291	-0.010	3.19	± 0.006
	0.70140	0.678	-0.023	3.34	± 0.012

#### 3.2 Reading on wavelength- Chromium (Cr) at 357.9 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cr	0.1002	0.101	0.001	0.80	± 0.007
	0.3006	0.298	-0.003	0.86	± 0.012
	0.7014	0.635	-0.066	9.47	± 0.023

#### 3.3 Reading on wavelength- Copper (Cu) at 324.7 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cu	0.0502	0.046	-0.004	8.37	± 0.004
	0.3012	0.295	-0.006	2.06	± 0.010
	0.7028	0.694	-0.009	1.25	± 0.021

Continue 4 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE



Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governing body.

#### Head Office

35 Mu. 3 Tambon Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : mtc@istat.or.th Website: www.istat.or.th

#### Office/Laboratory

Sol. 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@istat.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 8392  
Fax. (66) 0 2579 8392  
E-mail : sumlee@istat.or.th

เอกสารไม่ควบคุม



Request No. 25-65 / 0398

4 / 5

MTC. ACL. No. 486 / 65

#### 3.4 Reading on wavelength- Iron (Fe) at 248.3 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Fe	0.1003	0.106	0.006	5.68	± 0.008
	0.5015	0.522	0.021	4.09	± 0.017
	1.0030	0.993	-0.010	1.00	± 0.032

#### 3.5 Reading on wavelength- Lead (Pb) at 217.0 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Pb	0.1988	0.197	-0.002	0.91	± 0.014
	0.6958	0.722	0.026	3.77	± 0.022
	1.4910	1.463	-0.028	1.88	± 0.041

#### 3.6 Reading on wavelength- Manganese (Mn) at 279.5 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Mn	0.04955	0.054	0.004	8.98	± 0.004
	0.29730	0.317	0.0197	6.63	± 0.006
	0.69370	0.682	-0.0117	1.69	± 0.012

Continue 5 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE



Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governing body.

#### Head Office

35 Mu. 3 Tambon Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : mtc@istat.or.th Website: www.istat.or.th

#### Office/Laboratory

Sol. 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@istat.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 8392  
Fax. (66) 0 2579 8392  
E-mail : sumlee@istat.or.th

เอกสารไม่ควบคุม



TISTR

Request No. 25-65 / 0398

5 / 5

MTC. ACL No. 486 / 65

3.7 Reading on wavelength- Nickel (Ni) at 232.0 nm.

Element	Standard Value of RM (mg/L)	Reading (mg/L)	Error of Measurement (mg/L)	Error of Measurement (%)	Uncertainty (mg/L)
Ni	0.099	0.102	0.003	3.03	± 0.007
	0.495	0.489	-0.006	1.21	± 0.010
	0.990	0.975	-0.015	1.52	± 0.020

3.8 Reading on wavelength- Zinc (Zn) at 213.9 nm.

Element	Standard Value of RM (mg/L)	Reading (mg/L)	Error of Measurement (mg/L)	Error of Measurement (%)	Uncertainty (mg/L)
Zn	0.050	0.050	0.000	0.00	± 0.012
	0.300	0.307	0.007	2.33	± 0.011
	0.700	0.660	-0.040	5.71	± 0.015

Remark : The reported uncertainty is an expanded uncertainty calculated using a coverage factor of 2 ( $k = 2$ ) which gives a level of confidence of approximately 95%

Calibrate

(Mr. Danai Srithongkum)

Approved by.....

(Mrs. Thiropaya Junvee Fortune)

Director of Analytical Chemistry Laboratory

Calibration date : 3 February 2022

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

**Head Office**  
35 Mu 3 Tambon Khlong Luang, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : nmp@tistr.or.th Website: www.tistr.or.th

**Office/Laboratory**  
Soi 1C, Bangso Industrial Estate, Sukhumvit Road,  
Amphoe Muang Changwat Samutprakan 10580, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtg@tistr.or.th

**Office**  
190 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel.  
Fax. (66) 0 2319 6362  
E-mail : sum@tistr.or.th

PHBLATC-002 Rev-4

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



National Food Institute, Ministry of Industry, Thailand

200/6 Soi 36, Arun Amarin Road, Bang Yi Khan, Suktanet, Bang Phai District, Bangkok 10700, Thailand  
Tel. +66 (0) 2425 8555 Fax. +66 (0) 2425 8556 Website: www.nfi.or.th E-mail: info@nfi.or.th

## Calibration Certificate

Certificate No.: 2201793-001-01

Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Address: 3 Soi Udomsuk 41, Sukhumvit Road,

Bangchack, Prakhantong, Bangkok 10260

Page 1 of 5

Equipment: pH Meter

Manufacturer: METTLER TOLEDO

Model: SevenEasy pH

Serial No.: 1231155210

ID No.: UIAF WAT 01012653

Order No.: 2201793

Operation No.: 2201793-001

Date of Receipt: 21 February 2022

Date of Calibration: 1 March 2022

Calibrated by

Mr.Pheraphat Tuanjit

Scientist

Approved by

1 March 2022

Date of Issue:

Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CO-009 Revision: 00 Date: 14-12-61







## Calibration Report

**Certificate No.:** 2202093-001-01  
**Equipment:** pH Meter  
**Resolution:** 0.01 pH : 1 mV  
**Manufacturer:** METTLER TOLEDO  
**Model:** SevenEasy pH  
**Serial No.:** 123053212  
**Type:** Bench top  
**ID No.:** UAE.WAS.0032553

Page 2 of 5

**Date of Calibration:** 16 March 2022  
**Location:** Chemical Calibration Laboratory, National Food Institute.  
**Environment Condition:** Ambient Temperature: ( 23.0 ± 1.5 ) °C  
**Condition of Equipment:** Good Condition  
**Condition of this Results of Calibration**

1. Calibration Method In house method: W-CC-002 based on direct measurement by using standard voltage calibrator and certified reference material (CRM)

2. Reference Standards / Certified Reference Material

Instruments	Serial / ID No.	Manufacturer	Certificate No.	Due Date
2.1 DC Voltage Calibrator	2709007	Fluke	SCL-21F-0687	24 June 2022
2.2 Digital Thermometer	2709007	Fluke	CC-640598-01	30 October 2022
2.3 Thermocouple probe	00044157H 003056	PCVPE	Q021-2787	10 November 2022

Certified Reference Material	Lot No.	Manufacturer	Ref ID	Expiry Date
2.4 pH buffer 4.008 Primary pH buffer Solution	780012	CPAchem	PH2161.5	21 November 2023
2.5 pH buffer 6.865 Primary pH buffer Solution	780013	CPAchem	PH2171.5	21 November 2023
2.6 pH buffer 10.01 Primary pH buffer Solution	780015	CPAchem	PH2201.5	21 November 2022
2.7 pH buffer 7.00 (Standard pH buffer Solution)	776840	CPAchem	PH1071.5	8 November 2022

3. This certification is traceable to The International System of Unit (SI Unit)

3.1 Instruments No.2.1	through	NSC-TIS-TIS 17025 Laboratory Accreditation of Calibration No.0075
3.2 Instruments No.2.2	through	NSC-TIS-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.3 Instruments No.2.3	through	NSC-TIS-TIS 17025 Laboratory Accreditation of Calibration No.0392
3.4 Certified Reference Material No. 2.4 to 2.6	traceable to	Primary measurement method- Harned cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.5 Certified Reference Material No. 2.7	traceable to	BIM RefN HI-7 LoIN 30.04.2020; BIM RefN HI-3 LoIN 28.05.2020; BIM RefN HI-8 LoIN 30.04.2020; BIM RefN HI-10 LoIN 28.05.2020. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025

4. This certificate was certified only for the instrument we calibrated.  
5. This result of calibration was found accurate as shown on date and place of calibration only.

เอกสารไม่ควบคุม

## Calibration Report

**Certificate No.:** 2202093-001-01  
**Equipment:** pH Meter  
**Resolution:** 0.01 pH : 1 mV  
**Manufacturer:** METTLER TOLEDO  
**Model:** SevenEasy pH  
**Serial No.:** 123053212  
**Type:** Bench top  
**ID No.:** UAE.WAS.0032553

Page 3 of 5

**Date of Calibration:** 16 March 2022  
**Calibration Results:** ( Manual Temperature Compensation at 25 °C )  
1. Calibration of pH Meter

Nominal pH	DC Voltage Standard (mV)	Average Indicator Reading		Uncertainty (± mV)	Coverage Factor (k)
		mV	pH		
0	414.117	414	0.00	0.58	2.00
2	285.511	286	2.00	0.58	2.00
4	177.462	178	4.00	0.58	2.00
6	55.159	59	6.00	0.58	2.00
7	-0.001	0	7.00	0.58	2.00
8	-55.159	-59	8.00	0.58	2.00
10	-177.463	-177	10.00	0.58	2.00
12	-285.512	-296	12.00	0.58	2.00
14	-414.119	-414	14.00	0.58	2.00

2. Calibration of pH Meter with Electrode ( Manual Temperature Compensation at 25 °C )

Equipment:	pH Electrode	Type:	Combined Electrode
Manufacturer:	METTLER TOLEDO	Model:	INLAB 500S
Serial No.:	9433943	ID No.:	N/A

Performance of Electrode system (Three-Point Calibration at pH4, pH7 and pH10)

Certified Value @25 °C (pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty (± pH)	Coverage Factor (k)
	pH	mV			
4.008	4.01	172	98.1	0.0071	2.00
6.865	6.87	6	-	0.0074	2.00
10.015	10.01	-175	97.4	0.0050	2.00
5.983	5.98	-3	-	0.0082	2.00

เอกสารไม่ควบคุม

## Calibration Report

**Certificate No.:** 2202093-001-01  
**Equipment:** Digital Thermometer with RTD (pH Meter)  
 Resolution: 0.1 °C Model: SevenEasy pH  
 Serial No.: 1230525212 ID No.: UAE WAS.0032553  
 Manufacturer: METTLER TOLEDO  
**Date of Calibration:** 16 March 2022

Page 4 of 5

**Location:** Chemical Calibration Laboratory, National Food Institute  
**Environment Condition:**  
 Ambient Temperature ( 23.0 ± 1.0 ) °C  
 Relative Humidity ( 50 ± 4 ) %

### Condition of this results of Calibration:

- Calibration Method :
  - In house method: WTE-025 by comparison with standard thermometer.
  - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
  - The temperature scale in use at this laboratory is the International Temperature scale of 1990 (ITS-90).
- Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1623	2118164	PSL-T 085164	24-Jun-22	TISTR
Platinum Resistance Thermometer (PRT)	5627A	877332			

Support Equipment: - Low Temperature Bath (ISCCAL-6), Model Europe 6 Plus Basic, SN. 3415922

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Cordition of Calibrated Item : Good
- Result of Calibration :
 

☒ Without adjustment
 ☐ After adjustment

## Calibration Report

**Certificate No.:** 2202093-001-01  
**Equipment:** Digital Thermometer with RTD (pH Meter)  
 Resolution: 0.1 °C Model: SevenEasy pH  
 Serial No.: 1230525212 ID No.: UAE WAS.0032553  
 Manufacturer: METTLER TOLEDO  
**Date of Calibration:** 16 March 2022

Page 5 of 5

### Calibration point: Calibration result:

- The probe was immersed in liquid bath or dry bath to a minimum depth of 120 mm.
- Description of probe model: N/A SN: N/A
- Dimension of probe: Diameter 3.5 mm, Length 135 mm.
- Sheath material: Stainless Steel

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.2	15.001	-0.2	0.099
35.2	35.002	-0.2	0.099
35.2	35.002	-0.2	0.099

Note : - UUC\* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k = 2, providing approximately 95 %.

----- End -----



# Calibration Report

**Certificate No.:** 2201793-001-01

**Equipment:** Digital Thermometer with RTD (pH Meter)

**Resolution:** 0.1 °C

**Model:** SevenEasy pH

**Serial No.:** 123155210

**ID No.:** UAE.WAT.010/2553

**Manufacturer:** METTLER TOLEDO

**Date of Calibration:** 1 March 2022

**Calibration point:** 15.0, 25.0 and 35.0 °C

**Calibration result:**

**Page 5 of 5**

\* The probe was immersed in liquid bath or dry bath to a minimum depth of 100 mm.

- Description of probe, model: N/A S/N: N/A

Dimension of probe: Diameter 4 mm, Length 100 mm.

Sheath material: Stainless Steel

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.1	15.006	-0.1	0.069
25.1	25.004	-0.1	0.069
35.1	35.003	-0.1	0.069



**Note**

- UUC\* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k=2, providing a level of confidence of approximately 95 %.

**End**


**Page 5 of 5**

# Accuracy Calibration Certificate

**Customer:**

**Company:** United Analyst and Engineering Consultant Co., Ltd.  
**Address:** 3 Soi Udom Suk 41, Sukhumvit Rd., Bang Chak  
**City:** Phra Khanong  
**Zip / Postal:** 10260  
**State / Province:** Bangkok  
**Order Number:**

**Contact:** Suwit Chotirok



4 811917 7884

## Weighing Device

**Manufacturer:** Mettler Toledo

**Model:** XSR205DU

**Serial No.:** C210685394

**Building:** N/A

**Floor:** 2

**Room:** Balance Room

**Instrument Type:**

**Asset Number:** UAE.WAO.0102565

**Terminal Model:** SRAT

**Terminal Serial No.:** C210685394

**Terminal Asset No.:** N/A

Range	Max Capacity	Readability (d)
1	81 g	0.00001 g
2	220 g	0.0001 g

## Procedure

**Calibration Guideline:** EURAMET cg-18 v 4.0 (11/2015)

**METTLER TOLEDO Work Instruction:** CPW002/20

This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.

The seriality/ span of the weighing instrument was adjusted before calibration with a built-in weight.

In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

	Temperature	Humidity
As Found	Start: 22.4 °C End: 22.4 °C	Start: 47.5 % End: 46.2 %

**As Found Calibration Date:** 05 May 2022

**As Left Calibration Date:** N/A

**Issue Date:** 05-May-2022


**Calibrator:**

**Approved Signatory:**


**Technical Manager / Head of Calibration Center**

## Measurement Results

### Repeatability

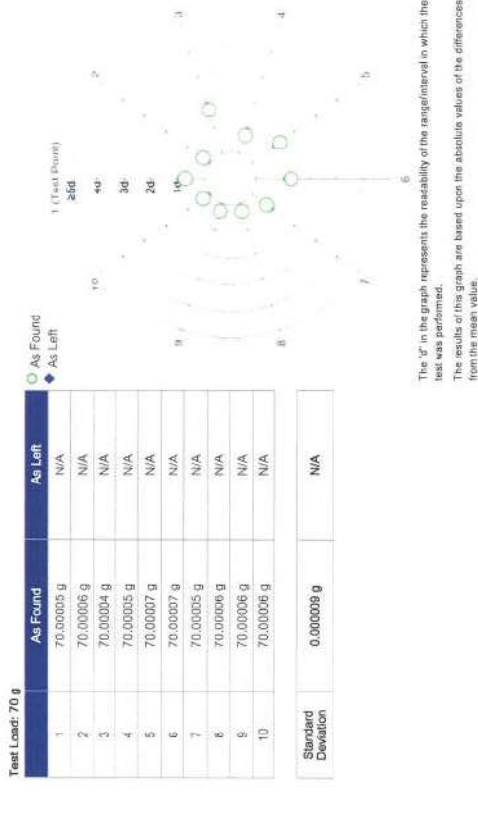

### Eccentricity

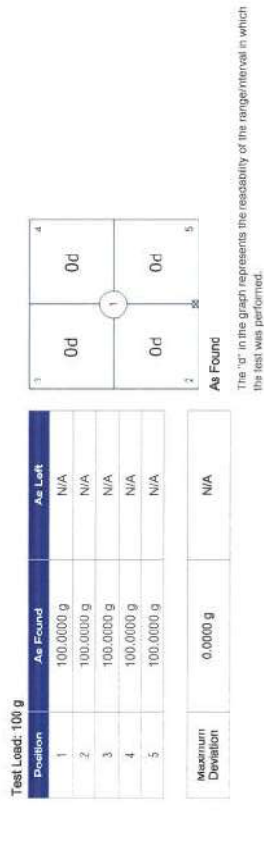

## Error of Indication



The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor k – which can be larger than 2 according to EURAMET cg-18. The value of the measurand lies within the assigned range of values with a probability of approximately 95%.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.

## Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML C2	
Weight Set No:	WS54
Certificate Number:	170240
Thermic Hygrometer:	
Equipment No:	IN161
Certificate Number:	21H1220
Date of Issue:	17-Nov-2020
Calibration Due Date:	15-Mar-2022
Date of Issue:	14-Jun-2021
Calibration Due Date:	01-Jun-2022

Remarks

- FACT adjustment functionality activated
- Equipment condition: Good
- Calibration after installation
- Next calibration according to customer's procedure
- Calibration data not decide by calibration laboratory

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with  $k=2$  in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value  $R$  represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use:  

1.5 · 10<sup>-7</sup> / K

Temperature range on site for the evaluation of the measurement uncertainty in use:  

3 K


Uncertainty of Uncertainty Equation

	Range d	Max	As Found		As Left	
			U <sub>1</sub> = 0.021 mg + 0.00450 mg/g · R	U <sub>2</sub> = 0.06 mg + 0.00448 mg/g · R	N/A	N/A
1	0.00001 g	81 g				
2	0.0001 g	220 g				

To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication		As Found		As Left	
0.00220 g		0.021 mg	0.95%	N/A	N/A
0.02200 g		0.021 mg	0.095%	N/A	N/A
0.22000 g		0.022 mg	0.0100%	N/A	N/A
2.20000 g		0.031 mg	0.0014%	N/A	N/A
220.0000 g		1.0 mg	0.00048%	N/A	N/A

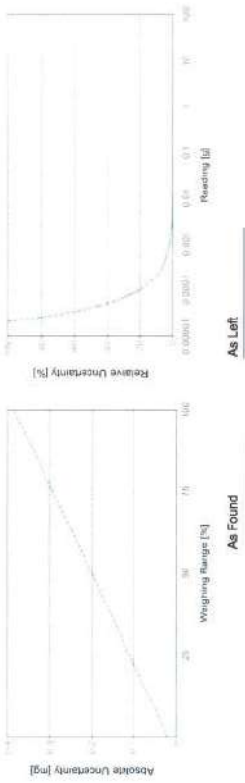

The weighing range shown in the absolute uncertainty graph refers to the first interval/average of the device.



GWP®

Certificate



As  
Found



As  
Left



The weighing device meets the given  
process requirements.

The weighing device meets the given  
process requirements.

Tests Performed: ☒ As Found ☐ As Left ☒ No adjustments/modifications made. As Left results correspond to As Found.


### Process Requirements

Weighing Tolerance: 0.5%

Smallest Net Weight: 0.05000 g

Safety Factor: 2

Safe Weighing Range

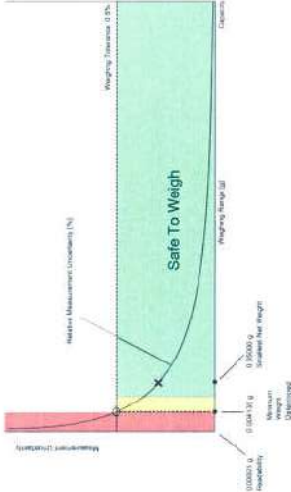

While the values in the graph reflect the actual calibration results, the measurement uncertainty curves are simply a visual representation. This graph reflects As Left testing, unless only As Found was performed.

เอกสารไม่ควบคุม

### Minimum Weight As Found Minimum Weight Table

Range 1

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.020748 g	0.041687 g	0.062816 g	0.105659 g	0.216300 g
0.2%	0.010351 g	0.020749 g	0.031195 g	0.052228 g	0.105659 g
0.5%	0.004135 g	0.008277 g	0.012427 g	0.020749 g	0.041687 g
1%	0.002067 g	0.004135 g	0.006205 g	0.010351 g	0.020749 g
2%	0.001033 g	0.002067 g	0.003100 g	0.005170 g	0.010351 g
5%	0.000413 g	0.000826 g	0.001240 g	0.002067 g	0.004135 g

The minimum weight table applies to the fine range of the weighing device.



Pass: The determined minimum weight meets the requirement for the smallest net weight.

### As Left Minimum Weight Table

Range 1

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.020748 g	0.041687 g	0.062816 g	0.105659 g	0.216300 g
0.2%	0.010351 g	0.020749 g	0.031195 g	0.052228 g	0.105659 g
0.5%	0.004135 g	0.008277 g	0.012427 g	0.020749 g	0.041687 g
1%	0.002067 g	0.004135 g	0.006205 g	0.010351 g	0.020749 g
2%	0.001033 g	0.002067 g	0.003100 g	0.005170 g	0.010351 g
5%	0.000413 g	0.000826 g	0.001240 g	0.002067 g	0.004135 g

The minimum weight table applies to the fine range of the weighing device.



Pass: The determined minimum weight meets the requirement for the smallest net weight.

At these net minimum weight values, the measurement uncertainty of the weighing device is equal to or less than 1/1 (no safety factor), 1/2, 1/3, 1/5, or 1/10 of the required tolerance. The values are calculated with  $k = 2$  and based on the linear formula of the measurement uncertainty of the weighing device in use.

The safety factor for As Found is always 1. This implies no safety factor. As Found testing looks at the behavior of the instrument from the past until test occurred. For the past, it is necessary to know that the tolerance was met, but not the safety factor. The safety factor is a proactive measure to apply for future measurements.

Notes on minimum weight values in above table:

1. If "N/A" is shown above, no appropriate value could be calculated.
2. METTLER TOLEDO is not responsible for the definition of the process requirements.

เอกสารไม่ควบคุม

## Measurement Results

### Results Summary

	As Found	Repeatability	Eccentricity	Error of Indication
	As Left	✓	✓	✓
	As Left	✓	✓	✓

✓ = Passed  
✗ = Failed  
⚠ = Safety Factor not met

### Repeatability

Test Load: 70 g

Tolerance	Control Limit	As Found	As Left
		Std. Deviation	Std. Deviation
0.1%	0.000025 g	Result	Result
0.2%	0.000050 g	✓	✓
0.5%	0.000125 g	✓	✓
1%	0.000250 g	0.000000 g	0.000000 g
2%	0.000500 g	✓	✓
5%	0.001250 g	✓	✓

The weighing tolerance is met if the standard deviation is less than or equal to the corresponding control limit.

### Eccentricity

Test Load: 100 g

Tolerance	Control Limit	As Found	As Left
		Deviation	Deviation
0.1%	0.0500 g	Result	Result
0.2%	0.1000 g	✓	✓
0.5%	0.2500 g	✓	✓
1%	0.5000 g	0.0000 g	0.0000 g
2%	1.0000 g	✓	✓
5%	2.5000 g	✓	✓

The weighing tolerance is met if the deviation is less than or equal to the corresponding control limit.

### Error of Indication

As Found

Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.00000 g	0.00000 g	N/A	N/A	N/A	N/A	N/A	N/A
20.00002 g	0.00000 g	0.01000 g	0.02000 g	0.05000 g	0.10000 g	0.20000 g	0.50000 g
50.00000 g	0.00002 g	0.02500 g	0.05000 g	0.12500 g	0.25000 g	0.50000 g	1.25000 g
80.00004 g	0.00005 g	0.04000 g	0.08000 g	0.20000 g	0.40000 g	0.80000 g	2.00000 g
100.00000 g	0.00000 g	0.05000 g	0.10000 g	0.25000 g	0.50000 g	1.00000 g	2.50000 g
150.00000 g	0.00000 g	0.07500 g	0.15000 g	0.37500 g	0.75000 g	1.50000 g	3.75000 g
200.00000 g	-0.00001 g	0.10000 g	0.20000 g	0.50000 g	1.00000 g	2.00000 g	5.00000 g
Result		✓	✓	✓	✓	✓	✓

As Left

Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.00000 g	0.00000 g	N/A	N/A	N/A	N/A	N/A	N/A
20.00002 g	0.00000 g	0.01000 g	0.02000 g	0.05000 g	0.10000 g	0.20000 g	0.50000 g
50.00000 g	0.00002 g	0.02500 g	0.05000 g	0.12500 g	0.25000 g	0.50000 g	1.25000 g
80.00004 g	0.00005 g	0.04000 g	0.08000 g	0.20000 g	0.40000 g	0.80000 g	2.00000 g
100.00000 g	0.00000 g	0.05000 g	0.10000 g	0.25000 g	0.50000 g	1.00000 g	2.50000 g
150.00000 g	0.00000 g	0.07500 g	0.15000 g	0.37500 g	0.75000 g	1.50000 g	3.75000 g
200.00000 g	-0.00001 g	0.10000 g	0.20000 g	0.50000 g	1.00000 g	2.00000 g	5.00000 g
Result		✓	✓	✓	✓	✓	✓

The weighing tolerance is met if the error (of indication) for each test point is less than or equal to the corresponding control limit for that particular weighing tolerance. Results at or close to the zero point cannot be assessed.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18 SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



MSC-T86-T817825  
CALIBRATION 0005

Cert. No.: 21TM1876  
Page.: 1 of 3

## Certificate of Calibration

**Equipment :** Hot Air Oven  
**Manufacturer :** Memmert  
**Model :** UF 55  
**Serial No. :** B216.1666  
**ID No. :** UAE WAO.027/2559  
**Submitted by :** United Analyst and Engineering Consultant Co., Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak Phrakhanong,  
Bangkok 10260  
**Location :** Lab Floor 2

**Received Order :** 29 October 2021  
**Calibration Date :** 29 October 2021  
**Ambient Temperature :** ( 26 ± 10 ) °C  
**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Kunchit Promrat  
**Approved by :** Approved Signatory

( ) Pornthippa Tamayakul  
( ) Malee Bulkrua  
( ) Suwit Imjai

**Issue Date :** 4 November 2021

The Uncertainties are for a confidence probability of approximately 95 %

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



**Equipment :** Hot Air Oven  
**Condition As-Received :** Used Item  
**Reference :** 2110-07010C-1

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard Instrument:-

**Instrument** **Model** **Serial No.** **Cert. No.** **Due Date**  
1 ) Data Acquisition 34970A MY44067817 21LM10 20 Jul 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	28	28
REL.Humid. ( % )	56	55
AC Supply ( Volt )	230	230



**Probe Installation Details :**

a = 5.0 cm  
b = 5.0 cm  
c = 5.0 cm  
D = 0.33 m  
W = 0.40 m  
H = 0.40 m  
Capacity = 0.053 m<sup>3</sup>

**Dimension of Chamber :**

Ref. Std. ID No.: @ Calibration Point	
Position : ( 140, 180 ) °C	( 104 ) °C
1	21-15TC-01 15RTD2/11
2	21-15TC-02 15RTD2/12
3	21-15TC-03 15RTD2/13
4	21-15TC-04 15RTD2/14
5	21-15TC-05 15RTD2/15
6	21-15TC-06 15RTD2/20
7	21-15TC-07 15RTD2/17
8	21-15TC-08 15RTD2/18
9 (ref.)	21-15TC-09 15RTD2/19

เอกสารไม่ควบคุม





**Equipment :** Hot Air Oven  
**Condition As-Received :** Used Item  
**Reference :** 2110-0701OC-1  
**Result of Calibration :-** (\*) Without Adjustment  
**Function of UUC\* :** Temperature Source  
**Fresh air setting :** Close

**Cert. No.:** 21TM1876  
**Page.:** 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
104.0	104.0	104.0	0.11	0.52	0.72	0.42	2
140.0	140.0	140.0	0.25	1.1	1.4	1.1	2
180.0	180.0	180.0	0.18	0.87	1.2	1.1	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	103.852	103.978	104.382	104.323	103.776	104.015	104.312	104.196	103.907
140.0	140.300	140.730	140.426	140.270	139.631	139.666	140.067	139.895	139.750
180.0	180.598	180.339	180.755	180.619	179.716	179.829	180.204	180.365	179.975

**Average\* :** The average of 30 values in each position.  
**Temperature stability :** One-half of the greatest maximum difference of measured temperature at any one sensor.  
**Temperature uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.  
**Overall Variation :** The Difference of the maximum and minimum measured temperatures throughout observation.  
**UUC\* :** Unit Under Calibration  
**Note :** The reported uncertainty of measurement was included stability and excluded uniformity .  
The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-000-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUKLUANG BANGKOK 10250  
TEL.0-2717-3000-23 FAX 0-2719-9484



**Cert. No.:** 22TM90  
**Page.:** 1 of 3

## Certificate of Calibration

**Equipment :** BOD Incubator  
**Manufacturer :** Arco  
**Model :** UC4-1320  
**Serial No. :** 13URC4S013201  
**ID No. :** UAE.WAO.015/2561

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10280  
**Location :** Lab Floor 2

**Received Order :** 17 February 2022  
**Calibration Date :** 17 February 2022  
**Ambient Temperature :** (26 ± 10 ) °C  
**Relative Humidity :** (50 ± 30 ) %

**Calibrated by :** Kunchit Promprat

**Approved by :**   
( ) Pornthippa Tameyakul  
( ) Malee Buikusa  
( ) Suwit Imjai

**Issue Date :** 22 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3. Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม  
A 0038099



Equipment : BOD Incubator  
Condition As-Received : Used Item  
Reference : 2202-04460C-1  
Procedure Used :-

Cert. No.: 22TM90  
Page.: 2 of 3

Calibration were conducted using calibration procedure CP-QT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).  
The temperature scale used was based on ITS-90.

#### Condition of this result of calibration

1. Reference standard instrument:-

Instrument Model Serial No. Cert. No. Due Date  
1 ) Data Acquisition 34970A MY44035217 21LM30 23 Dec 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- ( \* ) Without Adjustment

Function of UUC\* : Temperature Source

Fresh air setting : Not Available

Environment during calibration	
Beginning	Finished
Temp. ( °C )	28 28
REL.Humid. ( % )	68 75
AC Supply ( Volt )	226 226

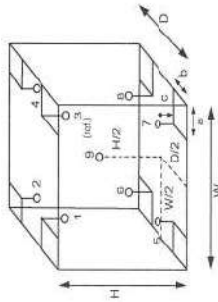

#### Probe Installation Details :

a = 10 cm  
b = 10 cm  
c = 10 cm

Dimension of Chamber :  
D = 0.62 m  
W = 1.2 m  
H = 1.2 m  
Capacity = 0.89 m<sup>3</sup>

Position :	Ref. Std. ID No.:
1	18-10RTD-01
2	18-10RTD-02
3	18-10RTD-03
4	18-10RTD-04
5	18-10RTD-05
6	22-10RTD-10
7	18-10RTD-07
8	18-10RTD-08
9 (ref.)	18-10RTD-09



Equipment : BOD Incubator  
Condition As-Received : Used Item  
Reference : 2202-04460C-1  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Not Available

Cert. No.: 22TM90  
Page.: 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( ± °C )	Coverage Factor k
20.0	19.5	19.4	0.30	0.58	1.0	0.55	2
Measured Temperature ( °C )							
Calibration Point ( °C )	Position						
20.0	1	2	3	4	5	6	7
	20.154	20.013	20.356	19.939	19.934	19.761	19.817
							8
							9 (ref.)
							19.922

Average\* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC\* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม  
a 1096042

เอกสารไม่ควบคุม  
a 1096041

## Calibration Certificate

**Certificate No.:** 2203120-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhonwong, Bangkok 10200

Page 1 of 3

**Equipment:** Electronic Balance  
**Manufacturer:** METTLER TOLEDO  
**Model:** AB204-S/FACT  
**Serial No.:** 1129361010  
**ID No.:** UAE-WAS.002/2552  
**Order No.:** 2203120

**Operation No.:** 2203120-001  
**Date of Receipt:** 1 June 2022  
**Date of Calibration:** 1 June 2022

**Calibrated by** Mr.Taveesak Seilee  
Scientist  
**Date of Issue:** 7 June 2022  
**Approved by**   
(Mr.Pieraprat Tuangjit)  
Manager, Division of Calibration Laboratory  
Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95%**  
This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-003 Revision: 01 Date: 20-04-65

## Calibration Report

**Certificate No.:** 2203120-001-01  
**Equipment:** Electronic Balance  
**Model:** AB204-S/FACT  
**Serial No.:** 1129361010  
**Capacity:** 220 g  
**Manufacturer:** METTLER TOLEDO  
**Resolution:** 0.0001 g  
**ID No.:** UAE-WAS.002/2552

Page 2 of 3

**Environment Condition:** Ambient Temperature: 19.9 ± 0.3 °C Relative Humidity: 45 ± 1.5 %

**Place of Calibration:** 108, Balance Room, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

**Condition of This Results of Calibration:**

1. Calibration Method: IFT Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	8308068554	TCS	M2010205	6 January 2023
Standard Weight Class E2	1-500g	8308068128	TCS	M2010215	6 January 2023

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	PONPE 490	NFLBTH 010718	Quality Reborn	QK22-0350	18 February 2023

3. This certification is traceable to SI UNIT

4. This certificate was verified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

**Calibration Results:**




**1. Repeatability of Reading:**

Nominal Value ( g )	Standard Deviation of Reading ( g )
100	0.00048
200	0.000952

**2. Off-Center Error:**

A mass of 50 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.

		
1 ( g )	2 ( g )	3 ( g )
4 ( g )	5 ( g )	6 ( g )
7 ( g )	8 ( g )	(Maximum Difference) ( g )
49.9999	49.9998	49.9999
49.9998	49.9998	49.9998
49.9999	49.9998	0.0001

F-CS-012 Revision: 01 Date: 20-04-65



# Calibration Report

**Certificate No.:** 2203120-001-01  
**Equipment:** Electronic Balance  
**Model:** AB204-S/FACT  
**Serial No.:** 1125061010  
**Capacity:** 220 g  
**Resolution:** 0.0001 g  
**ID No.:** UAE.WAS.00212552  
**Manufacturer:** METTLER TOLEDO

**Date of Calibration:** 1 June 2022

**Calibration Results:** (Continued)

**Calibration Range:** 0 - 200 g

**Calibration Adjustment:** Internal Calibration

### 3. Departure from Nominal Value:

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.0000	0.0000	0.0000	0.000088	2.00
0.01	0.01000	0.0100	0.0000	0.000088	2.00
0.05	0.05000	0.0499	0.0001	0.000088	2.00
0.1	0.10000	0.1000	0.0000	0.000088	2.00
0.2	0.20000	0.2000	0.0000	0.000088	2.00
0.5	0.50000	0.5000	0.0000	0.000088	2.00
1	1.00000	0.9999	0.0001	0.000088	2.00
2	2.00000	1.9999	0.0001	0.000089	2.00
5	5.00000	5.0000	0.0000	0.000089	2.00
10	9.99998	9.9999	0.0001	0.000092	2.00
20	19.99999	19.9999	0.0001	0.000094	2.00
50	49.99990	49.9999	0.0000	0.00012	2.00
70	69.99989	69.9998	0.0001	0.00014	2.00
100	100.00001	99.9999	0.0001	0.00017	2.00
150	149.99991	149.9997	0.0002	0.00022	2.00
200	200.00007	199.9998	0.0003	0.00030	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ ,  $t$  level of confidence of approximately 95 %.

-----End-----

f-CS-012 Revision: 01 Date: 20-04-65

# เอกสารไม่ควบคุม



Inflammation

ภาคผนวก ข-4

---

เอกสารอ้างอิงกฎหมายที่เกี่ยวข้อง

ประกาศกระทรวงสาธารณสุข

ฉบับที่ 61 (พ.ศ.2524)

เรื่อง น้ำบริโภคในภาชนะบรรจุที่ปิดสนิท

อาศัยอำนาจตามความในมาตรา 5 และมาตรา 6 (1)(2) และ (6) แห่งพระราชบัญญัติอาหาร

พ.ศ.2522 รัฐมนตรีว่าการกระทรวงสาธารณสุขออกประกาศไว้ ดังต่อไปนี้

ข้อ 1 ให้ออกเลิก

(1) ประกาศกระทรวงสาธารณสุข ฉบับที่ 20 (พ.ศ.2522) เรื่อง กำหนดน้ำบริโภคและเครื่องดื่มเป็นอาหารควบคุมเฉพาะและกำหนดคุณภาพหรือมาตรฐาน เงื่อนไข วิธีการผลิต และฉลาก ลงวันที่ 13 กันยายน พ.ศ.2522

(2) ประกาศกระทรวงสาธารณสุข ฉบับที่ 50 (พ.ศ.2523) เรื่อง แก้ไขเพิ่มเติมประกาศกระทรวงสาธารณสุข ฉบับที่ 20 (พ.ศ.2522) ลงวันที่ 18 มีนาคม พ.ศ.2523

ข้อ 2 ให้น้ำบริโภคในภาชนะบรรจุที่ปิดสนิทเป็นอาหารควบคุมเฉพาะ

ข้อ 3 น้ำบริโภคต้องมีคุณภาพหรือมาตรฐาน ดังต่อไปนี้

(1) คุณสมบัติทางฟิสิกส์

- (ก) สี ต้องไม่เกิน 20 อาเซนยูนิต
- (ข) กลิ่น ต้องไม่มีกลิ่น แต่ไม่รวมถึงกลิ่นคลอรีน
- (ค) ความขุ่น ต้องไม่เกิน 5.0 ซิลิกาสเกล
- (ง) ค่าความเป็นกรด-ด่าง ต้องอยู่ระหว่าง 6.5 ถึง 8.5

(2) คุณสมบัติทางเคมี

- (ก) ปริมาณสารทั้งหมด (Total Solid) ไม่เกิน 500.0 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
- (ข) ความกระด้างทั้งหมด โดยคำนวณเป็นแคลเซียมคาร์บอเนต ไม่เกิน 100.0 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร

- (ค) สารหนู ไม่เกิน 0.05 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
- (ง) แร่เยิ้ม ไม่เกิน 1.0 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
- (จ) แคดเมียม ไม่เกิน 0.01 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร

ความใน (ง) ถูกยกเลิกและใช้ความใหม่แทนแล้วโดยข้อ 1 แห่งประกาศกระทรวงสาธารณสุข ฉบับที่ 135

(พ.ศ.2534)

- (ฉ) คลอไรด์ โดยคำนวณเป็นคลอรีน ไม่เกิน 250.0 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
  - (ช) โครเมียม ไม่เกิน 0.05 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
  - (ช) ทองแดง ไม่เกิน 1.0 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
  - (ฌ) เหล็ก ไม่เกิน 0.5 มิลลิกรัมต่อหน่วยบริโภค 1 ลิตร
  - (ญ) ตะกั่ว ไม่เกิน 0.1 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
- ความใน (ฉ) และ (ญ) ถูกยกเลิกและใช้ความใหม่แทนแล้วโดยข้อ 2 แห่งประกาศกระทรวงสาธารณสุข

ฉบับที่ 135 (พ.ศ.2534)

- (ฎ) แอมโมเนีย ไม่เกิน 0.05 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
  - (ฏ) โปรท ไม่เกิน 0.002 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
  - (ฐ) ไนเตรท โดยคำนวณเป็นไนโตรเจน ไม่เกิน 4.0 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
  - (ฑ) ฟีนอล ไม่เกิน 0.001 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
  - (ฒ) ซีลีเนียม ไม่เกิน 0.01 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
  - (ณ) เงิน ไม่เกิน 0.05 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
  - (ด) ซัลเฟต ไม่เกิน 250.0 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
  - (ต) สังกะสี ไม่เกิน 5.0 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
  - (ถ) ฟลูออไรด์ โดยคำนวณเป็นฟลูออรีน ไม่เกิน 1.5 มิลลิกรัม ต่อหน่วยบริโภค 1 ลิตร
- มีความเพิ่มเติมเป็น (พ) (ธ) และ (ณ) ของ (2) โดยข้อ 3 แห่งประกาศ ฉบับที่ 135 (พ.ศ.2534)

(3) คุณสมบัติเกี่ยวกับจุลินทรีย์

- (ก) ตรวจพบแบคทีเรียชนิดโคลิฟอร์ม น้อยกว่า 2.2 ต่อหน่วยบริโภค 100 มิลลิลิตร โดยวิธี เอ็ม พี เอ็น (Most Probable Number)

(ข) ตรวจไม่พบแบคทีเรียชนิด อี.โคไล

(ค) ไม่มีจุลินทรีย์ที่ทำให้เกิดโรค

ข้อ 4 ภาชนะบรรจุที่บรรจุน้ำบริโภค ให้ปฏิบัติตามประกาศกระทรวงสาธารณสุขว่าด้วยเรื่อง ภาชนะบรรจุ และจะต้องมีลักษณะอย่างหนึ่งอย่างใด ดังต่อไปนี้ด้วย

(1) เป็นภาชนะบรรจุที่ต้องมีฝาหรือจุกปิด เมื่อใช้บรรจุจะต้องปิดสนิทหรือมีนิกโดยรอบระหว่างฝาหรือจุกกับขวดหรือภาชนะบรรจุ

(2) เป็นภาชนะบรรจุที่ปิดสนิทซึ่งไม่ใช้ภาชนะบรรจุตาม (1)

สิ่งที่ปิดสนิทหรือส่วนที่ปิดสนิทของภาชนะบรรจุตาม (1) และ (2) ต้องมีลักษณะที่เมื่อเปิดใช้ทำให้สิ่งที่ปิดสนิทหรือส่วนที่ปิดสนิทหรือภาชนะบรรจุนั้นเสียหาย



ข้อ 5 การแสดงฉลากของน้ำบริโภค ให้ปฏิบัติตามประกาศกระทรวงสาธารณสุขว่าด้วยเรื่อง

ฉลาก

ประกาศฉบับนี้ไม่กระทบกระเทือนถึงใบสำคัญการขึ้นทะเบียนตำรับอาหาร ซึ่งออกให้ตามประกาศกระทรวงสาธารณสุข ฉบับที่ 20 (พ.ศ.2522) เรื่อง กำหนดน้ำบริโภคและเครื่องดื่มเป็นอาหารควบคุมเฉพาะ และกำหนดคุณภาพหรือมาตรฐาน เงื่อนไข วิธีการผลิต และฉลาก ลงวันที่ 13 กันยายน 2522 ซึ่งได้แก้ไขเพิ่มเติมโดยประกาศกระทรวงสาธารณสุข ฉบับที่ 50 (พ.ศ.2523) เรื่อง แก้ไขเพิ่มเติมประกาศกระทรวงสาธารณสุข ฉบับที่ 20 (พ.ศ.2522) ลงวันที่ 18 มีนาคม พ.ศ.2523 และให้ผู้ที่ได้รับใบสำคัญการขึ้นทะเบียนตำรับอาหารตามประกาศกระทรวงสาธารณสุขดังกล่าว มาดำเนินการแก้ไขตำรับอาหารให้มีรายละเอียดถูกต้องตามประกาศฉบับนี้ ภายในเก้าสิบวันนับแต่วันนี้ประกาศนี้ใช้บังคับ

ประกาศฉบับนี้ให้ใช้บังคับตั้งแต่วันถัดจากวันประกาศในราชกิจจานุเบกษาเป็นต้นไป

ประกาศ ณ วันที่ 7 กันยายน พ.ศ.2524

ส. พิจิตรแก้ว

รัฐมนตรีว่ากระทรวงสาธารณสุข

(98 ร.จ. 52 ต.สนที่ 157 (ฉบับพิเศษ แผนกรากิจจาง) ลงวันที่ 24 กันยายน พ.ศ.2524)