



บริษัท ปตท. น้ำมันและการค้าปลีก จำกัด (มหาชน)

รายงานผลการปฏิบัติตามมาตรการป้องกันและแก้ไขผลกระทบสิ่งแวดล้อม
และมาตรการติดตามตรวจสอบผลกระทบสิ่งแวดล้อม

โครงการท่าเทียบเรือและคลังน้ำมันภูเก็ต

ระหว่างเดือนมกราคม-มิถุนายน พ.ศ. 2565

ภาคผนวก จ
ใบรับรองการสอบเทียบเครื่องมือ



Certificate of Calibration


Represent to Certificate of Calibration ,PTC/07/22071

Certificate No.:	PTC/07/22071	Page:	1 of 2
Equipment:	Digital Balance	Condition:	Normal
Manufacturer:	Sartorius	Serial No:	26207042
Model:	MSE224-100-DU	ID No:	BKK_EN0002
Type of Balance:	Single interval		



Customer: ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakarn 40 Phatthanakarn Rd.,
khwaeng Phatthanakarn, Khet Suan Luang, Bangkok 10250.

Environment Condition:	Temperature	21.5 °C	± 0.7 °C
	Humidity	61.8 %RH	± 4.7 %RH
	Air density	1.19	kg/m ³

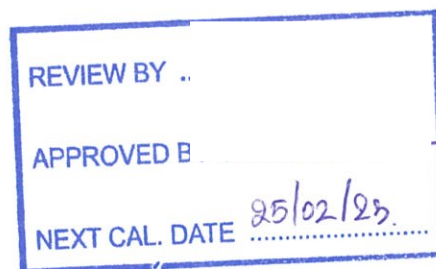

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakarn 40 Phatthanakarn Rd.,
khwaeng Phatthanakarn, Khet Suan Luang, Bangkok 10250.

The Method used: In house method, PTC-WI-07, base on Euramet cg. 18

Traceability: This certificate is traceable to the SI Units through Thai Calibration Service Co.,Ltd.
, NSC-ONSC Accreditation No.: Calibration 0189

Date Received: February 25, 2022

Calibration Date: February 25, 2022

Issued Date: March 01, 2022

Calibration By: Mr. Rungroje Metakul



PENTA CALIBRATION CO.,LTD

(Mr.Kriangsak Kalasri)

Reviewed by

Approved By :

(Mr. Keattisak Kerdto)

Laboratory Manager

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognised national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The effect that the results relate only to the items calibrated.

This calibration certificate shall not be reproduced except in full only, without written approval from penta calibration co., ltd



Represent to Certificate of Calibration ,PTC/07/22071

Certificate No.: PTC/07/22071



Page: 2 of 2

Measurement Results:

Without Adjustment :

Function Calibration: Non Adjustment

Eccentric Error: Weight to be 1/3 ,1/2 or of Maximum capacity

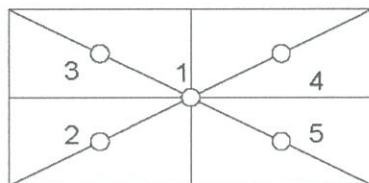

Eccentricity test 100 (g)

Position (g)				
1	2	3	4	5
0.0000	-0.0002	-0.0001	0.0001	-0.0001
Maximum deviation:			0.0002	

Repeatability Test : Weight to be $1/2 \leq L_1 \leq$ Maximum capacity

Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
200	0.00005

Error of indication : from nominal value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Indication (g)	Correction of Balance (g)	Uncertainty (g)	k
0	0.00000	0.0000	0.0000	0.00016	2.52
0.1	0.10000	0.1000	0.0000	0.00017	2.20
0.5	0.50000	0.5000	0.0000	0.00016	2.28
1	1.00001	1.0000	0.0000	0.00016	2.28
2	2.00001	2.0000	0.0000	0.00016	2.28
5	5.00001	5.0000	0.0000	0.00016	2.28
10	10.00002	10.0000	0.0000	0.00016	2.28
20	20.00002	20.0000	0.0000	0.00016	2.23
50	50.00001	50.0000	0.0000	0.00017	2.15
100	100.00002	99.9999	0.0001	0.00020	2.06
120	120.00004	120.0000	0.0000	0.00023	2.03
150	150.00003	150.0000	0.0000	0.00026	2.00
200	200.00003	199.9999	0.0001	0.00030	2.00

Note: Weight of adjust - (g)

The End of Certificate



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 21CH452
Page.: 1 of 3

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	SevenCompact S220
Serial No. :	B520948426
ID No. :	BKK_EN0072
Condition As-Received:	Used Item
Received Date :	24 March 2021
Calibration Date :	26 March 2021
Reference :	2103-1008DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer

REVIEW BY
APPROVED BY
NEXT CAL. DATE 24/9/22

Calibrated by : Warakorn Lernagatrakul

Approved by :

Approved Signatory

- (✓) Malee Butkruea
() Saithip Meangmai
() Warakorn Lernagatrakul

Issue Date : 31 March 2021

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0026590



Cert.No.: 21CH452

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	1385032	130RC022	20E4213	24 Nov 2021
2) Ref. Standard Thermometer	4982054	110RC044	20I1233	15 Oct 2021

This certification is traceable to the International System of Unit maintained at:-
- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	706694	06 Sep 2022
pH 6.985	CPA chem	722285	19 Dec 2021
pH 10.012	CPA chem	722287	19 Dec 2021

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: B520948426	4.000	177.48	177.4	4.000	0.058	2.00
	7.000	0.00	-0.1	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Malu.



Cert.No.: 21CH452

Page.: 3 of 3

Calibration Results**Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (\pm)	Coverage factor k
pH Electrode S/N.: 9265091	4.008	4.010	150.3	0.0048	2.05
	6.985	6.989	-22.5	0.0077	2.00
	10.012	10.011	-193.7	0.013	2.00

Function : Temperature Measurement**(*) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : InLab Expert Pro-ISM

- Serial No. : 9265091

Dimension of probe;

- Length : 120 mm.

- Diameter : 12 mm.

- Immersion Depth : 100 mm.

Calibration Point ($^{\circ}\text{C}$)	Standard Temperature ($^{\circ}\text{C}$)	UUC* Reading ($^{\circ}\text{C}$)	Error ($^{\circ}\text{C}$)	Uncertainty of measurement (\pm $^{\circ}\text{C}$)	Coverage factor k
25.0	25.003	25.2	0.197	0.20	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Malu.



บริษัท เอกเสคคิวทิฟ เทรดดิ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230
TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

ที่ RA 013/22

ใบรายงานผลการปรับเทียบ

ชื่อผู้ขอรับบริการ : บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด.
ที่อยู่ : 104 ซ.พัฒนาการ 40 ถ.พัฒนาการ แขวงสวนหลวง เขตสวนหลวง กรุงเทพมหานคร 10250.
ปรับเทียบที่ : บริษัท เอกเสคคิวทิฟ เทรดดิ้ง จำกัด
ที่อยู่ : 48/194-5 ซอย ประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวง/เขตลาดพร้าว กรุงเทพฯ 10230

รายละเอียดเครื่องมือที่ทำการปรับเทียบ :

เครื่องมือ : เครื่องตรวจวัดไอระเหยจากสารเคมี
ผลิตภัณฑ์ : RAE Systems
รุ่น : MiniRAE3000
หมายเลขเครื่อง : 592-906493
ID : BKK_FS0819

สภาวะแวดล้อม :

อุณหภูมิ : $(25 \pm 3) ^\circ\text{C}$
ความชื้นสัมพัทธ์ : $(36 \pm 15) \%$
ความดันบรรยากาศ : 760 มิลลิเมตรปรอท

วันที่ปรับเทียบมาตรฐาน : 4 กุมภาพันธ์ 2565

วิธีการปรับเทียบมาตรฐาน : ปรับเทียบโดยใช้ Standard Reference Gas ผลิตภัณฑ์ GASCO
- Isobutylene Standard Gas 100 ppm; Lot number: 304-402089381-1.

ผลการปรับเทียบมาตรฐาน

Sensor Type	Reference Concentration	Before Cal.	After Cal.	Error Reading	Result
PID	0.0 ppm (Air Zero)	0.0 ppm	0.0 ppm	0.0 ppm	Pass
PID	100 ppm (Isobutylene)	54.1 ppm	100.0 ppm	0.0 ppm	Pass

Flow Rate of Pump : 490 cc/min.

Accuracy : $\pm 2 \%$ at calibration point

ผู้ปรับเทียบ : ผู้ตรวจสอบ :

Service Engineer

Service Engineer Manager

ผลการสอบเทียบ/ปรับเทียบ นี้ รับรองเฉพาะตัวอย่างและรายการที่ได้รับระบุไว้เท่านั้น

การนำรายงานผล/ใบรับรองนี้ไปโฆษณาและการคัดลอกหรือการนำผลบางส่วนไปเผยแพร่ต่อสาธารณะต้องได้รับอนุญาตเป็นลายลักษณ์อักษรจากทางบริษัทฯ



บริษัท เอกเสคคิวทิฟเทรดดิ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230
TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

No. RA 013/22

Certificate of Calibration

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

Address : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang Bangkok 10250 TH.

Calibration location : Executive Trading Limited.

Address : 48/194-5 Soi Praditmanutham 19, Pradit Manutham Road, Latphrao, Bangkok 10230

Tools :

Instrument : Gas Detector

Product : RAE Systems

Model Name : MiniRAE3000

Serial Number : 592-906493

ID : BKK_FS0819

Environmental Condition :

Temperature : $(25 \pm 3) ^\circ\text{C}$

Relative Humidity : $(36 \pm 15) \%$

Pressure : 760 mmHg

Date of Calibration : February 4, 2022

Calibration Method : This instrument has been calibrated using calibration gases. Test and calibration data is On file with Executive trading limited.

Reference Standard : Isobutylene Standard Gas 100 ppm; Lot number: 304-402089381-1.

Test Result

Sensor Type	Reference Concentration	Before Cal.	After Cal.	Error Reading	Result
PID	0.0 ppm (Air Zero)	0.0 ppm	0.0 ppm	0.0 ppm	Pass
PID	100 ppm (Isobutylene)	54.1 ppm	100.0 ppm	0.0 ppm	Pass

Flow Rate of Pump : 490 cc/min.

Accuracy : $\pm 2 \%$ at calibration point

Calibrated By : _____

Approved By : _____

Service Engineer

Service Engineer Manager

The results relate only to the items tested or calibrated.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the company.



บริษัท เอกเสคคิวทิฟ เทรดดิ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230
TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

ที่ RA 013/22

ใบรายงานการตรวจเช็คเครื่องตรวจวัดก๊าซ รุ่น MiniRAE3000

หมายเลขเครื่อง : 592-906493

วันที่ตรวจเช็ค : 4 กุมภาพันธ์ 2565

ลำดับที่	รายละเอียด การตรวจสอบ	RAW COUNT		สรุป	หมายเหตุ
		REF.	REAL		
1.	PID RAW COUNT				
	Ch.H	10000-62500	39643	■ YES □ NO	
	Ch.L	<62500	29542	■ YES □ NO	
2.	Lamp	>40	45	■ YES □ NO	

ลำดับที่	รายละเอียด การตรวจซ่อม	การแก้ไข	สรุป	หมายเหตุ
1.	Motor Pump	Check flow rate	■ YES □ NO	490 cc/min.
2.	Buzzer	-	■ YES □ NO	-
3.	Li-ion Battery	-	■ YES □ NO	-
4.	Key Pad			
	Y/+	-	■ YES □ NO	-
	N/-	-	■ YES □ NO	-
	MODE	-	■ YES □ NO	-
5.	LCD Display	-	■ YES □ NO	-
6.	THP sensor	-	■ YES □ NO	-
7.	Light Sensor	-	■ YES □ NO	-
8.	Pocket Clip	-	□ YES □ NO	-
9.	PC Port	-	■ YES □ NO	-
10.	Slim Rubber Boot	-	■ YES □ NO	เปลี่ยนใหม่

ผู้ตรวจเช็ค :

(นายสุรินทร์ สายเนตร)

Service Engineer

ผลการสอบเทียบ/ปรับเทียบ นี้ รับรองเฉพาะตัวอย่างและรายการที่ได้รับอนุญาตไว้เท่านั้น

การนำรายงานผล/ใบรับรองนี้ไปโฆษณาและการคัดลอกหรือการนำผลบางส่วนไปเผยแพร่ต่อสาธารณะต้องได้รับอนุญาตเป็นลายลักษณ์อักษรจากทางบริษัทฯ



GASCO AFFILIATES, LLC.

320 Scarlet Blvd.
Oldsmar, FL 34677
(800) 910-0051
fax: (866) 755-8920
www.gascogas.com

CERTIFICATE OF ANALYSIS

Date: May 14, 2021
Order Number: 58376
Lot Number: 304-402089381-1

Customer: R C Systems Co Inc
Use Before: 05/14/2025

<u>Component</u>	<u>Requested Concentration</u>	<u>Analytical Result (+/- 2%)</u>
Isobutylene	100 PPM	101.2 PPM
Air	Balance	Balance

Cylinder Size: 3.70 Cu. Ft.
Contents: 105 Liter

Valve: 5/8"-18 UNF
Pressure: 1200 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/ or N.I.S.T. Gas Mixture reference materials.

Analyst: _____

Honeywell Analytics – Singapore Office
17 Changi Business Park Central 1
Singapore 486073
Cert Ref : 00317

Honeywell
THE POWER OF **CONNECTED**

Gas Detection



CERTIFICATE Of Attendance

It is hereby certified that

Mr Suttiwong Kongthongsang
(Executive Trading Limited)

has attended the

RAE Products & Maintenance Training Course

Conducted by

RAE Systems BY HONEYWELL

on **31st July to 2nd August 2018**



Conducted by : Desmond Tan
Service Engineer/Technical Trainer
Date of Issue : 2nd August 2018
Valid for 2 years from date of issue



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 21TM1693

Page.: 1 of 2

Certificate of Calibration

Equipment :	DO Meter With Sensor
Manufacturer :	YSI
Model :	Pro20
Serial No. :	17A102733
ID No. :	SGK_FS0052
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Songkhla Branch) 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru, A.Hat Yai, Songkhla 90250 Thailand
Location :	TPA On Site Calibration Laboratory
Received Order :	17 September 2021
Calibrated Date :	20 September 2021
Ambient Temperature :	(26 \pm 10) °C
Relative Humidity :	(50 \pm 30) %
AC Line Voltage :	(220 \pm 22) V
Calibrated by :	Preecha Hlahib
Approved by :	<div>REVIEW BY ..</div> <div>APPROVED B</div> <div>NEXT CAL. DATE 20/9/22</div>
	() Pornthippa Tameyakul
	(/) Malee Butkruea
	() Suwit Imjai
Issue Date :	22 September 2021

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0032176



Equipment : DO Meter With Sensor

Condition As-Received : Used Item

Reference : 2109-0705DSC-3

Cert. No.: 21TM1693

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1502A	A09204	201533	21 Dec 2021

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 487963

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (±°C)	<u>Coverage Factor</u> <i>k</i>
20.0	100	20.005	20.0	-0.005	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Maku .



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 21TW205

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	Pro20
Serial No. :	17A102733
ID No. :	SGK_FS0052
Received Date :	17 September 2021
Test Date :	21 September 2021
Reference :	2109-0705DSC-2
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru, A.Hat Yai, Songkhla 90250 Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	<div style="border: 1px solid black; height: 30px; width: 150px; margin: 0 auto;"></div> Approved Signatory
<input checked="" type="checkbox"/> Malee Butkruea <input type="checkbox"/> Saithip Meangmai <input type="checkbox"/> Warakorn Lerngagtrakul	
Issue Date :	22 September 2021



Cert.No.: 21TW205

Page.: 2 of 2

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 17A100388

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.14	8.09	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Mah.



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkhla 90250 Thailand

Tel: 081 599 0417 Fax: 074 805 133 Email: s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 8-Feb-2022

Certificate No. : 22EB149

CSR No. : A023/01123

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8 Karnchanawanich Rd. T.Ban Phru,
A. Hat Yai, Songkhla 90250 TH

Calibration Place : Chemical Laboratory

Instrument Name : Electronic Balance

Manufacturer : Sartorius

Model : MSE224S-100-DU

Serial No. : 34705158

ID No. : SGK_CL0045

Resolution : 0.0001 g

Received Date : 5-Feb-2022

Calibrated Date : 5-Feb-2022

Ambient Temperature : (30 ±10) °C

Relative Humidity : (50 ±20) %

REVIEW BY
APPROVED BY
NEXT CAL. DATE 5/02/2023

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.001 based on UKAS LAB 14 : 2015

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- Tcs : Thai Calibration Service Co.,Ltd.

Calibrated by : Imron Rattanaylum

Approved by :

Sakeereen Heemhad / Technical Manager

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.



Certificate No. : 22EB149

CSR No. : A023/01123

Page. : 2 of 3

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Weight Set	2mg-2kg	11119514/01	M2107051S	6-Jul-2022

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

1. Repeatability

Nominal Value (g)	Standard Deviation (g)
200	0.00000

2. Effect of tare

Nominal Value (g)	Standard Value (g)	Balance Reading (g)	Correction (g)
20	20.0000	20.0000	0.0000
40	40.0001	40.0000	0.0001
60	60.0000	60.0001	-0.0001
80	80.0001	80.0001	-0.0001
100	100.0000	100.0000	0.0000




Result of Calibration :

3. Off-centre loading

A mass approximately 50g was placed on a pan and moved to various position .

The balance reading obtained are given in the table.

Position					Maximum Difference (g)
1	2	3	4	5	
50.0000	50.0000	50.0000	50.0000	50.0000	0.0000



4. Departure from nominal value

Nominal Value (g)	Standard Value (g)	UUC Reading (g)	Correction (g)	Uncertainty (\pm g)	Coverage Factor (k)
0.01	0.0100	0.0100	0.0000	0.00008	2.0
0.1	0.1000	0.1000	0.0000	0.00008	2.0
0.5	0.5000	0.5000	0.0000	0.00008	2.0
1	1.0000	1.0000	0.0000	0.00008	2.0
2	2.0000	2.0000	0.0000	0.00008	2.0
5	5.0000	5.0000	0.0000	0.00009	2.0
10	10.0000	10.0000	0.0000	0.00009	2.0
20	20.0000	20.0000	0.0000	0.00009	2.0
50	50.0000	50.0000	0.0000	0.00011	2.0
100	100.0000	100.0000	0.0000	0.00016	2.0
120	120.0000	120.0000	0.0000	0.00024	2.0
140	140.0001	140.0000	0.0001	0.00024	2.0
160	160.0000	160.0000	0.0000	0.00026	2.0
180	180.0000	180.0000	0.0000	0.00029	2.0
200	200.0000	200.0000	0.0000	0.00030	2.0

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95%

...End...



CALIBRATION CERTIFICATE

Issued Date : 12-Nov-2021

Certificate No. : 21OV733

CSR No. : A012/00583

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8 Karnchanawanich Rd. T.Ban Phru,
A. Hat Yai, Songkhla 90250 TH

Calibration Place : Chemical Laboratory

Instrument Name : Hot Air Oven

Manufacturer : Memmert

Model : UF110

Serial No. : B416.3387

ID No. : SGK_CL0024

Resolution : 0.1 °C

Received Date : 9-Nov-2021

Calibrated Date : 9-Nov-2021

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY

APPROVED BY

NEXT CAL. DATE 10/05/2023

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on G-20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Ibrorhim Saleemin

Approved by :

Sakeereen Heemhad / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data logger With Sensor	34970A	MY44064411	QR21-0314	9-Feb-2022

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :.

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

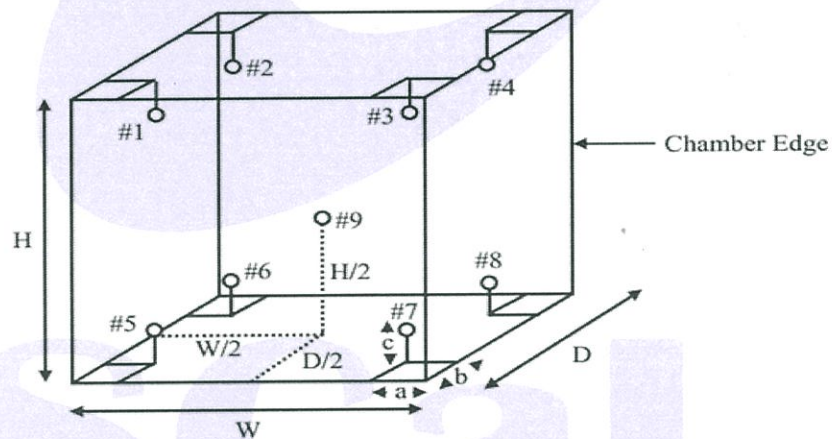

Sensor Installation Details

a = 5.0 cm

b = 5.0 cm

c = 5.0 cm

Dimension of the chamber

W = 40.0 cm

H = 40.0 cm

D = 33.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Hot Air Oven and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
40	39.85	39.81	39.68	39.57	39.94	39.80	39.81	39.93	39.69	0.36
70	70.53	70.23	70.08	69.74	70.51	70.37	70.43	69.79	70.15	0.36
103	103.47	102.96	102.95	102.77	103.40	103.46	103.33	102.73	102.83	0.36
104	104.47	103.92	103.95	103.77	104.33	104.46	104.30	103.73	103.80	0.36
105	105.34	104.85	104.85	104.67	105.16	105.27	105.07	104.81	105.06	0.36
180	180.04	180.03	179.99	179.86	180.11	180.28	180.27	180.16	180.26	0.41

3. Performance Result

The performance of the Hot Air Oven are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
40	40.0	40.0	0.10	0.34	0.47
70	70.0	70.0	0.10	0.48	0.82
103	103.0	103.0	0.10	0.71	0.74
104	104.0	104.0	0.10	0.71	0.74
105	105.0	105.0	0.20	0.39	0.70
180	180.0	180.0	0.20	0.53	0.62

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



CALIBRATION CERTIFICATE

Issued Date : 12-Nov-2021

Certificate No. : 21PH192

CSR No. : A012/00583

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8 Karnchanawanich Rd. T.Ban Phru,
A. Hat Yai, Songkhla 90250 TH

Calibration Place : Chemical Laboratory

Instrument Name : pH meter

Manufacturer : Mettler Toledo

Model : S220

Serial No. : B625631849

ID No. : SGK_CL0030

Electrode No. : 6404000

Received Date : 9-Nov-2021

Calibrated Date : 9-Nov-2021

Ambient Temperature : $(25 \pm 3) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \%$

REVIEW BY ..

APPROVED BY

CAL. DATE 10/05/2023

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HACH : LANGE United For Water Quality
- WK : WK Electric Co., Ltd.
- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Jessadagon Lemhud

Approved by :

Sakeereen Heemhad / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.005	C02840	1617	24-Aug-2022
Standard Solution	7.000	C02841	1618	24-Aug-2022
Standard Solution	10.012	C02843	1619	24-Aug-2022
Temperature/Electrical Calibrator	MC2-MF	23642	WK2102-006-229	21-Feb-2022
Digital Thermometer With Sensor	1529	B4C223	QR21-2009	15-Sep-2022

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :. (✓) Without Adjustment () After Adjustment

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading (mV)	Correction (mV)	Uncertainty (± mV)
177.48	177.5	-0.02	0.17
0.00	0.0	0.00	0.13
-177.48	-177.5	0.02	0.17

2. Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading (pH)	Correction (pH)	Uncertainty (± pH)
4.007	3.99	0.017	0.011
6.999	7.02	-0.021	0.014
10.011	10.01	0.001	0.036

3. Temperature Measurement

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25	24.93	25.0	-0.07	0.11

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CALIBRATION AND TESTING EQUIPMENT SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-24 FAX. 0-2719-9484

Cert.No.: 21CH1267

Page.: 1 of 2

Certificate of Calibration

Equipment :	Conductivity Meter
Manufacturer :	Mettler Toledo
Model :	Seven2GoS3
Serial No. :	B914464504
ID No. :	SGK_FS0051
Condition As-Received:	Used Item
Received Date :	17 September 2021
Calibration Date :	21 September 2021
Reference :	2109-0705DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru, A.Hat Yai, Songkhla 90250 Thailand
Ambient Temperature :	(25 \pm 2.5) °C
Relative Humidity :	(50 \pm 15) %
Calibration Procedure:	In -house method : - CP-CH6 : based on direct measurement by using reference material (RM)
Calibrated by :	Walalak Sirithean

Approved by :

(☒) Malee Butkruea
() Saithip Meangmai
() Warakorn Lernagtrakul

Approved Signatory

Issue Date :

22 September 2021

The Uncertainties are for a confidence probability of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration and Testing Equipment Services.

A 0007589



Cert.No.: 21CH1267

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	9549224	130RC003	21I451	15 Apr 2022

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835
- Conductivity calibration solution, Thermo Scientific (traceable to NIST)

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
84.001 $\mu\text{S/cm}$	CPA chem	725921	12 Jan 2022
1413 $\mu\text{S/cm}$	Thermo Scientific	081/02	26 Feb 2024
12.88 mS/cm	Thermo Scientific	230/01	07 June 2023

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results**Function : Conductivity Measurement**(*) After Adjustment at 1413 $\mu\text{S/cm}$

Conductivity Electrode Serial No.: 5819080541

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (\pm)	Coverage factor k
84.001 $\mu\text{S/cm}$	84.78 $\mu\text{S/cm}$	84.97 $\mu\text{S/cm}$	0.58 $\mu\text{S/cm}$	2.00
1413 $\mu\text{S/cm}$	1407 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	15 $\mu\text{S/cm}$	2.00
12.88 mS/cm	12.52 mS/cm	12.71 mS/cm	0.14 mS/cm	2.00

Remark

- UUC* = Unit Under Calibration

- Cell constant = 0.551 cm^{-1}

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Malu

a 1073158



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CH99

Page.: 1 of 3

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	S2Field Kit
Serial No. :	B731459205
ID No. :	SGK_FS0019
Condition As-Received:	Used Item
Received Date :	19 January 2022
Calibration Date :	20 January 2022
Reference :	2201-0586DSC-3
Submitted by :	ALS Laboratory Group (Thailand)Co.,Ltd. Songkhla Branch. 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru, A.Hat Yai, Songkhla 90250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	<div>Approved Signatory</div>
() Malee Butkruea	
() Saithip Meangmai	
(✓) Ponpan Paipim	
Issue Date :	31 January 2022



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 22CH99

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	21E2682	25 Aug 2022
2) Ref. Standard Thermometer	4982054	110RC044	21I1201	26 Oct 2022

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	766820	23 Sep 2023
pH 6.982	CPA chem	761017	02 Aug 2022
pH 10.015	CPA chem	766824	04 Sep 2022

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: B731459205	4.00	177.48	177	4.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-177	10.00	0.58	2.00

R2



Cert.No.: 22CH99

Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (\pm)	Coverage factor k
pH Electrode S/N.: 8111906	4.008	4.01	189	0.0079	2.00
	6.982	6.98	15	0.0099	2.00
	10.015	10.02	-160	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : InLab Expert Go-ISM
- Serial No. : 8111906

Dimension of probe;

- Length : 120 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point ($^{\circ}\text{C}$)	Standard Temperature ($^{\circ}\text{C}$)	UUC* Reading ($^{\circ}\text{C}$)	Error ($^{\circ}\text{C}$)	Uncertainty of measurement (\pm $^{\circ}\text{C}$)	Coverage factor k
25.0	25.002	25.2	0.198	0.13	2.00
45.0	45.002	45.3	0.298	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 21TM331

Page.: 1 of 3

Certificate of Calibration

Equipment :	Incubator
Manufacturer :	Memmert
Model :	ICP 750
Serial No. :	F816.0063
ID No. :	SGK_CL0028
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch 114/1 Moo 8 Kanjanavanij Rd., Banphru, Hatyai, Songkhla 90250 Thailand
Location :	BOD Room
Received Order :	10 February 2021
Calibration Date :	11 February 2021
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Khit Ruttanaprapachai
Approved by :	<div style="border: 1px solid black; width: 100px; height: 30px; margin: 0 auto;"></div> Approved Signatory
	() Pornthippa Tameyakul (<input checked="" type="checkbox"/>) Malee Butkruea () Suwit Imjai
Issue Date :	19 February 2021

REVIEW BY
APPROVED BY
NEXT CAL. DATE	12/8/22

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0024671



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2102-0248OC-3

Cert. No.: 21TM331

Page.: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	20LM6	NIST, NIMT	20 Apr 2021

2. This certification is traceable to the SI unit.

3. This certificate is valid only to the item calibrated on date and place of calibration.


Remark : NIST : National Institute of Standards and Technology, The United State of America.

NIMT : National Institute of Metrology Thailand.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

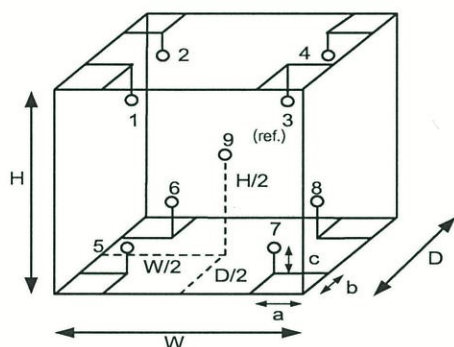

Environment during calibration		
	Beginning	Finished
Temp. (°C)	21	22
REL.Humid. (%)	46	48
AC Supply (Volt)	220	221

Position :	Ref. Std./ID No.:
1	20-16RTD-01
2	20-16RTD-02
3	20-16RTD-03
4	20-16RTD-04
5	20-16RTD-05
6	20-16RTD-06
7	20-16RTD-07
8	20-16RTD-08
9 (ref.)	20-16RTD-09

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.60 m
W = 1.0 m
H = 1.2 m
Capacity = 0.72 m³

Malu



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2102-0248OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 21TM331

Page.: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
20.0	20.0	20.0	0.10	0.32	0.62	0.30	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
20.0	20.294	20.186	20.327	20.313	20.058	20.105	20.008	19.863	20.109

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Maha .



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 21TW256

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter	<div>REVIEW BY</div> <div>APPROVED BY</div> <div>NEXT CAL. DATE <u>2/12/2022</u></div>
Manufacturer :	YSI	
Model :	5000	
Serial No. :	17B101473	
ID No. :	SGK_CL0073	
Received Date :	01 December 2021	
Test Date :	02 December 2021	
Reference :	2112-0025DSC-1	
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru, A.Hat Yai, Songkhla 90250 Thailand	
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %	
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method	
Tested by :	Walalak Sirithean	
Approved by :	<div>_____ Approved Signatory</div> <div>(/) Malee Butkruea () Saithip Meangmai () Warakorn Lernagatrakul</div>	
Issue Date :	6 December 2021	



Cert.No.: 21TW256

Page.: 2 of 2

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 17B100103

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.12	8.11	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Malu.

a 1084082



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 21LM26

Page.: 1 of 2

Certificate of Calibration

Equipment :	DO Meter with Sensor	<div>REVIEW BY ...</div> <div>APPROVED BY</div> <div>NEXT CAL. DA</div>
Manufacturer :	YSI	
Model :	5000	
Serial No. :	17B101473	
ID No. :	SGK_CL0073	
Submitted by :	ALS Laboratory Group (Thailand)Co.,Ltd. Songkhla Branch 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phur, A.Hat Yai, Songkhla 90250 Thailand	
Location :	On Site Calibration Service Laboratory	
Received Order :	1 December 2021	
Calibrated Date :	6 December 2021	
Ambient Temperature :	(26 ± 10) °C	
Relative Humidity :	(50 ± 30) %	
AC Line Voltage :	(220 ± 22) V	
Calibrated by :	Man Pattananonnnaiaboon	
Approved by :	<div>Approved Signatory</div> <div>(/) Pornthippa Tameyakul</div> <div>(✓) Malee Butkruea</div> <div>() Suwit Imjai</div>	
Issue Date :	9 December 2021	

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0032821



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2112-0025DSC-1

Cert. No.: 21LM26

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1502A	A52847	21I1144	20 Oct 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 17B100103

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.001	19.96	-0.041	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Mala



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 21TW256

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter	<div>REVIEW BY APPROVED BY ... NEXT CAL. DATE 2/12/2022</div>
Manufacturer :	YSI	
Model :	5000	
Serial No. :	17B101473	
ID No. :	SGK_CL0073	
Received Date :	01 December 2021	
Test Date :	02 December 2021	
Reference :	2112-0025DSC-1	
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru, A.Hat Yai, Songkhla 90250 Thailand	
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %	
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method	
Tested by :	Walalak Sirithean	
Approved by :	<div>Approved Signatory</div> (/) Malee Butkruea () Saithip Meangmai () Warakorn Lerngagtrakul	
Issue Date :	6 December 2021	



Cert.No.: 21TW256

Page.: 2 of 2

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 17B100103

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.12	8.11	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Malu.

a 1084082



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 21LM26

Page.: 1 of 2

Certificate of Calibration

Equipment :	DO Meter with Sensor	<div>REVIEW BY</div> <div>APPROVED BY</div> <div>NEXT CAL DATE <u>8/12/2021</u></div>
Manufacturer :	YSI	
Model :	5000	
Serial No. :	17B101473	
ID No. :	SGK_CL0073	
Submitted by :	ALS Laboratory Group (Thailand)Co.,Ltd. Songkhla Branch 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phur, A.Hat Yai, Songkhla 90250 Thailand	
Location :	On Site Calibration Service Laboratory	
Received Order :	1 December 2021	
Calibrated Date :	6 December 2021	
Ambient Temperature :	(26 ± 10) °C	
Relative Humidity :	(50 ± 30) %	
AC Line Voltage :	(220 ± 22) V	
Calibrated by :	Man Pattanapongpaiboon	
Approved by :	<div>Approved Signatory</div> <div>(/) Pornthippa Tameyakul</div> <div>(✓) Malee Butkruea</div> <div>() Suwit Imjai</div>	
Issue Date :	9 December 2021	

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0032821



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2112-0025DSC-1

Cert. No.: 21LM26

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1502A	A52847	21I1144	20 Oct 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 17B100103

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.001	19.96	-0.041	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Mala

a 1085890



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CALIBRATION AND TESTING EQUIPMENT SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-24 FAX. 0-2719-9484

Cert.No.: 21CH744

Page.: 1 of 2

Certificate of Calibration

Equipment :	Conductivity Meter
Manufacturer :	Mettler Toledo
Model :	Seven2Go TM Conductivity S3
Serial No. :	B914464506
ID No. :	SGK_FS0050
Condition As-Received:	Used Item
Received Date :	04 June 2021
Calibration Date :	08 June 2021
Reference :	2106-0171DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8 , Kanjanavanij Rd., Banphru , Hatyai, Songkhla 90250, Thailand
Ambient Temperature :	(25 \pm 2.5) °C
Relative Humidity :	(50 \pm 15) %
Calibration Procedure:	In -house method : - CP-CH6 : based on direct measurement by using certified reference material (CRM)
Calibrated by :	Uthen Kankawi
Approved by :	_____ Approved Signatory
(<input checked="" type="checkbox"/>) Malee Butkruea	
(<input type="checkbox"/>) Saithip Meangmai	
(<input type="checkbox"/>) Warakorn Lerngagtrakul	
Issue Date :	15 June 2021

REVIEW BY
APPROVED BY
NEXT CAL. DATE	8/6/22

The Uncertainties are for a confidence probability of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration and Testing Equipment Services.

A 0006943



Cert.No.: 21CH744

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	9549224	130RC003	211451	15 Apr 2022

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials :-

- Conductivity calibration solution, Thermo Scientific (traceable to NIST)

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
84 $\mu\text{S/cm}$	Thermo Scientific	081/02	23 Feb 2022
1413 $\mu\text{S/cm}$	Thermo Scientific	081/02	26 Feb 2022
12.88 mS/cm	Thermo Scientific	230/01	07 June 2023

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results**Function : Conductivity Measurement**

(*) After Adjustment at 1413 $\mu\text{S/cm}$

Conductivity Electrode Serial No.: 5819060890

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (\pm)	Coverage factor k
84 $\mu\text{S/cm}$	84.39 $\mu\text{S/cm}$	84.47 $\mu\text{S/cm}$	4.3 $\mu\text{S/cm}$	2.00
1413 $\mu\text{S/cm}$	1397 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	15 $\mu\text{S/cm}$	2.00
12.88 mS/cm	12.61 mS/cm	12.84 mS/cm	0.14 mS/cm	2.00

Remark

- UUC* = Unit Under Calibration

- Adjustment Cell constant = 0.550 cm^{-1}

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

Malu



บริษัท ดับเบิล เอส ไดแอกโนสติกส์ จำกัด
DOUBLE S DIAGNOSTICS CO., LTD.

4 ซอยอุดมสุข 14 แขวงบางนา เขตบางนา กรุงเทพฯ 10260 โทรศัพท์: (02) 747-7009 โทรสาร: (02) 747-7008
4 Soi Udomsuk 14, Bangna, Bangkok 10260 Tel. (02) 747-7009 Fax: (02) 747-7008

Maintenance Plan YEAR : 2021

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
รวม						10/10/21 OK						10/10/21 OK

Periodical maintenance check list for Konelab

	6M	12M	Note!
1.Diluent-wash tubing change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
2.ISE tubing change	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
3.Syringe check/change		<input checked="" type="checkbox"/>	
4.Dispensing check/ change		<input checked="" type="checkbox"/>	
5.Waste tubing change when necessary		<input checked="" type="checkbox"/>	
6.Lamp check/change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
7.Mixer paddle/paddle change(not Konelab20)		<input checked="" type="checkbox"/>	
8.ISE needles check/change		<input checked="" type="checkbox"/>	
9.Pump tubing check/ chance	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
10.Broken/worn out part check /change		<input checked="" type="checkbox"/>	
11.Peristaltic pump check /cleaning/ lubrication	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
12.Heating check		<input checked="" type="checkbox"/>	
13.Cooling check		<input checked="" type="checkbox"/>	
14.Dispenser mechanic check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
15.Cuvette transfer mechanic check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
16.Dispenser movement check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
17.Sample/reagent register check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
18.Dispensing tubing tightness check	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
19.Photometer and optics cleaning/check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
20.Workstation PC cleaning if necessary	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
21.Mechanic cleaning/lubrication	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
22.Instrument cleaning if necessary	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
23.Complete analyzer testing with waterblank/QC or sample	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
24.Test parameters/Adjustment/config. Save to USB key	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
25.UPS Test	<input type="checkbox"/>	<input checked="" type="checkbox"/>	

Place: ALS Lab Instrument: Aquakem 950
Date/Time: 28-06-21 Serial no: 22781
Service done by: [Signature] Install date:
Signature of customer: [Signature] Date/Time: 28/6/21



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM101

Page.: 1 of 3

Certificate of Calibration

Equipment :	Autoclave
Manufacturer :	Sanyo
Model :	MLS-3781
Serial No. :	830167
ID No. :	BKK_ML0037
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Media Preparation Room
Received Order :	21 January 2022
Calibration Date :	21 January 2022
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Krisda Malee

Approved by :

Approved Signatory

- (☒) Pornthippa Tameyakul
(☒) Malee Butkruea
(☐) Suwit Imjai

Issue Date :

3 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0037379



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2201-0616OC-3

Cert. No.: 22TM101

Page.: 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Data Acquisition	34972A	MY57013711	21LM7	16 Jun 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**


(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)

It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

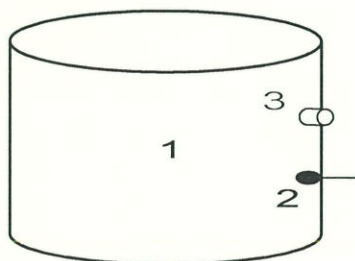

	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	27	57	220
Finished of Calibration	26	59	221

<u>Position</u>	<u>Description</u>	<u>Ref. Std. ID No.:</u>
1 =	Center of chamber	18-18TC-01
2 =	Temperature sensor	18-18TC-02
3 =	Exhaust port	18-18TC-03

Malu



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2201-0616OC-3

Cert. No.: 22TM101

Page.: 3 of 3

Result of Calibration :- (*) Without Adjustment

Operating parameter Set : Temperature = 108 °C

Sterilization period = 15 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
108	108	1	108.044	0.29	0.040	0.94	2
		2	108.133				
		3	108.142				

Operating parameter Set : Temperature = 121 °C

Sterilization period = 15 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
121	121	1	121.082	0.21	0.11	0.91	2
		2	121.068				
		3	121.128				

Average* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM102

Page.: 1 of 3

Certificate of Calibration

Equipment : Incubator
Manufacturer : SHEL-LAB
Model : 1915A
Serial No. : 0200599
ID No. : BKK_ML0010
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Location : Incubation & Micrological Reading
Received Order : 21 January 2022
Calibration Date : 21 January 2022
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Krisda Malee

REVIEW BY

APPROVED BY

NEXT CAL. DATE 22/07/22

Approved by :

Approved Signatory

() Pornthippa Tameyakul
() Malee Butkruea
() Suwit Imjai

Issue Date :

3 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0037377



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2201-0616OC-1

Cert. No.: 22TM102

Page.: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY57013711	21LM7	16 Jun 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

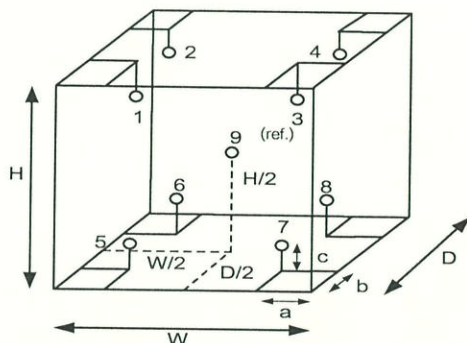

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	25
REL.Humid. (%)	53	54
AC Supply (Volt)	220	221

Position :	Ref. Std. ID No.:
1	18-18RTD-01
2	18-18RTD-02
3	18-18RTD-03
4	18-18RTD-04
5	18-18RTD-05
6	18-18RTD-06
7	18-18RTD-07
8	18-18RTD-08
9 (ref.)	18-18RTD-09

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.90 m
W = 0.75 m
H = 1.2 m
Capacity = 0.81 m³

Maku .



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2201-0616OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 22TM102

Page.: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
35.0	35.0	35.0	0.043	0.41	0.42	0.30	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
35.0	34.801	34.868	34.862	35.012	35.040	35.010	35.084	35.040	35.178

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 21TM1101

Page.: 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Binder

Model : ED240/E2

Serial No. : 00-15533

ID No. : BKK_ML0013

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 7 June 2021
Calibration Date : 7 June 2021
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Preecha Hlahib

REVIEW BY
APPROVED BY
NEXT CAL. DATE 6/12/22

Approved by :

Approved Signatory

- () Pornthippa Tameyakul
(/) Malee Butkruea
() Suwit Imjai

Issue Date :

21 June 2021

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0029135



Equipment : Hot Air Oven
 Condition As-Received : Used Item
 Reference : 2106-0101OC-2

Cert. No.: 21TM1101
 Page.: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY57013823	21LM3	26 Feb 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

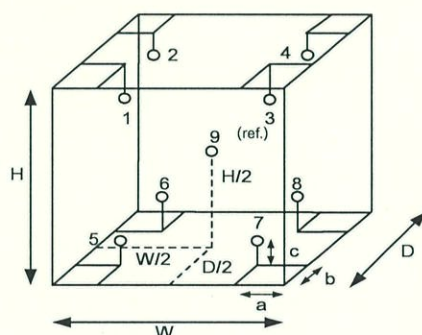

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	27
REL.Humid. (%)	65	72
AC Supply (Volt)	220	222

Position :	Ref. Std. ID No.:
1	19-17TC-01
2	19-17TC-02
3	19-17TC-03
4	19-17TC-04
5	19-17TC-05
6	19-17TC-06
7	19-17TC-07
8	19-17TC-08
9 (ref.)	19-17TC-09

Probe Installation Details :

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of Chamber :

D = 0.50 m
 W = 0.80 m
 H = 0.60 m
 Capacity = 0.24 m³

make



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2106-0101OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 21TM1101
Page.: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
180	180	180	0.67	2.4	3.3	1.5	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
180	179.315	181.249	178.684	180.035	179.941	180.511	178.429	180.268	179.065

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-000-

Maku



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM453

Page.: 1 of 3

Certificate of Calibration

Equipment :	Water Bath
Manufacturer :	Memmert
Model :	WB 45
Serial No. :	I704.0285
ID No. :	BKK_ML0052
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Incubation & Microbiological Reading
Received Order :	21 February 2022
Calibration Date :	21 February 2022
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Prawit Sodavitchit

REVIEW BY

APPROVED BY

NEXT CAL. DATE 21/2/23

Approved by :

Approved Signatory

- () Pornthippa Tameyakul
(/) Malee Butkruea
() Suwit Imjai

Issue Date :

25 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0038346



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2202-0615OC-2

Cert. No.: 22TM453

Page.: 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44035217	21LM30	23 Dec 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	51	220
Finished of Calibration	25	50	220

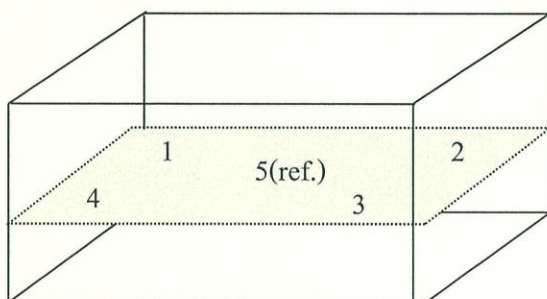

Front

Position :	Ref. Std. S/N.:
1	N37P300726
2	N37P300727
3	N37P300728
4	N37P300729
5(ref.)	N37P300730

Malu



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2202-0615OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 22TM453

Page.: 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)				
			Position				
			1	2	3	4	5 (ref.)
44.5	45.1	45.1	44.503	44.454	44.497	44.519	44.476

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
44.5	0.13	0.063	0.15	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T220133I01 "Substitute for Calibration Certificate Number T220133" Page 1 of 5

Certificate of Calibration

Equipment : Digestion Unit

Manufacturer : Environmental Express

Model : TKN100

Serial No. : 2017TKNBC142

Customer Code : BKK_EN0223

ID No. : T6773A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab1

Date of Receipt : 26 January 2022

Calibrated By : Watcharapon Sangtong (Technician)

Approved By : _____ / Sujjar Naknakred (Site Calibration Manager)

Date of Issue : 20 FEB 2022

REVIEW BY
APPROVED BY
NEXT CAL. DATE <u>1/2/23</u>

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T220133I01

Page 2 of 5

Calibration Report

Equipment : Digestion Unit
Date of Calibration : 1 February 2022
Environment : Temperature : 23.9 - 26.3 °C
Line Voltage : 221.4 - 225.1 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T10.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M20A1-(CH17-CH20)	T210011	14 March 2022
DATA LOGGER	34970A	T149	T210011	14 March 2022

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 2 Hour 1 Minute At 380 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

(X) without adjustment


() after adjustment

Approved By. _____

Certificate No. T220133I01

Page 3 of 5

Calibration Report

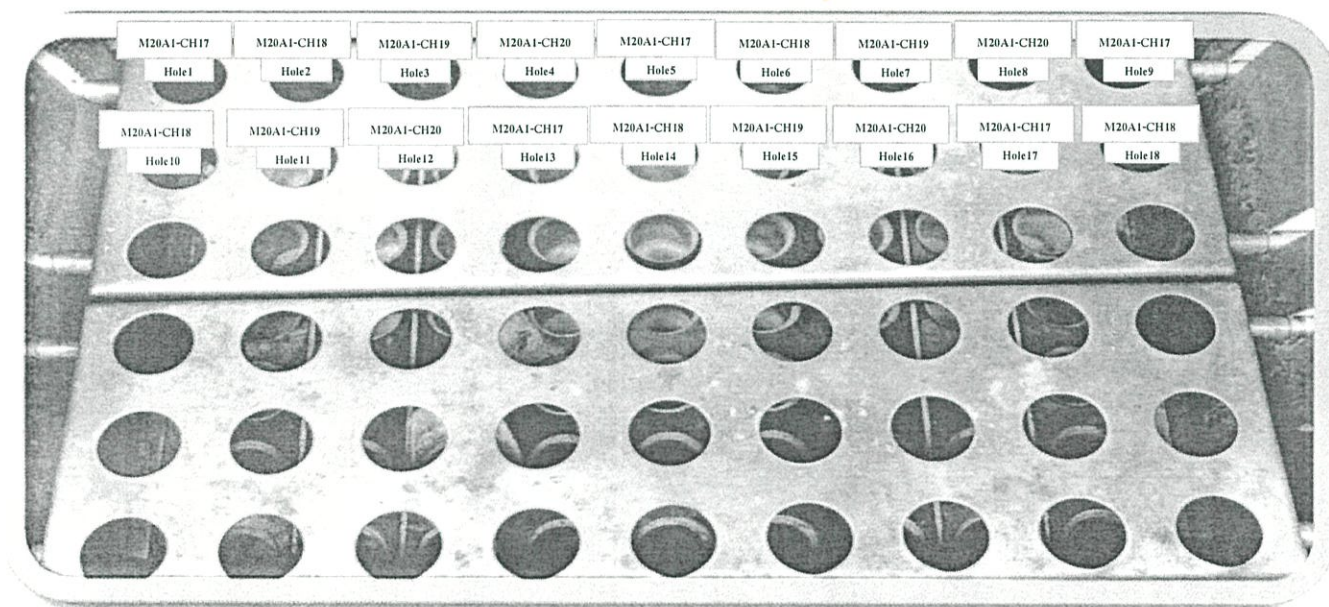

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	Hole1	Hole2	Hole3	Hole4	Hole5	Hole6	Hole7	Hole8	Hole9
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17
380.0	380.0	379.8 - 380.2	Max °C	376.5	377.1	377.3	382.0	383.8	380.9	376.0	377.0	376.3
			Min °C	376.1	376.7	377.0	381.8	383.5	380.6	375.7	376.7	375.9
			Average °C	376.3	376.9	377.1	381.9	383.6	380.8	375.8	376.9	376.1
			Stability ± °C	0.2	0.2	0.2	0.1	0.2	0.2	0.2	0.1	0.2


Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	Hole10	Hole11	Hole12	Hole13	Hole14	Hole15	Hole16	Hole17	Hole18
				M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18
380.0	380.0	379.8 - 380.2	Max °C	377.3	378.1	382.6	383.2	381.8	380.8	380.4	376.6	378.2
			Min °C	376.9	377.6	382.2	382.7	381.4	380.5	380.1	375.8	377.4
			Average °C	377.1	377.9	382.4	382.9	381.6	380.6	380.3	376.2	377.8
			Stability ± °C	0.2	0.3	0.2	0.2	0.2	0.1	0.1	0.4	0.4

Approved By. _____

Certificate No. T220133I01

Page 4 of 5

Calibration Report

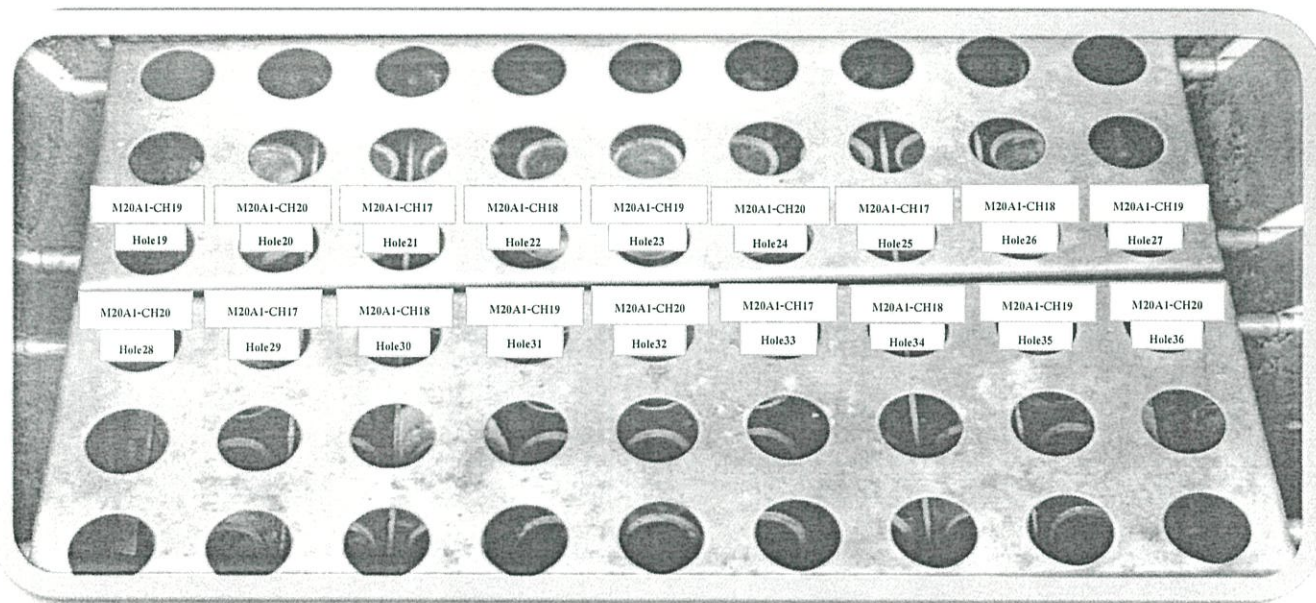

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	Hole19	Hole20	Hole21	Hole22	Hole23	Hole24	Hole25	Hole26	Hole27
				M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19
380.0	380.0	379.8 - 380.2	Max °C	379.2	383.0	382.8	384.1	383.1	384.1	377.2	377.4	378.4
			Min °C	378.4	382.3	382.2	383.6	382.6	383.7	376.9	377.1	378.0
			Average °C	378.8	382.7	382.5	383.9	382.8	383.9	377.0	377.2	378.2
			Stability ± °C	0.4	0.3	0.3	0.3	0.3	0.2	0.2	0.1	0.2


Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	Hole28	Hole29	Hole30	Hole31	Hole32	Hole33	Hole34	Hole35	Hole36
				M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.8 - 380.2	Max °C	380.6	381.9	383.9	381.4	382.0	378.3	379.4	380.4	376.2
			Min °C	380.1	381.5	383.5	381.1	381.7	377.9	379.0	379.8	375.8
			Average °C	380.4	381.7	383.7	381.2	381.8	378.1	379.2	380.1	376.0
			Stability ± °C	0.3	0.2	0.2	0.2	0.1	0.2	0.2	0.3	0.2

Approved By. _____

Certificate No. T220133101

Page 5 of 5

Calibration Report

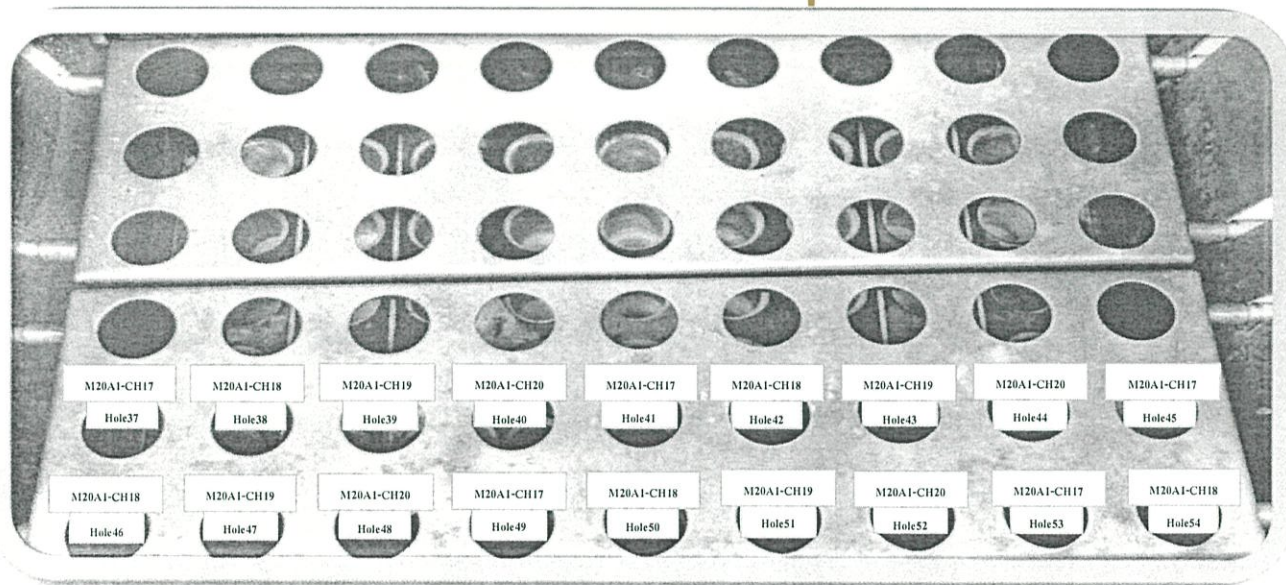

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	Hole37	Hole38	Hole39	Hole40	Hole41	Hole42	Hole43	Hole44	Hole45
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17
380.0	380.0	379.8 - 380.2	Max °C	381.1	383.5	384.2	379.8	381.3	381.4	381.3	380.6	380.7
			Min °C	380.8	383.2	383.9	379.4	380.8	381.0	380.9	380.2	380.4
			Average °C	381.0	383.4	384.1	379.6	381.1	381.2	381.1	380.4	380.6
			Stability ± °C	0.2	0.2	0.1	0.2	0.2	0.2	0.2	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	Hole46	Hole47	Hole48	Hole49	Hole50	Hole51	Hole52	Hole53	Hole54
				M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18
380.0	380.0	379.8 - 380.2	Max °C	377.2	377.8	382.8	378.6	379.5	380.4	383.3	383.0	378.1
			Min °C	376.8	377.2	382.2	378.3	379.3	380.1	383.1	382.7	377.8
			Average °C	377.0	377.5	382.5	378.4	379.4	380.2	383.2	382.8	377.9
			Stability ± °C	0.2	0.3	0.3	0.2	0.1	0.2	0.1	0.2	0.2


The expanded uncertainty of temperature measurement was ± 1.63 °C

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2 , providing a level of confidence of approximately 95 % .

Approved By. _____



Agilent CrossLab Compliance Services

Agilent
CrossLab

From Insight to Outcome

EQUIPMENT QUALIFICATION REPORT (EQR)**Agilent CrossLab Compliance**

Qualification Type: ICPMS-OQ

System ID: JP16511669

EQP Name: AgilentRecommended

EQP Revision: ICPMS.02.50

EQP Publish Date: March 2020

Date: February 8, 2022 11:47:17 AM

Report Type: Report

Org. Name: ALS laboratory Group (Thailand) Co.,Ltd.

Org. Location: 114/1 Moo8, Kanchanawanich Rd., T.Ban Phru,
A.Hatyai, Songkhla 90250

REVIEW BY
APPROVED BY
NEXT CAL. DATE	8/2/2023

Date: February 8, 2022 11:47:17 AM
System ID: JP16511669

Certificate of System Qualification

ICPMS-OQ

System ID: JP16511669

Organization Name: ALS laboratory Group (Thailand) Co.,Ltd.

Organization Location: 114/1 Moo8, Kanchanawanich Rd., T.Ban Phru, A.Hatyai, Songkhla 90250

Date: February 8, 2022 11:39:47 AM

EQP Name: AgilentRecommended

EQP Revision: ICPMS.02.50

Overall Qualification Status: Pass

Autosampler Check

Overall Autosampler Check Test Status

Pass

Integrated Sample Introduction System (ISIS) Check

Overall Integrated Sample Introduction System (ISIS) Check Test Status

Pass

Autotune

Peakwidth Mass 7	Pass
Peakwidth Mass 89	Pass
Peakwidth Mass 205	Pass
Mass Axis 7	Pass
Mass Axis 89	Pass
Mass Axis 205	Pass
Mass 7 Sensitivity No Gas	Pass
Mass 89 Sensitivity No Gas	Pass
Mass 205 Sensitivity No Gas	Pass
Mass 59 Sensitivity He	Pass
Mass 89 Sensitivity H2	Pass
Oxide Ratio 156/140	Pass
Doubly Charged Species Ratio 70/140	Pass

Date: February 8, 2022 11:39:47 AM

System ID: JP16511669

Overall Autotune Test Status

Pass

Background (No Gas Mode)

Setpoint Status:

Pass

Masses (AMU):

Measured Value:

Agilent Recommended:

Status:

	7	89	205		
	6.400	1.800	5.700	cps	
<=	6.9	<=	4.6	<=	11.5
Pass		Pass		Pass	

Overall Background (No Gas Mode) Test Status

Pass

Background (Gas Mode)

Gas Mode:

Helium

Setpoint Status:

Pass

Mass (AMU):

Measured Value:

Agilent Recommended:

Status:

	78	
	4.60	cps
<=	115	
Pass		

Gas Mode:

Hydrogen

Setpoint Status:

Pass

Mass (AMU):

Measured Value:

Agilent Recommended:

Status:

	78	
	1.45	cps
<=	4.6	
Pass		

Overall Background (Gas Mode) Test Status

Pass

Date: February 8, 2022 11:39:47 AM

System ID: JP16511669

20-Minute Stability (No Gas Mode)

Masses (AMU):

Stability RSD:

Agilent Recommended:

Status:

	7		89		205	
	1.26		0.28		0.43	%
<=	2.3	<=	2.3	<=	2.3	
Pass		Pass		Pass		

Overall 20-Minute Stability (No Gas Mode) Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

ICP-MS 1

Manufacturer	Agilent Technologies
Name	7900
Model Number	G8403A
Installed Options	#100H: Standard Package with Hydrogen option
Detector Type	SQ
Nebulizer	Mira Mist (G3161)
Spray Chamber	Quartz
Torch	Quartz
Sampling Cone	Ni
Skimmer Cone	Ni
Serial Number	JP16511669
Firmware Revision	4.00.02

ISIS 1

Manufacturer	Agilent Technologies
Name	ISIS3
Model Number	G8411A
Type	Peristaltic pump system
Serial Number	JP16510376

Autosampler 1

Manufacturer	Agilent Technologies
Name	SPS4
Model Number	G8410A
Serial Number	AU16351847

Chiller 1

Manufacturer	Agilent Technologies
Name	Chiller
Model Number	G3292A
Serial Number	701711328

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Burin Ngamvijit
Logged On User Name:	Burin_ngamvijit@agilent.com
Signature Creation Date:	February 8, 2022
Reason for Signature:	Published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: burin_ngamvjljt
 Hostname: ASSGKWX019

System Id: JP16511669
 Print Date: February 8, 2022 11:39:48 AM

OQ HW 7900ICPMS ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
February 8, 2022 9:19:05 AM	Audit	SessionCreated	Session	None
February 8, 2022 9:19:05 AM	Start	Configuration	Session	None
February 8, 2022 9:19:05 AM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
February 8, 2022 9:23:56 AM	Audit	EqpLoaded	Session	EQP details for primary technique [lcpMs] - File path: [ProtocolPacks/lcpMs/Configurations/02.50/lcpMs.02.50.eqp], EQP File Name: [lcpMs.02.50.eqp], EQP Name: [AgilentRecommended]
February 8, 2022 9:24:02 AM	End	Configuration	Session	None
February 8, 2022 9:24:09 AM	Start	Qualification	Session	OQ
February 8, 2022 9:24:09 AM	Start	Execution	Autosampler Check : SPS4: Autosampler Check	None
February 8, 2022 9:24:54 AM	End	Execution	Autosampler Check : SPS4: Autosampler Check	Run Count : 1
February 8, 2022 9:24:57 AM	Start	Execution	Integrated Sample Introduction System (ISIS) Check : ISIS3: Integrated Sample Introduction System (ISIS) Check	None
February 8, 2022 10:52:47 AM	End	Execution	Integrated Sample Introduction System (ISIS) Check : ISIS3: Integrated Sample Introduction System (ISIS) Check	Run Count : 1

User Name: burin_ngamvijit
 Hostname: ASSGKWX019

System Id: JP16511669
 Print Date: February 8, 2022 11:39:48 AM

OQ HW 7900iCPMS ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
February 8, 2022 10:52:50 AM	Start	Execution	Autotune : G8403A: Autotune 1	None
February 8, 2022 10:55:26 AM	End	Execution	Autotune : G8403A: Autotune 1	Run Count : 1
February 8, 2022 10:55:34 AM	Start	Execution	Background (No Gas Mode) : G8403A: No Gas Mode Background 1	None
February 8, 2022 10:55:56 AM	End	Execution	Background (No Gas Mode) : G8403A: No Gas Mode Background 1	Run Count : 1
February 8, 2022 10:56:00 AM	Start	Execution	Background (Gas Modes) : G8403A: Gas Mode Background :Helium	None
February 8, 2022 10:56:22 AM	End	Execution	Background (Gas Modes) : G8403A: Gas Mode Background :Helium	Run Count : 1
February 8, 2022 10:56:24 AM	Start	Execution	Background (Gas Modes) : G8403A: Gas Mode Background :Hydrogen	None
February 8, 2022 10:56:40 AM	End	Execution	Background (Gas Modes) : G8403A: Gas Mode Background :Hydrogen	Run Count : 1
February 8, 2022 10:56:43 AM	Start	Execution	20-Minute Stability (No Gas Mode) : G8403A: 20-Minute Stability (No Gas Mode) 1	None
February 8, 2022 11:01:33 AM	End	Execution	20-Minute Stability (No Gas Mode) : G8403A: 20-Minute Stability (No Gas Mode) 1	Run Count : 1
February 8, 2022 11:07:37 AM	End	Qualification	Session	OQ
February 8, 2022 11:07:37 AM	Start	Reporting	Session	None

Page 2 / 3

User Name: burln_ngamvijit

System Id: JP16511669

Hostname: ASSGKWX019

Print Date: February 8, 2022 11:39:48 AM

OQ HW 7900ICPMS ALS Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
February 8, 2022 11:38:19 AM	Audit	Reporting	Session	Report Generated : Certificate



CALIBRATION CERTIFICATE

Issued Date : 19-Aug-2021

Certificate No. : 21OV449

CSR No. : A078/3892

Page : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8 Karnchanawanich Rd. T.Ban Phru,
A. Hat Yai, Songkhla 90250 TH

Calibration Place : Chemical Laboratory

Instrument Name : Cold Room Water

Manufacturer : MODULAR

Model : N/A

Serial No. : N/N

ID No. : SGK_CL0065

Resolution : 0.1 °C

Received Date : 16-Aug-2021

Calibrated Date : 16-Aug-2021

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY

APPROVED BY

NEXT CAL. DATE 14/02/2023

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on G-20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Ibrorhim Saleemin

Approved by :

Sakeereen Heemhad / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data logger With Sensor	34970A	MY44064411	QR21-0314	9-Feb-2022

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

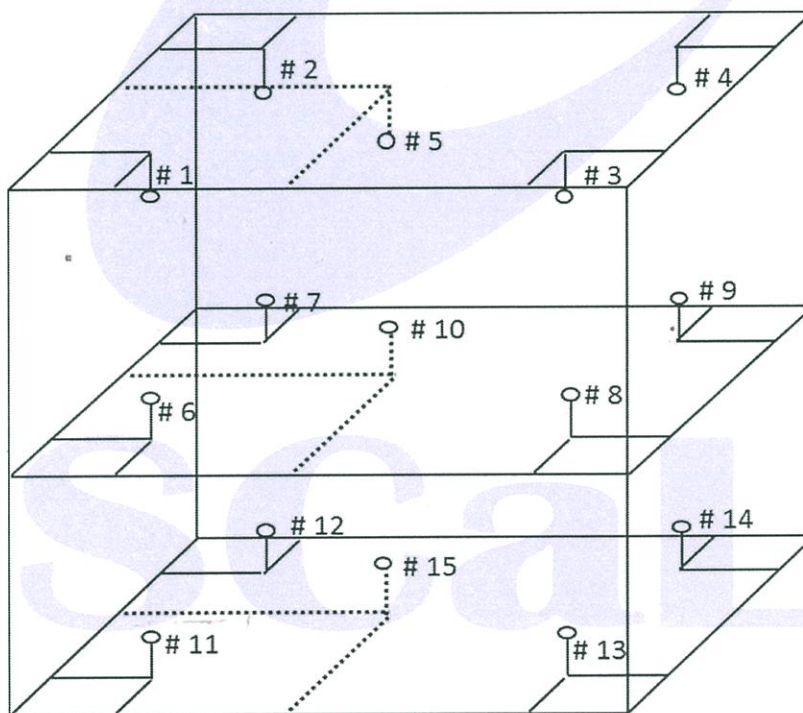

Sensor Installation Details

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of the chamber

W = 370.0 cm
H = 250.0 cm
D = 540.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Cold Room Water and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)														
	#1	#2	#3	#4	#5	#6	#7	#8	#9	Ref.10	#11	#12	#13	#14	#15
4	3.63	3.35	3.58	3.80	4.14	3.76	3.77	3.72	3.82	3.80	3.62	3.88	3.67	3.80	3.61

The uncertainty of measurement was ± 0.38 °C

3. Performance Result

The performance of the Cold Room Water are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (\pm °C)	Temperature Uniformity (°C)	Overall Variation (°C)
4	4.0	4.0	1.23	0.69	3.33

* UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

SCaL



Certificate of Calibration

Certificate No.:	PTC/10/22004	Page:	1 of 4
Equipment:	Cod Reactor	Condition:	New
Manufacturer:	Hach	Serial No. :	21120C1313
Model:	DRB200	ID No. :	-
Covers:	None	Holes:	30

Environment Condition:	Temperature:	25.2	°C	±	0.1	°C
	Humidity:	49.5	%RH	±	1.1	%RH
	Voltage:	221.8	VAC	±	0.6	VAC

Customer: ALS LABORATORY GROUP (THAILAND)
114/1 Moo.8, Karnchanawanich Rd., T.Ban Phru,
A.Hat Yai, Songkhla 90250 Thailand.

Calibration Place: Penta Calibration Co., Ltd. (Temperature Laboratory)
66/124 The connect 34 Village, Kanchanaphisek Road,
Dokmai, Prawet Bangkok 10250 Thailand

The Method used: In house method, PTC-WI-10, based on Compare with Standard Thermometer

Traceability: This certificate is traceable to the SI Units through Quality Reborn Co.,Ltd ,
NSC-ONSC Accreditation No.: Calibration 0292

Date Received: February 08, 2022
Date Calibrated: February 08, 2022
Date Issued: February 08, 2022
Calibrated By: Mr. Todsapol Moolsuang


Approved By : _____

(Mr.Kriangsak Kalasri)

Reviewed by

(Mr. Keattisak Kerdto)

Laboratory Manager

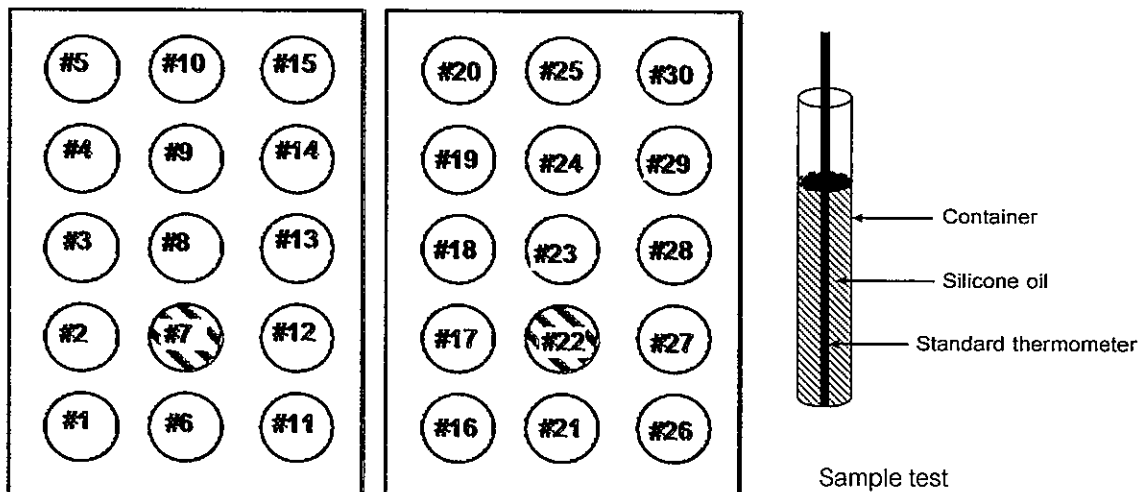

Standard Installation Position:

Module	1									
Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9	#10
Probe No.	1	2	3	4	5	6	7	8	9	10

Module	2									
Position of Std	#11	#12	#13	#14	#15	#16	#17	#18	#19	#20
Probe No.	1	2	3	4	5	6	7	8	9	10

Module	2									
Position of Std	#21	#22	#23	#24	#25	#26	#27	#28	#29	#30
Probe No.	1	2	3	4	5	6	7	8	9	10

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognised national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The effect that the results relate only to the items calibrated.

This calibration certificate shall not be reproduced except in full only, without written approval from penta calibration co., ltd



Measurement Results:

Without adjustment

Position heating block	Calibration point (°C)	Setting (°C)	UUC Reading (°C)
Left	150	150	150

Measurement Temperature (°C) @ Probe No.			
Position	Standard Reading (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	150.77	0.77	0.64
#2	149.49	-0.51	0.63
#3	150.38	0.38	0.63
#4	150.28	0.28	0.63
#5	149.74	-0.26	0.63
#6	150.94	0.94	0.64
#7	149.01	-0.99	0.64
#8	150.82	0.82	0.64
#9	149.49	-0.51	0.63
#10	149.11	-0.89	0.63
#11	149.31	-0.69	0.64
#12	150.73	0.73	0.64
#13	150.48	0.48	0.64
#14	149.13	-0.87	0.63
#15	149.19	-0.81	0.64

UUC Characterization

UUC Setting (°C)	UUC Reading (°C)	Measured Uniformity (°C)	Measured Stability (± °C)
150	150	1.55	0.12

Note: UUC = Unit Under Calibration

Definitions

UUC Reading : The average reading of indicating device which forms the integral part of UUC.

Standard Reading : The average reading of standards at any positions or location.

Measured Uniformity : The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with any holes of UUC at steady-state. The reference probe is preferably located in the geometric center of UUC.

Measured Stability : The one-half of greatest maximum difference of measured temperatures at any one probe.



Measurement Results:

Without adjustment

Position heating block	Calibration point (°C)	Setting (°C)	UUC Reading (°C)
Right	150	150	150

Measurement Temperature (°C) @ Probe No.			
Position	Standard Reading (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#16	149.46	-0.54	0.64
#17	149.79	-0.21	0.64
#18	149.27	-0.73	0.64
#19	150.14	0.14	0.64
#20	149.38	-0.62	0.64
#21	150.81	0.81	0.64
#22	150.80	0.80	0.65
#23	150.71	0.71	0.64
#24	149.86	-0.14	0.64
#25	149.23	-0.77	0.64
#26	150.61	0.61	0.64
#27	149.10	-0.90	0.64
#28	150.71	0.71	0.64
#29	149.10	-0.90	0.64
#30	150.74	0.74	0.64

UUC Characterization

UUC Setting (°C)	UUC Reading (°C)	Measured Uniformity (°C)	Measured Stability (± °C)
150	150	1.55	0.12

Note: UUC = Unit Under Calibration

Definitions

UUC Reading : The average reading of indicating device which forms the integral part of UUC.

Standard Reading : The average reading of standards at any positions or location.

Measured Uniformity : The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with any holes of UUC at steady-state. The reference probe is preferably located in the geometric center of UUC.

Measured Stability : The one-half of greatest maximum difference of measured temperatures at any one probe.

The End of Certificate



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CHO32

Page.: 1 of 3

Certificate of Calibration

Equipment : UV-VIS Spectrophotometer
Manufacturer : Hach
Model : DR 3900
Serial No. : 1687645
ID No. : SGK_CL0038
Condition As-Received: Used Item
Received Date : 24 January 2022
Calibration Date : 24 January 2022
Reference : 2201-0617OC-1
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Songkhla Branch
114/1 Moo 8, Kanjanavanij Rd., Banphru, Hatyai,
Songkhla 90250 , Thailand
Calibration Place : Chemistry Room
Ambient Temperature : (24.9 - 25.2) °C (On-Site)
Relative Humidity : (39.2 - 45.2) % (On-Site)
Calibration Procedure : In - house method :
CP-OCH4 based on ASTM E 275-01
Calibrated by : Kunchit Promprat

REVIEW BY

APPROVED BY

NEXT CAL. DATE 24/1/23

Approved by :

- (☒) Malee Butkruea
(☐) Saithip Meangmai
(☐) Warakorn Lerngagtrakul

Approved Signatory

Issue Date :

7 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0037403



Cert. No. : 22CHO32

Page : 2 of 3

Condition of calibration result

1. Reference Standard Material :

<u>Material</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1. Absorbance Standard set	8331	86623	08 Sep 2022
2. Wavelength Standard set	29829	94776	02 Sep 2023
3. Wavelength Standard set	29829	94777	02 Sep 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit maintained at :

- National Physical Laboratory (NPL), The United Kingdom of Great Britain and Northern Ireland
- National Institute of Standards and Technology (NIST), The United States of America

4. Spectral BandWidth : 5 nm

Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (\pm nm)	Coverage Factor <i>k</i>
418.40	418	0.59	2.00
479.88	480	0.59	2.00
513.75	514	0.59	2.00
537.00	536	0.59	2.00
638.00	638	0.59	2.00
747.61	748	0.59	2.00
807.04	807	0.59	2.00

Malu.



Cert. No. : 22CHO32

Page : 3 of 3

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (\pm Abs)	Coverage Factor <i>k</i>
420.0	Zero	0.000	0.0028	2.00
	0.5723	0.572	0.0033	2.00
	0.7522	0.751	0.0031	2.00
	1.0907	1.090	0.0033	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5616	0.560	0.0034	2.00
	0.7345	0.732	0.0032	2.00
	1.0646	1.063	0.0033	2.00
465.0	Zero	0.000	0.0028	2.00
	0.5118	0.514	0.0034	2.00
	0.6773	0.679	0.0031	2.00
	0.9809	0.984	0.0033	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5228	0.522	0.0030	2.00
	0.6861	0.684	0.0030	2.00
	0.9941	0.993	0.0030	2.00
590.0	Zero	0.000	0.0028	2.00
	0.5546	0.552	0.0029	2.00
	0.7159	0.712	0.0030	2.00
	1.0369	1.033	0.0030	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5401	0.538	0.0029	2.00
	0.6835	0.680	0.0029	2.00
	0.9889	0.986	0.0030	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

Malu.

-o0o-

a 1093314



CALIBRATION CERTIFICATE

Issued Date : 12-Nov-2021

Certificate No. : 21PH192

CSR No. : A012/00583

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8 Karnchanawanich Rd. T.Ban Phru,
A. Hat Yai, Songkhla 90250 TH

Calibration Place : Chemical Laboratory

Instrument Name : pH meter

Manufacturer : Mettler Toledo

Model : S220

Serial No. : B625631849

ID No. : SGK_CL0030

Electrode No. : 6404000

Received Date : 9-Nov-2021

Calibrated Date : 9-Nov-2021

Ambient Temperature : $(25 \pm 3) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \%$

REVIEW BY

APPROVED BY

TEST CAL. DATE 10/05/2025

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HACH : LANGE United For Water Quality
- WK : WK Electric Co., Ltd.
- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Jessadagon Lemhud

Approved by :

Sakeereen Heemhad / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.005	C02840	1617	24-Aug-2022
Standard Solution	7.000	C02841	1618	24-Aug-2022
Standard Solution	10.012	C02843	1619	24-Aug-2022
Temperature/Electrical Calibrator	MC2-MF	23642	WK2102-006-229	21-Feb-2022
Digital Thermometer With Sensor	1529	B4C223	QR21-2009	15-Sep-2022

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading (mV)	Correction (mV)	Uncertainty (± mV)
177.48	177.5	-0.02	0.17
0.00	0.0	0.00	0.13
-177.48	-177.5	0.02	0.17

2. Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading (pH)	Correction (pH)	Uncertainty (± pH)
4.007	3.99	0.017	0.011
6.999	7.02	-0.021	0.014
10.011	10.01	0.001	0.036

3. Temperature Measurement

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25	24.93	25.0	-0.07	0.11

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkhla 90250 Thailand

Tel: 081 599 0417 Fax: 074 805 133 Email: s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 8-Feb-2022

Certificate No. : 22WB004

CSR No. : A0223/01123

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8 Karnchanawanich Rd. T.Ban Phru,
A. Hat Yai, Songkhla 90250 TH

Calibration Place : Chemical Laboratory
Instrument Name : Water Bath
Manufacturer : Memmert
Model : WNE29
Serial No. : L616.0538
ID No. : SGK_CL0035
Resolution : 0.1 °C
Received Date : 5-Feb-2022
Calibrated Date : 5-Feb-2022
Ambient Temperature : (30 ± 10) °C
Relative Humidity : (50 ± 30) %

REVIEW BY

APPROVED BY

NEXT CAL. DATE 6/07/2023

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.W1.014 based on ASTM E 715 : 1980 (reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Imron Rattanaylum

Approved by .

Sakeereen Heemhad / Technical Manager

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data logger With Sensor	34970A	MY44064411	QR21-0314	9-Feb-2022

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

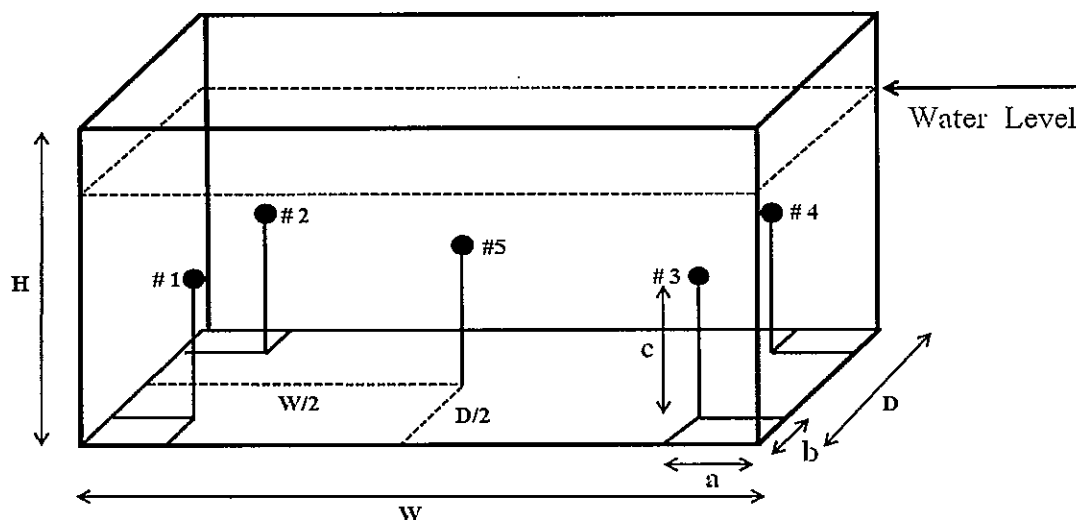

Sensor Installation Details

$a = 5$ cm
 $b = 5$ cm
 $c = 5$ cm

Dimension of the chamber

$W = 45$ cm
 $H = 30$ cm
 $D = 35$ cm

Result of Calibration .:

2. Temperature Measurement Accuracy Test

The measurement results of the Water Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (± °C)
	#1	#2	#3	#4	Ref.5	
80	79.95	80.07	79.95	79.99	80.03	0.14

3. Performance Result

The performance of the Water Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
80	81.0	81.0	0.10	0.19	0.19

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...