



ภาคผนวก จ

เอกสารสอบเทียบเครื่องมือฯ


TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	May 19, 2022
พื้นที่โครงการด้านทิศตะวันออกเชิงใต้ใกล้กับชุมชน				Start Time	9:44 AM
Sampler Number	TSP No.A6	Transfer Standard Type	Orifice	Stop Time	9:54 AM
Instrument Model	HIVOL-BBCBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Somprasong Thetsakun
Motor Serial Number	2012-01	Calibrator Serial Number	3362		
Recorder Serial Number	3140				

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	$Qstd = (1/m)[(A-b)]$	sample Flow Rate Indication	$IC = [(Pa/P_{std})(T_{std}/Ta)]^{1/2}$				
	Positive	Negative	ΔH_2O		(m ³ /min)	(ft ³ /min)		(°K = °C+273)	(mmHg)		
5	1.5	1.5	3.0	1.70868	0.84544	31.0	30.58	305.0	757.0		
7	2.6	2.6	5.2	2.24958	1.11457	40.0	39.46	305.0	757.0		
10	3.6	3.6	7.2	2.64707	1.31235	48.0	47.35	305.0	757.0		
13	4.5	4.5	9.0	2.95952	1.46781	54.0	53.27	305.0	757.0		
18	6.0	6.0	12.0	3.41735	1.69561	62.0	61.16	305.0	757.0		
Linear Regression Y ON X : Y= mX + b							Average	305.0	757.0		
1	Slope (m)			2.00980	Linear Equation			r ²	0.998948	Pstd(mmHg)	760.0
2	Intercept (b)			0.00951	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.9994739	T _{NTP}	298.0
3	Correlation Coefficient (r)			0.99999	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)			0.973192407
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5			0.986505148

COMMENT

Andersen Instruments, Inc.

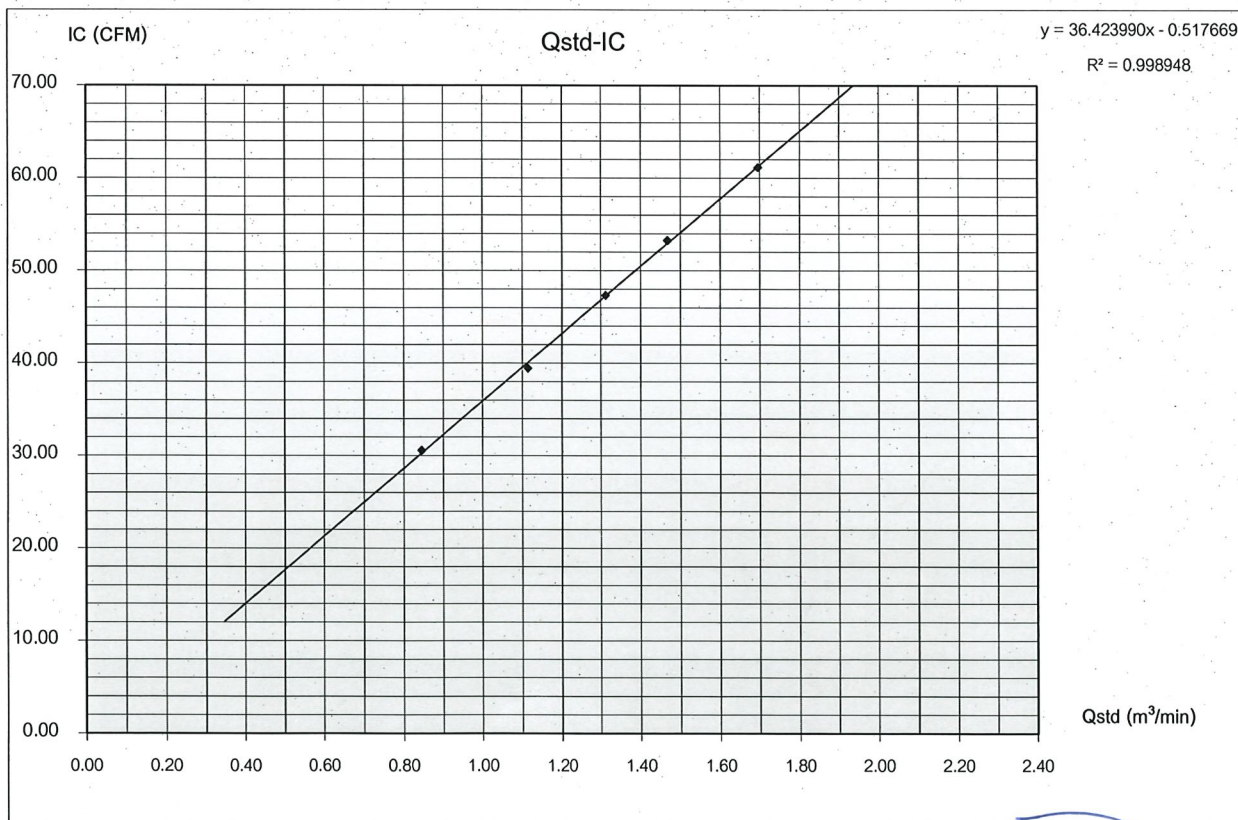

Checked By

(Mr. Prayun Detkla)
Technician



Approved By

(Mr. Panupon Podang)
Environmental Scientist


PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	May 19, 2022
พื้นที่โครงการด้านทิศตะวันตกเฉียงใต้ใกล้กับชุมชน				Start Time	9:54 AM
Sampler Number	PM-10 No.3	Transfer Standard Type	Orifice	Stop Time	10:04 AM
Instrument Model	HIVOL-BMBBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Somprasong Thetsakun
Motor Serial Number	TSP A9	Calibrator Serial Number	3362		
Recorder Serial Number	7351				

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric	Start	Stop
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	Qstd = (1/m)[(A-b)]	Sample Flow Rate Indication	$IC = I[(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	°K = °C+273)	Pressure	Meter	Meter
	Positive	Negative	ΔH ₂ O								
5	1.4	1.5	2.9	1.67996	0.83115	31.0	30.58	305.0	757.0		
7	2.5	2.6	5.1	2.22784	1.10376	41.0	40.45	305.0	757.0		
10	3.6	3.6	7.2	2.64707	1.31235	50.0	49.33	305.0	757.0		
13	4.6	4.6	9.2	2.99222	1.48408	57.0	56.23	305.0	757.0		
18	5.6	5.6	11.2	3.30148	1.63796	63.0	62.15	305.0	757.0		
Linear Regression Y ON X : Y= mX + b							Average	305.0	757.0		
1	Slope (m)			2.00980	Linear Equation			r ²	0.999242	Pstd(mmHg)	760.0
2	Intercept (b)			0.00951	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.9996209	T _{NTP}	298.0
3	Correlation Coefficient (r)			0.99999	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)		0.973192407	
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5		0.986505148	

COMMENT

Andersen Instruments, Inc.

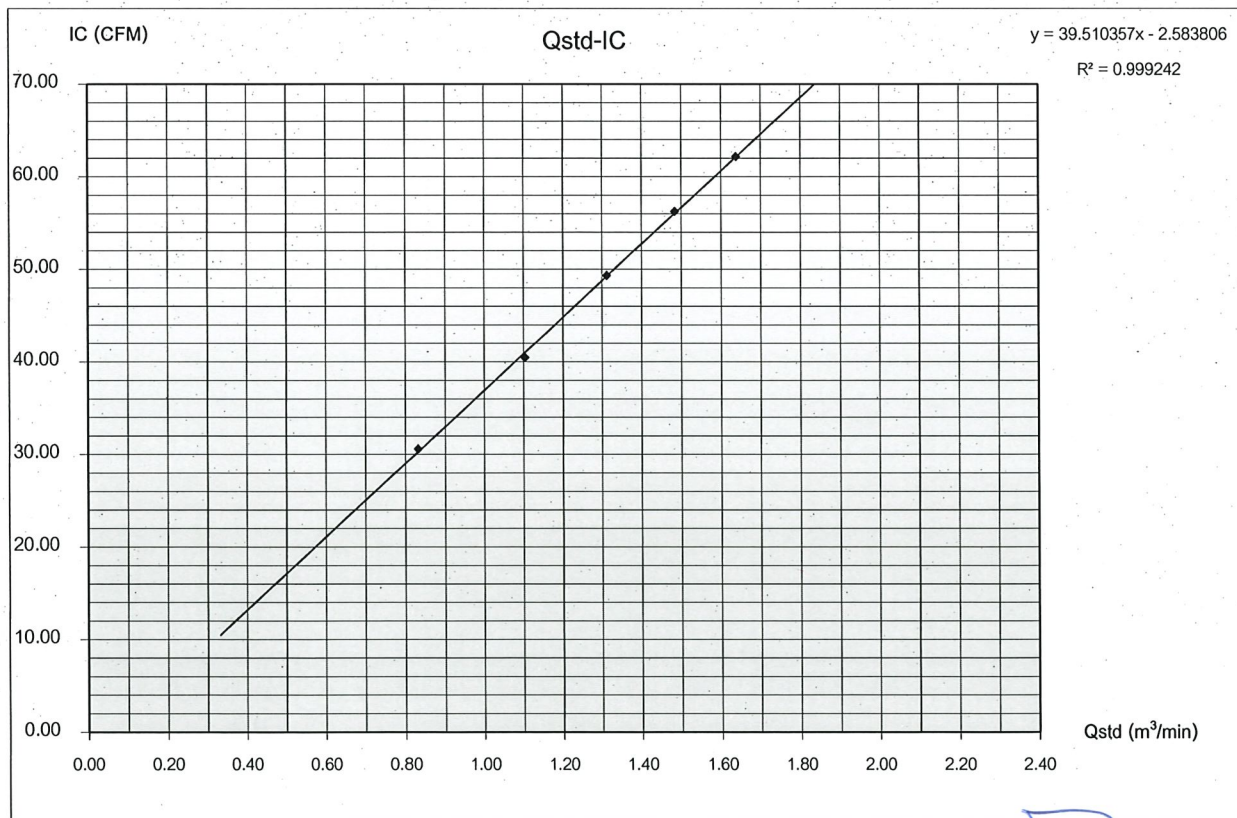

Checked By

(Mr. Prayun Detkla)
Technician



Approved By

(Mr. Panupon Podang)
Environmental Scientist


TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	May 19, 2022
บ้านเลขที่ 28 บ้านวังตะพาน หมู่ที่ 11				Start Time	11:01 AM
Sampler Number	TSP No.A9	Transfer Standard Type	Onfice	Stop Time	11:11 AM
Instrument Model	HIVOL-BBCBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Somprasong Thetsakun
Motor Serial Number	16119	Calibrator Serial Number	3362		
Recorder Serial Number	7137				

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication (ft ³ /min)	$IC = I[(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	(°K = °C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O								
5	1.5	1.5	3.0	1.70868	0.84544	36.0	35.51	305.0	757.0		
7	2.5	2.5	5.0	2.20589	1.09284	44.0	43.41	305.0	757.0		
10	3.5	3.5	7.0	2.61005	1.29393	50.0	49.33	305.0	757.0		
13	4.5	4.5	9.0	2.95952	1.46781	55.0	54.26	305.0	757.0		
18	5.5	5.5	11.0	3.27187	1.62322	60.0	59.19	305.0	757.0		
Linear Regression Y ON X : Y= mX + b							Average	305.0	757.0		
1	Slope (m)			2.00980	Linear Equation			r ²	0.999561	Pstd(mmHg)	760.0
2	Intercept (b)			0.00951	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.9997805	T _{NTP}	298.0
3	Correlation Coefficient (r)			0.99999	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)		0.973192407	
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5		0.986505148	

COMMENT

Andersen Instruments, Inc.

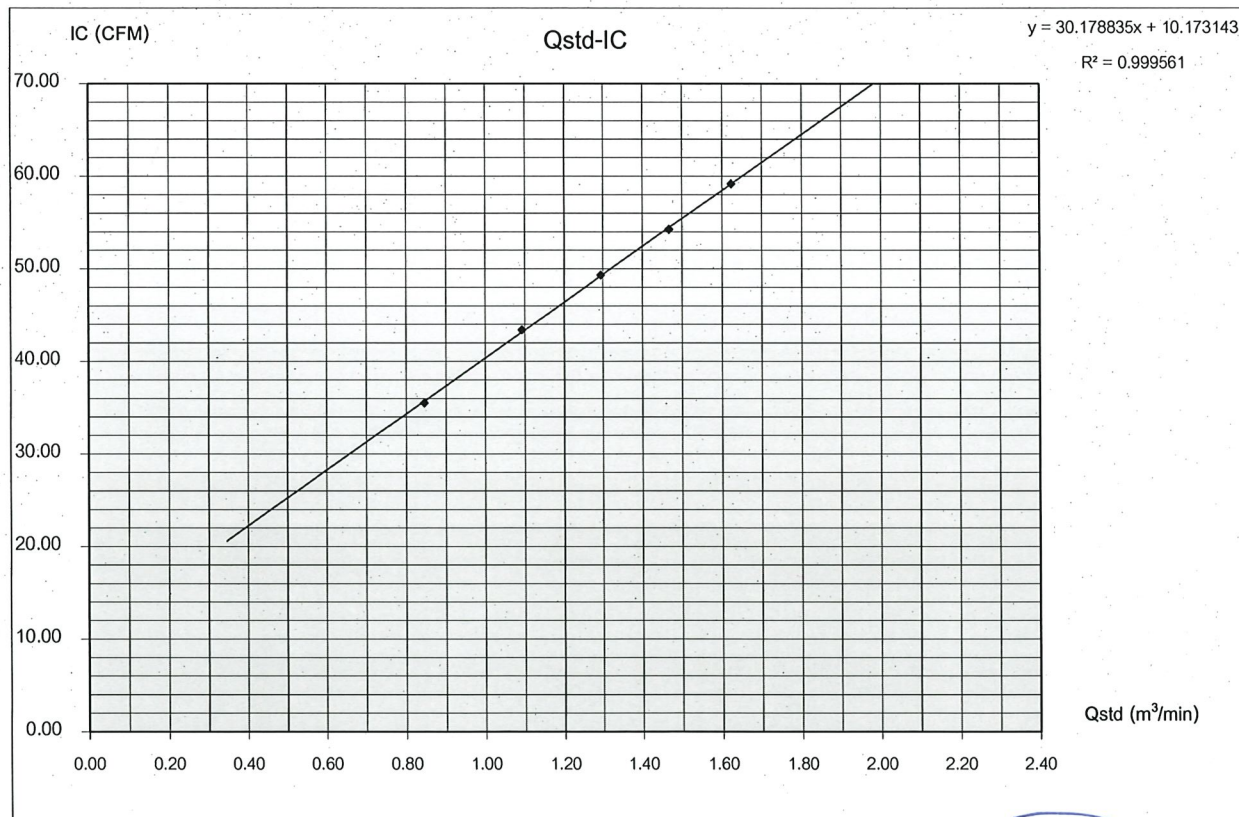

Checked By

Prayun
(Mr. Prayun Detkla)
Technician



Approved By

Mr. Panupon Podang
Environmental Scientist


PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	May 19, 2022
บ้านเลขที่ 28 บ้านจันทะพาบ หมู่ที่ 11				Start Time	10:50 AM
Sampler Number	PM-10 No.c1	Transfer Standard Type	Orifice	Stop Time	11:00 AM
Instrument Model	HIVOL-BMBBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Somprasong Thetsakun
Motor Serial Number	202001	Calibrator Serial Number	3362		
Recorder Serial Number					

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	$Qstd = (1/m)[(A-b)]$	Sample Flow Rate Indication	$IC = I[(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	(°K = °C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O		(m ³ /min)	(inch/min)					
5	1.4	1.4	2.8	1.65074	0.81661	0.8	0.79	305.0	757.0		
7	2.4	2.4	4.8	2.16132	1.07066	1.6	1.58	305.0	757.0		
10	3.3	3.4	6.7	2.55351	1.26580	2.2	2.17	305.0	757.0		
13	4.2	4.2	8.4	2.85916	1.41788	2.7	2.66	305.0	757.0		
18	5.0	5.0	10.0	3.11960	1.54746	3.1	3.06	305.0	757.0		
Linear Regression Y ON X : Y= mX + b							Average	305.0	757.0		
1	Slope (m)			2.00980	Linear Equation			r ²	0.999928	Pstd(mmHg)	760.0
2	Intercept (b)			0.00951	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.999964	T _{NTP}	298.0
3	Correlation Coefficient (r)			0.99999	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)		0.973192407	
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5		0.986505148	

COMMENT

Andersen Instruments, Inc.

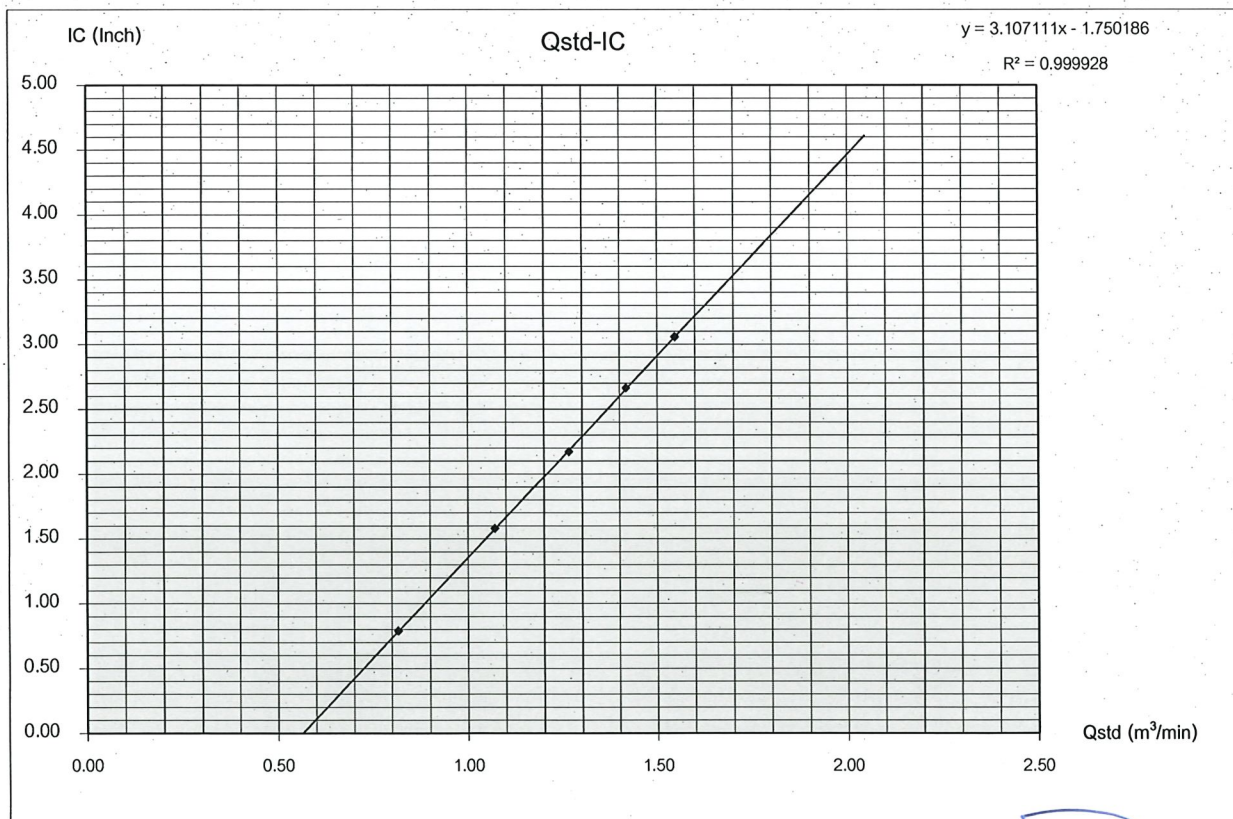

Checked By

(Mr. Prayun Detkla)
Technician



Approved By

(Mr. Panupon Podang)
Environmental Scientist


TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	May 19, 2022
โรงเรียนวัดใหม่ประจวบสมณัตถ์ภาพที่ 76				Start Time	12:15 PM
Sampler Number	TSP No.A3	Transfer Standard Type	Orifice	Stop Time	12:25 PM
Instrument Model	HIVOL-BBCBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Somprasong Thetsakun
Motor Serial Number	704	Calibrator Serial Number	3362		
Recorder Serial Number	465				

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	Qstd = (1/m)[(A-b)] (m ³ /min)	ample Flow Rate Indication (ft ³ /min)	IC = $I[(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(*K = °C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O								
5	1.4	1.5	2.9	1.67996	0.83115	35.0	34.53	305.0	757.0		
7	2.4	2.5	4.9	2.18372	1.08181	44.0	43.41	305.0	757.0		
10	3.5	3.5	7.0	2.61005	1.29393	50.0	49.33	305.0	757.0		
13	4.6	4.6	9.2	2.99222	1.48408	56.0	55.24	305.0	757.0		
18	5.4	5.5	10.9	3.25696	1.61581	60.0	59.19	305.0	757.0		
Linear Regression Y ON X : Y= mX + b							Average	305.0	757.0		
1	Slope (m)			2.00980	Linear Equation			r ²	0.998318	Pstd(mmHg)	760.0
2	Intercept (b)			0.00951	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.9991586	T _{MTP}	298.0
3	Correlation Coefficient (r)			0.99999	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)			0.973192407
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5			0.986505148


COMMENT

Andersen Instruments, Inc.

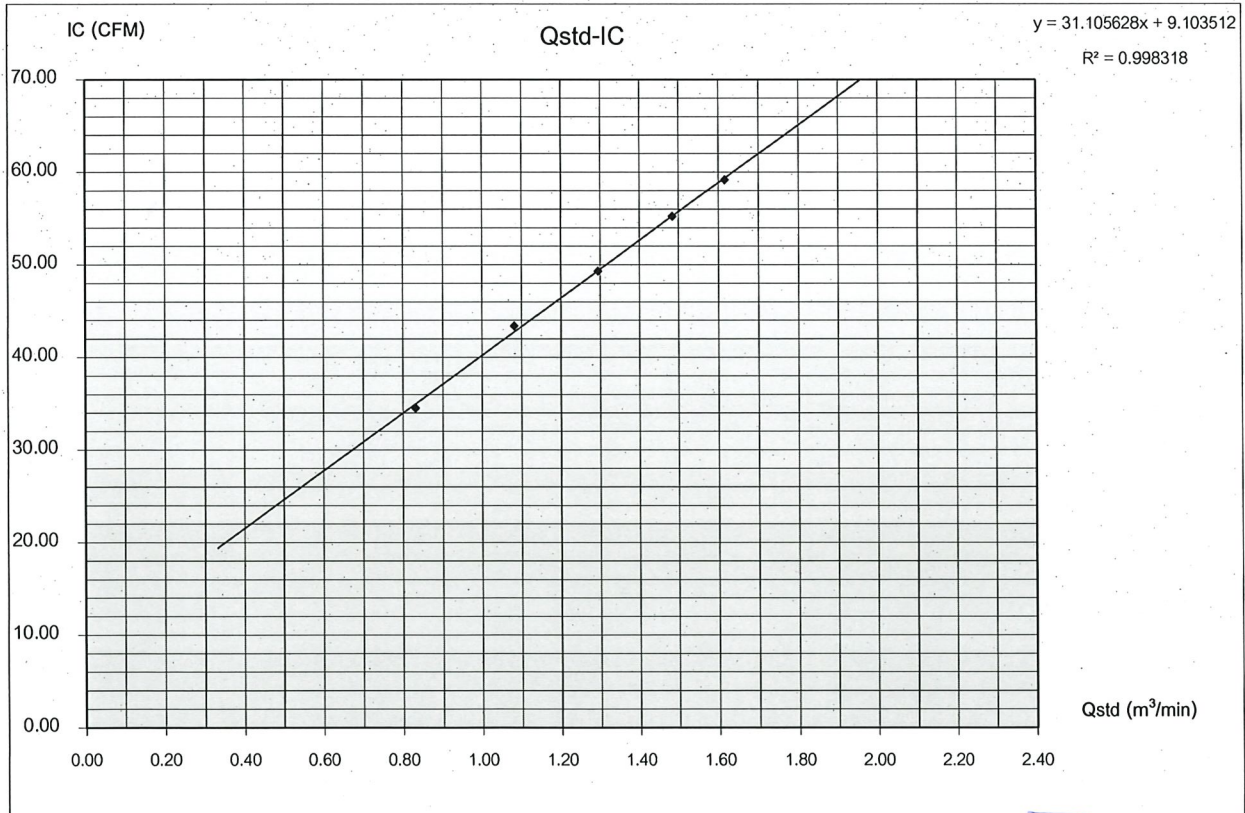

Checked By

(Mr. Prayun Detkla)
Technician



Approved By

(Mr. Panupon Podang)
Environmental Scientist


PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	May 19, 2022
โรงเรียนวัดใหม่ประชุมชนมิตร์ภาพที่ 76				Start Time	12:04 PM
Sampler Number	PM-10 No.c2	Transfer Standard Type	Orifice	Stop Time	12:14 PM
Instrument Model	HIVOL-BMBBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Somprasong Thetsakun
Motor Serial Number	PM10 202002	Calibrator Serial Number	3362		
Recorder Serial Number					

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			[ΔH ₂ O(Pa/P _{std})(T _{std} /Ta)] ^{1/2}	Qstd = (1/m)[(A-b)]	ample Flow Rate Indication	IC = I[(Pa/P _{std})(T _{std} /Ta)] ^{1/2}	(*K = °C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O		(m ³ /min)	(inch/min)					
5	1.4	1.5	2.9	1.67996	0.83115	0.9	0.89	305.0	757.0		
7	2.4	2.4	4.8	2.16132	1.07066	1.6	1.58	305.0	757.0		
10	3.5	3.5	7.0	2.61005	1.29393	2.3	2.27	305.0	757.0		
13	4.5	4.5	9.0	2.95952	1.46781	2.8	2.76	305.0	757.0		
18	5.2	5.3	10.5	3.19664	1.58580	3.2	3.16	305.0	757.0		
Linear Regression Y ON X : Y= mX + b							Average	305.0	757.0		
1	Slope (m)			2.00980	Linear Equation			r ²	0.999621	Pstd(mmHg)	760.0
2	Intercept (b)			0.00951	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.9998105	T _{NTP}	298.0
3	Correlation Coefficient (r)			0.99999	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)			0.973192407
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5			0.986505148

COMMENT

Andersen Instruments, Inc.

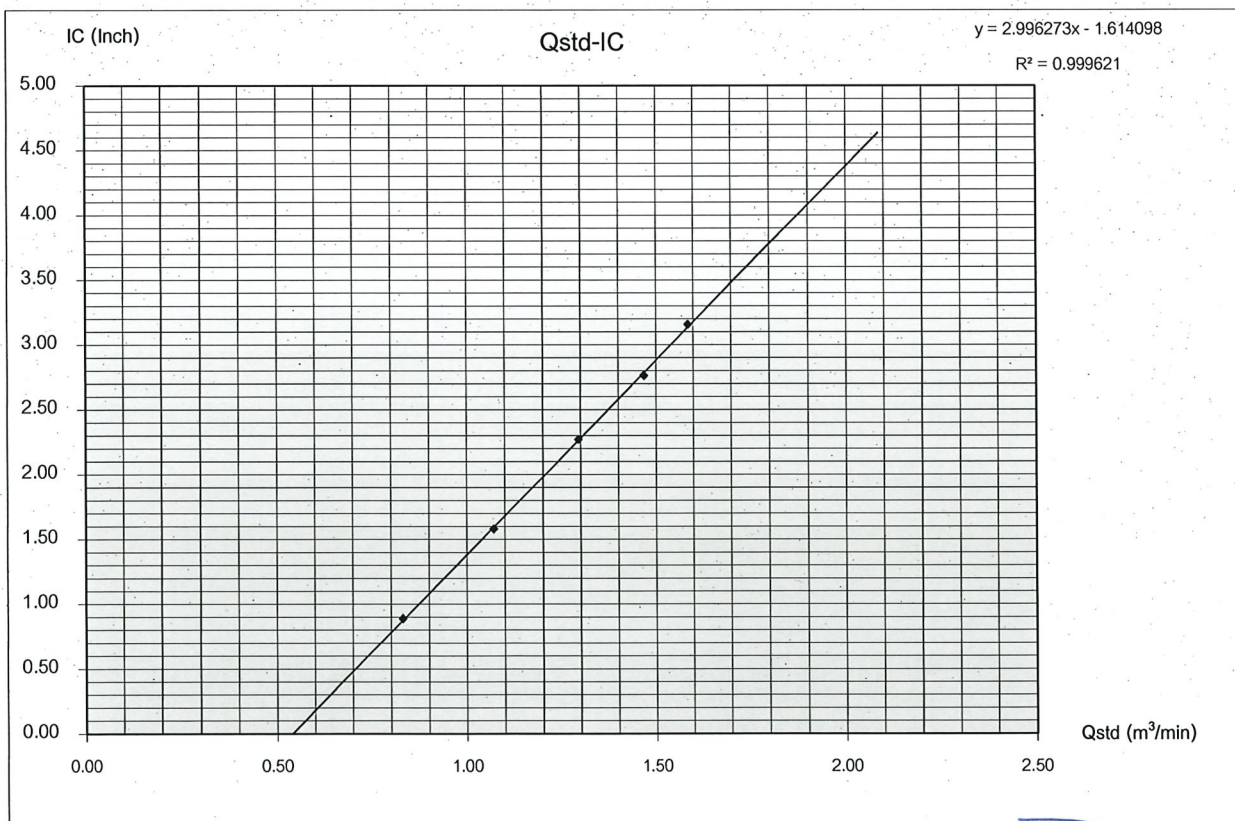


Checked By

(Mr. Prayun Detkla)
Technician

Approved By

(Mr. Panupon Podang)
Environmental Scientist



RECALIBRATION

DUE DATE:

July 26, 2022

Certificate of Calibration

Calibration Certification Information

Cal. Date: July 26, 2021 Rootsmeter S/N: 438320 Ta: 297 °K
 Operator: Jim Tisch Pa: 749.3 mm Hg
 Calibration Model #: TE-5025A Calibrator S/N: 3362

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.4180	3.2	2.00
2	3	4	1	0.9940	6.4	4.00
3	5	6	1	0.8890	8.0	5.00
4	7	8	1	0.8460	8.8	5.50
5	9	10	1	0.6970	12.8	8.00

Data Tabulation

Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9850	0.6947	1.4066	0.9957	0.7022	0.8904
0.9808	0.9867	1.9892	0.9915	0.9974	1.2592
0.9787	1.1009	2.2240	0.9893	1.1128	1.4078
0.9776	1.1556	2.3326	0.9883	1.1682	1.4765
0.9723	1.3950	2.8132	0.9829	1.4102	1.7807
QSTD	m=	2.00980	QA	m=	1.25850
	b=	0.00951		b=	0.00602
	r=	0.99999		r=	0.99999

Calculations

Vstd=	$\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$	Va=	$\Delta Vol((Pa-\Delta P)/Pa)$
Qstd=	Vstd/ΔTime	Qa=	Va/ΔTime
For subsequent flow rate calculations:			
Qstd=	$1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$	Qa=	$1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$

Standard Conditions

Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH: calibrator manometer reading (in H2O)	
ΔP: rootsmeter manometer reading (mm Hg)	
Ta: actual absolute temperature (°K)	
Pa: actual barometric pressure (mm Hg)	
b: intercept	
m: slope	

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30



PLAY SOLUTION TECHNOLOGY COMPANY LIMITED
179/75 Nawong Pracha Pattana Road, Sikan, Donmuang, Bangkok 10210
Tel.:+66 2 011 0505, Fax:+66 2 010 7700
www.playsotec.com



CERTIFICATE OF CALIBRATION

Customer _____ Certificate no. PST-0001-22
Page no. 1 of 3

Company : ENVIRONMENT RESEARCH & TECHNOLOGY CO.,LTD.
Address : 25/114 Moo 6 Soi Chinaket 1, Ngamwongwan Road, Toongsonghong,
City / Province : Laksi, Bangkok
Zip/Postal : 10210

Device

Equipment : Electronic Balance Capacity : 220 g
Manufacturer : METTLER TOLEDO Readability : 0.0001 g
Model : AB204-S ID No. : ERTC-L-in-0048
Serial No. : 1123103723

Environment Conditions

Location of Calibration : Calibration Laboratory at Play Solution Technology Co.,Ltd
Ambient Temperature : 25.9 (°C)
Relative Humidity : 53.1 (%RH)
Barometric Pressure : 1011.5 (mba)
Calibration Procedure : This Calibration was conducted by using In-House calibration procedure number CP-M-001 base on "UKAS LAB 14"
Comment :

Date of Receipt : January 4, 2022

Date of Calibration : January 4, 2022

Issue Date : January 4, 2022

Calibrated by : Kittichai R. Approved by : Kittichai Rattanatham
(Kittichai Rattanatham) (Kittichai Rattanatham)
Calibrator Approved Signature

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and is traceability to recognize national standards and to the unit of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval prior written approval of the calibration center, Play Solution Technology Co.,Ltd



PLAY SOLUTION TECHNOLOGY COMPANY LIMITED
179/75 Nawong Pracha Pattana Road, Sikan, Donmuang, Bangkok 10210
Tel.:+66 2 011 0505, Fax:+66 2 010 7700
www.playsotec.com



CERTIFICATE OF CALIBRATION

Result of Calibration : Without Adjustment Certificate no. PST-0001-22
Page no. 2 of 3

1. Repeatability

Weighing Rang 1 (g)	Normal Value (g)	Standard Deviation (g)
Max.capacity 220	200	0.00005

Weighing Rang 2 (g)	Normal Value (g)	Standard Deviation (g)
Max.capacity		

2. Linearity, Departure of Indication from nominal value

Weighing Range 1

Normal Value (g)	Standard Value (g)	Indication (g)	Error of Indication (g)	Expanded Uncertainty (g)	Factor k
0.001	0.00100	0.0010	0.0000	0.00011	2.07
0.01	0.01000	0.0100	0.0000	0.00011	2.07
0.1	0.10001	0.1000	0.0000	0.00011	2.07
1	1.00001	1.0000	0.0000	0.00011	2.06
5	5.00002	5.0000	0.0000	0.00011	2.06
10	10.00001	10.0000	0.0000	0.00011	2.05
50	50.00003	50.0000	0.0000	0.00013	2.03
100	100.00004	100.0001	0.0001	0.00018	2.00
150	150.00007	150.0001	0.0000	0.00024	2.00
200	200.00006	200.0002	0.0001	0.00031	2.00

Weighing Range 2

Normal Value (g)	Standard Value (g)	Indication (g)	Error of Indication (g)	Expanded Uncertainty (g)	Factor k

The given extended measurement uncertainty is the standard uncertainty of the measurement multiplied by cover factor k as per listed in table above, which corresponds to a confidence level of about 95%

CERTIFICATE OF CALIBRATION



Result of Calibration

Certificate no. PST-0001-22

Page no. 3 of 3

3. Eccentricity

Test load at least 1/3 of the maximum capacity, typically placed between 1/2 and 1/3 of the distance from the centre of the load receptor to the edge.



Weighing Range 1

Test Load : 100 (g)

Position	Indication (g)
1	100.0001
2	100.0001
3	100.0002
4	100.0001
5	100.0002
Max.Deviation	0.0001

Weighing Range 2

Test Load : (g)

Position	Indication (g)
1	
2	
3	
4	
5	
Max.Deviation	

Standard methode

The calibration was performed by using calibration laboratory's In-house calibration methode : CP-M-001 based on "UKAS LAB 14 : Calibration of weighing machine" : edition 6 | October 2019

Reference standards instrument

Instrument	OIML Class	S/N	Certificate No.	Due Date
Standard Weight Set	E2	4000021952	MM-0183-20	December 8, 2022
Standard Weight Set	-	-	-	-
Standard Weight Set	-	-	-	-
Standard Weight Set	-	-	-	-

Measurement Uncertainty

The given measurement uncertainty is the standard of the measurement multiplied by an extension factor k which corresponds to a confidence level of about 95% for a normal distribution. The standard uncertainty was calculated according to M3003

Traceability : The measurement is traceable to national standard, which realize the physical unit of measurement (SI)

- National Institute of Metrology (Thailand) through Calibration Laboratory

END OF REPORT

Calibration Data of NOx Analyzer

Analyzer Performance Test


Equipment	Gas Analyzer (NOx)	Customer Name	โพธิ์เทพย์ คอนซัลแตนต์
Manufacture	HORIBA	Location	Envi Research
Model	APNA-360	Scientist	Panupon
Serial No.	EYC70000	Calibration Date	May 9, 2022
Analyzer Unit	ppm	Time	1:31 PM

Instruments for Calibration

Instruments	Manufacture	Model	Serial Number
Zero Air Supply	Thermo Env.	111	0700419829
Dynamic Dilution Calibrator	Tanabyte	300T	0172
Standard Gas Components	CO = 4,516 ppm		
Cylinder No : EB0123013	NO = 55.3 ppm		
Expire Date : Oct 22, 2027	SO ₂ = 54.9 ppm		

Single Point Calibration

Standard Gas	Standard Gas Value	Analyzer Value								% Abs Error
		NO _x (ppb)		NO (ppb)		NO ₂ (ppb)		Stability		
		Before	After	Before	After	Before	After	Before	After	
Zero	0	0.2	0.0	0.6	0.0	-0.4	0.0	-	-	-
Span	400	386.7	400.0	385.3	400.0	1.4	0.0	-	-	3.7

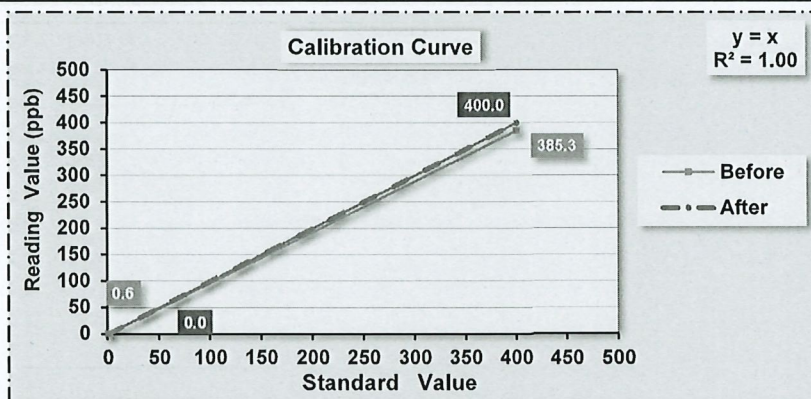

STATUS TEST AND VALIDATION OF NOx ANALYZER MODEL APNA-360

Parameter	Unit	Observed Value		Nominal Range
		Before Adjust	After Adjust	
Range	ppm	0.5	0.5	0.1 - 1.0 Standard
Signal NO	mV	3.5	3.9	Voltage of the measured NO value
Signal NOx	mV	6.4	3.7	Voltage of the measured NOx value
Detector	kPa	86.7	872.0	(Present Air Pressure/101.3 x100 - 20) \pm 4
Sample Flow	LPM	0.7	0.7	1.1 \pm 0.3
NO Slope	-	1.00000	1.12690	0.50000 - 2.0000
NOx Slope	-	1.00000	1.14580	0.50000 - 2.0000
Motherboard Status	-	OK	OK	OK
Alarm Detected	-	None	None	None

Calibrate By :

(MR.PANUPON PODANG)
May 9, 2022



Checked By :

(MS.SUTATIP IM-NOI)
May 9, 2022

Calibration Data of NOx Analyzer

Analyzer Performance Test


Equipment	Gas Analyzer (NOx)	Customer Name	โพธิ์เพชร คอนซัลแตนต์
Manufacture	API	Location	Envi Research
Model	200A	Scientist	Panupon
Serial No.	56	Calibration Date	April 18, 2022
Analyzer Unit	ppb	Time	11:07 AM

Instruments for Calibration

Instruments	Manufacture	Model	Serial Number
Zero Air Supply	Thermo Env.	111	0700419829
Dynamic Dilution Calibrator	Tanabyte	300T	0172
Standard Gas Components	CO = 4,516 ppm		
Cylinder No : EB0123013	NO = 55.3 ppm		
Expire Date : Oct 22, 2027	SO ₂ = 54.9 ppm		

Single Point Calibration

Standard Gas	Standard Gas Value	Analyzer Value								% Abs Error
		NO _x (ppb)		NO (ppb)		NO ₂ (ppb)		Stability		
		Before	After	Before	After	Before	After	Before	After	
Zero	0	1.3	0.0	0.3	0.0	1.0	0.0	-	-	-
Span	400	413.0	405.0	411.8	400.0	1.2	5.0	-	-	3.0

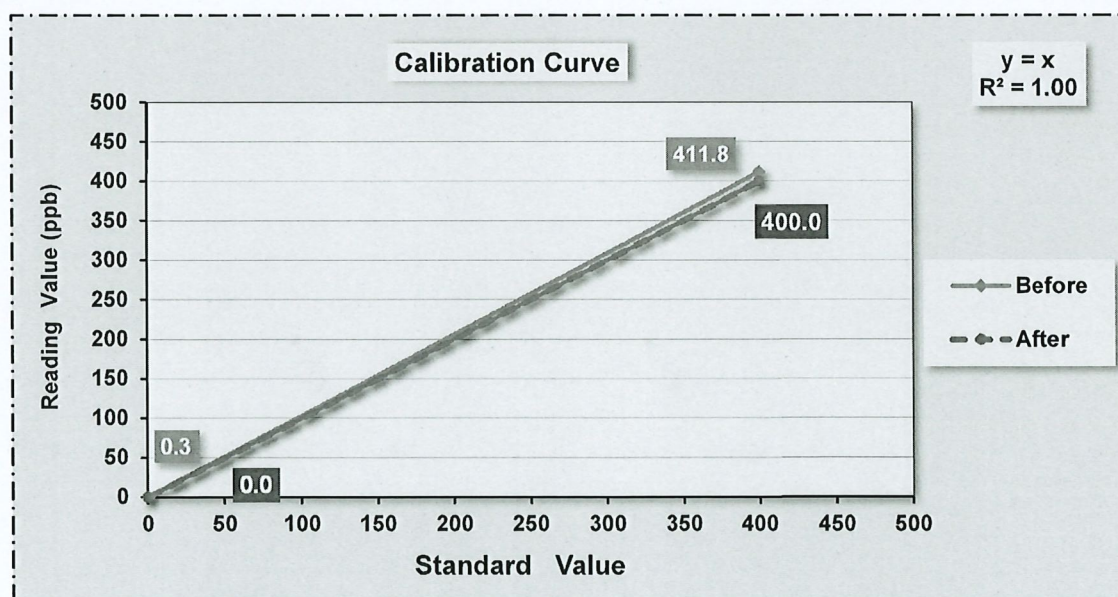

STATUS TEST AND VALIDATION OF NO_x ANALYZER MODEL 200A

Parameter	Display As	Unit	Observed Value		Nominal Range
			Before Adjust	After Adjust	
Range	RANGE	ppb	500	500	0 - 500 standard
Stability	STABIL	ppb	0.20	0.20	< 2 with zero air
Sample Flow	SAMP FL	cc / min	479.00	474.00	500 +/- 50
Ozone Flow	OZONE FL	cc / min	82.00	83.00	80 +/- 10
PMT signal	PMT	mV	49.00	24.00	0 to 5,000
Auto - Zero	AZERO	mV	16.8	13.7	-20 to 150
High Voltage Power Supply	HVPS	V	758.00	758.00	450 to 900
Reaction Cell Temperature	RCELL TEMP	°C	50.00	50.50	50 +/- 1
Box Temperature	BOX TEMP	°C	39.80	36.70	Ambient temp.+3 / -7
PMT Temperature	PMT TEMP	°C	6.40	6.50	7 +/- 1
Converter Temperature	MOLY TEMP	°C	314.70	314.50	315 +/- 5
Reaction Cell Pressure	RCEL	In - Hg - A	10.00	10.00	2 to 10 (Constant)
Sample Pressure	SAMP	In - Hg - A	30.60	31.20	Ambient - 1 (Constant)
NO _x Slope	NO _x SLOPE	-	1.466	1.223	1.000 +/- 0.300
NO _x Offset	NO _x OFFSET	mV	10.10	-6.80	0 +/- 20
NO Slope	NO SLOPE	-	1.420	1.198	1.000 +/- 0.300
NO Offset	NO OFFSET	mV	0.50	-5.50	0 +/- 20

Calibrate By :

(MR.PANUPON PODANG)

April 18, 2022



Checked By :

(MS.SUTATIP IM-NOI)

April 18, 2022

Calibration Data of NOx Analyzer

Analyzer Performance Test


Equipment	Gas Analyzer (NOx)	Customer Name	โพธิ์เขียว คอนซัลแตนต์
Manufacture	API	Location	Envi Research
Model	200A	Scientist	Panupon
Serial No.	1975	Calibration Date	July 18, 2022
Analyzer Unit	ppb	Time	11:19 AM

Instruments for Calibration

Instruments	Manufacture	Model	Serial Number
Zero Air Supply	Thermo Env.	111	0700419829
Dynamic Dilution Calibrator	Tanabyte	300T	0172
Standard Gas Components	CO = 4,516 ppm		
Cylinder No : EB0123013	NO = 55.3 ppm		
Expire Date : Oct 22, 2027	SO ₂ = 54.9 ppm		

Single Point Calibration

Standard Gas	Standard Gas Value	Analyzer Value								% Abs Error
		NO _x (ppb)		NO (ppb)		NO ₂ (ppb)		Stability		
		Before	After	Before	After	Before	After	Before	After	
Zero	0	-15.7	0.0	-2.8	0.0	-12.9	0.0	-	-	-
Span	400	403.3	405.0	390.9	400.0	12.4	5.0	-	-	2.3

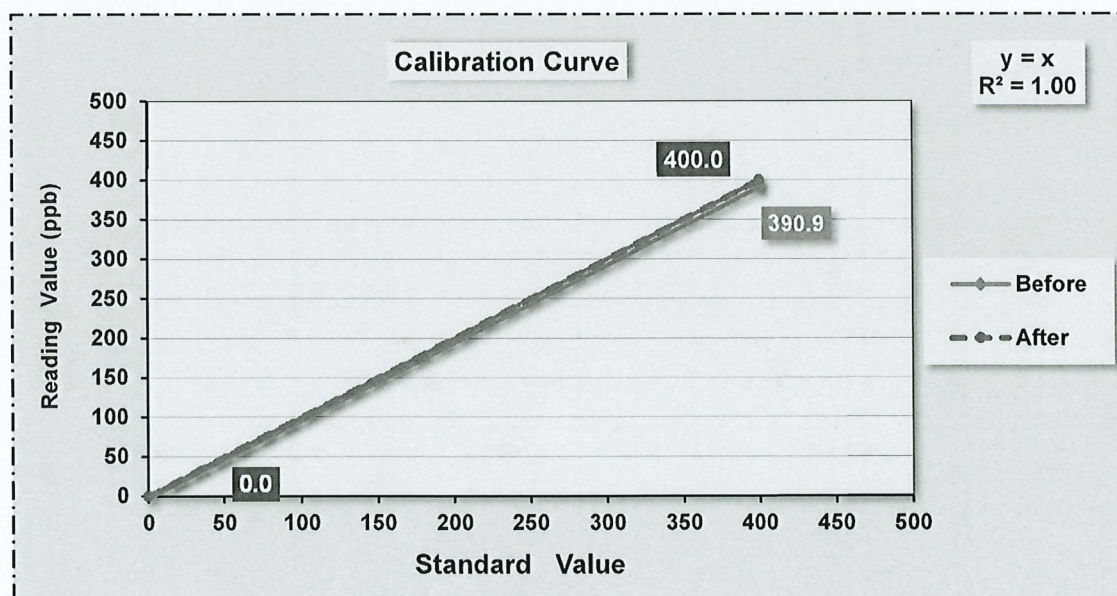

STATUS TEST AND VALIDATION OF NO_x ANALYZER MODEL 200A

Parameter	Display As	Unit	Observed Value		Nominal Range
			Before Adjust	After Adjust	
Range	RANGE	ppb	500	500	0 - 500 standard
Stability	STABIL	ppb	0.20	0.40	< 2 with zero air
Sample Flow	SAMP FL	cc / min	456.00	480.00	500 +/- 50
Ozone Flow	OZONE FL	cc / min	77.00	79.00	80 +/- 10
PMT signal	PMT	mV	52.90	39.40	0 to 5,000
Auto - Zero	AZERO	mV	37.6	34.8	-20 to 150
High Voltage Power Supply	HVPS	V	790.00	790.00	450 to 900
Reaction Cell Temperature	RCELL TEMP	°C	50.20	49.80	50 +/- 1
Box Temperature	BOX TEMP	°C	34.90	29.60	Ambient temp.+3 / -7
PMT Temperature	PMT TEMP	°C	7.00	7.30	7 +/- 1
Converter Temperature	MOLY TEMP	°C	314.30	314.40	315 +/- 5
Reaction Cell Pressure	RCEL	In - Hg - A	10.00	10.00	2 to 10 (Constant)
Sample Pressure	SAMP	In - Hg - A	30.80	31.20	Ambient - 1 (Constant)
NO _x Slope	NO _x SLOPE	-	0.955	0.945	1.000 +/- 0.300
NO _x Offset	NO _x OFFSET	mV	28.30	-4.70	0 +/- 20
NO Slope	NO SLOPE	-	0.870	0.907	1.000 +/- 0.300
NO Offset	NO OFFSET	mV	2.60	-3.70	0 +/- 20

Calibrate By :

(MR.PANUPON PODANG)

July 18, 2022



Checked By :

(MS.SUTATIP IM-NOI)

July 18, 2022

Calibration Data of SO₂ Analyzer

Analyzer Performance Test


Equipment	Gas Analyzer (SO ₂)	Customer Name	โพธิ์เกียรติ์ คอนซัลแตนต์
Manufacture	Thermo	Location	Envi Research
Model	43i-BNSAA	Scientist	Panupon
Serial No.	CM14430004	Calibration Date	April 10, 2022
Analyzer Unit	ppb	Time	12:55 PM

Instruments for Calibration

Instruments	Manufacture	Model	Serial Number
Zero Air Supply	Thermo Env.	111	0700419829
Dynamic Dilution Calibrator	Tanabyte	300T	0172
Standard Gas Components	CO = 4,516 ppm		
Cylinder No : EB0123013	NO = 55.3 ppm		
Expire Date : Oct 22, 2027	SO ₂ = 54.9 ppm		

Single Point Calibration

Standard Gas	Standard Gas Value	Analyzer Value (ppb)		Stability		% Abs Error
		Before	After	Before	After	
Zero	0	1.2	0.0	-	-	-
Span	400	397.0	400.0	-	-	0.8

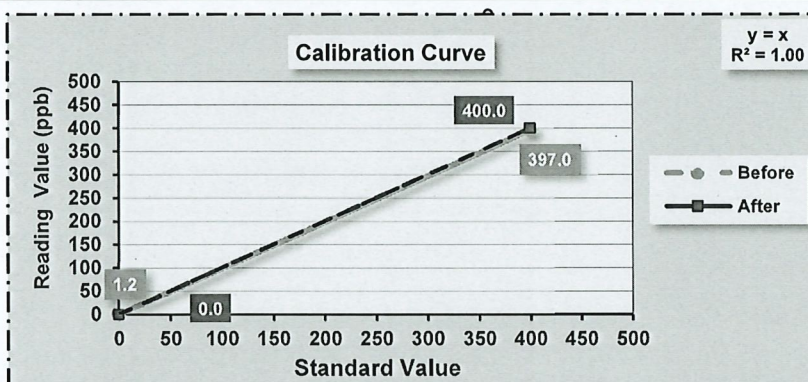

STATUS TEST AND VALIDATION OF SO₂ ANALYZER MODEL 43i-BNSAA

Parameter	Display As	Unit	Observed Value		Nominal Range
			Before Adjust	After Adjust	
Range	RANGE	ppb	500	500	0 - 500 standard
Internal Temperature	INTERNAL	°C	33.2	33.0	8.0 °C to 45.0 °C
Chamber Temp	CHAMBER	°C	45.1	44.9	43.0 °C to 47.0 °C
Pressure	PRESSURE	mmHg	733.7	733.8	400.0 to 1,000
Sample Flow	SAMP FLOW	LPM	0.410	0.411	0.350 to 0.750
Lamp Intensity	LAMP INTENSITY	%	93	94	20 to 100
Lamp Voltage	LAMP VOLTAGE	V	811	811	500 to 1200
SO ₂ Concentration	SO ₂ CONCENTRATION	ppb	3.2	2.6	0 to 10,000
Motherboard Status	MOTHERBOARD STATUS	-	OK	OK	OK
Interface Status	INTERFACE STATUS	-	OK	OK	OK

Calibrate By :

(MR.PANUPON PODANG)

April 10, 2022



Checked By :

(MS.SUTATIP IM-NOI)

April 10, 2022

Calibration Data of SO₂ Analyzer

Analyzer Performance Test


Equipment	Gas Analyzer (SO ₂)	Customer Name	โพธิ์เกียรติ์ คอนซัลแตนต์
Manufacture	Thermo	Location	Envi Research
Model	43C	Scientist	Panupon
Serial No.	0335804029	Calibration Date	April 10, 2022
Analyzer Unit	ppb	Time	12:55 PM

Instruments for Calibration

Instruments	Manufacture	Model	Serial Number
Zero Air Supply	Thermo Env.	111	0700419829
Dynamic Dilution Calibrator	Tanabyte	300T	0172
Standard Gas Components	CO = 4,516 ppm		
Cylinder No : EB0123013	NO = 55.3 ppm		
Expire Date : Oct 22, 2027	SO ₂ = 54.9 ppm		

Single Point Calibration

Standard Gas	Standard Gas Value	Analyzer Value (ppb)		Stability		% Abs Error
		Before	After	Before	After	
Zero	0	-0.6	0.0	-	-	-
Span	400	397.0	400.0	-	-	0.8

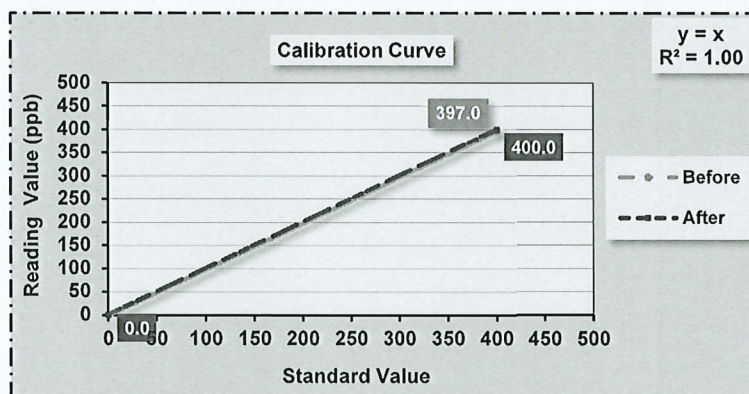

STATUS TEST AND VALIDATION OF SO₂ ANALYZER MODEL 43C

Parameter	Display As	Unit	Observed Value		Nominal Range
			Before Adjust	After Adjust	
Range	RANGE	ppb	500	500	0 - 500 standard
Internal Temperature	INTERNAL	°C	33.6	33.7	8.0 °C to 47.0 °C
Chamber Temp	CHAMBER	°C	44	43.9	43.0 °C to 47.0 °C
Pressure	PRESSURE	mmHg	723.2	723.3	400.0 to 1,000
Sample Flow	SAMP FLOW	LPM	0.639	0.640	0.350 to 1.000
Lamp Intensity	INTENSITY	Hz	26,335	26,412	20,000 to 50,000
Lamp Voltage	LAMP VOLTAGE	V	810	810	750 to 1,200
SO ₂ Concentration	SO ₂ CONCENTRATION	ppb	0.7	1.3	0 to 10,000
Motherboard Status	MOTHERBOARD STATUS	-	OK	OK	OK
Interface Status	INTERFACE STATUS	-	OK	OK	OK

Calibrate By :

(MR.PANUPON PODANG)
April 10, 2022

envi research
Checked By :
ENVIRONMENT RESEARCH & TECHNOLOGY CO., LTD.

(MS.SUTATIP IM-NOI)
April 10, 2022

Calibration Data of SO₂ Analyzer

Analyzer Performance Test


Equipment	Gas Analyzer (SO ₂)	Customer Name	โพธิ์เกียรติ์ คอนซัลแตนต์
Manufacture	Thermo	Location	Envi Research
Model	43C	Scientist	Panupon
Serial No.	73370-373	Calibration Date	April 18, 2022
Analyzer Unit	ppb	Time	11:34 AM

Instruments for Calibration

Instruments	Manufacture	Model	Serial Number
Zero Air Supply	Thermo Env.	111	0700419829
Dynamic Dilution Calibrator	Tanabyte	300T	0172
Standard Gas Components	CO = 4,516 ppm		
Cylinder No : EB0123013	NO = 55.3 ppm		
Expire Date : Oct 22, 2027	SO ₂ = 54.9 ppm		

Single Point Calibration

Standard Gas	Standard Gas Value	Analyzer Value (ppb)		Stability		% Abs Error
		Before	After	Before	After	
Zero	0	-3.0	0.0	-	-	-
Span	400	387.0	400.0	-	-	3.3

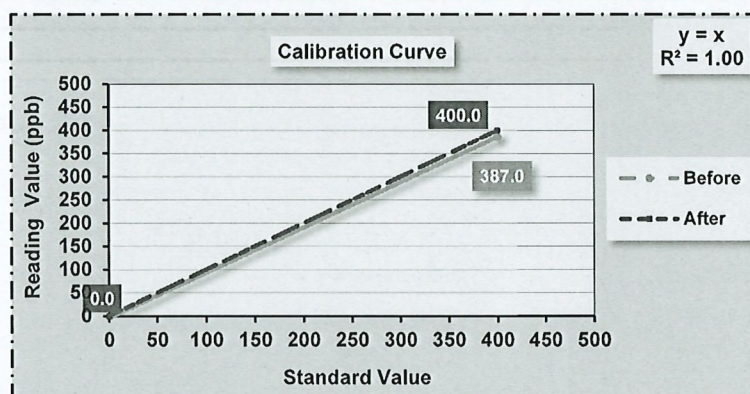

STATUS TEST AND VALIDATION OF SO₂ ANALYZER MODEL 43C

Parameter	Display As	Unit	Observed Value		Nominal Range
			Before Adjust	After Adjust	
Range	RANGE	ppb	500	500	0 - 500 standard
Internal Temperature	INTERNAL	°C	40.3	39.9	8.0 °C to 47.0 °C
Chamber Temp	CHAMBER	°C	46	46	43.0 °C to 47.0 °C
Pressure	PRESSURE	mmHg	706.7	706.7	400.0 to 1,000
Sample Flow	SAMP FLOW	LPM	0.627	0.627	0.350 to 1.000
Lamp Intensity	INTENSITY	Hz	22,934	23,770	20,000 to 50,000
Lamp Voltage	LAMP VOLTAGE	V	959	960	750 to 1,200
SO ₂ Concentration	SO ₂ CONCENTRATION	ppb	-3.4	1.0	0 to 10,000
Motherboard Status	MOTHERBOARD STATUS	-	OK	OK	OK
Interface Status	INTERFACE STATUS	-	OK	OK	OK

Calibrate By :

(MR.PANUPON PODANG)
April 18, 2022



Checked By :

(MS.SUTATIP IM-NOI)
April 18, 2022

Calibration Data of CO Analyzer

Analyzer Performance Test


Equipment	Gas Analyzer (CO)	Customer Name	โพธิ์เกียรติ์ คอนซัลแตนต์
Manufacture	HORIBA	Location	Envi Research
Model	APMA-360 CE	Scientist	Panupon
Serial No.	41346760054	Calibration Date	April 11, 2022
Analyzer Unit	ppm	Time	1:23 PM

Instruments for Calibration

Instruments	Manufacture	Model	Serial Number
Zero Air Supply	Thermo Env.	111	0700419829
Dynamic Dilution Calibrator	Tanabyte	300	0172
Standard Gas Components	CO = 4,516 ppm		
Cylinder No : EB0123013	NO = 55.3 ppm		
Expire Date : Oct 22, 2027	SO ₂ = 54.9 ppm		

Single Point Calibration

Standard Gas	Standard Gas Value	Analyzer Value (ppm)		Stability		% Abs Error
		Before	After	Before	After	
Zero	0	0.36	0.00	-	-	-
Span	40	40.47	40.05	-	-	1.05

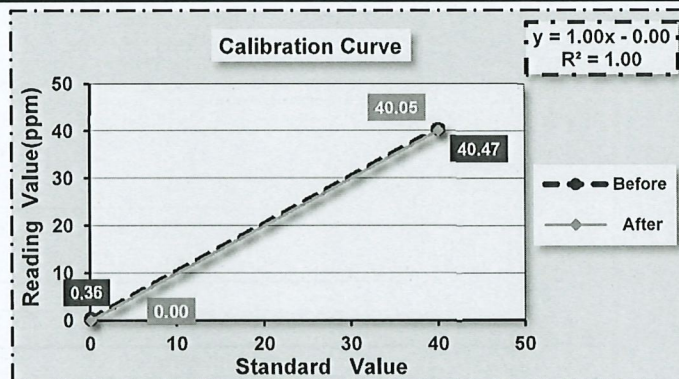

STATUS TEST AND VALIDATION OF CO ANALYZER MODEL APMA-360CE

Parameter	Unit	Observed Value		Nominal Range
		Before Adjust	After Adjust	
SIGNAL (MAIN)	mV	10.1	3.1	Voltage of the measured CO Value
SIGNALI (COMP)	mV	0.0	1.8	Voltage of the interference component Value
CELL	°C	39.1	39.1	Ambient + (5 to 15 °C)
SAMPLE	L/min	1.2	1.0	1 L/min to 2 L/min
OVER FLOW	LPM	0.0	0.0	< 1.2

Calibrate By :

(MR.PANUPON PODANG)
April 11, 2022



Checked By :

(MS.SUTATIP IM-NOI)
April 11, 2022

Calibration Data of CO Analyzer

Analyzer Performance Test


Equipment	Gas Analyzer (CO)	Customer Name	โพธิ์เกียรติ์ คอนซัลแตนต์
Manufacture	HORIBA	Location	Envi Research
Model	APMA-370	Scientist	Panupon
Serial No.	C06YT0NC	Calibration Date	April 22, 2022
Analyzer Unit	ppm	Time	11:10 AM

Instruments for Calibration

Instruments	Manufacture	Model	Serial Number
Zero Air Supply	Thermo Env.	111	0700419829
Dynamic Dilution Calibrator	Tanabyte	300T	0172
Standard Gas Components	CO = 4,487 ppm		
Cylinder No : EB0123013	NO = 46.1 ppm		
Expire Date : Oct 22, 2027	SO ₂ = 46.0 ppm		

Single Point Calibration

Standard Gas	Standard Gas Value	Analyzer Value (ppm)		Stability		% Abs Error
		Before	After	Before	After	
Zero	0	-0.03	0.00	-	-	-
Span	40	39.57	40.00	-	-	1.08

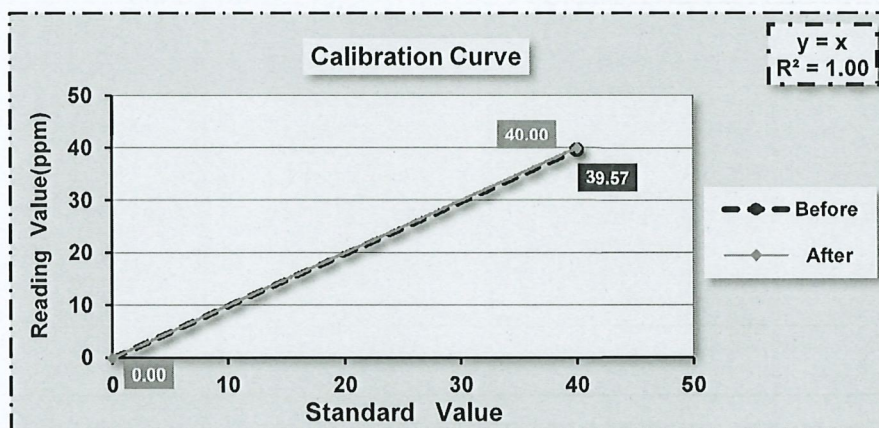

STATUS TEST AND VALIDATION OF CO ANALYZER MODEL APMA-370

Parameter	Unit	Observed Value		Nominal Range
		Before Adjust	After Adjust	
SIGNAL(MAIN)	mV	1.1	1.8	Voltage of the measured CO Value
SIGNAL (COMP)	mV	0.1	0.3	Voltage of the interference component Value
CELL	°C	33.1	32.8	Ambient + (5 to 10 C)
PUMP	kpa	41.2	40.9	less than 65
AMBIENT	kpa	101.6	101.3	Atmospheric pressure
DC 24V	mV	24.0	24.0	24+/- 0.5 V
DC 5V	mV	4.9	4.9	5+/- 0.5 V

Calibrate By :

(MR.PANUPON PODANG)
April 22, 2022



Checked By :

(MS.SUTATIP IM-NOI)
April 22, 2022

Calibration Data of CO Analyzer

Analyzer Performance Test


Equipment	Gas Analyzer (CO)	Customer Name	โพธิ์เพชร คอนซัลแตนต์
Manufacture	HORIBA	Location	Envi Research
Model	APMA-370	Scientist	Panupon
Serial No.	WNTLD9N8	Calibration Date	April 21, 2022
Analyzer Unit	ppm	Time	1:24 PM

Instruments for Calibration

Instruments	Manufacture	Model	Serial Number
Zero Air Supply	Thermo Env.	111	0700419829
Dynamic Dilution Calibrator	Tanabyte	300T	0172
Standard Gas Components	CO = 4,516 ppm		
Cylinder No : EB0123013	NO = 55.3 ppm		
Expire Date : Oct 22, 2027	SO ₂ = 54.9 ppm		

Single Point Calibration

Standard Gas	Standard Gas Value	Analyzer Value (ppm)		Stability		% Abs Error
		Before	After	Before	After	
Zero	0	-0.29	0.00	-	-	-
Span	40	40.03	40.00	-	-	0.08

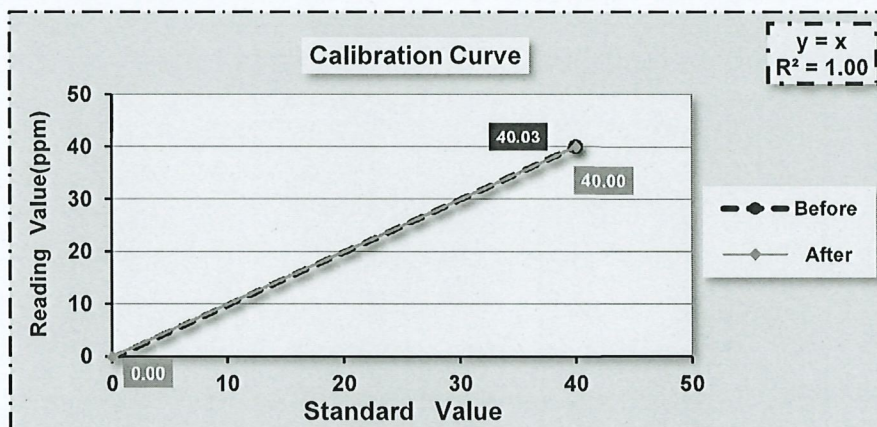

STATUS TEST AND VALIDATION OF CO ANALYZER MODEL APMA-370

Parameter	Unit	Observed Value		Nominal Range
		Before Adjust	After Adjust	
SIGNAL(MAIN)	mV	2.3	17.8	Voltage of the measured CO Value
SIGNAL (COMP)	mV	3.9	10	Voltage of the interference component Value
CELL	°C	32.4	32.3	Ambient + (5 to 10 C)
PUMP	kpa	55.7	55.5	less than 65
AMBIENT	kpa	101.3	101.1	Atmospheric pressure
DC 24V	mV	23.9	23.9	24+/- 0.5 V
DC 5V	mV	4.9	4.9	5+/- 0.5 V

Calibrate By :

(MR.PANUPON PODANG)
April 21, 2022



Checked By :

(MS.SUTATIP IM-NOI)
April 21, 2022

Signature of MS. SUTATIP IM-NOI

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number:	E04NI99E15A0292	Reference Number:	160-401604495-1
Cylinder Number:	EB0123013	Cylinder Volume:	144.4 Cubic Feet
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2015 PSIG
PGVP Number:	A12019	Valve Outlet:	660
Gas Code:	CO,NO,NOX,SO2,BALN	Certification Date:	Oct 22, 2019

Expiration Date: Oct 22, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	55.00 PPM	55.27 PPM	G1	+/- 0.8% NIST Traceable	10/14/2019, 10/22/2019
NITRIC OXIDE	55.00 PPM	55.27 PPM	G1	+/- 0.8% NIST Traceable	10/14/2019, 10/22/2019
SULFUR DIOXIDE	55.00 PPM	54.93 PPM	G1	+/- 0.9% NIST Traceable	10/14/2019, 10/22/2019
CARBON MONOXIDE	4500 PPM	4516 PPM	G1	+/- 0.6% NIST Traceable	10/14/2019
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	13010429	KAL004123	97.6 PPM NITRIC OXIDE/NITROGEN	+/- 0.8%	Jul 23, 2025
NTRM	13010429	KAL004123	97.6 PPM NOx/NITROGEN	+/- 0.8%	Jul 23, 2025
NTRM	16010235	KAL004419	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Dec 23, 2021
NTRM	08012318	KAL004620	4857 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Jun 07, 2024

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
MKS FTIR - CO - 000928781	FTIR	Sep 26, 2019
MKS FTIR - NO - 000928781	FTIR	Oct 18, 2019
MKS FTIR - NOx - 000928781	FTIR	Oct 18, 2019
MKS FTIR - SO2 - 000928781	FTIR	Oct 03, 2019

Triad Data Available Upon Request

NOTES: Gross Weight: 28.0 Kg, Net Weight: 4.6 Kg.



[Signature]
Approved for Release

Support Equipment Type : Sound Level Calibrator

Manufacture : LARSON DAVIS

Model : CAL200

Serial No. : 8413

Range of Calibrator

- Sound Pressure Level : 93.6 dB.

- **Frequency** : 1,000 Hz.

Calibrated By : Mr.Akarawat Kochabog

Calibration Date : May 19, 2022

Customer Name : บริษัท โปร้เทียร์ คอนซัลแตนต์ จำกัด: โครงการ อาคารอยู่อาศัยสวัสดิการสำหรับพนักงานหญิง
(ปราจีนบุรี) ของบริษัท หยงซิง สตีล (ไทยแลนด์) จำกัด

Checked By

Prayun.
.....
Mr. Prayun Detkla
Technician

envi research
Approved
ENVIRONMENT RESEARCH & TECHNOLOGY CO., LTD.

Approved By

Ms.Sutatip Im-noi
Environmental Scientist



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0209

MTC No. EEL. BP. 129/1264

CALIBRATION CERTIFICATE

Submitted by : Environment Research & Technology Co., Ltd.
Address : 25/114 Moo 6, Soi Chinaket 1, Ngamwongwan Road, Toongsonghong, Laksi, Bangkok 10210.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :
Description : Precision Acoustic Calibrator
Manufacturer : Larson Davis
Model : CAL 200
Serial No. : 8413

Ambient Environment
Temperature : $(23 \pm 3) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$
Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N 4106495.
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 29 Dec. 2021

Date of Calibration : 6 Jan. 2022

1 / 3

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpal@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : surnalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0209

MTC No. EEL. BP. 129/1264

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μPa at 1000 Hz

Acoustic Output in dB re 20 μPa , Corrected to Reference Conditions: 101.325 kPa, 23.0 $^\circ\text{C}$ and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.60	-0.40	± 0.10	$\pm 0.40 \text{ dB}$

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	± 1.5	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	2.20	± 0.55	$\pm 3.0\%$

- Note :** 1. No adjustment.
2. The calibrator pressure correction was not included.
3. The microphone volume correction was included at the level of 0.26 dB from manual.

Date of Calibration : 6 Jan. 2022

2 / 3

1

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpal@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : surnalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0209

MTC No. EEL. BP. 129/1264

Nominal Output of Unit Under Test = 114 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	113.61	-0.39	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	± 1.5	±1.0%

3. Total Distortion


Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	0.36	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was included at the level of 0.26 dB from manual.

Calibrated by :


(Mr. Tawikiat Iamsamran)

Approved by :


(Mr. Prawate Kluaypa)

Acting Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 6 Jan. 2022

Date of Issue : 7 Jan. 2022

Ref : 2011264122905422002

3 / 3

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL-MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
53/44 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CH13
Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Eutech
Model : pHTestr 30
Serial No. : 3011826
ID No. : NO.23
Condition As-Received: Used Item
Received Date : 29 December 2021
Calibration Date : 05 January 2022
Reference : 2112-0752WN-9
Submitted by : Environment Research & Technology Company Limited.
25/114 Moo 6, Soi Chinaket 1, Ngamwongwan Road,
Toongsonghong, Laksi, Bangkok 10210
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard
voltage calibrator and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with standard thermometer

Calibrated by : Walalak Sirithean

Approved by : 
Approved Signatory

(/) Malee Butkruea
() Saithip Meangmai
() Warakorn Lernagatrakul

Issue Date : 7 January 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 22CH13
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Ref. Standard Thermometer	4982054	110RC044	2111201	26 Oct 2022

This certification is traceable to the International System of Unit maintained at:-
- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	761016	02 Aug 2023
pH 6.982	CPA chem	761017	02 Aug 2022
pH 10.015	CPA chem	761018	02 Aug 2022

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor k
pH Electrode S/N.: 3011826	4.008	4.00	N/A	0.0085	2.05
	6.982	6.97	N/A	0.011	2.00
	10.015	10.02	N/A	0.0096	2.00

Remark - pH meter does not have voltage mode.
- Can not connect the BNC because the plug does not match with the socket.
- N/A = Not Available





Cert.No.: 22CH13

Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -
- Serial No. : 3011826
Dimension of probe;
- Length : 36 mm.
- Diameter : 6 mm.
- Immersion Depth : 33 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor <i>k</i>
25.0	24.998	25.3	0.302	0.13	2.00
30.0	29.998	30.3	0.302	0.13	2.00
35.0	35.002	35.3	0.298	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Madu.



CRYSTAL CALIBRATION SALES AND SERVICE CO., LTD.
45/48 Soi Salathammassop31, Salathammassop Rd.,
Salathammassop, Thawewatthana, Bangkok 10170 Thailand
Tel : 0-2408-8474-5 Fax : 0-2408-8477 Email : info@crystalcal.com www.crystalcal.com



CERTIFICATE OF CALIBRATION

Issue Date : 28 December 2021
Certificate No. : 21-1224-004
Work Order No. : 21/1224

Customer Name : Environment research & Technogy Co., Ltd.
25/114 Moo6 Soi Chinaket1, Ngamwongwan Road,
Toongsonghong, Laksi, Bangkok 10210
Date of Received : 15 December 2021
Date of Calibration : 15 December 2021

Instrument Details : Description : Temperature Controlled Enclosures [Incubator]
Manufacturer : Accuplus
Model : Smart i250
Serial No. : 2059-0218-0002
ID No. : ERTC-L-IN-143
Resolution : 0.1 °C
Location : Laboratory

Calibration Method : This instrument was calibrated by insert standard thermometer into the chamber according to calibration procedure no. CWI-T-10 follow up to TLAS G-20-1/02-08
(E) : Guidelines for Calibration and Checks of Temperature Controlled Enclosures.

Environmental Conditions :

Temperature : Area Monitoring between 15°C to 40°C
Humidity : Area Monitoring between 30%RH to 85%RH
Line Voltage : Area Monitoring 220 VAC \pm 10%

Traceability of Measurement :

This certificate of calibration documents the traceability to national standard, which realize the unit of measurement according to the International system of Units (SI) and The temperature scale in use at this laboratory is The International Temperature scale of 1990.

Calibrated by : Mr. Sitthisak Tonglim
Calibration Engineer

Approved by :
(Mr. Anuwat Yaklermjit)
Laboratory Manager

This certificate may not be reproduced other than in full except with the prior written approval of Crystal Calibration Sales and Service co., Ltd.

Crystal Calibration Sales and Service Co., Ltd.

45/48 Salathammassop 31, Salathammassop Rd., Salathammassop, Thawewatthana, Bangkok 10170

Phone : 0-2408-8474 Fax : 0-2408-8477 http://www.crystalcal.com Email : info@crystalcal.com



PAGE 1/3

15-1-65



CRYSTAL CALIBRATION SALES AND SERVICE CO., LTD.
45/48 Soi Salathammassop31, Salathammassop Rd.,
Salathammassop, Thawewatthana, Bangkok 10170 Thailand
Tel : 0-2408-8474-5 Fax : 0-2408-8477 Email : info@crystalcal.com www.crystalcal.com



CERTIFICATE OF CALIBRATION

Issue Date : 28 December 2021
Certificate No. : 21-1224-004
Work Order No. : 21/1224

Details of Calibration

1. Reference Standards Instrument

Instrument	Model	Serial No./Ins No.	Certificate No.	Due Date
Data Acquisition unit	34972A	MY57006241	21-719-014	03 September 2022
Sensor type	RTD	RTD# 101-109	21-719-014	03 September 2022

2. Certificate traceable : This certificate traceable to The International System of Unit refer to
Crystal Calibration Sales and Service Co., Ltd. , NAC Calibration No. 0260

3. Condition of item : Used

4. Calibration site : On - Site

5. Result of Calibration : Without adjustment

6. Evaluate Condition : Time Constant : - Hour 50 Minute At cal. point 20 °C
Air vent : Off
Fan speed status : Fixed Fan Speed

7. Calibration note : The results reported in this certificate refer to the condition of instrument on
the process into the steady state of chamber

8. Sensors Installation Diagram : When ; Sensor installation location in Chamber ϕ Working Space
A = Distance between sensor and wall of chamber is 5 cm

9. Dimensions of chamber : W = 0.5 m ; D = 0.5 m ; H = 0.9 m

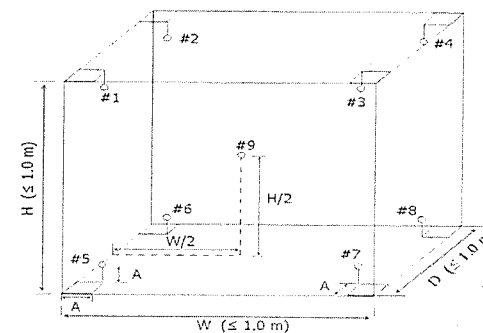


Diagram of Chamber

15-1-65 PAGE 2/3



CRYSTAL CALIBRATION SALES AND SERVICE CO., LTD.

45/48 Soi Salathammassop31, Salathammassop Rd.,
Salathammassop, Thawewattana, Bangkok 10170 Thailand

Tel : 0-2408-8474-5 Fax : 0-2408-8477 Email : info@crystalcal.com www.crystalcal.com



CERTIFICATE OF CALIBRATION

Certificate No. : 21-1224-004

Issue Date : 28 December 2021

Work Order No. : 21/1224

Result of Temperature Distribution and Performance Check

Table1 : Reporting of Temperature Distribution

Calibration point (°C)	Average Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	#1	#2	#3	#4	#5	#6	#7	#8	#9	
20.0	20.26	20.08	20.22	20.11	20.18	20.12	20.09	20.16	19.91	0.60

Table 2 : Reporting of Performance check

Indicator Set Point (°C)	Indicator Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
	MAX	MIN	Average			
20.0	20.0	19.6	19.9	0.39	0.58	1.03

Note

Customer would like to find internal temperature in chamber and this report customer request and accepted in certificate

The reference sensor is preferably located of the geometric center of chamber

The measured temperature data readout by software "Benchlink Datalogger 3"

The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.

Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature

at the reference location which are observed at the same time or at as close an observation time as possible

to determine the temperature pattern or homogeneity within the chamber under steady state conditions.

Overall Variation - The difference of the maximum and minimum measured temperatures throughout observation time.

Indicating Temperature - the average reading of indicating device that forms the integral part of the enclosure.

This result of calibration was found accurate as shown on date and place of calibration only.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$ providing a level of confidence of approximately 95%.

--END--


13-1-65 PAGE 3/3

Mettler-Toledo (Thailand) Ltd.
846/4 - 846/5 Laksalle Rd., Bangna Tai Sub-District
Bangna District, Bangkok 10260
+66 2723 0382
MT-TH.ServiceSupport@mt.com



Accuracy Calibration Certificate

Customer

Company: ENVIRONMENT RESEARCH&TECHNOLOGY CO., LTD.
Address: 25/114 Moo 6, Soi Chinaket 1, Ngamwongwan Rd., Toongsoengho
City: Laksi Contact: Ramita Tsengthai
Zip / Postal: 10210
State / Province: Bangkok
Order Number: 

Weighing Device

Manufacturer: Mettler Toledo Instrument Type: Weighing Instrument
Model: MS204S/01 Asset Number: ERTC-L-IN-088
Serial No.: B334691537 Terminal Model: N/A
Building: N/A Terminal Serial No.: N/A
Floor: 5 Terminal Asset No.: N/A
Room: 504

Range	Max. Capacity	Readability (d)
1	220 g	0.0001 g

Procedure



Calibration Guideline: EURAMET cg-18 v. 4.0 (11/2015)
METTLER TOLEDO Work Instruction: CP/W002/20

This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.

The sensitivity/span of the weighing instrument was adjusted before calibration with a built-in weight.

In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

	Temperature		Humidity	
As Found	Start: 23.9 °C	End: 24.2 °C	Start: 45.8 %	End: 54.8 %

As Found Calibration Date: 19-Jan-2022 Cellibrator: 
As Left Calibration Date: N/A
Issue Date: 20-Jan-2022 Approved Signatory: 
☒ Kassakorn Tassanachaisakul
☐ Santi Jitniyom
☐ Surachet Sukkate


Measurement Results

Repeatability

Test Load: 100 g

	As Found	As Left
1	99.9998 g	N/A
2	99.9998 g	N/A
3	99.9997 g	N/A
4	99.9999 g	N/A
5	99.9998 g	N/A
6	99.9998 g	N/A
7	99.9998 g	N/A
8	99.9998 g	N/A
9	99.9999 g	N/A
10	99.9999 g	N/A

Standard Deviation: 0.00006 g N/A

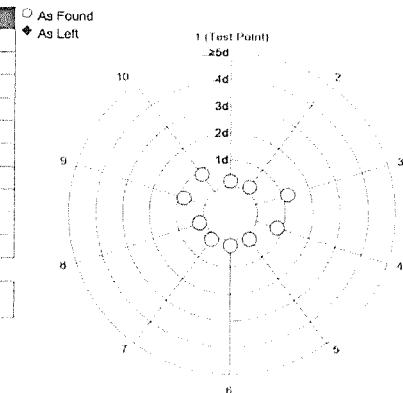


The "d" in the graph represents the readability of the range/interval in which the test was performed.
The results of this graph are based upon the absolute values of the differences from the mean value.

Eccentricity

Test Load: 100 g

Position	As Found	As Left
1	99.9998 g	N/A
2	99.9999 g	N/A
3	99.9997 g	N/A
4	99.9997 g	N/A
5	99.9999 g	N/A

Maximum Deviation: 0.0001 g N/A




As Found
The "d" in the graph represents the readability of the range/interval in which the test was performed.

Error of Indication

As Found

	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.0000 g	0.0000 g	0.0000 g	0.14 mg	2
2	0.0500 g	0.0500 g	0.0000 g	0.15 mg	2
3	0.1000 g	0.1000 g	0.0000 g	0.15 mg	2
4	0.5000 g	0.5000 g	0.0000 g	0.15 mg	2
5	1.0000 g	1.0000 g	0.0000 g	0.15 mg	2
6	5.0000 g	5.0000 g	0.0000 g	0.16 mg	2
7	10.0000 g	10.0000 g	0.0000 g	0.16 mg	2
8	50.0000 g	49.9999 g	-0.0001 g	0.19 mg	2
9	99.9999 g	99.9998 g	-0.0001 g	0.25 mg	2
10	149.9999 g	149.9997 g	-0.0002 g	0.35 mg	2
11	199.9999 g	199.9998 g	-0.0001 g	0.39 mg	2

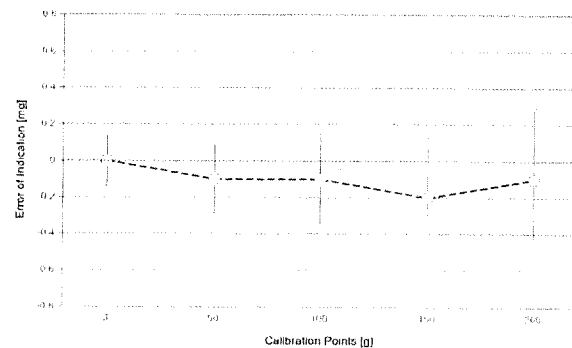

○ As Found

◆ As Left

For improved legibility of the graphics only increasing measurement points are shown and measurement points close to zero are not displayed.

The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor k – which can be larger than 2 according to EURAMET cg-18. The value of the measurand lies within the assigned range of values with a probability of approximately 95%.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2

Weight Set No.: WS03 Date of Issue: 21-Sep-2021
Certificate Number: 175498 Calibration Due Date: 14-Mar-2023

Thermo Hygrometer

Equipment No.: IN281 Date of Issue: 25-May-2021
Certificate Number: 21H1100 Calibration Due Date: 10-May-2022

26-1-65

Remarks

FACT adjustment functionality activated

Equipment condition: Good

Next calibration according to customer's procedure

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

26-1-65

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with $k=2$ in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use: $1.5 \cdot 10^{-6} / K$

Temperature range on site for the evaluation of the measurement uncertainty in use: 4 K


Linearization of Uncertainty Equation

	Range		As Found	As Left
	d	Max		
1	0.0001 g	220 g	$U_1 = 0.15 \text{ mg} + 0.00599 \text{ mg/g} \cdot R$	N/A

To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication	As Found		As Left	
0.0220 g	0.15 mg	0.68%	N/A	N/A
0.2200 g	0.15 mg	0.069%	N/A	N/A
2.2000 g	0.16 mg	0.0074%	N/A	N/A
22.0000 g	0.28 mg	0.0013%	N/A	N/A
220.0000 g	1.5 mg	0.00067%	N/A	N/A

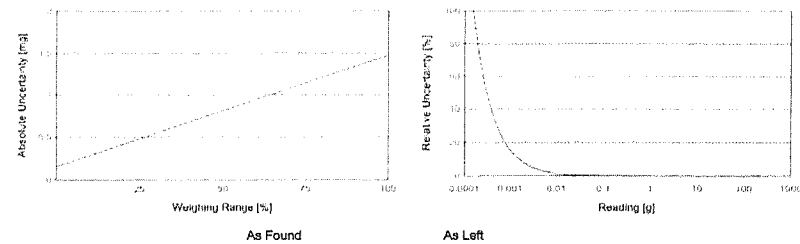

GWP® Certificate



As
Found



As
Left



The weighing device meets the given process requirements.

The weighing device meets the given process requirements.

Tests Performed: ☒ As Found ☐ As Left ☒ No adjustments/modifications made, As Left results correspond to As Found.


Process Requirements

Weighing Tolerance: 1%

Smallest Net Weight: 0.0500 g

Safety Factor: 2

Safe Weighing Range

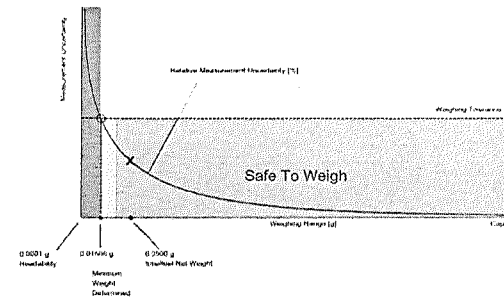

While the values in this graph reflect the actual calibration results, the measurement uncertainty curves are simply a visual representation. This graph reflects As Left loading, unless only As Found was performed.

26-1-65

26-1-65

Minimum Weight

As Found Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.15146 g	0.30476 g	0.45993 g	0.77601 g	1.60147 g
0.2%	0.07550 g	0.15146 g	0.22788 g	0.38211 g	0.77601 g
0.5%	0.03015 g	0.06037 g	0.09066 g	0.15146 g	0.30476 g
1%	0.01506 g	0.03015 g	0.04525 g	0.07550 g	0.15146 g
2%	0.00753 g	0.01506 g	0.02260 g	0.03770 g	0.07550 g
5%	0.00301 g	0.00602 g	0.00904 g	0.01506 g	0.03015 g

✓ Pass: The determined minimum weight meets the requirement for the smallest net weight.

As Left Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.15146 g	0.30476 g	0.45993 g	0.77601 g	1.60147 g
0.2%	0.07550 g	0.15146 g	0.22788 g	0.38211 g	0.77601 g
0.5%	0.03015 g	0.06037 g	0.09066 g	0.15146 g	0.30476 g
1%	0.01506 g	0.03015 g	0.04525 g	0.07550 g	0.15146 g
2%	0.00753 g	0.01506 g	0.02260 g	0.03770 g	0.07550 g
5%	0.00301 g	0.00602 g	0.00904 g	0.01506 g	0.03015 g

✓ Pass: The determined minimum weight meets the requirement for the smallest net weight.

At these net minimum weight values, the measurement uncertainty of the weighing device is equal to or less than 1/1 (no safety factor), 1/2, 1/3, 1/5, or 1/10 of the required tolerance. The values are calculated with $k = 2$ and based on the linear formula of the measurement uncertainty of the weighing device in use.

The safety factor for As Found is always 1. This implies no safety factor. As Found testing looks at the behavior of the instrument from the past until test occurred. For the past, it is necessary to know that the tolerance was met, but not the safety factor. The safety factor is a proactive measure to apply for future measurements.

Notes on minimum weight values in above table:

- If "N/A" is shown above, no appropriate value could be calculated.
- METTLER TOLEDO is not responsible for the definition of the process requirements.

Measurement Results

Results Summary

	Repeatability	Eccentricity	Error of Indication
As Found	✓	✓	✓
As Left	✓	✓	✓

✓ = Passed

✗ = Failed

Δ = Safety Factor not met

Repeatability

Test Load: 100 g

Tolerance	Control Limit	As Found		As Left	
		Std. Deviation	Result	Std. Deviation	Result
0.1%	N/A	0.00006 g*	N/A	0.00006 g*	N/A
0.2%	0.00005 g		✗		✗
0.5%	0.00013 g		✓		✓
1%	0.00025 g		✓		✓
2%	0.00050 g		✓		✓
5%	0.00125 g		✓		✓

*The calculated standard deviation value is below the rounding error of the balance. The 0.41*d rule is used for the assessment of this repeatability test and the calculation of the minimum weight.

The weighing tolerance is met if the standard deviation is less than or equal to the corresponding control limit.

Eccentricity

Test Load: 100 g

Tolerance	Control Limit	As Found		As Left	
		Deviation	Result	Deviation	Result
0.1%	0.0500 g	0.0001 g	✓	0.0001 g	✓
0.2%	0.1000 g		✓		✓
0.5%	0.2500 g		✓		✓
1%	0.5000 g		✓		✓
2%	1.0000 g		✓		✓
5%	2.5000 g		✓		✓

The weighing tolerance is met if the deviation is less than or equal to the corresponding control limit.

Error of Indication

As Found

		Control limits for various weighing tolerances					
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A
50.0000 g	-0.0001 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g
99.9999 g	-0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g
149.9999 g	-0.0002 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g
199.9999 g	-0.0001 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓	✓

As Left

		Control limits for various weighing tolerances					
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A
50.0000 g	-0.0001 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g
99.9999 g	-0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g
149.9999 g	-0.0002 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g
199.9999 g	-0.0001 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓	✓

The weighing tolerance is met if the error (of indication) for each test point is less than or equal to the corresponding control limit for that particular weighing tolerance. Results at or close to the zero point cannot be assessed.

Service Date: 2022-01-19
Document Number: TH2065-105-011922-LABBalanceHR
ENVIRONMENT RESEARCH&TECHNOLOGY CO., LTD
25/114 Moo 6, Soi Chinakot 1, Ngamwongwan Rd., Taongsongho, กรุงเทพมหานคร, Laksi, Bangkok 10210
Ramita Teangthai

Balance Health Report

Device Details

System Details			
Manufacturer:	Mettler Toledo	Accessory 1:	
Model:	MS204S	Accessory 2:	
Serial number:	B334601537	Weight set for routine testing:	Yes /
Firmware:	1.74		

History


Device History		Service History	
Instrument in use:	Yes	Last preventive maintenance:	< 1 year
Instrument age:	> 10 years	Last instrument calibration:	< 1 year
Spare parts available:	Yes	Last minimum weight determination:	
Regulations:	ISO		
Process tolerance in %:	1%	Routine testing performed:	Yes
Smallest sample not weight:	0.05g		

Check List

Environmental Conditions		General & Functional Checks	
Room temperature fluctuation	✓	Leveling	✓
Exposure to direct sun	✓	Cleanliness	✓
Vibrations	✓	Completeness - missing parts see additional remarks	✓
Draft	✓	Settings optimized for operating environment	✓
Dirt or dust	✓	Other - objections noted as additional remarks	—
Static	✓	Electrical Component Checks	
Mechanical Component Checks		Power supply	✓
Draft shield	✓	Sliding door drive	—
Weighing pan position	✓	Internal weight drive	✓
Housing	✓	Display	✓
Other - objections noted as additional remarks	—	Other - objections noted as additional remarks	—

Recommendations

Measurement Result Quality		Process Efficiency	
Instrument calibration		Uninstall instrument	
Identify safe weighing range		Replace instrument	
GWP verification / risk assessment		Replace / add parts (see additional remarks)	
Preventive maintenance		Onsite repair	
Perform routine testing with test weights		Depot repair	
User training		Use of accessories (see additional remarks)	

Contact	Name:	Ramita Teangthai	Position:	N/A	Phone:	0866334490	Email:	ramita@servicerearch.co.th
Additional Remarks & Recommendations							Engineer Details	
							Date:	19-Jan-2022
							Name:	Suwichai Choykamchu
							Signature:	

This is not a certificate.

It should not be used to interpret final results for the testing of these devices.

Legend: ✓ Good/Pass ⚠ Needs Attention ✗ Bad/Fail — Not Applicable

26-1-65

26-1-65



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3060-27 FAX. 0-2719-9484



Cert. No.: 22TM151
Page.: 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven
Manufacturer : Binder
Model : FED 115 E2
Serial No. : 11-22823
ID No. : ERTC-L-In.-076
Submitted by : Environment Research & Technology Company Limited
25/114 Moo 6 Soi Chinaket 1,
Ngamwongwan Road, Toongsonghong, Laksi,
Bangkok 10210
Location : Laboratory (ERTC)
Received Order : 5 January 2022
Calibration Date : 5 January 2022
Ambient Temperature : $(26 \pm 10) ^\circ\text{C}$
Relative Humidity : $(50 \pm 30) \%$
Calibrated by : Man Pattanapongpaiboon

Approved by :
Approved Signatory

() Pornthippa Tameyakul
() Malee Butkruea
() Suwit Imjai

Issue Date : 21 January 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

24-1-65

A 0036818



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2201-0006ON-2
Procedure Used :-

Cert. No.: 22TM151
Page.: 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44031769	21LM12	02 Sep 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close



Probe Installation Details :		Dimension of Chamber :	
a =	5.0 cm	D =	0.40 m
b =	5.0 cm	W =	0.60 m
c =	5.0 cm	H =	0.48 m
		Capacity =	0.12 m ³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	27	27
REL.Humid. (%)	54	58
AC Supply (Volt)	219	222

Ref. Std. ID No.: @ Calibration Point		
Position :	(180) °C	(104) °C
1	20-09TC-01	9RTD-2/1
2	20-09TC-02	9RTD-2/2
3	20-09TC-03	9RTD-2/3
4	20-09TC-04	9RTD-2/4
5	20-09TC-05	9RTD-2/5
6	20-09TC-06	9RTD-2/6
7	20-09TC-07	9RTD-2/7
8	20-09TC-08	9RTD-2/8
9 (ref.)	20-09TC-09	9RTD-2/9

24-1-65

a 1090220



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2201-0006ON-2
Result of Calibration :- (*) Without Adjustment

Cert. No.: 22TM151

Page.: 3 of 3

Function of UUC* : Temperature Source

Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
104	104	104	0.11	1.1	1.4	0.69	2
180	180	180	0.43	3.3	5.6	1.5	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104	103.167	102.948	104.098	104.155	104.013	103.198	103.619	103.294	103.159
180	177.080	177.342	181.816	181.065	179.474	177.914	181.064	179.354	178.751

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

26-1-6

a 1090219



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3090-27 FAX. 0-2719-9484



Cert. No.: 22TM152
Page.: 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven
Manufacturer : Memmert
Model : UF 110
Serial No. : B414.0652
ID No. : ERTC-L-In.-098
Submitted by : Environment Research & Technology Company Limited
25/114 Moo 6 Soi Chinaket 1,
Ngamwongwan Road, Toongsonghong, Laksi,
Bangkok 10210
Location : Laboratory (ERTC)
Received Order : 5 January 2022
Calibration Date : 5 January 2022
Ambient Temperature : $(26 \pm 10) ^\circ\text{C}$
Relative Humidity : $(50 \pm 30) \%$
Calibrated by : Man Pattanapongpaiboon

Approved by :

Malee
Approved Signatory

() Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date : 21 January 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

24-1-65

A 0036819



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2201-0006ON-3
Procedure Used :-

Cert. No.: 22TM152
Page.: 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44031769	21LM12	02 Sep 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close



Probe Installation Details : Dimension of Chamber :

a = 5.0 cm	D = 0.40 m
b = 5.0 cm	W = 0.56 m
c = 5.0 cm	H = 0.48 m
	Capacity = 0.11 m ³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	27	27
REL.Humid. (%)	54	58
AC Supply (Volt)	219	222

Ref. Std. ID No.: @ Calibration Point		
Position :	(180) °C	(104) °C
1	20-09TC-01	9RTD-2/1
2	20-09TC-02	9RTD-2/2
3	20-09TC-03	9RTD-2/3
4	20-09TC-04	9RTD-2/4
5	20-09TC-05	9RTD-2/5
6	20-09TC-06	9RTD-2/6
7	20-09TC-07	9RTD-2/7
8	20-09TC-08	9RTD-2/8
9 (ref.)	20-09TC-09	9RTD-2/9

24-1-65 *Malee*

a 1090218



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2201-0006ON-3
Result of Calibration :- (*) Without Adjustment

Cert. No.: 22TM152

Page.: 3 of 3

Function of UUC* : Temperature Source

Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
104.0	104.0	104.0	0.11	1.0	1.9	0.42	2
180.0	180.0	180.0	0.51	2.3	4.2	1.2	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	105.219	103.394	103.908	104.133	104.348	104.096	103.878	104.103	104.360
180.0	182.291	178.691	178.879	180.031	180.761	180.026	180.572	180.044	180.253

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

26-1-63

Mulu.


a 1090217

Mettler-Toledo (Thailand) Ltd.
846/4 - 846/5 Lasalle Rd., Bangna Tai Sub-District
Bangna District, Bangkok 10260
+66 2723 0382
MT-TH.ServiceSupport@mt.com



Accuracy Calibration Certificate

Customer

Company: ENVIRONMENT RESEARCH&TECHNOLOGY CO., LTD.
Address: 25/114 Moo 6, Soi Chinaket 1, Ngamwongwan Rd., Toongsongho
City: Laksi Contact: Ramita Taengthai
Zip / Postal: 10210
State / Province: Bangkok
Order Number: 

Weighing Device

Manufacturer: Mettler Toledo Instrument Type: Weighing Instrument
Model: MS204TS/00 Asset Number: ERTC-L-IN-114
Serial No.: B547728937 Terminal Model: N/A
Building: N/A Terminal Serial No.: N/A
Floor: 5 Terminal Assot No.: N/A
Room: 504

Range	Max Capacity	Readability (d)
1	220 g	0.0001 g

Procedure



Calibration Guideline: EURAMET cg-18 v. 4.0 (11/2015)
METTLER TOLEDO Work Instruction: CPW002/20

This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.

The sensitivity/span of the weighing instrument was adjusted before calibration with a built-in weight.

In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

	Temperature		Humidity	
As Found	Start: 23.8 °C	End: 24.5 °C	Start: 49.7 %	End: 55.1 %


As Found Calibration Date: 19-Jan-2022 Cellibrator: 
As Left Calibration Date: N/A
Issue Date: 20-Jan-2022
Approved Signatory: 
☒ Kassakorn Tassanachaisakul
☐ Santi Jitniyom
☐ Surachot Sukkate

Measurement Results

Repeatability

Test Load: 100 g

	As Found	As Left
1	99.9999 g	N/A
2	99.9998 g	N/A
3	99.9998 g	N/A
4	99.9999 g	N/A
5	99.9999 g	N/A
6	99.9999 g	N/A
7	99.9998 g	N/A
8	99.9999 g	N/A
9	99.9998 g	N/A
10	99.9999 g	N/A
Standard Deviation	0.00005 g	N/A

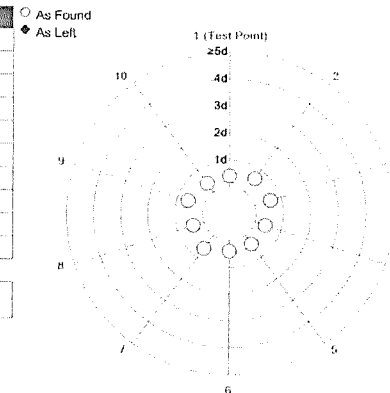


The "d" in the graph represents the readability of the range/interval in which the test was performed.
The results of this graph are based upon the absolute values of the differences from the mean value.

Eccentricity

Test Load: 100 g

Position	As Found	As Left
1	99.9998 g	N/A
2	99.9999 g	N/A
3	99.9998 g	N/A
4	99.9998 g	N/A
5	99.9997 g	N/A
Maximum Deviation	0.0001 g	N/A




As Found
The "d" in the graph represents the readability of the range/interval in which the test was performed.

Error of Indication

As Found

	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.0000 g	0.0000 g	0.0000 g	0.12 mg	2
2	0.0500 g	0.0500 g	0.0000 g	0.13 mg	2
3	0.1000 g	0.1000 g	0.0000 g	0.13 mg	2
4	0.5000 g	0.5000 g	0.0000 g	0.13 mg	2
5	1.0000 g	1.0000 g	0.0000 g	0.13 mg	2
6	5.0000 g	5.0000 g	0.0000 g	0.14 mg	2
7	10.0000 g	10.0000 g	0.0000 g	0.14 mg	2
8	50.0000 g	50.0000 g	0.0000 g	0.18 mg	2
9	99.9999 g	99.9998 g	-0.0001 g	0.24 mg	2
10	149.9999 g	149.9998 g	-0.0001 g	0.34 mg	2
11	199.9999 g	200.0000 g	0.0001 g	0.39 mg	2

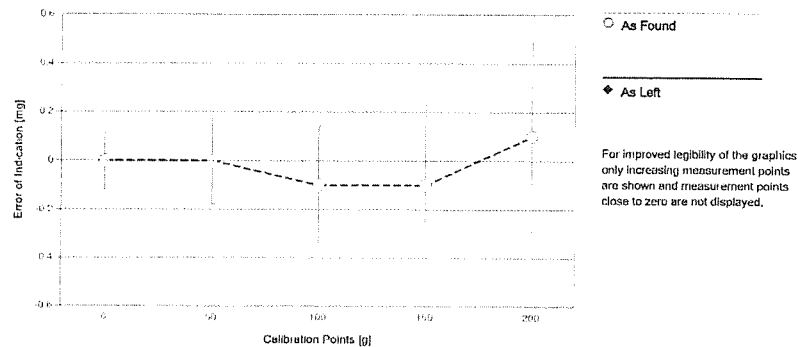

The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor k – which can be larger than 2 according to EURAMET cg-18. The value of the measurand lies within the assigned range of values with a probability of approximately 95%.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2

Weight Set No.: WS03 Date of Issue: 21-Sep-2021
Certificate Number: 175498 Calibration Due Date: 14-Mar-2023

Thermo Hygrometer

Equipment No.: IN281 Date of Issue: 25-May-2021
Certificate Number: 21H1100 Calibration Due Date: 10-May-2022

26-1-65

Remarks

FACT adjustment functionality activated
Equipment condition: Good
Next calibration according to customer's procedure

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

26-1-65

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with $k=2$ in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use: $3.0 \cdot 10^{-6} / K$

Temperature range on site for the evaluation of the measurement uncertainty in use: $4 K$


Linearization of Uncertainty Equation

	Range		As Found	As Left
	d	Max		
1	0.0001 g	220 g	$U_1 = 0.13 \text{ mg} + 0.00828 \text{ mg/g} \cdot R$	N/A


To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication	As Found		As Left	
0.0220 g	0.13 mg	0.59%	N/A	N/A
0.2200 g	0.13 mg	0.060%	N/A	N/A
2.2000 g	0.15 mg	0.0067%	N/A	N/A
22.0000 g	0.31 mg	0.0014%	N/A	N/A
220.0000 g	2.0 mg	0.00089%	N/A	N/A

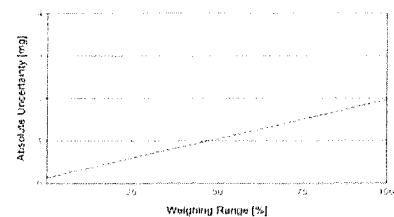

As Found

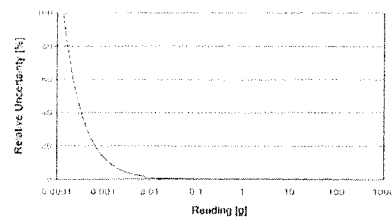

As Left

26-1-65

GWP® Certificate



As Found



As Left



The weighing device meets the given process requirements.

The weighing device meets the given process requirements.

Tests Performed:

☒ As Found

☐ As Left

☒ No adjustments/modifications made. As Left results correspond to As Found.


Process Requirements

Weighing Tolerance: 1%

Smallest Net Weight: 0.0500 g

Safety Factor: 2

Safe Weighing Range

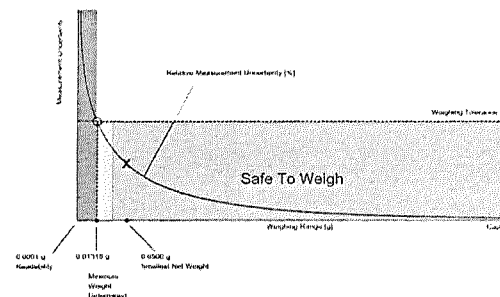

While the values in this graph reflect the actual calibration results, the measurement uncertainty curves are simply a visual representation. This graph reflects As Left findings, unless only As Found was performed.

26-1-65

Minimum Weight

As Found Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.13276 g	0.26775 g	0.40503 g	0.68670 g	1.43539 g
0.2%	0.06610 g	0.13276 g	0.19997 g	0.33610 g	0.68670 g
0.5%	0.02637 g	0.05284 g	0.07939 g	0.13276 g	0.26775 g
1%	0.01318 g	0.02637 g	0.03960 g	0.06610 g	0.13276 g
2%	0.00659 g	0.01318 g	0.01977 g	0.03298 g	0.06610 g
5%	0.00263 g	0.00527 g	0.00790 g	0.01318 g	0.02637 g

✓ Pass: The determined minimum weight meets the requirement for the smallest net weight.

As Left Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.13270 g	0.26775 g	0.40503 g	0.68670 g	1.43539 g
0.2%	0.06610 g	0.13276 g	0.19997 g	0.33610 g	0.68670 g
0.5%	0.02637 g	0.05284 g	0.07939 g	0.13276 g	0.26775 g
1%	0.01318 g	0.02637 g	0.03960 g	0.06610 g	0.13276 g
2%	0.00659 g	0.01318 g	0.01977 g	0.03298 g	0.06610 g
5%	0.00263 g	0.00527 g	0.00790 g	0.01318 g	0.02637 g

✓ Pass: The determined minimum weight meets the requirement for the smallest net weight.

At these not minimum weight values, the measurement uncertainty of the weighing device is equal to or less than 1/1 (no safety factor), 1/2, 1/3, 1/5, or 1/10 of the required tolerance. The values are calculated with $k = 2$ and based on the linear formula of the measurement uncertainty of the weighing device in use.

The safety factor for As Found is always 1. This implies no safety factor. As Found testing looks at the behavior of the instrument from the past until test occurred. For the past, it is necessary to know that the tolerance was met, but not the safety factor. The safety factor is a proactive measure to apply for future measurements.

Notes on minimum weight values in above table:

1. If "N/A" is shown above, no appropriate value could be calculated.
2. METTLER TOLEDO is not responsible for the definition of the process requirements.

Measurement Results

Results Summary

	Repeatability	Eccentricity	Error of Indication
As Found	✓	✓	✓
As Left	✓	✓	✓

✓ = Passed

✗ = Failed

k_1 = Safety Factor not met

Repeatability

Test Load: 100 g

Tolerance	Control Limit	As Found		As Left	
		Std. Deviation	Result	Std. Deviation	Result
0.1%	N/A	0.00005 g*	N/A	0.00005 g*	N/A
0.2%	0.00005 g		✓		✓
0.5%	0.00013 g		✓		✓
1%	0.00025 g		✓		✓
2%	0.00050 g		✓		✓
5%	0.00125 g		✓		✓

*The calculated standard deviation value is below the rounding error of the balance. The 0.41*d rule is used for the assessment of this repeatability test and the calculation of the minimum weight.

The weighing tolerance is met if the standard deviation is less than or equal to the corresponding control limit.

Eccentricity

Test Load: 100 g

Tolerance	Control Limit	As Found		As Left	
		Deviation	Result	Deviation	Result
0.1%	0.0500 g	0.0001 g	✓	0.0001 g	✓
0.2%	0.1000 g		✓		✓
0.5%	0.2500 g		✓		✓
1%	0.5000 g		✓		✓
2%	1.0000 g		✓		✓
5%	2.5000 g		✓		✓

The weighing tolerance is met if the deviation is less than or equal to the corresponding control limit.

Error of Indication

As Found

		Control limits for various weighing tolerances					
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A
50.0000 g	0.0000 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g
99.9999 g	-0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g
149.9999 g	-0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g
199.9999 g	0.0001 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓	✓

As Left

		Control limits for various weighing tolerances					
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A
50.0000 g	0.0000 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g
99.9999 g	-0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g
149.9999 g	-0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g
199.9999 g	0.0001 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓	✓

The weighing tolerance is met if the error (of indication) for each test point is less than or equal to the corresponding control limit for that particular weighing tolerance. Results at or close to the zero point cannot be assessed.

Service Date: 2022-01-19
Document Number: TH2065-164-011922-LABBalanceHR
ENVIRONMENT RESEARCH&TECHNOLOGY CO., LTD
25/114 Moo 6, Soi Chinaket 1, Ngamwongwan Rd., Toongsoinghro, บางกะปิ, Bangkok 10210
Ramita Taengthai

METTLER TOLEDO

Balance Health Report

Device Details

System Details			
Manufacturer:	Mettler Toledo	Accessory 1:	
Model:	MS204TS	Accessory 2:	
Serial number:	8541728937	Weight set for routine testing:	Yes /
Firmware:	3.50		


History

Device History		Service History	
Instrument in use:	Yes	Last preventive maintenance:	< 1 year
Instrument age:	3-10 years	Last instrument calibration:	< 1 year
Spare parts available:	Yes	Last minimum weight determination:	< 1 year
Regulations:	ISO		
Process tolerance in %:	1%	Routine testing performed:	Yes
Smallest sample not weight:	0.0500 g		

Check List

Environmental Conditions		General & Functional Checks	
Room temperature fluctuation	✓	Leveling	✓
Exposure to direct sun	✓	Cleanliness	✓
Vibrations	✓	Completeness - missing parts see additional remarks	✓
Draft	✓	Settings optimized for operating environment	✓
Dirt or dust	✓	Other - objections noted as additional remarks	—
Static	✓	Electrical Component Checks	
Mechanical Component Checks		Power supply	✓
Draft shield	✓	Sliding door drive	✓
Weighing pan position	✓	Internal weight drive	✓
Housing	✓	Display	✓
Other - objections noted as additional remarks	—	Other - objections noted as additional remarks	—

Recommendations

Measurement Result Quality		Process Efficiency	
Instrument calibration		Uninstall instrument	
Identify safe weighing range		Replace instrument	
GWP verification / risk assessment		Replace / add parts (see additional remarks)	
Preventive maintenance		Onsite repair	
Perform routine testing with test weights		Depot repair	
User training		Use of accessories (see additional remarks)	
Contact	Name: Ramita Taengthai	Position:	N/A
	Phone: 0866334950	Email:	ramita@enviresearch.co.th
Additional Remarks & Recommendations		Engineer Details	
		Date:	19-Jan-2022
		Name:	Suwichai Choykamchu
		Signature:	

This is not a certificate.

It should not be used to interpret final results for the testing of these devices.

Legend: ✓ Good/Pass ⚠ Needs Attention ✗ Bad/Fail — Not Applicable

26-1-65

26-1-65



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3090-27 FAX. 0-2719-9484



Cert. No.: 22TM4
Page.: 1 of 3

Certificate of Calibration

Equipment : Incubator
Manufacturer : Binder
Model : ED 115
Serial No. : 950433
ID No. : ERTC-L-In.-009
Submitted by : Environment Research & Technology Company Limited
25/114 Moo 6 Soi Chinaket 1,
Ngamwongwan Road, Toongsonghong, Laksi,
Bangkok 10210
Location : 408/2 ห้องปฏิบัติการนํ้าอาหารเลี้ยงเชื้อ
Received Order : 5 January 2022
Calibration Date : 6 January 2022
Ambient Temperature : $(26 \pm 10) ^\circ\text{C}$
Relative Humidity : $(50 \pm 30) \%$
Calibrated by : Khit Ruttanaprapachai
Approved by :
() Ponthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date : 19 January 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

26-1-65

A 0036711



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2201-0006ON-5
Procedure Used :-

Cert. No.: 22TM4
Page.: 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44060450	21LM4/1	06 Mar 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close



Probe Installation Details :

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :

D = 0.50 m
W = 0.60 m
H = 0.50 m
Capacity = 0.15 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	26
REL.Humid. (%)	59	61
AC Supply (Volt)	221	222

Position :	Ref. Std. ID No.:
1	19-14RTD-01
2	19-14RTD-02
3	19-14RTD-03
4	19-14RTD-04
5	19-14RTD-05
6	19-14RTD-06
7	21-14RTD-07
8	19-14RTD-08
9 (ref.)	19-14RTD-09

26-1-65

a 1089977



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2201-0006ON-5
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 22TM4

Page.: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
35	35	35	0.17	0.22	0.48	0.66	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
35	35.011	35.019	34.925	34.979	34.842	34.791	34.848	34.825	34.886

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-oOo-

26-1-65

Madu.

a 1089976