



รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ


Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Total Suspended Particulate	High Volume	RYG_FS0174	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0180	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0178	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0291	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	RYG_EN0001	23-Mar-22	23-Mar-23	12
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0295	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0191	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0185	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0188	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	Digital Balance	RYG_EN0001	23-Mar-22	23-Mar-23	12
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0545	14-Sep-21	15-Mar-23	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0531	14-Jul-21	12-Jan-23	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0530	14-Jul-21	12-Jan-23	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0544	15-Sep-21	15-Mar-23	18
Ambient	Temperature	Temperature Sensor	RYG_FS0545	14-Sep-21	15-Mar-23	18
Ambient	Temperature	Temperature Sensor	RYG_FS0531	14-Jul-21	12-Jan-23	18
Ambient	Temperature	Temperature Sensor	RYG_FS0530	14-Jul-21	12-Jan-23	18
Ambient	Temperature	Temperature Sensor	RYG_FS0544	15-Sep-21	15-Mar-23	18
Noise	Leq 24 hrs	Sound Calibrator	RYG_FS0216	9-Aug-21	9-Aug-22	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0439	6-Aug-21	6-Aug-22	12





High Volume Air Sampler Calibration Worksheet

Project Site :	B.Grimm Power(AIE-MTP)Limited	Barometric Pressure (mm Hg) :	757
Calibrate Location :	สถานที่ที่ 1 วัดประทุมมิตรบำรุง	Temperature (°C) :	32
Calibrate Date :	27-Apr-22	High Volume ID :	RYG_FS0174
CalibrationSheet No.:	C-270422-RYG_FS0174	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	4800
Calibrator Model :	TE-5028A	Calibrator Slope :	1.53016
Calibrator S/N :	1166	Calibrator Intercept :	-0.0468

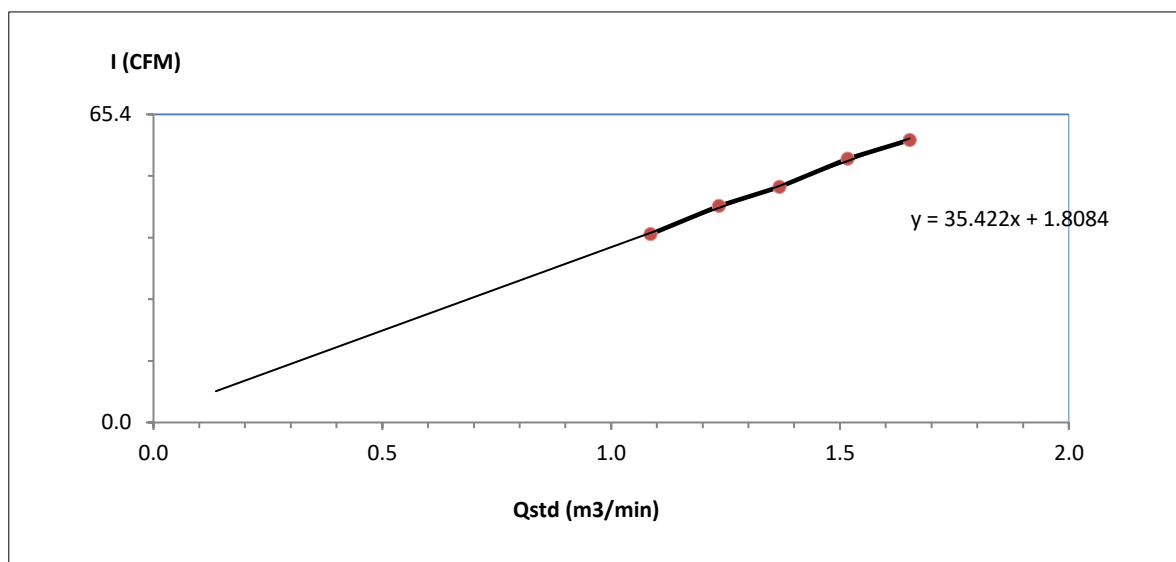Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.6	1.0864	40	Slope : 35.4217 Intercept : 1.8084 Correlation Coefficient : 0.9987
2	3.4	1.2356	46	
3	4.2	1.3680	50	
4	5.2	1.5169	56	
5	6.2	1.6521	60	



Calibrated by 
 (Mr.Santi Chaichana)
 Field Scientist(1)


Approved by : 
 (Mr. Noppong Juntarupan)
 Enviro Field Coordinator Scientist (3)



High Volume Air Sampler Calibration Worksheet

Project Site :	B.Grimm Power(AIE-MTP)Limited สถานที่ที่2 โรงเรียนระยองวิทยาคมนิคม	Barometric Pressure (mm Hg) :	757
Calibrate Location :	อุสาหกรรม	Temperature (°C) :	32
Calibrate Date :	27-Apr-22	High Volume ID :	RYG_FS0180
CalibrationSheet No.:	C-270422-RYG_FS0180	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	1328
Calibrator Model :	TE-5028A	Calibrator Slope :	1.53016
Calibrator S/N :	1166	Calibrator Intercept :	-0.0468

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.7	1.1062	40	Slope : 35.5606 Intercept : 1.0567 Correlation Coefficient : 0.9963
2	3.4	1.2356	46	
3	4.4	1.3991	50	
4	5.4	1.5450	56	
5	6.2	1.6521	60	

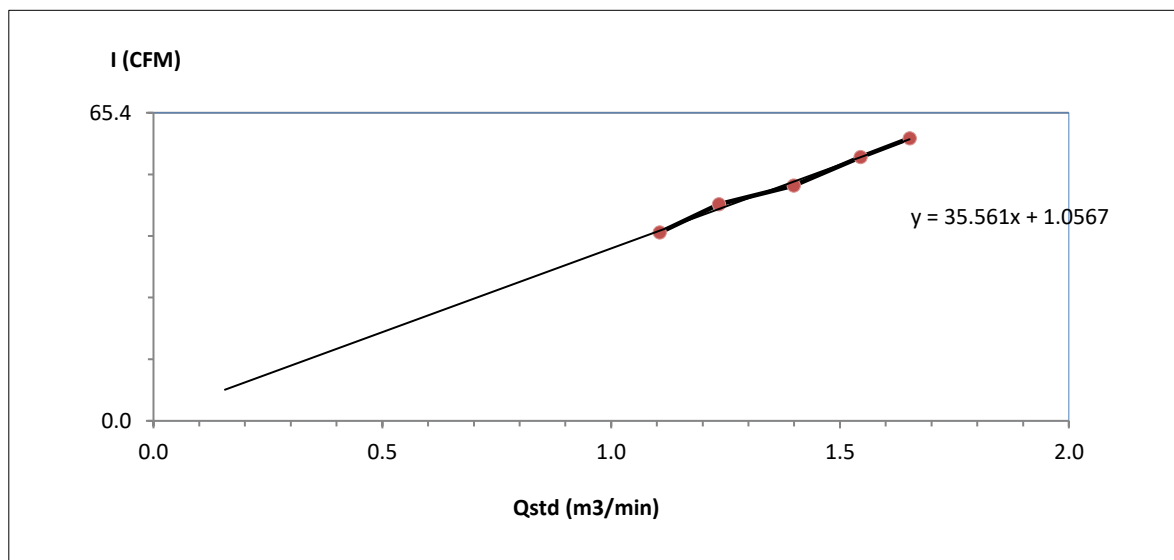

Calibrated by

(Mr.Santi Chaichana)
Field Scientist(1)

Approved by :


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)



High Volume Air Sampler Calibration Worksheet

Project Site :	B.Grimm Power(AIE-MTP)Limited	Barometric Pressure (mm Hg) :	757
Calibrate Location :	สถานที่ที่3 บ้านสำนักมะม่วง	Temperature (°C) :	32
Calibrate Date :	27-Apr-22	High Volume ID :	RYG_FS0178
CalibrationSheet No.:	C-270422-RYG_FS0178	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	4804
Calibrator Model :	TE-5028A	Calibrator Slope :	1.53016
Calibrator S/N :	1166	Calibrator Intercept :	-0.0468

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.6	1.0864	40	Slope : 33.4785 Intercept : 3.9064 Correlation Coefficient : 0.9974
2	3.4	1.2356	46	
3	4.4	1.3991	50	
4	5.4	1.5450	56	
5	6.4	1.6778	60	

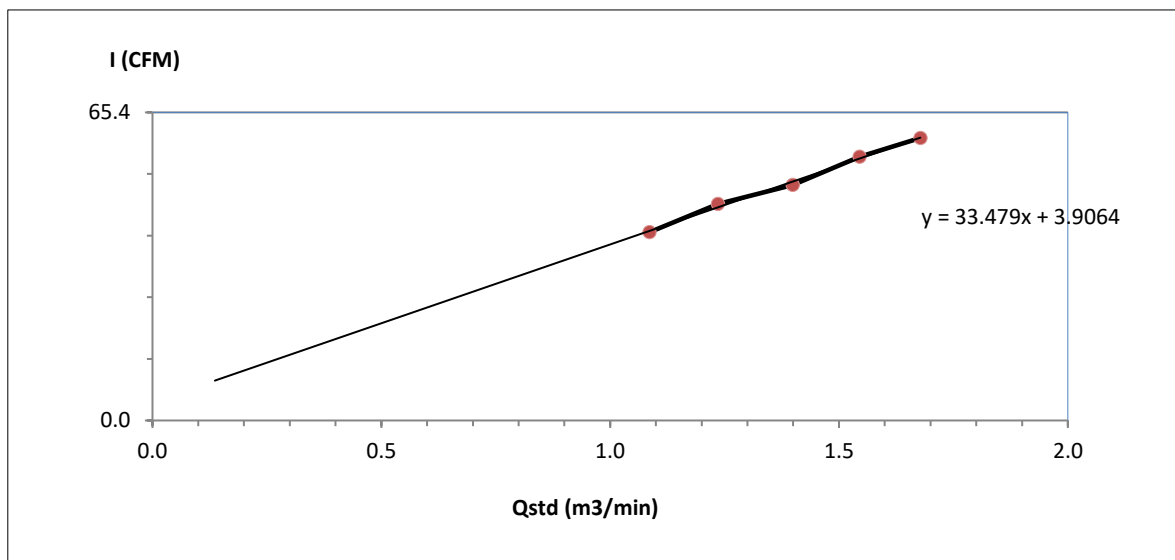

Calibrated by

(Mr.Santi Chaichana)
Field Scientist(1)

Approved by :


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)





High Volume Air Sampler Calibration Worksheet

Project Site :	B.Grimm Power(AIE-MTP)Limited	Barometric Pressure (mm Hg) :	757
Calibrate Location :	สถานที่ที่ 4 โรงเรียนอนุบาลรักภาษา	Temperature (°C) :	32
Calibrate Date :	27-Apr-22	High Volume ID :	RYG_FS0291
CalibrationSheet No.:	C-270422-RYG_FS0291	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	5333
Calibrator Model :	TE-5028A	Calibrator Slope :	1.53016
Calibrator S/N :	1166	Calibrator Intercept :	-0.0468

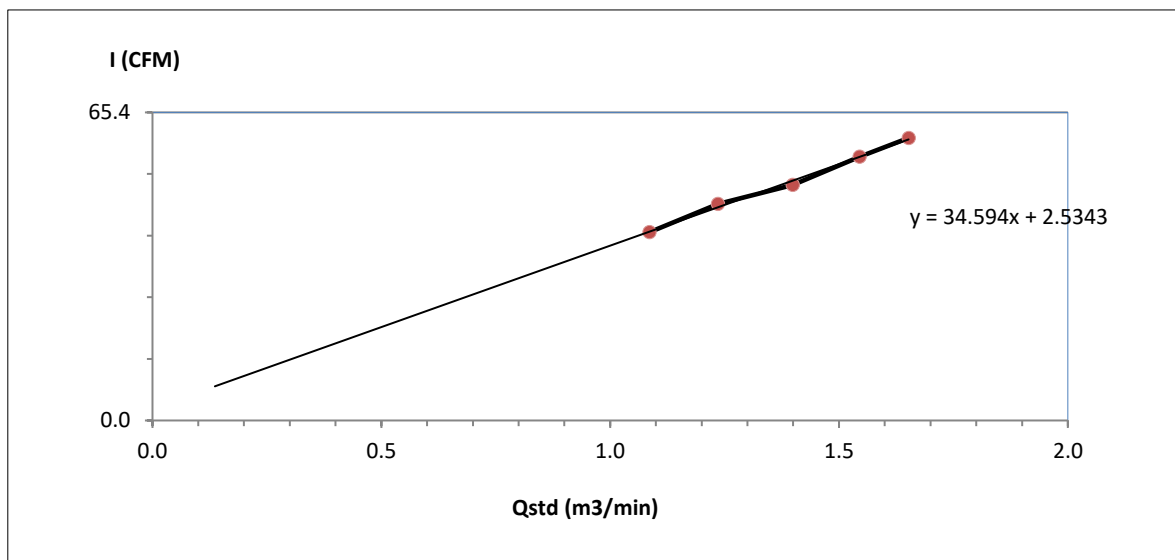Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.6	1.0864	40	Slope : 34.5945 Intercept : 2.5343 Correlation Coefficient : 0.9970
2	3.4	1.2356	46	
3	4.4	1.3991	50	
4	5.4	1.5450	56	
5	6.2	1.6521	60	



Calibrated by 
 (Mr.Santi Chaichana)
 Field Scientist(1)

Approved by : 
 (Mr. Noppong Juntarupan)
 Enviro Field Coordinator Scientist (3)



PENTA
CALIBRATION

PENTA CALIBRATION CO., LTD.

66/124 The Connect 33 Village Kanchanaphisek Road
Dokmai Prawet Bangkok 10250
Tel: +66 (0) 2069-9773
www.pentacal.com

Certificate of Calibration

Represent to Certificate of Calibration ,PTC/07/22102

Certificate No.:	PTC/07/22102	Page:	1 of 2
Equipment:	Digital Balance	Condition:	Normal
Manufacturer:	Sartorius	Serial No:	25409664
Model:	LA130S-F	ID No:	RYG_EN0001
Type of Balance:	Single interval		



Customer: ALS Laboratory Group (Thailand) Co.,Ltd.
616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand



Environment Condition: Temperature 23.9 °C ± 0.3 °C
Humidity 58.1 %RH ± 4.4 %RH
Air density 1.17 kg/m³

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd.
616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand

The Method used: In house method, PTC-WI-07, base on Euramet cg. 18

Traceability: This certificate is traceable to the SI Units through Thai Calibration Service Co.,Ltd.
, NSC-ONSC Accreditation No.: Calibration 0189

Date Received: March 23, 2022

Calibration Date: March 23, 2022

Issued Date: March 25, 2022

Calibration By: Mr. Rungroje Metakul



PENTA CALIBRATION CO.,LTD

[Signature]

(Mr.Kriangsak Kalasri)

Reviewed by

Approved By :

[Signature]

(Mr. Keattisak Kerdto)

Laboratory Manager

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognised national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The effect that the results relate only to the items calibrated.

This calibration certificate shall not be reproduced except in full only, without written approval from penta calibration co., ltd



Represent to Certificate of Calibration ,PTC/07/22102

Certificate No.: PTC/07/22102



Page: 2 of 2

Measurement Results:

Without Adjustment :

Function Calibration: Non Adjustment

Eccentric Error: Weight to be 1/3 ,1/2 or of Maximum capacity

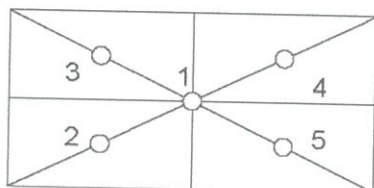

Eccentricity test 50 (g)

Position (g)				
1	2	3	4	5
0.0000	0.0000	-0.0001	0.0000	0.0001
Maximum deviation:			0.0001	

Repeatability Test : Weight to be $1/2 \leq L_1 \leq$ Maximum capacity

Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
100	0.00009

Error of indication : from nominal value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Indication (g)	Correction of Balance (g)	Uncertainty (g)	k
0	0.00000	0.0000	0.0000	0.00026	2.87
0.01	0.01000	0.0100	0.0000	0.00026	2.65
0.05	0.05000	0.0500	0.0000	0.00026	2.65
0.1	0.10000	0.1000	0.0000	0.00026	2.65
0.5	0.50000	0.4999	0.0001	0.00026	2.65
1	1.00000	0.9999	0.0001	0.00026	2.65
2	2.00000	1.9999	0.0001	0.00026	2.65
5	5.00001	5.0000	0.0000	0.00026	2.65
10	10.00000	10.0001	-0.0001	0.00026	2.65
20	20.00003	20.0001	-0.0001	0.00026	2.52
100	100.00004	100.0001	-0.0001	0.00027	2.18

Note: Weight of adjust - (g)


The End of Certificate



High Volume Air Sampler Calibration Worksheet

Project Site :	B.Grimm Power(AIE-MTP)Limited	Barometric Pressure (mm Hg) :	757
Calibrate Location :	สถานีที่1 วัดประชมมิตรบารุง	Temperature (°C) :	32
Calibrate Date :	27-Apr-22	High Volume ID :	RYG_FS0295
CalibrationSheet No.:	C-270422-RYG_FS0295	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	5502
Calibrator Model :	TE-5028A	Calibrator Slope :	1.53016
Calibrator S/N :	1166	Calibrator Intercept :	-0.0468

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	1.8	0.9118	32	Slope : 30.9077 Intercept : 3.8140 Correlation Coefficient : 0.9998
2	2.4	1.0456	36	
3	3.0	1.1635	40	
4	3.8	1.3036	44	
5	4.6	1.4295	48	

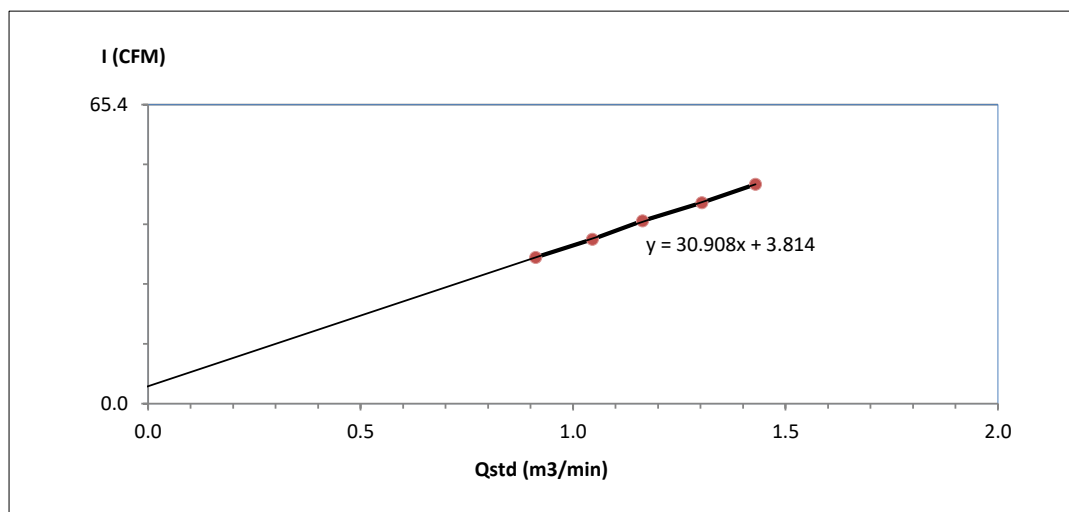

Calibrated by SA

(Mr.Santi Chaichana)
Field Scientist(1)

Approved by : 2. Noppong


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)



High Volume Air Sampler Calibration Worksheet

Project Site :	B.Grimm Power(AIE-MTP)Limited	Barometric Pressure (mm Hg) :	757
Calibrate Location :	สถานที่ 3 บ้านสำนักมวง	Temperature (°C) :	32
Calibrate Date :	27-Apr-22	High Volume ID :	RYG_FS0185
CalibrationSheet No.:	C-270422-RYG_FS0185	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	4793
Calibrator Model :	TE-5028A	Calibrator Slope :	1.53016
Calibrator S/N :	1166	Calibrator Intercept :	-0.0468

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	1.8	0.9118	32	Slope : 28.8287 Intercept : 5.6773 Correlation Coefficient : 0.9993
2	2.4	1.0456	36	
3	3.2	1.2001	40	
4	4.0	1.3362	44	
5	4.8	1.4593	48	

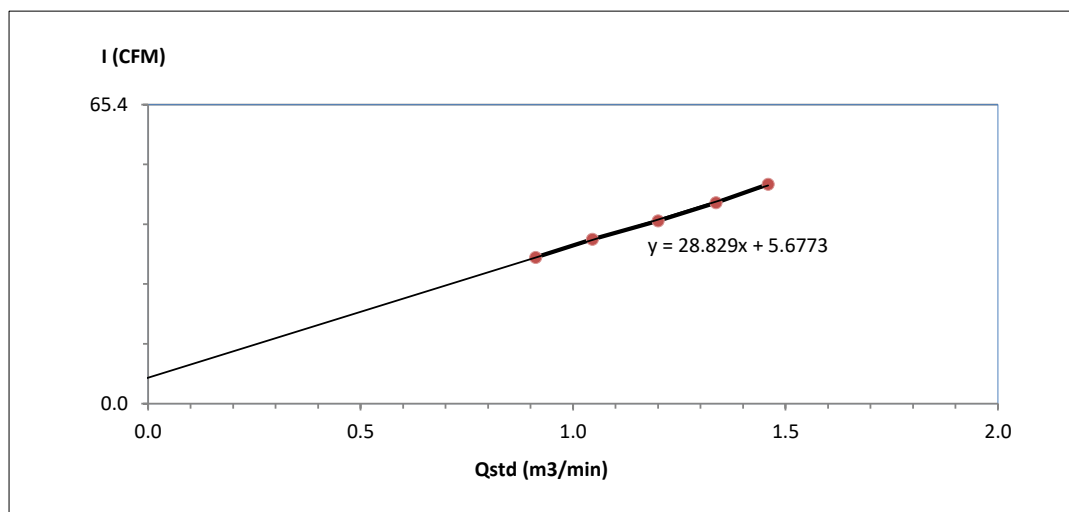

Calibrated by 

(Mr.Santi Chaichana)
Field Scientist(1)

Approved by : 


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)



High Volume Air Sampler Calibration Worksheet

Project Site :	B.Grimm Power(AIE-MTP)Limited	Barometric Pressure (mm Hg) :	757
Calibrate Location :	สถานที่ที่ 4 โรงเรียนอนุบาลรักภาษา	Temperature (°C) :	32
Calibrate Date :	27-Apr-22	High Volume ID :	RYG_FS0188
CalibrationSheet No.:	C-270422-RYG_FS0188	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	4796
Calibrator Model :	TE-5028A	Calibrator Slope :	1.53016
Calibrator S/N :	1166	Calibrator Intercept :	-0.0468

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	1.8	0.9118	32	Slope : 30.8089 Intercept : 3.7040 Correlation Coefficient : 0.9982
2	2.4	1.0456	36	
3	3.2	1.2001	40	
4	3.8	1.3036	44	
5	4.6	1.4295	48	

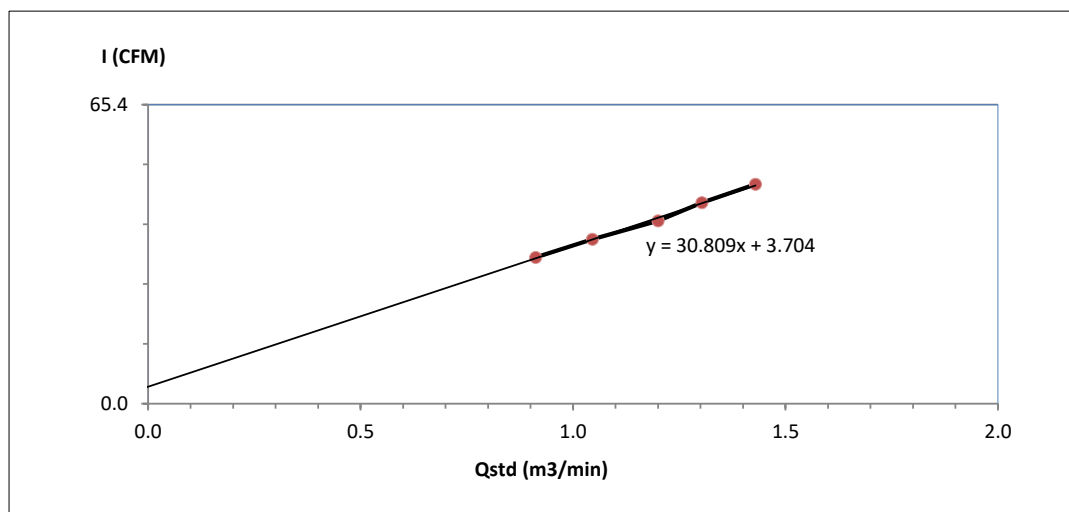

Calibrated by

(Mr.Santi Chaichana)
Field Scientist(1)

Approved by :

(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

CERTIFICATE OF CALIBRATION

Certificate No: WS-02092021

Page 1 of 2 pages

Measurement Item : Cup anemometer with data logger.

Manufacturer : Data logger: Novalynx.
: Cup anemometer: Novalynx.

Model/Type : Data logger: 110-WS-25DL-D
: Cup anemometer: WS-02F

Serial Number : Data logger: A5816
: Cup anemometer: WSD-016

ID No : Data logger: - R16 5509416
: Cup anemometer: -

Customer : ALS laboratory group (Thailand) co., ltd.
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

Test Conditions : Wind tunnel cross test section area 900 cm²
: Anemometer frontal area 100 cm²
: Diameter of mounting pipe - mm
: Blockage ratio of test object 0.111 [-]

Test Conditions : Air temperature 23.6 ±0.8 °C
: Air pressure 1012.9 ±0.4 hPa
: Relative air humidity 57.8 ±3.5 %RH

Calibration Procedure : Calibration was carried out base on;
IEC 61400-12-1 ED.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines;
MEASNET Anemometer Calibration Procedure – Version 2: 2009;

Traceability : This calibration documents the traceable to national standard, Which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).

Measurement Date : Sep 14, 2021.
Issued Date : Sep 15, 2021.

Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwitaya



Approved Signatory:

Mr. Parinya Booncharoen

Mr. Parinya Booncharoen
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-02092021

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V _{STD} Reading m/s	V _{UUC*} Reading m/s	Error (m/s)	Uncertainty (%)
2.045	2.0	0.0	2.4
4.087	4.0	-0.1	1.5
5.98	6.0	0.0	1.2
8.01	8.0	0.0	0.84
10.02	10.1	0.1	0.67
12.02	12.2	0.2	0.63
14.00	14.2	0.2	0.42
15.99	16.2	0.2	0.76
14.99	15.2	0.2	0.49
13.01	13.1	0.1	0.51
11.02	11.1	0.1	0.66
9.02	9.0	0.0	0.65
7.00	7.0	0.0	0.90
5.122	5.1	0.0	1.3
2.978	3.0	0.0	1.9
1.023	1.0	0.0	4.8

UUC*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TESTO INC.	06352145	Aug 07, 2021	MW-0034-21	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	Aug 07, 2021	MW-0034-21	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	Aug 08, 2021	MW-0035-21	0 – 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2021	CL-027-64	-30 – 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2021	RH-03032021	0 – 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2021	BP-01032021	500 – 1100 hPa
7	Wind tunnel	ESSOM	MP330D	-	-	0 – 50 Hz

End of certificate of calibration



CERTIFICATE OF CALIBRATION

Certificate No.: WD-02092021

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.
: Wind direction sensor: Novalynx.

Model/Type : Data logger: 110-WS-25DL-D
: Wind direction sensor: WS-02F.

Serial Number : Data logger: A5816.
: Wind direction sensor: WSD-016.

ID No : Data logger: -
: Wind direction sensor: -

Customer : ALS laboratory group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(23\pm3)^{\circ}\text{C}$, and relative humidity of $(40\pm10)\%$.

Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control, The measurement were taken at 45° intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: CC563-07-0045, Certificate No.: KWS63/0044.

Measurement Date : Sep 15, 2021.

Issued Date : Sep 15, 2021.

Performed by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:.....

Mr. Parinya Booncharoen.
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-02092021

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	360	359	-1	3.0
2		45	45	44	-1	3.0
3		90	90	87	-3	3.0
4		135	135	133	-2	3.0
5		180	180	180	0	3.0
6		225	225	225	0	3.0
7		270	270	273	3	3.0
8		315	315	317	2	3.0
9	Counter Clockwise	0/360	360	359	-1	3.0
10		45	45	44	-1	3.0
11		90	90	87	-3	3.0
12		135	135	133	-2	3.0
13		180	180	180	0	3.0
14		225	225	225	0	3.0
15		270	270	273	3	3.0
16		315	315	317	2	3.0

UUC*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

End of Certificate of Calibration

CERTIFICATE OF CALIBRATION

Certificate No. : CL-068-64

Page 1 of 2

Equipment Name : Data Logger with Temperature

Sensor

Manufacturer : Novalynx

Model : 110-WS-25 DL-D

Serial No. : A5816

ID No. : -

Customer

Name : ALS laboratory group (thailand) Co.,Ltd.

Address : 104 Phatthanakan 40, Phatthanakan
Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok
10250 Thailand.

Received date : 1 SEP 2021

Calibration date : 13 SEP 2021

Issue date : 15 SEP 2021

Reference Used During Calibration

1. Standard Temperature Probe Model : STS-100 A500,
Serial No. : 667682-09, Due date : 25 Mar 2022

2. Digital Temperature Indicator Model : DTI-1000-A MK
II, Serial No.: 671407-00591 Due date : 04 June 2022

Calibration Condition

Temperature : (23±3)°C

Relative Humidity : (55±15)%

Calibration Procedure


The temperature calibration was done by In-House
calibration method as WI-CL-001 according to
comparison method with standard digital temperature
indicator and standard temperature probe. The
temperature scale use was based on ITS-90.

Traceability

The measurement results are traceable to the
international system of units (SI) through National
Institute of Metrology Thailand (NIMT) Certificate
number : TT-0036-21, Certificate number : ER-0032-
21

Calibrated by

- ☐ Mr. Sorawit Thachalad
☒ Miss Orathai Wiwatwittaya

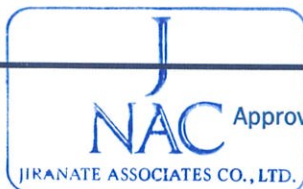

Approved Signatory: _____

25/09/21
Mr. Parinya Booncharoen
Technical Support
And Calibration Manager

Result of Calibration :- ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C – 40 °C

Function:

This equipment was connected with temperature sensor Model : HMP60 S/N : T2320595

Dimension : Diameter 12mm. Length 80 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
60	20.050	19.6	-0.4	0.080
60	24.878	24.5	-0.4	0.080
60	29.857	29.4	-0.4	0.13
60	34.848	34.3	-0.5	0.080
60	39.842	39.3	-0.5	0.080

UUC* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

*** End of Certificate ***



CALIBRATION REPORT

Calibration No. : RH-02092021

Page 1 of 1 Pages

Measurement Item : Relative humidity with data logger.

Manufacturer : Data logger: Novalynx.
: Relative humidity sensor: Novalynx.

Model/Type : Data logger: 110-WS-25 DL-D.
: Relative humidity sensor: HMP60.

Serial Number : Data logger: A5816.
: Relative humidity sensor: T2320595.

ID No : Data logger: -
: Relative humidity sensor: -.

Customer : ALS laboratory group (Thailand) co., ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(25 \pm 3)^{\circ}\text{C}$, and relative humidity of $(50 \pm 15)\%$.

Measurement Method:

The Relative humidity with data logger, Unit Under Calibration (UUC) was calibrated by comparison method with the equilibrium of standard salt solution CH_3COOK : Potassium Acetate, $\text{Mg}(\text{NO}_3)_2$: Magnesium Nitrate, KCl : Potassium Chloride to determine the errors.

Measurement Date : Sep 13, 2021

Issued Date : Sep 15, 2021

Measurement Results:

The results of calibration are reported in table below.

Standard salt solution.	Standard (%RH)	UUC _(Reading)	Error
CH_3COOK : Potassium Acetate	22.51	23.6	1.1
$\text{Mg}(\text{NO}_3)_2$: Magnesium Nitrate	52.89	53.1	0.2
KCl : Potassium Chloride	84.34	85.4	1.0

Performed by

- ☐ Mr. Sorawit Thachalad
☒ Miss Orathai Wiwatwittaya



Signatory:

Mr. Parinya Booncharoen.
Technical Support
and Calibration Manager

CERTIFICATE OF CALIBRATION

Certificate No: WS-05072021

Page 1 of 2 pages

Measurement Item : Cup anemometer with data logger.

Manufacturer : Data logger: Novalynx.
: Cup anemometer: Novalynx.

Model/Type : Data logger: 110-WS-25DL-D.
: Cup anemometer: WS-02F.

Serial Number : Data logger: A5789.
: Cup anemometer: WSD-011.

ID No : Data logger: -.
: Cup anemometer: -.

Customer : ALS laboratory group (Thailand) co., ltd.
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

Test Conditions : Wind tunnel cross test section area 900 cm²
: Anemometer frontal area 100 cm²
: Diameter of mounting pipe - mm
: Blockage ratio of test object 0.111 [-]

Test Conditions : Air temperature 23.9 ±0.8 °C
: Air pressure 1005.8 ±0.4 hPa
: Relative air humidity 61.4 ±3.5 %RH

Calibration Procedure : Calibration was carried out base on;
IEC 61400-12-1 ED.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines;
MCASNET Anemometer Calibration Procedure – Version 2: 2009;

Traceability : This calibration documents the traceable to national standard, Which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).

Measurement Date : Jul 14, 2021.

Issued Date : Jul 15, 2021.

REVIEW BY *Narakorn P.*
APPROVED BY *At U*
NEXT CAL. DATE *12/1/23*

Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:

Parinya Booncharoen
Mr. Parinya Booncharoen
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-05072021

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V _{STD} Reading m/s	V _{UUC} Reading m/s	Error (m/s)	Uncertainty (%)
2.074	1.9	-0.2	2.5
4.122	4.0	-0.1	1.4
6.00	6.0	0.0	0.99
8.02	8.0	0.0	1.04
10.03	10.0	0.0	0.59
11.98	12.3	0.3	0.57
14.02	14.2	0.2	0.48
16.02	16.3	0.3	0.36
14.96	15.2	0.2	0.46
12.99	13.2	0.2	0.51
11.02	11.1	0.1	0.66
9.02	9.0	0.0	0.97
7.02	7.0	0.0	0.96
5.120	5.0	-0.1	1.0
3.004	3.0	0.0	1.5
1.024	0.9	-0.1	5.3

UUC*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TESTO INC.	06352145	July 16, 2020	MW-0035-20	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	July 16, 2020	MW-0035-20	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	July 20, 2020	MW-0036AA-20	0 - 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2021	CL-027-64	-30 - 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2021	RH-03032021	0 – 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2021	BP-01032021	500 – 1100 hPa
7	Wind tunnel	ESSOM	MP330D	-	-	0 – 50 Hz

End of certificate of calibration



CERTIFICATE OF CALIBRATION

Certificate No.: WD-05072021

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.
: Wind direction sensor: Novalynx.

Model/Type : Data logger: 110-WS-25DL-D.
: Wind direction sensor: WS-02F.

Serial Number : Data logger: A5789.
: Wind direction sensor: WSD-011.

ID No : Data logger: -.
: Wind direction sensor: -.

Customer : ALS laboratory group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(23\pm3)^{\circ}\text{C}$, and relative humidity of $(40\pm10)\%$.

Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control, The measurement were taken at 45° intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: CC563-07-0045,
Certificate No.: KWS63/0044.

Measurement Date : Jul 14, 2021.

Issued Date : Jul 15, 2021.



Performed by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya

Approved Signatory:.....



Mr. Parinya Booncharoen.
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-05072021

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	0	0	0	3.0
2		45	45	45	0	3.0
3		90	90	90	0	3.0
4		135	135	136	1	3.0
5		180	180	183	3	3.0
6		225	225	228	3	3.0
7		270	270	272	2	3.0
8		315	315	317	2	3.0
9	Counter Clockwise	0/360	0	0	0	3.0
10		45	45	45	0	3.0
11		90	90	90	0	3.0
12		135	135	136	1	3.0
13		180	180	183	3	3.0
14		225	225	228	3	3.0
15		270	270	272	2	3.0
16		315	315	317	2	3.0

UUC*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No. : CL-051-64
Page 1 of 2

Equipment Name : Data Logger with Temperature
Sensor

Manufacturer : Novalynx

Model : 110-WS-25

Serial No. : A5789

ID No. : -

Customer

Name : ALS laboratory group (thailand) Co.,Ltd.

Address : 104 Phatthanakan 40, Phatthanakan
Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok
10250 Thailand.

Received date : 12 JUL 2021

Calibration date : 13 JUL 2021

Issue date : 13 JUL 2021

Reference Used During Calibration

1.Standard Temperature Probe Model : STS-100 A500,
Serial No. : 667682-09, Due date : 25 Mar 2022

2.Digital Temperature Indicator Model : DTI-1000-A MK
II, Serial No.: 671407-00591 Due date : 04 June 2022

Calibration Condition

Temperature : (23±3)°C

Relative Humidity : (55±15)%

Calibration Procedure

The temperature calibration was done by In-House
calibration method as WI-CL-001 according to
comparison method with standard digital temperature
indicator and standard temperature probe. The
temperature scale use was based on ITS-90.

Traceability

The measurement results are traceable to the
international system of units (SI) through National
Institute of Metrology Thailand (NIMT) Certificate
number : TT-0036-21, Certificate number : ER-0032-
21

Calibrated by

- ☐ Mr. Sorawit Thachalad
☒ Miss Orathai Wiwatwittaya



Approved Signatory:


Mr. Parinya Booncharoen
Technical Support
And Calibration Manager

Certificate No. : CL-051-64
Page 2 of 2

Result of Calibration :- ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C – 40 °C

Function:

This equipment was connected with temperature sensor Model : HMP60 S/N : S4620631

Dimension : Diameter 12mm. Length 80 mm.

<u>Immersion Depth (mm)</u>	<u>Standard Reading (°C)</u>	<u>UUC Reading (°C)</u>	<u>Error (°C)</u>	<u>Uncertainty (°C)</u>
60	20.050	19.7	-0.3	0.13
60	24.877	24.5	-0.4	0.16
60	29.860	29.4	-0.5	0.080
60	34.849	34.3	-0.5	0.080
60	39.815	39.3	-0.6	0.95

UUC* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

*** End of Certificate ***

CALIBRATION REPORT

Calibration No. : RH-01072021

Page 1 of 1 Pages

Measurement Item : Relative humidity with data logger.

Manufacturer : Data logger: Novalynx.
: Relative humidity sensor: Novalynx.

Model/Type : Data logger: 110-WS-25DL-D.
: Relative humidity sensor: HMP60.

Serial Number : Data logger: A5789.
: Relative humidity sensor: S4620631.

ID No : Data logger: -
: Relative humidity sensor: -

Customer : ALS laboratory group (Thailand) co., ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10260
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(25 \pm 3)^{\circ}\text{C}$, and relative humidity of $(50 \pm 15)\%$.

Measurement Method:

The Relative humidity with data logger, Unit Under Calibration (UUC) was calibrated by comparison method with the equilibrium of standard salt solution CH_3COOK : Potassium Acetate, $\text{Mg}(\text{NO}_3)_2$: Magnesium Nitrate, KCl : Potassium Chloride to determine the errors.

Measurement Date : Jul 14, 2021

Issued Date : Jul 14, 2021

Measurement Results:

The results of calibration are reported in table below.

Standard salt solution.	Standard (%RH)	UUC(Reading)	Error
CH_3COOK : Potassium Acetate	22.51	22.8	0.3
$\text{Mg}(\text{NO}_3)_2$: Magnesium Nitrate	52.89	53.2	0.3
KCl : Potassium Chloride	84.34	84.9	0.6

Performed by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:.....

Orathai Wiwatwittaya

Mr. Parinya Booncharoen.
Technical Support
and Calibration Manager

CERTIFICATE OF CALIBRATION

Certificate No: WS-08072021

Page 1 of 2 pages

Measurement Item : Cup anemometer with data logger.

Manufacturer : Data logger: Novalynx.
: Cup anemometer: Novalynx.

Model/Type : Data logger: 110-WS-25DL-D.
: Cup anemometer: WS-02F.

Serial Number : Data logger: A5660.
: Cup anemometer: WSD-014.

ID No : Data logger: -. 248.150930
: Cup anemometer: -.

Customer : ALS laboratory group (Thailand) co., ltd.
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

Test Conditions : Wind tunnel cross test section area 900 cm²
: Anemometer frontal area 100 cm²
: Diameter of mounting pipe - mm
: Blockage ratio of test object 0.111 [-]

Test Conditions : Air temperature 23.4 ±0.8 °C
: Air pressure 1006.2 ±0.4 hPa
: Relative air humidity 59.3 ±3.5 %RH

Calibration Procedure : Calibration was carried out base on;
IEC 61400-12-1 ED.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines;
MCASNET Anemometer Calibration Procedure – Version 2: 2009;

Traceability : This calibration documents the traceable to national standard, Which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).

Measurement Date : Jul 14, 2021.
Issued Date : Jul 15, 2021.

Calibrated by
☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



REVIEW BY *Parinya P.*
APPROVED BY *[Signature]*
NEXT CAL. DATE *12/1/23*

Approved Signatory: *[Signature]*
Mr. Parinya Booncharoen
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-08072021

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V _{STD} Reading m/s	V _{UUC} * Reading m/s	Error (m/s)	Uncertainty (%)
2.069	1.9	-0.2	2.5
4.122	4.0	-0.1	1.2
6.02	6.0	0.0	0.95
7.97	8.0	0.0	0.84
9.98	10.0	0.0	0.59
12.02	12.1	0.1	0.47
13.99	14.2	0.2	0.45
15.98	16.2	0.2	0.55
14.99	15.2	0.2	0.39
13.00	13.1	0.1	0.45
11.02	11.1	0.1	0.53
8.99	9.0	0.0	0.70
6.98	7.0	0.0	0.96
5.112	5.0	-0.1	1.2
2.975	3.0	0.0	1.5
1.023	0.9	-0.1	5.3

UUC*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TESTO INC.	06352145	July 16, 2020	MW-0035-20	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	July 16, 2020	MW-0035-20	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	July 20, 2020	MW-0036AA-20	0 - 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2021	CL-027-64	-30 - 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2021	RH-03032021	0 - 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2021	BP-01032021	500 – 1100 hPa
7	Wind tunnel	ESSOM	MP330D	-	-	0 – 50 Hz

End of certificate of calibration



CERTIFICATE OF CALIBRATION

Certificate No.: WD-08072021

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.
: Wind direction sensor: Novalynx.

Model/Type : Data logger: 110-WS-25DL-D.
: Wind direction sensor: WS-02F.

Serial Number : Data logger: A5660.
: Wind direction sensor: WSD-014.

ID No : Data logger: -.
: Wind direction sensor: -.

Customer : ALS laboratory group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(23\pm3)^{\circ}\text{C}$, and relative humidity of $(40\pm10)\%$.

Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control, The measurement were taken at 45° intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: CC563-07-0045,
Certificate No.: KWS63/0044.

Measurement Date : Jul 14, 2021.

Issued Date : Jul 15, 2021.



Performed by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya

Approved Signatory:.....

Mr. Parinya Booncharoen.
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-08072021

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	360	359	-1	3.0
2		45	45	42	-3	3.0
3		90	90	87	-3	3.0
4		135	135	134	-1	3.0
5		180	180	182	2	3.0
6		225	225	228	3	3.0
7		270	270	273	3	3.0
8		315	315	318	3	3.0
9	Counter Clockwise	0/360	360	359	-1	3.0
10		45	45	42	-3	3.0
11		90	90	87	-3	3.0
12		135	135	134	-1	3.0
13		180	180	182	2	3.0
14		225	225	228	3	3.0
15		270	270	273	3	3.0
16		315	315	318	3	3.0

UUC*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No. : CL-050-64

Page 1 of 2

Equipment Name : Data Logger with Temperature
Sensor

Manufacturer : Novalynx

Model : 110-WS-25

Serial No. : A5660

ID No. : -

Customer

Name : ALS laboratory group (thailand) Co.,Ltd.

Address : 104 Phatthanakan 40, Phatthanakan
Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok
10250 Thailand.

Received date : 12 JUL 2021

Calibration date : 13 JUL 2021

Issue date : 13 JUL 2021

Reference Used During Calibration

1.Standard Temperature Probe Model : STS-100 A500,
Serial No. : 667682-09, Due date : 25 Mar 2022

2.Digital Temperature Indicator Model : DTI-1000-A MK
II, Serial No.: 671407-00591 Due date : 04 June 2022

Calibration Condition

Temperature : $(23 \pm 3)^{\circ}\text{C}$

Relative Humidity : $(55 \pm 15)\%$

Calibration Procedure

The temperature calibration was done by In-House
calibration method as WI-CL-001 according to
comparison method with standard digital temperature
indicator and standard temperature probe. The
temperature scale use was based on ITS-90.

Traceability

The measurement results are traceable to the
international system of units (SI) through National
Institute of Metrology Thailand (NIMT) Certificate
number : TT-0036-21, Certificate number : ER-0032-
21

Calibrated by

- ☐ Mr. Sorawit Thachalad
☒ Miss Orathai Wiwatwittaya



Approved Signatory:

Mr. Parinya Booncharoen
Technical Support
And Calibration Manager

Certificate No. : CL-050-64
Page 2 of 2

Result of Calibration :- ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C – 40 °C

Function:

This equipment was connected with temperature sensor Model : HMP60 S/N : T0210901

Dimension : Diameter 12mm. Length 80 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
60	20.050	19.7	-0.3	0.080
60	24.875	24.5	-0.4	0.13
60	29.864	29.5	-0.4	0.080
60	34.829	34.3	-0.5	0.080
60	39.831	39.4	-0.5	0.95

UUC* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

*** End of Certificate ***

CALIBRATION REPORT

Calibration No. : RH-02072021

Page 1 of 1 Pages

Measurement Item : Relative humidity with data logger.

Manufacturer : Data logger: Novalynx.
: Relative humidity sensor: Novalynx.

Model/Type : Data logger: 110-WS-25DL-D.
: Relative humidity sensor: HMP60.

Serial Number : Data logger: A5660.
: Relative humidity sensor: T0210901.

ID No : Data logger: -
: Relative humidity sensor: -

Customer : ALS laboratory group (Thailand) co., ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(25 \pm 3)^{\circ}\text{C}$, and relative humidity of $(50 \pm 15)\%$.

Measurement Method:

The Relative humidity with data logger, Unit Under Calibration (UUC) was calibrated by comparison method with the equilibrium of standard salt solution CH_3COOK : Potassium Acetate, $\text{Mg}(\text{NO}_3)_2$: Magnesium Nitrate, KCl : Potassium Chloride to determine the errors.

Measurement Date : Jul 14, 2021
Issued Date : Jul 14, 2021

Measurement Results:

The results of calibration are reported in table below.

Standard salt solution.	Standard (%RH)	UUC _(Reading)	Error
CH_3COOK : Potassium Acetate	22.51	22.2	-0.3
$\text{Mg}(\text{NO}_3)_2$: Magnesium Nitrate	52.89	52.3	-0.6
KCl : Potassium Chloride	84.34	83.8	-0.5

Performed by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory: Orathai Wiwatwittaya

Mr. Parinya Booncharoen.
Technical Support
and Calibration Manager

CERTIFICATE OF CALIBRATION

Certificate No: WS-01092021

Page 1 of 2 pages

Measurement Item : Cup anemometer with data logger.

Manufacturer : Data logger: Novalynx.
: Cup anemometer: Novalynx.

Model/Type : Data logger: 110-WS-25DL-D
: Cup anemometer: WS-02F

Serial Number : Data logger: A5662
: Cup anemometer: WSD-015

ID No : Data logger: -. R16-5501A21
: Cup anemometer: -.

Customer : ALS laboratory group (Thailand) co., ltd.
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

Test Conditions : Wind tunnel cross test section area 900 cm²
: Anemometer frontal area 100 cm²
: Diameter of mounting pipe - mm
: Blockage ratio of test object 0.111 [-]


Test Conditions : Air temperature 23.0 ±0.8 °C
: Air pressure 1012.8 ±0.4 hPa
: Relative air humidity 50.4 ±3.5 %RH

Calibration Procedure : Calibration was carried out base on;
IEC 61400-12-1 ED.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines;
MEASNET Anemometer Calibration Procedure – Version 2: 2009;

Traceability : This calibration documents the traceable to national standard, Which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).

Measurement Date : Sep 14, 2021.

Issued Date : Sep 15, 2021.

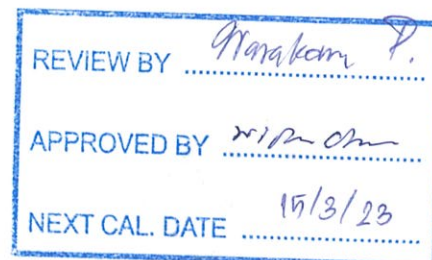

Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:

Leung P.
Mr. Parinya Booncharoen
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-01092021

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V _{STD} Reading m/s	V _{UUC} * Reading m/s	Error (m/s)	Uncertainty (%)
2.038	2.0	0.0	2.4
4.055	4.1	0.0	1.2
6.00	6.0	0.0	1.05
7.99	8.0	0.0	0.72
10.01	10.1	0.1	0.76
12.01	12.2	0.2	0.81
13.99	14.3	0.3	0.58
15.98	16.3	0.3	0.42
14.99	15.3	0.3	0.48
13.00	13.2	0.2	0.51
11.01	11.1	0.1	0.61
8.99	9.0	0.0	0.76
6.99	7.0	0.0	0.97
5.092	5.0	-0.1	1.1
2.992	3.0	0.0	1.7
1.008	1.0	0.0	4.8

UUC*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TESTO INC.	06352145	Aug 07, 2021	MW-0034-21	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	Aug 07, 2021	MW-0034-21	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	Aug 08, 2021	MW-0035-21	0 - 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2021	CL-027-64	-30 - 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2021	RH-03032021	0 - 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2021	BP-01032021	500 – 1100 hPa
7	Wind tunnel	ESSOM	MP330D	-	-	0 – 50 Hz

End of certificate of calibration



CERTIFICATE OF CALIBRATION

Certificate No.: WD-01092021

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.
: Wind direction sensor: Novalynx.

Model/Type : Data logger: 110-WS-25DL-D
: Wind direction sensor: WS-02F.

Serial Number : Data logger: A5662
: Wind direction sensor: WSD-015.

ID No : Data logger: -
: Wind direction sensor: -

Customer : ALS laboratory group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(23\pm3)^{\circ}\text{C}$, and relative humidity of $(40\pm10)\%$.

Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control, The measurement were taken at 45° intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: CC563-07-0045, Certificate No.: KWS63/0044.

Measurement Date : Sep 15, 2021.

Issued Date : Sep 15, 2021.

Performed by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory.....



Mr. Parinya Booncharoen.
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-01092021

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	0	0	0	3.0
2		45	45	42	-3	3.0
3		90	90	88	-2	3.0
4		135	135	134	-1	3.0
5		180	180	181	1	3.0
6		225	225	226	1	3.0
7		270	270	273	3	3.0
8		315	315	318	3	3.0
9	Counter Clockwise	0/360	0	0	0	3.0
10		45	45	42	-3	3.0
11		90	90	88	-2	3.0
12		135	135	134	-1	3.0
13		180	180	181	1	3.0
14		225	225	226	1	3.0
15		270	270	273	3	3.0
16		315	315	318	3	3.0

UUC*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No. : CL-067-64

Page 1 of 2

Equipment Name : Data Logger with Temperature
Sensor

Manufacturer : Novalynx
Model : 110-WS-25 DL-D
Serial No. : A5662
ID No. : -

Customer

Name : ALS laboratory group (thailand) Co.,Ltd.
Address : 104 Phatthanakan 40, Phatthanakan
Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok
10250 Thailand.

Received date : 1 SEP 2021

Calibration date : 13 SEP 2021

Issue date : 15 SEP 2021

Reference Used During Calibration

- 1.Standard Temperature Probe Model : STS-100 A500,
Serial No. : 667682-09, Due date : 25 Mar 2022
- 2.Digital Temperature Indicator Model : DTI-1000-A MK
II, Serial No.: 671407-00591 Due date : 04 June 2022

Calibration Condition

Temperature : $(23 \pm 3)^{\circ}\text{C}$
Relative Humidity : $(55 \pm 15)\%$

Calibration Procedure


The temperature calibration was done by In-House
calibration method as WI-CL-001 according to
comparison method with standard digital temperature
indicator and standard temperature probe. The
temperature scale use was based on ITS-90.

Traceability

The measurement results are traceable to the
international system of units (SI) through National
Institute of Metrology Thailand (NIMT) Certificate
number : TT-0036-21, Certificate number : ER-0032-
21

Calibrated by

- ☐ Mr. Sorawit Thachalad
☒ Miss Orathai Wiwatwittaya

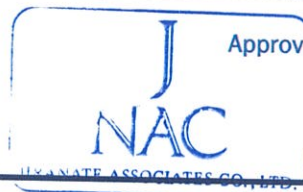

Approved Signatory:

Signature
Mr. Parinya Booncharoen
Technical Support
And Calibration Manager

Result of Calibration :- ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C – 40 °C

Function:

This equipment was connected with temperature sensor Model : HMP60 S/N : T2320591

Dimension : Diameter 12mm. Length 80 mm.

<u>Immersion Depth (mm)</u>	<u>Standard Reading (°C)</u>	<u>UUC Reading (°C)</u>	<u>Error (°C)</u>	<u>Uncertainty (°C)</u>
60	20.049	19.8	-0.2	0.080
60	24.879	24.5	-0.4	0.16
60	29.864	29.4	-0.5	0.080
60	34.847	34.4	-0.5	0.13
60	39.835	39.3	-0.5	0.080

UUC* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

* End of Certificate *



CALIBRATION REPORT

Calibration No. : RH-01092021

Page 1 of 1 Pages

Measurement Item : Relative humidity with data logger.

Manufacturer : Data logger: Novalynx.
: Relative humidity sensor: Novalynx.

Model/Type : Data logger: 110-WS-25 DL-D.
: Relative humidity sensor: HMP60.

Serial Number : Data logger: A5662.
: Relative humidity sensor: T2320591.

ID No : Data logger: -
: Relative humidity sensor: -.

Customer : ALS laboratory group (Thailand) co., ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(25 \pm 3)^{\circ}\text{C}$, and relative humidity of $(50 \pm 15)\%$.

Measurement Method:

The Relative humidity with data logger, Unit Under Calibration (UUC) was calibrated by comparison method with the equilibrium of standard salt solution CH_3COOK : Potassium Acetate, $\text{Mg}(\text{NO}_3)_2$: Magnesium Nitrate, KCl : Potassium Chloride to determine the errors.

Measurement Date : Sep 13, 2021
Issued Date : Sep 15, 2021

Measurement Results:

The results of calibration are reported in table below.

Standard salt solution.	Standard (%RH)	UUC _(Reading)	Error
CH_3COOK : Potassium Acetate	22.51	23.5	1.0
$\text{Mg}(\text{NO}_3)_2$: Magnesium Nitrate	52.89	53.1	0.2
KCl : Potassium Chloride	84.34	83.9	-0.4

Performed by

- ☐ Mr. Sorawit Thachalad
☒ Miss Orathai Wiwatwittaya



Signatory: _____

Handwritten signature

Mr. Parinya Booncharoen.
Technical Support
And Calibration Manager

SITHIPORN ASSOCIATES CO.,LTD.

CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACC21010

Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR
Manufacturer : RION
Model : NC-74
Serial No.: 34178124
ID No.: RYG_FS0216

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 05 AUGUST 2021
Calibration Date : 09 AUGUST 2021
Date of Issue : 11 AUGUST 2021

Calibrated by : Nathakorn Pisutpaisan

Approved by :


(Thanakul Petchurai)

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	9/8/22

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACC21010

Job No. : VC64AC0058

Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	8846A	1997025	EEL.BP. 06/0264	05-Feb-22
Digital Multimeter	33461A	MY53220116	EEL.BP. 04/0264	10-Feb-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22
Audio Analyzer	AVR-3360A	V744B6069	EF-0010-21	10-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACC21010
Job No. : VC64AC0058
Pages : 3 of 3

Result of calibration :**1. Sound pressure level**

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit (dB)
94	94.16	0.16	0.23	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Tolerance limit (%)
1000	1001.3	0.1	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Tolerance limit (%)
1.88	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL21080

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00597169 / 180411 / 88181
ID No.: RYG_FS0439

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 05 AUGUST 2021
Calibration Date : 06 -10 AUGUST 2021
Date of Issue : 11 AUGUST 2021

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	6/8/22

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL21080

Job No. : VC64AC0058

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	8846A	1997025	EEL.BP. 06/0264	05-Feb-22
Digital Multimeter	33461A	MY53220116	EEL.BP. 04/0264	10-Feb-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL21080

Job No. : VC64AC0058

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL21080

Job No. : VC64AC0058

Pages : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.96)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.6
C - weight	17.5
Flat	23.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.2	0.3	0.3	± 1.5
1000	0.0	0.0	0.1	± 1.0
8000	1.3	1.4	1.4	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL21080

Job No. : VC64AC0058

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL21080
Job No. : VC64AC0058
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.8	-0.2	± 1.1
25.0	24.9	-0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL21080

Job No. : VC64AC0058

Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.3	-1.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL21080

Job No. : VC64AC0058

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate