

# ภาคผนวก จ

---

ใบรับรองการสอบเทียบเครื่องมือ



ALS Laboratory Group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand  
T +66 2 760 3000 F +66 2 760 3197

### รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Total Suspended Particulate	High Volume	BKK_FS0373	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	BKK_FS1058	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	BKK_FS0370	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	BKK_EN0004	25-Feb-22	25-Feb-23	12
Ambient	Particulate Matter (PM-10)	High Volume	BKK_FS0382	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	BKK_FS0380	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	BKK_FS0381	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	Digital Balance	BKK_EN0004	25-Feb-22	25-Feb-23	12
Ambient	Nitrogen Dioxide	NO <sub>2</sub> Analyzer	BKK_FS0779	4-Jan-22	4-Jul-22	6
Ambient	Nitrogen Dioxide	NO <sub>2</sub> Analyzer	BKK_FS0728	4-Jan-22	4-Jul-22	6
Ambient	Nitrogen Dioxide	NO <sub>2</sub> Analyzer	BKK_FS0800	4-Jan-22	4-Jul-22	6
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0920	8-Oct-21	8-Apr-23	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0165	3-May-22	1-Nov-23	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0167	11-May-21	9-Nov-22	18
Stack	Oxides of Nitrogen	Console Control Unit	BKK_FS0507	4-Jan-22	4-Jul-22	6
Stack	Oxides of Nitrogen	Console Control Unit	BKK_FS0485	5-Jan-22	5-Jul-22	6
Stack	Oxides of Nitrogen	Console Control Unit	BKK_FS0547	11-Jan-22	11-Jul-22	6
Stack	Oxides of Nitrogen	Vacuum Gauge	BKK_FS0893	26-Nov-20	27-May-22	18
Stack	Oxides of Nitrogen	Vacuum Gauge	BKK_FS0483	24-May-21	22-Nov-22	18
Stack	Oxides of Nitrogen	Spectrophotometer	BKK_EN0018	15-Oct-21	15-Oct-22	12
Stack	Total Suspended Particulate	Console Control Unit	BKK_FS0507	4-Jan-22	4-Jul-22	6
Stack	Total Suspended Particulate	Console Control Unit	BKK_FS0485	5-Jan-22	5-Jul-22	6
Stack	Total Suspended Particulate	Console Control Unit	BKK_FS0547	11-Jan-22	11-Jul-22	6
Stack	Total Suspended Particulate	Digital Balance	BKK_EN0309	16-Dec-21	16-Dec-22	12
Workplace	Total Dust	Field Rotameter	BKK_FS1025	1-Apr-22	1-Jul-22	3
Workplace	Total Dust	Digital Balance	BKK_EN0004	25-Feb-22	25-Feb-23	12
Workplace	Respirable Dust	Field Rotameter	BKK_FS1025	1-Apr-22	1-Jul-22	3
Workplace	Respirable Dust	Digital Balance	BKK_EN0004	25-Feb-22	25-Feb-23	12
Noise	Leq 24 hrs	Sound Calibrator	BKK_FS0618	18-Oct-21	18-Oct-22	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0103	9-Nov-21	9-Nov-22	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0104	9-Nov-21	9-Nov-22	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0021	19-May-21	19-May-22	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0922	12-Jan-22	12-Jan-23	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0113	12-Jan-22	12-Jan-23	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0018	28-Jun-21	28-Jun-22	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0021	19-May-21	19-May-22	12
Noise	Leq 8 hrs	Sound Calibrator	BKK_FS0617	9-Aug-21	9-Aug-22	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0995	6-Aug-21	6-Aug-22	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0994	6-Aug-21	6-Aug-22	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0997	12-Jan-22	12-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0971	12-Jan-22	12-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0969	12-Jan-22	12-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0971	12-Jan-22	12-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0993	12-Oct-21	12-Oct-22	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0995	6-Aug-21	6-Aug-22	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0993	12-Oct-21	12-Oct-22	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0997	12-Jan-22	12-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0969	12-Jan-22	12-Jan-23	12



ALS Laboratory Group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand  
T +66 2 760 3000 F +66 2 760 3197

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ


Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Heat	Heat Stress	Heat Stress Monitor	BKK_FS0648	14-Feb-22	14-Feb-23	12
Heat	Heat Stress	Heat Stress Monitor	BKK_FS0649	17-Mar-22	17-Mar-23	12
Heat	Heat Stress	Heat Stress Monitor	BKK_FS0650	1-Jun-22	1-Jun-23	12
Heat	Heat Stress	Heat Stress Monitor	BKK_FS0651	1-Jun-22	1-Jun-23	12
Heat	Heat Stress	Heat Stress Monitor	BKK_FS0662	27-May-22	27-May-23	12
Heat	Heat Stress	Heat Stress Monitor	BKK_FS0667	14-Feb-22	14-Feb-23	12
Heat	Heat Stress	Heat Stress Monitor	BKK_FS0672	17-Mar-22	17-Mar-23	12
Heat	Heat Stress	Heat Stress Monitor	BKK_FS0680	15-Feb-22	15-Feb-23	12



## High Volume Air Sampler Calibration Worksheet

Project Site :	Kosei Aluminum(Thailand) Co.,Ltd.	Barometric Pressure (mm Hg) :	754
Calibrate Location :	สถานที่ 1 วัดโคกมะยม	Temperature ( °C ) :	37
Calibrate Date :	12-May-22	High Volume ID :	BKK_FS0373
CalibrationSheet No.:	C-120522-BKK_FS0373	High Volume Model :	G1051
Calibrator ID:	BKK_FS0624	High Volume S/N :	1330
Calibrator Model :	TE-5028A	Calibrator Slope :	1.64942
Calibrator S/N :	2584	Calibrator Intercept :	-0.02902

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	3.5	1.1367	40	Slope : 38.3179 Intercept : -4.0496 Correlation Coefficient : 0.9979
2	4.4	1.2710	44	
3	5.4	1.4049	50	
4	6.4	1.5268	54	
5	7.6	1.6612	60	

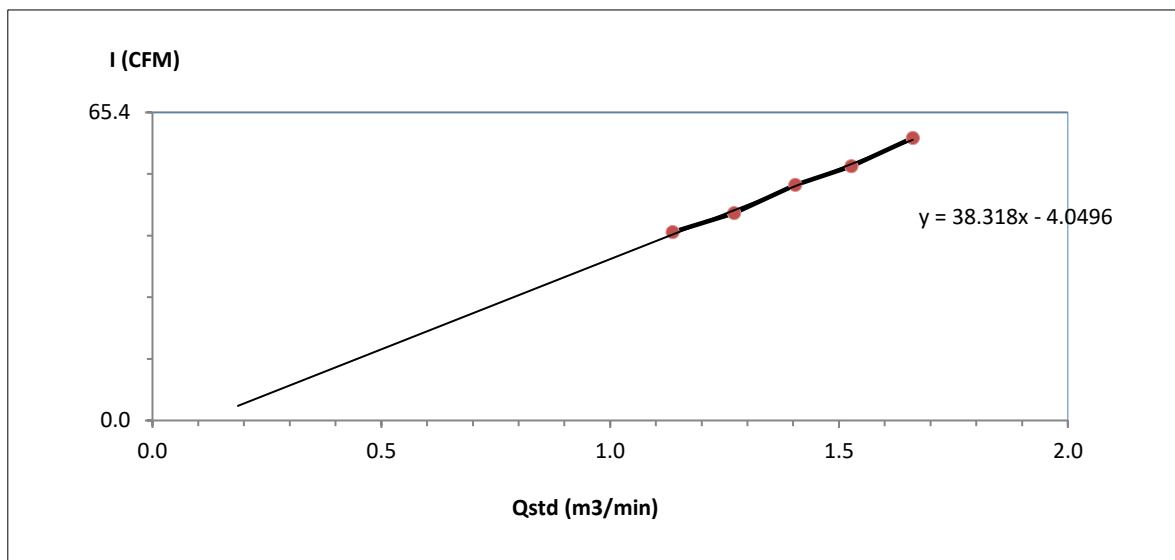

Calibrated by                       
 ( Mr. Thanong Wiriyasahakit )  
 Field Scientist(4)

Approved by :                       
 (Mr. Noppong Juntarupan)  
 Enviro Field Coordinator Scientist (3)






## High Volume Air Sampler Calibration Worksheet

Project Site :	Kosei Aluminum(Thailand) Co.,Ltd.	Barometric Pressure (mm Hg) :	754
Calibrate Location :	สถานที่ 2 วัดคานหาม	Temperature ( °C ) :	37
Calibrate Date :	12-May-22	High Volume ID :	BKK_FS1058
CalibrationSheet No.:	C-120522-BKK_FS1058	High Volume Model :	TE-5009X
Calibrator ID:	BKK_FS0624	High Volume S/N :	5689
Calibrator Model :	TE-5028A	Calibrator Slope :	1.64942
Calibrator S/N :	2584	Calibrator Intercept :	-0.02902

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	3.4	1.1207	40	Slope : 37.0040 Intercept : -1.8922 Correlation Coefficient : 0.9975
2	4.3	1.2568	44	
3	5.3	1.3921	50	
4	6.4	1.5268	54	
5	7.6	1.6612	60	

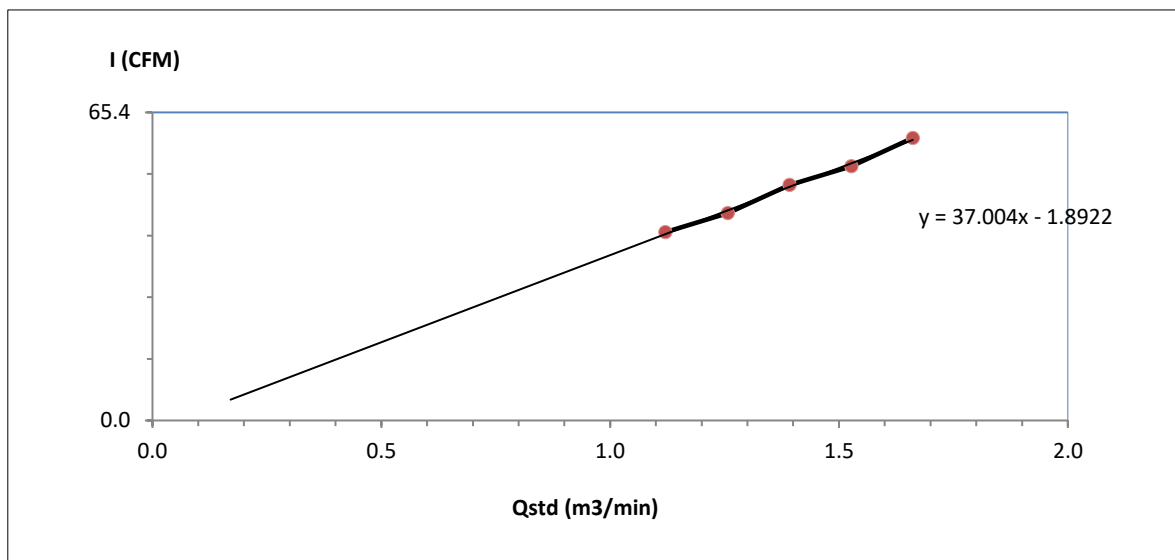

Calibrated by                       
 ( Mr. Thanong Wiriyasahakit )  
 Field Scientist(4)

Approved by :                       
 (Mr. Noppong Juntarupan)  
 Enviro Field Coordinator Scientist (3)



**Calibrator Intercept :** -0.02902

FORM NO.: F 06-073 REVISION NO.: - ISSUE DATE: 14/03/16



## Certificate of Calibration


Represent to Certificate of Calibration ,PTC/07/22072

Certificate No.:	PTC/07/22072	Page:	1 of 3
Equipment:	Digital Balance	Condition:	Normal
Manufacturer:	METTLER TOLEDO	Serial No:	1123091884
Model:	XP105	ID No:	BKK_EN0004
Type of Balance:	Multi interval		



Customer: ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakarn 40 Phatthanakarn Rd.,  
khwaeng Phatthanakarn, Khet Suan Luang, Bangkok 10250.

Environment Condition: Temperature 21.0 °C ± 0.4 °C  
Humidity 62.8 %RH ± 3.7 %RH  
Air density 1.20 kg/m<sup>3</sup>

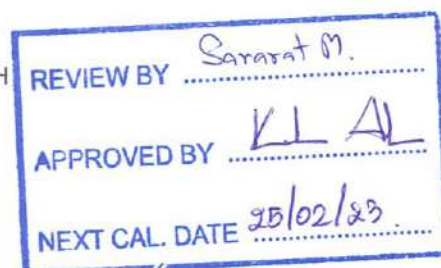

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakarn 40 Phatthanakarn Rd.,  
khwaeng Phatthanakarn, Khet Suan Luang, Bangkok 10250.

The Method used: In house method, PTC-WI-07, base on Euramet cg. 18

Traceability: This certificate is traceable to the SI Units through Thai Calibration Service Co.,Ltd.  
, NSC-ONSC Accreditation No.: Calibration 0189

Date Received: February 25, 2022

Calibration Date: February 25, 2022

Issued Date: March 01, 2022

Calibration By: Mr. Rungroje Metakul



PENTA CALIBRATION CO., LTD

( Mr.Kriangsak Kalasri )  
Reviewed by

Approved By :

( Mr. Keattisak Kerdto )  
Laboratory Manager

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognised national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The effect that the results relate only to the items calibrated.

This calibration certificate shall not be reproduced except in full only, without written approval from penta calibration co., ltd



Represent to Certificate of Calibration ,PTC/07/22072

Certificate No.: PTC/07/22072



Page: 2 of 3

## Measurement Results:

Without Adjustment :

Function Calibration: Non Adjustment

Eccentric Error: Weight to be 1/3 ,1/2 or of Maximum capacity

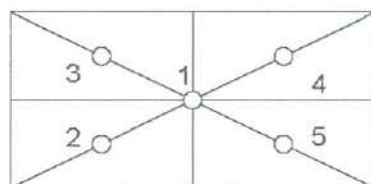

Eccentricity test 30 (g)

Position (g)				
1	2	3	4	5
0.0000	0.0000	0.0000	0.0000	0.0000
Maximum deviation:			0.0000	

Repeatability Test : Weight to be  $1/2 \leq L_1 \leq$  Maximum capacity

Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
100	0.00005

Error of indication : from nominal value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Indication (g)	Correction of Balance (g)	Uncertainty (g)	k
40	40.00005	40.0000	0.0000	0.00016	2.11
50	50.00001	50.0000	0.0000	0.00015	2.13
60	60.00003	60.0000	0.0000	0.00016	2.08
70	70.00003	70.0000	0.0000	0.00017	2.07
80	80.00005	80.0001	-0.0001	0.00019	2.04
90	90.00006	90.0001	0.0000	0.00020	2.03
100	100.00002	99.9999	0.0001	0.00018	2.06

Note: Weight of adjust - (g)



Represent to Certificate of Calibration ,PTC/07/22072

Certificate No.: PTC/07/22072



Page: 3 of 3

## Measurement Results:

Without Adjustment :

Function Calibration: Non Adjustment

Eccentric Error: Weight to be 1/3 ,1/2 or of Maximum capacity

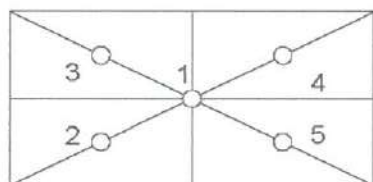

Eccentricity test 30 (g)

Position (g)				
1	2	3	4	5
0.00000	-0.00001	-0.00002	0.00000	0.00000
Maximum deviation:			0.00002	

Repeatability Test : Weight to be  $1/2 \leq L_1 \leq$  Maximum capacity

Determination of the standard deviation of weighing balance., Readability 0.00001 (g)

Nominal test value (g)	Standard Deviation
20	0.000005

Error of indication : from nominal value., Readability 0.00001 (g)

Nominal Value (g)	Conventional Mass (g)	Indication (g)	Correction of Balance (g)	Uncertainty (g)	k
0	0.000000	0.00000	0.00000	0.000016	2.52
0.1	0.100000	0.10000	0.00000	0.000019	2.00
0.5	0.499999	0.50000	0.00000	0.000019	2.00
2	2.000010	1.99999	0.00002	0.000024	2.00
5	5.000005	5.00001	0.00000	0.000027	2.00
10	10.000015	10.00001	0.00000	0.000031	2.00
20	20.000019	20.00001	0.00001	0.000042	2.00
30	30.000034	30.00006	-0.00003	0.000069	2.00

Note: Weight of adjust - (g)

The End of Certificate






## High Volume Air Sampler Calibration Worksheet

Project Site : Kosei Aluminum(Thailand) Co.,Ltd.  
Calibrate Location : สถานที่ 1 วัดโคกมะยม  
Calibrate Date : 12-May-22  
Calibration Sheet No.: C-120522-BKK\_FS0382  
Calibrator ID: BKK\_FS0624  
Calibrator Model : TE-5028A  
Calibrator S/N : 2584

Barometric Pressure (mm Hg) : 754  
Temperature ( °C ) : 37  
High Volume ID : BKK\_FS0382  
High Volume Model : TE-5009X  
High Volume S/N : 4786  
Calibrator Slope : 1.64942  
Calibrator Intercept : -0.02902

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.0	0.8663	32	Slope : 31.1255 Intercept : 5.1873 Correlation Coefficient : 0.9997
2	2.6	0.9837	36	
3	3.4	1.1207	40	
4	4.2	1.2424	44	
5	5.2	1.3791	48	

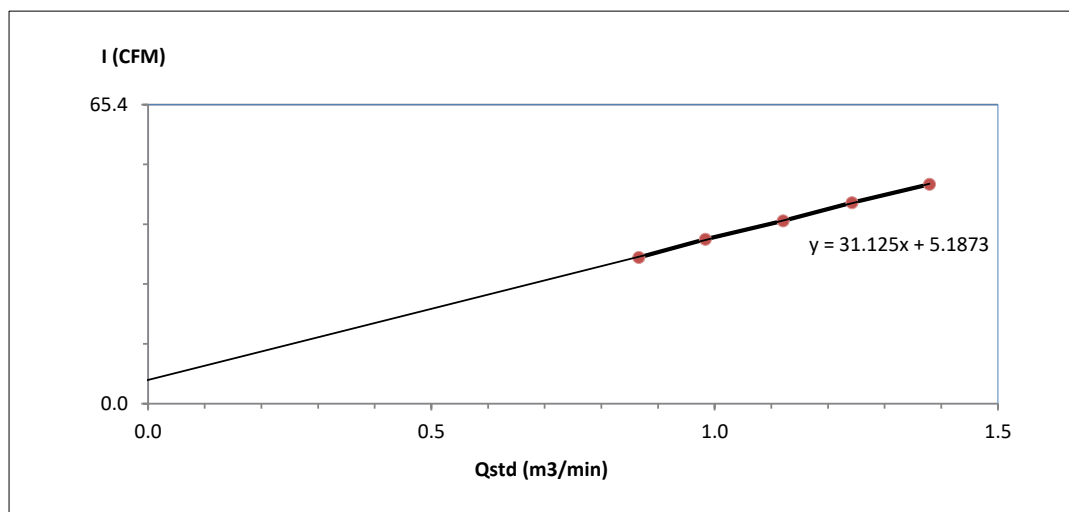

Calibrated by

( Mr. Thanong Wiriyaahakit )  
Field Scientist(4)

Approved by :


(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)



## High Volume Air Sampler Calibration Worksheet

Project Site :	<u>Kosei Aluminum(Thailand) Co.,Ltd.</u>	Barometric Pressure (mm Hg) :	<u>754</u>
Calibrate Location :	<u>สถานที่ 2 วัดคานหาม</u>	Temperature ( °C ) :	<u>37</u>
Calibrate Date :	<u>12-May-22</u>	High Volume ID :	<u>BKK_FS0380</u>
Calibration Sheet No.:	<u>C-120522-BKK_FS0380</u>	High Volume Model :	<u>TE-5009X</u>
Calibrator ID:	<u>BKK_FS0624</u>	High Volume S/N :	<u>4163</u>
Calibrator Model :	<u>TE-5028A</u>	Calibrator Slope :	<u>1.64942</u>
Calibrator S/N :	<u>2584</u>	Calibrator Intercept :	<u>-0.02902</u>

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.2	0.9072	32	Slope : 37.6190 Intercept : -2.2556 Correlation Coefficient : 0.9987
2	2.8	1.0197	36	
3	3.4	1.1207	40	
4	4.2	1.2424	44	
5	4.8	1.3262	48	

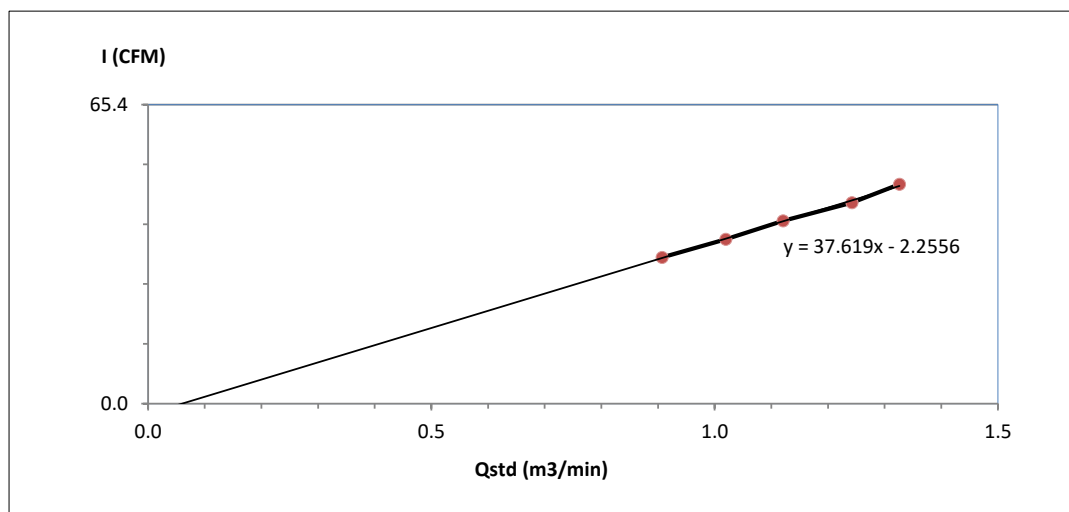

Calibrated by Thanong

( Mr. Thanong Wiriyasahakit )  
Field Scientist(4)

Approved by : Noppong

(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)






## High Volume Air Sampler Calibration Worksheet

Project Site :	Kosei Aluminum(Thailand) Co.,Ltd.	Barometric Pressure (mm Hg) :	754
Calibrate Location :	สถานีที่ 3 บ้านคานหมาม	Temperature ( °C) :	37
Calibrate Date :	12-May-22	High Volume ID :	BKK_FS0381
CalibrationSheet No.:	C-120522-BKK_FS0381	High Volume Model :	TE-5009X
Calibrator ID:	BKK_FS0624	High Volume S/N :	4161
Calibrator Model :	TE-5028A	Calibrator Slope :	1.64942
Calibrator S/N :	2584	Calibrator Intercept :	-0.02902

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.2	0.9072	32	Slope : 34.1807 Intercept : 1.2444 Correlation Coefficient : 0.9984
2	2.8	1.0197	36	
3	3.4	1.1207	40	
4	4.2	1.2424	44	
5	5.2	1.3791	48	

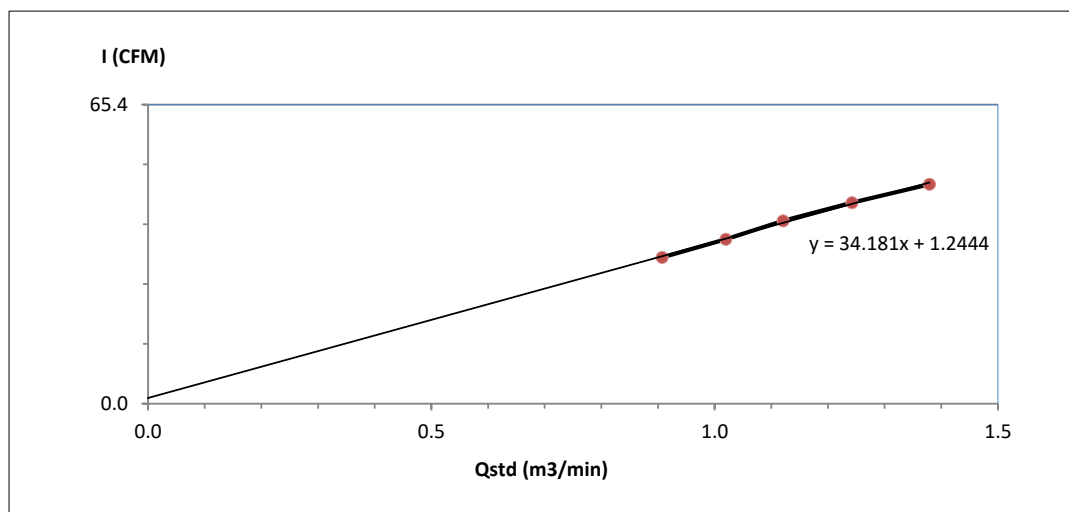

Calibrated by Thanong

( Mr. Thanong Wiriyasahakit )  
Field Scientist(4)

Approved by : Noppong

(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)




## MULTIPOINT CALIBRATION REPORT

Calibration Date 4-Jan-22  
Manufacturer HORIBA  
Serial No. VJVBGEPP  
Calibrator Manufacturer Teledyne API  
Serial No. 947  
Std. Gas Concentration (PPM) 51.33  
Cylinder Pressure (psi) 1200  
Certified Date 18-Mar-14

Equipment Name NOx Analyzer  
Model APNA-370  
Equipment ID BKK\_FS0779  
Model 700  
Cylinder No. LL36633  
Certified By Airgas Inc.  
Expired Date 18-Mar-22

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	100.10	0.10	0.10	101.00	1.00	1.00
2	200.00	199.80	-0.20	-0.10	200.50	0.50	0.25
3	300.00	299.60	-0.40	-0.13	301.20	1.20	0.40
4	400.00	400.50	0.50	0.13	402.20	2.20	0.55
AVERAGE (%)				0.02			0.46

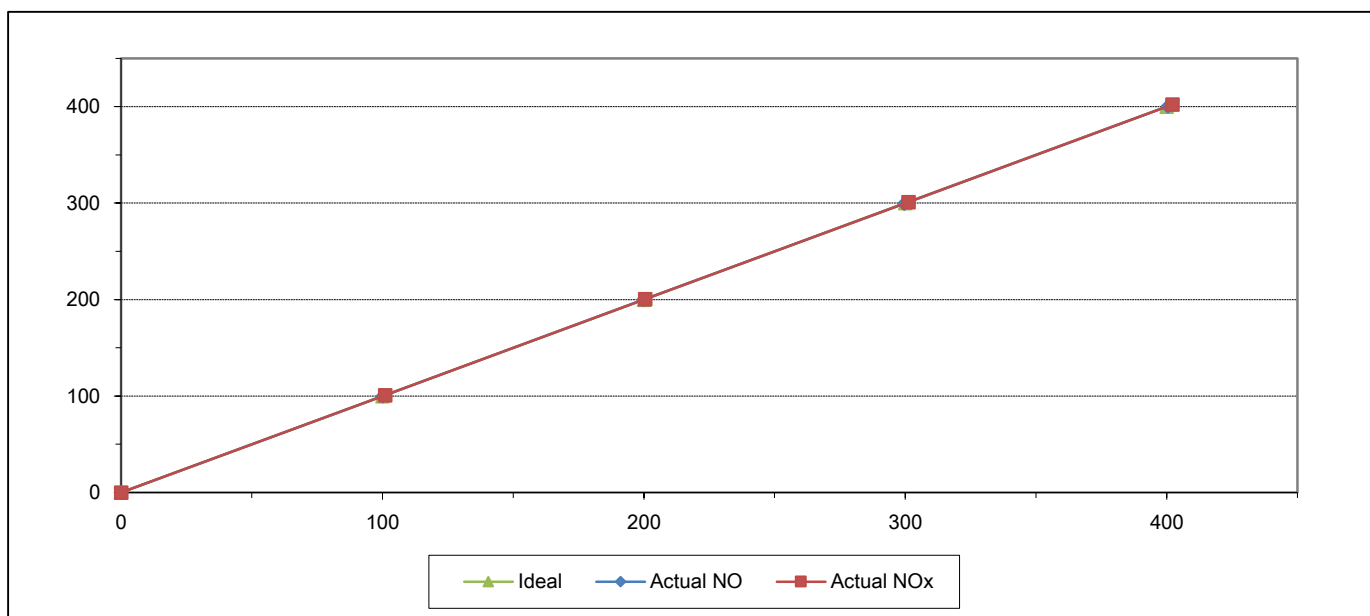

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By


( Mr.Sarayuth Jitranont )  
Assistant General Manager



## MULTIPOINT CALIBRATION REPORT

Calibration Date	4-Jan-22	Equipment Name	NOx Analyzer
Manufacturer	Teledyne API	Model	T200
Serial No.	1993	Equipment ID	BKK_FS0728
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	51.33	Cylinder No.	LL36633
Cylinder Pressure (psi)	1200	Certified By	Airgas Inc.
Certified Date	18-Mar-14	Expired Date	18-Mar-22

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	100.10	0.10	0.10	101.10	1.10	1.10
2	200.00	199.40	-0.60	-0.30	200.40	0.40	0.20
3	300.00	299.60	-0.40	-0.13	301.00	1.00	0.33
4	400.00	400.30	0.30	0.08	402.20	2.20	0.55
AVERAGE (%)				-0.03			0.46

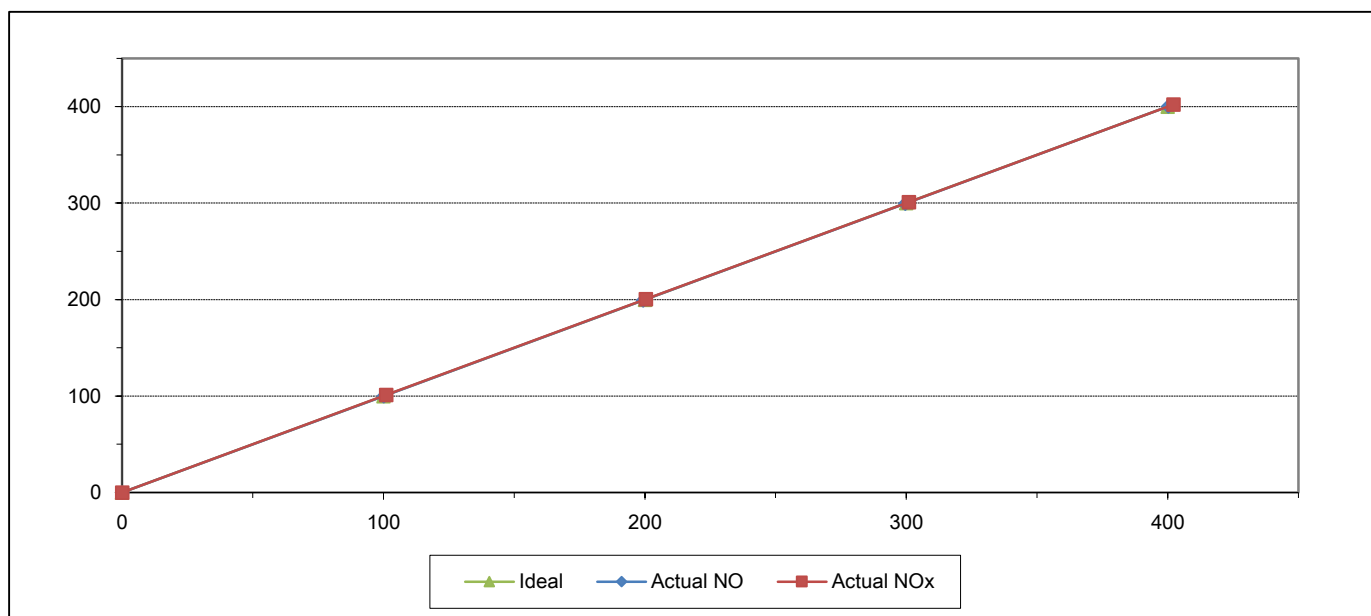

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By

( Mr.Sarayuth Jittranont )  
Assistant General Manager




## MULTIPOINT CALIBRATION REPORT

Calibration Date 4-Jan-22  
Manufacturer HORIBA  
Serial No. HCWSR681  
Calibrator Manufacturer Teledyne API  
Serial No. 947  
Std. Gas Concentration (PPM) 51.33  
Cylinder Pressure (psi) 1200  
Certified Date 18-Mar-14

Equipment Name NOx Analyzer  
Model APNA-370  
Equipment ID BKK\_FS0800  
Model 700  
Cylinder No. LL36633  
Certified By Airgas Inc.  
Expired Date 18-Mar-22

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.00	-1.00	-1.00	100.50	0.50	0.50
2	200.00	197.60	-2.40	-1.20	201.50	1.50	0.75
3	300.00	298.00	-2.00	-0.67	302.50	2.50	0.83
4	400.00	398.80	-1.20	-0.30	401.20	1.20	0.30
AVERAGE (%)				-0.61			0.50

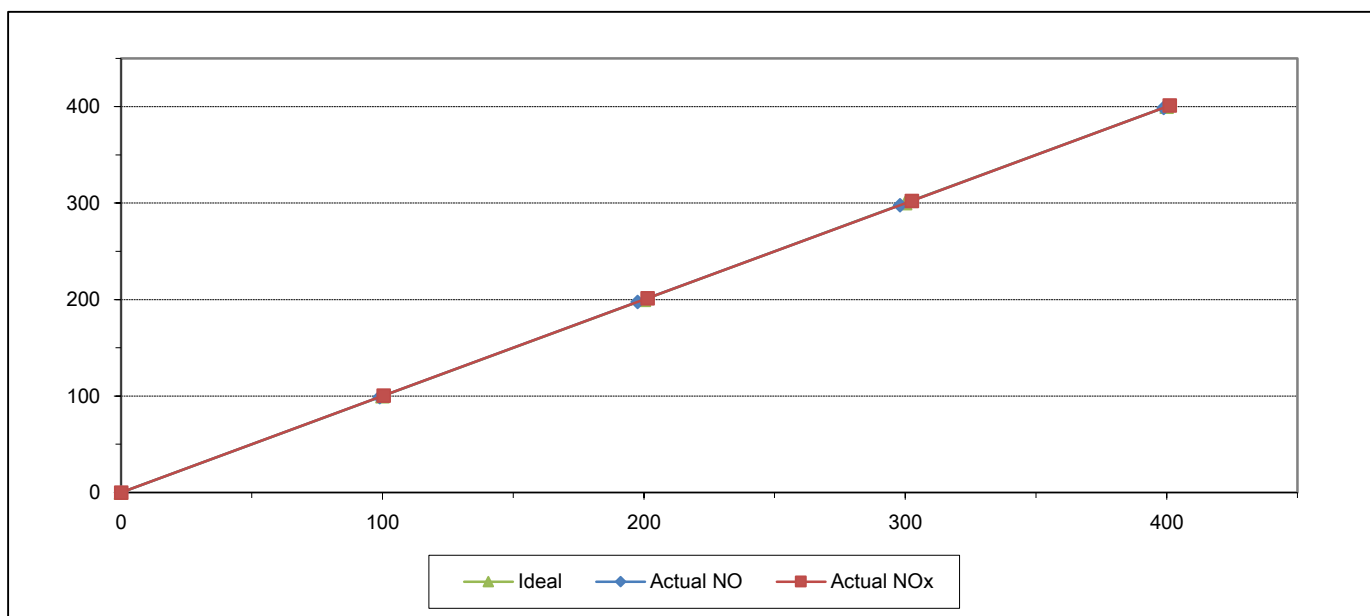

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By

( Mr.Sarayuth Jitranont )  
Assistant General Manager

## CERTIFICATE OF CALIBRATION

Certificate No: WS-02102021

Page 1 of 2 pages

Measurement Item : Cup anemometer with data logger.

Manufacturer : Data logger: Novalynx.  
: Cup anemometer: Novalynx.

Model/Type : Data logger: 200-WS-25LB  
: Cup anemometer: WS-02P

Serial Number : Data logger: A5380  
: Cup anemometer: -

ID No : Data logger: BKK\_FS0920  
: Cup anemometer: -

Customer : ALS laboratory group (Thailand) co., ltd.  
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

Test Conditions : Wind tunnel cross test section area 900 cm<sup>2</sup>  
: Anemometer frontal area 100 cm<sup>2</sup>  
: Diameter of mounting pipe - mm  
: Blockage ratio of test object 0.111 [-]

Test Conditions : Air temperature 23.3 ±0.8 °C  
: Air pressure 1007.5 ±0.4 hPa  
: Relative air humidity 46.9 ±3.5 %RH

Calibration Procedure : Calibration was carried out base on;  
IEC 61400-12-1 6D.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines;  
MGASNET Anemometer Calibration Procedure - Version 2: 2009;

Traceability : This calibration documents the traceable to national standard, which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).

Measurement Date : Oct 08, 2021.

Issued Date : Oct 11, 2021.

**Calibrated by**

- ☒ Mr. Sorawit Thachalad  
☐ Miss Orathai Wiwatwittaya



Approved Signatory: \_\_\_\_\_

*2Kmpns*  
Mr. Parinya Booncharoen  
Technical Support  
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-02102021

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V <sub>STD</sub> Reading m/s	V <sub>UUC</sub> * Reading m/s	Error (m/s)	Uncertainty (%)
2.040	2.0	0.0	2.7
4.090	4.0	-0.1	1.3
5.97	6.0	0.0	0.99
8.02	8.0	0.0	0.98
10.01	10.1	0.1	1.2
12.01	12.1	0.1	0.65
14.00	14.2	0.2	0.69
15.99	16.2	0.2	1.1
14.98	15.2	0.2	0.72
13.00	13.1	0.1	0.94
11.02	11.0	0.0	1.1
9.01	9.0	0.0	0.88
7.01	7.0	0.0	1.1
5.083	5.1	0.0	0.98
2.984	3.0	0.0	1.7
1.007	0.8	-0.2	4.6

UUC\*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

#### Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TESTO INC.	06352146	Aug 07, 2021	MW-0034-21	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	Aug 07, 2021	MW-0034-21	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	Aug 08, 2021	MW-0035-21	0 – 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2021	CL-027-64	-30 – 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2021	RH-03032021	0 – 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2021	BP-01032021	500 – 1100 hPa
7	Wind tunnel	GSSOM	MP330D	-	-	0 – 50 Hz

\*\*\*End of certificate of calibration\*\*\*





## CERTIFICATE OF CALIBRATION

Certificate No.: WD-02102021

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.  
: Wind direction sensor: Novalynx.

Model/Type : Data logger: 200-WS-25LB  
: Wind direction sensor: WS-02P

Serial Number : Data logger: A5380  
: Wind direction sensor: -

ID No : Data logger: BKK\_FS0920  
: Wind direction sensor: -

Customer : ALS laboratory group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250  
Thailand.

### Environmental Condition:

The measurement was carried out in an ambient temperature of  $(23 \pm 3)^{\circ}\text{C}$ , and relative humidity of  $(40 \pm 10)\%$ .

### Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control. The measurement were taken at  $45^{\circ}$  intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

### Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: CC563-07-0045, Certificate No.: KWS64/0025.

Measurement Date : Oct 08, 2021.

Issued Date : Oct 11, 2021.

### Performed by

- ☒ Mr. Sorawit Thachalad  
☐ Miss Orathai Wiwatwittaya



Approved Signatory: \_\_\_\_\_



Mr. Parinya Booncharoen,  
Technical Support  
and Calibration Manager



Continuation of Certificate of Calibration Number

Certificate No: WD-02102021

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	360	359	-1	3.0
2		45	45	42	-3	3.0
3		90	90	87	-3	3.0
4		135	135	132	-3	3.0
5		180	180	179	-1	3.0
6		225	225	226	1	3.0
7		270	270	272	2	3.0
8		315	315	318	3	3.0
9	Counter Clockwise	0/360	360	359	-1	3.0
10		45	45	42	-3	3.0
11		90	90	87	-3	3.0
12		135	135	132	-3	3.0
13		180	180	179	-1	3.0
14		225	225	226	1	3.0
15		270	270	272	2	3.0
16		315	315	318	3	3.0

UUC\*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

\*\*\*End of Certificate of Calibration\*\*\*



## CERTIFICATE OF CALIBRATION

Certificate No: WS-01052022

Page 1 of 2 pages

Measurement Item : Cup anemometer with data logger.

Manufacturer : Data logger: Novalynx  
: Cup anemometer: Novalynx

Model/Type : Data logger: 200-WS-25DL  
: Cup anemometer: WS-02P

Serial Number : Data logger: A4940  
: Cup anemometer: -

ID No : Data logger: BKK\_FS0165  
: Cup anemometer: -

Customer : ALS laboratory group (Thailand) co., ltd.  
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10260 Thailand.

Test Conditions : Wind tunnel cross test section area 900 cm<sup>2</sup>  
: Anemometer frontal area 100 cm<sup>2</sup>  
: Diameter of mounting pipe - mm  
: Blockage ratio of test object 0.111 [-]

Test Conditions : Air temperature 25.3 ±0.8 °C  
: Air pressure 1013.3 ±0.4 hPa  
: Relative air humidity 51.1 ±3.5 %RH

Calibration Procedure : Calibration was carried out base on;  
IEC 61400-12-1 ED.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines;  
MCASNET Anemometer Calibration Procedure – Version 2: 2009;

Traceability : This calibration documents the traceable to national standard, Which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).

Measurement Date : May 03, 2022.  
Issued Date : May 04, 2022.

Calibrated by  
☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved Signatory: \_\_\_\_\_

Mr. Parinya Booncharoen  
Calibration Department Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-01052022

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V <sub>STD</sub> Reading m/s	V <sub>UUC*</sub> Reading m/s	Error (m/s)	Uncertainty (%)
2.079	2.0	-0.1	2.4
4.145	4.0	-0.1	1.2
6.01	6.0	0.0	1.0
8.01	8.0	0.0	0.74
10.00	10.2	0.2	0.68
11.99	12.2	0.2	0.72
14.02	14.3	0.3	0.47
16.00	16.3	0.3	0.43
15.02	15.3	0.3	0.65
12.99	13.1	0.1	0.51
11.01	11.2	0.2	0.53
9.01	9.1	0.1	0.69
7.00	7.0	0.0	0.90
5.165	5.1	-0.1	0.86
3.009	3.0	0.0	1.7
1.027	0.8	-0.2	4.8

UUC\*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

#### Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TESTO INC.	06352145	Aug 07, 2021	MW-0034-21	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	Aug 07, 2021	MW-0034-21	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	Aug 08, 2021	MW-0035-21	0 - 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2022	CL-027-65	-30 - 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2022	RH-03032022	0 – 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2022	BP-01032022	500 – 1100 hPa
7	Wind tunnel	ESSOM	MP330D	-	-	0 – 50 Hz

\*\*\*End of certificate of calibration\*\*\*





## CERTIFICATE OF CALIBRATION

Certificate No.: WD-01052022

Page 1 of 2 pages

**Measurement Item** : Wind direction sensor with data logger.

**Manufacturer** : Data logger: Novalynx.  
: Wind direction sensor: Novalynx.

**Model/Type** : Data logger: 200-WS-25DL  
: Wind direction sensor: WS-02F

**Serial Number** : Data logger: A4940  
: Wind direction sensor: -

**ID No** : Data logger: BKK\_FS0165  
: Wind direction sensor: -

**Customer** : ALS laboratory group (Thailand) co., ltd.  
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250  
Thailand.

### Environmental Condition:

The measurement was carried out in an ambient temperature of  $(23 \pm 3) ^\circ\text{C}$ , and relative humidity of  $(40 \pm 10) \%$ .

### Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control. The measurement were taken at  $45^\circ$  intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

### Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: Q21086014, Certificate No.: KWS64/0025.

**Measurement Date** : May 03, 2022.  
**Issued Date** : May 04, 2022.

### Calibrated by

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved Signatory: \_\_\_\_\_

Mr. Parinya Booncharoen.  
Calibration Department Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-01052022

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 - 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	360	359	-1	3.0
2		45	45	41	-4	3.0
3		90	90	87	-3	3.0
4		135	135	132	-3	3.0
5		180	180	181	1	3.0
6		225	225	229	4	3.0
7		270	270	275	5	3.0
8		315	315	320	5	3.0
9	Counter Clockwise	0/360	360	359	-1	3.0
10		45	45	41	-4	3.0
11		90	90	87	-3	3.0
12		135	135	132	-3	3.0
13		180	180	181	1	3.0
14		225	225	229	4	3.0
15		270	270	275	5	3.0
16		315	315	320	5	3.0

UUC\*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

\*\*\*End of Certificate of Calibration\*\*\*



## CERTIFICATE OF CALIBRATION

Certificate No: WS-03062021  
Page 1 of 2 pages

Measurement Item : Cup anemometer with data logger.

Manufacturer : Data logger: Novalynx.  
: Cup anemometer: Novalynx.

Model/Type : Data logger: 200-WS-25DL.  
: Cup anemometer: WS-02P.

Serial Number : Data logger: A4984.  
: Cup anemometer: -

ID No : Data logger: BKK\_FS0167.  
: Cup anemometer: -

Customer : ALS laboratory group (Thailand) co., ltd.  
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

Test Conditions : Wind tunnel cross test section area 900 cm<sup>2</sup>  
: Anemometer frontal area 100 cm<sup>2</sup>  
: Diameter of mounting pipe - mm  
: Blockage ratio of test object 0.111 [-]

Test Conditions : Air temperature 24.1 ±0.8 °C  
: Air pressure 1014.4 ±0.4 hPa  
: Relative air humidity 60.1 ±3.5 %RH

Calibration Procedure : Calibration was carried out base on;  
: ISO 61400-12-1 CD.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines;  
: MGASNET Anemometer Calibration Procedure - Version 2: 2009;

Traceability : This calibration documents the traceable to national standard, Which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).

Measurement Date : May 11, 2021.  
Issued Date : May 12, 2021.

REVIEW BY Narakorn P.  
APPROVED BY [Signature]  
NEXT CAL. DATE 9/11/22

Calibrated by

- ☐ Mr. Sorawit Thachalad  
☒ Mr. Bongkoch Malithong



Approved Signatory: .....

[Signature]  
Mr. Parinya Booncharoen  
Technical Support  
and Calibration Manager



Continuation of Certificate of Calibration Number

Certificate No: WS-03052021

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V <sub>STD</sub> Reading m/s	V <sub>UUC</sub> * Reading m/s	Error (m/s)	Uncertainty (%)
2.053	1.9	-0.2	2.5
4.110	4.0	-0.1	1.4
5.97	6.0	0.0	1.4
8.02	8.3	0.3	1.6
9.97	10.4	0.4	0.77
11.98	12.5	0.5	0.92
14.03	14.6	0.6	0.47
16.02	17.0	1.0	0.95
15.02	15.4	0.4	0.85
12.96	13.4	0.4	1.5
10.98	11.2	0.2	1.4
8.98	9.2	0.2	1.6
6.97	7.1	0.1	2.5
5.175	5.1	-0.1	1.2
2.969	3.0	0.0	1.9
1.046	0.8	-0.2	6.0

UUC\*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

#### Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TCSTO INC.	06352145	July 16, 2020	MW-0035-20	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	July 16, 2020	MW-0035-20	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	July 20, 2020	MW-0036AA-20	0 - 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2021	CL-027-64	-30 - 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2021	RH-03032021	0 – 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2021	BP-01032021	500 – 1100 hPa
7	Wind tunnel	ESSOM	MP3300	-	-	0 – 50 Hz

\*\*\*End of certificate of calibration\*\*\*



## CERTIFICATE OF CALIBRATION

Certificate No.: WD-02052021

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.  
: Wind direction sensor: Novalynx.

Model/Type : Data logger: 200-WS-25DL  
: Wind direction sensor: WS-02F.

Serial Number : Data logger: A4984.  
: Wind direction sensor: -

ID No : Data logger: BKK\_FS0167.  
: Cup anemometer: -

Customer : ALS laboratory group (thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250  
Thailand.

### Environmental Condition:

The measurement was carried out in an ambient temperature of  $(23 \pm 3)^{\circ}\text{C}$ , and relative humidity of  $(40 \pm 10)\%$ .

### Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control. The measurement were taken at  $45^{\circ}$  intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

### Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: CC563-07-0045, Certificate No.: KWS63/0044.

Measurement Date : May 12, 2021.

Issued Date : May 12, 2021.

### Performed by

- ☐ Mr. Sorawit Thachalad  
☒ Mr. Bongkoch Malithong



Approved Signatory:.....



Mr. Parinya Booncharoen,  
Technical Support  
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-02052021

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	360	359	-1	3.0
2		45	45	44	-1	3.0
3		90	90	88	-2	3.0
4		135	135	133	-2	3.0
5		180	180	179	-1	3.0
6		225	225	227	2	3.0
7		270	270	273	3	3.0
8		315	315	318	3	3.0
9	Counter Clockwise	0/360	360	359	-1	3.0
10		45	45	44	-1	3.0
11		90	90	88	-2	3.0
12		135	135	133	-2	3.0
13		180	180	180	0	3.0
14		225	225	227	2	3.0
15		270	270	273	3	3.0
16		315	315	318	3	3.0

UUC\*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

\*\*\*End of Certificate of Calibration\*\*\*





## CONSOLE CONTROL UNIT CALIBRATION TEST REPORT

Calibration of Date : 4 Jan 22  
Next Calibration Date : 4 Jul 22

Barometric Pressure (mm.Hg) : 758  
Relative Humidity (%) : 49.0  
Temperature ( °C ) : 31.0

### Console Control Meter Data

Calibration No. : C-040122-BKK\_FS0507  
Dry Gas Meter No. : BKK\_FS0507  
Serial No. : 1503017  
Model No. : XC-572-V

### Reference Dry Gas Meter Data

Reference Dry Gas Meter ID.: BKK\_FS1122  
Serial No. : A2003240  
Correction Factor (Yr) : 1.0000  
Next Calibration Date : 1 Mar 22

$\Delta H$  (mm.H <sub>2</sub> O)	$\ominus$  Minutes	Reference Dry Gas Meter Calibration				Console Control ; Drygas Meter						Dry Gas Meter	Orifice
		Vr (Liters)			Tr  (°C)	Vm (Liters)			Ti  (°C)	To  (°C)	Avg.Tm  (°C)	Correction	Calibration
		Final	Initial	Total		Final	Initial	Total				Factor  (Y)	Factor  $\Delta H@$
15	12.06	150.00	0.00	150.00	35.0	439902.0	439750.0	152.00	33.0	33.0	33.0	0.9790	45.6446
25	9.10	150.00	0.00	150.00	34.0	440069.0	439916.0	153.00	33.0	33.0	33.0	0.9748	43.0330
50	6.27	150.00	0.00	150.00	35.0	441015.0	440860.0	155.00	32.0	32.0	32.0	0.9537	41.2601
80	5.06	150.00	0.00	150.00	35.0	441198.0	441044.0	154.00	32.0	32.0	35.0	0.9665	42.9948
120	4.06	150.00	0.00	150.00	35.0	441365.0	441212.0	153.00	32.0	32.0	36.0	0.9723	41.5201
											Avg.	0.9693	42.8905

Y : Ratio of reading of reference to dry gas meter : tolerance for individual values  $\pm 0.02$  from average .


$\Delta H@$  : Orifice pressure differential that equates to 21.24 lm of air @ 25 C and 760 mm of mercury , mmH<sub>2</sub>O ; tolerance for individual values  $\pm 5.08$  from average .

Procedure; 40 CFR 60,APP A,METH ,SEC 5.3 & 7

Calibrated by:

  
(Mr.Chawalit Wongchan )  
Field Scientist(2)

Approved by:

  
( Mr.Samart Roo-ngan )  
Specialist(1)



## Stopwatch Calibration Test Report

Calibration Date : 4 Jan 22

Next Cal. Date : 4 Jul 22

Barometric Pressure (mmHg) : 758

Temperature (°C) : 31.0

Relative Humidity (%) : 49.0

### Reference Stopwatch Data

Stopwatch ID No. : E18061

Model : F808

Serial No. : -

Calibration Date : 8 Sep 20

Certificate No. : E-2009018

### Console Control Meter Data

Dry Gas Meter No. : BKK\_FS0507

Model : XC-572-V

Serial No. : 1503017

Run No.	Time Actual (m:ss.ms)	Time Reading (m:ss)	Diff. (ms)	Diff. (min)
1	5:00:08	5:00	8	0.00013
2	5:00:11	5:00	11	0.00018
3	5:00:10	5:00	10	0.00017
4	5:00:10	5:00	10	0.00017
5	5:00:10	5:00	10	0.00017
6	5:00:10	5:00	10	0.00017
7	5:00:08	5:00	8	0.00013
8	5:00:09	5:00	9	0.00015
9	5:00:11	5:00	11	0.00018
10	5:00:12	5:00	12	0.00020
			Average	0.00017
			SD	0.00002

Calibrate by :

Mr. Chawalit Wongchan

Field Scientist (2)

Approved by :

Mr. Samart Roo-ngan

Specialist (1)



## DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	4 Jan 22	Ambient Temperature (°C) :	31
Calibration sheet No. :	C-040122-BKK_FS0508	Relative Humidity (%) :	49

Digital Temperature ID	BKK_FS0508	Reference Temperature ID :	BKK_FS0609
Serial No. :	1503017	Serial No. :	7688004
Model :	XC-572-V	Model :	FLUKE 714
		Next Calibrate :	4 Jul 22

Location	Reference Temperature °C	Digital Temperature °C	Error °C	Remark
Stack	0	1	1	
	25	26	1	
	50	51	1	
	100	101	1	
	150	151	1	
	200	201	1	
	250	252	2	
	300	302	2	
	500	503	3	
	1000	1003	3	
	1200	1203	3	
Probe	100	101	1	
	125	126	1	
	150	151	1	
Oven	100	100	0	
	125	125	0	
	150	151	1	
Filter	100	100	0	
	125	125	0	
	150	151	1	
Exit	0	1	1	
	10	11	1	
	20	21	1	
Meter	0	0	0	
	25	25	0	
	50	50	0	
AUX	0	0	0	
	25	25	0	
	50	50	0	

Calibrated by : \_\_\_\_\_

( Mr. Chawalit Wongchan )

Field Scientist (2)

Approved by : \_\_\_\_\_

( Mr.Samart Roo-ngan)

Specialist (1)



## Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK\_FS0511      Calibration Date : 4 Jan 21  
 Lab test duct Number : 258-1-13-01      Standard Pitot ID : BKK\_FS0441  
 Calibration Sheet No. : C-040122-BKK\_FS0511      Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube ( $\Delta P$ , mm.H <sub>2</sub> O)	Type s pitot tube ( $\Delta P$ , mm.H <sub>2</sub> O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			$\bar{C}_p$	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P(std)}{\Delta P(s)}}$$

$$\left| \bar{C}_{p(A)} - \bar{C}_{p(B)} \right| \text{ must BE } \leq 0.01$$

$$\text{Average deviation(A or B)} = \frac{\sum_i [Cp(s) - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by : Chawalit

( Mr. Chawalit Wongchan )

Field Scientist (2)

Approved by : [Signature]

( Mr.Samart Roo-ngan)

Specialist (1)



## Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK\_FS0512      Calibration Date : 4 Jan 22  
 Lab test duct Number : 258-1-13-01      Standard Pitot ID : BKK\_FS0441  
 Calibration Sheet No. : C-040122-BKK\_FS0512      Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube ( $\Delta P$ , mm.H <sub>2</sub> O)	Type s pitot tube ( $\Delta P$ , mm.H <sub>2</sub> O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			$\bar{C}_p$	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P(std)}{\Delta P(s)}}$$

$$\left| \bar{C}_{p(A)} - \bar{C}_{p(B)} \right| \text{ must BE } \leq 0.01$$

$$\text{Average deviation(A or B)} = \frac{\sum_{i=1}^3 [Cp(s) - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by : Chawalit

( Mr. Chawalit Wongchan )

Field Scientist (2)

Approved by : [Signature]

( Mr.Samart Roo-ngan)

Specialist (1)





## PROBE NOZZLE DIAMETER

### CALIBRATION DATA SHEET

Calibration Date	4 Jan 22	Nozzle Set ID.:	BKK_FS0513
Calibration Sheet No. :	C-040122-BKK_FS0513	Vernier Caliper ID.:	BKK_FS0626


Nozzle ID #	Nozzle Diameter (cm.)			Hi - Lo $\Delta D$	$(D_1 + D_2 + D_3) / 3$ $D_{avg}$
	$D_1$	$D_2$	$D_3$		
1	0.315	0.315	0.315	0.000	0.315
2	0.475	0.475	0.475	0.000	0.475
3	0.635	0.635	0.635	0.000	0.635
4	0.790	0.790	0.790	0.000	0.790
5	0.950	0.950	0.950	0.000	0.950
6	1.110	1.110	1.110	0.000	1.110
7	1.270	1.270	1.270	0.000	1.270

Where :

$D_1, D_2, D_3$  = Three different nozzle diameters at 60 degrees to each other, each measured the nearest 0.025 mm.

$\Delta D$  = Maximum distance between any two diameters, must be  $\leq 0.100$  mm.

$D_{avg}$  =  $(D_1 + D_2 + D_3) / 3$

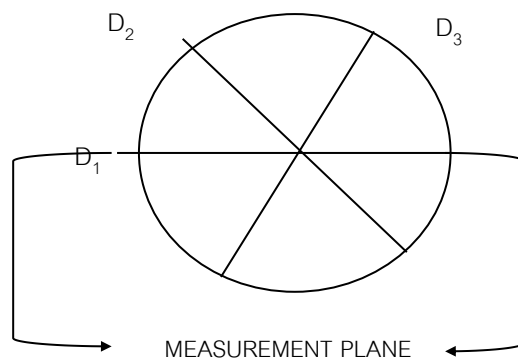

Calibrated by : \_\_\_\_\_

( Mr.Chawalit Wongchan)

Field Scientist (2)

Approved by : \_\_\_\_\_

Mr.Samart Roo-ngan

Specialist (1)



# CONSOLE CONTROL UNIT CALIBRATION TEST REPORT

Calibration of Date : 5 Jan 22

Next Calibration of Date : 5 Jul 22

Barometric Pressure (mm.Hg) : 759

Relative Humidity (%) : 61.0

Temperature ( °C ) : 30.0

## Console Control Meter Data

Calibration No. : C-050122-BKK\_FS0485

Dry Gas Meter No. : BKK\_FS0485

Serial No. : 1310055

Model No. : XC-572-V

## Reference Dry Gas Meter Data

Reference Dry Gas Meter ID.: BKK\_FS1122

Serial No. : A2003240

Correction Factor (Yr) : 1.0000

Next Calibration Date : 1 Mar 22

$\Delta H$  (mm.H <sub>2</sub> O)	$\ominus$  Minutes	Reference Dry Gas Meter Calibration				Console Control ; Drygas Meter						Dry Gas Meter Correction Factor  (Y)	Orifice Calibration Factor  $\Delta H@$
		Vr (Liters)			Tr (°C)	Vm (Liters)			Ti (°C)	To (°C)	Avg.Tm (°C)		
		Final	Initial	Total		Final	Initial	Total					
15	12.29	150.00	0.00	150.00	29.0	273149.0	272994.0	155.00	30.0	30.0	30.0	0.9695	45.9639
25	9.30	150.00	0.00	150.00	30.0	273572.0	273415.0	157.00	31.0	31.0	31.0	0.9563	44.0117
50	6.34	150.00	0.00	150.00	31.0	273743.0	273588.0	155.00	33.0	33.0	33.0	0.9694	40.9096
80	5.10	150.00	0.00	150.00	31.0	273917.0	273762.0	155.00	33.0	33.0	33.0	0.9666	42.3552
120	4.10	150.00	0.00	150.00	31.0	274120.0	273966.0	154.00	34.0	34.0	34.0	0.9723	40.9269
											Avg.	0.9668	42.8335

Y : Ratio of reading of reference to dry gas meter : tolerance for individual values  $\pm 0.02$  from average .

$\Delta H@$  : Orifice pressure differential that equates to 21.24 lm of air @ 25 C and 760 mm of mercury , mmH<sub>2</sub>O ; tolerance for individual values  $\pm 5.08$  from average .

Procedure; 40 CFR 60,APP A,METH ,SEC 5.3 & 7

Calibrated by:

Chawalit

( Mr.Chawalit Wongchan )

Field Scientist(2)

Approved by:

Samart

( Mr.Samart Roo-ngan)

Specialist(1)



## Stopwatch Calibration Test Report

Calibration Date : 5 Jan 22

Next Cal. Date : 5 Jul 22

Barometric Pressure (mmHg) : 759

Temperature (°C) : 31.0

Relative Humidity (%) : 61.0

### Reference Stopwatch Data

Stopwatch ID No. : E18061

Model : F808

Serial No. : -

Calibration Date : 8 Sep 20

Certificate No. : E-2009018

### Console Control Meter Data

Dry Gas Meter No. : BKK\_FS0485

Model : XC-572-V

Serial No. : 1310055

Run No.	Time Actual (m:ss.ms)	Time Reading (m:ss)	Diff. (ms)	Diff. (min)
1	5:00:11	5:00	11	0.00018
2	5:00:08	5:00	8	0.00013
3	5:00:09	5:00	9	0.00015
4	5:00:11	5:00	11	0.00018
5	5:00:10	5:00	10	0.00017
6	5:00:08	5:00	8	0.00013
7	5:00:08	5:00	8	0.00013
8	5:00:12	5:00	12	0.00020
9	5:00:08	5:00	8	0.00013
10	5:00:08	5:00	8	0.00013
			Average	0.00016
			SD	0.00003

Calibrate by :

Chawalit

Mr.Chawalit Wongchan

Field Scientist (2)

Approved by :

712

Mr. Samart Roo-ngan

Specialist (1)



## DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	5 Jan 22	Ambient Temperature (°C) :	32
Calibration sheet No. :	C-050122-BKK_FS0486	Relative Humidity (%) :	66

Digital Temperature ID	BKK_FS0486	Reference Temperature ID	BKK_FS0609
Serial No. :	1310055	Serial No. :	7688004
Model :	XC-572-V	Model :	FLUKE 714
		Next Calibrate :	13 Jan 22

Location	Reference Temperature °C	Digital Temperature °C	Error °C	Remark
Stack	0	0	0	
	25	24	-1	
	50	49	-1	
	100	99	-1	
	150	149	-1	
	200	199	-1	
	250	249	-1	
	300	298	-2	
	500	498	-2	
	1000	998	-2	
	1200	1198	-2	
Probe	100	98	-2	
	125	123	-2	
	150	148	-2	
Oven	100	99	-1	
	125	124	-1	
	150	150	0	
Filter	100	100	0	
	125	124	-1	
	150	149	-1	
Exit	0	-1	-1	
	10	9	-1	
	20	19	-1	
Meter	0	0	0	
	25	25	0	
	50	50	0	
AUX	0	-1	-1	
	25	25	0	
	50	50	0	

Calibrated by : \_\_\_\_\_

( Mr.Chawalit Wongchan )

Field Scientist (2)

Approved by : \_\_\_\_\_

( Mr.Samart Roo-ngan )

Specialist (1)



## Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK\_FS0489

Calibration Date : 5 Jan 22

Lab test duct Number : 258-1-13-01

Standard Pitot ID : BKK\_FS0441

Calibration Sheet No. : C-050122-BKK\_FS0489

Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube ( $\Delta P$ , mm.H <sub>2</sub> O)	Type s pitot tube ( $\Delta P$ , mm.H <sub>2</sub> O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			$\bar{C}_p$	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P(std)}{\Delta P(s)}}$$

$$\left| \bar{C}_{p(A)} - \bar{C}_{p(B)} \right| \text{ must BE } \leq 0.01$$

$$\text{Average deviation(A or B)} = \frac{\sum_{i=1}^3 [Cp(s) - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by : Chawalit

( Mr.Chawalit Wongchan )

Field Scientist (2)

Approved by : [Signature]

( Mr.Samart Roo-ngan)

Specialist (1)





## Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK\_FS0490

Calibration Date : 5 Jan 22

Lab test duct Number : 258-1-13-01

Standard Pitot ID : BKK\_FS0441

Calibration Sheet No. : C-050122-BKK\_FS0490

Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube ( $\Delta P$ , mm.H <sub>2</sub> O)	Type s pitot tube ( $\Delta P$ , mm.H <sub>2</sub> O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			$\bar{C}_p$	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P(std)}{\Delta P(s)}}$$

$$\left| \bar{C}_{p(A)} - \bar{C}_{p(B)} \right| \text{ must BE } \leq 0.01$$

$$\text{Average deviation(A or B)} = \frac{\sum_{i=1}^3 [Cp(s) - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by : Chawalit

( Mr.Chawalit Wongchan )

Field Scientist (2)

Approved by : [Signature]

( Mr.Samart Roo-ngan)

Specialist (1)



## PROBE NOZZLE DIAMETER CALIBRATION DATA SHEET

Calibration Date	5 Jan 22	Nozzle Set ID.:	BKK_FS0491
Calibration Sheet No. :	C-050122-BKK_FS0491	Vernier Caliper ID.:	BKK_FS0626


Nozzle ID #	Nozzle Diameter (cm.)			Hi - Lo $\Delta D$	$(D_1 + D_2 + D_3) / 3$ $D_{avg}$
	$D_1$	$D_2$	$D_3$		
1	0.315	0.315	0.315	0.000	0.315
2	0.475	0.475	0.475	0.000	0.475
3	0.635	0.635	0.635	0.000	0.635
4	0.790	0.790	0.790	0.000	0.790
5	0.955	0.955	0.955	0.000	0.955
6	1.110	1.110	1.110	0.000	1.110
7	1.270	1.270	1.270	0.000	1.270
8	1.600	1.600	1.600	0.000	1.600

Where :

$D_1, D_2, D_3$  = Three different nozzle diameters at 60 degrees to each other, each measured the nearest 0.025 mm.

$\Delta D$  = Maximum distance between any two diameters, must be  $\leq 0.100$  mm.

$D_{avg}$  =  $(D_1 + D_2 + D_3) / 3$

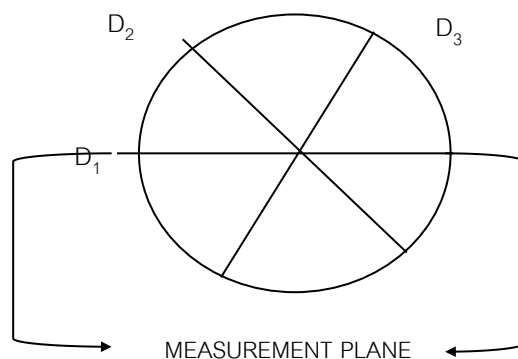

Calibrated by : Chawalit

( Mr.Chawalit Wongchan )

Field Scientist (2)

Approved by : [Signature]

Mr.Samart Roo-ngan

Specialist (1)



## CONSOLE CONTROL UNIT CALIBRATION TEST REPORT

Calibration of Date : 11 Jan 22  
 Next Calibration Date : 11 Jul 22

Barometric Pressure (mm.Hg) : 760  
 Relative Humidity (%) : 64.0  
 Temperature ( °C ) : 30.0

### Console Control Meter Data

Calibration No. : C-110122-BKK\_FS0547  
 Dry Gas Meter No. : BKK\_FS0547  
 Serial No. : 1606040  
 Model No. : XC-572-V

### Reference Dry Gas Meter Data

Reference Dry Gas Meter ID. : BKK\_FS1122  
 Serial No. : A2003240  
 Correction Factor (Yr) : 1.0000  
 Next Calibration Date : 1 Mar 22

$\Delta H$  (mm.H <sub>2</sub> O)	$\Theta$  Minutes	Reference Dry Gas Meter Calibration				Console Control ; Drygas Meter						Dry Gas Meter Correction Factor  (Y)	Orifice Calibration Factor  $\Delta H@$
		Vr (Liters)			Tr  (°C)	Vm (Liters)			Ti  (°C)	To  (°C)	Avg.Tm  (°C)		
		Final	Initial	Total		Final	Initial	Total					
15	12.90	150.00	0.00	150.00	29.0	2573.4	2420.0	153.40	29.0	29.0	29.0	0.9764	50.7407
25	9.90	150.00	0.00	150.00	29.0	2733.4	2580.0	153.40	30.0	30.0	30.0	0.9787	49.6433
50	6.86	150.00	0.00	150.00	30.0	2893.0	2740.0	153.00	31.0	31.0	31.0	0.9789	47.8310
80	5.35	150.00	0.00	150.00	30.0	3052.2	2900.0	152.20	32.0	32.0	32.0	0.9844	46.3940
120	4.35	150.00	0.00	150.00	30.0	3212.0	3060.0	152.00	33.0	33.0	33.0	0.9852	45.8567
											Avg.	0.9807	48.0932

Y : Ratio of reading of reference to dry gas meter : tolerance for individual values  $\pm 0.02$  from average .

$\Delta H@$  : Orifice pressure differential that equates to 21.24 lm of air @ 25 C and 760 mm of mercury , mmH<sub>2</sub>O ; tolerance for individual values  $\pm 5.08$  from average .

Procedure; 40 CFR 60,APP A,METH ,SEC 5.3 & 7

Calibrated by:

*Chawalit*

( Mr.Chawalit Wongchan )

Field Scientist(2)

Approved by:

*Samart*

( Mr.Samart Roo-ngan)

Specialist(1)



## Stopwatch Calibration Test Report

Calibration Date : 11 Jan 22      Next Cal. Date : 11 Jul 22  
Barometric Pressure (mmHg) : 760      Temperature (°C) : 30.0  
Relative Humidity (%) : 64.0

### Reference Stopwatch Data

Stopwatch ID No. : E18061  
Model : F808  
Serial No. : -  
Calibration Date : 8 Sep 20  
Certificate No. : E-2009018

### Console Control Meter Data

Dry Gas Meter No. : BKK\_FS0547  
Model : XC-572-V  
Serial No. : 1606040

Run No.	Time Actual (m:ss.ms)	Time Reading (m:ss)	Diff. (ms)	Diff. (min)
1	5:00:12	5:00	12	0.00020
2	5:00:12	5:00	12	0.00020
3	5:00:12	5:00	12	0.00020
4	5:00:12	5:00	12	0.00020
5	5:00:12	5:00	12	0.00020
6	5:00:12	5:00	12	0.00020
7	5:00:12	5:00	10	0.00017
8	5:00:14	5:00	15	0.00025
9	5:00:14	5:00	14	0.00023
10	5:00:14	5:00	11	0.00018
			Average	0.00020
			SD	0.00002

Calibrate by :

Mr. Worawich Tongpoom

Field Scientist (2)

Approved by :

Mr. Samart Roo-ngan

Specialist (1)



## DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	11 Jan 22	Ambient Temperature (°C) :	30
Calibration sheet No. :	C-110122-BKK_FS0548	Relative Humidity (%) :	64

Digital Temperature ID	BKK_FS0548	Reference Temperature ID :	BKK_FS1144
Console Serial No. :	1606040	Serial No. :	201090006013
Console Model :	XC-572-V	Model :	Digicon-CC-VT-MS
		Next Calibrate :	31 Jan 23

Location	Reference Temperature °C	Digital Temperature °C	Error °C	Remark
Stack	0	1	1	
	25	26	1	
	50	52	2	
	100	102	2	
	150	152	2	
	200	202	2	
	250	252	2	
	300	302	2	
	500	502	2	
	1000	1002	2	
	1200	1202	2	
Probe	100	101	1	
	125	126	1	
	150	151	1	
Oven	100	101	1	
	125	126	1	
	150	151	1	
Filter	100	101	1	
	125	126	1	
	150	151	1	
Exit	0	1	1	
	10	11	1	
	20	21	1	
Meter	0	2	2	
	25	27	2	
	50	52	2	
AUX	0	2	2	
	25	27	2	
	50	52	2	

Calibrated by : \_\_\_\_\_

Chawalit

( Mr.Chawalit Wongchan )

Field Scientist (2)

Approved by : \_\_\_\_\_

712 [Signature]

( Mr.Samart Roo-ngan)

Specialist (1)





## Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK\_FS0551

Calibration Date : 11 Jan 22

Lab test duct Number : 258-1-13-01

Standard Pitot ID : BKK\_FS0441

Calibration Sheet No. : C-110122-BKK\_FS0551

Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube ( $\Delta P$ , mm.H <sub>2</sub> O)	Type s pitot tube ( $\Delta P$ , mm.H <sub>2</sub> O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			$\bar{C}_p$	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P(std)}{\Delta P(s)}}$$

$$\left| \bar{C}_{p(A)} - \bar{C}_{p(B)} \right| \text{ must BE } \leq 0.01$$

$$\text{Average deviation(A or B)} = \frac{\sum_i [Cp(s) - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by : Chawalit

Mr.Chawalit Wongchan

Field Scientist (2)

Approved by : [Signature]

Mr.Samart Roo-ngan

Specialist (1)



## Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK\_FS0552      Calibration Date : 11 Jan 22  
 Lab test duct Number : 258-1-13-01      Standard Pitot ID : BKK\_FS0441  
 Calibration Sheet No. : C-110122-BKK\_FS0552      Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube ( $\Delta P$ , mm.H <sub>2</sub> O)	Type s pitot tube ( $\Delta P$ , mm.H <sub>2</sub> O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			$\bar{C}_p$	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P(std)}{\Delta P(s)}}$$

$$\left| \bar{C}_{p(A)} - \bar{C}_{p(B)} \right| \text{ must BE } \leq 0.01$$

$$\text{Average deviation(A or B)} = \frac{\sum_{i=1}^3 [Cp(s) - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by : Chawalit

Mr.Chawalit Wongchan  
Field Scientist (2)

Approved by : [Signature]

Mr.Samart Roo-ngan  
Specialist (1)



## PROBE NOZZLE DIAMETER CALIBRATION DATA SHEET

Calibration Date	11 Jan 22	Nozzle Set ID. :	BKK_FS0553
Calibration Sheet No. :	C-110122-BKK_FS0553	Vernier Caliper ID. :	BKK_FS0626


Nozzle ID #	Nozzle Diameter (cm.)			Hi - Lo	$(D_1 + D_2 + D_3) / 3$
	$D_1$	$D_2$	$D_3$	$\Delta D$	$D_{avg}$
1	0.310	0.310	0.310	0.000	0.310
2	0.450	0.450	0.450	0.000	0.450
3	0.635	0.635	0.635	0.000	0.635
4	0.790	0.790	0.790	0.000	0.790
5	0.950	0.950	0.950	0.000	0.950
6	1.110	1.110	1.110	0.000	1.110
7	1.270	1.270	1.270	0.000	1.270

Where :

$D_1, D_2, D_3$  = Three different nozzle diameters at 60 degrees to each other, each measured the nearest 0.025 mm.

$\Delta D$  = Maximum distance between any two diameters, must be  $\leq 0.100$  mm.

$D_{avg}$  =  $(D_1 + D_2 + D_3) / 3$

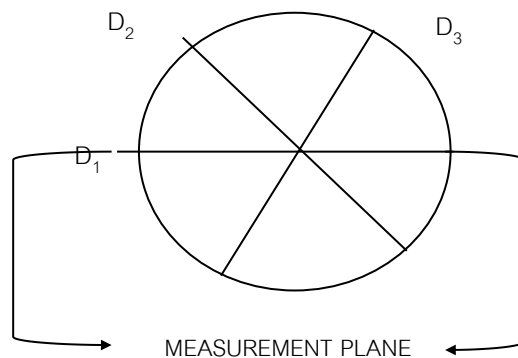

Calibrated by : Chawalit

Mr.Chawalit Wongchan  
Field Scientist (2)

Approved by : [Signature]

Mr.Samart Roo-ngan  
Specialist (1)



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 20P4915

Page : 1 of 2

Equipment : Vacuum Gauge  
Manufacturer: QualityWell  
Model : F221AVD  
Serial No.: VG03  
ID No.: BKK\_FS0893  
Condition As-Received: Used Item  
Received Date: 25 November 2020  
Calibration Date: 26 November 2020

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Reference: 2011-0973WSC  
Ambient Temperature: ( 23 ± 2 ) °C  
Relative Humidity: ( 50 ± 15 ) %  
Atmospheric Pressure: 1010 mbar

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P06, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Digital Pressure Gauge	15PSIXP2I	158670	20P3515	01 Sep 2021

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.Scale and conversion factor is 1 kPa = 0.2953 inHg

5.This instrument was used clean air as pressure media.

6.The certificate is valid only to the item calibrated on date and place of calibration.

7.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

REVIEW BY	W. Pookkuk
APPROVED BY	
NEXT CAL. DATE	27 Nov 2022

Calibrated by : Suwit Aussarree  
Issue Date : 27 November 2020

Approved Signatory : Attapol P.  
☐ Phalinee Prabpaipal  
☐ Sura Suwannasri  
☒ Attapol Panurach

B 0248078



Cert.No.: 20P4915

Page: 2 of 2

**Result of calibration:- Without adjustment**

**Range :** 0 inHg to -30 inHg

**Function:- Vacuum Pressure Measurement**

**Scale Interval :** 0.5 inHg( The Fifth Estimate )

**Increasing Pressure**

Applied Pressure (inHg)	0.00	-4.97	-9.99	-14.99	-20.00	-26.49
UUC* Indication (inHg)	0.0	-5.0	-10.0	-15.0	-20.0	-26.5
Error (inHg)	0.00	-0.03	-0.01	-0.01	0.00	-0.01

**Decreasing Pressure**

Applied Pressure (inHg)	-26.50	-20.02	-15.00	-9.99	-4.97	0.00
UUC* Indication (inHg)	-26.5	-20.0	-15.0	-10.0	-5.0	0.0
Error (inHg)	0.00	0.02	0.00	-0.01	-0.03	0.00

The uncertainty of measurement was  $\pm 0.12$  inHg

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-000-

Attapol P.

a 1030042





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 21P1828

Page : 1 of 2

Equipment : Digital Vacuum Gauge

Manufacturer: Dwyer

Model : DPGA-00

Serial No.: DVG08

ID No.: BKK\_FS0483

Condition As-Received: Used Item

Received Date: 20 May 2021

Calibration Date: 24 May 2021

Reference: 2105-0696WSC

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd.

Ambient Temperature: ( 23  $\pm$  2 ) °C

Relative Humidity: ( 50  $\pm$  15 ) %

Atmospheric Pressure: 1010 mbar

104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P06, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

### Condition of this result of calibration

#### 1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Pressure Calibrator	PC106P	1189	MP-0113-20	14 Jul 2021

2.This instrument was installed in vertical orientation and lower groove of pressure sensor was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.Scale and conversion factor is 1 kPa = 0.2953 inHg

5.This instrument was used clean air as pressure media.

6.The certificate is valid only to the item calibrated on date and place of calibration.

7.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

REVIEW BY	<i>Narakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	<i>22/11/22</i>

Calibrated by : Suwit Aussarree

Issue Date : 25 May 2021

Approved Signatory : *Attapol P.*

[ ] Phalinee Prabpaipal

[ ] Sura Suwannasri

[x] Attapol Panurach

B 0261193



Cert.No.: 21P1828

Page: 2 of 2

**Result of calibration:- Without adjustment**

**Range :** 0 inHg to -30 inHg

**Function:- Vacuum Pressure Measurement**

**Resolution :** 0.01 inHg

**Increasing Pressure**

Applied Pressure (inHg)	0.000	-4.998	-9.996	-14.994	-19.992	-26.487
UUC* Indication (inHg)	0.00	-5.08	-10.15	-15.24	-20.30	-26.89
Error (inHg)	0.000	-0.082	-0.154	-0.246	-0.308	-0.403

**Decreasing Pressure**

Applied Pressure (inHg)	-26.487	-19.992	-14.994	-9.996	-4.998	0.000
UUC* Indication (inHg)	-26.89	-20.30	-15.24	-10.15	-5.08	0.00
Error (inHg)	-0.403	-0.308	-0.246	-0.154	-0.082	0.000

The uncertainty of measurement was  $\pm 0.090$  inHg

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-

Attapol P.


a 1054849



# Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No. BSCC-UV-290/21  
Equipment UV/Vis Spectrophotometer  
Model UV-1800  
Manufacturer Shimadzu  
Serial No. A11454908533CD  
ID No. BKK\_EN0018  
Date of receipt 15 October 2021  
Date of calibration 15 October 2021  
Date of issue 25 October 2021

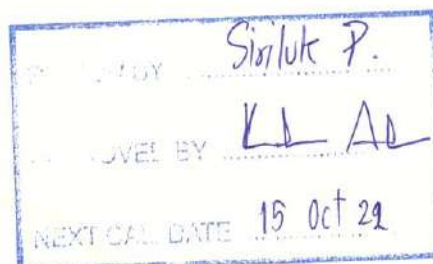

Customer name ALS Laboratory Group (Thailand) Co., Ltd.

Address 104 Soi Phatthanakan 40, Phatthanakan Road, Phatthanakan, Suan Luang, Bangkok 10250

Temperature (25.0 - 26.4) °C (On site)  
Humidity (49.5 - 53.4) %RH (On site)

Equipment condition Good Operation


Calibration Location Organic Prep

Calibration Procedure In-house method WI-UV-702-01 based on ASTM E275-01

Traceability Wavelength Accuracy is traceable to certificate No. 87839 and 87844  
Photometric Accuracy is traceable to certificate No. 87846 and 87877  
Stray Light is traceable to certificate No. 87825  
The above certificate are traceable to SI unit through Starna Scientific Ltd.  
(UKAS accredited calibration laboratory NO. 0659)

Calibrated by Mr.Wanchana Janloey

Approved by



**Mr.Kanchit Choothep**  
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

# Certificate of Calibration

Certificate No. **BSCC-UV-290/21**

Number of Page(s) **2 of 3**

## Calibration Results:

### 1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty ( $\pm$ nm)
241.70	241.55	-0.15	0.18
334.02	333.80	-0.22	0.18
418.53	418.40	-0.13	0.18
572.99	572.85	-0.14	0.18
879.41	879.15	-0.26	0.18

### 2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ( $\pm$ A)
235	0.0000	0.0000	0.0000	0.0075
	0.7174	0.7198	0.0024	0.0075
257	0.0000	-0.0001	-0.0001	0.0075
	0.8362	0.8377	0.0015	0.0075
313	0.0000	0.0000	0.0000	0.0075
	0.2778	0.2803	0.0025	0.0075
350	0.0000	-0.0001	-0.0001	0.0075
	0.6202	0.6221	0.0019	0.0075

\*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.



# Certificate of Calibration

Certificate No. **BSCC-UV-290/21**

Number of Page(s) **3 of 3**

## Calibration Results:

### 3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ( $\pm A$ )
420.0	0.0000	0.0000	0.0000	0.0042
	0.5631	0.5570	-0.0061	0.0042
	0.7390	0.7334	-0.0056	0.0042
	1.0863	1.0816	-0.0047	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5524	0.5469	-0.0055	0.0042
	0.7217	0.7166	-0.0051	0.0042
	1.0606	1.0570	-0.0036	0.0042
465.0	0.0000	0.0000	0.0000	0.0042
	0.5018	0.4966	-0.0052	0.0042
	0.6657	0.6610	-0.0047	0.0042
	0.9775	0.9740	-0.0035	0.0042
546.1	0.0000	0.0000	0.0000	0.0042
	0.5147	0.5113	-0.0034	0.0042
	0.6743	0.6705	-0.0038	0.0042
	0.9909	0.9890	-0.0019	0.0042
590.0	0.0000	0.0000	0.0000	0.0042
	0.5427	0.5394	-0.0033	0.0042
	0.7037	0.7001	-0.0036	0.0042
	1.0338	1.0323	-0.0015	0.0042
635.0	0.0000	0.0000	0.0000	0.0042
	0.5268	0.5235	-0.0033	0.0042
	0.6720	0.6685	-0.0035	0.0042
	0.9864	0.9847	-0.0017	0.0042

\*CNR = Customer not request

### 4. Stray Light\*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)		
	Wavelength (nm)	Transmission (%T)	Absorbance (A)
200.91 $\pm$ 0.11nm	200.31	0.9399	2.0274

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

\*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

**\*\*\*End of Certificate\*\*\***

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.





## Certificate of Calibration

Represent to Certificate of Calibration ,PTC/07/21161

Certificate No.:	PTC/07/21161	Page:	1 of 2
Equipment:	Digital Balance	Condition:	Normal
Manufacturer:	Sartorius	Serial No:	38304165
Model:	SECURA224-1S	ID No:	BKK_EN0309
Type of Balance:	Single interval		



Customer: ALS Laboratory Group ( Thailand ) Co.,Ltd.  
104 Phatthanakarn 40, Phatthanakarn Rd.,  
Khwaeng Phatthanakarn, Khet Suan Luang, Bangkok 10250.

Environment Condition: Temperature 23.8 °C  $\pm$  0.4 °C  
Humidity 58.1 %RH  $\pm$  0.7 %RH  
Air density 1.18 kg/m<sup>3</sup>

Calibration Place: ALS Laboratory Group ( Thailand ) Co.,Ltd.  
104 Phatthanakarn 40, Phatthanakarn Rd.,  
Khwaeng Phatthanakarn, Khet Suan Luang, Bangkok 10250.



The Method used: In house method, PTC-WI-07, base on Euramet cg. 18

Traceability: This certificate is traceable to the SI Units through Thai Calibration Service Co.,Ltd.  
, NSC-ONSC Accreditation No.: Calibration 0189

Date Received: December 16, 2021

Calibration Date: December 16, 2021

Issued Date: December 20, 2021

Calibration By: Mr. Keattisak Kerdto



PENTA CALIBRATION CO., LTD.

( Mr.Kriangsak Kalasri )

Reviewed by

Approved By :

( Mr. Keattisak Kerdto )

Laboratory Manager

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognised national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The effect that the results relate only to the items calibrated.

This calibration certificate shall not be reproduced except in full only, without written approval from penta calibration co., ltd



Represent to Certificate of Calibration ,PTC/07/21161

Certificate No.: PTC/07/21161



Page: 2 of 2

## Measurement Results:

Without Adjustment :

Function Calibration: Internal Calibration

Eccentric Error: Weight to be 1/3 ,1/2 or of Maximum capacity

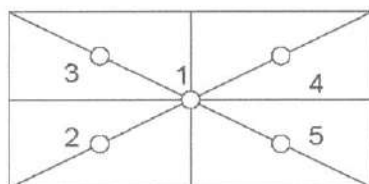

Eccentricity test 100 (g)

Position (g)				
1	2	3	4	5
0.0000	0.0000	0.0000	-0.0001	-0.0001
Maximum deviation:			0.0001	

Repeatability Test : Weight to be  $1/2 \leq L_1 \leq$  Maximum capacity

Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
200	0.00004

Error of indication : from nominal value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Indication (g)	Correction of Balance (g)	Uncertainty (g)	k
0	0.00000	0.0000	0.0000	0.00013	2.37
0.01	0.01000	0.0100	0.0000	0.00028	2.00
0.1	0.10000	0.1000	0.0000	0.00015	2.12
1	1.00000	1.0000	0.0000	0.00014	2.18
2	2.00000	2.0000	0.0000	0.00014	2.20
5	5.00001	5.0000	0.0000	0.00014	2.20
10	10.00000	10.0000	0.0000	0.00014	2.20
20	20.00003	20.0000	0.0000	0.00014	2.18
50	50.00004	50.0000	0.0000	0.00015	2.11
100	100.00004	100.0000	0.0000	0.00018	2.05
200	200.00011	200.0000	0.0001	0.00025	2.00

Note: Weight of adjust - (g)

The End of Certificate



## ROTA METER CALIBRATION RESULT APRIL 2022

Rotameter ID.	Calibration Date	Regression Result	Coefficient (R <sup>2</sup> )
BKK_FS0577	01 Apr 22	$Y = 1.0202x + 0.1976$	1.0000
BKK_FS0579	01 Apr 22	$Y = 1.0078x + 0.4789$	0.9998
BKK_FS0583	01 Apr 22	$Y = 1.016x + 0.3922$	1.0000
BKK_FS0584	01 Apr 22	$Y = 1.0036x + 2.2262$	0.9997
BKK_FS0585	01 Apr 22	$Y = 1.0189x - 5.6476$	0.9997
BKK_FS0586	01 Apr 22	$Y = 1.0095x - 1.1524$	0.9995
BKK_FS0587	01 Apr 22	$Y = 1.013x - 3.6619$	0.9996
BKK_FS0588	01 Apr 22	$Y = 1.0154x + 4.8357$	0.9999
BKK_FS0589	01 Apr 22	$Y = 0.9918x + 4.8069$	0.9999
BKK_FS0590	01 Apr 22	$Y = 1.0038x - 0.4857$	0.9996
BKK_FS0591	01 Apr 22	$Y = 0.9705x - 52.174$	0.9986
BKK_FS0592	01 Apr 22	$Y = 0.9646x - 37.642$	0.9985
BKK_FS0593	01 Apr 22	$Y = 0.9767x - 58.445$	0.9988
BKK_FS0594	01 Apr 22	$Y = 0.9902x - 62.87$	0.9999
BKK_FS0595	01 Apr 22	$Y = 1.0249x - 98.162$	0.9999
BKK_FS0596	01 Apr 22	$Y = 0.9843x - 26.806$	0.9991
BKK_FS0597	01 Apr 22	$Y = 0.9802x - 61.653$	0.9978
BKK_FS1004	01 Apr 22	$Y = 0.9696x + 17.69$	0.9990
BKK_FS1005	01 Apr 22	$Y = 1.0065x + 5.6786$	0.9997
BKK_FS1006	01 Apr 22	$Y = 1.2142x - 7.1037$	0.9993
BKK_FS1007	01 Apr 22	$Y = 0.9917x + 1.6592$	1.0000
BKK_FS1008	01 Apr 22	$Y = 1.0132x + 0.7207$	1.0000
BKK_FS1009	01 Apr 22	$Y = 1.0132x + 1.1633$	0.9960
BKK_FS1010	01 Apr 22	$Y = 1.0033x + 0.5758$	0.9999
BKK_FS1011	01 Apr 22	$Y = 1.0234x + 0.1759$	0.9996
BKK_FS1012	01 Apr 22	$Y = 1.0106x - 2.0048$	0.9997
BKK_FS1013	01 Apr 22	$Y = 0.9677x - 35.851$	0.9997
BKK_FS1014	01 Apr 22	$Y = 1.0021x + 0.3148$	0.9998
BKK_FS1015	01 Apr 22	$Y = 0.9994x + 1.786$	1.0000
BKK_FS1016	01 Apr 22	$Y = 1.0105x - 80.256$	0.9998
BKK_FS1017	01 Apr 22	$Y = 0.9995x + 0.649$	1.0000
BKK_FS1018	01 Apr 22	$Y = 1.0011x + 1.1786$	1.0000
BKK_FS1019	01 Apr 22	$Y = 1.0023x - 68.424$	0.9996
BKK_FS1020	01 Apr 22	$Y = 1.0547x - 0.666$	0.9998
BKK_FS1021	01 Apr 22	$Y = 1.018x - 3.3286$	0.9998
BKK_FS1022	01 Apr 22	$Y = 0.9932x - 57.035$	0.9986
BKK_FS1023	01 Apr 22	$Y = 1.0094x + 0.0717$	0.9999
BKK_FS1024	01 Apr 22	$Y = 1.0042x + 0.4086$	0.9997



## ROTA METER CALIBRATION RESULT APRIL 2022

Rotameter ID.	Calibration Date	Regression Result	Coefficient (R <sup>2</sup> )
BKK_FS1025	01 Apr 22	$Y = 1.0132x - 88.507$	0.9996
BKK_FS1026	01 Apr 22	$Y = 1.0018x + 1.0776$	0.9997
BKK_FS1027	01 Apr 22	$Y = 1.0053x + 0.231$	0.9995
BKK_FS1028	01 Apr 22	$Y = 0.9792x - 60.312$	0.9982
BKK_FS1029	01 Apr 22	$Y = 0.9935x + 0.8234$	1.0000
BKK_FS1030	01 Apr 22	$Y = 1.0039x + 0.515$	0.9999
BKK_FS1031	01 Apr 22	$Y = 1.009x - 79.295$	0.9998
BKK_FS1039	01 Apr 22	$Y = 0.9868x + 7.8119$	0.9993
BKK_FS1040	01 Apr 22	$Y = 1.0096x - 7.2905$	0.9990
BKK_FS1041	01 Apr 22	$Y = 1.076x - 2.0503$	0.9999
BKK_FS1042	01 Apr 22	$Y = 1.0054x + 1.6095$	0.9995
BKK_FS1043	01 Apr 22	$Y = 1.0108x - 11.048$	0.9999
BKK_FS1044	01 Apr 22	$Y = 1.0468x - 0.9391$	0.9997
BKK_FS1161	01 Apr 22	$Y = 1.0126x + 0.7738$	0.9999
BKK_FS1162	01 Apr 22	$Y = 0.9994x + 2.6357$	0.9995
BKK_FS1163	01 Apr 22	$Y = 0.977x - 55.03$	0.9987
BKK_FS1164	01 Apr 22	$Y = 0.9914x + 0.8427$	0.9997
BKK_FS1165	01 Apr 22	$Y = 0.9893x + 6.5919$	0.9998
BKK_FS1166	01 Apr 22	$Y = 1.0031x - 77.881$	0.9996
RYG_FS0197	01 Apr 22	$Y = 1.0055x + 1.1914$	0.9998
RYG_FS0198	01 Apr 22	$Y = 0.996x + 23.788$	0.9996
RYG_FS0199	01 Apr 22	$Y = 1.1166x - 3.3942$	0.9998

Review By :

(Mr. Wichan Choonharat)

Enviro Field Services Manager

Approved By :

(Mr. Sarayuth Jittrantont)

Assistant General Manager



# SITHIPORN ASSOCIATES CO.,LTD.

## CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd., Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : ACC21020

Pages : 1 of 3

### Calibration Certificate

**Equipment :** SOUND CALIBRATOR  
**Manufacturer :** RION  
**Model :** NC-74  
**Serial No.:** 34425567  
**ID No.:** BKK\_FS0618

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 06 OCTOBER 2021  
**Calibration Date :** 18 OCTOBER 2021  
**Date of Issue :** 19 OCTOBER 2021

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	18/10/22

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*[Signature]*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

Cert. No. : ACC21020

Job No. : VC65AC0002

Pages : 2 of 3

Calibration Procedure : CP-AC-03

**Calibration Method :**

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	8846A	1997025	EEL.BP. 06/0264	05-Feb-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22
Audio Analyzer	AVR-3360A	V744B6069	EF-0010-21	10-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



Continuation of Calibration Certificate

Cert. No. : ACC21020  
Job No. : VC65AC0002  
Pages : 3 of 3

**Result of calibration :**

**1. Sound pressure level**

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit (dB)
94	94.1	0.10	0.14	0.40

**2. Frequency**

Specified Frequency (Hz)	Measured value (Hz)	Deviated value ( % )	Uncertainty ( % )	Tolerance limit ( % )
1000	1002.4	0.2	0.1	1.0

**3. Total distortion**

Measured value ( % )	Uncertainty ( % )	Tolerance limit ( % )
1.57	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : ACL21150

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00858513 / 158763 / 58765  
**ID No.:** BKK\_FS0103

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.


**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 08 NOVEMBER 2021  
**Calibration Date :** 09-10 NOVEMBER 2021  
**Date of Issue :** 12 NOVEMBER 2021

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	9/11/22

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

Cert. No. : ACL21150

Job No. : VC65AC0015

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	8846A	1997025	EEL.BP. 06/0264	05-Feb-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



Continuation of Calibration Certificate

Cert. No. : ACL21150  
Job No. : VC65AC0015  
Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

**Cert. No. : ACL21150**  
**Job No. : VC65AC0015**  
**Pages : 4 of 8**

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	93.9	0.0	±0.3

**2. Self-generated noise**

2.1 Normal test

Measured Value ( dB )
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	11.6
C - weight	17.8
Flat	23.6

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.5	0.5	± 1.5
1000	-0.1	-0.1	0.0	± 1.0
8000	-2.6	-2.6	-2.6	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL21150  
Job No. : VC65AC0015  
Pages : 5 of 8

**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

**5. Frequency and time weightings at 1 kHz**

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3



## Continuation of Calibration Certificate

Cert. No. : ACL21150

Job No. : VC65AC0015

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	132.9	-0.1	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	130.9	-0.1	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.1	0.1	± 1.1

## Continuation of Calibration Certificate

Cert. No. : ACL21150

Job No. : VC65AC0015

Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	136.0	-0.4	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

## Continuation of Calibration Certificate

Cert. No. : ACL21150  
Job No. : VC65AC0015  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate



# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : ACL21151

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00858514 / 158764 / 58766  
**ID No.:** BKK\_FS0104

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 08 NOVEMBER 2021  
**Calibration Date :** 09-10 NOVEMBER 2021  
**Date of Issue :** 12 NOVEMBER 2021

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	9/11/22

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

*[Signature]*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

Cert. No. : ACL21151

Job No. : VC65AC0015

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	8846A	1997025	EEL.BP. 06/0264	05-Feb-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



Continuation of Calibration Certificate

Cert. No. : ACL21151  
Job No. : VC65AC0015  
Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1



## Continuation of Calibration Certificate

Cert. No. : ACL21151  
Job No. : VC65AC0015  
Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	93.9	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
13.5

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	9.9
C - weight	16.5
Flat	22.1

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.6	0.7	0.7	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-3.4	-3.4	-3.4	±5.0

Continuation of Calibration Certificate

**Cert. No. : ACL21151**  
**Job No. : VC65AC0015**  
**Pages : 5 of 8**

**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

**5. Frequency and time weightings at 1 kHz**

**5.1 Frequency weightings at 1 kHz**

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

**5.2 Time weighting at 1 kHz**

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

## Continuation of Calibration Certificate

Cert. No. : ACL21151

Job No. : VC65AC0015

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	132.9	-0.1	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	130.9	-0.1	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.1	0.1	± 1.1



## Continuation of Calibration Certificate

 Cert. No. : ACL21151  
 Job No. : VC65AC0015  
 Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	136.0	-0.4	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

Continuation of Calibration Certificate

**Cert. No. : ACL21151**

**Job No. : VC65AC0015**

**Pages : 8 of 8**

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

**12. High level stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

**End of Calibration Certificate**



Certificate No.: 0210SV21  
Operation No.: CP2021050018

## Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: RION

Model/Type: NL-42 (Meter), UC-52 (Microphone), NH-24 (Preamplifier)

Serial No.: 00710637 (Meter), 136954 (Microphone), 10638 (Preamplifier)

ID No.: BKK\_FS0021

Customer: ALS Laboratory Group (Thailand) Co.,Ltd.

Address: 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan  
Khet Suan Luang, Bangkok 10250 Thailand

Received Date: 17 May 2021

Calibrated Date: 19 - 24 May 2021

Issued Date: 25 May 2021

Calibrated by: Ms. Juntaporn Kunhakom

REVIEW BY	<i>Nana Kom P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	19/5/22

Approved by:



สถาบันไฟฟ้าและอิเล็กทรอนิกส์  
ELECTRICAL AND ELECTRONICS INSTITUTE

( Mr. Sittichai Swaksriyawong )  
Group Manager

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor  $k = 2.00$ , providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: 0210SV21

### Calibration Report

Equipment: Sound Level Meter  
Manufacturer: RION  
Model/Type: NL-42 (Meter), UC-52 (Microphone), NH-24 (Preamplifier)  
Serial No.: 00710637 (Meter), 136954 (Microphone), 10638 (Preamplifier)  
ID No.: BKK\_FS0021  
Ambient Temperature: ( 23 ± 2 ) °C  
Relative Humidity: ( 50 ± 15 ) %  
Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-

IEC 61672-3:2013.

#### Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1001-21	12 January 2022
2) Sine generator	1051	1501442	0151RF20	21 September 2021
3) Arbitrary Function Generator	AFG2021	C010063	0099RF20	17 June 2021
4) Programmable Attenuator	PA5	2755	EF-0034-20	10 November 2021
5) 6.5 Digit precision multimeter	8846A	9609027	0498EL20	10 August 2021
6) 6.5 Digit precision multimeter	8846A	9610014	0669EL20	27 October 2021
7) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P200051 0305TE20	31 May 2021 28 June 2021
8) Pressure humidity and Temperature Transmitter	PTU301	F0640003	CL1-P200052 0306TE20	1 June 2021 28 June 2021

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; ONSC Accredited Calibration No.0119

#### Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.0

Note : Absolute sensitivity was established by the use of the Sound Calibrator RION Type NC-74 S/N : 34615278.

Certificate No.: 0210SV21

## Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
16.0

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	11.6
C-weighting	18.1
Z-weighting	23.7

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.3	0.5	0.3	±1.5
1000	0.0	0.0	0.0	±1.0
8000	-1.8	-1.7	-1.7	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	-0.1	-0.1	±2.0
125	0.0	-0.2	-0.1	±1.5
250	0.0	-0.1	0.0	±1.5
500	0.1	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	-0.1	±2.0
4000	0.1	0.0	0.0	±3.0
8000	0.0	-0.1	0.0	±5.0

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2



Certificate No.: 0210SV21

### Calibration Report

#### 5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

#### Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

#### Function : 7. Level Linearity on the reference level range

##### 7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
130.0	130.0	0.0	±1.1
131.0	131.0	0.0	±1.1
132.0	132.0	0.0	±1.1
133.0	133.0	0.0	±1.1
134.0	134.0	0.0	±1.1
135.0	135.0	0.0	±1.1
136.0	136.0	0.0	±1.1
137.0	137.0	0.0	±1.1

##### 7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1

Certificate No.: 0210SV21

### Calibration Report

#### 7.2 Level Linearity on the reference level range, Lower (Cont.)

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.0	0.0	±1.1
39.0	39.0	0.0	±1.1
34.0	33.9	-0.1	±1.1
29.0	28.9	-0.1	±1.1
24.0	24.0	0.0	±1.1

#### Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	126.0	0.0	±1.0
	2	108.9	-0.1	+1.0 ; -2.5
	0.25	99.9	-0.1	+1.5 ; -5.0
Slow	200	119.6	0.0	±1.0
	2	100.0	0.0	+1.0 ; -5.0
LAE	200	120.0	0.0	±1.0
	2	100.0	0.0	+1.0 ; -2.5
	0.25	90.9	-0.1	+1.5 ; -5.0

#### Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	125.4	125.4	0.0	±3.0
Positive half cycle	124.4	124.1	-0.3	±2.0
Negative half cycle	124.4	124.1	-0.3	±2.0

#### Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
139.4	139.4	0.0	±1.5



Certificate No.: 0210SV21

### Calibration Report

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	129.0	129.0	0.0	±0.3

#### Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks: 1. The acceptance limit is for the deviated value.  
2. Acceptance limits was IEC61672-3:2013 Class 2.

-- End of Report --

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL22039

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00572452 / 171618 / 72790  
**ID No.:** BKK\_FS0922

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 05 JANUARY 2022  
**Calibration Date :** 12-14 JANUARY 2022  
**Date of Issue :** 17 JANUARY 2022

REVIEW BY	Narakorn P.
APPROVED BY	[Signature]
NEXT CAL. DATE	12/1/23

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

[Signature]  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL22039

Job No. : VC65AC0041

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

## Continuation of Calibration Certificate

Cert. No. : ACL22039

Job No. : VC65AC0041

Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1



## Continuation of Calibration Certificate

Cert. No. : ACL22039

Job No. : VC65AC0041

Pages : 4 of 8

**Result of calibration :**
**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	93.9	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.0
C - weight	18.8
Flat	24.4

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.2	0.2	0.2	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-0.5	-0.5	-0.4	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22039  
Job No. : VC65AC0041  
Pages : 5 of 8

**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

**5. Frequency and time weightings at 1 kHz**

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3



Continuation of Calibration Certificate

Cert. No. : ACL22039

Job No. : VC65AC0041

Pages : 6 of 8

**7. Level linearity on the reference level range**

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	43.9	-0.1	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.8	-0.2	± 1.1

## Continuation of Calibration Certificate

 Cert. No. : ACL22039  
 Job No. : VC65AC0041  
 Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	135.8	-0.6	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0



Continuation of Calibration Certificate

Cert. No. : ACL22039

Job No. : VC65AC0041

Pages : 8 of 8

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

**12. High level stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

**End of Calibration Certificate**

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : ACL22042

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00858523 / 158774 / 58775  
**ID No.:** BKK\_FS0113

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 05 JANUARY 2022  
**Calibration Date :** 12-14 JANUARY 2022  
**Date of Issue :** 17 JANUARY 2022

REVIEW BY	Narakorn R.
APPROVED BY	[Signature]
NEXT CAL. DATE	12/1/23

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

[Signature]  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL22042

Job No. : VC65AC0041

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22042  
Job No. : VC65AC0041  
Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1



Continuation of Calibration Certificate

**Cert. No. : ACL22042**

**Job No. : VC65AC0041**

**Pages : 4 of 8**

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	93.9	0.0	±0.3

**2. Self-generated noise**

2.1 Normal test

Measured Value ( dB )
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.0
C - weight	18.7
Flat	24.2

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.5	0.5	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-1.3	-1.3	-1.3	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22042  
Job No. : VC65AC0041  
Pages : 5 of 8

**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

**5. Frequency and time weightings at 1 kHz**

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3



## Continuation of Calibration Certificate

Cert. No. : ACL22042

Job No. : VC65AC0041

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	53.9	-0.1	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	38.9	-0.1	$\pm 1.1$
34.0	33.9	-0.1	$\pm 1.1$
30.0	29.9	-0.1	$\pm 1.1$
29.0	28.9	-0.1	$\pm 1.1$
28.0	27.9	-0.1	$\pm 1.1$
27.0	26.9	-0.1	$\pm 1.1$
26.0	25.9	-0.1	$\pm 1.1$
25.0	24.8	-0.2	$\pm 1.1$

## Continuation of Calibration Certificate

Cert. No. : ACL22042

Job No. : VC65AC0041

Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0



Continuation of Calibration Certificate

Cert. No. : ACL22042  
Job No. : VC65AC0041  
Pages : 8 of 8

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.7	89.7	0.0	±1.5

**12. High level stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : ACL21062

Pages : 1 of 9

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-21/ Microphone UC-52 / Preamplifier NH-21  
**Serial No.:** 00710220 / 75619 / 23998  
**ID No.:** BKK\_FS0018

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAEANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 22 JUNE 2021  
**Calibration Date :** 28-30 JUNE 2021  
**Date of Issue :** 05 JUNE 2021

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	28/6/22

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*[Signature]*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

Cert. No. : ACL21062

Job No. : VC64AC0048

Pages : 2 of 9

Calibration Procedure : CP-AC-02

## Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	33461A	MY53220116	EEL.BP. 04/0264	10-Feb-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

**Continuation of Calibration Certificate**

**Cert. No. : ACL21062**

**Job No. : VC64AC0048**

**Pages : 3 of 9**

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1



## Continuation of Calibration Certificate

Cert. No. : ACL21062

Job No. : VC64AC0048

Pages : 4 of 9

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	93.9	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
22.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	21.7
C - weight	22.3
Flat	24.8

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	-0.1	0.0	0.1	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	2.9	3.0	3.0	±5.0

## Continuation of Calibration Certificate

Cert. No. : ACL21062

Job No. : VC64AC0048

Pages : 5 of 9

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.2	-0.1	0.0	±2.0
125	-0.1	0.0	0.0	±1.5
250	-0.1	-0.1	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.1	0.1	0.1	±2.0
4000	0.1	0.1	0.1	±3.0
8000	0.1	0.2	0.2	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

## Continuation of Calibration Certificate

Cert. No. : ACL21062

Job No. : VC64AC0048

Pages : 6 of 9

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	38.9	-0.1	$\pm 1.1$

## Continuation of Calibration Certificate

Cert. No. : ACL21062

Job No. : VC64AC0048

Pages : 7 of 9

## 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
130	94.0	94.0	0.0	±0.5
120	94.0	94.0	0.0	±0.5
110	94.0	94.0	0.0	±0.5
100	94.0	94.0	0.0	±0.5
90	94.0	94.0	0.0	±0.5

## Level linearity on each level range

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
130	43.0	43.0	0.0	±0.5
120	33.0	33.0	0.0	±0.5

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0



Continuation of Calibration Certificate

Cert. No. : ACL21062

Job No. : VC64AC0048

Pages : 8 of 9

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.00	0.0	-
One	136.4	136.00	-0.4	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.3	-0.2	±1.5

## Continuation of Calibration Certificate

Cert. No. : ACL21062

Job No. : VC64AC0048

Pages : 9 of 9

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

\_\_\_\_\_ End of Calibration Certificate \_\_\_\_\_

Certificate No.: 0210SV21  
Operation No.: CP2021050018

## Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: RION

Model/Type: NL-42 (Meter), UC-52 (Microphone), NH-24 (Preamplifier)

Serial No.: 00710637 (Meter), 136954 (Microphone), 10638 (Preamplifier)

ID No.: BKK\_FS0021

Customer: ALS Laboratory Group (Thailand) Co.,Ltd.

Address: 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan  
Khet Suan Luang, Bangkok 10250 Thailand

Received Date: 17 May 2021

Calibrated Date: 19 - 24 May 2021

Issued Date: 25 May 2021

Calibrated by: Ms. Juntaporn Kunhakom

REVIEW BY	<i>Nana Kom P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	19/5/22

Approved by:



สถาบันไฟฟ้าและอิเล็กทรอนิกส์  
ELECTRICAL AND ELECTRONICS INSTITUTE

( Mr. Sittichai Swaksriyawong )  
Group Manager

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor  $k = 2.00$ , providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: 0210SV21

### Calibration Report

Equipment: Sound Level Meter  
Manufacturer: RION  
Model/Type: NL-42 (Meter), UC-52 (Microphone), NH-24 (Preamplifier)  
Serial No.: 00710637 (Meter), 136954 (Microphone), 10638 (Preamplifier)  
ID No.: BKK\_FS0021  
Ambient Temperature: ( 23 ± 2 ) °C  
Relative Humidity: ( 50 ± 15 ) %  
Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-

IEC 61672-3:2013.

#### Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1001-21	12 January 2022
2) Sine generator	1051	1501442	0151RF20	21 September 2021
3) Arbitrary Function Generator	AFG2021	C010063	0099RF20	17 June 2021
4) Programmable Attenuator	PA5	2755	EF-0034-20	10 November 2021
5) 6.5 Digit precision multimeter	8846A	9609027	0498EL20	10 August 2021
6) 6.5 Digit precision multimeter	8846A	9610014	0669EL20	27 October 2021
7) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P200051 0305TE20	31 May 2021 28 June 2021
8) Pressure humidity and Temperature Transmitter	PTU301	F0640003	CL1-P200052 0306TE20	1 June 2021 28 June 2021

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; ONSC Accredited Calibration No.0119

#### Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.0

Note : Absolute sensitivity was established by the use of the Sound Calibrator RION Type NC-74 S/N : 34615278.



Certificate No.: 0210SV21

## Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
16.0

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	11.6
C-weighting	18.1
Z-weighting	23.7

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.3	0.5	0.3	±1.5
1000	0.0	0.0	0.0	±1.0
8000	-1.8	-1.7	-1.7	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	-0.1	-0.1	±2.0
125	0.0	-0.2	-0.1	±1.5
250	0.0	-0.1	0.0	±1.5
500	0.1	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	-0.1	±2.0
4000	0.1	0.0	0.0	±3.0
8000	0.0	-0.1	0.0	±5.0

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

Certificate No.: 0210SV21

## Calibration Report

### 5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

### Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

### Function : 7. Level Linearity on the reference level range

#### 7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
130.0	130.0	0.0	±1.1
131.0	131.0	0.0	±1.1
132.0	132.0	0.0	±1.1
133.0	133.0	0.0	±1.1
134.0	134.0	0.0	±1.1
135.0	135.0	0.0	±1.1
136.0	136.0	0.0	±1.1
137.0	137.0	0.0	±1.1

#### 7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1

Certificate No.: 0210SV21

### Calibration Report

#### 7.2 Level Linearity on the reference level range, Lower (Cont.)

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.0	0.0	±1.1
39.0	39.0	0.0	±1.1
34.0	33.9	-0.1	±1.1
29.0	28.9	-0.1	±1.1
24.0	24.0	0.0	±1.1

#### Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	126.0	0.0	±1.0
	2	108.9	-0.1	+1.0 ; -2.5
	0.25	99.9	-0.1	+1.5 ; -5.0
Slow	200	119.6	0.0	±1.0
	2	100.0	0.0	+1.0 ; -5.0
LAE	200	120.0	0.0	±1.0
	2	100.0	0.0	+1.0 ; -2.5
	0.25	90.9	-0.1	+1.5 ; -5.0

#### Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	125.4	125.4	0.0	±3.0
Positive half cycle	124.4	124.1	-0.3	±2.0
Negative half cycle	124.4	124.1	-0.3	±2.0

#### Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
139.4	139.4	0.0	±1.5



Certificate No.: 0210SV21

### Calibration Report

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	129.0	129.0	0.0	±0.3

#### Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks: 1. The acceptance limit is for the deviated value.  
2. Acceptance limits was IEC61672-3:2013 Class 2.

-- End of Report --



# SITHIPHORN ASSOCIATES CO.,LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACC21012

Pages : 1 of 3

### Calibration Certificate

**Equipment :** SOUND CALIBRATOR  
**Manufacturer :** RION  
**Model :** NC-74  
**Serial No.:** 34425566  
**ID No.:** BBK\_FS0617

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 05 AUGUST 2021  
**Calibration Date :** 09 AUGUST 2021  
**Date of Issue :** 11 AUGUST 2021

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	<i>9/8/21</i>

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*T. Petchurai*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

Cert. No. : ACC21012

Job No. : VC64AC0060

Pages : 2 of 3

Calibration Procedure : CP-AC-03

**Calibration Method :**

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	8846A	1997025	EEL.BP. 06/0264	05-Feb-22
Digital Multimeter	33461A	MY53220116	EEL.BP. 04/0264	10-Feb-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22
Audio Analyzer	AVR-3360A	V744B6069	EF-0010-21	10-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

## Continuation of Calibration Certificate

Cert. No. : ACC21012

Job No. : VC64AC0060

Pages : 3 of 3

**Result of calibration :****1. Sound pressure level**

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit (dB)
94	94.1	0.10	0.22	0.40

**2. Frequency**

Specified Frequency (Hz)	Measured value (Hz)	Deviated value ( % )	Uncertainty ( % )	Tolerance limit ( % )
1000	1001.9	0.2	0.1	1.0

**3. Total distortion**

Measured value ( % )	Uncertainty ( % )	Tolerance limit ( % )
1.14	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————



# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL21083

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00597159 / 180402 / 88172  
**ID No.:** BKK\_FS0995

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 05 AUGUST 2021  
**Calibration Date :** 06 -10 AUGUST 2021  
**Date of Issue :** 11 AUGUST 2021

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	6/8/22

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*T. Petchurai*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL21083

Job No. : VC64AC0060

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	8846A	1997025	EEL.BP. 06/0264	05-Feb-22
Digital Multimeter	33461A	MY53220116	EEL.BP. 04/0264	10-Feb-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

## Continuation of Calibration Certificate

Cert. No. : ACL21083

Job No. : VC64AC0060

Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

## Continuation of Calibration Certificate

Cert. No. : ACL21083  
Job No. : VC64AC0060  
Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	93.9	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
15.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.0
C - weight	18.1
Flat	23.9

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.3	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.7	0.8	0.8	±5.0

## Continuation of Calibration Certificate

Cert. No. : ACL21083

Job No. : VC64AC0060

Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3



Continuation of Calibration Certificate

Cert. No. : ACL21083

Job No. : VC64AC0060

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	29.0	0.0	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL21083  
Job No. : VC64AC0060  
Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

## Continuation of Calibration Certificate

Cert. No. : ACL21083

Job No. : VC64AC0060

Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.1	-0.1	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate



# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL21082

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00597156 / 180399 / 88169  
**ID No.:** BKK\_FS0994

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 05 AUGUST 2021  
**Calibration Date :** 06 -10 AUGUST 2021  
**Date of Issue :** 11 AUGUST 2021

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	6/8/22

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*[Signature]*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL21082

Job No. : VC64AC0060

Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	8846A	1997025	EEL.BP. 06/0264	05-Feb-22
Digital Multimeter	33461A	MY53220116	EEL.BP. 04/0264	10-Feb-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

## Continuation of Calibration Certificate

Cert. No. : ACL21082

Job No. : VC64AC0060

Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

## Continuation of Calibration Certificate

Cert. No. : ACL21082

Job No. : VC64AC0060

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	93.9	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
16.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	11.6
C - weight	17.8
Flat	23.6

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.4	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.5	0.5	0.5	±5.0

**Continuation of Calibration Certificate**

**Cert. No. : ACL21082**

**Job No. : VC64AC0060**

**Pages : 5 of 8**

**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±2.0
125	0.0	0.0	-0.1	±1.5
250	0.0	-0.1	-0.1	±1.5
500	0.1	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.1	0.0	0.0	±2.0
4000	0.1	0.0	0.0	±3.0
8000	0.1	0.0	0.0	±5.0

**5. Frequency and time weightings at 1 kHz**

**5.1 Frequency weightings at 1 kHz**

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	93.9	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	93.9	0.0	± 0.2

**5.2 Time weighting at 1 kHz**

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	93.9	0.0	-
Slow	93.9	0.0	± 0.1
Leq	93.9	0.0	± 0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.1	0.1	± 0.3



## Continuation of Calibration Certificate

Cert. No. : ACL21082

Job No. : VC64AC0060

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.1	0.1	$\pm 1.1$
135.0	135.1	0.1	$\pm 1.1$
134.0	134.1	0.1	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.1	0.1	$\pm 1.1$
114.0	114.1	0.1	$\pm 1.1$
109.0	109.1	0.1	$\pm 1.1$
104.0	104.1	0.1	$\pm 1.1$
99.0	99.1	0.1	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	29.9	-0.1	$\pm 1.1$
29.0	28.9	-0.1	$\pm 1.1$
28.0	27.9	-0.1	$\pm 1.1$
27.0	27.0	0.0	$\pm 1.1$
26.0	26.0	0.0	$\pm 1.1$
25.0	24.9	-0.1	$\pm 1.1$

## Continuation of Calibration Certificate

Cert. No. : ACL21082

Job No. : VC64AC0060

Pages : 7 of 8

## 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	107.9	-0.1	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

## 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	136.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

**Continuation of Calibration Certificate**

**Cert. No. : ACL21082**

**Job No. : VC64AC0060**

**Pages : 8 of 8**

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

**12. High level stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

**End of Calibration Certificate**

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL22040

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00597162 / 180405 / 88175  
**ID No.:** BKK\_FS0997

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 05 JANUARY 2022  
**Calibration Date :** 12-14 JANUARY 2022  
**Date of Issue :** 17 JANUARY 2022

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	12/1/23

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*T. Petchurai*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL22040

Job No. : VC65AC0041

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

## Continuation of Calibration Certificate

 Cert. No. : ACL22040  
 Job No. : VC65AC0041  
 Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1



## Continuation of Calibration Certificate

Cert. No. : ACL22040

Job No. : VC65AC0041

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	93.9	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
16.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	13.6
C - weight	20.2
Flat	25.7

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.1	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.3	0.4	0.4	±5.0

## Continuation of Calibration Certificate

Cert. No. : ACL22040

Job No. : VC65AC0041

Pages : 5 of 8

**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

**5. Frequency and time weightings at 1 kHz**
**5.1 Frequency weightings at 1 kHz**

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

**5.2 Time weighting at 1 kHz**

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3



Continuation of Calibration Certificate

Cert. No. : ACL22040

Job No. : VC65AC0041

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	29.0	0.0	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

## Continuation of Calibration Certificate

 Cert. No. : ACL22040  
 Job No. : VC65AC0041  
 Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>cpeak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0



Continuation of Calibration Certificate

Cert. No. : ACL22040

Job No. : VC65AC0041

Pages : 8 of 8

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

**12. High level stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : ACL22038

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00296514 / 179116 / 87523  
**ID No.:** BKK\_FS0971

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 05 JANUARY 2022  
**Calibration Date :** 12-14 JANUARY 2022  
**Date of Issue :** 17 JANUARY 2022

REVIEW BY	<i>Worakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	12/1/23

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*[Signature]*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL22038

Job No. : VC65AC0041

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22038  
Job No. : VC65AC0041  
Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1



Continuation of Calibration Certificate

**Cert. No. :** ACL22038

**Job No. :** VC65AC0041

**Pages :** 4 of 8

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	93.9	0.0	±0.3

**2. Self-generated noise**

2.1 Normal test

Measured Value ( dB )
14.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.0
C - weight	13.7
Flat	24.2

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.5	0.5	-4.5	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-1.1	-1.0	-1.0	±5.0

## Continuation of Calibration Certificate

Cert. No. : ACL22038

Job No. : VC65AC0041

Pages : 5 of 8

**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

**5. Frequency and time weightings at 1 kHz**

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3



## Continuation of Calibration Certificate

Cert. No. : ACL22038

Job No. : VC65AC0041

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

## Continuation of Calibration Certificate

Cert. No. : ACL22038

Job No. : VC65AC0041

Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	135.9	-0.5	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0



Continuation of Calibration Certificate

Cert. No. : ACL22038  
Job No. : VC65AC0041  
Pages : 8 of 8

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.7	0.1	±1.5

**12. High level stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

**End of Calibration Certificate**

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL22036

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00296512 / 179113 / 87521  
**ID No.:** BKK\_FS0969

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 05 JANUARY 2022  
**Calibration Date :** 12-14 JANUARY 2022  
**Date of Issue :** 17 JANUARY 2022

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	12/1/23

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*[Signature]*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL22036  
Job No. : VC65AC0041  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

## Continuation of Calibration Certificate

Cert. No. : ACL22036

Job No. : VC65AC0041

Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1



## Continuation of Calibration Certificate

Cert. No. : ACL22036

Job No. : VC65AC0041

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	93.9	0.0	±0.3

**2. Self-generated noise****2.1 Normal test**

Measured Value ( dB )
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	13.1
C - weight	19.1
Flat	24.6

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.2	0.2	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-0.3	-0.1	-0.1	±5.0

## Continuation of Calibration Certificate

Cert. No. : ACL22036

Job No. : VC65AC0041

Pages : 5 of 8

**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

**5. Frequency and time weightings at 1 kHz**
**5.1 Frequency weightings at 1 kHz**

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

**5.2 Time weighting at 1 kHz**

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3



Continuation of Calibration Certificate

Cert. No. : ACL22036  
Job No. : VC65AC0041  
Pages : 6 of 8

**7. Level linearity on the reference level range**

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	26.0	0.0	± 1.1
25.0	24.9	-0.1	± 1.1

## Continuation of Calibration Certificate

Cert. No. : ACL22036  
 Job No. : VC65AC0041  
 Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	136.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0



## Continuation of Calibration Certificate

Cert. No. : ACL22036

Job No. : VC65AC0041

Pages : 8 of 8

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

**12. High level stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : ACL21124

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00597155 / 180398 / 88168  
**ID No.:** BKK\_FS0993

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 29 SEPTEMBER 2021  
**Calibration Date :** 12-14 OCTOBER 2021  
**Date of Issue :** 15 OCTOBER 2021

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	12/10/22

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*[Signature]*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL21124  
Job No. : VC64AC0071  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	8846A	1997025	EEL.BP. 06/0264	05-Feb-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

**Continuation of Calibration Certificate**

**Cert. No. : ACL21124**  
**Job No. : VC64AC0071**  
**Pages : 3 of 8**

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL21124  
Job No. : VC64AC0071  
Pages : 4 of 8

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.96)	93.9	0.0	±0.3

**2. Self-generated noise**

2.1 Normal test

Measured Value ( dB )
15.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	11.6
C - weight	17.7
Flat	23.3

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.4	1.5	1.5	±5.0



Continuation of Calibration Certificate

Cert. No. : ACL21124  
Job No. : VC64AC0071  
Pages : 5 of 8

**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.1	0.0	0.0	±1.5
500	0.1	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.1	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

**5. Frequency and time weightings at 1 kHz**

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.1	0.1	± 0.3



## Continuation of Calibration Certificate

Cert. No. : ACL21124

Job No. : VC64AC0071

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.1	0.1	± 1.1

**Continuation of Calibration Certificate**
**Cert. No. : ACL21124**
**Job No. : VC64AC0071**
**Pages : 7 of 8**
**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.5 ; -5.0
	200	800	127.6	127.5	-0.1	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	107.9	-0.1	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	136.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL21124  
Job No. : VC64AC0071  
Pages : 8 of 8

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.7	89.6	-0.1	±1.5

**12. High level stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate



## CERTIFICATE OF CALIBRATION

Certificate No. : CL-013-65  
Page 1 of 2

Equipment Name: Heat Stress Monitor with Sensor  
Manufacturer.: DeltaOHM  
Model: HD32.2  
Serial No: 13032239  
ID No: BKK\_FS0648

### Customer

Name: ALS laboratory group (thailand) Co.,Ltd.  
Address: 104 Phatthanakan 40, Phatthanakan  
Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok  
10250 Thailand.

Received date: 10 JAN 2022  
Calibration date: 14 FEB 2022  
Issue date: 17 FEB 2022

### Reference Used During Calibration

1.Standard Temperature Probe Model: STS-100 A500,  
Serial No.: 667682-09, Due date: 25 Mar 2022  
2.Digital Temperature Indicator Model: DTI-1000-A MK  
II, Serial No.: 671407-00591 Due date: 04 June 2022

### Calibration Condition

Temperature: (23±3)°C  
Relative Humidity: (55±15)%

### Calibration Procedure

The temperature calibration was done by In-House  
calibration method as WI-CL-001 according to  
comparison method with standard digital temperature  
indicator and standard temperature probe. The  
temperature scale use was based on ITS-90.


### Traceability

The measurement results are traceable to the  
international system of units (SI) through National  
Institute of Metrology Thailand (NIMT) Certificate  
number: TT-0036-21, Certificate number: ER-0032-  
21

REVIEW BY	<i>Parinya P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	14/2/23

### Calibrated by

- ☐ Mr. Sorawit Thachalad  
☒ Miss Orathai Wiwatwittaya

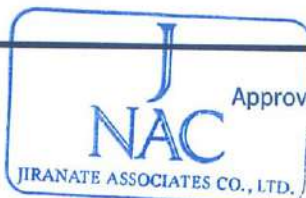

Approved Signatory: .....

*[Signature]*  
Mr. Parinya Booncharoen  
Calibration Department Manager



**Result of Calibration:** ☒ Without Adjustment ☐ With Adjustment

**Calibration Range:** 20 – 40 °C

**Function:**

**Table 1:** This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 13035040.  
Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.054	20.0	-0.1	0.099
30	25.035	25.0	0.0	0.099
30	30.024	30.0	0.0	0.099
30	35.026	35.0	0.0	0.099
30	40.002	40.0	0.0	0.099

**Table 2:** This equipment was connected with temperature probe Model: TP3207.2 S/N: 13033295.  
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.051	20.0	-0.1	0.099
70	24.990	24.9	-0.1	0.099
70	29.917	29.7	-0.2	0.099
70	34.873	34.6	-0.3	0.099
70	39.864	39.5	-0.4	0.099

**Table 3:** This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 13042462.  
Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.053	20.0	-0.1	0.099
110	25.032	24.9	-0.1	0.099
110	30.019	29.9	-0.1	0.099
110	35.023	34.9	-0.1	0.099
110	40.009	39.9	-0.1	0.099

UUC\* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

\* End of Certificate \*



## CERTIFICATE OF CALIBRATION

Certificate No.: CL-052-65  
Page 1 of 2

Equipment Name: Digital thermometer with RTD  
Manufacturer.: DeltaOHM  
Model: HD32.2  
Serial No: 13032240  
ID No: BKK\_FS0649

### Customer

Name: ALS laboratory group (thailand) Co.,Ltd.  
Address: 104 Phatthanakan 40, Phatthanakan  
Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok  
10250 Thailand.

Received date: 15 MAR 2022  
Calibration date: 17 MAR 2022  
Issue date: 18 MAR 2022

### Reference Used During Calibration

1.Standard Temperature Probe Model: STS-100 A500,  
Serial No.: 667682-09, Due date: 25 Mar 2022  
2.Digital Temperature Indicator Model: DTI-1000-A MK  
II, Serial No.: 671407-00591 Due date: 04 June 2022

### Calibration Condition

Temperature: (23±3)°C  
Relative Humidity: (55±15)%

### Calibration Procedure

The temperature calibration was done by In-House  
calibration method as WI-CL-001 according to  
comparison method with standard digital temperature  
indicator and standard temperature probe. The  
temperature scale use was based on ITS-90.

### Traceability

The measurement results are traceable to the  
international system of units (SI) through National  
Institute of Metrology Thailand (NIMT) Certificate  
number: TT-0036-21, Certificate number: ER-0032-  
21

REVIEW BY	<i>Narakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	17/3/23

### Calibrated by

- ☐ Mr. Sorawit Thachalad  
☒ Miss Orathai Wiwatwittaya



Approved Signatory: .....

*[Signature]*  
Mr. Parinya Booncharoen  
Calibration Department Manager

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 - 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 13035023.  
Dimension: Diameter 14 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
30	20.082	20.1	0.0	0.099
30	25.075	25.1	0.0	0.099
30	30.068	30.1	0.0	0.099
30	35.064	35.1	0.0	0.099
30	40.056	40.1	0.0	0.099

Table 2: This equipment was connected with temperature probe Model: TP3207.2 S/N: 13044776.  
Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
70	20.082	20.2	0.1	0.099
70	25.076	25.0	-0.1	0.099
70	30.068	29.9	-0.3	0.099
70	35.062	34.8	-0.6	0.099
70	40.031	39.7	-0.3	0.099

Table 3: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 17023215.  
Dimension: Diameter 8 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.082	20.0	-0.1	0.099
110	25.075	25.0	-0.1	0.099
110	30.068	30.0	-0.1	0.099
110	35.064	35.0	-0.1	0.099
110	40.056	40.0	-0.1	0.099

UUC\* ; Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

\* End of Certificate \*





## CERTIFICATE OF CALIBRATION

Certificate No. : CL-085-65  
Page 1 of 2

**Equipment Name:** Heat Stress Monitor  
**Manufacturer.:** DeltaOHM  
**Model:** HD32.2  
**Serial No:** 13024790  
**ID No:** BKK\_FS0650

### Customer

**Name:** ALS laboratory group (thailand) Co.,Ltd.  
**Address:** 104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok 10250 Thailand.

**Received date:** 25 May 2022  
**Calibration date:** 01 Jun 2022  
**Issue date:** 02 Jun 2022

### Reference Used During Calibration

- 1.Standard Temperature Probe Model: STS-100 A500, Serial No.: 667682-09, Due date: 23 Mar 2023
- 2.Digital Temperature Indicator Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 04 June 2022

### Calibration Condition

Temperature:  $(23 \pm 3)^{\circ}\text{C}$   
Relative Humidity:  $(55 \pm 15)\%$

### Calibration Procedure

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

### Traceability

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0034-22, Certificate number: ER-0032-21

REVIEW BY	<i>Parinya P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	1/6/23

### Calibrated by

- ☐ Mr. Sorawit Thachalad  
☒ Miss Jittrapor Lertsomphol



### Approved Signatory:

*[Signature]*  
Mr. Parinya Booncharoen  
Calibration Department Manager

Certificate No. : CL-085-65  
Page 2 of 2

**Result of Calibration:** ☒ Without Adjustment ☐ With Adjustment

**Calibration Range:** 20 – 40 °C

**Function:**

**Table 1:** This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 13030290.  
Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.053	20.0	-0.1	0.099
30	25.046	25.1	0.1	0.099
30	30.036	30.0	0.0	0.099
30	35.031	35.0	0.0	0.099
30	40.015	40.0	0.0	0.099

**Table 2:** This equipment was connected with temperature probe Model: TP3207.2 S/N: 12038136.  
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.053	20.1	0.0	0.099
70	25.046	25.0	0.0	0.099
70	30.036	29.9	-0.1	0.099
70	35.031	34.7	-0.3	0.099
70	40.014	39.6	-0.4	0.099

**Table 3:** This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 20032622.  
Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.053	20.0	-0.1	0.099
110	25.046	25.0	0.0	0.099
110	30.036	29.9	-0.1	0.099
110	35.036	34.9	-0.1	0.099
110	40.015	39.9	-0.1	0.099

**UUC\* :** Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

**\* End of Certificate \***

## CERTIFICATE OF CALIBRATION

Certificate No. : CL-086-65

Page 1 of 2

**Equipment Name:** Heat Stress Monitor

**Manufacturer.:** DeltaOHM

**Model:** HD32.2

**Serial No:** 13032503

**ID No:** BKK\_FS0651

### Customer

**Name:** ALS laboratory group (thailand) Co.,Ltd.

**Address:** 104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok 10250 Thailand.

**Received date:** 25 May 2022

**Calibration date:** 01 Jun 2022

**Issue date:** 02 Jun 2022

### Reference Used During Calibration

1.Standard Temperature Probe Model: STS-100 A500,  
Serial No.: 667682-09, Due date: 23 Mar 2023

2.Digital Temperature Indicator Model: DTI-1000-A MK II,  
Serial No.: 671407-00591 Due date: 04 June 2022

### Calibration Condition

Temperature:  $(23 \pm 3)^{\circ}\text{C}$

Relative Humidity:  $(55 \pm 15)\%$

### Calibration Procedure

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

### Traceability

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0034-22, Certificate number: ER-0032-21

REVIEW BY	<i>Maraphorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	1/6/23

### Calibrated by

☐ Mr. Sorawit Thachalad

☒ Miss Jittraporn Lertsomphol

### Approved Signatory:

*[Signature]*  
Mr. Parinya Booncharoen  
Calibration Department Manager





**Result of Calibration:** ☒ Without Adjustment ☐ With Adjustment

**Calibration Range:** 20 – 40 °C

**Function:**

**Table 1:** This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 16008223.  
Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.053	20.0	-0.1	0.099
30	25.046	25.0	0.0	0.099
30	30.035	30.0	0.0	0.099
30	35.026	35.0	0.0	0.099
30	40.014	40.0	0.0	0.099

**Table 2:** This equipment was connected with temperature probe Model: TP3207.2 S/N: 16010553.  
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.053	20.2	0.1	0.099
70	25.046	25.0	0.0	0.099
70	30.035	29.8	-0.2	0.099
70	35.026	34.6	-0.4	0.099
70	40.013	39.5	-0.5	0.099

**Table 3:** This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 16008189.  
Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.053	20.1	0.0	0.099
110	25.046	25.0	0.0	0.099
110	30.035	30.0	0.0	0.099
110	35.027	35.0	0.0	0.099
110	40.013	40.0	0.0	0.099

**UUC\*** : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

**\* End of Certificate \***

## CERTIFICATE OF CALIBRATION

Certificate No. : CL-081-65  
Page 1 of 2

**Equipment Name:** Heat Stress Monitor  
**Manufacturer.:** DeltaOHM  
**Model:** HD32.2  
**Serial No:** 15006301  
**ID No:** BKK\_FS0662

### Customer

**Name:** ALS laboratory group (thailand) Co.,Ltd.  
**Address:** 104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok 10250 Thailand.

**Received date:** 25 May 2022  
**Calibration date:** 27 May 2022  
**Issue date:** 02 Jun 2022

### Reference Used During Calibration

1.Standard Temperature Probe Model: STS-100 A500,  
Serial No.: 667682-09, Due date: 23 Mar 2023  
2.Digital Temperature Indicator Model: DTI-1000-A MK II,  
Serial No.: 671407-00591 Due date: 04 June 2022

### Calibration Condition

Temperature:  $(23 \pm 3)^{\circ}\text{C}$   
Relative Humidity:  $(55 \pm 15)\%$

### Calibration Procedure

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

### Traceability

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0034-22, Certificate number: ER-0032-21

REVIEW BY	<i>Parinya Booncharoen</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	27/5/2023

### Calibrated by

- ☐ Mr. Sorawit Thachalad  
☒ Miss Jitraporn Lertsomphol



### Approved Signatory:

*[Signature]*  
Mr. Parinya Booncharoen  
Calibration Department Manager

Certificate No. : CL-081-65

Page 2 of 2

**Result of Calibration:** ☒ Without Adjustment ☐ With Adjustment

**Calibration Range:** 20 – 40 °C

**Function:**

**Table 1:** This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 14039058.  
Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.041	20.0	0.0	0.099
30	25.051	25.0	-0.1	0.099
30	30.042	30.0	0.0	0.099
30	35.034	35.0	0.0	0.099
30	40.026	40.0	0.0	0.099

**Table 2:** This equipment was connected with temperature probe Model: TP3207.2 S/N: 15008013.  
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.041	20.2	0.2	0.099
70	25.051	25.0	-0.1	0.099
70	30.042	29.8	-0.2	0.099
70	35.034	34.7	-0.3	0.099
70	40.026	39.6	-0.4	0.099

**Table 3:** This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 14039052.  
Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.041	20.0	0.0	0.099
110	25.051	25.0	-0.1	0.099
110	30.042	30.0	0.0	0.099
110	35.034	35.0	0.0	0.099
110	40.026	40.0	0.0	0.099

**UUC\* :** Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

**\* End of Certificate \***



## CERTIFICATE OF CALIBRATION

Certificate No. : CL-014-65

Page 1 of 2

Equipment Name: Heat Stress Monitor with Sensor  
Manufacturer.: DeltaOHM  
Model: HD32.2  
Serial No: 15006309  
ID No: BKK\_FS0667

### Customer

Name: ALS laboratory group (thailand) Co.,Ltd.  
Address: 104 Phatthanakan 40, Phatthanakan  
Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok  
10250 Thailand.

Received date: 10 JAN 2022

Calibration date: 14 FEB 2022

Issue date: 17 FEB 2022

### Reference Used During Calibration

1. Standard Temperature Probe Model: STS-100 A500,  
Serial No.: 667682-09, Due date: 25 Mar 2022
2. Digital Temperature Indicator Model: DTI-1000-A MK  
II, Serial No.: 671407-00591 Due date: 04 June 2022

### Calibration Condition

Temperature:  $(23 \pm 3)^{\circ}\text{C}$

Relative Humidity:  $(55 \pm 15)\%$

### Calibration Procedure

The temperature calibration was done by In-House  
calibration method as WI-CL-001 according to  
comparison method with standard digital temperature  
indicator and standard temperature probe. The  
temperature scale use was based on ITS-90.

### Traceability

The measurement results are traceable to the  
international system of units (SI) through National  
Institute of Metrology Thailand (NIMT) Certificate  
number: TT-0036-21, Certificate number: ER-0032-  
21

REVIEW BY

*Parinya P.*

APPROVED BY

*[Signature]*

NEXT CAL. DATE

14/2/23

### Calibrated by

- ☐ Mr. Sorawit Thachalad  
☒ Miss Orathai Wiwatwittaya

**J**  
**NAC**

JIRANATE ASSOCIATES CO., LTD.

Approved Signatory: .....

*[Signature]*

Mr. Parinya Booncharoen  
Calibration Department Manager

**Result of Calibration:** ☒ Without Adjustment ☐ With Adjustment

**Calibration Range:** 20 – 40 °C

**Function:**

**Table 1:** This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 15017683.  
Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.056	20.2	0.1	0.099
30	25.046	25.2	0.2	0.099
30	30.036	30.2	0.2	0.099
30	35.032	35.2	0.2	0.099
30	40.027	40.2	0.2	0.099

**Table 2:** This equipment was connected with temperature probe Model: TP3207.2 S/N: 15015506.  
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.050	20.1	0.1	0.099
70	24.970	24.9	-0.1	0.099
70	29.932	29.8	-0.1	0.099
70	34.876	34.6	-0.3	0.099
70	39.805	39.5	-0.3	0.099

**Table 3:** This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 15009822.  
Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.055	20.0	-0.1	0.099
110	25.045	25.0	0.0	0.099
110	30.037	30.0	0.0	0.099
110	35.033	35.0	0.0	0.099
110	40.027	40.0	0.0	0.099

UUC\* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

\* End of Certificate \*



## CERTIFICATE OF CALIBRATION

Certificate No.: CL-053-65  
Page 1 of 2

Equipment Name: Digital thermometer with RTD  
Manufacturer.: DeltaOHM  
Model: HD32.2  
Serial No: 15006710  
ID No: BKK\_FS0672

Customer  
Name: ALS laboratory group (thailand) Co.,Ltd.  
Address: 104 Phatthanakan 40, Phatthanakan  
Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok  
10250 Thailand.

Received date: 15 MAR 2022  
Calibration date: 17 MAR 2022  
Issue date: 18 MAR 2022

### Reference Used During Calibration

1. Standard Temperature Probe Model: STS-100 A500,  
Serial No.: 667682-09, Due date: 25 Mar 2022  
2. Digital Temperature Indicator Model: DTI-1000-A MK  
II, Serial No.: 671407-00591 Due date: 04 June 2022

### Calibration Condition

Temperature:  $(23 \pm 3)^{\circ}\text{C}$   
Relative Humidity:  $(55 \pm 15)\%$

### Calibration Procedure

The temperature calibration was done by In-House  
calibration method as WI-CL-001 according to  
comparison method with standard digital temperature  
indicator and standard temperature probe. The  
temperature scale use was based on ITS-90.

### Traceability

The measurement results are traceable to the  
international system of units (SI) through National  
Institute of Metrology Thailand (NIMT) Certificate  
number: TT-0036-21, Certificate number: ER-0032-  
21

REVIEW BY	<i>Norakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	17/3/23

### Calibrated by

- ☐ Mr. Sorawit Thachalad  
☒ Miss Orathai Wiwatwittaya



Approved Signatory: .....

*[Signature]*  
Mr. Parinya Booncharoen  
Calibration Department Manager



**Result of Calibration:** ☒ Without Adjustment ☐ With Adjustment

**Calibration Range:** 20 – 40 °C

**Function:**

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 15015852  
Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.082	20.0	-0.1	0.099
30	25.077	25.1	0.0	0.099
30	30.069	30.0	-0.1	0.099
30	35.064	35.0	-0.1	0.099
30	40.056	40.0	-0.1	0.099

Table 2: This equipment was connected with temperature probe Model: TP3207.2 S/N: 14036714.  
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.082	20.2	0.1	0.099
70	25.076	25.0	-0.1	0.099
70	30.068	29.9	-0.4	0.099
70	35.062	34.4	-0.7	0.099
70	40.036	39.6	-0.4	0.099

Table 3: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 15021832.  
Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.082	20.1	0.0	0.099
110	25.077	25.1	0.0	0.099
110	30.069	30.1	0.0	0.099
110	35.064	35.1	0.0	0.099
110	40.056	40.1	0.0	0.099

UUC\* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

\* End of Certificate \*



## CERTIFICATE OF CALIBRATION

Certificate No. : CL-018-65  
Page 1 of 2

Equipment Name: Heat Stress Monitor with Sensor  
Manufacturer.: DeltaOHM  
Model: HD32.2  
Serial No: 15036132  
ID No: BKK\_FS0680

### Customer

Name: ALS laboratory group (thailand) Co.,Ltd.  
Address: 104 Phatthanakan 40, Phatthanakan  
Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok  
10250 Thailand.

Received date: 10 JAN 2022  
Calibration date: 15 FEB 2022  
Issue date: 17 FEB 2022

### Reference Used During Calibration

- 1.Standard Temperature Probe Model: STS-100 A500,  
Serial No.: 667682-09, Due date: 25 Mar 2022
- 2.Digital Temperature Indicator Model: DTI-1000-A MK  
II, Serial No.: 671407-00591 Due date: 04 June 2022

### Calibration Condition

Temperature:  $(23 \pm 3)^{\circ}\text{C}$   
Relative Humidity:  $(55 \pm 15)\%$

### Calibration Procedure

The temperature calibration was done by In-House  
calibration method as WI-CL-001 according to  
comparison method with standard digital temperature  
indicator and standard temperature probe. The  
temperature scale use was based on ITS-90.

### Traceability

The measurement results are traceable to the  
international system of units (SI) through National  
Institute of Metrology Thailand (NIMT) Certificate  
number: TT-0036-21, Certificate number: ER-0032-  
21

REVIEW BY

*Narakee P.*

APPROVED BY

*[Signature]*

NEXT CAL. DATE

15/2/23

### Calibrated by

- ☒ Mr. Sorawit Thachalad  
☐ Miss Orathai Wiwatwittaya



Approved Signatory: .....

*[Signature]*

Mr. Parinya Booncharoen  
Calibration Department Manager

**Result of Calibration:** ☒ Without Adjustment ☐ With Adjustment

**Calibration Range:** 20 – 40 °C

**Function:**

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 15015846.

Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.053	20.1	0.0	0.099
30	25.034	25.1	0.1	0.099
30	30.014	30.1	0.1	0.099
30	35.019	35.1	0.1	0.099
30	40.006	40.1	0.1	0.099

Table 2: This equipment was connected with temperature probe Model: TP3207.2 S/N: 14032362.

Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.051	20.1	0.0	0.099
70	24.990	25.0	0.0	0.099
70	29.917	29.8	-0.1	0.099
70	34.873	34.7	-0.2	0.099
70	39.864	39.6	-0.3	0.099

Table 3: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: -.

Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.054	20.0	-0.1	0.099
110	25.036	25.0	0.0	0.099
110	30.017	30.0	0.0	0.099
110	35.024	35.0	0.0	0.099
110	40.001	40.0	0.0	0.099

UUC\* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.





# ภาคผนวก จ

---

สำเนาใบอนุญาตขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

ที่ อก ๐๓๑๐(๑)/ ๑๐๖๙



กรมโรงงานอุตสาหกรรม  
ถนนพระรามที่ ๖ เขตราชเทวี  
กรุงเทพมหานคร ๑๐๔๐๐

๒๘ มกราคม ๒๕๖๕

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน  
ลงวันที่ ๓๐ กรกฎาคม ๒๕๖๓

- สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น  
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ แผ่น  
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอต่ออายุ  
หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๕ สถานที่ตั้งเลขที่ ๑๐๔  
ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร  
ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย)  
จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

- ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย ตามสิ่งที่ส่งมาด้วย ๑  
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๖๒ ราย ตามสิ่งที่ส่งมาด้วย ๒  
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย จำนวน ๕๙ รายการ น้ำใต้ดิน  
จำนวน ๑๒๖ รายการ อากาศเสีย ๑๖ รายการ สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน ๓๕ รายการ และดิน  
จำนวน ๑๒๕ รายการ รวมทั้งสิ้นจำนวน ๓๖๑ รายการ ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ กันยายน ๒๕๖๖ หากประสงค์จะต่ออายุหนังสือ  
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอ  
ต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์  
เอกชน ซึ่งคำขอต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิริ จันทรเจต)

นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๒๐๒ ๔๑๔๖ ๐ ๒๒๐๒ ๔๐๐๒

โทรสาร ๐ ๒๓๕๔ ๓๒๐๘ ๐ ๒๓๕๔ ๓๔๑๕

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

เลขทะเบียน ว-๒๐๔

ที่ อก ๐๓๑๐(๑)/

ลงวันที่ ๒๘ มกราคม ๒๕๖๕

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย

๑) นางสาวยุพาพร จันทร์เปล่ง

ทะเบียนเลขที่ ว-๒๐๔-ค-๔๗๐๐

๒) นางสาวชนัญ โกลมารกุล ณ นคร

ทะเบียนเลขที่ ว-๒๐๔-ค-๔๗๐๑

๓) นายศรายุทธ จิตรานนท์

ทะเบียนเลขที่ ว-๒๐๔-ค-๔๗๐๒

๔) นางสาวกนกกร เอนก

ทะเบียนเลขที่ ว-๒๐๔-ค-๖๑๑๑

๕) นายสุริยา สอนแก้ว

ทะเบียนเลขที่ ว-๒๐๔-ค-๖๑๑๒

๖) นายวิชาญ ชูณหะวัณ

ทะเบียนเลขที่ ว-๒๐๔-ค-๖๑๑๓

(นายศิริระ จันทร์เลิศ)

นักวิทยาศาสตร์ชำนาญการพิเศษ วิชาการราชการแทน

ผู้อำนวยการกองวิจัยและพัฒนามลพิษโรงงาน

ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม



เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

เลขทะเบียน ว-๒๐๔

ที่ อก ๐๓๑๐(๑)/ ๑๐๖๙

ลงวันที่ ๒๘ มกราคม ๒๕๖๕

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๖๒ ราย

๑) นางสาวจินดา ไชจุลธรรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๐๘
๒) นางสาวสาวิตรี น้อยเสงี่ยม	ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๐๙
๓) นางสาวชนัญญาญจน์ อัมขม	ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๐
๔) นางสาวนรินทร์ สายเส็ง	ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๕
๕) นางสาวนันทวดี สมบูรณ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๖
๖) นางสาวศรียา เฉลิมธำรงค์	ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๗
๗) นางสาวสรารัตน์ มงคลจิรวดี	ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๙
๘) นางสาวศิริลักษณ์ พึ่งแพง	ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๒๐
๙) นายณพพงศ์ จันทรพันธุ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๐๘
๑๐) นายนรเศรษฐ์ โกมลาลัย	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๑๑
๑๑) นายธินว จริยา	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๑๔
๑๒) นางสาวเกศรินทร์ แก้วมัน	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๑๖
๑๓) นางสาวสุวิมล ชัยเรืองวุฒิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๑๗
๑๔) นางสาวสุชาดา ธรรมถาวร	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๑
๑๕) นางสาวเปมิกา ชัยเดชธนกุล	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๓
๑๖) นางสาวศศิธร หมูสวัสดิ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๔
๑๗) นางสาวเสาวลักษณ์ ภู่นภาอำพร	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๕
๑๘) นายอภิสิทธิ์ สิงหา	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๖
๑๙) นายศักดิ์สิทธิ์ ไพศาลพิสุทธิ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๗
๒๐) ว่าที่ร้อยตรีหญิง พรรณิภา ขำเจริญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๘
๒๑) นางจิตดา คำภูแก้ว	ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๓๑
๒๒) นางสาวอรรพรรณ รักษย	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๑๕
๒๓) นางสาวนพรัตน์ แยมกรานต์	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๑๙
๒๔) นายจุลเดช วารินทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๐
๒๕) นางสาวดาญรัตน์ ร้องคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๑
๒๖) นายนคร สุขเจริญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๒
๒๗) นายบัญชา นามเขตต์	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๓
๒๘) นายพรมมี ศรีปัดเนตร	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๕
๒๙) นายอุทิศ อุ่นสิม	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๖
๓๐) ว่าที่ร้อยตรี เฉลิมเกียรติ อมรศรีเสริม	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๘
๓๑) นางสาววริยา สร้างนา	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๙
๓๒) นายอนุพงศ์ รัตนศรีประเสริฐ	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๓๐
๓๓) นางสาวจุฑารัตน์ โอนสันเทียะ	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๔๒
๓๔) นางสาวจารุวรรณ พิมพ์อภิกฤติยา	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๗๖

(นายศิริะ จันทร์เจิด)

๓๕) นางสาวปรางค์ทิพย์...

มหาวิทยาลัยราชภัฏวไลยอลงกรณ์ จังหวัดปทุมธานี

ผู้อำนวยการกองวิจัยและพัฒนาระบบสารสนเทศ

วิทยาลัยการอาชีพหนองปรือ อำเภอบางบาล จังหวัดสุพรรณบุรี

๓๕) นางสาวปรางค์ทิพย์ กิจไพศาลศักดิ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๗๙
๓๖) นางสาวเตือนใจ ทางกลาง	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๐
๓๗) นางสาวจิราพร ศิริเวช	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๑
๓๘) นายวรกร ผูกרך	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๓
๓๙) นายทง วิริยะสทกิจ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๔
๔๐) นายธนิศ เจนจบ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๕
๔๑) นายคณิศร ขำเพชร	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๖
๔๒) นายอรรคพล นิยมวิทยาพันธ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๗
๔๓) นายภูวิช พรหมสะอาด	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๘
๔๔) นายธนเดช โภคาพิพัฒน์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๙
๔๕) นายชวฤทธิ์ วงษ์จันทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๐
๔๖) นายอาทิตย์ ศรีแสน	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๑
๔๗) นายเจษดินทร์ คงศักดิ์ไทย	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๒
๔๘) นายจรัส บุญยั้ง	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๕
๔๙) นายธนาณัติ เอนก	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๖
๕๐) นายอภิวัฒน์ ทุมหนู	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๗
๕๑) นางสาวสุภาขวัญ มาก	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๘
๕๒) นางสาวหัตพร ขวาลสมบูรณ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๐
๕๓) นางสาวธิดิมา บุญเพ็ง	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๑
๕๔) นางสาวกนกอร เข้มเพ็ชร	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๒
๕๕) นางสาวพัชรียา หงษ์สมดี	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๓
๕๖) นางสาวภาวนิดา สุรวงศ์ตระกูล	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๔
๕๗) นางสาวภาณุมาศ นามวัฒน์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๕
๕๘) นางสาวอุไรรัตน์ ทิงสร้างแป้น	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๖
๕๙) นายธีรวัฒน์ ปวงสุข	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๗
๖๐) นายอิทธิพล ยะโส	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๘
๖๑) นายประพนธ์ วรรณชูชัย	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๙
๖๒) นายชยธร พวงทิพย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๑๐
๖๓) นางสาวกนกวรรณ จันทบาล	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๑๑
๖๔) นางสาวเกษร หลักบุญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๑๒
๖๕) นายสิทธิโชค ธงเงิน	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๑๓
๖๖) นางศิวารรณ ใจบุญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๐๕
๖๗) นางสาวพรรณธิดา พุ่มคง	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๐๘
๖๘) นางสาวศรณีย์ ยิ่งดี	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๐๙
๖๙) นายนวกัทร ศรีวิริยะ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๐
๗๐) นายสุวิชา ทองอ่อน	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๑
๗๑) นายวิญญู บุญตะนัย	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๓

(นายศิระ จันทรเจ็ด)

นักวิทยาศาสตร์ชำนาญการพิเศษ วิชาการการแพฐ

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

-----

๗๒) นายสมบูรณ์...

๗๒) นายสมบุรณ์ บุตรจันทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๔
๗๓) นายวิรัตน์ ไชยชนะรา	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๕
๗๔) นายณฤเบศน์ เพิ่มพูน	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๖
๗๕) นายจิรณัฐ ขาวละออ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๗
๗๖) นายสมโภช วันสา	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๘
๗๗) นายอัสรี นามบุรี	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๙
๗๘) นายณัฐนันท์ ปานประเสริฐ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๒๐
๗๙) นายอัครเวศ จ่อสาว	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๒๑
๘๐) นายประเสริฐ สุระขันธ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๒๒
๘๑) นายณกุล จันทร์เนียม	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๒๓
๘๒) นายพิรพงษ์ ทองคุณปรีดา	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๒๔
๘๓) นายณฤพล ทองนุช	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๒๕
๘๔) นายอนุวัฒน์ ม่วงแพร่	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๒๖
๘๕) นายเจตศราวุฒิ ปิตตะมะ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๒๗
๘๖) นายกฤษณะ สายวรรณ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๒๘
๘๗) นายพิชัย บุญยงค์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๒๙
๘๘) นายภาณุพงศ์ โหมวงศ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๓๐
๘๙) นายสามารถ คุ่มปลี	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๓๑
๙๐) นายสัญญาชัย โกศรีนาม	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๓๒
๙๑) นายณัฐวุฒิ ศรีประเสริฐ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๓๓
๙๒) นายชวัลรัช นาคพนม	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๓๔
๙๓) นายพงศธร ชัยทิพย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๓๕
๙๔) ว่าที่ร้อยตรี ภาณุพงศ์ แสนศรี	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๓๖
๙๕) นายสิทธิโชค ทาสีดา	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๓๗
๙๖) นายธนากร อินสุตา	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๓๘
๙๗) นางสาววรรณิษา ขาติวันชัย	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๓๙
๙๘) นางสาวพิมพ์ตะวัน มินากุล	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๔๐
๙๙) นางสาวเพชรรัตน์ สิงห์สมบูรณ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๔๑
๑๐๐) นางสาวชญานิษฐ์ พรหมจันทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๔๒
๑๐๑) นายเกียรติ ทวีราช	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๔๓
๑๐๒) นายจักริน หนัสนิชา	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๔๔
๑๐๓) นายฉัตรชัย สุขเปี้ย	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๔๕
๑๐๔) นายณรนนท์ ต๊ะทองคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๔๖
๑๐๕) นายตุลยพล สมนอก	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๔๗
๑๐๖) นายทักษ์ดนัย อุบลศรี	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๔๘
๑๐๗) นายธนศร นามะภูณนา	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๔๙
๑๐๘) นายธิตีพงศ์ บัวแดง	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๕๐

(นายธีระ จันทร์เฑียร)

นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาการแทน

ผู้อำนวยการกองวิจัยและพัฒนากยผลพืชโรงงาน

บริษัท การเกษตรและเทคโนโลยีการเกษตร จำกัด

๑๐๙) นายณนทชัย...



๑๐๙) นายพนนทชัย อุปถัมภ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๕๔
๑๑๐) นายนิรุฒ พลสุทธิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๕๕
๑๑๑) นายนิพนธ์วัฒน์ สาริน	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๕๖
๑๑๒) นายปิยะนัฐ พลมะศรี	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๕๗
๑๑๓) นายพงศ์สิริ โสมเขียว	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๕๘
๑๑๔) นายพีรพัฒน์ กำคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๕๙
๑๑๕) นายภาณุพงศ์ มานิตย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๐
๑๑๖) นายมงคล ผลาทิพย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๑
๑๑๗) นายมนินทร์ พูลศิริ	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๒
๑๑๘) นายสิรินันท์ ทองอิน	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๓
๑๑๙) นายอเนชา ทันสมัย	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๔
๑๒๐) นายอดิศักดิ์ ผมไผ	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๕
๑๒๑) นายอนันตชัย วิสุม	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๖
๑๒๒) นายณัฐดนัย เจือละออง	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๗
๑๒๓) นายวรวิธ ดินัก	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๘
๑๒๔) นายแสงตะวัน นະตะສັດ	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๙
๑๒๕) นายยุทธพงศ์ รัตนะ	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๐
๑๒๖) นายชัยณวุฒิ ไชยชนะนิจ	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๑
๑๒๗) นายวิศรุต ศรีธรรมมา	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๒
๑๒๘) นายพนนทกร เผือกผ่อง	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๓
๑๒๙) นายกำชัย สุทธะ	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๔
๑๓๐) นางสาวณัฐภรณ์ รักทะเล	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๑๙
๑๓๑) นางสาวประภาภรณ์ บุตรพรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๐
๑๓๒) นางสาวนิลาวัลย์ นามพรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๑
๑๓๓) นางสาวพัชรินทร์ แสนสร้อย	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๒
๑๓๔) นายไพโรจน์ เบรัมย์พิมาย	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๓
๑๓๕) นางสาวศุภมาศ ทองมาก	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๔
๑๓๖) นางสาวลลิตา จิตรสว่าง	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๕
๑๓๗) นางสาวชไมพร เสีกัญเขียว	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๖
๑๓๘) นางสาวกฤติมาพร คำมีแก่น	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๗
๑๓๙) นางสาวสกุลรัตน์ ภาควุฒิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๘
๑๔๐) นางสาวกาญจนา คงคุณ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๙
๑๔๑) นางสาวไพรินทร์ ศรีรูปี	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๐
๑๔๒) นางสาวทิพนันทร ผุยปัญญา	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๑
๑๔๓) นางสาวสาธิตา ปานทอง	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๒
๑๔๔) นางสาวอริสา ทองนวล	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๓
๑๔๕) นางสาวอรยา คำคล่อง	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๔

(นายศิระ จันทร์เจิด)

นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาการแทน

ผู้อำนวยการกองวิจัยและพัฒนากยผลพืชโรงงาน

๑๔๖) นางสาวชุตติภรณ์...

๑๔๖) นางสาวชุตากรณ์ สุนทรสนาน	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๕
๑๔๗) นางสาวสุตารัตน์ นนทประสาท	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๖
๑๔๘) นางสาวรัชนิกร เนียมกลาง	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๗
๑๔๙) นางสาวกัญญารัตน์ ศรีนิลทา	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๘
๑๕๐) นางสาวอัญชลี คำจันทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๙
๑๕๑) นายบุญฤทธิ์ เอี่ยมเทศ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๐
๑๕๒) นายศิริวัฒน์ พานิชย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๑
๑๕๓) นางสาวศุภรดา ปันมยุรา	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๒
๑๕๔) นางสาวพาฤดี คุณนาน	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๓
๑๕๕) นางสาวจิราเจต ฟองดา	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๔
๑๕๖) นางสาวกนกภรณ์ อุระ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๕
๑๕๗) นางสาวอารยา มีชัย	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๖
๑๕๘) นางสาวจิตสุภา ประเทืองสุข	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๗
๑๕๙) นางสาวอริสา วิริยขันติธรรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๘
๑๖๐) นางสาววิษชุดา นาคผจญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๙
๑๖๑) นางสาวพนิดา ยอดอินทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๕๐
๑๖๒) นางสาวนันทิยา จันทะลุน	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๕๑



(นายศิริระ จันทรเจ็ด)

นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาการแทน

ผู้อำนวยการกองวิจัยและพัฒนากิจการโรงงาน

ปฏิบัติการงานทอผ้าไหมและไหมโรงงานอุตสาหกรรม

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

เลขทะเบียน ว-๒๐๔

ที่ อก ๐๓๑๐(๑)/ ๑๐๖๕

ลงวันที่ ๒๘ มกราคม ๒๕๖๕

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๖๑ รายการ

น้ำเสีย จำนวน 59 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldicarb	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
2	Aldicarb Sulfone	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
3	Aldicarb Sulfoxide	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
4	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
5	Arsenic	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
6	Barium	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
7	$\alpha$ -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
8	$\beta$ -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
9	$\delta$ -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
10	$\gamma$ -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
11	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method <sup>[4]</sup> 2) 5-Day BOD Test, Membrane Electrode Method <sup>[4]</sup>
12	Carbaryl	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
13	Carbofuran	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
14	Cadmium	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
15	Chemical Oxygen Demand	1) Closed Reflux, Colorimetric Method <sup>[4]</sup> 2) Closed Reflux, Titrimetric Method <sup>[4]</sup>
16	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
17	Chromium	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[4]</sup>
18	Color	ADMI Weighted-Ordinate Spectrophotometric Method



(นางริกาญจน์ จิตรสกุลไชย)

ผู้อำนวยการกลุ่มมาตรฐานวิชาการวิเคราะห์ทดสอบมลพิษ

และทะเบียนห้องปฏิบัติการ

19 Copper...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Copper	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
20	Cyanide	Distillation, Colorimetric Method <sup>[4]</sup>
21	2,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
22	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
23	2,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
24	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
25	2,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
26	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
27	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
28	Endosulfan Sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
29	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
30	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
31	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
32	Endrin Aldehyde	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
33	Formaldehyde	Distillation, Colorimetric Method <sup>[3]</sup>
34	Free Chlorine	1) DPD Ferrous Titrimetric Method <sup>[4]</sup> 2) Iodometric Method <sup>[4]</sup>
35	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
36	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
37	Hexavalent Chromium	Filtration, Colorimetric Method <sup>[4]</sup>
38	3-Hydroxycarbofuran	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
39	Lead	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
40	Manganese	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
41	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/Mass spectrometric Method <sup>[4]</sup>
42	Methiocarb	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
43	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>

วิมล

44 Methomyl...



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
44	Methomyl	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
45	Nickel	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
46	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method <sup>[4]</sup> 2) Soxhlet Extraction Method <sup>[4]</sup>
47	Oxamyl	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
48	Propoxur	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
49	pH	Electrometric Method <sup>[4]</sup>
50	Phenols	1) Distillation, Chloroform Extraction Method <sup>[4]</sup> 2) Distillation, Direct Photometric Method <sup>[4]</sup>
51	Selenium	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
52	Sulfide	Iodometric Method <sup>[4]</sup>
53	Temperature	Laboratory and Field Methods <sup>[4]</sup>
54	Total Dissolved Solids	Dried at 180 °C <sup>[4]</sup>
55	Total Kjeldahl Nitrogen	Semi-Micro Kjeldahl Method <sup>[4]</sup>
56	Total Suspended Solids	Dried at 103-105 °C <sup>[4]</sup>
57	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
58	Trivalent Chromium	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation <sup>[4]</sup>
59	Zinc	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[4]</sup>

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>

*วิภา*

3 Aldrin...

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ  
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
5	Antimony	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
8	Barium	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
9	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
11	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
12	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
13	Benzoic Acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
14	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
15	Benzo[g,h,i]perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>


วิธีทาง)

18 Bis(2-ethylhexyl)phthalate...

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ  
และหน่วยงานที่เกี่ยวข้อง

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
21	Butanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup> Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
22	Butyl Benzyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
25	Carbon Disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
27	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
33	Chromium	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>



34 Chromium (III)...

(นางวิภาดาญจน์ นิตกรกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation <sup>[4]</sup>
35	Chromium (VI)	Colorimetric Method <sup>[4]</sup>
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
37	Cyanide	Distillation, Colorimetric Method <sup>[4]</sup>
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
39	DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
40	DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
41	DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
42	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
43	Di-n-Butyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
47	3,3-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>

วิมล

(นางริกาญจน์ ฉัตรสกุลใจ)


ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

กองควบคุมและปฏิบัติการ

51 cis-1,2-Dichloroethylene...



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
57	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
58	Diethyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
63	Di-n-Octyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
64	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
65	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
67	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>



(นางริกาญจน์ นัตถกุลวิไล)

ผู้อำนวยการศูนย์มาตรฐานวิชาการวิเคราะห์ทดสอบมลพิษ  
และทะเบียนห้องปฏิบัติการ

68 Fluorene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
68	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
69	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
70	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
74	$\alpha$ -HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
75	$\beta$ -HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
76	$\gamma$ -HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
81	Lead	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
82	Manganese	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
83	Mercury	1) Cold Vapor Atomic Absorption Spectrometric Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>

วิมล

84 Methanol...

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

กรมส่งเสริมการค้าระหว่างประเทศ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
84	Methanol	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup> 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
86	Methyl Bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
87	Methylene Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
89	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
90	Methyl tert-Butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
91	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
92	Nickel	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
95	N-Nitrosodi-n-Propylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB 1242 - PCB 1248 - PCB 1254 - PCB 1260	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>

วิมล

97 Pentachlorophenol...

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
98	pH	Electrometric Method <sup>[4]</sup>
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
100	Phenol	1) Distillation, Direct Photometric Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
102	Selenium	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
103	Silver	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
104	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
105	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
106	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
107	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
108	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
109	TPH (C <sub>5</sub> -C <sub>8</sub> )	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[13,24]</sup>
110	TPH (C <sub>8</sub> -C <sub>16</sub> )	Solvent Extraction, Gas Chromatographic Method <sup>[9,21]</sup>
111	TPH (C <sub>16</sub> -C <sub>35</sub> )	Solvent Extraction, Gas Chromatographic Method <sup>[9,21]</sup>
112	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
113	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>

วิมล

114 1,1,2-Trichloroethane...



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
114	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
115	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
118	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
119	Vanadium	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>
120	Vinyl Acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
121	Vinyl Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
122	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
123	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
124	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
125	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
126	Zinc	1) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[4]</sup>

**อากาศเสีย (ปล่อยระบาย) จำนวน 16 รายการ**

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
2	Arsenic	Isokinetic, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>

*วิมล*

3 Carbon Monoxide...

(นางริภาณูจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

กรมควบคุมมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Carbon Monoxide	1) Sampling Bag Non-Dispersive Infrared Method <sup>[5]</sup> 2) Non-Dispersive Infrared Method <sup>[5]</sup> 3) Instrumental Analyzer Method <sup>[5]</sup>
4	Chlorine	1) Absorption Sampling, Ion Chromatographic Method <sup>[5]</sup> 2) Isokinetic Sampling, Ion Chromatographic Method <sup>[5]</sup>
5	Copper	Isokinetic, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
6	Dioxins	Isokinetic Sampling, Analysis by ISO/IEC 17025 Accredited Laboratory or Analysis by Department of Industrial Works Registered Laboratory (Dioxins/Furans Analysis Approved) <sup>[5]</sup>
7	Hydrogen Chloride	1) Absorption Sampling, Ion Chromatographic Method <sup>[5]</sup> 2) Isokinetic Sampling, Ion Chromatographic Method <sup>[5]</sup>
8	Hydrogen Sulfide	Absorption Sampling, Iodometric Method <sup>[5]</sup>
9	Lead	Isokinetic, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
10	Mercury	1) Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[5]</sup> 2) Isokinetic, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
11	Opacity	Ringelmann's Method <sup>[2]</sup>
12	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method <sup>[5]</sup> 2) Chemiluminescence Method <sup>[5]</sup> 3) Instrumental Analyzer Method <sup>[5]</sup>
13	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method <sup>[5]</sup> 2) UV Fluorescence Method <sup>[5]</sup> 3) Instrumental Analyzer Method <sup>[5]</sup>
14	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method <sup>[5]</sup>
15	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method <sup>[5]</sup>
16	Xylene	Adsorption Sampling, Gas Chromatographic Method <sup>[5]</sup>

วิมล

สิ่งปลูก...

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup>
2	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
3	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>

วิมล

6 Cadmium...

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
6	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,19,25]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup>
8	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
9	Chromium (III)	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation Method <sup>[1,6,15,17]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation Method <sup>[1,6,16,17]</sup> 3) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method <sup>[7,8,15,17]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method <sup>[7,8, 16,17]</sup>
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method <sup>[1,6,17]</sup> 2) Alkaline Digestion, Colorimetric Method <sup>[8,17]</sup>

*วิมล*

(นางริกาญจน์ ฉัตรสกุลวิไล)

11 Cobalt...

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

.....แผนกปฏิบัติการ



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
12	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
13	2,4-D	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup>
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup>
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup>
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup>

จิรพร

2) Soxhlet...

(นางริภาณูจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

และคณะผู้รับผิดชอบปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
17	Dieldrin	2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup> 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup>
18	Endrin	2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup> 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup>
19	Heptachlor	2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup> 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup>
20	Lead	2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup> 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup>
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[1,6,18]</sup>

วิมล

2) Waste Extraction...

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
23	Methoxychlor	2) Waste Extraction, Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method <sup>[1,6,19]</sup> 3) Waste Extraction, Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method <sup>[1,6,20]</sup> 4) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[18]</sup> 5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method <sup>[19]</sup> 6) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method <sup>[20]</sup>
24	Mirex	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup>
25	Molybdenum	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup>
26	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>

วิภาดา

27 Polychlorinated...

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิชาการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	<p>Polychlorinated biphenyls (PCBs)</p> <ul style="list-style-type: none"> <li>- Aroclor 1016</li> <li>- Aroclor 1221</li> <li>- Aroclor 1232</li> <li>- Aroclor 1242</li> <li>- Aroclor 1248</li> <li>- Aroclor 1254</li> <li>- Aroclor 1260</li> <li>- 2-Chlorobiphenyl</li> <li>- 2,3-Dichlorobiphenyl</li> <li>- 2,2',5-Trichlorobiphenyl</li> <li>- 2,4',5-Trichlorobiphenyl</li> <li>- 2,2',3,5'-Tetrachlorobiphenyl</li> <li>- 2,2',5,5'-Tetrachlorobiphenyl</li> <li>- 2,3',4,4'-Tetrachlorobiphenyl</li> <li>- 2,2',3,4,5'-Pentachlorobiphenyl</li> <li>- 2,2',4,5,5'-Pentachlorobiphenyl</li> <li>- 2,3,3',4',6-Pentachlorobiphenyl</li> <li>- 2,2',3,4,4',5'-Hexachlorobiphenyl</li> <li>- 2,2',3,4,5,5'-Hexachlorobiphenyl</li> <li>- 2,2',3,5,5',6-Hexachlorobiphenyl</li> <li>- 2,2',4,4',5,5'-Hexachlorobiphenyl</li> <li>- 2,2',3,3',4,4',5-Heptachlorobiphenyl</li> <li>- 2,2',3,4,4',5,5'-Heptachlorobiphenyl</li> <li>- 2,2',3,4,4',5',6-Heptachlorobiphenyl</li> <li>- 2,2',3,4',5,5',6-Heptachlorobiphenyl</li> <li>- 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl</li> </ul>	<p>1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method<sup>[1,9,23]</sup></p> <p>2) Soxhlet Extraction, Gas Chromatographic Method<sup>[10,23]</sup></p> <p>3) Automated Soxhlet Extraction, Gas Chromatographic Method<sup>[22,31]</sup></p>

วิมล

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

28 Pentachlorophenol...



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
28	Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup>
29	pH	Electrometric Method <sup>[29,30]</sup>
30	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
31	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup>
32	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
33	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,25]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 3) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[22,31]</sup>
34	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>

Signature

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์หกลมลพิษ


4) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
35	Zinc	4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[7,16]</sup> 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[1,6,16]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[7,16]</sup>

ดิน จำนวน 125 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
3	Aldrin	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
4	Anthracene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
5	Antimony	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[7,16]</sup>
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[7,16]</sup>
7	Atrazine	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
8	Barium	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[7,16]</sup>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
9	Benz(a)anthracene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
11	Benzo(b)fluoranthene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
12	Benzo(k)fluoranthene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
13	Benzoic acid	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
14	Benzo(a)pyrene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
15	Benzo(g,h,i)perylene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[7,16]</sup>
17	Bis(2-chloroethyl)ether	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
18	Bis(2-ethylhexyl)phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
21	Butanol	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method <sup>[12,24]</sup>
22	Butyl Benzyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[7,16]</sup>
24	Carbazole	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
25	Carbon Disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>



(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

26 Carbon tetrachloride...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
27	Chlordane	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
28	p-Chloroaniline	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
32	2-Chlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
33	Chromium	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[7,16]</sup>
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method <sup>[7,8,15,17]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method <sup>[7,8,16,17]</sup>
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method <sup>[8,17]</sup>
36	Chrysene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
37	Cyanide	Extraction, Distillation, Colorimetric Method <sup>[26,27,28]</sup>
38	2,4-D	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
39	DDD	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>

วิฑูรย์

(นางริภาณูจน์ จิตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

40 DDE...



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
40	DDE	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
41	DDT	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
42	Dibenz(a,h)anthracene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
43	Di-n-Butyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
47	3,3-Dichlorobenzidine	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
53	2,4-Dichlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>

วิมล

(นางริกาญจน์ อัครสกุลใจ)

57 Dieldrin...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
57	Dieldrin	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
58	Diethyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
59	2,4-Dimethylphenol	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
60	2,4-Dinitrophenol	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
61	2,4-Dinitrotoluene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
62	2,6-Dinitrotoluene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
63	Di-n-Octyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
64	Endosulfan	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
65	Endrin	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
67	Fluoranthene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
68	Fluorene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
69	Heptachlor	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
70	Heptachlor Epoxide	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
71	Hexachlorobenzene	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
73	n-Hexane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
74	$\alpha$ -HCH	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
75	$\beta$ -HCH	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
76	$\gamma$ -HCH	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
77	Hexachlorocyclopentadiene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
78	Hexachloroethane	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
79	Indeno(1,2,3-cd)pyrene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
80	Isophorone	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
81	Lead	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
82	Manganese	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[18]</sup>

วิมล

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

กองควบคุมมลพิษ

2) Thermal...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
84	Methanol	2) Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry <sup>[19]</sup> 3) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method <sup>[20]</sup> Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method <sup>[12,24]</sup>
85	Methoxychlor	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
86	Methyl Bromide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
87	Methylene Chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
88	2-methylphenol	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
89	2-Methylnaphthalene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
90	Methyl tert-Butyl Ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,24]</sup>
91	Naphthalene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
92	Nickel	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method <sup>[7,16]</sup>
93	Nitrobenzene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
94	N-Nitrosodiphenylamine	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
95	N-Nitrosodi-n-propylamine	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
96	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[23,32]</sup>

วิฑูรย์

(นางวิภาณูจน์ ฉัตรสกุลวิไล)

- Aroclor 1242...



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
	<ul style="list-style-type: none"> <li>- Aroclor 1242</li> <li>- Aroclor 1248</li> <li>- Aroclor 1254</li> <li>- Aroclor 1260</li> <li>- 2-Chlorobiphenyl</li> <li>- 2,2',3,5'-Tetrachlorobiphenyl</li> <li>- 2,2',5,5'-Tetrachlorobiphenyl</li> <li>- 2,3',4,4'-Tetrachlorobiphenyl</li> <li>- 2,2',3,4,5'-Pentachlorobiphenyl</li> <li>- 2,2',4,5,5'-Pentachlorobiphenyl</li> <li>- 2,3,3',4',6-Pentachlorobiphenyl</li> <li>- 2,2',3,4,4',5'-Hexachlorobiphenyl</li> <li>- 2,2',3,4,5,5'-Hexachlorobiphenyl</li> <li>- 2,2',3,5,5',6-Hexachlorobiphenyl</li> <li>- 2,2',4,4',5,5'-Hexachlorobiphenyl</li> <li>- 2,2',3,3',4,4',5'-Heptachlorobiphenyl</li> <li>- 2,2',3,4,4',5,5'-Heptachlorobiphenyl</li> <li>- 2,2',3,4,4',5',6-Heptachlorobiphenyl</li> <li>- 2,2',3,4',5,5',6-Heptachlorobiphenyl</li> <li>- 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl</li> </ul>	
97	Pentachlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
98	Phenanthrene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
99	Phenol	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>
100	Pyrene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25,31]</sup>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
101	Selenium	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[7,16]</sup>
102	Silver	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[7,16]</sup>
103	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
106	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
107	Toxaphene	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
108	TPH (C <sub>5</sub> -C <sub>6</sub> )	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
109	TPH (C <sub>8</sub> - C <sub>16</sub> )	1) Solvent Extraction, Gas Chromatographic Method <sup>[11,21]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[21,31]</sup>
110	TPH (C <sub>16</sub> - C <sub>35</sub> )	1) Solvent Extraction, Gas Chromatographic Method <sup>[11,21]</sup> 2) Automated Soxhlet Extraction, Gas Chromatographic Method <sup>[21,31]</sup>
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
114	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
115	2,4,5-Trichlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>

วิมล

116 2,4,6-Trichlorophenol...


(นางวิภาดาญ์ ฉัตรสกุลวิไล)

ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
116	2,4,6-Trichlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[25,31]</sup>
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
118	Vanadium	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[7,16]</sup>
119	Vinyl Acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
120	Vinyl Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
121	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
122	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
123	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
124	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[14,24]</sup>
125	Zinc	1) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method <sup>[7,16]</sup>

#### เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2548. เรื่อง การกำจัดสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว.ราชกิจจานุเบกษา. 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 11ง.
- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้กลบเป็นเชื้อเพลิง.ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.
- สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
- APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 23<sup>rd</sup> ed. Washington, DC: APHA, 2017.
- United States Environmental Protection Agency. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2019.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SW-846, 1997.

  
 (นางริกาญจน์ อัครสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

7. United States...





20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury In Sediment and Tissue Sample by Atomic Fluorescence Spectrometry. SW-846 Method 7474, 2007.**

21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics Using GC/FID. SW-846 Method 8015B, 1996.**

22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticides by Gas Chromatography. SW-846 Method 8081B, 2007.**

23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Polychlorinate Biphenyls (PCBs) by Gas Chromatography. SW-846 Method 8082, 1996.**

24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8260D, 2018.**

25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8270E, 2018.**

26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Total and Amenable Cyanide: Distillation SW-846 Method 9010B, 1996.**

27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oil. SW-846 Method 9013A, 1996.**

28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014, 2014.**

29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement. SW-846 Method 9040C, 2004.**

30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D, 2004.**

31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Automated Soxhlet Extraction. SW-846 Method 3541, 1994.**



(นางริกาญจน์ นัตตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ  
และทะเบียนห้องปฏิบัติการ



ที่ อก ๐๓๑๐(๓)/ ๖๔๗๐

กรมโรงงานอุตสาหกรรม  
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท  
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๘ มิถุนายน ๒๕๖๔

เรื่อง ขันทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลборาทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน  
ลงวันที่ ๒๙ เมษายน ๒๕๖๔

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอแอลเอส แลборาทอรี กรุ๊ป (ประเทศไทย) จำกัด จำนวน ๒ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลборาทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอขึ้นทะเบียน  
ห้องปฏิบัติการวิเคราะห์เอกชน พร้อมรายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ เจ้าหน้าที่ประจำ  
ห้องปฏิบัติการวิเคราะห์ และรายการสารมลพิษที่จะทำการวิเคราะห์ ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลборาทอรี กรุ๊ป  
(ประเทศไทย) จำกัด ขันทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน มีเลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่  
๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอลวกแดง จังหวัดระยอง โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

- |                          |               |              |
|--------------------------|---------------|--------------|
| ๑) นายเดช ช้างชน         | ทะเบียนเลขที่ | ว-๓๒๓-ค-๙๔๔๒ |
| ๒) นางวิลาวณีย์ บริรักษ์ | ทะเบียนเลขที่ | ว-๓๒๓-ค-๙๔๔๓ |
| ๓) นายสุพจน์ สลามเต๊ะ    | ทะเบียนเลขที่ | ว-๓๒๓-ค-๙๔๔๔ |

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์

- |                                 |               |              |
|---------------------------------|---------------|--------------|
| ๑) นางสาวนฤมล บรรจงกิจ          | ทะเบียนเลขที่ | ว-๓๒๓-จ-๙๔๔๕ |
| ๒) นางพจนา สีดา                 | ทะเบียนเลขที่ | ว-๓๒๓-จ-๙๔๔๖ |
| ๓) นางสาวธนิดา กุลสุริวงค์      | ทะเบียนเลขที่ | ว-๓๒๓-จ-๙๔๔๗ |
| ๔) นายพิทยา ทองแดง              | ทะเบียนเลขที่ | ว-๓๒๓-จ-๙๔๔๘ |
| ๕) นางชลธิชา สุนงข              | ทะเบียนเลขที่ | ว-๓๒๓-จ-๙๔๔๙ |
| ๖) ว่าที่ ร.ต.รณชัย ม่วงมา      | ทะเบียนเลขที่ | ว-๓๒๓-จ-๙๔๕๐ |
| ๗) นายวรารุณ พับพา              | ทะเบียนเลขที่ | ว-๓๒๓-จ-๙๔๕๑ |
| ๘) นายศักดิ์รินทร์ จรัสกาย      | ทะเบียนเลขที่ | ว-๓๒๓-จ-๙๔๕๒ |
| ๙) นายสุรศักดิ์ สาชิน           | ทะเบียนเลขที่ | ว-๓๒๓-จ-๙๔๕๓ |
| ๑๐) นางสาวเพชรคุณ ภาภูตานนท์    | ทะเบียนเลขที่ | ว-๓๒๓-จ-๙๔๕๔ |
| ๑๑) นายสถาพร ถาแก้ว             | ทะเบียนเลขที่ | ว-๓๒๓-จ-๙๔๕๕ |
| ๑๒) นายสุทธิดำรงค์ โชคปิตินันท์ | ทะเบียนเลขที่ | ว-๓๒๓-จ-๙๔๕๖ |

๑๓) นายวัลลภ หันไชยเนา	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๕๗
๑๔) นางสาววนาลี เจริญตระกูล	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๕๘
๑๕) นางสาวนิตา ผดุงจิตต์	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๕๙
๑๖) นายธนะสิทธิ์ วงศ์ไชย	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๖๐
๑๗) นายชัยนุสรณ์ เลิศนันทกุลชัย	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๖๑
๑๘) นายสัจจา เพ็ชรแสง	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๖๒
๑๙) นายกันตภณ มณีสัมพันธ์	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๖๓
๒๐) นางสาวจันทนีย์ โกเมนชนะ	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๖๔
๒๑) นายธารินทร์ อ็อกจินดา	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๖๕
๒๒) นายศุภณัฐ พิสัยพันธ์	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๖๖
๒๓) นายศุภชัย วงศ์สุริย์ฉาย	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๖๗
๒๔) นายปฐมพงศ์ กรสวัสดิ์	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๖๘
๒๕) นายไสว ตันโพธิ์	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๖๙
๒๖) นางสาวกิตติยา สัญญาอริยาภรณ์	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๗๐
๒๗) นางสาวเจษฎาพร ศรีบุญเรือง	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๗๑
๒๘) นางสาวมธุรินทร์ สิงห์เงา	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๗๒
๒๙) นางสาวธิดารัตน์ ศิริมังคะโร	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๗๓
๓๐) นายพิพัฒน์ นิภัทร์เศรษฐ์	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๗๔
๓๑) นายศิริวิทย์ เรืองสม	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๗๕
๓๒) นายปารามศ สัตยาคุณ	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๗๖
๓๓) นายณนุท ธรรมสโร	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๗๗
๓๔) นางสาวศุภรัตน์ โสจันทร์	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๗๘
๓๕) นายพชรกร อินทรเสนา	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๗๙
๓๖) นายทิวากร เชื้อมาก	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๘๐
๓๗) นายอนุรักษ์ ทองขจรศักดิ์	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๘๑
๓๘) นายอภิชาติ วิชาส	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๘๒
๓๙) นายจรัสระวี ศรีรักษา	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๘๓
๔๐) นายประสานมิตร เชื้อนเพชร	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๘๔
๔๑) นายภาณุวัฒน์ วังบง	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๘๕
๔๒) นายสันติ ชัยชนะ	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๘๖
๔๓) นายสิทธิชัย แก้วเกตุ	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๘๗
๔๔) นายทินกร กุลชาติ	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๘๘

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย จำนวน ๑๔ รายการ  
อากาศเสีย (ปล่องระบาย) จำนวน ๗ รายการ และน้ำใต้ดิน จำนวน ๓ รายการ รวมทั้งสิ้นจำนวน ๒๔ รายการ  
ตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้มีอายุ ๓ ปี นับจากวันที่กรมโรงงานอุตสาหกรรมออกหนังสือ หากประสงค์  
จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบ  
คำขอต่อกรมโรงงานอุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการ  
วิเคราะห์เอกชน ซึ่งคำขอต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นางจินดา เตชะศรีนทร์)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน  
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

๒๘ มิ.ย. ๒๕๖๔

กองวิจัยและเตือนภัยมลพิษโรงงาน

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๘๐๕ ๗๒๖๑-๓

ไปรษณีย์อิเล็กทรอนิกส์ [eirw@diw.mail.go.th](mailto:eirw@diw.mail.go.th)



เอกสารแนบท้ายหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๓๒๓

ที่ อก ๐๓๑๐(๓)/

๖๔๗๐

ลงวันที่

๒๘

มิถุนายน

๒๕๖๔

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๒๔ รายการ

น้ำเสีย จำนวน 14 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Biochemical Oxygen Demand	1) 5-Day BOD Test, Membrane Electrode Method <sup>[2]</sup> 2) 5-Day BOD Test, Azide Modification Method <sup>[2]</sup>
2	Chemical Oxygen Demand	1) Open Reflux, Titrimetric Method <sup>[2]</sup> 2) Closed Reflux, Colorimetric Method <sup>[2]</sup> 3) Closed Reflux, Titrimetric Method <sup>[2]</sup>
3	Color	ADMI Weighted – Ordinate Spectrophotometric Method <sup>[2]</sup>
4	Cyanide	Distillation, Colorimetric Method <sup>[2]</sup>
5	Formaldehyde	Distillation, Colorimetric Method <sup>[1]</sup>
6	Free Chlorine	DPD-Ferrous Titrimetric Method <sup>[2]</sup>
7	Oil and Grease	Liquid-Liquid Partition-Gravimetric Method <sup>[2]</sup>
8	pH	Electrometric Method <sup>[2]</sup>
9	Phenols	1) Distillation, Chloroform Extraction Method <sup>[2]</sup> 2) Distillation, Direct Photometric Method <sup>[2]</sup>
10	Sulfide	ZnS Precipitation, Iodometric Method <sup>[2]</sup>
11	Temperature	Laboratory and Field Method <sup>[2]</sup>
12	Total Dissolved Solids	Dried at 180 °C <sup>[2]</sup>
13	Total Kjeldahl Nitrogen	Semi-Micro Kjeldahl Method <sup>[2]</sup>
14	Total Suspended Solids	Dried at 103-105 °C <sup>[2]</sup>

อากาศเสีย (ปล่อยระบาย) จำนวน 7 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Carbon Monoxide	1) Sampling Bag, Non-Dispersive Infrared Method <sup>[5]</sup> 2) Instrumental Analyzer Method <sup>[8]</sup>
2	Hydrogen Sulfide	Absorption Sampling, Iodometric Method <sup>[5]</sup>
3	Opacity	Ringelmann's Method <sup>[3,4]</sup>
4	Oxide of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method <sup>[6]</sup> 2) Instrumental Analyzer Method <sup>[9]</sup>
5	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method <sup>[5]</sup> 2) Instrumental Analyzer Method <sup>[10]</sup>

วิภา สัมฤทธิ์

(นางสาววิชุดา สัมฤทธิ์ผล)

ผู้อำนวยการ

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

Sulfuric Acid...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
6	Sulfuric Acid	Isokinetic Sampling, Barium – Thorin Titrimetric Method <sup>[6]</sup>
7	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method <sup>[7]</sup>

น้ำใต้ดิน จำนวน 3 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Cyanide	Distillation, Colorimetric Method <sup>[2]</sup>
2	pH	Electrometric Method <sup>[2]</sup>
3	Phenols	Distillation, Direct Photometric Method <sup>[2]</sup>

เอกสารอ้างอิง

1. ธงชัย พรหมสวัสดิ์ และวิบูลย์ลักษณ์ วิสุมธิดักดิ์, บรรณาธิการ. (2547) คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย.

2. APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 23<sup>rd</sup> ed. Washington, DC : APHA, 2017

3. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้เกลบเป็นเชื้อเพลิง.

ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

4. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของของหม้อน้ำของโรงงาน.

ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

5. United States Environmental Protection. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2017.

6. United States Environmental Protection. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2019.

7. United States Environmental Protection. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2020.

8. United States Environmental Protection Agency. Determination of Carbon Monoxide Emissions from Stationary Sources; Instrumental Analyzer Procedure. 40 CFR 60. Appendix A Method 10, 2017.

9. United States Environmental Protection Agency. Determination of Oxide of Nitrogen Emissions from Stationary Sources; Instrumental Analyzer Procedure. 40 CFR 60. Appendix A Method 7E, 2019.

10. United States Environmental Protection Agency. Determination of Sulfur Dioxide Emissions from Stationary Sources; Instrumental Analyzer Procedure. 40 CFR 60. Appendix A Method 6C, 2017.

วิภา สันกุล

(นางสาววิชุดา สัมฤทธิ์ผล)

ผู้อำนวยการ

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก