



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 21CH1201

Page.: 1 of 3

## Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	SevenCompact pH/Ion S220
Serial No. :	B329579021
ID No. :	TLC-L020
Condition As-Received:	Used Item
Received Date :	10 September 2021
Calibration Date :	13 September 2021
Reference :	2109-0403DN-1
Submitted by :	Tops-Lab Consultants Co.,Ltd 189 Moo 3, Bangrakpattana, Bangbuathong, Nonthaburi 11110
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lerngagtrakul

Approved by :

Approved Signatory

(☒) Malee Butkruea  
( ) Saithip Meangmai  
( ) Warakorn Lerngagtrakul

Issue Date : 20 September 2021

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0030260



Cert.No.: 21CH1201

Page.: 2 of 3

**Condition of this calibration result**

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	46530031	130RC098	20E3666	14 Oct 2021
2) Ref. Standard Thermometer	4982054	110RC044	20I1233	15 Oct 2021

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	754028	28 June 2023
pH 6.985	CPA chem	725927	12 Jan 2022
pH 10.015	CPA chem	761018	02 Aug 2022

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results**

**Function : mV Measurement**

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( ±mV )	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: B329579021	4.000	177.48	177.2	4.000	0.058	2.00
	7.000	0.00	-0.2	7.000	0.058	2.00
	10.000	-177.48	-177.6	10.000	0.058	2.00







Cert.No.: 21CH1201

Page.: 3 of 3

### Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading ( mV )	Uncertainty of pH measurement ( $\pm$ )	Coverage factor $k$
pH Electrode S/N.: 0414241	4.008	4.005	181.3	0.0044	2.00
	6.985	6.989	6.8	0.0078	2.00
	10.015	10.008	-171.1	0.013	2.07

### Function : Temperature Measurement

( \* ) Without adjustment

This equipment was connected with Temperature Probe;

- Model : InLab Expert Pro-ISM

- Serial No. : 0414241

Dimension of probe;

- Length : 120 mm.

- Diameter : 12 mm.

- Immersion Depth : 100 mm.

Calibration Point ( °C )	Standard Temperature ( °C )	UUC* Reading ( °C )	Error ( °C )	Uncertainty of measurement ( $\pm$ °C )	Coverage factor $k$
23.0	23.003	22.8	-0.203	0.20	2.00
25.0	25.003	24.8	-0.203	0.20	2.00
27.0	27.002	26.9	-0.102	0.20	2.00

Remark : - UUC\* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 21T5664  
REFERENCE No : 61413-5

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : INCUBATOR  
**MANUFACTURER** : AQUALYTIC  
**MODEL** : ET618-4  
**SERIAL No** : 0109/13922  
**ID No** : TLC-L005  
**CONDITION AS RECEIVED** : USED ITEM  
**SUBMITTED BY** : TOPS-LAB CONSULTANTS CO., LTD.  
189 MOO 3 BANGRAKPATTANA BANGBUATHONG  
NONTABURI 11110

**CALIBRATED BY** : CHAICHARN CH.

**CALIBRATION DATE** : 08-Jun-21

**APPROVED BY** : 

**ISSUED DATE** : 09-Jun-21

**RECEIVED DATE** : 08-Jun-21





CERTIFICATE No : 21T5664

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : INCUBATOR  
MANUFACTURER : AQUALYTIC  
MODEL : ET618-4  
ID No : TLC-L005  
RECEIVED DATE : 08-Jun-21  
AMBIENT TEMPERATURE : 25 °C ± 1 °C

S/N : 0109/13922  
CALIBRATION DATE : 08-Jun-21  
RELATIVE HUMIDITY : 50 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	6635300	20T7221	11-Jul-21

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

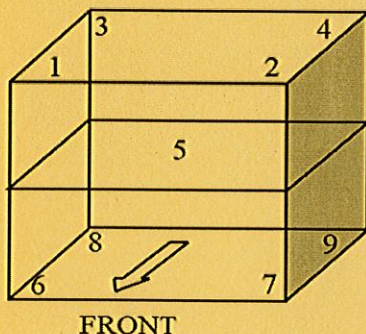

#### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 0
Overall Line Voltage (V) variation : 4
Instrument Condition : Normal
Chamber Size (W*L*H): 54*50*70 cm

#### CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
20.0	20.0	0.25	0.27	0.61

#### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
20.0	20.0	19.77	19.78	19.74	19.77	19.82	19.76	19.79	19.63	19.71	0.35

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 22T4929

REFERENCE No : 65109-8

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : INCUBATOR

**MANUFACTURER** : AQUALYTIC

**MODEL** : ET618-4

**SERIAL No** : 0109/13922

**ID No** : TLC-L005

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : TOPS-LAB CONSULTANTS CO., LTD.  
189 MOO.3 BANGRAKPHATTHANA  
BANGBUATHONG NONTHABURI 11110

**CALIBRATED BY** : CHAICHARN CH.

**CALIBRATION DATE** : 23-May-22

**APPROVED BY** : 

**ISSUED DATE** : 27-May-22

**RECEIVED DATE** : 23-May-22





CERTIFICATE No : 22T4929

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : INCUBATOR  
MANUFACTURER : AQUALYTIC  
MODEL : ET618-4  
ID No : TLC-L005  
RECEIVED DATE : 23-May-22  
AMBIENT TEMPERATURE : 29 °C ± 1 °C

S/N : 0109/13922  
CALIBRATION DATE : 23-May-22  
RELATIVE HUMIDITY : 53 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7408027	21T6766	10-Jul-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

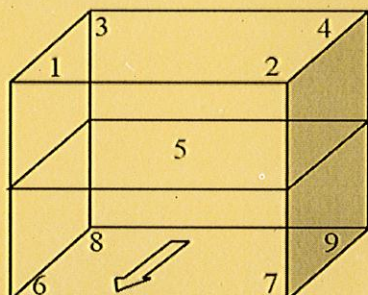

FRONT

#### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 0
Overall Line Voltage (V) variation : 5
Instrument Condition : Normal
Chamber Size (W*L*H): 55*44*57 cm

#### CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
20.0	20.0	0.15	0.47	0.68

#### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
20.0	20.0	19.85	19.46	19.84	19.91	19.86	19.88	19.86	19.83	19.88	0.25

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 21T5663

REFERENCE No : 61413-4

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : HOT AIR OVEN (AIR CHAMBER)

MANUFACTURER : BINDER

MODEL : FED 53

SERIAL No : 07-29050

ID No : TLC-L004

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TOPS-LAB CONSULTANTS CO., LTD.  
189 MOO 3 BANGRAKPATTANA BANGBUATHONG  
NONTABURI 11110

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 08-Jun-21

APPROVED BY : 

ISSUED DATE : 09-Jun-21

RECEIVED DATE : 08-Jun-21





CERTIFICATE No : 21T5663

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : HOT AIR OVEN (AIR CHAMBER)  
MANUFACTURER : BINDER  
MODEL : FED 53  
ID No : TLC-L004 S/N : 07-29050  
RECEIVED DATE : 08-Jun-21 CALIBRATION DATE : 08-Jun-21  
AMBIENT TEMPERATURE : 25 °C ± 1 °C RELATIVE HUMIDITY : 51 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOCOUPLE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	8009008	20T7223	11-Jul-21

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

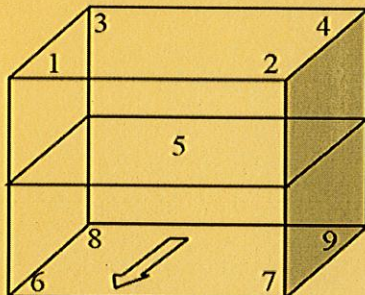

FRONT

#### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 2
Overall Line Voltage (V) variation : 12
Instrument Condition : Normal
Chamber Size (W*L*H): 40*33*40 cm

#### CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104	104	0.6	1.9	2.9
180	180	1.0	3.8	5.1

#### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (±°C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104	104	105.0	102.9	103.8	103.5	103.9	105.4	104.0	104.4	104.8	1.1
180	180	181.4	177.7	179.3	178.8	180.4	179.3	177.2	179.6	178.9	1.8

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 22T4925

REFERENCE No : 65109-4

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : HOT AIR OVEN (AIR CHAMBER)

MANUFACTURER : BINDER

MODEL : FED 53

SERIAL No : 07-29050

ID No : TLC-L004

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TOPS-LAB CONSULTANTS CO., LTD.  
189 MOO.3 BANGRAKPHATTHANA  
BANGBUATHONG NONTABURI 11110

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 23-May-22

APPROVED BY : 

ISSUED DATE : 27-May-22

RECEIVED DATE : 23-May-22





CERTIFICATE No : 22T4925

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : HOT AIR OVEN (AIR CHAMBER)  
MANUFACTURER : BINDER  
MODEL : FED 53  
ID No : TLC-L004 S/N : 07-29050  
RECEIVED DATE : 23-May-22 CALIBRATION DATE : 23-May-22  
AMBIENT TEMPERATURE : 28 °C ± 1 °C RELATIVE HUMIDITY : 52 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) DATA LOGGER WITH RTD	HYDRA 2635A	7408027	21T6766	10-Jul-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

**RESULT OF CALIBRATION** :- WITHOUT ADJUSTMENT

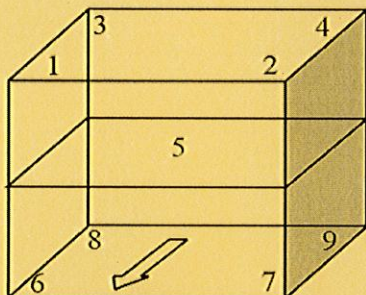

FRONT

### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 0
Overall Line Voltage (V) variation : 9
Instrument Condition : Normal
Chamber Size (W*L*H): 40*33*40 cm

### CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.0	0.38	1.39	1.81
180.0	180.0	0.23	0.94	1.13

### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	103.80	104.23	104.19	104.27	104.94	104.91	103.97	104.81	104.68	0.75
180.0	180.0	180.11	180.40	180.43	180.41	180.86	180.91	180.14	180.49	180.59	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 21T5670

REFERENCE No : 61414-3

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : WATER BATH

MANUFACTURER : MEMMERT

MODEL : WNB 14

SERIAL No : L410.1294

ID No : TLC-L009

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TOPS-LAB CONSULTANTS CO., LTD.  
189 MOO 3 BANGRAKPATTANA BANGBUATHONG  
NONTABURI 11110

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 08-Jun-21

APPROVED BY : 

ISSUED DATE : 09-Jun-21

RECEIVED DATE : 08-Jun-21

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 21T5670

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : WATER BATH  
MANUFACTURER : MEMMERT  
ID NUMBER : TLC-L009  
RECEIVED DATE : 08-Jun-21  
AMBIENT TEMPERATURE : 25 °C ± 1 °C

MODEL : WNB 14  
SERIAL NUMBER : L410.1294  
CALIBRATION DATE : 08-Jun-21  
RELATIVE HUMIDITY : 50 %RH ± 10 % RH


### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO ASTM E715-80 (REAPPROVED 2001) BY COMPARISON WITH CALIBRATED RTD. THE PROBES WERE PLACED ON FIVE POINTS AND LOCATED ONE PROBE IN EACH OF THE FOUR CORNERS OF THE BATH AND PLACED THE FIFTH RTD WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE WATER VOLUME (REFERENCE LOCATION) UNDER NO LOAD CONDITION.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	2625A	6603614	20T6466	06-Jul-21

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

**RESULT OF CALIBRATION :-** WITHOUT ADJUSTMENT

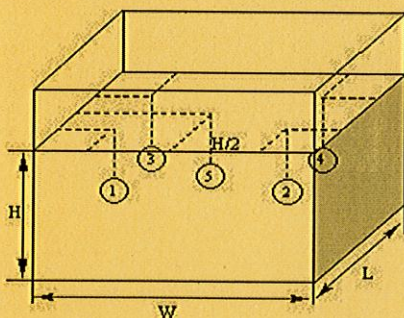

PROBE INSTALLATION  
POSITION IN THE BATH

### GENERAL INFORMATION

Overall Variation of Ambient Temperature around the Bath (°C) : 0
Overall Variation of Line Voltage (V) : 10
Instrument Condition : Normal
Bath Inner Size (W*L*H) : 36*33*16 cm

### BATH PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
85.0	85.0	0.14	0.20	0.46
95.0	95.0	0.15	0.53	0.72

### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations					Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	
85.0	85.0	85.10	85.00	85.06	84.91	85.11	0.21
95.0	95.0	93.67	93.28	93.41	93.15	93.43	0.21

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE BATH.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 21M5660

REFERENCE No : 61413-1

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : ELECTRONIC BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : MS205DU

SERIAL No : B420605448

ID No : TLC-L038

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TOPS-LAB CONSULTANTS CO., LTD.  
189 MOO 3 BANGRAKPATTANA  
BANGBUATHONG NONTABURI 11110

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 08-Jun-21

APPROVED BY : 

ISSUED DATE : 09-Jun-21

RECEIVED DATE : 08-Jun-21





CERTIFICATE No : 21M5660

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : ELECTRONIC BALANCE MODEL : MS205DU  
MANUFACTURER : METTLER TOLEDO S/N : B420605448  
ID No : TLC-L038 RECEIVED DATE : 08-Jun-21  
AIR PRESSURE : 1008mbar  $\pm$  1mbar CALIBRATION DATE : 08-Jun-21  
AMBIENT TEMPERATURE : 25° C  $\pm$  1° C RELATIVE HUMIDITY : 52 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING WEIGHT OF QUALITY CALIBRATION TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23
2) STANDARD WEIGHT	E2	15843	C02210419	10-Feb-23
3) STANDARD WEIGHT	E2	QK-I-349	M2103235S	26-Mar-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.0	0.00000	0.00000	0.000066
0.1	0.10002	-0.00002	0.000066
0.2	0.20003	-0.00003	0.000067
0.5	0.50003	-0.00003	0.000065
1.0	1.00004	-0.00004	0.000066
2.0	2.00002	-0.00002	0.000067
5.0	5.00000	0.00000	0.000068
10.0	9.99999	0.00001	0.000070
20.0	19.99994	0.00006	0.000075
50.0	49.99987	0.00013	0.00013
100.0	99.9998	0.0002	0.00019
200.0	199.9995	0.0005	0.00032

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	99.9997
2	99.9998
3	99.9997
4	99.9998
5	99.9998
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 22M4923

REFERENCE No : 65109-2

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : ELECTRONIC BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : MS205DU

SERIAL No : B420605448

ID No : TLC-L038

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TOPS-LAB CONSULTANTS CO., LTD.  
189 MOO.3 BANGRAKPHATTHANA  
BANGBUATHONG NONTHABURI 11110

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 23-May-22

APPROVED BY :   
PONGSAK J.

ISSUED DATE : 23-May-22

RECEIVED DATE : 23-May-22





CERTIFICATE No : 22M4923

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : ELECTRONIC BALANCE MODEL : MS205DU  
MANUFACTURER : METTLER TOLEDO S/N : B420605448  
ID No : TLC-L038 RECEIVED DATE : 23-May-22  
AIR PRESSURE : 1006mbar  $\pm$  1mbar CALIBRATION DATE : 23-May-22  
AMBIENT TEMPERATURE : 24°C  $\pm$  1°C RELATIVE HUMIDITY : 54 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING INTERNAL WEIGHT TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23
2) STANDARD WEIGHT	E2	15843	C02210419	10-Feb-23
3) STANDARD WEIGHT	E2	QK-I-349	M2103235S	26-Mar-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000045 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.000	0.0000	0.0000	0.000075
0.100	0.1000	0.0000	0.000075
0.20	0.2000	0.0000	0.000076
0.5	0.5000	0.0000	0.000076
1.0	1.0000	0.0000	0.000077
2.0	2.0000	0.0000	0.000077
5.0	5.0000	0.0000	0.000079
10.0	10.0000	0.0000	0.000082
20.0	20.0000	0.0000	0.000086
50.0	50.0000	0.0000	0.00011
100.0	100.0000	0.0000	0.00019
200.0	199.9999	0.0001	0.00032

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	99.9999
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT PRODUCTION AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 21T5665

REFERENCE No : 61413-6

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : INCUBATOR

**MANUFACTURER** : MEMMERT

**MODEL** : IF 55

**SERIAL No** : D216.1299

**ID No** : TLC-L069

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : TOPS-LAB CONSULTANTS CO., LTD.  
189 MOO 3 BANGRAKPATTANA BANGBUATHONG  
NONTABURI 11110

**CALIBRATED BY** : CHAICHARN CH.

**CALIBRATION DATE** : 08-Jun-21

**APPROVED BY** : 

**ISSUED DATE** : 09-Jun-21

**RECEIVED DATE** : 08-Jun-21





CERTIFICATE No : 21T5665

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : INCUBATOR  
MANUFACTURER : MEMMERT  
MODEL : IF 55  
ID No : TLC-L069  
RECEIVED DATE : 08-Jun-21  
AMBIENT TEMPERATURE : 25 °C ± 1 °C

S/N : D216.1299  
CALIBRATION DATE : 08-Jun-21  
RELATIVE HUMIDITY : 51 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7408027	20T7222	11-Jul-21

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

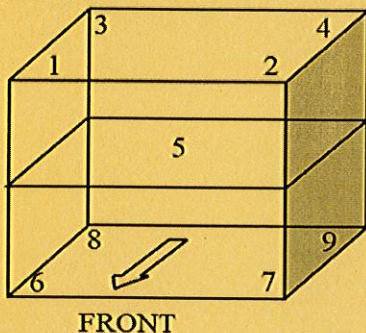

#### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 6
Instrument Condition : Normal

#### CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
35.0	35.0	0.06	0.29	0.31
44.5	44.5	0.06	0.30	0.43

#### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
35.0	35.0	35.07	35.14	35.19	35.12	35.17	35.06	34.96	35.06	35.09	0.25
44.5	44.5	44.77	44.81	44.89	44.79	44.81	44.67	44.57	44.76	44.86	0.36

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 22T4927

REFERENCE No : 65109-6

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : INCUBATOR

**MANUFACTURER** : MEMMERT

**MODEL** : IF 55

**SERIAL No** : D215.1343

**ID No** : TLC-L070

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : TOPS-LAB CONSULTANTS CO., LTD.  
189 MOO.3 BANGRAKPHATTHANA  
BANGBUATHONG NONTHABURI 11110

**CALIBRATED BY** : CHAICHARN CH.

**CALIBRATION DATE** : 23-May-22

**APPROVED BY** : 

**ISSUED DATE** : 31-May-22

**RECEIVED DATE** : 23-May-22





CERTIFICATE No : 22T4927

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : INCUBATOR  
MANUFACTURER : MEMMERT  
MODEL : IF 55  
ID No : TLC-L070  
RECEIVED DATE : 23-May-22  
AMBIENT TEMPERATURE : 21 °C ± 1 °C

S/N : D215.1343  
CALIBRATION DATE : 23-May-22  
RELATIVE HUMIDITY : 52 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	6635300	21T6765	10-Jul-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

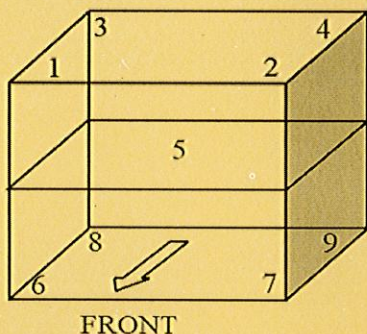

#### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 3
Overall Line Voltage (V) variation : 7
Instrument Condition : Normal
Chamber Size (W*L*H): 40*33*40 cm

#### CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
35.0	35.0	0.13	0.34	0.47
44.5	44.5	0.07	0.33	0.52

#### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
35.0	35.0	34.93	35.06	35.12	35.18	35.16	34.89	34.95	35.01	35.14	0.25
44.5	44.5	44.71	44.70	44.81	44.75	44.72	44.82	44.54	44.79	44.95	0.36

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 22T4934

REFERENCE No : 65110-5

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : AUTOCLAVE

**MANUFACTURER** : ZEALWAY

**MODEL** : GI54TW

**SERIAL No** : A515D096


**ID No** : TLC-L081

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : TOPS-LAB CONSULTANTS CO., LTD.  
189 MOO.3 BANGRAKPHATTHANA  
BANGBUATHONG NONTHABURI 11110

**CALIBRATED BY** : CHAICHARN CH.

**CALIBRATION DATE** : 23-May-22

**APPROVED BY** : 

**ISSUED DATE** : 23-May-22

**RECEIVED DATE** : 23-May-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02





CERTIFICATE No : 22T4934

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : AUTOCLAVE  
MANUFACTURER : ZEALWAY  
ID NUMBER : TLC-L081  
RECEIVED DATE : 23-May-22  
AMBIENT TEMPERATURE : 29° C ± 1° C

MODEL : GI54TW  
SERIAL NUMBER : A515D096  
CALIBRATION DATE : 23-May-22  
RELATIVE HUMIDITY : 57 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BASED ON BS 2646 : Part 5 : 1993 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON FIVE LOCATIONS AS SHOWN IN THE PICTURE. TWO PROBES WERE PLACES NEAR TOP AND BOTTOM WALL AND EACH PROBE WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE THIRD PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE INSTRUMENT CHAMBER. PROBE NUMBER 4 WAS ATTACHED TO THE LOAD TEMPERATURE PROBE, IF FITTED, WITHIN 20 mm OF ITS TIP. PROBE NUMBER 5 WAS PLACED IN THE CHAMBER DRAIN OR VENT WITHIN 100 mm OF ITS CONNECTION TO THE CHAMBER.

2. REFERENCE STANDARD INSTRUMENTS :-

#### INSTRUMENT

#### MODEL

#### SERIAL No

#### CERTIFICATE No

#### DUE DATE


1) DATA LOGGER WITH TC TYPE K HYDRA 2635A 6635300 21T6765 10-Jul-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

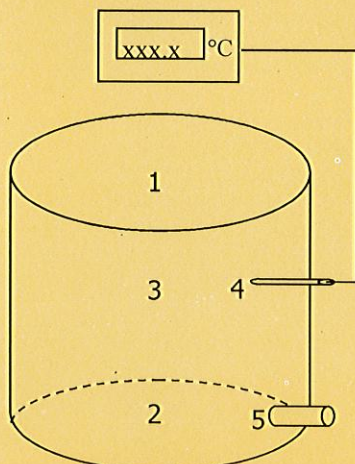

FRONT

#### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber variation : 0 °C

Autoclave Condition : Normal

Chamber Size (Diameter\*H): 32 \* 75 cm

#### CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)	Pressure (MPa)	Holding time (min)	Operating Cycle time (min)
121.0	121.0	0.1	0.2	0.3	0.12	15	60

#### TEMPERATURE MEASUREMENT ACCURACY TEST(° C)

Cont Temp	Ind Temp	Measured Temperature ( °C) at Spread Locations					Uncertainty (± °C)
		#1	#2	#3	#4	#5	
121.0	121.0	121.78	121.79	121.66	121.74	121.80	0.65

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT OF TEMPERATURE MEASUREMENT ACCURACY TEST EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : THE STABILITY TERM IN THE UNCERTAINTY BUDGET WAS REPLACED BY THE STANDARD REPEATABILITY.

NOTE 3 : LOCATION 3 WAS REFERENCE LOCATION.

NOTE 4 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 21T5672

REFERENCE No : 61414-5

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : AUTOCLAVE

**MANUFACTURER** : ZEALWAY

**MODEL** : GI54TW

**SERIAL No** : A515D096


**ID No** : TLC-L081

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : TOPS-LAB CONSULTANTS CO., LTD.  
189 MOO 3 BANGRAKPAITANA  
BANGBUATHONG NONTABURI 11110

**CALIBRATED BY** : CHAICHARN CH.

**CALIBRATION DATE** : 08-Jun-21

**APPROVED BY** : 

**ISSUED DATE** : 09-Jun-21

**RECEIVED DATE** : 08-Jun-21

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 21T5672

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : AUTOCLAVE  
MANUFACTURER : ZEALWAY  
ID NUMBER : TLC-L081  
RECEIVED DATE : 08-Jun-21  
AMBIENT TEMPERATURE : 25° C ± 1° C  
MODEL : GI54TW  
SERIAL NUMBER : A515D096  
CALIBRATION DATE : 08-Jun-21  
RELATIVE HUMIDITY : 50 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BASED ON BS 2646 : Part 5 : 1993 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON FIVE LOCATIONS AS SHOWN IN THE PICTURE. TWO PROBES WERE PLACES NEAR TOP AND BOTTOM WALL AND EACH PROBE WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE THIRD PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE INSTRUMENT CHAMBER. PROBE NUMBER 4 WAS ATTACHED TO THE LOAD TEMPERATURE PROBE, IF FITTED, WITHIN 20 mm OF ITS TIP. PROBE NUMBER 5 WAS PLACED IN THE CHAMBER DRAIN OR VENT WITHIN 100 mm OF ITS CONNECTION TO THE CHAMBER.
2. REFERENCE STANDARD INSTRUMENTS :-

#### INSTRUMENT

#### MODEL

#### SERIAL No

#### CERTIFICATE No

#### DUE DATE

1) DATA LOGGER

VALPROBE


S367, EV07, DW07

21T1320

28-Jan-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

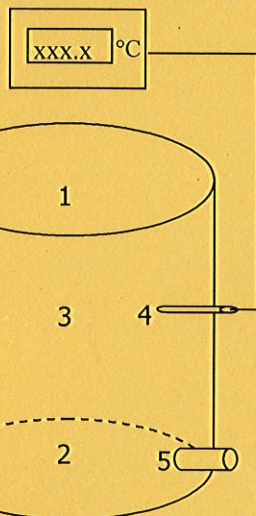

FRONT

#### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber variation : 0.3 °C

Autoclave Condition : Normal

Chamber Size (Diameter\*H): 32 \* 65 cm

#### CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)	Pressure (MPa)	Holding time (min)	Operating Cycle time (min)
121.0	121.0	0.05	0.11	0.18	0.11	15	60

#### TEMPERATURE MEASUREMENT ACCURACY TEST(° C)

Cont Temp	Ind Temp	Measured Temperature ( °C) at Spread Locations					Uncertainty (± °C)
		#1	#2	#3	#4	#5	
121.0	121.0	121.76	121.75	121.85	121.75	121.80	0.59

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT OF TEMPERATURE MEASUREMENT ACCURACY TEST EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : THE STABILITY TERM IN THE UNCERTAINTY BUDGET WAS REPLACED BY THE STANDARD REPEATABILITY.

NOTE 3: LOCATION 3 WAS REFERENCE LOCATION.

NOTE 4 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





RECALIBRATION

DUE DATE:

**April 13, 2022**

# Certificate of Calibration

## Calibration Certification Information

Cal. Date: April 13, 2021

Rootsmeter S/N: 438320

Ta: 295 °K

Operator: Jim Tisch

Pa: 753.1 mm Hg

Calibration Model #: TE-5025A

Calibrator S/N: **3092**

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.4380	3.3	2.00
2	3	4	1	1.0190	6.4	4.00
3	5	6	1	0.9090	8.0	5.00
4	7	8	1	0.8680	8.8	5.50
5	9	10	1	0.7150	12.9	8.00

## Data Tabulation

Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left( \frac{Ta}{Pa} \right)}$ (y-axis)
0.9966	0.6931	1.4149	0.9956	0.6924	0.8851
0.9925	0.9740	2.0010	0.9915	0.9730	1.2517
0.9904	1.0895	2.2372	0.9894	1.0884	1.3995
0.9893	1.1398	2.3464	0.9883	1.1386	1.4678
0.9839	1.3760	2.8299	0.9829	1.3746	1.7702
<b>QSTD</b>	m=	<b>2.07260</b>	<b>QA</b>	m=	<b>1.29783</b>
	b=	<b>-0.01963</b>		b=	<b>-0.01228</b>
	r=	<b>0.99999</b>		r=	<b>0.99999</b>

## Calculations

Vstd=	$\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$	Va=	$\Delta Vol((Pa-\Delta P)/Pa)$
Qstd=	$Vstd/\Delta Time$	Qa=	$Va/\Delta Time$
For subsequent flow rate calculations:			
Qstd=	$1/m \left( \left( \sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)} \right) - b \right)$	Qa=	$1/m \left( \left( \sqrt{\Delta H \left( \frac{Ta}{Pa} \right)} \right) - b \right)$

## Standard Conditions

Tstd: 298.15 °K

Pstd: 760 mm Hg

## Key

ΔH: calibrator manometer reading (in H2O)

ΔP: rootsmeter manometer reading (mm Hg)

Ta: actual absolute temperature (°K)

Pa: actual barometric pressure (mm Hg)

b: intercept

m: slope

## RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30





**National Institute of Metrology (Thailand)**  
Ministry of Higher Education, Science, Research and Innovation

## Certificate of Calibration

**Certificate No.** : MW-0045-22  
**Issued by** : Flow and Volume of Liquid Laboratory  
Mechanical Metrology Department

Page 1 of 3 pages

**MEASUREMENT ITEM** : Orifice Gas Flow Device

**MANUFACTURER** : Tisch Environmental, Inc.

**MODEL/TYPE** : TE-5025A

**SERIAL NUMBER** : 3092

**CUSTOMER** : TOPS-LAB Consultants Co.,Ltd  
189 Moo 3 Bangrakphattana Bangbuathong  
Nonthaburi 11110

**MEASUREMENT DATE** : April 28, 2022

*The reported measurement result relates only to the measurand and applies only at the time of measurement.*

**Reference:**  
MEC7199-01/22

**Date:**  
May 19, 2022

**Approved by:**



( Wirun Laopornpichayanuwat )

**Performed by:**



( Terdsak Neadkratoke )

*Partial reproduction of this certificate is permitted only with a written permission from NIMT.*





---

**ENVIRONMENTAL CONDITIONS:**

Ambient condition in the laboratory are as follows :

Temperature	: $23.0 \pm 2.0$	°C
Relative Humidity	: $55 \pm 15$	%RH

**Calibration Condition:**

Preconditioning	: 24 hours at ambient conditions.
Measurement Condition	: The average values during measurement are 21.5°C and 60 %RH.

**MEASUREMENT METHOD:**

The Orifice gas flow device was calibrated against NIMT's Standard Gas Meter Model DELTA S-Flow G65. The CP-MW 0009 was used as a calibration guideline.

**TABULATION OF RESULTS:**

The tables on the next page give the measured values.

**UNCERTAINTY OF MEASUREMENT:**

The stated uncertainty is the expanded uncertainty which is obtained by multiplying the standard uncertainty by the coverage factor  $k = 2$ . It has been determined in accordance with EA publication EA-4/02M:2013 "Evaluation of the Uncertainty of Measurement in Calibration" and "JCGM 100:2008 Evaluation of measurement data - Guide to the Expression of Uncertainty in Measurement (GUM 1995 with minor corrections)". The value of the measurand lies within the assigned range of values with a probability of 95 %.

**TRACEABILITY:**

This certificate provides a traceability of the measurement to recognized the national standards, and to the realization of the International System of Units (SI).



## MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Gas Meter standard. The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1. The results of  $Q$  actual calibration data

Plate	Flow rate m <sup>3</sup> /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	$\Delta p$ _Meter mmHg	$\Delta p$ _Orifice inH <sub>2</sub> O	Y	Actual Flow [ $Q_a$ ] m <sup>3</sup> /min
1	0.695	753.699	21.74	21.67	55.882	1.789	0.837	0.644
2	0.910	753.664	21.74	21.62	53.853	3.108	1.103	0.846
3	0.995	753.386	21.68	21.63	37.797	3.892	1.234	0.945
4	1.069	753.213	21.69	21.60	31.285	4.590	1.340	1.025
5	1.169	753.356	21.68	21.57	26.285	5.561	1.475	1.128

Slope ( $m$ ): **1.31990**

Intercept ( $b$ ): **-0.01327**

Correlation coefficient ( $r$ ): **0.99993**

Uncertainty ( $k=2$ ): **0.015** m<sup>3</sup>/min

Table 2. The results of  $Q$  standard calibration data

Plate	Flow rate m <sup>3</sup> /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	$\Delta p$ _Meter mmHg	$\Delta p$ _Orifice inH <sub>2</sub> O	Y	Standard Flow [ $Q_{std}$ ] m <sup>3</sup> /min
1	0.695	753.699	21.74	21.67	55.882	1.789	1.339	0.646
2	0.910	753.664	21.74	21.62	53.853	3.108	1.765	0.848
3	0.995	753.386	21.68	21.63	37.797	3.892	1.975	0.948
4	1.069	753.213	21.69	21.60	31.285	4.590	2.145	1.027
5	1.169	753.356	21.68	21.57	26.285	5.561	2.361	1.131

Slope ( $m$ ): **2.10732**

Intercept ( $b$ ): **-0.02123**

Correlation coefficient ( $r$ ): **0.99993**

Uncertainty ( $k=2$ ): **0.015** m<sup>3</sup>/min

End of Certificate of Calibration



# CERTIFICATE OF ANALYSIS

## Grade of Product: EPA Protocol

Part Number: E07NI99E15A0002  
Cylinder Number: EB0125123  
Laboratory: 124 - Durham (SAP) - NC  
PGVP Number: B22019  
Gas Code: APPVD

Reference Number: 122-401652592-1  
Cylinder Volume: 143.7 Cubic Feet  
Cylinder Pressure: 2016 PSIG  
Valve Outlet: 660  
Certification Date: Nov 06, 2019

Expiration Date: Nov 06, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

### ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	55.00 PPM	54.81 PPM	G1	+/- 0.9% NIST Traceable	10/29/2019, 11/06/2019
NITRIC OXIDE	55.00 PPM	54.80 PPM	G1	+/- 0.9% NIST Traceable	10/29/2019, 11/06/2019
SULFUR DIOXIDE	55.00 PPM	52.99 PPM	G1	+/- 1.0% NIST Traceable	10/29/2019, 11/06/2019
METHANE	180.0 PPM	172.9 PPM	G1	+/- 0.7% NIST Traceable	10/29/2019
PROPANE	180.0 PPM	178.5 PPM	G1	+/- 1.3% NIST Traceable	10/30/2019
CARBON DIOXIDE	950.0 PPM	958.7 PPM	G1	+/- 0.6% NIST Traceable	10/29/2019
CARBON MONOXIDE	4500 PPM	4469 PPM	G1	+/- 0.7% NIST Traceable	10/30/2019
NITROGEN	Balance				

### CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	16060657	CC465102	50.42 PPM NITRIC OXIDE/NITROGEN	+/- 0.8%	Jun 27, 2020
PRM	PRM	D562879	10.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.9%	Aug 17, 2018
NTRM	17060225	EB0079096	100.3 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Jul 23, 2023
RGM	12362	SG916305BAL	4.701% % PROPANE/NITROGEN	+/- 0.3%	Jun 04, 2020
GMIS	124206889114	CC322698	4.432 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.0%	Aug 15, 2021
NTRM	14010338	ND48595	49.08 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.9%	Apr 17, 2024
NTRM	12060910	CC356255	98.05 PPM METHANE/NITROGEN	+/- 0.6%	Dec 22, 2023
NTRM	10060806	CC317625	933.7 PPM CARBON DIOXIDE/NITROGEN	+/- 0.5	May 09, 2020
NTRM	080123	KAL004604	4857 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Jun 07, 2024
GMIS	124504060104	CC86856	4.8803 % PROPANE/NITROGEN	+/- 0.4%	Oct 22, 2023

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

### ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801549 CO2	FTIR	Oct 17, 2019
Horiba VIA510 CO RS2EGL6K	Nondispersive Infrared (NDIR)	Oct 30, 2019
Nicolet 6700 AHR0801549 CH4	FTIR	Oct 17, 2019
Nicolet 6700 AHR0801549 NO	FTIR	Oct 17, 2019
Nicolet 6700 AHR0801549 NO	FTIR	Oct 17, 2019
Varian 3800 C3H8	Gas Chromatograph	Oct 02, 2019
Nicolet 6700 AHR0801549 SO2	FTIR	Oct 17, 2019

Triad Data Available Upon Request

NOTES: GROSS WEIGHT: 28,750 g

NET WEIGHT: 4,327.9 g



Request No. 21-64/0289

MTC No. EEL. BP. 16/0264

## CALIBRATION CERTIFICATE

Submitted by : TOPS-LAB Consultants CO.,LTD.

Address : 189 Moo.3, Bang Bua Thong, Bangrak Phatthana, Nonthaburi 11110.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Calibrator

Manufacturer : QUEST

Model : QC-10

Serial No. : QIK100282

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
  2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
  3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
  4. Digital Multimeter Agilent 34401A S/N MY44005560.
  5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
  6. Audio Analyzer Keithley 2015-P S/N 4106495.
  7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

**Calibration Procedure:** CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 1 Feb. 2021

Date of Calibration : 4 Feb. 2021

1 / 2

The results relate only to the items tested or calibrated.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.3



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-64/0289

MTC No. EEL. BP. 16/0264

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 114 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0 °C and 50 %RH

### 1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	114.06	0.06	$\pm 0.10$	$\pm 0.40$ dB

### 2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	992.9	-7.1	$\pm 1.5$	$\pm 1.0\%$

### 3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	0.37	$\pm 0.50$	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :



Approved by :



Acting Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 4 Feb. 2021

Date of Issue : 8 Feb. 2021

Ref : 2011264020100427001

End of Certificate

2 / 2

The results relate only to the items tested or calibrated.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.3

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



Request No. 21-65/0284

MTC No. EEL. BP. 2/0265

## CALIBRATION CERTIFICATE

Submitted by : TOPS-LAB Consultants Co., Ltd.

Address : 189 Moo 3, Bang Bua Thong, Bangrak Phatthana, Nonthaburi 11110.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Calibrator

Manufacturer : 3M Quest Technologies

Model : QC-10

Serial No. : QIK100282

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Keithley 2015-P S/N 4106495.

7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

**Calibration Procedure:** CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 1 Feb. 2022

Date of Calibration : 8 Feb. 2022

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0284

MTC No. EEL. BP. 2/0265

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

**Nominal Output of Unit Under Test = 114 dB re 20 $\mu$ Pa at 1000 Hz**

**Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.**

**1. Sound Pressure Level**

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	114.09	0.09	$\pm 0.10$	$\pm 0.40$ dB

**2. Frequency**

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	992.6	-7.4	$\pm 1.5$	$\pm 1.0\%$

**3. Total Distortion**

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	0.37	$\pm 0.50$	$\pm 3.0\%$

- Note :**
1. No adjustment.
  2. The calibrator pressure correction was not included.
  3. The microphone volume correction was not included.

Calibrated by :

.....  
[Redacted Signature]

Approved by :

.....  
[Redacted Signature]

Director

**Electrical and Electronic Standards Laboratory  
Industrial Metrology and Testing Service Centre**

**Date of Calibration** : 8 Feb. 2022

**Date of Issue** : 9 Feb. 2022

Ref : 2011265020100419001

2 / 2

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4



# Calibration Certificate

Part Number: 721A2601

Description: Micromate with DIN Geophone

Serial Number: UM19250

Calibration Date: NOV 30 2021

Calibration Reference Equipment: 714J7402


*Instantel certifies that the above product was calibrated in accordance with the applicable Instantel procedures. These procedures are part of a quality system that is designed to assure that the product listed above meets or exceeds Instantel specifications.*

*Instantel further certifies that the measurement instruments used during the calibration of this product are traceable to the National Institute of Standards and Technology; or National Research Council of Canada. Evidence of traceability is on file at Instantel and is available upon request.*

*The environment in which this product was calibrated is maintained within the operating specifications of the instrument.*

*Please note that the sensor check function is intended to check that the sensors are connected to the unit, installed in the proper orientation and sufficiently level to operate properly. This function should not be confused with a formal calibration, which requires the sensors be checked against a reference that is traceable to a known standard. Instantel recommends that products be returned to Instantel or an authorized service and calibration facility for annual calibration.*

Calibrated By: \_\_\_\_\_

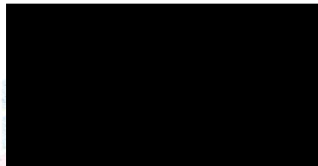

309 Legget Drive, Ottawa, Ontario, K2K 3A3, (613) 592-4642



# Frequency Response of UM19250

