
เอกสารสอบเทียบเครื่องมือที่ใช้ในการวิเคราะห์

CERTIFICATE OF CALIBRATION

Certificate No.: CO-2008004/21 Page 1 of total 4 pages

Customer
WATER ANALYSIS CENTER CO., LTD.
30/5 Soi Vipavadee 60, Vipavadee Rangsit Road,
Kwaeng Taladbangkhen, Khet Laksi, Bangkok 10210

Equipment
pH Meter
Manufacturer
METTLER TOLEDO
Model
B327527211
ID No.
SevenCompact
WWL 0068
Description
Range : 0 - 14 pH, Resolution : 0.01 pH

Environmental Conditions
Ambient Temperature: (20 ± 2) °C
Relative Humidity: (50 ± 10) %
Atmospheric Pressure: -

Calibration Location
Jayhawks Laboratory (CL&GL)
Received Date
20 August 2021
Calibration Date
20 August 2021

Date of Issue
23 August 2021

Checked by

Approved

() (Krisyosl K.) () (Sakda Y.)
() (Patiphan K.) () (Onnapa P.)
() (Pongsak H.) () (Nitiphong K.)
() (Kanung C.) () (Nonthachai K.)
() (Pramong P.) () (Noppol P.)

This calibration certificate shall not be reproduced other than in full except with the prior written approval of the Thai Heart Calibration Co., Ltd.

FE-169

REV.02.02/24/21

Certificate No.: CO-2008004/21 Page 2 of total 4 pages

Reference Method:

- The calibration method used was CP-178 based on an in-house method.
- This certificate can be traceable to the national standards, which is realized the shown measurement units according to the International System of Units (SI Units).

Reference Standard:

Type	pH Value	Lot No.	Due Date	Traceability
pH Standard Solution	4.01	081020	Feb. 1, 2022	NIMT
	7.01	020221	Dec. 25, 2021	
	10.00	091020	Jan. 19, 2022	

Type	Model	Serial No.	Certificate No.	Due Date	Traceability
Documenting Process Calibrator	753	3101007	10-0804001/21	Apr. 7, 2022	THC
Digital Thermometer with Sensor	1523 / 5622	1709138 / 4605984-005	10-1006001/21	Jun. 10, 2022	

Remark: This certificate is traceable to the International System of Unit (SI Unit) through:

- NIMT, National Institute of Metrology (Thailand).
- THC, Thai Heart Calibration Co., Ltd.

Measurement Results:

1. Function Simulated pH Meter

Standard Applied (mV)	Nominal Value (pH)	UUC Reading		Uncertainty (± mV)
		pH	mV	
177.48	4.00	4.01	177.4	0.060
0.00	7.00	7.00	0.0	0.060
-177.48	10.00	10.01	-177.4	0.060

UUC : Unit Under Calibration

Note : Adjust Curve to simulate pH (4,7,10)

Calibrated by

Kitipong
REV.02.02/24/21

FE-169

Certificate No.: C0-2008004/21

Page 3 of total 4 pages

Measurement Results (Cont.):

2. Calibration of pH Electrode

pH Standard Solution (pH)	Measured Value		Uncertainty (± pH)
	(pH)	(mV)	
4.01	4.00	187.0	0.013
7.01	7.00	11.1	0.013
10.00	10.02	-161.6	0.013

Note : Adjust Curve to Buffer Solution pH (4.7,10)

Temperature stability of micro bath : $25 \pm 0.2^{\circ}\text{C}$

The above reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

Certificate No.: C0-2008004/21

Page 4 of total 4 pages

Reference Method:

- The calibration method used was CP-096 based on an in-house method.

- The temperature scale used was an ITS-90.

- This certificate can be traceable to the national standards, which is realized the shown measurement units according to the International System of Units (SI Units).

Reference Standard Instruments:

Type	Model	Serial No.	Cert. No.	Due Date	Traceability
Thermometer Readout	1529-R	B7C853	20E3985	Nov. 9, 2021	TPA
Platinum Resistance Thermometer	5626	4853	C0A30046	Oct. 28, 2023	FLUKE
Liquid Bath	XORTS-40A	XO111019	IO-0306002/21	Jun. 3, 2023	THC

Remark: This certificate is traceable to the International System of Unit (SI Unit) through:

- TPA, Technology Promotion Association (Thailand-Japan).
- FLUKE, Fluke Corporation, U.S.A.
- THC, Thai Heart Calibration Co., Ltd.

Measurement Results:

(X) Without Adjustment

Dimension of probe : Diameter 4 mm. Sensor Type : RTD (PT100)

Immersion Depth (mm.)	Standard Reading ($^{\circ}\text{C}$)	UUC Reading ($^{\circ}\text{C}$)	Correction ($^{\circ}\text{C}$)	Uncertainty ($\pm ^{\circ}\text{C}$)
120	22.00	22.0	0.00	0.058
120	25.00	25.0	0.00	0.058
120	28.00	28.0	0.00	0.058

UUC : Unit Under Calibration

The above reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



THAI HEART CALIBRATION CO., LTD.
112/1 Moo 5, Phrak Sai, Muang, Samut Prakan 10280
Tel. 0-2394-2162, 0-2757-8435, 0-2757-8496 Fax. 0-2757-8507



CERTIFICATE OF CALIBRATION

Certificate No.: C0-2107005/21 Page 1 of total 2 pages

Customer
WATER ANALYSIS CENTER CO., LTD.
30/5 Soi Viphavadee 60, Viphavadee Rangsit Road,
Kwaeng Taladbangkhen, Khet Laksi, Bangkok 10210

Equipment Conductivity Meter
Manufacturer EUTECH **Model** CON 2700
Serial No. 2657889 **ID No.** WWL 0136
Description -

Environmental Conditions Ambient Temperature: $(20 \pm 2) ^\circ\text{C}$
Relative Humidity: $(50 \pm 10) \%$
Atmospheric Pressure: -

Calibration Location Jayhawks Laboratory (CL&GL)
Received Date 21 July 2021
Calibration Date 21 July 2021

Date of Issue 22 July 2021

Checked by

Approved by

() (Krisyosl K.) () (Sakda Y.)
() (Patiphan K.) () (Ommapa P.)
() (Pongsak H.) () (Niriphong K.)
() (Kanung C.) () (Nonthachai K.)
() (Pramong P.) () (Noppol P.)

This calibration certificate shall not be reproduced other than in full except with the prior written approval of the Thai Heart Calibration Co., Ltd.

FE-169

REV.02 02/24/21

929/929/1 Soi Pattanakarn 30, Pattanakarn Rd., Suanluang, Bangkok 10250
Head Office : Tel. 02-319-9994 ext.1 Fax.02-319-4961 E-mail : ats@automation.co.th
Rayong Branch : 1/15 Huaypong Rd., A. Muang, Rayong 21150 Tel. 038-692-152 Fax. 038-692-345
Lamphun Branch : 122/5 M.4, T.Ban Klang, A.Muang, Lamphun 51000 Tel/Fax. 053-581-876
website : www.automation.co.th

SV 212001/2021

Cert. No. WAC-065
Page 1 of 2

CERTIFICATE OF CALIBRATION

Instrument : DO Meter
Model : DO-31P
Serial No. : 780065
Manufacturer : TOA-DKK
Measuring Range : 0.00 ~ 20.00 mg/l
Customer : Water Analysis Center Co.,Ltd.
1/94 Moo.5 T.Kanham, A.U.-Thai
Ayutthaya 13210 Thailand

Machine : -
Location : -

Date Of Received : 03 / 12 / 2021
Date Of Calibration : 03 / 12 / 2021

Ambient Condition : Temperature 24 °C
Humidity 47 % RH

Calibrated By :

Approved By :

Date Of Issue : 03 / 12 / 2021

This Certificate may not be reproduced other than in full, except with the prior written approval of the head of the industrial instruments calibration center.

Instrument : DO Meter
Model : DO-31P
Serial No. : 780065

Cert. No. WAC-065
Page 2 of 2

Calibrate Procedure

- ☐ This instrument was calibrated by comparison with standard solution (PH/ORP)
- ☐ This instrument was calibrated by comparison with scattering plate value (Turbidity)
- ☐ This instrument was calibrated by comparison with conductivity (Conductivity)
- ☒ This instrument was calibrated by comparison with Sodium sulfite anhydrous (DO)

Condition of this result of calibration

1). Reference Standard Solution

Standard Lot No Batch Cert. No. Due Date

Sodium Sulfite Power 1.06657.0500 K52300357 - 31 Mar 2022

2). Traceability This certification is traceable to

- ☒ Merck KGaA 64271 Darmstadt
- ☐ DKK Corporation


Result Of Calibration

Standard Solution (mg/l) at 26.0°C	Before Adjust		After Adjust	
	Indicator	Error	Indicator	Error
Zero	0.00	+ 0.10	0.00	-
Span	7.99	+ 0.22	7.99	-

DO Electrode No. OE270AA(5) S/N 111F0029

Certificate of Calibration

TEMPERATURE CONTROLLER ENCLOSURES



Certificate No.: MC 2107214

Page 1 of 3

Customer : Water Analysis Center Co., Ltd.
1/94 Moo 5, T. Kantham, A.U.-Thai, Ayutthaya 13210.

Reference Job No. : 21-1565 Received Date : 13 July 2021

Description : Refrigerator

Manufacturer : SANDEN/TERCOOL Model : SEC-1500SBD

Serial No. : SEC1500201A-0708-00304 ID. No. : WWL0038

Marking : Additionally for the purpose of identification by this laboratory a label marked with this certificate number (MC 2107214) has been attached to the case.

Method : In-House calibration procedure MWI-T-033 this method is reference to TLAS G-20 "Temperature Controlled Enclosures".

Location of Calibration : Water Analysis Center Co., Ltd. : Laboratory.

Environmental Conditions : Ambient Temperature : (26.3) °C
Relative Humidity : (56.4 to 59.3) %

Date of Calibration : 13 July 2021 Date of Issue : 14 July 2021

Checked by :

Approved by :

The uncertainties are for a confidence probability of approximately 95%

This certificate is issued in accordance with the conditions of accreditation granted by the National Standardization Council of Thailand-Office of the National Standardization Council that has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of Master Calibration Co., Ltd.

[MCF-Q-077 ; Rev.6 ; Date : 22/04/2021]

Certificate No.: MC 2107214

Page 2 of 3

The Reference Standard :

Description	Certificate No.	Serial No.	Due date
Data Acquisition/Switch Unit	MC 2009600	MY44095818	8 August 2021
With Thermocouple Type "T" ID. No.6/1 to 6/9			

This certificate is traceable to the international system of units maintained at:

- Master Calibration Co., Ltd. And Quality Reborn Co., Ltd.

1. Calibration Procedure:

This Instrument was calibration according to TLAS G-20 by comparison with calibrated thermocouple type T under no load condition. The Thermocouples were placed on nine points and located one thermocouple in each of the eight corners of the chamber and was away from the each wall of 5 cm to 10 cm. And placed the ninth thermocouple within 2.5 cm of the geometric center of the chamber.

Temperature Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.

Temperature Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.

Overall Variation - The Difference of the maximum and minimum measured temperatures throughout observation.

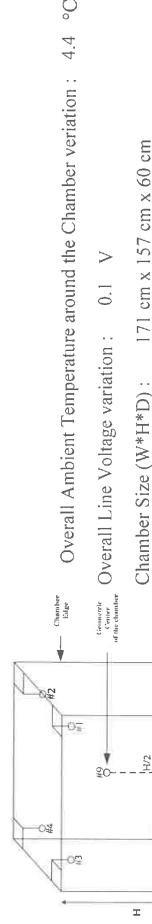


Figure 1 : Sensor Installation Location

[MCF-Q-077 ; Rev.6 ; Date : 22/04/2021]

Certificate No.: MC 2107214

Page 3 of 3

2. Result of calibration :

Temperature Measurement Accuracy Test

Indicating Temperature (°C)	Measured Temperature (°C) at Spread Locations								Uncertainty (±°C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. #9
2.6	4.0	4.0	4.1	4.0	3.9	3.8	3.7	3.8	3.4
									1.2

Chamber Characterization Result

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
2.0	2.6	2.7	1.4	5.8

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

This report will certify of the calibrated equipment only.

End of Certificate

TEMPERATURE CONTROLLER ENCLOSURES

Report No. : MC 2103787

Page 1 of 3



Customer : Water Analysis Center Co., Ltd.
1/94 Moo 5, T.Kantham, A.U-Thai, Ayutthaya 13210.

Reference Job No. : 21-0710 Received Date : 25 March 2021

Description : Oven

Manufacturer : Memmert Model : UF260

Serial No. : B620.0814 ID. No. : N/A

Marking : Additionally for the purpose of identification by this laboratory a label marked with this report number (MC 2103787) has been attached to the case.

Method : In-House calibration procedure MWI-T-033 this method is reference to TLAS G-20 "Temperature Controlled Enclosures".

Location of Calibration : Water Analysis Center Co., Ltd. ; Laboratory.

Environmental Conditions : Ambient Temperature : (31.8 to 35.3) °C

Relative Humidity : (44.7 to 55.9) %

Date of Calibration : 25 March 2021 Date of Issue : 26 March 2021

Checked by :

Approved by :

The uncertainties are for a confidence probability of approximately 95%

This certificate is issued in accordance with the condition of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full expect with the prior written approval of the issuing laboratory.

Continuation of Report No. : MC 2103787

Page 2 of 3

The Reference Standard :

Description	Report No.	Serial No.	Due date
Data Acquisition/Switch Unit	MC 2016027	MY41010916	10 January 2022
With Thermocouple Type " T " ID. No.17/1 to 17/9			

This certificate is traceable to the international system of units maintained at:

- Master Calibration Co., Ltd.

1. Calibration Procedure:

This Instrument was calibration according to TLAS G-20 by comparison with calibrated thermocouple type T under no load condition. The Thermocouples were placed on nine points and located one thermocouple in each of the eight corners of the chamber and was away from the each wall of 5 cm to 10 cm. And placed the ninth thermocouple within 2.5 cm of the geometric center of the chamber.

Temperature Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.

Temperature Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.

Overall Variation - The Difference of the maximum and minimum measured temperatures throughout observation.

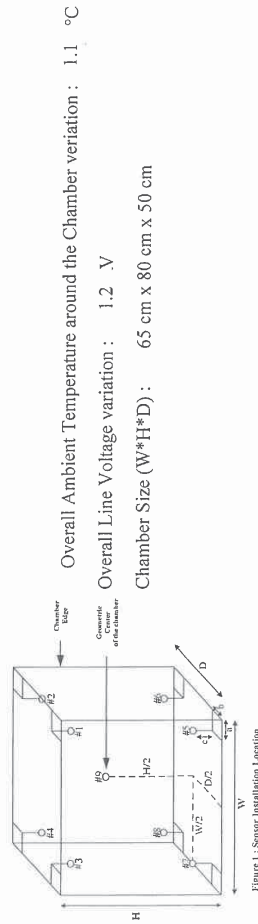


Figure 1 : Sensor Installation Location

Continuation of Report No. : MC 2103787

Page 3 of 3

2. Result of calibration :

Temperature Measurement Accuracy Test

Indicating Temperature (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (±°C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. #9	
104.0	103.7	103.7	103.7	103.9	104.2	104.3	104.3	104.3	104.0	0.67
180.0	179.1	179.1	179.0	179.2	180.4	180.5	180.6	180.6	180.2	0.99

Chamber Characterization Result

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.0	0.27	0.44	1.0
180.0	180.0	0.29	1.31	1.9


3. Uncertainty of Measurement

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

This report will certify of the calibrated equipment only.

End of Calibration Report

Calibration Report



TEMPERATURE CONTROLLER ENCLOSURES

Report No. : MC 2103787

Page 1 of 3

Customer : Water Analysis Center Co., Ltd.
1/94 Moo 5, T.Kantham, A.U.-Thai, Ayutthaya 13210.

Reference Job No. : 21-0710 Received Date : 25 March 2021
Description : Oven
Manufacturer : Memmert Model : UF260
Serial No. : B620.0814 ID. No. : N/A
Marking : Additionally for the purpose of identification by this laboratory a label marked with this report number (MC 2103787) has been attached to the case.

Method : In-House calibration procedure MWI-T-033 this method is reference to

TLAS G-20 "Temperature Controlled Enclosures".

Location of Calibration : Water Analysis Center Co., Ltd. ; Laboratory.

Environmental Conditions : Ambient Temperature : (31.8 to 35.3) °C

Relative Humidity : (44.7 to 55.9) %

Date of Calibration : 25 March 2021 Date of Issue : 26 March 2021

Checked by :

Approved by :

The uncertainties are for a confidence probability of approximately 95%

This certificate is issued in accordance with the condition of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full expect with the prior written approval of the issuing laboratory.

Continuation of Report No. : MC 2103787

Page 2 of 3

The Reference Standard :

Description : Report No. : Due date
Data Acquisition/Switch Unit MC 2016027 MY41010916 10 January 2022
With Thermocouple Type " T " ID. No.17/1 to 17/9

This certificate is traceable to the international system of units maintained at:

- Master Calibration Co., Ltd.

1. Calibration Procedure:

This Instrument was calibration according to TLAS G-20 by comparison with calibrated thermocouple type T under no load condition. The Thermocouples were placed on nine points and located one thermocouple in each of the eight corners of the chamber and was away from the each wall of 5 cm to 10 cm. And placed the ninth thermocouple within 2.5 cm of the geometric center of the chamber.

Temperature Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.

Temperature Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.

Overall Variation - The Difference of the maximum and minimum measured temperatures throughout observation.

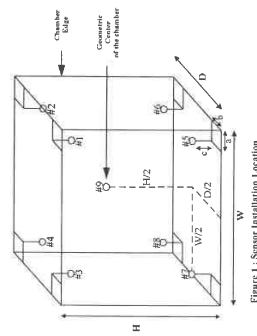


Figure 1 : Sensor Installation Location

Overall Ambient Temperature around the Chamber variation : 1.1 °C
Overall Line Voltage variation : 1.2 V
Chamber Size (W*H*D) : 65 cm x 80 cm x 50 cm

2. Result of calibration :

Temperature Measurement Accuracy Test

Indicating Temperature	Measured Temperature (°C) at Spread Locations									Uncertainty (±°C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. #9	
104.0	103.7	103.7	103.7	103.9	104.2	104.3	104.3	104.3	104.0	0.67
180.0	179.1	179.1	179.0	179.2	180.4	180.5	180.6	180.6	180.2	0.99

Chamber Characterization Result


Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.0	0.27	0.44	1.0
180.0	180.0	0.29	1.31	1.9

3. Uncertainty of Measurement

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

This report will certify of the calibrated equipment only.

End of Calibration Report



Certificate of Calibration

Equipment:	Balance	Certificate No.:	C01211841
Model:	BL210S	Issued Date:	24 June 2021
Serial No. (or ID.):	15808131 (WWL 0022)	Job No.:	KSPR2107969
Manufacturer:	Sartorius	Page:	1 of 2
Condition:	In condition		

Customer: Water Analysis Center Co., Ltd.
1/94 Moo 5, Rojana Industrial Park, Rojana Road,
Tambol Kanham, Amphur U-Thai, Ayutthaya 13210 Thailand

Environment Condition: Temperature 27 °C ± 0.3 °C
Humidity 40 %RH ± 1.7 %RH

Calibration Place: Water Analysis Center Co., Ltd. (องค์การน้ำ)
1/94 Moo 5, Rojana Industrial Park, Rojana Road,
Tambol Kanham, Amphur U-Thai, Ayutthaya 13210 Thailand

Calibration By: Mr. Phakapol Donmin

Calibration Date: 10 June 2021

The Method used: In house method, SPCC-WI47, base on UKAS Lab 14

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through SPC RT Co., Ltd. Certificate No. C02210017

Person in charge

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SPC RT Co., Ltd.

บริษัท เอสพีซี อาร์ที จำกัด
SPC RT CO., LTD.

SPECIFIC RT CO., LTD.
เลขประจำตัวประชาชน 00003
เลขที่ทางไปรษณีย์ 101/1 แขวงปทุมวัน เขตปทุมธานี กรุงเทพมหานคร 10260
ถนนสุขุมวิท 57, Sukhumvit 101/1 Road, Bangkok, Phrakhanong, Bangkok 10260 Thailand
โทรศัพท์ : 0 2185 4433 Ext. 3300-3308 Fax : 0 2185 4424 E-mail : info.spc@spec-ri.com Website : www.spc.com

[MCF-Q-077 ; Rev.5 ; Date : 15/07/2014]

SPCC-FM-C01-10: 23 Nov 2020

Calibration Results:

Without Adjustment

Eccentric Error: Weight to be 1/4 or 1/3 of Maximum capacity, taken from the center of the pan as a zero reference.

	Nominal Test Value			Reference Points (g)		
	A	B	C	D	E	
	-	0.0000	-0.0001	-0.0001	0.0000	0.0000


Repeatability: Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
20	0.00004
200	0.00005

Departure of indication from nominal value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Correction of Balance (g)	Uncertainty (g)	k
1	1.00001	1.0000	0.0000	0.00010	2.03
2	2.00002	2.0000	0.0000	0.00010	2.03
5	4.99999	5.0000	0.0000	0.00010	2.03
10	10.00000	10.0000	0.0000	0.00011	2.02
20	19.99999	20.0000	0.0000	0.00011	2.02
50	49.99997	50.0000	0.0000	0.00012	2.01
70	69.99996	70.0000	0.0000	0.00015	2.00
100	100.00000	100.0000	0.0000	0.00017	2.00
120	119.99999	120.0001	-0.0001	0.00021	2.00
150	149.99997	150.0000	0.0000	0.00023	2.00
200	199.99990	200.0003	-0.0004	0.00029	2.00

The End of Certificate

**Bara Scientific**
SPECIALIST OF CALIBRATION**Bara Scientific Co., Ltd.**
988 U Chu Liang Building Floor7 Rama4 Road
Siam Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com

Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No. BSCC-UV-135/21
Equipment UV/Vis Spectrophotometer
Model UV-1800
Manufacturer SHIMADZU
Serial No. A11635405598CD
ID No. WWL0082
Date of receipt 30 April 2021
Date of calibration 30 April 2021
Date of issue 10 May 2021

Customer name Water Analysis Center Co., Ltd.
Address 1/94 Moo 5, T. Kantham, A. Uthai, Ayuthaya 13210

Temperature (29.9-32.1) °C (On site)
Humidity (48.7-52.6) %RH (On site)

Equipment condition Good Operation

Calibration Location Laboratory Room Water Analysis Center

Calibration Procedure In-house method WI-UV-702-01 based on ASTM E275-01

Traceability Wavelength Accuracy is traceable to certificate No. 79670 and 79671
Photometric Accuracy is traceable to certificate No. 79672 and 79673
Stray Light is traceable to certificate No. 79669
The above certificate are traceable to SI unit through Stama Scientific Ltd.
(UKAS accredited calibration laboratory NO. 0659)

Calibrated by Mr. Waruth Janphung



The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Sliom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Certificate No.

BSCC-UV-135/Z1

Number of Page(s)

2 of 3

Calibration Results:

1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
360.89	360.82	-0.07	0.18
418.53	418.71	0.18	0.18
445.82	446.38	0.56	0.18
453.67	453.58	-0.09	0.18
459.99	459.80	-0.19	0.18
638.00	638.10	0.10	0.18
431.22	431.38	0.16	0.18
513.39	513.57	0.18	0.18
528.82	528.90	-0.08	0.18
572.99	572.58	-0.41	0.18
585.25	585.37	0.12	0.18
684.50	684.65	0.15	0.18
741.02	741.14	0.12	0.18
879.41	879.29	-0.12	0.18

2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	CNR	CNR	CNR	CNR
257	CNR	CNR	CNR	CNR
313	CNR	CNR	CNR	CNR
350	0.0000	0.0000	0.0000	0.0075
	0.6358	0.6310	-0.0048	0.0075

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Sliom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Certificate No.

BSCC-UV-135/Z1

Number of Page(s)

3 of 3

Calibration Results:

3.Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5473	0.5511	0.0038	0.0042
	0.7625	0.7655	0.0030	0.0042
	1.0484	1.0525	0.0041	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5369	0.5401	0.0032	0.0042
	0.7446	0.7464	0.0018	0.0042
	1.0235	1.0259	0.0024	0.0042
465.0	0.0000	0.0000	0.0000	0.0042
	0.4873	0.4906	0.0033	0.0042
	0.6868	0.6882	0.0014	0.0042
	0.9433	0.9453	0.0020	0.0042
546.1	0.0000	0.0000	0.0000	0.0042
	0.5009	0.5027	0.0018	0.0042
	0.6952	0.6950	-0.0002	0.0042
	0.9568	0.9556	-0.0012	0.0042
590.0	0.0000	0.0000	0.0000	0.0042
	0.5292	0.5303	0.0011	0.0042
	0.7228	0.7218	-0.0010	0.0042
	0.9893	0.9874	-0.0019	0.0042
635.0	0.0000	0.0000	0.0000	0.0042
	0.5140	0.5151	0.0011	0.0042
	0.6902	0.6889	-0.0013	0.0042
	0.9539	0.9519	-0.0020	0.0042

*CNR = Customer not request

4.Stray Light*

Standard cut-off wavelength (nm)	Wavelength (nm)	Transmission (%T)	Absorbance (A)
200.97±0.11nm	200.40	0.9524	2.0215

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

End of Certificate

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประจักษ์ไพบูลย์ แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200
80-82 Prachathipatai Rd., Bangkokphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

PREVENTATIVE MAINTENANCE (PM) CHECK LIST
FOR ATOMIC ABSORPTION SPECTROMETER

Model & Serial Number: 240FS AA & MY18290004

Customer: Water Analysis Center Co., Ltd

Date: 7 Apr 2021

Safety

- ☒ Flame, Inspect/replace o-ring nebulizer, spray chamber and burner
- ☒ Flame, Clean nebulizer, spray chamber and burner
- ☒ Flame, Check liquid trap interlock, burner interlock, pressure relief/bung interlock and shield interlock

☐ Furnace, Clean work head, electrode and shroud N/A

☐ Furnace, Clean PSD and PSD tray N/A

☐ Furnace, Check water pressure N/A

☒ Check drain tube

☒ Check exhaust system

☒ Check gas pressure sensor interlock

☒ Check and all gas hoses for SpectrAA

☒ Clean computer control

Optics

☒ Inspect/Replace that external optics surfaces

☒ Check Wavelength Accuracy the copper line at 323.0-326.0 nm = 324.6 nm

☒ Check that PMT % Gain the copper at 324.8 nm, 4 mA, 0.5 nm slit width, Gain = 33.7 % (should be $\leq 64\%$ or $\leq 380V$)

☒ Flame, Check D2 lamp is work



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประจักษ์ไพบูลย์ แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200
80-82 Prachathipatai Rd., Bangkokphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Electronics

- ☒ Check power supply voltage
- ☒ Check cables and connectors
- ☒ Check/Clean all boards in the instrument
- ☐ Furnace, Check camera and align** N/A

**Option for Graphite Zeeman only

Mechanisms

- ☒ Flame, Check the burner adjuster
- ☐ Furnace, Check PSD accessories N/A

Analytical performance

☒ Clear the sample compartment

☒ Flame, Check uptake rate form 7.2-10.6 mL per minute = 10.4 mL/min

☒ Test Photometric noise, STDV = 0.0002 Abs (should be ≤ 0.00050 Abs)

☒ Flame, Test high solids nebulizer setting use

-Air/acet Cu 5 ppm = 0.76 Abs, and Precision (%RSD)= 0.5 % (should be > 0.55 Abs and $< 0.5\%$ RSD)

or

-N2O/Acet Cu 5 ppm = _____ Abs, and Precision

(%RSD)= _____ % (should be > 0.3 Abs and $< 0.5\%$ RSD)

☐ Furnace, Characteristic mass and sensitivity Cu 25 ppb = _____ Abs, and N/A

Precision (%RSD)= _____ % (should be ≥ 0.15 Abs and $\leq 4.0\%$ RSD)

SIGN :

Engi

Custom

SVD Results Report

1

SVD

VARIAN

Report ID:4

Diagnostic Start Time:4/7/2021 11:21:56 AM

Diagnostic End Time:4/7/2021 12:04:17 PM

Customer: Water Analysis Center Co., Ltd.

Service Engineer: Suriya Nacharoen

Address: Uthai Ayuthraya

Contact Details: Kanitsara

Instrument Configuration

Configuration:

Serial Number: MY18230004

Turret Type: Automatic

Instrument Model: Varian AA140/240/280

Number Of Lamps: 4

Flame Instrument: True

Mono Type: Automatic

Furnace Instrument: True

Gasbox Type: 'Y' Gas Box

Zeeman Present: False

Auto Burner Adjuster: False

Internal Zeeman: False

Mains Frequency: 50

Internal UltraAA: False

Firmware Version: 2.12

Optics Type: Double Beam

Photomultiplier Type: Normal(900nm)

D2 BG Correction Fitted: True

PWB Version: 181

Boot Block Version: 2.02

EEPROM Data:

Instrument Run Hours: 16347.950

D2 Run Hours: 4626.033

Zero Wavelength Offset: 25.877

D2 Serial Number: not set !

Mono Correction: -0.605

D2 Install Date: 1/1/1970

Flame Hours: 5461.417

D2 Original Intensity: 1.000

D2 Last Intensity: 400.000

Frequency:

Averaging Period: 30.0

Datapoint Count: 20

Upper Limit:
51.00

Lower Limit:
49.00

Average Frequency:
50.00

Highest Measured Frequency:
50.00

Lowest Measured Frequency:
50.00

Result: Passed

Power Supply:

Averaging Period: 30.0

Datapoint Count: 20


	Lower Limit (V)	Actual (V)	Upper Limit (V)	Result:
12.00V Rail	10.80	12.10	13.20	Passed
-12.00V Rail	-13.20	-11.90	-10.80	Passed
5.00V Rail	4.50	5.00	5.50	Passed
310.00V Rail	279.00	318.00	341.00	Passed

Beam Balance:


Lamp Type: Copper
Lamp Socket Used: 3

Peak Selected: 324.80
Lamp Alignment: Performed

'X' Lamp Screw

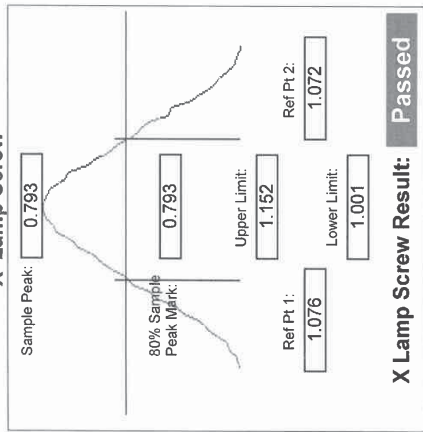

'Y' Lamp Screw

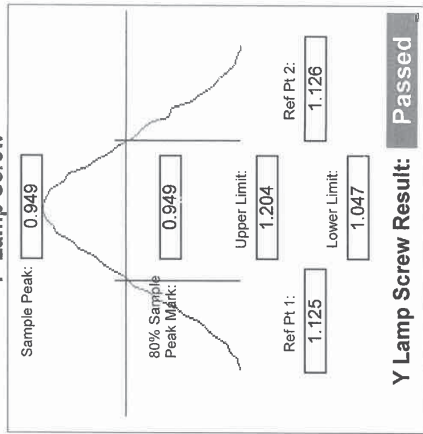

Grating Squareness:

Lamp Element(s): Copper
Lamp Turret Position: 3
Lamp Current(mA): 4.00
Slit Width(nm): 0.5
1st Order Wavelength(nm): 324.80
Lamp Alignment: Performed

	Lower Limit (nm)	Actual (nm)	Upper Limit (nm)	Result:
Zero Order	-0.10	0.00	0.10	Passed
First Order	324.45	324.62	325.15	Passed
Second Order	649.23	649.54	649.97	Passed

Wavelength Repeatability:

Lamp Used: Copper
Peak Used(nm): 324.750
Connected to Socket: 3
Lamp Current(mA): 4
Slit Width(nm): 0.2
Slit Height: Normal

Lamp Alignment: Performed

Lower Limit(nm)	324.551	324.671	Upper Limit(nm)
(Approach from Zero Order)			
Sample 1:	324.611		Sample 2: 324.611
Sample 3:	324.611		Sample 4: 324.611
Sample 5:	324.615		Sample 6: 324.611
Sample 7:	324.615		Sample 8: 324.611
Sample 9:	324.615		Sample 10: 324.611

Mean: 324.613
Standard Deviation: 0.002

Result: Passed

Mechanical

Wavelength Drive: Passed

Slit Drive: Passed

Turret Drive: Passed

Auto Burner Adjuster Drive: Untested

Miscellaneous

Signal Processing Linearity:

Calculate Mode: New Calc Mode				
	Lower Limit	Actual	Upper Limit	Result:
S0	114	258	297	Passed
S1	156	166	191	Passed
S2	271	300	332	Passed
S3	474	516	579	Passed
S4	825	933	1008	Passed
S5	1435	1555	1754	Passed
S6	2498	2802	3053	Passed
S7	4347	4795	5313	Passed

Interlocks:

Burner Fitted: Working

N2O Burner Fitted: Working

Flame Shield Closed: Working

Gas Control Fitted: Untested

Pressure Release Bung Fitted: Working

Liquid Trap Fitted: Working

Flame Detect: Working

GCU Active: Working

Oxidant Pressure: Working

Oxidant Changeover: Working

Ignition: Working

Auto Lamp Recognition:

Lamp 1: 42 - Potassium (K) Lamp 5: Not Supported

Lamp 2: 53 - Sodium (Na) Lamp 6: Not Supported

Lamp 3: 14 - Copper (Cu) Lamp 7: Not Supported

Lamp 4: 37 - Nickel (Ni) Lamp 8: Not Supported

Result: Passed

GTA Temperature Monitoring:

Not Performed

Notes:

C2104SU29 PM 1/2

Signatures:

Water Analysis Center Co., LtdDate Suriya Nacharoen Date



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาวิทย์ แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200
80-82 Prachathipatai Rd., Bangkokunphrom, Pranakorn, Bangkok 10200
Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawati@thaiunique.com, Website : www.thaiunique.com

PREVENTATIVE MAINTENANCE (PM) CHECK LIST FOR ATOMIC ABSORPTION SPECTROMETER

Model & Serial Number: AA 240FS & AA0911M073
Customer: Water Analysis Center Co., Ltd.
Date: 04 Feb 2021

Safety

- ☒ Flame, Inspect/replace o-ring nebulizer, spray chamber and burner
- ☒ Flame, Clean nebulizer, spray chamber and burner
- ☒ Flame, Check liquid trap interlock, burner interlock, pressure relief/bung interlock and shield interlock
- ☐ Furnace, Clean work head, electrode and shroud N/A
- ☐ Furnace, Clean PSD and PSD tray N/A
- ☐ Furnace, Check water pressure N/A
- ☒ Check drain tube
- ☒ Check exhaust system
- ☒ Check gas pressure sensor interlock
- ☒ Check and all gas hoses for SpectraAA
- ☒ Clean computer control

Optics

- ☒ Inspect/Replace that external optics surfaces
- ☒ Check Wavelength Accuracy the copper line at 323.0-326.0 nm = 324.8 nm
- ☒ Check that PMT % Gain the copper at 324.8 nm, 4 mA, 0.5 nm slit width, Gain = 56% (should be $\leq 64\%$ or $\leq 380V$)
- ☒ Flame, Check D2 lamp is work



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาวิทย์ แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200
80-82 Prachathipatai Rd., Bangkokunphrom, Pranakorn, Bangkok 10200
Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawati@thaiunique.com, Website : www.thaiunique.com

Electronics

- ☒ Check power supply voltage
- ☒ Check cables and connectors
- ☒ Check/Clean all boards in the instrument
- ☐ Furnace, Check camera and align** N/A

**Option for Graphite Zeeman only

Mechanisms

- ☒ Flame, Check the burner adjuster
- ☐ Furnace, Check PSD accessories N/A

Analytical performance

- ☒ Clear the sample compartment
- ☒ Flame, Check uptake rate form 7.2-10.6 mL per minute = 9.8 mL/min
- ☒ Test Photometric noise, STDV = 0.0001 Abs (should be ≤ 0.00050 Abs)
- ☒ Flame, Test high solids nebulizer setting use
 - Air/acet Cu 5 ppm = 0.75 Abs, and Precision
 - (%RSD) = 0.5 % (should be > 0.55 Abs and $< 0.5\%$ RSD)
- or
- N2O/Acet Cu 5 ppm = _____ Abs, and Precision
- (%RSD) = _____ % (should be > 0.3 Abs and $< 0.5\%$ RSD)
- ☐ Furnace, Characteristic mass and sensitivity Cu 25 ppb = _____ Abs, and N/A
- Precision (%RSD) = _____ % (should be ≥ 0.15 Abs and $\leq 4.0\%$ RSD)

SIGN :

Engineer

Customer

SVD Results Report



Report ID:3	Diagnostic Start Time:05-Dec-20 10:38:29 AM	Diagnostic End Time:04-Feb-21 11:58:44 AM
Customer: Water Analysis Center Co., Ltd.	Service Engineer: SuriyaNacharoen	
Address: Prana khon si ayuthaya	Contact Details: K_Kanitsara	
Instrument Configuration		

Configuration:

Serial Number: AA0911M073	Turret Type: Automatic
Instrument Model: Varian AA140/240/280	Number Of Lamps: 4
Flame Instrument: True	Mono Type: Automatic
Furnace Instrument: True	Gasbox Type: 'Y' Gas Box
Zeeman Present: False	Auto Burner Adjuster: False
Internal Zeeman: False	Mains Frequency: 50
Internal UltraAA: False	Firmware Version: 2.12
Optics Type: Double Beam	Photomultiplier Type: Normal(900nm)
D2 BG Correction Fitted: True	PWB Version: 181
Boot Block Version: 2.02	

EEPROM Data:

Instrument Run Hours: 20613.650	D2 Run Hours: 2906.000
Zero Wavelength Offset: -18.731	D2 Serial Number: not set !
Mono Correction: -0.370	D2 Install Date: 01-Jan-70
Flame Hours: 4025.000	D2 Original Intensity: 1.000
	D2 Last Intensity: 661.000

Frequency:

Averaging Period: 30.0	
Datapoint Count: 20	
Upper Limit: 51.00	Highest Measured Frequency: 50.00
Lower Limit: 49.00	Lowest Measured Frequency: 50.00
Average Frequency: 50.00	
Result: Passed	

Power Supply:


Averaging Period: 30.0
Datapoint Count: 20

	Lower Limit (V)	Actual (V)	Upper Limit (V)	Result:
12.00V Rail	10.80	12.20	13.20	Passed
-12.00V Rail	-13.20	-12.00	-10.80	Passed
5.00V Rail	4.50	5.10	5.50	Passed
310.00V Rail	279.00	318.00	341.00	Passed


Beam Balance:

Lamp Type: Copper
Lamp Socket Used: 3
Peak Selected: 324.80
Lamp Alignment: Performed

'X' Lamp Screw

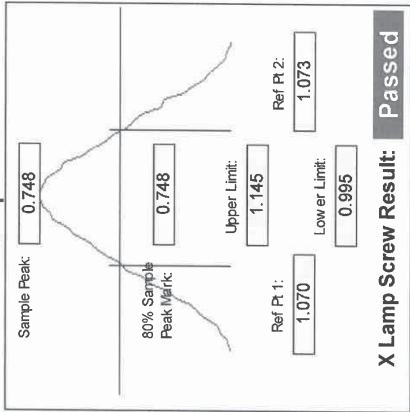

'Y' Lamp Screw

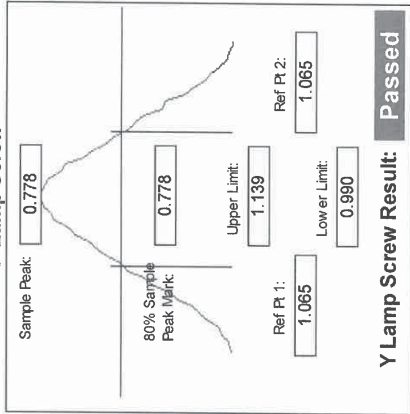

Grating Squareness:

Lamp Element(s): Copper
Lamp Turret Position: 3
Lamp Current(mA): 4.00
Slit Width(nm): 0.5
1st Order Wavelength(nm): 324.80
Lamp Alignment: Performed

	Lower Limit (nm)	Actual (nm)	Upper Limit (nm)	Result:
Zero Order	-0.10	0.00	0.10	Passed
First Order	324.45	324.73	325.15	Passed
Second Order	649.23	649.56	649.97	Passed

Wavelength Repeatability:

Lamp Used: Copper
Peak Used(nm): 324.750
Connected to Socket: 3
Lamp Current(mA): 4
Slit Width(nm): 0.2
Slit Height: Normal

Lamp Alignment: Performed

Lower Limit(nm)	324.751	324.871	Upper Limit(nm)
<i>(Approach from Zero Order)</i>			
Sample 1:	324.811	Sample 2:	324.807
Sample 3:	324.811	Sample 4:	324.811
Sample 5:	324.815	Sample 6:	324.811
Sample 7:	324.815	Sample 8:	324.811
Sample 9:	324.815	Sample 10:	324.815

Mean: 324.812
Standard Deviation: 0.003

Result: Passed

Mechanical

Wavelength Drive:

Passed

Slit Drive:

Passed

Turret Drive:

Passed

Auto Burner Adjuster Drive:

Untested

Miscellaneous

Signal Processing Linearity:

Calculate Mode: New Calc Mode

	Lower Limit	Actual	Upper Limit	Result:
S0	114	248	297	Passed
S1	156	165	191	Passed
S2	271	294	332	Passed
S3	474	506	579	Passed
S4	825	908	1008	Passed
S5	1435	1516	1754	Passed
S6	2498	2723	3053	Passed
S7	4347	4681	5313	Passed

Interlocks:

Burner Fitted:	Working	Flame Detect:	Working
N2O Burner Fitted:	Working	GCU Active:	Working
Flame Shield Closed:	Working	Oxidant Pressure:	Working
Gas Control Fitted:	Untested	Oxidant Changeover:	Working
Pressure Release Bung Fitted:	Working	Ignition:	Working
Liquid Trap Fitted:	Working		

Auto Lamp Recognition:

- Lamp 1: 50 - Selenium (Se)
- Lamp 2: 3 - Arsenic (As)
- Lamp 3: 14 - Copper (Cu)
- Lamp 4: 42 - Potassium (K)
- Lamp 5: Not Supported
- Lamp 6: Not Supported
- Lamp 7: Not Supported
- Lamp 8: Not Supported

Result: Passed


GTA Temperature Monitoring:

Not Performed

Notes:

C2102SU11 PM1/2

Signatures:



Water Analysis Center Co., Ltd.Date

BSC Certification Test Report

Page 1 of 6

Certificate No. : M0979/21

Customer Name : LABORATORY WATER ANALYSIS CENTER COMPANY LIMITED

Customer Address : 1/94 Moo 5 T.Kanharm, A.U-Thai,
Phra Nakhon Si Ayuthaya 13210

Equipment : Biological Safety Cabinet Class II Type A2

Manufacturer : Microtech

Model : V6-T

Serial No : 0972

ID No. : WWL0084

Were in accordance with ☒ EN 12469 ☐ NSF 49 ☐ Manufacturer's specification

Test Date : 23/09/2021

Due Date : 23/09/2022 or after HEPA filters are replaced or unit is moved

Test by : Mr. Puwadon Keawkia

Approved by :

Issued Date :

This calibration certificate documents the traceability to national standards, which realize the unit of measurement according to the International System of Units (SI).

This certificate may not be reproduced other than in full except with the prior written approval of the Megafil Company Limited.

Page 2 of 6

Certificate No. : M0979/21

- Procedure Used :
- : European Standard EN12469 : 2000 has the status of British Standard,
 - Biotechnology Performance criteria for microbiological safety cabinets.
 - : NSF International Standard / American National Standard NSF / ANSI 49-2008
 - Biosafety Cabinet : Design, Construction, Performance and Field Certification.
 - : Australian Standard : AS 1807.23-2000 Determination of intensity of radiation from germicidal ultraviolet lamps.
 - : Manufacturer's specification.

1. Downflow velocity test.

Measurement Information

No. of Rows	No. of Readings	Grid Spacing Front-Back	Grid Spacing Side-Side	Probe height Above sash
2	8	1/4,3/4	1/8,3/8	100 mm.

Measurement Data.

0.34	0.37	0.36	0.35
0.32	0.33	0.32	0.34

Average velocity 0.34 m/s (67 FPM.) Velocity range 0.25-0.50 m/s (49-98 FPM.)

Uniformity(EN: +/-20%avg. 0.27 - 0.41 m/s (54 - 80 FPM.)

Supply filter dimension 24 x 72 (inch x inch) Supply filter area 10.69 SQ.FT

Downflow volume (Q) 716 CFM.

Result Summary ☒ Pass ☐ Fail

Equipment used : Thermo Anemometer Model 425 S/N : 03004786 Calibration date : 23/02/2021

Certificate No. : M0979/21

2. Inflow velocity test.

Select method. : ☐ DIM ☒ Exhaust velocity. ☐ MFG's Specifications

0.57	0.59	0.56	0.61	0.63
0.58	0.6	0.56	0.59	0.58
0.61	0.57	0.56	0.54	0.56
0.59	0.56	0.62	0.59	0.62
0.59	0.57	0.63	0.59	0.58

Average Inflow velocity 0.50 m/s (98 FPM.) Velocity range ≥ 0.40 m/s (≥ 79 FPM.)

Inflow dimension 8 x 72 (inch x inch) Inflow area 4.00 SQ.FT

Inflow volume(Q) 392 CFM

Result Summary ☒ Pass ☐ Fail

Adjustments Required ☐ Fan Speed ☐ Damper

Equipment used : Thermo Anemometer Model 425 S/N : 03004786 Calibration date 23/02/2021

3. HEPA filter leak test.

Measurement Data

HEPA Filter	PAO Upstream Conc.(calculated)	Specification	Measured leak penetration
Supply HEPA Filter	18 $\mu\text{g/L}$	<0.003%	<0.003%
Exhaust HEPA Filter	18 $\mu\text{g/L}$	<0.003%	<0.003%

Certificate No. : M0979/21

Leak location

Supply HEPA Filter

Back



Exhaust HEPA Filter

Back



Result Summary ☒ Pass ☐ Fail

Equipment used : Aerosol Photometer Model TDA-2H S/N : 21683 Calibration date 24/02/2021

Equipment used : Smoke Generator Model TDA-6C S/N : 21623

4. Airflow smoke patterns test

Measurement Information

- Downflow Pattern test : Smoke shall be passed from one end of the cabinet to the other, along the centerline of the work surface, at a height of 4 inch (10 cm) above the top of the access opening
- View screen retention test : Smoke shall be passed from one end of the cabinet to the other, 1.0 in (2.5 cm) behind the view screen, at a height 6.0 inch (15 cm) above the top of the access opening.
- Work opening edge retention test : Smoke shall be passed along the entire perimeter of the work opening. Particular attention should be paid to corners and vertical edges.
- Sash/window seal test : Smoke shall be passed up the inside of the window 2 in (5 cm) from the sides and along the top of the work area.

Certificate No. : M0979/21

Result Summary

Downflow Pattern test	<input checked="" type="checkbox"/> Accept	<input type="checkbox"/> Non-Conforming
View screen retention test	<input checked="" type="checkbox"/> Accept	<input type="checkbox"/> Non-Conforming
Work opening edge retention test	<input checked="" type="checkbox"/> Accept	<input type="checkbox"/> Non-Conforming
Sash/window seal test	<input checked="" type="checkbox"/> Accept	<input type="checkbox"/> Non-Conforming

5. Site installation

Sash Alarm.	<input type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> N/A
Interlock System.	<input type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> N/A
Exhaust System Performance	<input type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> N/A

Remark / Recommendation

ระบบ Site installation ไม่มีการตรวจสอบ เนื่องจากตู้ไม่มีฟังก์ชันนี้

6. Illumination Test (Lighting) : Option

Lighting should be adequate for safe working within the cabinet. Illumination measured at the work surface.

Lux

632	1000	997	630
947	1456	1449	921

Remark :

Certificate No. : M0979/21

7. Ultraviolet Lamp Test (UV) : Option

Ultraviolet radiation where UV Lamp are fitted, the intensity of radiation at a wavelength of 254 nm. Shall be not less than 400 mW/m² when measures at work floor surface.

mW/m²

740	1580	1570	750
480	1040	1020	480

Remark :

-o0o-