

ANALYSIS REPORT

CUSTOMER NAME : ECO ORIENT RESOURCES (THAILAND) LTD.
ADDRESS : 555 RASA TOWER II, 12TH FLOOR, UNIT 1203 PHAHOLYOTHIN ROAD CHATUCHAK CHATUCHAK BANGKOK 10900
CONTACT INFORMATION : TEL : 0 2937 1124-9 e-mail : anucha@ecothai.net
SAMPLING SOURCE : GW2: MOO 5 BAN TUNG YAI (UTM WGS 84 ZONE 47P 730155E 1728942N)
SAMPLE TYPE : GROUNDWATER
SAMPLING DATE : FEBRUARY 10, 2022
SAMPLING TIME : 10:50 HOUR
SAMPLING METHOD ° : GRAB
SAMPLING BY ° : MR TEERAPONG SRIKAMHANG
ANALYZED BY : MISS NADNAPA KAMOLBOON

RECEIVED DATE : FEBRUARY 10, 2022
ANALYTICAL DATE : FEBRUARY 10-23, 2022
REPORT NO. : 2022-U013123
WORK NO. : 2021-008599
ANALYSIS NO. : T22AC414-0002

PARAMETER	UNIT	METHOD OF ANALYSIS	RESULT	REGULATORY STANDARD	DETECTION LIMIT
			GW2: MOO 5 BAN TUNG YAI T22AC414-0002		
pH °	-	ELECTROMETRIC METHOD AT SITE (SM:4500-H° B)	7.2 (30°C)	-	-
TEMPERATURE °	°C	THERMOMETER AT SITE (SM: 2550 B)	30	-	-
ELECTRICAL CONDUCTIVITY °	µmhos/cm	ELECTRICAL CONDUCTIVITY METHOD AT SITE (SM: 2510 B)	1,085 (30°C)	-	0.1
SALINITY °	ppt	ELECTRICAL CONDUCTIVITY METHOD AT SITE (SM: 2520 B)	0.7	-	0.1
TOTAL SUSPENDED SOLIDS °	mg/L	TOTAL SUSPENDED SOLIDS DRIED AT 103-105 °C (SM: 2540 D)	6.9	-	5.0
TOTAL DISSOLVED SOLIDS °	mg/L	TOTAL DISSOLVED SOLIDS DRIED AT 180 °C (SM: 2540 C)	704	-	25
TOTAL PETROLEUM HYDROCARBONS °	mg/L	SOXHLET EXTRACTION METHOD (SM: 5520 D AND 5520 F)	ND	-	3
METALS					
ARSENIC °	mg/L As	HYDRIDE GENERATION AAS METHOD (SM: 3114 C)	ND	≤ 0.01	0.0003
BARIUM °	mg/L Ba	NITRIC ACID-HYDROCHLORIC ACID DIGESTION AND INDUCTIVELY COUPLED PLASMA (ICP) METHOD (SM: 3030 F AND 3120 B)	0.071	-	0.003
CADMIUM °	mg/L Cd	IN-HOUSE METHOD: UAE.TP.GW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤ 0.003	0.002
HEXAVALENT CHROMIUM °	mg/L Cr ⁶⁺	COLOURIMETRIC METHOD (SM: 3500-Cr B)	ND	≤ 0.05	0.006
COPPER °	mg/L Cu	IN-HOUSE METHOD: UAE.TP.GW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	< LOQ	≤ 1.0	0.002
IRON °	mg/L Fe	IN-HOUSE METHOD: UAE.TP.GW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	0.227	-	0.005
LEAD °	mg/L Pb	IN-HOUSE METHOD: UAE.TP.GW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤ 0.01	0.003

PARAMETER	UNIT	METHOD OF ANALYSIS	RESULT	REGULATORY STANDARD	DETECTION LIMIT
			GW2: MOO 5 BAN TUNG YAI T22AC414-0002		
MANGANESE °	mg/L Mn	IN-HOUSE METHOD: UAE.TP.GW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	0.030	≤ 0.5	0.002
MERCURY °	mg/L Hg	IN-HOUSE METHOD: UAE.TP.HEM.002 (COLD VAPOUR ATOMIC ABSORPTION SPECTROMETRIC METHOD); SM: 3112 B	ND	≤ 0.001	0.0001
NICKEL °	mg/L Ni	IN-HOUSE METHOD: UAE.TP.GW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤ 0.02	0.005
SELENIUM °	mg/L Se	HYDRIDE GENERATION AAS METHOD (SM: 3114 C)	ND	≤ 0.01	0.0005
ZINC °	mg/L Zn	IN-HOUSE METHOD: UAE.TP.GW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤ 5.0	0.003
VOLATILE ORGANIC COMPOUNDS					
BENZENE °	µg/L	PURGE AND TRAP GAS CHROMATOGRAPHIC/MASS SPECTROMETRIC METHOD (SM: 6200 B)	< 0.20	≤ 5	0.20
ETHYLBENZENE °	µg/L	PURGE AND TRAP GAS CHROMATOGRAPHIC/MASS SPECTROMETRIC METHOD (SM: 6200 B)	< 0.20	≤ 700	0.20
TOLUENE °	µg/L	PURGE AND TRAP GAS CHROMATOGRAPHIC/MASS SPECTROMETRIC METHOD (SM: 6200 B)	< 0.20	≤ 1,000	0.20
TOTAL XYLENES °	µg/L	PURGE AND TRAP GAS CHROMATOGRAPHIC/MASS SPECTROMETRIC METHOD (SM: 6200 B)	< 0.60	≤ 10,000	0.60
SAMPLE CONDITION					
WATER'S COLOUR/TURBID SEDIMENT			YELLOW/CLEAR BROWN		

a : ISO/IEC 17025 ACCREDITED BY THAI INDUSTRIAL STANDARDS INSTITUTE (TISI)

b : ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

c : VERIFIED BY OWN LABORATORY QUALITY SYSTEM, BUT STILL NOT ACCREDITED

IN-HOUSE : BASED ON STANDARD METHODS FOR THE EXAMINATION OF WATER AND WASTEWATER, APHA, AWWA, WEF, 23rd EDITION, 2017.

SM : STANDARD METHODS FOR THE EXAMINATION OF WATER AND WASTEWATER, APHA, AWWA, WEF, 23rd EDITION, 2017.

REGULATORY STANDARD : GROUNDWATER QUALITY STANDARDS, NOTIFICATION OF THE NATIONAL ENVIRONMENT BOARD NO 20 (B.E. 2543) ISSUED UNDER THE ENHANCEMENT AND CONSERVATION OF NATIONAL ENVIRONMENTAL QUALITY ACT B.E. 2535.

ND : NON-DETECTABLE.

< LOQ : < LEVEL OF QUANTITATION (COPPER ≥ 0.002 AND < 0.025 mg/L).

Benjawan V.

(MISS BENJAWAN VIRIYOTHAI)
LABORATORY SUPERVISOR

FEBRUARY 28, 2022



คุณภาพน้ำผิวดิน



ANALYSIS REPORT

CUSTOMER NAME : ECO ORIENT RESOURCES (THAILAND) LTD.
ADDRESS : 555 RASA TOWER II, 12TH FLOOR, UNIT 1203 PHAHOLYOTHIN ROAD CHATUCHAK CHATUCHAK BANGKOK 10900
CONTACT INFORMATION : TEL : 0 2937 1124-9 e-mail : anucha@ecothai.net
SAMPLING SOURCE : SW3: KHLONG HUI PAI (UP GRADIENT OF WBNE-F) (UTM WGS 84 ZONE 47P 735618E 1731580N)
SAMPLE TYPE : SURFACE WATER
SAMPLING DATE : FEBRUARY 10, 2022
SAMPLING TIME : 09:00 HOUR
SAMPLING METHOD ° : GRAB, GRAB AND STERILE TECHNIQUE
SAMPLING BY ° : MR TEERAPONG SRIKAMHANG
ANALYZED BY : MISS PORNPIMOL WAENTHONG

RECEIVED DATE : FEBRUARY 10, 2022
ANALYTICAL DATE : FEBRUARY 10-23, 2022
REPORT NO. : 2022-U013216
WORK NO. : 2021-008599
ANALYSIS NO. : T22AC415-0001

PARAMETER	UNIT	METHOD OF ANALYSIS	RESULT	REGULATORY STANDARD	DETECTION LIMIT
			SURFACE WATER T22AC415-0001		
pH °	-	ELECTROMETRIC METHOD AT SITE (SM:4500-H° B)	7.9 (27°C)	5.0-9.0	-
TEMPERATURE °	°C	THERMOMETER AT SITE (SM: 2550 B)	27	n°	-
ELECTRICAL CONDUCTIVITY °	µmhos/cm	ELECTRICAL CONDUCTIVITY METHOD AT SITE (SM: 2510 B)	629 (27°C)	-	0.1
DISSOLVED OXYGEN °	mg/L	AZIDE MODIFICATION METHOD AT SITE (SM: 4500-O C)	4.0	≥ 4.0	0.5
SALINITY °	ppt	ELECTRICAL CONDUCTIVITY METHOD AT SITE (SM: 2520 B)	0.4	-	0.1
BIOCHEMICAL OXYGEN DEMAND °	mg/L	AZIDE MODIFICATION METHOD (SM: 4500-O C AND 5210 B)	3.8	≤ 2.0	1.0
TOTAL SUSPENDED SOLIDS °	mg/L	TOTAL SUSPENDED SOLIDS DRIED AT 103-105 °C (SM: 2540 D)	318	-	5.0
TOTAL DISSOLVED SOLIDS °	mg/L	TOTAL DISSOLVED SOLIDS DRIED AT 180 °C (SM: 2540 C)	412	-	25
TOTAL PETROLEUM HYDROCARBONS °	mg/L	SOXHLET EXTRACTION METHOD (SM: 5520 D AND 5520 F)	ND	-	3
FAT, OIL AND GREASE °	mg/L	SOXHLET EXTRACTION METHOD (SM: 5520 D)	ND	-	3
METALS					
ARSENIC °	mg/L As	HYDRIDE GENERATION AAS METHOD (SM: 3114 C)	0.0005	≤ 0.01	0.0003
BARIUM °	mg/L Ba	NITRIC ACID-HYDROCHLORIC ACID DIGESTION AND INDUCTIVELY COUPLED PLASMA (ICP) METHOD (SM: 3030 F AND 3120 B)	0.080	-	0.003
CADMIUM °	mg/L Cd	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤0.005*, ≤ 0.05**	0.002
HEXAVALENT CHROMIUM °	mg/L Cr ⁶⁺	COLOURIMETRIC METHOD (SM: 3500-Cr B)	ND	≤ 0.05	0.006
COPPER °	mg/L Cu	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	< LOQ	≤ 0.1	0.002
IRON °	mg/L Fe	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	1.28	-	0.005



PARAMETER	UNIT	METHOD OF ANALYSIS	RESULT	REGULATORY STANDARD	DETECTION LIMIT
			SURFACE WATER T22AC415-0001		
LEAD °	mg/L Pb	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤ 0.05	0.003
MANGANESE °	mg/L Mn	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	0.230	≤ 1.0	0.002
MERCURY °	mg/L Hg	IN-HOUSE METHOD: UAE.TP.HEM.002 (COLD VAPOUR ATOMIC ABSORPTION SPECTROMETRIC METHOD); SM: 3112 B	ND	≤ 0.002	0.0001
NICKEL °	mg/L Ni	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤ 0.1	0.005
SELENIUM °	mg/L Se	HYDRIDE GENERATION AAS METHOD (SM: 3114 C)	ND	-	0.0005
ZINC °	mg/L Zn	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤ 1.0	0.003
MICROBIOLOGY					
FAECAL COLIFORM BACTERIA °	MPN/100 mL	MULTIPLE-TUBE FERMENTATION TECHNIQUE (SM: 9221 E)	460	≤ 4,000	18
VOLATILE ORGANIC COMPOUNDS					
BENZENE °	µg/L	PURGE AND TRAP GAS CHROMATOGRAPHIC/MASS SPECTROMETRIC METHOD (SM: 6200 B)	< 0.20	-	0.20
ETHYLBENZENE °	µg/L	PURGE AND TRAP GAS CHROMATOGRAPHIC/MASS SPECTROMETRIC METHOD (SM: 6200 B)	< 0.20	-	0.20
TOLUENE °	µg/L	PURGE AND TRAP GAS CHROMATOGRAPHIC/MASS SPECTROMETRIC METHOD (SM: 6200 B)	< 0.20	-	0.20

PARAMETER	UNIT	METHOD OF ANALYSIS	RESULT	REGULATORY STANDARD	DETECTION LIMIT
			SURFACE WATER T22AC415-0001		
TOTAL XYLENES °	µg/L	PURGE AND TRAP GAS CHROMATOGRAPHIC/MASS SPECTROMETRIC METHOD (SM: 6200 B)	< 0.60	-	0.60
SAMPLE CONDITION					
WATER'S COLOUR/TURBID SEDIMENT			YELLOW/TURBID BROWN		

° : ISO/IEC 17025 ACCREDITED BY THAI INDUSTRIAL STANDARDS INSTITUTE (TISI)

° : ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

° : VERIFIED BY OWN LABORATORY QUALITY SYSTEM, BUT STILL NOT ACCREDITED

IN-HOUSE : BASED ON STANDARD METHODS FOR THE EXAMINATION OF WATER AND WASTEWATER, APHA, AWWA, WEF, 23rd EDITION, 2017.

SM : STANDARD METHODS FOR THE EXAMINATION OF WATER AND WASTEWATER, APHA, AWWA, WEF, 23rd EDITION, 2017.

REGULATORY STANDARD : SURFACE WATER QUALITY STANDARDS CLASS 3, NOTIFICATION OF THE NATIONAL ENVIRONMENT BOARD, NO.8, B.E. 2537 ISSUED UNDER THE ENHANCEMENT AND CONSERVATION OF NATIONAL ENVIRONMENTAL QUALITY ACT, B.E. 2535, PUBLISHED IN THE ROYAL GOVERNMENT GAZETTE, VOL. 111, PART 16, DATED FEBRUARY 24, B.E. 2537 (1994).

CLASS 3 : MEDIUM CLEAN FRESH SURFACE WATER RESOURCES USED FOR
(1) CONSUMPTION, BUT PASSING THROUGH ON ORDINARY TREATMENT PROCESS BEFORE USING
(2) AGRICULTURE

n° : NATURALLY BUT CHANGING NOT MORE THAN 3°C

≤ 0.005° : WHEN WATER HARDNESS NOT MORE THAN 100 mg/L AS CaCO₃

≤ 0.05° : WHEN WATER HARDNESS MORE THAN 100 mg/L AS CaCO₃

ND : NON-DETECTABLE.

< LOQ : < LEVEL OF QUANTITATION (COPPER ≥ 0.002 AND < 0.025 mg/L).

Benjawan V.

(MISS BENJAWAN VIRIYOTHA)
LABORATORY SUPERVISOR

FEBRUARY 28, 2022

ANALYSIS REPORT

CUSTOMER NAME : ECO ORIENT RESOURCES (THAILAND) LTD.
ADDRESS : 555 RASA TOWER II, 12TH FLOOR, UNIT 1203 PHAHOLYOTHIN ROAD CHATUCHAK CHATUCHAK BANGKOK 10900
CONTACT INFORMATION : TEL : 0 2937 1124-9 e-mail : anucha@ecothai.net
SAMPLING SOURCE : SW4: KHLONG HUI PAI (DOWN GRADIENT OF WBNE-F) (UTM WGS 84 ZONE 47P 733621E 1728215N)
SAMPLE TYPE : SURFACE WATER
SAMPLING DATE : FEBRUARY 10, 2022
SAMPLING TIME : 10:10 HOUR
SAMPLING METHOD ° : GRAB, GRAB AND STERILE TECHNIQUE
SAMPLING BY ° : MR TEERAPONG SRIKAMHANG
ANALYZED BY : MISS PORNPIMOL WAENTHONG

RECEIVED DATE : FEBRUARY 10, 2022
ANALYTICAL DATE : FEBRUARY 10-23, 2022
REPORT NO. : 2022-U013217
WORK NO. : 2021-008599
ANALYSIS NO. : T22AC415-0002

PARAMETER	UNIT	METHOD OF ANALYSIS	RESULT	REGULATORY STANDARD	DETECTION LIMIT
			SURFACE WATER T22AC415-0002		
pH °	-	ELECTROMETRIC METHOD AT SITE (SM:4500-H° B)	7.4 (27°C)	5.0-9.0	-
TEMPERATURE °	°C	THERMOMETER AT SITE (SM: 2550 B)	27	n°	-
ELECTRICAL CONDUCTIVITY °	µmhos/cm	ELECTRICAL CONDUCTIVITY METHOD AT SITE (SM: 2510 B)	338 (27°C)	-	0.1
DISSOLVED OXYGEN °	mg/L	AZIDE MODIFICATION METHOD AT SITE (SM: 4500-O C)	2.6	≥ 4.0	0.5
SALINITY °	ppt	ELECTRICAL CONDUCTIVITY METHOD AT SITE (SM: 2520 B)	0.2	-	0.1
BIOCHEMICAL OXYGEN DEMAND °	mg/L	AZIDE MODIFICATION METHOD (SM: 4500-O C AND 5210 B)	2.8	≤ 2.0	1.0
TOTAL SUSPENDED SOLIDS °	mg/L	TOTAL SUSPENDED SOLIDS DRIED AT 103-105 °C (SM: 2540 D)	23.1	-	5.0
TOTAL DISSOLVED SOLIDS °	mg/L	TOTAL DISSOLVED SOLIDS DRIED AT 180 °C (SM: 2540 C)	202	-	25
TOTAL PETROLEUM HYDROCARBONS °	mg/L	SOXHLET EXTRACTION METHOD (SM: 5520 D AND 5520 F)	ND	-	3
FAT, OIL AND GREASE °	mg/L	SOXHLET EXTRACTION METHOD (SM: 5520 D)	ND	-	3
METALS					
ARSENIC °	mg/L As	HYDRIDE GENERATION AAS METHOD (SM: 3114 C)	0.0010	≤ 0.01	0.0003
BARIUM °	mg/L Ba	NITRIC ACID-HYDROCHLORIC ACID DIGESTION AND INDUCTIVELY COUPLED PLASMA (ICP) METHOD (SM: 3030 F AND 3120 B)	0.047	-	0.003
CADMIUM °	mg/L Cd	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤ 0.005°, ≤ 0.05°	0.002
HEXAVALENT CHROMIUM °	mg/L Cr ⁶⁺	COLOURIMETRIC METHOD (SM: 3500-Cr B)	ND	≤ 0.05	0.006
COPPER °	mg/L Cu	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤ 0.1	0.002
IRON °	mg/L Fe	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	2.49	-	0.005



PARAMETER	UNIT	METHOD OF ANALYSIS	RESULT	REGULATORY STANDARD	DETECTION LIMIT
			SURFACE WATER T22AC415-0002		
LEAD ^c	mg/L Pb	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤ 0.05	0.003
MANGANESE ^c	mg/L Mn	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	0.778	≤ 1.0	0.002
MERCURY ^b	mg/L Hg	IN-HOUSE METHOD: UAE.TP.HEM.002 (COLD VAPOUR ATOMIC ABSORPTION SPECTROMETRIC METHOD); SM: 3112 B	ND	≤ 0.002	0.0001
NICKEL ^c	mg/L Ni	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤ 0.1	0.005
SELENIUM ^c	mg/L Se	HYDRIDE GENERATION AAS METHOD (SM: 3114 C)	ND	-	0.0005
ZINC ^c	mg/L Zn	IN-HOUSE METHOD: UAE.TP.SW.01 (NITRIC ACID DIGESTION AND DIRECT AIR ACETYLENE FLAME METHOD); SM: 3030 E AND 3111 B	ND	≤ 1.0	0.003
MICROBIOLOGY					
FAECAL COLIFORM BACTERIA ^b	MPN/100 mL	MULTIPLE-TUBE FERMENTATION TECHNIQUE (SM: 9221 E)	33	≤ 4,000	1.8
VOLATILE ORGANIC COMPOUNDS					
BENZENE ^c	µg/L	PURGE AND TRAP GAS CHROMATOGRAPHIC/MASS SPECTROMETRIC METHOD (SM: 6200 B)	< 0.20	-	0.20
ETHYLBENZENE ^c	µg/L	PURGE AND TRAP GAS CHROMATOGRAPHIC/MASS SPECTROMETRIC METHOD (SM: 6200 B)	< 0.20	-	0.20
TOLUENE ^c	µg/L	PURGE AND TRAP GAS CHROMATOGRAPHIC/MASS SPECTROMETRIC METHOD (SM: 6200 B)	< 0.20	-	0.20

PARAMETER	UNIT	METHOD OF ANALYSIS	RESULT	REGULATORY STANDARD	DETECTION LIMIT
			SURFACE WATER T22AC415-0002		
TOTAL XYLENES ^c	µg/L	PURGE AND TRAP GAS CHROMATOGRAPHIC/MASS SPECTROMETRIC METHOD (SM: 6200 B)	< 0.60	-	0.60
SAMPLE CONDITION					
WATER'S COLOUR/TURBID SEDIMENT			YELLOW/TURBID BROWN		

^a : ISO/IEC 17025 ACCREDITED BY THAI INDUSTRIAL STANDARDS INSTITUTE (TISI)

^b : ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

^c : VERIFIED BY OWN LABORATORY QUALITY SYSTEM, BUT STILL NOT ACCREDITED

IN-HOUSE : BASED ON STANDARD METHODS FOR THE EXAMINATION OF WATER AND WASTEWATER, APHA, AWWA, WEF, 23rd EDITION, 2017.

SM : STANDARD METHODS FOR THE EXAMINATION OF WATER AND WASTEWATER, APHA, AWWA, WEF, 23rd EDITION, 2017.

REGULATORY STANDARD : SURFACE WATER QUALITY STANDARDS CLASS 3, NOTIFICATION OF THE NATIONAL ENVIRONMENT BOARD, NO.8, B.E. 2537 ISSUED UNDER THE ENHANCEMENT AND CONSERVATION OF NATIONAL ENVIRONMENTAL QUALITY ACT, B.E. 2535, PUBLISHED IN THE ROYAL GOVERNMENT GAZETTE, VOL. 111, PART 16, DATED FEBRUARY 24, B.E. 2537 (1994).

CLASS 3 : MEDIUM CLEAN FRESH SURFACE WATER RESOURCES USED FOR
(1) CONSUMPTION, BUT PASSING THROUGH ON ORDINARY TREATMENT PROCESS BEFORE USING
(2) AGRICULTURE

n¹ : NATURALLY BUT CHANGING NOT MORE THAN 3°C

≤ 0.005* : WHEN WATER HARDNESS NOT MORE THAN 100 mg/L AS CaCO₃

≤ 0.05** : WHEN WATER HARDNESS MORE THAN 100 mg/L AS CaCO₃

ND : NON-DETECTABLE.

Benjawan V.

(MISS BENJAWAN VIRIYOTHAI)
LABORATORY SUPERVISOR

FEBRUARY 28, 2022

ภาคผนวก ฎ
เอกสารสอบเทียบเครื่องมือ



List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Tisch Environmental, Inc.	TE-5025A 3393	Tisch Environmental, Inc.	27072020	27 Jul 20	26 Jul 22	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	22P801	12 Mar 22	11 Mar 23	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	21P2499	21 Jul 21	20 Jul 22	-
4	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1191503038	UAE Consultant Co., Ltd.	04112021	4 Nov 21	3 Nov 22	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1201497724	UAE Consultant Co., Ltd.	10112021	10 Nov 21	9 Nov 22	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1201497725	UAE Consultant Co., Ltd.	10112021	10 Nov 21	9 Nov 22	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1201497726	UAE Consultant Co., Ltd.	17112021	17 Nov 21	16 Nov 22	-
8	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
9	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1200906876	UAE Consultant Co., Ltd.	07122021	7 Dec 21	6 Dec 22	-
10	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1182920012	UAE Consultant Co., Ltd.	09112021	22 Nov 21	21 Nov 22	-
11	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1182920013	UAE Consultant Co., Ltd.	09112021	22 Nov 21	21 Nov 22	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
12	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1182920014	UAE Consultant Co.,Ltd.	09112021	22 Nov 21	21 Nov 22	-
13	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
14	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1200636464	UAE Consultant Co.,Ltd.	24112021	24 Nov 21	23 Nov 22	-
15	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1200636465	UAE Consultant Co.,Ltd.	24112021	24 Nov 21	23 Nov 22	-
16	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1200636466	UAE Consultant Co.,Ltd.	24112021	24 Nov 21	23 Nov 22	-
17	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48i 1200636467	UAE Consultant Co.,Ltd.	24112021	24 Nov 21	23 Nov 22	-
18	Standard Gases (Mixture)	Carbon Monoxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
19	Wind Speed/Wind Direction	WS/WD	LSI LASTEM	E-LOG305 19040308	Thai Meteorological Department	385/21	16 Aug 21	15 Aug 22	-
20	Wind Speed/Wind Direction	WS/WD	LSI LASTEM	E-LOG305 19040406	Thai Meteorological Department	354/21	20 Jul 21	19 Jul 22	-
21	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6171	Innovative Instrument Co.,Ltd.	21-ACT-327	24 Aug 21	23 Aug 22	-
22	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax} , L_{A90} , L_{Adn}	Rion, Japan	NL-42 01010782	Sithiporn Associates Co., Ltd.	ACL22088	22 Apr 22	21 Apr 23	-
23	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax} , L_{A90} , L_{Adn}	Rion, Japan	NL-42 01010783	Sithiporn Associates Co., Ltd.	ACL22089	22 Apr 22	21 Apr 23	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
24	Sound Level Meter	L _{Aeq} 24 hours, L _{Amax} , L _{A90} , L _{Adn}	Rion, Japan	NL-42	Sithiporn Associates Co., Ltd.	ACL22090	22 Apr 22	21 Apr 23	-
				01010784					

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	YSI	pH100A JC03354	Technology Promotion Association (Thailand-Japan)	22CH60	13 Jan 22	12 Jan 23	-
2	Conductivity Meter	Conductivity	YSI	Pro30 18C105225	Technology Promotion Association (Thailand-Japan)	21CH1470	21 Oct 21	20 Oct 22	-

Certificate of Calibration

Calibration Certification Information				
Cal. Date:	July 27, 2020	Rootmeter S/N:	438320	Ta: 298 °K
Operator:	Jim Tisch	Pa:	749.3	mm Hg
Calibration Model #:	TE-5025A	Calibrator S/N:	3393	

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.3980	3.2	2.00
2	3	4	1	0.9960	6.3	4.00
3	5	6	1	0.8860	7.8	5.00
4	7	8	1	0.8430	8.7	5.50
5	9	10	1	0.7000	12.7	8.00

Data Tabulation					
Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9817	0.7022	1.4042	0.9957	0.7123	0.8919
0.9776	0.9816	1.9859	0.9916	0.9956	1.2613
0.9757	1.1012	2.2203	0.9896	1.1169	1.4101
0.9745	1.1560	2.3286	0.9884	1.1725	1.4790
0.9692	1.3846	2.8084	0.9831	1.4044	1.7837
m=		2.05151	m=		1.28462
b=		-0.03558	b=		-0.02260
r=		0.99994	r=		0.99994

Calculations			
Vstd=	$\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$	Va=	$\Delta Vol((Pa-\Delta P)/Pa)$
Qstd=	$Vstd/\Delta Time$	Qa=	$Va/\Delta Time$
For subsequent flow rate calculations:			
Qstd=	$1/m \left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} - b \right)$	Qa=	$1/m \left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} - b \right)$

Standard Conditions	
Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH:	calibrator manometer reading (in H2O)
ΔP:	rootsmeter manometer reading (mm Hg)
Ta:	actual absolute temperature (°K)
Pa:	actual barometric pressure (mm Hg)
b:	intercept
m:	slope

RECALIBRATION	
US EPA recommends annual recalibration per 1998	
40 Code of Federal Regulations Part 50 to 51,	
Appendix B to Part 50, Reference Method for the	
Determination of Suspended Particulate Matter in	
the Atmosphere, 9.2.17, page 30	

Tisch Environmental, Inc.
145 South Miami Avenue
Village of Cleves, OH 45002

www.tisch-env.com
TOLL FREE: (877)263-7610
FAX: (513)467-9009

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No.: 22P801
Page: 1 of 2

Equipment: U Tube Manometer

Manufacturer: Dwyer

Model: 1221-36-W/M

Serial No.: -

ID No.: UAE.EFM.178/2561

Condition As-Received: Used Item

Received Date: 03 March 2022

Calibration Date: 12 March 2022

Reference: 2203-0131WSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1010 mbar

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P04, using * DKD-R 6-1; Calibration of Pressure Gauges, Edition 03/2014 * as a guidelines.

Condition of this result of calibration

1.Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0110-21	09 Aug 2022
2.This result of calibration was made on requested at the point specified by customer.				
3.Scale and conversion factor is 1 kPa = 4.0146293 inH2O				
4.This instrument was used clean air as pressure media.				
5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.				
6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.				
7.The certificate is valid only to the item calibrated on date and place of calibration.				
8.This Certification is traceable to the International System of Unit maintained at:-				
-National Institute of Metrology Thailand (NIMT)				

Calibrated by: Suwit Aussarree
Issue Date: 14 March 2022

Approved Signatory: Attapol P.
[] Phalinee Prabpaipal
[] Sura Suwannasri
[x] Attapol Panurach

เอกสารไม่ควบคุม
B 0282414



Cert.No.: 22P801
Page: 2 of 2

Result of calibration:- Without adjustment

Function:- Pressure Measurement

Increasing Pressure

Range: 0 inH2O to 36 inH2O

Scale Interval: 0.1 inH2O (The Fifth Estimate)

UUC Indication				
Applied Pressure (inH2O)	High-port side (inH2O)	Low-port side (inH2O)	ΔP (inH2O)	Error (inH2O)
0.00	0.00	0.00	0.00	0.00
2.00	0.98	-0.94	1.92	-0.08
4.00	2.00	-1.98	3.98	-0.02
6.00	3.00	-2.98	5.98	-0.02
8.00	4.00	-3.98	7.98	-0.02
10.00	5.00	-4.98	9.98	-0.02
12.00	6.02	-5.96	11.98	-0.02
14.00	7.02	-6.96	13.98	-0.02
16.00	8.04	-7.98	16.02	0.02
18.00	9.04	-8.98	18.02	0.02
20.00	10.04	-9.98	20.02	0.02
22.00	11.06	-10.98	22.04	0.04
24.00	12.06	-12.00	24.06	0.06
26.00	13.06	-13.00	26.06	0.06
28.00	14.08	-14.02	28.10	0.10
30.00	15.08	-15.02	30.10	0.10
32.00	16.08	-16.04	32.12	0.12
34.00	17.10	-17.04	34.14	0.14
35.80	17.90	-17.86	35.76	-0.04

The uncertainty of measurement was ± 0.11 inH2O

* UUC = Unit Under Calibration

* ΔP = High-port side - Low-port side

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %.

-oOo-

เอกสารไม่ควบคุม
a 1099525



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No.: 21P2499
Page: 1 of 2

Equipment: Aneroid Barometer

Manufacturer: Barigo

Model: -

Serial No.: -

ID No.: UAE.ANV.122/2550

Condition As-Received: Used Item

Received Date: 20 July 2021

Calibration Date: 21 July 2021

Reference: 2107-0570WSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1009 mbar

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using * DKD-R 6-1; Calibration of Pressure Gauges, Edition 03/2014 * as a guidelines.

Condition of this result of calibration

1.Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DP1142	1422505046	MP-0053-21	08 Apr 2022
2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.				
3.This result of calibration was made on requested at the point specified by customer.				
4.This instrument was used clean air as pressure media.				
5.The certificate is valid only to the item calibrated on date and place of calibration.				
6.This Certification is traceable to the International System of Unit maintained at:-				
-National Institute of Metrology Thailand (NIMT)				

Calibrated by: Suwit Aussarree
Issue Date: 22 July 2021

Approved Signatory: Attapol P.
[] Phalinee Prabpaipal
[] Sura Suwannasri
[x] Attapol Panurach

เอกสารไม่ควบคุม
B 0264462



Cert.No.: 21P2499
Page: 2 of 2

Result of calibration:- Without adjustment

Range: 960 hPa to 1030 hPa

Function:- Absolute Pressure Measurement

Scale Interval: 1 hPa (The Fifth Estimate)

Increasing Pressure

Applied Pressure (hPa)	957.66	969.27	980.15	990.48	1000.69	1010.75	1020.58	1029.49
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0
Error (hPa)	2.34	0.73	-0.15	-0.48	-0.69	-0.75	-0.58	0.51

Decreasing Pressure

Applied Pressure (hPa)	1029.61	1020.69	1010.80	1000.75	990.59	980.30	969.41	957.79
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0
Error (hPa)	0.39	-0.69	-0.80	-0.75	-0.59	-0.30	0.59	2.21

The uncertainty of measurement was ± 0.30 hPa

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-00-

เอกสารไม่ควบคุม
a 1062243



United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaconsultant.com E-mail: uae@uaconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Nov 4, 2021

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1191503038

Standard Gas Concentration


Sulphur Dioxide (SO ₂)	44.75	PPM
Nitric Oxide (NO)	45.35	PPM
Methane (CH ₄)	-	PPM
Carbon Monoxide (CO)	1007	
Cylinder No. :	CC159599	
Expiration Date :	Jul 30, 2022	

Dilutor Detail

Manufacturer :	Thermo Scientific
Model :	146i
Serial Number :	1180540071

Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	1.1	1.10	1.10
Level 2	20.00%	100.0	101.1	1.10	1.09
Level 3	40.00%	200.0	201.3	1.30	0.65
Level 4	60.00%	300.0	301.5	1.50	0.50
Level 5	80.00%	400.0	400.6	0.60	0.15
Remark : Measuring Range	500.0 ppb			Average Difference (%)	0.70
				Acceptable Limit $\pm 5\%$	

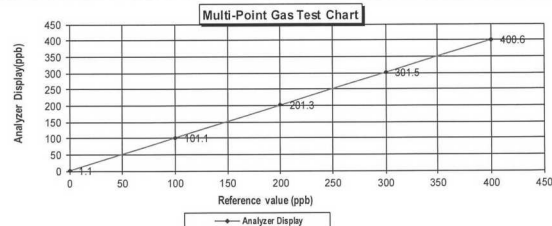

Calculate by
Sinchai Y.
10/11/21

Approve by
K. N. K.
10/11/21

Page 1 of 1

เอกสารไม่ควบคุม



United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaconsultant.com E-mail: uae@uaconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Nov 10, 2021


Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1201497724

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	44.75	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.35	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	1007			
Cylinder No. :	CC159599			
Expiration Date :	Jul 30, 2022			

Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	1.1	1.10	1.10
Level 2	20.00%	100.0	101.3	1.30	1.28
Level 3	40.00%	200.0	201.3	1.30	0.65
Level 4	60.00%	300.0	301.5	1.50	0.50
Level 5	80.00%	400.0	400.1	0.10	0.02
Remark : Measuring Range	500.0 ppb			Average Difference (%)	0.71
				Acceptable Limit $\pm 5\%$	

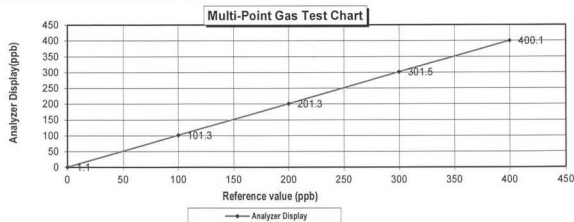

Calculate by
Sinchai Y.
10/11/21

Approve by
K. N. K.
10/11/21

Page 1 of 1

เอกสารไม่ควบคุม



United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaconsultant.com E-mail: uae@uaconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Nov 10, 2021


Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1201497725

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	44.75	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.35	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	1007			
Cylinder No. :	CC159599			
Expiration Date :	Jul 30, 2022			

Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.9	0.90	0.90
Level 2	20.00%	100.0	101.2	1.20	1.19
Level 3	40.00%	200.0	200.6	0.60	0.30
Level 4	60.00%	300.0	300.5	0.50	0.17
Level 5	80.00%	400.0	400.1	0.10	0.02
Remark : Measuring Range	500.0 ppb			Average Difference (%)	0.52
				Acceptable Limit $\pm 5\%$	

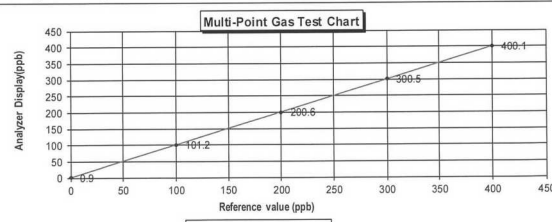

Calculate by
Sinchai Y.
10/11/21

Approve by
K. N. K.
10/11/21

Page 1 of 1

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Nov 17, 2021


Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1201497726

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.75 PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.35 PPM	Model :	146i
Methane (CH ₄)	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	1007		
Cylinder No. :	CC159599		
Expiration Date :	Jul 30, 2022		

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	1.2	1.20	1.20
Level 2 20.00%	100.0	101.4	1.40	1.38
Level 3 40.00%	200.0	201.3	1.30	0.65
Level 4 60.00%	300.0	300.9	0.90	0.30
Level 5 80.00%	400.0	400.2	0.20	0.05
Remark : Measuring Range	500.0 ppb	Average Difference (%)		0.72

Acceptable Limit $\pm 5\%$

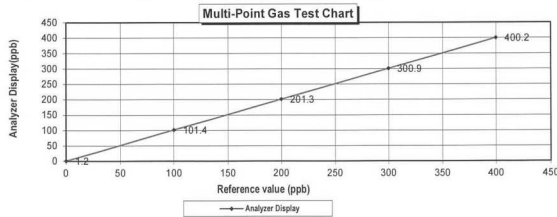

Calculate by
Srichai V.
22/11/21

Approve by
Petrak N.
22/Nov/2021

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04NI09E15A01D3 Reference Number: 122-402135167-1
Cylinder Number: EB0143262 Cylinder Volume: 144.4 CF
Laboratory: 124 - Durham (SAP) - NC Cylinder Pressure: 2015 PSIG
PGVP Number: B22021 Valve Outlet: 660
Gas Code: CO,NO,NOX,SO₂,BALN Certification Date: Jun 21, 2021

Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/331, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.
Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	$\pm 1.4\%$ NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	$\pm 1.4\%$ NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.88 PPM	G1	$\pm 1.0\%$ NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	$\pm 0.7\%$ NIST Traceable	06/14/2021
NITROGEN	Balance				

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20081120	CC708068	49.82 PPM NITRIC OXIDE/NITROGEN	$\pm 1.0\%$	Feb 02, 2025
PRM	12386	D85025	9.91 PPM NITROGEN DIOXIDE/AIR	$\pm 2.0\%$	Feb 20, 2020
GMIS	401423838102	CC505581	4.348 PPM NITROGEN DIOXIDE/NITROGEN	± 2.1	Feb 18, 2023
NTRM	16011043	CC473277	49.02 PPM SULFUR DIOXIDE/NITROGEN	$\pm 0.8\%$	Jun 17, 2022
NTRM	14060119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	$\pm 0.6\%$	Nov 15, 2025

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO ₂	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO ₂	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO #5221002807

GROSS WT: 28.40kg

NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

Approved for Release



เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Dec 7, 2021


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo Scientific Serial Number : 1200906876

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.75 PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	45.35 PPM	Model :	146i
Methane (CH ₄)	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	1007		
Cylinder No. :	CC159599		
Expiration Date :	Jul 30, 2022		

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	1.7	1.70	1.70
Level 2 20.00%	100.0	101.3	1.30	1.28
Level 3 40.00%	200.0	201.5	1.50	0.74
Level 4 60.00%	300.0	301.5	1.50	0.50
Level 5 80.00%	400.0	400.9	0.90	0.22
Remark : Measuring Range	500.0 ppb	Average Difference (%)		0.89

Acceptable Limit $\pm 5\%$

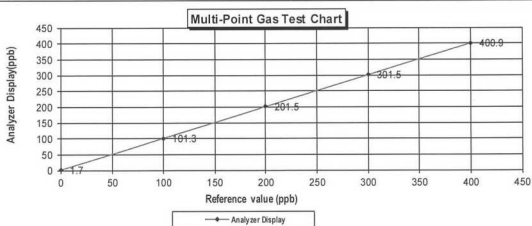

Calculate by
Srichai V.
22/12/21

Approve by
Petrak N.
22/Dec/2021

MULTI-POINT GAS TEST REPORT

Test Date : Nov 22, 2021


Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : 1182920012

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.75 PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	45.35 PPM	Model :	146i
Methane (CH ₄)	- PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	1007		
Cylinder No. :	CC159599		
Expiration Date :	Jul 30, 2022		

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	1.3	1.30	1.30
Level 2 20.00%	100.0	100.9	0.90	0.89
Level 3 40.00%	200.0	201.1	1.10	0.55
Level 4 60.00%	300.0	301.3	1.30	0.43
Level 5 80.00%	400.0	400.9	0.90	0.22
Remark : Measuring Range	500.0 ppb	Average Difference (%)		0.68

Acceptable Limit $\pm 5\%$

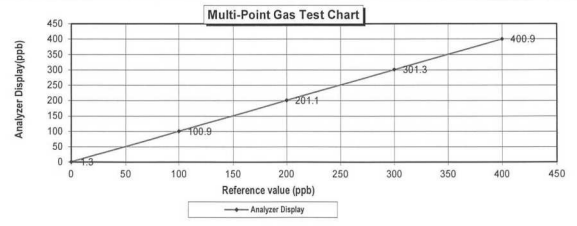

Calculate by
Srichai V.
22/11/21

Approve by
Petrak N.
22/Nov/2021

MULTI-POINT GAS TEST REPORT

Test Date : Nov 22, 2021

Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : 1182920013


Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.75 PPM Manufacturer : Thermo SCIENTIFIC
Nitric Oxide (NO) 45.35 PPM Model : 146i
Methane (CH₄) - PPM Serial Number : 1180540071
Carbon Monoxide (CO) 1007
Cylinder No. : CC159599
Expiration Date : Jul 30, 2022

Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	1.50	1.50	1.50
Level 2	20.00%	100.0	1.30	1.28	1.28
Level 3	40.00%	200.0	1.40	0.70	0.70
Level 4	60.00%	300.0	0.90	0.30	0.30
Level 5	80.00%	400.0	0.50	0.12	0.12
Remark : Measuring Range	500.0 ppb		Average Difference (%)		0.78

:Acceptable Limit $\pm 5\%$

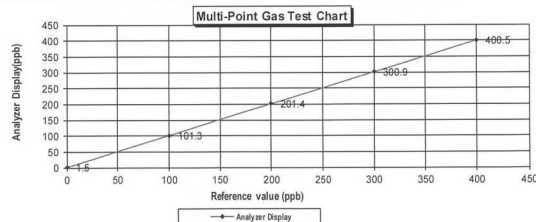

Calculate by
Sirichai Y.
22 Nov 2021

Approve by
Pattana U.
22 Nov 2021

MULTI-POINT GAS TEST REPORT

Test Date : Nov 22, 2021

Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : 1182920014


Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.75 PPM Manufacturer : Thermo SCIENTIFIC
Nitric Oxide (NO) 45.35 PPM Model : 146i
Methane (CH₄) - PPM Serial Number : 1180540071
Carbon Monoxide (CO) 1007
Cylinder No. : CC159599
Expiration Date : Jul 30, 2022

Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.90	0.90	0.90
Level 2	20.00%	100.0	1.10	1.09	1.09
Level 3	40.00%	200.0	1.30	0.65	0.65
Level 4	60.00%	300.0	1.50	0.50	0.50
Level 5	80.00%	400.0	0.90	0.22	0.22
Remark : Measuring Range	500.0 ppb		Average Difference (%)		0.67

:Acceptable Limit $\pm 5\%$

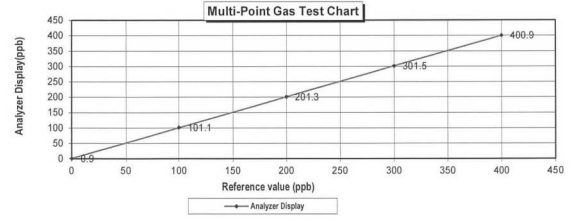

Calculate by
Sirichai Y.
22 Nov 2021

Approve by
Pattana U.
22 Nov 2021



Airgas Specialty Gases
Airgas USA, LLC
690 United Drive
Durham, NC 27713
airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04NI99E15A01D3 Reference Number: 122-402135167-1
Cylinder Number: EB0143262 Cylinder Volume: 144.4 CF
Laboratory: 124 - Durham (SAP) - NC Cylinder Pressure: 2015 PSIG
PGVP Number: B22021 Valve Outlet: 660
Gas Code: CO,NO,NOX,SO₂,BALN Certification Date: Jun 21, 2021

Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/331, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a notermole basis unless otherwise noted.
Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	08/14/2021, 08/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	08/14/2021, 08/21/2021
SULFUR DIOXIDE	45.00 PPM	44.86 PPM	G1	+/- 1.0% NIST Traceable	08/14/2021, 08/21/2021
CARBON MONOXIDE	1000 PPM	984.6 PPM	G1	+/- 0.7% NIST Traceable	08/14/2021
NITROGEN	Balance				

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20081120	CC708068	48.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D685025	9.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMIS	401423838102	CC505581	4.348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 16, 2023
NTRM	16011043	CC473277	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14080119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Nov 15, 2025

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO ₂	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO ₂	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO #5221002807
GROSS WT: 28.40kg
NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

Approved for Release



เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Nov 24, 2021

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1200636464


Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.75 PPM Manufacturer : Thermo Scientific
Nitric Oxide (NO) 45.35 PPM Model : 146i
Methane (CH₄) - PPM Serial Number : 1180540071
Carbon Monoxide (CO) 1007
Cylinder No. : CC159599
Expiration Date : Jul 30, 2022

Multi-point gas test data

	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	1.2	1.2	1.2
Level 2	20.00%	10.0	1.5	4.8	4.8
Level 3	40.00%	20.0	20.6	2.9	2.9
Level 4	60.00%	30.0	30.3	1.0	1.0
Level 5	80.00%	40.0	40.4	1.0	1.0
Remark : Measuring Range	50.0 ppm		Average Difference (%)		2.17

:Acceptable Limit $\pm 5\%$

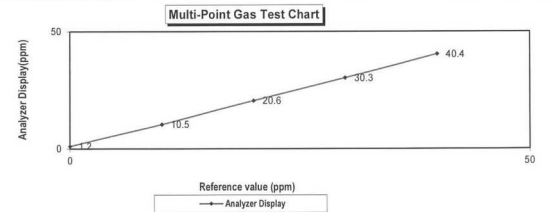

Calculate by
Sirichai Y.
24 Nov 2021

Approve by
Pattana U.
24 Nov 2021

MULTI-POINT GAS TEST REPORT

Test Date : Nov 24, 2021

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1200636465

Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.75 PPM
Nitric Oxide (NO) 45.35 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 1007 PPM
Cylinder No. : CC159599
Expiration Date : Jul 30, 2022


Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Level	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	% Error
Level 1	Zero	0.0	0.9	0.9	0.9
Level 2	20.00%	10.0	10.2	0.2	2.0
Level 3	40.00%	20.0	20.3	0.3	1.5
Level 4	60.00%	30.0	30.6	0.6	2.0
Level 5	80.00%	40.0	40.8	0.8	2.0

Remark : Measuring Range 50.0 ppm
Average Difference (%) 1.65
Acceptable Limit $\pm 5\%$

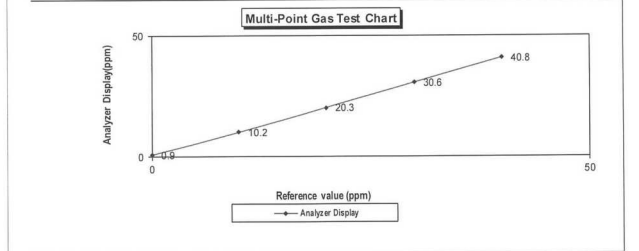

Calculate by *Sinchar*
24/11/21

Approve by *24 Nov 2021*

MULTI-POINT GAS TEST REPORT

Test Date : Nov 24, 2021

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1200636466

Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.75 PPM
Nitric Oxide (NO) 45.35 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 1007 PPM
Cylinder No. : CC159599
Expiration Date : Jul 30, 2022


Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Level	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	% Error
Level 1	Zero	0.0	1.0	1.0	1.0
Level 2	20.00%	10.0	10.4	0.4	3.8
Level 3	40.00%	20.0	20.2	0.2	1.0
Level 4	60.00%	30.0	30.4	0.4	1.3
Level 5	80.00%	40.0	40.6	0.6	1.5

Remark : Measuring Range 50.0 ppm
Average Difference (%) 1.73
Acceptable Limit $\pm 5\%$

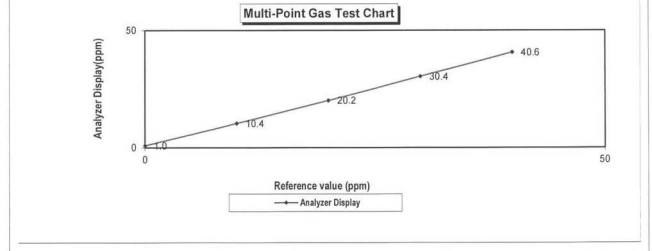

Calculate by *Sinchar*
24/11/21

Approve by *24 Nov 2021*

MULTI-POINT GAS TEST REPORT

Test Date : Nov 24, 2021

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1200636467

Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.75 PPM
Nitric Oxide (NO) 45.35 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 1007 PPM
Cylinder No. : CC159599
Expiration Date : Jul 30, 2022


Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Level	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	% Error
Level 1	Zero	0.0	1.3	1.3	1.3
Level 2	20.00%	10.0	10.7	0.7	6.5
Level 3	40.00%	20.0	20.5	0.5	2.4
Level 4	60.00%	30.0	30.7	0.7	2.3
Level 5	80.00%	40.0	40.9	0.9	2.2

Remark : Measuring Range 50.0 ppm
Average Difference (%) 2.95
Acceptable Limit $\pm 5\%$

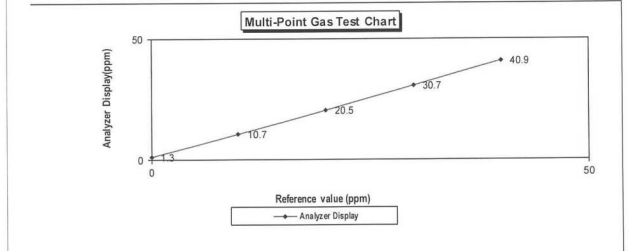

Calculate by *Sinchar*
24/11/21

Approve by *24 Nov 2021*

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04NI09E15A01D3
Cylinder Number: EB0143282
Laboratory: 124 - Durham (SAP) - NC
Gas Code: CO, NO, NOX, SO₂, BALN
Reference Number: 122-402135167-1
Cylinder Volume: 144.4 CF
Cylinder Pressure: 2015 PSIG
Valve Outlet: 660
Certification Date: Jun 21, 2021
Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/331, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	08/14/2021, 08/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	08/14/2021, 08/21/2021
SULFUR DIOXIDE	45.00 PPM	44.86 PPM	G1	+/- 1.0% NIST Traceable	08/14/2021, 08/21/2021
CARBON MONOXIDE	1000 PPM	984.6 PPM	G1	+/- 0.7% NIST Traceable	08/14/2021
NITROGEN	Balance				

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20081120	CC708068	48.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D685025	9.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2025
GMIS	401423838102	CC505581	4.348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 16, 2023
NTRM	16011043	CC473277	48.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14060119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Nov 15, 2025

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO2	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO2	FTIR	Jun 03, 2021

Triad Data Available Upon Request
NOTES: PO #5221002807
GROSS WT: 28.40kg
NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

Approved for Release



เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 16 August, 2021

Certification No. 385/21

Page : 1 of 7

Object : เครื่องมือตรวจวัดอุตุนิยมวิทยา

Manufacturer : LSI

Type : Dato Logger E-LOG 305 wind speed and wind direction DNA 827
Thermogrometers DMA875 Barometer DQA 801

Mfg Code : Dato Logger 19040308 wind speed and wind direction 19020211
Thermogrometers 19010187 Barometer 19040219

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1011.2 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02848057 : Thermoschneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB330 No. 1220015

: Digital Barometer Vaisala Type PTB330 No. 1220001

Calibrated by : Watcharapol Subwat

Signed : Mr. Pisood Promsut

(Authorised Signatory)

for the Chief
Sub-Standard Instrument

Mechanical Engineer



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Wind Speed And Wind Direction

Certification No. 385/21

16 August, 2021

Model DNA821 S/N

19020211

Page : 2 of 7

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacuum	Pressure	Velocity	Correction
Ultrasonic Anemometer	m/sec	inches	inches	hPa	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	2.7	0.32
5.00	-	-	-	5.0	0.00
7.04	-	-	-	6.7	0.34
9.02	-	-	-	9.0	0.02
11.02	-	-	-	10.7	0.32
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.7	0.31
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.7	0.32

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	

Calibrated by : Watcharapol Subwat

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 20 July, 2021

Certification No. 354/21

Page : 1 of 7

Object : เครื่องมือตรวจวัดอุตุนิยมวิทยา

Manufacturer : LSI

Type : Dato Logger E-LOG 305 wind speed and wind direction DNA 827
Thermogrometers DMA875 Barometer DQA 801

Mfg Code : Dato Logger 19040406 wind speed and wind direction 19020214
Thermogrometers 19050007 Barometer 19040190

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1007.8 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02848057 : Thermoschneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB330 No. 1220015

: Digital Barometer Vaisala Type PTB330 No. 1220001

Calibrated by : Watcharapol Subwat

Signed : Mr. Pisood Promsut

(Authorised Signatory)

for the Chief
Sub-Standard Instrument

Mechanical Engineer



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Wind Speed And Wind Direction

Certification No. 354/21

20 July, 2021

Model DNA821 S/N

19020214

Page : 2 of 7

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacuum	Pressure	Velocity	Correction
Ultrasonic Anemometer	m/sec	inches	inches	hPa	m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.9	0.10
7.04	-	-	-	6.7	0.34
9.02	-	-	-	8.9	0.12
11.02	-	-	-	10.7	0.32
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.7	0.31
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.7	0.32

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	

Calibrated by : Watcharapol Subwat

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 21-ACT-327
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Request No : Req-2021-0995
Prakanong, Bangkok 10260

Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 2
Manufacturer : LARSON DAVIS Range : 94 , 114 dB / 1000 Hz
Model : CAL150 Instrument Status : Used
Serial Number : 6171
ID : UAE.EFM.117/2562

Calibration Environment and Details


Temperature : (23 ± 2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ± 10.0 hPa)
Received Date : 22 July 2021
Calibration Date : 24 August 2021
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEL	14 May 2022
THD Multimeter	2015	1047765	NIMT	21 January 2022

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor
Issue Date : 24 August 2021

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม 07/19

Certificate No : 21-ACT-327
Request No : Req-2021-0995

Sound pressure level Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 2 (± dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	94.10	0.10	-	-	0.12	0.40
114 dB / 1000 Hz	114.12	0.12	-	-	0.11	0.40

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 2 (± %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.10	1.7
114 dB / 1000 Hz	1000.00	0.00	-	-	0.10	1.7

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 2 (± %)
	Measured (%)	Measured (%)		
94 dB / 1000 Hz	0.04	-	0.40	3.0
114 dB / 1000 Hz	0.21	-	0.40	3.0

Note :

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม 07/19

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



Cert. No. : ACL22088
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01010782 / 194537 / 14660
ID No.: -

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 11 APRIL 2022
Calibration Date : 18-22 APRIL 2022
Date of Issue : 25 APRIL 2022

Calibrated by : Nathakorn Pisutpaisan

Approved by :


(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL22088
Job No. : VC65AC0045
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม

Continuation of Calibration Certificate

Cert. No. : ACL22088
Job No. : VC65AC0045
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. R. K.

Continuation of Calibration Certificate

Cert. No. : ACL22088
Job No. : VC65AC0045
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. R. K.

Continuation of Calibration Certificate

Cert. No. : ACL22088
Job No. : VC65AC0045
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93,95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.0
C - weight	18.8
Flat	24.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.4	0.5	0.5	±5.0

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. R. K.

Continuation of Calibration Certificate

Cert. No. : ACL22088
Job No. : VC65AC0045
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. R. K.

Cert. No. : ACL22088
Job No. : VC65AC0045
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.4	-1.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. PetchurSITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY451-451/1 Sirinthorn Rd., Bangbunmru, Bangplud Bangkok 10700 THAILAND.
Tel: 0-2435-8800 Fax: 0-2433-1679 e-mail: cal-center@sithiporn.com http://www.sithiporn.comCert. No. : ACL22089
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01010783 / 194538 / 14661
ID No.: -

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 11 APRIL 2022
Calibration Date : 18-22 APRIL 2022
Date of Issue : 25 APRIL 2022

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

Cert. No. : ACL22088
Job No. : VC65AC0045
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. PetchurSITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORYCert. No. : ACL22089
Job No. : VC65AC0045
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม
T. Petchur

QF-TS12-04-04-020664

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. Petch

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	-0.1	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. Petch

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.7

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.6
C - weight	18.6
Flat	23.8

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.1	0.1	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-0.7	-0.7	-0.7	±5.0

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. Petch

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. Petch

Cert. No. : ACL22089
Job No. : VC65AC0045
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.0	-0.4	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. PetchurSITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY451-451/1 Sirinthorn Rd.,Bangbunrum, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.comCert. No. : ACL22090
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01010784 / 194539 / 14662
ID No.: -

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 11 APRIL 2022
Calibration Date : 18-22 APRIL 2022
Date of Issue : 25 APRIL 2022

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

QF-TS12-04-04-020664

Cert. No. : ACL22089
Job No. : VC65AC0045
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. PetchurCert. No. : ACL22090
Job No. : VC65AC0045
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM). The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม
T. Petchur

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL22090
Job No. : VC65AC0045
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. R. K.

Continuation of Calibration Certificate

Cert. No. : ACL22090
Job No. : VC65AC0045
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. R. K.

Continuation of Calibration Certificate

Cert. No. : ACL22090
Job No. : VC65AC0045
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.0
C - weight	18.5
Flat	24.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-0.9	-0.9	-0.8	±5.0

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. R. K.

Continuation of Calibration Certificate

Cert. No. : ACL22090
Job No. : VC65AC0045
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. R. K.

Cert. No. : ACL22090
Job No. : VC65AC0045
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.3	-1.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. K.

Cert. No. : ACL22090
Job No. : VC65AC0045
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.7	89.5	-0.2	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. K.



Cert.No.: 22CH60
Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : EcoSense
Model : pH100A
Serial No. : JC03354
ID No. : UAE.EFM.063/2562(ENV.pH 03/62)
Condition As-Received: Used Item
Received Date : 12 January 2022
Calibration Date : 13 January 2022
Reference : 2201-0350WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard
voltage calibrator and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lerngagtrakul

Approved by :
Approved Signatory

(/) Malee Butkruea
() Sathip Meangmai
() Warakorn Lerngagtrakul

Issue Date : 17 January 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Condition of this calibration result

1. Reference Standard Instrument : -

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	21E2682	25 Aug 2022
2) Ref. Standard Thermometer	4982054	110RC044	21I1201	26 Oct 2022

This certification is traceable to the International System of Unit maintained at:-
- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	766820	23 Sep 2023
pH 6.982	CPA chem	761017	02 Aug 2022
pH 10.015	CPA chem	766824	04 Sep 2022

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7),(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
			mV	pH		
pH Meter S/N.: JC03354	4.00	177.48	177	4.01	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-178	10.01	0.58	2.00

เอกสารไม่ควบคุม



Cert.No.: 22CH60
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7),(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor k
pH Electrode S/N.:200729SIA605377	4.008	4.01	144	0.0079	2.00
	6.982	6.98	-28	0.011	2.00
	6.982	6.98	-27	0.0099	2.00
	10.015	10.01	-200	0.0096	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model :
- Serial No. : 200729SIA605377

Dimension of probe;

- Length : 112 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
25.0	25.003	25.1	0.097	0.13	2.00
30.0	30.002	30.1	0.098	0.13	2.00
35.0	35.004	35.0	-0.004	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



Cert.No.: 21CH1470
Page.: 1 of 3

Certificate of Calibration

Equipment : Conductivity Meter
Manufacturer : YSI
Model : Pro 30
Serial No. : 18C105225
ID No. : UAE.EFM.206/2561(ENV.SCT.04/61)
Condition As-Received: Used Item
Received Date : 19 October 2021
Calibration Date : 21 October 2021
Reference : 2110-0604WSC-4
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In -house method :
- CP-CH6 by direct measurement
with certified reference material (CRM)
- CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lerngagtrakul

Approved by :
Approved Signatory

(/) Malee Butkruea
() Sathip Meangmai
() Warakorn Lerngagtrakul

Issue Date : 29 October 2021

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0033914



Cert.No.: 21CH1470

Page.: 2 of 3

Condition of this result of calibration**1. Reference Standard Instrument :-**

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	1963878	130RC095	211977	17 Sep 2022
2) Ref. Std. Thermometer	3240076	60RC033	211193	14 Feb 2022

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1413.0 $\mu\text{S/cm}$	CPA Chem	761021	02 Aug 2022
12.8806 mS/cm	CPA Chem	754037	28 June 2022

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results**Function : Conductivity Measurement**(*) After Adjustment at 1413.0 $\mu\text{S/cm}$

Conductivity Electrode Serial No.: 18C100559

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (\pm)	Coverage factor k
1413.0 $\mu\text{S/cm}$	1390 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	9.1 $\mu\text{S/cm}$	2.00
12.8806 mS/cm	12.73 mS/cm	12.85 mS/cm	0.082 mS/cm	2.00

Remark - UUC* = Unit Under Calibration

Malu .
เอกสารไม่ควบคุม
a 1079152



Cert.No.: 21CH1470

Page.: 3 of 3

Calibration Results**Function : Temperature Measurement**

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : PRO 30 COND-T

- Serial No. 18C100559

Dimension of probe;

- Length : 8 mm.

- Diameter : 2.5 mm.

- Immersion Depth : 80 mm.

Calibration Point ($^{\circ}\text{C}$)	Standard Temperature ($^{\circ}\text{C}$)	UUC* Reading ($^{\circ}\text{C}$)	Error ($^{\circ}\text{C}$)	Uncertainty of Measurement (\pm $^{\circ}\text{C}$)	Coverage factor k
25.0	25.005	25.0	-0.005	0.20	2.00
30.0	30.004	30.0	-0.004	0.20	2.00
35.0	35.004	35.0	-0.004	0.20	2.00

Remark : - UUC* = Unit Under CalibrationThe reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Malu .
เอกสารไม่ควบคุม
a 1079151

ใบรับรองสอบเทียบเครื่องมือประจำห้องปฏิบัติการ สำหรับตรวจวัดคุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือประจำห้องปฏิบัติการวิเคราะห์ สำหรับวิเคราะห์คุณภาพอากาศในบรรยากาศโดยทั่วไป									
1	Analytical Balance (Readability 0.1 mg)	ฝุ่นละอองรวม (TSP) ฝุ่นละอองขนาดเล็กไม่เกิน 10 ไมครอน	Mettler-Toledo	AB204-S / 1128312528	National Food Institute, Ministry of Industry, Thailand	2200704-001-01	24 Nov 21	23 Nov 22	-
2	Analytical Balance (Readability 0.1 mg)	(PM-10)	Mettler-Toledo	AB204-S/FACT / B108115858	National Food Institute, Ministry of Industry, Thailand	2102572-001-01	26 Apr 21	25 Apr 22	-
เครื่องมือประจำห้องปฏิบัติการวิเคราะห์ สำหรับวิเคราะห์คุณภาพน้ำ									
3	Inductively Coupled Plasma- Optical Emission (ICP-OES)	กลุ่มโลหะหนัก : ตะกั่ว (Pb), นิกเกิล (Ni), แบเรียม (Ba), ปรอททั้งหมด (Total Hg), ซีลีเนียม (Se),	Agilent Technologies	System ID:G8015A G8015AA / MY18030001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	9 Dec 21	8 Dec 22	-
4	Atomic Absorption Spectrometer (AAS)	ทองแดง (Cu),แมงกานีส (Mn),สังกะสี (Zn), เหล็ก (Fe), สารหนู (As), แคดเมียม (Cd), โครเมียมเฮกซะวาเลนท์ (Cr6+)	Agilent Technologies	System ID:G8432A AA240FS / MY13160001	Thailand Institute of Scientific and Technological Research (TISTR).	MTC.ACL. No. 335/64	28 Jan 22	27 Jan 23	-
5	Conductivity Meter	การนำไฟฟ้า(EC) ความเค็ม (Salinity)	SI Analytics	Lab955 / 16300356	SPC Calibration Center Co.,Ltd.	C24210091	29 Mar 21	28 Mar 22	-
6	pH Meter	ค่าความเป็นกรด-ด่าง (pH) อุณหภูมิ (Temperature)	Mettler-Toledo	Seven Easy S20 / 1231155210	National Food Institute, Ministry of Industry, Thailand	2103189-002-01	14 Jun 21	13 Jun 22	-
7	pH Meter		Hanna Instrument	HI2211 / 8165345	National Food Institute, Ministry of Industry, Thailand	2102015-001-01	17 Mar 21	16 Mar 22	-

ใบรับรองสอบเทียบเครื่องมือประจำห้องปฏิบัติการ สำหรับตรวจวัดคุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือประจำห้องปฏิบัติการวิเคราะห์ สำหรับวิเคราะห์คุณภาพน้ำผิวดิน และน้ำใต้ดิน									
8	Analytical Balance (Readability 0.1 mg)	ปิโตรเลียมไฮโดรคาร์บอนทั้งหมด (TPH), น้ำมันและไขมัน (Oil & Grease)	Mettler-Toledo	AB-204S/FACT / 1129361010	National Food Institute, Ministry of Industry, Thailand	2103270-001-01	11 Jun 21	10 Jun 22	-
9	Analytical Balance (Readability 0.01 mg)	ของแข็งแขวนลอย (Total Suspended Solids : TSS)	Mettler-Toledo	AX105DR / 1122100406	National Food Institute, Ministry of Industry, Thailand	2200708-001-01	24 Nov 21	23 Nov 22	-
10	Hot Air Oven	ของแข็งละลายน้ำทั้งหมด (Total Dissolved Solids : TDS)	Memmert	UF55 / B216.1666	Technology Promotion Association (Thailand-Japan)	21TM1876	29 Oct 21	28 Oct 22	-

Due Date of Calibration* : กำหนดตามแผนการสอบเทียบประจำปี อย่างน้อยปีละ 1 ครั้ง

Mettler-Toledo (Thailand) Ltd.
846/4 - 846/5 Lasalle Rd., Bangna Tai Sub-District
Bangna District, Bangkok 10260
+66 2723 0382
MT-TH.ServiceSupport@mt.com



Accuracy Calibration Certificate

Customer

Company: United Analyst and Engineering Consultant Co., Ltd.
Address: 3 Soi Udom Suk 41, Sukhumvit Rd., Bang Chak
City: Phra Khanong Contact: Suwit Chotnolk
Zip / Postal: 10260
State / Province: Bangkok
Order Number: 

Weighing Device



Manufacturer: Mettler Toledo Instrument Type: Weighing Instrument
Model: AB204-S Asset Number: UAE.AIR.019/2550
Serial No.: 1128312528 Terminal Model: N/A
Building: N/A Terminal Serial No.: N/A
Floor: 2 Terminal Asset No.: N/A
Room: Balance Room 2 (206)

Range	Max. Capacity	Readability (d)
1	220 g	0.0001 g

Procedure

Calibration Guideline: EURAMET cg-18 v. 4.0 (11/2015)
METTLER TOLEDO Work Instruction: CP/W002/20
This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.
The sensitivity/span of the weighing instrument was adjusted before calibration with a built-in weight.
In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.


As Found	Temperature	Humidity
Start: 22.5 °C	End: 21.4 °C	Start: 56.1 %
		End: 63.2 %

As Found Calibration Date: 07-Apr-2022 Calibrator: 
As Left Calibration Date: N/A
Issue Date: 08-Apr-2022
Approved Signatory: 
☒ Kassakorn Tassanachaisakul
☐ Santi Jitniyom
☐ Surachet Sukkate

เอกสารไม่ควบคุม

Error of Indication

As Found	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.0000 g	0.0000 g	0.0000 g	0.18 mg	2
2	0.1000 g	0.1000 g	0.0000 g	0.19 mg	2
3	1.0000 g	0.9999 g	-0.0001 g	0.19 mg	2
4	5.0000 g	5.0000 g	0.0000 g	0.19 mg	2
5	10.0000 g	9.9999 g	-0.0001 g	0.20 mg	2
6	20.0000 g	20.0000 g	0.0000 g	0.21 mg	2
7	50.0000 g	50.0000 g	0.0000 g	0.23 mg	2
8	70.0001 g	70.0000 g	-0.0001 g	0.28 mg	2
9	100.0000 g	100.0000 g	0.0000 g	0.29 mg	2
10	150.0000 g	150.0002 g	0.0002 g	0.40 mg	2
11	200.0001 g	200.0003 g	0.0002 g	0.46 mg	2

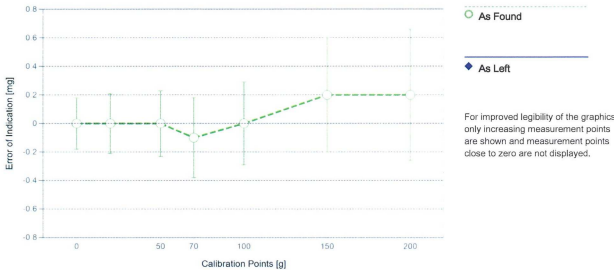

The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor k – which can be larger than 2 according to EURAMET cg-18. The value of the measurand lies within the assigned range of values with a probability of approximately 95%.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2

Weight Set No.: WS80 Date of Issue: 23-Feb-2022
Certificate Number: C208581631 Calibration Due Date: 14-Aug-2023

Thermo Hygrometer

Equipment No.: IN161 Date of Issue: 14-Jun-2021
Certificate Number: 21H1220 Calibration Due Date: 01-Jun-2022

เอกสารไม่ควบคุม

Measurement Results


Repeatability

Test Load: 100 g	As Found	As Left
1	99.9999 g	N/A
2	100.0000 g	N/A
3	99.9998 g	N/A
4	100.0000 g	N/A
5	99.9999 g	N/A
6	100.0000 g	N/A
7	99.9999 g	N/A
8	100.0001 g	N/A
9	99.9999 g	N/A
10	100.0000 g	N/A
Standard Deviation	0.00008 g	N/A



Eccentricity

Test Load: 100 g		
Position	As Found	As Left
1	100.0000 g	N/A
2	99.9998 g	N/A
3	99.9998 g	N/A
4	100.0001 g	N/A
5	100.0001 g	N/A
Maximum Deviation	0.0002 g	N/A



เอกสารไม่ควบคุม

Remarks

Equipment condition: Good
Next calibration according to customer's procedure
Calibration data not decide by calibration laboratory
Test weight by Filter pan : 1 g = 0.9999 g, 3 g = 3.0000 g, 5 g = 5.0000 g

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

เอกสารไม่ควบคุม

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with $k=2$ in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use: $3.0 \cdot 10^{-6} / K$

Temperature range on site for the evaluation of the measurement uncertainty in use: $3 K$


Linearization of Uncertainty Equation

Range			As Found	As Left
	d	Max		
1	0.0001 g	220 g	$U_1 = 0.19 \text{ mg} + 0.00817 \text{ mg/g} \cdot R$	N/A

To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty In Use for Various Net Indications (Examples)

Net Indication	As Found	As Found	As Left	As Left
0.0220 g	0.19 mg	0.86%	N/A	N/A
0.2200 g	0.19 mg	0.087%	N/A	N/A
2.2000 g	0.21 mg	0.0095%	N/A	N/A
22.0000 g	0.37 mg	0.0017%	N/A	N/A
220.0000 g	2.0 mg	0.00090%	N/A	N/A

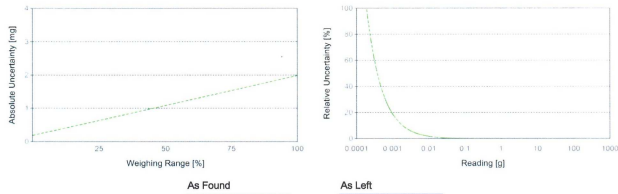

Mettler-Toledo (Thailand) Ltd.
846/4 - 846/5 Lasalle Rd., Bangna Tai Sub-District
Bangna District, Bangkok 10260
+66 2723 0382
MT-TH.ServiceSupport@mt.com



Accuracy Calibration Certificate

Customer

Company: United Analyst and Engineering Consultant Co., Ltd.
Address: 3 Soi Udom Suk 41, Sukhumvit Rd., Bang Chak
City: Phra Khanong
Zip / Postal: 10260
State / Province: Bangkok
Order Number:

Weighing Device

Manufacturer: Mettler Toledo
Model: AB204-S/FACT
Serial No.: B108115858
Building: N/A
Floor: 2
Room: Balance Room 2 (206)
Instrument Type: Weighing Instrument
Asset Number: UAE-AIR.016/2555
Terminal Model: N/A
Terminal Serial No.: N/A
Terminal Asset No.: N/A

Range	Max. Capacity	Readability (d)
1	220 g	0.0001 g

Procedure

Calibration Guideline: EURAMET cg-18 v. 4.0 (11/2015)
METTLER TOLEDO Work Instruction: CP/W002/20

This calibration certificate contains measurements for As Found and As Left calibrations.

The sensitivity/span of the weighing instrument was adjusted before As Found and As Left calibrations with a built-in weight.

In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

	Temperature		Humidity	
	Start	End	Start	End
As Found	22.6 °C	22.1 °C	56.0 %	51.9 %
As Left	22.3 °C	22.4 °C	46.2 %	55.8 %

As Found Calibration Date: 07-Apr-2022
As Left Calibration Date: 07-Apr-2022
Issue Date: 08-Apr-2022

Calibrator:
Approved Signatory:
☒ Kasakorn Tassanachaisakul
☐ Santi Jinyom
☐ Surachet Sukkate


Measurement Results

Repeatability

Test Load: 100 g

	As Found	As Left
1	100.0005 g	99.9999 g
2	100.0004 g	100.0000 g
3	100.0004 g	99.9999 g
4	100.0006 g	100.0000 g
5	100.0005 g	99.9999 g
6	100.0004 g	99.9998 g
7	100.0005 g	100.0000 g
8	100.0004 g	100.0000 g
9	100.0005 g	100.0000 g
10	100.0005 g	100.0000 g

Standard Deviation	0.00007 g	0.00007 g
--------------------	-----------	-----------

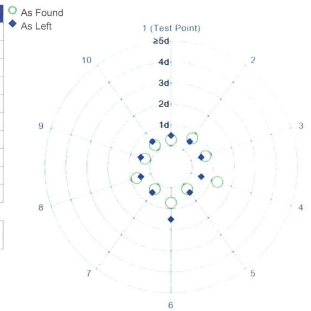


The "d" in the graph represents the readability of the range/interval in which the test was performed.
The results of this graph are based upon the absolute values of the differences from the mean value.

Eccentricity

Test Load: 100 g

Position	As Found	As Left
1	100.0005 g	100.0000 g
2	100.0003 g	99.9999 g
3	100.0003 g	99.9998 g
4	100.0007 g	100.0001 g
5	100.0007 g	100.0002 g

Maximum Deviation	0.0002 g	0.0002 g
-------------------	----------	----------

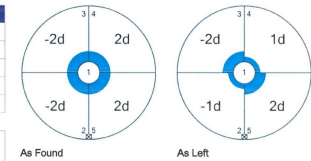

The "d" in the graph represents the readability of the range/interval in which the test was performed.

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2

Weight Set No.: WS80 Date of Issue: 23-Feb-2022
Certificate Number: C208581631 Calibration Due Date: 14-Aug-2023

Thermo Hygrometer

Equipment No.: IN161 Date of Issue: 14-Jun-2021
Certificate Number: 21H1220 Calibration Due Date: 01-Jun-2022

Remarks

FACT adjustment functionality activated
Value of the built-in weight adjusted
Equipment condition: Good
Next calibration according to customer's procedure
Calibration data not decide by calibration laboratory
Test weight by Filter pan : 1 g = 1.0000 g, 3 g = 3.0000 g, 5 g = 5.0000 g

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

เอกสารไม่ควบคุม

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with $k=2$ in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use: $2.5 \cdot 10^{-4} / K$
Temperature range on site for the evaluation of the measurement uncertainty in use: 3 K


Linearization of Uncertainty Equation

1	Range		As Found	As Left
	d	Max		
	0.0001 g	220 g	$U_1 = 0.16 \text{ mg} + 0.0111 \text{ mg/g} \cdot R$	$U_1 = 0.16 \text{ mg} + 0.00592 \text{ mg/g} \cdot R$

To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication	As Found	As Left
0.0220 g	0.16 mg, 0.73%	0.16 mg, 0.73%
0.2200 g	0.16 mg, 0.074%	0.16 mg, 0.073%
2.2000 g	0.18 mg, 0.0084%	0.17 mg, 0.0079%
22.0000 g	0.40 mg, 0.0018%	0.29 mg, 0.0013%
220.0000 g	2.6 mg, 0.0012%	1.5 mg, 0.00066%

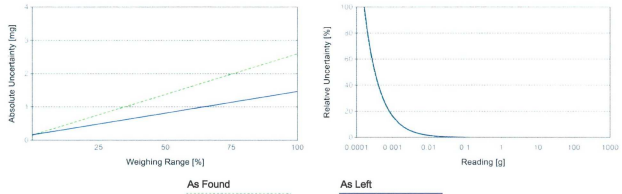

เอกสารไม่ควบคุม



Agilent 5110 and 5100 ICP-OES
Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical systems to assure reliable operation and the accuracy of your results. Delivered by highly-trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak.

For more information about Agilent Technologies services please visit our web site using the following URL <http://www.agilent.com/en-us/services/analytical-instrument-services>

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of additional or special procedures and/or parts for the instrument service, then these must be ordered separately and charged as a repair, which may incur additional

Service Engineer's Responsibilities

- Only complete/printout pages that relate to the system being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using a "X" or tick mark "✓" in the checkbox.
- Complete Not Applicable check boxes to indicate services not delivered, as needed.
- Complete the PM service in the order of the tasks listed.
- Complete the Service Review section together with the customer.

เอกสารไม่ควบคุม



Agilent 5110 and 5100 ICP-OES
Preventive Maintenance Checklist

System Information

Instrument system name and ID	ICP-OES 5100 v01
Instrument system site and location	UAE Consultant
List system component product numbers	List the serial numbers of each component
1. 83015A	1. MY19030001
2.	2.
3.	3.
4.	4.
5.	5.
6.	6.
7.	7.
8.	8.
9.	9.
10.	10.

ICP-OES Configuration table	Circle the type or write in the type if other
Nebulizer Type	SeaSpray OneNeb other
Spray Chamber	Cyclonic Single Pass Cyclonic Double Pass other
Torch	Radial Dual View other
Injector Diameter	2.4mm 1.8mm 1.4mm 0.8mm other
Injector Material	Quartz Ceramic other

เอกสารไม่ควบคุม