

ภาคผนวกที่ 4

ใบรับรองการสอบเทียบเครื่องมือ



National Institute of Metrology (Thailand)

Certificate of Calibration



Certificate No. : AA-2013-21
Issued by : Acoustics Laboratory
Acoustics and Vibration Group

Page 1 of 5 pages

MEASUREMENT ITEM : Sound Calibrator

MANUFACTURER : RION

MODEL/TYPE : NC-75

SERIAL NUMBER : 34480442

CUSTOMER : MET Co., Ltd.
36/659 Moo 6, T. Bangrakphatthana,
Bangbuathong, Nonthaburi 11110

MEASUREMENT DATE : 6 September 2021

*The calibration results only marked with an asterisk * in this certificate are not included in Appendix C of the MRA drawn up by the CIPM.*

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%. This calibration certificate may not be reproduced other than in full except with the permission of the Director of National Institute of Metrology (Thailand).

Reference
AUV084-01/21

Date
6 September 2021

Authorized Signatory

Person in charge



This certificate is consistent with the capabilities that are included in Appendix C of the MRA drawn up by the CIPM. Under the MRA, all participating institutes recognize the validity of each other's calibration and measurement certificates for the quantities, ranges and measurement uncertainties specified in Appendix C (for details see <http://www.bipm.org>).

National Institute of Metrology (Thailand)

Ministry of Higher Education, Science, Research and Innovation

3/4-5 Moo 3, Klong 5, Klong Luang, Pathumthani 12120, Thailand. Tel: (66) 2577 5100, Fax: (66) 2577 3659

75/7 Rama VI Road, Rachathewi, Bangkok 10400, Thailand. Tel: (66) 2354 3700, Fax: (66) 2354 3692



UNCERTAINTY OF MEASUREMENT

The stated uncertainty is the expanded uncertainty obtained by multiplying the standard uncertainty by the coverage factor $k=2$. It has been determined in accordance with EA publication EA-4/02 M:2013 "Evaluation of the Uncertainty of Measurement in Calibration" and JCGM 100:2008 "Evaluation of measurement data --Guide to the Expression of Uncertainty in Measurement (GUM 1995 with minor corrections)". The value of the measured lies within the assigned range of value with a probability of 95 %.

Parameter	Uncertainty at SPL94 dB	Maximum-permitted uncertainty of measurement for a coverage probability of 95%
1.Sound Pressure level	0.08	0.15
2. Frequency	0.1	0.2
3. THD+N	0.2	0.5

TRACEABILITY

This certificate provides traceability of measurement to recognized national standards, and to the realization of the International System of Units (SI).

NIMT



ENVIRONMENTAL CONDITIONS

Ambient condition in the laboratory are as follows :

Temperature	: (23.0 ± 1.0)	°C
Pressure	: (101.325 ± 1.500)	kPa
Relative Humidity	: (50.0 ± 15.0)	%

Reference Condition : 101.325 kPa , 23.0 °C and 50.0 %RH.

Calibration Condition

Preconditionings : 16 hours at ambient conditions.

Measurement Con : The average values during measurement are
(100.965 ± 0.013) kPa, (22.3 ± 0.3) °C and (62.2 ± 2.6) %RH

MEASUREMENT METHOD

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone. The insert voltage technique was employed and the measurement procedure was based on IEC 60942-2017.

Reference Microphone

B&K Type 4180 serial no.1395446

TABULATION OF RESULTS

The following tables give the calibration results and associated measurement uncertainties at 95% of confidence level. The calibration results of sound pressure level which quoted in dB with reference to 20 µPa are corrected to the values under the reference environmental conditions.

The microphone volume corrections and the calibrator pressure corrections are excluded in the calibration results.



MEASUREMENT RESULTS

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value ^[1] (dB)	Acceptance Limit (dB)
Microphone 4180 Serial No.1395446			
94	94.12	0.12	0.25

Note ^[1] : The deviated value is the absolute value of the difference between the measured value and the corresponding specified sound pressure level.

2. Frequency*

Specified Frequency (Hz)	Measured value (Hz)	Deviated value ^[2] (%)	Acceptance Limit (%)
At the sound pressure level of 94 dB			
1000	1000.0	0.0	0.7

Note ^[2] : The deviated value is the absolute value of the difference in percent between the measured value and the corresponding specified frequency.




3. Total distortion + Noise*

Microphone 4180 Serial No.1395446

Measured value ^[3] (%)	Maximum total distortion + Noise (%)
At the sound pressure level of 94 dB	
1.5	2.5

Note ^[3]: The measured value is the total distortion, measured over the frequency range from 20 Hz to 20 kHz. The measured value must not exceed the maximum total distortion + noise appeared in the table.

End of Certificate of Calibration

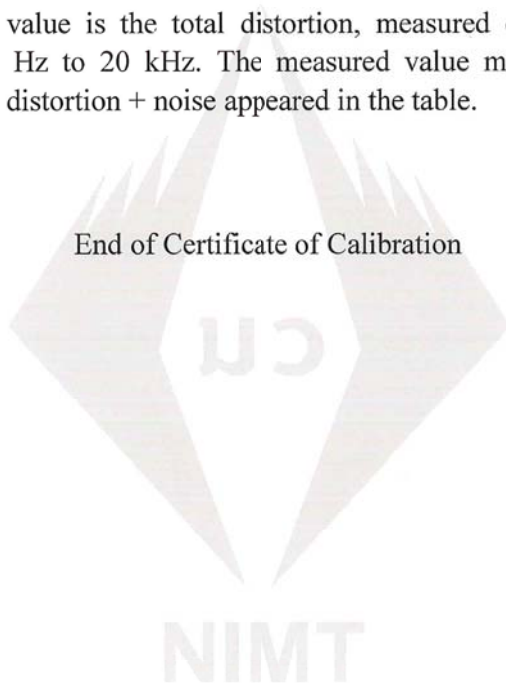



Certificate of Calibration

Certificate Number : SPR21120189- 1

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : Rion

Model : NL-21

Serial Number : 00722042

ID. Number : SLM-46

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 13 Dec 2021

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 13 Dec 2021

Location of Calibration : In-Lab

Recommend Due Date : 13 Dec 2022

Calibration Procedure : SP-CPE-04-01

Date of Issue : 14 Dec 2021

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Surasak Vakjan

Approved by :

Calibration Officer

Authorized Signatory



Calibration Report

Certificate Number : SPR21120189- 1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP.19/1063	15 Oct 2022

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR21120189-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select F

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR21120189-2

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : Rion

Model : NL-21

Serial Number : 00722043

ID. Number : SLM-45

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 13 Dec 2021

Calibration Date : 13 Dec 2021

Recommend Due Date : 13 Dec 2022

Date of Issue : 14 Dec 2021

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Surasak Vakjan

Calibration Officer

Approved by :



Authorized Signatory



Calibration Report

Certificate Number : SPR21120189-2

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP.19/1063	15 Oct 2022

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR21120189-2

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.1	114.1	0.1	0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.1	114.1	0.1	0.1	0.15

Select F

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.1	114.1	0.1	0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

– End of Certificate –

Certificate of Calibration

Certificate No. : 65-420003-2

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : pH Meter with electrode
pH meter
Manufacturer : Thermo Scientific Model : pH 150
Range : N/A pH Resolution : 0.01 pH
Serial No. : 2913288 ID No. : MET-PH05/63
Electrode
Model : N/A Serial No. : 48393

Environment : Ambient Temperature : $(25 \pm 2) ^\circ \text{C}$
Relative Humidity : $(50 \pm 15) \%$

Date of Received : 13 January 2022

Date of Calibration : 19 January 2022

Date of Issue : 19 January 2022

Calibrated by : Bunjerd Masri

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
440001	21E997	17 Mar 2023	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.004	61218215	769926	15 May 2022	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.985	61223875	769927	15 May 2022	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.963	61208865	769928	15 May 2022	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-420003-2

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement
pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.5	0.0	0.060
	0.0000	7	7.00	0.2	-0.2	0.058
	-177.4800	10	10.00	-177.2	-0.3	0.060

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.004	4.01	0.00	0.011
	6.985	7.00	-0.01	0.011
	9.963	10.01	-0.04	0.016

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o()o -



Certificate of Calibration

Certificate No. : 64-400425-5

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Incubator)

Manufacturer : M-LAB

Model : BIC-140

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 240412

ID No. : MET-BI01/55

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (31.0 to 33.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 23 August 2021

Date of Calibration : 23 August 2021

Date of Issue : 23 August 2021

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400032

64-400106-1

30 Sep 2021

National Institute of Metrology Thailand (NIMT)

Approved by :



Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 64-400425-5


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

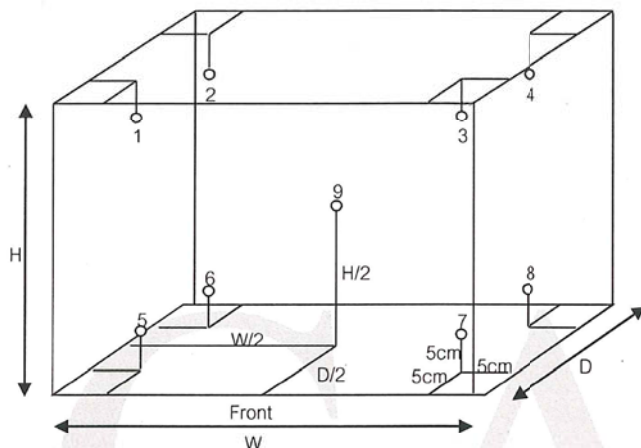

Inside of Chamber

W = 0.37 m

D = 0.33 m

H = 1.14 m

Capacity = 0.14 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	19.9	19.8	19.7	19.5	20.4	20.4	20.3	20.1	20.4	0.57

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	1.0	0.1	1.0

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 64-400425-7

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Refrigerator)

Manufacturer : Sanden Intercool

Model : SRR3-0687 AR

Range : N/A °C

Resolution : 1 °C

Serial No. : SRR3675A-210400065 R

ID No. : MET-RE04/64

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (28.6 to 30.5) °C

Relative Humidity : (55 to 58) %

Line Voltage : (220.0 to 220.8) V

Date of Received : 23 August 2021

Date of Calibration : 23 August 2021

Date of Issue : 23 August 2021

Calibrated by : Bunjerd Masri

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400022 & 400028	64-400103-1	02 Sep 2021	National Institute of Metrology Thailand (NIMT)

Approved by :



Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 64-400425-7


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

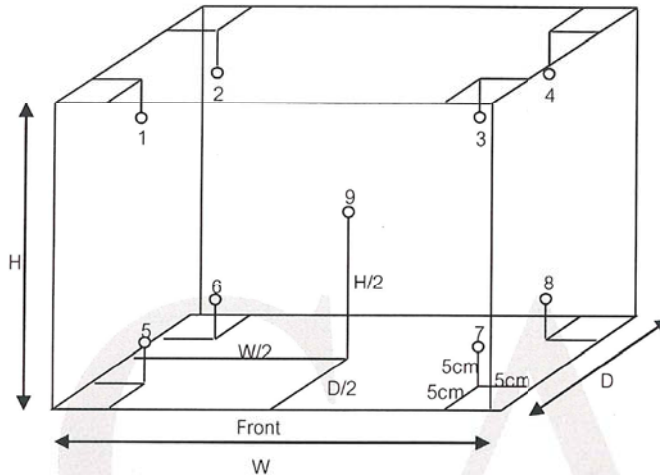

Inside of Chamber

W = 0.58 m

D = 0.60 m

H = 1.45 m

Capacity = 0.50 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
3	3	3	3.5	3.6	3.4	3.2	3.1	2.7	3.1	3.0	3.1	0.83

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
3	3	3	0.6	0.2	1.4

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 64-400425-2

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)

Manufacturer : Binder

Model : ED53

Range : N/A °C

Resolution : 1 °C

Serial No. : 13-07419

ID No. : MET-OV02/57

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (31.0 to 33.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 23 August 2021

Date of Calibration : 23 August 2021

Date of Issue : 23 August 2021

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400030	64-400104-1	29 Sep 2021	National Institute of Metrology Thailand (NIMT)

Approved by :

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 64-400425-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

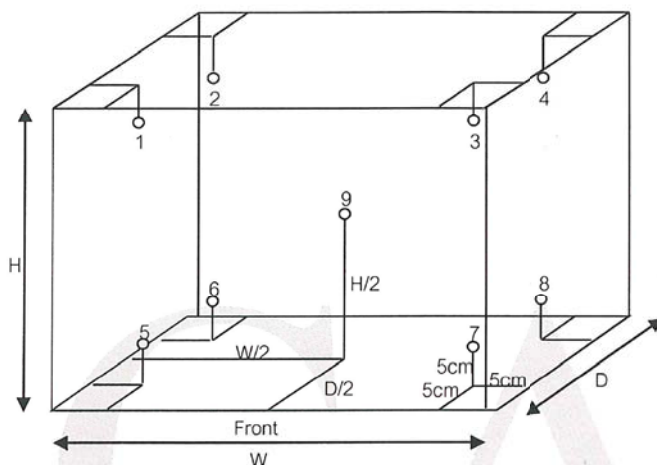

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.40 m

Capacity = 0.05 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104	109	109	104.8	105.0	104.4	104.6	103.4	103.5	103.6	103.7	103.7	0.96
180	184	184	180.8	181.8	179.9	180.6	180.6	180.8	180.6	180.9	180.5	1.1

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104	109	109	1.5	0.2	1.8
180	184	184	1.6	0.2	2.3

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 64-400425-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)

Manufacturer : Memmert

Model : UM 100

Range : N/A °C

Resolution : 0.1 °C

Serial No. : b197.0985

ID No. : MET-OV01/46

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (31.0 to 33.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 23 August 2021

Date of Calibration : 23 August 2021

Date of Issue : 23 August 2021

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400032	64-400106-1	30 Sep 2021	National Institute of Metrology Thailand (NIMT)

Approved by :



Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 64-400425-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

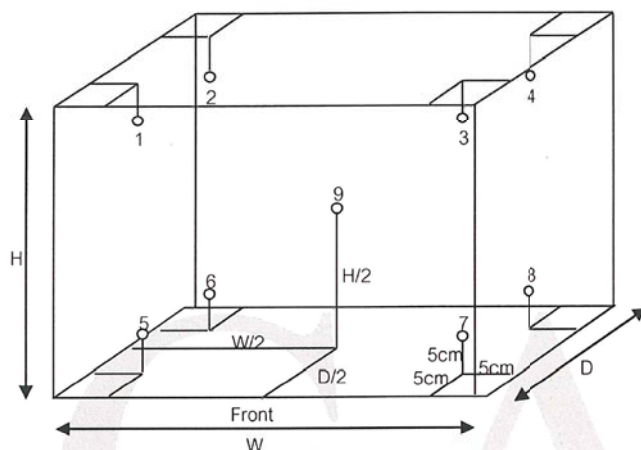

Inside of Chamber

W = 0.32 m

D = 0.18 m

H = 0.24 m

Capacity = 0.01 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
180.0	180.0	180.0	180.9	181.2	180.7	181.0	181.1	181.3	180.6	180.7	179.6	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
180.0	180.0	180.0	1.9	0.2	2.0

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 65-200064-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Electronic Balance

Manufacturer : METTLER TOLEDO Model : AG285

Serial No. : 1122140126 ID No. : MET-EB01/46

Capacity : 210 g Resolution : 0.00001g/81g, 0.0001g/210g

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (26.2 to 26.8) °C

Relative Humidity : (55.3 to 64.1) %

Air Pressure : 1011.0 mbar

Date of Received : 09 March 2022

Date of Calibration : 09 March 2022

Date of Issue : 16 March 2022

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 5, July 2015

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02213103	18 Nov 2022	National Institute of Metrology (Thailand), (NIMT)

Approved by :



Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-200064-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.01	0.00000	0.000016
0.1	0.00001	0.000021
1	-0.00001	0.000029
5	-0.00002	0.000043
10	-0.00006	0.000053
20	-0.00015	0.000071
50	-0.00035	0.00011
100	-0.0006	0.00021
150	-0.0009	0.00038
200	-0.0012	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.23$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A B C D E

0.00044 0.00006 -0.00052 -0.00019 0.00000 g



Repeatability

Load test : 200 g

Stdev. : 0.000052 g

- o0o -



Certificate of Calibration

Certificate No. : 65-200064-2

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Electronic Balance
Manufacturer : AND Model : FX-2000i
Serial No. : 15639789 ID No. : MET-EB03/61
Capacity : 2200 g Resolution : 0.01 g

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (26.1 to 26.2) °C
Relative Humidity : (55.5 to 61.9) %
Air Pressure : 1011.0 mbar

Date of Received : 09 March 2022

Date of Calibration : 09 March 2022

Date of Issue : 16 March 2022

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 5, July 2015

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
F181-F1821	65-210044-1	31 Jul 2022	National Institute of Metrology (Thailand), (NIMT)

Approved by :



Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-200064-2

Page : 2 of 2

Result of Calibration : After Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)	Error before Adjustment (g)
200	0.00	0.0083	-0.08
500	0.00	0.0085	-0.20
600	0.00	0.0086	-0.24
700	0.00	0.0087	-0.28
800	0.00	0.0089	-0.34
1000	0.01	0.0093	-0.41
1200	0.01	0.011	-0.50
1500	0.01	0.011	-0.61
2000	0.00	0.012	-0.79
2200	0.00	0.023	-0.87


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 500 g

A	B	C	D	E	
0.00	0.01	0.00	0.00	0.00	g



Repeatability

Load test : 2000 g

Stdev. : 0.000 g

- o0o -

