

เอกสารแนบ ง
ใบรับรองการสอบเทียบเครื่องมือ

บริษัท อินทิเกรตเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด

Certificate of Calibration

Calibration Certification Information

Cal. Date: May 25, 2022 Rootsmeter S/N: 438320 Ta: 296 °K
Operator: Jim Tisch Pa: 751.08 mm Hg
Calibration Model #: TE-5028A Calibrator S/N: **1836**

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.2210	4.5	1.50
2	3	4	1	0.9550	7.3	2.50
3	5	6	1	0.8660	8.8	3.00
4	7	8	1	0.7980	10.3	3.50
5	9	10	1	0.6080	17.5	6.00

Data Tabulation

Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9890	0.8100	1.2216	0.9940	0.8141	0.7689
0.9853	1.0317	1.5771	0.9903	1.0369	0.9926
0.9833	1.1354	1.7277	0.9883	1.1412	1.0873
0.9813	1.2297	1.8661	0.9863	1.2359	1.1745
0.9718	1.5983	2.4433	0.9767	1.6064	1.5377
QSTD	m=	1.54378	QA	m=	0.96669
	b=	-0.02519		b=	-0.01585
	r=	0.99990		r=	0.99990

Calculations

Vstd=	$\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$	Va=	$\Delta Vol((Pa-\Delta P)/Pa)$
Qstd=	$Vstd/\Delta Time$	Qa=	$Va/\Delta Time$
For subsequent flow rate calculations:			
Qstd=	$1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$	Qa=	$1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$

Standard Conditions

Tstd: 298.15 °K

Pstd: 760 mm Hg

Key

ΔH: calibrator manometer reading (in H2O)

ΔP: rootsmeter manometer reading (mm Hg)

Ta: actual absolute temperature (°K)

Pa: actual barometric pressure (mm Hg)

b: intercept

m: slope

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30.



Certificate of Calibration

Equipment: Balance
Model: ME36S
Serial No. (or ID.): 27206085
Manufacturer: Sartorius
Condition: In condition

Certificate No.: C01202535
Issued Date: 05 August 2020
Job No.: KSPR2009656
Page: 1 of 3

Customer: D.A. Research Center Co., Ltd.
122 Moo 2, Tambol Thatoom,
Amphur Srimahaphote, Prachinburi 25140 Thailand

Environment Condition: Temperature 25 °C ± 0.6 °C
Humidity 61 %RH ± 2.2 %RH

Calibration Place: D.A. Research Center Co., Ltd. (ห้องเครื่องชั่ง)
122 Moo 2, Tambol Thatoom,
Amphur Srimahaphote, Prachinburi 25140 Thailand

Calibration By: Mr. Ratchatapong Tanngam
Calibration Date: 24 July 2020
The Method used: In house method, SPCC-WI-47, base on UKAS Lab 14

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through SPC RT Co., Ltd. Certificate No. C02190531, C02193160

(Mr. Ratchatapong Tanngam)

Person in charge

(Mr. Rungrod Jenkitrakulchai)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

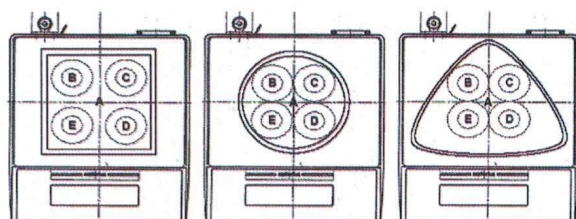
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SPC RT Co., Ltd.

Calibration Results:

Before Adjustment

Eccentric Error: Weight to be 1/4 or 1/3 of Maximum capacity, taken from the center of the pan as a zero reference.

			Nominal Test Value		1000	(mg)
Reference Points (mg)						
A	B	C	D	E		
-	-0.003	0.001	0.002	0.000		

Repeatability: Determination of the standard deviation of weighing balance., Readability 0.001 (mg)

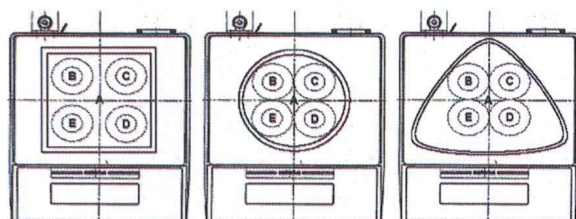
Nominal test value (mg)	Standard Deviation
2000	0.0011
20000	0.0012

Departure of indication from nominal value., Readability 0.001 (mg)

Nominal Value (mg)	Conventional Mass (mg)	Displayed Value (mg)	Correction of Balance (mg)	Uncertainty (mg)	k
1	1.0010	1.001	0.000	0.0035	2.01
5	5.0010	5.002	-0.001	0.0035	2.01
10	10.0010	10.000	0.001	0.0048	2.00
50	50.0040	50.002	0.002	0.0063	2.00
100	99.9980	99.997	0.001	0.0082	2.00
500	500.0000	500.000	0.000	0.013	2.00
1000	999.9880	999.987	0.001	0.016	2.00
5000	4999.9790	4999.974	0.005	0.027	2.00
10000	9999.9930	9999.987	0.006	0.033	2.00
20000	19999.9670	19999.960	0.007	0.048	2.00
30000	29999.9600	29999.951	0.009	0.080	2.00

After Adjustment

Eccentric Error: Weight to be 1/4 or 1/3 of Maximum capacity, taken from the center of the pan as a zero reference.

	Nominal Test Value	1000	(mg)	
Reference Points (mg)				
A	B	C	D	E
-	-0.002	0.001	0.002	0.000

Repeatability: Determination of the standard deviation of weighing balance., Readability 0.001 (mg)

Nominal test value (mg)	Standard Deviation
2000	0.0008
20000	0.0010

Departure of indication from nominal value., Readability 0.001 (mg)

Nominal Value (mg)	Conventional Mass (mg)	Displayed Value (mg)	Correction of Balance (mg)	Uncertainty (mg)	k
1	1.0010	1.001	0.000	0.0034	2.00
5	5.0010	5.001	0.000	0.0034	2.00
10	10.0010	10.001	0.000	0.0048	2.00
50	50.0040	50.003	0.001	0.0063	2.00
100	99.9980	99.998	0.000	0.0082	2.00
500	500.0000	499.999	0.001	0.013	2.00
1000	999.9880	999.988	0.000	0.016	2.00
5000	4999.9790	4999.977	0.002	0.027	2.00
10000	9999.9930	9999.990	0.003	0.033	2.00
20000	19999.9670	19999.964	0.003	0.048	2.00
30000	29999.9600	29999.956	0.004	0.080	2.00

The End of Certificate

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number:	E03NI99E80A0020	Reference Number:	82-401285019-1
Cylinder Number:	LL193324	Cylinder Volume:	83.4 CF
Laboratory:	124 - Riverton (SAP) - NJ	Cylinder Pressure:	2215 PSIG
PGVP Number:	B52018	Valve Outlet:	660
Gas Code:	NO,NOX,SO2,BALN	Certification Date:	Sep 05, 2018

Expiration Date: Sep 05, 2026

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	50.00 PPM	50.71 PPM	G1	+/- 1.4% NIST Traceable	08/27/2018, 09/05/2018
NITRIC OXIDE	50.00 PPM	50.67 PPM	G1	+/- 1.4% NIST Traceable	08/27/2018, 09/05/2018
SULFUR DIOXIDE	50.00 PPM	50.54 PPM	G1	+/- 1.0% NIST Traceable	08/27/2018, 09/05/2018
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	16060625	CC442585	50.42 PPM NITRIC OXIDE/NITROGEN	+/- 0.8%	Jun 27, 2020
PRM	12368	5604119	29.86 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Jun 02, 2017
GMIS	7042010104	CC503941	5.101 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.0%	Jun 01, 2020
NTRM	14010327	KAL004376	49.08 PPM SULFUR DIOXIDE/NITROGEN	+/- 1.0%	Apr 17, 2024

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 APW1100391 NO	FTIR	Aug 09, 2018
Nicolet 6700 APW1100391 NO2	FTIR	Aug 31, 2018
Nicolet 6700 APW1100391 SO2	FTIR	Aug 30, 2018

Triad Data Available Upon Request

NOTES:PO# 5218003935

Net weight: 2736 grams
Gross weight: 17393 grams

This calibration std. has been certified in accordance with the May 2012 EPA Traceability Protocol, Document EPA-600/R-12/531. All testing processes and measurements conform to the requirements of ISO/IEC 17025 and to Airgas ISO 9001:2008 and relate only to items identified on this certificate. All values are certified to be NIST Traceable with total uncertainty as detailed under Analytical Uncertainty. This document shall not be reproduced in full without written approval of the issuer.



TESTING CERT No. 3082.05

Approved for Release

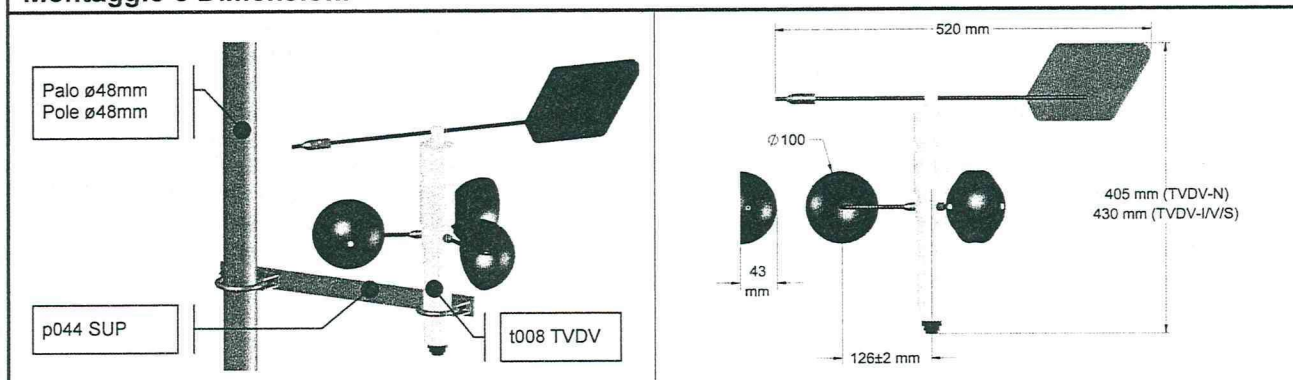
Specifiche Tecniche

Technical Data

Velocità Vento						Wind Speed
Campo di misura	0 ÷ 50 m/s					Range
Risoluzione	0,1 m/s					Resolution
Sensibilità	0,25 m/s					Sensitivity
Accuratezza	±0,25 m/s (0÷20m/s) ; ±0,7 m/s (>20m/s)					Accuracy
Costante strumentale	2,44 Hz/m/s					Conversion constant
Costante di distanza	< 5 m					Distance constant
Elemento sensibile	3 coppe con trasduttore magnetico 3 cups with magnetic transducer					Transducer
Direzione Vento						Wind Direction
Campo di misura	0 ÷ 360 °					Range
Risoluzione	0,1 °					Resolution
Sensibilità	0,25 m/s					Sensitivity
Accuratezza	± 2°					Accuracy
Elemento sensibile	Banderuola e trasduttore potenziometrico Wind vane and potenziometric transducer					Transducer
Caratteristiche Comuni						Common characteristics
Campo di funzionamento	0 ÷ 50 m/s					Operatine range
Temperatura di funzionamento	- 30 ÷ +60 °C					Working temperature
Protezioni	Controinversione di polarità e scariche atmosferiche Polarity reverse and transient					Protections
Alimentazione	10 ÷ 16 Vdc					Power supply
Corrente assorbita (mA)	TVDV-I		min.	typ.	max.	Supply current (mA)
		stand-by	5		21	
	meas.	14		30		
	TVDV-V/S	stand-by		7		
meas.			16			
Impedenza di uscita (t008b TVDV-V)	10 Ohm					Output resist (t008b TVDV-V)
Carico massimo (t008a TVDV-I)	390 ohm					Output resist (t008a TVDV-I)
Realizzato in	Lega di alluminio e viterie inox Aluminum alloy and stainless steel					Housing
Peso	930 g					Weight
Dimensioni	520mm ; H=405mm (TVDV-N) ; H=430mm (TVDV-I/V/S)					Dimensions
Connettore	(IP67) 4 o 7 poli maschio / 4 or 7 poles male					Connector

Montaggio e Dimensioni

Installation and Dimensions



Cablaggio del connettore

Electrical connections

 Connettore 4 o 7 poli maschio (IP67) - Visto da sotto 4 or 7 pole male connector - Bottom view	Pin 1	Pin 2	Pin 3	Pin 4	Pin 5	Pin 6	Pin 7
	TVDV-N	Alim. 10÷16Vdc	Alim. GND	OUT V.V. +2,5 Vdc	Alim. GND	OUT D.V.	N.C.
	TVDV-I	Alim. 10÷16Vdc	OUT V.V. +4÷20mA	OUT D.V. +4÷20mA	Alim. GND		
	TVDV-V	Alim. 10÷16Vdc	OUT V.V. +0÷2Vdc	OUT D.V. +0÷2Vdc	Alim. GND		
	TVDV-S	Alim. 10÷16Vdc	B-RS485	A-RS485	Alim. GND		

Accessori

Accessories

Descrizione		Description
Cavo da 5 metri con connettori	p041a CAV4P5M ; p041c CAV8P5M	Cable with connector, lenght 5 meters
Cavo da 12 metri con connettori	p041b CAV4P12M ; p041d CAV8P12M	Cable with connector, lenght 12 meters
Supporto per trasduttore meteo	p044 SUP	Steel bracket support for transducer
Certificato di taratura in laboratorio	rt008 KRTVDV	Laboratory calibration certificate

SIAP+MICROS S.r.l.

Via Del Lavoro, 1
I - 31010 - Castello Roganzuolo
di San Fior (TV)

tel +39 0438 491411 - fax +39 0438 401573
email info@siapmicros.com
www.siapmicros.com

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 10/1264

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.

Address : 122 Moo 2 T.Thatoom A.Srimahaphote Prachinburi 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 100012

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Keithley 2015-P S/N 4106495.
 7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 3 Dec. 2021

Date of Calibration : 15 Dec. 2021

1 / 2
W

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 10/1264

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.92	-0.08	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1008.4	8.4	± 1.5	$\pm 1.0\%$

3. Total Distortion


Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.70	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.


2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :


(Mr. Weerachai Deechaiyae)

Approved by :


(Mr. Prawate Kluaypa)
Acting Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 15 Dec. 2021

Date of Issue : 20 Dec. 2021

Ref : 2011264120305034001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 20/1264

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited.
Address : 122 Moo 2 T.Thatoom, A.Srimahaphote, Prachinburi 25140.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Integrating Sound Level Meter
Manufacturer : ACO
Model : 6236
Serial No. : 192014
Microphone : Type 7052NR No.73303
Preamplifier : -

Ambient Environment

Temperature : $(23 \pm 3)^{\circ}\text{C}$
Relative Humidity : $(50 \pm 15) \%$
Ambient Pressure : $(101.325 \pm 1.5) \text{ kPa}$

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 3 Dec. 2021

Date of Calibration : 27-29 Dec. 2021

1 / 8

1

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 20/1264

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
11. Digital Multimeter Agilent 34401A S/N MY44005560.
12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2006). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 27-29 Dec. 2021

2 / 8 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 20/1264

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Unit Under Test			Tolerance
	Measured Value (dB)	Deviation (dB)	Uncertainty (+dB)	Limit Class 2 (+dB)
113.97	114.0	0.0	0.30	1.4

Note: No adjustment. The internal calibration was display at 114.1 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (+dB)
19.4	0.10

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured Value (dB)	Uncertainty (+dB)
A-Weighting	13.1	0.10
C-Weighting	18.8	0.10
Flat	22.6	0.10

Date of Calibration : 27-29 Dec. 2021

3 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 20/1264

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from response curve			Uncertainty (+dB)	Tolerance Limits Class 2 (+dB)
	A-weighting (dB)	C-weighting (dB)	Flat (dB)		
125	0.2	0.3	0.2	0.40	2.0
1 000	-0.8	-0.8	-0.7	0.40	1.4
4 000	0.0	0.1	0.4	0.40	3.6

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from response curve			Uncertainty (+dB)	Tolerance Limits Class 2 (+dB)
	A-weighting (dB)	C-weighting (dB)	Flat (dB)		
63	0.2	0.0	0.0	0.20	2.5
125	0.1	0.0	0.0	0.20	2.0
250	0.1	0.0	0.0	0.20	1.9
500	0.1	0.1	0.0	0.20	1.9
1 000	0.0	0.0	0.0	0.20	1.4
2 000	-0.1	0.0	0.0	0.20	2.6
4 000	-0.4	-0.4	-0.1	0.20	3.6
8 000	-0.6	-0.6	-0.2	0.20	5.6

Date of Calibration : 27-29 Dec. 2021

4 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 20/1264

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Uncertainty (\pm dB)	Tolerance Limits Class 2 (\pm dB)
A-weighting	94.0	0.0	0.20	0.4
C-weighting	94.0	0.0	0.20	0.4
Flat	94.1	0.1	0.20	0.4

5.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Uncertainty (\pm dB)	Tolerance Limits Class 2 (\pm dB)
Fast	94.0	0.0	0.20	0.3
Slow	94.0	0.0	0.20	0.3
Leq	94.0	0.0	0.20	0.3

6. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Uncertainty (\pm dB)	Tolerance Limits Class 2 (\pm dB)
122	122.0	0.0	0.30	1.4
121	121.0	0.0	0.30	1.4
120	120.0	0.0	0.30	1.4
119	119.0	0.0	0.30	1.4
114	114.0	0.0	0.30	1.4
109	109.0	0.0	0.30	1.4

Date of Calibration : 27-29 Dec. 2021

5 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 20/1264

6. Level linearity on the reference level range (cont.)

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Uncertainty (\pm dB)	Tolerance Limits Class 2 (\pm dB)
104	104.0	0.0	0.30	1.4
99	99.0	0.0	0.30	1.4
94	94.0	0.0	0.30	1.4
89	89.0	0.0	0.30	1.4
84	84.0	0.0	0.30	1.4
79	79.0	0.0	0.30	1.4
74	74.1	0.1	0.30	1.4
69	69.1	0.1	0.30	1.4
64	64.0	0.0	0.30	1.4
59	59.0	0.0	0.30	1.4
54	54.0	0.0	0.30	1.4
49	49.0	0.0	0.30	1.4
44	44.0	0.0	0.30	1.4
39	38.9	-0.1	0.30	1.4
34	34.1	0.1	0.30	1.4
33	33.1	0.1	0.30	1.4
32	32.1	0.1	0.30	1.4
31	31.2	0.2	0.30	1.4
30	30.2	0.2	0.30	1.4

Date of Calibration : 27-29 Dec. 2021

6 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 20/1264

7. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Uncertainty (+dB)	Tolerance Limits Class 2 (+dB)
40-130	125	125.0	0.0	0.30	1.4
30-120	115	115.0	0.0	0.30	1.4
20-110	105	105.0	0.0	0.30	1.4
20-100	95	95.0	0.0	0.30	1.4
20-90	85	85.0	0.0	0.30	1.4
20-80	75	74.9	-0.1	0.30	1.4

8. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured Value (dB)	Deviated Value (dB)	Uncertainty (\pm dB)	Tolerance Limits Class 2 (dB)
Fast	200	115.8	-0.2	0.20	± 1.3
	2	98.8	-0.2	0.20	+1.3; -2.8
	0.25	89.8	-0.2	0.20	+1.8; -5.3
Slow	200	109.3	-0.3	0.20	± 1.3
	2	89.8	-0.2	0.20	+1.3; -5.3
SEL	200	109.9	-0.1	0.20	± 1.3
	2	90.0	0.0	0.20	+1.3; -2.8
	0.25	80.9	-0.1	0.20	+1.8; -5.3

Date of Calibration : 27-29 Dec. 2021

7 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 20/1264

9. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (\pm dB)	Tolerance limits Class 2 (\pm dB)
Complete cycle	125.4	125.3	-0.1	0.20	2.4
Positive half cycle	124.4	124.3	-0.1	0.20	1.4
Negative half cycle	124.4	124.3	-0.1	0.20	1.4

10. Overload indication

Measured value (dB)		Deviated value (dB)	Uncertainty (\pm dB)	Tolerance Limits Class 2 (\pm dB)
Positive one-half cycle	Negative one-half cycle			
133.0	132.9	0.1	0.30	1.8

Calibrated by :

Panya Phasingsoi

(Mr. Panya Phasingsoi)

Tawikiat Iamsamran

(Mr. Tawikiat Iamsamran)

Approved by :

Prawate Kluaypa

(Mr. Prawate Kluaypa)

Acting Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 27-29 Dec. 2021

Date of Issue : 4 Jan. 2022

Ref : 2011264120305034011

End of Certificate

8 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 21/1264

CALIBRATION CERTIFICATE

Submitted by : Integrated Research Center Company Limited

Address : 122 Moo 2, T.Thatoom, A.Srimahaphote, Prachinburi 25140.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Integrating Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial No. : 192015

Microphone : Type 7052NR No.73304

Preamplifier : -

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.5) \text{ kPa}$

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 3 Dec. 2021

Date of Calibration : 10-11 Jan. 2022

1 / 8

T

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 21/1264

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
11. Digital Multimeter Agilent 34401A S/N MY44005560.
12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2006). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 10-11 Jan. 2022

2 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 21/1264

1. Absolute Sensitivity

Reference	Unit Under Test				Tolerance
Acoustic Signal (dB)	Measured Value (dB)		Deviation	Uncertainty	Limit Class 2
	Before adjust	After adjust	(dB)	(+dB)	(+dB)
113.96	113.0	114.0	0.0	0.30	1.4

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 115.3 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (+dB)
16.8	0.10

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured Value (dB)	Uncertainty (+dB)
A-Weighting	14.8	0.10
C-Weighting	21.1	0.10
Flat	25.7	0.10

Date of Calibration : 10-11 Jan. 2022

3 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 21/1264

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from response curve			Uncertainty (+dB)	Tolerance Limits Class 2 (+dB)
	A-weighting (dB)	C-weighting (dB)	Flat (dB)		
125	0.2	0.1	0.1	0.40	2.0
1 000	-0.8	-0.7	-0.7	0.40	1.4
4 000	-0.1	-0.1	0.3	0.40	3.6

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from response curve			Uncertainty (+dB)	Tolerance Limits Class 2 (+dB)
	A-weighting (dB)	C-weighting (dB)	Flat (dB)		
63	0.2	0.0	0.0	0.20	2.5
125	0.0	0.1	0.1	0.20	2.0
250	0.0	0.0	0.0	0.20	1.9
500	0.0	0.0	0.0	0.20	1.9
1 000	0.0	0.0	0.0	0.20	1.4
2 000	-0.2	0.0	0.0	0.20	2.6
4 000	-0.5	-0.3	0.0	0.20	3.6
8 000	-0.6	-0.5	-0.1	0.20	5.6

Date of Calibration : 10-11 Jan. 2022

4 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 21/1264

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Uncertainty (+dB)	Tolerance Limits Class 2 (+dB)
A-weighting	94.0	0.0	0.20	0.4
C-weighting	94.0	0.0	0.20	0.4
Flat	94.1	0.1	0.20	0.4

5.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Uncertainty (+dB)	Tolerance Limits Class 2 (+dB)
Fast	94.0	0.0	0.20	0.3
Slow	94.0	0.0	0.20	0.3
Leq	94.0	0.0	0.20	0.3

6. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Uncertainty (+dB)	Tolerance Limits Class 2 (+dB)
122	122.1	0.1	0.30	1.4
121	121.1	0.1	0.30	1.4
120	120.0	0.0	0.30	1.4
119	119.0	0.0	0.30	1.4
114	114.0	0.0	0.30	1.4
109	108.9	-0.1	0.30	1.4
104	104.0	0.0	0.30	1.4
99	99.0	0.0	0.30	1.4

Date of Calibration : 10-11 Jan. 2022

5 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 21/1264

6. Level linearity on the reference level range (cont.)

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Uncertainty (+dB)	Tolerance Limits Class 2 (+dB)
94	94.0	0.0	0.30	1.4
89	89.0	0.0	0.30	1.4
84	83.9	-0.1	0.30	1.4
79	78.9	-0.1	0.30	1.4
74	74.2	0.2	0.30	1.4
69	69.2	0.2	0.30	1.4
64	64.1	0.1	0.30	1.4
59	59.0	0.0	0.30	1.4
54	54.1	0.1	0.30	1.4
49	49.1	0.1	0.30	1.4
44	44.1	0.1	0.30	1.4
39	39.0	0.0	0.30	1.4
34	34.2	0.2	0.30	1.4
33	33.2	0.2	0.30	1.4
32	32.3	0.3	0.30	1.4
31	31.3	0.3	0.30	1.4
30	30.4	0.4	0.30	1.4

Date of Calibration : 10-11 Jan. 2022

6 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 21/1264

7. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Uncertainty (+dB)	Tolerance Limits Class 2 (+dB)
40-130	125	125.1	0.1	0.30	1.4
30-120	115	115.0	0.0	0.30	1.4
20-110	105	105.0	0.0	0.30	1.4
20-100	95	95.0	0.0	0.30	1.4
20-90	85	85.0	0.0	0.30	1.4
20-80	75	75.0	0.0	0.30	1.4

8. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured Value (dB)	Deviated Value (dB)	Uncertainty (+dB)	Tolerance Limits Class 2 (dB)
Fast	200	115.7	-0.3	0.20	± 1.3
	2	98.8	-0.2	0.20	+1.3; -2.8
	0.25	88.3	-1.7	0.20	+1.8; -5.3
Slow	200	109.4	-0.2	0.20	± 1.3
	2	89.8	-0.2	0.20	+1.3; -5.3
SEL	200	109.9	-0.1	0.20	± 1.3
	2	90.0	0.0	0.20	+1.3; -2.8
	0.25	80.9	-0.1	0.20	+1.8; -5.3

Date of Calibration : 10-11 Jan. 2022

7 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0155

MTC No. EEL. BP. 21/1264

9. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (\pm dB)	Tolerance limits Class 2 (\pm dB)
Complete cycle	125.4	125.8	0.4	0.20	2.4
Positive half cycle	124.4	124.3	-0.1	0.20	1.4
Negative half cycle	124.4	124.3	-0.1	0.20	1.4

10. Overload indication

Measured value (dB)		Deviated value (dB)	Uncertainty (\pm dB)	Tolerance Limits Class 2 (\pm dB)
Positive one-half cycle	Negative one-half cycle			
133.1	133.1	0.0	0.30	1.8

Calibrated by :

Panya Phasingsri
.....
(Mr. Panya Phasingsri)
Tawikiat Iamsamran
.....
(Mr. Tawikiat Iamsamran)

Approved by :

Prawate Khuaypa
.....
(Mr. Prawate Khuaypa)
Acting Director

Date of Calibration : 10-11 Jan. 2022

Date of Issue : 12 Jan. 2022

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Ref : 2011264120305034012

End of Certificate

8 / 8

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

เอกสารแนบ จ

สำเนาหนังสืออนุญาตขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท อินทิเกรตเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด



ที่ อก ๐๓๒๐/๑๗๐๓๒

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๒ พฤศจิกายน ๒๕๖๕

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท อินทิเกรตเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด

อ้างถึง คำขอต่ออายุของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๕ ตุลาคม ๒๕๖๕

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท อินทิเกรตเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด จำนวน ๓ แผ่น

ตามหนังสือที่อ้างถึง บริษัท อินทิเกรตเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด ขอต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๙๙ สถานที่ตั้งเลขที่ ๑๒๒ หมู่ที่ ๒ ตำบลท่าตูม
อำเภอศรีมหาโพธิ จังหวัดปราจีนบุรี ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท อินทิเกรตเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด
ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

- | | |
|----------------------------------|----------------------------|
| ๑) นางสาววิไลรัตน์ เกียรติธนะชัย | ทะเบียนเลขที่ ว-๑๙๙-ค-๐๐๐๑ |
| ๒) นางสาวทิติยา นันหมื่น | ทะเบียนเลขที่ ว-๑๙๙-ค-๐๐๐๒ |
| ๓) นางวีราภรณ์ ผลเจริญ | ทะเบียนเลขที่ ว-๑๙๙-ค-๐๐๐๓ |

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์


- | | |
|------------------------------|----------------------------|
| ๑) นายไกรวิชญ์ แสงแก้ว | ทะเบียนเลขที่ ว-๑๙๙-จ-๐๐๐๑ |
| ๒) นางสาวณัฐนันท์ สังวาลวงศ์ | ทะเบียนเลขที่ ว-๑๙๙-จ-๐๐๐๒ |
| ๓) นางสาวอนันตพร งามสง่า | ทะเบียนเลขที่ ว-๑๙๙-จ-๐๐๐๓ |
| ๔) นางสาวหนึ่งฤทัย ออบมาลี | ทะเบียนเลขที่ ว-๑๙๙-จ-๐๐๐๔ |
| ๕) นางสาวแววตา คำสา | ทะเบียนเลขที่ ว-๑๙๙-จ-๐๐๐๕ |
| ๖) นายจักรีชัย อินตะ | ทะเบียนเลขที่ ว-๑๙๙-จ-๐๐๐๖ |
| ๗) นางสาวชนนิกันต์ แสนสุข | ทะเบียนเลขที่ ว-๑๙๙-จ-๐๐๐๗ |

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนในวิเคราะห์ในน้ำเสีย จำนวน ๒๓ รายการ น้ำใต้ดิน
จำนวน ๑๒ รายการ และสิ่งปฏิกูลหรือวัสดุที่ไม่ใช่แล้ว จำนวน ๑๐ รายการ รวมทั้งสิ้นจำนวน ๔๕ รายการ
ตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้จะหมดอายุในวันที่ ๑๘ พฤศจิกายน ๒๕๖๘ หากประสงค์จะต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงาน
อุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งคำขอ
ต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้า
เว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ท้ายหนังสือนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นายทวี อำพาพันธ์)

ผู้อำนวยการศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๕ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์



เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท อินทิเกรตเต็ด รีเสิร์ช เซ็นเตอร์ จำกัด

ที่ อก ๐๓๒๐/๑๗๐๓๒

เลขทะเบียน ว-๑๙๙

ลงวันที่ ๒๒ พฤศจิกายน ๒๕๖๕

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๔๕ รายการ
น้ำเสีย จำนวน 23 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Arsenic	Digestion, Inductively Coupled Plasma Method ^[1]
2	Barium	Digestion, Inductively Coupled Plasma Method ^[1]
3	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ^[1] 2) 5-Day BOD Test, Membrane Electrode Method ^[1]
4	Cadmium	Digestion, Inductively Coupled Plasma Method ^[1]
5	Chemical Oxygen Demand	Closed Reflux, Colorimetric Method ^[1]
6	Color	ADMI Weighted – Ordinate Spectrophotometric Method ^[1]
7	Copper	Digestion, Inductively Coupled Plasma Method ^[1]
8	Free Chlorine	Iodometric Method ^[1]
9	Hexavalent Chromium	Filtration, Colorimetric Method ^[1]
10	Lead	Digestion, Inductively Coupled Plasma Method ^[1]
11	Manganese	Digestion, Inductively Coupled Plasma Method ^[1]
12	Nickle	Digestion, Inductively Coupled Plasma Method ^[1]
13	Oil and Grease	Liquid-Liquid, Partition-Gravimetric Method ^[1]
14	pH	Electrometric Method ^[1]
15	Selenium	Digestion, Inductively Coupled Plasma Method ^[1]
16	Sulfide	ZnS Precipitation, Iodometric Method ^[1]
17	Temperature	Field Method ^[1]
18	Total Chromium	Digestion, Inductively Coupled Plasma Method ^[1]
19	Total Dissolved Solids	Dried at 180 °C ^[1]
20	Total Kjeldahl Nitrogen	Macro Kjeldahl Method ^[1]
21	Total Suspended Solids	Dried at 103-105 °C ^[1]
22	Trivalent Chromium	Digestion, Inductively Coupled Plasma Method Filtration, Colorimetric Method, Calculation ^[1]
23	Zinc	Digestion, Inductively Coupled Plasma Method ^[1]

น้ำใต้ดิน จำนวน 12 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Arsenic	Digestion, Inductively Coupled Plasma Method ^[1]
2	Barium	Digestion, Inductively Coupled Plasma Method ^[1]
3	Cadmium	Digestion, Inductively Coupled Plasma Method ^[1]
4	Chromium	Digestion, Inductively Coupled Plasma Method ^[1]
5	Hexavalent Chromium	Filtration, Colorimetric Method ^[1]
6	Lead	Digestion, Inductively Coupled Plasma Method ^[1]
7	Manganese	Digestion, Inductively Coupled Plasma Method ^[1]
8	Nickel	Digestion, Inductively Coupled Plasma Method ^[1]
9	pH	Electrometric Method ^[1]
10	Selenium	Digestion, Inductively Coupled Plasma Method ^[1]
11	Trivalent Chromium	Inductively Coupled Plasma Method; Filtration, Colorimetric Method; Calculation ^[1]
12	Zinc	Digestion, Inductively Coupled Plasma Method ^[1]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 10 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,4,5] 2) Digestion, Inductively Coupled Plasma Method ^[3,5]
2	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,4,5] 2) Digestion, Inductively Coupled Plasma Method ^[3,5]
3	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,4,5] 2) Digestion, Inductively Coupled Plasma Method ^[3,5]
4	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,4,5] 2) Digestion, Inductively Coupled Plasma Method ^[3,5]
5	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,4,5] 2) Digestion, Inductively Coupled Plasma Method ^[3,5]
6	Manganese	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,4,5] 2) Digestion, Inductively Coupled Plasma Method ^[3,5]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
7	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,4,5]
8	pH	2) Digestion, Inductively Coupled Plasma Method ^[3,5] Electrometric Method ^[6]
9	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,4,5]
10	Zinc	2) Digestion, Inductively Coupled Plasma Method ^[3,5] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,4,5] 2) Digestion, Inductively Coupled Plasma Method ^[3,5]

เอกสารอ้างอิง

1. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 23rd ed. Washington, DC : APHA, 2017
2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2548 เรื่อง การกำจัดสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. ราชกิจจานุเบกษา. 25 มกราคม 2549, เล่มที่ 123 ตอนพิเศษ 11ง.
3. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Acid Digestion of Sediments Sludges, and Soils. SW-846 Method 3050B**, 1996.
4. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **SW-846**, 2006.
5. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma – optical Emission Spectrometry. SW-846 Method 6010D**, 2018
6. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Solid and Waste pH. SW-846 Method 9045D**, 2004.

