

ภาคผนวก ง

ใบรับรองการสอบเทียบเครื่องมือ

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Stack	Total Suspended Particulate	Console Control Unit	BKK_FS0468	12-Jul-22	12-Jan-23	6
Stack	Total Suspended Particulate	Console Control Unit	BKK_FS0527	12-Jul-22	12-Jan-23	6
Stack	Total Suspended Particulate	Console Control Unit	BKK_FS0556	12-Jul-22	12-Jan-23	6
Stack	Total Suspended Particulate	Console Control Unit	BKK_FS0518	12-Jul-22	12-Jan-23	6
Stack	Total Suspended Particulate	Digital Balance	RYG_EN0003	23-Mar-22	23-Mar-23	12
Ambient	Total Suspended Particulate	High Volume	RYG_FS0177	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0395	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0394	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	RYG_EN0001	23-Mar-22	23-Mar-23	12
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0081	5-Jul-21	3-Jan-23	18
Noise	Leq 24 hrs	Sound Calibrator	RYG_FS0496	10-Jan-22	10-Jan-23	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0431	21-Jan-22	21-Jan-23	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0432	21-Jan-22	21-Jan-23	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0492	10-Jan-22	10-Jan-23	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0491	10-Jan-22	10-Jan-23	12
Heat	Heat Stress	Heat Stress Monitor	RYG_FS0221	17-Mar-22	17-Mar-23	12
Heat	Heat Stress	Heat Stress Monitor	RYG_FS0218	13-Dec-21	13-Dec-22	12
Heat	Heat Stress	Heat Stress Monitor	RYG_FS0219	14-Feb-22	14-Feb-23	12
Heat	Heat Stress	Heat Stress Monitor	RYG_FS0220	28-Dec-21	28-Dec-22	12
Heat	Heat Stress	Heat Stress Monitor	RYG_FS0221	17-Mar-22	17-Mar-23	12
Heat	Heat Stress	Heat Stress Monitor	RYG_FS0223	28-Dec-21	28-Dec-22	12
Heat	Heat Stress	Heat Stress Monitor	RYG_FS0228	25-Aug-22	25-Aug-23	12
Heat	Heat Stress	Heat Stress Monitor	RYG_FS0220	28-Dec-21	28-Dec-22	12
Workplace	Silica (Quartz)	Field Rotameter	RYG_FS0198	1-Jul-22	1-Oct-22	3
Workplace	Silica (Quartz)	Field Rotameter	RYG_FS0197	1-Oct-22	1-Jan-23	3
Workplace	Silica (Quartz)	Field Rotameter	RYG_FS0198	1-Oct-22	1-Jan-23	3
Noise	Leq 8 hrs	Sound Calibrator	RYG_FS0496	10-Jan-22	10-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0030	21-Jan-22	21-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0031	20-Jun-22	20-Jun-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0495	10-Jan-22	10-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0029	24-May-22	24-May-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0494	10-Jan-22	10-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0027	10-Jan-22	10-Jan-23	12
Noise	Leq 8 hrs	Sound Calibrator	RYG_FS0213	26-Apr-22	26-Apr-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0007	10-Jan-22	10-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0016	11-Jul-22	11-Jul-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0020	10-Jan-22	10-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0026	21-Jan-22	21-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0027	10-Jan-22	10-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0011	11-Jul-22	11-Jul-23	12
Rayong Lab	pH at 25 °C	pH meter	RYG_EN0183	17-Mar-22	17-Mar-23	12
Rayong Lab	Color (at Original pH)	Spectrophotometer	RYG_EN0037	27-Sep-22	27-Mar-24	18
Rayong Lab	Color (at pH 7.0)	Spectrophotometer	RYG_EN0037	27-Sep-22	27-Mar-24	18
Rayong Lab	BOD	DO meter with Sensor	RYG_EN0032	14-Feb-22	15-Aug-23	18
Rayong Lab	BOD	Incubator	RYG_EN0154	22-Apr-22	21-Oct-23	18
Rayong Lab	COD	Spectrophotometer	RYG_EN0037	27-Sep-22	27-Mar-24	18
Rayong Lab	Total Suspended Solids	Electronic Balance	RYG_EN0002	23-Mar-22	23-Mar-23	12
Rayong Lab	Total Suspended Solids	Hot Air Oven	RYG_EN0010	20-Oct-22	20-Apr-24	18
Rayong Lab	Total Dissolved Solids 180°C	Electronic Balance	RYG_EN0002	23-Mar-22	23-Mar-23	12
Rayong Lab	Total Dissolved Solids 180°C	Hot Air Oven	RYG_EN0010	20-Oct-22	20-Apr-24	18
Rayong Lab	Oil & Grease	Electronic Balance	RYG_EN0002	23-Mar-22	23-Mar-23	12
Rayong Lab	Oil & Grease	Hot Air Oven	RYG_EN0006	20-Oct-22	20-Apr-24	18
Rayong Lab	Oil & Grease	Water Bath	RYG_EN0061	20-Oct-22	20-Apr-24	18



CONSOLE CONTROL UNIT CALIBRATION TEST REPORT

Calibration of Date : 12 Jul 22
Next Cal. Date : 12 Jan 23

Barometric Pressure (mm.Hg) : 755
Relative Humidity (%) : 70.0
Temperature (°C) : 30.0

Console Control Meter Data

Calibration No. : C-120722-BKK_FS0468
Dry Gas Meter No. : BKK_FS0468
Console Serial No. : 1302005
Console Model No. : XC-572-V

Reference Dry Gas Meter Data

Serial No. : 1607009
Model No. : SK25EXSR-QC6
Correction Factor (Yr) : 1.0060
Next Calibration Date : 7 Oct 22

ΔH (mm.H ₂ O)	\ominus Minutes	Reference Dry Gas Meter Calibration				Console Control ; Drygas Meter						Dry Gas Meter	Orifice
		Vr (Liters)			Tr (°C)	Vm (Liters)			Ti (°C)	To (°C)	Avg.Tm (°C)	Correction	Calibration
		Final	Initial	Total		Final	Initial	Total				Factor (Y)	Factor $\Delta H@$
15	12.80	150.00	0.00	150.00	31.0	344.0	191.0	153.00	30.0	30.0	30.0	0.9816	50.7881
25	9.60	150.00	0.00	150.00	31.0	511.4	358.0	153.40	30.0	30.0	30.0	0.9781	47.6138
50	6.68	150.00	0.00	150.00	31.0	673.4	520.0	153.40	31.0	31.0	31.0	0.9789	45.9560
100	4.62	150.00	0.00	150.00	32.0	842.0	689.0	153.00	31.0	31.0	31.0	0.9736	44.2543
150	3.77	150.00	0.00	150.00	32.0	1005.5	853.0	152.45	32.0	32.0	32.0	0.9756	44.0575
											Avg.	0.9776	46.5339

Y : Ratio of reading of reference to dry gas meter : tolerance for individual values ± 0.02 from average .

$\Delta H@$: Orifice pressure differential that equates to 21.24 lm of air @ 25 C and 760 mm of mercury , mmH₂O ; tolerance for individual values ± 5.08 from average .

Procedure; 40 CFR 60,APP A,METH ,SEC 5.3 & 7

Calibrated by:

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by:

Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)



DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	12-Jul-22	Ambient Temperature (°C) :	30
Calibration sheet No. :	C-120722-BKK_FS0469	Relative Humidity (%) :	70
Digital Temperature ID	BKK_FS0469	Reference Temperature ID	BKK_FS0609
Serial No. :	1302005	Serial No. :	7688004
Model :	XC-572-V	Model :	FLUKE 714
		Next Calibrate :	26 Jul 23

Location	Reference Temperature °C	Digital Temperature °C	Error °C	Remark
Stack	0	0	0	
	25	24	-1	
	50	49	-1	
	100	98	-2	
	150	148	-2	
	200	197	-3	
	250	247	-3	
	300	297	-3	
	500	497	-3	
	1000	997	-3	
	1200	1197	-3	
Probe	100	99	-1	
	125	124	-1	
	150	149	-1	
Oven	100	99	-1	
	125	124	-1	
	150	149	-1	
Filter	100	100	0	
	125	125	0	
	150	149	-1	
Exit	0	0	0	
	10	11	1	
	20	21	1	
Meter	0	0	0	
	25	25	0	
	50	50	0	
AUX	0	0	0	
	25	25	0	
	50	50	0	

Calibrated by

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by :

Natthapol Jiengwareewong

(Mr.Natthapol Jiengwareewong)

Manager



Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK_FS0472 Calibration Date : 12 Jul 22
 Lab test duct Number : 258-1-13-01 Standard Pitot ID : BKK_FS0441
 Calibration Sheet No. : C-120722-BKK_FS0472 Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube (ΔP , mm.H ₂ O)	Type s pitot tube (ΔP , mm.H ₂ O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			\bar{C}_p	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P_{(std)}}{\Delta P_{(s)}}}$$

$$| \bar{C}_{p(A)} - \bar{C}_{p(B)} | \text{ must BE } \leq 0.01$$

$$\text{Average deviation}(A \text{ or } B) = \frac{\sum_i [Cp_{(s)} - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by

Nattapon Jengwareewong

(Mr.Nattapol Jengwareewong)

Field Specialist(1)



Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK_FS0473 Calibration Date : 12 Jul 22
 Lab test duct Number : 258-1-13-01 Standard Pitot ID : BKK_FS0441
 Calibration Sheet No. : C-120722-BKK_FS0473 Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube (ΔP, mm.H ₂ O)	Type s pitot tube (ΔP, mm.H ₂ O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			\bar{C}_p	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P(std)}{\Delta P(s)}}$$

$$| \bar{C}_{p(A)} - \bar{C}_{p(B)} | \text{ must BE } \leq 0.01$$

$$\text{Average deviation}(A \text{ or } B) = \frac{\sum_i [Cp(s) - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by

Natthapol Jiengwareewong

(Mr.Natthapol Jiengwareewong)

Field Specialist(1)



PROBE NOZZLE DIAMETER
CALIBRATION DATA SHEET

Calibration Date	12 Jul 22	Nozzle Set ID. :	BKK_FS0474
Calibration Sheet No. :	C-120722-BKK_FS0474	Vernier Caliper ID. :	BKK_FS0626


Nozzle ID #	Nozzle Diameter (cm.)			Hi - Lo	$(D_1 + D_2 + D_3) / 3$
	D_1	D_2	D_3	ΔD	D_{avg}
1	0.300	0.300	0.300	0.000	0.300
2	0.450	0.450	0.450	0.000	0.450
3	0.600	0.600	0.600	0.000	0.600
4	0.780	0.780	0.780	0.000	0.780
5	0.932	0.932	0.932	0.000	0.932
6	1.094	1.094	1.094	0.000	1.094
7	1.264	1.264	1.264	0.000	1.264

Where :

D_1, D_2, D_3 = There different nozzle diameters at 60 degrees to each other, each measured the nearest 0.025 mm.

ΔD = Maximum distance between any two diameters, must be ≤ 0.100 mm.

D_{avg} = $(D_1 + D_2 + D_3) / 3$

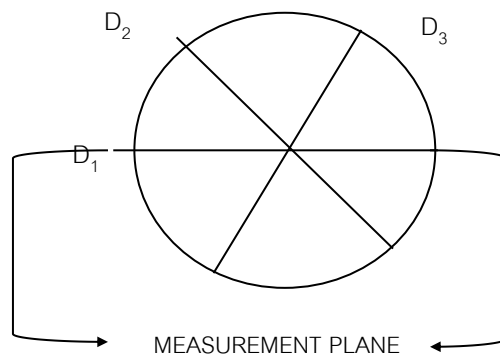

Calibrated by

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by

Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)



CONSOLE CONTROL UNIT CALIBRATION TEST REPORT

Calibration of Date : 12 Jul 22
Next Cal. Date : 12 Jan 23

Barometric Pressure (mm.Hg) : 755
Relative Humidity (%) : 70.0
Temperature (C°) : 30.0

Console Control Meter Data

Calibration No. : C-120722-BKK_FS0527
Dry Gas Meter No. : BKK_FS5027
Serial No. : 1508053
Model No. : XC-572-V

Reference Dry Gas Meter Data

Serial No. : 1607009
Model No. : SK25EXSR-QC6
Correction Factor (Yr) : 1.0060
Next Calibration Date : 7 Oct 22

ΔH (mm.H ₂ O)	Θ Minutes	Reference Dry Gas Meter Calibration				Console Control ; Drygas Meter						Dry Gas Meter	Orifice
		Vr (Liters)			Tr (°C)	Vm (Liters)			Ti (°C)	To (°C)	Avg.Tm (°C)	Correction	Calibration
		Final	Initial	Total		Final	Initial	Total				Factor (Y)	Factor $\Delta H@$
15	11.28	150.00	0.00	150.00	30.0	264368.6	264222.0	146.60	30.0	30.0	30.0	1.0278	39.1830
25	8.83	150.00	0.00	150.00	31.0	264526.8	264380.0	146.80	31.0	31.0	31.0	1.0254	40.1496
50	6.32	150.00	0.00	150.00	31.0	264685.2	264539.0	146.20	31.0	31.0	31.0	1.0271	41.1361
100	4.45	150.00	0.00	150.00	31.0	264845.0	264699.0	146.00	31.0	31.0	31.0	1.0236	40.7887
150	3.67	150.00	0.00	150.00	31.0	265059.0	264912.0	147.00	31.0	31.0	31.0	1.0118	41.6143
											Avg.	1.0232	40.5743

Y : Ratio of reading of reference to dry gas meter : tolerance for individual values ± 0.02 from average .

$\Delta H@$: Orifice pressure differential that equates to 21.24 lm of air @ 25 C and 760 mm of mercury , mmH₂O ; tolerance for individual values ± 5.08 from average .

Procedure; 40 CFR 60,APP A,METH ,SEC 5.3 & 7

Calibrated by:

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist(4)

Approved by:

Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)



DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	12 Jul 22	Ambient Temperature (°C) :	30
Calibration sheet No. :	C-120722-BKK_FS0528	Relative Humidity (%) :	70

Digital Temperature ID	BKK_FS0508	Reference Temperature ID. :	BKK_FS0609
Console Serial No. :	1503017	Serial No. :	7688004
Console Model :	XC-572-V	Model :	FLUKE 714
		Next Calibrate :	26 Jul 23

Location	Reference Temperature °C	Digital Temperature °C	Error °C	Remark
Stack	0	2	2	
	25	24	-1	
	50	51	1	
	100	103	3	
	150	151	1	
	200	202	2	
	250	251	1	
	300	301	1	
	500	503	3	
	1000	1001	1	
	1200	1202	2	
Probe	100	101	1	
	125	126	1	
	150	153	3	
Oven	100	101	1	
	125	126	1	
	150	151	1	
Filter	100	102	2	
	125	125	0	
	150	152	2	
Exit	0	0	0	
	10	10	0	
	20	20	0	
Meter	0	0	0	
	25	25	0	
	50	50	0	
AUX	0	0	0	
	25	25	0	
	50	50	0	

Calibrated by

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by :

Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)



Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK_FS0531 Calibration Date : 12 Jul 22
 Lab test duct Number : 258-1-13-01 Standard Pitot ID : BKK_FS0441
 Calibration Sheet No. : C-120722-BKK_FS0531 Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube (ΔP , mm.H ₂ O)	Type s pitot tube (ΔP , mm.H ₂ O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			\bar{C}_p	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P(std)}{\Delta P(s)}}$$

$$\left| \bar{C}_{p(A)} - \bar{C}_{p(B)} \right| \text{ must BE } \leq 0.01$$

$$\text{Average deviation(A or B)} = \frac{\sum_i [Cp(s) - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by : Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by : Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)



Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK_FS0532 Calibration Date : 12 Jul 22
 Lab test duct Number : 258-1-13-01 Standard Pitot ID : BKK_FS0441
 Calibration Sheet No. : C-120722-BKK_FS0532 Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube (ΔP, mm.H ₂ O)	Type s pitot tube (ΔP, mm.H ₂ O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			\bar{C}_p	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P_{(std)}}{\Delta P_{(s)}}}$$

$$\left| \bar{C}_{p(A)} - \bar{C}_{p(B)} \right| \text{ must BE } \leq 0.01$$

$$\text{Average deviation}(A \text{ or } B) = \frac{\sum_i [Cp_{(s)} - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by : Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by : Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)



PROBE NOZZLE DIAMETER
CALIBRATION DATA SHEET

Calibration Date	12 Jul 22	Nozzle Set ID. :	BKK_FS0533
Calibration Sheet No. :	C-120722-BKK_FS0533	Vernier Caliper ID. :	BKK_FS0626


Nozzle ID #	Nozzle Diameter (mm.)			Hi - Lo	$(D_1 + D_2 + D_3) / 3$
	D_1	D_2	D_3	ΔD	D_{avg}
1	0.318	0.318	0.318	0.000	0.318
2	0.475	0.475	0.475	0.000	0.475
3	0.635	0.635	0.635	0.000	0.635
4	0.792	0.792	0.792	0.000	0.792
5	0.952	0.952	0.952	0.000	0.952
6	1.110	1.110	1.110	0.000	1.110
7	1.270	1.270	1.270	0.000	1.270

Where :

D_1, D_2, D_3 = There different nozzle diameters at 60 degrees to each other, each measured the nearest 0.025 mm.

ΔD = Maximum distance between any two diameters, must be ≤ 0.100 mm.

D_{avg} = $(D_1 + D_2 + D_3) / 3$

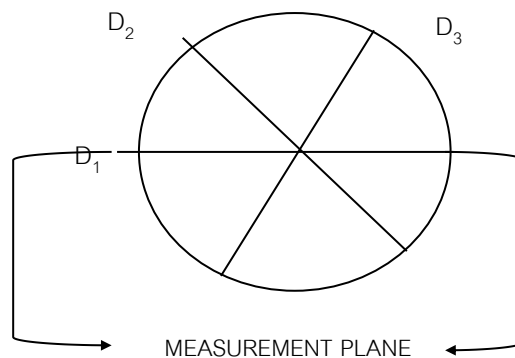

Calibrated by : Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by : Nattapon Jengwareewong

(Mr.Nattapon Jengwareewong)

Field Specialist(1)



CONSOLE CONTROL UNIT CALIBRATION TEST REPORT

Calibration of Date : 12 Jul 22
Next Cal. Date : 12 Jan 23

Barometric Pressure (mm.Hg) : 755
Relative Humidity (%) : 70.0
Temperature (°C) : 30.0

Console Control Meter Data

Calibration No. : C-120722-BKK_FS0556
Dry Gas Meter No. : BKK_FS0556
Console Serial No. : 1606041
Console Model No. : XC-572-V

Reference Dry Gas Meter Data

Serial No. : 1607009
Model No. : SK25EXSR-QC6
Correction Factor (Yr) : 1.0060
Next Calibration Date : 7 Oct 22

ΔH (mm.H ₂ O)	Θ Minutes	Reference Dry Gas Meter Calibration				Console Control ; Drygas Meter						Dry Gas Meter Correction	Orifice Calibration
		Vr (Liters)			Tr (°C)	Vm (Liters)			Ti (°C)	To (°C)	Avg.Tm (°C)	Factor (Y)	Factor $\Delta H@$
		Final	Initial	Total		Final	Initial	Total					
15	12.58	150.00	0.00	150.00	26.0	1734085.8	1733938.0	147.80	28.0	28.0	28.0	1.0263	47.7721
25	9.67	150.00	0.00	150.00	26.0	1734245.0	1734098.0	147.00	28.0	28.0	28.0	1.0309	47.0451
50	6.78	150.00	0.00	150.00	26.0	1734399.2	1734253.0	146.20	28.0	28.0	28.0	1.0340	46.2542
100	4.68	150.00	0.00	150.00	26.0	1734562.5	1734417.0	145.45	28.0	28.0	28.0	1.0343	44.0771
150	3.82	150.00	0.00	150.00	26.0	1734719.0	1734574.0	145.00	29.0	29.0	29.0	1.0360	43.9035
											Avg.	1.0323	45.8104

Y : Ratio of reading of reference to dry gas meter : tolerance for individual values ± 0.02 from average .

$\Delta H@$: Orifice pressure differential that equates to 21.24 lm of air @ 25 C and 760 mm of mercury , mmH₂O ; tolerance for individual values ± 5.08 from average .

Procedure; 40 CFR 60,APP A,METH ,SEC 5.3 & 7

Calibrated by:

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by:

Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)



DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	12-Jul-22	Ambient Temperature (°C) :	30
Calibration sheet No. :	C-120722-BKK_FS0557	Relative Humidity (%) :	70

Digital Temperature ID	BKK_FS0557	Reference Temperature ID.:	BKK_FS0609
Console Serial No. :	1606041	Serial No. :	7688004
Console Model :	XC-572-V	Model :	FLUKE 714
		Next Calibrate :	26 Jul 23

Location	Reference Temperature °C	Digital Temperature °C	Error °C	Remark
Stack	0	1	1	
	25	26	1	
	50	51	1	
	100	102	2	
	150	153	3	
	200	202	2	
	250	251	1	
	300	302	2	
	500	503	3	
	1000	1001	1	
	1200	1201	1	
Probe	100	102	2	
	125	128	3	
	150	153	3	
Oven	100	102	2	
	125	128	3	
	150	153	3	
Filter	100	102	2	
	125	128	3	
	150	153	3	
Exit	0	1	1	
	10	11	1	
	20	20	0	
Meter	0	1	1	
	25	26	1	
	50	51	1	
AUX	0	1	1	
	25	26	1	
	50	51	1	

Calibrated by

: Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by :

Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)



Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK_FS0561 Calibration Date : 12 Jul 22
 Lab test duct Number : 258-1-13-01 Standard Pitot ID : BKK_FS0441
 Calibration Sheet No. : C-120722-BKK_FS0561 Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube (ΔP, mm.H ₂ O)	Type s pitot tube (ΔP, mm.H ₂ O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			\bar{C}_p	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P(std)}{\Delta P(s)}}$$

$$\left| \bar{C}_{p(A)} - \bar{C}_{p(B)} \right| \text{ must BE } \leq 0.01$$

$$\text{Average deviation(A or B)} = \frac{\sum_i [Cp(s) - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by

Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)



Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK_FS0560 Calibration Date : 12 Jul 22
 Lab test duct Number : 258-1-13-01 Standard Pitot ID : BKK_FS0441
 Calibration Sheet No. : C-120722-BKK_FS0560 Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube (ΔP , mm.H ₂ O)	Type s pitot tube (ΔP , mm.H ₂ O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			\bar{C}_p	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P(std)}{\Delta P(s)}}$$

$$| \bar{C}_{p(A)} - \bar{C}_{p(B)} | \text{ must BE } \leq 0.01$$

$$\text{Average deviation(A or B)} = \frac{\sum_i [Cp(s) - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by

Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)



PROBE NOZZLE DIAMETER CALIBRATION DATA SHEET

Calibration Date	12 Jul 22	Nozzle Set ID. :	BKK_FS0562
Calibration Sheet No. :	C-120722-BKK_FS0562	Vernier Caliper ID. :	BKK_FS0626


Nozzle ID #	Nozzle Diameter (cm.)			Hi - Lo ΔD	$(D_1 + D_2 + D_3) / 3$ D_{avg}
	D_1	D_2	D_3		
1	0.300	0.306	0.302	0.006	0.303
2	0.480	0.475	0.480	0.005	0.478
3	0.625	0.630	0.630	0.005	0.628
4	0.755	0.750	0.765	0.015	0.757
5	0.975	0.980	0.970	0.010	0.975
6	1.095	1.090	1.095	0.005	1.093
7	1.275	1.275	1.270	0.005	1.273
8	1.610	1.610	1.610	0.000	1.610

Where :

D_1, D_2, D_3 = There different nozzle diameters at 60 degrees to each other, each measured the nearest 0.025 mm.

ΔD = Maximum distance between any two diameters, must be ≤ 0.100 mm.

D_{avg} = $(D_1 + D_2 + D_3) / 3$

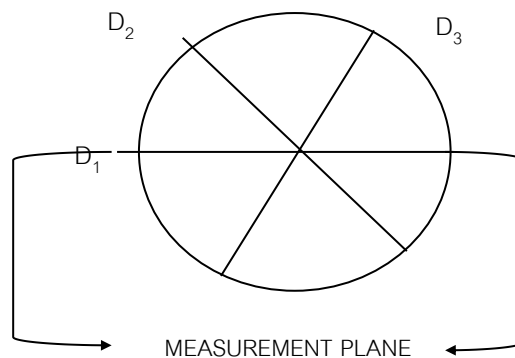

Calibrated by

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by

Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)



CONSOLE CONTROL UNIT CALIBRATION TEST REPORT

Calibration of Date : 12 Jul 22
Next Cal. Date : 12 Jan 23

Barometric Pressure (mm.Hg) : 755
Relative Humidity (%) : 70.0
Temperature (°C) : 30.0

Console Control Meter Data

Calibration No. : C-120722-BKK_FS0518
Dry Gas Meter No. : BKK_FS0518
Console Serial No. : 1504025
Console Model No. : XC-572-V

Reference Dry Gas Meter Data

Serial No. : A2003240
Model No. : DGM-SK25RM-QS8
Correction Factor (Yr) : 1.0160
Next Calibration Date : 27 May 23

ΔH (mm.H ₂ O)	\ominus Minutes	Reference Dry Gas Meter Calibration				Console Control ; Drygas Meter						Dry Gas Meter Correction	Orifice Calibration
		Vr (Liters)			Tr (°C)	Vm (Liters)			Ti (°C)	To (°C)	Avg.Tm (°C)	Factor (Y)	Factor $\Delta H@$
		Final	Initial	Total		Final	Initial	Total					
15	12.41	150.00	0.00	150.00	31.0	153838.0	153687.0	151.00	29.0	29.0	29.0	1.0012	47.8984
25	9.38	150.00	0.00	150.00	31.0	154002.0	153851.0	151.00	29.0	29.0	29.0	1.0002	45.6070
50	6.61	150.00	0.00	150.00	31.0	154164.0	154013.0	151.00	29.0	29.0	29.0	0.9978	45.2959
100	4.65	150.00	0.00	150.00	32.0	154330.0	154177.0	153.00	30.0	30.0	30.0	0.9800	44.9789
120	4.17	150.00	0.00	150.00	32.0	154616.0	154463.0	153.00	30.0	30.0	30.0	0.9781	43.4066
											Avg.	0.9915	45.4374

Y : Ratio of reading of reference to dry gas meter : tolerance for individual values ± 0.02 from average .

$\Delta H@$: Orifice pressure differential that equates to 21.24 lm of air @ 25 C and 760 mm of mercury , mmH₂O ; tolerance for individual values ± 5.08 from average .

Procedure; 40 CFR 60,APP A,METH ,SEC 5.3 & 7

Calibrated by:

(Mr.Tinnakorn Kulchart)
Field Scientist (1)

Approved by:

(Mr.Natthapol Jiengwareewong)

Field Specialist(1)



DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	12-Jul-22	Ambient Temperature (°C) :	30
Calibration sheet No. :	C-120722-BKK_FS0519	Relative Humidity (%) :	70

Digital Temperature ID	BKK_FS0519	Reference Temperature ID. :	BKK_FS1144
Console Serial No. :	1504025	Serial No. :	201090006013
Console Model :	XC-572-V	Model :	Digicon-CC-VT-MS
		Next Calibrate :	31 Jan 23

Location	Reference Temperature °C	Digital Temperature °C	Error °C	Remark
Stack	0	0	0	
	25	25	0	
	50	50	0	
	100	101	1	
	150	153	3	
	200	202	2	
	250	252	2	
	300	302	2	
	500	503	3	
	1000	1004	4	
	1200	1205	5	
Probe	100	101	1	
	125	127	2	
	150	153	3	
Oven	100	101	1	
	125	127	2	
	150	153	3	
Filter	100	101	1	
	125	127	2	
	150	153	3	
Exit	0	0	0	
	10	9	-1	
	20	19	-1	
Meter	0	0	0	
	25	24	-1	
	50	50	0	
AUX	0	0	0	
	25	25	0	
	50	50	0	

Calibrated by : _____

(Mr.tinnakorn Kulchart)

Field Scientist (1)

Approved by : _____

(Mr.Natthapol Jiengwareewong)

Field Specialist(1)



Pitot Tube Calibration Data

Pitot Tube Identification Number :	BKK_FS0522	Calibration Date :	12 Jul 22
Lab test duct Number :	258-1-13-01	Standard Pitot ID :	BKK_FS0441
Calibration Sheet No. :	C-120722-BKK_FS0522	Cp Standard :	0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube (ΔP , mm.H ₂ O)	Type s pitot tube (ΔP , mm.H ₂ O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			\bar{C}_p	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P(std)}{\Delta P(s)}}$$

$$\left| \bar{C}_{p(A)} - \bar{C}_{p(B)} \right| \text{ must BE } \leq 0.01$$

$$\text{Average deviation(A or B)} = \frac{\sum_i [Cp(s) - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by : _____

(Mr.Tinnakorn Kulchart)

Field Scientist ()

Approved by : _____

(Mr.Natthapol Jiengwareewong)

Field Specialist(1)



Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK_FS0523

Calibration Date : 12 Jul 22

Lab test duct Number : 258-1-13-01

Standard Pitot ID : BKK_FS0441

Calibration Sheet No. : C-120722-BKK_FS0523

Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube (ΔP , mm.H ₂ O)	Type s pitot tube (ΔP , mm.H ₂ O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			\bar{C}_p	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P_{(std)}}{\Delta P_{(s)}}}$$

$$\left| \bar{C}_{p(A)} - \bar{C}_{p(B)} \right| \text{ must BE } \leq 0.01$$

$$\text{Average deviation(A or B)} = \frac{\sum_i [Cp_{(s)} - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by : _____

(Mr.tinnakorn Kulchar)

Field Scientist (1)

Approved by : _____

(Mr.Natthapol Jiengwareewong)

Field Specialist(1)



PROBE NOZZLE DIAMETER
CALIBRATION DATA SHEET

Calibration Date	12 Jul 22	Nozzle Set ID. :	BKK_FS0524
Calibration Sheet No. :	C-120722-BKK_FS0524	Vernier Caliper ID. :	BKK_FS0626


Nozzle ID #	Nozzle Diameter (cm.)			Hi - Lo	$(D_1 + D_2 + D_3) / 3$
	D_1	D_2	D_3	ΔD	D_{avg}
1	0.318	0.318	0.318	0.000	0.318
2	0.475	0.475	0.475	0.000	0.475
3	0.635	0.635	0.635	0.000	0.635
4	0.792	0.792	0.792	0.000	0.792
5	0.952	0.952	0.952	0.000	0.952
6	1.110	1.110	1.110	0.000	1.110
7	1.270	1.270	1.270	0.000	1.270

Where :

D_1, D_2, D_3 = There different nozzle diameters at 60 degrees to each other, each measured the nearest 0.025 mm.

ΔD = Maximum distance between any two diameters, must be ≤ 0.100 mm.

D_{avg} = $(D_1 + D_2 + D_3) / 3$

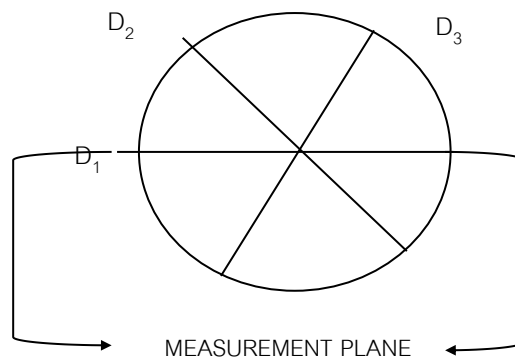

Calibrated by : _____

(Mr.tinnakorn Kulcha)

Field Scientist (1)

Approved by : _____

(Mr.Natthapol Jiengwareewong)

Field Specialist(1)



Certificate of Calibration

Represent to Certificate of Calibration ,PTC/07/22099

Certificate No.:	PTC/07/22099	Page:	1 of 2
Equipment:	Digital Balance	Condition:	Normal
Manufacturer:	Sartorius	Serial No:	31709552
Model:	MSU224S-100-DU	ID No:	RYG_EN0003
Type of Balance:	Single interval		



Customer: ALS Laboratory Group (Thailand) Co.,Ltd.
616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand

Environment Condition: Temperature 23.9 °C \pm 0.3 °C
Humidity 58.1 %RH \pm 4.4 %RH
Air density 1.17 kg/m³



Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd.
616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand

The Method used: In house method, PTC-WI-07, base on Euramet cg. 18

Traceability: This certificate is traceable to the SI Units through Thai Calibration Service Co.,Ltd.
, NSC-ONSC Accreditation No.: Calibration 0189

Date Received: March 23, 2022

Calibration Date: March 23, 2022

Issued Date: March 25, 2022

Calibration By: Mr. Rungroje Metakul



PENTA CALIBRATION CO.,LTD

[Signature]

(Mr.Kriangsak Kalasri)

Reviewed by

Approved By :

[Signature]

(Mr. Keattisak Kerdto)

Laboratory Manager

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognised national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The effect that the results relate only to the items calibrated.

This calibration certificate shall not be reproduced except in full only, without written approval from penta calibration co ., ltd



Represent to Certificate of Calibration ,PTC/07/22099

Certificate No.: PTC/07/22099



Page: 2 of 2

Measurement Results:

Without Adjustment :

Function Calibration: Non Adjustment

Eccentric Error: Weight to be 1/3 ,1/2 or of Maximum capacity

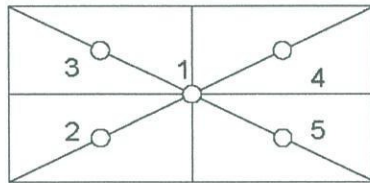

Eccentricity test 100 (g)

Position (g)				
1	2	3	4	5
0.0000	0.0000	-0.0001	-0.0001	0.0001
Maximum deviation:				0.0001

Repeatability Test : Weight to be $1/2 \leq L_1 \leq$ Maximum capacity

Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
20	0.000042
200	0.000071

Error of indication : from nominal value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Indication (g)	Correction of Balance (g)	Uncertainty (g)	k
0	0.00000	0.0000	0.0000	0.00020	2.65
0.01	0.01000	0.0099	0.0001	0.00020	2.43
0.1	0.10000	0.1000	0.0000	0.00020	2.43
0.5	0.50000	0.5000	0.0000	0.00020	2.43
1	1.00000	1.0000	0.0000	0.00020	2.43
5	5.00001	5.0000	0.0000	0.00020	2.43
10	10.00000	10.0000	0.0000	0.00020	2.43
20	20.00003	20.0000	0.0000	0.00020	2.43
50	50.00004	50.0000	0.0000	0.00021	2.32
100	100.00004	99.9999	0.0001	0.00022	2.17
200	200.00011	200.0000	0.0001	0.00027	2.05

Note: Weight of adjust - (g)


The End of Certificate





High Volume Air Sampler Calibration Worksheet

Project Site :	Kiriu (Thailand) Co., Ltd.	Barometric Pressure (mm Hg) :	756
Calibrate Location :	วัดจอมพลเจ้าพระยา	Temperature (°C) :	30
Calibrate Date :	25-Sep-22	High Volume ID :	RYG_FS0177
CalibrationSheet No.:	C-250922-RYG_FS0177	High Volume Model :	TE-5170D
Calibrator ID:	BKK_FS0625	High Volume S/N :	4803
Calibrator Model :	TE-5028A	Calibrator Slope :	1.67326
Calibrator S/N :	2585	Calibrator Intercept :	-0.01954

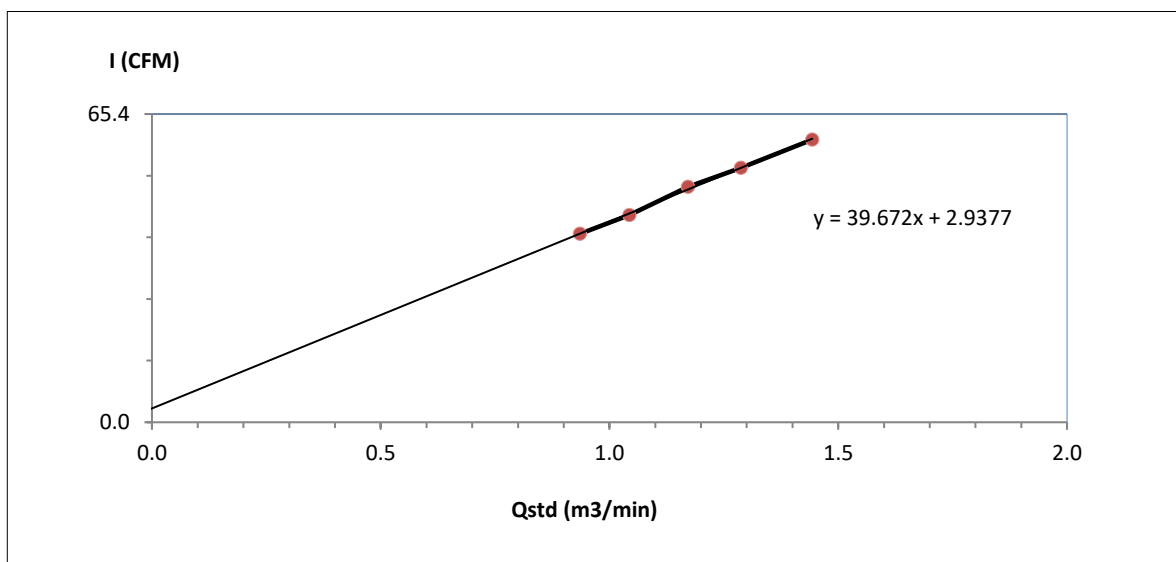Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.4	0.9353	40	Slope : 39.6720 Intercept : 2.9377 Correlation Coefficient : 0.9991
2	3.0	1.0434	44	
3	3.8	1.1718	50	
4	4.6	1.2873	54	
5	5.8	1.4431	60	



Calibrated by 
 (Mr. Saknarin jaraskay)
 Field Scientist(1)


Approved by : 
 (Mr. Noppong Juntarupan)
 Enviro Field Coordinator Scientist (3)



High Volume Air Sampler Calibration Worksheet

Project Site :	Kiriu (Thailand) Co., Ltd.	Barometric Pressure (mm Hg) :	756
Calibrate Location :	วัดคลองกร้า	Temperature (°C) :	30
Calibrate Date :	25-Sep-22	High Volume ID :	RYG_FS0395
CalibrationSheet No.:	C-250922-RYG_FS0395	High Volume Model :	TE-5170D
Calibrator ID:	BKK_FS0625	High Volume S/N :	5692
Calibrator Model :	TE-5028A	Calibrator Slope :	1.67326
Calibrator S/N :	2585	Calibrator Intercept :	-0.01954

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.6	0.9727	40	Slope : 39.8719 Intercept : 1.0406 Correlation Coefficient : 0.9990
2	3.2	1.0770	44	
3	4.2	1.2310	50	
4	5.0	1.3413	54	
5	6.0	1.4675	60	

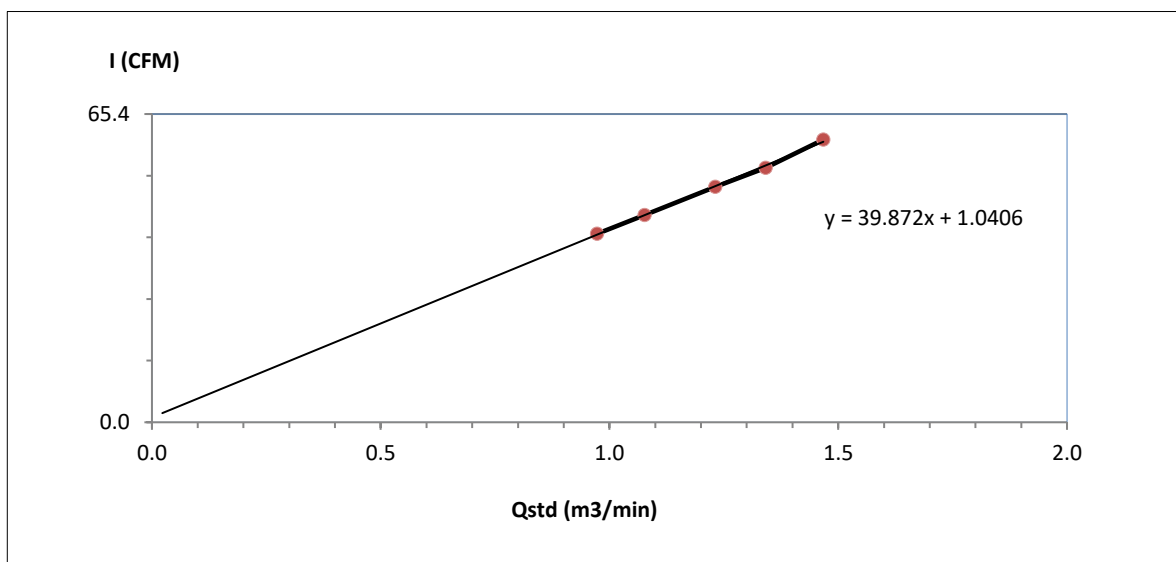

Calibrated by _____

(Mr. Saknarin jaraskay)
Field Scientist(1)

Approved by : _____


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)





High Volume Air Sampler Calibration Worksheet

Project Site :	Kiriu (Thailand) Co., Ltd.	Barometric Pressure (mm Hg) :	756
Calibrate Location :	วัดราษฎร์ศุภคาราม	Temperature (°C) :	30
Calibrate Date :	25-Sep-22	High Volume ID :	RYG_FS0394
CalibrationSheet No.:	C-250922-RYG_FS0394	High Volume Model :	TE-5170D
Calibrator ID:	BKK_FS0625	High Volume S/N :	5690
Calibrator Model :	TE-5028A	Calibrator Slope :	1.67326
Calibrator S/N :	2585	Calibrator Intercept :	-0.01954

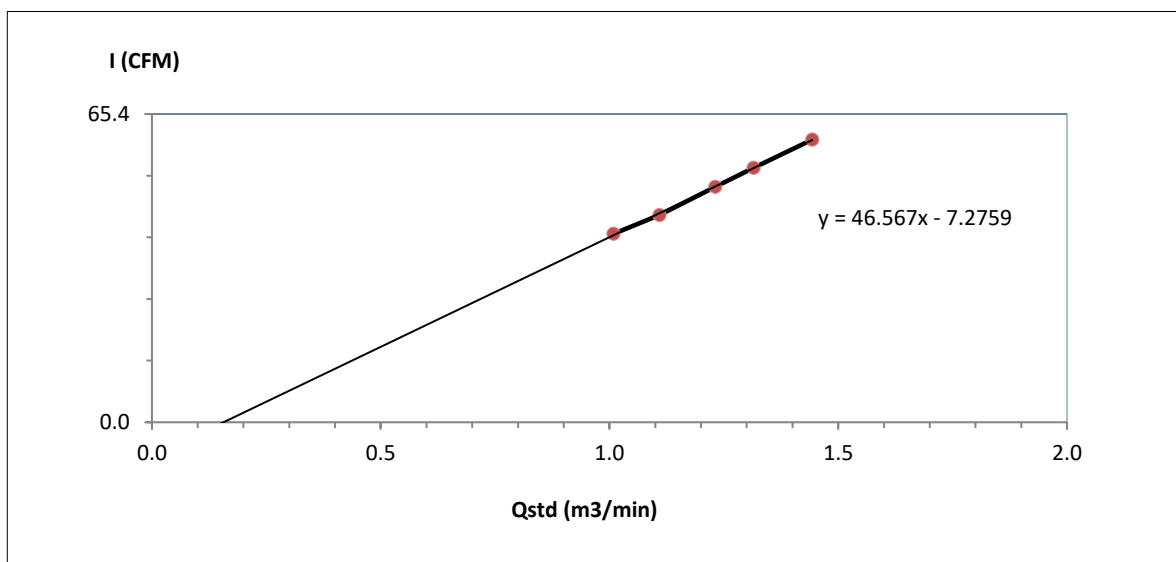Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.8	1.0087	40	Slope : 46.5668 Intercept : -7.2759 Correlation Coefficient : 0.9995
2	3.4	1.1095	44	
3	4.2	1.2310	50	
4	4.8	1.3146	54	
5	5.8	1.4431	60	



Calibrated by 
(Mr. Saknarin jaraskay)
Field Scientist(1)

Approved by : 
(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)




Certificate of Calibration

Represent to Certificate of Calibration ,PTC/07/22102

Certificate No.:	PTC/07/22102	Page:	1 of 2
Equipment:	Digital Balance	Condition:	Normal
Manufacturer:	Sartorius	Serial No:	25409664
Model:	LA130S-F	ID No:	RYG_EN0001
Type of Balance:	Single interval		



Customer: ALS Laboratory Group (Thailand) Co.,Ltd.
616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand

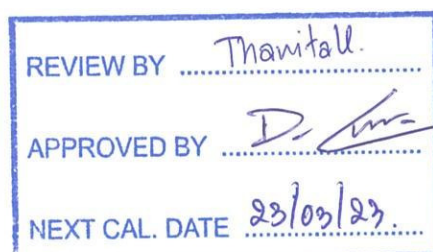

Environment Condition: Temperature 23.9 °C \pm 0.3 °C
Humidity 58.1 %RH \pm 4.4 %RH
Air density 1.17 kg/m³

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd.
616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand

The Method used: In house method, PTC-WI-07, base on Euramet cg. 18

Traceability: This certificate is traceable to the SI Units through Thai Calibration Service Co.,Ltd.
, NSC-ONSC Accreditation No.: Calibration 0189

Date Received: March 23, 2022

Calibration Date: March 23, 2022

Issued Date: March 25, 2022

Calibration By: Mr. Rungroje Metakul



PENTA CALIBRATION CO.,LTD

(Mr.Kriangsak Kalasri)

Reviewed by

Approved By :

(Mr. Keattisak Kerdto)

Laboratory Manager

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognised national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The effect that the results relate only to the items calibrated.

This calibration certificate shall not be reproduced except in full only, without written approval from penta calibration co., ltd



Represent to Certificate of Calibration ,PTC/07/22102

Certificate No.: PTC/07/22102



Page: 2 of 2

Measurement Results:

Without Adjustment :

Function Calibration: Non Adjustment

Eccentric Error: Weight to be 1/3 ,1/2 or of Maximum capacity

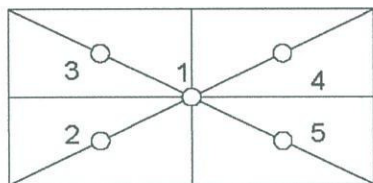

Eccentricity test 50 (g)

Position (g)				
1	2	3	4	5
0.0000	0.0000	-0.0001	0.0000	0.0001
Maximum deviation:			0.0001	

Repeatability Test : Weight to be $1/2 \leq L_1 \leq$ Maximum capacity

Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
10	0.00047
100	0.000089

Error of indication : from nominal value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Indication (g)	Correction of Balance (g)	Uncertainty (g)	k
0	0.00000	0.0000	0.0000	0.00026	2.87
0.01	0.01000	0.0100	0.0000	0.00026	2.65
0.05	0.05000	0.0500	0.0000	0.00026	2.65
0.1	0.10000	0.1000	0.0000	0.00026	2.65
0.5	0.50000	0.4999	0.0001	0.00026	2.65
1	1.00000	0.9999	0.0001	0.00026	2.65
2	2.00000	1.9999	0.0001	0.00026	2.65
5	5.00001	5.0000	0.0000	0.00026	2.65
10	10.00000	10.0001	-0.0001	0.00026	2.65
20	20.00003	20.0001	-0.0001	0.00026	2.52
100	100.00004	100.0001	-0.0001	0.00027	2.18

Note: Weight of adjust - (g)

The End of Certificate

CERTIFICATE OF CALIBRATION

Certificate No: WS-01072021

Page 1 of 2 pages

Measurement Item : Cup anemometer with data logger.

Manufacturer : Data logger: Novalynx.
: Cup anemometer: Novalynx.

Model/Type : Data logger: 110-WS-16N.
: Cup anemometer: WS-02E.

Serial Number : Data logger: 1159.
: Cup anemometer: -.

ID No : Data logger: RYG_FS0081.
: Cup anemometer: -.

Customer : ALS laboratory group (Thailand) co., Ltd.
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

Test Conditions : Wind tunnel cross test section area 900 cm²
: Anemometer frontal area 100 cm²
: Diameter of mounting pipe - mm
: Blockage ratio of test object 0.111 [-]

Test Conditions : Air temperature 23.9 ±0.8 °C
: Air pressure 1010.8 ±0.4 hPa
: Relative air humidity 52.8 ±3.5 %RH

Calibration Procedure Calibration was carried out base on;
IEC 61400-12-1 ED.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines;
MEASNET Anemometer Calibration Procedure – Version 2: 2009;

Traceability This calibration documents the traceable to national standard, Which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).

Measurement Date : Jul 05, 2021.

Issued Date : Jul 08, 2021.


REVIEW BY *Navakorn P.*

APPROVED BY *[Signature]*

NEXT CAL. DATE *3/1/23*

Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya

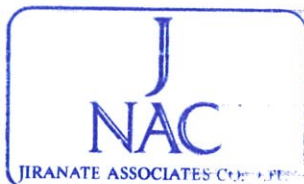

Approved Signatory:

[Signature]

Mr. Parinya Booncharoen
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-01072021

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 2 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V _{STD} Reading m/s	V _{UUC} Reading m/s	Error (m/s)	Uncertainty (%)
2.071	1.8	-0.3	2.7
4.089	3.8	-0.3	1.1
6.01	5.9	-0.1	1.03
8.01	7.8	-0.2	0.74
10.03	10.0	0.0	0.60
12.00	12.0	0.0	0.48
14.05	14.2	0.1	0.38
16.04	16.3	0.3	0.33
14.99	15.2	0.2	0.39
12.99	13.1	0.1	0.46
10.96	11.0	0.0	0.49
9.03	8.9	-0.1	0.66
7.01	6.9	-0.1	0.88
5.168	4.9	-0.3	1.00
3.011	2.7	-0.3	1.9

UUC*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TESTO INC.	06352145	July 16, 2020	MW-0035-20	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	July 16, 2020	MW-0035-20	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	July 20, 2020	MW-0036AA-20	0 - 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2021	CL-027-64	-30 - 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2021	RH-03032021	0 – 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2021	BP-01032021	500 – 1100 hPa
7	Wind tunnel	ESSOM	MP330D	-	-	0 – 50 Hz

End of certificate of calibration



CERTIFICATE OF CALIBRATION

Certificate No.: WD-01072021

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.
: Wind direction sensor: Novalynx.

Model/Type : Data logger: 110-WS-16N.
: Wind direction sensor: WS-02E.

Serial Number : Data logger: 1159.
: Wind direction sensor: -.

ID No : Data logger: RYG_FS0081.
: Cup anemometer: -.

Customer : ALS laboratory group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(23\pm3)^{\circ}\text{C}$, and relative humidity of $(40\pm10)\%$.

Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control, The measurement were taken at 45° intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: CC563-07-0045,
Certificate No.: KWS63/0044.

Measurement Date : Jul 05, 2021.

Issued Date : Jul 08, 2021.

Performed by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:.....



Mr. Parinya Booncharoen.
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-01072021

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	360	359	-1	3.0
2		45	45	41	-4	3.0
3		90	90	87	-3	3.0
4		135	135	132	-3	3.0
5		180	180	179	-1	3.0
6		225	225	227	2	3.0
7		270	270	273	3	3.0
8		315	315	317	2	3.0
9	Counter Clockwise	0/360	360	359	-1	3.0
10		45	45	41	-4	3.0
11		90	90	87	-3	3.0
12		135	135	132	-3	3.0
13		180	180	179	-1	3.0
14		225	225	227	2	3.0
15		270	270	273	3	3.0
16		315	315	317	2	3.0

UUC*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor $k=2$ providing a level of confidence of approximately 95%

End of Certificate of Calibration



SITHIPHORN ASSOCIATES CO.,LTD.

CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd., Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACC22001

Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR
Manufacturer : RION
Model : NC-75
Serial No.: 35002736
ID No.: - RY60496

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 05 JANUARY 2022
Calibration Date : 10 JANUARY 2022
Date of Issue : 13 JANUARY 2022

REVIEW BY	Narakorn P.
APPROVED BY	[Signature]
NEXT CAL. DATE	10/1/23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACC22001

Job No. : VC65AC0040

Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	33461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22
Audio Analyzer	AVR-3360A	V744B6069	EF-0010-21	10-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACC22001

Job No. : VC65AC0040

Pages : 3 of 3

Result of calibration :**1. Sound pressure level**

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit (dB)
94	93.99	-0.01	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Tolerance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Tolerance limit (%)
0.28	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL22058

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00296518 / 179118 / 87525
ID No.: RYG_FS0431

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 14 JANUARY 2022
Calibration Date : 21-24 JANUARY 2022
Date of Issue : 25 JANUARY 2022

REVIEW BY	<i>Narakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	<i>21/1/23</i>

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22058

Job No. : VC65AC0043

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22058
Job No. : VC65AC0043
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22058

Job No. : VC65AC0043

Pages : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.96)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.6
C - weight	17.6
Flat	23.2

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.1	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.8	0.9	0.9	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22058
Job No. : VC65AC0043
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	-0.1	±1.5
250	-0.1	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22058
Job No. : VC65AC0043
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.1	0.1	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22058

Job No. : VC65AC0043

Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.8	-0.6	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22058

Job No. : VC65AC0043

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.7	89.7	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



NSC-TISI-TIS 17025
CALIBRATION 0394

451-451/1 Sirinthorn Rd., Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

Cert. No. : ACL22055

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00296515 / 179119 / 87526
ID No.: RYG_FS0432

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 14 JANUARY 2022
Calibration Date : 21-24 JANUARY 2022
Date of Issue : 25 JANUARY 2022

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	21/1/22 ^{WPK}

23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22055
Job No. : VC65AC0043
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22055
Job No. : VC65AC0043
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22055

Job No. : VC65AC0043

Pages : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.96)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.6
C - weight	17.7
Flat	23.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.1	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-0.2	-0.2	-0.2	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22055
Job No. : VC65AC0043
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22055

Job No. : VC65AC0043

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	63.9	-0.1	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.1	0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22055

Job No. : VC65AC0043

Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22055

Job No. : VC65AC0043

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

————— **End of Calibration Certificate** —————

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd., Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL22026

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00900071 / 188464 / 01733
ID No.: RYG_FS0492

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 05 JANUARY 2022
Calibration Date : 10-12 JANUARY 2022
Date of Issue : 13 JANUARY 2022

REVIEW BY	<i>Marathon P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	10/1/23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22026

Job No. : VC65AC0040

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22026

Job No. : VC65AC0040

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22026

Job No. : VC65AC0040

Pages : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.96)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.6
C - weight	17.8
Flat	23.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.2	0.2	0.2	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	0.2	0.3	0.3	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22026

Job No. : VC65AC0040

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22026
Job No. : VC65AC0040
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.8	-0.2	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22026

Job No. : VC65AC0040

Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.1	0.1	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22026

Job No. : VC65AC0040

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL22024

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00709746 / 187332 / 01297
ID No.: RYG_FS0491

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 05 JANUARY 2022
Calibration Date : 10-12 JANUARY 2022
Date of Issue : 13 JANUARY 2022

VIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	10/1/23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22024

Job No. : VC65AC0040

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22024
Job No. : VC65AC0040
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22024

Job No. : VC65AC0040

Pages : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.96)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	13.4
C - weight	19.8
Flat	25.2

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.1	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.1	1.2	1.2	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22024

Job No. : VC65AC0040

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22024

Job No. : VC65AC0040

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22024

Job No. : VC65AC0040

Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.5	-0.9	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.1	0.1	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22024

Job No. : VC65AC0040

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	136.9	0.1	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

CERTIFICATE OF CALIBRATION

Certificate No.: CL-054-65

Page 1 of 2

Equipment Name: Digital thermometer with RTD

Manufacturer.: DeltaOHM

Model: HD32.2

Serial No: 15006716

ID No: RYG_FS0221

Customer

Name: ALS laboratory group (thailand) Co.,Ltd.

Address: 104 Phatthanakan 40, Phatthanakan
Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok
10250 Thailand.

Received date: 15 MAR 2022

Calibration date: 17 MAR 2022

Issue date: 18 MAR 2022

Reference Used During Calibration

1.Standard Temperature Probe Model: STS-100 A500,
Serial No.: 667682-09, Due date: 25 Mar 2022

2.Digital Temperature Indicator Model: DTI-1000-A MK
II, Serial No.: 671407-00591 Due date: 04 June 2022

Calibration Condition

Temperature: $(23 \pm 3)^{\circ}\text{C}$

Relative Humidity: $(55 \pm 15)\%$

Calibration Procedure

The temperature calibration was done by In-House
calibration method as WI-CL-001 according to
comparison method with standard digital temperature
indicator and standard temperature probe. The
temperature scale use was based on ITS-90.


Traceability

The measurement results are traceable to the
international system of units (SI) through National
Institute of Metrology Thailand (NIMT) Certificate
number: TT-0036-21, Certificate number: ER-0032-
21

REVIEW BY	<i>Marakon P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	17/3/23

Calibrated by

- ☐ Mr. Sorawit Thachalad
☒ Miss Orathai Wiwatwittaya

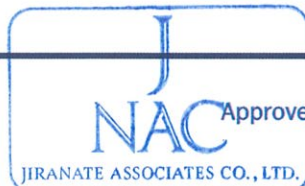

Approved Signatory:

[Signature]
Mr. Parinya Booncharoen
Calibration Department Manager

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 – 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 18009587
Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.082	20.1	0.0	0.099
30	25.076	25.1	0.0	0.099
30	30.069	30.0	-0.1	0.099
30	35.064	35.0	-0.1	0.099
30	40.055	40.0	-0.1	0.099

Table 2: This equipment was connected with temperature probe Model: TP3207.2 S/N: 15015492
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.080	20.4	0.3	0.099
70	25.076	25.2	0.1	0.099
70	30.068	30.0	-0.1	0.099
70	35.065	34.8	-0.3	0.099
70	40.057	39.6	-0.5	0.099

Table 3: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 15015967.
Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.082	20.0	-0.1	0.099
110	25.076	25.0	-0.1	0.099
110	30.069	30.0	-0.1	0.099
110	35.064	35.0	-0.1	0.099
110	40.055	40.0	-0.1	0.099

UUC* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

* End of Certificate *



CERTIFICATE OF CALIBRATION

Certificate No. : CL-095-64
Page 1 of 2

Equipment Name : Heat Stress Monitor with Sensor
Manufacturer. : DeltaOHM
Model: HD32.2
Serial No: 15006713
ID No: RYG_FS0218

Customer

Name: ALS laboratory group (thailand) Co.,Ltd.
Address: 104 Phatthanakan 40, Phatthanakan
Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok
10250 Thailand.

Received date: 8 DEC 2021

Calibration date: 13 DEC 2021

Issue date: 14 DEC 2021

Reference Used During Calibration

- 1.Standard Temperature Probe Model: STS-100 A500,
Serial No.: 667682-09, Due date: 25 Mar 2022
- 2.Digital Temperature Indicator Model: DTI-1000-A MK
II, Serial No.: 671407-00591 Due date: 04 June 2022

Calibration Condition

Temperature: (23±3)°C
Relative Humidity: (55±15)%

Calibration Procedure

The temperature calibration was done by In-House
calibration method as WI-CL-001 according to
comparison method with standard digital temperature
indicator and standard temperature probe. The
temperature scale use was based on ITS-90.

Traceability

The measurement results are traceable to the
international system of units (SI) through National
Institute of Metrology Thailand (NIMT) Certificate
number: TT-0036-21, Certificate number: ER-0032-
21

REVIEW BY	<i>Nirakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	13/12/22

Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:

[Signature]
Mr. Parinya Booncharoen
Technical Support
and Calibration Manager

Result of Calibration:- ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 – 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 15015847.
Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.056	20.2	0.1	0.099
30	25.045	25.2	0.2	0.099
30	30.039	30.2	0.2	0.099
30	35.033	35.2	0.2	0.099
30	40.025	40.2	0.2	0.099

Table 2: This equipment was connected with temperature probe Model: TP3207.2 S/N: 15015499.
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.060	20.1	0.0	0.099
70	24.878	25.0	0.1	0.099
70	29.828	29.9	0.1	0.099
70	34.794	34.8	0.0	0.099
70	39.748	39.7	0.0	0.099

Table 3: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 20019647.
Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.059	20.2	0.1	0.099
110	25.050	25.2	0.2	0.099
110	30.038	30.3	0.3	0.099
110	35.033	35.3	0.3	0.099
110	40.024	40.3	0.3	0.099

UUC* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.



CERTIFICATE OF CALIBRATION

Certificate No. : CL-015-65
Page 1 of 2

Equipment Name: Heat Stress Monitor with Sensor
Manufacturer.: DeltaOHM
Model: HD32.2
Serial No: 15006714
ID No: RYG_FS0219

Customer

Name: ALS laboratory group (thailand) Co.,Ltd.
Address: 104 Phatthanakan 40, Phatthanakan
Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok
10250 Thailand.

Received date: 10 JAN 2022
Calibration date: 14 FEB 2022
Issue date: 17 FEB 2022

Reference Used During Calibration

1.Standard Temperature Probe Model: STS-100 A500,
Serial No.: 667682-09, Due date: 25 Mar 2022
2.Digital Temperature Indicator Model: DTI-1000-A MK
II, Serial No.: 671407-00591 Due date: 04 June 2022

Calibration Condition

Temperature: (23±3)°C
Relative Humidity: (55±15)%

Calibration Procedure

The temperature calibration was done by In-House
calibration method as WI-CL-001 according to
comparison method with standard digital temperature
indicator and standard temperature probe. The
temperature scale use was based on ITS-90.

Traceability

The measurement results are traceable to the
international system of units (SI) through National
Institute of Metrology Thailand (NIMT) Certificate
number: TT-0036-21, Certificate number: ER-0032-
21

REVIEW BY	<i>Marakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	14/2/23

Calibrated by

- ☐ Mr. Sorawit Thachalad
☒ Miss Orathai Wiwatwittaya



Approved Signatory:

[Signature]
Mr. Parinya Booncharoen
Calibration Department Manager

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 – 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 15003276.

Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.053	20.3	0.2	0.099
30	25.030	25.3	0.3	0.099
30	30.019	30.3	0.3	0.099
30	35.017	35.3	0.3	0.099
30	40.010	40.3	0.3	0.099

Table 2: This equipment was connected with temperature probe Model: TP3207.2 S/N: 15015491.

Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.051	20.1	0.0	0.099
70	24.990	25.0	0.0	0.099
70	29.917	30.0	0.1	0.099
70	34.873	35.0	0.1	0.099
70	39.864	39.9	0.0	0.099

Table 3: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 17023217.

Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.054	20.2	0.1	0.099
110	25.035	25.2	0.2	0.099
110	30.018	30.2	0.2	0.099
110	35.015	35.2	0.2	0.099
110	40.003	40.2	0.2	0.099

UUC* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

* End of Certificate *



CERTIFICATE OF CALIBRATION

Certificate No. : CL-096-64
Page 1 of 2

Equipment Name : Heat Stress Monitor with Sensor
Manufacturer. : DeltaOHM
Model: HD32.2
Serial No: 15006715
ID No: RYG_FS0220

Customer

Name: ALS laboratory group (thailand) Co.,Ltd.
Address: 104 Phatthanakan 40, Phatthanakan
Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok
10250 Thailand.

Received date: 22 DEC 2021
Calibration date: 28 DEC 2021
Issue date: 29 DEC 2021

Reference Used During Calibration

1.Standard Temperature Probe Model: STS-100 A500,
Serial No.: 667682-09, Due date: 25 Mar 2022
2.Digital Temperature Indicator Model: DTI-1000-A MK
II, Serial No.: 671407-00591 Due date: 04 June 2022

Calibration Condition

Temperature: (23±3)°C
Relative Humidity: (55±15)%

Calibration Procedure

The temperature calibration was done by In-House
calibration method as WI-CL-001 according to
comparison method with standard digital temperature
indicator and standard temperature probe. The
temperature scale use was based on ITS-90.


Traceability

The measurement results are traceable to the
international system of units (SI) through National
Institute of Metrology Thailand (NIMT) Certificate
number: TT-0036-21, Certificate number: ER-0032-
21

REVIEW BY *Warakorn P.*
APPROVED BY *Wichai Chm.*
NEXT CAL. DATE *28/12/22*

Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya

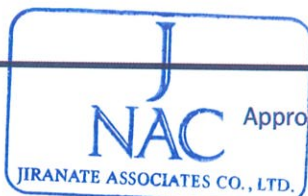

Approved Signatory: *2Jempb.*

Mr. Parinya Booncharoen
Technical Support
and Calibration Manager

Result of Calibration:- ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 – 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 15006715.
Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.056	20.0	-0.1	0.099
30	25.049	25.0	0.0	0.099
30	30.038	30.0	0.0	0.099
30	35.031	35.0	0.0	0.099
30	40.022	39.9	-0.1	0.099

Table 2: This equipment was connected with temperature probe Model: TP3207.2 S/N: 15015507.
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.058	20.2	0.1	0.099
70	24.879	25.0	0.1	0.099
70	29.832	29.8	0.0	0.099
70	34.801	34.7	-0.1	0.099
70	39.767	39.6	-0.2	0.099

Table 3: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: -.
Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.056	20.1	0.0	0.099
110	25.050	25.1	0.1	0.099
110	30.038	30.1	0.1	0.099
110	35.032	35.1	0.1	0.099
110	40.024	40.1	0.1	0.099

UUC* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

* End of Certificate *



CERTIFICATE OF CALIBRATION

Certificate No. : CL-097-64
Page 1 of 2

Equipment Name : Heat Stress Monitor with Sensor
Manufacturer. : DeltaOHM
Model: HD32.2
Serial No: 15006718
ID No: RYG_FS0223

Customer

Name: ALS laboratory group (thailand) Co.,Ltd.
Address: 104 Phatthanakan 40, Phatthanakan
Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok
10250 Thailand.

Received date: 22 DEC 2021
Calibration date: 28 DEC 2021
Issue date: 29 DEC 2021

Reference Used During Calibration

1. Standard Temperature Probe Model: STS-100 A500,
Serial No.: 667682-09, Due date: 25 Mar 2022
2. Digital Temperature Indicator Model: DTI-1000-A MK
II, Serial No.: 671407-00591 Due date: 04 June 2022

Calibration Condition

Temperature: $(23 \pm 3)^\circ\text{C}$
Relative Humidity: $(55 \pm 15)\%$

Calibration Procedure

The temperature calibration was done by In-House
calibration method as WI-CL-001 according to
comparison method with standard digital temperature
indicator and standard temperature probe. The
temperature scale use was based on ITS-90.

Traceability

The measurement results are traceable to the
international system of units (SI) through National
Institute of Metrology Thailand (NIMT) Certificate
number: TT-0036-21, Certificate number: ER-0032-
21

REVIEW BY	<i>Nasakorn P.</i>
APPROVED BY	<i>rich ch</i>
NEXT CAL. DATE	<i>28/12/22</i>

Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:

2Kmpd.
Mr. Parinya Booncharoen
Technical Support
and Calibration Manager

Result of Calibration:- ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 – 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 18009588.
Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u>	<u>Standard</u>	<u>UUC</u>	<u>Error</u>	<u>Uncertainty</u>
<u>Depth</u>	<u>Reading</u>	<u>Reading</u>	<u>(°C)</u>	<u>(°C)</u>
(mm)	(°C)	(°C)		
30	20.057	20.1	0.0	0.099
30	25.050	25.1	0.1	0.099
30	30.037	30.1	0.1	0.099
30	35.032	35.0	0.0	0.099
30	40.016	40.0	0.0	0.099

Table 2: This equipment was connected with temperature probe Model: TP3207.2 S/N: 15015496.
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u>	<u>Standard</u>	<u>UUC</u>	<u>Error</u>	<u>Uncertainty</u>
<u>Depth</u>	<u>Reading</u>	<u>Reading</u>	<u>(°C)</u>	<u>(°C)</u>
(mm)	(°C)	(°C)		
70	20.057	20.2	0.1	0.099
70	24.877	25.0	0.1	0.099
70	29.832	29.9	0.1	0.099
70	34.791	34.8	0.0	0.099
70	39.750	39.7	0.0	0.099

Table 3: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: -.
Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u>	<u>Standard</u>	<u>UUC</u>	<u>Error</u>	<u>Uncertainty</u>
<u>Depth</u>	<u>Reading</u>	<u>Reading</u>	<u>(°C)</u>	<u>(°C)</u>
(mm)	(°C)	(°C)		
110	20.057	20.2	0.1	0.099
110	25.050	25.2	0.1	0.099
110	30.038	30.2	0.2	0.099
110	35.032	35.2	0.2	0.099
110	40.016	40.3	0.3	0.099

UUC* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

* End of Certificate *



CERTIFICATE OF CALIBRATION

Certificate No. : CL-136-65
Page 1 of 2

Equipment Name: Heat Stress Monitor
Manufacturer.: DeltaOHM
Model: HD32.2
Serial No: 15020724
ID No: RYG_FS0228

Customer

Name: ALS laboratory group (thailand) Co.,Ltd.
Address: 104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

Received date: 23 Aug 2022
Calibration date: 25 Aug 2022
Issue date: 9 Sep 2022

Reference Used During Calibration

1.Standard Temperature Probe Model: STS-100 A500,
Serial No.: 667682-09, Due date: 23 Mar 2023
2.Digital Temperature Indicator Model: DTI-1000-A MK II,
Serial No.: 671407-00591 Due date: 22 July 2023

Calibration Condition

Temperature: $(23 \pm 3)^{\circ}\text{C}$
Relative Humidity: $(55 \pm 15)\%$

Calibration Procedure

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.


Traceability

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0034-22, Certificate number: ER-0092-22

REVIEW BY	<i>Manakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	25/8/23

Calibrated by

- ☐ Mr. Sorawit Thachalad
☒ Miss Jittrapon Lertsomphol

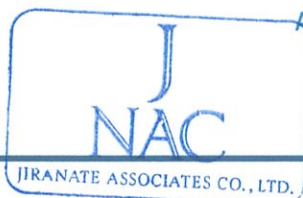

Approved Signatory:

[Signature]
Mr. Parinya Booncharoen
Calibration Department Manager

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 – 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 15003276.
Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.043	20.1	0.1	0.099
30	25.038	25.1	0.1	0.099
30	30.032	30.0	0.0	0.099
30	35.026	35.0	0.0	0.099
30	40.017	40.0	0.0	0.099

Table 2: This equipment was connected with temperature probe Model: TP3207.2 S/N: 15031951.
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.044	20.3	0.2	0.099
70	25.038	25.1	0.1	0.099
70	30.032	30.0	0.0	0.099
70	35.025	34.8	-0.2	0.099
70	40.018	39.7	-0.3	0.099


Table 3: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 15028490.
Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.044	20.0	0.0	0.099
110	25.038	25.0	0.0	0.099
110	30.032	30.0	0.0	0.099
110	35.026	35.0	0.0	0.099
110	40.018	40.0	0.0	0.099

UUC* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

✱ End of Certificate ✱

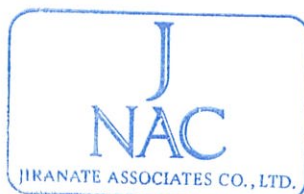

CERTIFICATE OF CALIBRATION

Certificate No. : CL-096-64
Page 1 of 2

Equipment Name : Heat Stress Monitor with Sensor
Manufacturer. : DeltaOHM
Model: HD32.2
Serial No: 15006715
ID No: RYG_FS0220

Customer

Name: ALS laboratory group (thailand) Co.,Ltd.
Address: 104 Phatthanakan 40, Phatthanakan
Rd.,Khwaeng Suan Luang, Khet Suan Luang,Bangkok
10250 Thailand.

Received date: 22 DEC 2021
Calibration date: 28 DEC 2021
Issue date: 29 DEC 2021

Reference Used During Calibration

1.Standard Temperature Probe Model: STS-100 A500,
Serial No.: 667682-09, Due date: 25 Mar 2022
2.Digital Temperature Indicator Model: DTI-1000-A MK
II, Serial No.: 671407-00591 Due date: 04 June 2022

Calibration Condition

Temperature: (23±3)°C
Relative Humidity: (55±15)%

Calibration Procedure

The temperature calibration was done by In-House
calibration method as WI-CL-001 according to
comparison method with standard digital temperature
indicator and standard temperature probe. The
temperature scale use was based on ITS-90.


Traceability

The measurement results are traceable to the
international system of units (SI) through National
Institute of Metrology Thailand (NIMT) Certificate
number: TT-0036-21, Certificate number: ER-0032-
21

REVIEW BY *Warakorn P.*
APPROVED BY *Wichit Chm.*
NEXT CAL. DATE *28/12/22*

Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya

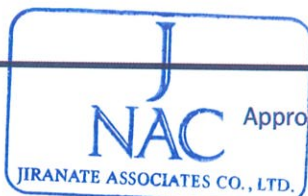

Approved Signatory: *2Jemp*

Mr. Parinya Booncharoen
Technical Support
and Calibration Manager

Result of Calibration:- ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 – 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 15006715.
Dimension: Diameter 14 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
30	20.056	20.0	-0.1	0.099
30	25.049	25.0	0.0	0.099
30	30.038	30.0	0.0	0.099
30	35.031	35.0	0.0	0.099
30	40.022	39.9	-0.1	0.099

Table 2: This equipment was connected with temperature probe Model: TP3207.2 S/N: 15015507.
Dimension: Diameter 14 mm. Length 150 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.058	20.2	0.1	0.099
70	24.879	25.0	0.1	0.099
70	29.832	29.8	0.0	0.099
70	34.801	34.7	-0.1	0.099
70	39.767	39.6	-0.2	0.099

Table 3: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: -.
Dimension: Diameter 8 mm. Length 170 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
110	20.056	20.1	0.0	0.099
110	25.050	25.1	0.1	0.099
110	30.038	30.1	0.1	0.099
110	35.032	35.1	0.1	0.099
110	40.024	40.1	0.1	0.099

UUC* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

* End of Certificate *





ROTA METER CALIBRATION RESULT JULY 2022

Rotameter ID.	Calibration Date	Regression Result	Coefficient (R ²)
BKK_FS0577	01 Jul 22	$Y = 1.0202x + 0.1976$	1.0000
BKK_FS0579	01 Jul 22	$Y = 1.0078x + 0.4789$	0.9998
BKK_FS0583	01 Jul 22	$Y = 1.016x + 0.3922$	1.0000
BKK_FS0584	01 Jul 22	$Y = 1.0036x + 2.2262$	0.9997
BKK_FS0585	01 Jul 22	$Y = 1.0189x - 5.6476$	0.9997
BKK_FS0586	01 Jul 22	$Y = 1.0095x - 1.1524$	0.9995
BKK_FS0587	01 Jul 22	$Y = 1.013x - 3.6619$	0.9996
BKK_FS0588	01 Jul 22	$Y = 1.0154x + 4.8357$	0.9999
BKK_FS0589	01 Jul 22	$Y = 0.9918x + 4.8069$	0.9999
BKK_FS0590	01 Jul 22	$Y = 1.0038x - 0.4857$	0.9996
BKK_FS0591	01 Jul 22	$Y = 0.9705x - 52.174$	0.9986
BKK_FS0592	01 Jul 22	$Y = 0.9646x - 37.642$	0.9985
BKK_FS0593	01 Jul 22	$Y = 0.9767x - 58.445$	0.9988
BKK_FS0594	01 Jul 22	$Y = 0.9902x - 62.87$	0.9999
BKK_FS0595	01 Jul 22	$Y = 1.0249x - 98.162$	0.9999
BKK_FS0596	01 Jul 22	$Y = 0.9843x - 26.806$	0.9991
BKK_FS0597	01 Jul 22	$Y = 0.9802x - 61.653$	0.9978
BKK_FS1004	01 Jul 22	$Y = 0.9696x + 17.69$	0.9990
BKK_FS1005	01 Jul 22	$Y = 1.0092x + 2.4571$	0.9999
BKK_FS1006	01 Jul 22	$Y = 1.168x - 5.566$	0.9997
BKK_FS1007	01 Jul 22	$Y = 0.9917x + 1.6592$	1.0000
BKK_FS1008	01 Jul 22	$Y = 1.0132x + 0.7207$	1.0000
BKK_FS1009	01 Jul 22	$Y = 1.0132x + 1.1633$	0.9960
BKK_FS1010	01 Jul 22	$Y = 1.0033x + 0.5758$	0.9999
BKK_FS1011	01 Jul 22	$Y = 1.0234x + 0.1759$	0.9996
BKK_FS1012	01 Jul 22	$Y = 1.0106x - 2.0048$	0.9997
BKK_FS1013	01 Jul 22	$Y = 0.9677x - 35.851$	0.9997
BKK_FS1014	01 Jul 22	$Y = 1.0021x + 0.3148$	0.9998
BKK_FS1015	01 Jul 22	$Y = 0.9994x + 1.786$	1.0000
BKK_FS1016	01 Jul 22	$Y = 1.0105x - 80.256$	0.9998
BKK_FS1017	01 Jul 22	$Y = 0.9995x + 0.649$	1.0000
BKK_FS1018	01 Jul 22	$Y = 1.0011x + 1.1786$	1.0000
BKK_FS1019	01 Jul 22	$Y = 1.0023x - 68.424$	0.9996
BKK_FS1020	01 Jul 22	$Y = 1.0547x - 0.666$	0.9998
BKK_FS1021	01 Jul 22	$Y = 1.018x - 3.3286$	0.9998
BKK_FS1022	01 Jul 22	$Y = 0.9932x - 57.035$	0.9986
BKK_FS1023	01 Jul 22	$Y = 1.0094x + 0.0717$	0.9999
BKK_FS1024	01 Jul 22	$Y = 1.0042x + 0.4086$	0.9997
BKK_FS1025	01 Jul 22	$Y = 1.0132x - 88.507$	0.9996



ROTA METER CALIBRATION RESULT JULY 2022

Rotameter ID.	Calibration Date	Regression Result	Coefficient (R ²)
BKK_FS1026	01 Jul 22	$Y = 1.0018x + 1.0776$	0.9997
BKK_FS1027	01 Jul 22	$Y = 1.0053x + 0.231$	0.9995
BKK_FS1028	01 Jul 22	$Y = 0.9792x - 60.312$	0.9982
BKK_FS1029	01 Jul 22	$Y = 0.9935x + 0.8234$	1.0000
BKK_FS1030	01 Jul 22	$Y = 1.0039x + 0.515$	0.9999
BKK_FS1031	01 Jul 22	$Y = 1.009x - 79.295$	0.9998
BKK_FS1039	01 Jul 22	$Y = 0.9879x + 7.3524$	0.9996
BKK_FS1040	01 Jul 22	$Y = 0.9704x + 88.336$	0.9987
BKK_FS1041	01 Jul 22	$Y = 1.0645x - 1.7878$	0.9999
BKK_FS1042	01 Jul 22	$Y = 0.9983x + 3.6262$	0.9998
BKK_FS1043	01 Jul 22	$Y = 1.0069x - 6.9619$	1.0000
BKK_FS1044	01 Jul 22	$Y = 1.0355x - 0.6214$	0.9997
BKK_FS1161	01 Jul 22	$Y = 1.0126x + 0.7738$	0.9999
BKK_FS1162	01 Jul 22	$Y = 0.9994x + 2.6357$	0.9995
BKK_FS1163	01 Jul 22	$Y = 0.977x - 55.03$	0.9987
BKK_FS1164	01 Jul 22	$Y = 0.9914x + 0.8427$	0.9997
BKK_FS1165	01 Jul 22	$Y = 0.9893x + 6.5919$	0.9998
BKK_FS1166	01 Jul 22	$Y = 1.0031x - 77.881$	0.9996
BKK_FS1200	01 Jul 22	$Y = 1.0313x - 0.4602$	0.9995
BKK_FS1201	01 Jul 22	$Y = 1.0045x + 0.15$	0.9996
BKK_FS1202	01 Jul 22	$Y = 0.9702x - 44.156$	0.9994
RYG_FS0197	01 Jul 22	$Y = 1.0039x - 0.179$	0.9999
RYG_FS0198	01 Jul 22	$Y = 0.9971x + 16.648$	0.9999
RYG_FS0199	01 Jul 22	$Y = 1.0832x - 2.6367$	1.0000

Review By :

(Mr. Wichan Choonharat)

Enviro Field Services Manager

Approved By :

(Mr. Sarayuth Jittranont)

Assistant General Manager



ROTA METER CALIBRATION RESULT OCTOBER 2022

Rotameter ID.	Calibration Date	Regression Result	Coefficient (R ²)
BKK_FS0577	01 Oct 22	$Y = 1.0202x + 0.1976$	1.0000
BKK_FS0579	01 Oct 22	$Y = 1.0078x + 0.4789$	0.9998
BKK_FS0583	01 Oct 22	$Y = 1.016x + 0.3922$	1.0000
BKK_FS0584	01 Oct 22	$Y = 1.0036x + 2.2262$	0.9997
BKK_FS0585	01 Oct 22	$Y = 1.0189x - 5.6476$	0.9997
BKK_FS0586	01 Oct 22	$Y = 1.0095x - 1.1524$	0.9995
BKK_FS0587	01 Oct 22	$Y = 1.013x - 3.6619$	0.9996
BKK_FS0588	01 Oct 22	$Y = 1.0154x + 4.8357$	0.9999
BKK_FS0589	01 Oct 22	$Y = 0.9918x + 4.8069$	0.9999
BKK_FS0590	01 Oct 22	$Y = 1.0038x - 0.4857$	0.9996
BKK_FS0591	01 Oct 22	$Y = 0.9705x - 52.174$	0.9986
BKK_FS0592	01 Oct 22	$Y = 0.9646x - 37.642$	0.9985
BKK_FS0593	01 Oct 22	$Y = 0.9767x - 58.445$	0.9988
BKK_FS0594	01 Oct 22	$Y = 0.9902x - 62.87$	0.9999
BKK_FS0595	01 Oct 22	$Y = 1.0249x - 98.162$	0.9999
BKK_FS0596	01 Oct 22	$Y = 0.9843x - 26.806$	0.9991
BKK_FS0597	01 Oct 22	$Y = 0.9802x - 61.653$	0.9978
BKK_FS1004	01 Oct 22	$Y = 0.9762x + 11.724$	0.9998
BKK_FS1005	01 Oct 22	$Y = 1.0081x + 1.5143$	1.0000
BKK_FS1006	01 Oct 22	$Y = 1.098x - 2.9327$	0.9999
BKK_FS1007	01 Oct 22	$Y = 0.9917x + 1.6592$	1.0000
BKK_FS1008	01 Oct 22	$Y = 1.0132x + 0.7207$	1.0000
BKK_FS1009	01 Oct 22	$Y = 1.0132x + 1.1633$	0.9960
BKK_FS1010	01 Oct 22	$Y = 1.0033x + 0.5758$	0.9999
BKK_FS1011	01 Oct 22	$Y = 1.0234x + 0.1759$	0.9996
BKK_FS1012	01 Oct 22	$Y = 1.0106x - 2.0048$	0.9997
BKK_FS1013	01 Oct 22	$Y = 0.9677x - 35.851$	0.9997
BKK_FS1014	01 Oct 22	$Y = 1.0021x + 0.3148$	0.9998
BKK_FS1015	01 Oct 22	$Y = 0.9994x + 1.786$	1.0000
BKK_FS1016	01 Oct 22	$Y = 1.0105x - 80.256$	0.9998
BKK_FS1017	01 Oct 22	$Y = 0.9995x + 0.649$	1.0000
BKK_FS1018	01 Oct 22	$Y = 1.0011x + 1.1786$	1.0000
BKK_FS1019	01 Oct 22	$Y = 1.0023x - 68.424$	0.9996
BKK_FS1020	01 Oct 22	$Y = 1.0547x - 0.666$	0.9998
BKK_FS1021	01 Oct 22	$Y = 1.018x - 3.3286$	0.9998
BKK_FS1022	01 Oct 22	$Y = 0.9932x - 57.035$	0.9986
BKK_FS1023	01 Oct 22	$Y = 1.0094x + 0.0717$	0.9999
BKK_FS1024	01 Oct 22	$Y = 1.0042x + 0.4086$	0.9997
BKK_FS1025	01 Oct 22	$Y = 1.0132x - 88.507$	0.9996



ROTA METER CALIBRATION RESULT OCTOBER 2022

Rotameter ID.	Calibration Date	Regression Result	Coefficient (R ²)
BKK_FS1026	01 Oct 22	$Y = 1.0018x + 1.0776$	0.9997
BKK_FS1027	01 Oct 22	$Y = 1.0053x + 0.231$	0.9995
BKK_FS1028	01 Oct 22	$Y = 0.9792x - 60.312$	0.9982
BKK_FS1029	01 Oct 22	$Y = 0.9935x + 0.8234$	1.0000
BKK_FS1030	01 Oct 22	$Y = 1.0039x + 0.515$	0.9999
BKK_FS1031	01 Oct 22	$Y = 1.009x - 79.295$	0.9998
BKK_FS1039	01 Oct 22	$Y = 0.9967x + 4.5048$	0.9999
BKK_FS1040	01 Oct 22	$Y = 0.9936x + 32.694$	0.9998
BKK_FS1041	01 Oct 22	$Y = 1.067x - 1.999$	1.0000
BKK_FS1042	01 Oct 22	$Y = 1.0019x + 2.1571$	1.0000
BKK_FS1043	01 Oct 22	$Y = 1.1569x - 96.479$	0.8412
BKK_FS1044	01 Oct 22	$Y = 1.0318x - 0.9374$	0.9999
BKK_FS1161	01 Oct 22	$Y = 1.0126x + 0.7738$	0.9999
BKK_FS1162	01 Oct 22	$Y = 0.9994x + 2.6357$	0.9995
BKK_FS1163	01 Oct 22	$Y = 0.977x - 55.03$	0.9987
BKK_FS1164	01 Oct 22	$Y = 0.9914x + 0.8427$	0.9997
BKK_FS1165	01 Oct 22	$Y = 0.9893x + 6.5919$	0.9998
BKK_FS1166	01 Oct 22	$Y = 1.0031x - 77.881$	0.9996
BKK_FS1200	01 Oct 22	$Y = 1.0313x - 0.4602$	0.9995
BKK_FS1201	01 Oct 22	$Y = 1.0045x + 0.15$	0.9996
BKK_FS1202	01 Oct 22	$Y = 0.9702x - 44.156$	0.9994
RYG_FS0197	01 Oct 22	$Y = 1.0039x - 0.179$	0.9999
RYG_FS0198	01 Oct 22	$Y = 0.9964x + 21.757$	1.0000
RYG_FS0199	01 Oct 22	$Y = 1.0577x - 1.7486$	1.0000

Review By :

(Mr. Wichan Choonharat)

Enviro Field Services Manager

Approved By :

(Mr. Sarayuth Jittranont)

Assistant General Manager

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL22060

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00734225 / 169439 / 72460
ID No.: RYG_FS0030

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -

Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 14 JANUARY 2022
Calibration Date : 21-24 JANUARY 2022
Date of Issue : 25 JANUARY 2022

REVIEW BY	<i>Marakon P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	21/1/23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22060
Job No. : VC65AC0043
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22060
Job No. : VC65AC0043
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.4	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22060

Job No. : VC65AC0043

Pages : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.96)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	10.8
C - weight	17.2
Flat	23.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.5	0.5	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-1.6	-1.5	-1.5	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22060

Job No. : VC65AC0043

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22060

Job No. : VC65AC0043

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	132.9	-0.1	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	130.9	-0.1	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22060

Job No. : VC65AC0043

Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.8	-0.6	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22060
Job No. : VC65AC0043
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL22154

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00734218 / 146937 / 34368
ID No.: RYG_FS0031

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 17 JUNE 2022
Calibration Date : 20-22 JUNE 2022
Date of Issue : 27 JUNE 2022

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	20/6/23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22154
Job No. : VC65AC0068
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22154
Job No. : VC65AC0068
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22154

Job No. : VC65AC0068

Pages : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
20.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.6
C - weight	17.4
Flat	23.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.5	0.5	0.5	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	-1.5	-1.5	-1.4	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22154

Job No. : VC65AC0068

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22154

Job No. : VC65AC0068

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	132.9	-0.1	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	130.9	-0.1	± 1.1
129.0	128.9	-0.1	± 1.1
124.0	123.9	-0.1	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22154
Job No. : VC65AC0068
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.7	-0.7	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22154

Job No. : VC65AC0068

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

————— **End of Calibration Certificate** —————

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL22029

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00900074 / 188467 / 01736
ID No.: RYG_FS0495

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 05 JANUARY 2022
Calibration Date : 10-12 JANUARY 2022
Date of Issue : 13 JANUARY 2022

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	10/1/23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22029

Job No. : VC65AC0040

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22029

Job No. : VC65AC0040

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1