

ประจำเดือนธันวาคม พ.ศ. 2565



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160  
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160  
Tel : 02-802-3577-8 Fax: 02-802-3773 E-mail : info@evltesting.com



Envilab & Need2Supply Distributor

## TSP High Volume Sampler Calibration

Verification Report No.

A6511 -TSP 02

☒ PM ☐ Onsite

Site: บริษัท เอ็นไวแล็บ จำกัด

UTM : 47P N1514475 E654269

Sampler: ETSP#01

Recorder: ECRANG15315224

Date: 2 Dec 22

Technical: Sanayu J.

Approval: Sarawut K.

### CONDITIONS

Barometric Press. (hPa): 1000.8

Temperature (deg C): 32.0

Average Press. (hPa): 1013.0

Average Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 750.7

Temperature (deg K): 305.0

Corrected Avg. Press. (mm Hg): 759.8

Average Temp. (deg K): 303.0

### CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc

Model: TE-5028A

Serial#: 1328


Qstd Slope: 1.63957

Qstd Intercept: -0.01202

Date Certified: 19 Jan 22

### CALIBRATIONS

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	12.44	2.121	52.0	51.08	Slope = 11.2096
2	9.73	1.876	48.0	47.15	Intercept = 26.7694
3	6.16	1.494	44.0	43.22	Corr. coeff. = 0.9957
4	4.34	1.256	42.0	41.26	# of Observations: 5
5	2.44	0.943	38.0	37.33	Range of Chart 40
					at 1.1 - 1.7 m3/min. 46

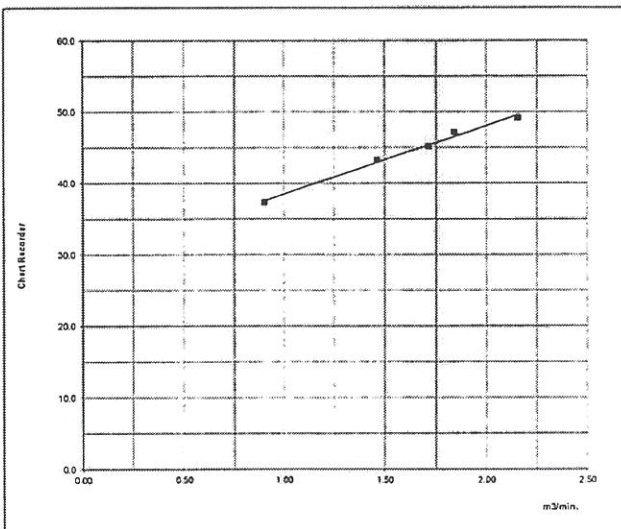

Calibrated by :

นาย จันทน

( Sanayu Jantason )

2 December 2022

Approved by :

( Sarawut Keawsrinual )

2 December 2022



รับรองสำเนาถูกต้อง

ผู้จัดการฝ่ายควบคุมคุณภาพ

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

FE-MNT-29 Rev.00:01/08/63



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160  
 Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkhae Bangkok 10160  
 Tel : 02-802-3577-8 Fax: 02-802-3773 E-mail : info@evltesting.com



Envilab is a member of the supply network

## PM10 High Volume Sampler Calibration

Verification Report No.

A6511 -PM 01

☒ PM ☐ Onsite

Site: บริษัท เอ็นไวแล็บ จำกัด

UTM : 47P N1514475 E654269

Sampler: EPM#12

Recorder: ECRDS01618124

Date: 2 Dec 22

Technical: Sanayu J.

Approval: Sarawut K.

### CONDITIONS

Barometric Press. (hPa): 1000.8

Temperature (deg C): 32.0

Average Press. (hPa): 1013.0

Average Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 750.7

Temperature (deg K): 305.0

Corrected Avg.Press. (mm Hg): 759.8

Average Temp. (deg K): 303.0

### CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc

Model: TE-5028A

Serial#: 1328

Slope: 1.02667

Intercept: -0.00753

Date Certified: 19 Jan 22

### CALIBRATIONS

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	12.66	2.216	50.0	31.87
2	9.28	1.899	44.0	28.05
3	7.67	1.727	42.0	26.77
4	4.21	1.281	36.0	22.95
5	2.13	0.913	30.0	19.12

### LINEAR REGRESSION

Slope = 9.4825

Intercept = 10.5104

Corr. coeff. = 0.9977

SFR = 1.151

SSP = 33.62


# of Observations: 5

Range of Chart

33

at SFR  $\pm 10\%$

35

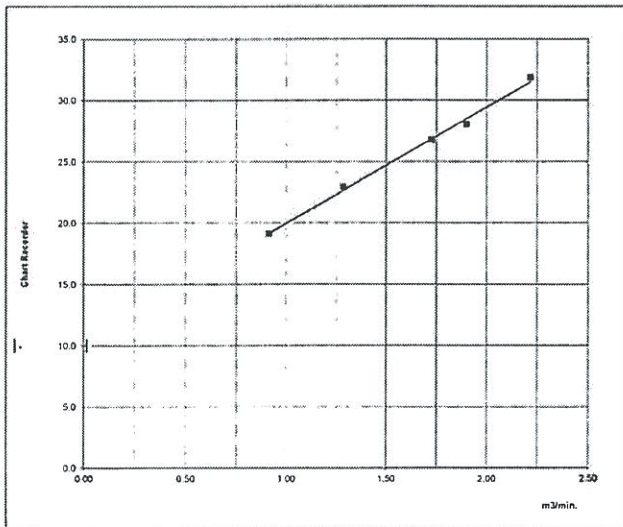

Calibrated by :

Sanayu Jantason  
 (Sanayu Jantason)  
 2 December 2022

Approved by :

Sarawut Keawsrinual  
 (Sarawut Keawsrinual)  
 2 December 2022



รับรองสำเนาถูกต้อง  
 ผู้จัดการฝ่ายควบคุมคุณภาพ

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

FE-MNT-29 Rev.00 01/08/63



**neediss**บริษัท นีดิส ซัพพลาย อินสตรูเมนต์ จำกัด  
Neediss Supply Instrument Co., Ltd.535 ซอยบางนา 7 แขวงบางนา เขตบางนา กรุงเทพมหานคร 10160 535 Soi Bangkhae 7 Bangkhae, Bangkok Bangkok  
Tel 02-802-3980-2 Fax 02-802-3988 Email: neediss.com

## SO<sub>2</sub> Analyzer Verification Test Report

Calibration Report No.: 6512007

Page:1/1

Calibrated Date: 1-Dec-22

☒ PM ☐ Onsite

### Instruments Information

Analyzer Type: SO2 Analyzer Model: THERMO.,43C	Manufacturer THERMO S/N: ESOTE43C053884
---	--


### Calibration System

Calibrator Unit	Standard Gas
Dilutor Model ESA MGC101 S/N: 792 ZERO AIR Generator ZAG7001 S/N: 644	NO Conc 44.68 PPM SO2 Conc 45.34 PPM CO Conc 4500 PPM Expire Date: Feb 19,2024 EB0140762

Environment: Temperature 25.3 °CHumidity: 53 %RH

### Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	1.4	0.0	400.0	408	2.0
After	0.0	0.5	0.5	400.0	401	0.3

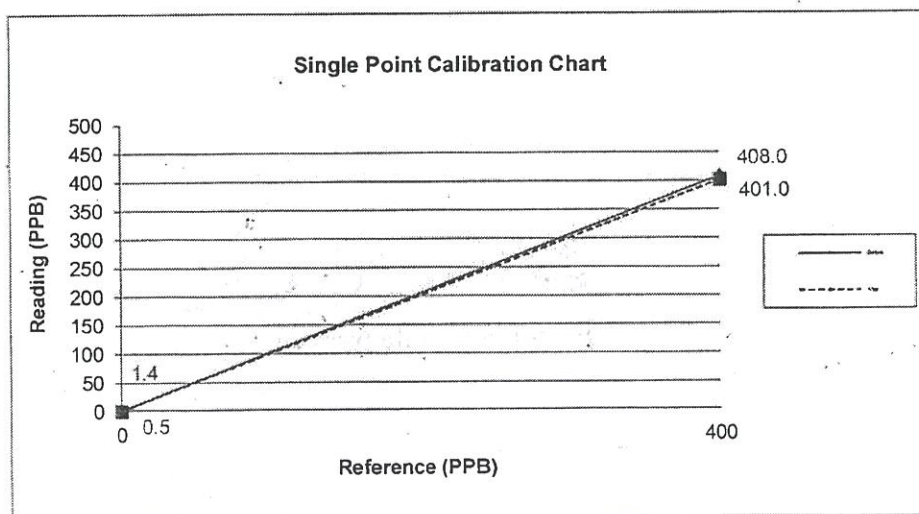รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

**www.neediss.com**

We know the best thing to solve for you.

02-802-3980-2



**neediss**บริษัท เน็ดิส ซัพพลาย อินสตรูเมนต์ จำกัด  
Neediss Supply Instrument Co., Ltd.536 ซอยบางนา 7 แขวงบางนา เขตบางนา กรุงเทพฯ 10180 536 Soi Bangkhae 7 Bangkhae Bangkok  
Tel. 02-802-3780-2 Fax. 02-802-3788 E: info@neediss.com

MODEL : SO2 ANALYZER Model 43C THERMO

DATE : 1-12-2022

S/N : ESOTE43C053884

Test Function Value	Before	After
Range 500 (PPB)	500	500
PMT VOLTS -450 - -850 ( V )	-650	-653
LAMP VOLTAGE 950 - 1,200 ( V )	990	985
LAMP INTENSITY 20000 - 50000 Hz	32568	32577
INTER TEMP 15 - 45 DEG C	37	37
CHAMBER TEMP 47 - 51 C	49	49
COOLER TEMP -5 - (-2) DEG C	-2.5	-2.5
PRESSURE 400 - 1000.0 mm Hg	764	765
FLOW 0.350 - 0.650 LPM	0.42	0.4

**neediss**

Neediss Supply Instrument Co., Ltd.

Calibrate By :

*Sirirat Poonlak*

Approve By :

*K*

Sirirat Poonlak

Sarawut Keawsrinual

Date:

1-Dec-22

Date:

1-Dec-22



Envilab Co., Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

**www.neediss.com**

We know the best thing to save environment

**neediss**

บริษัท นีดีส ซัพพลาย อินสตรูเมนต์ จำกัด  
Neediss Supply Instrument Co., Ltd.  
535 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10150 535 Soi Bangkhae 7 Bangkhae Bangkok Bangkok  
Tel. 02-802-3980-2 Fax. 02-802-3988 E.info@neediss.com



## NOx Analyzer Verification Test Report

Calibration Report No.: 6512008  
Calibrated Date: 1-Dec-22

Page:1/2

☒ PM ☐ Onsite

### Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 42C	Manufacturer THERMO S/N: ENOTE42CD74371
--	--

### Calibration System

Calibrator Unit	Standard Gas
Dilutor Model ESA MGC101 S/N: 792 ZERO AIR Generator ZAG7001 S/N: 644	NO Conc 44.68 PPM SO2 Conc 45.34 PPM CO Conc 4500 PPM Expire Date: Feb 19,2024 EB0140762

Environment: Temperature 24.9 °C


Humidity: 59 %RH

### Calibration Check ( Before adjust )

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	8.1	0.0	8.1	384	400.0	-2.0
NO <sub>2</sub>	1.2	0.0	1.2	24.0	0.0	3.0
NOx	9.3	0.0	9.3	408	400.0	1.0

### Calibration Check ( After adjust )

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.7	0.0	0.7	403	400.0	0.4
NO <sub>2</sub>	0.4	0.0	0.4	2.0	0.0	0.2
NOx	1.1	0.0	1.1	405	400.0	0.6

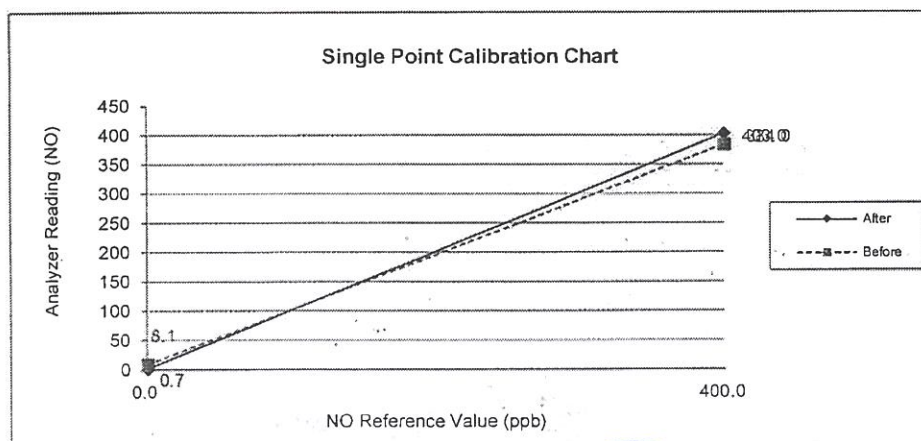

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

**www.neediss.com**

We know the best thing to sup environment



**neediss**บริษัท นีดีส ซัพพลาย อินสตรูमेंท์ จำกัด  
Neediss Supply Instrument Co., Ltd.535 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160 535 Soi Bangkhoe 7 Bangkhoe Bangkok  
Tel. 02-802-3980-2 Fax. 02-802-3988 E:info@neediss.com

MODEL : NOx ANALYZER Model 42C THERMO

DATE : 1-11-2022

S/N : ENOTE42CD74371

Page:2/2

Test Function Value	Before	After
Range 500 (PPB)	500	500
PMT VOLTS -450 - -850 (V)	-675	-678
LAMP VOLTAGE 950 - 1,200 (V)		
INTER TEMP 15 - 45 DEG C	43	43
CHAMBER TEMP 47 - 51 C	49	50
COOLER TEMP -5 - (-2) DEG C	-2	-2
PRESSURE 400 - 1000.0 mm Hg	350	380
SAMPLE FLOW 0.350 - 0.900 LPM	0.45	0.46
OZONEATOR FLOW 0.035 - 0.075 LPM	0.05	0.05
No/Nox BKG	12/9.0	12/9.1
No/Nox Slope	1.0/0.8	0.9/0.8

Calibrate By : Sirint PoonlakApprove By : SK

Sirint Poonlak

Sarawut Keawsrinual

Date:

1-Dec-22

Date:

1-Dec-22

**neediss**

Neediss Supply Instrument Co.,Ltd.



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

**www.neediss.com**

We know the best thing to save environment.





บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160  
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160  
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab & Envilab Supply Instrument

## Verification Test Report

Report No.:

6512 -SLM 01

☒ PM ☐ Onsite UTM : 47P N 1514462 E 654258

Calibrated Date: 1 December 2022

Site : บริษัทเอ็นไวแล็บ จำกัด

Equipment: Sound Level Meter

Manufacturer: NEEDISS

Model: NDSM 309

Serial : 565010

Environment: Temperature 25 °C Humidity 58 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer

Serial No.1351075

Date of Calibration : March.21, 2022

### Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.66	93.32	-0.34	93.66

Calibrated By:

( Sanayu Jantason )

Date:

1 December 2022

Approve By:

( Wisan Ritthikamon )

Date:

1 December 2022



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160  
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160  
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab 3 Needles Supply Instrument

## TSP High Volume Sampler Calibration

Verification Report No.

A6511 -TSP 01

☒ PM ☐ Onsite

Site: บริษัท เอ็นไวแล็บ จำกัด

UTM : 47P N1514475 E654269

Sampler: NTSP#15

Recorder: ECRANG15315224

Date: 2 Dec 22

Technical: Sanayu J.

Approval: Sarawut K.

### CONDITIONS

Barometric Press. (hPa): 1000.8

Temperature (deg C): 32.0

Average Press. (hPa): 1013.0

Average Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 750.7

Temperature (deg K): 305.0

Corrected Avg.Press. (mm Hg): 759.8

Average Temp. (deg K): 303.0

### CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc

Model: TE-5028A

Serial#: 1328


Qstd Slope: 1.63957

Qstd Intercept: -0.01202

Date Certified: 19 Jan 22

### CALIBRATIONS

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	12.87	2.157	50.0	49.12	Slope = 9.5726
2	9.32	1.836	48.0	47.15	Intercept = 28.9498
3	8.12	1.715	46.0	45.19	Corr. coeff. = 0.9951
4	5.89	1.461	44.0	43.22	# of Observations: 5
5	2.23	0.902	38.0	37.33	Range of Chart 41
					at 1.1 - 1.7 m3/min. 46

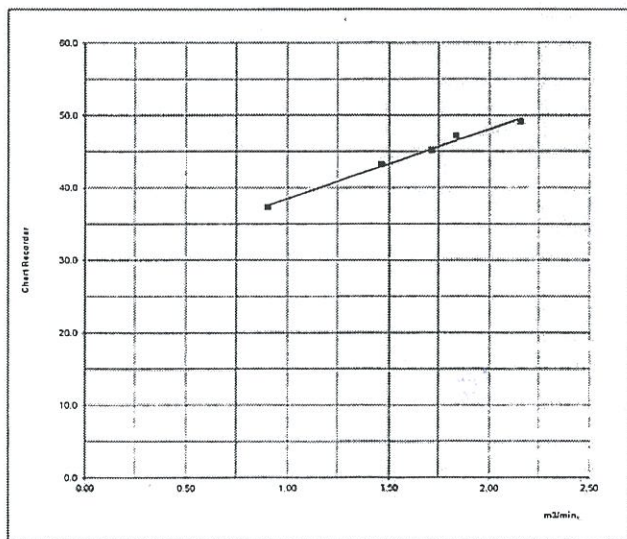

Calibrated by :

Sanayu Jantason

( Sanayu Jantason )

2 December 2022

Approved by :

Sarawut Keawsrinual

( Sarawut Keawsrinual )

2 December 2022



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

FE-MNT-29 Rev.00/03/63





บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพมหานคร 10160  
 Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160  
 Tel : 02-802-3577-S Fax, 02-802-3773 E-mail : info@evltesting.com



Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160

## PM10 High Volume Sampler Calibration

Verification Report No.

A6511 -PM 02

☒ PM

☐ Onsite

Site: บริษัท เอ็นไวแล็บ จำกัด

UTM : 47P N1514475 E654269

Sampler: EPM#01

Recorder: ECRDS01618124

Date: 2 Dec 22

Technical: Sanayu J.

Approval: Sarawut K.

### CONDITIONS

Barometric Press. (hPa): 1000.8

Temperature (deg C): 32.0

Average Press. (hPa): 1013.0

Average Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 750.7

Temperature (deg K): 305.0

Corrected Avg. Press. (mm Hg): 759.8

Average Temp. (deg K): 303.0

### CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc

Model: TE-5028A

Serial#: 1328

Slope: 1.02667

Intercept: -0.00753

Date Certified: 19 Jan 22

### CALIBRATIONS

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	12.56	2.208	52.0	33.15
2	10.97	2.064	48.0	30.60
3	8.95	1.865	46.0	29.32
4	5.74	1.495	40.0	25.50
5	4.91	1.383	38.0	24.22

### LINEAR REGRESSION

Slope = 10.2580

Intercept = 10.0633


Corr. coeff. = 0.9942

SFR = 1.151

SSP = 34.32

# of Observations: 5

Range of Chart 33  
at SFR  $\pm 10\%$  35

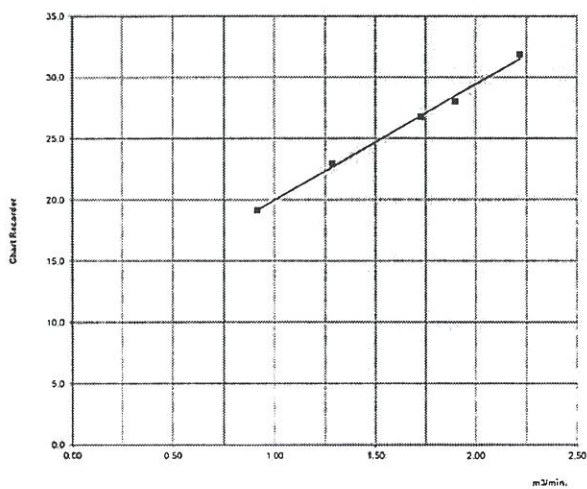

Calibrated by :

( Sanayu Jantason )  
2 December 2022

Approved by :

( Sarawut Keawsrinual )  
2 December 2022



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

[www.evltesting.com](http://www.evltesting.com)

Environmental responsibility with accuracy measurement

PM10 Cal. Rev.07 / Iss Date Mar 31, 2020

FE-MNT-29 Rev.00:01/08/03





**neediss**

บริษัท นีดีส ซัพพลาย อินสตรูमेंท์ จำกัด  
Neediss Supply Instrument Co., Ltd.  
535 ซอยลาดพร้าว 7 แขวงลาดพร้าว เขตคลองจั่น กรุงเทพมหานคร 10160 536 Soi Bangkhoe 7 Bangkhoe Bangkok Bangkok  
Tel. 02-602-3980-2 Fax. 02-602-3983 E-mail: info@neediss.com



## SO<sub>2</sub> Analyzer Verification Test Report

Calibration Report No.: 6512004

Page:1/1

Calibrated Date: 1-Dec-22

☒ PM ☐ Onsite

### Instruments Information

Analyzer Type: SO2 Analyzer Model: THERMO.,43C	Manufacturer THERMO S/N: ESOTE43C373373
---	--

### Calibration System



Calibrator Unit	Standard Gas
Dilutor Model ESA MGC101 S/N: 792 ZERO AIR Generator ZAG7001 S/N: 644	NO Conc 44.68 PPM SO2 Conc 45.34 PPM CO Conc 4500 PPM Expire Date: Feb 19,2024 EB0140762

Environment: Temperature 25.3 °C

Humidity: 53 %RH

### Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	2.9	2.9	400.0	394	-1.5
After	0.0	0.3	0.3	400.0	401	0.3

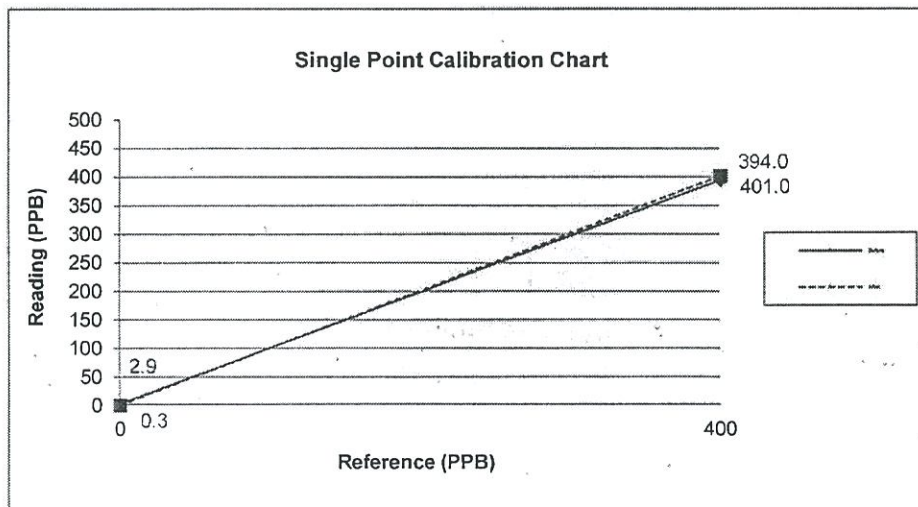

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.



[www.neediss.com](http://www.neediss.com)

We know the best thing to save environment

02-602-3980

**neediss**บริษัท นีดีส ซัพพลาย อินสตรูเมนต์ จำกัด  
Neediss Supply Instrument Co., Ltd.536 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160 536 Soi Bangkhae 7 Bangkhae Bangkok Bangkok  
Tel. 02-802-3980-2 Fax. 02-802-3988 E:info@neediss.com

MODEL : SO2 ANALYZER Model 43C THERMO

DATE : 1-12-2022

S/N : ESOTE43C373373

Test Function Value	Before	After
Range 500 (PPB)	500	500
PMT VOLTS -450 - -850 ( V )	-650	-653
LAMP VOLTAGE 950 - 1,200 ( V )	990	985
LAMP INTENSITY 20000 - 50000 Hz	32568	32577
INTER TEMP 15 - 45 DEG C	37	37
CHAMBER TEMP 47 - 51 C	49	49
COOLER TEMP -5 - (-2) DEG C	-2.5	-2.5
PRESSURE 400 - 1000.0 mm Hg	764	765
FLOW 0.350 - 0.650 LPM	0.42	0.4

**neediss**

Neediss Supply Instrument Co., Ltd.

Calibrate By :

*Sirirat Poonlak*

Approve By :

*Sarawat Keawsrinal*

Sirirat Poonlak

Sarawat Keawsrinal

Date:

1-Dec-22



Date:

*Ok Sir* 1-Dec-22รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

**www.neediss.com**

We know the best thing to save environment





neediss

บริษัท นีดีส ซัพพลาย อินสตรูमेंท์ จำกัด  
Neediss Supply Instrument Co., Ltd.

536 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพมหานคร 10150 536 Soi Bangkadee 7 Bangkok Bangkadee Bangkok  
Tel. 02-802-3980-2 Fax. 02-802-3988 E.info@neediss.com



## NOx Analyzer Verification Test Report

Calibration Report No.: 6512005

Page:1/2

Calibrated Date: 1-Dec-22

☒ PM ☐ Onsite

### Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 42C	Manufacturer THERMO S/N: ENOTE42C789390
--	--

### Calibration System

Calibrator Unit	Standard Gas
Dilutor Model ESA MGC101 S/N: 792 ZERO AIR Generator ZAG7001 S/N: 644	NO Conc 44.68 PPM SO2 Conc 45.34 PPM CO Conc 4500 PPM Expire Date: Feb 19,2024 EB0140762

Environment: Temperature 25.0 °C


Humidity: 53 %RH

### Calibration Check ( Before adjust )

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	3.7	0.0	3.7	393	400.0	-0.9
NO <sub>2</sub>	1.8	0.0	1.8	19.0	0.0	2.4
NOx	5.5	0.0	5.5	412	400.0	1.5

### Calibration Check ( After adjust )

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.4	0.0	0.4	402	400.0	0.2
NO <sub>2</sub>	0.5	0.0	0.5	4.0	0.0	0.5
NOx	0.9	0.0	0.9	406	400.0	0.7

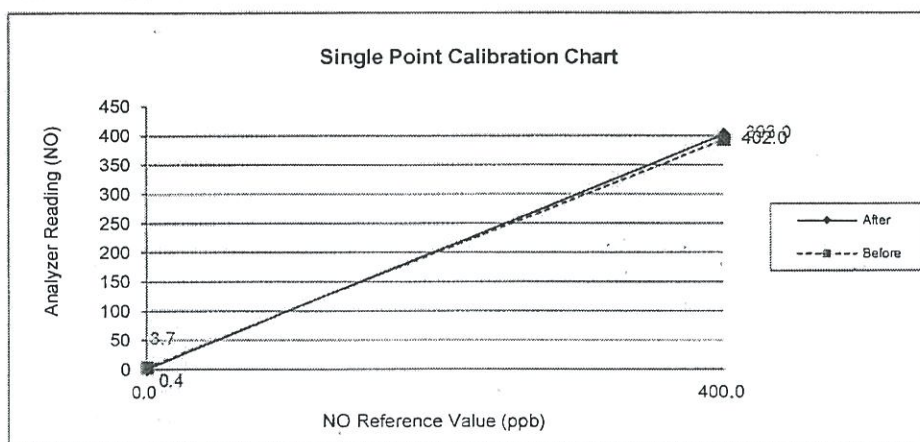

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

[www.neediss.com](http://www.neediss.com)

We know the best thing to save environment



**neediss**บริษัท นีดีส ซัพพลาย อินสตรูमेंท์ จำกัด  
Neediss Supply Instrument Co., Ltd.536 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160 536 Soi Bangkhoe 7 Bangkhoe Bangkok  
Tel. 02-802-3980-2 Fax. 02-802-3988 E: info@neediss.com

MODEL : NOx ANALYZER Model 42C THERMO

DATE : 1-12-2022

S/N : ENOTE42C789390

Page:2/2

Test Function Value	Before	After
Range 500 (PPB)	500	500
PMT VOLTS -450 - -850 ( V )	-675	-678
LAMP VOLTAGE 950 - 1,200 ( V )		
INTER TEMP 15 - 45 DEG C	43	43
CHAMBER TEMP 47 - 51 C	49	50
COOLER TEMP -5 - (-2) DEG C	-2	-2
PRESSURE 400 - 1000.0 mm Hg	350	380
SAMPLE FLOW 0.350 - 0.900 LPM	0.45	0.46
OZONEATOR FLOW 0.035 - 0.075 LPM	0.05	0.05
No/Nox BKG	12/9.0	12/9.1
No/Nox Slope	1.0/0.8	0.9/0.8

Calibrate By : Sirirat PoonlakApprove By : Sarawat Keawsrinual

Sirirat Poonlak

Sarawat Keawsrinual

Date: 1-Dec-22

Date: 1-Dec-22

**neediss**

Neediss Supply Instrument Co., Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

**www.neediss.com**

We know the best thing to save environment



บริษัท เอ็นไวแล็บ จำกัด 540.540/1 ซอยบางพลี 7 บางพลี บางพลี กรุงเทพมหานคร 10150  
Envilab Co., Ltd. 540.540/1 Soi Bangkhoe 7 Bangkhoe Bangkok Bangkok 10150  
Tel : 02-802-3577-8 Fax: 02-802-3773 E-mail : info@evltesting.com



Source: Evl-Test Supply Chain

## Verification Test Report

Report No.:

6512 -SLM 06

☐ PM

☐ Onsite UTM :

47P N 1514462 E 654258

Calibrated Date: 1 December 2022

Site : บริษัทเอ็นไวแล็บ จำกัด

Equipment: Sound Level Meter

Manufacturer: NEEDISS

Model: NDSM 309

Serial : 5012

Environment: Temperature 25 °C Humidity 58 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer

Serial No.1351075

Date of Calibration : March.21, 2022

### Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.66	93.47	-0.19	93.66

Calibrated By:

( Sanayu Jantason )

Date:

1 December 2022



Approve By:

( Wisan Ritthikamon )  
1 December 2022

รับรองสำเนาถูกต้อง Date:  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.





RECALIBRATION

DUE DATE:

January 19, 2023

## Certificate of Calibration

### Calibration Certification Information

Cal. Date: January 19, 2022      Rootsmeter S/N: 438320      Ta: 294 °K  
 Operator: Jim Tisch      Pa: 749.05 mm Hg  
 Calibration Model #: TE-5028A      Calibrator S/N: 1328

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.3190	3.7	1.50
2	3	4	1	1.0220	6.2	2.50
3	5	6	1	0.9290	7.5	3.00
4	7	8	1	0.8590	8.7	3.50
5	9	10	1	0.6530	14.8	6.00

### Data Tabulation

Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left( \frac{Ta}{Pa} \right)}$ (y-axis)
0.9941	0.7536	1.2241	0.9951	0.7544	0.7673
0.9907	0.9694	1.5803	0.9917	0.9704	0.9906
0.9890	1.0646	1.7312	0.9900	1.0656	1.0851
0.9874	1.1495	1.8699	0.9884	1.1506	1.1721
0.9793	1.4996	2.4483	0.9802	1.5011	1.5346
QSTD	m=	1.63957	QA	m=	1.02667
	b=	-0.01202		b=	-0.00753
	r=	0.99999		r=	0.99999

### Calculations

Vstd=	$\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$	Va=	$\Delta Vol((Pa-\Delta P)/Pa)$
Qstd=	Vstd/ΔTime	Qa=	Va/ΔTime
For subsequent flow rate calculations:			
Qstd=	$1/m \left( \left( \sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)} \right) - b \right)$	Qa=	$1/m \left( \left( \sqrt{\Delta H \left( \frac{Ta}{Pa} \right)} \right) - b \right)$

### Standard Conditions

Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH:	calibrator manometer reading (in H2O)
ΔP:	rootsmeter manometer reading (mm Hg)
Ta:	actual absolute temperature (°K)
Pa:	actual barometric pressure (mm Hg)
b:	intercept
m:	slope

### RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30.

Tisch Environmental, Inc.  
 145 South Miami Avenue  
 Village of Cleves, OH 45002



รับรองสำเนาถูกต้อง  
 ผู้จัดการฝ่ายควบคุมคุณภาพ

www.tisch-env.com

TOLL FREE: (877)263-7610

FAX: (513)467-9009



## Certificate of Calibration

Certificate No. : 65-200022-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Electronic Balance

Manufacturer : Sartorius

Model : SECURA224-1S

Serial No. : 0034803270

ID No. : ELABBALANCEN04

Capacity : 220 g

Resolution : 0.0001 g

Environment : On site calibration was carried out at the Balance Room, Envilab Co., Ltd.

Ambient Temperature : (23.7 to 23.8) °C

Relative Humidity : (57.1 to 58.0) %

Air Pressure : 1012.0 mbar

Date of Received : 02 February 2022

Date of Calibration : 02 February 2022

Date of Issue : 09 February 2022

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14  
Edition 5, July 2015

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02213103	18 Nov 2022	National Institute of Metrology (Thailand), (NIMT)

Approved by :

( Surachai Promthong )

Laboratory Manager



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 65-200022-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty $\pm$ (g)
0.01	0.0001	0.00011
0.1	0.0001	0.00011
1	0.0000	0.00011
2	0.0001	0.00011
5	0.0000	0.00012
10	0.0001	0.00012
20	-0.0001	0.00013
50	0.0000	0.00014
100	-0.0002	0.00020
200	-0.0004	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2.11$ , providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A B C D E

-0.0001 -0.0002 -0.0002 -0.0001 0.0000 g



Repeatability

Load test : 200 g

Stdev. : 0.00005 g

- o0o -



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ





## Certificate of Calibration

Certificate No. : 65-200022-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Electronic Balance

Manufacturer : Sartorius

Model : SECURA3102-IS

Serial No. : 0034409695

ID No. : ELABBALANCEN03

Capacity : 3100 g

Resolution : 0.01 g

Environment : On site calibration was carried out at the Balance Room, Envilab Co., Ltd.

Ambient Temperature : (23.7 to 24.2) °C

Relative Humidity : (57.6 to 57.8) %

Air Pressure : 1012.0 mbar

Date of Received : 02 February 2022

Date of Calibration : 02 February 2022

Date of Issue : 09 February 2022

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14

Edition 5, July 2015

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
F181-F1821	65-210044-1	31 Jul 2022	National Institute of Metrology (Thailand), (NIMT)

Approved by :



( Surachai Promthong )

Laboratory Manager

รับรองสำเนาถูกต้อง

ผู้จัดการฝ่ายควบคุมคุณภาพ

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.





# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 65-200022-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (g)	Correction (g)	Uncertainty $\pm$ (g)
10	0.00	0.0082
20	0.00	0.0082
50	0.00	0.0082
100	0.00	0.0082
200	0.00	0.0083
500	-0.01	0.0085
1000	-0.01	0.0093
1500	-0.01	0.011
2000	-0.01	0.012
3000	-0.01	0.023

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2.00$ , providing a level of confidence of approximately 95%

Eccentric error

Load test : 1000 g  
A B C D E  
0.00 0.01 0.02 0.00 0.00 g



Repeatability

Load test : 2000 g  
Stdev. : 0.000 g

- o o o -



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ







THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0383

MTC No. EEL. BP. 59/0365

## CALIBRATION CERTIFICATE

Submitted by : Envilab Co.,Ltd.

Address : 540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkok, 10160, Thailand.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Acoustic Calibrator

Manufacturer : Bruel&Kjaer

Model : 4230

Serial No. : 1351075

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.  
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.  
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.  
4. Digital Multimeter Agilent 34401A S/N MY44005560.  
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.  
6. Audio Analyzer Keithley 2015-P S/N 4106495.  
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 10 Mar. 2022

Date of Calibration : 21 Mar. 2022



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : runpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0383

MTC No. EEL. BP. 59/0365

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

### 1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.66	-0.34	$\pm 0.10$	$\pm 0.40$ dB

### 2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	997.8	-2.2	$\pm 1.5$	$\pm 1.0\%$

### 3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.55	$\pm 0.50$	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

(Mr. Weerachai Deechaiyae)

Approved by :

(Mr. Prawate Khuaypa)  
Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 21 Mar. 2022

Date of Issue : 22 Mar. 2022

Ref : 2011265031501147002

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E mail : rumpai@tistr.or.th Website: www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672 80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

EnviLab Co., Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

FM.BL.MTC.002 Rev.4



# CERTIFICATE OF ANALYSIS

## Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)  
LTD  
Part Number: E05NI91E15A0003  
Cylinder Number: EB0146406  
Laboratory: 124 - Plumsteadville - PA  
PGVP Number: A12022  
Gas Code: CO, CO2, NO, NOX, SO2, BALN  
Reference Number: 160-402305646-1  
Cylinder Volume: 148.7 CF  
Cylinder Pressure: 2015 PSIG  
Valve Outlet: 660  
Certification Date: Jan 03, 2022

Expiration Date: Jan 03, 2030

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

### ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	12/27/2021, 01/03/2022
CARBON MONOXIDE	100.0 PPM	98.02 PPM	G1	+/- 0.5% NIST Traceable	12/27/2021
NITRIC OXIDE	100.0 PPM	100.1 PPM	G1	+/- 1.0% NIST Traceable	12/27/2021, 01/03/2022
SULFUR DIOXIDE	100.0 PPM	100.2 PPM	G1	+/- 1.0% NIST Traceable	12/27/2021, 01/03/2022
CARBON DIOXIDE	8.000 %	7.962 %	G1	+/- 0.9% NIST Traceable	12/27/2021
NITROGEN	Balance				

### CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	09010241	KAL004894	98.48 PPM CARBON MONOXIDE/NITROGEN	+/- 0.5%	Oct 16, 2024
NTRM	200610-56	CC733475	98.61 PPM NITRIC OXIDE/NITROGEN	+/- 0.6%	Oct 06, 2026
GMIS	124206889119	CC322885	4.294 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.0%	Sep 03, 2024
NTRM	11010419	KAL004813	99.6 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jul 28, 2023
NTRM	08010636	K019200	13.94 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	Jan 30, 2024

### ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO2	FTIR	Dec 02, 2021
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Dec 09, 2021
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Dec 16, 2021
Nicolet iS50 FTIR AUP2010245 NO2	FTIR	Dec 29, 2021
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Dec 23, 2021

Triad Data Available Upon Request

NOTES: Gross Weight: 28.1 Kg, Net Weight: 5.1 Kg.

UF0X5CX



*[Signature]*  
Approved for Release

Page 1 of 160-402305646-1




*[Signature]*  
รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ



# CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



Supplement to Calibration Certificate No. Q22080017

## CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : VIBRATION METER  
MANUFACTURER : INSTANTEL  
MODEL / TYPE : 721A2601/721A3301  
SERIAL NO. : UM14632/UM14632[EVMINMMATE4632]  
CLID. NO. : 252101369  
JOB CONTROL NO. : 220809080017


CUSTOMER : ENVILAB CO., LTD.  
540, 540/1 SOI BANGKHAE 7, BANGKHAE,  
BANGKHAE, BANGKOK 10160 THAILAND

DATE OF RECEIVED : 09 August 2022

DATE OF ISSUED : 23 August 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
23 August 2022

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22080017A1  
F3-012-04/01-12



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

page 1 of 3




calibration





# CALIBRATION LABORATORY CO., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



## REPORT OF CALIBRATION FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2601/721A3301
SERIAL NO.	:	UM14632/UM14632[EVMINMMATE4632]
DATE OF CALIBRATION	:	10 August 2022

### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 15) \% \text{RH}$

### PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.  
The calibration was performed by using Digital Multimeter, High Resolution Programmable Timer/Counter, Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

1. Digital Multimeter, Hewlett Packard Model 34401A S/N. 3146A75935.
2. High Resolution Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2525 S/N. 397018, 2434988.

### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0112-21, Due Date 26 October 2022.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0001/22, Due Date 22 February 2023.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0009-22, Due Date 22 June 2023.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22080017

F3-011-04/01-12



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

page 2 of 3




@clccalibration



# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

## CALIBRATION DATA

### VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
( mm/s )	( frequency )		( mm/s )	( mm/s )	( mm/s )	± ( % of rdg. )
10	50 Hz	peak	10.000	10.224	-0.224	2.3
20	50 Hz		20.000	20.477	-0.477	1.8
30	50 Hz		30.000	30.692	-0.692	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 1 of 54

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q22080017

F3-011-04/01-12



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

page 3 of 3



gcalibration




Mettler-Toledo (Thailand) Ltd.  
846/4 - 846/5 Lasalle Rd., Bangna Tai Sub-District  
Bangna District, Bangkok 10260  
+662 723 0382  
MT-TH.ServiceSupport@mt.com



## Accuracy Calibration Certificate

### Customer

Company: EnviLab Co., Ltd.  
Address: 540, 540/1 Soi Bang Khae 7, Bang Khae  
City: Bang Khae Contact: Ngarmthip Sampanpuang  
Zip / Postal: 10160  
State / Province: Bangkok  
Order Number:   
\* 0 3 3 1 9 0 7 2 4 8 \*

### Weighing Device

Manufacturer: Mettler Toledo Instrument Type: Weighing Instrument  
Model: XSR205DU Asset Number: N/A  
Serial No.: B911363567 Terminal Model: SRAT  
Building: N/A Terminal Serial No.: B911363567  
Floor: 3 Terminal Asset No.: N/A  
Room: B304

Range	Max. Capacity	Readability (d)
1	81 g	0.00001 g
2	220 g	0.0001 g

### Procedure

Calibration Guideline: EURAMET cg-18 v. 4.0 (11/2015)  
METTLER TOLEDO Work Instruction: CP/W002/20

This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.

The sensitivity/span of the weighing instrument was adjusted before calibration with a built-in weight.

In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

	Temperature		Humidity	
As Found	Start: 22.2 °C	End: 22.6 °C	Start: 58.3 %	End: 59.7 %

As Found Calibration Date: 02-Mar-2022  
As Left Calibration Date: N/A  
Issue Date: 03-Mar-2022

Calibrator:

Naruephon C.

Naruephon Chonprasertsuk

Approved Signatory:



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

- ☒ Kassakorn Tassanachaisakul  
☐ Santi Jitniyom  
☐ Surachet Sukkate

## Measurement Results


### Repeatability

Test Load: 70 g

	As Found	As Left
1	70.00001 g	N/A
2	70.00002 g	N/A
3	70.00001 g	N/A
4	70.00002 g	N/A
5	70.00003 g	N/A
6	70.00001 g	N/A
7	70.00001 g	N/A
8	70.00002 g	N/A
9	70.00002 g	N/A
10	70.00003 g	N/A

Standard Deviation	0.000008 g	N/A
--------------------	------------	-----

○ As Found  
◆ As Left

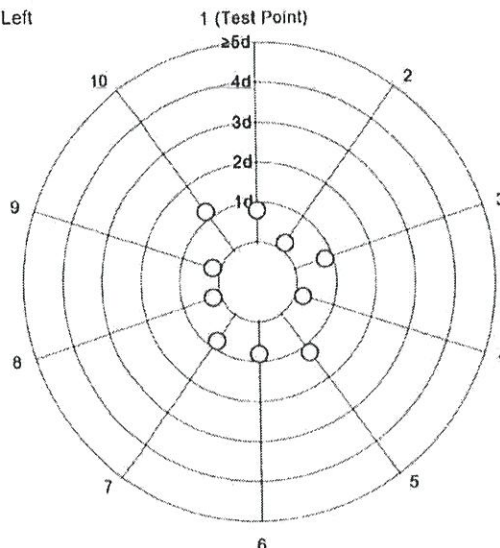

The "d" in the graph represents the readability of the range/interval in which the test was performed.


The results of this graph are based upon the absolute values of the differences from the mean value.

### Eccentricity

Test Load: 100 g

Position	As Found	As Left
1	100.0000 g	N/A
2	100.0002 g	N/A
3	99.9999 g	N/A
4	99.9998 g	N/A
5	100.0001 g	N/A

Maximum Deviation	0.0002 g	N/A
-------------------	----------	-----



As Found

The "d" in the graph represents the readability of the range/interval in which the test was performed.




รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ



## Error of Indication

As Found

	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.00000 g	0.00000 g	0.00000 g	0.017 mg	2
2	0.10000 g	0.10000 g	0.00000 g	0.023 mg	2
3	0.50000 g	0.50001 g	0.00001 g	0.028 mg	2
4	0.99999 g	0.99999 g	0.00000 g	0.032 mg	2
5	1.99999 g	2.00000 g	0.00001 g	0.040 mg	2
6	5.00001 g	5.00001 g	0.00000 g	0.048 mg	2
7	10.00001 g	10.00002 g	0.00001 g	0.062 mg	2
8	49.99998 g	50.00002 g	0.00004 g	0.13 mg	2
9	100.0000 g	100.0000 g	0.0000 g	0.23 mg	2
10	150.0000 g	150.0000 g	0.0000 g	0.35 mg	2
11	199.9999 g	199.9998 g	-0.0001 g	0.42 mg	2

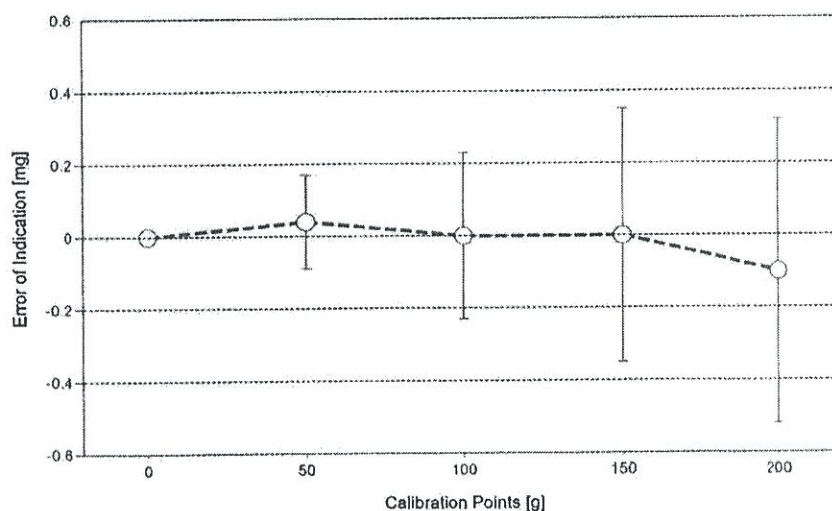

For improved legibility of the graphics only increasing measurement points are shown and measurement points close to zero are not displayed.

The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor  $k$  – which can be larger than 2 according to EURAMET cg-18. The value of the measurand lies within the assigned range of values with a probability of approximately 95%.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

## Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

### Weight Set 1: OIML E2

Weight Set No.:	WS22	Date of Issue:	06-Jan-2022
Certificate Number:	177036	Calibration Due Date:	03-Jul-2023

### Weight Set 2: OIML E2

Weight Set No.:	WS76	Date of Issue:	31-Jan-2022
Certificate Number:	C205470237	Calibration Due Date:	12-Jul-2023

### Thermo Hygrometer

Equipment No.:	IN193	Date of Issue:	14-Jun-2021
Certificate Number:	21H1221	Calibration Due Date:	01-Jun-2022

## Remarks

FACT adjustment functionality activated  
Equipment condition: Good  
Next calibration according to customer's procedure

### End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.



*Signature*  
รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ



## Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with  $k=2$  in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value  $R$  represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use:  $1.5 \cdot 10^{-5} / K$

Temperature range on site for the evaluation of the measurement uncertainty in use:  $3 K$


### Linearization of Uncertainty Equation

	Range		As Found	As Left
	d	Max		
1	0.00001 g	81 g	$U_1 = 0.018 \text{ mg} + 0.00497 \text{ mg/g} \cdot R$	N/A
2	0.0001 g	220 g	$U_2 = 0.06 \text{ mg} + 0.00492 \text{ mg/g} \cdot R$	N/A


To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

### Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication	As Found		As Left	
0.00220 g	0.018 mg	0.82%	N/A	N/A
0.02200 g	0.018 mg	0.082%	N/A	N/A
0.22000 g	0.019 mg	0.0087%	N/A	N/A
2.20000 g	0.029 mg	0.0013%	N/A	N/A
220.0000 g	1.1 mg	0.00052%	N/A	N/A

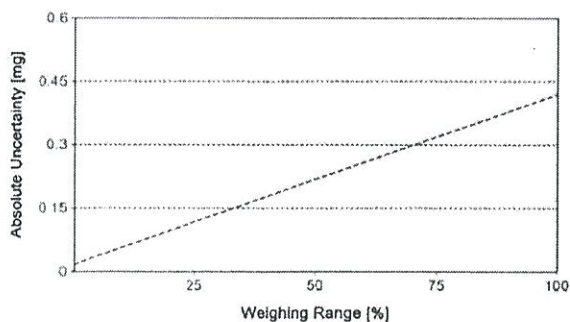

As Found

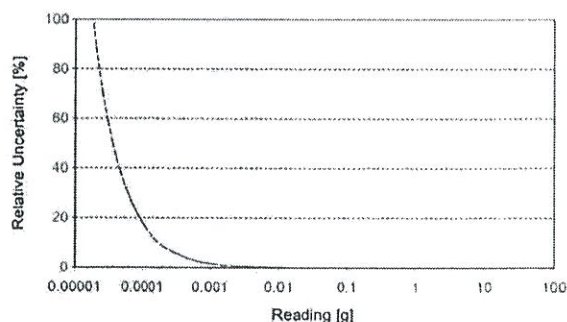

As Left

The weighing range shown in the absolute uncertainty graph refers to the first interval/range of the device.

TH2068-088-030222-ACC-TH



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ



S K SALES AND SERVICE CO.,LTD.  
194/56, 194/57 Thakham Rd. Samae Dam  
Bang Khun Thian Bangkok 10150  
Tel. : 02-417-2144 Fax : 02-417-2155



## Certificate of Calibration

Reference No. : 4182/2202-017 Certificate No. : L2203-290  
Customer : Envilab Co., Ltd. (Head Office) Page 1 of 2  
: 540, 540/1 Soi Bangkhao 7, Bangkhao,  
: Bangkhao Bangkok 10160  
Equipment : Digital Thermo-Hygrometer  
Manufacturer : Testo  
Model : 608-H1  
Serial No. : 83353607  
ID No. : -  
Received Date : 7 March 2022  
Calibrated Date : 9 March 2022  
Issued Date : 15 March 2022

Environment	Start Calibration	Stop Calibration
Ambient Temperature ( °C )	24.7	25.5
Relative Humidity (% RH)	51	52

Calibrated by : Mr. Nattawut Reangdech

### Calibration Method

In-house method : by comparison with standard hygrometer for humidity measurement function  
and comparison with standard thermometer for temperature measurement function into humidity/temperature chamber

### Condition of this result of calibration

#### 1. Reference standard instrument

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Hygrometer	HL-NT2-D	61468576	QR21-0851	13 May 22
2) Digital Thermometer With Probe	GT11	08000089	PSL-T 0072/65	14 November 2022

2. This result of calibration was found accurate as shown on date and place of calibration only

3. This certificate can be traceable to International System of Unit :

- Through Thailand Institute of Scientific And Technological Research (TISTR)
- Through Quality Reborn Co.,Ltd.

Approved by :

☐ Mr.Suphachai Saksri

☐ Mr.Phayak Toolit

☒ Miss Tantaraporn Peltong

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence level of approximately 95 %



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

This certificate may not be reproduced other than in full except with the prior written approval of the S K Sales And Service Company Limited.



Result of Calibration

Function : Humidity Measurement Reference Temperature at 25 °C

STD Reading (% RH)	UUC Reading (% RH)	UUC Error (% RH)	Measurement Uncertainty (±% RH)
50.00	49.0	-1.00	2.3

Function : Temperature Measurement

STD Reading (°C)	UUC Reading (°C)	UUC Error (°C)	Measurement Uncertainty (±°C)
25.012	25.0	-0.012	0.35

Resolution : 0.1 (°C) , 0.1 % RH

STD= Standard

UUC= Unit Under Calibration

\*\* End of Calibration Report \*\*



Envilab Co., Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

sp.

## Certificate of Calibration

Certificate No. : 65-420020-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540,540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : pH Meter with electrode

pH meter

Manufacturer : Horiba

Model : F-74BW-G

Range : N/A pH

Resolution : 0.001 pH

Serial No. : B41J0001

ID No. : ELABPHHB74BW01

Electrode

Model : 9615S

Serial No. : 9X1K0003

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (23.5 to 24.8)° C

Relative Humidity : (50 to 55) %

Date of Received : 02 March 2022

Date of Calibration : 02 March 2022

Date of Issue : 05 March 2022

Calibrated by : Bunjerd Masri

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

### 1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00473/64	27 Aug 2023	National Institute of Metrology Thailand (NIMT)

### 2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61235182	795894	14 Feb 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.985	61223875	769927	15 May 2022	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.008	61244986	795895	25 Feb 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

( Bunjerd Masri )

Supervisor



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.





## Certificate of Calibration

Certificate No. : 65-420020-1

Page : 2 of 2

### Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage ( mV )	Nominal Value ( pH )	UUC Reading		Correction ( mV )	Uncertainty ( ± mV )
			( pH )	( mV )		
4, 7, 10	177.4800	4	4.00	177.5	0.0	0.12
	0.0000	7	7.00	0.0	0.0	0.086
	-177.4800	10	10.00	-177.5	0.0	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer ( pH )	UUC Reading ( pH )	Correction ( pH )	Uncertainty ( ± pH )
4, 7, 10	4.008	4.005	0.003	0.0084
	6.985	7.001	-0.016	0.010
	10.008	10.009	-0.001	0.014

### Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- ๐0๐ -



EnviLab Co.,Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 22TW70  
Page.: 1 of 2

## Certificate of Testing

Equipment :	Dissolved Oxygen Meter
Manufacturer :	Hanna
Model :	HI 9147
Serial No. :	H0007030
ID No. :	ELABDOHI914701
Received Date :	15 March 2022
Test Date :	18 March 2022
Reference :	2203-0566DN-1
Submitted by :	Envilab Co.,Ltd (Head office) 540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkhuae, Bangkok 10160
Laboratory Condition :	Temperature ( $25 \pm 5$ ) °C Humidity ( $50 \pm 20$ ) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean

Approved by :

*Malee*

Approved Signatory

- (☒) Malee Butkruea  
( ) Saithip Meangmai  
( ) Warakorn Lernagtrakul

Issue Date :

22 March 2022



*Walalak*  
รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

B 0284369





Cert.No.: 22TW70

Page.: 2 of 2

**Result :** Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: KC3N0639K

Titration Method (Azide Modification Method) (mg/L)	Dissolved Oxygen Meter Reading (mg/L)	Standard Deviation (mg/L)
8.04	8.1	0.045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

Malu .

a 1100969



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkoe Bangkok 10160

Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



## CALIBRATION CERTIFICATE

Certificate No. : SS2202-154-0002

Date Issued : 24-Feb-22

Customer & : Envilab Co.,Ltd.  
Calibrated Place : 540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkhuae, Bangkok, Thailand  
10160

Equipment : Incubator

Manufacturer : Memmert

Model : IF75

Serial No. : D319.0066

ID No./Tag No. : -

Date Received : 22-Feb-22

Date Calibrated : 22-Feb-22

Calibrated by : Mr. Prakrit Laohawanit

### Calibration Method or Calibration Procedure Used

Standard method : CP-05 TLAS G-20.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

### Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by :

K. Nathong

(Mr. Nathapong Krudaum)



Page 1 of 2

*Oh Sthl*



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ



Certificate No. : SS2202-154-0002

Environment : Ambient Temperature : Start record 25.3 °C, Stop record 25.1 °C  
Relative Humidity : Start record 58.8 %RH, Stop record 58.5 %RH


Calibration Temperature (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Stability <sup>1</sup> (°C)	Measured Uniformity <sup>2</sup> (°C)	Overall Variation <sup>3</sup> (°C)
35	35.0	35.0	0.05	0.07	0.15
37	37.0	37.0	0.04	0.11	0.16
44.5	44.5	44.5	0.08	0.12	0.24

Without adjustment

Calibration Temperature (°C)	STD No. 1 (°C)	STD No. 2 (°C)	STD No. 3 (°C)	STD No. 4 (°C)	STD No. 5 (°C)	STD No. 6 (°C)	STD No. 7 (°C)	STD No. 8 (°C)	STD No. 9 (°C)	Uncertainty <sup>4</sup> ±°C
35	35.15	35.13	35.17	35.17	35.13	35.15	35.15	35.15	35.12	0.24
37	37.20	37.18	37.23	37.19	37.15	37.21	37.20	37.20	37.15	0.24
44.5	44.62	44.60	44.67	44.63	44.58	44.63	44.63	44.63	44.57	0.25

Note : Probe No. 9 is Reference Probe

Setting Air Fresh No. 0



Condition As-Received : New Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

#### Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. AD2112-212-0001 for Temperature Indicator with Sensor Serial No. US37020317, Due 28-Jun-22

Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.

2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.

3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The uncertainty of measurement is included temperature stability.

5. The temperature uniformity, stability, overall variation and indicating temperature is applicable to all air or gas filled temperature controlled enclosures at atmospheric pressure.

End of Certificate



Page 2 of 2  
รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ



## Certificate of Calibration

**Certificate No. :** 65-400577-1

**Page :** 1 of 2

**Submitted by :** Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

**Equipment :** Air Chamber (Refrigerator)

Manufacturer : M-LAB

Model : BIC-140

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 1011

ID No. : ELABBODC140N03

**Environment :** On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (22.0 to 23.0) °C

Relative Humidity : (55 to 58) %

Line Voltage : (224.0 to 226.0) V

**Date of Received :** 11 November 2022

**Date of Calibration :** 11 November 2022

**Date of Issue :** 12 November 2022

**Calibrated by :** Bunjerd Masri

**Calibration Method :** CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400046 & 400028

65-400522-3

03 Apr 2023

National Institute of Metrology Thailand (NIMT)

Approved by :



( Bunjerd Masri )

Supervisor



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง

ผู้จัดการฝ่ายควบคุมคุณภาพ

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.





## Certificate of Calibration

Certificate No. : 65-400577-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

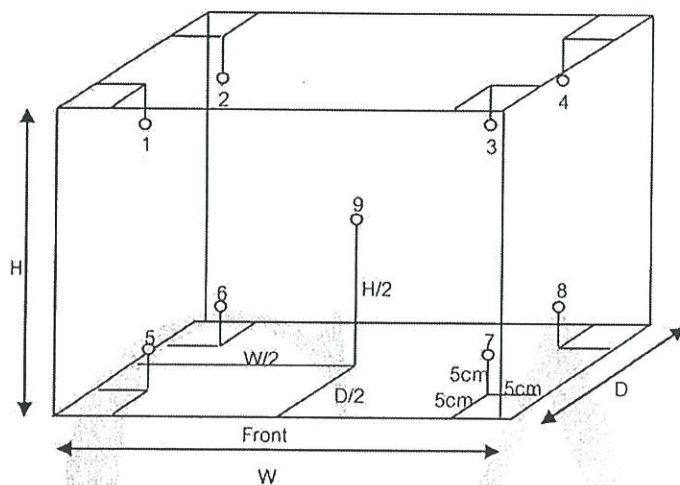

Inside of Chamber

W = 0.38 m

D = 0.35 m

H = 1.15 m

Capacity = 0.15 m<sup>3</sup>

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
4.0	4.0	4.0	3.9	3.9	4.1	3.5	4.1	4.1	4.1	3.8	4.2	0.56

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
4.0	4.0	4.0	0.7	0.1	0.7

**Remark** The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

- o o o -



รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ





## Certificate of Calibration

**Certificate No. :** 65-400155-2

**Page : 1 of 2**

**Submitted by :** Envilab Co., Ltd.  
540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

**Equipment :** Air Chamber (Oven)  
 Manufacturer : Memmert Model : UF 75  
 Range : N/A °C Resolution : 0.1 °C  
 Serial No. : B319.0600 ID No. : ELABHAOVEN0600

**Environment :** On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (30.0 to 31.0) °C

Relative Humidity : (60 to 65) %

Line Voltage : (224.2 to 225.2) V

**Date of Received :** 24 March 2022

**Date of Calibration :** 24 March 2022

**Date of Issue :** 29 March 2022

**Calibrated by :** Permpon Chanpu

**Calibration Method :** CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units  
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400032	64-400589-1	25 May 2022	National Institute of Metrology Thailand (NIMT)

Approved by :



( Bunjerd Masri )

Supervisor



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ





## Certificate of Calibration

Certificate No. : 65-400155-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

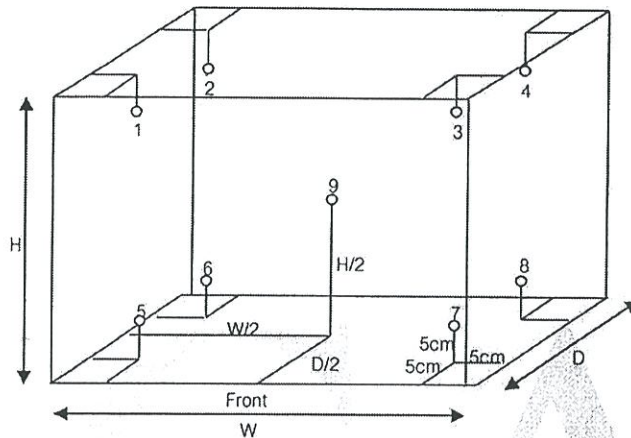

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.56 m

Capacity = 0.07 m<sup>3</sup>

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104.0	103.5	103.5	103.9	104.2	104.2	104.2	104.1	104.0	103.7	104.2	104.3	0.69
110.0	109.5	109.5	110.0	110.3	110.3	110.2	110.2	110.0	109.7	110.2	110.3	0.69
180.0	179.0	179.0	179.1	180.0	180.0	180.1	180.1	179.8	179.0	180.1	180.3	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104.0	103.5	103.5	0.7	0.1	0.8
110.0	109.5	109.5	0.7	0.1	0.8
180.0	179.0	179.0	1.5	0.2	1.5

**Remark** The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

- o0o -



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ





## Certificate of Calibration

Certificate No. : 65-400053-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540,540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : Water Bath

Manufacturer : Memmert

Model : WNB29

Range : N/A °C

Resolution : 0.1 °C

Serial No. : L617.0156

ID No. : ELABWBWNB29N01

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (22.7 to 23.5) °C

Relative Humidity : (45 to 50) %

Line Voltage : (224.0 to 225.0) V

Date of Received : 02 February 2022

Date of Calibration : 02 February 2022

Date of Issue : 07 February 2022

Calibrated by : Permpoon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80  
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units  
Standard Digital Thermometer with RTD probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400031	64-400588-1	24 May 2022	National Institute of Metrology Thailand (NIMT)

Approved by :

( Bunjerd Masri )

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



รับรองสำเนาถูกต้อง

ผู้จัดการฝ่ายควบคุมคุณภาพ





## Certificate of Calibration


Certificate No. : 65-400053-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

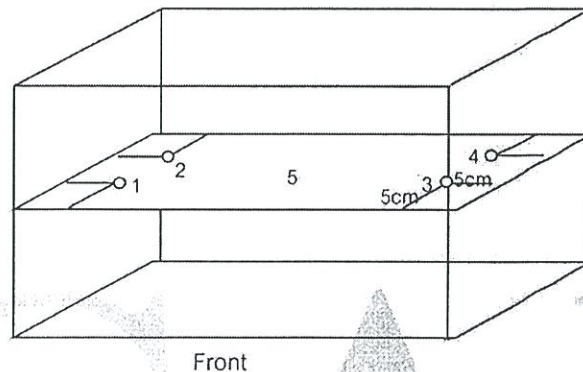

Test Point ( °C )	Setting Temperature ( °C )	Indicating Temperature ( °C )	Measured Temperature ( °C ) @					Uncertainty ( ± °C )	Measured Uniformity ( °C )	Measured Stability ( °C )
			Sensor No.							
			1	2	3	4	5			
95.0	95.0	95.0	95.35	95.45	95.51	95.66	95.56	0.19	0.27	0.06

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- o0o -



Envilab Co.,Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ



## Certificate of Calibration

**Certificate No. :** 65-300146-10

**Page :** 1 of 2

**Submitted by :** Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

**Equipment :** Cylinder

Manufacturer : PYREX

Class : A

Capacity : 50 ml

Graduation : 1 ml

ID No. : C-WW-020/18

**Environment :** Ambient Temperature :  $(23 \pm 2)$  °C

Relative Humidity :  $(50 \pm 15)$  %

Air Pressure : 1002.0 mbar.

**Date of Received :** 09 March 2022

**Date of Calibration :** 21 March 2022

**Date of Issue :** 21 March 2022

**Calibrated by :** Areerat Sombun

**Calibration Method :** In-house method CAL-M3001 based on ASTM E 542-01

**Reference Standard Instruments :** This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	64-200354-1	02 Jun 2022	National Institute of Metrology (Thailand) (NIMT)

Approved by :



( Wipa Tovadee )

Supervisor



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ





# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 65-300146-10

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume ( ml )	Measuring Volume ( ml )
30	29.79
50	49.73

Uncertainty of measurement with in  $\pm$  0.054 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2.00$  ,  
providing a level of confidence of approximately 95%

- o0o -



Envilab Co.,Ltd.

D.

*Signature*

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ



## Certificate of Calibration

**Certificate No. :** 65-300147-4

**Page :** 1 of 2

**Submitted by :** Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

**Equipment :** Cylinder

Manufacturer : ISOLAB

Class : A

Capacity : 1000 ml

Graduation : 10 ml

ID No. : C-WW-028/18

**Environment :** Ambient Temperature :  $(23 \pm 2)$  °C

Relative Humidity :  $(50 \pm 15)$  %

Air Pressure : 1002.0 mbar.

**Date of Received :** 09 March 2022

**Date of Calibration :** 21 March 2022

**Date of Issue :** 21 March 2022

**Calibrated by :** Areerat Sombun

**Calibration Method :** In-house method CAL-M3001 based on ASTM E 542-01

**Reference Standard Instruments :** This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	64-200354-1	02 Jun 2022	National Institute of Metrology (Thailand) (NIMT)

Approved by :



( Wipa Tovadce )

Supervisor



*Wipa*

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ





## Certificate of Calibration

**Certificate No. :** 65-300147-4

**Page :** 1 of 2

**Submitted by :** Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

**Equipment :** Cylinder

Manufacturer : ISOLAB

Class : A

Capacity : 1000 ml

Graduation : 10 ml

ID No. : C-WW-028/18

**Environment :** Ambient Temperature :  $(23 \pm 2)$  °C

Relative Humidity :  $(50 \pm 15)$  %

Air Pressure : 1002.0 mbar.

**Date of Received :** 09 March 2022

**Date of Calibration :** 21 March 2022

**Date of Issue :** 21 March 2022

**Calibrated by :** Areerat Sombun


**Calibration Method :** In-house method CAL-M3001 based on ASTM E 542-01

**Reference Standard Instruments :** This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	64-200354-1	02 Jun 2022	National Institute of Metrology (Thailand) (NIMT)

Approved by :



( Wipa Tovadce )

Supervisor



*Wipa*

รับรองสำเนาถูกต้อง

ผู้จัดการฝ่ายควบคุมคุณภาพ

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 65-300147-4

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume ( ml )	Measuring Volume ( ml )
500	501.84
1000	1001.39

Uncertainty of measurement with in  $\pm$  0.17 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2.00$  ,  
providing a level of confidence of approximately 95%

- o0o -

*D*



Envilab Co.,Ltd.

*OK*

รับรองสำเนาถูกต้อง  
ผู้จัดการฝ่ายควบคุมคุณภาพ

