

ภาคผนวก จ

ใบรับรองการสอบเทียบเครื่องมือ

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Total Suspended Particulate	High Volume	RYG_FS0291	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0292	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0179	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0396	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	RYG_EN0001	23-Mar-22	23-Mar-23	12
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0188	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0185	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0192	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0183	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	Digital Balance	RYG_EN0001	23-Mar-22	23-Mar-23	12
Ambient	Nitrogen Dioxide	NO ₂ Analyzer	RYG_FS0255	1-Jul-22	1-Jan-23	6
Ambient	Nitrogen Dioxide	NO ₂ Analyzer	BKK_FS0797	1-Jul-22	1-Jan-23	6
Ambient	Nitrogen Dioxide	NO ₂ Analyzer	RYG_FS0535	1-Jul-22	1-Jan-23	6
Ambient	Nitrogen Dioxide	NO ₂ Analyzer	RYG_FS0459	1-Jul-22	1-Jan-23	6
Ambient	Sulfur Dioxide	SO ₂ Analyzer	RYG_FS0254	1-Jul-22	1-Jan-23	6
Ambient	Sulfur Dioxide	SO ₂ Analyzer	BKK_FS0796	1-Jul-22	1-Jan-23	6
Ambient	Sulfur Dioxide	SO ₂ Analyzer	RYG_FS0266	1-Jul-22	1-Jan-23	6
Ambient	Sulfur Dioxide	SO ₂ Analyzer	RYG_FS0458	1-Jul-22	1-Jan-23	6
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0328	31-Jan-22	29-Jul-23	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0412	29-Jul-21	27-Jan-23	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0411	29-Jul-21	27-Jan-23	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0141	7-Jun-21	6-Dec-22	18
Ambient	1,3-Butadiene	GC-MSD	RYG_EN0136	7-Jul-22	7-Jan-24	18
Ambient	Styrene	GC-MSD	RYG_EN0136	7-Jul-22	7-Jan-24	18
Ambient	Cyclohexane	GC-MSD	RYG_EN0136	7-Jul-22	7-Jan-24	18
Ambient	Toluene	GC-MSD	RYG_EN0136	7-Jul-22	7-Jan-24	18
Stack	1,3-Butadiene	Console Control Unit	BKK_FS0468	12-Jul-22	12-Jan-23	6
Stack	1,3-Butadiene	Flue gas Analyzer	RYG_FS0465	19-Jan-22	19-Jan-23	12
Stack	1,3-Butadiene	Field Rotameter	BKK_FS1039	1-Oct-22	1-Jan-23	3
Stack	1,3-Butadiene	GC-MSD	BKK_EN0119	1-Oct-21	1-Apr-23	18
Stack	Oxides of Nitrogen	Console Control Unit	BKK_FS0468	12-Jul-22	12-Jan-23	6
Stack	Oxides of Nitrogen	Flue gas Analyzer	RYG_FS0465	19-Jan-22	19-Jan-23	12
Stack	Oxides of Nitrogen	Vacuum Gauge	BKK_FS0545	10-May-22	8-Nov-23	18
Stack	Oxides of Nitrogen	SPECTROPHOTOMETER	RYG_EN0037	27-Sep-22	27-Mar-24	18
Stack	Cyclohexane	Console Control Unit	BKK_FS0468	12-Jul-22	12-Jan-23	6
Stack	Cyclohexane	Flue gas Analyzer	RYG_FS0465	19-Jan-22	19-Jan-23	12
Stack	Cyclohexane	Field Rotameter	BKK_FS1039	1-Oct-22	1-Jan-23	3
Stack	Cyclohexane	GC-FID	BKK_EN0126	21-Oct-21	21-Apr-23	18
Stack	Sulfur Dioxide	Console Control Unit	BKK_FS0468	12-Jul-22	12-Jan-23	6
Stack	Sulfur Dioxide	Flue gas Analyzer	RYG_FS0465	19-Jan-22	19-Jan-23	12
Stack	Sulfur Dioxide	Dry Gas	BKK_FS0534	12-Jul-22	12-Jan-23	6
Stack	Total Suspended Particulate	Console Control Unit	BKK_FS0468	12-Jul-22	12-Jan-23	6
Stack	Total Suspended Particulate	Flue gas Analyzer	RYG_FS0465	19-Jan-22	19-Jan-23	12
Stack	Total Suspended Particulate	Digital Balance	RYG_EN0003	23-Mar-22	23-Mar-23	12
Workplace	1,3-Butadiene	Field Rotameter	RYG_FS0199	1-Jul-22	1-Oct-22	3
Workplace	1,3-Butadiene	Field Rotameter	RYG_FS0199	1-Oct-22	1-Jan-23	3
Workplace	1,3-Butadiene	GC-MSD	BKK_EN0119	1-Oct-21	1-Apr-23	18
Workplace	Cyclohexane	Field Rotameter	RYG_FS0199	1-Jul-22	1-Oct-22	3
Workplace	Cyclohexane	Field Rotameter	RYG_FS0199	1-Oct-22	1-Jan-23	3
Workplace	Cyclohexane	GC-FID	BKK_EN0126	21-Oct-21	21-Apr-23	18
Workplace	Formaldehyde	Field Rotameter	RYG_FS0199	1-Jul-22	1-Oct-22	3
Workplace	Formaldehyde	Field Rotameter	RYG_FS0199	1-Oct-22	1-Jan-23	3
Workplace	Formaldehyde	GC-FID	BKK_EN0126	21-Oct-21	21-Apr-23	18
Workplace	Styrene	Field Rotameter	RYG_FS0199	1-Jul-22	1-Oct-22	3
Workplace	Styrene	Field Rotameter	RYG_FS0199	1-Oct-22	1-Jan-23	3
Workplace	Styrene	GC-MSD	BKK_EN0119	1-Oct-21	1-Apr-23	18
Workplace	Toluene	Field Rotameter	RYG_FS0199	1-Jul-22	1-Oct-22	3
Workplace	Toluene	Field Rotameter	RYG_FS0199	1-Oct-22	1-Jan-23	3
Workplace	Toluene	GC-MSD	BKK_EN0119	1-Oct-21	1-Apr-23	18

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Noise	Leq 24 hrs	Sound Calibrator	RYG_FS0213	26-Apr-22	26-Apr-23	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0381	26-Aug-22	26-Aug-23	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0384	26-Aug-22	26-Aug-23	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0386	26-Aug-22	26-Aug-23	12
Noise	Leq 8 hrs	Sound Calibrator	RYG_FS0213	26-Apr-22	26-Apr-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0022	21-Jan-22	21-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0026	21-Jan-22	21-Jan-23	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0027	10-Jan-22	10-Jan-23	12
Noise	Noise Dose, TWA	Dose Badge Reader	RYG_FS0212	7-Oct-22	7-Oct-23	12
Rayong Lab	Formaldehyde	SPECTROPHOTOMETER	RYG_EN0037	27-Sep-22	27-Mar-24	18
Rayong Lab	pH at 25 °C	pH meter	RYG_EN0183	17-Mar-22	17-Mar-23	12
Rayong Lab	BOD	DO meter with Sensor	RYG_EN0032	14-Feb-22	15-Aug-23	18
Rayong Lab	BOD	Incubator	RYG_EN0154	22-Apr-22	21-Oct-23	18
Rayong Lab	COD	Spectrophotometer	RYG_EN0037	27-Sep-22	27-Mar-24	18
Rayong Lab	Total Suspended Solids	Electronic Balance	RYG_EN0002	23-Mar-22	23-Mar-23	12
Rayong Lab	Total Suspended Solids	Hot Air Oven	RYG_EN0010	20-Oct-22	20-Apr-24	18
Rayong Lab	Total Dissolved Solids 180°C	Electronic Balance	RYG_EN0002	23-Mar-22	23-Mar-23	12
Rayong Lab	Total Dissolved Solids 180°C	Hot Air Oven	RYG_EN0010	20-Oct-22	20-Apr-24	18
Rayong Lab	Oil & Grease	Electronic Balance	RYG_EN0002	23-Mar-22	23-Mar-23	12
Rayong Lab	Oil & Grease	Hot Air Oven	RYG_EN0006	20-Oct-22	20-Apr-24	18
Rayong Lab	Oil & Grease	Water Bath	RYG_EN0061	20-Oct-22	20-Apr-24	18
Rayong Lab	Temperature	pH Meter	RYG_FS0420	14-Mar-22	14-Mar-23	12
Rayong Lab	Total Kjeldahl Nitrogen	Block Digestion Unit	RYG_EN0188	17-Mar-22	17-Mar-23	12
Rayong Lab	Total Kjeldahl Nitrogen	pH Meter	RYG_EN0152	23-Dec-21	23-Dec-22	12
Water Lab	1,3-Butadiene	Gas Chromatography (MSD)	BKK_EN0059	21-Jun-22	21-Dec-23	18
Water Lab	Styrene	Gas Chromatography (MSD)	BKK_EN0059	21-Jun-22	21-Dec-23	18
Water Lab	Toluene	Gas Chromatography (MSD)	BKK_EN0059	21-Jun-22	21-Dec-23	18
Water Lab	Methanol	Gas Chromatography	BKK_EN0041	25-Nov-21	25-May-23	18
Water Lab	Zinc	ICP-MS	BKK_EL0043	30-Sep-21	29-Mar-23	18
Water Lab	Zinc	Hot Block	BKK_EL0054	7-Apr-22	7-Oct-23	18
Water Lab	Zinc	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Soil	1,3-Butadiene	Gas Chromatography (MSD)	BKK_EN0059	21-Jun-22	21-Dec-23	18
Soil	Styrene	Gas Chromatography (MSD)	BKK_EN0059	21-Jun-22	21-Dec-23	18
Soil	Toluene	Gas Chromatography (MSD)	BKK_EN0059	21-Jun-22	21-Dec-23	18
Soil	Methanol	Gas Chromatography	BKK_EN0041	25-Nov-21	25-May-23	18
Soil	Formaldehyde	Spectrophotometer	BKK_EN0356	21-Jan-22	21-Jan-23	12
Soil	Zinc	ICP-OES	BKK_EL0037	13-Sep-21	12-Mar-23	18
Soil	Zinc	Hot Block	BKK_EL0054	7-Apr-22	7-Oct-23	18
Soil	Zinc	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18




High Volume Air Sampler Calibration Worksheet

Project Site : Kuraray GC Advanced Materials Co., Ltd.
Calibrate Location : Mapchalood temple (A1)
Calibrate Date : 28-Sep-22
CalibrationSheet No.: C-280922-RYG_FS0291
Calibrator ID: RYG_FS0206
Calibrator Model : TE-5028A
Calibrator S/N : 1543

Barometric Pressure (mm Hg) : 755
Temperature (°C) : 30
High Volume ID : RYG_FS0291
High Volume Model : TE-5170D
High Volume S/N : 5333
Calibrator Slope : 1.47433
Calibrator Intercept : -0.01503

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.8	1.1369	40	Slope : 29.2570 Intercept : 7.1385 Correlation Coefficient : 0.9992
2	3.4	1.2512	44	
3	4.6	1.4530	50	
4	5.6	1.6016	54	
5	7.2	1.8140	60	

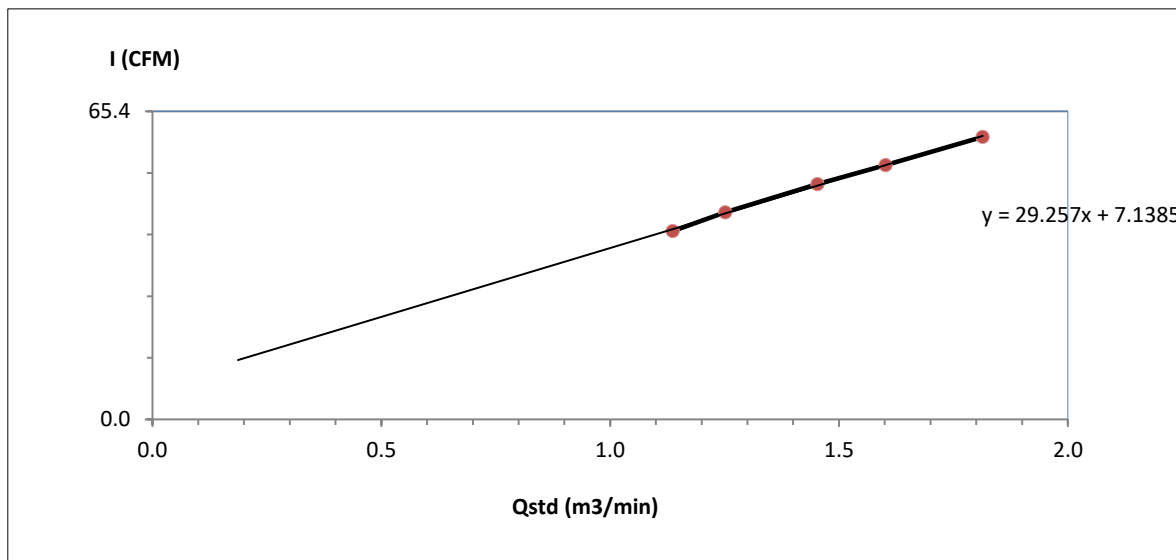

Calibrated by

(Mr.Anurak Tongkhajonsakda)
Field Scientist(1)

Approved by :


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)



High Volume Air Sampler Calibration Worksheet

Project Site :	Kuraray GC Advanced Materials Co., Ltd.	Barometric Pressure (mm Hg) :	755
Calibrate Location :	Nhong Fab community (A2)	Temperature (°C) :	30
Calibrate Date :	28-Sep-22	High Volume ID :	RYG_FS0292
CalibrationSheet No.:	C-280922-RYG_FS0292	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0206	High Volume S/N :	5497
Calibrator Model :	TE-5028A	Calibrator Slope :	1.47433
Calibrator S/N :	1543	Calibrator Intercept :	-0.01503

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	3.2	1.2143	40	Slope : 40.1694 Intercept : -9.4604 Correlation Coefficient : 0.9940
2	4.0	1.3559	44	
3	4.7	1.4685	50	
4	5.6	1.6016	54	
5	6.4	1.7111	60	

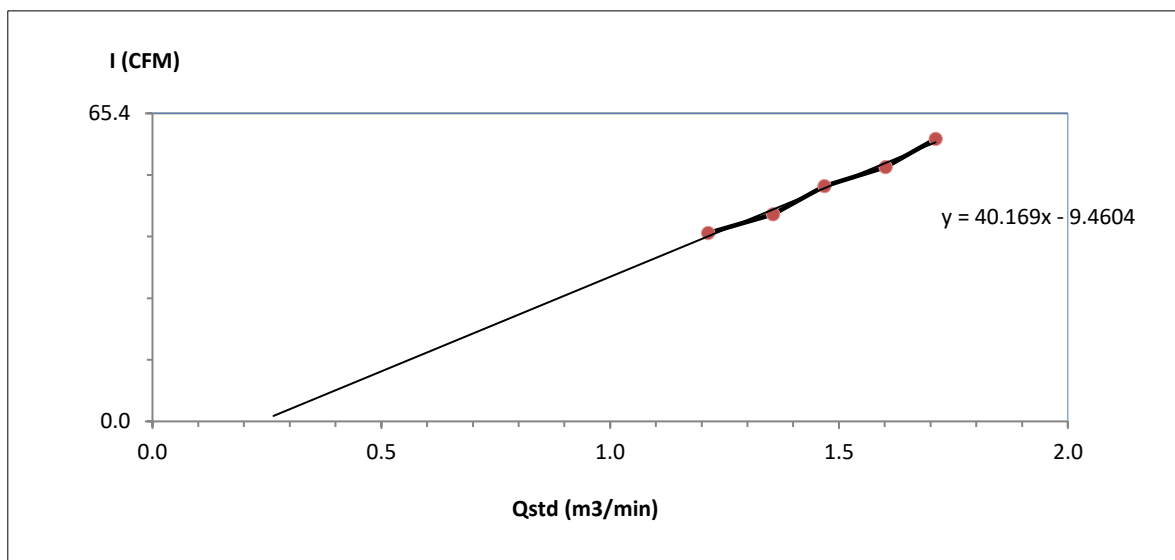

Calibrated by

(Mr.Anurak Tongkhajonsakda)
Field Scientist(1)

Approved by :


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)



High Volume Air Sampler Calibration Worksheet

Project Site :	Kuraray GC Advanced Materials Co., Ltd.	Barometric Pressure (mm Hg) :	755
Calibrate Location :	Prachummitbhumrung temple (A3)	Temperature (°C) :	30
Calibrate Date :	28-Sep-22	High Volume ID :	RYG_FS0179
CalibrationSheet No.:	C-280922-RYG_FS0179	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0206	High Volume S/N :	4805
Calibrator Model :	TE-5028A	Calibrator Slope :	1.47433
Calibrator S/N :	1543	Calibrator Intercept :	-0.01503

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	3.2	1.2143	40	Slope : 29.4084 Intercept : 3.8873 Correlation Coefficient : 0.9949
2	4.2	1.3890	44	
3	5.2	1.5439	50	
4	6.6	1.7374	54	
5	7.8	1.8874	60	

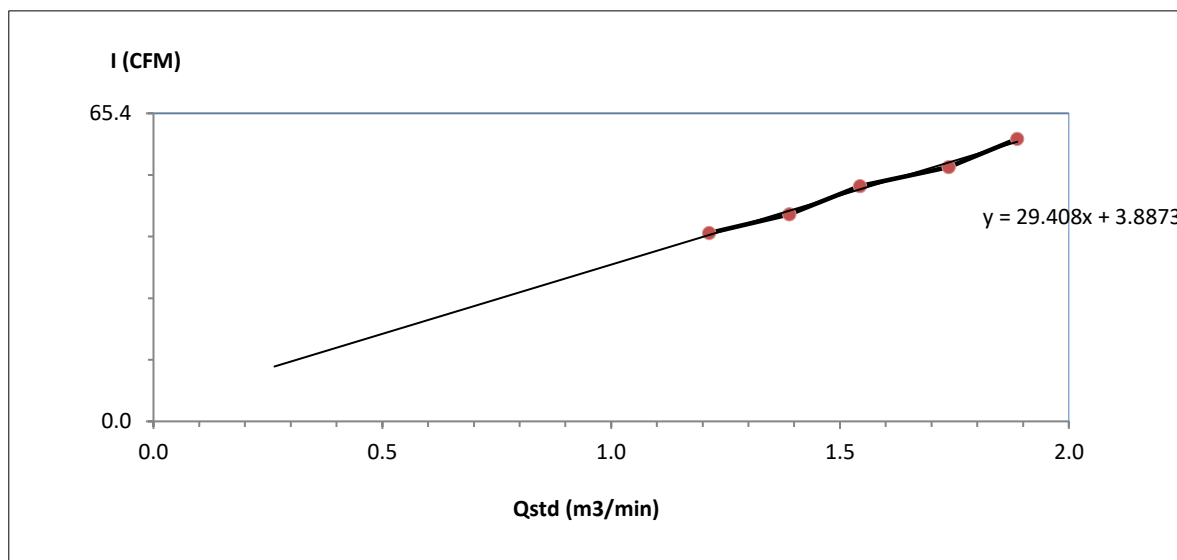

Calibrated by
(Mr.Anurak Tongkhajonsakda)
Field Scientist(1)


Approved by :
(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)



High Volume Air Sampler Calibration Worksheet

Project Site :	Kuraray GC Advanced Materials Co., Ltd.	Barometric Pressure (mm Hg) :	755
Calibrate Location :	Mapchalood-chark klang community (A4)	Temperature (°C) :	30
Calibrate Date :	28-Sep-22	High Volume ID :	RYG_FS0396
CalibrationSheet No.:	C-280922-RYG_FS0396	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0206	High Volume S/N :	5688
Calibrator Model :	TE-5028A	Calibrator Slope :	1.47433
Calibrator S/N :	1543	Calibrator Intercept :	-0.01503

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	3.2	1.2143	40	Slope : 41.9663 Intercept : -11.2227 Correlation Coefficient : 0.9978
2	3.8	1.3219	44	
3	4.6	1.4530	50	
4	5.4	1.5730	54	
5	6.2	1.6844	60	

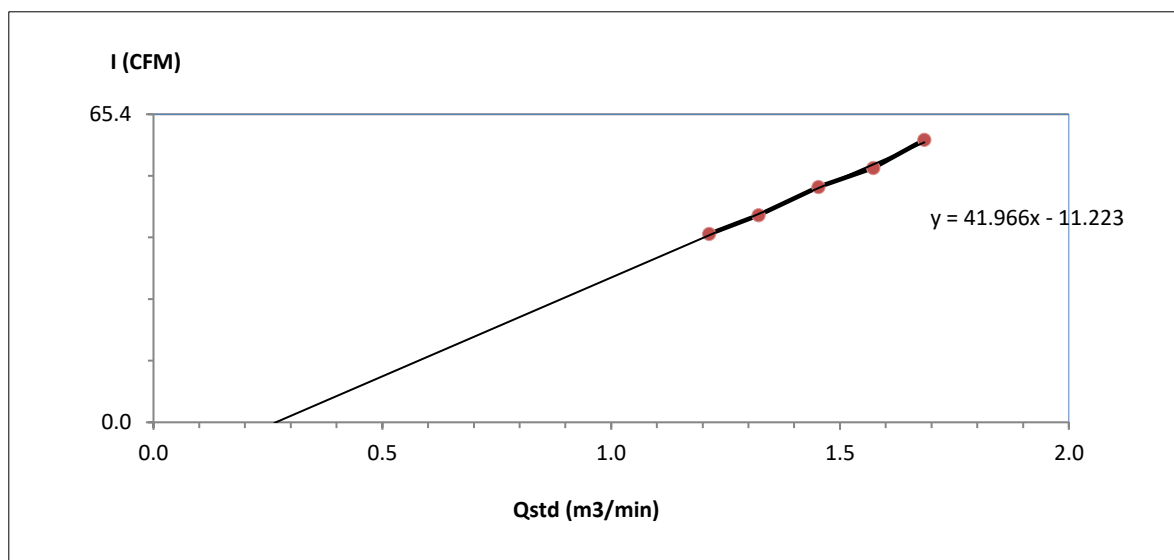

Calibrated by

(Mr.Anurak Tongkhajonsakda)
Field Scientist(1)

Approved by :

(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)



PENTA
CALIBRATION

PENTA CALIBRATION CO., LTD.

66/124 The Connect 33 Village Kanchanaphisek Road
Dokmai Prawet Bangkok 10250
Tel: +66 (0) 2069-9773
www.pentacal.com


Certificate of Calibration

Represent to Certificate of Calibration ,PTC/07/22102

Certificate No.:	PTC/07/22102	Page:	1 of 2
Equipment:	Digital Balance	Condition:	Normal
Manufacturer:	Sartorius	Serial No:	25409664
Model:	LA130S-F	ID No:	RYG_EN0001
Type of Balance:	Single interval		



Customer: ALS Laboratory Group (Thailand) Co.,Ltd.
616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand

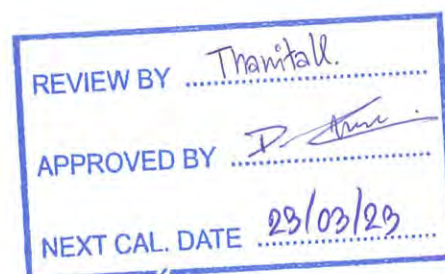

Environment Condition: Temperature 23.9 °C ± 0.3 °C
Humidity 58.1 %RH ± 4.4 %RH
Air density 1.17 kg/m³

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd.
616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand

The Method used: In house method, PTC-WI-07, base on Euramet cg. 18

Traceability: This certificate is traceable to the SI Units through Thai Calibration Service Co.,Ltd.
, NSC-ONSC Accreditation No.: Calibration 0189

Date Received: March 23, 2022

Calibration Date: March 23, 2022

Issued Date: March 25, 2022

Calibration By: Mr. Rungroje Metakul



PENTA CALIBRATION CO.,LTD

[Signature]

(Mr.Kriangsak Kalasri)

Reviewed by

Approved By :

[Signature]

(Mr. Keattisak Kerdto)

Laboratory Manager

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognised national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The effect that the results relate only to the items calibrated.

This calibration certificate shall not be reproduced except in full only, without written approval from penta calibration co., ltd



Represent to Certificate of Calibration ,PTC/07/22102

Certificate No.: PTC/07/22102



Page: 2 of 2

Measurement Results:

Without Adjustment :

Function Calibration: Non Adjustment

Eccentric Error: Weight to be 1/3 ,1/2 or of Maximum capacity

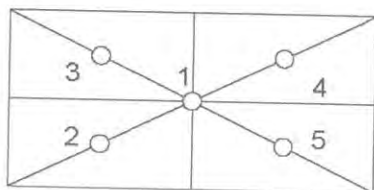

Eccentricity test 50 (g)

Position (g)				
1	2	3	4	5
0.0000	0.0000	-0.0001	0.0000	0.0001
Maximum deviation:			0.0001	

Repeatability Test : Weight to be $1/2 \leq L_1 \leq$ Maximum capacity

Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
100	0.00009

Error of indication : from nominal value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Indication (g)	Correction of Balance (g)	Uncertainty (g)	k
0	0.00000	0.0000	0.0000	0.00026	2.87
0.01	0.01000	0.0100	0.0000	0.00026	2.65
0.05	0.05000	0.0500	0.0000	0.00026	2.65
0.1	0.10000	0.1000	0.0000	0.00026	2.65
0.5	0.50000	0.4999	0.0001	0.00026	2.65
1	1.00000	0.9999	0.0001	0.00026	2.65
2	2.00000	1.9999	0.0001	0.00026	2.65
5	5.00001	5.0000	0.0000	0.00026	2.65
10	10.00000	10.0001	-0.0001	0.00026	2.65
20	20.00003	20.0001	-0.0001	0.00026	2.52
100	100.00004	100.0001	-0.0001	0.00027	2.18

Note: Weight of adjust - (g)

The End of Certificate




High Volume Air Sampler Calibration Worksheet

Project Site : Kuraray GC Advanced Materials Co., Ltd.
Calibrate Location : Mapchalood temple (A1)
Calibrate Date : 28-Sep-22
CalibrationSheet No.: C-280922-RYG_FS0188
Calibrator ID: RYG_FS0206
Calibrator Model : TE-5028A
Calibrator S/N : 1543

Barometric Pressure (mm Hg) : 755
Temperature (°C) : 30
High Volume ID : RYG_FS0188
High Volume Model : TE-5009X
High Volume S/N : 4796
Calibrator Slope : 1.47433
Calibrator Intercept : -0.01503

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	1.8	0.9145	32	Slope : 26.6885 Intercept : 7.2900 Correlation Coefficient : 0.9978
2	2.6	1.0961	36	
3	3.2	1.2143	40	
4	4.2	1.3890	44	
5	5.0	1.5142	48	

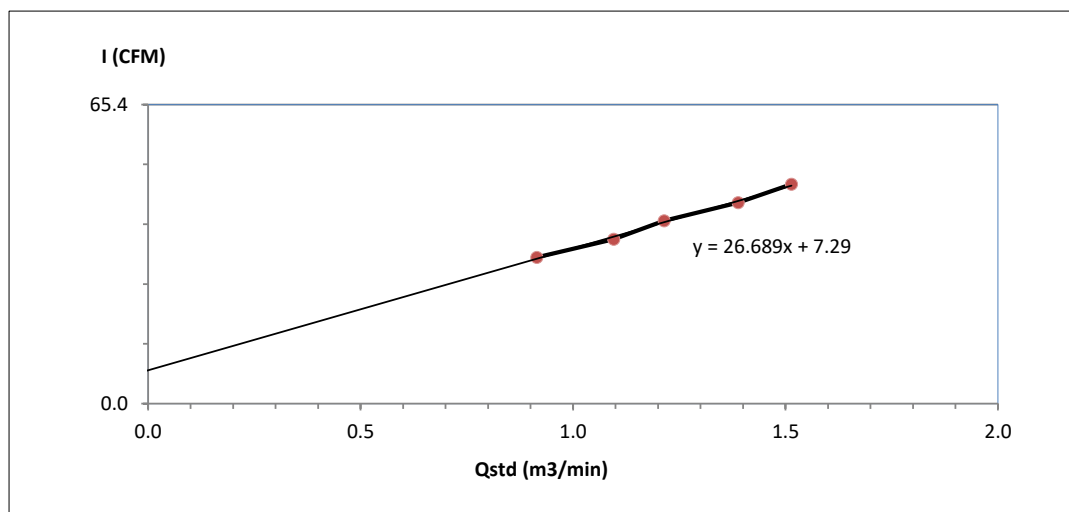

Calibrated by

(Mr.Anurak Tongkhajonsakda)
Field Scientist(1)

Approved by :


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)



High Volume Air Sampler Calibration Worksheet

Project Site :	Kuraray GC Advanced Materials Co., Ltd.	Barometric Pressure (mm Hg) :	755
Calibrate Location :	Nhong Fab community (A2)	Temperature (°C) :	30
Calibrate Date :	28-Sep-22	High Volume ID :	RYG_FS0185
CalibrationSheet No.:	C-280922-RYG_FS0185	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0206	High Volume S/N :	4793
Calibrator Model :	TE-5028A	Calibrator Slope :	1.47433
Calibrator S/N :	1543	Calibrator Intercept :	-0.01503

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	1.9	0.9392	32	Slope : 38.7558 Intercept : -4.6211 Correlation Coefficient : 0.9995
2	2.4	1.0537	36	
3	2.9	1.1567	40	
4	3.4	1.2512	44	
5	4.0	1.3559	48	

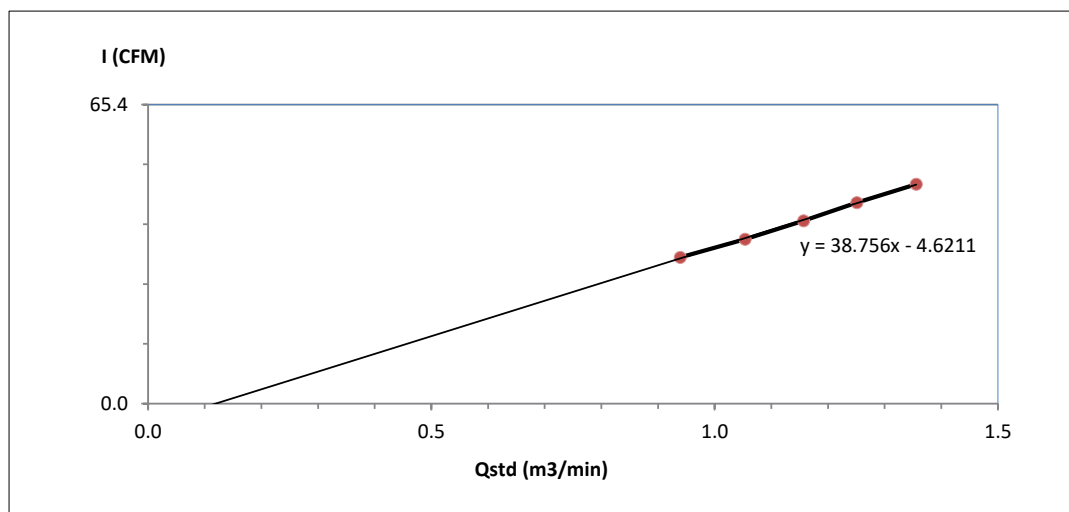

Calibrated by

(Mr.Anurak Tongkhajonsakda)
Field Scientist(1)

Approved by :


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)



High Volume Air Sampler Calibration Worksheet

Project Site :	Kuraray GC Advanced Materials Co., Ltd.	Barometric Pressure (mm Hg) :	755
Calibrate Location :	Prachummitbhumrung temple (A3)	Temperature (°C) :	30
Calibrate Date :	28-Sep-22	High Volume ID :	RYG_FS0192
CalibrationSheet No.:	C-280922-RYG_FS0192	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0206	High Volume S/N :	5331
Calibrator Model :	TE-5028A	Calibrator Slope :	1.47433
Calibrator S/N :	1543	Calibrator Intercept :	-0.01503

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.2	1.0094	32	Slope : 31.1270 Intercept : 1.4653 Correlation Coefficient : 0.9938
2	2.6	1.0961	36	
3	3.2	1.2143	40	
4	4.0	1.3559	44	
5	5.0	1.5142	48	

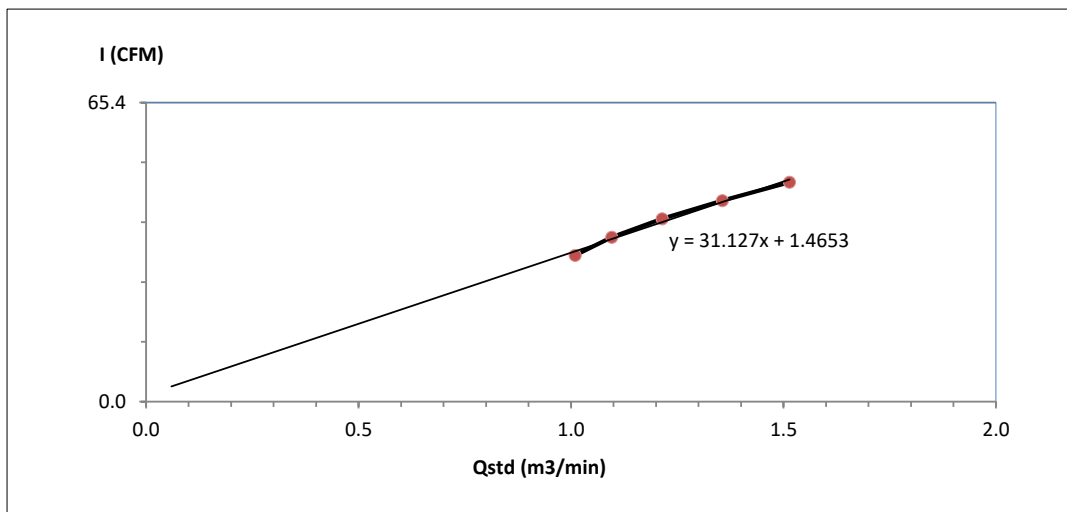

Calibrated by

(Mr.Anurak Tongkhajonsakda)
Field Scientist(1)

Approved by :

(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)




High Volume Air Sampler Calibration Worksheet

Project Site : Kuraray GC Advanced Materials Co., Ltd.
Calibrate Location : Mapchalood-chark klang community (A4)
Calibrate Date : 28-Sep-22
CalibrationSheet No.: C-280922-RYG_FS0183
Calibrator ID: RYG_FS0206
Calibrator Model : TE-5028A
Calibrator S/N : 1543

Barometric Pressure (mm Hg) : 755
Temperature (°C) : 30
High Volume ID : RYG_FS0183
High Volume Model : TE-5009X
High Volume S/N : 4791
Calibrator Slope : 1.47433
Calibrator Intercept : -0.01503

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.0	0.9632	32	Slope : 38.1059 Intercept : -4.6090 Correlation Coefficient : 0.9982
2	2.5	1.0751	36	
3	2.9	1.1567	40	
4	3.5	1.2693	44	
5	4.2	1.3890	48	

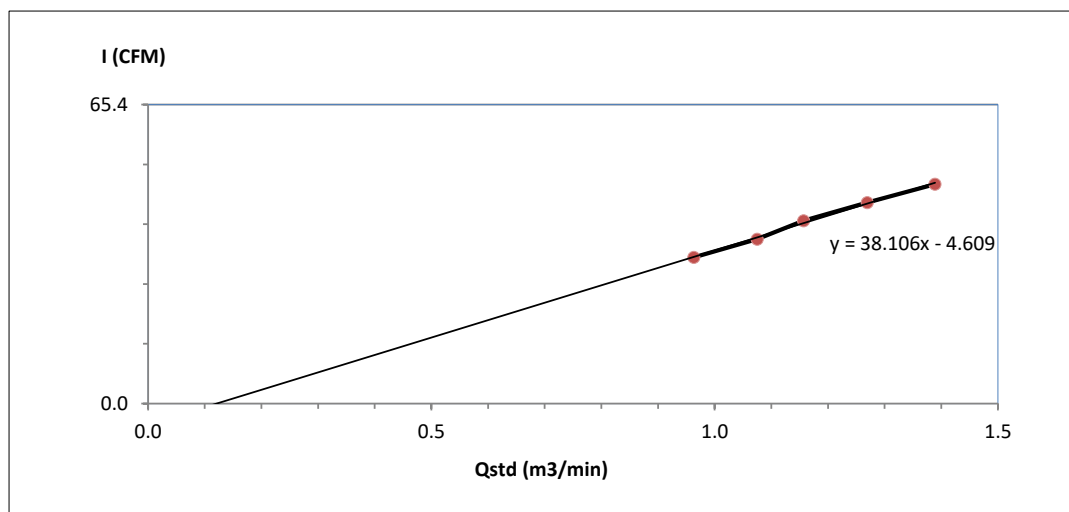

Calibrated by Anurak T.
 (Mr.Anurak Tongkhajonsakda)
 Field Scientist(1)

Approved by : N. Pong
 (Mr. Noppong Juntarupan)
 Enviro Field Coordinator Scientist (3)




MULTIPOINT CALIBRATION REPORT

Calibration Date 1-Jul-22
Manufacturer Teledyne API
Serial No. 2197
Calibrator Manufacturer Teledyne API
Serial No. 947
Std. Gas Concentration (PPM) 55.88
Cylinder Pressure (psi) 1800
Certified Date 9-Feb-22

Equipment Name NOx Analyzer
Model T200
Equipment ID RYG_FS0255
Model 700
Cylinder No. GN0027222
Certified By Airgas Inc.
Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.60	-0.40	-0.40	100.20	0.20	0.20
2	200.00	198.10	-1.90	-0.95	198.50	-1.50	-0.75
3	300.00	297.50	-2.50	-0.83	298.70	-1.30	-0.43
4	400.00	396.50	-3.50	-0.88	398.60	-1.40	-0.35
AVERAGE (%)				-0.59			-0.25

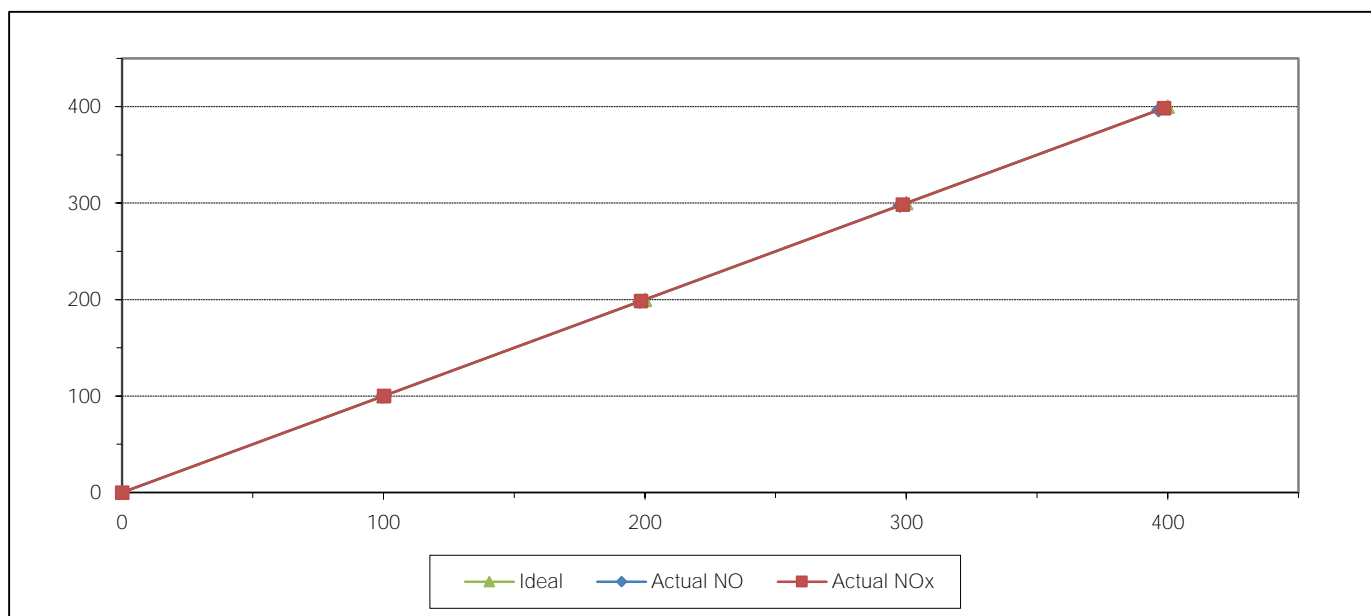

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager




MULTIPOINT CALIBRATION REPORT

Calibration Date 1-Jul-22
Manufacturer HORIBA
Serial No. H73KYD1M
Calibrator Manufacturer Teledyne API
Serial No. 947
Std. Gas Concentration (PPM) 55.88
Cylinder Pressure (psi) 1800
Certified Date 9-Feb-22

Equipment Name NOx Analyzer
Model APNA-370
Equipment ID BKK_FS0797
Model 700
Cylinder No. GN0027222
Certified By Airgas Inc.
Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.70	-0.30	-0.30	101.00	1.00	1.00
2	200.00	198.60	-1.40	-0.70	201.30	1.30	0.65
3	300.00	299.00	-1.00	-0.33	299.20	-0.80	-0.27
4	400.00	402.10	2.10	0.53	399.50	-0.50	-0.13
AVERAGE (%)				-0.14			0.27

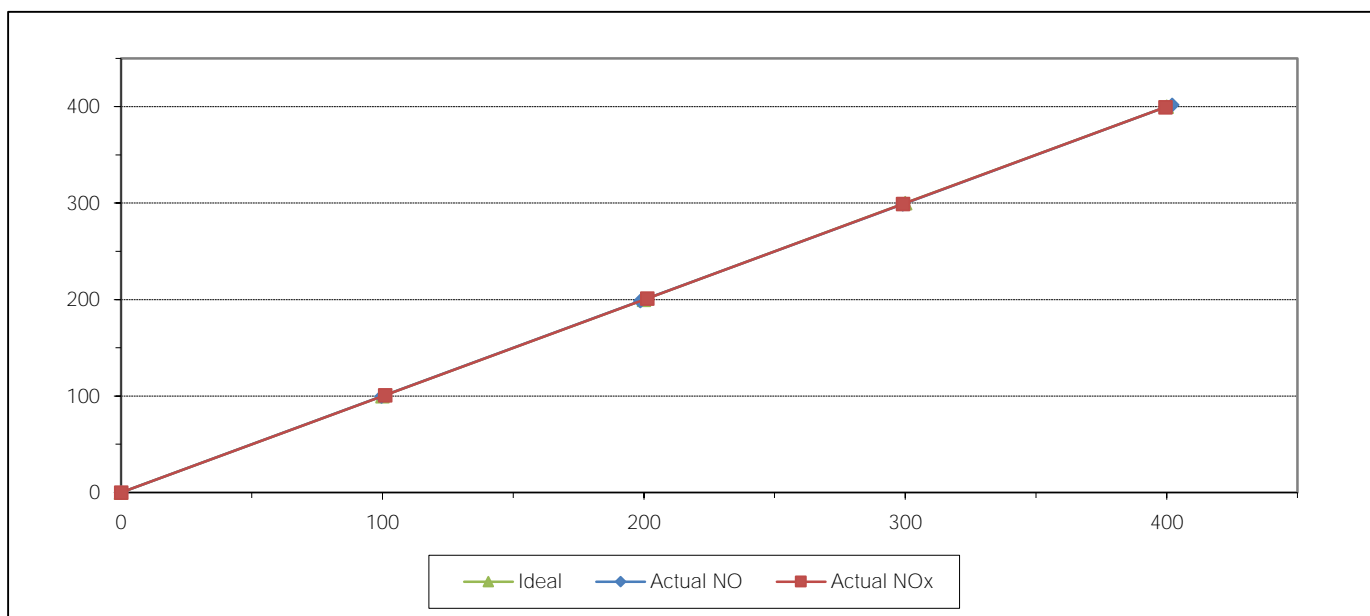

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager




MULTIPOINT CALIBRATION REPORT

Calibration Date 1-Jul-22
Manufacturer Teledyne API
Serial No. 7239
Calibrator Manufacturer Teledyne API
Serial No. 947
Std. Gas Concentration (PPM) 55.88
Cylinder Pressure (psi) 1800
Certified Date 9-Feb-22

Equipment Name NOx Analyzer
Model T200
Equipment ID RYG_FS0535
Model 700
Cylinder No. GN0027222
Certified By Airgas Inc.
Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.60	-0.40	-0.40	101.00	1.00	1.00
2	200.00	198.30	-1.70	-0.85	201.10	1.10	0.55
3	300.00	298.80	-1.20	-0.40	301.50	1.50	0.50
4	400.00	398.20	-1.80	-0.45	402.30	2.30	0.58
AVERAGE (%)				-0.40			0.55

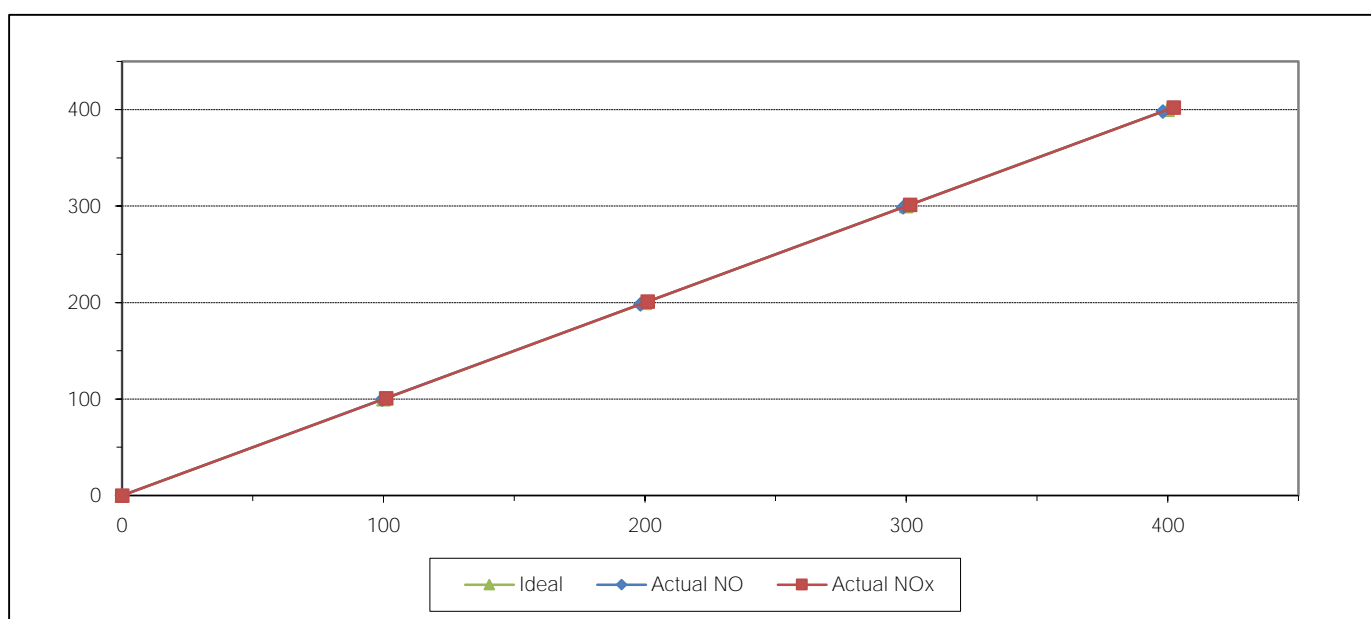

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager




MULTIPOINT CALIBRATION REPORT

Calibration Date 1-Jul-22
Manufacturer HORIBA
Serial No. NV0ER3YH
Calibrator Manufacturer Teledyne API
Serial No. 947
Std. Gas Concentration (PPM) 55.88
Cylinder Pressure (psi) 1800
Certified Date 9-Feb-22

Equipment Name NOx Analyzer
Model APNA-370
Equipment ID RYG_FS0459
Model 700
Cylinder No. GN0027222
Certified By Airgas Inc.
Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.05	0.05	0.05	0.10	0.10	0.10
1	100.00	99.50	-0.50	-0.50	101.80	1.80	1.80
2	200.00	198.70	-1.30	-0.65	199.70	-0.30	-0.15
3	300.00	301.10	1.10	0.37	301.50	1.50	0.50
4	400.00	401.30	1.30	0.33	398.90	-1.10	-0.28
AVERAGE (%)				-0.08			0.39

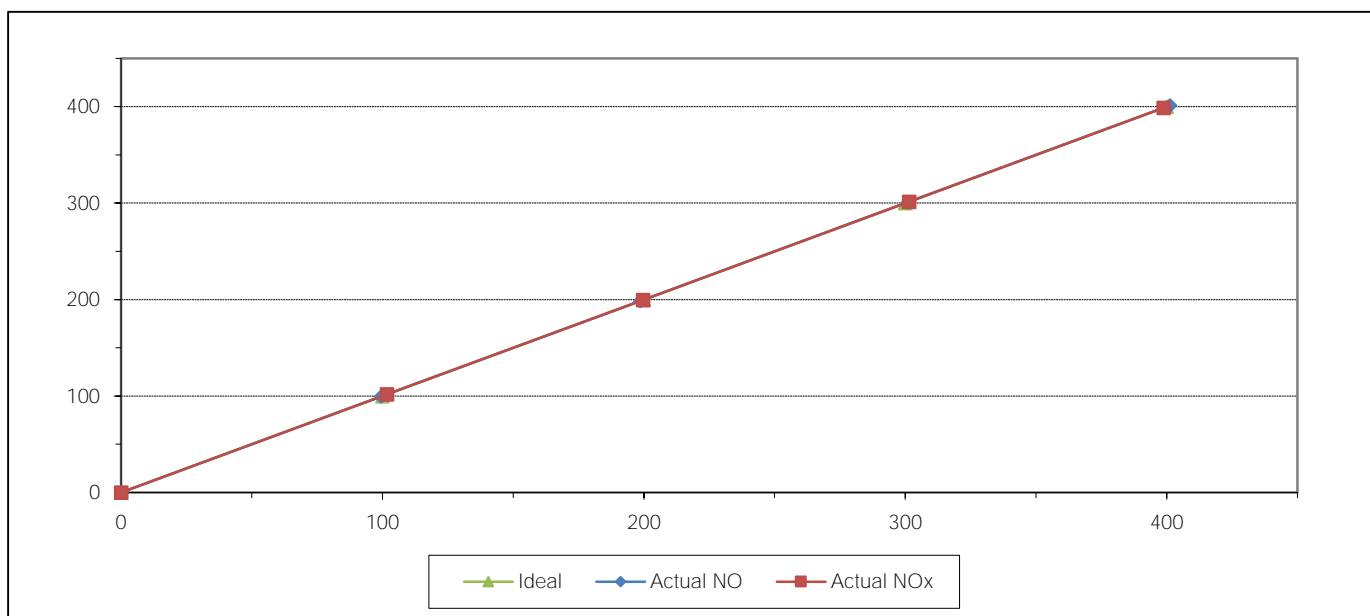

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By


(Mr.Sarayuth Jittranont)
Assistant General Manager



MULTIPOINT CALIBRATION REPORT

Calibration Date	1-Jul-22	Equipment Name	SO2 Analyzer
Manufacturer	Teledyne API	Model	T100
Serial No.	1772	Equipment ID	RYG_FS0254
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.05	0.05	0.05
1	100.00	99.10	-0.90	-0.90
2	200.00	199.50	-0.50	-0.25
3	300.00	297.50	-2.50	-0.83
4	400.00	398.80	-1.20	-0.30
AVERAGE (%)				-0.45

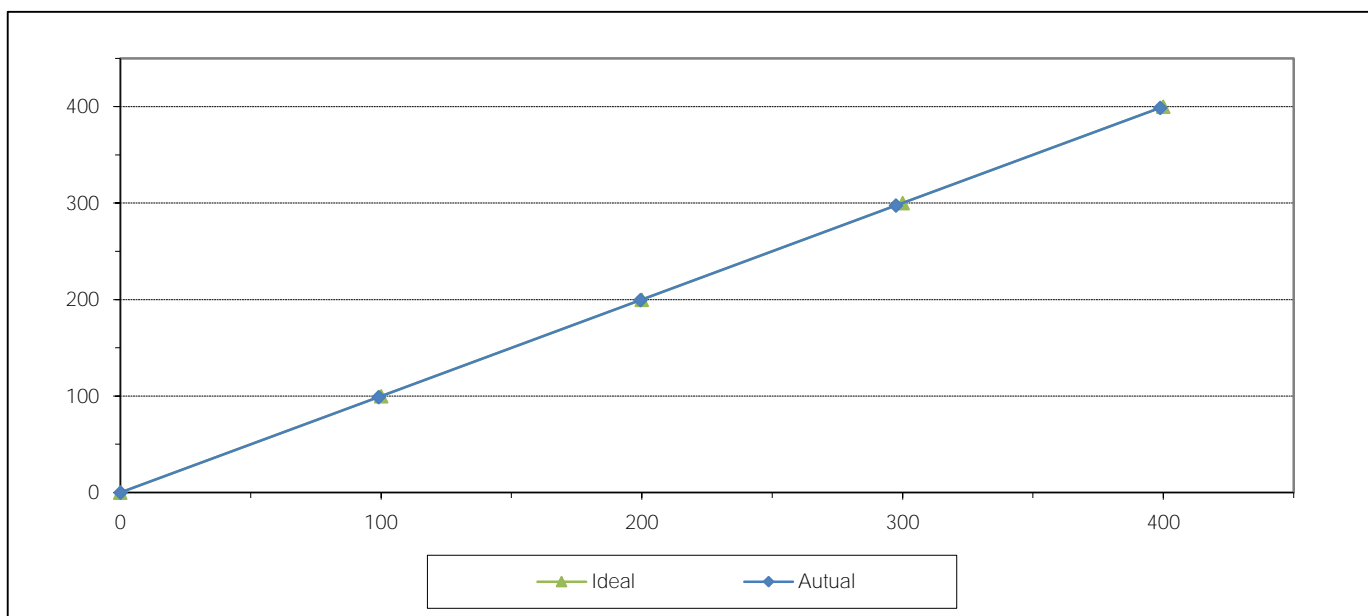

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By


(Mr.Sarayuth Jittranont)
Assistant General Manager



MULTIPOINT CALIBRATION REPORT

Calibration Date	1-Jul-21	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	G2CH436B	Equipment ID	BKK_FS0796
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	50.87	Cylinder No.	LL36633
Cylinder Pressure (psi)	1200	Certified By	Airgas Inc.
Certified Date	18-Mar-14	Expired Date	18-Mar-22

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.05	0.05	0.05
1	100.00	98.91	-1.09	-1.09
2	200.00	198.10	-1.90	-0.95
3	300.00	298.10	-1.90	-0.63
4	400.00	395.60	-4.40	-1.10
AVERAGE (%)				-0.74

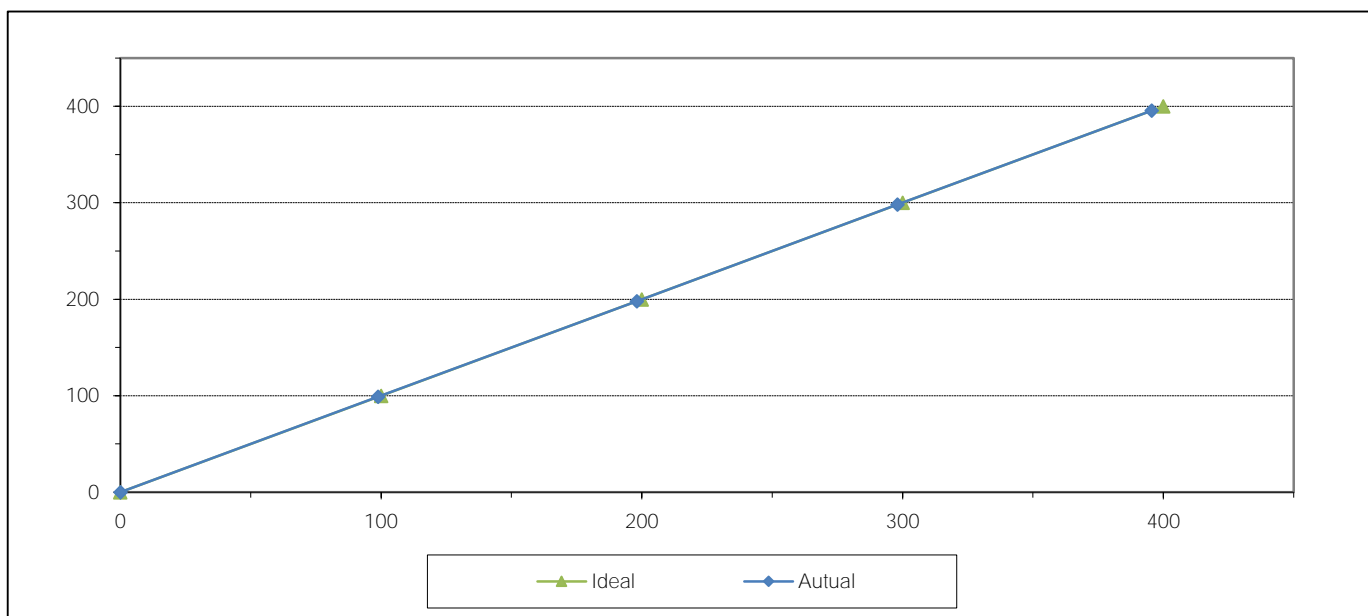

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By


(Mr.Sarayuth Jittranont)
Assistant General Manager



MULTIPOINT CALIBRATION REPORT

Calibration Date	1-Jul-22	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	NM3M2D5M	Equipment ID	RYG_FS0266
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.90	-1.10	-1.10
2	200.00	202.40	2.40	1.20
3	300.00	302.30	2.30	0.77
4	400.00	398.00	-2.00	-0.50
AVERAGE (%)				0.09

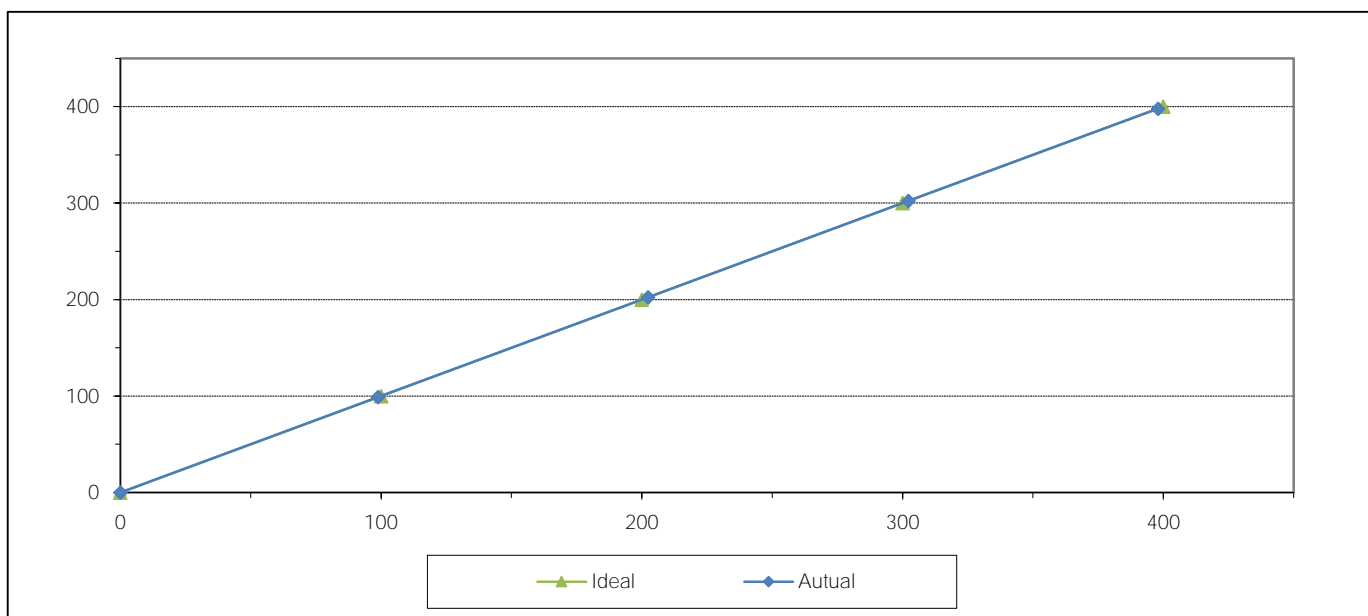

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By


(Mr.Sarayuth Jittranont)
Assistant General Manager



MULTIPOINT CALIBRATION REPORT

Calibration Date	1-Jul-22	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	PAUY0T7A	Equipment ID	RYG_FS0458
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.90	-1.10	-1.10
2	200.00	201.10	1.10	0.55
3	300.00	302.30	2.30	0.77
4	400.00	398.60	-1.40	-0.35
AVERAGE (%)				-0.01

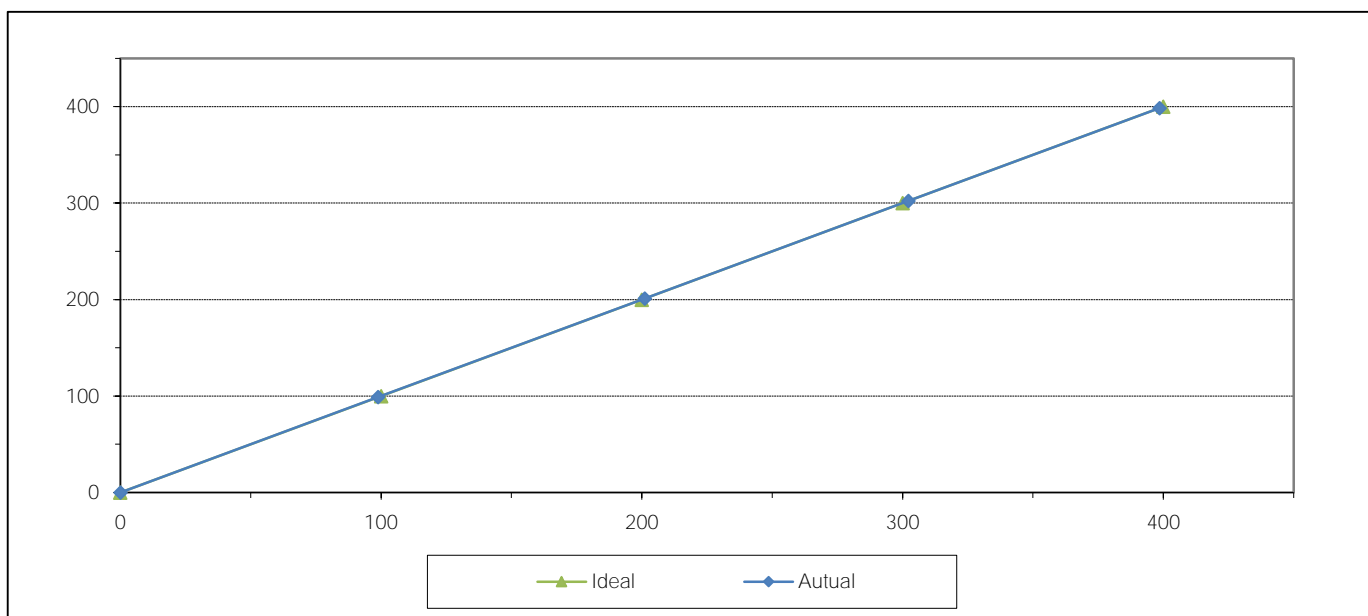

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

CERTIFICATE OF CALIBRATION

Certificate No: WS-06012022

Page 1 of 2 pages

Measurement Item	: Cup anemometer with data logger.		
Manufacturer	: Data logger: Novalynx : Cup anemometer: Novalynx		
Model/Type	: Data logger: 200-WS-25LB : Cup anemometer: WS-02F		
Serial Number	: Data logger: A5191 : Cup anemometer: -		
ID No	: Data logger: RYG_FS0328 : Cup anemometer: -		
Customer	: ALS laboratory group (Thailand) co., ltd. : 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.		
Test Conditions	: Wind tunnel cross test section area	900	cm ²
	: Anemometer frontal area	100	cm ²
	: Diameter of mounting pipe	-	mm
	: Blockage ratio of test object	0.111	[-]
Test Conditions	: Air temperature	23.9	±0.8 °C
	: Air pressure	1014.8	±0.4 hPa
	: Relative air humidity	58.9	±3.5 %RH
Calibration Procedure	Calibration was carried out base on; IEC 61400-12-1 ED.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines; M&SNET Anemometer Calibration Procedure – Version 2: 2009;		
Traceability	This calibration documents the traceable to national standard, Which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).		
Measurement Date	: JAN 28, 2022.		
Issued Date	: JAN 31, 2022.		



Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:


Mr. Parinya Booncharoen
Calibration Department Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-06012022

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V _{STD} Reading m/s	V _{UUC*} Reading m/s	Error (m/s)	Uncertainty (%)
2.078	2.0	-0.1	2.4
4.125	4.0	-0.1	1.5
6.00	5.8	-0.2	1.5
8.01	7.9	-0.1	1.0
10.00	9.8	-0.2	0.69
11.99	11.9	-0.1	0.67
14.00	13.6	-0.4	2.8
15.98	15.7	-0.3	1.2
14.99	14.8	-0.2	1.1
13.00	12.8	-0.2	1.5
11.01	10.8	-0.2	1.2
9.02	8.7	-0.3	0.90
7.02	6.7	-0.3	0.94
5.150	5.1	-0.1	1.1
2.976	3.0	0.0	2.0
1.024	0.8	-0.2	4.8

UUC*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TESTO INC.	06352145	Aug 07, 2021	MW-0034-21	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	Aug 07, 2021	MW-0034-21	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	Aug 08, 2021	MW-0035-21	0 – 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2021	CL-027-64	-30 – 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2021	RH-03032021	0 – 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2021	BP-01032021	500 – 1100 hPa
7	Wind tunnel	ESSOM	MP330D	-	-	0 – 50 Hz

End of certificate of calibration



CERTIFICATE OF CALIBRATION

Certificate No.: WD-06012022

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.
: Wind direction sensor: Novalynx.

Model/Type : Data logger: 200-WS-25LB
: Wind direction sensor: WS-02F

Serial Number : Data logger: A5191
: Wind direction sensor: -

ID No : Data logger: RYG_FS0328
: Wind direction sensor: -

Customer : ALS laboratory group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(23\pm3)^{\circ}\text{C}$, and relative humidity of $(40\pm10)\%$.

Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control, The measurement were taken at 45° intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: Q21086014, Certificate No.: KWS64/0025.

Measurement Date : JAN 26, 2022.

Issued Date : JAN 31, 2022.

Performed by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:.....



Mr. Parinya Booncharoen.
Calibration Department Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-06012022

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	0	1	1	3.0
2		45	45	45	0	3.0
3		90	90	91	1	3.0
4		135	135	134	-1	3.0
5		180	180	179	-1	3.0
6		225	225	225	0	3.0
7		270	270	272	2	3.0
8		315	315	319	4	3.0
9	Counter Clockwise	0/360	0	1	1	3.0
10		45	45	45	0	3.0
11		90	90	91	1	3.0
12		135	135	134	-1	3.0
13		180	180	179	-1	3.0
14		225	225	225	0	3.0
15		270	270	272	2	3.0
16		315	315	319	4	3.0

UUC*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No: WS-12072021

Page 1 of 2 pages

Measurement Item : Cup anemometer with data logger.

Manufacturer : Data logger: Novalynx.
: Cup anemometer: Novalynx.

Model/Type : Data logger: 200-WS-25LB.
: Cup anemometer: WS-02F.

Serial Number : Data logger: A5374.
: Cup anemometer: -.

ID No : Data logger: RYG_FS0412.
: Cup anemometer: -.

Customer : ALS laboratory group (Thailand) co., ltd.
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khel Suan Luang, Bangkok 10250
Thailand.

Test Conditions	: Wind tunnel cross test section area	900	cm ²
	: Anemometer frontal area	100	cm ²
	: Diameter of mounting pipe	-	mm
	: Blockage ratio of test object	0.111	[-]

Test Conditions	: Air temperature	23.9	±0.8 °C
	: Air pressure	1007.7	±0.4 hPa
	: Relative air humidity	57.7	±3.5 %RH

Calibration Procedure : Calibration was carried out base on;
IEC 61400-12-1 ED.1: 2005-Power Performance Measurements of Electricity Producing Wind
Turbines;
MCASNET Anemometer Calibration Procedure – Version 2: 2009;

Traceability : This calibration documents the traceable to national standard, Which realize the unit of
measurements according to the international system of units (SI) through National Institute of
Metrology Thailand (NIMT).

Measurement Date : Jul 29, 2021.

Issued Date : Jul 29, 2021.

Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:

Don

Mr. Parinya Booncharoen
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-12072021

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V _{STD} Reading m/s	V _{UUC*} Reading m/s	Error (m/s)	Uncertainty (%)
2.075	2.0	-0.1	2.5
4.150	4.1	-0.1	1.3
5.98	6.0	0.0	0.98
8.01	8.1	0.1	0.66
10.03	10.1	0.1	0.77
12.02	12.2	0.2	0.65
13.98	14.3	0.3	0.41
16.03	16.4	0.4	0.59
14.98	15.3	0.3	0.49
13.00	13.2	0.2	0.51
11.01	11.1	0.1	0.52
8.97	9.0	0.0	0.97
7.01	7.0	0.0	0.81
5.196	5.1	-0.1	0.98
2.980	3.1	0.1	1.7
1.037	0.9	-0.1	5.4

UUC*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TESTO INC.	06352145	July 16, 2020	MW-0035-20	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	July 16, 2020	MW-0035-20	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	July 20, 2020	MW-0036AA-20	0 - 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2021	CL-027-64	-30 - 70 °C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2021	RH-03032021	0 – 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2021	BP-01032021	500 – 1100 hPa
7	Wind tunnel	CSSOM	MP330D	-	-	0 – 50 Hz

End of certificate of calibration



CERTIFICATE OF CALIBRATION

Certificate No.: WD-12072021

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.
: Wind direction sensor: Novalynx.

Model/Type : Data logger: 200-WS-25LB.
: Wind direction sensor: WS-02F.

Serial Number : Data logger: A5374.
: Wind direction sensor: -.

ID No : Data logger: RYG_FSO412.
: Wind direction sensor: -.

Customer : ALS laboratory group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(23\pm3)^{\circ}\text{C}$, and relative humidity of $(40\pm10)\%$.

Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control, The measurement were taken at 45° intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: CC563-07-0045,
Certificate No.: KWS63/0044.

Measurement Date : Jul 29, 2021.

Issued Date : Jul 29, 2021.

Performed by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:.....



Mr. Parinya Booncharoen.
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-12072021

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	360	359	-1	3.0
2		45	45	42	-3	3.0
3		90	90	87	-3	3.0
4		135	135	133	-2	3.0
5		180	180	178	-2	3.0
6		225	225	226	1	3.0
7		270	270	273	3	3.0
8		315	315	318	3	3.0
9	Counter Clockwise	0/360	360	359	-1	3.0
10		45	45	42	-3	3.0
11		90	90	87	-3	3.0
12		135	135	133	-2	3.0
13		180	180	178	-2	3.0
14		225	225	226	1	3.0
15		270	270	273	3	3.0
16		315	315	318	3	3.0

UUC*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No: WS-11072021

Page 1 of 2 pages

Measurement Item : Cup anemometer with data logger.

Manufacturer : Data logger: Novalynx.
: Cup anemometer: Novalynx.

Model/Type : Data logger: 200-WS-25LB.
: Cup anemometer: WS-02F.

Serial Number : Data logger: A5369.
: Cup anemometer: -.

ID No : Data logger: RYG_FS0411.
: Cup anemometer: -.

Customer : ALS laboratory group (Thailand) co., ltd.
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

Test Conditions	: Wind tunnel cross test section area	900	cm ²
	: Anemometer frontal area	100	cm ²
	: Diameter of mounting pipe	-	mm
	: Blockage ratio of test object	0.111	[-]

Test Conditions	: Air temperature	24.3	±0.8 °C
	: Air pressure	1009.3	±0.4 hPa
	: Relative air humidity	58.5	±3.5 %RH

Calibration Procedure : Calibration was carried out base on;
IEC 61400-12-1 ED.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines;
MEASNET Anemometer Calibration Procedure - Version 2: 2009;

Traceability : This calibration documents the traceable to national standard, Which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).

Measurement Date : Jul 29, 2021.

Issued Date : Jul 29, 2021.

REVIEW BY *Marakorn P.*

APPROVED BY *[Signature]*

NEXT CAL. DATE *27/1/23*

Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:

[Signature]
Mr. Parinya Booncharoen
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-11072021

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V _{STD} Reading m/s	V _{UUC*} Reading m/s	Error (m/s)	Uncertainty (%)
2.084	1.9	-0.2	2.5
4.102	4.1	0.0	1.2
5.99	6.1	0.1	0.97
8.00	8.0	0.0	0.73
10.02	10.1	0.1	0.63
11.99	12.2	0.2	0.52
13.98	14.3	0.3	0.42
15.99	16.3	0.3	0.49
15.00	15.4	0.4	0.45
13.00	13.1	0.1	0.67
11.00	11.1	0.1	0.51
9.01	9.1	0.1	0.63
6.99	7.0	0.0	0.84
5.164	5.1	-0.1	1.1
3.001	3.0	0.0	1.9
1.032	0.8	-0.2	5.4

UUC*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	T&STO INC.	06352145	July 16, 2020	MW-0035-20	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	July 16, 2020	MW-0035-20	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	July 20, 2020	MW-0036AA-20	0 – 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2021	CL-027-64	-30 – 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2021	RH-03032021	0 – 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2021	BP-01032021	500 – 1100 hPa
7	Wind tunnel	ESSOM	MP330D	-	-	0 – 50 Hz

End of certificate of calibration



CERTIFICATE OF CALIBRATION

Certificate No.: WD-11072021

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.
: Wind direction sensor: Novalynx.

Model/Type : Data logger: 200-WS-25LB.
: Wind direction sensor: WS-02F.

Serial Number : Data logger: A5369.
: Wind direction sensor: -.

ID No : Data logger: RYG_FSO411.
: Wind direction sensor: -.

Customer : ALS laboratory group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(23 \pm 3)^{\circ}\text{C}$, and relative humidity of $(40 \pm 10)\%$.

Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control, The measurement were taken at 45° intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: CC563-07-0045,
Certificate No.: KWS63/0044.

Measurement Date : Jul 29, 2021.

Issued Date : Jul 29, 2021.

Performed by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:.....



Mr. Parinya Booncharoen.
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-11072021

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	360	359	-1	3.0
2		45	45	42	-3	3.0
3		90	90	87	-3	3.0
4		135	135	132	-3	3.0
5		180	180	180	0	3.0
6		225	225	228	3	3.0
7		270	270	273	3	3.0
8		315	315	318	3	3.0
9	Counter Clockwise	0/360	360	359	-1	3.0
10		45	45	42	-3	3.0
11		90	90	87	-3	3.0
12		135	135	132	-3	3.0
13		180	180	180	0	3.0
14		225	225	228	3	3.0
15		270	270	273	3	3.0
16		315	315	318	3	3.0

UUC*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No: WS-01062021

Page 1 of 2 pages

Measurement Item : Cup anemometer with data logger.

Manufacturer : Data logger: Novalynx.
: Cup anemometer: Novalynx.

Model/Type : Data logger: WS-25DL.
: Cup anemometer: WS-02F.

Serial Number : Data logger: A4481.
: Cup anemometer: -

ID No : Data logger: BKK_FSD141.
: Cup anemometer: -

Customer : ALS laboratory group (Thailand) co., Ltd.
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

Test Conditions : Wind tunnel cross test section area 900 cm²
: Anemometer frontal area 100 cm²
: Diameter of mounting pipe - mm
: Blockage ratio of test object 0.111 [-]

Test Conditions : Air temperature 23.7 ±0.8 °C
: Air pressure 1010.3 ±0.4 hPa
: Relative air humidity 53.7 ±3.5 %RH

Calibration Procedure Calibration was carried out base on;
IEC 61400-12-1 ED.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines;
MEASNET Anemometer Calibration Procedure – Version 2: 2009;

Traceability This calibration documents the traceable to national standard, Which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).

Measurement Date : Jun 07, 2021.
Issued Date : Jun 07, 2021.



Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory: _____

Mr. Parinya Booncharoen
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-01062021

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V _{STD} Reading m/s	V _{UUC} Reading m/s	Error (m/s)	Uncertainty (%)
2.065	2.0	-0.1	2.6
4.124	4.0	-0.1	1.2
5.99	6.0	0.0	1.01
8.00	8.0	0.0	0.74
9.99	10.1	0.1	0.60
11.96	12.2	0.2	0.67
14.02	14.4	0.4	0.45
16.03	16.6	0.6	0.36
15.01	15.3	0.3	2.8
12.99	13.3	0.3	0.41
10.99	11.2	0.2	0.53
9.01	9.3	0.3	1.2
7.05	7.0	0.0	0.77
5.121	5.0	-0.1	0.88
3.048	3.0	0.0	1.8
1.088	1.0	-0.1	5.3

UUC*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TESTO INC.	06352145	July 16, 2020	MW-0035-20	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	July 16, 2020	MW-0035-20	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	July 20, 2020	MW-0036AA-20	0 - 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2021	CL-027-64	-30 - 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2021	RH-03032021	0 – 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2021	BP-01032021	500 – 1100 hPa
7	Wind tunnel	ESSOM	MP330D	-	-	0 – 50 Hz

End of certificate of calibration



CERTIFICATE OF CALIBRATION

Certificate No.: WD-01062021

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.
: Wind direction sensor: Novalynx.

Model/Type : Data logger: WS-25DL.
: Wind direction sensor: WS-02F.

Serial Number : Data logger: A4481.
: Wind direction sensor: -

ID No : Data logger: BKK_FS0141.
: Cup anemometer: -

Customer : ALS laboratory group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(23 \pm 3)^{\circ}\text{C}$, and relative humidity of $(40 \pm 10)\%$.

Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control. The measurement were taken at 45° intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: CC563-07-0045, Certificate No.: KWS63/0044.

Measurement Date : Jun 07, 2021.
Issued Date : Jun 07, 2021.

Performed by

- ☒ Mr. Sorawit Thachalad
☐ Miss Orathai Wiwatwittaya



Approved Signatory:



Mr. Parinya Booncharoen.
Technical Support
and Calibration Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-01062021

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	0	0	0	3.0
2		45	45	42	-3	3.0
3		90	90	90	0	3.0
4		135	135	136	1	3.0
5		180	180	182	2	3.0
6		225	225	227	2	3.0
7		270	270	273	3	3.0
8		315	315	314	-1	3.0
9	Counter Clockwise	0/360	0	0	0	3.0
10		45	45	42	-3	3.0
11		90	90	90	0	3.0
12		135	135	136	1	3.0
13		180	180	182	2	3.0
14		225	225	227	2	3.0
15		270	270	273	3	3.0
16		315	315	314	-1	3.0

UUC*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor $k=2$ providing a level of confidence of approximately 95%

End of Certificate of Calibration



Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID: RYG_EN0136
Organization Name: ALS Laboratory Group (Thailand) Co Ltd.
Organization Location: 616/10 Moo 5, Tambol Mae Nam Koo, A.Pluakdaeng, Rayong, 21140, Thailand
Date: July 7, 2022 11:27:53 AM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.52, GCMS.02.52
Overall Qualification Status: Pass

REVIEW BY N. Banniy
APPROVED BY [Signature]
NEXT CAL. DATE 07/01/24

CDS Logon Verification - GC

Logon: dej.changchon

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Setpoint Status: Pass

	Setpoint	Actual
Inlet Pressure:	25.0 psi	25.1 psi
Accuracy:		0.1 psi
Agilent Recommended:		<= 1.2

Date: July 7, 2022 11:27:53 AM
System ID: RYG_EN0136

Overall Inlet Pressure Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name: 7890

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual

Temperature: 230.0 230.6 °C

Accuracy: 0.6 °C

Agilent Recommended: ≥ -1.0 % setpoint in K (-5.0 °C)
 ≤ 1.0 % setpoint in K (5.0 °C)

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual

Temperature: 100.0 99.9 °C

Accuracy: -0.1 °C

Agilent Recommended: ≥ -1.0 % setpoint in K (-3.7 °C)
 ≤ 1.0 % setpoint in K (3.7 °C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name: 7890

Setpoint Status: Pass

Setpoint/Average

Temperature: 100.0 99.91667 °C

Stability: 0.1 °C

Agilent Recommended: ≤ 0.5

Overall GC Oven Temperature Stability Test Status

Pass

Log Amp

Tested Combination1	Front	SSL	/ External	SQ
---------------------	-------	-----	------------	----

Name:	5977B			
-------	-------	--	--	--

Setpoint Status:	Pass			
------------------	------	--	--	--

Overall Log Amp Test Status

Pass

RFPA

Tested Combination1	Front	SSL	/ External	SQ
---------------------	-------	-----	------------	----

Name:	5977B			
-------	-------	--	--	--

Setpoint Status:	Pass			
------------------	------	--	--	--

Amu:	1050	m/z
------	------	-----

Drift After Five Minutes:

RFPA Voltage:

	-1	mV		479	mV
Agilent Recommended:	>=	-100	and	<=	100
				<=	1100

Overall RFPA Test Status

Pass

Tune EI

Tested Combination1	Front	SSL	/ External	SQ
---------------------	-------	-----	------------	----

Name:	5977B			
-------	-------	--	--	--

Setpoint Status:	Pass			
------------------	------	--	--	--

Filament:	1
-----------	---

Setpoint Status:	Pass			
------------------	------	--	--	--

Filament:	2
-----------	---

Overall Tune EI Test Status

Pass

Signal to Noise EI

Date:	July 7, 2022 11:27:53 AM
System ID:	RYG_EN0136

Tested Combination1

Front

SSL

/ External

SQ

Name:

5977B

Source:

EI - Extractor

Filament:

1

Setpoint Status:

Pass

Signal to Noise:

7485

Agilent Recommended:

>=

1200

Source:

EI - Extractor

Filament:

2

Setpoint Status:

Pass

Signal to Noise:

2097

Agilent Recommended:

>=

1200

This test's 2 comment(s) and 7 deviation(s) are available in the Attachments section.

Overall Signal to Noise EI Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	RYG_EN0136
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Manual Injection
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3442B
Serial Number	CN16463238
Firmware Revision	B.02.04.3
Component ID/Asset No.	081117000236
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5977B
Serial Number	US1701M008
Firmware Revision	5977 6.00.34
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std
Component ID/Asset No.	081117000236

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Extractor
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Eaknarin Puangsopa
Logged On User Name:	eaknarin_puangsopa@agilent.com
Signature Creation Date:	July 7, 2022
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Date:	July 7, 2022 11:27:53 AM
System ID:	RYG_EN0136

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 6, 2022 1:11:54 PM	Audit	SessionCreated	Session	None
July 6, 2022 1:11:54 PM	Start	Configuration	Session	None
July 6, 2022 1:11:54 PM	Audit	Entitlement	Licensing	User is Nonpaying and does not require an unlock code
July 6, 2022 1:17:19 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.52/Gc.02.52.eqp], EQP File Name: [Gc.02.52.eqp], EQP Name: [AgilentRecommended] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.52/GcMs.02.52.eqp], EQP File Name: [GcMs.02.52.eqp], EQP Name: [AgilentRecommended]
July 6, 2022 1:17:25 PM	End	Configuration	Session	None
July 6, 2022 1:17:29 PM	Start	Qualification	Session	OQ
July 6, 2022 1:17:30 PM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None
July 6, 2022 1:19:43 PM	End	Execution	CDS Logon Verification - GC : - Qualitative test	Run Count : 1
July 6, 2022 1:19:46 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 6, 2022 1:19:59 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
July 6, 2022 1:20:15 PM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
July 6, 2022 1:21:43 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
July 6, 2022 1:21:45 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
July 6, 2022 1:25:12 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
July 6, 2022 1:25:15 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
July 6, 2022 1:25:17 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
July 6, 2022 1:25:32 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
July 6, 2022 1:33:42 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry

Page 2 / 10

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 6, 2022 1:33:43 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
July 6, 2022 1:33:45 PM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
July 6, 2022 1:53:05 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
July 6, 2022 1:53:07 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
July 6, 2022 1:53:11 PM	Start	Execution	Log Amp - 5977B SQ: - Source: None EI - Extractor	
July 6, 2022 1:57:10 PM	End	Execution	Log Amp - 5977B SQ: - Source: EI EI - Extractor	Run Count : 1
July 6, 2022 1:57:24 PM	Start	Execution	RFPA - 5977B SQ: - Source: EI - Extractor	None
July 6, 2022 2:09:24 PM	End	Execution	RFPA - 5977B SQ: - Source: EI - Extractor	Run Count : 1
July 6, 2022 2:09:28 PM	Start	Execution	Tune EI - 5977B SQ: - Source: - None EI - Extractor Filament 1 (Qualitative - No setpoints associated)	
July 6, 2022 2:24:46 PM	End	Qualification	Session	OQ
July 6, 2022 2:24:46 PM	Start	Reporting	Session	None
July 6, 2022 2:41:39 PM	End	Reporting	Session	None
July 6, 2022 2:41:39 PM	Start	Configuration	Session	None
July 6, 2022 2:41:40 PM	End	Configuration	Session	None

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 6, 2022 2:41:40 PM	Start	Qualification	Session	OQ
July 6, 2022 2:41:40 PM	Start	Execution	Tune EI - 5977B SQ: - Source: - None EI - Extractor Filament 1 (Qualitative - No setpoints associated)	
July 6, 2022 2:41:56 PM	End	Execution	Tune EI - 5977B SQ: - Source: - Run Count : 1 EI - Extractor Filament 1 (Qualitative - No setpoints associated)	
July 6, 2022 2:41:58 PM	Start	Execution	Tune EI - 5977B SQ: - Source: - None EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
July 6, 2022 2:42:48 PM	End	Qualification	Session	OQ
July 6, 2022 2:42:48 PM	Start	Reporting	Session	None
July 6, 2022 2:50:52 PM	End	Reporting	Session	None
July 6, 2022 2:50:52 PM	Start	Qualification	Session	OQ
July 6, 2022 2:50:52 PM	Start	Execution	Tune EI - 5977B SQ: - Source: - None EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
July 6, 2022 2:51:12 PM	End	Qualification	Session	OQ
July 6, 2022 2:51:12 PM	Start	Reporting	Session	None
July 6, 2022 2:55:29 PM	End	Reporting	Session	None
July 6, 2022 2:55:29 PM	Start	Qualification	Session	OQ
July 6, 2022 2:55:29 PM	Start	Execution	Tune EI - 5977B SQ: - Source: - None EI - Extractor Filament 2 (Qualitative - No setpoints associated)	

User Name: eaknarin_puangsoapa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 6, 2022 2:55:40 PM	End	Execution	Tune EI - 5977B SQ: - Source: - Run Count : 1 EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
July 6, 2022 2:55:45 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 6, 2022 3:21:52 PM	End	Qualification	Session	QQ
July 6, 2022 3:21:52 PM	Start	Reporting	Session	None
July 6, 2022 3:25:04 PM	End	Reporting	Session	None
July 6, 2022 3:25:04 PM	Start	Qualification	Session	QQ
July 6, 2022 3:25:04 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 6, 2022 4:06:40 PM	Audit	AceClosed	Session	None
July 7, 2022 9:13:47 AM	Audit	AceRestarted	Session	None
July 7, 2022 9:13:49 AM	Audit	SessionReloaded	Session	None
July 7, 2022 9:13:54 AM	Start	Qualification	Session	QQ
July 7, 2022 9:13:54 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 7, 2022 9:58:06 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2022\OQF_SN_F01.D

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 7, 2022 9:59:53 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 1
July 7, 2022 10:01:46 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 1
July 7, 2022 10:01:46 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 7, 2022 10:02:00 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F01.D
July 7, 2022 10:04:55 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 2
July 7, 2022 10:07:30 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 2
July 7, 2022 10:07:30 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 7, 2022 10:07:44 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F01.D

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 7, 2022 10:08:18 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 3
July 7, 2022 10:10:28 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 3
July 7, 2022 10:10:28 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 7, 2022 10:10:55 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F01.D
July 7, 2022 10:14:03 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 4
July 7, 2022 10:14:54 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 4
July 7, 2022 10:14:54 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 7, 2022 10:15:15 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F01.D

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 7, 2022 10:15:27 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 5
July 7, 2022 10:16:48 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 5
July 7, 2022 10:16:48 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 7, 2022 10:17:05 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F01.D
July 7, 2022 10:17:14 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 6
July 7, 2022 10:18:40 AM	End	Qualification	Session	OQ
July 7, 2022 10:18:40 AM	Start	Reporting	Session	None
July 7, 2022 10:21:10 AM	End	Reporting	Session	None
July 7, 2022 10:21:10 AM	Start	Qualification	Session	OQ
July 7, 2022 10:21:17 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
July 7, 2022 10:56:49 AM	End	Qualification	Session	OQ
July 7, 2022 10:56:49 AM	Start	Reporting	Session	None
July 7, 2022 10:57:38 AM	End	Reporting	Session	None

Page 8 / 10

Date: July 7, 2022 11:27:53 AM
 System ID: RYG_EN0136

User Name: eaknarin_puangsoa

System id: RYG_EN0136

Hostname: ASRYGW7002

Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 7, 2022 10:57:38 AM	Start	Qualification	Session	OQ
July 7, 2022 10:57:38 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
July 7, 2022 11:06:50 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F021.D
July 7, 2022 11:11:47 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
July 7, 2022 11:13:13 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 1
July 7, 2022 11:14:29 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 1
July 7, 2022 11:14:29 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
July 7, 2022 11:14:47 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F021.D
July 7, 2022 11:16:34 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 2

User Name: eaknarin_puangsoa

System Id: RYG_EN0136

Hostname: ASRYGW7002

Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 7, 2022 11:19:56 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 2
July 7, 2022 11:19:56 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
July 7, 2022 11:20:13 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F021.D
July 7, 2022 11:21:52 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 3
July 7, 2022 11:22:49 AM	End	Qualification	Session	OQ
July 7, 2022 11:22:49 AM	Start	Reporting	Session	None
July 7, 2022 11:26:46 AM	Audit	Reporting	Session	Report Generated : Certificate



CONSOLE CONTROL UNIT CALIBRATION TEST REPORT

Calibration of Date : 12 Jul 22
Next Cal. Date : 12 Jan 23

Barometric Pressure (mm.Hg) : 755
Relative Humidity (%) : 70.0
Temperature (°C) : 30.0

Console Control Meter Data

Calibration No. : C-120722-BKK_FS0468
Dry Gas Meter No. : BKK_FS0468
Console Serial No. : 1302005
Console Model No. : XC-572-V

Reference Dry Gas Meter Data

Serial No. : 1607009
Model No. : SK25EXSR-QC6
Correction Factor (Yr) : 1.0060
Next Calibration Date : 7 Oct 22

ΔH (mm.H ₂ O)	\ominus Minutes	Reference Dry Gas Meter Calibration				Console Control ; Drygas Meter						Dry Gas Meter Correction Factor (Y)	Orifice Calibration Factor $\Delta H@$
		Vr (Liters)			Tr (°C)	Vm (Liters)			Ti (°C)	To (°C)	Avg.Tm (°C)		
		Final	Initial	Total		Final	Initial	Total					
15	12.80	150.00	0.00	150.00	31.0	344.0	191.0	153.00	30.0	30.0	30.0	0.9816	50.7881
25	9.60	150.00	0.00	150.00	31.0	511.4	358.0	153.40	30.0	30.0	30.0	0.9781	47.6138
50	6.68	150.00	0.00	150.00	31.0	673.4	520.0	153.40	31.0	31.0	31.0	0.9789	45.9560
100	4.62	150.00	0.00	150.00	32.0	842.0	689.0	153.00	31.0	31.0	31.0	0.9736	44.2543
150	3.77	150.00	0.00	150.00	32.0	1005.5	853.0	152.45	32.0	32.0	32.0	0.9756	44.0575
											Avg.	0.9776	46.5339

Y : Ratio of reading of reference to dry gas meter : tolerance for individual values ± 0.02 from average .

$\Delta H@$: Orifice pressure differential that equates to 21.24 lm of air @ 25 C and 760 mm of mercury , mmH₂O ; tolerance for individual values ± 5.08 from average .

Procedure; 40 CFR 60,APP A,METH ,SEC 5.3 & 7

Calibrated by:

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by:

Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)



DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date : 12-Jul-22	Ambient Temperature (°C) : 30
Calibration sheet No. : C-120722-BKK_FS0469	Relative Humidity (%) : 70
Digital Temperature ID BKK_FS0469	Reference Temperature ID BKK_FS0609
Serial No. : 1302005	Serial No. : 7688004
Model : XC-572-V	Model : FLUKE 714
	Next Calibrate : 26 Jul 23

Location	Reference Temperature °C	Digital Temperature °C	Error °C	Remark
Stack	0	0	0	
	25	24	-1	
	50	49	-1	
	100	98	-2	
	150	148	-2	
	200	197	-3	
	250	247	-3	
	300	297	-3	
	500	497	-3	
	1000	997	-3	
	1200	1197	-3	
Probe	100	99	-1	
	125	124	-1	
	150	149	-1	
Oven	100	99	-1	
	125	124	-1	
	150	149	-1	
Filter	100	100	0	
	125	125	0	
	150	149	-1	
Exit	0	0	0	
	10	11	1	
	20	21	1	
Meter	0	0	0	
	25	25	0	
	50	50	0	
AUX	0	0	0	
	25	25	0	
	50	50	0	

Calibrated by : Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by : Natthapol Jiengwareewong

(Mr.Natthapol Jiengwareewong)

Manager



Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK_FS0472 Calibration Date : 12 Jul 22
 Lab test duct Number : 258-1-13-01 Standard Pitot ID : BKK_FS0441
 Calibration Sheet No. : C-120722-BKK_FS0472 Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube (ΔP , mm.H ₂ O)	Type s pitot tube (ΔP , mm.H ₂ O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			\bar{C}_p	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P_{(std)}}{\Delta P_{(s)}}}$$

$$\bar{C}_{p(A)} - \bar{C}_{p(B)} \text{ must BE } \leq 0.01$$

$$\text{Average deviation(A or B)} = \frac{\sum_i [Cp_{(s)} - Cp(A \text{ or } B)]}{3} \text{ must BE } \leq 0.01$$

Calibrated by

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by

Nattapon Jengwareewong

(Mr.Nattapol Jengwareewong)

Field Specialist(1)



Pitot Tube Calibration Data

Pitot Tube Identification Number : BKK_FS0473 Calibration Date : 12 Jul 22
 Lab test duct Number : 258-1-13-01 Standard Pitot ID : BKK_FS0441
 Calibration Sheet No. : C-120722-BKK_FS0473 Cp Standard : 0.99

Type S Pitot Tube Coefficient Data					
	Type s pitot tube Leg A,B	Standard pitot tube (ΔP , mm.H ₂ O)	Type s pitot tube (ΔP , mm.H ₂ O)	Cp (s) Leg A	Cp (s) Leg B
Test 1	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 2	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
Test 3	A	12.00	16.60	0.842	-
	B	12.00	16.60	-	0.842
			\bar{C}_p	0.842	0.842

$$Cp(S) = Cp_{(std)} \sqrt{\frac{\Delta P(std)}{\Delta P(s)}}$$

$$\bar{C}_{p(A)} - \bar{C}_{p(B)} \Big] must BE \leq 0.01$$

$$Average\ deviation(A\ or\ B) = \frac{\sum_i [Cp(s) - Cp(A\ or\ B)]}{3} must\ BE \leq 0.01$$

Calibrated by

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by

Natthapol Jiengwareewong

(Mr.Natthapol Jiengwareewong)

Field Specialist(1)



PROBE NOZZLE DIAMETER
CALIBRATION DATA SHEET

Calibration Date	12 Jul 22	Nozzle Set ID. :	BKK_FS0474
Calibration Sheet No. :	C-120722-BKK_FS0474	Vernier Caliper ID. :	BKK_FS0626


Nozzle ID #	Nozzle Diameter (cm.)			Hi - Lo	$(D_1 + D_2 + D_3) / 3$
	D_1	D_2	D_3	ΔD	D_{avg}
1	0.300	0.300	0.300	0.000	0.300
2	0.450	0.450	0.450	0.000	0.450
3	0.600	0.600	0.600	0.000	0.600
4	0.780	0.780	0.780	0.000	0.780
5	0.932	0.932	0.932	0.000	0.932
6	1.094	1.094	1.094	0.000	1.094
7	1.264	1.264	1.264	0.000	1.264

Where :

D_1, D_2, D_3 = There different nozzle diameters at 60 degrees to each other, each measured the nearest 0.025 mm.

ΔD = Maximum distance between any two diameters, must be ≤ 0.100 mm.

D_{avg} = $(D_1 + D_2 + D_3) / 3$

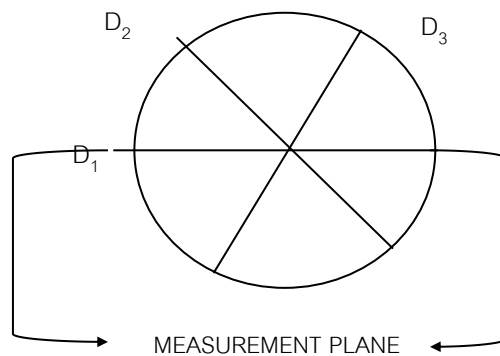

Calibrated by

Saksit Phaisanphisut

(Mr.Saksit Phaisanphisut)

Field Scientist (4)

Approved by

Nattapol Jiengwareewong

(Mr.Nattapol Jiengwareewong)

Field Specialist(1)

Certificate No: G 650023

Date of issue : 21-Jan-22

Instrument description : Flue gas Analyzer
Instrument model : Testo 340
Instrument serial no. : 62150585
ID no. or control no. : RYG_FS0465
Manufacturer : testo SE
Probe description : -
Probe model : -
Probe serial : -
Customer name : ALS LABORATORY GROUP (THAILAND) CO.,LTD.
Customer address : 104 Phatthanakan 40, Phatthanakan Road, Khwaeng Phatthanakan, Khet Suan Luang, Bangkok, 10250 Thailand
Total pages of certificate : 3 Pages
Receiving no. : L-220082
Receiving date. : 14-Jan-22
Parameter of calibration : Gas Calibration(Oxygen 2.501,10.00,21.00 %vol, Carbon Monoxide 80.97,309.9,1003 ppm, Nitric Oxide 10.08,150.9,320.6 ppm, Sulphur Dioxide 50.04,100.9,601.1 ppm)
Condition of UUC. : Used
Ambient condition : All of the Measurement were carried out the stabilized laboratory
Temperature : 23 ± 5 °C
Humidity : 55 ± 15 %RH
Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210
Calibration procedure no. : WI-CL-28-C

REVIEW BY	<i>Narakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	19/1/23

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement Multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test Environmental condition.

This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid.

This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 19-Jan-22



Mr. Sedtawut Nueathong

Calibration Technician



Mrs. Nongluck Wongsettee

Technical Manager

Certificate No.: G 650023

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O ₂) 2.501 % Vol	2431/19	Linde	16-Jul-23
Oxygen (O ₂) 10.00 % Vol	2453/19	Linde	18-Jul-23
Oxygen (O ₂) 21.00 % Vol	2426/19	Linde	16-Jul-23
Carbon monoxide (CO) 80.97 ppm	2842/21	Linde	24-Jun-23
Carbon monoxide (CO) 309.9 ppm	2803/21	Linde	22-Jun-23
Carbon monoxide (CO) 1003 ppm	2829/21	Linde	23-Apr-23
Nitric Oxide (NO) 10.08 ppm	3241/21	Linde	25-Jul-23
Nitric Oxide (NO) 150.9 ppm	2857/21	Linde	27-Jun-23
Nitric Oxide (NO) 320.6 ppm	2944/21	Linde	2 Jul 23
Sulphur Dioxide (SO ₂) 50.04 ppm	3205/21	Linde	25-Jul-23
Sulphur Dioxide (SO ₂) 100.9 ppm	4942/20	Linde	20-Nov-22
Sulphur Dioxide (SO ₂) 601.1 ppm	3204/21	Linde	20-Jul-23

Measured room conditions

Temperature : 22.5 °C Humidity : 56.2 %RH Pressure : 1018.3 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 600 ml/min Gas pressure : 1021.9 mbar

Calibration Results Before Adjustment (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.501	2.47	-0.031	0.20
O ₂ (%Vol)	10.00	9.89	-0.11	0.40
O ₂ (%Vol)	21.00	21.12	0.12	0.80
CO (ppm)	80.97	83	2.03	2.8
CO (ppm)	309.9	314	4.1	11
CO (ppm)	1003	1016	13	34
NO (ppm)	10.08	8	-2.08	3.0
NO (ppm)	150.9	162	11.1	5.0
NO (ppm)	320.6	345	24.4	10
SO ₂ (ppm)	50.04	38	-12.04	5.0
SO ₂ (ppm)	100.9	92	-8.9	5.0
SO ₂ (ppm)	601.1	593	-8.1	14

Calibration Results After Adjustment (Table 3)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.501	2.47	-0.031	0.20
O ₂ (%Vol)	10.00	9.89	-0.11	0.40
O ₂ (%Vol)	21.00	21.11	0.12	0.80
CO (ppm)	80.97	83	2.03	2.8
CO (ppm)	309.9	314	4.1	11
CO (ppm)	1003	1016	13	34
NO (ppm)	10.08	9	-1.08	3.0
NO (ppm)	150.90	150	-0.9	5.0
NO (ppm)	320.6	318	-2.6	10
SO ₂ (ppm)	50.04	48	-2.04	5.0
SO ₂ (ppm)	100.9	101	0.1	5.0
SO ₂ (ppm)	601.1	604	2.9	14

Remark : 1 cmol/mol = 1 %vol. , 1 μmol/mol = 1 ppm.

End of Report



ROTA METER CALIBRATION RESULT OCTOBER 2022

Rotameter ID.	Calibration Date	Regression Result	Coefficient (R ²)
BKK_FS0577	01 Oct 22	$Y = 1.0202x + 0.1976$	1.0000
BKK_FS0579	01 Oct 22	$Y = 1.0078x + 0.4789$	0.9998
BKK_FS0583	01 Oct 22	$Y = 1.016x + 0.3922$	1.0000
BKK_FS0584	01 Oct 22	$Y = 1.0036x + 2.2262$	0.9997
BKK_FS0585	01 Oct 22	$Y = 1.0189x - 5.6476$	0.9997
BKK_FS0586	01 Oct 22	$Y = 1.0095x - 1.1524$	0.9995
BKK_FS0587	01 Oct 22	$Y = 1.013x - 3.6619$	0.9996
BKK_FS0588	01 Oct 22	$Y = 1.0154x + 4.8357$	0.9999
BKK_FS0589	01 Oct 22	$Y = 0.9918x + 4.8069$	0.9999
BKK_FS0590	01 Oct 22	$Y = 1.0038x - 0.4857$	0.9996
BKK_FS0591	01 Oct 22	$Y = 0.9705x - 52.174$	0.9986
BKK_FS0592	01 Oct 22	$Y = 0.9646x - 37.642$	0.9985
BKK_FS0593	01 Oct 22	$Y = 0.9767x - 58.445$	0.9988
BKK_FS0594	01 Oct 22	$Y = 0.9902x - 62.87$	0.9999
BKK_FS0595	01 Oct 22	$Y = 1.0249x - 98.162$	0.9999
BKK_FS0596	01 Oct 22	$Y = 0.9843x - 26.806$	0.9991
BKK_FS0597	01 Oct 22	$Y = 0.9802x - 61.653$	0.9978
BKK_FS1004	01 Oct 22	$Y = 0.9762x + 11.724$	0.9998
BKK_FS1005	01 Oct 22	$Y = 1.0081x + 1.5143$	1.0000
BKK_FS1006	01 Oct 22	$Y = 1.098x - 2.9327$	0.9999
BKK_FS1007	01 Oct 22	$Y = 0.9917x + 1.6592$	1.0000
BKK_FS1008	01 Oct 22	$Y = 1.0132x + 0.7207$	1.0000
BKK_FS1009	01 Oct 22	$Y = 1.0132x + 1.1633$	0.9960
BKK_FS1010	01 Oct 22	$Y = 1.0033x + 0.5758$	0.9999
BKK_FS1011	01 Oct 22	$Y = 1.0234x + 0.1759$	0.9996
BKK_FS1012	01 Oct 22	$Y = 1.0106x - 2.0048$	0.9997
BKK_FS1013	01 Oct 22	$Y = 0.9677x - 35.851$	0.9997
BKK_FS1014	01 Oct 22	$Y = 1.0021x + 0.3148$	0.9998
BKK_FS1015	01 Oct 22	$Y = 0.9994x + 1.786$	1.0000
BKK_FS1016	01 Oct 22	$Y = 1.0105x - 80.256$	0.9998
BKK_FS1017	01 Oct 22	$Y = 0.9995x + 0.649$	1.0000
BKK_FS1018	01 Oct 22	$Y = 1.0011x + 1.1786$	1.0000
BKK_FS1019	01 Oct 22	$Y = 1.0023x - 68.424$	0.9996
BKK_FS1020	01 Oct 22	$Y = 1.0547x - 0.666$	0.9998
BKK_FS1021	01 Oct 22	$Y = 1.018x - 3.3286$	0.9998
BKK_FS1022	01 Oct 22	$Y = 0.9932x - 57.035$	0.9986
BKK_FS1023	01 Oct 22	$Y = 1.0094x + 0.0717$	0.9999
BKK_FS1024	01 Oct 22	$Y = 1.0042x + 0.4086$	0.9997
BKK_FS1025	01 Oct 22	$Y = 1.0132x - 88.507$	0.9996



ROTA METER CALIBRATION RESULT OCTOBER 2022

Rotameter ID.	Calibration Date	Regression Result	Coefficient (R ²)
BKK_FS1026	01 Oct 22	$Y = 1.0018x + 1.0776$	0.9997
BKK_FS1027	01 Oct 22	$Y = 1.0053x + 0.231$	0.9995
BKK_FS1028	01 Oct 22	$Y = 0.9792x - 60.312$	0.9982
BKK_FS1029	01 Oct 22	$Y = 0.9935x + 0.8234$	1.0000
BKK_FS1030	01 Oct 22	$Y = 1.0039x + 0.515$	0.9999
BKK_FS1031	01 Oct 22	$Y = 1.009x - 79.295$	0.9998
BKK_FS1039	01 Oct 22	$Y = 0.9967x + 4.5048$	0.9999
BKK_FS1040	01 Oct 22	$Y = 0.9936x + 32.694$	0.9998
BKK_FS1041	01 Oct 22	$Y = 1.067x - 1.999$	1.0000
BKK_FS1042	01 Oct 22	$Y = 1.0019x + 2.1571$	1.0000
BKK_FS1043	01 Oct 22	$Y = 1.1569x - 96.479$	0.8412
BKK_FS1044	01 Oct 22	$Y = 1.0318x - 0.9374$	0.9999
BKK_FS1161	01 Oct 22	$Y = 1.0126x + 0.7738$	0.9999
BKK_FS1162	01 Oct 22	$Y = 0.9994x + 2.6357$	0.9995
BKK_FS1163	01 Oct 22	$Y = 0.977x - 55.03$	0.9987
BKK_FS1164	01 Oct 22	$Y = 0.9914x + 0.8427$	0.9997
BKK_FS1165	01 Oct 22	$Y = 0.9893x + 6.5919$	0.9998
BKK_FS1166	01 Oct 22	$Y = 1.0031x - 77.881$	0.9996
BKK_FS1200	01 Oct 22	$Y = 1.0313x - 0.4602$	0.9995
BKK_FS1201	01 Oct 22	$Y = 1.0045x + 0.15$	0.9996
BKK_FS1202	01 Oct 22	$Y = 0.9702x - 44.156$	0.9994
RYG_FS0197	01 Oct 22	$Y = 1.0039x - 0.179$	0.9999
RYG_FS0198	01 Oct 22	$Y = 0.9964x + 21.757$	1.0000
RYG_FS0199	01 Oct 22	$Y = 1.0577x - 1.7486$	1.0000

Review By :

(Mr. Wichan Choonharat)

Enviro Field Services Manager

Approved By :

(Mr. Sarayuth Jittranont)

Assistant General Manager

Certificate of System Qualification

GC-OQ + GCMS-OQ

REVIEW BY	Sarat M.
APPROVED BY	Ch
NEXT CAL. DATE	1 April 23

System ID: GM-2
Organization Name: ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location: 104 Phatthanakan 40, Phattanakan Rd., Kheiwang Suan Luang, Khet Suan Luang, Bangkok 10250
Date: October 1, 2021 1:10:17 PM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.51, GCMS.02.51
Overall Qualification Status: Pass

System Inspection and Basic Safety and Operation

Name: 7890
Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890
Front MMI
Setpoint Status: Pass

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	24.9	psi
Accuracy:			0.1	psi
Agilent Recommended:			<= 1.2	

Overall Inlet Pressure Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name: 7890

Date: October 1, 2021 1:10:17 PM
System ID: GM-2

Setpoint Status:	Pass			
Zone:	Oven			
	Setpoint/Actual			
Temperature:	230.0	230.5	°C	
Accuracy:		0.5	°C	
Agilent Recommended:	>=	-1.0	% setpoint in K	(-5.0 °C)
	<=	1.0	% setpoint in K	(5.0 °C)

Setpoint Status:	Pass			
Zone:	Oven			
	Setpoint/Actual			
Temperature:	100.0	101.5	°C	
Accuracy:		1.5	°C	
Agilent Recommended:	>=	-1.0	% setpoint in K	(-3.7 °C)
	<=	1.0	% setpoint in K	(3.7 °C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:	7890			
Setpoint Status:	Pass			
	Setpoint/Average			
Temperature:	100.0	101.5	°C	
Stability:		0.0	°C	
Agilent Recommended:	<=	0.5		

Overall GC Oven Temperature Stability Test Status

Pass

Log Amp

Tested Combination1	Front	MMI	/ External	SQ
Name:	5975C inert XL with TAD			
Setpoint Status:	Pass			

Overall Log Amp Test Status

Pass

RFPA

Tested Combination1

Front

MMI

/ External

SQ

Name:

5975C inert XL with TAD

Setpoint Status:

Pass

Amu:

1050

m/z

Drift After Five Minutes:

6

mV

RFPA Voltage:

461

mV

Agilent Recommended:

>=

-100

and

<=

100

<=

1100

Overall RFPA Test Status

Pass

Tune EI

Tested Combination1

Front

MMI

/ External

SQ

Name:

5975C inert XL with TAD

Setpoint Status:

Pass

Filament:

1

Setpoint Status:

Pass

Filament:

2

Overall Tune EI Test Status

Pass

Scouting Run

Tested Combination1

Front

MMI

/ External

SQ

Injection Tower

Name:

7693A

Source:

EI - Inert

Date:

October 1, 2021 1:10:17 PM

System ID:

GM-2

Setpoint Status:

Completed

Injection Volume on Column:

1.0 uL

Overall Scouting Run Status

Completed

Signal to Noise EI

Tested Combination1

Front

MMI

/ External

SQ

Name:

5975C Inert XL with TAD

Source:

EI - Inert

Filament:

1

Setpoint Status:

Pass

Signal to Noise:

619

Agilent Recommended:

>=

320

Source:

EI - Inert

Filament:

2

Setpoint Status:

Pass

Signal to Noise:

647

Agilent Recommended:

>=

320

Overall Signal to Noise EI Test Status

Pass

Injection Precision

Tested Combination1

Front

MMI

/ External

SQ

Name:

7693A

Source:

EI - Inert

Setpoint Status:

Pass

Injection Volume on Column:

1.0 uL

Area RSD:

4.75

%

Retention Time RSD:

0.02

%

Agilent Recommended:

<=

5.00

<=

1.00

Overall Injection Precision Test Status

Pass

Date:

October 1, 2021 1:10:17 PM

System ID:

GM-2

Mass Ratio Precision

Tested Combination1	Front	MMI	/ External	SQ
Injection Tower				
Name:	7693A			
Source:	EI - Inert			
Setpoint Status:	Pass			
Injection Volume on Column:	1.0 uL			
	Area Mass 1		Mass Ratio	
	Abundance*s			
RSD:	4.75 %		0.81 %	
Agilent Recommended:	<= 5.00		<= 5.00	
	Pass		Pass	

Overall Mass Ratio Precision Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GM-2
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN10120123
Firmware Revision	A.10.08
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN10060099
Firmware Revision	A.10.16
Vial Heater	Not installed

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN10141049
Firmware Revision	A.01.16
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	MMI
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5975C inert XL with TAD
Serial Number	US10153217
Firmware Revision	5.02.12
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Inert
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Supasak Nimsongtham
Logged On User Name:	supasak.nimsongtham@agilent.com
Signature Creation Date:	October 1, 2021
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: supasak.nimsongtham
 Hostname: 5CG1115HKC

System id: GM-2
 Print Date: October 1, 2021 1:10:19 PM

ALS_GM2 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 1, 2021 12:42:37 PM	Audit	SessionCreated	Session	None
October 1, 2021 12:42:37 PM	Start	Configuration	Session	None
October 1, 2021 12:42:37 PM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
October 1, 2021 12:44:21 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.51/Gc.02.51.eqp], EQP File Name: [Gc.02.51.eqp], EQP Name: [AgilentRecommended] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.51/GcMs.02.51.eqp], EQP File Name: [GcMs.02.51.eqp], EOP Name: [AgilentRecommended]
October 1, 2021 12:44:24 PM	End	Configuration	Session	None
October 1, 2021 12:44:28 PM	Start	Qualification	Session	OQ
October 1, 2021 12:44:28 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None

Page 1 / 7

User Name: supasak.nimsongtham
 Hostname: 5CG1115HKC

System Id: GM-2
 Print Date: October 1, 2021 1:10:19 PM

ALS_GM2 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 1, 2021 12:47:35 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
October 1, 2021 12:47:37 PM	Start	Execution	Inlet Pressure Accuracy - Front MMf: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
October 1, 2021 12:47:42 PM	End	Execution	Inlet Pressure Accuracy - Front MMf: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
October 1, 2021 12:47:44 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 1, 2021 12:48:04 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
October 1, 2021 12:48:05 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
October 1, 2021 12:48:07 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 1, 2021 12:48:34 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
October 1, 2021 12:48:36 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1

Page 2 / 7

User Name: supasak.nimsongtham
 Hostname: 5CG1115HKC

System id: GM-2
 Print Date: October 1, 2021 1:10:19 PM

ALS_GM2 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 1, 2021 12:48:38 PM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
October 1, 2021 12:49:34 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
October 1, 2021 12:49:36 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
October 1, 2021 12:49:37 PM	Start	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Inert	None
October 1, 2021 12:49:47 PM	End	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Inert	Run Count : 1
October 1, 2021 12:49:48 PM	Start	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Inert	None
October 1, 2021 12:50:23 PM	End	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Inert	Run Count : 1
October 1, 2021 12:50:25 PM	Start	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Inert Filament 1 (Qualitative - No setpoints associated)	None
October 1, 2021 12:50:49 PM	End	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Inert Filament 1 (Qualitative - No setpoints associated)	Run Count : 1
October 1, 2021 12:50:50 PM	Start	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Inert Filament 2 (Qualitative - No setpoints associated)	None
October 1, 2021 12:50:59 PM	End	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Inert Filament 2 (Qualitative - No setpoints associated)	Run Count : 1

Page 3 / 7

User Name: supasak.nimsongtham
 Hostname: 5CG1115HKC

System Id: GM-2
 Print Date: October 1, 2021 1:10:19 PM

ALS_GM2 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 1, 2021 12:51:01 PM	Start	Execution	Scouting Run - Injection Tower, Front MMI, SQ: - Source: - EI - Inert- Part of GCMS System Preparation	None
October 1, 2021 12:51:18 PM	Audit	Data	Scouting Run - Injection Tower, Front MMI, SQ: - Source: - EI - Inert- Part of GCMS System Preparation	Data files Path : E:\GM2OQ2021\SCOUTING RUN001.D\DATA.MS
October 1, 2021 12:51:42 PM	Audit	Data	Scouting Run - Injection Tower, Front MMI, SQ: - Source: - EI - Inert- Part of GCMS System Preparation	Data files Path : E:\GM2OQ2021\SCOUTING RUN001.D\DATA.MS
October 1, 2021 12:52:42 PM	Audit	Data	Scouting Run - Injection Tower, Front MMI, SQ: - Source: - EI - Inert- Part of GCMS System Preparation	Data files Path : E:\GM2OQ2021\SCOUTING RUN001.D\DATA.MS
October 1, 2021 12:53:25 PM	End	Execution	Scouting Run - Injection Tower, Front MMI, SQ: - Source: - EI - Inert- Part of GCMS System Preparation	Run Count : 1
October 1, 2021 12:53:27 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front MMI, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	None
October 1, 2021 12:53:40 PM	Audit	Data	Signal to Noise EI - Injection Tower, Front MMI, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	Data files Path : E:\GM2OQ2021\SNF1_001.D\DATA.MS
October 1, 2021 12:53:56 PM	End	Execution	Signal to Noise EI - Injection Tower, Front MMI, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	Run Count : 1

User Name: supasak.nimsongtham
 Hostname: 5CG1115HKC

System Id: GM-2
 Print Date: October 1, 2021 1:10:19 PM

ALS_GM2 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 1, 2021 12:53:59 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front MMI, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	None
October 1, 2021 12:54:04 PM	Audit	Data	Signal to Noise EI - Injection Tower, Front MMI, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	Data files Path : E:\GM2OQ2021\SNF2_001.D D\DATA.MS
October 1, 2021 12:54:22 PM	End	Execution	Signal to Noise EI - Injection Tower, Front MMI, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	Run Count : 1
October 1, 2021 12:54:26 PM	Start	Execution	Injection Precision - Injection Tower, Front MMI, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	None
October 1, 2021 12:54:37 PM	Audit	Data	Injection Precision - Injection Tower, Front MMI, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : E:\GM2OQ2021\IP_MRP003. D\DATA.MS
October 1, 2021 12:54:37 PM	Audit	Data	Injection Precision - Injection Tower, Front MMI, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : E:\GM2OQ2021\IP_MRP004. D\DATA.MS
October 1, 2021 12:54:37 PM	Audit	Data	Injection Precision - Injection Tower, Front MMI, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : E:\GM2OQ2021\IP_MRP005. D\DATA.MS
October 1, 2021 12:54:37 PM	Audit	Data	Injection Precision - Injection Tower, Front MMI, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : E:\GM2OQ2021\IP_MRP006. D\DATA.MS

User Name: supasak.nimsongtham

System Id: GM-2

Hostname: 5CG1115HKC

Print Date: October 1, 2021 1:10:19 PM

ALS_GM2 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 1, 2021 12:54:37 PM	Audit	Data	Injection Precision - Injection Tower, Front MMI, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : E:\GM2OQ2021\IP_MRP007.D\DATA.MS
October 1, 2021 12:54:37 PM	Audit	Data	Injection Precision - Injection Tower, Front MMI, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : E:\GM2OQ2021\IP_MRP008.D\DATA.MS
October 1, 2021 12:54:52 PM	End	Execution	Injection Precision - Injection Tower, Front MMI, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Run Count : 1
October 1, 2021 12:54:55 PM	Start	Execution	Mass Ratio Precision - Injection Tower, Front MMI, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	None
October 1, 2021 12:55:06 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : E:\GM2OQ2021\IP_MRP003.D\DATA.MS
October 1, 2021 12:55:06 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : E:\GM2OQ2021\IP_MRP004.D\DATA.MS
October 1, 2021 12:55:06 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : E:\GM2OQ2021\IP_MRP005.D\DATA.MS
October 1, 2021 12:55:06 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : E:\GM2OQ2021\IP_MRP006.D\DATA.MS

Page 6 / 7

User Name: supasak.nimsongtham
Hostname: 5CG1115HKC

System Id: GM-2
Print Date: October 1, 2021 1:10:19 PM

ALS_GM2 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 1, 2021 12:55:06 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : E:\GM2OQ2021\IP_MRP007. D:\DATA.MS
October 1, 2021 12:55:06 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : E:\GM2OQ2021\IP_MRP008. D:\DATA.MS
October 1, 2021 12:55:10 PM	End	Execution	Mass Ratio Precision - Injection Tower, Front MMI, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Run Count : 1
October 1, 2021 12:55:13 PM	End	Qualification	Session	OQ
October 1, 2021 12:55:13 PM	Start	Reporting	Session	None
October 1, 2021 1:09:11 PM	Audit	Reporting	Session	Report Generated : Certificate



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)
Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No. 23-65/0316-02

MTC.No. 23-65/0316-02 (A1)

Number of Pages(S) 2

CALIBRATION CERTIFICATE

Nomenclature : "Dwyer" DIGITAL PRESSURE GAUGE

Manufactured by DWYER INSTRUMENTS, INC. U.S.A.

Model : DVGA-00

Serial No. : DVG10 ID. BKK_FS0545


Range : -30 in Hg to 0 in Hg

Resolution : 0.01 in Hg

Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.

104 Phatthanakan 40, Phattanakan Rd.,

Khwaeng Phattanakan, Khet Suan Luang, Bangkok 10250, Thailand.

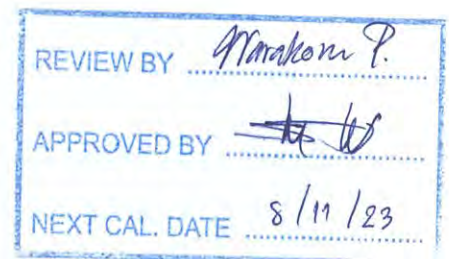

Calibration method : Normal

Received date : 17 March 2022

Calibration date : 10 May 2022

Standard : Reference Pressure Monitor, Serial 1950, Certificate no. 23-64/0581-01

Due Date 3 August 2022

The Standard used for the measurement is traceable to SI Unit through
National Institute of Metrology (THAILAND).

This certificate superseded the certificate no. 23-65/0316-02 dated 12 May 2022

CALIBRATED BY : (signature)

(Mr.Uthai Chaiyapat)

APPROVED BY : (signature)

(Ms.Kirana Luanghirun)

Director
TISTR

Mechanical Engineering Standards Laboratory

Ref. 2013265031701244002

Issued Date : 9 June 2022

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)
Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Reques 23-65/0316-02

2 / 2

MTC.No. 23-65/0316-02 (A1)

This certificate superseded the certificate no. 23-65/0316-02 dated 12 May 2022

Calibration range : -27 in Hg to 0 in Hg

Calibration method : The Digital Pressure Gauge Under Calibration (UUC) was calibrated by comparison method followed DAKKS-DKD-R 6-1: Calibration of Pressure Gauge, edition 03/2014

Calibration condition : Temperature (23.1 ± 2) °C , Relative Humidity (62 ± 10) %
Atmospheric pressure (1006 ± 10) hPa,
Local gravity (9.783003 ± 0.000050) m/s²

Measurement Data :

Gauge position : Vertical

Medium : Air

Reference level : Gauge inlet

Unit : in Hg

UUC Reading	Gauge Pressure	Error	(±) Uncertainty
0.00	0.000	0.000	0.090
-10.00	-9.906	-0.094	0.090
-20.00	-19.684	-0.316	0.090
-26.00	-25.544	-0.456	0.090
-27.00	-26.536	-0.464	0.090
-28.00	-27.507	-0.493	0.090

The reported expanded uncertainties are based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 % .

The End of Calibration Certificate



The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



Certificate of Calibration

Equipment: SPECTROPHOTOMETER
Model: DR6000
Serial No. (or ID.): 1627845 (RYG_EN0037)
Manufacturer: HACH
Condition: In Condition

Certificate No.: C06220464
Issued Date: 27 September 2022
Job No.: KSPR2212224
Page: 1 of 3

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
 616/10 Moo 5 T.Maenam Khu,
 A.Pluakdaeng, Rayong 21140, Thailand.

REVIEW BY *N. Banet*
 APPROVED BY *D. ...*
 NEXT CAL. DATE *27/3/24*

Environment Condition: Temperature 23.1 °C ±
 Humidity 65.4 %RH ±

3.2 %RH

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) (Wet Chemistry)
 616/10 Moo 5 T.Maenam Khu,
 A.Pluakdaeng, Rayong 21140, Thailand.


Calibration By: Mr. Chattuphon Foithong

Calibration Date: 27 September 2022

The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04

Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 91418 and 91435
 The standard for Photometric Certificate No. 91441 and 101088
 The standard for Stray light Certificate No. 101041 and 101040
 The standard for Spectral resolution Certificate No. 101037


 (Mr. Chattuphon Foithong)
 Person in charge


 (Mr. Thalerngkeat Pounngam)
 Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
 DKSH Technology Limited
 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
 2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
 Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:
Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.4	0.21	0.14
536.66	536.7	-0.04	0.14
637.98	638.3	-0.32	0.14
748.48	748.8	-0.32	0.14
807.03	807.4	-0.37	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.5605	0.563	-0.0025	0.0045
	0.7334	0.737	-0.0036	0.0045
	1.0534	1.057	-0.0036	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.5503	0.553	-0.0027	0.0045
	0.7179	0.720	-0.0021	0.0045
	1.0312	1.034	-0.0028	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.5024	0.506	-0.0036	0.0045
	0.6693	0.672	-0.0027	0.0045
	0.9604	0.964	-0.0036	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.5168	0.519	-0.0022	0.0045
	0.6903	0.691	-0.0007	0.0045
	0.9904	0.992	-0.0016	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.5525	0.554	-0.0015	0.0045
	0.7175	0.718	-0.0005	0.0045
	1.0301	1.031	-0.0009	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.5367	0.538	-0.0013	0.0045
	0.6847	0.685	-0.0003	0.0046
	0.9823	0.983	-0.0007	0.0045

Calibration Results:
Without Adjustment
Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7423	0.744	-0.0017	0.0083
257 nm	0.0000	0.000	0.0000	0.0080
	0.8609	0.861	-0.0001	0.0084
313 nm	0.0000	0.000	0.0000	0.0080
	0.2895	0.292	-0.0025	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6381	0.638	0.0001	0.0080

Stray light *

Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
260.67 +/- 0.11 nm	260.7	2.1	1.678
391.94 +/- 0.11 nm	391.9	1.7	1.770

Spectral Resolution *

Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength (nm)	268.60	266.63	1.39	2.00
UUC: Wavelength (nm)	268.2	266.1		
Std Absorbance (A)	0.4810	0.3176		
Absorbance (A)	0.373	0.268		

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: KSPR2212224

ชนิดเครื่องมือ: SPECTROPHOTOMETER

รุ่น: DR6000

หมายเลขเครื่อง: 1627845

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
27 Sep 2022			27 Sep 2022		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตช์ ปิด – เปิด เครื่อง (On-Off Swicth)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		Spectrophotometer			
<input type="checkbox"/>	<input type="checkbox"/>	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	<input type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	656.1 ได้ 656.1 nm
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		pH Meter and Conductivity Meter			
<input type="checkbox"/>	<input type="checkbox"/>	12. อิเล็กโทรด (Electrode and Connection Cable)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	13. ระดับสารละลายใน Electrode (Level KCl)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	15. ขาจับอิเล็กโทรด (Stand)	<input type="checkbox"/>	<input type="checkbox"/>	
		Turbidimeter			
<input type="checkbox"/>	<input type="checkbox"/>	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่เกิน 3.0)	<input type="checkbox"/>	<input type="checkbox"/>	
		Automatic titrator			
<input type="checkbox"/>	<input type="checkbox"/>	18. สภาพ Piston Burettes	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	19. Function Rinsing and Dosing	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	<input type="checkbox"/>	<input type="checkbox"/>	

เพิ่มเติม/ข้อแนะนำ :

Mr. Chattuphon Foithong


Service Engineer

Certificate of System Qualification

GC-OQ

System ID: GC-6
Organization Name: ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location: 104 Phattanakan 40, Phattanakan Rd., Suan Luang, Bangkok 10250

Date: October 21, 2021 10:05:40 AM
EQP Name: AgilentRecommended
EQP Revision: GC.02.50
Overall Qualification Status: Pass

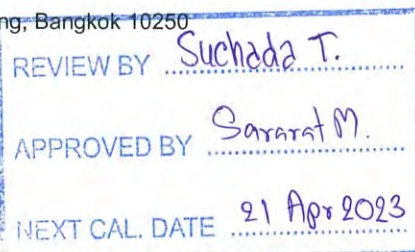

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Decay

Name: 7890

Front SSL

Setpoint Status: Pass

Pressure: 25.0 psi

Pressure Change: 0.0 psi /5 minutes

Agilent Recommended: ≥ -2.0 and ≤ 0.5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Date: October 21, 2021 10:05:40 AM

System ID: GC-6

Setpoint Status:

Pass

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	24.9	psi
Accuracy:			0.1	psi
Agilent Recommended:			<=	1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Inlet Pressure Decay

Name:

7890

Back

SSL

Setpoint Status:

Pass

Pressure:

25.0 psi

Pressure Change:

0.0 psi /5 minutes

Agilent Recommended:

>= -2.0 and <= 0.5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name:

7890

Back

SSL

Setpoint Status:

Pass

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	24.9	psi
Accuracy:			0.1	psi
Agilent Recommended:			<=	1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Detector Flow Accuracy

Date: October 21, 2021 10:05:40 AM

System ID: GC-6

Name: 7890

Front FID

Setpoint Status: Pass

Flow Type: Fuel

Setpoint: 30.0 mL/min Measured Flow: 30.5 mL/min

Accuracy: 0.5 mL/min

Agilent Recommended: ≤ 10.0 % setpoint (3.0 mL/min)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Setpoint Status: Pass

Flow Type: Oxidizer

Setpoint: 400.0 mL/min Measured Flow: 394.0 mL/min

Accuracy: 6.0 mL/min

Agilent Recommended: ≤ 10.0 % setpoint (40.0 mL/min)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Setpoint Status: Pass

Flow Type: Makeup

Setpoint: 25.0 mL/min Measured Flow: 24.2 mL/min

Accuracy: 0.8 mL/min

Agilent Recommended: ≤ 10.0 % setpoint (2.5 mL/min)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

Detector Flow Accuracy

Name: 7890

Back FID

Setpoint Status:

Pass

Flow Type:

Fuel

Setpoint:

30.0

mL/min

Measured Flow:

29.1

mL/min

Accuracy:

0.9

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

3.0

ml/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status:

Pass

Flow Type:

Oxidizer

Setpoint:

400.0

mL/min

Measured Flow:

397.3

mL/min

Accuracy:

2.7

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

40.0

ml/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status:

Pass

Flow Type:

Makeup

Setpoint:

25.0

mL/min

Measured Flow:

24.4

mL/min

Accuracy:

0.6

mL/min

Agilent Recommended:

<=

10.0

% setpoint

(

2.5

ml/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name:

7890

Date:

October 21, 2021 10:05:40 AM

System ID:

GC-6

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

230.0 231.5 °C

Accuracy:

1.5 °C

Agilent Recommended:

>= -1.0 % setpoint in K (-5.0 °C)

<= 1.0 % setpoint in K (5.0 °C)

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

100.0 100.5 °C

Accuracy:

0.5 °C

Agilent Recommended:

>= -1.0 % setpoint in K (-3.7 °C)

<= 1.0 % setpoint in K (3.7 °C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:

7890

Setpoint Status:

Pass

Setpoint/Average

Temperature:

100.0 100.4667 °C

Stability:

0.1 °C

Agilent Recommended:

<= 0.5

Overall GC Oven Temperature Stability Test Status

Pass

Scouting Run

Tested Combination1

Front

SSL

/ Front

FID

Injection Tower

Name:

7693A

Date:

October 21, 2021 10:05:40 AM

System ID:

GC-6

Setpoint Status: Completed

Injection Volume on Column: 1.0 uL

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination1 Front SSL / Front FID

Name: 7890

Setpoint Status: Pass

Base Signal: 12.7 pA

ASTM Noise

pA

0.06

<=

0.10

Drift

pA/Hr

0.10

<=

2.50

Agilent Recommended:

Status:

Pass

Pass

Overall Noise and Drift Test Status

Pass

Injection Precision

Tested Combination1 Front SSL / Front FID

Name: 7693A

Setpoint Status: Pass

Injection Volume on Column: 1.0 uL

Area RSD: 0.42 %

Retention Time RSD: 0.16 %

Agilent Recommended: <= 3.00

<= 1.00

Overall Injection Precision Test Status

Pass

Signal to Noise

Date: October 21, 2021 10:05:40 AM

System ID: GC-6

Tested Combination1 Front SSL / Front FID

Injection Tower

Name: 7890

Setpoint Status: Pass

Signal to Noise: 1174861

Agilent Recommended: \geq 300000

Overall Signal to Noise Test Status

Pass

Scouting Run

Tested Combination2 Back SSL / Back FID

Injection Tower

Name: 7693A

Setpoint Status: Completed

Injection Volume on Column: 1.0 μ L

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination2 Back SSL / Back FID

Name: 7890

Setpoint Status: Pass

Base Signal: 10.4 pA

ASTM Noise

pA

0.05

Agilent Recommended:

 \leq 0.10

Status:

Pass

Drift

pA/Hr

0.00

 \leq 2.50

Pass

Date: October 21, 2021 10:05:40 AM

System ID: GC-6

Overall Noise and Drift Test Status

Pass

Injection Precision

Tested Combination2

Back

SSL

/ Back

FID

Name:

7693A

Setpoint Status:

Pass

Injection Volume on Column:

1.0

uL

Area RSD:

1.16

%

Retention Time RSD:

0.12

%

Agilent Recommended:

<=

3.00

<=

1.00

Overall Injection Precision Test Status

Pass

Signal to Noise

Tested Combination2

Back

SSL

/ Back

FID

Injection Tower

Name:

7890

Setpoint Status:

Pass

Signal to Noise:

805466

Agilent Recommended:

>=

300000

Overall Signal to Noise Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GC-6
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Sampler Identifier	Sampler 2
Inlet	Front
Detector	Front
LTM Included?	No

Tested Combination2

Injection Technique	Injection Tower
Sampler Identifier	Sampler 3
Inlet	Back
Detector	Back
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN15380030
Firmware Revision	A.11.01
Vial Heater	Not installed

Sampler 2

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN10340103
Firmware Revision	A.10.09
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Sampler 3

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN16280128
Firmware Revision	A.10.09
Usage	Sample Injection
Location	Back
Syringe Volume (µL)	10

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN11461066
Firmware Revision	Version 4.27
Component ID/Asset No.	GC-6
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Detector 2

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Back
Makeup Gas	Nitrogen

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Suriya Thongkaew
Logged On User Name:	suriya.thongkaew@non.agilent.com
Signature Creation Date:	October 21, 2021
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: suriya.thongkaew

System Id: GC-6

Hostname: ASBKKW7015

Print Date: October 21, 2021 10:05:46 AM

OQ GC ALS CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 20, 2021 12:18:50 PM	Audit	SessionCreated	Session	None
October 20, 2021 12:18:50 PM	Start	Configuration	Session	None
October 20, 2021 12:18:50 PM	Audit	Entitlement	Licensing	User is Nonpaying and does not require an unlock code
October 20, 2021 12:24:57 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.51/Gc.02.51.eqp], EQP File Name: [Gc.02.51.eqp], EQP Name: [AgilentRecommended]
October 20, 2021 12:25:02 PM	End	Configuration	Session	None
October 20, 2021 12:25:09 PM	Start	Qualification	Session	OQ
October 20, 2021 12:25:09 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
October 20, 2021 12:30:25 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
October 20, 2021 12:56:29 PM	Start	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None

User Name: suriya.thongkaew

System Id: GC-6

Hostname: ASBKKW7015

Print Date: October 21, 2021 10:05:46 AM

OQ GC ALS CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 20, 2021 1:02:16 PM	End	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
October 20, 2021 1:02:18 PM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
October 20, 2021 1:02:26 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
October 20, 2021 1:02:29 PM	Start	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
October 20, 2021 1:04:21 PM	End	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
October 20, 2021 1:07:53 PM	Start	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
October 20, 2021 1:08:11 PM	End	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
October 20, 2021 1:08:16 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
October 20, 2021 1:20:23 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 20, 2021 1:20:26 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1

Page 2 / 10

User Name: suriya.thongkaew

System Id: GC-6

Hostname: ASBKKW7015

Print Date: October 21, 2021 10:05:46 AM

OQ GC ALS CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 20, 2021 1:20:29 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
October 20, 2021 1:23:27 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 20, 2021 1:23:29 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 20, 2021 1:23:31 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
October 20, 2021 1:27:40 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 20, 2021 1:27:42 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 20, 2021 1:27:46 PM	Start	Execution	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
October 20, 2021 1:32:10 PM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 20, 2021 1:32:12 PM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 20, 2021 1:32:14 PM	Start	Execution	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
October 20, 2021 1:34:13 PM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry

Page 3 / 10

User Name: suriya.thongkaew

System Id: GC-6

Hostname: ASBKW7015

Print Date: October 21, 2021 10:05:46 AM

OQ GC ALS CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 20, 2021 1:34:16 PM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 20, 2021 1:34:46 PM	Start	Execution	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
October 20, 2021 1:36:33 PM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 20, 2021 1:36:36 PM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 20, 2021 1:36:38 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 20, 2021 2:04:31 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
October 20, 2021 2:04:32 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
October 20, 2021 2:04:34 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 20, 2021 2:10:47 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry

User Name: suriya.thongkaew

System Id: GC-6

Hostname: ASBKW7015

Print Date: October 21, 2021 10:05:46 AM

OQ GC ALS CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 20, 2021 2:10:49 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
October 20, 2021 2:10:51 PM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
October 20, 2021 2:31:39 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
October 20, 2021 2:31:41 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
October 20, 2021 2:31:44 PM	Start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
October 20, 2021 2:43:06 PM	Audit	AceClosed	Session	None
October 21, 2021 9:18:59 AM	Audit	AceRestarted	Session	None
October 21, 2021 9:19:02 AM	Audit	SessionReloaded	Session	None
October 21, 2021 9:19:09 AM	Start	Qualification	Session	OQ
October 21, 2021 9:19:09 AM	Start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
October 21, 2021 9:19:41 AM	Audit	AceClosed	Session	None

User Name: suriya.thongkaew

System Id: GC-6

Hostname: ASBKKW7015

Print Date: October 21, 2021 10:05:46 AM

OQ GC ALS CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2021 9:20:08 AM	Audit	AceRestarted	Session	None
October 21, 2021 9:20:09 AM	Audit	SessionReloaded	Session	None
October 21, 2021 9:20:13 AM	Start	Qualification	Session	OQ
October 21, 2021 9:20:13 AM	Start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
October 21, 2021 9:29:45 AM	Audit	Data	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_F 2021-10-20 15-49-01\SCOUT_F001.D\FID1A.ch
October 21, 2021 9:30:05 AM	End	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Run Count : 1
October 21, 2021 9:30:08 AM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
October 21, 2021 9:30:41 AM	Audit	Data	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_F 2021-10-20 15-49-01\SIGNSDRF_F001.D\FID1A.ch
October 21, 2021 9:31:10 AM	End	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1

User Name: suriya.thongkaew

System Id: GC-6

Hostname: ASBKKW7015

Print Date: October 21, 2021 10:05:46 AM

OQ GC ALS CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2021 9:31:42 AM	Start	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
October 21, 2021 9:32:55 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_F 2021-10-20 16-51-16\INJPREC_F002.D\FID1A.ch
October 21, 2021 9:32:55 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_F 2021-10-20 16-51-16\INJPREC_F003.D\FID1A.ch
October 21, 2021 9:32:56 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_F 2021-10-20 16-51-16\INJPREC_F004.D\FID1A.ch
October 21, 2021 9:32:56 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_F 2021-10-20 16-51-16\INJPREC_F005.D\FID1A.ch
October 21, 2021 9:32:56 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_F 2021-10-20 16-51-16\INJPREC_F006.D\FID1A.ch
October 21, 2021 9:32:56 AM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_F 2021-10-20 16-51-16\INJPREC_F007.D\FID1A.ch

Page 7 / 10

User Name: suriya.thongkaew

System Id: GC-6

Hostname: ASBKKW7015

Print Date: October 21, 2021 10:05:46 AM

OQ GC ALS CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2021 9:33:07 AM	End	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
October 21, 2021 9:33:23 AM	Start	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	None
October 21, 2021 9:34:01 AM	Audit	Data	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Data files Path : C:\Chem32\1\DATA\OQPV20 21\OQPV2021_F 2021-10-20 16-51-16\SIGTONS_F001.D\FID1A.ch
October 21, 2021 9:34:15 AM	End	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Run Count : 1
October 21, 2021 9:34:19 AM	Start	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	None
October 21, 2021 9:35:04 AM	Audit	Data	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	Data files Path : C:\Chem32\1\DATA\OQPV20 21\OQPV2021_B 2021-10-20 17-13-45\SCOUT_B001.D\FID1A.ch
October 21, 2021 9:35:27 AM	End	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	Run Count : 1
October 21, 2021 9:35:32 AM	Start	Execution	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None

User Name: suriya.thongkaew

System Id: GC-6

Hostname: ASBKKW7015

Print Date: October 21, 2021 10:05:46 AM

OQ GC ALS CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2021 9:36:06 AM	Audit	Data	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_B 2021-10-20 17-13-45\SIGNSDRF_B001.D\FID2B.ch
October 21, 2021 9:36:16 AM	End	Execution	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
October 21, 2021 9:36:20 AM	Start	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
October 21, 2021 9:38:57 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_B 2021-10-20 17-13-45\INJPREC_B002.D\FID2B.ch
October 21, 2021 9:38:57 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_B 2021-10-20 17-13-45\INJPREC_B003.D\FID2B.ch
October 21, 2021 9:38:57 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_B 2021-10-20 17-13-45\INJPREC_B004.D\FID2B.ch
October 21, 2021 9:38:57 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Chem32\1\DATA\OQPV2021\OQPV2021_B 2021-10-20 17-13-45\INJPREC_B005.D\FID2B.ch

User Name: suriya.thongkaew

System Id: GC-6

Hostname: ASBKKW7015

Print Date: October 21, 2021 10:05:46 AM

OQ GC ALS CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2021 9:38:57 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Chem32\1\DATA\OQPV20 21\OQPV2021_B 2021-10-20 17-13-45\INJPREC_B006.D\FID2B.ch
October 21, 2021 9:38:57 AM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Chem32\1\DATA\OQPV20 21\OQPV2021_B 2021-10-20 17-13-45\INJPREC_B007.D\FID2B.ch
October 21, 2021 9:39:06 AM	End	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
October 21, 2021 9:39:11 AM	Start	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	None
October 21, 2021 9:39:28 AM	Audit	Data	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Data files Path : C:\Chem32\1\DATA\OQPV20 21\OQPV2021_B 2021-10-20 17-13-45\SIGTONS_B001.D\FID2B.ch
October 21, 2021 9:39:39 AM	End	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Run Count : 1
October 21, 2021 9:39:43 AM	End	Qualification	Session	OQ
October 21, 2021 9:39:43 AM	Start	Reporting	Session	None
October 21, 2021 10:04:15 AM	Audit	Reporting	Session	Report Generated : Certificate



DRY GAS METER CALIBRATION TEST REPORT

Calibration of Date : 12 Jul 22

Next Calibration Date : 12 Jan 23

Barometric Pressure (mm.Hg) : 755

Relative Humidity (%) 70.0

Temperature (°C) : 30.0

Dry Gas Meter Data

Calibration sheet No.: C-120722-BKK_FS0534

Dry Gas Meter No.: BKK_FS0534

Serial No.: 1509020

Model No.: XE-60-CV

Reference Dry Gas Meter Data

Serial No. : A2003240

Model No. : DGM-SK25RM-QS8

Correction Factor (Yr) : 1.0160

Next Calibration Date : 27 May 23

Reference Dry Gas Meter Calibration				Dry Gas Meter						Dry Gas Meter
Vr (Liters)			Tr (°C)	Vm (Liters)			Ti (°C)	To (°C)	Avg. Tm (°C)	Correction Factor (Y)
Final	Initial	Total		Final	Initial	Total				
30.00	0.00	30.00	29.0	29.39	0.00	29.39	28.0	28.0	28.0	1.0337
30.00	0.00	30.00	29.0	29.46	0.00	29.46	28.0	28.0	28.0	1.0312
60.00	0.00	60.00	29.0	58.93	0.00	58.93	30.0	30.0	30.0	1.0379
60.00	0.00	60.00	29.0	59.02	0.00	59.02	30.0	30.0	30.0	1.0363
90.00	0.00	90.00	29.0	89.02	0.00	89.02	31.0	31.0	31.0	1.0340
90.00	0.00	90.00	29.0	89.10	0.00	89.10	31.0	31.0	31.0	1.0331
									Avg.	1.0343

Y = Ratio of reading of reference dry gas meter to dry gas meter ; tolerance for individual ± 0.02 from average.

Calibrate by :

(Mr. Tinnakorn Kulchart

Field Scientist (1)

Approved by :

(Mr. Natthapol Jiengwareewong

Field Specialist(1)



DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	12-Jul-22	Ambient Temperature (°C) :	30
Calibration sheet No. :	C-120722-BKK_FS0534	Relative Humidity (%) :	70
Digital Temperature ID	BKK_FS0534	Reference Temperature ID :	BKK_FS1144
Console Serial No. :	1509020	Serial No. :	201090006013.00
Model :	XC-60-CV	Model :	Digicon-CC-VT-MS
		Next Calibrate :	31 Jan 23

Location	Reference Temperature °C	Digital Temperature °C	Error °C	Remark
Stack	0	1	1	
	25	26	1	
	50	51	1	
	100	101	1	
	150	151	1	
	200	201	1	
	250	252	2	
	300	302	2	
	500	502	2	
	1000	1002	2	
Probe	1200	1202	2	
	100	101	1	
	125	126	1	
Filter	150	151	1	
	100	101	1	
	125	126	1	
Exit	150	151	1	
	0	1	1	
	10	11	1	
Meter	20	21	1	
	0	1	1	
	25	26	1	
AUX	50	51	1	
	0	1	1	
	25	26	1	
	50	51	1	

Calibrated by : _____

Mr.tinnakorn Kulchart

Field Scientist (1)

Approved by : _____

(Mr.Natthapol Jiengwareewong)

Field Specialist(1)



Rotameter Calibration Report


Calibration Date	: 12 Jul22	Relative Humidity (%)	: 70.0
Rotameter ID	: BKK_FS0534	Barometric Pressure (mmHg)	: 755
Calibration Sheet No	: C-120722-BKK_FS0534	Temperature (°C)	: 30.0

Primary Equipment Data

Brand	: Bios	Model	: Defender 520 M
Serial No.	: 129958	ID	: RYG_FS0209

Calibration Data

Rotameter Reading(cc/min)	Actual Flowrate (cc/min)				Actual Flowrate at STP (cc/min)
	1	2	3	Avg.	
1000	1134.2	1136.0	1138.4	1136.2	1110.1
1500	1694.3	1698.0	1695.3	1695.9	1656.9
2000	2220.1	2229.0	2218.5	2222.5	2171.4
2500	2747.0	2729.3	2735.1	2737.1	2674.2
3000	3298.2	3296.1	3290.4	3294.9	3219.2

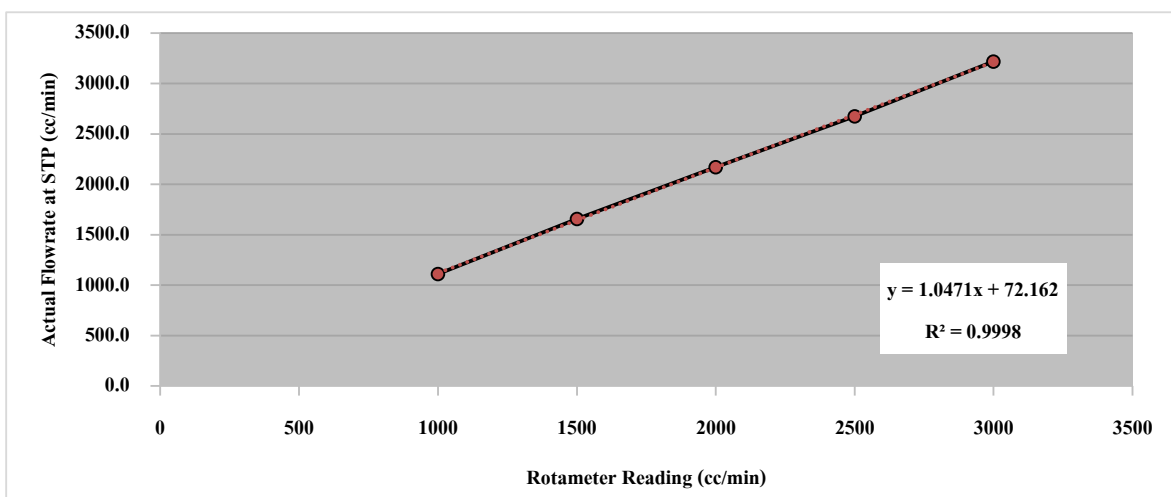

Calibrated by :

(Mr.tinnakorn Kulchart)

Field Scientist (1)

Approved By :

(Mr.Natthapol Jiengwareewong)

Field Specialist(1)



PENTA
CALIBRATION

PENTA CALIBRATION CO., LTD.

66/124 The Connect 33 Village Kanchanaphisek Road
Dokmai Prawet Bangkok 10250
Tel: +66 (0) 2069-9773
www.pentacal.com

Certificate of Calibration

Represent to Certificate of Calibration ,PTC/07/22099

Certificate No.:	PTC/07/22099	Page:	1 of 2
Equipment:	Digital Balance	Condition:	Normal
Manufacturer:	Sartorius	Serial No:	31709552
Model:	MSU224S-100-DU	ID No:	RYG_EN0003
Type of Balance:	Single interval		



Customer: ALS Laboratory Group (Thailand) Co.,Ltd.
616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand

REVIEW BY Thanitall.
APPROVED BY D. [Signature]
NEXT CAL. DATE 23/03/23

Environment Condition: Temperature 23.9 °C \pm 0.3 °C
Humidity 58.1 %RH \pm 4.4 %RH
Air density 1.17 kg/m³

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd.
616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand

The Method used: In house method, PTC-WI-07, base on Euramet cg. 18

Traceability: This certificate is traceable to the SI Units through Thai Calibration Service Co.,Ltd.
, NSC-ONSC Accreditation No.: Calibration 0189

Date Received: March 23, 2022

Calibration Date: March 23, 2022

Issued Date: March 25, 2022

Calibration By: Mr. Rungroje Metakul



PENTA CALIBRATION CO.,LTD

[Signature]

(Mr.Kriangsak Kalasri)

Reviewed by

Approved By :

[Signature]

(Mr. Keattisak Kerdto)

Laboratory Manager

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognised national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The effect that the results relate only to the items calibrated.

This calibration certificate shall not be reproduced except in full only, without written approval from penta calibration co., ltd



Represent to Certificate of Calibration ,PTC/07/22099

Certificate No.: PTC/07/22099



Page: 2 of 2

Measurement Results:

Without Adjustment :

Function Calibration: Non Adjustment

Eccentric Error: Weight to be 1/3 ,1/2 or of Maximum capacity

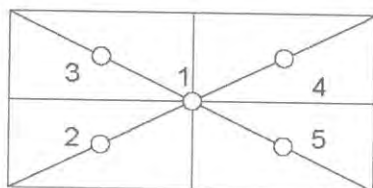

Eccentricity test 100 (g)

Position (g)				
1	2	3	4	5
0.0000	0.0000	-0.0001	-0.0001	0.0001
Maximum deviation:				0.0001

Repeatability Test : Weight to be $1/2 \leq L_1 \leq$ Maximum capacity

Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
200	0.00007

Error of indication : from nominal value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Indication (g)	Correction of Balance (g)	Uncertainty (g)	k
0	0.00000	0.0000	0.0000	0.00020	2.65
0.01	0.01000	0.0099	0.0001	0.00020	2.43
0.1	0.10000	0.1000	0.0000	0.00020	2.43
0.5	0.50000	0.5000	0.0000	0.00020	2.43
1	1.00000	1.0000	0.0000	0.00020	2.43
5	5.00001	5.0000	0.0000	0.00020	2.43
10	10.00000	10.0000	0.0000	0.00020	2.43
20	20.00003	20.0000	0.0000	0.00020	2.43
50	50.00004	50.0000	0.0000	0.00021	2.32
100	100.00004	99.9999	0.0001	0.00022	2.17
200	200.00011	200.0000	0.0001	0.00027	2.05

Note: Weight of adjust - (g)

The End of Certificate



ROTA METER CALIBRATION RESULT JULY 2022

Rotameter ID.	Calibration Date	Regression Result	Coefficient (R ²)
BKK_FS0577	01 Jul 22	$Y = 1.0202x + 0.1976$	1.0000
BKK_FS0579	01 Jul 22	$Y = 1.0078x + 0.4789$	0.9998
BKK_FS0583	01 Jul 22	$Y = 1.016x + 0.3922$	1.0000
BKK_FS0584	01 Jul 22	$Y = 1.0036x + 2.2262$	0.9997
BKK_FS0585	01 Jul 22	$Y = 1.0189x - 5.6476$	0.9997
BKK_FS0586	01 Jul 22	$Y = 1.0095x - 1.1524$	0.9995
BKK_FS0587	01 Jul 22	$Y = 1.013x - 3.6619$	0.9996
BKK_FS0588	01 Jul 22	$Y = 1.0154x + 4.8357$	0.9999
BKK_FS0589	01 Jul 22	$Y = 0.9918x + 4.8069$	0.9999
BKK_FS0590	01 Jul 22	$Y = 1.0038x - 0.4857$	0.9996
BKK_FS0591	01 Jul 22	$Y = 0.9705x - 52.174$	0.9986
BKK_FS0592	01 Jul 22	$Y = 0.9646x - 37.642$	0.9985
BKK_FS0593	01 Jul 22	$Y = 0.9767x - 58.445$	0.9988
BKK_FS0594	01 Jul 22	$Y = 0.9902x - 62.87$	0.9999
BKK_FS0595	01 Jul 22	$Y = 1.0249x - 98.162$	0.9999
BKK_FS0596	01 Jul 22	$Y = 0.9843x - 26.806$	0.9991
BKK_FS0597	01 Jul 22	$Y = 0.9802x - 61.653$	0.9978
BKK_FS1004	01 Jul 22	$Y = 0.9696x + 17.69$	0.9990
BKK_FS1005	01 Jul 22	$Y = 1.0092x + 2.4571$	0.9999
BKK_FS1006	01 Jul 22	$Y = 1.168x - 5.566$	0.9997
BKK_FS1007	01 Jul 22	$Y = 0.9917x + 1.6592$	1.0000
BKK_FS1008	01 Jul 22	$Y = 1.0132x + 0.7207$	1.0000
BKK_FS1009	01 Jul 22	$Y = 1.0132x + 1.1633$	0.9960
BKK_FS1010	01 Jul 22	$Y = 1.0033x + 0.5758$	0.9999
BKK_FS1011	01 Jul 22	$Y = 1.0234x + 0.1759$	0.9996
BKK_FS1012	01 Jul 22	$Y = 1.0106x - 2.0048$	0.9997
BKK_FS1013	01 Jul 22	$Y = 0.9677x - 35.851$	0.9997
BKK_FS1014	01 Jul 22	$Y = 1.0021x + 0.3148$	0.9998
BKK_FS1015	01 Jul 22	$Y = 0.9994x + 1.786$	1.0000
BKK_FS1016	01 Jul 22	$Y = 1.0105x - 80.256$	0.9998
BKK_FS1017	01 Jul 22	$Y = 0.9995x + 0.649$	1.0000
BKK_FS1018	01 Jul 22	$Y = 1.0011x + 1.1786$	1.0000
BKK_FS1019	01 Jul 22	$Y = 1.0023x - 68.424$	0.9996
BKK_FS1020	01 Jul 22	$Y = 1.0547x - 0.666$	0.9998
BKK_FS1021	01 Jul 22	$Y = 1.018x - 3.3286$	0.9998
BKK_FS1022	01 Jul 22	$Y = 0.9932x - 57.035$	0.9986
BKK_FS1023	01 Jul 22	$Y = 1.0094x + 0.0717$	0.9999
BKK_FS1024	01 Jul 22	$Y = 1.0042x + 0.4086$	0.9997
BKK_FS1025	01 Jul 22	$Y = 1.0132x - 88.507$	0.9996



ROTA METER CALIBRATION RESULT JULY 2022

Rotameter ID.	Calibration Date	Regression Result	Coefficient (R ²)
BKK_FS1026	01 Jul 22	$Y = 1.0018x + 1.0776$	0.9997
BKK_FS1027	01 Jul 22	$Y = 1.0053x + 0.231$	0.9995
BKK_FS1028	01 Jul 22	$Y = 0.9792x - 60.312$	0.9982
BKK_FS1029	01 Jul 22	$Y = 0.9935x + 0.8234$	1.0000
BKK_FS1030	01 Jul 22	$Y = 1.0039x + 0.515$	0.9999
BKK_FS1031	01 Jul 22	$Y = 1.009x - 79.295$	0.9998
BKK_FS1039	01 Jul 22	$Y = 0.9879x + 7.3524$	0.9996
BKK_FS1040	01 Jul 22	$Y = 0.9704x + 88.336$	0.9987
BKK_FS1041	01 Jul 22	$Y = 1.0645x - 1.7878$	0.9999
BKK_FS1042	01 Jul 22	$Y = 0.9983x + 3.6262$	0.9998
BKK_FS1043	01 Jul 22	$Y = 1.0069x - 6.9619$	1.0000
BKK_FS1044	01 Jul 22	$Y = 1.0355x - 0.6214$	0.9997
BKK_FS1161	01 Jul 22	$Y = 1.0126x + 0.7738$	0.9999
BKK_FS1162	01 Jul 22	$Y = 0.9994x + 2.6357$	0.9995
BKK_FS1163	01 Jul 22	$Y = 0.977x - 55.03$	0.9987
BKK_FS1164	01 Jul 22	$Y = 0.9914x + 0.8427$	0.9997
BKK_FS1165	01 Jul 22	$Y = 0.9893x + 6.5919$	0.9998
BKK_FS1166	01 Jul 22	$Y = 1.0031x - 77.881$	0.9996
BKK_FS1200	01 Jul 22	$Y = 1.0313x - 0.4602$	0.9995
BKK_FS1201	01 Jul 22	$Y = 1.0045x + 0.15$	0.9996
BKK_FS1202	01 Jul 22	$Y = 0.9702x - 44.156$	0.9994
RYG_FS0197	01 Jul 22	$Y = 1.0039x - 0.179$	0.9999
RYG_FS0198	01 Jul 22	$Y = 0.9971x + 16.648$	0.9999
RYG_FS0199	01 Jul 22	$Y = 1.0832x - 2.6367$	1.0000

Review By :

(Mr. Wichan Choonharat)

Enviro Field Services Manager

Approved By :

(Mr. Sarayuth Jittranont)

Assistant General Manager

SITHIPHORN ASSOCIATES CO.,LTD.

CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd., Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACC22013

Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR
Manufacturer : RION
Model : NC-74
Serial No.: 34178121
ID No.: RYG_FS0213

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 22 APRIL 2022
Calibration Date : 26 APRIL 2022
Date of Issue : 29 APRIL 2022

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	26/4/23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACC22013

Job No. : VC65AC0054

Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	33461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23
Audio Analyzer	AVR-3360A	V744B6069	EF-0010-22	07-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACC22013

Job No. : VC65AC0054

Pages : 3 of 3

Result of calibration :**1. Sound pressure level**

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit (dB)
94	94.11	0.11	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Tolerance limit (%)
1000	1003.1	0.3	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Tolerance limit (%)
2.02	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL22181

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00873057 / 171591 / 73333
ID No.: RYG_FS0381

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 22 AUGUST 2022
Calibration Date : 26-31 AUGUST 2022
Date of Issue : 02 SEPTEMBER 2022

REVIEW BY	Narakorn P.
APPROVED BY	[Signature]
NEXT CAL. DATE	26/8/23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22181

Job No. : VC65AC0077

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22181
Job No. : VC65AC0077
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.4	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22181

Job No. : VC65AC0077

Pages : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.0
C - weight	18.3
Flat	24.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.2	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.2	0.2	0.2	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22181

Job No. : VC65AC0077

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	-0.1	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22181

Job No. : VC65AC0077

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.1	0.1	± 1.1
136.0	136.1	0.1	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.1	0.1	± 1.1
124.0	124.1	0.1	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.1	0.1	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	25.0	0.0	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22181
Job No. : VC65AC0077
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.1	-0.3	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22181

Job No. : VC65AC0077

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL22182

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00873109 / 171842 / 73485
ID No.: RYG_FS0384

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 22 AUGUST 2022
Calibration Date : 26-31 AUGUST 2022
Date of Issue : 02 SEPTEMBER 2022

REVIEW BY	Narakorn P.
APPROVED BY	[Signature]
NEXT CAL. DATE	26/8/23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22182

Job No. : VC65AC0077

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22182

Job No. : VC65AC0077

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.4	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22182

Job No. : VC65AC0077

Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.5

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.2
C - weight	17.6
Flat	23.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.4	0.5	0.5	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-2.4	-2.4	-2.4	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22182

Job No. : VC65AC0077

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	-0.1	±1.5
250	-0.1	-0.1	-0.1	±1.5
500	-0.1	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22182
Job No. : VC65AC0077
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.1	0.1	± 1.1
136.0	136.1	0.1	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.1	0.1	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.1	0.1	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.1	0.1	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	24.9	-0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22182
Job No. : VC65AC0077
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22182
Job No. : VC65AC0077
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

_____ **End of Calibration Certificate** _____

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL22183

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01073423 / 169513 / 73684
ID No.: RYG_FS0386

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAEANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 22 AUGUST 2022
Calibration Date : 26-31 AUGUST 2022
Date of Issue : 02 SEPTEMBER 2022

REVIEW BY	<i>Marakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	26/8/23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22183

Job No. : VC65AC0077

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22183

Job No. : VC65AC0077

Pages : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.6
C - weight	18.6
Flat	24.5

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.2	0.2	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	1.5	1.5	1.6	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22183
Job No. : VC65AC0077
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22183
Job No. : VC65AC0077
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.8	-0.2	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22183
Job No. : VC65AC0077
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.8	-0.6	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.1	0.1	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22183

Job No. : VC65AC0077

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.7	89.5	-0.2	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

————— **End of Calibration Certificate** —————

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL22062

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01222723 / 143841 / 22770
ID No.: RYG_FS0022

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 14 JANUARY 2022
Calibration Date : 21-24 JANUARY 2022
Date of Issue : 25 JANUARY 2022



Calibrated by : Nathakorn Pisutpaisan

Approved by :

()
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22062
Job No. : VC65AC0043
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22062
Job No. : VC65AC0043
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22062

Job No. : VC65AC0043

Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.96)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.0
C - weight	18.0
Flat	24.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.4	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-0.4	-0.3	-0.3	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22062

Job No. : VC65AC0043

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz
5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22062

Job No. : VC65AC0043

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

Continuation of Calibration Certificate

 Cert. No. : ACL22062
 Job No. : VC65AC0043
 Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.8	-0.6	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22062

Job No. : VC65AC0043

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

————— **End of Calibration Certificate** —————

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL22059

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00734220 / 145272 / 34370
ID No.: RYG_FS0026

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAEANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 14 JANUARY 2022
Calibration Date : 21-24 JANUARY 2022
Date of Issue : 25 JANUARY 2022

REVIEW BY	Narakorn P.
APPROVED BY	[Signature]
NEXT CAL. DATE	21/1/23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22059

Job No. : VC65AC0043

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22059
Job No. : VC65AC0043
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22059

Job No. : VC65AC0043

Pages : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.96)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.6
C - weight	17.8
Flat	23.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.3	0.3	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-1.6	-1.5	-1.5	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22059
Job No. : VC65AC0043
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22059

Job No. : VC65AC0043

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.0	0.0	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22059

Job No. : VC65AC0043

Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.1	-0.3	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22059

Job No. : VC65AC0043

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.7	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL22025

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00734221 / 145286 / 34371
ID No.: RYG_FS0027

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 05 JANUARY 2022
Calibration Date : 10-12 JANUARY 2022
Date of Issue : 13 JANUARY 2022

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	10/1/23

Calibrated by : Nathakorn Pisutpaisan

Approved by :

[Signature]
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22025

Job No. : VC65AC0040

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0012-21	10-Feb-22
Waveform Generator	33511B	MY52302742	EF-0011-21	10-Feb-22
Digital Multimeter	33461A	MY53220104	EEL.BP. 05/0264	10-Feb-22
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0264	08-Feb-22
Digital Multimeter	34461A	MY60024273	1-15180725251-1	15-Sep-22
Programmable Attenuator	MAT-1070	62100114	1500-07774E	08-Mar-22
Condenser Microphone	4180	2977900	AA-1008-21	05-Feb-22
Measuring Amplifier	NA-42KAI	34560495	AA-3003-21	16-Feb-22

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22025

Job No. : VC65AC0040

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22025

Job No. : VC65AC0040

Pages : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.96)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.6
C - weight	18.0
Flat	23.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.5	0.5	0.6	± 1.5
1000	0.0	0.0	0.1	± 1.0
8000	-2.3	-2.3	-2.3	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22025

Job No. : VC65AC0040

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22025
Job No. : VC65AC0040
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.0	0.0	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22025
Job No. : VC65AC0040
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22025

Job No. : VC65AC0040

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

CERTIFICATE OF CALIBRATION

ISSUED BY **Cirrus Research plc**

DATE OF ISSUE **07 October 2022** CERTIFICATE NUMBER **181219**

REVIEW BY *Morahan P.*
 APPROVED BY *Nigel Smith*
 NEXT CAL. DATE **7/10/23**



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 1

Test engineer:
 Nigel Smith
 Electronically signed:

Nigel Smith

doseBadge Reader

Instrument

Manufacturer: Cirrus Research plc
 Model Number: RC:110A

Serial Number: 76062
 Notes:

Calibration Procedure

The tests were carried out in accordance with the requirements of IEC 60942:2003 where applicable.

Date of Calibration: 07 October 2022

Functionality Results

Function	Result
Keypad	Pass
Battery Power	Pass
Display	Pass
Communication	Pass
2 way IR link	Pass
Clock	Pass

Calibration Results

	Level (dB)	Frequency (Hz)	Distortion (% THD + Noise)
Initial	113.66	1009.5	0.36
Adjusted	113.99	1009.5	0.41
Uncertainty	± 0.11	± 0.14	± 0.10
Tolerances	± 0.60	± 2.00	± 4.00

Environmental Conditions

Pressure: 100.27 kPa
 Temperature: 23.8 °C
 Humidity: 45.9 %

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.




TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CH405
Page.: 1 of 3

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	Seven Compact S220
Serial No. :	C104059460
ID No. :	RYG_EN0183
Condition As-Received:	Used Item
Received Date :	16 March 2022
Calibration Date :	17 March 2022
Reference :	2203-0611DSC-4
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer

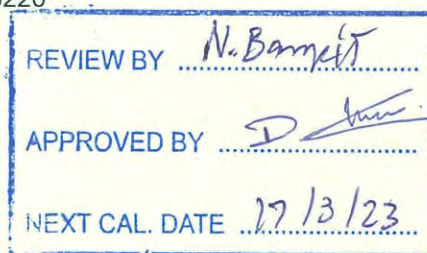

Calibrated by : Warakorn Lernagtrakul

Approved by :

Malee

Approved Signatory

- (☒) Malee Butkruea
() Saithip Meangmai
() Warakorn Lernagtrakul

Issue Date : 22 March 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 22CH405

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	21E2682	25 Aug 2022
2) Ref. Standard Thermometer	4982054	110RC044	21I1201	26 Oct 2022

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	788995	01 Jan 2024
pH 6.982	CPA chem	761017	02 Aug 2022
pH 10.015	CPA chem	766824	04 Sep 2022

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: C104059460	4.000	177.48	177.4	4.000	0.058	2.00
	7.000	0.00	-0.1	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Malu.



Cert.No.: 22CH405

Page.: 3 of 3

Calibration Results**Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (\pm)	Coverage factor k
pH Electrode S/N.: 1453404	4.008	4.010	177.7	0.0046	2.00
	6.982	6.988	3.6	0.0084	2.00
	10.015	10.010	-172.9	0.0073	2.05

Function : Temperature Measurement**(*) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : InLab Expert Pro-ISM

- Serial No. : 1453404

Dimension of probe;

- Length : 120 mm.

- Diameter : 12 mm.

- Immersion Depth : 100 mm.

Calibration Point ($^{\circ}\text{C}$)	Standard Temperature ($^{\circ}\text{C}$)	UUC* Reading ($^{\circ}\text{C}$)	Error ($^{\circ}\text{C}$)	Uncertainty of measurement (\pm $^{\circ}\text{C}$)	Coverage factor k
25.0	25.002	24.9	-0.102	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 22E986

Page : 1 of 2

Equipment : pH Meter
Manufacturer: Mettler Toledo
Model : SevenCompact S220
Serial No.: C104059460
ID No.: RYG_EN0183

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used Item
Received Date: 16 March 2022
Calibration Date: 21 March 2022

Reference: 2203-0611DSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 10) %

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong
21140, Thailand

Procedure used: Calibration were conducted using in-house calibration Procedure CP-E17 According to direct measurement method with Multi-Product Calibrator.

Condition of this result of calibration

1.Reference standards instruments :


<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Multi-Product Calibrator	5500A	6440007	21E1444	07 May 2022

2.This result of calibration was made on requested at the point specified by customer.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

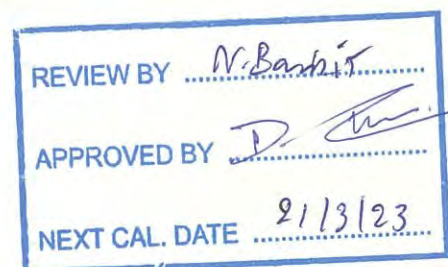

Calibrated by : Pongsagorn Boonyaporn
Issue Date : 22 March 2022

Approved Signatory :

☒ Phalinee Prabpaipal
☐ Nuntawat Khamchai
☐ Pornthippa Tameyakul

B 0284414



Cert. No.: 22E986

Page.: 2 of 2

Result of calibration :- (*) Without adjustment () After adjustment

Function:	DC voltage measurement		Range:	2000	mV
	<u>Standard Value</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>	
	(mV)	(mV)	(mV)	(\pm μ V)	
	-200.0000	-200.0	0.0	72	
	-150.0000	-150.0	0.0	69	
	-100.0000	-100.0	0.0	65	
	-50.0000	-50.0	0.0	62	
	0.0000	0.0	0.0	58	
	50.0000	50.0	0.0	62	
	100.0000	100.0	0.0	65	
	150.0000	150.0	0.0	69	
	200.0000	200.0	0.0	72	

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %

*UUC= Unit Under Calibration.

-o0o-

a 1101070



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 22TW34

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000-115V
Serial No. :	15E102796
ID No. :	RYG_EN0032
Received Date :	11 February 2022
Test Date :	14 February 2022
Reference :	2202-0404DSC-4
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	 Approved Signatory
() Malee Butkruea	
(<input checked="" type="checkbox"/>) Saithip Meangmai	
() Warakorn Lerngagtrakul	
Issue Date :	18 February 2022

REVIEW BY	<u>N. Bannit</u>
APPROVED BY	<u>D. Chai</u>
NEXT CAL. DATE	<u>15/8/23</u>



Cert.No.: 22TW34

Page.: 2 of 2

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 15E100464

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.02	8.02	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Saithip



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22LM12

Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000-115V

Serial No. : 15E102796

ID No. : RYG_EN0032

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 11 February 2022

Calibrated Date : 21 February 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Kunchit Promprat

Approved by : Malee Butkruea
Approved Signatory

() Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date : 21 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0038008



Equipment : DO Meter with Sensor

Condition As-Received : Used Item

Reference : 2202-0404DSC-5

Cert. No.: 22LM12

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1523	2188080	2111273	22 Nov 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 15E100464

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	45	20.001	19.88	-0.121	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Mahu



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM317

Page.: 1 of 3

Certificate of Calibration

Equipment : Low Temp. Incubator

Manufacturer : Memmert

Model : IPP750

Serial No. : V818.0084

ID No. : RYG_EN0154

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
(Rayong Branch)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand

Location : BOD Room

Received Order : 22 April 2022

Calibration Date : 22 April 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon

REVIEW BY	<i>N. Banvit</i>
APPROVED BY	<i>D. [Signature]</i>
NEXT CAL. DATE	21/10/23

Approved by :

Manu

Approved Signatory

- () Pornthippa Tameyakul
(/) Malee Butkruea
() Suwit Imjai

Issue Date :

3 May 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0040735



Equipment : Low Temp. Incubator

Condition As-Received : Used Item

Reference : 2204-0146OC-1

Cert. No.: 22TM317

Page.: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44031769	21LM12	02 Sep 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

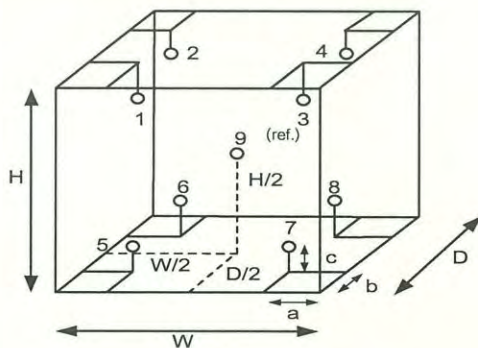

Environment during calibration		
	Beginning	Finished
Temp. (°C)	25	25
REL.Humid. (%)	54	58
AC Supply (Volt)	221	223

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.60 m
W = 1.0 m
H = 1.2 m
Capacity = 0.75 m³

Position :	Ref. Std. ID No.:
1	9RTD-2/1
2	9RTD-2/2
3	9RTD-2/3
4	9RTD-2/4
5	9RTD-2/5
6	9RTD-2/6
7	9RTD-2/7
8	9RTD-2/8
9 (ref.)	9RTD-2/9

Malu



Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2204-0146OC-1
Result of Calibration :- (*) Without Adjustment

Cert. No.: 22TM317

Page.: 3 of 3

Function of UUC* : Temperature Source

Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
20.0	20.0	20.0	0.022	0.20	0.22	0.30	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
20.0	20.209	20.174	20.199	20.110	20.075	20.062	20.027	20.069	20.030

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu



PENTA
CALIBRATION

PENTA CALIBRATION CO., LTD.

66/124 The Connect 33 Village Kanchanaphisek Road
Dokmai Prawet Bangkok 10250
Tel: +66 (0) 2069-9773
www.pentacal.com

Certificate of Calibration

Represent to Certificate of Calibration ,PTC/07/22103

Certificate No.:	PTC/07/22103	Page:	1 of 2
Equipment:	Digital Balance	Condition:	Normal
Manufacturer:	Sartorius	Serial No:	26207038
Model:	MSE224S-100-DU	ID No:	RYG_EN0002
Type of Balance:	Single interval		



Customer: ALS Laboratory Group (Thailand) Co.,Ltd.
616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand



Environment Condition: Temperature 23.9 °C ± 0.3 °C
Humidity 58.1 %RH ± 4.4 %RH
Air density 1.17 kg/m³

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd.
616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand

The Method used: In house method, PTC-WI-07, base on Euramet cg. 18

Traceability: This certificate is traceable to the SI Units through Thai Calibration Service Co.,Ltd.
, NSC-ONSC Accreditation No.: Calibration 0189

Date Received: March 23, 2022

Calibration Date: March 23, 2022

Issued Date: March 25, 2022

Calibration By: Mr. Rungroje Metakul



PENTA CALIBRATION CO.,LTD.

(Mr.Kriangsak Kalasri)
Reviewed by

Approved By :
(Mr. Keattisak Kerdto)
Laboratory Manager

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognised national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The effect that the results relate only to the items calibrated.

This calibration certificate shall not be reproduced except in full only, without written approval from penta calibration co., ltd



Represent to Certificate of Calibration ,PTC/07/22103

Certificate No.: PTC/07/22103



Page: 2 of 2

Measurement Results:

Without Adjustment :

Function Calibration: Non Adjustment

Eccentric Error: Weight to be 1/3 ,1/2 or of Maximum capacity

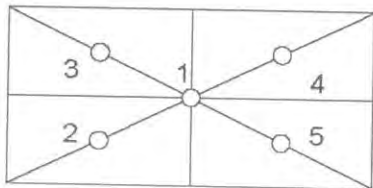

Eccentricity test 100 (g)

Position (g)				
1	2	3	4	5
0.0000	0.0000	-0.0002	0.0002	0.0002
Maximum deviation:			0.0002	

Repeatability Test : Weight to be $1/2 \leq L_1 \leq$ Maximum capacity

Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
200	0.00003

Error of indication : from nominal value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Indication (g)	Correction of Balance (g)	Uncertainty (g)	k
0	0.00000	0.0000	0.0000	0.000086	2.16
0.01	0.01000	0.0100	0.0000	0.00010	2.06
0.1	0.10000	0.1000	0.0000	0.00010	2.06
1	1.00000	1.0000	0.0000	0.00010	2.06
2	2.00000	1.9999	0.0001	0.00010	2.06
5	5.00001	5.0000	0.0000	0.00010	2.06
10	10.00000	10.0000	0.0000	0.00010	2.06
20	20.00003	19.9999	0.0001	0.00011	2.05
50	50.00004	49.9999	0.0001	0.00012	2.00
100	100.00004	100.0001	-0.0001	0.00017	2.00
200	200.00011	200.0000	0.0001	0.00027	2.00

Note: Weight of adjust - (g)

The End of Certificate



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1517

Page : 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Memmert

Model : UFE 500

Serial No. : G511.1572

ID No. : RYG_EN0010

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T. Maenam Khu,
A. Pluakdaeng,
Rayong 21140 Thailand

Location : Oven Room

Received Order : 20 October 2022

Calibration Date : 20 October 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon

REVIEW BY Thanitall

APPROVED BY D. [Signature]

NEXT CAL. DATE 20/04/24

Approved by :

Malu

Approved Signatory

- () Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date :

2 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Hot Air Oven
 Condition As-Received : Used Item
 Reference : 2210-0376OC-2

Cert. No.: 22TM1517
 Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY49023932	22LM97	29 Jul 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

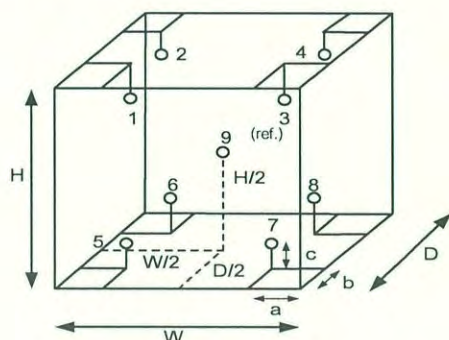

Environment during calibration		
	Beginning	Finished
Temp. (°C)	25	25
REL.Humid. (%)	54	59
AC Supply (Volt)	223	225

Ref. Std. ID No.: @ Calibration Point

Position :	(180) °C	(104) °C
1	21-16TC-01	20-16RTD-01
2	21-16TC-02	20-16RTD-02
3	21-16TC-03	20-16RTD-03
4	21-16TC-04	20-16RTD-04
5	21-16TC-05	22-16RTD-05
6	21-16TC-06	20-16RTD-06
7	21-16TC-07	20-16RTD-07
8	21-16TC-08	22-16RTD-08
9 (ref.)	21-16TC-09	22-16RTD-09

Probe Installation Details :

Dimension of Chamber :

a =	5.0	cm	D =	0.40	m
b =	5.0	cm	W =	0.56	m
c =	5.0	cm	H =	0.48	m
Capacity =			0.11	m ³	

Malu



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2210-0376OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 22TM1517

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
104.0	104.0	104.0	0.076	0.52	0.60	0.42	2
180.0	180.0	180.0	0.13	0.88	1.2	1.1	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	103.768	103.734	103.723	103.800	104.215	104.131	104.132	103.740	103.747
180.0	179.723	179.359	179.439	179.489	180.361	180.114	180.131	180.243	179.605

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu .



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1492

Page : 1 of 3

Certificate of Calibration

Equipment :	Hot Air Oven
Manufacturer :	Memmert
Model :	UM 400
Serial No. :	b495.0899
ID No. :	RYG_EN0006
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5, T. Maenam Khu, A. Pluakdaeng, Rayong 21140, Thailand
Location :	Oven Room
Received Order :	20 October 2022
Calibration Date :	20 October 2022
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %

Calibrated by : Preecha Hlahib

Approved by :

Malu.
Approved Signatory

- (☒) Pornthippa Tameyakul
(☒) Malee Butkruea
(☐) Suwit Imjai

Issue Date : 2 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Hot Air Oven
 Condition As-Received : Used Item
 Reference : 2210-0376OC-1

Cert. No.: 22TM1492
 Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44035217	21LM30	23 Dec 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	29
REL.Humid. (%)	43	47
AC Supply (Volt)	220	221

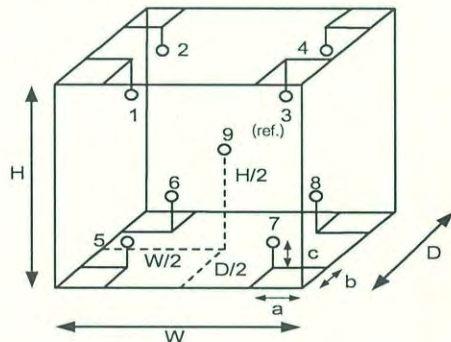

Position :	Ref. Std. ID No.:
1	18-10RTD-01
2	18-10RTD-02
3	18-10RTD-03
4	18-10RTD-04
5	18-10RTD-05
6	18-10RTD-06
7	18-10RTD-07
8	18-10RTD-08
9 (ref.)	18-10RTD-09

Probe Installation Details :

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of Chamber :

D = 0.33 m
 W = 0.40 m
 H = 0.40 m
 Capacity = 0.053 m³

Malu .



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2210-0376OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 22TM1492
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
70.0	70.0	70.0	0.079	0.47	0.77	0.42	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
70.0	70.262	69.995	70.079	70.177	70.664	70.039	70.688	70.149	70.328

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1491

Page : 1 of 3

Certificate of Calibration

Equipment :	Water Bath
Manufacturer :	Memmert
Model :	WNB22
Serial No. :	L513.0648
ID No. :	RYG_EN0061
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5, T. Maenam Khu, A. Pluakdaeng, Rayong 21140, Thailand
Location :	Wet Chemistry Lab
Received Order :	20 October 2022
Calibration Date :	20 October 2022
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Preecha Hlahib



Approved by :

Malee

Approved Signatory

- () Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date :

2 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2210-0376OC-4

Cert. No.: 22TM1491

Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Data Acquisition	34970A	MY44035217	21LM30	23 Dec 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	24	53	222
Finished of Calibration	24	50	221

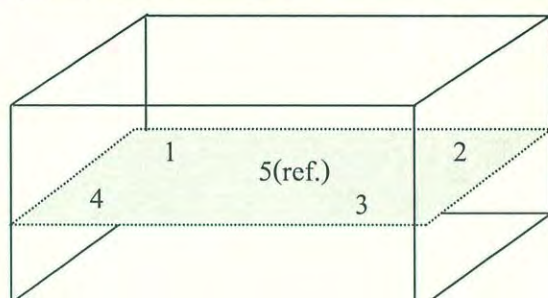

Front

Position :	Ref. Std. S/N.:
1	N37P300726
2	N37P300727
3	N37P300728
4	N37P300729
5(ref.)	N37P300730

Malu



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2210-0376OC-4
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 22TM1491
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)				
			Position				
			1	2	3	4	5 (ref.)
85.0	85.0	85.0	84.527	84.563	84.628	84.516	84.580

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
85.0	0.12	0.081	0.18	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CH377

Page.: 1 of 2

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	Seven2Go
Serial No. :	B531256371
ID No. :	RYG_FS0420
Condition As-Received:	Used Item
Received Date :	11 March 2022
Calibration Date :	14 March 2022
Reference :	2203-0495DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)



Calibrated by : Warakorn Lerngagtrakul

Approved by :

Malee

Approved Signatory

- (✓) Malee Butkruea
() Saithip Meangmai
() Warakorn Lerngagtrakul

Issue Date : 17 March 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0039308



Cert. No.: 22CH377

Page.: 2 of 2

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	21E2682	25 Aug 2022

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	766820	23 Sep 2023
pH 6.983	CPA chem	766822	04 Sep 2022
pH 10.015	CPA chem	766824	04 Sep 2022

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: B531256371	4.00	177.48	177	4.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-178	10.00	0.58	2.00

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor <i>k</i>
pH Electrode S/N.: 1311407	4.008	4.01	181	0.0079	2.00
	6.983	6.98	7	0.0093	2.00
	10.015	10.01	-171	0.0092	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

maker



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22LM41

Page.: 1 of 2

Certificate of Calibration

Equipment : pH Meter with Sensor

Manufacturer : Mettler Toledo

Model : Seven2Go

Serial No. : B531256371

ID No. : RYG_FS0420

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
(Rayong Branch)
616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng,
Rayong 21140 Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 11 March 2022

Calibrated Date : 15 March 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Malee Butkruea

Approved by :

Approved Signatory

() Pornthippa Tameyakul
(✓) Suwit Imjai

Issue Date : 17 March 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0039307



Equipment : pH Meter with Sensor

Cert. No.: 22LM41

Condition As-Received : Used Item

Page.: 2 of 2

Reference : 2203-0495DSC-2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1523	2188080	2111273	22 Nov 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 1311407

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
25.0	100	25.009	25.4	0.391	0.16	2.00
30.0	100	30.008	30.5	0.492	0.16	2.00
40.0	100	39.997	40.6	0.603	0.16	2.00
50.0	100	49.997	50.6	0.603	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Geni

Certificate of Calibration

Equipment:	Block Digestion Unit	Certificate No.:	C29220011
Model:	KT-20s	Issued Date:	18 March 2022
Serial No. (or ID.):	5720210009/5770200073	Job No.:	KSPR2203623
Manufacturer:	Gerhardt	Page:	1 of 3
Condition:	In Condition	Digestion Block:	20 holes.

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand.

Environment Condition:

Temperature:	24 °C	±	0.8 °C
Humidity:	67 %RH	±	2.2 %RH
Voltage:	226 VAC	±	1.7 VAC

REVIEW BY N-Barnir
APPROVED BY D. [Signature]
NEXT CAL. DATE 17/3/23

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
(Wet Chemistry Lab)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand.

Calibration By: Mr. Worachat Hongkaew

Calibration Date: 17 March 2022

The Method used: In house method, base on by comparison with standard

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through N.M. Technical Center Laboratory (NTL)
Certificate No.: TC21/0075



(Mr. Worachat Hongkaew)

Person in charge

SERT
บริษัท เอสพีซี อาร์ที จำกัด
SPC RT Co., Ltd.



(Mr. Udon Srichana)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SPC RT Co., Ltd.


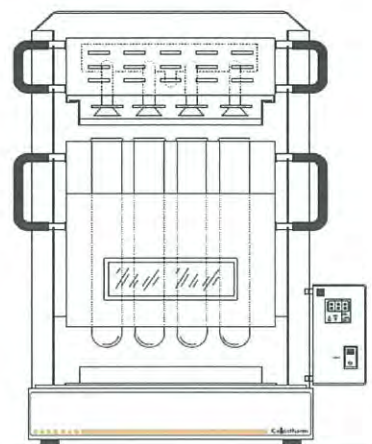


Fig. 1.: Front view

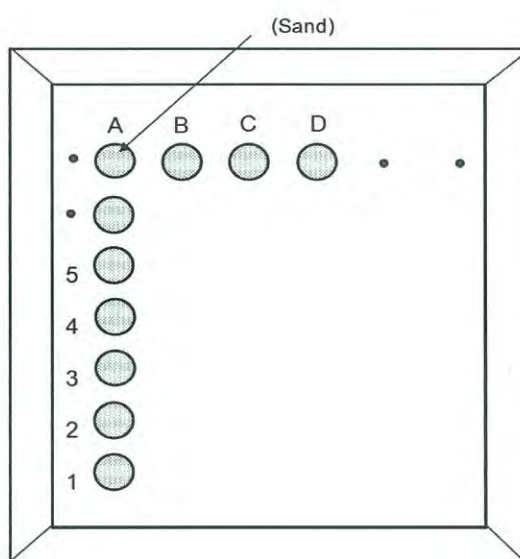

Location of standard

Fig. 2.: Digestion block

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the Digestion block.

Measured Temperature: The average reading of working standard at any positions or location.

Certificate No.: C29220011

Page: 3 of 3

Calibration Results:
Without adjustment

Locations	Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
A1	380	380	380	378.6	-1.4	1.5
A2				382.2	2.2	1.5
A3				380.2	0.2	1.5
A4				381.5	1.5	1.5
A5				381.2	1.2	1.5
B1				378.8	-1.2	1.5
B2				381.8	1.8	1.5
B3				379.4	-0.6	1.5
B4				382.1	2.1	1.5
B5				380.9	0.9	1.5
C1				378.2	-1.8	1.5
C2				380.0	0.0	1.5
C3				377.4	-2.6	1.5
C4				381.8	1.8	1.5
C5				382.3	2.3	1.5
D1				379.7	-0.3	1.5
D2				378.3	-1.7	1.5
D3				378.8	-1.2	1.5
D4				379.0	-1.0	1.5
D5				379.4	-0.6	1.5

The End of Certificate

ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: KSPR2203623

ชนิดเครื่องมือ: Block Digestion Unit รุ่น: KT-20s
หมายเลขเครื่อง: 5720210009/5770200073

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
17 Mar 2022			17 Mar 2022		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. สายไฟ	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. การทำงาน Main Switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. การทำงาน Selector Key	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. การแสดงผล Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. สภาพ Hole	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	6. สภาพฝาปิด	<input type="checkbox"/>	<input type="checkbox"/>	ไม่มี
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. สภาพตัวเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. สภาวะแวดล้อม ณ สถานที่ตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

ข้อแนะนำ :

Mr. Worachat Hongkaew
Service Engineer



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484




Cert.No.: 21CH1733

Page.: 1 of 3

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	SevenExcellence
Serial No. :	B834291445
ID No. :	RYG_EN0152
Condition As-Received:	Used Item
Received Date :	22 December 2021
Calibration Date :	23 December 2021
Reference :	2112-0636DSC-2
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer

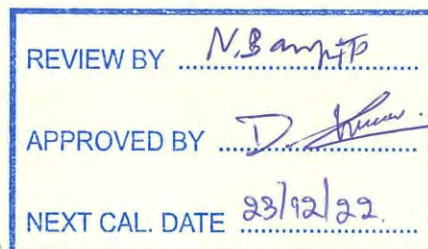

Calibrated by : Warakorn Lernagtrakul

Approved by :

Malee Butkruea

Approved Signatory

- (☒) Malee Butkruea
() Saithip Meangmai
() Warakorn Lernagtrakul

Issue Date : 24 December 2021

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0036356



Cert.No.: 21CH1733

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	21E2682	25 Aug 2022
2) Ref. Standard Thermometer	4982054	110RC044	21I1201	26 Oct 2022

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	761016	02 Aug 2023
pH 6.982	CPA chem	761017	02 Aug 2022
pH 10.015	CPA chem	761018	02 Aug 2022

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results**Function : mV Measurement****Performing standard curve by Fluke at pH (4,7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: B834291445	4.000	177.48	177.3	4.000	0.058	2.00
	7.000	0.00	-0.1	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Mahu



Cert.No.: 21CH1733

Page.: 3 of 3

Calibration Results**Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (\pm)	Coverage factor k
pH Electrode S/N.: 1475518	4.008	4.011	180.6	0.0049	2.05
	6.982	6.984	5.3	0.0077	2.00
	10.015	10.014	-171.3	0.0065	2.00

Function : Temperature Measurement**(*) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : InLab Expert Pro-ISM
- Serial No. : 1475518

Dimension of probe;

- Length : 120 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point ($^{\circ}\text{C}$)	Standard Temperature ($^{\circ}\text{C}$)	UUC* Reading ($^{\circ}\text{C}$)	Error ($^{\circ}\text{C}$)	Uncertainty of measurement (\pm $^{\circ}\text{C}$)	Coverage factor k
25.0	25.002	24.9	-0.102	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Malu



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 21E4151

Page : 1 of 2

Equipment : pH Meter
Manufacturer: Mettler Toledo
Model : SevenExcellence
Serial No.: B834291445
ID No.: RYG_EN0152
Condition As-Received: Used Item
Received Date: 22 December 2021
Calibration Date: 28 December 2021

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Reference: 2112-0636DSC
Ambient Temperature: (23 \pm 2) °C
Relative Humidity: (50 \pm 10) %
Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong
21140, Thailand

Procedure used: Calibration were conducted using In-house calibration Procedure CP-E17 According to direct measurement method with Multi-Product Calibrator.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Multi-Product Calibrator	5500A	6440007	21E1444	07 May 2022

2.This result of calibration was made on requested at the point specified by customer.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Wutchareeporn Wongchutikrane
Issue Date : 07 January 2022

Approved Signatory :

☒ Phalinee Prabpaipal

☐ Nuntawat Khamchai

☐ Pornthippa Tameyakul

B 0278122



Cert. No.: 21E4151

Page.: 2 of 2

Result of calibration :- (*) Without adjustment () After adjustment

Function:	DC voltage measurement		Range:	2000	mV	
	<u>Standard Value</u>		<u>UUC* Reading</u>		<u>Error</u>	<u>Uncertainty</u>
	(mV)		(mV)		(mV)	($\pm \mu V$)
	-100.0000		-100.0		0.0	65
	-50.0000		-50.0		0.0	62
	0.0000		0.0		0.0	58
	50.0000		50.0		0.0	62
	100.0000		100.0		0.0	65
	150.0000		150.0		0.0	69
	200.0000		199.9		-0.1	72

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %

*UUC= Unit Under Calibration.

-o0o-

92

a 1088610

REVIEW BY

Nont Somb

APPROVED BY

KL AL

NEXT CAL. DATE

21/12/23

Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID: GM-7
Organization Name: ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location: 104 Patthanakarn 40, Patthanakarn rd., Khwang Suan Luang, Khet Suan Luang, Bangkok 10250
Date: June 21, 2022 2:04:12 PM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.50, GCMS.02.50
Overall Qualification Status: Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Setpoint Status: Pass

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	25.0	psi
Accuracy:			0.0	psi
Agilent Recommended:			<= 1.2	

Overall Inlet Pressure Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name: 7890

Date: June 21, 2022 2:04:12 PM
System ID: GM-7

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

230.0

230.0

°C

Accuracy:

0.0

°C

Agilent Recommended:

>=

-1.0

% setpoint in K

(

-5.0

°C

)

<=

1.0

% setpoint in K

(

5.0

°C

)

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

100.0

100.4

°C

Accuracy:

0.4

°C

Agilent Recommended:

>=

-1.0

% setpoint in K

(

-3.7

°C

)

<=

1.0

% setpoint in K

(

3.7

°C

)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:

7890

Setpoint Status:

Pass

Setpoint/Average

Temperature:

100.0

100.0333

°C

Stability:

0.1

°C

Agilent Recommended:

<=

0.5

Overall GC Oven Temperature Stability Test Status

Pass

Log Amp

Tested Combination1

Front

SSL

/ External

SQ

Name:

5977A

Setpoint Status:

Pass

Date:

June 21, 2022 2:04:12 PM

System ID:

GM-7

Overall Log Amp Test Status

Pass

RFPA

Tested Combination1

Front

SSL

/ External

SQ

Name:

5977A

Setpoint Status:

Pass

Amu:

1050

m/z

Drift After Five Minutes:

22

mV

RFPA Voltage:

568

mV

Agilent Recommended:

>=

-100

and

<=

100

<=

1100

Overall RFPA Test Status

Pass

Tune EI

Tested Combination1

Front

SSL

/ External

SQ

Name:

5977A

Setpoint Status:

Pass

Filament:

1

Setpoint Status:

Pass

Filament:

2

Overall Tune EI Test Status

Pass

Signal to Noise EI

Tested Combination1

Front

SSL

/ External

SQ

Name:

5977A

Date:

June 21, 2022 2:04:12 PM

System ID:

GM-7

Source: Filament:

Setpoint Status:

Signal to Noise:

Agilent Recommended:

Source: Filament:

Setpoint Status:

Signal to Noise:

Agilent Recommended:

This test's 0 comment(s) and 1 deviation(s) are available in the Attachments section.

Overall Signal to Noise EI Test Status

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GM-7
Manufacturer	Agilent Technologies
Name	7890

Tested Combination1

Injection Technique	Manual Injection
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3442B
Serial Number	CN14133181
Firmware Revision	B.02.03
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5977A
Serial Number	US1415M209
Firmware Revision	5977 6.00.21
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Extractor
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Supasak Nimsongtham
Logged On User Name:	supasak.nimsongtham@agilent.com
Signature Creation Date:	June 21, 2022
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Date:	June 21, 2022 2:04:12 PM
System ID:	GM-7

User Name: supasak.nimsongtham
 Hostname: 5CG1115HKC

System Id: GM-7
 Print Date: June 21, 2022 2:04:17 PM

ALS-GM7-2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 21, 2022 10:25:05 AM	Audit	SessionCreated	Session	None
June 21, 2022 10:25:05 AM	Start	Configuration	Session	None
June 21, 2022 10:25:05 AM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
June 21, 2022 10:25:26 AM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.50/Gc.02.50.eqp], EQP File Name: [Gc.02.50.eqp], EQP Name: [AgilentRecommended] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.50/GcMs.02.50.eqp], EQP File Name: [GcMs.02.50.eqp], EQP Name: [AgilentRecommended]
June 21, 2022 10:25:39 AM	End	Configuration	Session	None
June 21, 2022 10:25:43 AM	Start	Qualification	Session	OQ
June 21, 2022 10:25:43 AM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
June 21, 2022 10:25:54 AM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1

User Name: supasak.nimsongtham
 Hostname: 5CG1115HKC

System Id: GM-7
 Print Date: June 21, 2022 2:04:17 PM

ALS-GM7-2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 21, 2022 10:26:00 AM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
June 21, 2022 10:26:10 AM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
June 21, 2022 10:26:12 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
June 21, 2022 10:34:09 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
June 21, 2022 10:34:10 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
June 21, 2022 10:34:11 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
June 21, 2022 10:38:42 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
June 21, 2022 10:38:44 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
June 21, 2022 10:38:46 AM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None

Page 2 / 8

Date: June 21, 2022 2:04:12 PM
 System ID: GM-7

User Name: supasak.nimsongtham
 Hostname: 5CG1115HKC

System Id: GM-7
 Print Date: June 21, 2022 2:04:17 PM

ALS-GM7-2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 21, 2022 11:01:00 AM	Audit	AceClosed	Session	None
June 21, 2022 11:01:47 AM	Audit	AceRestarted	Session	None
June 21, 2022 11:01:48 AM	Audit	SessionReloaded	Session	None
June 21, 2022 11:01:51 AM	Start	Qualification	Session	OQ
June 21, 2022 11:01:51 AM	Start	Execution	GC Oven Temperature Stability	None
			- 7890: - Temperature : Oven -	
			S: 100.0°C - L: <= 0.5°C	
June 21, 2022 11:03:14 AM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over.
June 21, 2022 11:04:19 AM	Audit	Data	GC Oven Temperature Stability	Manual Data Entry
			- 7890: - Temperature : Oven -	
			S: 100.0°C - L: <= 0.5°C	
June 21, 2022 11:04:22 AM	End	Execution	GC Oven Temperature Stability	Run Count : 1
			- 7890: - Temperature : Oven -	
			S: 100.0°C - L: <= 0.5°C	
June 21, 2022 11:04:24 AM	Start	Execution	Log Amp - 5977A SQ: - Source:	None
			EI - Extractor	
June 21, 2022 11:04:34 AM	End	Execution	Log Amp - 5977A SQ: - Source:	Run Count : 1
			EI - Extractor	
June 21, 2022 11:04:37 AM	Start	Execution	RFPA - 5977A SQ: - Source:	EI None
			- Extractor	
June 21, 2022 11:07:49 AM	End	Execution	RFPA - 5977A SQ: - Source:	EI Run Count : 1
			- Extractor	
June 21, 2022 11:07:52 AM	Start	Execution	Tune EI - 5977A SQ: - Source: -	None
			EI - Extractor Filament 1	
			(Qualitative - No setpoints associated)	

User Name: supasak.nimsongtham
 Hostname: 5CG1115HKC

System Id: GM-7
 Print Date: June 21, 2022 2:04:17 PM

ALS-GM7-2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 21, 2022 11:08:35 AM	End	Execution	Tune EI - 5977A SQ: - Source: - Run Count : 1 EI - Extractor Filament 1 (Qualitative - No setpoints associated)	
June 21, 2022 11:14:59 AM	Start	Execution	Tune EI - 5977A SQ: - Source: - None EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
June 21, 2022 11:16:48 AM	End	Execution	Tune EI - 5977A SQ: - Source: - Run Count : 1 EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
June 21, 2022 11:16:49 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
June 21, 2022 11:17:05 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
June 21, 2022 11:17:10 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
June 21, 2022 11:26:09 AM	Audit	AceClosed	Session	None
June 21, 2022 12:36:20 PM	Audit	AceRestarted	Session	None
June 21, 2022 12:36:22 PM	Audit	SessionReloaded	Session	None
June 21, 2022 12:36:26 PM	Start	Qualification	Session	OQ
June 21, 2022 12:36:26 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None

Page 4 / 8

User Name: supasak.nimsongtham
 Hostname: 5CG1115HKC

System Id: GM-7
 Print Date: June 21, 2022 2:04:17 PM

ALS-GM7-2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 21, 2022 12:37:07 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
June 21, 2022 12:37:08 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
June 21, 2022 12:38:54 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : H:\ALSGM7_2022\SNF1_001.D
June 21, 2022 12:39:24 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : H:\ALSGM7_2022\SNF1_001.D
June 21, 2022 12:40:09 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : H:\ALSGM7_2022\SNF1_001.D
June 21, 2022 12:42:04 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : H:\ALSGM7_2022\SNF1_001.D
June 21, 2022 12:42:17 PM	Audit	AceClosed	Session	None
June 21, 2022 12:33:31 PM	Audit	AceRestarted	Session	None
June 21, 2022 12:33:33 PM	Audit	SessionReloaded	Session	None
June 21, 2022 12:33:37 PM	Start	Qualification	Session	OQ
June 21, 2022 12:33:37 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None

User Name: supasak.nimsongtham
 Hostname: 5CG1115HKC

System Id: GM-7
 Print Date: June 21, 2022 2:04:17 PM

ALS-GM7-2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 21, 2022 12:34:44 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : E:\ALSGM7_2022\SNF1_001.D
June 21, 2022 12:36:26 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 1
June 21, 2022 12:37:11 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
June 21, 2022 12:38:15 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : E:\ALSGM7_2022\SNF2_001.D
June 21, 2022 12:38:30 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : E:\ALSGM7_2022\SNF2_001.D
June 21, 2022 12:38:45 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : E:\ALSGM7_2022\SNF2_001.D
June 21, 2022 12:39:00 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : E:\ALSGM7_2022\SNF2_001.D
June 21, 2022 12:39:14 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : E:\ALSGM7_2022\SNF2_001.D

User Name: supasak.nimsongtham
 Hostname: 5CG1115HKC

System Id: GM-7
 Print Date: June 21, 2022 2:04:17 PM

ALS-GM7-2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 21, 2022 12:39:45 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : E:\ALSGM7_2022\SNF2_001.D
June 21, 2022 12:40:16 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : E:\ALSGM7_2022\SNF2_001.D
June 21, 2022 12:40:40 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : E:\ALSGM7_2022\SNF2_001.D
June 21, 2022 12:41:09 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : E:\ALSGM7_2022\SNF2_001.D
June 21, 2022 12:41:29 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 1
June 21, 2022 12:42:30 PM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 1
June 21, 2022 12:42:30 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
June 21, 2022 12:42:35 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : E:\ALSGM7_2022\SNF2_001.D

User Name: supasak.nimsongtham
Hostname: 5CG1115HKC

System Id: GM-7
Print Date: June 21, 2022 2:04:17 PM

ALS-GM7-2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 21, 2022 12:42:45 PM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 2
June 21, 2022 12:42:50 PM	End	Qualification	Session	QQ
June 21, 2022 12:42:50 PM	Start	Reporting	Session	None
June 21, 2022 12:45:17 PM	Audit	AceClosed	Session	None
June 21, 2022 1:57:47 PM	Audit	AceRestarted	Session	None
June 21, 2022 1:57:50 PM	Audit	SessionReloaded	Session	None
June 21, 2022 1:57:56 PM	Start	Qualification	Session	QQ
June 21, 2022 2:02:42 PM	Audit	Reporting	Session	Report Generated : Certificate

REVIEW BY Nant SotAPPROVED BY LL ALNEXT CAL. DATE 25/05/23**Certificate of System Qualification**

GC-OQ + GCMS-OQ

System ID: GM-6
Organization Name: ALS Laboratory Group(Thailand) Co., Ltd.
Organization Location: 104 Patthanakarn 40, Patthanakarn Rd., Kwang Suan Luang< Khet Suan Luang, Bangkok 10250
Date: November 25, 2021 5:20:10 PM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.52, GCMS.02.51
Overall Qualification Status: Pass

CDS Logon Verification - GCLogon: Nanthawadee.Somboon**Overall CDS Logon Verification - GC Test Status**Pass**System Inspection and Basic Safety and Operation**Name: 7890Setpoint Status: Pass**Overall System Inspection and Basic Safety and Operation Test Status**Pass**Inlet Pressure Accuracy**Name: 7890Front SSLSetpoint Status: Pass

	Setpoint	Actual
Inlet Pressure:	<u>25.0</u> psi	<u>25.1</u> psi
Accuracy:		<u>0.1</u> psi
Agilent Recommended:	<u><=</u>	<u>1.2</u>

Date: November 25, 2021 5:20:10 PM
System ID: GM-6

Overall Inlet Pressure Accuracy Test Status

Pass

Headspace Leak

Name:

7697A with Tray

Sampler 1

Setpoint Status:

Pass

Overall Headspace Leak Test Status

Pass

Headspace Heated Zones Temperature Accuracy

Name:

7697A with Tray

Sampler 1

Setpoint Status:

Pass

Zone:

Transferline

Temperature:

Setpoint

115.0

°C

Actual

114.9

Accuracy:

-0.1

°C

Agilent Recommended:

>=

-1.8

% setpoint

(

-2.1

°C

)

<=

5.2

% setpoint

(

6.0

°C

)

Setpoint Status:

Pass

Zone:

Sample Loop

Temperature:

Setpoint

110.0

°C

Actual

109.8

Accuracy:

-0.2

°C

Agilent Recommended:

>=

-4.0

<=

4.0

Setpoint Status:

Pass

Zone:

Oven

Temperature:

Setpoint	100.0	°C
Actual	99.9	

Accuracy:

-0.1 °C

Agilent Recommended:

>=	-4.0
<=	4.0

Overall Headspace Heated Zones Temperature Accuracy Test

Pass

GC Oven Temperature Accuracy

Name:

7890

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:	230.0	229.8	°C
--------------	-------	-------	----

Accuracy:

-0.2 °C

Agilent Recommended:

>=	-1.0	% setpoint in K	(-5.0	°C)
<=	1.0	% setpoint in K	(5.0	°C)

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:	100.0	99.8	°C
--------------	-------	------	----

Accuracy:

-0.2 °C

Agilent Recommended:

>=	-1.0	% setpoint in K	(-3.7	°C)
<=	1.0	% setpoint in K	(3.7	°C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:

7890

Date:

November 25, 2021 5:20:10 PM

System ID:

GM-6

Setpoint Status:

Pass

Setpoint/Average

Temperature:

100.0 99.8 °C

Stability:

0.2 °C

Agilent Recommended:

<= 0.5

Overall GC Oven Temperature Stability Test Status

Pass

Log Amp

Tested Combination1

Front

SSL

/ External

SQ

Name:

5975C inert XL with TAD

Setpoint Status:

Pass

Overall Log Amp Test Status

Pass

RFPA

Tested Combination1

Front

SSL

/ External

SQ

Name:

5975C inert XL with TAD

Setpoint Status:

Pass

Amu: 1050 m/z

Drift After Five Minutes:

RFPA Voltage:

18 mV

519 mV

Agilent Recommended:

>= -100 and <= 100

<= 1100

Overall RFPA Test Status

Pass

Tune EI

Tested Combination1

Front

SSL

/ External

SQ

Name:

5975C inert XL with TAD

Setpoint Status:

Pass

Filament:

1

Date: November 25, 2021 5:20:10 PM

System ID: GM-6

Setpoint Status: Pass

Filament: 2

This test's 0 comment(s) and 1 deviation(s) are available in the Attachments section.

Overall Tune EI Test Status

Pass

Scouting Run

Tested Combination1	Front	SSL	/ External	SQ
Headspace				
Name:	7697A with Tray			
Source:	El - Inert			

Setpoint Status: Completed

Injection Volume on Column: 1000 uL

Overall Scouting Run Status

Completed

Injection Precision

Tested Combination1	Front	SSL	/ External	SQ
Name:	7697A with Tray			
Source:	El - Inert			

Setpoint Status: Pass

Injection Volume on Column: 1000 uL

Area RSD: 1.61 % Retention Time RSD: 0.01 %

Agilent Recommended: <= 5.00 <= 1.00

Overall Injection Precision Test Status

Pass

Mass Ratio Precision

Date: November 25, 2021 5:20:10 PM
System ID: GM-6

Tested Combination1	Front	SSL	/ External	SQ
Headspace				
Name:	7697A with Tray			
Source:	EI - Inert			
Setpoint Status:	Pass			
Injection Volume on Column:	1000	uL		
	Area Mass 1		Mass Ratio	
	Abundance*s			
RSD:	1.61	%	0.25	%
Agilent Recommended:	<= 5.00		<= 5.00	
	Pass		Pass	

Overall Mass Ratio Precision Test Status

Pass


Injection Carry Over

Tested Combination1	Front	SSL	/ External	SQ
Name:	7697A with Tray			
Source:	EI - Inert			
Setpoint Status:	Pass			
Injection Volume on Column:	1000	uL		
Area Carry Over:	0.00	%		
Agilent Recommended:	<= 1.00			

This test's 0 comment(s) and 2 deviation(s) are available in the Attachments section.

Overall Injection Carry Over Test Status

Pass

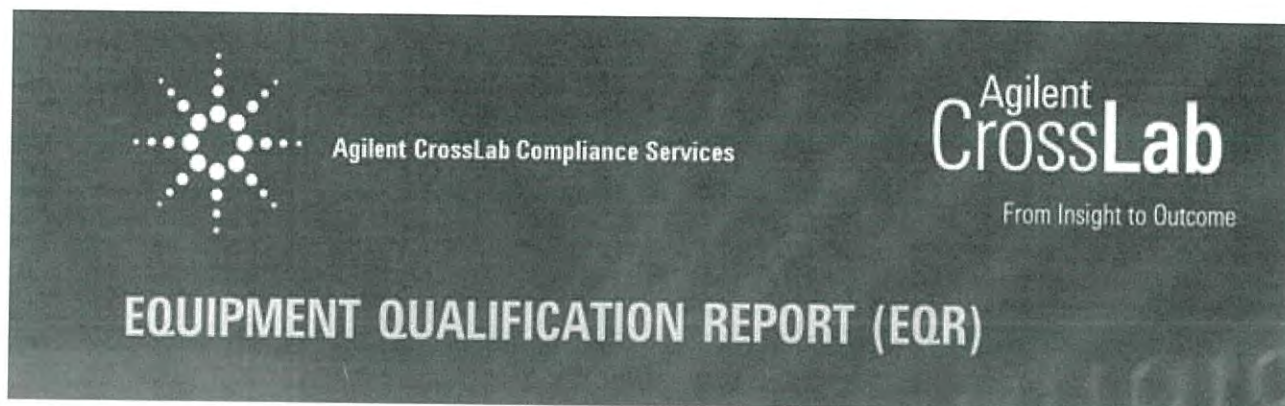

Agilent CrossLab Compliance

Qualification Type:	ICPMS-OQ
System ID:	JP15471169
EQP Name:	AgilentRecommended
EQP Revision:	ICPMS.02.50
EQP Publish Date:	March 2020
Date:	September 30, 2021 4:07:18 PM
Report Type:	Report
Org. Name:	ALS Laboratory Group (Thailand) Co.,Ltd.
Org. Location:	104 Phattanakarn 40, Suan Luang, Bangkok 10250.

REVIEW BY	Supakorn M.
APPROVED BY	Sauntan N.
NEXT CAL. DATE	29 March 2023

Date: September 30, 2021 4:07:18 PM
System ID: JP15471169

Table of Contents

Section	Page
Cover	1
Table of Contents	2
Test Summary	3
Service Details	4
Instrument Details	5
Calculation Formulas	7
Protocol Details	8
Tests	9
Autosampler Check : SPS4	9
Integrated Sample Introduction System (ISIS) Check : ISIS3	10
Autotune : G8403A	11
Background (No Gas Mode) : G8403A	13
Background (Gas Modes) : G8403A	14
20-Minute Stability (No Gas Mode) : G8403A	15
Declaration of Change Control	16
Attachments	17
Electronic Signature	31
Transaction Logs	32

Test Summary

Purpose

This section includes a status for each scheduled test and the overall qualification. For each test that is run, (1) the status is automatically determined based on pre-defined limits, and (2) the total number of times the test was run is displayed. For detailed results and specifications for a test, refer to the test results in this EQR.

Details

Test	Status	Runs
Autosampler Check : SPS4	Pass	1
Integrated Sample Introduction System (ISIS) Check : ISIS3	Pass	1
Autotune : G8403A	Pass	1
Background (No Gas Mode) : G8403A	Pass	1
Background (Gas Modes) : G8403A	Pass	1
20-Minute Stability (No Gas Mode) : G8403A	Pass	1

Overall Qualification Status

Pass

Service Details

Purpose

This section includes local contact and delivery details for this service.

General Details

Service Order No./Request: 6004837154
EQP Name: AgilentRecommended
EQP Revision: ICPMS.02.50
Report Type: Report

Organization Details

Name: ALS Laboratory Group (Thailand) Co.,Ltd.
Location: 104 Phattanakarn 40, Suan Luang, Bangkok 10250.

Local Contact Details

Name: Chatchanai Komarakul.
Job Title: Manager
Qualification Location: Laboratory

Operator Details

Name: Panthep Kurasathain
Job Title: Field Service Engineer.

Data Acquisition Details

Acquisition Software Name: MassHunter
Acquisition Software Revision: C.01.04

Customer Data System (CDS): IcpMs: MassHunter

Instrument Details

Purpose

This section describes the as found system configuration.

Details

ICP-MS 1

Manufacturer	Agilent Technologies
Name	7900
Model Number	G8403A
Installed Options	#100H: Standard Package with Hydrogen option
Detector Type	SQ
Nebulizer	Mira Mist (G3161)
Spray Chamber	Quartz
Torch	Quartz
Sampling Cone	Ni
Skimmer Cone	Ni
Serial Number	JP15471169
Firmware Revision	C.01.04

ISIS 1

Manufacturer	Agilent Technologies
Name	ISIS3
Model Number	G8411A
Type	Peristaltic pump system
Serial Number	JP15510227

Autosampler 1

Manufacturer	Agilent Technologies
Name	SPS4
Model Number	G8410A
Serial Number	AU15430722

Chiller 1

Manufacturer	Agilent Technologies
Name	Chiller
Model Number	G3292A
Serial Number	3U1610713

Calculation Formulas

Purpose

This section includes calculation formulas for all available tests. Depending upon which tests are scheduled, all or some apply to your qualification.

For a description of calculations for ICP-MS tests performed by the MassHunter software, refer to the MassHunter application and documentation.

Protocol Details

Purpose

This section lists the revisions for all test units used in this report. For complete test-specific and high-level change details, refer to the Revision History document.

Test Revision	Test
ICPMS.02.50	20-Minute Stability (No Gas Mode)
ICPMS.02.50	Autosampler Check
ICPMS.02.50	Autotune
ICPMS.02.50	Background (Gas Modes)
ICPMS.02.50	Background (No Gas Mode)
ICPMS.02.50	Integrated Sample Introduction System (ISIS) Check

Autosampler Check

Purpose

This test demonstrates that the autosampler module is correctly installed and connected. It does not test module performance.

Setpoint

Results

Criteria	Observed Result	Expected Result	Status
After the self test, is probe in the home position?	Yes	Yes	Pass
As commanded, is the probe positioned at vial 2?	Yes	Yes	Pass

Setpoint Status:

Pass

Runs: 1

Overall Autosampler Check Test Status

Pass

Integrated Sample Introduction System (ISIS) Check

Purpose

This test demonstrates that the ISIS module is correctly installed and connected. It does not test module performance.

Setpoint

Results

Criteria	Observed Result	Expected Result	Status
As commanded, does the pump rotate?	Yes	Yes	Pass
As commanded, do the valves load and inject?	Yes	Yes	Pass

Setpoint Status:

Pass

Runs: 1

Overall Integrated Sample Introduction System (ISIS) Check Test Status

Pass

Autotune

Purpose

This test uses traceable checkout standards to run a software-executed autotune in all modes. The tune report provides values for peak width, mass axis, sensitivity, oxide species, and doubly-charged species tests.

Setpoint

Results

Peakwidth Mass 7	0.719	AMU
Agilent Recommended:	>= 0.65	
	<= 0.80	
Status:	Pass	
Peakwidth Mass 89	0.750	AMU
Agilent Recommended:	>= 0.65	
	<= 0.80	
Status:	Pass	
Peakwidth Mass 205	0.713	AMU
Agilent Recommended:	>= 0.65	
	<= 0.80	
Status:	Pass	
Mass Axis 7	7.05	AMU
Agilent Recommended:	>= 6.9	
	<= 7.1	
Status:	Pass	
Mass Axis 89	88.95	AMU
Agilent Recommended:	>= 88.9	
	<= 89.1	
Status:	Pass	
Mass Axis 205	205.00	AMU
Agilent Recommended:	>= 204.9	
	<= 205.1	
Status:	Pass	

Mass 7 Sensitivity No Gas

94.28

Mcps/ppm

Agilent Recommended:

>=

25.5

Status:

Pass

Mass 89 Sensitivity No Gas

307.15

Mcps/ppm

Agilent Recommended:

>=

127.5

Status:

Pass

Mass 205 Sensitivity No Gas

203.77

Mcps/ppm

Agilent Recommended:

>=

76.5

Status:

Pass

Mass 59 Sensitivity He

28.38

Mcps/ppm

Agilent Recommended:

>=

23.8

Status:

Pass

Mass 89 Sensitivity H2

129.27

Mcps/ppm

Agilent Recommended:

>=

68

Status:

Pass

Oxide Ratio 156/140

1.047

%

Agilent Recommended:

<=

1.38

Status:

Pass

Doubly Charged Species Ratio 70/140

1.482

%

Agilent Recommended:

<=

2.3

Status:

Pass

Setpoint Status:

Pass

Runs: 1

Overall Autotune Test Status

Pass

Background (No Gas Mode)

Purpose

This test examines the background of the ICP-MS in no gas mode by monitoring ions during a blank run.

Setpoint

Conditions

Masses:	7	AMU
	89	AMU
	205	AMU

Measurements and Results

Masses (AMU):	7	89	205	
Measured Value:	3.200	3.300	9.900	cps
Agilent Recommended:	<= 6.9	<= 4.6	<= 11.5	
Status:	Pass	Pass	Pass	

Setpoint Status:	Pass	Runs:	1
------------------	------	-------	---

Overall Background (No Gas Mode) Test Status

Pass

Background (Gas Mode)

Purpose

This test examines the background of the ICP-MS in the various gas modes by monitoring ions during a blank run.

Setpoint Gas Mode: Helium

Conditions

Mass: 78 AMU
Integration Time: 1.0 sec
Cycles: 20

Measurements and Results

Mass (AMU): 78
Measured Value: 42.8500 cps
Agilent Recommended: ≤ 115
Status: Pass

Setpoint Status: Pass

Runs: 1

Setpoint Gas Mode: Hydrogen

Conditions

Mass: 78 AMU
Integration Time: 1.0 sec
Cycles: 20

Measurements and Results

Mass (AMU): 78
Measured Value: 2.1500 cps
Agilent Recommended: ≤ 4.6
Status: Pass

Setpoint Status: Pass

Runs: 1

Overall Background (Gas Mode) Test Status

Pass

20-Minute Stability (No Gas Mode)

Purpose

This test monitors the abundance of ions present in the checkout standard over a 20-minute period to verify that the signal is stable. The %RSD of the abundance of given ions is calculated internally by the software and compared to the limit.

Setpoint

Conditions

Mode:	Spectrum	
Masses:	7, 9, 59, 89, 140, 205	
Integration Time:	9.99	sec
Peak Pattern:	3	points/peak
Repetitions:	20	
Sweeps/Replicates:	100	

Measurements and Results

Masses (AMU):	7	89	205	
Stability RSD:	0.96400	0.51495	0.73011	%
Agilent Recommended:	<= 2.3	<= 2.3	<= 2.3	
Status:	Pass	Pass	Pass	

Setpoint Status:	Pass	Runs:	1
------------------	------	-------	---

Overall 20-Minute Stability (No Gas Mode) Test Status

Pass

Declaration of Change Control

This document is under change control. Revision history is maintained and printed on each document. Access to the master documents is limited to process owners. Documents receive periodic review and cannot be assigned an evergreen status. The qualification performed according to this document refers only to the hardware/software configuration in place at the time of the qualification. Agilent Technologies recommends that instrument configuration change management procedures be in place in order to maintain the validation process. Any changes to the analytical or computer hardware or software must be clearly specified. A change management system provides a means for determining the degree of requalification required according to the extent of the changes made. All details of the changes must be thoroughly recorded and documented, together with details of completed tests and their results. Note: Hardware/software configuration management is the customer's responsibility.

Attachments

Training requirements note: The delivery engineer attaches an ACE technique-specific training certificate to the Equipment Qualification Report (EQR). Obtaining ACE technique-specific certification includes pre-requisite trainings for Data Integrity, General Compliance topics (GMP, GLP, ALCOA, etc.), instrument hardware and software components, and the ACE technique itself. The one certificate encompasses all pre-requisite trainings as documented in the Agilent Learning Management System called Success Factors.

Location	Category	Document Name	Page
EQR	General	Certificate of System Qualification	18
EQR	General	Operator's training certificate and qualifications	19
EQR	General	Certificate of Qualification for ACE	20
EQR	General	Certificate of Qualification for ACE	21
EQR	General	Tune reports	22
EQR	General	Test Report	25
EQR	General	Test Report	27
EQR	General	Test Report	29

General

Document Name: Certificate of System Qualification



Agilent Technologies

Agilent Compliance Engine Self Qualification

Date: September 14, 2021 4:59:15 PM

Drive Serial #: ACA025C9

Platform Revision:

ACE 3.11

Individual self-qualification reports for each specific technique installed are also available upon request. They provide additional details on the general report from the concise summary and are structured by the actual algorithms challenged during the process. There is not a one-to-one relationship between algorithms and OQ program tests because some algorithms are used by several tests and across multiple similar hardware components of the qualified systems.

Technique Type	Tests Completed	Result
Atomic Absorption	7	Conforms
Capillary Electrophoresis	10	Conforms
Dissolution	6	Conforms
Emission Spectroscopy	3	Conforms
Gas Chromatography - GCMS	17	Conforms
Gas Chromatography	29	Conforms
Gel Permeation Chromatography	9	Conforms
ICP-MS	6	Conforms
Infrared Spectroscopy	7	Conforms
Liquid Chromatography	17	Conforms
Liquid Chromatography - LCMS	8	Conforms
Microfluidics	18	Conforms
Sample Preparation - Gas Chromatography	9	Conforms
Sample Preparation - Liquid Chromatography	8	Conforms
Supercritical Fluid Chromatography	15	Conforms
Software	6	Conforms
UV-Vis Spectrophotometer	13	Conforms

Overall Qualification Status

Conforms

Date: September 30, 2021 4:07:18 PM
System ID: JP15471169

General

Document Name: Operator's training certificate and qualifications



Certificate of Completion

Learner Name: Panthep Kurasathain

Title Of Course: AN-CE-ICPMS-2-038-A:Agilent 7900 ICPMS FSE update training

Completion Date: June 7, 2014

Certified By Company: Learning at Agilent

All Service and Support training certificates have the following specific limitations.

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's: Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.

General

Document Name:

Certificate of Qualification for ACE



Certificate of Completion

Learner Name: Panthep Kurasathain

Title Of Course: AN-CE-SS-II-030-A: ACE 3.X User Update Training

Completion Date: July 7, 2020

Certified By Company: Learning at Agilent

All Service and Support training certificates have the following specific limitations.

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's: Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.

General

Document Name:

Certificate of Qualification for ACE



Certificate of Completion

Learner Name: Panthep Kurasathain

Title Of Course: AN-CE-ICPMS-2-035-B: CrossLab Compliance Hardware Specific Delivery for Agilent ICP-MS Systems

Completion Date: October 31, 2020

Certified By Company: Learning at Agilent

All Service and Support training certificates have the following specific limitations.

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's: Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.

General


Document Name: Tune reports

Tune Report

Operator Name Supakwan Mak
 Acq/Data Batch C:\Agilent\ICPMS\11\UserTune_7900.b
 Acq. Date-Time 2021-09-30 14:44:08
 Report Comment OQ 30 Sep 2021
 Instrument Name GB403A JP15471169

[No Gas]

Sensitivity

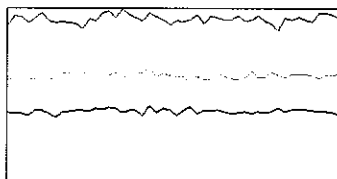


Mass	Range	Count	RSD%	Background
7	10000	9428	2.630	3.200
89	50000	30716	2.825	3.300
205	60000	20377	3.319	9.900

Sampling Period [sec] 0.311
 Integration Time [sec] 0.1

Oxide/Doubly Charged Ratio

Oxide 156 / 140 1.047 %
 Doubly Charged 70 / 140 1.482 %

Resolution/Axis

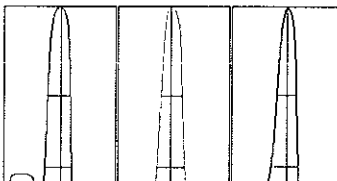

Mass	Peak Height	Axis	W-50%	W-10%
7	9474.89	7.05	0.62	0.719
89	30716.43	88.95	0.59	0.750
205	20596.12	205.00	0.52	0.713

Integration Time [sec] 0.1
 Acquisition Time [sec] 22.74
 Y Axis Linear

Tune Parameters

Plasma Parameters

Plasma Mode	---	Nebulizer Gas	1.00 L/min	Makeup Gas	0.10 L/min
RF Power	1550 W	Option Gas	---	Auxiliary Gas	0.90 L/min
RF Matching	1.10 V	Nebulizer Pump	0.10 rps	Plasma Gas	15.0 L/min
Sample Depth	9.0 mm	S/C Temp	2 °C		

Lens Parameters

Extract 1	0.0 V	Omega Lens	9.1 V	Deflect	13.6 V
Extract 2	-205.0 V	Cell Entrance	-30 V	Plate Bias	-35 V
Omega Bias	-90 V	Cell Exit	-50 V		

Cell Parameters

Use Gas	No	3rd Gas Flow	---	Energy Discrimination	5.0 V
He Flow	0.0 mL/min	OctP Bias	-8.0 V		

Document Name:

Tune reports

Tune Report

H2 Flow 0.0 mL/min

OctP RF 190 V

QP Parameters

Mass Gain 124

Axis Gain 0.9990

QP Bias -3.0 V

Mass Offset 125

Axis Offset 0.01

Hardware Settings

Torch

Torch H -0.3 mm

Torch V 0.1 mm

EM


Discriminator 4.0 mV

Analog HV 2247 V

Pulse HV 1318 V

[H2]

Sensitivity

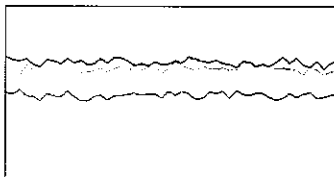

Mass	Range	Count	RSD%	Background
59	5000	2453	3.423	0.400
89	20000	12927	2.822	0.200
205	20000	13635	2.445	8.701

Sampling Period [sec] 0.31

Integration Time [sec] 0.1

Oxide/Doubly Charged Ratio

Oxide 156 / 140 0.804 %

Doubly Charged 70 / 140 1.020 %

Tune Parameters

Plasma Parameters

Plasma Mode ---

Nebulizer Gas 1.00 L/min

Makeup Gas 0.10 L/min

RF Power 1550 W

Option Gas ---

Auxiliary Gas 0.90 L/min

RF Matching 1.10 V

Nebulizer Pump 0.10 rps

Plasma Gas 15.0 L/min

Sample Depth 9.0 mm

S/C Temp 2 °C

Lens Parameters

Extract 1 0.0 V

Omega Lens 9.0 V

Deflect 6.0 V

Extract 2 -210.0 V

Cell Entrance -30 V

Plate Bias -100 V

Omega Bias -105 V

Cell Exit -90 V

Cell Parameters

Use Gas Yes

3rd Gas Flow ---

Energy Discrimination 3.5 V

He Flow 0.0 mL/min

OctP Bias -22.0 V

H2 Flow 5.0 mL/min

OctP RF 200 V

QP Parameters

Mass Gain 124

Axis Gain 0.9990

QP Bias -18.5 V

Mass Offset 125

Axis Offset 0.01

Hardware Settings

Torch

Torch H -0.3 mm

Torch V 0.1 mm

2 of 3

2021-09-30 2:44 PM

Document Name:

Tune reports

Tune Report

EM

Discriminator

4.0 mV

Analog HV


2247 V

Pulse HV

1318 V

[He]

Sensitivity

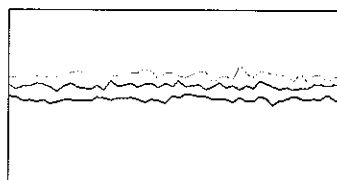

Mass	Range	Count	RSD%	Background
59	5000	2838	2.592	6.000
89	5000	3149	3.359	5.200
205	20000	9837	2.895	4.201

Sampling Period [sec] 0.31

Integration Time [sec] 0.1

Oxide/Doubly Charged Ratio

Oxide 156 / 140 0.498 %

Doubly Charged 70 / 140 0.788 %

Tune Parameters

Plasma Parameters

Plasma Mode	---	Nebulizer Gas	1.00 L/min	Makeup Gas	0.10 L/min
RF Power	1550 W	Option Gas	---	Auxiliary Gas	0.90 L/min
RF Matching	1.10 V	Nebulizer Pump	0.10 rps	Plasma Gas	15.0 L/min
Sample Depth	9.0 mm	S/C Temp	2 °C		

Lens Parameters

Extract 1	0.0 V	Omega Lens	9.2 V	Deflect	12.4 V
Extract 2	-225.0 V	Cell Entrance	-30 V	Plate Bias	-100 V
Omega Bias	-105 V	Cell Exit	-50 V		

Cell Parameters

Use Gas	Yes	3rd Gas Flow	---	Energy Discrimination	3.5 V
He Flow	3.8 mL/min	OctP Bias	-8.0 V		
H2 Flow	0.0 mL/min	OctP RF	200 V		

QP Parameters

Mass Gain	124	Axis Gain	0.9990	QP Bias	-4.5 V
Mass Offset	125	Axis Offset	0.01		

Hardware Settings

Torch

Torch H	-0.3 mm	Torch V	0.1 mm
---------	---------	---------	--------

EM

Discriminator

4.0 mV

Analog HV

2247 V

Pulse HV

1318 V

General

Document Name: Test Report

Batch Summary Report

Batch Folder: C:\Batch2021\BG He.b\
Analysis File: BG He.batch.bin
Tune Step: #1 He

	Rjct	Acq. Date-Time	Data File	Sample Name	Type	Level	Dilution
1		2021-09-30 14:21:47	BG He.d	BG He	Sample		1.0000

Document Name:

Test Report

Batch Summary Report

Analyte Table

		78 [He1]
	Sample Name	CPS
1	BG He	42.8500

Page 2 / 2

2021-09-30 14:23:40

General

Document Name: Test Report

Batch Summary Report

Batch Folder: D:\Agilent Service\CQ 30 Sep 2021\BG H2 new.b\
Analysis File: BG H2 new.batch.bin
Tune Step: #1 H2

	Rict	Acq. Date-Time	Data File	Sample Name	Type	Level	Dilution
1		2021-09-30 15:08:58	BG H2.d	BG H2	Sample		1.0000

Document Name:

Test Report

Batch Summary Report

Analyte Table

		78 [H2]
	Sample Name	CPS
1	BG H2	2.1500

General

Document Name:

Test Report

Batch Summary Report

Batch Folder: D:\Agilent Service\OQ 30 Sep 2021\20 Min.b\
Analysis File: 20 Min.batch.bin
Tune Step: #1 No Gas

	Rect	Acq. Date-Time	Data File	Sample Name	Type	Level	Dilution
1		2021-09-30 15:17:44	20 Min.d	20 Min	Sample		1.0000

Document Name:

Test Report

Batch Summary Report

Analyte Table

		7 [No Gas]	9 [No Gas]	59 [No Gas]	89 [No Gas]	140 [No Gas]	205 [No Gas]
Sample Name		CPS RSD	CPS RSD	CPS RSD	CPS RSD	CPS RSD	CPS RSD
1	20 Min	0.96400	7.02464	0.46857	0.51495	0.61014	0.73011

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Panthep Kurasathain
Logged On User Name:	panthep_kurasathain@agilent.com
Signature Creation Date:	September 30, 2021
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: panthep_kurasathain
 Hostname: ASBKKWX315

System Id: JP15471169
 Print Date: September 30, 2021 4:07:22 PM

ALS OQHW 7900 30Sep21 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
September 30, 2021 3:50:07 PM	Audit	SessionCreated	Session	None
September 30, 2021 3:50:07 PM	Start	Configuration	Session	None
September 30, 2021 3:50:07 PM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
September 30, 2021 3:52:52 PM	Audit	EqpLoaded	Session	EQP details for primary technique [lcpMs] - File path: [ProtocolPacks/lcpMs/Configurations/02.50/lcpMs.02.50.eqp], EQP File Name: [lcpMs.02.50.eqp], EQP Name: [AgilentRecommended]
September 30, 2021 3:52:54 PM	End	Configuration	Session	None
September 30, 2021 3:52:57 PM	Start	Qualification	Session	OQ
September 30, 2021 3:52:57 PM	Start	Execution	Autosampler Check : SPS4: Autosampler Check	None
September 30, 2021 3:53:03 PM	End	Execution	Autosampler Check : SPS4: Autosampler Check	Run Count : 1
September 30, 2021 3:53:04 PM	Start	Execution	Integrated Sample Introduction System (ISIS) Check : ISIS3: Integrated Sample Introduction System (ISIS) Check	None
September 30, 2021 3:53:08 PM	End	Execution	Integrated Sample Introduction System (ISIS) Check : ISIS3: Integrated Sample Introduction System (ISIS) Check	Run Count : 1

User Name: panthep_kurasathain
 Hostname: ASBKWX315

System Id: JP15471169
 Print Date: September 30, 2021 4:07:22 PM

ALS OQHW 7900 30Sep21 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
September 30, 2021 3:53:10 PM	Start	Execution	Autotune : G8403A: Autotune 1	None
September 30, 2021 3:55:08 PM	End	Execution	Autotune : G8403A: Autotune 1	Run Count : 1
September 30, 2021 3:55:12 PM	Start	Execution	Background (No Gas Mode) : G8403A: No Gas Mode Background 1	None
September 30, 2021 3:55:40 PM	End	Execution	Background (No Gas Mode) : G8403A: No Gas Mode Background 1	Run Count : 1
September 30, 2021 3:55:43 PM	Start	Execution	Background (Gas Modes) : G8403A: Gas Mode Background :Helium	None
September 30, 2021 3:56:17 PM	End	Execution	Background (Gas Modes) : G8403A: Gas Mode Background :Helium	Run Count : 1
September 30, 2021 3:56:19 PM	Start	Execution	Background (Gas Modes) : G8403A: Gas Mode Background :Hydrogen	None
September 30, 2021 3:56:38 PM	End	Execution	Background (Gas Modes) : G8403A: Gas Mode Background :Hydrogen	Run Count : 1
September 30, 2021 3:56:41 PM	Start	Execution	20-Minute Stability (No Gas Mode) : G8403A: 20-Minute Stability (No Gas Mode) 1	None
September 30, 2021 3:57:22 PM	End	Execution	20-Minute Stability (No Gas Mode) : G8403A: 20-Minute Stability (No Gas Mode) 1	Run Count : 1
September 30, 2021 3:57:24 PM	End	Qualification	Session	OQ
September 30, 2021 3:57:24 PM	Start	Reporting	Session	None

User Name: panthep_kurasathain
Hostname: ASBKKWX315

System Id: JP15471169
Print Date: September 30, 2021 4:07:22 PM

ALS OQHW 7900 30Sep21 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
September 30, 2021 4:03:07 PM	Audit	Reporting	Session	Report Generated : Certificate
September 30, 2021 4:03:17 PM	Audit	Reporting	Session	Report Generated : Report
September 30, 2021 4:03:59 PM	Start	Qualification	Session	OQ
September 30, 2021 4:04:08 PM	End	Qualification	Session	OQ
September 30, 2021 4:04:08 PM	Start	Reporting	Session	None
September 30, 2021 4:04:26 PM	Audit	Reporting	Session	Report Generated : Certificate
September 30, 2021 4:04:36 PM	Audit	Reporting	Session	Report Generated : Report

Certificate No. T220730

Page 1 of 6

Certificate of Calibration

Equipment : HEATING BLOCK

Manufacturer : Environmental Express

Model : SC 196

Serial No. : 6974CECW3285

Customer Code : BKK_EL0054


ID No. : T5306A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250

Customer Location : Acid Digestion Lab

Date of Receipt : 30 March 2022

Calibrated By : Watcharapon Sangtong (Technician)

Approved By :  / Sujjar Naknakred (Site Calibration Manager)

Date of Issue : 12 APR 2022

REVIEW BY	Tattaporn C.
APPROVED BY	Sangtong N.
NEXT CAL. DATE	7/10/23

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T220730

Page 2 of 6

Calibration Report

Equipment : HEATING BLOCK
Date of Calibration : 7 April 2022
Environment : Temperature : 21.8-23.1 °C
Line Voltage : 221.6-226.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN221-TN230	T210008	08 June 2022
TC	TYPE T	TN231-TN240	T210008	08 June 2022
DATA LOGGER	34970A	T149	T210008	08 June 2022

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good


Equipment Description :

Time Constant 2 Hour 25 Minute At 95 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

() without adjustment

(X) after adjustment

Approved By. 



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109


Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T220730

Page 3 of 6

Calibration Report

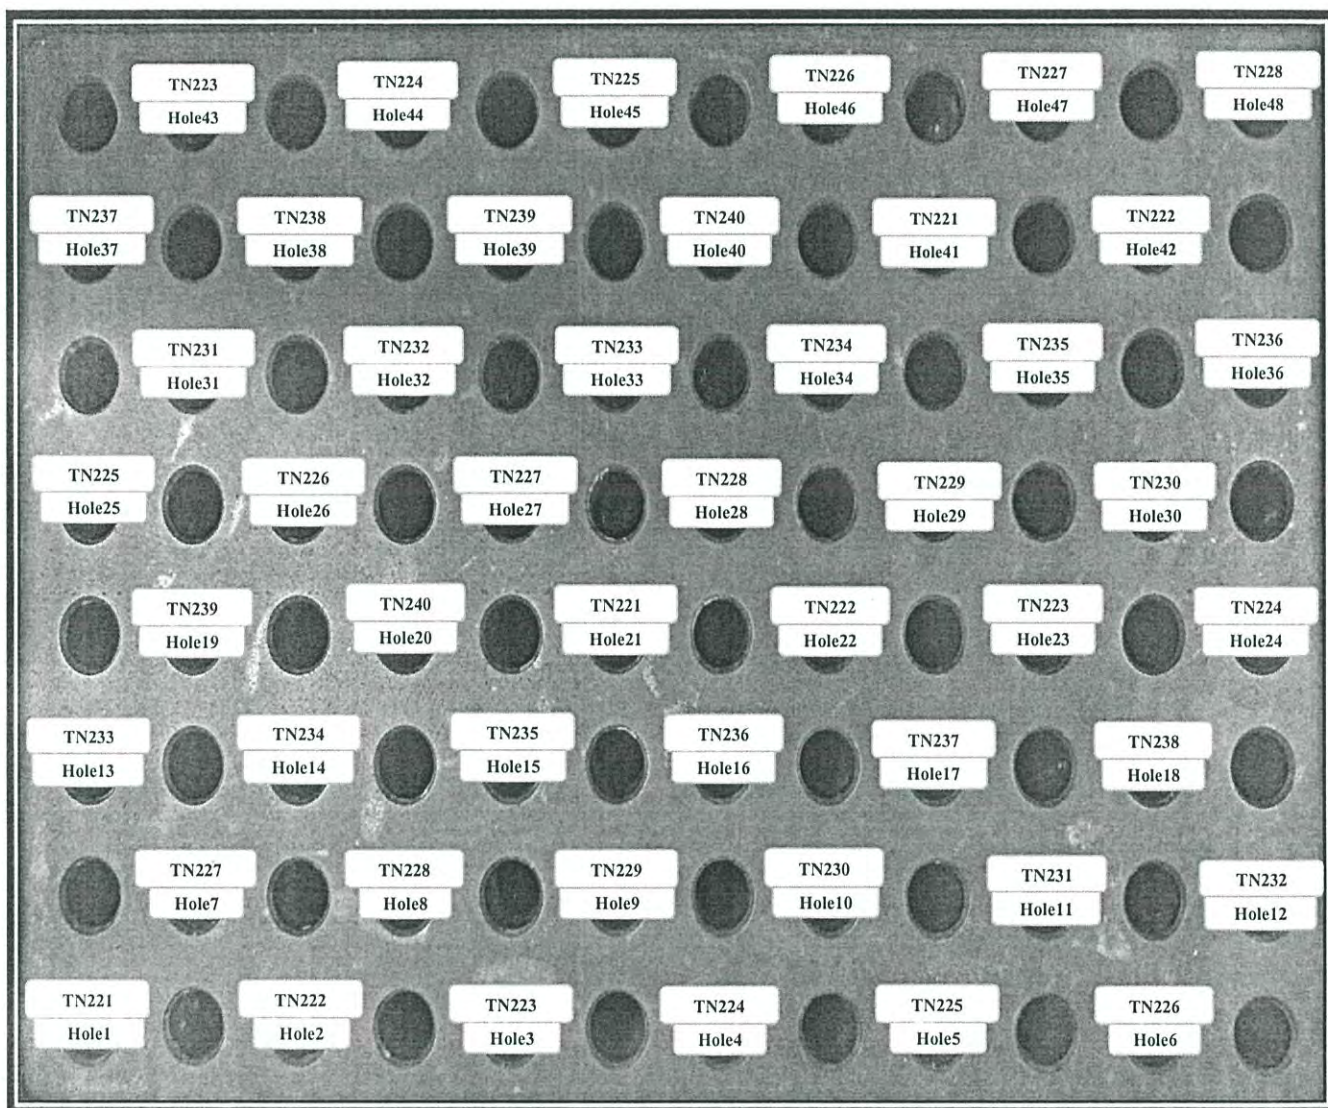

FRONT CONTROL

Approved By. _____

Certificate No. **T220730**

Page **4 of 6**

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (° C)					
R1 Hole1-Hole6		TN221	TN222	TN223	TN224	TN225	TN226
CAL POINT	Max	93.60	93.82	94.05	94.20	94.36	94.26
95	Min	93.07	93.26	93.51	93.66	93.82	93.71
	Average	93.33	93.54	93.78	93.93	94.09	93.98
R2 Hole7-Hole12		TN227	TN228	TN229	TN230	TN231	TN232
	Max	94.59	94.79	94.63	94.55	94.82	95.00
	Min	94.05	94.25	94.08	93.97	94.26	94.44
	Average	94.32	94.52	94.36	94.26	94.54	94.72
R3 Hole13-Hole18		TN233	TN234	TN235	TN236	TN237	TN238
	Max	95.03	94.54	94.78	94.84	95.06	94.73
	Min	94.46	93.98	94.20	94.28	94.49	94.18
	Average	94.74	94.26	94.49	94.56	94.78	94.45
R4 Hole19-Hole24		TN239	TN240	TN221	TN222	TN223	TN224
	Max	94.89	94.82	95.73	95.85	95.73	96.10
	Min	94.33	94.26	95.51	95.62	95.51	95.85
	Average	94.61	94.54	95.62	95.73	95.62	95.97
R5 Hole25-Hole30		TN225	TN226	TN227	TN228	TN229	TN230
	Max	96.28	96.39	96.37	96.54	96.19	96.04
	Min	96.01	96.10	96.02	96.20	95.89	95.71
	Average	96.15	96.24	96.20	96.37	96.04	95.88
R6 Hole31-Hole36		TN231	TN232	TN233	TN234	TN235	TN236
	Max	96.84	96.97	97.03	96.48	96.33	95.76
	Min	96.53	96.65	96.71	96.08	95.98	95.43
	Average	96.68	96.81	96.87	96.28	96.16	95.60
R7 Hole37-Hole42		TN237	TN238	TN239	TN240	TN221	TN222
	Max	96.46	96.15	96.19	96.06	96.95	97.09
	Min	96.13	95.84	95.85	95.72	96.64	96.78
	Average	96.30	95.99	96.02	95.89	96.80	96.93
R8 Hole43-Hole48		TN223	TN224	TN225	TN226	TN227	TN228
	Max	96.91	96.58	96.13	96.19	96.34	96.19
	Min	96.55	96.21	95.80	95.87	96.03	95.88
	Average	96.73	96.40	95.96	96.03	96.18	96.03

Approved By. _____



Certificate No. **T220730**

Page **5 of 6**

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (° C)					
R1 Hole1-Hole6		TN221	TN222	TN223	TN224	TN225	TN226
CAL POINT	Max	104.47	104.65	104.79	105.31	105.47	105.46
105	Min	104.15	104.27	104.45	104.98	105.14	105.20
	Average	104.31	104.46	104.62	105.15	105.31	105.33
R2 Hole7-Hole12		TN227	TN228	TN229	TN230	TN231	TN232
	Max	105.55	105.73	105.65	105.84	105.97	106.07
	Min	105.28	105.43	105.35	105.52	105.68	105.83
	Average	105.42	105.58	105.50	105.68	105.82	105.95
R3 Hole13-Hole18		TN233	TN234	TN235	TN236	TN237	TN238
	Max	106.14	106.06	105.81	106.05	105.81	105.87
	Min	105.85	105.81	105.55	105.80	105.53	105.64
	Average	106.00	105.94	105.68	105.92	105.67	105.75
R4 Hole19-Hole24		TN239	TN240	TN221	TN222	TN223	TN224
	Max	105.86	105.60	104.44	104.51	104.28	104.78
	Min	105.61	105.37	104.27	104.35	104.12	104.61
	Average	105.74	105.48	104.35	104.43	104.20	104.69
R5 Hole25-Hole30		TN225	TN226	TN227	TN228	TN229	TN230
	Max	104.94	104.93	104.97	105.08	104.68	104.69
	Min	104.77	104.75	104.76	104.90	104.51	104.49
	Average	104.85	104.84	104.86	104.99	104.60	104.59
R6 Hole31-Hole36		TN231	TN232	TN233	TN234	TN235	TN236
	Max	105.44	105.45	105.61	104.95	104.84	104.42
	Min	105.27	105.27	105.44	104.76	104.66	104.25
	Average	105.36	105.36	105.53	104.86	104.75	104.33
R7 Hole37-Hole42		TN237	TN238	TN239	TN240	TN221	TN222
	Max	105.17	104.70	104.59	104.51	105.22	105.53
	Min	105.00	104.53	104.41	104.35	105.04	105.37
	Average	105.08	104.62	104.50	104.43	105.13	105.45
R8 Hole43-Hole48		TN223	TN224	TN225	TN226	TN227	TN228
	Max	105.61	105.45	105.10	104.77	104.87	105.02
	Min	105.44	105.28	104.92	104.60	104.70	104.85
	Average	105.53	105.37	105.01	104.69	104.79	104.93

Approved By. _____



Certificate No. T220730

Page 5 of 6

Calibration Report

Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (\pm °C)	Uncertainty (\pm °C)
	Min , Max	Average		
100.0	100.0 , 100.4	100.1	0.29	0.83
105.0	105.0 , 105.4	105.1	0.20	0.79

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

 Approved By. 



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th



Certificate No. T221644

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Cold Room)

Manufacturer : KOLDTECH

Model : KM 320

Serial No. : TBN-1012061/05

Customer Code : BKK_EN0167

ID No. : T2463A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250



Customer Location : Environmental Laboratory

Date of Receipt : 27 June 2022

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 04 JUL 2022

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	30/12/23


The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T221644

Page 3 of 4

Calibration Report

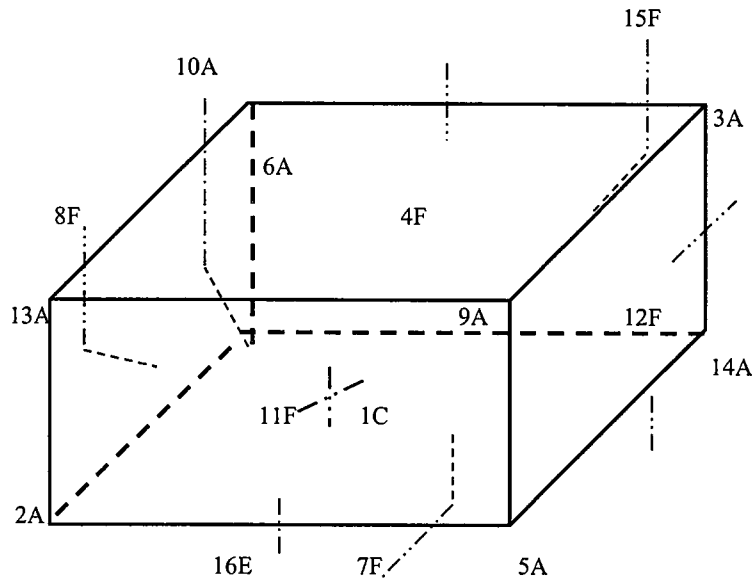

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN161
2A	=	TN162
3A	=	TN163
4F	=	TN164
5A	=	TN165
6A	=	TN166
7F	=	TN167
8F	=	TN168
9A	=	TN169
10A	=	TN170

11F	=	TN171
12F	=	TN172
13A	=	TN173
14A	=	TN174
15F	=	TN175
16E	=	TN176

Approved By. 

Certificate No. T221644

Page 4 of 4

Calibration Report

Measurement Results:

Average Standard Reading at each position (°C)										
Calibration Point	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170
3	2.71	2.82	2.75	2.89	2.95	3.68	3.02	2.96	3.03	2.85
	TN171	TN172	TN173	TN174	TN175	TN176				
	2.97	3.02	2.89	3.04	2.97	3.33				

Chamber (Cold Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage
	Min , Max	Average					Factor <i>k</i>
3.0	2.9 , 4.0	3.2	2.99	1.05	1.30	1.66	2.00

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CHO30

Page.: 1 of 3

Certificate of Calibration

Equipment : Spectrophotometer

Manufacturer : HACH

Model : DR3900

Serial No. : 2021559

ID No. : BKK_EN0356

Condition As-Received: Used Item

Received Date : 21 January 2022

Calibration Date : 21 January 2022

Reference : 2201-0616OC-4

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Calibration Place : Wet Chemistry Lab 2

Ambient Temperature : (22.8 - 22.3) °C (On-Site)

Relative Humidity : (60.3 - 61.8) % (On-Site)

Calibration Procedure : In - house method :
CP-OCH4 based on ASTM E 275-01

Calibrated by : Kunchit Promprat

Approved by :

Malee

Approved Signatory

(☒) Malee Butkruea

(☐) Saithip Meangmai

(☐) Warakorn Lerngagtrakul

Issue Date : 3 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0037380



Cert. No. : 22CHO30

Page : 2 of 3

Condition of calibration result

1. Reference Standard Material :

<u>Material</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1. Absorbance Standard set	8331	86623	08 Sep 2022
2. Wavelength Standard set	14536	89302	19 Jan 2023
3. Wavelength Standard set	14537	89303	19 Jan 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit maintained at :

- National Physical Laboratory (NPL), The United Kingdom of Great Britain and Northern Ireland
- National Institute of Standards and Technology (NIST), The United States of America

4. Spectral BandWidth : 5 nm

Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (\pm nm)	Coverage Factor <i>k</i>
418.40	418	0.59	2.00
479.88	479	0.59	2.00
513.75	513	0.59	2.00
537.00	536	0.59	2.00
638.00	638	0.59	2.00
747.61	748	0.59	2.00
807.04	807	0.59	2.00

Malu .



Cert. No. : 22CHO30

Page : 3 of 3

Calibration Results : without adjustment**Photometric Accuracy**

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (\pm Abs)	Coverage Factor <i>k</i>
420.0	Zero	0.000	0.0028	2.00
	0.5723	0.570	0.0033	2.00
	0.7522	0.750	0.0031	2.00
	1.0907	1.089	0.0032	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5616	0.559	0.0034	2.00
	0.7345	0.731	0.0032	2.00
	1.0646	1.062	0.0033	2.00
465.0	Zero	0.000	0.0028	2.00
	0.5118	0.513	0.0034	2.00
	0.6773	0.678	0.0031	2.00
	0.9809	0.983	0.0033	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5228	0.522	0.0030	2.00
	0.6861	0.684	0.0030	2.00
	0.9941	0.994	0.0030	2.00
590.0	Zero	0.000	0.0028	2.00
	0.5546	0.553	0.0029	2.00
	0.7159	0.713	0.0030	2.00
	1.0369	1.034	0.0030	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5401	0.539	0.0029	2.00
	0.6835	0.681	0.0029	2.00
	0.9889	0.987	0.0030	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

Malu

-o0o-

Certificate of System Qualification

ES-OQ

System ID: MY16010005
Organization Name: ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location: 104 Phatthanakan 40 Phatthanakan Rd., Bangkok 10250

Date: September 13, 2021 5:49:11 PM
EQP Name: AgilentRecommended
EQP Revision: ES.02.50
Overall Qualification Status: Pass

Preparation

Pass

Instrument Tests

Pass

Autosampler Operation

Pass

REVIEW BY	Thitima B.
APPROVED BY	Savitree N.
NEXT CAL. DATE	12 Mar 23

Date: September 13, 2021 5:49:11 PM
System ID: MY16010005