

# ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือ

ตรวจวัดคุณภาพสิ่งแวดล้อม

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
<b>คุณภาพอากาศในบรรยากาศ</b>		
Total Suspended Particulate (TSP)	High Volume Air Sampler No. R01, R17, R18	Digital Balance
Particulate Matter less than 10 microns (PM-10)	High Volume PM-10 Air Sampler No. R03, R05, R06	Digital Balance
Nitrogen Dioxide (NO <sub>2</sub> )	NO <sub>2</sub> Analyzer No. R02, R04, R07	NO <sub>2</sub> Analyzer No. R02, R04, R07
<b>คุณภาพอากาศจากปล่องระบาย</b>		
Total Suspended Particulate	Console No. R02 Pitot Tube No. B48	Digital Balance
Oxides of Nitrogen	Vacuum Gauge	Spectrophotometer
Hydrogen Chloride	Personal Pump SKC No. B66 Rotameter No. H-B06	IC
Hydrogen Fluoride	Personal Pump SKC No. B66 Rotameter No. H-B06	IC
<b>คุณภาพอากาศในสถานประกอบการ</b>		
Total Dust	Personal Pump SKC No. B32, B48, B51, R17, R23, R24, R32, R36 Rotameter No. H-R02	Digital Balance
Respirable Dust	Personal Pump SKC No. B29, B57, B77, R08, R14, R30, R43 Rotameter No. H-R02	Digital Balance
Aluminum Fume	Personal Pump SKC No. R08, R17, R43 Rotameter No. H-R02	ICP
Hydrogen Chloride	Personal Pump SKC No. B57 Rotameter No. L- R02	IC
Hydrogen Fluoride	Personal Pump SKC No. R14 Rotameter No. L- R02	IC
Ammonia	Personal Pump SKC No. R15 Rotameter No. L- R02	IC
<b>ระดับเสียงในบรรยากาศ</b>		
L <sub>eq</sub> 24 hr, L <sub>max</sub> , L <sub>90</sub> และเสียงรบกวน	Acoustic Calibrator Sound Level Meter : ACO-R05, R21, R22, R31, R32	-

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม (ต่อ)

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
ระดับเสียงในสถานประกอบการ $L_{eq}$ 8 hr และ $L_{max}$	Acoustic Calibrator Sound Level Meter : ACO-B29, B36, B41, B43, R50 Sound Level Meter : NL 21-B01	-
TWA	Sound Level Meter : NMD-R02, R03, R05, R06, R13	
คุณภาพน้ำทิ้ง		
pH	-	pH Meter
Total Dissolved Solids	-	Digital Balance
Total Suspended Solids	-	Digital Balance
BOD <sub>5</sub>	-	BOD Analyzer
COD	-	COD Reactor
Grease & Oil	-	Digital Balance
Total Aluminum	-	ICP
ระดับความร้อนในสถานประกอบการ WBGT	Digital Thermometer Heat Meter No. R14, R15, R16	-

คุณภาพอากาศในบรรยากาศ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

## High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

### Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
B35	B35	03/11/2022	y = 1.306x-9.466	0.997
B36	B36	02/11/2022	y = 1.213x-5.932	0.996
B37	B37	01/11/2022	y = 1.253x-5.209	0.999
B38	B38	01/11/2022	y = 1.228x-5.530	0.995
B39	B39	01/11/2022	y = 1.319x-9.149	0.998
B40	B40	01/11/2022	y = 1.196x-4.045	0.999
B41	B41	07/11/2022	y = 1.179x-2.611	0.999
B42	B42	01/11/2022	y = 1.209x-3.713	0.995
B43	B43	02/11/2022	y = 1.187x-3.331	0.998
B44	B44	07/11/2022	y = 1.298x-8.171	0.996
R01	R01	02/11/2022	y = 1.289x-8.287	0.998
R02	R02	07/11/2022	y = 1.307x-10.165	0.999
R03	R03	03/11/2022	y = 1.259x-7.634	0.995
R04	R04	04/11/2022	y = 1.157x-2.287	0.995
R05	R05	03/11/2022	y = 1.273x-8.311	0.999
R06	R06	01/11/2022	y = 1.297x-8.271	0.999
R07	R07	02/11/2022	y = 1.071x+1.468	0.995
R08	R08	01/11/2022	y = 1.206x-5.068	0.997
R09	R09	01/11/2022	y = 1.252x-7.084	0.995
R10	R10	03/11/2022	y = 1.246x-5.817	0.999
R11	R11	03/11/2022	y = 1.117x-1.156	0.998
R12	R12	02/11/2022	y = 1.351x-12.068	0.996
R13	R13	03/11/2022	y = 1.118x-0.601	0.999
R14	R14	03/11/2022	y = 1.164x-2.415	0.996
R15	R15	03/11/2022	y = 1.134x-1.793	0.998
R16	R16	04/11/2022	y = 1.182x-4.717	0.996
R17	R17	07/11/2022	y = 1.218x-5.356	0.998
R18	R18	04/11/2022	y = 1.233x-5.977	0.996
R19	R19	07/11/2022	y = 1.277x-7.752	0.997
R20	R20	04/11/2022	y = 1.327x-10.628	0.997

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Mr. Peera Detudom  
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

#### Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate ( $\text{m}^3/\text{min}$ )	$R^2$
R01	R01	02/11/2022	$y = 1.257x - 6.210$	0.998
R02	R02	07/11/2022	$y = 1.240x - 5.054$	0.996
R03	R03	03/11/2022	$y = 1.199x - 4.666$	0.996
R04	R04	04/11/2022	$y = 1.215x - 6.193$	0.999
R05	R05	04/11/2022	$y = 1.210x - 5.386$	0.998
R06	R06	02/11/2022	$y = 1.270x - 6.263$	0.995
R07	R07	07/11/2022	$y = 1.227x - 5.259$	0.998
R08	R08	03/11/2022	$y = 1.258x - 7.271$	0.998
R09	R09	07/11/2022	$y = 1.202x - 6.317$	0.999
R10	R10	03/11/2022	$y = 1.196x - 4.622$	0.997
R11	R11	02/11/2022	$y = 1.284x - 7.142$	0.996
R12	R12	02/11/2022	$y = 1.253x - 7.460$	0.996
R13	R13	04/11/2022	$y = 1.262x - 6.240$	0.998
R14	R14	04/11/2022	$y = 1.254x - 6.659$	0.999
R15	R15	03/11/2022	$y = 1.299x - 9.065$	0.998
R16	R16	09/11/2022	$y = 1.263x - 7.053$	0.995
R17	R17	07/11/2022	$y = 1.224x - 4.966$	0.997
R18	R18	07/11/2022	$y = 1.235x - 5.907$	0.999
R19	R19	03/11/2022	$y = 1.302x - 9.454$	0.995
R20	R20	04/11/2022	$y = 1.244x - 8.211$	0.999

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## CALIBRATION REPORT

### CHEMILUMINESCENT NO / NO<sub>2</sub> / NO<sub>x</sub> ANALYZER

DATE : 21 November 2022

BRAND : API

MODEL : 200E

NO. NOX-R02

SERIAL NO. 2285

#### Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 04 August 2022

Serial No. : 911

#### Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : D636192

Certified Date : 20 April 2022

Expired Date : 20 April 2024

Cylinder Conc. : 49.1 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.5 °C

% RH 48

#### CALIBRATION SETTING

Span	Initial Reading (Before Adj.), PPB			Final Reading (After Adj.), PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.5	-0.125	400.0	0.998
NO <sub>x</sub> Span	400	399.8	-0.050	400.0	1.003

#### API Model 200E NO<sub>x</sub> Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	509	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	103.1	mV	-20 - 150
AZERO	93.9	mV	-20 - 150
HVPS	669	V	420 - 900 constant
RCELL TEMP	50.0	°C	50 ± 1
BOX TEMP	28.8	°C	8 - 48
PMT TEMP	7.2	°C	7 ± 2
MOLY TEMP	315.3	°C	315 ± 5
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000
NO Slope	0.998	-	1.0 ± 0.3
NO <sub>x</sub> Slope	1.003	-	1.0 ± 0.3
NO Offset	1.0	mV	-20 to +150
NO <sub>x</sub> Offset	0.6	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by : Adul Dangklom  
(Mr. Adul Dangklom)

Approved by : Mr. Peera Detudom  
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	21 November 2022	BRAND :	API	MODEL :	200E
NO.	NOX-R04	SERIAL NO.	4411		
Calibrator (Dilution System)					
Brand	: API			Model	: 700
Last Cal. Date	: 04 August 2022			Serial No.	: 911
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: D636192
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024	Cylinder Conc.	: 49.1 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH	48				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.010
NO <sub>x</sub> Span	400	400.3	0.075	400.0	1.014
API Model 200E NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	513	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	102.9	mV	-20 - 150		
AZERO	93.7	mV	-20 - 150		
HVPS	674	V	420 - 900 constant		
RCELL TEMP	50.4	°C	50 ± 1		
BOX TEMP	29.2	°C	8 - 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	315.1	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000		
NO Slope	1.010	-	1.0 ± 0.3		
NO <sub>x</sub> Slope	1.014	-	1.0 ± 0.3		
NO Offset	1.6	mV	-20 to +150		
NO <sub>x</sub> Offset	1.0	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

Adul Dangklom  
(Mr.Adul Dangklom)

Approved by :

Peera Detudom  
(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

## CALIBRATION REPORT

### CHEMILUMINESCENT NO / NO<sub>2</sub> / NO<sub>x</sub> ANALYZER

DATE : 21 November 2022

BRAND : API

MODEL : 200E

NO. NOX-R07

SERIAL NO. 4468

#### Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 04 August 2022

Serial No. : 911

#### Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : D636192

Certified Date : 20 April 2022

Expired Date : 20 April 2024

Cylinder Conc. : 49.1 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.5 °C

% RH 48

#### CALIBRATION SETTING

Span	Initial Reading (Before Adj.), PPB			Final Reading (After Adj.), PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	399.8	-0.050	400.0	1.005
NO <sub>x</sub> Span	400	400.1	0.025	400.0	1.009

#### API Model 200E NO<sub>x</sub> Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	506	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	103.2	mV	-20 - 150
AZERO	94.1	mV	-20 - 150
HVPS	672	V	420 - 900 constant
RCELL TEMP	50.1	°C	50 ± 1
BOX TEMP	29.4	°C	8 - 48
PMT TEMP	7.3	°C	7 ± 2
MOLY TEMP	314.8	°C	315 ± 5
RCELL PRESS	8.2	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000
NO Slope	1.005	-	1.0 ± 0.3
NO <sub>x</sub> Slope	1.009	-	1.0 ± 0.3
NO Offset	1.4	mV	-20 to +150
NO <sub>x</sub> Offset	0.9	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 22M2567

REFERENCE No : 64386-1

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS 105DU

**SERIAL No** : 1126422905

**ID No** : BA 05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : TETNITHI W.

**CALIBRATION DATE** : 11-Mar-22

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 17-Mar-22

**RECEIVED DATE** : 11-Mar-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 22M2567

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	MODEL	:	XS 105DU
MANUFACTURER	:	METTLER TOLEDO	S/N	:	1126422905
ID No	:	BA 05/50	RECEIVED DATE	:	11-Mar-22
AIR PRESSURE	:	1008mbar $\pm$ 1mbar	CALIBRATION DATE	:	11-Mar-22
AMBIENT TEMPERATURE	:	22° C $\pm$ 1° C	RELATIVE HUMIDITY	:	49 %RH $\pm$ 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-


- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 20 g WAS 0.000004 g
4. REPEATABILITY OF READING AT 100 g WAS 0.000048 g
5. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000058
0.02	0.01999	0.00001	0.000058
0.10	0.09999	0.00001	0.000059
0.20	0.19999	0.00001	0.000059
0.50	0.50001	-0.00001	0.000058
1.00	1.00001	-0.00001	0.000059
2.00	2.00000	0.00000	0.000059
5.00	5.00001	-0.00001	0.000061
10.00	10.00005	-0.00005	0.000063
20.00	20.00006	-0.00006	0.000069
50.00	50.00000	0.00000	0.00011
100.00	100.00001	-0.00001	0.00019
120.00	120.00001	-0.00001	0.00022

6. OFF CENTER LOADING ERROR



POINT	READING (g)	
1	10.00001	50.0000
2	10.00002	50.0000
3	10.00001	50.0000
4	10.00001	50.0000
5	10.00002	50.00001
OFF-CENTER LOADING	0.00001	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT PRODUCTION AREA  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

คุณภาพอากาศจากปล่องระบาย



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## Console Calibration Report

Calibration Method

Critical Orifices

### Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	$\Delta H_{@}$ (mmH <sub>2</sub> O)
B01	1563	01/09/2022	1.004	50.11
B02	8002514	02/09/2022	1.006	49.25
B03	1503016	05/09/2022	1.008	50.30
B04	00006659	05/09/2022	1.005	47.45
B05	00007428	01/09/2022	1.002	49.96
R01	1561	02/09/2022	1.003	49.86
R02	8002513	05/09/2022	1.006	50.09
R03	1570	05/09/2022	1.004	49.23
R04	8002519	01/09/2022	1.005	49.17
R05	1503015	01/09/2022	0.996	49.68

Remark : Accept Value of y (test) is  $0.97 < y < 1.03$

Accept Value of  $\Delta H_{@}$  (test) is  $46.7 \pm 6.4$  (mmH<sub>2</sub>O)

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

### Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	02/11/2022	0.83	0.84
B37	S	0.99	01/11/2022	0.84	0.83
B38	S	0.99	02/11/2022	0.84	0.85
B39	S	0.99	04/11/2022	0.84	0.84
B40	S	0.99	02/11/2022	0.85	0.84
B41	S	0.99	02/11/2022	0.84	0.85
B44	S	0.99	02/11/2022	0.84	0.83
B45	S	0.99	01/11/2022	0.84	0.83
B46	S	0.99	01/11/2022	0.84	0.85
B47	S	0.99	03/11/2022	0.84	0.84
B48	S	0.99	03/11/2022	0.83	0.84
B49	S	0.99	04/11/2022	0.85	0.84
B54	S	0.99	01/11/2022	0.83	0.84
B56	S	0.99	01/11/2022	0.84	0.85
B57	S	0.99	04/11/2022	0.85	0.84
B58	S	0.99	04/11/2022	0.84	0.84

Remark : Accept value of Cp (test) is  $0.84 \pm 0.01$

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : VACUUM GAUGE  
MANUFACTURER : HI-LIGHT  
MODEL / TYPE : N/A  
SERIAL NO. : N/A[64-220066-1]  
CLID. NO. : 212201112  
JOB CONTROL NO. : 220720073201

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 20 July 2022

DATE OF ISSUED : 22 July 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
22 July 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22073201

F3-011-04/01-12

page 1 of 3



@clccalibration

## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : VACUUM GAUGE  
MANUFACTURER : HI-LIGHT  
MODEL / TYPE : N/A  
SERIAL NO. : N/A[64-220066-1]  
DATE OF CALIBRATION : 21 July 2022

---

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-05** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 744 S/N. 9226007 with Pressure Module Model 700PV4 S/N. 19298401.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).  
Certificate No. MP-0196-21, Due Date 17 November 2022.

#### UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of  $k = 2$ . It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. **Q22073201**

F3-011-04/01-12

page 2 of 3



@clccalibration

## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

### CALIBRATION DATA

#### CORRECTION OF PRESSURE

DUC Test point ( inHg )	STD Reading ( inHg )		Correction ( inHg )	
	Up	Down	Up	Down
0	0.0	0.0	0.0	0.0
-5	-4.6	-4.7	+0.4	+0.3
-10	-9.5	-9.6	+0.5	+0.4
-15	-14.4	-14.5	+0.6	+0.5
-20	-19.4	-19.5	+0.6	+0.5
-25	-24.5	-24.5	+0.5	+0.5
-30	-29.5	-29.5	+0.5	+0.5

Uncertainty of measurement  $\pm 0.2$  inHg

Transmitting fluid : Air.

Technical Note. k factor 1 kPa = 0.2952998 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 36 of 54

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q22073201

F3-011-04/01-12

page 3 of 3



@clccalibration



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
B41	SKC	224-PCXR4	612669	05/10/2022	1,000	1,500	2,000	998	1,496	1,990	0.994x + 3.271	1.000
B42	SKC	224-PCXR4	626041	06/10/2022	1,000	1,500	2,000	1,005	1,498	1,994	0.988x + 15.619	1.000
B43	SKC	224-PCXR4	034636	06/10/2022	1,000	1,500	2,000	999	1,501	1,992	0.991x + 10.565	1.000
B44	SKC	224-PCXR8	529341	06/10/2022	1,000	1,500	2,000	1,002	1,502	2,002	1.011x - 21.418	0.999
B45	SKC	224-PCXR8	529594	06/10/2022	1,000	1,500	2,000	998	1,498	1,989	0.993x + 5.959	1.000
B46	SKC	224-PCXR8	566743	06/10/2022	1,000	1,500	2,000	994	1,504	2,002	1.016x - 32.885	0.999
B47	SKC	224-PCXR8	566747	06/10/2022	1,000	1,500	2,000	1,002	1,500	2,004	1.013x - 24.960	0.999
B48	SKC	224-PCXR8	566753	03/10/2022	1,000	1,500	2,000	999	1,494	1,998	0.999x - 2.114	1.000
B49	SKC	224-PCXR8	566780	05/10/2022	1,000	1,500	2,000	1,003	1,502	2,003	1.012x - 22.706	0.999
B50	SKC	224-PCXR8	500400	06/10/2022	1,000	1,500	2,000	1,001	1,495	2,002	1.001x - 3.737	1.000
B51	SKC	224-PCXR8	500363	06/10/2022	1,000	1,500	2,000	995	1,504	1,999	1.011x - 25.590	0.999
B52	SKC	224-PCXR8	093186	03/10/2022	1,000	1,500	2,000	995	1,496	1,994	0.997x - 1.161	1.000
B53	SKC	224-PCXR8	707670	03/10/2022	1,000	1,500	2,000	1,002	1,500	2,002	1.010x - 20.668	0.999
B54	SKC	224-PCXR3	509821	03/10/2022	1,000	1,500	2,000	993	1,500	2,001	1.017x - 34.516	0.999
B55	SKC	224-PCXR3	510710	03/10/2022	1,000	1,500	2,000	999	1,494	1,994	0.995x + 2.521	1.000
B56	SKC	224-PCXR3	511450	03/10/2022	1,000	1,500	2,000	1,002	1,500	2,001	1.004x - 7.562	1.000
B57	SKC	224-PCXR3	510798	06/10/2022	1,000	1,500	2,000	997	1,492	1,998	0.996x +1.109	1.000
B58	SKC	224-PCXR3	509852	06/10/2022	1,000	1,500	2,000	1,000	1,498	1,999	1.007x - 19.113	0.999
B59	SKC	224-PCXR3	509862	03/10/2022	1,000	1,500	2,000	996	1,503	1,994	0.997x + 2.955	1.000
B60	SKC	224-PCXR3	512655	03/10/2022	1,000	1,500	2,000	1,005	1,500	2,003	1.010x - 19.862	0.999
B61	SKC	224-PCXR3	503915	04/10/2022	1,000	1,500	2,000	994	1,489	1,998	1.004x - 11.786	1.000
B62	SKC	224-PCXR3	505975	03/10/2022	1,000	1,500	2,000	999	1,494	1,996	0.997x - 0.064	1.000
B63	SKC	224-PCXR3	511432	03/10/2022	1,000	1,500	2,000	991	1,501	1,999	1.017x - 35.461	0.999
B64	SKC	224-PCXR3	508302	03/10/2022	1,000	1,500	2,000	997	1,492	1,989	0.992x + 6.266	1.000
B65	SKC	224-PCXR3	508310	06/10/2022	1,000	1,500	2,000	1,002	1,500	2,003	1.011x - 21.992	0.999
B66	SKC	224-PCXR3	509861	06/10/2022	1,000	1,500	2,000	1,002	1,491	1,991	0.988x + 13.904	1.000
B67	SKC	224-PCXR3	506295	06/10/2022	1,000	1,500	2,000	993	1,508	2,004	1.017x - 32.785	0.999
B68	SKC	224-PCXR3	505872	05/10/2022	1,000	1,500	2,000	1,002	1,491	1,997	0.994x + 5.237	1.000
B69	SKC	224-PCXR3	508375	05/10/2022	1,000	1,500	2,000	1,001	1,499	2,000	1.010x - 21.330	0.999
B70	SKC	224-PCXR3	510623	05/10/2022	1,000	1,500	2,000	992	1,503	1,997	1.002x - 6.054	1.000
B71	SKC	224-PCXR3	508367	05/10/2022	1,000	1,500	2,000	990	1,506	2,002	1.018x - 37.025	0.999
B72	SKC	224-PCXR3	505977	05/10/2022	1,000	1,500	2,000	1,001	1,498	1,993	0.993x + 5.731	1.000
B73	SKC	224-PCXR3	512606	05/10/2022	1,000	1,500	2,000	1,001	1,501	2,005	1.014x - 24.397	0.999
B74	SKC	224-PCXR3	505993	05/10/2022	1,000	1,500	2,000	996	1,495	1,994	0.999x - 4.284	1.000
B75	SKC	224-PCXR3	509820	05/10/2022	1,000	1,500	2,000	996	1,498	1,990	0.995x + 2.987	1.000
B76	SKC	224-PCXR3	509811	03/10/2022	1,000	1,500	2,000	993	1,498	1,998	1.006x - 14.003	1.000
B77	SKC	224-PCXR3	508301	06/10/2022	1,000	1,500	2,000	1,000	1,501	2,003	1.014x - 25.845	0.999
B78	SKC	224-PCXR3	510677	06/10/2022	1,000	1,500	2,000	996	1,503	1,999	1.012x - 27.321	0.999
B79	SKC	224-PCXR3	510920	06/10/2022	1,000	1,500	2,000	994	1,493	1,994	0.999x - 3.905	1.000

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
**S.P.S. CONSULTING SERVICE CO., LTD.**  
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
 Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
H-B01	Dwyer	VFB-65	05/10/2022	500	1,000	2,000	505.3	990.7	1975.7	0.990x + 8.856	1.000
H-B02	Dwyer	VFB-65	04/10/2022	500	1,000	2,000	495.7	997.8	1995.3	0.994x + 4.025	1.000
H-B03	Dwyer	VFB-65	04/10/2022	500	1,000	2,000	498.3	987.5	2010.2	1.004x - 14.483	0.999
H-B04	Dwyer	VFB-65	05/10/2022	500	1,000	2,000	501.2	999.9	2008.7	0.998x - 0.511	1.000
H-B05	Dwyer	VFB-65	05/10/2022	500	1,000	2,000	499.0	997.4	1972.3	0.987x + 14.507	1.000
H-B06	Dwyer	VFB-65	05/10/2022	500	1,000	2,000	503.9	993.4	1981.4	1.006x - 9.415	0.999
H-B07	Dwyer	VFB-65	05/10/2022	500	1,000	2,000	504.1	989.0	2018.3	1.002x - 2.255	1.000
H-B08	Dwyer	VFB-65	04/10/2022	500	1,000	2,000	499.8	999.2	1975.8	0.997x + 2.922	0.999
H-B09	Dwyer	VFB-65	06/10/2022	500	1,000	2,000	503.7	1006.6	2014.3	0.993x + 14.424	1.000
H-B10	Dwyer	VFB-65	06/10/2022	500	1,000	2,000	496.9	998.6	2012.4	0.998x + 1.450	1.000

Calibrated by :

*Adul Dangklom*

(Mr. Adul Dangklom)

Approved by :

*Peera Detudom*

(Mr. Peera Detudom)

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 22M2567

REFERENCE No : 64386-1

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS 105DU

**SERIAL No** : 1126422905

**ID No** : BA 05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : TETNITHI W.

**CALIBRATION DATE** : 11-Mar-22

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 17-Mar-22

**RECEIVED DATE** : 11-Mar-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 22M2567

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	MODEL	:	XS 105DU
MANUFACTURER	:	METTLER TOLEDO	S/N	:	1126422905
ID No	:	BA 05/50	RECEIVED DATE	:	11-Mar-22
AIR PRESSURE	:	1008mbar $\pm$ 1mbar	CALIBRATION DATE	:	11-Mar-22
AMBIENT TEMPERATURE	:	22° C $\pm$ 1° C	RELATIVE HUMIDITY	:	49 %RH $\pm$ 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-


- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 20 g WAS 0.000004 g
4. REPEATABILITY OF READING AT 100 g WAS 0.000048 g
5. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000058
0.02	0.01999	0.00001	0.000058
0.10	0.09999	0.00001	0.000059
0.20	0.19999	0.00001	0.000059
0.50	0.50001	-0.00001	0.000058
1.00	1.00001	-0.00001	0.000059
2.00	2.00000	0.00000	0.000059
5.00	5.00001	-0.00001	0.000061
10.00	10.00005	-0.00005	0.000063
20.00	20.00006	-0.00006	0.000069
50.00	50.0000	0.0000	0.00011
100.00	100.0001	-0.0001	0.00019
120.00	120.0001	-0.0001	0.00022

6. OFF CENTER LOADING ERROR



POINT	READING (g)	
1	10.00001	50.0000
2	10.00002	50.0000
3	10.00001	50.0000
4	10.00001	50.0000
5	10.00002	50.0001
OFF-CENTER LOADING	0.00001	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT PRODUCTION AREA  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : SP22018

Pages 1 of 3

## Calibration Certificate

**Equipment :** UV-VIS SPECTROPHOTOMETER  
**Manufacturer :** PERKINELMER  
**Model :** LAMBDA 25  
**Serial No.:** 501S14123010  
**ID No.:** SP03/58  
**Calibration Mode :** WAVELENGTH ACCURACY  
PHOTOMETRIC ACCURACY  
  
**Condition As Found :** GOOD  
  
**Customer :** S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,  
CHOMPHON, CHATUCHAK,  
BANGKOK 10900, THAILAND.  
  
**Location :** ORGANIC LABORATORY IV  
  
**Ambient Temperature :** ( 24.4 ± 5 ) °C  
**Relative Humidity :** ( 60.1 ± 25 ) %  
  
**Received Date :** 30 AUGUST 2022  
**Calibration Date :** 30 AUGUST 2022  
**Date of Issue :** 31 AUGUST 2022

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

Cert. No. : SP22018

Job No. : VC65SP0008

Pages : 2 of 3

**Calibration Method :**

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

**Condition of this result of calibration :**

## 1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	87569	13/10/2022
Didymium liquid	RM-DL	28912	87588	15/10/2022
Neutral density filter	RM-1N2N3N	13877	87600	15/10/2022
Potassium dichromate solutions	RM-0204060810	14204	87614	16/10/2022
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology, NIST.

**Result of calibration : Wavelength Accuracy**

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.4	0.15	0.16	2.00
	467.82	467.8	-0.02	0.16	2.00
	536.56	536.5	-0.06	0.16	2.00
	640.50	640.5	0.00	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.2	0.26	0.16	2.00

UUC\* = Unit Under Calibration

## Continuation of Calibration Certificate

Cert. No. : SP22018

Job No. : VC65SP0008

Pages : 3 of 3

**Result of calibration : Photometric Accuracy**

(Without adjustment)

Material	Wavelength (nm)	Filter: S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0524	1.0539	0.0015	0.0028	2.00
		29914	0.7	0.7454	0.7459	0.0005	0.0029	2.00
		29381	0.5	0.5426	0.5426	0.0000	0.0028	2.00
	546.1	29360	1.0	0.9822	0.9810	-0.0012	0.0028	2.00
		29914	0.7	0.6962	0.6960	-0.0002	0.0028	2.00
		29381	0.5	0.5076	0.5070	-0.0006	0.0029	2.00
	590.0	29360	1.0	1.0221	1.0202	-0.0019	0.0028	2.00
		29914	0.7	0.7238	0.7230	-0.0008	0.0029	2.00
		29381	0.5	0.5364	0.5360	-0.0004	0.0031	2.00
	635.0	29360	1.0	0.9751	0.9732	-0.0019	0.0028	2.00
		29914	0.7	0.6912	0.6902	-0.0010	0.0029	2.00
		29381	0.5	0.5214	0.5210	-0.0004	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2436	0.2419	-0.0017	0.0101	2.00	
		40	0.4905	0.4855	-0.0050	0.0115	2.00	
		60	0.7453	0.7388	-0.0065	0.0067	2.00	
		80	0.9920	0.9839	-0.0081	0.0071	2.00	
		100	1.2487	1.2414	-0.0073	0.0073	2.00	

UUC\* = Unit Under Calibration

**Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230**

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.0001 A

## Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 1100 nm-190 nm

Scanning Speed 7.5 nm/min

Data Pitch 0.1 nm

Band width(Wavelength) 1.0 nm

Band width(Vis) 1.0 nm

Band width(Uv) 1.0 nm

**Stray Light\*\* UUC\* Reading at 220 nm**

Transmission T(%) Absorbance(A)

0.0107

3.9886

\*\*Specific Acceptance :

Transmission  $\leq 1.0$  T(%), Absorbance  $\geq 2.0$  A

\*\*Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$ ,  
providing a level of confidence of approximately 95%

**End of Calibration Certificate**



## Certificate of Calibration

**Aquion : Anion (ID#894)**

This certificate is to verify that instrument below are calibrated  
by Archemica Lab Co.,Ltd.

AQUION S/N : 190840059

AS-DV S/N : 190915235

for

**S.P.S. Consulting Service Co., Ltd.**



Operator Signature : K. CHANNARONG Date : Jan 5, 2022

(Mr. Channarong Khiao-Un)

Test Engineer

คุณภาพอากาศในสถานประกอบการ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}\text{C}$   
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R²
B01	SKC	224-PCXR4	262101	06/10/2022	1,000	1,500	2,000	994	1,497	1,998	1.001x - 3.789	1.000
B02	SKC	224-PCXR4	626166	03/10/2022	1,000	1,500	2,000	1,002	1,505	2,001	1.009x - 19.707	0.999
B03	SKC	224-PCXR4	612968	03/10/2022	1,000	1,500	2,000	996	1,494	2,001	1.006x - 12.308	1.000
B04	SKC	224-PCXR4	602804	03/10/2022	1,000	1,500	2,000	1,000	1,502	2,000	1.004x - 5.919	1.000
B05	SKC	224-PCXR4	612693	06/10/2022	1,000	1,500	2,000	1,003	1,499	2,003	1.012x - 22.622	0.999
B06	SKC	224-PCXR4	262188	06/10/2022	1,000	1,500	2,000	995	1,507	1,999	1.005x - 11.738	1.000
B07	SKC	224-PCXR4	626262	04/10/2022	1,000	1,500	2,000	998	1,492	1,995	0.993x + 6.405	1.000
B08	SKC	224-PCXR4	626100	04/10/2022	1,000	1,500	2,000	1,002	1,499	2,003	1.013x - 24.18	0.999
B09	SKC	224-PCXR4	626479	06/10/2022	1,000	1,500	2,000	996	1,490	1,994	0.994x + 1.675	1.000
B10	SKC	224-PCXR4	091950	03/10/2022	1,000	1,500	2,000	993	1,503	2,001	1.017x - 34.588	0.999
B11	SKC	224-PCXR8	564315	06/10/2022	1,000	1,500	2,000	994	1,490	2,003	1.007x - 14.438	1.000
B12	SKC	224-PCXR4	034656	03/10/2022	1,000	1,500	2,000	1,003	1,503	2,003	1.010x - 19.005	0.999
B13	SKC	224-PCXR4	602073	03/10/2022	1,000	1,500	2,000	995	1,500	1,993	0.997x + 2.708	1.000
B14	SKC	224-PCXR4	626313	03/10/2022	1,000	1,500	2,000	998	1,491	1,988	0.992x + 6.007	1.000
B15	SKC	224-PCXR4	626474	03/10/2022	1,000	1,500	2,000	1,003	1,502	2,005	1.003x - 10.123	0.999
B16	SKC	224-PCXR4	626477	03/10/2022	1,000	1,500	2,000	993	1,504	2,001	1.015x - 31.624	0.999
B17	SKC	224-PCXR4	626860	03/10/2022	1,000	1,500	2,000	997	1,494	1,991	0.997x - 0.239	1.000
B18	SKC	224-PCXR4	691484	03/10/2022	1,000	1,500	2,000	1,003	1,500	2,001	1.008x - 16.073	0.999
B19	SKC	224-PCXR4	691599	03/10/2022	1,000	1,500	2,000	993	1,503	2,000	1.005x - 8.623	1.000
B20	SKC	224-PCXR4	691587	03/10/2022	1,000	1,500	2,000	991	1,504	1,999	1.016x - 33.631	0.999
B21	SKC	224-PCXR4	691531	06/10/2022	1,000	1,500	2,000	993	1,500	1,994	1.001x - 6.669	1.000
B22	SKC	224-PCXR4	691654	04/10/2022	1,000	1,500	2,000	1,003	1,501	2,003	1.011x - 20.429	0.999
B23	SKC	224-PCXR4	798393	04/10/2022	1,000	1,500	2,000	993	1,505	2,002	1.018x - 34.843	0.999
B24	SKC	224-PCXR4	626363	06/10/2022	1,000	1,500	2,000	999	1,502	2,000	1.012x - 23.225	0.999
B25	SKC	224-PCXR4	798489	06/10/2022	1,000	1,500	2,000	1,001	1,512	2,001	0.998x + 5.049	1.000
B26	SKC	224-PCXR4	798479	06/10/2022	1,000	1,500	2,000	999	1,499	1,993	0.996x + 2.892	1.000
B27	SKC	224-PCXR4	691673	06/10/2022	1,000	1,500	2,000	994	1,503	1,999	1.011x - 22.778	0.999
B28	SKC	224-PCXR4	691570	04/10/2022	1,000	1,500	2,000	1,001	1,500	2,002	1.007x - 13.301	1.000
B29	SKC	224-PCXR4	626472	06/10/2022	1,000	1,500	2,000	1,000	1,496	1,998	1.002x - 5.261	1.000
B30	SKC	224-PCXR4	691489	03/10/2022	1,000	1,500	2,000	1,007	1,500	2,004	1.010x - 18.482	0.999
B31	SKC	224-PCXR4	691509	03/10/2022	1,000	1,500	2,000	993	1,497	1,998	1.004x - 8.882	1.000
B32	SKC	224-PCXR4	091567	03/10/2022	1,000	1,500	2,000	992	1,504	2,001	1.007x - 15.930	1.000
B33	SKC	224-PCXR4	091756	06/10/2022	1,000	1,500	2,000	994	1,496	1,991	0.996x + 0.714	1.000
B34	SKC	224-PCXR4	612962	03/10/2022	1,000	1,500	2,000	1,002	1,501	2,001	1.009x - 17.944	0.999
B35	SKC	224-PCXR4	602682	03/10/2022	1,000	1,500	2,000	993	1,498	1,995	1.001x - 7.331	1.000
B36	SKC	224-PCXR4	626164	06/10/2022	1,000	1,500	2,000	999	1,495	1,999	1.000x - 4.866	1.000
B37	SKC	224-PCXR4	626256	06/10/2022	1,000	1,500	2,000	994	1,506	1,999	1.013x - 28.214	0.999
B38	SKC	224-PCXR4	626167	06/10/2022	1,000	1,500	2,000	997	1,496	1,996	1.002x - 6.342	1.000
B39	SKC	224-PCXR4	034637	06/10/2022	1,000	1,500	2,000	1,006	1,500	2,001	1.008x - 16.624	0.999
B40	SKC	224-PCXR4	798349	05/10/2022	1,000	1,500	2,000	994	1,505	1,998	1.014x - 29.642	0.999

Calibrated by :

*Adul Dangklom*  
(Mr. Adul Dangklom)

Approved by :

*Peera Detudom*  
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
B41	SKC	224-PCXR4	612669	05/10/2022	1,000	1,500	2,000	998	1,496	1,990	0.994x + 3.271	1.000
B42	SKC	224-PCXR4	626041	06/10/2022	1,000	1,500	2,000	1,005	1,498	1,994	0.988x + 15.619	1.000
B43	SKC	224-PCXR4	034636	06/10/2022	1,000	1,500	2,000	999	1,501	1,992	0.991x + 10.565	1.000
B44	SKC	224-PCXR8	529341	06/10/2022	1,000	1,500	2,000	1,002	1,502	2,002	1.011x - 21.418	0.999
B45	SKC	224-PCXR8	529594	06/10/2022	1,000	1,500	2,000	998	1,498	1,989	0.993x + 5.959	1.000
B46	SKC	224-PCXR8	566743	06/10/2022	1,000	1,500	2,000	994	1,504	2,002	1.016x - 32.885	0.999
B47	SKC	224-PCXR8	566747	06/10/2022	1,000	1,500	2,000	1,002	1,500	2,004	1.013x - 24.960	0.999
B48	SKC	224-PCXR8	566753	03/10/2022	1,000	1,500	2,000	999	1,494	1,998	0.999x - 2.114	1.000
B49	SKC	224-PCXR8	566780	05/10/2022	1,000	1,500	2,000	1,003	1,502	2,003	1.012x - 22.706	0.999
B50	SKC	224-PCXR8	500400	06/10/2022	1,000	1,500	2,000	1,001	1,495	2,002	1.001x - 3.737	1.000
B51	SKC	224-PCXR8	500363	06/10/2022	1,000	1,500	2,000	995	1,504	1,999	1.011x - 25.590	0.999
B52	SKC	224-PCXR8	093186	03/10/2022	1,000	1,500	2,000	995	1,496	1,994	0.997x - 1.161	1.000
B53	SKC	224-PCXR8	707670	03/10/2022	1,000	1,500	2,000	1,002	1,500	2,002	1.010x - 20.668	0.999
B54	SKC	224-PCXR3	509821	03/10/2022	1,000	1,500	2,000	993	1,500	2,001	1.017x - 34.516	0.999
B55	SKC	224-PCXR3	510710	03/10/2022	1,000	1,500	2,000	999	1,494	1,994	0.995x + 2.521	1.000
B56	SKC	224-PCXR3	511450	03/10/2022	1,000	1,500	2,000	1,002	1,500	2,001	1.004x - 7.562	1.000
B57	SKC	224-PCXR3	510798	06/10/2022	1,000	1,500	2,000	997	1,492	1,998	0.996x +1.109	1.000
B58	SKC	224-PCXR3	509852	06/10/2022	1,000	1,500	2,000	1,000	1,498	1,999	1.007x - 19.113	0.999
B59	SKC	224-PCXR3	509862	03/10/2022	1,000	1,500	2,000	996	1,503	1,994	0.997x + 2.955	1.000
B60	SKC	224-PCXR3	512655	03/10/2022	1,000	1,500	2,000	1,005	1,500	2,003	1.010x - 19.862	0.999
B61	SKC	224-PCXR3	503915	04/10/2022	1,000	1,500	2,000	994	1,489	1,998	1.004x - 11.786	1.000
B62	SKC	224-PCXR3	505975	03/10/2022	1,000	1,500	2,000	999	1,494	1,996	0.997x - 0.064	1.000
B63	SKC	224-PCXR3	511432	03/10/2022	1,000	1,500	2,000	991	1,501	1,999	1.017x - 35.461	0.999
B64	SKC	224-PCXR3	508302	03/10/2022	1,000	1,500	2,000	997	1,492	1,989	0.992x + 6.266	1.000
B65	SKC	224-PCXR3	508310	06/10/2022	1,000	1,500	2,000	1,002	1,500	2,003	1.011x - 21.992	0.999
B66	SKC	224-PCXR3	509861	06/10/2022	1,000	1,500	2,000	1,002	1,491	1,991	0.988x + 13.904	1.000
B67	SKC	224-PCXR3	506295	06/10/2022	1,000	1,500	2,000	993	1,508	2,004	1.017x - 32.785	0.999
B68	SKC	224-PCXR3	505872	05/10/2022	1,000	1,500	2,000	1,002	1,491	1,997	0.994x + 5.237	1.000
B69	SKC	224-PCXR3	508375	05/10/2022	1,000	1,500	2,000	1,001	1,499	2,000	1.010x - 21.330	0.999
B70	SKC	224-PCXR3	510623	05/10/2022	1,000	1,500	2,000	992	1,503	1,997	1.002x - 6.054	1.000
B71	SKC	224-PCXR3	508367	05/10/2022	1,000	1,500	2,000	990	1,506	2,002	1.018x - 37.025	0.999
B72	SKC	224-PCXR3	505977	05/10/2022	1,000	1,500	2,000	1,001	1,498	1,993	0.993x + 5.731	1.000
B73	SKC	224-PCXR3	512606	05/10/2022	1,000	1,500	2,000	1,001	1,501	2,005	1.014x - 24.397	0.999
B74	SKC	224-PCXR3	505993	05/10/2022	1,000	1,500	2,000	996	1,495	1,994	0.999x - 4.284	1.000
B75	SKC	224-PCXR3	509820	05/10/2022	1,000	1,500	2,000	996	1,498	1,990	0.995x + 2.987	1.000
B76	SKC	224-PCXR3	509811	03/10/2022	1,000	1,500	2,000	993	1,498	1,998	1.006x - 14.003	1.000
B77	SKC	224-PCXR3	508301	06/10/2022	1,000	1,500	2,000	1,000	1,501	2,003	1.014x - 25.845	0.999
B78	SKC	224-PCXR3	510677	06/10/2022	1,000	1,500	2,000	996	1,503	1,999	1.012x - 27.321	0.999
B79	SKC	224-PCXR3	510920	06/10/2022	1,000	1,500	2,000	994	1,493	1,994	0.999x - 3.905	1.000

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R²
R01	SKC	224-PCXR4	602467	06/10/2022	1,000	1,500	2,000	993	1,508	2,004	1.020x - 38.145	0.999
R02	SKC	224-PCXR4	626450	06/10/2022	1,000	2,000	3,000	998	1,499	1,990	0.989x + 12.189	1.000
R03	SKC	224-PCXR4	691592	03/10/2022	1,000	1,500	2,000	1,004	1,500	2,004	1.011x - 21.482	0.999
R04	SKC	224-PCXR4	691672	03/10/2022	1,000	1,500	2,000	996	1,493	1,994	0.997x - 0.766	1.000
R05	SKC	224-PCXR4	798470	06/10/2022	1,000	1,500	2,000	994	1,505	1,999	1.014x - 30.635	0.999
R06	SKC	224-PCXR4	798456	06/10/2022	1,000	1,500	2,000	994	1,498	1,994	1.002x - 7.000	1.000
R07	SKC	224-PCXR4	798480	06/10/2022	1,000	1,500	2,000	994	1,490	1,999	1.008x - 16.751	1.000
R08	SKC	224-PCXR4	883215	06/10/2022	1,000	1,500	2,000	1,001	1,501	2,005	1.014x - 26.148	0.999
R09	SKC	224-PCXR4	034650	06/10/2022	1,000	1,500	2,000	991	1,504	2,002	1.018x - 36.179	0.999
R10	SKC	224-PCXR4	091765	06/10/2022	1,000	1,500	2,000	996	1,512	1,994	1.000x + 0.140	1.000
R11	SKC	224-PCXR4	091763	06/10/2022	1,000	1,500	2,000	1,000	1,499	2,002	1.013x - 25.678	0.999
R12	SKC	224-PCXR4	091568	06/10/2022	1,000	1,500	2,000	997	1,501	1,999	1.001x - 5.065	1.000
R13	SKC	224-PCXR4	091638	06/10/2022	1,000	1,500	2,000	1,002	1,499	1,994	0.992x + 9.636	1.000
R14	SKC	224-PCXR4	091764	06/10/2022	1,000	1,500	2,000	994	1,502	1,999	1.014x - 30.053	0.999
R15	SKC	224-PCXR8	529457	06/10/2022	1,000	1,500	2,000	1,001	1,500	2,004	1.013x - 25.023	0.999
R16	SKC	224-PCXR8	529643	06/10/2022	1,000	1,500	2,000	998	1,497	1,994	0.998x - 1.017	1.000
R17	SKC	224-PCXR8	529645	06/10/2022	1,000	1,500	2,000	994	1,509	2,000	1.015x - 30.372	0.999
R18	SKC	224-PCXR8	566756	06/10/2022	1,000	1,500	2,000	991	1,498	1,998	1.001x - 6.880	1.000
R19	SKC	224-PCXR8	566802	06/10/2022	1,000	1,500	2,000	1,003	1,499	2,000	1.009x - 19.751	0.999
R20	SKC	224-PCXR8	529089	06/10/2022	1,000	1,500	2,000	990	1,501	2,003	1.020x - 40.195	0.999
R21	SKC	224-PCXR8	665728	06/10/2022	1,000	1,500	2,000	998	1,493	1,999	1.001x - 6.003	1.000
R22	SKC	224-PCXR8	707444	06/10/2022	1,000	1,500	2,000	1,002	1,500	2,002	1.011x - 21.733	0.999
R23	SKC	224-PCXR8	761067	06/10/2022	1,000	1,500	2,000	998	1,494	1,991	0.993x + 36535	1.000
R24	SKC	224-PCXR8	707893	06/10/2022	1,000	1,500	2,000	996	1,505	2,000	1.013x - 27.803	0.999
R25	SKC	224-PCXR8	761052	05/10/2022	1,000	1,500	2,000	998	1,499	1,993	0.993x + 6.713	1.000
R26	SKC	224-PCXR8	707956	05/10/2022	1,000	1,500	2,000	1,002	1,500	2,004	1.013x - 24.058	0.999
R27	SKC	224-PCXR8	707398	05/10/2022	1,000	1,500	2,000	996	1,503	2,001	1.006x - 15.683	1.000
R28	SKC	224-PCXR8	707481	05/10/2022	1,000	1,500	2,000	1,004	1,500	2,003	1.010x - 19.687	0.999
R29	SKC	224-PCXR8	707402	05/10/2022	1,000	1,500	2,000	1,005	1,493	1,991	0.988x + 14.366	1.000
R30	SKC	224-PCXR8	093811	05/10/2022	1,000	1,500	2,000	999	1,495	1,994	0.997x - 0.8069	1.000
R31	SKC	224-PCXR8	093183	06/10/2022	1,000	1,500	2,000	1,001	1,501	2,001	1.012x - 22.523	0.999
R32	SKC	224-PCXR8	671950	06/10/2022	1,000	1,500	2,000	1,000	1,498	1,994	0.994x + 8.041	1.000
R33	SKC	224-PCXR4	626254	06/10/2022	1,000	1,500	2,000	993	1,502	1,999	1.016x - 33.303	0.999
R34	SKC	224-PCXR4	626131	06/10/2022	1,000	1,500	2,000	1,002	1,498	2,004	1.013x - 24.453	0.999
R35	SKC	224-PCXR8	707460	06/10/2022	1,000	1,500	2,000	999	1,498	1,995	0.994x + 6.709	1.000
R36	SKC	224-PCXR8	707446	06/10/2022	1,000	1,500	2,000	1,003	1,499	2,001	1.009x - 19.432	0.999
R37	SKC	224-PCXR8	707432	06/10/2022	1,000	1,500	2,000	997	1,499	1,998	0.998x + 0.116	1.000
R38	SKC	224-PCXR8	707349	05/10/2022	1,000	1,500	2,000	996	1,500	2,002	1.015x - 31.640	0.999
R39	SKC	224-PCXR8	761095	05/10/2022	1,000	1,500	2,000	1,001	1,496	1,994	0.997x + 2.094	1.000

Calibrated by :

*Adul Dangklom*  
(Mr. Adul Dangklom)

Approved by :

*Peera Detudom*  
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R²
R40	SKC	224-PCXR4	612753	05/10/2022	1,000	1,500	2,000	1,001	1,501	2,003	1.012x - 23.763	0.999
R41	SKC	224-PCXR4	626140	05/10/2022	1,000	1,500	2,000	991	1,509	2,001	1.017x - 33.838	0.999
R42	SKC	224-PCXR4	626463	05/10/2022	1,000	1,500	2,000	995	1,493	1,999	1.003x - 6.593	1.000
R43	SKC	224-PCXR4	626129	05/10/2022	1,000	1,500	2,000	1,002	1,501	2,003	1.005x - 16.073	0.999
R44	SKC	224-PCXR4	602753	05/10/2022	1,000	1,500	2,000	1,002	1,496	1,993	0.996x + 1.571	1.000
R45	SKC	224-PCXR4	626137	05/10/2022	1,000	1,500	2,000	992	1,505	2,002	1.019x - 37.487	0.999

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164


Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
H-R01	Dwyer	VFB-65	04/10/2022	500	1,000	2,000	502.9	992.8	1978.7	0.999x + 3.447	0.999
H-R02	Dwyer	VFB-65	05/10/2022	500	1,000	2,000	500.8	995.3	1985.7	1.002x - 5.358	1.000
H-R03	Dwyer	VFB-65	06/10/2022	500	1,000	2,000	502.1	987.7	1996.9	0.994x + 1.850	1.000
H-R04	Dwyer	VFB-65	06/10/2022	500	1,000	2,000	496.0	989.6	2019.5	1.007x - 11.659	1.000
H-R05	Dwyer	VFB-65	05/10/2022	500	1,000	2,000	497.2	988.1	1988.1	1.004x - 9.026	1.000
H-R06	Dwyer	VFB-65	04/10/2022	500	1,000	2,000	505.6	992.4	1979.8	0.999x - 2.422	0.999

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

  
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R²
L-R01	Dwyer	VFA-21	04/10/2022	50	100	200	50.2	101.0	203.9	0.987x + 2.546	1.000
L-R02	Dwyer	VFA-21	05/10/2022	50	100	200	50.1	101.3	200.5	1.007x – 0.870	0.999
L-R03	Dwyer	VFA-21	06/10/2022	50	100	200	50.1	99.8	202.3	1.017x – 1.042	1.000
L-R04	Dwyer	VFA-21	06/10/2022	50	100	200	50.2	100.9	201.0	1.008x – 1.004	0.999
L-R05	Dwyer	VFA-21	05/10/2022	50	100	200	50.2	100.8	203.0	0.990x + 1.973	1.000
L-R06	Dwyer	VFA-21	04/10/2022	50	100	200	50.2	99.1	201.5	1.004x – 0.364	1.000

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 22M2567

REFERENCE No : 64386-1

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS 105DU

**SERIAL No** : 1126422905

**ID No** : BA 05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : TETNITHI W.

**CALIBRATION DATE** : 11-Mar-22

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 17-Mar-22

**RECEIVED DATE** : 11-Mar-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 22M2567

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	MODEL	:	XS 105DU
MANUFACTURER	:	METTLER TOLEDO	S/N	:	1126422905
ID No	:	BA 05/50	RECEIVED DATE	:	11-Mar-22
AIR PRESSURE	:	1008mbar $\pm$ 1mbar	CALIBRATION DATE	:	11-Mar-22
AMBIENT TEMPERATURE	:	22° C $\pm$ 1° C	RELATIVE HUMIDITY	:	49 %RH $\pm$ 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-


- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 20 g WAS 0.000004 g
4. REPEATABILITY OF READING AT 100 g WAS 0.000048 g
5. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000058
0.02	0.01999	0.00001	0.000058
0.10	0.09999	0.00001	0.000059
0.20	0.19999	0.00001	0.000059
0.50	0.50001	-0.00001	0.000058
1.00	1.00001	-0.00001	0.000059
2.00	2.00000	0.00000	0.000059
5.00	5.00001	-0.00001	0.000061
10.00	10.00005	-0.00005	0.000063
20.00	20.00006	-0.00006	0.000069
50.00	50.00000	0.00000	0.00011
100.00	100.00001	-0.00001	0.00019
120.00	120.00001	-0.00001	0.00022

6. OFF CENTER LOADING ERROR



POINT	READING (g)	
1	10.00001	50.0000
2	10.00002	50.0000
3	10.00001	50.0000
4	10.00001	50.0000
5	10.00002	50.00001
OFF-CENTER LOADING	0.00001	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT PRODUCTION AREA  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

<b>Customer :</b> <u>S.P.S.Consulting Service Co.,Ltd</u>	<b>Date Tested:</b> <u>July 11, 2022</u>	
	<b>Recommendation Recertification</b>	
<b>Address :</b> <u>7 Soi Phaholyothin 24</u>	<b>Period</b> <u>6</u> <b>Months</b>	
<u>Paholyothin Road</u>	<b>Recertification Due:</b> <u>January 11, 2023</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	<b>Date Last Certified:</b> <u>January 12, 2022</u>	
<b>User Name:</b> <u>K.Phenpha Vipasthawatt</u>	<b>Visit Number:</b> <u>1 of 2</u>	
<b>Phone:</b> <u>083-9269252</u>	<b>PerkinElmer Phone:</b> <u>02-719-6420 ext 206</u>	
<b>Fax:</b> <u>02-513-4221</u>	<b>PerkinElmer Fax:</b> <u>02-318-5597</u>	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
<b>MODEL</b>	<b>SERIAL NUMBER</b>	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
<b>TESTED EQUIPMENT</b>	<b>CALIBRATION NUMBER</b>	<b>EXPIRATION</b>
<u>IPV Methods</u>		
<b>TEST STANDARD USED</b>	<b>PART NUMBER</b>	<b>EXPIRATION DATE</b>
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>August 30, 2022</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>November 30, 2022</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>August 30, 2023</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>August 30, 2022</u>
<b>CUSTOMER SUPPLIED</b>	<b>COMMENTS</b>	<b>CUSTOMER INITIALS</b>
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		



## MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV

SERIAL NUMBER 077C7042401DATE TESTED July 11, 2022**1. MECHANICAL CHECKS**

- |  |                             |
|--|-----------------------------|
| A. Inspect and clean all fans and filters.                                       | <input type="checkbox"/> OK |
| B. Inspect and replace as necessary, all torch components including the RF coil. | <input type="checkbox"/> OK |
| C. Inspect all tubing for sign of clacking or leaking.                           | <input type="checkbox"/> OK |
| D. Adjust water and gas pressure regulator settings.                             | <input type="checkbox"/> OK |
| E. Inspect and leak check pneumatics drawers.                                    | <input type="checkbox"/> OK |
| F. Clean the exterior of the instrument.   | <input type="checkbox"/> OK |

**2. OPTICAL CHECKS**

- |   |                             |
|---|-----------------------------|
| A. Inspect and clean all optical components.        | <input type="checkbox"/> OK |
| B. As required, check and replace all purgefilters. | <input type="checkbox"/> OK |
| C. Recheck optical alignment.                       | <input type="checkbox"/> OK |

**3. COOLING SYSTEM CHECKS**

- |   |                              |
|---|------------------------------|
| A. Perform preventive maintenance on chiller. | <input type="checkbox"/> OK  |
| B. Flush out the chiller every year.          | <input type="checkbox"/> N/A |

**4. PERFORMANCE CHECKS**

- |                            |                             |
|----------------------------|-----------------------------|
| A. Torch View Alignment.   | <input type="checkbox"/> OK |
| B. Wavelength Calibration. | <input type="checkbox"/> OK |



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

SERIAL NUMBER : 077C7042401DATE TESTED : July 11, 2022

PARAMETER	SPECIFICATION			FINAL VALUE	
Spectral Resolution : UV	As 193.696 nm	≤ 0.007		0.00544	
	Ni 231.604 nm	≤ 0.008		0.00709	
	Ni 341.476 nm	≤ 0.012		0.00757	
Spectral Resolution : VIS	La 408.672 nm	≤ 0.020		0.01638	
	Ba 455.403 nm	≤ 0.025		0.02391	
Precision					
	As 193.656 nm	% RSD	< 1.0	0.91	%
	Zn 213.856 nm	% RSD	< 1.0	0.87	%
	Mn 257.610 nm	% RSD	< 1.0	0.76	%
	La 379.478 nm	% RSD	< 1.0	0.59	%
	Ba 455.403 nm	% RSD	< 1.0	0.53	%
	Ba 493.408 nm	% RSD	< 1.0	0.55	%
Detection Limits : Axial	Tl 190.080 nm	3(sd)		5.51	ppb
	As 193.696 nm	3(sd)		8.59	ppb
	Pb 220.353 nm	3(sd)		0.50	ppb
Detection Limits : Radial	As 193.696 nm	3(sd)		2.17	ppb
	Zn 213.856 nm	3(sd)		0.03	ppb
	Mn 257.610 nm	3(sd)		0.01	ppb
	La 379.478 nm	3(sd)		0.04	ppb
	Ba 455.403 nm	3(sd)		0.01	ppb
	Ba 493.408 nm	3(sd)		0.00	ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd 226.502 nm	≤ 150 ppb		12.46	
BEC : Radial (IB X 1000)/(IS-IB)	Mn 257.610 nm	≤ 45 ppb		30.82	



## MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV

SERIAL NUMBER 077C7042401DATE TESTED July 11, 2022**Remarks :**

Commissioning follow as commissioning performance sheets.

---

---

---

---

---

---

---

---

This is to certify that the above tests have been performed and the configuration tested

☒

meets

☐

does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,  
including warranty terms.

**Service Department PerkinElmer Ltd.**

**Authorized Representative:**

( Mr. Wiphan Promlumda )

Service Engineer



## Certificate of Calibration

**Aquion : Anion (ID#894)**

This certificate is to verify that instrument below are calibrated  
by Archemica Lab Co.,Ltd.

AQUION S/N : 190840059

AS-DV S/N : 190915235

for

**S.P.S. Consulting Service Co., Ltd.**



Operator Signature : K. CHANNARONG Date : Jan 5, 2022

(Mr. Channarong Khiao-Un)

Test Engineer

ระดับเสียงในบรรยากาศ

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0455

MTC No. EEL. BP. 41/0465

## CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Keithley 2015-P S/N 4106495.

7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.


**Calibration Procedure:** CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 22 Apr. 2022

Date of Calibration : 28 Apr. 2022



The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0455

MTC No. EEL. BP. 41/0465

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.93	-0.07	$\pm 0.10$	$\pm 0.40$ dB

2. Frequency


Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	$\pm 1.5$	$\pm 1.0\%$


3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.44	$\pm 0.50$	$\pm 3.0\%$

- Note :
1. No adjustment.
  2. The calibrator pressure correction was not included.
  3. The microphone volume correction was not included.

Calibrated by :

  
(Mr. Nuttapong Niljrusvanit)

  
(Mr. Tawikiat Iamsamran)

Date of Calibration : 28 Apr. 2022

Date of Issue : 28 Apr. 2022

Approved by :

  
(Mr. Prawate Kluaypa)  
Director

Electrical and Electronic Standards Laboratory  
Industrial Metrology and Testing Service Centre

Ref : 2011265042601787001

2 / 2

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise R\_612/22

## Sound Level Meter Calibration Report

### Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	28 April 2022
		Due Date	28 April 2023

### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R05	ACO	6236	00142020	21 November 2022	94.1	94.0
ACO-R21	ACO	6236	00182004	21 November 2022	94.1	94.0
ACO-R22	ACO	6236	00182010	21 November 2022	94.0	94.0
ACO-R31	ACO	6236	00192043	21 November 2022	94.0	94.0
ACO-R32	ACO	6236	00192044	21 November 2022	94.1	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.93 ± 0.10 dB	

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)

ระดับเสียงในสถานประกอบการ

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0455

MTC No. EEL. BP. 41/0465

## CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Keithley 2015-P S/N 4106495.

7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.


**Calibration Procedure:** CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 22 Apr. 2022

Date of Calibration : 28 Apr. 2022



The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0455

MTC No. EEL. BP. 41/0465

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.93	-0.07	$\pm 0.10$	$\pm 0.40$ dB

2. Frequency


Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	$\pm 1.5$	$\pm 1.0\%$


3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.44	$\pm 0.50$	$\pm 3.0\%$

- Note :
1. No adjustment.
  2. The calibrator pressure correction was not included.
  3. The microphone volume correction was not included.

Calibrated by :

  
(Mr. Nuttapong Niljrusvanit)

  
(Mr. Tawikiat Iamsamran)

Date of Calibration : 28 Apr. 2022

Date of Issue : 28 Apr. 2022

Approved by :

  
(Mr. Prawate Kluaypa)  
Director

Electrical and Electronic Standards Laboratory  
Industrial Metrology and Testing Service Centre

Ref : 2011265042601787001

2 / 2

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R\_654/22

## Sound Level Meter Calibration Report

### Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	28 April 2022
		Due Date	28 April 2023

### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B29	ACO	6236	00182011	27 November 2022	94.1	94.0
ACO-B36	ACO	6236	00192027	27 November 2022	94.0	94.0
ACO-B41	ACO	6236	00192032	27 November 2022	94.0	94.0
ACO-B43	ACO	6236	00192034	27 November 2022	94.1	94.0
ACO-R50	ACO	6236	00192062	27 November 2022	94.0	94.0
NL 21-B01	RION	NL-21	00554245	27 November 2022	94.0	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.93 ± 0.10 dB	

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)

Request No. 21-65/0760

MTC No. EEL. BP. 24/0965

## CALIBRATION CERTIFICATE

Submitted by : S.P.S. CONSULTING SERVICE CO., LTD.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Acoustic Calibrator

Manufacturer : SVANTEK

Model : SV34

Serial No. : 33139

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.

7. Condenser Microphone Bruel&Kjaer 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.


This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 13 Sep. 2022

Date of Calibration : 19 Sep. 2022

1 / 2



The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

Request No. 21-65/0760

MTC No. EEL. BP. 24/0965

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 114 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	113.63	-0.37	$\pm 0.10$	$\pm 0.75$ dB

2. Frequency


Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	$\pm 1.5$	$\pm 2.0$ %

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	0.24	$\pm 0.50$	$\pm 4.0$ %

- Note :
1. No adjustment.
  2. The calibrator pressure correction was not included.
  3. The microphone volume correction was not included.

Calibrated by :

  
(Mr. Nuttapong Niljrusvanit)

Approved by :

  
(Mr. Prawate Kluaypa)  
Director

Electrical and Electronic Standards Laboratory  
Industrial Metrology and Testing Service Centre

Date of Calibration : 19 Sep. 2022

Date of Issue : 20 Sep. 2022

Ref : 2011265091304034002

2 / 2

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise Dose R\_655/22

## Noise Dose Meter Calibration Report

### Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 06/62
Model	SV34	Serial No.	33139
Calibration Range	114 dB, 1000 Hz	Last Calibration	19 September 2022
		Due Date	19 September 2023

### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R02	SVANTEK	SV-104IS	60152	27 November 2022	113.6	113.6
NMD-R03	SVANTEK	SV-104IS	60153	27 November 2022	113.5	113.6
NMD-R05	SVANTEK	SV-104IS	60155	27 November 2022	113.6	113.6
NMD-R06	SVANTEK	SV-104IS	60146	27 November 2022	113.5	113.6
NMD-R13	SVANTEK	SV-104IS	63438	27 November 2022	113.6	113.6
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					113.63± 0.10 dB	

Calibrated by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)

คุณภาพน้ำทิ้ง

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 22E9693

REFERENCE No : 66476-1

PAGE : 1 OF 3

**Certificate of Calibration**

**EQUIPMENT** : pH METER

**MANUFACTURER** : HANNA

**MODEL** : HI 3512

**SERIAL No** : TH118035

**ID No** : pH 04/56

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 15-Sep-22

**APPROVED BY** : PONGSAK J.

**ISSUED DATE** : 15-Sep-22

**RECEIVED DATE** : 14-Sep-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.



# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22E9693

PAGE : 2 OF 3

## Calibration Report

EQUIPMENT : pH METER  
MANUFACTURER : HANNA  
ID No : pH 04/56  
RECEIVED DATE : 14-Sep-22  
AMBIENT TEMPERATURE : 20 ° C ± 1 ° C  
MODEL : HI 3512  
SERIAL NUMBER : TH118035  
CALIBRATION DATE : 15-Sep-22  
RELATIVE HUMIDITY : 50 % RH ± 10% RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/</u> <u>LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-06	CC719181	4880-12119147	05-Apr-23
2) pH STANDARD SOLUTION	00651-08	CC718727	4881-12110709	31-Mar-23
3) pH STANDARD SOLUTION	00651-10	CC717045	4882-12065386	17-Mar-23
4) PROCESS CALIBRATOR	CA150	91S6079	22E1145	31-Mar-23
5) BATH	260014	1247 48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
  - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
  - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

### RESULT OF CALIBRATION : ADJUSTMENT

#### 1. DISPLAY UNIT ONLY

SLOPE FACTOR  $k = 2.303 \text{ RT/F} = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.8	-0.69	-0.171	0.14	2.0
354.95	355.6	-0.65	0.860	0.14	2.0
295.80	296.4	-0.60	1.892	0.14	2.0
236.64	237.2	-0.56	2.922	0.14	2.0
177.48	178.0	-0.52	3.954	0.14	2.0
118.32	118.8	-0.48	4.985	0.14	2.0
59.16	59.7	-0.54	6.016	0.14	2.0
0.00	0.5	-0.50	7.049	0.14	2.0
-59.16	-58.8	-0.36	8.136	0.14	2.0
-118.32	-117.9	-0.42	9.223	0.14	2.0
-177.48	-177.1	-0.38	10.311	0.14	2.0
-236.64	-236.3	-0.34	11.399	0.14	2.0
-295.80	-295.5	-0.30	12.487	0.14	2.0
-354.95	-354.7	-0.25	13.575	0.14	2.0
-414.11	-413.9	-0.21	14.662	0.14	2.0

END OF CALIBRATION REPORT PAGE 2 OF 3

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22E9693

PAGE : 3 OF 3

**Calibration Report****RESULT OF CALIBRATION (CONTINUE) :****2. DISPLAY UNIT WITH pH ELECTRODE S/N: 09081C6M**

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ( $\pm$ pH)	COVERAGE FACTOR k
4.007	4.007	0.000	3.996	0.012	2.0
7.004	7.006	-0.002	6.944	0.012	2.0
10.016	10.012	0.004	10.194	0.014	2.0

**3. DISPLAY UNIT WITH TEMPERATURE**

STANDARD READING (°C)	UUC READING (°C)	CORRECTION (°C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ( $\pm$ °C)	COVERAGE FACTOR k
25.003	25.0	0.003	---	0.0085	2.0

**4. PERCENT SLOPE 100%**

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 22M2569

REFERENCE No : 64386-3

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : TETNITHI W.

CALIBRATION DATE : 11-Mar-22

APPROVED BY : PONGSAK J.

ISSUED DATE : 17-Mar-22

RECEIVED DATE : 11-Mar-22



CERTIFICATE No : 22M2569

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW  
MANUFACTURER : SARTORIUS S/N : 36591843  
ID No : BA 09/61 RECEIVED DATE : 11-Mar-22  
AIR PRESSURE : 1008mbar  $\pm$  1mbar CALIBRATION DATE : 11-Mar-22  
AMBIENT TEMPERATURE : 22° C  $\pm$  1° C RELATIVE HUMIDITY : 51 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING WEIGHT OF QUALITY CALIBRATION TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000048 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.0000	0.0000	0.000078
0.10	0.1000	0.0000	0.000078
0.20	0.2000	0.0000	0.000078
0.50	0.5000	0.0000	0.000079
1.00	1.0000	0.0000	0.000079
2.00	2.0000	0.0000	0.000080
5.00	5.0000	0.0000	0.000081
10.00	10.0000	0.0000	0.000084
20.00	20.0000	0.0000	0.000089
50.00	50.0000	0.0000	0.00011
100.00	100.0000	0.0000	0.00019
200.00	199.9999	0.0001	0.00032

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	99.9999
2	99.9999
3	100.0000
4	99.9999
5	99.9998
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT PRODUCTION AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES**


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

**Cert.No.:** 22TW98

**Page.:** 1 of 2

## Certificate of Testing

<b>Equipment :</b>	DO Meter
<b>Manufacturer :</b>	YSI
<b>Model :</b>	5000-230V
<b>Serial No. :</b>	15B100751
<b>ID No. :</b>	-
<b>Received Date :</b>	20 April 2022
<b>Test Date :</b>	21 April 2022
<b>Reference :</b>	2204-0429WC-1
<b>Submitted by :</b>	S.P.S. Consulting Service Co.,Ltd. 7 Phaholyothin 24, Phaholyothin Road., Jompol, Chatuchak, Bangkok 10900
<b>Laboratory Condition :</b>	Temperature ( $25 \pm 5$ ) °C Humidity ( $50 \pm 20$ ) %
<b>Test Procedure :</b>	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
<b>Tested by :</b>	Walalak Sirithean
<b>Approved by :</b>	 Approved Signatory
<input checked="" type="checkbox"/> Malee Butkruea <input type="checkbox"/> Saithip Meangmai <input type="checkbox"/> Warakorn Lerngagtrakul	
<b>Issue Date :</b>	25 April 2022



Cert.No.: 22TW98

Page.: 2 of 2

**Condition of this result of calibration**

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	21MM430	21 Sep 2022

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

**Result :** Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 14J100195

<b>Titration Method (Azide Modification Method)</b> (mg/L)	<b>DO Meter Reading</b> (mg/L)	<b>Standard Deviation</b> (mg/L)
8.12	8.14	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

*Malu*

a 1105753



# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 22T0570

REFERENCE No : 63773-2

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200


SERIAL No : 15110C0498

ID No : DRB 06/59

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 21-Jan-22

APPROVED BY :   
PONGSAK J.

ISSUED DATE : 21-Jan-22

RECEIVED DATE : 19-Jan-22



# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22T0570

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : COD REACTOR  
MANUFACTURER : HACH  
ID NUMBER : DRB 06/59  
RECEIVED DATE : 19-Jan-22  
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB 200  
SERIAL NUMBER : 15110C0498  
CALIBRATION DATE : 21-Jan-22  
RELATIVE HUMIDITY : 52 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT TEMPERATURE RECORDER WITH THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 15 POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE FOUR CORNERS OF THE REACTOR AND PLACED THE EIGHTH THERMOCOUPLE AT THE CENTER OF THE REACTOR.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	8009008	21T6767	10-Jul-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

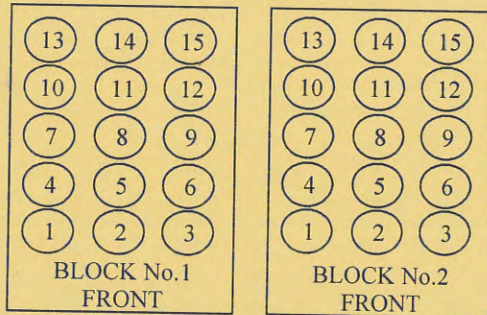

### TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	150.5
	2	150.6
	3	149.7
	4	150.2
	5	149.9
	6	150.1
	7	150.1
	8	149.7
	9	150.6
	10	149.6
	11	149.9
	12	149.6
	13	149.7
	14	149.8
	15	149.6
Uncertainty of Measurement(± °C)	0.86	0.86

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

<b>Customer :</b> <u>S.P.S.Consulting Service Co.,Ltd</u>	Date Tested: <u>July 11, 2022</u>	
	Recommendation Recertification	
<b>Address :</b> <u>7 Soi Phaholyothin 24</u>	Period <u>6</u> Months	
<u>Paholyothin Road</u>	Recertification Due: <u>January 11, 2023</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	Date Last Certified: <u>January 12, 2022</u>	
<b>User Name:</b> <u>K.Phenpha Vipasthawatt</u>	Visit Number: <u>1 of 2</u>	
<b>Phone:</b> <u>083-9269252</u>	PerkinElmer Phone: <u>02-719-6420 ext 206</u>	
<b>Fax:</b> <u>02-513-4221</u>	PerkinElmer Fax: <u>02-318-5597</u>	

CONFIGURATION TESTED	ACCESSORIES/COMPONENT NOT INCLUDED	
<b>MODEL</b>	<b>SERIAL NUMBER</b>	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
<b>TESTED EQUIPMENT</b>	<b>CALIBRATION NUMBER</b>	<b>EXPIRATION</b>
<u>IPV Methods</u>		
<b>TEST STANDARD USED</b>	<b>PART NUMBER</b>	<b>EXPIRATION DATE</b>
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>August 30, 2022</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>November 30, 2022</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>August 30, 2023</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>August 30, 2022</u>
<b>CUSTOMER SUPPLIED</b>	<b>COMMENTS</b>	<b>CUSTOMER INITIALS</b>
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		



## MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV

SERIAL NUMBER 077C7042401DATE TESTED July 11, 2022**1. MECHANICAL CHECKS**

- |  |                             |
|--|-----------------------------|
| A. Inspect and clean all fans and filters.                                       | <input type="checkbox"/> OK |
| B. Inspect and replace as necessary, all torch components including the RF coil. | <input type="checkbox"/> OK |
| C. Inspect all tubing for sign of clacking or leaking.                           | <input type="checkbox"/> OK |
| D. Adjust water and gas pressure regulator settings.                             | <input type="checkbox"/> OK |
| E. Inspect and leak check pneumatics drawers.                                    | <input type="checkbox"/> OK |
| F. Clean the exterior of the instrument.   | <input type="checkbox"/> OK |

**2. OPTICAL CHECKS**

- |   |                             |
|---|-----------------------------|
| A. Inspect and clean all optical components.        | <input type="checkbox"/> OK |
| B. As required, check and replace all purgefilters. | <input type="checkbox"/> OK |
| C. Recheck optical alignment.                       | <input type="checkbox"/> OK |

**3. COOLING SYSTEM CHECKS**

- |   |                              |
|---|------------------------------|
| A. Perform preventive maintenance on chiller. | <input type="checkbox"/> OK  |
| B. Flush out the chiller every year.          | <input type="checkbox"/> N/A |

**4. PERFORMANCE CHECKS**

- |                            |                             |
|----------------------------|-----------------------------|
| A. Torch View Alignment.   | <input type="checkbox"/> OK |
| B. Wavelength Calibration. | <input type="checkbox"/> OK |



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

SERIAL NUMBER : 077C7042401DATE TESTED : July 11, 2022

PARAMETER	SPECIFICATION			FINAL VALUE	
Spectral Resolution : UV	As 193.696 nm	≤ 0.007		0.00544	
	Ni 231.604 nm	≤ 0.008		0.00709	
	Ni 341.476 nm	≤ 0.012		0.00757	
Spectral Resolution : VIS	La 408.672 nm	≤ 0.020		0.01638	
	Ba 455.403 nm	≤ 0.025		0.02391	
Precision					
	As 193.656 nm	% RSD	< 1.0	0.91	%
	Zn 213.856 nm	% RSD	< 1.0	0.87	%
	Mn 257.610 nm	% RSD	< 1.0	0.76	%
	La 379.478 nm	% RSD	< 1.0	0.59	%
	Ba 455.403 nm	% RSD	< 1.0	0.53	%
	Ba 493.408 nm	% RSD	< 1.0	0.55	%
Detection Limits : Axial	Tl 190.080 nm	3(sd)		5.51	ppb
	As 193.696 nm	3(sd)		8.59	ppb
	Pb 220.353 nm	3(sd)		0.50	ppb
Detection Limits : Radial	As 193.696 nm	3(sd)		2.17	ppb
	Zn 213.856 nm	3(sd)		0.03	ppb
	Mn 257.610 nm	3(sd)		0.01	ppb
	La 379.478 nm	3(sd)		0.04	ppb
	Ba 455.403 nm	3(sd)		0.01	ppb
	Ba 493.408 nm	3(sd)		0.00	ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd 226.502 nm	≤ 150 ppb		12.46	
BEC : Radial (IB X 1000)/(IS-IB)	Mn 257.610 nm	≤ 45 ppb		30.82	



## MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV

SERIAL NUMBER 077C7042401DATE TESTED July 11, 2022**Remarks :**

Commissioning follow as commissioning performance sheets.

\_\_\_\_\_

\_\_\_\_\_

\_\_\_\_\_

\_\_\_\_\_

\_\_\_\_\_

\_\_\_\_\_

\_\_\_\_\_

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,  
including warranty terms.

**Service Department PerkinElmer Ltd.**

**Authorized Representative:**

( Mr. Wiphan Promlumda )

Service Engineer

ระดับความร้อนในสถานประกอบการ

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp° 46

SERIAL NO. : TSH120011

CLID. NO. : 232000795

JOB CONTROL NO. : 220505044292

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 05 May 2022

DATE OF ISSUED : 12 May 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Oranut Kamchatphai  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory

12 May 2022

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to  
the International System of Units (SI)

Certificate No. Q22044292

F3-011-04/01-12

page 1 of 3



@clccalibration

## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp° 46

SERIAL NO. : TSH120011

DATE OF CALIBRATION : 05 May 2022

---

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-74**. The calibration was performed by using  
Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 36151.  
Temperature & Humidity Chamber, PGC Model 9141-5114 S/N.0802282.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Thunder Scientific Corporation.  
Certificate No. 19317, Due Date 09 July 2022.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied  
by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. **Q22044292**

**F3-011-04/01-12**

page 2 of 3





**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter (thermal environment monitor).

## CALIBRATION DATA

### **\*1. CORRECTION OF TEMPERATURE [ WET ]**

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	29.99	31.4	-1.41	0.40
35.0	35.01	36.4	-1.39	
40.0	39.99	41.4	-1.41	

Note. \* means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

### **2. CORRECTION OF TEMPERATURE [ DRY ]**

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	29.99	30.0	-0.01	0.40
35.0	35.01	35.1	-0.09	
40.0	39.99	40.2	-0.21	

### **3. CORRECTION OF TEMPERATURE [ GLOBE BULB ]**

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	29.99	29.9	+0.09	0.40
35.0	35.01	34.8	+0.21	
40.0	39.99	39.6	+0.39	

Note. The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

**This report is valid for the above stated instrument/s only.**

**### End of Certificate ###**

Certificate No. Q22044292

F3-011-04/01-12

page 3 of 3



@clccalibration



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com


Heat B137\_1/22

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No.	: R14	Verification Date	: 04 September 2022
Brand	: 3M	Ambient Temp.	: 24.5 °C
Model	: QUESTemp <sup>®</sup> 46	Barometric Pressure	: 1011 mmbar
Serial No.	: TSH120011	Relative Humidity	: 49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C , DB = 47.1 °C , G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.4	0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.0	0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

  
(Mr. Peera Detudom)

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp° 46

SERIAL NO. : TSI0100006

CLID. NO. : 232000793

JOB CONTROL NO. : 220505044316

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 05 May 2022

DATE OF ISSUED : 12 May 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Oranut Kamchatphai

Calibration Engineer



Approved By :

Mongkol Yotsoontorn

Authorized Signatory

12 May 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22044316

F3-011-04/01-12

page 1 of 3



## REPORT OF CALIBRATION

### FOR

**NOMENCLATURE** : **DIGITAL THERMOHYGRO METER**  
**(THERMAL ENVIRONMENT MONITOR)**

**MANUFACTURER** : **3M**

**MODEL / TYPE** : **QUESTemp° 46**

**SERIAL NO.** : **TSI010006**

**DATE OF CALIBRATION** : **05 May 2022**

---

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-74**. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 36151.

Temperature & Humidity Chamber, PGC Model 9141-5114 S/N.0802282.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Thunder Scientific Corporation.

Certificate No. 19317, Due Date 09 July 2022.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. **Q22044316**

**F3-011-04/01-12**

page 2 of 3



## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter (thermal environment monitor).

### CALIBRATION DATA

#### \*1. CORRECTION OF TEMPERATURE [ WET ]

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	29.99	31.5	-1.51	0.40
35.0	35.01	36.5	-1.49	
40.0	39.99	41.5	-1.51	

Note. \* means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

#### 2. CORRECTION OF TEMPERATURE [ DRY ]

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	29.99	30.1	-0.11	0.40
35.0	35.01	35.0	+0.01	
40.0	39.99	40.1	-0.11	

#### 3. CORRECTION OF TEMPERATURE [ GLOBE BULB ]

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	29.99	30.1	-0.11	0.40
35.0	35.01	35.0	+0.01	
40.0	39.99	39.6	+0.39	

Note. The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q22044316

F3-011-04/01-12

page 3 of 3





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com.. www.spscon.com

Heat B147\_1/22

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No.	: R15	Verification Date	: 21 September 2022
Brand	: 3M	Ambient Temp.	: 24.5 °C
Model	: QUESTemp <sup>o</sup> 46	Barometric Pressure	: 1011 mmbar
Serial No.	: TSIO10006	Relative Humidity	: 49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C , DB = 47.1 °C , G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.4	0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.0	0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by :

Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

Peera Detudom

(Mr. Peera Detudom)

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp° 46

SERIAL NO. : TSH120025

CLID. NO. : 232000794

JOB CONTROL NO. : 220815082001

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 15 August 2022

DATE OF ISSUED : 20 August 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Oranut Kamchatphai  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
20 August 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to  
the International System of Units (SI)

Certificate No. Q22082001

F3-011-04/01-12

page 1 of 3



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp° 46

SERIAL NO. : TSH120025

DATE OF CALIBRATION : 18 August 2022

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-74**. The calibration was performed by using

Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.

Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Thunder Scientific Corporation.

Certificate No. 19944, Due Date 26 January 2023.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied

by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22082001

F3-011-04/01-12

page 2 of 3





**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel, 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter (thermal environment monitor).

### CALIBRATION DATA

#### \*1. CORRECTION OF TEMPERATURE [WET]

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	29.98	31.1	-1.12	0.40
35.0	34.98	36.2	-1.22	
40.0	40.00	41.2	-1.20	

Note. \* means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

#### 2. CORRECTION OF TEMPERATURE [DRY]

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	29.98	30.1	-0.12	0.40
35.0	34.98	34.9	+0.08	
40.0	40.00	39.9	+0.10	

#### 3. CORRECTION OF TEMPERATURE [GLOBE BULB]

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	29.98	30.1	-0.12	0.40
35.0	34.98	34.8	+0.18	
40.0	40.00	39.9	+0.10	

Note. The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q22082001

F3-011-04/01-12

page 3 of 3



@clccalibration



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Heat B137\_2/22

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No.	: R16	Verification Date	: 04 September 2022
Brand	: 3M	Ambient Temp.	: 24.5 °C
Model	: QUESTemp <sup>®</sup> 46	Barometric Pressure	: 1011 mmbar
Serial No.	: TSH120025	Relative Humidity	: 49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C , DB = 47.1 °C , G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.4	0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.0	0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by :

Adul Dangklom  
(Mr. Adul Dangklom)

Approved by :

Peera Detudom  
(Mr. Peera Detudom)