

เอกสารแนบ 6

เอกสารสอบเทียบเครื่องมือที่ใช้ในการวิเคราะห์

CERTIFICATE OF CALIBRATION

Certificate No.: C0-1908005/22 Page 1 of total 4 pages

Customer
WATER ANALYSIS CENTER CO., LTD.
30/5 Soi Vipavadee 60, Viphavadee Rangsit Road,
Kwaeng Taladbangkhen, Khet Laksi, Bangkok 10210

Equipment
pH Meter
Manufacturer
METTLER TOLEDO
Model
SevenCompact S220
Serial No.
B327527211
ID No.
WWL 0068
Description
Range : 0 - 14 pH, Resolution : 0.01 pH

Environmental Conditions
Ambient Temperature: (20 ± 2) °C
Relative Humidity: (50 ± 10) %
Atmospheric Pressure: -

Calibration Location
Jayhawks Laboratory (CL&GL)
Received Date
19 August 2022
Calibration Date
19 August 2022

Date of Issue
22 August 2022

Checked by [REDACTED]
Act as Technical Manager
Representative of Managing Director
() (Krisyosl K.) () (Sakda Y.)
() (Patiphan K.) () (Onnara P.)
() (Pongsak H.) () (Nitiiphong K.)
() (Kanung C.) () (Nonthachai K.)
() (Pramong P.) () (Noppol P.)
() (Dr. Ekachai Puritwong)

This calibration certificate shall not be reproduced other than in full except with the prior written approval of the Thai Heart Calibration Co., Ltd.

Certificate No.: C0-1908005/22

Page 2 of total 4 pages

Reference Method:

- The calibration method used was CP-178 based on an in-house method.
- This certificate can be traceable to the national standards, which is realized the shown measurement units according to the International System of Units (SI Units).

Reference Standard:

Type	pH Value	Lot No.	Due Date	Traceability
pH Standard Solution	4.01	081020	Jan. 22, 2023	NIMT
	7.01	020221	Jan. 18, 2023	
	10.00	091020	Feb. 7, 2023	

Type	Model	Serial No.	Certificate No.	Due Date	Traceability
Documenting Process Calibrator	753	3101007	10-0804001/22	Apr. 7, 2023	THC
Digital Thermometer with Sensor	1523 / 5622	1709138 / 4605984-005	10-1006004/22	Jun. 9, 2023	

Remark: This certificate is traceable to the International System of Unit (SI Unit) through:

- NIMT, National Institute of Metrology (Thailand).
- THC, Thai Heart Calibration Co., Ltd.

Measurement Results:

1. Function Simulated pH Meter

Standard Applied	Nominal Value	UUC Reading		Uncertainty
(mV)	(pH)	pH	mV	(± mV)
177.48	4.00	4.01	177.4	0.060
0.00	7.00	7.00	0.0	0.060
-177.48	10.00	10.01	-177.4	0.060

UUC : Unit Under Calibration

Note : Adjust Curve to simulate pH (4,7,10)

Certificate No.: C0-1908005/22

Page 3 of total 4 pages

Measurement Results (Cont.):

2. Calibration of pH Electrode (Serial No.: 3322791)

pH Standard Solution (pH)	Measured Value		Uncertainty (± pH)
	(pH)	(mV)	
4.01	4.01	185.9	0.013
7.01	7.01	9.3	0.013
10.00	10.01	-164.9	0.013

Note : Adjust Curve to Buffer Solution pH (4,7,10)
Temperature stability of micro bath : $25 \pm 0.2^{\circ}\text{C}$

The above reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

Certificate No.: C0-1908005/22

Page 4 of total 4 pages

Reference Method:

- The calibration method used was CP-096 based on an in-house method.
- The temperature scale used was an ITS-90.
- This certificate can be traceable to the national standards, which is realized the shown measurement units according to the International System of Units (SI Units).

Reference Standard Instruments:

Type	Model	Serial No.	Cert. No.	Due Date	Traceability
Thermometer Readout	1529-R	B7C853	10-1011001/21	Nov. 10, 2022	THC
Platinum Resistance Thermometer	5626	4854	C0A30047	Oct. 22, 2023	FLUKE
Liquid Bath	XORTS-40A	XO111019	10-0306002/21	Jun. 3, 2023	THC

Remark: This certificate is traceable to the International System of Unit (SI Unit) through:

- THC, Thai Heart Calibration Co., Ltd.
- FLUKE, Fluke Corporation, U.S.A.

Measurement Results:

(X) Without Adjustment

Dimension of probe : Diameter 4 mm. Sensor Type : RTD (PT100)

Immersion Depth (mm.)	Standard Reading ($^{\circ}\text{C}$)	UUC Reading ($^{\circ}\text{C}$)	Correction ($^{\circ}\text{C}$)	Uncertainty ($\pm ^{\circ}\text{C}$)
120	22.00	22.0	0.00	0.060
120	25.00	25.0	0.00	0.060
120	28.00	28.0	0.00	0.060

UUC : Unit Under Calibration

The above reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

Calibrated by

Instrument : DO Meter
Model : DO-31P
Serial No. : 780065

Calibrate Procedure

- ☐ This instrument was calibrated by comparison with standard solution (PH/ORP)
 - ☐ This instrument was calibrated by comparison with scattering plate value (Turbidity)
 - ☐ This instrument was calibrated by comparison with conductivity (Conductivity)
 - ☒ This instrument was calibrated by comparison with Sodium sulfite anhydrous (DO)
- Condition of this result of calibration
1). Reference Standard Solution

Standard Lot No Batch Cert. No. Due Date
Sodium Sulfite Power 1.06657.0500 K52300357 - 31 Mar 2022

- 2). Traceability This certification is traceable to
☒ Merck KGaA 64271 Darmstadt
☐ DKK Corporation

Result Of Calibration

Standard Solution (mg/l) at 26.0°C	Before Adjust		After Adjust	
	Indicator	Error	Indicator	Error
Zero	0.00	+ 0.10	0.00	-
Span	7.99	+ 0.22	7.99	-

DO Electrode No. OE270AA(5) S/N 111F0029

Calibrated By 
(Ms. Phanee Yooyen)
Technician

929/929/ Sol Pattanakarn 30, Pattanakarn Rd., Suanluang, Bangkok 10250
Head Office : Tel. 02-319-9994 ext.1 Fax.02-319-4961 E-mail : ats@automation.co.th
Ravong Branch : 1/15 Huayong Rd., A. Muang, Rayong 21150 Tel. 038-692-152 Fax. 038-692-345
Lamphun Branch : 122/5 M.4, T.Ban Klang, A.Muang, Lamphun 51000 Tel/Fax. 053-584-876
website : www.automation.co.th

SV 212001/2021

Cert. No. WAC-065
Page 1 of 2

CERTIFICATE OF CALIBRATION

Instrument : DO Meter Machine : -
Model : DO-31P Location : -
Serial No. : 780065
Manufacturer : TOA-DKK
Measuring Range : 0.00 ~ 20.00 mg/l

Customer : Water Analysis Center Co.,Ltd.
1/94 Moo.5 T.Kanham, A.U.-Thai
Ayutthaya 13210 Thailand

Date Of Received : 03 / 12 / 2021
Date Of Calibration : 03 / 12 / 2021

Ambient Condition : Temperature 24 °C
Humidity 47 % RH

Calibrated By : 
(Ms. Phanee Yooyen)

Approved By : 
(Mr. Phongsak)
Technical Manager

Date Of Issue : 03 / 12 / 2021

This Certificate may not be reproduced other than in full, except with the prior written approval of the head of the industrial instruments calibration center.

Certificate No.: MC 2207678

Page 2 of 3

The Reference Standard :

Description	Certificate No.	Serial No.	Due date
Data Acquisition/Switch Unit	MC 2114432	MY44096104	20 December 2022
With Thermocouple Type " T " ID. No.2/1 to 2/9			

This certificate is traceable to the international system of units maintained at:

- Master Calibration Co., Ltd.

1. Calibration Procedure:

This instrument was calibration according to TLAS G-20 by comparison with calibrated thermocouple type T under no load condition. The Thermocouples were placed on nine points and located one thermocouple in each of the eight corners of the chamber and was away from the each wall of 5 cm to 10 cm. And placed the ninth thermocouple within 2.5 cm of the geometric center of the chamber.

Temperature Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.

Temperature Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.

Overall Variation - The Difference of the maximum and minimum measured temperatures throughout observation.

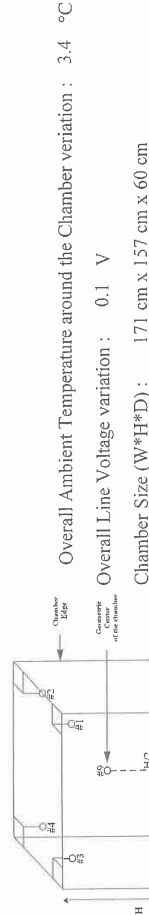


Figure 1 : Sensor Installation Location

Checked

[MCF-Q-077 ; Rev.6 ; Date : 22/04/2021]



**TEMPERATURE
CONTROLLER ENCLOSURES**


Certificate No.: MC 2207678

Page 1 of 3



Customer	Water Analysis Center Co., Ltd.	Received Date	12 July 2022
Reference Job No.	22-1601		
Description	Refrigerator		
Manufacturer	SANDENINTERCOOL	Model	SEC-1500SBD
Serial No.	SEC1500201A-0708-00304	ID. No.	WWL0038
Marking	Additionally for the purpose of identification by this laboratory a label marked with this certificate number (MC 2207678) has been attached to the case.		
Method	In-House calibration procedure MWI-T-033 this method is reference to TLAS G-20 "Temperature Controlled Enclosures".		
Location of Calibration	Water Analysis Center Co., Ltd. ; Laboratory.		
Environmental Conditions	Ambient Temperature : (25.8 to 27.5) °C		
	Relative Humidity : (48.8 to 52.2) %		
Date of Calibration	12 July 2022	Date of Issue	19 July 2022

Checked by

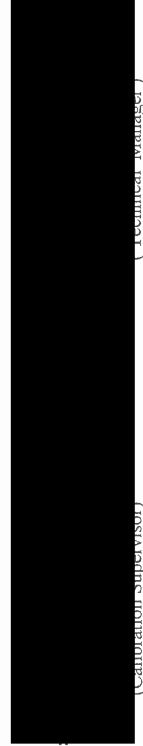

(Calibration Supervisor)

The uncertainties are for a confidence probability of approximately 95%

This certificate is issued in accordance with the conditions of accreditation granted by the National Standardization Council of Thailand-Office of the National Standardization Council that has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of Master Calibration Co.,Ltd.

[MCF-Q-077 ; Rev.6 ; Date : 22/04/2021]

Certificate No.: MC 2207678

Page 3 of 3

2. Result of calibration :

Temperature Measurement Accuracy Test

Indicating Temperature (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (±°C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. #9	
2.5	3.5	3.6	3.7	3.5	3.6	3.4	3.4	3.3	3.4	1.1

Chamber Characterization Result

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
2.0	2.5	1.5	0.6	3.1

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

This report will certify of the calibrated equipment only.

End of Certificate

Checked by :

[MCF-Q-077 ; Rev.6 ; Date : 22/04/2021]

Certificate of Calibration



TEMPERATURE
CONTROLLER ENCLOSURES

Certificate No.: MC 2203933

Page 1 of 3



Customer : Water Analysis Center Co., Ltd.
1/94 Moo 5, T. Kantham, A.U.-Thai, Ayutthaya 13210.

Reference Job No. : 22-0740 Received Date : 24 March 2022
Description : Oven

Manufacturer : Memmert Model : UF260
Serial No. : B620.0814 ID. No. : WWL0212
Marking : Additionally for the purpose of identification by this laboratory a label marked with this certificate number (MC 2203933) has been attached to the case.

Method : In-House calibration procedure MWI-T-033 this method is reference to TLAS G-20 "Temperature Controlled Enclosures".

Location of Calibration : Water Analysis Center Co., Ltd. ; Laboratory.

Environmental Conditions : Ambient Temperature : (30.5 to 32.6) °C

Relative Humidity : (56.2 to 61.2) %

Date of Calibration : 24 March 2022 Date of Issue : 28 March 2022

Checked by :

[Signature]
(Calibration Supervisor) (Technical Manager)

The uncertainties are for a confidence probability of approximately 95%

This certificate is issued in accordance with the conditions of accreditation granted by the National Standardization Council of Thailand-Office of the National Standardization Council that has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of Master Calibration Co.,Ltd.

Certificate No.: MC 2203933

Page 2 of 3

The Reference Standard :

Description	Certificate No.	Serial No.	Due date
Data Acquisition/Switch Unit With Thermocouple Type " T " ID. No.30/1 to 30/9	MC 2106035	93000641	8 August 2022

This certificate is traceable to the international system of units maintained at:

- Master Calibration Co., Ltd.

1. Calibration Procedure:

This Instrument was calibration according to TLAS G-20 by comparison with calibrated thermocouple type T under no load condition. The Thermocouples were placed on nine points and located one thermocouple in each of the eight corners of the chamber and was away from the each wall of 5 cm to 10 cm. And placed the ninth thermocouple within 2.5 cm of the geometric center of the chamber.

Temperature Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.

Temperature Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.

Overall Variation - The Difference of the maximum and minimum measured temperatures throughout observation.

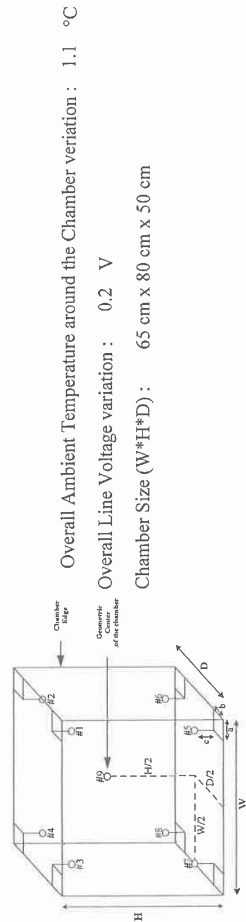


Figure 1: Sensor Installation Location

Checked by

Certificate No.: MC 2203933

Page 3 of 3

2. Result of calibration :

Temperature Measurement Accuracy Test

Indicating Temperature (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (±°C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. #9	
104.0	103.9	103.9	103.9	104.1	104.3	104.2	104.2	104.1	104.0	0.67
180.0	179.3	179.3	179.3	179.5	180.1	180.3	180.5	180.4	180.1	0.99

Chamber Characterization Result

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.0	0.27	0.45	0.92
180.0	180.0	0.29	1.00	1.65

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

This report will certify of the calibrated equipment only.

End of Certificate

Checked by



Certificate of Calibration

Equipment: Balance
Model: BL210S
Serial No. (or ID.): 15808131 (WWL 0022)
Manufacturer: Sartorius
Condition: In condition

Certificate No.: C01221685
Issued Date: 08 June 2022
Job No.: KSPR2206906
Page: 1 of 2

Customer: Water Analysis Center Co., Ltd.
1/94 Moo 5, Rojana Industrial Park, Rojana Road,
Tambol Kanham, Amphur U-Thai, Ayutthaya 13210 Thailand

Environment Condition: Temperature 27 °C ± 0.5 °C
Humidity 42 %RH ± 4.7 %RH

Calibration Place: Water Analysis Center Co., Ltd. (ห้างเครื่องชั่ง)
1/94 Moo 5, Rojana Industrial Park, Rojana Road,
Tambol Kanham, Amphur U-Thai, Ayutthaya 13210 Thailand

Calibration By: Mr. Preecha Phoarsai
Calibration Date: 08 June 2022

The Method used: In-house method, SPCC-WI-47, based on UKAS Lab 14
Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through SPC RT Co., Ltd. Certificate No. C02220794



(Mr. Preecha Phoarsai)

SPC RT Co., Ltd.

(Mr. Rungrod Jenkitrakulchai)

Person in charge

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to International or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SPC RT Co., Ltd.

Calibration Results:

Without Adjustment

Eccentric Error: Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.

	Nominal Test Value					(g)
	A	B	C	D	E	
	-	0.0001	0.0001	-0.0002	-0.0002	-0.0002

Repeatability: Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
20	0.00004
200	0.00004

Error of Indication from nominal or conventional mass value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Error of Indication (g)	Uncertainty (g)	k
1	0.99998	1.0000	0.0000	0.000097	2.02
2	1.99999	2.0000	0.0000	0.000098	2.02
5	5.00000	5.0000	0.0000	0.000099	2.02
10	10.00002	10.0000	0.0000	0.00010	2.02
20	19.99995	20.0000	0.0000	0.00011	2.01
50	50.00002	50.0000	0.0000	0.00012	2.01
70	69.99997	70.0000	0.0000	0.00015	2.00
100	100.00007	100.0001	0.0000	0.00017	2.00
120	120.00002	120.0000	0.0000	0.00020	2.00
150	150.00009	150.0002	0.0001	0.00023	2.00
200	199.99993	200.0003	0.0004	0.00029	2.00

The End of Certificate



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No.

BSCC-UV-149/22

Equipment

UV/Vis Spectrophotometer

Model

UV-1800

Manufacturer

Shimadzu

Serial No.

A11635405598CD

ID No.

WWL0082

Date of receipt

29 April 2022

Date of calibration

29 April 2022

Date of issue

6 May 2022

Customer name

Water Analysis Center Co., Ltd.

Address

1/94 Moo 5, T.Kantham, A.Uthai, Ayuthaya 13210

Temperature

(29.9-31.8) °C (On site)

Humidity

(48.7-52.6) %RH (On site)

Equipment condition

Good Operation

Calibration Location

Laboratory Room Water Analysis Center

Calibration Procedure

In-house method WI-UV-702-01 based on ASTM E275-01

Traceability

Wavelength Accuracy is traceable to certificate No. 95917 and 95918

Photometric Accuracy is traceable to certificate No. 95924 and 95937

Stray Light is traceable to certificate No. 95908


The above certificate are traceable to SI unit through Starna Scientific Ltd.

(UKAS accredited calibration laboratory NO. 0659)

Calibrated by

Mr.Waruth Janphung

Approved by



Mr.Kanchit Choothep
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Number of Page(s) 2 of 3

Certificate No.

BSCC-UV-149/22

Calibration Results:

1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
360.89	360.86	-0.03	0.18
418.53	418.72	0.19	0.18
445.82	446.51	0.69	0.18
453.67	453.56	-0.11	0.18
459.99	459.81	-0.18	0.18
638.00	638.17	0.17	0.18
431.22	431.52	0.30	0.18
513.39	513.60	0.21	0.18
528.90	528.80	-0.10	0.18
572.99	576.13	3.14	0.18
585.25	585.30	0.04	0.18
684.50	684.68	0.18	0.18
741.02	741.22	0.20	0.18
879.41	879.30	-0.11	0.18

2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	CNR	CNR	CNR	CNR
257	CNR	CNR	CNR	CNR
313	CNR	CNR	CNR	CNR
350	0.0000 0.6429	0.0000 0.6404	0.0000 -0.0025	0.0075 0.0075

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประดิษฐ์มิตรไทย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200
80-82 Prachathipatani Rd., Bangkokphrom, Pranakorn, Bangkok 10200
Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thnwat@thaiunique.com, Website : www.thaiunique.com

Electronics

- ☒ Check power supply voltage
- ☒ Check cables and connectors
- ☒ Check/Clean all boards in the instrument
- ☐ Furnace, Check camera and align** N/A

**Option for Graphite Zeeman only

Mechanisms

- ☒ Flame, Check the burner adjuster
- ☐ Furnace, Check PSD accessories N/A

Analytical performance

- ☒ Clear the sample compartment
- ☒ Flame, Check uptake rate form 7.2-10.6 mL per minute = 9.5 mL/min
- ☒ Test Photometric noise, STDV = 0.0003 Abs (should be ≤ 0.00050 Abs)
- ☒ Flame, Test high solids nebulizer setting use

-Air/acet Cu 5 ppm = 0.77 Abs, and Precision
(%RSD) = 0.4 % (should be > 0.55 Abs and $< 0.5\%$ RSD)

or

-N2O/Acet Cu 5 ppm = Abs, and Precision
(%RSD) = (should be > 0.3 Abs and $< 0.5\%$ RSD)

- ☐ Furnace, Characteristic mass and sensitivity Cu 25 ppb = N/A Abs, and Precision (%RSD) = % (should be ≥ 0.15 Abs and $\leq 4.0\%$ RSD)

SIGN :

Engineer

Customer : Kent
(.....)

SVD Results Report

VARIAN

Report ID:1 Diagnostic Start Time:10/2/2022 11:56:32 Diagnostic End Time:10/2/2022 12:36:59

Customer: Water Analysis Center Co., Ltd. Service Engineer: Suriya Nacharoen
Address: Ayuthaya Contact Details: Kanitsaya

Instrument Configuration

Configuration:

Serial Number: AA0911M073 Turret Type: Automatic
Instrument Model: Varian AA140/240/280 Number Of Lamps: 4
Flame Instrument: True Mono Type: Automatic
Furnace Instrument: True Gasbox Type: Y Gas Box
Zeeman Present: False Auto Burner Adjuster: False
Internal Zeeman: False Mains Frequency: 50
Internal UltraAA: False Firmware Version: 2.12
Optics Type: Double Beam Photomultiplier Type: Normal(900nm)
D2 BG Correction Fitted: True PWB Version: 181
Boot Block Version: 2.02

EEPROM Data:

Instrument Run Hours: 29533.551 D2 Run Hours: 4026.533
Zero Wavelength Offset: -18.735 D2 Serial Number: not set
Mono Correction: -0.360 D2 Install Date: 1/1/1970
Flame Hours: 7417.833 D2 Original Intensity: 1.000
D2 Last Intensity: 678.000

Frequency:

Averaging Period: 30.0
Datapoint Count: 20

Upper Limit:
51.00

Highest Measured Frequency:
50.00

Average Frequency:
50.00

Lower Limit:
49.00

Lowest Measured Frequency:
50.00

Result: Passed

Power Supply:

Averaging Period: 30.0
Datapoint Count: 20


	Lower Limit (V)	Actual (V)	Upper Limit (V)	Result:
12.00V Rail	10.80	12.20	13.20	Passed
-12.00V Rail	-13.20	-12.00	-10.80	Passed
5.00V Rail	4.50	5.10	5.50	Passed
310.00V Rail	279.00	318.00	341.00	Passed

Optics


Beam Balance:

Lamp Type: Copper
Lamp Socket Used: 3
Peak Selected: 324.80
Lamp Alignment: Performed

'X' Lamp Screw

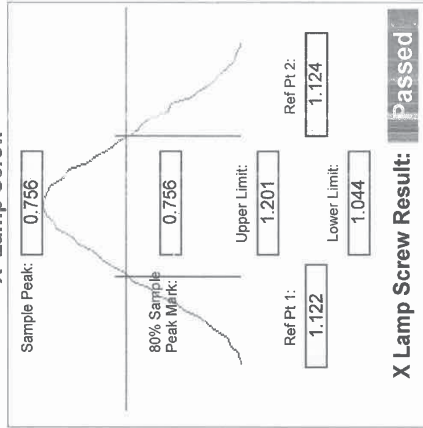

'Y' Lamp Screw

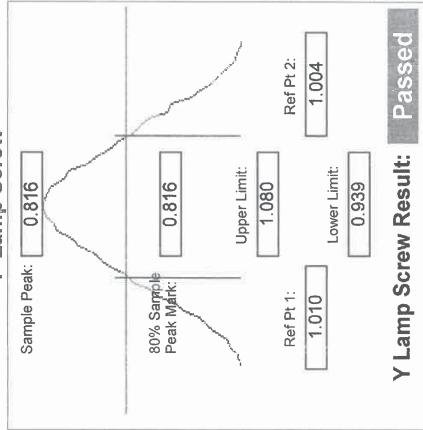

Grating Squareness:

Lamp Element(s): Copper
Lamp Turret Position: 3
Lamp Current(mA): 4.00
Slit Width(nm): 0.5
1st Order Wavelength(nm): 324.80
Lamp Alignment: Performed

	Lower Limit (nm)	Actual (nm)	Upper Limit (nm)	Result:
Zero Order	-0.10	0.00	0.10	Passed
First Order	324.45	324.74	325.15	Passed
Second Order	649.23	649.56	649.97	Passed

Wavelength Repeatability:

Lamp Used: Copper
Peak Used(nm): 324.750
Connected to Socket: 3
Lamp Current(mA): 4
Slit Width(nm): 0.2
Slit Height: Normal

Lamp Alignment: **Performed**
Lower Limit(nm) 324.759
Upper Limit(nm) 324.879

(Approach from Zero Order)
Sample 1: 324.819
Sample 2: 324.811
(Approach from end)
Sample 3: 324.819
Sample 4: 324.811
Sample 5: 324.815
Sample 6: 324.811
Sample 7: 324.819
Sample 8: 324.815
Sample 9: 324.819
Sample 10: 324.819

Mean: 324.816
Standard Deviation: 0.004

Result: **Passed**

Mechanical

Wavelength Drive: **Passed**

Slit Drive: **Passed**

Turret Drive: **Passed**

Auto Burner Adjuster Drive: **Untested**

Miscellaneous

Signal Processing Linearity:

Calculate Mode: New Calc Mode

	Lower Limit	Actual	Upper Limit	Result:
S0	114	248	297	Passed
S1	156	165	191	Passed
S2	271	293	332	Passed
S3	474	504	579	Passed
S4	825	904	1008	Passed
S5	1435	1510	1754	Passed
S6	2498	2711	3053	Passed
S7	4347	4658	5313	Passed

Interlocks:

Burner Fitted: **Working**
N2O Burner Fitted: **Working**
Flame Shield Closed: **Working**
Gas Control Fitted: **Untested**
Pressure Release Bung Fitted: **Working**
Liquid Trap Fitted: **Working**
Flame Detect: **Working**
GCU Active: **Working**
Oxidant Pressure: **Working**
Oxidant Changeover: **Working**
Ignition: **Working**

Auto Lamp Recognition:

Lamp 1: Uncoded Lamp/Not Connected

Lamp 2: Uncoded Lamp/Not Connected

Lamp 3: 14 - Copper (Cu)

Lamp 4: Uncoded Lamp/Not Connected

Lamp 5: Not Supported

Lamp 6: Not Supported

Lamp 7: Not Supported

Lamp 8: Not Supported

Result:

Passed

GTA Temperature Monitoring:

Not Performed

Notes:

C2202SU09_1
PM 10 Feb 2022

Signatures:

[Redacted Signature]

Water Analysis Center Co., Ltd Date

Suriya Nacharoen

Date

022



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประจักษ์ศิลปาคม แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipat Rd., Bangkokkhunprom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawit@thaiunique.com, Website : www.thaiunique.com

PREVENTATIVE MAINTENANCE (PM) CHECK LIST

FOR ATOMIC ABSORPTION SPECTROMETER

Model & Serial Number: 2402 AA X M918250004

Customer : ด.ช.วิฑูรย์ น. น. ๑๓.

Date: 29 Jan. 22

Safety

- ☐ Flame, Inspect/replace o-ring nebulizer, spray chamber and burner N/A
- ☐ Flame, Clean nebulizer, spray chamber and burner N/A
- ☐ Flame, Check liquid trap interlock, burner interlock, pressure relief bung interlock and shield interlock N/A

- ☒ Furnace, Clean work head, electrode and shroud

- ☒ Furnace, Clean PSD and PSD tray N/A

- ☒ Furnace, Check water pressure

- ☒ Check drain tube

- ☒ Check exhaust system

- ☒ Check gas pressure sensor interlock

- ☒ Check and all gas hoses for SpectrAA

- ☒ Clean computer control

Optics

- ☒ Inspect/Replace that external optics surfaces

- ☒ Check Wavelength Accuracy the copper line at 323.0-326.0 nm = 324.7 nm

- ☒ Check that PMT % Gain the copper at 324.8 nm, 4 mA, 0.5 nm slit width, Gain = 49% (should be $\leq 64\%$ or $\leq 380V$)

- ☐ Flame, Check D2 lamp is work N/A



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาวิทย์ แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200
80-82 Prachathipat Rd., Bangkokphrom, Pranakorn, Bangkok 10200
Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thavai@thaiunique.com, Website : www.thaiunique.com

Electronics

- ☒ Check power supply voltage
- ☒ Check cables and connectors
- ☒ Check/Clean all boards in the instrument
- ☒ Furnace, Check camera and align**

**Option for Graphite Zeeman only

Mechanisms

- ☒ Flame, Check the burner adjuster
- ☒ Furnace, Check PSD accessories

Analytical performance

- ☒ Clear the sample compartment
 - ☒ Flame, Check uptake rate form 7.2-10.6 mL per minute = N/A mL/min
 - ☒ Test Photometric noise, STDV = 0.0001 Abs (should be ≤ 0.00050 Abs)
 - ☒ Flame, Test high solids nebulizer setting use
 - ☒ -Air/acet Cu 5 ppm = N/A Abs, and Precision (%RSD) = N/A % (should be > 0.55 Abs and < 0.5 % RSD)
- or
- ☒ -N2O/Acet Cu 5 ppm = N/A Abs, and Precision (%RSD) = N/A % (should be > 0.3 Abs and < 0.5 % RSD)
 - ☒ Furnace, Characteristic mass and sensitivity Cu 25 ppb = 0.22 Abs, and Precision (%RSD) = 2.4 % (should be ≥ 0.15 Abs and ≤ 4.0 % RSD)

SIGN :
Engineer

Customer :



MEGAFIL CO., LTD.
99/183 Moo 3 Tambon Bang Rak Noi Amphur Mueang Nonthaburi 11000
Tel. 0-2528-6081-2 Fax. 0-2528-6083, 0-2525-7034
www.megafil.co.th E-mail : megafil.group@gmail.com

BSC Certification Test Report

Certificate No. : M01075/22

Customer Name : LABORATORY WATER ANALYSIS CENTER COMPANY LIMITED

Customer Address : 1/94 Moo 5 T.Kanharm, A.U-Thai,
Phra Nakhon Si Ayutthaya 13210

Equipment : Biological Safety Cabinet Class II Type A2

Manufacturer : Microtech

Model : V6-T

Serial No : 0972

ID No. : WWL0084

Were in accordance with ☒ EN 12469 ☐ NSF 49 ☐ Manufacturer's specification

Test Date : 23/09/2022

Due Date : 23/09/2023

or after HEPA filters are replaced or unit is moved

Test by : Mr. Piyaong Pusua

Approved by :

(Mr.Krudsada Thinhuatoci)
Authorized Signatory

Issued Date : 26/09/2022

This calibration certificate documents the traceability to national standards, which realize the unit of measurement according to the International System of Units (SI).

This certificate may not be reproduced other than in full except with the prior written approval of the Megafil Company Limited.

Certificate No. : M01075/22

Procedure Used :

- European Standard EN12469 : 2000 has the status of British Standard, Biotechnology Performance criteria for microbiological safety cabinets.
- NSF International Standard / American National Standard NSF / ANSI 49-2008 Biosafety Cabinet : Design, Construction, Performance and Field Certification.
- Australian Standard : AS 1807.23-2000 Determination of intensity of radiation from germicidal ultraviolet lamps.
- Manufacturer's specification.

1. Downflow velocity test.

Measurement Information

No. of Rows	No. of Readings	Grid Spacing Front-Back	Grid Spacing Side-Side	Probe height Above sash
2	8	1/4, 3/4	1/8, 3/8	100mm

Measurement Data.

0.36	0.42	0.43	0.41
0.40	0.34	0.34	0.33

Average velocity **0.38** m/s (**75** FPM.) Velocity range **0.25-0.50** m/s (**49-98** FPM.)

Uniformity(EN: +/-20%avg.) **0.30 - 0.46** m/s (**60 - 90** FPM.)

Supply filter dimension **24 x 72** (inch x inch) Supply filter area **10.69** SQ.FT

Downflow volume (Q) **802** CFM.

Result Summary ☒ Pass ☐ Fail

Equipment used : Thermo Anemometer Model 425 S/N : 02623979 Calibration date : 14/07/2022

Certificate No. : M01075/22

2. Inflow velocity test.

Select method. : ☐ DIM ☒ Exhaust velocity. ☐ MFG's Specifications

0.53	0.47	0.48	0.50	0.51
0.57	0.46	0.52	0.53	0.50
0.54	0.57	0.55	0.52	0.53
0.53	0.51	0.57	0.54	0.51
0.51	0.48	0.53	0.55	0.56

Average Inflow velocity **0.44** m/s (**86** FPM.) Velocity range **>0.40** m/s (**≥79** FPM.)

Inflow dimension **8 x 72** (inch x inch) Inflow area **4.00** SQ.FT

Inflow volume(Q) **344** CFM

Result Summary ☒ Pass ☐ Fail

Adjustments Required ☐ Fan Speed ☐ Damper

Equipment used : Thermo Anemometer Model 425 S/N : 02623979 Calibration date : 14/07/2022

3. HEPA filter leak test.

Measurement Data

HEPA Filter	PAO Upstream Conc.(calculated)	Specification	Measured leak penetration
Supply HEPA Filter	18 µg/l.	<0.003%	<0.003%
Exhaust HEPA Filter	18 µg/l.	<0.003%	<0.003%

Certificate No. : M01075/22

Leak location

Supply HEPA Filter

Back



Exhaust HEPA Filter

Back



Result Summary ☒ Pass ☐ Fail

Equipment used : Aerosol Photometer Model 2I S/N : 26468 Calibration date 14/07/2022

Equipment used : Smoke Generator Model TDA-6D S/N : 26530

4. Airflow smoke patterns test

Measurement Information

1. Downflow Pattern test : Smoke shall be passed from one end of the cabinet to the other, along the centerline of the work surface, at a height of 4 inch (10 cm) above the top of the access opening
2. View screen retention test : Smoke shall be passed from one end of the cabinet to the other, 1.0 in (2.5 cm) behind the view screen, at a height 6.0 inch (15 cm) above the top of the access opening.
3. Work opening edge retention test : Smoke shall be passed along the entire perimeter of the work opening
Particular attention should be paid to corners and vertical edges.
4. Sash/window seal test : Smoke shall be passed up the inside of the window 2 in (5 cm) from the sides and along the top of the work area.

Certificate No. : M01075/22

Result Summary

Downflow Pattern test	<input checked="" type="checkbox"/> Accept	<input type="checkbox"/> Non-Conforming
View screen retention test	<input checked="" type="checkbox"/> Accept	<input type="checkbox"/> Non-Conforming
Work opening edge retention test	<input checked="" type="checkbox"/> Accept	<input type="checkbox"/> Non-Conforming
Sash/window seal test	<input checked="" type="checkbox"/> Accept	<input type="checkbox"/> Non-Conforming

5. Site installation

Sash Alarm.	<input type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> N/A
Interlock System.	<input type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> N/A
Exhaust System Performance	<input type="checkbox"/> Pass	<input type="checkbox"/> Fail	<input checked="" type="checkbox"/> N/A

Remark / Recommendation

ระบบ Site installation ไม่มีการตรวจสอบ เนื่องจากตู้ไม่พียงกัน

6. Illumination Test (Lighting) : Option

Lighting should be adequate for safe working within the cabinet. Illumination measured at the work surface.

Lux

620	965	938	561
867	1446	1492	768

Remark :

Certificate No. : M01075/22

7. Ultraviolet Lamp Test (UV) : Option

Ultraviolet radiation where UV Lamp are fitted, the intensity of radiation at a wavelength of 254 nm.
Shall be not less than 400 mW/m² when measures at work floor surface.

mW/m²

720	1510	1540	760
470	980	990	450

Remark :

-000-