



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY CO., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yeak 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com


CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

CORRECTION OF TEMPERATURE

DUC Setting (°C)	Position	STD Reading (°C)	Correction (°C)	Uncertainty \pm (°C)
150	A1	152.2	+ 2.2	0.8
	A2	152.3	+ 2.3	
	A3	152.5	+ 2.5	
	A4	152.8	+ 2.8	
	A5	152.4	+ 2.4	
	B1	152.9	+ 2.9	
	B2	154.2	+ 4.2	
	B3	154.3	+ 4.3	
	B4	154.5	+ 4.5	
	B5	153.0	+ 3.0	
	C1	152.9	+ 2.9	
	C2	154.5	+ 4.5	
	C3	154.2	+ 4.2	
	C4	154.4	+ 4.4	
	C5	153.4	+ 3.4	
	D1	153.5	+ 3.5	
	D2	153.9	+ 3.9	
	D3	154.4	+ 4.4	
	D4	154.0	+ 4.0	
	D5	153.3	+ 3.3	
	E1	152.7	+ 2.7	
	E2	153.6	+ 3.6	
	E3	153.6	+ 3.6	
	E4	153.1	+ 3.1	
	E5	153.3	+ 3.3	

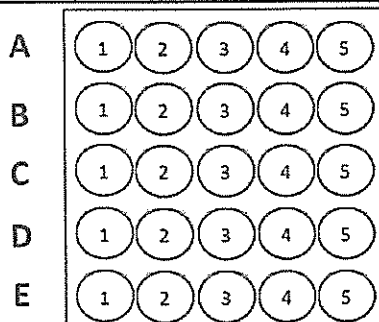

The picture show DUC Position

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q21062182

