

ภาคผนวกที่ 4

ใบรับรองการสอบเทียบเครื่องมือ



National Institute of Metrology (Thailand)

Certificate of Calibration



Certificate No. : AA-2018-22
Issued by : Acoustics Laboratory
Acoustics and Vibration Group



Page 1 of 5 pages

MEASUREMENT ITEM : Sound Calibrator
MANUFACTURER : RION
MODEL/TYPE : NC-75
SERIAL NUMBER : 34480442
CUSTOMER : MET Co., Ltd.
36/659 Moo 6, T. Bangrakphatthana,
A. Bangbuathong, Nonthaburi 11110
MEASUREMENT DATE : 28 September 2022

The reported measurement result relates only to the measurand and applies only at the time of measurement.

*The calibration results only marked with an asterisk * in this certificate are not included in the scope of accreditation.*

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%. This calibration certificate may not be reproduced other than in full except with the permission of the Director of National Institute of Metrology (Thailand).

| Reference | Date | Authorized Signatory | Person in charge |
|---------------|-------------------|---|--|
| AUVC844-01/22 | 29 September 2022 |  (Dr. Charun Yafa) |  (Sawitri Srisatjarak) |

This certificate is consistent with the capabilities that are included in Appendix C of the MRA drawn up by the CIPM. Under the MRA, all participating institutes recognize the validity of each other's calibration and measurement certificates for the quantities, ranges and measurement uncertainties specified in Appendix C (for details see <http://www.bipm.org>).

National Institute of Metrology (Thailand)

Ministry of Higher Education, Science, Research and Innovation

3/4-5 Moo 3, Klong 5, Klong Luang, Pathumthani 12120, Thailand. Tel: (66) 2577 5100, Fax: (66) 2577 3659

75/7 Rama VI Road, Rachathewi, Bangkok 10400, Thailand. Tel: (66) 2354 3700, Fax: (66) 2354 3692



UNCERTAINTY OF MEASUREMENT

The stated uncertainty is the expanded uncertainty obtained by multiplying the standard uncertainty by the coverage factor $k=2$. It has been determined in accordance with EA publication EA-4/02 M:2013 "Evaluation of the Uncertainty of Measurement in Calibration" and JCGM 100:2008 "Evaluation of measurement data --Guide to the Expression of Uncertainty in Measurement (GUM 1995 with minor corrections)". The value of the measured lies within the assigned range of value with a probability of 95 %.

| Parameter | Uncertainty at SPL94 dB | Maximum-permitted uncertainty of measurement for a coverage probability of 95% |
|------------------------|----------------------------|---|
| 1.Sound Pressure level | 0.08 | 0.15 |
| 2. Frequency | 0.1 | 0.2 |
| 3. THD+N | 0.1 | 0.5 |

TRACEABILITY

This certificate provides traceability of measurement to recognized national standards, and to the realization of the International System of Units (SI).



ENVIRONMENTAL CONDITIONS

Ambient condition in the laboratory are as follows :

| | | | |
|-------------------|---|-----------------------|-----|
| Temperature | : | (23.0 ± 1.0) | °C |
| Pressure | : | (101.325 ± 1.500) | kPa |
| Relative Humidity | : | (50.0 ± 15.0) | % |

Reference Condition : 101.325 kPa , 23.0 °C and 50.0 %RH.

Calibration Condition

Preconditionings : 16 hours at ambient conditions.

Measurement Conditions : The average values during measurement are
 (100.313 ± 0.014) kPa, (22.0 ± 0.3) °C and (57.0 ± 2.1) %RH

MEASUREMENT METHOD

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone. The insert voltage technique was employed and the measurement procedure was based on IEC 60942-2017.

Reference Microphone

4180 serial no.1395446

TABULATION OF RESULTS

The following tables give the calibration results and associated measurement uncertainties at 95% of confidence level. The calibration results of sound pressure level which quoted in dB with reference to 20 µPa are corrected to the values under the reference environmental conditions.

The calibration results exclude the calibrator pressure correction but include the microphone volume correction, which was obtained from the manufacturer instruction manual of the sound calibrator, at the level of 94 dB.



MEASUREMENT RESULTS

1. Sound pressure level

| Specified sound pressure level (dB) | Measured value (dB)* | Deviated value ^[1] (dB) | Acceptance Limit (dB) |
|--|----------------------|------------------------------------|-----------------------|
| Microphone 4180 Serial No.1395446 | | | |
| 94 | 94.15 | 0.15 | 0.25 |

Note ^[1] : The deviated value is the absolute value of the difference between the measured value and the corresponding specified sound pressure level.

2. Frequency*

| Specified Frequency (Hz) | Measured value (Hz) | Deviated value ^[2] (%) | Acceptance Limit (%) |
|---|---------------------|-----------------------------------|----------------------|
| At the sound pressure level of 94 dB | | | |
| 1000 | 1000.0 | 0.0 | 0.7 |

Note ^[2] : The deviated value is the absolute value of the difference in percent between the measured value and the corresponding specified frequency.



3. Total distortion + Noise*

Microphone 4180 Serial No.1395446

| Measured value ^[3] (%) | Maximum total distortion + Noise (%) |
|---|---|
| At the sound pressure level of 94 dB | |
| 0.2 | 2.5 |

Note ^[3]: The measured value is the total distortion, measured over the frequency range from 20 Hz to 20 kHz. The measured value must not exceed the maximum total distortion + noise appeared in the table.

End of Certificate of Calibration



Certificate of Calibration

Certificate Number : SPR22020311-7

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222072

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 18 Feb 2022

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 21 Feb 2022

Location of Calibration : In-Lab

Recommend Due Date : 21 Feb 2023

Calibration Procedure : SP-CPE-04-01

Date of Issue : 22 Feb 2022

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Approved by :

Calibration Officer

(Mr.Worapong Sinthusopa)

Authorized Signatory



Calibration Report

Certificate Number : SPR22020311-7

Page : 2 of 3

Reference Standards

| Equipment Name | Model | Serial No. | Certificate No. | Due. Date |
|------------------------|--------|------------|-----------------|-------------|
| Sound Level Calibrator | SC-942 | B014059 | EEL.BP. 34/1264 | 22 Dec 2022 |

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR22020311-7

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

| Standard Setting | UUC Reading | | Error | | Uncertainty (±) |
|------------------|-------------|-------|-------|------|-------------------|
| | Fast | Slow | Fast | Slow | |
| 94 | 94.0 | 94.0 | 0.0 | 0.0 | 0.15 |
| 114 | 114.0 | 114.0 | 0.0 | 0.0 | 0.15 |

Select C

Unit : dB

| Standard Setting | UUC Reading | | Error | | Uncertainty (±) |
|------------------|-------------|-------|-------|------|-------------------|
| | Fast | Slow | Fast | Slow | |
| 94 | 94.0 | 94.0 | 0.0 | 0.0 | 0.15 |
| 114 | 114.0 | 114.0 | 0.0 | 0.0 | 0.15 |

Select Z

Unit : dB

| Standard Setting | UUC Reading | | Error | | Uncertainty (±) |
|------------------|-------------|-------|-------|------|-------------------|
| | Fast | Slow | Fast | Slow | |
| 94 | 94.0 | 94.0 | 0.0 | 0.0 | 0.15 |
| 114 | 114.0 | 114.0 | 0.0 | 0.0 | 0.15 |

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR22020311-8

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222073

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 18 Feb 2022

Calibration Date : 21 Feb 2022

Recommend Due Date : 21 Feb 2023

Date of Issue : 22 Feb 2022

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by :

(Mr.Worapong Sinthusopa)

Authorized Signatory



Calibration Report

Certificate Number : SPR22020311-8

Page : 2 of 3

Reference Standards

| Equipment Name | Model | Serial No. | Certificate No. | Due. Date |
|------------------------|--------|------------|-----------------|-------------|
| Sound Level Calibrator | SC-942 | B014059 | EEL.BP. 34/1264 | 22 Dec 2022 |

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR22020311-8

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

| Standard Setting | UUC Reading | | Error | | Uncertainty (±) |
|------------------|-------------|-------|-------|------|-------------------|
| | Fast | Slow | Fast | Slow | |
| 94 | 94.0 | 94.0 | 0.0 | 0.0 | 0.15 |
| 114 | 113.9 | 113.9 | -0.1 | -0.1 | 0.15 |

Select C

Unit : dB

| Standard Setting | UUC Reading | | Error | | Uncertainty (±) |
|------------------|-------------|-------|-------|------|-------------------|
| | Fast | Slow | Fast | Slow | |
| 94 | 94.0 | 94.0 | 0.0 | 0.0 | 0.15 |
| 114 | 114.0 | 114.0 | 0.0 | 0.0 | 0.15 |

Select Z

Unit : dB

| Standard Setting | UUC Reading | | Error | | Uncertainty (±) |
|------------------|-------------|-------|-------|------|-------------------|
| | Fast | Slow | Fast | Slow | |
| 94 | 94.0 | 94.0 | 0.0 | 0.0 | 0.15 |
| 114 | 114.0 | 114.0 | 0.0 | 0.0 | 0.15 |

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

Certificate of Calibration

Certificate No. : 65-420102-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : pH Meter with electrode

pH meter

Manufacturer : Horiba

Model : LAQUA-PH210

Range : -2.00 to 16.00 pH

Resolution : 0.01 pH

Serial No. : HA0E0012

ID No. : MET-PH07/64

Electrode

Model : 9652

Serial No. : 992G0181

Environment : Ambient Temperature : $(25 \pm 2) ^\circ \text{C}$

Relative Humidity : $(50 \pm 15) \%$

Date of Received : 26 November 2022

Date of Calibration : 30 November 2022

Date of Issue : 30 November 2022

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

| ID No. | Cert. No. | Due Date | Traceability |
|--------|-----------|-------------|---|
| 440001 | 21E997 | 17 Mar 2023 | National Institute of Metrology Thailand (NIMT) |

2. Standard Buffer Solution

| pH | Cert. No. | Lot No. | Exp. Date | Traceability |
|--------|-----------|---------|-------------|---|
| 4.008 | 61235182 | 833447 | 19 Aug 2024 | CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025 |
| 6.985 | 61255708 | 833449 | 19 Aug 2023 | CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025 |
| 10.008 | 61244986 | 833448 | 19 Aug 2023 | CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025 |

Approved by :

(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-420102-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

| Adjustment Curve at nominal pH | Applied Voltage (mV) | Nominal Value (pH) | UUC Reading | | Correction (mV) | Uncertainty (± mV) |
|-----------------------------------|---------------------------|-------------------------|-------------|--------|----------------------|-------------------------|
| | | | (pH) | (mV) | | |
| 4, 7, 10 | 177.4800 | 4 | 4.00 | 177.4 | 0.1 | 0.060 |
| | 0.0000 | 7 | 7.00 | -0.1 | 0.1 | 0.060 |
| | -177.4800 | 10 | 10.00 | -177.5 | 0.0 | 0.060 |

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

| Adjustment Curve at nominal pH | Standard Buffer (pH) | UUC Reading (pH) | Correction (pH) | Uncertainty (± pH) |
|-----------------------------------|---------------------------|-----------------------|----------------------|-------------------------|
| 4, 7, 10 | 4.008 | 4.01 | 0.00 | 0.0097 |
| | 6.985 | 7.00 | -0.01 | 0.011 |
| | 10.008 | 10.01 | 0.00 | 0.014 |

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 64-400425-5

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Incubator)

Manufacturer : M-LAB

Model : BIC-140

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 240412

ID No. : MET-BI01/55

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (27.0 to 28.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by : Permpoon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400032

65-400274-1

25 Nov 2022

National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 64-400425-5


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

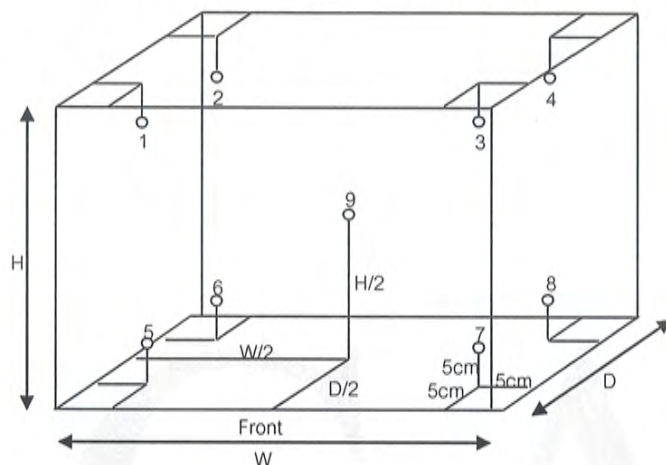

Inside of Chamber

W = 0.37 m

D = 0.33 m

H = 1.14 m

Capacity = 0.14 m³

| Test Point (°C) | Setting Temperature (°C) | Indicating Temperature (°C) | Measured Temperature (°C) @ Sensor No. | | | | | | | | | Uncertainty (± °C) |
|--------------------|-----------------------------|--------------------------------|--|------|------|------|------|------|------|------|------|-----------------------|
| | | | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | |
| 20.0 | 20.0 | 20.0 | 19.8 | 19.7 | 19.6 | 19.6 | 20.4 | 20.2 | 20.3 | 19.8 | 19.9 | 0.54 |

| Test Point (°C) | Setting Temperature (°C) | Indicating Temperature (°C) | Measured Uniformity (°C) | Measured Stability (°C) | Overall Variation (°C) |
|--------------------|-----------------------------|--------------------------------|-----------------------------|----------------------------|---------------------------|
| 20.0 | 20.0 | 20.0 | 0.6 | 0.1 | 1.0 |

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

B



Certificate of Calibration

Certificate No. : 65-400424-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)

Manufacturer : Memmert

Model : UM 100

Range : N/A °C

Resolution : 0.1 °C

Serial No. : b197.0985

ID No. : MET-OV01/46

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (27.0 to 28.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400032

65-400274-1

25 Nov 2022

National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-400424-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

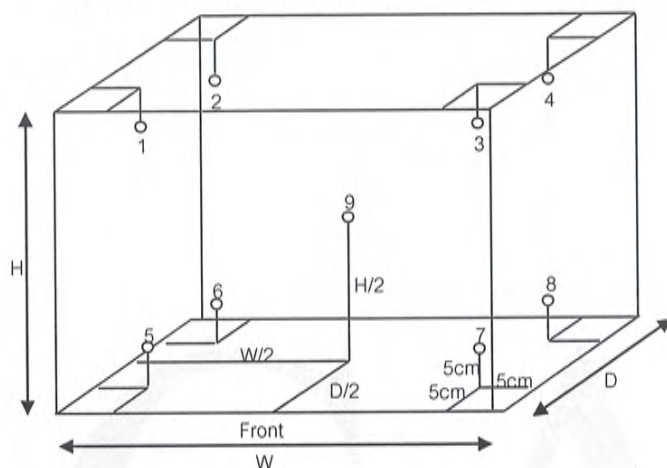

Inside of Chamber

W = 0.32 m

D = 0.18 m

H = 0.24 m

Capacity = 0.01 m³

| Test Point (°C) | Setting Temperature (°C) | Indicating Temperature (°C) | Measured Temperature (°C) @ Sensor No. | | | | | | | | | Uncertainty (± °C) |
|--------------------|-----------------------------|--------------------------------|--|-------|-------|-------|-------|-------|-------|-------|-------|-----------------------|
| | | | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | |
| 180.0 | 180.0 | 180.0 | 181.2 | 181.3 | 180.6 | 180.4 | 179.9 | 181.0 | 179.5 | 179.1 | 180.0 | 0.95 |

| Test Point (°C) | Setting Temperature (°C) | Indicating Temperature (°C) | Measured Uniformity (°C) | Measured Stability (°C) | Overall Variation (°C) |
|--------------------|-----------------------------|--------------------------------|-----------------------------|----------------------------|---------------------------|
| 180.0 | 180.0 | 180.0 | 1.4 | 0.3 | 2.5 |

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

[Handwritten signature]



Certificate of Calibration

Certificate No. : 65-400424-2

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)
Manufacturer : Binder Model : ED53
Range : N/A °C Resolution : 1 °C
Serial No. : 13-07419 ID No. : MET-OV02/57

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (27.0 to 28.0) °C
Relative Humidity : (50 to 55) %
Line Voltage : (210.0 to 210.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by : Permpon Chanpu


Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

| ID No. | Cert. No. | Due Date | Traceability |
|-----------------|-------------|-------------|---|
| 400029 & 400030 | 65-400272-1 | 24 Nov 2022 | National Institute of Metrology Thailand (NIMT) |

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-400424-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

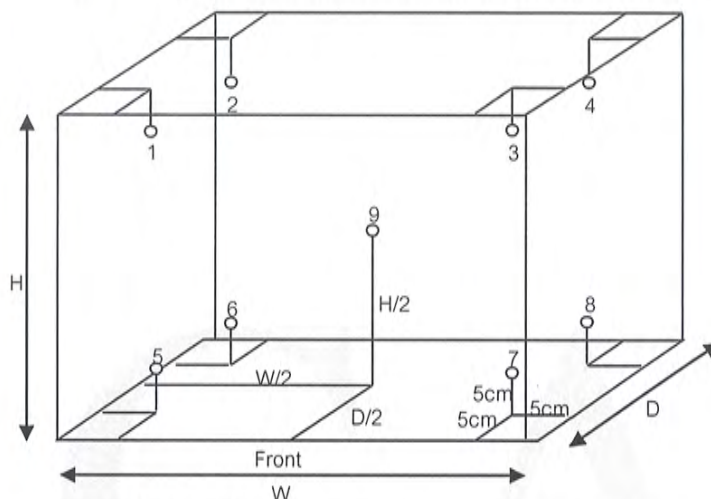

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.40 m

Capacity = 0.05 m³

| Test Point (°C) | Setting Temperature (°C) | Indicating Temperature (°C) | Measured Temperature (°C) @ Sensor No. | | | | | | | | | Uncertainty (± °C) |
|-----------------|--------------------------|-----------------------------|--|-------|-------|-------|-------|-------|-------|-------|-------|--------------------|
| | | | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | |
| 104 | 110 | 110 | 105.0 | 105.0 | 104.7 | 105.0 | 104.4 | 104.5 | 104.0 | 103.7 | 104.2 | 0.95 |
| 180 | 184 | 184 | 180.8 | 182.0 | 179.4 | 180.8 | 180.8 | 180.8 | 180.3 | 180.0 | 180.0 | 1.2 |

| Test Point (°C) | Setting Temperature (°C) | Indicating Temperature (°C) | Measured Uniformity (°C) | Measured Stability (°C) | Overall Variation (°C) |
|-----------------|--------------------------|-----------------------------|--------------------------|-------------------------|------------------------|
| 104 | 110 | 110 | 1.0 | 0.2 | 1.7 |
| 180 | 184 | 184 | 2.3 | 0.3 | 3.0 |

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 65-200253-1

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Electronic Balance
Manufacturer : Sartorius Model : BSA224S-CW
Serial No. : 35090472 ID No. : MET-EB 02/60
Capacity : 220 g Resolution : 0.0001 g

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (25.6 to 25.8) °C
Relative Humidity : (57.3 to 57.8) %
Air Pressure : 1005.0 mbar

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 11 August 2022

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 5, July 2015

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

| ID No. | Cert. No. | Due Date | Traceability |
|------------|-----------|-------------|--|
| E261-E2624 | C02213103 | 18 Nov 2022 | National Institute of Metrology (Thailand), (NIMT) |

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-200253-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


| Nominal Value (g) | Correction (g) | Uncertainty \pm (g) |
|----------------------|-------------------|--------------------------|
| 0.05 | 0.0000 | 0.00011 |
| 0.1 | 0.0000 | 0.00013 |
| 0.5 | 0.0000 | 0.00013 |
| 1 | 0.0000 | 0.00011 |
| 5 | 0.0000 | 0.00011 |
| 10 | 0.0001 | 0.00011 |
| 50 | 0.0001 | 0.00013 |
| 100 | 0.0000 | 0.00020 |
| 150 | 0.0000 | 0.00038 |
| 200 | 0.0000 | 0.00038 |

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.11$, providing a level of confidence of approximately 95%

Eccentric error Load test : 50 g

| | | | | | |
|--------|--------|--------|--------|--------|---|
| A | B | C | D | E | |
| 0.0001 | 0.0001 | 0.0001 | 0.0000 | 0.0000 | g |



Repeatability Load test : 200 g

Stdev. : 0.00005 g

- o0o -

Handwritten signature



Certificate of Calibration

Certificate No. : 65-400424-7

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Refrigerator)

Manufacturer : Sanden Intercool

Model : SRR3-0687 AR

Range : N/A °C

Resolution : 1 °C

Serial No. : SRR3675A-210400065 R

ID No. : MET-RE04/64

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (29.8 to 31.5) °C

Relative Humidity : (55 to 58) %

Line Voltage : (220.8 to 222.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by : Bunjerd Masri

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400046 & 400028

65-400157-3

04 Oct 2022

National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. :65-400424-7


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

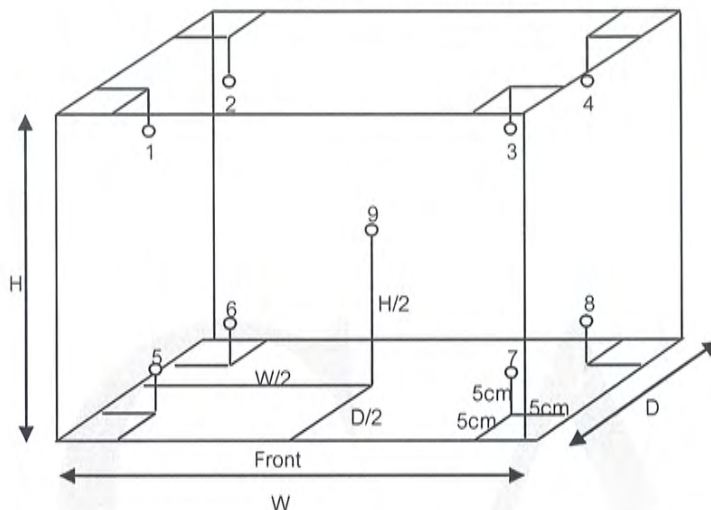

Inside of Chamber

W = 0.58 m

D = 0.60 m

H = 1.45 m

Capacity = 0.50 m³

| Test Point (°C) | Setting Temperature (°C) | Indicating Temperature (°C) | Measured Temperature (°C) @ Sensor No. | | | | | | | | | Uncertainty (± °C) |
|--------------------|-----------------------------|--------------------------------|--|-----|-----|-----|-----|-----|-----|-----|-----|-----------------------|
| | | | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | |
| 3 | 3 | 3 | 3.7 | 3.7 | 3.6 | 3.0 | 2.6 | 3.2 | 2.6 | 2.5 | 3.0 | 0.85 |

| Test Point (°C) | Setting Temperature (°C) | Indicating Temperature (°C) | Measured Uniformity (°C) | Measured Stability (°C) | Overall Variation (°C) |
|--------------------|-----------------------------|--------------------------------|-----------------------------|----------------------------|---------------------------|
| 3 | 3 | 3 | 0.8 | 0.3 | 1.5 |

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

B

