

ภาคผนวก ฉ

ใบรับรองการสอบเทียบเครื่องมือ



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Songkhla Lab	BOD	Incubator	SGK_CL0028	25-Jan-22	26-Jul-23	18
Songkhla Lab	BOD	DO/BOD Analyser	SGK_CL0073	21-Nov-22	21-May-24	18
Songkhla Lab	COD	COD Reactor	SGK_CL0085	23-Jan-23	23-Jan-24	12
Songkhla Lab	COD	Spectrophotometer	SGK_CL0038	24-Jan-23	24-Jan-24	12
Songkhla Lab	pH at 25 °C	pH meter	SGK_CL0030	28-Apr-23	28-Oct-24	18
Songkhla Lab	Oil & Grease	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Oil & Grease	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Oil & Grease	Water Bath	SGK_CL0035	5-Feb-22	6-Aug-23	18
Songkhla Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Total Dissolved Solids 180°C	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Total Suspended Solids	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Total Suspended Solids	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Water Lab	BOD	DO Meter	BKK_EN0017	24-May-22	24-Nov-23	18
Water Lab	BOD	Incubator	BKK_EN0305	5-Apr-23	5-Apr-24	18
Water Lab	COD	Hot Block	BKK_EN0222	25-Apr-23	25-Apr-24	12
Water Lab	COD	Spectrophotometer	BKK_EN0018	16-Sep-22	16-Sep-23	12
Water Lab	pH at 25 °C	pH meter	BKK_EN0072	12-Sep-22	12-Mar-24	18
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0148	31-Jan-22	1-Aug-23	18
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Ambient	Benzene	GC-MSD	RYG_EN0136	7-Jul-22	7-Jan-24	18
Ambient	Total Hydrocarbon	DRYCAL FLOWMETER	BKK_FS1346	24-Jan-23	24-Jan-24	12
Ambient	Total Hydrocarbon	Total Hydrocarbon Analyzer	BKK_EN0057	9-Aug-22	9-Feb-24	18



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM75

Page.: 1 of 3

Certificate of Calibration

Equipment : Incubator
Manufacturer : Memmert
Model : ICP 750
Serial No. : F816.0063
ID No. : SGK_CL0028
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Songkhla Branch.
114/1 Moo 8, Kanjanavanij Rd., Banphru,
Hatyai, Songkhla 90250, Thailand
Location : BOD Room
Received Order : 24 January 2022
Calibration Date : 25 January 2022
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Kunchit Promprat

REVIEW BY	Ananta B.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	26/7/23

Approved by :


Approved Signatory

- () Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date :

7 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0037405



Equipment : Incubator
 Condition As-Received : Used Item
 Reference : 2201-0617OC-3
 Procedure Used :-

Cert. No.: 22TM75

Page.: 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY57013823	21LM3/1	26 Feb 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

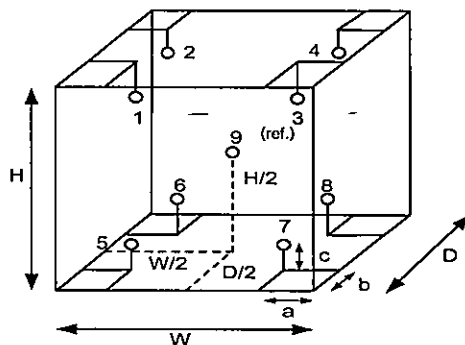

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	28
REL.Humid. (%)	57	52
AC Supply (Volt)	231	231

Probe Installation Details :

a = 10 cm
 b = 10 cm
 c = 10 cm

Dimension of Chamber :

D = 0.60 m
 W = 1.0 m
 H = 1.2 m
 Capacity = 0.75 m³

Position :	Ref. Std. ID No.:
1	21-17RTD-01
2	21-17RTD-02
3	17RTD-03
4	17RTD-04
5	17RTD-05
6	17RTD-06
7	17RTD-07
8	17RTD-08
9 (ref.)	17RTD-09

Malu.



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2201-0617OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 22TM75

Page.: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
20.0	20.0	20.1	0.094	0.50	0.83	0.30	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
20.0	20.280	20.370	20.363	20.378	19.915	19.925	19.673	19.727	20.098

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Mulu .



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22LM162

Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000

Serial No. : 17B101473

ID No. : SGK_CL0073

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Songkhla Branch.
114/1 Moo 8, Kanjanavanij Rd., Banphru,

Location : TPA Chemistry Calibration Lab.2

Received Order : 18 November 2022

Calibrated Date : 21 November 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lerngagtrakul

REVIEW BY	Ananta B.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	21 Nov 24.

Approved by :

Malu.

Approved Signatory

- () Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date :

22 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0047729



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2111-0663DSC-2

Cert. No.: 22LM162

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1523	3240076	221249	02 Mar 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 17B100103

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.001	19.88	-0.121	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Maku-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 22TW259

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000
Serial No. :	17B101473
ID No. :	SGK_CL0073
Received Date :	18 November 2022
Test Date :	21 November 2022
Reference :	2211-0663DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8, Kanjanavanij Rd., Banphru, Hatyai, Songkhla 90250, Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	 Approved Signatory
<input checked="" type="checkbox"/> Malee Butkruea <input type="checkbox"/> Saithip Meangmai <input type="checkbox"/> Warakorn Lerngagtrakul	
Issue Date :	22 November 2022



Cert.No.: 22TW259

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 17B100103

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.12	8.12	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Malu.

a 1136621



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484

Cert. No.: 23TM74/1

Page.: 1 of 3

Certificate of Calibration

This Certificate was issued to replace to the Certificate No.23TM74

Equipment : COD Reactor

Manufacturer : Hach

Model : DRB 200

Serial No. : 21120C1313

ID No. : SGK_CL0085

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch
114/1 Moo 8, Kanjanavanij Rd.,
Banphru, Hatyai,
Songkhla 90250 , Thailand

Location : Chemistry Room

Received Order : 23 January 2023

Calibration Date : 23 - 24 January 2023

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Kunchit Promprat

Approved by :

Malu

Approved Signatory

() Pornthippa Tameyakul

(✓) Malee Butkruea

() Suwit Imjai

Issue Date : 2 March 2023

The Uncertainties are for a confidence probability of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration and Testing Equipment Services.

A 0010625



Equipment : COD Reactor
Condition As-Received : Used Item
Reference : 2301-0661OC-4

Cert. No.: 23TM74/1
Page.: 2 of 3

Procedure Used :-

As agreed with customer the calibration was performed using in-house calibration method according to directed measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY44073381	22LM78/1	12 May 2023

- This certification is traceable to the SI unit.
- This result of calibration was found accurate as shown on date and place of calibration only.
- This certification is traceable to the International System of Unit.

Function of UUC* : Temperature Source

Heat transfer medium used : Alumina Calcined

Environment during calibration		
	Beginning	Finished
Temp.(°C)	28	28
REL.Humi.(%)	58	55
AC Supply (Volt)	225	225

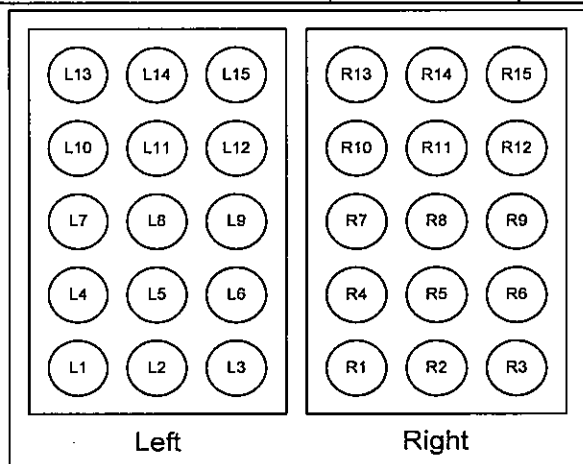

Top View

Left		Right	
Position	ID No. of Sensor	Position	ID No. of Sensor
L1	20-01TC-01	R1	20-01TC-01
L2	20-01TC-02	R2	20-01TC-02
L3	20-01TC-03	R3	20-01TC-03
L4	20-01TC-04	R4	20-01TC-04
L5	20-01TC-05	R5	20-01TC-05
L6	20-01TC-06	R6	20-01TC-06
L7	20-01TC-07	R7	20-01TC-07
L8	20-01TC-08	R8	20-01TC-08
L9	20-01TC-09	R9	20-01TC-09
L10	20-01TC-10	R10	20-01TC-10
L11	20-01TC-01	R11	20-01TC-01
L12	20-01TC-02	R12	20-01TC-02
L13	20-01TC-03	R13	20-01TC-03
L14	20-01TC-04	R14	20-01TC-04
L15	20-01TC-05	R15	20-01TC-05

Malu.



Equipment : COD Reactor
Condition As-Received : Used Item
Reference : 2301-0661OC-4
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM74/1

Page.: 3 of 3

Calibration Point 150 °C

UUC* Setting (°C)	UUC* Reading (°C)	Measured Temperature (°C)						Temperature stability (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
		Position								
		Left			Right					
150	150	L13	L14	L15	R13	R14	R15	Left 0.12	0.59	2
		148.290	148.623	148.360	149.812	150.003	149.566			
		L10	L11	L12	R10	R11	R12			
		148.929	148.812	149.120	150.357	149.814	149.593			
152	152	L7	L8	L9	R7	R8	R9	Right 0.10		
		149.534	149.895	150.362	151.629	151.699	151.581			
		L4	L5	L6	R4	R5	R6			
		149.999	149.972	149.971	151.721	151.690	151.682			
		L1	L2	L3	R1	R2	R3			
		149.639	149.855	149.415	151.444	151.419	150.728			

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.

a 1149779



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CHO30

Page.: 1 of 3

Certificate of Calibration

Equipment : Spectrophotometer
Manufacturer : HACH
Model : DR 3900
Serial No. : 1687645
ID No. : SGK_CL0038
Condition As-Received: Used Item
Received Date : 23 January 2023
Calibration Date : 24 January 2023
Reference : 2301-0661OC-1
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch.
114/1 Moo 8 , Kanjanavanij Rd.,
Banphru , Hatyai ,
Songkhla 90250 , Thailand

REVIEW BY	Ananta B.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	24/01/24

Calibration Place : Chemistry Room
Ambient Temperature : (28.3 - 27.3) °C (On-Site)
Relative Humidity : (49.6 - 49.9) % (On-Site)
Calibration Procedure : In - house method :
CP-OCH4 based on ASTM E 275-01

Calibrated by : Kunchit Promprat

Approved by :

Malee

Approved Signatory

- (☒) Malee Butkruea
() Saithip Meangmai
() Warakorn Lernagtrakul

Issue Date : 7 February 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0050506



Cert. No. : 23CHO30

Page : 2 of 3

Condition of calibration result

1. Reference Standard Material :

<u>Material</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1. Absorbance Standard set	32593	100581	30 Mar 2024
2. Wavelength Standard set	29829	94776	02 Sep 2023
3. Wavelength Standard set	29829	94777	02 Sep 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit maintained at :

- National Physical Laboratory (NPL), The United Kingdom of Great Britain and Northern Ireland
- National Institute of Standards and Technology (NIST), The United States of America

4. Spectral BandWidth : 5 nm

Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (\pm nm)	Coverage Factor <i>k</i>
418.40	418	0.59	2.00
479.88	480	0.59	2.00
513.75	514	0.59	2.00
537.00	536	0.59	2.00
638.00	638	0.59	2.00
684.70	685	0.59	2.00
747.61	748	0.59	2.00
807.04	807	0.59	2.00

Malu

a 1146846



Cert. No. : 23CHO30

Page : 3 of 3

Calibration Results : without adjustment**Photometric Accuracy**

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (\pm Abs)	Coverage Factor k
420.0	Zero	0.000	0.0028	2.00
	0.5701	0.568	0.0029	2.00
	0.7147	0.712	0.0030	2.00
	1.0031	0.999	0.0030	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5552	0.553	0.0029	2.00
	0.7031	0.700	0.0030	2.00
	0.9867	0.981	0.0029	2.00
465.0	Zero	0.000	0.0028	2.00
	0.5178	0.517	0.0030	2.00
	0.6642	0.663	0.0029	2.00
	0.9312	0.930	0.0030	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5195	0.517	0.0030	2.00
	0.7007	0.698	0.0029	2.00
	0.9833	0.979	0.0028	2.00
590.0	Zero	0.000	0.0028	2.00
	0.5537	0.550	0.0030	2.00
	0.7763	0.771	0.0029	2.00
	1.0912	1.083	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5615	0.558	0.0029	2.00
	0.7659	0.762	0.0030	2.00
	1.0763	1.070	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Malu.

a 1146845



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 1-May-2023

Certificate No. : 23CH0203

CSR No. : A088/04367

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : pH meter

Manufacturer : Mettler Toledo

Model : S220

Serial No. : B625631849

ID No. : SGK_CL0030

Electrode No. : 1204613

Received Date : 28-Apr-2023

Calibrated Date : 28-Apr-2023

Ambient Temperature : $(25 \pm 3) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \%$

REVIEW BY	Ananta B.
APPROVED BY	Kamrta H.
NEXT CAL. DATE	28 / 10 / 2024

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HACH : HACH LANGE GmbH

- SCaL : Sounthern Calibration Service Co., Ltd.,

- WK : WK Electric Co., Ltd.

Calibrated by : Alisara Ma

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.



Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.005	C02994	1777	5-Sep-2024
Standard Solution	7.000	C03007	1787	17-Oct-2024
Standard Solution	10.012	C02953	1735	29-Apr-2024
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	5-Jun-2024
Digital Thermometer With Sensor	DP-77	I.360896	22SDTH005	8-Aug-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading		Correction (mV)	Uncertainty (± mV)
	(mV)	(pH)		
177.48	177.5	3.70	-0.02	0.17
0.00	0.0	6.70	0.00	0.13
-177.48	-177.4	9.80	-0.08	0.17

2. Before Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.005	3.97	159.2	0.035	0.0090
6.999	6.98	-15.4	0.019	0.013
10.012	9.95	-188.0	0.062	0.036

3. After Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.005	3.97	158.9	0.035	0.0090
6.999	7.01	-17.5	-0.011	0.013
10.012	9.98	-187.6	0.032	0.036

4. Temperature Measurement

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25	25.032	25.1	-0.068	0.11

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com

**SARTORIUS**

Certificate

of Calibration

REVIEW BY Ananta B.
APPROVED BY Kanitta H.
NEXT CAL. DATE 25/1/23-24

Model Number : MSE224S-100-DUCertificate No. : 23BCI0044Description : Analytical BalanceIssued Date : Friday, January 27, 2023Serial Number : 0034705158Reference No. : 202361ID No. : SGK_CL0045Manufacturer : SartoriusPage No. : 1 of 2Customer Name : ALS Laboratory Group (Thailand) Co., Ltd.Songkhla Branch: 114/1 Moo 8 Karnchanawanich Rd., T. Ban Phru, A. Hat Yai, Songkhla. 90250.Calibrated Place : Balance Room.Calibrated By : Mr. Chonchai InthanaCalibration Date : Wednesday, January 25, 2023

Calibration

Procedure No. : This calibration was conducted byUsing in-house calibration procedure number (WI-003)Based on UKAS LAB 14 : 2019**Metrological data :**Capacity : 220 g Readability : 0.0001 g**Ambients Conditions:**Temperature : 22.4 °C ± 3.0 °CHumidity : 65.0 % RH ± 5.0 % RHPressure : ± **Reasons for calibration**☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ MaintenanceEquipment Condition: ☒ Good Operate ☐ Fair**Measurement Method UKAS Publication Ref :Lab 14**

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 1kg E2 s/n 37929119	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division
Sartorius (Thailand) Co., Ltd.

Mr. Chonchai Inthana (Technical Manager)

S
T
A
M
P

Certificate of Calibration

Model Number : MSE224S-100-DU

Certificate No. : 23BCI0044

Description : Analytical Balance

Issued Date : Friday, January 27, 2023

Serial Number : 0034705158

Reference No. : 202361

ID No. SGK_CL0045

Manufacturer : Sartorius

Page No. : 2 of 2

Calibration Results : Without Adjustment

Repeatability



The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0001	200.0000
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0000
	20.0000	200.0001
Nominal Value : (High Load)	20.0000	200.0000
200 g	20.0000	200.0001
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0001
	20.0000	200.0001
Standard Deviation	0.00003	0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 50 g
Tolerance 0.0004 g



	Difference
1	—
2	0.0001
3	0.0000
4	0.0000
5	0.0000
6	—

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00013
0.1	0.1000	0.1000	0.0000	0.00013
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	200.0001	0.0001	0.00030

End of Report.



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 1-May-2023

Certificate No. : 23TH1728

CSR No. : A088/04367

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : Hot Air Oven

Manufacturer : Memmert

Model : UF110

Serial No. : B416.3387

ID No. : SGK_CL0024

Resolution : 0.1 °C

Received Date : 28-Apr-2023

Calibrated Date : 28-Apr-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY Ananta B.
APPROVED BY Kanitta H. 10
NEXT CAL. DATE 28/11/2024 10

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- ScaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

(☒) Without Adjustment

(☐) After Adjustment

1. Sensor Installation Diagram

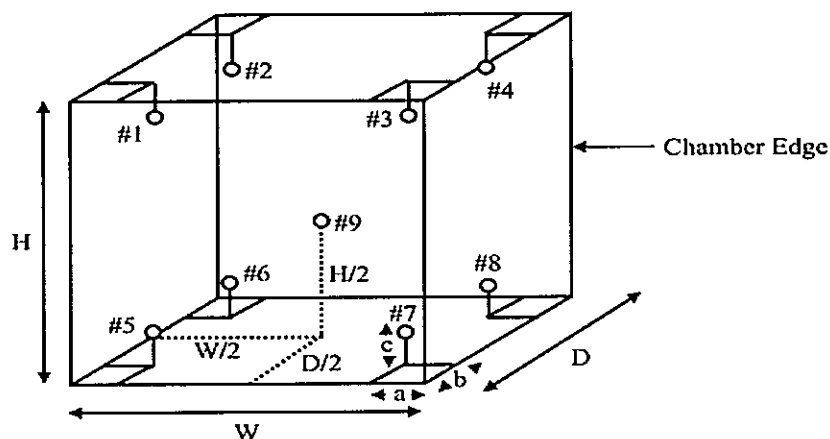

Sensor Installation Details

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of the chamber

W = 40.0 cm
H = 40.0 cm
D = 33.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Hot Air Oven and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
40	40.48	40.28	40.28	39.91	40.17	40.09	39.93	40.27	39.89	0.36
70	70.36	70.23	70.58	69.74	69.99	69.92	69.86	70.13	70.04	0.36
103	103.19	103.12	103.46	103.37	103.10	103.54	103.43	103.06	103.40	0.36
104	104.31	104.23	104.62	103.77	104.12	104.06	103.90	104.20	104.56	0.36
105	105.07	105.03	105.48	105.27	105.12	105.01	105.01	105.00	104.96	0.36
180	180.31	180.00	180.00	180.07	180.18	180.05	180.01	180.10	180.24	0.41

3. Performance Result

The performance of the Hot Air Oven are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
40	40.0	40.0	0.20	0.70	0.72
70	70.0	70.0	0.20	0.60	0.94
103	103.0	103.0	0.20	0.43	0.54
104	104.0	104.0	0.10	0.79	0.88
105	105.0	105.0	0.10	0.59	0.69
180	180.0	180.0	0.10	0.38	0.38

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkhla 90250 Thailand

Tel: 081 599 0417 Fax: 074 805 133 Email: s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 8-Feb-2022

Certificate No. : 22WB004

CSR No. : A0223/01123

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8 Karnchanawanich Rd. T.Ban Phru,
A. Hat Yai, Songkhla 90250 TH

Calibration Place : Chemical Laboratory
Instrument Name : Water Bath
Manufacturer : Memmert
Model : WNE29
Serial No. : L616.0538
ID No. : SGK_CL0035
Resolution : 0.1 °C
Received Date : 5-Feb-2022
Calibrated Date : 5-Feb-2022
Ambient Temperature : (30 ± 10) °C
Relative Humidity : (50 ± 30) %

REVIEW BY	Ananta B.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	6/07/2023

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.W1.014 based on ASTM E 715 : 1980 (reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Imron Rattanaylum

Approved by :

Sakeereen Heemhad / Technical Manager

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data logger With Sensor	34970A	MY44064411	QR21-0314	9-Feb-2022

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

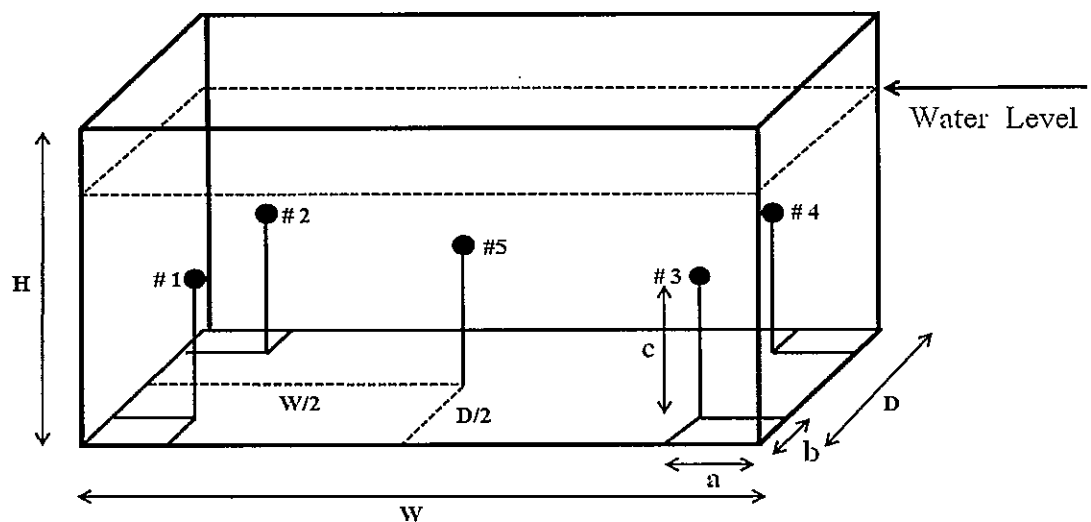

Sensor Installation Details

a = 5 cm
b = 5 cm
c = 5 cm

Dimension of the chamber

W = 45 cm
H = 30 cm
D = 35 cm

Result of Calibration .:

2. Temperature Measurement Accuracy Test

The measurement results of the Water Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (± °C)
	#1	#2	#3	#4	Ref.5	
80	79.95	80.07	79.95	79.99	80.03	0.14

3. Performance Result

The performance of the Water Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
80	81.0	81.0	0.10	0.19	0.19

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 22TW122

Page.: 1 of 2

Certificate of Testing

Equipment : DO Meter
Manufacturer : YSI
Model : 5000-230V
Serial No. : 09J101147
ID No. : BKK_EN0017
Received Date : 20 May 2022
Test Date : 24 May 2022
Reference : 2205-0638DSC-8
Submitted by :

ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Warakorn Lerngagtrakul

Approved by :

Malee

Approved Signatory

- (☒) Malee Butkruea
(☐) Saithip Meangmai
(☐) Warakorn Lerngagtrakul

Issue Date : 31 May 2022

REVIEW BY	<i>Siriluk P.</i>
APPROVED BY	<i>K. An</i>
NEXT CAL. DATE	<i>24/11/23</i>



Cert.No.: 22TW122

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	21MM430	21 Sep 2022

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 16K100498

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.12	8.13	0.015

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Malu

a 1110482



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22LM83

Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000-230V

Serial No. : 09J 101147

ID No. : BKK_EN0017

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 20 May 2022

Calibrated Date : 30 May 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Tawatchai Pama

Approved by :

Malee

Approved Signatory

- () Pornthippa Tameyakul
(☒) Malee Butkruea
() Suwit Imjai

Issue Date : 31 May 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0039957



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2205-0638DSC-10

Cert. No.: 22LM83

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1502A	A09204	2218	04 Jan 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with thermistor sensor , ID No.: 16K100498

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.003	20.01	0.007	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu -



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T230683

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Incubator)

Manufacturer : MEMMERT

Model : ICP 750

Serial No. : F818.0075

Customer Code : BKK_EN0305

ID No. : T9571A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab 2

Date of Receipt : 30 March 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Assistant Calibration Manager)

Date of Issue : 10 APR 2023

REVIEW BY	Sinluk P.
APPROVED BY	KL AL
NEXT CAL. DATE	05/04/24

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T230683

Page 2 of 4

Calibration Report

Equipment : Chamber (Incubator)
Date of Calibration : 5 April 2023 (Finished Time 4:30 PM)
Environment : Temperature 22.9-28.6 °C
Line Voltage 221.7-225.5 V

Condition of this results of test. :

1. This instrument was calibrated by insert 12 standard resistance thermometer into its chamber and test according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986.)

All data show below were final values and the initial data may be obtained upon request.

The temperature scale used was based on ITS - 90.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	37-(CH1-10)	T222493	28 November 2023
RTD	100 ohm	36-(CH1-10)	T222493	28 November 2023
DATA LOGGER	34970A	T193	T222493	28 November 2023

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

UUC Description :

Time Constant 2 Hour 24 Minute At 20 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Result of test :

() without adjustment

(X) after adjustment


Approved By. _____



Certificate No T230683

Calibration Report


Page 3 of 4

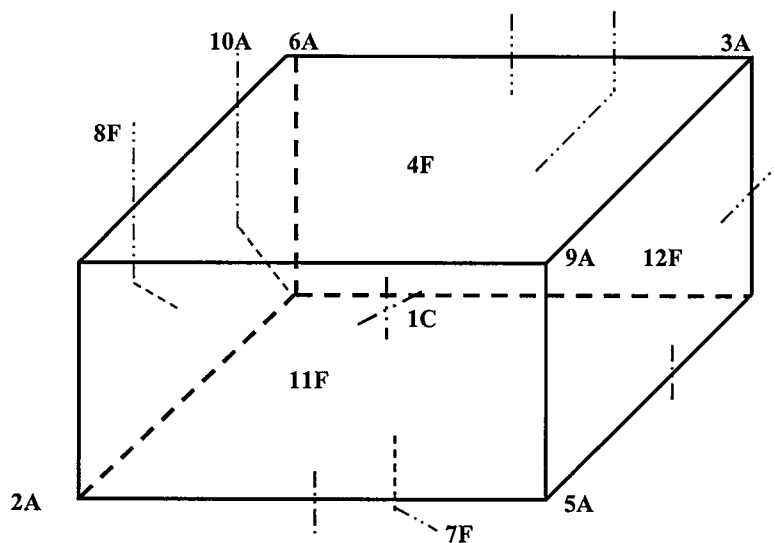

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	37CH1
2A	=	37CH2
3A	=	37CH3
4F	=	37CH4
5A	=	37CH5
6A	=	37CH6
7F	=	37CH7
8F	=	37CH8
9A	=	37CH9
10A	=	37CH10

11F	=	36CH1
12F	=	36CH2

Approved By. 

Certificate No. T230683

Calibration Report

Page 4 of 4

Measurement Results

Average Standard Reading at each position (°C)										
Calibration Point	37CH1	37CH2	37CH3	37CH4	37CH5	37CH6	37CH7	37CH8	37CH9	37CH10
20.0	20.32	20.28	20.17	20.22	20.22	20.04	20.17	19.74	20.31	19.93
	36CH1	36CH2								
	20.14	20.20								
Calibration Point	37CH1	37CH2	37CH3	37CH4	37CH5	37CH6	37CH7	37CH8	37CH9	37CH10
25	25.28	25.15	25.13	25.13	25.20	25.02	25.11	24.79	25.20	25.26
	36CH1	36CH2								
	25.13	24.94								

Chamber (Incubator)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor k
	Min , Max	Average					
20.0	19.9 , 20.1	20.0	20.02	0.09	0.54	0.38	2.00
25.0	24.9 , 25.1	25.0	25.03	0.03	0.51	0.38	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109


Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230760

Page 1 of 5

Certificate of Calibration

Equipment : HOT BLOCK
Manufacturer : Environmental Express
Model : B3000- 240
Serial No. : 2017CODW116
Customer Code : BKK_EN0222
ID No. : T6769A4
Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

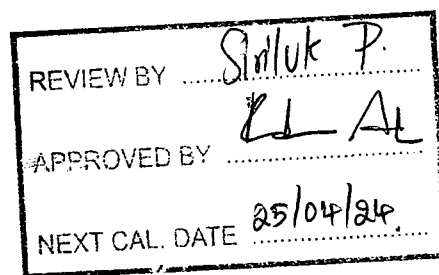

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab2

Date of Receipt : 21 April 2023

Calibrated By : Watcharasak Puttarat (Technician)

Approved By :  / Sujjar Naknakred (Site Calibration Manager)

Date of Issue : 12 MAY 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T230760

Page 2 of 5

Calibration Report

Equipment : HOT BLOCK
Date of Calibration : 25 April 2023
Environment : Temperature : 22.9-24.4 °C
Line Voltage : 222.7-227.8 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 20 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN121-TN130	T222122	5 October 2023
TC	TYPE T	TN131-TN140	T222122	5 October 2023
DATA LOGGER	34970A	T150	T222122	5 October 2023

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 32 Minute At 150 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

(X) without adjustment

() after adjustment

Approved By _____



SCG
CEMENT-BUILDING MATERIALS

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109


Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T230760

Page 3 of 5


Calibration Report

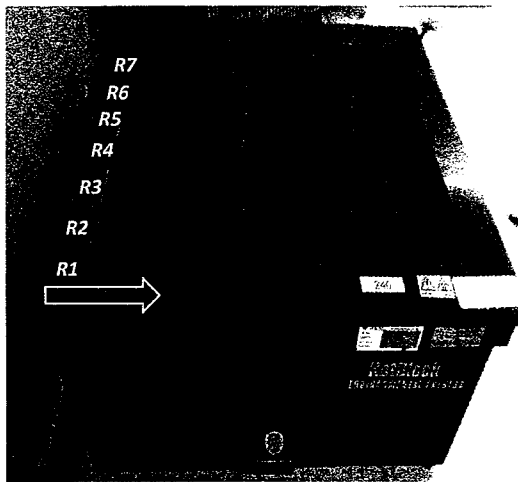

Row	Hole							
R7	H49	H50	H51	H52	H53	H54	H55	H56
R6	H41	H42	H43	H44	H45	H46	H47	H48
R5	H33	H34	H35	H36	H37	H38	H39	H40
R4	H25	H26	H27	H28	H29	H30	H31	H32
R3	H17	H18	H19	H20	H21	H22	H23	H24
R2	H9	H10	H11	H12	H13	H14	H15	H16
R1	H1	H2	H3	H4	H5	H6	H7	H8

H: STANDARD THERMOCOUPLE TYPE T

H1	=	TN121	H9	=	TN129	H17	=	TN137	H25	=	TN125	H33	=	TN133	H41	=	TN121	H49	=	TN129
H2	=	TN122	H10	=	TN130	H18	=	TN138	H26	=	TN126	H34	=	TN134	H42	=	TN122	H50	=	TN130
H3	=	TN123	H11	=	TN131	H19	=	TN139	H27	=	TN127	H35	=	TN135	H43	=	TN123	H51	=	TN131
H4	=	TN124	H12	=	TN132	H20	=	TN140	H28	=	TN128	H36	=	TN136	H44	=	TN124	H52	=	TN132
H5	=	TN125	H13	=	TN133	H21	=	TN121	H29	=	TN129	H37	=	TN137	H45	=	TN125	H53	=	TN133
H6	=	TN126	H14	=	TN134	H22	=	TN122	H30	=	TN130	H38	=	TN138	H46	=	TN126	H54	=	TN134
H7	=	TN127	H15	=	TN135	H23	=	TN123	H31	=	TN131	H39	=	TN139	H47	=	TN127	H55	=	TN135
H8	=	TN128	H16	=	TN136	H24	=	TN124	H32	=	TN132	H40	=	TN140	H48	=	TN128	H56	=	TN136

Approved By. 

Certificate No. T230760

Page 4 of 5

Calibration Report

Measurement Results

			Average Standard Reading at each position (° C)									
Calibration Point			TN121	TN122	TN123	TN124	TN125	TN126	TN127	TN128	TN129	TN130
Point	Setting	Max	149.31	149.49	149.73	148.49	149.26	149.81	149.42	148.86	148.78	149.19
150	150.0	Min	149.14	149.31	149.54	148.36	149.08	149.65	149.22	148.65	149.07	149.07
		Average	149.23	149.40	149.64	148.43	149.16	149.73	149.33	148.76	148.71	149.13
			TN131	TN132	TN133	TN134	TN135	TN136	TN137	TN138	TN139	TN140
		Max	149.90	150.18	150.18	149.16	148.89	149.72	149.28	149.50	150.01	149.32
		Min	149.78	150.06	149.69	149.03	148.76	149.49	149.12	149.37	149.90	149.23
		Average	149.84	150.12	149.76	149.09	148.81	149.62	149.19	149.43	149.95	149.27
			TN121	TN122	TN123	TN124	TN125	TN136	TN127	TN128	TN129	TN130
		Max	149.88	149.14	149.20	150.02	148.75	149.57	149.21	149.18	150.13	148.91
		Min	149.67	148.94	148.98	149.83	148.58	149.43	149.06	149.01	149.91	148.72
		Average	149.78	149.05	149.11	149.94	148.67	149.51	149.13	149.10	150.03	148.83
			TN131	TN132	TN133	TN134	TN135	TN136	TN137	TN138	TN139	TN140
		Max	149.42	149.52	149.13	148.94	148.84	150.16	149.42	149.54	149.66	150.08
		Min	149.27	149.36	148.99	148.81	148.70	149.99	149.27	149.39	149.52	149.97
		Average	149.36	149.45	149.06	148.88	148.76	150.08	149.36	149.48	149.60	150.03
			TN121	TN122	TN123	TN124	TN125	TN126	TN127	TN128	TN129	TN130
		Max	149.21	149.16	149.50	148.68	148.58	149.81	149.06	150.40	148.46	149.24
		Min	149.03	148.93	149.27	148.48	148.42	149.62	148.78	150.26	148.14	149.04
		Average	149.12	149.04	149.39	148.57	148.51	149.72	148.93	150.33	148.29	149.14
			TN131	TN132	TN133	TN134	TN135	TN136				
		Max	148.79	148.23	149.03	149.09	148.46	149.25				
		Min	148.49	147.98	148.88	148.94	148.29	149.12				
		Average	148.61	148.06	148.94	149.02	148.35	149.19				

Approved By.





Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T230760

Page 5 of 5

Calibration Report

Measurement Results

HOT BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (\pm °C)	Uncertainty (\pm °C)
	Min , Max	Average		
150.0	150 , 150.1	150.0	0.20	0.82

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 % .

Approved By. _____

Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No. BSCC-UV-307/22
Equipment UV/Vis Spectrophotometer
Model UV-1800
Manufacturer Shimadzu
Serial No. A11454908533CD
ID No. BKK_EN0018
Date of receipt 16 September 2022
Date of calibration 16 September 2022
Date of issue 23 September 2022

REVIEW BY *Shiruk P.*
APPROVED BY *Kw An*
16/9/23
NEXT CAL. DATE *23/9/22*

Customer name ALS Laboratory Group (Thailand) Co., Ltd.

Address 104 Soi Phatthanakan 40, Phatthanakan Road, Phatthanakan, Suan Luang, Bangkok 10250

Temperature (22.1-23.3) °C (On site)
Humidity (58.8-63.2) %RH (On site)

Equipment condition Good Operation

Calibration Location Organic Prep

Calibration Procedure In-house method WI-UV-702-01 based on ASTM E275-01

Traceability Wavelength Accuracy is traceable to certificate No. 95917 and 95918
Photometric Accuracy is traceable to certificate No. 95924 and 95937
Stray Light is traceable to certificate No. 95908
The above certificate are traceable to SI unit through Starna Scientific Ltd.
(UKAS accredited calibration laboratory NO. 0659)

Calibrated by Mr.Waruth Janphung

Approved by



Mr.Kanchit Choothep
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

Certificate of Calibration

Certificate No.

BSCC-UV-307/22

Number of Page(s)

2 of 3

Calibration Results:

1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (\pm nm)
241.70	241.65	-0.05	0.18
334.02	333.92	-0.10	0.18
418.53	418.46	-0.07	0.18
572.99	572.96	-0.03	0.18
879.41	879.17	-0.24	0.18

2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (\pm A)
235	0.0000	0.0000	0.0000	0.0075
	0.7467	0.7461	-0.0006	0.0075
257	0.0000	0.0000	0.0000	0.0075
	0.8662	0.8647	-0.0015	0.0075
313	0.0000	0.0000	0.0000	0.0075
	0.2904	0.2911	0.0007	0.0075
350	0.0000	0.0000	0.0000	0.0075
	0.6429	0.6426	-0.0003	0.0075

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

Certificate of Calibration

Certificate No. **BSCC-UV-307/22**

Number of Page(s)

3 of 3

Calibration Results:

3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ($\pm A$)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5783	0.5777	-0.0006	0.0042
	0.7628	0.7635	0.0007	0.0046
	1.0206	1.0230	0.0024	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5621	0.5618	-0.0003	0.0042
	0.7455	0.7460	0.0005	0.0048
	0.9985	1.0005	0.0020	0.0042
465.0	0.0000	0.0000	0.0000	0.0042
	0.5227	0.5219	-0.0008	0.0042
	0.6880	0.6884	0.0004	0.0051
	0.9487	0.9503	0.0016	0.0042
546.1	0.0000	0.0000	0.0000	0.0042
	0.5207	0.5199	-0.0008	0.0042
	0.6973	0.6971	-0.0002	0.0049
	0.9959	0.9964	0.0005	0.0042
590.0	0.0000	0.0000	0.0000	0.0042
	0.5544	0.5534	-0.0010	0.0042
	0.7253	0.7242	-0.0011	0.0050
	1.0942	1.0943	0.0001	0.0042
635.0	0.0000	0.0000	0.0000	0.0042
	0.5616	0.5606	-0.0010	0.0042
	0.6927	0.6921	-0.0006	0.0053
	1.0881	1.0885	0.0004	0.0042

*CNR = Customer not request

4. Stray Light*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)		
	Wavelength (nm)	Transmission (%T)	Absorbance (A)
200.96 \pm 0.11nm	200.30	0.9505	2.0229

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

*****End of Certificate*****

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CH1222

Page.: 1 of 2

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	Seven Compact S220
Serial No. :	B520948426
ID No. :	BKK_EN0072
Condition As-Received:	Used Item
Received Date :	09 September 2022
Calibration Date :	12 September 2022
Reference :	2209-0312DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)

REVIEW BY	Sinluk P.
APPROVED BY	KL AL
NEXT CAL. DATE	12/03/24

Calibrated by : Warakorn Lerngagtrakul

Approved by :

Malee

Approved Signatory

- (☒) Malee Butkruea
(☐) Saithip Meangmai
(☐) Warakorn Lerngagtrakul

Issue Date : 15 September 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert. No.: 22CH1222

Page.: 2 of 2

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	22E2769	24 Aug 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	823320	20 June 2024
pH 6.985	CPA chem	794122	14 Feb 2023
pH 10.008	CPA chem	823323	20 June 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results**Function : mV Measurement****Performing standard curve by Fluke at pH (4,7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (\pm mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: B520948426	4.000	177.48	177.4	4.000	0.058	2.00
	7.000	0.00	0.0	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Function : pH Measurement**Performing three buffers standard curve by using buffer nominal pH (4,7,10)**

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (\pm)	Coverage factor <i>k</i>
pH Electrode S/N.: PCE-86-EX1001	4.008	3.999	153.9	0.0055	2.09
	6.985	7.017	-13.7	0.0084	2.00
	10.008	9.996	-179.0	0.0078	2.06

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.

a 1126274

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com



NSC-TISI-TIS 17025

CALIBRATION 0426

SARTORIUS

Certificate

of Calibration

REVIEW BY	<u>Sirilut P.</u>
APPROVED BY	<u>LL AL</u>
NEXT CAL. DATE	<u>8/2/24</u>

Model Number : MSE224S-100-DUDescription : Analytical BalanceSerial Number : 26207042ID No. : BKK_EN0002Manufacturer : SartoriusCertificate No. : 23BCI0072Issued Date : Monday, February 13, 2023Reference No. : 203245Page No. : 1 of 2Customer Name : ALS Laboratory Group (Thailand)Co., Ltd.104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.Calibrated Place : Balance RoomCalibrated By : Mr. Chonchai InthanaCalibration Date : Wednesday, February 08, 2023**Calibration**Procedure No. : This calibration was conducted by
Using in-house calibration procedure number (WI-003)

Based on UKAS LAB 14 : 2019

Metrological data :Capacity : 220 g Readability : 0.0001 g**Ambients Conditions:**Temperature : 23.2 °C ± 5.0 °CHumidity : 60.0 % RH ± 10.0 % RHPressure : ± **Reasons for calibration**☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ MaintenanceEquipment Condition: ☒ Good Operate ☐ Fair**Measurement Method****UKAS Publication Ref :Lab 14**

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2, YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

SOP FM 33 03 February 2022

Mr. Chonchai Inthana (Technical Manager)S
T
A
M
P

Certificate of Calibration

Model Number : MSE224S-100-DU
 Description : Analytical Balance
 Serial Number : 26207042
 ID No. : BKK_EN0002
 Manufacturer : Sartorius

Certificate No. : 23BCI0072

Issued Date : Monday, February 13, 2023

Reference No. : 203245

Page No. : 2 of 2

Calibration Results : Without Adjustment

Repeatability



The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0000	199.9999
Tolerance	20.0000	200.0000
0.0001 g	20.0000	199.9999
	20.0001	200.0000
	20.0000	200.0000
Nominal Value : (High Load)	20.0000	199.9999
200 g	20.0000	199.9999
Tolerance	20.0000	200.0000
0.0001 g	20.0000	199.9999
	20.0001	199.9999
Standard Deviation	0.00004	0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 50 g
 Tolerance 0.0004 g



Difference	
1	—
2	-0.0001
3	0.0000
4	0.0001
5	0.0000
6	—

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00014
0.1	0.1000	0.1000	0.0000	0.00014
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	199.9999	-0.0001	0.00030

End of Report.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th



Certificate No. T220139

Page 1 of 3

Certificate of Calibration

Equipment : Liquid Bath (Water)

Manufacturer : MEMMERT

Model : WNB29

Serial No. : L611.0135

Customer Code : BKK_EN0148

ID No. : T6455A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250


Customer Location : ORGANIC PREPARATION LAB

Date of Receipt : 26 January 2022

Calibrated By : Watcharapon Sangtong (Technician)

Approved By :  / Sujjar Naknakred (Site Calibration Manager)

Date of Issue : 08 FEB 2022

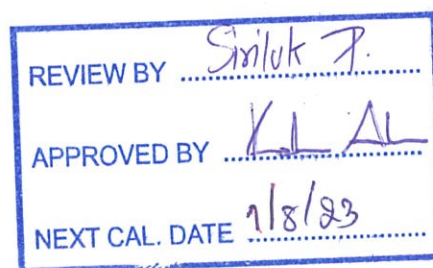

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T220139

Page 2 of 3

Calibration Report

Equipment : Liquid Bath (Water)
Date of Calibration : 31 January 2022
Environment : Temperature : 22.4-23.9 °C
Line Voltage : 221.4-225.4 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 (based on ASTM E715-80 (Reapproved 2001)).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M34 (CH1-CH5)	T210115	2 February 2022
DATA LOGGER	34970A	T47	T210115	2 February 2022

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour - Minute At 60 °C

5. Adjustment :

(X) without adjustment


() after adjustment

Approved By. 

Certificate No. T220139

Page 3 of 3

Calibration Report

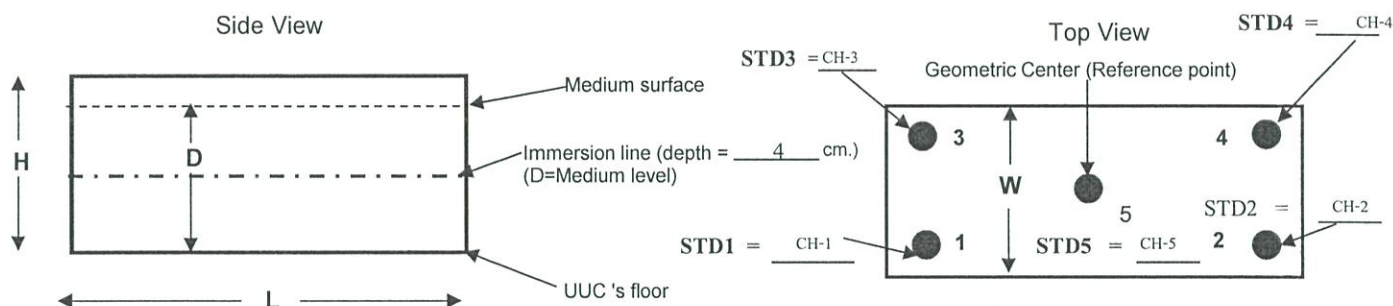

- D = Medium level : 8 cm.
 - UUC's medium : Water
 - Working standards are located at 2.5 cm. away from each corner and walls.
- Working space dimension : 62 × 41 × 14 (W×L×H)

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)				
	CH-1	CH-2	CH-3	CH-4	CH-5
60	59.95	60.04	60.12	60.01	59.89
85	85.17	84.89	85.34	84.78	84.93
95	93.46	93.14	93.81	93.05	93.28

Liquid Bath (Water)			Temperature Distribution			
Setting (°C)	Reading (°C)		Stability (± °C)	Uniformity (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
	Min , Max	Average				
61.0	60.9 , 61	61.0	0.10	0.19	0.25	2.00
86.0	85.9 , 86.1	86.0	0.12	0.39	0.32	2.06
95.0	94.8 , 95.1	94.9	0.14	0.51	0.38	2.11

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T222502

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Oven)

Manufacturer : Memmert

Model : UF 450

Serial No. : B7170531

Customer Code : BKK_EN0273

ID No. : T8042A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Oven Room

Date of Receipt : 23 November 2022

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  /Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 09 DEC 2022

REVIEW BY	Sinluk P.
APPROVED BY	KL AL
NEXT CAL. DATE	29/05/24

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T222502

Page 2 of 4

Calibration Report

Equipment : Chamber (Oven)
Date of Calibration : 29 November 2022
Environment : Temperature : 29.1-29.6 °C
Line Voltage : 221.3-223.2 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors and nine standard thermocouples type T into its chamber , the other one resistance thermometer detector use for ambient temperature measurement .
The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	27-(CH1-10)	T210004	30 December 2022
TC	TYPE T	TN261-TN270	T210010	30 December 2022
DATA LOGGER	34970A	T149	T210004	30 December 2022

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 49 Minute At 104 °C
Fresh Air Damper ☒ Open ☐ Min ☐ Medium ☒ Max
☐ Close
☐ Not Available

5. Adjustment :

() without adjustment


(X) after adjustment

Approved By. Bm Lani

Certificate No. T222502

Page 3 of 4

Calibration Report

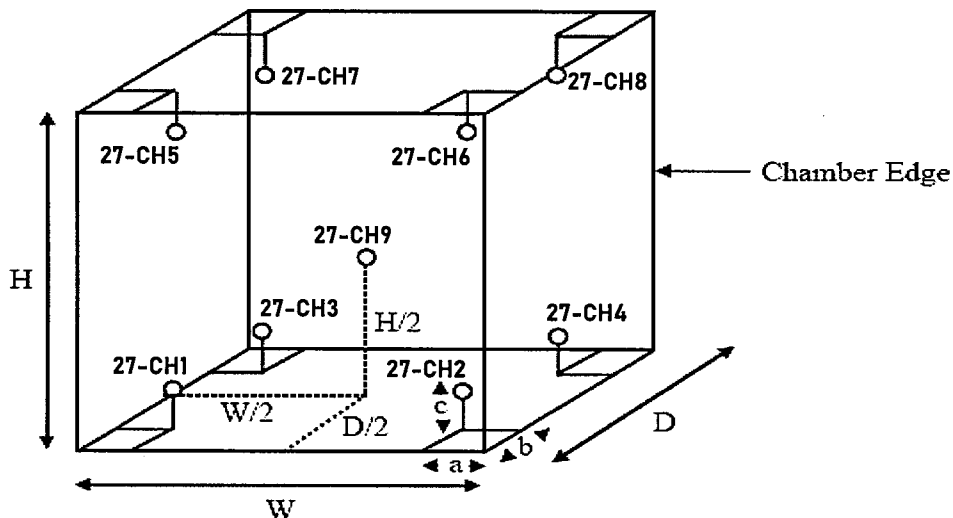

Remark :

Internal Dimensions of Chamber : W (Width) = 104 cm. , H (Height) = 72 cm. and D (Depth) = 60 cm.

Size of Installed Standard sensor number 27-CH1 to number 27-CH8 : a = 5 cm. , b = 5 cm. and c = 5 cm.

Size of Installed Standard sensor number 27-CH9 : W/2 = 104 cm./2 , H/2 = 72 cm./2 and D/2 = 60cm./2

Measurement Results

Average Standard Reading at each position (°C)									
Calibration Point	27-CH1	27-CH2	27-CH3	27-CH4	27-CH5	27-CH6	27-CH7	27-CH8	27-CH9
104	104.07	103.60	103.45	104.02	104.47	103.57	104.59	103.78	104.18


Chamber (Oven)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
	Min , Max	Average					
104.0	-	104.0	103.97	0.07	0.70	0.42	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.


The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 

Certificate No. T222502

Page 4 of 4

Calibration Report

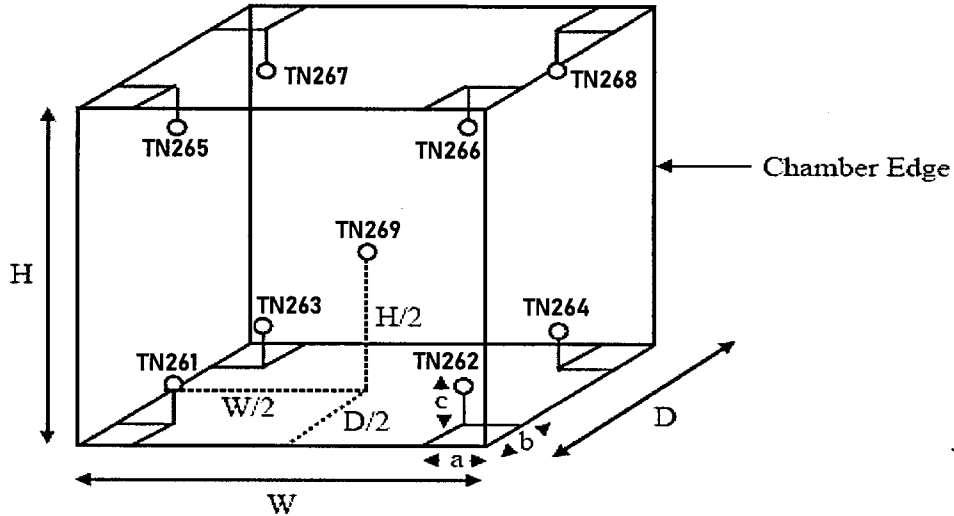

Remark :

Internal Dimensions of Chamber : W (Width) = 104 cm. , H (Height) = 72 cm. and D (Depth) = 60 cm.

Size of Installed Standard sensor number TN261 to number TN268 : a = 5 cm. ,b = 5 cm. and c = 5 cm.

Size of Installed Standard sensor number TN269 : W/2 = 104 cm./2 , H/2 = 72 cm./2 and D/2 = 60cm./2

Measurement Results

Calibration Point	Average Standard Reading at each position (° C)								
	TN261	TN262	TN263	TN264	TN265	TN266	TN267	TN268	TN269
180	179.14	179.17	179.65	179.26	180.41	179.64	181.18	180.99	180.36

Chamber (Oven)			Temperature Distribution				
Setting (° C)	Reading (° C)		Average (° C)	Stability (± ° C)	Uniformity (° C)	Uncertainty (± ° C)	Coverage Factor <i>k</i>
	Min , Max	Average					
180.0	-	180.0	179.98	0.38	1.78	1.10	2.00


* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing

a level of confidence of approximately 95 % .

Approved By. 

Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID: RYG_EN0136
Organization Name: ALS Laboratory Group (Thailand) Co Ltd.
Organization Location: 616/10 Moo 5, Tambol Mae Nam Koo, A.Pluakdaeng, Rayong, 21140, Thailand
Date: July 7, 2022 11:27:53 AM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.52, GCMS.02.52
Overall Qualification Status: Pass

REVIEW BY N. Banniy
APPROVED BY [Signature]
NEXT CAL. DATE 07/01/24

CDS Logon Verification - GC

Logon: dej.changchon

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Setpoint Status: Pass

	Setpoint	Actual
Inlet Pressure:	25.0 psi	25.1 psi
Accuracy:		0.1 psi
Agilent Recommended:		<= 1.2

Date: July 7, 2022 11:27:53 AM
System ID: RYG_EN0136

Overall Inlet Pressure Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name: 7890

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual

Temperature: 230.0 230.6 °C

Accuracy: 0.6 °C

Agilent Recommended: ≥ -1.0 % setpoint in K (-5.0 °C)
 ≤ 1.0 % setpoint in K (5.0 °C)

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual

Temperature: 100.0 99.9 °C

Accuracy: -0.1 °C

Agilent Recommended: ≥ -1.0 % setpoint in K (-3.7 °C)
 ≤ 1.0 % setpoint in K (3.7 °C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name: 7890

Setpoint Status: Pass

Setpoint/Average

Temperature: 100.0 99.91667 °C

Stability: 0.1 °C

Agilent Recommended: ≤ 0.5

Overall GC Oven Temperature Stability Test Status

Pass

Log Amp

Tested Combination1	Front	SSL	/ External	SQ
---------------------	-------	-----	------------	----

Name:	5977B			
-------	-------	--	--	--

Setpoint Status:	Pass			
------------------	------	--	--	--

Overall Log Amp Test Status

Pass

RFPA

Tested Combination1	Front	SSL	/ External	SQ
---------------------	-------	-----	------------	----

Name:	5977B			
-------	-------	--	--	--

Setpoint Status:	Pass			
------------------	------	--	--	--

Amu:	1050	m/z
------	------	-----

Drift After Five Minutes:

RFPA Voltage:

	-1	mV		479	mV
Agilent Recommended:	>= -100	and	<= 100	<= 1100	

Overall RFPA Test Status

Pass

Tune EI

Tested Combination1	Front	SSL	/ External	SQ
---------------------	-------	-----	------------	----

Name:	5977B			
-------	-------	--	--	--

Setpoint Status:	Pass			
------------------	------	--	--	--

Filament:	1
-----------	---

Setpoint Status:	Pass			
------------------	------	--	--	--

Filament:	2
-----------	---

Overall Tune EI Test Status

Pass

Signal to Noise EI

Date:	July 7, 2022 11:27:53 AM
System ID:	RYG_EN0136

Tested Combination1	Front	SSL	/ External	SQ
Name:	5977B			

Source:	El - Extractor	Filament:	1
---------	----------------	-----------	---

Setpoint Status:	Pass
------------------	------

Signal to Noise:	7485
------------------	------

Agilent Recommended:	>= 1200
----------------------	---------

Source:	El - Extractor	Filament:	2
---------	----------------	-----------	---

Setpoint Status:	Pass
------------------	------

Signal to Noise:	2097
------------------	------

Agilent Recommended:	>= 1200
----------------------	---------

This test's 2 comment(s) and 7 deviation(s) are available in the Attachments section.

Overall Signal to Noise EI Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	RYG_EN0136
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Manual Injection
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3442B
Serial Number	CN16463238
Firmware Revision	B.02.04.3
Component ID/Asset No.	081117000236
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5977B
Serial Number	US1701M008
Firmware Revision	5977 6.00.34
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std
Component ID/Asset No.	081117000236

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Extractor
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Eaknarin Puangsopa
Logged On User Name:	eaknarin_puangsopa@agilent.com
Signature Creation Date:	July 7, 2022
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Date:	July 7, 2022 11:27:53 AM
System ID:	RYG_EN0136

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 6, 2022 1:11:54 PM	Audit	SessionCreated	Session	None
July 6, 2022 1:11:54 PM	Start	Configuration	Session	None
July 6, 2022 1:11:54 PM	Audit	Entitlement	Licensing	User is Nonpaying and does not require an unlock code
July 6, 2022 1:17:19 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.52/Gc.02.52.eqp], EQP File Name: [Gc.02.52.eqp], EQP Name: [AgilentRecommended] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.52/GcMs.02.52.eqp], EQP File Name: [GcMs.02.52.eqp], EQP Name: [AgilentRecommended]
July 6, 2022 1:17:25 PM	End	Configuration	Session	None
July 6, 2022 1:17:29 PM	Start	Qualification	Session	OQ
July 6, 2022 1:17:30 PM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None
July 6, 2022 1:19:43 PM	End	Execution	CDS Logon Verification - GC : - Qualitative test	Run Count : 1
July 6, 2022 1:19:46 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 6, 2022 1:19:59 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
July 6, 2022 1:20:15 PM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
July 6, 2022 1:21:43 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
July 6, 2022 1:21:45 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
July 6, 2022 1:25:12 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
July 6, 2022 1:25:15 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
July 6, 2022 1:25:17 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
July 6, 2022 1:25:32 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
July 6, 2022 1:33:42 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry

Page 2 / 10

Date: July 7, 2022 11:27:53 AM
 System ID: RYG_EN0136

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 6, 2022 1:33:43 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
July 6, 2022 1:33:45 PM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
July 6, 2022 1:53:05 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
July 6, 2022 1:53:07 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
July 6, 2022 1:53:11 PM	Start	Execution	Log Amp - 5977B SQ: - Source: None EI - Extractor	
July 6, 2022 1:57:10 PM	End	Execution	Log Amp - 5977B SQ: - Source: EI EI - Extractor	Run Count : 1
July 6, 2022 1:57:24 PM	Start	Execution	RFPA - 5977B SQ: - Source: EI - Extractor	None
July 6, 2022 2:09:24 PM	End	Execution	RFPA - 5977B SQ: - Source: EI - Extractor	Run Count : 1
July 6, 2022 2:09:28 PM	Start	Execution	Tune EI - 5977B SQ: - Source: - None EI - Extractor Filament 1 (Qualitative - No setpoints associated)	
July 6, 2022 2:24:46 PM	End	Qualification	Session	OQ
July 6, 2022 2:24:46 PM	Start	Reporting	Session	None
July 6, 2022 2:41:39 PM	End	Reporting	Session	None
July 6, 2022 2:41:39 PM	Start	Configuration	Session	None
July 6, 2022 2:41:40 PM	End	Configuration	Session	None

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 6, 2022 2:41:40 PM	Start	Qualification	Session	OQ
July 6, 2022 2:41:40 PM	Start	Execution	Tune EI - 5977B SQ: - Source: - None EI - Extractor Filament 1 (Qualitative - No setpoints associated)	
July 6, 2022 2:41:56 PM	End	Execution	Tune EI - 5977B SQ: - Source: - Run Count : 1 EI - Extractor Filament 1 (Qualitative - No setpoints associated)	
July 6, 2022 2:41:58 PM	Start	Execution	Tune EI - 5977B SQ: - Source: - None EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
July 6, 2022 2:42:48 PM	End	Qualification	Session	OQ
July 6, 2022 2:42:48 PM	Start	Reporting	Session	None
July 6, 2022 2:50:52 PM	End	Reporting	Session	None
July 6, 2022 2:50:52 PM	Start	Qualification	Session	OQ
July 6, 2022 2:50:52 PM	Start	Execution	Tune EI - 5977B SQ: - Source: - None EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
July 6, 2022 2:51:12 PM	End	Qualification	Session	OQ
July 6, 2022 2:51:12 PM	Start	Reporting	Session	None
July 6, 2022 2:55:29 PM	End	Reporting	Session	None
July 6, 2022 2:55:29 PM	Start	Qualification	Session	OQ
July 6, 2022 2:55:29 PM	Start	Execution	Tune EI - 5977B SQ: - Source: - None EI - Extractor Filament 2 (Qualitative - No setpoints associated)	

User Name: eaknarin_puangsoapa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 6, 2022 2:55:40 PM	End	Execution	Tune EI - 5977B SQ: - Source: - Run Count : 1 EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
July 6, 2022 2:55:45 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 6, 2022 3:21:52 PM	End	Qualification	Session	OQ
July 6, 2022 3:21:52 PM	Start	Reporting	Session	None
July 6, 2022 3:25:04 PM	End	Reporting	Session	None
July 6, 2022 3:25:04 PM	Start	Qualification	Session	OQ
July 6, 2022 3:25:04 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 6, 2022 4:06:40 PM	Audit	AceClosed	Session	None
July 7, 2022 9:13:47 AM	Audit	AceRestarted	Session	None
July 7, 2022 9:13:49 AM	Audit	SessionReloaded	Session	None
July 7, 2022 9:13:54 AM	Start	Qualification	Session	OQ
July 7, 2022 9:13:54 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 7, 2022 9:58:06 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2022\OQF_N_SN_F01.D

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 7, 2022 9:59:53 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 1
July 7, 2022 10:01:46 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 1
July 7, 2022 10:01:46 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 7, 2022 10:02:00 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F01.D
July 7, 2022 10:04:55 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 2
July 7, 2022 10:07:30 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 2
July 7, 2022 10:07:30 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 7, 2022 10:07:44 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F01.D

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 7, 2022 10:08:18 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 3
July 7, 2022 10:10:28 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 3
July 7, 2022 10:10:28 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 7, 2022 10:10:55 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F01.D
July 7, 2022 10:14:03 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 4
July 7, 2022 10:14:54 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 4
July 7, 2022 10:14:54 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 7, 2022 10:15:15 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F01.D

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System Id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 7, 2022 10:15:27 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 5
July 7, 2022 10:16:48 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Deviation filed for Run Count : 5
July 7, 2022 10:16:48 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
July 7, 2022 10:17:05 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F01.D
July 7, 2022 10:17:14 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 6
July 7, 2022 10:18:40 AM	End	Qualification	Session	OQ
July 7, 2022 10:18:40 AM	Start	Reporting	Session	None
July 7, 2022 10:21:10 AM	End	Reporting	Session	None
July 7, 2022 10:21:10 AM	Start	Qualification	Session	OQ
July 7, 2022 10:21:17 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
July 7, 2022 10:56:49 AM	End	Qualification	Session	OQ
July 7, 2022 10:56:49 AM	Start	Reporting	Session	None
July 7, 2022 10:57:38 AM	End	Reporting	Session	None

Page 8 / 10

Date: July 7, 2022 11:27:53 AM
 System ID: RYG_EN0136

User Name: eaknarin_puangsoa
 Hostname: ASRYGW7002

System id: RYG_EN0136
 Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 7, 2022 10:57:38 AM	Start	Qualification	Session	OQ
July 7, 2022 10:57:38 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
July 7, 2022 11:06:50 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F021.D
July 7, 2022 11:11:47 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
July 7, 2022 11:13:13 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 1
July 7, 2022 11:14:29 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 1
July 7, 2022 11:14:29 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
July 7, 2022 11:14:47 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F021.D
July 7, 2022 11:16:34 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 2

User Name: eaknarin_puangsoa

System Id: RYG_EN0136

Hostname: ASRYGW7002

Print Date: July 7, 2022 11:27:56 AM

ALS_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
July 7, 2022 11:19:56 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 2
July 7, 2022 11:19:56 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
July 7, 2022 11:20:13 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2022\OFN_SN_F021.D
July 7, 2022 11:21:52 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 3
July 7, 2022 11:22:49 AM	End	Qualification	Session	OQ
July 7, 2022 11:22:49 AM	Start	Reporting	Session	None
July 7, 2022 11:26:46 AM	Audit	Reporting	Session	Report Generated : Certificate



Calibration Certificate

Certificate No. 520737
Product 200-510L Defender 510 Low Flow
Serial No. 206895
Cal. Date 24-Jan-2023
Sales Date

Sold To: Mesa Laboratories, Inc
12100 W 6th Ave
Lakewood, CO 80228
US

All calibrations are performed in accordance with ISO 17025 at Mesa Laboratories, Inc., 12100 W. 6th Ave, Lakewood, CO 80228, an ISO 17025:2017 accredited laboratory through NVLAP. This report shall not be reproduced except in full without the written approval of the laboratory. Results only relate to the items calibrated. This report must not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. Government.

Calibration Data

Certificate No 520737
Technician Derek Dellape
Lab. Pressure 617.3 mmHg
Lab. Temperature 23.6 °C

Instrument Reading	Lab Standard Reading	Deviation	Allowable Deviation	As Shipped
453.01 ccm	452.14 ccm	0.19%	1.00%	In Tolerance
101.86 ccm	102.2 ccm	-0.33%	1.00%	In Tolerance
31.91 ccm	31.88 ccm	0.09%	1.00%	In Tolerance

Mesa Laboratories Standards Used

Description	Standard Serial Number	Calibration Date	Calibration Due Date
ML_800_10	206627	19-Nov-2022	19-Nov-2023

Calibration Notes

The expanded uncertainty of flow has a coverage factor of $k = 2$ for a confidence interval of approximately 95%.

Flow testing is in accordance with our test number MP-00672 with an expanded uncertainty of 0.27% using high-purity nitrogen or filtered laboratory air.

Traceability to the International System of Units (SI) is verified by accreditation to ISO/IEC 17025 by NVLAP under NVLAP Code 200661-0.

Technician Notes:

By:

Approved By:

Derek Dellape
Production Assembler II

Christen Allen
Manager - Quality Assurance and Regulatory Affairs



MesaLabs



NVLAP Lab Code 200661-0
Calibration

Mesa Laboratories, Inc. certifies that the above instrument meets or exceeds published specifications, and that the calibration results in this certificate were obtained using equipment capable of producing results that are traceable through NIST to the International System of Units (SI). Calibration results are in compliance with ISO/IEC 17025:2017. Calibrations process has a Test Uncertainty Ratio (TUR) of 4:1 or greater. Any Pass/Fail determination is made without taking measurement uncertainty into account and is based on UUT performance against required tolerance only.




JIRANATEE ASSOCIATES CO., LTD.

CALIBRATION REPORTREVIEW BY Vichuta N.APPROVED BY Sararat M.NEXT CAL. DATE 9/2/67

CUSTOMER NAME : ALS Laboratory Group (Thailand) Co., Ltd.	
EQUIPMENT NAME : Total Hydrocarbon Analyzer	
MANUFACTURER : Baseline	MODEL : 9000 NMHC SERIAL NO : 0314DR0170
STANDARD GAS CONCENTRATION (PPM) : 100 PPM (Methane)	
CYLINDER NO : ND55981	
CYLINDER PRESSURE (psig) : 900 PSI	CERTIFIED DATE : 12/02/2022
CERTIFIED BY : AIRGAS	EXPIRED DATE : 12/02/2025

CALIBRATION RESULTS

POINT NO	CALIBRATION RESULTS			
	IDEAL	ACTUAL	ERROR	%ERROR
ZERO	0.00	0.00	0.00	-
1	100.00	101.00	1.0	1.00
AVERAGE (%)				0.25

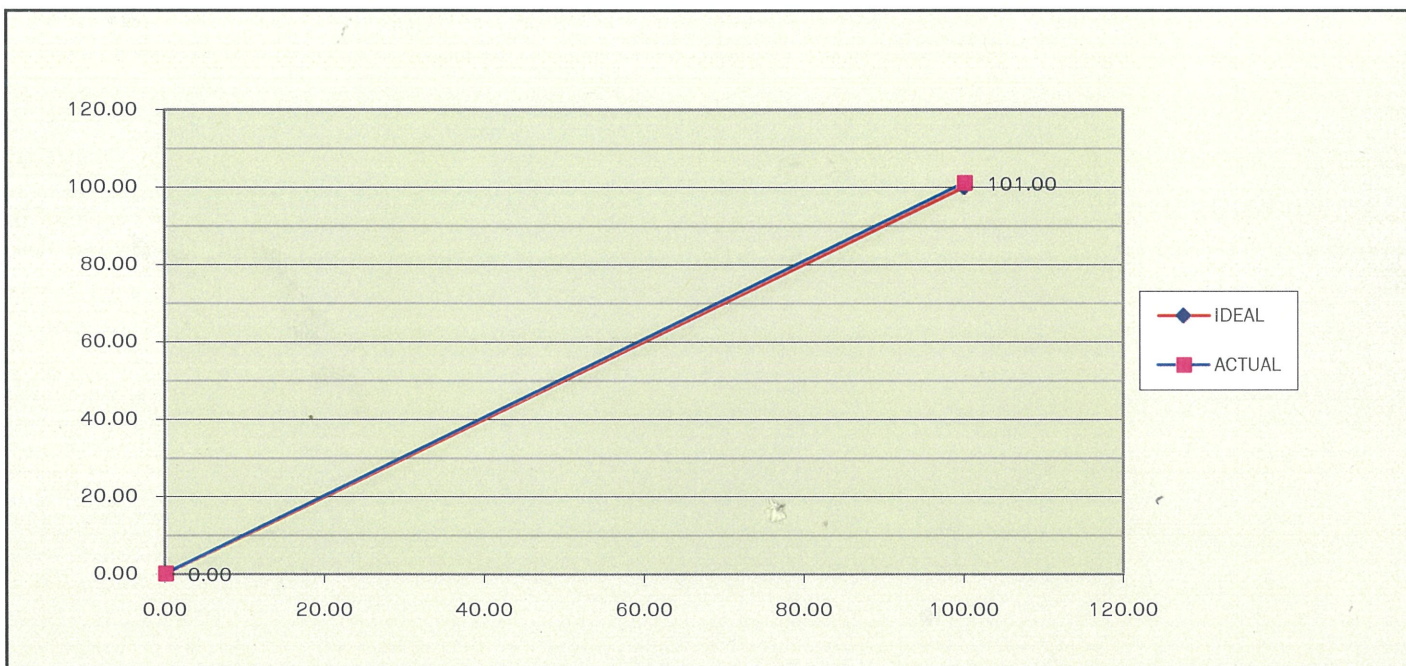CALIBRATED BY : วิภาพล ดุสิตเจริญDATE : 9/8/65CHECKED BY : ศุภชัย อังคารDATE : 9/8/65

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 31 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ถนน เพชรเกษม 7, 7/1 แขวง วัดท่าพระ เขต บางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02868-1889




JIRANATEE ASSOCIATES CO.,LTD.

CALIBRATION REPORT

CUSTOMER NAME : ALS Laboratory Group (Thailand) Co., Ltd.	
EQUIPMENT NAME : Total Hydrocarbon Analyzer	
MANUFACTURER : Baseline	MODEL : 9000 NMHC SERIAL NO : 0314DR0170
STANDARD GAS CONCENTRATION (PPM) : : 100 PPM (Propane)	
CYLINDER PRESSURE (psig) : 900 PSI	CERTIFIED DATE : 12/02/2022
CERTIFIED BY : AIRGAS	EXPIRED DATE : 12/02/2025

CALIBRATION RESULTS

POINT NO	CALIBRATION RESULTS			
	IDEAL	ACTUAL	ERROR	%ERROR
ZERO	0.00	0.00	0.00	-
1	300.00	301.00	1.0	0.33
AVERAGE (%)				0.08

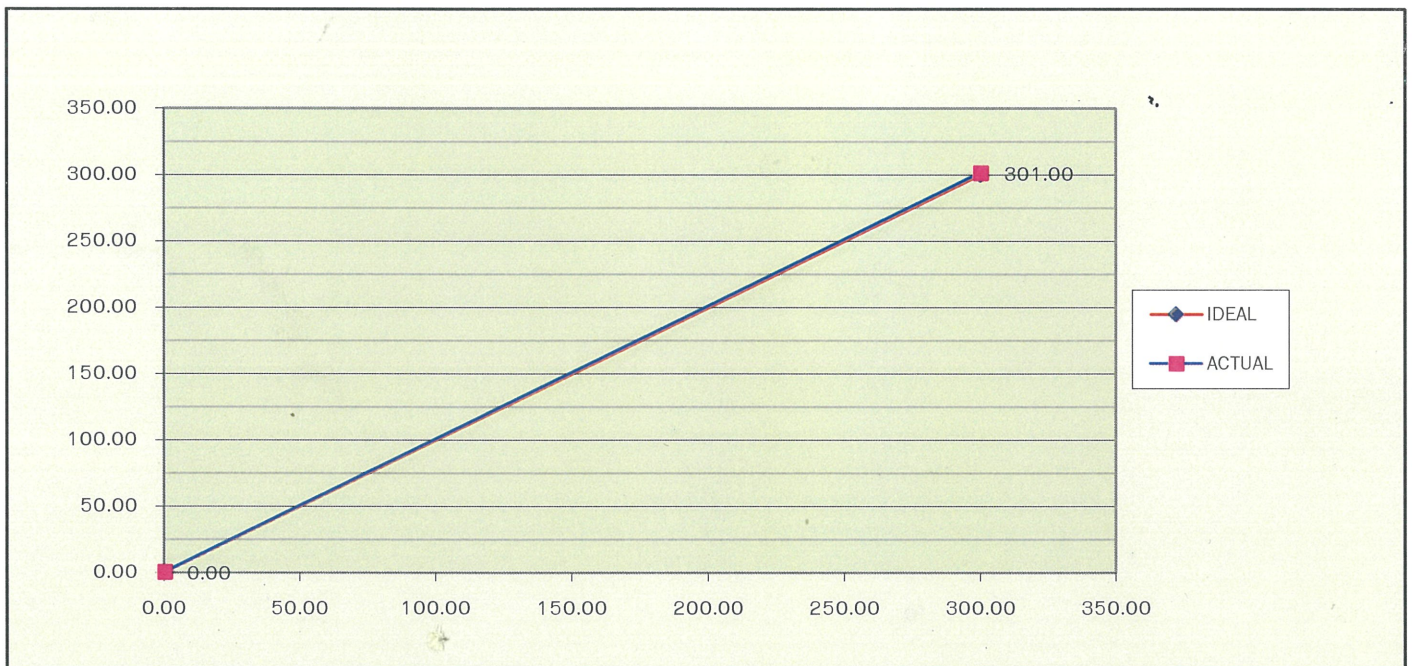

CALIBRATED BY : วรณล ศักดิ์เจริญ DATE : 9/8/65

CHECKED BY : ศิษฐ์ ด้วง DATE : 9/8/65



ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 31 , E-Mail : Engineer@jiranatee.com


เลขที่ 63/14-15,67/35-36 ถนนเพชรเกษม 7,7/1 แขวง วัดท่าพระ เขต บางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02868-1889

FLOW CALIBRATE

CUSTOMER NAME	: ALS Laboratory Group (Thailand) Co., Ltd.		
EQUIPMENT NAME	: Flow Calibrator		
MANUFACTURER	: Bios	MODEL : 510 L	SERIAL NO : 129549

Flow Parameter	Step	Set	Display	Flow Meter
Sample	Before	40	38	15 cc/min
	After	40	40	39.7 cc/min
Air	Before	175	175	190 cc/min
	After	175	175	176 cc/min
Fuel	Before	35	32	36 cc/min
	After	35	35	35 cc/min

CALIBRATED BY : วราพล ดวกังเจริญ **DATE :** 9/8/65
CHECKED BY : สันติ วัฒนา **DATE :** 9/8/65

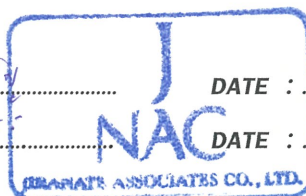

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ถนน เพชรเกษม 7,7/1 แขวง วัดท่าพระ เขต บางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02868-1889