

ประจำเดือนเมษายน พ.ศ. 2566



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax: 02-802-3773 E-mail : info@evltesting.com



Envilab & Navee Supply from evl

TSP High Volume Sampler Calibration

Verification Report No.

A6604 -TSP 02

☐ PM ☐ Onsite

Site: บริษัท เอ็นไวแล็บ จำกัด

UTM : 47P N1514475 E654269

Sampler: ETSP#15

Recorder: TEST Report

Date: 1 Apr 23

Technical: Sanayu J.

Approval: Wisan R.

CONDITIONS

Barometric Press. (hPa): 1010.0

Temperature (deg C): 32.0

Average Press. (hPa): 1013.0

Average Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 757.6

Temperature (deg K): 305.0

Corrected Avg. Press. (mm Hg): 759.8

Average Temp. (deg K): 303.0

CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc

Model: TE-5028A

Serial#: 1328


Qstd Slope: 1.63957

Qstd Intercept: -0.01202

Date Certified: 19 Jan 2023

CALIBRATIONS

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	12.97	2.175	52.0	51.32	Slope = 11.0469
2	9.42	1.855	48.0	47.37	Intercept = 26.9380
3	6.71	1.566	44.0	43.42	Corr. coeff. = 0.9957
4	4.46	1.278	42.0	41.45	# of Observations: 5
5	2.42	0.944	38.0	37.50	Range of Chart 40
					at 1.1 - 1.7 m3/min. 46

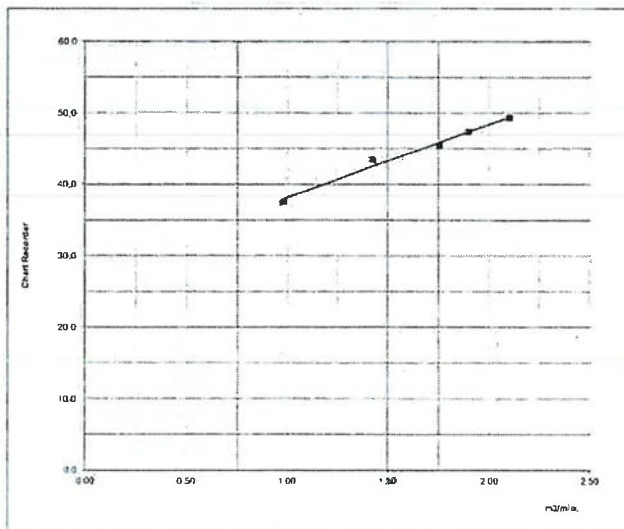

Calibrated by :

(Sanayu Jantason)
1 April 2023

Approved by :

(Wisan Ritthikamon)
1 April 2023

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

FE-MNT-29 Rev.00:01/08/63



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax: 02-802-3773 E-mail : info@evltesting.com



Printed & signed by instrument

PM10 High Volume Sampler Calibration

Verification Report No.

A6604 -PM 02

<input checked="" type="checkbox"/> PM	<input type="checkbox"/> Onsite
Site: บริษัท เอ็นไวแล็บ จำกัด	
UTM : 47P N1514475 E654269	
Sampler: EPM#01	
Recorder: Test Report	
Date: 1 Apr 23	
Technical: Sanayu J.	
Approval: Wisan R.	

CONDITIONS


Barometric Press. (hPa): 1010.0	Corrected Pressure (mm Hg): 757.6
Temperature (deg C): 32.0	Temperature (deg K): 305.0
Average Press. (hPa): 1013.0	Corrected Avg.Press. (mm Hg): 759.8
Average Temp. (deg C): 30.0	Average Temp. (deg K): 303.0

CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc	Qstd Slope: 1.02667
Model: TE-5028A	Qstd Intercept: -0.00753
Serial#: 1328	Date Certified: 19 Jan 2023

CALIBRATIONS

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	12.13	2,160	52.0	32.99	Slope = 11.0835
2	10.39	1,999	48.0	30.46	Intercept = 8.7062
3	8.86	1,847	46.0	29.19	Corr. coeff. = 0.9966
4	5.98	1,519	40.0	25.38	SFR = 1.141
5	4.87	1,371	38.0	24.11	SSP = 33.65
					# of Observations: 5
					Range of Chart at SFR $\pm 10\%$
					32
					35

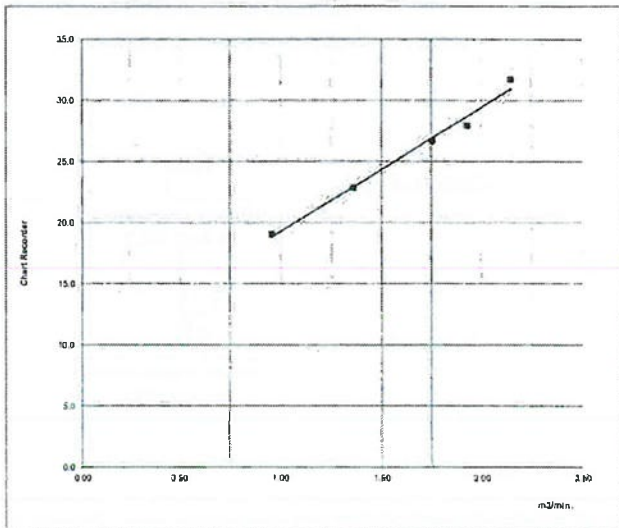

Calibrated by :
(Sanayu Jantason)
1 April 2023

Approved by :
(Wisan Ritthikamon)
1 April 2023

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

PM10 Cal. Rev.07 / Iss.Date Mar 17, 2020

Environmental responsibility with accuracy measurement

FE-MNT-29 Rev.001/38/53



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



neediss

บริษัท นีดิส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.

336 ซอยบางนา 7 แขวงบางนา เขตบางนา กรุงเทพมหานคร 10150 536 Soi Bangna 7 Bangnae Bangkok Bangkok
Tel 02-802-3980-2 Fax 02-802-3988 E:info@neediss.com



SO₂ Analyzer Verification Test Report

Calibration Report No.: 6604001

Page:1/1

Calibrated Date: 1-Apr-23

☒ PM ☐ Onsite

Instruments Information

Analyzer Type: SO2 Analyzer Model: THERMO.,43C	Manufacturer THERMO S/N: ESOTE43C102362
---	--

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model ESA MGC101 S/N: 792 ZERO AIR Generator ZAG7001 S/N: 644	NO Conc 44.68 PPM SO2 Conc 45.34 PPM CO Conc 4500 PPM Expire Date: Feb 19,2024 EB0140762

Environment: Temperature 26.2 °C

Humidity: 50 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	2.3	2.3	400.0	413	3.3
After	0.0	0.8	0.8	400.0	405	1.3

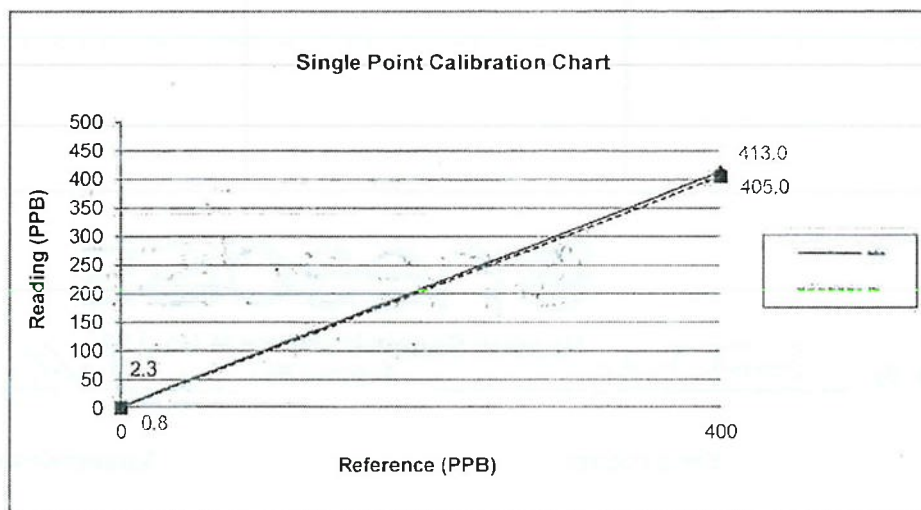

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.



www.neediss.com



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



MODEL : SO2 ANALYZER Model 43C THERMO

DATE : 1-04-2023

S/N : ESOTE43C102362

Test Function Value	Before	After
Range 500 (PPB)	500	500
PMT VOLTS -450 - -850 (V)	-650	-653
LAMP VOLTAGE 950 - 1,200 (V)	990	985
LAMP INTENSITY 20000 - 50000 Hz	32568	32577
INTER TEMP 15 - 45 DEG C	37	37
CHAMBER TEMP 47 - 51 C	49	49
COOLER TEMP -5 - (-2) DEG C	-2.5	-2.5
PRESSURE 400 - 1000.0 mm Hg	764	765
FLOW 0.350 - 0.650 LPM	0.42	0.4



Neediss Supply Instrument Co., Ltd.

Calibrate By :

Sirirat Poonlak

Approve By :

Sarawat Keawsrinal

Sirirat Poonlak

Sarawat Keawsrinal

Date:

1-Apr-23

Date:

1-Apr-23

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

www.neediss.com



รับรองสำเนาถูกต้อง
 ผู้จัดการฝ่ายควบคุมคุณภาพ



neediss

บริษัท นีดิส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.

535 ซอยบางนา 7 แขวงบางนา เขตคลองเตย กรุงเทพฯ 10160 535 Soi Bangna 7 Bangkok Bangkok Bangkok
Tel: 02-802-1780 E-Mail: info@neediss.com



NOx Analyzer Verification Test Report

Calibration Report No.: 6604001

Page:1/2

Calibrated Date: 1-Apr-23

☒ PM ☐ Onsite

Instruments Information

Analyzer Type: NO/NO₂/NOx Analyzer
Model: 42C

Manufacturer THERMO
S/N: ENOTE42C412226

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model ESA MGC101 S/N: 792 ZERO AIR Generator ZAG7001 S/N: 644	NO Conc 44.68 PPM SO ₂ Conc 45.34 PPM CO Conc 4500 PPM Expire Date: Feb 19,2024 EB0140762

Environment: Temperature 27.1 °C


Humidity: 52 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	2.4	0.0	2.4	412	400.0	1.5
NO ₂	0.7	0.0	0.7	2.0	0.0	0.2
NOx	3.1	0.0	3.1	414	400.0	1.7

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.5	0.0	0.5	402	400.0	0.2
NO ₂	0.7	0.0	0.7	2.0	0.0	0.2
NOx	1.2	0.0	1.2	404	400.0	0.5

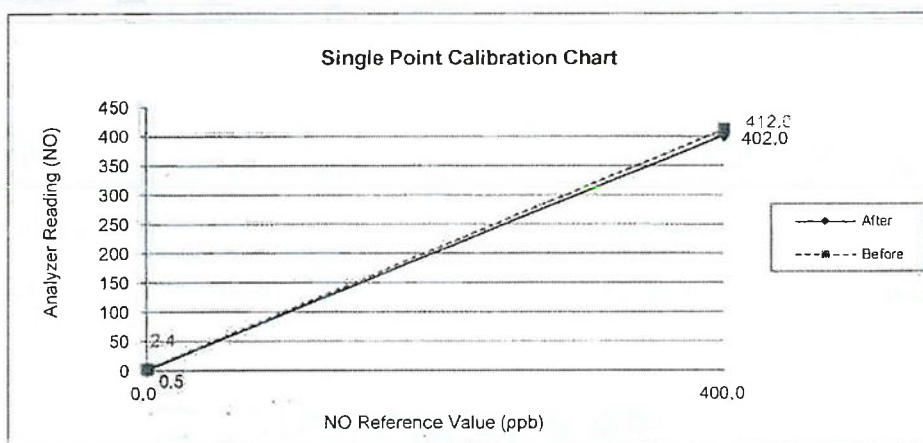

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

www.neediss.com



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



neediss

บริษัท นีดีส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.

538 ซอยปทุมมา 7 แขวงปทุมมา เขตปทุมธานี กรุงเทพมหานคร 10130 538 Soi Puthuma 7 Bangkhuae Bangkok 10130
Tel : 02-802-1990-2 Fax : 02-802-3908 E: info@neediss.com



MODEL : NOx ANALYZER Model 42C THERMO

DATE : 1-04-2023

S/N : CNOTE42C412226

Page: 2/2

Test Function Value	Before	After
Range 500 (PPB)	500	500
PMT VOLTS -450 - -850 (V)	-675	-678
LAMP VOLTAGE 950 - 1,200 (V)		
INTER TEMP 15 - 45 DEG C	43	43
CHAMBER TEMP 47 - 51 C	49	50
COOLER TEMP -5 - (-2) DEG C	-2	-2
PRESSURE 400 - 1000.0 mm Hg	350	380
SAMPLE FLOW 0.350 - 0.900 LPM	0.45	0.46
OZONEATOR FLOW 0.035 - 0.075 LPM	0.05	0.05
No/Nox BKG	12/9.0	12/9.1
No/Nox Slope	1.0/0.8	0.9/0.8

Calibrate By : Sirirat Poonlak

Approve By : Sarawat Keawsrinual

Sirirat Poonlak

Sarawat Keawsrinual

Date: 1-Apr-23

Date: 1-Apr-23



Neediss Supply Instrument Co., Ltd.

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

www.neediss.com



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ
EnviLab Co., Ltd.



บริษัท เอ็นไวเทสティング จำกัด 140/540/1 ซอย บางกะปิ 7 แขวง บางกะปิ เขต บางกะปิ กรุงเทพมหานคร 10180
Envilab Co., Ltd. 140,540/1 Soi Bangkok 7 Bangkok Bangkok Bangkok 10180
Tel : 02-602-3077-2 Fax : 02-602-3773 E-mail : info@evitestin.com



www.evitestin.com

Verification Test Report

Report No.:

CONDO -SLM 01

☒ PM

☐ Onsite UTM:

47P N 1514455 E 654248

Calibrated Date: 1 April 2023

Site : บริษัทเอ็นไวเทสติ้ง จำกัด

Equipment: Sound Level Meter

Manufacturer: PULSAR

Model: 45

Serial : 0012

Environment: Temperature 25 °C Humidity 71 %RH

Reference Standard: Acoustic Calibrator Class 1 Model CB011,CESVA

Serial No.T252953

Date of Calibration : 02 December 2022

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.92	93.94	0.02	93.92

Calibrated By:

(Sanayu Jantason)

Date:

1 April 2023

Approve By:

(Wisan Ritthikamon)

Date:

1 April 2023

This report shall not be reproduced except in full, without the written approval of Envilab Co.,Ltd.





บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-9577-8 Fax: 02-802-3773 E-mail : info@evltesting.com



Envilab, a. Environmental Quality Measurement

TSP High Volume Sampler Calibration

Verification Report No.

A6604 -TSP 01

<input checked="" type="checkbox"/> PM <input type="checkbox"/> Onsite	Site: บริษัท เอ็นไวแล็บ จำกัด	Date: 1 Apr 23
	UTM : 47P N1514475 E654269	Technical: Sanayu J.
	Sampler: NTSP#11	Approval: Wisan R.
	Recorder: TEST Report	

CONDITIONS


Barometric Press. (hPa): 1010.0	Corrected Pressure (mm Hg): 757.6
Temperature (deg C): 32.0	Temperature (deg K): 305.0
Average Press. (hPa): 1013.0	Corrected Avg. Press. (mm Hg): 759.8
Average Temp. (deg C): 30.0	Average Temp. (deg K): 303.0

CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc	Qstd Slope: 1.63957
Model: TE-5028A	Qstd Intercept: -0.01202
Serial#: 1328	Date Certified: 19 Jan 2023

CALIBRATIONS

Plate or Test #	H2O (In)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	12.10	2.101	50.0	49.34	Slope = 10.2722
2	9.88	1.899	48.0	47.37	Intercept = 27.8347
3	8.42	1.754	46.0	45.40	Corr. coeff.= 0.9925
4	5.57	1.428	44.0	43.42	# of Observations: 5
5	2.62	0.982	38.0	37.50	Range of Chart at 1.1 - 1.7 m3/min. 40 45

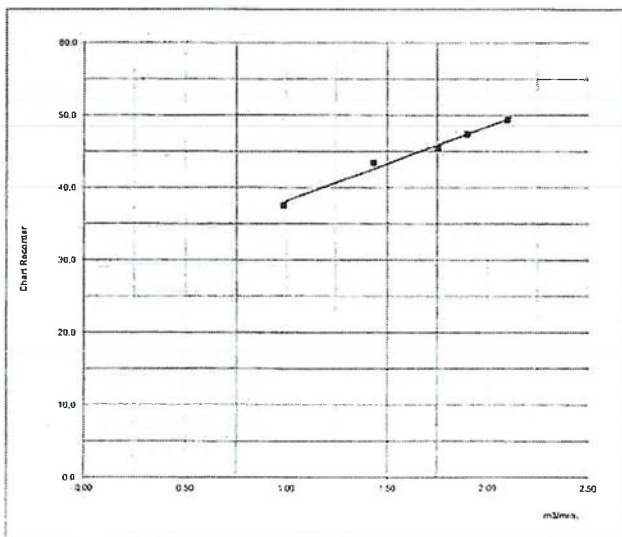

Calibrated by :

(Sanayu Jantason)
1 April 2023

Approved by :

(Wisan Ritthikamon)
1 April 2023

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

RE-MNT-29 Rev 00/01/08/63



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10150
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10150
Tel : 02-802-3577-8 Fax : 02-802-3773 E-mail : info@evltesting.com



Circle 3: Verify Supply Instrument

PM10 High Volume Sampler Calibration

Verification Report No.

ACC04 -PM 01

☒ PM ☐ Onsite

Site: บริษัท เอ็นไวแล็บ จำกัด
UTM : 47P N1514475 E654269
Sampler: NPM#13
Recorder: Test Report

Date: 1 Apr 23
Technical: Sanayu J.
Approval: Wisan R.

CONDITIONS

Barometric Press. (hPa): 1010.0
Temperature (deg C): 32.0
Average Press. (hPa): 1013.0
Average Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 757.6
Temperature (deg K): 305.0
Corrected Avg. Press. (mm Hg): 759.8
Average Temp. (deg K): 303.0

CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc
Model: TE-5028A
Serial#: 1328

Qstd Slope: 1.02667
Qstd Intercept: -0.00753
Date Certified: 19 Jan 2023


CALIBRATIONS

Plate or Test #	H2O (In)	Qa (m3/min)	I (chart)	IC (corrected)
1	12.03	2.151	50.0	31.73
2	9.67	1.929	44.0	27.92
3	7.99	1.754	42.0	26.65
4	4.76	1.356	36.0	22.84
5	2.34	0.953	30.0	19.04

LINEAR REGRESSION

Slope = 10.1267
Intercept = 9.1422
Corr. coeff. = 0.9929
SFR = 1.141
SSP = 32.62
of Observations: 5

Range of Chart at SFR $\pm 10\%$ 32 34

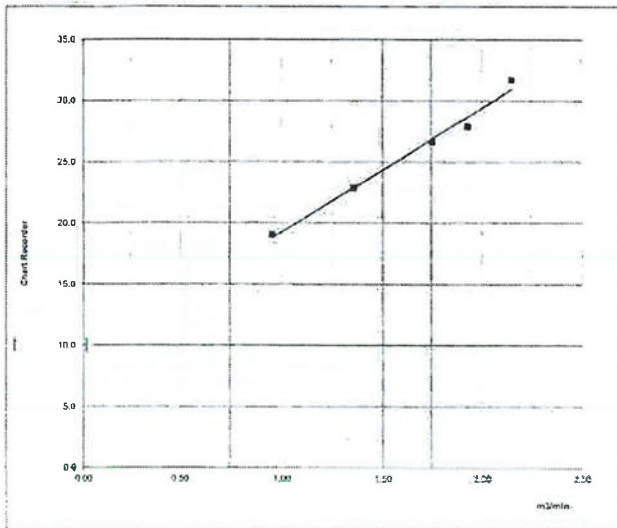

Calibrated by :

(Sanayu Jantason)
1 April 2023

Approved by :

(Wisan Ritthikamon)
1 April 2023

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

Rev. 01:20 Rev. 00:01/04/21



บริษัท เอ็นไวแล็บ จำกัด
ผู้ดำเนินการฝ่ายควบคุมคุณภาพ



บริษัท นีดิส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.
535 ซอยบางนา 7 แขวงบางนา เขตบางนา กรุงเทพฯ 10150. 535 Soi Bangnae 7 Bangnae Bangkok Bangkok
Tel: 02-802-3780-3 Fax: 02-802-3783 E-mail: neediss@neediss.com



SO₂ Analyzer Verification Test Report

Calibration Report No.: 6604002

Page:1/1

Calibrated Date: 1-Apr-23

☒ PM ☐ Onsite

Instruments Information

Analyzer Type: SO2 Analyzer Model: THERMO.,43C	Manufacturer THERMO S/N: ESOTE43C069865
---	--

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model ESA MGC101 S/N: 792 ZERO AIR Generator ZAG7001 S/N: 644	NO Conc 44.68 PPM SO2 Conc 45.34 PPM CO Conc 4500 PPM Expire Date: Feb 19,2024 EB0140762

Environment: Temperature 26.2 °C

Humidity: 50 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	4.5	4.5	400.0	411	2.8
After	0.0	0.2	0.2	400.0	402	0.5

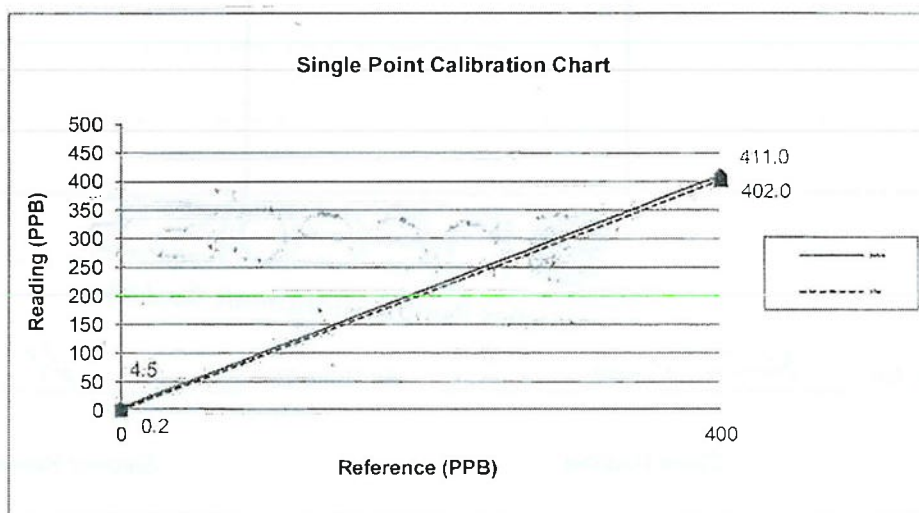

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.



www.neediss.com



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



neediss

บริษัท นีดิส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.
535 ซอยพหลโยธิน / แขวงสามยุค เขตบางพลี กรุงเทพมหานคร 10140 535 Soi Bangkhuae 7 Bangkhuae Bangkok
Tel 02 802 3580-2 Fax 02 802 3588 Email:info@neediss.com



MODEL : SO2 ANALYZER Model 43C THERMO

DATE : 1-04-2023

S/N : ESOTE43C069865

Test Function Value	Before	After
Range 500 (PPB)	500	500
PMT VOLTS -450 - -850 (V)	-650	-653
LAMP VOLTAGE 950 - 1,200 (V)	990	985
LAMP INTENSITY 20000 - 50000 Hz	32568	32577
INTER TEMP 15 - 45 DEG C	37	37
CHAMBER TEMP 47 - 51 C	49	49
COOLER TEMP -5 - (-2) DEG C	-2.5	-2.5
PRESSURE 400 - 1000.0 mm Hg	764	765
FLOW 0.350 - 0.650 LPM	0.42	0.4

neediss

Neediss Supply Instrument Co.,Ltd.

Calibrate By : Sirirat Poonlak

Approve By : Sarawat Keawsrinual

Sirirat Poonlak

Sarawat Keawsrinual

Date: 1-Apr-23

Date: 1-Apr-23

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.



www.neediss.com



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



neediss

บริษัท เน็ดิส ซัพพลาย อินสตรูमेंท์ จำกัด
Neediss Supply Instrument Co., Ltd.
535 ซอยวิภาวดี 7 แขวงวิภาวดี เขตจตุจักร กรุงเทพฯ 10160 535 Soi: Bangchao 7 Bangkok Bangkok Bangkok
Tel: 02-802-3980-2 Fax: 02-802-3988 Email: neediss.com



NOx Analyzer Verification Test Report

Calibration Report No.: 6604002

Page:1/2

Calibrated Date: 1-Apr-23

☒ PM ☐ Onsite

Instruments Information

Analyzer Type: NO/NO ₂ /NOx Analyzer Model: 42C	Manufacturer THERMO S/N: ENOTE42C304779
---	--

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model ESA MGC101 S/N: 792 ZERO AIR Generator ZAG7001 S/N: 644	NO Conc 44.68 PPM SO ₂ Conc 45.34 PPM CO Conc 4500 PPM Expire Date: Feb 19,2024 EB0140762

Environment: Temperature 27.1 °C


Humidity: 52 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	5.6	0.0	5.6	410	400.0	1.2
NO ₂	2.7	0.0	2.7	3.0	0.0	0.4
NOx	8.3	0.0	8.3	413	400.0	1.6

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.6	0.0	0.6	404	400.0	0.5
NO ₂	0.3	0.0	0.3	3.0	0.0	0.4
NOx	0.9	0.0	0.9	407	400.0	0.9

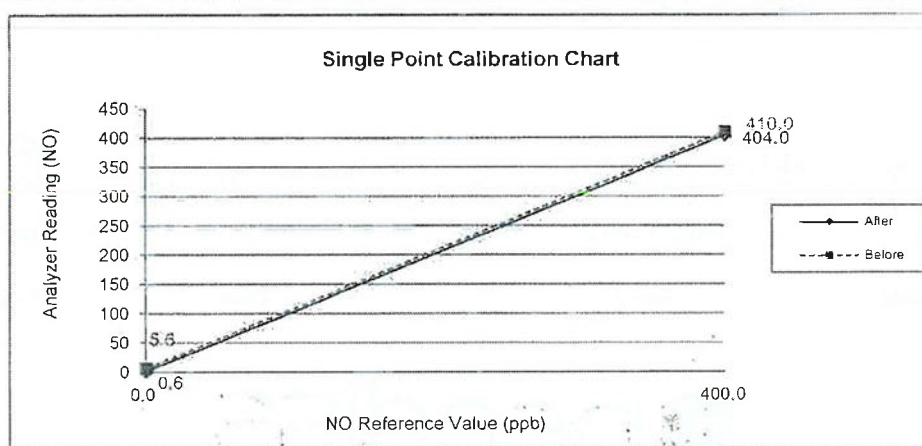

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

www.neediss.com



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



บริษัท นีดีส ซัพพลาย อิน스트รูमेंท์ จำกัด
Neediss Supply Instrument Co., Ltd.

506 ซอยรามคำแหง 7 แขวงบางนาแค เขตบางนา กรุงเทพมหานคร 10160 506 Soi Ramkhamhaeng 7 Bang Na Bangkhae Bangkok
Tel: 02-402 1997-9 Fax: 02-861 3288 Email: neediss.com



MODEL : NOx ANALYZER Model 42C THERMO

DATE : 1-04-2023

S/N : ENOTE12C304779

Page:2/2

Test Function Value	Before	After
Range 500 (PPB)	500	500
PMT VOLTS -450 - -850 (V)	-675	-678
LAMP VOLTAGE 950 - 1,200 (V)		
INTER TEMP 15 - 45 DEG C	43	43
CHAMBER TEMP 47 - 51 C	49	50
COOLER TEMP -5 - (-2) DEG C	-2	-2
PRESSURE 400 - 1000.0 mm Hg	350	380
SAMPLE FLOW 0.350 - 0.900 LPM	0.45	0.46
OZONEATOR FLOW 0.035 - 0.075 LPM	0.05	0.05
No/Nox BKG	12/9.0	12/9.1
No/Nox Slope	1.0/0.8	0.9/0.8

Calibrate By : Sirint Poonlak

Approve By : Sarawat Keawsrinual

Sirint Poonlak

Sarawat Keawsrinual

Date: 1-Apr-23

Date: 1-Apr-23



Neediss Supply Instrument Co.,Ltd.

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

www.neediss.com



EPB Co.,Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



บริษัท เอ็นวิล เทสติ้ง จำกัด (มหาชน)
Envilab Co., Ltd. 443/49/1 หมู่ 9 ซอยสุขุมวิท 23 แขวงคลองเตย เขตคลองเตย กรุงเทพฯ 10110
Tel : 02-262-3577-8 Fax : 02-262-3773 E-mail : info@evltesting.com



Verification Test Report

Report No.:

CONDO -SLM 02

☒ PM ☐ Onsite UTM : 47P N 1514455 E 654248

Calibrated Date: 1 April 2023

Site : บริษัทเอ็นไวแล็บ จำกัด

Equipment: Sound Level Meter

Manufacturer: PULSAR

Model: 45

Serial : 0013

Environment: Temperature 25 °C Humidity 71 %RH

Reference Standard: Acoustic Calibrator Class 1 Model CB011,CESVA

Serial No.T252953

Date of Calibration : 02 December 2022

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.92	93.94	0.02	93.92

Calibrated By:

(Sanayu Jantason)

Date:

1 April 2023

Approve By:

(Wisan Ritthikamon)

Date:

1 April 2023

This report shall not be reproduced except in full, without the written approval of Envilab Co.,Ltd.



Certificate of Calibration

Calibration Certification Information

Cal. Date: January 18, 2023 Rootsmeter S/N: 438320 Ta: 294 °K
 Operator: Jim Tisch Pa: 750.1 mm Hg
 Calibration Model #: TE-5025A Calibrator S/N: 0759

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.3960	3.2	2.00
2	3	4	1	0.9950	6.4	4.00
3	5	6	1	0.8850	8.0	5.00
4	7	8	1	0.8450	8.8	5.50
5	9	10	1	0.6990	12.8	8.00

Data Tabulation

Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9961	0.7135	1.4145	0.9957	0.7133	0.8854
0.9918	0.9968	2.0004	0.9915	0.9964	1.2521
0.9897	1.1183	2.2365	0.9893	1.1179	1.3999
0.9886	1.1700	2.3456	0.9883	1.1695	1.4683
0.9833	1.4067	2.8289	0.9829	1.4062	1.7708
QSTD	m=	2.03736	QA	m=	1.27576
	b=	-0.03733		b=	-0.02337
	r=	0.99997		r=	0.99997

Calculations

Vstd=	$\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$	Va=	$\Delta Vol((Pa-\Delta P)/Pa)$
Qstd=	Vstd/ΔTime	Qa=	Va/ΔTime
For subsequent flow rate calculations:			
$Qstd = 1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$		$Qa = 1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$	

Standard Conditions

Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH: calibrator manometer reading (in H2O)	
ΔP: rootsmeter manometer reading (mm Hg)	
Ta: actual absolute temperature (°K)	
Pa: actual barometric pressure (mm Hg)	
b: intercept	
m: slope	

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30

Certificate of Calibration

Certificate No. : 66 200035-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Electronic Balance
Manufacturer : Sartorius **Model :** SECURA224-1S
Serial No. : 0034803270 **ID No. :** ELABBALANCEN04
Capacity : 220 g **Resolution :** 0.0001 g

Environment : On site calibration was carried out at the Balance Room, Envilab Co., Ltd.
Ambient Temperature : (23.4 to 23.7) °C
Relative Humidity : (61.4 to 62.8) %
Air Pressure : 1011.0 mbar

Date of Received : 02 February 2023

Date of Calibration : 02 February 2023

Date of Issue : 04 February 2023

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02222345	10 Nov 2023	National Institute of Metrology (Thailand), (NIMT)

Approved by :



(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

Certificate of Calibration

Certificate No. : 66-200035-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.01	0.0001	0.00011
0.1	0.0001	0.00011
1	0.0000	0.00011
2	0.0001	0.00011
5	0.0000	0.00012
10	0.0000	0.00011
20	0.0000	0.00013
50	0.0001	0.00014
100	0.0000	0.00020
200	-0.0001	0.00038


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.11$, providing a level of confidence of approximately 95%

Eccentric error Load test : 50 g

A	B	C	D	E
-0.0001	0.0001	0.0000	-0.0001	0.0000

g



Repeatability Load test : 200 g

 Stdev. : 0.00000 g

- o0o -

Handwritten signature

Certificate of Calibration

Certificate No. : 66-200035-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhæ 7, Bangkhæ, Bangkok 10160

Equipment : Electronic Balance
Manufacturer : Sartorius **Model :** SECURA3102-1S
Serial No. : 0034409695 **ID No. :** ELABBALANCEN03
Capacity : 3100 g **Resolution :** 0.01 g

Environment : On site calibration was carried out at the Balance Room, Envilab Co., Ltd.
Ambient Temperature : (23.4 to 23.6) °C
Relative Humidity : (59.5 to 61.9) %
Air Pressure : 1011.0 mbar

Date of Received : 02 February 2023

Date of Calibration : 02 February 2023

Date of Issue : 04 February 2023

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
F181-F1821	66-210034-1	30 Jul 2023	National Institute of Metrology (Thailand), (NIMT)

Approved by :



(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-200035-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
10	0.00	0.0082
20	0.00	0.0082
50	0.00	0.0082
100	0.00	0.0082
200	0.00	0.0083
500	0.00	0.0085
1000	0.00	0.0110
1500	0.00	0.012
2000	0.00	0.012
3000	0.00	0.023


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 1000 g

A	B	C	D	E	
0.00	-0.01	0.01	0.00	0.00	g



Repeatability

Load test : 2000 g

Stdev. : 0.000 g

- o o o -

Handwritten signature





THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0123

MTC No. EEL. BP. 76/1165

CALIBRATION CERTIFICATE

Submitted by : Envilab Co.,Ltd.

Address : 540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkhuae, Bangkok 10160.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Acoustic Calibrator

Manufacturer : CESVA

Model : CB011

Serial No. : T252953

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 28 Nov. 2022

Date of Calibration : 2 Dec. 2022

1 / 2
✓

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121 30 ext. 3219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : mtc@tistr.or.th



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0123

MTC No. EEL. BP. 76/1165

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.92	-0.08	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	± 1.5	$\pm 1.0\%$

3. Total distortion


Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.30	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :


(Mr. Weerachai Deechaiyae)

Approved by :


(Mr. Prawate Kluaypa)
Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 2 Dec. 2022

Date of Issue : 2 Dec. 2022

Ref : 2011265112805100001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)
LTD
Part Number: E05NI91E15A0003
Cylinder Number: EB0146406
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12022
Gas Code: CO,CO2,NO,NOX,SO2,BALN
Reference Number: 160-402305646-1
Cylinder Volume: 148.7 CF
Cylinder Pressure: 2015 PSIG
Valve Outlet: 660
Certification Date: Jan 03, 2022

Expiration Date: Jan 03, 2030

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	12/27/2021, 01/03/2022
CARBON MONOXIDE	100.0 PPM	98.02 PPM	G1	+/- 0.5% NIST Traceable	12/27/2021
NITRIC OXIDE	100.0 PPM	100.1 PPM	G1	+/- 1.0% NIST Traceable	12/27/2021, 01/03/2022
SULFUR DIOXIDE	100.0 PPM	100.2 PPM	G1	+/- 1.0% NIST Traceable	12/27/2021, 01/03/2022
CARBON DIOXIDE	8.000 %	7.962 %	G1	+/- 0.9% NIST Traceable	12/27/2021
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	09010241	KAL004894	98.48 PPM CARBON MONOXIDE/NITROGEN	+/- 0.5%	Oct 16, 2024
NTRM	200610-56	CC733475	98.61 PPM NITRIC OXIDE/NITROGEN	+/- 0.6%	Oct 06, 2026
GMIS	124206889119	CC322885	4.294 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.0%	Sep 03, 2024
NTRM	11010419	KAL004813	99.6 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jul 28, 2023
NTRM	08010636	K019200	13.94 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	Jan 30, 2024

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO2	FTIR	Dec 02, 2021
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Dec 09, 2021
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Dec 16, 2021
Nicolet iS50 FTIR AUP2010245 NO2	FTIR	Dec 29, 2021
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Dec 23, 2021

Triad Data Available Upon Request

NOTES: Gross Weight: 28.1 Kg, Net Weight: 5.1 Kg.

UF0X5CX



Mulata Nukha
Approved for Release




รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



Supplement to Calibration Certificate No. Q22080017

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2601/721A3301
SERIAL NO.	:	UM14632/UM14632[EVMINMMATE4632]
CLID. NO.	:	252101369
JOB CONTROL NO.	:	220809080017

CUSTOMER : ENVILAB CO., LTD.
540, 540/1 SOI BANGKHAE 7, BANGKHAE,
BANGKHAE, BANGKOK 10160 THAILAND

DATE OF RECEIVED : 09 August 2022

DATE OF ISSUED : 23 August 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong
Calibration Engineer



Approved By : Mongkol Yotsoontorn
Authorized Signatory
23 August 2022

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22080017A1

F3-012-04/01-12




page 1 of 3
รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ
e:calibration





CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2601/721A3301
SERIAL NO. : UM14632/UM14632[EVMINMMATE4632]
DATE OF CALIBRATION : 10 August 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.
The calibration was performed by using Digital Multimeter, High Resolution Programmable Timer/Counter, Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Digital Multimeter, Hewlett Packard Model 34401A S/N. 3146A75935.
2. High Resolution Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2525 S/N. 397018, 2434988.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0112-21, Due Date 26 October 2022.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0001/22, Due Date 22 February 2023.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV 0009 22, Due Date 22 June 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22080017

F3-011-04/01-12

page 2 of 3



รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ
iactcalibration






CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
10	50 Hz	peak	10.000	10.224	-0.224	2.3
20	50 Hz		20.000	20.477	-0.477	1.8
30	50 Hz		30.000	30.692	-0.692	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 1 of 54

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22080017

F3-011-04/01-12

page 3 of 3



Certificate of Calibration

Certificate No. : 66-200066-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : Electronic Balance

Manufacturer : METTLER TOLEDO **Model :** XSR205DU

Serial No. : B911363567 **ID No. :** ELABBALANCEN06

Capacity : 220 g **Resolution :** 0.00001g/81g, 0.0001g/220g

Environment : On site calibration was carried out at the B304 Balance Room, Envilab Co., Ltd.

Ambient Temperature : (24.6 to 24.9) °C

Relative Humidity : (57.0 to 67.8) %

Air Pressure : 1015.0 mbar

Date of Received : 01 March 2023

Date of Calibration : 01 March 2023

Date of Issue : 04 March 2023

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref: LAB 14

Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02222345	10 Nov 2023	National Institute of Metrology (Thailand), (NIMT)

Approved by :



(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

Certificate of Calibration

Certificate No. : 66-200066-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.1	0.00000	0.000014
0.5	0.00002	0.000022
1	0.00000	0.000026
2	0.00001	0.000034
5	-0.00001	0.000043
10	0.00000	0.000053
50	0.00004	0.00011
100	-0.0001	0.00020
150	-0.0001	0.00038
200	-0.0002	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.07$, providing a level of confidence of approximately 95%

Eccentric error Load test : 50 g

A	B	C	D	E	
0.00000	0.00000	0.00001	0.00001	0.00000	g



Repeatability Load test : 200 g

Stdev. : 0.000042 g

- o0o -

Handwritten signature



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 66-410024-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Digital Thermo-Hygrometer

Manufacturer : Jedto

Model : HTC-1

Range Temperature : N/A °C

Resolution : 0.1 °C

Range Humidity : N/A %R.H.

Resolution : 1 %R.H.

Serial No. : PONPE5852094

ID No. : ELABTMHTC10003

Environment : Ambient Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Date of Received : 08 March 2023

Date of Calibration : 09 March 2023

Date of Issue : 09 March 2023

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4013 by compared with standard probe sensor humidity/temperature into humidity/temperature chamber.

Reference Standard Instruments : This certification is traceable to the International System of Units

Digital Indicator with Standard Probe Temp&Hum

ID No.

Cert. No.

Due Date

Traceability

400034 & 400036 SG-H-00021/66

11 Jul 2023

Success Gateway Co., Ltd., Accredited by TISI Calibration No.0268

Approved by :

(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



รับรองสำเนาถูกต้อง

Calibratech Co.,Ltd. ผู้จัดการฝ่ายควบคุมคุณภาพ

Certificate of Calibration

Certificate No. : 66-410024-1

Page : 2 of 2

UUC Condition As-Received : Good

Result of Calibration : Without Adjustment

Function : Temperature measurement

Reference Humidity @ 50 %R.H.

Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25.01	25.0	0.0	0.46

Result of Calibration : Without Adjustment

Function : Humidity measurement

Reference Temperature @ 25 °C

Standard Humidity (%R.H.)	UUC Reading (%R.H.)	Correction (%R.H.)	Uncertainty (± %R.H.)
50.00	49	1	2.2

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐0๐ -

B



Certificate of Calibration

Certificate No. : 66-420018-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : pH Meter with electrode

pH meter

Manufacturer : Adwa

Model : AD 12

Range : -2.00 to 16.00 pH

Resolution : 0.01 pH

Serial No. : 11004090402

ID No. : ELABPHADWA1201

Environment : Ambient Temperature : $(25 \pm 2) ^\circ \text{C}$

Relative Humidity : $(50 \pm 15) \%$

Date of Received : 08 February 2023

Date of Calibration : 13 February 2023

Date of Issue : 13 February 2023

Calibrated by : Bunjerd Masri

Calibration Method : In-house method CAL-M4201 direct measurement by using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61235182	857394	11 Dec 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61267169	857395	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61260481	857396	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-420018-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
7,10	6.986	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

Remark

1 UUC : Unit Under Calibration

2 pH meter does not have voltage mode because the plug can not BNC socket

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐0๐ -

B





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 23TW79

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	Hanna
Model :	HI9146-04
Serial No. :	G00007931
ID No. :	ELABDOHI914601
Received Date :	17 March 2023
Test Date :	20 March 2023
Reference :	2303-0651DN-1
Submitted by :	Envilab Co.,Ltd (Head office) 540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae, Bangkok 10160
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean

Approved by :

Approved Signatory

- (/) Malee Butkruea
() Saithip Meangmai
() Warakorn Lerngagtrakul

Issue Date :

23 March 2023



B 0310344
รับรองสำเนาถูกต้อง

ผู้จัดการฝ่ายควบคุมคุณภาพ



Cert.No.: 23TW79

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: KC1A01TAF

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.14	8.16	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Malu



1154259

รับรองสำเนาถูกต้อง

Co., Ltd.

ผู้จัดการฝ่ายควบคุมคุณภาพ

Certificate of Calibration

Certificate No. : 65-400577-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Air Chamber (Refrigerator)

Manufacturer : M-LAB

Model : BIC-140

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 1011

ID No. : ELABBODC140N03

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (22.0 to 23.0) °C

Relative Humidity : (55 to 58) %

Line Voltage : (224.0 to 226.0) V

Date of Received : 11 November 2022

Date of Calibration : 11 November 2022

Date of Issue : 12 November 2022

Calibrated by : Bunjerd Masri

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400028	65-400522-3	03 Apr 2023	National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co., Ltd.



Certificate of Calibration

Certificate No. : 65-400577-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

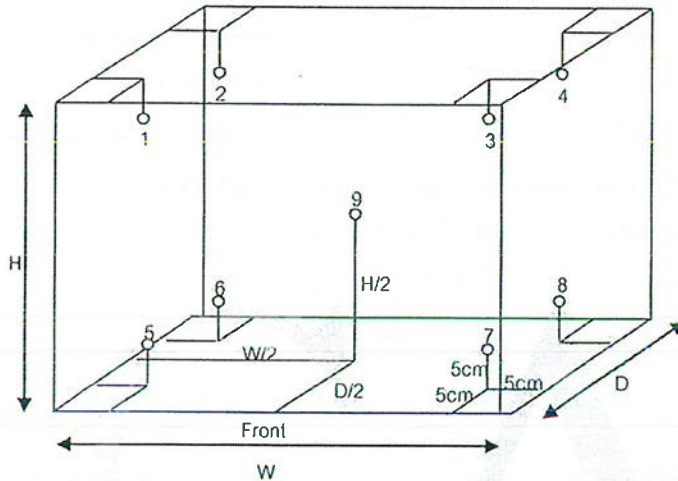

Inside of Chamber

W = 0.38 m

D = 0.35 m

H = 1.15 m

Capacity = 0.15 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
4.0	4.0	4.0	3.9	3.9	4.1	3.5	4.1	4.1	4.1	3.8	4.2	0.56

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
4.0	4.0	4.0	0.7	0.1	0.7

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -

B



Certificate of Calibration

Certificate No. : 66-400156-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Air Chamber (Oven)
Manufacturer : Memmert
Range : N/A °C
Serial No. : B319.0600
Model : UF 75
Resolution : 0.1 °C
ID No. : ELABHAOVEN0600

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (30.0 to 30.8) °C

Relative Humidity : (60 to 65) %

Line Voltage : (224.2 to 225.2) V

Date of Received : 23 March 2023

Date of Calibration : 23 March 2023

Date of Issue : 25 March 2023

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400030	65-400548-1	26 Apr 2023	National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

Certificate of Calibration

Certificate No. : 66-400156-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

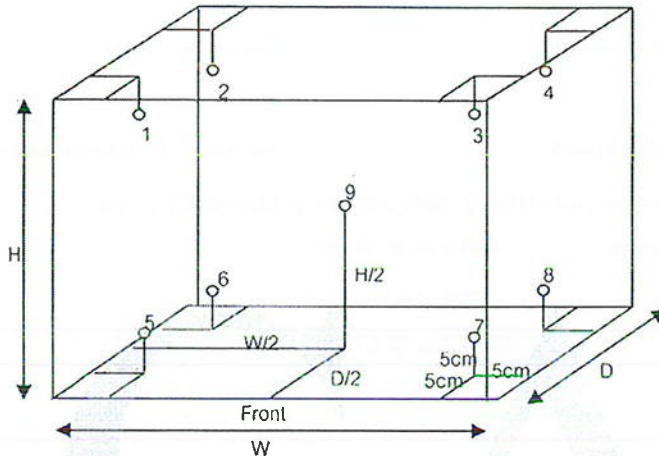

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.56 m

Capacity = 0.07 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104.0	103.5	103.5	104.3	104.3	104.3	104.2	104.3	104.1	103.7	104.0	104.3	0.70
110.0	109.5	109.5	110.3	110.3	110.3	110.3	110.3	110.1	109.7	110.0	110.3	0.71
180.0	179.0	179.0	179.4	180.1	180.3	180.1	180.6	179.9	179.2	179.6	180.4	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104.0	103.5	103.5	0.7	0.1	0.8
110.0	109.5	109.5	0.8	0.1	1.0
180.0	179.0	179.0	1.4	0.2	1.5

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

- o0o -

B



Certificate of Calibration

Certificate No. : 66-400056-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540,540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : Water Bath

Manufacturer : Memmert

Model : WNB29

Range : N/A °C

Resolution : 0.1 °C

Serial No. : L617.0156

ID No. : ELABWBWNB29N01

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (22.5 to 23.0) °C

Relative Humidity : (45 to 50) %

Line Voltage : (224.0 to 225.0)V

Date of Received : 02 February 2023

Date of Calibration : 02 February 2023

Date of Issue : 04 February 2023

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with RTD probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400031	65-400549-1	22 Apr 2023	National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

Certificate of Calibration


Certificate No. : 66-400056-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

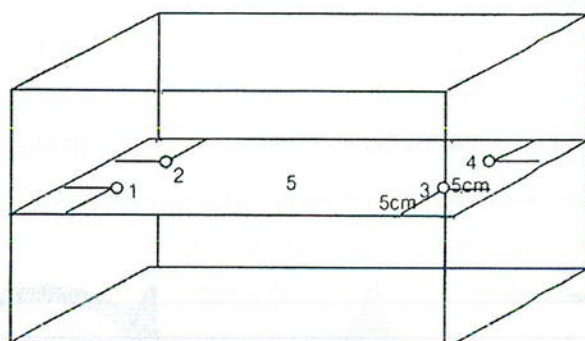

Front

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor					Uncertainty (± °C)	Measured Uniformity (°C)	Measured Stability (°C)
			No.							
			1	2	3	4	5			
95.0	95.0	95.0	95.41	95.41	95.68	95.62	95.57	0.22	0.33	0.10

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

B



Certificate of Calibration

Certificate No. : 66-300140-2

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkok 10160

Equipment : Cylinder

Manufacturer : PYREX

Class : A

Capacity : 50 ml

Graduation : 1 ml

ID No. : C-WW-003/23

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1009.9 mbar.

Date of Received : 15 March 2023

Date of Calibration : 20 March 2023

Date of Issue : 20 March 2023

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	65-200370-1	02 Jun 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :



(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-300140-2

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
30	29.98
50	50.12

Uncertainty of measurement with in \pm 0.054 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o O o -

D.



Certificate of Calibration

Certificate No. : 66-300140-6

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkok 10160

Equipment : Cylinder

Manufacturer : PYREX

Class : A

Capacity : 1000 ml

Graduation : 10 ml

ID No. : C-WW-006/23

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1009.9 mbar.

Date of Received : 15 March 2023

Date of Calibration : 20 March 2023

Date of Issue : 20 March 2023

Calibrated by : Areerat Sombun


Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	65-200370-1	02 Jun 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :



(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 66-300140-6

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
500	499.57
1000	999.89

Uncertainty of measurement with in \pm 0.17 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -

D.

