

ภาคผนวก ค : เอกสารสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 15 July, 2022

Certification No. 266/22

Page : 1 of 2

Object : Wireless Weather Station

Manufacturer : Davis Instruments Inc.

Type : Vantage Pro 2 Model No. 6152

Serial No. : BF211004031 ID No. : WIND-07

Customer : BPM ENVIRONMENT CO.,LTD.
124/208 Moo 2, Mahasawat, Bangkruay,
Nonthaburi 11130

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1004.6 hPa

NATIONAL STANDARD WIND TUNNEL :

: Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 266/22

15 July, 2022

Page : 2 of 2

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacumm	Velocity	Velocity	Correction
m/sec	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.9	0.10
7.00	-	-	-	6.7	0.30
9.02	-	-	-	8.9	0.12
11.01	-	-	-	10.7	0.31
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.8	0.21
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.8	0.22

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

TEMPERATURE DISPLAY CALIBRATION

Meter Console Information

Console Model : XC-572-V
 Console serial : A2011904
 Temp.Indicator Model : 765-KF
 Temp. Indicator Serial : JC17852

Calibration Conditions

Cal. Date : 17-Feb-23
 Issue Date : 17-Feb-23
 Cal. Report No. : WDS-SV660011
 Ambient Temp. (°C) : 25
 Pressure (mm Hg) : 758
 Humidity (%) : 55

Reference Equipment

Temp. Simulator Model : FLUKE 714B
 Serial No. : 60590035

Temperature Sensor Calibration

Reference Point	Ref. Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
1	-18.0	-17.0	1.0
2	38.0	38.0	0.0
3	93.0	94.0	-1.0
4	149.0	150.0	-1.0
5	260.0	259.0	1.0
6	371.0	372.0	-1.0
7	482.0	482.0	0.0
8	593.0	594.0	-1.0
9	816.0	816.0	0.0
10	1038.0	1038.0	0.0
Maximum ¹			1.0

PASS

Note

¹ For valid test results , the maximum difference between temperature readings should $\leq 1.0^{\circ}\text{C}$ (EPA Method 5, Section 6.1.1.8).
 Perform all TC Channel calibrations. Except meter (DGM) channel

DGM Out Temperature Sensor Calibration


Temperature point	Ref. Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
Ambient	25.0	25.2	-0.2
Heat	100.0	101.0	-1.0

Difference Rang

DGM Out Temp. Diff. $\pm 3^{\circ}\text{C}$

PASS

Approved By :



THERMOCOUPLE CALIBRATION

Thermocouple Informations

Console Model : XC-572-V
 Console serial : A2011904
 Thermocouple Type: K

Calibration Conditions

Cal. Date : 17-Feb-23
 Issue Date : 17-Feb-23
 Cal. Report No. : WDS-SV660011
 Ambient Temp. (°C) : 25
 Pressure (mm Hg) : 758
 Humidity (%) : 55

Reference Equipment

Temp Meter Model : Fluke 714B
 Serial No. : 60590035

Results			
Thermocouple Calibration			
Temperature Point	Reference Thermocouple Temperature	Thermocouple Temperature	Temperature difference
°C	°C	°C	°C
Stack Thermocouple for 3ft. Probe			
Ambient	25.0	25.6	-0.6
Heat	100	110	-10


Difference Range

Temp. Difference $\pm 2^\circ\text{F}$ or $\pm 16^\circ\text{C}$

Note

The temperatures of the thermocouple and reference thermometers shall agree to within $\pm 2^\circ\text{F}$. (EPA Method 5, section 10.5)

Approved



HEATER SYSTEM CALIBRATION

Heater Information

Console Model : XC-572-V
 Console serial : A2011904
 Tested heating equipment : Heated
 filter ovens
 Model : SB-2M-V
 Serial No. : 1903014
 Temp. Controller Model : 765-KF
 Temp. Controller Serial : JC17852

Calibration Conditions


Cal. Date : 17-Feb-23
 Issue Date : 17-Feb-23
 Cal. Report No. : WDS-SV660011
 Ambient Temp. (°C) : 25
 Pressure (mm Hg) : 758
 Humidity (%) : 0

Reference Equipment

Temp Meter Model: FLUKE 714B
 Serial No. : 60590035

Result				
Heat System	Control Acceptance °C	Reference Thermometer Temperature °C	Temperature Display °C	Temperature difference °C
Heated filter Ovens	120 °C±14 °C	120	116	4

Ap



HEATER SYSTEM CALIBRATION

Heater Information

Console Model : XC-572-V
 Console serial : A2011904
 Tested heating equipment : Heat tube
 Probe length : 3 ft.
 Probe Liner Material Type : Stainless
 Temp. Controller Model : 765-KF
 Temp. Controller Serial : JC17852

Calibration Conditions

Cal. Date : 17-Feb-23
 Issue Date : 17-Feb-23
 Cal. Report No. : WDS-SV660011
 Ambient Temp. (°C) : 25
 Pressure (mm Hg) : 758
 Humidity (%) : 55

Reference Equipment


Temp Meter Model: FLUKE 714B
 Serial No. : 60590035

Result				
Heat System	Control Acceptance °C	Reference Thermometer Temperature °C	Temperature Display °C	Temperature difference °C
Probe Heat System	120 °C±14 °C	120	115	5

Note

Heating system capable of maintaining a probe gas temperature during sampling of 120 ±14 °C (248 ±25 °F)
 (EPA Method 5 , section 6.1.1.2)

Approved



NOZZLE CALIBRATION

See the Code of Federal Regulations, Title 40, Part 60, Appendix A-3, Method5.

Nozzle Information

Console Model : XC-572-V
 Console serial : A2011904
 Material Type : Stainless

Calibration Conditions


Cal. Date : 17-Feb-23
 Issue Date : 17-Feb-23
 Cal. Report No. : WDS-SV660011
 Ambient Temp (°C) : 25
 Pressure (mm Hg) : 758
 Humidity (%) : 55

Reference Equipment

Measure Equipment : Digital Caliper
 Serial No. : A22222115

Calibration Data					Results	
Nozzle ID	Nozzle Diameter				Hi - Lo	$(D_1 + D_2 + D_3) / 3$
Sizes		D ₁	D ₂	D ₃	ΔD	Davg
	mm	mm	mm	mm	mm	mm
4	3.2	3.07	3.08	3.09	0.020	3.080
6	4.8	4.59	4.55	4.57	0.040	4.570
10	8.0	7.72	7.73	7.74	0.020	7.730
10(1)	8.0	7.53	7.60	7.52	0.080	7.550
12	9.5	9.47	9.49	9.51	0.040	9.490
14	11.1	10.77	10.81	10.84	0.070	10.807
16	12.7	12.81	12.75	12.82	0.070	12.793

D₁, D₂, D₃ = There difference nozzle diameters at 60 degrees to each other, each measured to the nearest 0.025 mm
 Hi-Lo ΔD = The difference between the high and low numbers shall not exceed <_0.100 mm
 Davg = $(D_1 + D_2 + D_3) / 3$

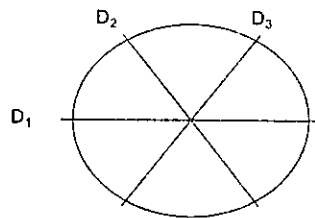


Result of physical: After checking the appearance of the nozzle, the nozzle is in normal condition.

Result of Calibration: After calibration the nozzle, we found that the size of the nozzle has changed.

Which can be seen from the new measured Davg value.

Recommendation: The size of the nozzle affects its use. Therefore, it is advisable to use a new size of the calibrated nozzle.

New Nozzle ID Size							
Size ID No.	4	6	10	10(1)	12	14	16
Diameter	3.08	4.57	7.73	7.55	9.49	10.81	12.79





WISDOM SCIENCE

FIELD AND SERVICE SUPPORT DIVISION

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m³)

Meter Console Information

Console Model :	XC-572-V
Console serial :	A2011904
DGM Model # :	SK25EX
DGM Serial # :	0009850
Calibration Date :	17-Feb-23
Issue Date :	17-Feb-23
Cal. Report No. :	WDS-SV660011
Ambient Temp (°C)	25
Pressure (mm Hg):	758
Relative Humidity (%) :	55

Calibration Condition

Std. Temp. (°C):	298
Std. Pressure (mm Hg):	760
K ₁ (K/mm Hg):	0.3857

Factors/Conversion

WTM Model:	W-NKoDa-5B	WTM Cal. Due Date:	Nov. 2022
WTM Serial:	600245	Gamma:	1.0000

Reference Equipment

UUT Meter (DGM)

Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial V _{ini}	Final V _{fin}	Initial t _{ini}	Final t _{fin}	Initial V _{ini}	Final V _{fin}	Initial t _{ini}	Final t _{fin}
15.00	13.0	2.1813	2.3546	26	26	7.84217	8.01256	25	25
10.00	25.0	2.3770	2.5400	26	26	8.03445	8.19433	25	25
8.00	50.0	2.5509	2.7288	26	26	8.20438	8.37905	25	25
7.00	80.0	2.7392	2.9366	26	26	8.38757	8.58216	25	25
5.00	120.0	2.8558	3.1285	26	26	8.59716	8.76783	25	25

Reference Meter (WTM)

Standardized Data

Test Meter	Reference Meter		Correction Factor		Flow Rate	
	Std. Volume V _{std} (m ³)	Std. Flow Rate Q _{std} (m ³ /min)	"Gamma" (Y)	Variation (ΔY)	Std & Corr Q _{std(corr)}	ΔH@ (mm H ₂ O) Variation ΔΔH _g
0.170	0.167	0.011	0.985	0.003	0.011	-0.983
0.160	0.157	0.016	0.982	0.000	0.016	-2.232
0.175	0.171	0.021	0.980	-0.001	0.021	1.265
0.194	0.191	0.027	0.981	0.000	0.027	0.914
0.171	0.167	0.033	0.980	-0.002	0.033	1.036
= Y Avg.					47.293	= ΔH@ Avg.


Calibration Results

Pass/Fail Result:

Pass

Note: For Calibration
Note: For ΔH_g or

Meter Gamma vs Flowrate

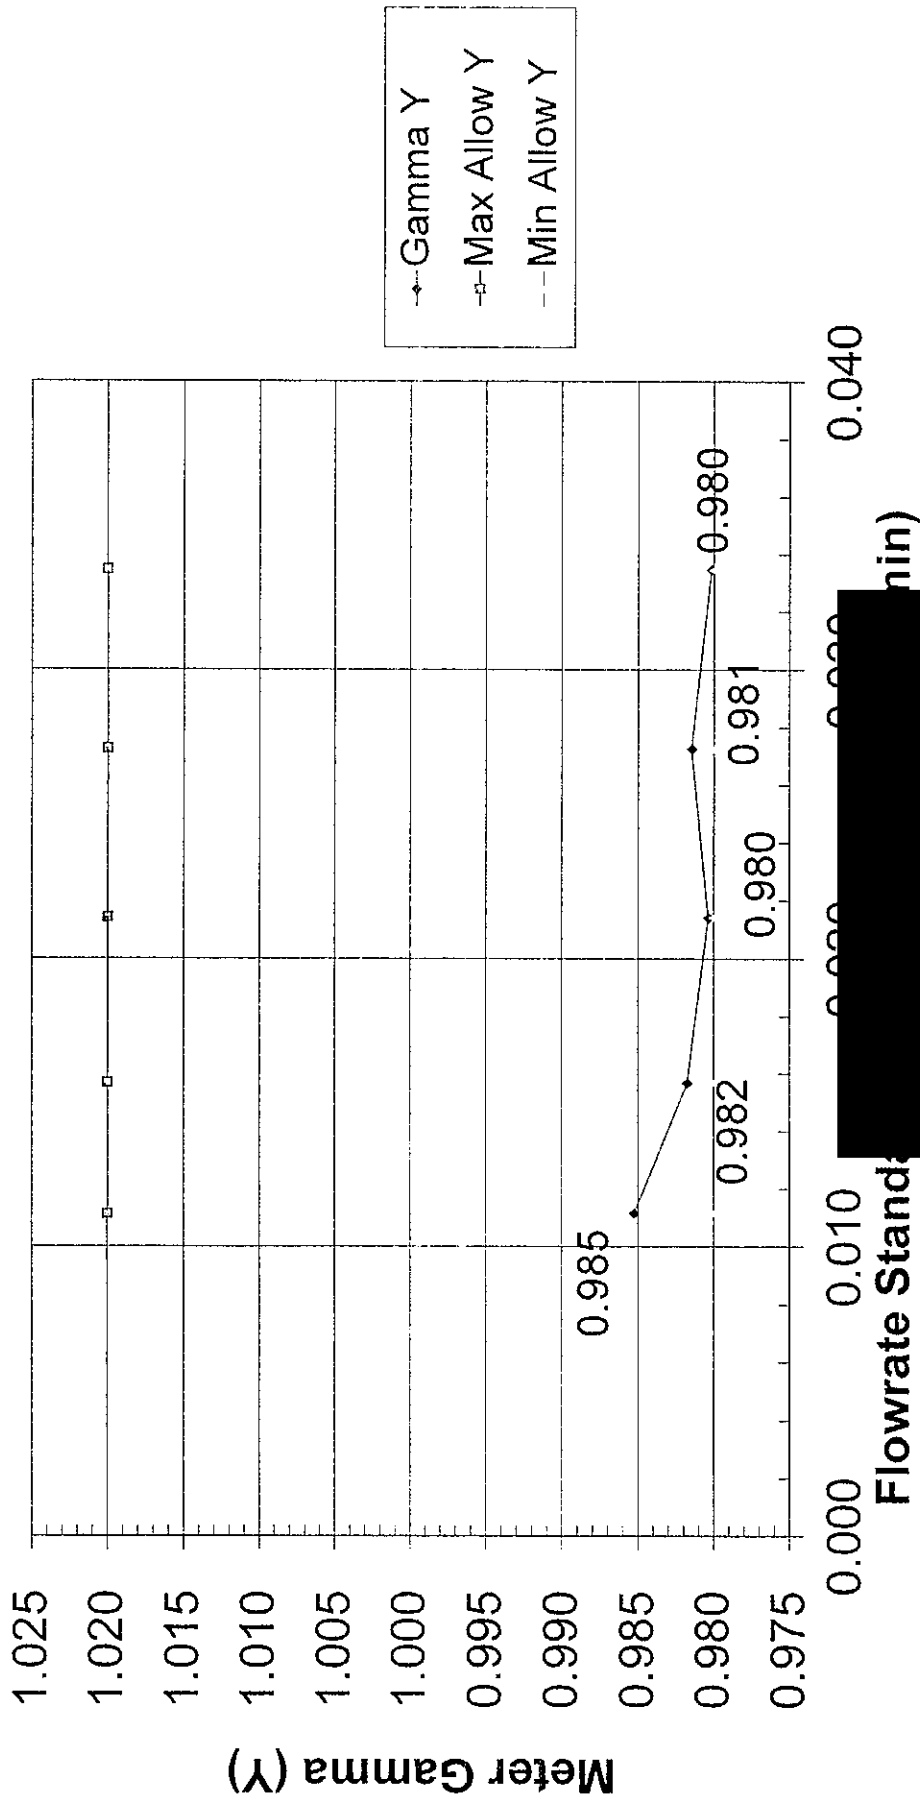


Console Serial:

A2011904

Console Model:

XC-572-V

Meter Pressure vs Flowrate

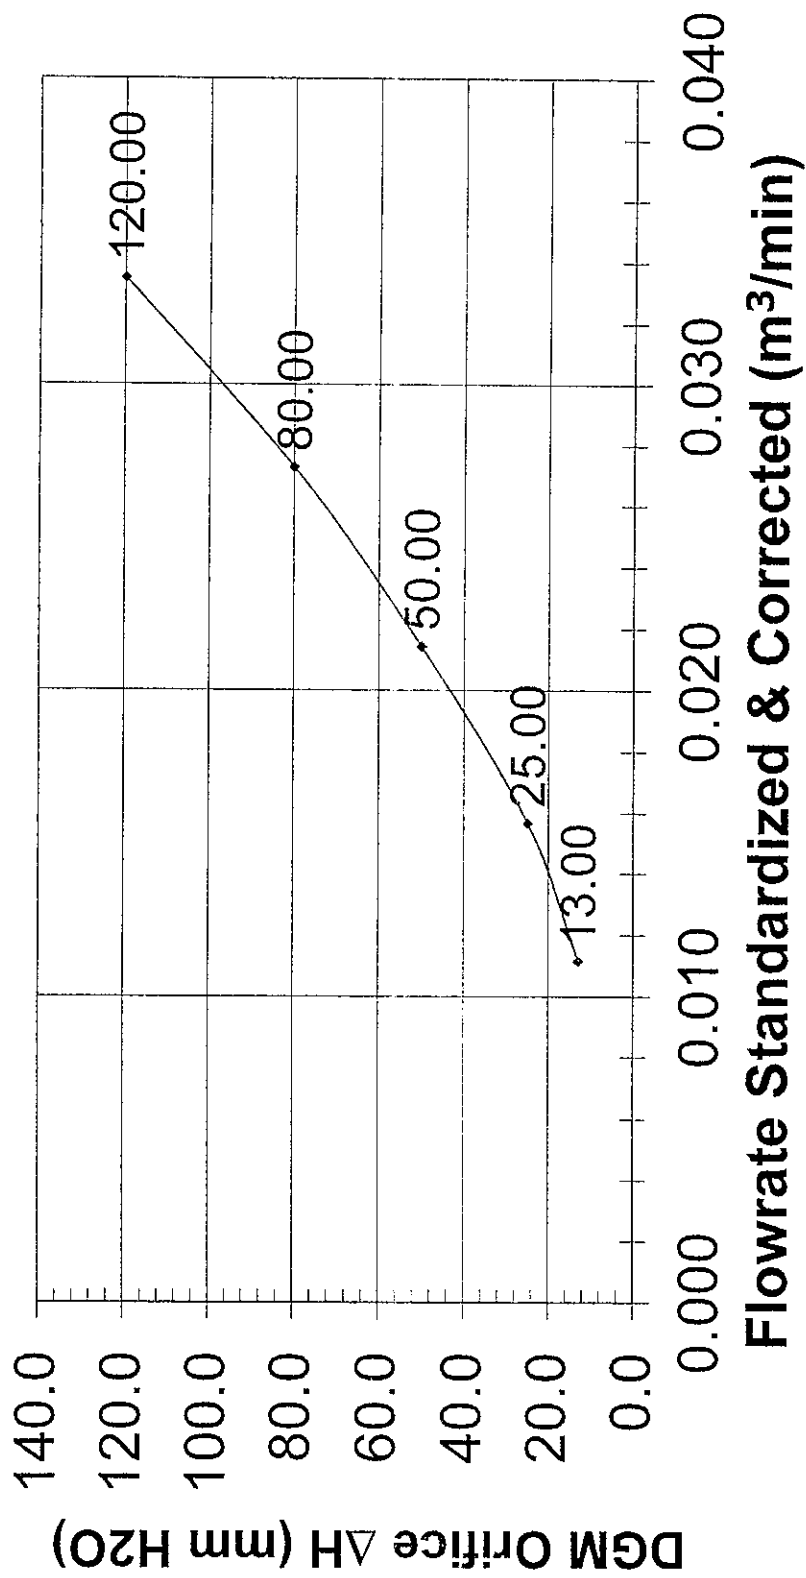

Console Serial:

A2011904

Console Model:

XC-572-V



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

Analyzer Performance Test

Calibrated Date: 08 November 2022

Instruments Information

Analyzer Type: NO/NO ₂ /NO _x Analyzer Model: 42C	Manufacturer: Thermo Environmental S/N: 42C-77282-385
---	--

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 55.47 PPM SO ₂ Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	393.3	400.0	-1.7
NO _x	0.1	0.0	0.1	400.0	400.0	0.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

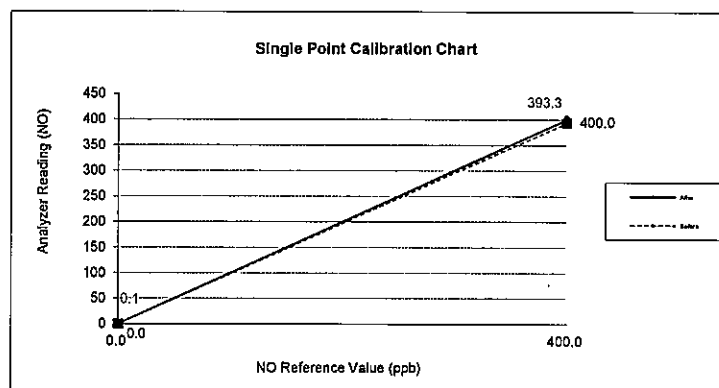



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

Analyzer Performance Test

Calibrated Date: 08 November 2022

Instruments Information

Analyzer Type: NO/NO ₂ /NO _x Analyzer Model: 42C	Manufacturer Thermo Environmental S/N: 42C-66375-352
---	---

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 55.47 PPM SO ₂ Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	393.4	400.0	-1.7
NO _x	0.1	0.0	0.1	398.7	400.0	-0.3

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

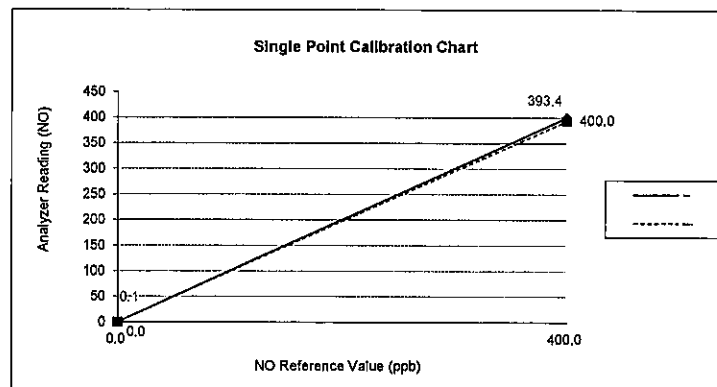



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

Analyzer Performance Test

Calibrated Date: 10 October 2022

Instruments Information

Analyzer Type: NO/NO ₂ /NO _x Analyzer Model: 42C	Manufacturer: Thermo Environmental S/N: 42C-78440-389
---	--

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 55.47 PPM SO ₂ Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	393.6	400.0	-1.6
NO _x	0.1	0.0	0.1	400.0	400.0	0.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

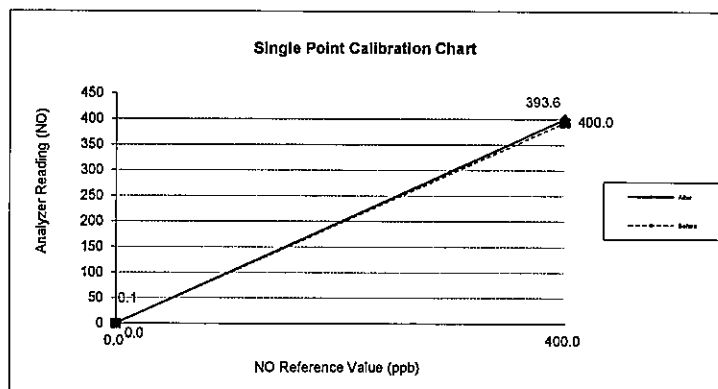



Certificate of Calibration

Certificate Number : SPR23030200-2

Page : 1 of 3

Customer : ENVI GREEN SOUTHERN CO.,LTD.

83/5 Moo.1 Kuan ru ,RattaPhum ,Songkhla 90180

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6239

Serial Number : 222179

ID. Number : No.7

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 13 Mar 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 17 Mar 2023

Location of Calibration : In-Lab

Recommend Due Date : 17 Mar 2024


Calibration Procedure : SP-CPE-04-01

Date of Issue : 18 Mar 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).





Calibration Report

Certificate Number : SPR23030200-2

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research

6769 km² (United Nations Population Data) (2007) 101 (62) 123-130 E 1997 www.elsevier.com/locate/jr

SP-FM-04-15 rev.0



Result of Calibration

Certificate No. : SPR23030200-2

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Result of Calibration

Certificate No. : SPR23030200-5

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.1	114.1	0.1	0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

~ End of Certificate ~



Certificate of Calibration

Certificate Number : SPR22090149-1

Page : 1 of 3

Customer : ENVI GREEN SOUTHERN CO.,LTD.

83/5 Moo.1 Kuan ru ,RattaPhum ,Songkhla 90180

Equipment Name : Sound Calibrator

Manufacturer : Extech

Model : 407744

Serial Number : H.397003

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23\text{ }^{\circ}\text{C} \pm 3\text{ }^{\circ}\text{C}$

Received Date : 08 Sep 2022

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 12 Sep 2022

Location of Calibration : In-Lab

Recommend Due Date : N/A

Calibration Procedure : In-House Method

Date of Issue : 13 Sep 2022

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).



Calibration Report

Certificate Number : SPR22090149-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2022

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR22090149-1

Page : 3 of 3

Function : Acoustic Test

UUC Setting		Standard Reading		Error		(±) Uncertainty	
Hz	dB	Hz	dB	Hz	dB	Hz	dB
1000	94	999.5	93.9	0.5	0.1	0.073	0.32

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



CERTIFICATE No : 23M2443
REFERENCE No : 68471-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SARTORIUS
MODEL : BSA224S-CW
SERIAL No : 36591842
ID No : BA 08/61
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATION DATE : 10-Mar-23

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 23M2443

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591842
ID No : BA 08/61 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23°C \pm 1°C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000058
0.1	0.1000	0.0000	0.000059
0.2	0.2000	0.0000	0.000059
0.5	0.5000	0.0000	0.000060
1.0	1.0000	0.0000	0.000060
2.0	2.0000	0.0000	0.000061
5.0	5.0000	0.0000	0.000063
10.0	10.0000	0.0000	0.000067
20.0	20.0001	-0.0001	0.000073
50.0	50.0000	0.0000	0.00011
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	99.9999
4	99.9998
5	100.0000
OFF-CENTER LOADING	0.0002

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com



CERTIFICATE No : 23M2442
REFERENCE No : 68471-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SARTORIUS
MODEL : BSA224S-CW
SERIAL No : 36591843
ID No : BA 09/61
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATION DATE : 10-Mar-23

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV 02



CERTIFICATE No : 23M2442

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591843
ID No : BA 09/61 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23° C \pm 1° C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000058
0.1	0.1000	0.0000	0.000059
0.2	0.2000	0.0000	0.000059
0.5	0.5000	0.0000	0.000060
1.0	1.0000	0.0000	0.000060
2.0	2.0000	0.0000	0.000061
5.0	5.0000	0.0000	0.000063
10.0	10.0000	0.0000	0.000067
20.0	20.0001	-0.0001	0.000073
50.0	50.0000	0.0000	0.00011
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	99.9999
3	99.9998
4	100.0001
5	100.0000
OFF-CENTER LOADING	0.0002

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 22T10972
REFERENCE No : 66837-1

PAGE : 1 OF 3

Certificate of Calibration

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
MODEL : DRB 200
SERIAL No : 15110C0497
ID No : DRB 04/59
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATION DATE : 20-Dec-22

ISSUED DATE : 20-Dec-22

RECEIVED DATE : 20-Dec-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02



CERTIFICATE No : 22T10972

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : DRB 04/59
RECEIVED DATE : 20-Dec-22
AMBIENT TEMPERATURE : 23° C ± 1° C
MODEL : DRB 200
SERIAL NUMBER : 15110C0497
CALIBRATION DATE : 20-Dec-22
RELATIVE HUMIDITY : 52 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT TEMPERATURE RECORDER WITH THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 15 POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE FOUR CORNERS OF THE REACTOR AND PLACED THE EIGHTH THERMOCOUPLE AT THE CENTER OF THE REACTOR.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	8009008	22T7511	10-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

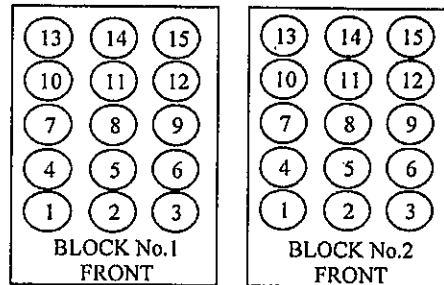

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	149.8
	2	149.6
	3	149.7
	4	149.8
	5	149.9
	6	149.8
	7	149.8
	8	149.8
	9	149.9
	10	149.8
	11	149.9
	12	149.7
	13	149.9
	14	149.9
	15	149.7
Uncertainty of Measurement(± °C)	0.86	0.86

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.
NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLYING COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.
END OF CALIBRATION REPORT

F-G01



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 22E9693
REFERENCE No : 66476-1

PAGE : 1 OF 3

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : HANNA
MODEL : HI 3512
SERIAL No : TH118035
ID No : pH 04/56
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATION DATE : 15-Sep-22

ISSUED DATE : 15-Sep-22

RECEIVED DATE : 14-Sep-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV 02



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22E9693

PAGE : 2 OF 3

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : HANNA
ID No : pH 04/56
RECEIVED DATE : 14-Sep-22
AMBIENT TEMPERATURE : 20 °C ± 1 °C
MODEL : HI 3512
SERIAL NUMBER : TH118035
CALIBRATION DATE : 15-Sep-22
RELATIVE HUMIDITY : 50 % RH ± 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No/ LOT No	CERTIFICATE No	DUE DATE
1) pH STANDARD SOLUTION	00651-06	CC719181	4880-12119147	05-Apr-23
2) pH STANDARD SOLUTION	00651-08	CC718727	4881-12110709	31-Mar-23
3) pH STANDARD SOLUTION	00651-10	CC717045	4882-12065386	17-Mar-23
4) PROCESS CALIBRATOR	CA150	91S6079	22E1145	31-Mar-23
5) BATH	260014	1247 48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
 - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : ADJUSTMENT

1. DISPLAY UNIT ONLY

SLOPE FACTOR $k = 2.303 RT/F = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.8	-0.69	-0.171	0.14	2.0
354.95	355.6	-0.65	0.860	0.14	2.0
295.80	296.4	-0.60	1.892	0.14	2.0
236.64	237.2	-0.56	2.922	0.14	2.0
177.48	178.0	-0.52	3.954	0.14	2.0
118.32	118.8	-0.48	4.985	0.14	2.0
59.16	59.7	-0.54	6.016	0.14	2.0
0.00	0.5	-0.50	7.049	0.14	2.0
-59.16	-58.8	-0.36	8.136	0.14	2.0
-118.32	-117.9	-0.42	9.223	0.14	2.0
-177.48	-177.1	-0.38	10.311	0.14	2.0
-236.64	-236.3	-0.34	11.399	0.14	2.0
-295.80	-295.5	-0.30	12.487	0.14	2.0
-354.95	-354.7	-0.25	13.575	0.14	2.0
-414.11	-413.9	-0.21	14.662	0.14	2.0

END OF CALIBRATION REPORT PAGE 2 OF 3

F-G010 REV 02



CERTIFICATE No : 22E9693

PAGE : 3 OF 3

Calibration Report

RESULT OF CALIBRATION (CONTINUE) :

2. DISPLAY UNIT WITH pH ELECTRODE S/N: 09081C6M

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (\pm pH)	COVERAGE FACTOR k
4.007	4.007	0.000	3.996	0.012	2.0
7.004	7.006	-0.002	6.944	0.012	2.0
10.016	10.012	0.004	10.194	0.014	2.0

3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING ($^{\circ}$ C)	UUC READING ($^{\circ}$ C)	CORRECTION ($^{\circ}$ C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (\pm $^{\circ}$ C)	COVERAGE FACTOR k
25.003	25.0	0.003	---	0.0085	2.0

4. PERCENT SLOPE 100%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : L202207235-001

Date Issued : 03-Aug-22

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment : Block Digestion (Gerhardt, TR)

Manufacturer : Gerhardt

Model : -

Serial No. : 4061832

ID No./Tag No. : KJ 01/43

Date Received : 02-Aug-22

Date Calibrated : 03-Aug-22

Calibrated by : Mr. Nirot Parnkamnoed

Calibration Method or Calibration Procedure Used


In-house method : CP-49 base on TLAS G-20 by comparing against Standard Thermometer.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.



Certificate No. : L202207235-001

Environment : Ambient Temperature : $(25 \pm 2)^{\circ}\text{C}$
Relative Humidity : $(50 \pm 15)\%\text{RH}$

ด้านซ้าย

Calibration Temperature ($^{\circ}\text{C}$)	Setting Temperature ($^{\circ}\text{C}$)	Indicating Temperature ($^{\circ}\text{C}$)	Measured Stability ¹ ($^{\circ}\text{C}$)	Measured Uniformity ² ($^{\circ}\text{C}$)	Overall Variation ³ ($^{\circ}\text{C}$)
380	380	380	1.45	0.57	4.01

Calibration Temperature ($^{\circ}\text{C}$)	Standard Reading ($^{\circ}\text{C}$), Probe No. 9 is Reference Probe					Uncertainty ⁴ ($\pm^{\circ}\text{C}$)
380	No. 1	No. 2	No. 3	No. 4	No. 5	2.2
	377.86	378.11	378.69	378.54	378.72	
	No. 6	No. 7	No. 8	No. 9	No. 10	
	378.09	378.07	377.93	378.17	377.61	

Without adjustment

No. 1	No. 2		
No. 3	No. 4		
No. 5	No. 6		
No. 7	No. 8		
No. 9	No. 10		

Top view position

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. AD2202-055-0002 for Digital Thermometer with Probe (Agilent) Module 2 (172) Type K Serial No. US37011204, Due 11-Aug-22

- Notes :
1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.
 2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.
 3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.
 4. The uncertainty of measurement is included temperature stability.

Certificate No. : L202207235-001

Environment : Ambient Temperature : $(25 \pm 2)^{\circ}\text{C}$
Relative Humidity : $(50 \pm 15)\%\text{RH}$

ด้านขวา

Calibration Temperature ($^{\circ}\text{C}$)	Setting Temperature ($^{\circ}\text{C}$)	Indicating Temperature ($^{\circ}\text{C}$)	Measured Stability ¹ ($^{\circ}\text{C}$)	Measured Uniformity ² ($^{\circ}\text{C}$)	Overall Variation ³ ($^{\circ}\text{C}$)
380	380	380	1.45	0.94	4.40

Calibration Temperature ($^{\circ}\text{C}$)	Standard Reading ($^{\circ}\text{C}$), Probe No. 9 is Reference Probe					Uncertainty ⁴ ($\pm^{\circ}\text{C}$)
380	No. 1	No. 2	No. 3	No. 4	No. 5	2.2
	378.91	379.16	378.76	378.60	378.78	
	No. 6	No. 7	No. 8	No. 9	No. 10	
	378.15	378.13	378.00	378.23	377.67	

Without adjustment

		No. 1	No. 2
		No. 3	No. 4
		No. 5	No. 6
		No. 7	No. 8
		No. 9	No. 10

Top view position

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. AD2202-055-0002 for Digital Thermometer with Probe (Agilent) Module 2 (172) Type K Serial No. US37011204, Due 11-Aug-22

- Notes :
1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.
 2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.
 3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.
 4. The uncertainty of measurement is included temperature stability.

End of Certificate

Page 3 of 3



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR




NOMENCLATURE : OVEN
MANUFACTURER : BINDER
MODEL / TYPE : FD53
SERIAL NO. : 08-51541[OV 03/51]
CLID. NO. : 332200143
JOB CONTROL NO. : 230125008183

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 25 January 2023

DATE OF ISSUED : 22 February 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23008183

F3-011-04/01-12

page 1 of 4



@clccalibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : OVEN
MANUFACTURER : BINDER
MODEL / TYPE : FD53
SERIAL NO. : 08-51541[OV 03/51]
LOCATION SITE : WET CHEMISTRY LABORATORY III
DATE OF CALIBRATION : 16 February 2023

ENVIRONMENT CONDITIONS :

Temperature : 29 °C to 31 °C

Relative Humidity : 54% to 58 %

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPTH-07 based on TLAS G-20 as calibration guidelines.

The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2620 S/N. 5592550.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q22066550, Due Date 07 July 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23008183

F3-011-04/01-12

page 2 of 4



@clccalibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring oven.

CALIBRATION DATA

1. OVEN PERFORMANCE

DUC		Measured Uniformity (°C)	Measured Stability (°C)	Measured Overall Variation (°C)
Setting (°C)	Indicating (°C)			
104	104	1.2	0.2	1.7
180	180	2.0	0.3	3.6

Certificate No. Q23008183

F3-011-04/01-12

page 3 of 4



@clccalibration


CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

DUC		Measured Temperature (°C)@Probe No.9 is Ref.									Uncertainty $\pm (^\circ\text{C})$	Coverage factor k
Setting (°C)	Indicating (°C)	1	2	3	4	5	6	7	8	9		
104	104	104.1	105.1	104.5	104.7	104.2	104.8	105.4	105.5	104.4	0.8	2,00
180	180	179.6	182.4	180.3	180.5	180.1	181.4	182.9	182.5	181.5	1.0	2,00

Technical Note : W = 40 cm, D = 34 cm, H = 40 cm.

The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 48 of 54

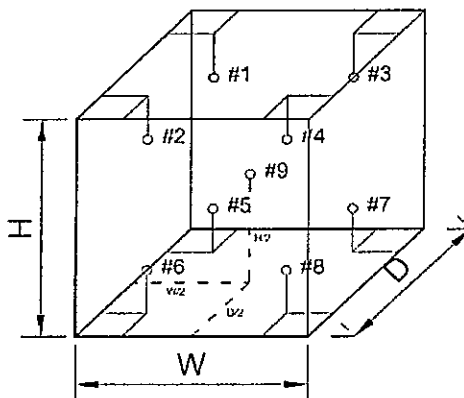

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23008183

F3-011-04/01-12

page 4 of 4



@clccalibration



Harikul Science Co.,Ltd.
 694 Soi Ratchadanivet 24, Pracharatbamphen,
 Samsaennok, Huaikhwang, Bangkok 10310
 Tel: 0-2274-2456 Fax: 0-2274-2443
 Email: info@harikul.com www.harikul.com

CERT.No.: HS-U017D

Certificate of Calibration

Calibration Date : 3 Apr 23	Model : YSI 5000
Submitted by : S.P.S CONSULTING SERVICE CO.,LTD	S/N : 15B100751
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,	Probe : YSI 5010
Chatuchak, Bangkok, Thailand 10900	S/N : 22D100097
	ID NO. : -
Avg Room Temp : 20 °C	Air Temp ref : S/N. E00522
Avg Water Temp : 20 °C	Barometric ref : S/N. E00522
Air Pressure : 760.00 mmHg	Water Temp ref : S/N. 11431
Salinity : 0 ppt	
	Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-	-
Measurement 2 (mg/l)	9.08	(PASS)	-	-
Measurement 3 (mg/l)	9.08	(PASS)	-	-
Measurement 4 (mg/l)	9.08	(PASS)	-	-
Measurement 5 (mg/l)	9.08	(PASS)	-	-
Measurement 6 (mg/l)	9.08	(PASS)	-	-
Measurement 7 (mg/l)	9.08	(PASS)	-	-
Measurement 8 (mg/l)	9.08	(PASS)	-	-
Measurement 9 (mg/l)	9.08	(PASS)	-	-
Measurement 10 (mg/l)	9.08	(PASS)	-	-
Mean Measurement	9.08	mg/l	-	-
Inaccuracy	0.01	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.