

ภาคผนวก ค : เอกสารสอบสวนเทียบความถูกต้อง
ของเครื่องมือเก็บตัวอย่าง

ANALYTICAL BALANCE (DU)

Model. : XS205DU

Serial No. : 1126323724



Certificate No. : 23-006683
Sample Code : 23-02820-006

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : 1126323724

ID No. : LABE 05/1

Date of Receipt : 20 January 2023

Date of Calibration : 20 January 2023

Calibrated by : Mr. Thanadol Pholthep
Scientist

Issue date : 25 January 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)



Certificate No. : 23-006683
Sample Code : 23-02820-006

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : METTLER TOLEDO
Model : XS205DU
Capacity : Max 81 g / 220 g
Resolution : 0.01 mg / 0.1 mg
Serial No. : 1126323724
ID No. : LABE 05/1

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 80	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
<input checked="" type="checkbox"/> No adjustment	Nominal value	40	30
<input type="checkbox"/> Adjustment	Standard weight	40.000042	30.000045
	Average reading of indicator	40.000015	30.000019
	Standard deviation	0.000004	0.000007

Unit : g	Range : 200	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
<input checked="" type="checkbox"/> No adjustment	Nominal value	100	200
<input type="checkbox"/> Adjustment	Standard weight	100.000022	200.000199
	Average reading of indicator	100.00001	200.00004
	Standard deviation	0.000004	0.000008

NSC-TISI-TIS17025
CALIBRATION 0152

Page 3 of 4

Certificate No. : 23-006683
Sample Code : 23-02820-006

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable,

Unit : g

Range : 80

Test Point	Sensitivity, S
0	0.99800
40	0.99800
80	0.99800

Range : 200

Test Point	Sensitivity, S
0	0.9980
100	0.9980
200	0.9980

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.00000	0.00000	0.0000090	2.01
0.01	0.0100036	0.01000	0.00000	0.0000093	2.01
0.1	0.1000062	0.10000	0.00001	0.000012	2.00
1	1.0000036	1.00001	-0.00001	0.000014	2.00
5	5.0000044	5.00003	-0.00003	0.000020	2.00
10	10.0000000	10.00007	-0.00007	0.000032	2.00
20	20.0000016	20.00011	-0.00009	0.000036	2.00
50	50.0000029	50.00013	-0.00010	0.000067	2.00
100	100.0000022	100.0001	-0.0001	0.00016	2.00
150	150.0000051	150.0001	0.0000	0.00023	2.00
200	200.0000199	200.0003	-0.0001	0.00028	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

NSC-TISI-TIS17025
CALIBRATION 0152

Page 4 of 4

Certificate No. : 23-006683
Sample Code : 23-02820-006

REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-center loading

Deviation of the measurement value through off-center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.


☐ Circle☐ Triangular☒ Rectangular

Weighing pan

Test weight : 50 and 100

Unit : g

Range	80	200
Position	Reading of indicator	Reading of indicator
1	50.00014	100.0001
2	50.00014	99.9998
3	50.00006	100.0000
4	50.00010	100.0001
5	50.00017	100.0001
6	50.00014	100.0001
Maximum difference	0.00008	0.0003

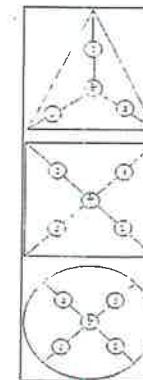

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at :-

- Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument	Class	ID No.	Certificate No.	Due Date
1) STANDARD WEIGHT 1 mg to 1 kg	E2	LB-WE-57	22-060633	27 Jun 2023

6. Ambient conditions	Min	Max
Temperature (°C)	21.3	22.4
Relative Humidity (%Rh)	38.2	40.4
Air pressure (hPa)	1008.4	1010.1

- End of Report -

BAROMETER

Equipment : Analog Barometer

ID No. / Tag No. : BM001/41



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 http://www.mit.in.th



CALIBRATION CERTIFICATE

Certificate No. : AD2205-163-0001

Date Issued : 20-May-22

Customer : Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11 Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment : Analog Barometer

Manufacturer : Barigo

Model : -

Serial No. : -

ID No./Tag No. : BM001/41

Date Received : 12-May-22

Date Calibrated : 20-May-22

Calibrated by : Mr. Saruth Srichutikul

Calibration Method or Calibration Procedure Used

In-house method : CP-21 base on DKD-R 6-1: Edition 3 2014.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k=2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: K. Nathong
(Mr. Nathapong Krudaum)



Page 1 of 2

Certificate No : AD2205-163-0001

Environment Ambient Temperature : $(25 \pm 2)^\circ\text{C}$
Relative Humidity : $(50 \pm 15)\%\text{RH}$

STD Reading hPa	UUC Reading (hPa) Before Adjusted	UUC Reading (hPa) After Adjusted	UUC Error hPa	Uncertainty \pm hPa
990.00	990.0	-	0.00	0.59
1000.00	1000.0	-	0.00	0.59
1010.00	1010.0	-	0.00	0.59
1020.00	1020.0	-	0.00	0.59
1030.00	1030.0	-	0.00	0.59

STD = Standard

UUC = Unit Under Calibration

Calibrated condition : Pressure Medium Air : Density = 1.19 kg/m^3 @ 20°C , 1 bar
Mounting Position Vertical
Reference Level at center of its dial

Description of UUC : Range 955 - 1075 hPa Absolute
Calibration Range 990 - 1030 hPa Absolute
Scale Interval 1 hPa
Resolution 0.5 hPa Absolute

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

iRPC Certificate No. CL1-P210086 for Reference Pressure Monitor Serial No. 1598, Due 08-Nov-22

End of Certificate



Page 2 of 2

Hot Air Oven

Model : UFE 500

Serial No. : G511.0182



Page 1 of 3

CERTIFICATE OF CALIBRATION

Certificate No. : 23-006679
Sample Code : 23-02820-002

NSC-TISI-TIS17025
CALIBRATION 0152

Page 2 of 3

REPORT OF CALIBRATION

Certificate No. : 23-006679

Sample Code : 23-02820-002

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Memmert

Serial No. : G511.0182

Date of Receipt : 20 January 2023

Model : UFE 500

ID No. : LABE 17/4

Date of Calibration : 20 January 2023

Condition of Calibration

- | | | | |
|----------------|---------------------------|-------------------|-------------------|
| 1. Environment | 1.1 Ambient temperature | Maximum 27.9 °C | Minimum 25.3 °C |
| | 1.2 Relative humidity | Maximum 50.9 % | Minimum 38.5 % |
| | 1.3 Line voltage supplied | Maximum 221.9 VAC | Minimum 218.5 VAC |

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-P1100)	LB-DA-11 (RTD-138 to RTD-146)	22-040309	21 April 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Sarawoot Thammo
Scientist

Approved by

Issue date

24 January 2023

The uncertainties are for a confidence probability of approximately 95%.
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be used for any other purpose without the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

CONTACT@AMARC.CO.TH

Results of Calibration

Resolution : 0.5 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 ^{Ref}		
104	103.5	103.5	104.10	104.08	103.87	103.99	104.08	104.08	103.96	104.01	103.84	0.47	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
104.0	0.08	0.32	0.39

Notes

UUC* = Unit Under Calibration

REPORT OF CALIBRATION

Certificate No. : 23-006679

Sample Code : 23-02820-002

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 56 cm ; D = 40 cm ; H = 48 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

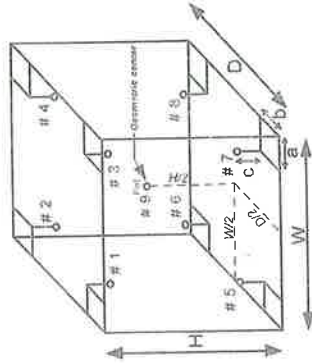


Figure: Example of sensor
installation Positions

- End of Report -

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

ORIFICE TRANSFER STANDARD CERTIFICATION

WORKSHEET TE-5025A

ROOTSMETER S/N 0438320

ORIFICE TRANSFER STANDARD CERTIFICATION WORKSHEET TE-5025A

Date - Mar 24, 2016 Rootmeter S/N 0438320 Ta (K) - 295
Operator Tisch Orifice I.D. - 0136 Pa (mm) - 742.95

PLATE OR Run #	VOLUME START (m3)	VOLUME STOP (m3)	DIFF VOLUME (m3)	DIFF TIME (min)	METER DIFF Hg (mm)	ORIFICE DIFF H2O (in.)
1	NA	NA	1.00	1.3400	3.2	2.00
2	NA	NA	1.00	0.9510	6.3	4.00
3	NA	NA	1.00	0.8510	7.8	5.00
4	NA	NA	1.00	0.8130	8.6	5.50
5	NA	NA	1.00	0.6690	12.6	8.00

9-10

DATA TABULATION

Vstd	(x axis) Qstd	(y axis)	Va	(x axis) Qa	(y axis)
0.9832	0.7337	1.4054	0.9957	0.7430	0.8911
0.9791	1.0296	1.9875	0.9915	1.0426	1.2603
0.9770	1.1481	2.2221	0.9894	1.1626	1.4090
0.9760	1.2006	2.3305	0.9884	1.2157	1.4778
0.9707	1.4510	2.8107	0.9830	1.4694	1.7823

Qstd slope (m)	= 1.96262				
intercept (b)	= -0.03249				
coefficient (r)	= 0.99993				

y axis = SQRT[H2O(Pa/760) (298/Ta)]					

y axis = SQRT[H2O(Ta/Pa)]					

CALCULATIONS

Vstd = Diff. Vol [(Pa-Diff. Hg) / 760] (298/Ta)
Qstd = Vstd/Time

Va = Diff Vol [(Pa-Diff Hg) / Pa]
Qa = Va/Time

For subsequent flow rate calculations:

Qstd = 1/m{ [SQRT(H2O(Pa/760) (298/Ta))] - b}
Qa = 1/m{ [SQRT H2O(Ta/Pa)] - b}

THERMO-HYGROMETER

Model : 608-H1

Serial No. : 45106737



CERTIFICATE OF CALIBRATION

Page 1 of 2
Certificate No. : 22-068062
Sample Code : 22-24591-002

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhaphan 8 Rd., Nongkham,
Sriacha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration laboratory)

Equipment : Digital thermo-hygrometer

Manufacturer : testo Model : 608-H1

Serial No. : 45106737 ID No. : LABE 09/7

Date of Receipt : 22 June 2022 Date of Calibration : 24 June 2022

Condition of Calibration

1. Environment
 - 1.1 Ambient temperature : 23.0 °C ± 3.0 °C
 - 1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

- 2.1 In-house method: WI-CL-045 By comparison with thermometer standard / chilled mirror hygrometer in controlled chamber.
- 2.2 The calibration by comparison unit under calibration (UUC) to the thermometer standard / chilled mirror hygrometer in a chamber at the controlled temperature / relative humidity.

3. Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Chilled Mirror	Optidew Vision	LB-DP-01 & LB-DP-01 (DP)	TH-0014-22	16 February 2023
3.2 Digital Thermometer	Optidew Vision	LB-DP-01 & LB-DP-01 (Temp.)	22-029549	14 March 2023
3.3 Digital Thermometer	34972A	LB-DA-07 with RTD-89	21-072473	13 September 2022

4. This certificate is traceable to the international system of unit (SI Unit).

- 4.1 Instrument No. 3.1 through National Institute of Metrology (Thailand).
- 4.2 Instrument No. 3.2 and 3.3 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Miss Pornsuda Lohabal Scientist Approved by :
Issue date : 27 June 2022

The uncertainties are for a confidence probability of approximately 95%.
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.
This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has been approved by the Thai Ministry of Commerce.
Laboratory and its traceability is recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory.
reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
PM CL 114
TEL 02-516-2422
FAX 02-516-6949
Rev 01
CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date 15/10/21



REPORT OF CALIBRATION

Page 2 of 2
Certificate No. : 22-068062
Sample Code : 22-24591-002

Results of Calibration

Temperature measurement

Resolution : 0.1 °C
Range : 0 °C to 50 °C

Calibration point °C	Average of standard reading		Unit under calibration		Expanded uncertainty °C
	Controlled humidity %RH	Temperature °C	Average reading °C	Correction value °C	
20	50	20.00	20.2	- 0.20	± 0.39
25	50	25.00	24.9	+ 0.10	± 0.39
30	50	30.00	29.8	+ 0.20	± 0.39

Humidity measurement

Resolution : 0.1 %RH
Range : 10 %RH to 95 %RH

Calibration point %RH	Average of standard reading		Unit under calibration		Expanded uncertainty %RH
	Air temperature °C	Calculated humidity %RH	Average reading %RH	Correction value %RH	
45	25.00	45.13	51.4	+ 6.27	± 1.3
60	25.00	60.03	66.5	+ 6.47	± 1.5
75	25.00	75.20	81.5	+ 6.30	± 1.7

Notes

- Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with ISO 17025.

• End of Report •

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
TEL 02-516-2422
FAX 02-516-6949
Rev 09
CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date 15/10/21

SOUND LEVEL CALIBRATOR

MODEL : NC-75

SERIAL No. : 34802645

Request No. 21-66/0021 MTC No. EEL. BP. 35/1065

CALIBRATION CERTIFICATE

Submitted by : Eastern Thai Consulting 1992 Co.,Ltd.
Address : 683 Moo 11 Sukaphibul Rd., Nongkham, Sriracha, Chonburi 20230.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator
Manufacturer : Rion
Model : NC-75
Serial No. : 34802645

Ambient Environment

Temperature : (23 ± 3) °C
Relative Humidity : (50 ± 15) %
Ambient Pressure : (101.325 ± 1.500) kPa

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.

7. Condenser Microphone B&K 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was

measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 10 Oct. 2022

Date of Calibration : 18 Oct. 2022

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumba@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

Request No. 21-66/0021 MTC No. EEL. BP. 35/1065

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit
1/2 inch Brüel&Kjær 4180	93.98	-0.02	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit
1/2 inch Brüel&Kjær 4180	1000.0	0.0	± 1.5	±1.0%

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit
1/2 inch Brüel&Kjær 4180	0.30	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by



Date of Calibration : 18 Oct. 2022

Date of Issue : 19 Oct. 2022

End of Certificate

The results relate only to the items tested/calibrated and the results except in full are prohibited unless written permission is obtained from TISTR.

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumba@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 00230994



NSC-TISI-TIS 17025
CALIBRATION 0037



NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

MTC No. EEL. BP. 156/0266

Request No. 21-66/0343

CALIBRATION CERTIFICATE

Submitted by : Eastern Thai Consulting 1992 Co., Ltd..
Address : 683 Moo 11 Sukhaphani 8 Rd., Nongkham, Sriracha, Chonburi 20230.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$
Ambient Pressure : $(101.325 \pm 1.5) \text{ kPa}$

Instrument Calibrated :

Description : Sound Level Meter
Manufacturer : Rion
Model : NL-52A
Serial No. : 00230994
Microphone : Type UC-59 No.22777
Preamplifier : Type NH-25 No.22430

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 27 Feb. 2023

Date of Calibration : 21-23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned by the Laboratory. The results except in full are prohibited unless written permission is obtained from the Laboratory of TISTR

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the Laboratory of TISTR

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 109
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0343

MTC No. EEL. BP. 156/0266

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
11. Digital Multimeter Agilent 34401A S/N MY44005560.
12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 21-23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned by the Laboratory. The results except in full are prohibited unless written permission is obtained from the Laboratory of TISTR

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the Laboratory of TISTR

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 109
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
113.89	114.1	113.9	0.0	0.7	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 123.7 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
20.5	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	10.5	0.10	N/A
C-Weight	14.8	0.10	N/A
Flat	20.4	0.10	N/A

Date of Calibration : 21-23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from TISTR.

FM.BL.MTC.002 R

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax (66) 0 2577 9009
E-mail : rumoal@tistr.or.th Website: www.tistr.or.th

Office/Laboratory
Sol 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 1 (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.0	0.1	0.0	±1.0	0.45	0.6
1 000	-0.5	-0.5	-0.5	±0.7	0.45	0.6
8 000	0.0	0.0	-0.1	+1.5; -2.5	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 1 (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	-0.1	-0.1	0.0	±1.0	0.20	0.5
125	0.1	0.0	0.0	±1.0	0.20	0.5
250	-0.1	0.0	0.0	±1.0	0.20	0.5
500	0.0	0.0	0.0	±1.0	0.20	0.5
1 000	0.0	0.0	0.0	±0.7	0.20	0.5
2 000	0.0	0.0	0.0	±1.0	0.20	0.5
4 000	0.0	0.0	0.0	±1.0	0.20	0.5
8 000	0.0	0.0	0.0	+1.5; -2.5	0.20	0.7
16 000	-1.3	-1.4	0.0	+2.5; -16.0	0.20	0.7

Date of Calibration : 21-23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from TISTR.

FM.BL.MTC.002 Rev.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax (66) 0 2577 9009
E-mail : rumoal@tistr.or.th Website: www.tistr.or.th

Office/Laboratory
Sol 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.1	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
137	137.1	0.1	0.8	0.30	0.3
136	136.1	0.1	0.8	0.30	0.3
135	135.1	0.1	0.8	0.30	0.3
134	134.1	0.1	0.8	0.30	0.3
133	133.1	0.1	0.8	0.30	0.3
132	132.0	0.0	0.8	0.30	0.3
131	131.1	0.1	0.8	0.30	0.3
130	130.1	0.1	0.8	0.30	0.3
129	129.1	0.1	0.8	0.30	0.3
124	124.0	0.0	0.8	0.30	0.3
119	119.0	0.0	0.8	0.30	0.3
114	114.0	0.0	0.8	0.30	0.3
109	109.0	0.0	0.8	0.30	0.3
104	104.0	0.0	0.8	0.30	0.3
99	99.0	0.0	0.8	0.30	0.3
94	94.0	0.0	0.8	0.30	0.3
89	89.0	0.0	0.8	0.30	0.3
84	84.0	0.0	0.8	0.30	0.3
79	79.1	0.1	0.8	0.30	0.3

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
74	74.1	0.1	0.8	0.30	0.3
69	69.0	0.0	0.8	0.30	0.3
64	64.0	0.0	0.8	0.30	0.3
59	59.0	0.0	0.8	0.30	0.3
54	53.9	-0.1	0.8	0.30	0.3
49	49.0	0.0	0.8	0.30	0.3
44	44.0	0.0	0.8	0.30	0.3
39	39.0	0.0	0.8	0.30	0.3
34	34.0	0.0	0.8	0.30	0.3
29	29.0	0.0	0.8	0.30	0.3
28	28.0	0.0	0.8	0.30	0.3
27	27.0	0.0	0.8	0.30	0.3
26	25.9	-0.1	0.8	0.30	0.3
25	24.9	-0.1	0.8	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	0.8	0.00	0.3

Date of Calibration : 21-23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpal@tistr.or.th Website: www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mt@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	35	35.0	0.0	0.8	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	±0.5	0.20	0.3
	2	108.9	-0.1	+1.0; -1.5	0.20	0.3
	0.25	99.9	-0.1	+1.0; -2.0	0.20	0.3
Slow	200	119.6	0.0	±0.5	0.20	0.3
	2	100.0	0.0	+1.0; -2.0	0.20	0.3
	200	120.0	0.0	±0.5	0.20	0.3
SEL	2	100.0	0.0	+1.0; -1.5	0.20	0.3
	0.25	90.8	-0.2	+1.0; -2.0	0.20	0.3

Date of Calibration : 21-23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpal@tistr.or.th Website: www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mt@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

MTC No. EEL. BP. 156/0266

Request No. 21-66/0343

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.4	0.0	2.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	1.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	1.0	0.20	0.35

11. Overload indication

Measured value (dB)	Deviated value (dB)		Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Positive one-half cycle	Negative one-half cycle			
136.5		136.5	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.1	0.10	0.1
End	129.0				

Calibrated by *Pannasit R.*

(Mr. Pannasit Phasingrui)

Approved by:

(Mr. Prawale Klomypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 21-23 Mar. 2023

Date of Issue : 23 Mar. 2023

Ref : 20112

End of Certificate

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the Institute.

FM.BL.MTC.002 Re

Lead Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,

Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : tunc@tistr.or.th Website: www.tistr.or.th

Office/Laboratory

Soi 1C, Bangsiao Industrial Estate, Sukhumvit Road,

Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak Bangkok 1090

Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 00230987



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0343

MTC No. EEL BP. 150/0266

CALIBRATION CERTIFICATE

Submitted by

Address

Calibrated at

Instrument Calibrated :

Description

Manufacturer

Model

Serial No.

Microphone

Preamplifier

Standards used :

: Eastern Thai Consulting 1992 Co., Ltd.

: 683 Moo 11, Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi, 20230

: Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.5) \text{ kPa}$

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.

2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.

3. Decade Attenuator Ando AL-205 S/N 00464602.

4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.

5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.

6. Digital Multimeter Fluke 8520A S/N 4985007.

7. Pistonphone Rion NC-72 S/N 00402446.

8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 27 Feb. 2023

Date of Calibration : 23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office

15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang

Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax (66) 0 2577 9009

E-mail : rumalai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,

Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phanomyothin Road, Chatuchak Bangkok 10900,

Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0343

MTC No. EEL BP. 150/0266

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.

10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.

11. Digital Multimeter Agilent 34401A S/N MY44005560.

12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office

15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang

Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax (66) 0 2577 9009

E-mail : rumalai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,

Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phanomyothin Road, Chatuchak Bangkok 10900,

Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation	Acceptance	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
113.92	114.0	113.9	0.0	0.7	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 113.8 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
16.4	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	10.7	0.10	N/A
C-Weight	14.9	0.10	N/A
Flat	20.6	0.10	N/A

Date of Calibration : 23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : nimmakitr@tistr.or.th, Web: www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mt@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response curve (dB)		Acceptance limit class I (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight			
125	0.6	0.6	±1.0	0.45	0.6
1 000	-0.4	-0.3	±0.7	0.45	0.6
8 000	0.7	0.6	+1.5 ; -2.5	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response curve (dB)		Acceptance limit class I (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight			
63	-0.1	0.0	±1.0	0.20	0.6
125	-0.1	0.1	±1.0	0.20	0.6
250	-0.1	0.1	±1.0	0.20	0.6
500	0.0	0.1	±1.0	0.20	0.6
1 000	0.0	0.0	±0.7	0.20	0.6
2 000	0.0	0.0	±1.0	0.20	0.6
4 000	0.0	0.0	±1.0	0.20	0.6
8 000	0.0	0.1	+1.5 ; -2.5	0.20	0.7
16 000	0.0	0.0	+2.5 ; -16.0	0.20	1.0

Date of Calibration : 23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : nimmakitr@tistr.or.th, Web: www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mt@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

5. Long-term stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class I (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.1	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class I (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class I (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rurnalee@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class I (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
135	134.2	-0.8	0.8	0.30	0.3
134	133.3	-0.7	0.8	0.30	0.3
133	132.5	-0.5	0.8	0.30	0.3
132	131.6	-0.4	0.8	0.30	0.3
131	130.6	-0.4	0.8	0.30	0.3
130	129.7	-0.3	0.8	0.30	0.3
129	128.8	-0.2	0.8	0.30	0.3
124	123.9	-0.1	0.8	0.30	0.3
119	119.0	0.0	0.8	0.30	0.3
114	114.0	0.0	0.8	0.30	0.3
109	109.0	0.0	0.8	0.30	0.3
104	104.0	0.0	0.8	0.30	0.3
99	99.0	0.0	0.8	0.30	0.3
94	94.0	0.0	0.8	0.30	0.3
89	89.1	0.1	0.8	0.30	0.3
84	84.0	0.0	0.8	0.30	0.3
79	79.0	0.0	0.8	0.30	0.3
74	74.0	0.0	0.8	0.30	0.3

Date of Calibration : 23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rurnalee@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class I (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
69	69.0	0.0	0.8	0.30	0.3
64	63.9	-0.1	0.8	0.30	0.3
59	59.0	0.0	0.8	0.30	0.3
54	53.9	-0.1	0.8	0.30	0.3
49	49.0	0.0	0.8	0.30	0.3
44	43.9	-0.1	0.8	0.30	0.3
39	38.9	-0.1	0.8	0.30	0.3
34	33.9	-0.1	0.8	0.30	0.3
29	29.0	0.0	0.8	0.30	0.3
28	28.0	0.0	0.8	0.30	0.3
27	27.0	0.0	0.8	0.30	0.3
26	26.0	0.0	0.8	0.30	0.3
25	25.0	0.0	0.8	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class I (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	0.8	0.30	0.3

Date of Calibration : 23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class I (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	35	35.0	0.0	0.8	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, T _b (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class I (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	+0.5	0.20	0.3
	2	109.0	0.0	+1.0, -1.5	0.20	0.3
	0.25	99.9	-0.1	+1.0, -3.0	0.20	0.3
Slow	200	119.6	0.0	±0.5	0.20	0.3
	2	100.0	0.0	+1.0, -3.0	0.20	0.3
	200	120.0	0.0	±0.5	0.20	0.3
SEL	2	100.0	0.0	+1.0, -1.5	0.20	0.3
	0.25	91.0	0.0	+1.0, -3.0	0.20	0.3

Date of Calibration : 23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : mtc@tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtr@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

Request No. 21-66/0343

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class I (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Complete cycle	125.4	125.4	0.0	2.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	1.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	1.0	0.20	0.35

11. Overload indication


Measured value (dB)		Deviated value (dB)	Acceptance limit class I (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Positive one-half cycle	Negative one-half cycle				
136.5	136.5	0.0	1.5	0.20	0.25

๑-26

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class I (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Begin	129.0	0.0	0.1	0.10	0.1
End	129.0				

Calibrated by



Approved by



Date of Calibration : 23 Mar. 2023
Date of Issue : 23 Mar. 2023

End of Certificate

The results relate only to the items tested/calibrated and the results of the tests are prohibited unless otherwise stated.

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 00230988

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0343

MTC No. EEL. BP. 151/0266

CALIBRATION CERTIFICATE

Submitted by : Eastern Thai Consulting 1992 Co., Ltd.
Address : 683 Moo 11, Sukhapirom 8 Rd., Nongkham, Sriracha, Chonburi, 20230
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :
Description : Sound Level Meter : $(23 \pm 3) ^\circ\text{C}$
Manufacturer : Rion : $(50 \pm 15) \%$
Model : NL-52A : $(101.325 \pm 1.5) \text{ kPa}$
Serial No. : 00230988
Microphone : UC-59 No.22332
Preamplifier : NH-25 No.22424

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 27 Feb. 2023

Date of Calibration : 24 Mar. 2023

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is granted by TISTR.

The results relate only to the items tested/calibrated or value assigned.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumalee@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumalee@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.6

Page 1 / 9

Request No. 21-66/0343

MTC No. EEL. BP. 151/0266

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation	Acceptance	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
	Before adjust	After adjust				
113.93	114.0	113.9	0.0	0.7	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 113.8 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
16.4	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency	Measured value (dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Weighting			
A-Weight	10.5	0.10	N/A
C-Weight	14.8	0.10	N/A
Flat	20.4	0.10	N/A

Date of Calibration : 24 Mar. 2023

The results relate only to the items tested/calibrated or value assigned
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Sol 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5223, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.4

Request No. 21-66/0343

MTC No. EEL. BP. 151/0266

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response curve (dB)		Acceptance limit class I (dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
	A-weight	C-weight			
125	0.4	0.6	Flat	0.5	0.6
1 300	-0.3	-0.4	± 1.0	0.45	0.6
8 300	0.2	0.4	± 0.7	0.45	0.6
			$\pm 1.5 ; -2.5$	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response curve (dB)		Acceptance limit class I (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
	A-weight	C-weight			
53	-0.6	0.1	Flat	0.0	0.6
125	-0.1	0.1	± 1.0	0.20	0.6
250	-0.1	0.1	± 1.0	0.20	0.6
500	-0.1	0.1	± 1.0	0.20	0.6
1 000	0.0	0.0	± 1.0	0.20	0.6
2 000	0.0	0.0	± 1.0	0.20	0.6
4 000	0.0	0.0	± 1.0	0.20	0.6
8 000	0.0	0.1	$\pm 1.5 ; -2.5$	0.20	0.7
16 000	0.1	0.0	$\pm 2.5 ; -16.0$	0.20	1.0

Date of Calibration : 24 Mar. 2023

The results relate only to the items tested/calibrated or value assigned
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Sol 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5223, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.4

5. Long-term stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.1	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 24 Mar. 2023

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Re

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sumalee@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
137	137.1	0.1	0.8	0.30	0.3
136	136.2	0.2	0.8	0.30	0.3
135	135.1	0.1	0.8	0.30	0.3
134	134.0	0.0	0.8	0.30	0.3
133	133.0	0.0	0.8	0.30	0.3
132	132.0	0.0	0.8	0.30	0.3
131	131.0	0.0	0.8	0.30	0.3
130	130.0	0.0	0.8	0.30	0.3
129	129.0	0.0	0.8	0.30	0.3
124	124.0	0.0	0.8	0.30	0.3
119	119.0	0.0	0.8	0.30	0.3
114	114.0	0.0	0.8	0.30	0.3
109	109.0	0.0	0.8	0.30	0.3
104	104.0	0.0	0.8	0.30	0.3
99	99.0	0.0	0.8	0.30	0.3
94	94.0	0.0	0.8	0.30	0.3
89	89.0	0.0	0.8	0.30	0.3
84	84.0	0.0	0.8	0.30	0.3
79	79.0	0.0	0.8	0.30	0.3
74	74.0	0.0	0.8	0.30	0.3

Date of Calibration : 24 Mar. 2023

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sumalee@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
69	69.0	0.0	0.8	0.30	0.3
64	63.9	-0.1	0.8	0.30	0.3
59	59.0	0.0	0.8	0.30	0.3
54	53.9	-0.1	0.8	0.30	0.3
49	49.0	0.0	0.8	0.30	0.3
44	43.9	-0.1	0.8	0.30	0.3
39	38.9	-0.1	0.8	0.30	0.3
34	33.9	-0.1	0.8	0.30	0.3
29	29.0	0.0	0.8	0.30	0.3
28	28.0	0.0	0.8	0.30	0.3
27	27.0	0.0	0.8	0.30	0.3
26	26.0	0.0	0.8	0.30	0.3
25	24.9	-0.1	0.8	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	0.8	0.30	0.3

Date of Calibration : 24 Mar. 2023

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is granted.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.4

8. Level linearity including the level range control.

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	35	35.0	0.0	0.8	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb(ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	±0.5	0.20	0.3
	2	108.9	-0.1	+1.0; -1.5	0.20	0.3
	0.25	99.8	-0.2	+1.0; -3.0	0.20	0.3
Slow	200	119.5	-0.1	±0.5	0.20	0.3
	2	99.9	-0.1	+1.0; -3.0	0.20	0.3
	200	119.9	-0.1	±0.5	0.20	0.3
SEL	2	99.9	-0.1	+1.0; -1.5	0.20	0.3
	0.25	90.9	-0.1	+1.0; -3.0	0.20	0.3

Date of Calibration : 24 Mar. 2023

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is granted.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.4

NSC-TISI-TIS 17025
CALIBRATION 0037

MTC No. EEL. BP. 151/0266

MTC No. EEL. BP. 151/0266

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class I (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Complete cycle	125.4	125.4	0.0	2.0	0.20	0.35
Positive half cycle	124.4	124.2	-0.2	1.0	0.20	0.35
Negative half cycle	124.4	124.2	-0.2	1.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
136.5	136.5	0.0	1.5	0.20	0.25

12. High-level stability

12. Flight-level stability					
Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.1	0.10	0.1
End	129.0				

Approved by :

Date of Calibration : 24 Mar. 2023

Date of Issue : 24 Mar. 2023

End of Certificate

The results relate only to the items tested/calibrated or value assessed. The results of the tests are not to be used for any other purpose without the written permission of the government of TSTR.

FM.BLMTC.002 Re'

<p>Head Office 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand Tel. (66) 0 2577 9000 Fax. (66) 0 2577 9009</p>	<p>Office/Laboratory 351 C, Bangsoe Industrial Estate, Sukhumvit Road, Amphoe Bangsoe, Changwat Samutprakan 10280, Thailand Tel. (66) 0 2323 1672-80 ext. 115, 116 Tel. (66) 0 2323 1672-80 ext. 115, 116</p>	<p>Office 196 Phahonyothin Road, Chatuchak, Bangkok 1090 Thailand Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217 Fax. (66) 0 2579 8592 E-mail: sumalee@nist.or.th</p>
---	--	---

ATOMIC ABSORPTION SPECTROPHOTOMETER

Model : PinAAcle 900F

Serial No. : PFBS22080801



PerkinElmer
For the Better

PER-INSTALLATION CHECKS:


- ☒ Verify that proper ventilation is installed and an adequate exhaust rate is accordance to PYL CFM N/A
- ☒ Verify that the gasses meet out PYL specifications---
- ☒ Verify that gas pressure regulators are installed with proper filters and pressure are set in accordance to PYL.
- ☒ Verify that the wiring in the lab meets our power and noise requirements specified in PYL.
- ☒ Verify that the lab environment conditions (room temperature, relative humidity) meet in our PYL specification
- ☒ Maintenance accessibility is adequate.
- ☒ Measured Mains Input Voltage under load is adequate per our PYL specifications (≥ 208 VAC)

PHYSICAL INSTALLATION:

- ☒ The instrument, cooling system, computer and any accessories are uncrated and installed on suitable bench
- ☒ Install all the electrical connections.
- ☒ Connect the gas hoses and tank regulators, set required pressures, and leak test as required.
- ☒ Install the burner System components. (PinAAcle Series 900T & 900F)
- ☒ Mount and connect the auto sample.
- ☒ Fill and connect the cooling system or connect external cooling according to specifications.
- ☒ Setup the computer and printer. Interconnect all cables between the computer, printer, and instrument.
- ☒ Setup and configure the computer to the instrument and install the software according to the installation chapter in the PinAAcle Service Manual.
- ☒ Record the furnace head voltage and manual temperature of 1200 Degrees Celsius.

INSTALLATION TESTING:

- ☒ Perform the following instrument performance tests according to the Installation and Test procedure.
Complete the Instrument Performance Test Data Sheet below.
 - PinAAcle900T, 900H & 900F
Flame Copper Sensitivity and Precision
 - PinAAcle900T & 900Z
Furnace Copper Characteristic Mass and Zeeman Ratio
 - PinAAcle900H
Furnace Chromium Characteristic Mass and Precision
- ☒ Make and electronic copy of the Instrument parameters file per SDB 900PIN_021 procedure on the customer computer



PerkinElmer
For the Better

PinAAcle 900 Series 900T, 900H, 900Z & 900F

Installation Checklist

Customer : EASTERN THAI CONSULTING
NONGKHAM, SIRACHA
CHONBURI 20230
Date Tested: 28-Nov-2022

CRM # _____ CSE: Pattayut Wanwongka

UPON SITE ARRIVAL:

- ☒ Verify that the instrument was not damaged during shipment
- ☒ Unpack the PC and all other accessories. Record the following:

PinAAcle Instrument Model:	PinAAcle 900F	S/N	PFBS22080801
Auto Sample Model:	N/A	S/N	-
Computer Model:	DELL	S/N	37024013667
Cooling System Model:	N/A	S/N	-
Printer Model:	N/A	S/N	-
Misc.	FIAS 100	S/N	100S22081101

- ☒ Record the software and firmware revision below:
 - Syngistix Software for AA Version: 5.0.1.2029
 - PinAAcle Spectrometer Firmware Version: 1.5.0.0126
 - PinAAcle Furnace Firmware Version: N/A
- ☒ Check the model specific Shipping Kit packed separately for completeness.
Verify the shipping Kit with each instrument order includes all items listed.



CUSTOMER ORIENTATION:

- ☒
- Refer to the Customer Orientation Script for details
- ☒
- Explain the warranty and customer replaceable parts policy
- ☒
- Inform the customer of relevant PerkinElmer training courses, websites, and phone number

PinAAcle 900 Series 900T, 900H, 900Z & 900F

Installation Performance Test Data Sheet

Flame Sensitivity and Precision
(PinAAcle Series 900T, 900H & 900F)

With Stainless Steel Nebulizer

Sensitivity	Mean Absorbance ≥ 0.250	N/A
Precision	%RSD ≤ 0.30 %	N/A

With High Sensitivity Nebulizer

Sensitivity	Mean Absorbance ≥ 0.250 Abs.	0.3759
Precision	%RSD ≤ 0.40 %	0.25 %

THGA Furnace Copper Characteristic Mass and Zeeman Ratio
(PinAAcle 900T & 900Z)

Copper Characteristic Mass

Characteristic Mass	14 ± 2.5 pg	N/A
Zeeman Ratio	0.52 ± 0.04	N/A
Precision	%RSD ≤ 2.0 %	N/A %
A.C Voltage measurement under load (Atomization)	≥ 208 VAC	231 VAC

HGA Furnace Chromium Characteristic Mass and Precision
(PinAAcle 900H)

Chromium Characteristic Mass

Characteristic Mass	3 ± 0.8 pg	N/A
Precision	≤ 2.0 %	N/A
A.C Voltage measurement under load (Atomization)	≥ 207 VAC	N/A



9. Mn Resolution Peak to Valley Ratio

HCL Sample Intensity (Valley) / HCL Sample Intensity (Peak) < 0.40 (40%) N/A
HCL Reference Intensity (Valley) / HCL Reference Intensity (Peak) < 0.40 (40%) N/A
Furnace Mode (900Z)
HCL Sample Intensity (Valley) / HCL Sample Intensity (Peak) < 0.40 (40%) N/A

10. Furnace and Baffles Alignment Check w/ Cu (900T/Z/H)

PK Area - AA < 0.005 A-s N/A
PK Area - BG < 0.005 A-s N/A

11. Furnace auto sample check valve test (900T/Z/H)

Places sample probe onto rinse alignment and for 2 minutes and watch for backwards flow of rinse solution
Does rinse solution go backward? Y/N N/A

Optional Test Check

[Flame only Verification - 900T/H/F]

12. Gas box calibration check default flow settings

Fuel flow N/A 20-22
Oxidant flow N/A around 43
Nebulizer Pressure N/A 29-29.5

[Furnace only Verification] *Note test 13&14 should be done simultaneously

13. Voltage drop*

2300C Atomization test N/A spec < 16 volts

14. Cr heating rate* : By design the ASCOM PS will output the right DC voltage regardless of the incoming voltage, so that is not the purpose of this test. We are using this to check the conductivity of the furnace head and the function of the pyrometer.

10ppb Cr standard @ 2300C Peak Height/Peak Area N/A > 1.3



PinaAcle 900 Added Installation Test Checklist:

Model: PinaAcle 900T Serial Number: PFBS22080801
Software Version: 5.0.1.2029 Spectrometer FW Version: 1.5.0.0126
Furnace FW Version: N/A
Instrument Control PCB revision: 3

NOTE: First 12 test checks are mandatory

1. 0.2, 0.7 & 2.0 Sifts and 8 Lamp turret position calibration.

Check ☒

2. Cu energy & Capacitance:

Cu 324.75nm Line:Energy can vary by model and configuration, but Capacitance should be > 7pF.

Capacitance= 7.0 pF

3. Wavelength Calibration Passed (As, Cu, Ba, K < 6 steps)

Yes ☒
No ☐

4. Wavelength Accuracy Check

AS 193.70 nm +/- 0.12 nm (193.58-193.82) 193.7 nm
Cu 324.75 nm +/- 0.12 nm (324.63-324.87) 324.7 nm
Ba 553.55 nm +/- 0.12 nm (553.43-553.67) 553.5 nm
K 766.49 nm +/- 0.12 nm (766.37-766.61) 766.5 nm

5. HCL Sample to HCL Reference Ratio with Cu #

30:70 N/A HCL = 0.43, spec 0.18-0.58, target 0.34-0.52
30:70 N/A D2 spec = 1.0-4.3
50:50 0.85 HCL = 1.0, spec 0.42-1.35, target 0.90-1.15
50:50 0.97 D2 spec = 0.43-1.84

6. Monochromator Bleed cover with Cu: Must be done with drak current checked (on) #

Sample beam blocked value 19 spec <60 counts, ideally <20
Reference beam blocked value (900TH) N/A spec <60 counts, ideally <20

7. Cu Flame Double-Beam Check #

Mean_15 mA - Mean_10 mA =< 0.004C 0.0024

8. Low UV Energy & Capacitance check: check on on all

Cu 216.5 nm 1.0 >= 1 pF Energy = 85 below 50 may be a problem
*Pb 217.0 nm N/A >= 1 pF Energy = N/A below 50 may be a problem
*Zn 213.0 nm N/A >= 1 pF Energy = N/A below 50 may be a problem

* Option tests

N/A for PinaAcle 900Z. Flame double-beam ode test

Comments:

PerkinElmer Service Engineer Signature:  Date: 28-11-22

Patrayut Wanwongka



ANALYTICAL BALANCE

Model. : SECURA224-1S

Serial No. : 0036707137

Certificate No. : 23-006682
Sample Code : 23-02820-005

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : SARTORIUS
Model : SECURA224-IS
Capacity : Max 220 g
Resolution : 0.0001 g
Serial No. : 0036707137
ID No. : LABE 05/2

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 220	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
<input checked="" type="checkbox"/> No adjustment	Nominal value	100	200
<input type="checkbox"/> Adjustment	Standard weight	100.000022	200.000199
	Average reading of indicator	99.9998	199.9999
	Standard deviation	0.00007	0.00007
Unit : -	Range : -	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
<input type="checkbox"/> No adjustment	Nominal value	*	*
<input type="checkbox"/> Adjustment	Standard weight	*	*
	Average reading of indicator	*	*
	Standard deviation	*	*

Certificate No. : 23-006682
Sample Code : 23-02820-005

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhaphan 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : SARTORIUS

Model : SECURA224-IS

Serial No. : 0036707137

ID No. : LABE 05/2

Date of Receipt : 20 January 2023

Date of Calibration : 20 January 2023

Calibrated by : Mr. Thanadol Pholthep
Scientist

Issue date : 25 January 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Board (TLAB) to the national standards laboratory and its traceability to recognized national standards and to the unit of measurement capability of the laboratory. This certificate may not be reproduced other than in full except with the prior written permission of the Laboratory and Research Center Public Company Limited (AMARC).

Certificate No. : 23-006682
Sample Code : 23-02820-005

Page 3 of 4

Certificate No. : 23-006682
Sample Code : 23-02820-005

Page 4 of 4

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range	Test Point	Sensitivity, S	Test Point	Sensitivity, S
220	0	0.9980		
	100	0.9980		
	200	0.9980		

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.0000	0.0000	0.00011	2.04
0.01	0.0100036	0.0100	0.0000	0.00011	2.04
0.1	0.1000062	0.1000	0.0000	0.00011	2.04
1	1.0000036	1.0000	0.0000	0.00011	2.04
2	2.0000128	2.0000	0.0000	0.00011	2.04
5	5.0000044	5.0000	0.0000	0.00011	2.04
10	10.0000000	10.0000	0.0000	0.00011	2.03
20	20.0000016	20.0000	0.0000	0.00012	2.03
50	50.0000029	50.0000	0.0000	0.00013	2.02
100	100.0000022	99.9998	0.0002	0.00017	2.01
200	200.0000199	200.0000	0.0002	0.00028	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty U is stated as the standard uncertainty distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty U is stated as the standard uncertainty distribution corresponds to a coverage probability of approximately 95%.

REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Range	Position	Reading of Indicator	Reading of Indicator
220	1	99.9998	
	2	100.0001	
	3	99.9997	
	4	99.9998	
	5	99.9998	
	6	99.9998	
Maximum difference		0.0003	

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : -

- Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument

1) STANDARD WEIGHT 1 mg to 1 kg

Class


E2

Certificate No.

22-060639

Due Date

27 June 2023

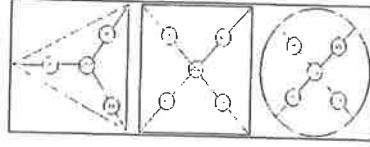

Ambient conditions	Min	Max
Temperature (°C)	21.2	22.5
Relative Humidity (%RH)	37.1	44.3
Air pressure (hPa)	102.1	1013.0

- End of Report -

AUTOCLAVE

Model : FLS-1000

Serial No. : 55169083



CERTIFICATE OF CALIBRATION

Page 1 of 2

Certificate No. : 22-102070
Sample Code : 22-37024-003

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Autoclave Room)

Equipment : Autoclave

Manufacturer : TOMY

Model : FLS-1000

Serial No. : 55169083

ID No. : LABE 43/2

Date of Receipt : 19 September 2022

Date of Calibration : 19 September 2022

Condition of Calibration

1. **Environment**
- 1.1 Ambient temperature : Maximum 30.3 °C ; Minimum 28.8 °C
- 1.2 Relative humidity : Maximum 56.1 % ; Minimum 45.1 %
- 1.3 Line voltage supplied : Maximum 227.3 VAC ; Minimum 219.2 VAC

2. Calibration method

The calibration use in-house method: WI-CL-025 based on BS 2646 part 5: 1993 item 3.1.

Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Temperature Data Logger	HiTemp 140	LB-TEM-17	22-089923	31 August 2023
3.2 Temperature Data Logger	HiTemp 140	LB-TEM-16	22-023565	08 March 2023
3.3 Temperature Data Logger	TEMP 1000S	LB-TEM-14	22-089922	31 August 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Sarawoot Thammo
Scientist

Issue date : 22 September 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CI-114

TEL 02-516-2422
FAX 02-516-6949

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH



REPORT OF CALIBRATION

Page 2 of 2

Certificate No. : 22-102070
Sample Code : 22-37024-01

Results of Calibration

Resolution : 1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading		Measured Temperature at each positions (°C)			Uncertainty ± (°C)	Coverage factor <i>k</i>
		Temperature (°C)	Pressure (MPa)	# 1	# 2 ^{ref}	# 3		
121	121	121	0.11	121.81	121.80	121.83	0.64	2.00

2. Characterization results

Calibration Point (°C)	Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
121	0.08	0.12	0.17

Notes

- UUC* = Unit Under Calibration
- The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
- Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
- Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
- Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
- UUC* reading - the average reading of indicating device that forms the integral part of the autoclave.
- Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.




Figure: Example of sensor
installation Positions

- Standard 1 = In the chamber drain, within 100 mm.
Standard 2 = In the upper half of the chamber.
Standard 3 = Attached to the load temperature probe, within 20 mm.

- End of Report -

TEL 02-516-2422
FAX 02-516-6949

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310

CONTACT@AMARC.CO.
WWW.AMARC.CO.

BOD INCUBATOR

ID No. : LABE 19/2

NSC-TS17517025
CALIBRATION 0352

Page 1 of 3

Certificate No. : 22-136844

Sample Code : 22-51164-006

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhepiban 8 Rd., Nongkham,

Sirachra, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.

(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : N/A Model : N/A

Serial No. : S540040277 ID No. : LABE 19/2

Date of Receipt : 21 December 2022 Date of Calibration : 21 December 2022

Condition of Calibration

1. Environment	1.1 Ambient temperature	Maximum	25.1 °C	Minimum	24.3 °C
	1.2 Relative humidity	Maximum	52.3 %	Minimum	48.5 %
	1.3 Line voltage supplied	Maximum	223.6 VAC	Minimum	221.9 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-PT100)	LB-DA-T1 (RTD-148 to RTD-155, RTD-227)	22-040308	24 April 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Nathanan Phosri

Approved by

Scientist

Issue date

26 December 2022

The uncertainties are for a confidence probability of approximately 95%.
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.
The Certificate is issued in accordance with the conditions of accreditation gained by the Thai Laboratory Accreditation scheme which has been recognized by the Thai Laboratory Accreditation Center (TLAC) and is traceable to the international system of unit (SI Unit).
The calibration result is not valid for use for other items without the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

FM-CL-114

TEL 02-516-2422

FAX 02-516-6949

Rev 01

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

Effective Date 15/10/21

NSC-TS17517025
CALIBRATION 0352

Page 2 of 3

Certificate No. : 22-136844

Sample Code : 22-51164-006

REPORT OF CALIBRATION

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)								Uncertainty ± (°C)	Coverage factor k	
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8			# 9 ^{Ref}
20	20.0	20.0	19.65	19.56	19.47	19.29	20.96	20.47	20.23	20.58	20.29	0.35	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.13	1.09	1.90

Notes

UUC* = Unit Under Calibration

TEL 02-516-2422

FAX 02-516-6949

Rev 09



NSC-TSI-7617025
CALIBRATION 0152

Page 3 of 3

REPORT OF CALIBRATION

Certificate No. : 22-136844

Sample Code : 22-51164-006

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 60 cm ; D = 70 cm ; H = 124 cm
3. Air valve or fresh air level : Off
4. Fan level : open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

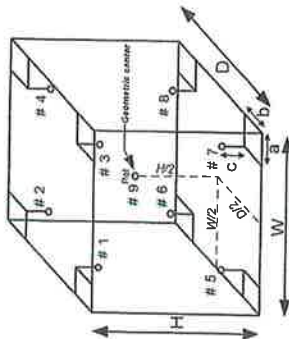


Figure: Example of sensor
Installation Positions

- End of Report -

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with ISO 17025.

BOD INCUBATOR

ID No. : LABE 19/5



ASIA MEDICAL AND
AGRICULTURAL LABORATORY
AND RESEARCH CENTER

AMARC

Page 2 of 3
Certificate No. : 22-053227
Sample Code : 22-19571-002

REPORT OF CALIBRATION

Results of Calibration
Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C) reading (°C)	Measured temperature at each positions (°C)								Uncertainty ± (°C)	Coverage factor k
		# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8		
20	20.6	20.09	19.99	20.00	20.03	19.95	19.98	20.00	19.81	19.90	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.17	0.32	0.57

Notes

- UUC* = Unit Under Calibration

47

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-P100)	LB-DA-10 (RTD-257 to RTD-265)	21-056687	05 July 2022

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Pettarakorn Panklong

Scientist

Issue date : 25 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme.

This certificate is traceable to recognized national standards and to the unit of measurement realized at the corresponding national laboratory and its traceability is recognized by the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road, Phlabphla, Wang Thonglang, Bangkok 10310

Rev 01

Effective Date 15/10/21

WWW.AMARC.CO.TH

CONTACT@AMARC.CO.TH

TEL 02-516-2422 FAX 02-516-6949

TEL 02-516-2422

FAX 02-516-6949

Rev 09

Effective Date 15/10/21

WWW.AMARC.CO.TH

CONTACT@AMARC.CO.TH

TEL 02-516-2422

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

Rev 09

Effective Date 15/10/21

WWW.AMARC.CO.TH

CONTACT@AMARC.CO.TH

TEL 02-516-2422

REPORT OF CALIBRATION

Certificate No. : 22-053227
Sample Code : 22-19571-002

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber : (Working space)
W = 65 cm ; D = 55 cm ; H = 146 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes " Stability of chamber and loading effect in chamber at 20% of uniformity ".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC" reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

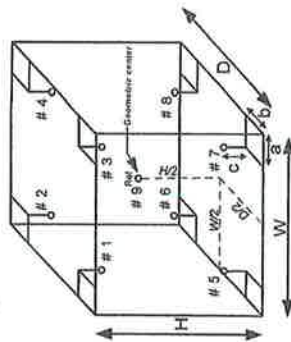


Figure: Example of sensor installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS.

- End of Report -

CONDUCTIVITY METER

Type : SevenCompactTM Conductivity meter S230

Serial No. : B744909989

Certificate Number CCP-2407-23

Certificate Number CCP-2407-23

Calibration Certificate SevenCompact™ Conductivity Meter S230

Certification Tools

Certified conductivity resistors
 Manufacturer METTLER TOLEDO
 Type 51302861
 Serial number S260
 Certificate number 62619
 Date of certification February 15, 2022

Customer

Company EASTERN THAI CONSULTING 1992 CO., LTD.
 Address 683 Moo 11, Sukhaphiban 8 Rd., Nong Kham, Sriracha
 Chonburi 20230
 Customer ID number 301608441
 Customer representative Sasiport Nakin

Instrument

Type SevenCompact™ S230
 Instrument serial number B744909889
 Internal identification LABE 132
 Firmware version 2.01.03

Technical Specifications

Measuring range 0.001 µS/cm ... 1000 mS/cm
 Resolution Auto range
 Limit of error ±0.5%
 Temperature range MTC -30.0 ... 130.0 °C
 Temperature range ATC -5.0 ... 130.0 °C
 Resolution 0.1 °C
 Limit of error ±0.1 °C

Procedure Statement

METTLER TOLEDO Certification SOP (Doc. No. 30027577) is used as referring documentation to adjust and certify the instrument indicated in the "Type" and "Serial number" section. The measurement results of this certification were obtained at ambient conditions.

Designation	Nominal value	Certified value
Conductivity 10 Ω	10.000 Ω	10.013 Ω
Conductivity 150 Ω	150.00 Ω	150.05 Ω
Conductivity 1.5 kΩ	1.5000 kΩ	1.5001 kΩ
Conductivity 15 kΩ	15.0000 kΩ	15.001 kΩ
Conductivity 150 kΩ	150.00 kΩ	149.92 kΩ
Conductivity 1 MΩ	1.0000 MΩ	1.0004 MΩ

Certified temperature resistors
 Manufacturer METTLER-TOLEDO
 Type 51302410
 Serial number A275
 Certificate number 62591
 Date of certification February 14, 2022

Designation	Nominal value	Certified value
NTC 30 kΩ, 0 °C	94.980 kΩ	95.049 kΩ
NTC 30 kΩ, 25 °C	30.000 kΩ	29.994 kΩ
NTC 30 kΩ, 50 °C	10.969 kΩ	10.965 kΩ
NTC 30 kΩ, 75 °C	4.528 kΩ	4.529 kΩ
NTC 30 kΩ, 100 °C	2.070 kΩ	2.070 kΩ

Certificate Number CCP-2407-23

Certification Measurements

Designation	Certified value	Measured value	Max. tolerance	Passed / Failed
Conductivity sensor input (resistance)				
10 Ω	10.013 Ω	10.010 Ω	0.5 %	Passed
150 Ω	150.050 Ω	150.100 Ω	0.5 %	Passed
1.5 kΩ	1.500 kΩ	1500.00 Ω	0.5 %	Passed
15 kΩ	15.001 kΩ	15000 Ω	0.5 %	Passed
150 kΩ	149.920 kΩ	149900 Ω	0.5 %	Passed
1 MΩ	1.000 MΩ	1000000 Ω	0.5 %	Passed

Designation	Nominal value	Measured value	Max. tolerance	Passed / Failed
Conductivity sensor input (temperature)				
NTC 30 kΩ, 0 °C	0.0 °C	0.0 °C	0.1 °C	Passed
NTC 30 kΩ, 25 °C	25.0 °C	25.0 °C	0.1 °C	Passed
NTC 30 kΩ, 50 °C	50.0 °C	50.0 °C	0.1 °C	Passed
NTC 30 kΩ, 75 °C	75.0 °C	75.0 °C	0.1 °C	Passed
NTC 30 kΩ, 100 °C	100.0 °C	100.0 °C	0.1 °C	Passed

Resistor designation	Certified value	Measured value	Max. tolerance	Passed / Failed
Verification according to USP <645> cell constant = 0.100 /cm				
1 MΩ	0.100 μS/cm	0.100 μS/cm	0.1 μS/cm	Passed
150 kΩ	0.667 μS/cm	0.667 μS/cm	0.1 μS/cm	Passed
15 kΩ	6.666 μS/cm	6.667 μS/cm	0.1 μS/cm	Passed

Digital sensor input with conductivity sensor	The sensor was recognized correctly by the meter	Passed
---	--	--------

Summary of Certification

Certification of instrument

Passed

The instrument referred to in this certificate has fulfilled the criteria of the certification. This is indicated by the notation Passed above.

Remarks

Service Assignment ID : 0332630077

Certification of the instrument was performed by

Name	Thiraphong Salanoi	Function	Service Engineer
Company	Mettler-Toledo (Thailand) Ltd.		

Date February 6, 2023 Signature

Mettler-Toledo (Thailand) Limited

METTLER TOLEDO

Performance Test

Attachment to Certificate No. CCP-2407-23

Conductivity Sensor

Type: InLab 731-ISM S/N: 5821041078

Certified standards used

Standard 1:	Type:	Cond. Standard	Manufacturer: METTLER TOLEDO	Exp. date: 18-Mar-23
		Nominal value: (25.00 °C):	1413 μS/cm	Lot No.: 1G077C

Standard 2:	Type:	Cond. Standard	Manufacturer: METTLER TOLEDO	Exp. date: 31-Mar-23
		Nominal value: (25.00 °C):	12.88 mS/cm	Lot No.: 1G090B

Cell Constant Adjustment

Nominal	Old (cm ⁻¹)	New (cm ⁻¹)
1413 μS/cm	0.504069	0.550105

Measurements

(Reference Temperature: 25 °C and Temperature correction is 2.00 % / °C)

Before adjustment			After adjustment		
Buffer Values	Measured	Difference	Buffer Values	Measured	Difference
1413 uS/cm	26.5 °C	1316	1413 uS/cm	27.5 °C	1405
12.88 mS/cm	26.9 °C	-0.74	12.88 mS/cm	27.4 °C	12.68
					-8
					-0.20

Note: The difference result of calibrated electrode should be within +/- 2.5%

Remarks:

Place:

Laboratory Room

Performance Date:

February 6, 2023

Service Specialist:

Thiraphong Salanoi

Signature:

DO

Model : YSI 5000

Serial No. : 18E101961



Harikul Science Co., Ltd.
694 Soi Ratchadaniwet 24, Pracharabamphen,
Samsenok, Huaihwang, Bangkok 10310
Tel: 0-2274-2456 Fax: 0-2274-2443
Email: info@harikul.com www.harikul.com

CERT No.: HS-T055H

Certificate of Calibration

Calibration Date : 23 Aug 22

Submitted by : Eastern Thai Consulting 1992 Company Limited
683 Moo.11 Sukaphibab8 Rd., Nongkham, Sriracha,
Chonburi 20230

Model : YSI 5000
S/N : 18E101961
Probe : YSI 5010
S/N : 18A100724
ID NO. :
Air Temp ref : S/N. E00522
Barometric ref : S/N. E00522
Water Temp ref : S/N. 11431

Avg Room Temp : 20 °C
Avg Water Temp : 20 °C
Air Pressure : 760.00 mmHg
Salinity : 0 ppt

Technician : Kitipong M.

Calibration Details			
Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.09	(PASS)	-
Measurement 4 (mg/l)	9.10	(PASS)	-
Measurement 5 (mg/l)	9.10	(PASS)	-
Measurement 6 (mg/l)	9.09	(PASS)	-
Measurement 7 (mg/l)	9.09	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.09	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-

Mean Measurement	9.09	mg/l	-
Inaccuracy	0.00	mg/l	-
Overall Status	(PASS)		

Manufacturer Specification	
Accuracy = +/- 0.02 mg/l	

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Hot Air Oven

Model. : UM 400

Serial No. : 900982

REPORT OF CALIBRATION

Certificate No. : 23-018635
Sample Code : 23-07651-001

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 40 cm ; D = 28 cm ; H = 39 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes " Stability of chamber and loading effect in chamber at 20% of uniformity ".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

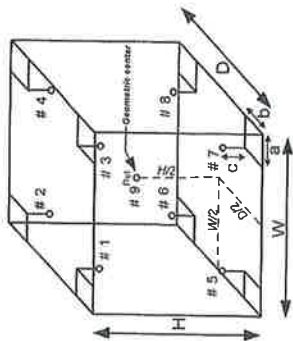


Figure: Example of sensor installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS

- End of Report -

INDUCTIBELY COUPLED PLASMA SPECTROMETER

Model : Prodigy 7

Serial No. : P70177



บริษัท แอปพลิเคชัน สี่พันเจ็ด จำกัด
Application Define Company Limited
133/318 ถนนพหลโยธิน แขวงสามยุค เขตเมืองใหม่ กรุงเทพมหานคร 10510
Tel: (66)8456-5991 E-mail: support@apdefine.co.th Website : http://www.apdefine.co.th
เลขประจำตัวผู้เสียภาษี 0105556032491

CERTIFICATE OF INSTRUMENT PERFORMANCE

INSTRUMENT:

INDUCTIVELY COUPLED PLASMA SPECTROMETER

BRAND:

Teledyne Leeman Labs

MODEL:

Prodigy 7

SERIAL NO.

P70177

CUSTOMER:

บริษัท อีสเทิร์นไทย คอนกรีต 1992 จำกัด

CHECKING:

SPECTROMETER

Wavelength Accuracy check by use emission line of Hg Lamp

Mercury line 253.652 nm.

Plasma View (Dual View)

CMOS Detector check

Align View by Mn line 257.610 nm.

RF GENERATOR

Incident Power 1,200 ±10 Watt Reading = 1200 Watt

SAMPLE INTRODUCTION

Plasma Torch, Injector, Spray chamber, Nebulizer

Partialtic pump & Tubing

EXHAUSTING & COOLING SYSTEM

Safety Interlock Switch (Door, Argon pressure, Water pressure)

Cooling System, water flowrate & low pressure switch

Flowrate of Air blower

COMPUTER & SOFTWARE

Plasma Ignition software & Analytical Software

ANALYTICAL TEST

Full Frame Capture & Echellogram check

Calibration Cuve & QC Test

DATE :






Dec.17, 2022

PREVENTIVE MAINTENANCE / CALIBRATION REPORT FOR PRODIGY7

Customer: บริษัท อีสเทิร์นไทย คอนกรีต 1992 จำกัด Date: Dec 12, 2022

Instrument: ICP-OES Model: Prodigy 7 S/N: P70177

1. Gas Supply /Water Re-circulator/Exhaust Hood Check:

Gas system: ตรวจสอบแรงดันแก๊สและทำการรั่วซึม Argon Pressure: 5-10 psi Leak inspected (✓) No leak Nitrogen Pressure: 5-10 psi Leak inspected (✓) No leak Oxygen Pressure: 5-10 psi Leak inspected (✓) No leak	
() Change camera purge gas Dehydrator (1 times /years) Next time replacement 25/12/2562 เปลี่ยนตัวความชื้นดีไฮเดรต ทุก 1 ปี	
Water Chiller: RF generator flow rate 4.44 LPM Temperature 25.0 C ตรวจอุณหภูมิ Leak inspected (✓) No leak ตรวจทดสอบการรั่วซึม	
Water Chiller : Camera (✓) check water level and refill ตรวจระดับน้ำและเติมน้ำ (✓) change water เปลี่ยนน้ำ Temperature -3.1 °C ตรวจอุณหภูมิ	
Exhaust Hood Flow rate 700 CFM (system request > 150)	

TELEDYNE LEEEMAN LABS
PURITY. PRECISION. PERFORMANCE.



PREVENTIVE MAINTENANCE / CALIBRATION REPORT FOR PRODIGY7

Customer: บริษัท อีทีพีไทย คอนสตรัคชั่น 1992 จำกัด	Date: Dec 12, 2022
Instrument: ICP-OES	Model: Prodigy 7

2. Computer & Software Check

Description	Status
Interface Cable USB (✓) No broken	OK
Software Version	OK
(✓) Operation function check :	OK
(✓) Open /Save /Edit method	OK
(✓) Instrument Control	OK
(✓) Sequence	OK
(✓) Full Frame Capture (Echelle Mode)	OK
(✓) Auto alignment /Hg alignment	OK
(✓) Calibration Curve	OK
(✓) Re-Calculation	OK
(✓) Print Report	OK

PREVENTIVE MAINTENANCE / CALIBRATION REPORT FOR PRODIGY7

Customer: บริษัท อีทีพีไทย คอนสตรัคชั่น 1992 จำกัด	Date: Dec 12, 2022
Instrument: ICP-OES	Model: Prodigy 7

3. Instrument Control

Description	Status
Optical view position: ตรวจสอบตำแหน่งพัฒนาที่ติดตั้งในเตาและมุมอง	
Hg Lamp Deltas	
X 2 Y - 9	OK
XUV 0	OK
Axial peak positions X 3325 Y 1225	OK
Radial peak positions X 4151 Y 1225	OK
Hg lamp peak positions X 2220 Y 2630	OK
Plasma Control ตรวจสอบการทำงานภาคจุดและดับพลาสมา	
(✓) Auto Start	OK
(✓) Extinguish	OK
(✓) RF power setting	OK
(✓) Igniter	OK
(✓) Air Knife	OK
Torch Gas ตรวจสอบการทำงานของระบบแก๊สที่ใช้ในเตาพลาสมา	
(✓) Coolant/Plasma Flow control	OK
(✓) Aux Flow	OK
(✓) Nebulizer Flow	OK
(✓) Optimize sample introduction function	OK
(✓) Peristaltic pump control	OK
(✓) Auto sampler Control	OK
(✓) Camera Support Module	OK
(✓) Diagnostic	OK

PREVENTIVE MAINTENANCE / CALIBRATION REPORT FOR PRODIGY7

Customer: บริษัท อีสเทิร์นไทย คอนสตรัคชั่น 1992 จำกัด	Date: Dec 12, 2022
Instrument: ICP-OES	Model: Prodigy 7

4. Cleaning & Replacement

Description	Status
(✓) O-Ring Torch replacement	OK
(✓) Pump Tubing replacement	OK
(✓) Glassware cleaning (Torch, Nebulizer, Spray chamber)	OK
(✓) Lube the roll peristaltic pump	OK
(✓) Optical windows cleaning	OK
(✓) Camera Water Re-circulator (water change/ refilled)	OK
(✓) RF Generator Water Re-circulator (water change/ refilled)	OK
(✓) Cleaning Electronics Board with spray cleaner	OK
(✓) Cleaning dust inside Unit	OK
(✓) Cleaning dust filter	OK

5. Safety Interlock

Description	Status
(✓) Door switch	OK
(✓) RF Water Re-circulator	OK
(✓) Camera Water Re-circulator	OK
(✓) Camera purge gas	OK
(✓) Argon pressure	OK
(✓) Nitrogen pressure	OK

PREVENTIVE MAINTENANCE / CALIBRATION REPORT FOR PRODIGY7

Customer: บริษัท อีสเทิร์นไทย คอนสตรัคชั่น 1992 จำกัด	Date: Dec 12, 2022
Instrument: ICP-OES	Model: Prodigy 7

6. Hardware Check with SALSA.EXE Diagnostics

Power Supply	Value	Status
-12 VDC (11 - 14.5 VDC)	-13.75V	OK
+12 VDC (11 - 14.5 VDC)	+12.01V	OK
+3.3VDC	3.26V	OK
+5.0VDC	4.94V	OK
+13.5VDC	13.48V	OK

Plasma Generator	Value	Status
ICP Current 0.500A = 1kW	0.54A	OK
ICP Ref 5.0Vdc = 1kW	5.46V	OK
ICP Current 0.00 Vdc = 0kW	0	OK
ICP Ref 0.00Vdc = 0kW	0	OK
RF Water (Hz) OFF	0	OK
RF Water (Hz) ON	23	OK
Air Knife Pres. (0.00V) OFF	0	OK
Air Knife Pres. (3.0 - 7.0 V) ON	4.05V	OK
Neb 25 @ setting of 25 PSI	25	OK
Cool 18 @ setting of 18 LPM	18	OK
Aux 0.6 @ setting of 6 LPM	0.6	OK
Pump Current (0.000 A) OFF	0	OK
Pump Voltage (0.000 V) OFF	0	OK
Pump Current (0.8 to 4.0A) ON	1.0A	OK
Pump Voltage (8 to 13 V) ON	12.52	OK

Set Points	Value	Status
Air In Set Point 32°C	31	OK
Cam Tee Temperature -32°C	-32	OK
Op Purge Low 0.77 LPM	0.7	OK
Op Purge High 15.50 LPM	15.5	OK
Cam Wtr T 28°C	28	OK

PREVENTIVE MAINTENANCE / CALIBRATION REPORT FOR PRODIGY7

Customer: บริษัท อีทีพีไทย คอนสตรัคชั่น 1992 จำกัด	Date: Dec 12, 2022
Instrument: ICP-OES	Model: Prodigy 7
	S/N: P70177

7. Mn Check for performance Test

	Condition for performance Test	Condition Test	Status
Standard	1 ppm, 5 ppm, 10 ppm	10 ppm	ok
Power plasma	1.20 kw	1.2	ok
Plasma gas	16.0 LPM	16	ok
Auxiliary Gas	0.8 LPM	0.8	ok
Nebulizer	1.2 LPM	25 psi	ok
Pump Speed	25 RPM	25	ok
Integration time	15 s Axial, 5 s Radial	10 s, 5 s	ok
Nebulizer Type	Seaspray, Conical, Meinhard	Seaspray	ok
Intensity first performance	1 ppm ≥ 4,000,000 5 ppm ≥ 15,000,000 10 ppm ≥ 50,000,000	2,65,000,000	ok

12 Dec 2022



LIQUID IN GLASS THERMOMETER

Model : Total immersion

Serial No. : 43560

Calibration Certificate

Certificate No.: 2300368-001-01
Client name: EASTERN THAI CONSULTING 1992 CO., LTD.
Address: 683 Moo 11, Sukhapibam 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Equipment: Liquid-in-Glass Thermometer
Manufacturer: Precision
Model / Type: Total Immersion
Serial No.: 43560
ID No.: LABE 16/1
Order No.: 2300368
Operation No.: 2300368-001
Date of Receipt: 7 November 2022
Date of Calibration: 15 November 2022

Calibrated by Mr. Nutapol Miyomchet
Specialist

Date of Issue: 18 November 2022

The uncertainties are for a confidence probability of approximately 95%.
This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.



Calibration Report

Certificate No.: 2300368-001-01
Equipment: Liquid-in-Glass Thermometer Type: Total Immersion
Range: -1.9 to 101.1 °C Resolution: 0.1 °C
ID No.: LABE 16/1 Serial No.: 43560
Manufacturer: Precision
Date of Calibration: 15 November 2022

Location: Temperature Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature 23 °C ± 3 °C
Relative Humidity 55 % ± 15 %

Condition of this results of Calibration:

1. Calibration Method : - In-house method : W-TE-015 based on ASTM E77-07
- The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
- The temperature Scale in use at this laboratory is the International Temperature Scale of 1990 (ITS-90).

2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
BLACK STACK THERMOMETER	1560/2560	A39258/A39719	PSL-T 0674/65	7-Jun-23	TISTR
Platinum Resistance Thermometer (PRT)	5615	808926			

Support Equipment : - Ice point Unit, ID No.: ana. 614/21

- Low Temperature Bath (Deep Well Compact Bath), Model: 7381, S/N: B53496.
- Low Temperature Bath (Deep Well Compact Bath), Model: 7341, S/N: A5A084.
- High Temperature Bath (Deep Well Compact Bath), Model: 6331, S/N: A5A087.

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
7. Result of Calibration : ☒ Without adjustment ☐ After adjustment



Calibration Report

Certificate No.: 2300368-001-01
Equipment: Liquid-in-Glass Thermometer
Type: Total Immersion
Range: -1.9 to 101.1 °C
Resolution: 0.1 °C
ID No.: LABE 16/1
Serial No.: 43560
Manufacturer: Precision
Date of Calibration: 15 November 2022

Page 3 of 3

Calibration point: 3.0, 25.0 and 50.0 °C
Calibration result:

Reporting of ice-point or reference point

UUC* Reading (°C)	Standard Temperature/Ice Point (°C)	Correction Value (°C)	Uncertainty ± (°C)
0.0	0.0032	0.0	0.091

Reporting of temperature calibration point

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
25.0	24.9990	0.0	0.088
50.0	49.9943	0.0	0.088

Note

* UUC* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied providing a level of confidence of approximately 95 %.

----- End -----



pH Meter

Model. : SevenCompact S220

Serial No. : B448305208



CERTIFICATE OF CALIBRATION

Page 1 of 3
Certificate No. : 23-011524
Sample Code : 23-04833-001Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siriracha, Chonburi 20230Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)Equipment : pH Meter
Manufacturer : METTLER TOLEDO Model : SevenCompact S220
Serial No. : B448305208 ID No. : LABE 11/4
Date of Receipt : 01 February 2023 Date of Calibration : 01 February 2023

Condition of Calibration

1. Environment
1.1 Ambient temperature : 25.0 ± 2.5 °C 1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

In house method WI-CL-019: based on direct measurement by using standard voltage calibrator and using certified reference material (CRM).

20

3. Reference standard / Certified reference material

Instrument	ID No.	Certificate No.	Due Date
3.1 Voltage Calibrator	LB-AMC-01	22E3240	03 October 2023
3.2 Digital Thermometer	LB-TH-33	22-107027	02 October 2023
Certified Reference Material			
Lot No.	Ref No.	Lot No.	Expire Date
3.3 Buffer Solution pH 4.008	838357	PH16.L5	15 September 2024
3.4 Buffer Solution pH 6.985	838358	PH107.L5	15 September 2023
3.5 Buffer Solution pH 10.008	838359	PH220.L5	15 September 2023

4. This certificate is traceable to the international system of unit (SI Unit).

- Instrument No. 3.1 through Technology Promotion Association (Thailand-Japan).
- Instrument No. 3.2 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.
- Buffer Solution No. 3.3 and No. 3.5 traceable to CPA chem (through primary measurement method-Harned cell using calibrated thermometer, barometer, and nanovoltmeter. Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).
- Buffer Solution No. 3.4 traceable to CPA chem (BIM RefN HI-27 LoIN 04.06.2021 ; BIM RefN HI-28 LoIN 28.05.2021 ; BIM RefN HI-27 LoIN 04.06.2021 ; BIM RefN HI-28 LoIN 28.05.2021 Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Anupong Lakawin Approved by : [Redacted]

Scientist

Issue date : 03 February 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme.

laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be

reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-114TEL 02-516-2422
FAX 02-516-6949
Rev 01CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date 15/10/23

REPORT OF CALIBRATION

Page 2 of 3
Certificate No. : 23-011524
Sample Code : 23-04833-001Equipment : pH Meter Resolution : 0.01 pH ; 0.1 mV ; 0.1°C
Manufacturer : METTLER TOLEDO Model : SevenCompact S220
Serial No. : B448305208 ID No. : LABE 11/4
Range : -2.000 pH to 20.000 pH ; ± 2000.0 mV ; -5.0°C to 130.0°C

Results of Calibration

Part 1. DC Voltage measurement

pH Meter Serial No. : B448305208

Nominal Value	Applied DC Voltage	Average indicator reading		Uncertainty	Coverage factor
		mV	pH		
0	414.113	414.0	0.00	± 0.083	2.00
4	177.477	177.5	4.00	± 0.083	2.00
7	0.000	0.1	7.00	± 0.083	2.00
10	-177.477	-178.3	10.00	± 0.083	2.00
14	-414.113	-413.8	14.00	± 0.083	2.00

Part 2. Performance of Electrode system

Electrode Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Electrode Serial No. : 2365921


Three-Point Calibration at pH4 and pH7 Percent Slope : 99.6 ; at pH7 and pH10 Percent Slope : 98.4

Standard Buffer Solution	Average indicator reading		Error Value	Uncertainty	Coverage factor
	pH (@ 25 °C)	mV			
4.008	4.01	184.2	0.002	± 0.011	2.00
6.985	6.99	8.9	0.005	± 0.010	2.00
10.008	10.01	-166.8	0.002	± 0.010	2.00

The result expanded uncertainty (U) is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

22

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-016TEL 02-516-2422
FAX 02-516-6949
Rev 09CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date 15/10/23



REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 23-011524

Sample Code : 23-04833-001

Equipment : pH Meter (Digital Thermometer with sensor)

Thermometer readout

Manufacturer : METTLER TOLEDO Model : SevenCompact S220

Serial No. : B448305208 ID No. : LABE 11/4

Resolution : 0.1 °C Range : -5.0 °C to 130.0 °C

Thermometer sensor

Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Serial No. : 2365921 ID No. : N/A

Condition of Calibration

1. Environment
 - 1.1 Ambient temperature : 23.0 °C ± 3.0 °C
 - 1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

- 2.1 The calibration use in house method WI-CL-021 : by comparison with standard thermometer
- 2.2 The calibration by comparison unit under calibration (UUC) to the standard thermometer in a calibration bath at the controlled temperature.
- 2.3 The temperature scale in use of this laboratory is the international temperature scale of 1990 (ITS-90).

3. Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due date
3.1 Platinum Resistance Thermometer	PT-100	RTD-90	22-107027	02 October 2023
3.2 Thermometer Readout	GT-11	LB-TM-33	22-107027	02 October 2023

4. This certificate is traceable to the international system of unit (SI Unit).

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Accreditation Under TLAS Laboratory Calibration No.0152)

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibration item : Normal

Results of Calibration

Calibration point °C	Average of standard reading °C	Unit under calibration		Expanded uncertainty °C	Coverage factor k
		Immersion depth mm	Average reading °C		
25	25.002	120	25.0	± 0.13	2.00

Notes

- Calibration results without adjustment

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with ISO 17025.

- End of report -

STANDARD WEIGHT 50 g



Certificate No. : 22-052238
Sample Code : 22-19150-003

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist
Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052238
Sample Code : 22-19150-003

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Result of Calibration : ☒ Without adjustment ☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	± (mg)	
50 g	-0.324	49.999676 g	0.10	0.30	LABE 10/1

The result expanded uncertainty of measurement U is stated as the standard uncertainty multiplied by the coverage factor $k = 2.0$, which for a normal distribution gives a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS

Certificate No. : 22-052238
Sample Code : 22-19150-003

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature 20 °C ± 1.5°C, Relative humidity 50% ± 10% and air density 1.20 kg/m³
2. Calibration Method : Direct comparison weighing according to OIML R111-1 : 2004(E)
3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-078366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

STANDARD WEIGHT 100 g



Certificate No. : 22-052239
Sample Code : 22-19150-004

Page 1 of 3

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist
Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052239
Sample Code : 22-19150-004

Page 2 of 3

REPORT OF CALIBRATION

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Result of Calibration :

☒ Without adjustment☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	± (mg)	
100 g	-0.171	99.999829 g	0.16	0.50	LABE 10/2

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with U

COPY



Certificate No. : 22-052239

Sample Code : 22-19150-004

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature 20 °C ± 1.5°C, Relative humidity 50% ± 10% and air density 1.18 kg/m³

2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-78	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated item :

Type and Nominal Value :	Standard Weight 100 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

STANDARD WEIGHT 50 g



Certificate No. : 22-052237

Sample Code : 22-19150-002

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

689 Moo 11, Sukhapiban 8 Rd., Nongkham,

Siracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052237

Sample Code : 22-19150-002

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Result of Calibration :

☒ Without adjustment☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	± (mg)	
50 g	-0.111	49.999889 g	0.10	0.30	LABE 10/4

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2.0$, which for a normal distribution gives a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M



Certificate No. : 22-052237

Sample Code : 22-19150-002

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$, Relative humidity $50\% \pm 10\%$ and air density 1.18 kg/m^3
2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at :-

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

UV/VIS SPECTROPHOTOMETER

Model : UV – 1800

Serial No. : A11635101643CD



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No. BSCC-UV-167/22
Equipment UV/Vis Spectrophotometer
Model UV-1800
Manufacturer Shimadzu
Serial No. A11635101643 CD
ID No. LABE 03/2
Date of receipt 18 May 2022
Date of calibration 18 May 2022
Date of issue 25 May 2022

Customer name Eastern Thai Consulting 1992 Co., Ltd.
Address 683 Moo 11, Sukkaphibarn 8 Rd., Nongkham, Siraacha, Chonburi 20230.

Temperature (23.8-24.5) °C (On site)
Humidity (47.6-48.3) %RH (On site)

Equipment condition Good Operation

Calibration Location Analysis Department.

Calibration Procedure In-house method WI-UV-702-01 based on ASTM E275-01

Traceability Wavelength Accuracy is traceable to certificate No. 96367 and 96366
Photometric Accuracy is traceable to certificate No. 99925 and 100147
Stray Light is traceable to certificate No. 96346
The above certificate are traceable to SI unit through Siam Scientific Ltd.
(UKAS accredited calibration laboratory NO. 06559)

Calibrated by Mr.Kanchit Choolthep



The above results are valid exclusively for the calibrated item(s) as mentioned in this report. Adversing the report / Certificate and publicity of the results are prohibited except in full, without written approval of the Bara Scientific Co., Ltd.



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Number of Page(s) 2 of 3

Certificate No. BSCC-UV-167/22

Calibration Results:
1. Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (nm)
287.71	287.80	0.09	0.18
445.82	445.95	0.13	0.18
536.52	536.60	0.08	0.18
741.02	741.00	-0.02	0.18
879.41	879.40	-0.01	0.18

2. Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000	0.0000	0.0000	0.00075
	0.7311	0.7321	0.0010	0.0075
257	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
313	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
350	0.0000	0.0000	0.0000	0.0008
	0.6306	0.6314	0.0008	

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mentioned in this report. Adversing the report / Certificate and publicity of the results are prohibited except in full, without written approval of the Bara Scientific Co., Ltd.



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor 7 Rama4 Road
Silom Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Certificate No. BSCC-UV-167122 Number of Page(s) 3 of 3

Calibration Results:

3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5472	0.5481	0.0009	0.0042
	0.7637	0.7636	-0.0001	0.0042
440.0	1.0480	1.0497	0.0017	0.0042
	0.0000	0.0000	0.0000	0.0042
	0.5371	0.5377	0.0006	0.0042
465.0	0.7457	0.7451	-0.0006	0.0042
	1.0233	1.0240	0.0016	0.0042
	CNR	CNR	CNR	CNR
546.1	CNR	CNR	CNR	CNR
	0.0000	0.0000	0.0000	0.0042
	0.5006	0.5006	0.0000	0.0042
590.0	0.6961	0.6944	-0.0017	0.0042
	0.9563	0.9550	-0.0013	0.0042
	CNR	CNR	CNR	CNR
635.0	0.0000	0.0000	0.0000	0.0042
	0.5137	0.5137	0.0000	0.0042
	0.6907	0.6891	-0.0016	0.0042
	0.9533	0.9519	-0.0014	0.0042

*CNR = Customer not request

4. Stray Light*

Unit Under Calibration(UUC)			
Standard	Wavelength (nm)	Transmission (%)	Absorbance (A)
cut-off wavelength (nm)	201.10	0.9543	2.0204

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of 95%

End of Certificate

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate. Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.

FM-UV-708-02 Rev.01 (23/01/63)

MERCURY ANALYZER

Model : RA-4500

Serial No. : 21780504



บริษัท โคแอก กรุ๊ป คอร์ปอเรชั่น จำกัด
COAX GROUP CORPORATION LTD.

COAX GROUP CORPORATION LTD.

DATE : March 24, 2023

Certificate of Calibration

MERCURY ANALYZER FOR WORKING ENVIRONMENT
THERMOMETER / RA-4500

Customer name : Eastern Thai Consulting 1992 Co.,Ltd.

Certificate No : SRP001-23
Customer P/O : PO.no.PI5602053
Sale Order No : -

Model # RA-4500
Serial No. # 21780504

Results : Quality Reborn Reference Standard Laboratory, NSC-TISI-TIS 17025 Calibration No.0292

Cal. Points	TIME	PRESET TEMP	Avr.	FACTOR ±0.5
3 Point	60 Minutes	95 (°C)	90.73	0.950 - 1.050

This instrument is calibrated at factor 0.955

TEST APPARATUS

Instrument Type	Serial Number	Certificate No.
PONPE 429TP	5845166	TM23-0008
PONPE 429TP	5845167	TM23-0009
PONPE 429TP	5845168	TM23-0010

Date of Calibrate : March 24, 2023

Next due date : March 24, 2024

Calibrate by :

Eastern Thai Consulting 1992 Co., Ltd.

Automatic Mercury Analyzer

Model RA-4500

Preventive Maintenance Report

Serial No. : 21780504

Soft version : Ver 2.0.7

ROM version : Ver 2.0.1

Date : February 09, 2023

Next due date : August 09, 2023

PM by

Approved by




Coax Group Corporation Ltd.

1131/62,64,325-331 Nakornchaisri road,
Kwang ThanonNakornchaisri, Dusit, Bangkok 10300 Thailand
Tel. 02-2435263, 02-6682436 Fax. 02-2437386

Inspection result

ITEM	STANDARD	RESULT	JUDGE
1. Self Check			
1.1 Leak check	0.14 - 2.0L/min	0.17L/min	PASS
1.2 Sig/Ref check	Signal 3.00 - 4.00V Sig:3.97V, Ref:3.89V		PASS
1.3 Drift check	0.0000236 - 0.0000061	0.0000175	PASS
2. Analytical curve inspection(AREA)			
2.1 Calibration curve 0-100ng (Hight)	Correlation coefficient	1.0000	PASS
(r') ≥ 0.9999			
3. Repeatability(AREA)			
3.1 Repeat STD 50ng, n=3			
	1.	50.60	ng
	2.	50.94	ng
	3.	50.71	ng
4. Blank			
	C.V. ≤ 5%	0.34%	PASS
	Below 1.0(AREA)	0.0158	PASS




SMP

No.	NAME	SVOL [mL]	CVOL [mL]	DVOL [mL]	AREA [ON]	MEAS [ng]	CONC [ug/L]	Color		Note
								[1]	[2]	
1	100ppb Hg	0.500	5.000	5.000	73.5373	50.6006	101.2012	-	-	
2	100ppb Hg	0.500	5.000	5.000	74.0347	50.9422	101.8844	-	-	
3	100ppb Hg	0.500	5.000	5.000	73.6938	50.7081	101.4162	-	-	

Statistics

No.	NAME	TRY	AV [ug/L]	SD [ug/L]	Cv [%]
1	100ppb Hg	3	101.50060	0.3493323	0.34

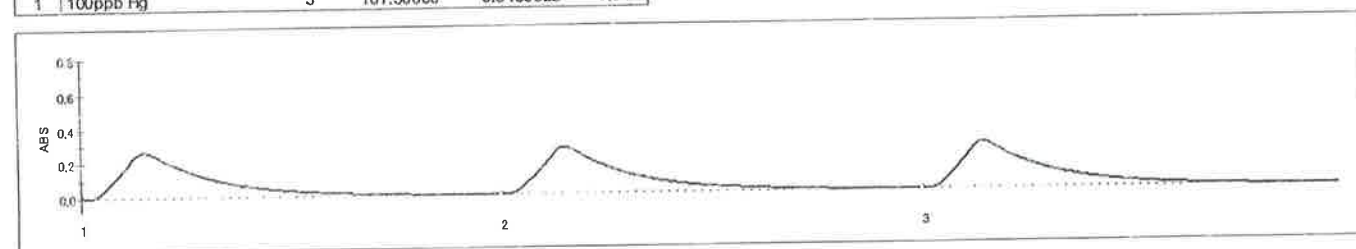

Self Check

Heat check: PASS!! (27.1degC[05:00] -> 31.2degC[03:03])
 Sensor check: PASS!! (3488- 133=3355)
 Leak check: PASS!! (0.17L/min)
 Sig/Ref check: PASS!! (Sig:3.97V, Ref:3.89V)
 Drift check: PASS!! (0.0000236 - 0.0000061 = 0.0000175)

-2-


NIC NIPPON INSTRUMENTS CORPORATION

9/2/2566 16:11

Title : RA-4500 Preventive Maintenance no.2of2 in Warranty
 Date : 9/2/2566
 Name : Coax Group Corporation Ltd.
 Memo : Calibration curve, range 0-100ng


Method


Method1 (Pretreatment: without)
 (1+1)H2SO4 : 0.9mL
 10w/v% SnCl2 : 0.5mL
 Measurement Time (sec) : 120sec



STD

No.	STD [ppb]	SVOL [mL]	CVOL [mL]	DVOL [mL]	STD [ng]	AREA [ON]	MEAS [ng]	Dev [%]	Color		Note
									[1]	[2]	
1	100.000	0.000	5.000	5.000	0.000	0.0158	0.1011	-	-	-	
2	100.000	0.050	5.000	5.000	5.000	7.4089	5.1791	3.6	-	-	
3	100.000	0.100	5.000	5.000	10.000	14.1152	9.7855	2.1	-	-	
4	100.000	0.250	5.000	5.000	25.000	35.6872	24.6026	1.6	-	-	
5	100.000	0.500	5.000	5.000	50.000	73.3032	50.4398	0.9	-	-	
6	100.000	1.000	5.000	5.000	100.000	145.2998	99.8919	0.1	-	-	

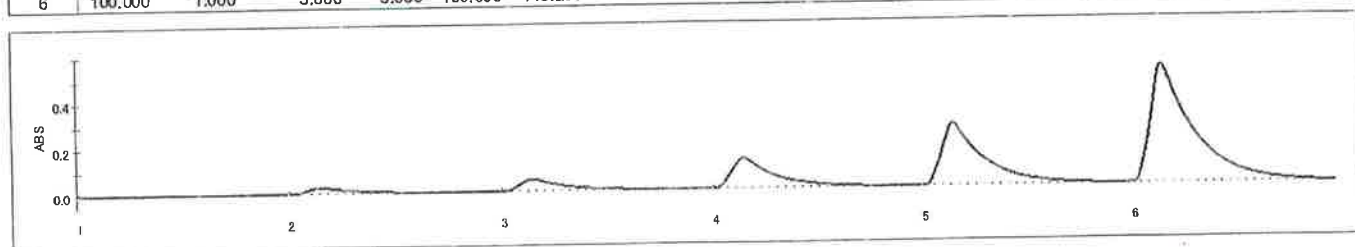



Agilent CrossLab Compliance Services

Agilent
CrossLab

From Insight to Outcome

EQUIPMENT QUALIFICATION REPORT (EQR)

Agilent CrossLab Compliance

Qualification Type:	ICPMS-OQ
System ID:	LB-ICP-03
EQP Name:	AgilentRecommended
EQP Revision:	ICPMS.02.52
EQP Publish Date:	June 2021
Date:	August 24, 2022 3:08:27 PM
Report Type:	Report with Certificate
Org. Name:	Asia Medical and Agricultural Laboratory
Org. Location:	361,361/1-4 Ladprao soi 22 Rd., Phlabphla, Khet Wang Thonglang, Bangkok 10310 Thailand

Date: August 24, 2022 3:08:27 PM
System ID: LB-ICP-03

Test Summary

Purpose

This section includes a status for each scheduled test and the overall qualification. For each test that is run, (1) the status is automatically determined based on pre-defined limits, and (2) the total number of times the test was run is displayed. For detailed results and specifications for a test, refer to the test results in this EQR.

Details

Test	Status	Runs
CDS Logon Verification	Pass	1
Autosampler Check : SPS4	Pass	1
Autotune : G8421A	Pass	1
Background (No Gas Mode) : G8421A	Pass	1
Background (Gas Modes) : G8421A	Pass	1
20-Minute Stability (No Gas Mode) : G8421A	Pass	1

Overall Qualification Status

Pass

Service Details

Purpose

This section includes local contact and delivery details for this service.

General Details

Service Order No./Request:	6005426974
EQP Name:	AgilentRecommended
EQP Revision:	ICPMS.02.52
Report Type:	Report with Certificate

Organization Details

Name:	Asia Medical and Agricultural Laboratory
Location:	361,361/1-4 Ladprao soi 22 Rd., Phlabphla, Khet Wang Thonglang, Bangkok 10310 Thailand

Local Contact Details

Name:	Ratcharin Kanjanarat
Job Title:	Laboratory Manager
Qualification Location:	3rd Floor Laboratory

Operator Details

Name:	Dachochai Wilairat
Job Title:	Field Service Engineer

Data Acquisition Details

Acquisition Software Name:	MassHunter
Acquisition Software Revision:	C.01.05
Customer Data System (CDS):	IcpMs: MassHunter

ภาคผนวก ง : หนังสืออนุญาตขึ้นทะเบียน
ห้องปฏิบัติการวิเคราะห์เอกชน



บริษัท อีสเทิร์นไทยคอนกรีตติ้ง 1992 จำกัด
เลขที่..... 235 / 2563 -
วัน..... 6 พฤศจิกายน 2563
เวลา..... 14.10

ที่ อก ๐๓๑๐(๓)/ ๑๒๕๐๐

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ เขตราชเทวี
กรุงเทพมหานคร ๑๐๕๐๐

๐๓ พฤศจิกายน ๒๕๖๓

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท อีสเทิร์น ไทย คอนกรีตติ้ง ๑๙๙๒ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๕ มิถุนายน ๒๕๖๓

- สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๓๑ ราย
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓๑ ราย
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๑๗ รายการ

ตามหนังสือที่อ้างถึง บริษัท อีสเทิร์น ไทย คอนกรีตติ้ง ๑๙๙๒ จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ๖-๐๐๓ สถานที่ตั้งเลขที่ ๖๘๓ หมู่ที่ ๑๑ ถนนสุขาภิบาล ๘ ตำบลหนองขาม อำเภอสรีราชา จังหวัดชลบุรี ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท อีสเทิร์น ไทย คอนกรีตติ้ง ๑๙๙๒ จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

- ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๓๑ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓๑ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย จำนวน ๔๓ รายการ
อากาศเสีย (ปล่องระบาย) จำนวน ๒๑ รายการ น้ำใต้ดิน จำนวน ๑๙ รายการ ดิน จำนวน ๑๖ รายการ
และสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน ๑๘ รายการ รวมทั้งสิ้นจำนวน ๑๑๗ รายการ ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๕ กรกฎาคม ๒๕๖๖ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อมารถโรงงานอุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งคำขอต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

กองวิจัยและเตือนภัยมลพิษโรงงาน
ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๘๐๕ ๗๒๖๑-๓
โทรสาร ๐ ๓๘๐๕ ๗๒๖๓

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน


บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

เลขทะเบียน ว-๐๐๓

ที่ อก ๐๓๑๐(๓)/ ๑ ๒ ๔ ๐ ๐

ลงวันที่ ๐๓ พฤศจิกายน ๒๕๖๓

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๓๑ ราย



เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน


บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

เลขทะเบียน ว-๐๐๓

ที่ ออก ๐๓๑๐(๓)/ ๑ ๒ ๕ ๐ ๐

ลงวันที่ ๐๓ พฤศจิกายน ๒๕๖๓

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓๑ ราย



เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

เลขทะเบียน ว-๐๐๓

ที่ อก ๐๓๑๐(๓)/ ๑ ๒ ๕ ๐ ๐

ลงวันที่ ๐๓ พฤศจิกายน ๒๕๖๓

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๑๗ รายการ
น้ำเสีย จำนวน 43 รายการ

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
1	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
2	Arsenic	1) Continuous Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
3	Barium	Digestion, Inductively Coupled Plasma Method ^[4]
4	α -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
5	β -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
6	δ -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
7	γ -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Membrane Electrode Method ^[4] 2) 5-Day BOD Test, Azide Modification Method ^[4]
9	Cadmium	Digestion, Inductively Coupled Plasma Method ^[4]
10	Chemical Oxygen Demand	Closed Reflux, Titrimetric Method ^[4]
11	cis-Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
12	trans-Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
13	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
14	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[4]
15	Copper	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
16	Cyanide	Distillation, Colorimetric Method ^[4]

17 4,4'-DDD...

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
17	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
18	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
19	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
20	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
21	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
22	Endosulfan sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
23	Endrin aldehyde	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
24	Endrin ketone	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
25	Formaldehyde	Distillation, Colorimetric Method ^[3]
26	Free Chlorine	1) Iodometric Method ^[4] 2) Colorimetric Method ^[c]
27	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
28	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
29	Hexavalent Chromium	Filtration, Colorimetric Method ^[4]
30	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
31	Manganese	Digestion, Inductively Coupled Plasma Method ^[4]
32	Mercury	Cold-Vapor Atomic Absorption Spectrometric Method ^[4]
33	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
34	Oil and Grease	Partition-Gravimetric Method ^[4]
35	pH	Electrometric Method ^[4]

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
36	Phenols	Distillation, Direct Photometric Method ^[4]
37	Sulfide	ZnS Precipitation, Iodometric Method ^[4]
38	Temperature	Laboratory and Field Method ^[4]
39	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Filtration, Colorimetric Method; Calculation ^[4] 2) Digestion, Inductively Coupled Plasma Method; Filtration, Colorimetric Method; Calculation ^[4]
40	Total Dissolved Solids	Dried at 180 °C ^[4]
41	Total Kjeldahl Nitrogen	Macro Kjeldahl Method ^[4]
42	Total Suspended Solids	Dried at 103-105 °C ^[4]
43	Zinc	Digestion, Inductively Coupled Plasma Method ^[4]

อากาศเสีย (ปล่อยระบาย) จำนวน 21 รายการ

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
2	Arsenic	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
3	Cadmium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
4	Carbon Monoxide	Bag, Non-Dispersive Infrared Method ^[5]
5	Chromium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
6	Cobalt	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
7	Copper	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
8	Hydrogen Sulfide	Absorption Sampling, Iodometric Method ^[5]
9	Lead	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
10	Manganese	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
11	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[5]
12	Nickel	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
13	Opacity	Ringelmann's Method ^[1]
14	Oxide of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method ^[5] 2) Instrumental Analyzer Method ^[5]
15	Selenium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
16	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method ^[5] 2) Instrumental Analyzer Method ^[5]
17	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method ^[5]
18	Tin	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
19	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method ^[5]
20	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
21	Xylene	Adsorption Sampling, Gas Chromatographic Method ^[5]

น้ำใต้ดิน จำนวน 19 รายการ

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
1	Antimony	Digestion, Inductively Coupled Plasma Method ^[4]
2	Arsenic	1) Continuous Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
3	Barium	Digestion, Inductively Coupled Plasma Method ^[4]
4	Beryllium	Digestion, Inductively Coupled Plasma Method ^[4]
5	Cadmium	Digestion, Inductively Coupled Plasma Method ^[4]
6	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
7	Cyanide	Distillation, Colorimetric Method ^[4]
8	Hexavalent Chromium	Filtration, Colorimetric Method ^[4]

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
9	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
10	Manganese	Digestion, Inductively Coupled Plasma Method ^[4]
11	Mercury	Cold-Vapor Atomic Absorption Spectrometric Method ^[4]
12	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
13	pH	Electrometric Method ^[4]
14	Phenols	Distillation, Direct Photometric Method ^[4]
15	Selenium	Digestion, Inductively Coupled Plasma Method ^[4]
16	Silver	Digestion, Inductively Coupled Plasma Method ^[4]
17	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Filtration, Colorimetric Method; Calculation ^[4] 2) Digestion, Inductively Coupled Plasma Method; Filtration, Colorimetric Method; Calculation ^[4]
18	Vanadium	Digestion, Inductively Coupled Plasma Method ^[4]
19	Zinc	Digestion, Inductively Coupled Plasma Method ^[4]

ดิน จำนวน 16 รายการ

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
1	Antimony	Digestion, Inductively Coupled Plasma Method ^[6,7]
2	Arsenic	Digestion, Inductively Coupled Plasma Method ^[6,7]
3	Barium	Digestion, Inductively Coupled Plasma Method ^[6,7]
4	Beryllium	Digestion, Inductively Coupled Plasma Method ^[6,7]
5	Cadmium	Digestion, Inductively Coupled Plasma Method ^[6,7]
6	Chromium	Digestion, Inductively Coupled Plasma Method ^[6,7]
7	Hexavalent Chromium	Alkaline Digestion, Colorimetric Method ^[9,10]
8	Lead	Digestion, Inductively Coupled Plasma Method ^[6,7]
9	Manganese	Digestion, Inductively Coupled Plasma Method ^[6,7]
10	Mercury	Digestion, Cold vapor Atomic Absorption Spectrometric Method ^[6,8]
11	Nickel	Digestion, Inductively Coupled Plasma Method ^[6,7]
12	Selenium	Digestion, Inductively Coupled Plasma Method ^[6,7]
13	Silver	Digestion, Inductively Coupled Plasma Method ^[6,7]

วิทย์ สัมฤทธิ์

(นางสาววิชุดา สัมฤทธิ์ผล)

รักษาการนักวิทยาศาสตร์ชำนาญการพิเศษ ทำหน้าที่แทน

ผู้อำนวยการศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

COPY

14 Trivalent...

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
14	Trivalent Chromium	1) Digestion, Inductively Coupled Plasma Method; Filtration, Colorimetric Method; Calculation ^[6,7] 2) Alkaline Digestion, Colorimetric Method; Calculation ^[9,10]
15	Vanadium	Digestion, Inductively Coupled Plasma Method ^[6,7]
16	Zinc	Digestion, Inductively Coupled Plasma Method ^[6,7]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 18 รายการ


ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
1	Antimony	Digestion, Inductively Coupled Plasma Method ^[6,7]
2	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
3	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
4	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
5	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
6	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
7	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
8	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
9	Hexavalent chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Alkaline Digestion, Colorimetric Method ^[9,10]

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
10	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
11	Mercury	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Cold Vapor Atomic Absorption Spectrometric Method ^[2,8] 2) Digestion, Cold vapor Atomic Absorption Spectrometric Method ^[6,8]
12	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
13	Molybdenum	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
14	Selenium	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
15	Silver	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
16	Thallium	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
17	Vanadium	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
18	Zinc	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]


เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม พ.ศ.2549 เรื่องกำหนดค่าปริมาณ
เขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แก๊สเป็นเชื้อเพลิง.
ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125 ง.

2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม พ.ศ.2548 เรื่อง การกำจัดสิ่งปฏิกูล
หรือวัสดุที่ไม่ใช้แล้ว. ราชกิจจานุเบกษา. 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 11ง.



3. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 23rd ed. Washington, DC : APHA, 2017
5. United States Environmental Protection Agency. **Standard of Performance for New Stationary Sources**. 40 CFR Part 60. Appendix A, 2019.
6. United States Environmental Protection Agency. Acid Digestion of Sediments Sludge and Soils. **SW-846 Method 3050B**, 1996.
7. United States Environment Protection Agency, Inductively Coupled Plasma-Atomic Emission spectrometry. **SW-846 Method 6010C**, 2007.
8. United States Environment Protection Agency. Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). **SW-846 Method 7471B**, 2007.
9. United States Environment Protection Agency. Alkaline digestion for Hexavalent Chromium. **SW-846 Method 3060A**, 1996.
10. United States Environment Protection Agency. Chromium. Hexavalent (Colormetric). **SW-846 Method 7196A**, 1992



COPY



บริษัท อีสเทิร์นไทย คอนซัลติ้ง จำกัด
เลขที่ ๐๔๘/๒๕๖๔
วันที่ ๒๖/๘/๖๔
เวลา ๑๕:๒๐

ที่ อก ๐๓๑๐(๓)/ ๗ ๔ ๒๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๔ สิงหาคม ๒๕๖๔

เรื่อง เปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๕ มิถุนายน ๒๕๖๔

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์
บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด จำนวน ๓ แผ่น

ตามหนังสือที่อ้างถึง บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด ห้องปฏิบัติการวิเคราะห์
เอกชน เลขทะเบียน ๖-๐๐๓ สถานที่ตั้งเลขที่ ๖๘๓ หมู่ที่ ๑๑ ถนนสุขาภิบาล ๘ ตำบลหนองขาม อำเภอสรีราชา
จังหวัดชลบุรี ขอเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

ก. ให้ยกเลิกผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย

ข. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑ ราย

ค. ให้เพิ่มเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ ราย

ง. ให้เพิ่มขอบข่ายสารมลพิษที่วิเคราะห์ในน้ำใต้ดิน จำนวน ๔๑ รายการ ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์
เอกชน ที่ อก ๐๓๑๐(๓)/๑๒๔๐๐ ลงวันที่ ๓ พฤศจิกายน ๒๕๖๓ คือในวันที่ ๕ กรกฎาคม ๒๕๖๖

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

กองวิจัยและเตือนภัยมลพิษโรงงาน
ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาค
โทร. ๐ ๓๘๐๕ ๗๒๖๑-๓
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและชนิดสารมลพิษที่วิเคราะห์
บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด เลขทะเบียน ว-๐๐๓
ที่ ออก ๐๓๑๐(๓)/ ๗๔๒๓ ลงวันที่ ๐๔ สิงหาคม ๒๕๖๔

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๔๑ รายการ
น้ำใต้ดิน จำนวน 41 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acetone	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
2	Benzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
3	Bromodichloromethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
4	Bromoform	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
5	Butanol	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
6	Carbon disulfide	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
7	Carbon tetrachloride	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
8	Chlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
9	Chlorodibromomethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
10	Chloroform	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
11	Dichloromethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
12	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
13	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
14	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method

15 1,1-Dichloroethane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
15	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
16	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
17	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
18	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
19	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
20	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
21	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
22	Ethylbenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
23	n-Hexane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
24	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
25	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method
26	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method
27	Styrene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
28	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
29	Tetrachloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
30	Toluene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
31	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
32	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
33	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
34	Trichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
35	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
36	Vinyl acetate	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
37	Vinyl chloride	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
38	m-Xylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
39	o-Xylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
40	p-Xylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
41	Xylene Total	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method

เอกสารอ้างอิง

APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater, 23rd ed. Washington, DC : APHA, 2017



ที่ อก ๐๓๑๐(๓)/ ๑ ๒ ๒๘ ๐

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๗ ธันวาคม ๒๕๖๔

เรื่อง เปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

อ้างถึง คำขอเปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๔ ตุลาคม ๒๕๖๔

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์
บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด จำนวน ๔ แผ่น

ตามที่อ้างถึง บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน
เลขทะเบียน ว-๐๐๓ สถานที่ตั้งเลขที่ ๖๘๓ หมู่ที่ ๑๑ ถนนสุขาภิบาล ๘ ตำบลหนองขาม อำเภอศรีราชา
จังหวัดชลบุรี ขอเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้เพิ่มเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย




๒. ให้เพิ่มขอบข่ายสารมลพิษที่วิเคราะห์ในน้ำเสีย จำนวน ๑ รายการ น้ำใต้ดิน จำนวน
๑ รายการ และดิน จำนวน ๔๑ รายการ รวมทั้งสิ้นจำนวน ๔๓ รายการ ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์
เอกชน ที่ อก ๐๓๑๐(๓)/๑๒๔๐๐ ลงวันที่ ๓ พฤศจิกายน ๒๕๖๓ คือในวันที่ ๕ กรกฎาคม ๒๕๖๖

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



กองวิจัยและเตือนภัยมลพิษโรงงาน
ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๘๐๕ ๗๒๖๑-๓
ไปรษณีย์อิเล็กทรอนิกส์ einw@diw.mail.go.th



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและชนิดสารมลพิษที่วิเคราะห์

บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

เลขทะเบียน ว-๐๐๓

ที่ อก ๐๓๑๐(๓)/ ๑๒๒๘๐

ลงวันที่ ๐๗ ธันวาคม ๒๕๖๕

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๔๓ รายการ
น้ำเสีย จำนวน 1 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrophotometer Method ^[1]

น้ำใต้ดิน จำนวน 1 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrophotometer Method ^[1]

ดิน จำนวน 41 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acetone	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
2	Benzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
3	Bromodichloromethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
4	Bromoform	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
5	Butanol	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
6	Carbon disulfide	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
7	Carbon tetrachloride	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]


ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
8	Chlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
9	Chlorodibromomethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
10	Chloroform	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
11	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
12	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
13	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
14	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
15	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
16	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
17	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
18	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
19	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
20	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
21	Ethylbenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
22	n-Hexane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
23	Methylene Chloride	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
24	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
25	Naphthalene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
26	Nitrobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
27	Styrene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
28	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
29	Tetrachloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
30	Toluene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
31	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
32	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
33	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
34	Trichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
35	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
36	Vinyl Acetate	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
37	Vinyl Chloride	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
38	m-Xylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
39	o-Xylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
40	p-Xylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
41	Xylene (Total)	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]

เอกสารอ้างอิง

1. APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 23rd ed. Washington, DC : APHA, 2017
2. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples. SW-846 Method 5035A, 2002.
3. United States Environment Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8260D, 2018.



ที่ อก ๐๓๒๐/ ๑๒๒๔ ๓



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๒ กันยายน ๒๕๖๕

เรื่อง เปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท อีสเทิร์น ไทย คอนซัลติง ๑๙๙๒ จำกัด


อ้างถึง คำขอเปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒๐ กรกฎาคม ๒๕๖๕

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์
บริษัท อีสเทิร์น ไทย คอนซัลติง ๑๙๙๒ จำกัด จำนวน ๕ แผ่น

ตามคำขอที่อ้างถึง บริษัท อีสเทิร์น ไทย คอนซัลติง ๑๙๙๒ จำกัด ห้องปฏิบัติการวิเคราะห์
เอกชน เลขทะเบียน ว-๐๐๓ สถานที่ตั้งเลขที่ ๖๘๓ หมู่ที่ ๑๑ ถนนสุขาภิบาล ๘ ตำบลหนองขาม อำเภอสรีราชา
จังหวัดชลบุรี ขอเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓ ราย

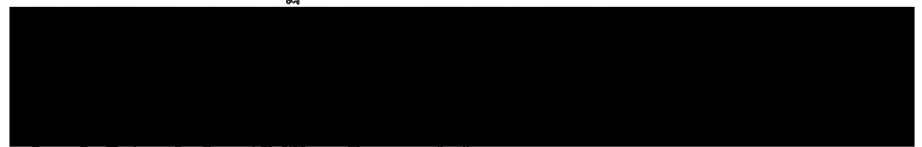


๒. ให้เพิ่มเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย



๓. ให้เพิ่มขอบข่ายสารมลพิษที่วิเคราะห์ในน้ำใต้ดิน จำนวน ๓๘ รายการ และดิน จำนวน
๓๘ รายการ รวมทั้งสิ้นจำนวน ๗๖ รายการ ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ที่ อก ๐๓๑๐(๓)/๑๒๔๐๐ ลงวันที่ ๓ พฤศจิกายน ๒๕๖๓ คือในวันที่ ๕ กรกฎาคม ๒๕๖๖ ทั้งนี้ สามารถยื่น
คำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ท้ายหนังสือนี้


จึงเรียนมาเพื่อทราบ



ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๓๑๓ ๖๐๕๕ ต่อ ๕๐๐๑-๒
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกัน”



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและชนิดสารมลพิษที่วิเคราะห์
บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด เลขทะเบียน ว-๐๐๓
ที่ ออก ๐๓๒๐/ ๑ ๒ ๒ ๔ ๓ ลงวันที่ ๐ ๒ กันยายน ๒๕๖๕

ขอข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๗๖ รายการ
น้ำใต้ดิน จำนวน 38 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
2	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
3	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
4	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
5	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
6	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
7	Benzo(g,h,i)perylene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
8	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
9	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
10	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
11	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
12	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
13	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
14	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
15	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
16	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
17	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
18	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
19	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
20	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
21	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
22	Di-n-octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
23	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
24	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
25	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
26	Hexachloro-1,3-butadiene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
27	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
28	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
29	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
30	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
31	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
32	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾

Nitrosodi...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
33	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
34	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
35	Phenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
36	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
37	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
38	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]

ดิน จำนวน 38 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
2	Anthracene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
3	Benz(a)anthracene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
4	Benzo(b)fluoranthene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
5	Benzo(k)fluoranthene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
6	Benzo(a)pyrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
7	Benzo[g,h,i]perylene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
8	Bis(2-chloroethyl)ether	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
9	Bis(2-ethylhexyl)phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
10	Butyl benzyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
11	Carbazole	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
12	p-Chloroaniline	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
13	2-Chlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
14	Chrysene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
15	Dibenz(a,h)anthracene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
16	Di-n-butyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
17	2,4-Dichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
18	Diethyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
19	2,4-Dimethylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
20	2,4-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
21	2,6-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
22	Di-n-octyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
23	Fluoranthene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
24	Fluorene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
25	Hexachlorobenzene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
26	Hexachloro-1,3-butadiene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]

27 Hexachloro

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	Hexachlorocyclopentadiene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
28	Hexachloroethane	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
29	Indeno(1,2,3-cd)pyrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
30	Isophorone	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
31	2-Methylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
32	2-Methylnaphthalene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
33	N-Nitrosodi-n-propylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
34	Phenanthrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
35	Phenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
36	Pyrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
37	2,4,5-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
38	2,4,6-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]

เอกสารอ้างอิง

1. APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 23rd ed. Washington, DC : APHA; 2017
2. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Ultrasonic Extraction. SW-846 Method 3550C, 2007
3. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270