




## ภาคผนวก ฉ

---

เอกสารสอบเทียบเครื่องมือ



การตรวจวัดคุณภาพสิ่งแวดล้อม  
การเปลี่ยนแปลงรายละเอียดโครงการทุนผูกเรือ ท่อส่งน้ำมันใต้ทะเลและคลังน้ำมัน (ย้ายตำแหน่งที่ตั้งสถานีไฟฟ้าย่อย)  
ระหว่างเดือนมกราคม-มิถุนายน พ.ศ. 2566

รายการใบรับรองสอบเทียบ ทวนสอบ เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับคุณภาพน้ำ

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์สำหรับคุณภาพน้ำ									
1	Turbidity Meter	ความขุ่น	Oakton	T100IR / 1120501017	Technology Promotion Association (Thailand-Japan)	22CH1184	5 Sep 22	4 Sep 23	-
2	Analytical Balance (Repeatability 0.01 mg)	สารแขวนลอย	Mettler-Toledo	XSR205DU / C009071872	Calibration Laboratory Mettler-Toledo (Thailand) Limited	2102573-001-01	26 Apr 22	25 Apr 23	-
3	Hot Air Oven		Memmert	UF55 / B216.1666	Technology Promotion Association (Thailand-Japan)	22TM1490	19 Oct 22	18 Oct 23	-
4	BOD Incubator	บีโอดี	Arco	UC4-1320 / (UAE.LAB.015/2561)	Technology Promotion Association (Thailand-Japan)	22TM90	17 Feb 22	16 Feb 23	-
5	BOD Incubator		Arco	UR-1320 / (UAE.LAB.018/2551)	Technology Promotion Association (Thailand-Japan)	22TM305	7 Apr 22	6 Apr 23	-
6	Analytical Balance (Repeatability 0.1 mg)	น้ำมันและไขมัน	Mettler-Toledo	AB-204S/FACT / 1129361010	National Food Institute, Ministry of Industry, Thailand	2203120-001-01	1 Jun 22	31 May 23	-
7	Incubator	ปริมาณโคลิฟอร์มแบคทีเรียทั้งหมด	Memmert	IPP 260 / V616.0066	Technology Promotion Association (Thailand-Japan)	22TM672	5 May 22	4 May 23	-
8	Incubator		Memmert	IPP 260 / V615.0187	Technology Promotion Association (Thailand-Japan)	22TM563	7 Apr 22	6 Apr 23	-
9	Water Bath		Memmert	WNE 14 / L416.0606	Technology Promotion Association (Thailand-Japan)	22TM333	17 Feb 22	16 Feb 23	-
10	Water Bath		Memmert	WNE 14 / L416.0612	Technology Promotion Association (Thailand-Japan)	22TM334	17 Feb 22	16 Feb 23	-
11	Analytical Balance		Mettler-Toledo	MS603S / B0070110311	National Food Institute, Ministry of Industry, Thailand	2058-096-040722-ACC	7 Apr 22	6 Apr 23	-
12	Autoclave		ALP	CL-40L / 802664	Technology Promotion Association (Thailand-Japan)	22TM89	17 Feb 22	16 Feb 23	-
13	Autoclave		ALP	CL-40L / 808763	National Food Institute, Technology Promotion Association	22TM681	27 May 22	26 May 23	-

Due Date of Calibration\* : Based on the annual calibration plan. At least 1 time per year.



Cert.No.: 22CH1184  
Page.: 1 of 2

## Certificate of Calibration

Equipment : Turbidity Meter  
Manufacturer : Oakton  
Model : T100IR  
Serial No. : 1120501017  
ID. No. : UAE.WAT.056/2563  
Condition As-Received: Used Item  
Received Date : 31 August 2022  
Calibration Date : 05 September 2022  
Reference : 2208-1106WSC-1  
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260  
Ambient Temperature : (25 ± 2.5) °C  
Relative Humidity : (50 ± 20) %  
Calibration Procedure : In - house method : CP-CH11  
based on direct measurement by  
using Formazin standard solution

Calibrated by : Walalak Sirithean

Approved by :   
Approved Signatory

(✓) Malee Butkruea  
( ) Sathip Meangmai  
( ) Warakorn Lernagatrakul

Issue Date : 6 September 2022

The Uncertainties are for a confidence probability of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written  
approval of the head of Calibration and Testing Equipment Services.

เอกสารไม่ควบคุม

A 0009588



Cert.No.: 22CH1184  
Page.: 2 of 2

### Condition of this calibration result

- Reference Standard Instruments :  
This certification is traceable to the International System of unit (SI unit) through  
Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due date
1) Thermo-Hygrograph	1103328	130EC010	22H1313	12 June 2023
2) Electronic Balance	N03679	140RC001	21MM429	21 Sep 2022

- Standard Material : The Formazin suspension has been prepared gravimetric from

Material	Manufacturer	Lot No.	Assay
1) Hexamethylenetetramine	HIMEDIA	0000493947	99.65%
2) Hydrazinium Sulfate	HIMEDIA	0000522014	99.40%

- This certificate is valid only to the item calibrated on date and place of calibration.

### Calibration result

Performing five - Formazin suspension standard curve by using 0,20,100,400,800 NTU  
Turbidity Meter Serial Number : 1120501017

Standard Formazine suspension ( NTU )	UUC* Reading ( NTU )	Uncertainty of Measurement ( ± NTU )	Coverage Factor k
0	0.00	0.0062	2.00
20	20.1	0.39	2.00
100	102	0.74	2.00
400	403	1.5	2.13
800	804	2.1	2.20

Remark - UUC\* = Unit Under Calibration  
- NTU = Nephelometric Turbidity Units

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage  
factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

a 1124976



Cert.No.: 22MM210  
Page.: 1 of 3

## Certificate of Calibration

Equipment : Electronic Balance  
Manufacturer : Mettler Toledo  
Model : XSR205  
Serial No. : C009071872  
ID No. : UAE.WAO.012/2563  
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phakhanong,  
Bangkok 10260

Location : Balance Room

Received order : 26 April 2022  
Calibration Date : 26 April 2022  
Ambient Temperature : 15 °C to 40 °C  
Relative Humidity : 30 % to 90 %

Calibrated by : Kunchit Promprap

Approved by :   
Approved Signatory

( ) Pornthippa Tameyakul  
(✓) Malee Butkruea  
( ) Suwit Imjai

Issue Date : 29 April 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2204-0542OC-1

Cert.No.: 22MM210  
Page: 2 of 3

### Procedure used :-

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct  
measurement method against standard weight.

### Condition of this result of calibration

- Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	-	70RC138	MM-0009-21	3 Feb 2023

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certification is traceable to the International System of Unit.

Result of calibration ( ) Without Adjustment ( \* ) After Adjustment by Internal Calibration

Range capacity : 0 g to 81 g Resolution 0.00001 g  
81 g to 220 g Resolution 0.0001 g

### Before Adjustment :

Applied Weight ( g )	Balance Reading ( g )	Correction ( g )	Measurement Uncertainty ( ± mg )	Coverage Factor ( k )
80	80.00004	-0.00004	0.15	2.00
200	199.9999	+0.0001	0.35	2.00

### After Adjustment :

- Determination of the standard deviation of weighing machine ( n = 10 )

Applied Weight ( g )	Standard Deviation of Reading ( g )
80	0.000008
200	0.000005


เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2204-0542OC-1

Cert.No.: 22MM210  
Page: 3 of 3



Maximum difference between  
off-center and central loading

Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)	(g)
-0.0002	-0.0001	0.0000	-0.0002	-0.0002	0.0002

### 3. Departure from nominal value

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty ( $\pm$ mg)	Coverage Factor (k)
Unload	0.00000	0.00000	0.016	2.13
0.05	0.05001	-0.00001	0.016	2.13
0.1	0.10001	-0.00001	0.017	2.11
1	1.00002	-0.00002	0.019	2.05
5	5.00003	-0.00003	0.026	2.00
20	20.00008	-0.00008	0.049	2.00
50	50.00010	-0.00010	0.080	2.00
80	80.00014	-0.00014	0.15	2.00
100	100.0001	-0.0001	0.21	2.00
150	150.0001	-0.0001	0.29	2.00
200	200.0001	-0.0001	0.35	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1490  
Page: 1 of 3

## Certificate of Calibration

Equipment : Hot Air Oven  
Manufacturer : Memmert  
Model : UF 55  
Serial No. : B216.1666  
ID No. : UAE.WAO.027/2559  
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udornasuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
Location : Lab Floor 2  
Received Order : 19 October 2022  
Calibration Date : 19 October 2022  
Ambient Temperature : ( 26  $\pm$  10 ) °C  
Relative Humidity : ( 50  $\pm$  30 ) %  
Calibrated by : Preecha Hlahib  
Approved by :   
( ) Pornthippa Tameyakul  
( ) Malee Butkrua  
(✓) Suwit Imjai

Issue Date : 31 October 2022

The Uncertainties are for a confidence probability of approximately 95 %

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0046800



Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2210-0575OC-1

Cert. No.: 22TM1490  
Page: 2 of 3

### Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

### Condition of this result of calibration

#### 1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34970A	MY41021843	22LM4	10 Jan 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- ( \* ) Without Adjustment

Function of UUC\* : Temperature Source

Fresh air setting : Close



Probe Installation Details : Dimension of Chamber :  
a = 5.0 cm D = 0.33 m  
b = 5.0 cm W = 0.40 m  
c = 5.0 cm H = 0.40 m  
Capacity = 0.053 m<sup>3</sup>

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	29	30
REL.Humid. ( % )	47	40
AC Supply ( Volt )	221	220

Ref. Std. ID No.: @ Calibration Point		
Position :	( 104 ) °C	( 140,180 ) °C
1	18-04RTD-01	21-04TC-01
2	18-04RTD-02	21-04TC-02
3	18-04RTD-03	21-04TC-03
4	18-04RTD-04	21-04TC-04
5	18-04RTD-05	21-04TC-05
6	18-04RTD-06	21-04TC-06
7	18-04RTD-07	21-04TC-07
8	18-04RTD-08	21-04TC-08
9 (ref.)	18-04RTD-09	21-04TC-09

เอกสารไม่ควบคุม

a 1133252



Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2210-0575OC-1  
Result of Calibration :- ( \* ) Without Adjustment

Cert. No.: 22TM1490  
Page: 3 of 3

Function of UUC\* : Temperature Source

Fresh air setting : Close

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( $\pm$ °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( $\pm$ °C )	Coverage Factor k
104.0	104.0	104.0	0.061	1.3	1.7	0.42	2
140.0	140.0	140.0	0.14	2.3	2.4	1.1	2
180.0	180.0	180.0	0.21	3.5	3.0	1.3	2

Measured Temperature ( °C )									
Calibration Point ( °C )	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	103.076	103.876	103.777	104.124	104.667	104.426	104.012	103.928	104.370
140.0	138.199	139.189	138.808	139.550	140.266	139.622	139.293	139.385	140.369
180.0	177.930	179.267	178.643	179.753	181.011	180.093	179.496	179.743	181.278

Average\* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation UUC\* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม

a 1133251





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM90  
Page.: 1 of 3

## Certificate of Calibration

**Equipment :** BOD Incubator  
**Manufacturer :** Arco  
**Model :** UC4-1320  
**Serial No. :** 13URC4S013201  
**ID No. :** UAE.WAO.015/2561  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
**Location :** Lab Floor 2  
**Received Order :** 17 February 2022  
**Calibration Date :** 17 February 2022  
**Ambient Temperature :** (26 ± 10) °C  
**Relative Humidity :** (50 ± 30) %  
**Calibrated by :** Kunchit Promprat

**Approved by :**   
( ) Ponthippa Tameyakul  
(✓) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 22 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม  
A 0038099



**Equipment :** BOD Incubator  
**Condition As-Received :** Used Item  
**Reference :** 2202-0446OC-1

**Cert. No.:** 22TM90  
**Page.:** 2 of 3

### Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).  
The temperature scale used was based on ITS-90.

### Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44035217	21LM30	23 Dec 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Not Available



**Probe Installation Details :**

**Dimension of Chamber :**  
a = 10 cm D = 0.62 m  
b = 10 cm W = 1.2 m  
c = 10 cm H = 1.2 m  
Capacity = 0.89 m<sup>3</sup>

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	28	28
REL.Humid. ( % )	68	75
AC Supply ( Volt )	226	226

Position :	Ref. Std. ID No.:
1	18-10RTD-01
2	18-10RTD-02
3	18-10RTD-03
4	18-10RTD-04
5	18-10RTD-05
6	22-10RTD-10
7	18-10RTD-07
8	18-10RTD-08
9 (ref.)	18-10RTD-09

เอกสารไม่ควบคุม  
A 1096042



**Equipment :** BOD Incubator  
**Condition As-Received :** Used Item  
**Reference :** 2202-0446OC-1  
**Result of Calibration :-** ( \* ) Without Adjustment  
**Function of UUC\* :** Temperature Source  
**Fresh air setting :** Not Available

**Cert. No.:** 22TM90  
**Page.:** 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( ± °C )	Coverage Factor k
20.0	19.5	19.4	0.30	0.58	1.0	0.55	2

Calibration Point ( °C )	Measured Temperature ( °C )								
	Position								
20.0	1	2	3	4	5	6	7	8	9 (ref.)
	20.154	20.013	20.356	19.939	19.834	19.761	19.817	19.824	19.922

**Average\* :** The average of 30 values in each position.

**Temperature stability :** One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation :** The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม  
A 1096041



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



**Cert. No.:** 22TM305  
**Page.:** 1 of 3

## Certificate of Calibration

**Equipment :** BOD Incubator  
**Manufacturer :** ARCO  
**Model :** UR 1320  
**Serial No. :** -  
**ID No. :** UAE.WAO.018/2551  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
**Location :** Lab Floor 2  
**Received Order :** 7 April 2022  
**Calibration Date :** 7 April 2022  
**Ambient Temperature :** (26 ± 10) °C  
**Relative Humidity :** (50 ± 30) %  
**Calibrated by :** Man Pattanapongpaiboon

**Approved by :**   
( ) Ponthippa Tameyakul  
(✓) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 18 April 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม  
A 0040246



## Calibration Report

**Certificate No.:** 2203120-001-01  
**Equipment:** Electronic Balance  
**Model:** AS204-S/FACT  
**Serial No.:** 1129361010  
**Capacity:** 220 g  
**Manufacturer:** METTLER TOLEDO  
**Resolution:** 0.0001 g  
**ID No.:** UAE.WAS.002/2552

**Date of Calibration:** 1 June 2022 **Page 3 of 3**

**Calibration Results:** (Continued)  
**Calibration Range:** 0 - 200 g  
**Calibration Adjustment:** Internal Calibration

### 3. Departure from Nominal Value:

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.00000	0.0000	0.0000	0.000088	2.00
0.01	0.01000	0.0100	0.0000	0.000088	2.00
0.05	0.05000	0.0499	0.0001	0.000088	2.00
0.1	0.10000	0.1000	0.0000	0.000088	2.00
0.2	0.20000	0.2000	0.0000	0.000088	2.00
0.5	0.50000	0.5000	0.0000	0.000088	2.00
1	1.00000	0.9999	0.0001	0.000088	2.00
2	2.00000	1.9999	0.0001	0.000089	2.00
5	5.00000	5.0000	0.0000	0.000089	2.00
10	9.99998	9.9999	0.0001	0.000092	2.00
20	19.99999	19.9999	0.0001	0.000094	2.00
50	49.99990	49.9999	0.0000	0.00012	2.00
70	69.99989	69.9998	0.0001	0.00014	2.00
100	100.00001	99.9999	0.0001	0.00017	2.00
150	149.99991	149.9997	0.0002	0.00022	2.00
200	200.00007	199.9998	0.0003	0.00030	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

**Cert. No.:** 22TM672  
**Page.:** 1 of 3

## Certificate of Calibration

**Equipment :** Incubator  
**Manufacturer :** Memmert  
**Model :** IPP 260  
**Serial No. :** V616.0066  
**ID No. :** UAE.MIC.032/2559  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
**Location :** Microbiology Laboratory (302)  
**Received Order :** 3 May 2022  
**Calibration Date :** 5 May 2022  
**Ambient Temperature :** ( 26 ± 10 ) °C  
**Relative Humidity :** ( 50 ± 30 ) %  
**Calibrated by :** Preecha Hlahib  
**Approved by :**   
( ) Pornthippa Tameyakul  
(✓) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 11 May 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



**Equipment :** Incubator  
**Condition As-Received :** Used Item  
**Reference :** 2205-0003OC-3

**Cert. No.:** 22TM672  
**Page.:** 2 of 3

### Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).  
The temperature scale used was based on ITS-90.

### Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34970A	MY44067817	21LM10	20 Jul 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.  
3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Not Available



**Probe Installation Details :**  
a = 5.0 cm  
b = 5.0 cm  
c = 5.0 cm  
**Dimension of Chamber :**  
D = 0.50 m  
W = 0.60 m  
H = 0.80 m  
Capacity = 0.24 m<sup>3</sup>

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	25	23
REL.Humid. ( % )	62	57
AC Supply ( Volt )	221	221

Position :	Ref. Std. ID No.:
1	19-15RTD-01
2	19-15RTD-02
3	19-15RTD-03
4	19-15RTD-04
5	19-15RTD-05
6	21-15RTD-06
7	19-15RTD-07
8	19-15RTD-08
9 (ref.)	19-15RTD-09

เอกสารไม่ควบคุม



**Equipment :** Incubator  
**Condition As-Received :** Used Item  
**Reference :** 2205-0003OC-3  
**Result of Calibration :-** ( \* ) Without Adjustment  
**Function of UUC\* :** Temperature Source  
**Fresh air setting :** Not Available

**Cert. No.:** 22TM672  
**Page.:** 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( ± °C )	Coverage Factor k
25.0	25.0	25.0	0.021	0.18	0.33	0.30	2
36.0	36.0	36.0	0.077	0.96	1.8	0.33	2

Calibration Point ( °C )	Measured Temperature ( °C )								
	Position								
25.0	25.221	25.146	25.127	25.113	24.968	24.986	24.933	25.017	25.047
36.0	35.637	35.238	36.130	36.515	36.928	36.845	36.630	36.761	36.113

**Average\* :** The average of 30 values in each position.

**Temperature stability :** One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation :** The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM563  
Page: 1 of 3

## Certificate of Calibration

**Equipment :** Incubator  
**Manufacturer :** Memmert  
**Model :** IPP 260  
**Serial No. :** V615.0187  
**ID No. :** UAE.MIC.003/2559  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
**Location :** Microbiology Laboratory  
**Received Order :** 7 April 2022  
**Calibration Date :** 7 April 2022  
**Ambient Temperature :** (26 ± 10) °C  
**Relative Humidity :** (50 ± 30) %

**Calibrated by :** Prawit Sodavitchit

**Approved by :**   
Approved Signatory  
( ) Pormthippa Tameyakul  
(✓) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 18 April 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0040248



**Equipment :** Incubator  
**Condition As-Received :** Used Item  
**Reference :** 2204-0016OC-1

Cert. No.: 22TM563  
Page: 2 of 3

### Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

### Condition of this result of calibration

#### 1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34970A	MY44067817	21LM10	20 Jul 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certificate is traceable to the International System of Unit

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	26	26
REL.Humid. ( % )	60	62
AC Supply ( Volt )	220	220



#### Probe Installation Details :

a = 5.0 cm	D = 0.50 m
b = 5.0 cm	W = 0.64 m
c = 5.0 cm	H = 0.80 m
	Capacity = 0.26 m³

Position :	Ref. Std. ID No.:
1	15RTD2/11
2	15RTD2/12
3	15RTD2/13
4	15RTD2/14
5	15RTD2/15
6	15RTD2/16
7	15RTD2/17
8	15RTD2/18
9 (ref.)	15RTD2/19

เอกสารไม่ควบคุม

a 1104310



**Equipment :** Incubator  
**Condition As-Received :** Used Item  
**Reference :** 2204-0016OC-1  
**Result of Calibration :-** ( \* ) Without Adjustment  
**Function of UUC\* :** Temperature Source  
**Fresh air setting :** Close

Cert. No.: 22TM563  
Page: 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( ± °C )	Coverage Factor k
35.0	35.0	35.0	0.12	0.53	0.79	0.30	2

Calibration Point ( °C )	Measured Temperature ( °C )							
	Position							
	1	2	3	4	5	6	7	8
35.0	35.170	35.167	34.938	34.844	34.816	34.854	34.584	34.730
								9 (ref.) 34.780

**Average\* :** The average of 30 values in each position.

**Temperature stability :** One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation :** The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

a 1104309



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM333  
Page: 1 of 3

## Certificate of Calibration

**Equipment :** Water Bath  
**Manufacturer :** Memmert  
**Model :** WNE 14  
**Serial No. :** L416.0606  
**ID No. :** UAE.MIC.002/2560  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
**Location :** Microbiology Laboratory  
**Received Order :** 17 February 2022  
**Calibration Date :** 17 February 2022  
**Ambient Temperature :** (26 ± 10) °C  
**Relative Humidity :** (50 ± 30) %  
**Calibrated by :** Suwit Imjai

**Approved by :**   
Approved Signatory  
( ) Pormthippa Tameyakul  
( ) Malee Butkruea

**Issue Date :** 22 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Water Bath  
 Condition As-Received : Used Item  
 Reference : 2202-0444OC-3  
 Cert. No.: 22TM333  
 Page.: 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

**1. Reference standard instrument:-**

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	21LM10	20 Jul 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

	Environmental		AC Voltage Supply
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	21	65	229
Finished of Calibration	22	58	230



Front

Position :	Ref. Std. ID No.:
1	70RC143
2	70RC144
3	70RC145
4	70RC146
5(ref.)	70RC147

เอกสารไม่ควบคุม



Equipment : Water Bath  
 Condition As-Received : Used Item  
 Reference : 2202-0444OC-3  
 Cert. No.: 22TM333  
 Page.: 3 of 3

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

Calibration point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Average* Standard Reading ( °C )				
			Position				
			1	2	3	4	5 (ref.)
44.5	44.5	44.5	44.498	44.481	44.482	44.518	44.534

Calibration point ( °C )	Uniformity ( °C )	Stability ( ± °C )	Uncertainty ( ± °C )	Coverage Factor k
44.5	0.13	0.057	0.15	2

**Average\* :** The average of 30 values in each position.

**Uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Stability :** One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
 CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
 534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
 TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM334  
 Page.: 1 of 3

## Certificate of Calibration

**Equipment :** Water Bath  
**Manufacturer :** Memmert  
**Model :** WNE 14  
**Serial No. :** L416.0612  
**ID No. :** UAE.MIC.003/2560  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
 3 Soi Udomsuk 41, Sukhumvit Road,  
 Bangchak, Phrakhanong,  
 Bangkok 10260  
**Location :** Microbiology Laboratory  
**Received Order :** 17 February 2022  
**Calibration Date :** 17 February 2022  
**Ambient Temperature :** ( 26 ± 10 ) °C  
**Relative Humidity :** ( 50 ± 30 ) %  
**Calibrated by :** Suwit Imjai

**Approved by :**   
 ( ) Ponthippa Tameyakul  
 ( / ) Malee Butkruea

**Issue Date :** 22 February 2022

The Uncertainties are for a confidence probability of approximately 95 %

This certificate may not be reproduced other than in full, except with the prior written  
 Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0038095



Equipment : Water Bath  
 Condition As-Received : Used Item  
 Reference : 2202-0444OC-4  
 Cert. No.: 22TM334  
 Page.: 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

**1. Reference standard instrument:-**

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	21LM10	20 Jul 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

	Environmental		AC Voltage Supply
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	21	65	229
Finished of Calibration	22	57	230



Front

Position :	Ref. Std. ID No.:
1	70RC143
2	70RC144
3	70RC145
4	70RC146
5(ref.)	70RC147

เอกสารไม่ควบคุม

a 1096055



Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2202-0444OC-4  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 22TM334  
Page.: 3 of 3

Calibration point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Average* Standard Reading ( °C )				
			Position				
			1	2	3	4	5 (ref.)
44.5	44.5	44.5	44.572	44.514	44.507	44.530	44.565

Calibration point ( °C )	Uniformity ( °C )	Stability ( ± °C )	Uncertainty ( ± °C )	Coverage Factor k
44.5	0.10	0.042	0.15	2

**Average\*** : The average of 30 values in each position.

**Uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Stability** : One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม  
a 1096054

Calibration Certificate ID  
TH2058-096-040722-ACC-TH

METTLER TOLEDO

Mettler-Toledo (Thailand) Ltd.  
846/4 - 846/5 Lasalle Rd., Bangna Tai Sub-District  
Bangna District, Bangkok 10260  
+66 2723 0392  
MT-TH.ServiceSupport@mt.com



## Accuracy Calibration Certificate

### Customer

Company: United Analyst and Engineering Consultant Co., Ltd.  
Address: 3 Soi Udom Suk 41, Sukhumvit Rd., Bang Chak  
City: Phra Khanong  
Zip / Postal: 10260  
State / Province: Bangkok  
Order Number: 

Contact: Suwit Chotnok

### Weighing Device

Manufacturer: Mettler Toledo  
Model: MS603S/01  
Serial No.: B007010311  
Building: N/A  
Floor: 2  
Room: Balance Room (206)

Instrument Type: Weighing Instrument  
Asset Number: UAE.MIC.008/2553  
Terminal Model: N/A  
Terminal Serial No.: N/A  
Terminal Asset No.: N/A

Range	Max. Capacity	Readability (d)
1	620 g	0.001 g

### Procedure

Calibration Guideline: EURAMET cg-18 v. 4.0 (11/2015)  
Mettler TOLEDO Work Instruction: CP/W00220

This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.

The sensitivity/span of the weighing instrument was adjusted before calibration with a built-in weight.

In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

Temperature		Humidity	
As Found	Start: 22.8 °C End: 23.0 °C	Start: 49.9 %	End: 58.3 %

As Found Calibration Date: 07-Apr-2022  
As Left Calibration Date: N/A  
Issue Date: 08-Apr-2022

Calibrator:

Siravit Chanchan

Approved Signatory:

  
☒ Kasakorn Tassanachaisakul  
☐ Santi Jitniyom  
☐ Surachet Sukkate

Software Version: 1.23.0.268  
Report Version: 2.16.13  
Form Number: F103C

© METTLER TOLEDO  
This is an original document and may not be partially reproduced without the written permission of the issuing calibration laboratory.

Page 1 of 5

เอกสารไม่ควบคุม

Calibration Certificate ID  
TH2058-096-040722-ACC-TH

METTLER TOLEDO Service


## Measurement Results

### Repeatability

Test Load: 200 g

	As Found	As Left
1	200.001 g	N/A
2	200.001 g	N/A
3	200.001 g	N/A
4	200.001 g	N/A
5	200.001 g	N/A
6	200.000 g	N/A
7	200.001 g	N/A
8	200.001 g	N/A
9	200.000 g	N/A
10	200.001 g	N/A

Standard Deviation	0.0004 g	N/A
--------------------	----------	-----




The "1d" in the graph represents the readability of the range/interval in which the test was performed.  
The results of this graph are based upon the absolute values of the differences from the mean value.

### Eccentricity

Test Load: 200 g

Position	As Found	As Left
1	200.001 g	N/A
2	200.001 g	N/A
3	200.002 g	N/A
4	200.002 g	N/A
5	200.000 g	N/A

Maximum Deviation	0.001 g	N/A
-------------------	---------	-----



The "1d" in the graph represents the readability of the range/interval in which the test was performed.

Software Version: 1.23.0.268  
Report Version: 2.16.13  
Form Number: F103C

© METTLER TOLEDO  
This is an original document and may not be partially reproduced without the written permission of the issuing calibration laboratory.

เอกสารไม่ควบคุม

Page 2 of 5


Calibration Certificate ID  
TH2058-096-040722-ACC-TH

METTLER TOLEDO Service

## Error of Indication

As Found

	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.000 g	0.000 g	0.000 g	1.0 mg	2
2	0.500 g	0.500 g	0.000 g	1.2 mg	2
3	1.000 g	1.000 g	0.000 g	1.2 mg	2
4	50.000 g	50.000 g	0.000 g	1.2 mg	2
5	100.000 g	100.000 g	0.000 g	1.3 mg	2
6	150.000 g	150.000 g	0.000 g	1.5 mg	2
7	200.000 g	200.001 g	0.001 g	1.6 mg	2
8	300.001 g	300.001 g	0.000 g	2.0 mg	2
9	400.001 g	400.001 g	0.000 g	2.5 mg	2
10	500.002 g	500.002 g	0.001 g	2.9 mg	2
11	600.001 g	600.001 g	0.000 g	3.4 mg	2

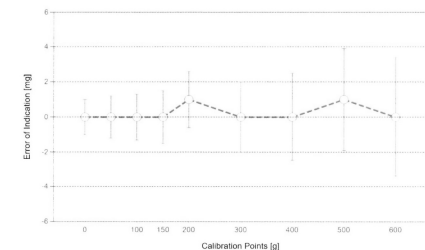

The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor  $k$  - which can be larger than 2 according to EURAMET cg-18. The value of the measurand lies within the assigned range of values with a probability of approximately 95%.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.

Software Version: 1.23.0.268  
Report Version: 2.16.13  
Form Number: F103C

© METTLER TOLEDO  
This is an original document and may not be partially reproduced without the written permission of the issuing calibration laboratory.

เอกสารไม่ควบคุม

Page 3 of 5

### Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

#### Weight Set 1: OIML F1

Weight Set No.: WS55 Date of Issue: 09-Jul-2021  
Certificate Number: CCM-0137-21-C Calibration Due Date: 07-Jul-2022

#### Weight Set 2: OIML E2

Weight Set No.: WS80 Date of Issue: 23-Feb-2022  
Certificate Number: C208581631 Calibration Due Date: 14-Aug-2023

#### Thermo Hygrometer

Equipment No.: IN161 Date of Issue: 14-Jun-2021  
Certificate Number: 21H1220 Calibration Due Date: 01-Jun-2022

### Remarks

FACT adjustment functionality activated  
Equipment condition: Good  
Next calibration according to customer's procedure  
Calibration data not decide by calibration laboratory

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

### Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with  $k=2$  in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use:  $3.0 \cdot 10^{-5} / K$

Temperature range on site for the evaluation of the measurement uncertainty in use: 3 K


#### Linearization of Uncertainty Equation

Range		As Found		As Left	
d	Max				
1	0.001 g	620 g	$U_1 = 1.2 \text{ mg} + 0.0186 \text{ mg/g} \cdot R$		N/A

To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

#### Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication	As Found	As Left
0.062 g	1.2 mg	1.9%
0.620 g	1.2 mg	0.20%
6.200 g	1.3 mg	0.021%
62.000 g	2.4 mg	0.0038%
620.000 g	13 mg	0.0021%

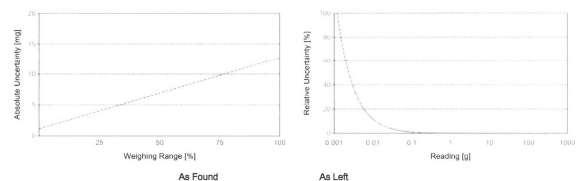

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



## Certificate of Calibration

Cert. No.: 22TM89  
Page.: 1 of 3

**Equipment :** Autoclave  
**Manufacturer :** ALP  
**Model :** CL-40L  
**Serial No. :** 802664  
**ID No. :** UAE.MIC.014/2550  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
**Location :** Air Analysis Unit  
**Received Order :** 17 February 2022  
**Calibration Date :** 17 February 2022  
**Ambient Temperature :** ( 26 ± 10 ) °C  
**Relative Humidity :** ( 50 ± 30 ) %  
**Calibrated by :** Kunchit Promprat

**Approved by :**  
( / ) Ponthippa Tameyakul  
( ✓ ) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 22 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



**Equipment :** Autoclave  
**Condition As-Received :** Used Item  
**Reference :** 2202-0444OC-1  
**Procedure Used :-**

Cert. No.: 22TM89  
Page.: 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T  
The temperature scale used was based on ITS-90.

#### Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34970A	MY44035217	21LM30	23 Dec 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.  
3. This certification is traceable to the International System of Unit.


4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3\*\*

(\*\* = Categorization of pathogens according to hazard and categories of containment, second edition, 1990 )

It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.  
This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source



	Environmental		
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	27	68	226
Finished of Calibration	27	65	226

Position	Description	Ref. Std. ID No.:
1 =	Center of chamber	22-10TC-01
2 =	Temperature sensor	22-10TC-02
3 =	Exhaust port	22-10TC-03



Equipment : Autoclave  
 Condition As-Received : Used Item  
 Reference : 2202-0444OC-1  
 Result of Calibration :- ( \* ) Without Adjustment

Cert. No.: 22TM89  
 Page.: 3 of 3

Operating parameter Set : Temperature = 122 °C  
 Sterilization period = 30 minute

UUC* Setting ( °C )	UUC* Reading ( °C )	Position	Average* Standard Reading ( °C )	Stability ( ± °C )	Pressure Reading ( MPa )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
122	122	1	122.373	0.32	0.12	1.2	2
		2	122.421				
		3	122.292				

Average\* : The average of 30 values in each position.  
 Stability : One-half of the greatest maximum difference of measured temperature at any one probe.  
 UUC\* : Unit Under Calibration  
 Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

๑ 1096060



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
 CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
 534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
 TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM681  
 Page.: 1 of 3

## Certificate of Calibration

Equipment : Autoclave  
 Manufacturer : ALP  
 Model : CL-40L  
 Serial No. : 808763  
 ID No. : UAE.MIC.026/2563  
 Submitted by : United Analyst and Engineering Consultant Co.,Ltd.  
 3 Soi Udomsuk 41, Sukhumvit Road,  
 Bangkok, Phrakhanong,  
 Bangkok 10260  
 Location : Microbiology Laboratory (301)  
 Received Order : 27 May 2022  
 Calibration Date : 27 May 2022  
 Ambient Temperature : ( 26 ± 10 ) °C  
 Relative Humidity : ( 50 ± 30 ) %  
 Calibrated by : Preecha Hlahib

Approved by :   
 Approved Signatory

( / ) Pongthippa Tameyakul  
 ( / ) Malee Butkruea  
 ( ) Suwit Imjai

Issue Date : 2 June 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
 Approval of the head of Corporate Services 3 : Equipment Calibration and Testing

เอกสารไม่ควบคุม



Equipment : Autoclave  
 Condition As-Received : Used Item  
 Reference : 2205-0764OC-2  
 Procedure Used :-

Cert. No.: 22TM681  
 Page.: 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T  
 The temperature scale used was based on ITS-90.

### Condition of this result of calibration


1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34970A	MY44060450	22LM46	28 Mar 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.  
 3. This certification is traceable to the International System of Unit.  
 4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3\*\*  
 (\*\* = Categorization of pathogens according to hazard and categories of containment, second edition, 1990 )  
 It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.  
 This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Result of Calibration :- ( \* ) Without Adjustment

Function of UUC\* : Temperature Source



	Environmental		
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	27	56	220
Finished of Calibration	27	59	221

Position	Description	Ref. Std. ID No.:
1 =	Center of chamber	22-14TC-01
2 =	Temperature sensor	22-14TC-02
3 =	Exhaust port	22-14TC-03

เอกสารไม่ควบคุม



Equipment : Autoclave  
 Condition As-Received : Used Item  
 Reference : 2205-0764OC-2  
 Result of Calibration :- ( \* ) Without Adjustment

Cert. No.: 22TM681  
 Page.: 3 of 3

Operating parameter Set : Temperature = 115.0 °C  
 Sterilization period = 15 minute

UUC* Setting ( °C )	UUC* Reading ( °C )	Position	Average* Standard Reading ( °C )	Stability ( ± °C )	Pressure Reading ( MPa )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
115.0	115.0	1	115.553	0.4	0.08	0.82	2
		2	115.582				
		3	115.325				

Operating parameter Set : Temperature = 121 °C  
 Sterilization period = 30 minute

UUC* Setting ( °C )	UUC* Reading ( °C )	Position	Average* Standard Reading ( °C )	Stability ( ± °C )	Pressure Reading ( MPa )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
121.0	121.0	1	121.484	0.21	1.1	0.75	2
		2	121.581				
		3	121.311				

Average\* : The average of 30 values in each position.  
 Stability : One-half of the greatest maximum difference of measured temperature at any one probe.  
 UUC\* : Unit Under Calibration  
 Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม