

ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือตรวจวัดคุณภาพสิ่งแวดล้อม

- 1) คุณภาพอากาศในบรรยากาศ
- 2) คุณภาพอากาศจากปล่อง
- 3) ระดับเสียง
- 4) คุณภาพน้ำ
- 5) คุณภาพอากาศในสถานประกอบการ
- 6) ระดับความร้อนในสถานประกอบการ

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
1. คุณภาพอากาศในบรรยากาศ		
Total Suspended Particulate	High Volume Air Sampler No. B03, B08, B10, B18, B20, B23, B29	Digital Balance
PM ₁₀	High Volume PM-10 Air Sampler No. B01, B02, B06, B07, B12, B15, B21	Digital Balance
PM _{2.5}	High Volume PM-2.5 Air Sampler No. B01, B05, B06, B07, B09, B10	Digital Balance
Hydrogen Chloride	Gas Box No. B02	Ion Chromatography
Sulfur Dioxide	SO ₂ Analyzer No. B01, B04, B05, B06, B07, B11, B13	SO ₂ Analyzer No. B01, B04, B05, B06, B07, B11, B13
Nitrogen Dioxide	NO _x Analyzer No. B06, B07, B08, B09, B16, B18, B20	NO _x Analyzer No. B06, B07, B08, B09, B16, B18, B20
2. คุณภาพอากาศจากปล่อง		
Particulate	Console No. B01, B04 Pitot Tube No. B04, B35	Digital Balance
PM ₁₀	Console No. B01, B04 Pitot Tube No. B04, B35	Digital Balance
Sulfur Dioxide	Personal Pump No. B06, B10 Rotameter No. H-B07, B09	Digital Balance
Oxides of Nitrogen	Vacuum Gauge	Spectrophotometer
Carbon Monoxide	Personal Pump No. B01, B17 Rotameter No. H-B07, B09	CO Analyzer No. B01
3. ระดับเสียง L _{eq} 8 hr, L _{eq} 24 hr, L _{eq} 5 min, L _{max} , L ₉₀ , L _{dn} , ระดับเสียงรบกวน	Acoustic Calibrator Sound Level Meter No. ACO-B01, B08, B11, B16, B18, B23, B27, B37, B29, B36, B43, B46 Sound Level Meter No. CR-B01, B02, B03, B06, B07, B08, B09	-
4. คุณภาพน้ำ		
Conductivity	-	Conductivity Meter
pH	-	pH Meter
Total Suspended Solids	-	Digital Balance
Total Dissolved Solids	-	Digital Balance
Grease & Oil	-	Digital Balance
BOD ₅	-	BOD Analyzer
COD	-	COD Reactor
Manganese	-	Inductively Coupled Plasma
Total Iron	-	Inductively Coupled Plasma Atomic Absorption Spectrophotometer

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม (ต่อ)**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
4. คุณภาพน้ำ (ต่อ)		
Acidity	-	Digital Balance
Alkalinity	-	Digital Balance
Total Coliform Bacteria	-	Digital Balance
Silica	-	Spectrophotometer
5. คุณภาพอากาศ ในสถานประกอบการ		
Total Dust	Personal Pump No. B47, B85 Rotameter No. H-B05, B10	Digital Balance
Sulfur Dioxide	Personal Pump No. B13, B80 Rotameter No. H-B05, B10	Digital Balance
Carbon Monoxide	Personal Pump No. B10, B61 Rotameter No. L-B05, B10	Digital Balance
Hydrogen Chloride	Personal Pump No. B55, B93 Rotameter No. L-B05, B10	Digital Balance
6. ระดับความร้อน ในสถานประกอบการ		
WBGT	-	Digital Thermometer No. B11, B28 Heat Stress WBGT Meter No. B11, B28

คุณภาพอากาศในบรรยากาศ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B01	B01	01/02/2023	$y = 1.278x - 5.652$	0.997
B02	B02	02/02/2023	$y = 1.147x + 0.663$	0.999
B03	B03	01/02/2023	$y = 1.123x - 0.622$	0.995
B04	B04	01/02/2023	$y = 1.229x - 4.835$	0.996
B05	B05	02/02/2023	$y = 1.280x - 6.358$	0.997
B06	B06	01/02/2023	$y = 1.251x - 5.438$	0.999
B07	B07	03/02/2023	$y = 1.165x - 3.515$	0.996
B08	B08	03/02/2023	$y = 1.269x - 7.559$	0.997
B09	B09	01/02/2023	$y = 1.198x - 2.843$	0.998
B10	B10	01/02/2023	$y = 1.128x + 0.785$	0.999
B11	B11	02/02/2023	$y = 1.138x - 1.752$	0.999
B12	B12	01/02/2023	$y = 1.195x - 4.080$	0.998
B13	B13	01/02/2023	$y = 1.254x - 5.913$	0.999
B14	B14	03/02/2023	$y = 1.291x - 7.822$	0.999
B15	B15	01/02/2023	$y = 1.149x - 1.829$	0.997
B16	B16	01/02/2023	$y = 1.287x - 7.502$	0.997
B17	B17	02/02/2023	$y = 1.207x - 4.147$	1.000
B18	B18	01/02/2023	$y = 1.277x - 7.238$	0.999
B19	B19	03/02/2023	$y = 1.243x - 6.520$	0.995
B20	B20	01/02/2023	$y = 1.267x - 7.055$	1.000
B21	B21	03/02/2023	$y = 1.141x - 1.101$	0.999
B22	B22	03/02/2023	$y = 1.221x - 5.534$	0.996
B23	B23	02/02/2023	$y = 1.197x - 4.328$	0.995
B24	B24	01/02/2023	$y = 1.159x - 2.269$	0.999
B25	B25	01/02/2023	$y = 1.050x + 2.684$	0.998
B26	B26	03/02/2023	$y = 1.253x - 6.203$	0.997
B27	B27	03/02/2023	$y = 1.220x - 5.822$	0.997
B28	B28	01/02/2023	$y = 1.251x - 6.762$	0.999
B29	B29	01/02/2023	$y = 1.201x - 3.793$	0.998
B30	B30	03/02/2023	$y = 1.242x - 6.540$	0.995
B31	B31	03/02/2023	$y = 1.255x - 6.608$	0.999
B32	B32	02/02/2023	$y = 1.249x - 6.292$	0.997
B33	B33	02/02/2023	$y = 1.260x - 5.168$	0.997
B34	B34	01/02/2023	$y = 1.272x - 7.454$	1.000

Calibrated by :

[Redacted Signature]

(Mr. Adul Dangklom)

Approved by :

[Redacted Signature]

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B01	B01	02/02/2023	$y = 1.210x - 0.261$	0.997
B02	B02	02/02/2023	$y = 1.046x + 2.414$	0.998
B03	B03	02/02/2023	$y = 1.199x - 4.047$	0.996
B04	B04	02/02/2023	$y = 1.288x - 7.602$	0.997
B05	B05	01/02/2023	$y = 1.222x - 4.886$	1.000
B06	B06	01/02/2023	$y = 1.210x - 3.612$	0.996
B07	B07	03/02/2023	$y = 1.270x - 6.088$	0.999
B08	B08	01/02/2023	$y = 1.277x - 5.288$	0.998
B09	B09	03/02/2023	$y = 1.289x - 6.478$	0.999
B10	B10	03/02/2023	$y = 1.266x - 8.106$	0.997
B11	B11	01/02/2023	$y = 1.258x - 6.917$	0.995
B12	B12	02/02/2023	$y = 1.192x - 3.640$	0.998
B13	B13	02/02/2023	$y = 1.289x - 7.913$	0.998
B14	B14	02/02/2023	$y = 1.250x - 4.233$	0.999
B15	B15	01/02/2023	$y = 1.118x + 0.802$	0.999
B16	B16	03/02/2023	$y = 1.297x - 3.106$	0.998
B17	B17	01/02/2023	$y = 1.204x - 4.477$	0.996
B18	B18	02/02/2023	$y = 1.176x - 1.624$	0.998
B19	B19	02/02/2023	$y = 1.097x + 1.230$	0.999
B20	B20	03/02/2023	$y = 1.188x - 4.372$	0.999
B21	B21	03/02/2023	$y = 1.156x - 0.146$	0.996
B22	B22	03/02/2023	$y = 1.269x - 6.647$	0.998
B23	B23	02/02/2023	$y = 1.197x - 2.685$	1.000
B24	B24	02/02/2023	$y = 1.251x - 6.437$	0.995
B25	B25	01/02/2023	$y = 1.144x - 2.851$	0.997
B26	B26	01/02/2023	$y = 1.249x - 5.704$	0.996
B27	B27	01/02/2023	$y = 1.241x - 5.428$	0.997
B28	B28	01/02/2023	$y = 1.198x - 4.626$	0.998
B29	B29	02/02/2023	$y = 1.244x - 7.658$	0.997
B30	B30	02/02/2023	$y = 1.246x - 7.229$	0.997
B31	B31	02/02/2023	$y = 1.178x - 0.243$	0.995
B32	B32	03/02/2023	$y = 1.201x - 2.954$	0.998
B33	B33	03/02/2023	$y = 1.168x - 1.341$	0.997
B34	B34	01/02/2023	$y = 1.237x - 2.684$	0.995

Calibrated by :

[Redacted Signature]

(Mr. Adul Dangklom)

Approved by :

[Redacted Signature]

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompof, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Gas Sampler Box Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Dry Cal DCL-ML

S/N : 136164

Calibration Data

Gas Sampler Data		Calibration Data					
No.	Rotameter	Date	Setting (Constant Flow) (ml/min)	Actual Flow Rate (ml/min)			
				Sampling Line A		Sampling Line B	
				Normal Condition	Standard Condition	Normal Condition	Standard Condition
B01	2 (A&B)	01/12/2022	200	200.4	199.0	200.5	199.1
B02	2 (A&B)	01/12/2022	200	200.5	199.1	200.8	199.3
B03	2 (A&B)	05/12/2022	200	200.4	199.0	200.5	199.0
B04	2 (A&B)	05/12/2022	200	200.8	199.3	200.7	199.3
B05	2 (A&B)	02/12/2022	200	200.5	199.1	200.4	199.0
B06	2 (A&B)	02/12/2022	200	200.4	199.0	200.5	199.1
B07	2 (A&B)	02/12/2022	200	200.8	199.4	200.9	199.5
B08	2 (A&B)	06/12/2022	200	200.4	199.0	200.5	199.1
B09	2 (A&B)	06/12/2022	200	200.6	199.2	200.4	199.0
B10	2 (A&B)	01/12/2022	200	200.6	199.1	200.5	199.1
B11	2 (A&B)	02/12/2022	200	200.4	199.0	200.7	199.3
B12	2 (A&B)	05/12/2022	200	200.8	199.4	200.5	199.0
B13	2 (A&B)	06/12/2022	200	200.6	199.1	200.8	199.3
B14	2 (A&B)	02/12/2022	200	200.7	199.2	200.5	199.1
B15	2 (A&B)	01/12/2022	200	200.4	199.0	200.7	199.2
B16	2 (A&B)	01/12/2022	200	200.6	199.1	200.4	199.0
B17	2 (A&B)	02/12/2022	200	200.5	199.0	200.6	199.1

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chaituchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	19 February 2023	BRAND :	API	MODEL :	100A
NO.	SO ₂ -B01	SERIAL NO.	1749		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 04 August 2022		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO ₂)		Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 50.0 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
SO ₂ Span	400.0	400.2	0.050	400.0	1.012
API Model 100A SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.5	in-Hg	25-35		
SAMPLE FLOW	654	cc/min	650 ± 10%		
PMT	103.2	mV	-20-150 with Zero Air		
UV LAMP	3039.4	mV	1000-4900		
STR. LGT	61.3	PPB	<100		
DRK PMT	62.9	mV	-50 - 200		
DRK LMP	57.8	mV	-50 - 200		
HVPS	671	V	550-900 constant		
DCPS	2518	mV	2500 ± 200		
RCELL TEMP	50.4	°C	50 ± 1		
BOX TEMP	29.2	°C	5-40		
PMT TEMP	7.0	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.012	-	1.0 ± 0.3		
SO ₂ Offset	21.9	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com... www.spscon.com

CALIBRATION REPORT

SO₂ FLUORESCENT ANALYZER

DATE : 19 February 2023

BRAND : API

MODEL : 100E

NO. SO₂-B04

SERIAL NO. 3159

Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 04 August 2022

Serial No. : 911

Reference Standard Gas

Standard Gas : Sulphur Dioxide (SO₂)

Cylinder No. : A00814SK

Certified Date : 21 June 2021

Expired Date : 21 June 2029

Cylinder Conc. : 50.0 ppm

CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.6 °C

% RH 49

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
SO ₂ Span	400.0	400.1	0.025	400.0	1.010

API Model 100E SO₂ Analyzer Check list

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	0-500
SAMPLE PRESS	28.7	in-Hg	25-35
SAMPLE FLOW	657	cc/min	650 ± 10%
PMT	103.4	mV	-20-150 with Zero Air
UV LAMP	3079.5	mV	1000-4900
STR. LGT	61.8	PPB	<100
DRK PMT	63.6	mV	-50 - 200
DRK LMP	58.1	mV	-50 - 200
HVPS	672	V	550-900 constant
DCPS	2528	mV	2500 ± 200
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.1	°C	5-40
PMT TEMP	7.4	°C	7 ± 2.0
SO ₂ Span Conc	400	PPB	20-20,000
SO ₂ Slope	1.010	-	1.0 ± 0.3
SO ₂ Offset	22.2	mV	<250
Stability at Zero	0.1	PPB	<0.2
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chafuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com www.spscon.com

CALIBRATION REPORT						
SO ₂ FLUORESCENT ANALYZER						
DATE :	19 February 2023	BRAND :	API	MODEL :	100E	
NO.	SO ₂ -B05	SERIAL NO.	3270			
Calibrator (Dilution System)						
Brand	: API			Model	: 700	
Last Cal. Date	: 04 August 2022			Serial No.	: 911	
Reference Standard Gas						
Standard Gas	: Sulphur Dioxide (SO ₂)			Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 50.0 ppm	
CALIBRATING CONDITION						
Pressure	1011	mmbar	Temp.	24.6	°C	
% RH						49
CALIBRATION SETTING						
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB		
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope	
Zero	0	-0.10	-	0	-	
SO ₂ Span	400.0	399.7	-0.075	400.0	1.006	
API Model 100E SO ₂ Analyzer Check list						
Test Values	Observed Value	Units	Nominal Range			
RANGE	500	PPB	0-500			
SAMPLE PRESS	28.6	in-Hg	25-35			
SAMPLE FLOW	655	cc/min	650 ± 10%			
PMT	102.9	mV	-20-150 with Zero Air			
UV LAMP	3011.7	mV	1000-4900			
STR. LGT	61.4	PPB	<100			
DRK PMT	63.0	mV	-50 - 200			
DRK LMP	57.7	mV	-50 - 200			
HVPS	669	V	550-900 constant			
DCPS	2515	mV	2500 ± 200			
RCELL TEMP	50.1	°C	50 ± 1			
BOX TEMP	29.4	°C	5-40			
PMT TEMP	7.2	°C	7 ± 2.0			
SO ₂ Span Conc	400	PPB	20-20,000			
SO ₂ Slope	1.006	-	1.0 ± 0.3			
SO ₂ Offset	21.8	mV	<250			
Stability at Zero	0.1	PPB	<0.2			
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)			

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscn.com www.spscn.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	19 February 2023	BRAND :	API	MODEL :	100E
NO.	SO ₂ -B06	SERIAL NO.	3430		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 04 August 2022		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO ₂)		Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 50.0 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO ₂ Span	400.0	399.8	-0.050	400.0	1.008
API Model 100E SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.4	in-Hg	25-35		
SAMPLE FLOW	660	cc/min	650 ± 10%		
PMT	103.3	mV	-20-150 with Zero Air		
UV LAMP	3024.5	mV	1000-4900		
STR. LGT	61.5	PPB	<100		
DRK PMT	63.2	mV	-50 - 200		
DRK LMP	57.9	mV	-50 - 200		
HVPS	674	V	550-900 constant		
DCPS	2523	mV	2500 ± 200		
RCELL TEMP	50.2	°C	50 ± 1		
BOX TEMP	29.3	°C	5-40		
PMT TEMP	7.0	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.008	-	1.0 ± 0.3		
SO ₂ Offset	22.1	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaiyachak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	19 February 2023	BRAND :	API	MODEL :	100E
NO.	SO ₂ -B07	SERIAL NO.	1706		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 04 August 2022		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO ₂)		Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 50.0 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO ₂ Span	400.0	400.4	0.100	400.0	1.015
API Model 100E SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.7	in-Hg	25-35		
SAMPLE FLOW	658	cc/min	650 ± 10%		
PMT	103.1	mV	-20-150 with Zero Air		
UV LAMP	3017.4	mV	1000-4900		
STR. LGT	61.9	PPB	<100		
DRK PMT	63.4	mV	-50 - 200		
DRK LMP	58.2	mV	-50 - 200		
HVPS	673	V	550-900 constant		
DCPS	2521	mV	2500 ± 200		
RCELL TEMP	50.5	°C	50 ± 1		
BOX TEMP	29.0	°C	5-40		
PMT TEMP	7.1	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.015	-	1.0 ± 0.3		
SO ₂ Offset	22.0	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spsscon.com, www.spsscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	19 February 2023	BRAND :	TELEDYNE	MODEL :	TML-50
NO.	SO ₂ -B11	SERIAL NO.	SO2187		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 04 August 2022		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO ₂)		Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 50.0 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
SO ₂ Span	400.0	399.6	-0.100	400.0	1.003
API Model TML-50 SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.6	in-Hg	25-35		
SAMPLE FLOW	653	cc/min	650 ± 10%		
PMT	103.0	mV	-20-150 with Zero Air		
UV LAMP	3020.4	mV	1000-4900		
STR. LGT	61.6	PPB	<100		
DRK PMT	63.3	mV	-50 - 200		
DRK LMP	58.0	mV	-50 - 200		
HVPS	675	V	550-900 constant		
DCPS	2517	mV	2500 ± 200		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.0	°C	5-40		
PMT TEMP	7.2	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.003	-	1.0 ± 0.3		
SO ₂ Offset	21.7	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	19 February 2023	BRAND :	TELEDYNE	MODEL :	TML-50
NO.	SO ₂ -B13	SERIAL NO.	1891		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 04 August 2022		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO ₂)		Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 50.0 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
SO ₂ Span	400.0	400.3	0.075	400.0	1.014
API Model TML-50 SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.4	in-Hg	25-35		
SAMPLE FLOW	656	cc/min	650 ± 10%		
PMT	103.3	mV	-20-150 with Zero Air		
UV LAMP	3036.2	mV	1000-4900		
STR. LGT	61.7	PPB	<100		
DRK PMT	63.5	mV	-50 - 200		
DRK LMP	58.1	mV	-50 - 200		
HVPS	672	V	550-900 constant		
DCPS	2525	mV	2500 ± 200		
RCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	28.8	°C	5-40		
PMT TEMP	7.1	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.014	-	1.0 ± 0.3		
SO ₂ Offset	21.8	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพลโฮลิค 24 ถนนพลโฮลิค แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO₂ / NO_x ANALYZER

DATE : 19 February 2023

BRAND : API

MODEL : 200E

NO. NOX-B06

SERIAL NO. 2286

Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 04 August 2022

Serial No. : 911

Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : D636192

Certified Date : 20 April 2022

Expired Date : 20 April 2024

Cylinder Conc. : 49.1 ppm

CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.6 °C

% RH 49

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.007
NO _x Span	400	400.2	0.050	400.0	1.011

API Model 200E NO_x Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	508	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	103.3	mV	-20 - 150
AZERO	94.1	mV	-20 - 150
HVPS	669	V	420 - 900 constant
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.5	°C	8 - 48
PMT TEMP	7.1	°C	7 ± 2
MOLY TEMP	315.2	°C	315 ± 5
RCELL PRESS	8.2	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO _x Span Conc	400	PPB	20 - 20,000
NO Slope	1.007	-	1.0 ± 0.3
NO _x Slope	1.011	-	1.0 ± 0.3
NO Offset	1.4	mV	-20 to +150
NO _x Offset	0.9	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol. Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	19 February 2023	BRAND :	API	MODEL :	200E
NO.	NOX-B07	SERIAL NO.	4338		
Calibrator (Dilution System)					
Brand	: API			Model	: 700
Last Cal. Date	: 04 August 2022			Serial No.	: 911
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: D636192
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024	Cylinder Conc.	: 49.1 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	400.2	0.050	400.0	1.010
NO _x Span	400	400.5	0.125	400.0	1.014
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	513	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.2	mV	-20 - 150		
AZERO	93.9	mV	-20 - 150		
HVPS	674	V	420 - 900 constant		
RCELL TEMP	50.2	°C	50 ± 1		
BOX TEMP	29.3	°C	8 - 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	314.9	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.010	-	1.0 ± 0.3		
NO _x Slope	1.014	-	1.0 ± 0.3		
NO Offset	1.7	mV	-20 to +150		
NO _x Offset	1.0	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	19 February 2023	BRAND :	API	MODEL :	200E
NO.	NOX-B08	SERIAL NO.	4336		
Calibrator (Dilution System)					
Brand	: API			Model	: 700
Last Cal. Date	: 04 August 2022			Serial No.	: 911
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: D636192
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024	Cylinder Conc.	: 49.1 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	49	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.5	-0.125	400.0	0.998
NO _x Span	400	399.8	-0.050	400.0	1.003
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	504	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	102.9	mV	-20 - 150		
AZERO	94.0	mV	-20 - 150		
HVPS	672	V	420 - 900 constant		
RCELL TEMP	50.1	°C	50 ± 1		
BOX TEMP	29.0	°C	8 - 48		
PMT TEMP	7.4	°C	7 ± 2		
MOLY TEMP	315.1	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	0.998	-	1.0 ± 0.3		
NO _x Slope	1.003	-	1.0 ± 0.3		
NO Offset	1.0	mV	-20 to +150		
NO _x Offset	0.6	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaitachak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT						
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER						
DATE :	19 February 2023	BRAND :	API	MODEL :	200E	
NO.	NOX-B09	SERIAL NO.	4412			
Calibrator (Dilution System)						
Brand	: API			Model	: 700	
Last Cal. Date	: 04 August 2022			Serial No.	: 911	
Reference Standard Gas						
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: D636192	
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024	Cylinder Conc.	: 49.1 ppm	
CALIBRATING CONDITION						
Pressure	1011	mmbar	Temp.	24.6	°C	
% RH						49
CALIBRATION SETTING						
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB		
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope	
Zero	0	-0.11	-	0	-	
NO Span	400	399.9	-0.025	400.0	1.005	
NO _x Span	400	400.2	0.050	400.0	1.009	
API Model 200E NO _x Analyzer Check List						
Test Values	Observed Value	Units	Nominal Range			
RANGE	500	PPB	500 standard			
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air			
SAMPLE FLOW	511	cc/min	500 ± 50			
OZONE FLOW	79	cc/min	80 ± 15			
PMT	103.0	mV	-20 - 150			
AZERO	93.8	mV	-20 - 150			
HVPS	673	V	420 - 900 constant			
RCELL TEMP	50.4	°C	50 ± 1			
BOX TEMP	29.5	°C	8 - 48			
PMT TEMP	7.2	°C	7 ± 2			
MOLY TEMP	314.7	°C	315 ± 5			
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant			
SAMPLE PRESS	28.7	IN-Hg-A	25 - 30 constant			
NO Span Conc	400	PPB	20 - 20,000			
NO _x Span Conc	400	PPB	20 - 20,000			
NO Slope	1.005	-	1.0 ± 0.3			
NO _x Slope	1.009	-	1.0 ± 0.3			
NO Offset	1.1	mV	-20 to +150			
NO _x Offset	0.7	mV	-20 to 150			
Stability at Zero	0.1	PPB	< 0.2			
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas			

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	19 February 2023	BRAND :	API	MODEL :	200E
NO.	NOX-B16	SERIAL NO.	249		
Calibrator (Dilution System)					
Brand	: API			Model	: 700
Last Cal. Date	: 04 August 2022			Serial No.	: 911
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: D636192
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024	Cylinder Conc.	: 49.1 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.009
NO _x Span	400	400.3	0.075	400.0	1.012
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	506	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	103.5	mV	-20 - 150		
AZERO	94.2	mV	-20 - 150		
HVPS	671	V	420 - 900 constant		
RCELL TEMP	50.1	°C	50 ± 1		
BOX TEMP	28.8	°C	8 - 48		
PMT TEMP	7.0	°C	7 ± 2		
MOLY TEMP	315.4	°C	315 ± 5		
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.009	-	1.0 ± 0.3		
NO _x Slope	1.012	-	1.0 ± 0.3		
NO Offset	1.5	mV	-20 to +150		
NO _x Offset	0.9	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	19 February 2023	BRAND :	API	MODEL :	TML-41M
NO.	NOX-B18	SERIAL NO.	N07543		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 04 August 2022		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: D636192	
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024	Cylinder Conc.	: 49.1 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	400.2	0.050	400.0	1.011
NO _x Span	400	400.4	0.100	400.0	1.015
API Model TML-41M NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	510	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.1	mV	-20 - 150		
AZERO	94.0	mV	-20 - 150		
HVPS	670	V	420 - 900 constant		
RCELL TEMP	50.5	°C	50 ± 1		
BOX TEMP	29.4	°C	8 - 48		
PMT TEMP	7.3	°C	7 ± 2		
MOLY TEMP	315.3	°C	315 ± 5		
RCELL PRESS	8.2	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.011	-	1.0 ± 0.3		
NO _x Slope	1.015	-	1.0 ± 0.3		
NO Offset	1.6	mV	-20 to +150		
NO _x Offset	1.0	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	19 February 2023	BRAND :	API	MODEL :	TML-41M
NO.	NOX-B20	SERIAL NO.	N02782		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 04 August 2022		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: D636192	
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024	Cylinder Conc.	: 49.1 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.8	-0.050	400.0	1.006
NO _x Span	400	400.1	0.025	400.0	1.009
API Model TML-41M NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	509	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	102.9	mV	-20 - 150		
AZERO	93.7	mV	-20 - 150		
HVPS	675	V	420 - 900 constant		
RCELL TEMP	50.4	°C	50 ± 1		
BOX TEMP	29.2	°C	8 - 48		
PMT TEMP	7.3	°C	7 ± 2		
MOLY TEMP	314.8	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.006	-	1.0 ± 0.3		
NO _x Slope	1.009	-	1.0 ± 0.3		
NO Offset	1.2	mV	-20 to +150		
NO _x Offset	0.8	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)




บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

CALIBRATION REPORT			
PM2.5 AIR SAMPLER (VERY SHARP CUT CYCLONE-VSCC)			
DATE :	19 February 2023	BRAND :	BGI
		MODEL :	PQ200
NO.	PM2.5-B01	SERIAL NO.	000927
CALIBRATING CONDITION			
Pressure	1011	mmbar	Temp. 24.5 °C
		% RH	48
Calibration Method : Dry Cal Primary Flowmeter		Model : Defender 510 H	S/N : 136164
CALIBRATION SETTING			
detaCal	PM2.5 AIR SAMPLER		
Flowrate Reading, L/min	Initial Flowrate Reading (Before Adj.), L/min	% Dif.	Final Flowrate Reading (After Adj.), L/min
16.70	16.65	0.299	16.70

Calibrated by :


(Mr. Adul Dangklom)

Approved by :


(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

CALIBRATION REPORT

PM2.5 AIR SAMPLER (VERY SHARP CUT CYCLONE-VSCC)

DATE : 19 February 2023

BRAND : BGI

MODEL : PQ200

NO. PM2.5-B05

SERIAL NO. 160810-14(VSCC)

CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.5 °C

% RH 48

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510 H

S/N : 136164

CALIBRATION SETTING

detaCal

PM2.5 AIR SAMPLER

Flowrate Reading, L/min

Initial Flowrate Reading (Before Adj.), L/min

% Dif.

Final Flowrate Reading (After Adj.), L/min

16.70

16.68

0.120

16.70

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT			
PM2.5 AIR SAMPLER (VERY SHARP CUT CYCLONE-VSCC)			
DATE :	19 February 2023	BRAND :	BGI
NO.	PM2.5-B06	MODEL :	PQ200
		SERIAL NO.	164589 (VSCC)
CALIBRATING CONDITION			
Pressure	1011	mmbar	Temp. 24.5 °C
		% RH	48
Calibration Method : Dry Cal Primary Flowmeter		Model : Defender 510 H	S/N : 136164
CALIBRATION SETTING			
detaCal	PM2.5 AIR SAMPLER		
Flowrate Reading, L/min	Initial Flowrate Reading (Before Adj.), L/min	% Dif.	Final Flowrate Reading (After Adj.), L/min
16.70	16.64	0.359	16.70

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

CALIBRATION REPORT

PM2.5 AIR SAMPLER (VERY SHARP CUT CYCLONE-VSCC)

DATE : 19 February 2023

BRAND : BGI

MODEL : PQ200

NO. PM2.5-B07

SERIAL NO. 152099 (VSCC)

CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.5 °C

% RH 48

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510 H

S/N : 136164

CALIBRATION SETTING

detaCal

PM2.5 AIR SAMPLER

Flowrate Reading, L/min

Initial Flowrate Reading (Before Adj.), L/min

% Dif.

Final Flowrate Reading (After Adj.), L/min

16.70

16.66

0.240

16.70

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

CALIBRATION REPORT			
PM2.5 AIR SAMPLER (VERY SHARP CUT CYCLONE-VSCC)			
DATE :	19 February 2023	BRAND :	BGI
MODEL :	PQ200	SERIAL NO.	152125 (VSCC)
NO.	PM2.5-B09		
CALIBRATING CONDITION			
Pressure	1011	mmbar	Temp. 24.5 °C
% RH		48	
Calibration Method : Dry Cal Primary Flowmeter		Model : Defender 510 H	S/N : 136164
CALIBRATION SETTING			
detaCal	PM2.5 AIR SAMPLER		
Flowrate Reading, L/min	Initial Flowrate Reading (Before Adj.), L/min	% Dif.	Final Flowrate Reading (After Adj.), L/min
16.70	16.68	0.120	16.70

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

PM2.5 AIR SAMPLER (VERY SHARP CUT CYCLONE-VSCC)

DATE : 19 February 2023

BRAND : BGI

MODEL : PQ200

NO. PM2.5-B10

SERIAL NO. 164598 (VSCC)

CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.5 °C

% RH 48

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510 H

S/N : 136164

CALIBRATION SETTING

detaCal

PM2.5 AIR SAMPLER

Flowrate Reading, L/min

Initial Flowrate Reading (Before Adj.), L/min

% Dif.

Final Flowrate Reading (After Adj.), L/min

16.70

16.65

0.299

16.70

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 23M2441

REFERENCE No : 68471-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 23M2441

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23°C \pm 1°C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.0001	-0.0001	0.00011
100.00	100.0001	-0.0001	0.00019
200.00	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



Certificate of Calibration

Aquion : Anion (ID#894)

This certificate is to verify that instrument below are calibrated
by Archemica Lab Co.,Ltd.


AQUION S/N : 190840059

AS-DV S/N : 190915235

for

S.P.S. Consulting Service Co., Ltd.



Operator Signature :  Date : Jan 4, 2023

(Mr. Channarong Khiao-Un)

Test Engineer

คุณภาพอากาศจากปล่อง



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	$\Delta H_{@}$ (mmH ₂ O)
B01	1563	01/12/2022	1.007	49.94
B02	8002514	02/12/2022	1.002	49.41
B03	1503016	05/12/2022	1.004	50.46
B04	00006659	01/12/2022	1.007	49.43
B05	00007428	01/12/2022	0.998	49.80
R01	1561	01/12/2022	1.004	49.52
R02	8002513	01/12/2022	1.003	49.77
R03	1570	05/12/2022	1.008	49.68
R04	8002519	05/12/2022	0.997	50.12
R05	1503015	01/12/2022	1.003	50.08

Remark : Accept Value of y (test) is $0.97 < y < 1.03$

Accept Value of $\Delta H_{@}$ (test) is 46.7 ± 6.4 (mmH₂O)

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	DH _@ (mmH ₂ O)
B01	1563	02/03/2023	0.998	50.11
B02	8002514	03/03/2023	1.004	49.25
B03	1503016	03/03/2023	1.002	50.62
B04	00006659	02/03/2023	1.004	50.14
B05	00007428	03/03/2023	1.001	49.76
R01	1561	01/03/2023	0.997	49.86
R02	8002513	03/03/2023	0.996	49.93
R03	1570	02/03/2023	1.003	49.57
R04	8002519	01/03/2023	1.002	48.90
R05	1503015	01/03/2023	0.998	50.20

Remark : Accept Value of y (test) is $0.97 < y < 1.03$

Accept Value of $\Delta H_{@}$ (test) is 46.7 ± 6.4 (mmH₂O)

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B03	S	0.99	02/02/2023	0.84	0.84
B04	S	0.99	01/02/2023	0.84	0.83
B05	S	0.99	02/02/2023	0.84	0.85
B07	S	0.99	02/02/2023	0.85	0.84
B08	S	0.99	01/02/2023	0.83	0.84
B09	S	0.99	01/02/2023	0.84	0.84
B11	S	0.99	01/02/2023	0.84	0.84
B16	S	0.99	01/02/2023	0.84	0.83
B18	S	0.99	02/02/2023	0.84	0.84
B19	S	0.99	02/02/2023	0.85	0.84
B21	S	0.99	03/02/2023	0.84	0.84
B24	S	0.99	03/02/2023	0.84	0.83
B27	S	0.99	02/02/2023	0.84	0.84
B30	S	0.99	01/02/2023	0.83	0.84
B31	S	0.99	02/02/2023	0.84	0.85
B33	S	0.99	03/02/2023	0.84	0.84
B35	S	0.99	02/02/2023	0.84	0.85

Remark : Accept value of Cp (test) is 0.84 ± 0.01

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B03	S	0.99	02/05/2023	0.85	0.84
B04	S	0.99	02/05/2023	0.84	0.84
B05	S	0.99	02/05/2023	0.84	0.83
B07	S	0.99	02/05/2023	0.83	0.84
B08	S	0.99	03/05/2023	0.84	0.85
B09	S	0.99	04/05/2023	0.85	0.84
B11	S	0.99	04/05/2023	0.84	0.83
B16	S	0.99	04/05/2023	0.84	0.85
B18	S	0.99	02/05/2023	0.84	0.84
B19	S	0.99	02/05/2023	0.85	0.84
B21	S	0.99	03/05/2023	0.84	0.85
B24	S	0.99	03/05/2023	0.84	0.83
B27	S	0.99	02/05/2023	0.83	0.84
B30	S	0.99	04/05/2023	0.84	0.84
B31	S	0.99	02/05/2023	0.83	0.84
B33	S	0.99	03/05/2023	0.85	0.84
B35	S	0.99	02/05/2023	0.84	0.83

Remark : Accept value of Cp (test) is 0.84 ± 0.01

Calibrated by :

[Redacted Signature]

(Mr. Adul Dangklom)

Approved by :

[Redacted Signature]

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B01	SKC	224-PCXR4	262101	03/01/2023	1,000	1,500	2,000	993	1,497	1,998	1.003x - 5.584	1.000
B02	SKC	224-PCXR4	626166	03/01/2023	1,000	1,500	2,000	1,003	1,505	2,001	1.009x - 19.667	0.999
B03	SKC	224-PCXR4	612968	03/01/2023	1,000	1,500	2,000	996	1,494	2,000	1.006x - 12.109	1.000
B04	SKC	224-PCXR4	602804	04/01/2023	1,000	1,500	2,000	1,000	1,502	1,995	1.000x - 0.893	1.000
B05	SKC	224-PCXR4	612693	04/01/2023	1,000	1,500	2,000	1,003	1,500	2,003	1.012x - 22.224	0.999
B06	SKC	224-PCXR4	262188	03/01/2023	1,000	1,500	2,000	995	1,508	2,005	1.011x - 20.273	1.000
B07	SKC	224-PCXR4	626262	03/01/2023	1,000	1,500	2,000	998	1,492	1,995	0.993x + 6.086	1.000
B08	SKC	224-PCXR4	626100	03/01/2023	1,000	1,500	2,000	1,003	1,500	2,003	1.012x - 23.308	0.999
B09	SKC	224-PCXR4	626479	03/01/2023	1,000	1,500	2,000	996	1,490	1,994	0.995x + 1.117	1.000
B10	SKC	224-PCXR4	091950	03/01/2023	1,000	1,500	2,000	992	1,503	2,001	1.018x - 36.582	0.999
B11	SKC	224-PCXR8	564315	05/01/2023	1,000	1,500	2,000	996	1,490	1,999	1.003x - 8.256	1.000
B12	SKC	224-PCXR4	034656	05/01/2023	1,000	1,500	2,000	1,003	1,503	2,003	1.010x - 19.324	0.999
B13	SKC	224-PCXR4	602073	05/01/2023	1,000	1,500	2,000	995	1,500	1,998	1.001x - 3.474	1.000
B14	SKC	224-PCXR4	626313	04/01/2023	1,000	1,500	2,000	999	1,491	1,988	0.992x + 6.844	1.000
B15	SKC	224-PCXR4	626474	04/01/2023	1,000	1,500	2,000	1,001	1,502	2,005	1.014x - 25.558	0.999
B16	SKC	224-PCXR4	626477	04/01/2023	1,000	1,500	2,000	994	1,504	2,001	1.015x - 31.345	0.999
B17	SKC	224-PCXR4	626860	04/01/2023	1,000	1,500	2,000	997	1,494	1,991	0.997x - 0.359	1.000
B18	SKC	224-PCXR4	691484	04/01/2023	1,000	1,500	2,000	1,003	1,500	2,001	1.008x - 17.589	0.999
B19	SKC	224-PCXR4	691599	03/01/2023	1,000	1,500	2,000	993	1,503	1,999	1.007x - 11.574	1.000
B20	SKC	224-PCXR4	691587	03/01/2023	1,000	1,500	2,000	992	1,504	1,999	1.015x - 32.235	0.999
B21	SKC	224-PCXR4	691531	03/01/2023	1,000	1,500	2,000	993	1,499	1,994	1.001x - 7.107	1.000
B22	SKC	224-PCXR4	691654	05/01/2023	1,000	1,500	2,000	1,003	1,501	2,003	1.011x - 21.107	0.999
B23	SKC	224-PCXR4	798393	05/01/2023	1,000	1,500	2,000	992	1,507	2,002	1.018x - 34.883	0.999
B24	SKC	224-PCXR4	626363	05/01/2023	1,000	1,500	2,000	1,000	1,502	2,000	1.011x - 22.387	0.999
B25	SKC	224-PCXR4	798489	05/01/2023	1,000	1,500	2,000	1,001	1,492	2,001	0.998x + 1.101	1.000
B26	SKC	224-PCXR4	798479	05/01/2023	1,000	1,500	2,000	999	1,500	1,993	0.996x + 4.008	1.000
B27	SKC	224-PCXR4	691673	04/01/2023	1,000	1,500	2,000	994	1,503	2,002	1.016x - 32.071	0.999
B28	SKC	224-PCXR4	691570	04/01/2023	1,000	1,500	2,000	1,002	1,500	2,002	1.012x - 22.515	0.999
B29	SKC	224-PCXR4	626472	04/01/2023	1,000	1,500	2,000	1,000	1,496	1,998	1.001x - 4.942	1.000
B30	SKC	224-PCXR4	691489	03/01/2023	1,000	1,500	2,000	1,004	1,510	2,004	1.008x - 12.460	0.999
B31	SKC	224-PCXR4	691509	03/01/2023	1,000	1,500	2,000	992	1,497	1,998	1.006x - 12.711	1.000
B32	SKC	224-PCXR4	091567	05/01/2023	1,000	1,500	2,000	991	1,504	2,001	1.016x - 32.322	0.999
B33	SKC	224-PCXR4	091756	05/01/2023	1,000	1,500	2,000	993	1,497	1,991	0.997x - 0.004	1.000
B34	SKC	224-PCXR4	612962	05/01/2023	1,000	1,500	2,000	1,002	1,501	2,002	1.007x - 14.195	1.000
B35	SKC	224-PCXR4	602682	05/01/2023	1,000	1,500	2,000	993	1,498	1,995	1.002x - 8.448	1.000
B36	SKC	224-PCXR4	626164	03/01/2023	1,000	1,500	2,000	999	1,496	1,999	1.001x - 5.424	1.000
B37	SKC	224-PCXR4	626256	03/01/2023	1,000	1,500	2,000	994	1,506	1,999	1.013x - 27.815	0.999
B38	SKC	224-PCXR4	626167	03/01/2023	1,000	1,500	2,000	997	1,496	1,996	0.999x - 0.997	1.000
B39	SKC	224-PCXR4	034637	03/01/2023	1,000	1,500	2,000	1,005	1,501	2,001	1.010x - 18.618	0.999
B40	SKC	224-PCXR4	798349	05/01/2023	1,000	1,500	2,000	994	1,506	1,999	1.014x - 29.602	0.999

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}\text{C}$
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R²
B01	SKC	224-PCXR4	262101	04/04/2023	1,000	1,500	2,000	994	1,498	2,003	1.005x - 7.897	1.000
B02	SKC	224-PCXR4	626166	04/04/2023	1,000	1,500	2,000	1,004	1,503	2,003	1.010x - 19.866	0.999
B03	SKC	224-PCXR4	612968	07/04/2023	1,000	1,500	2,000	995	1,496	2,001	1.007x - 13.664	1.000
B04	SKC	224-PCXR4	602804	05/04/2023	1,000	1,500	2,000	998	1,499	1,994	0.999x - 1.611	1.000
B05	SKC	224-PCXR4	612693	07/04/2023	1,000	1,500	2,000	1,002	1,501	2,004	1.014x - 24.856	0.999
B06	SKC	224-PCXR4	262188	07/04/2023	1,000	1,500	2,000	994	1,509	2,006	1.012x - 21.589	0.999
B07	SKC	224-PCXR4	626262	04/04/2023	1,000	1,500	2,000	997	1,490	1,996	0.994x + 3.454	1.000
B08	SKC	224-PCXR4	626100	04/04/2023	1,000	1,500	2,000	1,001	1,499	2,005	1.015x - 27.137	0.999
B09	SKC	224-PCXR4	626479	05/04/2023	1,000	1,500	2,000	997	1,492	1,994	0.994x + 2.385	1.000
B10	SKC	224-PCXR4	091950	03/04/2023	1,000	1,500	2,000	993	1,504	2,005	1.013x - 23.779	1.000
B11	SKC	224-PCXR8	564315	10/04/2023	1,000	1,500	2,000	995	1,492	1,998	1.002x - 7.259	1.000
B12	SKC	224-PCXR4	034656	04/04/2023	1,000	1,500	2,000	1,002	1,504	2,001	1.009x - 17.609	0.999
B13	SKC	224-PCXR4	602073	04/04/2023	1,000	1,500	2,000	997	1,501	2,000	1.004x - 7.622	1.000
B14	SKC	224-PCXR4	626313	03/04/2023	1,000	1,500	2,000	997	1,492	1,991	0.996x + 1.699	1.000
B15	SKC	224-PCXR4	626474	07/04/2023	1,000	1,500	2,000	1,003	1,503	2,006	1.013x - 23.245	0.999
B16	SKC	224-PCXR4	626477	03/04/2023	1,000	1,500	2,000	995	1,506	2,003	1.011x - 22.132	0.999
B17	SKC	224-PCXR4	626860	04/04/2023	1,000	1,500	2,000	996	1,493	1,993	1.000x - 4.627	1.000
B18	SKC	224-PCXR4	691484	04/04/2023	1,000	1,500	2,000	1,001	1,496	2,002	1.010x - 21.179	0.999
B19	SKC	224-PCXR4	691599	04/04/2023	1,000	1,500	2,000	994	1,504	2,000	1.006x - 10.498	1.000
B20	SKC	224-PCXR4	691587	03/04/2023	1,000	1,500	2,000	991	1,502	2,000	1.016x - 35.102	0.999
B21	SKC	224-PCXR4	691531	04/04/2023	1,000	1,500	2,000	994	1,501	1,995	1.001x - 5.153	1.000
B22	SKC	224-PCXR4	691654	07/04/2023	1,000	1,500	2,000	1,000	1,502	2,004	1.014x - 25.574	0.999
B23	SKC	224-PCXR4	798393	05/04/2023	1,000	1,500	2,000	990	1,508	2,004	1.013x - 23.994	1.000
B24	SKC	224-PCXR4	626363	03/04/2023	1,000	1,500	2,000	1,002	1,503	1,999	1.009x - 18.837	0.999
B25	SKC	224-PCXR4	798489	07/04/2023	1,000	1,500	2,000	1,002	1,494	2,000	0.997x + 3.494	1.000
B26	SKC	224-PCXR4	798479	07/04/2023	1,000	1,500	2,000	1,001	1,501	1,994	0.995x + 5.564	1.000
B27	SKC	224-PCXR4	691673	04/04/2023	1,000	1,500	2,000	995	1,505	2,004	1.013x - 25.091	0.999
B28	SKC	224-PCXR4	691570	04/04/2023	1,000	1,500	2,000	1,003	1,501	2,001	1.010x - 19.922	0.999
B29	SKC	224-PCXR4	626472	05/04/2023	1,000	1,500	2,000	1,001	1,498	2,000	0.999x - 1.831	1.000
B30	SKC	224-PCXR4	691489	04/04/2023	1,000	1,500	2,000	1,002	1,507	2,003	1.009x - 13.936	0.999
B31	SKC	224-PCXR4	691509	07/04/2023	1,000	1,500	2,000	994	1,496	1,997	1.004x - 9.680	1.000
B32	SKC	224-PCXR4	091567	10/04/2023	1,000	1,500	2,000	992	1,506	2,001	1.013x - 25.542	0.999
B33	SKC	224-PCXR4	091756	05/04/2023	1,000	1,500	2,000	993	1,498	1,992	0.998x - 1.121	1.000
B34	SKC	224-PCXR4	612962	07/04/2023	1,000	1,500	2,000	1,002	1,503	2,003	1.008x - 14.753	0.999
B35	SKC	224-PCXR4	602682	05/04/2023	1,000	1,500	2,000	991	1,497	1,996	1.003x - 11.598	1.000
B36	SKC	224-PCXR4	626164	05/04/2023	1,000	1,500	2,000	997	1,495	1,998	1.002x - 8.097	1.000
B37	SKC	224-PCXR4	626256	07/04/2023	1,000	1,500	2,000	993	1,505	1,996	1.012x - 27.161	0.999
B38	SKC	224-PCXR4	626167	07/04/2023	1,000	1,500	2,000	998	1,493	1,997	1.003x - 8.615	1.000
B39	SKC	224-PCXR4	034637	10/04/2023	1,000	1,500	2,000	1,003	1,500	2,003	1.013x - 23.125	0.999
B40	SKC	224-PCXR4	798349	07/04/2023	1,000	1,500	2,000	993	1,507	1,998	1.015x - 30.204	0.999

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-B01	Dwyer	VFB-65	05/01/2023	500	1,000	2,000	506.1	989.5	1973.5	0.990x + 8.311	1.000
H-B02	Dwyer	VFB-65	05/01/2023	500	1,000	2,000	494.9	998.2	1995.3	0.993x + 4.772	1.000
H-B03	Dwyer	VFB-65	05/01/2023	500	1,000	2,000	498.3	987.5	2010.6	1.005x - 15.690	0.999
H-B04	Dwyer	VFB-65	03/01/2023	500	1,000	2,000	500.4	999.5	2008.7	0.998x - 2.369	1.000
H-B05	Dwyer	VFB-65	03/01/2023	500	1,000	2,000	499.0	997.8	1972.3	0.981x + 20.957	0.999
H-B06	Dwyer	VFB-65	03/01/2023	500	1,000	2,000	503.6	995.0	1981.4	1.005x - 8.788	0.999
H-B07	Dwyer	VFB-65	04/01/2023	500	1,000	2,000	504.1	989.0	2018.7	1.002x - 2.144	1.000
H-B08	Dwyer	VFB-65	06/01/2023	500	1,000	2,000	499.8	999.2	1975.8	0.996x + 3.270	0.999
H-B09	Dwyer	VFB-65	06/01/2023	500	1,000	2,000	503.7	1006.6	2014.3	0.994x + 14.202	1.000
H-B10	Dwyer	VFB-65	06/01/2023	500	1,000	2,000	496.1	998.6	2012.4	0.997x + 2.443	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-B01	Dwyer	VFB-65	05/04/2023	500	1,000	2,000	506.9	990.3	1974.3	0.989x + 9.271	1.000
H-B02	Dwyer	VFB-65	04/04/2023	500	1,000	2,000	495.3	999.1	1996.1	0.994x + 4.127	1.000
H-B03	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	497.5	988.1	2009.6	1.003x - 14.485	0.999
H-B04	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	501.2	1000.3	2006.5	0.997x - 1.216	1.000
H-B05	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	500.2	999.6	1974.3	0.980x + 21.307	0.999
H-B06	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	504.3	996.2	1984.0	1.004x - 6.770	1.000
H-B07	Dwyer	VFB-65	04/04/2023	500	1,000	2,000	502.3	990.7	2016.7	1.001x - 1.154	1.000
H-B08	Dwyer	VFB-65	05/04/2023	500	1,000	2,000	500.2	1000.6	1979.8	0.995x + 5.040	0.999
H-B09	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	504.4	1007.4	2010.7	0.993x + 15.376	1.000
H-B10	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	495.7	1001.6	2009.2	0.996x + 3.956	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VACUUM GAUGE
MANUFACTURER : HI-LIGHT
MODEL / TYPE : N/A
SERIAL NO. : N/A[64-220066-1]
CLID. NO. : 212201112
JOB CONTROL NO. : 220720073201

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 20 July 2022

DATE OF ISSUED : 22 July 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer



Approved By : Mongkol Yotsoontorn
Authorized Signatory
22 July 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22073201

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : VACUUM GAUGE
MANUFACTURER : HI-LIGHT
MODEL / TYPE : N/A
SERIAL NO. : N/A[64-220066-1]
DATE OF CALIBRATION : 21 July 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-05** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 744 S/N. 9226007 with Pressure Module Model 700PV4 S/N. 19298401.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. MP-0196-21, Due Date 17 November 2022.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. **Q22073201**

F3-011-04/01-12

page 2 of 3



@clccalibration

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (inHg)	STD Reading (inHg)		Correction (inHg)	
	Up	Down	Up	Down
0	0.0	0.0	0.0	0.0
-5	-4.6	-4.7	+0.4	+0.3
-10	-9.5	-9.6	+0.5	+0.4
-15	-14.4	-14.5	+0.6	+0.5
-20	-19.4	-19.5	+0.6	+0.5
-25	-24.5	-24.5	+0.5	+0.5
-30	-29.5	-29.5	+0.5	+0.5

Uncertainty of measurement ± 0.2 inHg

Transmitting fluid : Air.

Technical Note. k factor 1 kPa = 0.2952998 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 36 of 54

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22073201

F3-011-04/01-12

page 3 of 3



@clccalibration



CERTIFICATE No : 23M2441

REFERENCE No : 68471-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY : [REDACTED]
PONGSAK J.

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23



CERTIFICATE No : 23M2441

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23°C \pm 1°C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.0001	-0.0001	0.00011
100.00	100.0001	-0.0001	0.00019
200.00	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : SP22018

Pages 1 of 3

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY

Condition As Found : GOOD

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON, CHATUCHAK,
BANGKOK 10900, THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (24.4 ± 5) °C
Relative Humidity : (60.1 ± 25) %

Received Date : 30 AUGUST 2022
Calibration Date : 30 AUGUST 2022
Date of Issue : 31 AUGUST 2022

Calibrated by :

Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : SP22018

Job No. : VC65SP0008

Pages : 2 of 3

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01,ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	87569	13/10/2022
Didymium liquid	RM-DL	28912	87588	15/10/2022
Neutral density filter	RM-1N2N3N	13877	87600	15/10/2022
Potassium dichromate solutions	RM-0204060810	14204	87614	16/10/2022
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology,NIST.

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.4	0.15	0.16	2.00
	467.82	467.8	-0.02	0.16	2.00
	536.56	536.5	-0.06	0.16	2.00
	640.50	640.5	0.00	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.2	0.26	0.16	2.00

UUC* = Unit Under Calibration

Continuation of Calibration Certificate

Cert. No. : SP22018
Job No. : VC65SP0008
Pages : 3 of 3

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Filter: S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0524	1.0539	0.0015	0.0028	2.00
		29914	0.7	0.7454	0.7459	0.0005	0.0029	2.00
		29381	0.5	0.5426	0.5426	0.0000	0.0028	2.00
	546.1	29360	1.0	0.9822	0.9810	-0.0012	0.0028	2.00
		29914	0.7	0.6962	0.6960	-0.0002	0.0028	2.00
		29381	0.5	0.5076	0.5070	-0.0006	0.0029	2.00
	590.0	29360	1.0	1.0221	1.0202	-0.0019	0.0028	2.00
		29914	0.7	0.7238	0.7230	-0.0008	0.0029	2.00
		29381	0.5	0.5364	0.5360	-0.0004	0.0031	2.00
	635.0	29360	1.0	0.9751	0.9732	-0.0019	0.0028	2.00
		29914	0.7	0.6912	0.6902	-0.0010	0.0029	2.00
		29381	0.5	0.5214	0.5210	-0.0004	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2436	0.2419	-0.0017	0.0101	2.00	
		40	0.4905	0.4855	-0.0050	0.0115	2.00	
		60	0.7453	0.7388	-0.0065	0.0067	2.00	
		80	0.9920	0.9839	-0.0081	0.0071	2.00	
		100	1.2487	1.2414	-0.0073	0.0073	2.00	

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230

Resolution of Wavelength Mode 0.1 nm
Resolution of Photometric Mode 0.0001 A
Parameter Setting
Measurement Mode Wavelength, Absorbance
Wavelength Scan 1100 nm-190 nm
Scanning Speed 7.5 nm/min
Data Pitch 0.1 nm
Band width(Wavelength) 1.0 nm
Band width(Vis) 1.0 nm
Band width(Uv) 1.0 nm

Stray Light** UUC* Reading at 220 nm	
Transimission T(%)	Absorbance(A)
0.0107	3.9886

**Specific Acceptance :
Transmission \leq 1.0 T(%), Absorbance \geq 2.0 A
**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	01 February 2023	Brand :	API	Model :	300E
No.	CO-B01			Serial No.	782
Calibrator (Dilution System)					
Brand : API			Model : 700		
Last Cal. Date : 06 September 2022			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D196045		
Certified Date : 16 April 2022		Expired Date : 15 April 2024		Cylinder Conc. : 4,570 ppm	
Calibrating Condition					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH 48					
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	-0.10	-	0	
CO Span	40.00	39.92	-0.200	40.00	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4015.7	mV	2500-4800 mV		
CO Reference	3948.2	mV	2500-4800 mV		
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.5	In-Hg-A	~2" < Ambient Absolute Pressure		
Sample Flow	809	CC/Min	800 ± 10%		
Sample Temperature	48.4	°C	48 ± 4		
Bench Temperature	48.1	°C	48 ± 2		
Wheel Temperature	68.3	°C	68 ± 2		
Box Temperature	30.6	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3025.2	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	02 May 2023	Brand :	API	Model :	300E
No.	CO-B01			Serial No.	782
Calibrator (Dilution System)					
Brand : API			Model : 700		
Last Cal. Date : 06 September 2022			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D196045		
Certified Date : 16 April 2022		Expired Date : 15 April 2024		Cylinder Conc. : 4,570 ppm	
Calibrating Condition					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	0.11	-	0	
CO Span	40.00	39.89	-0.275	40.00	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4016.3	mV	2500-4800 mV		
CO Reference	3949.1	mV	2500-4800 mV		
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.6	In-Hg-A	~2" < Ambient Absolute Pressure		
Sample Flow	803	CC/Min	800 ± 10%		
Sample Temperature	48.2	°C	48 ± 4		
Bench Temperature	48.0	°C	48 ± 2		
Wheel Temperature	68.2	°C	68 ± 2		
Box Temperature	30.8	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3031.6	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		

Calibrated by :

[Redacted Signature]

(Mr. Adul Dangklom)

Approved by :

[Redacted Signature]

(Mr. Peera Detudom)

ระดับเสียง

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N 4106495.
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 27 Mar. 2023

Date of Calibration : 29 Mar. 2023

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.94	-0.06	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.80	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

(Mr. Weerachai Deechaiyae)

Approved by :

(Mr. Prawate Kluaypa)
Director

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 29 Mar. 2023

Date of Issue : 30 Mar. 2023

Ref : 2011266032701228001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website: www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise B_056/23

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	28 April 2022
		Due Date	28 April 2023

Calibration Data


Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B01	ACO	6236	00132025	18 February 2023	93.9	94.0
ACO-B08	ACO	6236	00142008	18 February 2023	94.0	94.0
ACO-B11	ACO	6236	00152079	18 February 2023	94.1	94.0
ACO-B16	ACO	6236	00172039	18 February 2023	94.1	94.0
ACO-B18	ACO	6236	00172048	18 February 2023	94.0	94.0
ACO-B23	ACO	6236	00182002	18 February 2023	94.0	94.0
ACO-B27	ACO	6236	00182008	18 February 2023	93.9	94.0
ACO-B37	ACO	6236	00192028	18 February 2023	94.0	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.93 ± 0.10 dB	

Calibrated by :



(Mr. Abdul Dangklom)

Approved by :

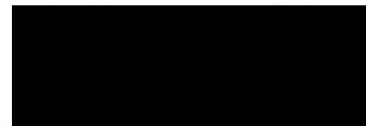

(Mr. Peera Detudom)

คุณภาพน้ำ

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : CONDUCTIVITY METER
MANUFACTURER : METTLER TOLEDO
MODEL / TYPE : SEVEN COMPACT S230
SERIAL NO. : C141708983/5821320179
CLID. NO. : 272300452
JOB CONTROL NO. : 230211016445

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 11 February 2023

DATE OF ISSUED : 15 February 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Calibration Engineer



Approved By : Mongkol Yotsoontorn
Authorized Signatory
15 February 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23016445

F3-011-04/01-12

page 1 of 4



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	CONDUCTIVITY METER
MANUFACTURER	:	METTLER TOLEDO
MODEL / TYPE	:	SEVEN COMPACT S230
SERIAL NO.	:	C141708983/5821320179
DATE OF CALIBRATION	:	13 February 2023

ENVIRONMENT CONDITIONS :

Temperature : $(25 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \% \text{ RH}$

PROCEDURE USED :

This instrument [Conductivity Meter] was calibrated under procedure No. **WI-305-130**. The calibration was performed by direct measurement with Certified Reference Material (CRM) and Reference Material (RM) .

This instrument [Temperature] was calibrated under procedure No. **WI-305-244**. The calibration was performed by Comparison with Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Potassium Chloride Solution (nominal 1.41 mS/cm , nominal 12.8 mS/cm)
2. Conductivity Solution , Hanna Product Code HI 7033L Lot Number 6436.
3. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
4. Precision Thermometer, ASL Model F250 S/N. 1334023800.
5. IPRT, ASL Model T100-250-1D S/N. L0193A-1-1.



TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through Merck Co., Ltd.

Certificate No. HC02139203 , HC04515254. Due Date 30 June 2023 , 30 November 2023.

2. The measurements are traceable to International System of Units (SI) , through Hanna instruments.

Certificate No. 12E12 , Due Date May 2024 .

3. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q22130792, Due Date 05 January 2024.

4. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0823/65, Due Date 22 August 2023.

5. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).

Certificate No. TT-0166-22, Due Date 01 December 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of Conductivity Meter.

CALIBRATION DATA

1. Conductivity Solution Test @ 25°C

Standard Conductivity Solution	DUC Reading	Uncertainty of Measurement	k Factor
*84.00 µS/cm	84.04 µS/cm [Cell Constant 0.548589]	± 1.00 µS/cm	2,00
1412.0 µS/cm	1413 µS/cm [Cell Constant 0.548589]	± 21.0 µS/cm	2,00
12.85 mS/cm	12.88 mS/cm [Cell Constant 0.573538]	± 0.19 mS/cm	2,00

Note. * means Calibrations marked "Not TISI Accredited" in this Certificate have been included for completeness.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 138 of 138

*2. Temperature Result [Probe Conductivity]

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ± (°C)
100	25.00	25.0	0.00	0.07

Note. The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2,00$.

* means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

End of Certificate



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : pH METER
MANUFACTURER : ECOSENSE/YSI
MODEL / TYPE : PH100A
SERIAL NO. : JC03158/YSI60537718A[PH 06/61]
CLID. NO. : 272101138
JOB CONTROL NO. : 230314028618

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 14 March 2023

DATE OF ISSUED : 17 March 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Monthira Treechum
Calibration Engineer



Approved By : Mongkol Yotsoontorn
Authorized Signatory
17 March 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23028618

F3-011-04/01-12

page 1 of 4



@clccalibration

REPORT OF CALIBRATION FOR

NOMENCLATURE : pH METER
MANUFACTURER : ECOSENSE/YSI
MODEL / TYPE : PH100A
SERIAL NO. : JC03158/YSI60537718A[PH 06/61]
DATE OF CALIBRATION : 15 March 2023

ENVIRONMENT CONDITIONS :

Temperature : $(25 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPCH-01** [pH Meter]. The calibration was performed by direct measurement with Certified Reference Material (CRM).

This instrument was calibrated under procedure No. **CLC-CPTH-04** [pH Temperature] based on **ASTM E 644-04** as calibration guidelines. The calibration was performed by using Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. pH Standard Solution, NIMT TRM CODE TRM-S-2003, TRM CODE TRM-S-2007.
2. pH Standard Solution, Control Company Catalog Number 06-664-260,11754256, Lot Number CC728484.
3. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
4. Precision Thermometer, ASL Model F200-A-8 S/N. 014433/03.
5. IPRT, ASL Model T100-250-1D S/N. L0193A-1-1.



TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Lot Number. 160221 , 180121. Due Date 05 May 2023.
2. The measurements are traceable to International System of Units (SI) , through Control Company.
Certificate No. 4281-12405788 , Due Date 30 June 2023.
3. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.
Certificate No. Q22130792, Due Date 05 January 2024.
4. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0010/66, Due Date 06 November 2023.
5. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Certificate No. TT-0166-22, Due Date 01 December 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of pH meter.

CALIBRATION DATA

1. pH METER RESULT @ 25 °C

Standard pH Buffer Solution (pH)	pH Meter Reading (pH)	pH Meter Reading (mV)	Correction (pH)	Uncertainty of pH Measurement (± pH)	k Factor
4.000	4.00	141	0.000	0.012	2,20
6.996	6.99	-25	+0.006	0.015	2,06
10.007	9.99	-201	+0.017	0.015	2,05

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 2,3 of 54

2. TEMPERATURE RESULT [pH PROBE]

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ± (°C)
100	25.00	24.8	+0.20	0.07

Note. Probe Ø 12 mm

The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 47 of 54

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2,00$.

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23028618

F3-011-04/01-12

page 4 of 4





CERTIFICATE No : 23M2442

REFERENCE No : 68471-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY : [REDACTED]
PONGSAK J.

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23



CERTIFICATE No : 23M2442

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591843
ID No : BA 09/61 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23°C \pm 1°C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000058
0.1	0.1000	0.0000	0.000059
0.2	0.2000	0.0000	0.000059
0.5	0.5000	0.0000	0.000060
1.0	1.0000	0.0000	0.000060
2.0	2.0000	0.0000	0.000061
5.0	5.0000	0.0000	0.000063
10.0	10.0000	0.0000	0.000067
20.0	20.0001	-0.0001	0.000073
50.0	50.0000	0.0000	0.00011
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	99.9999
3	99.9998
4	100.0001
5	100.0000
OFF-CENTER LOADING	0.0002

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

CERT.No.: HS-U017D

Calibration Date : 3 Apr 23
Submitted by : S.P.S CONSULTING SERVICE CO.,LTD
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
Chatuchak, Bangkok, Thailand 10900

Model : YSI 5000
S/N : 15B100751
Probe : YSI 5010
S/N : 22D100097
ID NO. : -
Air Temp ref : S/N. E00522
Barometric ref : S/N. E00522
Water Temp ref : S/N. 11431
Technician : Kittipong M.

Avg Room Temp : 20 °C
Avg Water Temp : 20 °C
Air Pressure : 760.00 mmHg
Salinity : 0 ppt

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-
<hr/>			
Mean Measurement	9.08	mg/l	-
Inaccuracy	0.01	mg/l	-
<hr/>			
Overall Status	(PASS)		

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature

(Kittipong Maekwong)

Laboratory Manager

(Natenapha Pisatkunchon)



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 23T0959

REFERENCE No : 68047-2

PAGE : 1 OF 3

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB200

SERIAL No : 15110C0235

ID No : CRB 05/59

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 07-Feb-23

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 07-Feb-23

RECEIVED DATE : 31-Jan-23



CERTIFICATE No : 23T0959

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : CRB 05/59
RECEIVED DATE : 31-Jan-23
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB200
SERIAL NUMBER : 15110C0235
CALIBRATION DATE : 07-Feb-23
RELATIVE HUMIDITY : 52 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT TEMPERATURE RECORDER WITH THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 15 POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE FOUR CORNERS OF THE REACTOR AND PLACED THE EIGHTH THERMOCOUPLE AT THE CENTER OF THE REACTOR.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	8009008	22T7511	10-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

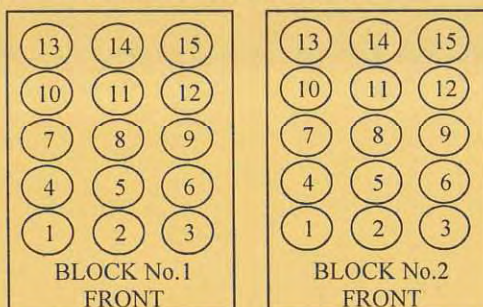

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	149.4
	2	149.5
	3	149.4
	4	149.4
	5	149.7
	6	149.4
	7	149.6
	8	149.6
	9	149.6
	10	149.7
	11	149.7
	12	149.3
	13	149.3
	14	149.5
	15	149.8
Uncertainty of Measurement(± °C)	0.86	0.86

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

Customer : <u>S.P.S.Consulting Service Co.,Ltd</u>	Date Tested: <u>January 11, 2023</u>	
	Recommendation Recertification	
Address : <u>7 Soi Phaholyothin 24</u>	Period <u>6</u> Months	
<u>Paholyothin Road</u>	Recertification Due: <u>July 11, 2023</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	Date Last Certified: <u>July 11, 2022</u>	
User Name: <u>K.Phenpha Vipasthawatt</u>	Visit Number: <u>2 of 2</u>	
Phone: <u>083-9269252</u>	PerkinElmer Phone: <u>02-719-6420 ext 206</u>	
Fax: <u>02-513-4221</u>	PerkinElmer Fax: <u>02-318-5597</u>	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
MODEL	SERIAL NUMBER	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
TESTED EQUIPMENT	CALIBRATION NUMBER	EXPIRATION
<u>IPV Methods</u>		
TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>May 30, 2023</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>February 28, 2023</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>August 30, 2023</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>November 30, 2023</u>
CUSTOMER SUPPLIED	COMMENTS	CUSTOMER INITIALS
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER 077C7042401
DATE TESTED January 11, 2023
1. MECHANICAL CHECKS

- | | |
|--|-----------------------------|
| A. Inspect and clean all fans and filters. | <input type="checkbox"/> OK |
| B. Inspect and replace as necessary, all torch components including the RF coil. | <input type="checkbox"/> OK |
| C. Inspect all tubing for sign of clacking or leaking. | <input type="checkbox"/> OK |
| D. Adjust water and gas pressure regulator settings. | <input type="checkbox"/> OK |
| E. Inspect and leak check pneumatics drawers. | <input type="checkbox"/> OK |
| F. Clean the exterior of the instrument. | <input type="checkbox"/> OK |

2. OPTICAL CHECKS

- | | |
|---|-----------------------------|
| A. Inspect and clean all optical components. | <input type="checkbox"/> OK |
| B. As required, check and replace all purgefilters. | <input type="checkbox"/> OK |
| C. Recheck optical alignment. | <input type="checkbox"/> OK |

3. COOLING SYSTEM CHECKS

- | | |
|---|------------------------------|
| A. Perform preventive maintenance on chiller. | <input type="checkbox"/> OK |
| B. Flush out the chiller every year. | <input type="checkbox"/> N/A |

4. PERFORMANCE CHECKS

- | | |
|----------------------------|-----------------------------|
| A. Torch View Alignment. | <input type="checkbox"/> OK |
| B. Wavelength Calibration. | <input type="checkbox"/> OK |



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER : 077C7042401
DATE TESTED : January 11, 2023

PARAMETER		SPECIFICATION		FINAL VALUE	
Spectral Resolution : UV	As 193.696 nm	≤ 0.007		<u>0.00504</u>	
	Ni 231.604 nm	≤ 0.008		<u>0.00646</u>	
	Ni 341.476 nm	≤ 0.012		<u>0.00768</u>	
Spectral Resolution : VIS	La 408.672 nm	≤ 0.020		<u>0.01597</u>	
	Ba 455.403 nm	≤ 0.025		<u>0.02185</u>	
Precision					
	As 193.656 nm	% RSD	< 1.0	<u>0.89</u>	%
	Zn 213.856 nm	% RSD	< 1.0	<u>0.77</u>	%
	Mn 257.610 nm	% RSD	< 1.0	<u>0.51</u>	%
	La 379.478 nm	% RSD	< 1.0	<u>0.44</u>	%
	Ba 455.403 nm	% RSD	< 1.0	<u>0.44</u>	%
	Ba 493.408 nm	% RSD	< 1.0	<u>0.46</u>	%
Detection Limits : Axial	Tl 190.080 nm	3(sd)		<u>4.04</u>	ppb
	As 193.696 nm	3(sd)		<u>3.58</u>	ppb
	Pb 220.353 nm	3(sd)		<u>1.90</u>	ppb
Detection Limits : Radial	As 193.696 nm	3(sd)		<u>47.72</u>	ppb
	Zn 213.856 nm	3(sd)		<u>1.02</u>	ppb
	Mn 257.610 nm	3(sd)		<u>0.68</u>	ppb
	La 379.478 nm	3(sd)		<u>1.43</u>	ppb
	Ba 455.403 nm	3(sd)		<u>0.10</u>	ppb
	Ba 493.408 nm	3(sd)		<u>0.36</u>	ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd 226.502 nm	≤ 150 ppb		<u>58.36</u>	
BEC : Radial (IB X 1000)/(IS-IB)	Mn 257.610 nm	≤ 45 ppb		<u>13.26</u>	



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER 077C7042401**DATE TESTED** January 11, 2023**Remarks :**

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

Service Department PerkinElmer Ltd.


Authorized Representative:

(Mr. Wiphan Promlumda)

Service Engineer

PinAAcle 900T Preventive Maintenance (PM)

Company Name:	SPS CONSULTING SERVICE CO.,LTD.		
Address (Instrument Location):	7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD. JOMPOL, CHATUCHAK, BANGKOK		
Serial Number:	PTCS14111103	PM Number:	1-2
Customer Name (if applicable):	K. PHENPHA	Telephone Number:	083-926-9252
Customer Support Engineer Name:	K. DUANG	Service Order Number:	WO-02044564
Date PM Performed: (DD-MMM-YYYY)	06-Jan-2023	Next PM Due Date: (DD-MMM-YYYY)	06-Jul-2023
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	
09370143 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900T by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes
AS900	AS9S14B1002	WINLAB 32

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	2
B3002013	THGA Contact Cylinders	1
B3141064	Glycerol for THGA Cooling	N/A
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	2
N9301714	Replacement Acetylene Filter Cartridge	1
TH001022	Replacement Air Filter Cartridge	2

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	26-87CUY1	30-Jan-2024
N9300244	GFAAS Mixed Standard	AR	56-021CRY1	30-Jun-2023

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 ml.	AR	AR
N/A	0.5% HNO ₃	250 ml.	AR	AR

Additional Tools Required for PM			
Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	MG0-252
N1013002	1.0A Neutral density filter	1	MG2-358
B3100652 Or N9307029	Electronic Flow Meter	1	NA
B0505495	Test Jig	1	NA
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	092216-010130
N3050109	Ba Lumina HCL	1	102416-040160
N3050139	K Lumina HCL	1	110716-010060
N3050152	Ni Lumina HCL	1	100516-030190
N3050119	Cr Lumina HCL	1	091911-020150

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ✓ Review the instrument performance with the customer and document any recent problems.
- ✓ Inspect the customer log book and make any appropriate PM entries.
- ✓ Perform general inspection of system for cleanliness.

2. PC Instrument Software:

- ✓ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. Mechanical:

- ✓ Inspect and clean all fans and filters. Replace filters if necessary
- ✓ Inspect all gas and water lines for leaks and/or wear. Replace if needed. Thoroughly inspect all quick connects. Replace the Y connector, P/N 09921079, if needed.
- ✓ Clean exterior of the instrument.

3.1 Flame Technique

- ✓ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ✓ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
- ✓ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ✓ Check the drain system for signs of wear. Replace worn or damaged parts.
- ✓ Visually check for proper flame conditions when igniting the Air-C₂H₂ and N₂O-C₂H₂ flames (if applicable).

3.2 THGA Technique

- ✓ Inspect the pole pieces and clean where the pole pieces contact the furnace. Replace the pole piece p-rings as needed, P/N's B0501018 & B0501250. Grease the O-rings as needed with Apiezon L grease, P/N 09905148
- ✓ Inspect the four insulation pads on the front contact housing of the THGA in furnace. If the pads are missing replace the THGA furnace or replace the insulator pads on the furnace.
- ✓ Inspect the graphite tube and clean the contact cylinders. Replace if necessary.
- ✓ Check internal and external gas flows with the Electronic Gas Flow Meter and the Gas Flow Test Probe as described in the Service Manual. Correct if necessary.
- ✓ Check furnace open/close function.
- ✓ Verify the operation of the GFTV Camera for proper operation and viewing alignment in the furnace camera Tube View window. Align if needed.
- ✓ Check the operation of the Halogen Light ASSY for the GFTV Camera. Replace if needed.
- ✓ Check the water level/quality in the recirculation (if applicable). Add distilled water if necessary.
- ✓ Check the cooling system fluid flow rate with the FCS In-Line Flow Meter for proper levels if needed. Refer to SDB# COSY008.STN

- ✓ Perform Cooling System maintenance if needed per SDB# COSY005.STN.
- ✓ Check auto sampler operation.
- ✓ Perform an auto sampler check valve test as described in the Service Manual.
- ✓ Lubricate the spindles of the auto sampler pumps and all moving parts of the tray mechanics as described in the Service Manual.
- ✓ Inspect the auto sampler sampling capillary as described in the Service Manual. Replace if necessary.

4. Electrical:

- ✓ Inspect PC boards. Clean if necessary.
- ✓ Carefully check all internal and external cable connections.
- ✓ Check instrument firmware revisions upgrade to current levels (if necessary)
- ✓ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

5. Optics:

- ✓ Inspect and clean the sample compartment windows, if needed.
- ✓ Inspect and clean the furnace windows, if needed.
- ✓ Inspect and clean the GFTV camera lens, if needed.
- ✓ Inspect optics. Clean or replace if necessary,

6. Gasses:

- ✓ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ✓ Verify that the air filter element is dry. Replace if necessary.

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests [Flame]:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	0.9798	0.1982	Passed
0.2 A ND Filter	± 5% from Cert.	0.2042	0.9942	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0014	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed

8.4 D₂ Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0083	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0002	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0021	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	NA	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	0.3281	Passed

9. After PM Performance tests [THGA]:

9.1 Furnace Gas Flows

Description: Ensures the flow rates are within specification.

Parameter	Specification	Test Results	Pass/Fail
Internal Flow Rate	250 mL/min \pm 25 mL/min	255	Passed
External Flow Rate	100 mL/min \pm 10 mL/min	105	Passed

9.2 Chromium Baseline Noise

Description: Signal to noise check.

Parameter	Specification	Results	Pass/Fail
Baseline Noise	≤ 0.005 Abs.	0.0000	Passed
Standard Deviation	≤ 0.005	0.0002	Passed

9.3 Chromium Characteristic Mass and Precision

Description: Calculate the characteristic mass using the characteristic mass tool and precision from the integrated absorbance values.

Parameter	Specification	Results	Pass/Fail
Cr m_0 Results	≤ 7.0 pg/0.0044 A-s	5.7	Passed
Precision	≤ 2.0 %	0.74	Passed

9.4 Copper Characteristic Mass and Zeeman Ratio

Description: Calculate the characteristic mass using the characteristic mass tool and check the Zeeman Ratio.

Parameter	Specification	Results	Pass/Fail
Cu m ₀ Result	≤ 16.5 pg/0.0044 A-s	12.3	Passed
Zeeman Ratio	0.52 ± 0.04	0.54	Passed



10. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

Additional Comments

Additional Comments Regarding the PM	
Zeeman Ratio	$= \frac{\text{Atomic Signal (Peak area)}}{\text{Atomic Signal (Peak area)} + \text{Background Signal (Peak area)}}$ $= \frac{0.1855}{0.1855+0.1563}$ $= 0.54$
REPLACE PM KIT	

Review

<i>The preventive maintenance checks and if applicable performance tests for PinAAcle 900T have been completed.</i>		
<i>This PinAAcle 900T Passes <input checked="" type="checkbox"/> Fails <input type="checkbox"/> the preventive maintenance.</i>		
Review of Preventive Maintenance:		
Authorized PerkinElmer Representative:		Date: 06-Jan-2023 <small>(DD-MMM-YYYY)</small>
Authorized Customer Representative:		Date: 06-Jan-2023 <small>(DD-MMM-YYYY)</small>

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : SP22018

Pages 1 of 3

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY

Condition As Found : GOOD

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON, CHATUCHAK,
BANGKOK 10900, THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (24.4 ± 5) °C
Relative Humidity : (60.1 ± 25) %

Received Date : 30 AUGUST 2022
Calibration Date : 30 AUGUST 2022
Date of Issue : 31 AUGUST 2022

Calibrated by :

Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : SP22018

Job No. : VC65SP0008

Pages : 2 of 3

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01,ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	87569	13/10/2022
Didymium liquid	RM-DL	28912	87588	15/10/2022
Neutral density filter	RM-1N2N3N	13877	87600	15/10/2022
Potassium dichromate solutions	RM-0204060810	14204	87614	16/10/2022
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology,NIST.

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.4	0.15	0.16	2.00
	467.82	467.8	-0.02	0.16	2.00
	536.56	536.5	-0.06	0.16	2.00
	640.50	640.5	0.00	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.2	0.26	0.16	2.00

UUC* = Unit Under Calibration

Continuation of Calibration Certificate

Cert. No. : SP22018
Job No. : VC65SP0008
Pages : 3 of 3

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Filter: S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0524	1.0539	0.0015	0.0028	2.00
		29914	0.7	0.7454	0.7459	0.0005	0.0029	2.00
		29381	0.5	0.5426	0.5426	0.0000	0.0028	2.00
	546.1	29360	1.0	0.9822	0.9810	-0.0012	0.0028	2.00
		29914	0.7	0.6962	0.6960	-0.0002	0.0028	2.00
		29381	0.5	0.5076	0.5070	-0.0006	0.0029	2.00
	590.0	29360	1.0	1.0221	1.0202	-0.0019	0.0028	2.00
		29914	0.7	0.7238	0.7230	-0.0008	0.0029	2.00
		29381	0.5	0.5364	0.5360	-0.0004	0.0031	2.00
	635.0	29360	1.0	0.9751	0.9732	-0.0019	0.0028	2.00
		29914	0.7	0.6912	0.6902	-0.0010	0.0029	2.00
		29381	0.5	0.5214	0.5210	-0.0004	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2436	0.2419	-0.0017	0.0101	2.00	
		40	0.4905	0.4855	-0.0050	0.0115	2.00	
		60	0.7453	0.7388	-0.0065	0.0067	2.00	
		80	0.9920	0.9839	-0.0081	0.0071	2.00	
		100	1.2487	1.2414	-0.0073	0.0073	2.00	

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230

Resolution of Wavelength Mode 0.1 nm
Resolution of Photometric Mode 0.0001 A
Parameter Setting
Measurement Mode Wavelength, Absorbance
Wavelength Scan 1100 nm-190 nm
Scanning Speed 7.5 nm/min
Data Pitch 0.1 nm
Band width(Wavelength) 1.0 nm
Band width(Vis) 1.0 nm
Band width(Uv) 1.0 nm

Stray Light** UUC* Reading at 220 nm	
Transmission T(%)	Absorbance(A)
0.0107	3.9886

**Specific Acceptance :
Transmission \leq 1.0 T(%), Absorbance \geq 2.0 A
**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate

คุณภาพอากาศในสถานประกอบการ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B01	SKC	224-PCXR4	262101	03/01/2023	1,000	1,500	2,000	993	1,497	1,998	1.003x - 5.584	1.000
B02	SKC	224-PCXR4	626166	03/01/2023	1,000	1,500	2,000	1,003	1,505	2,001	1.009x - 19.667	0.999
B03	SKC	224-PCXR4	612968	03/01/2023	1,000	1,500	2,000	996	1,494	2,000	1.006x - 12.109	1.000
B04	SKC	224-PCXR4	602804	04/01/2023	1,000	1,500	2,000	1,000	1,502	1,995	1.000x - 0.893	1.000
B05	SKC	224-PCXR4	612693	04/01/2023	1,000	1,500	2,000	1,003	1,500	2,003	1.012x - 22.224	0.999
B06	SKC	224-PCXR4	262188	03/01/2023	1,000	1,500	2,000	995	1,508	2,005	1.011x - 20.273	1.000
B07	SKC	224-PCXR4	626262	03/01/2023	1,000	1,500	2,000	998	1,492	1,995	0.993x + 6.086	1.000
B08	SKC	224-PCXR4	626100	03/01/2023	1,000	1,500	2,000	1,003	1,500	2,003	1.012x - 23.308	0.999
B09	SKC	224-PCXR4	626479	03/01/2023	1,000	1,500	2,000	996	1,490	1,994	0.995x + 1.117	1.000
B10	SKC	224-PCXR4	091950	03/01/2023	1,000	1,500	2,000	992	1,503	2,001	1.018x - 36.582	0.999
B11	SKC	224-PCXR8	564315	05/01/2023	1,000	1,500	2,000	996	1,490	1,999	1.003x - 8.256	1.000
B12	SKC	224-PCXR4	034656	05/01/2023	1,000	1,500	2,000	1,003	1,503	2,003	1.010x - 19.324	0.999
B13	SKC	224-PCXR4	602073	05/01/2023	1,000	1,500	2,000	995	1,500	1,998	1.001x - 3.474	1.000
B14	SKC	224-PCXR4	626313	04/01/2023	1,000	1,500	2,000	999	1,491	1,988	0.992x + 6.844	1.000
B15	SKC	224-PCXR4	626474	04/01/2023	1,000	1,500	2,000	1,001	1,502	2,005	1.014x - 25.558	0.999
B16	SKC	224-PCXR4	626477	04/01/2023	1,000	1,500	2,000	994	1,504	2,001	1.015x - 31.345	0.999
B17	SKC	224-PCXR4	626860	04/01/2023	1,000	1,500	2,000	997	1,494	1,991	0.997x - 0.359	1.000
B18	SKC	224-PCXR4	691484	04/01/2023	1,000	1,500	2,000	1,003	1,500	2,001	1.008x - 17.589	0.999
B19	SKC	224-PCXR4	691599	03/01/2023	1,000	1,500	2,000	993	1,503	1,999	1.007x - 11.574	1.000
B20	SKC	224-PCXR4	691587	03/01/2023	1,000	1,500	2,000	992	1,504	1,999	1.015x - 32.235	0.999
B21	SKC	224-PCXR4	691531	03/01/2023	1,000	1,500	2,000	993	1,499	1,994	1.001x - 7.107	1.000
B22	SKC	224-PCXR4	691654	05/01/2023	1,000	1,500	2,000	1,003	1,501	2,003	1.011x - 21.107	0.999
B23	SKC	224-PCXR4	798393	05/01/2023	1,000	1,500	2,000	992	1,507	2,002	1.018x - 34.883	0.999
B24	SKC	224-PCXR4	626363	05/01/2023	1,000	1,500	2,000	1,000	1,502	2,000	1.011x - 22.387	0.999
B25	SKC	224-PCXR4	798489	05/01/2023	1,000	1,500	2,000	1,001	1,492	2,001	0.998x + 1.101	1.000
B26	SKC	224-PCXR4	798479	05/01/2023	1,000	1,500	2,000	999	1,500	1,993	0.996x + 4.008	1.000
B27	SKC	224-PCXR4	691673	04/01/2023	1,000	1,500	2,000	994	1,503	2,002	1.016x - 32.071	0.999
B28	SKC	224-PCXR4	691570	04/01/2023	1,000	1,500	2,000	1,002	1,500	2,002	1.012x - 22.515	0.999
B29	SKC	224-PCXR4	626472	04/01/2023	1,000	1,500	2,000	1,000	1,496	1,998	1.001x - 4.942	1.000
B30	SKC	224-PCXR4	691489	03/01/2023	1,000	1,500	2,000	1,004	1,510	2,004	1.008x - 12.460	0.999
B31	SKC	224-PCXR4	691509	03/01/2023	1,000	1,500	2,000	992	1,497	1,998	1.006x - 12.711	1.000
B32	SKC	224-PCXR4	091567	05/01/2023	1,000	1,500	2,000	991	1,504	2,001	1.016x - 32.322	0.999
B33	SKC	224-PCXR4	091756	05/01/2023	1,000	1,500	2,000	993	1,497	1,991	0.997x - 0.004	1.000
B34	SKC	224-PCXR4	612962	05/01/2023	1,000	1,500	2,000	1,002	1,501	2,002	1.007x - 14.195	1.000
B35	SKC	224-PCXR4	602682	05/01/2023	1,000	1,500	2,000	993	1,498	1,995	1.002x - 8.448	1.000
B36	SKC	224-PCXR4	626164	03/01/2023	1,000	1,500	2,000	999	1,496	1,999	1.001x - 5.424	1.000
B37	SKC	224-PCXR4	626256	03/01/2023	1,000	1,500	2,000	994	1,506	1,999	1.013x - 27.815	0.999
B38	SKC	224-PCXR4	626167	03/01/2023	1,000	1,500	2,000	997	1,496	1,996	0.999x - 0.997	1.000
B39	SKC	224-PCXR4	034637	03/01/2023	1,000	1,500	2,000	1,005	1,501	2,001	1.010x - 18.618	0.999
B40	SKC	224-PCXR4	798349	05/01/2023	1,000	1,500	2,000	994	1,506	1,999	1.014x - 29.602	0.999

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B41	SKC	224-PCXR4	612669	05/01/2023	1,000	1,500	2,000	998	1,497	1,990	0.997x + 0.718	1.000
B42	SKC	224-PCXR4	626041	05/01/2023	1,000	1,500	2,000	1,004	1,498	1,991	0.986x + 18.291	1.000
B43	SKC	224-PCXR4	034636	05/01/2023	1,000	1,500	2,000	1,000	1,501	1,992	0.991x + 11.882	1.000
B44	SKC	224-PCXR8	529341	06/01/2023	1,000	1,500	2,000	1,002	1,502	2,002	1.005x - 9.213	1.000
B45	SKC	224-PCXR8	529594	06/01/2023	1,000	1,500	2,000	999	1,501	1,989	0.991x + 11.184	1.000
B46	SKC	224-PCXR8	566743	06/01/2023	1,000	1,500	2,000	995	1,504	2,002	1.014x - 30.571	0.999
B47	SKC	224-PCXR8	566747	06/01/2023	1,000	1,500	2,000	1,002	1,502	2,004	1.013x - 24.601	0.999
B48	SKC	224-PCXR8	566753	04/01/2023	1,000	1,500	2,000	1,000	1,494	1,998	0.998x + 0.319	1.000
B49	SKC	224-PCXR8	566780	04/01/2023	1,000	1,500	2,000	1,003	1,502	2,006	1.013x - 23.982	0.999
B50	SKC	224-PCXR8	500400	04/01/2023	1,000	1,500	2,000	1,001	1,496	2,002	1.001x - 3.538	1.000
B51	SKC	224-PCXR8	500363	04/01/2023	1,000	1,500	2,000	996	1,504	1,999	1.011x - 25.031	0.999
B52	SKC	224-PCXR8	093186	04/01/2023	1,000	1,500	2,000	995	1,496	1,994	0.997x - 0.602	1.000
B53	SKC	224-PCXR8	707670	03/01/2023	1,000	1,500	2,000	1,002	1,500	2,002	1.008x - 15.403	0.999
B54	SKC	224-PCXR3	509821	03/01/2023	1,000	1,500	2,000	993	1,502	2,001	1.017x - 34.237	0.999
B55	SKC	224-PCXR3	510710	03/01/2023	1,000	1,500	2,000	999	1,494	1,994	0.997x - 0.989	1.000
B56	SKC	224-PCXR3	511450	03/01/2023	1,000	1,500	2,000	1,002	1,500	2,001	1.004x - 8.081	1.000
B57	SKC	224-PCXR3	510798	06/01/2023	1,000	1,500	2,000	997	1,492	1,998	1.000x - 2.680	1.000
B58	SKC	224-PCXR3	509852	06/01/2023	1,000	1,500	2,000	1,000	1,498	1,999	1.007x - 18.953	0.999
B59	SKC	224-PCXR3	509862	06/01/2023	1,000	1,500	2,000	996	1,503	1,994	0.997x + 3.235	1.000
B60	SKC	224-PCXR3	512655	06/01/2023	1,000	1,500	2,000	1,002	1,500	2,003	1.006x - 11.407	1.000
B61	SKC	224-PCXR3	503915	06/01/2023	1,000	1,500	2,000	994	1,489	1,998	1.004x - 12.623	1.000
B62	SKC	224-PCXR3	505975	06/01/2023	1,000	1,500	2,000	999	1,494	1,996	0.997x + 0.343	1.000
B63	SKC	224-PCXR3	511432	03/01/2023	1,000	1,500	2,000	991	1,501	1,999	1.016x - 34.624	0.999
B64	SKC	224-PCXR3	508302	03/01/2023	1,000	1,500	2,000	997	1,492	1,989	0.992x + 6.226	1.000
B65	SKC	224-PCXR3	508310	03/01/2023	1,000	1,500	2,000	1,002	1,500	2,003	1.007x - 13.936	1.000
B66	SKC	224-PCXR3	509861	03/01/2023	1,000	1,500	2,000	1,002	1,491	1,991	0.987x + 14.183	1.000
B67	SKC	224-PCXR3	506295	04/01/2023	1,000	1,500	2,000	993	1,508	2,004	1.009x - 15.555	1.000
B68	SKC	224-PCXR3	505872	04/01/2023	1,000	1,500	2,000	1,002	1,490	1,997	0.995x + 3.841	1.000
B69	SKC	224-PCXR3	508375	04/01/2023	1,000	1,500	2,000	1,002	1,499	2,000	1.010x - 20.772	0.999
B70	SKC	224-PCXR3	510623	05/01/2023	1,000	1,500	2,000	992	1,503	1,997	1.002x - 5.855	1.000
B71	SKC	224-PCXR3	508367	05/01/2023	1,000	1,500	2,000	992	1,506	2,002	1.017x - 34.791	0.999
B72	SKC	224-PCXR3	505977	05/01/2023	1,000	1,500	2,000	1,001	1,498	1,993	0.991x + 8.962	1.000
B73	SKC	224-PCXR3	512606	05/01/2023	1,000	1,500	2,000	1,002	1,501	2,005	1.009x - 14.785	1.000
B74	SKC	224-PCXR3	505993	05/01/2023	1,000	1,500	2,000	996	1,495	1,994	1.000x - 6.916	1.000
B75	SKC	224-PCXR3	509820	04/01/2023	1,000	1,500	2,000	995	1,498	1,990	0.996x + 1.791	1.000
B76	SKC	224-PCXR3	509811	04/01/2023	1,000	1,500	2,000	993	1,498	1,998	1.006x - 14.322	1.000
B77	SKC	224-PCXR3	508301	04/01/2023	1,000	1,500	2,000	1,000	1,501	2,003	1.014x - 26.603	0.999
B78	SKC	224-PCXR3	510677	04/01/2023	1,000	1,500	2,000	995	1,503	1,999	1.013x - 28.158	0.999
B79	SKC	224-PCXR3	510920	03/01/2023	1,000	1,500	2,000	994	1,493	1,994	0.999x - 4.184	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R²
B80	SKC	224-PCXR3	504569	03/01/2023	1,000	1,500	2,000	1,002	1,499	2,002	1.012x - 24.026	0.999
B81	SKC	224-PCXR3	503480	03/01/2023	1,000	1,500	2,000	996	1,499	2,000	1.014x - 30.524	0.999
B82	SKC	224-PCXR3	505673	06/01/2023	1,000	1,500	2,000	994	1,498	1,996	1.001x - 5.943	1.000
B83	SKC	224-PCXR3	510785	06/01/2023	1,000	1,500	2,000	1,010	1,499	2,002	1.004x - 10.466	0.999
B84	SKC	224-PCXR3	508333	06/01/2023	1,000	1,500	2,000	997	1,495	1,991	0.996x + 1.260	1.000
B85	SKC	224-PCXR3	505757	06/01/2023	1,000	1,500	2,000	994	1,502	1,998	1.005x - 13.844	1.000
B86	SKC	224-PCXR3	512625	03/01/2023	1,000	1,500	2,000	1,013	1,503	2,004	1.001x - 0.726	0.999
B87	SKC	224-PCXR3	504324	03/01/2023	1,000	1,500	2,000	998	1,496	2,000	1.000x - 1.109	1.000
B88	SKC	224-PCXR3	508307	03/01/2023	1,000	1,500	2,000	996	1,498	1,994	0.996x + 1.532	1.000
B89	SKC	224-PCXR3	509860	04/01/2023	1,000	1,500	2,000	1,000	1,499	2,003	1.008x - 15.156	1.000
B90	SKC	224-PCXR3	508366	04/01/2023	1,000	1,500	2,000	993	1,508	1,999	1.006x - 12.512	1.000
B91	SKC	224-PCXR3	510919	04/01/2023	1,000	1,500	2,000	1,000	1,498	1,996	0.990x + 8.719	1.000
B92	SKC	224-PCXR3	510987	04/01/2023	1,000	1,500	2,000	1,002	1,501	1,999	1.000x + 0.299	1.000
B93	SKC	224-PCXR3	509845	04/01/2023	1,000	1,500	2,000	995	1,496	2,004	1.009x - 16.979	1.000
B94	SKC	224-PCXR8	A127871	03/01/2023	1,000	1,500	2,000	1,000	1,500	2,002	1.007x - 19.105	0.999
B95	SKC	224-PCXR8	A127921	03/01/2023	1,000	1,500	2,000	993	1,502	2,001	1.015x - 30.898	0.999
B96	SKC	224-PCXR8	A127942	03/01/2023	1,000	1,500	2,000	998	1,498	1,995	0.998x - 1.485	1.000
B97	SKC	224-PCXR8	A127955	03/01/2023	1,000	1,500	2,000	1,003	1,501	2,003	1.011x - 20.356	0.999
B98	SKC	224-PCXR8	A127956	03/01/2023	1,000	1,500	2,000	996	1,498	1,997	1.003x - 7.473	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R²
B01	SKC	224-PCXR4	262101	04/04/2023	1,000	1,500	2,000	994	1,498	2,003	1.005x - 7.897	1.000
B02	SKC	224-PCXR4	626166	04/04/2023	1,000	1,500	2,000	1,004	1,503	2,003	1.010x - 19.866	0.999
B03	SKC	224-PCXR4	612968	07/04/2023	1,000	1,500	2,000	995	1,496	2,001	1.007x - 13.664	1.000
B04	SKC	224-PCXR4	602804	05/04/2023	1,000	1,500	2,000	998	1,499	1,994	0.999x - 1.611	1.000
B05	SKC	224-PCXR4	612693	07/04/2023	1,000	1,500	2,000	1,002	1,501	2,004	1.014x - 24.856	0.999
B06	SKC	224-PCXR4	262188	07/04/2023	1,000	1,500	2,000	994	1,509	2,006	1.012x - 21.589	0.999
B07	SKC	224-PCXR4	626262	04/04/2023	1,000	1,500	2,000	997	1,490	1,996	0.994x + 3.454	1.000
B08	SKC	224-PCXR4	626100	04/04/2023	1,000	1,500	2,000	1,001	1,499	2,005	1.015x - 27.137	0.999
B09	SKC	224-PCXR4	626479	05/04/2023	1,000	1,500	2,000	997	1,492	1,994	0.994x + 2.385	1.000
B10	SKC	224-PCXR4	091950	03/04/2023	1,000	1,500	2,000	993	1,504	2,005	1.013x - 23.779	1.000
B11	SKC	224-PCXR8	564315	10/04/2023	1,000	1,500	2,000	995	1,492	1,998	1.002x - 7.259	1.000
B12	SKC	224-PCXR4	034656	04/04/2023	1,000	1,500	2,000	1,002	1,504	2,001	1.009x - 17.609	0.999
B13	SKC	224-PCXR4	602073	04/04/2023	1,000	1,500	2,000	997	1,501	2,000	1.004x - 7.622	1.000
B14	SKC	224-PCXR4	626313	03/04/2023	1,000	1,500	2,000	997	1,492	1,991	0.996x + 1.699	1.000
B15	SKC	224-PCXR4	626474	07/04/2023	1,000	1,500	2,000	1,003	1,503	2,006	1.013x - 23.245	0.999
B16	SKC	224-PCXR4	626477	03/04/2023	1,000	1,500	2,000	995	1,506	2,003	1.011x - 22.132	0.999
B17	SKC	224-PCXR4	626860	04/04/2023	1,000	1,500	2,000	996	1,493	1,993	1.000x - 4.627	1.000
B18	SKC	224-PCXR4	691484	04/04/2023	1,000	1,500	2,000	1,001	1,496	2,002	1.010x - 21.179	0.999
B19	SKC	224-PCXR4	691599	04/04/2023	1,000	1,500	2,000	994	1,504	2,000	1.006x - 10.498	1.000
B20	SKC	224-PCXR4	691587	03/04/2023	1,000	1,500	2,000	991	1,502	2,000	1.016x - 35.102	0.999
B21	SKC	224-PCXR4	691531	04/04/2023	1,000	1,500	2,000	994	1,501	1,995	1.001x - 5.153	1.000
B22	SKC	224-PCXR4	691654	07/04/2023	1,000	1,500	2,000	1,000	1,502	2,004	1.014x - 25.574	0.999
B23	SKC	224-PCXR4	798393	05/04/2023	1,000	1,500	2,000	990	1,508	2,004	1.013x - 23.994	1.000
B24	SKC	224-PCXR4	626363	03/04/2023	1,000	1,500	2,000	1,002	1,503	1,999	1.009x - 18.837	0.999
B25	SKC	224-PCXR4	798489	07/04/2023	1,000	1,500	2,000	1,002	1,494	2,000	0.997x + 3.494	1.000
B26	SKC	224-PCXR4	798479	07/04/2023	1,000	1,500	2,000	1,001	1,501	1,994	0.995x + 5.564	1.000
B27	SKC	224-PCXR4	691673	04/04/2023	1,000	1,500	2,000	995	1,505	2,004	1.013x - 25.091	0.999
B28	SKC	224-PCXR4	691570	04/04/2023	1,000	1,500	2,000	1,003	1,501	2,001	1.010x - 19.922	0.999
B29	SKC	224-PCXR4	626472	05/04/2023	1,000	1,500	2,000	1,001	1,498	2,000	0.999x - 1.831	1.000
B30	SKC	224-PCXR4	691489	04/04/2023	1,000	1,500	2,000	1,002	1,507	2,003	1.009x - 13.936	0.999
B31	SKC	224-PCXR4	691509	07/04/2023	1,000	1,500	2,000	994	1,496	1,997	1.004x - 9.680	1.000
B32	SKC	224-PCXR4	091567	10/04/2023	1,000	1,500	2,000	992	1,506	2,001	1.013x - 25.542	0.999
B33	SKC	224-PCXR4	091756	05/04/2023	1,000	1,500	2,000	993	1,498	1,992	0.998x - 1.121	1.000
B34	SKC	224-PCXR4	612962	07/04/2023	1,000	1,500	2,000	1,002	1,503	2,003	1.008x - 14.753	0.999
B35	SKC	224-PCXR4	602682	05/04/2023	1,000	1,500	2,000	991	1,497	1,996	1.003x - 11.598	1.000
B36	SKC	224-PCXR4	626164	05/04/2023	1,000	1,500	2,000	997	1,495	1,998	1.002x - 8.097	1.000
B37	SKC	224-PCXR4	626256	07/04/2023	1,000	1,500	2,000	993	1,505	1,996	1.012x - 27.161	0.999
B38	SKC	224-PCXR4	626167	07/04/2023	1,000	1,500	2,000	998	1,493	1,997	1.003x - 8.615	1.000
B39	SKC	224-PCXR4	034637	10/04/2023	1,000	1,500	2,000	1,003	1,500	2,003	1.013x - 23.125	0.999
B40	SKC	224-PCXR4	798349	07/04/2023	1,000	1,500	2,000	993	1,507	1,998	1.015x - 30.204	0.999

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)			y	R ²
					1	2	3	1	2	3		
B41	SKC	224-PCXR4	612669	07/04/2023	1,000	1,500	2,000	997	1,496	1,991	0.998x - 1.396	1.000
B42	SKC	224-PCXR4	626041	10/04/2023	1,000	1,500	2,000	1,006	1,496	1,992	0.988x + 14.223	1.000
B43	SKC	224-PCXR4	034636	07/04/2023	1,000	1,500	2,000	1,001	1,503	1,993	0.992x + 8.810	1.000
B44	SKC	224-PCXR8	529341	10/04/2023	1,000	1,500	2,000	1,000	1,499	2,005	1.008x - 14.358	1.000
B45	SKC	224-PCXR8	529594	10/04/2023	1,000	1,500	2,000	998	1,506	1,987	0.990x + 12.580	1.000
B46	SKC	224-PCXR8	566743	05/04/2023	1,000	1,500	2,000	996	1,502	2,000	1.012x - 26.902	0.999
B47	SKC	224-PCXR8	566747	07/04/2023	1,000	1,500	2,000	998	1,501	2,002	1.014x - 27.552	0.999
B48	SKC	224-PCXR8	566753	10/04/2023	1,000	1,500	2,000	998	1,493	1,996	0.997x - 0.359	1.000
B49	SKC	224-PCXR8	566780	05/04/2023	1,000	1,500	2,000	1,007	1,501	2,007	1.011x - 19.156	0.999
B50	SKC	224-PCXR8	500400	07/04/2023	1,000	1,500	2,000	1,004	1,495	2,004	1.000x - 1.663	1.000
B51	SKC	224-PCXR8	500363	04/04/2023	1,000	1,500	2,000	997	1,502	1,998	1.008x - 21.322	0.999
B52	SKC	224-PCXR8	093186	05/04/2023	1,000	1,500	2,000	993	1,493	1,995	1.000x - 6.106	1.000
B53	SKC	224-PCXR8	707670	05/04/2023	1,000	1,500	2,000	1,000	1,498	2,002	1.009x - 18.883	0.999
B54	SKC	224-PCXR3	509821	05/04/2023	1,000	1,500	2,000	995	1,500	2,001	1.016x - 32.482	0.999
B55	SKC	224-PCXR3	510710	10/04/2023	1,000	1,500	2,000	998	1,497	1,992	0.996x - 0.191	1.000
B56	SKC	224-PCXR3	511450	05/04/2023	1,000	1,500	2,000	1,003	1,501	2,003	1.005x - 8.081	1.000
B57	SKC	224-PCXR3	510798	05/04/2023	1,000	1,500	2,000	999	1,490	2,000	1.001x - 2.920	1.000
B58	SKC	224-PCXR3	509852	10/04/2023	1,000	1,500	2,000	1,002	1,496	1,998	1.004x - 15.922	0.999
B59	SKC	224-PCXR3	509862	10/04/2023	1,000	1,500	2,000	998	1,501	1,996	0.996x + 4.471	1.000
B60	SKC	224-PCXR3	512655	07/04/2023	1,000	1,500	2,000	1,003	1,499	2,004	1.005x - 9.971	1.000
B61	SKC	224-PCXR3	503915	10/04/2023	1,000	1,500	2,000	993	1,488	1,999	1.007x - 15.934	1.000
B62	SKC	224-PCXR3	505975	10/04/2023	1,000	1,500	2,000	1,001	1,495	1,997	1.000x - 4.802	1.000
B63	SKC	224-PCXR3	511432	07/04/2023	1,000	1,500	2,000	993	1,500	2,000	1.015x - 32.709	0.999
B64	SKC	224-PCXR3	508302	05/04/2023	1,000	1,500	2,000	998	1,491	1,987	0.989x + 9.855	1.000
B65	SKC	224-PCXR3	508310	10/04/2023	1,000	1,500	2,000	998	1,502	2,005	1.012x - 20.596	1.000
B66	SKC	224-PCXR3	509861	10/04/2023	1,000	1,500	2,000	1,000	1,492	1,992	0.990x + 10.912	1.000
B67	SKC	224-PCXR3	506295	07/04/2023	1,000	1,500	2,000	993	1,506	2,002	1.007x - 13.999	1.000
B68	SKC	224-PCXR3	505872	05/04/2023	1,000	1,500	2,000	998	1,488	1,997	0.998x - 1.743	1.000
B69	SKC	224-PCXR3	508375	04/04/2023	1,000	1,500	2,000	1,004	1,502	2,002	1.009x - 18.897	0.999
B70	SKC	224-PCXR3	510623	05/04/2023	1,000	1,500	2,000	994	1,505	1,998	1.004x - 8.846	1.000
B71	SKC	224-PCXR3	508367	10/04/2023	1,000	1,500	2,000	994	1,503	2,003	1.011x - 23.544	0.999
B72	SKC	224-PCXR3	505977	10/04/2023	1,000	1,500	2,000	1,005	1,493	1,992	0.988x + 13.309	1.000
B73	SKC	224-PCXR3	512606	05/04/2023	1,000	1,500	2,000	1,000	1,504	2,004	1.008x - 14.506	1.000
B74	SKC	224-PCXR3	505993	05/04/2023	1,000	1,500	2,000	997	1,497	1,996	1.001x - 7.514	1.000
B75	SKC	224-PCXR3	509820	07/04/2023	1,000	1,500	2,000	997	1,496	1,992	0.997x + 0.195	1.000
B76	SKC	224-PCXR3	509811	05/04/2023	1,000	1,500	2,000	995	1,498	1,999	1.004x - 11.212	1.000
B77	SKC	224-PCXR3	508301	10/04/2023	1,000	1,500	2,000	1,003	1,502	2,004	1.013x - 23.811	0.999
B78	SKC	224-PCXR3	510677	04/04/2023	1,000	1,500	2,000	997	1,505	2,000	1.007x - 16.113	0.999
B79	SKC	224-PCXR3	510920	10/04/2023	1,000	1,500	2,000	996	1,495	1,993	0.998x - 1.232	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
 Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}\text{C}$
 Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B80	SKC	224-PCXR3	504569	05/04/2023	1,000	1,500	2,000	1,003	1,498	2,003	1.011x - 22.431	0.999
B81	SKC	224-PCXR3	503480	05/04/2023	1,000	1,500	2,000	995	1,500	2,001	1.016x - 32.797	0.999
B82	SKC	224-PCXR3	505673	05/04/2023	1,000	1,500	2,000	995	1,496	1,997	1.003x - 7.259	1.000
B83	SKC	224-PCXR3	510785	05/04/2023	1,000	1,500	2,000	1,007	1,498	2,001	1.006x - 13.816	0.999
B84	SKC	224-PCXR3	508333	10/04/2023	1,000	1,500	2,000	995	1,498	1,993	0.998x - 1.970	1.000
B85	SKC	224-PCXR3	505757	10/04/2023	1,000	1,500	2,000	996	1,500	2,000	1.004x - 12.009	1.000
B86	SKC	224-PCXR3	512625	05/04/2023	1,000	1,500	2,000	1,011	1,501	2,005	1.002x - 3.877	0.999
B87	SKC	224-PCXR3	504324	05/04/2023	1,000	1,500	2,000	999	1,495	1,998	0.999x + 0.606	1.000
B88	SKC	224-PCXR3	508307	05/04/2023	1,000	1,500	2,000	997	1,497	1,992	0.994x + 4.682	1.000
B89	SKC	224-PCXR3	509860	05/04/2023	1,000	1,500	2,000	1,001	1,498	2,002	1.007x - 13.92	1.000
B90	SKC	224-PCXR3	508366	05/04/2023	1,000	1,500	2,000	995	1,507	1,998	1.004x - 9.640	1.000
B91	SKC	224-PCXR3	510919	04/04/2023	1,000	1,500	2,000	1,003	1,500	1,995	0.988x + 13.505	1.000
B92	SKC	224-PCXR3	510987	05/04/2023	1,000	1,500	2,000	1,003	1,503	1,998	0.997x + 5.125	1.000
B93	SKC	224-PCXR3	509845	10/04/2023	1,000	1,500	2,000	996	1,498	2,003	1.007x - 13.628	1.000
B94	SKC	224-PCXR8	A127871	04/04/2023	1,000	1,500	2,000	1,001	1,495	2,003	1.006x - 18.746	0.999
B95	SKC	224-PCXR8	A127921	03/04/2023	1,000	1,500	2,000	995	1,504	2,001	1.013x - 26.112	0.999
B96	SKC	224-PCXR8	A127942	07/04/2023	1,000	1,500	2,000	999	1,499	1,997	1.000x - 2.010	1.000
B97	SKC	224-PCXR8	A127955	07/04/2023	1,000	1,500	2,000	1,006	1,503	2,005	1.011x - 18.638	0.999
B98	SKC	224-PCXR8	A127956	07/04/2023	1,000	1,500	2,000	994	1,497	1,998	1.005x - 11.436	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
 Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-B01	Dwyer	VFB-65	05/01/2023	500	1,000	2,000	506.1	989.5	1973.5	0.990x + 8.311	1.000
H-B02	Dwyer	VFB-65	05/01/2023	500	1,000	2,000	494.9	998.2	1995.3	0.993x + 4.772	1.000
H-B03	Dwyer	VFB-65	05/01/2023	500	1,000	2,000	498.3	987.5	2010.6	1.005x - 15.690	0.999
H-B04	Dwyer	VFB-65	03/01/2023	500	1,000	2,000	500.4	999.5	2008.7	0.998x - 2.369	1.000
H-B05	Dwyer	VFB-65	03/01/2023	500	1,000	2,000	499.0	997.8	1972.3	0.981x + 20.957	0.999
H-B06	Dwyer	VFB-65	03/01/2023	500	1,000	2,000	503.6	995.0	1981.4	1.005x - 8.788	0.999
H-B07	Dwyer	VFB-65	04/01/2023	500	1,000	2,000	504.1	989.0	2018.7	1.002x - 2.144	1.000
H-B08	Dwyer	VFB-65	06/01/2023	500	1,000	2,000	499.8	999.2	1975.8	0.996x + 3.270	0.999
H-B09	Dwyer	VFB-65	06/01/2023	500	1,000	2,000	503.7	1006.6	2014.3	0.994x + 14.202	1.000
H-B10	Dwyer	VFB-65	06/01/2023	500	1,000	2,000	496.1	998.6	2012.4	0.997x + 2.443	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
 Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-B01	Dwyer	VFA-21	04/01/2023	50	100	200	50.7	99.1	198.5	0.985x + 1.102	1.000
L-B02	Dwyer	VFA-21	04/01/2023	50	100	200	51.0	99.4	198.7	0.994x + 1.097	0.999
L-B03	Dwyer	VFA-21	06/01/2023	50	100	200	50.8	99.2	198.3	1.006x – 0.866	1.000
L-B04	Dwyer	VFA-21	06/01/2023	50	100	200	49.1	101.6	201.1	1.016x – 1.187	1.000
L-B05	Dwyer	VFA-21	06/01/2023	50	100	200	50.5	98.1	200.8	1.001x + 0.196	0.999
L-B06	Dwyer	VFA-21	03/01/2023	50	100	200	50.1	100.1	203.4	1.010x + 0.062	1.000
L-B07	Dwyer	VFA-21	03/01/2023	50	100	200	49.4	100.8	199.7	1.019x – 2.253	1.000
L-B08	Dwyer	VFA-21	03/01/2023	50	100	200	49.8	101.3	198.1	0.999x – 0.218	1.000
L-B09	Dwyer	VFA-21	03/01/2023	50	100	200	50.0	99.2	200.7	0.993x + 1.212	0.999
L-B10	Dwyer	VFA-21	05/01/2023	50	100	200	51.0	99.8	202.8	1.004x + 0.747	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-B01	Dwyer	VFB-65	05/04/2023	500	1,000	2,000	506.9	990.3	1974.3	0.989x + 9.271	1.000
H-B02	Dwyer	VFB-65	04/04/2023	500	1,000	2,000	495.3	999.1	1996.1	0.994x + 4.127	1.000
H-B03	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	497.5	988.1	2009.6	1.003x - 14.485	0.999
H-B04	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	501.2	1000.3	2006.5	0.997x - 1.216	1.000
H-B05	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	500.2	999.6	1974.3	0.980x + 21.307	0.999
H-B06	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	504.3	996.2	1984.0	1.004x - 6.770	1.000
H-B07	Dwyer	VFB-65	04/04/2023	500	1,000	2,000	502.3	990.7	2016.7	1.001x - 1.154	1.000
H-B08	Dwyer	VFB-65	05/04/2023	500	1,000	2,000	500.2	1000.6	1979.8	0.995x + 5.040	0.999
H-B09	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	504.4	1007.4	2010.7	0.993x + 15.376	1.000
H-B10	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	495.7	1001.6	2009.2	0.996x + 3.956	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-B01	Dwyer	VFA-21	05/04/2023	50	100	200	50.3	98.7	198.9	0.986x + 0.859	1.000
L-B02	Dwyer	VFA-21	04/04/2023	50	100	200	50.6	99.8	198.3	0.995x + 0.956	0.999
L-B03	Dwyer	VFA-21	07/04/2023	50	100	200	50.4	99.6	197.9	1.009x - 1.350	1.000
L-B04	Dwyer	VFA-21	07/04/2023	50	100	200	49.5	102.0	200.7	1.012x - 0.487	1.000
L-B05	Dwyer	VFA-21	07/04/2023	50	100	200	50.9	98.9	201.2	0.998x + 1.040	0.999
L-B06	Dwyer	VFA-21	07/04/2023	50	100	200	50.8	99.7	202.8	1.009x + 0.150	1.000
L-B07	Dwyer	VFA-21	04/04/2023	50	100	200	49.0	101.2	200.5	1.014x - 1.381	1.000
L-B08	Dwyer	VFA-21	05/04/2023	50	100	200	50.2	102.1	197.7	0.997x + 0.307	1.000
L-B09	Dwyer	VFA-21	07/04/2023	50	100	200	50.8	99.6	201.1	0.990x + 2.095	0.999
L-B10	Dwyer	VFA-21	10/04/2023	50	100	200	51.0	99.0	203.2	1.005x + 0.453	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 23M2441

REFERENCE No : 68471-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY : [REDACTED]
PONGSAK J.

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 23M2441

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23°C \pm 1°C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.0001	-0.0001	0.00011
100.00	100.0001	-0.0001	0.00019
200.00	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

ระดับความร้อนในสถานประกอบการ



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp^o34

SERIAL NO. : TEL080034

CLID. NO. : 231801937

JOB CONTROL NO. : 221028109974

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 28 October 2022

DATE OF ISSUED : 31 October 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Oranut Kamchatphai
Calibration Engineer



Approved By : Mongkol Yotsoontorn
Authorized Signatory

31 October 2022

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22109974

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp^o34

SERIAL NO. : TEL080034

DATE OF CALIBRATION : 29 October 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-74**. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.

Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Thunder Scientific Corporation.

Certificate No. 19944, Due Date 26 January 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22109974

F3-011-04/01-12



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter (thermal environment monitor).

CALIBRATION DATA

1. CORRECTION OF TEMPERATURE : WET

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	30.0	+0.01	0.40
35.0	35.00	35.0	0.00	
40.0	40.01	39.9	+0.11	

2. CORRECTION OF TEMPERATURE : DRY

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	30.2	-0.19	0.40
35.0	35.00	35.1	-0.10	
40.0	40.01	40.1	-0.09	

3. CORRECTION OF TEMPERATURE : GLOBE BULB

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	30.0	+0.01	0.40
35.0	35.00	34.9	+0.10	
40.0	40.01	39.9	+0.11	

Note. The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22109974

F3-011-04/01-12

page 3 of 3



@clccalibration

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp°32

SERIAL NO. : TPH050046

CLID. NO. : 231801943

JOB CONTROL NO. : 221028109979

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 28 October 2022

DATE OF ISSUED : 31 October 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Oranut Kamchatphai
Calibration Engineer



Approved By : Mongkol Yotsoontorn
Authorized Signatory
31 October 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22109979

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp^o32

SERIAL NO. : TPH050046

DATE OF CALIBRATION : 29 October 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-74**. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.

Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Thunder Scientific Corporation.
Certificate No. 19944, Due Date 26 January 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22109979

F3-011-04/01-12

page 2 of 3



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter (thermal environment monitor).

CALIBRATION DATA

1. CORRECTION OF TEMPERATURE : WET

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	30.0	+0.01	0.40
35.0	35.00	35.0	0.00	
40.0	40.01	39.8	+0.21	

2. CORRECTION OF TEMPERATURE : DRY

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	30.1	-0.09	0.40
35.0	35.00	35.1	-0.10	
40.0	40.01	40.0	+0.01	

3. CORRECTION OF TEMPERATURE : GLOBE BULB

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	30.0	+0.01	0.40
35.0	35.00	35.0	0.00	
40.0	40.01	39.8	+0.21	

Note. The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22109979

F3-011-04/01-12

page 3 of 3





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com... www.spscon.com

Heat B091_1/23

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No.	: B11	Verification Date	: 20 April 2023
Brand	: 3M	Ambient Temp.	: 24.5 °C
Model	: QUESTemp ^o 34	Barometric Pressure	: 1011 mmbar
Serial No.	: TEL080034	Relative Humidity	: 49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C , DB = 47.1 °C , G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.5	0.0	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.0	0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.4	-0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by :



(Mr. Adul Dangklom)

Approved by :



(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Heat B091_2/23

Heat Stress WBGT Meter Verification Report

Verification Data

Heat Stress WBGT Meter No.	: B28	Verification Date	: 20 April 2023
Brand	: 3M	Ambient Temp.	: 24.5 °C
Model	: QUESTemp [®] 32	Barometric Pressure	: 1011 mmbar
Serial No.	: TPH050046	Relative Humidity	: 49 %

Verification Module (Electronic Sensor Check) :

Verification Module No. : 21 WB = 12.5 °C , DB = 47.1 °C , G = 69.3 °C

Result of Verification : Without Adjustment

Wet Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.5	0.0	± 0.5

Dry Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.0	0.1	± 0.5

Globe Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.4	-0.1	± 0.5

UUC* = UNIT UNDER CALIBRATION

Verified by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)