

เอกสารแนบ 10
ใบสอบเทียบเครื่องมือตรวจวัด

TSP High Volume Sampler Calibration

SITE

Site: Blue
Sampler: PM#18
Recorder: Kimhan P.

Date: 08/09/2022
Test: Supackak S.
Approval: Nidida A.

CONDITIONS

Sea Level Pressure (hPa): 1008.0
Temperature (deg C): 32.0
Seasonal SL Press. (hPa): 1013.0
Seasonal Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 756.1
Temperature (deg K): 305.0
Corrected Seasonal (mm Hg): 759.8
Seasonal Temp. (deg K): 303.0

CALIBRATION ORIFICE

Make: Tisch
Model:
Serial#: 1635

Slope: 1.26614
Intercept: -0.02116
Date Certified: 1 Aug 22


TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	8.00	1.185	42.0	26.68
2	7.40	1.062	38.0	24.14
3	5.20	0.937	34.0	21.59
4	3.40	0.760	30.0	19.05
5	2.20	0.593	26.0	16.51

LINEAR REGRESSION

Slope (m)= 16.9572
Intercept (b)= 6.2073
Corr. coeff.(r)= 0.9964
SFR = 1.143
SSP = 40.29
of Observations: 5

Range of Chart 38
at SFR $\pm 10\%$ 42

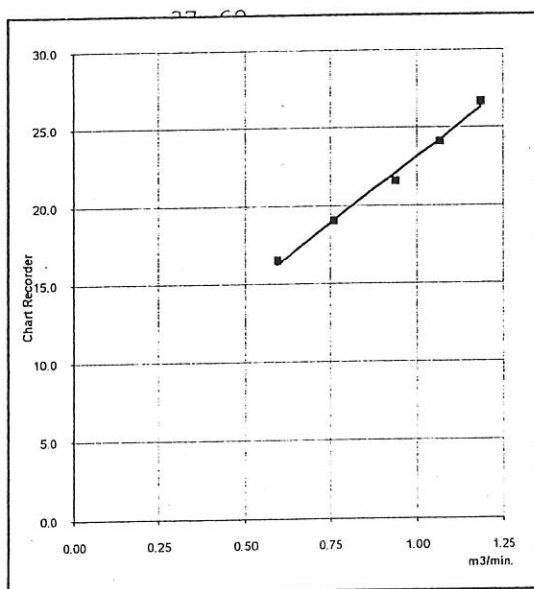

Calibrated by :

Kimhan Paepipat
08/09/2022

Approved by :

Nidida Anansuwanchai
08/09/2022

TSP High Volume Sampler Calibration

SITE

Site: Blue
Sampler: PM#4
Recorder: Kimhan P.

Date: 08/09/2022
Test: Supackak S.
Approval: Nidida A.

CONDITIONS

Sea Level Pressure (hPa): 1008.0
Temperature (deg C): 32.0
Seasonal SL Press. (hPa): 1013.0
Seasonal Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 756.1
Temperature (deg K): 305.0
Corrected Seasonal (mm Hg): 759.8
Seasonal Temp. (deg K): 303.0

CALIBRATION ORIFICE

Make: Tisch
Model:
Serial#: 1635

Slope: 1.26614
Intercept: -0.02116
Date Certified: 1 Aug 22


TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	12.00	1.185	50.0	31.76
2	10.00	1.062	44.0	27.95
3	7.60	0.937	38.0	24.14
4	5.00	0.760	30.0	19.05
5	2.00	0.593	20.0	12.70

LINEAR REGRESSION

Slope (m)= 31.6581
Intercept (b)= -5.6084
Corr. coeff. (r)= 0.9986
SFR = 1.143
SSP = 48.15
of Observations: 5

Range of Chart 44
at SFR $\pm 10\%$ 53

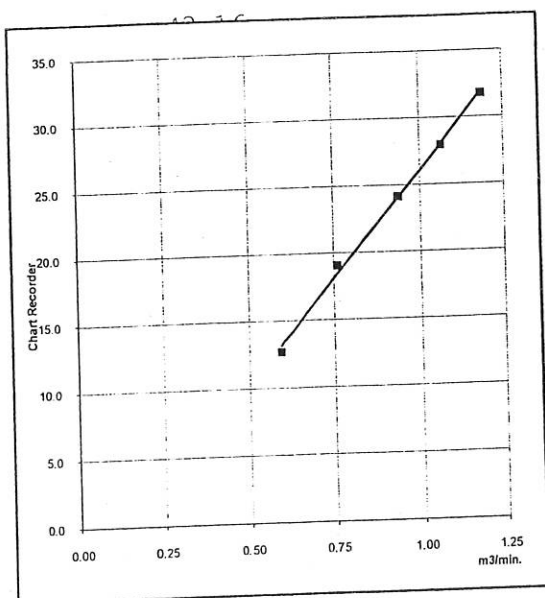

Calibrated by : _____

Kimhan Paepipat
08/09/2022

Approved by : _____

Nidida Anansuwanchai
08/09/2022

TSP High Volume Sampler Calibration

SITE

Site: Blue
Sampler: PM#16
Recorder: Kimhan P.

Date: 08/09/2022

Test: Supackak S.

Approval: Nidida A.

CONDITIONS

Sea Level Pressure (hPa): 1008.0
Temperature (deg C): 32.0
Seasonal SL Press. (hPa): 1013.0
Seasonal Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 756.1
Temperature (deg K): 305.0
Corrected Seasonal (mm Hg): 759.8
Seasonal Temp. (deg K): 303.0

CALIBRATION ORIFICE

Make: Tisch
Model:
Serial#: 1635

Slope: 1.26614
Intercept: -0.02116
Date Certified: 1 Aug 22


TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	9.20	1.185	32.0	20.32
2	7.60	1.062	30.0	19.05
3	5.60	0.937	28.0	17.78
4	2.80	0.760	24.0	15.24
5	2.20	0.593	20.0	12.70

LINEAR REGRESSION

Slope (m)= 12.9075
Intercept (b)= 5.3091
Corr. coeff. (r)= 0.9959
SFR = 1.143
SSP = 31.59
of Observations: 5

Range of Chart 30
at SFR $\pm 10\%$ 33

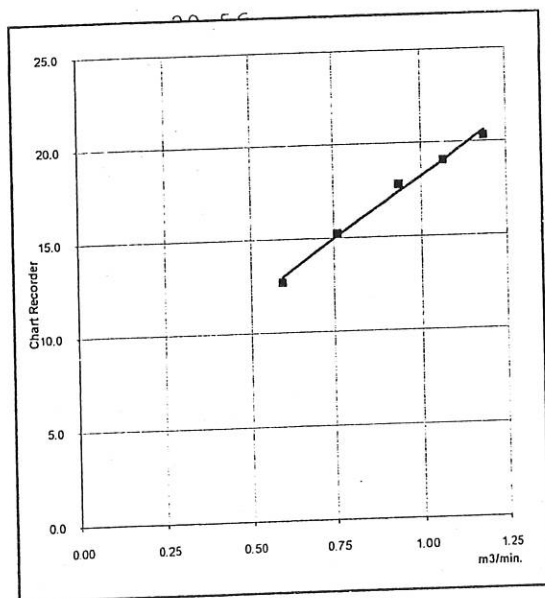

Calibrated by :

Kimhan Paepipat
08/09/2022

Approved by :

Nidida Anansuwanchai
08/09/2022

TSP High Volume Sampler Calibration

Site: Blue
Sampler: TSP#1
Recorder: Kimhan P.

Date: 08/09/2022
Test: Supackak S.
Approval: Nidida A.

CONDITIONS

Sea Level Pressure (hPa): 1008.0
Temperature (deg C): 32.0
Seasonal SL Press. (hPa): 1013.0
Seasonal Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 756.1
Temperature (deg K): 305.0
Corrected Seasonal (mm Hg): 759.8
Seasonal Temp. (deg K): 303.0

CALIBRATION ORIFICE

Make: Tisch
Model:
Serial#: 1635

Qstd Slope: 1.26614
Qstd Intercept: -0.02116
Date Certified: 1 Aug 22

CALIBRATIONS


Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)
1	10.60	2.552	54.0	53.24
2	8.60	2.300	50.0	49.29
3	6.60	2.017	44.0	43.38
4	4.60	1.687	38.0	37.46
5	2.80	1.320	30.0	29.58

LINEAR REGRESSION

Slope = 19.2705
Intercept = 4.5291
Corr. coeff. = 0.9990

of Observations: 5

Range of Chart at 1.1 - 1.7 m3/min. 27
37

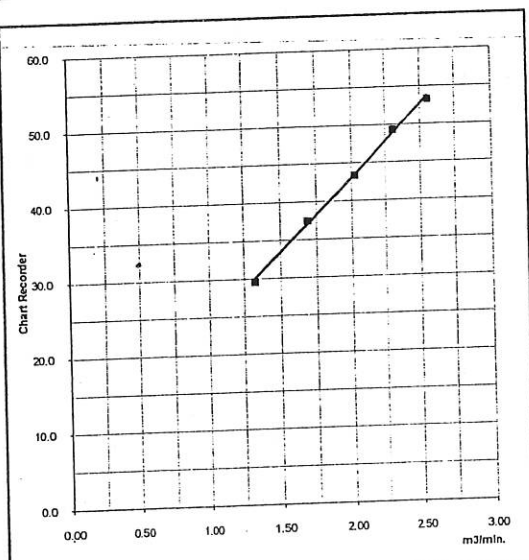

Calibrated by :

Kimhan Paepipat
08/09/2022

Approved by :

Nidida Anansuwanchai
08/09/2022



69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 / 5 คู่สาย www.สอบเทียบเครื่องมือวัด.com

Page : 1 of 3

Customer : Safety Lab Co., Ltd.

20 Soi Borommaratchachonnani 34, Taling Chan Sub-district, Taling
Chan District, Bangkok 10170 Thailand

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 44

Serial Number : PN1916

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 28 Sep 2022

Relative Humidity : 50 % \pm 15 %

Calibration Date : 29 Sep 2022

Location of Calibration : In-Lab

Recommend Due Date : 29 Sep 2023

Calibration Procedure : SP-CPE-04-01

Date of Issue : 30 Sep 2022

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :

(Mr.Worapong Sinthusopa)

Authorized Signatory



Calibration Report

Certificate Number : SPR22090471-7


Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2022

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR22090471-7

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.1	114.0	0.1	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.2	114.1	0.2	0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010104-7

Page : 1 of 3

Customer : Safety Lab Co., Ltd.

20 Soi Borommaratchachonnani 34, Taling Chan Sub-district, Taling
Chan District, Bangkok 10170 Thailand

Equipment Name : Sound Calibrator

Manufacturer : PONPE

Model : N/A

Serial Number : N753415

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 11 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 12 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 12 Jan 2024

Calibration Procedure : In-House Method

Date of Issue : 13 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Karoon Pengsalung

Calibration Officer

Approved by :

(Ms. Bussakorn Chaikaew)

Authorized Signatory



Calibration Report

Certificate Number : SPR23010104-7

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Measuring Receiver	8902A	2950A02471	EF-0005-22	01 Feb 2023
AUDIO Analyzer	8903B	3011A09975	EL05615/22	22 Feb 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

NIMT - The National Institute of Metrology, Thailand.

PCAL - Professional Calibration & Services Co.,Ltd



Result of Calibration

Certificate No. : SPR23010104-7

Page : 3 of 3

Function : Sound Level

UUC Setting (\pm dB)	Standard Reading (dB)	Error (dB)	Uncertainty (\pm dB)
94	93.9	0.10	1.5
114	114.1	-0.10	1.5

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



Metrology and Calibration Department

Electrical Maintenance Division

Electricity Generating Authority of Thailand

81 Moo 11 Bangkruai - Sainoi Rd., Sainoi, Nonthaburi 11150 Tel. (662) 436-8789 Ext. 6155



Certificate of Calibration

Issued by : Vibration Laboratory

Certificate No. : 22V027


Reference No. : CBLUE01V004

Received Date : 08 March 2022

Calibrated Date : 15 March 2022

Page 1 of 5

Client : ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์
Address : 32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพมหานคร 10140
Equipment : VIBRATION METER
Manufacture /Brand : INSTANTEL
Model : Micromate
Serial No./ ID No. : UM8171


(Mr. Bamrung Sangthian)
Authorised Signatory

Issue Date : 16 / March 2022

This certificate is issued in accordance with the conditions of accreditation granted by The National Accreditation Council of Thailand which has assessed the measurement capability of the laboratory and its traceability to recognised national standards and to the units of measurement realised at the corresponding national standards laboratory. This certificate may not be reproduced other than in full, except with the prior written approval of the head of calibration services and environmental analysis department.

FM-02/QP-MCC-09 Rev.3

e-mail : MCC@egat.co.th



Metrology and Calibration Department
Electrical Maintenance Division
Electricity Generating Authority of Thailand

Continued of Calibration Report

Certificate Number. 22V027

Page 2 of 5

Standard Used

The table below is described the calibrator through the International System of Unit.

Description	Manufacture/Model	Serial No.	Traceable No.	Due Date
Conditioning Amplifier Type 2626	Bruel & Kjaer	1242376	AV-0045-20	18 September 2022
Accelerometer Type 8305	Bruel & Kjaer	1262817	AV- 0043-20	02 December 2022
Digital Multimeter /8846A	FLUKE	4330020	21E287	20 September 2022

Ambient Environment :

The Calibration was performed in an environment of $(23 \pm 2) ^\circ\text{C}$ and $(50 \pm 10) \%$ relative humidity.

Measurement Method :

The unit under calibration was calibrated by comparison with standard accelerometer. The calibration method is based on WI-MCC-E-301 by comparison with reference accelerometer standard .

Measurement Results

The measurement results, labeled in the following pages give the calibration results and associated with measurement uncertainties.

Measurement Uncertainty

The Measurement Uncertainty are labeled on the following pages Completed the expanded uncertainty, that was calculated in accordance with the method in M3003, using coverage factor $k = 2$. The value of the measured lies within the assigned ranges of values of confidence level of approximately 95%.

Traceability :

The measurement is traceable to the International System of Unit through

- The National Institute of Metrology (Thailand)
- Metrology and Calibration Department



Metrology and Calibration Department
Electrical Maintenance Division
Electricity Generating Authority of Thailand

Continued of Calibration Report

Certificate Number. 22V027

Page 3 of 5

DESCRIPTION	INSTRUMENT VALUE		UNCERTAINTY
	STANDARD SETTING	UUC READING	
Vertical			
Frequency (Hz)	mm/s _p	mm/s _p	± mm/s _p
* 20	10.00	10.21	0.15
*30	10.00	10.19	0.15
40	10.00	10.18	0.15
80	10.00	10.12	0.15

* Calibration made "Not TISI Accredited" in this Certificate have been included for completeness.

Tranducer Part : ENSL 16117

Condition : Installation by vertical direction



Metrology and Calibration Department
Electrical Maintenance Division
Electricity Generating Authority of Thailand

Continued of Calibration Report

Certificate Number. 22V027

Page 4 of 5

DESCRIPTION	INSTRUMENT VALUE		UNCERTAINTY
	STANDARD SETTING	UUC READING	
Transverse Frequency (Hz)	mm/s _p	mm/s _p	± mm/s _p
*20	10.00	10.22	0.15
*30	10.00	10.07	0.15
40	10.00	10.01	0.15
80	10.00	9.90	0.14

* Calibration made "Not TISI Accredited" in this Certificate have been included for completeness.

Transducer Part : ENSL 16117

Condition : Installation by Transverse direction



Metrology and Calibration Department
Electrical Maintenance Division
Electricity Generating Authority of Thailand

Continued of Calibration Report

Certificate Number. 22V027

Page 5 of 5

DESCRIPTION	INSTRUMENT VALUE		UNCERTAINTY
	STANDARD SETTING	UUC READING	
Longitude			
Frequency (Hz)	mm/s _p	mm/s _p	± mm/s _p
*20	10.00	10.19	0.15
*30	10.00	10.06	0.15
40	10.00	10.04	0.15
80	10.00	9.99	0.14

* Calibration made "Not TISI Accredited" in this Certificate have been included for completeness.

Transducer Part : ENSL 16117

Condition : Installation by Longitude direction

* End Certificate of Calibration *

เอกสารแนบ 11
รายงานแผนและผลการดำเนินงาน
ด้านการฟื้นฟูพื้นที่ทำเหมือง

โครงการฟื้นฟู

บริษัท สุดมิน จำกัด ปบ.33154/16452

บริษัท ยูนิโฮม จำกัด ปบ.33121/16128



ตัดขั้นบันได



ปลูกต้นไม้



คุรระบายน้ำ



โครงการฟื้นฟูปลูกต้นไม้

บริษัท ยูนิโอม จำกัด ประทานบัตรที่ 33121/16128



โครงการฟื้นฟูปลูกต้นไม้

บริษัท ยูนิโสม จำกัด ประทานบัตรที่ 33121/16128

