



บริษัท ปตท. น้ำมันและ การค้าปลีก จำกัด (มหาชน)

รายงานผลการปฏิบัติตามมาตรการป้องกันและแก้ไขผลกระทบสิ่งแวดล้อม

และมาตรการติดตามตรวจสอบผลกระทบสิ่งแวดล้อม

โครงการปรับปรุงท่าเทียบเรือขนถ่ายน้ำมันและก๊าซปิโตรเลียมเหลว จังหวัดสุราษฎร์ธานี

ระหว่างเดือนมกราคม - มิถุนายน พ.ศ. 2566

ภาคผนวก จ

เอกสารสอบเทียบเครื่องมือ



right solutions.  
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ


Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Water Lab	Cadmium	ICP-MS	BKK_EL0026	14-Jun-22	14-Dec-23	18
Water Lab	Cadmium	Hot Block	BKK_EL0054	7-Apr-22	7-Oct-23	18
Water Lab	Cadmium	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Lead	ICP-MS	BKK_EL0026	14-Jun-22	14-Dec-23	18
Water Lab	Lead	Hot Block	BKK_EL0054	7-Apr-22	7-Oct-23	18
Water Lab	Lead	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	BOD	DO Meter	BKK_EN0017	24-May-22	24-Nov-23	18
Water Lab	BOD	Incubator	BKK_EN0305	5-Apr-23	5-Apr-24	18
Water Lab	BOD	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	COD	Hot Block	BKK_EN0222	1-Mar-23	1-Mar-24	12
Water Lab	COD	Spectrophotometer	BKK_EN0018	16-Sep-22	16-Sep-23	12
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0148	31-Jan-22	1-Aug-23	18
Water Lab	pH at 25 °C	pH meter	BKK_EN0072	12-Sep-22	12-Mar-24	18
Water Lab	Temperature	Digital Thermometer With Sensor	BKK_LG0048	12-Sep-22	12-Sep-23	12
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0007	1-Dec-21	1-Jun-23	18
Water Lab	Total Kjeldahl Nitrogen	Digestion Unit	BKK_EN0366	30-Jun-22	30-Jun-23	12
Water Lab	Total Kjeldahl Nitrogen	Discrete analyzer	BKK_EN0037	5-Jan-23	5-Jan-24	12
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Water Lab	Fecal Coliform	Autoclave	BKK_ML0037	21-Jan-22	22-Jul-23	18
Water Lab	Fecal Coliform	Incubator	BKK_ML0010	21-Jan-22	22-Jul-23	18
Water Lab	Fecal Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Fecal Coliform	Water Bath	BKK_ML0056	20-Apr-23	20-Apr-24	12
Water Lab	Total Solids	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Solids	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Water Lab	Total Coliform	Autoclave	BKK_ML0037	21-Jan-22	22-Jul-23	18
Water Lab	Total Coliform	Incubator	BKK_ML0011	21-Nov-22	21-May-24	18
Water Lab	Total Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Songkhla Lab	Fecal Coliform	Autoclave	SGK_ML0001	5-Jan-23	5-Jul-24	18
Songkhla Lab	Fecal Coliform	Incubator	SGK_ML0013	6-Aug-22	6-Feb-24	18
Songkhla Lab	Fecal Coliform	pH Meter	SGK_ML0016	5-Jan-23	5-Jul-24	18
Songkhla Lab	Fecal Coliform	Water Bath	SGK_ML0021	30-Jan-23	30-Jul-24	18
Songkhla Lab	Total Coliform	Autoclave	SGK_ML0001	5-Jan-23	5-Jul-24	18
Songkhla Lab	Total Coliform	Incubator	SGK_ML0013	6-Aug-22	6-Feb-24	18
Songkhla Lab	Total Coliform	pH Meter	SGK_ML0016	5-Jan-23	5-Jul-24	18
Songkhla Lab	Total Coliform	Water Bath	SGK_ML0021	30-Jan-23	30-Jul-24	18
Songkhla Lab	BOD	Incubator	SGK_CL0028	25-Jan-22	26-Jul-23	18
Songkhla Lab	BOD	DO/BOD Analyser	SGK_CL0073	21-Nov-22	21-May-24	18
Songkhla Lab	Conductivity	Conductivity Meter	SGK_FS0051	29-Aug-22	29-Aug-23	12
Songkhla Lab	Oil & Grease	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Oil & Grease	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Oil & Grease	Water Bath	SGK_CL0035	5-Feb-22	6-Aug-23	18
Songkhla Lab	pH at 25 °C	pH meter	SGK_CL0030	28-Apr-23	28-Oct-24	18
Songkhla Lab	Salinity	Conductivity meter	SGK_FS0051	29-Aug-22	29-Aug-23	12
Songkhla Lab	Temperature	pH meter	SRT_MKT0001	1-Feb-23	1-Feb-24	12
Songkhla Lab	Total Alkalinity	pH meter	SGK_CL0030	28-Apr-23	28-Oct-24	18
Songkhla Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Total Dissolved Solids 180°C	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Total Suspended Solids	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Total Suspended Solids	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Turbidity	Turbidity Meter	SGK_FS0045	20-Jun-22	20-Jun-23	12
Water Lab	Ammonia Nitrogen	Discrete analyzer	BKK_EN0037	5-Jan-23	5-Jan-24	12
Water Lab	Nitrate	Ion Chromatography	BKK_EN0069	12-Jan-23	12-Jan-24	12
Water Lab	Phosphate	Ion Chromatography	BKK_EN0069	12-Jan-23	12-Jan-24	12
Sludge	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Sludge	Total Petroleum Hydrocarbon	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Sludge	pH aqueous phase 50% (w/v)	pH meter	BKK_EN0072	12-Sep-22	12-Mar-24	18



right solutions.  
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Total Hydrocarbon	Total Hydrocarbon Analyzer	BKK_EN0057	9-Aug-22	9-Feb-24	18
Ambient	Total VOC	TVOC Analyzer	BKK_FS0819	4-Feb-22	5-Aug-23	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	SGK_FS0088	13-Jan-23	13-Jul-24	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0975	5-Jan-23	5-Jan-24	12
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	SGK_FS0035	13-Jul-22	11-Jan-24	18
Noise	Leq 24 hrs	Sound Calibrator	SGK_FS0114	14-Nov-22	14-Nov-23	13
Noise	Leq 24 hrs	Sound Level Meter	SGK_FS0030	25-Oct-22	25-Oct-23	12
Noise	Noise Annoyance	Sound Calibrator	SGK_FS0114	14-Nov-22	14-Nov-23	13
Noise	Noise Annoyance	Sound Level Meter	SGK_FS0030	25-Oct-22	25-Oct-23	12

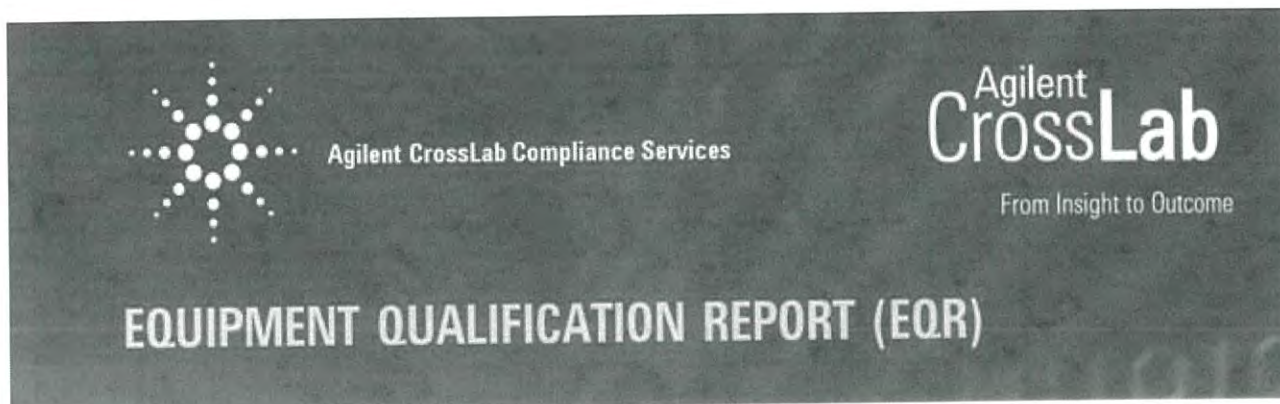**Agilent CrossLab Compliance**

Qualification Type: ICPMS-OQ

System ID: JP12091612

EQP Name: AgilentRecommended

EQP Revision: ICPMS.02.50

EQP Publish Date: March 2020

Date: June 14, 2022 10:32:16 AM

Report Type: Report

Org. Name: ALS Laboratory Group (Thailand) Co.,Ltd.

Org. Location: 104 Phatthanakarn 40, Suan Luang, Bangkok 10250  
Thailand.REVIEW BY Tattaporn C.APPROVED BY Santana N.NEXT CAL. DATE 14/12/23



## Table of Contents

Section	Page
Cover	1
Table of Contents	2
Test Summary	3
Service Details	4
Instrument Details	5
Calculation Formulas	6
Protocol Details	7
Tests	8
Autosampler Check : ASX-520	8
Integrated Sample Introduction System (ISIS) Check : ISIS2	9
Autotune : G3281A	10
Background (No Gas Mode) : G3281A	12
Background (Gas Modes) : G3281A	13
20-Minute Stability (No Gas Mode) : G3281A	14
Declaration of Change Control	15
Attachments	16
Electronic Signature	28
Transaction Logs	29

## Test Summary

### Purpose

This section includes a status for each scheduled test and the overall qualification. For each test that is run, (1) the status is automatically determined based on pre-defined limits, and (2) the total number of times the test was run is displayed. For detailed results and specifications for a test, refer to the test results in this EQR.

### Details

Test	Status	Runs
Autosampler Check : ASX-520	Pass	1
Integrated Sample Introduction System (ISIS) Check : ISIS2	Pass	1
Autotune : G3281A	Pass	1
Background (No Gas Mode) : G3281A	Pass	1
Background (Gas Modes) : G3281A	Pass	1
20-Minute Stability (No Gas Mode) : G3281A	Pass	1

### Overall Qualification Status

Pass

## Service Details

### Purpose

This section includes local contact and delivery details for this service.

### General Details

Service Order No./Request: 6005218484  
EQP Name: AgilentRecommended  
EQP Revision: ICPMS.02.50  
Report Type: Report

### Organization Details

Name: ALS Laboratory Group (Thailand) Co.,Ltd.  
Location: 104 Phatthanakarn 40, Suan Luang, Bangkok 10250 Thailand.

### Local Contact Details

Name: Khan Chatchanai  
Job Title: Lab Manager  
Qualification Location: Spectro Room

### Operator Details

Name: Panthep Kurasathain  
Job Title: Field Service Engineer

### Data Acquisition Details

Acquisition Software Name: MassHunter  
Acquisition Software Revision: D.01.01

Customer Data System (CDS): IcpMs: MassHunter

## Instrument Details

### Purpose

This section describes the as found system configuration.

### Details

#### ICP-MS 1

Manufacturer	Agilent Technologies
Name	7700x
Model Number	G3281A
Detector Type	SQ
Nebulizer	Mira Mist (G3161)
Spray Chamber	Quartz
Torch	Quartz
Sampling Cone	Ni
Skimmer Cone	Ni
Serial Number	JP12091612
Firmware Revision	D.01.01

#### ISIS 1

Manufacturer	Agilent Technologies
Name	ISIS2
Model Number	G4911A
Installed Options	#003: 2 pumps, 1 valve, auto dilution and discrete sampling
Type	Peristaltic pump system

#### Autosampler 1

Manufacturer	Agilent Technologies
Name	ASX-520
Model Number	G3286A
Serial Number	031403A520

#### Chiller 1

Manufacturer	Agilent Technologies
Name	Chiller
Model Number	G3292A
Serial Number	4N1220700

## Calculation Formulas

### Purpose

This section includes calculation formulas for all available tests. Depending upon which tests are scheduled, all or some apply to your qualification.

For a description of calculations for ICP-MS tests performed by the MassHunter software, refer to the MassHunter application and documentation.

## Protocol Details

### Purpose

This section lists the revisions for all test units used in this report. For complete test-specific and high-level change details, refer to the Revision History document.

Test Revision	Test
ICPMS.02.50	20-Minute Stability (No Gas Mode)
ICPMS.02.50	Autosampler Check
ICPMS.02.50	Autotune
ICPMS.02.50	Background (Gas Modes)
ICPMS.02.50	Background (No Gas Mode)
ICPMS.02.50	Integrated Sample Introduction System (ISIS) Check

# Autosampler Check

## Purpose

This test demonstrates that the autosampler module is correctly installed and connected. It does not test module performance.

---

## Setpoint

### Results

		Observed Result	Expected Result	Status
Criteria				
After the self test, is probe in the home position?		Yes	Yes	Pass
As commanded, is the probe positioned at vial 2?		Yes	Yes	Pass

Setpoint Status: Pass Runs: 1

### Overall Autosampler Check Test Status

Pass

---



# Integrated Sample Introduction System (ISIS) Check

Purpose

This test demonstrates that the ISIS module is correctly installed and connected. It does not test module performance.

Setpoint

Results

Criteria	Observed Result	Expected Result	Status
As commanded, does the pump rotate?	Yes	Yes	Pass
As commanded, do the valves load and inject?	Yes	Yes	Pass
Setpoint Status:	Pass		Runs: 1

Overall Integrated Sample Introduction System (ISIS) Check Test Status

Pass

## Autotune

### Purpose

This test uses traceable checkout standards to run a software-executed autotune in all modes. The tune report provides values for peak width, mass axis, sensitivity, oxide species, and doubly-charged species tests.

---

### Setpoint

### Results

Peakwidth Mass 7

Agilent Recommended:

Status:

	0.735	AMU
>=	0.65	
<=	0.80	
Pass		

Peakwidth Mass 89

Agilent Recommended:

Status:

	0.732	AMU
>=	0.65	
<=	0.80	
Pass		

Peakwidth Mass 205

Agilent Recommended:

Status:

	0.746	AMU
>=	0.65	
<=	0.80	
Pass		

Mass Axis 7

Agilent Recommended:

Status:

	7.00	AMU
>=	6.9	
<=	7.1	
Pass		

Mass Axis 89

Agilent Recommended:

Status:

	89.00	AMU
>=	88.9	
<=	89.1	
Pass		

Mass Axis 205

Agilent Recommended:

Status:

	205.00	AMU
>=	204.9	
<=	205.1	
Pass		

Mass 7 Sensitivity No Gas

81.18

Mcps/ppm

Agilent Recommended:

&gt;= 25.5

Status:

Pass

Mass 89 Sensitivity No Gas

247.81

Mcps/ppm

Agilent Recommended:

&gt;= 85

Status:

Pass

Mass 205 Sensitivity No Gas

184.87

Mcps/ppm

Agilent Recommended:

&gt;= 51

Status:

Pass

Mass 59 Sensitivity He

84.86

Mcps/ppm

Agilent Recommended:

&gt;= 20.4

Status:

Pass

Oxide Ratio 156/140

1.119

%

Agilent Recommended:

&lt;= 1.38

Status:

Pass

Doubly Charged Species Ratio 70/140

1.140

%

Agilent Recommended:

&lt;= 2.3

Status:

Pass

Setpoint Status:

Pass

Runs: 1

Overall Autotune Test Status

Pass

## Background (No Gas Mode)

### Purpose

This test examines the background of the ICP-MS in no gas mode by monitoring ions during a blank run.

### Setpoint

#### Conditions

Masses:

7	AMU
89	AMU
205	AMU

#### Measurements and Results

Masses (AMU):

Measured Value:

Agilent Recommended:

Status:

	7	89	205	
Measured Value:	4.900	7.100	18.400	cps
Agilent Recommended:	<= 10	<= 10	<= 30	
Status:	Pass	Pass	Pass	

Setpoint Status:

Pass

Runs: 1

#### Overall Background (No Gas Mode) Test Status

Pass

## Background (Gas Mode)

### Purpose

This test examines the background of the ICP-MS in the various gas modes by monitoring ions during a blank run.

Setpoint Gas Mode: Helium

### Conditions

Mass: 78 AMU  
Integration Time: 1.0 sec  
Cycles: 20

### Measurements and Results

Mass (AMU): 78  
Measured Value: 21.1000 cps  
Agilent Recommended: ≤ 460  
Status: Pass

Setpoint Status: Pass

Runs: 1

### Overall Background (Gas Mode) Test Status

Pass

## 20-Minute Stability (No Gas Mode)

### Purpose

This test monitors the abundance of ions present in the checkout standard over a 20-minute period to verify that the signal is stable. The %RSD of the abundance of given ions is calculated internally by the software and compared to the limit.

### Setpoint

#### Conditions

Mode:	Spectrum	
Masses:	7, 9, 59, 89, 140, 205	
Integration Time:	9.99	sec
Peak Pattern:	3	points/peak
Repetitions:	20	
Sweeps/Replicates:	100	

#### Measurements and Results

Masses (AMU):	7	89	205	
Stability RSD:	0.2	0.6	0.6	%
Agilent Recommended:	<= 3.45	<= 3.45	<= 3.45	
Status:	Pass	Pass	Pass	

Setpoint Status: Pass Runs: 1

#### Overall 20-Minute Stability (No Gas Mode) Test Status

Pass

## Declaration of Change Control

This document is under change control. Revision history is maintained and printed on each document. Access to the master documents is limited to process owners. Documents receive periodic review and cannot be assigned an evergreen status. The qualification performed according to this document refers only to the hardware/software configuration in place at the time of the qualification. Agilent Technologies recommends that instrument configuration change management procedures be in place in order to maintain the validation process. Any changes to the analytical or computer hardware or software must be clearly specified. A change management system provides a means for determining the degree of requalification required according to the extent of the changes made. All details of the changes must be thoroughly recorded and documented, together with details of completed tests and their results. Note: Hardware/software configuration management is the customer's responsibility.



## Attachments

Training requirements note: The delivery engineer attaches an ACE technique-specific training certificate to the Equipment Qualification Report (EQR). Obtaining ACE technique-specific certification includes pre-requisite trainings for Data Integrity, General Compliance topics (GMP, GLP, ALCOA, etc.), instrument hardware and software components, and the ACE technique itself. The one certificate encompasses all pre-requisite trainings as documented in the Agilent Learning Management System called Success Factors.

Location	Category	Document Name	Page
EQR	General	Certificate of System Qualification	17
EQR	General	Operator's training certificate and qualifications	18
EQR	General	Certificate of Qualification for ACE	19
EQR	General	Certificate of Qualification for ACE	20
EQR	General	Tune reports	21
EQR	General	Test Report	24
EQR	General	Test Report	26

## General

Document Name: Certificate of System Qualification



## Agilent Compliance Engine Self Qualification

Date: September 14, 2021 4:59:15 PM

Drive Serial #: ACA025C9

Platform Revision:

ACE 3.11

Individual self-qualification reports for each specific technique installed are also available upon request. They provide additional details on the general report from the concise summary and are structured by the actual algorithms challenged during the process. There is not a one-to-one relationship between algorithms and OQ program tests because some algorithms are used by several tests and across multiple similar hardware components of the qualified systems.

Technique Type	Tests Completed	Result
Atomic Absorption	7	Conforms
Capillary Electrophoresis	10	Conforms
Dissolution	6	Conforms
Emission Spectroscopy	3	Conforms
Gas Chromatography - GCMS	17	Conforms
Gas Chromatography	29	Conforms
Gel Permeation Chromatography	9	Conforms
ICP-MS	6	Conforms
Infrared Spectroscopy	7	Conforms
Liquid Chromatography	17	Conforms
Liquid Chromatography - LCMS	8	Conforms
Microfluidics	18	Conforms
Sample Preparation - Gas Chromatography	9	Conforms
Sample Preparation - Liquid Chromatography	8	Conforms
Supercritical Fluid Chromatography	15	Conforms
Software	6	Conforms
UV-Vis Spectrophotometer	13	Conforms

## Overall Qualification Status

Conforms

## General

Document Name: Operator's training certificate and qualifications



## Certificate of Completion

Learner Name: Panthep Kurasathain

Title Of Course: AN-CE-ICPMS-2-017-B:7700x/7700s ICP-MS Intro. -Oper.H/W.S/W & OQ/PV

Completion Date: November 22, 2012

Certified By Company: Learning at Agilent

All Service and Support training certificates have the following specific limitations.

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's: Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.

Date: June 14, 2022 10:32:16 AM  
System ID: JP12091612

General

Document Name:

Certificate of Qualification for ACE



## Certificate of Completion

Learner Name: Panthep Kurasathain

Title Of Course: AN-CE-SS-II-030-A: ACE 3.X User Update Training

Completion Date: July 7, 2020

Certified By Company: Learning at Agilent

**All Service and Support training certificates have the following specific limitations.**

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's: Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.

General

Document Name: Certificate of Qualification for ACE



## Certificate of Completion

Learner Name: Panthep Kurasathain

Title Of Course: AN-CE-ICPMS-2-035-B: CrossLab Compliance Hardware Specific Delivery for Agilent ICP-MS Systems

Completion Date: October 31, 2020

Certified By Company: Learning at Agilent

All Service and Support training certificates have the following specific limitations.

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's: Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.

## General


Document Name: Tune reports

## Tune Report

Operator Name Supakwan Mak  
 Acq/Data Batch C:\Agilent\ICPMH11\UserTune.b  
 Acq. Date-Time 6/14/2022 9:03:15 AM  
 Report Comment PMOQ 14 June 2022  
 Instrument Name G3281A JP12091612

## [No Gas]

## Sensitivity

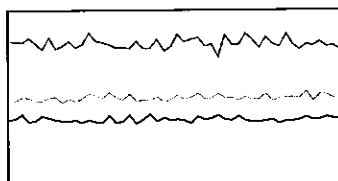


Mass	Range	Count	RSD%	Background
7	10000	8118	3.585	4.900
89	50000	24781	3.128	7.100
205	50000	18487	3.808	18.400

Sampling Period [sec] 0.311  
 Integration Time [sec] 0.1

## Oxide/Doubly Charged Ratio

Oxide 156 / 140 1.119 %  
 Doubly Charged 70 / 140 1.140 %

## Resolution/Axis

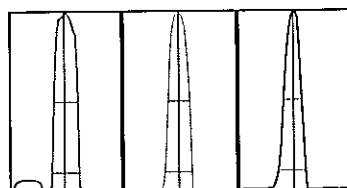

Mass	Peak Height	Axis	W-50%	W-10%
7	8050.47	7.00	0.65	0.735
89	24725.81	89.00	0.57	0.732
205	18559.81	205.00	0.49	0.746

Integration Time [sec] 0.1  
 Acquisition Time [sec] 22.74  
 Y Axis Linear

## Tune Parameters

## Plasma Parameters

Plasma Mode	---	Nebulizer Gas	1.05 L/min	Makeup Gas	0.00 L/min
RF Power	1550 W	Option Gas	---	Auxiliary Gas	0.90 L/min
RF Matching	1.80 V	Nebulizer Pump	0.10 rps	Plasma Gas	15.0 L/min
Sample Depth	8.0 mm	S/C Temp	2 °C		

## Lens Parameters

Extract 1	0.0 V	Omega Lens	8.6 V	Deflect	12.0 V
Extract 2	-190.0 V	Cell Entrance	-30 V	Plate Bias	-40 V
Omega Bias	-90 V	Cell Exit	-50 V		

## Cell Parameters

Use Gas	No	3rd Gas Flow	---	Energy Discrimination	5.0 V
He Flow	0.0 mL/min	OctP Bias	-8.0 V		

Document Name: Tune reports

## Tune Report

H2 Flow — OctP RF 200 V

**QP Parameters**

Mass Gain	152	Axis Gain	1.0032	QP Bias	-3.0 V
Mass Offset	123	Axis Offset	0.12		

**Hardware Settings**

**Torch**


Torch H	-0.4 mm	Torch V	0.0 mm
---------	---------	---------	--------

**EM**

Discriminator	4.5 mV	Analog HV	1708 V	Pulse HV	1356 V
---------------	--------	-----------	--------	----------	--------

[He]

## Sensitivity

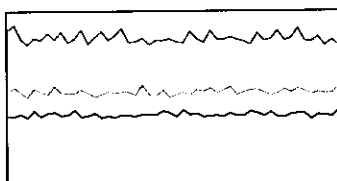

Mass	Range	Count	RSD%	Background
59	10000	8486	3.392	15,700
89	20000	10724	3.135	13,900
205	50000	20200	3.166	22,100

Sampling Period [sec] 0.31  
Integration Time [sec] 0.1

## Oxide/Doubly Charged Ratio

Oxide 156 / 140 1.122 %  
Doubly Charged 70 / 140 1.288 %

## Tune Parameters

## Plasma Parameters

Plasma Mode	—	Nebulizer Gas	1.05 L/min	Makeup Gas	0.00 L/min
RF Power	1550 W	Option Gas	—	Auxiliary Gas	0.90 L/min
RF Matching	1.80 V	Nebulizer Pump	0.10 rps	Plasma Gas	15.0 L/min
Sample Depth	8.0 mm	S/C Temp	2 °C		

## Lens Parameters

Extract 1	0.0 V	Omega Lens	7.4 V	Deflect	3.6 V
Extract 2	-200.0 V	Cell Entrance	-90 V	Plate Bias	-115 V
Omega Bias	-90 V	Cell Exit	-70 V		

## Cell Parameters

Use Gas	Yes	3rd Gas Flow	—	Energy Discrimination	3.0 V
He Flow	4.5 mL/min	OctP Bias	-21.0 V		
H2 Flow	—	OctP RF	190 V		

## QP Parameters

Mass Gain	152	Axis Gain	1.0032	QP Bias	-18.0 V
Mass Offset	123	Axis Offset	0.12		

## Hardware Settings

**Torch**

Torch H	-0.4 mm	Torch V	0.0 mm
---------	---------	---------	--------

2 of 3

6/14/2022 9:03 AM

Date: June 14, 2022 10:32:16 AM  
System ID: JP12091612



Document Name: Tune reports

## Tune Report

### EM

Discriminator

4.5 mV

Analog HV

1708 V

Pulse HV

1356 V

3 of 3

6/14/2022 9:03 AM

Date: June 14, 2022 10:32:16 AM  
System ID: JP12091612

## General

Document Name: Test Report

## Batch Summary Report

Batch Folder: D:\Agilent Service\PMOQ 13-6-22\BG He.b\

Analysis File: BG He.batch.bin

Tune Step: #1 He

	Rjct	Acq. Date-Time	Data File	Sample Name	Type	Level	Dilution
1		6/14/2022 10:03:39 AM	001SMPL.d	BG He	Sample		1.0000

Document Name: Test Report

## Batch Summary Report

Analyte Table

		78 (He1)	
Sample Name		CPS	CPS RSD
1	BG He	21.1000	38.0

Page 2 / 2

6/14/2022 10:09:04 AM

Date: June 14, 2022 10:32:16 AM  
System ID: JP12091612

## General

Document Name: Test Report

## Batch Summary Report

Batch Folder: D:\Agilent Service\PMOQ 13-6-22\ OQ 20 Min.b\  
Analysis File: OQ 20 Min.batch.bin  
Tune Step: #1 No Gas

	Ret	Acq. Date-Time	Data File	Sample Name	Type	Level	Dilution
1		6/14/2022 9:29:27 AM	001SMPL.d	20 min	Sample		1.0000

Document Name:

Test Report

## Batch Summary Report

Analyte Table

		7 [No Gas]		9 [No Gas]		59 [No Gas]		89 [No Gas]	
	Sample Name	CPS	CPS RSD	CPS	CPS RSD	CPS	CPS RSD	CPS	CPS RSD
1	20 min	82477.8975	0.2	285.3875	5.8	162011.0035	0.7	241211.0790	0.6

		140 [No Gas]		205 [No Gas]	
	Sample Name	CPS	CPS RSD	CPS	CPS RSD
1	20 min	252452.6980	0.7	181154.8205	0.6

## Electronic Signature

### Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

### Details

Full Name of Signer:	Panthep Kurasathain
Logged On User Name:	panthep_kurasathain@agilent.com
Signature Creation Date:	June 14, 2022
Reason for Signature:	Executed protocol and published this original version of document

### Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

### Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: panthep\_kurasathain  
 Hostname: ASBKKWX313

System Id: JP12091612  
 Print Date: June 14, 2022 10:32:20 AM

ALS OQHW 7700 14Jun2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 14, 2022 10:14:43 AM	Audit	SessionCreated	Session	None
June 14, 2022 10:14:43 AM	Start	Configuration	Session	None
June 14, 2022 10:14:43 AM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
June 14, 2022 10:19:18 AM	Audit	EqpLoaded	Session	EQP details for primary technique [lcpMs] - File path: [Protocol]Packs/lcpMs/Configurations/02.50/lcpMs.02.50.eqp], EQP File Name: [lcpMs.02.50.eqp], EQP Name: [AgilentRecommended]
June 14, 2022 10:19:20 AM	End	Configuration	Session	None
June 14, 2022 10:19:24 AM	Start	Qualification	Session	OQ
June 14, 2022 10:19:24 AM	Start	Execution	Autosampler Check : ASX-520: Autosampler Check	None
June 14, 2022 10:19:42 AM	End	Execution	Autosampler Check : ASX-520: Autosampler Check	Run Count : 1
June 14, 2022 10:19:43 AM	Start	Execution	Integrated Sample Introduction System (ISIS) Check : ISIS2: Integrated Sample Introduction System (ISIS) Check	None
June 14, 2022 10:19:47 AM	End	Execution	Integrated Sample Introduction System (ISIS) Check : ISIS2: Integrated Sample Introduction System (ISIS) Check	Run Count : 1
June 14, 2022 10:19:50 AM	Start	Execution	Autotune : G3281A: Autotune 1	None
June 14, 2022 10:22:22 AM	End	Execution	Autotune : G3281A: Autotune 1	Run Count : 1



User Name: panthep\_kurasathain  
 Hostname: ASBKKWX313

System Id: JP12091612  
 Print Date: June 14, 2022 10:32:20 AM

## ALS OQHW 7700 14Jun2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 14, 2022 10:22:24 AM	Start	Execution	Background (No Gas Mode) : G3281A: No Gas Mode Background 1	None
June 14, 2022 10:22:48 AM	End	Execution	Background (No Gas Mode) : G3281A: No Gas Mode Background 1	Run Count : 1
June 14, 2022 10:22:49 AM	Start	Execution	Background (Gas Modes) : G3281A: Gas Mode Background :Helium	None
June 14, 2022 10:23:35 AM	End	Execution	Background (Gas Modes) : G3281A: Gas Mode Background :Helium	Run Count : 1
June 14, 2022 10:23:37 AM	Start	Execution	20-Minute Stability (No Gas Mode) : G3281A: 20-Minute Stability (No Gas Mode) 1	None
June 14, 2022 10:24:06 AM	End	Execution	20-Minute Stability (No Gas Mode) : G3281A: 20-Minute Stability (No Gas Mode) 1	Run Count : 1
June 14, 2022 10:24:08 AM	End	Qualification	Session	OQ
June 14, 2022 10:24:08 AM	Start	Reporting	Session	None
June 14, 2022 10:30:26 AM	Audit	Reporting	Session	Report Generated : Certificate
June 14, 2022 10:30:39 AM	Audit	Reporting	Session	Report Generated : Report

# Certificate of System Qualification

ICPMS-OQ

System ID: JP12091612  
Organization Name: ALS Laboratory Group (Thailand) Co.,Ltd.  
Organization Location: 104 Phatthanakarn 40, Suan Luang, Bangkok 10250 Thailand.

Date: June 14, 2022 10:32:51 AM  
EQP Name: AgilentRecommended  
EQP Revision: ICPMS.02.50  
Overall Qualification Status: Pass

## Autosampler Check

### Overall Autosampler Check Test Status

Pass

## Integrated Sample Introduction System (ISIS) Check

### Overall Integrated Sample Introduction System (ISIS) Check Test Status

Pass

## Autotune

Peakwidth Mass 7	Pass
Peakwidth Mass 89	Pass
Peakwidth Mass 205	Pass
Mass Axis 7	Pass
Mass Axis 89	Pass
Mass Axis 205	Pass
Mass 7 Sensitivity No Gas	Pass
Mass 89 Sensitivity No Gas	Pass
Mass 205 Sensitivity No Gas	Pass
Mass 59 Sensitivity He	Pass
Oxide Ratio 156/140	Pass
Doubly Charged Species Ratio 70/140	Pass

### Overall Autotune Test Status

Pass

Date: June 14, 2022 10:32:51 AM  
System ID: JP12091612

## Background (No Gas Mode)

Setpoint Status: Pass

Masses (AMU):	7	89	205	
Measured Value:	4.900	7.100	18.400	cps
Agilent Recommended:	<= 10	<= 10	<= 30	
Status:	Pass	Pass	Pass	

## Overall Background (No Gas Mode) Test Status

Pass

## Background (Gas Mode)

Gas Mode: Helium

Setpoint Status: Pass

Mass (AMU):	78	
Measured Value:	21.1000	cps
Agilent Recommended:	<= 460	
Status:	Pass	

## Overall Background (Gas Mode) Test Status

Pass

## 20-Minute Stability (No Gas Mode)

Masses (AMU):	7	89	205	
Stability RSD:	0.2	0.6	0.6	%
Agilent Recommended:	<= 3.45	<= 3.45	<= 3.45	
Status:	Pass	Pass	Pass	

## Overall 20-Minute Stability (No Gas Mode) Test Status

Pass

## Instrument Details

### Purpose

This section describes the as found system configuration.

### Details

#### ICP-MS 1

Manufacturer	Agilent Technologies
Name	7700x
Model Number	G3281A
Detector Type	SQ
Nebulizer	Mira Mist (G3161)
Spray Chamber	Quartz
Torch	Quartz
Sampling Cone	Ni
Skimmer Cone	Ni
Serial Number	JP12091612
Firmware Revision	D.01.01

#### ISIS 1

Manufacturer	Agilent Technologies
Name	ISIS2
Model Number	G4911A
Installed Options	#003: 2 pumps, 1 valve, auto dilution and discrete sampling
Type	Peristaltic pump system

#### Autosampler 1

Manufacturer	Agilent Technologies
Name	ASX-520
Model Number	G3286A
Serial Number	031403A520

#### Chiller 1

Manufacturer	Agilent Technologies
Name	Chiller
Model Number	G3292A
Serial Number	4N1220700

## Electronic Signature

### Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

### Details

Full Name of Signer:	Panthep Kurasathain
Logged On User Name:	panthep_kurasathain@agilent.com
Signature Creation Date:	June 14, 2022
Reason for Signature:	Executed protocol and published this original version of document

### Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

### Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: panthep\_kurasathain  
 Hostname: ASBKKWX313

System Id: JP12091612  
 Print Date: June 14, 2022 10:32:52 AM

ALS OQHW 7700 14Jun2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 14, 2022 10:14:43 AM	Audit	SessionCreated	Session	None
June 14, 2022 10:14:43 AM	Start	Configuration	Session	None
June 14, 2022 10:14:43 AM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
June 14, 2022 10:19:18 AM	Audit	EqpLoaded	Session	EQP details for primary technique [lcpMs] - File path: [ProtocolPacks/lcpMs/Configurations/02.50/lcpMs.02.50.eqp], EQP File Name: [lcpMs.02.50.eqp], EQP Name: [AgilentRecommended]
June 14, 2022 10:19:20 AM	End	Configuration	Session	None
June 14, 2022 10:19:24 AM	Start	Qualification	Session	OO
June 14, 2022 10:19:24 AM	Start	Execution	Autosampler Check : ASX-520: Autosampler Check	None
June 14, 2022 10:19:42 AM	End	Execution	Autosampler Check : ASX-520: Autosampler Check	Run Count : 1
June 14, 2022 10:19:43 AM	Start	Execution	Integrated Sample Introduction System (ISIS) Check : ISIS2: Integrated Sample Introduction System (ISIS) Check	None
June 14, 2022 10:19:47 AM	End	Execution	Integrated Sample Introduction System (ISIS) Check : ISIS2: Integrated Sample Introduction System (ISIS) Check	Run Count : 1
June 14, 2022 10:19:50 AM	Start	Execution	Autotune : G3281A: Autotune 1	None
June 14, 2022 10:22:22 AM	End	Execution	Autotune : G3281A: Autotune 1	Run Count : 1

Page 1 / 3

User Name: panthep\_kurasathaln  
 Hostname: ASBKKWX313

System Id: JP12091612  
 Print Date: June 14, 2022 10:32:52 AM

ALS OQHW 7700 14Jun2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 14, 2022 10:22:24 AM	Start	Execution	Background (No Gas Mode) : G3281A: No Gas Mode Background 1	None
June 14, 2022 10:22:48 AM	End	Execution	Background (No Gas Mode) : G3281A: No Gas Mode Background 1	Run Count : 1
June 14, 2022 10:22:49 AM	Start	Execution	Background (Gas Modes) : G3281A: Gas Mode Background :Helium	None
June 14, 2022 10:23:35 AM	End	Execution	Background (Gas Modes) : G3281A: Gas Mode Background :Helium	Run Count : 1
June 14, 2022 10:23:37 AM	Start	Execution	20-Minute Stability (No Gas Mode) : G3281A: 20-Minute Stability (No Gas Mode) 1	None
June 14, 2022 10:24:06 AM	End	Execution	20-Minute Stability (No Gas Mode) : G3281A: 20-Minute Stability (No Gas Mode) 1	Run Count : 1
June 14, 2022 10:24:08 AM	End	Qualification	Session	OQ
June 14, 2022 10:24:08 AM	Start	Reporting	Session	None
June 14, 2022 10:30:26 AM	Audit	Reporting	Session	Report Generated : Certificate
June 14, 2022 10:30:39 AM	Audit	Reporting	Session	Report Generated : Report

User Name: panthep\_kurasathain  
Hostname: ASBKKWX313

System Id: JP12091612  
Print Date: June 14, 2022 10:32:52 AM

**ALS OQHW 7700 14Jun2022 Transaction log :**

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 14, 2022 10:32:26 AM	Audit	Reporting	Session	Report Signed : Report PDF Name: ALS OQHW 7700 14Jun2022_20220614_OQ Report_1.pdf User Name: panthep_kurasathain@agilen t.com Full Name of Signer: Panthep Kuresathain Reason for signature: Executed protocol and published this original version of document



Certificate No. T220730

Page 1 of 6

## Certificate of Calibration

Equipment : HEATING BLOCK

Manufacturer : Environmental Express

Model : SC 196

Serial No. : 6974CECW3285

Customer Code : BKK\_EL0054


ID No. : T5306A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,  
Khet Suan Luang, Bangkok 10250

Customer Location : Acid Digestion Lab

Date of Receipt : 30 March 2022

Calibrated By : Watcharapon Sangtong (Technician )

Approved By :  / Sujjar Naknakred ( Site Calibration Manager )

Date of Issue : 12 APR 2022

REVIEW BY	Tattaporn C.
APPROVED BY	Sangtong N.
NEXT CAL. DATE	7/10/23

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T220730

Page 2 of 6

## Calibration Report

**Equipment** : HEATING BLOCK  
**Date of Calibration** : 7 April 2022  
**Environment** : Temperature : 21.8-23.1 °C  
Line Voltage : 221.6-226.3 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN221-TN230	T210008	08 June 2022
TC	TYPE T	TN231-TN240	T210008	08 June 2022
DATA LOGGER	34970A	T149	T210008	08 June 2022

3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 2 Hour 25 Minute At 95 °C  
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

5. Adjustment :

( ) without adjustment

( X ) after adjustment

Approved By. 





# Metrological Center

## SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109


Website : [www.scieco.co.th](http://www.scieco.co.th)

E-Mail : [calibrate@scg.co.th](mailto:calibrate@scg.co.th)

Certificate No. T220730

Page 3 of 6

## Calibration Report

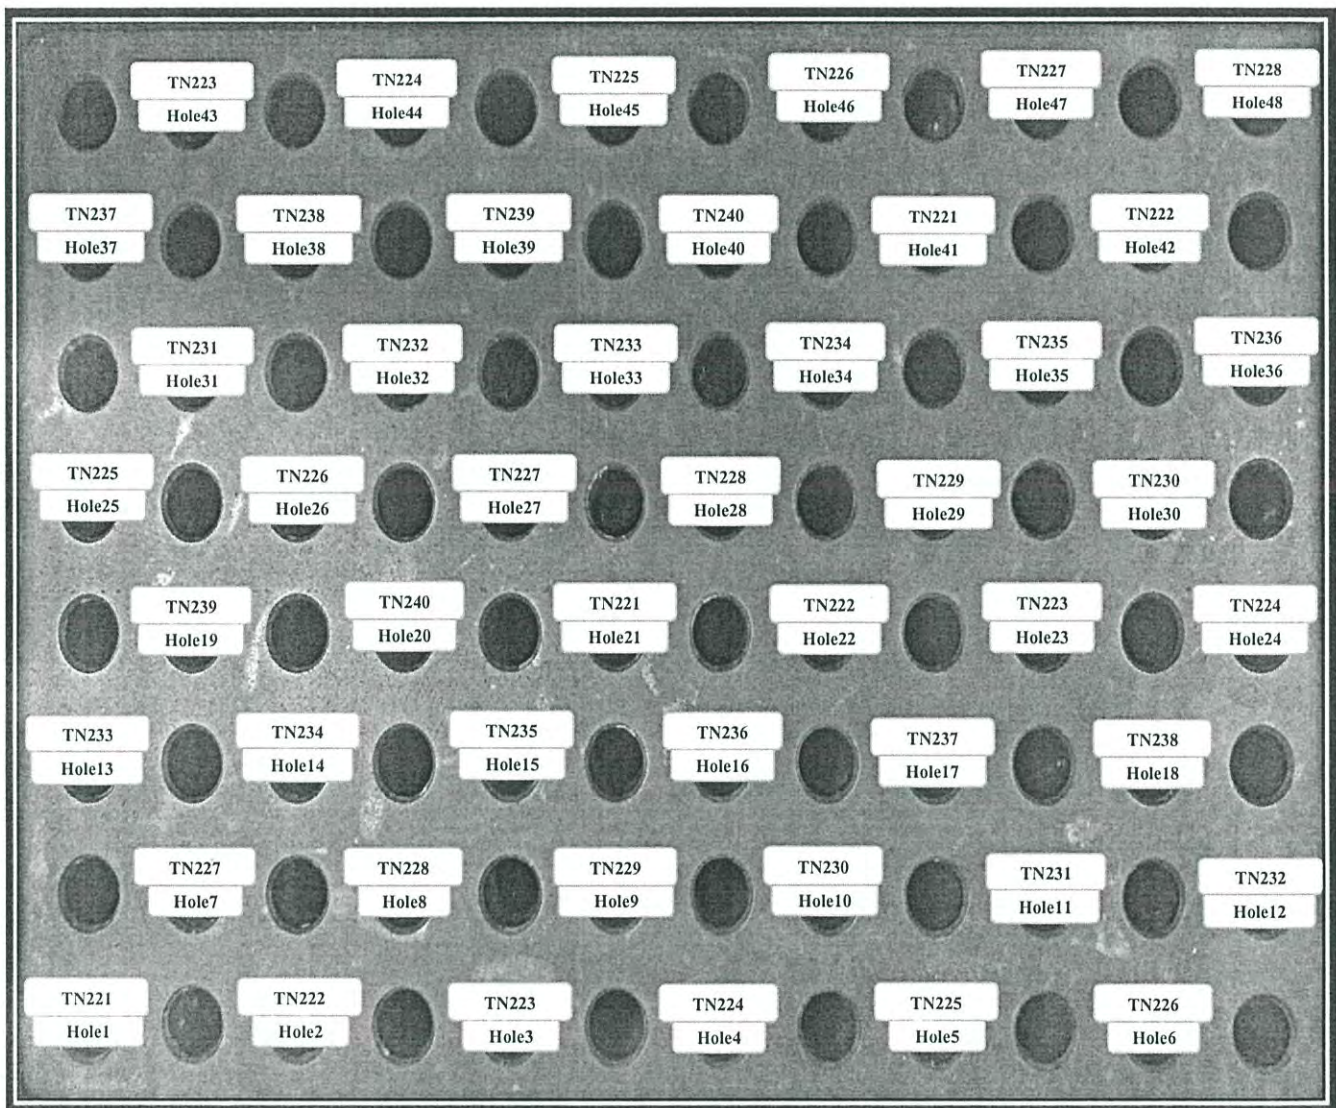

FRONT CONTROL

Approved By. \_\_\_\_\_



## Calibration Report

### Measurement Results

Calibration Point		Average Standard Reading at each position ( ° C )					
<b>R1 Hole1-Hole6</b>		<b>TN221</b>	<b>TN222</b>	<b>TN223</b>	<b>TN224</b>	<b>TN225</b>	<b>TN226</b>
CAL POINT	Max	93.60	93.82	94.05	94.20	94.36	94.26
95	Min	93.07	93.26	93.51	93.66	93.82	93.71
	Average	93.33	93.54	93.78	93.93	94.09	93.98
<b>R2 Hole7-Hole12</b>		<b>TN227</b>	<b>TN228</b>	<b>TN229</b>	<b>TN230</b>	<b>TN231</b>	<b>TN232</b>
	Max	94.59	94.79	94.63	94.55	94.82	95.00
	Min	94.05	94.25	94.08	93.97	94.26	94.44
	Average	94.32	94.52	94.36	94.26	94.54	94.72
<b>R3 Hole13-Hole18</b>		<b>TN233</b>	<b>TN234</b>	<b>TN235</b>	<b>TN236</b>	<b>TN237</b>	<b>TN238</b>
	Max	95.03	94.54	94.78	94.84	95.06	94.73
	Min	94.46	93.98	94.20	94.28	94.49	94.18
	Average	94.74	94.26	94.49	94.56	94.78	94.45
<b>R4 Hole19-Hole24</b>		<b>TN239</b>	<b>TN240</b>	<b>TN221</b>	<b>TN222</b>	<b>TN223</b>	<b>TN224</b>
	Max	94.89	94.82	95.73	95.85	95.73	96.10
	Min	94.33	94.26	95.51	95.62	95.51	95.85
	Average	94.61	94.54	95.62	95.73	95.62	95.97
<b>R5 Hole25-Hole30</b>		<b>TN225</b>	<b>TN226</b>	<b>TN227</b>	<b>TN228</b>	<b>TN229</b>	<b>TN230</b>
	Max	96.28	96.39	96.37	96.54	96.19	96.04
	Min	96.01	96.10	96.02	96.20	95.89	95.71
	Average	96.15	96.24	96.20	96.37	96.04	95.88
<b>R6 Hole31-Hole36</b>		<b>TN231</b>	<b>TN232</b>	<b>TN233</b>	<b>TN234</b>	<b>TN235</b>	<b>TN236</b>
	Max	96.84	96.97	97.03	96.48	96.33	95.76
	Min	96.53	96.65	96.71	96.08	95.98	95.43
	Average	96.68	96.81	96.87	96.28	96.16	95.60
<b>R7 Hole37-Hole42</b>		<b>TN237</b>	<b>TN238</b>	<b>TN239</b>	<b>TN240</b>	<b>TN221</b>	<b>TN222</b>
	Max	96.46	96.15	96.19	96.06	96.95	97.09
	Min	96.13	95.84	95.85	95.72	96.64	96.78
	Average	96.30	95.99	96.02	95.89	96.80	96.93
<b>R8 Hole43-Hole48</b>		<b>TN223</b>	<b>TN224</b>	<b>TN225</b>	<b>TN226</b>	<b>TN227</b>	<b>TN228</b>
	Max	96.91	96.58	96.13	96.19	96.34	96.19
	Min	96.55	96.21	95.80	95.87	96.03	95.88
	Average	96.73	96.40	95.96	96.03	96.18	96.03

Approved By. \_\_\_\_\_





Certificate No. T220730

Page 5 of 6

## Calibration Report

### Measurement Results

Calibration Point		Average Standard Reading at each position ( ° C )					
<b>R1 Hole1-Hole6</b>		<b>TN221</b>	<b>TN222</b>	<b>TN223</b>	<b>TN224</b>	<b>TN225</b>	<b>TN226</b>
CAL POINT	Max	104.47	104.65	104.79	105.31	105.47	105.46
105	Min	104.15	104.27	104.45	104.98	105.14	105.20
	Average	104.31	104.46	104.62	105.15	105.31	105.33
<b>R2 Hole7-Hole12</b>		<b>TN227</b>	<b>TN228</b>	<b>TN229</b>	<b>TN230</b>	<b>TN231</b>	<b>TN232</b>
	Max	105.55	105.73	105.65	105.84	105.97	106.07
	Min	105.28	105.43	105.35	105.52	105.68	105.83
	Average	105.42	105.58	105.50	105.68	105.82	105.95
<b>R3 Hole13-Hole18</b>		<b>TN233</b>	<b>TN234</b>	<b>TN235</b>	<b>TN236</b>	<b>TN237</b>	<b>TN238</b>
	Max	106.14	106.06	105.81	106.05	105.81	105.87
	Min	105.85	105.81	105.55	105.80	105.53	105.64
	Average	106.00	105.94	105.68	105.92	105.67	105.75
<b>R4 Hole19-Hole24</b>		<b>TN239</b>	<b>TN240</b>	<b>TN221</b>	<b>TN222</b>	<b>TN223</b>	<b>TN224</b>
	Max	105.86	105.60	104.44	104.51	104.28	104.78
	Min	105.61	105.37	104.27	104.35	104.12	104.61
	Average	105.74	105.48	104.35	104.43	104.20	104.69
<b>R5 Hole25-Hole30</b>		<b>TN225</b>	<b>TN226</b>	<b>TN227</b>	<b>TN228</b>	<b>TN229</b>	<b>TN230</b>
	Max	104.94	104.93	104.97	105.08	104.68	104.69
	Min	104.77	104.75	104.76	104.90	104.51	104.49
	Average	104.85	104.84	104.86	104.99	104.60	104.59
<b>R6 Hole31-Hole36</b>		<b>TN231</b>	<b>TN232</b>	<b>TN233</b>	<b>TN234</b>	<b>TN235</b>	<b>TN236</b>
	Max	105.44	105.45	105.61	104.95	104.84	104.42
	Min	105.27	105.27	105.44	104.76	104.66	104.25
	Average	105.36	105.36	105.53	104.86	104.75	104.33
<b>R7 Hole37-Hole42</b>		<b>TN237</b>	<b>TN238</b>	<b>TN239</b>	<b>TN240</b>	<b>TN221</b>	<b>TN222</b>
	Max	105.17	104.70	104.59	104.51	105.22	105.53
	Min	105.00	104.53	104.41	104.35	105.04	105.37
	Average	105.08	104.62	104.50	104.43	105.13	105.45
<b>R8 Hole43-Hole48</b>		<b>TN223</b>	<b>TN224</b>	<b>TN225</b>	<b>TN226</b>	<b>TN227</b>	<b>TN228</b>
	Max	105.61	105.45	105.10	104.77	104.87	105.02
	Min	105.44	105.28	104.92	104.60	104.70	104.85
	Average	105.53	105.37	105.01	104.69	104.79	104.93

Approved By. \_\_\_\_\_



Certificate No. T220730

Page 5 of 6

## Calibration Report

### Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability ( $\pm$ °C)	Uncertainty ( $\pm$ °C)
	Min , Max	Average		
100.0	100.0 , 100.4	100.1	0.29	0.83
105.0	105.0 , 105.4	105.1	0.20	0.79

\* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$  which for a t-distribution, providing a level of confidence of approximately 95 % .

 Approved By. 



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th



Certificate No. T221644

Page 1 of 4

## Certificate of Calibration

Equipment : Chamber ( Cold Room )

Manufacturer : KOLDTECH

Model : KM 320

Serial No. : TBN-1012061/05

Customer Code : BKK\_EN0167

ID No. : T2463A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250



Customer Location : Environmental Laboratory

Date of Receipt : 27 June 2022

Calibrated By : Sujjar Naknakred ( Site Calibration Manager )

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 04 JUL 2022

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	30/12/23

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T221644

Page 2 of 4

## Calibration Report

**Equipment** : Chamber ( Cold Room )  
**Date of Calibration** : 30 June - 1 July 2022  
**Environment** : Temperature : 18.9-23.7 °C  
Line Voltage : 222.9-226.5 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 ( based on ASTM E145-94 ( Reapproved 2001) and AS2853-1986 ).  
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T210009	30 July 2022
TC	TYPE T	TN171-TN180	T210009	30 July 2022
DATA LOGGER	34970A	T149	T210009	30 July 2022

3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 3 Hour - Minute At 3 °C  
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

5. Adjustment :

( ) without adjustment

( X ) after adjustment


Approved By. 



Certificate No. T221644

Page 3 of 4

## Calibration Report

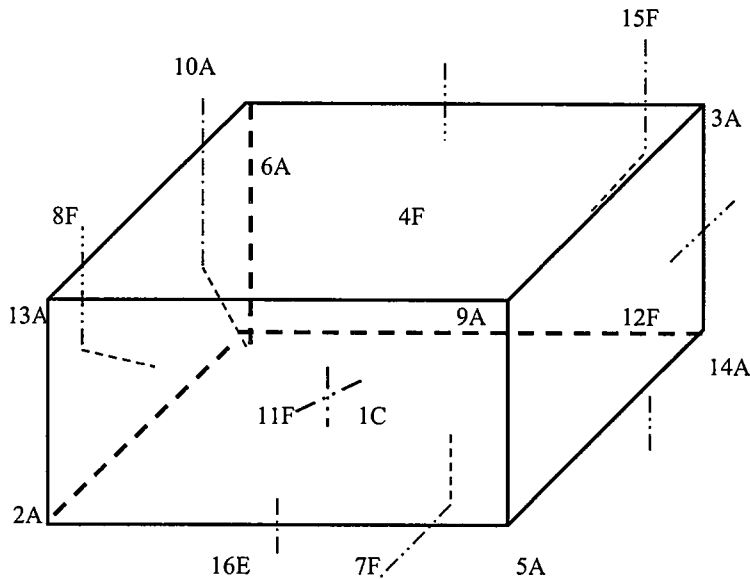

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN161
2A	=	TN162
3A	=	TN163
4F	=	TN164
5A	=	TN165
6A	=	TN166
7F	=	TN167
8F	=	TN168
9A	=	TN169
10A	=	TN170

11F	=	TN171
12F	=	TN172
13A	=	TN173
14A	=	TN174
15F	=	TN175
16E	=	TN176

Approved By. 

Certificate No. T221644

Page 4 of 4

## Calibration Report

**Measurement Results:**

Average Standard Reading at each position (°C)										
Calibration Point	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170
3	2.71	2.82	2.75	2.89	2.95	3.68	3.02	2.96	3.03	2.85
	TN171	TN172	TN173	TN174	TN175	TN176				
	2.97	3.02	2.89	3.04	2.97	3.33				

Chamber ( Cold Room )			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage
	Min , Max	Average					Factor <i>k</i>
3.0	2.9 , 4.0	3.2	2.99	1.05	1.30	1.66	2.00

\* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES**

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

**Cert.No.:** 22TW122

**Page.:** 1 of 2

## Certificate of Testing

**Equipment :** DO Meter  
**Manufacturer :** YSI  
**Model :** 5000-230V  
**Serial No. :** 09J101147  
**ID No. :** BKK\_EN0017  
**Received Date :** 20 May 2022  
**Test Date :** 24 May 2022  
**Reference :** 2205-0638DSC-8

**Submitted by :** ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

**Laboratory Condition :** Temperature (  $25 \pm 5$  ) °C  
Humidity (  $50 \pm 20$  ) %

**Test Procedure :** In - house method : CP-CH9  
by Comparison Technique with Azide Modification Method

**Tested by :** Warakorn Lernagtrakul

**Approved by :**

*Malee*

Approved Signatory

- ( ☒ ) Malee Butkruea  
( ☐ ) Saithip Meangmai  
( ☐ ) Warakorn Lernagtrakul

**Issue Date :** 31 May 2022

REVIEW BY	<i>Siriluk P.</i>
APPROVED BY	<i>Ku An</i>
NEXT CAL. DATE	<i>24/11/23</i>



Cert.No.: 22TW122

Page.: 2 of 2

**Condition of this result of calibration**

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	21MM430	21 Sep 2022

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

**Result :** Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 16K100498

<b>Titration Method (Azide Modification Method) (mg/L)</b>	<b>DO Meter Reading (mg/L)</b>	<b>Standard Deviation (mg/L)</b>
8.12	8.13	0.015

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

*Malu*

**a 1110482**



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22LM83

Page.: 1 of 2

## Certificate of Calibration

**Equipment :** DO Meter with Sensor

**Manufacturer :** YSI

**Model :** 5000-230V

**Serial No. :** 09J 101147

**ID No. :** BKK\_EN0017

**Submitted by :** ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

**Location :** TPA On Site Calibration Laboratory

**Received Order :** 20 May 2022

**Calibrated Date :** 30 May 2022

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**AC Line Voltage :** ( 220 ± 22 ) V

**Calibrated by :** Tawatchai Pama

**Approved by :** Malee Butkruea  
Approved Signatory

( ) Pornthippa Tameyakul  
( ✓ ) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 31 May 2022

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0039957



Equipment : DO Meter with Sensor  
Condition As-Received : Used Item  
Reference : 2205-0638DSC-10  
Procedure Used :-

Cert. No.: 22LM83

Page.: 2 of 2

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer ( IPRT ) into Temperature Bath.

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1502A	A09204	2218	04 Jan 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function :** Temperature measurement.

This instrument was connected with thermistor sensor , ID No.: 16K100498

<u>Calibration Point</u> ( °C )	<u>Immersion Depth</u> ( mm )	<u>Standard Temperature</u> ( °C )	<u>UUC* Reading</u> ( °C )	<u>Error</u> ( °C )	<u>Uncertainty</u> ( ± °C )	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.003	20.01	0.007	0.15	2.00

**UUC\* :** Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu -

a 1090806



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T230683

Page 1 of 4

## Certificate of Calibration

**Equipment** : Chamber ( Incubator )

**Manufacturer** : MEMMERT

**Model** : ICP 750

**Serial No.** : F818.0075

**Customer Code** : BKK\_EN0305

**ID No.** : T9571A4

**Customer** : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

**Customer Location** : Wet Chemistry Lab 2

**Date of Receipt** : 30 March 2023

**Calibrated By** : Sujjar Naknakred ( Site Calibration Manager )

**Approved By** :  / Boonchai Suriyawong ( Assistant Calibration Manager )

**Date of Issue** : 10 APR 2023

REVIEW BY	Sinluk P.
APPROVED BY	KL AL
NEXT CAL. DATE	05/04/24

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T230683

Page 2 of 4

## Calibration Report

**Equipment** : Chamber ( Incubator )  
**Date of Calibration** : 5 April 2023 ( Finished Time 4:30 PM )  
**Environment** : Temperature 22.9-28.6 °C  
Line Voltage 221.7-225.5 V

### Condition of this results of test. :

1. This instrument was calibrated by insert 12 standard resistance thermometer into its chamber and test according to WI-T20 ( based on ASTM E145-94 ( Reapproved 2001 ) and AS2853-1986. )

All data show below were final values and the initial data may be obtained upon request.

The temperature scale used was based on ITS - 90.

### 2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	37-(CH1-10)	T222493	28 November 2023
RTD	100 ohm	36-(CH1-10)	T222493	28 November 2023
DATA LOGGER	34970A	T193	T222493	28 November 2023

### 3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244. )

### 4. Condition of calibrated item : good

UUC Description :

Time Constant 2 Hour 24 Minute At 20 °C  
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

### 5. Result of test :

( ) without adjustment

( X ) after adjustment


Approved By. 



Certificate No T230683

## Calibration Report

Page 3 of 4

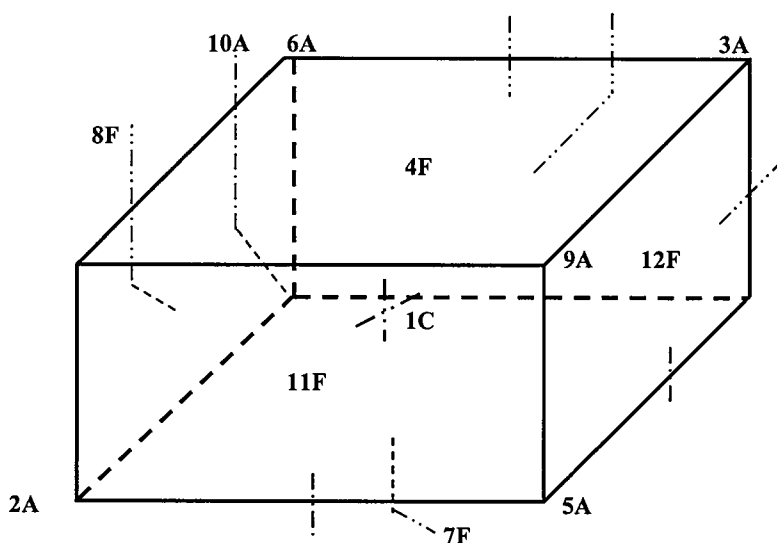

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	37CH1
2A	=	37CH2
3A	=	37CH3
4F	=	37CH4
5A	=	37CH5
6A	=	37CH6
7F	=	37CH7
8F	=	37CH8
9A	=	37CH9
10A	=	37CH10

11F	=	36CH1
12F	=	36CH2

Approved By. 

Certificate No. T230683

## Calibration Report

Page 4 of 4

### Measurement Results

Average Standard Reading at each position (°C)										
Calibration Point	37CH1	37CH2	37CH3	37CH4	37CH5	37CH6	37CH7	37CH8	37CH9	37CH10
20.0	20.32	20.28	20.17	20.22	20.22	20.04	20.17	19.74	20.31	19.93
	36CH1	36CH2								
	20.14	20.20								
Calibration Point	37CH1	37CH2	37CH3	37CH4	37CH5	37CH6	37CH7	37CH8	37CH9	37CH10
25	25.28	25.15	25.13	25.13	25.20	25.02	25.11	24.79	25.20	25.26
	36CH1	36CH2								
	25.13	24.94								


Chamber ( Incubator )			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor k
	Min , Max	Average					
20.0	19.9 , 20.1	20.0	20.02	0.09	0.54	0.38	2.00
25.0	24.9 , 25.1	25.0	25.03	0.03	0.51	0.38	2.00

\* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CG3154

Page.: 1 of 2

## Certificate of Calibration

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	BKK_EN0171
Manufacturer :	Witeg
Made in :	Germany
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd. Khwaeng Phatthanakan, Khet Suan Luang Bangkok 10250 Thailand
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	759 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Panward Pramklam

REVIEW BY	<i>Sin'luk P.</i>
APPROVED BY	<i>KLAL</i>
NEXT CAL. DATE	<i>29/03/2024</i>

Approved by :

Approved Signatory

- ( ) Pornthippa Tameyakul  
( ) Malee Butkruea  
(☒) Ponpan Paipim  
( ) Srisuda Khamtha

Issue Date :

31 August 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0044607



Equipment : Burette  
Received Date : 26 August 2022  
Condition As-Received : Used Item  
Calibration Date : 30 August 2022  
Reference : 2208-0918DSC-2

Cert.No.: 22CG3154

Page.: 2 of 2

**Condition of this result of calibration**

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID. No.</u>	<u>Certificate No.</u>	<u>Traceability</u>	<u>Due date</u>
1) Balance	AE200S	N03679	140RC001	21MM429	NIMT	22 Sep 2022
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	22H1243	NIST,NIMT	09 June 2023
3) Thermometer	-	1594592	140EC010	22I181	NIMT	10 Feb 2023

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.  
3. True value is converted to true volume at the standard temperature of 20 °C

**Calibration result :**

<b>Nominal capacity ( mL )</b>	<b>Reading ( mL )</b>	<b>Uncertainty ( ± mL )</b>	<b>k Factor</b>
50	49.9959	0.010	2.00

**Remark** mL = cm<sup>3</sup>

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$  , providing a level of confidence of approximately 95 %.

-o0o-

**a 1123908**



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230352

Page 1 of 5

## Certificate of Calibration

Equipment : HOT BLOCK

Manufacturer : Environmental Express

Model : B3000- 240

Serial No. : 2017CODW116

Customer Code : BKK\_EN0222

ID No. : T6769A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab2

Date of Receipt : 21 February 2023

Calibrated By : Watcharasak Puttarat (Technician )

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 20 MAR 2023

REVIEW BY	Simlut P.
APPROVED BY	KL AL
NEXT CAL. DATE	01/03/24

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230352

Page 2 of 5

## Calibration Report

Equipment : HOT BLOCK  
Date of Calibration : 1 March 2023  
Environment : Temperature : 22.9-24.4 °C  
Line Voltage : 222.7-227.8 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert 20 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20. All data show below were final values and the initial data from customer request .  
The temperature scale used was based on ITS - 90 .

#### 2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN121-TN130	T222122	5 October 2023
TC	TYPE T	TN131-TN140	T222122	5 October 2023
DATA LOGGER	34970A	T150	T222122	5 October 2023

#### 3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

#### 4. Condition of calibrated item : good

##### Equipment Description :

Time Constant 2 Hour 22 Minute At 150 °C  
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

#### 5. Adjustment :

( X ) without adjustment


( ) after adjustment

Approved By

Certificate No T230352

Page 3 of 5

## Calibration Report

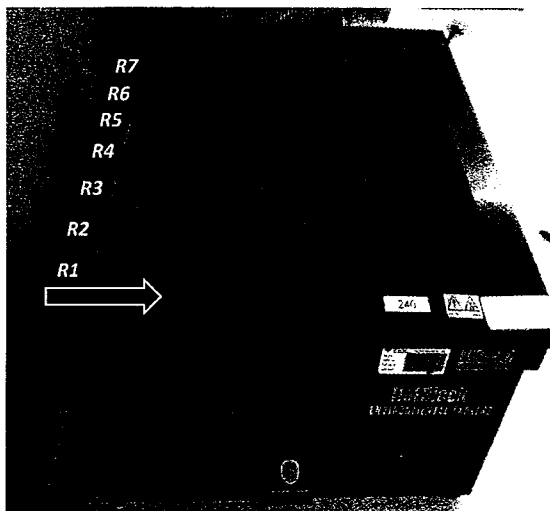

Row	Hole							
R7	H49	H50	H51	H52	H53	H54	H55	H56
R6	H41	H42	H43	H44	H45	H46	H47	H48
R5	H33	H34	H35	H36	H37	H38	H39	H40
R4	H25	H26	H27	H28	H29	H30	H31	H32
R3	H17	H18	H19	H20	H21	H22	H23	H24
R2	H9	H10	H11	H12	H13	H14	H15	H16
R1	H1	H2	H3	H4	H5	H6	H7	H8

**H: STANDARD THERMOCOUPLE TYPE T**

H1	=	TN121	H9	=	TN129	H17	=	TN137	H25	=	TN125	H33	=	TN133	H41	=	TN121	H49	=	TN129
H2	=	TN122	H10	=	TN130	H18	=	TN138	H26	=	TN126	H34	=	TN134	H42	=	TN122	H50	=	TN130
H3	=	TN123	H11	=	TN131	H19	=	TN139	H27	=	TN127	H35	=	TN135	H43	=	TN123	H51	=	TN131
H4	=	TN124	H12	=	TN132	H20	=	TN140	H28	=	TN128	H36	=	TN136	H44	=	TN124	H52	=	TN132
H5	=	TN125	H13	=	TN133	H21	=	TN121	H29	=	TN129	H37	=	TN137	H45	=	TN125	H53	=	TN133
H6	=	TN126	H14	=	TN134	H22	=	TN122	H30	=	TN130	H38	=	TN138	H46	=	TN126	H54	=	TN134
H7	=	TN127	H15	=	TN135	H23	=	TN123	H31	=	TN131	H39	=	TN139	H47	=	TN127	H55	=	TN135
H8	=	TN128	H16	=	TN136	H24	=	TN124	H32	=	TN132	H40	=	TN140	H48	=	TN128	H56	=	TN136

Approved By.





# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T230352

Page 4 of 5

## Calibration Report

### Measurement Results

			Average Standard Reading at each position ( ° C )									
Calibration Point			TN121	TN122	TN123	TN124	TN125	TN126	TN127	TN128	TN129	TN130
150	150.0	Max	152.61	150.49	150.10	148.27	149.85	151.19	149.99	149.29	149.97	150.03
		Min	152.15	149.87	149.73	147.75	149.26	150.78	149.49	148.56	149.15	149.15
		Average	152.41	150.22	149.90	147.99	149.48	150.92	149.71	148.92	149.51	149.67
			TN131	TN132	TN133	TN134	TN135	TN136	TN137	TN138	TN139	TN140
Max			149.84	148.34	148.34	149.88	152.39	149.73	149.66	149.16	149.76	151.18
Min			149.35	147.85	148.40	148.94	152.39	149.19	148.83	148.68	149.51	150.92
Average			149.67	148.10	148.59	149.55	152.39	149.36	149.25	148.96	149.64	151.05
			TN121	TN122	TN123	TN124	TN125	TN136	TN127	TN128	TN129	TN130
Max			152.91	150.56	149.20	148.63	149.78	151.28	150.09	148.83	148.16	148.33
Min			152.72	150.04	148.59	147.96	149.42	150.96	149.83	148.20	147.62	147.29
Average			152.80	150.29	148.89	148.30	149.60	151.08	149.97	148.52	147.90	147.80
			TN131	TN132	TN133	TN134	TN135	TN136	TN137	TN138	TN139	TN140
Max			148.81	148.04	148.56	148.11	149.07	149.06	148.58	149.85	149.07	150.89
Min			148.08	147.63	148.07	147.63	148.81	148.62	148.18	149.60	148.86	150.63
Average			148.45	147.84	148.36	147.81	148.94	148.84	148.37	149.74	148.96	150.78
			TN121	TN122	TN123	TN124	TN125	TN126	TN127	TN128	TN129	TN130
Max			150.76	152.63	151.14	150.47	151.07	150.93	149.35	150.31	149.28	149.81
Min			150.59	152.40	150.69	150.17	150.77	150.54	148.80	149.93	148.84	149.23
Average			150.69	152.52	150.95	150.33	150.94	150.73	149.18	150.10	149.04	149.56
			TN131	TN132	TN133	TN134	TN135	TN136				
Max			150.97	150.34	151.70	149.10	153.13	150.74				
Min			150.77	149.94	151.36	148.83	152.91	150.61				
Average			150.87	150.13	151.53	148.97	153.05	150.66				

Approved By





# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T230352

Page 5 of 5

## Calibration Report


### Measurement Results

HOT BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability ( $\pm$ °C)	Uncertainty ( $\pm$ °C)
	Min , Max	Average		
150.0	150 , 150.1	150.0	0.60	1.01

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k=2$  , providing a level of confidence of approximately 95 % .

Approved By. 

# Certificate of Calibration

Number of Page(s) 1 of 3

**Certificate No.** BSCC-UV-307/22  
**Equipment** UV/Vis Spectrophotometer  
**Model** UV-1800  
**Manufacturer** Shimadzu  
**Serial No.** A11454908533CD  
**ID No.** BKK\_EN0018  
**Date of receipt** 16 September 2022  
**Date of calibration** 16 September 2022  
**Date of issue** 23 September 2022

REVIEW BY *Siriluk P.*  
APPROVED BY *Kw An*  
16/9/23  
NEXT CAL. DATE *23/9/22*

**Customer name** ALS Laboratory Group (Thailand) Co., Ltd.

**Address** 104 Soi Phatthanakan 40, Phatthanakan Road, Phatthanakan, Suan Luang, Bangkok 10250

**Temperature** (22.1-23.3) °C (On site)

**Humidity** (58.8-63.2) %RH (On site)

**Equipment condition** Good Operation

**Calibration Location** Organic Prep

**Calibration Procedure** In-house method WI-UV-702-01 based on ASTM E275-01

**Traceability** Wavelength Accuracy is traceable to certificate No. 95917 and 95918  
Photometric Accuracy is traceable to certificate No. 95924 and 95937  
Stray Light is traceable to certificate No. 95908  
The above certificate are traceable to SI unit through Starna Scientific Ltd.  
(UKAS accredited calibration laboratory NO. 0659)

**Calibrated by** Mr.Waruth Janphung

Approved by



**Mr.Kanchit Choothep**  
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

# Certificate of Calibration

Certificate No.

BSCC-UV-307/22

Number of Page(s)

2 of 3

## Calibration Results:

### 1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty ( $\pm$ nm)
241.70	241.65	-0.05	0.18
334.02	333.92	-0.10	0.18
418.53	418.46	-0.07	0.18
572.99	572.96	-0.03	0.18
879.41	879.17	-0.24	0.18

### 2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ( $\pm$ A)
235	0.0000	0.0000	0.0000	0.0075
	0.7467	0.7461	-0.0006	0.0075
257	0.0000	0.0000	0.0000	0.0075
	0.8662	0.8647	-0.0015	0.0075
313	0.0000	0.0000	0.0000	0.0075
	0.2904	0.2911	0.0007	0.0075
350	0.0000	0.0000	0.0000	0.0075
	0.6429	0.6426	-0.0003	0.0075

\*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

# Certificate of Calibration

Certificate No. **BSCC-UV-307/22**

Number of Page(s)

3 of 3

## Calibration Results:

### 3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ( $\pm A$ )
420.0	0.0000	0.0000	0.0000	0.0042
	0.5783	0.5777	-0.0006	0.0042
	0.7628	0.7635	0.0007	0.0046
	1.0206	1.0230	0.0024	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5621	0.5618	-0.0003	0.0042
	0.7455	0.7460	0.0005	0.0048
	0.9985	1.0005	0.0020	0.0042
465.0	0.0000	0.0000	0.0000	0.0042
	0.5227	0.5219	-0.0008	0.0042
	0.6880	0.6884	0.0004	0.0051
	0.9487	0.9503	0.0016	0.0042
546.1	0.0000	0.0000	0.0000	0.0042
	0.5207	0.5199	-0.0008	0.0042
	0.6973	0.6971	-0.0002	0.0049
	0.9959	0.9964	0.0005	0.0042
590.0	0.0000	0.0000	0.0000	0.0042
	0.5544	0.5534	-0.0010	0.0042
	0.7253	0.7242	-0.0011	0.0050
	1.0942	1.0943	0.0001	0.0042
635.0	0.0000	0.0000	0.0000	0.0042
	0.5616	0.5606	-0.0010	0.0042
	0.6927	0.6921	-0.0006	0.0053
	1.0881	1.0885	0.0004	0.0042

\*CNR = Customer not request

### 4. Stray Light\*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)		
	Wavelength (nm)	Transmission (%T)	Absorbance (A)
200.96 $\pm$ 0.11nm	200.30	0.9505	2.0229

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

\*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

**\*\*\*End of Certificate\*\*\***

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

**Sartorius (Thailand) Co., Ltd.**

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com

**SARTORIUS**

# Certificate

## of Calibration

REVIEW BY	<u>Sirilut P.</u>
APPROVED BY	<u>LL AL</u>
NEXT CAL. DATE	<u>8/2/24</u>

Model Number : MSE224S-100-DUDescription : Analytical BalanceSerial Number : 26207042ID No. : BKK\_EN0002Manufacturer : SartoriusCertificate No. : 23BCI0072Issued Date : Monday, February 13, 2023Reference No. : 203245Page No. : 1 of 2Customer Name : ALS Laboratory Group (Thailand)Co., Ltd.104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.Calibrated Place : Balance RoomCalibrated By : Mr. Chonchai InthanaCalibration Date : Wednesday, February 08, 2023**Calibration**Procedure No. : This calibration was conducted by  
Using in-house calibration procedure number (WI-003)Based on UKAS LAB 14 : 2019**Metrological data :**Capacity : 220 g Readability : 0.0001 g**Ambients Conditions:**Temperature : 23.2 °C ± 5.0 °CHumidity : 60.0 % RH ± 10.0 % RHPressure :                      ±                     **Reasons for calibration**☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ MaintenanceEquipment Condition: ☒ Good Operate ☐ Fair**Measurement Method****UKAS Publication Ref :Lab 14**

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

**Traceability:**

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2, YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

SOP FM 33 03 February 2022

  
Mr. Chonchai Inthana (Technical Manager)S  
T  
A  
M  
P

# Certificate of Calibration

Model Number : MSE224S-100-DU  
 Description : Analytical Balance  
 Serial Number : 26207042  
 ID No. : BKK\_EN0002  
 Manufacturer : Sartorius

Certificate No. : 23BCI0072  
 Issued Date : Monday, February 13, 2023  
 Reference No. : 203245  
 Page No. : 2 of 2

## Calibration Results : Without Adjustment

### Repeatability



The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0000	199.9999
Tolerance	20.0000	200.0000
0.0001 g	20.0000	199.9999
	20.0001	200.0000
	20.0000	200.0000
Nominal Value : (High Load)	20.0000	199.9999
200 g	20.0000	199.9999
Tolerance	20.0000	200.0000
0.0001 g	20.0000	199.9999
	20.0001	199.9999
Standard Deviation	0.00004	0.00005

### Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 50 g  
 Tolerance 0.0004 g



Difference	
1	—
2	-0.0001
3	0.0000
4	0.0001
5	0.0000
6	—

### Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00014
0.1	0.1000	0.1000	0.0000	0.00014
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	199.9999	-0.0001	0.00030

End of Report.



# Metrological Center

## SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th



Certificate No. T220139

Page 1 of 3

## Certificate of Calibration

Equipment : Liquid Bath ( Water )

Manufacturer : MEMMERT

Model : WNB29

Serial No. : L611.0135

Customer Code : BKK\_EN0148

ID No. : T6455A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250


Customer Location : ORGANIC PREPARATION LAB

Date of Receipt : 26 January 2022

Calibrated By : Watcharapon Sangtong (Technician )

Approved By :  / Sujjar Naknakred (Site Calibration Manager)

Date of Issue : 08 FEB 2022

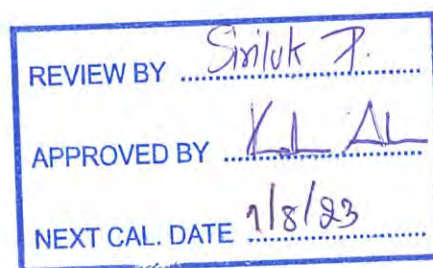

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Certificate No. T220139

Page 2 of 3

## Calibration Report

**Equipment** : Liquid Bath ( Water )  
**Date of Calibration** : 31 January 2022  
**Environment** : Temperature : 22.4-23.9 °C  
Line Voltage : 221.4-225.4 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 ( based on ASTM E715-80 ( Reapproved 2001 ) ).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M34 (CH1-CH5)	T210115	2 February 2022
DATA LOGGER	34970A	T47	T210115	2 February 2022

3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour - Minute At 60 °C

5. Adjustment :

( X ) without adjustment

( ) after adjustment


Approved By. 



Certificate No. T220139

Page 3 of 3

## Calibration Report

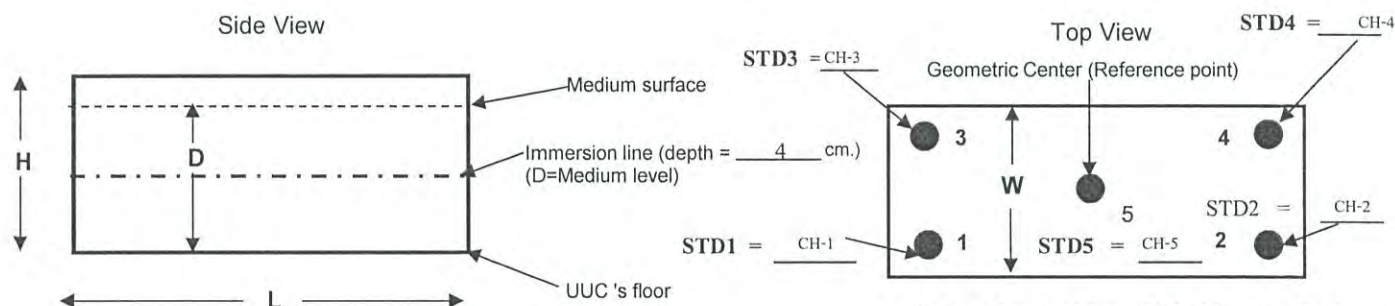

- D = Medium level : 8 cm.
  - UUC's medium : Water
  - Working standards are located at 2.5 cm. away from each corner and walls.
- Working space dimension : 62 × 41 × 14 (W×L×H)

### Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)				
	CH-1	CH-2	CH-3	CH-4	CH-5
60	59.95	60.04	60.12	60.01	59.89
85	85.17	84.89	85.34	84.78	84.93
95	93.46	93.14	93.81	93.05	93.28

Liquid Bath ( Water )			Temperature Distribution			
Setting (°C)	Reading (°C)		Stability (± °C)	Uniformity (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
	Min , Max	Average				
61.0	60.9 , 61	61.0	0.10	0.19	0.25	2.00
86.0	85.9 , 86.1	86.0	0.12	0.39	0.32	2.06
95.0	94.8 , 95.1	94.9	0.14	0.51	0.38	2.11

\* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CH1222

Page.: 1 of 2

## Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	Seven Compact S220
Serial No. :	B520948426
ID No. :	BKK_EN0072
Condition As-Received:	Used Item
Received Date :	09 September 2022
Calibration Date :	12 September 2022
Reference :	2209-0312DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)

REVIEW BY	Sinluk P.
APPROVED BY	KL AL
NEXT CAL. DATE	12/03/24

Calibrated by : Warakorn Lerngagtrakul

Approved by :

*Malee*

Approved Signatory

- ( ☒ ) Malee Butkruea  
( ☐ ) Saithip Meangmai  
( ☐ ) Warakorn Lerngagtrakul

Issue Date : 15 September 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert. No.: 22CH1222

Page.: 2 of 2

**Condition of this calibration result**

## 1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	22E2769	24 Aug 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	823320	20 June 2024
pH 6.985	CPA chem	794122	14 Feb 2023
pH 10.008	CPA chem	823323	20 June 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results****Function : mV Measurement****Performing standard curve by Fluke at pH (4,7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( $\pm$ mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: B520948426	4.000	177.48	177.4	4.000	0.058	2.00
	7.000	0.00	0.0	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

**Function : pH Measurement****Performing three buffers standard curve by using buffer nominal pH (4,7,10)**

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement ( $\pm$ )	Coverage factor <i>k</i>
pH Electrode S/N.: PCE-86-EX1001	4.008	3.999	153.9	0.0055	2.09
	6.985	7.017	-13.7	0.0084	2.00
	10.008	9.996	-179.0	0.0078	2.06

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.

a 1126274





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 22T1678

Page : 1 of 2

Equipment : Digital Thermometer With Sensor

Manufacturer: Testo

Model : 106

Serial No.: 83637356/0122

ID No.: BKK\_LG0048

Condition As-Received: New Item

Received Date: 26 August 2022

Calibration Date: 12 September 2022  
to 19 September 2022

Reference: 2208-0918DSC

Ambient Temperature: ( 25 ± 3 ) °C

Relative Humidity: ( 50 ± 20 ) %

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Procedure used: Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.  
The temperature scale used was based on ITS-90.

### Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Digital Thermometer	1529	A7A609	2111126	14 Oct 2022
2) Industrial Platinum Resistance Thermometer	5627	824304	2111126	14 Oct 2022

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

REVIEW BY	<i>Chayathorn P.</i>
APPROVED BY	<i>Wanlop P.</i>
NEXT CAL. DATE	12/09/23

Calibrated by : Thatchanan Chankong

Issue Date : 22 September 2022

Approved Signatory :

- [ ] Phalinee Prabpaipal  
[ ] Chatchawan Khunpiluek  
[✓] Wanlop Larpkurn



Cert. No.: 22T1678

Page.: 2 of 2

**Result of Calibration:-**

Without Adjustment

**Function:**

Temperature measurement

Dimension of probe : Diameter 3 mm., Length 55 mm. Sheath material : Stainless Steel

<b>Immersion</b>	<b>Standard</b>	<b>UUC*</b>		<b>Uncertainty</b>
<b><u>Depth</u></b>	<b><u>Temperature</u></b>	<b><u>Reading</u></b>	<b><u>Error</u></b>	<b><u>of Measurement</u></b>
( mm.)	( °C )	( °C )	( °C )	( ±°C )
50	25.0038	25.1	0.0962	0.12
50	30.0027	30.0	-0.0027	0.12
50	35.0026	35.1	0.0974	0.12
50	40.0043	40.1	0.0957	0.12
50	45.0074	45.1	0.0926	0.12

**UUC\*** : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

-o0o-





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 21TM2189

Page.: 1 of 3

## Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Memmert

Model : UFE 500

Serial No. : G511.1574

ID No. : BKK\_EN0007

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Location : Oven Room

Received Order : 1 December 2021

Calibration Date : 1 December 2021

Ambient Temperature : (  $26 \pm 10$  ) °C

Relative Humidity : (  $50 \pm 30$  ) %

Calibrated by : Khit Ruttanaprapachai

Approved by :

*Malee*

Approved Signatory

( ☒ ) Pornthippa Tameyakul

( ☒ ) Malee Butkruea

( ☐ ) Suwit Imjai

Issue Date : 7 December 2021

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0032815





Equipment : Hot Air Oven  
 Condition As-Received : Used Item  
 Reference : 2112-0002OC-1

Cert. No.: 21TM2189  
 Page.: 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34970A	MY44060450	21LM4/1	06 Mar 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

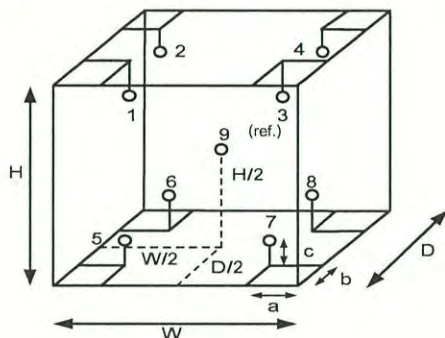

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	25	25
REL.Humid. ( % )	51	53
AC Supply ( Volt )	221	222

Ref. Std. ID No.: @ Calibration Point		
Position :	( 104 ) °C	( 121,175,180 ) °C
1	19-14RTD-01	19-14TC-01
2	19-14RTD-02	19-14TC-02
3	19-14RTD-03	19-14TC-03
4	19-14RTD-04	19-14TC-04
5	19-14RTD-05	19-14TC-05
6	19-14RTD-06	19-14TC-06
7	21-14RTD-07	19-14TC-07
8	19-14RTD-08	19-14TC-08
9 (ref.)	19-14RTD-09	19-14TC-09

Probe Installation Details :		Dimension of Chamber :	
a =	5.0 cm	D =	0.40 m
b =	5.0 cm	W =	0.56 m
c =	5.0 cm	H =	0.48 m
Capacity =			0.11 m <sup>3</sup>

*Malu*





Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2112-0002OC-1  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Close

Cert. No.: 21TM2189

Page.: 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
104.0	104.0	104.0	0.059	0.52	0.59	0.45	2
121.0	121.0	121.0	0.11	0.75	1.2	1.1	2
175.0	175.0	175.0	0.13	0.90	1.6	1.1	2
180.0	180.0	180.0	0.13	0.93	1.6	1.1	2

Calibration Point ( °C )	Measured Temperature ( °C )								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	104.265	104.229	104.080	103.922	104.390	104.304	104.284	103.994	103.909
121.0	120.838	120.519	120.661	120.524	121.162	120.855	120.703	120.126	120.726
175.0	175.021	174.603	174.848	174.652	175.830	175.321	175.411	174.440	175.222
180.0	179.792	179.374	179.575	179.376	180.643	180.081	180.174	179.217	180.014

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.





# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T221642

Page 1 of 5

## Certificate of Calibration

Equipment : Digestion Unit

Manufacturer : SCP Science

Model : DigiPRER HT

Serial No. : HTC1120480658

Customer Code : BKK\_EN0366

ID No. : T2635A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab 1

Date of Receipt : 27 June 2022

Calibrated By : Sujjar Naknakred ( Site Calibration Manager )

Approved By :  / Boonchai Suriyawong ( Site Calibration Manager )

Date of Issue : 04 JUL 2022

REVIEW BY	<u>Sinluk P.</u>
APPROVED BY	<u>Kel AL</u>
NEXT CAL. DATE	<u>30/06/23</u>

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T221642

Page 2 of 5

## Calibration Report

**Equipment** : Digestion Unit  
**Date of Calibration** : 30 June 2022  
**Environment** : Temperature : 23.9 - 26.3 °C  
Line Voltage : 221.4 - 225.1 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T10.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M7-(CH16-17,CH19-CH20)	T212004	15 October 2022
DATA LOGGER	34970A	T121	T212004	15 October 2022

3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant - Hour 26 Minute At 380 °C

Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max

☐ Close


☒ Not Available

5. Adjustment :

( X ) without adjustment

( ) after adjustment


Approved By. \_\_\_\_\_



Certificate No. T221642

Page 3 of 5

## Calibration Report

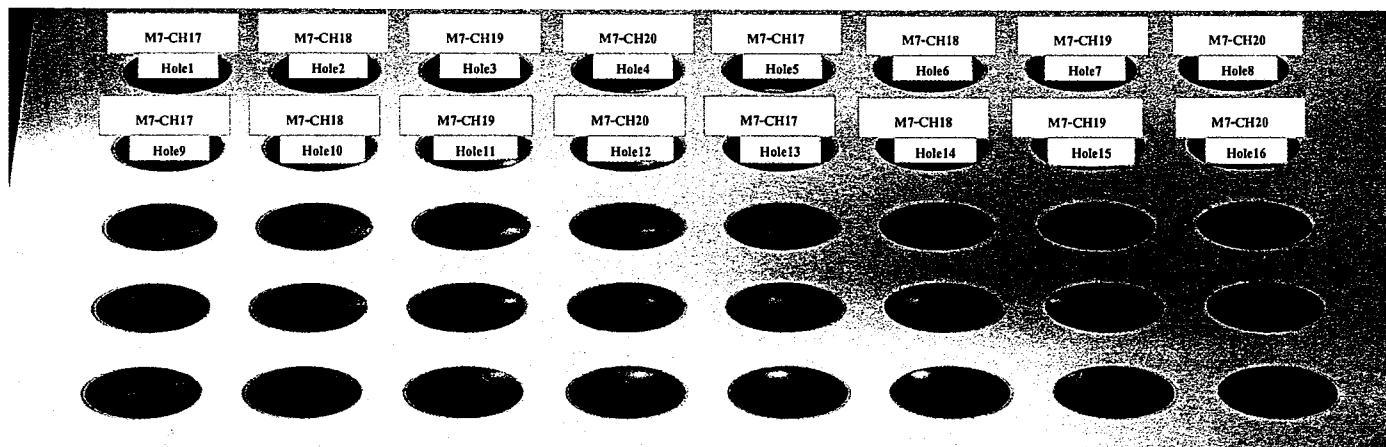

FRONT

### Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
°C	°C	°C	Reading	Hole1	Hole2	Hole3	Hole4	Hole5	Hole6	Hole7	Hole8
				M7-CH17	M7-CH18	M7-CH19	M7-CH20	M7-CH17	M7-CH18	M7-CH19	M7-CH20
380.0	380.0	379.4 - 380.7	Max °C	379.1	379.8	379.3	377.4	377.6	379.3	379.6	377.9
			Min °C	378.7	379.4	378.9	377.0	377.3	378.8	379.1	377.3
			Average °C	378.9	379.6	379.1	377.2	377.4	379.1	379.3	377.6
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.2	0.2	0.3

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
°C	°C	°C	Reading	Hole9	Hole10	Hole11	Hole12	Hole13	Hole14	Hole15	Hole16
				M7-CH17	M7-CH18	M7-CH19	M7-CH20	M7-CH17	M7-CH18	M7-CH19	M7-CH20
380.0	380.0	379.4 - 380.7	Max °C	378.5	378.8	378.1	379.0	380.3	381.6	381.0	379.5
			Min °C	377.8	378.2	377.6	378.6	379.9	381.2	380.5	378.9
			Average °C	378.2	378.5	377.9	378.8	380.1	381.4	380.7	379.2
			Stability ± °C	0.3	0.3	0.2	0.2	0.2	0.2	0.3	0.3


Approved By.



Certificate No. T221642

Page 4 of 5

## Calibration Report

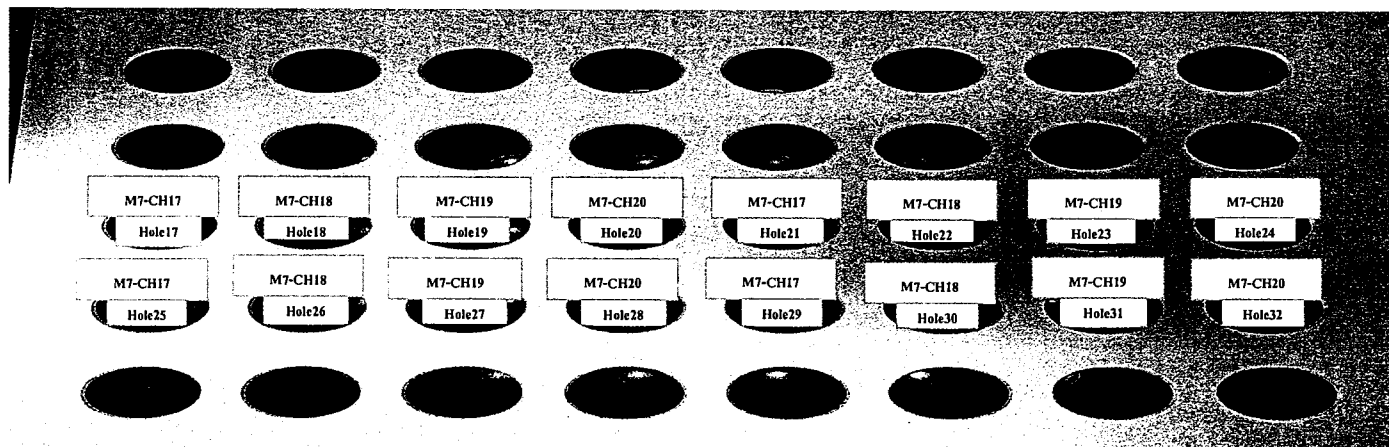

FRONT

### Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole17	Hole18	Hole19	Hole20	Hole21	Hole22	Hole23	Hole24
				M7-CH17	M7-CH18	M7-CH19	M7-CH20	M7-CH17	M7-CH18	M7-CH19	M7-CH20
380.0	380.0	379.4 - 380.7	Max °C	378.4	378.8	378.0	379.2	379.0	382.0	381.5	380.3
			Min °C	377.8	378.2	377.7	378.8	378.7	381.5	381.1	379.6
			Average °C	378.1	378.5	377.9	379.0	378.9	381.8	381.3	379.9
			Stability ± °C	0.3	0.3	0.2	0.2	0.2	0.3	0.2	0.4

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole25	Hole26	Hole27	Hole28	Hole29	Hole30	Hole31	Hole32
				M7-CH17	M7-CH18	M7-CH19	M7-CH20	M7-CH17	M7-CH18	M7-CH19	M7-CH20
380.0	380.0	379.4 - 380.7	Max °C	378.3	378.7	378.4	378.8	379.6	382.6	382.0	380.8
			Min °C	377.6	378.3	377.9	378.4	379.3	382.2	381.4	380.0
			Average °C	378.0	378.5	378.1	378.6	379.5	382.4	381.7	380.4
			Stability ± °C	0.3	0.2	0.2	0.2	0.2	0.2	0.3	0.4


Approved By.



Certificate No. T221642

Page 5 of 5

## Calibration Report

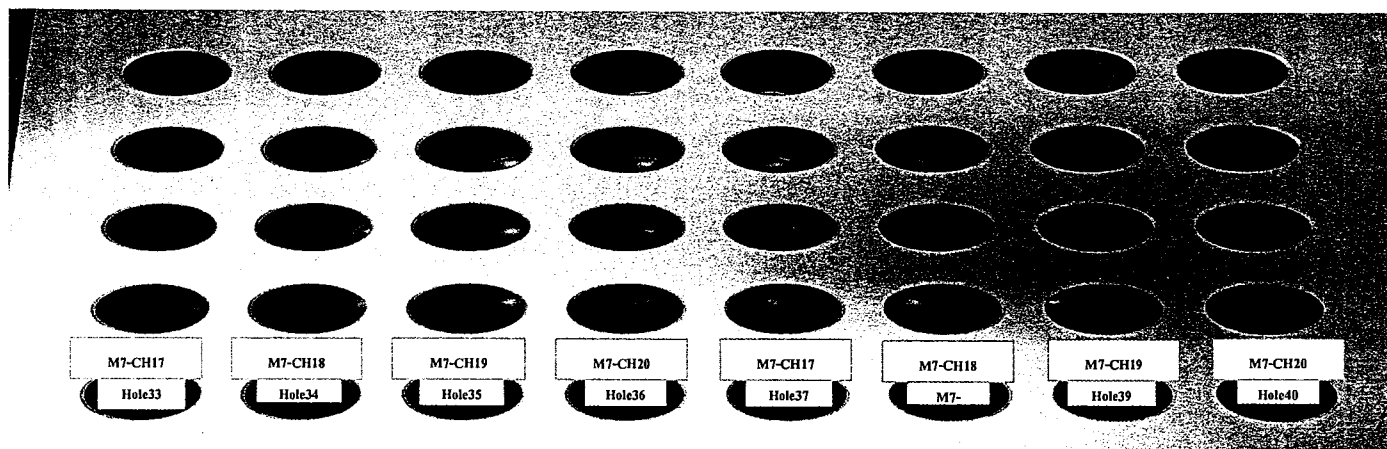

FRONT

### Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole33	Hole34	Hole35	Hole36	Hole37	Hole38	Hole39	Hole40
				M7-CH17	M7-CH18	M7-CH19	M7-CH20	M7-CH17	M7-CH18	M7-CH19	M7-CH20
380.0	380.0	379.4 - 380.7	Max °C	378.6	376.7	377.2	378.0	380.0	382.2	381.5	379.7
			Min °C	378.1	376.2	376.7	377.5	379.5	381.7	380.9	379.1
			Average °C	378.3	376.5	377.0	377.7	379.8	381.9	381.2	379.4
			Stability ± °C	0.3	0.3	0.3	0.3	0.3	0.3	0.3	0.3

 The expanded uncertainty of temperature measurement was  $\pm 2.49$  °C

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95 %.

Approved By.





บริษัท ดับเบิล เอส ไดแอกโนสติกส์ จำกัด  
DOUBLE S DIAGNOSTICS CO., LTD.

4 ซอยอุดมสุข 14 แขวงบางนา เขตบางนา กรุงเทพฯ 10260 โทรศัพท์: (02) 747-7009 โทรสาร: (02) 747-7008  
4 Soi Udomsuk 14, Bangna, Bangkok 10260 Tel. (02) 747-7009 Fax: (02) 747-7008

Maintenance Plan YEAR : 2023

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
รอบ	PM-6M ck											

Periodical maintenance check list for Konelab

	6M	12M	Note!
1.Diluent-wash tubing change	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
2.ISE tubing change	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	none.
3.Syringe check/change		<input type="checkbox"/>	
4.Dispensing check/ change		<input type="checkbox"/>	
5.Waste tubing change when necessary		<input type="checkbox"/>	
6.Lamp check/change	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
7.Mixer paddle/paddle change(not Konelab20)		<input type="checkbox"/>	
8.ISE needles check/change		<input type="checkbox"/>	
9.Pump tubing check/ chance	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
10.Broken/worn out part check /change		<input type="checkbox"/>	
11.Peristaltic pump check /cleaning/ lubrication	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
12.Heating check		<input type="checkbox"/>	
13.Cooling check		<input type="checkbox"/>	
14.Dispenser mechanic check/adjustment	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
15.Cuvette transfer mechanic check/adjustment	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
16.Dispenser movement check/adjustment	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
17.Sample/reagent register check/adjustment	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
18.Dispensing tubing tightness check	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
19.Photometer and optics cleaning/check/adjustment	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
20.Workstation PC cleaning if necessary	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
21.Mechanic cleaning/lubrication	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
22.Instrument cleaning if necessary	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
23.Complete analyzer testing with waterblank/QC or sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
24.Test parameters/Adjustment/config. Save to USB key	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
25.UPS Test	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

Place: ALS Laboratory Instrument: Konelab Aquakem 250  
Date/Time: 05-01-66 Serial no: 22781  
Service done by: M. S. S. Install date:  
Signature of customer: Date/Time:



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T222502

Page 1 of 4

## Certificate of Calibration

Equipment : Chamber ( Oven )

Manufacturer : Memmert

Model : UF 450

Serial No. : B7170531

Customer Code : BKK\_EN0273

ID No. : T8042A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Oven Room

Date of Receipt : 23 November 2022

Calibrated By : Sujjar Naknakred ( Site Calibration Manager )

Approved By :  /Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 09 DEC 2022

REVIEW BY	Sinluk P.
APPROVED BY	KL AL
NEXT CAL. DATE	29/05/24

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T222502

Page 2 of 4

## Calibration Report

**Equipment** : Chamber ( Oven )  
**Date of Calibration** : 29 November 2022  
**Environment** : Temperature : 29.1-29.6 °C  
Line Voltage : 221.3-223.2 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors and nine standard thermocouples type T into its chamber , the other one resistance thermometer detector use for ambient temperature measurement .  
The calibration was done in according to WI-T20 ( based on ASTM E145-94 ( Reapproved 2001) and AS2853-1986 ).  
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	27-(CH1-10)	T210004	30 December 2022
TC	TYPE T	TN261-TN270	T210010	30 December 2022
DATA LOGGER	34970A	T149	T210004	30 December 2022

3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 49 Minute At 104 °C  
Fresh Air Damper ☒ Open ☐ Min ☐ Medium ☒ Max  
☐ Close  
☐ Not Available

5. Adjustment :

( ) without adjustment

( X ) after adjustment


Approved By. Bm Loi



Certificate No. T222502

Page 3 of 4

## Calibration Report

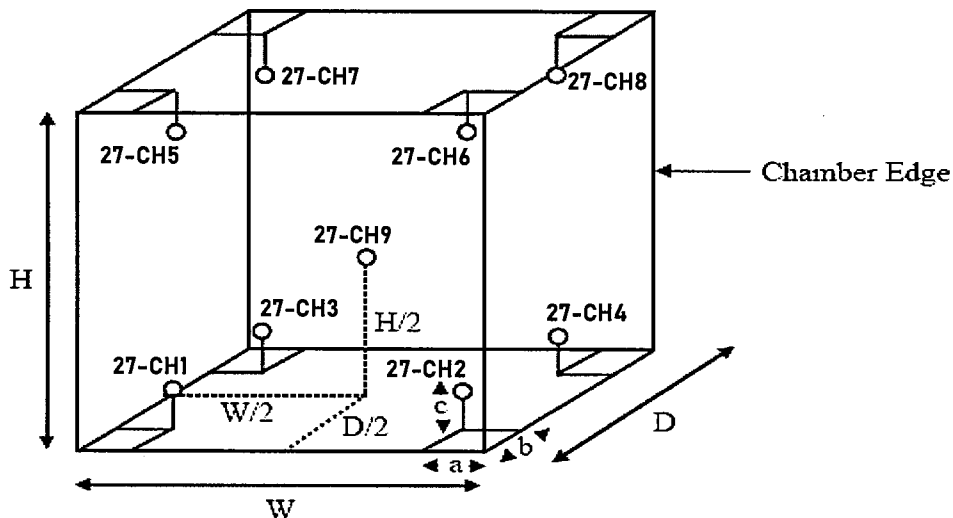

### Remark :

Internal Dimensions of Chamber : W (Width) = 104 cm. , H (Height) = 72 cm. and D (Depth) = 60 cm.

Size of Installed Standard sensor number 27-CH1 to number 27-CH8 : a = 5 cm. , b = 5 cm. and c = 5 cm.

Size of Installed Standard sensor number 27-CH9 : W/2 = 104 cm./2 , H/2 = 72 cm./2 and D/2 = 60cm./2

### Measurement Results

Average Standard Reading at each position ( °C )									
Calibration Point	27-CH1	27-CH2	27-CH3	27-CH4	27-CH5	27-CH6	27-CH7	27-CH8	27-CH9
104	104.07	103.60	103.45	104.02	104.47	103.57	104.59	103.78	104.18


Chamber ( Oven )			Temperature Distribution				
Setting ( °C )	Reading ( °C )		Average ( °C )	Stability ( ± °C )	Uniformity ( °C )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
	Min , Max	Average					
104.0	-	104.0	103.97	0.07	0.70	0.42	2.00

\* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.


The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 

Certificate No. T222502

Page 4 of 4

## Calibration Report

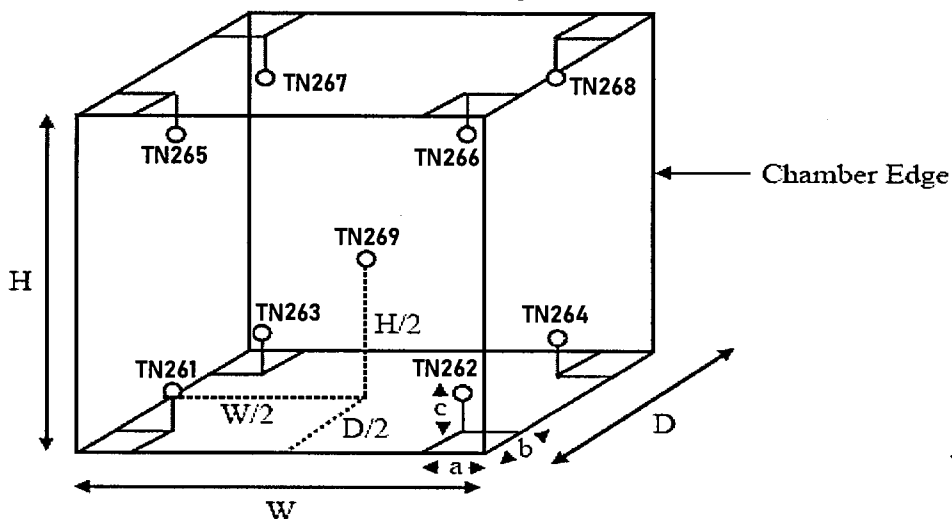

**Remark :**

Internal Dimensions of Chamber : W (Width) = 104 cm. , H (Height) = 72 cm. and D (Depth) = 60 cm.

Size of Installed Standard sensor number TN261 to number TN268 : a = 5 cm. ,b = 5 cm. and c = 5 cm.

Size of Installed Standard sensor number TN269 : W/2 = 104 cm./2 , H/2 = 72 cm./2 and D/2 = 60cm./2

**Measurement Results**

Calibration Point	Average Standard Reading at each position ( ° C )								
	TN261	TN262	TN263	TN264	TN265	TN266	TN267	TN268	TN269
180	179.14	179.17	179.65	179.26	180.41	179.64	181.18	180.99	180.36

Chamber ( Oven )			Temperature Distribution				
Setting ( ° C )	Reading ( ° C )		Average ( ° C )	Stability ( ± ° C )	Uniformity ( ° C )	Uncertainty ( ± ° C )	Coverage Factor <i>k</i>
	Min , Max	Average					
180.0	-	180.0	179.98	0.38	1.78	1.10	2.00


\* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing

a level of confidence of approximately 95 % .

Approved By. 



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM101

Page.: 1 of 3

## Certificate of Calibration

**Equipment :** Autoclave  
**Manufacturer :** Sanyo  
**Model :** MLS-3781  
**Serial No. :** 830167  
**ID No. :** BKK\_ML0037  
**Submitted by :** ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand  
**Location :** Media Preparation Room  
**Received Order :** 21 January 2022  
**Calibration Date :** 21 January 2022  
**Ambient Temperature :** ( 26 ± 10 ) °C  
**Relative Humidity :** ( 50 ± 30 ) %  
**Calibrated by :** Krisda Malee

REVIEW BY	Sithichok T.
APPROVED BY	[Signature]
NEXT CAL. DATE	22/07/23

**Approved by :**

*Malee*

Approved Signatory

- ( ☒ ) Pornthippa Tameyakul  
( ☒ ) Malee Butkruea  
( ☐ ) Suwit Imjai

**Issue Date :**

3 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0037379





Equipment : Autoclave  
 Condition As-Received : Used Item  
 Reference : 2201-0616OC-3

Cert. No.: 22TM101

Page.: 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1 ) Data Acquisition	34972A	MY57013711	21LM7	16 Jun 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3\*\*


(\*\* = Categorization of pathogens according to hazard and categories of containment, second edition, 1990 )

It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

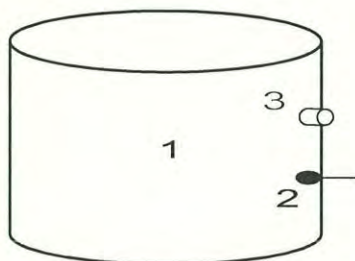

	<u>Environmental</u>		
	( °C )	( %R.H. )	( Volt )
<b>Beginning of Calibration</b>	27	57	220
<b>Finished of Calibration</b>	26	59	221

<u>Position</u>	<u>Description</u>	<u>Ref. Std. ID No.:</u>
1 =	Center of chamber	18-18TC-01
2 =	Temperature sensor	18-18TC-02
3 =	Exhaust port	18-18TC-03

*Malu*





Equipment : Autoclave  
Condition As-Received : Used Item  
Reference : 2201-0616OC-3

Cert. No.: 22TM101

Page.: 3 of 3

**Result of Calibration :-** ( \* ) Without Adjustment

Operating parameter Set : Temperature = 108 °C

Sterilization period = 15 minute

UUC* Setting ( °C )	UUC* Reading ( °C )	Position	Average* Standard Reading ( °C )	Stability ( ± °C )	Pressure Reading ( MPa )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
108	108	1	108.044	0.29	0.040	0.94	2
		2	108.133				
		3	108.142				

Operating parameter Set : Temperature = 121 °C

Sterilization period = 15 minute

UUC* Setting ( °C )	UUC* Reading ( °C )	Position	Average* Standard Reading ( °C )	Stability ( ± °C )	Pressure Reading ( MPa )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
121	121	1	121.082	0.21	0.11	0.91	2
		2	121.068				
		3	121.128				

**Average\*** : The average of 30 values in each position.

**Stability** : One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM102

Page.: 1 of 3

## Certificate of Calibration

Equipment : Incubator  
Manufacturer : SHEL-LAB  
Model : 1915A  
Serial No. : 0200599  
ID No. : BKK\_ML0010  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand  
Location : Incubation & Micrological Reading  
Received Order : 21 January 2022  
Calibration Date : 21 January 2022  
Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %  
Calibrated by : Krisda Malee

REVIEW BY	Sithichok T.
APPROVED BY	[Signature]
NEXT CAL. DATE	22/07/23

Approved by :

*Malee*

Approved Signatory

- ( ☒ ) Pornthippa Tameyakul  
( ☒ ) Malee Butkruea  
( ☐ ) Suwit Imjai

Issue Date :

3 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0037377





Equipment : Incubator  
 Condition As-Received : Used Item  
 Reference : 2201-0616OC-1

Cert. No.: 22TM102

Page.: 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34972A	MY57013711	21LM7	16 Jun 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

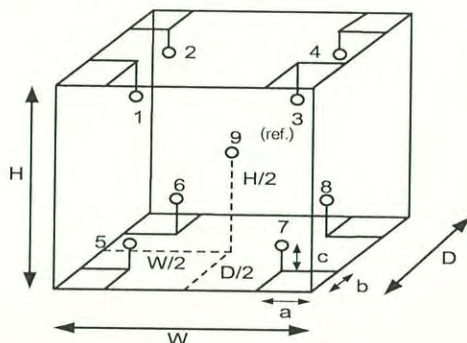

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	26	25
REL.Humid. ( % )	53	54
AC Supply ( Volt )	220	221

Position :	Ref. Std. ID No.:
1	18-18RTD-01
2	18-18RTD-02
3	18-18RTD-03
4	18-18RTD-04
5	18-18RTD-05
6	18-18RTD-06
7	18-18RTD-07
8	18-18RTD-08
9 (ref.)	18-18RTD-09

**Probe Installation Details :**

a = 10 cm  
 b = 10 cm  
 c = 10 cm

**Dimension of Chamber :**

D = 0.90 m  
 W = 0.75 m  
 H = 1.2 m  
 Capacity = 0.81 m<sup>3</sup>

*Malu .*



Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2201-0616OC-1  
**Result of Calibration :-** ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Close

Cert. No.: 22TM102

Page.: 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
35.0	35.0	35.0	0.043	0.41	0.42	0.30	2

Calibration Point ( °C )	Measured Temperature ( °C )								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
35.0	34.801	34.868	34.862	35.012	35.040	35.010	35.084	35.040	35.178

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Mahu.





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1571

Page : 1 of 3

## Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Binder

Model : ED 240/E2

Serial No. : 00-15533

ID No. : BKK\_ML0013

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 21 November 2022

Calibration Date : 21 November 2022

Ambient Temperature : (  $26 \pm 10$  ) °C

Relative Humidity : (  $50 \pm 30$  ) %

Calibrated by : Krisda Malee

Approved by :

*Malee*

Approved Signatory

( ) Pornthippa Tameyakul

(✓) Malee Butkruea

( ) Suwit Imjai

Issue Date : 29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0048150



Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2211-0623OC-1

Cert. No.: 22TM1571

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) After Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Not Available

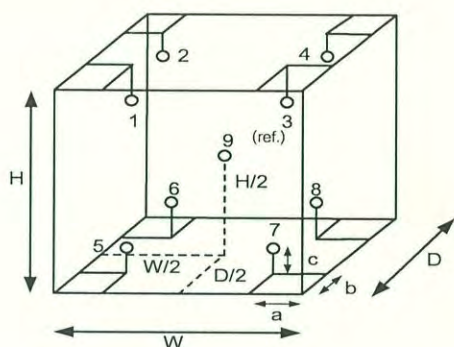

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	26	26
REL.Humid. ( % )	53	55
AC Supply ( Volt )	219	220

Position :	Ref. Std. ID No.:
1	21-15TC-01
2	21-15TC-02
3	21-15TC-03
4	21-15TC-04
5	21-15TC-05
6	21-15TC-06
7	21-15TC-07
8	21-15TC-08
9 (ref.)	21-15TC-09

**Probe Installation Details :**

a = 5.0 cm  
b = 5.0 cm  
c = 5.0 cm

**Dimension of Chamber :**

D = 0.50 m  
W = 0.80 m  
H = 0.60 m  
Capacity = 0.24 m<sup>3</sup>

*Malu.*





Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2211-0623OC-1  
Result of Calibration :- ( \* ) After Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Not Available

Cert. No.: 22TM1571

Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
180	180	180	0.70	1.5	2.9	1.4	2

Calibration Point ( °C )	Measured Temperature ( °C )								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
180	179.520	180.585	178.855	179.482	178.827	179.938	179.074	180.199	180.068

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

*Malu*



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM637

Page : 1 of 3

## Certificate of Calibration

**Equipment :** Water Bath

**Manufacturer :** Memmert

**Model :** WNE 45

**Serial No. :** L712.0429

**ID No. :** BKK\_ML0056

**Submitted by :** ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

**Location :** Incubator & Microbiological Reading

**Received Order :** 20 April 2023

**Calibration Date :** 20 April 2023

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Kunchit Promprat

REVIEW BY	Sithichok
APPROVED BY	
NEXT CAL. DATE	20/4/24

Approved by :

*Malee*

Approved Signatory

- ( ) Pornthippa Tameyakul  
( ☒ ) Malee Butkruea  
( ) Suwit Imjai

Issue Date :

24 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0053357





Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2304-0253OC-1

Cert. No.: 23TM637

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer ( IPRT ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1 ) Data Acquisition	34970A	MY44073381	22LM78/1	12 May 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Heat transfer medium used :** Water

	<u>Environmental</u>		<u>AC Voltage Supply</u>
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	25	45	223
Finished of Calibration	25	43	223

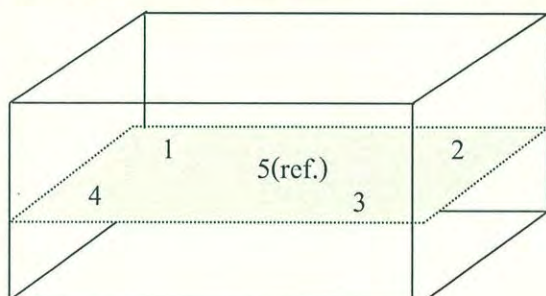

Front

<u>Position :</u>	<u>Ref. Std. S/N.:</u>
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016

*Malu*



Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2304-0253OC-1  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 23TM637

Page : 3 of 3

Calibration point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Average* Standard Reading ( °C )					Uncertainty  ( ± °C )
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.492	44.463	44.475	44.510	44.491	0.15
45.0	45.0	45.0	45.005	44.962	44.979	45.016	44.986	0.15

Calibration point ( °C )	Uniformity ( °C )	Stability ( ± °C )	Coverage Factor <i>k</i>
44.5	0.051	0.022	2
45.0	0.080	0.026	2

**Average\*** : The average of 30 values in each position.

**Uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Stability** : One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1583

Page : 1 of 3

## Certificate of Calibration

**Equipment :** Low Temp. Incubator

**Manufacturer :** ShellLab

**Model :** 2020-2E

**Serial No. :** 0601299

**ID No. :** BKK\_ML0011

**Submitted by :** ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

**Location :** Incubation & Microbiological Reading

**Received Order :** 21 November 2022

**Calibration Date :** 21 November 2022

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Krisda Malee

REVIEW BY	Sithichok
APPROVED BY	
NEXT CAL. DATE	21/05/24

**Approved by :**   
Approved Signatory

- ( ☒ ) Pornthippa Tameyakul  
( ☒ ) Malee Butkruea  
( ☐ ) Suwit Imjai

**Issue Date :** 29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0048153



**Equipment :** Low Temp. Incubator  
**Condition As-Received :** Used Item  
**Reference :** 2211-0623OC-4

**Cert. No.:** 22TM1583  
**Page :** 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1 ) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) After Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Not Available

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	26	24
REL.Humid. ( % )	50	54
AC Supply ( Volt )	219	220

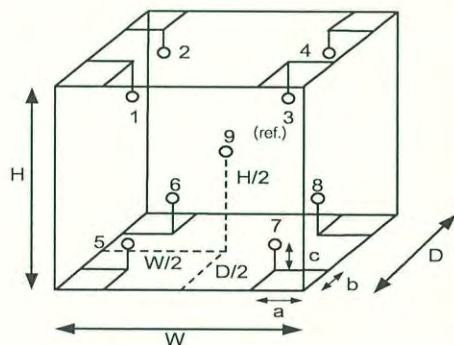

Position :	Ref. Std. ID No.:
1	19-15RTD-01
2	19-15RTD-02
3	19-15RTD-03
4	19-15RTD-04
5	19-15RTD-05
6	21-15RTD-06
7	19-15RTD-07
8	19-15RTD-08
9 (ref.)	19-15RTD-09

**Probe Installation Details :**

a = 5.0 cm  
 b = 5.0 cm  
 c = 5.0 cm

**Dimension of Chamber :**

D = 0.55 m  
 W = 1.2 m  
 H = 0.69 m  
 Capacity = 0.46 m<sup>3</sup>

*Malu*





Equipment : Low Temp. Incubator  
Condition As-Received : Used Item  
Reference : 2211-0623OC-4  
Result of Calibration :- ( \* ) After Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Not Available

Cert. No.: 22TM1583

Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
25.0	25.0	25.0	0.019	0.29	0.34	0.30	2

Calibration Point ( °C )	Measured Temperature ( °C )								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
25.0	25.177	25.199	25.166	25.172	25.027	24.893	25.061	25.152	25.173

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand  
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



## CALIBRATION CERTIFICATE

Issued Date : 8-Jan-2023

Certificate No. : 23TH0050

CSR No. : A047/02339

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd  
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,  
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : Autoclave

Manufacturer : TOMY

Model : SX-700

Serial No. : 52134079

ID No. : SGK\_ML0001

Resolution : 1 °C

Received Date : 5-Jan-2023

Calibrated Date : 5-Jan-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	Nattawut P.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	Jul 05-May-2024

### Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.16.013 based on BS 2646 : 1993 (part 5)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

### Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

  
Kanyarat Chaipet / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.



### Details of Calibration


#### 1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data logger With Sensor	GL220	C90432223	22SDAT005	4-May-2023

- The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.
- This certificate is not certified any commercial transaction
- Condition of Item : normal condition , no indication for any damage or malfunction

**Result of Calibration :** ( ✓ ) Without Adjustment ( ) After Adjustment

#### 1. Sensor Installation Diagram

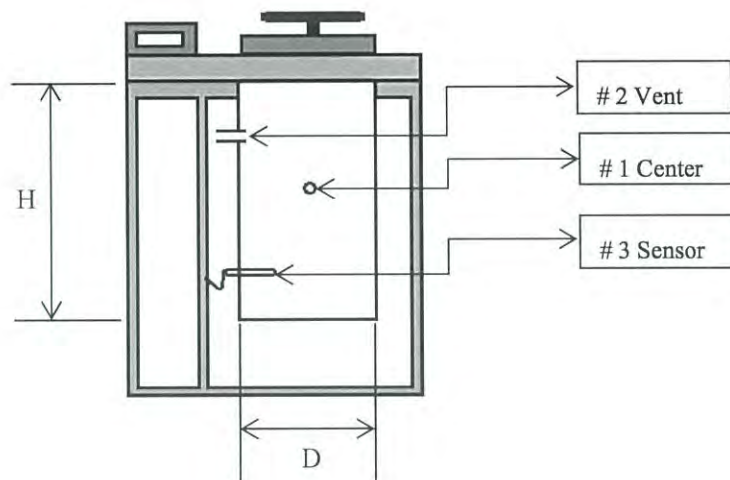

Chamber Diameter (D) : 30 cm

Chamber Height (H) : 70 cm



Certificate No. : 23TH0050

CSR No. : A047/02339

Page. : 3 of 3

### Result of Calibration :

#### 2. Temperature Measurement Accuracy Test

The measurement results of the Autoclave and associates are reported in the manner as shown below

Cal point ( °C )	Measured Standard Temperature At Spread Locations ( °C )			Pressure Reading	Uncertainty ( ± °C )
	Center #1	Vent #2	Sensor #3		
115	115.5	115.4	115.5	0.07 MPa	0.76
118	118.7	118.9	119.1	0.09 MPa	0.76
121	122.0	122.1	122.1	0.11 MPa	0.76

#### 3. Performance Result

The performance of the Autoclave are reported as shown below

Cal point ( °C )	UUC Setting ( °C )	UUC Reading ( °C )	Temperature Stability ( ± °C )	Temperature Uniformity ( °C )	Overall Variation ( °C )
115	115	115	0.20	0.30	0.30
118	118	118	0.70	0.70	0.90
121	121	121	0.50	0.40	0.60

- Operating Time = 1800.65 sec

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

... End ...



**Southern Calibration Service Co., Ltd.**

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand  
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



## CALIBRATION CERTIFICATE

Issued Date : 9-Aug-2022

Certificate No. : 22OV529

CSR No. : A037/01847

Page : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd  
114/1 Moo 8, Kamchanawanich Rd. Tambon, Ban Phru,  
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : Incubator

Manufacturer : Memmert

Model : ICP750

Serial No. : F816.0061

ID No. : SGK\_ML0013

Resolution : 0.1 °C

Received Date : 6-Aug-2022

Calibrated Date : 6-Aug-2022

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	APPROVED BY
APPROVED BY	APPROVED BY
NEXT CAL. DATE	

### Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on G-20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

### Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Kanyarat Chaipet / Technical Manager

**The uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

### Details of Calibration

#### 1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

#### Result of Calibration :

( ☒ ) Without Adjustment

( ☐ ) After Adjustment

#### 1. Sensor Installation Diagram

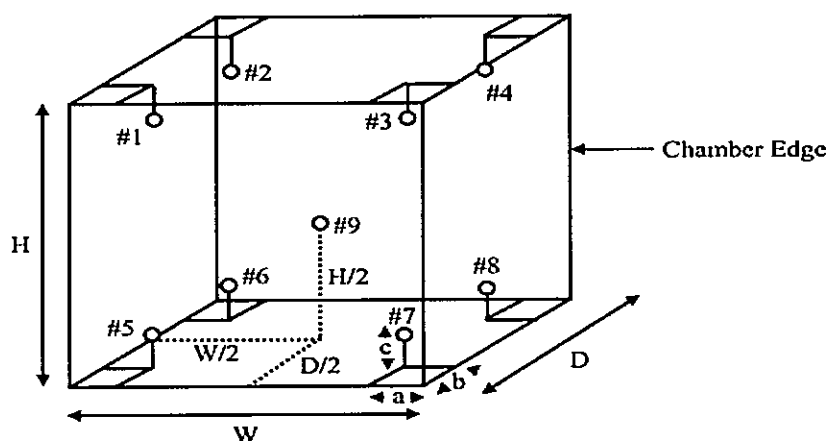

#### Sensor Installation Details

a = 5.0 cm

b = 5.0 cm

c = 5.0 cm

#### Dimension of the chamber

W = 104.0 cm

H = 120.0 cm

D = 60.0 cm



Certificate No. : 22OV529

CSR No. : A037/01847

Page. : 3 of 3

**Result of Calibration .:**

**2. Temperature Measurement Accuracy Test**

The measurement results of the Incubator and associates are reported in the manner as shown below

Cal point ( °C )	Measured Standard Temperature At Spread Locations ( °C )									Uncertainty ( ± °C )
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
35	34.99	34.92	34.95	34.88	34.96	35.00	34.94	34.94	34.94	0.38

**3. Performance Result**

The performance of the Incubator are reported as shown below

Cal point ( °C )	UUC Setting ( °C )	UUC Reading ( °C )	Temperature Stability ( ± °C )	Temperature Uniformity ( °C )	Overall Variation ( °C )
35	35.0	35.0	0.10	0.12	0.19

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

... End ...





Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand  
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



## CALIBRATION CERTIFICATE

Issued Date : 8-Jan-2023

Certificate No. : 23CH0016

CSR No. : A047/02339

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd  
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,  
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : pH meter

Manufacturer : Sartorius

Model : Basic pH Meter PB-10

Serial No. : C70160695

ID No. : SGK\_ML0016

Electrode No. : N/A

Received Date : 5-Jan-2023

Calibrated Date : 5-Jan-2023

Ambient Temperature :  $(25 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 15) \%$

REVIEW BY	Nattawut P.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	05-Jul-24 Nattawut P.

### Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

### Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HACH : HACH LANGE GmbH
- WK : WK Electric Co., Ltd.

Calibrated by : Jessadagon Lemhud

Approved by :

Kanyarat Chaipet / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.



### Details of Calibration

#### 1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.005	C02950	1733	22-Apr-2024
Standard Solution	7.000	C03001	1783	23-Sep-2024
Standard Solution	10.013	C02953	1735	29-Apr-2024
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	5-Jun-2024

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment ( ) After Adjustment

#### 1. Electrical Measurement

Applied Voltage ( mV )	pH meter Reading ( mV )	Correction ( mV )	Uncertainty ( ± mV )
177.48	177.4	0.08	0.17
0.00	0.0	0.00	0.13
-177.48	-177.4	-0.08	0.17

#### 2. Sample Test Measurement

Standard Buffer Solutions ( pH )	pH meter Reading ( pH )	Correction ( pH )	Uncertainty ( ± pH )
4.004	4.02	-0.016	0.011
7.000	7.01	-0.010	0.013
10.013	10.02	-0.007	0.036

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

... End ...



# Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand  
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



## CALIBRATION CERTIFICATE

Issued Date : 2-Feb-2023

Certificate No. : 23TH0521

CSR No. : A075/03704

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd  
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,  
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : Water Bath

Manufacturer : Memmert

Model : WPE45

Serial No. : L716.0558

ID No. : SGK\_ML0021

Resolution : 0.1 °C

Received Date : 30-Jan-2023

Calibrated Date : 30-Jan-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	Nattawut P.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	30-Jul-24

### Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.014 based on ASTM E 715 : 1980 (reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

### Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCAL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

### Details of Calibration

#### 1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

#### Result of Calibration :

( ✓ ) Without Adjustment

( ) After Adjustment

#### 1. Sensor Installation Diagram

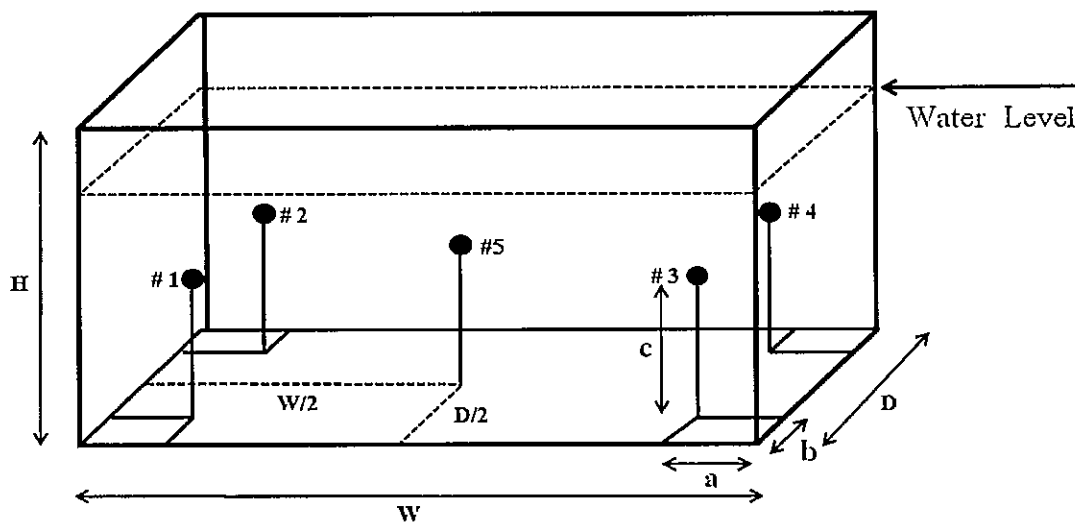

#### Sensor Installation Details

$a = 5$  cm  
 $b = 5$  cm  
 $c = 5$  cm

#### Dimension of the chamber

$W = 45$  cm  
 $H = 30$  cm  
 $D = 35$  cm



Certificate No. : 23TH0521

CSR No. : A075/03704

Page. : 3 of 3

**Result of Calibration :**

**2. Temperature Measurement Accuracy Test**

The measurement results of the Water Bath and associates are reported in the manner as shown below

Cal point ( °C )	Measured Standard Temperature At Spread Locations ( °C )					Uncertainty ( ± °C )
	#1	#2	#3	#4	Ref.5	
44.5	44.47	44.48	44.45	44.51	44.50	0.14

**3. Performance Result**

The performance of the Water Bath are reported as shown below

Cal point ( °C )	UUC Setting ( °C )	UUC Reading ( °C )	Temperature Stability ( ± °C )	Temperature Uniformity ( °C )	Overall Variation ( °C )
44.5	44.5	44.5	0.10	0.24	0.25

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

... End ...



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM75

Page.: 1 of 3

## Certificate of Calibration

Equipment : Incubator  
Manufacturer : Memmert  
Model : ICP 750  
Serial No. : F816.0063  
ID No. : SGK\_CL0028  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
Songkhla Branch.  
114/1 Moo 8, Kanjanavanij Rd., Banphru,  
Hatyai, Songkhla 90250, Thailand  
Location : BOD Room  
Received Order : 24 January 2022  
Calibration Date : 25 January 2022  
Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %  
Calibrated by : Kunchit Promprat

REVIEW BY Ananta B.  
APPROVED BY Kanitta H.  
NEXT CAL. DATE 26/7/23

Approved by : Malee Butkruea  
Approved Signatory

- ( ) Pornthippa Tameyakul  
(✓) Malee Butkruea  
( ) Suwit Imjai

Issue Date : 7 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0037405



Equipment : Incubator  
 Condition As-Received : Used Item  
 Reference : 2201-0617OC-3  
 Procedure Used :-

Cert. No.: 22TM75

Page.: 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34972A	MY57013823	21LM3/1	26 Feb 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

Function of UUC\* : Temperature Source

Fresh air setting : Close

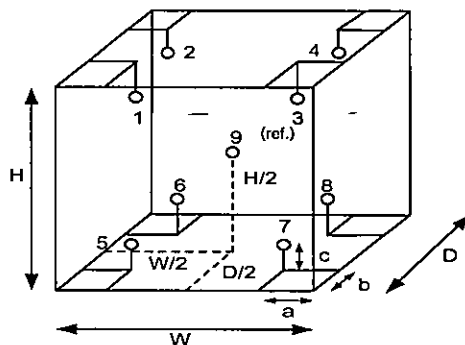

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	28	28
REL.Humid. ( % )	57	52
AC Supply ( Volt )	231	231

**Probe Installation Details :**

a = 10 cm  
 b = 10 cm  
 c = 10 cm

**Dimension of Chamber :**

D = 0.60 m  
 W = 1.0 m  
 H = 1.2 m  
 Capacity = 0.75 m<sup>3</sup>

Position :	Ref. Std. ID No.:
1	21-17RTD-01
2	21-17RTD-02
3	17RTD-03
4	17RTD-04
5	17RTD-05
6	17RTD-06
7	17RTD-07
8	17RTD-08
9 (ref.)	17RTD-09

*Mulu.*





Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2201-0617OC-3  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Close

Cert. No.: 22TM75

Page.: 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
20.0	20.0	20.1	0.094	0.50	0.83	0.30	2

Calibration Point ( °C )	Measured Temperature ( °C )								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
20.0	20.280	20.370	20.363	20.378	19.915	19.925	19.673	19.727	20.098

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

*Mulu .*



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22LM162

Page.: 1 of 2

## Certificate of Calibration

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000

Serial No. : 17B101473

ID No. : SGK\_CL0073

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
Songkhla Branch.  
114/1 Moo 8, Kanjanavanij Rd., Banphru,

Location : TPA Chemistry Calibration Lab.2

Received Order : 18 November 2022

Calibrated Date : 21 November 2022

Ambient Temperature : (  $26 \pm 10$  ) °C

Relative Humidity : (  $50 \pm 30$  ) %

AC Line Voltage : (  $220 \pm 22$  ) V

Calibrated by : Warakorn Lerngagtrakul

REVIEW BY	Ananta B.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	21 Nov 24.

Approved by :

*Malu.*

Approved Signatory

- ( ) Pornthippa Tameyakul  
(✓) Malee Butkruea  
( ) Suwit Imjai

Issue Date :

22 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0047729



Equipment : DO Meter with Sensor  
Condition As-Received : Used Item  
Reference : 2111-0663DSC-2

Cert. No.: 22LM162

Page.: 2 of 2

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer ( IPRT ) into Temperature Bath.

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1523	3240076	221249	02 Mar 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 17B100103

<u>Calibration Point</u> ( °C )	<u>Immersion Depth</u> ( mm )	<u>Standard Temperature</u> ( °C )	<u>UUC* Reading</u> ( °C )	<u>Error</u> ( °C )	<u>Uncertainty</u> ( ± °C )	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.001	19.88	-0.121	0.15	2.00

**UUC\* : Unit Under Calibration**

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Maku-



**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES**

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

**Cert.No.: 22TW259**

**Page.: 1 of 2**

## **Certificate of Testing**

<b>Equipment :</b>	DO Meter
<b>Manufacturer :</b>	YSI
<b>Model :</b>	5000
<b>Serial No. :</b>	17B101473
<b>ID No. :</b>	SGK_CL0073
<b>Received Date :</b>	18 November 2022
<b>Test Date :</b>	21 November 2022
<b>Reference :</b>	2211-0663DSC-1
<b>Submitted by :</b>	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8, Kanjanavanij Rd., Banphru, Hatyai, Songkhla 90250, Thailand
<b>Laboratory Condition :</b>	Temperature ( $25 \pm 5$ ) °C Humidity ( $50 \pm 20$ ) %
<b>Test Procedure :</b>	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
<b>Tested by :</b>	Walalak Sirithean

**Approved by :**

Malee Butkruea  
Approved Signatory

( ☒ ) Malee Butkruea  
( ☐ ) Saithip Meangmai  
( ☐ ) Warakorn Lerngagtrakul

**Issue Date :**

22 November 2022



Cert.No.: 22TW259

Page.: 2 of 2

**Condition of this result of calibration**

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

**Result :** Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 17B100103

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.12	8.12	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

*Malu.*

a 1136621



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CALIBRATION AND TESTING EQUIPMENT SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-24 FAX. 0-2719-9484

Cert.No.: 22CH1137

Page.: 1 of 2

## Certificate of Calibration

Equipment :	Conductivity Meter
Manufacturer :	Mettler Toledo
Model :	Seven2Go S3
Serial No. :	B914464504
ID No. :	SGK_FS0051
Condition As-Received:	Used Item
Received Date :	26 August 2022
Calibration Date :	29 August 2022
Reference :	2208-0961DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru, A.Hat Yai, Songkhla 90250 Thailand
Ambient Temperature :	(25 $\pm$ 2.5) °C
Relative Humidity :	(50 $\pm$ 15) %
Calibration Procedure:	In -house method : - CP-CH6 : based on direct measurement by using certified reference material (CRM)

REVIEW BY	<i>Marakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	29/8/23

Calibrated by : Uthen Kankawi

Approved by :

*Malee*

Approved Signatory

- (☒) Malee Butkruea  
( ) Saithip Meangmai  
( ) Warakorn Lerngagtrakul

Issue Date : 2 September 2022

The Uncertainties are for a confidence probability of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration and Testing Equipment Services.

A 0009518





Cert.No.: 22CH1137

Page.: 2 of 2

**Condition of this result of calibration**

1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	9549224	130RC003	22I484	17 Apr 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials :-

- Conductivity calibration solution, Thermo Scientific (traceable to NIST)

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
84 $\mu\text{S/cm}$	Thermo Scientific	152/02	14 Apr 2023
1413 $\mu\text{S/cm}$	Thermo Scientific	081/02	26 Feb 2024
12.88 mS/cm	Thermo Scientific	041/01	29 Jan 2024

- Control Conductivity calibration solution temperature by Water bath ( $25 \pm 0.1$ )  $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration results**

**Function : Conductivity Measurement**

**(\*) After Adjustment at 1413  $\mu\text{S/cm}$**

**Conductivity Electrode Serial No.: 5819080541**

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement ( $\pm$ )	Coverage factor k
84 $\mu\text{S/cm}$	82.15 $\mu\text{S/cm}$	84.25 $\mu\text{S/cm}$	4.3 $\mu\text{S/cm}$	2.00
1413 $\mu\text{S/cm}$	1374 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	15 $\mu\text{S/cm}$	2.00
12.88 mS/cm	12.51 mS/cm	12.83 mS/cm	0.14 mS/cm	2.00

**Remark** - UUC\* = Unit Under Calibration

- Cell constant =  $0.548 \text{ cm}^{-1}$

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

Malu.

**Sartorius (Thailand) Co., Ltd.**

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com

**SARTORIUS**

# Certificate

## of Calibration

REVIEW BY Ananta B.  
APPROVED BY Kanitta H.  
NEXT CAL. DATE 25/1/23/24

Model Number : MSE224S-100-DUCertificate No. : 23BCI0044Description : Analytical BalanceIssued Date : Friday, January 27, 2023Serial Number : 0034705158Reference No. : 202361ID No. : SGK\_CL0045Manufacturer : SartoriusPage No. : 1 of 2Customer Name : ALS Laboratory Group (Thailand) Co., Ltd.Songkhla Branch: 114/1 Moo 8 Karnchanawanich Rd., T. Ban Phru, A. Hat Yai, Songkhla. 90250.Calibrated Place : Balance Room.Calibrated By : Mr. Chonchai InthanaCalibration Date : Wednesday, January 25, 2023

Calibration

Procedure No. : This calibration was conducted byUsing in-house calibration procedure number (WI-003)Based on UKAS LAB 14 : 2019

Metrological data :

Capacity : 220 g Readability : 0.0001 g

Ambients Conditions:

Temperature : 22.4 °C ± 3.0 °CHumidity : 65.0 % RH ± 5.0 % RHPressure :                      ±                     

Reasons for calibration

☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ MaintenanceEquipment Condition: ☒ Good Operate ☐ Fair

### Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

### Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 1kg E2 s/n 37929119	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division  
Sartorius (Thailand) Co., Ltd.

Mr. Chonchai Inthana (Technical Manager)

S  
T  
A  
M  
P

# Certificate of Calibration

Model Number : MSE224S-100-DU

Certificate No. : 23BCI0044

Description : Analytical Balance

Issued Date : Friday, January 27, 2023

Serial Number : 0034705158

Reference No. : 202361

ID No. SGK\_CL0045

Manufacturer : Sartorius

Page No. : 2 of 2

## Calibration Results : Without Adjustment

### Repeatability



The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0001	200.0000
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0000
	20.0000	200.0001
Nominal Value : (High Load)	20.0000	200.0000
200 g	20.0000	200.0001
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0001
	20.0000	200.0001
<b>Standard Deviation</b>	0.00003	0.00005

### Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 50 g  
Tolerance 0.0004 g



	Difference
1	—
2	0.0001
3	0.0000
4	0.0000
5	0.0000
6	—

### Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00013
0.1	0.1000	0.1000	0.0000	0.00013
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	200.0001	0.0001	0.00030

End of Report.



**Southern Calibration Service Co., Ltd.**

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand  
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



## CALIBRATION CERTIFICATE

Issued Date : 1-May-2023

Certificate No. : 23TH1728

CSR No. : A088/04367

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd  
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,  
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : Hot Air Oven

Manufacturer : Memmert

Model : UF110

Serial No. : B416.3387

ID No. : SGK\_CL0024

Resolution : 0.1 °C

Received Date : 28-Apr-2023

Calibrated Date : 28-Apr-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	..... Ananta B. ....
APPROVED BY	..... Kanitta H. .... 10
NEXT CAL. DATE	..... 28/11/2024 .... 10

### Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

### Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

**The uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

### Details of Calibration

#### 1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

#### Result of Calibration .:

( ☒ ) Without Adjustment

( ☐ ) After Adjustment

#### 1. Sensor Installation Diagram

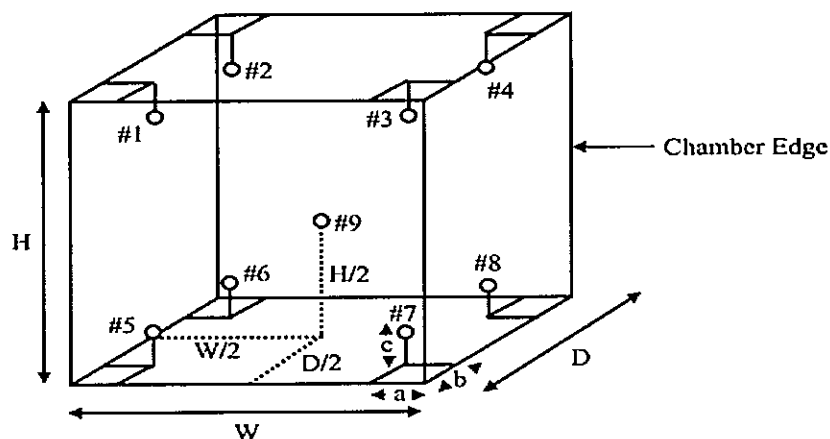

#### Sensor Installation Details

a = 5.0 cm

b = 5.0 cm

c = 5.0 cm

#### Dimension of the chamber

W = 40.0 cm

H = 40.0 cm

D = 33.0 cm

## Result of Calibration :

### 2. Temperature Measurement Accuracy Test

The measurement results of the Hot Air Oven and associates are reported in the manner as shown below

Cal point ( °C )	Measured Standard Temperature At Spread Locations ( °C )									Uncertainty ( ± °C )
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
40	40.48	40.28	40.28	39.91	40.17	40.09	39.93	40.27	39.89	0.36
70	70.36	70.23	70.58	69.74	69.99	69.92	69.86	70.13	70.04	0.36
103	103.19	103.12	103.46	103.37	103.10	103.54	103.43	103.06	103.40	0.36
104	104.31	104.23	104.62	103.77	104.12	104.06	103.90	104.20	104.56	0.36
105	105.07	105.03	105.48	105.27	105.12	105.01	105.01	105.00	104.96	0.36
180	180.31	180.00	180.00	180.07	180.18	180.05	180.01	180.10	180.24	0.41

### 3. Performance Result

The performance of the Hot Air Oven are reported as shown below

Cal point ( °C )	UUC Setting ( °C )	UUC Reading ( °C )	Temperature Stability ( ± °C )	Temperature Uniformity ( °C )	Overall Variation ( °C )
40	40.0	40.0	0.20	0.70	0.72
70	70.0	70.0	0.20	0.60	0.94
103	103.0	103.0	0.20	0.43	0.54
104	104.0	104.0	0.10	0.79	0.88
105	105.0	105.0	0.10	0.59	0.69
180	180.0	180.0	0.10	0.38	0.38

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

... End ...





# Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkhla 90250 Thailand

Tel: 081 599 0417 Fax: 074 805 133 Email: s.calibration@gmail.com www.scal-lab.com



## CALIBRATION CERTIFICATE

Issued Date : 8-Feb-2022

Certificate No. : 22WB004

CSR No. : A0223/01123

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd  
114/1 Moo 8 Karnchanawanich Rd. T.Ban Phru,  
A. Hat Yai, Songkhla 90250 TH

Calibration Place : Chemical Laboratory  
Instrument Name : Water Bath  
Manufacturer : Memmert  
Model : WNE29  
Serial No. : L616.0538  
ID No. : SGK\_CL0035  
Resolution : 0.1 °C  
Received Date : 5-Feb-2022  
Calibrated Date : 5-Feb-2022  
Ambient Temperature : (30 ± 10) °C  
Relative Humidity : (50 ± 30) %

REVIEW BY	Ananta B.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	6/07/2023

### Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.W1.014 based on ASTM E 715 : 1980 (reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

### Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Imron Rattanaylum

Approved by :

Sakeereen Heemhad / Technical Manager

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

### Details of Calibration

#### 1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data logger With Sensor	34970A	MY44064411	QR21-0314	9-Feb-2022

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

### Result of Calibration :

(✓) Without Adjustment

( ) After Adjustment

#### 1. Sensor Installation Diagram

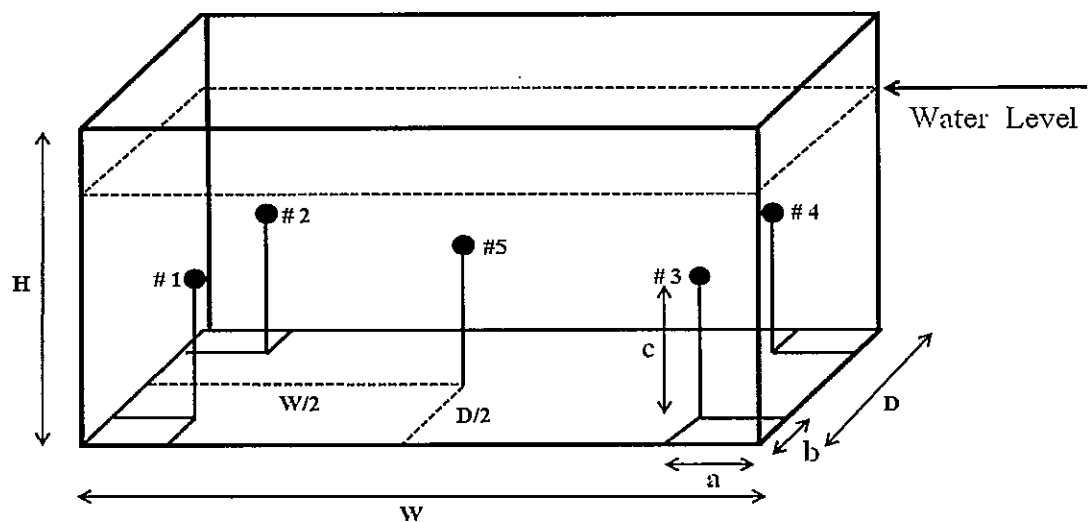

#### Sensor Installation Details

a = 5 cm  
b = 5 cm  
c = 5 cm

#### Dimension of the chamber

W = 45 cm  
H = 30 cm  
D = 35 cm

**Result of Calibration .:**

**2. Temperature Measurement Accuracy Test**

The measurement results of the Water Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (±°C)
	#1	#2	#3	#4	Ref.5	
80	79.95	80.07	79.95	79.99	80.03	0.14

**3. Performance Result**

The performance of the Water Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
80	81.0	81.0	0.10	0.19	0.19

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

... End ...



**Southern Calibration Service Co., Ltd.**

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand  
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.seal-lab.com



## CALIBRATION CERTIFICATE

Issued Date : 1-May-2023

Certificate No. : 23CH0203

CSR No. : A088/04367

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd  
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,  
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : pH meter

Manufacturer : Mettler Toledo

Model : S220

Serial No. : B625631849

ID No. : SGK\_CL0030

Electrode No. : 1204613

Received Date : 28-Apr-2023

Calibrated Date : 28-Apr-2023

Ambient Temperature : (25 ± 3) °C

Relative Humidity : (55 ± 15) %

REVIEW BY	Ananta B.
APPROVED BY	Kamrta H.
NEXT CAL. DATE	28 / 10 / 2024

### Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

### Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HACH : HACH LANGE GmbH

- SCaL : Sounthern Calibration Service Co., Ltd.,

- WK : WK Electric Co., Ltd.

Calibrated by : Alisara Ma

Approved by :

Imron Rattanaylum / Technical Manager

**The uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

**Details of Calibration****1. Reference Standard Equipment Used:**

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.005	C02994	1777	5-Sep-2024
Standard Solution	7.000	C03007	1787	17-Oct-2024
Standard Solution	10.012	C02953	1735	29-Apr-2024
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	5-Jun-2024
Digital Thermometer With Sensor	DP-77	I.360896	22SDTH005	8-Aug-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

**Result of Calibration :****1. Electrical Measurement**

Applied Voltage ( mV )	pH meter Reading		Correction ( mV )	Uncertainty ( ± mV )
	( mV )	( pH )		
177.48	177.5	3.70	-0.02	0.17
0.00	0.0	6.70	0.00	0.13
-177.48	-177.4	9.80	-0.08	0.17

**2. Before Sample Test Measurement**

Standard Buffer Solutions ( pH )	pH meter Reading		Correction ( pH )	Uncertainty ( ± pH )
	( pH )	( mV )		
4.005	3.97	159.2	0.035	0.0090
6.999	6.98	-15.4	0.019	0.013
10.012	9.95	-188.0	0.062	0.036

**3. After Sample Test Measurement**

Standard Buffer Solutions ( pH )	pH meter Reading		Correction ( pH )	Uncertainty ( ± pH )
	( pH )	( mV )		
4.005	3.97	158.9	0.035	0.0090
6.999	7.01	-17.5	-0.011	0.013
10.012	9.98	-187.6	0.032	0.036

**4. Temperature Measurement**

Cal Point ( °C )	Standard Temperature ( °C )	UUC Reading ( °C )	Correction ( °C )	Uncertainty ( ± °C )
25	25.032	25.1	-0.068	0.11

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

... End ...



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484




Cert.No.: 23CH131

Page.: 1 of 3

## Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	Seven2Go S2
Serial No. :	B728378040
ID No. :	SRT_MKT0001
Condition As-Received:	Used Item
Received Date :	31 January 2023
Calibration Date :	01 February 2023
Reference :	2301-1029DSC-12
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer

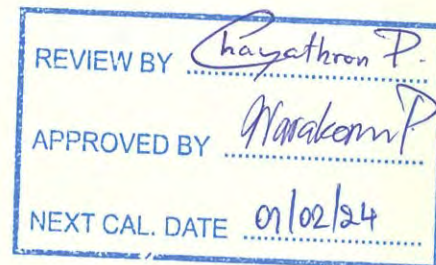

Calibrated by : Warakorn Lernagtrakul

Approved by :

*Malee*

Approved Signatory

- ( / ) Malee Butkruea  
( ) Saithip Meangmai  
( ) Warakorn Lernagtrakul

Issue Date : 3 February 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0050482





Cert.No.: 23CH131

Page.: 2 of 3

**Condition of this calibration result**

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	22E2769	24 Aug 2023
2) Ref. Standard Thermometer	4982054	110RC044	22I1306	27 Oct 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	826588	09 July 2024
pH 6.987	CPA chem	826589	09 July 2023
pH 10.008	CPA chem	826590	09 July 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results**

**Function : mV Measurement**

**Performing standard curve by Fluke at pH (4,7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( ±mV )	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: B728378040	4.00	177.48	178	4.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-178	10.00	0.58	2.00

*Malu*



Cert.No.: 23CH131

Page.: 3 of 3

**Calibration Results****Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading ( mV )	Uncertainty of pH measurement ( $\pm$ )	Coverage factor $k$
pH Electrode S/N.: 1033814	4.008	4.01	162	0.0085	2.05
	6.987	6.99	-14	0.011	2.00
	10.008	10.01	-189	0.0092	2.00

**Function : Temperature Measurement****( \* ) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : InLab Expert Go-ISM  
- Serial No. : 1033814

Dimension of probe;

- Length : 120 mm.  
- Diameter : 12 mm.  
- Immersion Depth : 100 mm.

Calibration Point ( $^{\circ}\text{C}$ )	Standard Temperature ( $^{\circ}\text{C}$ )	UUC* Reading ( $^{\circ}\text{C}$ )	Error ( $^{\circ}\text{C}$ )	Uncertainty of measurement ( $\pm$ $^{\circ}\text{C}$ )	Coverage factor $k$
25.0	25.002	25.2	0.198	0.13	2.00
30.0	30.003	30.3	0.297	0.13	2.00
45.0	45.002	45.3	0.298	0.13	2.00

**Remark : - UUC\* = Unit Under Calibration**

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

Malu



## Internal Calibration

REVIEWED BY	Somsak J.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	20/06/23

Equipment :	<u>Turbidity Meter</u>	Manufacture :	<u>HACH</u>
ID No. :	<u>SGK_FS0045</u>	Model :	<u>2100Q/QIS</u>
Calibrate Date :	<u>June 20, 2022</u>	Serial No. :	<u>19010C073443</u>

Calibration Point	1st (NTU)	2nd (NTU)	3rd (NTU)	AVG (NTU)	Specifications	Evaluate
Standard 20 NTU	20.0	20.2	20.1	20.1	19 to 21 NTU	Pass
Standard 100 NTU	99.6	99.8	99.8	99.7	95 to 105 NTU	Pass
Standard 800 NTU	791.0	793.0	794.0	792.7	760 to 840 NTU	Pass

Calibrated by Somsak J.  
( Scientist 2 )

Approved by : Kanitta H.  
( Section Head )

# Certificate of Analysis List

For request number 1568060

Catalog Number Entered	Lot Number Entered	Related Catalog Number	Related Lot Code	Description
2660501 STANDARD	1236R 800 NTU	2659405-TH	1291	STABLCAL sup TS sup0 FORMAZIN
2684701	1284	2659405-TH	1291	<0.1 NTU Calibration Solution
2684801 STANDARD	1265 20 NTU	2659405-TH	1291	STABLCAL sup TS sup0 FORMAZIN
2684901 STANDARD	1246 100 NTU	2659405-TH	1291	STABLCAL sup TS sup0 FORMAZIN

Total Enclosures: 4



An ISO 9001 Certified Company

***Certificate of Analysis******This is a Component of 2659405-TH lot A1291***

Page 1

COMMODITY: &lt;0.1 NTU Calibration Solution

COMMODITY NUMBER: 2684701

MANUFACTURE DATE:

DATE OF ANALYSIS:

LOT NUMBER: A1284

10/21/2021

10/22/2021

---

<b><i>TEST</i></b>	<b><i>SPECIFICATIONS</i></b>	<b><i>RESULTS</i></b>
Turbidity	0 to 0.1 NTU	0.06 NTU

The expiration date is Jan 2023

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NI does not carry turbidity standards. However, the use of Formazin and StablCal® as used in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

Certified by

---

Scott Als  
Analytical Services Chemist



An ISO 9001 Certified Company

***Certificate of Analysis******This is a Component of 2659405-TH lot A1291***

Page 1

COMMODITY: **STABLCAL|sup|TS|sup0 FORMAZIN STANDARD 20 NTU**  
COMMODITY NUMBER: **2684801** MANUFACTURE DATE: DATE OF ANALYSIS:  
LOT NUMBER: **A1265** 10/21/2021 10/28/2021

---

<b><i>TEST</i></b>	<b><i>SPECIFICATIONS</i></b>	<b><i>RESULTS</i></b>
Turbidity	19 to 21 NTU	20.4 NTU

The expiration date is Jan 2023

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NI does not carry turbidity standards. However, the use of Formazin and StablCal® as us in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

Certified by \_\_\_\_\_

Scott Als  
Analytical Services Chemist





An ISO 9001 Certified Company

***Certificate of Analysis******This is a Component of 2659405-TH lot A1291***

Page 1

COMMODITY: **STABLCAL|sup|TS|sup0 FORMAZIN STANDARD 100 NTU**  
COMMODITY NUMBER: **2684901** MANUFACTURE DATE: DATE OF ANALYSIS:  
LOT NUMBER: **A1246** 11/5/2021 11/11/2021

---

<b><i>TEST</i></b>	<b><i>SPECIFICATIONS</i></b>	<b><i>RESULTS</i></b>
Turbidity	95 to 105 NTU	103.0 NTU

The expiration date is Feb 2023

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NI does not carry turbidity standards. However, the use of Formazin and StablCal® as used in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

Certified by

---

Scott Als  
Analytical Services Chemist



An ISO 9001 Certified Company

***Certificate of Analysis******This is a Component of 2659405-TH lot A1291***

Page 1

COMMODITY: STABLCAL|sup|TS|sup0 FORMAZIN STANDARD 800 NTU

COMMODITY NUMBER: 2660501

MANUFACTURE DATE:

DATE OF ANALYSIS:

LOT NUMBER: A1236R

9/10/2021

9/10/2021

---

<b><i>TEST</i></b>	<b><i>SPECIFICATIONS</i></b>	<b><i>RESULTS</i></b>
Turbidity	760 to 840 NTU	819.0 NTU

The expiration date is Jan 2023

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NI does not carry turbidity standards. However, the use of Formazin and StablCal® as used in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

Certified by

---

Scott Als  
Analytical Services Chemist

REVIEW BY Aulcharawan S.APPROVED BY Sararat M.NEXT CAL. DATE 12 Jan 24

## Certificate of Calibration

### ICS-2100: Anion (ID#659)

This certificate is to verify that instrument below are calibrated  
by Archemica Lab Co., Ltd.

ICS-2100 S/N: 15010977

AS-HV S/N: 5450A36659

For

**ALS Laboratory Group (Thailand) Co., Ltd.**



Operator Signature: Nutdanai

Date: Jan 12, 2023

(Mr.Nutdanai Laekhwan)

Application Chemist


**CALIBRATION REPORT**

REVIEW BY Vichuta N.  
APPROVED BY Sararat M.  
NEXT CAL. DATE 9/2/67

CUSTOMER NAME : ALS Laboratory Group (Thailand) Co., Ltd.	
EQUIPMENT NAME : Total Hydrocarbon Analyzer	
MANUFACTURER : Baseline	MODEL : 9000 NMHC SERIAL NO : 0314DR0170
STANDARD GAS CONCENTRATION (PPM) : 100 PPM (Methane)	
CYLINDER PRESSURE (psig) : 900 PSI	CERTIFIED DATE : 12/02/2022
CERTIFIED BY : AIRGAS	EXPIRED DATE : 12/02/2025

**CALIBRATION RESULTS**

POINT NO	CALIBRATION RESULTS			
	IDEAL	ACTUAL	ERROR	%ERROR
ZERO	0.00	0.00	0.00	-
1	100.00	101.00	1.0	-1.00
AVERAGE (%)				0.25

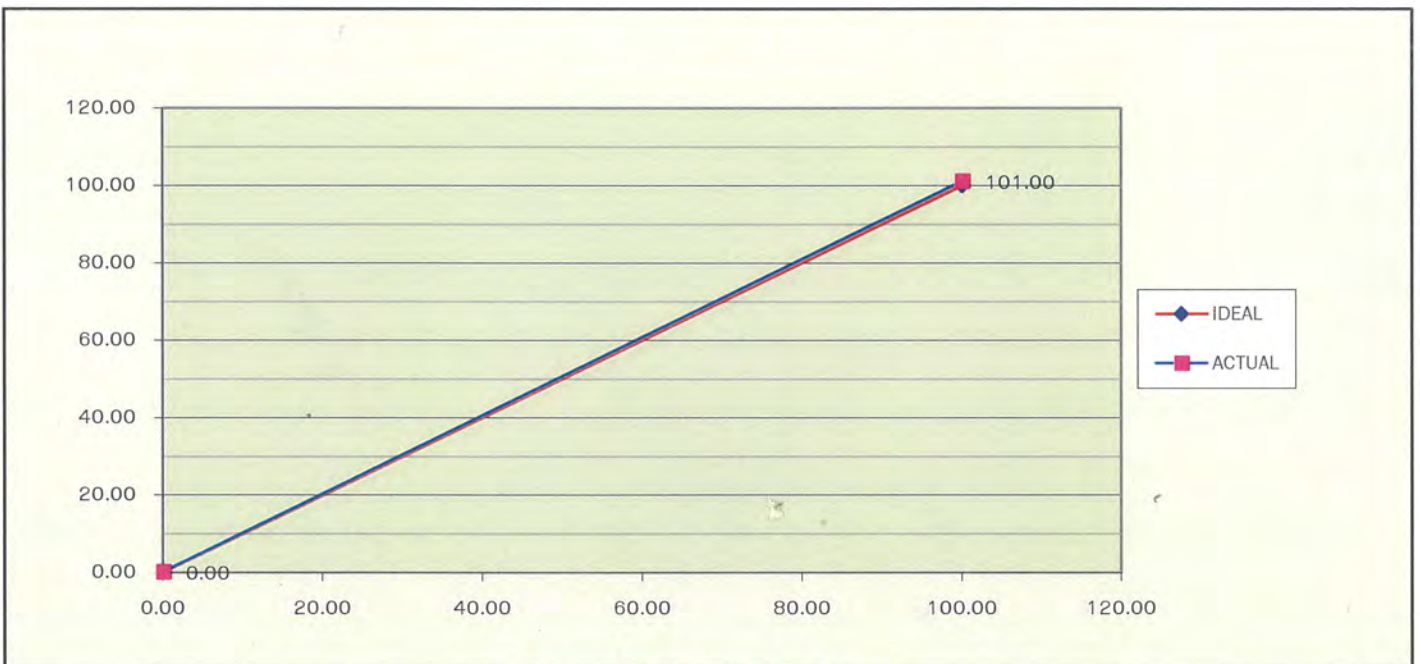

CALIBRATED BY : วิภาพล ดุสิตเจริญ

DATE : 9/8/65

CHECKED BY : ศุภชัย อังคาร

DATE : 9/8/65



ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 31 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ถนน เพชรเกษม 7,7/1 แขวง วัดท่าพระ เขต บางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02868-1889




**CALIBRATION REPORT**

<b>CUSTOMER NAME :</b> ALS Laboratory Group (Thailand) Co., Ltd.	
<b>EQUIPMENT NAME :</b> Total Hydrocarbon Analyzer	
<b>MANUFACTURER :</b> Baseline	<b>MODEL :</b> 9000 NMHC
<b>SERIAL NO :</b> 0314DR0170	
<b>STANDARD GAS CONCENTRATION (PPM) :</b> 100 PPM ( Propane )	
<b>CYLINDER NO :</b> ND55981	
<b>CYLINDER PRESSURE (psig) :</b> 900 PSI	
<b>CERTIFIED DATE :</b> 12/02/2022	
<b>CERTIFIED BY :</b> AIRGAS	
<b>EXPIRED DATE :</b> 12/02/2025	

**CALIBRATION RESULTS**

POINT NO	CALIBRATION RESULTS			
	IDEAL	ACTUAL	ERROR	%ERROR
<b>ZERO</b>	0.00	0.00	0.00	-
<b>1</b>	300.00	301.00	1.0	0.33
<b>AVERAGE (%)</b>				0.08

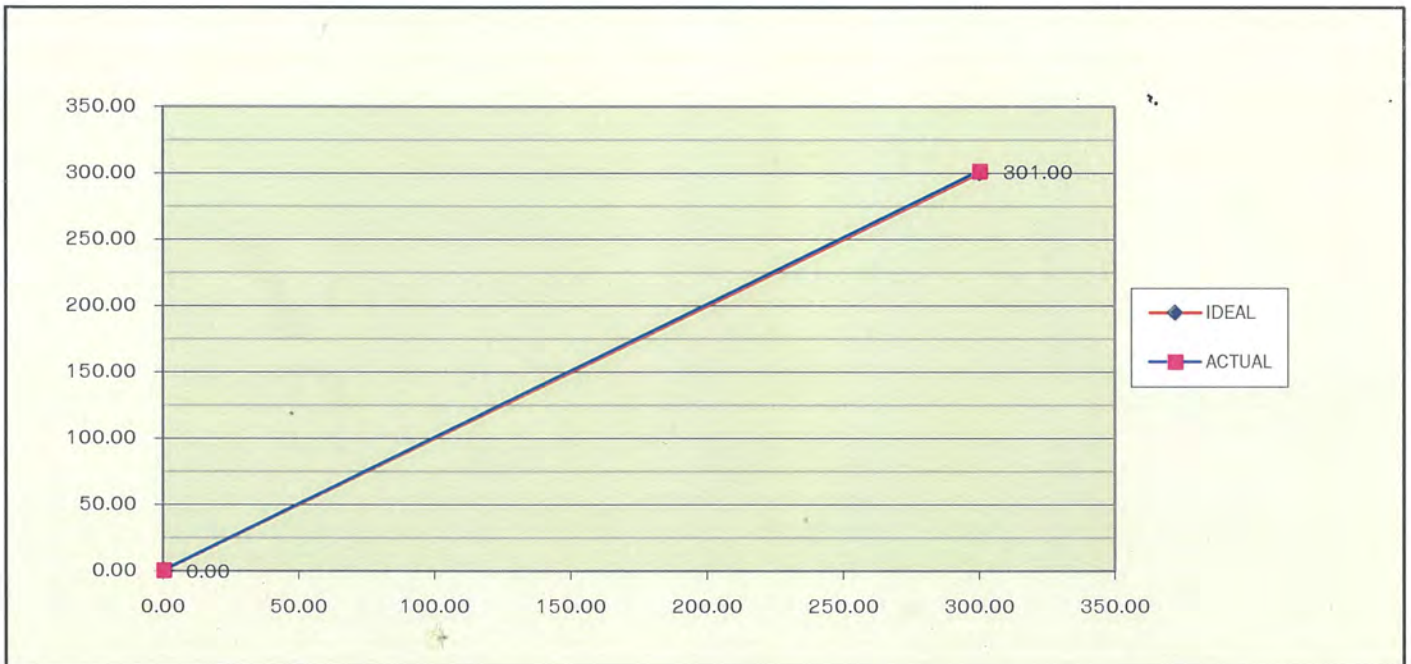

**CALIBRATED BY :** วรณล ศักดิ์เจริญ **DATE :** 9/8/65

**CHECKED BY :** ศิษฐ์ วัฒนา **DATE :** 9/8/65



ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 31 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ถนนเพชรเกษม 7,7/1 แขวง วัดท่าพระ เขต บางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02868-1889

**FLOW CALIBRATE**

CUSTOMER NAME	:	ALS Laboratory Group (Thailand) Co., Ltd.		
EQRIPMENT NAME	:	Flow Calibrator		
MANUFACTURER	:	Bios	MODEL : 510 L	SERIAL NO : 129549

Flow Parameter	Step	Set	Display	Flow Meter
Sample	Before	40	38	15 cc/min
	After	40	40	39.7 cc/min
Air	Before	175	175	190 cc/min
	After	175	175	176 cc/min
Fuel	Before	35	32	36 cc/min
	After	35	35	35 cc/min

**CALIBRATED BY :** วราพล ดวกิ่งเจริญ **DATE :** 9/8/65  
**CHECKED BY :** สันติ วัฒนะ **DATE :** 9/8/65



ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com  
 เลขที่ 63/14-15,67/35-36 ถนน เพชรเกษม 7,7/1 แขวง วัดท่าพระ เขต บางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02868-1889





# บริษัท เอกเสคคิวทิฟ เทรดดิ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230  
TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

ที่ RA 013/22

## ใบรายงานผลการปรับเทียบ

ชื่อผู้ขอรับบริการ : บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด.  
ที่อยู่ : 104 ซ.พัฒนาการ 40 ถ.พัฒนาการ แขวงสวนหลวง เขตสวนหลวง กรุงเทพมหานคร 10250.  
ปรับเทียบที่ : บริษัท เอกเสคคิวทิฟ เทรดดิ้ง จำกัด  
ที่อยู่ : 48/194-5 ซอย ประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวง/เขตลาดพร้าว กรุงเทพฯ 10230

### รายละเอียดเครื่องมือที่ทำการปรับเทียบ :

เครื่องมือ : เครื่องตรวจวัดไอระเหยจากสารเคมี  
ผลิตภัณฑ์ : RAE Systems  
รุ่น : MiniRAE3000  
หมายเลขเครื่อง : 592-906493  
ID : BKK\_FS0819

### สภาวะแวดล้อม :

อุณหภูมิ :  $(25 \pm 3) ^\circ\text{C}$   
ความชื้นสัมพัทธ์ :  $(36 \pm 15) \%$   
ความดันบรรยากาศ : 760 มิลลิเมตรปรอท

REVIEW BY Makom P.  
APPROVED BY [Signature]  
NEXT CAL. DATE 5/8/23

วันที่ปรับเทียบมาตรฐาน : 4 กุมภาพันธ์ 2565

วิธีการปรับเทียบมาตรฐาน : ปรับเทียบโดยใช้ Standard Reference Gas ผลิตภัณฑ์ GASCO  
- Isobutylene Standard Gas 100 ppm; Lot number: 304-402089381-1.

### ผลการปรับเทียบมาตรฐาน

Sensor Type	Reference Concentration	Before Cal.	After Cal.	Error Reading	Result
PID	0.0 ppm (Air Zero)	0.0 ppm	0.0 ppm	0.0 ppm	Pass
PID	100 ppm (Isobutylene)	54.1 ppm	100.0 ppm	0.0 ppm	Pass

Flow Rate of Pump : 490 cc/min.

Accuracy :  $\pm 2 \%$  at calibration point

ผู้ปรับเทียบ : [Signature]  
(นายสุรินทร์ สายเนตร)  
Service Engineer

ผู้ตรวจสอบ : [Signature]  
(นายสุทธิวงศ์ คงทองสังข์)  
Service Engineer Manager

ผลการสอบเทียบ/ปรับเทียบ นี้ รับรองเฉพาะตัวอย่างและรายการที่ได้รับไว้เท่านั้น

การนำรายงานผล/ใบรับรองนี้ไปโฆษณาและการคัดลอกหรือการนำผลบางส่วนไปเผยแพร่ต่อสาธารณะต้องได้รับอนุญาตเป็นลายลักษณ์อักษรจากทางบริษัทฯ



บริษัท เอกเสคคิวทิฟเทรดดิ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230  
TEL.(662) 515-0145-50 FAX.(662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

No. RA 013/22

## Certificate of Calibration

**Customer** : ALS Laboratory Group (Thailand) Co.,Ltd.  
**Address** : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang Bangkok 10250 TH.  
**Calibration location** : Executive Trading Limited.  
**Address** : 48/194-5 Soi Praditmanutham 19, Pradit Manutham Road, Latphrao, Bangkok 10230  
**Tools :**  
Instrument : Gas Detector  
Product : RAE Systems  
Model Name : MiniRAE3000  
Serial Number : 592-906493  
ID : BKK\_FS0819  
**Environmental Condition :**  
Temperature :  $(25 \pm 3) ^\circ\text{C}$   
Relative Humidity :  $(36 \pm 15) \%$   
Pressure : 760 mmHg  
**Date of Calibration** : February 4, 2022  
**Calibration Method** : This instrument has been calibrated using calibration gases. Test and calibration data is On file with Executive trading limited.  
**Reference Standard** : Isobutylene Standard Gas 100 ppm; Lot number: 304-402089381-1.

### Test Result

Sensor Type	Reference Concentration	Before Cal.	After Cal.	Error Reading	Result
PID	0.0 ppm (Air Zero)	0.0 ppm	0.0 ppm	0.0 ppm	Pass
PID	100 ppm (Isobutylene)	54.1 ppm	100.0 ppm	0.0 ppm	Pass

**Flow Rate of Pump** : 490 cc/min.

**Accuracy** :  $\pm 2 \%$  at calibration point

Calibrated By : Surinthorn S.  
(Mr. Surinthorn Sainate)  
Service Engineer

Approved By : Suttawong Kongtongsang  
(Mr. Suttawong Kongtongsang.)  
Service Engineer Manager

The results relate only to the items tested or calibrated.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the company.





บริษัท เอกเสคคิวทิฟ เทรดดิ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230  
TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

ที่ RA 013/22

ใบรายงานการตรวจเช็คเครื่องตรวจวัดก๊าซ รุ่น MiniRAE3000

หมายเลขเครื่อง : 592-906493

วันที่ตรวจเช็ค : 4 กุมภาพันธ์ 2565

ลำดับที่	รายละเอียด การตรวจสอบ	RAW COUNT		สรุป	หมายเหตุ
		REF.	REAL		
1.	PID RAW COUNT				
	Ch.H	10000-62500	39643	■ YES □ NO	
	Ch.L	<62500	29542	■ YES □ NO	
2.	Lamp	>40	45	■ YES □ NO	

ลำดับที่	รายละเอียด การตรวจซ่อม	การแก้ไข	สรุป	หมายเหตุ
1.	Motor Pump	Check flow rate	■ YES □ NO	490 cc/min.
2.	Buzzer	-	■ YES □ NO	-
3.	Li-ion Battery	-	■ YES □ NO	-
4.	Key Pad			
	Y/+	-	■ YES □ NO	-
	N/-	-	■ YES □ NO	-
	MODE	-	■ YES □ NO	-
5.	LCD Display	-	■ YES □ NO	-
6.	THP sensor	-	■ YES □ NO	-
7.	Light Sensor	-	■ YES □ NO	-
8.	Pocket Clip	-	□ YES □ NO	-
9.	PC Port	-	■ YES □ NO	-
10.	Slim Rubber Boot	-	■ YES □ NO	เปลี่ยนใหม่

ผู้ตรวจเช็ค : สุรินทร์ สายเนตร  
(นายสุรินทร์ สายเนตร)  
Service Engineer

ผลการสอบเทียบ/ปรับเทียบ นี้ รับรองเฉพาะตัวอย่างและรายการที่ได้รับอนุญาตไว้เท่านั้น

การนำรายงานผล/ใบรับรองนี้ไปโฆษณาและการคัดลอกหรือการนำผลบางส่วนไปเผยแพร่ต่อสาธารณะต้องได้รับอนุญาตเป็นลายลักษณ์อักษรจากทางบริษัทฯ



**GASCO AFFILIATES, LLC.**

320 Scarlet Blvd.  
Oldsmar, FL 34677  
(800) 910-0051  
fax: (866) 755-8920  
www.gascogas.com

## **CERTIFICATE OF ANALYSIS**

**Date:** May 14, 2021  
**Order Number:** 58376  
**Lot Number:** 304-402089381-1

**Customer:** R C Systems Co Inc  
**Use Before:** 05/14/2025


<u><b>Component</b></u>	<u><b>Requested Concentration</b></u>	<u><b>Analytical Result (+/- 2%)</b></u>
Isobutylene	100 PPM	101.2 PPM
Air	Balance	Balance

**Cylinder Size:** 3.70 Cu. Ft.  
**Contents:** 105 Liter

**Valve:** 5/8"-18 UNF  
**Pressure:** 1200 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/ or N.I.S.T. Gas Mixture reference materials.

**Analyst:**

  
Brandon Brewer



# CERTIFICATE Of Attendance

It is hereby certified that

**Mr Suttiwong Kongthongsang**  
**(Executive Trading Limited)**

has attended the

**RAE Products & Maintenance Training Course**

Conducted by

**RAE Systems BY HONEYWELL**

on **31<sup>st</sup> July to 2<sup>nd</sup> August 2018**

A handwritten signature in blue ink, appearing to be "Desmond Tan".



Conducted by : Desmond Tan  
Service Engineer/Technical Trainer  
Date of Issue : 2<sup>nd</sup> August 2018  
Valid for 2 years from date of issue





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.

REVIEW BY	Mmakorn P
APPROVED BY	[Signature]
NEXT CAL DATE	13/4/24

Certificate Number

CL-007-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Cup anemometer  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 110-WS-25DL-D  
**SERIAL NUMBER** : Sensor: WSD-012  
Data logger: A5791  
**ID NUMBER** : SGK\_FS0088  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) co., ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 10 Jan 2023  
**MEASUREMENT DATE** : 13 Jan 2023  
**ISSUE DATE** : 13 Jan 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

<b>CALIBRATION CONDITIONS</b>	: Wind tunnel cross-section area <sup>1</sup>	900	cm <sup>2</sup>
	Win direction frontal area <sup>2</sup>	100	cm <sup>2</sup>
	Diameter of mounting pipe <sup>3</sup>	-	mm
	Blockage ratio of test object <sup>4</sup>	0.111	[-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (23.4) °C, (46.3) %RH and (1011.3) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jittraporn Lertsomphol



Approved signatory: .....

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>

### Calibration procedure:

The cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm<sup>2</sup> cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

### Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0052-21 and MW-0066-22

### Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'



**MEASUREMENT RESULTS<sup>5</sup>**

The cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle, UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.


$v_{std}^6$ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	$v_{uuc}^7$ (m/s)	Error (m/s)	$U (k=2)$ (m/s)
0.981	23.64	23.35	0.8	-0.2	0.15
2.041	23.10	23.35	1.8	-0.2	0.16
3.049	23.68	23.35	2.8	-0.2	0.18
4.138	23.12	23.35	3.8	-0.3	0.20
5.00	23.72	23.35	4.8	-0.2	0.19
5.98	23.16	23.35	5.8	-0.2	0.19
7.04	23.66	23.35	6.8	-0.2	0.18
8.16	23.18	23.35	7.8	-0.3	0.18
9.09	23.52	23.35	8.8	-0.3	0.20
10.07	23.42	23.35	9.8	-0.3	0.23
11.15	23.50	23.35	10.8	-0.3	0.22
12.13	23.50	23.35	11.8	-0.3	0.22
13.20	23.58	23.35	12.8	-0.4	0.22
14.26	23.50	23.35	13.9	-0.4	0.22
15.23	23.60	23.35	14.8	-0.4	0.22
16.30	23.52	23.35	15.9	-0.4	0.26

**Remark:**

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Velocity of standard

<sup>7</sup> Velocity of Unit Under Calibration

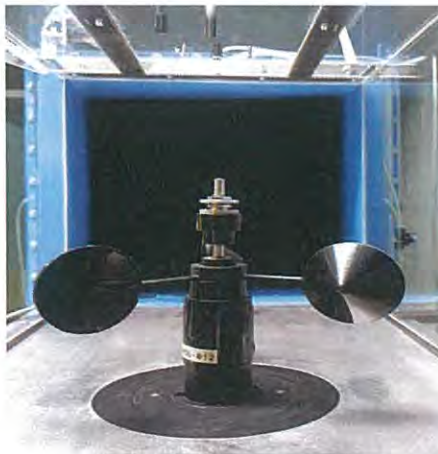**PHOTO OF CALIBRATION SET-UP**

Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.

\*\*\*End of Certificate of Calibration\*\*\*





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.

Certificate Number

CL-007-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Wind Direction Sensor  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 110-WS-25DL-D  
**SERIAL NUMBER** : Sensor: WSD-012  
Data logger: A5791  
**ID NUMBER** : SGK\_FS0088  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

### Calibration procedure:

The wind direction sensor was calibrated against Standard Rotary Encoder model: AX4009TS-DM04-P3-S-U0 in an close test-section of Eiffel-type wind tunnel with 900 cm<sup>2</sup> cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

### Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: DA-0043-22

### Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

**RECEIVED DATE** : 10 Jan 2023  
**MEASUREMENT DATE** : 13 Jan 2023  
**ISSUE DATE** : 13 Jan 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C  
Relative Humidity : 55.0 ± 15.0 %RH  
Atmospheric Pressure : 1010 ± 10 hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

**CALIBRATION CONDITION** : Wind tunnel cross-section area<sup>1</sup> 900 cm<sup>2</sup>  
Win direction frontal area<sup>2</sup> 129 cm<sup>2</sup>  
Diameter of mounting pipe<sup>3</sup> - mm  
Blockage ratio of test object<sup>4</sup> 0.143 [-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (23.7)°C, (46.8) %RH and (1011.8) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved signatory: .....

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>



MEASUREMENT RESULTS <sup>5</sup>

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	$D^6_{std}$ Degree (°)	$D^7_{uuc}$ Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.02	0.000	0	0	0.58
	45.000	42	-3	0.82
	90.000	90	0	0.74
	135.000	136	1	0.74
	180.000	182	1	0.76
	225.000	228	2	0.76
	270.000	273	3	0.74
	315.000	318	3	0.74

## Remark:

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Direction of standard

<sup>7</sup> Direction of Unit Under Calibration



\*\*\*End of Certificate of Calibration\*\*\*



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Pressure measurement laboratory  
Calibration services department.



NSC - TISI - TIS 17025  
CALIBRATION 0367

## CERTIFICATE OF CALIBRATION

Certificate No. : CL-004-66

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Digital barometer  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : 110-WS-25BP  
**SERIAL NUMBER** : A5791  
**ID NUMBER** : SGK\_FS0088  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd,  
Khwaeng Suan Luang, Khet Suan Luang,  
Bangkok 10250 Thailand.  
**RECEIVED DATE** : 10 Jan 2023  
**MEASUREMENT DATE** : 13 Jan 2023  
**ISSUE DATE** : 13 Jan 2023

### Calibration procedure:

The pressure calibration was done by In-house calibration method as WI-CL-003 according to comparison method with Digital pressure calibrator based on DKD-R 6-1

### Traceability:

The measurement results are traceable to the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) which complies with the requirements of ISO/IEC17025:2017, ANSI/NCSL Z540-1 via Certificate number: MP-0205-22

The reported uncertainty is based on a standard uncertainty multiplied by a coverage  $k=2$ , providing a level of confidence of approximately 95%.

### CONDITION OF THIS RESULT OF CALIBRATION:

1. Reference Standard Instrument:

Instrument	Model	Serial No.	Certificate No.	Due Date
Absolute Pressure Transducer	CPG2500	4100126P	MP-0205-22	02 Dec 2023

1. Calibration effort for calibration sequence A

2. The UUC\* was installed in vertical orientation above reference standard instrument and center of UUC\* was used as the reference level.

3. Calibration conditions:

4. Condition : ☒ Normal ☐ Abnormal  
Pressure transmitting medium : Air  
 $\rho_{Fl}$  (20°C, 1 bar) : 1.19 kg/m<sup>3</sup>  
 $H_{amb}$  : (55±15) %  
 $t_{amb}$  : (23±3) °C  
 $p_{amb}$  : (1010±10) mbar

5. The certificate is valid only to the item calibrated on date and place of calibration

### Calibrated by:

☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved signatory: \_\_\_\_\_

215/mv

Mr. Parinya Booncharoen  
Calibration Department Manager





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Pressure measurement laboratory  
Calibration services department.



NSC - TISI - TIS 17025  
CALIBRATION 0367

## CERTIFICATE OF CALIBRATION

Certificate No. : CL-004-66

Page 2 of 2 Pages

MEASUREMENT RESULTS : ☒ Without adjustment ☐ With adjustment

CALIBRATION IN THE RANGE OF : 950 – 1050 mbar

The results of calibration and associated measurement uncertainties are reported in the table below.

STD (mbar)	UUC* (mbar)	Error (mbar)	Uncertainty (k=2) (mbar)
950.13	951.0	0.9	1.1
970.10	970.7	0.6	0.79
990.10	990.5	0.4	0.64
1010.11	1010.3	0.2	0.42
1030.08	1030.0	-0.1	0.40
1050.10	1049.7	-0.4	0.60

Note: UUC\* Unit Under Calibration

: To convert the result in report unit to Pa should be multiply by 100



REVIEW BY	<i>Narakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	5/17/24

Certificate Number

CL-003-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Cup anemometer  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 110-WS-25DL-D  
**SERIAL NUMBER** : Sensor: WSD-002  
Data logger: A5443  
**ID NUMBER** : BKK\_FS0975  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 28 Dec 2022  
**MEASUREMENT DATE** : 05 Jan 2023  
**ISSUE DATE** : 09 Jan 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

<b>CALIBRATION CONDITIONS</b>	: Wind tunnel cross-section area <sup>1</sup>	900	cm <sup>2</sup>
	Win direction frontal area <sup>2</sup>	100	cm <sup>2</sup>
	Diameter of mounting pipe <sup>3</sup>	-	mm
	Blockage ratio of test object <sup>4</sup>	0.111	[-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (23.8) °C, (45.8) %RH and (1016.2) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved signatory: .....

*[Signature]*

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>



**MEASUREMENT RESULTS<sup>5</sup>**

The cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle, UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

$V_{std}$ <sup>6</sup> (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	$V_{UUC}$ <sup>7</sup> (m/s)	Error (m/s)	$U$ ( $k=2$ ) (m/s)
0.989	23.96	23.80	0.9	-0.1	0.19
2.035	23.72	23.80	1.9	-0.2	0.16
3.058	23.98	23.80	3.0	-0.1	0.32
4.139	23.86	23.80	4.0	-0.1	0.20
5.01	23.90	23.80	5.0	0.0	0.20
6.01	23.98	23.80	6.0	0.0	0.19
7.06	23.80	23.80	7.0	-0.1	0.22
8.17	23.84	23.80	8.2	0.0	0.24
9.10	23.90	23.80	9.2	0.1	0.32
10.09	23.90	23.80	10.0	-0.1	0.27
11.14	23.90	23.80	11.1	0.0	0.23
12.14	24.00	23.80	12.1	0.0	0.34
13.20	23.90	23.80	13.2	0.0	0.32
14.27	23.90	23.80	14.2	0.0	0.35
15.25	23.92	23.80	15.3	0.0	0.34
16.30	23.92	23.80	16.3	0.0	0.29

**Remark:**

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Velocity of standard

<sup>7</sup> Velocity of Unit Under Calibration

**PHOTO OF CALIBRATION SET-UP**

Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Wind Direction Sensor  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 110-WS-25DL-D  
**SERIAL NUMBER** : Sensor: WSD-002  
Data logger: A5443  
**ID NUMBER** : BKK\_FS0975  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 28 Dec 2022  
**MEASUREMENT DATE** : 06 Jan 2023  
**ISSUE DATE** : 09 Jan 2023

**ENVIRONMENTAL CONDITIONS:**

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

<b>CALIBRATION CONDITION</b>	: Wind tunnel cross-section area <sup>1</sup>	900	cm <sup>2</sup>
	Win direction frontal area <sup>2</sup>	129	cm <sup>2</sup>
	Diameter of mounting pipe <sup>3</sup>	-	mm
	Blockage ratio of test object <sup>4</sup>	0.143	[-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (24.0)°C, (53.7) %RH and (1015.2) hPa.

**TABULATION OF RESULTS:**

The table on next page give the measured values.

**Calibrated by:**

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved signatory: .....

Mr. Parinya Booncharoen  
Calibration Department Manager

**Remark:**

<sup>1</sup> Nozzle cross-section area of the wind tunnel

<sup>2</sup> Projected cross-section area of the tested object include mounting pipe

<sup>3</sup> Diameter of mounting pipe

<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>

**Calibration procedure:**

The wind direction sensor was calibrated against Standard Rotary Encoder model: AX4009TS-DM04-P3-S-U0 in an close test-section of Eiffel-type wind tunnel with 900 cm<sup>2</sup> cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

**Traceability:**

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: DA-0043-22

**Uncertainty of Measurement:**

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

MEASUREMENT RESULTS<sup>5</sup>

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	$D_{std}^6$ Degree (°)	$D_{uuc}^7$ Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.00	0.000	0	0	0.58
	45.000	42	-3	0.74
	90.000	88	-2	0.68
	135.000	133	-2	0.74
	180.001	181	1	0.74
	225.000	227	2	0.74
	270.000	273	3	0.74
	315.000	318	3	0.74

## Remark:

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Direction of standard

<sup>7</sup> Direction of Unit Under Calibration



\*\*\*End of Certificate of Calibration\*\*\*





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Pressure measurement laboratory  
Calibration services department.



## CERTIFICATE OF CALIBRATION

Certificate No. : CL-001-66

Page 1 of 2 Pages

MEASUREMENT ITEM : Digital barometer  
MANUFACTURER : Novalynx  
MODEL/TYPE : 110-WS-25BP  
SERIAL NUMBER : A5443  
ID NUMBER : BKK\_FS0975  
CONDITION AS-RECEIVED : Used item  
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd,  
Khwaeng Suan Luang, Khet Suan Luang,  
Bangkok 10250 Thailand.  
RECEIVED DATE : 28 Dec 2022  
MEASUREMENT DATE : 06 Jan 2023  
ISSUE DATE : 09 Jan 2023

### Calibration procedure:

The pressure calibration was done by In-house calibration method as WI-CL-003 according to comparison method with Digital pressure calibrator based on DKD-R 6-1

### Traceability:

The measurement results are traceable to the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) which complies with the requirements of ISO/IEC17025:2017, ANSI/NCSL Z540-1 via Certificate number: MP-0205-22

The reported uncertainty is based on a standard uncertainty multiplied by a coverage  $k=2$ , providing a level of confidence of approximately 95%.

### CONDITION OF THIS RESULT OF CALIBRATION:

#### 1. Reference Standard Instrument:

Instrument	Model	Serial No.	Certificate No.	Due Date
Absolute Pressure Transducer	CPG2500	4100126P	MP-0205-22	02 Dec 2023

#### 1. Calibration effort for calibration sequence A

2. The UUC\* was installed in vertical orientation above reference standard instrument and center of UUC\* was used as the reference level.

#### 3. Calibration conditions:

4. Condition : ☒ Normal ☐ Abnormal  
Pressure transmitting medium : Air  
 $\rho_{F1}$  (20°C, 1 bar) : 1.19 kg/m<sup>3</sup>  
 $H_{amb}$  : (55±15) %  
 $t_{amb}$  : (23±3) °C  
 $p_{amb}$  : (1010±10) mbar

5. The certificate is valid only to the item calibrated on date and place of calibration

### Calibrated by:

☒ Mr. Sorawit Thachalad  
☐ Miss Jittraporn Lertsomphol



Approved signatory: .....

Mr. Parinya Booncharoen  
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Pressure measurement laboratory  
Calibration services department.



## CERTIFICATE OF CALIBRATION

Certificate No. : CL-001-66

Page 2 of 2 Pages

MEASUREMENT RESULTS : ☒ Without adjustment ☐ With adjustment

CALIBRATION IN THE RANGE OF : 950 – 1050 mbar

The results of calibration and associated measurement uncertainties are reported in the table below.

STD (mbar)	UUC* (mbar)	Error (mbar)	Uncertainty (k=2) (mbar)
950.16	950.9	0.7	0.93
970.12	970.6	0.5	0.77
990.09	990.4	0.3	0.53
1010.10	1010.1	0.0	0.37
1030.11	1029.8	-0.3	0.48
1050.12	1049.7	-0.4	0.61

Note: UUC\* Unit Under Calibration

: To convert the result in report unit to Pa should be multiply by 100





## CERTIFICATE OF CALIBRATION

Certificate No.: WD-02072022

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.  
: Wind direction sensor: Novalynx.

Model/Type : Data logger: 200-WS-25LB  
: Wind direction sensor: WS-02F

Serial Number : Data logger: A5192  
: Wind direction sensor: -

ID No : Data logger: SGK\_FS0035  
: Wind direction sensor: -

Customer : ALS laboratory group (Thailand) co., ltd.  
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250  
Thailand.

### Environmental Condition:

The measurement was carried out in an ambient temperature of  $(23 \pm 3) ^\circ\text{C}$ , and relative humidity of  $(40 \pm 10) \%$ .

### Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control. The measurement were taken at  $45^\circ$  intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

### Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: Q21086014, Certificate No.: KWS64/0025.

Measurement Date : Jul 13, 2022.  
Issued Date : Jul 14, 2022.

### Calibrated by

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jittrapon Lertsomphol



### Approved Signatory:

  
Mr. Parinya Booncharoen.  
Calibration Department Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-02072022

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	360	359	-1	3.0
2		45	45	43	-2	3.0
3		90	90	87	-3	3.0
4		135	135	133	-2	3.0
5		180	180	180	0	3.0
6		225	225	228	3	3.0
7		270	270	274	4	3.0
8		315	315	320	5	3.0
9	Counter Clockwise	0/360	360	359	-1	3.0
10		45	45	43	-2	3.0
11		90	90	87	-3	3.0
12		135	135	133	-2	3.0
13		180	180	180	0	3.0
14		225	225	228	3	3.0
15		270	270	274	4	3.0
16		315	315	320	5	3.0

UUC\*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

\*\*\*End of Certificate of Calibration\*\*\*





## CERTIFICATE OF CALIBRATION

Certificate No: WS-02072022

Page 1 of 2 pages

**Measurement Item** : Cup anemometer with data logger.

**Manufacturer** : Data logger: Novalynx  
: Cup anemometer: Novalynx

**Model/Type** : Data logger: 200-WS-25LB  
: Cup anemometer: WS-02F

**Serial Number** : Data logger: A5193  
: Cup anemometer: -

**ID No** : Data logger: SGK\_FS0035  
: Cup anemometer: -

**Customer** : ALS laboratory group (Thailand) co., ltd.  
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

**Test Conditions**

: Wind tunnel cross test section area	900	cm <sup>2</sup>
: Anemometer frontal area	100	cm <sup>2</sup>
: Diameter of mounting pipe	-	mm
: Blockage ratio of test object	0.111	[-]

**Test Conditions**

: Air temperature	24.0	±0.8 °C
: Air pressure	1005.3	±0.4 hPa
: Relative air humidity	45.1	±3.5 %RH

**Calibration Procedure** : Calibration was carried out base on;  
IEC 61400-12-1 ED.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines;  
MEASNET Anemometer Calibration Procedure – Version 2: 2009;

**Traceability** : This calibration documents the traceable to national standard, Which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).

**Measurement Date** : Jul 13, 2022.

**Issued Date** : Jul 14, 2022.

**Calibrated by**

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved Signatory: .....

Mr. Parinya Booncharoen  
Calibration Department Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-02072022

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V <sub>STD</sub> Reading m/s	V <sub>UUC</sub> * Reading m/s	Error (m/s)	Uncertainty (%)
2.063	2.0	-0.1	2.4
4.115	4.1	0.0	1.1
5.97	6.1	0.1	0.97
7.99	8.0	0.0	0.79
9.99	10.2	0.2	0.69
12.03	12.3	0.3	0.63
14.02	14.3	0.3	0.58
15.98	16.4	0.4	0.48
14.99	15.3	0.3	0.57
13.01	13.3	0.3	0.52
10.97	11.1	0.1	0.52
8.98	9.0	0.0	0.74
6.99	7.0	0.0	0.81
5.121	5.1	0.0	0.86
3.000	3.0	0.0	1.7
1.040	0.9	-0.1	4.5

UUC\*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

#### Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TESTO INC.	06352145	Aug 07, 2021	MW-0034-21	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	Aug 07, 2021	MW-0034-21	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	Aug 08, 2021	MW-0035-21	0 - 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2022	CL-027-65	-30 - 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2022	RH-03032022	0 - 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2022	BP-01032022	500 - 1100 hPa
7	Wind tunnel	ESSOM	MP330D	-	-	0 - 50 Hz

\*\*\*End of certificate of calibration\*\*\*





# SITHIPHORN ASSOCIATES CO.,LTD.

## CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

Cert. No. : ACC22038

Pages : 1 of 3

### Calibration Certificate

**Equipment :** SOUND CALIBRATOR  
**Manufacturer :** RION  
**Model :** NC-75  
**Serial No.:** 35024429  
**ID No.:** - S&K FS 0114

REVIEW BY	<i>Mongkorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	14/11/23

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 03 NOVEMBER 2022  
**Calibration Date :** 14 NOVEMBER 2022  
**Date of Issue :** 15 NOVEMBER 2022

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*[Signature]*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACC22038

Job No. : VC66AC0006

Pages : 2 of 3

Calibration Procedure : CP-AC-03

**Calibration Method :**

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	33461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23
Audio Analyzer	AVR-3360A	V744B6069	EF-0010-22	07-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

## Continuation of Calibration Certificate

Cert. No. : ACC22038

Job No. : VC66AC0006

Pages : 3 of 3

**Result of calibration :****1. Sound pressure level**

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit (dB)
94	93.94	-0.06	0.14	0.40

**2. Frequency**

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Tolerance limit (%)
1000	1000.0	0.0	0.1	1.0

**3. Total distortion**

Measured value (%)	Uncertainty (%)	Tolerance limit (%)
0.33	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————



# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL22248

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 01173617 / 172179 / 74029  
**ID No.:** SGK\_FS0030

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAEANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 11 OCTOBER 2022  
**Calibration Date :** 25-26 OCTOBER 2022  
**Date of Issue :** 27 OCTOBER 2022

REVIEW BY	<i>Nathakorn P</i>
APPROVED BY	<i>Nathakorn P</i>
NEXT CAL. DATE	25/10/23

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*T. Petchurai*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

Cert. No. : ACL22248

Job No. : VC65AC0090

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



Continuation of Calibration Certificate

Cert. No. : ACL22248

Job No. : VC65AC0090

Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1



## Continuation of Calibration Certificate

Cert. No. : ACL22248

Job No. : VC65AC0090

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.95)	93.9	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
15.9

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	13.1
C - weight	19.2
Flat	25.0

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.1	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.6	0.7	0.7	±5.0

## Continuation of Calibration Certificate

Cert. No. : ACL22248

Job No. : VC65AC0090

Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.1	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.1	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.1	0.1	± 0.3



## Continuation of Calibration Certificate

Cert. No. : ACL22248

Job No. : VC65AC0090

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22248  
Job No. : VC65AC0090  
Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0



## Continuation of Calibration Certificate

Cert. No. : ACL22248

Job No. : VC65AC0090

Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.7	89.6	-0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate