

ภาคผนวก ค

เอกสารสอบเทียบเครื่องมือ



List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Andersen Instruments, Inc.	G25A 1901	Tisch Environmental, Inc.	05072022	5 Jul 22	4 Jul 24	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	23P1400	9 May 23	8 May 24	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀) Hydrogen Chloride	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	22P2722	22 Jul 22	21 Jul 23	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀) Hydrogen Chloride	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	22H1583	27 Jul 22	26 Jul 23	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1201778110	UAE Consultant Co.,Ltd.	07042023	7 Apr 23	6 Apr 24	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1200636462	UAE Consultant Co.,Ltd.	28032023	28 Mar 23	27 Mar 24	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1200636463	UAE Consultant Co.,Ltd.	24012023	24 Jan 23	23 Jan 24	-
8	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
9	Wind Speed/Wind Direction	WS/WD	LSI LASTEM	05103-5 30905375	Thai Meteorological Department	263/22	14 Jul 22	13 Jul 23	-
10	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Svantek	SV35A 73246	Innovative Instrument Co.,Ltd.	22-ACT-405	1 Jul 22	30 Jun 23	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
11	Sound Level Meter	L _{Aeq} 24 hrs*, L _{Amax} *, L _{A90}	Larson Davis	LxT2	Innovative Instrument Co.,Ltd.	22-ACT-104	11 Feb 22	10 Feb 24	-
				0006614					
12	Sound Level Meter	L _{Aeq} 24 hrs*, L _{Amax} *, L _{A90}	Larson Davis	LxT2	Innovative Instrument Co.,Ltd.	22-ACT-102	11 Feb 22	10 Feb 24	-
				0006615					

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Stack									
1	Pre-Test Console	Total Suspended Particulate Hydrogen Chloride	Apex Instruments, USA.	XC-572-V 1904012	Envi Equipment Service Co., Ltd.	E22-07026	26 Jul 22	25 Jul 23	-
2	Flue gas Analyzer	Sulphur Dioxide Oxide of Nitrogen as Nitrogen Dioxide Carbon Monoxide	Testo	Testo 350 60723967	Entech Industrial Solution Co., Ltd.	G 650806	28 Nov 22	27 Nov 23	-

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	Horiba	LAQUA-PH210 HA0D0081	Technology Promotion Association (Thailand-Japan)	23CH6	5 Jan 23	4 Jan 24	-
2	DO Meter	DO	Horiba	LAQUA-DO210 HE0H0008	Technology Promotion Association (Thailand-Japan)	23TW3	5 Jan 23	4 Jan 24	-
3	Conductivity Meter	Conductivity	Horiba	LAQUA-EC210 HC0J0016	Technology Promotion Association (Thailand-Japan)	23CH7	5 Jan 23	4 Jan 24	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Workplace									
1	Thermal Environment Monitor	Heat Meter	3M	QuesTemp 32 TPT060015	Innovative Instrument Co.,Ltd.	23-TPM-049	25 Jan 23	24 Jan 24	-
2	Thermal Environment Monitor	Heat Meter	TSI QUEST	QuesTemp 32 TPT060013	Innovative Instrument Co.,Ltd.	23-TPM-045	25 Jan 23	24 Jan 24	-
3	Thermal Environment Monitor	Heat Meter	3M	QuesTemp 32 TPQ020022	Innovative Instrument Co.,Ltd.	22-TPM-303	26 Jul 22	25 Jul 23	-
4	Thermal Environment Monitor	Heat Meter	3M	QuesTemp 32 TPS030008	Innovative Instrument Co.,Ltd.	23-TPM-046	25 Jan 23	24 Jan 24	-
5	Primary Flow Calibrator	Calibrate personal pump	TSI,Inc	5300 53002052003	Innovative Instrument Co.,Ltd.	22-AFM-039	22 Mar 22	21 Mar 23	-
6	Aneroid Barometer	Total Dust Respirable Dust Hydrogen Chloride	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	22P2729	22 Jul 22	21 Jul 23	-
7	Digital Thermo - Hygrometer	Total Dust Respirable Dust Hydrogen Chloride	Testo, Germany	608-H1 34843033	Technology Promotion Association (Thailand-Japan)	22H1990	27 Sep 22	26 Sep 23	-
8	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Svantek	SV35 44783	Innovative Instrument Co.,Ltd.	22-ACT-524	19 Aug 22	18 Aug 23	-
9	Sound Level Meter	$L_{Aeq\ 8\ hrs}$ L_{Amax}	Rion, Japan	NL-42 00609500	Sithiporn Associates Co., Ltd.	ACL23028	12 Jan 23	11 Jan 24	-
10	Sound Level Meter	$L_{Aeq\ 8\ hrs}$ L_{Amax}	Rion, Japan	NL-42 00709670	Sithiporn Associates Co., Ltd.	ACL23031	12 Jan 23	11 Jan 24	-
11	Sound Level Meter	$L_{Aeq\ 8\ hrs}$ L_{Amax}	Rion, Japan	NL-42 01010777	Sithiporn Associates Co., Ltd.	ACL23117	11 Apr 23	10 Apr 24	-

RECALIBRATION

DUE DATE:

July 5, 2023

Certificate of Calibration

Calibration Certification Information

Cal. Date: July 5, 2022 Rootsmeter S/N: 438320 Ta: 297 °K
Operator: Jim Tisch Pa: 750.1 mm Hg
Calibration Model #: G25A Calibrator S/N: 1901

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.3540	3.3	2.00
2	3	4	1	0.9650	6.4	4.00
3	5	6	1	0.8640	8.0	5.00
4	7	8	1	0.8200	8.9	5.50
5	9	10	1	0.6780	12.9	8.00

Data Tabulation

Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9859	0.7281	1.4073	0.9956	0.7353	0.8899
0.9818	1.0174	1.9902	0.9915	1.0274	1.2585
0.9797	1.1339	2.2251	0.9893	1.1451	1.4071
0.9785	1.1933	2.3337	0.9881	1.2050	1.4757
0.9732	1.4354	2.8146	0.9828	1.4496	1.7798
QSTD	m=	1.98897	QA	m=	1.24546
	b=	-0.03691		b=	-0.02334
	r=	0.99996		r=	0.99996

Calculations

$Vstd = \Delta Vol \left(\frac{Pa - \Delta P}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)$	$Va = \Delta Vol \left(\frac{Pa - \Delta P}{Pa} \right)$
$Qstd = Vstd / \Delta Time$	$Qa = Va / \Delta Time$

For subsequent flow rate calculations:

$Qstd = 1/m \left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} - b \right)$	$Qa = 1/m \left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} - b \right)$
---	--

Standard Conditions

Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH: calibrator manometer reading (in H2O)	
ΔP: rootsmeter manometer reading (mm Hg)	
Ta: actual absolute temperature (°K)	
Pa: actual barometric pressure (mm Hg)	
b: intercept	
m: slope	

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
53/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No.: 23P14C0
Page: 1 of 2

Equipment: U-Tube Manometer
Manufacturer: Dwyer
Model: 1221-36-W/M
Serial No.:
ID No.: UAE.EFM.02C/2560

Condition As-Received: Used Item

Received Date: 26 April 2023

Calibration Date: 09 May 2023

Reference: 2304-0703WSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1010 mbar

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0137-22	24 Aug 2023

2.This result of calibration was made on requested at the point specified by customer.

3.Scale and conversion factor is 1 kPa = 4.0146293 inH2O

4.This instrument was used clean air as pressure media.

5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by: Suwit Aussarree
Issue Date: 11 May 2023

Approved Signatory: Attapol P.
[] Phalinee Prabpaipal
[] Sura Suwannasri
[x] Attapol Panurach

B 0314240



Cert.No.: 23P1400
Page: 2 of 2

Result of calibration:- Without adjustment

Range: 0 inH₂O to 36 inH₂O

Function:- Pressure Measurement

Scale Interval: 0.1 inH₂O (The Fifth Estimate)

Increasing Pressure

UUC Indication				
Applied Pressure (inH ₂ O)	High-port side (inH ₂ O)	Low-port side (inH ₂ O)	ΔP (inH ₂ O)	Error (inH ₂ O)
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-1.00	2.00	0.00
4.00	2.00	-2.00	4.00	0.00
6.00	3.00	-3.00	6.00	0.00
8.00	4.00	-4.00	8.00	0.00
10.00	5.00	-5.00	10.00	0.00
12.00	6.00	-6.00	12.00	0.00
14.00	7.02	-7.02	14.04	0.04
16.00	8.02	-8.02	16.04	0.04
18.00	9.04	-9.04	18.08	0.08
20.00	10.04	-10.04	20.08	0.08
22.00	11.02	-11.02	22.04	0.04
24.00	12.02	-12.02	24.04	0.04
26.00	13.02	-13.02	26.02	0.02
28.00	14.00	14.00	0.00	-28.00
30.00	15.00	-15.00	30.00	0.00
32.00	16.00	-16.00	32.00	-0.02
34.00	17.00	-17.00	34.00	-0.04
35.80	18.00	-18.00	35.80	0.14

The uncertainty of measurement was ± 0.11 inH₂O

* UUC = Unit Under Calibration

* ΔP = High-port side - Low-port side

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-

Attapol P.

a 1160341



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No.: 22P2722
Page: 1 of 2

Equipment: Aneroid Barometer

Manufacturer: Barigo

Model: -

Serial No.: -

ID No.: UAE.ANV.013/2547

Condition As-Received: Used Item

Received Date: 20 July 2022

Calibration Date: 22 July 2022

Reference: 2207-C584WSC

Submitted by: United Analyst and Engineering Consultant Co.Ltd.

Ambient Temperature: $(23 \pm 2) ^\circ\text{C}$

Relative Humidity: $(50 \pm 15) \%$

Atmospheric Pressure: 1010 mbar

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure C²-P10, using "DKD-R 6-1; Calibration of Pressure Gauges, Edition 03/2014" as a guidelines.

Condition of this result of calibration

1.Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505045	MP-0076-22	02 May 2023

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.Scale and conversion factor is 1 kPa = 7.50062 mmHg

5.This result of calibration instrument was in absolute pressure.

6.This instrument was used clean air as pressure media.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by: Suwit Aussarree

Issue Date: 25 July 2022

Approved Signatory: Attapol P.

| | Phalinee Prabpaipal

| | Sura Suwannasri

| | Attapol Panurach

เอกสารไม่ควบคุม

B 0293205



Cert.No.: 22P2722
Page: 2 of 2

Result of calibration:- Without adjustment

Range : 720 mmHg to 780 mmHg

Function:- Absolute Pressure Measurement

Scale Interval : 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	718.46	729.33	739.85	750.22	760.90	772.01	785.89
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	760.0	770.0	780.0
Error (mmHg)	1.54	0.67	0.15	-0.22	-0.90	-2.01	-5.99

Decreasing Pressure

Applied Pressure (mmHg)	785.90	771.99	760.85	750.17	739.90	729.57	718.62
UUC* Indication (mmHg)	780.0	770.0	760.0	750.0	740.0	730.0	720.0
Error (mmHg)	-5.90	-1.99	-0.85	-0.17	0.10	0.43	1.38

The uncertainty of measurement was ± 0.24 mmHg

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม
a 1118533



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLLANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 22H1583
Page : 1 of 2

Equipment : Dial Thermo-Hygrometer

Manufacturer: Barjo

Model : -

Serial No. : -

ID No. : UAE.ANV.016/2547

Condition As-Received: Used Item

Received Date: 20 July 2022

Calibration Date: 22 July 2022

to 27 July 2022

Reference: 2207-0586WSC

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Chilled Mirror Hygrometer Sensor	Dew Prime II	31863	19714	17 Sep 2022
2) Standard Humidity/Temperature Meter	400	10240757	TH-0125-21	13 Dec 2022

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained at:-

- National Institute of Standards and Technology (NIST) , The United States of America

- National Institute of Metrology Thailand (NIMT)

Calibrated by : Somchai Durnwor
Issue Date : 03 August 2022

Approved Signatory :

[✓] Chakrit Waewanjua
[] Pornthippa Tameyakul
[] Viporn Tantiyawuti

เอกสารไม่ควบคุม
B 0293719



Cert. No.: 22H1583
Page.: 2 of 2

Result of Calibration:-

Function: Humidity measurement. Without Adjustment

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	42	1.9	1.6
25.0	60.0	63	3.0	1.8
25.0	80.0	78	-2.0	2.0

Result of Calibration:-

Function: Temperature measurement. Without Adjustment

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
20.00	20.0	0.00	0.72
30.01	30.0	-0.01	0.72
35.04	35.0	-0.04	0.72
39.98	40.0	0.02	0.72

UUC*: Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-o0o-

[Signature]

เอกสารไม่ควบคุม
a 1119777



United Analyst and Engineering Consultant Co., Ltd.

3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Apr 7, 2023

Equipment : Gas Analyzer (NO₂)

Model : 42i

Manufacturer : Thermo Scientific

Serial Number : 1201778110

Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.68

PPM Manufacturer :

Thermo Scientific

Nitric Oxide (NO)

45.94

PPM Model :

146i

Methane (CH₄)

-

PPM Serial Number :

1180540071

Carbon Monoxide (CO)

984.8

Cylinder No. :


EB0143262

Expiration Date :

Jun 21, 2024

Multi-point gas test data

Level	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	101.1	1.10	1.09
Level 3	40.00%	200.0	200.9	0.90	0.45
Level 4	60.00%	300.0	300.5	0.50	0.17
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)		
: Acceptable Limit ± 5%			0.34		

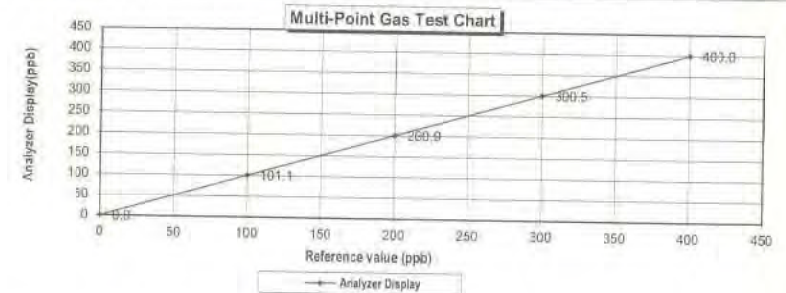

Calculate by

Aphivest K.
2, 4, 66

Approve by

P. J. Uerni
7, Apr, 2023

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Mar 28, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1200636462

Standard Gas Concentration


Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 21, 2024

Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	101.5	1.50	1.48	1.48
Level 3	40.00%	200.0	201.0	1.00	0.50	0.50
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.45

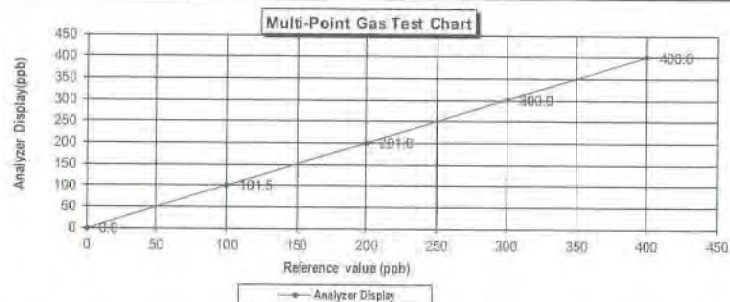

Calculate by

Sirichai Samgan
28 / 3 / 66

Approve by

Peterson W.
28 / Mar / 2023

MULTI-POINT GAS TEST REPORT

Test Date : Jan 24, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1200636463

Standard Gas Concentration


Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 21, 2024

Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.5	0.50	0.25	0.25
Level 4	60.00%	300.0	301.0	1.00	0.33	0.33
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.26
: Acceptable Limit $\pm 5\%$						

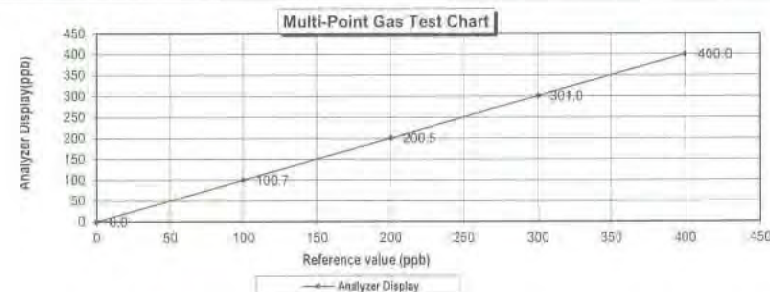

Calculate by

Sirichai Samgan
24 / 1 / 66

Approve by

Peterson W.
24 / Jan / 2023

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04NI99E15A01D3 Reference Number: 122-402135167-1
Cylinder Number: EB0143262 Cylinder Volume: 144.4 CF
Laboratory: 124 - Durham (SAP) - NC Cylinder Pressure: 2015 PSIG
PGVP Number: B22021 Valve Outlet: 660
Gas Code: CO,NO,NOX,SO2,BALN Certification Date: Jun 21, 2021

Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 820/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	03/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	03/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.68 PPM	G1	+/- 1.0% NIST Traceable	03/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 0.7% NIST Traceable	06/14/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20061120	CC708088	49.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D685026	3.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMIS	401423838102	CC505581	4.348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 18, 2023
NTRM	16011043	CC473277	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14060119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Nov 15, 2025

The SRM, PRM or GMIS noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO2	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO2	FTIR	Jun 03, 2021

Triad Data Available Upon Request:

NOTES: PO #E221002807

GROSS WT: 28.40kg

NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

[Signature]

Approved for Release



CERT 3082.01

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by: Calibration & Test Section: Meteorological Instruments Bureau

Date of Issue: 14 July, 2022

Certification No. 263/22

Page: 1 of 2

Object: Wind speed and wind direction

Manufacturer: Sensor: YOUNG

Basic Datalogger: NRG

Type: Sensor: 05103-45 Basic Datalogger: LR20

Serial No.: Sensor: 97947 Basic Datalogger: 30905375

Customer: United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,

Bangchak, Prakanong, Bangkok 10260.

Calibration Condition: Temperature 25.1 °C Barometric Pressure 1004.8 hPa

NATIONAL STANDARD WIND TUNNEL:

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 20 m/sec

Calibrated by: Nalorapol

Signed:

Mr. Watcharapol Subwa:

Mr. Pisood Promsut

Mechanical Engineer

(Authorised Signatory)

for the Chief

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Certification No. 263/22

14 July, 2022

Page : 2 of 2

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacuum	Velocity	Velocity	Correction
m/sec	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	0.95	0.05
3.02	-	-	-	2.94	0.08
5.00	-	-	-	4.94	0.06
7.04	-	-	-	6.98	0.06
9.02	-	-	-	8.93	0.09
11.01	-	-	-	10.92	0.09
13.01	-	-	-	12.92	0.09
15.01	-	-	-	15.02	-0.01
17.02	-	-	-	17.01	0.01
20.02	-	-	-	20.16	-0.14

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Watcharapol Subwat

Mr. Watcharapol Subwat

Mechanical Engineer



เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SONTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5966-1 FAX: (66)0-2116-7140



Page 1 of 2

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT
CO.,LTD.

Certificate No : 22-ACT-405

Request No : Req-2022-1080

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Prakanong, Bangkok 10260

Unit Under Calibration Details

Measurement item : Acoustic Calibrator
Manufacturer : SVANTEK
Model : SV 35A
Serial Number : 73246
ID : UAE.EFM.104/2561

Class : 1
Range : 94 , 114 dB / 1000 Hz
Instrument Status : Used

Calibration Environment and Details

Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 15 June 2022
Calibration Date : 1 July 2022
Location of Calibration : LAB : Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEL	31 May 2023
THD Multimeter	2015	1047765	NIMT	2 February 2023

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By :

Mr. Noppadon Luangart
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 1 July 2022

(The results related only to the item mentioned. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.)

เอกสารไม่ควบคุม



เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
 INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
 7/139 MOD 13, SOI SUTJITNAKORN 11 TAMBON BANG KAEU,
 AMPHOE BANG PHU SAMUT PRAKAN PROVINCE 10540 THAILAND
 TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140



Certificate No : 22-ACT-405
 Request No : Req-2022-1080

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	93.80	-0.20	-	-	0.12	0.25
114 dB / 1000 Hz	113.77	-0.23	-	-	0.11	0.25

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.10	0.70
114 dB / 1000 Hz	1000.00	0.00	-	-	0.10	0.70

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 1 (± %)
	Measured (%)	Measured (%)		
94 dB / 1000 Hz	0.09	-	0.40	2.5
114 dB / 1000 Hz	0.31	-	0.40	2.5

Note :

- Acceptance limit was (IEC60942:2017 Class 1)
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 22-ACT-104
 Address : 81 Soi Udcmsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok Request No : Req-2022-0232
 10260

Unit Under Calibration Details

Measurement item : Sound Level Meter Microphone Class : 2
 Manufacturer : LARSON DAVIS Microphone Model : 375A04
 Model : LxT2 Microphone S/N : 329352
 Serial Number : 0006614 Preamplifier Model : PRMLxT2C
 ID : UAE.EFM 045/2564 Preamplifier S/N : 071534
 Resolution : 0.1 dB Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
 Humidity : 50 %RH ± 20 %RH
 Barometric Pressure : 1013 hPa ± 10 hPa
 Received Date : 31 January 2022
 Calibrated Date : 11 February 2022
 Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
 Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	15 September 2022	GRAS
Multi-frequency Calibrator	Quest	Quest-cal	EFA000214	14 June 2022	TSI
Audio Generator	SvanteK	Svan401	131	18 October 2022	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart
 Calibration Officer

Approved By : Mr. Pacit Mathavorn
 Calibration Engineer Supervisor
 Issue Date : 11 February 2022

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม

Certificate No : 22-ACT-104
 Request No : Req-2022-0232

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		Adjust		UNCERTAINTY	Acceptance
		UUC	ERR	UUC	ERR		
FAST / A / 37-139	Level	(dB)	(dB)	(dB)	(dB)	(± dB)	(± dB)
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)	(± dB)
1000 Hz 114.00 dB	113.85	114.0	+0.15	113.9	-0.05	0.20	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN.58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	28.7	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	28.6	0.10
C	28.8	0.10
Z	34.7	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency			UNCERTAINTY	Acceptance Limit
	Weighting Response curve				
FAST / 37-139	A	C	Z	(± dB)	(± dB)
STD Setting	(dB)	(dB)	(dB)		
125 Hz	0.0	0.1	0.1	0.50	2.0
1000 Hz	0.0	0.0	0.0	0.60	1.0
4000 Hz	0.7	0.7	0.7	0.60	3.0
8000 Hz	1.0	0.9	0.8	0.70	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม



Certificate No : 22-ACT-104

Request No : Req-2022-0232

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency			UNCERTAINTY	Acceptance
FAST/ 37-139	Weighting Response curve				
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)	(± dB)
63 Hz	-0.2	0.0	0.0	0.2	±0
125 Hz	-0.1	0.0	0.0		±1.5
250 Hz	-0.1	0.0	0.0		±1.5
500 Hz	-0.1	0.0	0.0		±1.5
1000 Hz	0.0	0.0	0.0		±1.0
2000 Hz	0.0	0.1	0.0		±0
4000 Hz	0.0	0.0	0.0		±0
8000 Hz	0.0	0.0	0.0		±0
16000 Hz	-0.1	-0.1	-0.1		+5, -INF

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
FAST / 37-139	REF	UUC	ERR		
UUC Weighting	(dB)	(dB)	(dB)	0.2	0.2
A	114.00	114.0	0.0		
C	114.00	114.0	0.0		
Z	114.00	114.0	0.0		

UUC Setting	STD	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
37-139 / A	REF	UUC	ERR		
UUC Time Response	(dB)	(dB)	(dB)	0.2	0.1
Fast	114.00	114.0	0.0		
Slow	114.00	114.0	0.0		
Loq	114.00	114.0	0.0		



Certificate No : 22-ACT-104

Request No : Req-2022-0232

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
FAST / A / 37-139	UUC		
STD Setting	(dB)	0.1	0.3
Initial	114.0		
Final	114.0		
Deviated	0.0		

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
FAST / A / 37-139	REF	UUC	ERR		
STD dB	(dB)	(dB)	(dB)	0.3	1.1
140.00	140	140.0	0.0		
139.00	139	139.0	0.0		
134.00	134	134.0	0.0		
129.00	129	129.0	0.0		
124.00	124	124.0	0.0		
119.00	119	119.0	0.0		
114.00	114	114.0	0.0		
109.00	109	109.0	0.0		
104.00	104	104.0	0.0		
99.00	99	99.0	0.0		
94.00	94	94.0	0.0		
89.00	89	89.0	0.0		
84.00	84	84.0	0.0		
79.00	79	79.0	0.0		
74.00	74	74.0	0.0		
69.00	69	69.0	0.0		
64.00	64	64.0	0.0		
59.00	59	59.0	0.0		
54.00	54	54.0	0.0		
49.00	49	49.0	0.0		
44.00	44	44.1	0.1		
39.00	39	39.3	0.3		

Certificate No : 22-ACT-104
 Request No : Req-2022-0232

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance
FAST / A	REF	UUC	ERR	(± dB)	Limit
UUC Range	(dB)	(dB)	(dB)		(± dB)
37-139	44.1	43.7	-0.4	0.3	1.1
	114	114.0	0.0		1.1

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance
A / 37-139	Toneburst	Ref	UUC	ERR	(± dB)	Limit
UUC Time Response	(ms)	(dB)	(dB)	(dB)		(± dB)
Fast	200	135.0	135.0	0.0	0.3	1.0
	2	118.0	117.9	-0.1		+1.0, -2.5
	0.25	109.0	108.7	-0.3		+1.5, -5.0
Slow	200	128.6	128.5	-0.1		1.0
	2	109.0	108.8	-0.2		+1.0, -5.0
SEL	200	129.0	129.0	0.0		1.0
	2	109.0	109.1	+0.1		+1.0, -2.5
	0.25	100.0	99.7	-0.3		+1.5, -5.0

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY	Acceptance
FAST / C / 95-142	REF	UUC	ERR	(± dB)	Limit
STD Setting	(dB)	(dB)	(dB)		(± dB)
Complete cycle	137.4	136.7	-0.70	0.2	3.0
Positive half cycle	136.4	136.2	-0.20		2.0
Negative half cycle	136.4	136.2	-0.20		2.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม

Certificate No : 22-ACT-104
 Request No : Req-2022-0232

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC	(± dB)	Limit
STD Setting	(dB)		(± dB)
Positive one-half cycle	142.7		
Negative one-half cycle	142.6		
Deviated	0.0	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC	(± dB)	Limit
STD Setting	(dB)		(± dB)
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
 Address : 81 Soi Udomsuk 41, Sukhamvit Road, Bangchak, Prakanong, Bangkok
 10260

Certificate No : 22-ACT-102
 Request No : Req-2022-0233

Unit Under Calibration Details

Measurement item : Sound Level Meter
 Manufacturer : LARSON DAVIS
 Model : LxT2
 Serial Number : 0066615
 ID : UAE.EFM 046/2564
 Resolution : 0.1 dB
 Microphone Class : 2
 Microphone Model : 375A04
 Microphone S/N : 328672
 Preamplifier Model : PRMLxT2C
 Preamplifier S/N : 071539
 Instrument Status : Used

Calibration Environment and Details


Temperature : 23 °C ± 2 °C
 Humidity : 50 %RH ± 20 %RH
 Barometric Pressure : 1013 hPa ± 10 hPa
 Received Date : 31 January 2022
 Calibrated Date : 11 February 2022
 Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
 Location of Calibration : Lab Acoustic


Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	15 September 2022	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	14 June 2022	TSI
Audio Generator	SvanteK	Svan401	131	18 October 2022	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : 
 Mr. Noppadon Luangart
 Calibration Officer

Approved By : 
 Mr. Pait Mathavorn
 Calibration Engineer Supervisor
 Issue Date : 11 February 2022

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม

Certificate No : 22-ACT-102

Request No : Req-2022-0233

1. Indication at the calibration check frequency

UUC Setting	Nominal Level (dB)	Before Adjust		Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)		
FAST / A / 37-139							
Calibrator Setting							
1000 Hz 114.00 dB	113.85	113.9	+0.05	113.9	0.05	0.20	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN.58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	27.8	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	27.7	0.10
C	27.5	0.10
Z	34.0	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	A (dB)	C (dB)	Z (dB)		
FAST / 37-139					
STD Setting					
125 Hz	-0.1	0.1	0.1	0.50	2.0
1000 Hz	0.0	0.0	0.0	0.60	1.0
4000 Hz	0.5	0.5	0.6	0.60	3.0
8000 Hz	0.3	0.3	0.4	0.70	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม

Certificate No : 22-ACT-102
 Request No : Req-2022-0233

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency			UNCERTAINTY	Acceptance
FAST / 37-139	Weighting Response curve				
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)	Limit (± dB)
63 Hz	-0.2	0.0	0.0	0.2	2.0
125 Hz	-0.1	0.0	0.0		1.5
250 Hz	-0.1	0.0	0.0		1.5
500 Hz	-0.1	0.0	0.0		1.5
1000 Hz	0.0	0.0	0.0		1.0
2000 Hz	0.0	0.0	0.0		2.0
4000 Hz	0.0	0.0	0.0		3.0
8000 Hz	0.0	0.0	0.0		5.0
16000 Hz	-0.1	-0.1	-0.1		+5, -INF.

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / 37-139	REF	UUC	ERR		
UUC Weighting	(dB)	(dB)	(dB)	0.2	0.2
A	114.00	114.0	0.0		
C	114.00	114.0	0.0		
Z	114.00	114.0	0.0		

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
37-139 / A	REF	UUC	ERR		
UUC Time Response	(dB)	(dB)	(dB)	0.2	0.1
Fast	114.00	114.0	0.0		
Slow	114.00	114.0	0.0		
Leq	114.00	114.0	0.0		

Certificate No : 22-ACT-102
 Request No : Req-2022-0233

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	UUC		
STD Setting	(dB)		
Initial	114.0		
Final	114.0		
Deviated	0.0	0.1	0.3

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	REF	UUC	ERR		
STD dB	(dB)	(dB)	(dB)	0.3	1.1
140.00	140	140.0	0.0		
139.00	139	139.0	0.0		
134.00	134	134.0	0.0		
129.00	129	129.0	0.0		
124.00	124	124.0	0.0		
119.00	119	119.0	0.0		
114.00	114	114.0	0.0		
109.00	109	109.0	0.0		
104.00	104	104.0	0.0		
99.00	99	99.0	0.0		
94.00	94	93.9	-0.1		
89.00	89	88.9	-0.1		
84.00	84	83.9	-0.1		
79.00	79	78.9	-0.1		
74.00	74	73.9	-0.1		
69.00	69	68.9	-0.1		
64.00	64	63.9	-0.1		
59.00	59	58.9	-0.1		
54.00	54	53.9	-0.1		
49.00	49	48.9	-0.1		
44.00	44	44.0	0.0		
39.00	39	39.2	0.2		
34.00	34	34.3	0.3		

Certificate No : 22-ACT-102
 Request No : Req-2022-0233

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit
FAST / A	REF	UUC	ERR		(\pm dB)
UUC Range	(dB)	(dB)	(dB)		
37-139	43.2	42.9	-0.3	0.3	1.1
	114	114.0	0.0		1.1

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit
A / 37-139	Toneburst	Ref	UUC	ERR		(\pm dB)
UUC Time Response	(ms)	(dB)	(dB)	(dB)		
Fast	200	135.0	135.0	0.0	0.3	1.0
	2	118.0	117.8	-0.2		+1.3, -2.5
	0.25	109.0	108.6	-0.4		+1.3, -5.0
Slow	200	128.6	128.5	-0.1		1.0
	2	109.0	108.9	-0.1		+1.3, -5.0
	200	129.0	129.0	0.0		1.0
SEL	2	109.0	109.0	0.0		+1.3, -2.5
	0.25	100.0	99.8	-0.2		+1.5, -5.0

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit
FAST / C / 95-142	REF	UUC	ERR		(\pm dB)
STD Setting	(dB)	(dB)	(dB)		
Complete cycle	137.4	136.8	-0.60	0.2	3.0
Positive half cycle	136.4	136.2	-0.20		2.0
Negative half cycle	136.4	136.2	-0.20		2.0

Certificate No : 22-ACT-102
 Request No : Req-2022-0233

12. Overload indication

UUC Setting	Measured	UNCERTAINTY (\pm dB)	Acceptance Limit
FAST / A / 37-139	UUC		(\pm dB)
STD Setting	(dB)		
Positive one-half cycle	141.7		
Negative one-half cycle	141.7		
Deviated	0.0	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY (\pm dB)	Acceptance Limit
FAST / A / 37-139	UUC		(\pm dB)
STD Setting	(dB)		
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

E-mail: sales@envi-ees.com

Page :1 of 6

เอกสารไม่ควบคุม

Page : 2 of 6

เอกสารไม่ควบคุม

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	26/07/2022	01:00 PM	Std Temp	293	K
Console Serial Number	1904012	Calibration Reference No.	E22-07026			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	755.24		mm Hg	K ₁	0.386	
DGM Serial Number	00004116	Calibration Meter Gamma	0.999			Console Leak Check	PASS	


Calibration Data								
Results								
Standardized Data				Dry Gas Meter				
Dry Gas Meter		Calibration Meter		Calibration Factor		Flowrate		Variation
(V _{m(std)})	(Q _{m(std)})	(V _{w(std)})	(Q _{w(std)})	(Y)	(ΔY)	(Q _{std@corr})	(ΔH _{std})	
m ³	m ³ /min	m ³	m ³ /min			m ³ /min	mm H ₂ O	(ΔH _{std})
0.137	0.011	0.136	0.011	0.998	0.008	0.011	48.348	1.191
0.137	0.011	0.136	0.011	0.998	0.009	0.011	48.564	1.407
0.137	0.016	0.136	0.016	0.998	0.009	0.016	47.020	-0.138
0.137	0.016	0.136	0.016	0.997	0.007	0.016	47.167	0.010
0.274	0.019	0.272	0.019	0.994	0.004	0.019	48.109	0.952
0.274	0.019	0.272	0.019	0.994	0.004	0.019	48.229	1.072
0.275	0.027	0.271	0.026	0.985	-0.004	0.026	45.481	-1.676
0.275	0.027	0.270	0.026	0.981	-0.008	0.026	45.535	-1.622
0.276	0.030	0.270	0.029	0.977	-0.013	0.029	46.499	-0.658
0.276	0.030	0.269	0.029	0.974	-0.016	0.029	46.619	-0.538
				0.990	Y Average			ΔH@ Average
						47.157		

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.
For ΔH_{std}, orifice pressure differential that equates to 0.75 cfm (0.0212 m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2 inches (5.1 mm) H₂O.



เอกสารไม่ควบคุม

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	26/07/2022	01:00 PM	Std Temp	293	K
Console Serial Number	1904012	Calibration Reference No.	E22-07026			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	755.24		mm Hg	K ₁	0.386	
DGM Serial Number	00004116	Calibration Meter Gamma	0.999			Console Leak Check	PASS	

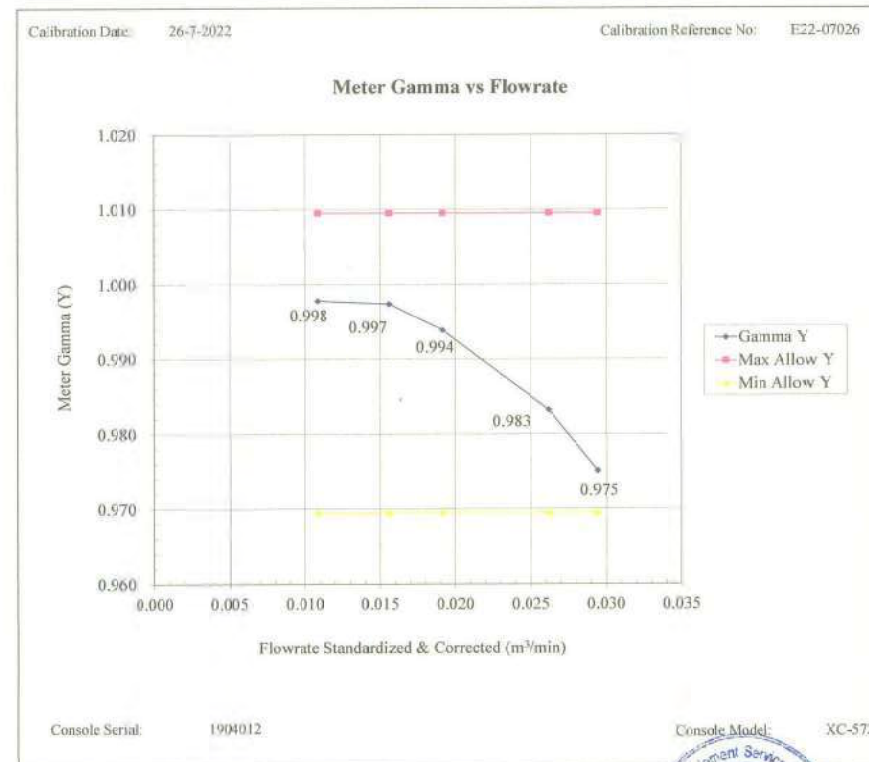


เอกสารไม่ควบคุม

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	26/07/2022	01:00 PM	Std Temp	293	K
Console Serial Number	1904012	Calibration Reference No.	E22-07026			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	755.24	mm Hg		K ₁	0.386	
DGM Serial Number	00004116	Calibration Meter Gamma	0.999			Console Leak Check	PASS	

Calibration Date: 26-7-2022

Calibration Reference No: E22-07026

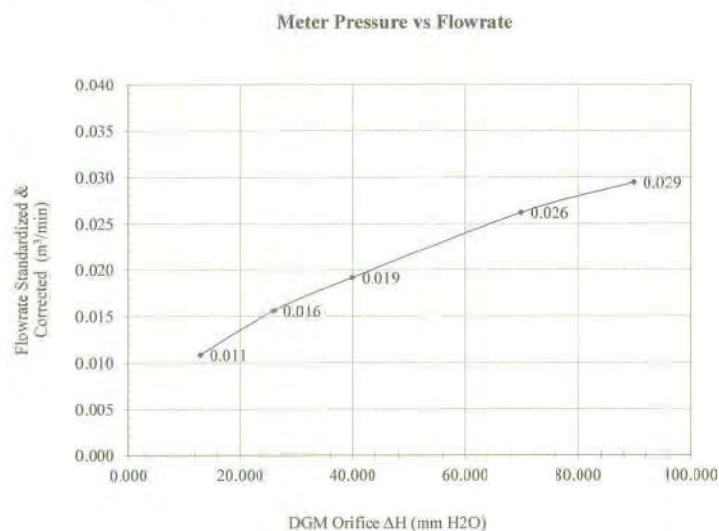

Console Serial: 1904012

Console Model: XC-572-V



เอกสารไม่ควบคุม

THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information	
Console Model Number	XC-572-V
Console Serial Number	1904012
DGM Model Number	SK25EX
DGM Serial Number	00004116
Meter Box Model Number	JENCO 765 KF
Meter Box Serial Number	JC 17118

Calibration Conditions			
Date	Time	26/07/2565	02:45 PM
Calibration Reference No.	E22-07026		
Reference Thermometer	DIGICON		
Serial Number	183169105		

Results

Console Thermocouple Simulator											
Channel and test point	Meter Box Channel Temperature Reading (°C)										
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	816.0	1038.0
Stack	-17.0	23.0	36.0	92.0	148.0	257.0	370.0	480.0	592.0	814.0	1036.0
Aux	-18.0	23.0	36.0	92.0	148.0						
Probe	-17.0	23.0	36.0	92.0	148.0						
Filter	-17.0	23.0	36.0	92.0	148.0						
Oven	-17.0	23.0	36.0	92.0	148.0						
Exit	-17.0	24.0	37.0								

Stack ± 1.50% Absolute
Probe ± 3.0 °C
Filter ± 3.0 °C

Tolerance Range

Meter ± 3.0 °C
Exit ± 2.0 °C



เอกสารไม่ควบคุม

Certificate No: S 650806
Date of issue: 29-Nov-22

ENTECH	<input checked="" type="radio"/> PASS <input type="radio"/> NOT PASS
Remarks	
Verify <i>[Signature]</i>	Approve <i>[Signature]</i>

Acceptance Limit $\leq 5\%$

Instrument description: Flue gas Analyzer
Instrument model: Testo 350 New
Instrument serial no.: 60723967
ID no. or control no.: UAE.EFM.027/2559
Manufacturer: Testo SE & Co. KGaA
Probe description: :
Probe model: :
Probe serial: :
Customer name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD
Customer address: 81 SOI UDOMSUK41, SUKHUMVIT ROAD, BANGCHAK PRAKANONG BANGKOK 10260

Total pages of certificate: 3 Pages
Receiving no.: L-224183
Receiving date: 25-Nov-22
Parameter of calibration: Gas Calibration (Oxygen 2.498, 10.04, 21.02 %vol, Carbon Monoxide 80.14, 309.9, 1003 ppm, Nitrogen Dioxide 30.34, 80.96, 202.2 ppm, Nitric Oxide 30.08, 150.9, 320.6 ppm, Sulphur Dioxide 50.04, 100.8, 601.1 ppm)

Condition of UUC: Used

Ambient condition: All of the Measurement were carried out the stabilized labotary

Temperature : 23 ± 5 °C

Humidity : 55 ± 15 %RH

Calibration place: 17/121 Soi Ngarnwongwan 47 Yaek 48, Toengsonghong, Lakse, Bangkok 10210

Calibration procedure no.: WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test. Environmental condition.

This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid.

This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration: 28-Nov-22

[Signature]

Mr. Sedawut Nueathong
Calibration Technician

[Signature]

Mrs. Nongluck Wongsettee
Technical Manager

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O ₂) 2.498 % Vol	#219/21	Linde	30-Sep-25
Oxygen (O ₂) 10.04 % Vol	CG-0153-21	Nimit	18-Nov-26
Oxygen (O ₂) 21.02 % Vol	CG-0041-22	Nimit	10-Feb-27
Carbon monoxide (CO) 80.14 ppm	CG-0040-22	Nimit	14-Feb-27
Carbon monoxide (CO) 309.9 ppm	2903/21	Linde	22-Jun-23
Carbon monoxide (CO) 1003 ppm	2583/22	Linde	09-Aug-24
Nitrogen Dioxide (NO ₂) 30.34 ppm	2703/22	Linde	22-Aug-24
Nitrogen Dioxide (NO ₂) 80.96 ppm	2041/22	Linde	26-Jun-24
Nitrogen Dioxide (NO ₂) 202.2 ppm	3239/21	Linde	20-Jul-23
Nitric Oxide (NO) 30.08 ppm	CG-0089-22	Nimit	13-Jun-24
Nitric Oxide (NO) 150.9 ppm	2857/21	Linde	27-Jun-23
Nitric Oxide (NO) 320.6 ppm	2944/21	Linde	02-Jul-23
Sulphur Dioxide (SO ₂) 50.04 ppm	3205/21	Linde	25-Jul-23
Sulphur Dioxide (SO ₂) 100.8 ppm	3507/22	Linde	09-Nov-24
Sulphur Dioxide (SO ₂) 601.1 ppm	3204/21	Linde	20-Jul-23

Measured room conditions

Temperature : 23.4 °C Humidity : 54.1 %RH Pressure : 1015.6 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,200 ml/min Gas pressure : 1021.8 mbar

Calibration Results Before Adjustment (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.498	2.54	0.042	0.20
O ₂ (%Vol)	10.04	10.07	0.03	0.40
O ₂ (%Vol)	21.02	21.08	0.06	0.80
CO (ppm)	80.14	80	-0.14	3.0
CO (ppm)	309.9	308	-1.9	6.0
CO (ppm)	1003	997	-6	12
NO ₂ (ppm)	30.34	26.9	-3.44	8.0
NO ₂ (ppm)	80.96	68.8	-11.16	8.0
NO ₂ (ppm)	202.2	187.3	-14.9	12
NO (ppm)	30.08	29	-1.08	8.0
NO (ppm)	150.9	150	-0.9	8.0
NO (ppm)	320.6	314	-6.6	12
SO ₂ (ppm)	50.04	45	-5.04	6.0
SO ₂ (ppm)	100.8	95	-5.8	6.0
SO ₂ (ppm)	601.1	590	-11.1	13

Calibration Results After Adjustment (Table 3)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.498	2.54	0.042	0.20
O ₂ (%Vol)	10.04	10.07	0.03	0.40
O ₂ (%Vol)	21.02	21.08	0.06	0.80
CO (ppm)	80.14	80	-0.14	3.0
CO (ppm)	309.9	308	-1.9	6.0
CO (ppm)	1003	997	-6	12
NO ₂ (ppm)	30.34	31.2	0.86	8.0
NO ₂ (ppm)	80.96	81.2	0.24	8.0
NO ₂ (ppm)	202.2	204.8	2.6	12
NO (ppm)	30.08	29	-1.08	8.0
NO (ppm)	150.9	150	-0.9	8.0
NO (ppm)	320.6	314	-6.6	12
SO ₂ (ppm)	50.04	50	-0.04	6.0
SO ₂ (ppm)	100.8	100	-0.8	6.0
SO ₂ (ppm)	601.1	603	1.9	13

Remark : 1 nmol/mol = 1 %vol , 1 μmol/mol = 1 ppm.

End of Report



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 23CH6
Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA0D0081
ID No. : UAE.EFM.074/2564(EFM.pH.07/64)
Condition As-Received: Used Item
Received Date : 04 January 2023
Calibration Date : 05 January 2023
Reference : 2301-0060WSC-2
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature : $(25 \pm 2.5) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with standard thermometer

Calibrated by : Saithip Meangmai

Approved by : Malee
Approved Signatory

(/) Malee Butkruea
() Saithip Meangmai
() Warakorn Lemgagtrakul

Issue Date : 10 January 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

DATE	<input checked="" type="radio"/> PASS <input type="radio"/> NOT PASS
Remarks	Temp 20.5 (5+3. Thermo meter) pH 7.00 (Std. Voltage Input) pH 7.00 (Std. Buffer Solution)
By	<u>Saithip</u>
(Signature)	(Signature)
Verified	Approved

เอกสารไม่ควบคุม



Cert.No.: 23CH6
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	22E2769	24 Aug 2023
2) Ref. Standard Thermometer	4982054	110RC044	22I1306	27 Oct 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials :- The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	826588	09 July 2024
pH 6.987	CPA chem	823322	20 June 2023
pH 10.008	CPA chem	826590	09 July 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (\pm mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: HA0D0081	4.00	177.48	177.4	4.01	0.058	2.00
	7.00	0.00	0.1	6.98	0.058	2.00
	7.00	0.00	0.1	6.98	0.058	2.00
	10.00	-177.48	-177.4	10.01	0.058	2.00

เอกสารไม่ควบคุม



Cert.No.: 23CH6
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (\pm)	Coverage factor k
pH Electrode S/N.: 990C0039	4.008	4.01	138.5	0.0085	2.05
	6.987	6.98	-32.1	0.011	2.00
	6.987	7.00	-33.1	0.011	2.00
	10.008	10.03	-205.2	0.0096	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe:

- Model : 9652

- Serial No. : 990C0039

Dimension of probe:

- Length : 102 mm.

- Diameter : 15.5 mm.

- Immersion Depth : 85 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (\pm °C)	Coverage factor k
25.0	25.004	25.0	-0.004	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
35.0	35.003	35.0	-0.003	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

53/4/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 23TW3

Page.: 1 of 2

Certificate of Testing

Equipment : DO Meter
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE0H0008
ID No. : UAE.EFM.086/2564(EFM.DO.05/64)
Received Date : 04 January 2023
Test Date : 05 January 2023
Reference : 2301-0061WSC-5
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : Walalak Srithean

Approved by :


Approved Signatory

(/) Malee Butkruea
() Saithip Meangmai
() Warakorn Lernagatrakul

Issue Date : 6 January 2023

เอกสารไม่ควบคุม



Cert.No.: 23TW3

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 9K0L0009

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.14	8.14	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency. The environmental impact control and present to organization it may concerned intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 23LM3
Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter With Sensor
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE0H0008
ID No. : UAE.EFM.086/2564(EFM.DO.05/64)
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : TPA On Site Calibration Laboratory
Received Order : 4 January 2023
Calibrated Date : 6 January 2023
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Malee Bulkruea

Approved by : 
Approved Signatory

() Pornthippa Tameyakul
(✓) Suwit Imjai

Issue Date : 10 January 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : DO Meter With Sensor
Condition As-Received : Used Item
Reference : 2301-0061WSC-6
Procedure Used :-

Cert. No.: 23LM3
Page.: 2 of 2

Calibration were conducted using in-house calibration procedure GP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Digital Thermometer	1523	2188080	2211285	21 Oct 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 9K0L0009

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
25.0	80	24.996	25.0	0.004	0.16	2.00
30.0	80	29.995	30.1	0.105	0.16	2.00
35.0	80	34.996	35.0	0.004	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 / FAX. 0-2719-9484



Cert.No.: 23CH7
Page.: 1 of 3

Certificate of Calibration

Equipment : Conductivity Meter
Manufacturer : Horiba
Model : LAQUA-EC210
Serial No. : HCQJ0016
ID No. : UAE.EFM.076/2564(EFM.SCT.02/64)
Condition As-Received: Used Item
Received Date : 04 January 2023
Calibration Date : 05 January 2023
Reference : 2301-0059WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Ambient Temperature : $(25 \pm 2.5) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$
Calibration Procedure: In-house method
- CP-CH6 by direct measurement
with certified reference material (CRM)
- CP-CH8 by comparison with standard thermometer
Calibrated by : Walalak Sirithean

Approved by :

Approved Signatory

(/) Malee Butkruea
() Saithip Meangmai
() Warakorn Lemgagtrakul

Issue Date : 10 January 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 23CH7

Page.: 2 of 3

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	9549224	130RC003	221484	17 Apr 2023
2) Ref. Std. Thermometer	4982054	110RC044	2211306	27 Oct 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI
through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1413.0 $\mu\text{S/cm}$	CPA Chem	823328	20 June 2023
12.880 mS/cm	CPA Chem	823329	20 June 2023

- Control Conductivity calibration solution temperature by Water bath $(25 \pm 0.1) ^\circ\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 1413.0 $\mu\text{S/cm}$

Conductivity Electrode Serial No.: 9B0K0160

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (\pm)	Coverage factor k
1413.0 $\mu\text{S/cm}$	1375 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	9.2 $\mu\text{S/cm}$	2.00
12.880 mS/cm	12.43 mS/cm	12.70 mS/cm	0.086 mS/cm	2.00

Remark - UUC* = Unit Under Calibration

เอกสารไม่ควบคุม



Cert.No.: 23CH7

Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9383

- Serial No. : 9B0K0160

Dimension of probe;

- Length : 104 mm.

- Diameter : 16 mm.

- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (\pm °C)	Coverage factor <i>k</i>
25.0	25.000	25.0	0.000	0.13	2.00
30.0	29.999	30.1	0.101	0.13	2.00
35.0	34.999	35.1	0.101	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAE0,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140



Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING
CONSULTANT CO.,LTD.

Certificate No : 23-TPM-049

Request No : Req-2023-0048

Address : 81 Soi Udomsak 41, Sukhumvit Road, Bangchak, Prakanong,
Bangkok 10260

Page : 1/2

Unit Under Calibration Details

Calibration Parameter : Temperature

Instrument Name : Thermal Environment Monitor

Range Calibration : 20 °C to 60 °C

Manufacturer : TSI QUEST

Type of Sensor : RTD

Model : QT-32

Sensor Diameter (mm) : 4.5

Serial Number : TPT060015

Calibration Position (mm) : 67.5

Resolution : 0.1 °C

Instrument Status : Used

ID Number : UAE.EFM222/2562

Calibration Environment and Details

Temperature : 23 °C \pm 3 °C

Humidity : 55 %RH \pm 15 %RH

Received Date : 10 January 2023

Calibrated Date : 25 January 2023

Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard

Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN:
08000057, ID: 02-TPM Which was calibrated on 10 March 2022, Calibration Certificate No.: QR22-0578

Traceability

This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.:
Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor *k*=2, providing a level of confidence approximately 95 %.

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date :

25 January 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม



เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
 INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
 7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KALU,
 AMPHOE BANG PHU SAMUT PRAKAN PROVINCE 10540 THAILAND
 TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140



Calibration Note

UUC Adjustment: ☐ Not Adjust

Certificate No : 23-IPM-049

Request No : Req-2023-0048

Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (°C)
WET	20.003	20.0	0.0	0.14
	25.004	25.0	0.0	0.14
	30.005	30.0	0.0	0.14
	35.006	35.0	0.0	0.14
	40.005	40.0	0.0	0.14
	45.005	45.0	0.0	0.14
	50.004	50.0	0.0	0.14
	60.007	60.0	0.0	0.14
DRY	20.006	20.0	0.0	0.14
	25.004	25.0	0.0	0.14
	30.006	30.0	0.0	0.14
	35.006	35.0	0.0	0.14
	40.006	40.1	- 0.1	0.14
	45.006	45.1	- 0.1	0.14
	50.006	50.1	- 0.1	0.14
	60.006	60.1	- 0.1	0.14
GLOBE	20.004	19.9	+ 0.1	0.14
	25.006	24.9	+ 0.1	0.14
	30.004	29.9	+ 0.1	0.14
	35.003	34.9	+ 0.1	0.14
	40.007	40.0	0.0	0.14
	45.006	45.0	0.0	0.14
	50.006	50.0	0.0	0.14
	60.005	60.0	0.0	0.14

End of Certificate

Calibrated By :

Smit

M: Sittichok Jirapakdeesakun

The result related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม



Certificate of Calibration

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangehak, Prakanong, Bangkok 10260
Certificate No : 23-TPM-045
Request No : Req-2023-0044
Page : 1/2

Unit Under Calibration Details

Calibration Parameter : Temperature
Instrument Name : Thermal Environment Monitor
Manufacturer : TSI QUEST
Model : QT-32
Serial Number : TPT060013
Resolution : 0.1 °C
ID Number : UAE.EFM220/2562
Range Calibration : 20 °C to 60 °C
Type of Sensor : RTD
Sensor Diameter (mm) : 4.5
Calibration Position (mm) : 67.5
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 15 %RH
Received Date : 10 January 2023
Calibrated Date : 25 January 2023
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN: 08C00057, ID: 02-TPM Which was calibrated on 10 March 2022, Calibration Certificate No.: QR22-0578

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.: Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Approved By :
Mr. Pasit Mathavorn
Calibration Engineer Supervisor
Issue Date : 25 January 2023

	<input checked="" type="radio"/> PASS <input type="radio"/> NOT PASS
Remarks Accuracy $\pm 0.5^\circ\text{C}$ Uncertainty $\pm 0.1^\circ\text{C}$ Date 25/1/23 Approve	



Calibration Note

UUC Adjustment : Not Adjust

Certificate No : 23-TPM-045

Request No : Req-2023-0044

Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Corrective (°C)	Uncertainty (±°C)
WET	20.003	19.9	-0.1	0.14
	25.005	24.9	-0.1	0.14
	30.003	29.9	-0.1	0.14
	35.003	34.9	-0.1	0.14
	40.007	40.0	0.0	0.14
	45.004	45.0	0.0	0.14
	50.005	50.0	0.0	0.14
DRY	60.005	60.0	0.0	0.14
	20.004	20.0	0.0	0.14
	25.003	25.0	0.0	0.14
	30.004	30.0	0.0	0.14
	35.004	35.0	0.0	0.14
	40.003	40.1	-0.1	0.14
	45.004	45.1	-0.1	0.14
GLOBE	50.005	50.1	-0.1	0.14
	60.007	60.1	-0.1	0.14
	20.003	20.1	-0.1	0.14
	25.006	25.1	-0.1	0.14
	30.005	30.1	-0.1	0.14
	35.005	35.1	-0.1	0.14
	40.005	40.1	-0.1	0.14
	45.006	45.1	-0.1	0.14
	50.003	50.1	-0.1	0.14
	60.003	60.1	-0.1	0.14

End of Certificate

Calibrated By :

Mr. Sirichok Jirapukdeesakun



Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING

CONSULTANT CO.,LTD.

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,
 Bangkok 10260

Certificate No : 22-TPM-303

Request No : Req-2022-1244

Page : 1/2

Unit Under Calibration Details

Calibration Parameter : Temperature

Instrument Name : Thermal Environment Monitor

Manufacturer : 3M

Model : QT-32

Serial Number : TPQ020022

Resolution : 0.1 °C

ID Number : UAE.EFM.005/2559

Range Calibration : -20 °C to 60 °C

Type of Sensor : RTD

Sensor Diameter (mm) : 4.5

Calibration Position (mm) : 67.5

Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 15 %RH

Received Date : 11 July 2022

Calibrated Date : 26 July 2022

Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard

Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN:

08000057, ID: 02-TPM Which was calibrated on 10 March 2022, Calibration Certificate No.: QR22-0578

Traceability

This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.: Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Approved By :

Mr. Paci Mathavorn

Calibration Engineer Supervisor

Issue Date :

26 July 2022


☒ PASS
☐ NOT PASS

Remarks:
 Accuracy = $\pm 0.5^\circ$
 Uncertainty = $\pm 0.14^\circ$

Verify: 
 Approve:  (10/05/25)

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
 INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
 7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEU,
 AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10340 THAILAND
 TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140



Calibration Note

UUC Adjustment ☒ Not Adjust

Certificate No : 22-TPM-303

Request No : Req-2022-1244


Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (±°C)
WET	20.003	19.7	+ 0.3	0.14
	25.004	24.7	+ 0.3	0.14
	30.004	29.7	+ 0.3	0.14
	35.004	34.7	+ 0.3	0.14
	40.003	39.8	+ 0.2	0.14
	45.005	44.8	+ 0.2	0.14
	50.004	49.9	+ 0.1	0.14
	60.007	59.9	+ 0.1	0.14
DRY	20.004	19.8	+ 0.2	0.14
	25.004	24.8	+ 0.2	0.14
	30.006	29.8	+ 0.2	0.14
	35.007	34.8	+ 0.2	0.14
	40.007	39.8	+ 0.2	0.14
	45.004	44.8	+ 0.2	0.14
	50.006	50.0	0.0	0.14
	60.002	60.0	0.0	0.14
GLOBE	20.005	19.7	+ 0.3	0.14
	25.004	24.7	+ 0.3	0.14
	30.003	29.7	+ 0.3	0.14
	35.005	34.7	+ 0.3	0.14
	40.006	39.8	+ 0.2	0.14
	45.007	44.8	+ 0.2	0.14
	50.008	50.0	0.0	0.14
	60.006	60.0	0.0	0.14

End of Certificate

Calibrated By :


 Mr. Sittichok Jirapukdeesakun

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม



Certificate of Calibration

Customer : UNITED ANALYST AND ENGINEERING
Name : UNITED ANALYST AND ENGINEERING
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,
Bangkok 10260

Certificate No : 23-TPM-046
Request No : Req-2023-0045

Page : 1/2

Unit Under Calibration Details

Calibration Parameter : Temperature
Instrument Name : Thermal Environment Monitor
Manufacturer : 3M
Model : QT-32
Serial Number : TPS030008
Resolution : 0.1 °C
ID Number : UAE.EFM083/2561

Range Calibration : 20 °C to 60 °C
Type of Sensor : RTD
Sensor Diameter (mm) : 4.5
Calibration Position (mm) : 67.5
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 15 %RH
Received Date : 10 January 2023
Calibrated Date : 25 January 2023
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.


Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN:
08000057, ID: 02-TPM Which was calibrated on 10 March 2022, Calibration Certificate No. : QR22-0578

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.:
Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Approved By : Mr. Pasit Mathavorn
Mr. Pasit Mathavorn
Calibration Engineer Supervisor
Issue Date : 25 January 2023





Calibration Note

UUC Adjustment : Not Adjust

Certificate No : 23-TPM-046

Request No : Req-2023-0045

Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (°C)
WET	20.003	20.0	0.0	0.14
	25.006	25.0	0.0	0.14
	30.005	30.0	0.0	0.14
	35.003	35.0	0.0	0.14
	40.005	40.0	0.0	0.14
	45.005	45.0	0.0	0.14
	50.006	50.0	0.0	0.14
	60.004	60.0	0.0	0.14
DRY	20.003	20.2	-0.2	0.14
	25.002	25.2	-0.2	0.14
	30.004	30.2	-0.2	0.14
	35.004	35.2	-0.2	0.14
	40.004	40.2	-0.2	0.14
	45.003	45.2	-0.2	0.14
	50.004	50.2	-0.2	0.14
	60.007	60.2	-0.2	0.14
GLOBE	20.004	20.0	0.0	0.14
	25.005	25.0	0.0	0.14
	30.004	30.0	0.0	0.14
	35.005	35.0	0.0	0.14
	40.006	40.1	-0.1	0.14
	45.006	45.1	-0.1	0.14
	50.004	50.1	-0.1	0.14
	60.005	60.1	-0.1	0.14

End of Certificate

Calibrated By :

Mr. Sittichok Jirapakdeesakun



Page 1/2

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 22-AFM-039

Request No : Req-2022-0398

Unit Under Calibration Details

Measurement Item : Primary Flow Calibrator

Sensor Model : -

Manufacturer : TSI

Sensor Serial Number : -

Model : 5300

Serial Number : 53002052003

ID : UAE.EFM.162/2564

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 14 February 2022

Calibration Date : 22 March 2022

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	20 May 2022
Air Flow Meter	Gilibrator 3 High flow	18501012012	Sensidyne	21 May 2022
Air Flow Meter	4045 F	4045 0533 001	MIT	10 January 2023

Traceability :

This certificate provides traceability of measurement to recognized national standard, and to the realization of the International System of Units (SI)

Units (SI)

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Liangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mahavorn

Calibration Engineer Supervisor

Issue Date : 22 March 2022

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.00 Issue date 01/07/19

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

☒ PASS
☐ NOT PASS

Remarks: 250 ml Accuracy for water sampling for NIOSH 2-51,
 11032 L/S
 Approve 250 ml 6.5

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
 INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
 7-139 MOO 13, SOI SUTENAKORN 11 TAMBON BANG KAEO,
 AMPHOE BANG PHU SAMUT PRAKAN PROVINCE 10540 THAILAND
 TEL: (6690-2116-5860) FAX: (6690-2116-7140)



Certificate No : 22-AFM-039

Request No : Req-2022-0198

Result of Calibration :

Flow Setting	STD Flow Reading	UUC Flow Reading	Correction Flow	Uncertainty
(L/min)	(L/min)	(L/min)	(L/min)	(L/min)
1.6	1.586	1.57	0.016	0.024
10	9.99	9.40	0.59	0.14
20	19.98	18.94	1.04	0.28
50	50.1	48.10	2.0	1.3
100	99.9	95.02	4.8	2.5
150	150.4	145.83	4.6	3.9
200	200.2	192.71	7.5	5.2

Note

STD : Standard

UUC : Unit Under Calibration

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.00 Issue date 01/07/19

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 22P2729
Page : 1 of 2

Equipment : Aneroid Barometer
Manufacturer: Bargo
Model: 111MS
Serial No.: -
ID No.: UAE.EMA2.065/2552

Condition As-Received: Used Item

Received Date: 20 July 2022

Calibration Date: 22 July 2022

Reference: 2207-0584WSC Submitted by: United Analyst and Engineering Consultant Co., Ltd.

Ambient Temperature: $(23 \pm 2) ^\circ\text{C}$

Relative Humidity: $(50 \pm 15) \%$

Atmospheric Pressure: 1010 mbar

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using "DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505046	MP-0376-22	02 May 2023

2. This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3. This result of calibration was made on requested at the point specified by customer.

4. Scale and conversion factor is $1 \text{ kPa} = 7.50062 \text{ mmHg}$

5. This result of calibration instrument was in absolute pressure.

6. This instrument was used clean air as pressure media.

7. The certificate is valid only to the item calibrated on date and place of calibration.

8. This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suwit Aussarree
Issue Date : 25 July 2022

Approved Signatory : Attapol P.
[] Phalinee Prabpaipal
[] Sura Suwannasri
[x] Attapol Panurach

เอกสารไม่ควบคุม
B 0293210



Cert.No.: 22P2729
Page: 2 of 2

Result of calibration:- Without adjustment

Range : 720 mmHg to 770 mmHg

Function:- Absolute Pressure Measurement

Scale Interval : 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	715.65	726.13	737.65	748.11	759.89	772.31
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	760.0	770.0
Error (mmHg)	4.35	3.87	2.35	1.89	0.11	-2.31

Decreasing Pressure

Applied Pressure (mmHg)	772.35	759.90	748.14	737.68	726.16	715.69
UUC* Indication (mmHg)	770.0	760.0	750.0	740.0	730.0	720.0
Error (mmHg)	-2.35	0.10	1.86	2.32	3.84	4.31

The uncertainty of measurement was $\pm 0.24 \text{ mmHg}$

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม
a 1118528



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 22H1990
Page : 1 of 2

Equipment : Digital Thermo-Hygrometer
Manufacturer : Testo
Model : 608-H1
Serial No. : 34843033
ID No. : UAE.ANV.135/2550

Condition As-Received: Used Item

Received Date: 21 September 2022

Calibration Date: 23 September 2022
to 27 September 2022

Reference: 2209-0729WSC

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Hygro-M2 Dew Point Monitor	5112	2360195	20703	02 Aug 2023
2) Standard Humidity/Temperature Meter	400	10240757	TH-0125-21	13 Dec 2022

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained at:-

- National Institute of Standards and Technology (NIST) , The United States of America
- National Institute of Metrology Thailand (NIMT)

Calibrated by : Viporn Tantiyawutti
Issue Date : 29 September 2022

Approved Signatory :

[☒] Chakrit Waewanjua
[☐] Pornthippa Tameyakul
[☐] Viporn Tantiyawutti

เอกสารไม่ควบคุม

B 0298131

Q PASS
Q NOT PASS
Remarks: 23/09/2022
Temp = $\pm 0.5^\circ\text{C}$
%RH = $\pm 3\%$
Verify: [Signature]
Approve: [Signature]

2 N/A

เอกสารไม่ควบคุม



Cert. No.: 22H1990
Page: 2 of 2

Result of Calibration:-

Function: Humidity measurement. Without Adjustment

Reference Temperature	Standard Humidity	UUC* Reading	Error	Uncertainty of Measurement
(°C)	(%R.H.)	(%R.H.)	(%R.H.)	(±%R.H.)
25.0	40.1	44.7	4.6	1.3
25.0	50.1	53.4	3.3	1.6
25.0	60.0	62.7	2.7	1.6
25.0	70.2	71.9	1.7	1.6

Result of Calibration:-

Function: Temperature measurement. Without Adjustment

Standard Temperature	UUC* Reading	Error	Uncertainty of Measurement
(°C)	(°C)	(°C)	(±°C)
15.02	15.1	0.08	0.42
20.03	20.0	-0.03	0.42
25.02	25.0	-0.02	0.42
30.03	29.9	-0.13	0.42
40.03	39.7	-0.33	0.42

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-o0o-

[Signature]

เอกสารไม่ควบคุม
a 1128756

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/135 MOO 11, SOI SUTINAKORN 11 TAMBON BANG CAEO,
AMPHOE BANG PHI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (660-2116-5860-1 FAX: (660-2116-7140



Page 1 of 2.

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT
CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangehak,
Prakanong, Bangkok 10260

Certificate No : 22-ACT-524
Request No : Req-2022-1546

Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1
Manufacturer : SVANTEK Range : 94 , 114 dB / 1000 Hz
Model : SV 35 Instrument Status : Used
Serial Number : 44783
ID : UAE.EFM.019/2559

Calibration Environment and Details

Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 9 August 2022
Calibration Date : 19 August 2022
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	31 May 2023
THD Multimeter	2015	1047765	NIMT	2 February 2023

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By : *[Signature]*
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : *[Signature]*
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 19 August 2022

The results related only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม
a 1128756



เอกสารไม่ควบคุม

Certificate No : 22-ACT-524

Request No : Req-2022-1546

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	94.23	0.23	-	-	0.11	0.25
114 dB / 1000 Hz	114.23	0.23	-	-	0.11	0.25

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.10	0.70
114 dB / 1000 Hz	1000.00	0.00	-	-	0.10	0.70

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 1 (± %)
	Measured (%)	Measured (%)		
94 dB / 1000 Hz	0.05	-	0.40	2.5
114 dB / 1000 Hz	0.02	-	0.40	2.5

Note :

- Acceptance limit was IEC60942:2017 Class 1
- The calibration result exclude the calibrator pressure correction
- The calibration result exclude the microphone volume correction

End of Calibration

เอกสารไม่ควบคุม 07/15

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL23028

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00609500 / 189689 / 01126
ID No.: -

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND,

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 06 JANUARY 2023
Calibration Date : 10-12 JANUARY 2023
Date of Issue : 16 JANUARY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)



This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Continuation of Calibration Certificate

Cert. No. : ACL23028
Job No. : VC66AC0023
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม

T. Petch...

Continuation of Calibration Certificate

Cert. No. : ACL23028
Job No. : VC66AC0023
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long-term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

เอกสารไม่ควบคุม

T. Petch...

Continuation of Calibration Certificate

Cert. No. : ACL23028
Job No. : VC66AC0023
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
17.5

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	14.1
C - weight	20.6
Flat	26.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.0	0.0	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.2	0.3	0.3	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL23028
Job No. : VC66AC0023
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL23028
Job No. : VC66AC0023
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.1	0.1	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.2	0.2	± 1.1
28.0	28.2	0.2	± 1.1
27.0	27.3	0.3	± 1.1
26.0	26.3	0.3	± 1.1
25.0	25.4	0.4	± 1.1

เอกสารไม่ควบคุม

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23028
Job No. : VC66AC0023
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

เอกสารไม่ควบคุม

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23028
Job No. : VC66AC0023
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม

T. Petchurai

451-451/1 Sirinthorn Rd., Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel: 0-2435-8800 Fax: 0-2433-1679 e-mail: cal-center@sithiporn.com http://www.sithiporn.com

Cert. No. : ACL23031
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00709670 / 188531 / 01221
ID No.: -

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 06 JANUARY 2023
Calibration Date : 10 -12 JANUARY 2023
Date of Issue : 16 JANUARY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced
other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

		<input checked="" type="radio"/> PASS <input type="radio"/> NOT PASS
Remarks: Reception Limit (1000 Hz) = ± 1.0 dB		
Verify  1/1/66	Approve  1/1/66	

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23031
 Job No. : VC66AC0023
 Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
 The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
 For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.


3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม

QF-TS12-04-04-020664

เอกสารไม่ควบคุม



Continuation of Calibration Certificate

Cert. No. : ACL23031
Job No. : VC66AC0023
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long-term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

เอกสารไม่ควบคุม

Signature

Continuation of Calibration Certificate

Cert. No. : ACL23031
Job No. : VC66AC0023
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A-weight	11.6
C-weight	17.5
Flat	23.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.1	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.8	0.9	0.9	±5.0

เอกสารไม่ควบคุม

Signature

Continuation of Calibration Certificate

Cert. No. : ACL23031
Job No. : VC66AC0023
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

เอกสารไม่ควบคุม

T. Petch.

Continuation of Calibration Certificate

Cert. No. : ACL23031
Job No. : VC66AC0023
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

เอกสารไม่ควบคุม

T. Petch.

Continuation of Calibration Certificate

Cert. No. : ACL23031
Job No. : VC66AC0023
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

เอกสารไม่ควบคุม

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23031
Job No. : VC66AC0023
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม

7. Petch

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd, Bangbunru, Bangplud Bangkok 10700 THAILAND
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



Cert. No. : ACL22083

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01010777 / 194532 / 14655
ID No.: -

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 11 APRIL 2022
Calibration Date : 18-22 APRIL 2022
Date of Issue : 25 APRIL 2022

Calibrated by : Nathakorn Pisutpaisan

Approved by :


(Thanakul Petchurai)



This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Continuation of Calibration Certificate

Cert. No. : ACL22083
Job No. : VC65AC0045
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017075	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220075	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60924273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม

7. Reth

Continuation of Calibration Certificate

Cert. No. : ACL22083
Job No. : VC65AC0045
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

เอกสารไม่ควบคุม

7. Reth

Continuation of Calibration Certificate

Cert. No. : ACL22083
Job No. : VC65AC0045
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93,95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.6
C - weight	19.3
Flat	24.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.0	0.1	0.1	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	0.7	0.8	0.8	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22083
Job No. : VC65AC0045
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22083
Job No. : VC65AC0045
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±1.1
136.0	136.0	0.0	±1.1
135.0	135.0	0.0	±1.1
134.0	134.0	0.0	±1.1
133.0	133.0	0.0	±1.1
132.0	132.0	0.0	±1.1
131.0	131.0	0.0	±1.1
129.0	129.0	0.0	±1.1
124.0	124.0	0.0	±1.1
119.0	119.0	0.0	±1.1
114.0	114.0	0.0	±1.1
109.0	109.0	0.0	±1.1
104.0	104.0	0.0	±1.1
99.0	99.0	0.0	±1.1
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.1	0.1	±1.1
79.0	79.0	0.0	±1.1
74.0	74.1	0.1	±1.1
69.0	69.1	0.1	±1.1
64.0	64.0	0.0	±1.1
59.0	59.1	0.1	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.0	0.0	±1.1
39.0	39.0	0.0	±1.1
34.0	34.0	0.0	±1.1
30.0	30.0	0.0	±1.1
29.0	29.0	0.0	±1.1
28.0	28.0	0.0	±1.1
27.0	27.0	0.0	±1.1
26.0	26.0	0.0	±1.1
25.0	24.9	-0.1	±1.1

เอกสารไม่ควบคุม

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL22083
Job No. : VC65AC0045
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.1	0.1	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.3	-0.1	±2.0

เอกสารไม่ควบคุม

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL22083

Job No. : VC65AC0045

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

แผนการติดตามตรวจสอบคุณภาพสิ่งแวดล้อม ประจำปี พ.ศ. 2566

โครงการโรงงานผลิตลวดเหล็ก (ส่วนขยายครั้งที่ 2)

ระหว่างเดือนมกราคม-มิถุนายน พ.ศ. 2566

รายการใบรับรองสอบเทียบเครื่องมือหลักประจำห้องปฏิบัติการสำหรับวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือสำหรับวิเคราะห์คุณภาพน้ำ และดิน									
1	pH Meter	pH Temperature	Hanna Instrument	HI2211 / 8165345	National Food Institute, Ministry of Industry, Thailand	2202097-001-01	16 Mar 22	15 Mar 23	-
2	pH Meter		Mettler-Toledo	Seven Easy S20 / 1231155210	National Food Institute, Ministry of Industry, Thailand	2301846-001-01	24 Feb 23	23 Feb 24	-
3	BOD Incubator	Biochemical Oxygen Demand	Arco	UC4-1320 / (UAE.WAO.002/2550)	Technology Promotion Association (Thailand-Japan)	22TM1232	15 Aug 22	14 Aug 23	-
4	BOD Incubator		Arco	UC4-1320 / (UAE.WAO.018/2559)	Technology Promotion Association (Thailand-Japan)	22TM1233	15 Aug 22	14 Aug 23	-
5	Analytical Balance (Readability 0.01 mg)	Total Suspended Solids Total Dissolved Solids	Mettler-Toledo	XSR205DU / C210685394	Technology Promotion Association (Thailand-Japan)	23MM113	26 Apr 23	24 Apr 24	-
6	Hot Air Oven		Memmert	UF55 / B216.1666	Technology Promotion Association (Thailand-Japan)	22TM1490	19 Oct 22	18 Oct 23	-
7	Analytical Balance (Readability 0.1 mg)	Fat oil & Grease	Mettler-Toledo	XSR204 / C117635043	National Food Institute, Ministry of Industry, Thailand	2302827-001-01	10 May 23	8 May 24	-
8	Conductivity Meter	Conductivity	SI Analytics	Lab955 / 16300356	DKSH Technology Limited	C24230059	16 Mar 23	14 Mar 24	-
9	UV-VIS Spectrophotometer	Phenol, Ammonia Nitrogen,Sulphate, Nitrate Nitrogen,Phosphate,	Agilent Technologies	Cary60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP23-021	20 May 23	18 May 24	-
10	UV-VIS Spectrophotometer		Hitachi	U-1900 / 2021-064	DQE Services Co.,Ltd.	SP23-007	6 Jan 23	5 Jan 24	-
11	UV-VIS Spectrophotometer		Hitachi	U-2900 / 21E22-009	DQE Services Co.,Ltd.	SP23-008	6 Jan 23	5 Jan 24	-

บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

ห้องปฏิบัติการวิเคราะห์มาตรฐาน ISO/IEC 17025

รายการใบรับรองสอบเทียบเครื่องมือหลักประจำห้องปฏิบัติการสำหรับวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือสำหรับวิเคราะห์คุณภาพน้ำ และดิน									
12	Atomic Absorption Spectrophotometer (AAS)	Lead, Chromium, Hexavalent, Mercury, Copper, Zinc, Nickel, Iron, Fe, Zinc, Chromium Trivalent, Manganese	Perkin Elmer	PinAAcle 900F / PFBS20031902	Perkin Elmer Co.,Ltd.	PM Service No. WO-01710010	20 Jul 22	19 Jul 23	-
13	Inductively Coupled Plasma (ICP)		Agilent Technologies	System ID:G8015A G8015AA / MY18030001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	30 Nov 22	29 Nov 23	-
14	Cold Vapor Atomic (CVAAS)	Mercury	Milestone	DMA-80 / 11030982	Sithiporn Associates Co.,Ltd.	Service Protocol Report	18 Nov 22	17 Nov 23	-
15	Incubator (Cooled Incubator)	Fecal Coliform Total Coliform Bacteria	Binder	BD 53 / 13-07343	Technology Promotion Association (Thailand-Japan)	23TM192	16 Feb 23	15 Feb 24	-
16	Incubator (Cooled Incubator)		Memmert	INB400 / E411.1325	Technology Promotion Association (Thailand-Japan)	22TM1063	11 Jul 22	10 Jul 23	-
17	Incubator		Memmert	BE400 / e402.1032	Technology Promotion Association (Thailand-Japan)	22TM1064	11 Jul 22	10 Jul 23	-
18	Water Bath		Memmert	WNE 14 / L416.0614	Technology Promotion Association (Thailand-Japan)	23TM250	16 Feb 23	15 Feb 24	-
19	Water Bath		Memmert	WB 14 / I401.0569	Technology Promotion Association (Thailand-Japan)	22TM1065	11 Jul 22	10 Jul 23	-
20	Auto Clave		ALP	CL-40L / 807298	Technology Promotion Association (Thailand-Japan)	22TM1121	11 Jul 22	10 Jul 23	-

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.

แผนการติดตามตรวจสอบคุณภาพสิ่งแวดล้อม ประจำปี พ.ศ. 2566

โครงการโรงงานผลิตลวดเหล็ก (ส่วนขยายครั้งที่ 2)

ระหว่างเดือนมกราคม-มิถุนายน พ.ศ. 2566

รายการใบรับรองสอบเทียบเครื่องมือหลักประจำห้องปฏิบัติการสำหรับวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือสำหรับวิเคราะห์คุณภาพอากาศ									
1	Analytical Balance (Repeatability 0.1 mg)	TSP, PM ₁₀	Mettler-Toledo	AB204-S / 1128312528	Mettler-Toledo (Thailand) Ltd.	23MM331	7 Apr 23	5 Apr 24	-
2	Analytical Balance (Repeatability 0.1 mg)		Mettler-Toledo	AB204-S/FACT / B108115858	Mettler-Toledo (Thailand) Ltd.	23MM332	7 Apr 23	5 Apr 24	-
3	Analytical Balance (Readability 0.001 mg)	Respirable Dust Total Dust	Mettler-Toledo	XP6 / B322373893	Mettler-Toledo (Thailand) Ltd.	23MM333	7 Apr 23	5 Apr 24	-
4	UV-VIS Spectrophotometer	NO _x as NO ₂	Agilent Technologies	Cary60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP22-016	31 May 22	30 May 23	-
5	UV-VIS Spectrophotometer		Hitachi	U-1900 / 2021-064	DQE Services Co.,Ltd.	SP23-007	6 Jan 23	5 Jan 24	-
6	Ion Chromatrography (IC)	HCL	Dionex	DX-120 / 03010223	Archemica Lab Co.Ltd.	Qualification Report Anion (ID#042)	9 Dec 22	8 Dec 23	-

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.



National Food Institute, Ministry of Industry, Thailand

2008 Soi 36, Anu Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel : +66 (0) 2422 8588 Fax : +66 (0) 2422 8558 Website : www.nfi.or.th E-mail : cal@nfi.or.th



Calibration Certificate

Certificate No.: 2202097-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakanong, Bangkok 10260

Page 1 of 5

Equipment: pH Meter
Manufacturer: HANNA INSTRUMENTS
Model: HI 2211
Serial No.: 08165345
ID No.: UAE.WAT.004/2556
Order No.: 2202097
Operation No.: 2202097-001
Date of Receipt: 11 March 2022
Date of Calibration: 16 March 2022

Calibrated by Mr.Manas Somsak Specialist
Approved by (Mr.Pheraphat Tuanjit) Manager, Division of Calibration Laboratory
Date of Issue: 21 March 2022 Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full, except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 00 Date: 14-12-61

เอกสารไม่ควบคุม



National Food Institute, Ministry of Industry, Thailand

2008 Soi 36, Anu Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel : +66 (0) 2422 8588 Fax : +66 (0) 2422 8558 Website : www.nfi.or.th E-mail : cal@nfi.or.th



Calibration Report

Certificate No.: 2202097-001-01
Equipment: pH Meter Resolution: 0.01 pH ; 0.1/1 mV
Manufacturer: HANNA INSTRUMENTS Model: HI 2211
Serial No.: 08165345 Type: Bench top
ID No.: UAE.WAT.004/2556

Date of Calibration: 16 March 2022 Page 2 of 5

Location: Chemical Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature: (23.0 ± 1.5) °C Relative Humidity: (49.5 ± 5) %
Condition of Equipment: Good Condition

Condition of this Results of Calibration

1. Calibration Method In house method : W-CC-002 based on direct measurement by using standard voltage calibrator and certified reference material (CRM)
2. Reference Standards / Certified Reference Material

Instruments	Serial / ID No.	Manufacturer	Certificate No.	Due Date
2.1 DC Voltage Calibrator	2709007	Fluke	ISCL-21 F-0687	24 June 2022
2.2 Digital Thermometer	2709007	Fluke	DC-640599-01	30 October 2022
2.3 Thermo-Hygro Meter	ana.hi.BTH 005/58	PONPE	QR21-2787	15 November 2022

Certified Reference Material	Lot No.	Manufacturer	Ref N	Expire Date
2.4 pH buffer 4.008 (Primary pH buffer Solution)	780012	CPAchem	PH216.L5	21 November 2023
2.5 pH buffer 6.865 (Primary pH buffer Solution)	780013	CPAchem	PH217.L5	21 November 2023
2.6 pH buffer 10.01 (Primary pH buffer Solution)	780015	CPAchem	PH220.L5	21 November 2022
2.7 pH buffer 7.00 (Standard pH buffer Solution)	775840	CPAchem	PH107.L5	8 November 2022

3. This certification is traceable to The International System of Unit (SI Unit)

3.1 Instruments No.2.1	through	VSC-TISI-TIS 17225 Laboratory Accreditation of Calibration No.0075
3.2 Instruments No.2.2	through	VSC-TISI-TIS 17225 Laboratory Accreditation of Calibration No.0061
3.3 Instruments No.2.3	through	VSC-TISI-TIS 17225 Laboratory Accreditation of Calibration No.0292
3.4 Certified Reference Material No. 2.4 to 2.6	traceable to	Primary measurement method: Harned cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.5 Certified Reference Material No. 2.7	traceable to	SIM RefN HI-7 LotN 30.04.2020; BIM RefN HI-9 LotN 28.05.2020; BIM RefN HI-E LotN 30.04.2020; BIM RefN HI-10 LotN 28.05.2020. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

F-CS-012 Revision: 00 Date: 14-12-61

เอกสารไม่ควบคุม



National Food Institute, Ministry of Industry, Thailand

200 Anusorn Road, Bang Phli District, Bangkok 10700, Thailand
(T) 2428 6553 Fax: +66 (0) 2428 6553 Website: www.nfi.or.th E-mail: cal@nfi.or.th



National Food Institute, Ministry of Industry, Thailand

200 Anusorn Road, Bang Phli District, Bangkok 10700, Thailand
(T) 2428 6553 Fax: +66 (0) 2428 6553 Website: www.nfi.or.th E-mail: cal@nfi.or.th



Calibration Report

Certificate No.: 2202187-001-01
Equipment: pH Meter
Resolution: 0.01 pH ; 0.01 mV
Manufacturer: HANNA INSTRUMENTS
Model: HI 2311
Serial No.: 08165345
Type: Bench top
ID No.: UAE.WAT.004/2556
Date of Calibration: 18 March 2022 Page 3 of 5

Calibration Results

1. Calibration of pH Meter (Manual Temperature Compensation at 25 °C)

Nominal pH	OC Voltage Standard (mV)	Average Indicator Reading		Uncertainty (±mV)	Coverage Factor (k)
		mV	pH		
0	+14.117	414	0.00	0.58	2.00
2	295.811	295.7	2.00	0.063	2.00
4	177.462	177.4	4.00	0.063	2.00
6	59.159	59.2	6.00	0.063	2.00
7	-0.001	0.1	7.00	0.063	2.00
8	-59.169	-59.1	8.00	0.063	2.00
10	-177.463	-177.3	10.00	0.063	2.00
12	-295.812	-295.6	12.00	0.063	2.00
14	-414.119	-414	14.00	0.58	2.00

2. Calibration of pH Meter with Electrode (Manual Temperature Compensation at 25 °C)

Equipment: pH Electrode
Type: Combined Electrode
Manufacturer: METTLER TOLEDO
Model: LE420
Serial No.: 11A2602
ID No.: N/A

Performance of Electrode system (Three-Point Calibration at pH4, pH7 and pH10)

Certified Value (25 °C (pH))	Average Indicator Reading		Relative Slope (%)	Uncertainty (±pH)	Coverage Factor (k)
	pH	mV			
4.003	4.01	180.5	99.3	0.0071	2.00
6.863	6.87	12.5	-	0.0074	2.00
10.015	10.01	-171.5	99.4	0.0098	2.00
6.863	6.89	5.2	-	0.0092	2.00

Calibration Report

Certificate No.: 2202097-001-01
Equipment: Digital Thermometer with RTD (pH Meter)
Resolution: 0.1 °C
Mode: HI 2211
Serial No.: 08165345
ID No.: UAE.WAT.004/2556
Manufacturer: HANNA INSTRUMENTS
Date of Calibration: 18 March 2022 Page 4 of 5

Location: Chemical Calibration Laboratory, National Food Institute.

Environment Condition:
Ambient Temperature (23.0 ± 1.0) °C
Relative Humidity (50 ± 4) %

Condition of this results of Calibration:

1. Calibration Method:
 - In house method: W-TE-025 by comparison with standard thermometer.
 - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
 - The temperature scale in use at this laboratory is the International Temperature scale of 1990 (ITS-90)

2. Reference Standard Instrument:

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1523	2118154	PSL-T 0821/64	24-Jun-22	TISTR
Platinum Resistance Thermometer (PRT)	5627A	877332			

Support Equipment: - Low Temperature Bath (ISOCAL-6), Model: Europa-6 Plus Basic, S/N: 341592/2

3. This certificate is traceable to International System of Units (SI Units)
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and piece of calibration only.

6. Condition of Calibrated item: Good
7. Result of Calibration: ☒ Without adjustment ☐ After adjustment



National Food Institute, Ministry of Industry, Thailand

2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel : +66 (0) 2422 8588 Fax : +66 (0) 2422 8558 Website : www.nfi.or.th E-mail : cal@nfi.or.th



Calibration Report

Certificate No.: 2202097-001-01
Equipment: Digital Thermometer with RTD (pH Meter)
Resolution: 0.1 °C Model: HI 2211
Serial No.: 08165345 ID No.: UAE.WAT.004/2556
Manufacturer: HANNA INSTRUMENTS

Date of Calibration: 18 March 2022 Page 5 of 5

Calibration point: 15.0, 25.0 and 35.0 °C

Calibration result:

- The probe was immersed in liquid bath or dry bath to a minimum depth of 100 mm.

- Description of probe, model: N/A S/N: N/A

Dimension of probe: Diameter 3.5 mm, Length 100 mm.

Sheath material: Stainless Steel

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.0	15.0C1	0.0	0.099
25.0	25.0C2	0.0	0.099
35.0	35.0C2	0.0	0.099

Note - UUC* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k=2$, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 00 Date: 14-12-61

เอกสารไม่ควบคุม



ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center



Calibration Certificate

Certificate No.: 2301846-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakanong, Bangkok 10260

Page 1 of 5

Equipment: pH Meter
Manufacturer: Mettler Toledo
Model: SevenEasy TM S20 pH
Serial No.: 1231155210
ID No.: UAE.WAT.010/2553
Order No.: 2301846
Operation No.: 2301846-001
Date of Receipt: 17 February 2023
Date of Calibration: 24 February 2023

Calibrated by Mr.Worapob Socktong
Scientist
Approved by N. Niyomchart
(Mr.Nutapoi Niyomchart)
Specialist, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 24 February 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2008 ซอย 36, ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel : +66(0) 2422 8588 Fax : +66(0) 2422 8558

เอกสารไม่ควบคุม



nfi.or.th

Calibration Report

Certificate No.: 2301846-001-01
Equipment: pH Meter
Resolution: 0.01 pH ; 1 mV
Manufacturer: Mettler Toledo
Model: SevenEasy TM S210 pH
Serial No.: 1231155210
Type: Bench top
ID No.: UAE.WAT.010/2553

Date of Calibration: 24 February 2023 **Page 2 of 5**

Location: Chemical Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature: (25.1 ± 1.5) °C Relative Humidity: (50 ± 5) %
Condition of Equipment: Good Condition

Condition of this Results of Calibration

1. Calibration Method In house method : W-CO-002 based on direct measurement by using standard voltage calibrator and certified reference material (CRM)

2. Reference Standards / Certified Reference Material

Instruments	Serial / ID No.	Manufacturer	Certificate No.	Due Date
2.1 DC Voltage Calibrator	2709007	Fluke	22E1959	17 June 2023
2.2 Digital Thermometer	2709007	Fluke	CC 650577-01	30 October 2023
2.3 Thermo-Hygro Meter	NFLBTH 00718	PONPE 490	QR22-0866	26 April 2023
Certified Reference Material	Lot No.	Manufacturer	Ref N	Expire Date
2.4 pH buffer 4.008 (Primary pH buffer Solution)	832506	CPAchem	PH216.L5	8 August 2024
2.5 pH buffer 6.865 (Primary pH buffer Solution)	832507	CPAchem	PH217.L5	8 August 2024
2.6 pH buffer 10.01 (Primary pH buffer Solution)	832309	CPAchem	PH220.L5	8 August 2023
2.7 pH buffer 7.00 (Standard pH buffer Solution)	832510	CPAchem	PH107.L5	8 August 2023

3. This certification is traceable to The International System of Unit (SI Unit)

3.1 Instruments No.2.1	through	NSC-TISI-TS 17025 Laboratory Accreditation of Calibration No.0008
3.2 Instruments No.2.2	through	NSC-TISI-TS 17025 Laboratory Accreditation of Calibration No.0061
3.3 Instruments No.2.3	through	NSC-TISI-TS 17025 Laboratory Accreditation of Calibration No.0292
3.4 Certified Reference Material No. 2.4 to 2.6	traceable to	Primary measurement method- Harned cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.5 Certified Reference Material No.2.7	traceable to	BIM RefN HI-27 LotN 04.06.2021; BIM RefV HI-38 LotN 28.05.2021; BIM RefN HI-27 LotN 04.06.2021; BIM RefV HI-38 LotN 28.05.2021, the Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

F-C5-012 Revision: 01 Date: 20-04-65

N. nigudat



Calibration Report

Certificate No.: 2301846-001-01
Equipment: pH Meter
Resolution: 0.01 pH ; 1 mV
Manufacturer: Mettler Toledo
Model: SevenEasy TM S210 pH
Serial No.: 1231155210
Type: Bench top
ID No.: UAE.WAT.010/2553

Date of Calibration: 24 February 2023 **Page 3 of 5**

Calibration Results:

1. Calibration of pH Meter (Manual Temperature Compensation at 25 °C)

Nominal pH	DC Voltage Standard (mV)	Average Indicator Reading		Uncertainty (±mV)	Coverage Factor (k)
		mV	pH		
0	414.120	414	0.00	0.58	2.00
2	295.614	296	2.00	0.58	2.00
4	177.484	178	4.00	0.58	2.00
6	59.160	59	6.00	0.58	2.00
7	0.000	0	7.00	0.58	2.00
8	-59.158	-59	8.00	0.58	2.00
10	-177.490	-177	10.00	0.58	2.00
12	-295.811	-296	12.00	0.58	2.00
14	-414.117	-414	14.00	0.58	2.00

2. Calibration of pH Meter with Electrode (Manual Temperature Compensation at 25 °C)


Equipment: pH Electrode **Type:** Combined Electrode
Manufacturer: Mettler Toledo **Model:** InLab SoliS
Serial No.: 9018311 **ID No.:** N/A

Performance of Electrode system (Three-Point Calibration at pH 4, 7 and 10 pH)

Certified Value @25 °C (pH)	Average Indicator Reading		Rising Slope (%)	Uncertainty (± pH)	Coverage Factor (k)
	pH	mV			
4.003	4.01	186	-	0.0071	2.00
6.865	6.90	16	11.68	0.0075	2.00
10.008	10.01	-160	17.29	0.0095	2.00
6.865	6.99	16	-	0.0092	2.00

F-C5-012 Revision: 01 Date: 20-04-65

N. nigudat



Calibration Report

Certificate No.: 2301846-001-01
Equipment: Digital Thermometer with RTD
 Resolution: 0.1 °C Model: SevenEasy TM 520 pH
 Serial No.: 1231155210 ID No.: UAE.WAT.010/2553
 Manufacturer: Mettler Toledo
Date of Calibration: 24 February 2023

Page 4 of 5

Location: Chemical Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature 25 °C ± 1 °C
 Relative Humidity 48 % ± 3 %

Condition of this results of Calibration:

- Calibration Method : - In house method: W-TE-025 by comparison with standard thermometer.
 - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
 - The temperature scale in use at this laboratory is the International Temperature scale of 1990 (ITS-90).

2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1523	2118154	PSL-T 0673/65	07-Jun-23	TISTR
Platinum Resistance Thermometer (PRT)	5627A	877332			

Support Equipment : - Low Temperature Bath (Micro Bath), Model: 7103, S/N: A39533, AN65 A85181.

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good
- Result of Calibration : ☒ Without adjustment ☐ After adjustment

N. Inpradit

F-CS-012 Revision: 01 Date: 20-04-65



nfi.or.th

เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2301846-001-01
Equipment: Digital Thermometer with RTD
 Resolution: 0.1 °C Model: SevenEasy TM 520 pH
 Serial No.: 1231155210 ID No.: UAE.WAT.010/2553
 Manufacturer: Mettler Toledo
Date of Calibration: 24 February 2023

Page 5 of 5

Calibration point: 15.0, 25.0 and 35.0 °C
Calibration result:

- The probe was immersed in liquid bath or dry bath to a minimum depth of 120 mm.
- Description of probe, model : - S/N : -
 Dimension of probe : Diameter 9 mm., Length 120 mm.,
 Sheath material : Stainless Steel

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.1	15.015	- 0.1	0.11
25.0	25.014	0.0	0.11
35.1	35.015	- 0.1	0.11

Note

- UUC* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

N. Inpradit

F-CS-012 Revision: 01 Date: 20-04-65



nfi.or.th

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUI, LUMMI BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-4464



Cert. No.: 22TM1232
Page.: 1 of 3

Certificate of Calibration

Equipment : BCD Incubator
Manufacturer : Arco
Model : UC4-1320
Serial No. : -
ID No. : UAE.WAO.002/2550
Submitted by : United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Lab Floor 2
Received Order : 15 August 2022
Calibration Date : 15 August 2022
Ambient Temperature : $(26 \pm 10) ^\circ\text{C}$
Relative Humidity : $(50 \pm 30) \%$
Calibrated by : Kundhit Promprat

Approved by : Malee
Approved Signatory

() Pornthippa Tameyakul
() Malee Bulkruea
() Suwit Imjai

Issue Date : 16 August 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced or further used without the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0044201



Equipment : BOD Incubator
Condition As Received : Used Item
Reference : 2203-0186QC-1
Procedure Used :-

Cert. No.: 22TM1232
Page.: 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard Instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44035217	21LM30	23 Dec 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

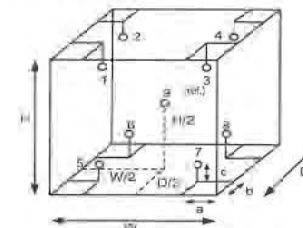

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.53 m
W = 1.2 m
H = 1.2 m
Capacity = 0.76 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	26
REL.Humid. (%)	81	83
AC Supply (Volt)	227	227

Position :	Ref. Std. ID No.:
1	18-10RTD-01
2	18-10RTD-02
3	18-10RTD-03
4	18-10RTD-04
5	18-10RTD-05
6	18-10RTD-06
7	18-10RTD-07
8	18-10RTD-08
9 (ref.)	18-10RTD-09

เอกสารไม่ควบคุม

A 0044201



Equipment : BOD Incubator
 Condition As-Received : Used Item
 Reference : 2208-01B6QC-1
 Result of Calibration : (*) Without Adjustment
 Function of UUC* : Temperature Source
 Fresh air setting : Not Available

Cert. No.: 22TM1232
 Page.: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
20.0	18.6	19.5	0.38	0.39	1.1	0.70	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
20.0	20.050	20.264	19.851	19.771	19.828	20.169	19.886	19.829	20.001

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

Malu

เอกสารไม่ควบคุม

A 121246



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
 CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
 53/44 PATTANAKARN ROAD BOI 18, SUANLUANG, BANGKOK 10250
 TEL. 0-2717-3000-27 FAX. 0-27791348



Cert. No.: 22TM1233
 Page.: 1 of 3

Certificate of Calibration

Equipment : BOD Incubator
 Manufacturer : Arco
 Model : UC4-1320
 Serial No. : -
 ID No. : UAE.WAO.018/2559
 Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangchak, Phrakhanong,
 Bangkok 10260
 Location : Lab Floor 2
 Received Order : 15 August 2022
 Calibration Date : 15 August 2022
 Ambient Temperature : (26 ± 10) °C
 Relative Humidity : (50 ± 30) %
 Calibrated by : Kunchit Prompret

Approved by : *Malu*
 Approved Signatory
 (/) Pornthippa Tamayakul
 (/) Malee Bulkruea
 () Suwit Imjai

Issue Date : 16 August 2022

The Uncertainties are for a confidence probability of approximately 95 %

This certificate may not be reproduced other than in full, except with the prior written
 Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0044202



Equipment : BOD Incubator
 Condition As-Received : Used Item
 Reference : 2208-0186OC-2

Cert. No.: 22TM1233
 Page.: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44035217	21LM30	23 Dec 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

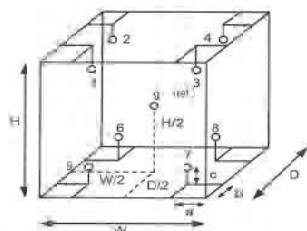

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	28
REL.Humid. (%)	65	62
AC Supply (Volt)	227	227

Position :	Ref. Std. ID No.:
1	18-10RTD-01
2	18-10RTD-02
3	18-10RTD-03
4	18-10RTD-04
5	18-10RTD-05
6	18-10RTD-06
7	18-10RTD-07
8	18-10RTD-08
9 (ref.)	18-10RTD-09

Probe Installation Details :

a = 10 cm
 b = 10 cm
 c = 10 (mm)

Dimension of Chamber :

D = 0.53 m
 W = 1.2 m
 H = 1.2 m
 Capacity = 0.76 m³

เอกสารไม่ควบคุม

a 1121245



Equipment : BOD Incubator
 Condition As-Received : Used Item
 Reference : 2208-0186OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 22TM1233
 Page.: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
20.0	19.8	19.7	0.31	0.29	0.77	0.64	2

Calibration Point (°C)	Measured Temperature (°C)							
	Position							
	1	2	3	4	5	6	7	8
20.0	19.956	19.783	19.988	19.842	19.843	19.908	19.770	19.910
								19.824

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-๑๑๐-

เอกสารไม่ควบคุม

a 1121244




TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
53/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9444



Cert.No.: 23MM113
Page.: 1 of 3

Certificate of Calibration

Equipment : Electronic Balance
Manufacturer : Mettler Toledo
Model : XSR205
Serial No. : C210685394
ID No. : UAE.WAO.010/2565
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phakhanong,
Bangkok 10260
Location : Balance Room
Received order : 26 April 2023
Calibration Date : 26 April 2023
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 90 %
Calibrated by : Man Pattanapongpaiboon
Approved by : 
Approved Signatory
() Pornthippa Tameyakul
() Malee Butkruea
(✓) Suwit Imjai
Issue Date : 2 May 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-04590C-2
Procedure used :-

Cert.No.: 23MM113
Page: 2 of 3

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0010-22	20 Jan 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This result of calibration was made on requested at the point specified by customer.

4. This certificate is not certified for any commercial transaction.

5. This certification is traceable to the International System of Unit.

Result of calibration () Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity :	0 g to 81 g	Resolution	0.00001 g
	81 g to 220 g	Resolution	0.0001 g

Before Adjustment :

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
(g)	(g)	(g)	(± mg)	(k)
80	79.99992	-0.00008	0.15	2.00
200	199.9995	+0.0005	0.29	2.00

After Adjustment :

1. Determination of the standard deviation of weighing machine (n = 10)

Applied Weight	Standard Deviation of Reading (g)
(g)	
80	0.000007
200	0.00004

เอกสารไม่ควบคุม




Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0459OC-2

Result of calibration

2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.
The weighing machine reading error obtained is given in the table

Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)
-0.0001	-0.0001	0.0000	-0.0001	-0.0001



Maximum difference between
off-center and central loading
(g)
0.0001

3. Departure from nominal value

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
Unload	0.00000	0.00000	0.014	2.11
0.05	0.04999	+0.00001	0.015	2.09
0.1	0.09999	+0.00001	0.015	2.07
1	1.00000	0.00000	0.018	2.04
5	5.00000	0.00000	0.026	2.00
20	20.00002	-0.00002	0.045	2.00
50	50.00002	-0.00002	0.080	2.00
80	80.00002	-0.00002	0.15	2.00
100	100.00000	0.00000	0.17	2.00
150	150.00000	0.00000	0.29	2.00
200	199.99999	+0.00001	0.29	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 FATTANAKARN ROAD MOI 18, SUANLUANG, SUANLUANG BAN KOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1490

Page : 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven
Manufacturer : Memmert
Model : UF 55
Serial No. : B216.1666
ID No. : UAE.WAO.027/2559
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Lab Floor 2
Received Order : 19 October 2022
Calibration Date : 19 October 2022
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Preecha Hlahib
Approved by :
() Ponthippa Tameyakul
() Malee Butkruea
(✓) Suwit Imjai

Issue Date : 31 October 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0046800



Equipment : Hot Air Oven
 Condition As-Received : Used Item
 Reference : 2210-0575OC-1

Cert. No : 22TM1490
 Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY41021843	22LM4	10 Jan 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close



Probe Installation Details :

a = 5.0 cm	D = 0.33 m
b = 5.0 cm	W = 0.40 m
c = 5.0 cm	H = 0.40 m
	Capacity = 0.053 m ³

Dimension of Chamber :

Environment during calibration		
	Beginning	Finished
Temp. (°C)	29	30
REL.Humid. (%)	47	40
AC Supply (Volt)	221	220

Position :	Ref. Std. ID No. : @ Calibration Point	
	(104) °C	(140,180) °C
1	18-04RTD-01	21-04TC-01
2	18-04RTD-02	21-04TC-02
3	18-04RTD-03	21-04TC-03
4	18-04RTD-04	21-04TC-04
5	18-04RTD-05	21-04TC-05
6	18-04RTD-06	21-04TC-06
7	18-04RTD-07	21-04TC-07
8	18-04RTD-08	21-04TC-08
9 (ref.)	18-04RTD-09	21-04TC-09

เอกสารไม่ควบคุม

1133252



Equipment : Hot Air Oven
 Condition As-Received : Used Item
 Reference : 2210-0575OC-1

Cert. No : 22TM1490
 Page : 3 of 3

Result of Calibration :-

(*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
104.0	104.0	104.0	0.061	1.3	1.7	0.42	2
140.0	140.0	140.0	0.14	2.3	2.4	1.1	2
180.0	180.0	180.0	0.21	3.5	3.6	1.3	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	103.076	103.876	103.777	104.124	104.667	104.426	104.012	103.928	104.370
140.0	138.199	139.189	139.808	139.550	140.266	139.622	139.293	139.385	140.369
180.0	177.930	179.267	178.643	179.753	181.011	180.083	179.496	179.743	181.278

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k providing a level of confidence of approximately 95 %.

1000-

เอกสารไม่ควบคุม

1133251

Calibration Certificate

Certificate No.: 2302827-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangchak, Phrakhanong, Bangkok 10260

Page 1 of 4

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR204
Serial No.: C117635043
ID No.: UAE.WAS.012/2564
Order No.: 2302827

Operation No.: 2302827-001
Date of Receipt: 10 May 2023
Date of Calibration: 10 May 2023

Calibrated by Mr.Manas Somsak
 Specialist

Approved by 
 (Mr.Pheraphat Tuanjit)
 Manager, Division of Calibration Laboratory
 Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2302827-001-01
Equipment: Electronic Balance
Model: XSR204
Serial No.: C117635043
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.0001 g
ID No.: UAE.WAS.012/2564

Page 2 of 4

Date of Calibration: 10 May 2023

Environment Condition: Ambient Temperature: 21.4 ± 0.2 °C Relative Humidity: 43.4 ± 0.9 %

Place of Calibration: Balance room (Water Analysis Unit), UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M23040535	8 April 2024
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFLBTH 016/23	Quality Reborn	QR23-0489	21 February 2024

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
100	0.000032
200	0.000032

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table

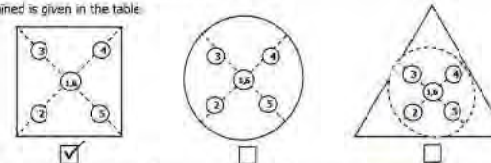

1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100.0002	100.0002	100.0002	100.0002	100.0003	100.0002	0.0001

F-CS-012 Revision: 01 Date: 20-04-65



nfi.or.th

เอกสารไม่ควบคุม



nfi.or.th

เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2302827-001-01

Equipment:

Electronic Balance

Manufacturer: METTLER TOLEDO

Model: XSR204

Resolution: 0.0001 g

Serial No.: C117635043

ID No.: UAE.WAS.012/2564

Capacity: 220 g

Date of Calibration: 10 May 2023

Page 3 of 4

Calibration Results: (Continued)

Calibration Range: 0 - 200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.00000	0.0000	0.0000	0.000085	2.00
0.01	0.01000	0.0100	0.0000	0.000085	2.00
0.02	0.02001	0.0200	0.0000	0.000085	2.00
0.05	0.05000	0.0500	0.0000	0.000085	2.00
0.1	0.10001	0.1000	0.0000	0.000085	2.00
0.2	0.20001	0.2000	0.0000	0.000085	2.00
0.5	0.50002	0.5000	0.0000	0.000085	2.00
1	1.00000	1.0000	0.0000	0.000086	2.00
2	2.00002	2.0000	0.0000	0.000086	2.00
3	3.00003	3.0000	0.0000	0.000087	2.00
5	5.00002	5.0000	0.0000	0.000087	2.00
10	10.00001	10.0000	0.0000	0.000088	2.00
20	20.00003	20.0000	0.0000	0.000092	2.00
30	30.00004	30.0000	0.0000	0.000098	2.00
40	40.00007	40.0000	0.0000	0.00011	2.00
45	45.00009	45.0001	0.0000	0.00013	2.00

FCS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม



nfi.or.th

Calibration Report

Certificate No.: 2302827-001-01

Equipment:

Electronic Balance

Manufacturer: METTLER TOLEDO

Model: XSR204

Resolution: 0.0001 g

Serial No.: C117635043

ID No.: UAE.WAS.012/2564

Capacity: 220 g

Date of Calibration: 10 May 2023

Page 4 of 4

Calibration Results: (Continued)

Calibration Range: 0 - 200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
50	50.00003	50.0000	0.0000	0.00011	2.00
55	55.00005	55.0000	0.0000	0.00012	2.00
60	60.00004	60.0000	0.0000	0.00012	2.00
65	65.00005	65.0000	0.0000	0.00013	2.00
70	70.00006	70.0001	-0.0001	0.00013	2.00
75	75.00008	75.0002	-0.0001	0.00013	2.00
80	80.00007	80.0002	-0.0001	0.00014	2.00
85	85.00009	85.0002	-0.0001	0.00014	2.00
90	90.00010	90.0002	-0.0001	0.00015	2.00
100	100.00006	100.0002	-0.0001	0.00016	2.00
120	120.00009	120.0002	-0.0001	0.00018	2.00
150	150.00009	150.0002	-0.0001	0.00021	2.00
200	200.00016	200.0003	-0.0001	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

End

FCS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม



nfi.or.th



Certificate of Calibration



Equipment: CONDUCTIVITY METER
Model: Lab 955
Serial No. (or ID.): 16300356
Manufacturer: SI Analytics
Electrode Serial No.: 16070067
Condition: In Condition

Certificate No.: C24230059
Issued Date: 16 March 2023
Job No.: KSPR2304472
Page: 1 of 2
Model: LF413T **Brand:** SI Analytics

Customer: United Analyst and Engineering Consultant Company Limited
3 Soi Udomsuk 41 Sukhumvit Road,
Bangkok, Prakanong, Bangkok 10260 Thailand

Environment Condition: Temperature 23 °C ± 2 °C
Humidity 50 %RH ± 15 %RH

Calibration Place: Environment Laboratory, DKSH Technology Limited,
2533 Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Mr Atachai Ngamchanai
Calibration Date: 16 March 2023
The Method used: In house method, CAL-WI-09, base on ASTM D 1125-14 and D 5391-14

Traceability: This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through
CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 838312, 838313, 838316

Certificate No.: C24230059

Page: 2 of 2

Calibration Results:

Before Adjustment

Standard Conductivity Solution	Unit Under Calibration Reading	Correction	Coverage Factor (k)	Uncertainty (±)
25.000 µS/cm	24.5 µS/cm	0.500 µS/cm	2.00	0.21 µS/cm
1413.0 µS/cm	1403 µS/cm	10.0 µS/cm	2.00	9.0 µS/cm
111.3 mS/cm	108.5 mS/cm	2.80 mS/cm	2.00	0.67 mS/cm

After Adjustment: at 1413 µS/cm

Standard Conductivity Solution	Unit Under Calibration Reading	Correction	Coverage Factor (k)	Uncertainty (±)
25.000 µS/cm	24.8 µS/cm	0.200 µS/cm	2.00	0.21 µS/cm
1413.0 µS/cm	1413 µS/cm	0.0 µS/cm	2.00	9.0 µS/cm
111.3 mS/cm	108.8 mS/cm	2.50 mS/cm	2.00	0.67 mS/cm

The End of Certificate

(Mr. Atachai Ngamchanai)

Person in charge

(Mr. Nitinun Srihawan)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพฯ 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2039 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

เอกสารไม่ควบคุม

Delivering Growth - in Asia and Beyond.

CAL-FM-C24-09: 12 Sep 2022

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพฯ 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2039 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond

เอกสารไม่ควบคุม

CAL-FM-C24-09: 12 Sep 2022



ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: KSPR2304472

ชนิดเครื่องมือ CONDUCTIVITY METER

รุ่น: Lab 958

หมายเลขเครื่อง: 163003226

ตรวจซ่อม (รับ)		รายการตรวจเช็ค	ตรวจซ่อม (ส่ง)		หมายเหตุ
16 Mar 2023			16 Mar 2023		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตช์ เปิด - ปิด เครื่อง (On-Off Switch)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		Spectrophotometer			
<input type="checkbox"/>	<input type="checkbox"/>	6. แรงดันไฟฟ้า (Battery Backup) ≥ 2.5 VDC	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	9. แหล่งกำเนิดแสง (UV $< 3,000$ hour)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	10. แหล่งกำเนิดแสง (Visible $< 5,000$ hour)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	<input type="checkbox"/>	<input type="checkbox"/>	
		pH Meter and Conductivity Meter			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. อิเล็กโทรด (Electrode and Connection Cable)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	13. ระดับสารละลายใน Electrode (Level KCl)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	15. ขาจับอิเล็กโทรด (Stand)	<input type="checkbox"/>	<input type="checkbox"/>	
		Turbidimeter			
<input type="checkbox"/>	<input type="checkbox"/>	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	17. ระดับการส่องสว่างของแสง (≥ 2.5 ไม่น้อย 3.0)	<input type="checkbox"/>	<input type="checkbox"/>	
		Automatic titrator			
<input type="checkbox"/>	<input type="checkbox"/>	18. สภาพ Piston Burettes	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	19. Function Rinsing and Dosing	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	<input type="checkbox"/>	<input type="checkbox"/>	

หมายเหตุ: Electrode วัดอุณหภูมิได้ 25.1°C โดย Control Waterbath ที่ 25.0 $\pm 0.1^\circ\text{C}$

Mr. Atachai Ngamchanai

Service Engineer

เอกสารไม่ควบคุม

DKSH Services (Thailand) Co., Ltd.
2503 Sukhumvit Road, Bangchak, Bangkok 10260
Phone: +66 (0)2 538 2054, Email: dqeservicesinfo@gmail.com Website: www.dksh.com/thailand-thailand

Delivering Growth – Inside and Beyond

CALIBRATION 2022

DQEServices Co., Ltd.



32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone: +66 (0)2 538 2054, Email: dqeservicesinfo@gmail.com



CERTIFICATE OF CALIBRATION

Certificate No.: SP23-021

Page 1 of 5

Customer: United Analyst and Engineering Consultant Co., Ltd. (Head Office)

Address: 31 Sol Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong,

Bangkok 10260

Location of calibration: Laboratory 315

Equipment: L'V-Vis Spectrophotometer

Manufacturer: Agilent Technologies

Model: Cary 60

Serial No.: MY15410009

ID No.: N/A

Received Date: 20 May 2023

Calibration Date: 20 May 2023

Issue Date: 23 May 2023

Condition Instrument: Good

Calibrated by:

Mr. Tanawat Rittiduch
(Mr. Tanawat Rittiduch)

Technical Manager

Approved by:

Ms. Chonticha Sargngern
(Ms. Chonticha Sargngern)


Quality Manager

The calibration result is applied only to the above calibration item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

FM-738-02 R01 1/1/2021

เอกสารไม่ควบคุม



DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP23-021
Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	95935	22 October 2023
Absorbance Standard set	25757	95929	22 October 2023
Wavelength Standard set	25806	95916	22 October 2023
Wavelength Standard set	25758	95915	22 October 2023

Traceability This certification is traceable to the International System of Unit maintained at National -
Institute of Standards and Technology (NIST) through Sarna Scientific Limited


Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min


Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength 0.1 nm.



DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



REPORT OF CALIBRATION

Certificate No. : SP23-021
Page 3 of 5

Calibration Results : Without adjustment


Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5787	0.5742	0.0045	0.0031	2.00
	1.0490	1.0423	0.0067	0.0029	2.00
	2.1900	2.1847	0.0053	0.0075	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5607	0.5577	0.0030	0.0034	2.00
	1.0247	1.0234	0.0013	0.0035	2.00
	2.1229	2.1171	0.0058	0.0088	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5236	0.5184	0.0052	0.0029	2.00
	0.9634	0.9607	0.0027	0.0029	2.00
	1.9763	1.9715	0.0048	0.0081	2.00
546.1	0.0000	-0.0001	0.0001	0.0028	2.00
	0.5191	0.5159	0.0032	0.0031	2.00
	1.0003	0.9980	0.0023	0.0033	2.00
	1.9987	1.9917	0.0070	0.0087	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5523	0.5501	0.0022	0.0030	2.00
	1.0809	1.0808	0.0001	0.0030	2.00
	2.0391	2.0336	0.0055	0.0081	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5601	0.5585	0.0016	0.0031	2.00
	1.0512	1.0485	0.0027	0.0030	2.00
	1.9294	1.9317	-0.0023	0.0083	2.00

DQE Services Co.,Ltd.

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2-538 2054, Email : dqeservicesinfo@gmail.com



ISO-TISI-TIS-17025
CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP23-1121

Page: 4 of 5


Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7478	0.7436	0.0042	0.0058	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8686	0.8648	0.0038	0.0064	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2912	0.2908	0.0004	0.0052	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6448	0.6398	0.0050	0.0058	2.00

DQE Services Co.,Ltd.

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2-538 2054, Email : dqeservicesinfo@gmail.com



ISO-TISI-TIS-17025
CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP23-021

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.5	0.31	0.18	2.00
334.06	333.5	0.56	0.18	2.00
360.93	360.3	0.63	0.18	2.00
418.59	418.0	0.59	0.18	2.00
445.94	445.3	0.64	0.18	2.00
453.66	453.0	0.66	0.18	2.00
460.02	459.6	0.42	0.18	2.00
536.59	536.4	0.19	0.18	2.00
637.98	638.3	-0.32	0.18	2.00
431.38	431.0	0.38	0.18	2.00
472.50	472.5	0.00	0.18	2.00
513.47	513.5	-0.03	0.18	2.00
528.88	529.0	-0.12	0.18	2.00
573.17	573.0	0.17	0.18	2.00
585.35	585.0	0.35	0.20	2.00
684.40	684.5	-0.10	0.18	2.00
740.72	741.0	-0.28	0.20	2.00
748.55	748.5	0.05	0.18	2.00
807.03	807.0	0.03	0.18	2.00
879.28	879.5	-0.22	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%

- * Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

CERTIFICATE OF CALIBRATION

Certificate No. : SP23-007 Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : Hitachi

Model : U-1900

Serial No. : 2021-064

ID No. : UAE.WAS.006/2552

Received Date : 6 January 2023

Calibration Date : 6 January 2023

Issue Date : 10 January 2023

Condition Instrument : Used

Calibrated by : 
 (Mr. Tanawut Rittidach)

Technical Manager

Approved by : 
 (Ms. Chonthicha Sangern)

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

REPORT OF CALIBRATION

Certificate No. : SP23-007 Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	95935	22 October 2023
Absorbance Standard set	25757	95929	22 October 2023
Wavelength Standard set	25806	95916	22 October 2023
Wavelength Standard set	25758	95915	22 October 2023

Traceability : This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 4.0 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

REPORT OF CALIBRATION

Certificate No. : SP23-007

Page 1 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5787	0.575	0.0037	0.0031	2.00
	1.0490	1.044	0.0050	0.0029	2.00
	2.1900	2.181	0.0090	0.0080	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5607	0.558	0.0027	0.0034	2.00
	1.0247	1.021	0.0037	0.0035	2.00
	2.1229	2.115	0.0079	0.0081	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5236	0.520	0.0036	0.0030	2.00
	0.9634	0.961	0.0024	0.0029	2.00
	1.9763	1.968	0.0083	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5191	0.518	0.0011	0.0031	2.00
	1.0003	1.000	0.0003	0.0033	2.00
	1.9987	1.993	0.0057	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5523	0.552	0.0003	0.0030	2.00
	1.0809	1.082	-0.0011	0.0030	2.00
	2.0391	2.031	0.0081	0.0080	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5601	0.562	-0.0019	0.0032	2.00
	1.0512	1.052	-0.0008	0.0030	2.00
	1.9294	1.923	0.0064	0.0079	2.00

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP23-007

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7478	0.743	0.0048	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8686	0.861	0.0076	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2912	0.291	0.0002	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6448	0.639	0.0058	0.0055	2.00

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP23-007

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor <i>k</i>
241.54	240.8	0.74	0.18	2.00
279.40	278.5	0.90	0.18	2.00
288.70	288.0	0.70	0.18	2.00
334.22	333.5	0.72	0.18	2.00
361.26	360.5	0.76	0.18	2.00
418.48	417.8	0.68	0.21	2.00
446.70	445.9	0.80	0.18	2.00
453.20	452.5	0.70	0.18	2.00
460.06	459.5	0.56	0.18	2.00
536.90	536.0	0.90	0.18	2.00
637.94	637.1	0.84	0.18	2.00
440.74	440.0	0.74	0.18	2.00
472.22	471.5	0.72	0.18	2.00
513.70	513.0	0.70	0.18	2.00
528.72	528.0	0.72	0.18	2.00
574.60	574.0	0.60	0.18	2.00
585.48	584.6	0.88	0.20	2.00
684.63	684.0	0.63	0.18	2.00
740.27	740.0	0.27	0.20	2.00
748.28	747.5	0.78	0.18	2.00
807.16	806.5	0.66	0.18	2.00
879.70	879.0	0.70	0.18	2.00

Remark : - UUC = 1/|U| Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement *U* is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*.

which for a normal distribution corresponds to a coverage probability of approximately 95%

- * ISO/IEC 17025 TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

CERTIFICATE OF CALIBRATION

Certificate No. : SP23-008

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 213

Equipment : UV-Vis Spectrophotometer

Manufacturer : Hitachi

Model : U-2900

Serial No. : 21E22-009

ID No. : UAE.WAT.051/2564

Received Date : 6 January 2023

Calibration Date : 6 January 2023

Issue Date : 10 January 2023

Condition Instrument : Used

Calibrated by :



 (Mr.Tanawut Rittidach)

Technical Manager

Approved by :



 (Ms. Chonthicha Sangngern)

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

REPORT OF CALIBRATION

Certificate No. : SP23-008

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °CRelative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	95935	22 October 2023
Absorbance Standard set	25757	95929	22 October 2023
Wavelength Standard set	25806	95916	22 October 2023
Wavelength Standard set	25758	95915	22 October 2023

Traceability : This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Sarna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP23-008

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5787	0.574	0.0047	0.0031	2.00
	1.0490	1.044	0.0050	0.0029	2.00
	2.1900	2.182	0.0080	0.0080	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5607	0.558	0.0027	0.0034	2.00
	1.0247	1.021	0.0037	0.0035	2.00
	2.1229	2.114	0.0089	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5236	0.520	0.0036	0.0030	2.00
	0.9634	0.960	0.0034	0.0029	2.00
	1.9763	1.969	0.0073	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5191	0.516	0.0031	0.0031	2.00
	1.0003	0.997	0.0033	0.0033	2.00
	1.9987	1.991	0.0077	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5523	0.550	0.0023	0.0030	2.00
	1.0809	1.078	0.0029	0.0030	2.00
	2.0391	2.032	0.0071	0.0080	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5601	0.558	0.0021	0.0031	2.00
	1.0512	1.049	0.0022	0.0030	2.00
	1.9294	1.922	0.0074	0.0079	2.00

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP23-008

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7478	0.744	0.0038	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8686	0.863	0.0056	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2912	0.290	0.0012	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6448	0.639	0.0058	0.0055	2.00

REPORT OF CALIBRATION

Certificate No. : SP23-008

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor <i>k</i>
241.72	241.0	0.72	0.18	2.00
279.45	278.8	0.65	0.18	2.00
287.81	287.9	-0.09	0.18	2.00
334.06	333.5	0.56	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	418.0	0.59	0.18	2.00
445.94	445.8	0.14	0.18	2.00
453.66	453.0	0.66	0.18	2.00
460.02	459.5	0.52	0.18	2.00
536.59	536.5	0.09	0.18	2.00
637.98	638.0	-0.02	0.18	2.00
431.38	430.6	0.78	0.18	2.00
472.50	472.0	0.50	0.18	2.00
513.47	513.0	0.47	0.18	2.00
528.88	528.5	0.38	0.18	2.00
573.17	573.7	-0.53	0.18	2.00
585.35	585.0	0.35	0.20	2.00
684.40	684.0	0.40	0.18	2.00
740.72	740.5	0.22	0.20	2.00
748.55	748.5	0.05	0.18	2.00
807.03	807.0	0.03	0.18	2.00
879.28	879.5	-0.22	0.18	2.00

Remark : - UUC = $U_{95}(t)$ Under Calibration

- N/A = Not available

- The result expanded uncertainty k (measurement U is stated) as the standard uncertainty of measurement multiplied by the coverage factor k ,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- * Institutes (on TISI accredited)

- End of Certificate -

เอกสารไม่ควบคุม

FM-70802 R01 1/11/2021

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021



PinAAcle 900F Preventive Maintenance Report

Company Name: UNITED ANALYST AND ENGINEERING
Instrument Location: BANGCHAK, PRAKHANONG
BANGKOK, 10260
Instrument Serial No.: PFBS20031902
Date: 20-Jul-2022

เอกสารไม่ควบคุม

PinAAcle 900F Preventive Maintenance (PM)

Company Name:	UNITED ANALYST AND ENGINEERING		
Address (Instrument Location):	BANGCHAK, PRAKHANONG, BANGKOK, 10260		
Serial Number:	PFBS20031902	PM Number:	2/2
Customer Name (if applicable):	K. SATHIDA	Telephone Number:	095-5580-049
Customer Support Engineer Name:	K. DUANG	Service Order Number:	WO-01710010
Date PM Performed: (DD-MMM-YYYY)	Jul 20, 2022	Next PM Due Date: (DD-MMM-YYYY)	Jan 20, 2023
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.

The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.

Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved.

No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.

Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไม่ควบคุม

Component List

Component / Specific Model	Serial #	Configuration Notes

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	N/A
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	N/A
N9301714	Replacement Acetylene Filter Cartridge	N/A
TH001022	Replacement Air Filter Cartridge	N/A

Additional Reagents and Standards Required for PM

Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	25-76CUY1	30-Oct-2022

Additional Reagents and Standards Required for PM (Customer Support Solution)

Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 mL	AR	AR
N/A	0.5% HNO ₃	250 mL	AR	AR

เอกสารไม่ควบคุม

Additional Tools Required for PM

Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	MG0-252
N1013002	1.0A Neutral density filter	1	MG0-358
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	092216-010130
N3050109	Ba Lumina HCL	1	102416-040160
N3050139	K Lumina HCL	1	110716-010060
N3050152	Ni Lumina HCL	1	100516-030190

เอกสารไม่ควบคุม

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Perform general inspection of system for cleanliness.

2. PC Instrument Software:

- ☒ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. Mechanical:

- ☒ Inspect and clean all fans and filters. Replace filters if necessary.
- ☒ Inspect all gas lines for leaks and/or wear. Replace if needed.
- ☒ Clean exterior of the instrument.
- ☒ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ☒ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking slot width. Replace if out of specification.
- ☒ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ☒ Check the drain system for signs of wear. Replace worn or damaged parts.
- ☒ Visually check for proper flame conditions when igniting the Air-C₂H₂ and N₂O-C₂H₂ flames (if applicable).

4. Electrical:

- ☒ Inspect PC boards. Clean if necessary.
- ☒ Carefully check all internal and external cable connections.
- ☒ Check instrument firmware revisions upgrade to current levels (if necessary).
- ☒ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

5. Optics:

- ☒ Inspect and clean the sample compartment windows, if needed.
- ☒ Inspect optics. Clean or replace if necessary.

6. Gasses:

- ☒ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ☒ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	0.9798	0.9848	Passed
0.2 A ND Filter	± 5% from Cert.	0.2042	0.1963	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0008	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed

8.4 D₂ Background Compensation with Copper

Description: Verifies the Instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0049	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0003	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0005	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	NA	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	0.3353	Passed



10. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.	
This PinAAcle 900F Passes <input checked="" type="checkbox"/> Fails <input type="checkbox"/> the preventive maintenance.	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: 	Date: 20-Jul-2022 (DD-MMM-YYYY)
Authorized Customer Representative: 	Date: 20-Jul-2022 (DD-MMM-YYYY)

**Agilent 5110 and 5100 ICP-OES
Preventive Maintenance Checklist**

Agilent Preventive Maintenance provides factory recommended service for your analytical systems to assure reliable operation and the accuracy of your results. Delivered by highly-trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak.

For more information about Agilent Technologies services please visit our web site using the following URL, <http://www.agilent.com/en-us/services/analytical-instrument-services>

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of additional or special procedures and/or parts for the instrument service, then these must be ordered separately and charged as a repair, which may incur additional

Service Engineer's Responsibilities

- Only complete/printout pages that relate to the system being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using a "X" or tick mark "✓" in the checkbox.
- Complete Not Applicable check boxes to indicate services not delivered, as needed.
- Complete the PM service in the order of the tasks listed.
- Complete the Service Review section together with the customer.

**Agilent 5110 and 5100 ICP-OES
Preventive Maintenance Checklist**
System Information

Instrument system name and ID		ICP 5110 VDV	
Instrument system site and location		UAE 3rd Floor Laboratory	
List system component product numbers		List the serial numbers of each component	
1.	G 8019A	1.	M418030001
2.	G 8481A	2.	1801-01988
3.		3.	
4.		4.	
5.		5.	
6.		6.	
7.		7.	
8.		8.	
9.		9.	
10.		10.	

ICP-OES Configuration table	Circle the type or write in the type if other
Nebulizer Type	Senspray (OneNeb) other
Spray Chamber	Cyclonic Single Pass Cyclonic Double Pass other
Torch	Radial Dual View other
Injector Diameter	2.4mm 1.8mm 1.4mm 0.8mm other
Injector Material	Quartz Ceramic other

Agilent 5110 and 5100 ICP-OES Preventive Maintenance Checklist

General Preparation

- ☒ Discuss any specific questions or issues with the customer prior to starting.
- ☒ Review the instrument logbook.
- ☒ Perform general external inspection of system for cleanliness.
- ☒ Check for proper installation of safety-related parts, assemblies, sensors etc.
- ☒ Check for required firmware/software updates and verify with customers if they would like it installed.
- ☒ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. *N/A*
- ☒ Run Instrument Performance test and record results in Instrument Performance Test Results Table - Pre PM.

Inspect and clean the system

- ☒ Look for any obvious external damage or problems.
- ☒ Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- ☒ Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- ☒ Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- ☒ Record the instrument operating conditions in the ICP-OES Status Results Table.
- ☒ Replace the polychromator purge filter.
- ☒ Replace the radial pre-optics window
- ☒ Replace the axial pre-optics window for SVDV and VDV instruments.
- ☒ Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- ☒ Replace air inlet dust filter.
- ☒ Replace high capacity air inlet dust filter element if installed. *N/A*
- ☒ Remove and clean instrument water inlet filter.

G8481A Cooling water system

- ☐ Section NOT Applicable
- ☒ Drain cooling fluid and remove any particles from the chiller reservoir
- ☒ Remove, clean and reinstall water inlet metal mesh filter.
- ☒ Re fill with Polyclear cooling fluid.
- ☒ Clean the cooling system Air filter and the condenser by compressed air or vacuum cleaner.

Agilent 5110 and 5100 ICP-OES Preventive Maintenance Checklist

SPS 3 Auto Sampler

- ☒ Section NOT Applicable
- ☐ Power cycle the autosampler and verify successful initialization.
- ☐ Inspect X and Z-axis belts for wear. Replace is necessary.
- ☐ Clean X and Z axis slide shafts.
- ☐ Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

SPS 4 Auto Sampler

- ☒ Section NOT Applicable
- ☐ Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- ☐ Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner
- ☐ Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☐ Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- ☐ Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles

AVS 4, 6, 7

- ☒ Section NOT Applicable
- ☐ Replace valve rotor seal
- ☐ Check fittings for signs of leaks
- ☐ Check tubing including autosampler tubing for kinks or excessive wear
- ☐ Check high flow pump for signs of leaks

Instrument Adjustment

- ☒ Check position of Zn peak, adjust if required.
- ☒ Check Argon Ratio, adjust to specified value if required.
- ☒ Perform Detector Calibration.
- ☒ Perform Instrument Calibration.
- ☒ Run Instrument Performance Test and record results in Instrument Performance Test Results Table - Post PM.
- ☒ For systems using ICP Expert version 7.3 and above run the following Instrument tests and record the result in the Instrument Test Results Table
 - ☒ Subsystem Communications Test
 - ☒ Air Flow

**Agilent 5110 and 5100 ICP-OES
Preventive Maintenance Checklist**

- ☒ Water Flow
- ☒ Gas Flows
- ☒ RF Generator
- ☒ Camera Test
- ☒ Optics Test
- ☒ Nebulizer Test

Instrument Performance Test Results Table

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial *
Zn 213.857 nm SRBR	4105.6	8364.0	4375.0	8400.8
Mn 257.610 nm SRBR	11064.7	31842.1	12801.7	30846.2
Al 396.152 nm SBR	7.5	14.9	9.9	16.8
K 766.401 nm SBR	5.1	36.8	6.4	39.7

* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

Instrument Test Results Table

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	pass
Air Flow	pass
Water Flow	pass
Gas Flows	pass
RF Generator	pass
Camera Test	pass
Optics Test	pass
Nebulizer test	pass

**Agilent 5110 and 5100 ICP-OES
Preventive Maintenance Checklist**
ICP-OES Status Results Table

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standard Mode	Plasma On
Mains Voltage	224.540 VAC	227.973 VAC
Mains Current	0.204 A	0.104 A
Instrument Temperature	22.8 °C	22.7 °C
RF Air Flow (sensor speed)	15.0 Hz	19.0 Hz
Plasma Exhaust Temperature	No measurement	26.7 °C
Water Flow Oscillator	No measurement	1.64 L/min
Water Flow Detector	1.06 L/min	1.06 L/min
Water Inlet Temperature	18.0 °C	18.0 °C
Polychromator Temperature	35.0 °C	35.0 °C
CCD Temperature	-39.8 °C	-39.8 °C
Thermal Stabilizer	35.0 °C	35.0 °C
Argon Supply Pressure	677.94 kPa	627.33 kPa
Purge Gas Supply Pressure*1	674.90 kPa	645.40 kPa
Option Gas Supply Pressure*1	N/A kPa	N/A kPa
Nebulizer Flow	No measurement	0.70 L/min
Nebulizer Back Pressure	No measurement	164.63 kPa
Plasma Gas Flow	No measurement	11.92 L/min
Auxiliary Gas Flow	No measurement	1.00 L/min
RF Power	No measurement	1200 W
RF Supply Current	No measurement	8.663 A
RF Supply Voltage	No measurement	184.66 V

*1 If option installed

**Agilent 5110 and 5100 ICP-OES
Preventive Maintenance Checklist**
ICP-OES Parts List Table

Part description	Part Number	Product / Model # where used	Quantity Consumed
Axial Pre-Optic Window	G8010-68014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-68015	All	1
Polyclear Cooling Fluid	G8292-80010	G8481A	
Purge Gas Filter	G8010-60136	All	1
Air inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60189	Optional	
Rotor seal for 6-7 port valve for AVS6/7	G8494-60002	G8494A/G8495	
Rotor seal for 4 port valve for AVS4	G8493-60002	G8493A	
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	
PVC waste tubing, 8mm od x 5mm id, 2m	G8410-80122	SPS 4	
Additional Parts may be required from engineers stock			
X axis drive belt	5410047500	SPS 3	
Z axis drive belt	5410047400	SPS 3	
Peristaltic pump tubing, PVC Schvalflex, 3 bridged,	3710049000	SPS 4	

Restore system

For HF applications, ask the customer to reinstall their sample introduction system.

Leave system in an idle state, on and purging.

Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Service Review

- ☒ Affix the PM sticker to the system or instrument label based on the customer's request.
- ☒ Complete the Service Engineer Comments section below if there are additional comments.

**Agilent 5110 and 5100 ICP-OES
Preventive Maintenance Checklist**

- ☒ Review the service and any test results with the customer.
- ☒ If the Instrument firmware was updated, record the details of the change in the Service Engineer's Comments box below or if necessary, in the customer's IQ records.

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

Other Important Customer Web Links

How to get information on your product:

- ☒ Literature Library - <http://www.agilent.com/en-us/products/icp-oes/icp-oes-systems/5110-icp-oes#literature>
- ☒ Need to know more? - <http://www.agilent.com/crosslab/university/>
- ☒ Need technical support, FAQs? - <http://www.agilent.com/en-us/support/landing/icp-oes>
- ☒ Need supplies? - www.agilent.com/chem/supplies

Service Completion

Service request number 602568511 Date service completed 30 Nov 2017

Agilent signature Hovavit Customer signature gim

Document part number: G8014-90075

Report Summary

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	Test Before PM
Test Completed On	11/30/2022 9:35:32 AM

Result Summary

Subsystem Communications Test	Skipped
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Pass
Precision Test	Pass

เอกสารไม่ควบคุม

Resolution Test**Pass**

Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.62
As (188.980 nm)	≤ 8.20	6.20
C (193.027 nm)	≤ 11.50	8.35
Mo (202.032 nm)	≤ 8.20	6.41
Cr (206.158 nm)	≤ 13.40	9.04
Zn (213.857 nm)	≤ 8.70	6.62
Pb (220.353 nm)	≤ 9.50	7.13
Co (228.615 nm)	≤ 17.20	11.71
Ba (230.424 nm)	≤ 9.40	7.21
Mn (257.610 nm)	≤ 13.30	9.50
Mn (260.568 nm)	≤ 20.30	14.33
Cr (267.716 nm)	≤ 11.00	8.14
Cu (324.754 nm)	≤ 25.00	18.98
Cu (327.395 nm)	≤ 14.20	11.24
Sr (338.071 nm)	≤ 33.50	24.47
Ba (455.403 nm)	≤ 44.00	33.88
Sr (460.733 nm)	≤ 36.00	17.22
Ba (493.408 nm)	≤ 36.00	25.48
Ba (614.171 nm)	≤ 42.00	25.47
Ar (675.283 nm)	≤ 74.00	59.82
K (766.491 nm)	≤ 80.00	64.94

เอกสารไม่ควบคุม

Sensitivity Test

Pass

Radial

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	147.7	1156.5	55.5
Se (196.026 nm)	≥ 41.0	SRBR	111.1	1195.3	97.7
Zn (213.857 nm)	≥ 1421.0	SRBR	4100.6	51959.5	159.6
Pb (220.353 nm)	≥ 46.0	SRBR	192.5	2808.6	185.7
Mn (257.610 nm)	≥ 3516.0	SRBR	11064.7	264165.0	567.6
Al (396.152 nm)	≥ 3.4	SBR	7.5	49047.9	5770.5
Ba (493.408 nm)	≥ 34.0	SBR	107.4	1887710.3	17407.5
K (766.491 nm)	≥ 1.8	SBR	5.1	100805.9	16826.4

Axial

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	234.9	3056.4	152.9
Se (196.026 nm)	≥ 159.0	SRBR	218.1	3865.1	271.6
Zn (206.200 nm)	≥ 234.0	SRBR	1306.5	15850.4	144.5
Zn (213.857 nm)	≥ 1743.0	SRBR	8364.0	183037.8	476.4
Cd (214.439 nm)	≥ 4227.0	SRBR	7718.5	143240.2	342.8
Pb (220.353 nm)	≥ 320.0	SRBR	576.3	14465.2	580.4
Mn (257.610 nm)	≥ 10625.0	SRBR	31842.1	1411257.3	1958.9
Cr (267.716 nm)	≥ 1048.0	SRBR	4492.1	183110.6	1632.2
Cu (324.754 nm)	≥ 19.0	SBR	46.2	371487.5	7862.9
Al (396.152 nm)	≥ 6.0	SBR	14.9	278447.4	17552.6
Ba (493.408 nm)	≥ 60.0	SBR	190.6	10061527.3	52519.8
K (766.491 nm)	≥ 24.0	SBR	36.8	1922163.4	50858.1

เอกสารไม่ควบคุม

Precision Test

Pass

Radial

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 2.60	0.82
Se (196.026 nm)	≤ 2.60	0.71
Zn (213.857 nm)	≤ 1.50	0.43
Pb (220.353 nm)	≤ 2.60	0.76
Mn (257.610 nm)	≤ 1.50	0.60
Al (396.152 nm)	≤ 1.50	0.48
Ba (493.408 nm)	≤ 1.50	0.89
K (766.491 nm)	≤ 1.50	0.42

Axial

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 1.50	0.57
Se (196.026 nm)	≤ 1.50	0.76
Zn (206.200 nm)	≤ 1.50	0.61
Zn (213.857 nm)	≤ 1.50	0.51
Cd (214.439 nm)	≤ 1.50	0.56
Pb (220.353 nm)	≤ 1.50	0.52
Mn (257.610 nm)	≤ 1.50	0.54
Cr (267.716 nm)	≤ 1.50	0.54
Cu (324.754 nm)	≤ 1.50	0.69
Al (396.152 nm)	≤ 1.50	0.91
Ba (493.408 nm)	≤ 1.50	0.85
K (766.491 nm)	≤ 1.50	1.22

เอกสารไม่ควบคุม

Report Summary

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.2.1.9507
Firmware Version	3442
Tested By	FM Functional test
Test Completed On	11/30/2022 11:43:36 AM

Result Summary

Subsystem Communications Test	Pass
Air Flow Test	Pass
Water Flow Test	Pass
Gas Flows Test	Pass
RF Generator Test	Pass
Camera Test	Pass
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Skipped
Sensitivity Test	Skipped
Precision Test	Skipped

Subsystem Communications Test Pass

Air Flow Test Pass

30% Air Flow (relative speed)	75% Air Flow (relative speed)
14.00	19.00

Water Flow Test Pass

RF Water Flow(L/min)	Camera Water Flow (L/min)	Water Inlet Temperature (°C)
1.44	1.05	18.51

เอกสารไม่ควบคุม

Gas Flows Test

Pass

Nebulizer Target Flow	Actual Flow	Back Pressure	Auxiliary Target Flow	Actual Flow	Back Pressure
0.70	0.70	163.37	2.00	1.99	108.48
Makeup Target Flow	Actual Flow	Back Pressure	Plasma Target Flow	Actual Flow	Back Pressure
2.00	2.00	112.85	18.00	17.91	23.45

RF Generator Test

Pass

RF Power Supply Test	Passed
RF Power Supply (V)	147.437
RF Oscillator Test	Passed
RF Oscillator Frequency (MHz)	0.000
Work Coil Current (A)	45.069
RF Power Supply Current (A)	1.997

Camera Test

Pass

	Integration Time (ms)	Standard Deviation	Status
Electronic Offset Test	1000	5.305	Passed
Dark Current Test	6000	0.578	Passed
Array Test	5	0.024	Passed
Linearity Test		0.118	Passed

เอกสารไม่ควบคุม

Report Summary

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY1803C001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	PM Performance test
Test Completed On	11/30/2022 12:10:42 PM

Result Summary

Subsystem Communications Test	Skipped
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Pass
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Pass
Precision Test	Pass

Optics Test**Pass**

	Radial	Axial
Intensity	5674608	5823476
Wavelength	737.212	737.212

เอกสารไม่ควบคุม**Resolution Test****Pass**

Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.79
As (188.980 nm)	≤ 8.20	6.09
C (193.027 nm)	≤ 11.50	8.29
Mo (202.032 nm)	≤ 8.20	6.30
Cr (206.158 nm)	≤ 13.40	9.05
Zn (213.857 nm)	≤ 8.70	6.77
Pb (220.353 nm)	≤ 9.50	7.02
Co (228.615 nm)	≤ 17.20	11.67
Ba (230.424 nm)	≤ 9.40	7.39
Mn (257.610 nm)	≤ 13.30	9.48
Mn (260.568 nm)	≤ 20.30	14.25
Cr (267.716 nm)	≤ 11.00	7.94
Cu (324.754 nm)	≤ 25.00	18.99
Cu (327.395 nm)	≤ 14.20	11.33
Sr (338.071 nm)	≤ 33.50	24.44
Ba (455.403 nm)	≤ 44.00	33.86
Sr (460.733 nm)	≤ 36.00	17.51
Ba (493.408 nm)	≤ 36.00	25.56
Ba (614.171 nm)	≤ 42.00	24.96
Ar (675.283 nm)	≤ 74.00	59.38
K (766.491 nm)	≤ 80.00	65.63

เอกสารไม่ควบคุม

Sensitivity Test			Pass		
Radial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	147.8	1149.3	54.8
Se (196.026 nm)	≥ 41.0	SRBR	111.6	1222.8	101.0
Zn (213.857 nm)	≥ 1421.0	SRBR	4375.0	52592.3	143.7
Pb (220.353 nm)	≥ 46.0	SRBR	199.8	2744.4	166.5
Mn (257.610 nm)	≥ 3516.0	SRBR	12801.7	285591.3	496.0
Al (396.152 nm)	≥ 3.4	SBR	9.9	52888.6	4873.6
Ba (493.408 nm)	≥ 34.0	SBR	154.6	2287291.6	14698.1
K (766.491 nm)	≥ 1.8	SBR	6.4	106701.6	14350.9
Axial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	242.4	3170.1	154.8
Se (196.026 nm)	≥ 159.0	SRBR	226.1	4134.5	289.3
Zn (206.200 nm)	≥ 234.0	SRBR	1126.6	13782.0	146.5
Zn (213.857 nm)	≥ 1743.0	SRBR	8400.8	177166.3	442.5
Cd (214.439 nm)	≥ 4227.0	SRBR	7001.9	125884.2	321.6
Pb (220.353 nm)	≥ 320.0	SRBR	536.3	12909.3	532.6
Mn (257.610 nm)	≥ 10625.0	SRBR	30846.2	1287989.0	1738.8
Cr (267.716 nm)	≥ 1048.0	SRBR	4396.0	167335.6	1424.4
Cu (324.754 nm)	≥ 19.0	SBR	52.1	373690.7	7033.1
Al (396.152 nm)	≥ 6.0	SBR	16.8	268357.7	15112.4
Ba (493.408 nm)	≥ 60.0	SBR	225.2	10173441.5	44971.7
K (766.491 nm)	≥ 24.0	SBR	39.7	1874136.2	46055.7

เอกสารไม่ควบคุม

Precision Test			Pass
Radial			
Element Wavelength	Specification	Measured Value % RSD	
As (188.980 nm)	≤ 2.60	0.60	
Se (196.026 nm)	≤ 2.60	0.84	
Zn (213.857 nm)	≤ 1.50	0.29	
Pb (220.353 nm)	≤ 2.60	0.59	
Mn (257.610 nm)	≤ 1.50	0.28	
Al (396.152 nm)	≤ 1.50	0.28	
Ba (493.408 nm)	≤ 1.50	0.59	
K (766.491 nm)	≤ 1.50	0.23	
Axial			
Element Wavelength	Specification	Measured Value % RSD	
As (188.980 nm)	≤ 1.50	0.71	
Se (196.026 nm)	≤ 1.50	0.43	
Zn (206.200 nm)	≤ 1.50	0.46	
Zn (213.857 nm)	≤ 1.50	0.37	
Cd (214.439 nm)	≤ 1.50	0.48	
Pb (220.353 nm)	≤ 1.50	0.48	
Mn (257.610 nm)	≤ 1.50	0.74	
Cr (267.716 nm)	≤ 1.50	0.26	
Cu (324.754 nm)	≤ 1.50	0.51	
Al (396.152 nm)	≤ 1.50	0.45	
Ba (493.408 nm)	≤ 1.50	0.81	
K (766.491 nm)	≤ 1.50	0.84	

เอกสารไม่ควบคุม

DMA-80 Direct Mercury Analyzer SERVICE PROTOCOL REPORT

To be filled in before service visit (1st page)**Customer information:**

Company: บริษัท อีคอนเทคโนโลยี จำกัด
 Department: Lab
 Person in charge: คุณ อดิสรณ์
 Address: 3 หมู่ 2 ตำบลบ้านใหม่ อำเภอเมือง จังหวัดนนทบุรี 11000
 Tel.:
 E-mail:

Technical data:

Unit Serial Number: 11030982
 Terminal type or USB-640 Gateway: Terminal 640 SN 1010000091
 Software type and revision: Easy control Rev. 02-D
 Air Compressor (if present): - SN -
 Gas system pump (if present): - SN -
 Installation and last maintenance dates: Inst. on: Maint. on:

NOTE: after achievement of the following protocol a filled and signed copy of this report has to be sent to Milestone srl at: service@milestonesrl.com

For the best result of the test below we recommended to use the Milestone DMA-80 Service Kit (PN DMA-SKIT).

1. VISUAL INSPECTION

	Good	Damaged	Corroded/Dirty
External chassis	↓		
Inside	↓		
Electric parts	↓		
Screws	↓		

2. ELECTRICAL SAFETY TEST

Using a suitable testing device check the below reported parameters and take note of the results.

Parameter	Result	OK	Not OK
Insulating resistance: $R_{iso} \geq 0.5 M\Omega$	Actual value: 225 MΩ	↓	
Grounding resistance: $R_{gs} \leq 100 m\Omega$	Actual value: 0.7 MΩ	↓	

3. PRESSURE CHECK

	Oxygen (purity $O_2 > 99.95\%$)	Milestone air compressor
Gas carrier	Oxygen Purity: 99.995%	-

The pressure at the supply source manometer should be approx. 4.0 bar
 The flow rate depends by type of cuvette installed on the DMA-80 unit.



	Correct value	Actual value	Final value	Correct value	Actual value	Final value	Correct value	Actual value	Final value
Inlet pressure	3.1 bar	-	-	3.1 bar	-	-	3.1 bar	3.1 bar	Pass
Flow rate	10-12 l/h	-	-	8-10 l/h	-	-	6-8 l/h	7 l/h	Pass

Check all possible leakage points and their conditions:

	Good	Damaged	Corroded
Tubing	↓		
Silicon joints	↓		
O-rings	↓		
Cuvette sealing O-rings	↓		
Gas connections	↓		
Valves	↓		
Sample boat carrier	↓		
Catalyst flange	↓		

4. AUTOSAMPLER SYSTEM

	OK	Not OK	Re-Adjusted
Calibration of autosampler motor	✓		
Cylinders alignment	✓		

	Fast	Slow	Normal
Speed of pneumatic cylinders			✓

Using the maintenance grease, periodically lightly lubricate all exposed steel rods of the horizontal and vertical cylinders.

5. COMPONENTS CHECK

Conditions of the different parts used/installed on DMA unit:



	OK	Not OK	Replaced	Cleaned
Catalyst tube			✓	
Amalgamator			✓	
Quartz boats			✓	
Nickel boats				
Autosampler plate	✓			
Gas kit accessories				

6. TEMPERATURES

	Correct value	Actual value	Final value
Drying/ Decomposition furnace	f controlled by infrared sensor	850°C ± 10°C	-
	f controlled by thermocouple	650°C ± 10°C	-
Catalyst furnace	515°C ± 10°C	565 °C	Pass
Amalgamator start by temperature	170°C ± 10°C	170 °C	Pass
Amalgamator heating temperature	350°C ± 10°C	350 °C	Pass
Cuvette	125°C ± 5°C	125 °C	Pass

7. SPECTROMETER

The spectrometer can be equipped with a single beam system (ducelor lamp) or with a dual beam system (tricolor lamp)

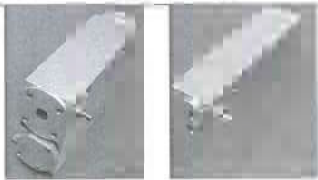	Old cuvette type						Actual cuvette type					
												
	Gain			Offset			Gain			Offset		
	Correct value	Actual value	Final value	Correct value	Actual value	Final value	Correct value	Actual value	Final value	Correct value	Actual value	Final value
Dualcell system	3.5VDC	-	-	0.015VDC ± 0.005VDC	-	-	3.55VDC	3.2V	Pass	0.015VDC ± 0.005VDC	0.015V	Pass
Tricell system*	-	-	-	-	-	-	3.55VDC	-	-	0.015VDC ± 0.005VDC	-	-

(*)The recommended Hg lamp operating signal should be around 3.95VDC (for detector 2) and 3.95VDC (for detector 1).

	OK	Not OK
Conditions of the spectrometer system	✓	
Alignment between lamp, cuvette and detector	✓	
Cuvette cleaning (glass windows, sealing O-rings...)	✓	
Lamp intensity	✓	
Operation of the mechanical shutter (if present)	✓	

8. MILESTONE AIR COMPRESSOR

Maintenance	OK	Date last service
Drain (compressor)		
Replacing air filters (air filter)		
Check sealing connections		

9. PARTS TO BE REPLACED


PN	DESCRIPTION	Replaced	Not
----	-------------	----------	-----

			Replaced
DMA8133	Catalyst tube: 6 months if the unit runs daily. 1 year if the unit is used rarely. <i>In case of analyse of sample with high organic concentration the lifetime of the catalyst can be less than 6 months.</i>	↓	
DMA8134	Amalgamator: 6 months if the unit runs daily 1 year if the unit is used rarely	↓	
DMA8195A	Hg lamp tri-cell (model 2011) (for kit p/n DMA8355): 2 years	↓	
DMA8137	Hg lamp dual-cell: 2 years	↓	
70200	Hg trap 1 year	↓	
DMA8058/B	Amalgamator coil 1 year or as soon as the heating is not more homogeneous	↓	
DMA8142	Nickel sample boats (set of 40pcs) 2 years if strongly used, replace after 1 year	↓	
DMA8347	Quartz sample boats (set of 10pcs) 4 years	↓	
DMA8335	Metal sample boat carrier 2 years	↓	
SL0108	PU-tube diam. 6/4 mm for internal O ₂ /air supply 2 years	↓	
SO0376D	Heating coil for drying/decomposition 2 years	↓	

10. TESTING PROCEDURE


It consists to run some measurements for the evaluation of the analytical performance of the unit, like: absorbance, peaks shape, temperatures, lamp signal and verify the proper working of whole system.

- 1) Run minimum 2 blanks on the same sample boat (quartz if possible) in manner to clean it
- 2) Run blanks until absorbance value (Height) decrease under 0.0020
- 3) Set a fresh and stabilized 100µg/L Hg standard according to the prescriptions reported on the DMA80 User Manual. The quality of the used standard is fundamental for the success of the entire procedure
- 4) Weight approximately 10Cµg of the fresh 100µg/L –Standard (10ng) and start the analysis as a single measurement mode
- 5) Repeat five times the test
- 6) Run again two blanks measurements

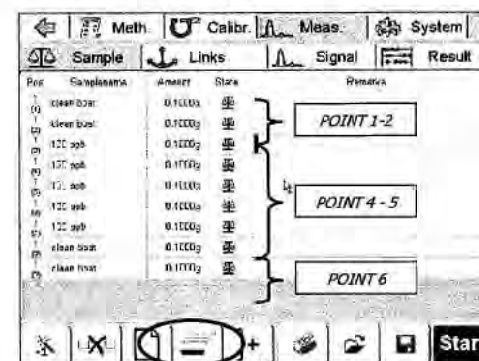

Now, it is possible to evaluate:

- Peaks



- The shape of the peak must be regular.
- The distance between Peak Cell 1 and Peak Cell 2 must be between 11 to 15 seconds.

- Results



- The obtained absorbance (height) of the Blank must be < 0.0020.
- The obtained absorbance (height) must be > 0.42 for each 100ppb analysis (0.22 with cuvette installed until December 2005, DMA s/n 05120292.)
- The relative standard deviation (rsd) is < 1.5 %.
- After two blanks (after 10ng measurements), the absorbance is < 0.0020.

- Temperatures & signal profiles

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



- The Hg absorbance peaks must be correctly detected and reported.

13. FINAL REPORT

Page 5

Working Hours of Service Engineer:	
------------------------------------	--

10	11	63	Controllable	Variable	Controllable	Fixed
----	----	----	--------------	----------	--------------	-------

acceptance signature: _____



TECHNOLOGY PROMOTION ASSOCIATION (THAI) AND JAPAN
CORPORATE SERVICES : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD 11, SUANLUANG, SUANLUANG BANGKOK 10550
TEL: 02-2717-8803-29 FAX: 0-2716-4488



Cert. No.: 23TM192
Page : 1 of 3

Certificate of Calibration

Equipment : Incubator
Manufacturer : Binder
Model : BD 53 E2
Serial No. : 13-07343
ID No. : UAE.MIC.005/2558
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong
Bangkok 10260
Location : Microbiology Laboratory
Received Order : 15 February 2023
Calibration Date : 15 February 2023
Ambient Temperature : $(26 \pm 1) ^\circ\text{C}$
Relative Humidity : $(50 \pm 3) \%$
Calibrated by : Suwit Injai
Approved by :
() Ponthippa Tameyakul
() Malee Butnuea
Issue Date : 24 February 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full or exact copy the print/written
Approval of the head of Corporate Services : Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2302-02950C-1
Procedure Used :-

Cert. No.: 23TM192
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY59003411	22LM165	26 Nov 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	22	23
REL Humid. (%)	65	61
AC Supply (Volt)	231	231



Probe Installation Details :

a = 5.0 mm
b = 5.0 mm
c = 5.0 mm

Dimension of Chamber :

D = 0.33 m
W = 0.40 m
H = 0.40 m
Capacity = 0.053 m³

Position :	Ref. Std. ID No.:
1	20RTD-2/1
2	20RTD-2/2
3	20RTD-2/3
4	20RTD-2/4
5	20RTD-2/5
6	20RTD-2/6
7	20RTD-2/7
8	20RTD-2/8
9 (ref)	20RTD-2/9

เอกสารไม่ควบคุม



Equipment : Incubator
 Condition As-Received : Used Item
 Reference : 2302-02850C-1
 Result of Calibration :- (*) Without Adjustment
 Function of UUC* : Temperature Source
 Fresh air setting : Close

Cert. No.: 23TM192
 Page: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
35.0	35.4	35.4	0.037	0.56	0.86	0.30	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
35.0	35.256	35.308	35.116	35.453	34.700	34.798	34.718	34.657	34.838

Average* : The average of 30 values in each position

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
 CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES
 534/4 PATANAKARNY ROAD (SOI 16) SUANLUANG, SUANLUANG BANGKOK 10250
 TEL: 0-2717-9000-27 FAX: 0-2719-9484



NAC-TISI-TIS17025
 CALIBRATION 4008

Cert. No.: 22TM1063
 Page.: 1 of 3

Certificate of Calibration

Equipment : Incubator
 Manufacturer : Memmert
 Model : INB 40C
 Serial No. : E4111325
 ID No. : UAE.MIC.003/2555
 Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangkok, Phrakhanong
 Bangkok 10260
 Location : Microbiology Laboratory
 Received Order : 11 July 2022
 Calibration Date : 11 July 2022
 Ambient Temperature : (26 ± 1) °C
 Relative Humidity : (50 ± 3) %
 Calibrated by : Man Pattanapongpaiboon

Approved by :
 Approved Signatory

() Pornthippa Tameyakul
 (x) Malee Butkulea
 () Suwit Imjai

Issue Date : 18 July 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services & Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2207-0245OC-3

Cert. No.: 22TM1063

Page: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-CTC2 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY57013823	22LM24	28 Feb 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close



Environment during calibration		
	Beginning	Finished
Temp. (°C)	25	25
REL.Humid. (%)	56	62
AC Supply (Vcvt)	219	223

Position :	Ref. Std. ID No.:
1	21-17RTD-01
2	21-17RTD-02
3	17RTD-03
4	17RTD-04
5	17RTD-05
6	17RTD-06
7	17RTD-07
8	17RTD-08
9 (ref.)	17RTD-09

Probe Installation Details :

Dimension of Chamber :	
a = 5.0 cm	D = 0.40 m
b = 5.0 cm	W = 0.33 m
c = 5.0 cm	H = 0.40 m
	Capacity = 0.053 m ³

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2207-0245OC-3

Cert. No.: 22TM1063

Page: 3 of 3

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
36.0	35.5	35.5	0.10	0.63	0.88	0.30	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
36.0	35.896	35.803	35.646	35.766	36.272	35.561	36.212	35.519	35.887

Average* : The average of 30 values in each position

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %

-oOo-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKAENG ROAD SOI 14, SUANLUANG, SUKUMVIT ROAD, BANGKOK 10250
TEL. 0-2317-3000-27 FAX. 0-2799-9484



Cert. No.: 22TM1064
Page.: 1 of 3

Certificate of Calibration

Equipment : Incubator
Manufacturer : Memmert
Model : BE 400
Serial No. : e402.1032
ID No. : UAE.MIC.001/2546
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakharong,
Bangkok 10260
Location : Microbiology Laboratory
Received Order : 11 July 2022
Calibration Date : 11 July 2022
Ambient Temperature : $(26 \pm 10) ^\circ\text{C}$
Relative Humidity : $(50 \pm 30) \%$
Calibrated by : Man Pattanapongpaiboon

Approved by :

Approved Signatory

() Ponnhippa Tameyakul
(✓) Malee Butkruea
() Suwit Itirjai

Issue Date : 18 July 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services & Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2207-02450C-2
Procedure Used :-

Cert. No.: 22TM1064
Page.: 2 of 3

Calibration were conducted using calibration procedure CP-DT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY57013823	22LM/24	26 Feb 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	25	25
REL Humid. (%)	62	63
AC Supply (Volt)	222	223



Probe Installation Details :

a = 5.0 mm
b = 5.0 mm
c = 5.0 mm

Dimension of Chamber :

D = 0.40 m
W = 0.33 m
H = 0.40 m
Capacity = 0.053 m³

Position :	Ref. Std ID No.:
1	21-17RTD-01
2	21-17RTD-02
3	17RTD-03
4	17RTD-04
5	17RTD-05
6	17RTD-06
7	17RTD-07
8	17RTD-08
9 (ref.)	17RTD-09

เอกสารไม่ควบคุม



Equipment : Incubator
 Condition As-Received : Used Item
 Reference : 2207-02450C-2
 Result of Calibration : () Without Adjustment
 Function of UUC* : Temperature Source
 Fresh air setting : Close

Cert No.: 22TM1064

Page: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
37.0	38.0	38.0	0.092	0.62	0.94	0.30	2
56.0	57.5	57.5	0.083	0.87	1.3	0.42	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
37.0	37.329	37.575	37.476	37.577	36.834	36.997	36.924	37.035	37.387
56.0	56.489	56.520	56.445	56.465	55.291	55.589	55.899	55.591	56.097

Average*: The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
 CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES
 534/4 PATTANAKUL ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
 TEL: 0-2717-3000-29 FAX: 0-2717-3444



Cert. No.: 23TV250

Page : 1 of 3

Certificate of Calibration

Equipment : Water Bath
 Manufacturer : Memmert
 Model : WNE 14
 Serial No. : L416 0614
 ID No. : UAE.MIC.020/2561
 Submitted by : United Analyst and Engineering Consultant Co. Ltd.
 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangkok, Phra Khanong,
 Bangkok 10260
 Location : Microbiology Laboratory
 Received Order : 15 February 2023
 Calibration Date : 16 February 2023
 Ambient Temperature : (26 ± 10) °C
 Relative Humidity : (50 ± 30) %
 Calibrated by : Preecha Hahib

Approved by : 
 Approved Signatory

() Ponthepa Tameyakul
 () Melae Butkruea
 () Suwit Imjai

Issue Date : 24 February 2023

The Uncertainties are for a confidence probability of approximately 95 %

This certificate shall not be reproduced other than in full except with the prior written
 Approval of the head of Corporate Services & Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2302-0295OC-4
 Result of Calibration :- (*) Without Adjustment
 Function of UUC* : Temperature Source

Cert. No.: 23TM250
 Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)				
			Position				
			1	2	3	4	5 (ref.)
44.5	44.4	44.4	44.482	44.458	44.481	44.461	44.460
50.0	50.0	50.0	50.087	50.061	50.066	50.064	50.068

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Uncertainty (± °C)	Coverage Factor k
44.5	0.058	0.030	0.15	2
50.0	0.058	0.036	0.15	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-๐๐๐-

เอกสารไม่ควบคุม



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2302-0295OC-4
 Procedure Used :-

Cert. No.: 23TM250
 Page : 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY59003411	22LM165	26 Nov 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	22	55	220
Finished of Calibration	23	58	221

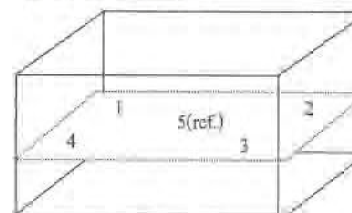

Front

Position :	Ref. Std ID No.:
1	4804539-001
2	4804539-002
3	4804539-003
4	4804539-004
5(ref.)	4804539-005

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAPONGPAIBOON RD. VJH111, SUANLUANG, SUTHEP/BANGKOK 10250
TEL. 0-2717-6000-27 / FAX. 0-2719-8488



Cert. No.: 22TM1085
Page.: 1 of 3

Certificate of Calibration

Equipment : Water Bath
Manufacturer : Memmert
Model : WB 14
Serial No. : I401.0569
ID No. : UAE.MIC.004/2544
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Microbiology Laboratory
Received Order : 11 July 2022
Calibration Date : 11 - 12 July 2022
Ambient Temperature : $(26 \pm 1) ^\circ\text{C}$
Relative Humidity : $(50 \pm 3) \%$
Calibrated by : Man Pattanapongpaiboon

Approved by :

Approved Signatory

- () Pornthippa Tameyakul
(x) Malee Butkruea
() Suwit Imjai

Issue Date : 18 July 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of (The Bureau of Corporate Services & Equipment Calibration and Testing Services)

เอกสารไม่ควบคุม



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2207-02450C-5
Procedure Used :-

Cert. No.: 22TM1085

Page.: 2 of 3

Calibration were conducted using in-house calibration procedure CP-0704 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY57013823	22LM24	26 Feb 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (+) Without Adjustment

Function of UUC : Temperature Source

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	59	223
Finished of Calibration	25	63	224

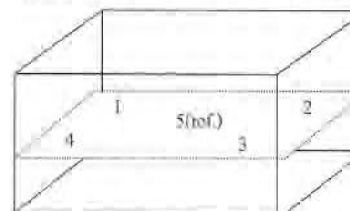

Position :	Ref. Std. S/N.
1	4804539-006
2	4804539-007
3	4804539-008
4	4804539-009
5 (ref.)	4804539-010

Figure

เอกสารไม่ควบคุม



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2207-0245DC-5
 Result of Calibration :- (°) Without Adjustment
 Function of UUC : Temperature Source

Cert. No.: 22TM1065
 Page.: 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)				
			Position				
			1	2	3	4	5 (ref.)
41.5	41.2	41.2	41.475	41.459	41.427	41.485	41.493

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Uncertainty (± °C)	Coverage Factor k
41.5	0.097	0.065	0.15	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location, which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
 CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
 534/4 PATTANABURI RD. SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
 TEL: 0-2717-1000-27 FAX: 0-2719-9484



Cert. No.: 22TM1121
 Page.: 1 of 3

Certificate of Calibration

Equipment : Autoclave
 Manufacturer : ALP
 Model : CL-40L
 Serial No. : 507298
 ID No. : UAE.MIC.019/2560
 Submitted by : United Analyst and Engineering Consultant Co., Ltd.
 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangchak, Phrakhadong,
 Bangkok 10260
 Location : 301 Room
 Received Order : 11 July 2022
 Calibration Date : 11 July 2022
 Ambient Temperature : (25 ± 10) °C
 Relative Humidity : (50 ± 30) %
 Calibrated by : Preecha Hahib

Approved by :
 Approved Signatory

(/) Porntipasa Fameyakul
 (/) Malee Butkruea
 (/) Suwit Imjai

Issue Date : 18 July 2022

The Uncertainties are for a confidence probability of approximately 95 %

This certificate may not be reproduced other than in full, except with the prior written
 Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



Equipment : Autoclave Cert. No.: 22TM1121
 Condition As-Received Used Item Page.: 2 of 3
 Reference : 2207-0245QC-7
 Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.
 The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1.) Data Acquisition	34970A	MY44080450	22LM46	28 Mar 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**

(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)
 It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Result of Calibration :- (°) Without Adjustment

Function of UUC* : Temperature Source



	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	29	48	220
Finished of Calibration	32	48	220

Position	Description	Ref. Std. ID No.:
1 =	Center of chamber	22-14TC-01
2 =	Temperature sensor	22-14TC-02
3 =	Exhaust port	22-14TC-03

เอกสารไม่ควบคุม



Equipment : Autoclave Cert. No.: 22TM1121
 Condition As-Received Used Item Page.: 3 of 3
 Reference : 2207-0245QC-7
 Result of Calibration :- (°) Without Adjustment

Operating parameter Set : Temperature = 115 °C

Sterilization period = 15 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor k
116	116	1	116.523	0.14	0.08	0.90	2
		2	116.566				
		3	116.440				

Operating parameter Set : Temperature = 121 °C

Sterilization period = 30 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor k
122	122	1	122.503	0.19	0.12	0.91	2
		2	122.637				
		3	122.558				

Average* : The average of 30 values in each position

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-๐๐๐-

เอกสารไม่ควบคุม




TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANA KARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23MM331

Page.: 1 of 3

Certificate of Calibration

Equipment : Electronic Balance
Manufacturer : Mettler Toledo
Model : AB204-S
Serial No. : 1128312528
ID No. : UAE.AIR.019/2550
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Balance Room 2
Received order : 07 April 2023
Calibration Date : 07 April 2023
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 90 %
Calibrated by : Suwit Imjai
Approved by : 
() Ponthippa Tameyakul
(/) Ma'lee Butkruea
Issue Date : 10 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-00150C-1
Procedure used :-

Cert.No.: 23MM331

Page: 2 of 3

Calibration was conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15384	24053	70RC007	MM-0010-22	20 Jan 2024

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certification is traceable to the International System of Unit.

Result of calibration () Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity : 0 g to 220 g **Resolution** 0.0001 g

Before Adjustment :

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
(g)	(g)	(g)	(± mg)	(k)
100	99.9999	+0.0001	0.19	2.03
200	200.0001	-0.0001	0.29	2.00

After Adjustment :

1. Determination of the standard deviation of weighing machine (n = 10)

Applied Weight	Standard Deviation of Reading (g)
(g)	
100	0.00007
200	0.00007


เอกสารไม่ควบคุม



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0015OC-1

Cert.No.: 23MM331

Page: 3 of 3



Maximum difference between
off-center and central loading

Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)
-0.0001	-0.0002	+0.0004	-0.0001	-0.0006

0.0005

3. Departure from nominal value

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (\pm mg)	Coverage Factor (k)
Unload	0.0000	0.0000	0.15	2.13
0.1	0.0999	+0.0001	0.15	2.13
1	0.9999	+0.0001	0.15	2.13
5	4.9999	+0.0001	0.15	2.13
10	9.9999	+0.0001	0.15	2.11
20	20.0000	0.0000	0.15	2.11
50	50.0000	0.0000	0.16	2.06
70	69.9999	+0.0001	0.18	2.04
100	99.9999	+0.0001	0.19	2.03
150	150.0003	-0.0003	0.29	2.00
200	200.0005	-0.0005	0.29	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3006-29 FAX. 0-2719-9484



Cert.No.: 23MM332

Page.: 1 of 3

Certificate of Calibration

Equipment : Electronic Balance
Manufacturer : Mettler Toledo
Model : AB204-S /FACT
Serial No. : B108115858
ID No. : UAE.AIR.016/2555
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Balance Room 2
Received order : 07 April 2023
Calibration Date : 07 April 2023
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 90 %
Calibrated by : Suwit Imjai
Approved by :
Approved Signatory
() Ponthippa Tameyakul
(/) Malee Butkruea
Issue Date : 10 April 2023

The Uncertainties are for a confidence probability of approximately 95 %

This certificate may not be reproduced other than in full, except with the prior written
Approval of the Head of Corporate Services 3: Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



Equipment : Electronic Balance
 Condition As-Received : Used Item
 Reference : 2304-0015OC-2
 Procedure used :-

Cert.No.: 23MM332
 Page: 2 of 3

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0010-22	20 Jan 2024

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certification is traceable to the International System of Unit.

Result of calibration () Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity : 0 g to 220 g Resolution 0.0001 g

Before Adjustment :

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
(g)	(g)	(g)	(± mg)	(k)
100	100.0002	-0.0002	0.21	2.06
200	200.0003	-0.0003	0.29	2.00

After Adjustment :

1. Determination of the standard deviation of weighing machine (n = 10)

Applied Weight	Standard Deviation of Reading (g)
(g)	
100	0.00009
200	0.00007

เอกสารไม่ควบคุม




Equipment : Electronic Balance
 Condition As-Received : Used Item
 Reference : 2304-0015OC-2

Cert.No.: 23MM332
 Page: 3 of 3

Result of calibration

2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.
 The weighing machine reading error obtained is given in the table



Maximum difference between off-center and central loading

Position 1	Position 2	Position 3	Position 4	Position 5	
(g)	(g)	(g)	(g)	(g)	(g)
+0.0001	-0.0003	+0.0003	+0.0006	+0.0002	0.0005

3. Departure from nominal value

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
(g)	(g)	(g)	(± mg)	(k)
Unload	0.0000	0.0000	0.18	2.17
0.1	0.0999	+0.0001	0.18	2.17
1	0.9998	+0.0002	0.18	2.17
5	5.0000	0.0000	0.18	2.17
10	10.0000	0.0000	0.18	2.17
20	20.0000	0.0000	0.18	2.15
50	50.0001	-0.0001	0.19	2.11
70	70.0001	-0.0001	0.20	2.07
100	100.0002	-0.0002	0.21	2.06
150	150.0004	-0.0004	0.29	2.00
200	200.0005	-0.0005	0.29	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANA KARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484




Cert.No.: 23MM333
Page.: 1 of 3

Certificate of Calibration

Equipment : Electronic Balance
Manufacturer : Mettler Toledo
Model : XP6
Serial No. : B322373893
ID No. : UAE.AIR.019/2556
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Balance Room 2
Received order : 07 April 2023
Calibration Date : 07 April 2023
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 60 %

Calibrated by : Suwit Imjai

Approved by : 
Approved Signatory

() Pornthippa Tameyakul
() Malee Butkruea

Issue Date : 10 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-00150C-3
Procedure used :-

Cert.No.: 23MM333

Page: 2 of 3

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15384	24053	70RC007	MM-0010-22	20 Jan 2024

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certification is traceable to the International System of Unit.

Result of calibration () Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity : 0 g to 6.1 g **Resolution** 0.000001 g

Before Adjustment :

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
(g)	(g)	(g)	(± mg)	(k)
3	2.999987	+0.000013	0.026	2.00
6	6.000003	-0.000003	0.036	2.00

After Adjustment :

1. Determination of the standard deviation of weighing machine (n = 10)

Applied Weight	Standard Deviation of Reading (g)
3	0.0000027
6	0.0000030

เอกสารไม่ควบคุม



Equipment : Electronic Balance
 Condition As-Received : Used Item
 Reference : 2304-00150C-3

Result of calibration


2. Effect of off center loading

A mass of 2 g was placed to various position on the pan.
 The weighing machine reading error obtained is given in the table

Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)
-0.000006	-0.000007	-0.000007	-0.000010	-0.000002

Cert.No.: 23MM333

Page: 3 of 3



Maximum difference between
 off-center and central loading
 (g)
 0.000004

3. Departure from nominal value

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
Unload	0.000000	0.000000	0.0060	2.37
0.01	0.009998	+0.000002	0.0060	2.13
0.05	0.050003	-0.000003	0.0070	2.05
0.1	0.100007	-0.000007	0.0090	2.03
0.15	0.150000	0.000000	0.011	2.00
0.17	0.169998	+0.000002	0.014	2.00
0.2	0.200002	-0.000002	0.014	2.00
1.5	1.500001	-0.000001	0.020	2.00
3	2.999990	+0.000010	0.028	2.00
4.5	4.499994	+0.000006	0.036	2.00
8	5.999982	+0.000018	0.038	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-c0o-

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.

DQE Services

32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com



CERTIFICATE OF CALIBRATION

Certificate No. : SP22-016

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong,
 Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009

ID No. : N/A

Received Date : 23 May 2022

Calibration Date : 23 May 2022

Issue Date : 26 May 2022

Condition Instrument : Good

Calibrated by :

Mr. Tanawut Rittidach
 Technical Manager

Approved by :

Ms. Chonthicha Sangngern
 Quality Manager

The calibration (result is applied) only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP22-016

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °CRelative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	95935	22 October 2023
Absorbance Standard set	25757	95929	22 October 2023
Wavelength Standard set	25806	95916	22 October 2023
Wavelength Standard set	25758	95915	22 October 2023

Traceability : This certification is traceable to the International System of Unit maintained at National -
Institute of Standards and Technology (NIST) through Sarna Scientific Limited.

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 90 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength : 0.1 nm.

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP22-016

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5787	0.5755	0.0032	0.0031	2.00
	1.0490	1.0436	0.0054	0.0029	2.00
	2.1900	2.1847	0.0053	0.0075	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5607	0.5588	0.0019	0.0034	2.00
	1.0247	1.0232	0.0015	0.0035	2.00
	2.1229	2.1211	0.0018	0.0082	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5236	0.5197	0.0039	0.0029	2.00
	0.9634	0.9625	0.0009	0.0028	2.00
	1.9763	1.9752	0.0011	0.0070	2.00
546.1	0.0000	-0.0001	0.0001	0.0028	2.00
	0.5191	0.5171	0.0020	0.0031	2.00
	1.0003	0.9984	0.0019	0.0033	2.00
	1.9987	1.9946	0.0041	0.0084	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5523	0.5509	0.0014	0.0030	2.00
	1.0809	1.0799	0.0010	0.0029	2.00
	2.0391	2.0329	0.0062	0.0080	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5601	0.5584	0.0017	0.0031	2.00
	1.0512	1.0498	0.0014	0.0029	2.00
	1.9294	1.9265	0.0029	0.0082	2.00

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP22-016

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
235	0.0000	0.0001	-0.0001	0.0050	2.00
	0.7478	0.7421	0.0057	0.0056	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8686	0.8619	0.0067	0.0059	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2912	0.2896	0.0016	0.0051	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6448	0.6403	0.0045	0.0055	2.00

REPORT OF CALIBRATION

Certificate No. : SP22-016

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor <i>k</i>
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.5	0.31	0.18	2.00
334.06	333.5	0.56	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	418.0	0.59	0.18	2.00
445.94	445.4	0.54	0.18	2.00
453.66	453.2	0.46	0.18	2.00
460.02	459.7	0.32	0.18	2.00
536.59	536.2	0.39	0.18	2.00
637.98	638.3	-0.32	0.18	2.00
431.38	431.0	0.38	0.18	2.00
472.50	472.5	0.00	0.18	2.00
513.47	513.5	-0.03	0.18	2.00
528.88	528.5	0.38	0.18	2.00
573.17	573.0	0.17	0.18	2.00
585.35	585.0	0.35	0.20	2.00
684.40	684.7	-0.30	0.18	2.00
740.72	740.8	-0.08	0.20	2.00
748.55	748.5	0.05	0.18	2.00
807.03	807.3	-0.27	0.18	2.00
879.28	879.0	0.28	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty e_f (measurement U is stated) is the standard uncertainty of measurement multiplied by the coverage factor k ,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- * Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

CERTIFICATE OF CALIBRATION

Certificate No. : SP23-007 Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : Hitachi

Model : U-1900

Serial No. : 2021-064

ID No. : UAE.WAS.006/2552

Received Date : 6 January 2023

Calibration Date : 6 January 2023

Issue Date : 10 January 2023

Condition Instrument : Used

Calibrated by : 
 (Mr. Tanawut Rittidach)

Technical Manager

Approved by : 
 (Ms. Chonthicha Sangern)

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

REPORT OF CALIBRATION

Certificate No. : SP23-007 Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	95935	22 October 2023
Absorbance Standard set	25757	95929	22 October 2023
Wavelength Standard set	25806	95916	22 October 2023
Wavelength Standard set	25758	95915	22 October 2023

Traceability : This certification is traceable to the International System of Unit maintained at National -
 Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 4.0 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

REPORT OF CALIBRATION

Certificate No. : SP23-007

Page 1 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5787	0.575	0.0037	0.0031	2.00
	1.0490	1.044	0.0050	0.0029	2.00
	2.1900	2.181	0.0090	0.0080	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5607	0.558	0.0027	0.0034	2.00
	1.0247	1.021	0.0037	0.0035	2.00
	2.1229	2.115	0.0079	0.0081	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5236	0.520	0.0036	0.0030	2.00
	0.9634	0.961	0.0024	0.0029	2.00
	1.9763	1.968	0.0083	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5191	0.518	0.0011	0.0031	2.00
	1.0003	1.000	0.0003	0.0033	2.00
	1.9987	1.993	0.0057	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5523	0.552	0.0003	0.0030	2.00
	1.0809	1.082	-0.0011	0.0030	2.00
	2.0391	2.031	0.0081	0.0080	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5601	0.562	-0.0019	0.0032	2.00
	1.0512	1.052	-0.0008	0.0030	2.00
	1.9294	1.923	0.0064	0.0079	2.00

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP23-007

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7478	0.743	0.0048	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8686	0.861	0.0076	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2912	0.291	0.0002	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6448	0.639	0.0058	0.0055	2.00

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP23-007

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor <i>k</i>
241.54	240.8	0.74	0.18	2.00
279.40	278.5	0.90	0.18	2.00
288.70	288.0	0.70	0.18	2.00
334.22	333.5	0.72	0.18	2.00
361.26	360.5	0.76	0.18	2.00
418.48	417.8	0.68	0.21	2.00
446.70	445.9	0.80	0.18	2.00
453.20	452.5	0.70	0.18	2.00
460.06	459.5	0.56	0.18	2.00
536.90	536.0	0.90	0.18	2.00
637.94	637.1	0.84	0.18	2.00
440.74	440.0	0.74	0.18	2.00
472.22	471.5	0.72	0.18	2.00
513.70	513.0	0.70	0.18	2.00
528.72	528.0	0.72	0.18	2.00
574.60	574.0	0.60	0.18	2.00
585.48	584.6	0.88	0.20	2.00
684.63	684.0	0.63	0.18	2.00
740.27	740.0	0.27	0.20	2.00
748.28	747.5	0.78	0.18	2.00
807.16	806.5	0.66	0.18	2.00
879.70	879.0	0.70	0.18	2.00

Remark : - UUC = 1/10 Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement *U* is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- * ISO/IEC 17025 (or TIS) accredited

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021



Certificate of Calibration

DX-120 : (Anion System ID#042)


This certificate is to verify that instrument below are calibrated

by Archemica Lab Co.,Ltd.

DX-120 S/N : 03010223

for

UAE Consultant Co.,Ltd.

Operator Signature : 

Date : Dec 9, 2022

(Mr.Channarong Khiao-un)

Test Engineer

เอกสารไม่ควบคุม

Qualification Report

**PM_Checklist : CM_OQ and PQ
DX-120 (ID#042)**

**For
UAE Consultant Co.,Ltd.
(2nd Contract)**

**Preventive Maintenance
Check List**

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Preventive Maintenance Checklist

Dionex Ion Chromatography
Preventive Maintenance Report

Customer Organization	Name/ Department
UAE Consultant Co., Ltd. (2nd Contract)	K Suwan
Engineer Name	Date
Mr. Channarong Khiao-Un	09-Dec-2022

Instrument Detail

Instrument Model	Application
DX-120 (ID#042)	Anion
Instrument components	Serial Number
DX-120	03010223

Consumable Detail

Columns	Guard Columns	Suppressors	Concentrators	Etc.
AS22	AG22	ASRS-300 4-mm	-	-
Remark:				

Perform By
Archimica Lab Co., Ltd.Archimica Lab Co., Ltd. บริษัท อารเคมีคัล แล็บ จำกัด
ARCHIMICA LAB CO., LTD.

Date

Customer
9/12/2022

Date

เอกสารไม่ควบคุม



Preventive Maintenance Checklist

General Inspection Checklist

Item	Description	Result		Action Taken	N.A.
		Pass	Fail		
1	Power line 220 Vac	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
2	Pneumatic Line	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
3	Pressure outlet 80-100 psi	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
4	Barbed fitting and tee fitting	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
5	Crimped and blocked tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
6	Rheodyne Valve for Leak	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
7	Slider valve for leak	<input type="checkbox"/>	<input type="checkbox"/>	-	<input checked="" type="checkbox"/>
8	Inspect slider	<input type="checkbox"/>	<input type="checkbox"/>	-	<input checked="" type="checkbox"/>
9	Inspect port face	<input type="checkbox"/>	<input type="checkbox"/>	-	<input checked="" type="checkbox"/>
10	Inspect pressure bolt	<input type="checkbox"/>	<input type="checkbox"/>	-	<input checked="" type="checkbox"/>
11	Inspect fitting and ferrule	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
12	Suppressor for leak	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
13	Cell for leak	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
14	Electronic cable connected	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
15	Column selection valve for leak	<input type="checkbox"/>	<input type="checkbox"/>	-	<input checked="" type="checkbox"/>
16	Inspect all fitting and line	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
17	Eluent reservoir	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
18	Inspect cap o-ring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
19	Inspect air for leak	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
20	Piston seal has been replaced	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
21	Back up seal has been replaced	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
22	Pump Lubricate	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
23	Front panel test	<input type="checkbox"/>	<input type="checkbox"/>	-	<input checked="" type="checkbox"/>
24	Low limit alarm	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
25	Hi limit alarm	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
26	Conductivity electronic test 160+/-1 uS	<input type="checkbox"/>	<input type="checkbox"/>	Checked	<input checked="" type="checkbox"/>
27	Check noise for suppressor (pk to pk <0.005uS)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
28	Check column	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
29	Check suppressor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
30	Check pump	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
31	Check cell	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
32	Check leak sensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
33	Flow rate	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
34	System pressure	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>
35	Detector background	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Checked	<input type="checkbox"/>

เอกสารไม่ควบคุม

Chromeleon Operational Qualification (CM_OQ)



Chromeleon Operational Qualification

General Information

Computer Name (Server): LAB-IC
Computer Name (Client): LAB-IC
Version Number: 6.80 SR12 Build 3578 (207169)
Operator: Mr.Channarong Khiao-Un

General System Suitability Test: *Test passed*

Comparison Formats:

All Parameters: (Exceptions see below)	Significant Digits: (They must match exactly)	10
Time Related Frac. Coll. Parameters: (The parameters are marked with *.)	Max. Deviation:	0.02 s

Simon 9/12/2022
Reviewer's Signature // Date


บริษัท อาร์เคมีโก้ แล็บ จำกัด
ARCHEMIG LAB CO.,LTD.
Channarong 9/12/2022
Operator's Signature // Date

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 1

Verification of Selected Results

Calibration Type: LOff
 Integration Type: Area
 Standard Method: External
 Calibration Mode: Total
 Auto Recalibrate: ON

Report Variable	Peak Name	Status
Offset (c0)	n.a.	ok
	n.a.	ok
	n.a.	ok
Slope (c1)	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok
Correlation Coeff.	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok
Variance	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok
Std. Deviation	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok
Rel. Std. Dev.	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok
Variance Coeff.	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 1

Verification of Selected Results

Report Variable	Peak Name	Status
Calibration Point X	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok
Calibration Point Y	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok
Amount [ng]	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok
Resolution (EP)	Methylparabene	ok
	Ethylparabene	ok
Resolution (USP)	Methylparabene	ok
	Ethylparabene	ok
Peak Asymmetry (EP/USP)	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok
Peak Asymmetry (AIA)	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 1

Verification of Selected Results

<u>Report Variable</u>	<u>Peak Name</u>	<u>Status</u>
Theoretical Plates (EP)	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok
Theoretical Plates (USP)	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok
Theoretical Plates (JP)	Methylparabene	ok
	Ethylparabene	ok
	Propylparabene	ok

Test Result: Passed

Reviewed by: Simon 9/10/2022
Reviewer's Signature // Date


บริษัท อาร์เคมิคัล แล็บ จำกัด
ARCHEMICA LAB CO., LTD.
K. N. K. 9/12/2022
Operator's Signature // Date

เอกสารไม่ควบคุม




Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Calibration Type:	LOff
Integration Type:	Area
Standard Method:	External
Calibration Mode:	Total
Auto Recalibrate:	ON

Variable Category	Report Variable	Peak Name	Status
Sample	No.		ok
	Name		ok
	Sample Type		ok
	Position		ok
	Status		ok
	Inj.Vol.		ok
	Dil.Fac.		ok
	Weight		ok
	Amount		ok
	Program		ok
	Quantification Method		ok
Chromatogram	Channel		ok
	No. of Peaks		ok
	Start Time		ok
	Signal Min.		ok
	Signal Max.		ok
	Signal Dimension		ok
	Noise 2.1-2.3		ok
Peak Results	No.	Methylparabene	ok
	No.	Ethylparabene	ok
	No.	Propylparabene	ok
	Peak Name	Methylparabene	ok
	Peak Name	Ethylparabene	ok
	Peak Name	Propylparabene	ok
	Ret.Time	Methylparabene	ok
	Ret.Time	Ethylparabene	ok
	Ret.Time	Propylparabene	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Results	Ret.Dev.(abs)	Methylparabene	ok
	Ret.Dev.(abs)	Ethylparabene	ok
	Ret.Dev.(abs)	Propylparabene	ok
	Ret.Dev.(rel)	Methylparabene	ok
	Ret.Dev.(rel)	Ethylparabene	ok
	Ret.Dev.(rel)	Propylparabene	ok
	Area	Methylparabene	ok
	Area	Ethylparabene	ok
	Area	Propylparabene	ok
	Rel.Area (Total)	Methylparabene	ok
	Rel.Area (Total)	Ethylparabene	ok
	Rel.Area (Total)	Propylparabene	ok
	Height	Methylparabene	ok
	Height	Ethylparabene	ok
	Height	Propylparabene	ok
	Rel.Height (Total)	Methylparabene	ok
	Rel.Height (Total)	Ethylparabene	ok
	Rel.Height (Total)	Propylparabene	ok
	Amount	Methylparabene	ok
	Amount	Ethylparabene	ok
	Amount	Propylparabene	ok
	Concentration	Methylparabene	ok
	Concentration	Ethylparabene	ok
	Concentration	Propylparabene	ok
	Rel.Amount	Methylparabene	ok
	Rel.Amount	Ethylparabene	ok
	Rel.Amount	Propylparabene	ok
	Peak Width (0%)	Methylparabene	ok
	Peak Width (0%)	Ethylparabene	ok
	Peak Width (0%)	Propylparabene	ok
	Peak Width (5%)	Methylparabene	ok
	Peak Width (5%)	Ethylparabene	ok
	Peak Width (5%)	Propylparabene	ok
	Peak Width (10%)	Methylparabene	ok
	Peak Width (10%)	Ethylparabene	ok
	Peak Width (10%)	Propylparabene	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Results	Peak Width (50%)	Methylparabene	ok
	Peak Width (50%)	Ethylparabene	ok
	Peak Width (50%)	Propylparabene	ok
	Left Width (0%)	Methylparabene	ok
	Left Width (0%)	Ethylparabene	ok
	Left Width (0%)	Propylparabene	ok
	Right Width (0%)	Methylparabene	ok
	Right Width (0%)	Ethylparabene	ok
	Right Width (0%)	Propylparabene	ok
	Peak Start	Methylparabene	ok
	Peak Start	Ethylparabene	ok
	Peak Start	Propylparabene	ok
	Peak Stop	Methylparabene	ok
	Peak Stop	Ethylparabene	ok
	Peak Stop	Propylparabene	ok
	Peak Start Value	Methylparabene	ok
	Peak Start Value	Ethylparabene	ok
	Peak Start Value	Propylparabene	ok
	Peak Stop Value	Methylparabene	ok
	Peak Stop Value	Ethylparabene	ok
	Peak Stop Value	Propylparabene	ok
	BL-Value Peak Start	Methylparabene	ok
	BL-Value Peak Start	Ethylparabene	ok
	BL-Value Peak Start	Propylparabene	ok
	BL-Value Peak Stop	Methylparabene	ok
	BL-Value Peak Stop	Ethylparabene	ok
	BL-Value Peak Stop	Propylparabene	ok
	Type	Methylparabene	ok
	Type	Ethylparabene	ok
	Type	Propylparabene	ok
	Resolution(EP)	Methylparabene	ok
	Resolution(EP)	Ethylparabene	ok
	Resolution(USP)	Methylparabene	ok
	Resolution(USP)	Ethylparabene	ok
	Asymmetry(EP)	Methylparabene	ok
	Asymmetry(EP)	Ethylparabene	ok
	Asymmetry(EP)	Propylparabene	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Results	Asymmetry(AIA)	Methylparabene	ok
	Asymmetry(AIA)	Ethylparabene	ok
	Asymmetry(AIA)	Propylparabene	ok
	Theoretical Plates(EP)	Methylparabene	ok
	Theoretical Plates(EP)	Ethylparabene	ok
	Theoretical Plates(EP)	Propylparabene	ok
	Theoretical Plates(USP)	Methylparabene	ok
	Theoretical Plates(USP)	Ethylparabene	ok
	Theoretical Plates(USP)	Propylparabene	ok
	Theoretical Plates(JF)	Methylparabene	ok
	Theoretical Plates(JF)	Ethylparabene	ok
	Theoretical Plates(JF)	Propylparabene	ok
Peak Calibration	Cal.Mode	Methylparabene	ok
	Cal.Mode	Ethylparabene	ok
	Cal.Mode	Propylparabene	ok
	Auto.Recal.	Methylparabene	ok
	Auto.Recal.	Ethylparabene	ok
	Auto.Recal.	Propylparabene	ok
	Cal.Type	Methylparabene	ok
	Cal.Type	Ethylparabene	ok
	Cal.Type	Propylparabene	ok
	Weights	Methylparabene	ok
	Weights	Ethylparabene	ok
	Weights	Propylparabene	ok
	Offset	Methylparabene	ok
	Offset	Ethylparabene	ok
	Offset	Propylparabene	ok
	Slope	Methylparabene	ok
	Slope	Ethylparabene	ok
	Slope	Propylparabene	ok
	RF-Value	Methylparabene	ok
	RF-Value	Ethylparabene	ok
	RF-Value	Propylparabene	ok
	No. of Points	Methylparabene	ok
	No. of Points	Ethylparabene	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Calibration	No. of Points	Propylparabene	ok
	No. of Points(disabled)	Methylparabene	ok
	No. of Points(disabled)	Ethylparabene	ok
	No. of Points(disabled)	Propylparabene	ok
	Variance	Methylparabene	ok
	Variance	Ethylparabene	ok
	Variance	Propylparabene	ok
	Var.Coeff	Methylparabene	ok
	Var.Coeff	Ethylparabene	ok
	Var.Coeff	Propylparabene	ok
	Std.Dev.	Methylparabene	ok
	Std.Dev.	Ethylparabene	ok
	Std.Dev.	Propylparabene	ok
	Rel.Std.Dev.	Methylparabene	ok
	Rel.Std.Dev.	Ethylparabene	ok
	Rel.Std.Dev.	Propylparabene	ok
	Corr.Coeff.	Methylparabene	ok
	Corr.Coeff.	Ethylparabene	ok
	Corr.Coeff.	Propylparabene	ok
	Coeff.Det.	Methylparabene	ok
	Coeff.Det.	Ethylparabene	ok
	Coeff.Det.	Propylparabene	ok
	Adj. Coeff.Det.	Methylparabene	ok
	Adj. Coeff.Det.	Ethylparabene	ok
	Adj. Coeff.Det.	Propylparabene	ok
	X	Methylparabene	ok
	X	Ethylparabene	ok
	X	Propylparabene	ok
	Y	Methylparabene	ok
	Y	Ethylparabene	ok
	Y	Propylparabene	ok
	W	Methylparabene	ok
	W	Ethylparabene	ok
	W	Propylparabene	ok
	F(X)	Methylparabene	ok
	F(X)	Ethylparabene	ok
	F(X)	Propylparabene	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Calibration	Residual for Cal.Point X	Methylparabene	ok
	Residual for Cal.Point X	Ethylparabene	ok
	Residual for Cal.Point X	Propylparabene	ok
	Calibration Point Status	Methylparabene	ok
	Calibration Point Status	Ethylparabene	ok
	Calibration Point Status	Propylparabene	ok
	Amount	Methylparabene	ok
	Amount	Ethylparabene	ok
Peak Table	Amount	Propylparabene	ok
	Peak Tab. Cal.Type	Methylparabene	ok
	Peak Tab. Peak Type	Methylparabene	ok
	Peak Tab. Left Limit	Methylparabene	ok
	Peak Tab. Right Limit	Methylparabene	ok
	Peak Tab. Group	Methylparabene	ok
	Peak Tab. Resp.Factor	Methylparabene	ok
	Peak Tab. Amount	Methylparabene	ok
	Peak Tab. Amnt.Dim	Methylparabene	ok



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Purity	PPI	Methylparabene	ok
	PPI	Ethylparabene	ok
	PPI	Propylparabene	ok
	RSD PPI	Methylparabene	ok
	RSD PPI	Ethylparabene	ok
	RSD PPI	Propylparabene	ok
	Match	Methylparabene	ok
	Match	Ethylparabene	ok
	Match	Propylparabene	ok
	RSD Match	Methylparabene	Deviation
	RSD Match	Ethylparabene	Deviation
	RSD Match	Propylparabene	Deviation
	Rel.Max at	Methylparabene	ok
	Rel.Max at	Ethylparabene	ok
	Rel.Max at	Propylparabene	ok

Test Result: **Failed**

Simon 9/12/2022
 Reviewer's Signature // Date


 บริษัท อารเคมีโก้ จำกัด
 ARCHEMICA LAB. CO., LTD.
Simon 9/12/2022
 Operator's Signature // Date

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 3

Post-Acquisition Steps: Comparison with Expected Results

Calibration Type: LOFF
 Integration Type: Area
 Standard Method: External
 Calibration Mode: Total
 Auto Recalibrate: ON

Channel Name	Report Variable	Peak Name	Status
Extract UV Channel:			
EXT230NM	Area	Methylparabene	ok
	Area	Ethylparabene	ok
	Area	Propylparabene	ok
	Height	Methylparabene	ok
	Height	Ethylparabene	ok
	Height	Propylparabene	ok
	Base Peak Width	Methylparabene	ok
	Base Peak Width	Ethylparabene	ok
	Base Peak Width	Propylparabene	ok
EXT290NM	Area	Methylparabene	ok
	Area	Ethylparabene	ok
	Area	Propylparabene	ok
	Height	Methylparabene	ok
	Height	Ethylparabene	ok
	Height	Propylparabene	ok
	Base Peak Width	Methylparabene	ok
	Base Peak Width	Ethylparabene	ok
	Base Peak Width	Propylparabene	ok
Smooth Data:			
UV_VIS_1_MA_005_001	Noise (1.9-2.4 min)		ok
UV_VIS_1_OL_051_001	Noise (1.9-2.4 min)		ok
EXT290NM_SG_005_010	Noise (1.9-2.4 min)		ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 3

Post-Acquisition Steps: Comparison with Expected Results

Channel Name	Report Variable	Peak Name	Status
Arith. Comb. of Channels:			
ADD_UV_VIS_1_UV_VIS_1	Area	Methylparabene	ok
ADD_UV_VIS_1_UV_VIS_1	Area	Ethylparabene	ok
ADD_UV_VIS_1_UV_VIS_1	Area	Propylparabene	ok
MUL_UV_VIS_1_UV_VIS_1	Area	Methylparabene	ok
MUL_UV_VIS_1_UV_VIS_1	Area	Ethylparabene	ok
MUL_UV_VIS_1_UV_VIS_1	Area	Propylparabene	ok

Test Result: Passed



Signature 9/12/2022
 Reviewer's Signature // Date

Signature 9/12/2022
 Operator's Signature // Date

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 4

System Suitability Test: Comparison with Expected Results

Calibration Type: LOff
 Integration Type: Area
 Standard Method: External
 Calibration Mode: Total
 Auto Recalibrate: ON

Variable Category	Report Variable	Status
SST	Test No.	ok
	Test Name	ok
	Sample Condition	ok
	Sample Condition Result	ok
	Test Condition	ok
	Peak Condition	ok
	Aggregate Condition	ok
	Compare Operator	ok
	Compare Value	ok
	Result of Compare Value	ok
	Channel	ok
	Aggregated Samples	ok
	List of Aggr. Smp.	ok
	Result List for Aggr. Smp.	ok
	Result of Test Condition or Aggregate	ok
	N.A.	ok
	Test Result	ok
	Fail-Action	ok

Test Result: **Passed**



K. K. K. 9/12/2022
 Operator's Signature // Date

S. S. 9/12/2022
 Reviewer's Signature // Date

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 5

Fraction Collection: Comparison with Expected Results

Calibration Type: LOff
 Integration Type: Area
 Standard Method: External
 Calibration Mode: Total
 Auto Recalibrate: ON

Variable Category	Report Variable	Status
Fraction Report	Fract. No.	ok
	Fract. Starttime *)	ok
	Fract. Endtime *)	ok
	No. of Tubes	ok
	Position	ok
	Peak Name	ok
	No. of Peaks	ok
Tube Report	Position	ok
	Tube Starttime *)	ok
	Tube Endtime *)	ok
	Max. Tube Volume	ok
	Peak Name	ok
	No. of Peaks	ok
	Fract. No.	ok
	Fract. Starttime *)	ok
	Fract. Endtime *)	ok
	No. of Tubes	ok
	No. of Peaks	ok

Test Result: **Passed**



K. K. K. 9/12/2022
 Operator's Signature // Date

S. S. 9/12/2022
 Reviewer's Signature // Date

เอกสารไม่ควบคุม

Performance Qualification (PQ)

Sequence: PQ_1/C_ Warm-Up
Sample: Water WL

Page 1 of 2
Date: 12/9/2022



Performance Qualification

Instruments:

Instrument Name	Model	Supplier	Serial Number	Moduleware Version
Pump	DX120	Dionex	03010223	3.03
Detector	DX120	Dionex	03010223	3.03
Autosampler	AS40 or man inj.	Dionex	n.a.	0.00
Eluent Generator	n.a.	Dionex	n.a.	0.00
Chromeleon	5.6C SR12 Build 3578 (2017169)	Dionex	33305	n.a.

Accessories:

Name	Description	Lot	Serial Number	Expire Date
Backpressure Tubing	0.13 mm (0.008" ID PEEK, 18 in (512"))	n.a.		n.a.
Blank	Water	n.a.		n.a.
Sample 1	Nitrate, 5 ppm	220203		Feb-2023
Sample 2	Nitrate, 10 ppm	220203		Feb-2023
Sample 3	Nitrate, 25 ppm	220203		Feb-2023
Sample 4	Nitrate, 50 ppm	220203		Feb-2023
Sample 5	Nitrate, 100 ppm	220203		Feb-2023
Sample 6	Nitrate, 1000 ppm	220203		Feb-2023
Eluent	Water	n.a.		n.a.
Autosampler Reservoir A	Water	n.a.		n.a.



Signature 9/12/2022

Signature

Signature

Customer Signature

Qualification Executor

Date

Customer signature indicates that all information in the following reports has been reviewed and accepted.

PeakNet (c) DIONEX 2021
Version: 3.60 SR12 Build: 3578 (2017169)

PQ_PQ_DX2C_Validation / Specification
Printed: 12/9/2022 (0:55 AM)

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Limits:

Test	Customized Limits	Dionex Recommended Limits
DX120 Conductivity Noise (nS)	2	2
DX120 Conductivity Drift (nS/hr)	20	20
Injector Precision (Area %RSD)	1.0	1.0
Injector Carry Over (Area %)	0.1	0.1
DX120 Detector Linearity (Corr.)	0.999	0.999
DX120 Detector Linearity (%RSD)	5	5

Additional Information:

Customer/Company:	UAE Consultant Co.,Ltd.	Date:	9-Dec-2022
Qualification Executor:	Mr.Channarong / Archemica	Period between Qualifications:	12 months
		Next Qualification:	Dec-2023



Signature
Customer Signature

Signature
Qualification Executor

9/12/2022
Date

เอกสารไม่ควบคุม



Performance Qualification

Detector Noise and Drift

Instruments:

Instrument Name	Model	Supplier	Serial Number	Moduleware Version
Pump	DX120	Dionex	03010223	3.03
Detector	DX120	Dionex	03010223	3.03
Autosampler	AS40 (on main line)	Dionex	n.a.	0.00
Eluent Generator	n.a.	Dionex	n.a.	0.00

Accessories

Name	Description
Backpressure Tubing	0.13 mm (0.005") ID PEEK, 13 m (5'12")
Eluent	Water

Additional Information

Customer/Company:	UAE Consultant Co.,Ltd.	Date:	9-Dec-2022
Qualification Executor:	Mr.Channarong / Archemica	Next Qualification:	Dec-2023

Test Results Summary

Test	Result
DX120 Conductivity Noise (nS)	PASS
DX120 Conductivity Drift (nS/hr)	PASS



Signature
Customer Signature

Signature
Qualification Executor

9/12/2022
Date

เอกสารไม่ควบคุม

Data for detector noise

Segment number	Noise, nS
1	0.773
2	0.871
3	1.301
4	0.936
5	0.861
6	0.409
7	1.624
8	0.991
9	0.750
10	0.877
11	0.570
12	1.009
13	0.861
14	1.135
15	0.688
16	0.669
17	1.480
18	1.206
19	0.691
20	0.910
Average, nS	0.930
Limit, nS	2
Result	PASS

Data for detector drift

20 Minute drift, nS	Drift, nS/hr	Limit, nS/hr	Result
0.553	1.660	20.000	PASS


Customer Signature



ARCHEMICA LAB
บริษัท อารีเคมีคอล แล็บ จำกัด
ARCHEMICA LAB CO.,LTD.

Qualification Executor

9/12/2022
Date

เอกสารไม่ควบคุม

Chromatogram of Detector Noise and Drift

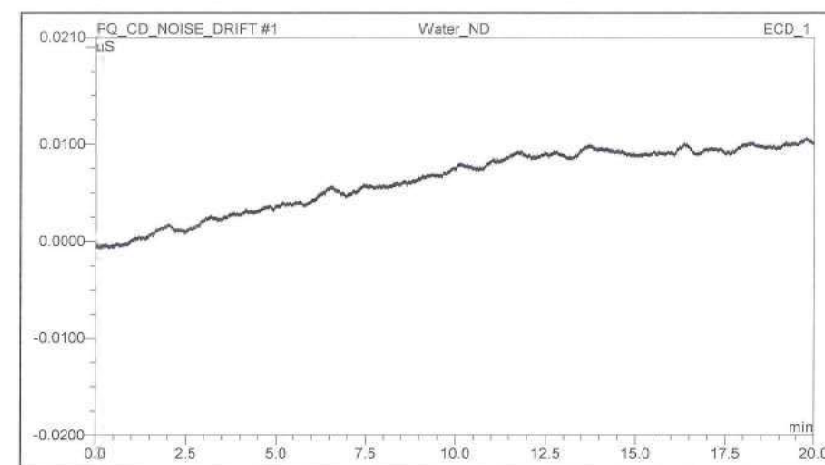


Customer Signature


ARCHEMICA LAB
บริษัท อารีเคมีคอล แล็บ จำกัด
ARCHEMICA LAB CO.,LTD.

Qualification Executor

9/12/2022
Date

เอกสารไม่ควบคุม



Performance Qualification

Injector Precision

Instruments:

Instrument Name	Model	Supplier	Serial Number	Moduleware Version
Pump	DX120	Dionex	03010223	3.05
Detector	DX120	Dionex	03010223	3.05
Autosampler	AS40 Smart III	Dionex	n.a.	0.00
Eluent Generator	n.a.	Dionex	n.a.	0.00

Accessories

Name	Description
Backpressure Tubing	0.10 mm ID 005' ID PEEK, 50 mm (5'2")
Sample 5	Nitrate 100 ppm
Eluent	Water

Additional Information

Customer/Company:	UAE Consultant Co., Ltd.	Date:	9-Dec-2022
Qualification Executor	Mr. Channetong Archemita	Next Qualification:	Dec-2023

Test Results Summary

Test	Result
Injector Precision (Area %RSD)	PASS




Customer Signature


Qualification Executor

9/12/2022
Date

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Data for Injector Precision test

Name	Area uS/min Nitrate ECD_1
Inj Precision_1	1.678
Inj Precision_2	1.671
Inj Precision_3	1.672
Inj Precision_4	1.662
Inj Precision_5	1.654
Inj Precision_6	1.648
Inj Precision_7	1.671
Inj Precision_8	1.670
Inj Precision_9	1.674
Inj Precision_10	1.668
Average:	1.667
Std. Dev:	0.009
% RSD:	0.560 %
Limit:	1.0 %
Result:	PASS


Customer Signature


Qualification Executor

9/12/2022
Date

เอกสารไม่ควบคุม



Performance Qualification

Injector Carry Over

Instruments:

Instrument Name	Model	Supplier	Serial Number	Moduleware Version
Pump	DX120	Dionex	03010223	3.03
Detector	DX120	Dionex	03010223	3.03
Autosampler	AS40 (or later)	Dionex	n.a.	0.00
Eluent Generator	n.a.	Dionex	n.a.	0.00

Accessories

Name	Description
Backpressure Tubing	Ø 1/8" (3.18 mm) ID PEEK, 15 ft (4.57 m)
Sample 6	Nitrate 1000 ppm
Blank	Water
Eluent	Water

Additional Information

Customer/Company:	UAE Consultant Co., Ltd.	Date:	9-Dec-2022
Qualification Executor:	Mr. Chantarang / Archemica	Next Qualification:	Dec-2023

Test Results Summary

Test	Result
Injector Carry Over (Area %)	PASS



Customer Signature


Qualification Executor

9/12/2022
Date

เอกสารไม่ควบคุม

Chromatogram for Carry Over test

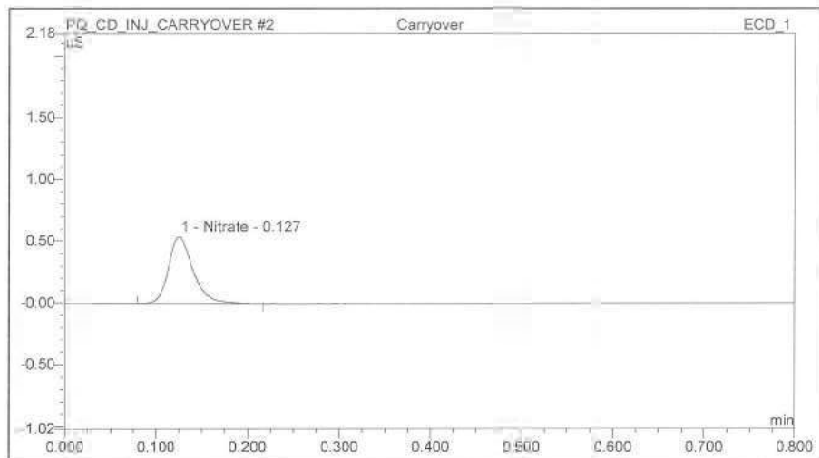

Data for Carry Over test

Name	Ret. Time (detected) min	Area uS*min
	Nitrate	Nitrate
	ECD_1	ECD_1
High Level	0.12	30.066
Carryover	0.13	0.017
Water	0.12	0.010
Carry over:		0.035 %
Limit:		0.1 %
Result:		PASS

Signature
Customer Signature

Signature
Qualification Executor

9/12/2022
Date

เอกสารไม่ควบคุม



Performance Qualification

Detector Linearity

Instruments:

Instrument Name	Model	Supplier	Serial Number	Moduleware Version
Pump	DX120	Dionex	03010223	3.03
Detector	DX120	Dionex	03010223	3.03
Autosampler	AS10 autosampler	Dionex	n.a.	0.00
Eluent Generator	n.a.	Dionex	n.a.	0.00

Accessories

Name	Description
Backpressure Tubing	0.13 mm ID, 0.002" ID, 15 m (5.12')
Sample 1	Nitrate, 5 ppm
Sample 2	Nitrate, 10 ppm
Sample 3	Nitrate, 25 ppm
Sample 4	Nitrate, 50 ppm
Sample 5	Nitrate, 100 ppm
Eluent	Water

Additional Information

Customer/Company	UAE Consultant Co., Ltd.	Date:	9-Dec-2022
Qualification Executor	Mr. Chanmarong / Archemica	Next Qualification:	Dec-2023

Test Results Summary

Test	Result
DX120 Detector Linearity (Corr.)	PASS
DX120 Detector Linearity (%RSD)	PASS

Signature
Customer Signature

Signature
Qualification Executor


9/12/2022
Date

เอกสารไม่ควบคุม

Data for Detector Linearity

Name	Amount ppm Nitrate ECD_1	Height uS Nitrate ECD_1
Detector linearity_1	5.000	4.956
Detector linearity_2	10.000	9.972
Detector linearity_3	25.000	25.762
Detector linearity_4	50.000	50.334
Detector linearity_5	100.000	99.921

Linearity Plot

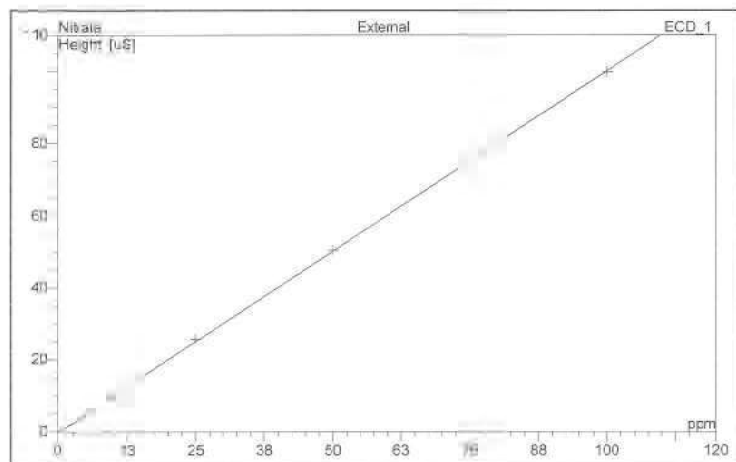

Calibration Type	Number of Points	Offset	Slope
Lin	5	0.000	1.002

	Correlation Coefficient	% RSD
Linearity:	1.000	1.362
Limit:	0.999	5
Result:	PASS	PASS



[Signature]
Customer Signature

[Signature]
Qualification Executor

9/12/2022
Date

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

CERTIFICATE

การอบรมเฉพาะตัว

The world leader in serving science

The certificate is only valid during employment with the Thermo Fisher Scientific including its subsidiaries and certified contractors.

Valid for 3 years from:
Nov/19/2021



K. Channarong 9/12/2022

Issued electronically and
approved by:
TFS - Learning Management
System, Training, Mentoring,
and Certification Group
tmc.training@thermofisher.com

eLearn: RPG IC-Specific Qualification Service Training

Has successfully completed

Channarong Khiao-Un

This certifies that

Certificate of Completion

ThermoFisher
SCIENTIFIC

Certificate of Analysis

Better Separations Through
Better Chemistry

Dionex Nitrate OQ/PQ IC Standards Kit (Set of 6)

Product Number 060254
Certificate of Analysis

Lot Number 220208

Expiration of Certification
February 2023

The Dionex Nitrate Standard was developed to aid the analysis of anions by Ion Chromatography (IC). The single-ion standard was prepared by the dissolution of high-purity salt in ≥ 18.2 megohm deionized water, which was tested by IC for ionic contaminants. The bottle label states the nominal concentration value of the ionic component for informational purposes only. The actual ion concentration value was determined by Ion Chromatography. The IC system was standardized using the National Institute of Standards & Technology (NIST), Standard Reference Material, SRM 3185 (Nitrate Standard Solution). Actual concentration values determined for the single-ion is listed below.

Dionex Nitrate Standard

Vial #	Concentration (mg/L)
1	5.07 \pm 0.03
2	10.09 \pm 0.04
3	24.97 \pm 0.13
4	49.83 \pm 0.13
5	99.6 \pm 1
6	996 \pm 3

ARCHCHEMICAL LAB
ARCHCHEMICAL LAB CO., LTD
K. Channarong
9/12/2022

The concentration value is based a proven reliable method of analysis. The estimated uncertainties are two standard deviations of the concentration value. The concentration value is warranted to be stable for one year from the date of manufacture.

The preparation and analyses of the Dionex Nitrate Standard was performed with extreme care by Thermo Scientific Corporation Consumables Manufacturing Department in Sunnyvale California.

Document No. 078698-01 26-Dec-2011

thermo.com/thermo/dionex

© 2011 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific Inc. or its subsidiaries. Reproduction, translation, and distribution are prohibited without written permission. Please consult your local sales representative for details.

XX21146 EN 0215S 031316-10

Thermo Fisher Scientific
1223 Trap Way
P.O. Box 3603
Sunnyvale, CA 94088-3603
(408) 737-0700



Thermo Fisher Scientific
Sunnyvale, CA 94088-3603
(408) 737-0700

thermo
scientific

เอกสารไม่ควบคุม