

ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B35	B35	01/05/2023	$y = 1.310x - 9.363$	0.996
B36	B36	02/05/2023	$y = 1.201x - 4.686$	0.999
B37	B37	02/05/2023	$y = 1.239x - 4.586$	0.998
B38	B38	02/05/2023	$y = 1.304x - 9.606$	0.997
B39	B39	01/05/2023	$y = 1.240x - 5.469$	0.998
B40	B40	03/05/2023	$y = 1.196x - 4.045$	0.999
B41	B41	03/05/2023	$y = 1.179x - 2.611$	0.999
B42	B42	02/05/2023	$y = 1.246x - 7.813$	0.996
B43	B43	02/05/2023	$y = 1.206x - 3.694$	0.999
B44	B44	02/05/2023	$y = 1.302x - 9.108$	0.999
R01	R01	02/05/2023	$y = 1.268x - 7.113$	0.995
R02	R02	01/05/2023	$y = 1.235x - 6.759$	0.997
R03	R03	03/05/2023	$y = 1.247x - 7.848$	0.996
R04	R04	02/05/2023	$y = 1.161x - 1.778$	0.999
R05	R05	02/05/2023	$y = 1.288x - 9.494$	0.999
R06	R06	02/05/2023	$y = 1.277x - 6.891$	0.997
R07	R07	02/05/2023	$y = 1.046x + 2.772$	1.000
R08	R08	02/05/2023	$y = 1.206x - 5.068$	0.997
R09	R09	02/05/2023	$y = 1.296x - 8.463$	0.999
R10	R10	02/05/2023	$y = 1.244x - 6.477$	0.999
R11	R11	02/05/2023	$y = 1.097x - 0.462$	0.998
R12	R12	02/05/2023	$y = 1.210x - 5.084$	0.998
R13	R13	01/05/2023	$y = 1.149x - 1.965$	1.000
R14	R14	01/05/2023	$y = 1.189x - 3.035$	0.998
R15	R15	02/05/2023	$y = 1.161x - 3.437$	0.998
R16	R16	01/05/2023	$y = 1.158x - 4.330$	0.997
R17	R17	02/05/2023	$y = 1.218x - 5.356$	0.998
R18	R18	02/05/2023	$y = 1.234x - 5.546$	0.999
R19	R19	02/05/2023	$y = 1.267x - 7.058$	0.999
R20	R20	01/05/2023	$y = 1.264x - 8.743$	0.999

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.comCERTIFICATE No : 23M2441
REFERENCE No : 68471-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY : 

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 23M2441

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23° C \pm 1° C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
 Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	DH _@ (mmH ₂ O)
B01	1563	02/03/2023	0.998	50.11
B02	8002514	03/03/2023	1.004	49.25
B03	1503016	03/03/2023	1.002	50.62
B04	00006659	02/03/2023	1.004	50.14
B05	00007428	03/03/2023	1.001	49.76
R01	1561	01/03/2023	0.997	49.86
R02	8002513	03/03/2023	0.996	49.93
R03	1570	02/03/2023	1.003	49.57
R04	8002519	01/03/2023	1.002	48.90
R05	1503015	01/03/2023	0.998	50.20

Remark : Accept Value of y (test) is $0.97 < y < 1.03$

Accept Value of $\Delta H_{@}$ (test) is 46.7 ± 6.4 (mmH₂O)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	02/05/2023	0.84	0.84
B37	S	0.99	02/05/2023	0.83	0.84
B38	S	0.99	03/05/2023	0.85	0.84
B39	S	0.99	03/05/2023	0.84	0.83
B40	S	0.99	02/05/2023	0.84	0.83
B41	S	0.99	02/05/2023	0.84	0.84
B44	S	0.99	03/05/2023	0.85	0.84
B45	S	0.99	03/05/2023	0.85	0.84
B46	S	0.99	04/05/2023	0.84	0.83
B47	S	0.99	03/05/2023	0.84	0.85
B48	S	0.99	03/05/2023	0.83	0.84
B49	S	0.99	03/05/2023	0.85	0.84
B54	S	0.99	03/05/2023	0.83	0.84
B56	S	0.99	02/05/2023	0.84	0.85
B57	S	0.99	02/05/2023	0.84	0.83
B58	S	0.99	02/05/2023	0.85	0.84

Remark : Accept value of Cp (test) is 0.84 ± 0.01



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VACUUM GAUGE
MANUFACTURER : HI-LIGHT
MODEL / TYPE : N/A
SERIAL NO. : N/A[64-220066-1]
CLID. NO. : 212201112
JOB CONTROL NO. : 220720073201


CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 20 July 2022

DATE OF ISSUED : 22 July 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer



Approved By :

Authorized Signatory
22 July 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22073201

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : VACUUM GAUGE
MANUFACTURER : HI-LIGHT
MODEL / TYPE : N/A
SERIAL NO. : N/A[64-220066-1]
DATE OF CALIBRATION : 21 July 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-05** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 744 S/N. 9226007 with Pressure Module Model 700PV4 S/N. 19298401.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. MP-0196-21, Due Date 17 November 2022.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q22073201

F3-011-04/01-12

page 2 of 3



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (inHg)	STD Reading (inHg)		Correction (inHg)	
	Up	Down	Up	Down
0	0.0	0.0	0.0	0.0
-5	-4.6	-4.7	+0.4	+0.3
-10	-9.5	-9.6	+0.5	+0.4
-15	-14.4	-14.5	+0.6	+0.5
-20	-19.4	-19.5	+0.6	+0.5
-25	-24.5	-24.5	+0.5	+0.5
-30	-29.5	-29.5	+0.5	+0.5

Uncertainty of measurement ± 0.2 inHg

Transmitting fluid : Air.

Technical Note. k factor 1 kPa = 0.2952998 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 36 of 54

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22073201

F3-011-04/01-12

page 3 of 3



@clccalibration



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R²
B01	SKC	224-PCXR4	262101	04/04/2023	1,000	1,500	2,000	994	1,498	2,003	1.005x - 7.897	1.000
B02	SKC	224-PCXR4	626166	04/04/2023	1,000	1,500	2,000	1,004	1,503	2,003	1.010x - 19.866	0.999
B03	SKC	224-PCXR4	612968	07/04/2023	1,000	1,500	2,000	995	1,496	2,001	1.007x - 13.664	1.000
B04	SKC	224-PCXR4	602804	05/04/2023	1,000	1,500	2,000	998	1,499	1,994	0.999x - 1.611	1.000
B05	SKC	224-PCXR4	612693	07/04/2023	1,000	1,500	2,000	1,002	1,501	2,004	1.014x - 24.856	0.999
B06	SKC	224-PCXR4	262188	07/04/2023	1,000	1,500	2,000	994	1,509	2,006	1.012x - 21.589	0.999
B07	SKC	224-PCXR4	626262	04/04/2023	1,000	1,500	2,000	997	1,490	1,996	0.994x + 3.454	1.000
B08	SKC	224-PCXR4	626100	04/04/2023	1,000	1,500	2,000	1,001	1,499	2,005	1.015x - 27.137	0.999
B09	SKC	224-PCXR4	626479	05/04/2023	1,000	1,500	2,000	997	1,492	1,994	0.994x + 2.385	1.000
B10	SKC	224-PCXR4	091950	03/04/2023	1,000	1,500	2,000	993	1,504	2,005	1.013x - 23.779	1.000
B11	SKC	224-PCXR8	564315	10/04/2023	1,000	1,500	2,000	995	1,492	1,998	1.002x - 7.259	1.000
B12	SKC	224-PCXR4	034656	04/04/2023	1,000	1,500	2,000	1,002	1,504	2,001	1.009x - 17.609	0.999
B13	SKC	224-PCXR4	602073	04/04/2023	1,000	1,500	2,000	997	1,501	2,000	1.004x - 7.622	1.000
B14	SKC	224-PCXR4	626313	03/04/2023	1,000	1,500	2,000	997	1,492	1,991	0.996x + 1.699	1.000
B15	SKC	224-PCXR4	626474	07/04/2023	1,000	1,500	2,000	1,003	1,503	2,006	1.013x - 23.245	0.999
B16	SKC	224-PCXR4	626477	03/04/2023	1,000	1,500	2,000	995	1,506	2,003	1.011x - 22.132	0.999
B17	SKC	224-PCXR4	626860	04/04/2023	1,000	1,500	2,000	996	1,493	1,993	1.000x - 4.627	1.000
B18	SKC	224-PCXR4	691484	04/04/2023	1,000	1,500	2,000	1,001	1,496	2,002	1.010x - 21.179	0.999
B19	SKC	224-PCXR4	691599	04/04/2023	1,000	1,500	2,000	994	1,504	2,000	1.006x - 10.498	1.000
B20	SKC	224-PCXR4	691587	03/04/2023	1,000	1,500	2,000	991	1,502	2,000	1.016x - 35.102	0.999
B21	SKC	224-PCXR4	691531	04/04/2023	1,000	1,500	2,000	994	1,501	1,995	1.001x - 5.153	1.000
B22	SKC	224-PCXR4	691654	07/04/2023	1,000	1,500	2,000	1,000	1,502	2,004	1.014x - 25.574	0.999
B23	SKC	224-PCXR4	798393	05/04/2023	1,000	1,500	2,000	990	1,508	2,004	1.013x - 23.994	1.000
B24	SKC	224-PCXR4	626363	03/04/2023	1,000	1,500	2,000	1,002	1,503	1,999	1.009x - 18.837	0.999
B25	SKC	224-PCXR4	798489	07/04/2023	1,000	1,500	2,000	1,002	1,494	2,000	0.997x + 3.494	1.000
B26	SKC	224-PCXR4	798479	07/04/2023	1,000	1,500	2,000	1,001	1,501	1,994	0.995x + 5.564	1.000
B27	SKC	224-PCXR4	691673	04/04/2023	1,000	1,500	2,000	995	1,505	2,004	1.013x - 25.091	0.999
B28	SKC	224-PCXR4	691570	04/04/2023	1,000	1,500	2,000	1,003	1,501	2,001	1.010x - 19.922	0.999
B29	SKC	224-PCXR4	626472	05/04/2023	1,000	1,500	2,000	1,001	1,498	2,000	0.999x - 1.831	1.000
B30	SKC	224-PCXR4	691489	04/04/2023	1,000	1,500	2,000	1,002	1,507	2,003	1.009x - 13.936	0.999
B31	SKC	224-PCXR4	691509	07/04/2023	1,000	1,500	2,000	994	1,496	1,997	1.004x - 9.680	1.000
B32	SKC	224-PCXR4	091567	10/04/2023	1,000	1,500	2,000	992	1,506	2,001	1.013x - 25.542	0.999
B33	SKC	224-PCXR4	091756	05/04/2023	1,000	1,500	2,000	993	1,498	1,992	0.998x - 1.121	1.000
B34	SKC	224-PCXR4	612962	07/04/2023	1,000	1,500	2,000	1,002	1,503	2,003	1.008x - 14.753	0.999
B35	SKC	224-PCXR4	602682	05/04/2023	1,000	1,500	2,000	991	1,497	1,996	1.003x - 11.598	1.000
B36	SKC	224-PCXR4	626164	05/04/2023	1,000	1,500	2,000	997	1,495	1,998	1.002x - 8.097	1.000
B37	SKC	224-PCXR4	626256	07/04/2023	1,000	1,500	2,000	993	1,505	1,996	1.012x - 27.161	0.999
B38	SKC	224-PCXR4	626167	07/04/2023	1,000	1,500	2,000	998	1,493	1,997	1.003x - 8.615	1.000
B39	SKC	224-PCXR4	034637	10/04/2023	1,000	1,500	2,000	1,003	1,500	2,003	1.013x - 23.125	0.999
B40	SKC	224-PCXR4	798349	07/04/2023	1,000	1,500	2,000	993	1,507	1,998	1.015x - 30.204	0.999



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B41	SKC	224-PCXR4	612669	07/04/2023	1,000	1,500	2,000	997	1,496	1,991	0.998x - 1.396	1.000
B42	SKC	224-PCXR4	626041	10/04/2023	1,000	1,500	2,000	1,006	1,496	1,992	0.988x + 14.223	1.000
B43	SKC	224-PCXR4	034636	07/04/2023	1,000	1,500	2,000	1,001	1,503	1,993	0.992x + 8.810	1.000
B44	SKC	224-PCXR8	529341	10/04/2023	1,000	1,500	2,000	1,000	1,499	2,005	1.008x - 14.358	1.000
B45	SKC	224-PCXR8	529594	10/04/2023	1,000	1,500	2,000	998	1,506	1,987	0.990x + 12.580	1.000
B46	SKC	224-PCXR8	566743	05/04/2023	1,000	1,500	2,000	996	1,502	2,000	1.012x - 26.902	0.999
B47	SKC	224-PCXR8	566747	07/04/2023	1,000	1,500	2,000	998	1,501	2,002	1.014x - 27.552	0.999
B48	SKC	224-PCXR8	566753	10/04/2023	1,000	1,500	2,000	998	1,493	1,996	0.997x - 0.359	1.000
B49	SKC	224-PCXR8	566780	05/04/2023	1,000	1,500	2,000	1,007	1,501	2,007	1.011x - 19.156	0.999
B50	SKC	224-PCXR8	500400	07/04/2023	1,000	1,500	2,000	1,004	1,495	2,004	1.000x - 1.663	1.000
B51	SKC	224-PCXR8	500363	04/04/2023	1,000	1,500	2,000	997	1,502	1,998	1.008x - 21.322	0.999
B52	SKC	224-PCXR8	093186	05/04/2023	1,000	1,500	2,000	993	1,493	1,995	1.000x - 6.106	1.000
B53	SKC	224-PCXR8	707670	05/04/2023	1,000	1,500	2,000	1,000	1,498	2,002	1.009x - 18.883	0.999
B54	SKC	224-PCXR3	509821	05/04/2023	1,000	1,500	2,000	995	1,500	2,001	1.016x - 32.482	0.999
B55	SKC	224-PCXR3	510710	10/04/2023	1,000	1,500	2,000	998	1,497	1,992	0.996x - 0.191	1.000
B56	SKC	224-PCXR3	511450	05/04/2023	1,000	1,500	2,000	1,003	1,501	2,003	1.005x - 8.081	1.000
B57	SKC	224-PCXR3	510798	05/04/2023	1,000	1,500	2,000	999	1,490	2,000	1.001x - 2.920	1.000
B58	SKC	224-PCXR3	509852	10/04/2023	1,000	1,500	2,000	1,002	1,496	1,998	1.004x - 15.922	0.999
B59	SKC	224-PCXR3	509862	10/04/2023	1,000	1,500	2,000	998	1,501	1,996	0.996x + 4.471	1.000
B60	SKC	224-PCXR3	512655	07/04/2023	1,000	1,500	2,000	1,003	1,499	2,004	1.005x - 9.971	1.000
B61	SKC	224-PCXR3	503915	10/04/2023	1,000	1,500	2,000	993	1,488	1,999	1.007x - 15.934	1.000
B62	SKC	224-PCXR3	505975	10/04/2023	1,000	1,500	2,000	1,001	1,495	1,997	1.000x - 4.802	1.000
B63	SKC	224-PCXR3	511432	07/04/2023	1,000	1,500	2,000	993	1,500	2,000	1.015x - 32.709	0.999
B64	SKC	224-PCXR3	508302	05/04/2023	1,000	1,500	2,000	998	1,491	1,987	0.989x + 9.855	1.000
B65	SKC	224-PCXR3	508310	10/04/2023	1,000	1,500	2,000	998	1,502	2,005	1.012x - 20.596	1.000
B66	SKC	224-PCXR3	509861	10/04/2023	1,000	1,500	2,000	1,000	1,492	1,992	0.990x + 10.912	1.000
B67	SKC	224-PCXR3	506295	07/04/2023	1,000	1,500	2,000	993	1,506	2,002	1.007x - 13.999	1.000
B68	SKC	224-PCXR3	505872	05/04/2023	1,000	1,500	2,000	998	1,488	1,997	0.998x - 1.743	1.000
B69	SKC	224-PCXR3	508375	04/04/2023	1,000	1,500	2,000	1,004	1,502	2,002	1.009x - 18.897	0.999
B70	SKC	224-PCXR3	510623	05/04/2023	1,000	1,500	2,000	994	1,505	1,998	1.004x - 8.846	1.000
B71	SKC	224-PCXR3	508367	10/04/2023	1,000	1,500	2,000	994	1,503	2,003	1.011x - 23.544	0.999
B72	SKC	224-PCXR3	505977	10/04/2023	1,000	1,500	2,000	1,005	1,493	1,992	0.988x + 13.309	1.000
B73	SKC	224-PCXR3	512606	05/04/2023	1,000	1,500	2,000	1,000	1,504	2,004	1.008x - 14.506	1.000
B74	SKC	224-PCXR3	505993	05/04/2023	1,000	1,500	2,000	997	1,497	1,996	1.001x - 7.514	1.000
B75	SKC	224-PCXR3	509820	07/04/2023	1,000	1,500	2,000	997	1,496	1,992	0.997x + 0.195	1.000
B76	SKC	224-PCXR3	509811	05/04/2023	1,000	1,500	2,000	995	1,498	1,999	1.004x - 11.212	1.000
B77	SKC	224-PCXR3	508301	10/04/2023	1,000	1,500	2,000	1,003	1,502	2,004	1.013x - 23.811	0.999
B78	SKC	224-PCXR3	510677	04/04/2023	1,000	1,500	2,000	997	1,505	2,000	1.007x - 16.113	0.999
B79	SKC	224-PCXR3	510920	10/04/2023	1,000	1,500	2,000	996	1,495	1,993	0.998x - 1.232	1.000



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R²
H-R01	Dwyer	VFB-65	05/04/2023	500	1,000	2,000	502.1	993.6	1981.1	1.000x – 3.647	0.999
H-R02	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	500.4	998.7	1988.7	1.001x – 3.457	1.000
H-R03	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	502.1	990.3	1997.7	0.993x + 4.022	1.000
H-R04	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	497.2	992.2	2016.9	1.007x – 11.203	1.000
H-R05	Dwyer	VFB-65	05/04/2023	500	1,000	2,000	499.2	988.5	1990.7	1.003x – 7.136	1.000
H-R06	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	504.8	994.6	1982.6	0.999x – 1.961	0.999



CERTIFICATE No : 23M2441
REFERENCE No : 68471-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA 05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY : 

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23



CERTIFICATE No : 23M2441

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23° C \pm 1° C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA. THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : SP22018

Pages 1 of 3

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY

Condition As Found : GOOD

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON, CHATUCHAK,
BANGKOK 10900, THAILAND.

Location : ORGANIC LABORATORY IV


Ambient Temperature : (24.4 ± 5) °C
Relative Humidity : (60.1 ± 25) %

Received Date : 30 AUGUST 2022
Calibration Date : 30 AUGUST 2022
Date of Issue : 31 AUGUST 2022

Calibrated by :

Nathakorn Pisutpaisan

Approved by :

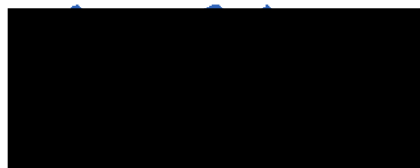

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : SP22018

Job No. : VC65SP0008

Pages : 2 of 3

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01,ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

<u>Material</u>	<u>Ref. type</u>	<u>Cell serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Holmium liquid	RM-HL	29706	87569	13/10/2022
Didymium liquid	RM-DL	28912	87588	15/10/2022
Neutral density filter	RM-1N2N3N	13877	87600	15/10/2022
Potassium dichromate solutions	RM-0204060810	14204	87614	16/10/2022
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology,NIST.

Result of calibration : Wavelength Accuracy

(Without adjustment)

<u>Material</u>	<u>Certified Values of Reference Material (nm)</u>	<u>UUC* Reading (nm)</u>	<u>Error (nm)</u>	<u>Uncertainty ± (nm)</u>	<u>k Factor</u>
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.4	0.15	0.16	2.00
	467.82	467.8	-0.02	0.16	2.00
	536.56	536.5	-0.06	0.16	2.00
	640.50	640.5	0.00	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.2	0.26	0.16	2.00

UUC* = Unit Under Calibration

Continuation of Calibration Certificate

Cert. No. : SP22018
Job No. : VC65SP0008
Pages : 3 of 3

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Filter: S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0524	1.0539	0.0015	0.0028	2.00
		29914	0.7	0.7454	0.7459	0.0005	0.0029	2.00
		29381	0.5	0.5426	0.5426	0.0000	0.0028	2.00
	546.1	29360	1.0	0.9822	0.9810	-0.0012	0.0028	2.00
		29914	0.7	0.6962	0.6960	-0.0002	0.0028	2.00
		29381	0.5	0.5076	0.5070	-0.0006	0.0029	2.00
	590.0	29360	1.0	1.0221	1.0202	-0.0019	0.0028	2.00
		29914	0.7	0.7238	0.7230	-0.0008	0.0029	2.00
		29381	0.5	0.5364	0.5360	-0.0004	0.0031	2.00
	635.0	29360	1.0	0.9751	0.9732	-0.0019	0.0028	2.00
		29914	0.7	0.6912	0.6902	-0.0010	0.0029	2.00
		29381	0.5	0.5214	0.5210	-0.0004	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2436	0.2419	-0.0017	0.0101	2.00	
		40	0.4905	0.4855	-0.0050	0.0115	2.00	
		60	0.7453	0.7388	-0.0065	0.0067	2.00	
		80	0.9920	0.9839	-0.0081	0.0071	2.00	
		100	1.2487	1.2414	-0.0073	0.0073	2.00	

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230

Resolution of Wavelength Mode 0.1 nm
Resolution of Photometric Mode 0.0001 A
Parameter Setting
Measurement Mode Wavelength, Absorbance
Wavelength Scan 1100 nm-190 nm
Scanning Speed 7.5 nm/min
Data Pitch 0.1 nm
Band width(Wavelength) 1.0 nm
Band width(Vis) 1.0 nm
Band width(Uv) 1.0 nm

Stray Light** UUC* Reading at 220 nm	
Transmission T(%)	Absorbance(A)
0.0107	3.9886

**Specific Acceptance :

Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A

**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Calibration Report

Non-Dispersive Infrared CO Analyzer

Date : 04 May 2023 Brand : API Model : 300E
No. CO-R01 Serial No. 704

Calibrator (Dilution System)

Brand : API Model : 700
Last Cal. Date : 06 September 2022 Serial No. : 421

Reference Standard Gas

Standard Gas : Carbon Monoxide (CO) Cylinder No. : D196045
Certified Date : 16 April 2022 Expired Date : 15 April 2024 Cylinder Conc. : 4,570 ppm

Calibrating Condition

Pressure 1011 mmbar Temp. 24.6 °C % RH 50

Calibration Setting

Span Set Point	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response
Zero	0	0.10	-	0
CO Span	40.00	40.11	0.275	40.00

API Model 300E CO Analyzer Check List

Parameter	Observed Value	Units	Nominal Range
Range	50	PPM	0-1000 ppm
Stability	0.10	PPM	< 1 ppm With Zero Air
CO Measure	4013.9	mV	2500-4800 mV
CO Reference	3947.7	mV	2500-4800 mV
Measure/Reference Ratio	1.179	-	1.1-1.3 W/Zero Air
Sample Pressure	28.7	In-Hg-A	~2" < Ambient Absolute Pressure
Sample Flow	805	CC/Min	800 ± 10%
Sample Temperature	48.3	°C	48 ± 4
Bench Temperature	48.0	°C	48 ± 2
Wheel Temperature	68.2	°C	68 ± 2
Box Temperature	30.6	°C	Ambient Temp + 7 ± 10
Photo-Drive	3038.9	mV	250 mV to 4750 mV
Slope	1.017	-	1.0 ± 0.3
Offset	0.2	-	0 ± 0.3



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaitachak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	04 May 2023	Brand :	API	Model :	300E
No.	CO-R02			Serial No.	171-S
Calibrator (Dilution System)					
Brand : API			Model : 700		
Last Cal. Date : 06 September 2022			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D196045		
Certified Date : 18 April 2022		Expired Date : 15 April 2024		Cylinder Conc. : 4,570 ppm	
Calibrating Condition					
Pressure : 1011 mmbar		Temp. : 24.6 °C		% RH : 50	
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	0.11	-	0	
CO Span	40.00	40.09	0.225	40.00	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4016.1	mV	2500-4800 mV		
CO Reference	3948.8	mV	2500-4800 mV		
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.6	In-Hg-A	~2" < Ambient Absolute Pressure		
Sample Flow	814	CC/Min	800 ± 10%		
Sample Temperature	48.3	°C	48 ± 4		
Bench Temperature	48.1	°C	48 ± 2		
Wheel Temperature	68.4	°C	68 ± 2		
Box Temperature	30.8	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3034.5	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		



WO-01981290/2023

MAINTENANCE AND TEST CERTIFICATE MODEL
OPTIMA 5300DV

Customer : S.P.S.Consulting Service Co.,Ltd **Date Tested:** January 11, 2023
Address : 7 Soi Phaholyothin 24 **Recommendation Recertification**
Paholyothin Road **Period** 6 **Months**
Jompol Chatuchak, Bangkok 1090 **Recertification Due:** July 11, 2023
User Name: K.Phenpha Vipasthawatt **Date Last Certified:** July 11, 2022
Phone: 083-9269252 **Visit Number:** 2 of 2
Fax: 02-513-4221 **PerkinElmer Phone:** 02-719-6420 ext 206
PerkinElmer Fax: 02-318-5597

CONFIGURATION TESTED

MODEL
OPTIMA 5300DV

SERIAL NUMBER
077C7042401

TESTED EQUIPMENT

IPV Methods

TEST STANDARD USED

Multielement Standard

Wavecal Solution

VIS Wavecal solution

Instrument Cal. STD4

CUSTOMER SUPPLIED

2 % HNO3

10 % HNO3

**ACCESSORIES/COMPONENT
NOT INCLUDED**

EXPIRATION

EXPIRATION DATE

May 30, 2023

February 28, 2023

August 30, 2023

November 30, 2023

CUSTOMER INITIALS



WO-01981290/2023

MAINTENANCE AND TEST CERTIFICATE MODEL
OPTIMA 5300DV

SERIAL NUMBER 077C7042401 **DATE TESTED** January 11, 2023

1. MECHANICAL CHECKS

A. Inspect and clean all fans and filters.

☐ OK

B. Inspect and replace as necessary, all torch components including the RF coil.

☐ OK

C. Inspect all tubing for sign of clacking or leaking.

☐ OK

D. Adjust water and gas pressure regulator settings.

☐ OK

E. Inspect and leak check pneumatics drawers.

☐ OK

F. Clean the exterior of the instrument.

☐ OK

2. OPTICAL CHECKS

A. Inspect and clean all optical components.

☐ OK

B. As required, check and replace all purgefilters.

☐ OK

C. Recheck optical alignment.

☐ OK

3. COOLING SYSTEM CHECKS

A. Perform preventive maintenance on chiller.

☐ OK

B. Flush out the chiller every year.

☐ N/A

4. PERFORMANCE CHECKS

A. Torch View Alignment.

☐ OK

B. Wavelength Calibration.

☐ OK



MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV


SERIAL NUMBER : 077C7042401		DATE TESTED : January 11, 2023	
PARAMETER	SPECIFICATION	FINAL VALUE	
Spectral Resolution : UV	As 193.696 nm	≤ 0.007	0.00504
	Ni 231.604 nm	≤ 0.008	0.00646
	Ni 341.476 nm	≤ 0.012	0.00768
Spectral Resolution : VIS	La 408.672 nm	≤ 0.020	0.01597
	Ba 455.403 nm	≤ 0.025	0.02185
Precision	As 193.656 nm	% RSD < 1.0	0.89 %
	Zn 213.856 nm	% RSD < 1.0	0.77 %
	Mn 257.610 nm	% RSD < 1.0	0.51 %
	La 379.478 nm	% RSD < 1.0	0.44 %
	Ba 455.403 nm	% RSD < 1.0	0.44 %
	Ba 493.408 nm	% RSD < 1.0	0.46 %
Detection Limits : Axial	Ti 190.080 nm	3(sd)	4.04 ppb
	As 193.696 nm	3(sd)	3.58 ppb
	Pb 220.353 nm	3(sd)	1.90 ppb
Detection Limits : Radial	As 193.696 nm	3(sd)	47.72 ppb
	Zn 213.856 nm	3(sd)	1.02 ppb
	Mn 257.610 nm	3(sd)	0.68 ppb
	La 379.478 nm	3(sd)	1.43 ppb
	Ba 455.403 nm	3(sd)	0.10 ppb
	Ba 493.408 nm	3(sd)	0.36 ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd 226.502 nm	≤ 150 ppb	58.36
BEC : Radial (IB X 1000)/(IS-IB)	Mn 257.610 nm	≤ 45 ppb	104142.80



MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV

SERIAL NUMBER	077C7042401	DATE TESTED	January 11, 2023
Remarks :			
Commissioning follow as commissioning performance sheets.			
This is to certify that the above tests have been performed and the configuration tested			
<input checked="" type="checkbox"/> meets			
<input type="checkbox"/> does not meet			
the PerkinElmer Specifications listed on this certificate.			
This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranties.			
<div style="background-color: black; width: 100%; height: 100px; position: relative;"> <div style="position: absolute; top: 0; right: 0; bottom: 0; left: 0; display: flex; align-items: center; justify-content: center;"> <div style="width: 100%; height: 100%; background-color: black;"></div> </div> </div>			
Authorized Representative: _____			
Service Engineer			

PinAAcle 900T Preventive Maintenance (PM)			
Company Name:	SPS CONSULTING SERVICE CO.,LTD.		
Address (Instrument Location):	7 SOI PHAHOLYOTHIN 24,PHAHOLYOTHIN RD. JOMPOL,CHATUCHAK, BANGKOK 10110		
Serial Number:	PTCS14111103	PM Number:	1-2
Customer Name (if applicable):	K. PHENPHA	Telephone Number:	083-926-9252
Customer Support Engineer Name:	K. DUANG	Service Order Number:	WO-02044564
Date PM Performed: (DD-MMM-YYYY)	06-Jan-2023	Next PM Due Date: (DD-MMM-YYYY)	06-Jul-2023
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	
09370143 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900T by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes
AS900	AS9S14B1002	WINLAB 32

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	2
B3002013	THGA Contact Cylinders	1
B3141064	Glycerol for THGA Cooling	N/A
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	2
N9301714	Replacement Acetylene Filter Cartridge	1
TH001022	Replacement Air Filter Cartridge	2

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	26-87CUY1	30-Jan-2024
N9300244	GFAAS Mixed Standard	AR	56-021CRY1	30-Jun-2023

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 ml.	AR	AR
N/A	0.5% HNO ₃	250 ml.	AR	AR

Additional Tools Required for PM			
Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	MG0-252
N1013002	1.0A Neutral density filter	1	MG2-358
B3100652 Or N9307029	Electronic Flow Meter	1	NA
B0505495	Test Jig	1	NA
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	092216-010130
N3050109	Ba Lumina HCL	1	102416-040160
N3050139	K Lumina HCL	1	110716-010060
N3050152	Ni Lumina HCL	1	100516-030190
N3050119	Cr Lumina HCL	1	091911-020150

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Perform general inspection of system for cleanliness.

2. PC Instrument Software:

- ☒ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. Mechanical:

- ☒ Inspect and clean all fans and filters. Replace filters if necessary
- ☒ Inspect all gas and water lines for leaks and/or wear. Replace if needed. Thoroughly inspect all quick connects. Replace the Y connector, P/N 09921079, if needed.
- ☒ Clean exterior of the instrument.

3.1 Flame Technique

- ☒ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ☒ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
- ☒ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ☒ Check the drain system for signs of wear. Replace worn or damaged parts.
- ☒ Visually check for proper flame conditions when igniting the Air-C2H2 and N2O-C2H2 flames (if applicable).

3.2 THGA Technique

- ☒ Inspect the pole pieces and clean where the pole pieces contact the furnace. Replace the pole piece p-rings as needed, P/N's B0501018 & B0501250. Grease the O-rings as needed with Apiezon L grease, P/N 09905148
- ☒ Inspect the four insulation pads on the front contact housing of the THGA in furnace. If the pads are missing replace the THGA furnace or replace the insulator pads on the furnace.
- ☒ Inspect the graphite tube and clean the contact cylinders. Replace if necessary.
- ☒ Check internal and external gas flows with the Electronic Gas Flow Meter and the Gas Flow Test Probe as described in the Service Manual. Correct if necessary.
- ☒ Check furnace open/close function.
- ☒ Verify the operation of the GFTV Camera for proper operation and viewing alignment in the furnace camera Tube View window. Align if needed.
- ☒ Check the operation of the Halogen Light ASSY for the GFTV Camera. Replace if needed.
- ☒ Check the water level/quality in the recirculation (if applicable). Add distilled water if necessary.
- ☒ Check the cooling system fluid flow rate with the FCS In-Line Flow Meter for proper levels if needed. Refer to SDB# COSY008.STN

- ✓ Perform Cooling System maintenance if needed per SDB# COSY005.STN.
- ✓ Check auto sampler operation.
- ✓ Perform an auto sampler check valve test as described in the Service Manual.
- ✓ Lubricate the spindles of the auto sampler pumps and all moving parts of the tray mechanics as described in the Service Manual.
- ✓ Inspect the auto sampler sampling capillary as described in the Service Manual. Replace if necessary.

4. Electrical:

- ✓ Inspect PC boards. Clean if necessary.
- ✓ Carefully check all internal and external cable connections.
- ✓ Check instrument firmware revisions upgrade to current levels (if necessary)
- ✓ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

5. Optics:

- ✓ Inspect and clean the sample compartment windows, if needed.
- ✓ Inspect and clean the furnace windows, if needed.
- ✓ Inspect and clean the GFTV camera lens, if needed.
- ✓ Inspect optics. Clean or replace if necessary,

6. Gasses:

- ✓ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ✓ Verify that the air filter element is dry. Replace if necessary.

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests [Flame]:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	0.9798	0.1982	Passed
0.2 A ND Filter	± 5% from Cert.	0.2042	0.9942	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0014	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed

8.4 D₂ Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0083	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0002	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0021	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	NA	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	0.3281	Passed

9. After PM Performance tests [THGA]:

9.1 Furnace Gas Flows

Description: Ensures the flow rates are within specification.

Parameter	Specification	Test Results	Pass/Fail
Internal Flow Rate	250 mL/min \pm 25 mL/min	255	Passed
External Flow Rate	100 mL/min \pm 10 mL/min	105	Passed

9.2 Chromium Baseline Noise

Description: Signal to noise check.

Parameter	Specification	Results	Pass/Fail
Baseline Noise	≤ 0.005 Abs.	0.0000	Passed
Standard Deviation	≤ 0.005	0.0002	Passed

9.3 Chromium Characteristic Mass and Precision

Description: Calculate the characteristic mass using the characteristic mass tool and precision from the integrated absorbance values.

Parameter	Specification	Results	Pass/Fail
Cr m_0 Results	≤ 7.0 pg/0.0044 A-s	5.7	Passed
Precision	≤ 2.0 %	0.74	Passed

9.4 Copper Characteristic Mass and Zeeman Ratio

Description: Calculate the characteristic mass using the characteristic mass tool and check the Zeeman Ratio.

Parameter	Specification	Results	Pass/Fail
Cu m_0 Result	≤ 16.5 pg/0.0044 A-s	12.3	Passed
Zeeman Ratio	0.52 ± 0.04	0.54	Passed


10. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

Additional Comments

Additional Comments Regarding the PM	
Zeeman Ratio	$= \frac{\text{Atomic Signal (Peak area)}}{\text{Atomic Signal (Peak area)} + \text{Background Signal (Peak area)}}$ $= \frac{0.1855}{0.1855 + 0.1563}$ $= 0.54$
REPLACE PM KIT	

Review

<i>The preventive maintenance checks and if applicable performance tests for PinAAcle 900T have been completed.</i>		
This PinAAcle 900T Passes <input checked="" type="checkbox"/> Fails <input type="checkbox"/> the preventive maintenance.		
Review of Preventive Maintenance:		
Authorized PerkinElmer Representative:		Date: 06-Jan-2023 (DD-MMM-YYYY)
Authorized Customer Representative:		Date: 06-Jan-2023 (DD-MMM-YYYY)

Certificate of System Qualification

GC-OQ - GCMS-OQ

System ID: GC_MS_03_52_CN10925102
Organization Name: S.P.S Consulting service
Organization Location: 7 Sol Pheholyothin Road, Ledyao, Khet Jetyak, Bangkok 10900

Date: March 31, 2023 1:21:52 PM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.50, GCMS.02.50
Overall Qualification Status: Pass

System Inspection and Basic Safety and Operation

Name: 7890
Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Decay

Name: 7890
Front SSL
Setpoint Status: Pass
Pressure: 25.0 psi
Pressure Change: -0.1 psi /5 minutes
Agilent Recommended: ≥ -2.0 and ≤ 0.5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 7890
Front SSL

Date: March 31, 2023 1:21:52 PM
System ID: GC_MS_03_52_CN10925102

Setpoint Status: Pass
Inlet Pressure: Setpoint 25.0 psi Actual 25.0 psi
Accuracy: 0.0 psi
Agilent Recommended: ≤ 1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Inlet Pressure Accuracy

Name: 7890
Back SSL
Setpoint Status: Pass
Inlet Pressure: Setpoint 25.0 psi Actual 25.2 psi
Accuracy: 0.2 psi
Agilent Recommended: ≤ 1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Detector Flow Accuracy

Name: 7890
Front FID
Setpoint Status: Pass
Flow Type: Fuel
Setpoint 30.0 mL/min Measured Flow: 30.3 mL/min
Accuracy: 0.3 mL/min
Agilent Recommended: ≤ 10.0 % setpoint (3.0 mL/min)
Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Date: March 31, 2023 1:21:52 PM
System ID: GC_MS_03_52_CN10925102

Setpoint Status: Pass

Flow Type: Oxidizer

Setpoint: 400.0 mL/min **Measured Flow:** 396.2 mL/min

Accuracy: 3.8 mL/min

Agilent Recommended: ≤ 10.0 % setpoint (40.0 mL/min)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Setpoint Status: Pass

Flow Type: Makeup

Setpoint: 25.0 mL/min **Measured Flow:** 25.1 mL/min

Accuracy: 0.1 mL/min

Agilent Recommended: ≤ 10.0 % setpoint (2.5 mL/min)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name: 7890

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual:

Temperature:	230.0	230.6	°C
--------------	-------	-------	----

Accuracy: 0.6 °C

Agilent Recommended: ≥ -1.0 % setpoint in K (-5.0 °C)
≤ 1.0 % setpoint in K (5.0 °C)

Date: March 31, 2023 1:21:52 PM
System ID: GC_MS_03_52_CN10926102

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual:

Temperature:	100.0	100.4	°C
--------------	-------	-------	----

Accuracy: 0.4 °C

Agilent Recommended: ≥ -1.0 % setpoint in K (-3.7 °C)
≤ 1.0 % setpoint in K (3.7 °C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name: 7890

Setpoint Status: Pass

Setpoint/Average:

Temperature:	100.0	100.3633	°C
--------------	-------	----------	----

Stability: 0.1 °C

Agilent Recommended: ≤ 0.5

Overall GC Oven Temperature Stability Test Status

Pass

Scouting Run

Tested Combination1	Front	SSL	/ Front	FID
	Manual Injection			
Name:	Not applicable			
Setpoint Status:	Completed			
Injection Volume on Column:	1.0 µL			

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination1	Front	SSL	/ Front	FID
---------------------	-------	-----	---------	-----

Date: March 31, 2023 1:21:52 PM
System ID: GC_MS_03_52_CN10926102

Name: 7890

Setpoint Status: Pass

Base Signal: 89800 /Ab

ASTM Noise counts	Drift counts/Hr
285.31	96.04
768.00	19200.00

Agilent Recommended: \leq

Status: Pass Pass

Overall Noise and Drift Test Status

Pass

Signal to Noise

Tested Combination1 Front SSL / Front FID

Name: Manual Injection 7890

Setpoint Status: Pass

Signal to Noise: 3814254

Agilent Recommended: \geq 300000

Overall Signal to Noise Test Status

Pass

Log Amp

Tested Combination2 Back SSL / External SQ

Name: 5975C

Setpoint Status: Pass

Overall Log Amp Test Status

Pass

RFPA

Date: March 31, 2023 1:21:52 PM
System ID: GC_MS_03_52_CN10925102

Tested Combination2 Back SSL / External SQ

Name: 5975C

Setpoint Status: Pass

Amu: 1050 m/z Drift After Five Minutes: 1 mV RFPA Voltage: 479 mV

Agilent Recommended: \geq -100 and \leq -100 \leq 1100

Overall RFPA Test Status

Pass

Tune EI

Tested Combination2 Back SSL / External SQ

Name: 5975C

Setpoint Status: Pass

Filament: 1

Setpoint Status: Pass

Filament: 2

Overall Tune EI Test Status

Pass

Signal to Noise EI

Tested Combination2 Back SSL / External SQ

Name: 5975C

Source: EI - Inert Filament: 1

Setpoint Status: Pass

Signal to Noise: 425

Agilent Recommended: \geq 180

Date: March 31, 2023 1:21:52 PM
System ID: GC_MS_03_52_CN10925102

Source:	El - Inert	Filament:	2
Setpoint Status:	Pass		
Signal to Noise:	566		
Agilent Recommended:	>= 160		
Overall Signal to Noise EI Test Status	Pass		

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GC_MS_03_52_CN10925102
Manufacturer	Agilent Technologies
Name	7890

Tested Combination1

Injection Technique	Manual Injection
Sampler Identifier	Sampler 1
Inlet	Front
Detector	Front
LTM Included?	No

Tested Combination2

Injection Technique	Manual Injection
Sampler Identifier	Sampler 2
Inlet	Back
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN10925102
Firmware Revision	A.01.10.3
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Date: March 31, 2023 1:21:52 PM
System ID: GC_MS_03_52_CN10925102

Detector 2

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5975C
Serial Number	US91732743
Firmware Revision	5975 5.02.07
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Inert
Number of filaments	2

Date: March 31, 2023 1:21:52 PM
System ID: GC_MS_03_52_CN10925102

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and login to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer: Saenguthai Tarak
Logged On User Name: saenguthai.tarak@non.agilent.com
Signature Creation Date: March 31, 2023
Reason for Signature: Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configurations and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties of merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: saenguthai.tarak
Host Name: LAPTOP-CQ39KQMY

System ID: GC_MS_03_52_CN10925102
Print Date: March 31, 2023 1:21:03 PM

GC_MS_03_52_CN10925102 Transaction log

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 31, 2023 9:12:28 AM Audit		Session Created	Session	None
March 31, 2023 9:12:28 AM Start		Configuration	Session	None
March 31, 2023 9:12:28 AM Audit		Exit/Logout	Licensing	User is Not playing and does not require an unlock code
March 31, 2023 9:27:14 AM Audit		Execution	Session	EQP details for primary technique (GC) - File path: [ProtocolPacks\GC\Configurations\07_52\GC_02_50.eqp], EQP File Name: [GC_02_50.eqp], EQP Name: [AgilentRecommended], Protocol Revisor: [GC_02_90], EQP details for synthesized technique (GC/MS) - File path: [ProtocolPacks\GC\MS\Configurations\02_52\GC/MS_02_50.eqp], EQP File Name: [GC/MS_02_50.eqp], EQP Name: [AgilentRecommended]
March 31, 2023 9:20:17 AM End		Configuration	Session	None
March 31, 2023 9:20:27 AM Start		Configuration	Session	QC
March 31, 2023 9:20:27 AM Run		Execution	System Inspection and Basic Safety and Operation - 7890 - Qualitative Test - No reports associated	None
March 31, 2023 9:27:33 AM End		Execution	System Inspection and Basic Safety and Operation - 7890 - Qualitative Test - No reports associated	Run Count: 1

User Name: saenguthai.sarak
 Hostname: LAPTOP-CQ3SKOMV
 System ID: GC_MS_03_52_CN10925102
 Print Date: March 31, 2023 1:21:53 PM

GC_MS_03_52_CN10925102 Transaction Log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 31, 2023 9:21:35 AM Start	Execution	Inlet Pressure Decay - Front	None	SSL - Pressure Controlled Inlet - S: 25.0 psi - L: >= 2.0 psi and - <= 0.5 psi
March 31, 2023 9:21:51 AM End	Execution	Inlet Pressure Decay - Front	Run Count: 1	SSL - Pressure Controlled Inlet - S: 20.0 psi - L: >= 2.0 psi and - <= 0.5 psi
March 31, 2023 9:21:54 AM Start	Execution	Inlet Pressure Accuracy - Front	None	SSL - Pressure Controlled Inlet - S: 20.0 psi - L: <= 1.2 psi
March 31, 2023 9:21:59 AM End	Execution	Inlet Pressure Accuracy - Front	Run Count: 1	SSL - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi
March 31, 2023 9:22:02 AM Start	Execution	Inlet Pressure Accuracy - Back	None	SSL - Pressure Controlled Inlet - S: 20.0 psi - L: <= 1.2 psi
March 31, 2023 9:22:07 AM End	Execution	Inlet Pressure Accuracy - Back	Run Count: 1	SSL - Pressure Controlled Inlet - S: 20.0 psi - L: <= 1.2 psi
March 31, 2023 9:22:39 AM Start	Execution	Detector Flow Accuracy - Front	None	FID - Type: Fuel - S: 33.0 mL/min - L: <= 10.0% setpoint
March 31, 2023 9:22:29 AM End	Execution	Detector Flow Accuracy - Front	Run Count: 1	FID - Type: Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint
March 31, 2023 9:22:36 AM Start	Execution	Detector Flow Accuracy - Front	None	FID - Type: Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint
March 31, 2023 9:22:41 AM End	Execution	Detector Flow Accuracy - Front	Run Count: 1	FID - Type: Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint

Page 2 / 6

Date: March 31, 2023 1:21:52 PM
 System ID: GC_MS_03_52_CN10925102

Page 13 / 19

User Name: saenguthai.sarak
 Hostname: LAPTOP-CQ3SKOMV
 System ID: GC_MS_03_52_CN10925102
 Print Date: March 31, 2023 1:21:53 PM

GC_MS_03_52_CN10925102 Transaction Log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 31, 2023 9:22:42 AM Start	Execution	Detector Flow Accuracy - Front	None	FID - Type: Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint
March 31, 2023 9:22:48 AM End	Execution	Detector Flow Accuracy - Front	Run Count: 1	FID - Type: Makeup - S: 20.0 mL/min - L: <= 10.0% setpoint
March 31, 2023 9:22:45 AM Start	Execution	GC Oven Temperature	None	Accuracy: 7890 - Temperature Oven - S: 230.0°C - L: >= 1.0 AND <= 1.0% setpoint in K
March 31, 2023 9:23:01 AM Audit	Data	GC Oven Temperature	Manual Data Entry	Accuracy: 7890 - Temperature Oven - S: 230.0°C - L: >= 1.0 AND <= 1.0% setpoint in K
March 31, 2023 9:23:04 AM End	Execution	GC Oven Temperature	Run Count: 1	Accuracy: 7890 - Temperature Oven - S: 230.0°C - L: >= 1.0 AND <= 1.0% setpoint in K
March 31, 2023 9:23:37 AM Start	Execution	GC Oven Temperature	None	Accuracy: 7890 - Temperature Oven - S: 100.0°C - L: >= 1.0 AND <= 1.0% setpoint in K
March 31, 2023 9:28:03 AM Audit	Data	GC Oven Temperature	Manual Data Entry	Accuracy: 7890 - Temperature Oven - S: 100.0°C - L: >= 1.0 AND <= 1.0% setpoint in K
March 31, 2023 9:28:03 AM End	Execution	GC Oven Temperature	Run Count: 1	Accuracy: 7890 - Temperature Oven - S: 100.0°C - L: >= 1.0 AND <= 1.0% setpoint in K
March 31, 2023 9:28:05 AM Start	Execution	GC Oven Temperature Stability	None	- 7890 - Temperature - Oven - S: 100.0°C - L: <= 0.5°C

Page 3 / 6

Date: March 31, 2023 1:21:52 PM
 System ID: GC_MS_03_52_CN10925102

Page 14 / 19

User Name: saengutthakarnak
Host Name: LAPTOP-DQ3SKORV

System ID: GC_MS_03_52_CN10925102
Print Date: March 31, 2023 1:21:53 PM

GC_MS_03_52_CN10925102 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 31, 2023 9:28:42 AM Start	Execution	GC Oven Temperature Stability	None	- 7890 - Temperature - Oven - S: 190.0°C - L: <= 0.5°C
March 31, 2023 9:27:35 AM Audit	Data	GC Oven Temperature Stability	Manual Data Entry	- 7890 - Temperature - Oven - S: 100.0°C - L: <= 0.5°C
March 31, 2023 9:27:46 AM End	Execution	GC Oven Temperature Stability	Run Count: 1	- 7890 - Temperature - Oven - S: 190.0°C - L: <= 0.5°C
March 31, 2023 9:27:51 AM Start	Execution	GC Scouting Run - Manual Injection, Front SSL, Front FID	None	- Part of System Preparation - No limits associated
March 31, 2023 9:54:35 AM Start	Execution	Log Amp - 5975C SQ - Source: None	None	El - inert
March 31, 2023 9:55:05 AM Start	Execution	HPFA - 5975C SQ - Source: El	None	None
March 31, 2023 10:23:19 AM	Start	Signal to Noise - Manual Injection, Back SSL, SQ - Source: El - Inert Gas	None	Fillament 1 (Qualitative) - No setpoints associated
March 31, 2023 10:37:54 AM	Start	Line El - 5975C SQ - Source: None	None	El - Inert Gas - 1 (Qualitative) - No setpoints associated
March 31, 2023 10:38:04 AM	Start	Line El - 5975C SQ - Source: None	None	El - Inert Gas - 2 (Qualitative) - No setpoints associated
March 31, 2023 10:38:11 AM	Start	Line El - 5975C SQ - Source: None	None	El - Inert Gas - 1 (Qualitative) - No setpoints associated

Page 4 / 8

Date: March 31, 2023 1:21:52 PM
System ID: GC_MS_03_52_CN10925102

Page 15 / 19

User Name: saengutthakarnak
Host Name: LAPTOP-DQ3SKORV

System ID: GC_MS_03_52_CN10925102
Print Date: March 31, 2023 1:21:53 PM

GC_MS_03_52_CN10925102 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 31, 2023 10:38:14 AM	Start	Noise and Drift - Front FID - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None	None
March 31, 2023 10:38:12 AM	Start	GC Scouting Run - Manual Injection, Front SSL, Front FID	None	- Part of System Preparation - No limits associated
March 31, 2023 10:46:28 AM	Audit	GC Scouting Run - Manual Injection, Front SSL, Front FID	Data Files Path:	F:\Data\GC_H1\J091014.cn
March 31, 2023 10:47:01 AM	End	GC Scouting Run - Manual Injection, Front SSL, Front FID	Run Count: 1	- Part of System Preparation - No limits associated
March 31, 2023 10:58:22 AM	Start	Noise and Drift - Front FID - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None	None
March 31, 2023 10:58:52 AM	Audit	Noise and Drift - Front FID - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data Files Path:	F:\Data\ND_FID\J091014.cn
March 31, 2023 11:02:53 AM	End	Noise and Drift - Front FID - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count: 1	None
March 31, 2023 11:02:02 AM	Start	Signal to Noise - Manual Injection, Front SSL, Front FID	None	- Detector FID - L: <= 360000
March 31, 2023 11:14:57 AM	Audit	Scouting	None	None

Page 5 / 8

Date: March 31, 2023 1:21:52 PM
System ID: GC_MS_03_52_CN10925102

Page 16 / 19

User Name: saanguthai.tarak
 Hostname: LAPTOP-4QJ39KDRV
 System ID: GC_MS_03_52_CN10925102
 Print Date: March 31, 2023 1:21:54 PM

GC_MS_03_52_CN10925102 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 31, 2023 11:15:13 AM	Audit	AccRestarted	Session	None
March 31, 2023 11:15:14 AM	Audit	SessionReloaded	Session	None
March 31, 2023 11:15:19 AM	Start	Qualification	Session	QQ
March 31, 2023 11:15:19 AM	Start	Execution	Signal to Noise - Manual Injection, Front SSL, Front FID, - Detector: FID - L: >= 300000	None
March 31, 2023 11:16:20 AM	Audit	AccClosed	Session	None
March 31, 2023 11:21:34 AM	Audit	AccRestarted	Session	None
March 31, 2023 11:21:04 AM	Audit	SessionReloaded	Session	None
March 31, 2023 11:21:09 AM	Start	Qualification	Session	QQ
March 31, 2023 11:21:09 AM	Start	Execution	Signal to Noise - Manual Injection, Front SSL, Front FID, - Detector: FID - L: >= 300000	None
March 31, 2023 11:22:15 AM	Audit	Data	Signal to Noise - Manual Injection, Front SSL, Front FID, - Detector: FID - L: >= 300000	Data File Path: F:\3N_51_01\DATA\SUMMARY
March 31, 2023 11:24:02 AM	End	Execution	Signal to Noise - Manual Injection, Front SSL, Front FID, - Detector: FID - L: >= 300000	Run Count: 1
March 31, 2023 11:24:17 AM	Start	Execution	Log Amp - 5575C SQ: - Source: None	El - Inert
March 31, 2023 11:24:31 AM	End	Execution	Log Amp - 5575C SQ: - Source: None	Run Count: 1

User Name: saanguthai.tarak
 Hostname: LAPTOP-4QJ39KDRV
 System ID: GC_MS_03_52_CN10925102
 Print Date: March 31, 2023 1:21:59 PM

GC_MS_03_52_CN10925102 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 31, 2023 11:24:39 AM	Start	Execution	RPPA - 5575C SQ: - Source: El - None	El - Inert
March 31, 2023 11:27:22 AM	End	Execution	RPPA - 5575C SQ: - Source: El - None	Run Count: 1
March 31, 2023 11:27:23 AM	Start	Execution	Tune El - 5575C SQ: - Source: None	El - Inert, Filament 1: Qualitative - No setpoints associated
March 31, 2023 11:28:04 AM	End	Execution	Tune El - 5575C SQ: - Source: None	Run Count: 1
March 31, 2023 11:28:09 AM	Start	Execution	Tune El - 5575C SQ: - Source: None	El - Inert, Filament 2: Qualitative - No setpoints associated
March 31, 2023 11:28:26 AM	End	Execution	Tune El - 5575C SQ: - Source: None	Run Count: 1
March 31, 2023 11:28:28 AM	Start	Execution	Signal to Noise El - Liquid Injection, Back SSL, SQ: - Source: El - Inert using Filament 1 - L: >= 180	None
March 31, 2023 11:29:45 PM	Start	Execution	Signal to Noise El - Liquid Injection, Back SSL, SQ: - Source: El - Inert using Filament 1 - L: >= 180	None
March 31, 2023 1:00:09 PM	Audit	Data	Signal to Noise El - Liquid Injection, Back SSL, SQ: - Source: El - Inert using Filament 1 - L: >= 180	Data File Path: F:\3N_51_01\DATA\SUMMARY
March 31, 2023 1:00:14 PM	End	Execution	Signal to Noise El - Liquid Injection, Back SSL, SQ: - Source: El - Inert using Filament 1 - L: >= 180	Run Count: 1

User Name: kshidig@hillsrak
 Machine: LAPIPP-CQ38K0VV

System ID: GC_MS_03_52_CN10925102
 Print Date: March 31, 2023 1:21:52 PM

GC_MS_03_52_CN10925102 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 31, 2023 1:00:43 PM Start	Execution		Signal to Noise EI - Liquid Injection, Back SSI, SIQ - Source: EI - Inlet using Filament 2 - L: >= 160	None
March 31, 2023 1:01:05 PM Audit	Data		Signal to Noise EI - Liquid Injection, Back SSI, SIQ - Source: EI - Inlet using Filament 2 - L: >= 160	Data File Path : F:\MS_F2_01.D\DATA\31M.M
March 31, 2023 1:02:09 PM End	Execution		Signal to Noise EI - Liquid Injection, Back SSI, SIQ - Source: EI - Inlet using Filament 2 - L: >= 160	Run Count: 1
March 31, 2023 1:02:13 PM End	Queue Action	Session	Session	CQ
March 31, 2023 1:04:13 PM Start	Reporting	Session	Session	None
March 31, 2023 1:20:27 PM Audit	Reporting	Session	Session	Report Generated : Certificate



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

GAS CHROMATOGRAPH TEST CERTIFICATION

Certificate No. : SV0822/20530

Instrument Type : GC

Model : CP-3800

Serial Number : 00734

Organization : S.P.S. Consulting Service Co., Ltd.

Address : 7 Phahonyothin Soi 24 Phahonyothin Rd. Ladyao Chatuchak Bangkok 10900

Date : 10/08/2022

ELECTRONIC TEST

CPU	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
LCD TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
VENT TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
KEY ECHO TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
DESTRUCTION RAM TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL

RUN CHROMATOGRAM TEST

DETECTOR : Flame Ionization Detector (FID Channel Front)

INJECTOR : Capillary Injector Model 1079

GC CONDITION:

Column	80 °C hold 1 min., rate 20 °C/min. to 200 °C hold 1min.
Injector	220 °C
Detector	300 °C
Column flow	5 mL/min
Makeup flow	25 mL/min
Air flow	300 mL/min
Hydrogen flow	30 mL/min

Column: Capillary Column CP sil 5 CB 0.25 ID x 15 M

Sample: 1 µL Injection FID Test Sample 0.218 g/L C14, C15, C16 in hexane

SENSITIVITY TEST: C15. (Area count) = 118,103 Counts.



VARIAN

1/2

SERVICE DEPARTMENT
FR-SV-029 Rev. 04



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Detector Sensitivity (FID)

Detector Response	Result	Specification
Baseline Noise (µV)	2.94	≤ 50
Baseline Drift (%)	0.18	≤ 1
Sensitivity (S/N for C15)	4,000	≥ 1,024

Temperature Specification

Temperature	Set	Result	Specification
Column Oven (° C)	80	80	± 5
Injector (° C)	220	220	± 5
Detector (° C)	300	300	± 5
Incubator (° C)	60	N/A	± 5

Relative Standard Deviation % (% RSD)

Checkout Procedure	Result	Specification
Area C15 (%)	1.68	≤ 5
Retention Time C15(%)	0.01	≤ 0.5

APPROVAL :

Signature:

Engineer :

Date : 10/08/2022



VARIAN

2/2

SERVICE DEPARTMENT
FR-SV-029 Rev. 04



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com


Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 Area 1	117,172
C15 Area 2	119,182
C15 Area 3	117,982
C15 Area 4	118,589
C15 Area 5	117,592
C15 Area Average	118,103
* % RSD (< 5 %)	1.68

* The precision specification should be less than 2.0 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the C15 peak area for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$



VARIAN

1/1

SERVICE DEPARTMENT



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com


Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 RT 1	4.048
C15 RT 2	4.048
C15 RT 3	4.048
C15 RT 4	4.048
C15 RT 5	4.048
C15 RT Average	4.000
* % RSD (< 0.5 %)	0.01

* The precision specification should be less than 0.5 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the RT C15 peak for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$



VARIAN

1/1

SERVICE DEPARTMENT



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
[THERMAL ENVIRONMENT MONITOR]
MANUFACTURER : 3M
MODEL / TYPE : QUESTemp[®]34
SERIAL NO. : TEN040005
CLID. NO. : 231802516
JOB CONTROL NO. : 220901088340

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 01 September 2022

DATE OF ISSUED : 07 September 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Tanawan Seenam-Ngoen

Calibrating Engineer



Approved By :

Authorized Signatory

07 September 2022

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22088340

F3-011-04/01-12

page 1 of 3



@ckcalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
[THERMAL ENVIRONMENT MONITOR]
MANUFACTURER : 3M
MODEL / TYPE : QUESTemp[®]34
SERIAL NO. : TEN040005
DATE OF CALIBRATION : 02 September 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. WI-305-74. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.

Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Thunder Scientific Corporation. Certificate No. 19944, Due Date 26 January 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22088340

F3-011-04/01-12

page 2 of 3



@ckcalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4 Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-573-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter [thermal environment monitor].

CALIBRATION DATA

1. CORRECTION OF TEMPERATURE : WET

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	30.0	+0.01	0.40
35.0	35.00	35.0	0.00	
40.0	40.02	40.0	+0.02	

2. CORRECTION OF TEMPERATURE : DRY

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	29.8	+0.21	0.40
35.0	35.00	34.8	+0.20	
40.0	40.02	39.8	+0.22	

3. CORRECTION OF TEMPERATURE : GLOBE BULB

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	30.0	+0.01	0.40
35.0	35.00	35.0	0.00	
40.0	40.02	40.0	+0.02	

Note: The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22088340

F3-011-04/01-12

page 3 of 3



METROLOGY SYSTEM (THAILAND) CO.,LTD.



Certificate of Calibration

Certificate Number : SPR23030505-5

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Metrosonics

Model : hs-32

Serial Number : MCD070035

ID. Number : R05

Environmental Conditions

Ambient Temperature : 23 °C ± 2 °C Received Date : 30 Mar 2023

Relative Humidity : 50 % ± 15 % Calibration Date : 31 Mar 2023

Location of Calibration : In-Lab Recommend Due Date : 31 Mar 2024

Calibration Procedure : SP-CPT-04-13 Date of Issue : 01 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full without written approval of SP Metrology System (Thailand) Co., Ltd.

Calibrated by :

Approved by :

Authorized Signatory

SP-FM-04-15 rev.0

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 68888 www.spsmetrology.com



Calibration Report

Certificate Number : SPR23030505-5

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR23010480-5	22 Feb 2024
THERMO-HYGROMETER	5020A	A47046	QR23-0176	26 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
 SP Metrology - SP Metrology system (Thailand) Co.Ltd.
 Quality Reborn Co., Ltd

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 ๕๙๓๖ www.spmetrology.com



Result of Calibration

Certificate No. : SPR23030505-5

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	29.9	-0.113	0.50
35.0	35.010	34.9	-0.110	0.50
40.0	40.015	39.9	-0.115	0.50

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	29.9	-0.113	0.50
35.0	35.010	34.9	-0.110	0.50
40.0	40.015	39.9	-0.115	0.50

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	29.8	-0.213	0.50
35.0	35.010	34.8	-0.210	0.50
40.0	40.015	39.8	-0.215	0.50

Note:

The result of calibration was found accurate as show on date and place of calibration only.
 This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 ๕๙๓๖ www.spmetrology.com



CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : **DIGITAL THERMOHYGRO METER**
[THERMAL ENVIRONMENT MONITOR]
MANUFACTURER : **METROSONICS**
MODEL / TYPE : **hs-32**
SERIAL NO. : **MCD070028**
CLID. NO. : **231802275**
JOB CONTROL NO. : **220901088338**

CUSTOMER : **S.P.S. CONSULTING SERVICE CO., LTD.**
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 01 September 2022

DATE OF ISSUED : 07 September 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : **Tanawan Seenam-Ngoen**
Calibration Engineer



Approved By :

Authorized Signatory
07 September 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22088338

F3-011-04/01-12

page 1 of 3



CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : **DIGITAL THERMOHYGRO METER**
[THERMAL ENVIRONMENT MONITOR]
MANUFACTURER : **METROSONICS**
MODEL / TYPE : **hs-32**
SERIAL NO. : **MCD070028**
DATE OF CALIBRATION : **02 September 2022**

ENVIRONMENT CONDITIONS :

Temperature : **(23 ± 2) °C**

Relative Humidity : **(55 ± 10) %RH**

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-74**. The calibration was performed by using
Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.
Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Thunder Scientific Corporation.
Certificate No. 19944, Due Date 26 January 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22088338

F3-011-04/01-12

page 2 of 3





CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrac, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



SP METROLOGY SYSTEM (THAILAND) CO.,LTD.



Certificate of Calibration

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter [thermal environment monitor].

CALIBRATION DATA

1. CORRECTION OF TEMPERATURE : WET

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	30.0	+0.01	0.40
35.0	35.00	35.0	0.00	
40.0	40.02	40.0	+0.02	

2. CORRECTION OF TEMPERATURE : DRY

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	29.8	+0.21	0.40
35.0	35.00	34.8	+0.20	
40.0	40.02	39.8	+0.22	

3. CORRECTION OF TEMPERATURE : GLOBE BULB

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	29.5	+0.51	0.40
35.0	35.00	34.5	+0.50	
40.0	40.02	39.5	+0.52	

Note, The Scope of Accredited TISI Certificate No. 19C987/0655 Issue 1 Page 36 of 111

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22088338

F3-011-04/01-12

page 3 of 3



Certificate Number : SPR23030505-6

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 32

Serial Number : TPE080058

ID. Number : R07

Environmental Conditions

Ambient Temperature : 23 °C ± 2 °C Received Date : 30 Mar 2023

Relative Humidity : 50 % ± 15 % Calibration Date : 31 Mar 2023

Location of Calibration : In-Lab Recommend Due Date : 31 Mar 2024

Calibration Procedure : SP-CPT-04-13 Date of Issue : 01 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by

Approved by :

Authorized Signatory

SP-FM-04-15 rev.0



Calibration Report

Certificate Number : SPR23030505-6

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR23010480-5	22 Feb 2024
THERMO-HYGROMETER	5020A	A47046	QR23-0176	26 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
SP Metrology - SP Metrology system (Thailand) Co.Ltd.

Quality Reborn Co., Ltd



Result of Calibration

Certificate No. : SPR23030505-6

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.4	0.387	0.50
35.0	35.010	35.4	0.390	0.50
40.0	40.015	40.4	0.385	0.50

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.3	0.287	0.50
35.0	35.010	35.3	0.290	0.50
40.0	40.015	40.3	0.285	0.50

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.3	0.287	0.50
35.0	35.010	35.3	0.290	0.50
40.0	40.015	40.3	0.285	0.50

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor k = 2, providing a level of confidence approximately 95%.

- End of Certificate -



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)
MANUFACTURER : 3M
MODEL / TYPE : QUESTemp[®]36
SERIAL NO. : TKE060012
CLID. NO. : 231901875
JOB CONTROL NO. : 220901088341


CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 01 September 2022

DATE OF ISSUED : 07 September 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Tanawan Seenam-Ngoen
Calibration Engineer



Approved By :

Authorized Signatory
07 September 2022

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22088341

F3-011-04/01-12

page 1 of 3



@clcalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)
MANUFACTURER : 3M
MODEL / TYPE : QUESTemp[®]36
SERIAL NO. : TKE060012
DATE OF CALIBRATION : 02 September 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. WI-305-74. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.
Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Thunder Scientific Corporation. Certificate No. 19944, Due Date 26 January 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22088341

F3-011-04/01-12

page 2 of 3



@clcalibration



Certificate of Calibration

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermo/hygro meter (thermal environment monitor).

CALIBRATION DATA

1. CORRECTION OF TEMPERATURE : WET

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	30.0	+0.01	0.40
35.0	35.00	35.0	0.00	
40.0	40.02	40.0	+0.02	

2. CORRECTION OF TEMPERATURE : DRY

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	30.01	29.7	+0.31	0.40
35.0	35.00	34.7	+0.30	
40.0	40.02	39.7	+0.32	

3. CORRECTION OF TEMPERATURE : GLOBE BULB

Test point (°C)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ± (°C)
30.0	30.01	29.8	+0.21	0.40
35.0	35.00	34.8	+0.20	
40.0	40.02	39.8	+0.22	

Note: The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22088341

F3-011-04/01-12

page 3 of 3



Certificate Number : SPR23030505-8

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 32

Serial Number : TPE070C01

ID, Number : R12

Environmental Conditions

Ambient Temperature : 23 °C ± 2 °C Received Date : 30 Mar 2023

Relative Humidity : 50 % \pm 15 % Calibration Date : 31 Mar 2023

Location of Calibration : In-Lab Recommend Due Date : 31 Mar 2024

Calibration Procedure : SP-CPT-04-13 Date of Issue : 01 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :

Approved by :

Authorized Signatory

SP-FM-04-15 rev.0



Calibration Report

Certificate Number : SPR23030505-8

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR23010480-5	22 Feb 2024
THERMO-HYGROMETER	5020A	A47046	QR23-0176	26 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
SP Metrology - SP Metrology system (Thailand) Co.Ltd.

Quality Reborn Co., Ltd

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 6870 www.spmetrology.com



Result of Calibration

Certificate No. : SPR23030505-8

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.0	-0.013	0.50
35.0	35.010	35.0	-0.010	0.50
40.0	40.015	40.0	-0.015	0.50

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.0	-0.013	0.50
35.0	35.010	35.0	-0.010	0.50
40.0	40.015	40.0	-0.015	0.50

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.1	0.087	0.50
35.0	35.010	35.1	0.090	0.50
40.0	40.015	40.1	0.085	0.50

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 6870 www.spmetrology.com



CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)
MANUFACTURER : 3M
MODEL / TYPE : QUESTemp° 46
SERIAL NO. : TSI010006
CLID. NO. : 232000793
JOB CONTROL NO. : 220505044316

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 05 May 2022

DATE OF ISSUED : 12 May 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Oranut Kamchatphai
Calibration Engineer

Approved By : 
Authorized Signatory
12 May 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22044316

F3-011-04/01-12

page 1 of 3



@clc calibration



CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)
MANUFACTURER : 3M
MODEL / TYPE : QUESTemp° 46
SERIAL NO. : TSI010006
DATE OF CALIBRATION : 05 May 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. WI-305-74. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 36151.
Temperature & Humidity Chamber, PGC Model 9141-5114 S/N.0802282.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Thunder Scientific Corporation. Certificate No. 19317, Due Date 09 July 2022.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22044316

F3-011-04/01-12

page 2 of 3



@clc calibration



CALIBRATION LABORATORY CO.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermo hygro meter (thermal environment monitor).

CALIBRATION DATA

*1. CORRECTION OF TEMPERATURE [WET]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.99	31.5	-1.51	0.40
35.0	35.01	36.5	-1.49	
40.0	39.99	41.5	-1.51	

Note, * means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

2. CORRECTION OF TEMPERATURE [DRY]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.99	30.1	-0.11	0.40
35.0	35.01	35.0	+0.01	
40.0	39.99	40.1	-0.11	

3. CORRECTION OF TEMPERATURE [GLOBE BULB]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.99	30.1	-0.11	0.40
35.0	35.01	35.0	+0.01	
40.0	39.99	39.6	+0.39	

Note, The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22044316

F3-011-04/01-12

page 3 of 3



@clccalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sae@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : LUX METER
MANUFACTURER : EXTECH INSTRUMENTS
MODEL / TYPE : 407026
SERIAL NO. : A.052323/A.052323 [LUX-R07]
CLID. NO. : 252201553
JOB CONTROL NO. : 220704067252


CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD,
JOMPOL, CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 04 July 2022

DATE OF ISSUED : 18 July 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong
Calibration Engineer

Approved By : 
Authorized Signatory
18 July 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22067252

F3-011-04/01-12

page 1 of 3



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sae@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : LUX METER
MANUFACTURER : EXTECH INSTRUMENTS
MODEL / TYPE : 407026
SERIAL NO. : A.052323/A.052323 [LUX-R07]
DATE OF CALIBRATION : 12 July 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPEE-18 by comparison with Illuminance Sensor which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Illuminance Sensor, Bentharn Model ORM400/DH400VL S/N. 27710/1/27585/3.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Optical Test and Calibration Ltd. Certificate No. 1319/6/ABU/1. Due Date 25 February 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22067252

F3-011-04/01-12

page 2 of 3





CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

LUX METER RESULT

STD Applied (lux)	DUC Reading (lux)	Correction (lux)	Uncertainty \pm (% of rdg.)
100	103	-3	3.5
200	206	-6	3.8
300	309	-9	4.7
1000	1028	-28	4.7
2000	2020	-20	4.9
3000	3040	-40	5.6

Note: The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 46 of 54

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22067252

F3-011-04/01-12

page 3 of 3



@clccalibration

Certificate No.: CP20220335EA

Operation No.: CP2022100023

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: RION

Model/Type: NL-42 (Meter), UC-52 (Microphone), NH-24 (Preamplifier)

Serial No.: 00546401 (Meter), 152917 (Microphone), 46612 (Preamplifier)

ID No.: -

Customer: IRPC Public Company Limited.

Address: 299 Moo 5, Sukhumvit Rd., Tumbon Chungnern,
Amphor Muang, Rayong 21000

Received Date: 25 October 2022

Calibrated Date: 2 - 7 November 2022

Issued Date: 16 November 2022

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: _____

Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20220335EA

Calibration Report

Equipment: Sound Level Meter
 Manufacturer: RION
 Model/Type: NL-42 (Meter), UC-52 (Microphone), NH-24 (Preamplifier)
 Serial No.: 00546401 (Meter), 152917 (Microphone), 46612 (Preamplifier)
 ID No.: -
 Ambient Temperature: (23 ± 2) °C
 Relative Humidity: (50 ± 15) %
 Pressure: (101.3 ± 1.5) kPa
 Method of Calibration :-
 IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2661000	AA-1020-22	14 June 2023
2) Arbitrary Function Generator	AFG2021	C010063	CK20220059EA	19 June 2023
3) Programmable Attenuator	PA5	2913	EF-0014-22	3 April 2023
4) 6.5 Digit precision multimeter	8846A	9610014	CB20220223EA	14 November 2023
5) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P220024 CD20220164EA	17 March 2023 24 July 2023
6) Pressure humidity and Temperature Transmitter	PTU301	F0640003	CL1-P220029 CD20220165EA	31 March 2023 24 July 2023
7) Performance Audio Analyzer	U8903B	MY56510003	CB20220063EA CK20220080EA	15 February 2023 8 September 2023

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
94.1	94.1	0.0	±1.0

Note : Absolute sensitivity was established by the use of the Sound Calibrator RION Type NC-74 S/N : 34536113.

Certificate No.: CP20220335EA

Calibration Report

Equipment: Sound Level Meter
 Manufacturer: RION
 Model/Type: NL-42 (Meter), UC-52 (Microphone), NH-24 (Preamplifier)
 Serial No.: 00546401 (Meter), 152917 (Microphone), 46612 (Preamplifier)
 ID No.: -
 Ambient Temperature: $(23 \pm 2) ^\circ\text{C}$
 Relative Humidity: $(50 \pm 15) \%$
 Pressure: $(101.3 \pm 1.5) \text{ kPa}$

Method of Calibration :-

IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

	Instrument	Model	Serial No.	Cert. No.	Due Date
1)	Standard microphone	4180	2661000	AA-1020-22	14 June 2023
2)	Arbitrary Function Generator	AFG2021	C010063	CK20220059EA	19 June 2023
3)	Programmable Attenuator	PA5	2913	EF-0014-22	3 April 2023
4)	6.5 Digit precision multimeter	8846A	9610014	CB20220223EA	14 November 2023
5)	Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P220024 CD20220164EA	17 March 2023 24 July 2023
6)	Pressure humidity and Temperature Transmitter	PTU301	F0640003	CL1-P220029 CD20220165EA	31 March 2023 24 July 2023
7)	Performance Audio Analyzer	U8903B	MY56510003	CB20220063EA CK20220080EA	15 February 2023 8 September 2023

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
94.1	94.1	0.0	± 1.0

Note : Absolute sensitivity was established by the use of the Sound Calibrator RION Type NC-74 S/N : 34536113.

Certificate No.: CP20220335EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
15.4

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	11.3
C-weighting	17.1
Z-weighting	23.2

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.7	0.7	0.8	±1.5
1000	0.2	0.2	0.2	±1.0
8000	-2.4	-2.3	-2.4	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	-0.1	0.0	±2.0
125	0.0	-0.1	0.0	±1.5
250	0.0	-0.1	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.1	0.1	0.0	±5.0

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

Certificate No.: CP20220335EA

Calibration Report

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
130.0	130.0	0.0	±1.1
131.0	131.0	0.0	±1.1
132.0	132.0	0.0	±1.1
133.0	133.0	0.0	±1.1
134.0	134.0	0.0	±1.1
135.0	135.0	0.0	±1.1
136.0	136.0	0.0	±1.1
137.0	137.0	0.0	±1.1

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1

Certificate No.: CP20220335EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower (Cont.)

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.0	0.0	±1.1
39.0	39.0	0.0	±1.1
34.0	33.8	-0.2	±1.1
29.0	28.9	-0.1	±1.1

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	126.0	0.0	±1.0
	2	109.0	0.0	+1.0 ; -2.5
	0.25	99.9	-0.1	+1.5 ; -5.0
Slow	200	119.6	0.0	±1.0
	2	100.0	0.0	+1.0 ; -5.0
LAE	200	120.0	0.0	±1.0
	2	100.0	0.0	+1.0 ; -2.5
	0.25	90.9	-0.1	+1.5 ; -5.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	125.4	125.2	-0.2	±3.0
Positive half cycle	124.4	124.1	-0.3	±2.0
Negative half cycle	124.4	124.1	-0.3	±2.0

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
139.5	139.6	0.1	±1.5

Certificate No.: CP20220335EA

Calibration Report

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	129.0	129.0	0.0	±0.3

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks: 1. The acceptance limit is for the deviated value.
2. Acceptance limits was IEC61672-3:2013 Class 2.
3. The coverage factor $k = 2.00$

-- End of Report --

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0455

MTC No. EEL. BP. 41/0465

CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Keithley 2015-P S/N 4106495.

7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 22 Apr. 2022

Date of Calibration : 28 Apr. 2022

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0455

MTC No. EEL. BP. 41/0465

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.93	-0.07	± 0.10	± 0.40 dB

2. Frequency


Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.44	± 0.50	$\pm 3.0\%$

- Note :
1. No adjustment.
 2. The calibrator pressure correction was not included.
 3. The microphone volume correction was not included.

Calibrated by :



Approved by :



(Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 28 Apr. 2022

Date of Issue : 28 Apr. 2022

Ref : 2011265042601787001

2 / 2

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



บริษัท เอกเสคคิวทิฟ เทรดดิง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230
TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

ที่ RA 033/23

ใบรายงานผลการปรับเทียบ

ชื่อผู้ขอรับบริการ : บริษัท ไออาร์พีซี จำกัด (มหาชน)

ที่อยู่ : 299 หมู่ 5 ถนนสุขุมวิท ตำบลเชิงเนิน อำเภอเมืองระยอง จังหวัดระยอง 21000

ปรับเทียบที่ : บริษัท เอกเสคคิวทิฟ เทรดดิง จำกัด

ที่อยู่ : 48/194-5 ซอย ประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวง/เขตลาดพร้าว กรุงเทพฯ 10230

รายละเอียดเครื่องมือที่ทำการปรับเทียบ :

เครื่องมือ : เครื่องตรวจวัดไอระเหยจากสารเคมี

ผลิตภัณฑ์ : RAE Systems

รุ่น : MiniRAE3000

หมายเลขเครื่อง : 592-001193

สภาวะแวดล้อม :

อุณหภูมิ : $(25 \pm 3) ^\circ\text{C}$

ความชื้นสัมพัทธ์ : $(24 \pm 15) \%$

ความดันบรรยากาศ : 760 มิลลิเมตรปรอท

วันที่ปรับเทียบมาตรฐาน : 7 มีนาคม 2566

วันที่ครบกำหนดการปรับเทียบ : 7 มีนาคม 2567

วิธีการปรับเทียบมาตรฐาน : ปรับเทียบ โดยใช้ Standard Reference Gas ผลิตภัณฑ์ CALGAZ.

- Isobutylene Standard Gas 100 ppm; Lot number 304-402257108-1.

- Isobutylene Standard Gas 1000 ppm; Lot number 304-402250416-1.

ผลการปรับเทียบมาตรฐาน

Sensor Type	Reference Concentration	Before Cal.	After Cal.	Error Reading	Result
PID	0 ppm (Air Zero)	0.0 ppm	0.0 ppm	0.0 ppm	Pass
PID	100 ppm (Isobutylene 100 ppm)	85.0 ppm	100.0 ppm	0.0 ppm	Pass
PID	1000 ppm (Isobutylene 1000 ppm)	899.5 ppm	991.8 ppm	8.2 ppm	Pass

Flow Rate of Pump : 480 cc/min.

Accuracy : $\pm 2 \%$ at calibration point

ผลการสอบเทียบ/ปรับเทียบ นี้ รับรองเฉพาะตัวอย่างและรายการที่ได้ระบุไว้เท่านั้น

การนำรายงานผล/ใบรับรองนี้ไปโฆษณาและการคัดลอกหรือการนำผลบางส่วนไปเผยแพร่ต่อสาธารณะต้องได้รับอนุญาตเป็นลายลักษณ์อักษรจากทางบริษัทฯ



บริษัท เอกเสคคิวทิฟ เทรตติ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230

TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

No. RA 033/23

Certificate of Calibration

Customer : IRPC Public Company Limited.

Address : 169 Moo 9, Suk Sawat 45, Suk Sawat Road, Bang Kru, Phra Pradaeng, Samut Prakan 10130
Thailand.

Calibration location : Executive Trading Limited.

Address : 48/194-5 Soi Praditmanutham 19, Pradit Manutham Road, Latphrao, Bangkok 10230

Tools :

Environmental Condition :

Instrument : Gas Detector

Temperature : $(25 \pm 3) ^\circ\text{C}$

Product : RAE Systems

Relative Humidity : $(24 \pm 15) \%$

Model Name : MiniRAE3000

Pressure : 760 mmHg

Serial Number : 592-001193

Date of Calibration : March 7, 2023

Due Date of Calibration : March 7, 2024

Calibration Method : This instrument has been calibrated using calibration gases. Test and calibration data is
On file with Executive trading limited.

Reference Standard : - Isobutylene Standard Gas 100 ppm; Lot number 304-402257108-1.
- Isobutylene Standard Gas 1000 ppm; Lot number 304-402250416-1.

Test Result

Sensor Type	Reference Concentration	Before Cal.	After Cal.	Error Reading	Result
PID	0 ppm (Air Zero)	0.0 ppm	0.0 ppm	0.0 ppm	Pass
PID	100 ppm (Isobutylene 100 ppm)	85.0 ppm	100.0 ppm	0.0 ppm	Pass
PID	1000 ppm (Isobutylene 1000 ppm)	899.5 ppm	991.8 ppm	8.2 ppm	Pass

Flow Rate of Pump : 480 cc/min.

Accuracy : $\pm 2 \%$ at calibration point

The results relate only to the items tested or calibrated.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the company.



บริษัท เอกเสคคิวทิฟ เทรตติ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230
TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

ที่ RA 033/23

ใบรายงานการตรวจเช็คเครื่องตรวจวัดก๊าซ รุ่น MiniREA3000

หมายเลขเครื่อง : 592-001193

วันที่ตรวจเช็ค : 7 มีนาคม 2566

ลำดับที่	รายละเอียดการตรวจสอบ	RAW COUNT		สรุป	หมายเหตุ
		REF.	REAL		
1.	PID RAW COUNT				
	Ch.H	10000-62500	48079	■ YES □ NO	
	Ch.L	<62500	52722	■ YES □ NO	
2.	Lamp	>40	48	■ YES □ NO	

ลำดับที่	รายละเอียดการตรวจซ่อม	การแก้ไข	สรุป	หมายเหตุ
1.	Motor Pump	Check flow rate	■ YES □ NO	480 cc/min.
2.	Buzzer	-	■ YES □ NO	-
3.	Li-ion Battery	-	■ YES □ NO	-
4.	Key Pad			
	Y/+	-	■ YES □ NO	-
	N/-	-	■ YES □ NO	-
	MODE	-	■ YES □ NO	-
5.	LCD Display	-	■ YES □ NO	-
6.	Light Sensor	-	■ YES □ NO	-
7.	Pocket Clip	-	□ YES □ NO	-
8.	PC Port	-	■ YES □ NO	-
9.	Slim Rubber Boot	-	■ YES □ NO	-
10.	Tube adapter assembly	-	□ YES □ NO	-

ผลการสอบเทียบ/ปรับเทียบ นี้ รับรองเฉพาะตัวอย่างและรายการที่ได้รับอนุญาตไว้เท่านั้น

การนำรายงานผล/ใบรับรองนี้ไปโฆษณาและการคัดค้านหรือการนำผลบางส่วนไปเผยแพร่ต่อสาธารณะต้องได้รับอนุญาตเป็นลายลักษณ์อักษรจากทางบริษัทฯ



CERTIFICATE OF ANALYSIS

Date: November 8, 2021
PO Number: 0000020821
Lot Number: 304-402257108-1

Customer: CalGaz Internl LLC

Use Before: 11/08/2025


<u>Component</u>	<u>Requested Concentration</u>	<u>Analytical Result (+/- 2%)</u>
Isobutylene	100 PPM	100.5 PPM
Air	Balance	Balance

Cylinder Size: 3.6 Cu. Ft.
Contents: 103 Liter

Valve: 5/8" -18UNF
Pressure: 1000 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/ or N.I.S.T. Gas Mixture reference materials.

Analyst:





CERTIFICATE OF ANALYSIS

Date: November 8, 2021
Order Number: 0000020821
Lot Number: 304-402250416-1

Customer: CalGaz Internl LLC
Use Before: 11/08/2025


<u>Component</u>	<u>Requested Concentration</u>	<u>Analytical Result (+/- 2%)</u>
Isobutylene Air	1000 PPM Balance	995 PPM Balance

Cylinder Size: 1.2 Cu. Ft.
Contents: 34 Liter

Valve: CGA 600
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/ or N.I.S.T. Gas Mixture reference materials.

Analyst:



**CERTIFICATE
of
Attendance**

It is hereby certified that

Mr Surinthorn Sainate
(Executive Trading Limited)


has successfully completed the

RAE Service Training Course

Conducted by

HONEYWELL

on **2nd August 2022**



Conducted by : Desmond Tan
Service Engineer / Technical Trainer
Date of Issue : 2nd August 2022
Certificate valid for 2 years from date of issue

DATA SHEET FOR CALIBRATION / VERIFICATION AND INSPECTION


Calibration

Verification

Inspection
เครื่องมือ / อุปกรณ์ ที่สอบเทียบหรือทวนสอบ

Equipment / Tools : Multimeter (pH , DO) Tag No. / I.D. No. : L09-AT-SP003-A2 Serial No. : 130500088588

Cal. / Ver. date : 4/4/2022
เครื่องมือ / อุปกรณ์ที่เป็น Master

Equipment / Tools :	I.D. No.	Model /Serial No.	Cert. No.	Expired date

Reference Materials ที่ใช้

Chemical	Grade	Assay (%)	Cert. No.	Expired date
Buffer pH 4.00 ; Lot No. HC99677935				31/7/2022
Buffer pH 7.00 ; Lot No. HC04269139				31/10/2023
Buffer pH 10.00 ; Lot No. HC02905338				30/6/2023


Calibration / verification item	Result	Error	Acceptance Criteria	Pass / Fail
1.การสอบเทียบ Observed Slope (slope)	98	-	95 to 105%	Pass
2.verification pH6.86	6.85	-0.01	± 0.05	Pass

Inspection item	Result	Correction
1.ตรวจเช็คสภาพพร้อมใช้งาน	ปกติ	

Next Due date 31/5/2022

Performed by : 

Date : 4/4/2022

Approved By : 

Date : 4/4/2022

Certificate of Analysis – Certified Reference Material

Certipur® Buffer solution pH 10.00 (20°C)

Certified Reference Material for pH measurement

Product no.: 1.09438.1000
Lot no.: HC02905338
Description of CRM: Certipur® Buffer solution pH 10.00 (20°C)
Certified Reference Material for pH measurement
Expiry date: 2023/06/30
Storage: +15°C to +25°C tightly closed in the original container
Composition: boric acid / potassium chloride / sodium hydroxide



Certified value

Associated uncertainty, $U = k \cdot u$
($k=2$)

pH value 10.01

± 0.03 (20°C)

Metrological traceability:

The pH value of this certified buffer solution is directly traceable to primary certified reference materials characterised by PTB and verified by SRMs from NIST.

NIST 189c, 188, 185i, 186 Ig, 186 IIg, 187f

PTB OX-405/18, TA-442/19, PHT-340/16, PHO-346/16, BO-373/17

PTB: Physikalisch Technische Bundesanstalt, Braunschweig, Germany

NIST: National Institute of Standards and Technology, Gaithersburg, USA.

Measurement method:

pH value is measured with a combined glass electrode after 5-point calibration according to DIN 19268 with reference buffer solutions according to DIN 19266, IUPAC, NIST, Ph.Eur. and USP.

Accreditation:

Merck KGaA, Darmstadt, Germany is accredited by the German accreditation authority DAkkS as registered reference material producer D-RM-15185-01-00 in accordance with ISO 17034 and registered calibration laboratory D-K-15185-01-00 according to DIN EN ISO/IEC 17025.

Certificate issue date:

2020/06/24



ISO 17034



ISO/IEC 17025

CRM released by Approving Officer
or delegate LS-OII-QS3

Dipl.-Ing. Ayfer Yildirim
Responsible Manager of LS-OII-QS3
(Calibration Laboratory D-K-15185-01)



Intended use:	This reference material is intended for use as a calibration standard for pH instruments or pH electrodes or as a control sample for measuring the pH value.
Instructions for handling and correct use:	The pH value is strongly dependent on the temperature. It is therefore necessary to keep the temperature constant within the measurement.
Health and safety information:	Please refer to the Safety Data Sheet for detailed information about the nature of any hazard and appropriate precautions to be taken.
Preparation:	This reference material is prepared gravimetrically from boric acid, potassium chloride, sodium hydroxide and high purity water.

Associated uncertainty:

The expanded uncertainty U_{CRM} is calculated as $U_{CRM} = k \cdot u_{CRM}$, where $k = 2$ is the coverage factor for a 95% coverage probability and u_{CRM} is the combined standard uncertainty in accordance to ISO 17034.

The combined uncertainty u_{CRM} is derived from combination of the squared uncertainty contributions:

$$u_{CRM} = \sqrt{u^2_{\text{Characterisation}} + u^2_{\text{Homogeneity}} + u^2_{\text{Stability}}}$$

$u_{\text{characterisation}}$:	is the uncertainty in accordance with DIN EN ISO/IEC 17025 which includes the contributions of the primary reference material and the measuring system.
$u_{\text{homogeneity}}$:	is the between-bottle variation in accordance with ISO 17034. The assessment of homogeneity is performed by analysis of a representative number of systematically chosen sample units.
$u_{\text{stability}}$:	is the uncertainty obtained from short-term and long-term stability in accordance with ISO 17034. The stability studies are the basis for the quantification of the expiry date of this reference material for the unopened bottle.

Informative values:

Temperature dependence¹:

Temperature [°C]	Δ pH
0	+ 0.26
5	+ 0.17
10	+ 0.11
15	+ 0.05
20	± 0
25	- 0.06
30	- 0.11
35	- 0.16
40	- 0.18
50	- 0.26

¹Temperature deviation data provided for reference only. Values are not batch-specific and should not be considered certified values.

For more detailed information please read the certification report on our website.

Certificate of analysis revision history:

Certificate version	Date	Reason for version
01	2020/06/24	Initial version





PETRO-INSTRUMENTS CORP., LTD.

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak Bangkok 10900 Thailand

Tel. : (+66) 2939 5711 (12 Lines), (+66) 2513 2333 (12 Lines), Fax. : (+66) 939 4207, (+66) 2939 4207

Website : <http://www.pico.co.th> email-address: pico@pico.co.th , service@pico.co.th

DOC. NUMBER

CMV-S23-0034

SERVICE REPORT

REPORT DATE

June 21, 2023

EQUIPMENT: Multi Water Quality Checker, U-5000G	SERIAL NUMBER / TAG NUMBER RAAGSEN3	BRAND / MANUFACTURER HORIBA
CUSTOMER NAME: IRPC PUBLIC COMPANY LIMITED	LACATION: rayong	JOB NUMBER / REQUESTED NUMBER JID2300281-002

SCOPE OF WORK / REASON FOR VISIT

Repair and Calibration

FOUND FAILURE & CORRECTIVE ACTION DETAILS

1. ตรวจสอบสภาพเครื่อง Multi Water Quality Checker

- Meter Model: U-5000G S/N: RAAGSEN3 สามารถใช้งานได้ปกติ
- Probe Model: U-53 S/N: V39CGM6U พบว่า **Sensor Turbidity** ไม่สามารถใช้งานได้
- Sensor pH,COND,ORP,DO ใช้งานได้ปกติ

2. ทำการ Cleaning sensor ทุก parameter

- เติมน Internal Solution (KCl) ใน Reference sensor

3. ปรับเทียบ Auto Calibration ด้วย Buffer pH 4

- พบว่าสามารถปรับเทียบค่าผ่าน คือ pH , COND, ORP, Temp, DO and Depth

4. ปรับเทียบ Manual Calibration 2 จุด (zero , span)

- พบว่าสามารถปรับเทียบค่าผ่าน คือ pH , COND,ORP, Temp, DO and Depth

สรุป : เครื่อง Multi Water Quality Checker Meter Model: U-5000G S/N: RAAGSEN3 และ

Sensor Model: U-53 S/N: V39CGM6U สามารถใช้งานได้ตามปกติ ยกเว้น Sensor Turbidity

WORK CONCLUSION

<input checked="" type="checkbox"/> COMPLETED		<input type="checkbox"/> IN COMPLETED	PARTS REPLACEMENT		
<input checked="" type="checkbox"/> CHARGE	<input type="checkbox"/> NO CHARGE		PARTS NAME	P/N	QTY.
<input checked="" type="checkbox"/> Service Fee	<input type="checkbox"/> Project Warranty	<input type="checkbox"/> Take to Office			
<input type="checkbox"/> Travelling	<input type="checkbox"/> Service Warranty	<input type="checkbox"/> Wait for Parts			
<input type="checkbox"/> Spare Parts	<input type="checkbox"/> Spare Parts Warranty	<input type="checkbox"/> In Progress			
<input type="checkbox"/> Other	<input type="checkbox"/> Service Contract	<input type="checkbox"/> Other			

TIME SPENT (HOURS)

YEAR	2023							TOTAL HOURS	TRAVELING DETAILS	
MONTH	6									
DATE	21								TRAVEL BY	-
SERVICE TIME	4							4	FROM	-
OVERTIME	-							-	TO	-
TRAVELING TIME	-							-	TOTAL ROUND TRIP	-
TOTAL HOURS	4							4	DISTANCE (KM.)	-

SERVICE CREW

NAME		NAME	
1. Chamaiporn Vongchalee		3.	
2.		4.	

CUSTOMER'S NAME	CUSTOMER'S SIGNATURE	DATE



บริษัท เพทโร-อินสตรูเมนต์ จำกัด
PETRO-INSTRUMENTS CORP., LTD.

7/409 ซ.วิภาวดีรังสิต 36 ถ.วิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak, Bangkok 10900, Thailand.

TEL : (662) 9395711 (12 Lines), 5132333 (12 Lines), 5139575-9 FAX : (662) 9394207, 9394208


<http://www.pico.co.th> E-mail-address : pico@pico.co.th

TEST REPORT OF CALIBRATION

We hereby certify that the equipment mentioned below have been maintained and have duly performed in accordance with HORIBA specifications.

Equipment	:	Multi Water Quality Checker
Model	:	U-5000G
Manufacture	:	HORIBA
Serial No.	:	RAAGSEN3
Job No.	:	JID2300281-002
Customer	:	IRPC Public Company Limited
Calibration date	:	June 21, 2023
Calibration due	:	June 21, 2024

Petro-Instruments Corp., Ltd.





บริษัท เพทโร-อินสตรูเมนต์ จำกัด
PETRO-INSTRUMENTS CORP., LTD.

7/409 ซ.วิภาวดีรังสิต 36 ถ.วิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak, Bangkok 10900, Thailand.

TEL : (662) 9395711 (12 Lines), 5132333 (12 Lines), 5139575-9 FAX : (662) 9394207, 9394208

<http://www.pico.co.th> E-mail-address : pico@pico.co.th

CALIBRATION REPORT

Equipment : Multi Water Quality Checker
Manufacturer : HORIBA
Model : U-53
Serial No. : V39CGM6U
Date of Calibration : June 21, 2023
Customer Name : IRPC Public Company Limited

HORIBA, Multi Water Quality Checker model U-53 was tested according to service manual.

Auto Calibration (1- point)

Check function	Calibration	Before Calibrate	After Calibrate
pH	1- point auto (Zero) (4.01 pH)	4.05 pH	4.01 pH
CONDUCTIVITY	1- point auto (Span) (4.49 mS/cm)	4.45 mS/cm	4.49 mS/cm
DO	1- point auto (Span) (8.92 mg/L)	8.87 mg/L	8.92 mg/L
Depth	(0 m)	0 m	0 m

Reference Standard

- Standard Solution of HORIBA, pH 4 Lot No. S3316/03



บริษัท เพทโร-อินสตรูเมนต์ จำกัด
PETRO-INSTRUMENTS CORP., LTD.

7/409 ซ.วิภาวดีรังสิต 36 ถ.วิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak, Bangkok 10900, Thailand.

TEL : (662) 9395711 (12 Lines), 5132333 (12 Lines), 5139575-9 FAX : (662) 9394207, 9394208

<http://www.pico.co.th> E-mail-address : pico@pico.co.th

Manual Calibration (2- point)

A. pH Measurement.

Check item	pH Standard Solution	Before Calibrate	After Calibrate	Error	Judgment
Zero Calibration	6.86	6.86	6.86	0.00	PASS
Span Calibration	4.01	4.01	4.01	0.00	PASS

Measure at temperature 25 °C Within ± 0.1 pH

B. Conductivity Measurement.

Check item	Conductivity Standard Solution	Before Calibrate	After Calibrate	Error	Judgment
Zero Calibration	0.00 mS/cm	0.000 mS/cm	0.00 mS/cm	0.000 mS/cm	PASS
Span Calibration	Range 1 (0.100-0.999 S/m) 0.718 mS/cm	0.728 mS/cm	0.718 mS/cm	0.01 mS/cm	PASS
	Range 2 (1.00-10.00 S/m) 6.67 mS/cm	6.70 mS/cm	6.67 mS/cm	0.003 mS/cm	PASS
	Range 3 (0.0-99.9 mS/m) 58.7 mS/cm	59.0 mS/cm	58.7 mS/cm	0.3 mS/cm	PASS

Measure at temperature 25 °C Within $\pm 1\%$ /F.S.



บริษัท เพทโร-อินสตรูเมนต์ จำกัด
PETRO-INSTRUMENTS CORP., LTD.

7/409 ซ.วิภาวดีรังสิต 36 ถ.วิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak, Bangkok 10900, Thailand.

TEL : (662) 9395711 (12 Lines), 5132333 (12 Lines), 5139575-9 FAX : (662) 9394207, 9394208

http://www.pico.co.th E-mail-address : pico@pico.co.th

C. DO Measurement.

Check item	DO Standard Solution	Before Calibrate	After Calibrate	Error	Judgment
Zero Calibration	(Solution of NaSO ₃) 0.00 mg/l	0.00 mg/l	0.00 mg/l	0.00 mg/l	PASS
Span Calibration	(Saturated with oxygen in air) 8.11 mg/l	8.15 mg/l	8.11 mg/l	0.04 mg/l	PASS

Measure at temperature 25 °C With in 0 to 20 mg/L :± 0.2 mg/l, 20 to 50 mg/L :± 0.5 mg/l

Calibrated by : Chamaiporn Vongchalee

Approved by : Athitphong Kanchanasathian