

ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft^3/min)	R^2
B35	B35	01/02/2023	$y = 1.194x - 4.992$	0.995
B36	B36	02/02/2023	$y = 1.201x - 3.946$	0.997
B37	B37	02/02/2023	$y = 1.284x - 6.745$	0.997
B38	B38	02/02/2023	$y = 1.250x - 6.733$	0.998
B39	B39	01/02/2023	$y = 1.268x - 7.186$	0.998
B40	B40	03/02/2023	$y = 1.214x - 4.324$	0.998
B41	B41	03/02/2023	$y = 1.176x - 2.734$	0.999
B42	B42	02/02/2023	$y = 1.283x - 8.167$	0.997
B43	B43	02/02/2023	$y = 1.197x - 3.772$	0.996
B44	B44	02/02/2023	$y = 1.249x - 7.038$	0.995
R01	R01	01/02/2023	$y = 1.287x - 8.462$	0.998
R02	R02	01/02/2023	$y = 1.239x - 6.678$	0.998
R03	R03	03/02/2023	$y = 1.254x - 7.928$	0.999
R04	R04	02/02/2023	$y = 1.206x - 3.694$	0.999
R05	R05	02/02/2023	$y = 1.237x - 6.503$	0.997
R06	R06	02/02/2023	$y = 1.239x - 4.541$	0.995
R07	R07	03/02/2023	$y = 1.060x + 1.983$	0.999
R08	R08	03/02/2023	$y = 1.274x - 8.050$	0.998
R09	R09	02/02/2023	$y = 1.280x - 7.005$	0.998
R10	R10	03/02/2023	$y = 1.244x - 5.980$	1.000
R11	R11	03/02/2023	$y = 1.097x - 0.462$	0.998
R12	R12	02/02/2023	$y = 1.151x - 2.727$	0.995
R13	R13	02/02/2023	$y = 1.134x - 1.526$	1.000
R14	R14	02/02/2023	$y = 1.172x - 2.510$	0.999
R15	R15	01/02/2023	$y = 1.131x - 2.129$	0.998
R16	R16	01/02/2023	$y = 1.202x - 5.830$	0.998
R17	R17	01/02/2023	$y = 1.182x - 3.281$	0.998
R18	R18	03/02/2023	$y = 1.217x - 5.060$	0.999
R19	R19	03/02/2023	$y = 1.228x - 6.084$	0.998
R20	R20	03/02/2023	$y = 1.277x - 9.434$	0.997



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume PM-10 Data

Calibration Data

Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
R01	R01	01/02/2023	y = 1.253x-8.016	0.996
R02	R02	01/02/2023	y = 1.246x-5.052	0.998
R03	R03	02/02/2023	y = 1.239x-5.451	0.999
R04	R04	03/02/2023	y = 1.263x-8.320	0.999
R05	R05	03/02/2023	y = 1.193x-4.904	0.998
R06	R06	03/02/2023	y = 1.270x-7.534	0.995
R07	R07	03/02/2023	y = 1.244x-5.727	0.998
R08	R08	02/02/2023	y = 1.277x-7.820	0.998
R09	R09	02/02/2023	y = 1.183x-5.015	0.996
R10	R10	01/02/2023	y = 1.200x-4.576	0.999
R11	R11	01/02/2023	y = 1.225x-4.833	0.995
R12	R12	03/02/2023	y = 1.273x-8.109	0.998
R13	R13	01/02/2023	y = 1.281x-6.830	1.000
R14	R14	01/02/2023	y = 1.288x-7.622	0.999
R15	R15	02/02/2023	y = 1.282x-8.311	0.997
R16	R16	02/02/2023	y = 1.246x-5.817	0.995
R17	R17	03/02/2023	y = 1.263x-7.123	0.999
R18	R18	03/02/2023	y = 1.203x-5.483	0.999
R19	R19	01/02/2023	y = 1.204x-4.399	0.996
R20	R20	01/02/2023	y = 1.259x-8.655	0.997



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B35	B35	01/05/2023	$y = 1.310x - 9.363$	0.996
B36	B36	02/05/2023	$y = 1.201x - 4.686$	0.999
B37	B37	02/05/2023	$y = 1.239x - 4.586$	0.998
B38	B38	02/05/2023	$y = 1.304x - 9.606$	0.997
B39	B39	01/05/2023	$y = 1.240x - 5.469$	0.998
B40	B40	03/05/2023	$y = 1.196x - 4.045$	0.999
B41	B41	03/05/2023	$y = 1.179x - 2.611$	0.999
B42	B42	02/05/2023	$y = 1.246x - 7.813$	0.996
B43	B43	02/05/2023	$y = 1.206x - 3.694$	0.999
B44	B44	02/05/2023	$y = 1.302x - 9.108$	0.999
R01	R01	02/05/2023	$y = 1.268x - 7.113$	0.995
R02	R02	01/05/2023	$y = 1.235x - 6.759$	0.997
R03	R03	03/05/2023	$y = 1.247x - 7.848$	0.996
R04	R04	02/05/2023	$y = 1.161x - 1.778$	0.999
R05	R05	02/05/2023	$y = 1.288x - 9.494$	0.999
R06	R06	02/05/2023	$y = 1.277x - 6.891$	0.997
R07	R07	02/05/2023	$y = 1.046x + 2.772$	1.000
R08	R08	02/05/2023	$y = 1.206x - 5.068$	0.997
R09	R09	02/05/2023	$y = 1.296x - 8.463$	0.999
R10	R10	02/05/2023	$y = 1.244x - 6.477$	0.999
R11	R11	02/05/2023	$y = 1.097x - 0.462$	0.998
R12	R12	02/05/2023	$y = 1.210x - 5.084$	0.998
R13	R13	01/05/2023	$y = 1.149x - 1.965$	1.000
R14	R14	01/05/2023	$y = 1.189x - 3.035$	0.998
R15	R15	02/05/2023	$y = 1.161x - 3.437$	0.998
R16	R16	01/05/2023	$y = 1.158x - 4.330$	0.997
R17	R17	02/05/2023	$y = 1.218x - 5.356$	0.998
R18	R18	02/05/2023	$y = 1.234x - 5.546$	0.999
R19	R19	02/05/2023	$y = 1.267x - 7.058$	0.999
R20	R20	01/05/2023	$y = 1.264x - 8.743$	0.999



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
R01	R01	01/05/2023	$y = 1.189x - 4.728$	0.996
R02	R02	01/05/2023	$y = 1.265x - 5.602$	0.999
R03	R03	01/05/2023	$y = 1.215x - 5.146$	0.997
R04	R04	01/05/2023	$y = 1.226x - 6.655$	0.997
R05	R05	01/05/2023	$y = 1.212x - 5.960$	1.000
R06	R06	04/05/2023	$y = 1.238x - 5.381$	0.995
R07	R07	04/05/2023	$y = 1.283x - 7.908$	0.998
R08	R08	04/05/2023	$y = 1.281x - 7.778$	1.000
R09	R09	03/05/2023	$y = 1.202x - 6.317$	0.999
R10	R10	02/05/2023	$y = 1.169x - 2.499$	0.999
R11	R11	01/05/2023	$y = 1.210x - 4.423$	0.996
R12	R12	01/05/2023	$y = 1.176x - 3.099$	0.997
R13	R13	01/05/2023	$y = 1.276x - 6.852$	0.997
R14	R14	03/05/2023	$y = 1.207x - 4.849$	0.996
R15	R15	03/05/2023	$y = 1.198x - 4.617$	0.997
R16	R16	04/05/2023	$y = 1.199x - 5.485$	0.995
R17	R17	04/05/2023	$y = 1.184x - 4.669$	0.998
R18	R18	04/05/2023	$y = 1.167x - 4.142$	0.998
R19	R19	04/05/2023	$y = 1.197x - 5.308$	0.997
R20	R20	02/05/2023	$y = 1.244x - 8.211$	0.999



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

CALIBRATION REPORT

NON-DISPERSIVE INFRARED CO ANALYZER

DATE : 6 February 2023

BRAND : API

MODEL : 300E

NO. CO-R03

SERIAL NO. 1352

Calibrator (Dilution System)

Brand : API Model : 700
Last Cal. Date : 06 September 2022 Serial No. : 421

Reference Standard Gas

Standard Gas : Carbon Monoxide (CO) Cylinder No. : D196045
Certified Date : 16 April 2022 Expired Date : 15 April 2024 Cylinder Conc. : 4,570 PPM

CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.5 °C % RH 49

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response
Zero	0	0.11	-	0
CO Span	40.00	40.11	0.275	40.00

API Model 300E CO Analyzer Check list

Parameter	Observed Value	Units	Nominal Range
RANGE	50	PPM	0-1000 ppm
STABILITY	0.10	PPM	< 1 ppm with zero air
CO MEASURE	4017.6	mV	2500-4800 mV
CO REFERENCE	3948.5	mV	2500-4800 mV
MEASURE/REFERENCE RATIO	1.180	-	1.1-1.3 w/zero air
SAMPLE PRESSURE	28.4	In-Hg-A	~2" < ambient absolute pressure
SAMPLE FLOW	807	cc/min	800 ± 10%
SAMPLE TEMPERATURE	48.5	°C	48 ± 4
BENCH TEMPERATURE	48.2	°C	48 ± 2
WHEEL TEMPERATURE	68.3	°C	68 ± 2
BOX TEMPERATURE	30.6	°C	Ambient temp + 7 ± 10
PHOTO-DRIVE	3040.7	mV	250 mV to 4750 mV
SLOPE	1.018	-	1.0 ± 0.3
OFFSET	0.2	-	0 ± 0.3



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

CALIBRATION REPORT

NON-DISPERSIVE INFRARED CO ANALYZER

DATE : 15 May 2023

BRAND : API

MODEL : 300E

NO. CO-R02

SERIAL NO. 171-S

Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 06 September 2022

Serial No. : 421

Reference Standard Gas

Standard Gas : Carbon Monoxide (CO)

Cylinder No. : D196045

Certified Date : 16 April 2022

Expired Date : 15 April 2024

Cylinder Conc. : 4,570 PPM

CALIBRATING CONDITION

Pressure 1011

mmbar

Temp. 24.5

°C

% RH

49

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response
Zero	0	-0.10	-	0
CO Span	40.00	39.95	-0.125	40.00

API Model 300E CO Analyzer Check list

Parameter	Observed Value	Units	Nominal Range
RANGE	50	PPM	0-1000 ppm
STABILITY	0.10	PPM	< 1 ppm with zero air
CO MEASURE	4014.8	mV	2500-4800 mV
CO REFERENCE	3947.5	mV	2500-4800 mV
MEASURE/REFERENCE RATIO	1.180	-	1.1-1.3 w/zero air
SAMPLE PRESSURE	28.6	In-Hg-A	~2" < ambient absolute pressure
SAMPLE FLOW	805	cc/min	800 ± 10%
SAMPLE TEMPERATURE	48.6	°C	48 ± 4
BENCH TEMPERATURE	48.3	°C	48 ± 2
WHEEL TEMPERATURE	68.4	°C	68 ± 2
BOX TEMPERATURE	30.8	°C	Ambient temp + 7 ± 10
PHOTO-DRIVE	3025.6	mV	250 mV to 4750 mV
SLOPE	1.017	-	1.0 ± 0.3
OFFSET	0.2	-	0 ± 0.3



CALIBRATION REPORT

SO₂ FLUORESCENT ANALYZER

DATE : 6 February 2023

BRAND : API

MODEL : 100E

NO. SO₂-R04

SERIAL NO. 3489

Calibrator (Dilution System)

Brand	: API	Model	: 700
Last Cal. Date	: 04 August 2022	Serial No.	: 911

Reference Standard Gas

Standard Gas	: Sulphur Dioxide (SO ₂)	Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029
		Cylinder Conc.	: 50.0 ppm

CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.5 °C % RH 49

CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO ₂ Span	400.0	400.2	0.050	400.0	1.010

API Model 100E SO₂ Analyzer Check list

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	0-500
SAMPLE PRESS	28.4	in-Hg	25-35
SAMPLE FLOW	658	cc/min	650 ± 10%
PMT	103.1	mV	-20-150 with Zero Air
UV LAMP	3022.7	mV	1000-4900
STR. LGT	61.5	PPB	<100
DRK PMT	63.0	mV	-50 - 200
DRK LMP	57.7	mV	-50 - 200
HVPS	670	V	550-800 constant
DCPS	2528	mV	2500 ± 200
RCELL TEMP	50.1	°C	50 ± 1
BOX TEMP	29.3	°C	5-40
PMT TEMP	7.4	°C	7 ± 2.0
SO ₂ Span Conc	400	PPB	20-20,000
SO ₂ Slope	1.010	-	1.0 ± 0.3
SO ₂ Offset	21.7	mV	<250
Stability at Zero	0.1	PPB	<0.2
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

SO₂ FLUORESCENT ANALYZER

DATE : 15 May 2023

BRAND : API

MODEL : 100E

NO. SO₂-R01

SERIAL NO. 3415

Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 04 August 2022

Serial No. : 911

Reference Standard Gas

Standard Gas : Sulphur Dioxide (SO₂)

Cylinder No. : A00814SK

Certified Date : 21 June 2021

Expired Date : 21 June 2029

Cylinder Conc. : 50.0 ppm

CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.5 °C

% RH 49

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.), PPB			Final Reading (After Adj.), PPB	
	Expected Concentration	Analyzer Response	% Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
SO ₂ Span	400.0	400.2	0.050	400.0	1.011

API Model 100E SO₂ Analyzer Check list

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	0-500
SAMPLE PRESS	28.6	in-Hg	25-35
SAMPLE FLOW	658	cc/min	650 ± 10%
PMT	103.2	mV	-20-150 with Zero Air
UV LAMP	3028.7	mV	1000-4900
STR. LGT	61.9	PPB	<100
DRK PMT	63.4	mV	-50 - 200
DRK LMP	58.2	mV	-50 - 200
HVPS	674	V	550-900 constant
DCPS	2523	mV	2500 ± 200
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.1	°C	5-40
PMT TEMP	7.2	°C	7 ± 2.0
SO ₂ Span Conc	400	PPB	20-20,000
SO ₂ Slope	1,011	-	1.0 ± 0.3
SO ₂ Offset	21.8	mV	<250
Stability at Zero	0.1	PPB	<0.2
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO₂ / NO_x ANALYZER

DATE : 6 February 2023

BRAND : API

MODEL : 200E

NO. NOX-R01

SERIAL NO. 769

Calibrator (Dilution System)

Brand : API Model : 700
Last Cal. Date : 04 August 2022 Serial No. : 911

Reference Standard Gas

Standard Gas : Nitric Oxide (NO) Cylinder No. : D636192
Certified Date : 20 April 2022 Expired Date : 20 April 2024 Cylinder Conc. : 49.1 ppm

CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.5 °C % RH 49

CALIBRATION SETTING

Span	Initial Reading (Before Adj.), PPB			Final Reading (After Adj.), PPB	
Set Point	Expected Concentration	Analyzer Response	% Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.8	-0.050	400.0	1.004
NO _x Span	400	400.1	0.025	400.0	1.008

API Model 200E NO_x Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	504	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	103.3	mV	-20 - 150
AZERO	94.1	mV	-20 - 150
HVPS	672	V	420 - 900 constant
RCELL TEMP	50.0	°C	50 ± 1
BOX TEMP	29.1	°C	8 - 48
PMT TEMP	7.3	°C	7 ± 2
MOLY TEMP	315.2	°C	315 ± 5
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO _x Span Conc	400	PPB	20 - 20,000
NO Slope	1.004	-	1.0 ± 0.3
NO _x Slope	1.008	-	1.0 ± 0.3
NO Offset	1.1	mV	-20 to +150
NO _x Offset	0.7	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO₂ / NO_x ANALYZER

DATE : 15 May 2023

BRAND : API

MODEL : TML-41M

NO. NOX-B18

SERIAL NO. N07543

Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 04 August 2022

Serial No. : 911

Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : D636192

Certified Date : 20 April 2022

Expired Date : 20 April 2024

Cylinder Conc. : 49.1 ppm

CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.5 °C

% RH 49

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	399.7	-0.075	400.0	1.004
NO _x Span	400	400.2	0.050	400.0	1.008

API Model TML-41M NO_x Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	506	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	103.2	mV	-20 - 150
AZERO	93.9	mV	-20 - 150
HVPS	671	V	420 - 900 constant
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.2	°C	8 - 48
PMT TEMP	7.5	°C	7 ± 2
MOLY TEMP	315.4	°C	315 ± 5
RCELL PRESS	8.5	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.7	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO _x Span Conc	400	PPB	20 - 20,000
NO Slope	1.004	-	1.0 ± 0.3
NO _x Slope	1.008	-	1.0 ± 0.3
NO Offset	1.2	mV	-20 to +150
NO _x Offset	0.8	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com... www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R01	SKC	224-PCXR4	602467	03/01/2023	1,000	1,500	2,000	993	1,508	2,004	1.008x - 13.936	0.999
R02	SKC	224-PCXR4	626450	06/01/2023	1,000	2,000	3,000	998	1,499	1,990	0.989x + 12.268	1.000
R03	SKC	224-PCXR4	691592	06/01/2023	1,000	1,500	2,000	1,003	1,500	2,004	1.011x - 21.761	0.999
R04	SKC	224-PCXR4	691672	06/01/2023	1,000	1,500	2,000	996	1,493	1,995	0.997x - 1.563	1.000
R05	SKC	224-PCXR4	798470	06/01/2023	1,000	1,500	2,000	993	1,505	1,999	1.014x - 31.752	0.999
R06	SKC	224-PCXR4	798456	06/01/2023	1,000	1,500	2,000	993	1,498	1,994	1.003x - 8.555	1.000
R07	SKC	224-PCXR4	798480	04/01/2023	1,000	1,500	2,000	994	1,490	1,999	1.007x - 16.073	1.000
R08	SKC	224-PCXR4	883215	04/01/2023	1,000	1,500	2,000	1,011	1,501	2,005	0.999x + 3.207	1.000
R09	SKC	224-PCXR4	034650	04/01/2023	1,000	1,500	2,000	991	1,504	2,002	1.018x - 35.900	0.999
R10	SKC	224-PCXR4	091765	04/01/2023	1,000	1,500	2,000	997	1,512	1,994	0.999x + 0.977	1.000
R11	SKC	224-PCXR4	091763	03/01/2023	1,000	1,500	2,000	1,000	1,499	2,002	1.013x - 25.119	0.999
R12	SKC	224-PCXR4	091568	03/01/2023	1,000	1,500	2,000	997	1,501	1,999	1.001x - 4.906	1.000
R13	SKC	224-PCXR4	091638	03/01/2023	1,000	1,500	2,000	1,002	1,499	1,994	0.992x + 9.636	1.000
R14	SKC	224-PCXR4	091764	03/01/2023	1,000	1,500	2,000	994	1,502	1,999	1.014x - 30.212	0.999
R15	SKC	224-PCXR8	529457	03/01/2023	1,000	1,500	2,000	1,001	1,500	2,004	1.006x - 11.941	1.000
R16	SKC	224-PCXR8	529643	05/01/2023	1,000	1,500	2,000	998	1,497	1,994	1.000x - 4.686	1.000
R17	SKC	224-PCXR8	529645	05/01/2023	1,000	1,500	2,000	994	1,509	2,000	1.015x - 30.731	0.999
R18	SKC	224-PCXR8	566756	05/01/2023	1,000	1,500	2,000	991	1,498	1,998	1.001x - 6.840	1.000
R19	SKC	224-PCXR8	566802	05/01/2023	1,000	1,500	2,000	1,002	1,499	2,000	1.010x - 21.027	0.999
R20	SKC	224-PCXR8	529089	03/01/2023	1,000	1,500	2,000	991	1,501	2,003	1.020x - 39.916	0.999
R21	SKC	224-PCXR8	665728	03/01/2023	1,000	1,500	2,000	998	1,493	1,999	1.000x - 5.404	1.000
R22	SKC	224-PCXR8	707444	03/01/2023	1,000	1,500	2,000	1,002	1,500	2,002	1.004x - 7.135	1.000
R23	SKC	224-PCXR8	761067	03/01/2023	1,000	1,500	2,000	998	1,494	1,991	0.993x + 4.132	1.000
R24	SKC	224-PCXR8	707893	04/01/2023	1,000	1,500	2,000	996	1,505	2,000	1.008x - 17.553	0.999
R25	SKC	224-PCXR8	761052	04/01/2023	1,000	1,500	2,000	1,010	1,499	1,993	0.984x + 23.464	1.000
R26	SKC	224-PCXR8	707956	04/01/2023	1,000	1,500	2,000	1,002	1,500	2,004	1.009x - 15.842	1.000
R27	SKC	224-PCXR8	707398	04/01/2023	1,000	1,500	2,000	996	1,503	2,001	1.005x - 13.449	1.000
R28	SKC	224-PCXR8	707461	04/01/2023	1,000	1,500	2,000	1,004	1,500	2,002	1.010x - 19.288	0.999
R29	SKC	224-PCXR8	707402	03/01/2023	1,000	1,500	2,000	1,004	1,493	1,991	0.988x + 14.167	1.000
R30	SKC	224-PCXR8	093811	03/01/2023	1,000	1,500	2,000	1,000	1,495	1,994	0.996x + 1.922	1.000
R31	SKC	224-PCXR8	093183	03/01/2023	1,000	1,500	2,000	1,001	1,501	2,001	1.002x - 3.618	1.000
R32	SKC	224-PCXR8	671950	03/01/2023	1,000	1,500	2,000	998	1,498	1,994	0.995x + 4.970	1.000
R33	SKC	224-PCXR4	626254	03/01/2023	1,000	1,500	2,000	995	1,502	1,999	1.014x - 31.070	0.999
R34	SKC	224-PCXR4	626131	03/01/2023	1,000	1,500	2,000	1,002	1,498	2,004	1.006x - 11.810	1.000
R35	SKC	224-PCXR8	707460	03/01/2023	1,000	1,500	2,000	999	1,498	1,995	0.994x + 6.669	1.000
R36	SKC	224-PCXR8	707446	03/01/2023	1,000	1,500	2,000	1,004	1,499	2,001	1.009x - 18.036	0.999
R37	SKC	224-PCXR8	707432	03/01/2023	1,000	1,500	2,000	996	1,499	1,998	1.000x - 2.070	1.000
R38	SKC	224-PCXR8	707349	03/01/2023	1,000	1,500	2,000	996	1,500	2,001	1.004x - 9.345	1.000
R39	SKC	224-PCXR8	761095	03/01/2023	1,000	1,500	2,000	1,001	1,496	1,994	0.997x + 2.373	1.000



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscn.com.. www.spscn.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}\text{C}$
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R01	SKC	224-PCXR4	602467	10/04/2023	1,000	1,500	2,000	992	1,507	2,005	1.009x - 15.491	1.000
R02	SKC	224-PCXR4	626450	10/04/2023	1,000	2,000	3,000	997	1,497	1,989	0.990x + 10.155	1.000
R03	SKC	224-PCXR4	691592	10/04/2023	1,000	1,500	2,000	1,005	1,498	2,003	1.010x - 19.567	0.999
R04	SKC	224-PCXR4	691672	04/04/2023	1,000	1,500	2,000	998	1,491	1,997	0.998x - 1.962	1.000
R05	SKC	224-PCXR4	798470	10/04/2023	1,000	1,500	2,000	994	1,506	1,998	1.012x - 28.038	0.999
R06	SKC	224-PCXR4	798456	05/04/2023	1,000	1,500	2,000	993	1,497	1,995	1.004x - 10.749	1.000
R07	SKC	224-PCXR4	798480	10/04/2023	1,000	1,500	2,000	996	1,492	1,998	1.005x - 11.766	1.000
R08	SKC	224-PCXR4	883215	10/04/2023	1,000	1,500	2,000	1,010	1,503	2,003	0.988x + 3.526	1.000
R09	SKC	224-PCXR4	034650	04/04/2023	1,000	1,500	2,000	994	1,505	2,003	1.017x - 33.985	0.999
R10	SKC	224-PCXR4	091765	07/04/2023	1,000	1,500	2,000	998	1,492	1,996	1.000x - 3.929	1.000
R11	SKC	224-PCXR4	091763	04/04/2023	1,000	1,500	2,000	1,002	1,497	2,003	1.012x - 23.883	0.999
R12	SKC	224-PCXR4	091568	10/04/2023	1,000	1,500	2,000	995	1,503	1,998	1.002x - 7.698	1.000
R13	SKC	224-PCXR4	091638	10/04/2023	1,000	1,500	2,000	1,005	1,497	1,993	0.989x + 13.679	1.000
R14	SKC	224-PCXR4	091764	10/04/2023	1,000	1,500	2,000	992	1,503	1,998	1.015x - 32.167	0.999
R15	SKC	224-PCXR8	529457	10/04/2023	1,000	1,500	2,000	1,003	1,501	2,005	1.005x - 9.429	1.000
R16	SKC	224-PCXR8	529643	04/04/2023	1,000	1,500	2,000	999	1,496	1,995	0.999x - 3.290	1.000
R17	SKC	224-PCXR8	529645	05/04/2023	1,000	1,500	2,000	995	1,511	2,001	1.012x - 23.233	0.999
R18	SKC	224-PCXR8	566756	07/04/2023	1,000	1,500	2,000	992	1,497	1,999	1.002x - 7.359	1.000
R19	SKC	224-PCXR8	566802	07/04/2023	1,000	1,500	2,000	1,002	1,498	1,999	1.009x - 19.671	0.999
R20	SKC	224-PCXR8	529089	07/04/2023	1,000	1,500	2,000	992	1,501	2,004	1.015x - 28.270	1.000
R21	SKC	224-PCXR8	665728	10/04/2023	1,000	1,500	2,000	997	1,494	1,997	1.001x - 7.797	1.000
R22	SKC	224-PCXR8	707444	05/04/2023	1,000	1,500	2,000	1,003	1,501	2,003	1.003x - 6.218	1.000
R23	SKC	224-PCXR8	761067	10/04/2023	1,000	1,500	2,000	996	1,495	1,993	0.995x + 0.263	1.000
R24	SKC	224-PCXR8	707893	10/04/2023	1,000	1,500	2,000	997	1,506	2,002	1.009x - 17.713	0.999
R25	SKC	224-PCXR8	761052	10/04/2023	1,000	1,500	2,000	1,009	1,497	1,992	0.983x + 22.945	1.000
R26	SKC	224-PCXR8	707956	10/04/2023	1,000	1,500	2,000	1,004	1,502	2,005	1.008x - 14.326	0.999
R27	SKC	224-PCXR8	707398	07/04/2023	1,000	1,500	2,000	995	1,502	2,002	1.007x - 16.361	1.000
R28	SKC	224-PCXR8	707481	10/04/2023	1,000	1,500	2,000	1,006	1,501	2,003	1.009x - 18.291	0.999
R29	SKC	224-PCXR8	707402	07/04/2023	1,000	1,500	2,000	1,002	1,494	1,989	0.987x + 14.566	1.000
R30	SKC	224-PCXR8	093811	04/04/2023	1,000	1,500	2,000	1,001	1,494	1,996	0.997x + 0.646	1.000
R31	SKC	224-PCXR8	093183	10/04/2023	1,000	1,500	2,000	1,001	1,502	2,004	1.004x - 5.652	1.000
R32	SKC	224-PCXR8	671950	05/04/2023	1,000	1,500	2,000	999	1,501	1,993	0.994x + 7.163	1.000
R33	SKC	224-PCXR4	626254	10/04/2023	1,000	1,500	2,000	996	1,504	2,001	1.015x - 30.192	0.999
R34	SKC	224-PCXR4	626131	04/04/2023	1,000	1,500	2,000	1,003	1,498	2,004	1.004x - 9.377	1.000
R35	SKC	224-PCXR8	707460	10/04/2023	1,000	1,500	2,000	998	1,496	1,996	0.996x + 3.677	1.000
R36	SKC	224-PCXR8	707446	10/04/2023	1,000	1,500	2,000	1,003	1,498	2,002	1.010x - 20.668	0.999
R37	SKC	224-PCXR8	707432	10/04/2023	1,000	1,500	2,000	998	1,496	2,000	0.999x - 0.873	1.000
R38	SKC	224-PCXR8	707349	07/04/2023	1,000	1,500	2,000	997	1,497	2,001	1.003x - 8.747	1.000
R39	SKC	224-PCXR8	761095	10/04/2023	1,000	1,500	2,000	1,001	1,497	1,997	0.999x + 0.140	1.000



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-R01	Dwyer	VFA-21	04/01/2023	50	100	200	50.6	100.6	203.9	0.982x + 2.803	1.000
L-R02	Dwyer	VFA-21	04/01/2023	50	100	200	49.7	101.3	200.1	1.008x - 1.204	0.999
L-R03	Dwyer	VFA-21	04/01/2023	50	100	200	50.5	99.8	202.3	1.017x - 0.913	1.000
L-R04	Dwyer	VFA-21	03/01/2023	50	100	200	49.8	100.5	201.0	1.010x - 1.439	0.999
L-R05	Dwyer	VFA-21	03/01/2023	50	100	200	50.6	100.0	203.4	0.991x + 1.807	1.000
L-R06	Dwyer	VFA-21	03/01/2023	50	100	200	50.6	99.1	201.9	1.003x - 0.031	1.000



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-R01	Dwyer	VFA-21	05/04/2023	50	100	200	50.2	101.0	204.3	0.981x + 2.956	0.999
L-R02	Dwyer	VFA-21	10/04/2023	50	100	200	50.1	102.0	201.0	1.007x - 0.506	0.999
L-R03	Dwyer	VFA-21	07/04/2023	50	100	200	50.1	100.2	202.7	1.015x - 0.825	1.000
L-R04	Dwyer	VFA-21	10/04/2023	50	100	200	50.2	100.9	200.6	1.005x - 0.751	0.999
L-R05	Dwyer	VFA-21	05/04/2023	50	100	200	50.2	101.0	202.6	0.994x + 1.409	1.000
L-R06	Dwyer	VFA-21	10/04/2023	50	100	200	50.8	100.2	202.3	1.001x + 0.717	1.000

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 22M2567

REFERENCE No : 64386-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS 105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : TETNITHI W.

CALIBRATION DATE : 11-Mar-22

APPROVED BY : 

ISSUED DATE : 17-Mar-22

RECEIVED DATE : 11-Mar-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 22M2567

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS 105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 11-Mar-22
AIR PRESSURE : 1008mbar \pm 1mbar CALIBRATION DATE : 11-Mar-22
AMBIENT TEMPERATURE : 22° C \pm 1° C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL


3. REPEATABILITY OF READING AT 20 g WAS 0.000004 g

4. REPEATABILITY OF READING AT 100 g WAS 0.000048 g

5. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000058
0.02	0.01999	0.00001	0.000058
0.10	0.09999	0.00001	0.000059
0.20	0.19999	0.00001	0.000059
0.50	0.50001	-0.00001	0.000058
1.00	1.00001	-0.00001	0.000059
2.00	2.00000	0.00000	0.000059
5.00	5.00001	-0.00001	0.000061
10.00	10.00005	-0.00005	0.000063
20.00	20.00006	-0.00006	0.000069
50.00	50.00000	0.00000	0.00011
100.00	100.00001	-0.00001	0.00019
120.00	120.00001	-0.00001	0.00022

6. OFF CENTER LOADING ERROR



POINT	READING (g)	
1	10.00001	50.0000
2	10.00002	50.0000
3	10.00001	50.0000
4	10.00001	50.0000
5	10.00002	50.00001
OFF-CENTER LOADING	0.00001	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT PRODUCTION AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%

END OF CALIBRATION REPORT



CERTIFICATE No : 23M2441

REFERENCE No : 68471-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY : 

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23



CERTIFICATE No : 23M2441

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
ID No : BA 05/50
AIR PRESSURE : 1010mbar \pm 1mbar
AMBIENT TEMPERATURE : 23° C \pm 1° C
MODEL : XS105DU
S/N : 1126422905
RECEIVED DATE : 10-Mar-23
CALIBRATION DATE : 10-Mar-23
RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

CALIBRATION REPORT			
Total Hydrocarbon Analyzer			
DATE :	6 February 2023	BRAND :	HORIBA
MODEL :	APHA-370		
NO.	THC-R02	SERIAL NO.	6F3AC3V4
Calibrator (Dilution System)			
Brand :	API	Model :	700
Last Cal. Date :	06 September 2022	Serial No.	421
Reference Standard Gas			
Standard Gas :	Methane (CH ₄)	Cylinder No.	D59075
Certified Date :	17 March 2015	Expired Date :	17 March 2023
		Cylinder Conc.	456 ppm
Calibrating Condition			
Pressure	1011	mmbar	Temp. 24.5 °C
		% RH	49
		Start Time :	1:00 PM
Pre-Calibration Checks			
Change Particulate Filter	YES	Station Temp :	25.0 °C
Leak Test	YES		
Calibration Setting			
Span Set Point	Initial Reading (Before Adj)		Final Reading (After Adj)
	Expected Concentration (PPM)	Analyzer Response (PPM)	Analyzer Response (PPM)
Zero	0	0.10	0
Span	10	10.05	10
Calibration Setting (Final)			
Span Instrument Gain:	0.997	Finish Time:	2:00 PM
APHA-370 Total Hydrocarbon Analyzer			
Test Values	Observed Value	Units	Nominal Range
SIGNAL (CH ₄)	911.3	mV	800-1,350
SIGNAL (THC)	916.4	mV	800-1,350
DETECTOR	77.9	kPa	((Pressure air/1013)x100)-20 ± 4 kPa
PURIFIER	19.1	kPa	8 - 25
NMC	258.9	°C	260 ± 10
BYPATH	0.9	L / min	0.9 ± 0.3
OVER FLOW	0.8	L / min	0.8



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

CALIBRATION REPORT

Total Hydrocarbon Analyzer

DATE : 15 May 2023

BRAND : HORIBA

MODEL : APHA-370

NO. THC-R02

SERIAL NO. 6F3AC3V4

Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 06 September 2022

Serial No. 421

Reference Standard Gas

Standard Gas : Methane (CH₄)

Cylinder No. : D59075

Certified Date : 17 March 2015

Expired Date : 17 March 2023

Cylinder Conc. : 456 ppm

Calibrating Condition

Pressure 1011 mmbar

Temp. 24.5 °C

% RH 49

Start Time : 1:00 PM

Pre-Calibration Checks

Change Particulate Filter YES

Station Temp : 25.0 °C

Leak Test YES

Calibration Setting

Span Set Point	Initial Reading (Before Adj)		Final Reading (After Adj)
	Expected Concentration (PPM)	Analyzer Response (PPM)	Analyzer Response (PPM)
Zero	0	0.10	0
Span	10	10.04	10

Calibration Setting (Final)

Span Instrument Gain: 0.997

Finish Time: 2:00 PM

APHA-370 Total Hydrocarbon Analyzer

Test Values	Observed Value	Units	Nominal Range
SIGNAL (CH ₄)	910.2	mV	800-1,350
SIGNAL (THC)	915.2	mV	800-1,350
DETECTOR	77.9	kPa	((Pressure air/1013)x100)-20 ± 4 kPa
PURIFIER	18.9	kPa	8 - 25
NMC	259.2	°C	260 ± 10
BYPATH	0.9	L / min	0.9 ± 0.3
OVER FLOW	0.8	L / min	0.8



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	DH _@ (mmH ₂ O)
B01	1563	02/03/2023	0.998	50.11
B02	8002514	03/03/2023	1.004	49.25
B03	1503016	03/03/2023	1.002	50.62
B04	00006659	02/03/2023	1.004	50.14
B05	00007428	03/03/2023	1.001	49.76
R01	1561	01/03/2023	0.997	49.86
R02	8002513	03/03/2023	0.996	49.93
R03	1570	02/03/2023	1.003	49.57
R04	8002519	01/03/2023	1.002	48.90
R05	1503015	01/03/2023	0.998	50.20

Remark : Accept Value of y (test) is $0.97 < y < 1.03$

Accept Value of $\Delta H_{@}$ (test) is 46.7 ± 6.4 (mmH₂O)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	02/05/2023	0.84	0.84
B37	S	0.99	02/05/2023	0.83	0.84
B38	S	0.99	03/05/2023	0.85	0.84
B39	S	0.99	03/05/2023	0.84	0.83
B40	S	0.99	02/05/2023	0.84	0.83
B41	S	0.99	02/05/2023	0.84	0.84
B44	S	0.99	03/05/2023	0.85	0.84
B45	S	0.99	03/05/2023	0.85	0.84
B46	S	0.99	04/05/2023	0.84	0.83
B47	S	0.99	03/05/2023	0.84	0.85
B48	S	0.99	03/05/2023	0.83	0.84
B49	S	0.99	03/05/2023	0.85	0.84
B54	S	0.99	03/05/2023	0.83	0.84
B56	S	0.99	02/05/2023	0.84	0.85
B57	S	0.99	02/05/2023	0.84	0.83
B58	S	0.99	02/05/2023	0.85	0.84

Remark : Accept value of Cp (test) is 0.84 ± 0.01

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VACUUM GAUGE
MANUFACTURER : HI-LIGHT
MODEL / TYPE : N/A
SERIAL NO. : N/A[64-220066-3]
CLID. NO. : 212201114
JOB CONTROL NO. : 220720073203

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 20 July 2022

DATE OF ISSUED : 22 July 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By :



Authorized Signatory
22 July 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22073203

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : VACUUM GAUGE
MANUFACTURER : HI-LIGHT
MODEL / TYPE : N/A
SERIAL NO. : N/A[64-220066-3]
DATE OF CALIBRATION : 21 July 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-05** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 744 S/N. 9226007 with Pressure Module Model 700PV4 S/N. 19298401.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. MP-0196-21, Due Date 17 November 2022.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q22073203

F3-011-04/01-12

page 2 of 3



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (inHg)	STD Reading (inHg)		Correction (inHg)	
	Up	Down	Up	Down
0	0.0	0.0	0.0	0.0
-5	-4.8	-4.9	+0.2	+0.1
-10	-9.9	-9.9	+0.1	+0.1
-15	-15.0	-15.0	0.0	0.0
-20	-20.0	-20.0	0.0	0.0
-25	-25.0	-25.0	0.0	0.0
-30	-29.9	-29.9	+0.1	+0.1

Uncertainty of measurement ± 0.2 inHg

Transmitting fluid : Air.

Technical Note. k factor 1 kPa = 0.2952998 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 36 of 54

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22073203

F3-011-04/01-12

page 3 of 3



@clccalibration



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}\text{C}$
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B41	SKC	224-PCXR4	612669	07/04/2023	1,000	1,500	2,000	997	1,496	1,991	0.998x - 1.396	1.000
B42	SKC	224-PCXR4	626041	10/04/2023	1,000	1,500	2,000	1,006	1,496	1,992	0.988x + 14.223	1.000
B43	SKC	224-PCXR4	034636	07/04/2023	1,000	1,500	2,000	1,001	1,503	1,993	0.992x + 8.810	1.000
B44	SKC	224-PCXR8	529341	10/04/2023	1,000	1,500	2,000	1,000	1,499	2,005	1.008x - 14.358	1.000
B45	SKC	224-PCXR8	529594	10/04/2023	1,000	1,500	2,000	998	1,506	1,987	0.990x + 12.580	1.000
B46	SKC	224-PCXR8	566743	05/04/2023	1,000	1,500	2,000	996	1,502	2,000	1.012x - 26.902	0.999
B47	SKC	224-PCXR8	566747	07/04/2023	1,000	1,500	2,000	998	1,501	2,002	1.014x - 27.552	0.999
B48	SKC	224-PCXR8	566753	10/04/2023	1,000	1,500	2,000	998	1,493	1,996	0.997x - 0.359	1.000
B49	SKC	224-PCXR8	566780	05/04/2023	1,000	1,500	2,000	1,007	1,501	2,007	1.011x - 19.156	0.999
B50	SKC	224-PCXR8	500400	07/04/2023	1,000	1,500	2,000	1,004	1,495	2,004	1.000x - 1.663	1.000
B51	SKC	224-PCXR8	500363	04/04/2023	1,000	1,500	2,000	997	1,502	1,998	1.008x - 21.322	0.999
B52	SKC	224-PCXR8	093186	05/04/2023	1,000	1,500	2,000	993	1,493	1,995	1.000x - 6.106	1.000
B53	SKC	224-PCXR8	707670	05/04/2023	1,000	1,500	2,000	1,000	1,498	2,002	1.009x - 18.883	0.999
B54	SKC	224-PCXR3	509821	05/04/2023	1,000	1,500	2,000	995	1,500	2,001	1.016x - 32.482	0.999
B55	SKC	224-PCXR3	510710	10/04/2023	1,000	1,500	2,000	998	1,497	1,992	0.996x - 0.191	1.000
B56	SKC	224-PCXR3	511450	05/04/2023	1,000	1,500	2,000	1,003	1,501	2,003	1.005x - 8.081	1.000
B57	SKC	224-PCXR3	510798	05/04/2023	1,000	1,500	2,000	999	1,490	2,000	1.001x - 2.920	1.000
B58	SKC	224-PCXR3	509852	10/04/2023	1,000	1,500	2,000	1,002	1,496	1,998	1.004x - 15.922	0.999
B59	SKC	224-PCXR3	509862	10/04/2023	1,000	1,500	2,000	998	1,501	1,996	0.996x + 4.471	1.000
B60	SKC	224-PCXR3	512655	07/04/2023	1,000	1,500	2,000	1,003	1,499	2,004	1.005x - 9.971	1.000
B61	SKC	224-PCXR3	503915	10/04/2023	1,000	1,500	2,000	993	1,488	1,999	1.007x - 15.934	1.000
B62	SKC	224-PCXR3	505975	10/04/2023	1,000	1,500	2,000	1,001	1,495	1,997	1.000x - 4.802	1.000
B63	SKC	224-PCXR3	511432	07/04/2023	1,000	1,500	2,000	993	1,500	2,000	1.015x - 32.709	0.999
B64	SKC	224-PCXR3	508302	05/04/2023	1,000	1,500	2,000	998	1,491	1,987	0.989x + 9.855	1.000
B65	SKC	224-PCXR3	508310	10/04/2023	1,000	1,500	2,000	998	1,502	2,005	1.012x - 20.596	1.000
B66	SKC	224-PCXR3	509861	10/04/2023	1,000	1,500	2,000	1,000	1,492	1,992	0.990x + 10.912	1.000
B67	SKC	224-PCXR3	506295	07/04/2023	1,000	1,500	2,000	993	1,506	2,002	1.007x - 13.999	1.000
B68	SKC	224-PCXR3	505872	05/04/2023	1,000	1,500	2,000	998	1,488	1,997	0.998x - 1.743	1.000
B69	SKC	224-PCXR3	508375	04/04/2023	1,000	1,500	2,000	1,004	1,502	2,002	1.009x - 18.897	0.999
B70	SKC	224-PCXR3	510623	05/04/2023	1,000	1,500	2,000	994	1,505	1,998	1.004x - 8.846	1.000
B71	SKC	224-PCXR3	508367	10/04/2023	1,000	1,500	2,000	994	1,503	2,003	1.011x - 23.544	0.999
B72	SKC	224-PCXR3	505977	10/04/2023	1,000	1,500	2,000	1,005	1,493	1,992	0.988x + 13.309	1.000
B73	SKC	224-PCXR3	512606	05/04/2023	1,000	1,500	2,000	1,000	1,504	2,004	1.008x - 14.506	1.000
B74	SKC	224-PCXR3	505993	05/04/2023	1,000	1,500	2,000	997	1,497	1,996	1.001x - 7.514	1.000
B75	SKC	224-PCXR3	509820	07/04/2023	1,000	1,500	2,000	997	1,496	1,992	0.997x + 0.195	1.000
B76	SKC	224-PCXR3	509811	05/04/2023	1,000	1,500	2,000	995	1,498	1,999	1.004x - 11.212	1.000
B77	SKC	224-PCXR3	508301	10/04/2023	1,000	1,500	2,000	1,003	1,502	2,004	1.013x - 23.811	0.999
B78	SKC	224-PCXR3	510677	04/04/2023	1,000	1,500	2,000	997	1,505	2,000	1.007x - 16.113	0.999
B79	SKC	224-PCXR3	510920	10/04/2023	1,000	1,500	2,000	996	1,495	1,993	0.998x - 1.232	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}\text{C}$
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R01	SKC	224-PCXR4	602467	10/04/2023	1,000	1,500	2,000	992	1,507	2,005	1.009x - 15.491	1.000
R02	SKC	224-PCXR4	626450	10/04/2023	1,000	2,000	3,000	997	1,497	1,989	0.990x + 10.155	1.000
R03	SKC	224-PCXR4	691592	10/04/2023	1,000	1,500	2,000	1,005	1,498	2,003	1.010x - 19.567	0.999
R04	SKC	224-PCXR4	691672	04/04/2023	1,000	1,500	2,000	998	1,491	1,997	0.998x - 1.962	1.000
R05	SKC	224-PCXR4	798470	10/04/2023	1,000	1,500	2,000	994	1,506	1,998	1.012x - 28.038	0.999
R06	SKC	224-PCXR4	798456	05/04/2023	1,000	1,500	2,000	993	1,497	1,995	1.004x - 10.749	1.000
R07	SKC	224-PCXR4	798480	10/04/2023	1,000	1,500	2,000	996	1,492	1,998	1.005x - 11.766	1.000
R08	SKC	224-PCXR4	883215	10/04/2023	1,000	1,500	2,000	1,010	1,503	2,003	0.998x + 3.526	1.000
R09	SKC	224-PCXR4	034650	04/04/2023	1,000	1,500	2,000	994	1,505	2,003	1.017x - 33.985	0.999
R10	SKC	224-PCXR4	091765	07/04/2023	1,000	1,500	2,000	998	1,492	1,996	1.000x - 3.929	1.000
R11	SKC	224-PCXR4	091763	04/04/2023	1,000	1,500	2,000	1,002	1,497	2,003	1.012x - 23.883	0.999
R12	SKC	224-PCXR4	091568	10/04/2023	1,000	1,500	2,000	995	1,503	1,998	1.002x - 7.698	1.000
R13	SKC	224-PCXR4	091638	10/04/2023	1,000	1,500	2,000	1,005	1,497	1,993	0.989x + 13.679	1.000
R14	SKC	224-PCXR4	091764	10/04/2023	1,000	1,500	2,000	992	1,503	1,998	1.015x - 32.167	0.999
R15	SKC	224-PCXR8	529457	10/04/2023	1,000	1,500	2,000	1,003	1,501	2,005	1.005x - 9.429	1.000
R16	SKC	224-PCXR8	529643	04/04/2023	1,000	1,500	2,000	999	1,496	1,995	0.999x - 3.290	1.000
R17	SKC	224-PCXR8	529645	05/04/2023	1,000	1,500	2,000	995	1,511	2,001	1.012x - 23.233	0.999
R18	SKC	224-PCXR8	566756	07/04/2023	1,000	1,500	2,000	992	1,497	1,999	1.002x - 7.359	1.000
R19	SKC	224-PCXR8	566802	07/04/2023	1,000	1,500	2,000	1,002	1,498	1,999	1.009x - 19.671	0.999
R20	SKC	224-PCXR8	529089	07/04/2023	1,000	1,500	2,000	992	1,501	2,004	1.015x - 28.270	1.000
R21	SKC	224-PCXR8	665728	10/04/2023	1,000	1,500	2,000	997	1,494	1,997	1.001x - 7.797	1.000
R22	SKC	224-PCXR8	707444	05/04/2023	1,000	1,500	2,000	1,003	1,501	2,003	1.003x - 6.218	1.000
R23	SKC	224-PCXR8	761067	10/04/2023	1,000	1,500	2,000	996	1,495	1,993	0.995x + 0.263	1.000
R24	SKC	224-PCXR8	707893	10/04/2023	1,000	1,500	2,000	997	1,506	2,002	1.009x - 17.713	0.999
R25	SKC	224-PCXR8	761052	10/04/2023	1,000	1,500	2,000	1,009	1,497	1,992	0.983x + 22.945	1.000
R26	SKC	224-PCXR8	707956	10/04/2023	1,000	1,500	2,000	1,004	1,502	2,005	1.008x - 14.326	0.999
R27	SKC	224-PCXR8	707398	07/04/2023	1,000	1,500	2,000	995	1,502	2,002	1.007x - 16.361	1.000
R28	SKC	224-PCXR8	707481	10/04/2023	1,000	1,500	2,000	1,006	1,501	2,003	1.009x - 18.291	0.999
R29	SKC	224-PCXR8	707402	07/04/2023	1,000	1,500	2,000	1,002	1,494	1,989	0.987x + 14.566	1.000
R30	SKC	224-PCXR8	093811	04/04/2023	1,000	1,500	2,000	1,001	1,494	1,996	0.997x + 0.646	1.000
R31	SKC	224-PCXR8	093183	10/04/2023	1,000	1,500	2,000	1,001	1,502	2,004	1.004x - 5.652	1.000
R32	SKC	224-PCXR8	671950	05/04/2023	1,000	1,500	2,000	999	1,501	1,993	0.994x + 7.163	1.000
R33	SKC	224-PCXR4	626254	10/04/2023	1,000	1,500	2,000	996	1,504	2,001	1.015x - 30.192	0.999
R34	SKC	224-PCXR4	626131	04/04/2023	1,000	1,500	2,000	1,003	1,498	2,004	1.004x - 9.377	1.000
R35	SKC	224-PCXR8	707460	10/04/2023	1,000	1,500	2,000	998	1,496	1,996	0.996x + 3.677	1.000
R36	SKC	224-PCXR8	707446	10/04/2023	1,000	1,500	2,000	1,003	1,498	2,002	1.010x - 20.668	0.999
R37	SKC	224-PCXR8	707432	10/04/2023	1,000	1,500	2,000	998	1,496	2,000	0.999x - 0.873	1.000
R38	SKC	224-PCXR8	707349	07/04/2023	1,000	1,500	2,000	997	1,497	2,001	1.003x - 8.747	1.000
R39	SKC	224-PCXR8	761095	10/04/2023	1,000	1,500	2,000	1,001	1,497	1,997	0.999x + 0.140	1.000



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
 Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R²
H-R01	Dwyer	VFB-65	05/04/2023	500	1,000	2,000	502.1	993.6	1981.1	1.000x - 3.647	0.999
H-R02	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	500.4	998.7	1988.7	1.001x - 3.457	1.000
H-R03	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	502.1	990.3	1997.7	0.993x + 4.022	1.000
H-R04	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	497.2	992.2	2016.9	1.007x - 11.203	1.000
H-R05	Dwyer	VFB-65	05/04/2023	500	1,000	2,000	499.2	988.5	1990.7	1.003x - 7.136	1.000
H-R06	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	504.8	994.6	1982.6	0.999x - 1.961	0.999



CERTIFICATE No : 23M2441
REFERENCE No : 68471-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY : 

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23



CERTIFICATE No : 23M2441

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23° C \pm 1° C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : SP22018

Pages 1 of 3

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY

Condition As Found : GOOD

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON, CHATUCHAK,
BANGKOK 10900, THAILAND.


Location : ORGANIC LABORATORY IV

Ambient Temperature : (24.4 ± 5) °C
Relative Humidity : (60.1 ± 25) %

Received Date : 30 AUGUST 2022
Calibration Date : 30 AUGUST 2022
Date of Issue : 31 AUGUST 2022

Calibrated by :

Approved by :

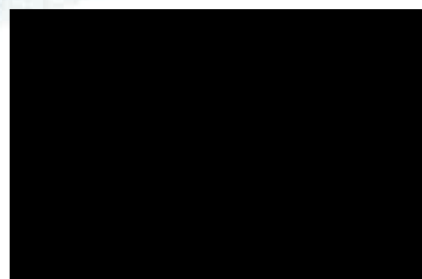

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : SP22018

Job No. : VC65SP0008

Pages : 2 of 3

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01,ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

<u>Material</u>	<u>Ref. type</u>	<u>Cell serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Holmium liquid	RM-HL	29706	87569	13/10/2022
Didymium liquid	RM-DL	28912	87588	15/10/2022
Neutral density filter	RM-1N2N3N	13877	87600	15/10/2022
Potassium dichromate solutions	RM-0204060810	14204	87614	16/10/2022
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology,NIST.

Result of calibration : Wavelength Accuracy

(Without adjustment)

<u>Material</u>	<u>Certified Values of Reference Material (nm)</u>	<u>UUC* Reading (nm)</u>	<u>Error (nm)</u>	<u>Uncertainty ± (nm)</u>	<u>k Factor</u>
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.4	0.15	0.16	2.00
	467.82	467.8	-0.02	0.16	2.00
	536.56	536.5	-0.06	0.16	2.00
	640.50	640.5	0.00	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.2	0.26	0.16	2.00

UUC* = Unit Under Calibration

Continuation of Calibration Certificate

Cert. No. : SP22018
Job No. : VC65SP0008
Pages : 3 of 3

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Filter: S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0524	1.0539	0.0015	0.0028	2.00
		29914	0.7	0.7454	0.7459	0.0005	0.0029	2.00
		29381	0.5	0.5426	0.5426	0.0000	0.0028	2.00
	546.1	29360	1.0	0.9822	0.9810	-0.0012	0.0028	2.00
		29914	0.7	0.6962	0.6960	-0.0002	0.0028	2.00
		29381	0.5	0.5076	0.5070	-0.0006	0.0029	2.00
	590.0	29360	1.0	1.0221	1.0202	-0.0019	0.0028	2.00
		29914	0.7	0.7238	0.7230	-0.0008	0.0029	2.00
		29381	0.5	0.5364	0.5360	-0.0004	0.0031	2.00
	635.0	29360	1.0	0.9751	0.9732	-0.0019	0.0028	2.00
		29914	0.7	0.6912	0.6902	-0.0010	0.0029	2.00
		29381	0.5	0.5214	0.5210	-0.0004	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2436	0.2419	-0.0017	0.0101	2.00	
		40	0.4905	0.4855	-0.0050	0.0115	2.00	
		60	0.7453	0.7388	-0.0065	0.0067	2.00	
		80	0.9920	0.9839	-0.0081	0.0071	2.00	
		100	1.2487	1.2414	-0.0073	0.0073	2.00	

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230

Resolution of Wavelength Mode 0.1 nm
Resolution of Photometric Mode 0.0001 A
Parameter Setting
Measurement Mode Wavelength, Absorbance
Wavelength Scan 1100 nm-190 nm
Scanning Speed 7.5 nm/min
Data Pitch 0.1 nm
Band width(Wavelength) 1.0 nm
Band width(Vis) 1.0 nm
Band width(Uv) 1.0 nm

Stray Light** UUC* Reading at 220 nm	
Transmission T(%)	Absorbance(A)
0.0107	3.9886

**Specific Acceptance :
Transmission \leq 1.0 T(%), Absorbance \geq 2.0 A
**Stray light not TISI Accredited


The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com


Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	02 May 2023	Brand :	API	Model :	300E
No.	CO-B02			Serial No.	965
Calibrator (Dilution System)					
Brand : API			Model : 700		
Last Cal. Date : 06 September 2022			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D196045		
Certified Date : 16 April 2022		Expired Date : 15 April 2024		Cylinder Conc. : 4,570 ppm	
Calibrating Condition					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response	% Dif	Analyzer Response	
Zero	0	-0.10	-	0	
CO Span	40.00	39.97	-0.075	40.00	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4017.1	mV	2500-4800 mV		
CO Reference	3949.4	mV	2500-4800 mV		
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.7	In-Hg-A	~2" < Ambient Absolute Pressure		
Sample Flow	812	CC/Min	800 ± 10%		
Sample Temperature	48.3	°C	48 ± 4		
Bench Temperature	48.1	°C	48 ± 2		
Wheel Temperature	68.2	°C	68 ± 2		
Box Temperature	30.6	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3023.8	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	03 May 2023	Brand :	API	Model :	300E
No.	CO-B03			Serial No.	3019
Calibrator (Dilution System)					
Brand : API			Model : 700		
Last Cal. Date : 06 September 2022			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D196045		
Certified Date : 16 April 2022		Expired Date : 15 April 2024		Cylinder Conc. : 4,570 ppm	
Calibrating Condition					
Pressure : 1011 mmbar		Temp. : 24.6 °C		% RH : 50	
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response		%Dif	
Zero	0	0.10		-	
CO Span	40.00	40.03		0.075	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4014.3	mV	2500-4800 mV		
CO Reference	3948.1	mV	2500-4800 mV		
Measure/Reference Ratio	1.179	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.5	In-Hg-A	-2" < Ambient Absolute Pressure		
Sample Flow	807	CC/Min	800 ± 10%		
Sample Temperature	48.5	°C	48 ± 4		
Bench Temperature	48.2	°C	48 ± 2		
Wheel Temperature	68.3	°C	68 ± 2		
Box Temperature	30.9	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3041.4	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		

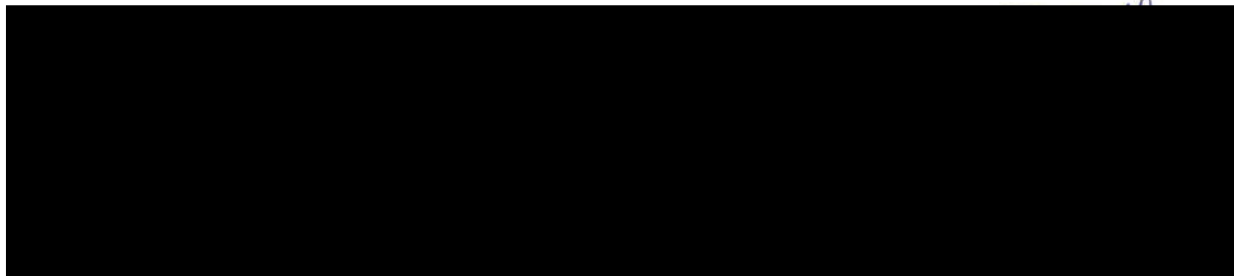



Certificate of Calibration

Aquion : Anion (ID#894)

This certificate is to verify that instrument below are calibrated
by Archemica Lab Co.,Ltd.

AQUION S/N : 190840059

AS-DV S/N : 190915235

for

S.P.S. Consulting Service Co., Ltd.



Operator Signature

Date : Jan 4, 2023

(N

Test Engineer

Certificate No.: CP20220335EA

Operation No.: CP2022100023

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: RION

Model/Type: NL-42 (Meter), UC-52 (Microphone), NH-24 (Preamplifier)

Serial No.: 00546401 (Meter), 152917 (Microphone), 46612 (Preamplifier)

ID No.: -

Customer: IRPC Public Company Limited.

Address: 299 Moo 5, Sukhumvit Rd., Tumbon Chungnern,
Amphor Muang, Rayong 21000

Received Date: 25 October 2022

Calibrated Date: 2 - 7 November 2022

Issued Date: 16 November 2022

Calibrated by: Ms. Juntaporn Kunhakom

Approved by

Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20220335EA

Calibration Report

Equipment: Sound Level Meter
 Manufacturer: RION
 Model/Type: NL-42 (Meter), UC-52 (Microphone), NH-24 (Preamplifier)
 Serial No.: 00546401 (Meter), 152917 (Microphone), 46612 (Preamplifier)
 ID No.: -
 Ambient Temperature: (23 ± 2) °C
 Relative Humidity: (50 ± 15) %
 Pressure: (101.3 ± 1.5) kPa
 Method of Calibration :-
 IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2661000	AA-1020-22	14 June 2023
2) Arbitrary Function Generator	AFG2021	C010063	CK20220059EA	19 June 2023
3) Programmable Attenuator	PA5	2913	EF-0014-22	3 April 2023
4) 6.5 Digit precision multimeter	8846A	9610014	CB20220223EA	14 November 2023
5) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P220024 CD20220164EA	17 March 2023 24 July 2023
6) Pressure humidity and Temperature Transmitter	PTU301	F0640003	CL1-P220029 CD20220165EA	31 March 2023 24 July 2023
7) Performance Audio Analyzer	U8903B	MY56510003	CB20220063EA CK20220080EA	15 February 2023 8 September 2023

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
94.1	94.1	0.0	±1.0

Note : Absolute sensitivity was established by the use of the Sound Calibrator RION Type NC-74 S/N : 34536113.

Certificate No.: CP20220335EA

Calibration Report

Equipment: Sound Level Meter
Manufacturer: RION
Model/Type: NL-42 (Meter), UC-52 (Microphone), NH-24 (Preamplifier)
Serial No.: 00546401 (Meter), 152917 (Microphone), 46612 (Preamplifier)
ID No.: -
Ambient Temperature: $(23 \pm 2) ^\circ\text{C}$
Relative Humidity: $(50 \pm 15) \%$
Pressure: $(101.3 \pm 1.5) \text{ kPa}$

Method of Calibration :-

IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

	Instrument	Model	Serial No.	Cert. No.	Due Date
1)	Standard microphone	4180	2661000	AA-1020-22	14 June 2023
2)	Arbitrary Function Generator	AFG2021	C010063	CK20220059EA	19 June 2023
3)	Programmable Attenuator	PA5	2913	EF-0014-22	3 April 2023
4)	6.5 Digit precision multimeter	8846A	9610014	CB20220223EA	14 November 2023
5)	Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P220024 CD20220164EA	17 March 2023 24 July 2023
6)	Pressure humidity and Temperature Transmitter	PTU301	F0640003	CL1-P220029 CD20220165EA	31 March 2023 24 July 2023
7)	Performance Audio Analyzer	U8903B	MY56510003	CB20220063EA CK20220080EA	15 February 2023 8 September 2023

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
94.1	94.1	0.0	± 1.0

Note : Absolute sensitivity was established by the use of the Sound Calibrator RION Type NC-74 S/N : 34536113.

Certificate No.: CP20220335EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
15.4

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	11.3
C-weighting	17.1
Z-weighting	23.2

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.7	0.7	0.8	±1.5
1000	0.2	0.2	0.2	±1.0
8000	-2.4	-2.3	-2.4	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	-0.1	0.0	±2.0
125	0.0	-0.1	0.0	±1.5
250	0.0	-0.1	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.1	0.1	0.0	±5.0

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

Certificate No.: CP20220335EA

Calibration Report

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
130.0	130.0	0.0	±1.1
131.0	131.0	0.0	±1.1
132.0	132.0	0.0	±1.1
133.0	133.0	0.0	±1.1
134.0	134.0	0.0	±1.1
135.0	135.0	0.0	±1.1
136.0	136.0	0.0	±1.1
137.0	137.0	0.0	±1.1

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1

Certificate No.: CP20220335EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower (Cont.)

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.0	0.0	±1.1
39.0	39.0	0.0	±1.1
34.0	33.8	-0.2	±1.1
29.0	28.9	-0.1	±1.1

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	126.0	0.0	±1.0
	2	109.0	0.0	+1.0 ; -2.5
	0.25	99.9	-0.1	+1.5 ; -5.0
Slow	200	119.6	0.0	±1.0
	2	100.0	0.0	+1.0 ; -5.0
LAE	200	120.0	0.0	±1.0
	2	100.0	0.0	+1.0 ; -2.5
	0.25	90.9	-0.1	+1.5 ; -5.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	125.4	125.2	-0.2	±3.0
Positive half cycle	124.4	124.1	-0.3	±2.0
Negative half cycle	124.4	124.1	-0.3	±2.0

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
139.5	139.6	0.1	±1.5

Certificate No.: CP20220335EA

Calibration Report

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	129.0	129.0	0.0	±0.3

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks: 1. The acceptance limit is for the deviated value.
2. Acceptance limits was IEC61672-3:2013 Class 2.
3. The coverage factor $k = 2.00$

-- End of Report --

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0455

MTC No. EEL. BP. 41/0465

CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Keithley 2015-P S/N 4106495.

7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 22 Apr. 2022

Date of Calibration : 28 Apr. 2022

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-65/0455

MTC No. EEL. BP. 41/0465

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.93	-0.07	± 0.10	± 0.40 dB

2. Frequency


Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.44	± 0.50	$\pm 3.0\%$

- Note :
1. No adjustment.
 2. The calibrator pressure correction was not included.
 3. The microphone volume correction was not included.

Calibrated by :



(Mr. Pawikiat Tamsamran)

Approved by :



(Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 28 Apr. 2022

Date of Issue : 28 Apr. 2022

Ref : 2011265042601787001

2 / 2

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N 4106495.
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 27 Mar. 2023

Date of Calibration : 29 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.94	-0.06	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.80	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :



Approved by :


(Mr. Prawate Kluaypa)
Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 29 Mar. 2023

Date of Issue : 30 Mar. 2023

Ref : 2011266032701228001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



Certificate of Calibration

Certificate Number : SPR23030505-8

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 32

Serial Number : TPE070001

ID. Number : R12

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$

Received Date : 30 Mar 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 31 Mar 2023

Location of Calibration : In-Lab

Recommend Due Date : 31 Mar 2024

Calibration Procedure : SP-CPT-04-13

Date of Issue : 01 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Sarawut Khitmai

Approved by

Calibration Officer

Authorized Signatory



Calibration Report

Certificate Number : SPR23030505-8

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR23010480-5	22 Feb 2024
THERMO-HYGROMETER	5020A	A47046	QR23-0176	26 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

Quality Reborn Co., Ltd



Result of Calibration

Certificate No. : SPR23030505-8

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.0	-0.013	0.50
35.0	35.010	35.0	-0.010	0.50
40.0	40.015	40.0	-0.015	0.50

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.0	-0.013	0.50
35.0	35.010	35.0	-0.010	0.50
40.0	40.015	40.0	-0.015	0.50

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.1	0.087	0.50
35.0	35.010	35.1	0.090	0.50
40.0	40.015	40.1	0.085	0.50

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)
MANUFACTURER : 3M
MODEL / TYPE : QUESTemp° 46
SERIAL NO. : TSI010011
CLID. NO. : 232000797
JOB CONTROL NO. : 220815082000

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900


DATE OF RECEIVED : 15 August 2022

DATE OF ISSUED : 20 August 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Oranut Kamchatphai
Calibration Engineer

Approved By :



20 August 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22082000

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp° 46

SERIAL NO. : TSI010011

DATE OF CALIBRATION : 18 August 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-74**. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.

Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Thunder Scientific Corporation.

Certificate No. 19944, Due Date 26 January 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22082000

F3-011-04/01-12

page 2 of 3





CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter (thermal environment monitor).

CALIBRATION DATA

*1. CORRECTION OF TEMPERATURE [WET]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.98	31.0	-1.02	0.40
35.0	34.98	36.2	-1.22	
40.0	40.00	41.3	-1.30	

Note. * means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

2. CORRECTION OF TEMPERATURE [DRY]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.98	30.0	-0.02	0.40
35.0	34.98	34.9	+0.08	
40.0	40.00	40.1	-0.10	

3. CORRECTION OF TEMPERATURE [GLOBE BULB]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.98	30.0	-0.02	0.40
35.0	34.98	34.9	+0.08	
40.0	40.00	39.7	+0.30	

Note. The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22082000

F3-011-04/01-12

page 3 of 3



@clccalibration

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp° 46

SERIAL NO. : TSI0100006

CLID. NO. : 232000793

JOB CONTROL NO. : 220505044316

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900


DATE OF RECEIVED : 05 May 2022

DATE OF ISSUED : 12 May 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Oranut Kamchatphai
Calibration Engineer

Approved By :



12 May 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22044316

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : **DIGITAL THERMOHYGRO METER**
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : **3M**

MODEL / TYPE : **QUESTemp° 46**

SERIAL NO. : **TSI010006**

DATE OF CALIBRATION : **05 May 2022**

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-74**. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 36151.
Temperature & Humidity Chamber, PGC Model 9141-5114 S/N.0802282.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Thunder Scientific Corporation.
Certificate No. 19317, Due Date 09 July 2022.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. **Q22044316**

F3-011-04/01-12

page 2 of 3



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter (thermal environment monitor).

CALIBRATION DATA

*1. CORRECTION OF TEMPERATURE [WET]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.99	31.5	-1.51	0.40
35.0	35.01	36.5	-1.49	
40.0	39.99	41.5	-1.51	

Note. * means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

2. CORRECTION OF TEMPERATURE [DRY]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.99	30.1	-0.11	0.40
35.0	35.01	35.0	+0.01	
40.0	39.99	40.1	-0.11	

3. CORRECTION OF TEMPERATURE [GLOBE BULB]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.99	30.1	-0.11	0.40
35.0	35.01	35.0	+0.01	
40.0	39.99	39.6	+0.39	

Note. The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22044316

F3-011-04/01-12

page 3 of 3





CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)
MANUFACTURER : 3M
MODEL / TYPE : QUESTemp° 46
SERIAL NO. : TSH120025
CLID. NO. : 232000794
JOB CONTROL NO. : 220815082001

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900


DATE OF RECEIVED : 15 August 2022

DATE OF ISSUED : 20 August 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Oranut Kamchatphai
Calibration Engineer

Approved By :



20 August 2022

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to
the International System of Units (SI)

Certificate No. Q22082001

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp° 46

SERIAL NO. : TSH120025

DATE OF CALIBRATION : 18 August 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-74**. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.

Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Thunder Scientific Corporation.

Certificate No. 19944, Due Date 26 January 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22082001

F3-011-04/01-12

page 2 of 3





CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter (thermal environment monitor).

CALIBRATION DATA

***1. CORRECTION OF TEMPERATURE [WET]**

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.98	31.1	-1.12	0.40
35.0	34.98	36.2	-1.22	
40.0	40.00	41.2	-1.20	

Note. * means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

2. CORRECTION OF TEMPERATURE [DRY]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.98	30.1	-0.12	0.40
35.0	34.98	34.9	+0.08	
40.0	40.00	39.9	+0.10	

3. CORRECTION OF TEMPERATURE [GLOBE BULB]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.98	30.1	-0.12	0.40
35.0	34.98	34.8	+0.18	
40.0	40.00	39.9	+0.10	

Note. The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22082001

F3-011-04/01-12

page 3 of 3



@clccalibration



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp° 46

SERIAL NO. : TSH120011

CLID. NO. : 232000795

JOB CONTROL NO. : 220505044292

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 05 May 2022

DATE OF ISSUED : 12 May 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Oranut Kamchatphai
Calibration Engineer



Approved By :

12 May 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to
the International System of Units (SI)

Certificate No. Q22044292

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : **DIGITAL THERMOHYGRO METER**
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : **3M**

MODEL / TYPE : **QUESTemp° 46**

SERIAL NO. : **TSH120011**

DATE OF CALIBRATION : **05 May 2022**

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-74**. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 36151.

Temperature & Humidity Chamber, PGC Model 9141-5114 S/N.0802282.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Thunder Scientific Corporation.
Certificate No. 19317, Due Date 09 July 2022.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. **Q22044292**

F3-011-04/01-12

page 2 of 3





CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter (thermal environment monitor).

CALIBRATION DATA

*1. CORRECTION OF TEMPERATURE [WET]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.99	31.4	-1.41	0.40
35.0	35.01	36.4	-1.39	
40.0	39.99	41.4	-1.41	

Note. * means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

2. CORRECTION OF TEMPERATURE [DRY]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.99	30.0	-0.01	0.40
35.0	35.01	35.1	-0.09	
40.0	39.99	40.2	-0.21	

3. CORRECTION OF TEMPERATURE [GLOBE BULB]

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
30.0	29.99	29.9	+0.09	0.40
35.0	35.01	34.8	+0.21	
40.0	39.99	39.6	+0.39	

Note. The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22044292

F3-011-04/01-12

page 3 of 3



@clccalibration



บริษัท เอกเสคคิวทิฟ เทรดดิง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230
TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etithai.com E-mail : info@etithai.com

ที่ RA 033/23

ใบรายงานผลการปรับเทียบ

ชื่อผู้ขอรับบริการ : บริษัท ไออาร์พีซี จำกัด (มหาชน)

ที่อยู่ : 299 หมู่ 5 ถนนสุขุมวิท ตำบลเชิงเนิน อำเภอเมืองระยอง จังหวัดระยอง 21000

ปรับเทียบที่ : บริษัท เอกเสคคิวทิฟ เทรดดิง จำกัด

ที่อยู่ : 48/194-5 ซอย ประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวง/เขตลาดพร้าว กรุงเทพฯ 10230

รายละเอียดเครื่องมือที่ทำการปรับเทียบ :

เครื่องมือ : เครื่องตรวจวัดไอระเหยจากสารเคมี

ผลิตภัณฑ์ : RAE Systems

รุ่น : MiniRAE3000

หมายเลขเครื่อง : 592-001193

สภาวะแวดล้อม :

อุณหภูมิ : $(25 \pm 3) ^\circ\text{C}$

ความชื้นสัมพัทธ์ : $(24 \pm 15) \%$

ความดันบรรยากาศ : 760 มิลลิเมตรปรอท

วันที่ปรับเทียบมาตรฐาน : 7 มีนาคม 2566

วันที่ครบกำหนดการปรับเทียบ : 7 มีนาคม 2567

วิธีการปรับเทียบมาตรฐาน : ปรับเทียบ โดยใช้ Standard Reference Gas ผลิตภัณฑ์ CALGAZ.

- Isobutylene Standard Gas 100 ppm; Lot number 304-402257108-1.

- Isobutylene Standard Gas 1000 ppm; Lot number 304-402250416-1.

ผลการปรับเทียบมาตรฐาน

Sensor Type	Reference Concentration	Before Cal.	After Cal.	Error Reading	Result
PID	0 ppm (Air Zero)	0.0 ppm	0.0 ppm	0.0 ppm	Pass
PID	100 ppm (Isobutylene 100 ppm)	85.0 ppm	100.0 ppm	0.0 ppm	Pass
PID	1000 ppm (Isobutylene 1000 ppm)	899.5 ppm	991.8 ppm	8.2 ppm	Pass

Flow Rate of Pump : 480 cc/min.

Accuracy : $\pm 2 \%$ at calibration point

Service Engineer

Service Engineer Manager

ผลการสอบเทียบ/ปรับเทียบ นี้ รับรองเฉพาะตัวอย่างและรายการที่ได้ระบุไว้เท่านั้น

การนำรายงานผล/ใบรับรองนี้ไปโฆษณาและการคัดลอกหรือการนำผลบางส่วนไปเผยแพร่ต่อสาธารณะต้องได้รับอนุญาตเป็นลายลักษณ์อักษรจากทางบริษัทฯ



บริษัท เอกเสคคิวทิฟ เทรตติ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230

TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

No. RA 033/23

Certificate of Calibration

Customer : IRPC Public Company Limited.
Address : 169 Moo 9, Suk Sawat 45, Suk Sawat Road, Bang Kru, Phra Pradaeng, Samut Prakan 10130
Thailand.

Calibration location : Executive Trading Limited.
Address : 48/194-5 Soi Praditmanutham 19, Pradit Manutham Road, Latphrao, Bangkok 10230

Tools :

Environmental Condition :

Instrument	: Gas Detector	Temperature	: $(25 \pm 3) ^\circ\text{C}$
Product	: RAE Systems	Relative Humidity	: $(24 \pm 15) \%$
Model Name	: MiniRAE3000	Pressure	: 760 mmHg
Serial Number	: 592-001193		

Date of Calibration : March 7, 2023

Due Date of Calibration : March 7, 2024

Calibration Method : This instrument has been calibrated using calibration gases. Test and calibration data is
On file with Executive trading limited.

Reference Standard : - Isobutylene Standard Gas 100 ppm; Lot number 304-402257108-1.
- Isobutylene Standard Gas 1000 ppm; Lot number 304-402250416-1.

Test Result

Sensor Type	Reference Concentration	Before Cal.	After Cal.	Error Reading	Result
PID	0 ppm (Air Zero)	0.0 ppm	0.0 ppm	0.0 ppm	Pass
PID	100 ppm (Isobutylene 100 ppm)	85.0 ppm	100.0 ppm	0.0 ppm	Pass
PID	1000 ppm (Isobutylene 1000 ppm)	899.5 ppm	991.8 ppm	8.2 ppm	Pass

Flow Rate of Pump : 480 cc/min.

Accuracy : $\pm 2 \%$ at calibration point

Service Engineer

Service Engineer Manager

The results relate only to the items tested or calibrated.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the company.



บริษัท เอกเสคคิวทิฟ เทรตติ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230
TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

ที่ RA 033/23

ใบรายงานการตรวจเช็คเครื่องตรวจวัดก๊าซ รุ่น MiniREA3000

หมายเลขเครื่อง : 592-001193

วันที่ตรวจเช็ค : 7 มีนาคม 2566

ลำดับที่	รายละเอียดการตรวจสอบ	RAW COUNT		สรุป	หมายเหตุ
		REF.	REAL		
1.	PID RAW COUNT				
	Ch.H	10000-62500	48079	■ YES □ NO	
	Ch.L	<62500	52722	■ YES □ NO	
2.	Lamp	>40	48	■ YES □ NO	

ลำดับที่	รายละเอียดการตรวจสอบ	การแก้ไข	สรุป	หมายเหตุ
1.	Motor Pump	Check flow rate	■ YES □ NO	480 cc/min.
2.	Buzzer	-	■ YES □ NO	-
3.	Li-ion Battery	-	■ YES □ NO	-
4.	Key Pad			
	Y/+	-	■ YES □ NO	-
	N/-	-	■ YES □ NO	-
	MODE	-	■ YES □ NO	-
5.	LCD Display	-	■ YES □ NO	-
6.	Light Sensor	-	■ YES □ NO	-
7.	Pocket Clip	-	□ YES □ NO	-
8.	PC Port	-	■ YES □ NO	-
9.	Slim Rubber Boot	-	■ YES □ NO	-
10.	Tube adapter assembly	-	□ YES □ NO	-

Service Engineer

ผลการสอบเทียบ/ปรับเทียบ นี้ รับรองเฉพาะตัวอย่างและรายการที่ได้รับอนุญาตไว้เท่านั้น

การนำรายงานผล/ใบรับรองนี้ไปโฆษณาและการคัดค้านหรือการนำผลบางส่วนไปเผยแพร่ต่อสาธารณะต้องได้รับอนุญาตเป็นลายลักษณ์อักษรจากทางบริษัทฯ



CERTIFICATE OF ANALYSIS

Date: November 8, 2021
PO Number: 0000020821
Lot Number: 304-402257108-1

Customer: CalGaz Internl LLC

Use Before: 11/08/2025


<u>Component</u>	<u>Requested Concentration</u>	<u>Analytical Result (+/- 2%)</u>
Isobutylene Air	100 PPM Balance	100.5 PPM Balance

Cylinder Size: 3.6 Cu. Ft.
Contents: 103 Liter

Valve: 5/8" -18UNF
Pressure: 1000 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/ or N.I.S.T.
Gas Mixture reference materials.

Analyst:





CERTIFICATE OF ANALYSIS

Date: November 8, 2021
Order Number: 0000020821
Lot Number: 304-402250416-1

Customer: CalGaz Internl LLC
Use Before: 11/08/2025


<u>Component</u>	<u>Requested Concentration</u>	<u>Analytical Result (+/- 2%)</u>
Isobutylene Air	1000 PPM Balance	995 PPM Balance

Cylinder Size: 1.2 Cu. Ft.
Contents: 34 Liter

Valve: CGA 600
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/ or N.I.S.T. Gas Mixture reference materials.

Analyst:

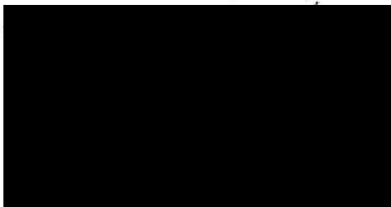

**CERTIFICATE
of
Attendance**

It is hereby certified that

Mr Surinthorn Sainate
(Executive Trading Limited)


has successfully completed the

RAE Service Training Course

Conducted by

HONEYWELL

on **2nd August 2022**



Conducted by : Desmond Tan
Service Engineer / Technical Trainer
Date of Issue : 2nd August 2022
Certificate valid for 2 years from date of issue



PETRO-INSTRUMENTS CORP., LTD.

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak Bangkok 10900 Thailand

Tel. : (+66) 2939 5711 (12 Lines), (+66) 2513 2333 (12 Lines), Fax. : (+66) 939 4207, (+66) 2939 4207

Website : <http://www.pico.co.th> email-address: pico@pico.co.th , service@pico.co.th

DOC. NUMBER

CMV-S23-0034

SERVICE REPORT

REPORT DATE

June 21, 2023

EQUIPMENT: Multi Water Quality Checker, U-5000G	SERIAL NUMBER / TAG NUMBER RAAGSEN3	BRAND / MANUFACTURER HORIBA
CUSTOMER NAME: IRPC PUBLIC COMPANY LIMITED	LACATION: rayong	JOB NUMBER / REQUESTED NUMBER JID2300281-002

SCOPE OF WORK / REASON FOR VISIT

Repair and Calibration

FOUND FAILURE & CORRECTIVE ACTION DETAILS

1. ตรวจสอบสภาพเครื่อง Multi Water Quality Checker

- Meter Model: U-5000G S/N: RAAGSEN3 สามารถใช้งานได้ปกติ
- Probe Model: U-53 S/N: V39CGM6U พบว่า **Sensor Turbidity** ไม่สามารถใช้งานได้
- Sensor pH,COND,ORP,DO ใช้งานได้ปกติ

2. ทำการ Cleaning sensor ทุก parameter

- เติมน Internal Solution (KCl) ใน Reference sensor

3. ปรับเทียบ Auto Calibration ด้วย Buffer pH 4

- พบว่าสามารถปรับเทียบค่าผ่าน คือ pH , COND, ORP, Temp, DO and Depth

4. ปรับเทียบ Manual Calibration 2 จุด (zero , span)

- พบว่าสามารถปรับเทียบค่าผ่าน คือ pH , COND,ORP, Temp, DO and Depth

สรุป : เครื่อง Multi Water Quality Checker Meter Model: U-5000G S/N: RAAGSEN3 และ

Sensor Model: U-53 S/N: V39CGM6U สามารถใช้งานได้ตามปกติ ยกเว้น Sensor Turbidity

WORK CONCLUSION

<input checked="" type="checkbox"/> COMPLETED		<input type="checkbox"/> IN COMPLETED	PARTS REPLACEMENT		
<input checked="" type="checkbox"/> CHARGE	<input type="checkbox"/> NO CHARGE		PARTS NAME	P/N	QTY.
<input checked="" type="checkbox"/> Service Fee	<input type="checkbox"/> Project Warranty	<input type="checkbox"/> Take to Office			
<input type="checkbox"/> Travelling	<input type="checkbox"/> Service Warranty	<input type="checkbox"/> Wait for Parts			
<input type="checkbox"/> Spare Parts	<input type="checkbox"/> Spare Parts Warranty	<input type="checkbox"/> In Progress			
<input type="checkbox"/> Other	<input type="checkbox"/> Service Contract	<input type="checkbox"/> Other			

TIME SPENT (HOURS)

YEAR	2023							TOTAL HOURS	TRAVELING DETAILS	
MONTH	6									
DATE	21								TRAVEL BY	-
SERVICE TIME	4							4	FROM	-
OVERTIME	-							-	TO	-
TRAVELING TIME	-							-	TOTAL ROUND TRIP	-
TOTAL HOURS	4							4	DISTANCE (KM.)	-

SERVICE CREW

NAME		NAME	
1. Chamaiporn Vongchalee		3.	
2.		4.	

CUSTOMER'S NAME	CUSTOMER'S SIGNATURE	DATE



บริษัท เพทโร-อินสตรูเมนต์ จำกัด
PETRO-INSTRUMENTS CORP., LTD.

7/409 ซ.วิภาวดีรังสิต 36 ถ.วิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak, Bangkok 10900, Thailand.

TEL : (662) 9395711 (12 Lines), 5132333 (12 Lines), 5139575-9 FAX : (662) 9394207, 9394208

<http://www.pico.co.th> E-mail-address : pico@pico.co.th

TEST REPORT OF CALIBRATION

We hereby certify that the equipment mentioned below have been maintained and have duly performed in accordance with HORIBA specifications.

Equipment	:	Multi Water Quality Checker
Model	:	U-5000G
Manufacture	:	HORIBA
Serial No.	:	RAAGSEN3
Job No.	:	JID2300281-002
Customer	:	IRPC Public Company Limited
Calibration date	:	June 21, 2023
Calibration due	:	June 21, 2024

Petro-Instruments Corp., Ltd.

Calibrated by

Approved by

Assistant Section Manager

Scientific Product Business Unit



บริษัท เพทโร-อินสตรูเมนต์ จำกัด
PETRO-INSTRUMENTS CORP., LTD.

7/409 ซ.วิภาวดีรังสิต 36 ถ.วิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak, Bangkok 10900, Thailand.

TEL : (662) 9395711 (12 Lines), 5132333 (12 Lines), 5139575-9 FAX : (662) 9394207, 9394208

<http://www.pico.co.th> E-mail-address : pico@pico.co.th

CALIBRATION REPORT

Equipment : Multi Water Quality Checker
Manufacturer : HORIBA
Model : U-53
Serial No. : V39CGM6U
Date of Calibration : June 21, 2023
Customer Name : IRPC Public Company Limited

HORIBA, Multi Water Quality Checker model U-53 was tested according to service manual.

Auto Calibration (1- point)

Check function	Calibration	Before Calibrate	After Calibrate
pH	1- point auto (Zero) (4.01 pH)	4.05 pH	4.01 pH
CONDUCTIVITY	1- point auto (Span) (4.49 mS/cm)	4.45 mS/cm	4.49 mS/cm
DO	1- point auto (Span) (8.92 mg/L)	8.87 mg/L	8.92 mg/L
Depth	(0 m)	0 m	0 m

Reference Standard

- Standard Solution of HORIBA, pH 4 Lot No. S3316/03



บริษัท เพทโร-อินสตรูเมนต์ จำกัด
PETRO-INSTRUMENTS CORP., LTD.

7/409 ซ.วิภาวดีรังสิต 36 ถ.วิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak, Bangkok 10900, Thailand.

TEL : (662) 9395711 (12 Lines), 5132333 (12 Lines), 5139575-9 FAX : (662) 9394207, 9394208

<http://www.pico.co.th> E-mail-address : pico@pico.co.th

Manual Calibration (2- point)

A. pH Measurement.

Check item	pH Standard Solution	Before Calibrate	After Calibrate	Error	Judgment
Zero Calibration	6.86	6.86	6.86	0.00	PASS
Span Calibration	4.01	4.01	4.01	0.00	PASS

Measure at temperature 25 °C Within ± 0.1 pH

B. Conductivity Measurement.

Check item	Conductivity Standard Solution	Before Calibrate	After Calibrate	Error	Judgment
Zero Calibration	0.00 mS/cm	0.000 mS/cm	0.00 mS/cm	0.000 mS/cm	PASS
Span Calibration	Range 1 (0.100-0.999 S/m) 0.718 mS/cm	0.728 mS/cm	0.718 mS/cm	0.01 mS/cm	PASS
	Range 2 (1.00-10.00 S/m) 6.67 mS/cm	6.70 mS/cm	6.67 mS/cm	0.003 mS/cm	PASS
	Range 3 (0.0-99.9 mS/m) 58.7 mS/cm	59.0 mS/cm	58.7 mS/cm	0.3 mS/cm	PASS

Measure at temperature 25 °C Within $\pm 1\%$ /F.S.



บริษัท เพทโร-อินสตรูเมนต์ จำกัด
PETRO-INSTRUMENTS CORP., LTD.

7/409 ซ.วิภาวดีรังสิต 36 ถ.วิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900

7/409 Soi Vibhavadi-Rangsit 36, Vibhavadi-Rangsit Rd., Chatuchak, Chatuchak, Bangkok 10900, Thailand.

TEL : (662) 9395711 (12 Lines), 5132333 (12 Lines), 5139575-9 FAX : (662) 9394207, 9394208

http://www.pico.co.th E-mail-address : pico@pico.co.th

C. DO Measurement.

Check item	DO Standard Solution	Before Calibrate	After Calibrate	Error	Judgment
Zero Calibration	(Solution of NaSO ₃) 0.00 mg/l	0.00 mg/l	0.00 mg/l	0.00 mg/l	PASS
Span Calibration	(Saturated with oxygen in air) 8.11 mg/l	8.15 mg/l	8.11 mg/l	0.04 mg/l	PASS

Measure at temperature 25 °C With in 0 to 20 mg/L :± 0.2 mg/l, 20 to 50 mg/L :± 0.5 mg/l

Calibrated by : Chamaiporn Vongchalee

Approved by : Athitphong Kanchanasathian

DATA SHEET FOR CALIBRATION / VERIFICATION AND INSPECTION


Calibration

Verification

Inspection
เครื่องมือ / อุปกรณ์ ที่สอบเทียบหรือทวนสอบ

Equipment / Tools : Multimeter (pH , DO) Tag No. / I.D. No. : L09-AT-SP003-A2 Serial No. : 130500088588

Cal. / Ver. date : 4/4/2022
เครื่องมือ / อุปกรณ์ที่เป็น Master

Equipment / Tools :	I.D. No.	Model /Serial No.	Cert. No.	Expired date

Reference Materials ที่ใช้

Chemical	Grade	Assay (%)	Cert. No.	Expired date
Buffer pH 4.00 ; Lot No. HC99677935				31/7/2022
Buffer pH 7.00 ; Lot No. HC04269139				31/10/2023
Buffer pH 10.00 ; Lot No. HC02905338				30/6/2023


Calibration / verification item	Result	Error	Acceptance Criteria	Pass / Fail
1.การสอบเทียบ Observed Slope (slope)	98	-	95 to 105%	Pass
2.verification pH6.86	6.85	-0.01	± 0.05	Pass

Inspection item	Result	Correction
1.ตรวจเช็คสภาพพร้อมใช้งาน	ปกติ	

Next Due date 31/5/2022

Performed by : 

Date : 4/4/2022

Approved By : 

Date : 4/4/2022

Certificate of Analysis – Certified Reference Material

Certipur® Buffer solution pH 10.00 (20°C)

Certified Reference Material for pH measurement

Product no.: 1.09438.1000
Lot no.: HC02905338
Description of CRM: Certipur® Buffer solution pH 10.00 (20°C)
Certified Reference Material for pH measurement
Expiry date: 2023/06/30
Storage: +15°C to +25°C tightly closed in the original container
Composition: boric acid / potassium chloride / sodium hydroxide



Certified value

Associated uncertainty, $U = k \cdot u$
($k=2$)

pH value 10.01

± 0.03 (20°C)

Metrological traceability:

The pH value of this certified buffer solution is directly traceable to primary certified reference materials characterised by PTB and verified by SRMs from NIST.

NIST 189c, 188, 185i, 186 Ig, 186 IIg, 187f

PTB OX-405/18, TA-442/19, PHT-340/16, PHO-346/16, BO-373/17

PTB: Physikalisch Technische Bundesanstalt, Braunschweig, Germany

NIST: National Institute of Standards and Technology, Gaithersburg, USA.

Measurement method:

pH value is measured with a combined glass electrode after 5-point calibration according to DIN 19268 with reference buffer solutions according to DIN 19266, IUPAC, NIST, Ph.Eur. and USP.

Accreditation:

Merck KGaA, Darmstadt, Germany is accredited by the German accreditation authority DAkkS as registered reference material producer D-RM-15185-01-00 in accordance with ISO 17034 and registered calibration laboratory D-K-15185-01-00 according to DIN EN ISO/IEC 17025.

Certificate issue date:

2020/06/24



ISO 17034



ISO/IEC 17025

CRM released by Approving Officer
or delegate LS-OII-QS3



Dipl.-Ing. Ayfer Yildirim
Responsible Manager of LS-OII-QS3
(Calibration Laboratory D-K-15185-01)



Intended use:	This reference material is intended for use as a calibration standard for pH instruments or pH electrodes or as a control sample for measuring the pH value.
Instructions for handling and correct use:	The pH value is strongly dependent on the temperature. It is therefore necessary to keep the temperature constant within the measurement.
Health and safety information:	Please refer to the Safety Data Sheet for detailed information about the nature of any hazard and appropriate precautions to be taken.
Preparation:	This reference material is prepared gravimetrically from boric acid, potassium chloride, sodium hydroxide and high purity water.

Associated uncertainty:

The expanded uncertainty U_{CRM} is calculated as $U_{CRM} = k \cdot u_{CRM}$, where $k = 2$ is the coverage factor for a 95% coverage probability and u_{CRM} is the combined standard uncertainty in accordance to ISO 17034.

The combined uncertainty u_{CRM} is derived from combination of the squared uncertainty contributions:

$$u_{CRM} = \sqrt{u^2_{Characterisation} + u^2_{Homogeneity} + u^2_{Stability}}$$

$u_{characterisation}$:	is the uncertainty in accordance with DIN EN ISO/IEC 17025 which includes the contributions of the primary reference material and the measuring system.
$u_{homogeneity}$:	is the between-bottle variation in accordance with ISO 17034. The assessment of homogeneity is performed by analysis of a representative number of systematically chosen sample units.
$u_{stability}$:	is the uncertainty obtained from short-term and long-term stability in accordance with ISO 17034. The stability studies are the basis for the quantification of the expiry date of this reference material for the unopened bottle.

Informative values:

Temperature dependence ¹ :	Temperature [°C]	Δ pH
	0	+ 0.26
	5	+ 0.17
	10	+ 0.11
	15	+ 0.05
	20	± 0
	25	- 0.06
	30	- 0.11
	35	- 0.16
	40	- 0.18
	50	- 0.26

¹Temperature deviation data provided for reference only. Values are not batch-specific and should not be considered certified values.

For more detailed information please read the certification report on our website.

Certificate of analysis revision history:

Certificate version	Date	Reason for version
01	2020/06/24	Initial version

