ภาคผนวก ง

เอกสารสอบเทียบเครื่องมือ

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Laboratory Instrument/Equipments.(คุณภาพอากาศ)									
1	Analytical Balance (Repeatability 0.1 mg)	ฝุ่นละอองรวม	Mettler-Toledo	AB204-S / 1128312528	Mettler-Toledo (Thailand) Ltd.	23MM331	7 Apr 23	5 Apr 24	-
2	Analytical Balance (Repeatability 0.1 mg)		Mettler-Toledo	AB204-S/FACT / B108115858	Mettler-Toledo (Thailand) Ltd.	23MM332	7 Apr 23	5 Apr 24	-
3	Analytical Balance (Repeatability 0.001 mg)	ฝุ่นทุกขนาด	Mettler-Toledo	XP6 / B322373893	Mettler-Toledo (Thailand) Ltd.	23MM333	7 Apr 23	5 Apr 24	-
Laboratory Instrument/Equipments.(คุณภาพน้ำ)									
1	pH Meter	ความเป็นกรดและด่าง	Mettler-Toledo	Seven Easy S20 / 1230525212	National Food Institute, Ministry of Industry, Thailand	2302181-001-01	24 Mar 23	22 Mar 24	-
2	pH Meter		Mettler-Toledo	SevenCompact S220/ C113432421	National Food Institute, Ministry of Industry, Thailand	2203527-001-01	5 Jul 22	4 Jul 23	-
3	BOD Incubator	บีโอดี	Arco	UC4-1320 / (UAE.WAO.015/2561)	Technology Promotion Association (Thailand-Japan)	23TM249	15 Feb 23	14 Feb 24	-
4	BOD Incubator		Arco	UR-1320 / (UAE.WAO.018/2551)	Technology Promotion Association (Thailand-Japan)	23TM375	12 Apr 23	10 Apr 24	-
5	Analytical Balance (Repeatability 0.01 mg)	สารแขวนลอย	Mettler-Toledo	XSR205DU / C009071872	Technology Promotion Association (Thailand-Japan)	23MM112	26 Apr 23	24 Apr 24	-
6	Hot Air Oven		Memmert	UF55 / B216.1666	Technology Promotion Association (Thailand-Japan)	22TM1490	19 Oct 22	18 Oct 23	-
Laboratory Instrument/Equipments.(คุณภาพน้ำ)									

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
7	Analytical Balance (Readability 0.1 mg)	น้ำมันและไขมัน	Mettler-Toledo	XSR204 / C117635043	National Food Institute, Ministry of Industry, Thailand	2302827-001-01	10 May 23	8 May 24	-
8	UV-VIS Spectrophotometer	ไนเตรท คำนวณเป็นไนโตรเจน	Agilent Technologies	Cary60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP23-021	20 May 23	18 May 24	-
9	UV-VIS Spectrophotometer		Hitachi	U-1900 / 2021-064	DQE Services Co.,Ltd.	SP23-007	6 Jan 23	5 Jan 24	-

Due Date of Calibration* : Schedule the program once a year at least once a year.

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Equipment :	Electronic Balance
Manufacturer :	Mettler Toledo
Model :	AB204-S
Serial No. :	1128312528
ID No. :	UAE.AIR.019/2550
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Location :	Balance Room 2
Received order :	07 April 2023
Calibration Date :	07 April 2023
Ambient Temperature :	15 °C to 40 °C
Relative Humidity :	30 % to 90 %
Calibrated by :	Suwit Imjai
Approved by :	[redacted]
	( ) Pornthippa Tameyakul (✓) Malee Butkruea
Issue Date :	10 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0015OC-1

Procedure used :-

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0010-22	20 Jan 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This result of calibration was made on requested at the point specified by customer.
4. This certificate is not certified for any commercial transaction.
5. This certification is traceable to the International System of Unit.

Result of calibration ( ) Without Adjustment (*) After Adjustment by Internal Calibration
Range capacity : 0 g to 220 g **Resolution** 0.0001 g

Before Adjustment :

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
100	99.9999	+0.0001	0.19	2.03
200	200.0001	-0.0001	0.29	2.00

After Adjustment :

1. **Determination of the standard deviation of weighing machine** (n = 10)

Applied Weight (g)	Standard Deviation of Reading (g)
100	0.00007
200	0.00007

เอกสารไม่ค[redacted]

Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0015OC-1

Cert.No.: 23MM331
Page: 3 of 3

Result of calibration

2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.
The weighing machine reading error obtained is given in the table



Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)	Maximum difference between off-center and central loading (g)
-0.0001	-0.0002	+0.0004	-0.0001	-0.0006	0.0005

3. Departure from nominal value

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
Unload	0.0000	0.0000	0.15	2.13
0.1	0.0999	+0.0001	0.15	2.13
1	0.9999	+0.0001	0.15	2.13
5	4.9999	+0.0001	0.15	2.13
10	9.9999	+0.0001	0.15	2.11
20	20.0000	0.0000	0.15	2.11
50	50.0000	0.0000	0.16	2.06
70	69.9999	+0.0001	0.18	2.04
100	99.9999	+0.0001	0.19	2.03
150	150.0003	-0.0003	0.29	2.00
200	200.0005	-0.0005	0.29	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k*** , providing a level of confidence of approximately 95 %.

-o0o-

[redacted]

เอกสารไม่ค

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert.No.: 23MM332
Page.: 1 of 3

Certificate of Calibration

Equipment : Electronic Balance

Manufacturer : Mettler Toledo

Model : AB204-S /FACT

Serial No. : B108115858

ID No. : UAE.AIR.016/2555

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260

Location : Balance Room 2

Received order : 07 April 2023
Calibration Date : 07 April 2023
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 90 %

Calibrated by : Suwit Imjai

Approved by : [redacted]

( ) Pornthippa Tameyakul
(✓) Malee Butkruea

Issue Date : 10 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0015OC-2

Cert.No.: 23MM332

Procedure used :-

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0010-22	20 Jan 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This result of calibration was made on requested at the point specified by customer.
4. This certificate is not certified for any commercial transaction.
5. This certification is traceable to the International System of Unit.

Result of calibration ( ) Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity : 0 g to 220 g **Resolution** 0.0001 g

Before Adjustment :

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
100	100.0002	-0.0002	0.21	2.06
200	200.0003	-0.0003	0.29	2.00

After Adjustment :

1. **Determination of the standard deviation of weighing machine** (n = 10)

Applied Weight (g)	Standard Deviation of Reading (g)
100	0.00009
200	0.00007

เอกสารไม่คว[redacted]

Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0015OC-2

Cert.No.: 23MM332

Result of calibration

2. **Effect of off center loading**

A mass of 100 g was placed to various position on the pan.
The weighing machine reading error obtained is given in the table



Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)	Maximum difference between off-center and central loading (g)
+0.0001	-0.0003	+0.0003	+0.0006	+0.0002	0.0005

3. **Departure from nominal value**

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
Unload	0.0000	0.0000	0.18	2.17
0.1	0.0999	+0.0001	0.18	2.17
1	0.9998	+0.0002	0.18	2.17
5	5.0000	0.0000	0.18	2.17
10	10.0000	0.0000	0.18	2.17
20	20.0000	0.0000	0.18	2.15
50	50.0001	-0.0001	0.19	2.11
70	70.0001	-0.0001	0.20	2.07
100	100.0002	-0.0002	0.21	2.06
150	150.0004	-0.0004	0.29	2.00
200	200.0005	-0.0005	0.29	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k*** , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่คว[redacted]

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert.No.: 23MM333
Page.: 1 of 3

Certificate of Calibration

Equipment :	Electronic Balance
Manufacturer :	Mettler Toledo
Model :	XP6
Serial No. :	B322373893
ID No. :	UAE.AIR.019/2556
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Location :	Balance Room 2
Received order :	07 April 2023
Calibration Date :	07 April 2023
Ambient Temperature :	15 °C to 40 °C
Relative Humidity :	30 % to 90 %
Calibrated by :	Suwit Imjai
Approved by :	[redacted]

( ) Pornthippa Tameyakul
(✓) Malee Butkruea

Issue Date : 10 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0015OC-3

Procedure used :-

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0010-22	20 Jan 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This result of calibration was made on requested at the point specified by customer.
4. This certificate is not certified for any commercial transaction.
5. This certification is traceable to the International System of Unit.

Result of calibration ( ) Without Adjustment (*) After Adjustment by Internal Calibration
Range capacity : 0 g to 6.1 g **Resolution** 0.000001 g

Before Adjustment :

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
3	2.999987	+0.000013	0.026	2.00
6	6.000003	-0.000003	0.036	2.00

After Adjustment :

1. **Determination of the standard deviation of weighing machine** (n = 10)

Applied Weight (g)	Standard Deviation of Reading (g)
3	0.0000027
6	0.0000030

เอกสารไม่ค[redacted]

Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0015OC-3

Cert.No.: 23MM333
Page: 3 of 3

Result of calibration

2. Effect of off center loading

A mass of 2 g was placed to various position on the pan.
The weighing machine reading error obtained is given in the table



Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)	Maximum difference between off-center and central loading (g)
-0.000006	-0.000007	-0.000007	-0.000010	-0.000002	0.000004

3. Departure from nominal value

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (*k*)
Unload	0.000000	0.000000	0.0060	2.37
0.01	0.009998	+0.000002	0.0060	2.13
0.05	0.050003	-0.000003	0.0070	2.05
0.1	0.100007	-0.000007	0.0090	2.03
0.15	0.150000	0.000000	0.011	2.00
0.17	0.169998	+0.000002	0.014	2.00
0.2	0.200002	-0.000002	0.014	2.00
1.5	1.500001	-0.000001	0.020	2.00
3	2.999990	+0.000010	0.026	2.00
4.5	4.499994	+0.000006	0.036	2.00
6	5.999982	+0.000018	0.036	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k*** , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่คว[redacted]

สถาบันอุตสาหกรรมพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2302181-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: pH Meter
Manufacturer: METTLER TOLEDO
Model: SevenEasy pH
Serial No.: 1230525212
ID No.: UAE.WAS.003/2553
Order No.: 2302181
Operation No.: 2302181-001
Date of Receipt: 14 March 2023
Date of Calibration: 24 March 2023

Calibrated by Mr.Pheraphat Tuanjit
Scientist

Approve[redacted]
Specialist, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 24 March 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอุดมสุข 35 ถนนอุดมสุข แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร
2008 Soi 35, Ayun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax. +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันอาหาร
กระทรวงอุตสาหกรรม
national food institute
ministry of industry
สถาบันพัฒนาอุตสาหกรรมเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2302181-001-01

Equipment: pH Meter — **Resolution:** 0.01 pH ; 1 mV

Manufacturer: METTLER TOLEDO — **Model:** SevenEasy pH

Serial No.: 1230525212 — **Type:** Bench top

ID No.: UAE.WAS.003/2553

Date of Calibration: 24 March 2023

Location: Chemical Calibration Laboratory, National Food Institute

Environment Condition: **Ambient Temperature:** (23.4 ± 1.5) °C **Relative Humidity:** (52 ± 3) %

Condition of Equipment: Good Condition

Condition of this Results of Calibration

1.Calibration Method: In house method : W-CC-002 based on direct measurement by using standard voltage calibrator and certified reference material (CRM)

2. Reference Standards / Certified Reference Material

	Instruments	Serial / ID No.	Manufacturer	Certificate No.	Due Date
2.1	DC Voltage Calibrator	2709007	Fluke	22E1959	17 June 2023
2.2	Digital Thermometer	2709007	Fluke	CC-650557-01	30 October 2023
2.3	Thermo-Hygro Meter	NFI.BTH003/17	PONPE	TE 650555-01	21 September 2023
	Certified Reference Material	**Lot. No.**	**Manufacturer**	**Ref N**	**Expire Date**
2.4	pH buffer 4.008 (Primary pH buffer Solution)	873608	CPAchem	PH216.L5	16 February 2025
2.5	pH buffer 6.865 (Primary pH buffer Solution)	873609	CPAchem	PH217.L5	16 February 2025
2.6	pH buffer 10.01 (Primary pH buffer Solution)	873611	CPAchem	PH220.L5	16 February 2024
2.7	pH buffer 7.00 (Standard pH buffer Solution)	873612	CPAchem	PH107.L5	16 February 2024

3. This certification is traceable to The International System of Unit (SI Unit)

3.1	Instruments No.2.1	through	NSC-TISI-TIS 17025 Laboratory Accredition of Calibration No.0008
3.2	Instruments No.2.2	through	NSC-TISI-TIS 17025 Laboratory Accredition of Calibration No.0061
3.3	Instruments No.2.3	through	NSC-TISI-TIS 17025 Laboratory Accredition of Calibration No.0061
3.4	Certified Reference Material No. 2.4 to 2.6	traceable to	Primary measurement method- Harned cell using calibrated thermometer, barometer, and nanovoltmeter.The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.5	Certified Reference Material No.2.7	traceable to	BIM RefN HI-13 LotN 25.05.2022; BIM RefN HI-16 LotN 02.06.2022; BIM RefN HI-13 LotN 25.05.2022; BIM RefN HI-16 LotN 02.06.2022, the Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

[redacted]

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันอาหาร
กระทรวงอุตสาหกรรม
national food institute
ministry of industry
สถาบันพัฒนาอุตสาหกรรมเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2302181-001-01

Equipment: pH Meter — **Resolution:** 0.01 pH ; 1 mV

Manufacturer: METTLER TOLEDO — **Model:** SevenEasy pH

Serial No.: 1230525212 — **Type:** Bench top

ID No.: UAE.WAS.003/2553

Date of Calibration: 24 March 2023

Calibration Results:

1. Calibration of pH Meter (Manual Temperature Compensation at 25 °C)

Nominal pH	DC Voltage Standard (mV)	Average Indicator Reading		Uncertainty (±mV)	Coverage Factor (k)
		mV	pH		
0	414.120	414	0.00	0.58	2.00
2	295.814	296	2.00	0.58	2.00
4	177.464	178	4.00	0.58	2.00
6	59.160	59	6.00	0.58	2.00
7	0.000	0	7.00	0.58	2.00
8	-59.158	-59	8.00	0.58	2.00
10	-177.460	-177	10.00	0.58	2.00
12	-295.811	-296	12.00	0.58	2.00
14	-414.117	-414	14.00	0.58	2.00

2. Calibration of pH Meter with Electrode (Manual Temperature Compensation at 25 °C)

Equipment: pH Electrode — **Type:** Combined Electrode

Manufacturer: METTLER TOLEDO — **Model:** InLab Solids

Serial No.: 1156883 — **ID.No.** N/A

Performance of Electrode system (Three Point Calibration at pH 4, pH 7 and pH 10)

Certified Value @25 °C (pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty (± pH)	Coverage Factor (k)
	pH	mV			
4.008	4.01	187	-	0.0071	2.00
6.865	6.86	22	97.86	0.0075	2.00
10.010	10.01	-160	97.66	0.0086	2.00
6.985	6.99	14	-	0.0093	2.00

[redacted]

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2302181-001-01

Equipment: Digital Thermometer with RTD (pH Meter)
Resolution: 0.1 °C Model: SevenEasy pH
Serial No.: 1230525212 ID No.: UAE.WAS.003/2553
Manufacturer: METTLER TOLEDO

Date of Calibration: 24 March 2023

Location: Chemical Calibration Laboratory, National Food Institute

Environment Condition: Ambient Temperature 25 °C ± 1 °C
Relative Humidity 55 % ± 5 %

Condition of this results of Calibration:

1. Calibration Method : - In house method: W-TE-025 by comparison with standard thermometer.
   - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
   - The temperature scale in use at this laboratory is the International Temperature scale of 1990 (ITS-90).
2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1521	A85997	TE 660039-01	10-Dec-23	NATIONAL FOOD INSTITUTE
Platinum Resistance Thermometer (PRT)	385	509201			

Support Equipment : - Low Temperature Bath (ISOCAL-6), Model: Europa-6 Plus Basic, S/N: 341592/2

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
7. Result of Calibration : [X] Without adjustment [ ] After adjustment

[redacted]

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันอาหาร
กระทรวงอุตสาหกรรม
ศูนย์บริการห้องปฏิบัติการสถาบันอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center
NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2302181-001-01

Equipment: Digital Thermometer with RTD (pH Meter)
Resolution: 0.1 °C Model: SevenEasy pH
Serial No.: 1230525212 ID No.: UAE.WAS.003/2553
Manufacturer: METTLER TOLEDO

Date of Calibration: 24 March 2023

Calibration point: 15.0, 25.0 and 30.0 °C

Calibration result:

- The probe was immersed in liquid bath or dry bath to a minimum depth of 120 mm.
- Description of probe, model : N/A S/N : N/A
  Dimension of probe : Diameter 3 mm., Length 120 mm.,
  Sheath material : N/A

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.2	14.999	- 0.2	0.12
25.2	24.999	- 0.2	0.12
30.2	29.999	- 0.2	0.12

Note

UUC* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

[redacted]

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th
เอกสารไม่ควบคุม

สถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการสถาบันอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2203527-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: pH Meter
Manufacturer: METTLER TOLEDO
Model: Seven Compact S220
Serial No.: C113432421
ID No.: UAE.WAT.009/2564
Order No.: 2203527
Operation No.: 2203527-001
Date of Receipt: 30 June 2022
Date of Calibration: 5 July 2022

Calibrated by Mr.Worapob Sooktong
Scientist

Approved b [redacted]
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 5 July 2022

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตบางพลัด กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการสถาบันอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2203527-001-01
Equipment: pH Meter — **Resolution:** 0.01 pH ; 1 mV
Manufacturer: METTLER TOLEDO — **Model:** Seven Compact S220
Serial No.: C113432421 — **Type:** Bench top
ID No.: UAE.WAT.009/2564
Date of Calibration: 5 July 2022

Location: Calibration Laboratory, National Food Institute
Environment Condition: **Ambient Temperature:** (23.5 ± 1.5) °C **Relative Humidity:** (53 ± 5) %
Condition of Equipment: Good Condition
Condition of this Results of Calibration

1.Calibration Method: In house method : W-CC-002 based on direct measurement by using standard voltage calibrator and certified reference material (CRM)

2. Reference Standards / Certified Reference Material

Instruments	Serial / ID No.	Manufacturer	Certificate No.	Due Date
2.1 DC Voltage Calibrator	2709007	Fluke	22E1959	17 June 2023
2.2 Digital Thermometer	2709007	Fluke	CC-640599-01	30 October 2022
2.3 Thermo-Hygro Meter	NFI.BTH005/18	PONPE	QR22-0351	18 February 2023
Certified Reference Material	**Lot. No.**	**Manufacturer**	**Ref N**	**Expire Date**
2.4 pH buffer 4.008 (Primary pH buffer Solution)	805203	CPAchem	PH216.L5	21 April 2024
2.5 pH buffer 6.865 (Primary pH buffer Solution)	805204	CPAchem	PH217.L5	21 April 2024
2.6 pH buffer 10.01 (Primary pH buffer Solution)	805205	CPAchem	PH220.L5	21 April 2023
2.7 pH buffer 7.00 (Standard pH buffer Solution)	805206	CPAchem	PH107.L5	21 April 2023

3. This certification is traceable to The International System of Unit (SI Unit)

3.1 Instruments No.2.1		through	NSC-TISI-TIS 17025 Laboratory Accredition of Calibration No.0075
3.2 Instruments No.2.2		through	NSC-TISI-TIS 17025 Laboratory Accredition of Calibration No.0061
3.3 Instruments No.2.3		through	NSC-TISI-TIS 17025 Laboratory Accredition of Calibration No.0292
3.4 Certified Reference Material No.	2.4 to 2.6	traceable to	Primary measurement method- Harned cell using calibrated thermometer, barometer, and nanovoltmeter.The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.5 Certified Reference Material No.2.7		traceable to	BIM RefN HI-27 LotN 04.06.2021; BIM RefN HI-28 LotN 28.05.2021; BIM RefN HI-27 LotN 04.06.2021; BIM RefN HI-28 LotN 28.05.2021, the Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

[redacted]

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตบางพลัด กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สุดสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการสุดสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2203527-001-01

Equipment: pH Meter **Resolution:** 0.01 pH : 1 mV

Manufacturer: METTLER TOLEDO **Model:** Seven Compact S220

Serial No.: C113432421 **Type:** Bench top

ID No.: UAE.WAT.009/2564

Date of Calibration: 5 July 2022

Calibration Results:

1. Calibration of pH Meter (Manual Temperature Compensation at 25 °C)

Nominal pH	DC Voltage Standard (mV)	Average Indicator Reading		Uncertainty (±mV)	Coverage Factor (*k*)
		mV	pH		
0	414.117	414	0.00	0.58	2.00
2	295.811	296	2.00	0.58	2.00
4	177.462	177	4.00	0.58	2.00
6	59.159	59	6.00	0.58	2.00
7	-0.001	0	7.00	0.58	2.00
8	-59.159	-59	8.00	0.58	2.00
10	-177.463	-177	10.00	0.58	2.00
12	-295.812	-296	12.00	0.58	2.00
14	-414.119	-414	14.00	0.58	2.00

2. Calibration of pH Meter with Electrode (Manual Temperature Compensation at 25 °C)

Equipment: pH Electrode **Type:** Combined Electrode

Manufacturer: METTLER TOLEDO **Model:** InLab Expert Pro-ISM

Serial No.: 2210418 **ID.No.** N/A

Performance of Electrode system (Three-Point Calibration at pH4, pH7 and pH10)

Certified Value @25 °C (pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty (± pH)	Coverage Factor (*k*)
	pH	mV			
4.008	4.010	182	-	0.0071	2.00
6.865	6.850	14	100.0	0.0075	2.00
10.008	10.010	-169	97.9	0.0093	2.00
6.985	6.990	6	-	0.0087	2.00

[redacted]

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สุดสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการสุดสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2203527-001-01

Equipment: Digital Thermometer with RTD

Resolution: 0.1 °C Model: Seven Compact S220

Serial No.: C113432421 ID No.: UAE.WAT.009/2564

Manufacturer: METTLER TOLEDO

Date of Calibration: 5 July 2022

Location: Calibration Laboratory, National Food Institute

Environment Condition: Ambient Temperature 25 °C ± 1 °C

Relative Humidity 48 % ± 3 %

Condition of this results of Calibration:

1. Calibration Method : - In house method: W-TE-025 by comparison with standard thermometer.
   - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
   - The temperature scale in use at this laboratory is the International Temperature scale of 1990 (ITS-90).
2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1521	A85997	TE 650057-01	10-Dec-22	NATIONAL FOOD INSTITUTE
Platinum Resistance Thermometer (PRT)	385	509201			

Support Equipment : - Low Temperature Bath (ISOCAL-6), Model: Europa-6 Plus Basic, S/N: 341592/2

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
7. Result of Calibration : [X] Without adjustment [ ] After adjustment

[redacted]

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการสถาบันอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2203527-001-01

Equipment: Digital Thermometer with RTD

Resolution: 0.1 °C Model: Seven Compact S220

Serial No.: C113432421 ID No.: UAE.WAT.009/2564

Manufacturer: METTLER TOLEDO

Date of Calibration: 5 July 2022

Calibration point: 15.0, 25.0 and 35.0 °C

Calibration result:

- The probe was immersed in liquid bath or dry bath to a minimum depth of 120 mm.
- Description of probe, model : - S/N : -

Dimension of probe : Diameter 9 mm., Length 120 mm.,

Sheath material : Stainless Steel

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.1	15.038	- 0.1	0.12
25.1	25.038	- 0.1	0.12
35.2	35.024	- 0.2	0.12

Note

- UUC* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

[redacted]

--------- End ---------

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตบางพลัด กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Equipment : BOD Incubator

Manufacturer : Arco

Model : UC4-1320

Serial No. : 13URC4S013201

ID No. : UAE.WAO.015/2561

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260

Location : Lab Floor 2

Received Order : 15 February 2023
Calibration Date : 15 February 2023
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Preecha Hlahib

Approved by : [redacted]

( ) Pornthippa Tameyakul
(✓) Malee Butkruea
( ) Suwit Imjai

Issue Date : 24 February 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0051476

Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2302-0297OC-1

Cert. No.: 23TM249

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY57013711	22LM93	02 Jul 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	29	31
REL.Humid. (%)	63	67
AC Supply (Volt)	220	220

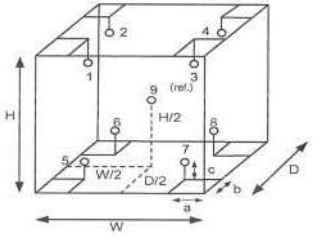

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.62	m
W =	1.2	m
H =	1.2	m
Capacity =	0.89	m^3

Position :	Ref. Std. ID No.:
1	22-18RTD-2/1
2	18RTD-2/2
3	18RTD-2/3
4	18RTD-2/4
5	18RTD-2/5
6	18RTD-2/6
7	18RTD-2/7
8	18RTD-2/8
9 (ref.)	18RTD-2/9

เอกส[redacted]

Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2302-0297OC-1

Cert. No.: 23TM249

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (±°C)	Coverage Factor *k*
20.0	20.0	19.3	0.32	0.57	1.0	0.60	2

Calibration Point (°C)	Measured Temperature (°C) Position								
	1	2	3	4	5	6	7	8	9 (ref.)
20.0	20.086	19.916	20.386	19.976	19.973	19.838	19.837	19.821	19.949

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

เอกส[redacted]

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 23TM375
Page : 1 of 3

Certificate of Calibration

Equipment :	BOD Incubator
Manufacturer :	ARCO
Model :	UR-1320
Serial No. :	-
ID No. :	UAE.WAO.018/2551
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Location :	Lab Floor 2
Received Order :	11 April 2023
Calibration Date :	12 April 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Krisda Malee
Approved by :	[redacted]

( ) Pornthippa Tameyakul
(✓) Malee Butkruea
( ) Suwit Imjai

Issue Date : 24 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Equipment :	BOD Incubator
Condition As-Received :	Used Item
Reference :	2304-0156OC-2

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY59003411	22LM165	26 Nov 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	27
REL.Humid. (%)	42	45
AC Supply (Volt)	219	220

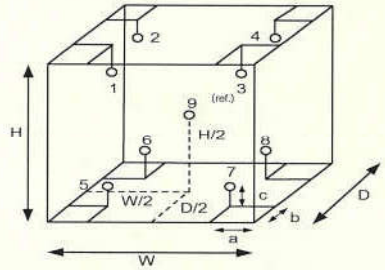

Position :	Ref. Std. ID No.:
1	20RTD-2/1
2	20RTD-2/2
3	20RTD-2/3
4	20RTD-2/4
5	20RTD-2/5
6	20RTD-2/6
7	20RTD-2/7
8	20RTD-2/8
9 (ref.)	20RTD-2/9

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.62	m
W =	1.2	m
H =	1.2	m
Capacity =	0.89	m^3

[redacted]

เอกสารไม่ควบคุม

Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2304-0156OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 23TM375
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
20.0	20.0	20.0	0.48	0.42	1.2	2

Calibration Point	Measured Temperature (°C) Position									Uncertainty
(°C)	1	2	3	4	5	6	7	8	9 (ref.)	(±°C)
20.0	20.040	20.170	20.263	20.093	19.749	19.704	19.920	20.191	20.020	0.66

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

[redacted]

เอกสารไม่ควบคุม

a 1158258

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert.No.: 23MM112
Page.: 1 of 3

Certificate of Calibration

Equipment : Electronic Balance
Manufacturer : Mettler Toledo
Model : XSR205
Serial No. : C009071872
ID No. : UAE.WAO.012/2563
Submitted by : United Analyst and Engineering Consulant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phakhanong,
Bangkok 10260
Location : Balance Room
Received order : 26 April 2023
Calibration Date : 26 April 2023
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 90 %
Calibrated by : Man Pattanapongpaiboon
Approved by : [redacted]

( ) Pornthippa Tameyakul
( ) Malee Butkruea
(✓) Suwit Imjai

Issue Date : 2 May 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0459OC-1

Cert.No.: 23MM112

Procedure used :-

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0010-22	20 Jan 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This result of calibration was made on requested at the point specified by customer.
4. This certificate is not certified for any commercial transaction.
5. This certification is traceable to the International System of Unit.

Result of calibration ( ) Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity : 0 g to 81 g **Resolution** 0.00001 g
81 g to 220 g **Resolution** 0.0001 g

Before Adjustment :

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (*k*)
80	80.00005	-0.00005	0.15	2.00
200	199.9999	+0.0001	0.29	2.00

After Adjustment :

1. **Determination of the standard deviation of weighing machine** (n = 10)

Applied Weight (g)	Standard Deviation of Reading (g)
80	0.000007
200	0.00000

[redacted]

Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0459OC-1

Cert.No.: 23MM112

Result of calibration

2. **Effect of off center loading**

A mass of 100 g was placed to various position on the pan.
The weighing machine reading error obtained is given in the table



Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)	Maximum difference between off-center and central loading (g)
-0.0001	-0.0001	0.0000	-0.0001	-0.0001	0.0001

3. **Departure from nominal value**

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (*k*)
Unload	0.00000	0.00000	0.014	2.13
0.05	0.05001	-0.00001	0.015	2.09
0.1	0.10001	-0.00001	0.015	2.09
1	1.00001	-0.00001	0.018	2.04
5	5.00003	-0.00003	0.026	2.00
20	20.00006	-0.00006	0.045	2.00
50	50.00006	-0.00006	0.080	2.00
80	80.00004	-0.00004	0.15	2.00
100	100.0000	0.0000	0.16	2.00
150	150.0000	0.0000	0.29	2.00
200	200.0000	0.0000	0.29	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k*** , providing a level of confidence of approximately 95 %.

-o0o-

[redacted]

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484

ilac-MRA

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 22TM1490
Page : 1 of 3

Certificate of Calibration

Equipment :	Hot Air Oven
Manufacturer :	Memmert
Model :	UF 55
Serial No. :	B216.1666
ID No. :	UAE.WAO.027/2559
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Location :	Lab Floor 2
Received Order :	19 October 2022
Calibration Date :	19 October 2022
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Preecha Hlahib
Approved by :	[redacted]

( ) Pornthippa Tameyakul
( ) Malee Butkruea
(✓) Suwit Imjai

Issue Date : 31 October 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2210-0575OC-1

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY41021843	22LM4	10 Jan 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

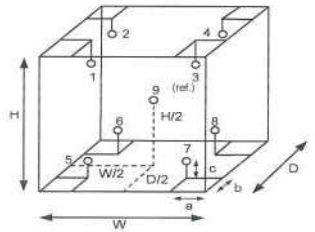

Environment during calibration		
	Beginning	Finished
Temp. (°C)	29	30
REL.Humid. (%)	47	40
AC Supply (Volt)	221	220

Probe Installation Details :

a =	5.0	cm
b =	5.0	cm
c =	5.0	cm

Dimension of Chamber :

D =	0.33	m
W =	0.40	m
H =	0.40	m
Capacity =	0.053	m³

Position :	Ref. Std. ID No.: @ Calibration Point (104) °C	(140,180) °C
1	18-04RTD-01	21-04TC-01
2	18-04RTD-02	21-04TC-02
3	18-04RTD-03	21-04TC-03
4	18-04RTD-04	21-04TC-04
5	18-04RTD-05	21-04TC-05
6	18-04RTD-06	21-04TC-06
7	18-04RTD-07	21-04TC-07
8	18-04RTD-08	21-04TC-08
9 (ref.)	18-04RTD-09	21-04TC-09

เอกส[redacted]

Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2210-0575OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 22TM1490
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (±°C)	Coverage Factor *k*
104.0	104.0	104.0	0.061	1.3	1.7	0.42	2
140.0	140.0	140.0	0.14	2.3	2.4	1.1	2
180.0	180.0	180.0	0.21	3.5	3.6	1.3	2

Calibration Point (°C)	Measured Temperature (°C) Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	103.076	103.876	103.777	104.124	104.667	104.426	104.012	103.928	104.370
140.0	138.199	139.189	138.808	139.550	140.266	139.622	139.293	139.385	140.369
180.0	177.930	179.267	178.643	179.753	181.011	180.093	179.496	179.743	181.278

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one senso
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

[redacted]

a 1133251

สถาบันพัฒนาอุตสาหกรรมเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2302827-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR204
Serial No.: C117635043
ID No.: UAE.WAS.012/2564
Order No.: 2302827
Operation No.: 2302827-001
Date of Receipt: 10 May 2023
Date of Calibration: 10 May 2023

Calibrated by Mr.Manas Somsak
Specialist

Approved by [redacted]
Manager, [redacted] atory
Responsible for the Technical Management Team

Date of Issue: 18 May 2023

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอุดมสุข 36 ถนนสุขุมวิท แขวงบางจักรี เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Ayun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2302827-001-01

Equipment: Electronic Balance — **Manufacturer:** METTLER TOLEDO

Model: XSR204 — **Resolution:** 0.0001 g

Serial No.: C117635043 — **ID No.:** UAE.WAS.012/2564

Capacity: 220 g

Date of Calibration: 10 May 2023

Environment Condition: Ambient Temperature 21.4 ± 0.2 °C Relative Humidity: 43.4 ± 0.9 %

Place of Calibration: Balance room (Water Analysis Unit), UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M2304053S	8 April 2024
Instrument	**Model**	**Serial No.**	**Calibrated By**	**Certificate No.**	**Due Date**
Thermo-Hygro Meter	608-H1	NFI.BTH 016/23	Quality Reborn	QR23-0489	21 February 2024

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
100	0.000032
200	0.000032

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.

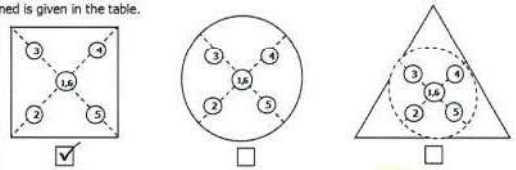

1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	6 (g)	(Maximum Difference) (g)
100.0002	100.0002	100.0002	100.0002	100.0003	100.0002	0.0001

[redacted]

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th
เอกสารไม่ควบคุม

สถาบันอาหาร
กระทรวงอุตสาหกรรม
สถาบันพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center
NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2302827-001-01

Equipment: Electronic Balance — **Manufacturer:** METTLER TOLEDO

Model: XSR204 — **Resolution:** 0.0001 g

Serial No.: C117635043 — **ID No.:** UAE.WAS.012/2564

Capacity: 220 g

Date of Calibration: 10 May 2023

Calibration Results: **(Continued)**

Calibration Range: 0 - 200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor *k*
Unload	0.00000	0.0000	0.0000	0.000085	2.00
0.01	0.01000	0.0100	0.0000	0.000085	2.00
0.02	0.02001	0.0200	0.0000	0.000085	2.00
0.05	0.05000	0.0500	0.0000	0.000085	2.00
0.1	0.10001	0.1000	0.0000	0.000085	2.00
0.2	0.20001	0.2000	0.0000	0.000085	2.00
0.5	0.50002	0.5000	0.0000	0.000085	2.00
1	1.00000	1.0000	0.0000	0.000086	2.00
2	2.00002	2.0000	0.0000	0.000086	2.00
3	3.00003	3.0000	0.0000	0.000087	2.00
5	5.00002	5.0000	0.0000	0.000087	2.00
10	10.00001	10.0000	0.0000	0.000088	2.00
20	20.00003	20.0000	0.0000	0.000092	2.00
30	30.00004	30.0000	0.0000	0.000098	2.00
40	40.00007	40.0000	0.0000	0.00011	2.00
45	45.00009	45.0001	0.0000	0.00013	2.00

[redacted]

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th
เอกสารไม่ควบคุม

สุรสาหกรรมอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: **2302827-001-01**

Equipment: Electronic Balance **Manufacturer:** METTLER TOLEDO

Model: XSR204 **Resolution:** 0.0001 g

Serial No.: C117635043 **ID No.:** UAE.WAS.012/2564

Capacity: 220 g

Date of Calibration: 10 May 2023 **Page 4 of 4**

Calibration Results: **(Continued)**

Calibration Range: 0 - 200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
50	50.00003	50.0000	0.0000	0.00011	2.00
55	55.00005	55.0000	0.0000	0.00012	2.00
60	60.00004	60.0000	0.0000	0.00012	2.00
65	65.00005	65.0000	0.0000	0.00013	2.00
70	70.00006	70.0001	-0.0001	0.00013	2.00
75	75.00008	75.0002	-0.0001	0.00013	2.00
80	80.00007	80.0002	-0.0001	0.00014	2.00
85	85.00009	85.0002	-0.0001	0.00014	2.00
90	90.00010	90.0002	-0.0001	0.00015	2.00
100	100.00006	100.0002	-0.0001	0.00016	2.00
120	120.00009	120.0002	-0.0001	0.00018	2.00
150	150.00009	150.0002	-0.0001	0.00021	2.00
200	200.00016	200.0003	-0.0001	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* providing a level of confidence of approximately 95 %.

[redacted]

---------- End ----------

F-CS-012 Revision: 01 Date: 20-04-65

2008 ถนนอรุณอมรินทร์ 36 แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

DQE Services

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025
CALIBRATION 0404

CERTIFICATE OF CALIBRATION

Certificate No. : SP23-021 Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009

ID No. : N/A

Received Date : 20 May 2023

Calibration Date : 20 May 2023

Issue Date : 23 May 2023

Condition Instrument : Good

Calibrated by : [redacted] Technical Manager

Approved by : [redacted] Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP23-021

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	95935	22 October 2023
Absobance Standard set	25757	95929	22 October 2023
Wavelength Standard set	25806	95916	22 October 2023
Wavelength Standard set	25758	95915	22 October 2023

Traceability This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP23-021

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5787	0.5742	0.0045	0.0031	2.00
	1.0490	1.0423	0.0067	0.0029	2.00
	2.1900	2.1847	0.0053	0.0075	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5607	0.5577	0.0030	0.0034	2.00
	1.0247	1.0234	0.0013	0.0035	2.00
	2.1229	2.1171	0.0058	0.0088	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5236	0.5184	0.0052	0.0029	2.00
	0.9634	0.9607	0.0027	0.0029	2.00
	1.9763	1.9715	0.0048	0.0081	2.00
546.1	0.0000	-0.0001	0.0001	0.0028	2.00
	0.5191	0.5159	0.0032	0.0031	2.00
	1.0003	0.9980	0.0023	0.0033	2.00
	1.9987	1.9917	0.0070	0.0087	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5523	0.5501	0.0022	0.0030	2.00
	1.0809	1.0808	0.0001	0.0030	2.00
	2.0391	2.0336	0.0055	0.0081	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5601	0.5585	0.0016	0.0031	2.00
	1.0512	1.0485	0.0027	0.0030	2.00
	1.9294	1.9317	-0.0023	0.0083	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP23-021

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7478	0.7436	0.0042	0.0058	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8686	0.8648	0.0038	0.0064	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2912	0.2908	0.0004	0.0052	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6448	0.6398	0.0050	0.0058	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP23-021

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor *k*
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.5	0.31	0.18	2.00
334.06	333.5	0.56	0.18	2.00
360.93	360.3	0.63	0.18	2.00
418.59	418.0	0.59	0.18	2.00
445.94	445.3	0.64	0.18	2.00
453.66	453.0	0.66	0.18	2.00
460.02	459.6	0.42	0.18	2.00
536.59	536.4	0.19	0.18	2.00
637.98	638.3	-0.32	0.18	2.00
431.38	431.0	0.38	0.18	2.00
472.50	472.5	0.00	0.18	2.00
513.47	513.5	-0.03	0.18	2.00
528.88	529.0	-0.12	0.18	2.00
573.17	573.0	0.17	0.18	2.00
585.35	585.0	0.35	0.20	2.00
684.40	684.5	-0.10	0.18	2.00
740.72	741.0	-0.28	0.20	2.00
748.55	748.5	0.05	0.18	2.00
807.03	807.0	0.03	0.18	2.00
879.28	879.5	-0.22	0.18	2.00

Remark : - UUC = Unit Under Calinration

- N/A = Not Avaiable
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*, which for a normal distribution corresponds to a coverage probability of approximately 95%
- * Indicates non TISI accredited

- End of Certificate -

FM-708-02 R01 1/11/2021

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

CERTIFICATE OF CALIBRATION

Certificate No. : SP23-007

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : Hitachi

Model : U-1900

Serial No. : 2021-064

ID No. : UAE.WAS.006/2552

Received Date : 6 January 2023

Calibration Date : 6 January 2023

Issue Date : 10 January 2023

Condition Instrument : Used

Calibrated by : [redacted] **Approved by :** [redacted]

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP23-007

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	95935	22 October 2023
Absobance Standard set	25757	95929	22 October 2023
Wavelength Standard set	25806	95916	22 October 2023
Wavelength Standard set	25758	95915	22 October 2023

Traceability This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 4.0 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP23-007

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5787	0.575	0.0037	0.0031	2.00
	1.0490	1.044	0.0050	0.0029	2.00
	2.1900	2.181	0.0090	0.0080	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5607	0.558	0.0027	0.0034	2.00
	1.0247	1.021	0.0037	0.0035	2.00
	2.1229	2.115	0.0079	0.0081	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5236	0.520	0.0036	0.0030	2.00
	0.9634	0.961	0.0024	0.0029	2.00
	1.9763	1.968	0.0083	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5191	0.518	0.0011	0.0031	2.00
	1.0003	1.000	0.0003	0.0033	2.00
	1.9987	1.993	0.0057	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5523	0.552	0.0003	0.0030	2.00
	1.0809	1.082	-0.0011	0.0030	2.00
	2.0391	2.031	0.0081	0.0080	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5601	0.562	-0.0019	0.0032	2.00
	1.0512	1.052	-0.0008	0.0030	2.00
	1.9294	1.923	0.0064	0.0079	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP23-007

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7478	0.743	0.0048	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8686	0.861	0.0076	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2912	0.291	0.0002	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6448	0.639	0.0058	0.0055	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP23-007

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor *k*
241.54	240.8	0.74	0.18	2.00
279.40	278.5	0.90	0.18	2.00
288.70	288.0	0.70	0.18	2.00
334.22	333.5	0.72	0.18	2.00
361.26	360.5	0.76	0.18	2.00
418.48	417.8	0.68	0.21	2.00
446.70	445.9	0.80	0.18	2.00
453.20	452.5	0.70	0.18	2.00
460.06	459.5	0.56	0.18	2.00
536.90	536.0	0.90	0.18	2.00
637.94	637.1	0.84	0.18	2.00
440.74	440.0	0.74	0.18	2.00
472.22	471.5	0.72	0.18	2.00
513.70	513.0	0.70	0.18	2.00
528.72	528.0	0.72	0.18	2.00
574.60	574.0	0.60	0.18	2.00
585.48	584.6	0.88	0.20	2.00
684.63	684.0	0.63	0.18	2.00
740.27	740.0	0.27	0.20	2.00
748.28	747.5	0.78	0.18	2.00
807.16	806.5	0.66	0.18	2.00
879.70	879.0	0.70	0.18	2.00

Remark : - UUC = Unit Under Calinration

- N/A = Not Avaiable
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*, which for a normal distribution corresponds to a coverage probability of approximately 95%
- * Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP)	Tisch Environmental,Inc.	TE-5025A 3383	Jiranatee Associates Co., Ltd.	CL-003-65	26 Jul 22	25 Jul 24	-
2	U-Tube Manometer	Total Suspended Particulate (TSP)	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	22P967	12 Aug 22	11 Aug 23	-
3	Aneroid Barometer	Total Suspended Particulate (TSP)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	22P2722	22 Jul 22	21 Jul 23	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	22H1583	22 Jul 22	21 Jul 23	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Workplace									
1	Flow Meter	Calibrate personal pump	TSI.Inc	4146 41461922007	Miracle International Technology Co.,Ltd.	L202209305-001	6 Oct 22	5 Oct 23	-
2	Aneroid Barometer	Total Dust	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	22P2724	22 Jul 22	21 Jul 23	-
3	Digital Thermo - Hygrometer	Total Dust	Testo, Germany	608-H1 34843033	Technology Promotion Association (Thailand-Japan)	22H1990	27 Sep 22	26 Sep 23	-

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	Horiba	LAQUA-PH210 HA1G0008	Technology Promotion Association (Thailand-Japan)	22CH1441	21 Oct 22	20 Oct 23	-

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department.

CERTIFICATE OF CALIBRATION

Certificate No. : CL-003-65

MEASUREMENT ITEM	: Top Load Orifice
MANUFACTURER	: Tisch Environmental, Inc.
MODEL/TYPE	: TE-5025A
SERIAL NUMBER	: 3383
ID NUMBER	: UAE.EFM.063/2560
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: United Analyst and Engineering Consultant Co.,Ltd. 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
RECEIVED DATE	: 15 Jul 2022
MEASUREMENT DATE	: 25 Jul 2022
ISSUE DATE	: 26 Jul 2022

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the VSL (National Metrology Institute of Netherlands) via Certificate number: G2211901

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:
Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 24.8 °C and 55.1 %RH.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol

Approved signatory: [redacted]
Calibration Department Manager

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR [redacted] HAS BEEN GRANTED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CL-003-65

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH_2O	Y	Standard Flow $[Q_s]$ m^3/min
1	0.697	754.265	24.640	23.960	55.399	1.699	1.299	0.643
2	1.000	754.236	24.950	24.350	62.172	3.444	1.849	0.913
3	1.118	754.323	24.730	24.210	41.925	4.582	2.133	1.051
4	1.169	754.212	24.640	24.160	31.045	5.150	2.262	1.116
5	1.416	754.175	24.480	24.210	30.117	7.629	2.754	1.353

Slope (m): **2.04804**
Intercept (b): **-0.01939**
Correlation coefficient (r): **0.99982**
Uncertainty ($k=2$): **0.011** m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH_2O	Y	Standard Flow $[Q_a]$ m^3/min
1	0.697	754.265	24.640	23.960	55.399	1.699	0.819	0.647
2	1.000	754.236	24.950	24.350	62.172	3.444	1.167	0.919
3	1.118	754.323	24.730	24.210	41.925	4.582	1.345	1.058
4	1.169	754.212	24.640	24.160	31.045	5.150	1.426	1.123
5	1.416	754.175	24.480	24.210	30.117	7.629	1.735	1.361

Slope (m): **1.28277**
Intercept (b): **-0.01223**
Correlation coefficient (r): **0.99982**
Uncertainty ($k=2$): **0.012** m^3/min

End of Certificate of Calibration

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No. : 22P967

Equipment :	U Tube Manometer
Manufacturer:	Dwyer
Model :	1221-36-W/M
Serial No.:	-
ID No.:	UAE.EFM.178/2561
Condition As-Received:	Used Item
Received Date:	03 August 2022
Calibration Date:	12 August 2022
Reference:	2208-0131WSC
Ambient Temperature:	(23 ± 2) °C
Relative Humidity:	(50 ± 15) %
Atmospheric Pressure:	1010 mbar

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1.Reference standards instuments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0113-22	14 Jul 2023

2.This result of calibration was made on requested at the point specified by customer.

3.Scale and conversion factor is 1 kPa = 4.0146293 inH_2O

4.This instrument was used clean air as pressure media.

5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suwit Aussarree
Issue Date : 14 August 2022

Approved Signatory [redacted]

[ ] Sura Suwannash
[/] Attapol Panurach

เอกสารไม่ควบคุม

B 0282414

Result of calibration:- Without adjustment **Range :** 0 inH_2O to 36 inH_2O
Function:- Pressure Measurement **Scale Interval :** 0.1 inH_2O(The Fifth Estimate)
Increasing Pressure

	UUC Indication			
Applied Pressure (inH_2O)	High-port side (inH_2O)	Low-port side (inH_2O)	ΔP (inH_2O)	Error (inH_2O)
0.00	0.00	0.00	0.00	0.00
2.00	0.98	-0.94	1.92	-0.08
4.00	2.00	-1.98	3.98	-0.02
6.00	3.00	-2.98	5.98	-0.02
8.00	4.00	-3.98	7.98	-0.02
10.00	5.00	-4.98	9.98	-0.02
12.00	6.02	-5.96	11.98	-0.02
14.00	7.02	-6.96	13.98	-0.02
16.00	8.04	-7.98	16.02	0.02
18.00	9.04	-8.98	18.02	0.02
20.00	10.04	-9.98	20.02	0.02
22.00	11.06	-10.98	22.04	0.04
24.00	12.06	-12.00	24.06	0.06
26.00	13.06	-13.00	26.06	0.06
28.00	14.08	-14.02	28.10	0.10
30.00	15.08	-15.02	30.10	0.10
32.00	16.08	-16.04	32.12	0.12
34.00	17.10	-17.04	34.14	0.14
35.80	17.90	-17.86	35.76	-0.04

The uncertainty of measurement was ± 0.11 inH_2O
* UUC = Unit Under Calibration
* ΔP = High-port side - Low-port side
The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-

เอกส[redacted]

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Certificate No. : 22P2722
Page : 1 of 2

Equipment : Aneroid Barometer
Manufacturer: Barigo
Model : -
Serial No.: -
ID No.: UAE.ANV.013/2547
Condition As-Received: Used Item
Received Date: 20 July 2022
Calibration Date: 22 July 2022

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Reference: 2207-0584WSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Atmospheric Pressure: 1010 mbar

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1.Reference standards instuments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505046	MP-0076-22	02 May 2023

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.
3.This result of calibration was made on requested at the point specified by customer.
4.Scale and conversion factor is 1 kPa = 7.50062 mmHg
5.This result of calibration instrument was in absolute pressure.
6.This instrument was used clean air as pressure media.
7.The certificate is valid only to the item calibrated on date and place of calibration.
8.This Certification is traceable to the International System of Unit maintained at:-
-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suwit Aussarree
Issue Date : 25 July 2022

Approved Signatory : [redacted]
Attapol Panurach

เอกสารไม่ควบคุม

B 0293205

Result of calibration:- Without adjustment **Range :** 720 mmHg to 780 mmHg
Function:- Absolute Pressure Measurement **Scale Interval :** 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	716.46	729.33	739.85	750.22	760.90	772.01	785.09
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	760.0	770.0	780.0
Error (mmHg)	1.54	0.67	0.15	-0.22	-0.90	-2.01	-5.89

Decreasing Pressure

Applied Pressure (mmHg)	785.90	771.99	760.85	750.17	739.90	729.57	718.62
UUC* Indication (mmHg)	780.0	770.0	760.0	750.0	740.0	730.0	720.0
Error (mmHg)	-5.90	-1.99	-0.85	-0.17	0.10	0.43	1.38

The uncertainty of measurement was ± 0.24 mmHg
* UUC = Unit Under Calibration
The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-

เอก[redacted]

a 1118533

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

ilac-MRA

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Certificate No. : 22H1583
Page : 1 of 2

Equipment :	Dial Thermo-Hygrometer
Manufacturer:	Barigo
Model :	-
Serial No.:	-
ID No.:	UAE.ANV.016/2547
Condition As-Received:	Used Item
Received Date:	20 July 2022
Calibration Date:	22 July 2022 to 27 July 2022
Reference:	2207-0586WSC
Ambient Temperature:	(25 ± 3) °C
Relative Humidity:	(50 ± 20) %

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instuments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Chilled Mirror Hygrometer Sensor	Dew Prime II	31863	19714	17 Sep 2022
2) Standard Humidity/Temperature Meter	400	10240757	TH-0125-21	13 Dec 2022

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Standards and Technology (NIST) , The United States of America

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Somchai Dumwor
Issue Date : 03 August 2022

Approved Signatory : [redacted]

[√] [redacted]
[ ] Pornthippa Tameyakul
[ ] Viporn Tantiyawutti

เอกสารไม่ควบคุม

B 0293719

Result of Calibration:- Without Adjustment
Function: Humidity measurement.

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	42	1.9	1.6
25.0	60.0	63	3.0	1.8
25.0	80.0	78	-2.0	2.0

Result of Calibration:- Without Adjustment
Function: Temperature measurement.

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
20.00	20.0	0.00	0.72
30.01	30.0	-0.01	0.72
35.04	35.0	-0.04	0.72
39.98	40.0	0.02	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-o0o-

[redacted]

เอกสารไม่ควบคุม

a 1119777

MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD
214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 http://www.mit.in.th

NSC-TISI-TIS 17025 CALIBRATION 0052

CALIBRATION CERTIFICATE

Certificate No. : L202209305-001
Date Issued : 31-Oct-22

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41,Sukhumvit Road,Bangchak,Phrakanong,Bangkok 10260

Equipment : Primary Air Flow Meter

Manufacturer : TSI
Model : 4146 F
Serial No. : 41461922007
ID No./Tag No. : UAE.EFM.223/2562
Date Received : 27-Sep-22
Date Calibrated : 06-Oct-22

Calibrated by : Mr. Jame Khaothong

Calibration Method or Calibration Procedure Used

In-house method : CP-26 by comparison against Bell Prover.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor k = 2, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by [redacted]

CERTIFIED MIT

เอกสารไม่ควบคุม

Certificate No. : L202209305-001

Environment : Ambient temperature : (23 ± 2)°C
Relative humidity : (50 ± 15)%RH

Capacity Range : 20 l/min

Calibration Media : Air

Type : Mass Flowmeter

UUC Reference Condition : Pressure 101.325 kPa(abs) , 21.1 °C , Air

Measurement Gas Flow rate function

Temperature (°C)	Pressure (kPa)	UUC (l/min)	STD (l/min)	Error (l/min)	Uncertainty (± l/min)
22.96	101.20	1.000	0.9716	0.0284	0.0035
23.16	101.29	1.700	1.6620	0.0380	0.0059
23.57	101.33	2.000	1.9505	0.0495	0.0069
23.22	101.45	3.000	2.9166	0.0834	0.0078
22.89	101.66	4.000	3.911	0.089	0.011
23.17	101.91	5.000	4.890	0.110	0.015

Error = Unit Under Calibration - Standard

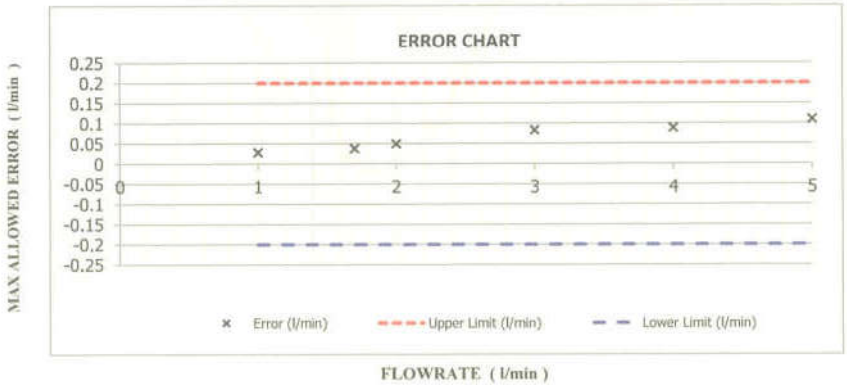

Note : Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{Meas} = Q_{Ref} \times \frac{P_{Ref}}{P_{Meas}} \times \frac{T_{Meas}}{T_{Ref}}$$

where Q = Flow rate P = Absolute pressure T = Absolute temperature
M = Gas molecular weight , Mstandard (Air) = 28.9646431 g/mol
Subscript "Meas" = Measurement condition
Subscript "Standard" = Standard condition

เอกสารไม่ควบคุม

Certificate No. : L202209305-001

Condition As-Received : Used Item

The measurment results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Calibration Certificate No. AD2204-030-0002 for Bell Prover Volume (60L) Serial No. 9511HC028626, Due 11-Apr-24

MIT Calibration Certificate No. L2022-08263-001 for Bell Prover Timer Serial No. 9511HC028626, Due 09-Aug-23

MIT Calibration Certificate No. AD2205-300-0001 for Temperature Transmitter with probe Serial No. MIT-STD-122, Due 04-Jun-23

MIT Calibration Certificate No. AD2205-300-0002 for Pressure Transmitter with indicator Serial No. MIT-STD-123, Due 04-Jun-23

End of Certificate

เอกสารไม่ควบคุม

MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD
214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 http://www.mit.in.th

ilac-MRA

ISO/IEC 17025 CALIBRATION 0052

CALIBRATION CERTIFICATE

Certificate No. : L202211085-001

Date Issued : 18-Nov-22

Customer	:	United Analyst and Engineering Consultant Co.,Ltd. 81 Soi Udomsuk 41,Sukhumvit Road,Bangchak,Phrakanong,Bangkok 10260
Equipment	:	Primary Air Flow Meter
Manufacturer	:	TSI
Model	:	4146 F
Serial No.	:	4146 1922 007
ID No./Tag No.	:	UAE.EFM.223/2562
Date Received	:	10-Nov-22
Date Calibrated	:	17-Nov-22
Calibrated by	:	Mr. Jame Khaothong

Calibration Method or Calibration Procedure Used

In-house method : CP-26 by comparison against Bell Prover.
In-house method : CP-44 by comparison against Piston Prover.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor k = 2, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: [redacted]

CERTIFIED MIT

เอกสารไม่ควบคุม

Environment : Ambient temperature : (23 ±2) °C

Relative humidity : (50 ±15) % RH

Capacity Range : 20000 ml/min

Calibration Media : Air

UUC Reference Condition : Pressure 101.325 kPa @ 21.1 °C , Air

Temperature (°C)	Pressue (kPa)	Flow Rate Reading (ml/min) UUC Reading	STD Reading	Error (ml/min)	Uncertainty (ml/min)
23.330	100.62	0.0	0.000 *	0.000	0.58
23.192	101.34	20.00	20.992	-0.992	0.58
23.142	101.32	50.0	49.830	0.170	0.75
23.223	101.31	100.0	98.200	1.800	1.1
23.162	101.32	200.0	195.182	4.818	1.2
23.11	101.11	500.0	495.900	4.100	2.6

Error = Unit Under Calibration - Standard

Marked * are not included in the TISI accreditation schedule for our laboratory.

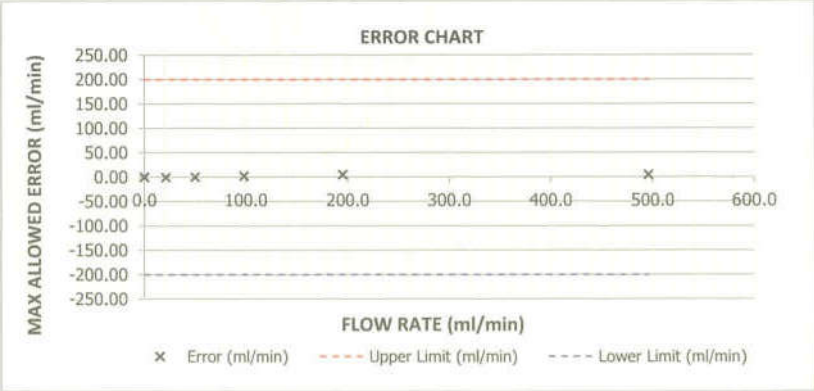

เอกสารไม่ควบคุม

Certificate No. : L202211085-001

Note : The actual flow rate is determined by the equation :

$$Q_{Meas} = Q_{Ref} \times \frac{P_{Ref}}{P_{Meas}} \times \frac{T_{Meas}}{T_{Ref}}$$

; Q = Flow rate

; P = Absolute pressure

; T = Absolute temperature

; Subscript "Meas" = Measurement condition

; Subscript "Ref" = Reference condition

Condition As-Received : Used Item

The measurment results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used :

MIT Calibration Certificate No. AD2204-030-0002 for Bell Prover Volume (60L) Serial No. 9511HC028626, Due 11-Apr-24

MIT Calibration Certificate No. L2022-08263-001 for Bell Prover Timer Serial No. 9511HC028626, Due 09-Aug-23

MIT Calibration Certificate No. AD2205-300-0001 for Temperature Transmitter with probe Serial No. MIT-STD-122, Due 04-Jun-23

MIT Calibration Certificate No. AD2205-300-0002 for Pressure Transmitter with indicator Serial No. MIT-STD-123, Due 04-Jun-23

MIT Calibration Certificate No. AD2205-312-0001 for Piston Prover Volume Serial No. 85, Due 20-May-24

MIT Calibration Certificate No. AD2202-261-0002 for Piston Prover Timer Serial No. 122199, Due 03-Mar-24

MIT Calibration Certificate No. AD2202-261-0003 for Absolute Pressure (Piston Prover) Serial No. 220368, Due 22-Feb-24

MIT Calibration Certificate No. AD2202-261-0004 for Temperature Indicator with Sensor (Piston Prover) Serial No. MIT-STD-258, Due 02-Mar-24

End of Certificate

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Certificate No. : 22P2724
Page : 1 of 2

Equipment :	Aneroid Barometer
Manufacturer:	Barigo
Model :	111MS
Serial No.:	-
ID No.:	UAE.EMA2.067/2552
Condition As-Received:	Used Item
Received Date:	20 July 2022
Calibration Date:	22 July 2022
Reference:	2207-0584WSC
Ambient Temperature:	(23 ± 2) °C
Relative Humidity:	(50 ± 15) %
Atmospheric Pressure:	1010 mbar

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1.Reference standards instuments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505046	MP-0076-22	02 May 2023

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.
3.This result of calibration was made on requested at the point specified by customer.
4.Scale and conversion factor is 1 kPa = 7.50062 mmHg
5.This result of calibration instrument was in absolute pressure.
6.This instrument was used clean air as pressure media.
7.The certificate is valid only to the item calibrated on date and place of calibration.
8.This Certification is traceable to the International System of Unit maintained at:-
-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suwit Aussarree
Issue Date : 25 July 2022

Approved Signatory [redacted]
[ ] Sura Suwannasri
[/] Attapol Panurach

เอกสารไม่ควบคุม

B 0293207

Cert.No.: 22P2724
Page: 2 of 2

Result of calibration:- Without adjustment Range : 720 mmHg to 780 mmHg
Function:- Absolute Pressure Measurement Scale Interval : 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	717.10	727.91	738.89	749.35	759.90	771.01	783.02
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	760.0	770.0	780.0
Error (mmHg)	2.84	2.09	1.11	0.65	0.10	-1.01	-3.82

Decreasing Pressure

Applied Pressure (mmHg)	783.79	770.96	759.88	749.29	738.71	727.84	717.11
UUC* Indication (mmHg)	780.0	770.0	760.0	750.0	740.0	730.0	720.0
Error (mmHg)	-3.79	-0.96	0.12	0.71	1.29	2.16	2.89

The uncertainty of measurement was ± 0.24 mmHg
* UUC = Unit Under Calibration
The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-

[redacted]

เอกสารไม่ควบคุม

a 1118531

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

ilac-MRA

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Certificate No. : 22H1990
Page : 1 of 2

Equipment :	Digital Thermo-Hygrometer
Manufacturer:	Testo
Model :	608-H1
Serial No.:	34843033
ID No.:	UAE.ANV.135/2550
Condition As-Received:	Used Item
Received Date:	21 September 2022
Calibration Date:	23 September 2022 to 27 September 2022
Reference:	2209-0729WSC
Ambient Temperature:	(25 ± 3) °C
Relative Humidity:	(50 ± 20) %

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instuments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Hygro-M2 Dew Point Monitor	5112	2360195	20703	02 Aug 2023
2) Standard Humidity/Temperature Meter	400	10240757	TH-0125-21	13 Dec 2022

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Standards and Technology (NIST) , The United States of America

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Viporn Tantiyawutti
Issue Date : 29 September 2022

Approved Signatory : [redacted]

[ ] Pornthippa Tameyakul
[ ] Viporn Tantiyawutti

เอกสารไม่ควบคุม

B 0298131

Result of Calibration:- Without Adjustment
Function: Humidity measurement.

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	44.7	4.6	1.3
25.0	50.1	53.4	3.3	1.6
25.0	60.0	62.7	2.7	1.6
25.0	70.2	71.9	1.7	1.6

Result of Calibration:- Without Adjustment
Function: Temperature measurement.

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
15.02	15.1	0.08	0.42
20.03	20.0	-0.03	0.42
25.02	25.0	-0.02	0.42
30.03	29.9	-0.13	0.42
40.03	39.7	-0.33	0.42

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-o0o-

[redacted]

เอกสารไม่ควบคุม

a 1128756

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert.No.: 22CH1441
Page.: 1 of 3

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Horiba
Model :	LAQUA-PH210
Serial No. :	HA1G0008
ID No. :	UAE.EFM.201/2564(EFM.pH.09/64)
Condition As-Received:	Used Item
Received Date :	20 October 2022
Calibration Date :	21 October 2022
Reference :	2210-0694WSC-2
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer
Calibrated by :	Walalak Sirithean
Approved by :	[redacted]

(✓) Malee Butkruea
( ) Saithip Meangmai
( ) Warakorn Lerngagtrakul

Issue Date : 26 October 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0046602

Cert.No.: 22CH1441
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	22E2769	24 Aug 2023
2) Ref. Standard Thermometer	4982054	110RC044	21I1201	26 Oct 2022

This certification is traceable to the International System of Unit maintained at:-
- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	788995	01 Jan 2024
pH 6.987	CPA chem	823322	20 June 2023
pH 10.008	CPA chem	823323	20 June 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	*k*
pH Meter	4.00	177.48	177.5	4.01	0.058	2.00
S/N.: HA1G0008	7.00	0.00	0.0	7.02	0.058	2.00
	7.00	0.00	0.0	7.02	0.058	2.00
	10.00	-177.48	-177.5	10.01	0.058	2.00

[redacted]

เอกสารไม่ควบคุม

a 1132040

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor *k*
pH Electrode	4.008	4.01	144.6	0.0085	2.05
S/N.: 991F0169	6.987	6.99	-28.3	0.011	2.00
	6.987	7.00	-28.7	0.011	2.00
	10.008	10.01	-203.3	0.0085	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652
- Serial No. : 991F0169

Dimension of probe;

- Length : 103 mm.
- Diameter : 16 mm.
- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor *k*
25.0	25.000	24.9	-0.100	0.13	2.00
30.0	30.001	29.9	-0.101	0.13	2.00
35.0	34.999	34.9	-0.099	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

[redacted]

เอกสารไม่ควบคุม