

## ภาคผนวกที่ 4

เอกสารการสอบเทียบความถูกต้องของเครื่องมือ

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
<b>คุณภาพอากาศในบรรยากาศ</b>		
TSP	High Volume Air Sampler No. R02, R04, R13, R16	Digital Balance
PM <sub>10</sub>	High Volume PM <sub>10</sub> Air Sampler No. R03, R11, R12, R13	Digital Balance
HCl	Gas Sampler Box No. B05, B06, B07, B09	Ion Chromatography (IC)
H <sub>2</sub> SO <sub>4</sub>	Gas Sampler Box No. B05, B06, B07, B09	Ion Chromatography (IC)
NO <sub>2</sub>	NO <sub>2</sub> Analyzer No. R01, R03, R10, R11	NO <sub>2</sub> Analyzer No. R01, R03, R10, R11
SO <sub>2</sub>	SO <sub>2</sub> Analyzer No. R02, R04, R08, R07	SO <sub>2</sub> Analyzer No. R02, R04, R08, R07
<b>คุณภาพอากาศจากปล่อง</b>		
TSP	Console No. B04, R04, R05 Pitot Tube No. B47, B58	Digital Balance
SO <sub>2</sub>	Personal Pump No. B04, R04, R05 Rotameter No. R03, R02	-
NO <sub>x</sub>	Vacuum Gauge	Spectrophotometer
H <sub>2</sub> SO <sub>4</sub>	Console No. R03, R04 Pitot Tube No. B47, B58	-
HCl	Console No. R03, R04 Pitot Tube No. B47, B48	Ion Chromatography (IC)
<b>ระดับเสียงในบรรยากาศ</b>		
L <sub>eq</sub> 24 hr, L <sub>90</sub>	Acoustic Calibrator Integrated Sound Level Meter No. CIRRU-S-B01,B02, B03, B06, B07, B08, B010	-
<b>คุณภาพน้ำ</b>		
pH	-	pH Meter
Temperature	-	Thermometer
TDS	-	Digital Balance
Conductivity	-	Conductivity Meter
BOD <sub>5</sub>	-	BOD Analyzer
COD	-	COD Reactor
SS	-	Digital Balance
Grease & Oil	-	Digital Balance
Zn	-	Inductive Coupled Plasma (ICP)
Al	-	Inductive Coupled Plasma (ICP)
Iron	-	Inductive Coupled Plasma (ICP)

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม (ต่อ)

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
ระดับความร้อน WBGT	Heat Stress WBGT Meter No. R06,R08,B17	-
คุณภาพอากาศในสถานประกอบการ Total Dust	Personal Pump No. R22, R33 Rotameter No. H-R04	Digital Balance
HCl	Personal Pump No. R39 Rotameter No. L- R04	Ion Chromatography (IC)
H <sub>2</sub> SO <sub>4</sub>	Personal Pump No. R37 Rotameter No. L- R04	Ion Chromatography (IC)
Zinc Oxide Fume	Personal Pump No. R25 Rotameter No. H - R04	Inductive Coupled Plasma (ICP)
ระดับเสียงในสถานประกอบการ L <sub>eq</sub> 8 hr, L <sub>eq</sub> 12 hr, L <sub>90</sub>	Acoustic Calibrator Integrated Sound Level Meter No. ACO- B18, B29, B33, B36	-
Noise Dose	Noise Dose Meter No.NMD-B02, B03, B04, B08, B09, B10, B11, B12, B13, B19, R22, R26, R27, R35	-

คุณภาพอากาศในบรรยากาศ





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

## High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

### Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
B35	B35	01/02/2023	y = 1.194x-4.992	0.995
B36	B36	02/02/2023	y = 1.201x-3.946	0.997
B37	B37	02/02/2023	y = 1.284x-6.745	0.997
B38	B38	02/02/2023	y = 1.250x-6.733	0.998
B39	B39	01/02/2023	y = 1.268x-7.186	0.998
B40	B40	03/02/2023	y = 1.214x-4.324	0.998
B41	B41	03/02/2023	y = 1.176x-2.734	0.999
B42	B42	02/02/2023	y = 1.283x-8.167	0.997
B43	B43	02/02/2023	y = 1.197x-3.772	0.996
B44	B44	02/02/2023	y = 1.249x-7.038	0.995
R01	R01	01/02/2023	y = 1.287x-8.462	0.998
R02	R02	01/02/2023	y = 1.239x-6.678	0.998
R03	R03	03/02/2023	y = 1.254x-7.928	0.999
R04	R04	02/02/2023	y = 1.206x-3.694	0.999
R05	R05	02/02/2023	y = 1.237x-6.503	0.997
R06	R06	02/02/2023	y = 1.239x-4.541	0.995
R07	R07	03/02/2023	y = 1.060x+1.983	0.999
R08	R08	03/02/2023	y = 1.274x-8.050	0.998
R09	R09	02/02/2023	y = 1.280x-7.005	0.998
R10	R10	03/02/2023	y = 1.244x-5.980	1.000
R11	R11	03/02/2023	y = 1.097x-0.462	0.998
R12	R12	02/02/2023	y = 1.151x-2.727	0.995
R13	R13	02/02/2023	y = 1.134x-1.526	1.000
R14	R14	02/02/2023	y = 1.172x-2.510	0.999
R15	R15	01/02/2023	y = 1.131x-2.129	0.998
R16	R16	01/02/2023	y = 1.202x-5.830	0.998
R17	R17	01/02/2023	y = 1.182x-3.281	0.998
R18	R18	03/02/2023	y = 1.217x-5.060	0.999
R19	R19	03/02/2023	y = 1.228x-6.084	0.998
R20	R20	03/02/2023	y = 1.277x-9.434	0.997

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

### Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
R01	R01	01/02/2023	y = 1.253x-8.016	0.996
R02	R02	01/02/2023	y = 1.246x-5.052	0.998
R03	R03	02/02/2023	y = 1.239x-5.451	0.999
R04	R04	03/02/2023	y = 1.263x-8.320	0.999
R05	R05	03/02/2023	y = 1.193x-4.904	0.998
R06	R06	03/02/2023	y = 1.270x-7.534	0.995
R07	R07	03/02/2023	y = 1.244x-5.727	0.998
R08	R08	02/02/2023	y = 1.277x-7.820	0.998
R09	R09	02/02/2023	y = 1.183x-5.015	0.996
R10	R10	01/02/2023	y = 1.200x-4.576	0.999
R11	R11	01/02/2023	y = 1.225x-4.833	0.995
R12	R12	03/02/2023	y = 1.273x-8.109	0.998
R13	R13	01/02/2023	y = 1.281x-6.830	1.000
R14	R14	01/02/2023	y = 1.288x-7.622	0.999
R15	R15	02/02/2023	y = 1.282x-8.311	0.997
R16	R16	02/02/2023	y = 1.246x-5.817	0.995
R17	R17	03/02/2023	y = 1.263x-7.123	0.999
R18	R18	03/02/2023	y = 1.203x-5.483	0.999
R19	R19	01/02/2023	y = 1.204x-4.399	0.996
R20	R20	01/02/2023	y = 1.259x-8.655	0.997

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## Gas Sampler Box Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Dry Cal DCL-ML

S/N : 136164

### Calibration Data

Gas Sampler Data		Calibration Data					
No.	Rotameter	Date	Setting (Constant Flow) (ml/min)	Actual Flow Rate (ml/min)			
				Sampling Line A		Sampling Line B	
				Normal Condition	Standard Condition	Normal Condition	Standard Condition
B01	2 (A&B)	01/03/2023	200	200.4	199.0	200.6	199.1
B02	2 (A&B)	01/03/2023	200	200.5	199.1	200.7	199.2
B03	2 (A&B)	01/03/2023	200	200.4	199.0	200.8	199.3
B04	2 (A&B)	02/03/2023	200	200.5	199.1	200.4	199.0
B05	2 (A&B)	01/03/2023	200	200.7	199.2	200.9	199.4
B06	2 (A&B)	03/03/2023	200	200.8	199.4	200.5	199.1
B07	2 (A&B)	03/03/2023	200	200.7	199.2	200.4	199.0
B08	2 (A&B)	03/03/2023	200	200.5	199.1	200.5	199.1
B09	2 (A&B)	03/03/2023	200	200.7	199.2	200.7	199.3
B10	2 (A&B)	01/03/2023	200	200.4	199.0	200.5	199.1
B11	2 (A&B)	02/03/2023	200	200.6	199.1	200.7	199.2
B12	2 (A&B)	02/03/2023	200	200.5	199.0	200.5	199.1
B13	2 (A&B)	01/03/2023	200	200.6	199.1	200.4	199.0
B14	2 (A&B)	03/03/2023	200	200.7	199.3	200.5	199.1
B15	2 (A&B)	03/03/2023	200	200.4	199.0	200.4	199.0
B16	2 (A&B)	03/03/2023	200	200.6	199.1	200.5	199.1
B17	2 (A&B)	01/03/2023	200	200.5	199.0	200.7	199.3

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## CALIBRATION REPORT

### CHEMILUMINESCENT NO / NO<sub>2</sub> / NO<sub>x</sub> ANALYZER

DATE : 30 April 2023 BRAND : API MODEL : 200E  
NO. NOX-R01 SERIAL NO. 769

#### Calibrator (Dilution System)

Brand : API Model : 700  
Last Cal. Date : 04 August 2022 Serial No. : 911

#### Reference Standard Gas

Standard Gas : Nitric Oxide (NO) Cylinder No. : D636192  
Certified Date : 20 April 2022 Expired Date : 20 April 2024 Cylinder Conc. : 49.1 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.5 °C % RH 48

#### CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	399.8	-0.050	400.0	1.007
NO <sub>x</sub> Span	400	400.2	0.050	400.0	1.011

#### API Model 200E NO<sub>x</sub> Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	505	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	102.9	mV	-20 - 150
AZERO	93.7	mV	-20 - 150
HVPS	674	V	420 - 900 constant
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.2	°C	8 - 48
PMT TEMP	7.1	°C	7 ± 2
MOLY TEMP	315.1	°C	315 ± 5
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000
NO Slope	1.007	-	1.0 ± 0.3
NO <sub>x</sub> Slope	1.011	-	1.0 ± 0.3
NO Offset	1.2	mV	-20 to +150
NO <sub>x</sub> Offset	0.8	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT						
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER						
DATE :	30 April 2023	BRAND :	API	MODEL :	200E	
NO.	NOX-R03	SERIAL NO.	4410			
Calibrator (Dilution System)						
Brand	: API			Model	: 700	
Last Cal. Date	: 04 August 2022			Serial No.	: 911	
Reference Standard Gas						
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: D636192	
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024	Cylinder Conc.	: 49.1 ppm	
CALIBRATING CONDITION						
Pressure	1011	mmbar	Temp.	24.5	°C	
% RH						48
CALIBRATION SETTING						
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB		
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope	
Zero	0	-0.10	-	0	-	
NO Span	400	400.1	0.025	400.0	1.008	
NO <sub>x</sub> Span	400	400.2	0.050	400.0	1.012	
API Model 200E NO <sub>x</sub> Analyzer Check List						
Test Values	Observed Value	Units	Nominal Range			
RANGE	500	PPB	500 standard			
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air			
SAMPLE FLOW	504	cc/min	500 ± 50			
OZONE FLOW	78	cc/min	80 ± 15			
PMT	103.2	mV	-20 - 150			
AZERO	93.9	mV	-20 - 150			
HVPS	670	V	420 - 900 constant			
RCELL TEMP	50.5	°C	50 ± 1			
BOX TEMP	29.3	°C	8 - 48			
PMT TEMP	7.4	°C	7 ± 2			
MOLY TEMP	314.9	°C	315 ± 5			
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant			
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant			
NO Span Conc	400	PPB	20 - 20,000			
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000			
NO Slope	1.008	-	1.0 ± 0.3			
NO <sub>x</sub> Slope	1.012	-	1.0 ± 0.3			
NO Offset	1.4	mV	-20 to +150			
NO <sub>x</sub> Offset	0.9	mV	-20 to 150			
Stability at Zero	0.1	PPB	< 0.2			
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas			

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

## CALIBRATION REPORT

### CHEMILUMINESCENT NO / NO<sub>2</sub> / NO<sub>x</sub> ANALYZER

DATE : 30 April 2023

BRAND : API

MODEL : 200E

NO. NOX-R10

SERIAL NO. 1991

#### Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 04 August 2022

Serial No. : 911

#### Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : D636192

Certified Date : 20 April 2022

Expired Date : 20 April 2024

Cylinder Conc. : 49.1 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.5 °C

% RH 48

#### CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	400.1	0.025	400.0	1.010
NO <sub>x</sub> Span	400	400.4	0.100	400.0	1.015

#### API Model 200E NO<sub>x</sub> Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	512	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	103.4	mV	-20 - 150
AZERO	94.1	mV	-20 - 150
HVPS	673	V	420 - 900 constant
RCELL TEMP	50.2	°C	50 ± 1
BOX TEMP	29.4	°C	8 - 48
PMT TEMP	7.0	°C	7 ± 2
MOLY TEMP	314.7	°C	315 ± 5
RCELL PRESS	8.5	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.7	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000
NO Slope	1.010	-	1.0 ± 0.3
NO <sub>x</sub> Slope	1.015	-	1.0 ± 0.3
NO Offset	1.7	mV	-20 to +150
NO <sub>x</sub> Offset	1.0	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

## CALIBRATION REPORT

### CHEMILUMINESCENT NO / NO<sub>2</sub> / NO<sub>x</sub> ANALYZER

DATE : 30 April 2023

BRAND : API

MODEL : 200E

NO. NOX-R11

SERIAL NO. 2621

#### Calibrator (Dilution System)

Brand	: API	Model	: 700
Last Cal. Date	: 04 August 2022	Serial No.	: 911

#### Reference Standard Gas

Standard Gas	: Nitric Oxide (NO)	Cylinder No.	: D636192
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024
		Cylinder Conc.	: 49.1 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.5 °C % RH 48

#### CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.6	-0.100	400.0	1.005
NO <sub>x</sub> Span	400	399.9	-0.025	400.0	1.008

#### API Model 200E NO<sub>x</sub> Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	509	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	103.1	mV	-20 - 150
AZERO	94.0	mV	-20 - 150
HVPS	675	V	420 - 900 constant
RCELL TEMP	50.1	°C	50 ± 1
BOX TEMP	29.5	°C	8 - 48
PMT TEMP	7.2	°C	7 ± 2
MOLY TEMP	315.3	°C	315 ± 5
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000
NO Slope	1.005	-	1.0 ± 0.3
NO <sub>x</sub> Slope	1.008	-	1.0 ± 0.3
NO Offset	1.1	mV	-20 to +150
NO <sub>x</sub> Offset	0.7	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO <sub>2</sub> FLUORESCENT ANALYZER					
DATE :	30 April 2023	BRAND :	API	MODEL :	100E
NO.	SO <sub>2</sub> -R02	SERIAL NO.	3431		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 04 August 2022		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO <sub>2</sub> )		Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 50.0 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH	48				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
SO <sub>2</sub> Span	400.0	399.9	-0.025	400.0	1.008
API Model 100E SO <sub>2</sub> Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.5	in-Hg	25-35		
SAMPLE FLOW	657	cc/min	650 ± 10%		
PMT	103.1	mV	-20-150 with Zero Air		
UV LAMP	3027.6	mV	1000-4900		
STR. LGT	61.6	PPB	<100		
DRK PMT	63.1	mV	-50 - 200		
DRK LMP	57.9	mV	-50 - 200		
HVPS	673	V	550-900 constant		
DCPS	2515	mV	2500 ± 200		
RCELL TEMP	50.2	°C	50 ± 1		
BOX TEMP	29.1	°C	5-40		
PMT TEMP	7.5	°C	7 ± 2.0		
SO <sub>2</sub> Span Conc	400	PPB	20-20,000		
SO <sub>2</sub> Slope	1.008	-	1.0 ± 0.3		
SO <sub>2</sub> Offset	21.7	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO <sub>2</sub> FLUORESCENT ANALYZER					
DATE :	30 April 2023	BRAND :	API	MODEL :	100E
NO.	SO <sub>2</sub> -R04	SERIAL NO.	3489		
Calibrator (Dilution System)					
Brand	: API			Model	: 700
Last Cal. Date	: 04 August 2022			Serial No.	: 911
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO <sub>2</sub> )			Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 50.0 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH 48					
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO <sub>2</sub> Span	400.0	400.3	0.075	400.0	1.014
API Model 100E SO <sub>2</sub> Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.4	in-Hg	25-35		
SAMPLE FLOW	655	cc/min	650 ± 10%		
PMT	103.2	mV	-20-150 with Zero Air		
UV LAMP	3018.4	mV	1000-4900		
STR. LGT	61.5	PPB	<100		
DRK PMT	62.9	mV	-50 - 200		
DRK LMP	57.8	mV	-50 - 200		
HVPS	671	V	550-900 constant		
DCPS	2522	mV	2500 ± 200		
RCELL TEMP	50.4	°C	50 ± 1		
BOX TEMP	29.3	°C	5-40		
PMT TEMP	7.2	°C	7 ± 2.0		
SO <sub>2</sub> Span Conc	400	PPB	20-20,000		
SO <sub>2</sub> Slope	1.014	-	1.0 ± 0.3		
SO <sub>2</sub> Offset	21.9	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO <sub>2</sub> FLUORESCENT ANALYZER					
DATE :	30 April 2023	BRAND :	TELEDYNE	MODEL :	TML-60
NO.	SO <sub>2</sub> -R07	SERIAL NO.	TRS1068		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 04 August 2022		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO <sub>2</sub> )		Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 50.0 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
			% RH	48	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO <sub>2</sub> Span	400.0	399.8	-0.050	400.0	1.006
API Model TML-60 SO <sub>2</sub> Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.7	in-Hg	25-35		
SAMPLE FLOW	654	cc/min	650 ± 10%		
PMT	103.3	mV	-20-150 with Zero Air		
UV LAMP	3042.1	mV	1000-4900		
STR. LGT	61.8	PPB	<100		
DRK PMT	63.3	mV	-50 - 200		
DRK LMP	58.2	mV	-50 - 200		
HVPS	670	V	550-900 constant		
DCPS	2519	mV	2500 ± 200		
RCELL TEMP	50.1	°C	50 ± 1		
BOX TEMP	29.4	°C	5-40		
PMT TEMP	7.3	°C	7 ± 2.0		
SO <sub>2</sub> Span Conc	400	PPB	20-20,000		
SO <sub>2</sub> Slope	1.006	-	1.0 ± 0.3		
SO <sub>2</sub> Offset	22.2	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO <sub>2</sub> FLUORESCENT ANALYZER					
DATE :	30 April 2023	BRAND :	TELEDYNE	MODEL :	TML-60
NO.	SO <sub>2</sub> -R08	SERIAL NO.	TRS1064		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 04 August 2022		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO <sub>2</sub> )		Cylinder No.	: A00814SK	
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 50.0 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH	48				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO <sub>2</sub> Span	400.0	400.1	0.025	400.0	1.012
API Model TML-60 SO <sub>2</sub> Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.6	in-Hg	25-35		
SAMPLE FLOW	658	cc/min	650 ± 10%		
PMT	103.0	mV	-20-150 with Zero Air		
UV LAMP	3048.5	mV	1000-4900		
STR. LGT	61.7	PPB	<100		
DRK PMT	63.0	mV	-50 - 200		
DRK LMP	58.1	mV	-50 - 200		
HVPS	669	V	550-900 constant		
DCPS	2527	mV	2500 ± 200		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.5	°C	5-40		
PMT TEMP	7.1	°C	7 ± 2.0		
SO <sub>2</sub> Span Conc	400	PPB	20-20,000		
SO <sub>2</sub> Slope	1.012	-	1.0 ± 0.3		
SO <sub>2</sub> Offset	22.1	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 23M2441

REFERENCE No : 68471-1

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS105DU

**SERIAL No** : 1126422905


**ID No** : BA 05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 10-Mar-23

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 16-Mar-23

**RECEIVED DATE** : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 23M2441

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 10-Mar-23  
AMBIENT TEMPERATURE : 23° C  $\pm$  1° C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





## Certificate of Calibration

**Aquion : Anion (ID#894)**

This certificate is to verify that instrument below are calibrated  
by Archemica Lab Co.,Ltd.

AQUION S/N : 190840059

AS-DV S/N : 190915235

for

**S.P.S. Consulting Service Co., Ltd.**



Operator Signature : \_\_\_\_\_

Date : Jan 5, 2022

(Mr. Channarong Khiao-Un)

Test Engineer

คุณภาพอากาศจากปล่อง



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## Console Calibration Report

Calibration Method

Critical Orifices

### Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	DH <sub>@</sub> (mmH <sub>2</sub> O)
B01	1563	02/03/2023	0.998	50.11
B02	8002514	03/03/2023	1.004	49.25
B03	1503016	03/03/2023	1.002	50.62
B04	00006659	02/03/2023	1.004	50.14
B05	00007428	03/03/2023	1.001	49.76
R01	1561	01/03/2023	0.997	49.86
R02	8002513	03/03/2023	0.996	49.93
R03	1570	02/03/2023	1.003	49.57
R04	8002519	01/03/2023	1.002	48.90
R05	1503015	01/03/2023	0.998	50.20

Remark : Accept Value of y (test) is  $0.97 < y < 1.03$

Accept Value of  $\Delta H_{@}$  (test) is  $46.7 \pm 6.4$  (mmH<sub>2</sub>O)

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

## Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

### Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	02/02/2023	0.85	0.84
B37	S	0.99	02/02/2023	0.84	0.85
B38	S	0.99	01/02/2023	0.84	0.84
B39	S	0.99	03/02/2023	0.85	0.84
B40	S	0.99	02/02/2023	0.84	0.84
B41	S	0.99	02/02/2023	0.84	0.85
B44	S	0.99	03/02/2023	0.84	0.84
B45	S	0.99	01/02/2023	0.84	0.85
B46	S	0.99	01/02/2023	0.84	0.83
B47	S	0.99	01/02/2023	0.84	0.84
B48	S	0.99	03/02/2023	0.84	0.83
B49	S	0.99	03/02/2023	0.83	0.84
B54	S	0.99	03/02/2023	0.85	0.84
B56	S	0.99	02/02/2023	0.84	0.83
B57	S	0.99	02/02/2023	0.84	0.84
B58	S	0.99	02/02/2023	0.84	0.84

Remark : Accept value of Cp (test) is  $0.84 \pm 0.01$

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R²
B01	SKC	224-PCXR4	262101	04/04/2023	1,000	1,500	2,000	994	1,498	2,003	1.005x - 7.897	1.000
B02	SKC	224-PCXR4	626166	04/04/2023	1,000	1,500	2,000	1,004	1,503	2,003	1.010x - 19.866	0.999
B03	SKC	224-PCXR4	612968	07/04/2023	1,000	1,500	2,000	995	1,496	2,001	1.007x - 13.664	1.000
B04	SKC	224-PCXR4	602804	05/04/2023	1,000	1,500	2,000	998	1,499	1,994	0.999x - 1.611	1.000
B05	SKC	224-PCXR4	612693	07/04/2023	1,000	1,500	2,000	1,002	1,501	2,004	1.014x - 24.856	0.999
B06	SKC	224-PCXR4	262188	07/04/2023	1,000	1,500	2,000	994	1,509	2,006	1.012x - 21.589	0.999
B07	SKC	224-PCXR4	626262	04/04/2023	1,000	1,500	2,000	997	1,490	1,996	0.994x + 3.454	1.000
B08	SKC	224-PCXR4	626100	04/04/2023	1,000	1,500	2,000	1,001	1,499	2,005	1.015x - 27.137	0.999
B09	SKC	224-PCXR4	626479	05/04/2023	1,000	1,500	2,000	997	1,492	1,994	0.994x + 2.385	1.000
B10	SKC	224-PCXR4	091950	03/04/2023	1,000	1,500	2,000	993	1,504	2,005	1.013x - 23.779	1.000
B11	SKC	224-PCXR8	564315	10/04/2023	1,000	1,500	2,000	995	1,492	1,998	1.002x - 7.259	1.000
B12	SKC	224-PCXR4	034656	04/04/2023	1,000	1,500	2,000	1,002	1,504	2,001	1.009x - 17.609	0.999
B13	SKC	224-PCXR4	602073	04/04/2023	1,000	1,500	2,000	997	1,501	2,000	1.004x - 7.622	1.000
B14	SKC	224-PCXR4	626313	03/04/2023	1,000	1,500	2,000	997	1,492	1,991	0.996x + 1.699	1.000
B15	SKC	224-PCXR4	626474	07/04/2023	1,000	1,500	2,000	1,003	1,503	2,006	1.013x - 23.245	0.999
B16	SKC	224-PCXR4	626477	03/04/2023	1,000	1,500	2,000	995	1,506	2,003	1.011x - 22.132	0.999
B17	SKC	224-PCXR4	626860	04/04/2023	1,000	1,500	2,000	996	1,493	1,993	1.000x - 4.627	1.000
B18	SKC	224-PCXR4	691484	04/04/2023	1,000	1,500	2,000	1,001	1,496	2,002	1.010x - 21.179	0.999
B19	SKC	224-PCXR4	691599	04/04/2023	1,000	1,500	2,000	994	1,504	2,000	1.006x - 10.498	1.000
B20	SKC	224-PCXR4	691587	03/04/2023	1,000	1,500	2,000	991	1,502	2,000	1.016x - 35.102	0.999
B21	SKC	224-PCXR4	691531	04/04/2023	1,000	1,500	2,000	994	1,501	1,995	1.001x - 5.153	1.000
B22	SKC	224-PCXR4	691654	07/04/2023	1,000	1,500	2,000	1,000	1,502	2,004	1.014x - 25.574	0.999
B23	SKC	224-PCXR4	798393	05/04/2023	1,000	1,500	2,000	990	1,508	2,004	1.013x - 23.994	1.000
B24	SKC	224-PCXR4	626363	03/04/2023	1,000	1,500	2,000	1,002	1,503	1,999	1.009x - 18.837	0.999
B25	SKC	224-PCXR4	798489	07/04/2023	1,000	1,500	2,000	1,002	1,494	2,000	0.997x + 3.494	1.000
B26	SKC	224-PCXR4	798479	07/04/2023	1,000	1,500	2,000	1,001	1,501	1,994	0.995x + 5.564	1.000
B27	SKC	224-PCXR4	691673	04/04/2023	1,000	1,500	2,000	995	1,505	2,004	1.013x - 25.091	0.999
B28	SKC	224-PCXR4	691570	04/04/2023	1,000	1,500	2,000	1,003	1,501	2,001	1.010x - 19.922	0.999
B29	SKC	224-PCXR4	626472	05/04/2023	1,000	1,500	2,000	1,001	1,498	2,000	0.999x - 1.831	1.000
B30	SKC	224-PCXR4	691489	04/04/2023	1,000	1,500	2,000	1,002	1,507	2,003	1.009x - 13.936	0.999
B31	SKC	224-PCXR4	691509	07/04/2023	1,000	1,500	2,000	994	1,496	1,997	1.004x - 9.680	1.000
B32	SKC	224-PCXR4	091567	10/04/2023	1,000	1,500	2,000	992	1,506	2,001	1.013x - 25.542	0.999
B33	SKC	224-PCXR4	091756	05/04/2023	1,000	1,500	2,000	993	1,498	1,992	0.998x - 1.121	1.000
B34	SKC	224-PCXR4	612962	07/04/2023	1,000	1,500	2,000	1,002	1,503	2,003	1.008x - 14.753	0.999
B35	SKC	224-PCXR4	602682	05/04/2023	1,000	1,500	2,000	991	1,497	1,996	1.003x - 11.598	1.000
B36	SKC	224-PCXR4	626164	05/04/2023	1,000	1,500	2,000	997	1,495	1,998	1.002x - 8.097	1.000
B37	SKC	224-PCXR4	626256	07/04/2023	1,000	1,500	2,000	993	1,505	1,996	1.012x - 27.161	0.999
B38	SKC	224-PCXR4	626167	07/04/2023	1,000	1,500	2,000	998	1,493	1,997	1.003x - 8.615	1.000
B39	SKC	224-PCXR4	034637	10/04/2023	1,000	1,500	2,000	1,003	1,500	2,003	1.013x - 23.125	0.999
B40	SKC	224-PCXR4	798349	07/04/2023	1,000	1,500	2,000	993	1,507	1,998	1.015x - 30.204	0.999

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





**บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด**  
**S.P.S. CONSULTING SERVICE CO., LTD.**  
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
 Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

**Personal Pump Calibration Report**

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

**Environmental Conditions**

Temperature : 25  $\pm$  3  $^{\circ}$ C  
 Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
R01	SKC	224-PCXR4	602467	10/04/2023	1,000	1,500	2,000	992	1,507	2,005	1.009x - 15.491	1.000
R02	SKC	224-PCXR4	626450	10/04/2023	1,000	2,000	3,000	997	1,497	1,989	0.990x + 10.155	1.000
R03	SKC	224-PCXR4	691592	10/04/2023	1,000	1,500	2,000	1,005	1,498	2,003	1.010x - 19.567	0.999
R04	SKC	224-PCXR4	691672	04/04/2023	1,000	1,500	2,000	998	1,491	1,997	0.998x - 1.962	1.000
R05	SKC	224-PCXR4	798470	10/04/2023	1,000	1,500	2,000	994	1,506	1,998	1.012x - 28.038	0.999
R06	SKC	224-PCXR4	798456	05/04/2023	1,000	1,500	2,000	993	1,497	1,995	1.004x - 10.749	1.000
R07	SKC	224-PCXR4	798480	10/04/2023	1,000	1,500	2,000	996	1,492	1,998	1.005x - 11.766	1.000
R08	SKC	224-PCXR4	883215	10/04/2023	1,000	1,500	2,000	1,010	1,503	2,003	0.998x + 3.526	1.000
R09	SKC	224-PCXR4	034650	04/04/2023	1,000	1,500	2,000	994	1,505	2,003	1.017x - 33.985	0.999
R10	SKC	224-PCXR4	091765	07/04/2023	1,000	1,500	2,000	998	1,492	1,996	1.000x - 3.929	1.000
R11	SKC	224-PCXR4	091763	04/04/2023	1,000	1,500	2,000	1,002	1,497	2,003	1.012x - 23.883	0.999
R12	SKC	224-PCXR4	091568	10/04/2023	1,000	1,500	2,000	995	1,503	1,998	1.002x - 7.698	1.000
R13	SKC	224-PCXR4	091638	10/04/2023	1,000	1,500	2,000	1,005	1,497	1,993	0.989x + 13.679	1.000
R14	SKC	224-PCXR4	091764	10/04/2023	1,000	1,500	2,000	992	1,503	1,998	1.015x - 32.167	0.999
R15	SKC	224-PCXR8	529457	10/04/2023	1,000	1,500	2,000	1,003	1,501	2,005	1.005x - 9.429	1.000
R16	SKC	224-PCXR8	529643	04/04/2023	1,000	1,500	2,000	999	1,496	1,995	0.999x - 3.290	1.000
R17	SKC	224-PCXR8	529645	05/04/2023	1,000	1,500	2,000	995	1,511	2,001	1.012x - 23.233	0.999
R18	SKC	224-PCXR8	566756	07/04/2023	1,000	1,500	2,000	992	1,497	1,999	1.002x - 7.359	1.000
R19	SKC	224-PCXR8	566802	07/04/2023	1,000	1,500	2,000	1,002	1,498	1,999	1.009x - 19.671	0.999
R20	SKC	224-PCXR8	529089	07/04/2023	1,000	1,500	2,000	992	1,501	2,004	1.015x - 28.270	1.000
R21	SKC	224-PCXR8	665728	10/04/2023	1,000	1,500	2,000	997	1,494	1,997	1.001x - 7.797	1.000
R22	SKC	224-PCXR8	707444	05/04/2023	1,000	1,500	2,000	1,003	1,501	2,003	1.003x - 6.218	1.000
R23	SKC	224-PCXR8	761067	10/04/2023	1,000	1,500	2,000	996	1,495	1,993	0.995x + 0.263	1.000
R24	SKC	224-PCXR8	707893	10/04/2023	1,000	1,500	2,000	997	1,506	2,002	1.009x - 17.713	0.999
R25	SKC	224-PCXR8	761052	10/04/2023	1,000	1,500	2,000	1,009	1,497	1,992	0.983x + 22.945	1.000
R26	SKC	224-PCXR8	707956	10/04/2023	1,000	1,500	2,000	1,004	1,502	2,005	1.008x - 14.326	0.999
R27	SKC	224-PCXR8	707398	07/04/2023	1,000	1,500	2,000	995	1,502	2,002	1.007x - 16.361	1.000
R28	SKC	224-PCXR8	707481	10/04/2023	1,000	1,500	2,000	1,006	1,501	2,003	1.009x - 18.291	0.999
R29	SKC	224-PCXR8	707402	07/04/2023	1,000	1,500	2,000	1,002	1,494	1,989	0.987x + 14.566	1.000
R30	SKC	224-PCXR8	093811	04/04/2023	1,000	1,500	2,000	1,001	1,494	1,996	0.997x + 0.646	1.000
R31	SKC	224-PCXR8	093183	10/04/2023	1,000	1,500	2,000	1,001	1,502	2,004	1.004x - 5.652	1.000
R32	SKC	224-PCXR8	671950	05/04/2023	1,000	1,500	2,000	999	1,501	1,993	0.994x + 7.163	1.000
R33	SKC	224-PCXR4	626254	10/04/2023	1,000	1,500	2,000	996	1,504	2,001	1.015x - 30.192	0.999
R34	SKC	224-PCXR4	626131	04/04/2023	1,000	1,500	2,000	1,003	1,498	2,004	1.004x - 9.377	1.000
R35	SKC	224-PCXR8	707460	10/04/2023	1,000	1,500	2,000	998	1,496	1,996	0.996x + 3.677	1.000
R36	SKC	224-PCXR8	707446	10/04/2023	1,000	1,500	2,000	1,003	1,498	2,002	1.010x - 20.668	0.999
R37	SKC	224-PCXR8	707432	10/04/2023	1,000	1,500	2,000	998	1,496	2,000	0.999x - 0.873	1.000
R38	SKC	224-PCXR8	707349	07/04/2023	1,000	1,500	2,000	997	1,497	2,001	1.003x - 8.747	1.000
R39	SKC	224-PCXR8	761095	10/04/2023	1,000	1,500	2,000	1,001	1,497	1,997	0.999x + 0.140	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R²
H-R01	Dwyer	VFB-65	05/04/2023	500	1,000	2,000	502.1	993.6	1981.1	1.000x - 3.647	0.999
H-R02	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	500.4	998.7	1988.7	1.001x - 3.457	1.000
H-R03	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	502.1	990.3	1997.7	0.993x + 4.022	1.000
H-R04	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	497.2	992.2	2016.9	1.007x - 11.203	1.000
H-R05	Dwyer	VFB-65	05/04/2023	500	1,000	2,000	499.2	988.5	1990.7	1.003x - 7.136	1.000
H-R06	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	504.8	994.6	1982.6	0.999x - 1.961	0.999

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : VACUUM GAUGE  
MANUFACTURER : HI-LIGHT  
MODEL / TYPE : N/A  
SERIAL NO. : N/A[64-220066-4]  
CLID. NO. : 212201115  
JOB CONTROL NO. : 220720073204

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 20 July 2022

DATE OF ISSUED : 22 July 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
22 July 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22073204

F3-011-04/01-12

page 1 of 3



@clccalibration

## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : VACUUM GAUGE  
MANUFACTURER : HI-LIGHT  
MODEL / TYPE : N/A  
SERIAL NO. : N/A[64-220066-4]  
DATE OF CALIBRATION : 21 July 2022

---

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-05** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 744 S/N. 9226007 with Pressure Module Model 700PV4 S/N. 19298401.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).  
Certificate No. MP-0196-21, Due Date 17 November 2022.

#### UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of  $k = 2$ . It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q22073204

F3-011-04/01-12

page 2 of 3



@clccalibration

## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

### CALIBRATION DATA

#### CORRECTION OF PRESSURE

DUC Test point ( inHg )	STD Reading ( inHg )		Correction ( inHg )	
	Up	Down	Up	Down
0	0.0	0.0	0.0	0.0
-5	-5.1	-5.1	-0.1	-0.1
-10	-10.0	-10.1	0.0	-0.1
-15	-15.0	-15.0	0.0	0.0
-20	-19.9	-20.0	+0.1	0.0
-25	-24.9	-24.9	+0.1	+0.1
-30	-29.9	-29.9	+0.1	+0.1

Uncertainty of measurement  $\pm 0.2$  inHg

Transmitting fluid : Air.

Technical Note. k factor 1 kPa = 0.2952998 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 36 of 54

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q22073204

F3-011-04/01-12

page 3 of 3



@clccalibration





CERTIFICATE No : 23M2442

REFERENCE No : 68471-2

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : SARTORIUS

**MODEL** : BSA224S-CW

**SERIAL No** : 36591843

**ID No** : BA 09/61

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 10-Mar-23

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 16-Mar-23

**RECEIVED DATE** : 10-Mar-23





CERTIFICATE No : 23M2442

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	MODEL	:	BSA224S-CW
MANUFACTURER	:	SARTORIUS	S/N	:	36591843
ID No	:	BA 09/61	RECEIVED DATE	:	10-Mar-23
AIR PRESSURE	:	1010mbar $\pm$ 1mbar	CALIBRATION DATE	:	10-Mar-23
AMBIENT TEMPERATURE	:	23° C $\pm$ 1° C	RELATIVE HUMIDITY	:	49 %RH $\pm$ 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.0	0.0000	0.0000	0.000058
0.1	0.1000	0.0000	0.000059
0.2	0.2000	0.0000	0.000059
0.5	0.5000	0.0000	0.000060
1.0	1.0000	0.0000	0.000060
2.0	2.0000	0.0000	0.000061
5.0	5.0000	0.0000	0.000063
10.0	10.0000	0.0000	0.000067
20.0	20.0001	-0.0001	0.000073
50.0	50.0000	0.0000	0.00011
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	99.9999
3	99.9998
4	100.0001
5	100.0000
OFF-CENTER LOADING	0.0002

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : SP22018

Pages 1 of 3

## Calibration Certificate

**Equipment :** UV-VIS SPECTROPHOTOMETER  
**Manufacturer :** PERKINELMER  
**Model :** LAMBDA 25  
**Serial No.:** 501S14123010  
**ID No.:** SP03/58  
**Calibration Mode :** WAVELENGTH ACCURACY  
PHOTOMETRIC ACCURACY  
  
**Condition As Found :** GOOD  
  
**Customer :** S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,  
CHOMPHON, CHATUCHAK,  
BANGKOK 10900, THAILAND.  
  
**Location :** ORGANIC LABORATORY IV  
  
**Ambient Temperature :** ( 24.4 ± 5 ) °C  
**Relative Humidity :** ( 60.1 ± 25 ) %  
  
**Received Date :** 30 AUGUST 2022  
**Calibration Date :** 30 AUGUST 2022  
**Date of Issue :** 31 AUGUST 2022

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

Cert. No. : SP22018

Job No. : VC65SP0008

Pages : 2 of 3

**Calibration Method :**

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01,ASTM E925-02

**Condition of this result of calibration :**

## 1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	87569	13/10/2022
Didymium liquid	RM-DL	28912	87588	15/10/2022
Neutral density filter	RM-1N2N3N	13877	87600	15/10/2022
Potassium dichromate solutions	RM-0204060810	14204	87614	16/10/2022
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology,NIST.

**Result of calibration : Wavelength Accuracy**

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.4	0.15	0.16	2.00
	467.82	467.8	-0.02	0.16	2.00
	536.56	536.5	-0.06	0.16	2.00
	640.50	640.5	0.00	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.2	0.26	0.16	2.00

UUC\* = Unit Under Calibration

Continuation of Calibration Certificate

Cert. No. : SP22018  
Job No. : VC65SP0008  
Pages : 3 of 3

**Result of calibration : Photometric Accuracy**

(Without adjustment)

Material	Wavelength (nm)	Filter: S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0524	1.0539	0.0015	0.0028	2.00
		29914	0.7	0.7454	0.7459	0.0005	0.0029	2.00
		29381	0.5	0.5426	0.5426	0.0000	0.0028	2.00
	546.1	29360	1.0	0.9822	0.9810	-0.0012	0.0028	2.00
		29914	0.7	0.6962	0.6960	-0.0002	0.0028	2.00
		29381	0.5	0.5076	0.5070	-0.0006	0.0029	2.00
	590.0	29360	1.0	1.0221	1.0202	-0.0019	0.0028	2.00
		29914	0.7	0.7238	0.7230	-0.0008	0.0029	2.00
		29381	0.5	0.5364	0.5360	-0.0004	0.0031	2.00
	635.0	29360	1.0	0.9751	0.9732	-0.0019	0.0028	2.00
		29914	0.7	0.6912	0.6902	-0.0010	0.0029	2.00
		29381	0.5	0.5214	0.5210	-0.0004	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2436	0.2419	-0.0017	0.0101	2.00	
		40	0.4905	0.4855	-0.0050	0.0115	2.00	
		60	0.7453	0.7388	-0.0065	0.0067	2.00	
		80	0.9920	0.9839	-0.0081	0.0071	2.00	
		100	1.2487	1.2414	-0.0073	0.0073	2.00	

UUC\* = Unit Under Calibration

**Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230**

Resolution of Wavelength Mode 0.1 nm  
Resolution of Photometric Mode 0.0001 A  
Parameter Setting  
Measurement Mode Wavelength, Absorbance  
Wavelength Scan 1100 nm-190 nm  
Scanning Speed 7.5 nm/min  
Data Pitch 0.1 nm  
Band width(Wavelength) 1.0 nm  
Band width(Vis) 1.0 nm  
Band width(Uv) 1.0 nm

Stray Light** UUC* Reading at 220 nm	
Transmission T(%)	Absorbance(A)
0.0107	3.9886

\*\*Specific Acceptance :  
Transmission  $\leq 1.0$  T(%), Absorbance  $\geq 2.0$  A  
\*\*Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95%

**End of Calibration Certificate**





## Certificate of Calibration

**Aquion : Anion (ID#894)**

This certificate is to verify that instrument below are calibrated  
by Archemica Lab Co.,Ltd.

AQUION S/N : 190840059

AS-DV S/N : 190915235

for

**S.P.S. Consulting Service Co., Ltd.**



Operator Signature : \_\_\_\_\_

Date : Jan 5, 2022

(Mr. Channarong Khiao-Un)

Test Engineer

ระดับเสียงในบรรยากาศ



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

**Request No.** 21-66/0358

**MTC No.** EEL. BP. 22/0366

## CALIBRATION CERTIFICATE

**Submitted by** : S.P.S. Consulting Service Co., Ltd.

**Address** : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

**Calibrated at** : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

**Instrument Calibrated :**

Description : Sound Calibrator

Manufacturer : Cirrus

Model : CR:515

Serial No. : 92002

**Ambient Environment**

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

**Standards used :** 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Keithley 2015-P S/N 4106495.

7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

**Calibration Procedure:** CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

**Date of Receipt** : 3 Mar. 2023

**Date of Calibration** : 13 Mar. 2023

1 / 2

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0358

MTC No. EEL. BP. 22/0366

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.99	-0.01	$\pm 0.10$	$\pm 0.40$ dB

2. Frequency


Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1000.3	0.3	$\pm 1.5$	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.39	$\pm 0.50$	$\pm 3.0\%$

- Note :
1. No adjustment.
  2. The calibrator pressure correction was not included.
  3. The microphone volume correction was not included.

Calibrated by :

  
(Mr. Nuttapong Niljrusvanit)

Approved by :

  
(Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 13 Mar. 2023

Date of Issue : 14 Mar. 2023

Ref : 2011266030300928001

2 / 2

End of Certificate

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Noise R\_226/23

## Sound Level Meter Calibration Report

### Acoustic Calibrator Data

Brand	CIRRUS	Number	AC-CR01/63
Model	CR515	Serial No.	92002
Calibration Range	94 dB, 1000 Hz	Last Calibration	13 March 2023
		Due Date	13 March 2024

### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
CR-B01	Cirrus	CR161B	G301393	30 April 2023	94.1	94.0
CR-B02	Cirrus	CR161B	G301157	30 April 2023	94.0	94.0
CR-B03	Cirrus	CR161B	G301155	30 April 2023	94.0	94.0
CR-B06	Cirrus	CR161B	G301151	30 April 2023	94.1	94.0
CR-B07	Cirrus	CR161B	G301167	30 April 2023	94.0	94.0
CR-B08	Cirrus	CR161B	G301397	30 April 2023	94.0	94.0
CR-B10	Cirrus	CR161B	G301407	30 April 2023	94.0	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.99 ± 0.10 dB	

Calibrated by :



(Mr. Adul Dangklom )

Approved by :



(Mr. Peera Detudom)

คุณภาพน้ำเสีย



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 22E9693

REFERENCE No : 66476-1

PAGE : 1 OF 3

**Certificate of Calibration**

**EQUIPMENT** : pH METER

**MANUFACTURER** : HANNA

**MODEL** : HI 3512

**SERIAL No** : TH118035


**ID No** : pH 04/56

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 15-Sep-22

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 15-Sep-22

**RECEIVED DATE** : 14-Sep-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22E9693

PAGE : 2 OF 3

## Calibration Report

EQUIPMENT : pH METER  
MANUFACTURER : HANNA  
ID No : pH 04/56  
RECEIVED DATE : 14-Sep-22  
AMBIENT TEMPERATURE : 20 ° C ± 1 ° C  
MODEL : HI 3512  
SERIAL NUMBER : TH118035  
CALIBRATION DATE : 15-Sep-22  
RELATIVE HUMIDITY : 50 % RH ± 10% RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/</u> <u>LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-06	CC719181	4880-12119147	05-Apr-23
2) pH STANDARD SOLUTION	00651-08	CC718727	4881-12110709	31-Mar-23
3) pH STANDARD SOLUTION	00651-10	CC717045	4882-12065386	17-Mar-23
4) PROCESS CALIBRATOR	CA150	91S6079	22E1145	31-Mar-23
5) BATH	260014	1247 48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
  - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
  - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

### RESULT OF CALIBRATION : ADJUSTMENT

#### 1. DISPLAY UNIT ONLY

SLOPE FACTOR  $k = 2.303 \text{ RT/F} = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.8	-0.69	-0.171	0.14	2.0
354.95	355.6	-0.65	0.860	0.14	2.0
295.80	296.4	-0.60	1.892	0.14	2.0
236.64	237.2	-0.56	2.922	0.14	2.0
177.48	178.0	-0.52	3.954	0.14	2.0
118.32	118.8	-0.48	4.985	0.14	2.0
59.16	59.7	-0.54	6.016	0.14	2.0
0.00	0.5	-0.50	7.049	0.14	2.0
-59.16	-58.8	-0.36	8.136	0.14	2.0
-118.32	-117.9	-0.42	9.223	0.14	2.0
-177.48	-177.1	-0.38	10.311	0.14	2.0
-236.64	-236.3	-0.34	11.399	0.14	2.0
-295.80	-295.5	-0.30	12.487	0.14	2.0
-354.95	-354.7	-0.25	13.575	0.14	2.0
-414.11	-413.9	-0.21	14.662	0.14	2.0

END OF CALIBRATION REPORT PAGE 2 OF 3



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22E9693

PAGE : 3 OF 3

**Calibration Report****RESULT OF CALIBRATION (CONTINUE) :****2. DISPLAY UNIT WITH pH ELECTRODE S/N: 09081C6M**

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ( $\pm$ pH)	COVERAGE FACTOR k
4.007	4.007	0.000	3.996	0.012	2.0
7.004	7.006	-0.002	6.944	0.012	2.0
10.016	10.012	0.004	10.194	0.014	2.0

**3. DISPLAY UNIT WITH TEMPERATURE**

STANDARD READING (°C)	UUC READING (°C)	CORRECTION (°C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ( $\pm$ °C)	COVERAGE FACTOR k
25.003	25.0	0.003	---	0.0085	2.0

**4. PERCENT SLOPE 100%**

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



## Certificate of Calibration

**Certificate No. :** 65-400210-1

**Page : 1 of 2**

**Submitted by :** S. P. S Consulting Service Co.,Ltd.  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

**Equipment :** Liquid in Glass Thermometer

Manufacturer : SK

Model : N/A

Range : 0 °C to 100 °C

Resolution : 1 °C

Serial No. : N/A

Immersion : Total

ID No. : TM21/59

**Environment :** Ambient Temperature :  $(23 \pm 2)$  °C

Relative Humidity :  $(50 \pm 15)$  %

Line Voltage :  $(220 \pm 22)$  VAC

**Date of Received :** 19 April 2022

**Date of Calibration :** 23 April 2022

**Date of Issue :** 23 April 2022

**Calibrated by :** Chortip Samchusri

**Calibration Method :** This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0016-22	07 Feb 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)
400004	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)

Approved by :

( Bunjerd Masri )

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



## Certificate of Calibration

**Certificate No. :** 65-400210-1

**Page : 2 of 2**

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

Ice point check : UUC\* reading 0 °C Standard reading 0.6439 °C

Standard Reading ( °C )	UUC Reading ( °C )	Correction ( °C )	Uncertainty ( ± °C )
20.6690	20	0.7	0.31

### Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- o0o -







CERTIFICATE No : 22M2569

REFERENCE No : 64386-3

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : TETNITHI W.

CALIBRATION DATE : 11-Mar-22

APPROVED BY :   
PONGSAK J.

ISSUED DATE : 17-Mar-22

RECEIVED DATE : 11-Mar-22





CERTIFICATE No : 22M2569

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	MODEL	:	BSA224S-CW
MANUFACTURER	:	SARTORIUS	S/N	:	36591843
ID No	:	BA 09/61	RECEIVED DATE	:	11-Mar-22
AIR PRESSURE	:	1008mbar $\pm$ 1mbar	CALIBRATION DATE	:	11-Mar-22
AMBIENT TEMPERATURE	:	22° C $\pm$ 1° C	RELATIVE HUMIDITY	:	51 %RH $\pm$ 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING WEIGHT OF QUALITY CALIBRATION TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000048 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.0000	0.0000	0.000078
0.10	0.1000	0.0000	0.000078
0.20	0.2000	0.0000	0.000078
0.50	0.5000	0.0000	0.000079
1.00	1.0000	0.0000	0.000079
2.00	2.0000	0.0000	0.000080
5.00	5.0000	0.0000	0.000081
10.00	10.0000	0.0000	0.000084
20.00	20.0000	0.0000	0.000089
50.00	50.0000	0.0000	0.00011
100.00	100.0000	0.0000	0.00019
200.00	199.9999	0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	99.9999
2	99.9999
3	100.0000
4	99.9999
5	99.9998
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT PRODUCTION AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 23M2442

REFERENCE No : 68471-2

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : SARTORIUS

**MODEL** : BSA224S-CW

**SERIAL No** : 36591843


**ID No** : BA 09/61

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 10-Mar-23

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 16-Mar-23

**RECEIVED DATE** : 10-Mar-23





CERTIFICATE No : 23M2442

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW  
MANUFACTURER : SARTORIUS S/N : 36591843  
ID No : BA 09/61 RECEIVED DATE : 10-Mar-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 10-Mar-23  
AMBIENT TEMPERATURE : 23° C  $\pm$  1° C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.0	0.0000	0.0000	0.000058
0.1	0.1000	0.0000	0.000059
0.2	0.2000	0.0000	0.000059
0.5	0.5000	0.0000	0.000060
1.0	1.0000	0.0000	0.000060
2.0	2.0000	0.0000	0.000061
5.0	5.0000	0.0000	0.000063
10.0	10.0000	0.0000	0.000067
20.0	20.0001	-0.0001	0.000073
50.0	50.0000	0.0000	0.00011
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	99.9999
3	99.9998
4	100.0001
5	100.0000
OFF-CENTER LOADING	0.0002

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CH140

Page.: 1 of 2

## Certificate of Calibration

**Equipment :** Conductivity Meter  
**Manufacturer :** Mettler Toledo  
**Model :** SevenCompact  
**Serial No. :** C141708983  
**ID No. :** -  
**Condition As-Received:** Used Item  
**Received Date :** 31 January 2022  
**Calibration Date :** 02 February 2022  
**Reference :** 2201-0954WSC-1  
**Submitted by :** S.P.S. Consulting Service Co.,Ltd.  
7 Soi Phahonyothin 24, Phahonyothin Rd.,  
Chom Phon, Chatuchak, Bangkok 10900  
**Ambient Temperature :**  $(25 \pm 2.5) ^\circ\text{C}$   
**Relative Humidity :**  $(50 \pm 15) \%$   
**Calibration Procedure:** In -house method :  
- CP-CH6 : based on direct measurement by  
using certified reference material (CRM)

**Calibrated by :** Warakorn Lerngagtrakul

**Approved by :**

Approved Signatory

- ( ✓ ) Malee Butkruea  
( ) Saithip Meangmai  
( ) Warakorn Lerngagtrakul

**Issue Date :** 10 February 2022

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0037795



Cert.No.: 22CH140

Page.: 2 of 2

**Condition of this result of calibration**

## 1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	1963878	130RC095	21I977	17 Sep 2022

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

## 2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
147.0 $\mu\text{S/cm}$	CPA Chem	761020	02 Aug 2022
1413.0 $\mu\text{S/cm}$	CPA Chem	761021	02 Aug 2022
12.880 $\text{mS/cm}$	CPA Chem	761022	02 Aug 2022
111.3 $\text{mS/cm}$	CPA Chem	768164	12 Sep 2022

- Control Conductivity calibration solution temperature by Water bath ( $25 \pm 0.1$ )  $^{\circ}\text{C}$

## 3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration results****Function : Conductivity Measurement**(\*) After Adjustment at 0.147, 1.413, 12.880, 111.3  $\text{mS/cm}$ 

Conductivity Electrode Serial No.: 5821320179

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement ( $\pm$ )	Coverage factor k
147.0 $\mu\text{S/cm}$	148.1 $\mu\text{S/cm}$	147.0 $\mu\text{S/cm}$	0.99 $\mu\text{S/cm}$	2.00
1413.0 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	9.2 $\mu\text{S/cm}$	2.00
12.880 $\text{mS/cm}$	12.61 $\text{mS/cm}$	12.88 $\text{mS/cm}$	0.086 $\text{mS/cm}$	2.00
111.3 $\text{mS/cm}$	105.7 $\text{mS/cm}$	111.4 $\text{mS/cm}$	0.76 $\text{mS/cm}$	2.00

**Remark**

- UUC\* = Unit Under Calibration

- 147.0  $\mu\text{S/cm}$  Adjustment Cell constant =  $0.550585 \text{ cm}^{-1}$ - 1413.0  $\mu\text{S/cm}$  Adjustment Cell constant =  $0.554585 \text{ cm}^{-1}$ - 12.880  $\text{mS/cm}$  Adjustment Cell constant =  $0.562585 \text{ cm}^{-1}$ - 111.3  $\text{mS/cm}$  Adjustment Cell constant =  $0.578585 \text{ cm}^{-1}$ 

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

a 1093760



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : CONDUCTIVITY METER  
MANUFACTURER : METTLER TOLEDO  
MODEL / TYPE : SEVEN COMPACT S230  
SERIAL NO. : C141708983/5821320179  
CLID. NO. : 272300452  
JOB CONTROL NO. : 230211016445

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 11 February 2023

DATE OF ISSUED : 15 February 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart  
Calibration Engineer

Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
15 February 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units ( SI )

Certificate No. Q23016445

F3-011-04/01-12

page 1 of 4



@clccalibration

## REPORT OF CALIBRATION

### FOR

NOMENCLATURE	:	CONDUCTIVITY METER
MANUFACTURER	:	METTLER TOLEDO
MODEL / TYPE	:	SEVEN COMPACT S230
SERIAL NO.	:	C141708983/5821320179
DATE OF CALIBRATION	:	13 February 2023

#### ENVIRONMENT CONDITIONS :

Temperature :  $(25 \pm 2.5) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \% \text{ RH}$

#### PROCEDURE USED :

This instrument [ Conductivity Meter ] was calibrated under procedure No. **WI-305-130**. The calibration was performed by direct measurement with Certified Reference Material (CRM) and Reference Material (RM) .

This instrument [ Temperature ] was calibrated under procedure No. **WI-305-244**. The calibration was performed by Comparison with Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

1. Potassium Chloride Solution ( nominal 1.41 mS/cm , nominal 12.8 mS/cm )
2. Conductivity Solution , Hanna Product Code HI 7033L Lot Number 6436.
3. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
4. Precision Thermometer, ASL Model F250 S/N. 1334023800.
5. IPRT, ASL Model T100-250-1D S/N. L0193A-1-1.





## TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through Merck Co., Ltd.

Certificate No. HC02139203 , HC04515254. Due Date 30 June 2023 , 30 November 2023.

2. The measurements are traceable to International System of Units (SI) , through Hanna instruments.

Certificate No. 12E12 , Due Date May 2024 .

3. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q22130792, Due Date 05 January 2024.

4. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0823/65, Due Date 22 August 2023.

5. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).

Certificate No. TT-0166-22, Due Date 01 December 2023.

## UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"



## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of Conductivity Meter.

### CALIBRATION DATA

#### 1. Conductivity Solution Test @ 25°C

Standard Conductivity Solution	DUC Reading	Uncertainty of Measurement	k Factor
*84.00 µS/cm	84.04 µS/cm [Cell Constant 0.548589]	± 1.00 µS/cm	2,00
1412.0 µS/cm	1413 µS/cm [Cell Constant 0.548589]	± 21.0 µS/cm	2,00
12.85 mS/cm	12.88 mS/cm [Cell Constant 0.573538]	± 0.19 mS/cm	2,00

Note. \* means Calibrations marked "Not TISI Accredited" in this Certificate have been included for completeness.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 138 of 138

#### \*2. Temperature Result [ Probe Conductivity ]

Immersion depth (mm)	Actual Temperature ( °C )	DUC Reading ( °C )	Correction ( °C )	Uncertainty ± ( °C )
100	25.00	25.0	0.00	0.07

Note. The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of  $k = 2,00$ .

\* means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

**This report is valid for the above stated instrument/s only.**

**### End of Certificate ###**







**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES**

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

**Cert.No.:** 22TW98

**Page.:** 1 of 2

## Certificate of Testing

<b>Equipment :</b>	DO Meter
<b>Manufacturer :</b>	YSI
<b>Model :</b>	5000-230V
<b>Serial No. :</b>	15B100751
<b>ID No. :</b>	-
<b>Received Date :</b>	20 April 2022
<b>Test Date :</b>	21 April 2022
<b>Reference :</b>	2204-0429WC-1
<b>Submitted by :</b>	S.P.S. Consulting Service Co.,Ltd. 7 Phaholyothin 24, Phaholyothin Road., Jompol, Chatuchak, Bangkok 10900
<b>Laboratory Condition :</b>	Temperature ( $25 \pm 5$ ) °C Humidity ( $50 \pm 20$ ) %
<b>Test Procedure :</b>	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
<b>Tested by :</b>	Walalak Sirithean
<b>Approved by :</b>	<div style="background-color: gray; width: 200px; height: 20px; margin-bottom: 5px;"></div> Approved Signatory
<input checked="" type="checkbox"/> Malee Butkruea <input type="checkbox"/> Saithip Meangmai <input type="checkbox"/> Warakorn Lerngagtrakul	
<b>Issue Date :</b>	25 April 2022



Cert.No.: 22TW98

Page.: 2 of 2

**Condition of this result of calibration**

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	21MM430	21 Sep 2022

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

**Result :** Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 14J100195

<b>Titration Method (Azide Modification Method)</b> (mg/L)	<b>DO Meter Reading</b> (mg/L)	<b>Standard Deviation</b> (mg/L)
8.12	8.14	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

a 1105753



CERT.No.: HS-U017D

Calibration Date : 3 Apr 23  
Submitted by : S.P.S CONSULTING SERVICE CO.,LTD  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,  
Chatuchak, Bangkok, Thailand 10900

Model : YSI 5000  
S/N : 15B100751  
Probe : YSI 5010  
S/N : 22D100097  
ID NO. : -  
Air Temp ref : S/N. E00522  
Barometric ref : S/N. E00522  
Water Temp ref : S/N. 11431  
Technician : Kittipong M.

Avg Room Temp : 20 °C  
Avg Water Temp : 20 °C  
Air Pressure : 760.00 mmHg  
Salinity : 0 ppt

#### Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-

Mean Measurement	9.08	mg/l	-	-
Inaccuracy	0.01	mg/l	-	-

Overall Status (PASS)

#### Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature

(Kittipong Maekwong)

Laboratory Manager

(Natenapha Pisatkunchon)





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 22T10972

REFERENCE No : 66837-1

PAGE : 1 OF 3

## Certificate of Calibration

**EQUIPMENT** : COD REACTOR

**MANUFACTURER** : HACH

**MODEL** : DRB 200


**SERIAL No** : 15110C0497

**ID No** : DRB 04/59

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : CHAICHARN CH.

**CALIBRATION DATE** : 20-Dec-22

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 20-Dec-22

**RECEIVED DATE** : 20-Dec-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02





CERTIFICATE No : 22T10972

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : COD REACTOR  
MANUFACTURER : HACH  
ID NUMBER : DRB 04/59  
RECEIVED DATE : 20-Dec-22  
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB 200  
SERIAL NUMBER : 15110C0497  
CALIBRATION DATE : 20-Dec-22  
RELATIVE HUMIDITY : 52 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT TEMPERATURE RECORDER WITH THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 15 POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE FOUR CORNERS OF THE REACTOR AND PLACED THE EIGHTH THERMOCOUPLE AT THE CENTER OF THE REACTOR.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	8009008	22T7511	10-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

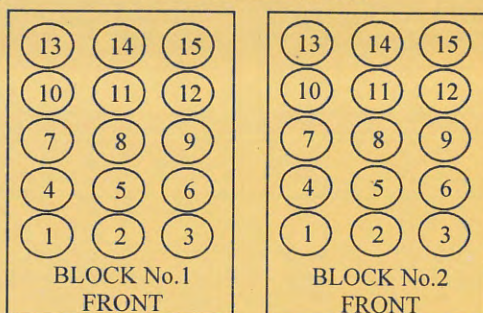

### TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	149.8
	2	149.6
	3	149.7
	4	149.8
	5	149.9
	6	149.8
	7	149.8
	8	149.8
	9	149.9
	10	149.8
	11	149.9
	12	149.7
	13	149.9
	14	149.9
	15	149.7
Uncertainty of Measurement(± °C)	0.86	0.86

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

<b>Customer :</b> <u>S.P.S.Consulting Service Co.,Ltd</u>	<b>Date Tested:</b> <u>January 12, 2022</u>	
	<b>Recommendation Recertification</b>	
<b>Address :</b> <u>7 Soi Phaholyothin 24</u>	<b>Period</b> <u>6</u> <b>Months</b>	
<u>Paholyothin Road</u>	<b>Recertification Due:</b> <u>July 12, 2022</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	<b>Date Last Certified:</b> <u>July 14, 2021</u>	
<b>User Name:</b> <u>K.Phenpha Viphasathawat</u>	<b>Visit Number:</b> <u>2 of 2</u>	
<b>Phone:</b> <u>083-9269252</u>	<b>PerkinElmer Phone:</b> <u>02-719-6420 ext 206</u>	
<b>Fax:</b> <u>02-513-4221</u>	<b>PerkinElmer Fax:</b> <u>02-318-5597</u>	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
<b>MODEL</b>	<b>SERIAL NUMBER</b>	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
<b>TESTED EQUIPMENT</b>	<b>CALIBRATION NUMBER</b>	<b>EXPIRATION</b>
<u>IPV Methods</u>		
<b>TEST STANDARD USED</b>	<b>PART NUMBER</b>	<b>EXPIRATION DATE</b>
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>August 30, 2022</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>January 30, 2022</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>June 30, 2022</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>August 30, 2022</u>
<b>CUSTOMER SUPPLIED</b>	<b>COMMENTS</b>	<b>CUSTOMER INITIALS</b>
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER**    077C7042401
**DATE TESTED**    January 12, 2022
**1. MECHANICAL CHECKS**

A. Inspect and clean all fans and filters.

☐ OK

B. Inspect and replace as necessary, all torch components including the RF coil.

☐ OK

C. Inspect all tubing for sign of clacking or leaking.

☐ OK

D. Adjust water and gas pressure regulator settings.

☐ OK

E. Inspect and leak check pneumatics drawers.

☐ OK

F. Clean the exterior of the instrument.

☐ OK

**2. OPTICAL CHECKS**

A. Inspect and clean all optical components.

☐ OK

B. As required, check and replace all purgefilters.

☐ OK

C. Recheck optical alignment.

☐ OK

**3. COOLING SYSTEM CHECKS**

A. Perform preventive maintenance on chiller.

☐ OK

B. Flush out the chiller every year.

☐ N/A

**4. PERFORMANCE CHECKS**

A. Torch View Alignment.

☐ OK

B. Wavelength Calibration.

☐ OK



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

SERIAL NUMBER : 077C7042401

DATE TESTED : January 12, 2022

PARAMETER	SPECIFICATION			FINAL VALUE	
Spectral Resolution : UV	As	193.696 nm	≤ 0.007	0.00554	
	Ni	231.604 nm	≤ 0.008	0.00725	
	Ni	341.476 nm	≤ 0.012	0.00752	
Spectral Resolution : VIS	La	408.672 nm	≤ 0.020	0.01616	
	Ba	455.403 nm	≤ 0.025	0.02416	
Precision					
	As	193.656 nm	% RSD < 1.0	0.34	%
	Zn	213.856 nm	% RSD < 1.0	0.27	%
	Mn	257.610 nm	% RSD < 1.0	0.41	%
	La	379.478 nm	% RSD < 1.0	0.57	%
	Ba	455.403 nm	% RSD < 1.0	0.33	%
	Ba	493.408 nm	% RSD < 1.0	0.26	%
Detection Limits : Axial	Tl	190.080 nm	3(sd)	5.51	ppb
	As	193.696 nm	3(sd)	8.59	ppb
	Pb	220.353 nm	3(sd)	0.50	ppb
Detection Limits : Radial	As	193.696 nm	3(sd)	21.00	ppb
	Zn	213.856 nm	3(sd)	0.32	ppb
	Mn	257.610 nm	3(sd)	0.18	ppb
	La	379.478 nm	3(sd)	0.44	ppb
	Ba	455.403 nm	3(sd)	0.17	ppb
	Ba	493.408 nm	3(sd)	0.12	ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd	226.502 nm	≤ 150 ppb	12.46	
BEC : Radial (IB X 1000)/(IS-IB)	Mn	257.610 nm	≤ 45 ppb	30.82	





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER** 077C7042401**DATE TESTED** January 12, 2022**Remarks :**

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,  
including warranty terms.

**Service Department PerkinElmer Ltd.**

**Authorized Representative:**

( Mr. Wiphan Promlumda )

Service Engineer



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

<b>Customer :</b> <u>S.P.S.Consulting Service Co.,Ltd</u>	Date Tested: <u>January 11, 2023</u>	
	Recommendation Recertification	
<b>Address :</b> <u>7 Soi Phaholyothin 24</u>	Period <u>6</u> Months	
<u>Paholyothin Road</u>	Recertification Due: <u>July 11, 2023</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	Date Last Certified: <u>July 11, 2022</u>	
<b>User Name:</b> <u>K.Phenpha Vipasthawatt</u>	Visit Number: <u>2 of 2</u>	
<b>Phone:</b> <u>083-9269252</u>	PerkinElmer Phone: <u>02-719-6420 ext 206</u>	
<b>Fax:</b> <u>02-513-4221</u>	PerkinElmer Fax: <u>02-318-5597</u>	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
<b>MODEL</b>	<b>SERIAL NUMBER</b>	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
<b>TESTED EQUIPMENT</b>	<b>CALIBRATION NUMBER</b>	<b>EXPIRATION</b>
<u>IPV Methods</u>		
<b>TEST STANDARD USED</b>	<b>PART NUMBER</b>	<b>EXPIRATION DATE</b>
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>May 30, 2023</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>February 28, 2023</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>August 30, 2023</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>November 30, 2023</u>
<b>CUSTOMER SUPPLIED</b>	<b>COMMENTS</b>	<b>CUSTOMER INITIALS</b>
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER** 077C7042401**DATE TESTED** January 11, 2023**1. MECHANICAL CHECKS**

- |  |                             |
|--|-----------------------------|
| A. Inspect and clean all fans and filters.                                       | <input type="checkbox"/> OK |
| B. Inspect and replace as necessary, all torch components including the RF coil. | <input type="checkbox"/> OK |
| C. Inspect all tubing for sign of clacking or leaking.                           | <input type="checkbox"/> OK |
| D. Adjust water and gas pressure regulator settings.                             | <input type="checkbox"/> OK |
| E. Inspect and leak check pneumatics drawers.                                    | <input type="checkbox"/> OK |
| F. Clean the exterior of the instrument.   | <input type="checkbox"/> OK |

**2. OPTICAL CHECKS**

- |   |                             |
|---|-----------------------------|
| A. Inspect and clean all optical components.        | <input type="checkbox"/> OK |
| B. As required, check and replace all purgefilters. | <input type="checkbox"/> OK |
| C. Recheck optical alignment.                       | <input type="checkbox"/> OK |

**3. COOLING SYSTEM CHECKS**

- |   |                              |
|---|------------------------------|
| A. Perform preventive maintenance on chiller. | <input type="checkbox"/> OK  |
| B. Flush out the chiller every year.          | <input type="checkbox"/> N/A |

**4. PERFORMANCE CHECKS**

- |                            |                             |
|----------------------------|-----------------------------|
| A. Torch View Alignment.   | <input type="checkbox"/> OK |
| B. Wavelength Calibration. | <input type="checkbox"/> OK |



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER :** 077C7042401
**DATE TESTED :** January 11, 2023

PARAMETER		SPECIFICATION		FINAL VALUE	
<b>Spectral Resolution : UV</b>	<b>As</b> 193.696 nm	≤ 0.007		<u>0.00504</u>	
	<b>Ni</b> 231.604 nm	≤ 0.008		<u>0.00646</u>	
	<b>Ni</b> 341.476 nm	≤ 0.012		<u>0.00768</u>	
<b>Spectral Resolution : VIS</b>	<b>La</b> 408.672 nm	≤ 0.020		<u>0.01597</u>	
	<b>Ba</b> 455.403 nm	≤ 0.025		<u>0.02185</u>	
<b>Precision</b>					
	<b>As</b> 193.656 nm	% RSD	< 1.0	<u>0.89</u>	%
	<b>Zn</b> 213.856 nm	% RSD	< 1.0	<u>0.77</u>	%
	<b>Mn</b> 257.610 nm	% RSD	< 1.0	<u>0.51</u>	%
	<b>La</b> 379.478 nm	% RSD	< 1.0	<u>0.44</u>	%
	<b>Ba</b> 455.403 nm	% RSD	< 1.0	<u>0.44</u>	%
	<b>Ba</b> 493.408 nm	% RSD	< 1.0	<u>0.46</u>	%
<b>Detection Limits : Axial</b>	<b>Tl</b> 190.080 nm	3(sd)		<u>4.04</u>	ppb
	<b>As</b> 193.696 nm	3(sd)		<u>3.58</u>	ppb
	<b>Pb</b> 220.353 nm	3(sd)		<u>1.90</u>	ppb
<b>Detection Limits : Radial</b>	<b>As</b> 193.696 nm	3(sd)		<u>47.72</u>	ppb
	<b>Zn</b> 213.856 nm	3(sd)		<u>1.02</u>	ppb
	<b>Mn</b> 257.610 nm	3(sd)		<u>0.68</u>	ppb
	<b>La</b> 379.478 nm	3(sd)		<u>1.43</u>	ppb
	<b>Ba</b> 455.403 nm	3(sd)		<u>0.10</u>	ppb
	<b>Ba</b> 493.408 nm	3(sd)		<u>0.36</u>	ppb
<b>BEC : Axial (IB X 500)/(IS-IB)</b>	<b>Cd</b> 226.502 nm	≤ 150 ppb		<u>58.36</u>	
<b>BEC : Radial (IB X 1000)/(IS-IB)</b>	<b>Mn</b> 257.610 nm	≤ 45 ppb		<u>104142.80</u>	





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER** 077C7042401**DATE TESTED** January 11, 2023**Remarks :**

Commissioning follow as commissioning performance sheets.

---

---

---

---

---

---

---

---

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,  
including warranty terms.

**Service Department PerkinElmer Ltd.**

**Authorized Representative:**

( Mr. Wiphan Promlumda )

Service Engineer

ระดับความร้อนในสถานประกอบการ



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
[THERMAL ENVIRONMENT MONITOR]  
MANUFACTURER : METROSONICS  
MODEL / TYPE : hs-32  
SERIAL NO. : MCD070028  
CLID. NO. : 231802275  
JOB CONTROL NO. : 220901088338

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 01 September 2022

DATE OF ISSUED : 07 September 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Tanawan Seenam-Ngoen  
Calibration Engineer

Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
07 September 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22088338

F3-011-04/01-12

page 1 of 3



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
[THERMAL ENVIRONMENT MONITOR]  
MANUFACTURER : METROSONICS  
MODEL / TYPE : hs-32  
SERIAL NO. : MCD070028  
DATE OF CALIBRATION : 02 September 2022

---

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-74**. The calibration was performed by using

Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.

Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Thunder Scientific Corporation.

Certificate No. 19944, Due Date 26 January 2023.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22088338

F3-011-04/01-12

page 2 of 3





## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter [thermal environment monitor].

### CALIBRATION DATA

#### 1. CORRECTION OF TEMPERATURE : WET

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	30.01	30.0	+0.01	0.40
35.0	35.00	35.0	0.00	
40.0	40.02	40.0	+0.02	

#### 2. CORRECTION OF TEMPERATURE : DRY

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	30.01	29.8	+0.21	0.40
35.0	35.00	34.8	+0.20	
40.0	40.02	39.8	+0.22	

#### 3. CORRECTION OF TEMPERATURE : GLOBE BULB

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	30.01	29.5	+0.51	0.40
35.0	35.00	34.5	+0.50	
40.0	40.02	39.5	+0.52	

Note. The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q22088338

F3-011-04/01-12

page 3 of 3



@clccalibration



## Certificate of Calibration

Certificate Number : SPR23030505-7

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,  
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 34

Serial Number : TEH090208

ID. Number : R08

### Environmental Conditions

Ambient Temperature :  $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$

Received Date : 30 Mar 2023

Relative Humidity :  $50\% \pm 15\%$

Calibration Date : 31 Mar 2023

Location of Calibration : In-Lab

Recommend Due Date : 31 Mar 2024

Calibration Procedure : SP-CPT-04-13

Date of Issue : 01 Apr 2023

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Sarawut Khitmai

Calibration Officer

Approved by :

( Mr. Nirut Loha )

Authorized Signatory





## Calibration Report

Certificate Number : SPR23030505-7

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR23010480-5	22 Feb 2024
THERMO-HYGROMETER	5020A	A47046	QR23-0176	26 Jan 2024

### Traceability

This certification is traceable to the International System of Unit maintained at :

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

Quality Reborn Co., Ltd



## Result of Calibration

Certificate No. : SPR23030505-7

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
30.0	30.013	30.1	0.087	0.50
35.0	35.010	35.1	0.090	0.50
40.0	40.015	40.1	0.085	0.50

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
30.0	30.013	30.1	0.087	0.50
35.0	35.010	35.1	0.090	0.50
40.0	40.015	40.1	0.085	0.50

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
30.0	30.013	30.2	0.187	0.50
35.0	35.010	35.2	0.190	0.50
40.0	40.015	40.2	0.185	0.50

### Note:

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2$ , providing a level of confidence approximately 95%.

- End of Certificate -



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
(THERMAL ENVIRONMENT MONITOR)

MANUFACTURER : 3M

MODEL / TYPE : QUESTemp° 34

SERIAL NO. : TEF050029

CLID. NO. : 231802269

JOB CONTROL NO. : 221028109976

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 28 October 2022

DATE OF ISSUED : 31 October 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Oranut Kamchatphai  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
31 October 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units ( SI )

Certificate No. Q22109976

F3-011-04/01-12

page 1 of 3



@clccalibration



CLC  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOHYGRO METER  
(THERMAL ENVIRONMENT MONITOR)  
MANUFACTURER : 3M  
MODEL / TYPE : QUESTemp° 34  
SERIAL NO. : TEF050029  
DATE OF CALIBRATION : 29 October 2022

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-74**. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 44602.

Temperature & Humidity Chamber, PGC Model 9141-5116 S/N. 1304261.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Thunder Scientific Corporation.  
Certificate No. 19944, Due Date 26 January 2023.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22109976

F3-011-04/01-12

page 2 of 3



@clccalibration



## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermohygro meter (thermal environment monitor).

### CALIBRATION DATA

#### 1. CORRECTION OF TEMPERATURE : WET

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	30.01	29.8	+0.21	0.40
35.0	35.00	34.9	+0.10	
40.0	40.01	39.8	+0.21	

#### 2. CORRECTION OF TEMPERATURE : DRY

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	30.01	30.0	+0.01	0.40
35.0	35.00	35.2	-0.20	
40.0	40.01	40.1	-0.09	

#### 3. CORRECTION OF TEMPERATURE : GLOBE BULB

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
30.0	30.01	29.7	+0.31	0.40
35.0	35.00	34.8	+0.20	
40.0	40.01	39.8	+0.21	

Note. The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 36 of 111

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q22109976

F3-011-04/01-12

page 3 of 3





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Heat R025\_1

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No.	: R06	Verification Date	: 26 April 2023
Brand	: METROSONICS	Ambient Temp.	: 24.5 °C
Model	: hs-32	Barometric Pressure	: 1011 mmbar
Serial No.	: MCD070028	Relative Humidity	: 49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C , DB = 47.1 °C , G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.5	0.0	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.1	0.0	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.3	0.0	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by :

(Mr.Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com., www.spscon.com

Heat R025\_2

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No.	: R08	Verification Date	: 26 April 2023
Brand	: Quest Technologies	Ambient Temp.	: 24.5 °C
Model	: QUESTemp 34	Barometric Pressure	: 1011 mmbar
Serial No.	: TEH090208	Relative Humidity	: 49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C , DB = 47.1 °C , G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.6	-0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.0	0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.3	0.0	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by :   
(Mr. Adul Dangklom)

Approved by :   
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Heat R025\_4

### Heat Stress WBGT Meter Verification Report

#### Verification Data

Heat Stress WBGT Meter No.	: B17	Verification Date	: 26 April 2023
Brand	: 3M	Ambient Temp.	: 24.5 °C
Model	: QUESTemp <sup>o</sup> 34	Barometric Pressure	: 1011 mmbar
Serial No.	: TEF050029	Relative Humidity	: 49 %

Verification Module (Electronic Sensor Check) :

Verification Module No. : 21 WB = 12.5 °C , DB = 47.1 °C , G = 69.3 °C

#### Result of Verification : Without Adjustment

##### Wet Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.7	-0.2	± 0.5

##### Dry Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.3	-0.2	± 0.5

##### Globe Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5

UUC\* = UNIT UNDER CALIBRATION

Verified by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



คุณภาพอากาศในสถานประกอบการ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spsccon.com.. www.spsccon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
R01	SKC	224-PCXR4	602467	10/04/2023	1,000	1,500	2,000	992	1,507	2,005	1.009x - 15.491	1.000
R02	SKC	224-PCXR4	626450	10/04/2023	1,000	2,000	3,000	997	1,497	1,989	0.990x + 10.155	1.000
R03	SKC	224-PCXR4	691592	10/04/2023	1,000	1,500	2,000	1,005	1,498	2,003	1.010x - 19.567	0.999
R04	SKC	224-PCXR4	691672	04/04/2023	1,000	1,500	2,000	998	1,491	1,997	0.998x - 1.962	1.000
R05	SKC	224-PCXR4	798470	10/04/2023	1,000	1,500	2,000	994	1,506	1,998	1.012x - 28.038	0.999
R06	SKC	224-PCXR4	798456	05/04/2023	1,000	1,500	2,000	993	1,497	1,995	1.004x - 10.749	1.000
R07	SKC	224-PCXR4	798480	10/04/2023	1,000	1,500	2,000	996	1,492	1,998	1.005x - 11.766	1.000
R08	SKC	224-PCXR4	883215	10/04/2023	1,000	1,500	2,000	1,010	1,503	2,003	0.998x + 3.526	1.000
R09	SKC	224-PCXR4	034650	04/04/2023	1,000	1,500	2,000	994	1,505	2,003	1.017x - 33.985	0.999
R10	SKC	224-PCXR4	091765	07/04/2023	1,000	1,500	2,000	998	1,492	1,996	1.000x - 3.929	1.000
R11	SKC	224-PCXR4	091763	04/04/2023	1,000	1,500	2,000	1,002	1,497	2,003	1.012x - 23.883	0.999
R12	SKC	224-PCXR4	091568	10/04/2023	1,000	1,500	2,000	995	1,503	1,998	1.002x - 7.698	1.000
R13	SKC	224-PCXR4	091638	10/04/2023	1,000	1,500	2,000	1,005	1,497	1,993	0.989x + 13.679	1.000
R14	SKC	224-PCXR4	091764	10/04/2023	1,000	1,500	2,000	992	1,503	1,998	1.015x - 32.167	0.999
R15	SKC	224-PCXR8	529457	10/04/2023	1,000	1,500	2,000	1,003	1,501	2,005	1.005x - 9.429	1.000
R16	SKC	224-PCXR8	529643	04/04/2023	1,000	1,500	2,000	999	1,496	1,995	0.999x - 3.290	1.000
R17	SKC	224-PCXR8	529645	05/04/2023	1,000	1,500	2,000	995	1,511	2,001	1.012x - 23.233	0.999
R18	SKC	224-PCXR8	566756	07/04/2023	1,000	1,500	2,000	992	1,497	1,999	1.002x - 7.359	1.000
R19	SKC	224-PCXR8	566802	07/04/2023	1,000	1,500	2,000	1,002	1,498	1,999	1.009x - 19.671	0.999
R20	SKC	224-PCXR8	529089	07/04/2023	1,000	1,500	2,000	992	1,501	2,004	1.015x - 28.270	1.000
R21	SKC	224-PCXR8	665728	10/04/2023	1,000	1,500	2,000	997	1,494	1,997	1.001x - 7.797	1.000
R22	SKC	224-PCXR8	707444	05/04/2023	1,000	1,500	2,000	1,003	1,501	2,003	1.003x - 6.218	1.000
R23	SKC	224-PCXR8	761067	10/04/2023	1,000	1,500	2,000	996	1,495	1,993	0.995x + 0.263	1.000
R24	SKC	224-PCXR8	707893	10/04/2023	1,000	1,500	2,000	997	1,506	2,002	1.009x - 17.713	0.999
R25	SKC	224-PCXR8	761052	10/04/2023	1,000	1,500	2,000	1,009	1,497	1,992	0.983x + 22.945	1.000
R26	SKC	224-PCXR8	707956	10/04/2023	1,000	1,500	2,000	1,004	1,502	2,005	1.008x - 14.326	0.999
R27	SKC	224-PCXR8	707398	07/04/2023	1,000	1,500	2,000	995	1,502	2,002	1.007x - 16.361	1.000
R28	SKC	224-PCXR8	707481	10/04/2023	1,000	1,500	2,000	1,006	1,501	2,003	1.009x - 18.291	0.999
R29	SKC	224-PCXR8	707402	07/04/2023	1,000	1,500	2,000	1,002	1,494	1,989	0.987x + 14.566	1.000
R30	SKC	224-PCXR8	093811	04/04/2023	1,000	1,500	2,000	1,001	1,494	1,996	0.997x + 0.646	1.000
R31	SKC	224-PCXR8	093183	10/04/2023	1,000	1,500	2,000	1,001	1,502	2,004	1.004x - 5.652	1.000
R32	SKC	224-PCXR8	671950	05/04/2023	1,000	1,500	2,000	999	1,501	1,993	0.994x + 7.163	1.000
R33	SKC	224-PCXR4	626254	10/04/2023	1,000	1,500	2,000	996	1,504	2,001	1.015x - 30.192	0.999
R34	SKC	224-PCXR4	626131	04/04/2023	1,000	1,500	2,000	1,003	1,498	2,004	1.004x - 9.377	1.000
R35	SKC	224-PCXR8	707460	10/04/2023	1,000	1,500	2,000	998	1,496	1,996	0.996x + 3.677	1.000
R36	SKC	224-PCXR8	707446	10/04/2023	1,000	1,500	2,000	1,003	1,498	2,002	1.010x - 20.668	0.999
R37	SKC	224-PCXR8	707432	10/04/2023	1,000	1,500	2,000	998	1,496	2,000	0.999x - 0.873	1.000
R38	SKC	224-PCXR8	707349	07/04/2023	1,000	1,500	2,000	997	1,497	2,001	1.003x - 8.747	1.000
R39	SKC	224-PCXR8	761095	10/04/2023	1,000	1,500	2,000	1,001	1,497	1,997	0.999x + 0.140	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
H-R01	Dwyer	VFB-65	05/04/2023	500	1,000	2,000	502.1	993.6	1981.1	1.000x - 3.647	0.999
H-R02	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	500.4	998.7	1988.7	1.001x - 3.457	1.000
H-R03	Dwyer	VFB-65	07/04/2023	500	1,000	2,000	502.1	990.3	1997.7	0.993x + 4.022	1.000
H-R04	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	497.2	992.2	2016.9	1.007x - 11.203	1.000
H-R05	Dwyer	VFB-65	05/04/2023	500	1,000	2,000	499.2	988.5	1990.7	1.003x - 7.136	1.000
H-R06	Dwyer	VFB-65	10/04/2023	500	1,000	2,000	504.8	994.6	1982.6	0.999x - 1.961	0.999

Calibrated by :

(Mr. Abdul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
L-R01	Dwyer	VFA-21	05/04/2023	50	100	200	50.2	101.0	204.3	0.981x + 2.956	0.999
L-R02	Dwyer	VFA-21	10/04/2023	50	100	200	50.1	102.0	201.0	1.007x - 0.506	0.999
L-R03	Dwyer	VFA-21	07/04/2023	50	100	200	50.1	100.2	202.7	1.015x - 0.825	1.000
L-R04	Dwyer	VFA-21	10/04/2023	50	100	200	50.2	100.9	200.6	1.005x - 0.751	0.999
L-R05	Dwyer	VFA-21	05/04/2023	50	100	200	50.2	101.0	202.6	0.994x + 1.409	1.000
L-R06	Dwyer	VFA-21	10/04/2023	50	100	200	50.8	100.2	202.3	1.001x + 0.717	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



ระดับเสียงในสถานประกอบการ

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

## CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.  
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.  
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.  
4. Digital Multimeter Agilent 34401A S/N MY44005560.  
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.  
6. Audio Analyzer Keithley 2015-P S/N 4106495.  
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

**Calibration Procedure:** CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 27 Mar. 2023

Date of Calibration : 29 Mar. 2023

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa , Corrected to Reference Conditions : 101.325 kPa , 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.94	-0.06	$\pm 0.10$	$\pm 0.40$ dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	$\pm 1.5$	$\pm 1.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.80	$\pm 0.50$	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

...

(Mr.Weerachai Deechaiyae)

Approved by :

...

(Mr.Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 29 Mar. 2023

Date of Issue : 30 Mar. 2023

Ref : 2011266032701228001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise R\_222/23

## Sound Level Meter Calibration Report

### Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	29 March 2023
		Due Date	29 March 2024

### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B18	ACO	6236	00172048	26 April 2023	94.1	94.0
ACO-B29	ACO	6236	00182011	26 April 2023	94.0	94.0
ACO-B33	ACO	6236	00182015	26 April 2023	94.1	94.0
ACO-B36	ACO	6236	00192027	26 April 2023	94.0	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.94 ± 0.10 dB	

Calibrated by :

(Mr.Adul Dangklom )

Approved by :

(Mr. Peera Detudom)



Noise Dose
------------

Request No. 21-65/0760

MTC No. EEL. BP. 24/0965

## CALIBRATION CERTIFICATE

Submitted by : S.P.S. CONSULTING SERVICE CO., LTD.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Acoustic Calibrator

Manufacturer : SVANTEK

Model : SV34

Serial No. : 33139

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.

7. Condenser Microphone Bruel&Kjaer 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 13 Sep. 2022

Date of Calibration : 19 Sep. 2022

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



Request No. 21-65/0760

MTC No. EEL. BP. 24/0965

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

**Nominal Output of Unit Under Test = 114 dB re 20 $\mu$ Pa at 1000 Hz****Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.****1. Sound Pressure Level**

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	113.63	-0.37	$\pm 0.10$	$\pm 0.75$ dB

**2. Frequency**

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	$\pm 1.5$	$\pm 2.0$ %

**3. Total Distortion**

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	0.24	$\pm 0.50$	$\pm 4.0$ %

- Note :**
1. No adjustment.
  2. The calibrator pressure correction was not included.
  3. The microphone volume correction was not included.

Calibrated by :



(Mr. Nuttapong Niljrusvanit)

Approved by :



(Mr. Prawate Kluaypa)

Director

**Electrical and Electronic Standards Laboratory**  
**Industrial Metrology and Testing Service Centre**

Date of Calibration : 19 Sep. 2022

Date of Issue : 20 Sep. 2022

Ref : 2011265091304034002

2 / 2

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website: www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise Dose R\_684/22

## Noise Dose Meter Calibration Report

### Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 06/62
Model	SV34	Serial No.	33139
Calibration Range	114 dB, 1000 Hz	Last Calibration	19 September 2022
		Due Date	19 September 2023

### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R06	ACO	6236	00152005	05 December 2022	113.5	113.6
ACO-R13	ACO	6236	00172041	05 December 2022	113.6	113.6
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					113.63 ± 0.10 dB	

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

Noise Dose R\_225/23

## Noise Dose Meter Calibration Report

### Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 06/62
Model	SV34	Serial No.	33139
Calibration Range	114 dB, 1000 Hz	Last Calibration	19 September 2022
		Due Date	19 September 2023

### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B02	SVANTEK	SV-104IS	80842	27 April 2023	113.6	113.6
NMD-B03	SVANTEK	SV-104IS	80852	27 April 2023	113.5	113.6
NMD-B04	SVANTEK	SV-104IS	80854	27 April 2023	113.6	113.6
NMD-B08	SVANTEK	SV-104IS	80818	27 April 2023	113.6	113.6
NMD-B09	SVANTEK	SV-104IS	80829	27 April 2023	113.5	113.6
NMD-B10	SVANTEK	SV-104IS	80830	27 April 2023	113.6	113.6
NMD-B11	SVANTEK	SV-104IS	80831	27 April 2023	113.6	113.6
NMD-B12	SVANTEK	SV-104IS	80832	27 April 2023	113.6	113.6
NMD-B13	SVANTEK	SV-104IS	80834	27 April 2023	113.5	113.6
NMD-B19	SVANTEK	SV-104IS	106124	27 April 2023	113.6	113.6
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					113.63± 0.10 dB	

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Noise Dose R\_312/23

### Noise Dose Meter Calibration Report

Acoustic Calibrator Data						
Brand	SVANTEK			Number	SV 06/62	
Model	SV34			Serial No.	33139	
Calibration Range	114 dB, 1000 Hz			Last Calibration	19 September 2022	
				Due Date	19 September 2023	
Calibration Data						
Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R22	SVANTEK	SV-104IS	80801	21 June 2023	113.5	113.6
NMD-R26	SVANTEK	SV-104IS	80836	21 June 2023	113.5	113.6
NMD-R27	SVANTEK	SV-104IS	80837	21 June 2023	113.6	113.6
NMD-R35	SVANTEK	SV-104IS	80873	21 June 2023	113.5	113.6
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					113.63± 0.10 dB	

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)