

## เอกสารสอบเทียบเครื่องมือที่ใช้ในการวิเคราะห์



CERTIFICATE No : 23E0843

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : pH METER  
MANUFACTURER : DKK-TOA  
ID No : EQL-183  
RECEIVED DATE : 27-Jan-23  
AMBIENT TEMPERATURE : 23° C ± 1° C  
MODEL : HM-25R  
SERIAL NUMBER : 760205  
CALIBRATION DATE : 27-Jan-23  
RELATIVE HUMIDITY : 51 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

- THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTROD WAS CALIBRATED BY USING STANDARD pH BUFFER SOLUTION.
- REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No/ LOT No	CERTIFICATE No	DUE DATE
1) pH STANDARD SOLUTION	00651-06	CC719181	4880-12119147	05-Apr-23
2) pH STANDARD SOLUTION	00651-08	CC718727	4881-12110709	31-Mar-23
3) pH STANDARD SOLUTION	00651-10	CC717045	4882-12065386	17-Mar-23
4) PROCESS CALIBRATOR	CA150	91S6079	22E1145	31-Mar-23
5) BATH	260014	124748074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

- THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION.
- THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

- THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
  - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
  - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

### RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

#### 1. DISPLAY UNIT WITH pH ELECTRODE S/N: 202F0138MK

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	ACTUAL READING (mV)	UNCERTAINTY OF MEASUREMENT (± pH)	COVERAGE FACTOR k
4.007	4.01	-0.003	178	0.013	2.0
7.004	7.00	0.004	0.0	0.013	2.0
10.014	10.01	0.004	-177	0.014	2.0

#### 2. DISPLAY UNIT MEASUREMENT TEMPERATURE WITH PROBE

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
25.002	25.0	80	0.002	0.21

#### 3. PERCENT SLOPE 98%

UUC : UNIT UNDER CALIBRATION

THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.  
END OF CALIBRATION REPORT

*[Signature]*

F-G010 REV 02

CERTIFICATE No : 23E0843

REFERENCE No : 67999-1

## Certificate of Calibration

EQUIPMENT : pH METER  
MANUFACTURER : DKK-TOA  
MODEL : HM-25R  
SERIAL No : 760205  
ID No : EQL-183  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT P.  
CALIBRATION DATE : 27-Jan-23  
APPROVED BY : *[Signature]* PONGSAK J.  
ISSUED DATE : 03-Jan-23  
RECEIVED DATE : 27-Jan-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV 02





CERTIFICATE No : 22T8989

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : INCUBATOR  
MANUFACTURER : N/A  
ID No : EQL-182  
RECEIVED DATE : 19-Aug-22  
AMBIENT TEMPERATURE : 27 °C ± 1 °C  
MODEL : N/A  
SERIAL NUMBER : N/A  
CALIBRATION DATE : 19-Aug-22  
RELATIVE HUMIDITY : 51 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 13 POINTS AND LOCATED AS THE PICTURE BELOW AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE SEVENTH THERMOCOUPLE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

### 2. REFERENCE STANDARD INSTRUMENTS :-

- INSTRUMENT MODEL SERIAL No CERTIFICATE No DUE DATE
- 1) DATA LOGGER WITH TC TYPE K HYDRA 2635A 7301307 22T7508 05-Jul-23
3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

#### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 3  
Overall Line Voltage (V) variation : 3  
Instrument Condition : Normal  
Chamber Size (W\*H) : 190\*70\*170 cm

#### CHAMBER PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
20.0	19.90	0.05	0.46	0.69

#### TEMPERATURE MEASUREMENT ACCURACY TEST


Controller temperature (°C)	20.0
Indicating Temperature	19.7
Measured Temperature (°C) at Spread Locations	1 20.16
	2 19.79
	3 20.07
	4 19.63
	5 19.89
	6 19.87
	7 Ref. 20.08
	8 19.76
	9 19.67
	10 19.97
	11 20.30
	12 19.82
	13 19.73
Uncertainty of Measurement (± °C)	0.39

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 7 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%  
END OF CALIBRATION REPORT

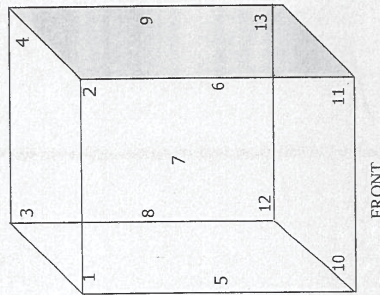

CERTIFICATE No : 22T8989  
REFERENCE No : 66263-2

## Certificate of Calibration

EQUIPMENT : INCUBATOR  
MANUFACTURER : N/A  
MODEL : N/A  
SERIAL No : N/A  
ID No : EQL-182  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEADAM,  
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.  
CALIBRATION DATE : 19-Aug-22

APPROVED BY : PONGSAK J.  
ISSUED DATE : 19-Aug-22  
RECEIVED DATE : 19-Aug-22





CERTIFICATE No : 22M9914

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE : GR-200  
MANUFACTURER : AND : 14243876  
ID No : EQL-130  
AIR PRESSURE : 101mmbar ± 1mmbar  
AMBIENT TEMPERATURE : 21° C ± 1° C  
RELATIVE HUMIDITY : 55 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING WEIGHT OF QUALITY CALIBRATION TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-1-151	C02210415	09-Feb-23
2) STANDARD WEIGHT	E2	15843	C02210419	10-Feb-23
3) STANDARD WEIGHT	E2	QK-1-349	M21032355	26-Mar-23

4. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

3. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-


- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 200 g WAS 0.000048 g
4. DEPARTURE FROM NOMINAL VALUE/LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.00	0.0000	0.0000	0.000078
0.10	0.1000	0.0000	0.000078
0.20	0.2000	0.0000	0.000078
0.50	0.5000	0.0000	0.000079
1.00	1.0000	0.0000	0.000079
2.00	2.0000	0.0000	0.000080
5.00	5.0000	0.0000	0.000081
10.00	10.0000	0.0000	0.000084
20.00	20.0001	-0.0001	0.000089
50.00	50.0001	-0.0001	0.00011
100.00	100.0001	-0.0001	0.00019
200.00	200.0000	0.0000	0.00032

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0001
4	100.0000
5	99.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT PRODUCTION AREA. THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 22T9917

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : HOT AIR OVEN  
MANUFACTURER : MEMMERT  
MODEL : UFE 500  
ID No : EQL-128  
RECEIVED DATE : 15-Sep-22  
AMBIENT TEMPERATURE : 25 °C ± 1 °C

S/N : G508.0791  
CALIBRATION DATE : 15-Sep-22  
RELATIVE HUMIDITY : 51 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLA5 G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.


### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT : MODEL : SERIAL No : CERTIFICATE No : DUE DATE :  
1) DATA LOGGER WITH RTD HYDRA 2635A 6635300 22T7509 10-Jul-23  
3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

#### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1  
Overall Line Voltage (V) variation : 3  
Instrument Condition : Normal  
Chamber Size (W\*L\*H) : 56\*40\*48 cm



#### CHAMBER PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.32	0.15	0.62	1.02
180.0	180.09	0.29	1.23	1.86

#### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	#5	#6	#7	#8	#9	
104.0	104.0	104.23	103.89	104.54	104.02	104.33	104.63	104.42	104.48	104.39	0.38
180.0	180.0	180.16	179.13	180.46	179.35	179.79	180.66	180.36	180.29	180.61	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.  
END OF CALIBRATION REPORT

Signature

F-G010 REV : 02

CERTIFICATE No : 22T9917  
REFERENCE No : 66549-4

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : HOT AIR OVEN  
MANUFACTURER : MEMMERT  
MODEL : UFE 500  
SERIAL No : G508.0791  
ID No : EQL-128  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
3032 RAMA II SOI 63, RAMA II RD., SAMAEADAM,  
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.  
CALIBRATION DATE : 15-Sep-22

APPROVED BY : PONGSAK J.  
ISSUED DATE : 21-Sep-22  
RECEIVED DATE : 15-Sep-22





CERTIFICATE No : 22T9920

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT	:	WATER BATH	MODEL	:	SUP IV
MANUFACTURER	:	N/A	SERIAL NUMBER	:	N/A
ID NUMBER	:	EQL-056	CALIBRATION DATE	:	15-Sep-22
RECEIVED DATE	:	15-Sep-22	RELATIVE HUMIDITY	:	49%RH ± 10 % RH
AMBIENT TEMPERATURE	:	25 °C ± 1 °C			


### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO ASTM E715-80 (REAPPROVED 2001) BY COMPARISON WITH CALIBRATED RTD. THE PROBES WERE PLACED ON FIVE POINTS AND LOCATED ONE PROBE IN EACH OF THE FOUR CORNERS OF THE BATH AND PLACED THE FIFTH RTD WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE WATER VOLUME (REFERENCE LOCATION) UNDER NO LOAD CONDITION.

### 2. REFERENCE STANDARD INSTRUMENTS :-

- 1) DATA LOGGER WITH RTD  
MODEL : 2625A  
SERIAL No : 6603614  
CERTIFICATE No : 22T7514  
DUE DATE : 05-Jul-23
3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT



PROBE INSTALLATION  
POSITION IN THE BATH

### GENERAL INFORMATION

Overall Variation of Ambient Temperature around the Bath (°C) : 0.6
Overall Variation of Line Voltage (V) : 3
Instrument Condition : Normal
Bath Inner Size (W*L*H) : 59*35*20 cm

### BATH PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
83.0	82.94	0.07	0.04	0.17

### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Measured Temperature (°C) at Spread Locations					Uncertainty (± °C)
	#1	#2	#3	#4	Ref. 5	
83.0	82.93	82.92	82.93	82.96	82.95	0.16

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE BATH.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

*[Signature]*

F-G010 REV : 02

CERTIFICATE No : 22T9920  
REFERENCE No : 66549-7

## Certificate of Calibration

EQUIPMENT	:	WATER BATH
MANUFACTURER	:	N/A
MODEL	:	SUP IV
SERIAL No	:	N/A
ID No	:	EQL-056
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	TEST TECH CO., LTD. 30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM, BANGKHUNTHIAN, BANGKOK 10150
CALIBRATED BY	:	PRASERT P.
CALIBRATION DATE	:	15-Sep-22

APPROVED BY	:	<i>[Signature]</i> PONGSAK J.
ISSUED DATE	:	21-Sep-22
RECEIVED DATE	:	15-Sep-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02





CERTIFICATE No : 22M7652

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE : QUINTIX 224-15  
MANUFACTURER : SARTORIUS : 29302452  
ID No : EQL-164 : 14-Jul-22  
AIR PRESSURE : 1008mbar  $\pm$  1mbar : 57 %RH  $\pm$  10 % RH  
AMBIENT TEMPERATURE : 26° C  $\pm$  1° C

**CONDITION OF THIS RESULTS OF CALIBRATION**  
1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING WEIGHT OF QUALITY CALIBRATION TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

1) STANDARD WEIGHT SET E2 : QUINTIX 224-15  
2) STANDARD WEIGHT E2 : 29302452  
3) STANDARD WEIGHT E2 : 14-Jul-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.


5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

**RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT**

1. ZERO SETTING FUNCTION : NORMAL  
2. TARE FUNCTION : NORMAL  
3. REPEATABILITY OF READING AT 200 g WAS 0.000042 g  
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.0	0.0000	0.0000	0.000073
0.1	0.1000	0.0000	0.000074
0.2	0.2000	0.0000	0.000074
1.0	1.0000	0.0000	0.000075
2.0	2.0000	0.0000	0.000085
20.0	20.0000	0.0000	0.00014
45.0	45.0001	-0.0001	0.00013
65.0	65.0001	-0.0001	0.00017
80.0	80.0001	-0.0001	0.00019
100.0	100.0000	0.0000	0.00022
120.0	120.0000	0.0000	0.00025
140.0	140.0000	0.0000	0.00027
160.0	160.0000	0.0000	0.00030
180.0	180.0000	0.0000	0.00032
200.0	199.9998	0.0002	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	99.9999
2	99.9998
3	99.9998
4	99.9999
5	99.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA. THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

CERTIFICATE No : 22M7652  
REFERENCE No : 65843-6

## Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE  
MANUFACTURER : SARTORIUS  
MODEL : QUINTIX 224-15  
SERIAL No : 29302452  
ID No : EQL-164  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD.,  
SAMAEDAM, BANGKHUNTHIAN, BANGKOK  
10150

CALIBRATED BY : TETNITHI W.  
CALIBRATION DATE : 14-Jul-22  
APPROVED BY : PONGSAK J.  
ISSUED DATE : 15-Jul-22  
RECEIVED DATE : 14-Jul-22