

ภาคผนวก จ

เอกสารสอบเทียบเครื่องมือ

ภาคผนวก ฉ-1

เอกสารสอบเทียบเครื่องมือ
บริษัท เอส. พี. เอส. คอนซัลติ้ง เซอร์วิส จำกัด

ตารางสรุปรายการสอบเทียบเครื่องมือ

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
คุณภาพอากาศ - Total Suspended Particulate (TSP) - Particulate Matter less than 10 micron (PM-10) - Carbon Monoxide (CO) - Nitrogen Dioxide (NO ₂)	- High Volume Air Sampler - High Volume PM-10 Air Sampler - CO Analyzer - NO ₂ Analyzer	- Electronic Balance - Electronic Balance - CO Analyzer - NO ₂ Analyzer



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B35	B35	01/02/2023	y = 1.194x-4.992	0.995
B36	B36	02/02/2023	y = 1.201x-3.946	0.997
B37	B37	02/02/2023	y = 1.284x-6.745	0.997
B38	B38	02/02/2023	y = 1.250x-6.733	0.998
B39	B39	01/02/2023	y = 1.268x-7.186	0.998
B40	B40	03/02/2023	y = 1.214x-4.324	0.998
B41	B41	03/02/2023	y = 1.176x-2.734	0.999
B42	B42	02/02/2023	y = 1.283x-8.167	0.997
B43	B43	02/02/2023	y = 1.197x-3.772	0.996
B44	B44	02/02/2023	y = 1.249x-7.038	0.995
R01	R01	01/02/2023	y = 1.287x-8.462	0.998
R02	R02	01/02/2023	y = 1.239x-6.678	0.998
R03	R03	03/02/2023	y = 1.254x-7.928	0.999
R04	R04	02/02/2023	y = 1.206x-3.694	0.999
R05	R05	02/02/2023	y = 1.237x-6.503	0.997
R06	R06	02/02/2023	y = 1.239x-4.541	0.995
R07	R07	03/02/2023	y = 1.060x+1.983	0.999
R08	R08	03/02/2023	y = 1.274x-8.050	0.998
R09	R09	02/02/2023	y = 1.280x-7.005	0.998
R10	R10	03/02/2023	y = 1.244x-5.980	1.000
R11	R11	03/02/2023	y = 1.097x-0.462	0.998
R12	R12	02/02/2023	y = 1.151x-2.727	0.995
R13	R13	02/02/2023	y = 1.134x-1.526	1.000
R14	R14	02/02/2023	y = 1.172x-2.510	0.999
R15	R15	01/02/2023	y = 1.131x-2.129	0.998
R16	R16	01/02/2023	y = 1.202x-5.830	0.998
R17	R17	01/02/2023	y = 1.182x-3.281	0.998
R18	R18	03/02/2023	y = 1.217x-5.060	0.999
R19	R19	03/02/2023	y = 1.228x-6.084	0.998
R20	R20	03/02/2023	y = 1.277x-9.434	0.997

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B01	B01	01/02/2023	y = 1.278x-5.652	0.997
B02	B02	02/02/2023	y = 1.147x+0.663	0.999
B03	B03	01/02/2023	y = 1.123x-0.622	0.995
B04	B04	01/02/2023	y = 1.229x-4.835	0.996
B05	B05	02/02/2023	y = 1.280x-6.358	0.997
B06	B06	01/02/2023	y = 1.251x-5.438	0.999
B07	B07	03/02/2023	y = 1.165x-3.515	0.996
B08	B08	03/02/2023	y = 1.269x-7.559	0.997
B09	B09	01/02/2023	y = 1.198x-2.843	0.998
B10	B10	01/02/2023	y = 1.128x+0.785	0.999
B11	B11	02/02/2023	y = 1.138x-1.752	0.999
B12	B12	01/02/2023	y = 1.195x-4.080	0.998
B13	B13	01/02/2023	y = 1.254x-5.913	0.999
B14	B14	03/02/2023	y = 1.291x-7.822	0.999
B15	B15	01/02/2023	y = 1.149x-1.829	0.997
B16	B16	01/02/2023	y = 1.287x-7.502	0.997
B17	B17	02/02/2023	y = 1.207x-4.147	1.000
B18	B18	01/02/2023	y = 1.277x-7.238	0.999
B19	B19	03/02/2023	y = 1.243x-6.520	0.995
B20	B20	01/02/2023	y = 1.267x-7.055	1.000
B21	B21	03/02/2023	y = 1.141x-1.101	0.999
B22	B22	03/02/2023	y = 1.221x-5.534	0.996
B23	B23	02/02/2023	y = 1.197x-4.328	0.995
B24	B24	01/02/2023	y = 1.159x-2.269	0.999
B25	B25	01/02/2023	y = 1.050x+2.684	0.998
B26	B26	03/02/2023	y = 1.253x-6.203	0.997
B27	B27	03/02/2023	y = 1.220x-5.822	0.997
B28	B28	01/02/2023	y = 1.251x-6.762	0.999
B29	B29	01/02/2023	y = 1.201x-3.793	0.998
B30	B30	03/02/2023	y = 1.242x-6.540	0.995
B31	B31	03/02/2023	y = 1.255x-6.608	0.999
B32	B32	02/02/2023	y = 1.249x-6.292	0.997
B33	B33	02/02/2023	y = 1.260x-5.168	0.997
B34	B34	01/02/2023	y = 1.272x-7.454	1.000

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard Model : TE 5025A S/N : 3611


Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (l ³ /min)	R ²
R01	R01	01/02/2023	y = 1.253x-8.016	0.996
R02	R02	01/02/2023	y = 1.246x-5.052	0.998
R03	R03	02/02/2023	y = 1.239x-5.451	0.999
R04	R04	03/02/2023	y = 1.263x-8.320	0.999
R05	R05	03/02/2023	y = 1.193x-4.904	0.998
R06	R06	03/02/2023	y = 1.270x-7.534	0.995
R07	R07	03/02/2023	y = 1.244x-5.727	0.998
R08	R08	02/02/2023	y = 1.277x-7.820	0.998
R09	R09	02/02/2023	y = 1.183x-5.015	0.996
R10	R10	01/02/2023	y = 1.200x-4.576	0.999
R11	R11	01/02/2023	y = 1.225x-4.833	0.995
R12	R12	03/02/2023	y = 1.273x-8.109	0.998
R13	R13	01/02/2023	y = 1.281x-6.830	1.000
R14	R14	01/02/2023	y = 1.288x-7.622	0.999
R15	R15	02/02/2023	y = 1.282x-8.311	0.997
R16	R16	02/02/2023	y = 1.246x-5.817	0.995
R17	R17	03/02/2023	y = 1.263x-7.123	0.999
R18	R18	03/02/2023	y = 1.203x-5.483	0.999
R19	R19	01/02/2023	y = 1.204x-4.399	0.996
R20	R20	01/02/2023	y = 1.259x-8.655	0.997

Calibrated by :


 (Mr. Adul Dangklom)

Approved by :


 (Mr. Peera Detudom)

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard Model : TE 5025A S/N : 3611


Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (l ³ /min)	R ²
B01	B01	02/02/2023	y = 1.210x-0.261	0.997
B02	B02	02/02/2023	y = 1.046x-2.414	0.998
B03	B03	02/02/2023	y = 1.199x-4.047	0.996
B04	B04	02/02/2023	y = 1.288x-7.602	0.997
B05	B05	01/02/2023	y = 1.222x-4.886	1.000
B06	B06	01/02/2023	y = 1.210x-3.612	0.996
B07	B07	03/02/2023	y = 1.270x-6.088	0.999
B08	B08	01/02/2023	y = 1.277x-5.288	0.998
B09	B09	03/02/2023	y = 1.289x-6.478	0.999
B10	B10	03/02/2023	y = 1.266x-8.106	0.997
B11	B11	01/02/2023	y = 1.258x-6.917	0.995
B12	B12	02/02/2023	y = 1.192x-3.640	0.998
B13	B13	02/02/2023	y = 1.289x-7.913	0.998
B14	B14	02/02/2023	y = 1.250x-4.233	0.999
B15	B15	01/02/2023	y = 1.118x-0.802	0.999
B16	B16	03/02/2023	y = 1.297x-3.106	0.998
B17	B17	01/02/2023	y = 1.204x-4.477	0.996
B18	B18	02/02/2023	y = 1.176x-1.624	0.998
B19	B19	02/02/2023	y = 1.097x-1.230	0.999
B20	B20	03/02/2023	y = 1.188x-4.372	0.999
B21	B21	03/02/2023	y = 1.156x-0.146	0.996
B22	B22	03/02/2023	y = 1.269x-6.647	0.998
B23	B23	02/02/2023	y = 1.197x-2.685	1.000
B24	B24	02/02/2023	y = 1.251x-6.437	0.995
B25	B25	01/02/2023	y = 1.144x-2.851	0.997
B26	B26	01/02/2023	y = 1.249x-5.704	0.996
B27	B27	01/02/2023	y = 1.241x-5.428	0.997
B28	B28	01/02/2023	y = 1.198x-4.626	0.998
B29	B29	02/02/2023	y = 1.244x-7.658	0.997
B30	B30	02/02/2023	y = 1.246x-7.229	0.997
B31	B31	02/02/2023	y = 1.178x-0.243	0.995
B32	B32	03/02/2023	y = 1.201x-2.954	0.998
B33	B33	03/02/2023	y = 1.168x-1.341	0.997
B34	B34	01/02/2023	y = 1.237x-2.684	0.995

Calibrated by :


 (Mr. Adul Dangklom)

Approved by :


 (Mr. Peera Detudom)



CERTIFICATE No : 23M2445

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
ID No : BA 10/62
AIR PRESSURE : 1010mbar \pm 1mbar
AMBIENT TEMPERATURE : 23°C \pm 1°C

MODEL : XSR105DU
S/N : B926859981
RECEIVED DATE : 10-Mar-23
CALIBRATION DATE : 10-Mar-23
RELATIVE HUMIDITY : 49%RH \pm 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 100 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20000	0.00000	0.000040
0.50	0.50000	0.00000	0.000040
1.00	1.00001	-0.00001	0.000041
2.00	2.00000	0.00000	0.000042
5.00	5.00000	0.00000	0.000046
10.00	10.00004	-0.00004	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00005	-0.00005	0.00011
100.00	100.00009	-0.00009	0.00019
120.00	120.00015	-0.00015	0.00019

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.00000
2	50.00003
3	50.00000
4	49.99997
5	50.00003
OFF-CENTER LOADING	0.00003

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 23M2445

REFERENCE No : 68471-5

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XSR105DU
SERIAL No : B926859981
ID No : BA 10/62
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY : PONGSAK J.

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
NON-DISPERSIVE INFRARED CO ANALYZER					
DATE :	31 March 2023	BRAND :	API	MODEL :	300E
NO.	CO-B06	SERIAL NO.	3117		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 06 September 2022		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Carbon Monoxide (CO)		Cylinder No.	: D196045	
Certified Date	: 16 April 2022	Expired Date	: 15 April 2024	Cylinder Conc.	: 4,570 PPM
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	48				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	0.10	-	0	
CO Span	40.00	40.06	0.150	40.00	
API Model 300E CO Analyzer Check list					
Parameter	Observed Value	Units	Nominal Range		
RANGE	50	PPM	0-1000 ppm		
STABILITY	0.10	PPM	< 1 ppm with zero air		
CO MEASURE	4016.3	mV	2500-4800 mV		
CO REFERENCE	3947.1	mV	2500-4800 mV		
MEASURE/REFERENCE RATIO	1.180	-	1.1-1.3 w/zero air		
SAMPLE PRESSURE	28.4	In-Hg-A	~2" < ambient absolute pressure		
SAMPLE FLOW	810	cc/min	800 ± 10%		
SAMPLE TEMPERATURE	48.2	°C	48 ± 4		
BENCH TEMPERATURE	48.0	°C	48 ± 2		
WHEEL TEMPERATURE	68.4	°C	68 ± 2		
BOX TEMPERATURE	30.7	°C	Ambient temp + 7 ± 10		
PHOTO-DRIVE	3022.8	mV	250 mV to 4750 mV		
SLOPE	1.018	-	1.0 ± 0.3		
OFFSET	0.2	-	0 ± 0.3		

Calibrated by : Adul Dangklom
(Mr.Adul Dangklom)

Approved by : Peera Detudom
(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
NON-DISPERSIVE INFRARED CO ANALYZER					
DATE :	31 March 2023	BRAND :	API	MODEL :	300E
NO.	CO-B02	SERIAL NO.	965		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 06 September 2022		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Carbon Monoxide (CO)		Cylinder No.	: D196045	
Certified Date	: 16 April 2022	Expired Date	: 15 April 2024	Cylinder Conc.	: 4,570 PPM
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	48				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	-0.10	-	0	
CO Span	40.00	40.08	0.200	40.00	
API Model 300E CO Analyzer Check list					
Parameter	Observed Value	Units	Nominal Range		
RANGE	50	PPM	0-1000 ppm		
STABILITY	0.10	PPM	< 1 ppm with zero air		
CO MEASURE	4015.7	mV	2500-4800 mV		
CO REFERENCE	3949.2	mV	2500-4800 mV		
MEASURE/REFERENCE RATIO	1.180	-	1.1-1.3 w/zero air		
SAMPLE PRESSURE	28.6	In-Hg-A	~2" < ambient absolute pressure		
SAMPLE FLOW	813	cc/min	800 ± 10%		
SAMPLE TEMPERATURE	48.3	°C	48 ± 4		
BENCH TEMPERATURE	48.1	°C	48 ± 2		
WHEEL TEMPERATURE	68.5	°C	68 ± 2		
BOX TEMPERATURE	30.9	°C	Ambient temp + 7 ± 10		
PHOTO-DRIVE	3026.5	mV	250 mV to 4750 mV		
SLOPE	1.017	-	1.0 ± 0.3		
OFFSET	0.2	-	0 ± 0.3		

Calibrated by : Adul Dangklom
(Mr.Adul Dangklom)

Approved by : Peera Detudom
(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO₂ / NO_x ANALYZER

DATE : 31 March 2023 BRAND : API MODEL : 200A
NO. NOX-B02 SERIAL NO. 2409

Calibrator (Dilution System)

Brand : API Model : 700
Last Cal. Date : 04 August 2022 Serial No. : 911

Reference Standard Gas

Standard Gas : Nitric Oxide (NO) Cylinder No. : D636192
Certified Date : 20 April 2022 Expired Date : 20 April 2024 Cylinder Conc. : 49.1 ppm

CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.6 °C % RH 48

CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.8	-0.050	400.0	1.005
NO _x Span	400	400.1	0.025	400.0	1.008

API Model 200A NO_x Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	507	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	103.1	mV	-20 - 150
AZERO	93.9	mV	-20 - 150
HVPS	670	V	420 - 900 constant
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.4	°C	8 - 48
PMT TEMP	7.2	°C	7 ± 2
MOLY TEMP	314.9	°C	315 ± 5
RCELL PRESS	8.2	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO _x Span Conc	400	PPB	20 - 20,000
NO Slope	1.005	-	1.0 ± 0.3
NO _x Slope	1.008	-	1.0 ± 0.3
NO Offset	1.1	mV	-20 to +150
NO _x Offset	0.7	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

CALIBRATION REPORT

NON-DISPERSIVE INFRARED CO ANALYZER

DATE : 31 March 2023 BRAND : Thermo MODEL : 48C
NO. CO-B11 SERIAL NO. 0401304262

Calibrator (Dilution System)

Brand : API Model : 700
Last Cal. Date : 06 September 2022 Serial No. : 421

Reference Standard Gas

Standard Gas : Carbon Monoxide (CO) Cylinder No. : D196045
Certified Date : 16 April 2022 Expired Date : 15 April 2024 Cylinder Conc. : 4,570 PPM

CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.6 °C % RH 48

CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	-0.10	-	0	
CO Span	40.00	39.95	-0.125	40.00	

INSTRUMENT STATUS

CHAMBER TEMP 47.5 °C FLOW 1.5 LPM
PRESSURE 730.8 mm Hg MOTOR SPEED 100.00%

Calibrated by : Adul Dangklom
(Mr.Adul Dangklom)

Approved by : Peera Detudom
(Mr.Peera Detudom)

Calibrated by : Adul Dangklom
(Mr.Adul Dangklom)

Approved by : Peera Detudom
(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO₂ / NO_x ANALYZER

DATE : 31 March 2023

BRAND : API

MODEL : 200A

NO. NOX-B17

SERIAL NO. 1977

Calibrator (Dilution System)

Brand	: API	Model	: 700
Last Cal. Date	: 04 August 2022	Serial No.	: 911

Reference Standard Gas

Standard Gas	: Nitric Oxide (NO)	Cylinder No.	: D636192
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024
		Cylinder Conc.	: 49.1 ppm

CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.6 °C % RH 48

CALIBRATION SETTING

Span	Initial Reading (Before Adj.), PPB			Final Reading (After Adj.), PPB	
	Expected Concentration	Analyzer Response	% Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.6	-0.100	400.0	1.003
NO _x Span	400	399.9	-0.025	400.0	1.006

API Model 200A NO_x Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	512	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	103.5	mV	-20 - 150
AZERO	94.2	mV	-20 - 150
HVPS	673	V	420 - 900 constant
RCELL TEMP	50.2	°C	50 ± 1
BOX TEMP	29.3	°C	8 - 48
PMT TEMP	7.1	°C	7 ± 2
MOLY TEMP	315.2	°C	315 ± 5
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO _x Span Conc	400	PPB	20 - 20,000
NO Slope	1.003	-	1.0 ± 0.3
NO _x Slope	1.006	-	1.0 ± 0.3
NO Offset	1.0	mV	-20 to +150
NO _x Offset	0.6	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by : Adul Dangklom
(Mr.Adul Dangklom)

Approved by : Peera Detudom
(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO₂ / NO_x ANALYZER

DATE : 31 March 2023

BRAND : API

MODEL : 200E

NO. NOX-B08

SERIAL NO. 4336

Calibrator (Dilution System)

Brand	: API	Model	: 700
Last Cal. Date	: 04 August 2022	Serial No.	: 911

Reference Standard Gas

Standard Gas	: Nitric Oxide (NO)	Cylinder No.	: D636192
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024
		Cylinder Conc.	: 49.1 ppm

CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.6 °C % RH 48

CALIBRATION SETTING

Span	Initial Reading (Before Adj.), PPB			Final Reading (After Adj.), PPB	
	Expected Concentration	Analyzer Response	% Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.008
NO _x Span	400	400.2	0.050	400.0	1.011

API Model 200E NO_x Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	504	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	103.2	mV	-20 - 150
AZERO	94.0	mV	-20 - 150
HVPS	672	V	420 - 900 constant
RCELL TEMP	50.1	°C	50 ± 1
BOX TEMP	29.0	°C	8 - 48
PMT TEMP	7.4	°C	7 ± 2
MOLY TEMP	315.1	°C	315 ± 5
RCELL PRESS	8.5	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.7	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO _x Span Conc	400	PPB	20 - 20,000
NO Slope	1.008	-	1.0 ± 0.3
NO _x Slope	1.011	-	1.0 ± 0.3
NO Offset	1.4	mV	-20 to +150
NO _x Offset	0.9	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by : Adul Dangklom
(Mr.Adul Dangklom)

Approved by : Peera Detudom
(Mr.Peera Detudom)

ภาคผนวก จ-2

เอกสารสอบเทียบเครื่องมือ

บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริง คอนซัลแตนท์ จำกัด

RECALIBRATION
DUE DATE:
July 5, 2023

Certificate of Calibration

Calibration Certification Information

Cal. Date: July 5, 2022 Rootmeter S/N: 438320 Ta: 297 °K
 Operator: Jim Tisch Pa: 750.1 mm Hg
 Calibration Model #: G25A Calibrator S/N: 158M

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.3240	3.2	2.00
2	3	4	1	0.9480	6.4	4.00
3	5	6	1	0.8480	7.9	5.00
4	7	8	1	0.8060	8.7	5.50
5	9	10	1	0.6670	12.7	8.00

Data Tabulation

Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9860	0.7447	1.4073	0.9957	0.7521	0.8899
0.9818	1.0357	1.9902	0.9915	1.0459	1.2585
0.9798	1.1554	2.2251	0.9895	1.1668	1.4071
0.9788	1.2143	2.3337	0.9884	1.2263	1.4757
0.9735	1.4595	2.8146	0.9831	1.4739	1.7798
QSTD	m=	1.96745	QA	m=	1.23199
	b=	-0.05315		b=	-0.03361
	r=	0.99995		r=	0.99995

Calculations

Vstd= ΔVol((Pa-ΔP)/Pstd)(Tstd/Ta)	Va= ΔVol((Pa-ΔP)/Pa)
Qstd= Vstd/ΔTime	Qa= Va/ΔTime
For subsequent flow rate calculations:	
Qstd= $1/m \left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} - b \right)$	Qa= $1/m \left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} - b \right)$

Standard Conditions

Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH: calibrator manometer reading (in H2O)	
ΔP: rootmeter manometer reading (mm Hg)	
Ta: actual absolute temperature (°K)	
Pa: actual barometric pressure (mm Hg)	
b: intercept	
m: slope	

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
 CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
 534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
 TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No. : 23P1402

Page : 1 of 2

Equipment : U Tube Manometer

Manufacturer: Dwyer

Model : 1221-36-W/M

Serial No.: -

ID No.: UAE.EFM.180/2561

Condition As-Received: Used Item

Received Date: 26 April 2023

Calibration Date: 09 May 2023

Reference: 2304-0703WSC

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1010 mbar

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
 Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0137-22	24 Aug 2023

2.This result of calibration was made on requested at the point specified by customer.

3.Scale and conversion factor is 1 kPa = 4.0146293 inH2O

4.This instrument was used clean air as pressure media.

5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suwit Aussarree

Issue Date : 11 May 2023

Approved Signatory : Attapol P.

☐ Phalinee Prabpaipal

☐ Sura Suwannasri

☒ Attapol Panurach

เอกสารไม่ควบคุม
 B 0314242



Cert.No.: 23P1402
Page: 2 of 2

Result of calibration:- Without adjustment

Range : 0 inH₂O to 36 inH₂O

Function:- Pressure Measurement

Scale Interval : 0.1 inH₂O (The Fifth Estimate)

Increasing Pressure

UUC Indication				
Applied Pressure	High-port side	Low-port side	ΔP	Error
(inH ₂ O)	(inH ₂ O)	(inH ₂ O)	(inH ₂ O)	(inH ₂ O)
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-1.00	2.00	0.00
4.00	2.00	-2.00	4.00	0.00
6.00	3.00	-3.00	6.00	0.00
8.00	4.00	-4.00	8.00	0.00
10.00	5.00	-5.00	10.00	0.00
12.00	6.00	-6.00	12.00	0.00
14.00	7.00	-7.02	14.02	0.02
16.00	8.00	-8.02	16.02	0.02
18.00	9.02	-9.04	18.06	0.06
20.00	10.02	-10.04	20.06	0.06
22.00	11.00	-11.04	22.04	0.04
24.00	12.02	-12.06	24.08	0.08
26.00	13.02	-13.06	26.08	0.08
28.00	14.02	-14.04	28.06	0.06
30.00	15.02	-15.02	30.04	0.04
32.00	16.00	-16.02	32.02	0.02
34.00	17.00	-17.00	34.00	0.00
35.80	17.96	-17.98	35.94	0.14

The uncertainty of measurement was ± 0.11 inH₂O

* UUC = Unit Under Calibration

* ΔP = High-port side - Low-port side

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-

Attapol P.

เอกสารไม่ควบคุม
a 1160343



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 22P2722
Page : 1 of 2

Equipment : Aneroid Barometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: UAE.ANV.013/2547

Condition As-Received: Used Item

Received Date: 20 July 2022

Calibration Date: 22 July 2022

Reference: 2207-0584WSC

Ambient Temperature: (23 \pm 2) °C

Relative Humidity: (50 \pm 15) %

Atmospheric Pressure: 1010 mbar

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,

Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505046	MP-0076-22	02 May 2023

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.Scale and conversion factor is 1 kPa = 7.50062 mmHg

5.This result of calibration instrument was in absolute pressure.

6.This instrument was used clean air as pressure media.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suwit Aussarree

Issue Date : 25 July 2022

Approved Signatory : Attapol P.

[] Phalinee Prabpaipal

[] Sura Suwannasri

[x] Attapol Panurach

เอกสารไม่ควบคุม
B 0293205



Cert.No.: 22P2722

Page: 2 of 2

Result of calibration:- Without adjustmentRange: 720 mmHg to 780 mmHgFunction:- Absolute Pressure MeasurementScale Interval: 1 mmHg (The Fifth Estimate)Increasing Pressure

Applied Pressure (mmHg)	718.46	729.33	739.85	750.22	760.90	772.01	785.89
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	760.0	770.0	780.0
Error (mmHg)	1.54	0.67	0.15	-0.22	-0.90	-2.01	-5.89

Decreasing Pressure

Applied Pressure (mmHg)	785.90	771.99	760.85	750.17	739.90	729.57	718.62
UUC* Indication (mmHg)	780.0	770.0	760.0	750.0	740.0	730.0	720.0
Error (mmHg)	-5.90	-1.99	-0.85	-0.17	0.10	0.43	1.38

The uncertainty of measurement was ± 0.24 mmHg

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม
a 1118533TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No. : 22H1583

Page : 1 of 2

Equipment : Dial Thermo-Hygrometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: UAE.ANV.016/2547

Condition As-Received: Used Item

Received Date: 20 July 2022

Calibration Date: 22 July 2022
to 27 July 2022

Reference: 2207-0586WSC

Ambient Temperature: (25 \pm 3) °CRelative Humidity: (50 \pm 20) %This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Chilled Mirror Hygrometer Sensor	Dew Prime II	31863	19714	17 Sep 2022
2) Standard Humidity/Temperature Meter	400	10240757	TH-0125-21	13 Dec 2022

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Standards and Technology (NIST) , The United States of America

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Somchai Dumwor
Issue Date : 03 August 2022Approved Signatory : 

[✓] Chakrit Waewanjua

[] Ponthippa Tameyakul

[] Viporn Tantiyawutti

เอกสารไม่ควบคุม
B 0293719



Cert. No.: 22H1583
Page.: 2 of 2

Result of Calibration:- Without Adjustment

Function: Humidity measurement.

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	42	1.9	1.6
25.0	60.0	63	3.0	1.8
25.0	80.0	78	-2.0	2.0

Result of Calibration:- Without Adjustment

Function: Temperature measurement.

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
20.00	20.0	0.00	0.72
30.01	30.0	-0.01	0.72
35.04	35.0	-0.04	0.72
39.98	40.0	0.02	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-o0o-

[Signature]

เอกสารไม่ควบคุม
a 1119777



United Analyst and Engineering Consultant Co., Ltd.

3 Soi Udornasuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Tel. 0 2763 2828 Fax 0 2763 2800 www.uaec consultant.com E-mail: uae@uaec consultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Mar 28, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1201778108

Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8
Cylinder No. : EB0143262
Expiration Date : Jun 21, 2024

Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data


Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	301.3	1.30	0.43	0.43
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00

Remark : Measuring Range 500.0 ppb

:Acceptable Limit ± 5%

Average Difference (%) 0.28

Multi-Point Gas Test Chart

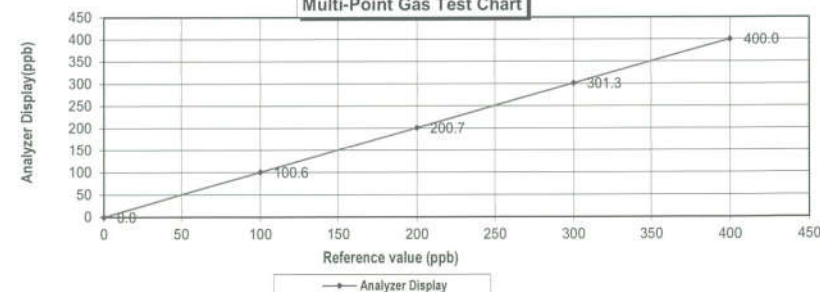

Calculate by

Sirichai Sangsri
28 / 3 / 66

Approve by

Pattana N.
28 / Mar / 2023

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Feb 28, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1201778109

Standard Gas Concentration


Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 21, 2024

Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	101.4	1.40	1.38
Level 3	40.00%	200.0	200.9	0.90	0.45
Level 4	60.00%	300.0	300.7	0.70	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)		0.41
:Acceptable Limit $\pm 5\%$					

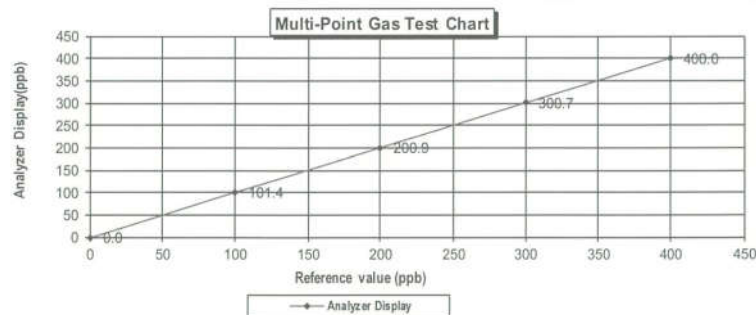

Calculate by
Sirichai Gamchai
28.2.23

Approve by
Dilun h.
28 Feb 2023

CERTIFICATE OF ANALYSIS
Grade of Product: EPA Protocol

Part Number: E04NI99E15A01D3 Reference Number: 122-402135167-1
Cylinder Number: EB0143262 Cylinder Volume: 144.4 CF
Laboratory: 124 - Durham (SAP) - NC Cylinder Pressure: 2015 PSIG
PGVP Number: B22021 Valve Outlet: 660
Gas Code: CO,NO,NOX,SO₂,BALN Certification Date: Jun 21, 2021

Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.68 PPM	G1	+/- 1.0% NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 0.7% NIST Traceable	06/14/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20061120	CC708068	49.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D685025	9.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMIS	401423838102	CC505581	4.348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 18, 2023
NTRM	16011043	CC473277	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14080119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/-0.6%	Nov 15, 2025

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO ₂	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO ₂	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO #5221002807

GROSS WT: 28.40kg

NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

[Signature]

Approved for Release



CERT 3082.01

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Jan 9, 2023

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1200636467

Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 20, 2024


Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.2	0.2	0.2	0.2
Level 2	20.00%	10.0	10.3	0.3	2.9	2.9
Level 3	40.00%	20.0	21.7	1.7	7.8	7.8
Level 4	60.00%	30.0	30.5	0.5	1.6	1.6
Level 5	80.00%	40.0	40.0	0.0	0.0	0.0
Remark : Measuring Range		50.0 ppm	Average Difference (%)			2.52

Multi-Point Gas Test Chart

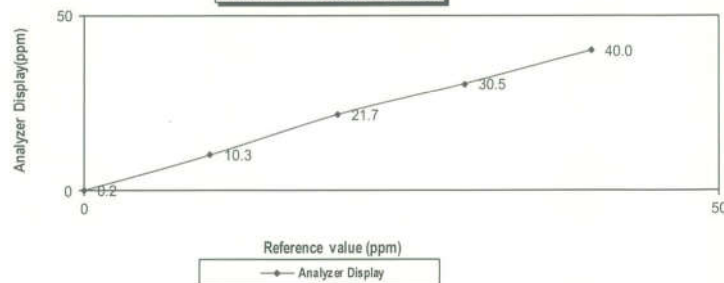

Calculate by

Apinart h.
9/1/66

Approve by

Apinart h.
10/Jan/2023

MULTI-POINT GAS TEST REPORT

Test Date : Jan 9, 2023

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1200906880

Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 20, 2024


Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.5	0.5	0.5	0.5
Level 2	20.00%	10.0	10.3	0.3	2.9	2.9
Level 3	40.00%	20.0	20.8	0.8	3.8	3.8
Level 4	60.00%	30.0	30.7	0.7	2.3	2.3
Level 5	80.00%	40.0	40.0	0.0	0.0	0.0
Remark : Measuring Range		50.0 ppm	Average Difference (%)			1.91

Multi-Point Gas Test Chart

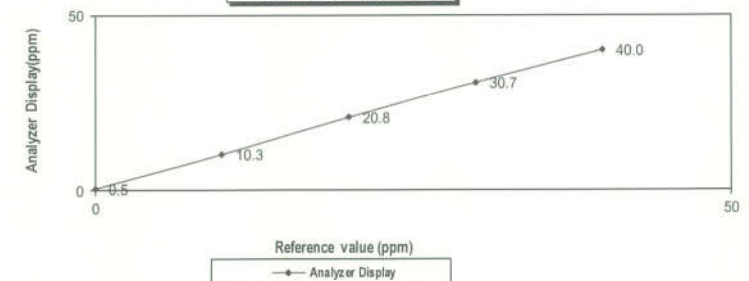

Calculate by

Apinart h.
9/1/66

Approve by

Apinart h.
10/Jan/2023

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04NI99E15A01D3 Reference Number: 122-402135167-1
Cylinder Number: EB0143262 Cylinder Volume: 144.4 CF
Laboratory: 124 - Durham (SAP) - NC Cylinder Pressure: 2015 PSIG
PGVP Number: B22021 Valve Outlet: 660
Gas Code: CO,NO,NOX,SO₂,BALN Certification Date: Jun 21, 2021

Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.68 PPM	G1	+/- 1.0% NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 0.7% NIST Traceable	06/14/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20061120	CC708068	49.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D685025	9.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMIS	401423838102	CC505581	4.348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 18, 2023
NTRM	16011043	CC473277	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14080119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/-0.6%	Nov 15, 2025

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO ₂	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO ₂	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO #5221002807

GROSS WT: 28.40kg

NET WT: 4.73kg



CERT 3082.01

เอกสารไม่ควบคุม

The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

[Signature]

Approved for Release

Certificate of Calibration

WL-21 Wireless Anemometer

Scarlet Tech Ltd. hereby certifies that the WL-21 wireless anemometer listed below was thoroughly calibrated, tested and inspected following the standard calibration procedure (st-wl-21) and is within manufacturer's specification at the time when the calibration is done.

Client: Envir Service Co., Ltd.

Serial No.: 2205DT0106

Calibration Date: 2022/9/14

Calibration Expiry Date: 2023/9/13

The Result of Calibration

Velocity				
Measured Value(m/s)	Actual Value (m/s)	Deviation	Tolerance	Result
1.0	1.0	0.0	0.9-1.1	Pass
1.9	2.0	0.1	1.8-2.2	Pass
5.0	5.0	0.0	4.7-5.3	Pass
7.1	7.0	0.1	6.0-8.0	Pass
10.1	10.0	0.1	9.5-10.5	Pass
19.6	20.0	0.4	19.0-21.0	Pass

Wind Direction				
Measured Value	Actual Value	Deviation	Tolerance	Result
45°	45°	0	42-48	Pass
136°	135°	1	132-138	Pass
225°	225°	0	222-228	Pass
316°	315°	1	312-318	Pass
359°	0°	1	357-3	Pass

Inspection Room Temp	Actual Value	Deviation	Tolerance	Result
22.4°C	22.5°C	0.3	21.5-23.5	Pass

Atmospheric Pressure Inspection	Actual Value	Deviation	Tolerance	Result
1005	1005	0	1001-1019	Pass

Environment conditions :

Air temperature: 22 °C

Relative humidity: 55 %

Static pressure: 102.2 kPa

Performed by: *[Signature]*

Certified by Head of Engineering department



This certificate may not be published or reproduced, except in full, unless obtaining permission in writing form from Scarlet Tech Ltd.
4F-3, No. 347, 2nd Sec., Heping E. Rd., Daan Dist. Taipei City 106, Taiwan

เอกสารไม่ควบคุม

Certificate of Calibration

WL-21 Wireless Anemometer

Scarlet Tech Ltd. hereby certifies that the WL-21 wireless anemometer listed below was thoroughly calibrated, tested and inspected following the standard calibration procedure (st-wl-21) and is within manufacturer's specification at the time when the calibration is done.

Client: Envir Service Co., Ltd.

Serial No.: 2205DT0113

Calibration Date: 2022/9/14

Calibration Expiry Date: 2023/9/13

The Result of Calibration

Velocity				
Measured Value(m/s)	Actual Value (m/s)	Deviation	Tolerance	Result
1.0	1.0	0.0	0.9-1.1	Pass
2.1	2.0	0.1	1.8-2.2	Pass
5.1	5.0	0.1	4.7-5.3	Pass
7.0	7.0	0.0	6.0-8.0	Pass
10.2	10.0	0.2	9.5-10.5	Pass
19.8	20.0	0.2	19.0-21.0	Pass

Wind Direction				
Measured Value	Actual Value	Deviation	Tolerance	Result
45°	45°	0	42-48	Pass
136°	135°	1	132-138	Pass
227°	225°	2	222-228	Pass
316°	315°	1	312-318	Pass
358°	0°	2	357-3	Pass

Inspection Room Temp	Actual Value	Deviation	Tolerance	Result
22.5°C	22.5°C	0.0	21.5-23.5	Pass

Atmospheric Pressure Inspection	Actual Value	Deviation	Tolerance	Result
1005	1005	0	1001-1019	Pass

Environment conditions :

Air temperature: 22 °C

Relative humidity: 55 %

Static pressure: 102.2 kPa

Performed by: 

Certified by Head of Engineering Department



This certificate may not be published or reproduced, except in full, unless obtaining permission in writing form from Scarlet Tech Ltd.

4F-3, No. 347, 2nd Sec., Heping E. Rd., Daan Dist. Taipei City 106, Taiwan

เอกสารไม่ควบคุม