

ภาคผนวกที่ 4

ใบรับรองการสอบเทียบเครื่องมือ

Certificate of Calibration

Certificate No. : 66-200067-1

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Electronic Balance
Manufacturer : METTLER TOLEDO Model : AG285
Serial No. : 1122140126 ID No. : MET-EB01/46
Capacity : 210 g Resolution : 0.00001g/81g, 0.0001g/210g

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (26.4 to 26.8) °C
Relative Humidity : (54.9 to 58.8) %
Air Pressure : 1013.0 mbar

Date of Received : 02 March 2023

Date of Calibration : 02 March 2023

Date of Issue : 13 March 2023

Calibrated by : [REDACTED]

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02222345	10 Nov 2023	National Institute of Metrology (Thailand), (NIMT)

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-200067-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.01	0.00001	0.000020
0.1	0.00000	0.000019
1	-0.00002	0.000031
5	-0.00004	0.000043
10	-0.00008	0.000054
20	-0.00027	0.000071
50	-0.00059	0.00011
100	-0.0009	0.00023
150	-0.0012	0.00038
200	-0.0019	0.00040

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.43$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A B C D E

0.00055 0.00027 -0.00015 -0.00018 0.00000 g



Repeatability

Load test : 200 g

Stdev. : 0.000053 g

- o O o -



Calibration Certificate

Cert. No. : CT-23-05-23470

Page : 1 of 4

Issued date : 08 May 2023

Equipment : COD Reader , Manufacturer : MLAB , Model : DB1602
S/N = 0169 , Customer ID = -

Client : M E T COMPANY LIMITED.

36/659 M.6 Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

Received Date : 03 May 2023

Ref. Job No. : SO6605-00001

Calibrate by : Cert. prepare by : 

Calibrated Date : 03 May 2023

Approved by : 

Calibration Place : Laboratory room

Environment Condition : Temperature 28.6 ± 0.4 (°C) , Humidity 59.5 ± 3.5 (%RH)

Calibration Method : Measure temperature distribution by 9 channel in flat level. , (MTEC WI No. # WICAL-02-005-R01)

Reference Standard Instrument :

No	Instrument	code	Model	Due date
1	Temperature Datalogger	MTEC-CE-0180	MLAB	10/2023
2	Thermo Hygrometer	MTEC-CE-0181	TH-03A	06/2023

Condition of certificate :

(1) This certificate is traceable to International System of units (SI Units). , (2) This certificate was certified only for the instrument we calibrated. , (3) This result of calibration was found accurate as show on date and place of calibration only. , (4) The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k =$ (see result table) , providing a level of confidence of approximately 95%. , (5) This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration Division, Metrology Technical Co.,Ltd.

CER04-R01-DF01

44 Soi ChokChai 4 Soi 40 ,LadPrap ,Bangkok ,Tel.: 0-2538-9205 ,0-2935-7096 ,Fax. : 0-2931-4015 ,Email : contact@mttec.co.th , www.mttec.co.th


Certificate No. : CT-23-05-23470

Calibration Result :

Page : 2 of 4

Condition of UUC :

- 1) Without Adjustment
- 2) Immersion : 1/2 of the depth of the hole

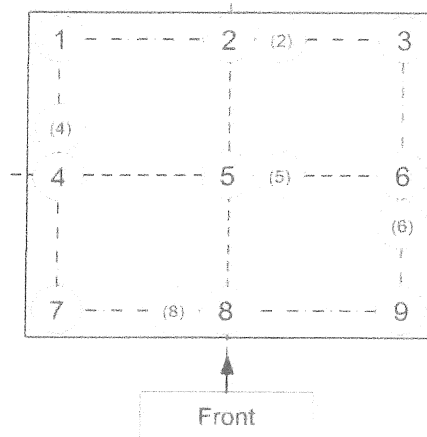

Pic 1 : Position of each sensor No.

- (1) The quoted uncertainty include with "Stability".
- (2) Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors , for at least half an hour after reaching sted state.
- (3) Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
- (4) Overall variation = The difference of the maximum and the minimum measured temperature throughtout observation time.

Section 1 : Report of Temperature distribution

Unit : (°c)

Calibration Point	UUC Setting (*)	UUC Reading (*)	Measured Temperature @ Sensor No.									Uncertainty (±)	k (**)
			#1	#2	#3	#4	#5	#6	#7	#8	#9		
150	150	150	150.51	149.89	150.16	149.93	150.56	150.67	149.80	150.25	149.76	0.627	2

(*) = The average of 30 values in each point , (**) = Coverage factor (k) value

Section 2 : Report of Chamber Performance

Unit : (°c)

Calibration Point	UUC Setting	UUC Reading (*)	Temperature Uniformity	Temperature Stability (± °c)	Temperature Overall Variation
150	150	150	1	0.05	1

(*) = The average of 30 values in each point

Approved Signatory : 

Certificate No. : CT-23-05-23470

Page : 3 of 4


Section 3 : Possible of temperature. Show minimum and maximum of the average values and include with uncertainty of measurement. The average values is average of each position standard sensor throughout observation time.

Unit : (°C)

Calibration Point	UUC Setting (*)	UUC Reading (*)	Possible of Minimum temperature	Possible of Maximum temperature
150	150	150	149.14	151.30

(*) = The average of 30 values in each point

Section 4 : Trend of accuracy

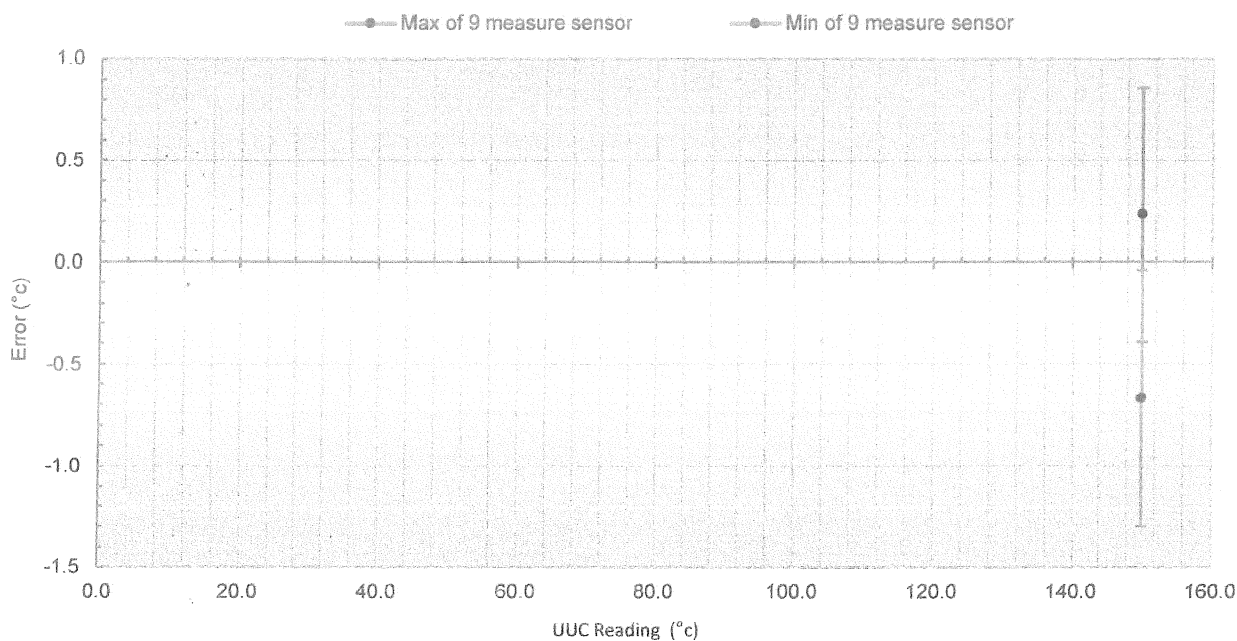


Approved Signatory :

Certificate No. : CT-23-05-23470

Page : 4 of 4

Section 5 : Graph report for Temperature distribution , not include uncertainty of measurement

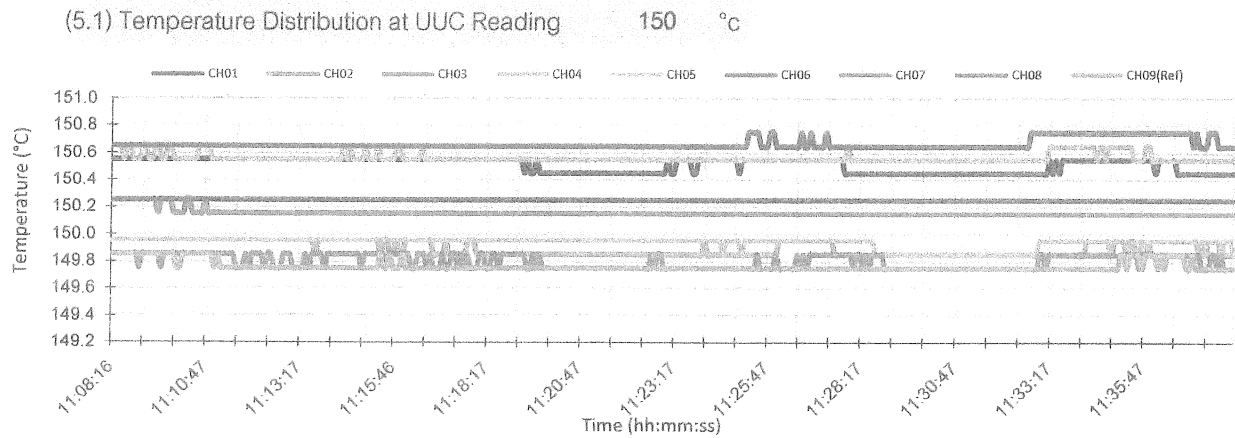

Approved Signatory :



Certificate of Calibration

Certificate No. : 64-400425-5

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Incubator)

Manufacturer : M-LAB

Model : BIC-140

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 240412

ID No. : MET-BI01/55

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (27.0 to 28.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by :

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400032

65-400274-1

25 Nov 2022

National Institute of Metrology Thailand (NIMT)

Approved by :

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. :64-400425-5


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

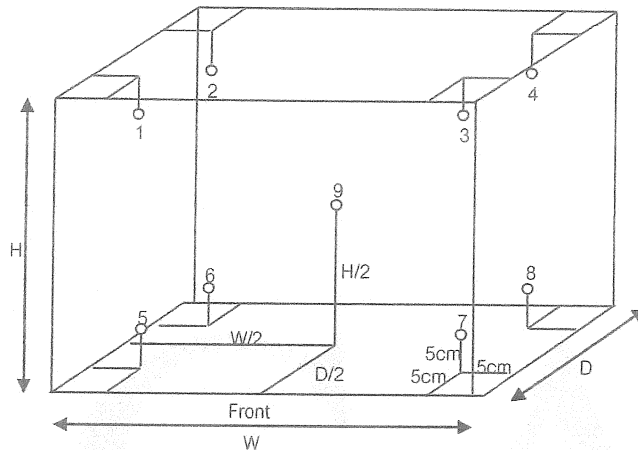

Inside of Chamber

W = 0.37 m

D = 0.33 m

H = 1.14 m

Capacity = 0.14 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	19.8	19.7	19.6	19.6	20.4	20.2	20.3	19.8	19.9	0.54

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	0.6	0.1	1.0

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 65-400424-2

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)

Manufacturer : Binder

Model : ED53

Range : N/A °C

Resolution : 1 °C

Serial No. : 13-07419

ID No. : MET-OV02/57

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (27.0 to 28.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by :

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400030	65-400272-1	24 Nov 2022	National Institute of Metrology Thailand (NIMT)

Approved by :

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-400424-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

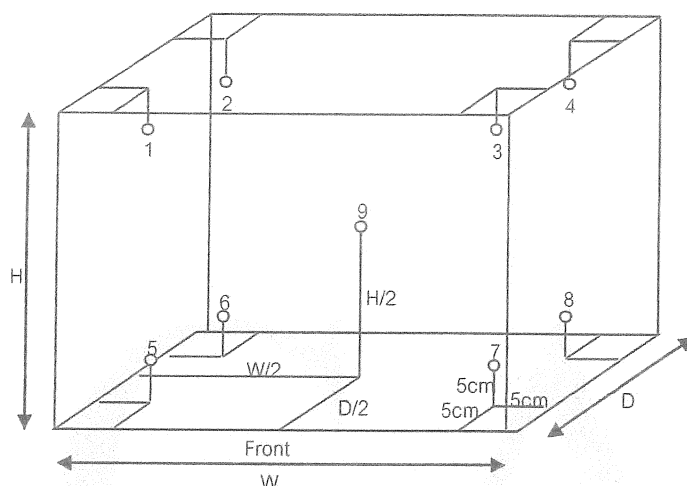

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.40 m

Capacity = 0.05 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104	110	110	105.0	105.0	104.7	105.0	104.4	104.5	104.0	103.7	104.2	0.95
180	184	184	180.8	182.0	179.4	180.8	180.8	180.8	180.3	180.0	180.0	1.2

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104	110	110	1.0	0.2	1.7
180	184	184	2.3	0.3	3.0

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 65-400424-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)

Manufacturer : Memmert

Model : UM 100

Range : N/A °C

Resolution : 0.1 °C

Serial No. : b197.0985

ID No. : MET-OV01/46

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (27.0 to 28.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by :

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400032

65-400274-1

25 Nov 2022

National Institute of Metrology Thailand (NIMT)

Approved by :

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. :65-400424-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

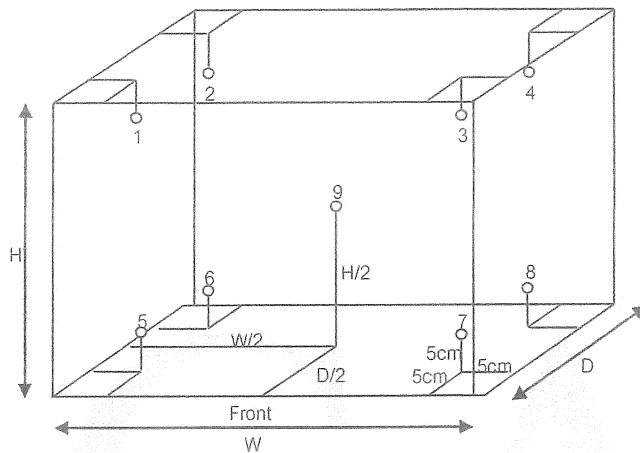

Inside of Chamber

W = 0.32 m

D = 0.18 m

H = 0.24 m

Capacity = 0.01 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
180.0	180.0	180.0	181.2	181.3	180.6	180.4	179.9	181.0	179.5	179.1	180.0	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
180.0	180.0	180.0	1.4	0.3	2.5

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-400012-1

Page : 1 of 2

Submitted by : M E T Company Limited

6/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Digital Thermometer with Thermistor Probe

Temperature Indicator

Manufacturer : Thermo Scientific

Model : pH 150

Range : N/A

Resolution : 0.1 °C

Serial No. : 2657036

ID No. : MET-PH04/60

Thermistor Probe

Model : PHWPTEM01W

Sheath Material : Stainless

Diameter : 3 mm.

Length : 85 mm.

Serial No. : 237

ID No. : MET-PH04/60

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Line Voltage : (220 ± 22) VAC

Date of Received : 05 January 2023

Date of Calibration : 11 January 2023

Date of Issue : 11 January 2023

Calibrated by :

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0016-20	04 Mar 2022	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)
400004	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400012-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
85	10.0035	9.8	0.2	0.11
85	50.0025	50.0	0.0	0.11

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐0๐ -



Certificate of Calibration

Certificate No. : 66-420002-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : pH 150

Range : -2.00 to 16.00 pH

Resolution : 0.01 pH

Serial No. : 2657036

ID No. : MET-PH04/60

Electrode

Model : N/A

Serial No. : 66365

Environment : Ambient Temperature : $(25 \pm 2) ^\circ \text{C}$

Relative Humidity : $(50 \pm 15) \%$

Date of Received : 05 January 2023

Date of Calibration : 11 January 2023

Date of Issue : 11 January 2023

Calibrated by :

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
440001	21E997	17 Mar 2023	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

<u>pH</u>	<u>Cert. No.</u>	<u>Lot No.</u>	<u>Exp. Date</u>	<u>Traceability</u>
4.008	61235182	857394	11 Dec 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61267169	857395	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61260481	857396	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-420002-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.1	0.4	0.060
	0.0000	7	6.99	-0.1	0.1	0.060
	-177.4800	10	10.00	-177.3	-0.2	0.060

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o() o -



Certificate of Calibration

Certificate No. : 65-400424-3

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Refrigerator)

Manufacturer : Sanden Intercool

Model : YPR-068S

Range : N/A °C

Resolution : 1 °C

Serial No. : YPR0659S-141200060R

ID No. : MET-RE03/59

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (29.8 to 31.5) °C

Relative Humidity : (55 to 58) %

Line Voltage : (220.8 to 222.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by :

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400046 & 400023 65-400157-1

02 Oct 2022

National Institute of Metrology Thailand (NIMT)

Approved by



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-400424-3


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

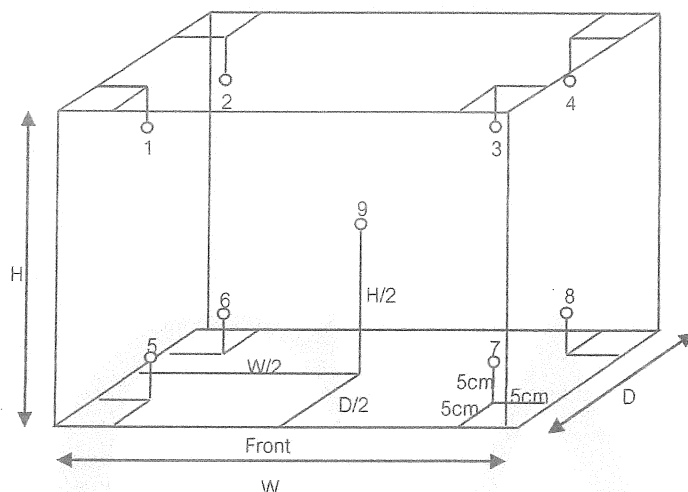

Inside of Chamber

W = 0.58 m

D = 0.60 m

H = 1.45 m

Capacity = 0.50 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
3	2	2	3.7	3.7	4.0	3.7	3.0	3.5	2.8	3.4	2.9	0.84

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
3	2	2	1.2	0.2	1.5

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -





บริษัท เอ็ม ซี ที จำกัด MET CO., LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ. นนทบุรี 11110

36/659 Moo. 6 Tambol. Bangragpattana Amphur. Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_jj@yahoo.com

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	January 7, 2023
Project Site				Start Time	10:00 AM
Sampler Number	TSP No 21	Transfer Standard Type	Orifice	Stop Time	10:05 AM
Motor Serial Number	BL-21	Calibrator Model	TE-5925A		
Recorder Serial Number	-	Calibrator Serial Number	1	Person	


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Positive	Negative	ΔH_2O	$[\Delta H_2O(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)(A-b)$ (m ³ /min)	Sample Flow Rate Indicator (inch)	$IC = [(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(°K = °C+273)	(mmHg)		
5	1.5	1.5	3.0	1.70868	0.87849	1.0	0.99	305.0	757.0		
7	2.4	2.4	4.8	2.16132	1.11505	1.4	1.38	305.0	757.0		
10	3.5	3.8	7.3	2.85625	1.37371	2.0	1.97	305.0	757.0		
13	4.6	4.6	9.2	2.99222	1.54929	2.5	2.47	305.0	757.0		
18	5.8	5.8	11.6	3.35992	1.74145	3.0	2.96	305.0	757.0		

Linear Regression Y ON X : Y = mX + a

1	Slope (m)	1.91345	Linear Equation		r^2	0.989283	Pstd(mmHg)	760.0
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)	1.133	r	0.9946271	T _{mp}	296.0
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)	0	(Pa/Pstd) ² *(Tstd/Ta)		0.973192407	
Result					C=(Pa/Pstd) ² *(Tstd/Ta) ^{0.5}		0.986505146	

COMMENT

Andersen Instruments, Inc.

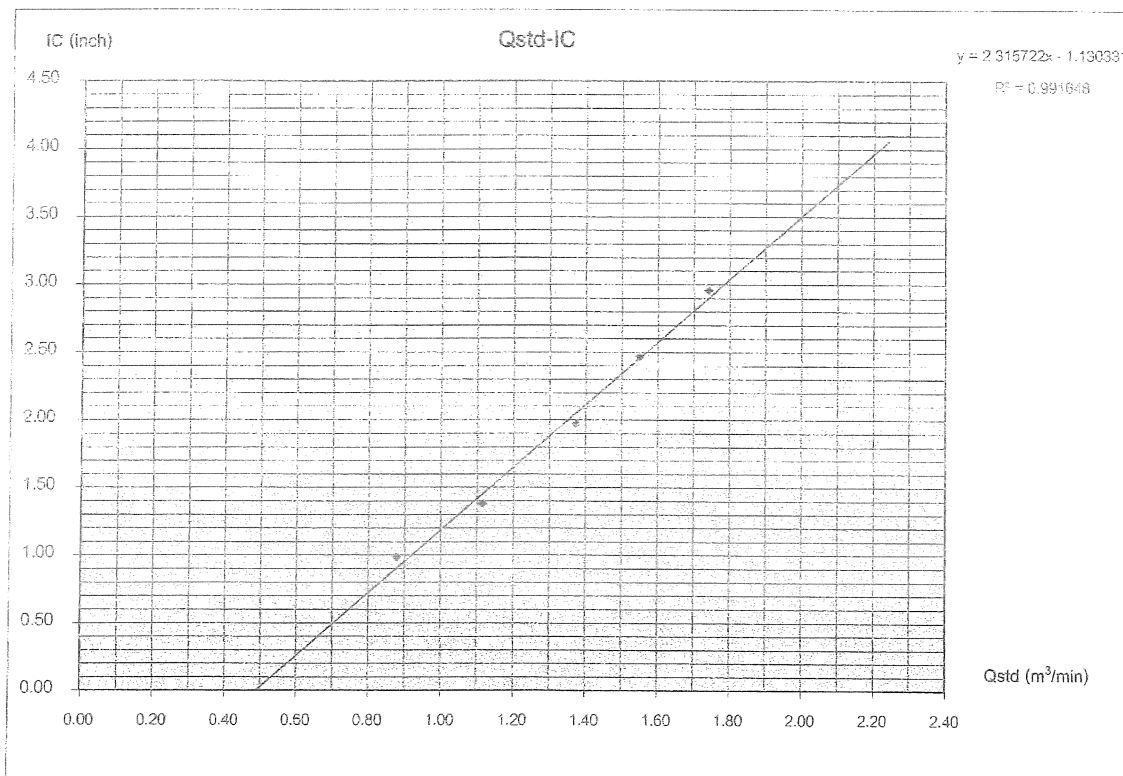

Calibrated By ..

Approved By

(M)



บริษัท เอ็ม ซี ที จำกัด MET CO.,LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ. นนทบุรี 11110

36/659 Moo. 6 Tambol. Bangragpattana Amphur. Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_jj@yahoo.com

PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	January 7, 2023
Project Site				Start Time	10:00 AM
Sampler Number	PM-10 No.4	Transfer Standard Type	Orifice	Stop Time	10:05 AM
Motor Serial Number	HVL-04	Calibrator Model	TE-5025A		
Recorder Serial Number		Calibrator Serial Number		Person	


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Positive	Negative	ΔH_2O	$[\Delta H_2O(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indicator (inch)	$IC = [(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(°K = °C+273)	(mmHg)		
5	1.0	1.0	2.0	1.39513	0.71462	0.7	0.69	305.0	757.0		
7	1.8	1.8	3.6	1.87176	0.96372	1.1	1.09	305.0	757.0		
10	2.6	2.6	5.2	2.24958	1.16117	1.6	1.56	305.0	757.0		
13	3.4	3.4	6.8	2.57249	1.32993	2.1	2.07	305.0	757.0		
16	4.1	4.1	8.2	2.82492	1.46186	2.6	2.56	305.0	757.0		

Linear Regression Y ON X: Y = mX + b

1	Slope (m)	1.91345	Linear Equation		Average	305.0	757.0		
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)	1.133	r ²	0.975431	Pstd(mmHg)	760.0	
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)	0	r	0.9876391	T _{std}	298.0	
Result							(Pa/Pstd)*(Tstd/Ta)	0.973192407	
							C=(Pa/Pstd)*(Tstd/Ta)^0.5	0.986505148	

COMMENT

Andersen instruments, Inc.

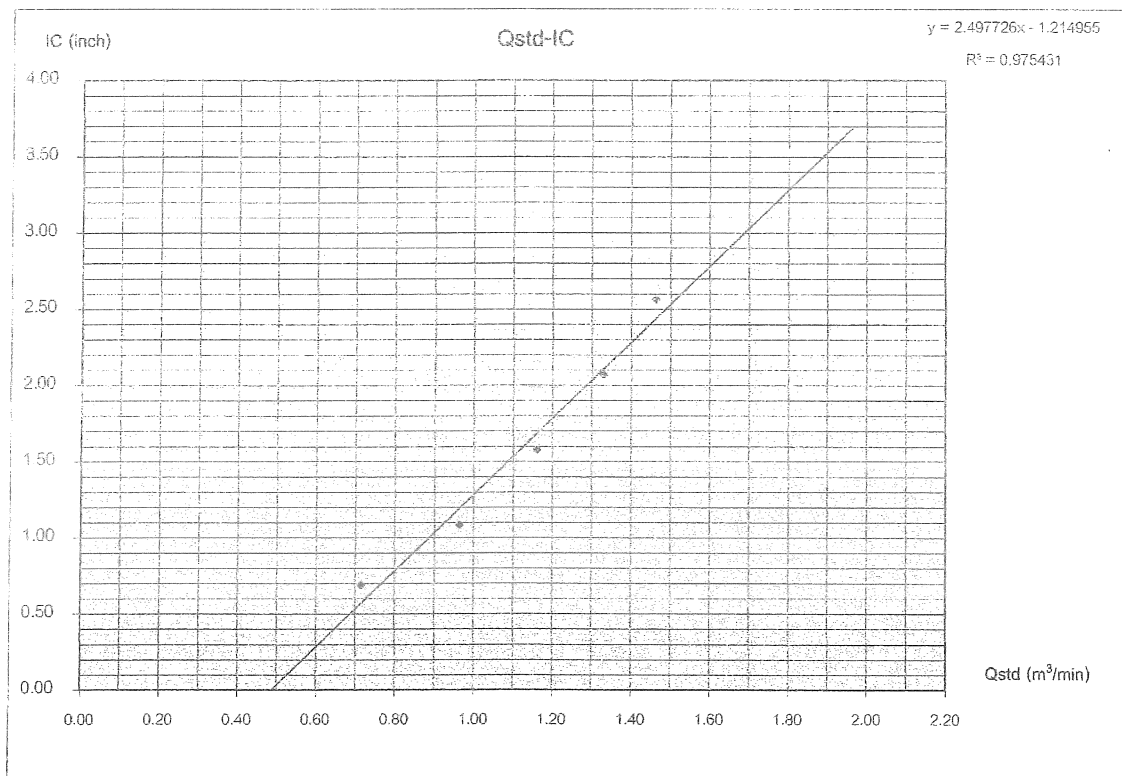

Calibrated By

Approved By



บริษัท เอ็ม ซี ที จำกัด MET CO.,LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ. นนทบุรี 11110

36/659 Moo. 6 Tambol. Bangragpattana Amphur. Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_jj@yahoo.com

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	January 7, 2023
Project Site				Start Time	10:30 AM
Sampler Number	TSP No. 13	Transfer Standard Type	Orifice	Stop Time	10:35 AM
Motor Serial Number	BL-10	Calibrator Model	TE-5025A		
Recorder Serial Number		Calibrator Serial Number	1		


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric	Start	Stop
	Pressure Drop Across Orifice (inH ₂ O)	Positive	Negative	$[\Delta H_2O(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indicator (inch)	$IC = [(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(°K = °C+273)	Pressure (mmHg)	Meter	Meter
5	1.3	1.3	2.6	1.59279	0.81793	1.0	0.99	305.0	757.0		
7	2.1	2.1	4.2	2.02440	1.04349	1.5	1.48	305.0	758.0		
10	3.4	3.4	6.8	2.57569	1.33171	2.1	2.07	305.0	759.0		
13	4.2	4.2	8.4	2.86294	1.48173	2.6	2.57	305.0	760.0		
16	5.1	5.1	10.2	3.15460	1.63426	3.1	3.06	305.0	761.0		

Linear Regression Y ON X : Y = mX + b

1	Slope (m)	1.91345	Linear Equation		Average	305.0	759.0		
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)	1.133	r ²	0.988425	Pstd(mmHg)	760.0	
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)	0	r	0.9941957	T _{std} (°C)	298.0	
Result					C	(Pa/Pstd)*(Tstd/Ta)		0.975763589	
						C=(Pa/Pstd)*(Tstd/Ta)^0.5		0.987807466	

COMMENT

Andersen Instruments, Inc.

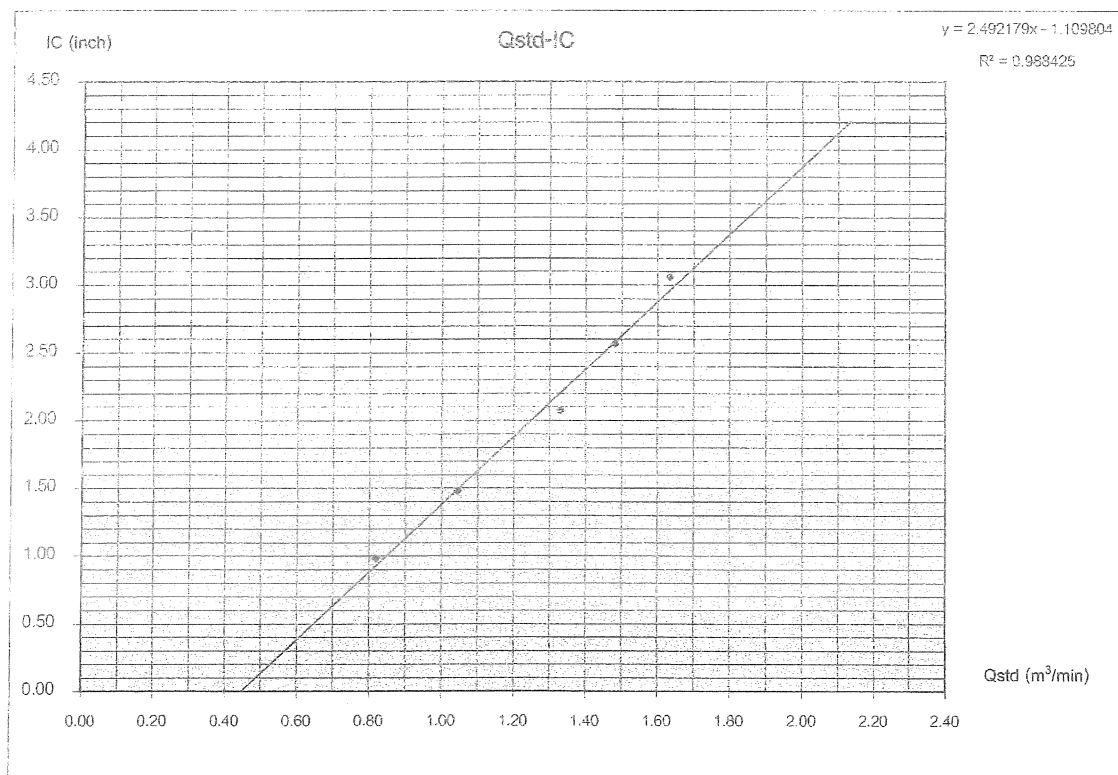

Calibrated By

Approved By

(Mr



บริษัท เอ็ม ซี ที จำกัด MET CO.,LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ. นนทบุรี 11110

36/659 Moo. 6 Tambol. Bangragpattana Amphur. Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_ji@yahoo.com

PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	January 7, 2023
Project Site				Start Time	10:40 AM
Sampler Number	PM-10 No.10	Transfer Standard Type	Orifice	Stop Time	10:45 AM
Motor Serial Number	HVL-10	Calibrator Model	TE-5025A		
Recorder Serial Number	-	Calibrator Serial Number	-	Person	


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric	Start	Stop
	Pressure Drop Across Orifice (inH ₂ O)	Positive	Negative	$[\Delta H_{H_2O}(Pa/P_{atm})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indicator (inch)	$IC = [(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(°K = °C+273)	Pressure (mmHg)	Meter	Meter
5		1.5	1.5	3.0	1.70868	0.87849	1.2	305.0	757.0		
7		2.6	2.6	5.2	2.24958	1.16117	1.8	305.0	757.0		
10		3.7	3.7	7.4	2.68358	1.38799	2.6	305.0	757.0		
13		4.6	4.6	9.2	2.99222	1.54929	3.3	305.0	757.0		
16		5.7	5.8	11.5	3.34640	1.73997	4.0	305.0	757.0		

Linear Regression Y ON X : Y = mX + b

1	Slope (m)	1.91345	Linear Equation		r^2	0.995355	Pstd(mmhg)	760.0
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)	1.133	r	0.951502	T _{HTP}	298.0
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)	0		(Pa/Pstd)*(Tstd/Ta)	0.973192407	
Result						C=(Pa/Pstd)*(Tstd/Ta) ^{0.5}	0.986505148	

COMMENT

Andersen Instruments, Inc.

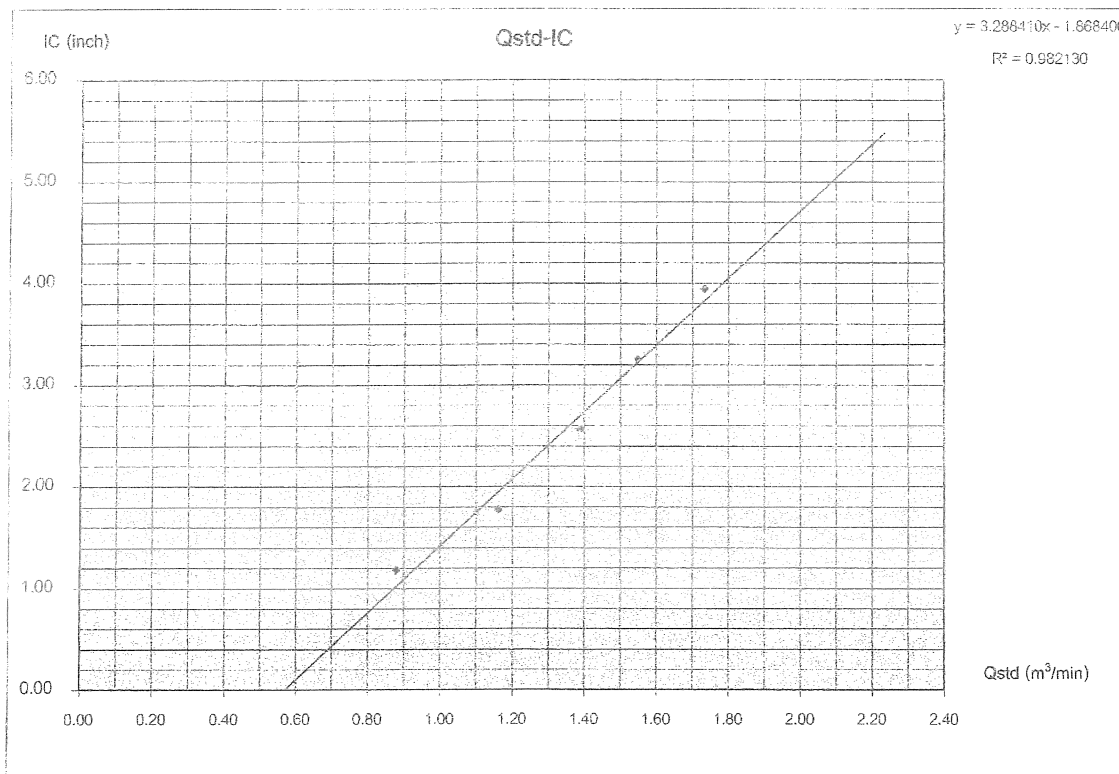

Calibrated By

Approved By



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
 บริษัท เอ็นไวร์ เซอร์วิส จำกัด
 ENVIR SERVICE CO., LTD. 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 5 January 2023

Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 42C	Manufacturer Thermo Environmental S/N: 601114763
--	---

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	393.5	400.0	-1.6
NOx	0.1	0.0	0.1	396.2	400.0	-1.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

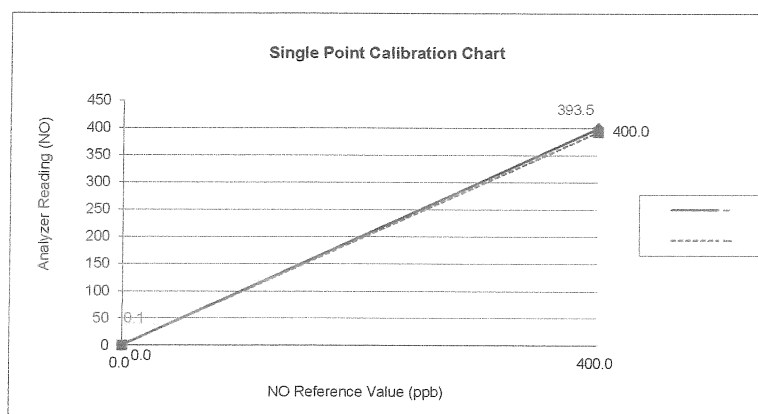



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
 บริษัท เอ็นไวร์ เซอร์วิส จำกัด
 ENVIR SERVICE CO., LTD. 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 5 January 2023

Instruments Information

Analyzer Type: NO/NO ₂ /NO _x Analyzer Model: 42C	Manufacturer Thermo Environmental S/N: 601114773
---	---

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 55.47 PPM SO ₂ Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C


Humidity: 51 %RH


Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	393.3	400.0	-1.7
NO _x	0.1	0.0	0.1	396.4	400.0	-0.9

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

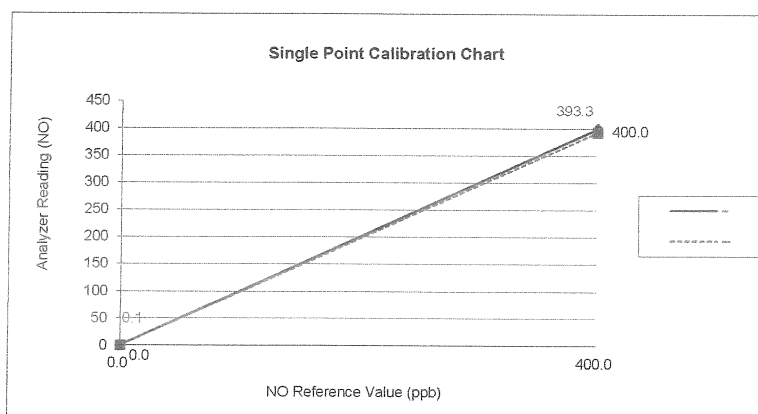



National Institute of Metrology (Thailand)

Certificate of Calibration

Certificate No. : AA-2018-22
Issued by : Acoustics Laboratory
Acoustics and Vibration Group



Page 1 of 5 pages

MEASUREMENT ITEM : Sound Calibrator
MANUFACTURER : RION
MODEL/TYPE : NC-75
SERIAL NUMBER : 34480442
CUSTOMER : MET Co., Ltd.
36/659 Moo 6, T. Bangrakphatthana,
A. Bangbuathong, Nonthaburi 11110
MEASUREMENT DATE : 28 September 2022

The reported measurement result relates only to the measurand and applies only at the time of measurement.

*The calibration results only marked with an asterisk * in this certificate are not included in the scope of accreditation.*

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%. This calibration certificate may not be reproduced other than in full except with the permission of the Director of National Institute of Metrology (Thailand).

Reference	Date	Authorized Signatory	Person in charge
AUVC844-01/22	29 September 2022		

This certificate is consistent with the capabilities that are included in Appendix C of the MRA drawn up by the CIPM. Under the MRA, all participating institutes recognize the validity of each other's calibration and measurement certificates for the quantities, ranges and measurement uncertainties specified in Appendix C (for details see <http://www.bipm.org>).

National Institute of Metrology (Thailand)

Ministry of Higher Education, Science, Research and Innovation

3/4-5 Moo 3, Klong 5, Klong Luang, Pathumthani 12120, Thailand. Tel: (66) 2577 5100, Fax: (66) 2577 3659
75/7 Rama VI Road, Rachathewi, Bangkok 10400, Thailand. Tel: (66) 2354 3700, Fax: (66) 2354 3692




UNCERTAINTY OF MEASUREMENT

The stated uncertainty is the expanded uncertainty obtained by multiplying the standard uncertainty by the coverage factor $k=2$. It has been determined in accordance with EA publication EA-4/02 M:2013 "Evaluation of the Uncertainty of Measurement in Calibration" and JCGM 100:2008 "Evaluation of measurement data --Guide to the Expression of Uncertainty in Measurement (GUM 1995 with minor corrections)". The value of the measured lies within the assigned range of value with a probability of 95 %.

Parameter	Uncertainty at SPL94 dB	Maximum-permitted uncertainty of measurement for a coverage probability of 95%
1.Sound Pressure level	0.08	0.15
2. Frequency	0.1	0.2
3. THD+N	0.1	0.5

TRACEABILITY

This certificate provides traceability of measurement to recognized national standards, and to the realization of the International System of Units (SI).



ENVIRONMENTAL CONDITIONS

Ambient condition in the laboratory are as follows :

Temperature	:	(23.0 ± 1.0)	°C
Pressure	:	(101.325 ± 1.500)	kPa
Relative Humidity	:	(50.0 ± 15.0)	%

Reference Condition : 101.325 kPa , 23.0 °C and 50.0 %RH.

Calibration Condition

Preconditionings : 16 hours at ambient conditions.

Measurement Conditions : The average values during measurement are
 (100.313 ± 0.014) kPa, (22.0 ± 0.3) °C and (57.0 ± 2.1) %RH

MEASUREMENT METHOD

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone. The insert voltage technique was employed and the measurement procedure was based on IEC 60942-2017.


Reference Microphone

4180 serial no.1395446

TABULATION OF RESULTS

The following tables give the calibration results and associated measurement uncertainties at 95% of confidence level. The calibration results of sound pressure level which quoted in dB with reference to 20 µPa are corrected to the values under the reference environmental conditions.

The calibration results exclude the calibrator pressure correction but include the microphone volume correction, which was obtained from the manufacturer instruction manual of the sound calibrator, at the level of 94 dB.



MEASUREMENT RESULTS

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)*	Deviated value ^[1] (dB)	Acceptance Limit (dB)
Microphone 4180 Serial No.1395446			
94	94.15	0.15	0.25

Note ^[1] : The deviated value is the absolute value of the difference between the measured value and the corresponding specified sound pressure level.

2. Frequency*

Specified Frequency (Hz)	Measured value (Hz)	Deviated value ^[2] (%)	Acceptance Limit (%)
At the sound pressure level of 94 dB			
1000	1000.0	0.0	0.7

Note ^[2] : The deviated value is the absolute value of the difference in percent between the measured value and the corresponding specified frequency.




3. Total distortion + Noise*

Microphone 4180 Serial No.1395446

Measured value ^[3] (%)	Maximum total distortion + Noise (%)
At the sound pressure level of 94 dB	
0.2	2.5

Note ^[3]: The measured value is the total distortion, measured over the frequency range from 20 Hz to 20 kHz. The measured value must not exceed the maximum total distortion + noise appeared in the table.

End of Certificate of Calibration



Certificate of Calibration

Certificate Number : SPR23010010-3

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 79210

ID. Number : SLM-39

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 04 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jan 2023



Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :





Calibration Report

Certificate Number : SPR23010010-3

Page : 2 of 3

Reference Standards



Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research





Certificate of Calibration

Certificate Number : SPR23010010-4

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 76239

ID. Number : SLM-35

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 04 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :





Calibration Report

Certificate Number : SPR23010010-4

Page : 2 of 3



Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010010-4

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15



Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010010-5

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 76238

ID. Number : SLM-47

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 04 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jan 2023


Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :





Calibration Report

Certificate Number : SPR23010010-5

Page : 2 of 3


Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010010-5

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.1	114.1	0.1	0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010010-1

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : Rion

Model : NL-21

Serial Number : 00722042

ID. Number : SLM-46

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 04 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :





Calibration Report

Certificate Number : SPR23010010-1

Page : 2 of 3



Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010010-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15


Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010010-2

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : Rion

Model : NL-21

Serial Number : 00722043

ID. Number : SLM-45

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 04 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Authorized Signatory



Certificate Number : SPR23010010-2

Page : 2 of 3

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010010-2

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15


Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010249-5

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222064

ID. Number : SLM-31

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 19 Jan 2023

Calibration Date : 23 Jan 2023

Recommend Due Date : 23 Jan 2024

Date of Issue : 24 Jan 2023


Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :





Calibration Report

Certificate Number : SPR23010249-5


Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Page : 3 of 3

Function : @1kHz

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.1	114.1	0.1	0.1	0.15



Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.3	94.2	0.3	0.2	0.15
114	114.1	114.1	0.1	0.1	0.15

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010249-6

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222065

ID. Number : SLM-32

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 19 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 23 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 23 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 24 Jan 2023


Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :





Calibration Report

Certificate Number : SPR23010249-6

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010249-6

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.1	114.1	0.1	0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty


The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : L202301038-001

Date Issued : 16-Jan-23

Customer : MET CO.,LTD.
36/659 Moo 6 T. Bangrakpattana A.Bangbuatong Nonthaburi 11110

Equipment : Heat Stress Meter

Manufacturer : Metrosonic

Model : hs-32

Serial No. : MCE010018

ID No./Tag No. : HT-02

Date Received : 13-Jan-23

Date Calibrated : 13-Jan-23

Calibrated by : Mr. Apiwat Peanrungrot

Calibration Method or Calibration Procedure Used

In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:



Page 1 of 2

Environment : Ambient Temperature : $(25 \pm 2)^\circ\text{C}$
Relative Humidity : $(50 \pm 15)\%\text{RH}$

STD	UUC Reading (°C)			UUC Error	Measurement
Reading (°C)		Before Adjusted	After Adjusted	(°C)	Uncertainty (\pm °C)
24.00	WET	23.9	-	-0.10	0.35
28.01	DRY	27.7	-	-0.31	0.40
30.00	GLOBE	30.1	-	0.10	0.35
27.02	WET	26.9	-	-0.12	0.35
32.00	DRY	31.9	-	-0.10	0.40
35.00	GLOBE	35.1	-	0.10	0.35
30.00	WET	29.8	-	-0.20	0.35
36.01	DRY	35.6	-	-0.41	0.40
40.01	GLOBE	40.0	-	-0.01	0.35

UUC = Unit Under Calibration

Description of UUC :	Range	0 to 100	°C
	Resolution	0.1	°C

Measurement Standards Used & Traceability :


MIT Certificate No. L202210258-006 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 10-Nov-23

End of Certificate



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : L202301038-002

Date Issued : 16-Jan-23

Customer : MET CO.,LTD.
36/659 Moo 6 T. Bangrakpattana A.Bangbuatong Nonthaburi 11110

Equipment : Heat Stress Meter

Manufacturer : Quest

Model : Questtemp 34

Serial No. : TFB060016

ID No./Tag No. : HT-11

Date Received : 13-Jan-23

Date Calibrated : 13-Jan-23

Calibrated by : Mr. Apiwat Peanrungrot

Calibration Method or Calibration Procedure Used

In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:



Environment : Ambient Temperature : $(25 \pm 2)^\circ\text{C}$
Relative Humidity : $(50 \pm 15)\%\text{RH}$

STD	UUC Reading (°C)			UUC Error	Measurement
Reading (°C)		Before Adjusted	After Adjusted	(°C)	Uncertainty (±°C)
24.00	WET	24.1	-	0.10	0.35
28.01	DRY	28.2	-	0.19	0.35
30.00	GLOBE	30.3	-	0.30	0.35
27.02	WET	27.2	-	0.18	0.35
32.00	DRY	32.3	-	0.30	0.35
35.00	GLOBE	35.3	-	0.30	0.35
30.00	WET	30.2	-	0.20	0.35
36.01	DRY	36.4	-	0.39	0.35
40.01	GLOBE	40.4	-	0.39	0.35

UUC = Unit Under Calibration

Description of UUC :	Range	0 to 100	°C
	Resolution	0.1	°C

MIT Certificate No. L202210258-006 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 10-Nov-23

End of Certificate