

ภาคผนวกที่ 6-1
เอกสารสอบเทียบคุณภาพอากาศในบรรยากาศ



RECALIBRATION DUE DATE:
August 2, 2023

Certificate of Calibration

Calibration Certification Information			
Cal. Date: August 3, 2022	Rootsmer S/N: 438320	Ta: 296	*K
Operator: Jim Tisch		Pa: 748.3	mm Hg
Calibration Model #: TE-5025A	Calibrator S/N: 710725		

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.3740	3.2	2.00
2	3	4	1	0.9780	6.4	4.00
3	5	6	1	0.8730	7.9	5.00
4	7	8	1	0.8300	8.8	5.50
5	9	10	1	0.6870	12.8	8.00

Data Tabulation					
Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9870	0.7183	1.4080	0.9957	0.7247	0.8895
0.9828	1.0049	1.9912	0.9914	1.0137	1.2579
0.9808	1.1234	2.2262	0.9894	1.1334	1.4064
0.9796	1.1802	2.3349	0.9882	1.1907	1.4750
0.9743	1.4182	2.8160	0.9829	1.4307	1.7789
QSTD	m=	2.00936	QA	m=	1.25823
	b=	-0.03294		b=	-0.02081
	r=	0.99998		r=	0.99998

Calculations	
Vstd= $\Delta Vol \left(\frac{Pa - \Delta P}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)$	Va= $\Delta Vol \left(\frac{Pa - \Delta P}{Pa} \right)$
Qstd= $Vstd / \Delta Time$	Qa= $Va / \Delta Time$
For subsequent flow rate calculations:	
Qstd= $1/m \left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} - b \right)$	Qa= $1/m \left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} - b \right)$

Standard Conditions	
Tstd:	298.15 *K
Pstd:	760 mm Hg
Key	
ΔH:	calibrator manometer reading (in H2O)
ΔP:	rootsmer manometer reading (mm Hg)
Ta:	actual absolute temperature (*K)
Pa:	actual barometric pressure (mm Hg)
b:	intercept
m:	slope

RECALIBRATION
US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30

Tisch Environmental, Inc.
145 South Miami Avenue
Village of Cleves, OH 45002

www.tisch-env.com
TOLL FREE: (877)263-7610
FAX: (513)467-9009



ENVIR SERVICE CO., LTD.
42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

Analyzer Performance Test

Calibrated Date: 21 March 2023

Instruments Information

Analyzer Type : SO2 Analyzer	Manufacturer : Thermo Environmental
Model : 43C	Serial Number : 43C-58207-316

Calibrator Unit

Dilutor Model :	Dasibi Model 5008
Serial Number :	705
ZERO AIR Generator :	API MODEL 701
Serial Number :	1924


Standard Gas Concentration

Nitric Oxide (NO)	55.47	PPM
Sulphur Dioxide (SO2)	55.11	PPM
Carbon Monoxide (CO)	4,535	PPM
Cylinder number	EB0129027	
Expire Date:	29 Oct. 2027	

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.2	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

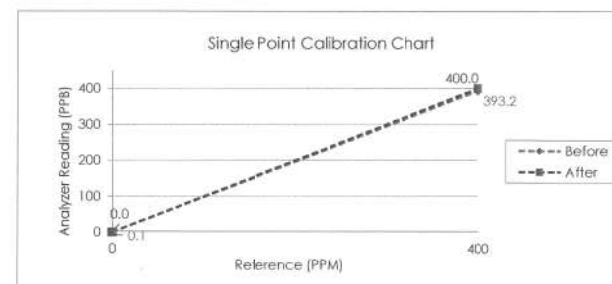

Calibrate By :

Approve by :

ENVIR SERVICE CO., LTD.

42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

Analyzer Performance Test

Calibrated Date: 21 March 2023

Instruments Information

Analyzer Type : SO2 Analyzer

Model : 43C

Manufacturer :

Thermo Environmental

Serial Number :

43C-58286-317

Calibrator Unit

Dilutor Model :

Dasibi Model 5008

Serial Number :

705

ZERO AIR Generator :

API MODEL 701

Serial Number :

1924

Standard Gas Concentration

Nitric Oxide (NO)

55.47 PPM

Sulphur Dioxide (SO2)

55.11 PPM

Carbon Monoxide (CO)

4,535 PPM

Cylinder number

EB0129027


Expire Date:

29 Oct. 2027

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.4	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

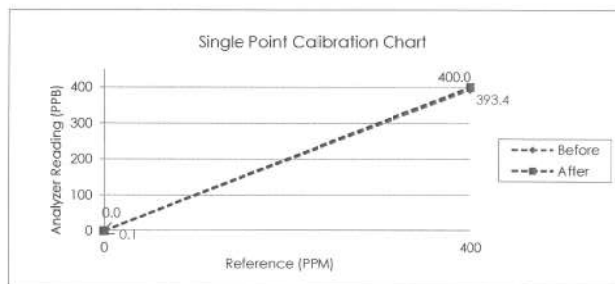

Calibrate By :

Approve by :

ENVIR SERVICE CO., LTD.

42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

Analyzer Performance Test

Calibrated Date: 21 March 2023

Instruments Information

Analyzer Type : NO-NO2-NOx Analyzer

Model : 42C

Manufacturer :

Thermo Environmental

Serial Number :

42C-70626-366

Calibrator Unit

Dilutor Model :

Dasibi Model 5008

Serial Number :

705

ZERO AIR Generator :

API MODEL 701

Serial Number :

1924

Standard Gas Concentration

Nitric Oxide (NO)

55.47 PPM

Sulphur Dioxide (SO2)

55.11 PPM

Carbon Monoxide (CO)

4,535 PPM

Cylinder number

EB0129027


Expire Date:

29 Oct. 2027

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.1	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

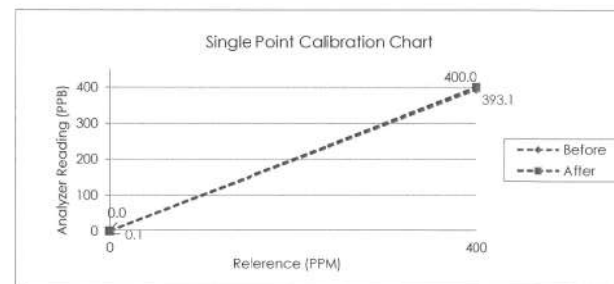

Calibrate By :

Approve by :

ENVIR SERVICE CO., LTD.

42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

Analyzer Performance Test

Calibrated Date: 21 March 2023

Instruments Information

Analyzer Type : NO-NO2-NOx Analyzer

Manufacturer : Thermo Environmental

Model : 42C

Serial Number : 42C-70412-365

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Standard Gas Concentration

Serial Number : 705

Nitric Oxide (NO) 55.47 PPM

ZERO AIR Generator : API MODEL 701

Sulphur Dioxide (SO2) 55.11 PPM

Serial Number : 1924

Carbon Monoxide (CO) 4,535 PPM


Cylinder number EB0129027

Expire Date: 29 Oct. 2027

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.3	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

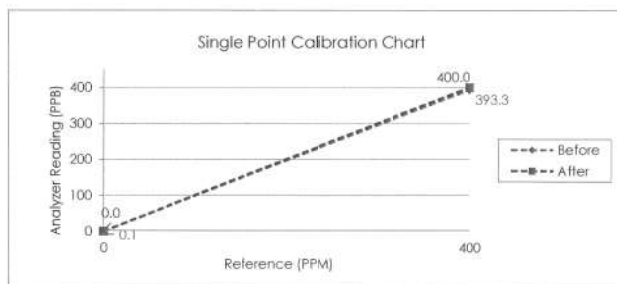

Calibrate By :

Approve by :

ภาคผนวกที่ 6-2
เอกสารสอบเทียบ
ปริมาณสารเจือปนในอากาศที่ระบายออกจากปล่อง



Envi Equipment Service Co., Ltd.

110/254 Moo 3, Tambon Bang Rak Phatthana, Amphur Bang Bua Thong, Nonthaburi 11110

Tel. 098 362 9152, 089 478 7885

E-mail: sales@envi-ees.com

Certificate No. : E23-01009

Page : 1 of 6

CERTIFICATE OF CALIBRATION

Customer : Pacific Laboratory Co., Ltd.

Address : 14/5358 Moo 14, Tambon Bang Bua Thong, Amphoe Bang Bua Thong, Nonthaburi 11110

Description of Equipment : Console meter

Manufacturer : Apex Instrument

Model Number : XC-572-OV

Serial Number : 1306033

ID./Control No. : -

Environment Conditions : Temperature (25 ± 2) °C
Humidity (50 ± 15) % RH

Cal. Date : 06/01/2023

Issue Date : 06/01/2023

Calibration Method or Calibration Procedure Used

US EPA Method (United State Environmental Protection Agency)

This certificate is traceable to national standard, which realize the units of measurement according to the International System of Units (IS).

Result of Calibration

This certificate may not be reproduced other than in full except with prior Written approval of the Technical Manager, Envi Equipment Service Company Limited.

These reported uncertainties of measurement are expanded by a coverage factor of k=2, providing a 95% confidence level

Calibrated by :

Approved by :

Technical Manager



Certificate No. : E23-01009

Page : 2 of 6

METHOD 5 CONSOLE CALIBRATION USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425 5-POINT METRIC UNIT

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-OV	Date	Time	06/01/2023	10:00 AM	Std Temp	293	K
Console Serial Number	1306033	Calibration Reference No.	SER23-01003			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	759.74		mmHg	K ₁	0.386	
DGM Serial Number	00009149	Calibration Meter Gamma	0.999			Console Leak Check	PASS	

Calibration Data									
Run Time	Metering Console					Calibration Meter			
Elapsed	DGM Orifice DH	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final
(Q)	(P _m)	(V _{mi})	(V _{mf})	(t _{mi})	(t _{mf})	(V _{wi})	(V _{wf})	(t _{wi})	(t _{wf})
min	mm H ₂ O	m ³	m ³	°C	°C	m ³	m ³	°C	°C
12.42	13.0	0.1450	0.2850	24	24	118.50438	118.64402	25	25
12.40	13.0	0.2850	0.4250	25	25	118.64402	118.78246	25	25
8.75	26.0	0.4360	0.5760	25	25	118.78792	118.92572	25	25
8.75	26.0	0.5760	0.7160	26	26	118.92572	119.06308	25	25
14.02	40.0	0.7220	1.0020	27	27	119.06932	119.34854	25	25
14.02	40.0	1.0020	1.2820	28	28	119.34854	119.62648	25	25
10.53	70.0	1.2930	1.5730	28	28	119.63648	119.91388	25	25
10.50	70.0	1.5730	1.8530	28	28	119.91388	120.19082	25	25
9.17	90.0	1.8640	2.1440	29	29	120.20082	120.48048	25	25
9.15	90.0	2.1440	2.4240	29	29	120.48048	120.75954	25	25


METHOD 5 CONSOLE CALIBRATION
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425
5-POINT METRIC UNIT

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-OV	Date	Time	06/01/2023	10:10 AM	Std Temp	293	K
Console Serial Number	1306033	Calibration Reference No.	SER23-01003			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	759.74			K ₁	0.386	
DGM Serial Number	00009149	Calibration Meter Gamma	0.999			Console Leak Check	PASS	

Calibration Data									
Results									
Standardized Data				Dry Gas Meter					
				Calibration Factor		Flowrate			
Dry Gas Meter	Calibration Meter			Value	Variation	Std & Corr	.0212 m ³ _{std} /min	Variation	
(V _{m(Std)})	(Q _{m(Std)})	(V _{W(Std)})	(Q _{W(Std)})	(Y)	(ΔY)	(Q _{m(Std&Corr)})	(ΔH _g)	(ΔH _g)	
m ³	m ³ /min	m ³	m ³ /min			m ³ /min	mm H ₂ O		
0.138	0.011	0.137	0.011	0.995	0.009	0.011	47.368	0.286	
0.138	0.011	0.136	0.011	0.987	0.001	0.011	48.063	0.981	
0.138	0.016	0.135	0.015	0.981	-0.005	0.015	48.432	1.350	
0.138	0.016	0.135	0.015	0.978	-0.008	0.015	48.743	1.661	
0.276	0.020	0.274	0.020	0.992	0.006	0.020	46.695	-0.387	
0.276	0.020	0.273	0.019	0.988	0.002	0.019	47.126	0.044	
0.277	0.026	0.272	0.026	0.983	-0.003	0.026	47.026	-0.056	
0.277	0.026	0.272	0.026	0.981	-0.005	0.026	46.884	-0.198	
0.278	0.030	0.275	0.030	0.989	0.003	0.030	45.227	-1.855	
0.278	0.030	0.274	0.030	0.987	0.001	0.030	45.256	-1.826	
				0.986	Y Average			47.082	ΔH _g Average

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.
For ΔH_g, orifice pressure differential that equates to 0.75 cfm (0.0212 m³/min) at standard pressure, acceptable tolerance of individual values from the average is ±0.2 inches (5.1mm)


Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-OV	Date	Time	06/01/2023	10:10 AM	Std Temp	293	K
Console Serial Number	1306033	Calibration Reference No.	SER23-01003			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	759.74			K ₁	0.386	
DGM Serial Number	00009149	Calibration Meter Gamma	0.999			Console Leak Check	PASS	

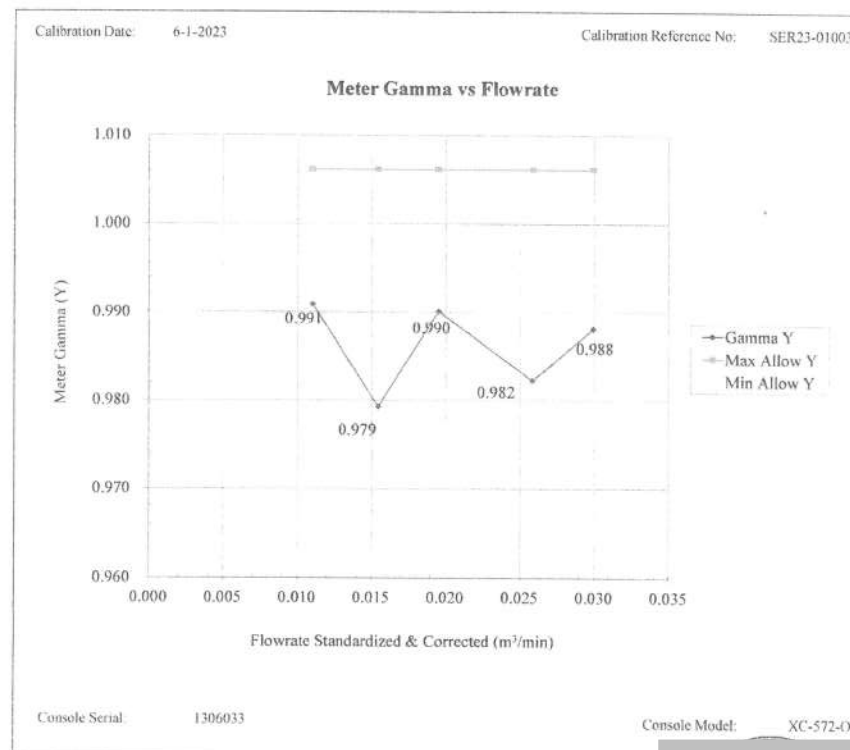

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-OV	Date	Time	06/01/2023	10:10 AM	Std Temp	293	K
Console Serial Number	1306033	Calibration Reference No.	SER23-01003			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	759.74			K ₁	0.386	
DGM Serial Number	00009149	Calibration Meter Gamma	0.999			Console Leak Check	PASS	

Calibration Date: 6-1-2023

Calibration Reference No: SER23-01003

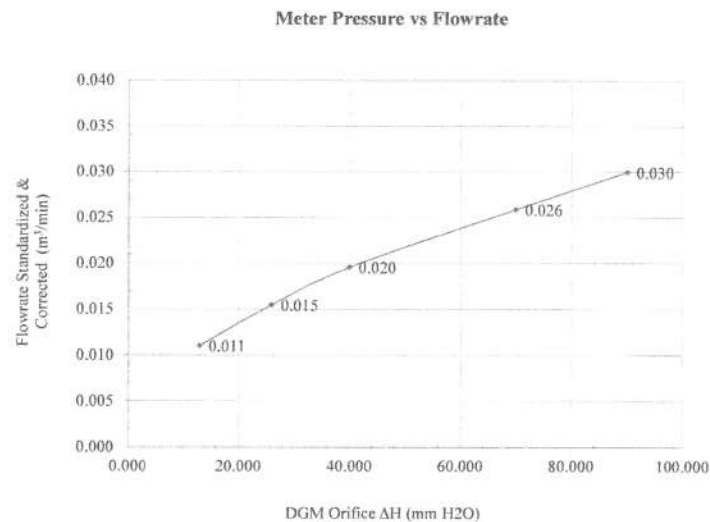

Console Serial: 1306033

Console Model: XC-572-OV

THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information		Calibration Conditions			
Console Model Number	XC-572-OV	Date	Time	06/01/2023	12:10 PM
Console Serial Number	1306033	Calibration Reference No.	SER23-01003		
DGM Model Number	SK25EX	Reference Thermometer	DIGICON		
DGM Serial Number	00009149	Serial Number	183169105		
Meter Box Model Number	JENCO 765 KF				
Meter Box Serial Number	JC 13335				

Results											
Console Thermocouple Simulator											
Channel and test point	Meter Box Channel Temperature Reading (°C)										
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	816.0	1038.0
Stack	-17.0	27.0	37.0	93.0	149.0	259.0	372.0	484.0	595.0	819.0	1042.0
Aux	-17.0	27.0	37.0	92.0	149.0						
Probe	-17.0	27.0	37.0	93.0	149.0						
Filter	-17.0	27.0	37.0	93.0	149.0						
Oven	-17.0	27.0	37.0	93.0	149.0						
Exit	-17.0	27.0	37.0								

Stack ± 1.50% Absolute
Probe ± 3.0 °C
Filter ± 3.0 °C

Tolerance Range

Meter ± 3.0 °C
Exit ± 2.0 °C

Envi Equipment Service Co., Ltd.
110/254 Moo 3, Tambon Bang Rak Phatthana, Amphur Bang Bua Thong, Nonthaburi 11110
Tel. 098 362 9152, 089 478 7885
E-mail: sales@envi-ees.com

Certificate No. : E23-01010
Page : 1 of 3

CERTIFICATE OF CALIBRATION

Customer : Pacific Laboratory Co., Ltd.
Address : 14/5358 Moo 14, Tambon Bang Bua Thong, Amphoe Bang Bua Thong, Nonthaburi 11110
Description of Equipment : Standard Probe Method 5
Manufacturer : Apex Instrument
Model Number : PS-4HV
Serial Number : -
ID./Control No. : -
Environment Conditions : Temperature (25 ± 2) °C
Humidity (50 ± 15) % RH
Cal. Date : 06/01/2023
Issue Date : 06/01/2023

Calibration Method or Calibration Procedure Used

US EPA Method (United State Environmental Protection Agency)

This certificate is traceable to national standard, which realize the units of measurement according to the International System of Units (IS).

Result of Calibration

This certificate may not be reproduced other than in full except with prior Written approval of the Technical Manager, Envi Equipment Service Company Limited.

These reported uncertainties of measurement are expanded by a coverage factor of k=2, providing a 95% confidence level

Calibrated by :

Approved by :

Technical Manager

Certificate No. : E23-01010
Page : 2 of 3

CALIBRATION RESULTS S-Type Geometric Pitot Tube Calibration

Sampling System Equipment Information

Probe Model : PS-4HV
Probe Number : -
Pitot Number : A9148
Pitot Tube Type : S-type

Calibration Condition

Date : 6 January 2023
Barometric Pressure : 759.74 mm Hg
Digital Caliper : CD-6" ASX
Serial number : A18008059

Pitot tube/Probe: # PS-4HV			
Parameter	Value	Allowable Range	Check
Assembly level?	Yes	Yes	Pass
Ports Damage?	No	No	Pass
$\alpha 1$	0	$-10^\circ < \alpha 1 < +10^\circ$	Pass
$\alpha 2$	1	$-10^\circ < \alpha 2 < +10^\circ$	Pass
$\beta 1$	0	$-5^\circ < \beta 1 < +5^\circ$	Pass
$\beta 2$	0	$-5^\circ < \beta 2 < +5^\circ$	Pass
γ	0	N/A	-
θ	0	N/A	-
Dt	0.374	.188" to .375"	Pass
A	0.966	$2.1Dt \leq A \leq 3Dt$	Pass
A/2Dt	1.291	$1.05 \leq A/Dt \leq 1.5$	Pass
$Z = A \tan \gamma$	0.047	$Z \leq .125"$	Pass
$W = A \tan \theta$	0.019	$W \leq .031"$	Pass

Remark:

I certified that probe model: **PS-4HV** meets or exceeds all specifications, criteria and/or applicable design and is hereby assigned a pitot tube certification factor of **0.84**. See 40 CFR Pt. 60, App. A, EPA 1

THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information	
Probe Model Number	PS-4HV
Probe Serial Number	-
Meter Box Model Number	JENCO 765 KF
Meter Box Serial Number	JC 13335

Calibration Conditions			
Date	Time	06/01/2023	01:00 PM
Calibration Reference No.		SER23-01003	
Reference Thermometer		DIGICON	
Serial Number		183169105	

Thermocouple of Standard Probe method 5 = length 4 foot			
Set Point	Reference Thermocouple	Probe Thermocouple	Difference
100	100.0	97.0	0.80
250	250.0	247.0	0.19
300	300.0	298.0	0.35
350	350.0	347.0	0.48

Certificate of Calibration



CUSTOMER

Name
Pacific Laboratory Co., Ltd.
Address
14/5358 Moo 14, Tambon Bang Bua Thong,
Amphoe Bang Bua Thong, Nonthaburi 11110
Department/ Division/ Vessel
N/A

UNIT UNDER CALIBRATION (UUC)

Description
Flue gas analyzer
Manufacturers
testo Model 310
S/N.42848034
Measuring Range
O2 : 0-21 %Vol, CO : 0-4000 PPM

Cert. No. SE-CM23SER117

Cal. Date : 10-Mar-23
Cal. Due : 09-Mar-24
Work Order No. : SE-CM23SER117
Cal. Temp. : 25.0 ± 1°C
Cal. Humidity : 55.0 ± 10 %RH

Reference Standard

Description	Cert. No.	Expired Date
- GASCO Nitrogen = 99.99 %Vol	81-0078RK-01	6-May-25
- Linde Mixture Gas in Nitrogen	3278/22	17-Oct-24
Component : CO = 100 PPM, O2 = 18.0 %		

Function Setup

Items	O2	CO
Low alarm	None	None
High alarm	None	None
Unit	%Vol	PPM

Test Result

Visual Check	Criteria	Result	Operation Check	Criteria	Result
Structure	Proper	Good	Battery storage	Function	Pass
Indication, Symbol and letter	Proper	Good	Suction pump	Function	Pass
Gas sampling hose & probe	Proper	Good			




Calibration Result

Parameter	Zero						Span						Respond time Sec.		Judgment	Note:
	Std.	Acc.	Before	Cal.	After	Err.	Std.	Acc.	Before	Cal.	After	Err.	Acc.	Read		
O2 (%Vol)	0.0	± 1.5	0.0	0.0	0.0	0.0	18.0	± 1.0	18.4	18.4	18.4	0.0	≤30	14.0	Pass	- Respond time must be within 30 sec. to reach to 90% of Std. concentration.
CO (PPM)	0.0	0.0	0.0	0.0	0.0	0.0	100.0	± 5	85.0	85.0	85.0	0.0	≤30	18.0	Pass	

Std. = Standard, Read = Reading, Cal = Calibrate, Acc. = Acceptance, Err. = Error, Sec. = Second

Comment/ Suggestion :

This UUC that has been tested and calibrated to meet the manufacturer's published specifications in accordance with our quality control system. The standards used for calibration are on record and traceable to the National Institute of Standard and Technology (NIST), and have accuracies equal to or greater than the UUC being tested. This result of calibration was found accurate as shown on date and place of calibration only.

Engineer Signatory	Approval Signatory	Company Stamp
		



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com




CERTIFICATE No : 22M8888
REFERENCE No : 66223-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SHIMADZU
MODEL : AF225WD
SERIAL No : D316301828
ID No : LAB-BL-003
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : PACIFIC LABORATORY CO., LTD.
14/5358 MOO. 14 TAMBOL BANGBUA THONG
AMPHOE BANG NUA THONG, NONTHABURI
11110

CALIBRATED BY : ATSAWIN Y.
CALIBRATION DATE : 01-Aug-22
APPROVED BY : 
ISSUED DATE : 02-Aug-22
RECEIVED DATE : 01-Aug-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV 02

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 22M8888

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : AF225WD
MANUFACTURER : SHIMADZU S/N : D316301828
ID No : LAB-BL-003 RECEIVED DATE : 01-Aug-22
AIR PRESSURE : 1005mbar \pm 1mbar CALIBRATION DATE : 01-Aug-22
AMBIENT TEMPERATURE : 25° C \pm 1° C RELATIVE HUMIDITY : 56 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING WEIGHT OF QUALITY CALIBRATION TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23
2) STANDARD WEIGHT	E2	15843	C02210419	10-Feb-23
3) STANDARD WEIGHT	E2	QK-I-349	M2103235S	26-Mar-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT


1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000045 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.000	0.0000	0.0000	0.000075
0.001	0.0010	0.0000	0.000075
0.010	0.0100	0.0000	0.000075
0.050	0.0500	0.0000	0.000076
0.100	0.1000	0.0000	0.000075
1.000	1.0000	0.0000	0.000077
2.000	2.0000	0.0000	0.000077
5.000	5.0000	0.0000	0.000079
20.000	20.0000	0.0000	0.000086
50.000	50.0000	0.0000	0.00011
100.000	100.0001	-0.0001	0.00019
150.000	150.0001	-0.0001	0.00026
200.000	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR

POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA. THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



Certificate of Calibration

Equipment: SPECTROPHOTOMETER
Model: DR3900
Serial No. (or ID.): 2076219
Manufacturer: HACH
Condition: In Condition

Certificate No.: C06220310
Issued Date: 18 July 2022
Job No.: KSPR2207318
Page: 1 of 2

Customer: PACIFIC LABORATORY CO.,LTD.
14/5358 Moo 14 Tambol Bang Bua Thong,
Amphoe Bang Bua Thong, Nonthaburi 11110

Environment Condition: Temperature 23 °C ± 2 °C
Humidity 50 %RH ± 15 %RH

Calibration Place: Environment Laboratory, SPC RT Co., Ltd.
1194 Soi Wachirathamsathit 57, Sukhumvit 101/1 Rd.,
Bangchak, Prakhonong, Bangkok 10260 Thailand

Calibration By: Miss. Kaewkan Suradech
Calibration Date: 18 July 2022
The Method used: In house method, SPCC-WI-24, base on ASTM E 275-08 and ASTM E 387-04
Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 93907 and 93914

The standard for Photometric Certificate No. 94010

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SPC RT Co., Ltd.

Calibration Results:

Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 5 nm and UUC at 5 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.40	418	0.40	0.59
537.00	537	0.00	0.59
638.00	638	0.00	0.59
747.61	747	0.61	0.59
807.04	807	0.04	0.59

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.5816	0.577	0.0046	0.0045
	0.7130	0.709	0.0040	0.0045
	1.0151	1.009	0.0061	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.5649	0.560	0.0049	0.0045
	0.7012	0.700	0.0012	0.0045
	0.9982	0.995	0.0032	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.5249	0.524	0.0009	0.0045
	0.6621	0.662	0.0001	0.0045
	0.9420	0.940	0.0020	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.5214	0.519	0.0024	0.0045
	0.6982	0.699	-0.0008	0.0045
	0.9947	0.992	0.0027	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.5549	0.552	0.0029	0.0045
	0.7736	0.771	0.0026	0.0045
	1.1041	1.099	0.0051	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.5621	0.561	0.0011	0.0045
	0.7630	0.762	0.0010	0.0045
	1.0890	1.085	0.0040	0.0045

The End of Certificate

ภาคผนวกที่ 6-3
เอกสารสอบเทียบปริมาณความเข้มข้นละอองและสารเคมี
ในบรรยากาศการทำงาน

Calibration By



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No.23-66/0141

MTC.No.23-66/0141

Number of page(s) 2

CALIBRATION CERTIFICATE

Nomenclature : DRYCAL DC-LITE FLOWMETER

Manufacturer : BIOS International Corporation, USA.

Serial No.: 104699

Model : DCL-M, Rev 1.09

Scale range : 100 ml/min to 7 l/min

Subdivision : (0.0001, 0.001) l/min

Submitted by : PACIFIC LABORATORY CO.,LTD.

14/5358 Moo14, T.Bang Bua Thong, A.Bang Bua Thong,

Nonthaburi 11110, Thailand.

Received date : 23 December 2022 Condition of measured item : Normal

Calibration date : 5 January 2023

Standard :

Standard	Certificate No.	Date due	Traceability
RTD Thermometer	PSL-T 643/65	1-Jun-24	TISTR
Molbox/PressureTransducer/UpStream	MP-0013-21	25-Jan-23	NIMT
Primary Flow Calibrator S/N 117982	MW-0011-21	8-Apr-23	NIMT
Primary Flow Calibrator S/N 119521	MW-0012-21	31-Mar-23	NIMT

Calibrated by :

Approved by

Director

Mechanical Engineering Standards Laboratory

Ref. 2013265122305450001

Issued Date 5 January 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No.23-66/0141

2/2

MTC.No.23-66/0141

Calibration point : (0.05, 0.1, 0.2, 1.0, 2.0, 3.0) l/min

Ambient condition : Temperature (23 ± 3) °C , Relative humidity (55 ± 15) %

Atmospheric pressure (1010±13) hPa

Calibration method : The flowmeter (UUC) was calibrated by comparison method with standard flowmeter according to CP-370.01.

The reported value is the value that converted to value at reference condition within pressure and temperature of the actual gas entering the UUC

Measurement data :

UUC Value (l/min)	Standard Value (l/min)	Temperature (°C)	Pressure (hPa)	Deviation (%)	Uncertainty (%)
0.0532	0.052339	22.933	1012.22	+1.58	1.05
0.1007	0.99507	22.940	1012.27	+1.20	1.00
0.2027	0.20121	22.989	1012.39	+0.76	0.98
1.013	1.0068	22.977	1012.93	+0.62	0.86
2.008	2.0000	22.955	1013.60	+0.42	0.85
3.010	2.9971	22.949	1014.31	+0.42	0.85

The reported expanded uncertainties are based on standard uncertainties multiplied by a coverage factor $k=2$, which provides a level of confidence of approximately 95%.

The end of calibration certificate.



The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com




CERTIFICATE No : 22M8888
REFERENCE No : 66223-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SHIMADZU
MODEL : AF225WD
SERIAL No : D316301828
ID No : LAB-BL-003
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : PACIFIC LABORATORY CO., LTD.
14/5358 MOO. 14 TAMBOL BANGBUA THONG
AMPHOE BANG NUA THONG, NONTHABURI
11110

CALIBRATED BY : ATSAWIN Y.
CALIBRATION DATE : 01-Aug-22
APPROVED BY : 
ISSUED DATE : 02-Aug-22
RECEIVED DATE : 01-Aug-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV 02

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 22M8888

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : AF225WD
MANUFACTURER : SHIMADZU S/N : D316301828
ID No : LAB-BL-003 RECEIVED DATE : 01-Aug-22
AIR PRESSURE : 1005mbar \pm 1mbar CALIBRATION DATE : 01-Aug-22
AMBIENT TEMPERATURE : 25° C \pm 1° C RELATIVE HUMIDITY : 56 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING WEIGHT OF QUALITY CALIBRATION TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23
2) STANDARD WEIGHT	E2	15843	C02210419	10-Feb-23
3) STANDARD WEIGHT	E2	QK-I-349	M2103235S	26-Mar-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT


1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000045 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.000	0.0000	0.0000	0.000075
0.001	0.0010	0.0000	0.000075
0.010	0.0100	0.0000	0.000075
0.050	0.0500	0.0000	0.000076
0.100	0.1000	0.0000	0.000075
1.000	1.0000	0.0000	0.000077
2.000	2.0000	0.0000	0.000077
5.000	5.0000	0.0000	0.000079
20.000	20.0000	0.0000	0.000086
50.000	50.0000	0.0000	0.00011
100.000	100.0001	-0.0001	0.00019
150.000	150.0001	-0.0001	0.00026
200.000	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR

POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA. THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

ใบรับรองการสอบเทียบ “เครื่อง Ion chromatography”
(Calibration Certificate of Ion chromatography)



Document Type	Certificate of Performance (CofP)
Description	CofP for 881 Compact IC pro
Document ID	CofP.881 Version 1.4 / 8.881.3006EN

Metrohm Compliance Service

Certificate of Performance (CofP) for
881 Compact IC pro

Instrument details

Type:	18810000
Serial No.:	PM220395/ME (1881000010137)
Manufacturer:	Metrohm AG Ionenstrasse CH-9100 Herisau Switzerland
Firmware:	5.850.0113
Customer Instrument ID:	N/A

Customer details

Name of company:	EMEX Association Co., Ltd.
Address:	27, 29 Bang Mot, Chomthong, Bangkok 10150
Department:	Laboratory
Responsible person:	คุณอัครา วงษ์นิม
Calibration place:	Laboratory EMEX Association Co., Ltd

Date and time of calibration: 22/12/2022 - 08:30

Certificate of Performance (CofP) No.: PM220395/ME (1881
08:30



Document Type Certificate of Performance (CoP)
Description CoP for 881 Compact IC pro
Document ID CoP.881 Version 1.4 / 8.881.3006EN

Certificate of Performance (CoP)

Introduction

The instrument stated above has been inspected in accordance with the corresponding test instructions of Metrohm Ltd. Servicing instructions are compiled and checked for correctness with account taken of the technical apparatus and ambient conditions available to the service engineer at the servicing location. This Certificate of Performance (CoP) declares the results regarding calibration and operational status obtained when carrying out the test instructions referred to below.

Calibration status

We certify that the instrument stated above meets or exceeds the electrical specifications at the points tested. Test equipment is calibrated and traceable back to national and/or international standards (ISO 17025, NIST).

Operational status

We certify that the instrument stated above executes the instrument's specific functions tested except where detailed overleaf.

Declaration

Document

Test instructions used: C.1 Test instructions for 881 Compact IC pro, Version 1.4

Reference standards

Type / Model	Manufacturer	Serial No. / Batch No.	Certificate No.	Due date / Expiry date
Multimeter	Fluke	89490190	E1U222184	25/05/2023
Temperature meas. Instr.	Fluke	82090101	TMU221923	10/06/2023
High pressure gauge	Metrohm	349648018913	CC_00017008	11/04/2023
Flow meter	ANALYT-MTC	94306	AD2201-280-0001	31/01/2023

Protocol

Instrument had to be repaired beforehand

Yes ☐ No ☒

If yes, see Certificate of Performance (CoP) No.:

Instrument had to be readjusted beforehand

Yes ☐ No ☒

If yes, see Certificate of Performance (CoP) No.:

Certificate of Performance (CoP) No.: PM220395/ME (1881000010137)
08:30



Document Type Certificate of Performance (CoP)
Description CoP for 881 Compact IC pro
Document ID CoP.881 Version 1.4 / 8.881.3006EN

Conclusion of test results

	Yes	No
Instrument satisfies the specified technical requirements	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Recommended date for next maintenance:		

Comments

Metrohm representative

			Yes	No
Metrohm representative confirms correct execution of instrument calibration			<input checked="" type="checkbox"/>	<input type="checkbox"/>
Date	Name	Signature		
22/12/2022	Mr.Prutchaya Kumpairee			

Customer representative

			Yes	No
Customer representative accepts results of instrument calibration			<input checked="" type="checkbox"/>	<input type="checkbox"/>
Date	Name	Signature		
22/12/2022	คุณอัครวิทย์ วรณนิต			

Certificate of Performance (CoP) No.: PM220395/ME (1881000010137)
08:30



Document Type Certificate of Performance (CoP)
Description CoP for 881 Compact IC pro
Document ID CoP.881 Version 1.4 / 8.881.3006EN

Test results

No.	Title	Comments	Pass		
			Yes	No	N/A
100	Visual test		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
101	Safety test		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
102	LED		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
103	Fan		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
104	Communication		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
105	Leak detector		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
106	MSB interface		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
107	USB interface		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
108	Column plug interface		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
109	Column heater		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
110	IC pump		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
111	Injector		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
112	Degasser		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
113	MSM (option)				

Certificate of Performance (CoP) No.: PM220395/ME (1881000010137)
08:30



Document Type Certificate of Performance (CoP)
Description CoP for 881 Compact IC pro
Document ID CoP.881 Version 1.4 / 8.881.3006EN

No.	Title	Comments	Pass		
			Yes	No	N/A
114	Peristaltic pump (option)		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
115	MCS (option)		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Certificate of Performance (CoP) No.: PM220395/ME (1881000010137)
08:30



Document Type Certificate of Performance (CofP)
Description CoP for 881 Compact IC pro
Document ID CoP.881 Version 1.4 / 8.881.3006EN

CofP.881 Document History

Date	Version	Author	Description/Changes
16.04.2012	8.881.3004EN	pr	Layout adapted to Metrohm Compliance Service
20.02.2013	8.881.3006EN	pr	Test step 113.2 tolerance increased according C.3 notice of modification CRM-10456
30.03.2021	1.4	pr	Change of document history and versioning (article no. remains the same; new versions are indicated by increase of version number only). Test no. 103 Fan depends on the installed power supply version according C.3 notice of modification CRM-28908.

End of CofP Document

Certificate of Performance (CofP) No.: PM220395/ME (1881000010137) - 08:30



Document Type Certificate of Performance (CofP)
Description CoP for 850.9010 Conductivity Detector
Document ID CoP.850 Version 1.3 / 8.850.3023EN

Metrohm Compliance Service

Certificate of Performance (CofP) for 850.9010 Conductivity Detector

Instrument details

Type: 18509010
Serial No.: PM220395/ME (1850901012155)
Manufacturer: Metrohm AG, Ionenstrasse, CH-9100 Herisau
Switzerland
Customer instrument ID: N/A

Control device details

Type: 1.881.0030
Serial No.: 1881000010137
Firmware: 5.850.0113

Customer details

Name of company: EMEX Association Co., Ltd.
Address: 27, 29 Bang Mot, Chomthong, Bangkok 10150

Department: Laboratory
Responsible person: คุณอัครา วัฒนชัย
Calibration place: Laboratory
EMEX Association Co., Ltd

Date and time of calibration: 22/12/2022 - 08:30

Certificate of Performance (CofP) No.: PM220395/ME (1850901012155) - 08:30



Document Type Certificate of Performance (CoP)
Description CoP for 850.9010 Conductivity Detector
Document ID CoP.850 Version 1.3 / 8.850.3023EN

Certificate of Performance (CoP)

Introduction

The instrument stated above has been inspected in accordance with the corresponding test instructions of Metrohm Ltd. Servicing instructions are compiled and checked for correctness with account taken of the technical apparatus and ambient conditions available to the service engineer at the servicing location. This Certificate of Performance (CoP) declares the results regarding calibration and operational status obtained when carrying out the test instructions referred to below.

Calibration status

We certify that the instrument stated above meets or exceeds the electrical specifications at the points tested. Test equipment is calibrated and traceable back to national and/or international standards (ISO 17025, NIST).

Operational status

We certify that the instrument stated above executes the instrument's specific functions tested except where detailed overleaf.

Declaration

Document

Test instructions used: C.1 Test Instructions for 850.9010 Conductivity Detector, Version 1.3

Reference standards

Type / Model	Manufacturer	Serial No. / Batch No.	Certificate No.	Due date / Expiry date
Temperature meas. instr.	Fluke	82090101	TMU221923	10/08/2023
Conductivity standard (opt.)	N/A	N/A	N/A	N/A

Protocol

	Yes	No
Instrument had to be repaired beforehand	<input type="checkbox"/>	<input checked="" type="checkbox"/>
If yes, see Certificate of Performance (CoP) No.:		
Instrument had to be readjusted beforehand	<input type="checkbox"/>	<input checked="" type="checkbox"/>
If yes, see Certificate of Performance (CoP) No.:		

Certificate of Performance (CoP) No.: PM220395/ME (185090101215)
08:30



Document Type Certificate of Performance (CoP)
Description CoP for 850.9010 Conductivity Detector
Document ID CoP.850 Version 1.3 / 8.850.3023EN

Conclusion of test results

	Yes	No
Instrument satisfies the specified technical requirements	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Recommended date for next maintenance:		

Comments

Metrohm representative

	Yes	No
Metrohm representative confirms correct execution of instrument calibration	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Date	Name	Signature
22/12/2022	Mr. Prutchaya Kumpalree	

Customer representative

	Yes	No
Customer representative accepts results of instrument calibration	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Date	Name	Signature
22/12/2022	สุพจน์ วรรณรัตน์	

Certificate of Performance (CoP) No.: PM220395/ME (185090101215)
08:30



Document Type	Certificate of Performance (CoP)
Description	CoP for 850.9010 Conductivity Detector
Document ID	CoP.850 Version 1.3 / 8.850.3023EN

Test results

No.	Title	Comments	Pass		
			Yes	No	N/A
100	Visual inspection		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
101	Temperature absolute		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
102	Temperature stability		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
103	Signal noise		<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
104	Conductivity dry test		<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
105	Conductivity cell (optional)		<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>

CoP.850 Document History

Date	Article No.	Author	Description/Changes
26.04.2012	8.850.3023EN	Philipp Rüegg	Layout adapted to Metrohm Compliance Service

End of CoP Document

ภาคผนวกที่ 6-4
เอกสารสอบเทียบระดับความดังเสียง
(Sound Level Meter)



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917



NSC-7981-TIS 17020
CALIBRATION 0159

Certificate No.: CP20230151EA

Operation No.: CP2023030003

Certificate of Calibration

Equipment: Sound Calibrator

Manufacturer: TENMARS

Model/Type: TM-100

Serial No.: 220501964

ID No.: -

Customer: Pacific Laboratory Co., Ltd.

Address: 14/5358 Moo 14 T. Bang Bua Thong
A. Bang Bua Thong, Nonthaburi 11110

Received Date: 3 March 2023

Calibrated Date: 14 March 2023

Issued Date: 16 March 2023

Calibrated by: Ms. Juntaporn Kunhakom

Approved by:



This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20230151EA

Calibration Report

Equipment: Sound Calibrator

Manufacturer: TENMARS

Model/Type: TM-100

Serial No.: 220501964

ID No.: -

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-

IEC 60942:2017

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2661000	AA-1020-22	14 June 2023
2) Waveform Generator	33511B	MY52302264	CK20220058EA	19 June 2023
3) Audio Analyzing DMM	2015-P	4079144	E1U221042	16 March 2023
4) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P220024 CD20220164EA	17 March 2023 24 July 2023

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

1. Function : Sound pressure level

Normal	Specified Sound	Measured value	Deviated value ^[1]	Acceptance limit ^[3]
Frequency (Hz)	Pressure level (dB)	(dB)	(dB)	(dB)
1000	94	94.25	0.25	±0.40
1000	114	114.39	0.39	±0.40

2. Function : Frequency

Normal Sound	Specified Frequency	Measured value	Deviated value ^[2]	Acceptance limit ^[3]
Pressure level (dB)	(Hz)	(Hz)	(%)	(%)
94	1000	970.1	-2.99	±1.7
114	1000	967.4	-3.26	±1.7



Certificate No.: CP20230151EA

Calibration Report

3. Function : Total distortion + noise

Normal level	Normal	Measured value ^[4]	Acceptance limit ^[5]
Sound Pressure level (dB)	Frequency (Hz)	(%)	(%)
94	1000	1.7	3.0
114	1000	1.4	3.0

Uncertainty of measurement

Function	Uncertainty	Maximum-permitted uncertainty of measurement
Sound pressure level	0.10 dB	0.35 dB
Frequency	0.10 %	0.20 %
Total distortion + noise	0.40 %	1.00 %

Note:

- [1] The deviated value is the absolute value of the difference between the measured value and the corresponding specified sound pressure level.
- [2] The deviated value is the absolute value of the difference in percent between the measured value and the corresponding specified frequency.
- [3] The acceptance limit is for the deviated value.
- [4] The measured value is the total distortion + noise, measured over the frequency range from 20 Hz to 20 kHz.
- [5] The acceptance limit is for the Measured value.

Remarks: 1. Acceptance limit was IEC 60942:2017 Class 2.
2. The coverage factor $k = 2.00$.

- - End of Report - -



PACIFIC LABORATORY CO. LTD.

Pacific Laboratory Co., Ltd.

Sound Level Meter Calibration Report

Calibrate No. : SLM 031/2566

Calibrate Date : April 19, 2023

Equipment : Sound Calibrator
Manufacturer : TENMARS
Model/Type : TM-100
Serial No. : 190301469
Customer Name : บริษัท อสมิเนี่ยม อีจ อีจ จำกัด

[illegible]

Approved By



CERTIFICATE OF CALIBRATION

NO. 20230217118



Name of Product: Sound Level Meter
Model: ST-11D
Serial Number: 820968
Specification: Class 1
Conclusion: Pass
Date of calibration: 2023-02-24
Due Date: 2024-02-23

- This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-58818

4. Measuring up limit: 140 dBA

3. Adjustments to indicated sound levels:

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Type of Calibrator: B&K 4231

Sound Pressure Level: 94.0 dB

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.0	-14.7	-1.3	1000	0.0	0.0	-0.1
20	-50.2	-6.2	-0.3	2000	1.3	-0.1	0.0
31.5	-39.5	-3.0	-0.1	4000	1.2	-0.7	0.0
63	-26.2	-0.7	-0.1	8000	-1.0	-3.0	0.0
125	-16.2	-0.2	-0.1	12500	-5.9	-7.8	-0.1
250	-8.6	0.0	-0.1	16000	-11.7	-13.7	0.0
500	-3.2	0.0	0.0	20000	-23.8	-25.8	-0.2

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L _{Aeq,T}	103.2	103.2	0.0
L ₅	110.8	110.8	0.0
L ₁₀	108.8	108.8	0.0
L ₅₀	92.9	92.8	0.1
L ₉₀	76.9	76.8	0.1
L ₉₅	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions:

Air temperature: 18 °C
Relative humidity: 60 %
Static pressure: 101.8 kPa

Reference equipment used in the calibration:

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2024-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2024-10-15	CIGISMEC
Signal generator	DS 360	33873	2024-10-15	CEPREI

Test specifications:

- All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
- The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of $\pm 20\%$.
- The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC230140

Customer : Pacific Laboratory Co., Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong,
Amphoe Bang Thong, Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC230140
Manufacturer	: Scarlet Tech	Calibration Location	: Laboratory
Model	: ST-11D	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 820967	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: -	Received Date	: 21-Mar-2023

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20220161EA	NIMT	13-May-24

Authority of Calibration

Calibration Date : 23-Mar-2023
Issued Date : 27-Mar-2023
Calibrated By : Mr. Rattapong Janpanya

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC230140

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use	: Good
Results of Calibration	: Without any adjustment
Sound Level Calibration	
- Frequency Weighting	: A
- Resolution	: 0.1 dB

Sound Level Measurement (Slow Mode)

Parameter	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LFp	20-140 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB
LSp	20-140 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB
Llp	20-140 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Parameter	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LFp	20-140 dB	93.86 dB	93.7 dB	-0.16 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB
LSp	20-140 dB	93.86 dB	93.7 dB	-0.16 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB
Llp	20-140 dB	93.86 dB	93.7 dB	-0.16 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB

--- End of Certificate ---



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC230015

Customer : Pacific Laboratory Co.,Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC230015
Manufacturer	: ACO	Calibration Location	: Laboratory
Model	: 6236	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 222014	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 04-Jan-23

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20220161EA	TISI: 22-LB0125	13-May-24

APTITECH

Authority of Calibration

Calibration Date : 05-Jan-2023
Issued Date : 10-Jan-2023
Calibrated By : Mr. Rattapong Janpanya

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC230015

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment

Sound Level Measurement (Slow Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.7 dB	-0.16 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.7 dB	-0.16 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.7 dB	-0.16 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.7 dB	-0.16 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB

--- End of Certificate ---



APTITECH CALIBRATION CO., LTD.
50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC230023

Customer : Pacific Laboratory Co.,Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC230023
Manufacturer	: ACO	Calibration Location	: Laboratory
Model	: 6236	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 222023	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 04-Jan-23

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20220161EA	TISI: 22-LB0125	13-May-24

APTITECH

Authority of Calibration

Calibration Date : 05-Jan-2023
Issued Date : 10-Jan-2023
Calibrated By : Mr. Rattapong Janpanya

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.
50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC230023

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment

Sound Level Measurement (Slow Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB

--- End of Certificate ---



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC230102

Customer : Pacific Laboratory Co.,Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC230102
Manufacturer	: ACO	Calibration Location	: Laboratory
Model	: 6236	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 222138	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 24-Feb-23

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor k=2 such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20220161EA	TISI: 22-LB0125	13-May-24

Authority of Calibration

Calibration Date : 27-Feb-2023
Issued Date : 2-Mar-2023
Calibrated By : Mr. Sataporn Petnoi

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC230102

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment

Sound Level Measurement (Slow Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.9 dB	0.04 dB	0.60 dB
		113.87 dB	113.9 dB	0.03 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.9 dB	0.04 dB	0.60 dB
		113.87 dB	113.9 dB	0.03 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB

--- End of Certificate ---



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC230037

Customer : Pacific Laboratory Co.,Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC230037
Manufacturer	: ACO	Calibration Location	: Laboratory
Model	: 6236	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 222046	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 13-Jan-23

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20220161EA	TIS: 22-LB0125	13-May-24

Authority of Calibration

Calibration Date : 15-Jan-2023
Issued Date : 20-Jan-2023
Calibrated By : Mr. Sataporn Petnoi

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC230037

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment

Sound Level Measurement (Slow Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	94.00 dB	93.8 dB	-0.20 dB	0.60 dB
		114.00 dB	113.8 dB	-0.20 dB	0.60 dB
LC	40-130 dB	94.00 dB	93.8 dB	-0.20 dB	0.60 dB
		114.00 dB	113.8 dB	-0.20 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	94.00 dB	93.8 dB	-0.20 dB	0.60 dB
		114.00 dB	113.7 dB	-0.30 dB	0.60 dB
LC	40-130 dB	94.00 dB	93.8 dB	-0.20 dB	0.60 dB
		114.00 dB	113.7 dB	-0.30 dB	0.60 dB

--- End of Certificate ---



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email: sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC230107

Customer : Pacific Laboratory Co. Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC230107
Manufacturer	: ACO	Calibration Location	: Laboratory
Model	: 6236	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 222170	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 24-Feb-23

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20220151EA	TISI: 22-LB0125	13-May-24

Authority of Calibration



Calibration Date : 27-Feb-2023
Issued Date : 2-Mar-2023
Calibrated By : Mr. Sataporn Petnoi

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email: sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC230107

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment

Sound Level Measurement (Slow Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB

--- End of Certificate ---



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC230018

Customer : Pacific Laboratory Co., Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC230018
Manufacturer	: ACO	Calibration Location	: Laboratory
Model	: 6236	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 222017	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 04-Jan-23

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20220161EA	TISI: 22-LB0125	13-May-24

APTITECH

Authority of Calibration

Calibration Date : 05-Jan-2023
Issued Date : 10-Jan-2023
Calibrated By : Mr. Rattapong Janpanya

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC230018

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment

Sound Level Measurement (Slow Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.7 dB	-0.16 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB

--- End of Certificate ---



APTITECH CALIBRATION CO., LTD.
50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC230017

Customer : Pacific Laboratory Co.,Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC230017
Manufacturer	: ACO	Calibration Location	: Laboratory
Model	: 6236	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 222016	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 04-Jan-23

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20220161EA	TISI: 22-LB0125	13-May-24

Authority of Calibration

Calibration Date : 05-Jan-2023
Issued Date : 10-Jan-2023
Calibrated By : Mr. Rattapong Janpanya

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.
50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC230017

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment

Sound Level Measurement (Slow Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.7 dB	-0.16 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB

Sound Level Measurement (Fast Mode)


Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.7 dB	-0.16 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB

--- End of Certificate ---



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC230112

Customer : Pacific Laboratory Co.,Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC230112
Manufacturer	: ACO	Calibration Location	: Laboratory
Model	: 6236	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 222177	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 24-Feb-23

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20220151EA	TISI: 22-LB0125	13-May-24

APTITECH

Authority of Calibration



Calibration Date : 27-Feb-2023
Issued Date : 2-Mar-2023
Calibrated By : Mr. Sataporn Petnoi

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC230112

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment

Sound Level Measurement (Slow Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB

--- End of Certificate ---



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email: sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC230097

Customer : Pacific Laboratory Co., Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC230097
Manufacturer	: ACO	Calibration Location	: Laboratory
Model	: 6236	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 222133	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 24-Feb-23

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20220161EA	TISI: 22-LB0125	13-May-24



Authority of Calibration



Calibration Date : 27-Feb-2023
Issued Date : 2-Mar-2023
Calibrated By : Mr. Sataporn Petnoi

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email: sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC230097

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment

Sound Level Measurement (Slow Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.8 dB	-0.07 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.8 dB	-0.06 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB

--- End of Certificate ---



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamlukka, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC230022

Customer : Pacific Laboratory Co., Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC230022
Manufacturer	: ACO	Calibration Location	: Laboratory
Model	: 6236	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 222022	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 04-Jan-23

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	141011576	CP20220161EA	TISI: 22-LB0125	13-May-24

APTITECH

Authority of Calibration

Calibration Date : 05-Jan-2023
Issued Date : 10-Jan-2023
Calibrated By : Mr. Rattapong Janpanya

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamlukka, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC230022

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment

Sound Level Measurement (Slow Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.5 dB	-0.37 dB	0.60 dB

--- End of Certificate ---



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CERTIFICATE OF CALIBRATION

Certificate Number : SC230020

Customer : Pacific Laboratory Co., Ltd.
Address : 14/5358 Moo 14 Tambol Bang Bua Thong, Amphoe Bang Thong,
Nonthaburi 11110

Description	: Sound Level Meter	W/O Number	: SC230020
Manufacturer	: ACO	Calibration Location	: Laboratory
Model	: 6236	Ambient Temperature	: 22 ± 2 °C
Serial Number	: 222019	Ambient Humidity	: 55 ± 15 %RH
ID. Number	: N/A	Received Date	: 04-Jan-23

This certifies that the above instrument was calibrated in compliance with the Calibration Systems Requirement of ISO/IEC 17025:2017 in accordance with referenced procedures. Standards used to perform this calibration are certified by or traceable to National Institute of Metrology (Thailand) and/or other recognized national measurement institutes which realizes the units of measurement according to the International System of Units (SI Unit).

Measurement uncertainties at the time of test are given where applicable. They are calculated in accordance with the method described in The Expression of Uncertainty and Confidence in Measurement (M3003).

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$ such that the coverage probability corresponds to approximately 95%. This result of calibration was found accurate as shown on date and place of calibration only.

Standard Equipments

Description	Serial No.	Certificate No.	Traceability	Due Date
Sound Level Calibrator	14101:576	CP20220161EA	TISI: 22-LB0:25	13-May-24

APTITECH

Authority of Calibration


Calibration Date : 05-Jan-2023
Issued Date : 10-Jan-2023
Calibrated By : Mr. Rattapong Janpanya

Calibration certificates without signatures are not valid. This certificate applied to only the item identified and shall not be reproduced other than in full, without the specific written approval by APTITECH CALIBRATION CO., LTD.



APTITECH CALIBRATION CO., LTD.

50/40 Moo 5 T. Lat Sawai, A. Lamukha, Pathumthani 12150
Tel. +66 2103-6290 Fax. +66 2103-6291
Email. sales@aptitech-cal.com



CALIBRATION REPORT

Certificate Number : SC230020

Calibration Method

The Unit Under Calibration (UUC) was calibrated by comparison measurement with sound level calibrator. The calibration has been accomplished in an ambient environment controlled, base on the in-house calibration procedure. The identification of the laboratory's calibration procedure employed are CP-7.2-01-107

Calibration Results

Appearance and function of use : Good
Results of Calibration : Without any adjustment

Sound Level Measurement (Slow Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.7 dB	-0.16 dB	0.60 dB
		113.87 dB	113.7 dB	-0.17 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.7 dB	-0.16 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB

Sound Level Measurement (Fast Mode)

Function	UUC Range	Standard Value	UUC Reading	UUC Error	(±) Uncertainty
LA	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB
LC	40-130 dB	93.86 dB	93.6 dB	-0.26 dB	0.60 dB
		113.87 dB	113.6 dB	-0.27 dB	0.60 dB

--- End of Certificate ---

ภาคผนวกที่ 6-5
เอกสารสอบเทียบสภาพความร้อน (Heat Stress)



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 31 January, 2023

Certification No. 038/23

Page : 1 of 2

Object : Thermal Environment Monitor

Manufacturer : QUEST TECHNOLOGIES

Type : QUESTemp°34

Serial No. : TED060012

Customer : Pacific Laboratory Co.,Ltd.
14/5358 Moo 14, T. Bang Bua,
A.Bang Bua Thong, Nonthaburi 11110.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1014.8 hPa

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02848057 : Thermoschneider No.6169 , No.6178

: TT-3 Serial 43BE04

Japan Meteorological Agency





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 038/23

31 January, 2023

Page : 2 of 2

Standard Temp. °C	Temperature Sensor Reading					
	Dry Bulb °C	Correction °C	Globe °C	Correction °C	Wet Bulb °C	Correction °C
50.08	49.9	0.18	50.0	0.08	49.9	0.18
41.02	41.0	0.02	41.1	-0.08	41.1	-0.08
30.45	30.4	0.05	30.5	-0.05	30.4	0.05



Request No. 22-66 / 0323

MTC No. PSL-H 0148 / 66

Certificate of Calibration

Customer : Envilab Co.,Ltd.
540, 540/1 Soi Bangkhae7, Bangkhae, Bangkok, 10160

Item : Thermo-Hygrometer (Area Heat Stress Monitor)

Model /Type : hs-32

Serial Number : MCE030043

Manufacturer : METROSONICS

Date of Request : 9 February 2023

Date of Calibration : 24 February 2023

The certifies the above equipment was calibrated in accordance with the recognised International Standard ISO/IEC 17025:2017 and the operation according to procedure no. WI.CP.18.

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95 %.

Calibrated by :

Approved by :

Photometry and Temperature Standards Laboratory

Ref. No : 2012266020900611003

Issued Date : 8 March 2023

Page 1 of 4

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BL.MTC.002 Rev.4

Request No. 22-66 / 0323

MTC No. PSL-H 0148 / 66

Description of Unit Under Calibration :

Customer : Envilab Co.,Ltd.
Address : 540, 540/1 Soi Bangkhae7, Bangkhae, Bangkok, 10160
Item : Thermo-Hygrometer (Area Heat Stress Monitor)
Serial Number : MCE030043
Calibration Required : Temperature at (20, 30, 40) °C
Ambient Condition : Ambient temperature (23 ± 3) °C
Relative humidity (55 ± 20) %
Laboratory Address : Photometry and Temperature Standards Laboratory
Soi 1, Bangpoo Industrial Estate, Sukhumvit Rd., Samutprakan

Reference Standard :

Digital Thermometer with Sensor, Model : F250H, S/N : 9345 008 2331, Sensor RTD Probe No. RTD-01 and RTD-02 which was calibrated by Industrial Metrology and Testing Service Centre, Certificate No. PSL-T 0786/65.

The temperature scale in use of this laboratory is the International Temperature Scale of 1990.

Calibration Procedure :

The certifies the above equipment was calibrated according to procedure no. WI.CP.18.

Support Equipment :

Temperature & Humidity Controlled Chamber, Model : 9141-5110, S/N : 1205101

Adjustments : NONE

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

Request No. 22-66 / 0323

MTC No. PSL-H 0148 / 66

Results of Calibration :- (/) Without Adjustment () After Adjustment

Table : Temperature Measurement @ Wet Bulb

Average Measured Temperature (°C)	Average Displayed of UUC (°C)	Correction Measured of UUC (°C)	Expanded Uncertainty of Measurement (± °C)
20.1	20.4	-0.3	0.50
30.0	29.9	0.1	0.50
40.0	39.6	0.4	0.50

Table : Temperature Measurement @ Dry Bulb

Average Measured Temperature (°C)	Average Displayed of UUC (°C)	Correction Measured of UUC (°C)	Expanded Uncertainty of Measurement (± °C)
20.1	20.4	-0.3	0.50
30.0	29.8	0.2	0.50
40.0	39.5	0.5	0.50

Request No. 22-66 / 0323

MTC No. PSL-H 0148 / 66

Results of Calibration :-

Table : Temperature Measurement @ Globe Bulb

Average Measured Temperature (°C)	Average Displayed of UUC (°C)	Correction Measured of UUC (°C)	Expanded Uncertainty of Measurement (± °C)
20.0	20.7	-0.7	0.50
30.0	29.6	0.4	0.50
40.0	39.4	0.6	0.50

- Note :**
1. This calibration was done without removing reservoir cover, white plates and blackened copper sphere of the instrument.
 2. The calibration data for instrument in this report is reported within the condition existing at the time of measurement only.

...end of certificate...

Request No. 22-66 / 0323

MTC No. PSL-H 0150 / 66

Certificate of Calibration

Customer : Envilab Co.,Ltd.
540, 540/1 Soi Bangkhae7, Bangkhae, Bangkok, 10160

Item : Thermo-Hygrometer (Area Heat Stress Monitor)

Model /Type : hs-32

Serial Number : MCG080040

Manufacturer : METROSONICS

Date of Request : 9 February 2023

Date of Calibration : 24 February 2023

The certifies the above equipment was calibrated in accordance with the recognised International Standard ISO/IEC 17025:2017 and the operation according to procedure no. WL.CP.18.

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95 %.

Calibrated by :

Approved by :

Photometry and Temperature Standards Laboratory

Ref. No : 2012266020900611005

Issued Date : 8 March 2023

Page 1 of 4

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Request No. 22-66 / 0323

MTC No. PSL-H 0150 / 66

Description of Unit Under Calibration :

Customer : Envilab Co.,Ltd.
Address : 540, 540/1 Soi Bangkhae7, Bangkhae, Bangkok, 10160
Item : Thermo-Hygrometer (Area Heat Stress Monitor)
Serial Number : MCG080040
Calibration Required : Temperature at (20, 30, 40) °C
Ambient Condition : Ambient temperature (23 ± 3) °C
Relative humidity (55 ± 20) %
Laboratory Address : Photometry and Temperature Standards Laboratory
Soi 1, Bangpoo Industrial Estate, Sukhumvit Rd., Samutprakan

Reference Standard :

Digital Thermometer with Sensor, Model : F250H, S/N : 9345 008 2331, Sensor RTD Probe No. RTD-01 and RTD-02 which was calibrated by Industrial Metrology and Testing Service Centre, Certificate No. PSL-T 0786/65.

The temperature scale in use of this laboratory is the International Temperature Scale of 1990.

Calibration Procedure :

The certifies the above equipment was calibrated according to procedure no. WI.CP.18.

Support Equipment :

Temperature & Humidity Controlled Chamber, Model : 9141-5110, S/N : 1205101

Adjustments : NONE

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

Request No. 22-66 / 0323

MTC No. PSL-H 0150 / 66

Results of Calibration :- (/) Without Adjustment () After Adjustment

Table : Temperature Measurement @ Wet Bulb

Average Measured Temperature (°C)	Average Displayed of UUC (°C)	Correction Measured of UUC (°C)	Expanded Uncertainty of Measurement (± °C)
19.9	20.4	-0.5	0.50
30.0	30.2	-0.2	0.50
40.1	40.2	-0.1	0.50

Table : Temperature Measurement @ Dry Bulb

Average Measured Temperature (°C)	Average Displayed of UUC (°C)	Correction Measured of UUC (°C)	Expanded Uncertainty of Measurement (± °C)
19.9	20.2	-0.3	0.50
30.0	30.2	-0.2	0.50
40.1	40.1	0.0	0.50

Request No. 22-66 / 0323

MTC No. PSL-H 0150 / 66

Results of Calibration :-

Table : Temperature Measurement @ Globe Bulb

Average Measured Temperature (°C)	Average Displayed of UUC (°C)	Correction Measured of UUC (°C)	Expanded Uncertainty of Measurement (± °C)
20.0	20.2	-0.2	0.50
30.0	30.1	-0.1	0.50
40.1	40.0	0.1	0.50

- Note :**
1. This calibration was done without removing reservoir cover, white plates and blackened copper sphere of the instrument.
 2. The calibration data for instrument in this report is reported within the condition existing at the time of measurement only.

...end of certificate...

Request No. 22-66 / 0323

MTC No. PSL-H 0149 / 66

Certificate of Calibration

Customer : Envilab Co.,Ltd.
540, 540/1 Soi Bangkhae7, Bangkhae, Bangkok, 10160

Item : Thermo-Hygrometer (Area Heat Stress Monitor)

Model /Type : hs-32

Serial Number : MCG010014

Manufacturer : METROSONICS

Date of Request : 9 February 2023

Date of Calibration : 24 February 2023

The certifies the above equipment was calibrated in accordance with the recognised International Standard ISO/IEC 17025:2017 and the operation according to procedure no. WI.CP.18.

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95 %.

Calibrated by :

Approved by :

Photometry and Temperature Standards Laboratory

Ref. No : 2012266020900611004

Issued Date : 8 March 2023

Page 1 of 4

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Request No. 22-66 / 0323

MTC No. PSL-H 0149 / 66

Description of Unit Under Calibration :

Customer : Envilab Co.,Ltd.
Address : 540, 540/1 Soi Bangkhae7, Bangkhae, Bangkok, 10160
Item : Thermo-Hygrometer (Area Heat Stress Monitor)
Serial Number : MCG010014
Calibration Required : Temperature at (20, 30, 40) °C
Ambient Condition : Ambient temperature (23 ± 3) °C
Relative humidity (55 ± 20) %
Laboratory Address : Photometry and Temperature Standards Laboratory
Soi 1, Bangpoo Industrial Estate, Sukhumvit Rd., Samutprakan

Reference Standard :

Digital Thermometer with Sensor, Model : F250H, S/N : 9345 008 2331, Sensor RTD Probe No. RTD-01 and RTD-02 which was calibrated by Industrial Metrology and Testing Service Centre, Certificate No. PSL-T 0786/65.

The temperature scale in use of this laboratory is the International Temperature Scale of 1990.

Calibration Procedure :

The certifies the above equipment was calibrated according to procedure no. WI.CP.18.

Support Equipment :

Temperature & Humidity Controlled Chamber, Model : 9141-5110, S/N : 1205101

Adjustments : NONE

Request No. 22-66 / 0323

MTC No. PSL-H 0149 / 66

Results of Calibration :- (/) Without Adjustment () After Adjustment

Table : Temperature Measurement @ Wet Bulb

Average Measured Temperature (°C)	Average Displayed of UUC (°C)	Correction Measured of UUC (°C)	Expanded Uncertainty of Measurement (± °C)
19.9	20.2	-0.3	0.50
30.0	30.0	0.0	0.50
40.1	39.8	0.3	0.50

Table : Temperature Measurement @ Dry Bulb

Average Measured Temperature (°C)	Average Displayed of UUC (°C)	Correction Measured of UUC (°C)	Expanded Uncertainty of Measurement (± °C)
19.9	20.1	-0.2	0.50
30.0	30.0	0.0	0.50
40.1	39.9	0.2	0.50

Request No. 22-66 / 0323

MTC No. PSL-H 0149 / 66

Results of Calibration :-

Table : Temperature Measurement @ Globe Bulb

Average Measured Temperature (°C)	Average Displayed of UUC (°C)	Correction Measured of UUC (°C)	Expanded Uncertainty of Measurement (± °C)
20.0	20.4	-0.4	0.50
30.0	30.0	0.0	0.50
40.1	39.6	0.5	0.50

- Note :**
1. This calibration was done without removing reservoir cover, white plates and blackened copper sphere of the instrument.
 2. The calibration data for instrument in this report is reported within the condition existing at the time of measurement only.

...end of certificate...

ภาคผนวกที่ 6-6
เอกสารสอบเทียบคุณภาพน้ำทิ้ง

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964 5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 65-420108-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co.,Ltd.

14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : pH 700

Range : N/A

pH

Resolution : 0.01 pH

Serial No. : 2841305

ID No. : LAB-PH-002

Electrode

Model : N/A

Serial No. : 3093341

Environment : On site calibration was carried out at the Laboratory Pacific Laboratory Co.,Ltd.

Ambient Temperature : (25.2 to 25.8)°C

Relative Humidity : (50 to 55) %

Date of Received : 17 December 2022

Date of Calibration : 17 December 2022

Date of Issue : 19 December 2022

Calibrated by : Bunjerd Masri

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00473/64	27 Aug 2023	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61235182	857394	11 Dec 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61267169	857395	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61260481	857396	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



Certificate of Calibration

Certificate No. : 65-420108-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (\pm mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.5	0.0	0.12
	0.0000	7	7.00	0.0	0.0	0.086
	-177.4800	10	10.00	-177.5	0.0	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (\pm pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

Signature



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. : 65-400648-1

Page : 1 of 2

Submitted by : Pacific Laboratory Co., Ltd.
14/5358 Moo 14, T. Bang Bua Thong, A. Bang Bua Thong, Nonthaburi 11110 Thailand

Equipment : Digital Thermometer with Thermistor probe
Temperature Indicator
Manufacturer : Eutech Model : pH 700
Range : N/A °C Resolution : 0.1 °C
Serial No. : 2841305 ID No. : LAB-PH-002
Thermistor probe
Model : N/A Sheath Material : Stainless
Diameter : 3 mm. Length : 115 mm.
Serial No. : PI1STEMB01P 049 ID No. : LAB-PH-002

Environment : On site calibration was carried out at the Laboratory, Pacific Laboratory Co., Ltd

Ambient Temperature : (25.2 to 25.8) °C
Relative Humidity : (50 to 55) %
Line Voltage : (220.0 to 222.0) VAC

Date of Received : 17 December 2022

Date of Calibration : 17 December 2022

Date of Issue : 19 December 2022

Calibrated by : Bunjerd Masri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400002	TT-0074-22	20 Jun 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400033	22E569	22 Feb 2024	National Institute of Metrology Thailand (NIMT)

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Northaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cali@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 65-400648-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
115	25.003	24.9	0.1	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

~*~





CERTIFICATE No : 22M8888
REFERENCE No : 66223-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SHIMADZU
MODEL : AF225WD
SERIAL No : D316301828
ID No : LAB-BL-003
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : PACIFIC LABORATORY CO., LTD.
14/5358 MOO. 14 TAMBOL BANGBUA THONG
AMPHOE BANG NUA THONG, NONTABURI
11110

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 01-Aug-22

APPROVED BY : 

ISSUED DATE : 02-Aug-22

RECEIVED DATE : 01-Aug-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 22M8888

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : AF225WD
MANUFACTURER : SHIMADZU S/N : D316301828
ID No : LAB-BL-003 RECEIVED DATE : 01-Aug-22
AIR PRESSURE : 1005mbar \pm 1mbar CALIBRATION DATE : 01-Aug-22
AMBIENT TEMPERATURE : 25°C \pm 1°C RELATIVE HUMIDITY : 56%RH \pm 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING WEIGHT OF QUALITY CALIBRATION TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23
2) STANDARD WEIGHT	E2	15843	C02210419	10-Feb-23
3) STANDARD WEIGHT	E2	QK-I-349	M2103235S	26-Mar-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000045 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.000	0.0000	0.0000	0.000075
0.001	0.0010	0.0000	0.000075
0.010	0.0100	0.0000	0.000075
0.050	0.0500	0.0000	0.000076
0.100	0.1000	0.0000	0.000075
1.000	1.0000	0.0000	0.000077
2.000	2.0000	0.0000	0.000077
5.000	5.0000	0.0000	0.000079
20.000	20.0000	0.0000	0.000086
50.000	50.0000	0.0000	0.00011
100.000	100.0001	-0.0001	0.00019
150.000	150.0001	-0.0001	0.00026
200.000	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTI
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

F-G



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkac, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com



CERTIFICATE No : 22T8890
REFERENCE No : 66223-4

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : INCUBATOR
MANUFACTURER : AQUA LYTIC
MODEL : TC135S
SERIAL No : 0614/000033
ID No : LAB-IB-001
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : PACIFIC LABORATORY CO., LTD.
14/5358 MOO. 14 TAMBOL BANGBUA THONG
AMPHOE BANG NUA THONG, NONTHABURI 11110

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 01-Aug-22

APPROVED BY : _____

ISSUED DATE : _____

RECEIVED DATE : _____

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22T8890

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : INCUBATOR
MANUFACTURER : AQUA LYTIC
MODEL : TC135S
ID No : LAB-IB-001
RECEIVED DATE : 01-Aug-22
AMBIENT TEMPERATURE : 26 °C ± 1 °C
S/N : 0614/000033
CALIBRATION DATE : 01-Aug-22
RELATIVE HUMIDITY : 53 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOCOUPLE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT

MODEL

SERIAL No

CERTIFICATE No

DUE DATE

1) DATA LOGGER WITH TC TYPE K

HYDRA 2635A


8009008

22T7512

05-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

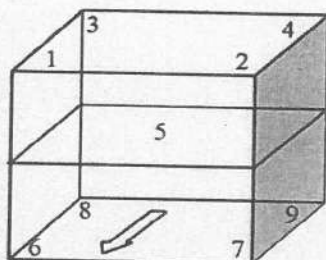

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 7

Overall Line Voltage (V) variation : 10

Instrument Condition : Normal

CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
20.0	20.0	0.63	0.48	1.43

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (±°C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
20.0	20.0	20.07	20.08	20.07	20.07	20.11	20.07	20.01	19.96	19.83	0.91

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 22T8889

REFERENCE No : 66223-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : HOT AIR OVEN

MANUFACTURER : MEMMERT

MODEL : UN55

SERIAL No : B214.1879

ID No : LAB-OV-001

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : PACIFIC LABORATORY CO., LTD.
14/5358 MOO. 14 TAMBOL BANGBUA THONG
AMPHOE BANG NUA THONG, NONTHABURI 11110

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 01-Aug-22

APPROVED BY :

ISSUED DATE : 02-Aug-22

RECEIVED DATE : 01-Aug-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22T8889

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : MEMMERT
MODEL : UN55
ID No : LAB-OV-001
RECEIVED DATE : 01-Aug-22
AMBIENT TEMPERATURE : 26 °C ± 1 °C

S/N : B214.1879
CALIBRATION DATE : 01-Aug-22
RELATIVE HUMIDITY : 53 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOCOUPLE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-


INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7903007	22T7512	05-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

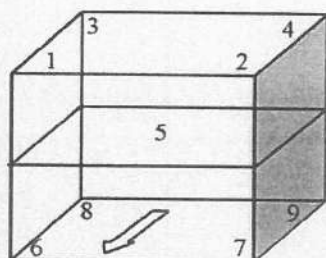

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 0
Overall Line Voltage (V) variation : 10
Instrument Condition : Normal
Chamber Size (W*L*H): 40*33*40 cm

CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.0	0.41	1.27	1.41
180.0	180.0	0.67	2.27	2.44

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (±°C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.09	103.96	103.60	103.84	103.93	103.57	103.64	103.15	103.76	0.83
180.0	180.0	179.96	179.74	179.20	179.71	180.02	179.24	179.40	178.55	179.70	1.2

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com



CERTIFICATE No : 22T8896
REFERENCE No : 66224-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : WATER BATH
MANUFACTURER : MEMMERT
MODEL : WNB22
SERIAL No : L514.0184
ID No : LAB-WB-001
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : PACIFIC LABORATORY CO., LTD.
14/5358 MOO. 14 TAMBOL BANGBUA THONG
AMPHOE BANG NUA THONG, NONTHABURI 11110

CALIBRATED BY : CHAICHARN CH.
CALIBRATION DATE : 01-Aug-22

APPROVED BY : _____
ISSUED DATE : _____
RECEIVED DATE : _____

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkoe, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 22T8896

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : WATER BATH
MANUFACTURER : MEMMERT
ID NUMBER : LAB-WB-001
RECEIVED DATE : 01-Aug-22
AMBIENT TEMPERATURE : 29 °C ± 1 °C
MODEL : WNB22
SERIAL NUMBER : L514.0184
CALIBRATION DATE : 01-Aug-22
RELATIVE HUMIDITY : 53 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO ASTM E715-80 (REAPPROVED 2001) BY COMPARISON WITH CALIBRATED RTD. THE PROBES WERE PLACED ON FIVE POINTS AND LOCATED ONE PROBE IN EACH OF THE FOUR CORNERS OF THE BATH AND PLACED THE FIFTH RTD WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE WATER VOLUME (REFERENCE LOCATION) UNDER NO LOAD CONDITION.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	2625A	6603614	22T7514	05-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

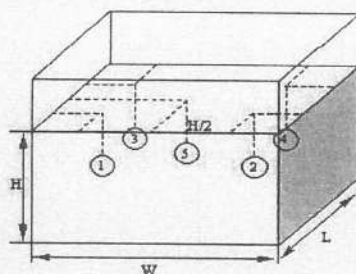

PROBE INSTALLATION
POSITION IN THE BATH

GENERAL INFORMATION

Overall Variation of Ambient Temperature around the Bath (°C) : 1.5

Overall Variation of Line Voltage (V) : 11

Instrument Condition : Normal

BATH PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
85.0	85.0	0.16	0.12	0.33
95.0	95.0	0.17	0.09	0.35

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations					Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	
85.0	85.0	84.71	84.72	84.66	84.70	84.77	0.23
95.0	95.0	94.71	94.71	94.72	94.66	94.75	0.24

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE BATH.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



Certificate of Calibration

Equipment:	SPECTROPHOTOMETER	Certificate No.:	C06220575
Model:	DR1900	Issued Date:	10 November 2022
Serial No. (or ID.):	141350001007	Job No.:	KSPR2214072
Manufacturer:	HACH	Page:	1 of 2
Condition:	In Condition		

Customer: Pacific Laboratory Co., Ltd.
14/5358 Moo 14, T. Bang Bua Thong,
A. Bang Bua Thong, Nonthaburi 11110 Thailand

Environment Condition:

Temperature	23	°C	±	2	°C
Humidity	50	%RH	±	15	%RH

Calibration Place: Environment Laboratory, DKSH Technology Limited.
2533 Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Mr.Wasan Nuchnabee

Calibration Date: 10 November 2022

The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04

Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 97349 and 97350

The standard for Photometric Certificate No. 9112739

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางนา เขตคลองเตย กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:
Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 5 nm and UUC at 5 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
361.40	360	1.40	0.59
418.40	417	1.40	0.59
537.00	537	0.00	0.59
638.00	637	1.00	0.59
747.61	747	0.61	0.59

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.2899	0.283	0.0069	0.0045
	0.5170	0.509	0.0080	0.0045
	1.0286	1.020	0.0086	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2837	0.279	0.0047	0.0045
	0.5074	0.503	0.0044	0.0045
	1.0071	1.000	0.0071	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2487	0.243	0.0057	0.0045
	0.4593	0.456	0.0033	0.0045
	0.9322	0.929	0.0032	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2434	0.241	0.0024	0.0045
	0.4649	0.463	0.0019	0.0045
	0.9457	0.944	0.0017	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2570	0.254	0.0030	0.0045
	0.5035	0.501	0.0025	0.0045
	1.0022	1.000	0.0022	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2560	0.252	0.0040	0.0045
	0.4968	0.493	0.0038	0.0045
	0.9713	0.969	0.0023	0.0045

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

DKSH Technology Limited

2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260

2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

The End of Certificate



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484

Cert. No.: 23LM28

Page.: 1 of 3

Certificate of Calibration

Equipment : COD Tester

Manufacturer : Hanna

Model : HI839800-02

Serial No. : 04500100101

ID No. : LAB-CD-002

Submitted by : Pacific Laboratory Co.,Ltd.
14/5358 Moo 14 Tambol Bang Bua Thong,
Amphoe Bang Bua Thong,
Nonthaburi 11110

Location : TPA Calibration Lab.

Received Order : 16 February 2023

Calibration Date : 2 March 2023

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

Approved by :

() Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date : 9 March 2023

The Uncertainties are for a confidence probability of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration and Testing Equipment Services.

A 0010656



Equipment : COD Tester
 Condition As-Received : Used Item
 Reference : 2302-0617WN-1
 Procedure Used :-

Cert. No.: 23LM28
 Page.: 2 of 3

As agreed with customer the calibration was perform using in-house calibration method according to directed measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44073381	22LM78/1	12 May 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Alumina (Alumium Hydroxide)

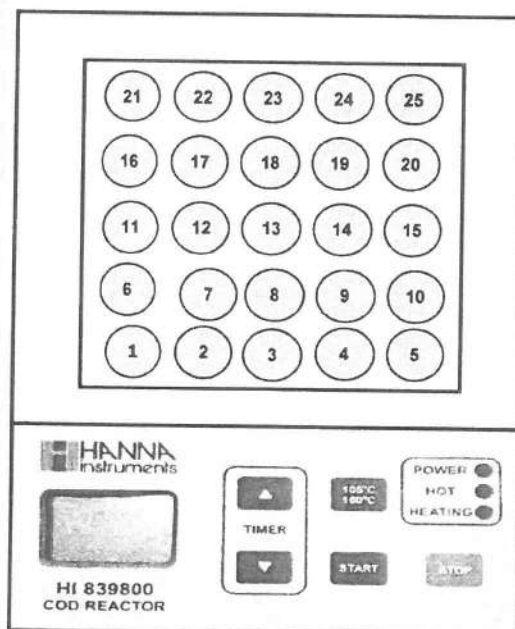

Top View

Environment during calibration		
	Beginning	End
Temp.(°C)	25	24
REL.Humi.(%)	50	51
AC Supply (Volt)	220	221

Position :	21	22	23	24	25
Ref. Std./ID No.:	20-01TC-01	20-01TC-02	20-01TC-03	20-01TC-04	20-01TC-05
Position :	16	17	18	19	20
Ref. Std./ID No.:	20-01TC-06	20-01TC-07	20-01TC-08	20-01TC-09	20-01TC-10
Position :	11	12	13	14	15
Ref. Std./ID No.:	20-01TC-01	20-01TC-02	20-01TC-03	20-01TC-04	20-01TC-05
Position :	6	7	8	9	10
Ref. Std./ID No.:	20-01TC-06	20-01TC-07	20-01TC-08	20-01TC-09	20-01TC-10
Position :	1	2	3	4	5
Ref. Std./ID No.:	20-01TC-01	20-01TC-02	20-01TC-03	20-01TC-04	20-01TC-05

Malu.



Equipment : COD Tester
Condition As-Received : Used Item
Reference : 2302-0617WN-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Calibration Point : 150.0 °C

Cert. No.: 23LM28
Page.: 3 of 3

UUC* Setting (°C)	UUC* Reading (°C)	Measured Temperature (°C)					Stability (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
		Position							
150.0	150.0	21	22	23	24	25	0.29	1.1	2
		149.730	149.845	149.279	150.508	149.119			
		16	17	18	19	20			
		150.048	150.313	151.045	150.224	149.083			
		11	12	13	14	15			
		150.084	149.769	151.078	150.483	149.028			
		6	7	8	9	10			
		149.912	150.324	150.448	151.155	149.947			
		1	2	3	4	5			
		150.101	149.921	149.923	150.488	149.366			

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-