

ภาคผนวก ค : เอกสารสอบเทียบความถูกต้อง
ของเครื่องมือเก็บตัวอย่าง

CERTIFICATE OF ANALYSIS

EPA PROTOCOL GAS

Cylinder No. : EB0062815

CERTIFICATE OF ANALYSIS Grade of Product: EPA Protocol

Part Number: E04N199E15ACX9C Reference Number: 82-401135335-1
Cylinder Number: EB0062815 Cylinder Volume: 144.4 CF
Laboratory: 124 - Riverton (SAP) - NJ Cylinder Pressure: 2015 PSIG
PGVP Number: B52018 Valve Outlet: 660
Gas Code: CO,NO,NOX,S02,BALN Certification Date: Mar 13, 2018
Expiration Date: Mar 13, 2026

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS				
Component	Requested Concentration	Actual Concentration	Protocol Method	Assay Dates
NOX	50.00 PPM	50.55 PPM	G1	03/06/2018, 03/13/2018
NITRIC OXIDE	50.00 PPM	50.50 PPM	G1	03/06/2018, 03/13/2018
SULFUR DIOXIDE	50.00 PPM	51.01 PPM	G1	03/06/2018, 03/13/2018
CARBON MONOXIDE	2000 PPM	1977 PPM	G1	03/06/2018
NITROGEN	Balance			

CALIBRATION STANDARDS		
Type	Cylinder No	Expiration Date
NTRM	15060607	
PRM	12367	
GRS	0315201604	
NTRM	16011025	
NTRM	12060735	

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 APW1100391 CO	FTIR	Feb 08, 2018
Nicolet 6700 APW1100391 NO	FTIR	Feb 15, 2018
Nicolet 6700 APW1100391 NO2	FTIR	Feb 16, 2018
Nicolet 6700 APW1100391 SO2	FTIR	Mar 01, 2018

Triad Data Available Upon Request

NOTES:NET WEIGHT: 10.43lbs
GROSS WEIGHT: 60.93lbs
PO# 5218000763

This calibration std. has been certified in accordance with the May 2012 EPA Traceability Protocol, Document EPA-600/R-12/531. All testing processes and measurements conform to the requirements of ISO/IEC 17025 and to Airgas ISO 9001:2000 and relate only to items identified on this certificate. All gases are certified to be NIST Traceable with total uncertainty as detailed under Analytical Uncertainty. This document shall not be reproduced in full without written approval of the issuer.



TESTING CERT No. 3082.05

Don Moran
Approved for Release

SOUND LEVEL CALIBRATOR

MODEL : NC-75

SERIAL No. : 34802645



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0021 MTC No. EEL. BP. 35/1065

CALIBRATION CERTIFICATE

Submitted by : Eastern Thai Consulting 1992 Co., Ltd.
Address : 683 Moo 11 Sukaphai Rd., Nongkham, Sriracha, Chonburi 20230.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :
Description : Sound Calibrator : Temperature : $(23 \pm 3) ^\circ\text{C}$
Manufacturer : Rion : Relative Humidity : $(50 \pm 15) \%$
Model : NC-75 : Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$
Serial No. : 34802645

Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Brüel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tanagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
7. Condenser Microphone B&K 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942:2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 10 Oct. 2022

Date of Calibration : 18 Oct. 2022

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office : 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000 Fax (66) 0 2577 9000
Office : 196 Phahonyothin Road, Chatuchak Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217 Fax (66) 0 2579 8592

FMBL/MTC.002 Rev.



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0021 MTC No. EEL. BP. 35/1065

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = $94 \text{ dB re } 20 \mu\text{Pa at } 1000 \text{ Hz}$

Acoustic Output in dB re $20 \mu\text{Pa}$, Corrected to Reference Conditions : 101.325 kPa , 23.0°C and $50 \% \text{RH}$

1. Sound Pressure Level

Standard Microphone	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit
Type	1/2 inch Brüel&Kjaer 4180	93.98	-0.02	± 0.10
				IEC60942:2003 Class 1

2. Frequency

Standard Microphone	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit
Type	1/2 inch Brüel&Kjaer 4180	1000.0	0.0	± 1.5
				$\pm 1.0\%$

3. Total distortion

Standard Microphone	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit
Type	1/2 inch Brüel&Kjaer 4180	0.30	± 0.50
			$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

Approved by :

(Mr. Weerachai Deechaiyai)



Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 18 Oct. 2022

Date of Issue : 19 Oct. 2022

Ref : 2011265101004372001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office : 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000 Fax (66) 0 2577 9000
Office : 196 Phahonyothin Road, Chatuchak Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217 Fax (66) 0 2579 8592

FMBL/MTC.002 Rev.

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 01120947

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sinitthorn Rd, Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



NSC-TSI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL23098

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 01120947 / 21960 / 22336
ID No.:

Condition As Found : GOOD
Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 24 JANUARY 2023
Calibration Date : 26-30 JANUARY 2023
Date of Issue : 01 FEBRUARY 2023

Calibrated by : Nathakorn Pisutpaian

Approved by : 
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	BEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	BEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	BEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY



Continuation of Calibration Certificate

Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

COPY

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	9.9
C - weight	15.5
Flat	21.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.2	0.2	0.2
1000	0.1	0.1	0.1
8000	-0.4	-0.4	-0.3
			Acceptance Limits
			± 1.0
			± 0.7
			+ 1.5, - 2.5

COPY

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
63	0.0	0.0	±1.0
125	0.0	0.0	±1.0
250	0.0	0.0	±1.0
500	0.0	0.0	±1.0
1000	0.0	0.0	±1.0
2000	0.0	0.0	±1.0
4000	0.0	0.0	±1.0
8000	0.0	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	+ 2.5, -16.0

20

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

Continuation of Calibration Certificate

Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.1	0.1	±0.8
84.0	84.1	0.1	±0.8
79.0	79.0	0.0	±0.8
74.0	74.1	0.1	±0.8
69.0	69.1	0.1	±0.8
64.0	64.0	0.0	±0.8
59.0	59.1	0.1	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.0	0.0	±0.8
29.0	29.0	0.0	±0.8
28.0	28.0	0.0	±0.8
27.0	27.0	0.0	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.9	-0.1	±0.8

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.2	-0.2	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 8 of 8

11. Overload indication

Measured value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	
89.6	89.5	-0.1
		±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 00230992

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

MTC No. EEL. BP. 154/0266

Request No. 21-66/0343

CALIBRATION CERTIFICATE

Submitted by : Eastern Thai Consulting 1992 Co., Ltd.
Address : 683 Moo 11 Sukhapibam 8 Rd., Nongkham, Sriracha, Chonburi 20230.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan. 10280.

Instrument Calibrated :
Description : Sound Level Meter
Manufacturer : Rion
Model : NL-52A
Serial No. : 00230992
Microphone : Type UC-59 No.22769
Preamplifier : Type NH-25 No.22423

Ambient Environment
Temperature : $(23 \pm 3) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$
Ambient Pressure : $(101.325 \pm 1.5) \text{ kPa}$

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator An30 AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 27 Feb. 2023

Date of Calibration : 21-23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand Tel. (66) 0 2577 9000 Fax. (66) 0 2577 9009	Office/Laboratory Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand Tel. (66) 0 2323 1672-80 ext. 115, 116 Fax. (66) 0 2323 9165	Office 196 Phahonyothin Road, Chatuchak Bangkok 10900, Thailand Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217 Fax. (66) 0 2579 8592 E-mail : sumalee@tistr.or.th
--	---	---

FM.BL.MTC.002 Rev.4

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

MTC No. EEL. BP. 154/0266

Request No. 21-66/0343

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
11. Digital Multimeter Agilent 34401A S/N MY44005560.
12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 21-23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand Tel. (66) 0 2577 9000 Fax. (66) 0 2577 9009 E-mail : sumalee@tistr.or.th	Office/Laboratory Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand Tel. (66) 0 2323 1672-80 ext. 115, 116 Fax. (66) 0 2323 9165	Office 196 Phahonyothin Road, Chatuchak Bangkok 10900, Thailand Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217 Fax. (66) 0 2579 8592 E-mail : sumalee@tistr.or.th
--	---	---

FM.BL.MTC.002 Rev.4

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class I (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
113.89	114.0	113.9	0.0	0.7	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 123.9 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
20.8	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	10.8	0.10	N/A
C-Weight	15.2	0.10	N/A
Flat	20.8	0.10	N/A

Date of Calibration : 21-23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FVBLMTC.002 R

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpal@tistr.or.th Website: www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mt@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)		Acceptance limit class I (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight			
125	0.4	0.5	±1.0	0.45	0.6
1 000	-0.2	-0.2	±0.7	0.45	0.6
8 000	-1.2	-1.2	+1.5; -2.5	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)		Acceptance limit class I (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight			
63	-0.1	0.0	±1.0	0.20	0.6
125	-0.1	0.0	±1.0	0.20	0.6
250	-0.1	0.0	±1.0	0.20	0.6
500	0.0	0.0	±1.0	0.20	0.6
1 000	0.0	0.0	±0.7	0.20	0.6
2 000	0.0	0.1	±1.0	0.20	0.6
4 000	0.0	0.0	±1.0	0.20	0.6
8 000	0.1	0.1	+1.5; -2.5	0.20	0.7
16 000	-1.3	-1.3	+2.5; -16.0	0.20	0.7

Date of Calibration : 21-23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FVBLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpal@tistr.or.th Website: www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mt@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.1	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Weighting					
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Weighting					
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
137	137.1	0.1	0.8	0.30	0.3
136	136.1	0.1	0.8	0.30	0.3
135	135.1	0.1	0.8	0.30	0.3
134	134.1	0.1	0.8	0.30	0.3
133	133.0	0.0	0.8	0.30	0.3
132	132.0	0.0	0.8	0.30	0.3
131	131.0	0.0	0.8	0.30	0.3
130	130.0	0.0	0.8	0.30	0.3
129	129.0	0.0	0.8	0.30	0.3
124	124.0	0.0	0.8	0.30	0.3
119	119.0	0.0	0.8	0.30	0.3
114	114.0	0.0	0.8	0.30	0.3
109	109.0	0.0	0.8	0.30	0.3
104	104.0	0.0	0.8	0.30	0.3
99	99.0	0.0	0.8	0.30	0.3
94	94.0	0.0	0.8	0.30	0.3
89	89.0	0.0	0.8	0.30	0.3
84	84.0	0.0	0.8	0.30	0.3
79	79.1	0.1	0.8	0.30	0.3

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class I ($\pm$ dB)	Uncertainty ($\pm$ dB)	Maximum-permitted uncertainty of measurement ($\pm$ dB)
74	74.0	0.0	0.8	0.30	0.3
69	69.0	0.0	0.8	0.30	0.3
64	64.0	0.0	0.8	0.30	0.3
59	59.0	0.0	0.8	0.30	0.3
54	53.9	-0.1	0.8	0.30	0.3
49	49.0	0.0	0.8	0.30	0.3
44	43.9	-0.1	0.8	0.30	0.3
39	39.0	0.0	0.8	0.30	0.3
34	34.0	0.0	0.8	0.30	0.3
29	28.9	-0.1	0.8	0.30	0.3
28	28.0	0.0	0.8	0.30	0.3
27	27.0	0.0	0.8	0.30	0.3
26	26.0	0.0	0.8	0.30	0.3
25	24.9	-0.1	0.8	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	0.8	0.00	0.3

Date of Calibration : 21-23 Mar. 2023

Date of Calibration : 21-23 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

The results relate only to the items tested/calibrated or value assigned.

The results relate only to the items tested/calculated or value assigned.

The results relate only to the items tested/calculated or value assigned.

FM.BLMTC 002 Rev.

EM-BL-MTC-002 Rev.4

Lead Office

Office/Laboratory

Lead Office	Office/Laboratory	Office
15 Mu. 3 Tambon Khlong Ha, Amphoe Khlong Luang	Sol. 1C Bannon Industrial Estate Sukhumvit Road	196 Phatonyotin Road, Chatuchak Bangkok 10900.

Office

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,

hangewat Pathumthani

12120, Thailand

Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Thailand

Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

ax. (66) 0 2577 9009

Fax: (66) 0 2577 9009
 Fax: (66) 0 2577 9009
 E-mail: sunumalee@listroth
 E-mail: sunumalee@listroth

Fax: (603) 883-2222

Fax: (66) 0 2579 8592
E-mail: sunelee@tiscor.th



NSC-TISI-TIS 17025
CALIBRATION 0037



NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

MTC No. EEL BP. 154/0266

Request No. 21-66/0343

10. Peak C sound level


Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.4	0.0	2.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	1.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	1.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle					
136.5		0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 1 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.1	0.10	0.1
End	129.0				

Calibrated by : 
(Mr. Pannasit Phasingsti)

Approved by :

(Mr. Prawate Klungsap)

Director

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 21-23 Mar. 2023

Date of Issue : 23 Mar. 2023

Ref : 2011266022700825007

End of Certificate

9 /

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Re

Head Office
15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Bangkok 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak Bangkok 1090
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 01120945

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirthorn Rd, Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



Cert. No. : ACL23096
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preampifier NH-25
Serial No.: 01120945 / 21951 / 22334
ID No.:

Condition As Found :

GOOD

Customer :

EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :

Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date :

24 JANUARY 2023

Calibration Date :

26-30 JANUARY 2023

Date of Issue :

01 FEBRUARY 2023

Calibrated by :

Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23096
Job No. : VC66AC0035
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

T. Petchurai

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

COPY

7. Reth...

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	9.9
C - weight	14.9
Flat	20.5

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.2	0.2	0.2
1000	0.1	0.1	0.1
8000	0.0	0.0	0.0
			Acceptance Limits
			± 1.0
			± 0.7
			+ 1.5, - 2.5

COPY

7. Reth...

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	-0.1	0.0	0.0
125	0.0	0.0	0.0
250	0.0	0.0	0.0
500	0.0	0.0	0.0
1000	0.0	0.0	0.0
2000	0.0	0.1	0.0
4000	0.0	0.0	0.0
8000	0.0	0.1	0.1
16000	0.0	-1.2	-1.2
			Acceptance Limits
			±1.0
			±1.0
			±1.0
			±1.0
			±1.0
			±1.0
			±1.0
			+1.5, -2.5
			+2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A-weight	94.0	0.0	-
C-weight	94.0	0.0	±0.2
Flat	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	±0.1
Leq	94.0	0.0	±0.1

6. Long-term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A-weight	94.0	94.0	0.0	±0.1

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	29.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8
28.0	28.0	0.0	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.8	-0.2	±0.8

Cert. No. : ACL23096
Job No. : VC66AC0035
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.1	-0.3	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

COPY

T. Petch...

Cert No. : ACL23096
Job No. : VC66AC0035
Pages : 8 of 8

11. Overload indication

Measured value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	89.5	0.0
Negative one-half cycle	89.5	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A-weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

T. Petch...

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 01120944



SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru,Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com

NEC-TS12-TIS 17025
CALIBRATION 0394

Cert. No. : ACL23095
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 01120944 / 21950 / 22333
ID No.:

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 24 JANUARY 2023
Calibration Date : 26-30 JANUARY 2023
Date of Issue : 01 FEBRUARY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

SITHIPORN SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23095
Job No. : VC66AC0035
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY532220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

T. Petchurai

Continuation of Calibration Certificate

Cert. No. : ACL23095
Job No. : VC66AC0035
Pages : 3 of 8Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL23095
Job No. : VC66AC0035
Pages : 4 of 8Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	9.9
C - weight	15.2
Flat	20.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.2	0.2	0.2
1000	0.1	0.1	0.1
8000	-0.4	-0.3	-0.3
			Acceptance Limits
			± 1.0
			± 0.7
			+ 1.5, - 2.5

Continuation of Calibration Certificate

Cert. No. : ACL23095
Job No. : VC66AC0035
Pages : 5 of 8Cert. No. : ACL23095
Job No. : VC66AC0035
Pages : 6 of 84. Electrical signal tests of frequency weightings
Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Limits
63	0.0	0.0	-0.1
125	0.0	0.0	0.0
250	0.0	0.0	0.0
500	0.0	0.0	0.0
1000	0.0	0.0	0.0
2000	0.0	0.0	0.0
4000	0.0	0.0	0.0
8000	0.0	0.0	0.0
16000	0.0	0.0	0.0

9-24

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	±0.2
Flat	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	±0.1
Leq	94.0	0.0	±0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	±0.1

QF-TS12-04-04-020664

7. Ketch

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	53.9	-0.1	±0.8
49.0	48.9	-0.1	±0.8
44.0	43.9	-0.1	±0.8
39.0	38.9	-0.1	±0.8
34.0	33.9	-0.1	±0.8
30.0	29.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8
28.0	27.9	-0.1	±0.8
27.0	26.8	-0.2	±0.8
26.0	25.8	-0.2	±0.8
25.0	24.8	-0.2	±0.8

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert No. : ACL23095
Job No. : VC66AC0035
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.3	-0.1	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

COPY

T. Reteh

Continuation of Calibration Certificate

Cert No. : ACL23095
Job No. : VC66AC0035
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	89.6	-0.2
89.8			±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

T. Reteh

ANALYTICAL BALANCE

Model : MS204TS/00

Serial No. : B904136539

Mettler-Toledo (Thailand) Ltd.
846/4 - 846/5 Lasalle Rd., Bangna Tai Sub-District
Bangna District, Bangkok 10260
+662 723 0382
MT-TH.ServiceSupport@mt.com

NSC-TISI-TIS 17025
CALIBRATION 0062

Accuracy Calibration Certificate

Customer

Company: EASTERN THAI CONSULTING 1992 CO., LTD.
Address: 683 Moo 11, Sukhaphiban 8 Rd., Nong Kham
City: Sriracha
Zip / Postal: 20230
State / Province: Chonburi
Contact: Sasiporn Nakin
Order Number: 0332630077

Weighing Device

Manufacturer: Mettler Toledo
Model: MS204TS/00
Serial No.: B904136539
Building: Laboratory
Floor: 1
Room: Balance
Instrument Type: Weighing Instrument
Asset Number: LABE 05/4
Terminal Model: N/A
Terminal Serial No.: N/A
Terminal Asset No.: N/A

2027

Procedure

Calibration Guideline: EURAMET cg-18 v. 4.0 (11/2015)
CP/W002/20
METTLER TOLEDO Work Instruction:
This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.
The sensitivity/span of the weighing instrument was adjusted before calibration with a built-in weight.
In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

As Found	Temperature		Humidity	
	Start: 25.6 °C	End: 25.2 °C	Start: 50.5 %	End: 44.8 %

As Found Calibration Date: 06-Feb-2023
As Left Calibration Date: N/A
Issue Date: 07-Feb-2023
Calibrator: Thiraphong Salanoi
Approved Signatory: [Signature]

Technical Manager / Head of Calibration Center


COPY

Measurement Results

Repeatability

Test Load: 100 g

	As Found	As Left
1	100.0002 g	N/A
2	100.0002 g	N/A
3	100.0001 g	N/A
4	100.0002 g	N/A
5	100.0002 g	N/A
6	100.0001 g	N/A
7	100.0002 g	N/A
8	100.0002 g	N/A
9	100.0001 g	N/A
10	100.0002 g	N/A
Standard Deviation	0.00005 g	N/A

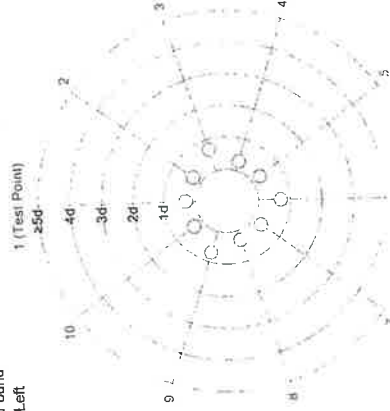


The 'd' in the graph represents the readability of the range/interval in which the test was performed.
The results of this graph are based upon the absolute values of the differences from the mean value.

Eccentricity

Test Load: 100 g

Position	As Found	As Left
1	100.0002 g	N/A
2	100.0002 g	N/A
3	100.0001 g	N/A
4	100.0001 g	N/A
5	100.0001 g	N/A
Maximum Deviation	0.0001 g	N/A




As Found

The 'd' in the graph represents the readability of the range/interval in which the test was performed.

COPY

Error of Indication

As Found		Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.0000 g	0.0000 g	0.0000 g	0.0000 g	0.11 mg	2
2	0.0100 g	0.0100 g	0.0100 g	0.0000 g	0.13 mg	2
3	0.0500 g	0.0500 g	0.0500 g	0.0000 g	0.13 mg	2
4	0.1000 g	0.0999 g	0.0999 g	-0.0001 g	0.13 mg	2
5	1.0000 g	0.9999 g	0.9999 g	-0.0001 g	0.13 mg	2
6	5.0000 g	4.9999 g	4.9999 g	-0.0001 g	0.13 mg	2
7	10.0000 g	9.9999 g	9.9999 g	-0.0001 g	0.14 mg	2
8	50.0000 g	50.0001 g	50.0001 g	0.0001 g	0.17 mg	2
9	100.0001 g	100.0002 g	100.0002 g	0.0001 g	0.24 mg	2
10	150.0001 g	150.0002 g	150.0002 g	0.0001 g	0.34 mg	2
11	200.0001 g	200.0002 g	200.0002 g	0.0001 g	0.39 mg	2

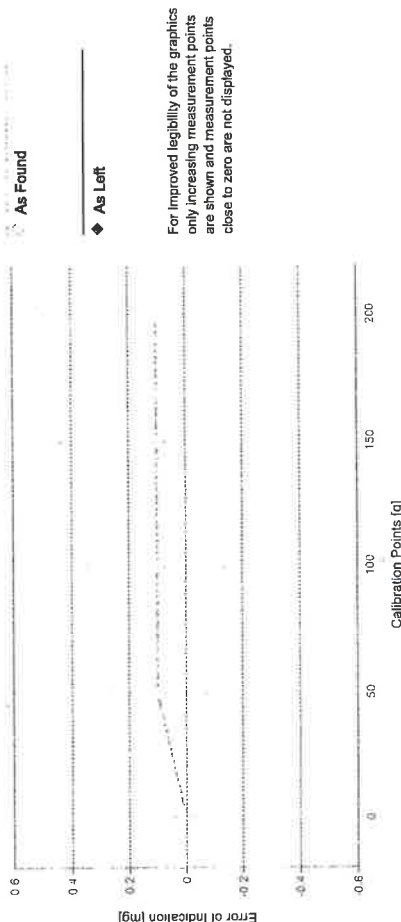

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2

Weight Set No.: WS28 Date of Issue: 01-Apr-2022
Certificate Number: 178498 Calibration Due Date: 17-Sep-2023

Thermo Hygrometer

Equipment No.: IN306 Date of Issue: 10-Jan-2023
Certificate Number: 23H4 Calibration Due Date: 03-Jan-2024

Remarks

FACT adjustment functionality activated
Equipment condition: Good
Next calibration according to customer's procedure
Calibration data not decide by calibration laboratory

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

COPY

COPY

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with $k=2$ in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use: $1.5 \cdot 10^{-6} / K$

Temperature range on site for the evaluation of the measurement uncertainty in use: 5 K


Linearization of Uncertainty Equation

d	Range		As Found	As Left
	Min	Max		
1	0.0001 g	220 g	$U_1 = 0.13 \text{ mg} + 0.00625 \text{ mg/g} \cdot R$	N/A

To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication	As Found		As Left	
	Absolute	Relative	Absolute	Relative
0.0220 g	0.13 mg	0.59%	N/A	N/A
0.2200 g	0.13 mg	0.060%	N/A	N/A
2.2000 g	0.14 mg	0.0065%	N/A	N/A
22.0000 g	0.27 mg	0.0012%	N/A	N/A
220.0000 g	1.5 mg	0.00068%	N/A	N/A

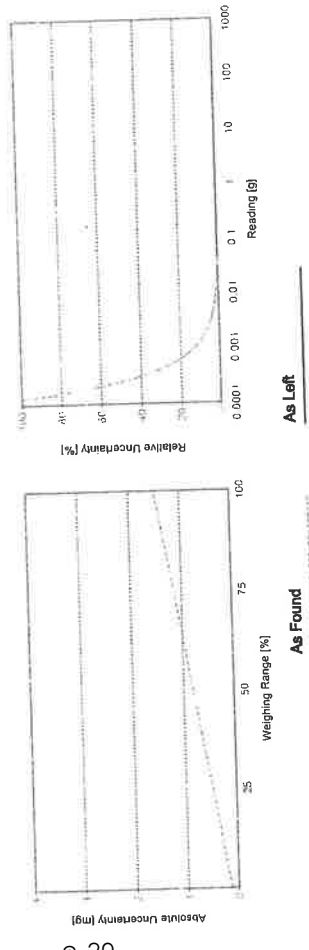

GWP®
Certificate



As Found ✓ As Left ✓

The weighing device meets the given process requirements.

The weighing device meets the given process requirements.

Tests Performed:

As Found

As Left

No adjustments/modifications made. As Left results correspond to As Found.


Process Requirements

Weighting Tolerance: 1%

Smallest Net Weight: 1.0000 g

Safety Factor: 2

Safe Weighing Range

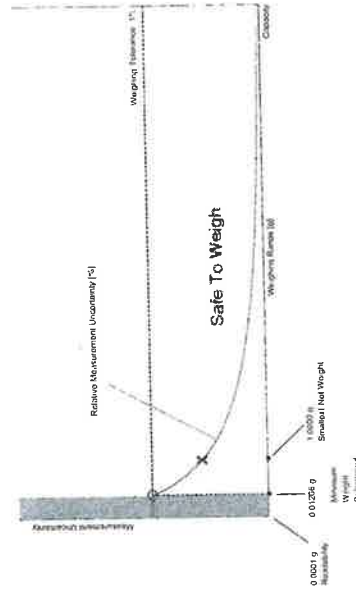

While the values in this graph reflect the actual calibration results, the measurement uncertainty curves are simply a visual representation. This graph reflects As Left testing, unless only As Found was performed.

COPY

Minimum Weight

As Found Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.12729 g	0.25618 g	0.38672 g	0.65284 g	1.34917 g
0.2%	0.06344 g	0.12729 g	0.19153 g	0.32124 g	0.65284 g
0.5%	0.02533 g	0.05072 g	0.07618 g	0.12729 g	0.25618 g
1%	0.01266 g	0.02533 g	0.03802 g	0.06344 g	0.12729 g
2%	0.00633 g	0.01266 g	0.01899 g	0.03167 g	0.06344 g
5%	0.00253 g	0.00506 g	0.00759 g	0.01266 g	0.02533 g

Pass: The determined minimum weight meets the requirement for the smallest net weight.

As Left Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.12729 g	0.25618 g	0.38672 g	0.65284 g	1.34917 g
0.2%	0.06344 g	0.12729 g	0.19153 g	0.32124 g	0.65284 g
0.5%	0.02533 g	0.05072 g	0.07618 g	0.12729 g	0.25618 g
1%	0.01266 g	0.02533 g	0.03802 g	0.06344 g	0.12729 g
2%	0.00633 g	0.01266 g	0.01899 g	0.03167 g	0.06344 g
5%	0.00253 g	0.00506 g	0.00759 g	0.01266 g	0.02533 g

Pass: The determined minimum weight meets the requirement for the smallest net weight.

At these net minimum weight values, the measurement uncertainty of the weighing device is equal to or less than 1/1 (no safety factor), 1/2, 1/3, 1/5, or 1/10 of the required tolerance. The values are calculated with $k = 2$ and based on the linear formula of the measurement uncertainty of the weighing device in use.

The safety factor for As Found is always 1. This implies no safety factor. As Found testing looks at the behavior of the instrument from the past until test occurred. For the past, it is necessary to know that the tolerance was met, but not the safety factor. The safety factor is a proactive measure to apply for future measurements.

Notes on minimum weight values in above table:

1. If "N/A" is shown above, no appropriate value could be calculated.
2. METTLER TOLEDO is not responsible for the definition of the process requirements.

COPY

Measurement Results

Results Summary

Repeatability		Eccentricity		Error of Indication	
As Found	✓	As Found	✓	As Found	✓
As Left	✓	As Left	✓	As Left	✓

- ✓ = Passed
- ✗ = Failed
- ! = Safety Factor not met

Repeatability

Test Load: 100 g

Tolerance		Control Limit		As Found		As Left	
Tolerance	Control Limit	Std. Deviation	Result	Std. Deviation	Result	Std. Deviation	Result
0.1%	0.00050 g		✓		✓		✓
0.2%	0.00100 g		✓		✓		✓
0.5%	0.00250 g		✓		✓		✓
1%	0.00500 g	0.00005 g	✓	0.00005 g	✓	0.00005 g	✓
2%	0.01000 g		✓		✓		✓
5%	0.02500 g		✓		✓		✓

The weighing tolerance is met if the standard deviation is less than or equal to the corresponding control limit

Eccentricity

Test Load: 100 g

Tolerance		Control Limit		As Found		As Left	
Tolerance	Control Limit	Std. Deviation	Result	Std. Deviation	Result	Std. Deviation	Result
0.1%	0.0500 g		✓		✓		✓
0.2%	0.1000 g		✓		✓		✓
0.5%	0.2500 g		✓		✓		✓
1%	0.5000 g	0.0001 g	✓	0.0001 g	✓	0.0001 g	✓
2%	1.0000 g		✓		✓		✓
5%	2.5000 g		✓		✓		✓

The weighing tolerance is met if the deviation is less than or equal to the corresponding control limit

COPY

Error of Indication

As Found

Reference Value	Error	Control limits for various weighing tolerances				
		0.1%	0.2%	0.5%	1%	5%
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A
50.0000 g	0.0001 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	1.2500 g
100.0001 g	0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	2.5000 g
150.0001 g	0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	3.7500 g
200.0001 g	0.0001 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓

As Left

Reference Value	Error	Control limits for various weighing tolerances				
		0.1%	0.2%	0.5%	1%	5%
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A
50.0000 g	0.0001 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	1.2500 g
100.0001 g	0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	2.5000 g
150.0001 g	0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	3.7500 g
200.0001 g	0.0001 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓

The weighing tolerance is met if the error (of indication) for each test point is less than or equal to the corresponding control limit for that particular weighing tolerance. Results at or close to the zero point cannot be assessed.

COPY

BAROMETER

Equipment : Analog Barometer

ID No. / Tag No. : BM001/41

CALIBRATION CERTIFICATE

Certificate No. : AD2205-163-0001

Date Issued : 20-May-22

Customer : Eastern Thai Consulting 1992 Co., Ltd.
 683 Moo 11 Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment : Analog Barometer

Manufacturer : Barigo
Model : -
Serial No. : -
ID No./Tag No. : BM001/41
Date Received : 12-May-22
Date Calibrated : 20-May-22
Calibrated by : Mr. Saruth Srichutikul

Calibration Method or Calibration Procedure Used

In-house method : CP-21 base on DKD-R 6-1: Edition 3 2014.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: K. Nathapong
 (Mr. Nathapong Krudaum)

Page 1 of 2



COPY

Certificate No : AD2205-163-0001
 Environment : Ambient Temperature : (25 ± 2)°C
 Relative Humidity : (50 ± 15)%RH

STD Reading hPa	UUC Reading (hPa) Before Adjusted	UUC Reading (hPa) After Adjusted	UUC Error hPa	Uncertainty ± hPa
990.00	990.0	-	0.00	0.59
1000.00	1000.0	-	0.00	0.59
1010.00	1010.0	-	0.00	0.59
1020.00	1020.0	-	0.00	0.59
1030.00	1030.0	-	0.00	0.59

STD = Standard

UUC = Unit Under Calibration

Calibrated condition :

Pressure Medium : Air : Density = 1.19 kg/m³ @ 20°C, 1 bar
 Mounting Position : Vertical
 Reference Level : at center of its dial

Description of UUC :
 Range : 955 - 1075 hPa Absolute
 Calibration Range : 990 - 1030 hPa Absolute
 Scale Interval : 1 hPa
 Resolution : 0.5 hPa Absolute

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

IRPC Certificate No. CLJ-P210086 for Reference Pressure Monitor Serial No. 1598, Due 08-Nov-22

End of Certificate

COPY

Page 2 of 2

Hot Air Oven

Model. : UM 400

Serial No. : 900982



CERTIFICATE OF CALIBRATION

Page 1 of 3

Certificate No. : 23-018635
Sample Code : 23-07651-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)
Manufacturer : Memmert
Serial No. : 900982
Date of Receipt : 21 February 2023
Model : UM 400
ID No. : LABE 17/1
Date of Calibration : 21 February 2023

Condition of Calibration

1. Environment	1.1 Ambient temperature	Maximum 31.2 °C	Minimum 28.7 °C
	1.2 Relative humidity	Maximum 50.2 %	Minimum 40.1 %
	1.3 Line voltage supplied	Maximum 223.9 VAC	Minimum 221.5 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data acquisition with sensor (RTD-PT100)	LB-DA-12 (RTD-158 to RTD-166)	22-040312	02 May 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Sarawoot Thammoo

Approved by

(Mr. Somchai Neampunt)

Scientist

Signed for Director

Issue date

24 February 2023

The uncertainties are for a confidence probability of approximately 95%.
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognised national standards and to the unit of measurement realised at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
TEL 02-516-2422 FAX 02-516-6949
Rev. 01

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date 15/10/21



REPORT OF CALIBRATION

Page 2 of 3

Certificate No. : 23-018635
Sample Code : 23-07651-001

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 ^{ref}		
85	85.0	85.0	85.18	85.04	84.62	84.82	85.03	85.04	85.00	84.96	85.08	0.25	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
85	0.07	0.49	0.68

Notes

* UUC* = Unit Under Calibration

COPY

REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 23-018635

Sample Code : 23-07651-001

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 40 cm ; D = 28 cm ; H = 39 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

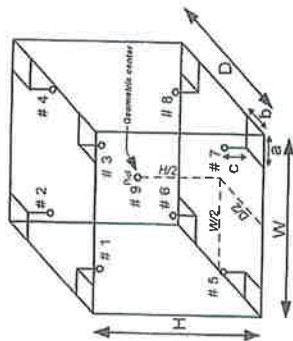


Figure: Example of sensor installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

COPY

ORIFICE TRANSFER STANDARD CERTIFICATION

WORKSHEET TE-5025A

ROOTSMETER S/N 0438320



TISCH ENVIRONMENTAL, INC.
145 SOUTH MIAMI AVE
VILLAGE OF CLEVELAND, OH
44102
613.467.9000
877.263.7810 TOLL FREE
613.467.9009 FAX

ORIFICE TRANSFER STANDARD CERTIFICATION WORKSHEET TE-5025A

Date - Mar 24, 2016 Rootmeter S/N 0438320 Ta (K) - 295
Operator Tisch Orifice I.D. - 0136 Pa (mm) - 742.95

PLATE OR Run #	VOLUME START (m3)	VOLUME STOP (m3)	DIFF VOLUME (m3)	DIFF TIME (min)	METER DIFF Hg (mm)	ORIFICE DIFF H2O (in.)
1	NA	NA	1.00	1.3400	3.2	2.00
2	NA	NA	1.00	0.9510	6.3	4.00
3	NA	NA	1.00	0.8510	7.8	5.00
4	NA	NA	1.00	0.8130	8.6	5.50
5	NA	NA	1.00	0.6690	12.6	8.00

9-38

DATA TABULATION

Vstd	(x axis) Qstd	(y axis)			(y axis)
			Va	Qa	
0.9832	0.7337	1.4054	0.9957	0.7430	0.8911
0.9791	1.0296	1.9875	0.9915	1.0426	1.2603
0.9770	1.1481	2.2221	0.9894	1.1626	1.4090
0.9760	1.2006	2.3305	0.9884	1.2157	1.4778
0.9707	1.4510	2.8107	0.9830	1.4694	1.7823
Qstd slope (m)	= 1.96262		Qa slope (m)	= 1.22896	
intercept (b)	= -0.03249		intercept (b)	= -0.02060	
coefficient (r)	= 0.99993		coefficient (r)	= 0.99993	
y axis = SQRT[H2O (Pa/760) (298/Ta)]			y axis = SQRT[H2O(Ta/Pa)]		

CALCULATIONS

Vstd = Diff. Vol [(Pa-Diff. Hg)/760] (298/Ta)
Qstd = Vstd/Time

Va = Diff Vol [(Pa-Diff Hg)/Pa]
Qa = Va/Time

For subsequent flow rate calculations:

Qstd = 1/m{ [SQRT(H2O(Pa/760) (298/Ta))] - b}
Qa = 1/m{ [SQRT H2O(Ta/Pa)] - b}

COPY

THERMO-HYGROMETER

Model : 608-H1

Serial No. : 45106737



CERTIFICATE OF CALIBRATION

Page 1 of 2
Certificate No. : 22-068062
Sample Code : 22-24591-002

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriacha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration laboratory)

Equipment : Digital thermo-hygrometer

Manufacturer : testo

Model : 608-H1

Serial No. : 45706737

ID No. : LABE 09/7

Date of Receipt : 22 June 2022

Date of Calibration : 24 June 2022

Condition of Calibration

1. Environment : 1.1 Ambient temperature : 23.0 °C ± 3.0 °C

1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

2.1 In-house method: WI-CL-045 By comparison with thermometer standard / chilled mirror hygrometer in controlled chamber.

2.2 The calibration by comparison unit under calibration (UUC) to the thermometer standard / chilled mirror hygrometer in a chamber at the controlled temperature / relative humidity.

3. Reference standard instrument

Instrument : Model : ID No. : Certificate No. : Due Date

3.1 Chilled Mirror : Optidew Vision : LB-DP-01 & LB-DP-01 (DP) : TH-0014-22 : 16 February 2023

3.2 Digital Thermometer : Optidew Vision : LB-DP-01 & LB-DP-01 (Temp.) : 22-023549 : 14 March 2023

3.3 Digital Thermometer : 34972A : LB-DA-07 with RTD-88 : 21-072473 : 13 September 2022

4. This certificate is traceable to the international system of unit (SI Unit).

4.1 Instrument No. 3.1 through National Institute of Metrology (Thailand).

4.2 Instrument No. 3.2 and 3.3 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Miss Pornsuda Lohabal : Approved by : (Mr. Somchai Neampunt)

Issue date : 27 June 2022

Scientist

Signed for Director

(Mr. Somchai Neampunt)

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

FM-CL-114

TEL 02-516-2422

FAX 02-516-6949

Rev 01

Effective Date 15/10/21

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

Effective Date 15/10/21

Rev 01

Effective Date 15/10/21

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH



REPORT OF CALIBRATION

Page 2 of 2
Certificate No. : 22-068062
Sample Code : 22-24591-002

Results of Calibration

Temperature measurement

Resolution : 0.1 °C
Range : 0 °C to 50 °C

Calibration point °C	Average of standard reading		Unit under calibration		Expanded uncertainty °C
	Controlled humidity %RH	Temperature °C	Average reading °C	Correction value °C	
20	50	20.00	20.2	- 0.20	± 0.39
25	50	25.00	24.9	+ 0.10	± 0.39
30	50	30.00	29.8	+ 0.20	± 0.39

Humidity measurement

Resolution : 0.1 %RH
Range : 10 %RH to 95 %RH

Calibration point %RH	Average of standard reading		Unit under calibration		Expanded uncertainty %RH
	Air temperature °C	Calculated humidity %RH	Average reading %RH	Correction value %RH	
45	25.00	45.13	51.4	- 6.27	± 1.3
60	25.00	60.03	66.5	- 6.47	± 1.5
75	25.00	75.20	81.5	- 6.30	± 1.7

Notes

- Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of Report -

COPY

The uncertainties are for a confidence probability of approximately 95%.
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.
This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-114
TEL 02-516-2422
FAX 02-516-6949
Rev 01
Effective Date 15/10/21
CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date 15/10/21

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-018
TEL 02-516-2422
FAX 02-516-6949
Rev 09
CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date 15/10/21

COPY

ANALYTICAL BALANCE (DU)

Model. : XS205DU

Serial No. : 1126323724

Certificate No. : 23-006683
Sample Code : 23-02820-006

Certificate No. : 23-006683
Sample Code : 23-02820-006

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siiracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : 1126323724

ID No. : LABE 05/1

Date of Receipt : 20 January 2023

Date of Calibration : 20 January 2023

Calibrated by : Mr. Thanadol Phothep
Scientist

Approved by : (Mr. Somchai Neampunt)
Signed for Director

Issue date : 25 January 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)

361 Soi Ladprao 122, Ladprao Road,
Phiephla, Wang Thonglang, Bangkok 10310

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21

TEL 02-516-2422
FAX 02-516-6949
Rev.05

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : METTLER TOLEDO
Model : XS205DU
Capacity : Max 81 g / 220 g
Resolution : 0.01 mg / 0.1 mg
Serial No. : 1126323724
ID No. : LABE 05/1

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 80	Before adjustment	After adjustment
☒ No adjustment	Nominal value	40	90
☐ Adjustment	Standard weight	40.000042	60.000045
	Average reading of indicator	40.000015	90.000019
	Standard deviation	0.000004	0.000007
Unit : g	Range : 200	Before adjustment	After adjustment
☒ No adjustment	Nominal value	100	200
☐ Adjustment	Standard weight	100.000022	200.000019
	Average reading of indicator	100.00001	200.00004
	Standard deviation	0.000004	0.000008

COPY

361 Soi Ladprao 122, Ladprao Road,
Phiephla, Wang Thonglang, Bangkok 10310

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21

TEL 02-516-2422
FAX 02-516-6949
Rev.03



Certificate No. : 23-006683

Sample Code : 23-02820-006

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g		Range : 200	
Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	0.99800	0	0.9980
40	0.99800	100	0.9980
80	0.99800	200	0.9980

3. Departure of indication from nominal value, Linearity

Unit : g					
Nominal	Standard	Average Reading	Correction	Expanded	Coverage
Value	Value	of Indicator	Value	Uncertainty	Factor (k)
Unload	0.0000000	0.00000	0.00000	0.0000090	2.01
0.01	0.0100036	0.01000	0.00000	0.0000093	2.01
0.1	0.1000062	0.10000	0.00001	0.000012	2.00
1	1.0000036	1.00001	-0.00001	0.000014	2.00
5	5.0000044	5.00003	-0.00003	0.000020	2.00
10	10.0000000	10.00007	-0.00007	0.000032	2.00
20	20.0000016	20.00011	-0.00009	0.000036	2.00
50	50.0000029	50.00013	-0.00010	0.000067	2.00
100	100.0000022	100.00001	-0.00001	0.00016	2.00
150	150.0000051	150.00001	0.00000	0.00023	2.00
200	200.0000199	200.00003	-0.00001	0.00028	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY



Certificate No. : 23-006683

Sample Code : 23-02820-006

REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan ☐ Circle ☐ Triangular ☒ Rectangular
Test weight : 50 and 100
Unit : g

Range	Position	Reading of indicator	Reading of indicator
1	50.00014	100.0001	100.0001
2	50.00014	99.9998	99.9998
3	50.00006	100.0000	100.0000
4	50.00010	100.0001	100.0001
5	50.00017	100.0001	100.0001
6	50.00014	100.0001	100.0001
Maximum difference	0.00008	0.00003	0.00003

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : -

- Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument :
1) STANDARD WEIGHT 1 mg to 1 kg

Class : E2
ID No. : LB-WE-57
Certificate No. : 22-060639

Due Date :
27 June 2023

Amiient conditions	Min	Max
Temperature (°C)	21.3	22.4
Relative Humidity (%Rh)	38.2	40.4
Air Pressure (hPa)	1008.4	1010.1

- End of Report -

CERTIFICATE OF ANALYSIS

EPA PROTOCOL GAS

Cylinder No. : EB0145030

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E03N199E15AC0U4
Cylinder Number: EB0145030
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12021
Gas Code: CH4,PPN,BALN
Reference Number: 160-40224242-1
Cylinder Volume: 144.4 CF
Cylinder Pressure: 2015 PSIG
Valve Outlet: 350
Certification Date: Oct 15, 2021
Expiration Date: Oct 15, 2023

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)", document EPA-000R-12/201, using the assay procedures listed. Analytical Methodology does not require correction for analytical interferences. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
METHANE	180.0 PPM	177.0 PPM	G1	+/- 1.0% NIST Traceable	10/15/2021
PROPANE	185.0 PPM	187.0 PPM	G1	+/- 1.0% NIST Traceable	10/15/2021
NITROGEN	Balance				
CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
FORM	08011503	K002564	246.7 PPM METHANE/AIR	+/- 0.6%	May 15, 2025
NTRM	200602-06	6162660Y	243.3 PPM PROPANE/AIR	+/- 0.5%	Mar 17, 2027
ANALYTICAL EQUIPMENT					
Instrument/Make/Model			Last Multipoint Calibration		
Nicolet IS50 FTIR AUP2110295 CH4			Oct 13, 2021		
Nicolet IS50 FTIR AUP2110295 C3H8			Oct 14, 2021		

Triad Data Available Upon Request

NOTES:

Gross Weight: 28.0 Kg
Net Weight: 4.9 Kg
PO# 5221004861



COPY

Michael A. Huber

Approved for Release

DRY GAS METER XC-572V

Serial No. : 1110070

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic Meters (m³)

Meter Console Information

Console Model #: XC-572V

Console Serial #: 1110070

DGM Model #: SK25EX

DGM Serial #: 0005413

Calibration Conditions

Calibration Reference No.: WDS-SV680004

Ambient Temp (°C): 26.4

Barometric Pressure (mm Hg): 766

Relative Humidity (%): 65

Factors/Conversions

Std Temp (°K): 298

Std Press. (mm Hg): 760

K₁: 0.392

Reference Equipment

WTM Model: W-NKoDa-6B

WTM Serial: 546321

WTM Cal. Due: Mar-23

Gamma: 1.0000

WTM Thermometer: Internal

Metering Console				Calibration Meter					
Run Time (minutes)	Orifice, ΔH (mm H ₂ O)	Volume (m³)		Outlet Temperature (°C)		Volume (m³)		Outlet Temp Initial	Outlet Temp Final
		Initial	Final	Initial	Final	Initial	Final		
(Q)	(P _o)	(V _o)	(V _o)	(T _o)	(T _o)	(V _o)	(V _o)	(T _o)	(T _o)
min	mm H ₂ O	m³	m³	°C	°C	m³	m³	°C	°C
15.00	13.0	397.7244	397.9056	25	25	289.58787	289.76942	25	25
10.00	25.0	397.9285	398.0984	25	26	289.79207	289.95964	25	25
8.00	50.0	398.1162	398.3058	26	26	289.97735	290.16549	25	25
7.00	80.0	398.3386	398.5469	26	26	290.19612	290.40517	25	25
5.00	120.0	398.5893	398.7513	26	27	290.42752	290.60906	25	25

Standardized Data				Calibration Results			
Test Meter		Reference Meter		Calibration Factor		Flowrate	
(V _{test})	(Q _{test})	(V _{ref})	(Q _{ref})	Value	Variation	Std & Corr	ΔH @ (mm H ₂ O)
m³	m³/min	m³	m³/min	(Y)	(ΔY)	(Q _{corrected})	(ΔH@)
						m³/min	mm H ₂ O
0.180	0.012	0.181	0.012	1.001	0.009	0.012	41.038
0.169	0.017	0.167	0.017	0.986	-0.008	0.017	41.198
0.189	0.024	0.187	0.023	0.991	-0.001	0.023	41.966
0.210	0.030	0.208	0.030	0.990	-0.002	0.030	41.881
0.182	0.036	0.180	0.036	0.991	0.001	0.036	42.759
				0.992	0.000		41.768
							= ΔH @ Average

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.01.

Note: For ΔH_o, orifice pressure differential that equals to 0.75cm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O

Pass/Fail Result:

Pass


Signature

(Palpasu Chaisana)
Service Engineer

บริษัท วิสโดม ไนน์แอนด์ เซอร์วิส กรุ๊ป จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Date:

13/06/2020

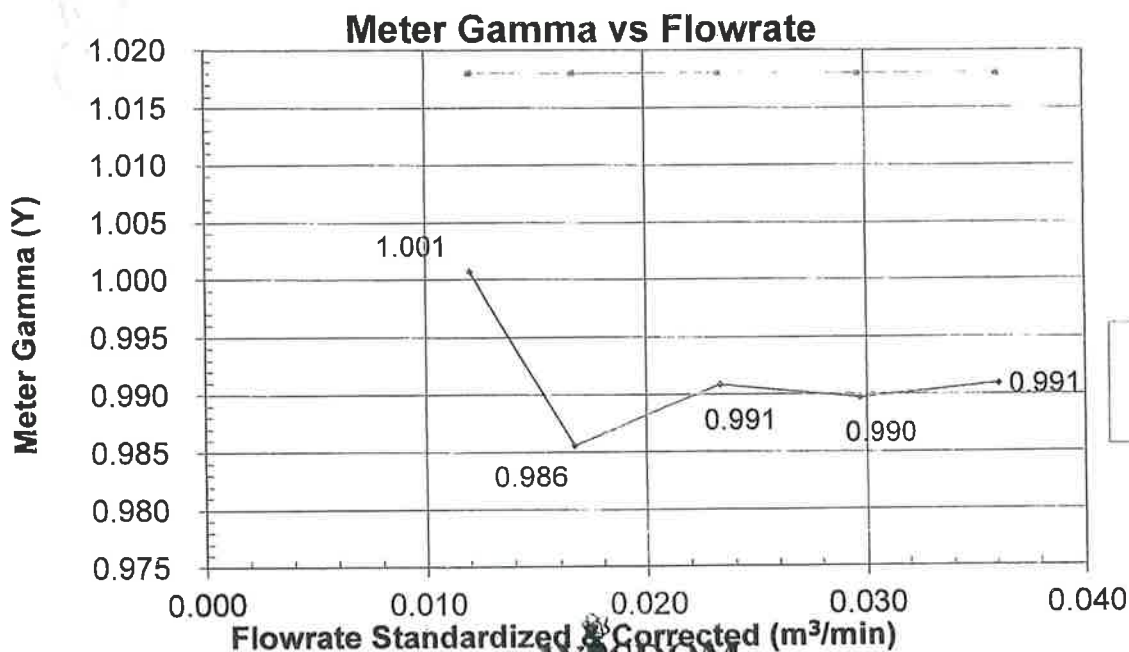

Console Serial: 1110070

Console Model: XC-572V

บริษัท วิสโดม ไนน์แอนด์ เซอร์วิส กรุ๊ป จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

WSDOM THERMOCOUPLES SYSTEM CALIBRATION

บริษัท วิสโดม ไซนซ์ แอนด์ เซอร์วิส กรุ๊ป จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Sampling System Equipment Information		Calibration Conditions	
Console Model Number	XC-572V	Calibration Reference No.	WDS-SV650004
Console Serial Number	1110070	Ambient Temp	25.4 °C
Meter Box Model Number	JENCO 765	Barometric Pressure	756 mm Hg
Meter Box Serial Number	JC02484	Relative Humidity	55 %
		Reference Thermometer	FLUKE 714
		Serial Number	9038005

Results												
Console Thermocouple Simulator												
Channel and test point	Temperature Reading (°C)											
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	816.0	1035.0	
Stack	-18	24	37	92	150	261	373	485	596	821	1045	
Probe	-18	24	37	92	150							
Filter	-18	24	37	92	150							
Aux	-18	24	37	92	150							
Exit	-18	24	37									

Tolerance Range
Stack ± 1.50% Absolute
Probe ± 3.0 °C
Filter ± 3.0 °C


Meter Exit ± 3.0 °C
Exit ± 2.0 °C

Signature _____
(Papat Chaisana)
Service Engineer

WISDOM SCIENCE
บริษัท วิสโดม ไซนซ์ แอนด์ เซอร์วิส กรุ๊ป จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

Meter Pressure vs Flowrate

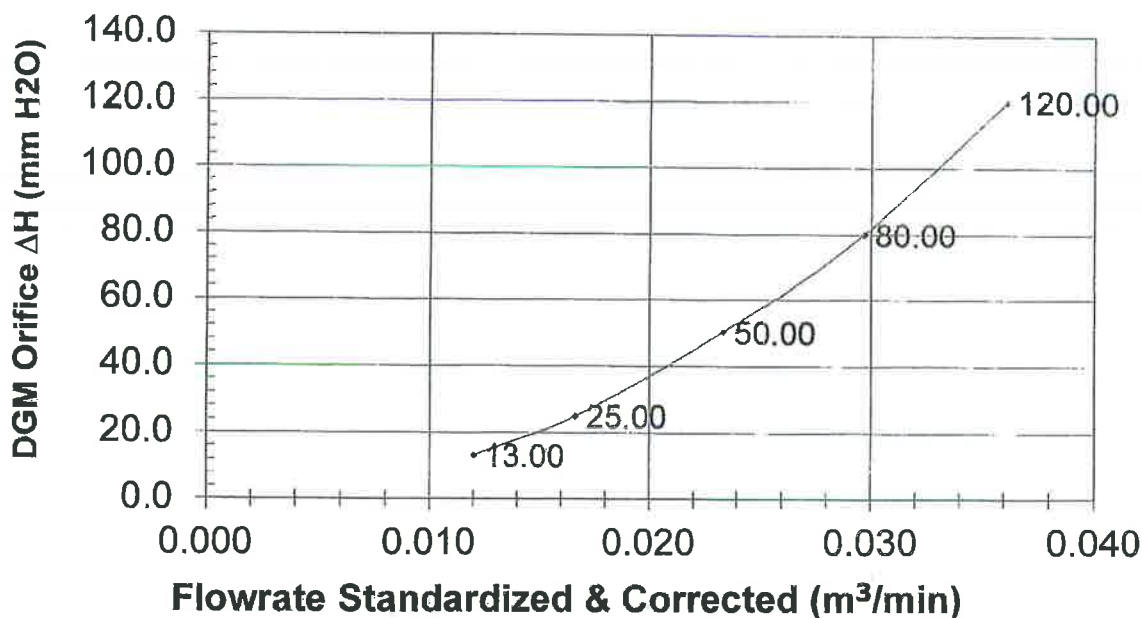

Console Serial: 1110070

WISDOM SCIENCE
บริษัท วิสโดม ไซนซ์ แอนด์ เซอร์วิส กรุ๊ป จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Console Model: XC-572V

COPY

DRY GAS METER MC-572V

Serial No. : 1007055

WISDOM

บริษัท วิสโดม ไซนส์ จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m³)

Meter Console Information

Model #: MC-572V
Serial #: 1007055
DGM Model #: SK26EX
DGM Serial #: 00008432

Calibration Condition

Calibration Date: 27/07/2022
Calibration Ref.: WDS-SV650005
Ambient Temp (°C): 23.5
Pressure (mm Hg): 766
Relative Humidity (%): 60

Factors/Conversion

Std. Temp. (°K): 298
Std. Pressure (mm Hg): 760
K₁ (K/mm Hg): 0.3857

Reference Equipment

WTM Model: W-NKoDa-5B TM Cal. Due Date: Feb. 2022
WTM Serial: 546258 Gamma: 0.9980

Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
#	P _{avg}	V _{in}	V _{out}	t _{in}	t _{out}	V _{in}	V _{out}	t _{in}	t _{out}
15.00	13.0	0.0025	0.1685	25	25	307.83244	307.99618	25	25
10.00	25.0	0.1810	0.3489	25	25	308.00127	308.15867	25	25
8.00	50.0	0.3711	0.5509	25	25	308.18244	308.34119	25	25
7.00	80.0	0.5844	0.7881	25	25	308.34877	308.55037	25	25
5.00	120.0	0.8310	1.0074	25	25	308.59261	308.77072	25	25


Standardized Data				Calibration Results				
Test Meter		Reference Meter		Correction Factor		Flow Rate	ΔH _g (mm H ₂ O)	
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	0.0212 SCMM	Variation
V _{std} (m ³)	Q _{std} m ³ /min	V _{ref} (m ³)	Q _{ref} m ³ /min	(Y)	(ΔY)	Q _{ref} m ³ /min	ΔH _g	ΔΔH _g
0.183	0.011	0.160	0.011	0.983	-0.005	0.011	50.885	3.735
0.158	0.016	0.154	0.015	0.986	-0.002	0.015	48.980	0.030
0.177	0.022	0.174	0.022	0.987	-0.001	0.022	46.834	-0.098
0.199	0.028	0.197	0.028	0.990	0.001	0.028	45.366	-1.564
0.175	0.035	0.174	0.035	0.988	0.008	0.035	44.824	-2.106
				0.988	= Y Avg.		46.930	= ΔH _g Avg

Pass/Fail Result: **Pass**

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02


Note: For ΔH_g, orifice pressure differential that equates to 0.75cm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O

Signature


(Palpasu Chaisana)
Service Engineer
บริษัท วิสโดม ไซนส์ จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Date 27/07/2022

Meter Gamma vs Flowrate

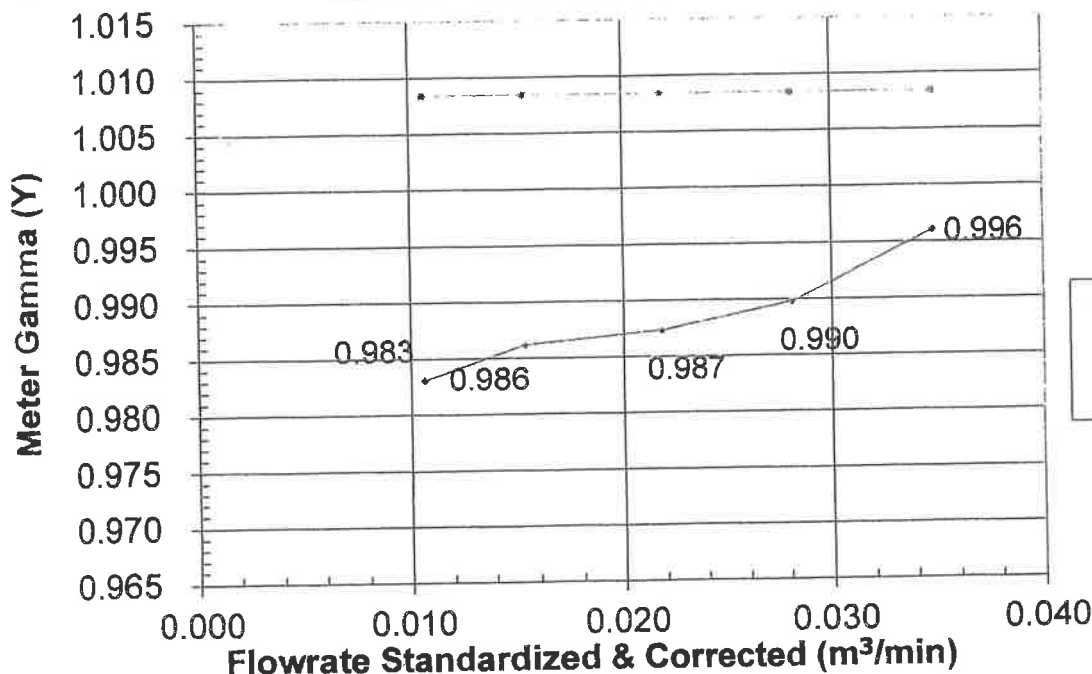


Console Serial: 1007055

A-50

Console Model:

MC-572V

Meter Pressure vs Flowrate

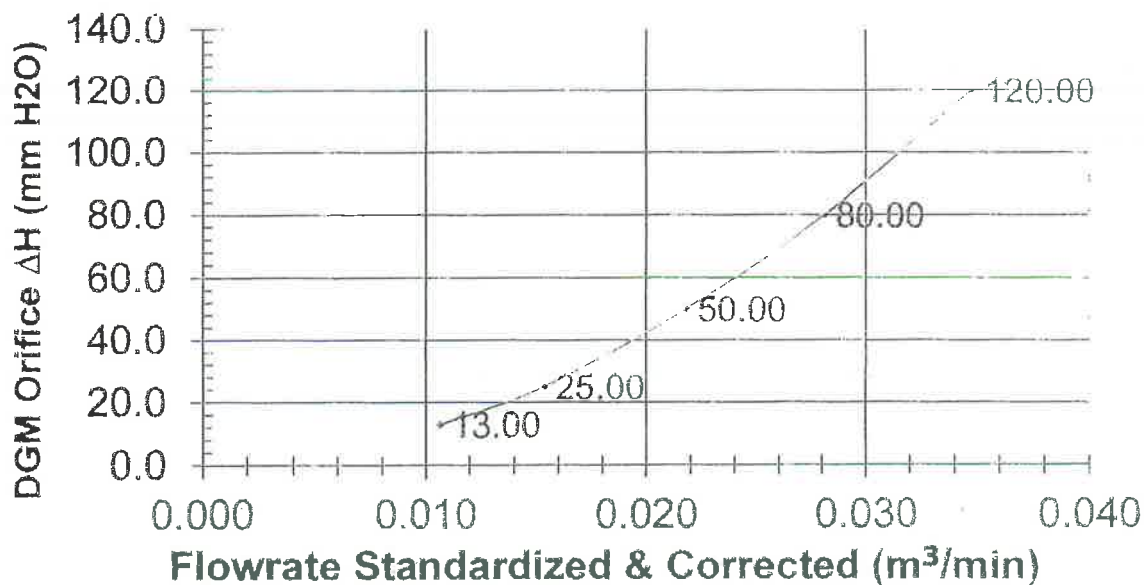

Console Serial:

1007055

Console Model:

MC-572V

COPY

THERMOCOUPLES SYSTEM CALIBRATION

W SDOM

WSDOM has been calibrated and used for the purpose of this report.

Sampling System Equipment Information		Calibration Conditions	
Console Model Number	MC-572V	Date	27/07/2022
Console Serial Number	1007055	Calibration Reference No.	WDS-SV650005
Meter Box Model Number	DIGICON	Barometric Pressure	756 mm Hg
Meter Box Serial Number	N/A	Reference Thermometer	FLUKE 714
		Serial Number	9038005

Results									
Console Thermocouple Simulator									
Channel and test point		Meter Box Channel Temperature Reading (°C)							
		-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0
Stack		-18	25	38	93	150	261	373	485
Probe		-18	25	38	92	150			
Filter		-18	25	38	92	150			
Aux		-18	25	38	92	150			
Exit		-18	25	38					

ance Range
Stack
Probe
Filter

± 1.50% °K
± 3.0 °C
± 3.0 °C

Meter
Exit

Signature

(Patpasu Chaisana)
Service Engineer

COPY

DRY GAS METER MC-572V

Serial No. : 0504003

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m³)

Meter Console Information

Console Model : MC572V
Console Serial : 0504003
DGM Model # : SK25EX
DGM Serial # : 0009854

Calibration Condition

Calibration Date : 3-Apr-23
Issue Date : 3-Apr-23
Cal. Report No. : WDS-SV660039
Ambient Temp (°C) : 25
Pressure (mm Hg) : 758
Relative Humidity (%) : 60

Factors/Conversion

Std. Temp (°K) : 298
Std. Pressure (mm Hg) : 760
K₁ (K/mm Hg) : 0.3857

Reference Equipment

WTM Model : W-NK0Da-5B WTM Cal. Due Date : Nov. 2022
WTM Serial : 600245 Gamma : 1.0000

UUT Meter (DGM)				Reference Meter (WTM)					
Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
0	P _{min}	V _{in}	V _{out}	t _{in}	t _{out}	V _{in}	V _{out}	L _{in}	L _{out}
15.00	13.0	2.1249	2.2873	26	26	11.24924	11.40853	25	25
10.00	25.0	1.9384	2.0954	26	26	11.06645	11.22136	25	25
8.00	50.0	1.7294	1.9105	26	26	10.66093	11.03905	25	25
7.00	80.0	1.4887	1.6921	26	26	10.62322	10.82407	25	25
5.00	120.0	1.1950	1.3736	26	26	10.33100	10.50914	25	25

Standardized Data

Calibration Results

Test Meter		Reference Meter		Correction Factor		Flow Rate		ΔH@ (mm H ₂ O)
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma" (Y)	Variation (ΔY)	Std & Corr	0.0212 SCMM	Variation
V _{test} (m ³)	Q _{test} m ³ /min	V _{ref} (m ³)	Q _{ref} m ³ /min			Q _{corrected}	ΔH ₀	ΔΔH ₀
0.159	0.011	0.156	0.010	0.983	-0.001	0.010	52.990	5.531
0.155	0.015	0.152	0.015	0.981	-0.002	0.015	47.999	0.540
0.178	0.022	0.175	0.022	0.982	-0.002	0.022	46.696	-0.763
0.200	0.029	0.197	0.028	0.983	-0.001	0.028	45.249	-2.210
0.177	0.035	0.175	0.035	0.989	0.006	0.035	44.361	-3.098
				0.984	= Y Avg		47.459	= ΔH@ Avg

Pass/Fail Result: **Pass**

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter acceptable tolerance: of individual values from the average is ±0.02
Note: For ΔH₀, orifice pressure differential that equates to 0.75cfm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O


Approved By:

(Palpasu Chaisana)
Service Manager

Date: 3-Apr-23

COPY

Meter Gamma vs Flowrate

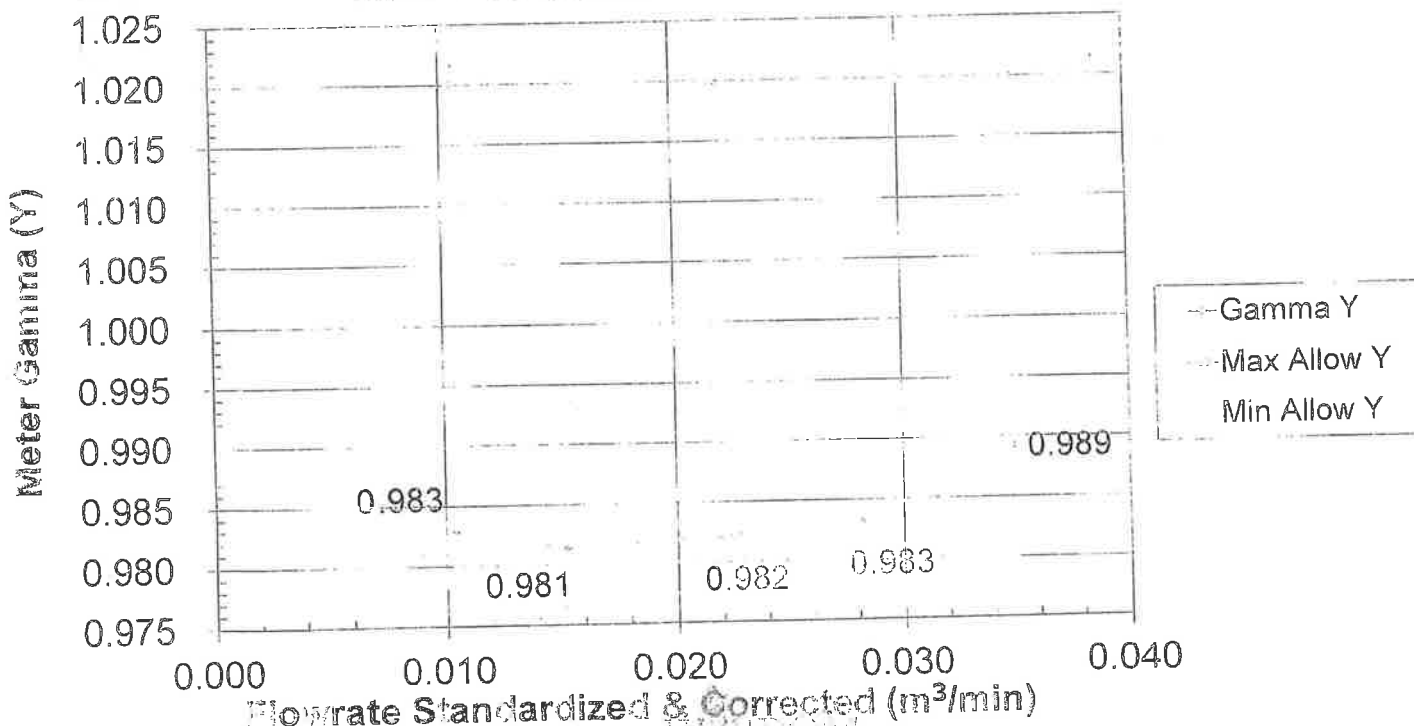

Console Serial

0504003

Console Model

MC572V

COPY

TEMPERATURE DISPLAY CALIBRATION

Meter Console Information

Console Model : MC572V
Console Serial : 0504003
Temp Indicator Model : 765-KF
Temp Indicator Serial : JC17852

Calibration Conditions

Cal. Date : 3-Apr-23
Issue Date : 3-Apr-23
Cal. Report No. : WDS-SV600039
Ambient Temp. (°C) : 25
Pressure (mm Hg) : 758
Humidity (%) : 60

Reference Equipment

Temp. Simulator Model : FLUKE 7148
Serial No. : 605900035

Temperature Sensor Calibration

Reference Point	Ref. Temperature Temperature	°C	°C
#			
1	-18.0	-17.0	1.0
2	38.0	37.0	1.0
3	93.0	92.0	1.0
4	149.0	148.0	1.0
5	260.0	259.0	1.0
6	371.0	372.0	-1.0
7	482.0	482.0	0.0
8	593.0	594.0	-1.0
9	816.0	816.0	0.0
10	1038.0	1038.0	0.0
		Maximum	1.0

Note

* For valid test results, the maximum difference between temperature readings should $\leq 1.0^{\circ}\text{C}$ (EPA Method 5, Section 6.1.1.8).
Perform all TC Channel calibrations. Except meter (DGM) channel

PASS

DGM Out Temperature Sensor Calibration

Temperature point	Ref. Temperature Temperature	°C	°C
#			
Ambient	26.5	26.0	0.5
Heat	100.5	102.0	-1.5

Difference Rang

DGM Out Temp. Diff. $\pm 3^{\circ}\text{C}$

PASS


Approved By :

(Signature)
(Signature)
Service Manager

Signature

COPY

Meter Pressure vs Flowrate

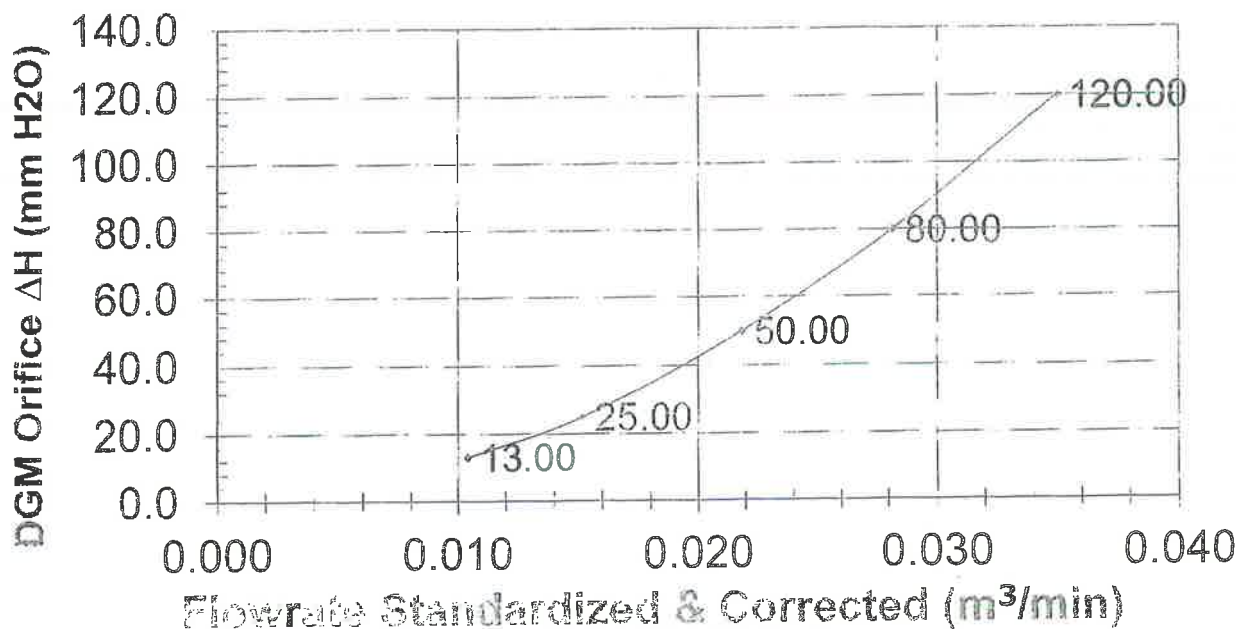

Console Serial:

0504003

Console Model:

MC572V

WISDOM SCIENCE
บริษัท วิสโดม ไซนซ์ แอนด์ เซอร์วิส กรุ๊ป จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

Flue gas Analyzer
Testo 350XL
Serial No. 01807527



Calibration Certificate

Certificate No.: G 650383

ENTECH

Where



Calibration Certificate

Certificate No: G 650383
Date of issue : 15-Jun-22

ENTECH

Where

Instrument description : Flue gas Analyzer
Instrument model : Testo 350XL
Instrument serial no. : 01807527
ID no. or control no. :
Manufacturer : Testo SE & Co. KGaA
Probe description :
Probe model :
Probe serial :
Customer name : Eastern Thai Consulting 1992 Company Limited
Customer address : 683 Moo 11, Sukhapibarn 8 Road, Nongkham, Si Rachia, Chon Buri 20280

Total pages of certificate : 3 Pages
Receiving no. : L-222062
Receiving date. : 09-Jun-22

Parameter of calibration : Gas Calibration (Oxygen 2.498,10.00,21.00 %vol, Carbon Monoxide 80.97,309.9,1003 ppm, Nitrogen Dioxide 10.19,80.62,202.2 ppm, Nitric Oxide 10.08,150.9,320.6 ppm, Sulphur Dioxide 50.04,100.9,601.1 ppm)

Condition of UUC. : Used
Ambient condition : All of the Measurement were carried out the stabilized laboratory

Temperature : 23 ± 5 °C
Humidity : 55 ± 15 %RH

Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210

Calibration procedure no. : WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.
This certificate is applied only to item under test Environmental condition.

This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory.
Calibration certificates without signature and seal not valid.
This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 15-Jun-22

Mr. Sedawut Nueathong
Calibration Technician

Mrs. Nongluck Wongsettee
Technical Manager

COPY

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O2) 2.498 % Vol	4219/21	Linde	30-Sep-25
Oxygen (O2) 10.00 % Vol	2453/19	Linde	18-Jul-23
Oxygen (O2) 21.00 % Vol	2426/19	Linde	16-Jul-23
Carbon monoxide (CO) 80.97 ppm	2842/21	Linde	24-Jun-23
Carbon monoxide (CO) 309.9 ppm	2803/21	Linde	22-Jun-23
Carbon monoxide (CO) 1003 ppm	2829/21	Linde	23-Apr-23
Nitrogen Dioxide (NO2) 10.19 ppm	3372/21	Linde	02-Aug-23
Nitrogen Dioxide (NO2) 80.62 ppm	3240/21	Linde	25-Jul-23
Nitrogen Dioxide (NO2) 202.2 ppm	3239/21	Linde	20-Jul-23
Nitric Oxide (NO) 10.08 ppm	3241/21	Linde	25-Jul-23
Nitric Oxide (NO) 150.9 ppm	2857/21	Linde	27-Jun-23
Nitric Oxide (NO) 320.6 ppm	2944/21	Linde	02-Jul-23
Sulphur Dioxide (SO2) 50.04 ppm	3205/21	Linde	25-Jul-23
Sulphur Dioxide (SO2) 100.9 ppm	4942/20	Linde	20-Nov-22
Sulphur Dioxide (SO2) 601.1 ppm	3204/21	Linde	20-Jul-23

Measured room conditions

Temperature : 25.1 °C Humidity : 51.8 %RH Pressure : 1011.5 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,000 ml/min Gas pressure : 1021.9 mbar

Calibration Results Before Adjustment (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.498	2.53	0.032	0.20
O2 (%Vol)	10.00	10.01	0.01	0.40
O2 (%Vol)	21.00	21.14	0.14	0.80
CO (ppm)	80.97	83	2.03	2.8
CO (ppm)	309.9	323	13.1	11
CO (ppm)	1003	1050	47	34
NO2 (ppm)	10.19	9.2	-0.99	1.5
NO2 (ppm)	80.62	77.5	-3.12	5.0
NO2 (ppm)	202.2	194.6	-7.6	5.0
NO (ppm)	10.08	8	-2.08	6.0
NO (ppm)	150.9	148	-2.9	5.0
NO (ppm)	320.6	312	-8.6	10
SO2 (ppm)	50.04	46	-4.04	5.0
SO2 (ppm)	100.9	98	-2.9	5.0
SO2 (ppm)	601.1	598	-3.1	14

COPY

Calibration Results After Adjustment (Table 3)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty ($\pm$)
O ₂ (%Vol)	2.498	2.53	0.032	0.20
O ₂ (%Vol)	10.00	10.01	0.01	0.40
O ₂ (%Vol)	21.00	21.14	0.14	0.80
CO (ppm)	80.97	81	0.03	2.8
CO (ppm)	309.9	310	0.1	11
CO (ppm)	1003	1005	2	34
NO ₂ (ppm)	10.19	9.2	-0.99	1.5
NO ₂ (ppm)	80.62	77.5	-3.12	5.0
NO ₂ (ppm)	202.2	194.6	-7.6	5.0
NO (ppm)	10.08	8	-2.08	6.0
NO (ppm)	150.9	148	-2.9	5.0
NO (ppm)	320.6	312	-8.6	10
SO ₂ (ppm)	50.04	46	-4.04	5.0
SO ₂ (ppm)	100.9	98	-2.9	5.0
SO ₂ (ppm)	601.1	598	-3.1	14

Remark : 1 cmol/mol = 1 %vol , 1 μ mol/mol = 1 ppm.

End of Report

COPY

Hot Air Oven

Model : UFE 500

Serial No. : G511.0182



AMARC



AMARC

ASIA MEDICAL AND AGRICULTURAL LABORATORY AND RESEARCH CENTER

NSC-TSI-TSI17025
CALIBRATION 0152

Page 2 of 3

REPORT OF CALIBRATION

Certificate No. : 23-006679

Sample Code : 23-02820-002

CERTIFICATE OF CALIBRATION

Certificate No. : 23-006679

Sample Code : 23-02820-002

Customer

EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Si Racha, Chonburi 20230

Location of Calibration

EASTERN THAI CONSULTING 1992 CO., LTD.
(Hot Lab)

Equipment

Temperature controlled enclosures (Hot air oven)

Manufacturer

Model : UFE 500

Serial No.

ID No. : LABE 17/4

Date of Receipt

Date of Calibration : 20 January 2023

Condition of Calibration

1. Environment	1.1 Ambient temperature	27.9 °C	Minimum	25.3 °C
2. Relative humidity	2.1 Maximum	50.9 %	Minimum	38.5 %
3. Line voltage supplied	3.1 Maximum	221.9 VAC	Minimum	218.5 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-P100)	LB-DA-11 (RTD-138 to RTD-146)	22-040309	21 April 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Sarawoot Thammo

Scientist

24 January 2023

Approved by

(Mr. Somchai Neampunt)

Signed for Director

Issue date

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be used for any other purpose without the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

AMARC

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

361 Soi Ladprao 122, Ladprao Road, Bangkok 10330, Thailand

TEL 02-516-2422

FAX 02-516-6948

Created Date: 15/01/21

COPY



REPORT OF CALIBRATION

Page 3 of 3
Certificate No. : 23-006679
Sample Code : 23-02820-002

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 56 cm ; D = 40 cm ; H = 48 cm
3. Air valve or fresh air level : Off
4. Fan level : Open

5. The quoted uncertainty includes " Stability of chamber and loading effect in chamber at 20% of uniformity ".

6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference

location which are observed at the same time.

Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.

8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.

9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.

10. Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M2003

- End of Report -

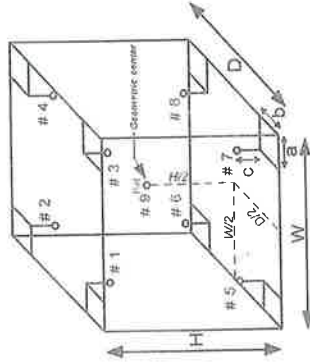


Figure: Example of sensor installation positions

COPY

UV/VIS SPECTROPHOTOMETER

Model : UV – 1800

Serial No. : A11635101643CD



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor 7 Rama4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No. BSCC-UV-167/22
Equipment UV/Vis Spectrophotometer
Model UV-1800
Manufacturer Shimadzu
Serial No. A11635101643 CD
ID No. LAGE 03/2
Date of receipt 18 May 2022
Date of calibration 18 May 2022
Date of issue 25 May 2022

Customer name Eastern Thal Consulting 1992 Co., Ltd.
Address 683 Moo 11, Sukkaphibarn 8 Rd., Nongkham, Siracha, Chonburi 20230.

Temperature (23.8-24.5) °C (On site)
Humidity (47.6-48.3) %RH (On site)

Equipment condition Good Operation

Calibration Location Analysis Department

Calibration Procedure In-house method WJUV-702-01 based on ASTM E275-01

Traceability
Wavelength Accuracy is traceable to certificate No. 96367 and 96366
Photometric Accuracy is traceable to certificate No. 99825 and 100147
Stray Light is traceable to certificate No. 96346
The above certificate are traceable to SI unit through Starna Scientific Ltd.
(UKAS accredited calibration laboratory NO. 0659)

Calibrated by Mr.Kanchit Choothep

Approved by

Mr.Kanchit Choothep
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

FM-UV-708-02 Rev.01 (2301/63)



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor 7 Rama4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Number of Page(s) 2 of 3

Certificate No. BSCC-UV-167/22

Calibration Results:
1. Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
287.71	287.80	0.09	0.18
445.82	445.95	0.13	0.18
536.52	536.60	0.08	0.18
741.02	741.00	-0.02	0.18
879.41	879.40	-0.01	0.18

2. Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000	0.0000	0.0000	0.0075
	0.7311	0.7321	0.0010	0.0075
257	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
313	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
350	0.0000	0.0000	0.0000	0.0075
	0.6306	0.6314	0.0008	0.0075

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

FM-UV-708-02 Rev.01 (2301/63)



Bara Scientific
968 U Chu Lang Building Floor 7 Rama 4 Road
Siam Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6379496-7
www.barscientific.com



Certificate of Calibration

Certificate No. BSCC-UV-167/22

3 of 3

Calibration Results:

3 Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
420.0	0.0000 0.5472 0.7637 1.0480	0.0000 0.5481 0.7636 1.0497	0.0000 0.0003 -0.0001 0.0017	0.0042 0.0042 0.0042 0.0042
440.0	0.0000 0.5371 0.7467 1.0233	0.0000 0.5377 0.7451 1.0240	0.0000 0.0006 -0.0006 0.0016	0.0042 0.0042 0.0042 0.0042
465.0	CNR CNR CNR CNR	CNR CNR CNR CNR	CNR CNR CNR CNR	CNR CNR CNR CNR
546.1	0.0000 0.5006 0.6961 0.9563	0.0000 0.5006 0.6944 0.9550	0.0000 0.0000 -0.0017 -0.0013	0.0042 0.0042 0.0042 0.0042
590.0	CNR CNR CNR CNR	CNR CNR CNR CNR	CNR CNR CNR CNR	CNR CNR CNR CNR
635.0	0.0000 0.5137 0.6907 0.9533	0.0000 0.5137 0.6891 0.9519	0.0000 0.0000 -0.0016 -0.0014	0.0042 0.0042 0.0042 0.0042

*CNR = Customer not request

4. Stray Light*

Standard cut-off wavelength (nm)	Wavelength (nm)	Unit Under Calibration(UUC) Transmission (%T)	Absorbance (A)
200.91±0.11nm	201.10	0.9543	2.0204

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A
*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%
End of Certificate

COPY

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

FM-UV-708-02 Rev.01 (2309183)

ANALYTICAL BALANCE (DU)

Model. : XS205DU

Serial No. : 1126323724



Certificate No. : 23-006683

Sample Code : 23-02820-006

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkhram,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : 1126323724

ID No. : LABE 05/1

Date of Receipt : 20 January 2023

Date of Calibration : 20 January 2023

Calibrated by Mr. Thanadol Pholthep
Scientist

Issue date : 25 January 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)



Certificate No. : 23-006683

Sample Code : 23-02820-006

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : METTLER TOLEDO
Model : XS205DU
Capacity : Max 81 g / 220 g
Resolution : 0.01 mg / 0.1 mg
Serial No. : 1126323724
ID No. : LABE 05/1

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 80	☐ Before adjustment	☐ After adjustment
☒ No adjustment	Nominal value	40	90
☐ Adjustment	Standard weight	40.000042	60.000045
	Average reading of indicator	40.00015	90.00019
	Standard deviation	0.000004	0.000007
Unit : g	Range : 200	☐ Before adjustment	☐ After adjustment
☒ No adjustment	Nominal value	100	200
☐ Adjustment	Standard weight	100.000022	200.000199
	Average reading of indicator	100.0001	200.0004
	Standard deviation	0.00004	0.00008

COPY

Certificate No. : 23-006683

Sample Code : 23-02820-006

Page 3 of 4

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range :		Range :	
Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	0.99800	0	0.9980
40	0.99800	100	0.9980
80	0.99800	200	0.9980

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.000000	0.00000	0.00000	0.0000090	2.01
0.01	0.0100036	0.01000	0.00000	0.0000093	2.01
0.1	0.1000062	0.10000	0.00001	0.000012	2.00
1	1.0000036	1.00001	-0.00001	0.000014	2.00
5	5.0000044	5.00003	-0.00003	0.000020	2.00
10	10.000000	10.00007	-0.00007	0.000032	2.00
20	20.000016	20.00011	-0.00009	0.000036	2.00
50	50.000029	50.00013	-0.00010	0.000067	2.00
100	100.000022	100.0001	-0.0001	0.00016	2.00
150	150.000051	150.0001	0.0000	0.00023	2.00
200	200.000199	200.0003	-0.0001	0.00028	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY

Certificate No. : 23-006683

Sample Code : 23-02820-006

Page 4 of 4

REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighting pan ☐ Circle ☐ Triangular ☒ Rectangular

Test weight : 50 and 100
Unit : g

Range	Position	Reading of indicator	Reading of indicator
1	50.00014	50.00014	100.0001
2	50.00014	50.00014	99.9998
3	50.00006	50.00006	100.0000
4	50.00010	50.00010	100.0001
5	50.00017	50.00017	100.0001
6	50.00014	50.00014	100.0001
Maximum difference	0.00008	0.00008	0.0003

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019
2. This result of calibration was found accurate as shown on date and place of calibration only.
3. Condition of Calibration item: Normal
4. This certification is traceable to the International System of Unit maintained at :-
Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument
1) STANDARD WEIGHT 1 mg to 1 kgClass ID No.
E2 LB-WE-57Certificate No.
22-060639Due Date
27 June 2023

6. Ambient conditions	Min	Max
Temperature (°C)	21.3	22.4
Relative Humidity (%Rh)	39.2	40.4
Air pressure (hPa)	1008.4	1010.1

COPY

End of Report -

ANALYTICAL BALANCE

Model. : SECURA224-1S

Serial No. : 0036707137

Certificate No. : 23-006682
Sample Code : 23-02820-005

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : SARTORIUS
Model : SECURA224-IS
Capacity : Max 220 g
Resolution : 0.0001 g
Serial No. : 0036707137
ID No. : LABE 05/2

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 220	☐ Before adjustment	☐ After adjustment
☒ No adjustment	Nominal value	100	200
☐ Adjustment	Standard weight	100.000022	200.000199
	Average reading of indicator	99.9998	199.9999
	Standard deviation	0.00007	0.00007

Unit : .	Range : .	☐ Before adjustment	☐ After adjustment
☐ No adjustment	Nominal value	.	.
☐ Adjustment	Standard weight	.	.
	Average reading of indicator	.	.
	Standard deviation	.	.

COPY

Certificate No. : 23-006682
Sample Code : 23-02820-005

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : SARTORIUS

Model : SECURA224-IS

Serial No. : 0036707137

ID No. : LABE 05/2

Date of Receipt : 20 January 2023

Date of Calibration : 20 January 2023

Calibrated by : Mr. Thanadol Pholthep
Scientist

Issue date : 25 January 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 23-006682

Sample Code : 23-02820-005

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Test Point	Range	Sensitivity, S	Test Point	Range	Sensitivity, S
0	220	0.9980			
100		0.9980			
200		0.9980			

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.0000	0.0000	0.00011	2.04
0.01	0.0100036	0.0100	0.0000	0.00011	2.04
0.1	0.1000062	0.1000	0.0000	0.00011	2.04
1	1.0000036	1.0000	0.0000	0.00011	2.04
2	2.0000128	2.0000	0.0000	0.00011	2.04
5	5.0000044	5.0000	0.0000	0.00011	2.04
10	10.0000000	10.0000	0.0000	0.00011	2.03
20	20.0000016	20.0000	0.0000	0.00012	2.03
50	50.0000029	50.0000	0.0000	0.00013	2.02
100	100.0000022	99.9998	0.0002	0.00017	2.01
200	200.0000199	200.0000	0.0002	0.00028	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY

27 June 2023



Certificate No. : 23-006682

Sample Code : 23-02820-005


REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighting pan	Test weight : 100
☒ Circle	Unit : g
☐ Triangular	
☐ Rectangular	
Range	Reading of indicator
220	
Position	Reading of indicator
1	99.9998
2	100.0001
3	99.9997
4	99.9998
5	99.9998
6	99.9998
Maximum difference	0.0003
Condition of Calibration	

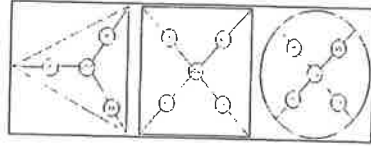

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : -

- Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument

1) STANDARD WEIGHT 1 mg to 1 kg

Class LB-WE-57

Certificate No. 22-060639

Due Date 27 June 2023

27 June 2023

COPY

- End of Report -

AUTOCLAVE

Model : FLS-1000

Serial No. : 55169083



CERTIFICATE OF CALIBRATION

Page 1 of 2

Certificate No. : 22-102070

Sample Code : 22-37024-003

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapiban 8 Rd., Nongkham,

Siracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.

(Autoclave Room)

Equipment : Autoclave

Manufacturer : TOMY

Model : FLS-1000

Serial No. : 55169083

ID No. : LABE 43/2

Date of Receipt : 19 September 2022

Date of Calibration : 19 September 2022

Condition of Calibration

1. Environment
- 1.1 Ambient temperature : Maximum 30.3 °C ; Minimum 28.8 °C
- 1.2 Relative humidity : Maximum 56.1 % ; Minimum 45.1 %
- 1.3 Line voltage supplied : Maximum 227.3 VAC ; Minimum 219.2 VAC

2. Calibration method

The calibration use in-house method; WI-CL-025 based on BS 2646 part 5: 1993 item 3.1.

3. Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Temperature Data Logger	HiTemp 140	LB-TEM-17	22-089923	31 August 2023
3.2 Temperature Data Logger	HiTemp 140	LB-TEM-16	22-023565	08 March 2023
3.3 Temperature Data Logger	TEMP 1000S	LB-TEM-14	22-089922	31 August 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Sarawoot Thammo

Approved by

(Mr. Somchai Neampunt)

Scientist

Issue date

22 September 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

FM-CI-114

TEL 02-516-2422

FAX 02-516-6949

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

REPORT OF CALIBRATION

Page 2 of 2

Certificate No. : 22-102070

Sample Code : 22-37024-01

Results of Calibration

Resolution : 1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading		Measured Temperature at each positions (°C)			Uncertainty ± (°C)	Coverage factor k
		Temperature (°C)	Pressure (MPa)					
				# 1	# 2 <i>Ref</i>	# 3		
121	121	121	0.11	121.81	121.80	121.83	0.64	2.00

2. Characterization results

Calibration Point (°C)	Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
121	0.08	0.12	0.17

Notes

- UUC* = Unit Under Calibration
- The quoted uncertainty includes* Stability of chamber and loading effect in chamber at 20% of uniformity*.
- Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
- Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
- Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
- UUC* reading - the average reading of indicating device that forms the integral part of the autoclave.
- Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -




Figure: Example of sensor installation Positions

- Standard 1 = In the chamber drain, within 100 mm.
- Standard 2 = In the upper half of the chamber.
- Standard 3 = Attached to the load temperature probe, within 20 mm.

COPY

TEL 02-516-2422

FAX 02-516-6949

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

CONTACT@AMARC.CO.

WWW.AMARC.CO.

BOD INCUBATOR

ID No. : LABE 19/2



CERTIFICATE OF CALIBRATION

Certificate No. : 22-136844
Sample Code : 22-51164-006

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhepiban 8 Rd., Nongkham,
Siracha, Chonburi 20230
Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)
Manufacturer : N/A
Model : N/A
Serial No. : S540040277
ID No. : LABE 19/2
Date of Receipt : 21 December 2022
Date of Calibration : 21 December 2022

Condition of Calibration

1. Environment : 1.1 Ambient temperature : Maximum 25.1 °C : Minimum 24.3 °C
: 1.2 Relative humidity : Maximum 52.3 % : Minimum 48.5 %
: 1.3 Line voltage supplied : Maximum 223.6 VAC : Minimum 221.9 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-PT100)	LB-DA-T1 (RTD-148 to RTD-155, RTD-227)	22-040308	24 April 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Nathanan Phosri

Approved by

(Mr. Sornchai Neampunt)

Scientist

Issue date

26 December 2022

The uncertainties are for a confidence probability of approximately 95%.
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation gained by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
PM-CL-114
Rev 01
Effective Date 15/10/21

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH

TEL 02-516-2422
FAX 02-516-6949

Rev 01

Effective Date 15/10/21



REPORT OF CALIBRATION

Certificate No. : 22-136844
Sample Code : 22-51164-006

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C) reading (°C)	Measured temperature at each positions (°C)										Uncertainty ± (°C)	Coverage factor k
		# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 nd	# 10		
20	20.0	20.0	20.0	19.65	19.56	19.47	20.29	20.47	20.58	20.29	20.29	0.35	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.13	1.09	1.90

Notes

UUC* = Unit Under Calibration

Signature

COPY

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
PM-CL-018
Rev 09
Effective Date 15/10/21
CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
TEL 02-516-2422
FAX 02-516-6949



NSC-TSI-7617025
CALIBRATION 0152

Page 3 of 3

REPORT OF CALIBRATION

Certificate No. : 22-136844

Sample Code : 22-51164-006

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 60 cm ; D = 70 cm ; H = 124 cm
3. Air valve or fresh air level : Off
4. Fan level : open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

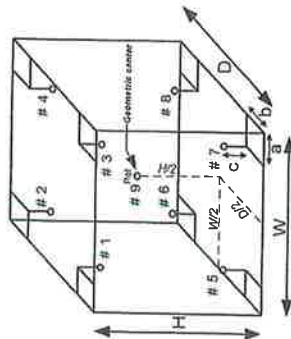


Figure: Example of sensor
Installation Positions

- End of Report -

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY

BOD INCUBATOR

ID No. : LABE 19/5



REPORT OF CALIBRATION

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C) reading (°C)	Measured temperature at each positions (°C)								Uncertainty ± (°C)	Coverage factor k
		# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8		
20	20.6	20.09	19.99	20.00	20.03	19.95	19.98	20.00	19.81	19.90	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.17	0.32	0.57

Notes

UUC* = Unit Under Calibration

CERTIFICATE OF CALIBRATION

Customer

EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhaphan 8 Rd., Nongkham,
Sriacha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : Lovibond Model : TC445S

Serial No. : 0520/005227 ID No. : LABE 19/5

Date of Receipt : 23 May 2022 Date of Calibration : 23 May 2022

Condition of Calibration

1. Environment	1.1 Ambient temperature	Maximum 34.6 °C	Minimum 34.0 °C
	1.2 Relative humidity	Maximum 50.7 %	Minimum 43.1 %
	1.3 Line voltage supplied	Maximum 225.9 VAC	Minimum 220.4 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-P100)	LB-DA-10 (RTD-257 to RTD-265)	21-056687	05 July 2022

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Pettarakorn Panklong

Approved by

(Mr. Somchai Neampunt)

Signed for Director

Issue date

25 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road, Phlabphla, Wang Thonglang, Bangkok 10310

TEL 02-516-2422 FAX 02-516-6949

Rev 01 Effective Date 15/10/21

COPY

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

FM-CL-018

TEL 02-516-2422

FAX 02-516-6949

Rev 09

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

Effective Date 15/10/21



REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 22-053227
Sample Code : 22-19571-002

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber : (Working space)
W = 65 cm ; D = 55 cm ; H = 146 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC² reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

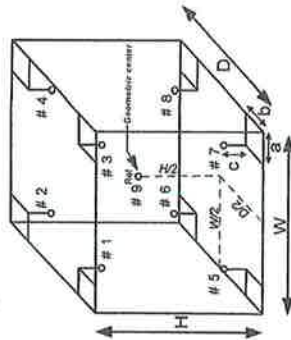


Figure: Example of sensor installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

Handwritten signature

COPY

DO

Model : YSI 5000

Serial No. : 18E101961



Harikul Science Co., Ltd.
694 Soi Ratchadaniwet 24, Pracharabamphen,
Samsenok, HuaiKhwang, Bangkok 10310
Tel: 0-2274-2456 Fax: 0-2274-2443
Email: info@harikul.com www.harikul.com

CERT No.: HS-T055H

Certificate of Calibration

Calibration Date : 23 Aug 22

Submitted by : Eastern Thai Consulting 1992 Company Limited
683 Moo.11 Sukaphibab8 Rd., Nongkham, Sriracha,
Chonburi 20230

Model : YSI 5000
S/N : 18E101961
Probe : YSI 5010
S/N : 18A100724
ID NO. :
Air Temp ref : S/N. E00522
Barometric ref : S/N. E00522
Water Temp ref : S/N. 11431

Avg Room Temp : 20 °C
Avg Water Temp : 20 °C
Air Pressure : 760.00 mmHg
Salinity : 0 ppt

Technician : Kitipong M.

Calibration Details			
Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.09	(PASS)	-
Measurement 4 (mg/l)	9.10	(PASS)	-
Measurement 5 (mg/l)	9.10	(PASS)	-
Measurement 6 (mg/l)	9.09	(PASS)	-
Measurement 7 (mg/l)	9.09	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.09	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-

Mean Measurement	9.09	mg/l	-
Inaccuracy	0.00	mg/l	-
Overall Status	(PASS)		

Manufacturer Specification	
Accuracy = +/- 0.02 mg/l	

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.


Technician Signature


Laboratory Manager

Hot Air Oven

Model : UM 400

Serial No. : 900982



CERTIFICATE OF CALIBRATION

Page 1 of 3

Certificate No. : 22-025399

Sample Code : 22-09604-002

Customer : EASTERN THAI CONSULTING-1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.

(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)
Manufacturer : Memmert
Serial No. : 900982
ID No. : LABE 17/1
Date of Receipt : 11 March 2022
Date of Calibration : 11 March 2022

Condition of Calibration

1. Environment 1.1 Ambient temperature : Maximum 28.7 °C ; Minimum 27.4 °C
1.2 Relative humidity : Maximum 61.5 % ; Minimum 55.8 %
1.3 Line voltage supplied : Maximum 226.5 VAC ; Minimum 224.7 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-PT100)	LB-DA-11 (RTD-138 to RTD-146)	21-035792	18 May 2022

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Nathanan Phosri

Scientist

14 March 2022

Approved by

(Mr. Somchai Naampunt)

Signed for Director

Issue date

14 March 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



REPORT OF CALIBRATION

Page 2 of 3

Certificate No. : 22-025399

Sample Code : 22-09604-002

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C) reading (°C)	Measured temperature at each positions (°C)								Uncertainty ± (°C)	Coverage factor k
		# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8		
85	85.0	85.05	84.99	84.66	84.71	84.85	84.92	84.96	84.86	0.25	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
85	0.08	0.35	0.54

Notes

- UUC* = Unit Under Calibration

COPY



REPORT OF CALIBRATION

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 40 cm ; D = 28 cm ; H = 39 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

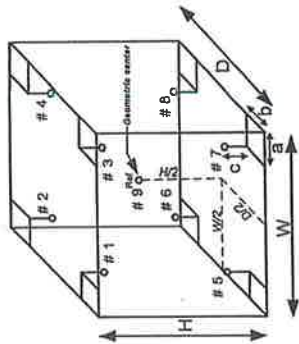


Figure: Example of sensor
Installation Positions

- End of Report -

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M0003.

COPY

LIQUID IN GLASS THERMOMETER

Model : Total immersion

Serial No. : 43560

Calibration Certificate

Certificate No.: 2300368-001-01
Client name: EASTERN THAI CONSULTING 1992 CO., LTD.
Address: 683 Moo 11, Sukhapibam 8 Rd.,
 Nongkham, Sriracha, Chonburi 20230

Equipment: Liquid-in-Glass Thermometer
Manufacturer: Precision
Model / Type: Total Immersion
Serial No.: 43560
ID No.: LABE 16/1
Order No.: 2300368
Operation No.: 2300368-001
Date of Receipt: 7 November 2022
Date of Calibration: 15 November 2022

Calibrated by Mr.Nuttapol Miyomchet
 Specialist
Approved by (Mr.Pheraphat Tuanjit)
 Manager, Division of Calibration Laboratory
 Responsible for the Technical Management Team

Date of Issue: 18 November 2022

The uncertainties are for a confidence probability of approximately 95 %.
 This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.



Calibration Report

Certificate No.: 2300368-001-01
Equipment: Liquid-in-Glass Thermometer
Type: Total Immersion
Range: -1.9 to 101.1 °C
Resolution: 0.1 °C
ID No.: LABE 16/1
Serial No.: 43560
Manufacturer: Precision
Date of Calibration: 15 November 2022

Location: Temperature Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature 23 °C ± 3 °C,
 Relative Humidity 55 % ± 15 %

Condition of this results of Calibration:

- Calibration Method : - In-house method : W-TE-015 based on ASTM E77-07
 - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
 - The temperature Scale in use at this laboratory is the International Temperature Scale of 1990 (ITS-90).
- Reference Standard Instrument :
 - Low Temperature Bath (Deep Well Compact Bath), Model: 7381, S/N: B53496.
 - Low Temperature Bath (Deep Well Compact Bath), Model: 7341, S/N: A5A084.
 - High Temperature Bath (Deep Well Compact Bath), Model: 6331, S/N: A5A087.

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
BLACK STACK THERMOMETER	1560/2560	A39258/A39719	PSL-T 0674/65	7-Jun-23	TISTR
Platinum Resistance Thermometer (PRT)	5615	808926			

Support Equipment : - Ice point Unit, ID No.: ana. 614/21

3. This certificate is traceable to International System of Units (SI Units).

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibrated item : Good

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment



Calibration Report

Certificate No.: 2300368-001-01
Equipment: Liquid-in-Glass Thermometer
Type: Total Immersion
Range: -1.9 to 101.1 °C
Resolution: 0.1 °C
ID No.: LABE 16/1
Serial No.: 43560
Manufacturer: Precision
Date of Calibration: 15 November 2022

Page 3 of 3

Calibration point: 3.0, 25.0 and 50.0 °C
Calibration result:

Reporting of ice-point or reference point

UUC* Reading (°C)	Standard Temperature/Ice Point (°C)	Correction Value (°C)	Uncertainty ± (°C)
0.0	0.0032	0.0	0.091

Reporting of temperature calibration point

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
25.0	24.9990	0.0	0.088
50.0	49.9943	0.0	0.088

Note

* UUC* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k=2$, providing a level of confidence of approximately 95 %.

----- End -----



COPY

AZ

pH Meter

Model. : SevenCompact S220

Serial No. : B448305208

NSC-TISI-TSI 7025
CALIBRATION 0152

Page 1 of 3

CERTIFICATE OF CALIBRATION

Certificate No. : 23-011524
Sample Code : 23-04833-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : pH Meter
Manufacturer : METTLER TOLEDO Model : SevenCompact S220
Serial No. : B448305208 ID No. : LABE 11/4
Date of Receipt : 01 February 2023 Date of Calibration : 01 February 2023

Condition of Calibration

1. Environment
1.1 Ambient temperature : 25.0 ± 2.5 °C 1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

In house method WI-CL-019: based on direct measurement by using standard voltage calibrator and using certified reference material (CRM).

3. Reference standard / Certified reference material

Instrument	ID No.	Certificate No.	Due Date
3.1 Voltage Calibrator	LB-AMC-01	22E3240	03 October 2023
3.2 Digital Thermometer	LB-TH-33	22-107027	02 October 2023
Certified Reference Material		Lot No.	Expire Date
3.3 Buffer Solution pH 4.008	838357	PH216.L5	15 September 2024
3.4 Buffer Solution pH 6.985	838358	PH107.L5	15 September 2023
3.5 Buffer Solution pH 10.008	838359	PH220.L5	15 September 2023

4. This certificate is traceable to the international system of unit (SI Unit).

- 4.1 Instrument No. 3.1 through Technology Promotion Association (Thailand-Japan).
4.2 Instrument No. 3.2 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.
4.3 Buffer Solution No. 3.3 and No. 3.5 traceable to CPA chem (through primary measurement method-Harned cell using calibrated thermometer, barometer, and nanovoltmeter. Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).
4.4 Buffer Solution No. 3.4 traceable to CPA chem (BIM RefN HI-27 LoIN 04.06.2021 ; BIM RefN HI-28 LoIN 28.05.2021 ; BIM RefN HI-27 LoIN 04.06.2021 ; BIM RefN HI-28 LoIN 28.05.2021 Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Anupong Lakawin Approved by : (Ms. Pawana Pan-on)

Scientist

Issue date : 03 February 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

NSC-TISI-TSI 7025
CALIBRATION 0152

Page 2 of 3

REPORT OF CALIBRATION

Certificate No. : 23-011524
Sample Code : 23-04833-001

Equipment : pH Meter Resolution : 0.01 pH ; 0.1 mV ; 0.1°C
Manufacturer : METTLER TOLEDO Model : SevenCompact S220
Serial No. : B448305208 ID No. : LABE 11/4
Range : -2.000 pH to 20.000 pH ; ± 2000.0 mV ; -5.0°C to 130.0°C

Results of Calibration

Part 1. DC Voltage measurement

pH Meter Serial No. : B448305208

Nominal Value	Applied DC Voltage	Average indicator reading		Uncertainty	Coverage factor
		mV	pH		
0	414.113	414.0	0.00	± 0.083	2.00
4	177.477	177.5	4.00	± 0.083	2.00
7	0.000	0.1	7.00	± 0.083	2.00
10	-177.477	-178.3	10.00	± 0.083	2.00
14	-414.113	-413.8	14.00	± 0.083	2.00

Part 2. Performance of Electrode system

Electrode Manufacturer : METTLER TOLEDO

Model

Electrode Serial No. : 2365921

InLab Expert Pro-ISM


Three-Point Calibration at pH4 and pH7 Percent Slope : 99.6 ; at pH7 and pH10 Percent Slope : 98.4

Standard Buffer Solution	Average indicator reading		Error Value	Uncertainty	Coverage factor
	pH (@ 25 °C)	mV			
4.008	4.01	184.2	0.002	± 0.011	2.00
6.985	6.99	8.9	0.005	± 0.010	2.00
10.008	10.01	-166.8	0.002	± 0.010	2.00

The result expanded uncertainty (U) is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

D.D.





REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 23-011524

Sample Code : 23-04833-001

Equipment : pH Meter (Digital Thermometer with sensor)

Thermometer readout

Manufacturer : METTLER TOLEDO Model : SevenCompact S220

Serial No. : B448305208 ID No. : LABE 11/4

Resolution : 0.1 °C Range : -5.0 °C to 130.0 °C

Thermometer sensor

Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Serial No. : 2365921 ID No. : N/A

Condition of Calibration

1. Environment
 - 1.1 Ambient temperature : 23.0 °C ± 3.0 °C
 - 1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

- 2.1 The calibration use in house method WI-CL-021 : by comparison with standard thermometer
- 2.2 The calibration by comparison unit under calibration (UUC) to the standard thermometer in a calibration bath at the controlled temperature.

2.3 The temperature scale in use of this laboratory is the international temperature scale of 1990 (ITS-90).

3. Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due date
3.1 Platinum Resistance Thermometer	PT-100	RTD-90	22-107027	02 October 2023
3.2 Thermometer Readout	GT-11	LB-TM-33	22-107027	02 October 2023

4. This certificate is traceable to the international system of unit (SI Unit).

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Accreditation Under TLAS Laboratory Calibration No.0152)

5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibration item : Normal

Results of Calibration

Calibration point °C	Average of standard reading °C	Unit under calibration		Expanded uncertainty °C	Coverage factor k
		Immersion depth mm	Average reading °C		
25	25.002	120	25.0	± 0.13	2.00

Notes

- Calibration results without adjustment

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with JGAS M3003

DD

- End of report -

COPY

STANDARD WEIGHT 50 g



Certificate No. : 22-052238
Sample Code : 22-19150-003

Page 1 of 3

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist
Approved by : (Mr. Somchai Neampunt)
Signed for Director

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-007
TEL 02-516-2422
FAX 02-516-6949
Rev.05
CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21



REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Result of Calibration :

☒ Without adjustment

☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
	(mg)	Mass	Uncertainty	Permissible Error	
			(mg)	$\pm$ (mg)	
50 g	-0.324	49.999676 g	0.10	0.30	LABE 10/1

The result expanded uncertainty of measurement U is stated as the standard uncertainty multiplied by the coverage factor $k=2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-084
TEL 02-516-2422
FAX 02-516-6949
Rev.03
CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21



Certificate No. : 22-052238

Sample Code : 22-19150-003

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$, Relative humidity $50\% \pm 10\%$ and air density 1.20 kg/m^3
2. Calibration Method : Direct comparison weighing according to OIML R111-1 : 2004(E)
3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-078366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY

STANDARD WEIGHT 100 g



Certificate No. : 22-052239
Sample Code : 22-19150-004

Page 1 of 3

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-017

TEL 02-516-2422
FAX 02-516-6949
Rev.05

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21



Certificate No. : 22-052239
Sample Code : 22-19150-004

REPORT OF CALIBRATION

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Result of Calibration : ☒ Without adjustment ☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_a) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	$\pm$ (mg)	
100 g	-0.171	99.999829 g	0.16	0.50	LABE 10/2

The result expanded uncertainty of measurement U is stated as the standard uncertainty multiplied by the coverage factor $k = 2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY



Certificate No. : 22-052239

Sample Code : 22-19150-004

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature 20 °C ± 1.5°C, Relative humidity 50% ± 10% and air density 1.18 kg/m³

2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-78	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at :-

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated item :

Type and Nominal Value :	Standard Weight 100 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY

STANDARD WEIGHT 50 g

MSC 7151-T15170025
CALIBRATION 0152

Page 1 of 3

Certificate No. : 22-052237

Sample Code : 22-19150-002

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
689 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

MSC 7151-T15170025
CALIBRATION 0152

Page 2 of 3

Certificate No. : 22-052237

Sample Code : 22-19150-002

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Result of Calibration :

☒ Without adjustment☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
50 g	(mg)	Mass	Uncertainty	Permissible Error	
			(mg)	± (mg)	
	-0.111	49.999889 g	0.10	0.30	LABE 10/4

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY



Certificate No. : 22-052237

Sample Code : 22-19150-002

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature 20 °C ± 1.5°C, Relative humidity 50% ± 10% and air density 1.18 kg/m³
2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at :-

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY

UV/VIS SPECTROPHOTOMETER

Model : UV – 1800

Serial No. : A11635101643CD



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No. BSSC-UV-167/22
Equipment UV/Vis Spectrophotometer
Model UV-1800
Manufacturer Shimadzu
Serial No. A11635101643 CD
ID No. LABE 03/2
Date of receipt 18 May 2022
Date of calibration 18 May 2022
Date of issue 25 May 2022

Customer name Eastern Thai Consulting 1992 Co., Ltd.
Address 683 Moo 11, Sukhaphibarn 8 Rd., Nongkham, Sitracha, Chonburi 20230.

Temperature (23.8-24.5) °C (On site)
Humidity (47.6-48.3) %RH (On site)

Equipment condition Good Operation

Calibration Location Analysis Department.

Calibration Procedure In-house method WI-UV-702-01 based on ASTM E275-01

Traceability Wavelength Accuracy is traceable to certificate No. 96367 and 96366
Photometric Accuracy is traceable to certificate No. 99925 and 100147
96346
Stray Light is traceable to certificate No.
The above certificate are traceable to SI unit through Siam Scientific Ltd.
(UKAS accredited calibration laboratory NO. 06559)

Calibrated by Mr.Kanchit Choolthep

Approved by

Mr.Kanchit Choolthep
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

FM-UV-708-02 Rev.01 (2301/653)



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Number of Page(s) 2 of 3

Certificate No. BSSC-UV-167/22

Calibration Results:
1. Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (nm)
287.71	287.80	0.09	0.18
445.82	445.95	0.13	0.18
536.52	536.60	0.08	0.18
741.02	741.00	-0.02	0.18
879.41	879.40	-0.01	0.18

2. Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (A)
235	0.0000	0.0000	0.0000	0.0075
	0.7311	0.7321	0.0010	0.0075
257	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
313	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
350	0.0000	0.0000	0.0000	0.0075
	0.6306	0.6314	0.0008	0.0075

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

FM-UV-708-02 Rev.01 (2301/653)



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor 7 Rama4 Road
Silom Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Certificate No. BSCC-UV-167122 Number of Page(s) 3 of 3

Calibration Results:

3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5472	0.5481	0.0009	0.0042
	0.7637	0.7636	-0.0001	0.0042
440.0	1.0480	1.0497	0.0017	0.0042
	0.0000	0.0000	0.0000	0.0042
	0.5371	0.5377	0.0006	0.0042
465.0	0.7457	0.7451	-0.0006	0.0042
	1.0233	1.0240	0.0016	0.0042
	CNR	CNR	CNR	CNR
546.1	CNR	CNR	CNR	CNR
	0.0000	0.0000	0.0000	0.0042
	0.5006	0.5006	0.0000	0.0042
590.0	0.6961	0.6944	-0.0017	0.0042
	0.9563	0.9550	-0.0013	0.0042
	CNR	CNR	CNR	CNR
635.0	0.0000	0.0000	0.0000	0.0042
	0.5137	0.5137	0.0000	0.0042
	0.6907	0.6891	-0.0016	0.0042
	0.9533	0.9519	-0.0014	0.0042
	CNR	CNR	CNR	CNR

*CNR = Customer not request

4. Stray Light*

Standard	Wavelength (nm)	Unit Under Calibration(UUC)	Wavelength (nm)	Transmission (%)	Absorbance (A)
cut-off wavelength (nm)	200.9±0.11nm		201.10	0.9543	2.0204

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

End of Certificate

COPY

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

FM-UV-708-02 Rev.01 (23/01/63)

ANALYTICAL BALANCE (DU)

Model. : XS205DU

Serial No. : 1126323724



Certificate No. : 23-006683

Sample Code : 23-02820-006

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkhram,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : 1126323724

ID No. : LABE 05/1

Date of Receipt : 20 January 2023

Date of Calibration : 20 January 2023

Calibrated by Mr. Thanadol Pholthep
Scientist

Issue date : 25 January 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)



Certificate No. : 23-006683

Sample Code : 23-02820-006

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : METTLER TOLEDO
Model : XS205DU
Capacity : Max 81 g / 220 g
Resolution : 0.01 mg / 0.1 mg
Serial No. : 1126323724
ID No. : LABE 05/1

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 80	☐ Before adjustment	☐ After adjustment
☒ No adjustment	Nominal value	40	90
☐ Adjustment	Standard weight	40.000042	60.000045
	Average reading of indicator	40.00015	90.00019
	Standard deviation	0.000004	0.000007
Unit : g	Range : 200	☐ Before adjustment	☐ After adjustment
☒ No adjustment	Nominal value	100	200
☐ Adjustment	Standard weight	100.000022	200.000199
	Average reading of indicator	100.0001	200.0004
	Standard deviation	0.00004	0.00008

COPY



Certificate No. : 23-006683

Sample Code : 23-02820-006

Page 3 of 4

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Test Point	Sensitivity, S	Range :	Test Point	Sensitivity, S
0	0.99800	200	0	0.9980
40	0.99800		100	0.9980
80	0.99800		200	0.9980

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.000000	0.00000	0.00000	0.000090	2.01
0.01	0.0100036	0.01000	0.00000	0.000093	2.01
0.1	0.1000062	0.10000	0.00001	0.000012	2.00
1	1.0000036	1.00001	-0.00001	0.000014	2.00
5	5.0000044	5.00003	-0.00003	0.000020	2.00
10	10.000000	10.00007	-0.00007	0.000032	2.00
20	20.000016	20.00011	-0.00009	0.000036	2.00
50	50.000029	50.00013	-0.00010	0.000067	2.00
100	100.000022	100.00001	-0.00001	0.000016	2.00
150	150.000051	150.00001	0.00000	0.000023	2.00
200	200.000199	200.00003	-0.00001	0.000028	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.



Certificate No. : 23-006683

Sample Code : 23-02820-006

Page 4 of 4

REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighting pan ☐ Circle ☐ Triangular ☒ Rectangular
Test weight : 50 and 100
Unit : g

Range	Position	Reading of indicator	Reading of indicator
80	1	50.00014	100.00001
200	2	50.00014	99.99988
	3	50.00006	100.00000
	4	50.00010	100.00001
	5	50.00017	100.00001
	6	50.00014	100.00001
Maximum difference		0.00008	0.00003

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019
2. This result of calibration was found accurate as shown on date and place of calibration only.
3. Condition of Calibration item: Normal
4. This certification is traceable to the International System of Unit maintained at : -
Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).


5. Reference standard instrument :

Instrument
1) STANDARD WEIGHT 1 mg to 1 kg

Class ID No.
E2 LB-WE-57

Certificate No.
22-060639

Due Date
27 June 2023

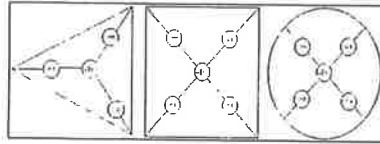

6. Ambient conditions	Min	Max
Temperature (°C)	21.3	22.4
Relative Humidity (%Rh)	39.2	40.4
Air pressure (hPa)	1008.4	1010.1

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-064

TEL 02-516-2422
FAX 02-516-6949
Rev.03

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21

TEL 02-516-2422
FAX 02-516-6949
Rev.03

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21

ANALYTICAL BALANCE

Model. : SECURA224-1S

Serial No. : 0036707137

Certificate No. : 23-006682
Sample Code : 23-02820-005

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : SARTORIUS
Model : SECURA224-IS
Capacity : Max 220 g
Resolution : 0.0001 g
Serial No. : 0036707137
ID No. : LABE 05/2

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 220	☐ Before adjustment	☐ After adjustment
☒ No adjustment	Nominal value	100	200
☐ Adjustment	Standard weight	100.000022	200.000199
	Average reading of indicator	99.9998	199.9999
	Standard deviation	0.00007	0.00007

Unit : .	Range : .	☐ Before adjustment	☐ After adjustment
☐ No adjustment	Nominal value	.	.
☐ Adjustment	Standard weight	.	.
	Average reading of indicator	.	.
	Standard deviation	.	.

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-064

TEL 02-516-2422
FAX 02-516-6949
Rev.03

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21

Certificate No. : 23-006682
Sample Code : 23-02820-005

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : SARTORIUS

Model : SECURA224-IS

Serial No. : 0036707137

ID No. : LABE 05/2

Date of Receipt : 20 January 2023

Date of Calibration : 20 January 2023

Calibrated by : Mr. Thanadol Pholthep
Scientist

Issue date : 25 January 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-07

TEL 02-516-2422
FAX 02-516-6949
Rev.05

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21



Certificate No. : 23-006682

Sample Code : 23-02820-005

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Test Point	Range	Sensitivity, S	Test Point	Range	Sensitivity, S
0	220	0.9980			
100		0.9980			
200		0.9980			

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.0000	0.0000	0.00011	2.04
0.01	0.0100036	0.0100	0.0000	0.00011	2.04
0.1	0.1000062	0.1000	0.0000	0.00011	2.04
1	1.0000036	1.0000	0.0000	0.00011	2.04
2	2.0000128	2.0000	0.0000	0.00011	2.04
5	5.0000044	5.0000	0.0000	0.00011	2.04
10	10.0000000	10.0000	0.0000	0.00011	2.03
20	20.0000016	20.0000	0.0000	0.00012	2.03
50	50.0000029	50.0000	0.0000	0.00013	2.02
100	100.0000022	99.9998	0.0002	0.00017	2.01
200	200.0000199	200.0000	0.0002	0.00028	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY

Certificate No. : 23-006682

Sample Code : 23-02820-005


REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan			Test weight : 100
			Unit : g
Range	Reading of indicator	220	
Position	Reading of indicator		
1	99.9998		
2	100.0001		
3	99.9997		
4	99.9998		
5	99.9998		
6	99.9998		
Maximum difference	0.0003		

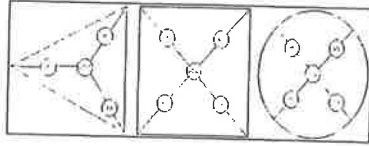

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : -

- Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument

1) STANDARD WEIGHT 1 mg to 1 kg

Class

E2

Certificate No.

22-060639

Due Date

27 June 2023

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY

- End of Report -

AUTOCLAVE

Model : FLS-1000

Serial No. : 55169083



CERTIFICATE OF CALIBRATION

Page 1 of 2

Certificate No. : 22-102070

Sample Code : 22-37024-003

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapiban 8 Rd., Nongkham,

Siracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.

(Autoclave Room)

Equipment : Autoclave

Manufacturer : TOMY

Model : FLS-1000

Serial No. : 55169083

ID No. : LABE 43/2

Date of Receipt : 19 September 2022

Date of Calibration : 19 September 2022

Condition of Calibration

1. Environment
- 1.1 Ambient temperature : Maximum 30.3 °C ; Minimum 28.8 °C
- 1.2 Relative humidity : Maximum 56.1 % ; Minimum 45.1 %
- 1.3 Line voltage supplied : Maximum 227.3 VAC ; Minimum 219.2 VAC

2. Calibration method

The calibration use in-house method; WI-CL-025 based on BS 2646 part 5: 1993 item 3.1.

Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Temperature Data Logger	HiTemp 140	LB-TEM-17	22-089923	31 August 2023
3.2 Temperature Data Logger	HiTemp 140	LB-TEM-16	22-023565	08 March 2023
3.3 Temperature Data Logger	TEMP 1000S	LB-TEM-14	22-089922	31 August 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Sarawoot Thammo

Approved by

(Mr. Somchai Neampunt)

Scientist

Issue date

22 September 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

FM-CI-114

TEL 02-516-2422

FAX 02-516-6949

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

REPORT OF CALIBRATION

Page 2 of 2

Certificate No. : 22-102070

Sample Code : 22-37024-01

Results of Calibration

Resolution : 1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading		Measured Temperature at each positions (°C)			Uncertainty ± (°C)	Coverage factor <i>k</i>
		Temperature (°C)	Pressure (MPa)					
				# 1	# 2 <i>ref</i>	# 3		
121	121	121	0.11	121.81	121.80	121.83	0.64	2.00

2. Characterization results

Calibration Point (°C)	Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
121	0.08	0.12	0.17

Notes

- UUC* = Unit Under Calibration
- The quoted uncertainty includes* Stability of chamber and loading effect in chamber at 20% of uniformity*.
- Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
- Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
- Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
- UUC* reading - the average reading of indicating device that forms the integral part of the autoclave.
- Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -




Figure: Example of sensor installation Positions

- Standard 1 = In the chamber drain, within 100 mm.
- Standard 2 = In the upper half of the chamber.
- Standard 3 = Attached to the load temperature probe, within 20 mm.

COPY

TEL 02-516-2422

FAX 02-516-6949

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

CONTACT@AMARC.CO.

WWW.AMARC.CO.

BOD INCUBATOR

ID No. : LABE 19/2

NSC-TSI-TSI7025
CALIBRATION 0152

Page 1 of 3

Certificate No. : 22-136844

Sample Code : 22-51164-006

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriacha, Cho-buri 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)
Manufacturer : N/A Model : N/A
Serial No. : SS40040277 ID No. : LABE 19/2
Date of Receipt : 21 December 2022 Date of Calibration : 21 December 2022

Condition of Calibration

1. Environment
- | | | | | | | |
|---------------------------|---|---------|-----------|---|---------|-----------|
| 1.1 Ambient temperature | ± | Maximum | 25.1 °C | ± | Minimum | 24.3 °C |
| 1.2 Relative humidity | ± | Maximum | 52.3 % | ± | Minimum | 48.5 % |
| 1.3 Line voltage supplied | ± | Maximum | 223.6 VAC | ± | Minimum | 221.9 VAC |

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-PT100)	LB-DA-11 (RTD-148 to RTD-155, RTD-227)	22-040308	24 April 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Nathanan Phosri
Issue date : 26 December 2022

Approved by :
Signed for Director

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
Rev.01
Effective Date 15/10/21

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

Effective Date 15/10/21

NSC-TSI-TSI7025
CALIBRATION 0152

Page 2 of 3

Certificate No. : 22-136844

Sample Code : 22-51164-006

REPORT OF CALIBRATION

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)										Uncertainty ± (°C)	Coverage factor k
			#1	#2	#3	#4	#5	#6	#7	#8	#9 ^{Ref}	#10		
20	20.0	20.0	19.65	19.56	19.47	19.29	20.96	20.47	20.23	20.58	20.29	20.29	0.35	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.13	1.09	1.90

Notes

- UUC* = Unit Under Calibration

COPY

TEL 02-516-2422

FAX 02-516-6949

Rev.09

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

Effective Date 15/10/21



REPORT OF CALIBRATION

Page 3 of 3


Certificate No. : 22-136844

Sample Code : 22-51164-006

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 60 cm ; D = 70 cm ; H = 124 cm
3. Air valve or fresh air level : Off
4. Fan level : open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC^o reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

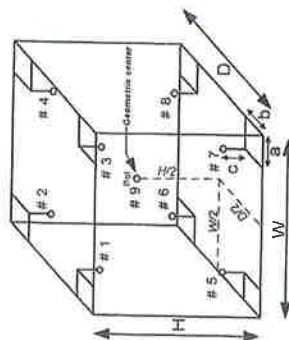Figure. Example of sensor
Installation Positions

- End of Report -

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY

BOD INCUBATOR

ID No. : LABE 19/5



NSC-TSI-11517025
CALIBRATION 0152

Page 3 of 3

REPORT OF CALIBRATION

Certificate No. : 23-040768

Sample Code : 23-16178-002

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 60 cm ; D = 56 cm ; H = 146 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

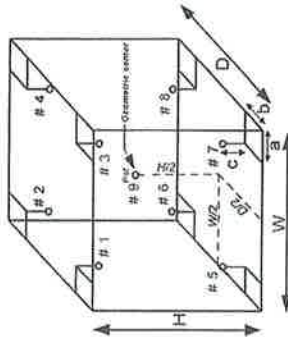


Figure:-Example of sensor
Installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of Report -

COPY

DO

Model : YSI 5000

Serial No. : 18E101961



Harikul Science Co., Ltd.
694 Soi Ratchadaniwet 24, Pracharabamphen,
Samsenok, Huai Khwang, Bangkok 10310
Tel: 0-2274-2456 Fax: 0-2274-2443
Email: info@harikul.com www.harikul.com

CERT No.: HS-T055H

Certificate of Calibration

Calibration Date : 23 Aug 22

Submitted by : Eastern Thai Consulting 1992 Company Limited
683 Moo.11 Sukaphibat8 Rd., Nongkham, Sriracha,
Chonburi 20230

Model : YSI 5000
S/N : 18E101961
Probe : YSI 5010
S/N : 18A100724
ID NO. :
Air Temp ref : S/N. E00522
Barometric ref : S/N. E00522
Water Temp ref : S/N. 11431

Avg Room Temp : 20 °C
Avg Water Temp : 20 °C
Air Pressure : 760.00 mmHg
Salinity : 0 ppt

Technician : Kitipong M.

Calibration Details			
Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.09	(PASS)	-
Measurement 4 (mg/l)	9.10	(PASS)	-
Measurement 5 (mg/l)	9.10	(PASS)	-
Measurement 6 (mg/l)	9.09	(PASS)	-
Measurement 7 (mg/l)	9.09	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.09	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-

Mean Measurement	9.09	mg/l	-
Inaccuracy	0.00	mg/l	-
Overall Status	(PASS)		

Manufacturer Specification	
Accuracy = +/- 0.02 mg/l	

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature

Kitipong M.
Laboratory Manager

Hot Air Oven

Model. : UM 400

Serial No. : 900982

REPORT OF CALIBRATION

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)								Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 ^{Ref}	
85	85.0	85.0	85.18	85.04	84.62	84.82	85.03	85.04	85.00	84.96	85.08	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
85	0.07	0.49	0.68

Notes

UUC* = Unit Under Calibration

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibon 8 Rd., Nongkham,
Siracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Memmert

Model : UM 400

ID No. : LABE 17/1

Date of Receipt : 21 February 2023

Date of Calibration : 21 February 2023

Condition of Calibration

1. Environment	1.1 Ambient temperature	Maximum : 31.2 °C	Minimum : 28.7 °C
	1.2 Relative humidity	Maximum : 50.2 %	Minimum : 40.1 %
	1.3 Line voltage supplied	Maximum : 223.9 VAC	Minimum : 221.5 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data acquisition with sensor (RTD-PT100)	LB-DA-12 (RTD-158 to RTD-166)	22-040312	02 May 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Sarawoot Thammo
Approved by : (Mr. Somchai Neampunt)
Signed for Director

Issue date : 24 February 2023

The uncertainties are for a confidence probability of approximately 95%.
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

COPY

REPORT OF CALIBRATION

Certificate No. : 23-018635
Sample Code : 23-07651-001

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 40 cm ; D = 28 cm ; H = 39 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes " Stability of chamber and loading effect in chamber at 20% of uniformity ".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

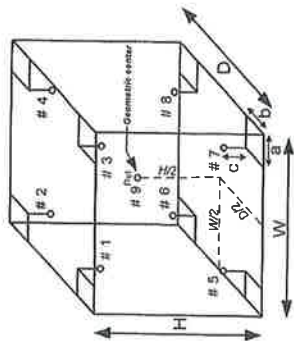


Figure: Example of sensor installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

COPY

LIQUID IN GLASS THERMOMETER

Model : Total immersion

Serial No. : 43560

Calibration Certificate

Certificate No.: 2300368-001-01
Client name: EASTERN THAI CONSULTING 1992 CO., LTD.
Address: 683 Moo 11, Sukhapibam 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Equipment: Liquid-in-Glass Thermometer
Manufacturer: Precision
Model / Type: Total Immersion
Serial No.: 43560
ID No.: LABE 16/1
Order No.: 2300368
Operation No.: 2300368-001
Date of Receipt: 7 November 2022
Date of Calibration: 15 November 2022

Calibrated by Mr.Nuttapol Miyomchet
Specialist
Approved by (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 18 November 2022

The uncertainties are for a confidence probability of approximately 95 %.
This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.



Calibration Report

Certificate No.: 2300368-001-01
Equipment: Liquid-in-Glass Thermometer
Range: -1.9 to 101.1 °C
ID No.: LABE 16/1
Manufacturer: Precision
Date of Calibration: 15 November 2022

Location: Temperature Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature 23 °C ± 3 °C
Relative Humidity 55 % ± 15 %

Condition of this results of Calibration:

1. Calibration Method : - In-house method : W-TE-015 based on ASTM E77-07
- The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
- The temperature Scale in use at this laboratory is the International Temperature Scale of 1990 (ITS-90).

2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
BLACK STACK THERMOMETER	1560/2560	A39258/A39719	PSL-T 0674/65	7-Jun-23	TISTR
Platinum Resistance Thermometer (PRT)	5615	808926			

Support Equipment : - Ice point Unit, ID No.: ana. 614/21

- Low Temperature Bath (Deep Well Compact Bath), Model: 7381, S/N: B53496.
- Low Temperature Bath (Deep Well Compact Bath), Model: 7341, S/N: A5A084.
- High Temperature Bath (Deep Well Compact Bath), Model: 6331, S/N: A5A087.

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
7. Result of Calibration : ☒ Without adjustment ☐ After adjustment

COPY



Calibration Report

Certificate No.: 2300368-001-01
Equipment: Liquid-in-Glass Thermometer
Type: Total Immersion
Range: -1.9 to 101.1 °C
Resolution: 0.1 °C
ID No.: LABE 16/1
Serial No.: 43560
Manufacturer: Precision
Date of Calibration: 15 November 2022

Page 3 of 3

Calibration point: 3.0, 25.0 and 50.0 °C
Calibration result:

Reporting of ice-point or reference point

UUC* Reading (°C)	Standard Temperature/Ice Point (°C)	Correction Value (°C)	Uncertainty ± (°C)
0.0	0.0032	0.0	0.091

Reporting of temperature calibration point

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
25.0	24.9990	0.0	0.088
50.0	49.9943	0.0	0.088

Note

* UUC* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k=2$, providing a level of confidence of approximately 95 %.

----- End -----



COPY

AZ

pH Meter

Model. : SevenCompact S220

Serial No. : B448305208



CERTIFICATE OF CALIBRATION

Page 1 of 3
Certificate No. : 23-011524
Sample Code : 23-04833-001Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siriracha, Chonburi 20230Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)Equipment : pH Meter
Manufacturer : METTLER TOLEDO Model : SevenCompact S220
Serial No. : B448305208 ID No. : LABE 11/4
Date of Receipt : 01 February 2023 Date of Calibration : 01 February 2023

Condition of Calibration

1. Environment
1.1 Ambient temperature : 25.0 ± 2.5 °C 1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

In house method WI-CL-019: based on direct measurement by using standard voltage calibrator and using certified reference material (CRM).

3. Reference standard / Certified reference material

Instrument	ID No.	Certificate No.	Due Date
3.1 Voltage Calibrator	LB-AMC-01	22E3240	03 October 2023
3.2 Digital Thermometer	LB-TH-33	22-107027	02 October 2023
Certified Reference Material			
3.3 Buffer Solution pH 4.008	838357	PH216.L5	15 September 2024
3.4 Buffer Solution pH 6.985	838358	PH107.L5	15 September 2023
3.5 Buffer Solution pH 10.008	838359	PH220.L5	15 September 2023

4. This certificate is traceable to the international system of unit (SI Unit).

- 4.1 Instrument No. 3.1 through Technology Promotion Association (Thailand-Japan).
4.2 Instrument No. 3.2 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.
4.3 Buffer Solution No. 3.3 and No. 3.5 traceable to CPA chem (through primary measurement method-Harned cell using calibrated thermometer, barometer, and nanovoltmeter. Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).
4.4 Buffer Solution No. 3.4 traceable to CPA chem (BIM RefN HI-27 LoIN 04.06.2021 ; BIM RefN HI-28 LoIN 28.05.2021 ; BIM RefN HI-27 LoIN 04.06.2021 ; BIM RefN HI-28 LoIN 28.05.2021 Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Anupong Lakawin Approved by : (Ms. Pawana Pan-on)
Scientist
Issue date : 03 February 2023
The uncertainties are for a confidence probability of approximately 95%.
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-114
TEL 02-516-2422
FAX 02-516-6949
Rev 01
CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date 15/10/23

REPORT OF CALIBRATION

Page 2 of 3
Certificate No. : 23-011524
Sample Code : 23-04833-001Equipment : pH Meter Resolution : 0.01 pH ; 0.1 mV ; 0.1°C
Manufacturer : METTLER TOLEDO Model : SevenCompact S220
Serial No. : B448305208 ID No. : LABE 11/4
Range : -2.000 pH to 20.000 pH ; ± 2000.0 mV ; -5.0°C to 130.0°C

Results of Calibration

Part 1. DC Voltage measurement

pH Meter Serial No. : B448305208

Nominal Value	Applied DC Voltage	Average indicator reading		Uncertainty	Coverage factor
		mV	pH		
0	414.113	414.0	0.00	± 0.083	2.00
4	177.477	177.5	4.00	± 0.083	2.00
7	0.000	0.1	7.00	± 0.083	2.00
10	-177.477	-178.3	10.00	± 0.083	2.00
14	-414.113	-413.8	14.00	± 0.083	2.00

Part 2. Performance of Electrode system

Electrode Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Electrode Serial No. : 2365921


Three-Point Calibration at pH4 and pH7 Percent Slope : 99.6 ; at pH7 and pH10 Percent Slope : 98.4

Standard Buffer Solution	Average indicator reading		Error Value	Uncertainty	Coverage factor
	pH (@ 25 °C)	mV			
4.008	4.01	184.2	0.002	± 0.011	2.00
6.985	6.99	8.9	0.005	± 0.010	2.00
10.008	10.01	-166.8	0.002	± 0.010	2.00

The result expanded uncertainty (U) is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-016
TEL 02-516-2422
FAX 02-516-6949
Rev 09
CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date 15/10/23



REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 23-011524

Sample Code : 23-04833-001

Equipment : pH Meter (Digital Thermometer with sensor)

Thermometer readout

Manufacturer : METTLER TOLEDO Model : SevenCompact S220

Serial No. : B448305208 ID No. : LABE 11/4

Resolution : 0.1 °C Range : -5.0 °C to 130.0 °C

Thermometer sensor

Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Serial No. : 2365921 ID No. : N/A

Condition of Calibration

1. Environment
 - 1.1 Ambient temperature : 23.0 °C ± 3.0 °C
 - 1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

- 2.1 The calibration use in house method WI-CL-021 : by comparison with standard thermometer
- 2.2 The calibration by comparison unit under calibration (UUC) to the standard thermometer in a calibration bath at the controlled temperature.

- 2.3 The temperature scale in use of this laboratory is the international temperature scale of 1990 (ITS-90).

Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due date
3.1 Platinum Resistance Thermometer	PT-100	RTD-90	22-107027	02 October 2023
3.2 Thermometer Readout	GT-11	LB-TM-33	22-107027	02 October 2023

4. This certificate is traceable to the international system of unit (SI Unit).

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Accreditation Under TLAS Laboratory Calibration No.0152)

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibration item : Normal

Results of Calibration

Calibration point °C	Average of standard reading °C	Unit under calibration		Expanded uncertainty °C	Coverage factor k
		Immersion depth mm	Average reading °C		
25	25.002	120	25.0	± 0.13	2.00

Notes

- Calibration results without adjustment

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS MD003

DD

- End of report -

COPY

STANDARD WEIGHT 50 g



Certificate No. : 22-052238
Sample Code : 22-19150-003

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052238
Sample Code : 22-19150-003

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Result of Calibration :

☒ Without adjustment

☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_a) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
	(mg)	Mass	Uncertainty	Permissible Error	
			(mg)	$\pm$ (mg)	
50 g	-0.324	49.999676 g	0.10	0.30	LABE 10/1

The result expanded uncertainty of measurement U is stated as the standard uncertainty multiplied by the coverage factor $k=2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY



Certificate No. : 22-052238

Sample Code : 22-19150-003

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$, Relative humidity $50\% \pm 10\%$ and air density 1.20 kg/m^3
2. Calibration Method : Direct comparison weighing according to OIML R111-1 : 2004(E)
3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-078366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY

STANDARD WEIGHT 100 g



Certificate No. : 22-052239
Sample Code : 22-19150-004

Page 1 of 3

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-017

TEL 02-516-2422
FAX 02-516-6949
Rev.05

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21



Certificate No. : 22-052239
Sample Code : 22-19150-004

REPORT OF CALIBRATION

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Result of Calibration : ☒ Without adjustment ☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_a) of 1.2 kg.m⁻³

Description	Deviation (mg)	Conventional Mass	Expanded Uncertainty (mg)	Maximum Permissible Error $\pm$ (mg)	ID No.
100 g	-0.171	99.999829 g	0.16	0.50	LABE 10/2

The result expanded uncertainty of measurement U is stated as the standard uncertainty multiplied by the coverage factor $k = 2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

[Signature]

[Signature]
COPY

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-064

TEL 02-516-2422
FAX 02-516-6949
Rev.03

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21



Certificate No. : 22-052239

Sample Code : 22-19150-004

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature 20 °C ± 1.5°C, Relative humidity 50% ± 10% and air density 1.18 kg/m³

2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-78	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at :-

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated item :

Type and Nominal Value :	Standard Weight 100 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY

STANDARD WEIGHT 50 g



Certificate No. : 22-052237

Sample Code : 22-19150-002

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

689 Moo 11, Sukhapiban 8 Rd., Nongkham,

Siracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052237

Sample Code : 22-19150-002

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Result of Calibration :

☒ Without adjustment☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional		Expanded	Maximum		ID No.
		Mass			Permissible Error		
				Uncertainty	± (mg)		
	(mg)			(mg)			
50 g	-0.111	49.999889 g		0.10	0.30		LABE 10/4

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

NSC-TIS-71517025
CALIBRATION 0152

Certificate No. : 22-052237

Sample Code : 22-19150-002

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature 20 °C ± 1.5°C, Relative humidity 50% ± 10% and air density 1.18 kg/m³
2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at :-

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration


- End of Report -

COPY

UV/VIS SPECTROPHOTOMETER

Model : UV - 1800

Serial No. : A11635101643 CD



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor 7 Rama4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

2 of 3

Certificate No. BSCC-UV-152/23

Calibration Results:

1. Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty ($\pm$ nm)
287.71	287.65	-0.06	0.18
445.82	445.80	-0.02	0.18
536.52	536.35	-0.17	0.18
741.02	740.99	-0.03	0.18
879.41	879.27	-0.14	0.18

2. Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ($\pm$ A)
235	0.0000	0.0000	0.0000	0.0075
257	0.7311	0.7313	0.0002	0.0075
257	CNR	CNR	CNR	CNR
313	CNR	CNR	CNR	CNR
350	0.0000	0.0000	0.0000	0.0075
350	0.6306	0.6314	0.0008	0.0075

*CNR = Customer not request

Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor 7 Rama4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor 7 Rama4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

1 of 3

Number of Page(s)

Certificate No. BSCC-UV-152/23
Equipment UV/Vis Spectrophotometer
Model UV-1800
Manufacturer Shimadzu
Serial No. A11635101643 CD
ID No. N/A
Date of receipt 25 April 2023
Date of calibration 25 April 2023
Date of issue 27 April 2023

Customer name Eastern Thai Consulting 1992 Co., Ltd

Address 683 Moo 11, Sukkaphibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Temperature (22.4-23.1) °C (On site)
Humidity (44.5-45.2) %RH (On site)

Equipment condition Good Operation

Calibration Location Analysis Department

Calibration Procedure In-house method WI-UV-702-01 based on ASTM E275-01

Traceability
Wavelength Accuracy is traceable to certificate No. 94780 and 94775
Photometric Accuracy is traceable to certificate No. 94808 and 100147
Stray Light is traceable to certificate No. 94791
The above certificate are traceable to SI unit through Starna Scientific Ltd.
(UKAS accredited calibration laboratory NO. 0659)

Calibrated by Mr.Pannaphong Phannmekakul

Approved by

Mr.Kanchit Choothep

Technical Manager

Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor 7 Rama4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.



Bara Scientific
SILICON OF SUCCESS

Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor 7 Rama 4 Road
Silom Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Certificate No. **BSCC-UV-152/23** Number of Page(s) **3 of 3**

Calibration Results:

3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ($\pm A$)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5488	0.5508	0.0020	0.0042
	0.7527	0.7535	0.0008	0.0042
	1.0756	1.0758	0.0002	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5391	0.5406	0.0015	0.0042
	0.7355	0.7360	0.0005	0.0042
	1.0509	1.0501	-0.0008	0.0042
465.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
546.1	0.0000	0.0000	0.0000	0.0042
	0.5045	0.5044	-0.0001	0.0042
	0.6884	0.6885	0.0001	0.0042
	0.9816	0.9808	-0.0008	0.0042
590.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
635.0	0.0000	0.0000	0.0000	0.0042
	0.5183	0.5178	-0.0005	0.0042
	0.6864	0.6868	0.0004	0.0042
	0.9747	0.9739	-0.0008	0.0042

*CNR = Customer not request

4. Stray Light*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)	
	Wavelength (nm)	Absorbance (A)
200.75 $\pm$ 0.1 nm	200.72	2.0164

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%
End of Certificate

The above results are valid exclusively for the calibrated item(s) as mention in this report / Certificate
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

COPY

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL21155

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00609553 / 187117 / 01179
ID No.: -

Condition As Found : GOOD

Customer : SAMGSOM CO., LTD.
14 VIBHAVADI RANGSIT ROAD,
CHOMPHON SUB-DISTRICT
CHATUCHAK DISTRICT, BANGKOK 10900
THAILAND.

Location : -
Ambient Temperature : (23.0 $\pm$ 3) °C
Pressure : (101.3 $\pm$ 3) kPa
Relative Humidity : (50.0 $\pm$ 20) %

Received Date : 08 NOVEMBER 2021
Calibration Date : 15 NOVEMBER 2021
Date of Issue : 16 NOVEMBER 2021

Calibrated by : Nathakorn Pisutpaisan

Approved by :


(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL21155

Job No. : VC64AC0067

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL21155

Job No. : VC64AC0067

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL21155
Job No. : VC64AC0067
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL21156

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00609554 / 187118 / 01180
ID No.: -

Condition As Found : GOOD

Customer : SAMGSOM CO., LTD.
14 VIBHAVADI RANGSIT ROAD,
CHOMPHON SUB-DISTRICT
CHATUCHAK DISTRICT, BANGKOK 10900
THAILAND.

Location : -
Ambient Temperature : (23.0 $\pm$ 3) °C
Pressure : (101.3 $\pm$ 3) kPa
Relative Humidity : (50.0 $\pm$ 20) %

Received Date : 08 NOVEMBER 2021
Calibration Date : 15 NOVEMBER 2021
Date of Issue : 16 NOVEMBER 2021

Calibrated by :

Nathakorn Pisutpaisan

Approved by :


(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL21156

Job No. : VC64AC0067

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL21156

Job No. : VC64AC0067

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL21156
Job No. : VC64AC0067
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

Certificate of Calibration

Customer

Name : Sangsom Co., Ltd.
Address : 260 Paholyothin Rd., Samsennai, Phayathai, Bangkok 10400

Certificate No : 22-LXM-239

Request No : Req-2022-1669

Page : 1/2

Unit Under Calibration Details

Instrument Name : Digital Lux Meter
Manufacturer : EXTECH
Model : 407026
Serial Number : Q272147
Resolution : 1 lx
ID Number : -

Range Calibration : 0 to 2000 lx

Instrument Status : Used

Calibration Environment and Details

Temperature : $25\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$
Humidity : $60\text{ \%RH} \pm 20\text{ \%RH}$
Received Date : 06 September 2022
Calibrated Date : 14 September 2022

Calibration Procedure : The measurement was done in accordance with CP-LXM-01

Reference Standard : Photometer and Illuminance Sensor, Serial No.: 30662/2, 30592/2, which was calibrated on 26 October 2021,
Certificate No.: TP-1026-21

Traceability : This Certificate is traceable to International System of Unit (SI) Unit through National Institute of
Metrology (Thailand)

Note

The reported uncertainty is based on a standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Approved By :



Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date :

14 September 2022

Calibration Note

UUC Adjustment : Zero adjustment before use

Certificate No : 22-LXM-239

Request No : Req-2022-1669

Page : 2/2

Result of Calibration :

UUC Range (lx)	Standard (lx)	UUC Reading (lx)	Correction (lx)	Uncertainty (± lx)
2000	0	0	0	0.58
	100	101	-1	1.8 % of Reading
	500	504	-4	
	1000	1007	-7	
	1500	1511	-11	
	2000	1988	12	

End of Certificate

Calibrated By :



Mr. Noppadon Luangart

Certificate of Calibration

Customer

Name : Sangsom Co., Ltd.
Address : 260 Paholyothin Rd., Samsennai, Phayathai, Bangkok 10400

Certificate No : 22-TPM-376

Request No : Req-2022-1674

Page : 1/2

Unit Under Calibration Details

Calibration Parameter	: Temperature	Range Calibration	: 30 °C to 40 °C
Instrument Name	: Area Heat Stress Monitor	Type of Sensor	: RTD
Manufacturer	: Quest Technologies	Sensor Diameter (mm)	: 4.5
Model	: QT-34	Calibration Position (mm)	: 67.5
Serial Number	: TEK120019	Instrument Status	: Used
Resolution	: 0.1 °C		
ID Number	: -		

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 15 %RH
Received Date : 6 September 2022
Calibrated Date : 8 September 2022
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/RTD100, SN: 08000057, ID: 02-TPM Which was calibrated on 10 March 2022, Calibration Certificate No. : QR22-0578

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.: Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Approved By :



Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date :

8 September 2022

Calibration Note

UUC Adjustment : Not Adjust

Certificate No : 22-TPM-376

Request No : Req-2022-1674

Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	30.004	30.2	- 0.2	0.14
	35.003	35.2	- 0.2	0.14
	40.006	40.2	- 0.2	0.14
DRY	30.006	30.2	- 0.2	0.14
	35.006	35.2	- 0.2	0.14
	40.005	40.2	- 0.2	0.14
GLOBE	30.005	30.2	- 0.2	0.14
	35.004	35.2	- 0.2	0.14
	40.004	40.2	- 0.2	0.14

End of Certificate

Calibrated By :



Mr. Sittichok Jirapukdeesakun

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL22281

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00609553 / 187117 / 01179
ID No.: -

Condition As Found : GOOD

Customer : SAMGSOM CO., LTD.
14 VIBHAVADI RANGSIT ROAD,
CHOMPHON SUB-DISTRICT,
CHATUCHAR DISTRICT, BANGKOK 10900
THAILAND.

Location : -
Ambient Temperature : (23.0 $\pm$ 3) °C
Pressure : (101.3 $\pm$ 3) kPa
Relative Humidity : (50.0 $\pm$ 20) %

Received Date : 30 NOVEMBER 2022
Calibration Date : 01 DECEMBER 2022
Date of Issue : 07 DECEMBER 2022

Calibrated by :

Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22281

Job No. : VC65AC0082

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22281

Job No. : VC65AC0082

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22281

Job No. : VC65AC0082

Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.6
C - weight	18.6
Flat	24.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.6	0.7	0.7	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22281

Job No. : VC65AC0082

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22281
Job No. : VC65AC0082
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22281

Job No. : VC65AC0082

Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{cpeak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.9	-0.5	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22281

Job No. : VC65AC0082

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL22282

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00609554 / 187118 / 01180
ID No.: -

Condition As Found : GOOD

Customer : SAMGSOM CO., LTD.
14 VIBHAVADI RANGSIT ROAD,
CHOMPHON SUB-DISTRICT,
CHATUCHAK DISTRICT, BANGKOK 10900
THAILAND.

Location : -
Ambient Temperature : (23.0 $\pm$ 3) °C
Pressure : (101.3 $\pm$ 3) kPa
Relative Humidity : (50.0 $\pm$ 20) %

Received Date : 30 NOVEMBER 2022
Calibration Date : 01 DECEMBER 2022
Date of Issue : 07 DECEMBER 2022

Calibrated by :

Nathakorn Pisutpaisan

Approved by :


(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL22282
Job No. : VC65AC0082
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL22282
Job No. : VC65AC0082
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Continuation of Calibration Certificate

Cert. No. : ACL22282

Job No. : VC65AC0082

Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.0
C - weight	18.1
Flat	23.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.1	0.1	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-0.8	-0.7	-0.7	±5.0

Continuation of Calibration Certificate

Cert. No. : ACL22282

Job No. : VC65AC0082

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL22282

Job No. : VC65AC0082

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.1	0.1	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.1	0.1	± 1.1
69.0	69.1	0.1	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.1	0.1	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.2	0.2	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL22282
Job No. : VC65AC0082
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.1	0.1	-
One	136.4	135.4	-1.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL22282

Job No. : VC65AC0082

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5


12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

ภาคผนวก ง : หนังสืออนุญาตขึ้นทะเบียนห้องปฏิบัติการ
วิเคราะห์เอกชน

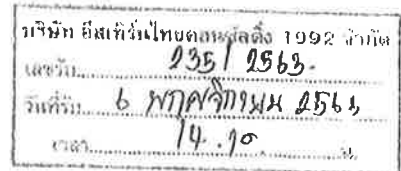

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ เขตราชเทวี
กรุงเทพมหานคร ๑๐๕๐๐

๐๓ พฤศจิกายน ๒๕๖๓

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๕ มิถุนายน ๒๕๖๓

- สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๓๑ ราย
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓๑ ราย
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๑๗ รายการ

ตามหนังสือที่อ้างถึง บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ๖-๐๐๓ สถานที่ตั้งเลขที่ ๖๘๓ หมู่ที่ ๑๑ ถนนสุขาภิบาล ๘ ตำบลหนองขาม อำเภอสรีราชา จังหวัดชลบุรี ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

- ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๓๑ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓๑ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย จำนวน ๔๓ รายการ
อากาศเสีย (ปล่องระบาย) จำนวน ๒๑ รายการ น้ำใต้ดิน จำนวน ๑๙ รายการ ดิน จำนวน ๑๖ รายการ
และสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน ๑๘ รายการ รวมทั้งสิ้นจำนวน ๑๑๗ รายการ ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๕ กรกฎาคม ๒๕๖๖ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกกรมโรงงานอุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งคำขอต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

กองวิจัยและเตือนภัยมลพิษโรงงาน
ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออกเฉียงเหนือ
โทร. ๐ ๓๘๐๕ ๗๒๖๑-๓
โทรสาร ๐ ๓๘๐๕ ๗๒๖๓

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

เลขทะเบียน

ลงวันที่ ๐๓ พฤศจิกายน ๒๕๖๓

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓๑ ราย

๑) น	ทะเบียนเลขที่
๒) น	ทะเบียนเลขที่
๓) น	ทะเบียนเลขที่
๔) น	ทะเบียนเลขที่
๕) น	ทะเบียนเลขที่
๖) น	ทะเบียนเลขที่
๗) น	ทะเบียนเลขที่
๘) น	ทะเบียนเลขที่
๙) น	ทะเบียนเลขที่
๑๐)	ทะเบียนเลขที่
๑๑)	ทะเบียนเลขที่
๑๒)	ทะเบียนเลขที่
๑๓)	ทะเบียนเลขที่
๑๔)	ทะเบียนเลขที่
๑๕)	ทะเบียนเลขที่
๑๖)	ทะเบียนเลขที่
๑๗)	ทะเบียนเลขที่
๑๘)	ทะเบียนเลขที่
๑๙)	ทะเบียนเลขที่
๒๐)	ทะเบียนเลขที่
๒๑)	ทะเบียนเลขที่
๒๒)	ทะเบียนเลขที่
๒๓)	ทะเบียนเลขที่
๒๔)	ทะเบียนเลขที่
๒๕)	ทะเบียนเลขที่
๒๖)	ทะเบียนเลขที่
๒๗)	ทะเบียนเลขที่
๒๘)	ทะเบียนเลขที่
๒๙)	ทะเบียนเลขที่
๓๐)	ทะเบียนเลขที่
๓๑)	ทะเบียนเลขที่

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

เลขทะเบียน

ลงวันที่ ๐๓ พฤศจิกายน ๒๕๖๓

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๑๗ รายการ
น้ำเสีย จำนวน 43 รายการ

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
1	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
2	Arsenic	1) Continuous Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
3	Barium	Digestion, Inductively Coupled Plasma Method ^[4]
4	α -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
5	β -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
6	δ -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
7	γ -BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Membrane Electrode Method ^[4] 2) 5-Day BOD Test, Azide Modification Method ^[4]
9	Cadmium	Digestion, Inductively Coupled Plasma Method ^[4]
10	Chemical Oxygen Demand	Closed Reflux, Titrimetric Method ^[4]
11	cis-Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
12	trans-Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
13	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
14	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[4]
15	Copper	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
16	Cyanide	Distillation, Colorimetric Method ^[4]

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
17	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
18	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
19	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
20	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
21	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
22	Endosulfan sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
23	Endrin aldehyde	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
24	Endrin ketone	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
25	Formaldehyde	Distillation, Colorimetric Method ^[3]
26	Free Chlorine	1) Iodometric Method ^[4] 2) Colorimetric Method ^[c]
27	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
28	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method ^[4]
29	Hexavalent Chromium	Filtration, Colorimetric Method ^[4]
30	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
31	Manganese	Digestion, Inductively Coupled Plasma Method ^[4]
32	Mercury	Cold-Vapor Atomic Absorption Spectrometric Method ^[4]
33	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
34	Oil and Grease	Partition-Gravimetric Method ^[4]
35	pH	Electrometric Method ^[4]

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
36	Phenols	Distillation, Direct Photometric Method ^[4]
37	Sulfide	ZnS Precipitation, Iodometric Method ^[4]
38	Temperature	Laboratory and Field Method ^[4]
39	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Filtration, Colorimetric Method; Calculation ^[4] 2) Digestion, Inductively Coupled Plasma Method; Filtration, Colorimetric Method; Calculation ^[4]
40	Total Dissolved Solids	Dried at 180 °C ^[4]
41	Total Kjeldahl Nitrogen	Macro Kjeldahl Method ^[4]
42	Total Suspended Solids	Dried at 103-105 °C ^[4]
43	Zinc	Digestion, Inductively Coupled Plasma Method ^[4]

อากาศเสีย (ปล่อยระบาย) จำนวน 21 รายการ

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
2	Arsenic	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
3	Cadmium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
4	Carbon Monoxide	Bag, Non-Dispersive Infrared Method ^[5]
5	Chromium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
6	Cobalt	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
7	Copper	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
8	Hydrogen Sulfide	Absorption Sampling, Iodometric Method ^[5]
9	Lead	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
10	Manganese	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
11	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[5]
12	Nickel	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
13	Opacity	Ringelmann's Method ^[1]
14	Oxide of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method ^[5] 2) Instrumental Analyzer Method ^[5]
15	Selenium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
16	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method ^[5] 2) Instrumental Analyzer Method ^[5]
17	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method ^[5]
18	Tin	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
19	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method ^[5]
20	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
21	Xylene	Adsorption Sampling, Gas Chromatographic Method ^[5]

น้ำใต้ดิน จำนวน 19 รายการ

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
1	Antimony	Digestion, Inductively Coupled Plasma Method ^[4]
2	Arsenic	1) Continuous Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
3	Barium	Digestion, Inductively Coupled Plasma Method ^[4]
4	Beryllium	Digestion, Inductively Coupled Plasma Method ^[4]
5	Cadmium	Digestion, Inductively Coupled Plasma Method ^[4]
6	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
7	Cyanide	Distillation, Colorimetric Method ^[4]
8	Hexavalent Chromium	Filtration, Colorimetric Method ^[4]

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
9	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
10	Manganese	Digestion, Inductively Coupled Plasma Method ^[4]
11	Mercury	Cold-Vapor Atomic Absorption Spectrometric Method ^[4]
12	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
13	pH	Electrometric Method ^[4]
14	Phenols	Distillation, Direct Photometric Method ^[4]
15	Selenium	Digestion, Inductively Coupled Plasma Method ^[4]
16	Silver	Digestion, Inductively Coupled Plasma Method ^[4]
17	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Filtration, Colorimetric Method; Calculation ^[4] 2) Digestion, Inductively Coupled Plasma Method; Filtration, Colorimetric Method; Calculation ^[4]
18	Vanadium	Digestion, Inductively Coupled Plasma Method ^[4]
19	Zinc	Digestion, Inductively Coupled Plasma Method ^[4]

ดิน จำนวน 16 รายการ

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
1	Antimony	Digestion, Inductively Coupled Plasma Method ^[6,7]
2	Arsenic	Digestion, Inductively Coupled Plasma Method ^[6,7]
3	Barium	Digestion, Inductively Coupled Plasma Method ^[6,7]
4	Beryllium	Digestion, Inductively Coupled Plasma Method ^[6,7]
5	Cadmium	Digestion, Inductively Coupled Plasma Method ^[6,7]
6	Chromium	Digestion, Inductively Coupled Plasma Method ^[6,7]
7	Hexavalent Chromium	Alkaline Digestion, Colorimetric Method ^[9,10]
8	Lead	Digestion, Inductively Coupled Plasma Method ^[6,7]
9	Manganese	Digestion, Inductively Coupled Plasma Method ^[6,7]
10	Mercury	Digestion, Cold vapor Atomic Absorption Spectrometric Method ^[6,8]
11	Nickel	Digestion, Inductively Coupled Plasma Method ^[6,7]
12	Selenium	Digestion, Inductively Coupled Plasma Method ^[6,7]
13	Silver	Digestion, Inductively Coupled Plasma Method ^[6,7]

14 Trivalent...

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
14	Trivalent Chromium	1) Digestion, Inductively Coupled Plasma Method; Filtration, Colorimetric Method; Calculation ^[6,7] 2) Alkaline Digestion, Colorimetric Method; Calculation ^[9,10]
15	Vanadium	Digestion, Inductively Coupled Plasma Method ^[6,7]
16	Zinc	Digestion, Inductively Coupled Plasma Method ^[6,7]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 18 รายการ


ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
1	Antimony	Digestion, Inductively Coupled Plasma Method ^[6,7]
2	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
3	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
4	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
5	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
6	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
7	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
8	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Digestion, Inductively Coupled Plasma Method ^[6,7]
9	Hexavalent chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7] 2) Alkaline Digestion, Colorimetric Method ^[9,10]

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
10	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
11	Mercury	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Cold Vapor Atomic Absorption Spectrometric Method ^[2,8] 2) Digestion, Cold vapor Atomic Absorption Spectrometric Method ^[6,8]
12	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
13	Molybdenum	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
14	Selenium	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
15	Silver	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
16	Thallium	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
17	Vanadium	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]
18	Zinc	2) Digestion, Inductively Coupled Plasma Method ^[6,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,6,7]

เอกสารอ้างอิง


1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม พ.ศ.2549 เรื่องกำหนดค่าปริมาณ
เขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แก๊สเป็นเชื้อเพลิง.
ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125 ง.

2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม พ.ศ.2548 เรื่อง การกำจัดสิ่งปฏิกูล
หรือวัสดุที่ไม่ใช้แล้ว. ราชกิจจานุเบกษา. 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 11ง.



3 ส.มาคม...

3. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 23rd ed. Washington, DC : APHA, 2017
5. United States Environmental Protection Agency. **Standard of Performance for New Stationary Sources**. 40 CFR Part 60. Appendix A, 2019.
6. United States Environmental Protection Agency. Acid Digestion of Sediments Sludge and Soils. **SW-846 Method 3050B**, 1996.
7. United States Environment Protection Agency, Inductively Coupled Plasma-Atomic Emission spectrometry. **SW-846 Method 6010C**, 2007.
8. United States Environment Protection Agency. Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). **SW-846 Method 7471B**, 2007.
9. United States Environment Protection Agency. Alkaline digestion for Hexavalent Chromium. **SW-846 Method 3060A**, 1996.
10. United States Environment Protection Agency. Chromium. Hexavalent (Colormetric). **SW-846 Method 7196A**, 1992





บันทึก ส่งคลังไทยคดี ๑๑๑๒ ๖๖๖
เลขที่ ๐๔๘/๒๕๖๔
วันที่ ๒๖/๘/๖๔
เวลา ๑๕:๒๐

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๔ สิงหาคม ๒๕๖๔

เรื่อง เปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๕ มิถุนายน ๒๕๖๔

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์
บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด จำนวน ๓ แผ่น

ตามหนังสือที่อ้างถึง บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด ห้องปฏิบัติการวิเคราะห์

เอกชน

ขอเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

ก. ให้ยกเลิกผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย

๑) [REDACTED] ทะเบียนเลขที่ [REDACTED]

๒) [REDACTED] ทะเบียนเลขที่ [REDACTED]

ข. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑ ราย

[REDACTED] ทะเบียนเลขที่ [REDACTED]

ค. ให้เพิ่มเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ ราย

๑) [REDACTED] ทะเบียนเลขที่ [REDACTED]

๒) [REDACTED] ทะเบียนเลขที่ [REDACTED]

๓) [REDACTED] ทะเบียนเลขที่ [REDACTED]

๔) [REDACTED] ทะเบียนเลขที่ [REDACTED]

๕) [REDACTED] ทะเบียนเลขที่ [REDACTED]

ง. ให้เพิ่มขอบข่ายสารมลพิษที่วิเคราะห์ในน้ำใต้ดิน จำนวน ๔๑ รายการ ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์

เอกชน ที่ [REDACTED] ลงวันที่ ๓ พฤศจิกายน ๒๕๖๓ คือในวันที่ ๕ กรกฎาคม ๒๕๖๖

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

กองวิจัยและเตือนภัยมลพิษโรงงาน

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๘๐๕ ๗๒๖๑-๓

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและชนิดสารมลพิษที่วิเคราะห์

บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด


เลขทะเบียน [REDACTED]

ที่ [REDACTED]

ลงวันที่ ๐๔ สิงหาคม ๒๕๖๔

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๕๑ รายการ
น้ำใต้ดิน จำนวน 41 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acetone	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
2	Benzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
3	Bromodichloromethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
4	Bromoform	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
5	Butanol	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
6	Carbon disulfide	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
7	Carbon tetrachloride	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
8	Chlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
9	Chlorodibromomethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
10	Chloroform	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
11	Dichloromethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
12	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
13	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
14	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method

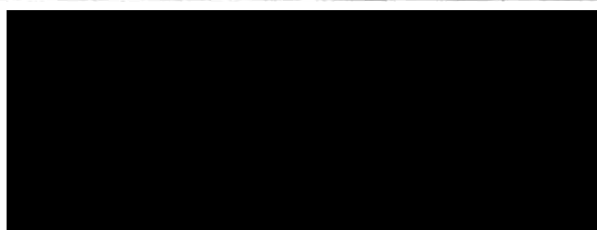

15 1,1-Dichloroethane...


ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
15	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
16	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
17	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
18	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
19	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
20	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
21	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
22	Ethylbenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
23	n-Hexane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
24	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
25	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method
26	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method
27	Styrene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
28	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
29	Tetrachloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
30	Toluene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method

31 1,2,4-Trichlorobenzene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
31	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
32	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
33	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
34	Trichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
35	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
36	Vinyl acetate	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
37	Vinyl chloride	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
38	m-Xylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
39	o-Xylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
40	p-Xylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method
41	Xylene Total	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method

เอกสารอ้างอิง

APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater, 23rd ed. Washington, DC : APHA, 2017



ศูนย์วิจัยและเฝ้าระวังมลพิษโรงงานภาคตะวันออก กองวิจัยและเฝ้าระวังมลพิษโรงงาน กรมโรงงานอุตสาหกรรม โทร ๐ ๓๘๐๕ ๗๖๖๑-๓๑



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๗ ธันวาคม ๒๕๖๕

เรื่อง เปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

อ้างถึง คำขอเปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๔ ตุลาคม ๒๕๖๔

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์
บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด จำนวน ๔ แผ่น

ตามที่อ้างถึง บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน

[REDACTED]

[REDACTED] ขอเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้เพิ่มเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย

๑) [REDACTED] ทะเบียนเลขที่ [REDACTED]


๒) [REDACTED] ทะเบียนเลขที่ [REDACTED]

๒. ให้เพิ่มขอบข่ายสารมลพิษที่วิเคราะห์ในน้ำเสีย จำนวน ๑ รายการ น้ำใต้ดิน จำนวน
๑ รายการ และดิน จำนวน ๔๑ รายการ รวมทั้งสิ้นจำนวน ๔๓ รายการ ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์
เอกชน ที่ [REDACTED] ลงวันที่ ๓ พฤศจิกายน ๒๕๖๓ คือในวันที่ ๕ กรกฎาคม ๒๕๖๖

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



กองวิจัยและเตือนภัยมลพิษโรงงาน
ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๘๐๕ ๗๒๖๑-๓
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและชนิดสารมลพิษที่วิเคราะห์

บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

เลขทะเบียน

ลงวันที่ ๐๗ ธันวาคม ๒๕๖๕

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๔๓ รายการ
น้ำเสีย จำนวน 1 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrophotometer Method ^[1]

น้ำใต้ดิน จำนวน 1 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrophotometer Method ^[1]


ดิน จำนวน 41 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acetone	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
2	Benzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
3	Bromodichloromethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
4	Bromoform	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
5	Butanol	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
6	Carbon disulfide	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
7	Carbon tetrachloride	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]

8 Chlorobenzene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
8	Chlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
9	Chlorodibromomethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
10	Chloroform	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
11	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
12	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
13	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
14	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
15	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
16	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
17	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
18	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
19	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
20	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
21	Ethylbenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
22	n-Hexane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
23	Methylene Chloride	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]


ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
24	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
25	Naphthalene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
26	Nitrobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
27	Styrene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
28	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
29	Tetrachloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
30	Toluene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
31	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
32	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
33	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
34	Trichloroethylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
35	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
36	Vinyl Acetate	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
37	Vinyl Chloride	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
38	m-Xylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
39	o-Xylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
40	p-Xylene	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]
41	Xylene (Total)	Purge and Trap, Gas Chromatographic / Mass Spectrometric Method ^[2,3]

เอกสารอ้างอิง

1. APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 23rd ed. Washington, DC : APHA, 2017
2. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples. SW-846 Method 5035A, 2002.
3. United States Environment Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8260D, 2018.





กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐ ๒ กันยายน ๒๕๖๕

เรื่อง เปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

อ้างถึง คำขอเปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒๐ กรกฎาคม ๒๕๖๕

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์
บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด จำนวน ๕ แผ่น

ตามคำขอที่อ้างถึง บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด ห้องปฏิบัติการวิเคราะห์
เอกชน

ขอเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓ ราย



ทะเบียนเลขที่
ทะเบียนเลขที่
ทะเบียนเลขที่



๒. ให้เพิ่มเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย



ทะเบียนเลขที่
ทะเบียนเลขที่




๓. ให้เพิ่มขอบข่ายสารมลพิษที่วิเคราะห์ในน้ำใต้ดิน จำนวน ๓๘ รายการ และดิน จำนวน
๓๘ รายการ รวมทั้งสิ้นจำนวน ๗๖ รายการ ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ที่ ลงวันที่ ๓ พฤศจิกายน ๒๕๖๓ คือในวันที่ ๕ กรกฎาคม ๒๕๖๖ ทั้งนี้ สามารถยื่น
คำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ท้ายหนังสือนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

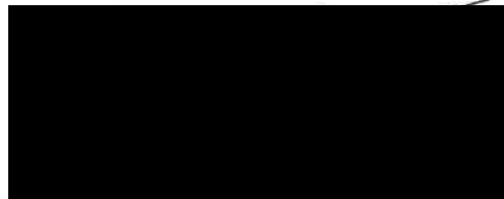


ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๕ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและชนิดสารมลพิษที่วิเคราะห์
บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด เลขทะเบียน ว-๐๐๓
ที่ ออก ๐๓๒๐/ ๑ ๒ ๒ ๔ ๓ ลงวันที่ ๐ ๒ กันยายน ๒๕๖๕

ขอข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๗๖ รายการ
น้ำใต้ดิน จำนวน 38 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
2	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
3	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
4	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
5	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
6	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
7	Benzo[g,h,i]perylene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
8	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
9	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
10	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
11	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
12	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
13	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
14	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
15	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾

16 Di-n-butyl phthalate...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
16	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
17	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
18	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
19	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
20	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
21	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
22	Di-n-octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
23	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
24	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
25	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
26	Hexachloro-1,3-butadiene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
27	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
28	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
29	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
30	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
31	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾
32	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ⁽¹⁾

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
33	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
34	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
35	Phenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
36	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
37	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
38	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]

ดิน จำนวน 38 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
2	Anthracene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
3	Benz(a)anthracene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
4	Benzo(b)fluoranthene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
5	Benzo(k)fluoranthene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
6	Benzo(a)pyrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
7	Benzo[g,h,i]perylene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
8	Bis(2-chloroethyl)ether	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
9	Bis(2-ethylhexyl)phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]

Butyl benzyl...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
10	Butyl benzyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
11	Carbazole	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
12	p-Chloroaniline	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
13	2-Chlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
14	Chrysene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
15	Dibenz(a,h)anthracene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
16	Di-n-butyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
17	2,4-Dichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
18	Diethyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
19	2,4-Dimethylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
20	2,4-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
21	2,6-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
22	Di-n-octyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
23	Fluoranthene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
24	Fluorene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
25	Hexachlorobenzene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
26	Hexachloro-1,3-butadiene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]

27 Hexachlorocyclopentadiene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	Hexachlorocyclopentadiene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
28	Hexachloroethane	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
29	Indeno(1,2,3-cd)pyrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
30	Isophorone	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
31	2-Methylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
32	2-Methylnaphthalene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
33	N-Nitrosodi-n-propylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
34	Phenanthrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
35	Phenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
36	Pyrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
37	2,4,5-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
38	2,4,6-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]

เอกสารอ้างอิง

1. APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 23rd ed. Washington, DC : APHA; 2017
2. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Ultrasonic Extraction. SW-846 Method 3550C, 2007
3. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270E, 2018