

List Certificate of Laboratory Instrument

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Laboratory Instrument for Water Quality Analysis									
1	pH Meter	pH	Mettler-Toledo	Seven Easy S20 / 1230525212	National Food Institute, Ministry of Industry, Thailand	2302181-001-01	24 Mar 23	22 Mar 24	-
2	pH Meter		Mettler-Toledo	SevenCompact S220/ C113432421	National Food Institute, Ministry of Industry, Thailand	2303560-001-01	26 Jun 23	24 Jun 24	-
3	Analytical Balance (Readability 0.01 mg)	Suspended Solids Total Dissolved Solids	Mettler-Toledo	XSR205DU / C210685394	Technology Promotion Association (Thailand-Japan)	23MM113	26 Apr 23	24 Apr 24	-
4	Hot Air Oven		Memmert	UF55 / B216.1666	Technology Promotion Association (Thailand-Japan)	22TM1490	19 Oct 22	18 Oct 23	-
5	Analytical Balance (Readability 0.1 mg)	Fat, Oil & Grease	Mettler-Toledo	XSR204 / C117635043	National Food Institute, Ministry of Industry, Thailand	2302827-001-01	10 May 23	8 May 24	-
6	Digestor Unit	TKN	FOSS TECATOR	2520auto / 91794469	National Food Institute, Ministry of Industry, Thailand	2302413-001-01	30 Mar 23	28 Mar 24	-
7	Distillation Unit (Kjeldahl Method)		FOSS TECATOR	KT8100/ 91889052	FOSS South East Asia	8411	29 May 23	27 May 24	-
8	BOD Incubator	BOD	Arco	UC4-1320 / (UAE.WAO.015/2561)	Technology Promotion Association (Thailand-Japan)	23TM249	15 Feb 23	14 Feb 24	-
9	DO Meter		YSI	4010-2W / 20260326	Technology Promotion Association (Thailand-Japan)	22TW240	27 Oct 22	26 Oct 23	-

Due Date of Calibration\* : Based on the annual calibration plan. At least 1 time per year.

เอกสารไม่ควบคุม

## Calibration Certificate

**Certificate No.:** 2302181-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 5

**Equipment:** pH Meter  
**Manufacturer:** METTLER TOLEDO  
**Model:** SevenEasy pH  
**Serial No.:** 1230525212  
**ID No.:** UAE.WAS.003/2553  
**Order No.:** 2302181  
**Operation No.:** 2302181-001  
**Date of Receipt:** 14 March 2023  
**Date of Calibration:** 24 March 2023

**Calibrated by** Mr.Pheraphat Tuanjit  
Scientist

**Approved by**   
( Mr.Nuttapol Niyomchart )

Specialist, Division of Calibration Laboratory

**Date of Issue:** 24 March 2023

Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2302181-001-01

**Equipment:**

pH Meter

**Resolution:** 0.01 pH ; 1 mV

**Manufacturer:** METTLER TOLEDO

**Model:** SevenEasy pH

**Serial No.:** 1230525212

**Type:** Bench top

**ID No.:** UAE.WAS.003/2553

**Date of Calibration:**

24 March 2023

Page 2 of 5

**Location:**

Chemical Calibration Laboratory, National Food Institute

**Environment Condition:**

**Ambient Temperature:** ( 23.4 ± 1.5 ) °C **Relative Humidity:** ( 52 ± 3 ) %

**Condition of Equipment:**

Good Condition

**Condition of this Results of Calibration**

1. Calibration Method

In house method : W-CC-002 based on direct measurement by using standard voltage calibrator and certified reference material (CRM)

2. Reference Standards / Certified Reference Material

<u>Instruments</u>	<u>Serial / ID No.</u>	<u>Manufacturer</u>	<u>Certificate No.</u>	<u>Due Date</u>
2.1 DC Voltage Calibrator	2709007	Fluke	22E1959	17 June 2023
2.2 Digital Thermometer	2709007	Fluke	CC-650557-01	30 October 2023
2.3 Thermo-Hygro Meter	NFI.BTH003/17	PONPE	TE 650555-01	21 September 2023
<u>Certified Reference Material</u>	<u>Lot. No.</u>	<u>Manufacturer</u>	<u>Ref N</u>	<u>Expire Date</u>
2.4 pH buffer 4.008 (Primary pH buffer Solution)	873608	CPAchem	PH216.L5	16 February 2025
2.5 pH buffer 6.865 (Primary pH buffer Solution)	873609	CPAchem	PH217.L5	16 February 2025
2.6 pH buffer 10.01 (Primary pH buffer Solution)	873611	CPAchem	PH220.L5	16 February 2024
2.7 pH buffer 7.00 (Standard pH buffer Solution)	873612	CPAchem	PH107.L5	16 February 2024

3. This certification is traceable to The International System of Unit (SI Unit)

3.1 Instruments No.2.1	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0008
3.2 Instruments No.2.2	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.3 Instruments No.2.3	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.4 Certified Reference Material No. 2.4 to 2.6	traceable to	Primary measurement method- Harned cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.5 Certified Reference Material No.2.7	traceable to	BIM RefN HI-13 LotN 25.05.2022; BIM RefN HI-16 LotN 02.06.2022; BIM RefN HI-13 LotN 25.05.2022; BIM RefN HI-16 LotN 02.06.2022, the Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

*N. Niyadot*

F-CS-012 Revision: 01 Date: 20-04-65





## Calibration Report

Certificate No.: 2302181-001-01

Equipment:

pH Meter

Resolution: 0.01 pH ; 1 mV

Manufacturer: METTLER TOLEDO

Model: SevenEasy pH

Serial No.: 1230525212

Type: Bench top

ID No.: UAE.WAS.003/2553

Date of Calibration: 24 March 2023

Page 3 of 5

### Calibration Results:

#### 1. Calibration of pH Meter

( Manual Temperature Compensation at 25 °C )

Nominal pH	DC Voltage Standard ( mV )	Average Indicator Reading		Uncertainty ( ±mV )	Coverage Factor ( k )
		mV	pH		
0	414.120	414	0.00	0.58	2.00
2	295.814	296	2.00	0.58	2.00
4	177.464	178	4.00	0.58	2.00
6	59.160	59	6.00	0.58	2.00
7	0.000	0	7.00	0.58	2.00
8	-59.158	-59	8.00	0.58	2.00
10	-177.460	-177	10.00	0.58	2.00
12	-295.811	-296	12.00	0.58	2.00
14	-414.117	-414	14.00	0.58	2.00

#### 2. Calibration of pH Meter with Electrode ( Manual Temperature Compensation at 25 °C )

Equipment: pH Electrode

Type: Combined Electrode

Manufacturer: METTLER TOLEDO

Model: InLab Solids

Serial No.: 1156883

ID.No. N/A

Performance of Electrode system (Three-Point Calibration at pH 4, pH 7 and pH 10)

Certified Value @25 °C (pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty ( ± pH )	Coverage Factor ( k )
	pH	mV			
4.008	4.01	187	-	0.0071	2.00
6.865	6.86	22	97.86	0.0075	2.00
10.010	10.01	-160	97.66	0.0086	2.00
6.985	6.99	14	-	0.0093	2.00

F-CS-012 Revision: 01 Date: 20-04-65

*N. Impudat*





## Calibration Report

**Certificate No.:** 2302181-001-01

**Equipment:** Digital Thermometer with RTD (pH Meter)

Resolution: 0.1 °C Model: SevenEasy pH

Serial No.: 1230525212 ID No.: UAE.WAS.003/2553

Manufacturer: METTLER TOLEDO

**Date of Calibration:** 24 March 2023

Page 4 of 5

**Location:** Chemical Calibration Laboratory, National Food Institute

**Environment Condition:** Ambient Temperature 25 °C ± 1 °C

Relative Humidity 55 % ± 5 %

### Condition of this results of Calibration:

- Calibration Method : - In house method: W-TE-025 by comparison with standard thermometer.
  - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
  - The temperature scale in use at this laboratory is the International Temperature scale of 1990 ( ITS-90 ).

### 2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1521	A85997	TE 660039-01	10-Dec-23	NATIONAL FOOD INSTITUTE
Platinum Resistance Thermometer (PRT)	385	509201			

Support Equipment : - Low Temperature Bath (ISOCAL-6), Model: Europa-6 Plus Basic, S/N: 341592/2

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good
- Result of Calibration : ☒ Without adjustment ☐ After adjustment

*N. mignobert*

F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2302181-001-01

**Equipment:** Digital Thermometer with RTD (pH Meter)

Resolution: 0.1 °C Model: SevenEasy pH

Serial No.: 1230525212 ID No.: UAE.WAS.003/2553

Manufacturer: METTLER TOLEDO

**Date of Calibration:** 24 March 2023

Page 5 of 5

**Calibration point:** 15.0, 25.0 and 30.0 °C

**Calibration result:**

- The probe was immersed in liquid bath or dry bath to a minimum depth of 120 mm.
- Description of probe, model : N/A S/N : N/A
- Dimension of probe : Diameter 3 mm., Length 120 mm.,
- Sheath material : N/A

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.2	14.999	- 0.2	0.12
25.2	24.999	- 0.2	0.12
30.2	29.999	- 0.2	0.12

Note

- UUC\* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

*N. Vinyuth*

F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Certificate

**Certificate No.:** 2303560-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhong, Bangkok 10260

Page 1 of 5

**Equipment:** pH Meter  
**Manufacturer:** Mettler Toledo  
**Model:** Seven Compact S220  
**Serial No.:** C113432421  
**ID No.:** UAE.WAT.009/2564  
**Order No.:** 2303560  
**Operation No.:** 2303560-001  
**Date of Receipt:** 23 June 2023  
**Date of Calibration:** 26 June 2023

**Calibrated by** Mr.Worapob Sooktong  
Scientist

**Approved by** *P. Pheraphat Tuanjit*  
( Mr.Pheraphat Tuanjit ) (for)  
Manager, Division of Calibration Laboratory

**Date of Issue:** 27 June 2023

Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65





## Calibration Report

**Certificate No.:** 2303560-001-01

**Equipment:**

pH Meter

**Resolution:** 0.01 pH ; 1 mV

**Manufacturer:** Mettler Toledo

**Model:** Seven Compact S220

**Serial No.:** C113432421

**Type:** Bench top

**ID No.:** UAE.WAT.009/2564

**Date of Calibration:** 26 June 2023

Page 2 of 5

**Location:** Chemical Calibration Laboratory, National Food Institute

**Environment Condition:** **Ambient Temperature:** ( 24.3 ± 1.5 ) °C **Relative Humidity:** ( 49 ± 3 ) %

**Condition of Equipment:** Good Condition

**Condition of this Results of Calibration**

1. Calibration Method In house method : W-CC-002 based on direct measurement by using standard voltage calibrator and certified reference material (CRM)

2. Reference Standards / Certified Reference Material

Instruments	Serial / ID No.	Manufacturer	Certificate No.	Due Date
2.1 DC Voltage Calibrator	2709007	Fluke	23E2003	14 June 2024
2.2 Digital Thermometer	2709007	Fluke	CC-650557-01	30 October 2023
2.3 Thermo-Hygro Meter	NFI.BTH003/17	PONPE	TE 650555-01	21 September 2023
Certified Reference Material	Lot. No.	Manufacturer	Ref N	Expire Date
2.4 pH buffer 4.008 (Primary pH buffer Solution)	873608	CPAchem	PH216.L5	16 February 2025
2.5 pH buffer 7.00 (Standard pH buffer Solution)	873612	CPAchem	PH107.L5	16 February 2024
2.6 pH buffer 10.01 (Primary pH buffer Solution)	873611	CPAchem	PH220.L5	16 February 2024
2.7 pH buffer 6.865 (Primary pH buffer Solution)	873609	CPAchem	PH217.L5	16 February 2025

3. This certification is traceable to The International System of Unit (SI Unit)

3.1 Instruments No.2.1	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0008
3.2 Instruments No.2.2	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.3 Instruments No.2.3	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.4 Certified Reference Material No. 2.4 to 2.6	traceable to	Primary measurement method- Harned cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.5 Certified Reference Material No.2.7	traceable to	BIM RefN HI-13 LotN 25.05.2022; BIM RefN HI-16 LotN 02.06.2022; BIM RefN HI-13 LotN 25.05.2022; BIM RefN HI-16 LotN 02.06.2022, the Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

*S. Jenghambit*  
27 June 2023

F-CS-012 Revision: 01 Date: 20-04-65



# Calibration Report

Certificate No.: 2303560-001-01

Equipment:

pH Meter

Resolution: 0.01 pH ; 1 mV

Manufacturer: Mettler Toledo

Model: Seven Compact S220

Serial No.: C113432421

Type: Bench top

ID No.: UAE.WAT.009/2564

Date of Calibration: 26 June 2023

Page 3 of 5

## Calibration Results:

### 1. Calibration of pH Meter

( Manual Temperature Compensation at 25 °C )

Nominal pH	DC Voltage Standard ( mV )	Average Indicator Reading		Uncertainty ( ±mV )	Coverage Factor ( k )
		mV	pH		
0	414.121	414	0.00	0.58	2.00
2	295.814	295	2.00	0.58	2.00
4	177.464	177	4.00	0.58	2.00
6	59.160	59	6.00	0.58	2.00
7	0.001	0	7.00	0.58	2.00
8	-59.159	-59	8.00	0.58	2.00
10	-177.461	-177	10.00	0.58	2.00
12	-295.811	-296	12.00	0.58	2.00
14	-414.118	-414	14.00	0.58	2.00

### 2. Calibration of pH Meter with Electrode ( Manual Temperature Compensation at 25 °C )

Equipment: pH Electrode

Type: Combined Electrode

Manufacturer: Mettler Toledo

Model: InLab Expert Pro-ISM

Serial No.: 3114136

ID.No. N/A

Performance of Electrode system (Three-Point Calibration at pH 4, pH 7 and pH 10)

Certified Value @25 °C (pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty ( ± pH )	Coverage Factor ( k )
	pH	mV			
4.008	4.01	177	-	0.0071	2.00
6.865	6.90	9	98.26	0.0074	2.00
10.01	10.01	-168	96.20	0.0085	2.00
6.986	7.02	3	-	0.0093	2.00

*P. Jongsamrit*

27 June 2023





# Calibration Report

**Certificate No.:** 2303560-001-01

**Equipment:** Digital Thermometer with RTD (pH Meter)

**Resolution:** 0.1 °C **Model:** Seven Compact S220

**Serial No.:** C113432421 **ID No.:** UAE.WAT.009/2564

**Manufacturer:** Mettler Toledo

**Date of Calibration:** 26 June 2023

Page 4 of 5

**Location:** Chemical Calibration Laboratory, National Food Institute

**Environment Condition:** Ambient Temperature ( 24.4 ± 1.0 ) °C

Relative Humidity ( 54 ± 2 ) %

## Condition of this results of Calibration:

- Calibration Method :
  - In house method: W-TE-025 by comparison with standard thermometer.
  - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
  - The temperature scale in use at this laboratory is the International Temperature scale of 1990 ( ITS-90 ).

## 2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1523	2933097	PSL-T 1282/65	03-Nov-23	TISTR
Platinum Resistance Thermometer (PRT)	5627A	923972			

Support Equipment : - Low Temperature Bath (ISOCAL-6), Model: Europa-6 Plus Basic, S/N: 341592/2

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibrated item : Good

7. Result of Calibration :



Without adjustment



After adjustment

*P. Janghantit*

27 June 2023





## Calibration Report

**Certificate No.:** 2303560-001-01

**Equipment:** Digital Thermometer with RTD (pH Meter)

Resolution: 0.1 °C Model: Seven Compact S220

Serial No.: C113432421 ID No.: UAE.WAT.009/2564

Manufacturer: Mettler Toledo

**Date of Calibration:** 26 June 2023

Page 5 of 5

**Calibration point:** 15.0, 25.0 and 35.0 °C

**Calibration result:**

- The probe was immersed in liquid bath or dry bath to a minimum depth of 100 mm.
- Description of probe, model : HI11310 S/N : 078743
- Dimension of probe : Diameter 12 mm., Length 175 mm.,
- Sheath material : Plastic

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.0	15.003	0.0	0.099
24.9	25.005	0.1	0.099
34.9	35.005	0.1	0.099

Note - UUC\* : Unit Under Calibration

*P. Pengkhanit*  
27 June 2023

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23MM113  
Page.: 1 of 3

## Certificate of Calibration

**Equipment :** Electronic Balance

**Manufacturer :** Mettler Toledo

**Model :** XSR205

**Serial No. :** C210685394

**ID No. :** UAE.WAO.010/2565

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phakhanong,  
Bangkok 10260

**Location :** Balance Room


**Received order :** 26 April 2023

**Calibration Date :** 26 April 2023

**Ambient Temperature :** 15 °C to 40 °C

**Relative Humidity :** 30 % to 90 %

**Calibrated by :** Man Pattanapongpaiboon

**Approved by :**   
Approved Signatory

( ) Pornthippa Tameyakul  
( ) Malee Butkruea  
(☒) Suwit Imjai

**Issue Date :** 2 May 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม





**Equipment :** Electronic Balance  
**Condition As-Received :** Used Item  
**Reference :** 2304-0459OC-2

**Cert.No.:** 23MM113

**Page:** 2 of 3

**Procedure used :-**

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

**Condition of this result of calibration**

**1. Reference standard instruments:-**

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Test report No.</u>	<u>Due date</u>
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0010-22	20 Jan 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This result of calibration was made on requested at the point specified by customer.
4. This certificate is not certified for any commercial transaction.
5. This certification is traceable to the International System of Unit.

**Result of calibration** ( ) Without Adjustment ( \* ) After Adjustment by Internal Calibration

<b>Range capacity :</b>	0 g to 81 g	<b>Resolution</b>	0.00001 g
	81 g to 220 g	<b>Resolution</b>	0.0001 g

**Before Adjustment :**

<u>Applied Weight</u> ( g )	<u>Balance Reading</u> ( g )	<u>Correction</u> ( g )	<u>Measurement Uncertainty</u> ( ± mg )	<u>Coverage Factor</u> ( k )
80	79.99992	+0.00008	0.15	2.00
200	199.9995	+0.0005	0.29	2.00

**After Adjustment :**

**1. Determination of the standard deviation of weighing machine** ( n = 10 )

<u>Applied Weight</u> ( g )	<u>Standard Deviation of Reading ( g )</u>
80	0.000007
200	0.00004

เอกสารไม่ควบคุม





Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2304-0459OC-2


Cert.No.: 23MM113

Page: 3 of 3

## Result of calibration

### 2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.  
The weighing machine reading error obtained is given in the table

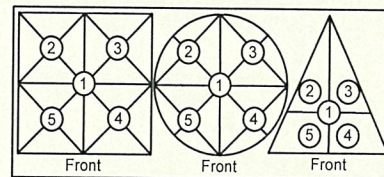

Maximum difference between  
off-center and central loading  
( g )  
0.0001

Position 1	Position 2	Position 3	Position 4	Position 5
( g )	( g )	( g )	( g )	( g )
-0.0001	-0.0001	0.0000	-0.0001	-0.0001

### 3. Departure from nominal value

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
( g )	( g )	( g )	( $\pm$ mg )	( k )
Unload	0.00000	0.00000	0.014	2.11
0.05	0.04999	+0.00001	0.015	2.09
0.1	0.09999	+0.00001	0.015	2.07
1	1.00000	0.00000	0.018	2.04
5	5.00000	0.00000	0.026	2.00
20	20.00002	-0.00002	0.045	2.00
50	50.00002	-0.00002	0.080	2.00
80	80.00002	-0.00002	0.15	2.00
100	100.0000	0.0000	0.17	2.00
150	150.0000	0.0000	0.29	2.00
200	199.9999	+0.0001	0.29	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$  , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม  
Date



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1490

Page : 1 of 3

## Certificate of Calibration

**Equipment :** Hot Air Oven

**Manufacturer :** Memmert

**Model :** UF 55

**Serial No. :** B216.1666

**ID No. :** UAE.WAO.027/2559

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Lab Floor 2

**Received Order :** 19 October 2022

**Calibration Date :** 19 October 2022

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Preecha Hlahib

**Approved by :**

Approved Signatory

- ( ) Pornthippa Tameyakul  
( ) Malee Butkruea  
( ☒ ) Suwit Imjai

**Issue Date :** 31 October 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0046800





**Equipment :** Hot Air Oven  
**Condition As-Received :** Used Item  
**Reference :** 2210-0575OC-1

**Cert. No.:** 22TM1490

**Page :** 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1 ) Data Acquisition	34970A	MY41021843	22LM4	10 Jan 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

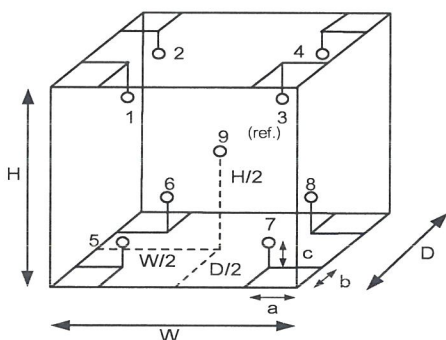

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	29	30
REL.Humid. ( % )	47	40
AC Supply ( Volt )	221	220

Probe Installation Details :		Dimension of Chamber :	
a =	5.0 cm	D =	0.33 m
b =	5.0 cm	W =	0.40 m
c =	5.0 cm	H =	0.40 m
		Capacity =	0.053 m <sup>3</sup>

Ref. Std. ID No.: @ Calibration Point		
Position :	( 104 ) °C	( 140,180 ) °C
1	18-04RTD-01	21-04TC-01
2	18-04RTD-02	21-04TC-02
3	18-04RTD-03	21-04TC-03
4	18-04RTD-04	21-04TC-04
5	18-04RTD-05	21-04TC-05
6	18-04RTD-06	21-04TC-06
7	18-04RTD-07	21-04TC-07
8	18-04RTD-08	21-04TC-08
9 (ref.)	18-04RTD-09	21-04TC-09

เอกสารไม่ควบคุม





Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2210-0575OC-1  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Close

Cert. No.: 22TM1490

Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
104.0	104.0	104.0	0.061	1.3	1.7	0.42	2
140.0	140.0	140.0	0.14	2.3	2.4	1.1	2
180.0	180.0	180.0	0.21	3.5	3.6	1.3	2

Calibration Point ( °C )	Measured Temperature ( °C )								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	103.076	103.876	103.777	104.124	104.667	104.426	104.012	103.928	104.370
140.0	138.199	139.189	138.808	139.550	140.266	139.622	139.293	139.385	140.369
180.0	177.930	179.267	178.643	179.753	181.011	180.093	179.496	179.743	181.278

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation

**UUC\*** : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

a 1133251

## Calibration Certificate

**Certificate No.:** 2302827-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260

Page 1 of 4

**Equipment:** Electronic Balance  
**Manufacturer:** METTLER TOLEDO  
**Model:** XSR204  
**Serial No.:** C117635043  
**ID No.:** UAE.WAS.012/2564  
**Order No.:** 2302827  
**Operation No.:** 2302827-001  
**Date of Receipt:** 10 May 2023  
**Date of Calibration:** 10 May 2023

**Calibrated by** Mr.Manas Somsak  
Specialist

**Approved by**   
( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 18 May 2023

Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95%**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65





# Calibration Report

**Certificate No.:** 2302827-001-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR204

**Resolution:** 0.0001 g

**Serial No.:** C117635043

**ID No.:** UAE.WAS.012/2564

**Capacity:** 220 g

**Date of Calibration:** 10 May 2023

Page 2 of 4

**Environment Condition:** Ambient Temperature 21.4 ± 0.2 °C Relative Humidity: 43.4 ± 0.9 %

**Place of Calibration:** Balance room (Water Analysis Unit), UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

## Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M2304053S	8 April 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 016/23	Quality Reborn	QR23-0489	21 February 2024

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

## Calibration Results:

### 1. Repeatability of Reading:


Nominal Value ( g )	Standard Deviation of Reading ( g )
100	0.000032
200	0.000032


### 2. Off-Center Error:


A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.

Reading obtained is given in the table.







1	2	3	4	5	6	(Maximum Difference)
( g )	( g )	( g )	( g )	( g )	( g )	( g )
100.0002	100.0002	100.0002	100.0002	100.0003	100.0002	0.0001

F-CS-012 Revision: 01 Date: 20-04-65



# Calibration Report

**Certificate No.:** 2302827-001-01

**Equipment:** Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR204

**Resolution:** 0.0001 g

**Serial No.:** C117635043

**ID No.:** UAE.WAS.012/2564

**Capacity:** 220 g

**Date of Calibration:** 10 May 2023

Page 3 of 4

**Calibration Results:** (Continued)

**Calibration Range:** 0 - 200 g

**Calibration Adjustment:** Internal Calibration

## 3. Departure from Nominal Value:

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.00000	0.0000	0.0000	0.000085	2.00
0.01	0.01000	0.0100	0.0000	0.000085	2.00
0.02	0.02001	0.0200	0.0000	0.000085	2.00
0.05	0.05000	0.0500	0.0000	0.000085	2.00
0.1	0.10001	0.1000	0.0000	0.000085	2.00
0.2	0.20001	0.2000	0.0000	0.000085	2.00
0.5	0.50002	0.5000	0.0000	0.000085	2.00
1	1.00000	1.0000	0.0000	0.000086	2.00
2	2.00002	2.0000	0.0000	0.000086	2.00
3	3.00003	3.0000	0.0000	0.000087	2.00
5	5.00002	5.0000	0.0000	0.000087	2.00
10	10.00001	10.0000	0.0000	0.000088	2.00
20	20.00003	20.0000	0.0000	0.000092	2.00
30	30.00004	30.0000	0.0000	0.000098	2.00
40	40.00007	40.0000	0.0000	0.00011	2.00
45	45.00009	45.0001	0.0000	0.00013	2.00

F-CS-012 Revision: 01 Date: 20-04-65

RT

# Calibration Report

**Certificate No.:** 2302827-001-01

**Equipment:** Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR204

**Resolution:** 0.0001 g

**Serial No.:** C117635043

**ID No.:** UAE.WAS.012/2564

**Capacity:** 220 g

**Date of Calibration:** 10 May 2023

Page 4 of 4

**Calibration Results:** (Continued)

**Calibration Range:** 0 - 200 g

**Calibration Adjustment:** Internal Calibration

## 3. Departure from Nominal Value:

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
50	50.00003	50.0000	0.0000	0.00011	2.00
55	55.00005	55.0000	0.0000	0.00012	2.00
60	60.00004	60.0000	0.0000	0.00012	2.00
65	65.00005	65.0000	0.0000	0.00013	2.00
70	70.00006	70.0001	-0.0001	0.00013	2.00
75	75.00008	75.0002	-0.0001	0.00013	2.00
80	80.00007	80.0002	-0.0001	0.00014	2.00
85	85.00009	85.0002	-0.0001	0.00014	2.00
90	90.00010	90.0002	-0.0001	0.00015	2.00
100	100.00006	100.0002	-0.0001	0.00016	2.00
120	120.00009	120.0002	-0.0001	0.00018	2.00
150	150.00009	150.0002	-0.0001	0.00021	2.00
200	200.00016	200.0003	-0.0001	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65





## Verification Certificate

**Certificate No.:** 2302413-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 4

**Equipment:** HEATING BLOCK DIGESTION

**Manufacturer:** FOSS

**Model:** 2520

**Serial No.:** 91794469

**ID No.:** UAE.WAS.011/2560

**Order No.:** 2302413

**Operation No.:** 2302413-001

**Date of Receipt:** 28 March 2023

**Date of Calibration:** 30-31 March 2023

**Calibrated by** Mr.Nuttapol Niyomchat  
Specialist

**Approved by**

( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 10 April 2023

Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95 %.**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65





## Verification Report

**Certificate No.:**

2302413-001-01

**Equipment:**

HEATING BLOCK DIGESTION

Model: 2520

Serial No.: 91794469

Resolution: 1 °C

ID No.: UAE.WAS.011/2560

Manufacturer: FOSS

**Date of Calibration:**

30-31 March 2023

Page 2 of 4

**Location:**

Laboratory Room, NATIONAL FOOD INSTITUTE

**Environment Condition:**

Ambient Temperature ( 25 ± 3 ) °C

Relative Humidity ( 55 ± 15 ) %

Line Voltage ( 220 ± 10 ) Volt

### Condition of this results of Calibration:

1. This instrument was calibrated by insert standard thermocouples type R into its heating block digestion and compared to temperature obtained from reference standards thermometer at calibrated point.

- The temperature scale used was based on ITS - 90 .

- All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with Thermocouple	34970A	MY44045576/MY41194453	TC22/0044	5-May-2023	N.M. Technical Center Laboratory
	Type R	TC#101-103 / CH#101-103			

3. This certificate is traceable to international system of units (SI Units).

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibrated item : Good

UUC\* Description

Time of Record - Hour 30 Minute At 380 °C

7. Result of Calibration :

☒

Without adjustment

☐

After adjustment



## Verification Report

**Certificate No.:**

2302413-001-01

**Equipment:**

HEATING BLOCK DIGESTION

Model: 2520

Serial No.: 91794469

Resolution: 1 °C

ID No.: UAE.WAS.011/2560

Manufacturer: FOSS

**Date of Calibration:**

30-31 March 2023

Page 3 of 4

**Calibration point:**

380 °C

**Calibration result:**

**Reporting of Temperature**

Block No.	UUC* Setting (°C)	UUC* Reading (°C)	Stability (±°C)	Standard Thermometer (°C)	Uncertainty (±°C)
1	380	380	0.96	377.74	2.1
2	380	380	0.40	377.28	2.1
3	380	380	1.18	377.82	2.1
4	380	380	0.44	377.19	1.6
5	380	380	0.11	377.30	1.6
6	380	380	0.14	377.90	1.6
7	380	380	1.17	373.85	2.1
8	380	380	0.33	376.96	2.1
9	380	380	0.14	374.18	2.1
10	380	380	0.96	378.56	2.0
11	380	380	1.04	378.34	2.0
12	380	380	0.35	378.06	2.0
13	380	380	0.48	377.05	1.6
14	380	380	0.38	379.19	1.6
15	380	380	0.50	377.48	1.6
16	380	380	0.48	378.33	1.7
17	380	380	0.71	377.60	1.7
18	380	380	0.35	376.77	1.7
19	380	380	0.84	377.06	1.8
20	380	380	0.41	378.58	1.8

**Note:**

- UUC\* = Unit Under Calibration
- Immersion depth of standard thermometer in tube level high of sand is equal heater plate of UUC.
- Stability = One-half of the greatest maximum difference of measured temperatures at one sensors, for at least half an hour after reaching steady state.

*ATZ*

F-CS-009 Revision: 01 Date: 20-04-65





## Verification Report

**Certificate No.:** 2302413-001-01

**Equipment:** HEATING BLOCK DIGESTION

Model: 2520 Serial No.: 91794469

Resolution: 1 °C ID No.: UAE.WAS.011/2560

Manufacturer: FOSS


**Date of Calibration:** 30-31 March 2023

**Calibration point:** 380 °C

**Calibration result:** Continued

Page 4 of 4

Figure 1. Location of Reference Standard and Block Diagram of Digestion Unit

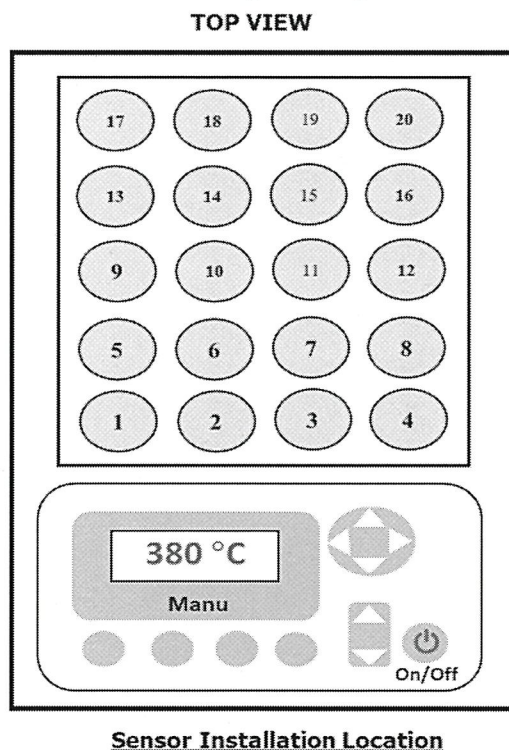

**Sensor Installation Location**

**Note:**

- UUC\* = Unit Under Calibration
- Immersion depth of standard thermometer in tube level high of sand is equal heater plate of UUC.
- Stability = One-half of the greatest maximum difference of measured temperatures at one sensors, for at least half an hour after reaching steady state.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-009 Revision: 01 Date: 20-04-65



# FOSS

## Customer Service Report

FOSS South East Asia

3388 Sirinrat Building, 25th – 26th Floor, Unit No. 3388/90,  
Rama IV Road, Klongton , Klongtoey, Bangkok, Thailand 10110

Report No:

8411

Date:

29/05/23

Customer:

UAE

Address:

Bangkok, Thailand

Instrument:

KT8100

Serial:

91829052

Hours

Travel To Customer

07:00

1.5 hr

Start

08:30

Finish

Labour

09:00

15:00

6 hr.

Travel From Customer

16:30

18:30

2 hr

### Job Type

Application	Special	Standard
Normal	Courtesy Visit	Installation
Distributor	PMA Onboarding	Quote
Internal	Warranty	Repair
Digital Service	Sales Support	Remote
		Training
		In House
		PM
		Other

PO/Quote Number:

if applicable

PMA Type

For score if applicable

Contract No.

if applicable


### Details of Work / Test

### Condition / Status

- นกขาว Function Test เครื่องมือ PM	OK
- ตรวจสอบส่วน Part ของ PM - kit 8100/8200 12 Mo	OK
- ตรวจสอบเครื่องทำความร้อน Heating coil = 32.3 ๐C	OK
- ตรวจสอบหัวฉีด Splash head, Steam Generator	OK
- ตรวจสอบวาล์ว Steam valve = 54.8 ๐C	OK
- ตรวจสอบวาล์ว Condenser Water Cooling Valve A, B = 54.8 ๐C	OK
- ตรวจสอบปริมาณน้ำยา water 100 ml → 100 ml Alkal 10ml → 10 ml	OK
- ตรวจสอบปริมาณน้ำยา 500 ml → 170 ml	OK
- นกขาว Blank = 0.12 Recovery = 100 %	
Instrument Ready for Use	OK
Not OK	If not OK - Comment

Part No:	Batch	Description	Qty
60031807	18.07.2022	Foss PM kit KT8100/8200 12 Mo.	1

I confirm this report is accurate and complete

Signed FOSS		Signed Customer	นางสาว
Name	Patchara Dechaeng	Name	

Would you be willing to participate in a brief survey in order to tell us how we performed?

karnphong.b@uaeconsultant.co.th

เอกสารไม่ควบคุม





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM249

Page : 1 of 3

## Certificate of Calibration

**Equipment :** BOD Incubator

**Manufacturer :** Arco

**Model :** UC4-1320

**Serial No. :** 13URC4S013201

**ID No. :** UAE.WAO.015/2561

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Lab Floor 2

**Received Order :** 15 February 2023  
**Calibration Date :** 15 February 2023  
**Ambient Temperature :** ( 26 ± 10 ) °C  
**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Preecha Hlahib

**Approved by :**

Approved Signatory

- ( ) Pornthippa Tameyakul  
( ✓ ) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 24 February 2023

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0051476



Equipment : BOD Incubator  
Condition As-Received : Used Item  
Reference : 2302-0297OC-1

Cert. No.: 23TM249

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

**1. Reference standard instrument:-**

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1 ) Data Acquisition	34972A	MY57013711	22LM93	02 Jul 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Not Available

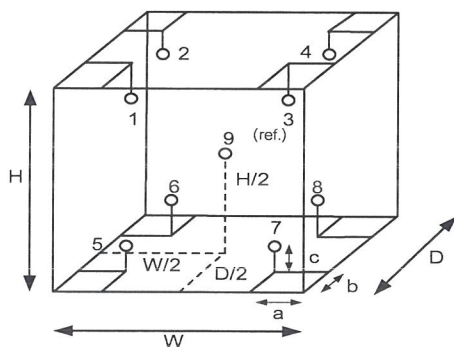

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	29	31
REL.Humid. ( % )	63	67
AC Supply ( Volt )	220	220

Position :	Ref. Std. ID No.:
1	22-18RTD-2/1
2	18RTD-2/2
3	18RTD-2/3
4	18RTD-2/4
5	18RTD-2/5
6	18RTD-2/6
7	18RTD-2/7
8	18RTD-2/8
9 (ref.)	18RTD-2/9

**Probe Installation Details :**

**Dimension of Chamber :**

a =	10	cm	D =	0.62	m
b =	10	cm	W =	1.2	m
c =	10	cm	H =	1.2	m
			Capacity =	0.89	m <sup>3</sup>

เอกสารไม่ควบคุม *Malu.*





**Equipment :** BOD Incubator  
**Condition As-Received :** Used Item  
**Reference :** 2302-0297OC-1  
**Result of Calibration :-** ( \* ) Without Adjustment  
**Function of UUC\* :** Temperature Source  
**Fresh air setting :** Not Available

**Cert. No.:** 23TM249

**Page :** 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
20.0	20.0	19.3	0.32	0.57	1.0	0.60	2

Calibration Point ( °C )	Measured Temperature ( °C )								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
20.0	20.086	19.916	20.386	19.976	19.973	19.838	19.837	19.821	19.949

**Average\* :** The average of 30 values in each position.

**Temperature stability :** One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation :** The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-oOo-

เอกสารไม่ควบคุม

Malu.

a 1149512



**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES**

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

**Cert.No.:** 22TW240

**Page.:** 1 of 2

## Certificate of Testing

<b>Equipment :</b>	DO Meter
<b>Manufacturer :</b>	YSI
<b>Model :</b>	4010-2W
<b>Serial No. :</b>	20260326
<b>ID No. :</b>	UAE.WAO.063/2563
<b>Received Date :</b>	21 October 2022
<b>Test Date :</b>	26 October 2022
<b>Reference :</b>	2210-0734DSC-1
<b>Submitted by :</b>	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
<b>Laboratory Condition :</b>	Temperature ( $25 \pm 5$ ) °C Humidity ( $50 \pm 20$ ) %
<b>Test Procedure :</b>	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
<b>Tested by :</b>	Walalak Sirithean
<b>Approved by :</b>	 Approved Signatory
( ) Malee Butkruea	
( <input checked="" type="checkbox"/> ) Saithip Meangmai	
( ) Warakorn Lerngagtrakul	
<b>Issue Date :</b>	27 October 2022

**เอกสารไม่ควบคุม**





Cert.No.: 22TW240

Page.: 2 of 2

**Condition of this result of calibration**

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

**Result :** Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 20E103527

<b>Titration Method (Azide Modification Method)</b> (mg/L)	<b>DO Meter Reading</b> (mg/L)	<b>Standard Deviation</b> (mg/L)
8.14	8.12	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม *Santhip*

a 1132301