

ภาคผนวกที่ 4

ใบรับรองการสอบเทียบเครื่องมือ



บริษัท เอ็ม อี ที จำกัด MET CO.,LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ. นนทบุรี 11110

36/659 Moo 6 Tambol Bangrakpattana Amphur Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_jj@yahoo.com

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	January 18, 2023
Project Site				Start Time	9:05 AM
Sampler Number	TSP No.2	Transfer Standard Type	Onifice	Stop Time	9:10 AM
Motor Serial Number	BL-02	Calibrator Model	TE-5025A	Person	
Recorder Serial Number	-	Calibrator Serial Number	1		


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric	Start	Stop
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication (inch)	$IC = I[(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(^°K = ^°C+273)	(mmHg)	Meter	Meter
	Positive	Negative	ΔH ₂ O								
5	1.7	1.7	3.4	1.81903	0.93616	1.0	#VALUE!	305.0	757.0		
7	2.8	2.8	5.6	2.33450	1.20555	1.6	1.58	305.0	757.0		
10	4.2	4.3	8.5	2.87613	1.48862	2.7	2.66	305.0	757.0		
13	5.4	5.4	10.8	3.24199	1.67982	3.3	3.26	305.0	757.0		
18	6.6	6.7	13.3	3.59770	1.86573	4.1	4.04	305.0	757.0		

Linear Regression Y ON X : Y= mX + b

1	Slope (m)	1.91345	Linear Equation		Average	305.0	757.0	
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)	1.133	r ²	0.971641	Pstd(mmHg)	760.0
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)	0	r	0.98571852	T _{NTP}	298.0
Result						(Pa/Pstd)*(Tstd/Ta)	0.973192407	
						C=(Pa/Pstd)*(Tstd/Ta)^0.5	0.986505148	

COMMENT

Andersen Instruments, Inc.

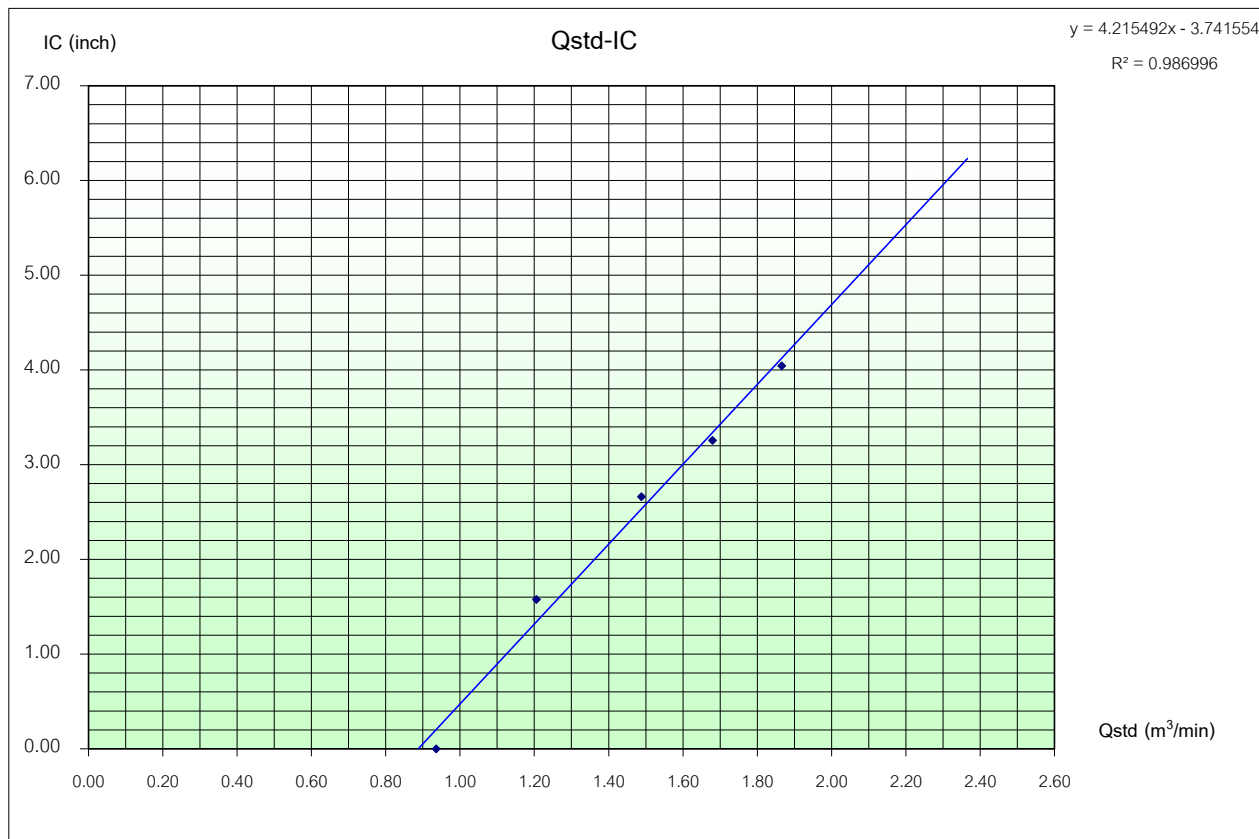

Calibrated By ...

Approved By



บริษัท เอ็ม อี ที จำกัด MET CO.,LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ. นนทบุรี 11110

36/659 Moo 6 Tambol Bangrakpattana Amphur Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_jj@yahoo.com

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	January 18, 2023
Project Site				Start Time	9:15 AM
Sampler Number	TSP No.3	Transfer Standard Type	Onifice	Stop Time	9:20 AM
Motor Serial Number	BL-03	Calibrator Model	TE-5025A	Person	
Recorder Serial Number	-	Calibrator Serial Number	1		


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication (inch)	$IC = I[(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(°K = °C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O								
5	1.2	1.2	2.4	1.52829	0.78422	1.0	0.99	305.0	757.0		
7	2.6	2.7	5.3	2.27111	1.17242	1.1	1.09	305.0	757.0		
10	4.0	4.1	8.1	2.80764	1.45283	2.6	2.56	305.0	757.0		
13	5.1	5.1	10.2	3.15064	1.63209	3.2	3.16	305.0	757.0		
18	6.2	6.2	12.4	3.47384	1.80099	4.0	3.95	305.0	757.0		

Linear Regression Y ON X : Y= mX + b

1	Slope (m)	1.91345	Linear Equation		Average	305.0	757.0	
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)	1.133	r ²	0.930028	Pstd(mmHg)	760.0
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)	0	r	0.96437959	T _{NTP}	298.0
Result						(Pa/Pstd)*(Tstd/Ta)	0.973192407	
						C=(Pa/Pstd)*(Tstd/Ta)^0.5	0.986505148	

COMMENT

Andersen Instruments, Inc.

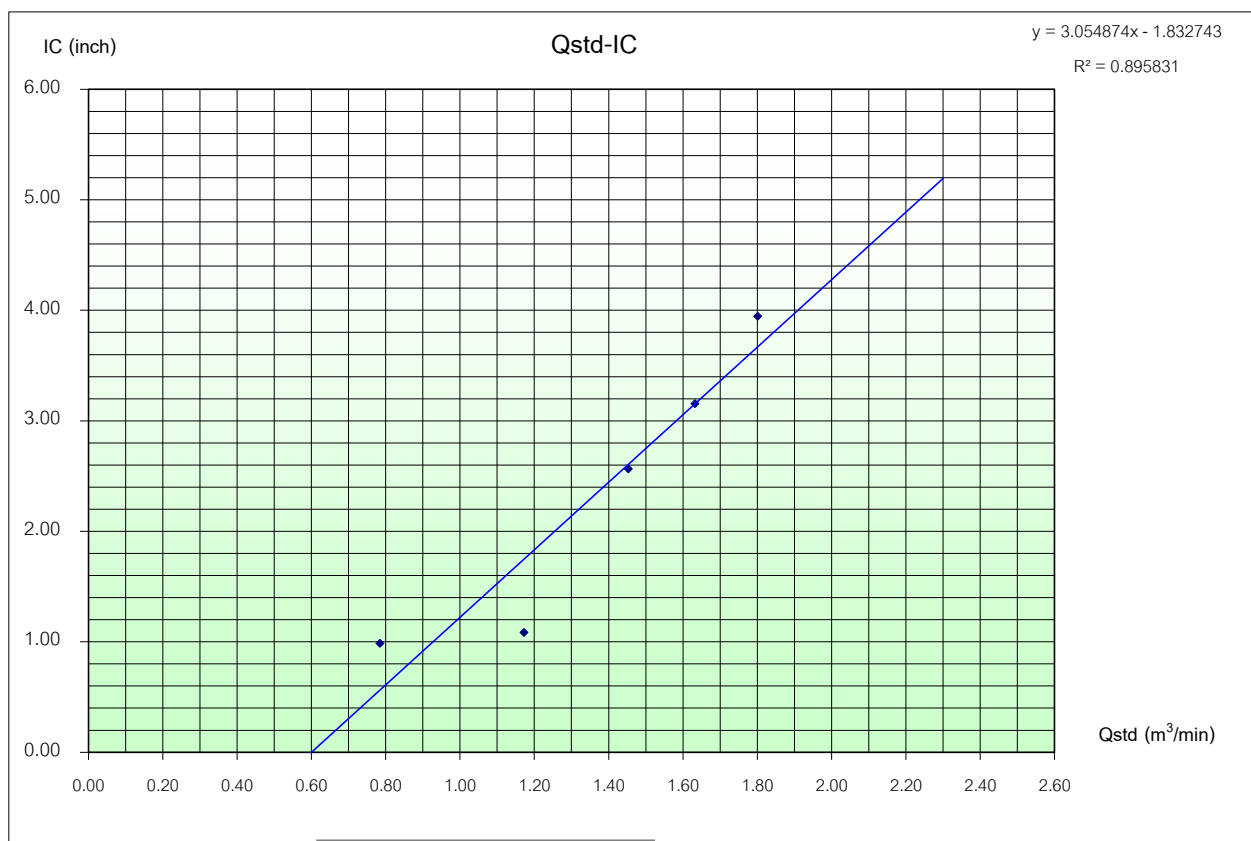

Calibrated By ...

Approved By



บริษัท เอ็ม อี ที จำกัด MET CO.,LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ. นนทบุรี 11110

36/659 Moo 6 Tambol Bangrakpattana Amphur Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_jj@yahoo.com

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	January 18, 2023
Project Site				Start Time	9:25 AM
Sampler Number	TSP No.4	Transfer Standard Type	Onifice	Stop Time	9:30 AM
Motor Serial Number	BL-04	Calibrator Model	TE-5025A	Person	
Recorder Serial Number	-	Calibrator Serial Number	1		


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric	Start	Stop
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$	Sample Flow Rate Indication	$IC = I[(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(°K = °C+273)	Pressure	Meter	Meter
	Positive	Negative	ΔH ₂ O		(m ³ /min)	(inch)			(mmHg)		
5	1.5	1.5	3.0	1.70868	0.87849	1.1	1.09	305.0	757.0		
7	1.7	1.7	3.4	1.81903	0.93616	1.6	1.58	305.0	757.0		
10	2.7	2.7	5.4	2.29243	1.18357	2.5	2.47	305.0	757.0		
13	5.5	5.5	11.0	3.27187	1.69544	3.2	3.16	305.0	757.0		
18	5.9	6.0	11.9	3.40309	1.76402	4.0	3.95	305.0	757.0		

Linear Regression Y ON X : Y= mX + b

1	Slope (m)	1.91345	Linear Equation		Average	305.0	757.0	
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)	1.133	r ²	0.978461	Pstd(mmHg)	760.0
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)	0	r	0.98917188	T _{NTP}	298.0
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5
								0.973192407
								0.986505148

COMMENT

Andersen Instruments, Inc.

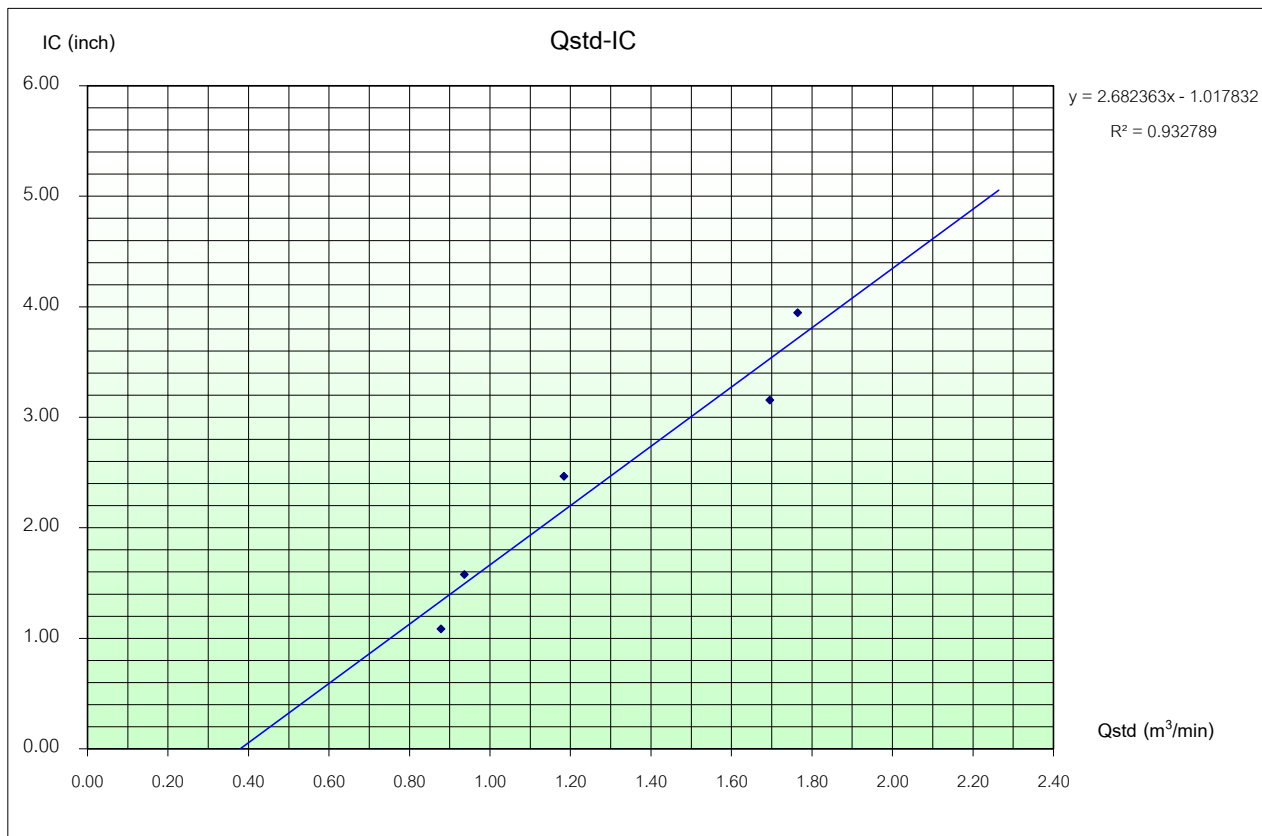

Calibrated By ..

Approved By



บริษัท เอ็ม อี ที จำกัด MET CO.,LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ. นนทบุรี 11110

36/659 Moo 6 Tambol Bangrakpattana Amphur Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_jj@yahoo.com

PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	January 18, 2023
Project Site				Start Time	10:35 AM
Sampler Number	PM-10 No.2	Transfer Standard Type	Onifice	Stop Time	10:40 AM
Motor Serial Number	HVL-02	Calibrator Model	TE-5025A	Person	
Recorder Serial Number	-	Calibrator Serial Number	1		


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication (inch)	$IC = I[(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(°K = °C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O								
5	1.4	1.5	2.9	1.68661	0.86696	1.0	0.99	303.0	758.0		
7	2.3	2.3	4.6	2.12419	1.09564	1.5	1.49	303.0	758.0		
10	3.5	3.5	7.0	2.62038	1.35496	2.1	2.08	303.0	758.0		
13	4.3	4.4	8.7	2.92129	1.51222	2.7	2.67	303.0	758.0		
18	5.5	5.6	11.1	3.29971	1.70999	3.1	3.07	303.0	758.0		

Linear Regression Y ON X : Y= mX + b

1	Slope (m)	1.91345	Linear Equation			r^2	0.950727	Pstd(mmHg)	760.0
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.97505231	T _{NTP}	298.0
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)	0.980910196		
Result						C=(Pa/Pstd)*(Tstd/Ta)^0.5		0.990409106	

COMMENT

Andersen Instruments, Inc.

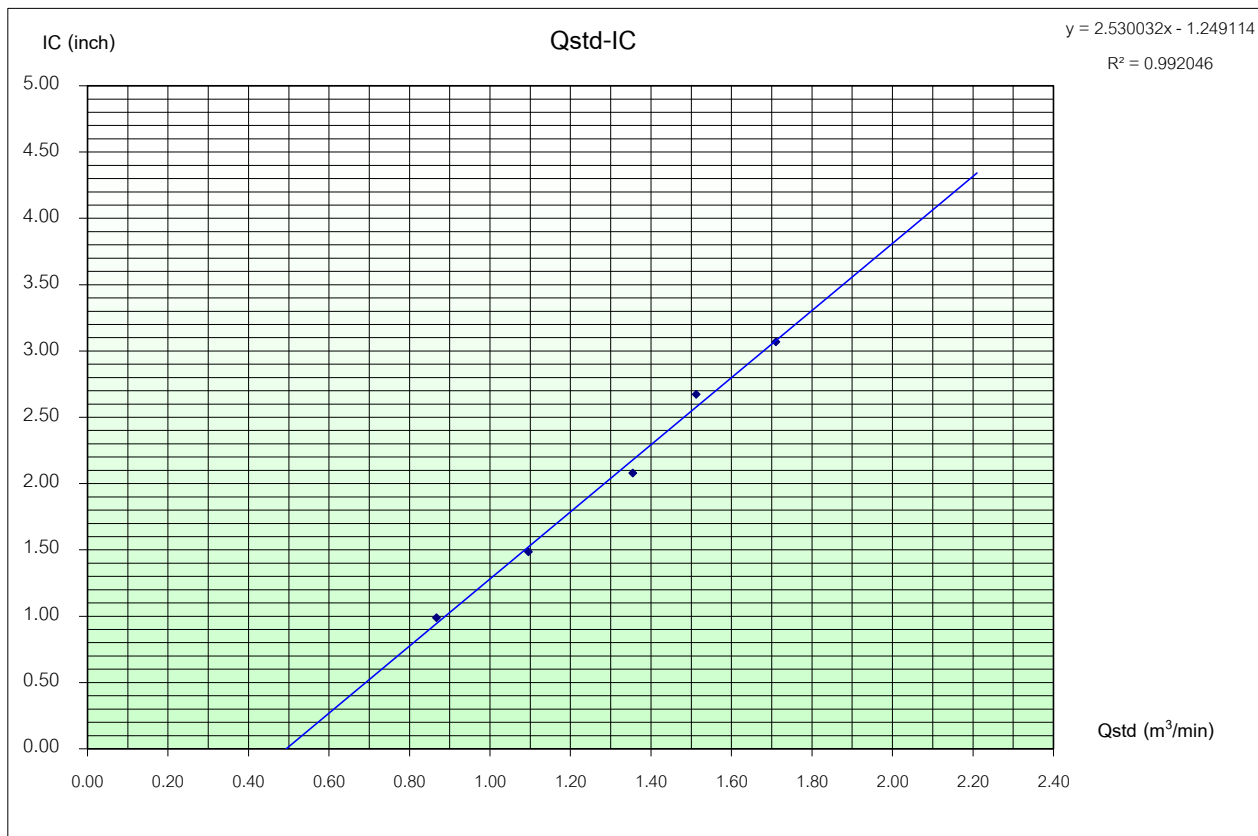

Calibrated By ...

Approved By



บริษัท เอ็ม อี ที จำกัด MET CO.,LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ. นนทบุรี 11110

36/659 Moo 6 Tambol Bangrakpattana Amphur Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_jj@yahoo.com

PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	January 18, 2023
Project Site				Start Time	10:45 AM
Sampler Number	PM-10 No.3	Transfer Standard Type	Onifice	Stop Time	10:50 AM
Motor Serial Number	HVL-03	Calibrator Model	TE-5025A	Person	
Recorder Serial Number	-	Calibrator Serial Number	1		


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication (inch)	$IC = I[(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(°K = °C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O								
5	1.8	1.8	3.6	1.87176	0.96372	1.7	1.68	305.0	757.0		
7	2.8	2.9	5.7	2.35525	1.21640	2.0	1.97	305.0	757.0		
10	4.5	4.5	9.0	2.95952	1.53220	2.8	2.76	305.0	757.0		
13	5.7	5.7	11.4	3.33082	1.72625	3.6	3.55	305.0	757.0		
18	7.0	7.1	14.1	3.70432	1.92145	4.4	4.34	305.0	757.0		

Linear Regression Y ON X : Y= mX + b

1	Slope (m)	1.91345	Linear Equation		Average	305.0	757.0	
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)	1.133	r ²	0.942435	Pstd(mmHg)	760.0
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)	0	r	0.97079091	T _{NTP}	298.0
Result						(Pa/Pstd)*(Tstd/Ta)	0.973192407	
						C=(Pa/Pstd)*(Tstd/Ta)^0.5	0.986505148	

COMMENT

Andersen Instruments, Inc.	
----------------------------	--

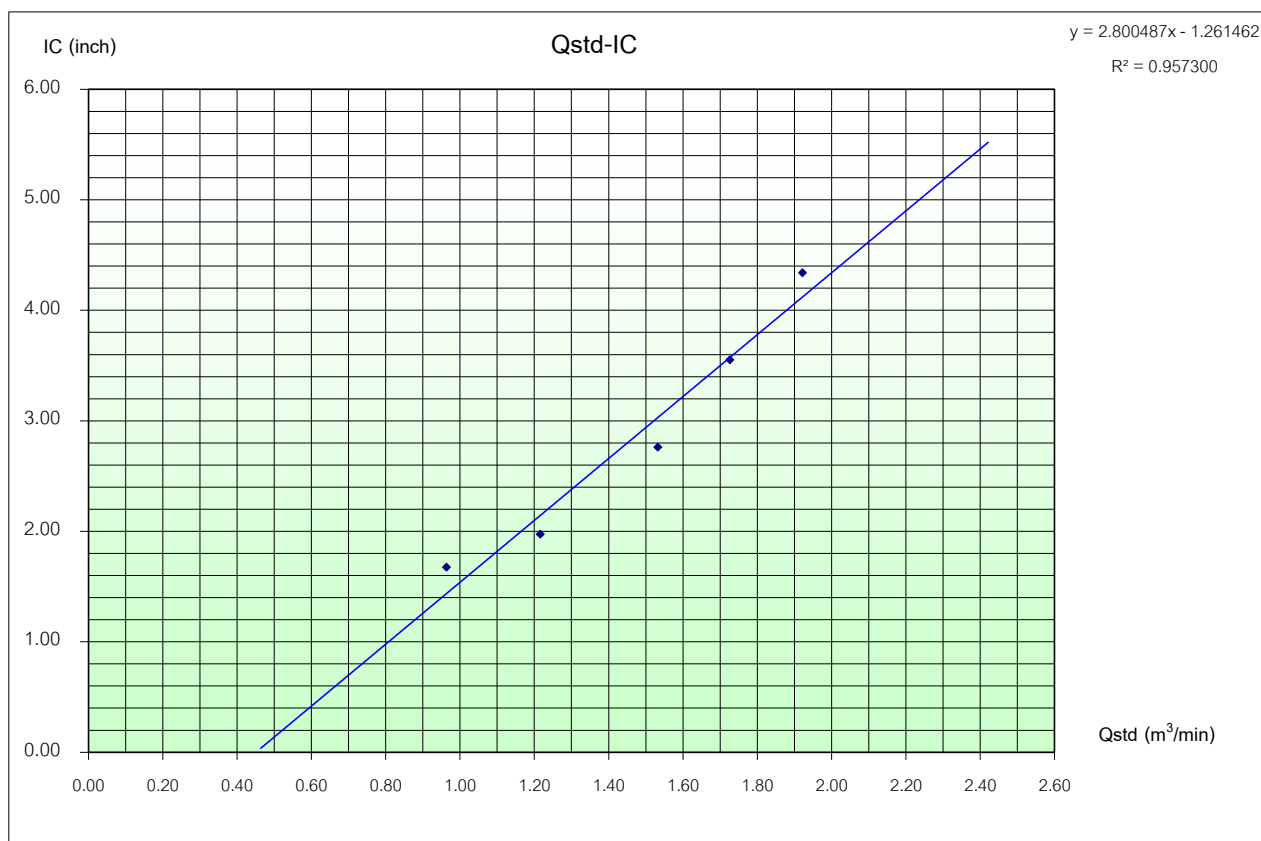

Calibrated By

Approved By



บริษัท เอ็ม อี ที จำกัด MET CO.,LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ. นนทบุรี 11110

36/659 Moo 6 Tambol Bangrakpattana Amphur Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_jj@yahoo.com

PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	January 18, 2023
Project Site				Start Time	10:35 AM
Sampler Number	PM-10 No.2	Transfer Standard Type	Onifice	Stop Time	10:40 AM
Motor Serial Number	HVL-02	Calibrator Model	TE-5025A	Person	
Recorder Serial Number	-	Calibrator Serial Number	1		


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication (inch)	$IC = I[(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(°K = °C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O								
5	1.4	1.5	2.9	1.68661	0.86696	1.0	0.99	303.0	758.0		
7	2.3	2.3	4.6	2.12419	1.09564	1.5	1.49	303.0	758.0		
10	3.5	3.5	7.0	2.62038	1.35496	2.1	2.08	303.0	758.0		
13	4.3	4.4	8.7	2.92129	1.51222	2.7	2.67	303.0	758.0		
18	5.5	5.6	11.1	3.29971	1.70999	3.1	3.07	303.0	758.0		

Linear Regression Y ON X : Y= mX + b

1	Slope (m)	1.91345	Linear Equation		Average	303.0	758.0	
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)	1.133	r ²	0.950727	Pstd(mmHg)	760.0
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)	0	r	0.97505231	T _{NTP}	298.0
Result							$C = (Pa/P_{std}) * (T_{std}/T_a)^{0.5}$	
							0.980910196	
							0.990409106	

COMMENT

Andersen Instruments, Inc.

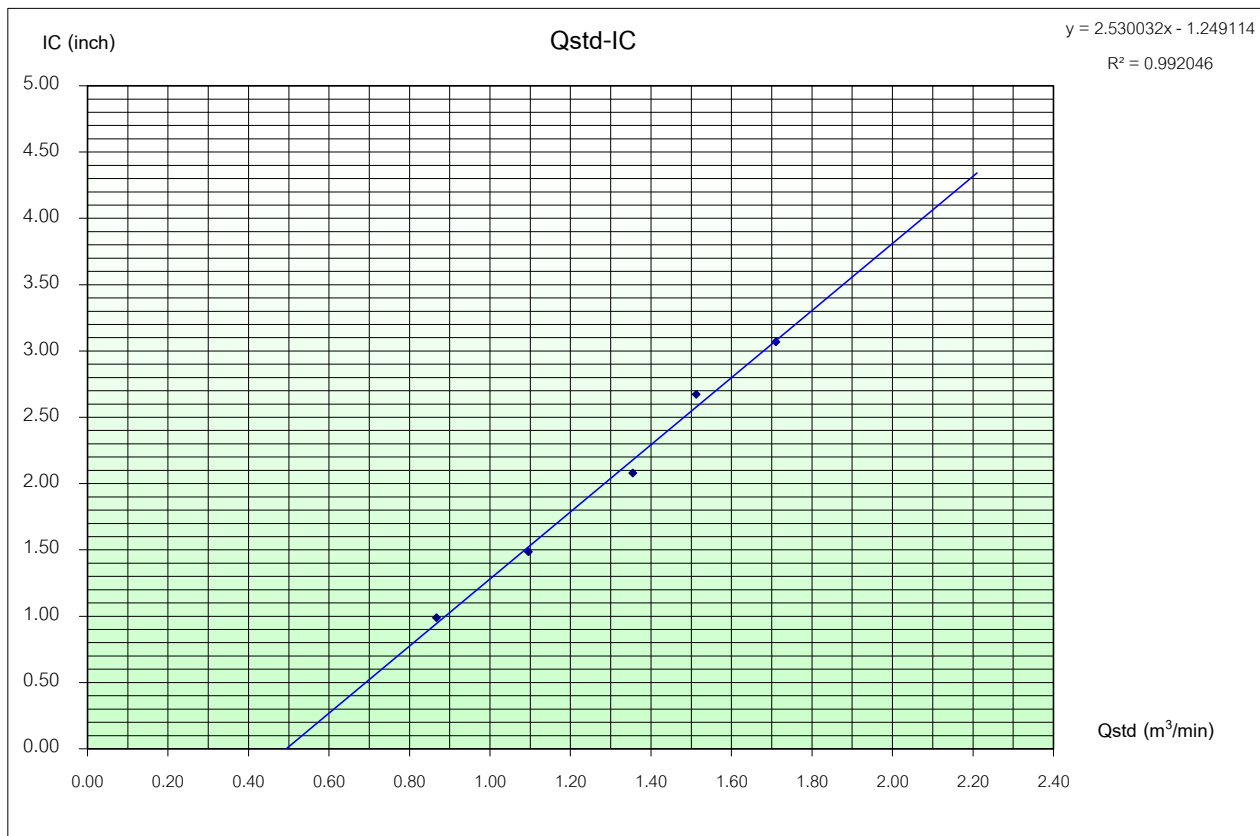

Calibrated By

Approved By



บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD.

บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201

42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 18 January 2023

Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 42C	Manufacturer Thermo Environmental S/N: 72706374
--	--

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 46.05 PPM SO2 Conc 46.01 PPM CO Conc 4,487 PPM Cylinder number CC507080 Expire Date: 23 Jul. 2025

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	395.2	400.0	-1.2
NOx	0.1	0.0	0.1	400.0	400.0	0.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

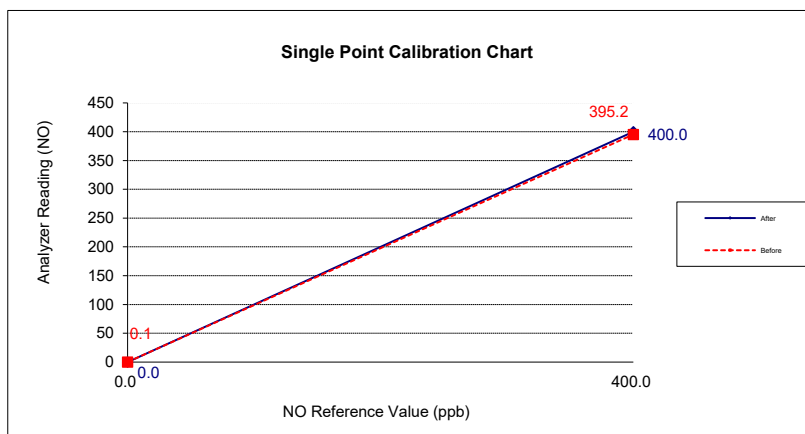

Calibrate I



บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD.

บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201

42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 18 January 2023

Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 40	Manufacturer ECOTECH S/N: E020040
---	--------------------------------------

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	397.6	400.0	-0.6
NOx	0.1	0.0	0.1	400.0	400.0	0.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

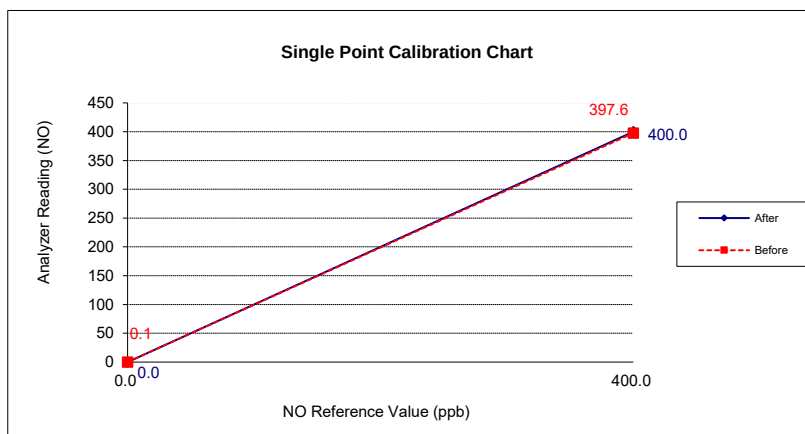

Calibrate I



บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD.

บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201

42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 18 January 2023

Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 42C	Manufacturer Thermo Environmental S/N: 72706371
--	--

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	393.4	400.0	-1.7
NOx	0.1	0.0	0.1	396.7	400.0	-0.8

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

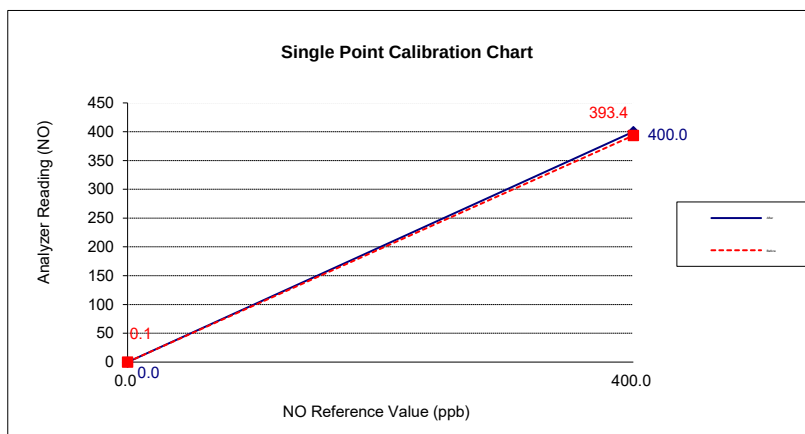

Calibrate I



บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD.

บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201

42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 18 January 2023

Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 42C	Manufacturer Thermo Environmental S/N: 601114773
--	---

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	393.3	400.0	-1.7
NOx	0.1	0.0	0.1	396.4	400.0	-0.9

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

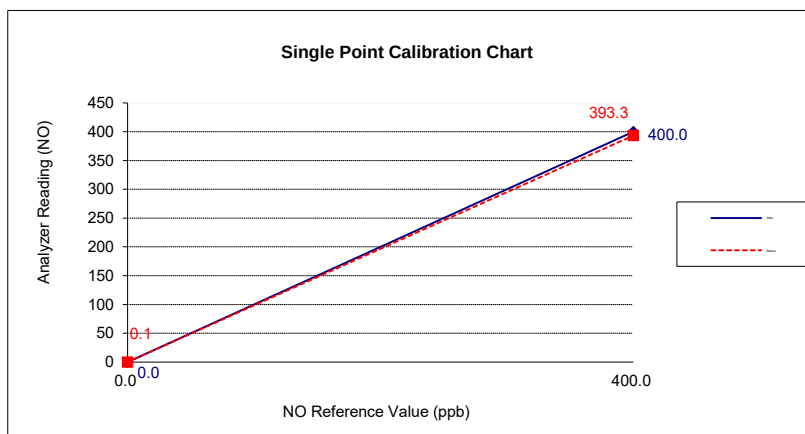

Calibrate I



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201
ENVIR SERVICE CO., LTD.

Analyzer Performance Test

Calibrated Date: 18 January 2023

Instruments Information

Analyzer Type: SO2 Analyzer Model: 43C	Manufacturer Thermo Environmental S/N: 335003719
---	---

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.3	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

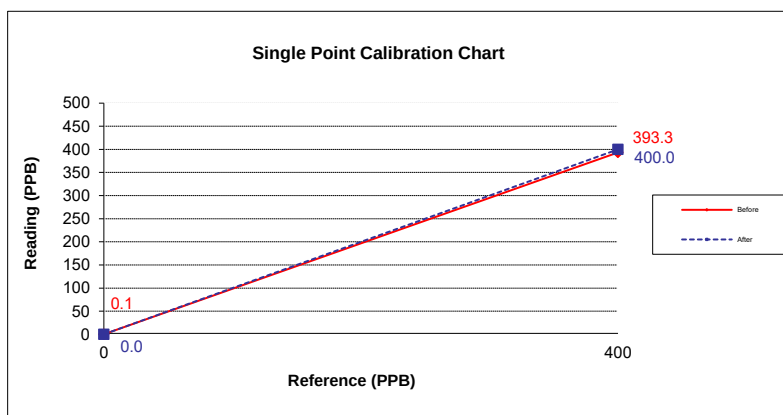

Calibrate By :



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201
ENVIR SERVICE CO., LTD.

Analyzer Performance Test

Calibrated Date: 18 January 2023

Instruments Information

Analyzer Type: SO2 Analyzer Model: 43C	Manufacturer Thermo Environmental S/N: 71354368
---	--

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.4	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

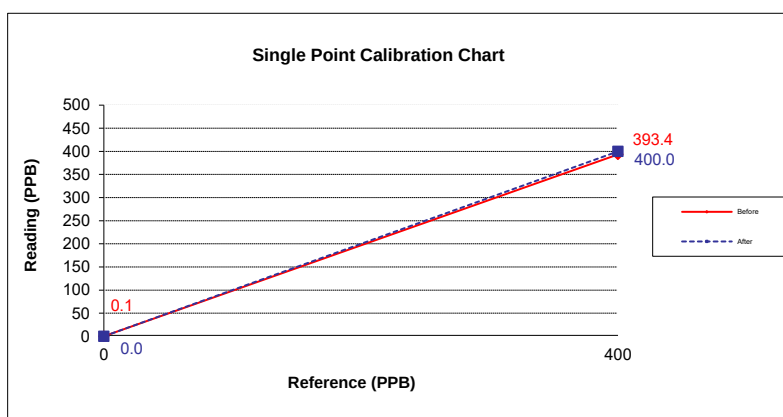

Calibrate By :



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 18 January 2023

Instruments Information

Analyzer Type: SO2 Analyzer Model: 100A	Manufacturer API S/N: 193
--	------------------------------

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.4	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

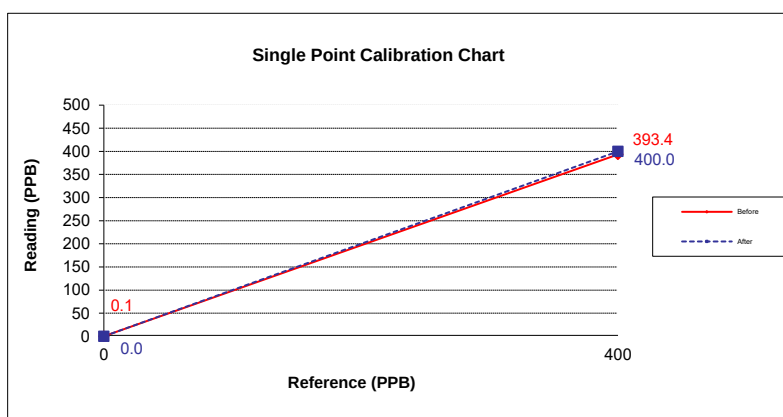

Calibrate By :



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201
ENVIR SERVICE CO., LTD.

Analyzer Performance Test

Calibrated Date: 18 January 2023

Instruments Information

Analyzer Type: SO2 Analyzer Model: 50	Manufacturer ECOTECH S/N: E020050
--	--------------------------------------

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.3	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

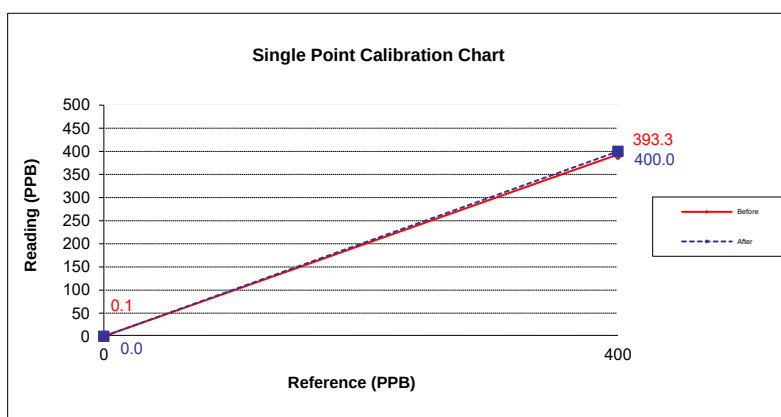

Calibrate By :

Certificate of Calibration

Certificate No. : 66-200067-1

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Electronic Balance
Manufacturer : METTLER TOLEDO Model : AG285
Serial No. : 1122140126 ID No. : MET-EB01/46
Capacity : 210 g Resolution : 0.00001g/81g, 0.0001g/210g

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (26.4 to 26.8) °C
Relative Humidity : (54.9 to 58.8) %
Air Pressure : 1013.0 mbar

Date of Received : 02 March 2023

Date of Calibration : 02 March 2023

Date of Issue : 13 March 2023

Calibrated by :

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02222345	10 Nov 2023	National Institute of Metrology (Thailand), (NIMT)

Approved by :

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-200067-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty $\pm$ (g)
0.01	0.00001	0.000020
0.1	0.00000	0.000019
1	-0.00002	0.000031
5	-0.00004	0.000043
10	-0.00008	0.000054
20	-0.00027	0.000071
50	-0.00059	0.00011
100	-0.0009	0.00023
150	-0.0012	0.00038
200	-0.0019	0.00040

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.43$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A B C D E

0.00055 0.00027 -0.00015 -0.00018 0.00000 g



Repeatability

Load test : 200 g

Stdev. : 0.000053 g

- o0o -



Certificate of Calibration

Certificate No. : 65-400424-2

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)
Manufacturer : Binder Model : ED53
Range : N/A °C Resolution : 1 °C
Serial No. : 13-07419 ID No. : MET-OV02/57

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (27.0 to 28.0) °C
Relative Humidity : (50 to 55) %
Line Voltage : (210.0 to 210.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by :

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400030	65-400272-1	24 Nov 2022	National Institute of Metrology Thailand (NIMT)

Approved

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-400424-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

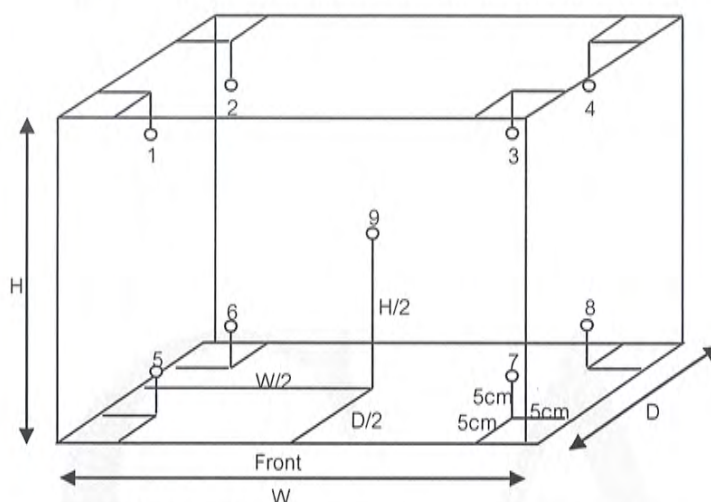

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.40 m

Capacity = 0.05 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104	110	110	105.0	105.0	104.7	105.0	104.4	104.5	104.0	103.7	104.2	0.95
180	184	184	180.8	182.0	179.4	180.8	180.8	180.8	180.3	180.0	180.0	1.2

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104	110	110	1.0	0.2	1.7
180	184	184	2.3	0.3	3.0


Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



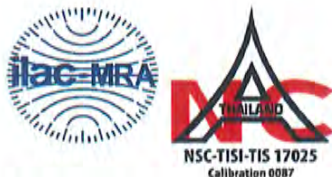

Certificate of Calibration

Equipment:	SPECTROPHOTOMETER	Certificate No.:	C06220514
Model:	SP-2100	Issued Date:	17 October 2022
Serial No. (or ID.):	KJ0G05083001 (MET-SP 01/46)	Job No.:	KSPR2212976
Manufacturer:	Spectrum	Page:	1 of 2
Condition:	In Condition		

Customer: M E T CO.,LTD.
36/659 Moo 6, Tambol Bangrakpattana,
Amphur Bangbuathong, Nonthaburi 11110 Thailand

Environment Condition:

Temperature	23.9	°C	±	0.2	°C
Humidity	60.5	%RH	±	1.8	%RH

Calibration Place: M E T CO.,LTD. (Laboratory Room)
36/659 Moo 6, Tambol Bangrakpattana,
Amphur Bangbuathong, Nonthaburi 11110 Thailand

Calibration By:

Calibration Date: 17 October 2022

The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04

Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 103124 and 103123

The standard for Photometric Certificate No. 9112739

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:
Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 4 nm and UUC at 4 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
334.22	334	0.22	0.59
418.48	419	-0.52	0.59
536.90	537	-0.10	0.59
637.94	638	-0.06	0.59
748.28	748	0.28	0.59
879.70	879	0.70	0.59

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.2899	0.287	0.0029	0.0045
	0.5170	0.514	0.0030	0.0045
	1.0286	1.026	0.0026	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2837	0.280	0.0037	0.0045
	0.5074	0.505	0.0024	0.0045
	1.0071	1.005	0.0021	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2487	0.246	0.0027	0.0045
	0.4593	0.457	0.0023	0.0045
	0.9322	0.929	0.0032	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2434	0.241	0.0024	0.0045
	0.4649	0.462	0.0029	0.0045
	0.9457	0.941	0.0047	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2570	0.256	0.0010	0.0045
	0.5035	0.502	0.0015	0.0045
	1.0022	0.999	0.0032	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2560	0.255	0.0010	0.0045
	0.4968	0.495	0.0018	0.0045
	0.9713	0.969	0.0023	0.0045

The End of Certificate

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: KSPR2212976

ชนิดเครื่องมือ: SPECTROPHOTOMETER

รุ่น: SP-2100

หมายเลขเครื่อง: KJ0G05083001

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
17 Oct 2022			17 Oct 2022		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
☒	☐	1. ความสมบูรณ์เครื่อง	☒	☐	
☒	☐	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	☒	☐	
☒	☐	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swicth)	☒	☐	
☒	☐	4. ปุ่มกด (Keypad)	☒	☐	
☒	☐	5. หน้าจอ (Display, Screen Contrast)	☒	☐	
		Spectrophotometer			
☐	☐	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	☐	☐	
☐	☐	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	☐	☐	
☒	☐	8. ความยาวคลื่น (Wavelength Check)	☒	☐	
☐	☐	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	☐	☐	
☒	☐	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	☒	☐	
☒	☐	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	☒	☐	
		pH Meter and Conductivity Meter			
☐	☐	12. อิเล็กโทรด (Electrode and Connection Cable)	☐	☐	
☐	☐	13. ระดับสารละลายใน Electrode (Level KCl)	☐	☐	
☐	☐	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	☐	☐	
☐	☐	15. ขาจับอิเล็กโทรด (Stand)	☐	☐	
		Turbidimeter			
☐	☐	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	☐	☐	
☐	☐	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่เกิน 3.0)	☐	☐	
		Automatic titrator			
☐	☐	18. สภาพ Piston Burettes	☐	☐	
☐	☐	19. Function Rinsing and Dosing	☐	☐	
☐	☐	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	☐	☐	

เพิ่มเติม/ข้อแนะนำ :



Certificate no. : G 630585

Date of issue : 22-Sep-20

Instrument description : Gas Detector
Instrument model : MX4
Instrument serial no. : 18051AW-004
ID no. or control no. : RT61046
Manufacturer : Industrial Scientific Corporation
Probe description : -
Probe model : -
Probe serial : -
Customer name : Entech Industrial Solution Co.,Ltd.
Customer address : 17/121 Soi Ngamwongwan 47 Yaek 48 , Toongsonghong, Laksi, Bangkok 10210 THAILAND

Total pages of certificate : 2 Pages
Receiving no. : L-202180
Receiving date : 17-Sep-20
Parameter of calibration : Gas Calibration(Oxygen 18.01 %vol, Carbon Monoxide 105 ppm, Methane in Air 49.84 %LEL, Hydrogen sulfide 26.5 ppm)

Condition of UUC. : Used
Ambient condition : All of the measurement were carried out in the stabilized laboratory
Temperature : 23 ± 5 °C
Humidity : 55 ± 15 %RH

Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48 Toongsonghong Laksi Bangkok

Calibration procedure no. : WI-CL-17-C

The calibration certificate expanded uncertainty of measurements is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test environmental condition.

This calibration certificate may not be reproduced other than in full except with the permission of the issuing laboratory.

Calibration certificates without signature and seal are not valid.

This calibration certificate documents are traceability to national standards, which realize the unit of measurement according to the International System of Units (SI). Refer to certificate as table 1 of page 2.

Date of calibration : 18-Sep-20

Certificate no. : G 630585

Standard references (Table 1)

Standard	Reference no.	Vendor	Due date
Oxygen (O ₂) 18.01 %vol	2425/19	Linde	16-Jul-23
Methane in Air (CH ₄) 49.84 %LEL	CG-0016-19	NIMT	09-Jul-22
Carbon Monoxide (CO) 105 ppm	4159/18	Linde	19-Nov-20
Hydrogen sulfide (H ₂ S) 26.5 ppm	4159/18	Linde	19-Nov-20

Measured room conditions

Temperature : 24.3 °C Humidity : 51.6 %RH Pressure : 1014.8 mbar

Calibration conditions

Gas temperature : 23 °C Flow rate : 300 ml/min Gas pressure : 1021.6 mbar

Calibration results (without adjustment) (Table 2)

Parameter of standard	Standard values	Mean of UUC.	Error	Uncertainty (±)
O ₂ (%vol)	18.01	18.1	0.09	0.60
CH ₄ (%LEL)	49.84	48	-1.84	2.2
*CO (ppm)	105	104	-1	3.0
*H ₂ S (ppm)	26.5	26.8	0.3	2.0

Remark : 1 cmol/mol = 1 %vol. 1 μmol/mol = 1ppm. 2.2 cmol/mol = 50%LEL(CH₄)

* Calibrations marked Not TISI Accredited "in this Certificate have been included for completeness."

End of report



National Institute of Metrology (Thailand)

Certificate of Calibration



Certificate No. : AA-2018-22
Issued by : Acoustics Laboratory
Acoustics and Vibration Group

Page 1 of 5 pages

MEASUREMENT ITEM : Sound Calibrator
MANUFACTURER : RION
MODEL/TYPE : NC-75
SERIAL NUMBER : 34480442
CUSTOMER : MET Co., Ltd.
36/659 Moo 6, T. Bangrakphatthana,
A. Bangbuathong, Nonthaburi 11110
MEASUREMENT DATE : 28 September 2022

The reported measurement result relates only to the measurand and applies only at the time of measurement.

*The calibration results only marked with an asterisk * in this certificate are not included in the scope of accreditation.*

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%. This calibration certificate may not be reproduced other than in full except with the permission of the Director of National Institute of Metrology (Thailand).

Reference	Date	Authorized Signatory	Person in charge
AUVC844-01/22	29 September 2022		

This certificate is consistent with the capabilities that are included in Appendix C of the MRA drawn up by the CIPM. Under the MRA, all participating institutes recognize the validity of each other's calibration and measurement certificates for the quantities, ranges and measurement uncertainties specified in Appendix C (for details see <http://www.bipm.org>).

National Institute of Metrology (Thailand)

Ministry of Higher Education, Science, Research and Innovation

3/4-5 Moo 3, Klong 5, Klong Luang, Pathumthani 12120, Thailand. Tel: (66) 2577 5100, Fax: (66) 2577 3659

75/7 Rama VI Road, Rachathewi, Bangkok 10400, Thailand. Tel: (66) 2354 3700, Fax: (66) 2354 3692



UNCERTAINTY OF MEASUREMENT

The stated uncertainty is the expanded uncertainty obtained by multiplying the standard uncertainty by the coverage factor $k=2$. It has been determined in accordance with EA publication EA-4/02 M:2013 "Evaluation of the Uncertainty of Measurement in Calibration" and JCGM 100:2008 "Evaluation of measurement data --Guide to the Expression of Uncertainty in Measurement (GUM 1995 with minor corrections)". The value of the measured lies within the assigned range of value with a probability of 95 %.

Parameter	Uncertainty at SPL94 dB	Maximum-permitted uncertainty of measurement for a coverage probability of 95%
1.Sound Pressure level	0.08	0.15
2. Frequency	0.1	0.2
3. THD+N	0.1	0.5

TRACEABILITY

This certificate provides traceability of measurement to recognized national standards, and to the realization of the International System of Units (SI).



ENVIRONMENTAL CONDITIONS

Ambient condition in the laboratory are as follows :

Temperature	:	(23.0 ± 1.0)	°C
Pressure	:	(101.325 ± 1.500)	kPa
Relative Humidity	:	(50.0 ± 15.0)	%

Reference Condition : 101.325 kPa , 23.0 °C and 50.0 %RH.

Calibration Condition

Preconditionings : 16 hours at ambient conditions.

Measurement Conditions : The average values during measurement are
 (100.313 ± 0.014) kPa, (22.0 ± 0.3) °C and (57.0 ± 2.1) %RH

MEASUREMENT METHOD

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone. The insert voltage technique was employed and the measurement procedure was based on IEC 60942-2017.

Reference Microphone

4180 serial no.1395446

TABULATION OF RESULTS

The following tables give the calibration results and associated measurement uncertainties at 95% of confidence level. The calibration results of sound pressure level which quoted in dB with reference to 20 µPa are corrected to the values under the reference environmental conditions.

The calibration results exclude the calibrator pressure correction but include the microphone volume correction, which was obtained from the manufacturer instruction manual of the sound calibrator, at the level of 94 dB.



MEASUREMENT RESULTS

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)*	Deviated value ^[1] (dB)	Acceptance Limit (dB)
Microphone 4180 Serial No.1395446			
94	94.15	0.15	0.25

Note ^[1] : The deviated value is the absolute value of the difference between the measured value and the corresponding specified sound pressure level.

2. Frequency*

Specified Frequency (Hz)	Measured value (Hz)	Deviated value ^[2] (%)	Acceptance Limit (%)
At the sound pressure level of 94 dB			
1000	1000.0	0.0	0.7

Note ^[2] : The deviated value is the absolute value of the difference in percent between the measured value and the corresponding specified frequency.



3. Total distortion + Noise*

Microphone 4180 Serial No.1395446

Measured value ^[3] (%)	Maximum total distortion + Noise (%)
At the sound pressure level of 94 dB	
0.2	2.5

Note ^[3]: The measured value is the total distortion, measured over the frequency range from 20 Hz to 20 kHz. The measured value must not exceed the maximum total distortion + noise appeared in the table.

End of Certificate of Calibration



Certificate of Calibration

Certificate Number : SPR23010010-5

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 76238

ID. Number : SLM-47

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 04 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Approved by :





Calibration Report

Certificate Number : SPR23010010-5

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010010-5

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.1	114.1	0.1	0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010010-4

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 76239

ID. Number : SLM-35

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 04 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Approved by :





Calibration Report

Certificate Number : SPR23010010-4

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010010-4

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010010-3

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 79210

ID. Number : SLM-39

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 04 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Approved by :





Calibration Report

Certificate Number : SPR23010010-3

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010010-3

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.1	114.1	0.1	0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.1	114.1	0.1	0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010010-1

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : Rion

Model : NL-21

Serial Number : 00722042

ID. Number : SLM-46

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 04 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Approved by :





Calibration Report

Certificate Number : SPR23010010-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010010-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

Certificate of Calibration

Certificate No. : 65-400424-3

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Refrigerator)
Manufacturer : Sanden Intercool Model : YPR-068S
Range : N/A °C Resolution : 1 °C
Serial No. : YPR0659S-141200060R ID No. : MET-RE03/59

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (29.8 to 31.5) °C
Relative Humidity : (55 to 58) %
Line Voltage : (220.8 to 222.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by :

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400023	65-400157-1	02 Oct 2022	National Institute of Metrology Thailand (NIMT)

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-400424-3


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

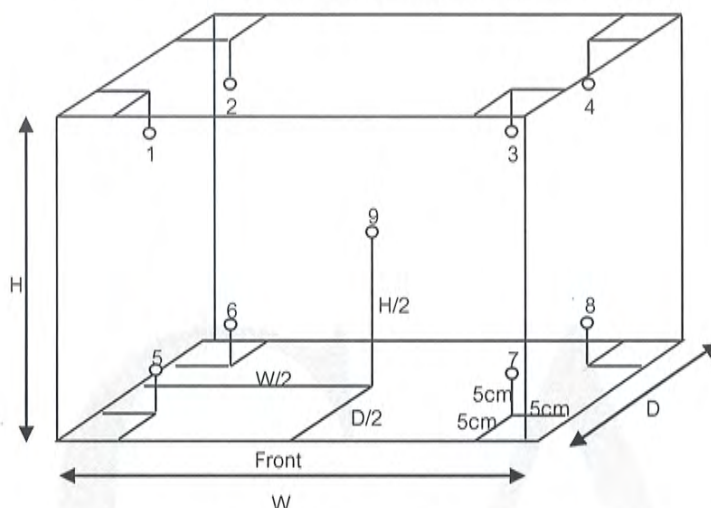

Inside of Chamber

W = 0.58 m

D = 0.60 m

H = 1.45 m

Capacity = 0.50 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
3	2	2	3.7	3.7	4.0	3.7	3.0	3.5	2.8	3.4	2.9	0.84

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
3	2	2	1.2	0.2	1.5

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-420002-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : pH 150

Range : -2.00 to 16.00 pH

Resolution : 0.01 pH

Serial No. : 2657036

ID No. : MET-PH04/60

Electrode

Model : N/A

Serial No. : 66365

Environment : Ambient Temperature : $(25 \pm 2) ^\circ \text{C}$

Relative Humidity : $(50 \pm 15) \%$

Date of Received : 05 January 2023

Date of Calibration : 11 January 2023

Date of Issue : 11 January 2023

Calibrated by :

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
440001	21E997	17 Mar 2023	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

<u>pH</u>	<u>Cert. No.</u>	<u>Lot No.</u>	<u>Exp. Date</u>	<u>Traceability</u>
4.008	61235182	857394	11 Dec 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61267169	857395	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61260481	857396	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-420002-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement
pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.1	0.4	0.060
	0.0000	7	6.99	-0.1	0.1	0.060
	-177.4800	10	10.00	-177.3	-0.2	0.060

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o()o -



Certificate of Calibration

Certificate No. : 65-300144-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Cylinder

Manufacturer : Witeg

Class : A

Capacity : 100 ml Graduation : 1 ml

ID No. : MET-CY100:01/61

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1007.4 mbar.

Date of Received : 09 March 2022

Date of Calibration : 15 March 2022

Date of Issue : 15 March 2022

Calibrated by :



Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	64-200354-1	02 Jun 2022	National Institute of Metrology (Thailand) (NIMT)

Approved by :



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-300144-1

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
50	50.29
100	99.99

Uncertainty of measurement with in $\pm$ 0.063 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 65-300144-2

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Cylinder

Manufacturer : Witeg

Class : A

Capacity : 100 ml

Graduation : 1 ml

ID No. : MET-CY100:01/64

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1007.4 mbar.

Date of Received : 09 March 2022

Date of Calibration : 15 March 2022

Date of Issue : 15 March 2022

Calibrated by :



Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	64-200354-1	02 Jun 2022	National Institute of Metrology (Thailand) (NIMT)

Approved by :



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-300144-2

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
50	50.02
100	100.07

Uncertainty of measurement with in $\pm$ 0.063 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 65-300144-3

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Cylinder(Plasstic)

Manufacturer : N/A

Class : N/A

Capacity : 1000 ml

Graduation : 10 ml

ID No. : MET-CY1000:01/61

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1007.4 mbar.

Date of Received : 09 March 2022

Date of Calibration : 15 March 2022

Date of Issue : 15 March 2022

Calibrated by :



Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	64-200354-1	02 Jun 2022	National Institute of Metrology (Thailand) (NIMT)

Approved by :



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-300144-3

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
500	488.51
1000	992.91

Uncertainty of measurement with in $\pm$ 0.17 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 65-300144-4

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Buret

Manufacturer : Witeg

Class : A

Capacity : 10 ml

Graduation : 0.02 ml

ID No. : MET-MB-01/64

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1007.1 mbar.

Date of Received : 09 March 2022

Date of Calibration : 15 March 2022

Date of Issue : 15 March 2022

Calibrated by :



Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
241003	64-200354-2	02 Jun 2022	National Institute of Metrology (Thailand) (NIMT)

Approved by :



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-300144-4

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 31.89 sec.

Nominal Volume (ml)	Measuring Volume (ml)
2	2.0091
5	5.0223
10	10.0425

Uncertainty of measurement with in $\pm$ 0.0039 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- oOo -



Certificate of Calibration

Certificate No. : 65-300144-5

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Buret

Manufacturer : Witeg

Class : B

Capacity : 50 ml Graduation : 0.1 ml

ID No. : MET-BU50:01/64

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1007.1 mbar.

Date of Received : 09 March 2022

Date of Calibration : 15 March 2022

Date of Issue : 15 March 2022

Calibrated by :



Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241003	64-200354-2	02 Jun 2022	National Institute of Metrology (Thailand) (NIMT)

Approved by :



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-300144-5

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 24.79 sec.

Nominal Volume (ml)	Measuring Volume (ml)
10	10.0406
30	29.9786
50	49.9808

Uncertainty of measurement with in $\pm$ 0.0069 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-300123-4

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Burette

Manufacturer : TS

Class : A

Capacity : 10 ml

Graduation : 0.02 ml

ID No. : MET-BU10:02/64

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1015.1 mbar.

Date of Received : 02 March 2023

Date of Calibration : 09 March 2023

Date of Issue : 09 March 2023

Calibrated by : Anusorn Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	65-200370-4	02 Jun 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-300123-4

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 36.97 sec.

Nominal Volume (ml)	Measuring Volume (ml)
2	2.0008
5	5.0035
10	10.0072

Uncertainty of measurement with in $\pm$ 0.0039 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-400012-1

Page : 1 of 2

Submitted by : M E T Company Limited
6/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Digital Thermometer with Thermistor Probe
Temperature Indicator

Manufacturer :	Thermo Scientific	Model :	pH 150
Range :	N/A	Resolution :	0.1 °C
Serial No. :	2657036	ID No. :	MET-PH04/60
Thermistor Probe			
Model :	PHWPTEM01W	Sheath Material :	Stainless
Diameter :	3 mm.	Length :	85 mm.
Serial No. :	237	ID No. :	MET-PH04/60

Environment : Ambient Temperature : (23 ± 2) °C
Relative Humidity : (50 ± 15) %
Line Voltage : (220 ± 22) VAC

Date of Received : 05 January 2023

Date of Calibration : 11 January 2023

Date of Issue : 11 January 2023

Calibrated by : [REDACTED]

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0016-20	04 Mar 2022	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)
400004	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)

Approve [REDACTED]

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400012-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
85	10.0035	9.8	0.2	0.11
85	50.0025	50.0	0.0	0.11

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

- ๐0๐ -



Packing List

Unit : K-446 Kjeldigester standard



151111112791000281006111

Serial Number 1000281006

Page 1(1)

Item	Pieces	Description		
11059833	1.0000	Packing parts Kjeldigester K-446/K-449 Beipackteile K-446/K-449		✓ OK
037377	5.0000	Sample tubes 300 ml (set of 4) Probengläser 300 ml (Set à 4 Stück)		✓ OK
11059754	1.0000	Rack 20 cpl. Rack 20 kpl.		✓ OK
11058955	1.0000	Aspiration device Kjeldigester K-446/K-449 cpl. Absaugeinheit K-446/K-449		✓ OK
040444	1.0000	Weighing boat 20pcs. Wägeschiffchen 20 Stk.		✓ OK
010020	1.0000	Power cable type USA, 3 pole 120V Anschlusskabel USA W 120V		✓ OK
11058825	1.0000	Fume collection tube with ball joint Dampfsammelrohr mit Kugelschliff		✓ OK
11592548	1.0000	Kjeldahl Practice Guide en Kjeldahl Practice Guide en		✓ OK
11593546	1.0000	Operation Manual K-446/K-449 english Bedienungsanleitung K-446/K-449 englisch		✓ OK
11593635	1.0000	Supplemantary sheet Kjeldigester K-446/K-449 Beiblatt K-446/K-449		✓ OK

Packed by





BUCHI Certificate Final Test Inspection

Unit : BÜCHI Kjeldigester K-446

Serial number 1000281006

Examination Procedure

1. **Visual control of the glass parts and the unit**

✓ OK

- No scratches on the coated surface
- Mounted in accordance to the specific drawing

2. **Security tests**

✓ OK

- High voltage test in accordance with EN 61010-1 (IEC 1010)
- Ground connection test in accordance with EN 61010-1 (IEC 1010)

3. **Functional tests**

Operating panel

✓ OK

- All buttons are working
- Cooling system is working after the instrument has been switched on

Connector plugs

✓ OK

- Scrubber connector is working

Heating element

✓ OK

- Heating-up temperature 420 °C is reached after 40 minutes
- Temperature calibration at 420 °C (3 measuring points)

4. **Completeness of order checked**

✓ OK

BÜCHI Labortechnik AG hereby declares that this unit is in accordance with the specifications



Packing List

Unit : K-415 TripleScrub 230V



151111112781000281005111

Serial Number

1000281005

Page 1(1)

Item	Pieces	Description		
11057332	1.0000	Tray for adsorption storage Ablage für Adsorption		✓ OK
048355	1.0000	Silicone hose D6/9 L=3m Silikonschlauch D6/9 L=3.0m		✓ OK
033701	1.0000	Glass wool 30g Glaswolle 30g		✓ OK
028737	2.0000	Hose clamp Anschlussklemme		✓ OK
11064971	1.0000	Activated Charcoal 2-6mm, 150g Aktivkohle 2-6mm, 150g		✓ OK
010020	1.0000	Power cable type USA, 3 pole 120V Anschlusskabel USA W 120V		✓ OK
11593505	1.0000	Operation Manual K-415 english Bedienungsanleitung K-415 englisch		✓ OK

Packed by

h. J. J.





BUCHI Certificate Final Test Inspection

Unit : BÜCHI Scrubber K-415

Serial number 1000281005

Examination Procedure

1. **Visual control of the glass parts and the unit**

✓ OK

- No scratches or splinters on the glass parts
- Mounted in accordance to the specific drawing

2. **Security tests**

✓ OK

- High voltage test in accordance with EN 61010-1 (IEC 1010)
- Ground connection test in accordance with EN 61010-1 (IEC 1010)

3. **Functional tests**

Vacuum test

✓ OK

- Bypass valve open: Pressure is 0 - 65 mbar below the atmospheric pressure
- Bypass valve closed: Pressure is 400 mbar (+/- 10 %) below the atmospheric pressure

4. **Completeness of order checked**

✓ OK

BÜCHI Labortechnik AG hereby declares that this unit is in accordance with the specifications

Packing List

Unit : K-360 Plastik Basic



151111113001000281014111

Serial Number

1000281014

Page 1(1)

Item	Pieces	Description		
043410	3.0000	Canister 10L thin-walled Kanister 10L dünnwandig		OK
043603	1.0000	Packing parts K-360 Beipackteile K-360		OK
047871	1.0000	Suppl. sheet distillation unit Beiblatt Distillation Unit		OK
010020	1.0000	Power cable type USA, 3 pole 120V Anschlusskabel USA W 120V		OK
11592548	1.0000	Kjeldahl Practice Guide en Kjeldahl Practice Guide en		OK
093176	1.0000	Operation Manual K-360 english Bedienungsanleitung K-360 englisch		OK

Packed by







BUCHI Certificate Final Test Inspection

Unit : BÜCHI BÜCHI KjeIFlex K-360

Serial number 1000281014

Examination Procedure

1. **Visual control of the glass parts and the unit** ✓ OK

- No scratches on the coated surface or splinters on the glass parts
- Mounted in accordance to the specific drawing

2. **Security tests** ✓ OK

- High voltage test in accordance with EN 61010-1:2002 (IEC 61010-1, VDE 0411)
- Ground connection test in accordance with EN 61010-1:2002 (IEC 61010-1, VDE 0411)
- Safety door sensor checked

3. **Functional tests** ✓ OK
Electronics

- Electronic modul is tested with the checking device PG157
- Connector plugs are working

Operating panel ✓ OK

- Display is working
- All buttons of the keypad are working

Pump testing ✓ OK

- All pumps are working
- All pumps (exception: water pump of the steam generator) are precalibrated

Valve testing ✓ OK

- All valves are working

Steam generator testing ✓ OK

- The steam generator is filled with water
- The steam generator valve is working
- The amount of distillate corresponds to specifications

Further testing ✓ OK

- Beeper is working

4. **Unit configuration and completeness of order checked** ✓ OK

BÜCHI Labortechnik AG hereby declares that this unit is in accordance with the specifications

H.

Certificate of Calibration

Certificate No. : 66-200067-1

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Electronic Balance
Manufacturer : METTLER TOLEDO Model : AG285
Serial No. : 1122140126 ID No. : MET-EB01/46
Capacity : 210 g Resolution : 0.00001g/81g, 0.0001g/210g

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (26.4 to 26.8) °C
Relative Humidity : (54.9 to 58.8) %
Air Pressure : 1013.0 mbar

Date of Received : 02 March 2023

Date of Calibration : 02 March 2023

Date of Issue : 13 March 2023

Calibrated by :

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02222345	10 Nov 2023	National Institute of Metrology (Thailand), (NIMT)

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-200067-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty $\pm$ (g)
0.01	0.00001	0.000020
0.1	0.00000	0.000019
1	-0.00002	0.000031
5	-0.00004	0.000043
10	-0.00008	0.000054
20	-0.00027	0.000071
50	-0.00059	0.00011
100	-0.0009	0.00023
150	-0.0012	0.00038
200	-0.0019	0.00040

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.43$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A B C D E

0.00055 0.00027 -0.00015 -0.00018 0.00000 g



Repeatability

Load test : 200 g

Stdev. : 0.000053 g

- oOo -



Certificate of Calibration

Certificate No. : 65-400424-2

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)
Manufacturer : Binder Model : ED53
Range : N/A °C Resolution : 1 °C
Serial No. : 13-07419 ID No. : MET-OV02/57

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (27.0 to 28.0) °C
Relative Humidity : (50 to 55) %
Line Voltage : (210.0 to 210.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by :

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400030	65-400272-1	24 Nov 2022	National Institute of Metrology Thailand (NIMT)

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-400424-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

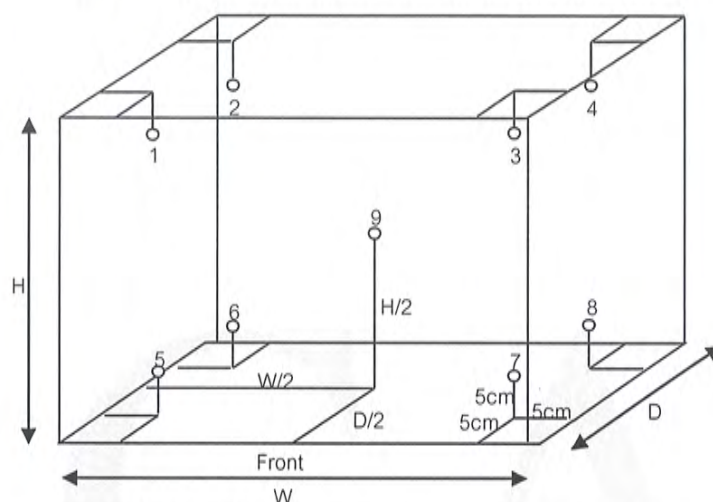

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.40 m

Capacity = 0.05 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104	110	110	105.0	105.0	104.7	105.0	104.4	104.5	104.0	103.7	104.2	0.95
180	184	184	180.8	182.0	179.4	180.8	180.8	180.8	180.3	180.0	180.0	1.2

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104	110	110	1.0	0.2	1.7
180	184	184	2.3	0.3	3.0

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 65-400424-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)

Manufacturer : Memmert

Model : UM 100

Range : N/A °C

Resolution : 0.1 °C

Serial No. : b197.0985

ID No. : MET-OV01/46

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (27.0 to 28.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by :

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400032

65-400274-1

25 Nov 2022

National Institute of Metrology Thailand (NIMT)

Approved by :

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-400424-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

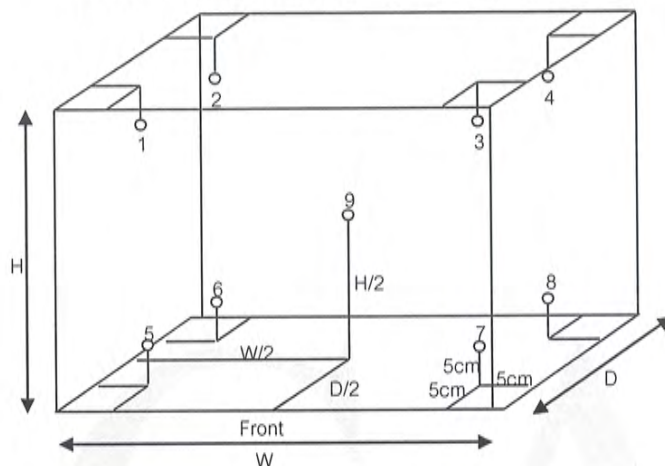

Inside of Chamber

W = 0.32 m

D = 0.18 m

H = 0.24 m

Capacity = 0.01 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
180.0	180.0	180.0	181.2	181.3	180.6	180.4	179.9	181.0	179.5	179.1	180.0	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
180.0	180.0	180.0	1.4	0.3	2.5

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Calibration Certificate

Cert. No. : CT-23-05-23470

Page : 1 of 4

Issued date : 08 May 2023

Equipment : COD Reader , Manufacturer : MLAB , Model : DB1602

S/N = 0169 , Customer ID = -

Client : M E T COMPANY LIMITED.

36/659 M.6 Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

Received Date : 03 May 2023

Ref. Job No. : SO6605-00001

Calibrate by :

Cert. prepare by :

Calibrated Date : 03 May 2023

Approved by :

Calibration Place : Laboratory room

Environment Condition : Temperature 28.6 ± 0.4 (°c) , Humidity 59.5 ± 3.5 (%RH)

Calibration Method : Measure temperature distribution by 9 channel in flat level. , (MTEC WI No. # WICAL-02-005-R01)

Reference Standard Instrument :

No	Instrument	code	Model	Due date
1	Temperature Datalogger	MTEC-CE-0180	MLAB	10/2023
2	Thermo Hygrometer	MTEC-CE-0181	TH-03A	06/2023

Condition of certificate :

(1) This certificate is traceable to International System of units (SI Units). , (2) This certificate was certified only for the instrument we calibrated. , (3) This result of calibration was found accurate as show on date and place of calibration only. , (4) The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k =$ (see result table) , providing a level of confidence of approximately 95%. , (5) This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration Division, Metrology Technical Co.,Ltd.

Certificate No. : CT-23-05-23470

Calibration Result :

Page : 2 of 4

Condition of UUC :


- 1) Without Adjustment
- 2) Immersion : 1/2 of the depth of the hole

(1) The quoted uncertainty include with * Stability*.

(2) Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors , for at least half an hour after reaching steted state.

(3) Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

(4) Overall variation = The difference of the maximum and the minimum measured temperature throughout observation time.

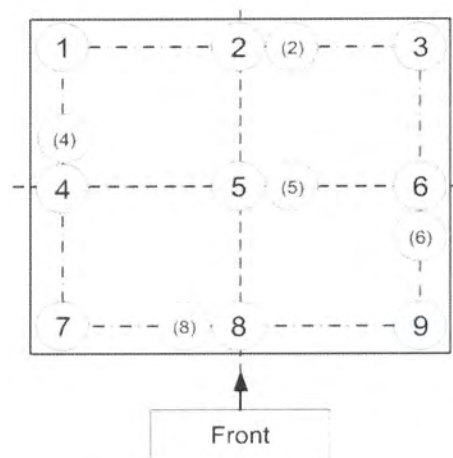

Pic 1 : Position of each sensor No.

Section 1 : Report of Temperature distribution

Unit : (°c)

Calibration Point	UUC Setting (*)	UUC Reading (*)	Measured Temperature @ Sensor No.									Uncertainty (±)	k ^(**)
			#1	#2	#3	#4	#5	#6	#7	#8	#9		
150	150	150	150.51	149.89	150.16	149.93	150.56	150.67	149.80	150.25	149.76	0.627	2

(*) = The average of 30 values in each point , (**) = Coverage factor (k) value

Section 2 : Report of Chamber Performance

Unit : (°c)

Calibration Point	UUC Setting	UUC Reading (*)	Temperature Uniformity	Temperature Stability (± °c)	Temperature Overall Variation
150	150	150	1	0.05	1

(*) = The average of 30 values in each point

Approved Signatory : ...

Certificate No. : CT-23-05-23470

Page : 3 of 4


Section 3 : Possible of temperature. Show minimum and maximum of the average values and Include with uncertainty of measurement. The average values is average of each position standard sensor throughtout observation time.


Unit : (°c)

Calibration Point	UUC Setting ^(*)	UUC Reading ^(*)	Possible of Minimum temperature	Possible of Maximum temperature
150	150	150	149.14	151.30

(*) = The average of 30 values in each point

Section 4 : Trend of accuracy

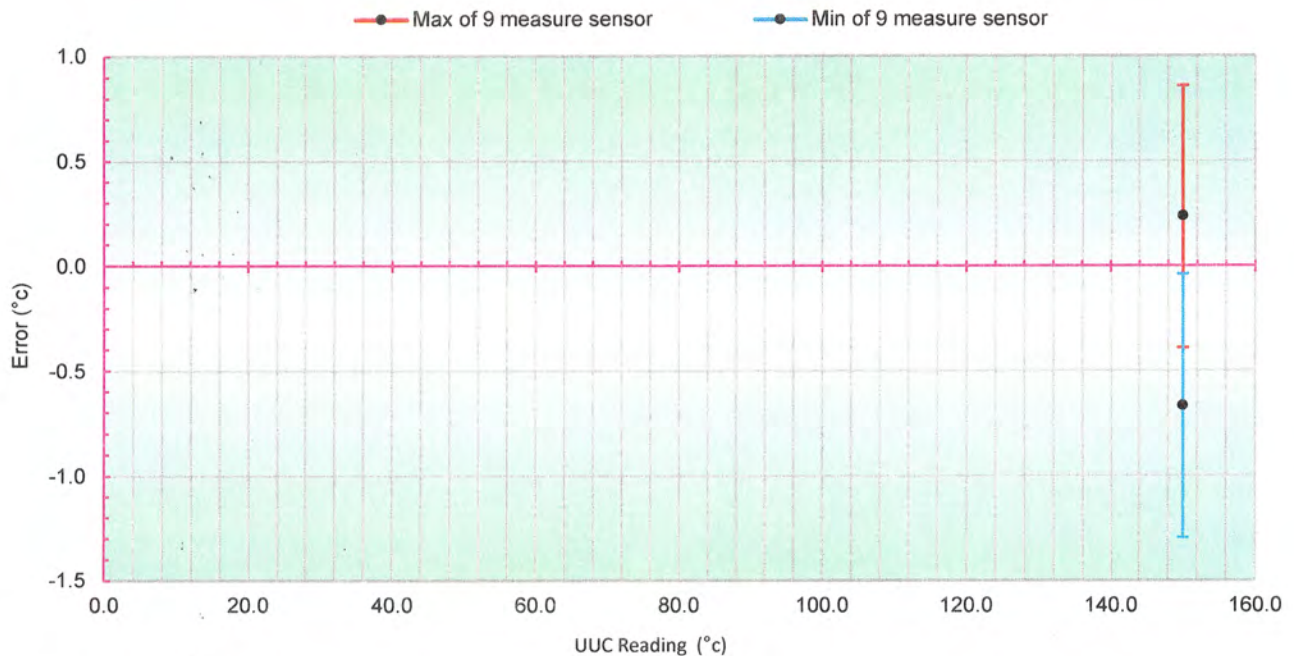


Approved Signatory : 

Certificate No. : CT-23-05-23470

Page : 4 of 4

Section 5 : Graph report for Temperature distribution , not include uncertainty of measurement

(5.1) Temperature Distribution at UUC Reading 150 °C

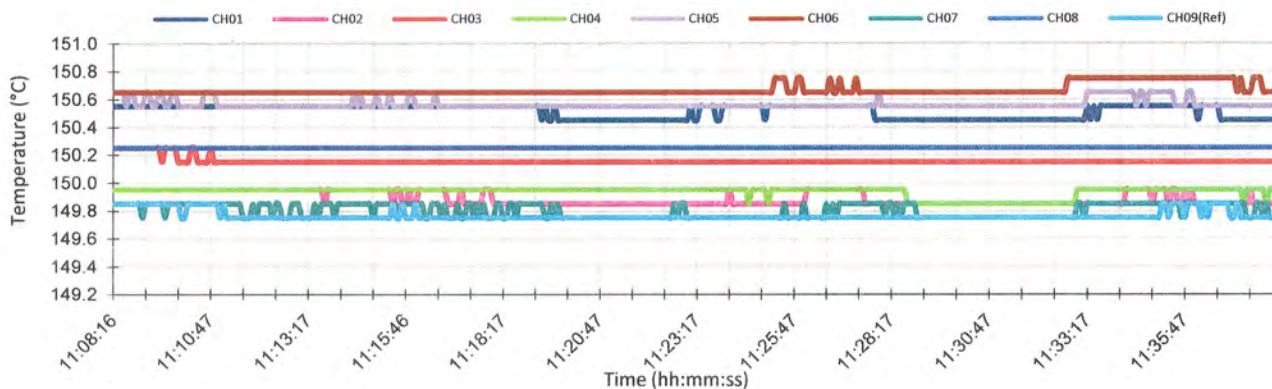

Approved Sign

Certificate of Calibration

Certificate No. : 66-300003-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6 T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Volumetric Flask

Manufacturer : ISOLAB

Class : A

Capacity : 1000 ml

ID No. : MET:VF1000:02/61

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1012.0 mbar.

Date of Received : 05 January 2023

Date of Calibration : 13 January 2023

Date of Issue : 13 January 2023

Calibrated by : [Redacted]

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	65-200370-1	02 Jun 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-300003-1

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
1000	1000.55

Uncertainty of measurement with in $\pm$ 0.14 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -





Optima8000 Preventive Maintenance Report

Company Name: MET Company Limited.

Instrument Location: 36 659 Soi Mu Ban Monwadi Park 6,
Bang Rak Phatthana, Bang Bua Thong District, Nonthaburi 11110

Instrument Serial No.: 078S1407053C

Date: 8-Dec-2022

ICP-OES/Optima8000 Preventive Maintenance (PM)

Company Name:	MET Company Limited.		
Address (Instrument Location):	Bang Rak Phatthana, Bang Bua Thong District, Nonthaburi 11110		
Serial Number:	078S1407053C	PM Number:	1 of 2
Customer Name (if applicable):		Telephone Number:	065 850 0726
Service Engineer Name:		Service Order Number:	WO-01877169
Date PM Performed: (DD-MMM-YYYY)	8-Dec-2022	Next PM Due Date: (DD-MMM-YYYY)	8-June-2023
Standard Labor Hours to Complete PM :		4 hours	

Part Number	Release	Publication Date	
09370140 Rev.5	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PerkinElmer/Optima8000 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes
Optima8000	078S1407053C	Winlab V 5.5.0.0714
S10 Autosampler		

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
09995098	Air Filter-Spectrometer	1
N077520	Air Filter-RF Generator	1
09992731	Axial Window	1
B0810377	Radial Window	1
N0770438	O-ring kit, injector support adapter	1
N0780437	O-ring kit, torch	1

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date: (MM/YY)
N0691579	Multi-Element Standard (N069-1579 diluted 10X)	1	58-146CRX1	Oct-2023
N9300221	Instrument Calibration-4 (N9300221 diluted 100X)	1	58-169CRY1	Nov-2023

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ✓ Ask customer about unit's performance since last visit.
- ✓ Check incoming AC line voltage under load for proper levels and grounding.
- ✓ Is the instrument operational?

2. Mechanical:

- ✓ Inspect and clean all fans and filters.
- ✓ Inspect and replace torch components and necessary.

Torch Components Replaced: ☒ Yes ☐ No

If yes, list components replaced:

- ✓ Inspect all tubing for signs of cracking or leaking and replace as necessary.

Tubing Replaced: ☒ Yes ☐ No

If yes, list tubing replaced:

- ✓ Inspect the peristaltic pump for proper operation.
- ✓ Check and adjust if necessary, the external nitrogen, argon shear gas and water supply pressures.
- ✓ Check and adjust if necessary, the internal nitrogen, main argon, torch argon and shear gas pressures

Regulator	Measured Pressure	Set Pressure
Nitrogen	N/A	NA (calibrated in Factory)
Main Argon	76	76psig
Torch Argon	67	67psig
Shear Gas	65	65psig
Water	35	35psi

- ✓ Check the shear gas nozzle for blockages and proper, uniform flow.
- ✓ Inspect nitrogen Hi/Low purge and shear gas solenoids for proper function.
- ✓ Inspect the function of all spectrometer motors. Drive the motors from the Spectrometer DCM. Check all motors, couplings, set screws, gears or drive assembly located on the spectrometer (prism/grating wavelength drives, slits, shutter, DV mirror, X/Y mirror) if problems are found.
- ✓ Perform preventative maintenance on the chiller as required. Make the customer aware of the importance of maintaining the chiller fluid level and filter replacement.
- ✓ Drain air compressor surge tank.
- ✓ Clean exterior of instrument.

3. Electrical:

- ☒ Visually inspect all PC boards for cleanliness and signs of corrosion.
 - ☒ Check all RF generator and spectrometer power supply voltages.
 - ☒ Run instrument diagnostic checks from the appropriate Device Control Module.

RF Generator:

- ☒ Check the RF generator status screens.
- ☒ Check the function of all interlocks.

Spectrometer:

- ☒ Check the spectrometer status screens.
- ☒ Check for proper function of all motors from the Motor Control window.

4. Optical:

- ☒ Check the neon lamp for proper operation.
- ☒ Ensure that neon initialization passes at power up.
- ☒ Ensure that there is a single, well defined peak of sufficient intensity (approximately 15,000 to 60,000 cts.) for the 703.241nm neon line viewed in the DCM Collect Spectra window. Re-generate the neon correction table if problems are encountered. If problems are still exhibited after the table is re-generated, replace the neon lamp assembly.

Neon Lamp Replaced: ☐ Yes ☒ No

- ☒ Perform the Initialize Optics routine from the Spectrometer Control window.
- ☒ Insure that the routine passes with no error codes. If it fails, run a manual prism scan from the spectrometer DCM.
- ☒ Insure the Dark Current measurement (Detector Calibration) passes at initialization.
- ☒ Check the shutter home sensor position.
- ☒ Check prism/electronics temperature sensor readback values from the DCM. It is normal for these readings to be shown in red. A typical prism temperature is approximately 29.5 degree C. A typical electronics temperature is approximately 35 degree C.
- ☒ Check the detector temperature from the DCM for -7.0 to -8.5 degree C. If outside of this range the detector cooling fan may not be operational. Further inspection may be necessary.
- ☒ Inspect for proper function of the transfer optics. 1) shutter 2) DV mirror 3) X/Y mirror.
- ☒ Clean or replace the axial and radial view windows as necessary.

Axial Window Replaced: ☒ Yes ☐ No

Radial Window Replaced: ☒ Yes ☐ No

5. Post PM Performance Tests:

- ☒ Perform View Align.

5.1 Spectral Resolution:

- ☒ Measure the spectrometers ability to separate two adjacent wavelengths.

Parameter	Specification	Test Result	Pass/Fail
As 193.696 - Resolution	≤0.009	0.007	Passed
Ni 231.604 - Resolution	≤0.011	0.008	Passed
Ni 341.476 - Resolution	≤0.015	0.012	Passed
Ba 455.403 - Resolution	≤0.020	0.015	Passed

5.2 Precision:

☒ Test for reproducibility of a set of measurement.

Parameter	Specification	Test Result	Pass/Fail
Zn 213.856	%RSD ≤ 1 %	0.35	Passed
Mg 280.856	%RSD ≤ 1 %	0.46	Passed
Mg 285.207	%RSD ≤ 1 %	0.65	Passed
Ba 455.403	%RSD ≤ 1 %	0.38	Passed

5.3 Mn BEC:

☒ Run Axial and Radial BEC according to the A&T spec, or the commissioning test procedure.

Mn Background Equivalent Concentration:

Method "MnBEC" For Samples "IB (2%HNO3)" and "IS (N069-1579/10)", record intensities.

Calculated BEC: $BEC = (IB * Conc\ of\ Std) / (IS - IB)$. Where Conc of Std = 1,000 PPB

Element	Mode	Conc.	IB	IS	
Mn 257.610	Radial	1,000 ppb	5123.3	409288.2	
Mn 257.610	Axial	1,000 ppb	10397.4	1879864.3	
Mn 257.610	IB*Conc.	IS - IB	BEC	Spec	Pass/Fail
Radial	5123300	404164.9	12.67	<30 PPB	Passed
Axial	10397400	1869466.9	5.56	<30 PPB	Passed

6. Review:

- ☒ Review with the customer PM work performed.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

Additional Comments

Additional Comments Regarding the PM

This image shows a completely blank white rectangular area enclosed within a thin black frame. There are no markings, text, or illustrations present on the page.

Review

The preventive maintenance checks and if applicable performance tests for ICP-OES/Optima8000 have been completed.

This ICP-OES/Optima8000 Passes ☒ Fails ☐ the preventive maintenance.

Review of Preventive Maintenance:

Authorized PerkinElmer Representative:

Date:

8-Dec-2022

(DD-MMM-YYYY)

Authorized Customer Representative:

Date:

8-Dec-2022

(DD-MMM-YYYY)

Certificate of Calibration

Certificate No. : 66-400013-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Liquid in Glass Thermometer

Manufacturer : SK

Model : N/A

Range : 0 °C to 100 °C

Resolution : 1 °C

Serial No. : N/A

Immersion : Total

ID No. : MET-TH09/20

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Line Voltage : (220 ± 22) VAC

Date of Received : 05 January 2023

Date of Calibration : 07 January to 10 January 2023

Date of Issue : 10 January 2023

Calibrated by :

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0016-22	07 Feb 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)
400004	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)

Approved

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400013-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Ice point check : UUC* reading 0 °C Standard reading 0.8073 °C

Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
11.3107	10	1.3	0.31
50.6036	50	0.6	0.31

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



ใบรับรองการสอบเทียบ “เครื่อง Inductively Coupled Plasma (ICP-OES)”
(Calibration Certificate of Inductively Coupled Plasma (ICP-OES))

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO., LTD.

ห้องปฏิบัติการวิเคราะห์เอกชน
เลขทะเบียน ว-244

ICP-OES/Optima8300 Preventive Maintenance (PM)

Company Name:	บริษัท เอ็มเม็กซ์แอสโซซิเอชั่น จำกัด		
Address (Instrument Location):	27, 29 ซอยพระรามที่ 2 ซอย 30 แขวงบางมด เขตจอมทอง กทม		
Serial Number:	078S1604262	PM Number:	2 of 2
Customer Name (if applicable):		Telephone Number:	
Service Engineer Name:		Service Order Number:	WO-01844676
Date PM Performed: (DD-MMM-YYYY)	01-Sep-2022	Next PM Due Date: (DD-MMM-YYYY)	01-Mar-2023
Standard Labor Hours to Complete PM :		4 hours	

Part Number	Release	Publication Date	
09370141 Rev.3	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PerkinElmer / Optima8300 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

EMEX Environmental
and Medical Expert

ICP-OES/Optima8300 Preventive Maintenance (PM)

EMEX ASSOCIATION CO. LTD.

Page 1 of 7

ห้องปฏิบัติการวิเคราะห์เอกชน

เลขทะเบียน ว-244

Component List

Component / Specific Model	Serial #	Configuration Notes

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
09995098	Air Filter-Spectrometer	NA
N077520	Air Filter-RF Generator	NA
09992731	Axial Window	NA
B0810377	Radial Window	NA
N0770438	O-ring kit, injector support adapter	NA
N0780437	O-ring kit, torch	NA

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N0691579	Muti-Element Standard	AR	58-146CRX1	11/23
N9300221	DL Standard diluted 100 X	AR	58-169CRY1	11/23
N0582152	Wave Cal Solution	AR	58-110CRX1	08/23
N9302946	VIS Wavecal Solution	AR	58-145CRT1	11/23

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO., LTD.

ICP-OES/Optima8300 Preventive Maintenance (PM) ห้องปฏิบัติการวิเคราะห์ออสัน

เลขทะเบียน ว-24

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Ask customer about unit's performance since last visit.
- ☒ Check incoming AC line voltage under load for proper levels and grounding.
- ☒ Is the instrument operational? If not, please comment.

2. Mechanical:

- ☒ Inspect and clean all fans and filters.
- ☒ Inspect and replace torch components and necessary.

Torch Components Replaced: ☐ Yes ☒ No

- ☒ Inspect all tubing for signs of cracking or leaking and replace as necessary.

Tubing Replaced: ☒ Yes ☐ No

- ☒ Inspect the peristaltic pump for proper operation.
- ☒ Check and adjust if necessary, the external nitrogen, argon shear gas and water supply pressures.
- ☒ Check and adjust if necessary, the internal nitrogen, main argon, torch argon and shear gas pressures.

Regulator	Measured Pressure	Set Pressure
Nitrogen	NA	NA (calibrated in Factory)
Main Argon	76	76 psig
Torch Argon	67	67 psig
Shear Gas	65	65 psig
Water	35	35 psi

- ☒ Check shear gas nozzle for blockages and proper, uniform flow.
- ☒ Inspect nitrogen Hi/Low purge and shear gas solenoids for proper function.
 - ☒ Inspect the function of all spectrometer motors. Drive the motors from the Spectrometer DCM. (slits, XY motor)
- ☒ Inspect the function of the pneumatic shutter for proper operation.
 - ☒ Perform preventative maintenance on the chiller as required. Make the customer aware of the importance of maintaining the chiller fluid level and filter replacement.
- ☒ Drain air compressor surge tank.
- ☒ Clean exterior of instrument.
- ☒ Visually inspect all PC boards for cleanliness and signs of corrosion.

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO., LTD.

ICP-OES/Optima8300 Preventive Maintenance (PM)

ห้องปฏิบัติการ วิเคราะห์


เลขทะเบียน ว-2

3. Electrical

☒ Check all RF generator and spectrometer power supply voltages.

Spectrometer Control/Interface PCB Test Points

TP	Voltage (DC)	Tolerance	Description
1	+24V	$\pm 500\text{mV}$	From Main Supply
2	+12V	$\pm 20\text{mV}$	Onboard – For View X/Y Motors
3	+15V	$\pm 600\text{mV}$	Onboard – For Spectrometer Control Electronics
4	-15V	$\pm 600\text{mV}$	Onboard – For Spectrometer Control Electronics
5	+3.3V	$\pm 100\text{mV}$	Onboard – Source of 3.3V for Icarus Engine and SCB elect.
6	+2.5V	$\pm 25\text{mV}$	Onboard – For Xilinx FPGA
7	+5.0V		From Main Supply
8			$\pm 5.0\text{ GND}$
9			$\pm 5.0\text{ GND}$
10			$\pm 5.0\text{ GND}$
11			$\pm 5.0\text{ GND}$
12			$\pm 5.0\text{ GND}$
13	+1.5V	$\pm 45\text{mV}$	Onboard – For Icarua Engine
22	+6.5V	-0mV, + 100mV	UV TEC
23	+6.5V	-0mV, + 100mV	VIS TEC

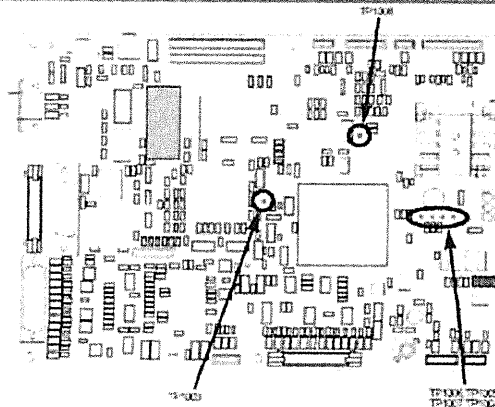

RF Controller PCB Test Points

TP	Voltage (DC)	RF Control PCB Location
1005	-14 to -16 (-15)	Right of U1001
1006	23-25 (24)	Right of U1001
1008	4.75-5.25 (5)	Upper Right of U1001
1003	14-16 (15)	Upper Left of U1001
1004	Ground	Upper Right of U1001

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO., LTD.

☒ Run instrument diagnostic checks from the appropriate Device Control Module.

RF Generator:

- ☒ Check the RF generator status screens.
☒ Check the function of all interlocks.

Spectrometer:

- ☒ Check the spectrometer status screens. Ensure Ready mode with no fatal errors.
☒ Check the spectrometer optical tub temperatures (top, bottom, fin, optical base).
☒ Check detector temperatures.
☒ Check TEC voltages (6.5VDC)

4. Optical:

- ☒ Clean or replace the axial and radial view windows as necessary.

Axial Window Replaced: ☐ Yes ☒ No

Radial Window Replaced: ☐ Yes ☒ No

5. PM Performance Tests:

- ☒ Perform View Align.

5.1 Spectral Resolution :

- ☒ Measure the spectrometers ability to separate two adjacent wavelengths.

Parameter	Specification	Test Result	Pass/Fail
As 193.696 - Resolution	≤ 0.007	0.00494	Pass
Ni 231.604 - Resolution	≤ 0.008	0.00599	Pass
Ni 341.476 - Resolution	≤ 0.012	0.00771	Pass
La 408.672 - Resolution	≤ 0.020	0.01508	Pass
Ba 455.403 - Resolution	≤ 0.025	0.02059	Pass

5.2 Precision :

- ☒ Test for reproducibility of a set of measurement.

Parameter	Specification	Test Result	Pass/Fail
As 193.696	%RSD $\leq 1\%$	0.76	Pass
Zn 213.856	%RSD $\leq 1\%$	0.67	Pass
Mn 257.610	%RSD $\leq 1\%$	0.80	Pass
La 379.478	%RSD $\leq 1\%$	0.64	Pass
Ba 455.403	%RSD $\leq 1\%$	0.60	Pass
Ba 493.408	%RSD $\leq 1\%$	0.55	Pass

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO., LTD.

ICP-OES/Optima8300 Preventive Maintenance (PM)

ห้องปฏิบัติการวิเคราะห์

เลขทะเบียน ว-24

☒ Run an Axial & Radial BEC according to the A&T spec.

5.1 Axial BEC Cd:

Method "BEC-XL" For Samples "IB (2%HNO3)" and "IS (N930-0221/100)", record intensities.

Calculated BEC: $BEC = (IB * Conc\ of\ Std) / (IS - IB)$. Where Conc of Std = 500 PPB

Element	Conc.	IB	IS	
Cd 226	500	4427.9	130911	
IB*Conc	IS-IB	BEC	Spec	Pass/Fail
2213950	126483.1	17.50	<150 PPB	Pass

5.2 Radial BEC Mn:

Method "BEC-RL" For Samples "IB (2%HNO3)" and "IS (N069-1579)", record intensities.

Calculated BEC: $BEC = (IB * Conc\ of\ Std) / (IS - IB)$. Where Conc of Std = 1,000 PPB

Element	Conc.	IB	IS	
Mn 257	1,000	2770.2	87479.6	
IB*Conc	IS-IB	BEC	Spec	Pass/Fail
2770200	84709.4	32.70	<45 PPB	Pass

7. Review:

- ☐ Review with the customer PM work performed.
- ☐ Discuss recommended customer supplied materials to have on hand.
- ☐ Attach PM sticker.



ICP-OES/Optima8300 Preventive Maintenance (PM) ๗

ห้องปฏิบัติการวิเคราะห์ห้อง

เลขทะเบียน ว-244

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for ICP-OES/Optima8300 have been completed.

This ICP-OES/Optima8300 Passes ☒ Fails ☐ the preventive maintenance.

Review of Preventive Maintenance:

Authorized PerkinElmer Representative:

Date:
01-Sep-2022
(DD-MMM-YYYY)

Authorized Customer Representative:

Date:
01-Sep-2022
(DD-MMM-YYYY)

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO., LTD.

ICP-OES/Optima8300 Preventive Maintenance (PM)

ของปฏิบัติการวิเคราะห์

เลขทะเบียน ว-244

ใบรับรองการสอบเทียบ “เครื่อง pH Meter”

(Calibration Certificate of pH Meter)



ห้องปฏิบัติการวิเคราะห์เอกซน
เลขทะเบียน ว-244



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/1 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL: 0-2717-3000-27 FAX: 0-2719-9484



Cert.No.: 22CHO508

Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Mettler Toledo
Model : SevenCompact
Serial No. : B224014992
ID No. : 0403-0101-10
Condition As-Received: Used Item
Received Date : 30 August 2022
Calibration Date : 31 August 2022
Reference : 2208-0862ON-8
Submitted by : Emex Association Co.,Ltd.
27,29 Soirama II, Soi 30,
Bangmod, Jomthong, Bangkok 10150
Calibration Place : ห้องปฏิบัติการ 7
Ambient Temperature : (24.8 - 24.4) °C
Relative Humidity : (48.1 - 47.9) %
Calibration Procedure : In - house method :
- CP-OCH2 by direct measurement with standard
voltage calibrator and direct measurement with
certified reference material (CRM)

Calibrated by :

Approved by :

Approved Signatory

Issue Date :

7 September 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be valid if used for purposes other than those stated on the certificate.
Approval of the head of Calibration and Testing Services
EMEX Environmental and Medical Expert
EMEX ASSOCIATION CO.,LTD.

ห้องปฏิบัติการวิเคราะห์เอกชน
เลขทะเบียน ว-244

A 0043434



Cert. No.: 22CHO508

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	46530031	130RC098	21E3245	07 Oct 2022
2) Digital Thermometer	-	130RC113	21T1689	23 Sep 2022

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through Merck Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15185-01-00

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
* pH 2.01	Merck	HC03981033	30 Sep 2023
pH 4.008	CPA chem	823320	20 June 2024
pH 6.985	CPA chem	794122	14 Feb 2023
pH 10.015	CPA chem	794124	14 Feb 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : pH Measurement

Performing four buffers standard curve by using buffer nominal pH (2,4,7,10)

<u>Unit Under Calibration</u>	<u>Standard pH Buffer Solution</u>	<u>Actual pH Reading</u>	<u>Actual mV Reading (mV)</u>	<u>Uncertainty of pH measurement (±)</u>	<u>Coverage factor k</u>
pH Electrode S/N.: 5441612	*2.01	2.015	295.4	0.21	2.00
	4.008	4.004	180.2	0.0067	2.15
	6.985	6.989	6.0	0.0092	2.00
	10.015	10.005	-169.1	0.019	2.21

Remark : * = Not NSC-ONSC Accredited

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO.,LTD.

กองปฏิบัติการวิเคราะห์เอกชน
จดทะเบียน ๖-๖14

a 1124784



Cert.No.: 22CHO508

Page.: 3 of 3

Calibration Results**Function : mV Measurement****Performing standard curve by Fluke at pH (2,4,7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: B224014992	0.000	414.12	414.2	0.000	0.058	2.00
	1.000	354.96	355.1	1.000	0.058	2.00
	2.000	295.80	296.0	2.000	0.11	2.52
	3.000	236.64	236.8	3.000	0.058	2.00
	4.000	177.48	177.7	4.000	0.058	2.00
	5.000	118.32	118.5	5.000	0.058	2.00
	6.000	59.16	59.4	6.000	0.058	2.00
	7.000	0.00	0.3	7.000	0.058	2.00
	8.000	-59.16	-58.9	8.000	0.058	2.00
	9.000	-118.32	-118.0	9.000	0.058	2.00
	10.000	-177.48	-177.1	10.000	0.058	2.00
	11.000	-236.64	-236.3	11.000	0.058	2.00
	12.000	-295.80	-295.4	12.000	0.058	2.00
	13.000	-354.96	-354.6	13.000	0.11	2.52
	14.000	-414.12	-413.7	14.000	0.058	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



ห้องปฏิบัติการวิเคราะห์เอกชน
เลขทะเบียน ๖-244

a 1124783

ใบรับรองการสอบเทียบ “เครื่อง Inductively Coupled Plasma (ICP-OES)”
(Calibration Certificate of Inductively Coupled Plasma (ICP-OES))

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO., LTD.

ห้องปฏิบัติการวิเคราะห์เอกชน
เลขทะเบียน ว-244

ICP-OES/Optima8300 Preventive Maintenance (PM)

Company Name:	บริษัท เอ็มเม็กซ์แอสโซซิเอชั่น จำกัด		
Address (Instrument Location):	27, 29 ซอยพระรามที่ 2 ซอย 30 แขวงบางมด เขตจอมทอง กทม		
Serial Number:	078S1604262	PM Number:	2 of 2
Customer Name (if applicable):		Telephone Number:	
Service Engineer Name:		Service Order Number:	WO-01844676
Date PM Performed: (DD-MMM-YYYY)	01-Sep-2022	Next PM Due Date: (DD-MMM-YYYY)	01-Mar-2023
Standard Labor Hours to Complete PM :		4 hours	

Part Number	Release	Publication Date	
09370141 Rev.3	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PerkinElmer / Optima8300 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

EMEX Environmental
and Medical Expert

ICP-OES/Optima8300 Preventive Maintenance (PM)

EMEX ASSOCIATION CO., LTD.

Page 1 of 7

ห้องปฏิบัติการวิเคราะห์เอกสาร

เลขทะเบียน ว-244

Component List

Component / Specific Model	Serial #	Configuration Notes

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
09995098	Air Fiter-Spectrometer	NA
N077520	Air Fiter-RF Generetor	NA
09992731	Axial Window	NA
B0810377	Radial Window	NA
N0770438	O-ring kit, injector support adapter	NA
N0780437	O-ring kit, torch	NA

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N0691579	Muti-Element Standard	AR	58-146CRX1	11/23
N9300221	DL Standard diluted 100 X	AR	58-169CRY1	11/23
N0582152	Wave Cal Solution	AR	58-110CRX1	08/23
N9302946	VIS Wavecal Solution	AR	58-145CRT1	11/23

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO.,LTD.

ICP-OES/Optima8300 Preventive Maintenance (PM) ห้องปฏิบัติการวิเคราะห์สิ่งแวดล้อม

เลขทะเบียน ว

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Ask customer about unit's performance since last visit.
- ☒ Check incoming AC line voltage under load for proper levels and grounding.
- ☒ Is the instrument operational? If not, please comment.

2. Mechanical:

- ☒ Inspect and clean all fans and filters.
- ☒ Inspect and replace torch components and necessary.

Torch Components Replaced: ☐ Yes ☒ No

- ☒ Inspect all tubing for signs of cracking or leaking and replace as necessary.

Tubing Replaced: ☒ Yes ☐ No

- ☒ Inspect the peristaltic pump for proper operation.
- ☒ Check and adjust if necessary, the external nitrogen, argon shear gas and water supply pressures.
- ☒ Check and adjust if necessary, the internal nitrogen, main argon, torch argon and shear gas pressures.

Regulator	Measured Pressure	Set Pressure
Nitrogen	NA	NA (calibrated in Factory)
Main Argon	76	76 psig
Torch Argon	67	67 psig
Shear Gas	65	65 psig
Water	35	35 psi

- ☒ Check shear gas nozzle for blockages and proper, uniform flow.
- ☒ Inspect nitrogen Hi/Low purge and shear gas solenoids for proper function.
 - ☒ Inspect the function of all spectrometer motors. Drive the motors from the Spectrometer DCM. (slits, XY motor)
- ☒ Inspect the function of the pneumatic shutter for proper operation.
 - ☒ Perform preventative maintenance on the chiller as required. Make the customer aware of the importance of maintaining the chiller fluid level and filter replacement.
- ☒ Drain air compressor surge tank.
- ☒ Clean exterior of instrument.
- ☒ Visually inspect all PC boards for cleanliness and signs of corrosion.

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO., LTD.

ICP-OES/Optima8300 Preventive Maintenance (PM)

ห้องปฏิบัติการ วิเคราะห์


เลขทะเบียน ว-244

3. Electrical

☒ Check all RF generator and spectrometer power supply voltages.

Spectrometer Control/Interface PCB Test Points

TP	Voltage (DC)	Tolerance	Description
1	+24V	$\pm 500\text{mV}$	From Main Supply
2	+12V	$\pm 20\text{mV}$	Onboard – For View X/Y Motors
3	+15V	$\pm 600\text{mV}$	Onboard – For Spectrometer Control Electronics
4	-15V	$\pm 600\text{mV}$	Onboard – For Spectrometer Control Electronics
5	+3.3V	$\pm 100\text{mV}$	Onboard – Source of 3.3V for Icarus Engine and SCB elect.
6	+2.5V	$\pm 25\text{mV}$	Onboard – For Xilinx FPGA
7	+5.0V		From Main Supply
8			$\pm 5.0\text{ GND}$
9			$\pm 5.0\text{ GND}$
10			$\pm 5.0\text{ GND}$
11			$\pm 5.0\text{ GND}$
12			$\pm 5.0\text{ GND}$
13	+1.5V	$\pm 45\text{mV}$	Onboard – For Icarua Engine
22	+6.5V	-0mV, + 100mV	UV TEC
23	+6.5V	-0mV, + 100mV	VIS TEC

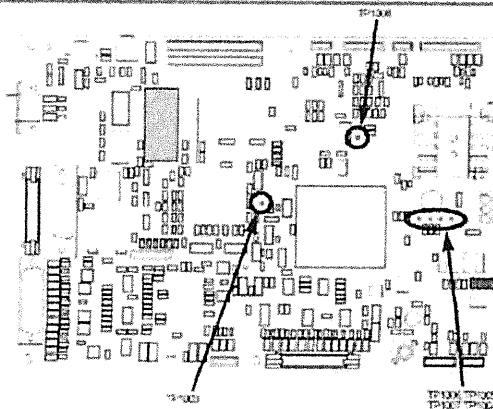

RF Controller PCB Test Points

TP	Voltage (DC)	RF Control PCB Location
1005	-14 to -16 (-15)	Right of U1001
1006	23-25 (24)	Right of U1001
1008	4.75-5.25 (5)	Upper Right of U1001
1003	14-16 (15)	Upper Left of U1001
1004	Ground	Upper Right of U1001

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO., LTD.

☒ Run instrument diagnostic checks from the appropriate Device Control Module.

RF Generator:

- ☒ Check the RF generator status screens.
☒ Check the function of all interlocks.

Spectrometer:

- ☒ Check the spectrometer status screens. Ensure Ready mode with no fatal errors.
☒ Check the spectrometer optical tub temperatures (top, bottom, fin, optical base).
☒ Check detector temperatures.
☒ Check TEC voltages (6.5VDC)

4. Optical:

- ☒ Clean or replace the axial and radial view windows as necessary.

Axial Window Replaced: ☐ Yes ☒ No

Radial Window Replaced: ☐ Yes ☒ No

5. PM Performance Tests:

- ☒ Perform View Align.

5.1 Spectral Resolution :

- ☒ Measure the spectrometers ability to separate two adjacent wavelengths.

Parameter	Specification	Test Result	Pass/Fail
As 193.696 - Resolution	≤ 0.007	0.00494	Pass
Ni 231.604 - Resolution	≤ 0.008	0.00599	Pass
Ni 341.476 - Resolution	≤ 0.012	0.00771	Pass
La 408.672 - Resolution	≤ 0.020	0.01508	Pass
Ba 455.403 - Resolution	≤ 0.025	0.02059	Pass

5.2 Precision :

- ☒ Test for reproducibility of a set of measurement.

Parameter	Specification	Test Result	Pass/Fail
As 193.696	%RSD $\leq 1\%$	0.76	Pass
Zn 213.856	%RSD $\leq 1\%$	0.67	Pass
Mn 257.610	%RSD $\leq 1\%$	0.80	Pass
La 379.478	%RSD $\leq 1\%$	0.64	Pass
Ba 455.403	%RSD $\leq 1\%$	0.60	Pass
Ba 493.408	%RSD $\leq 1\%$	0.55	Pass

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO., LTD.

ICP-OES/Optima8300 Preventive Maintenance (PM)

ห้องปฏิบัติการวิเคราะห์

เลขทะเบียน ว-2

☒ Run an Axial & Radial BEC according to the A&T spec.

5.1 Axial BEC Cd:

Method "BEC-XL" For Samples "IB (2%HNO3)" and "IS (N930-0221/100)", record intensities.

Calculated BEC: $BEC = (IB * Conc\ of\ Std) / (IS - IB)$. Where Conc of Std = 500 PPB

Element	Conc.	IB	IS	
Cd 226	500	4427.9	130911	
IB*Conc	IS-IB	BEC	Spec	Pass/Fail
2213950	126483.1	17.50	<150 PPB	Pass

5.2 Radial BEC Mn:

Method "BEC-RL" For Samples "IB (2%HNO3)" and "IS (N069-1579)", record intensities.

Calculated BEC: $BEC = (IB * Conc\ of\ Std) / (IS - IB)$. Where Conc of Std = 1,000 PPB

Element	Conc.	IB	IS	
Mn 257	1,000	2770.2	87479.6	
IB*Conc	IS-IB	BEC	Spec	Pass/Fail
2770200	84709.4	32.70	<45 PPB	Pass

7. Review:

- ☐ Review with the customer PM work performed.
- ☐ Discuss recommended customer supplied materials to have on hand.
- ☐ Attach PM sticker.



ICP-OES/Optima8300 Preventive Maintenance (PM) ๗

ห้องปฏิบัติการวิเคราะห์

เลขทะเบียน ว-244

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for ICP-OES/Optima8300 have been completed.

This ICP-OES/Optima8300 Passes ☒ Fails ☐ the preventive maintenance.

Review of Preventive Maintenance:

Authorized PerkinElmer Representative:

Date:
01-Sep-2022
(DD-MMM-YYYY)

Authorized Customer Representative:

Date:
01-Sep-2022
(DD-MMM-YYYY)

EMEX Environmental
and Medical Expert
EMEX ASSOCIATION CO., LTD.

ICP-OES/Optima8300 Preventive Maintenance (PM)

ห้องปฏิบัติการวิเคราะห์

เลขทะเบียน ว-244

ใบรับรองการสอบเทียบ “เครื่อง Spectrophotometer”
(Calibration Certificate of Spectrophotometer)



ห้องปฏิบัติการวิเคราะห์เอกชน
เลขทะเบียน ว-244



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-22-439

Page : 1 of 3

CERTIFICATE OF CALIBRATION

Equipment	:	Spectrophotometer
Manufacturer	:	Thermo Scientific
Model	:	Genesys 10S VIS
Serial No.	:	2E8R020104
ID No.	:	N/A
Customer	:	Emex Association Co., Ltd.
	:	27, 29 Soi Rama 2, Soi 30, Rama Road,
	:	Bangmod, Jomthong, Bangkok 10150
Location	:	Becthai Laboratory
Date of Receipt	:	15 June 2022
Date of Calibration	:	16 June 2022
Date of Issue	:	17 June 2022
Ambient Temperature	:	(25±10) °C
Relative Humidity	:	(60±20) %
Condition As-Received	:	Used Item

Calibrated by



Approved by



The reported expanded uncertainty of measurement was based on a combined standard uncertainty multiplied by a coverage factor $k=2.00$, providing a level of confidence of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Indicated values are valid for the state of the Spectrophotometer at the time of calibration only.



ห้องปฏิบัติการวิเคราะห์เอกสาร

เลขทะเบียน ว-244



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-22-439

Page : 2 of 3

CALIBRATION REPORT

Conditions of this result of calibration

1. Reference Standard Material :

<u>Material</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert.No.</u>	<u>Due date</u>
Holmium Glass Filter	RM-HG	12705	98236	12 Feb 24
Didymium Glass Filter	RM-DG	13498	98233	12 Feb 24
Neutral Density Filter	RM-1N2N3N	8323	98259	13 Feb 24

2. Traceability : This certification is traceable to the International System of Unit maintained at:

The Starna Scientific Ltd. Accredited Calibration Laboratory No. 0659.

3. Method of calibration :

The calibration procedure was carried out according to the Guide to CPM-CAL-02 based on ASTM E275-08 (2013) and-
ASTM E925-09 (2014).

4. Result of calibration :

(✓) without adjustment

() after adjustment

5. Equipment Specifications:

Spectral Bandwidth :	5	nm
Data Interval :	1	nm
Scan Speed :	Slow	nm/min

EMEX Environment and Medical Exp
EMEX ASSOCIATION CO.,L

ห้องปฏิบัติการวิเคราะห์เอก

เลขทะเบียน ว-244



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1
 E-mail: bkk@beccthai.com Website: www.beccthai.com



Certificate No. : CAL-22-439

Page : 3 of 3

CALIBRATION REPORT

Wavelength Calibration

Certified Values of Reference Material (nm)	Nominal Value (nm)	UUC*Reading (nm)	Error (nm)	Uncertainty of Measurement ($\pm$ nm)
361.40	361.40	362	0.60	0.59
528.59	528.59	530	1.41	0.59
879.68	879.68	880	0.32	0.59

Photometric Calibration for Visible

Wavelength (nm)	Certified Values of Reference Material (A)	UUC* Reading (A)	Error (A)	Uncertainty of Measurement ($\pm$ A)
420.0	Zero	0.000	0.0000	0.0028
	0.5716	0.575	0.0034	0.0031
	0.7358	0.739	0.0032	0.0034
	1.0713	1.079	0.0077	0.0032
440.0	Zero	0.000	0.0000	0.0028
	0.561	0.560	-0.0010	0.0031
	0.718	0.717	-0.0010	0.0031
	1.0459	1.047	0.0011	0.0032
465.0	Zero	0.000	0.0000	0.0028
	0.5111	0.513	0.0019	0.0032
	0.6618	0.663	0.0012	0.0030
	0.9635	0.967	0.0035	0.0034
546.1 (546.0)	Zero	0.000	0.0000	0.0028
	0.5222	0.522	-0.0002	0.0034
	0.6687	0.668	-0.0007	0.0029
	0.9768	0.978	0.0012	0.0043
590.0	Zero	0.000	0.0000	0.0028
	0.5541	0.553	-0.0011	0.0033
	0.6975	0.697	-0.0005	0.0032
	1.0206	1.021	0.0004	0.0045
635.0	Zero	0.000	0.0000	0.0028
	0.5398	0.539	-0.0008	0.0033
	0.6658	0.666	0.0002	0.0033
	0.9741	0.975	0.0009	0.0045

Remark : Each individual filter is measured against the empty filter holder (blank) used to zero the Spectrophotometer.

Note:

UUC* : Unit Under Calibration

EMEX Environmental
 and Medical Exp
EMEX ASSOCIATION CO.,L
 ห้องปฏิบัติการวิเคราะห์เอก
 - End of Report

เลขทะเบียน ว-2



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

Customer : <u>S.P.S.Consulting Service Co.,Ltd</u>	Date Tested: <u>January 11, 2023</u>	
	Recommendation Recertification	
Address : <u>7 Soi Phaholyothin 24</u>	Period <u>6</u> Months	
<u>Paholyothin Road</u>	Recertification Due: <u>July 11, 2023</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	Date Last Certified: <u>July 11, 2022</u>	
User Name: XXXXXXXXXX	Visit Number: <u>2 of 2</u>	
Phone: XXXXXXXXXX	PerkinElmer Phone: <u>02-719-6420 ext 206</u>	
Fax: <u>02-513-4221</u>	PerkinElmer Fax: <u>02-318-5597</u>	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
MODEL	SERIAL NUMBER	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
TESTED EQUIPMENT	CALIBRATION NUMBER	EXPIRATION
<u>IPV Methods</u>		
TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>May 30, 2023</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>February 28, 2023</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>August 30, 2023</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>November 30, 2023</u>
CUSTOMER SUPPLIED	COMMENTS	CUSTOMER INITIALS
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER 077C7042401**DATE TESTED** January 11, 2023**1. MECHANICAL CHECKS**

- | | |
|--|-----------------------------|
| A. Inspect and clean all fans and filters. | ☐ OK |
| B. Inspect and replace as necessary, all torch components including the RF coil. | ☐ OK |
| C. Inspect all tubing for sign of clacking or leaking. | ☐ OK |
| D. Adjust water and gas pressure regulator settings. | ☐ OK |
| E. Inspect and leak check pneumatics drawers. | ☐ OK |
| F. Clean the exterior of the instrument. | ☐ OK |

2. OPTICAL CHECKS

- | | |
|---|-----------------------------|
| A. Inspect and clean all optical components. | ☐ OK |
| B. As required, check and replace all purgefilters. | ☐ OK |
| C. Recheck optical alignment. | ☐ OK |

3. COOLING SYSTEM CHECKS

- | | |
|---|------------------------------|
| A. Perform preventive maintenance on chiller. | ☐ OK |
| B. Flush out the chiller every year. | ☐ N/A |

4. PERFORMANCE CHECKS

- | | |
|----------------------------|-----------------------------|
| A. Torch View Alignment. | ☐ OK |
| B. Wavelength Calibration. | ☐ OK |



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER : 077C7042401
DATE TESTED : January 11, 2023

PARAMETER		SPECIFICATION		FINAL VALUE	
Spectral Resolution : UV	As 193.696 nm	≤ 0.007		<u>0.00504</u>	
	Ni 231.604 nm	≤ 0.008		<u>0.00646</u>	
	Ni 341.476 nm	≤ 0.012		<u>0.00768</u>	
Spectral Resolution : VIS	La 408.672 nm	≤ 0.020		<u>0.01597</u>	
	Ba 455.403 nm	≤ 0.025		<u>0.02185</u>	
Precision					
	As 193.656 nm	% RSD	< 1.0	<u>0.89</u>	%
	Zn 213.856 nm	% RSD	< 1.0	<u>0.77</u>	%
	Mn 257.610 nm	% RSD	< 1.0	<u>0.51</u>	%
	La 379.478 nm	% RSD	< 1.0	<u>0.44</u>	%
	Ba 455.403 nm	% RSD	< 1.0	<u>0.44</u>	%
	Ba 493.408 nm	% RSD	< 1.0	<u>0.46</u>	%
Detection Limits : Axial	Tl 190.080 nm	3(sd)		<u>4.04</u>	ppb
	As 193.696 nm	3(sd)		<u>3.58</u>	ppb
	Pb 220.353 nm	3(sd)		<u>1.90</u>	ppb
Detection Limits : Radial	As 193.696 nm	3(sd)		<u>47.72</u>	ppb
	Zn 213.856 nm	3(sd)		<u>1.02</u>	ppb
	Mn 257.610 nm	3(sd)		<u>0.68</u>	ppb
	La 379.478 nm	3(sd)		<u>1.43</u>	ppb
	Ba 455.403 nm	3(sd)		<u>0.10</u>	ppb
	Ba 493.408 nm	3(sd)		<u>0.36</u>	ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd 226.502 nm	≤ 150 ppb		<u>58.36</u>	
BEC : Radial (IB X 1000)/(IS-IB)	Mn 257.610 nm	≤ 45 ppb		<u>13.26</u>	



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER 077C7042401**DATE TESTED** January 11, 2023**Remarks :**

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested

☒

meets

☐

does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,
including warranty terms.

Service Department PerkinElmer Ltd.

Authorized Representative:

(

Service Engineer

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : SP22018

Pages 1 of 3

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY

Condition As Found : GOOD

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON, CHATUCHAK,
BANGKOK 10900, THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (24.4 ± 5) °C
Relative Humidity : (60.1 ± 25) %

Received Date : 30 AUGUST 2022
Calibration Date : 30 AUGUST 2022
Date of Issue : 31 AUGUST 2022

Calibrated by :

Approved by :

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : SP22018

Job No. : VC65SP0008

Pages : 2 of 3

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01,ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	87569	13/10/2022
Didymium liquid	RM-DL	28912	87588	15/10/2022
Neutral density filter	RM-1N2N3N	13877	87600	15/10/2022
Potassium dichromate solutions	RM-0204060810	14204	87614	16/10/2022
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology,NIST.

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.4	0.15	0.16	2.00
	467.82	467.8	-0.02	0.16	2.00
	536.56	536.5	-0.06	0.16	2.00
	640.50	640.5	0.00	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.2	0.26	0.16	2.00

UUC* = Unit Under Calibration

Continuation of Calibration Certificate

Cert. No. : SP22018

Job No. : VC65SP0008

Pages : 3 of 3

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Filter: S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0524	1.0539	0.0015	0.0028	2.00
		29914	0.7	0.7454	0.7459	0.0005	0.0029	2.00
		29381	0.5	0.5426	0.5426	0.0000	0.0028	2.00
	546.1	29360	1.0	0.9822	0.9810	-0.0012	0.0028	2.00
		29914	0.7	0.6962	0.6960	-0.0002	0.0028	2.00
		29381	0.5	0.5076	0.5070	-0.0006	0.0029	2.00
	590.0	29360	1.0	1.0221	1.0202	-0.0019	0.0028	2.00
		29914	0.7	0.7238	0.7230	-0.0008	0.0029	2.00
		29381	0.5	0.5364	0.5360	-0.0004	0.0031	2.00
	635.0	29360	1.0	0.9751	0.9732	-0.0019	0.0028	2.00
		29914	0.7	0.6912	0.6902	-0.0010	0.0029	2.00
		29381	0.5	0.5214	0.5210	-0.0004	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2436	0.2419	-0.0017	0.0101	2.00	
		40	0.4905	0.4855	-0.0050	0.0115	2.00	
		60	0.7453	0.7388	-0.0065	0.0067	2.00	
		80	0.9920	0.9839	-0.0081	0.0071	2.00	
		100	1.2487	1.2414	-0.0073	0.0073	2.00	

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.0001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 1100 nm-190 nm

Scanning Speed 7.5 nm/min

Data Pitch 0.1 nm

Band width(Wavelength) 1.0 nm

Band width(Vis) 1.0 nm

Band width(Uv) 1.0 nm

Stray Light UUC* Reading at 220 nm**

Transmission T(%) Absorbance(A)

0.0107

3.9886

**Specific Acceptance :

Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A

**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate