

## ภาคผนวกที่ 4

---

### ใบรับรองการสอบเทียบเครื่องมือ

## Certificate of Calibration

**Certificate No. :** 65-200253-1

**Page : 1 of 2**

**Submitted by :** M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

**Equipment :** Electronic Balance

Manufacturer : Sartorius

Model : BSA224S-CW

Serial No. : 35090472

ID No. : MET-EB 02/60

Capacity : 220 g

Resolution : 0.0001 g

**Environment :**

On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (25.6 to 25.8) °C

Relative Humidity : (57.3 to 57.8) %

Air Pressure : 1005.0 mbar

**Date of Received :** 10 August 2022

**Date of Calibration :** 10 August 2022

**Date of Issue :** 11 August 2022

**Calibrated by :** Akaradath Thippichai

**Calibration Method :** In-house method CAL-M2001 based on UKAS Publication ref : LAB 14  
Edition 5, July 2015

**Reference Standard Instruments :** This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02213103	18 Nov 2022	National Institute of Metrology (Thailand), (NIMT)

Approved by :



Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



## Certificate of Calibration

**Certificate No. :** 65-200253-1

**Page :** 2 of 2

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty $\pm$ (g)
0.05	0.0000	0.00011
0.1	0.0000	0.00013
0.5	0.0000	0.00013
1	0.0000	0.00011
5	0.0000	0.00011
10	0.0001	0.00011
50	0.0001	0.00013
100	0.0000	0.00020
150	0.0000	0.00038
200	0.0000	0.00038


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2.11$ , providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A B C D E  
0.0001 0.0001 0.0001 0.0000 0.0000 g



Repeatability

Load test : 200 g

Stdev. : 0.00005 g

- o0o -



## Certificate of Calibration

**Certificate No. :** 64-400425-5

**Page : 1 of 2**

**Submitted by :** M E T Company Limited  
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

**Equipment :** Air Chamber (Incubator)  
Manufacturer : M-LAB Model : BIC-140  
Range : N/A °C Resolution : 0.1 °C  
Serial No. : 240412 ID No. : MET-BI01/55

**Environment :** On site calibration was carried out at the Laboratory, M E T Company Limited  
Ambient Temperature : (27.0 to 28.0) °C  
Relative Humidity : (50 to 55) %  
Line Voltage : (210.0 to 210.8) V

**Date of Received :** 10 August 2022

**Date of Calibration :** 10 August 2022

**Date of Issue :** 13 August 2022

**Calibrated by :** Permporn Chanpu

**Calibration Method :** CAL-M4004, TLAS G-20  
The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units  
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400032	65-400274-1	25 Nov 2022	National Institute of Metrology Thailand (NIMT)

Approved by



Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.





## Certificate of Calibration

Certificate No. :64-400425-5


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

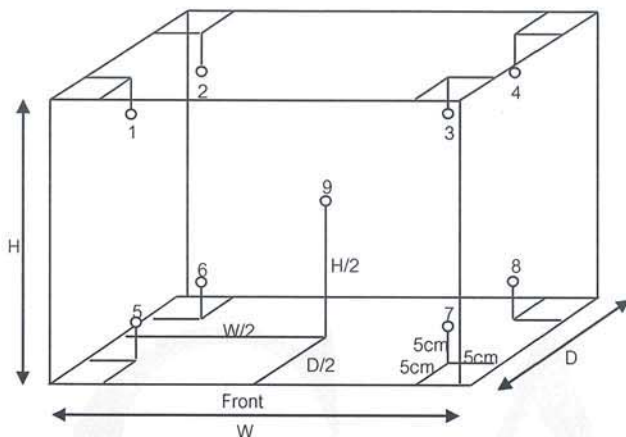

Inside of Chamber

W = 0.37 m

D = 0.33 m

H = 1.14 m

Capacity = 0.14 m<sup>3</sup>

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	19.8	19.7	19.6	19.6	20.4	20.2	20.3	19.8	19.9	0.54

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	0.6	0.1	1.0

**Remark** The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



## Certificate of Calibration

**Certificate No. :** 65-400666-1

**Page : 1 of 2**

**Submitted by :** M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

**Equipment :** Air Chamber (Incubator)

Manufacturer : M-LAB

Model : BIC-140

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 1022

ID No. : MET-BI02/64

**Environment :** On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (25.2 to 25.5) °C

Relative Humidity : (40 to 45) %

Line Voltage : (210.0 to 210.8) V

**Date of Received :** 27 December 2022

**Date of Calibration :** 27 December 2022

**Date of Issue :** 28 December 2022

**Calibrated by :** Permpon Chanpu

**Calibration Method :** CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units  
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400043	65-400552-1	25 Apr 2023	National Institute of Metrology Thailand (NIMT)

Approved by :

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.







## Certificate of Calibration

**Certificate No. :** 65-400424-2

**Page : 1 of 2**

**Submitted by :** M E T Company Limited  
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

**Equipment :** Air Chamber (Oven)  
Manufacturer : Binder Model : ED53  
Range : N/A °C Resolution : 1 °C  
Serial No. : 13-07419 ID No. : MET-OV02/57

**Environment :** On site calibration was carried out at the Laboratory, M E T Company Limited  
Ambient Temperature : (27.0 to 28.0) °C  
Relative Humidity : (50 to 55) %  
Line Voltage : (210.0 to 210.8) V

**Date of Received :** 10 August 2022

**Date of Calibration :** 10 August 2022

**Date of Issue :** 13 August 2022

**Calibrated by :** Permpoon Chanpu

**Calibration Method :** CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units  
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400030	65-400272-1	24 Nov 2022	National Institute of Metrology Thailand (NIMT)

Approved by :

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.





## Certificate of Calibration

**Certificate No. : 65-400424-2**


**Page : 2 of 2**

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

This instrument was setting air ventilation at position 0 (close)

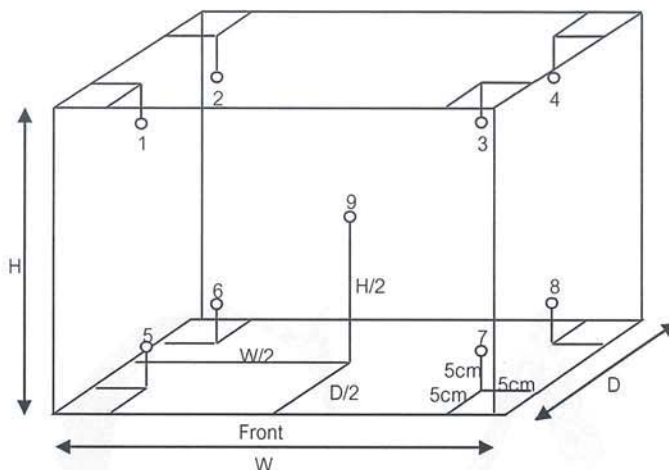

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.40 m

Capacity = 0.05 m<sup>3</sup>

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104	110	110	105.0	105.0	104.7	105.0	104.4	104.5	104.0	103.7	104.2	0.95
180	184	184	180.8	182.0	179.4	180.8	180.8	180.8	180.3	180.0	180.0	1.2

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104	110	110	1.0	0.2	1.7
180	184	184	2.3	0.3	3.0

**Remark** The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



## Certificate of Calibration

**Certificate No. :** 65-400424-1

**Page : 1 of 2**

**Submitted by :** M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

**Equipment :** Air Chamber (Oven)

Manufacturer : Memmert

Model : UM 100

Range : N/A °C

Resolution : 0.1 °C

Serial No. : b197.0985

ID No. : MET-OV01/46

**Environment :** On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (27.0 to 28.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (210.0 to 210.8) V

**Date of Received :** 10 August 2022

**Date of Calibration :** 10 August 2022

**Date of Issue :** 13 August 2022

**Calibrated by :** Permpon Chanpu

**Calibration Method :** CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units  
Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400032

65-400274-1

25 Nov 2022

National Institute of Metrology Thailand (NIMT)

Approved by

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.







## Certificate of Calibration

**Certificate No. :** 65-400424-3

**Page : 1 of 2**

**Submitted by :** M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

**Equipment :** Air Chamber (Refrigerator)

Manufacturer : Sanden Intercool

Model : YPR-068S

Range : N/A °C

Resolution : 1 °C

Serial No. : YPR0659S-141200060R

ID No. : MET-RE03/59

**Environment :** On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (29.8 to 31.5) °C

Relative Humidity : (55 to 58) %

Line Voltage : (220.8 to 222.8) V

**Date of Received :** 10 August 2022

**Date of Calibration :** 10 August 2022

**Date of Issue :** 13 August 2022

**Calibrated by :** Bunjerd Masri

**Calibration Method :** CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400046 & 400023

65-400157-1

02 Oct 2022

National Institute of Metrology Thailand (NIMT)

Approved by :



Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.





## Certificate of Calibration

**Certificate No. : 65-400424-3**


**Page : 2 of 2**

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

This instrument was setting air ventilation at position 0 (close)

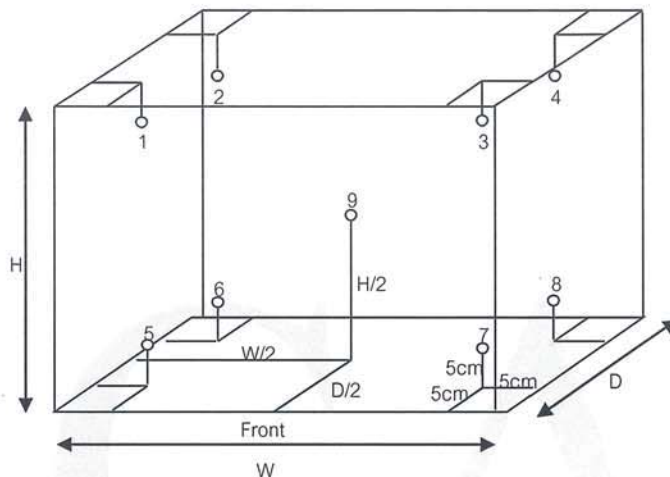

Inside of Chamber

W = 0.58 m

D = 0.60 m

H = 1.45 m

Capacity = 0.50 m<sup>3</sup>

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
3	2	2	3.7	3.7	4.0	3.7	3.0	3.5	2.8	3.4	2.9	0.84

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
3	2	2	1.2	0.2	1.5

**Remark** The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- o0o -



## Certificate of Calibration

**Certificate No. :** 66-420002-1

**Page :** 1 of 2

**Submitted by :** M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

**Equipment :** pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : pH 150

Range : -2.00 to 16.00 pH

Resolution : 0.01 pH

Serial No. : 2657036

ID No. : MET-PH04/60

Electrode

Model : N/A

Serial No. : 66365

**Environment :** Ambient Temperature :  $(25 \pm 2) ^\circ \text{C}$

Relative Humidity :  $(50 \pm 15) \%$

**Date of Received :** 05 January 2023

**Date of Calibration :** 11 January 2023

**Date of Issue :** 11 January 2023

**Calibrated by :** Bunjerd Masri

**Calibration Method :** In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

**Reference Standard Instruments :** This certification is traceable to the International System of Units

### 1. Multiproduct Calibrator

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
440001	21E997	17 Mar 2023	National Institute of Metrology Thailand (NIMT)

### 2. Standard Buffer Solution

<u>pH</u>	<u>Cert. No.</u>	<u>Lot No.</u>	<u>Exp. Date</u>	<u>Traceability</u>
4.008	61235182	857394	11 Dec 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61267169	857395	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61260481	857396	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



## Certificate of Calibration

**Certificate No. : 66-420002-1**

**Page : 2 of 2**

**Result of Calibration :**

**UUC Condition As-Received :** Good

**Function :** Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage ( mV )	Nominal Value ( pH )	UUC Reading		Correction ( mV )	Uncertainty ( ± mV )
			( pH )	( mV )		
4, 7, 10	177.4800	4	4.00	177.1	0.4	0.060
	0.0000	7	6.99	-0.1	0.1	0.060
	-177.4800	10	10.00	-177.3	-0.2	0.060

**Function :** pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer ( pH )	UUC Reading ( pH )	Correction ( pH )	Uncertainty ( ± pH )
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- ๐0๐ -







National Institute of Metrology (Thailand)

## Certificate of Calibration



Certificate No. : AA-2018-22  
Issued by : Acoustics Laboratory  
Acoustics and Vibration Group

Page 1 of 5 pages

MEASUREMENT ITEM : Sound Calibrator  
MANUFACTURER : RION  
MODEL/TYPE : NC-75  
SERIAL NUMBER : 34480442  
CUSTOMER : MET Co., Ltd.  
36/659 Moo 6, T. Bangrakphatthana,  
A. Bangbuathong, Nonthaburi 11110  
MEASUREMENT DATE : 28 September 2022

*The reported measurement result relates only to the measurand and applies only at the time of measurement.*

*The calibration results only marked with an asterisk \* in this certificate are not included in the scope of accreditation.*

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. This calibration certificate may not be reproduced other than in full except with the permission of the Director of National Institute of Metrology (Thailand).

Reference	Date	Authorized Signatory	Person in charge
AUVC844-01/22	29 September 2022		

This certificate is consistent with the capabilities that are included in Appendix C of the MRA drawn up by the CIPM. Under the MRA, all participating institutes recognize the validity of each other's calibration and measurement certificates for the quantities, ranges and measurement uncertainties specified in Appendix C (for details see <http://www.bipm.org>).

National Institute of Metrology (Thailand)

Ministry of Higher Education, Science, Research and Innovation

3/4-5 Moo 3, Klong 5, Klong Luang, Pathumthani 12120, Thailand. Tel: (66) 2577 5100, Fax: (66) 2577 3659

75/7 Rama VI Road, Rachathewi, Bangkok 10400, Thailand. Tel: (66) 2354 3700, Fax: (66) 2354 3692





## **UNCERTAINTY OF MEASUREMENT**

The stated uncertainty is the expanded uncertainty obtained by multiplying the standard uncertainty by the coverage factor  $k=2$ . It has been determined in accordance with EA publication EA-4/02 M:2013 "Evaluation of the Uncertainty of Measurement in Calibration" and JCGM 100:2008 "Evaluation of measurement data --Guide to the Expression of Uncertainty in Measurement (GUM 1995 with minor corrections)". The value of the measured lies within the assigned range of value with a probability of 95 %.

Parameter	Uncertainty at SPL94 dB	Maximum-permitted uncertainty of measurement for a coverage probability of 95%
1.Sound Pressure level	0.08	0.15
2. Frequency	0.1	0.2
3. THD+N	0.1	0.5

## **TRACEABILITY**

This certificate provides traceability of measurement to recognized national standards, and to the realization of the International System of Units (SI).



## **ENVIRONMENTAL CONDITIONS**

Ambient condition in the laboratory are as follows :

Temperature	:	$(23.0 \pm 1.0)$	°C
Pressure	:	$(101.325 \pm 1.500)$	kPa
Relative Humidity	:	$(50.0 \pm 15.0)$	%

**Reference Condition** : 101.325 kPa , 23.0 °C and 50.0 %RH.

## **Calibration Condition**

Preconditionings : 16 hours at ambient conditions.

Measurement Conditions : The average values during measurement are  
 $(100.313 \pm 0.014)$  kPa,  $(22.0 \pm 0.3)$  °C and  $(57.0 \pm 2.1)$  %RH

## **MEASUREMENT METHOD**

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone. The insert voltage technique was employed and the measurement procedure was based on IEC 60942-2017.

## **Reference Microphone**

4180 serial no.1395446

## **TABULATION OF RESULTS**

The following tables give the calibration results and associated measurement uncertainties at 95% of confidence level. The calibration results of sound pressure level which quoted in dB with reference to 20 µPa are corrected to the values under the reference environmental conditions.

The calibration results exclude the calibrator pressure correction but include the microphone volume correction, which was obtained from the manufacturer instruction manual of the sound calibrator, at the level of 94 dB.



## MEASUREMENT RESULTS

### 1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)*	Deviated value <sup>[1]</sup> (dB)	Acceptance Limit (dB)
<b>Microphone 4180 Serial No.1395446</b>			
94	94.15	0.15	0.25

Note <sup>[1]</sup> : The deviated value is the absolute value of the difference between the measured value and the corresponding specified sound pressure level.

### 2. Frequency\*

Specified Frequency (Hz)	Measured value (Hz)	Deviated value <sup>[2]</sup> (%)	Acceptance Limit (%)
<b>At the sound pressure level of 94 dB</b>			
1000	1000.0	0.0	0.7

Note <sup>[2]</sup> : The deviated value is the absolute value of the difference in percent between the measured value and the corresponding specified frequency.



**3. Total distortion + Noise\***

**Microphone 4180 Serial No.1395446**

Measured value <sup>[3]</sup> (%)	Maximum total distortion + Noise (%)
<b>At the sound pressure level of 94 dB</b>	
0.2	2.5

Note <sup>[3]</sup>: The measured value is the total distortion, measured over the frequency range from 20 Hz to 20 kHz. The measured value must not exceed the maximum total distortion + noise appeared in the table.

End of Certificate of Calibration





## Certificate of Calibration

Certificate Number : SPR23010249-8

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,  
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222073

ID. Number : SLM-40

### Environmental Conditions

Ambient Temperature :  $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity :  $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 19 Jan 2023

Calibration Date : 23 Jan 2023

Recommend Due Date : 23 Jan 2024

Date of Issue : 24 Jan 2023

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :

Authorized Signatory



## Calibration Report

Certificate Number : SPR23010249-8

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

### Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



## Result of Calibration

Certificate No. : SPR23010249-8

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.2	94.2	0.2	0.2	0.15
114	114.1	114.1	0.1	0.1	0.15

### Note:

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -