

ภาคผนวกที่ 5

เอกสารสอบเทียบความถูกต้องของเครื่องมือ

- 5-1 เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศ
- 5-2 เอกสารสอบเทียบเครื่องมือตรวจวัดระดับเสียงโดยทั่วไป
- 5-3 เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพน้ำ



ภาคผนวกที่ 5-1

เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศ



PM-10 High Volume Sampler Calibration

SITE

Site: Blue
 Sampler: PM#1
 Recorder: Kimhan P.

Date: 02/05/2023
 Test: Supackak S.
 Approval: Nidda A.

CONDITIONS

Sea Level Pressure (hPa): 1009.0
 Temperature (deg C): 30.0
 Seasonal SL Press. (hPa): 1013.0
 Seasonal Temp. (deg C): 31.0

Corrected Pressure (mm Hg): 756.8
 Temperature (deg K): 303.0
 Corrected Seasonal (mm Hg): 759.8
 Seasonal Temp. (deg K): 304.0

CALIBRATION ORIFICE

Make: Tisch
 Model:
 Serial#: 1635

Slope: 1.26614
 Intercept: -0.02116
 Date Certified: 1 Aug 22


TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	<u>12.40</u>	<u>1.185</u>	<u>34.0</u>	<u>21.51</u>
2	<u>10.00</u>	<u>1.062</u>	<u>30.0</u>	<u>18.98</u>
3	<u>7.40</u>	<u>0.937</u>	<u>26.0</u>	<u>16.45</u>
4	<u>4.80</u>	<u>0.760</u>	<u>22.0</u>	<u>13.92</u>
5	<u>3.00</u>	<u>0.593</u>	<u>18.0</u>	<u>11.39</u>

LINEAR REGRESSION

Slope (m) = 16.8932
 Intercept (b) = 1.1219
 Corr. coeff. (r) = 0.9964
 SFR = 1.131
 SSP = 31.96
 # of Observations: 5

Range of Chart 30
 at SFR $\pm 10\%$ 34

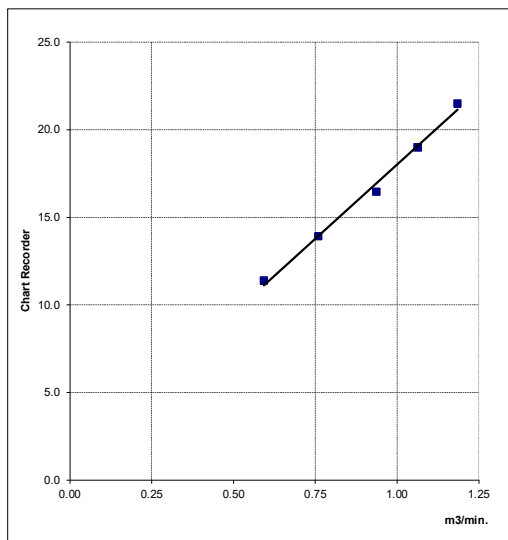

Calibrated by : _____

Approved by : _____

Nidda Anusawanchai
 02/05/2023

PM-10 High Volume Sampler Calibration

SITE

Site: Blue
 Sampler: PM#4
 Recorder: Kimhan P.

Date: 02/05/2023
 Test: Supackak S.
 Approval: Nidida A.

CONDITIONS

Sea Level Pressure (hPa): 1009.0
 Temperature (deg C): 30.0
 Seasonal SL Press. (hPa): 1013.0
 Seasonal Temp. (deg C): 31.0

Corrected Pressure (mm Hg): 756.8
 Temperature (deg K): 303.0
 Corrected Seasonal (mm Hg): 759.8
 Seasonal Temp. (deg K): 304.0

CALIBRATION ORIFICE


Make: Tisch
 Model:
 Serial#: 1635

Slope: 1.26614
 Intercept: -0.02116
 Date Certified: 1 Aug 22

TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	<u>11.00</u>	1.185	<u>42.0</u>	26.58	Slope (m)= 18.4703
2	<u>8.00</u>	1.062	<u>36.0</u>	22.78	Intercept (b)= 3.7403
3	<u>6.20</u>	0.937	<u>32.0</u>	20.25	Corr. coeff.(r)= 0.9863
4	<u>4.00</u>	0.760	<u>28.0</u>	17.72	SFR = 1.131
5	<u>2.40</u>	0.593	<u>24.0</u>	15.19	SSP = 38.92
					# of Observations: 5

Range of Chart 36
 at SFR $\pm 10\%$ 41

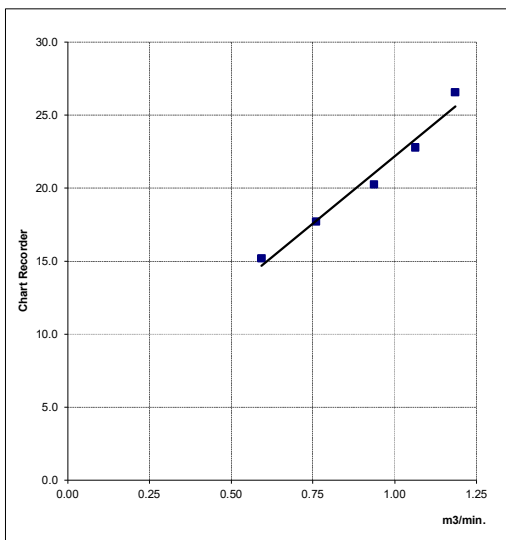

ผล Cal ไม่ผ่านเนื่องจากค่า Corr. coeff. น้อยกว่า 0.99

Calibrated by

Approved by

02/05/2023

PM-10 High Volume Sampler Calibration

SITE

Site: Blue
 Sampler: PM#5
 Recorder: Kimhan P.

Date: 02/05/2023
 Test: Supackak S.
 Approval: Nidda A.

CONDITIONS

Sea Level Pressure (hPa): 1009.0
 Temperature (deg C): 30.0
 Seasonal SL Press. (hPa): 1013.0
 Seasonal Temp. (deg C): 31.0

Corrected Pressure (mm Hg): 756.8
 Temperature (deg K): 303.0
 Corrected Seasonal (mm Hg): 759.8
 Seasonal Temp. (deg K): 304.0

CALIBRATION ORIFICE

Make: Tisch
 Model:
 Serial#: 1635


Slope: 1.26614
 Intercept: -0.02116
 Date Certified: 1 Aug 22

TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	<u>6.00</u>	<u>1.185</u>	<u>38.0</u>	<u>24.04</u>
2	<u>4.40</u>	<u>1.062</u>	<u>36.0</u>	<u>22.78</u>
3	<u>3.80</u>	<u>0.937</u>	<u>32.0</u>	<u>20.25</u>
4	<u>2.80</u>	<u>0.760</u>	<u>26.0</u>	<u>16.45</u>
5	<u>0.80</u>	<u>0.593</u>	<u>22.0</u>	<u>13.92</u>

LINEAR
REGRESSION
 Slope (m)= 17.9416
 Intercept (b)= 3.2077
 Corr. coeff.(r)= 0.9955
 SFR = 1.131
 SSP = 37.13
 # of Observations: 5

Range of Chart 35
 at SFR $\pm 10\%$ 39

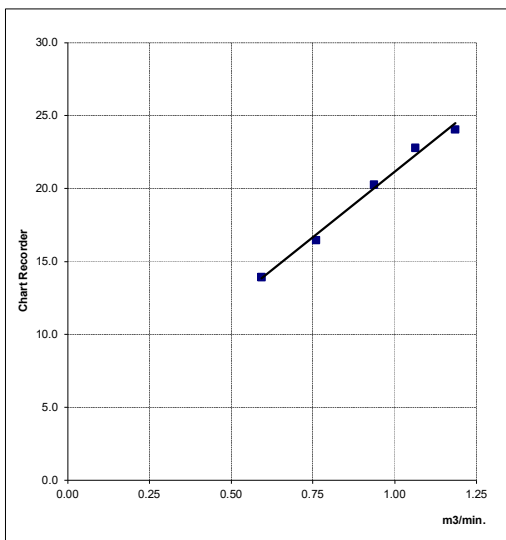

Calibrated by :

Approved by :

02/05/2023

PM-10 High Volume Sampler Calibration

SITE

Site: Blue
 Sampler: PM#8
 Recorder: Kimhan P.

Date: 02/05/2023
 Test: Supackak S.
 Approval: Nidida A.

CONDITIONS

Sea Level Pressure (hPa): 1009.0
 Temperature (deg C): 30.0
 Seasonal SL Press. (hPa): 1013.0
 Seasonal Temp. (deg C): 31.0

Corrected Pressure (mm Hg): 756.8
 Temperature (deg K): 303.0
 Corrected Seasonal (mm Hg): 759.8
 Seasonal Temp. (deg K): 304.0

CALIBRATION ORIFICE


Make: Tisch
 Model:
 Serial#: 1635

Slope: 1.26614
 Intercept: -0.02116
 Date Certified: 1 Aug 22

TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	<u>3.60</u>	<u>1.185</u>	<u>34.0</u>	<u>21.51</u>	Slope (m)= <u>14.4358</u>
2	<u>2.80</u>	<u>1.062</u>	<u>30.0</u>	<u>18.98</u>	Intercept (b)= <u>4.1111</u>
3	<u>2.00</u>	<u>0.937</u>	<u>28.0</u>	<u>17.72</u>	Corr. coeff.(r)= <u>0.9966</u>
4	<u>1.40</u>	<u>0.760</u>	<u>24.0</u>	<u>15.19</u>	SFR = <u>1.131</u>
5	<u>1.00</u>	<u>0.593</u>	<u>20.0</u>	<u>12.65</u>	SSP = <u>32.29</u>
					# of Observations: <u>5</u>

Range of Chart 31
 at SFR $\pm 10\%$ 34

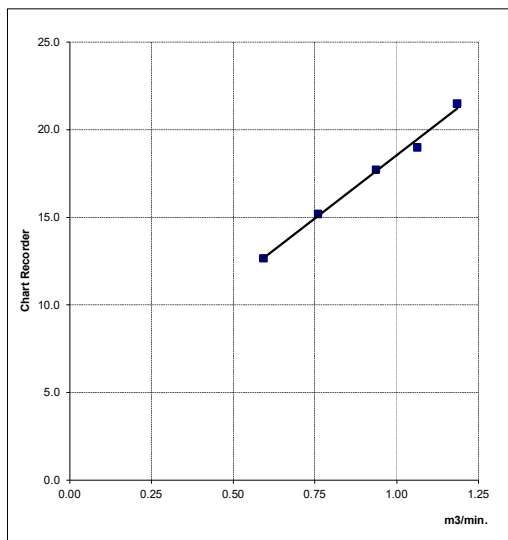

Calibrated by :

Approved by :

02/05/2023

PM-10 High Volume Sampler Calibration

SITE

Site: Blue
 Sampler: PM#10
 Recorder: Kimhan P.

Date: 02/05/2023
 Test: Supackak S.
 Approval: Nidida A.

CONDITIONS

Sea Level Pressure (hPa): 1009.0
 Temperature (deg C): 30.0
 Seasonal SL Press. (hPa): 1013.0
 Seasonal Temp. (deg C): 31.0

Corrected Pressure (mm Hg): 756.8
 Temperature (deg K): 303.0
 Corrected Seasonal (mm Hg): 759.8
 Seasonal Temp. (deg K): 304.0

CALIBRATION ORIFICE

Make: Tisch
 Model:
 Serial#: 1635

Slope: 1.26614
 Intercept: -0.02116
 Date Certified: 1 Aug 22


TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	<u>11.00</u>	1.185	<u>56.0</u>	35.43
2	<u>9.00</u>	1.062	<u>50.0</u>	31.64
3	<u>7.00</u>	0.937	<u>44.0</u>	27.84
4	<u>4.60</u>	0.760	<u>38.0</u>	24.04
5	<u>2.80</u>	0.593	<u>30.0</u>	18.98

LINEAR REGRESSION

Slope (m) = 27.1264
 Intercept (b) = 2.9722
 Corr. coeff. (r) = 0.9980
 SFR = 1.131
 SSP = 53.17
 # of Observations: 5

Range of Chart 49
 at SFR $\pm 10\%$ 57

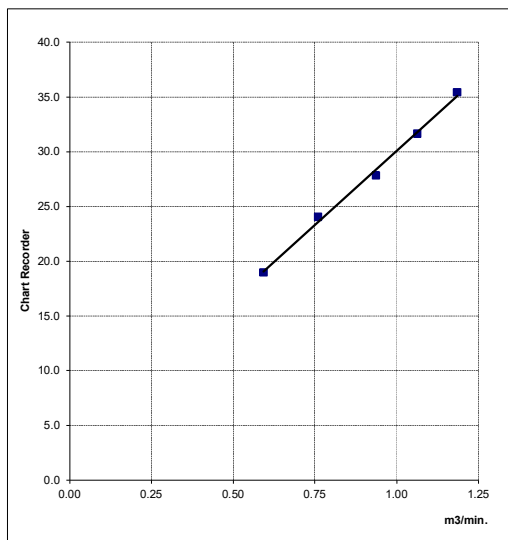

Calibrated by : _____

Approved by : _____

02/05/2023

PM-10 High Volume Sampler Calibration

SITE

Site: Blue
 Sampler: PM#12
 Recorder: Kimhan P.

Date: 02/05/2023
 Test: Supackak S.
 Approval: Nidida A.

CONDITIONS

Sea Level Pressure (hPa): 1009.0
 Temperature (deg C): 30.0
 Seasonal SL Press. (hPa): 1013.0
 Seasonal Temp. (deg C): 31.0

Corrected Pressure (mm Hg): 756.8
 Temperature (deg K): 303.0
 Corrected Seasonal (mm Hg): 759.8
 Seasonal Temp. (deg K): 304.0

CALIBRATION ORIFICE

Make: Tisch
 Model:
 Serial#: 1635


Slope: 1.26614
 Intercept: -0.02116
 Date Certified: 1 Aug 22

TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	<u>11.20</u>	1.185	<u>48.0</u>	30.37
2	<u>8.80</u>	1.062	<u>42.0</u>	26.58
3	<u>7.00</u>	0.937	<u>38.0</u>	24.04
4	<u>4.40</u>	0.760	<u>32.0</u>	20.25
5	<u>2.80</u>	0.593	<u>24.0</u>	15.19

LINEAR
REGRESSION
 Slope (m)= 24.6690
 Intercept (b)= 0.8995
 Corr. coeff. (r)= 0.9970
 SFR = 1.131
 SSP = 45.51
 # of Observations: 5

Range of Chart 42
 at SFR $\pm 10\%$ 49

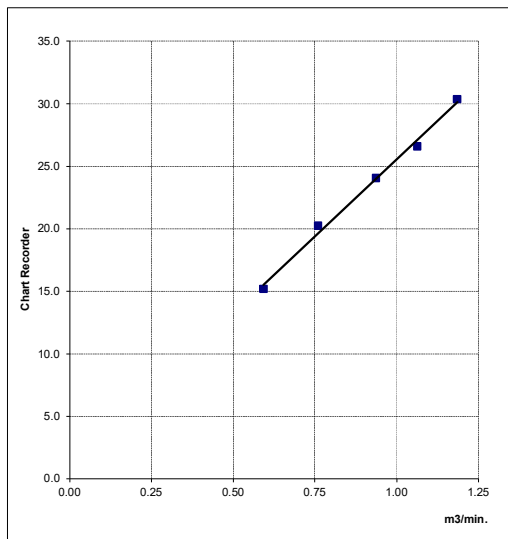

Calibrated by : _____

Approved by : _____

02/05/2023



ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพมหานคร 10140

เลขประจำตัวผู้เสียภาษี 0103546024094 (สำนักงานใหญ่)

Tel: 02-8736045-6 Email: blueconsultant2546@gmail.com

PM-10 High Volume Sampler Calibration

SITE

Site: Blue
Sampler: PM#14
Recorder: Kimhan P.

Date: 02/05/2023
Test: Supackak S.
Approval: Nidda A.

CONDITIONS

Sea Level Pressure (hPa): 1009.0
Temperature (deg C): 30.0
Seasonal SL Press. (hPa): 1013.0
Seasonal Temp. (deg C): 31.0

Corrected Pressure (mm Hg): 756.8
Temperature (deg K): 303.0
Corrected Seasonal (mm Hg): 759.8
Seasonal Temp. (deg K): 304.0

CALIBRATION ORIFICE

Make: Tisch
Model:
Serial#: 1635

Slope: 1.26614
Intercept: -0.02116
Date Certified: 1 Aug 22


TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	<u>11.80</u>	1.185	<u>54.0</u>	34.17
2	<u>9.80</u>	1.062	<u>48.0</u>	30.37
3	<u>7.60</u>	0.937	<u>42.0</u>	26.58
4	<u>5.00</u>	0.760	<u>34.0</u>	21.51
5	<u>3.20</u>	0.593	<u>26.0</u>	16.45

LINEAR REGRESSION

Slope (m) = 29.7519
Intercept (b) = -1.1819
Corr. coeff. (r) = 0.9999
SFR = 1.131
SSP = 51.30
of Observations: 5

Range of Chart 47
at SFR $\pm 10\%$ 56

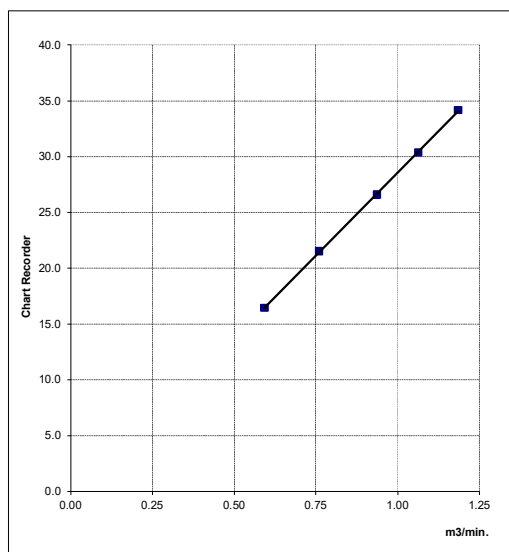

Calibrated by : _____

Approved by : _____

02/05/2023

PM-10 High Volume Sampler Calibration

SITE

Site: Blue
 Sampler: PM#15
 Recorder: Kimhan P.

Date: 02/05/2023
 Test: Supackak S.
 Approval: Nidda A.

CONDITIONS

Sea Level Pressure (hPa): 1009.0
 Temperature (deg C): 30.0
 Seasonal SL Press. (hPa): 1013.0
 Seasonal Temp. (deg C): 31.0

Corrected Pressure (mm Hg): 756.8
 Temperature (deg K): 303.0
 Corrected Seasonal (mm Hg): 759.8
 Seasonal Temp. (deg K): 304.0

CALIBRATION ORIFICE

Make: Tisch
 Model:
 Serial#: 1635


Slope: 1.26614
 Intercept: -0.02116
 Date Certified: 1 Aug 22

TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	<u>10.60</u>	1.185	<u>62.0</u>	39.23
2	<u>9.20</u>	1.062	<u>56.0</u>	35.43
3	<u>7.20</u>	0.937	<u>50.0</u>	31.64
4	<u>4.60</u>	0.760	<u>40.0</u>	25.31
5	<u>2.80</u>	0.593	<u>34.0</u>	21.51

LINEAR
REGRESSION
 Slope (m)= 30.5908
 Intercept (b)= 2.8656
 Corr. coeff. (r)= 0.9978
 SFR = 1.131
 SSP = 59.20
 # of Observations: 5

Range of Chart 55
 at SFR $\pm 10\%$ 64

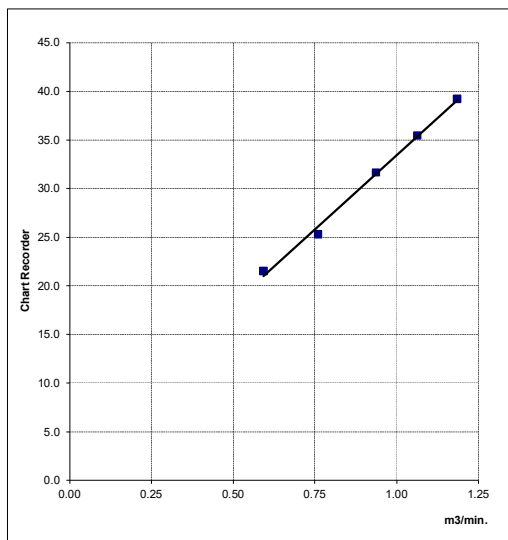

Calibrated by : _____

Approved by : _____

02/05/2023



ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพมหานคร 10140

เลขประจำตัวผู้เสียภาษี 0103546024094 (สำนักงานใหญ่)

Tel: 02-8736045-6 Email: blueconsultant2546@gmail.com

PM-10 High Volume Sampler Calibration

SITE

Site: Blue
Sampler: PM#16
Recorder: Kimhan P.

Date: 02/05/2023
Test: Supackak S.
Approval: Nidida A.

CONDITIONS

Sea Level Pressure (hPa): 1009.0
Temperature (deg C): 30.0
Seasonal SL Press. (hPa): 1013.0
Seasonal Temp. (deg C): 31.0

Corrected Pressure (mm Hg): 756.8
Temperature (deg K): 303.0
Corrected Seasonal (mm Hg): 759.8
Seasonal Temp. (deg K): 304.0

CALIBRATION ORIFICE

Make: Tisch
Model:
Serial#: 1635

Slope: 1.26614
Intercept: -0.02116
Date Certified: 1 Aug 22


TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	<u>8.20</u>	<u>1.185</u>	<u>50.0</u>	<u>31.64</u>
2	<u>6.60</u>	<u>1.062</u>	<u>48.0</u>	<u>30.37</u>
3	<u>5.00</u>	<u>0.937</u>	<u>44.0</u>	<u>27.84</u>
4	<u>3.20</u>	<u>0.760</u>	<u>40.0</u>	<u>25.31</u>
5	<u>1.80</u>	<u>0.593</u>	<u>36.0</u>	<u>22.78</u>

LINEAR REGRESSION

Slope (m) = 15.3161
Intercept (b) = 13.6893
Corr. coeff. (r) = 0.9976
SFR = 1.131
SSP = 49.01
of Observations: 5

Range of Chart 47
at SFR $\pm 10\%$ 51

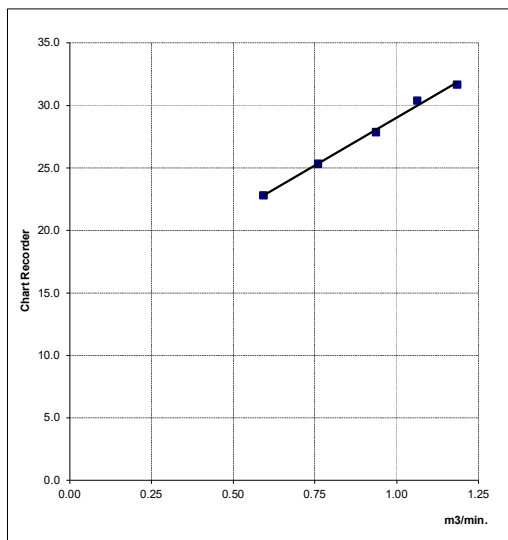

Calibrated by :

Approved by :

02/05/2023

PM-10 High Volume Sampler Calibration

SITE

Site: Blue
 Sampler: PM#17
 Recorder: Kimhan P.

Date: 02/05/2023
 Test: Supackak S.
 Approval: Nidda A.

CONDITIONS

Sea Level Pressure (hPa): 1009.0
 Temperature (deg C): 30.0
 Seasonal SL Press. (hPa): 1013.0
 Seasonal Temp. (deg C): 31.0

Corrected Pressure (mm Hg): 756.8
 Temperature (deg K): 303.0
 Corrected Seasonal (mm Hg): 759.8
 Seasonal Temp. (deg K): 304.0

CALIBRATION ORIFICE

Make: Tisch
 Model:
 Serial#: 1635

Slope: 1.26614
 Intercept: -0.02116
 Date Certified: 1 Aug 22


TEST

Plate or Test #	H2O (in)	Qa (m3/min)	I (chart)	IC (corrected)
1	<u>12.60</u>	1.185	<u>50.0</u>	31.64
2	<u>10.00</u>	1.062	<u>44.0</u>	27.84
3	<u>7.60</u>	0.937	<u>40.0</u>	25.31
4	<u>4.80</u>	0.760	<u>32.0</u>	20.25
5	<u>3.00</u>	0.593	<u>26.0</u>	16.45

LINEAR REGRESSION

Slope (m) = 25.5079
 Intercept (b) = 1.1506
 Corr. coeff. (r) = 0.9986
 SFR = 1.131
 SSP = 47.40
 # of Observations: 5

Range of Chart 44
 at SFR $\pm 10\%$ 51

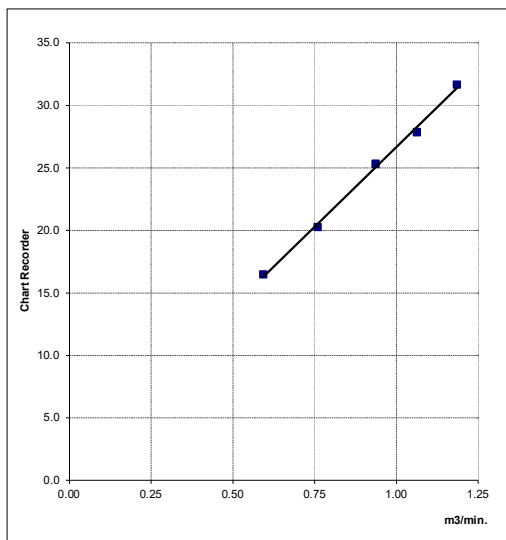

Calibrated by :

Approved by :

02/05/2023

Certificate of Calibration

Calibration Certification Information

Cal. Date: November 28, 2022 Rootsmeter S/N: 438320 Ta: 294 °K
Operator: Jim Tisch Pa: 748.8 mm Hg
Calibration Model #: TE-5025A Calibrator S/N: 1290

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.3960	3.2	2.00
2	3	4	1	0.9800	6.4	4.00
3	5	6	1	0.8770	8.0	5.00
4	7	8	1	0.8370	8.8	5.50
5	9	10	1	0.6930	12.8	8.00

Data Tabulation

Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9944	0.7123	1.4133	0.9957	0.7133	0.8862
0.9901	1.0103	1.9987	0.9915	1.0117	1.2532
0.9880	1.1266	2.2346	0.9893	1.1281	1.4011
0.9869	1.1791	2.3436	0.9882	1.1807	1.4695
0.9816	1.4164	2.8265	0.9829	1.4183	1.7723
QSTD	m=	2.00726	QA	m=	1.25691
	b=	-0.02247		b=	-0.01409
	r=	0.99994		r=	0.99994

Calculations

Vstd= $\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$	Va= $\Delta Vol((Pa-\Delta P)/Pa)$
Qstd= $Vstd/\Delta Time$	Qa= $Va/\Delta Time$
For subsequent flow rate calculations:	
Qstd= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$	Qa= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$

Standard Conditions

Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH: calibrator manometer reading (in H2O)	
ΔP: rootsmeter manometer reading (mm Hg)	
Ta: actual absolute temperature (°K)	
Pa: actual barometric pressure (mm Hg)	
b: intercept	
m: slope	

RECALIBRATION

US EPA recommends annual recalibration per 1998
40 Code of Federal Regulations Part 50 to 51,
Appendix B to Part 50, Reference Method for the
Determination of Suspended Particulate Matter in
the Atmosphere, 9.2.17, page 30

Certificate of Calibration

Certificate No. : 65-400665-1

Page : 1 of 2

Submitted by : TNP Environment Co., Ltd.

332/173 Moo 3 Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

Equipment : Air Chamber (Oven)

Manufacturer : Memmert

Model : UF75

Range : N/A °C

Resolution : 0.1 °C

Serial No. : B320.0251

ID No. : N/A

Environment : On site calibration was carried out at the Laboratory, TNP Environment Co., Ltd.

Ambient Temperature : (27.0 to 28.0 °C

Relative Humidity : (40 to 45) %

Line Voltage : (228.0 to 230.0) V

Date of Received : 26 December 2022

Date of Calibration : 26 December 2022

Date of Issue : 28 December 2022

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20


The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400030	65-400548-1	26 Apr 2023	National Institute of Metrology Thailand (NIMT)

Approved by



Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-400665-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

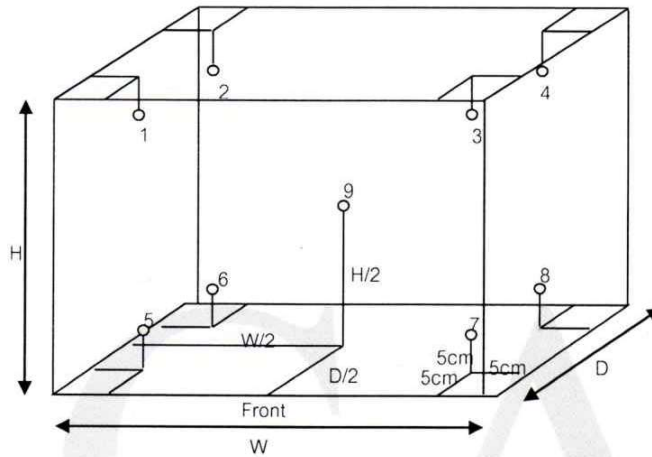

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.56 m

Capacity = 0.07 m³

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty (± ° C)
			1	2	3	4	5	6	7	8	9	
104.0	104.0	104.0	104.2	104.1	104.2	104.0	103.8	103.9	103.9	103.9	104.0	0.69
180.0	180.0	180.0	179.6	179.6	179.7	179.8	180.2	179.5	179.0	179.8	180.5	1.0

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Uniformity (° C)	Measured Stability (° C)	Overall Variation (° C)
104.0	104.0	104.0	0.4	0.1	0.7
180.0	180.0	180.0	1.7	0.3	2.0

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 22H1779

Page : 1 of 2

Equipment : Digital Thermo-Hygrometer

Manufacturer: Exttech

Model : 448514

Serial No.: PONPE 5816745

ID No.: TNP.LAB.04

Condition As-Received: Used Item

Received Date: 24 August 2022

Calibration Date: 27 August 2022

Reference: 2208-0843WN

Submitted by: TNP ENVIRONMENT CO.,LTD

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

332/173 Moo 3, Bang Rak Phatthana, Bang Bua Thong,
Nonthaburi 11110

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard Chilled Mirror Hygrometer Sensor	Dew Prime II	31863	19714	17 Sep 2022
2) Standard Humidity/Temperature Meter	400	10240757	TH-0125-21	13 Dec 2022


2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained at:-

- National Institute of Standards and Technology (NIST) , The United States of America
- National Institute of Metrology Thailand (NIMT)

Calibrated by : Somchai Dumwor
Issue Date : 30 August 2022

Approved Signatory :

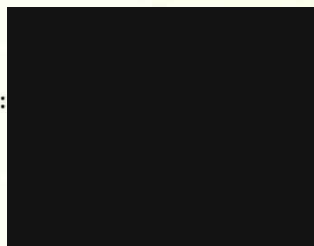

B 0295353



Cert. No.: 22H1779

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Humidity measurement.

<u>Reference</u> <u>Temperature</u> (°C)	<u>Standard</u> <u>Humidity</u> (%R.H.)	<u>UUC*</u> <u>Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty</u> <u>of Measurement</u> (±%R.H.)
25.0	50.1	47	-3.1	1.6

Result of Calibration:-

Without Adjustment

Function:


Temperature measurement for indoor sensor.

<u>Standard</u> <u>Temperature</u> (°C)	<u>UUC*</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> <u>of Measurement</u> (±°C)
20.02	20.1	0.08	0.42
25.03	25.4	0.37	0.42

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-o0o-



a 1123737



MCL
Microtech Calibration laboratory



53/154 Moo 2, Semafahkarm Road, Tumbon Khukhot, Amphur Lamlukka, Pathumthani 12130

53/154 หมู่ 2 ถนนเสมาฟ้าคราม ตำบลกุศต อำเภอลำลูกกา จังหวัดปทุมธานี 12130

Tel. 02-9877200 Fax. 02-9877205

Certificate No. : M22 - 1588A

Page : 1 of 4

Certificate of Calibration

Customer : TNP ENVIRONMENT CO.,LTD.
Address : 332/173 Moo 3 Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11111

Description of Equipment : Electronic Balance
Manufacturer : Shimadzu
Model : AP225WD
Serial Number : D316301848
ID. / Control Number : TNP.LAB.30
Made In : Philippines
Location : On - Site
Environmental Conditions : Temperature (25 +/- 10) °C
Humidity (50 +/- 25) % RH
Atmospheric Pressure (1010 +/- 10) mbar

Calibration Date : APR 18, 2022
Issue Date : APR 20, 2022

Uncertainty of Measurement

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Expression of the Uncertainty of Measurement in Calibration (M3003)" which provides a level of confidence approximately 95%.

Calibrated by : Sarawut Khrueapan

Approved by :

Laboratory Manager

Certificate of Calibration

Description : Electronic Balance **Serial Number** : D316301848 **Resolution** : 0.0001,0.00001 g
Manufacturer : Shimadzu **ID. /Control Number** : TNP.LAB.30 **Order No.** : 1398 - 22
Model : AP225WD **Made In** : Philippines **Received Date** : APR 18, 2022
Unit : g **Capacity** : 220 g **Calibration Date** : APR 18, 2022

Result of Calibration : Without Adjustment **Resolution** : 0.0001,0.00001 g

Range : 200 g

2. Departure From Nominal Value

Nominal Value g	UUC* Reading g	UUC* Error g	Uncertainty of Measurement +/- g
0	0.00000	0.00000	0.00013
0.1	0.10003	0.00003	0.00013
0.2	0.20002	0.00002	0.00022
0.5	0.50002	0.00002	0.00043
1	1.00002	0.00002	0.00043
2	2.00005	0.00005	0.00043
5	5.00007	0.00007	0.00068
10	10.00006	0.00006	0.00068
20	20.00003	0.00003	0.00068
50	49.99997	-0.00003	0.00068
100	99.99999	-0.00001	0.00068
200	199.9999	-0.0001	0.00068

UUC* = Unit Under Calibration

Certificate of Calibration

Description : Electronic Balance **Serial Number** : D316301848 **Resolution** :
Manufacturer : Shimadzu **ID. /Control Number** : TNP.LAB.30 **Order No.** : 1398 - 22
Model : AP225WD **Made In** : Philippines **Received Date** : APR 18, 2022
Unit : g **Capacity** : 220 g **Calibration Date** : APR 18, 2022

Result of Calibration : Without Adjustment **Resolution** : 0.0001,0.00001 g

Range : 200 g

3. Effect of Center Loading



Nominal Load g	UUC* Reading					Maximum Difference g
	A g	B g	C g	D g	E g	
50	49.99997	49.99997	49.99995	49.99996	49.99996	0.00002

A Mass of 50 g Was Placed to Various Position on The Pan.

The Weighing Machine Reading Error Obtained Is Given In Table

4. Effect Tare Function

Nominal Tare Weight g	Standard Weight g		UUC* Reading g	UUC* Error g
	Tare		0.00000	0.00000
100	at 20 %	20.0000	20.0001	0.0001
	at 100 %	100.0000	100.0002	0.0002

UUC* = Unit Under Calibration

..... END.....

Certificate of Calibration

Description :	Electronic Balance	Serial Number :	D316301848	Resolution :	0.0001,0.00001 g
Manufacturer :	Shimadzu	ID. /Control Number :	TNP.LAB.30	Order No. :	1398 - 22
Model :	AP225WD	Made In :	Philippines	Received Date :	APR 18, 2022
Unit :	g	Capacity :	220 g	Calibration Date :	APR 18, 2022

Calibration Method

The Electronic balance was measured using standard weight following to in house calibration method MCL-CP14 and based on UKAS LAB 14: Edition 5 July 2015

This result was found accurate as shown on date and place of calibration only.

Reference Standard

Description	Model	Serial No.	Certificate No.	Due Date
Standard Weight Set	50 mg - 2 kg	N/A	B0-0805057/20	MAY 09, 2021

Traceability of Measurement

The measurements are traceable to international system of units (SI)

The certificate is traceable to through Thai Heart Calibration Co.,Ltd.

Range : 200 g

Resolution : 0.0001,0.00001 g

1. Repeatability of Balance

Nominal Value g	Standard Deviation of Reading g
0	0.00000
200	0.0000



Certificate of Calibration

Certificate Number : SPR22110273-1

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Electronic Balance

Manufacturer : N/A

Model : 20002

Serial Number : 4181

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$

Received Date : 15 Nov 2022

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 17 Nov 2022

Location of Calibration : In-Lab

Recommend Due Date : 17 Nov 2023

Calibration Procedure : SP-CPM-04-01

Date of Issue : 18 Nov 2022

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Navaporn Uengseng

Approved by :

Calibration Officer

Authorized Signatory



Calibration Report

Certificate Number : SPR22110273-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Standard Weight Set	N/A	SS6K3324-16	SPR21120375-3	06 Jan 2023

Traceability

This certification is traceable to the International System of Unit maintained at :
SP Metrology - SP Metrology system (Thailand) Co.Ltd.



Result of Calibration

Certificate No. : SPR22110273-1

Page : 3 of 3

Range capacity : 0 to 2000 g

Resolution: 0.01 g

Repeatability (n = 10 number of measurement)

Standard Weight (g)	Standard Deviation
2000	0.000

Departure of indication from nominal Value


Unit : g

Nominal Value	UUC Reading	Error	Uncertainty (±)
No Load	0.00	0.00	0.0058
200.0	200.00	0.00	0.0058
400.0	400.00	0.00	0.0058
600.0	600.00	0.00	0.0058
800.0	800.00	0.00	0.0059
1000.0	1000.00	0.00	0.0061
1200.0	1200.00	0.00	0.0062
1400.0	1400.00	0.00	0.0063
1600.0	1600.00	0.00	0.0065
1800.0	1800.00	0.00	0.0066
2000.0	2000.00	0.00	0.0065

Off – Center Loading

A mass of 500 g was placed to various positions on the pan. The weighing machine reading error obtained is given in table.

Center	500.00 g
Front	500.00 g
Back	500.00 g
Left	500.00 g
Right	500.00 g
Maximum difference	0.00 g



Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%

– End of Certificate –

SP-FM-04-15 REV.0

ผู้จัดการห้องปฏิบัติการ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 17 May, 2022

Certification No. 181/22

Page : 1 of 6

Object : Precision Weather Station

Manufacturer : Davis Instruments

Type : Vantage Pro 2 Model No. : 6152C

Mfg Code : Display BE190314017 Transmitter BE190314017

Customer : Blue Consultant Limited Partnership.
32/751 Thanon Pracha Uthit, Thung Khru,
Thung Khru, Bangkok 10140.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1010.5 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: Thermoschneider No.9188 : testo, testo 645 Serial No. 02848057

Type PTB220 No. V1220015

(Authorised Signatory)

for the Chief

Sub-Standard Instrument

Mechanical Engineer



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 181/22

17 May, 2022

Page : 2 of 6

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacuum inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.9	0.10
7.00	-	-	-	6.7	0.30
9.02	-	-	-	8.9	0.12
11.01	-	-	-	10.7	0.31
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.8	0.21
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.3	0.72

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibration

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 0-2396-0156,0-2399-0469

The Result of Calibration

Certification No. 181/22

17 May, 2022

Page : 3 of 6

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
756.11	756.4	-0.29
756.26	756.6	-0.34
755.92	756.2	-0.28
753.01	753.3	-0.29
752.57	752.8	-0.23
752.92	753.2	-0.28
753.26	753.5	-0.24
753.92	754.2	-0.28
754.33	754.6	-0.27
754.98	755.3	-0.32
755.51	755.9	-0.39
753.83	754.1	-0.27
754.25	754.6	-0.35
755.29	755.6	-0.31
756.27	756.5	-0.23
756.59	756.9	-0.31
756.87	757.1	-0.23
756.23	756.5	-0.27
755.63	755.9	-0.27
754.89	755.1	-0.21

Average

Cali



Mechanical Engineer



Calibration & Test Section
Meteorological Instruments Bureau



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration


Certification No. 181/22

17 May, 2022

Page : 4 of 6

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.2	45.4	-0.2
30.4	30.5	-0.1
15.2	15.3	-0.1

Calibra



Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration


Certification No. 181/22

17 May, 2022

Page : 5 of 6

Standard Humidity % R.H.	Relative Humidity Sensor Reading	
	Reading	Correction
	% R.H.	% R.H.
82.40	79	3.40
61.62	59	2.62
45.32	44	1.32

Calibr

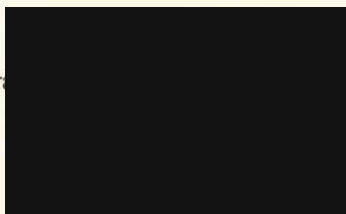

Mechanical Engineer





Date of Issue 17 May, 2022

Certification No. 181/22

Page : 6 of 6

ใบรับรอง

หนังสือฉบับนี้ขอรับรองว่า เครื่องวัดฝน ยี่ห้อ Davis Instruments แบบ TIPPING
BUCKET Product No. 6152 CUK Mfg. Code. A111101P020 ทำการสอบเทียบกับ
แก้วฝนแบบแก้วดวง GAUGE DIAMETER 8.0 INCHES , NEGRETTI & ZAMBRA
LONDON No 71082 และสามารถนำไปใช้ได้ มีค่าถูกต้องตามรายละเอียดของ
เครื่องมือ (0.2 mm/ TIP)



วิศวกรชำนาญการ

ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ Blue Consultant Limited Partnership

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกซเรย์ไอออนธาตุลงวันที่ 14 สิงหาคม 2563

CALIBRATION REPORT

Equipment : CO Analyzer

Brand/Model: API/300,API/300EU,Thermo/48C,
Teledyne-API/T300, Horiba/APMA-370

Serial No.: 139, 1069, 1119, 131, 678, 3445,
48C-62630-336, 48C-74104-375,
UT0THDS3

Date of Calibrate : May 2, 2023

Reference Standard

Cylinder No.: EB0128767

Certification Date: October 29, 2019

Expiry Date: October 29, 2027

Component: SO2: 55.62 ppm , NO: 57.21 ppm , CO : 4,551 ppm

Calibration Check (Before adjust)

Serial No.	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)
1069	0.4	0	0.4	39.5	40	-0.5
1119	0.2	0	0.2	39.8	40	-0.2
139	-0.1	0	-0.1	39.2	40	-0.8
131	0.2	0	0.2	39.1	40	-0.9
678	0.2	0	0.2	39.5	40	-0.5
3445	0.3	0	0.3	40.2	40	0.2
48C-62630-336	0.2	0	0.2	39.8	40	-0.2
48C-74104-375	0.2	0	0.2	39.7	40	-0.3
UT0THDS3	0.1	0	0.1	40.4	40	0.4

Calibration Check (After adjust)

Serial No.	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)
1069	0	0	0	40	40	0
1119	0	0	0	40	40	0
139	0	0	0	40	40	0
131	0	0	0	40	40	0
678	0	0	0	40	40	0
3445	0	0	0	40	40	0
48C-62630-336	0	0	0	40	40	0
48C-74104-375	0	0	0	40	40	0
UT0THDS3	0	0	0	40	40	0

ผู้จัดการห้องปฏิบัติการ

ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ **Blue Consultant Limited Partnership**

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกซนใบอนุญาตลงวันที่ 14 สิงหาคม 2563

CALIBRATION REPORT

Equipment : NOx Analyzer

Serial No. : 374

Brand/Model: Teledyne-API/T200

Date of Calibrate : May 17, 2023

Reference Standard


Certification Date: October 29, 2019

Component: SO2: 55.62 ppm , NO: 57.21 ppm , CO : 4,551 ppm

Cylinder No.: EB0128767

Expiry Date: October 29, 2027

Calibration Check (Before adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx
374	4.3/1.8/6.1	0/0/0	4.3/1.8/6.1	398.5/4.0/402.5	400/0/400	-1.5/4.0/2.5
Calibration Check (After adjust)						
Serial No.	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)
	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx	NO/NO2/NOx
374	0/0/0	0/0/0	0/0/0	400/0/400	400/0/400	0/0/0

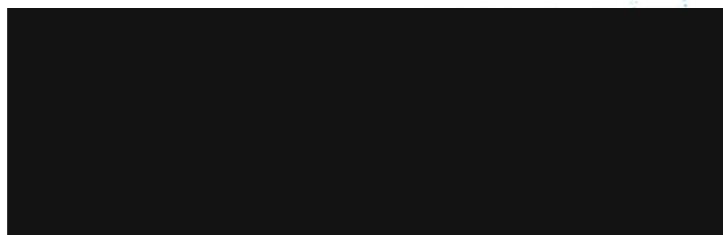

ผู้จัดการห้องปฏิบัติการ

ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ Blue Consultant Limited Partnership

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกซเรย์อนุญาตลงวันที่ 14 สิงหาคม 2563

CALIBRATION REPORT

Equipment : CO Analyzer
Serial No.: 678

Brand/Model: Teledyne-API/T300
Date of Calibrate : May 17, 2023

Reference Standard


Certification Date: October 29, 2019

Component: SO₂: 55.62 ppm , NO: 57.21 ppm , CO : 4,551 ppm

Cylinder No.: EB0128767

Expiry Date: October 29, 2027

Calibration Check (Before adjust)						
Serial No.	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)
678	0.3	0	0.3	40.2	40	0.2
Calibration Check (After adjust)						
Serial No.	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)
678	0	0	0	40	40	0



ผู้จัดการห้องปฏิบัติการ

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number:	E05NI99E15A0022	Reference Number:	160-401615775-1
Cylinder Number:	EB0128767	Cylinder Volume:	144.4 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2015 PSIG
PGVP Number:	A12019	Valve Outlet:	660
Gas Code:	CH ₄ ,CO,NO,NOX,SO ₂ ,BALN	Certification Date:	Oct 29, 2019

Expiration Date: Oct 29, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	55.00 PPM	57.21 PPM	G1	+/- 0.8% NIST Traceable	10/22/2019, 10/29/2019
NITRIC OXIDE	55.00 PPM	57.21 PPM	G1	+/- 0.8% NIST Traceable	10/22/2019, 10/29/2019
SULFUR DIOXIDE	55.00 PPM	55.62 PPM	G1	+/- 0.9% NIST Traceable	10/22/2019, 10/29/2019
METHANE	180.0 PPM	181.1 PPM	G1	+/- 0.9% NIST Traceable	10/22/2019
CARBON MONOXIDE	4500 PPM	4551 PPM	G1	+/- 0.6% NIST Traceable	10/22/2019
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	13010429	KAL004123	97.6 PPM NITRIC OXIDE/NITROGEN	+/- 0.8%	Jul 23, 2025
NTRM	13010429	KAL004123	97.6 PPM NOx/NITROGEN	+/- 0.8%	Jul 23, 2025
NTRM	16010235	KAL004419	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Dec 23, 2021
NTRM	08011503	K002564	246.7 PPM METHANE/AIR	+/- 0.6%	May 15, 2025
NTRM	072508	KAL004522	970.0 PPM CARBON MONOXIDE/NITROGEN	0.36%	May 14, 2021

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
MKS FTIR - CO - 000928781	FTIR	Sep 26, 2019
MKS FTIR CH4 000929060	FTIR	Scp 30, 2019
MKS FTIR - NO - 000928781	FTIR	Oct 18, 2019
MKS FTIR - NOx - 000928781	FTIR	Oct 18, 2019
MKS FTIR - SO2 - 000928781	FTIR	Oct 03, 2019

Triad Data Available Upon Request

NOTES:Gross Weight: 28.9 Kg, Net Weight: 4.7 Kg.





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 17 May, 2022

Certification No. 182/22

Page : 1 of 6

Object : Precision Weather Station

Manufacturer : Davis Instruments

Type : Vantage Pro 2 Model No. : 6152C

Mfg Code : Display BE190314019 Transmitter BE190314019

Customer : Blue Consultant Limited Partnership.
32/751 Thanon Pracha Uthit, Thung Khru,
Thung Khru, Bangkok 10140.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1006.7 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: Thermoschneider No.9188 : testo, testo 645 Serial No. 02678057

Type PTB220 No. V1220015

(Authorised Signatory)

for the Chief

Sub-Standard Instrument



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 182/22

17 May, 2022

Page : 2 of 6

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacumm inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.9	0.10
7.00	-	-	-	6.7	0.30
9.02	-	-	-	8.9	0.12
11.01	-	-	-	10.7	0.31
13.01	-	-	-	12.5	0.51
15.01	-	-	-	14.7	0.31
17.02	-	-	-	16.5	0.52
20.02	-	-	-	19.3	0.72

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibr

Mechanical Engineer





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 0-2396-0156,0-2399-0469

The Result of Calibration

Certification No. 182/22

17 May, 2022

Page : 3 of 6

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
756.11	755.9	0.21
756.26	756.0	0.26
755.92	755.7	0.22
753.01	752.7	0.31
752.57	752.3	0.27
752.92	752.6	0.32
753.26	753.0	0.26
753.92	753.6	0.32
754.33	754.0	0.33
754.98	754.8	0.18
755.51	755.2	0.31
753.83	753.6	0.23
754.25	753.9	0.35
755.29	755.0	0.29
756.27	756.0	0.27
756.59	756.3	0.29
756.87	756.6	0.27
756.23	756.0	0.23
755.63	755.4	0.23
754.89	754.6	0.29

Average

0.27

Calib

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration


Certification No. 182/22

17 May, 2022

Page : 4 of 6

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.2	45.4	-0.2
30.4	30.6	-0.2
15.2	15.3	-0.1

Calib

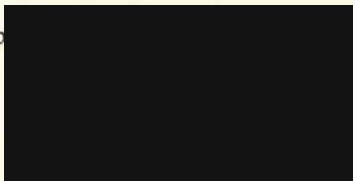

Mechanical Engineer





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration


Certification No. 182/22

17 May, 2022

Page : 5 of 6

Standard Humidity % R.H.	Relative Humidity Sensor Reading	
	Reading	Correction
	% R.H.	% R.H.
82.40	85	-2.60
61.62	63	-1.38
45.32	46	-0.68

Calib

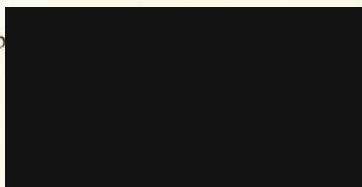

Mechanical Engineer






Date of Issue 17 May, 2022

Certification No. 182/22

Page : 6 of 6

ใบรับรอง

หนังสือฉบับนี้ขอรับรองว่า เครื่องวัดฝน ยี่ห้อ Davis Instruments แบบ TIPPING
BUCKET Product No. 6152 CUK Mfg No. A111101P016 ทำการสอบเทียบกับ
แก้วฝนแบบแก้วดวง GAUGE DIAMETER 8.0 INCHES, NEGRETTI & ZAMBRA
LONDON No 71082 และสามารถนำไปใช้ได้ มีค่าถูกต้องตามรายละเอียดของ
เครื่องมือ (0.2 mm./ TIP)

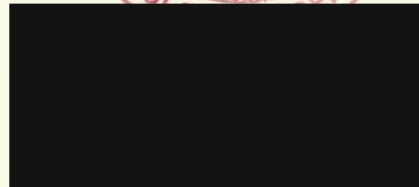

วิศวกรชำนาญการ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 4 March, 2022

Certification No. 087/22

Page : 1 of 6

Object : Precision Weather Station

Manufacturer : Davis Instruments

Type : Vantage Pro 2 Model No. : 6152C

Mfg Code : Display BE190314045 Transmitter BE190314045

Customer : Blue Consultant Limited Partnership.
32/751 Thanon Pracha Uthit, Thung Khru,
Thung Khru, Bangkok 10140.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1007.1 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: Thermoschneider No.9188 : testo, testo 645 Serial No. 302948057

Type PTB220 No. V1220015

(Authorised Signatory)

for the Chief

Sub-Standard Instrument



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Certification No. 087/22

4 March, 2022

Page : 2 of 6

Standard Ultrasonic Anemometer	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacumm	Velocity	Velocity	Correction
	m/sec	inches H2O	inches H2O	m/sec	m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.9	0.10
7.00	-	-	-	6.7	0.30
9.02	-	-	-	8.9	0.12
11.01	-	-	-	10.3	0.71
13.01	-	-	-	12.5	0.51
15.01	-	-	-	14.3	0.71
17.02	-	-	-	16.5	0.52
20.02	-	-	-	19.3	0.72

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibra

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 0-2396-0156, 0-2399-0469

The Result of Calibration

Certification No. 087/22

4 March, 2022

Page : 3 of 6


Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
754.87	755.9	-1.03
754.75	755.8	-1.05
754.27	755.3	-1.03
754.55	755.7	-1.15
754.74	755.9	-1.16
755.22	756.2	-0.98
755.49	756.4	-0.91
755.78	756.8	-1.02
755.99	757.0	-1.01
756.51	757.7	-1.19
756.05	757.1	-1.05
756.33	757.4	-1.07
756.47	757.6	-1.13
753.77	754.9	-1.13
754.03	755.1	-1.07
755.03	756.1	-1.07
755.25	756.4	-1.15
756.59	757.5	-0.91
755.74	756.8	-1.06
755.99	757.1	-1.11

Average

-1.06

Cal

Mechanical Engineer

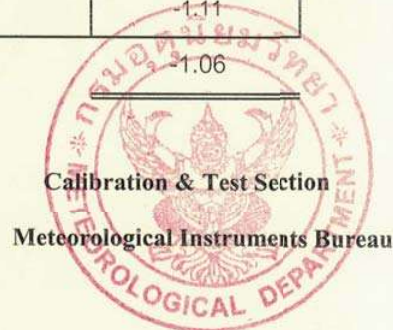



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 087/22

4 March, 2022

Page : 4 of 6

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.5	45.6	-0.1
30.2	30.2	0.0
15.4	15.3	0.1

Cali



Mechanical Engineer





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration


Certification No. 087/22

4 March, 2022

Page : 5 of 6

Standard Humidity % R.H.	Relative Humidity Sensor Reading	
	Reading	Correction
	% R.H.	% R.H.
83.02	85	-1.98
62.18	63	-0.82
43.27	42	1.27

Calibra

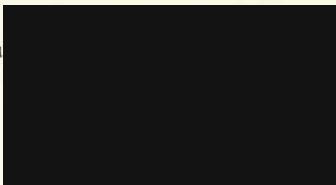

Mechanical Engineer





Date of Issue 4 March, 2022

Certification No. 087/22

Page : 6 of 6

ใบรับรอง

หนังสือฉบับนี้ขอรับรองว่า เครื่องวัดฝน ยี่ห้อ Davis Instruments แบบ TIPPING
BUCKET Product No. 6152 C Mfg. Code. BD190415078 ทำการสอบเทียบกับแก้ว
ฝนแบบแก้วดวง GAUGE DIAMETER 8.0 INCHES , NEGRETTI & ZAMBRA
LONDON No 71082 และสามารถนำไปใช้ได้ มีค่าถูกต้องตามรายละเอียดของ
เครื่องมือ (0.01 in / TIP)



วิศวกรชำนาญการ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 20 January, 2022

Certification No. 018/22

Page : 1 of 6

Object : Precision Weather Station

Manufacturer : Davis Instruments

Type : Vantage Pro 2 Model No. : 6152C

Mfg Code : Display BE190318028 Transmitter BE190318028

Customer : Blue Consultant Limited Partnership.
32/751 Thanon Pracha Uthit, Thung Khru,
Thung Khru, Bangkok 10140.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1011.3 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: Thermoschneider No.9188 : testo, testo 345 Serial No. 02648057

la Type PTB226 No. V1220015

(Authorised Signatory)

for the Chief

Sub-Standard Instrument



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 018/22

20 January, 2022

Page : 2 of 6

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H ₂ O	Vacumm inches H ₂ O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.4	0.60
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.5	0.50
7.00	-	-	-	6.7	0.30
9.02	-	-	-	8.5	0.52
11.01	-	-	-	10.7	0.31
13.01	-	-	-	12.5	0.51
15.01	-	-	-	14.8	0.21
17.02	-	-	-	16.5	0.52
20.02	-	-	-	19.3	0.72

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calib

Mechanical Engineer





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 0-2396-0156, 0-2399-0469

The Result of Calibration

Certification No. 018/22

20 January, 2022

Page : 3 of 6

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
760.50	761.3	-0.80
760.13	761.0	-0.87
760.67	761.5	-0.83
760.73	761.6	-0.87
757.28	758.1	-0.82
757.34	758.2	-0.86
757.52	758.4	-0.88
757.79	758.7	-0.91
758.10	759.0	-0.90
758.16	759.1	-0.94
758.66	759.5	-0.84
758.47	759.3	-0.83
758.56	759.4	-0.84
758.75	759.7	-0.95
758.98	759.9	-0.92
759.36	760.2	-0.84
756.54	757.4	-0.86
756.66	757.5	-0.84
757.00	757.9	-0.90
757.15	758.0	-0.85

Average

0.8

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469


The Result of Calibration

Certification No. 018/22

20 January, 2022

Page : 4 of 6

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.2	45.2	0.0
30.4	30.4	0.0
15.1	15.2	-0.1

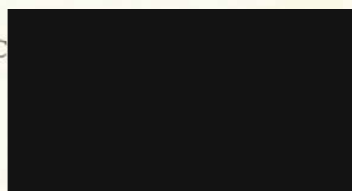

Mechanical Engineer





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration


Certification No. 018/22

20 January, 2022

Page : 5 of 6

Standard Humidity % R.H.	Relative Humidity Sensor Reading	
	Reading	Correction
	% R.H.	% R.H.
81.15	83	-1.85
60.23	64	-3.77
45.21	49	-3.79

Cali

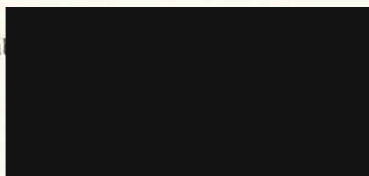

Mechanical Engineer






Date of Issue 20 January, 2022

Certification No. 018/22

Page : 6 of 6

ใบรับรอง

หนังสือฉบับนี้ขอรับรองว่า เครื่องวัดฝน ยี่ห้อ Davis Instruments แบบ TIPPING BUCKET Product No. 6152 C Mfg No. AM140127096 ทำการสอบเทียบกับแก้ว ฝนแบบแก้วตวง GAUGE DIAMETER 8.0 INCHES, NEGRETTI & ZAMBRA LONDON No 71082 และสามารถนำไปใช้ได้ มีค่าถูกต้องตามรายละเอียดของ เครื่องมือ (0.01 in/ TIP)

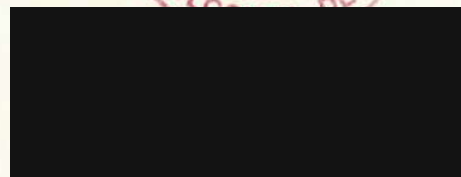

วิศวกรชำนาญการ



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 17 May, 2022

Certification No. 183/22

Page : 1 of 6

Object : Precision Weather Station

Manufacturer : Davis Instruments

Type : Vantage Pro 2 Model No. : 6152C

Mfg Code : Display BE190314046 Transmitter BE190314046

Customer : Blue Consultant Limited Partnership.
32/751 Thanon Pracha Uthit, Thung Khru,
Thung Khru, Bangkok 10140.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1006.5 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: Thermoschneider No.9188 : testo, testo 645 Serial No. 02848057

la Type PTB220 No. V1220015

(Authorised Signatory)

for the Chief

Sub-Standard Instrument



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Certification No. 183/22

17 May, 2022

Page : 2 of 6

Standard Ultrasonic Anemometer	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacumm	Velocity	Velocity	Correction
	m/sec inches H2O	m/sec inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.9	0.10
7.00	-	-	-	6.7	0.30
9.02	-	-	-	8.9	0.12
11.01	-	-	-	10.7	0.31
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.7	0.31
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.3	0.72

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibration & Test Section

Meteorological Instruments Bureau

Mechanical Engineer



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 0-2396-0156,0-2399-0469

The Result of Calibration

Certification No. 183/22

17 May, 2022

Page : 3 of 6

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
756.11	756.1	0.01
756.26	756.3	-0.04
755.92	756.1	-0.18
753.01	753.1	-0.09
752.57	752.7	-0.13
752.92	753.0	-0.08
753.26	753.4	-0.14
753.92	754.1	-0.18
754.33	754.4	-0.07
754.98	755.0	-0.02
755.51	755.6	-0.09
753.83	754.0	-0.17
754.25	754.4	-0.15
755.29	755.3	-0.01
756.27	756.4	-0.13
756.59	756.7	-0.11
756.87	757.0	-0.13
756.23	756.4	-0.17
755.63	755.7	-0.07
754.89	755.0	-0.11

Average

-0.10

Cal

Mechanical Engineer





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469


The Result of Calibration

Certification No. 183/22

17 May, 2022

Page : 4 of 6

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.2	45.3	-0.1
30.4	30.4	0.0
15.2	15.3	-0.1

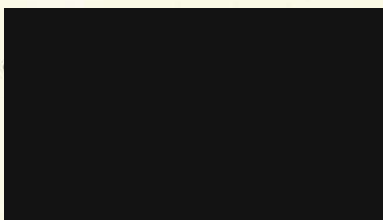

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration


Certification No. 183/22

17 May, 2022

Page : 5 of 6

Standard Humidity % R.H.	Relative Humidity Sensor Reading	
	Reading	Correction
	% R.H.	% R.H.
82.40	84	-1.60
61.62	62	-0.38
45.32	46	-0.68

Calib

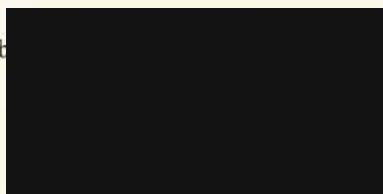

Mechanical Engineer






Date of Issue 17 May, 2022

Certification No. 183/22

Page : 6 of 6

ใบรับรอง

หนังสือฉบับนี้ขอรับรองว่า เครื่องวัดฝน ชี้อ Davis Instruments แบบ TIPPING
BUCKET Product No. 6152 C Mfg. Code. AZ170619045 ทำการสอบเทียบกับแก้ว
ฝนแบบแก้วตวง GAUGE DIAMETER 8.0 INCHES , NEGRETTI & ZAMBRA
LONDON No 71082 และสามารถนำไปใช้ได้ มีค่าถูกต้องตามรายละเอียดของ
เครื่องมือ (0.01 in/ TIP)

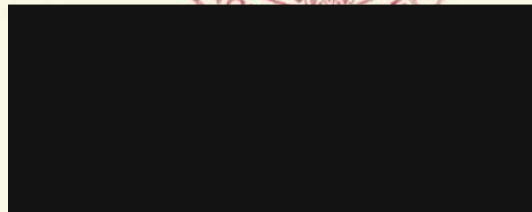

วศุกรชานาญการ

ภาคผนวกที่ 5-2

เอกสารสอบเทียบเครื่องมือตรวจวัดระดับเสียงโดยทั่วไป



ห้างหุ้นส่วนจำกัด บลู คอนซัลแตนท์ **Blue Consultant Limited Partnership**

32/751 ถนนประชาอุทิศ แขวงทุ่งครุ เขตทุ่งครุ กรุงเทพฯ 10140

โทร.0-2873-6045-6 โทรสาร 0-2873-6046

ห้องปฏิบัติการวิเคราะห์เอกซเรย์ใบอนุญาตลงวันที่ 14 สิงหาคม 2563

CALIBRATION REPORT

Instrument : Sound Level Meter

Manufacturer : ACO Co.,Ltd. Model 6236

Date of Calibrate : January 16, 2023

Dued Date of Calibrate : January 16, 2024

Calibrator : Sound Calibrator

Manufacturer : Scarlet Tech Co., Ltd.

Model : ST-120

Serial No. : ST120C0267E

Range of Calibrator : 93.97 dB

Calibration Report

No.	Serial No.	Before Adjust	After Adjust	Inspection Result
2	090148	93.9	94.0	Pass
5	090156	93.8	94.0	Pass
8	090171	93.9	94.0	Pass
10	090175	94.0	94.0	Pass
23	162034	93.9	94.0	Pass
26	162037	94.0	94.0	Pass
30	172104	94.0	94.0	Pass
33	212006	94.0	94.0	Pass
34	212007	94.1	94.0	Pass
35	212008	93.9	94.0	Pass



ผู้จัดการห้องปฏิบัติการ

Certificate of Calibrator

for ST-120 Sound Calibrator

No. 20230501J148

Name of Product Sound Calibrator
Type ST-120
Serial Number ST120C0267E
Specification Class 1
Date 2023/05/01

Tested by



1. Outside : OK
2. Sound Pressure Level : 94.01 dB ; 114.08 dB
3. Frequency : 1002.0 Hz
4. Distortion : 1.04 % ; 1.14 %

Environment conditions :

Air temperature : 20 °C
Relative humidity : 50 %
Static pressure : 101.8 kPa

Scarlet Tech Co., Ltd.

4F-3, No. 347, HePing E Rd, 2nd Sec, DaAn District, Taipei City 106, Taiwan
E-mail: info@scarlet.com.tw www.scarlet-tech.com

ภาคผนวกที่ 5-3

เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพน้ำ





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CH1128


Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH1100
Serial No. : B80A0042
ID No. : TNP.LAB.02
Condition As-Received: Used Item
Received Date : 24 August 2022
Calibration Date : 25 August 2022
Reference : 208-0843WN-1
Submitted by : TNP ENVIRONMENT CO.,LTD
332/173 Moo 3, Bang Rak Phatthana,
Bang Bua Thong, Nonthaburi 11110
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard
voltage calibrator and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lerngagtrakul

Approved by :

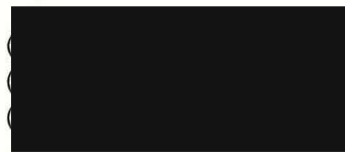

Issue Date :

29 August 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0044697



Cert.No.: 22CH1128

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	46530031	130RC098	21E3245	07 Oct 2022
2) Ref. Standard Thermometer	4982054	110RC044	21I1201	26 Oct 2022

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	823320	20 June 2024
pH 6.985	CPA chem	794122	14 Feb 2023
pH 10.008	CPA chem	823323	20 June 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: B80A0042	4.00	177.48	177.4	4.01	0.058	2.00
	7.00	0.00	0.0	7.00	0.058	2.00
	10.00	-177.48	-177.5	10.01	0.058	2.00

a 1123682



Cert.No.: 22CH1128

Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (\pm)	Coverage factor k
pH Electrode S/N.: 9X0B0575	4.008	4.01	153.9	0.0086	2.05
	6.985	6.99	-18.8	0.012	2.05
	10.008	10.01	-190.3	0.011	2.05

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 961X5S
- Serial No. : 9X0B0575

Dimension of probe;

- Length : 87 mm.
- Diameter : 12 mm.
- Immersion Depth : 80 mm.

Calibration Point ($^{\circ}\text{C}$)	Standard Temperature ($^{\circ}\text{C}$)	UUC* Reading ($^{\circ}\text{C}$)	Error ($^{\circ}\text{C}$)	Uncertainty of measurement (\pm $^{\circ}\text{C}$)	Coverage factor k
20.0	20.003	20.0	-0.003	0.13	2.00
25.0	25.002	25.0	-0.002	0.13	2.00
30.0	30.004	30.0	-0.004	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

a 1123681



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484




Cert.No.: 23CH126

Page.: 1 of 2

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Adwa
Model : AD 12
Serial No. : 1328
ID No. : TNP.LAB.13
Condition As-Received: Used Item
Received Date : 27 January 2023
Calibration Date : 30 January 2023
Reference : 2301-0937WN-2
Submitted by : TNP ENVIRONMENT CO.,LTD
332/173 Moo 3, Bang Rak Phatthana,
Bang Bua Thong, Nonthaburi 11110
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard
voltage calibrator and direct measurement
with certified reference material (CRM)

Calibrated by : Walalāk Sirithean

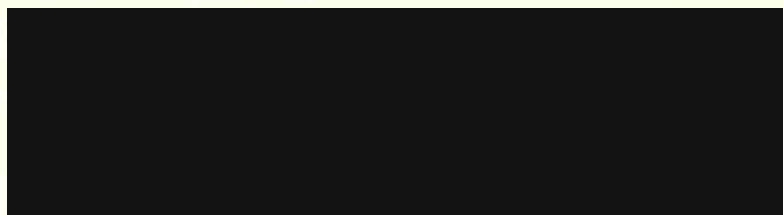

Issue Date : 31 January 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written

Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0050390



Cert.No.: 23CH126

Page.: 2 of 2

Condition of this calibration result

1. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	826588	09 July 2024
pH 6.987	CPA chem	826589	09 July 2023
pH 10.008	CPA chem	826590	09 July 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : pH Measurement

Performing two buffers standard curve by using buffer nominal pH (4,7)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: 1328	4.008	4.01	N/A	0.0085	2.05
	6.987	6.99	N/A	0.011	2.00
	10.008	10.02	N/A	0.0095	2.00

Remark

- pH meter does not have voltage mode.
- Can not connect the BNC because the plug does not match with the socket.
- N/A = Not Available

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %

-o0o-

Certificate of Calibration

Certificate No. : 65-400557-1

Page : 1 of 2

Submitted by : TNP Enviroment Co., Ltd.

332/173 Moo 3 Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

Equipment : Digital Thermometer (Pocket)

Temperature Indicator

Manufacturer : Extech

Model : 39240

Range : N/A °C

Resolution : 0.1 °C

Serial No. : PONPE5877172

ID No. : TNP.LAB.34-2564

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Line Voltage : (220 ± 22) VAC

Date of Received : 28 October 2022

Date of Calibration : 29 October 2022

Date of Issue : 29 October 2022

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0016-22	07 Feb 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)
400004	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)

Approved

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-400557-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
100	20.0019	19.9	0.1	0.18
100	30.0022	29.9	0.1	0.22
100	40.0021	39.9	0.1	0.22


Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 22H1779

Page : 1 of 2

Equipment : Digital Thermo-Hygrometer

Manufacturer: Exttech

Model : 448514

Serial No.: PONPE 5816745

ID No.: TNP.LAB.04

Condition As-Received: Used Item

Received Date: 24 August 2022

Calibration Date: 27 August 2022

Reference: 2208-0843WN

Submitted by: TNP ENVIRONMENT CO.,LTD

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

332/173 Moo 3, Bang Rak Phatthana, Bang Bua Thong,
Nonthaburi 11110

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard Chilled Mirror Hygrometer Sensor	Dew Prime II	31863	19714	17 Sep 2022
2) Standard Humidity/Temperature Meter	400	10240757	TH-0125-21	13 Dec 2022

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained at:-

- National Institute of Standards and Technology (NIST) , The United States of America
- National Institute of Metrology Thailand (NIMT)

Calibrated by : Somchai Dumwor
Issue Date : 30 August 2022

Approved Signatory



B 0295353



Cert. No.: 22H1779

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Humidity measurement.

<u>Reference</u> <u>Temperature</u> (°C)	<u>Standard</u> <u>Humidity</u> (%R.H.)	<u>UUC*</u> <u>Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty</u> <u>of Measurement</u> (±%R.H.)
25.0	50.1	47	-3.1	1.6

Result of Calibration:-

Without Adjustment

Function:


Temperature measurement for indoor sensor.

<u>Standard</u> <u>Temperature</u> (°C)	<u>UUC*</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> <u>of Measurement</u> (±°C)
20.02	20.1	0.08	0.42
25.03	25.4	0.37	0.42

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-o0o-



a 1123737

Certificate of Calibration

Certificate No. : 65-400665-1

Page : 1 of 2

Submitted by : TNP Environment Co., Ltd.

332/173 Moo 3 Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

Equipment : Air Chamber (Oven)

Manufacturer : Memmert

Model : UF75

Range : N/A °C

Resolution : 0.1 °C

Serial No. : B320.0251

ID No. : N/A

Environment : On site calibration was carried out at the Laboratory, TNP Environment Co., Ltd.

Ambient Temperature : (27.0 to 28.0 °C

Relative Humidity : (40 to 45) %

Line Voltage : (228.0 to 230.0) V

Date of Received : 26 December 2022

Date of Calibration : 26 December 2022

Date of Issue : 28 December 2022

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400030	65-400548-1	26 Apr 2023	National Institute of Metrology Thailand (NIMT)

Approved by

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-400665-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

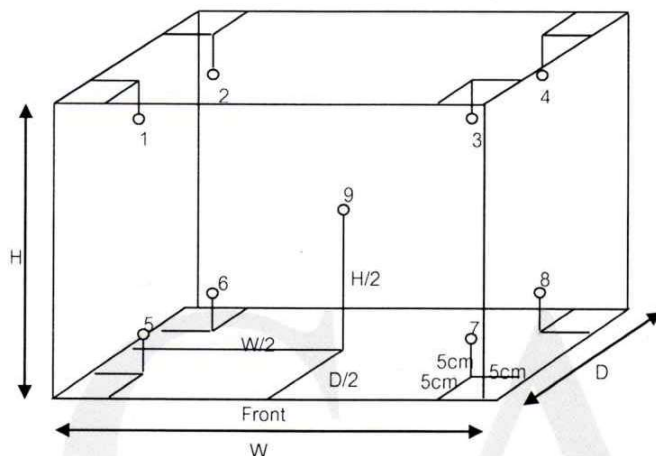

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.56 m

Capacity = 0.07 m³

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty (± ° C)
			1	2	3	4	5	6	7	8	9	
104.0	104.0	104.0	104.2	104.1	104.2	104.0	103.8	103.9	103.9	103.9	104.0	0.69
180.0	180.0	180.0	179.6	179.6	179.7	179.8	180.2	179.5	179.0	179.8	180.5	1.0

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Uniformity (° C)	Measured Stability (° C)	Overall Variation (° C)
104.0	104.0	104.0	0.4	0.1	0.7
180.0	180.0	180.0	1.7	0.3	2.0

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate No.: T/O 650134

Date of issue : 11-Oct-2022

Equipment Description : Refrigerator
Equipment Model : P1010
Equipment Serial No. : P1010-1020-0005
I.D. No. or Control No. : TNP.LAB.01
Manufacturer : Entech Industrial Solution Co.,Ltd.
Customer Name : TNP ENVIRONMENT CO.,LTD.
Customer Address : 332/173 Moo. 3 Tambon Bang Rak Phatthana, Amphoe Bang Bua Thong,
Nonthaburi 11110
Total pages of certificate : 2 pages
Instrument Receiving Date : 10-Oct-2022
Receiving No. : O-220115
Environmental Conditions : All of the measurement were carried out in the working area
Temperature : (25 ± 15) °C
Humidity : (55 ± 30) % RH
Voltage : (220 ± 22) VAC
Calibration Place : 332/173 Moo. 3 Tambon Bang Rak Phatthana, Amphoe Bang Bua Thong,
Nonthaburi 11110
Calibration Procedure No. : WI-CL-18-C

The calibration certificate expended uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%

*The standard uncertainty of measurement has been determined in accordance with M 3003
The expression uncertainty and confidence in measurement.*

This certificate is applied only to item under test environmental condition.

*This calibration certificate may not be reproduced other than in full except with the permission of the issuing laboratory.
Calibration certificates without signature and seal are not valid.*

This calibration certificate documents are traceability to national standards, which realize the unit of measurement according to the International system of units (SI).

Date of Calibration : 10-Oct-2022

Calibration Engineer

Technical Manager

Certificate No. : T/O 650134


The Reference Standard Instrument :-

Instrument	Model	Serial No.	Cert No.	
1) Data logger with RTD Probe	Agilent 34972A	MY60008352	PSL-T 0524-3/65	4-Apr-2023

Measured room conditions

Temperature :	Minimum: 30.4 °C	Maximum: 31.6 °C
Humidity :	Minimum: 51.4 %RH	Maximum: 56.7 %RH
Voltage :	Minimum: 220.1 VAC	Maximum: 223.2 VAC
Fresh Air Setting:	off	

Sensor Position :

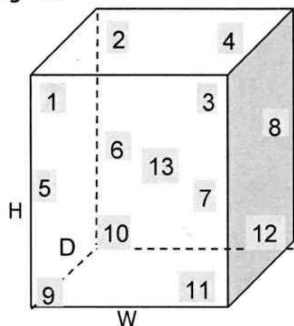

Working Space of chamber :

(Inside Dimensions) W x D x H : 1560 mm x 500 mm x 1380 mm

Sensor Installation Details :

- Sensor Number 1 to 12 installed approximately 50 mm From each wall.
- Sensor Number 13 installed approximately geometric of the chamber.

Results : The measurement results of the calibration were reported in the table below.

(*) Without adjustment

() After adjustment

UUC* Setting	UUC* Reading	Temperature Reading of Standard Sensor								
(°C)	(°C)	Sensor Position								
		1	2	3	4	5	6	7	8	9
		4.52	4.36	4.21	4.00	4.52	4.20	4.77	4.39	4.07
		Sensor Position								
		10	11	12	13					
		4.16	4.17	4.54	4.07					

UUC* Setting	UUC* Reading	Temperature Uniformity	Temperature Stability	Overall Variation	Uncertainty of Measurement	Coverage Factor
(°C)	(°C)	(°C)	(± °C)	(°C)	(± °C)	K
4.0	4.0	1.07	0.93	2.23	1.2	2

UUC* = Unit Under Calibration

Remark :-

- Temperature reading of Standard Sensors shown in the table were taken from the average of Standard reading at each position.
- Temperature Uniformity was calculated from the difference between the maximum and minimum of actual temperature reading from all reference sensors at the same time.
- Temperature Stability was calculated from the maximum stability of nine positions, and formula of Stability is [(Maximum Temperature Value - Minimum Temperature Value) / 2]
- Overall Variation was calculated from the difference between the maximum and minimum measured temperature throughout observation time.

End of Report

Calibration Certificate

Cert. No. : CT-23-01-23295

Page : 1 of 4

Issued date : 24 January 2023

Equipment : Water Bath , Manufacturer : MLAB , Model : WBN30
S/N = 0347 , Customer ID = -

Client : TNP ENVIRONMENT CO.,LTD.
332/173 Moo 3 Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

Received Date : 20 January 2023

Ref. Job No. : SO6601-00020

Calibrated by : Mr.Apiwat Mungsamak

Cert. prepare by : Ms.Nattanicha Panumram

Calibrated Date : 20 January 2023

Approved by : Mr.Montree Ruschasetkul

Calibration Place : ห้องปฏิบัติการ2

Environment Condition : Temperature 28.5 ± 2.7 (°C) , Humidity 57.5 ± 14.5 (%RH)

Calibration Method : In-house method based on ASTM E715-80 (Reapproved 2006) , (MTEC WI No. # WICAL-02-003-R01)

Reference Standard Instrument :

No	Instrument	code	Model	Due date
1	Temperature Data Logger	MTEC-CE-0175	MLAB	10/2023
2	Thermo Hygrometer	MTEC-CE-0183	TP-50	06/2023


Condition of certificate :

(1) This certificate is traceable to International System of units (SI Units) . , (2) This certificate was certified only for the instrument we calibrated.
, (3) This result of calibration was found accurate as show on date and place of calibration only. , (4) The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k =$ (see result table) , providing a level of confidence of approximately 95%. , (5) This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration Division, Metrology Technical Co.,Ltd.

Calibration Result :

Condition of UUC :

- 1) Adjust Condition : Without Adjustment
- 2) Lid Cover : Flat Sheet (Plastic , from
- 3) Circulation : without circulation
- 4) X ,Y = 5 cm. , B ~ 3 cm.

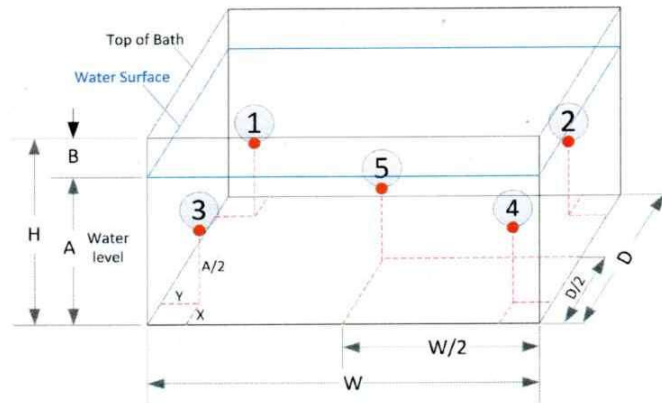

Pic 1 : Position of each sensor No.

- (1) The quoted uncertainty include with " Stability".
- (2) Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors , for at least half an hour after reaching sted state.
- (3) Uniformity = The maximum difference of measured temperatures at two any sensor which are observed at the same time.
- (4) Overall variation = The difference of the maximum and the minimum measured temperature throughtout observation time.

Section 1 : Report of Temperature distribution

Unit : (°c)

Calibration Point	UUC Setting (*)	UUC Reading (*)	Measured Temperature @ Sensor No.					Uncertainty (±)	k (**)
			#1	#2	#3	#4	#5		
85	85	85.0	85.30	85.30	84.83	84.76	85.51	0.627	2

(*) = The average of 30 values in each point , (**) = Coverage factor (k) value

Section 2 : Report of Chamber Performance

Unit : (°c)

Calibration Point	UUC Setting (*)	UUC Reading (*)	Temperature Uniformity	Temperature Stability (± °c)	Temperature Overall Variation
85	85	85.0	1.34	0.45	1.64

(*) = The average of 30 values in each point

Approved Signatory :

Certificate No. : CT-23-01-23295

Page : 3 of 4


Section 3 : Possible of temperature in chamber. Show minimum and maximum of the average values and include with uncertainty of measurement. , The average values is average of each position standard sensor throughout observation time.

Unit : (°C)

Calibration Point	UUC Setting ^(*)	UUC Reading ^(*)	Possible of Minimum temperature in chamber	Possible Maximum temperature in chamber
85	85	85.0	84.13	86.13

(*) = The average of 30 values in each point


Section 4 : Trend of accuracy

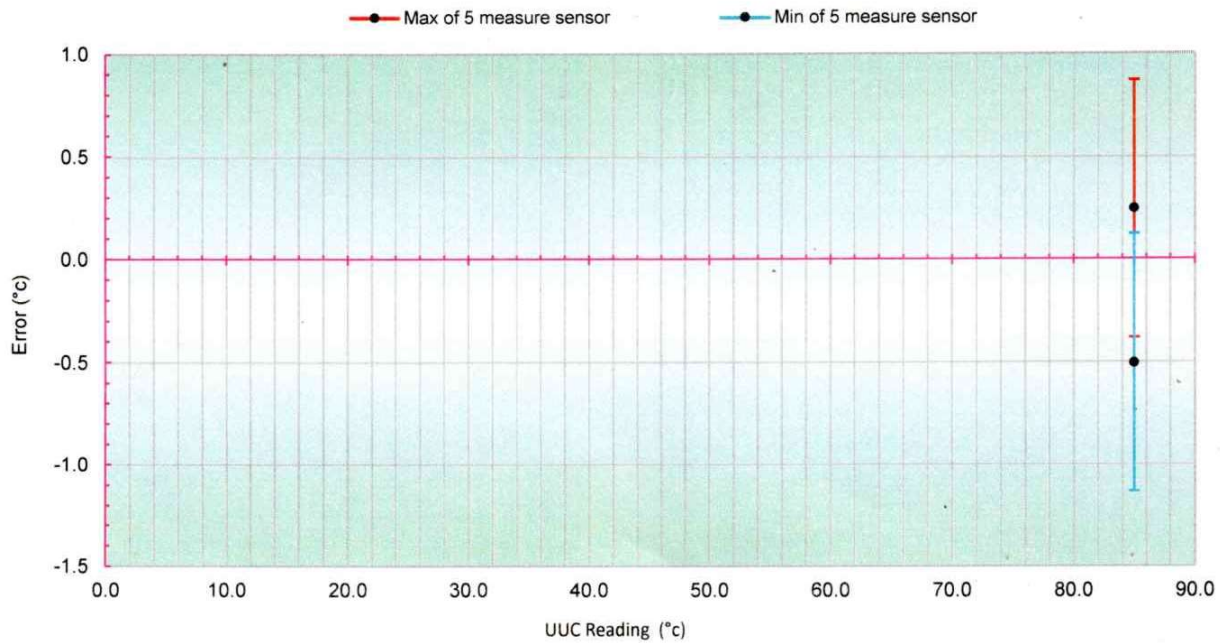

Approved Signator

Section 5 : Graph report for Temperature distribution , not include uncertainty of measurement

(5.1) Temperature Distribution at UUC Reading 85.0 °c

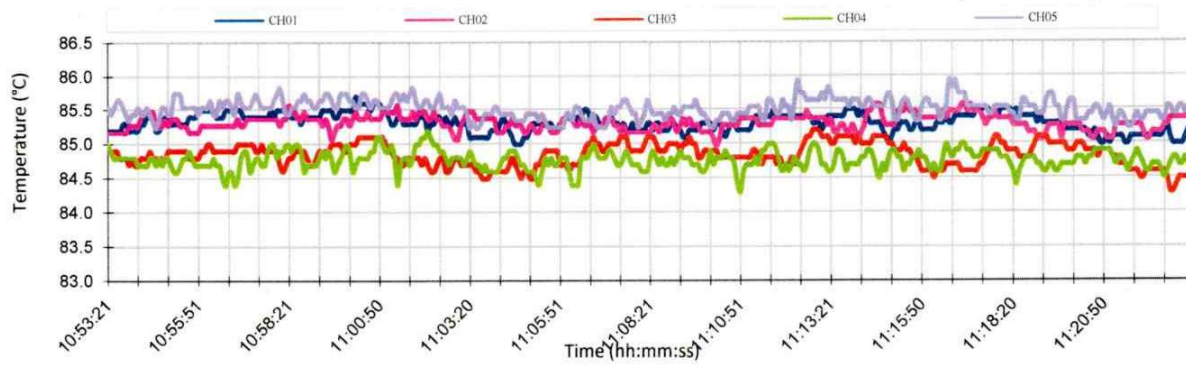

Approved Signatory

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com



CALIBRATION No.0426

SARTORIUS

Certificate of Calibration

Model Number : SECURA224-1S

Description : Analytical Balance

Serial Number : 41305301

Manufacturer : Sartorius

Certificate No. : 22BCI0160

Issued Date : Tuesday, June 21, 2022

Reference No. : 186783

Page No. : 1 of 2

Customer Name : TNP Environment Co., Ltd.

332/173 Moo 3, Bang Rak Phatthana Bang Bua Thong, Nonthaburi 11110 Thailand.

Calibrated Place : Weighing Room

Calibrated By : Mr.Chonchai Inthana

Calibration Date : Thursday, June 16, 2022

Calibration

Procedure No. : This calibration was conducted by

Using in-house calibration procedure number (WI-003)

Based on UKAS LAB 14 : 2019

Metrological data :

Capacity : 220 g Readability 0.0001 g

Ambients Conditions:

Temperature : 23.8 °C ± 5.0 °C

Humidity : 66.5 % RH ± 10.0 % RH

Pressure : — ± —

Reasons for calibration☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance**Equipment Condition:** ☒ Good Operate ☐ Fair**Measurement Method UKAS Publication Ref :Lab 14**

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI).

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2, YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	SPC-RT	C19210498	31-Aug-2022

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division
Sartorius (Thailand) Co., Ltd.

SOP FM 33 03 February 2022

S
T
A
M
P

Certificate of Calibration

Model Number : SECURA224-1S

Description : Analytical Balance

Serial Number : 41305301

Manufacturer : Sartorius

Certificate No. : 22BCI0160

Issued Date : Tuesday, June 21, 2022

Reference No. : 186783

Page No. : 2 of 2

Calibration Results : Without Adjustment

Repeatability



The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0001
20 g	20.0000	200.0000
Tolerance	20.0000	200.0001
0.0001 g	20.0000	200.0000
	20.0000	200.0000
Nominal Value : (High Load)	20.0000	200.0000
200 g	20.0000	200.0000
Tolerance	20.0000	200.0001
0.0001 g	20.0001	200.0000
	20.0000	200.0000
Standard Deviation	0.00003	0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 50 g
Tolerance 0.0004 g



Difference

1	—
2	0.0000
3	0.0000
4	0.0000
5	0.0000
6	—

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00013
0.1	0.1000	0.1000	0.0000	0.00013
1	1.0000	1.0000	0.0000	0.00013
2	2.0000	2.0000	0.0000	0.00013
5	5.0000	5.0000	0.0000	0.00013
10	10.0000	10.0000	0.0000	0.00013
20	20.0000	20.0000	0.0000	0.00013
50	50.0000	50.0000	0.0000	0.00014
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	200.0000	0.0000	0.00030

End of Report.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 23T238

Page : 1 of 2

Equipment : Liquid-in Glass Thermometer

Manufacturer: SK

Model : -

Serial No.: -

ID No.: TNP.LAB.12

Condition As-Received: Used Item

Received Date: 27 January 2023

Calibration Date: 07 February 2023
to 10 February 2023

Reference: 2301-0937WN

Submitted by: TNP ENVIRONMENT CO.,LTD

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

332/173 Moo 3, Bang Rak Phatthana, Bang Bua Thong,
Nonthaburi 11110

Procedure used: Calibration were conducted using in-house calibration procedure CP-T02 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Digital Thermometer	1529	A7A609	22I1274	17 Oct 2023
2) Industrial Platinum Resistance Thermometer	5627-12	571975	22I1274	17 Oct 2023

2.The UUC* was immersed into liquid bath temperature controller and the top about 12 mm of the liquid column above the bath medium in every calibration points.


3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Thammanoon Phuwadkien
Issue Date : 14 February 2023

Approved Signa

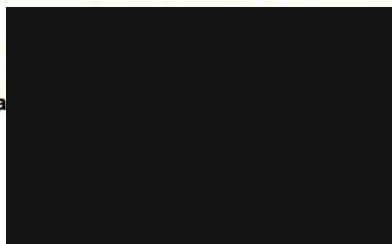

B 0307331



Cert. No.: 23T238

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Temperature measurement.

Type:

Total Immersion

Scale Division:

1 °C

Reference point (0 °C) Error = -0.9681 °C, with Uncertainty of Measurement of ± 0.16 °C

<u>UUC*</u> <u>Reading</u> (°C)	<u>Standard</u> <u>Temperature</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> <u>of Measurement</u> (\pm °C)
20	21.4342	-1.4342	0.16
30	31.5544	-1.5544	0.16
40	41.1382	-1.1382	0.16

Note: UUC* : Unit Under Calibration

The UUC* readings were made under magnification and resolved to one tenth of one scale division.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

-o0o-

รายการใบรับรองสอบเทียบ/ทวนสอบ เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวัดคุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือหลักสำหรับตรวจสอบคุณภาพน้ำ									
1	BOD Incubator	BOD	Arco	UC4-1320 / (UAE.WAO.015/2561)	Technology Promotion Association (Thailand-Japan)	22TM90	17 Feb 22	16 Feb 23	-
2	BOD Incubator		Arco	UC4-1320 / (UAE.WAO.018/2559)	Technology Promotion Association (Thailand-Japan)	21TM1406	17 Aug 21	16 Aug 22	-
3	Analytical Balance (Readability 0.01 mg)	Total Dissolved Solids Suspended solids	Mettler-Toledo	XSR205DU / C009071872	Technology Promotion Association (Thailand-Japan)	22MM210	26 Apr 22	25 Apr 23	-
4	Hot Air Oven		Memmert	UF55 / B216.1666	Technology Promotion Association (Thailand-Japan)	21TM1876	29 Oct 21	28 Oct 22	-
5	Digestor Unit	TKN	FOSS TECATOR	2520auto / 91794469	National Food Institute, Ministry of Industry, Thailand	2202361-001-01	4 Apr 22	3 Apr 23	-
6	Distillation Unit (Kjeldahl Method)		FOSS TECATOR	KT200 / 91790524	FOSS South East Asia	5874	30 Nov 21	29 Nov 22	-
7	Analytical Balance (Readability 0.1 mg)	Fat, Oil & Grease	Mettler-Toledo	AB-204S/FACT / 1129361010	National Food Institute, Ministry of Industry, Thailand	2103270-001-01	11 Jun 21	10 Jun 22	-
8	UV-VIS Spectrophotometer	Ammonia, Cyanuric Acid Nitrate, Total Nitrogen	Hitachi	U-1900 / 2021-064	DQE Services Co.,Ltd.	SP22-007	20 Jan 22	19 Jan 23	-
9	UV-VIS Spectrophotometer	Total phosphorus	Hitachi	U-2900 / 21E22-009	DQE Services Co.,Ltd.	SP22-008	20 Jan 22	19 Jan 23	-
10	Incubator	Total Coliform Bacteria Fecal Coliform Bacteria	Memmert	IPP 260 / V616.0066	Technology Promotion Association (Thailand-Japan)	21TM1874	28 Oct 21	27 Oct 22	-
11	Incubator	Escherichia coli Staphylococcus aureus	Memmert	IPP 260 / V615.0187	Technology Promotion Association (Thailand-Japan)	22TM563	07 Apr 22	06 Apr 23	-
12	Incubator	Pseudomonas aeruginosa Clostridium perfringens	Memmert	IN 75 / D317.0307	Technology Promotion Association (Thailand-Japan)	22TM335	17 Feb 22	16 Feb 23	-

บริษัท ยูเน็ด แอนาไลสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด
ห้องปฏิบัติการวิเคราะห์มาตรฐาน ISO/IEC 17025

รายการใบรับรองสอบเทียบ/พวนสอบ เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวัดคุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือหลักสำหรับตรวจสอบคุณภาพน้ำ									
13	Incubator	Total Coliform Bacteria Fecal Coliform Bacteria	Memmert	BE400 / e402.1032	Technology Promotion Association (Thailand-Japan)	21TM1358	15 Jul 21	14 Jul 22	-
14	Water Bath	Escherichia coli Staphylococcus aureus	Memmert	WNE 14 / L416.0612	Technology Promotion Association (Thailand-Japan)	22TM334	17 Feb 22	16 Feb 23	-
15	Water Bath	Pseudomonas aeruginosa Clostridium perfringens	Memmert	WNE 14 / L414.1407	Technology Promotion Association (Thailand-Japan)	22TM565	7 Apr 22	6 Apr 23	-
16	Analytical Balance		Mettler-Toledo	MS603S / B0070110311	Mettler-Toledo (Thailand) Ltd.	TH2058-096-040722-ACC-TH	7 Apr 22	6 Apr 23	-
17	Auto Clave		ALP	CL-40L / 802664	Technology Promotion Association (Thailand-Japan)	22TM89	17 Feb 22	16 Feb 23	-

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22MM210
Page.: 1 of 3

Certificate of Calibration

Equipment : Electronic Balance
Manufacturer : Mettler Toledo
Model : XSR205
Serial No. : C009071872
ID No. : UAE.WAO.012/2563
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phakhanong,
Bangkok 10260
Location : Balance Room
Received order : 26 April 2022
Calibration Date : 26 April 2022
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 90 %
Calibrated by : Kunchit Promprat



Issue Date : 29 April 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม
00949716



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2204-0542OC-1

Cert.No.: 22MM210
Page: 2 of 3

Procedure used :-

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Test report No.</u>	<u>Due date</u>
1) Standard Weight Set (E2)	15884	-	70RC138	MM-0009-21	3 Feb 2023

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certification is traceable to the International System of Unit.

Result of calibration () Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity :	0 g to 81 g	Resolution	0.00001 g
	81 g to 220 g	Resolution	0.0001 g

Before Adjustment :

<u>Applied Weight</u>	<u>Balance Reading</u>	<u>Correction</u>	<u>Measurement Uncertainty</u>	<u>Coverage Factor</u>
(g)	(g)	(g)	(\pm mg)	(k)
80	80.00004	-0.00004	0.15	2.00
200	199.9999	+0.0001	0.35	2.00

After Adjustment :

1. Determination of the standard deviation of weighing machine (n = 10)

<u>Applied Weight</u>	<u>Standard Deviation of Reading (g)</u>
(g)	
80	0.000008
200	0.00005



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2204-0542OC-1


Cert.No.: 22MM210

Page: 3 of 3

Result of calibration

2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.
The weighing machine reading error obtained is given in the table

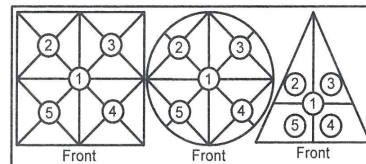

Maximum difference between
off-center and central loading
(g)
0.0002

Position 1	Position 2	Position 3	Position 4	Position 5
(g)	(g)	(g)	(g)	(g)
-0.0002	-0.0001	0.0000	-0.0002	-0.0002

3. Departure from nominal value

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
(g)	(g)	(g)	(\pm mg)	(k)
Unload	0.00000	0.00000	0.016	2.13
0.05	0.05001	-0.00001	0.016	2.13
0.1	0.10001	-0.00001	0.017	2.11
1	1.00002	-0.00002	0.019	2.05
5	5.00003	-0.00003	0.026	2.00
20	20.00008	-0.00008	0.049	2.00
50	50.00010	-0.00010	0.080	2.00
80	80.00014	-0.00014	0.15	2.00
100	100.0001	-0.0001	0.21	2.00
150	150.0001	-0.0001	0.29	2.00
200	200.0001	-0.0001	0.35	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Calibration Certificate

Certificate No.: 2203120-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance

Manufacturer: METTLER TOLEDO

Model: AB204-S/FACT

Serial No.: 1129361010

ID No.: UAE.WAS.002/2552

Order No.: 2203120

Operation No.: 2203120-001

Date of Receipt: 1 June 2022

Date of Calibration: 1 June 2022

Calibrated by Mr.Taveesak Seilee
Scientist

Approved

Manager, Division of Calibration Laboratory

Date of Issue: 7 June 2022

Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2203120-001-01

Equipment:

Electronic Balance

Manufacturer: METTLER TOLEDO

Model: AB204-S/FACT

Resolution: 0.0001 g

Serial No.: 1129361010

ID No.: UAE.WAS.002/2552

Capacity: 220 g

Date of Calibration: 1 June 2022

Page 2 of 3

Environment Condition: Ambient Temperature: 19.9 ± 0.3 °C Relative Humidity: 45 ± 1.5 %

Place of Calibration: 108, Balance Room, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	B308068554	TCS	M2201020S	6 January 2023
Standard Weight Class E2	1-500g	B308068128	TCS	M2201021S	6 January 2023

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	PONPE 490	NFI.BTH 010/18	Quality Reborn	QR22-0350	18 February 2023

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:




1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
100	0.000048
200	0.000052

2. Off-Center Error:

A mass of 50 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
49.9999	49.9998	49.9998	49.9999	49.9998	49.9998	0.0001



Calibration Report

Certificate No.: 2203120-001-01

Equipment:

Electronic Balance

Manufacturer: METTLER TOLEDO

Model: AB204-S/FACT

Resolution: 0.0001 g

Serial No.: 1129361010

ID No.: UAE.WAS.002/2552

Capacity: 220 g

Date of Calibration: 1 June 2022

Page 3 of 3

Calibration Results: (Continued)

Calibration Range: 0 - 200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.00000	0.0000	0.0000	0.000088	2.00
0.01	0.01000	0.0100	0.0000	0.000088	2.00
0.05	0.05000	0.0499	0.0001	0.000088	2.00
0.1	0.10000	0.1000	0.0000	0.000088	2.00
0.2	0.20000	0.2000	0.0000	0.000088	2.00
0.5	0.50000	0.5000	0.0000	0.000088	2.00
1	1.00000	0.9999	0.0001	0.000088	2.00
2	2.00000	1.9999	0.0001	0.000089	2.00
5	5.00000	5.0000	0.0000	0.000089	2.00
10	9.99998	9.9999	0.0001	0.000092	2.00
20	19.99999	19.9999	0.0001	0.000094	2.00
50	49.99990	49.9999	0.0000	0.00012	2.00
70	69.99989	69.9998	0.0001	0.00014	2.00
100	100.00001	99.9999	0.0001	0.00017	2.00
150	149.99991	149.9997	0.0002	0.00022	2.00
200	200.00007	199.9998	0.0003	0.00030	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1064

Page.: 1 of 3

Certificate of Calibration

Equipment : Incubator

Manufacturer : Memmert

Model : BE 400

Serial No. : e402.1032

ID No. : UAE.MIC.001/2546

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260

Location : Microbiology Laboratory


Received Order : 11 July 2022

Calibration Date : 11 July 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon



Issue Date : 18 July 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2207-0245OC-2

Cert. No.: 22TM1064

Page.: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Data Acquisition	34972A	MY57013823	22LM24	26 Feb 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration

	Beginning	Finished
Temp. (°C)	25	25
REL.Humid. (%)	62	63
AC Supply (Volt)	222	223

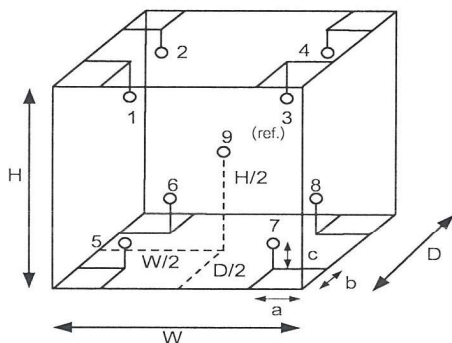

Position :	Ref. Std. ID No.:
1	21-17RTD-01
2	21-17RTD-02
3	17RTD-03
4	17RTD-04
5	17RTD-05
6	17RTD-06
7	17RTD-07
8	17RTD-08
9 (ref.)	17RTD-09

Probe Installation Details :

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :

D = 0.40 m
W = 0.33 m
H = 0.40 m
Capacity = 0.053 m³

เอกสารไม่ค



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2207-0245OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 22TM1064

Page.: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
37.0	38.0	38.0	0.092	0.62	0.94	0.30	2
56.0	57.5	57.5	0.083	0.87	1.3	0.42	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
37.0	37.629	37.576	37.476	37.577	36.834	36.997	36.824	37.038	37.387
56.0	56.489	56.520	56.445	56.485	55.291	55.589	55.899	55.591	56.097

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation

UUC* : Unit Under Calibration


Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่คว



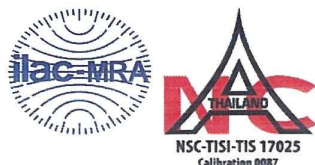

Certificate of Calibration

Equipment:	Balance	Certificate No.:	C01223732
Model:	PX623	Issued Date:	09 December 2022
Serial No. (or ID.):	C236754745	Job No.:	KSPR2215576
Manufacturer:	Ohaus	Page:	1 of 2
Condition:	New		

Customer: United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak Sub-District,
Phrakhanong District, Bangkok, THAILAND 10260

Environment Condition: Temperature 26 °C ± 0.5 °C
Humidity 53 %RH ± 3.9 %RH

Calibration Place: United Analyst and Engineering Consultant Co., Ltd. (301 Microbiology Room)
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak Sub-District,
Phrakhanong District, Bangkok, THAILAND 10260

Calibration By: Mr. Adisai Maknoi

Calibration Date: 09 December 2022

The Method used: In-house method, CAL-WI-47, based on UKAS Lab 14

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Co., Ltd. Certificate No. C02221765


Person in charge

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.


The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

Calibration Results:

Without Adjustment

Eccentric Error: Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.

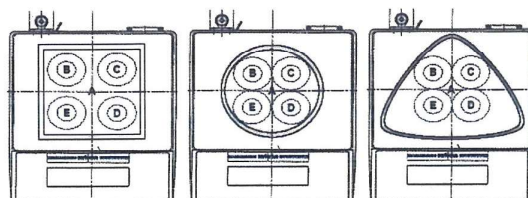

The diagrams illustrate the placement of weights on a balance pan for eccentric error testing. The first diagram shows a square pan with weights at the four corners, labeled B, C, D, and E. The second diagram shows a circular pan with weights at the four corners, labeled B, C, D, and E. The third diagram shows a triangular pan with weights at the four corners, labeled B, C, D, and E.

Nominal Test Value	200	(g)
Reference Points (g)		
A	B	C
-	0.000	0.000

Reference Points (g)				
A	B	C	D	E
-	0.000	0.000	0.000	0.000

Repeatability: Determination of the standard deviation of weighing balance., Readability 0.001 (g)

Nominal test value (g)	Standard Deviation
50	0.0004
500	0.0005

Error of indication from nominal or conventional mass value., Readability 0.001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Error of Indication (g)	Uncertainty (g)	k
1	1.0000	1.000	0.000	0.0010	2.03
5	5.0001	5.000	0.000	0.0010	2.03
10	10.0001	10.000	0.000	0.0010	2.03
20	20.0001	20.000	0.000	0.0010	2.03
50	50.0001	50.000	0.000	0.0010	2.03
100	100.0001	100.000	0.000	0.0011	2.03
200	200.0004	200.000	0.000	0.0011	2.02
300	300.0005	300.000	-0.001	0.0013	2.01
400	400.0008	400.001	0.000	0.0014	2.01
500	500.0003	500.000	0.000	0.0017	2.00
600	600.0004	600.000	0.000	0.0019	2.00

The End of Certificate

Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate:

The error of indication determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, UKAS Lab14. Therefore, those parameters have not been assessed separately.

Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :** ☐ Choice A Binary Statement for Simple Acceptance Rule ($w = 0$), Specific Risk $< 50\%$ PFA.
- ☒ Choice B Non-binary statement with guard band ($w = 1 U$), Pass or Fail Specific Risk $< 2.5\%$ PFA and Condition Pass or Condition Fail Specific Risk $< 50\%$ PFA.
- ☐ Choice C Customer defined, Customers may define arbitrary multiple of r to have applied as guard band ($w = r U$).
- ; PFA – Probability of False Accept



Authorized signatory

Statements of conformity:

Without Adjustment

Readability; 0.001 g

Nominal Value g	Error of indication g	Guard band (w) g	Tolerance (\pm) g	Conformity
1	0.000	0.0010	0.002	Pass
5	0.000	0.0010	0.010	Pass
10	0.000	0.0010	0.020	Pass
20	0.000	0.0010	0.040	Pass
50	0.000	0.0010	0.100	Pass
100	0.000	0.0011	0.200	Pass
200	0.000	0.0011	0.400	Pass
300	-0.001	0.0013	0.600	Pass
400	0.000	0.0014	0.800	Pass
500	0.000	0.0017	1.000	Pass
600	0.000	0.0019	1.200	Pass

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.


The End of Statements of conformity

Without Adjustment

Job No.KSPR2215576

Readability:0.001g

Error of indication

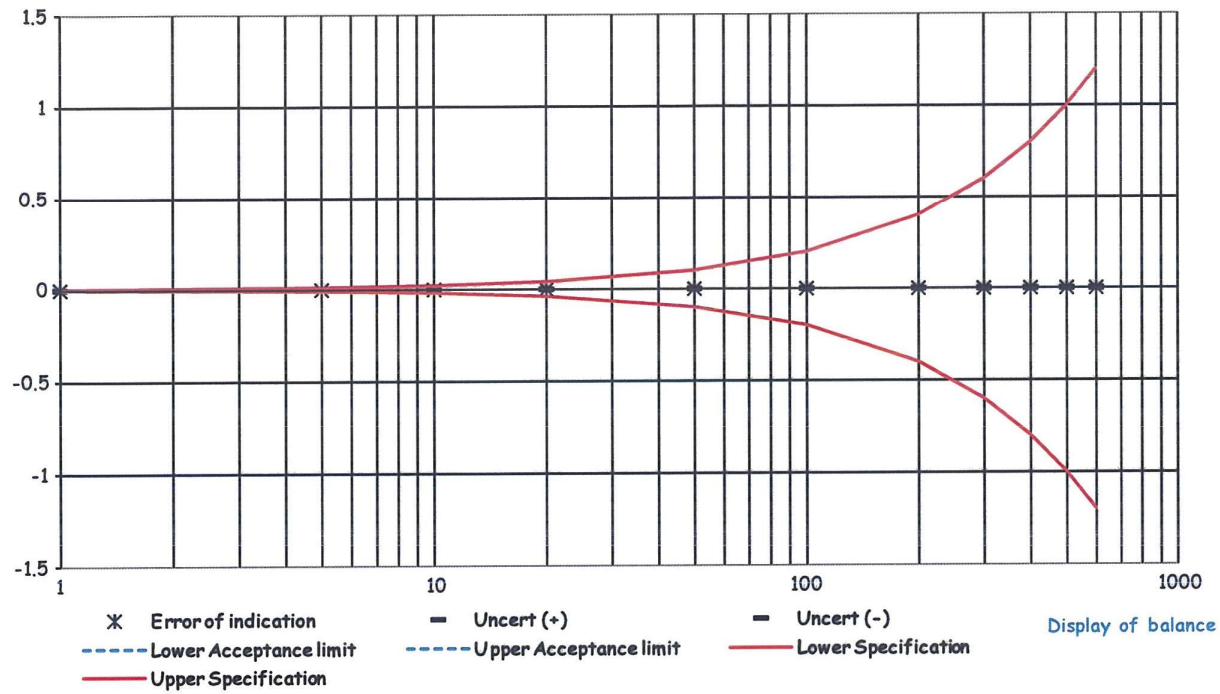

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1121

Page.: 1 of 3

Certificate of Calibration

Equipment : Autoclave

Manufacturer : ALP

Model : CL-40L

Serial No. : 807298

ID No. : UAE.MIC.019/2560

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260

Location : 301 Room


Received Order : 11 July 2022

Calibration Date : 11 July 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Preecha Hlahib



Issue Date : 18 July 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2207-0245OC-7

Cert. No.: 22TM1121

Page.: 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Data Acquisition	34970A	MY44060450	22LM46	28 Mar 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**


(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)

It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

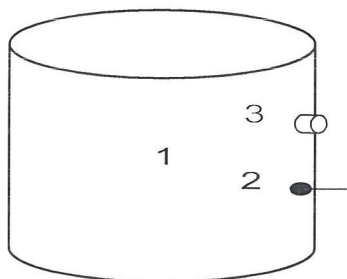

	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	29	49	220
Finished of Calibration	32	48	220

<u>Position</u>	<u>Description</u>	<u>Ref. Std. ID No.:</u>
1 =	Center of chamber	22-14TC-01
2 =	Temperature sensor	22-14TC-02
3 =	Exhaust port	22-14TC-03

เอกสารไม่คว



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2207-0245OC-7

Cert. No.: 22TM1121

Page.: 3 of 3

Result of Calibration :- (*) Without Adjustment

Operating parameter Set : Temperature = 115 °C

Sterilization period = 15 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
116	116	1	116.523	0.14	0.08	0.90	2
		2	116.566				
		3	116.440				

Operating parameter Set : Temperature = 121 °C

Sterilization period = 30 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
122	122	1	122.503	0.19	0.12	0.91	2
		2	122.637				
		3	122.558				

Average* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควา

CERTIFICATE OF CALIBRATION

Certificate No. : SP23-007

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)**Address :** 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260**Location of calibration :** Laboratory 315**Equipment :** UV-Vis Spectrophotometer**Manufacturer :** Hitachi**Model :** U-1900**Serial No. :** 2021-064**ID No. :** UAE.WAS.006/2552**Received Date :** 6 January 2023**Calibration Date :** 6 January 2023**Issue Date :** 10 January 2023**Condition Instrument :** Used**Calibrated by :**

Technical Manager

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

REPORT OF CALIBRATION

Certificate No. : SP23-007

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °CRelative humidity 55 ± 20 %RH**Calibration method :** In-house method CP-01 Based on ASTM E275-08**Certified Reference Materials :**

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	95935	22 October 2023
Absorbance Standard set	25757	95929	22 October 2023
Wavelength Standard set	25806	95916	22 October 2023
Wavelength Standard set	25758	95915	22 October 2023

Traceability : This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 4.0 nm.**Scan Speed of UUC :** 200 nm/min**Scan Interval of UUC :** 0.1 nm.**Resolution of UUC :** Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP23-007

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5787	0.575	0.0037	0.0031	2.00
	1.0490	1.044	0.0050	0.0029	2.00
	2.1900	2.181	0.0090	0.0080	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5607	0.558	0.0027	0.0034	2.00
	1.0247	1.021	0.0037	0.0035	2.00
	2.1229	2.115	0.0079	0.0081	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5236	0.520	0.0036	0.0030	2.00
	0.9634	0.961	0.0024	0.0029	2.00
	1.9763	1.968	0.0083	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5191	0.518	0.0011	0.0031	2.00
	1.0003	1.000	0.0003	0.0033	2.00
	1.9987	1.993	0.0057	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5523	0.552	0.0003	0.0030	2.00
	1.0809	1.082	-0.0011	0.0030	2.00
	2.0391	2.031	0.0081	0.0080	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5601	0.562	-0.0019	0.0032	2.00
	1.0512	1.052	-0.0008	0.0030	2.00
	1.9294	1.923	0.0064	0.0079	2.00

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP23-007

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7478	0.743	0.0048	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8686	0.861	0.0076	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2912	0.291	0.0002	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6448	0.639	0.0058	0.0055	2.00

REPORT OF CALIBRATION

Certificate No. : SP23-007

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor <i>k</i>
241.54	240.8	0.74	0.18	2.00
279.40	278.5	0.90	0.18	2.00
288.70	288.0	0.70	0.18	2.00
334.22	333.5	0.72	0.18	2.00
361.26	360.5	0.76	0.18	2.00
418.48	417.8	0.68	0.21	2.00
446.70	445.9	0.80	0.18	2.00
453.20	452.5	0.70	0.18	2.00
460.06	459.5	0.56	0.18	2.00
536.90	536.0	0.90	0.18	2.00
637.94	637.1	0.84	0.18	2.00
440.74	440.0	0.74	0.18	2.00
472.22	471.5	0.72	0.18	2.00
513.70	513.0	0.70	0.18	2.00
528.72	528.0	0.72	0.18	2.00
574.60	574.0	0.60	0.18	2.00
585.48	584.6	0.88	0.20	2.00
684.63	684.0	0.63	0.18	2.00
740.27	740.0	0.27	0.20	2.00
748.28	747.5	0.78	0.18	2.00
807.16	806.5	0.66	0.18	2.00
879.70	879.0	0.70	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k ,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- * Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม

Certificate No. : HIT-2219-0480

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment :	COD Test Tube Heater		
Meter Model :	HI839800-02	Serial No. :	04500052101
Tube Heater :	25 Vial Capacity	Accuracy :	$\pm 2^{\circ}\text{C}$
Temperature Range :	-10°C to 160°C	Temperature of Reaction :	150°C
Ambient Temperature :	$(25 \pm 2)^{\circ}\text{C}$	Relative Humidity :	$(50 \pm 15)\% \text{ RH}$
Manufacturer :	Hanna Instruments	Made in :	Romania
Condition As-Received :	Used Product	Reference :	RE220588
Customer name :	United Analyst and Engineering Consultant Co., Ltd. 3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak, Phrakhanong, Bangkok 10260		
Received date :	29 April 2022		
Calibrate date :	9 May 2022		
Issue date :	10 May 2022		
Calibrated Location :	Hanna Instruments (Thailand) Ltd.		
Calibration Procedure :	This calibrator was conducted by using in-house: calibration procedure CP-04 by using certified reference material		

Calibrated by :

Calibration Engineer

Authorized Signatory



This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written **
approval of the head of Hanna Instrument (Thailand).

เอกสารไม่ควบคุม

Condition of this calibration result

Reference Standard Instruments:

Instruments	Model	Serial No.	Certificate No.	Traceable
Data Acquisition Switch Unit	34970A	US37038858	WK2106-154-1	WK Electric Co., Ltd.

Calibration Result:

Measurement Temperature Source Accuracy for COD Reactor

Capacity (Vial)	Nominal Value (°C)	Average Value (°C)	(±) Uncertainty (°C)	(±) Tolerance of UUC (°C)	Acceptance Criteria
25 Vial	150.0	150.2	0.55	2	Pass

Figure: Shows the location of the temperature source.

(1A)	(2A)	(3A)	(4A)	(5A)
149.82°C	149.36°C	149.92°C	149.43°C	149.83°C
(1B)	(2B)	(3B)	(4B)	(5B)
150.45°C	150.66°C	150.37°C	149.66°C	150.01°C
(1C)	(2C)	(3C)	(4C)	(5C)
150.78°C	151.30°C	151.33°C	149.57°C	150.52°C
(1D)	(2D)	(3D)	(4D)	(5D)
151.12°C	151.59°C	150.80°C	149.62°C	149.81°C
(1E)	(2E)	(3E)	(4E)	(5E)
150.69°C	149.58°C	149.60°C	149.24°C	149.93°C

Remark: The Acceptance criteria is the error value plus or minus the Measurement Uncertainty, and then Not More than the Tolerance value of UUC, therefore concluded that pass.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

** End of certificate **

เอกสารไม่ควบคุม