



ภาคผนวก จ

เอกสารสอบเทียบเครื่องมือวิเคราะห์



เอกสารการสอบเทียบเครื่องมือตรวจวัด
บริษัท เอ็นไวรอนเมนต์ รีเสิร์ช แอนด์ เทคโนโลยี จำกัด

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT


Sampler Location				Date	May 22, 2023
วัดเขาโพธิ์(2023-00024)				Start Time	11:54 AM
Sampler Number	TSP No.A19	Transfer Standard Type	Orifice	Stop Time	12:04 PM
Instrument Model	HIVOL-BBCBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Nikul Phokamla
Motor Serial Number	2014-04	Calibrator Serial Number	3362		
Recorder Serial Number	7372				

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$	ample Flow Rate Indication	$IC = I[(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	(°K = °C+273)	(mmHg)		
	Positive	Negative	ΔH_2O		(m ³ /min)	(ft ³ /min)					
5	1.5	1.5	3.0	1.71149	0.84503	30.0	29.64	304.0	757.0		
7	2.4	2.4	4.8	2.16488	1.06702	41.0	40.51	304.0	757.0		
10	3.5	3.5	7.0	2.61434	1.28710	50.0	49.41	304.0	757.0		
13	4.5	4.5	9.0	2.96438	1.45849	55.0	54.35	304.0	757.0		
18	5.5	5.5	11.0	3.27724	1.61168	60.0	59.29	304.0	757.0		
Linear Regression Y ON X : Y= mX + b								Average	304.0	757.0	

Linear Regression Y ON X : Y= mX + b					Average	304.0	757.0		
1	Slope (m)	2.04234	Linear Equation		r^2	0.988773	Pstd(mmHg)	760.0	
2	Intercept (b)	-0.01435	Set Point Flow Rate (X) (m ³ /min)	1.133	r	0.9943707	T _{NTP}	298.0	
3	Correlation Coefficient (r)	0.99993	Final Set Flow Rate = (I)	0	(Pa/Pstd)*(Tstd/Ta)	0.976393698			
Result						C=(Pa/Pstd)*(Tstd/Ta)^0.5	0.988126357		

COMMENT

Andersen Instruments, Inc.

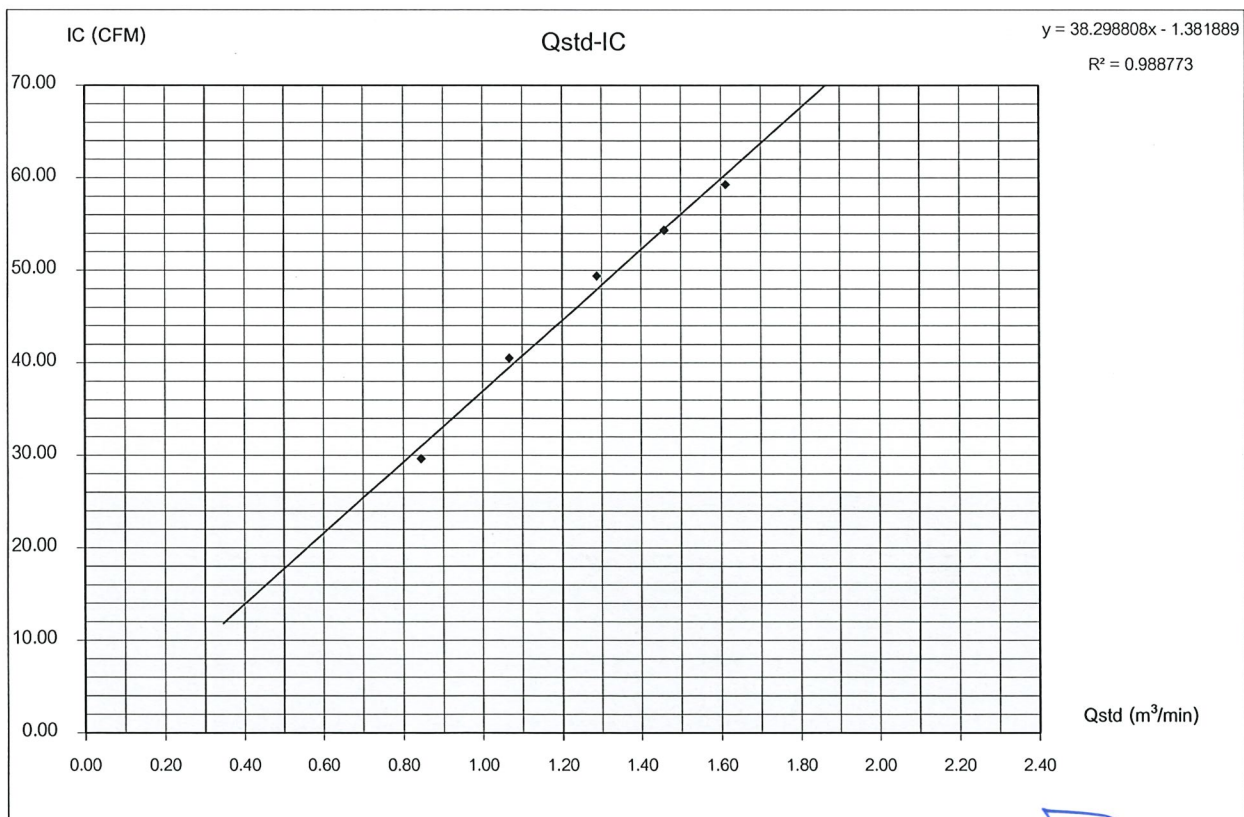

Checked By

Narongrit Tibsaj (Mr. Prayun Detkla)

Technician

Approved By

Mr. Panupon Podang

(Mr.Panupon Podang)
Environmental Scientist


PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	May 22, 2023
วัดเขาโพธิ์(2023-00024)				Start Time	11:44 AM
Sampler Number	PM10 No.14	Transfer Standard Type	Orifice	Stop Time	11:54 AM
Instrument Model	HIVOL-BMBBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Nikul Phokamla
Motor Serial Number	PM10No.14	Calibrator Serial Number	3362		
Recorder Serial Number	102950701				

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			[ΔH ₂ O(Pa/P _{std})(T _{std} /Ta)] ^{1/2}	Qstd = (1/m)[(A-b)] (m ³ /min)	ample Flow Rate Indicato (ft ³ /min)	IC = I[(Pa/P _{std})(T _{std} /Ta)] ^{1/2}	(°K = °C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O								
5	1.4	1.4	2.8	1.65345	0.81661	30.0	29.64	304.0	757.0		
7	2.4	2.4	4.8	2.16488	1.06702	40.0	39.53	304.0	757.0		
10	3.5	3.5	7.0	2.61434	1.28710	50.0	49.41	304.0	757.0		
13	4.5	4.5	9.0	2.96438	1.45849	56.0	55.34	304.0	757.0		
18	5.6	5.6	11.2	3.30690	1.62620	62.0	61.26	304.0	757.0		
Linear Regression Y ON X : Y= mX + b							Average	304.0	757.0		
1	Slope (m)			2.04234	Linear Equation			r ²	0.997850	Pstd(mmHg)	760
2	Intercept (b)			-0.01435	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.9989244	T _{NTP}	298
3	Correlation Coefficient (r)			-0.99993	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)		0.976393698	
Result								C=(Pa/Pstd)*(Tstd/Ta)*0.5		0.988126357	

COMMENT

Andersen Instruments, Inc.

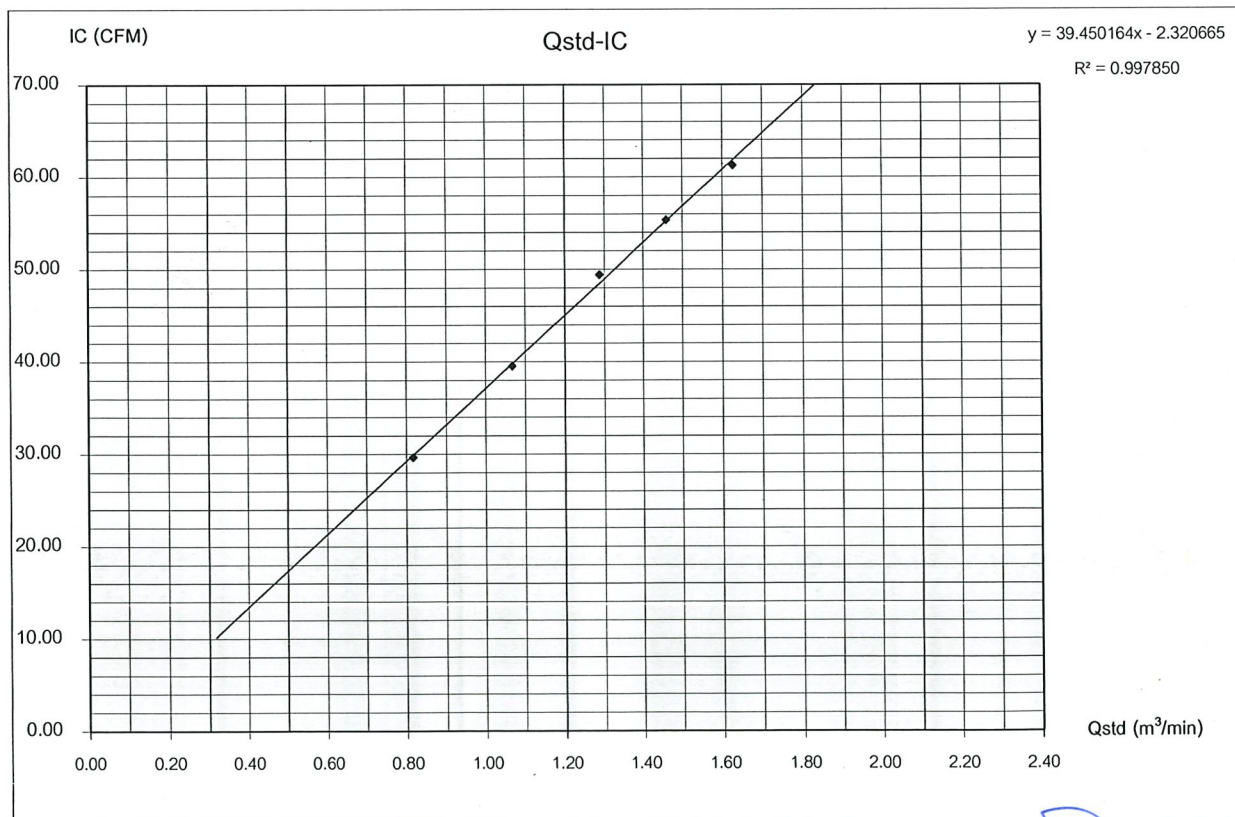

Checked By

(Mr. Prayun Detkla)
Technician

Approved By

(Mr. Panupon Podang)
Environmental Scientist

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	May 22, 2023
วัดมปากอง(2023-00024)				Start Time	1:07 PM
Sampler Number	TSP No.A18	Transfer Standard Type	Orifice	Stop Time	1:17 PM
Instrument Model	HIVOL-BBCBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Nikul Phokamla
Motor Serial Number	2014-03	Calibrator Serial Number	3362		
Recorder Serial Number	7373				


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Positive	Negative	ΔH_2O	$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	ample Flow Rate Indication (ft ³ /min)	$IC = I[(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	(°K = °C+273)	(mmHg)		
5	1.5	1.5	3.0	1.71149	0.84503	29.0	28.66	304.0	757.0		
7	2.4	2.4	4.8	2.16488	1.06702	38.0	37.55	304.0	757.0		
10	3.6	3.6	7.2	2.65142	1.30525	48.0	47.43	304.0	757.0		
13	4.6	4.6	9.2	2.99714	1.47453	56.0	55.34	304.0	757.0		
18	5.6	5.6	11.2	3.30690	1.62620	60.0	59.29	304.0	757.0		

Linear Regression Y ON X : Y= mX + b

1	Slope (m)	2.04234	Linear Equation		Average	304.0	757.0		
2	Intercept (b)	-0.01435	Set Point Flow Rate (X) (m ³ /min)	1.133	r ²	0.996215	Pstd(mmHg)	760.0	
3	Correlation Coefficient (r)	0.99993	Final Set Flow Rate = (I)	0	r	0.9981057	T _{NTP}	298.0	
Result								$C=(Pa/P_{std})(T_{std}/Ta)^{0.5}$	
								0.976393698	
								0.988126357	

COMMENT

Andersen Instruments, Inc.

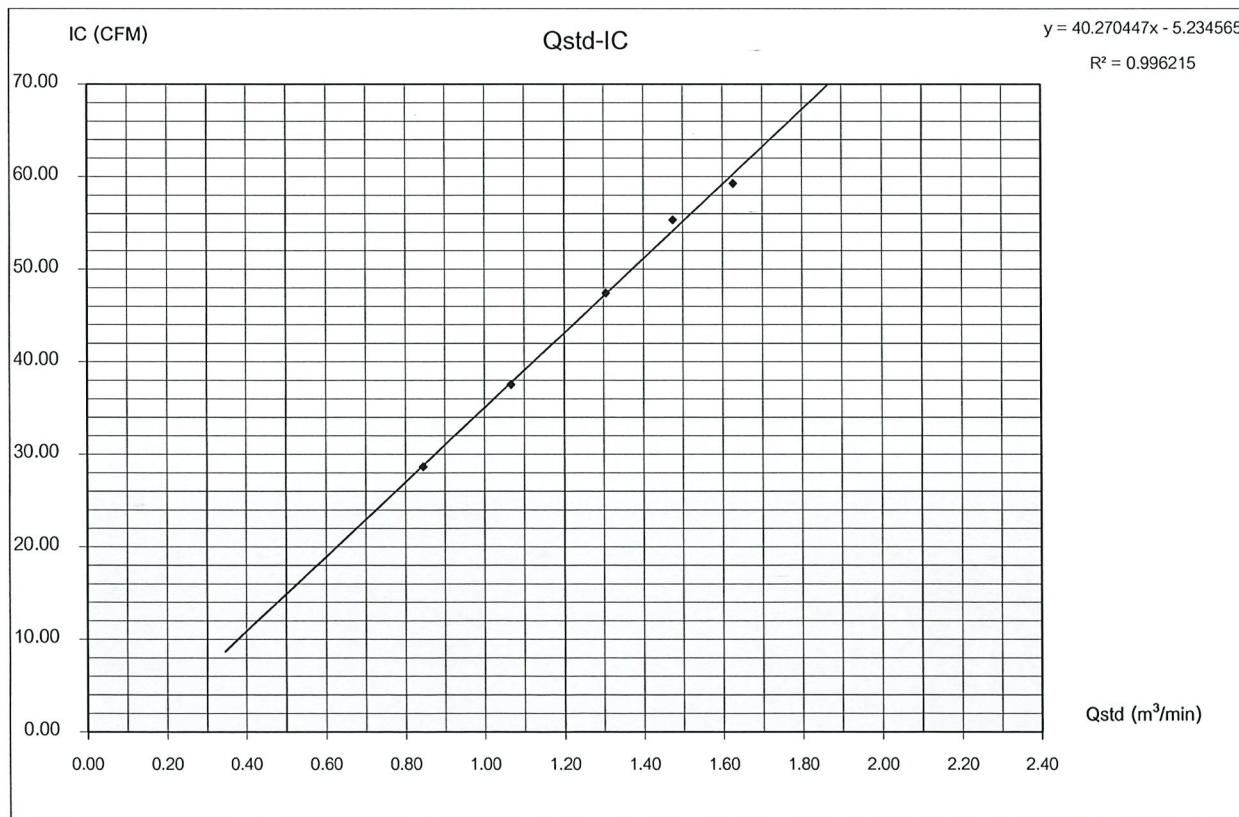

Checked By

(Mr. Prayun Detkla)
Technician



Approved By

(Mr. Panupon Podang)
Environmental Scientist


PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location		Date	
วัดบางคอง(2023-00024)		May 22, 2023	
Sampler Number	PM10 No.9	Transfer Standard Type	Orifice
Instrument Model	HIVOL-BMBBE	Calibrator Model	TE-5025A
Motor Serial Number	2012-5	Calibrator Serial Number	3362
Recorder Serial Number	R0411-003	Calibrated By	
		Mr.Nikul Phokamla	

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric	Start	Stop
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$	ample Flow Rate Indicato	$IC = I[(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	(°K = °C+273)	Pressure (mmHg)	Meter	Meter
	Positive	Negative	ΔH ₂ O		(m ³ /min)	(ft ³ /min)					
5	1.4	1.4	2.8	1.65345	0.81661	30.0	29.64	304.0	757.0		
7	2.4	2.4	4.8	2.16488	1.06702	42.0	41.50	304.0	757.0		
10	3.4	3.4	6.8	2.57672	1.26868	50.0	49.41	304.0	757.0		
13	4.5	4.5	9.0	2.96438	1.45849	56.0	55.34	304.0	757.0		
18	5.5	5.5	11.0	3.27724	1.61168	60.0	59.29	304.0	757.0		
Linear Regression Y ON X : Y= mX + b							Average	304.0	757.0		
1	Slope (m)			2.04234	Linear Equation			r ²	0.986425	Pstd(mmHg)	760.0
2	Intercept (b)			-0.01435	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.9931893	T _{NTP}	298.0
3	Correlation Coefficient (r)			0.99993	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)		0.976393698	
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5		0.988126357	

COMMENT

Andersen Instruments, Inc.

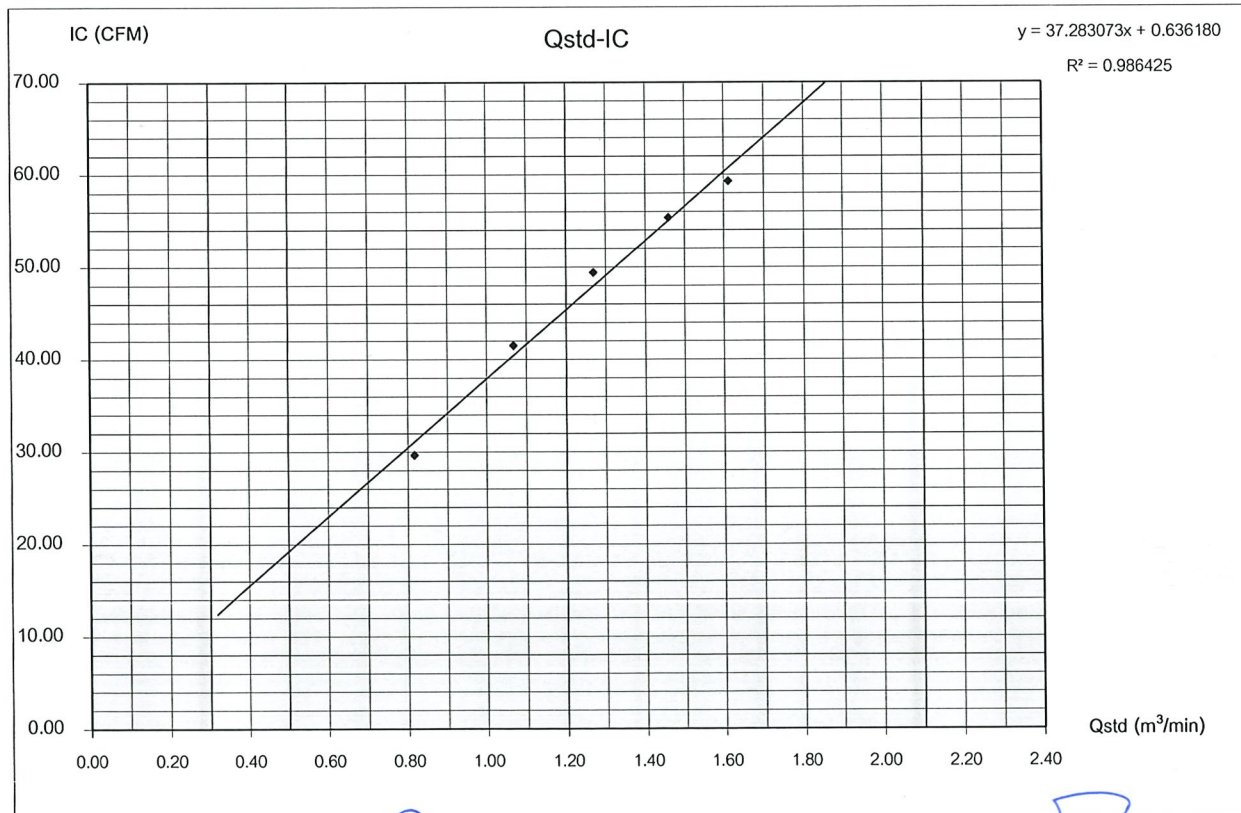

Checked By

(Mr. Prayun Detkla)
Technician



Approved By

(Mr. Panupon Podang)
Environmental Scientist

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT


Sampler Location				Date	May 22, 2023
วัดมวน้ำ(2023-00024)				Start Time	3:02 PM
Sampler Number	TSP No.A10	Transfer Standard Type	Orifice	Stop Time	3:12 PM
Instrument Model	HIVOL-BBCBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Nikul Phokamla
Motor Serial Number	2012-04	Calibrator Serial Number	3362		
Recorder Serial Number	1504				

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$	Sample Flow Rate Indication	$IC = [(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	(°K = °C+273)	(mmHg)		
	Positive	Negative	ΔH_2O		(m ³ /min)	(ft ³ /min)					
5	1.4	1.4	2.8	1.65454	0.81715	30.0	29.66	304.0	758.0		
7	2.4	2.4	4.8	2.16631	1.06772	41.0	40.54	304.0	758.0		
10	3.4	3.4	6.8	2.57842	1.26951	48.0	47.46	304.0	758.0		
13	4.5	4.5	9.0	2.96634	1.45945	55.0	54.38	304.0	758.0		
18	5.5	5.5	11.0	3.27941	1.61274	61.0	60.32	304.0	758.0		
Linear Regression Y ON X : Y= mX + b								Average	304.0	758.0	

Linear Regression Y ON X : Y= mX + b					Average	304.0	758.0		
1	Slope (m)	2.04234	Linear Equation			r^2	0.998209	Pstd(mmHg)	760.0
2	Intercept (b)	-0.01435	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.9991041	T _{NTP}	298.0
3	Correlation Coefficient (r)	0.99993	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)	0.977683518		
Result						C=(Pa/Pstd)*(Tstd/Ta)^0.5		0.988778801	

COMMENT

Andersen Instruments, Inc.

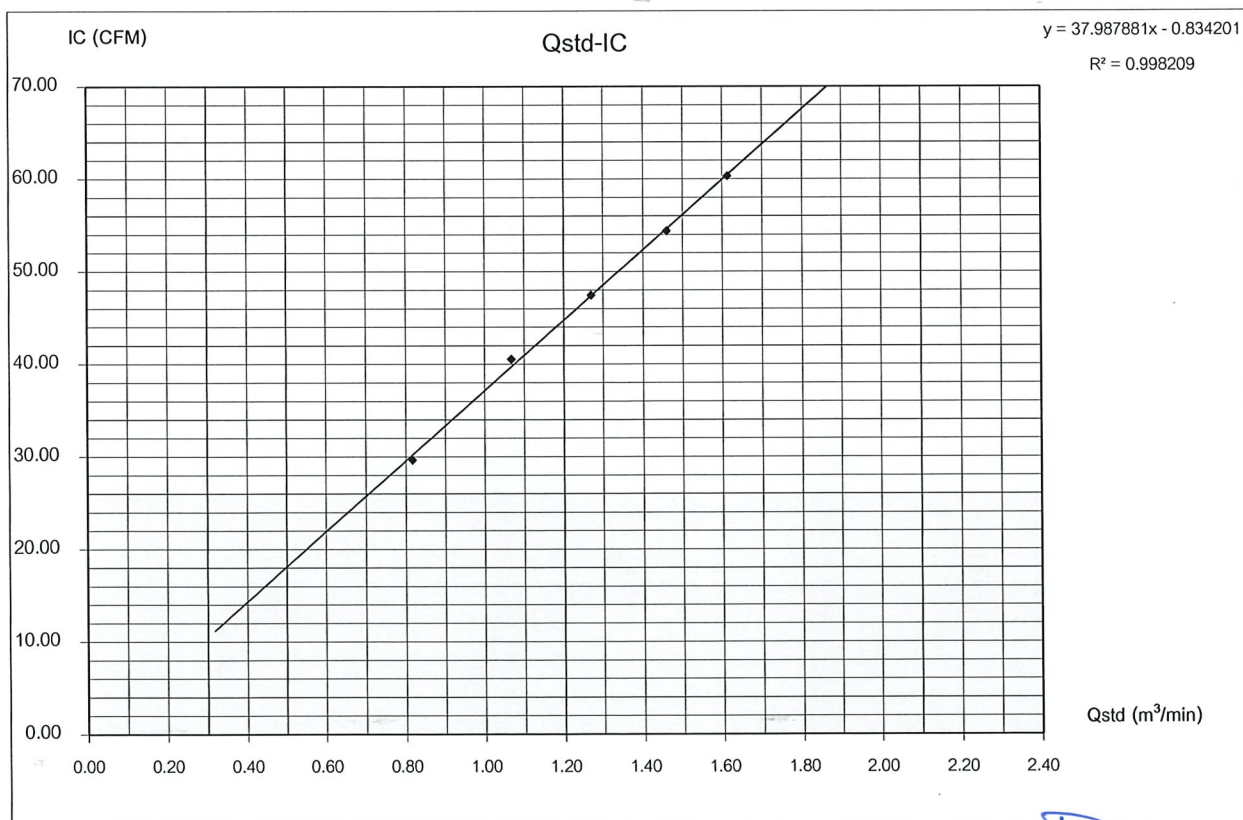

Checked By

Varonrit Tibsag

(Mr. Prayun Detkla)
Technician

Approved By

Panupon Podang

(Mr. Panupon Podang)
Environmental Scientist


PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	May 22, 2023
วัดหน้าป่า(2024-00024)				Start Time	2:51 PM
Sampler Number	PM-10 No.C1	Transfer Standard Type	Orifice	Stop Time	3:01 PM
Instrument Model	HIVOL-BMBBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Nikul Phokamla
Motor Serial Number	PM10No.C1	Calibrator Serial Number	3362		
Recorder Serial Number	-				

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	$Qstd = (1/m)[(A-b)]$	sample Flow Rate Indication	$IC = I[(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	(^°K = ^°C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O		(m ³ /min)	(inch/min)					
5	1.4	1.4	2.8	1.65454	0.81715	1.0	0.99	304.0	758.0		
7	2.3	2.3	4.6	2.12069	1.04539	1.9	1.88	304.0	758.0		
10	3.4	3.4	6.8	2.57842	1.26951	2.6	2.57	304.0	758.0		
13	4.5	4.5	9.0	2.96634	1.45945	3.3	3.26	304.0	758.0		
18	5.6	5.6	11.2	3.30909	1.62727	3.8	3.76	304.0	758.0		
Linear Regression Y ON X : Y= mX + b							Average	304.0	758.0		
1	Slope (m)			2.04234	Linear Equation			r ²	0.998042	Pstd(mmHg)	760.0
2	Intercept (b)			-0.01435	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.9990205	T _{NTP}	298.0
3	Correlation Coefficient (r)			0.99993	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)			0.977683518
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5			0.988778801

COMMENT

Andersen Instruments, Inc.

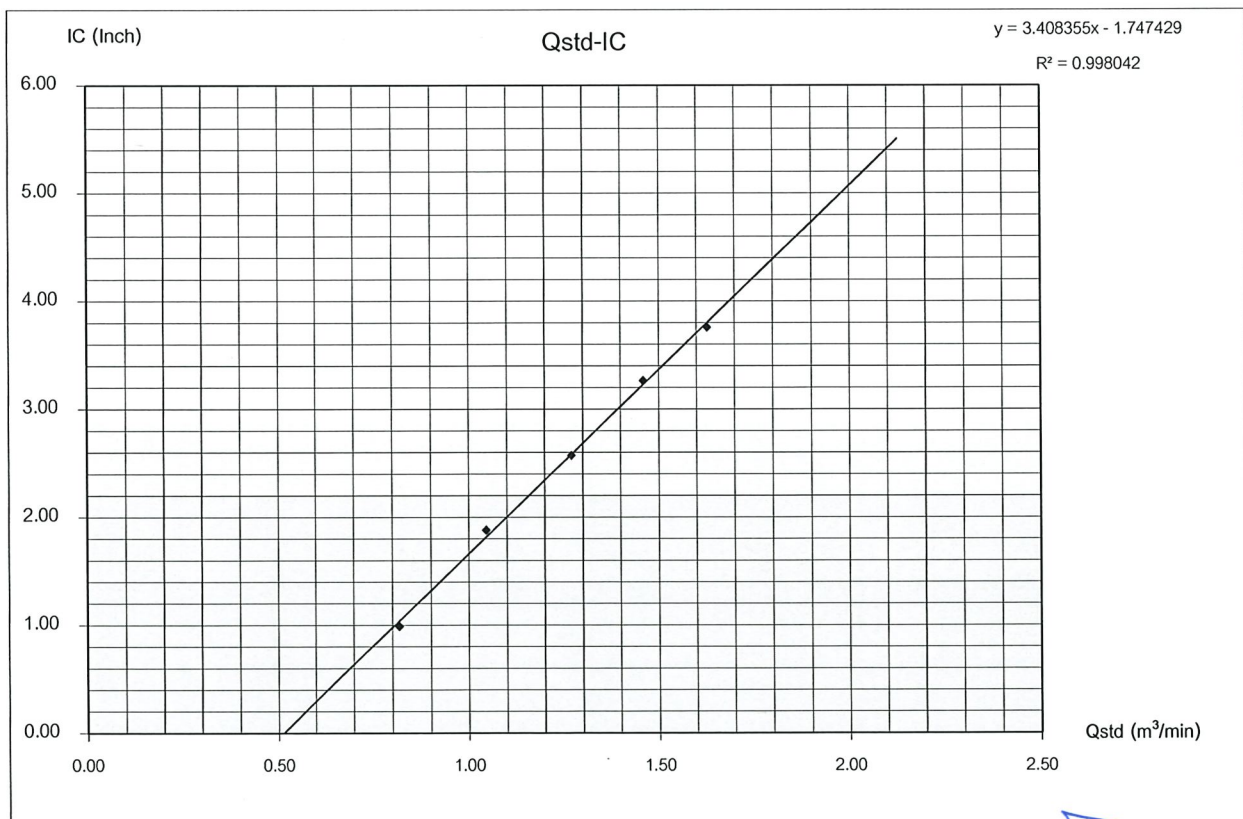

Checked By

Narongrit Tibsa cmm

(Mr. Prayun Detkla)
Technician

Approved By

R

(Mr.Panupon Podang)
Environmental Scientist


TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	May 22, 2023
วัดหนองจิกถนน(2023-00024)				Start Time	2:12 PM
Sampler Number	TSP No.A9	Transfer Standard Type	Orifice	Stop Time	2:22 PM
Instrument Model	HIVOL-BBCBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Nikul Phokamla
Motor Serial Number	A9	Calibrator Serial Number	3362		
Recorder Serial Number	7137				

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	$Qstd = (1/m)[(A-b)]$	ample Flow Rate Indication	$IC = I[(Pa/P_{std})(T_{std}/Ta)]^{1/2}$				
	Positive	Negative	ΔH_2O		(m ³ /min)	(ft ³ /min)		(°K = °C+273)	(mmHg)		
5	1.4	1.4	2.8	1.65183	0.81582	29.0	28.63	305.0	758.0		
7	2.3	2.3	4.6	2.11721	1.04369	40.0	39.49	305.0	758.0		
10	3.3	3.3	6.6	2.53605	1.24876	48.0	47.38	305.0	758.0		
13	4.4	4.4	8.8	2.92838	1.44086	56.0	55.28	305.0	758.0		
18	5.5	5.5	11.0	3.27403	1.61010	62.0	61.20	305.0	758.0		
Linear Regression Y ON X : Y= mX + b							Average	305.0	758.0		
1	Slope (m)			2.04234	Linear Equation			r^2	0.997247	Pstd(mmHg)	760
2	Intercept (b)			-0.01435	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.9986226	T _{NTP}	298
3	Correlation Coefficient (r)			0.99993	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)		0.974477998	
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5		0.987156522	

COMMENT

Andersen Instruments, Inc.

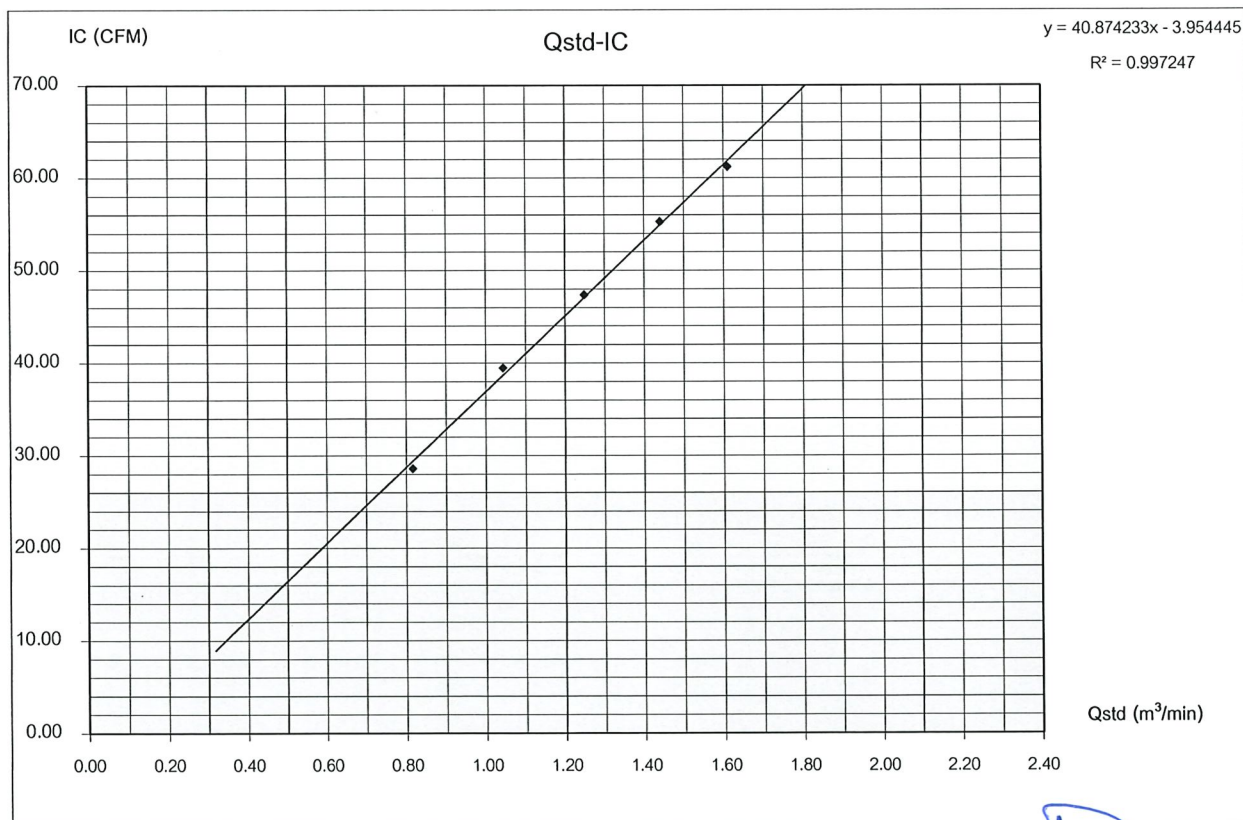

Checked By

Narongrit Tibja am-07

(Mr. Prayun Detkla)
Technician

Approved By

R

(Mr. Panupon Podang)
Environmental Scientist


PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	May 22, 2023
วัดหนองจันทน์(2023-00024)				Start Time	2:02 PM
Sampler Number	PM10 No.29	Transfer Standard Type	Orifice	Stop Time	2:12 PM
Instrument Model	HIVOL-BMBBE	Calibrator Model	TE-5025A	Calibrated By	Mr.Nikul Phokamla
Motor Serial Number	2210	Calibrator Serial Number	3362		
Recorder Serial Number	2614				

Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	Qstd = (1/m)[(A-b)] (m ³ /min)	ample Flow Rate Indicato (ft ³ /min)	IC = I[(Pa/P _{std})(T _{std} /Ta)] ^{1/2}	(*K = °C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O								
5	1.4	1.4	2.8	1.65183	0.81582	30.0	29.61	305.0	758.0		
7	2.4	2.4	4.8	2.16275	1.06598	40.0	39.49	305.0	758.0		
10	3.5	3.5	7.0	2.61177	1.28584	48.0	47.38	305.0	758.0		
13	4.5	4.5	9.0	2.96147	1.45706	56.0	55.28	305.0	758.0		
18	5.6	5.6	11.2	3.30366	1.62461	62.0	61.20	305.0	758.0		
Linear Regression Y ON X : Y= mX + b							Average	305.0	758.0		
1	Slope (m)			2.04234	Linear Equation			r ²	0.998855	Pstd(mmHg)	760.0
2	Intercept (b)			-0.01435	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.9994273	T _{HTP}	298.0
3	Correlation Coefficient (r)			0.99993	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)		0.974477998	
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5		0.987156522	

COMMENT

Andersen Instruments, Inc.

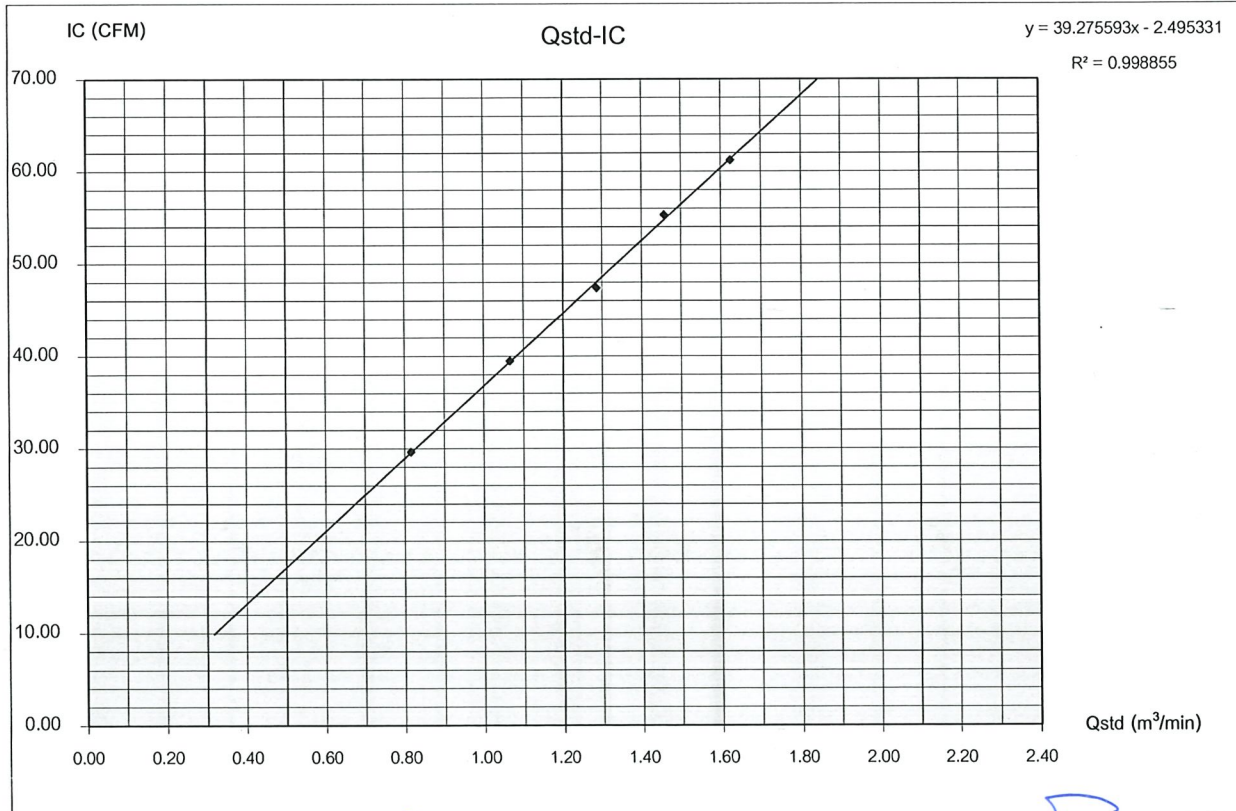

Checked By

(Mr. Prayun Detkla)
Technician



Approved By

(Mr. Panupon Podang)
Environmental Scientist

Certificate of Calibration

Calibration Certification Information			
Cal. Date: January 17, 2023	Rootsmeter S/N: 438320	Ta: 295 °K	
Operator: Jim Tisch		Pa: 740.2 mm Hg	
Calibration Model #: TE-5025A	Calibrator S/N: 3362		

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.4140	3.2	2.00
2	3	4	1	0.9920	6.4	4.00
3	5	6	1	0.8930	8.0	5.00
4	7	8	1	0.8490	8.8	5.50
5	9	10	1	0.7000	12.8	8.00

Data Tabulation					
Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9795	0.6927	1.4027	0.9957	0.7042	0.8928
0.9753	0.9832	1.9837	0.9914	0.9993	1.2626
0.9732	1.0898	2.2179	0.9892	1.1077	1.4117
0.9721	1.1450	2.3261	0.9881	1.1639	1.4806
0.9668	1.3811	2.8054	0.9827	1.4039	1.7856
QSTD	m=	2.04234	QA	m=	1.27888
	b=	-0.01435		b=	-0.00913
	r=	0.99993		r=	0.99993

Calculations	
Vstd= $\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$	Va= $\Delta Vol((Pa-\Delta P)/Pa)$
Qstd= Vstd/ΔTime	Qa= Va/ΔTime
For subsequent flow rate calculations:	
Qstd= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$	Qa= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$

Standard Conditions	
Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH:	calibrator manometer reading (in H2O)
ΔP:	rootsmeter manometer reading (mm Hg)
Ta:	actual absolute temperature (°K)
Pa:	actual barometric pressure (mm Hg)
b:	intercept
m:	slope

RECALIBRATION
US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30

Mettler-Toledo (Thailand) Ltd.
846/4 - 846/5 Lasalle Rd., Bangna Tai Sub-District
Bangna District, Bangkok 10260
+66 2723 0382
MT-TH.ServiceSupport@mt.com



Accuracy Calibration Certificate

Customer

Company: Environment Research & Technology Co., Ltd.
Address: 25/114 Moo 6, Soi Chinaket 1, Ngamwongwan Rd., Toongsonghong
City: Laksi Contact: Ramita Taengthai
Zip / Postal: 10210
State / Province: Bangkok
Order Number:



Weighing Device

Manufacturer: Mettler Toledo Instrument Type: Weighing Instrument
Model: AB204-S Asset Number: ERTC-L-IN-0048
Serial No.: 1123103723 Terminal Model: N/A
Building: N/A Terminal Serial No.: N/A
Floor: 4 Terminal Asset No.: N/A
Room: 406

Range	Max. Capacity	Readability (d)
1	220 g	0.0001 g

Procedure

Calibration Guideline: EURAMET cg-18 v. 4.0 (11/2015)
METTLER TOLEDO Work Instruction: CPW002/20

This calibration certificate contains measurements for As Found and As Left calibrations.

The sensitivity/span of the weighing instrument was adjusted before As Found and As Left calibrations with a built-in weight.

In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

	Temperature		Humidity	
As Found	Start: 23.6 °C	End: 23.5 °C	Start: 34.6 %	End: 35.1 %
As Left	Start: 23.6 °C	End: 23.5 °C	Start: 35.0 %	End: 35.7 %

As Found Calibration Date: 17-Jan-2023
As Left Calibration Date: 17-Jan-2023
Issue Date: 19-Jan-2023
Calibrator: Chawalit Martsuloke
Approved Signatory: Technical Manager / Head of Calibration Center


Measurement Results

Repeatability

Test Load: 100 g

	As Found	As Left
1	99.9992 g	100.0001 g
2	99.9991 g	100.0001 g
3	99.9991 g	100.0001 g
4	99.9991 g	100.0001 g
5	99.9992 g	100.0002 g
6	99.9993 g	100.0002 g
7	99.9992 g	100.0002 g
8	99.9992 g	100.0001 g
9	99.9991 g	100.0001 g
10	99.9992 g	100.0001 g

Standard Deviation	0.00007 g	0.00005 g
--------------------	-----------	-----------

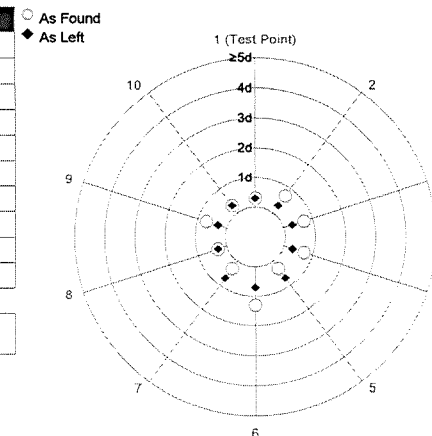

The "d" in the graph represents the readability of the range/interval in which the test was performed.


The results of this graph are based upon the absolute values of the differences from the mean value.

Eccentricity

Test Load: 100 g

Position	As Found	As Left
1	99.9991 g	100.0001 g
2	99.9993 g	100.0002 g
3	99.9992 g	100.0002 g
4	99.9990 g	100.0001 g
5	99.9991 g	100.0001 g

Maximum Deviation	0.0002 g	0.0001 g
-------------------	----------	----------

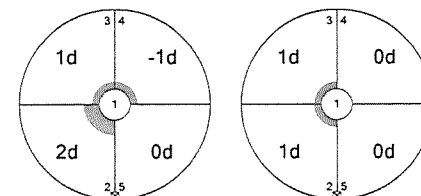

As Found

As Left

The "d" in the graph represents the readability of the range/interval in which the test was performed.


Error of Indication

As Found

	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.0000 g	0.0000 g	0.0000 g	0.15 mg	2
2	0.0500 g	0.0500 g	0.0000 g	0.16 mg	2
3	0.1000 g	0.0999 g	-0.0001 g	0.16 mg	2
4	0.5000 g	0.4999 g	-0.0001 g	0.16 mg	2
5	1.0000 g	1.0000 g	0.0000 g	0.16 mg	2
6	5.0000 g	5.0001 g	0.0001 g	0.16 mg	2
7	10.0000 g	10.0001 g	0.0001 g	0.17 mg	2
8	50.0000 g	49.9997 g	-0.0003 g	0.20 mg	2
9	100.0000 g	99.9992 g	-0.0008 g	0.27 mg	2
10	150.0000 g	149.9987 g	-0.0013 g	0.38 mg	2
11	200.0000 g	199.9982 g	-0.0018 g	0.44 mg	2

As Left

	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.0000 g	0.0000 g	0.0000 g	0.11 mg	2
2	0.0500 g	0.0500 g	0.0000 g	0.13 mg	2
3	0.1000 g	0.1000 g	0.0000 g	0.13 mg	2
4	0.5000 g	0.5000 g	0.0000 g	0.13 mg	2
5	1.0000 g	1.0000 g	0.0000 g	0.13 mg	2
6	5.0000 g	5.0001 g	0.0001 g	0.13 mg	2
7	10.0000 g	10.0000 g	0.0000 g	0.14 mg	2
8	50.0000 g	50.0000 g	0.0000 g	0.17 mg	2
9	100.0000 g	100.0001 g	0.0001 g	0.24 mg	2
10	150.0000 g	150.0001 g	0.0001 g	0.34 mg	2
11	200.0000 g	200.0002 g	0.0002 g	0.39 mg	2

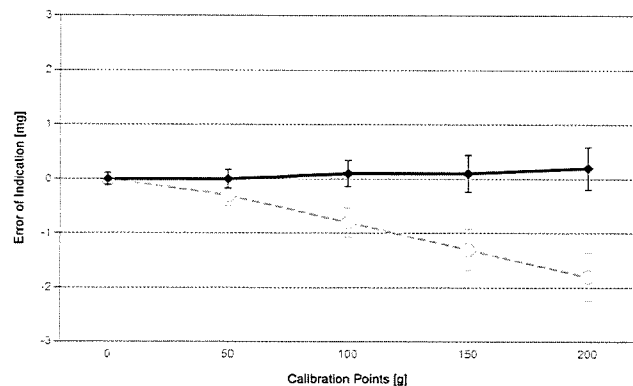

For improved legibility of the graphics only increasing measurement points are shown and measurement points close to zero are not displayed.

The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor k – which can be larger than 2 according to EURAMET cg-18. The value of the measurand lies within the assigned range of values with a probability of approximately 95%.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2

Weight Set No.:	WS57	Date of Issue:	06-Jan-2022
Certificate Number:	177037	Calibration Due Date:	03-Jul-2023

Thermo Hygrometer

Equipment No.:	IN255	Date of Issue:	20-Jul-2022
Certificate Number:	22H1503	Calibration Due Date:	04-Jul-2023

Remarks

Equipment condition: Good
Next calibration according to customer's procedure
Calibration data not decide by calibration laboratory

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with $k=2$ in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use: $3.0 \cdot 10^{-6} / K$

Temperature range on site for the evaluation of the measurement uncertainty in use: $3 K$


Linearization of Uncertainty Equation

Range			As Found	As Left
	d	Max		
1	0.0001 g	220 g	$U_1 = 0.16 \text{ mg} + 0.0147 \text{ mg/g} \cdot R$	$U_1 = 0.13 \text{ mg} + 0.00671 \text{ mg/g} \cdot R$


To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication	As Found		As Left	
0.0220 g	0.16 mg	0.73%	0.13 mg	0.59%
0.2200 g	0.16 mg	0.074%	0.13 mg	0.060%
2.2000 g	0.19 mg	0.0087%	0.14 mg	0.0066%
22.0000 g	0.48 mg	0.0022%	0.28 mg	0.0013%
220.0000 g	3.4 mg	0.0015%	1.6 mg	0.00073%

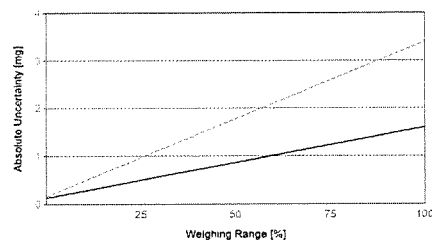

As Found

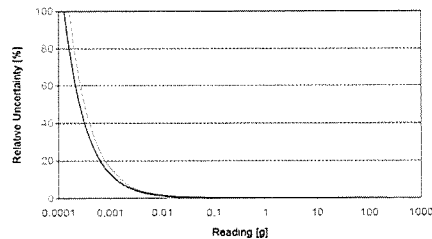

As Left

GWP® Certificate



As
Found



As
Left



The weighing device meets the given
process requirements.


The weighing device meets the given
process requirements.

Tests Performed: ☒ As Found ☒ As Left

Process Requirements

Weighing Tolerance: **1%** | Smallest Net Weight: **0.0500 g** | Safety Factor: **2**

Safe Weighing Range

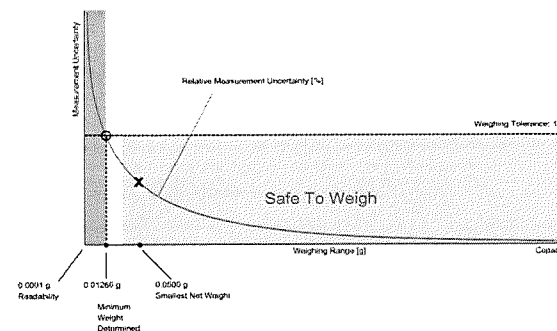

While the values in this graph reflect the actual calibration results, the measurement uncertainty curves are simply a visual representation. This graph reflects As Left testing, unless only As Found was performed.

Minimum Weight

As Found Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.16012 g	0.32511 g	0.49518 g	0.85155 g	1.85026 g
0.2%	0.07947 g	0.16012 g	0.24199 g	0.40949 g	0.85155 g
0.5%	0.03165 g	0.06348 g	0.09550 g	0.16012 g	0.32511 g
1%	0.01580 g	0.03165 g	0.04754 g	0.07947 g	0.16012 g
2%	0.00789 g	0.01580 g	0.02372 g	0.03959 g	0.07947 g
5%	0.00316 g	0.00631 g	0.00947 g	0.01580 g	0.03165 g

✓ Pass: The determined minimum weight meets the requirement for the smallest net weight.

As Left Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.12735 g	0.25642 g	0.38726 g	0.65440 g	1.35584 g
0.2%	0.06346 g	0.12735 g	0.19166 g	0.32162 g	0.65440 g
0.5%	0.02533 g	0.05073 g	0.07620 g	0.12735 g	0.25642 g
1%	0.01266 g	0.02533 g	0.03802 g	0.06346 g	0.12735 g
2%	0.00633 g	0.01266 g	0.01899 g	0.03168 g	0.06346 g
5%	0.00253 g	0.00506 g	0.00759 g	0.01266 g	0.02533 g

✓ Pass: The determined minimum weight meets the requirement for the smallest net weight.

At these net minimum weight values, the measurement uncertainty of the weighing device is equal to or less than 1/1 (no safety factor), 1/2, 1/3, 1/5, or 1/10 of the required tolerance. The values are calculated with $k = 2$ and based on the linear formula of the measurement uncertainty of the weighing device in use.

The safety factor for As Found is always 1. This implies no safety factor. As Found testing looks at the behavior of the instrument from the past until test occurred. For the past, it is necessary to know that the tolerance was met, but not the safety factor. The safety factor is a proactive measure to apply for future measurements.

Notes on minimum weight values in above table:

1. If "N/A" is shown above, no appropriate value could be calculated.
2. METTLER TOLEDO is not responsible for the definition of the process requirements.

Measurement Results

Results Summary

	Repeatability	Eccentricity	Error of Indication
As Found	✓	✓	✓
As Left	✓	✓	✓

✓ = Passed

✗ = Failed

⚠ = Safety Factor not met

Repeatability

Test Load: 100 g

Tolerance	Control Limit	As Found		As Left	
		Std. Deviation	Result	Std. Deviation	Result
0.1%	N/A	0.00007 g*	N/A	0.00005 g*	N/A
0.2%	0.00005 g		✗		⚠
0.5%	0.00013 g		✓		✓
1%	0.00025 g		✓		✓
2%	0.00050 g		✓		✓
5%	0.00125 g		✓		✓

*The calculated standard deviation value is below the rounding error of the balance. The $0.41 \cdot d$ rule is used for the assessment of this repeatability test and the calculation of the minimum weight.

The weighing tolerance is met if the standard deviation is less than or equal to the corresponding control limit.

Eccentricity

Test Load: 100 g

Tolerance	Control Limit	As Found		As Left	
		Deviation	Result	Deviation	Result
0.1%	0.0500 g	0.0002 g	✓	0.0001 g	✓
0.2%	0.1000 g		✓		✓
0.5%	0.2500 g		✓		✓
1%	0.5000 g		✓		✓
2%	1.0000 g		✓		✓
5%	2.5000 g		✓		✓

The weighing tolerance is met if the deviation is less than or equal to the corresponding control limit.

Error of Indication

As Found

		Control limits for various weighing tolerances					
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A
50.0000 g	-0.0003 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g
100.0000 g	-0.0008 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g
150.0000 g	-0.0013 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g
200.0000 g	-0.0018 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓	✓

As Left

		Control limits for various weighing tolerances					
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A
50.0000 g	0.0000 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g
100.0000 g	0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g
150.0000 g	0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g
200.0000 g	0.0002 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g
Result		✓	✓	✓	✓	✓	✓

The weighing tolerance is met if the error (of indication) for each test point is less than or equal to the corresponding control limit for that particular weighing tolerance. Results at or close to the zero point cannot be assessed.



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 14 June, 2022

Certification No. 213/22

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Davis Instruments Inc.

Type : Weather Wizard III Product No. 7425

Serial No. : WE91016A07 ID No. : No.9

Customer : Environment Research & Technology Company Limited.
25/113-114 Moo 6 Soi Chinaket 1, Ngamwongwan Road,
Toongsonghong, Laksi, Bangkok 10210.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1008.8 hPa

NATIONAL STANDARD WIND TUNNEL :

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec


Calibrated by :

Mr. Watcharapol Subwat

Mechanical Engineer

Signed :

Mr. Pisood Promsut

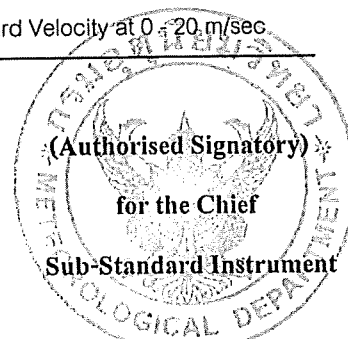



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 213/22

14 June, 2022

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H ₂ O	Vacuum inches H ₂ O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.5	0.50
7.04	-	-	-	6.7	0.34
9.02	-	-	-	8.5	0.52
11.01	-	-	-	10.7	0.31
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.8	0.21
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.8	0.22


Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Watanapong

Mr. Watcharapol Subwat

Mechanical Engineer

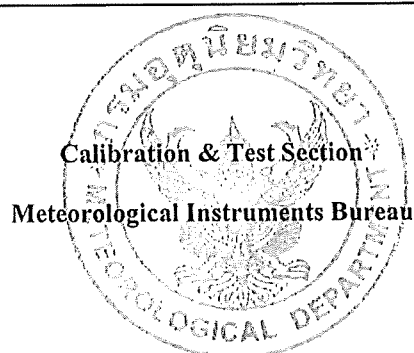



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 14 June, 2022

Certification No. 214/22

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Davis Instruments Inc.

Type : Weather Wizard III Product No. 7425

Serial No. : WC30506A54A ID No. : No.4

Customer : Environment Research & Technology Company Limited.
25/113-114 Moo 6 Soi Chinaket 1, Ngamwongwan Road,
Toongsonghong, Laksi, Bangkok 10210.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1008.5 hPa

NATIONAL STANDARD WIND TUNNEL :

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION

: Standard Velocity at 0 - 20 m/sec


Calibrated by :

Mr. Watcharapol Subwat

Mechanical Engineer

Signed :

Mr. Risood Promsut

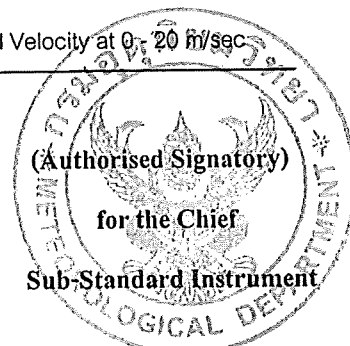



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 214/22

14 June, 2022

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacumm inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.4	0.60
3.02	-	-	-	2.2	0.82
5.00	-	-	-	4.5	0.50
7.04	-	-	-	6.3	0.74
9.02	-	-	-	8.5	0.52
11.01	-	-	-	10.3	0.71
13.01	-	-	-	12.5	0.51
15.01	-	-	-	14.3	0.71
17.02	-	-	-	16.5	0.52
20.02	-	-	-	19.3	0.72


Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Watcharapol Subwat

Mr. Watcharapol Subwat

Mechanical Engineer

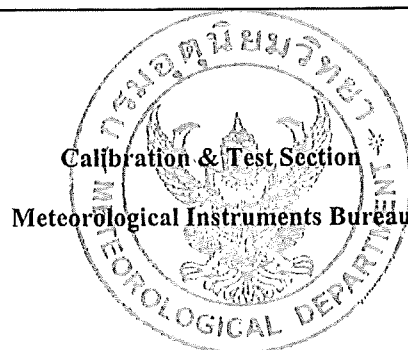



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 20 August, 2022

Certification No. 342/22

Page : 1 of 3

Object : Weather Station

Manufacturer : Davis Instruments Inc.

Type : Vantage Pro2

Serial No. : AS160105025 ID No. : No.24

Customer : Environment Research & Technology Company Limited.
25/113-114 Moo 6 Soi Chinaket 1, Ngamwongwan Road,
Toongsonghong, Laksi, Bangkok 10210.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1007.4 hPa

NATIONAL STANDARD WIND TUNNEL :

: Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: Thermoschneider No.918802

Calibrated by :


Watchapol Subwat

Signed :

Mr. Pisod Promsut

Mr. Watchapol Subwat

Mechanical Engineer

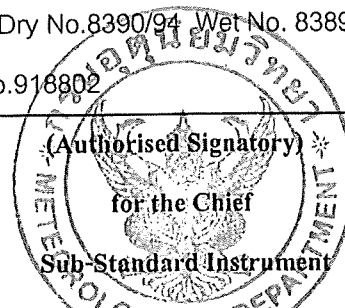



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Certification No. 342/22

20 August, 2022

Page : 2 of 3

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacumm inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.9	0.10
7.00	-	-	-	6.7	0.30
9.02	-	-	-	8.9	0.12
11.01	-	-	-	10.7	0.31
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.8	0.21
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.1	-0.08


Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Watcharapol Subwat

Mr. Watcharapol Subwat

Mechanical Engineer

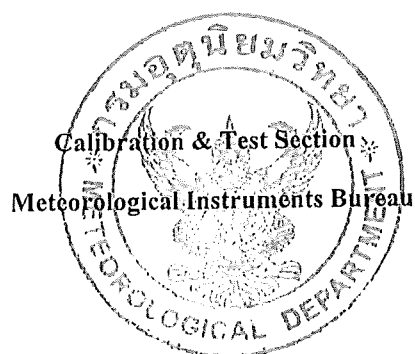



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 342/22


20 August, 2022

Page : 3 of 3

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.1	45.1	0.0
30.2	30.2	0.0
15.4	15.5	-0.1

Calibrated by :

Mr. Watcharapol Subwat
Mechanical Engineer

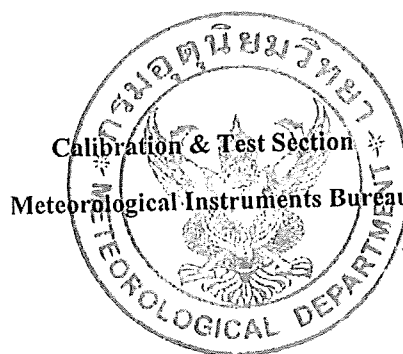



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 20 August, 2022

Certification No. 341/22

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Davis Instruments Inc.

Type : Weather Wizard III Product No. 7425

Serial No. : WC20214A68 ID No. : No.3

Customer : Environment Research & Technology Company Limited.
25/113-114 Moo 6 Soi Chinaket 1, Ngamwongwan Road,
Toongsonghong, Laksi, Bangkok 10210.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1007.8 hPa

NATIONAL STANDARD WIND TUNNEL :

: Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION

: Standard Velocity at 0 - 20 m/sec

Calibrated by :


Watchapol

Signed :

Pisood Promsut

Mr. Watchapol Subwat

Mechanical Engineer

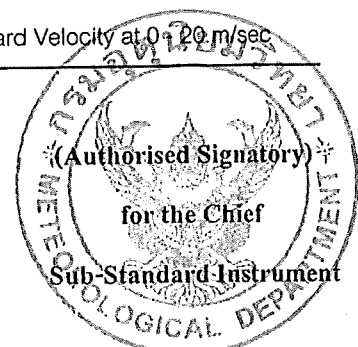



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 341/22

20 August, 2022

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacumm	Velocity	Velocity	Correction
	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	0.4	0.60
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.5	0.50
7.04	-	-	-	6.7	0.34
9.02	-	-	-	8.5	0.52
11.01	-	-	-	10.8	0.21
13.01	-	-	-	12.5	0.51
15.01	-	-	-	14.8	0.21
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.8	0.22


Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

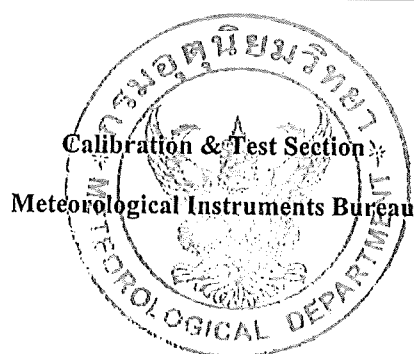

Sound Level Meter Calibration Report

Support Equipment Type : Sound Level Calibrator

Manufacture : BSWA Technology

Model : CA111

Serial No. : 590335

Range of Calibrator

- Sound Pressure Level : 94.0 dB.

- **Frequency** : 1,000 Hz.

Calibrated By : Mr.Suriya Choothong

Calibration Date : May 22, 2023

Customer Name : บริษัท โฟรท์เทียร์ คอนซัลแตนต์ จำกัด : โครงการนิคมอุตสาหกรรม ซีพีจีซี บริษัท ซีจี คอร์ปอเรชั่น จำกัด

[illegible]

Checked By

Mr. Prayun Detkla
Technician

Approved By

Ms.Sutatip Im-noi
Environmental Scientist

Sound Level Meter Calibration Report

Support Equipment Type : Sound Level Calibrator

Manufacture : BSWA Technology

Model : CA111

Serial No. : 590335

Range of Calibrator

- Sound Pressure Level : 94.0 dB.

- **Frequency** : 1,000 Hz.

Calibrated By : Mr.Suriya Choothong

Calibration Date : May 23, 2023

Customer Name : บริษัท โฟรเทียร์ คอนซัลแตนต์ จำกัด : โครงการนิคมอุตสาหกรรม ซีพีจีซี บริษัท ซีจี คอร์เปอเรชั่น จำกัด


[illegible]

Checked By

Prayun

Mr. Prayun Detkla
Technician

Approved By


.....
Ms.Sutatip Im-noi
Environmental Scientist



Calibration Chart

BSWA TECH

BSWA-IV-C021-03-0048A

Sound Calibrator model CA111
Serial Number 590335
Appearance OK
Power Supply 1.5V LR6 (AA battery) x2
Sound Pressure Level 93.97 / 112.98 dB
Frequency 1000.9 / 1000.9 Hz
THD (@1000Hz) 0.51 / 1.31 %

Copying and using select parts, or tampering with this document without the permission of BSWA is forbidden!

BSWA Technology Ltd.

www.bswa-tech.com

This equipment was calibrated at the following ambient conditions:

Temperature: 20 °C
Humidity: 40 %RH
Pressure: 1025 hPa

This equipment is qualified!


Calibrated

2023-3-7
Date



เอกสารการสอบเทียบเครื่องมือตรวจวัด
บริษัท เทสท์ เทค จำกัด

๕1

ใบรับรองการสอบเทียบ “เทอร์โมมิเตอร์”

(Calibration Certificate of Liquid in Glass Thermometer)



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 23T793

Page : 1 of 2

Equipment : Digital Thermometer With Sensor

Manufacturer: Testo

Model : 926

Serial No.: 5609260110250914

ID No.: EQL-058

Condition As-Received: Used Item

Received Date: 07 April 2023

Calibration Date: 18 April 2023
to 08 May 2023

Reference: 2304-0179DN

Ambient Temperature: (25 \pm 3) °C

Relative Humidity: (50 \pm 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

30, 32 Rama II Soi 63, Rama II Rd.,
Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with
Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Black Stack Thermometer	1560	8C454	22I616	23 May 2023
2) PRT Scanner Module	2562	A01303	22I616	23 May 2023
3) Industrial Platinum Resistance Thermometer	5627	739433	22I616	23 May 2023
4) Industrial Platinum Resistance Thermometer	5627	739434	22I616	23 May 2023

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Sitthinon Poomai
Issue Date : 12 May 2023

Approved Signatory :

[] Phalinee Prabpaipal
[] Chatchawan Khunpiluek
[✓] Wanlop Larpkurn

B 0313441



Cert. No.: 23T793

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Temperature measurement

This equipment was connected with Thermocouple Type T

ID No. EQL-058

Immersion	Standard	UUC*		Uncertainty
<u>Depth</u>	<u>Temperature</u>	<u>Reading</u>	<u>Error</u>	<u>of Measurement</u>
(mm.)	(°C)	(°C)	(°C)	(±°C)
150	3.0045	2.9	-0.1045	0.24
150	20.0060	19.9	-0.1060	0.24
150	35.0057	34.8	-0.2057	0.24
150	103.0046	102.6	-0.4046	0.37
150	104.0025	103.6	-0.4025	0.37
150	120.0046	119.7	-0.3046	0.42
150	140.0018	139.7	-0.3018	0.47
150	150.0083	149.7	-0.3083	0.49
150	170.0054	169.5	-0.5054	0.55
150	180.0026	178.9	-1.1026	0.58

Result of Calibration:-

Without Adjustment

Function:

Temperature measurement

This equipment was connected with Thermocouple Type T

ID No. EQL-058 Water Proof

Dimension of probe : Diameter 6 mm., Length 111 mm. Sheath material : Stainless Steel

Immersion	Standard	UUC*		Uncertainty
<u>Depth</u>	<u>Temperature</u>	<u>Reading</u>	<u>Error</u>	<u>of Measurement</u>
(mm.)	(°C)	(°C)	(°C)	(±°C)
100	41.5080	41.3	-0.2080	0.24
100	45.0040	44.8	-0.2040	0.24
100	50.0045	49.8	-0.2045	0.24
100	83.0082	82.7	-0.3082	0.31
100	92.0024	91.7	-0.3024	0.33
100	95.0054	94.7	-0.3054	0.34
100	150.0076	149.4	-0.6076	0.49

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 23T475

Page : 1 of 2

Equipment : Digital Thermometer With Sensor

Manufacturer: Testo

Model : 926

Serial No.: 33824123/004

ID No.: EQL-138

Condition As-Received: Used Item

Received Date: 09 March 2023

Calibration Date: 20 March 2023
to 22 March 2023

Reference: 2303-0314DN

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

30, 32 Rama II Soi 63, Rama II Rd.,
Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with
Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Digital Thermometer	1529	A7A609	2211274	17 Oct 2023
2) Industrial Platinum Resistance Thermometer	5627-12	571970	2211274	17 Oct 2023
3) Industrial Platinum Resistance Thermometer	5627	824304	2211274	17 Oct 2023

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Sataporn Mulkamnee
Issue Date : 23 March 2023

Approved Signatory :

[] Phalinee Prabpaipal
[] Chatchawan Khunpiluek
[✓] Wanlop Larpkurn

B 0310381



Cert. No.: 23T475

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Temperature measurement

This equipment was connected with Thermocouple Type T ID No. EQL-138

Immersion	Standard	UUC*		Uncertainty
Depth	Temperature	Reading	Error	of Measurement
(mm.)	(°C)	(°C)	(°C)	(±°C)
150	2.9962	2.6	-0.3962	0.24
150	35.0051	34.8	-0.2051	0.24
150	36.0061	35.8	-0.2061	0.24
150	36.9974	36.8	-0.1974	0.24
150	41.5051	41.4	-0.1051	0.24
150	43.9973	43.9	-0.0973	0.24
150	55.0047	55.0	-0.0047	0.25
150	169.9960	170.4	0.4040	0.55

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

-o0o-



CERTIFICATE No : 22T8762
REFERENCE No : 66179-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : LIQUID IN GLASS THERMOMETER
MANUFACTURER : PRECISION
MODEL : ---
SERIAL No : 8925
No : EQL-103
RESOLUTION : 0.1 °C
TYPE : TOTAL IMMERSION
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

ALIBRATED BY : CHARUKIT L.
CALIBRATION DATE : 18-Aug-22
APPROVED BY : PONGSAK J.
ISSUED DATE : 18-Aug-22
RECEIVED DATE : 11-Aug-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 22T8762

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : LIQUID IN GLASS THERMOMETER
MANUFACTURER : PRECISION
MODEL : ---
ID No : EQL-103
RESOLUTION : 0.1 °C
RECEIVED DATE : 11-Aug-22
AMBIENT TEMPERATURE : 23 °C ± 3 °C
SERIAL NUMBER : 8925
TYPE : TOTAL IMMERSION
CALIBRATION DATE : 18-Aug-22
RELATIVE HUMIDITY : 50 %RH ± 20 %RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BASED ON ASTM E77:1992 BY COMPARISON WITH STANDARD PLATINUM RESISTANCE THERMOMETER (SPRT) INTO LIQUID BATH TEMPERATURE CONTROLLER. THE TEMPERATURE SCALE USED WAS BASED ON S-90.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD THERMOMETER	1529	A22167	21T12439	09-Dec-22
2) SPRT PROBE	5612	587312	21T12439	09-Dec-22
3) PRECISION BATH	7320	A21105	21T12433	16-Dec-22
4) PRECISION BATH	CTR-40	A68155	21T12434	10-Dec-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND).

RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	EMERGENT STEM TEMPERATURE (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
20.0214	20.0	140	0.0214	N/A	0.079
25.0309	25.0	160	0.0309	N/A	0.079
41.5541	41.5	225	0.0541	N/A	0.079
44.5416	44.5	235	0.0416	N/A	0.079
45.0409	45.0	240	0.0409	N/A	0.079
50.0520	50.0	260	0.0520	N/A	0.084

UUC* : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 22H2197

Page : 1 of 2

Equipment : Dial Thermo-Hygrometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: EQL-064

Condition As-Received: Used Item

Received Date: 17 October 2022

Calibration Date: 25 October 2022
to 28 October 2022

Reference: 2210-0461DN

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

30, 32 Rama II Soi 63, Rama II Rd.,
Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Chilled-Mirror Hygrometer	Dew Master	41292	19848	03 Nov 2022
2) Handheld Thermometer With Sensor	1523	3240076	22I249	02 Mar 2023

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained at:-

- National Institute of Standards and Technology (NIST) , The United States of America
- National Institute of Metrology Thailand (NIMT)

Calibrated by : Surasit Phansudnoi
Issue Date : 01 November 2022

Approved Signatory : _____

☒ Chakrit Waewanjua

☐ Pornthippa Tameyakul

☐ Viporn Tantiyawutti



Cert. No.: 22H2197

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Humidity measurement.

<u>Reference</u> <u>Temperature</u> (°C)	<u>Standard</u> <u>Humidity</u> (%R.H.)	<u>UUC*</u> <u>Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty</u> <u>of Measurement</u> (±%R.H.)
25.0	30.1	29.0	-1.1	1.5
25.0	40.1	39.0	-1.1	1.5
25.0	50.1	50.0	-0.1	1.7
25.0	60.0	61.0	1.0	1.7
25.0	75.2	76.5	1.3	1.7

Result of Calibration:-

Without Adjustment

Function:

Temperature measurement.

<u>Standard</u> <u>Temperature</u> (°C)	<u>UUC*</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> <u>of Measurement</u> (±°C)
15.013	15.0	-0.013	0.72
20.023	20.0	-0.023	0.72
25.019	25.0	-0.019	0.72
30.009	30.0	-0.009	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-o0o-

a 1133179

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 22T8761

REFERENCE No : 66179-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : LIQUID IN GLASS THERMOMETER

MANUFACTURER : PRECISION

MODEL : G13004

SERIAL No : N/A

No : EQL-111

RESOLUTION : 1 °C

TYPE : TOTAL IMMERSION

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

LIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 18-Aug-22

APPROVED BY : PONGSAK J.

ISSUED DATE : 18-Aug-22

RECEIVED DATE : 11-Aug-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 22T8761

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : LIQUID IN GLASS THERMOMETER
MANUFACTURER : PRECISION
MODEL : G13004
ID No : EQL-111
RESOLUTION : 1 °C
RECEIVED DATE : 11-Aug-22
AMBIENT TEMPERATURE : 23 °C ± 3 °C
SERIAL NUMBER : N/A
TYPE : TOTAL IMMERSION
CALIBRATION DATE : 18-Aug-22
RELATIVE HUMIDITY : 50 %RH ± 20 %RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BASED ON ASTM E77:1992 BY COMPARISON WITH STANDARD PLATINUM RESISTANCE THERMOMETER (SPRT) INTO LIQUID BATH TEMPERATURE CONTROLLER. THE TEMPERATURE SCALE USED WAS BASED ON ITS -90.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD THERMOMETER	1529	A22167	21T12439	09-Dec-22
2) SPRT PROBE	5612	587312	21T12439	09-Dec-22
3) PRECISION BATH	7320	A21105	21T12433	16-Dec-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND).

RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	EMERGENT STEM TEMPERATURE (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
115.0063	115.0	110	0.0063	N/A	0.15
121.0191	121.0	120	0.0191	N/A	0.15

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

ซ2

ใบรับรองการสอบเทียบ “เครื่องวัดความนำไฟฟ้า”
(Calibration Certificate of Conductivity Meter)



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 23CH92

Page.: 1 of 3

Certificate of Calibration

Equipment :	Conductivity Meter
Manufacturer :	TOA
Model :	CM-41X
Serial No. :	842572
ID No. :	EQL-211
Condition As-Received:	Used Item
Received Date :	19 January 2023
Calibration Date :	20 January 2023
Reference :	2301-0614DN-1
Submitted by :	TEST TECH CO.,LTD. (HEAD Office) 30, 32 Rama II Soi 63, Rama II Rd., Samaedam, Bangkhunthian, Bangkok 10150
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure:	In -house method : - CP-CH6 by direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer
Calibrated by :	Warakorn Lerngagtrakul

Approved by :

Approved Signatory

- (/) Malee Butkruea
() Saithip Meangmai
() Warakorn Lerngagtrakul

Issue Date :

24 January 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0049391



Cert.No.: 23CH92

Page.: 2 of 3

Condition of this result of calibration

1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	1963878	130RC095	22I1140	12 Sep 2023
2) Ref. Std. Thermometer	4982054	110RC044	22I1306	27 Oct 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
147.0 $\mu\text{S/cm}$	CPA Chem	823327	20 June 2023
1.413 mS/cm	CPA Chem	823328	20 June 2023
12.880 mS/cm	CPA Chem	823329	20 June 2023

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results**Function : Conductivity Measurement**(*) After Adjustment at 147.0, 1413.0, 12880 $\mu\text{S/cm}$

Conductivity Electrode Serial No.: 806F0005

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (\pm)	Coverage factor k
147.0 $\mu\text{S/cm}$	150.3 $\mu\text{S/cm}$	147.0 $\mu\text{S/cm}$	0.99 $\mu\text{S/cm}$	2.00
1.413 mS/cm	1.428 mS/cm	1.413 mS/cm	0.0092 mS/cm	2.00
12.880 mS/cm	12.71 mS/cm	12.88 mS/cm	0.086 mS/cm	2.00

Remark

- UUC* = Unit Under Calibration

- 147.0 $\mu\text{S/cm}$ Adjustment Cell constant = 98.5m^{-1} - 1.413 mS/cm Adjustment Cell constant = 99.5m^{-1} - 12.880 mS/cm Adjustment Cell constant = 101.8m^{-1}

Malu

a 1144880



Cert.No.: 23CH92

Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : CT-58101B
- Serial No. : 806F0005

Dimension of probe;

- Length : 114 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor <i>k</i>
25.0	25.003	25.0	-0.003	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.

ซ3

ใบรับรองการสอบเทียบ “ตุ้มน้ำหนักมาตรฐาน”
(Calibration Certificate of Standard Weights)



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 23M259

Page : 1 of 2

Equipment : Standard Weight

Manufacturer: LS

Model : -

Serial No.: -

ID No.: EQL-121

Condition As-Received: Used Item

Received Date: 02 February 2023

Calibration Date: 07 February 2023

Reference: 2302-0080DN

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1008.9 mbar

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

30, 32 Rama II Soi 63, Rama II Rd.,
Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-M01 according to comparison method against standard weights on the basis of weighings at an average air density of 1.2 kg/m³ and a temperature of 23.4 °C material density of weight is 8000 kg/m³.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard weight Set (E2)	YCS31-712-00	50202965	MM-0109-22	11 Jul 2024

2.This certificate is not certified for any commercial transaction.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Chaowalit Rittirak
Issue Date : 08 February 2023

Approved Signatory :

[] Phalinee Prabpaipal

[x] Sura Suwannasri

[] Chaowalit Rittirak



Cert No.: 23M259

Page: 2 of 2

Result of calibration

Without adjustment

Nominal Value	Conventional mass	Uncertainty of Measurement (\pm)	Maximum Permissible error (\pm)
50 g	50.00015 g	0.10 mg	0.30 mg

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 23M260

Page : 1 of 2

Equipment : Standard Weight

Manufacturer: -

Model : -

Serial No.: -

ID No.: EQL-258

Condition As-Received: Used Item

Received Date: 02 February 2023

Calibration Date: 07 February 2023

Reference: 2302-0080DN

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1012 mbar

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

30, 32 Rama II Soi 63, Rama II Rd.,
Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-M01 according to comparison method against standard weights on the basis of weighings at an average air density of 1.2 kg/m³ and a temperature of 23.6 °C material density of weight is 8000 kg/m³.

Condition of this result of calibration

1. Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard weight Set (E2)	YCS31-712-00	50202965	MM-0109-22	11 Jul 2024

2. This certificate is not certified for any commercial transaction.

3. The certificate is valid only to the item calibrated on date and place of calibration.

4. This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Chaowalit Rittirak
Issue Date : 08 February 2023

Approved Signatory :


[] Phalinee Prabpaipal

☒ Sura Suwannasri

[] Chaowalit Rittirak

B 0307756



Cert No.: 23M260

Page: 2 of 2

Result of calibration

Without adjustment

Nominal Value	Conventional mass	Uncertainty of Measurement (\pm)	Maximum Permissible error (\pm)
2 kg	2.0000034 kg	3.0 mg	10 mg

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-

a 1146232



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 22M1563

Page : 1 of 2

Equipment : Standard Weight

Manufacturer: -

Model : -

Serial No.: M 0030/11

ID No.: EQL-139

Condition As-Received: Used Item

Received Date: 11 August 2022

Calibration Date: 24 August 2022

Reference: 2208-0438DN

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

Ambient Temperature: (23 \pm 2) °C

Relative Humidity: (50 \pm 15) %

Atmospheric Pressure: 1008 mbar

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

30, 32 Rama II Soi 63, Rama II Rd.,
Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-M01 according to comparison method against standard weights on the basis of weighings at an average air density of 1.2 kg/m³ and a temperature of 23.0 °C material density of weight is 8000 kg/m³.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard weight Set (E2)	YCS31-712-00	50202965	MM-0109-22	11 Jul 2024

2.This certificate is not certified for any commercial transaction.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Chaowalit Rittirak

Issue Date : 25 August 2022

Approved Signatory :

[] Phalinee Prabpaipal

[x] Sura Suwannasri

[] Chaowalit Rittirak

B 0295804



Cert No.: 22M1563

Page: 2 of 2

Result of calibration

Without adjustment

Nominal Value	Conventional mass	Uncertainty of Measurement (\pm)	Maximum Permissible error (\pm)
2 g	2.000020 g	0.040 mg	0.12 mg

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-

a 1122451



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 22M1562

Page : 1 of 2

Equipment : Standard Weight

Manufacturer: Mettler Toledo

Model : -

Serial No.: 11119459

ID No.: EQL-149

Condition As-Received: Used Item

Received Date: 11 August 2022

Calibration Date: 24 August 2022

Reference: 2208-0438DN

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

Ambient Temperature: (23 \pm 2) °C

Relative Humidity: (50 \pm 15) %

Atmospheric Pressure: 1008 mbar

30, 32 Rama II Soi 63, Rama II Rd.,
Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-M01 according to comparison method against standard weights on the basis of weighings at an average air density of 1.2 kg/m³ and a temperature of 23.0 °C material density of weight is 8000 kg/m³.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard weight Set (E2)	YCS31-712-00	50202965	MM-0109-22	11 Jul 2024

2.This certificate is not certified for any commercial transaction.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Chaowalit Rittirak

Issue Date : 25 August 2022

Approved Signatory : _____

☐ Phalinee Prabpaipal

☒ Sura Suwannasri

☐ Chaowalit Rittirak

B 0295803



Cert No.: 22M1562

Page: 2 of 2

Result of calibration

Without adjustment

Nominal Value	Conventional mass	Uncertainty of Measurement (\pm)	Maximum Permissible error (\pm)
20 g	20.000011 g	0.080 mg	0.25 mg

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-

a 1122452

๕๔

ใบรับรองการสอบเทียบ “เครื่องวัดความขุ่น”

(Calibration Certificate of Turbidimeter)

Certificate of Calibration

Equipment:	TURBIDIMETER	Certificate No.:	C08220157
Model:	2100N	Issued Date:	21 September 2022
Serial No. (or ID.):	970400003415 (EQL-024)	Job No.:	KSPR2211615
Manufacturer:	HACH	Page:	1 of 2
Condition:	In Condition		

Customer: TEST TECH CO., LTD.
30,32 Rama II Soi 63, Rama II Rd.,
Samaedam, Bangkhuntien Bangkok 10150 Thailand

Environment Condition: Temperature 23 °C ± 2 °C
Humidity 50 %RH ± 15 %RH

Calibration Place: Environment Laboratory, DKSH Technology Limited.
1194 Soi Wachirathamsathit 57, Sukhumvit 101/1 Rd.,
Bangchak, Prakhnong, Bangkok 10260 Thailand

Calibration By: Mr. Wasan Nuchnabee

Calibration Date: 21 September 2022

The Method used: In house method, CAL-WI-23, base on Hach Manufacturer Method 8195

Traceability: This certificate is traceable to Primary standard Fromazin and StablCal accepted by United States Environmental Protection Agency (EPA) through Hach Company
Certificate No. A1075 , A1074 , A1091 , A1074 , A1074



(Mr. Wasan Nuchnabee)

Person in charge



(Mr. Thalemgkeat Pounngam)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

Calibration Results:**Before Adjustment**

Std Turbidity (NTU)	UUC Reading	Correction	Deviation	Uncertainty
0.060	0.048	0.012	0.0004	0.070
20.40	20.1	0.30	0.05	1.0
206.0	204	2.0	0.5	10
1020.0	1013	7.0	1.2	50
4065.0	3875	190.0	1.8	200

After Adjustment

Std Turbidity (NTU)	UUC Reading	Correction	Deviation	Uncertainty
0.060	0.057	0.003	0.0015	0.070
20.40	20.5	-0.10	0.04	1.0
206.0	206	0.0	0.5	10
1020.0	1018	2.0	0.5	50
4065.0	4064	1.0	0.5	200

The End of Certificate

๕5

ใบรับรองการสอบเทียบ “เครื่องวัด pH”
(Calibration Certificate of pH Meter)



CERTIFICATE No : 23E0843
REFERENCE No : 67999-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : DKK-TOA
MODEL : HM-25R
SERIAL No : 760205
ID No : EQL-183
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT P.

CALIBRATION DATE : 27-Jan-23

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 03-Jan-23

RECEIVED DATE : 27-Jan-23



CERTIFICATE No : 23E0843

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : DKK-TOA
ID No : EQL-183
RECEIVED DATE : 27-Jan-23
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : HM-25R
SERIAL NUMBER : 760205
CALIBRATION DATE : 27-Jan-23
RELATIVE HUMIDITY : 51 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER SOLUTION.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No/ LOT No	CERTIFICATE No	DUE DATE
1) pH STANDARD SOLUTION	00651-06	CC719181	4880-12119147	05-Apr-23
2) pH STANDARD SOLUTION	00651-08	CC718727	4881-12110709	31-Mar-23
3) pH STANDARD SOLUTION	00651-10	CC717045	4882-12065386	17-Mar-23
4) PROCESS CALIBRATOR	CA150	91S6079	22E1145	31-Mar-23
5) BATH	260014	1247.48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
 - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

1. DISPLAY UNIT WITH pH ELECTRODE S/N: 202F0138MK

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	ACTUAL READING (mV)	UNCERTAINTY OF MEASUREMENT (± pH)	COVERAGE FACTOR k
4.007	4.01	-0.003	178	0.013	2.0
7.004	7.00	0.004	0.0	0.013	2.0
10.014	10.01	0.004	-177	0.014	2.0

2. DISPLAY UNIT MEASUREMENT TEMPERATURE WITH PROBE

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
25.002	25.0	80	0.002	0.21

3. PERCENT SLOPE 98%

UUC : UNIT UNDER CALIBRATION

THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 21E11277
REFERENCE No : 63049-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : TOA DKK
MODEL : HM-41X
SERIAL No : 784787
ID No : EQL-199
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT P.
CALIBRATION DATE : 15-Oct-21

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 15-Oct-21

RECEIVED DATE : 15-Oct-21

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 21E11277

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : TOA DKK
ID No : EQL-199
RECEIVED DATE : 15-Oct-21
AMBIENT TEMPERATURE : 25° C ± 1° C
MODEL : HM-41X
SERIAL NUMBER : 784787
CALIBRATION DATE : 15-Oct-21
RELATIVE HUMIDITY : 51 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER SOLUTION.
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/</u> <u>LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-06	CC719181	4880-12119147	05-Apr-23
2) pH STANDARD SOLUTION	00651-08	CC718727	4881-12110709	31-Mar-23
3) pH STANDARD SOLUTION	00651-10	CC717045	4882-12065386	17-Mar-23
4) PROCESS CALIBRATOR	744	7514008	21E1392	29-Apr-22
5) BATH	260014	1247 48074	21T9121	10-Sep-22
6) THERMOMETER WITH PROBE	421504	55000379	21T9129	14-Sep-22
7) STANDARD THERMOMETER	2560	A14546	PSL-T0049/64	23-Nov-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
 - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : ADJUSTMENT**1. DISPLAY UNIT WITH pH ELECTRODE S/N: 903F0008MK**

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	ACTUAL READING (mV)	UNCERTAINTY OF MEASUREMENT (± pH)	COVERAGE FACTOR k
4.007	4.01	-0.003	177	0.013	2.00
7.003	7.00	0.003	0	0.013	2.00
10.014	10.01	0.004	-177	0.014	2.00

2. DISPLAY UNIT MEASUREMENT TEMPERATURE WITH PROBE

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
25.008	25.0	80	0.008	0.21

UUC : UNIT UNDER CALIBRATION

THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

ซ6

ใบรับรองการสอบเทียบ “เครื่องวัดอุณหภูมิ-ความชื้นสัมพัทธ์”
(Calibration Certificate of Thermo - Hygrometer)



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 22H2197

Page : 1 of 2

Equipment : Dial Thermo-Hygrometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: EQL-064

Condition As-Received: Used Item

Received Date: 17 October 2022

Calibration Date: 25 October 2022
to 28 October 2022

Reference: 2210-0461DN

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

30, 32 Rama II Soi 63, Rama II Rd.,
Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Chilled-Mirror Hygrometer	Dew Master	41292	19848	03 Nov 2022
2) Handheld Thermometer With Sensor	1523	3240076	221249	02 Mar 2023

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained at:-

- National Institute of Standards and Technology (NIST) , The United States of America
- National Institute of Metrology Thailand (NIMT)

Calibrated by : Surasit Phansudnoi
Issue Date : 01 November 2022

Approved Signatory :


[✓] Chakrit Waewanjua

[] Pornthippa Tameyakul

[] Viporn Tantiyawutti



Cert. No.: 22H2197

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Humidity measurement.

Reference Temperature	Standard Humidity	UUC* Reading	Error	Uncertainty of Measurement
(°C)	(%R.H.)	(%R.H.)	(%R.H.)	(±%R.H.)
25.0	30.1	29.0	-1.1	1.5
25.0	40.1	39.0	-1.1	1.5
25.0	50.1	50.0	-0.1	1.7
25.0	60.0	61.0	1.0	1.7
25.0	75.2	76.5	1.3	1.7

Result of Calibration:-

Without Adjustment

Function:

Temperature measurement.

Standard Temperature	UUC* Reading	Error	Uncertainty of Measurement
(°C)	(°C)	(°C)	(±°C)
15.013	15.0	-0.013	0.72
20.023	20.0	-0.023	0.72
25.019	25.0	-0.019	0.72
30.009	30.0	-0.009	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-o0o-

๗7

ใบรับรองการสอบเทียบ “ตู้อบ”
(Calibration Certificate of Oven)



CERTIFICATE No : 22T9917
REFERENCE No : 66549-4

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : HOT AIR OVEN,
MANUFACTURER : MEMMERT
MODEL : UFE 500
SERIAL No : G508.0791
ID No : EQL-128
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 15-Sep-22

APPROVED BY : PONGSAK J.

ISSUED DATE : 21-Sep-22

RECEIVED DATE : 15-Sep-22



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22T9917

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : MEMMERT
MODEL : UFE 500
ID No : EQL-128
RECEIVED DATE : 15-Sep-22
AMBIENT TEMPERATURE : 25 °C ± 1 °C

S/N : G508.0791
CALIBRATION DATE : 15-Sep-22
RELATIVE HUMIDITY : 51 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	6635300	22T7509	10-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

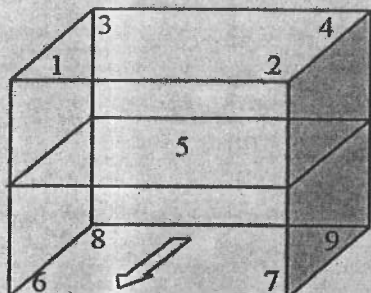

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 3
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

CHAMBER PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.32	0.15	0.62	1.02
180.0	180.09	0.29	1.23	1.86

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.23	103.89	104.54	104.02	104.33	104.63	104.42	104.48	104.39	0.38
180.0	180.0	180.16	179.13	180.46	179.35	179.79	180.66	180.36	180.29	180.61	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 22T9919

REFERENCE No : 66549-6

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : HOT AIR OVEN

MANUFACTURER : MEMMERT

MODEL : UF 110

SERIAL No : B414.0764

ID No : EQL-169

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 15-Sep-22

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 21-Sep-22

RECEIVED DATE : 15-Sep-22



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22T9919

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : MEMMERT
MODEL : UF 110
ID No : EQL-169
RECEIVED DATE : 15-Sep-22
AMBIENT TEMPERATURE : 25 °C ± 1 °C

S/N : B414.0764
CALIBRATION DATE : 15-Sep-22
RELATIVE HUMIDITY : 51 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	22T7508	10-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

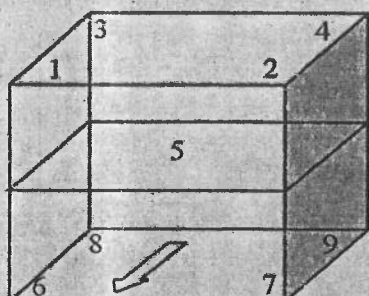

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 2
Overall Line Voltage (V) variation : 4
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

CHAMBER PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.04	0.25	0.51	0.79
180.0	179.85	0.40	1.56	2.23

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.32	103.97	104.32	104.09	103.95	103.81	104.07	103.87	103.97	0.38
180.0	180.0	180.27	179.84	180.63	179.72	179.53	179.28	180.77	179.46	179.18	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



PAGE : 1 OF 2

CERTIFICATE No : 22T9918

REFERENCE No : 66549-5

Certificate of Calibration

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : MEMMERT
MODEL : UFE 500
SERIAL No : G512.2005
ID No : EQL-161
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 15-Sep-22

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 21-Sep-22

RECEIVED DATE : 15-Sep-22



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22T9918

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : MEMMERT
MODEL : UFE 500
ID No : EQL-161 S/N : G512.2005
RECEIVED DATE : 15-Sep-22 CALIBRATION DATE : 15-Sep-22
AMBIENT TEMPERATURE : 25 °C ± 1 °C RELATIVE HUMIDITY : 51 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	22T7508	10-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

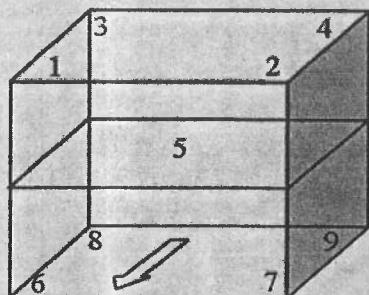

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 8
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

CHAMBER PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	103.98	0.12	0.91	1.00
120.0	119.98	0.13	1.06	1.13
140.0	140.09	0.13	1.35	1.39
150.0	150.03	0.14	1.38	1.49

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.07	104.09	104.21	103.93	103.58	103.79	103.99	103.78	104.36	0.38
120.0	120.0	120.03	120.13	120.34	119.94	119.53	119.69	119.94	119.71	120.48	0.38
140.5	140.5	140.15	140.30	140.44	140.10	139.56	139.74	140.03	139.80	140.72	0.46
150.5	150.5	150.04	150.25	150.54	150.35	149.46	149.55	149.83	149.60	150.67	0.46

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

ใบรับรองการสอบเทียบ “เครื่องชั่ง”

(Calibration Certificate of Electronic Balance)



CERTIFICATE No : 22M9915
REFERENCE No : 66549-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SARTORIUS
MODEL : BP210S
SERIAL No : S0736477
ID No : EQL-008
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD.,
SAMAEDAM, BANGKHUNTHIAN, BANGKOK
10150

CALIBRATED BY : PRASERT P.

CALIBRATION DATE : 15-Sep-22

APPROVED BY : PONGSAK J.

ISSUED DATE : 21-Sep-22

RECEIVED DATE : 15-Sep-22



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 22M9915

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BP210S
MANUFACTURER : SARTORIUS S/N : S0736477
ID No : EQL-008 RECEIVED DATE : 15-Sep-22
AIR PRESSURE : 1011mbar \pm 1mbar CALIBRATION DATE : 15-Sep-22
AMBIENT TEMPERATURE : 21°C \pm 1°C RELATIVE HUMIDITY : 51 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING INTERNAL WEIGHT TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN. THE INTERNAL WEIGHT WAS CHECKED BY USING

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23
2) STANDARD WEIGHT	E2	15843	C02210419	10-Feb-23
3) STANDARD WEIGHT	E2	QK-I-349	M2103235S	26-Mar-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000063 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.0000	0.0000	0.000090
0.10	0.1000	0.0000	0.000090
0.20	0.2000	0.0000	0.000090
0.50	0.5000	0.0000	0.000091
1.00	1.0000	0.0000	0.000091
2.00	2.0000	0.0000	0.000092
5.00	5.0000	0.0000	0.000093
10.00	10.0000	0.0000	0.000095
20.00	19.9999	0.0001	0.00010
50.00	49.9998	0.0002	0.00012
100.00	99.9998	0.0002	0.00019
200.00	199.9993	0.0007	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	99.9997
2	99.9996
3	99.9995
4	99.9997
5	99.9998
OFF-CENTER LOADING	0.0002

6. INTERNAL WEIGHT ERROR : 0.00066666666666660376 g

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT PRODUCTION AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 22M9914
REFERENCE No : 66549-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : AND

MODEL : GR-200

SERIAL No : 14243876

ID No : EQL-130

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD.,
SAMAEDAM, BANGKHUNTHIAN, BANGKOK
10150

CALIBRATED BY : PRASERT P.

CALIBRATION DATE : 15-Sep-22

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 21-Sep-22

RECEIVED DATE : 15-Sep-22



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 22M9914

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : GR-200
MANUFACTURER : AND S/N : 14243876
ID No : EQL-130 RECEIVED DATE : 15-Sep-22
AIR PRESSURE : 1011mbar \pm 1mbar CALIBRATION DATE : 15-Sep-22
AMBIENT TEMPERATURE : 21° C \pm 1° C RELATIVE HUMIDITY : 53 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING WEIGHT OF QUALITY CALIBRATION TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02210415	09-Feb-23
2) STANDARD WEIGHT	E2	15843	C02210419	10-Feb-23
3) STANDARD WEIGHT	E2	QK-I-349	M2103235S	26-Mar-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000048 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.0000	0.0000	0.000078
0.10	0.1000	0.0000	0.000078
0.20	0.2000	0.0000	0.000078
0.50	0.5000	0.0000	0.000079
1.00	1.0000	0.0000	0.000079
2.00	2.0000	0.0000	0.000080
5.00	5.0000	0.0000	0.000081
10.00	10.0000	0.0000	0.000084
20.00	20.0001	-0.0001	0.000089
50.00	50.0001	-0.0001	0.00011
100.00	100.0001	-0.0001	0.00019
200.00	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0001
4	100.0000
5	99.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT PRODUCTION AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

ใบรับรองการสอบเทียบ “ห้องเย็น”

(Calibration Certificate of Cool Room)



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th

E-Mail : calibrate@scg.com



Certificate No. T230022

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Cooling Room)

Manufacturer : -

Model : -

Serial No. : -

Customer Code : EQL-167

ID No. : T1447A1


Customer : Test Tech Co.,Ltd

30, 32 Rama II Soi 63, Rama II Rd., Samaedam,
Bangkhunthian Bangkok 10150

Customer Location : LABORATORY FLOOR 3

Date of Receipt : 13 January 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 24 JAN 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T230022

Page 2 of 4

Calibration Report

Equipment : Chamber (Cooling Room)
Date of Calibration : 18 January 2023
Environment : Temperature : 25.0-27.2 °C
Line Voltage : 221.9-227.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN141-TN150	T222123	5 October 2023
TC	TYPE T	TN151-TN160	T222123	5 October 2023
DATA LOGGER	34970A	T150	T222123	5 October 2023

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 2 Hour 8 Minute At 3 °C

Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max

☐ Close

☒ Not Available

5. Adjustment :

() without adjustment

(X) after adjustment


Approved By _____



Certificate No. T230022

Page 3 of 4

Calibration Report

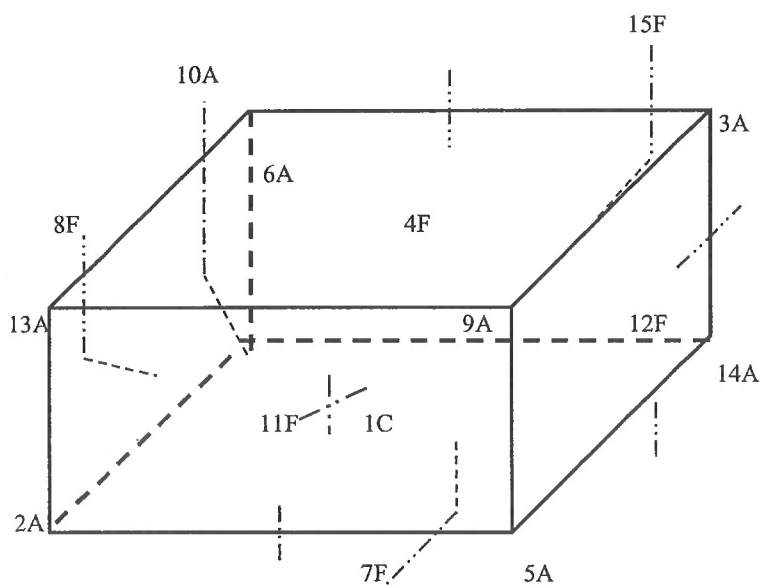

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN141
2A	=	TN142
3A	=	TN143
4F	=	TN144
5A	=	TN145
6A	=	TN146
7F	=	TN147
8F	=	TN148
9A	=	TN149
10A	=	TN150

11F	=	TN151
12F	=	TN152
13A	=	TN153
14A	=	TN154
15F	=	TN155

Approved By. _____



Certificate No. T230022

Page 4 of 4

Calibration Report

Measurement Results:

Average Standard Reading at each position (°C)										
Calibration Point	TN141	TN142	TN143	TN144	TN145	TN146	TN147	TN148	TN149	TN150
3	2.93	2.77	2.79	2.26	3.04	3.39	2.91	3.05	3.54	2.95
	TN151	TN152	TN153	TN154	TN155					
	3.32	3.28	3.00	2.96	2.90					


Chamber (Cooling Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage
	Min , Max	Average					Factor <i>k</i>
3.0	2.9 , 3.1	3.0	3.01	0.47	1.04	0.98	2.00

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th

E-Mail : calibrate@scg.com



Certificate No. T230121

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Cooling Room)

Manufacturer : -

Model : -

Serial No. : -

Customer Code : EQL-181

ID No. : T0399A5


Customer : Test Tech Co.,Ltd

30, 32 Rama II Soi 63, Rama II Rd., Samaedam,
Bangkhunthian Bangkok 10150

Customer Location : LABORATORY FLOOR 4

Date of Receipt : 26 January 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)
01 FEB 2023

Date of Issue : _____

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T230121

Page 2 of 4

Calibration Report

Equipment : Chamber (Cooling Room)
Date of Calibration : 30 January 2023
Environment : Temperature : 25.0-27.2 °C
Line Voltage : 221.9-227.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN141-TN150	T222123	5 October 2023
TC	TYPE T	TN151-TN160	T222123	5 October 2023
DATA LOGGER	34970A	T150	T222123	5 October 2023

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 30 Minute At 3 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

() without adjustment


(X) after adjustment

Approved By. 

Certificate No. T230121

Page 3 of 4

Calibration Report

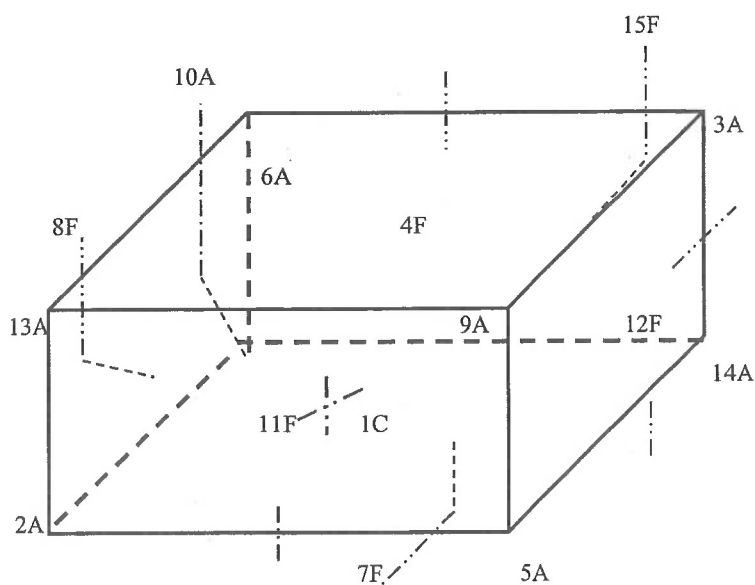

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN141
2A	=	TN142
3A	=	TN143
4F	=	TN144
5A	=	TN145
6A	=	TN146
7F	=	TN147
8F	=	TN148
9A	=	TN149
10A	=	TN150

11F	=	TN151
12F	=	TN152
13A	=	TN153
14A	=	TN154
15F	=	TN155

Approved By. Bm Loi

Certificate No. T230121

Page 4 of 4

Calibration Report

Measurement Results:

Average Standard Reading at each position (°C)										
Calibration Point	TN141	TN142	TN143	TN144	TN145	TN146	TN147	TN148	TN149	TN150
3	2.84	2.89	3.01	3.07	3.13	3.19	3.04	2.99	3.15	2.94
	TN151	TN152	TN153	TN154	TN155					
	2.99	2.99	3.14	2.85	2.88					

Chamber (Cooling Room)			Temperature Distribution				
S. g (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage
	Min , Max	Average					Factor <i>k</i>
3.0	2.8 , 3.1	3.0	3.01	0.48	0.93	0.99	2.00

The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 

ซ10

ใบรับรองการสอบเทียบ “ตู้บ่มเชื้อ”

(Calibration Certificate of Incubator)



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 22T7650

REFERENCE No : 65843-4

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : INCUBATOR

MANUFACTURER : MEMMERT

MODEL : INB 400

SERIAL No : E405.0946

ID No : EQL-087

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT P.

CALIBRATION DATE : 14-Jul-22

APPROVED BY : PONGSAK J.

ISSUED DATE : 15-Jul-22

RECEIVED DATE : 14-Jul-22



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22T7650

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : INCUBATOR
MANUFACTURER : MEMMERT
MODEL : INB 400
ID No : EQL-087
RECEIVED DATE : 14-Jul-22
AMBIENT TEMPERATURE : 24 °C ± 1 °C
S/N : E405.0946
CALIBRATION DATE : 14-Jul-22
RELATIVE HUMIDITY : 50 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	22T7509	10-Jul-23


3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

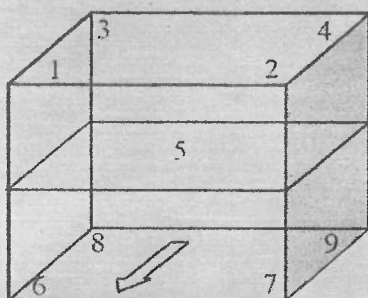

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 8
Instrument Condition : Normal
Chamber Size (W*L*H): 40*33*40 cm

CHAMBER PERFORMANCE

Calibration Point (°C)	Controller Temperature (°C)	Indicating Temperature (°C)	Average All Locations (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
44.0	44.0	44.0	44.16	0.11	0.85	1.04
55.0	55.0	55.0	55.19	0.07	0.76	0.97

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
44.0	44.0	44.00	44.08	43.56	43.66	44.39	44.40	44.48	44.36	44.47	0.36
55.0	55.0	55.00	55.46	54.60	54.79	55.33	55.30	55.46	55.30	55.48	0.36

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2. PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 22T1725

REFERENCE No : 64109-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : INCUBATOR

MANUFACTURER : MEMMERT

MODEL : IF 110

SERIAL No : D415.0802

ID No : EQL-190

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 21-Feb-22

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 22-Feb-22

RECEIVED DATE : 21-Feb-22



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22T1725

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : INCUBATOR
MANUFACTURER : MEMMERT
MODEL : IF 110
ID No : EQL-190
RECEIVED DATE : 21-Feb-22
AMBIENT TEMPERATURE : 24 °C ± 1 °C
S/N : D415.0802
CALIBRATION DATE : 21-Feb-22
RELATIVE HUMIDITY : 50 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7408027	21T6766	10-Jul-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

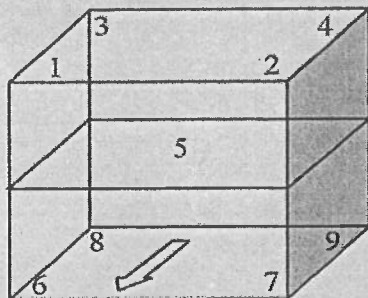

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 5
Overall Line Voltage (V) variation : 8
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

CHAMBER PERFORMANCE

Calibration Point (°C)	Controller Temperature (°C)	Indicating Temperature (°C)	Average All Locations (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
37.0	37.0	37.0	36.91	0.07	0.22	0.28
44.0	44.0	44.0	44.17	0.07	0.22	0.27

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
37.0	37.0	36.97	36.95	36.84	36.96	36.94	36.92	36.91	36.90	36.84	0.25
44.0	44.0	44.21	44.23	44.09	44.23	44.23	44.13	44.21	44.15	44.07	0.36

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

NSC-TISI-TIS17025
CALIBRATION 0049

CERTIFICATE No : 22T1726

REFERENCE No : 64109-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : INCUBATOR

MANUFACTURER : MEMMERT

MODEL : IF 160

SERIAL No : D518.0082

ID No : EQL-205

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 21-Feb-22

APPROVED BY : PONGSAK J.

ISSUED DATE : 22-Feb-22

RECEIVED DATE : 21-Feb-22



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22T1726

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : INCUBATOR
MANUFACTURER : MEMMERT
MODEL : IF 160
ID No : EQL-205
RECEIVED DATE : 21-Feb-22
AMBIENT TEMPERATURE : 24 °C ± 1 °C
S/N : D518.0082
CALIBRATION DATE : 21-Feb-22
RELATIVE HUMIDITY : 50 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	6635300	21T6765	10-Jul-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

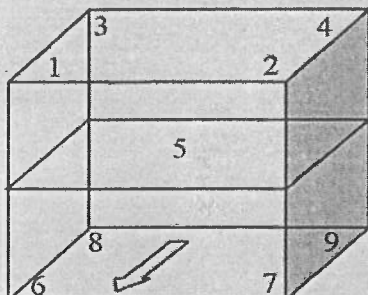

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 2
Overall Line Voltage (V) variation : 9
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*72 cm

CHAMBER PERFORMANCE

Calibration Point (°C)	Controller Temperature (°C)	Indicating Temperature (°C)	Average All Locations (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
35.0	35.0	35.0	34.99	0.02	0.14	0.20
36.0	36.0	36.0	36.00	0.03	0.14	0.22
41.5	41.5	41.5	41.46	0.05	0.10	0.19

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
35.0	35.0	34.91	34.94	34.93	34.93	34.98	35.03	35.08	35.01	35.08	0.25
36.0	36.0	35.93	35.95	35.95	35.94	36.00	36.05	36.10	36.01	36.10	0.25
41.5	41.5	41.46	41.47	41.41	41.47	41.50	41.47	41.45	41.43	41.49	0.36

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkac, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 22T1728

REFERENCE No : 64109-4

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : INCUBATOR

MANUFACTURER : MEMMERT

MODEL : IF 160

SERIAL No : D518.0240

ID No : EQL-218

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 21-Feb-22

APPROVED BY : PONGSAK J.

ISSUED DATE : 22-Feb-22

RECEIVED DATE : 21-Feb-22



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 22T1728

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : INCUBATOR
MANUFACTURER : MEMMERT
MODEL : IF 160
ID No : EQL-218
RECEIVED DATE : 21-Feb-22
AMBIENT TEMPERATURE : 24 °C ± 1 °C
S/N : D518.0240
CALIBRATION DATE : 21-Feb-22
RELATIVE HUMIDITY : 50 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	21T6764	10-Jul-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

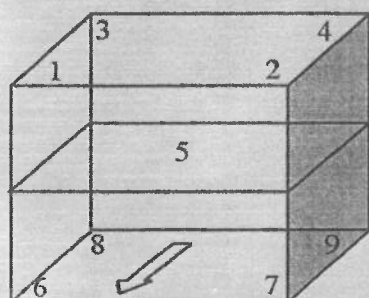

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 2
Overall Line Voltage (V) variation : 12
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*72 cm

CHAMBER PERFORMANCE

Calibration Point (°C)	Controller Temperature (°C)	Indicating Temperature (°C)	Average All Locations (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
35.0	35.0	35.0	35.00	0.05	0.15	0.26
36.0	36.0	36.0	36.00	0.04	0.16	0.26

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
35.0	35.0	34.94	34.98	34.93	34.97	35.07	35.10	34.94	35.04	35.05	0.25
36.0	36.0	35.94	35.97	35.92	35.96	36.07	36.11	35.95	36.05	36.05	0.25

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

๗11

ใบรับรองการทวนสอบ “เครื่อง Atomic Absorption Spectrophotometer”
(Calibration Certificate of Atomic Absorption Spectrophotometer)




PinAAcle 900F Preventive Maintenance Report

Company Name: TEST TECH CO.,LTD
Instrument Location: 30, 32 Rama II Soi 63 Rama II Road.
Samaedam, Bangkhuntien, Bangkok, 10510
Instrument Serial No.: PFBS21091601
Date: 06-Jul-2022

PinAAcle 900F Preventive Maintenance (PM)

Company Name:	TEST TECH CO.,LTD		
Address (Instrument Location):	30,32 Rama II Soi 63 Rama II Road.Samaedam, Bangkhuntien, Bangkok, 10510		
Serial Number:	PFBS21091601	PM Number:	1/2
Customer Name (if applicable):	K. AOYJAI	Telephone Number:	02-877-3271
Customer Support Engineer Name:	K. DUANG	Service Order Number:	WO-01833526
Date PM Performed: (DD-MMM-YYYY)	Jul 6, 2022	Next PM Due Date: (DD-MMM-YYYY)	Jan 6, 2023
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.

The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.

Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved.

No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.

Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	N/A
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	N/A
N9301714	Replacement Acetylene Filter Cartridge	N/A
TH001022	Replacement Air Filter Cartridge	N/A

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	25-76CUY1	30-Oct-2022

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 ml.	AR	AR
N/A	0.5% HNO ₃	250 ml.	AR	AR

Additional Tools Required for PM			
Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	MG0-252
N1013002	1.0A Neutral density filter	1	MG0-358
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	092216-010130
N3050109	Ba Lumina HCL	1	102416-040160
N3050139	K Lumina HCL	1	110716-010060
N3050152	Ni Lumina HCL	1	100516-030190

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Perform general inspection of system for cleanliness.

2. PC Instrument Software:

- ☒ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. Mechanical:

- ☒ Inspect and clean all fans and filters. Replace filters if necessary
- ☒ Inspect all gas lines for leaks and/or wear. Replace if needed.
- ☒ Clean exterior of the instrument.
- ☒ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ☒ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking slot width. Replace if out of specification
- ☒ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ☒ Check the drain system for signs of wear. Replace worn or damaged parts.
- ☒ Visually check for proper flame conditions when igniting the Air-C₂H₂ and N₂O-C₂H₂ flames (if applicable).

4. Electrical:

- ☒ Inspect PC boards. Clean if necessary.
- ☒ Carefully check all internal and external cable connections.
- ☒ Check instrument firmware revisions upgrade to current levels (if necessary)
- ☒ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

5. Optics:

- ☒ Inspect and clean the sample compartment windows, if needed.
- ☒ Inspect optics. Clean or replace if necessary,

6. Gasses:

- ☒ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ☒ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	0.9798	0.9806	Passed
0.2 A ND Filter	± 5% from Cert.	0.2042	0.2008	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0009	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed

8.4 D₂ Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0063	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0003	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0001	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	NA	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	0.3566	Passed

10. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

Additional Comments

Additional Comments Regarding the PM	
PERFORMANCE TEST FOR FIAS	
1. Characteristic mass for Mercury (500 ul of 10 ug/l for Hg And 5 replicates)	0.0674 Abs. 326.4 pg/ 0.0044 Abs.
Characteristic Mass	
% RSD	1.62%
2. Characteristic mass for Arsenic (500 ul of 10 ug/l for As And 5 replicates)	0.1631 Abs. 1.3e+03 pg/ 0.0044 Abs.
Characteristic Mass	
% RSD	1.29%
3. Characteristic mass for Selenium (500 ul of 10 ug/l for Se And 5 replicates)	0.3055 Abs. 72.0 pg/ 0.0044 Abs.
Characteristic Mass	
% RSD	0.92%
Wavelength Accuracy Check	
(As 193.70 nm +/-0.3 nm	193.70)
(Cu 324.75 nm +/-0.3 nm	324.70)
(Ba 553.55 nm +/-0.3 nm	553.50)
(K 766.49 nm +/-0.3 nm	766.60)

Review

<i>The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.</i>	
This PinAAcle 900F Passes <input checked="" type="checkbox"/> Fails <input type="checkbox"/> the preventive maintenance.	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative:	<div style="display: flex; justify-content: space-between;"> <div style="text-align: center;"> </div> <div style="text-align: right;"> Date: 06-Jul-2022 <small>(DD-MMM-YYYY)</small> </div> </div>
Authorized Customer Representative:	<div style="display: flex; justify-content: space-between;"> <div style="text-align: center;"> </div> <div style="text-align: right;"> Date: 06-Jul-2022 <small>(DD-MMM-YYYY)</small> </div> </div>

ซ12

ใบรับรองการทวนสอบ “เครื่องอ่างไอน้ำ”

(Calibration Certificate of Water bath)

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 22T8990

REFERENCE No : 66263-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : WATER BATH

MANUFACTURER : MEMMERT

MODEL : WNE 45

SERIAL No : L720.0266

ID No : EQL-241

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 19-Aug-22

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 19-Aug-22

RECEIVED DATE : 19-Aug-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 22T8990

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : WATER BATH
MANUFACTURER : MEMMERT
ID NUMBER : EQL-241
RECEIVED DATE : 19-Aug-22
AMBIENT TEMPERATURE : 27 °C ± 1 °C
MODEL : WNE 45
SERIAL NUMBER : L720.0266
CALIBRATION DATE : 19-Aug-22
RELATIVE HUMIDITY : 51 %RH ± 10 % RH


CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO ASTM E715-80 (REAPPROVED 2001) BY COMPARISON WITH CALIBRATED RTD. THE PROBES WERE PLACED ON FIVE POINTS AND LOCATED ONE PROBE IN EACH OF THE FOUR CORNERS OF THE BATH AND PLACED THE FIFTH RTD WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE WATER VOLUME (REFERENCE LOCATION) UNDER NO LOAD CONDITION.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	2625A	6603614	22T7514	05-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

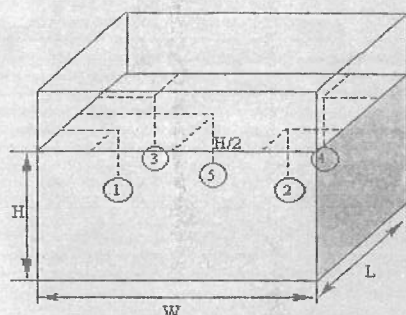

PROBE INSTALLATION
POSITION IN THE BATH

GENERAL INFORMATION

Overall Variation of Ambient Temperature around the Bath (°C) : 0.5
Overall Variation of Line Voltage (V) : 3
Instrument Condition : Normal
Bath Inner Size (W*L*H) : 59*35*22 cm

BATH PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
83.0	82.97	0.03	0.03	0.09
92.0	91.95	0.07	0.03	0.14

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations					Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	
83.0	83.0	82.97	82.97	82.96	82.98	82.99	0.14
92.0	92.0	91.95	91.97	91.94	91.96	91.95	0.15

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE BATH.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 22T7648

REFERENCE No : 65843-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : WATER BATH

MANUFACTURER : MEMMERT

MODEL : WPE 45

SERIAL No : L711.0024

No : EQL-147

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT P.

CALIBRATION DATE : 14-Jul-22

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 15-Jul-22

RECEIVED DATE : 14-Jul-22

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 22T7648

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : WATER BATH
MANUFACTURER : MEMMERT
ID NUMBER : EQL-147
RECEIVED DATE : 14-Jul-22
AMBIENT TEMPERATURE : 24 °C ± 1 °C
MODEL : WPE 45
SERIAL NUMBER : L711.0024
CALIBRATION DATE : 14-Jul-22
RELATIVE HUMIDITY : 50 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO ASTM E715-80 (REAPPROVED 2001) BY COMPARISON WITH CALIBRATED RTD. THE PROBES WERE PLACED ON FIVE POINTS AND LOCATED ONE PROBE IN EACH OF THE FOUR CORNERS OF THE BATH AND PLACED THE FIFTH RTD WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE WATER VOLUME (REFERENCE LOCATION) UNDER NO LOAD CONDITION.

2. REFERENCE STANDARD INSTRUMENTS :-


INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	2625A	6603614	22T7514	05-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

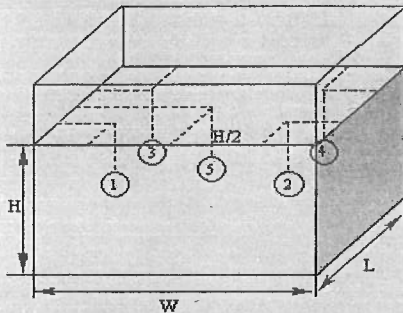

PROBE INSTALLATION
POSITION IN THE BATH

GENERAL INFORMATION

Overall Variation of Ambient Temperature around the Bath (°C) : 0.9
Overall Variation of Line Voltage (V) : 3
Instrument Condition : Normal
Bath Inner Size (W*L*H) : 60*42*24 cm

BATH PERFORMANCE

Calibration Point (°C)	Controller Temperature (°C)	Indicating Temperature (°C)	Average All Locations (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
41.5	41.5	41.5	41.54	0.05	0.03	0.12
44.5	44.5	44.5	44.50	0.07	0.02	0.15

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations					Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	
41.5	41.5	41.54	41.55	41.52	41.55	41.55	0.14
44.5	44.5	44.48	44.51	44.50	44.50	44.51	0.15

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE BATH.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT QC LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

ซ13

ใบรับรองการทวนสอบ “เครื่องนึ่งฆ่าเชื้อ”
(Calibration Certificate of Autoclave)



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 23T1391
REFERENCE No : 68175-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : AUTOCLAVE

MANUFACTURER : HIRAYAMA

MODEL : HVE-50

SERIAL No : 30612085166


No : EQL-155

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD.,
SAMAEDAM, BANGKHUNTHIAN, BANGKOK
10150

CALIBRATED BY : PRASERT P.

CALIBRATION DATE : 13-Feb-23

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 14-Feb-23

RECEIVED DATE : 13-Feb-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 23T1391

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : AUTOCLAVE
MANUFACTURER : HIRAYAMA
ID NUMBER : EQL-155
RECEIVED DATE : 13-Feb-23
AMBIENT TEMPERATURE : 30° C ± 1° C
MODEL : HVE-50
SERIAL NUMBER : 30612085166
CALIBRATION DATE : 13-Feb-23
RELATIVE HUMIDITY : 50 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BASED ON BS 2646 : Part 5 : 1993 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON FIVE LOCATIONS AS SHOWN IN THE PICTURE. TWO PROBES WERE PLACES NEAR TOP AND BOTTOM WALL AND EACH PROBE WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE THIRD PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE INSTRUMENT CHAMBER. PROBE NUMBER 4 WAS ATTACHED TO THE LOAD TEMPERATURE PROBE, IF FITTED, WITHIN 20 mm OF ITS TIP. PROBE NUMBER 5 WAS PLACED IN THE CHAMBER DRAIN OR VENT WITHIN 100 mm OF ITS CONNECTION TO THE CHAMBER.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT

MODEL

SERIAL No

CERTIFICATE No

DUE DATE

1) DATA LOGGER

VALPROBE


S350, DV35, DN94

23T0885

27-Jan-24

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

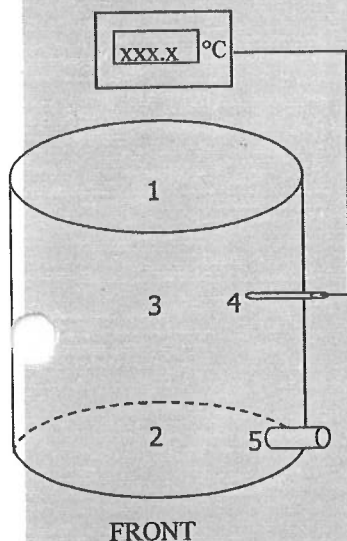

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber variation : 1.2 °C

Autoclave Condition : Normal

Chamber Size (Diameter*H): 30 * 71 cm

CHAMBER PERFORMANCE

Controller Temperature (°C)	Average All Locations (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)	Pressure (MPa)	Holding time (min)	Operating Cycle time (min)
116	116.48	0.09	0.10	0.27	0.090	15	60
122	122.43	0.09	0.13	0.27	0.130	15	60

TEMPERATURE MEASUREMENT ACCURACY TEST(° C)

Cont Temp	Ind Temp	Measured Temperature (°C) at Spread Locations					Uncertainty (± °C)
		#1	#2	#3	#4	#5	
116	116	116.45	116.50	116.53	116.45	116.45	0.59
122	122	122.40	122.46	122.50	122.39	122.39	0.59

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT OF TEMPERATURE MEASUREMENT ACCURACY TEST EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : THE STABILITY TERM IN THE UNCERTAINTY BUDGET WAS REPLACED BY THE STANDARD REPEATABILITY.

NOTE 3: LOCATION 3 WAS REFERENCE LOCATION.

NOTE 4 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

๗14

ใบรับรองการทวนสอบ “เครื่อง Spectrophotometer”
(Calibration Certificate of Spectrophotometer)

Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No. BSCC-UV-163/23
Equipment UV/Vis Spectrophotometer
Model UV-1900i
Manufacturer Shimadzu
Serial No. A12535780311ML
ID No. EQL-233
Date of receipt 27 April 2023
Date of calibration 27 April 2023
Date of issue 8 May 2023

Customer name Test Tech Co., Ltd.

Address 30, 32 Rama II Soi 63, Rama II RD., Samaedam, Bangkhunthian, Bangkok 10150

Temperature (23.5-24.4) °C (On site)
Humidity (50.8-48.2) %RH (On site)

Equipment condition Good Operation

Calibration Location Clean Room Circubond

Calibration Procedure In-house method WI-UV-702-01 based on ASTM E275-01

Traceability Wavelength Accuracy is traceable to certificate No. 96367 and 96366
Photometric Accuracy is traceable to certificate No. 99925 and 96363
Stray Light is traceable to certificate No. 96346
The above certificate are traceable to SI unit through Starna Scientific Ltd.
(UKAS accredited calibration laboratory NO. 0659)

Calibrated by Mr.Poomjai Korsawatvorakul

Approved by



Mr.Kanchit Choothep
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

Certificate of Calibration

Certificate No. **BSCC-UV-163/23**

Number of Page(s) 2 of 3

Calibration Results:

1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (\pm nm)
279.44	279.17	-0.27	0.18
418.53	418.45	-0.08	0.18
536.52	536.58	0.06	0.18
684.50	684.62	0.12	0.18
879.41	879.43	0.02	0.18

2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (\pm A)
235	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
257	0.0000	0.0000	0.0000	0.0075
	0.8552	0.8532	-0.0020	0.0075
313	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
350	0.0000	0.0001	0.0001	0.0075
	0.6349	0.6336	-0.0013	0.0075

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

Certificate of Calibration

Certificate No. **BSCC-UV-163/23**

Number of Page(s) **3 of 3**

Calibration Results:

3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ($\pm A$)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5472	0.5485	0.0013	0.0042
	0.7637	0.7637	0.0000	0.0042
	1.0480	1.0494	0.0014	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5371	0.5384	0.0013	0.0042
	0.7457	0.7457	0.0000	0.0042
	1.0233	1.0247	0.0014	0.0042
465.0	CNR	CNR	CNR	0.0042
	CNR	CNR	CNR	0.0042
	CNR	CNR	CNR	0.0042
	CNR	CNR	CNR	0.0042
546.1	0.0000	0.0000	0.0000	0.0042
	0.5006	0.5017	0.0011	0.0042
	0.6961	0.6954	-0.0007	0.0042
	0.9563	0.9565	0.0002	0.0042
590.0	CNR	CNR	CNR	0.0042
	CNR	CNR	CNR	0.0042
	CNR	CNR	CNR	0.0042
	CNR	CNR	CNR	0.0042
635.0	0.0000	0.0000	0.0000	0.0042
	0.5137	0.5147	0.0010	0.0042
	0.6907	0.6900	-0.0007	0.0042
	0.9533	0.9536	0.0003	0.0042

*CNR = Customer not request

4. Stray Light*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)		
	Wavelength (nm)	Transmission (%T)	Absorbance (A)
200.91 \pm 0.11nm	200.55	0.9670	2.0147


The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

End of Certificate

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.

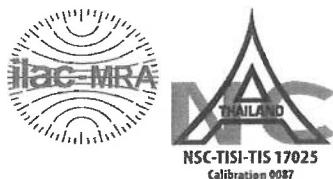

Certificate of Calibration

Equipment:	SPECTROPHOTOMETER	Certificate No.:	C06230165
Model:	DR6000	Issued Date:	24 April 2023
Serial No. (or ID.):	1693421 (EQL-197)	Job No.:	KSPR2306121
Manufacturer:	HACH	Page:	1 of 3
Condition:	In Condition		

Customer: TEST TECH CO., LTD.
30,32 Rama II Soi 63, Rama II Rd.,
Samaedam, Bangkhuntien Bangkok 10150 Thailand

Environment Condition:

Temperature	25.3	°C	±	0.2	°C
Humidity	48.9	%RH	±	1.7	%RH

Calibration Place: TEST TECH CO., LTD. (แผนกน้ำดี)
30,32 Rama II Soi 63, Rama II Rd.,
Samaedam, Bangkhuntien Bangkok 10150 Thailand

Calibration By: Mr. Atachai Ngamchanat
Calibration Date: 21 April 2023
The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04

Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 93907 and 93914

The standard for Photometric Certificate No. 94010 and 93900

The standard for Stray light Certificate No. 93903 and 93902

The standard for Spectral resolution Certificate No. 103140


(Mr. Atachai Ngamchanat)

Person in charge


(Mr. Nitinun Srihawan)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:
Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.5	0.11	0.13
536.66	536.7	-0.04	0.13
637.98	637.9	0.08	0.13
748.48	748.7	-0.22	0.13
807.03	807.5	-0.47	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.5816	0.580	0.0016	0.0045
	0.7130	0.712	0.0010	0.0045
	1.0151	1.013	0.0021	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.5649	0.563	0.0019	0.0045
	0.7012	0.699	0.0022	0.0045
	0.9982	0.996	0.0022	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.5249	0.524	0.0009	0.0045
	0.6621	0.661	0.0011	0.0045
	0.9420	0.939	0.0030	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.5214	0.520	0.0014	0.0045
	0.6982	0.697	0.0012	0.0045
	0.9947	0.992	0.0027	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.5549	0.553	0.0019	0.0045
	0.7736	0.771	0.0026	0.0045
	1.1041	1.101	0.0031	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.5621	0.561	0.0011	0.0045
	0.7630	0.761	0.0020	0.0045
	1.0890	1.086	0.0030	0.0045

Calibration Results:
Without Adjustment
Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7440	0.737	0.0070	0.0080
257 nm	0.0000	0.000	0.0000	0.0080
	0.8635	0.855	0.0085	0.0080
313 nm	0.0000	0.000	0.0000	0.0080
	0.2902	0.288	0.0022	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6409	0.634	0.0069	0.0080

Stray light *

Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
260.51 +/- 0.11 nm	260.5	0.7	2.155
391.84 +/- 0.11 nm	391.8	1.2	1.921

Spectral Resolution *

Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength (nm)	268.73	266.77	1.35	2.00
UUC: Wavelength (nm)	268.6	266.6		
Std Absorbance (A)	0.4237	0.2591		
Absorbance (A)	0.385	0.285		

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

ใบรับรองการทวนสอบ “เครื่องกลั่นไนโตรเจน”

(Calibration Certificate of Distillation Unit VAPODEST

VAP20, VAP30s)

การดูแลบำรุงรักษาเชิงป้องกัน

Preventive Maintenance



บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

ฝ่ายบริการหลังการขาย

โทร 0 2 639 7000 E-mail: service.tec.th@dksh.com

ฝ่ายขายและการตลาด

โทร 0 2 639 7000 E-Mail : marketing.tec.th@dksh.com

Website : www.dksh.co.th/technology/scientific-thailand

เงื่อนไขการให้บริการ Preventive Maintenance

บริษัทฯ จะส่งวิศวกรผู้ชำนาญ เพื่อให้บริการตามขอบข่ายของการบริการ เฉพาะ ในวันและเวลา ราชการ หากมีความประสงค์ที่จะรับบริการนอกเหนือจากวัน เวลา ราชการ (วันหยุดเสาร์ – อาทิตย์ หรือวันหยุด นักชดถุณ) บริษัทฯ จะคิดค่าบริการเพิ่มเติมตามอัตราที่กฎหมายแรงงานกำหนดไว้

ขอบข่ายการบริการ

- ตรวจสอบสภาพการทำงานต่าง ๆ ของเครื่องมือ
- ทดสอบประสิทธิภาพการทำงานของเครื่องมือ
- รายการผลการตรวจสอบเครื่องมือ

หมายเหตุ

- ราคานี้ไม่รวมถึงค่าบริการซ่อม หรือ เปลี่ยนอะไหล่ที่ชำรุดเสียหาย หรือหมดสภาพการใช้งาน
- ในกรณีที่ผู้รับบริการอยู่นอกเขตพื้นที่ให้บริการ บริษัทฯ จำเป็นต้องคิดค่าใช้จ่ายเพิ่มเติม ได้แก่ ค่าเดินทาง เป็นต้น
- บริษัท ฯ ขอสงวนสิทธิ์ในการเปลี่ยนแปลงราคา โดยไม่แจ้งให้ทราบล่วงหน้า

ช่องทางการติดต่อ



DKSH Technology Limited (บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด)

เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260

เลขประจำตัวผู้เสียภาษี 010-555-001-4547 (สำนักงานใหญ่)



Call center 0 2 639 7000



DKSH Scientific



www.dksh.com/scientific-thailand



marketing_tec.th@dksh.com



@dkshscientific

Preventive Maintenance Contract

จำนวนในการทำสัญญาบริการ 1 ครั้ง ต่อ ปี

ครั้งที่ 1/1 วันที่ 28 Mar 2023

รายละเอียดผู้รับบริการ

หน่วยงาน	บริษัท เทสท์ เทค จำกัด		
ที่อยู่	30,32 ซอยพระรามที่ 2 ซอย 63 ถนนพระรามที่ 2 แขวงสามก่า เขตบางขุนเทียน กรุงเทพมหานคร 10150		
โทรศัพท์	0-2893-4211-7	แฟกซ์	0-2893-4218


ผู้ติดต่อ

ชื่อ - นามสกุล	คุณมาริสา วิเศษสังข์			
ตำแหน่ง	หัวหน้าส่วน			
โทรศัพท์	0-2893-4211-7	เบอร์ต่อ		แฟกซ์ 0-2893-4218
E-mail	Lab_center@testtech.co.th			

รายละเอียดผู้ให้บริการ

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด (ฝ่ายบริการหลังการขาย) (สำนักงานใหญ่)		
เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260		
โทรศัพท์ 0 2 693 7000 Email: siriporn.sy@dksh.com Line ID : siripon3007		
เจ้าหน้าที่ประสานงาน : คุณศิริพร อยู่ทองจ้อย โทรศัพท์ 090 678 6924 , 02 301 7467		
เจ้าหน้าที่ผู้ให้บริการ	นายจิรายุช สเลอาด	
ตำแหน่ง	Specialist, Technical Service.	
โทรศัพท์	0938138736	แฟกซ์ -
E-mail	Jirayut.js@dksh.com	

ลงนามผู้รับบริการ	
ตัวบรรจง	(.....)
ตำแหน่ง	
วันที่ / ประทับตราบริษัท	


ลงนามผู้ให้บริการ	
ตัวบรรจง	(นายจิรายุช สเลอาด)
ตำแหน่ง	Specialist, Technical Service
วันที่ / ประทับตราบริษัท	28/3/2023

JOB No: Lspr2302591..... MODEL: Vap30..... S/N: 003718.....

Part : Operational Qualification (OQ)


ตรวจสอบสภาพเครื่อง

FRONT

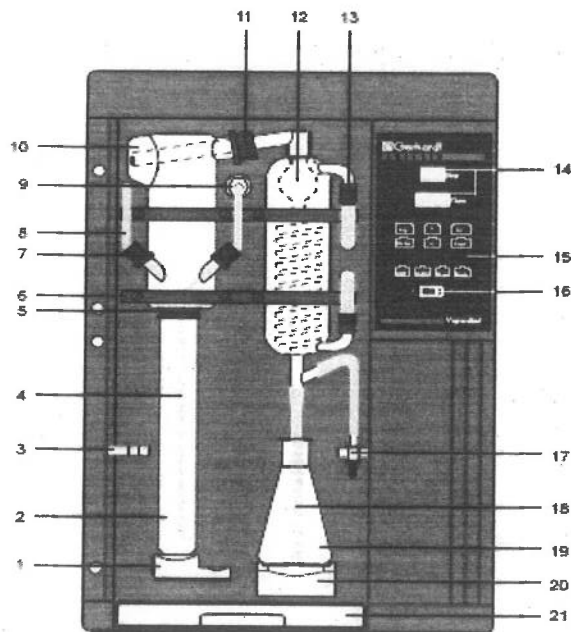

	Pass	Fail	N/A	Remark
1.Quick clamping device with wedge	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
2. Kjeldatherm digestion tube	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
3. Holder for steam inlet tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4. PTFP-Inlet tubing, steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5. Viton-cone	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6. Clamping for glassware	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7. Screw cap GL18 with silicone seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8. PTFP-Inlet tubing, NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9. PP-Distributor with PP-threaded joint	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10. Distribution head, glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11. Screw cap GL32 with silicone seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12. Distillation condenser	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13. Screw cap GL14 with plastic screw connection	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14. Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15. Keyboard, chemical-resistant	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16. Main switch, green	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17. Ventilation valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
18. Distillate outlet tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19. Erlenmeyer flask	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20. Platform	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21. Drip tray	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

REAR

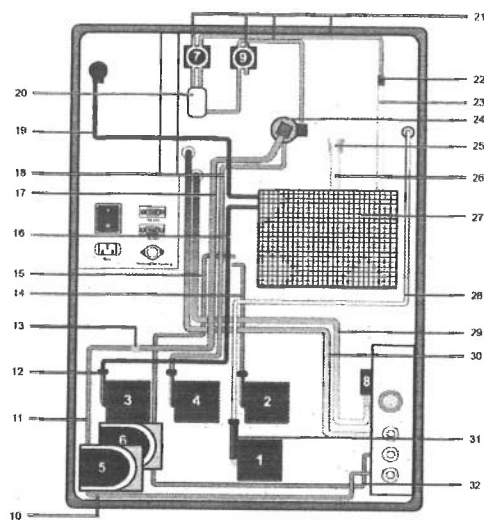

	Pass	Fail	N/A	Remark
1. Diaphragm pump NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
2. Diaphragm pump H ₃ BO ₃	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	vap 40 only
3. Diaphragm pump H ₂ O for steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4. Diaphragm pump H ₂ O for sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
5. Peristaltic pump for suction sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
6. Peristaltic pump for suction receiver	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	option
7. Pinch-solenoid valve, steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8. Magnetic valve with pressure control	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9. Pinch-solenoid valve, shut-off	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10. Verprene-tubing 4x8 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11. Verprene-tubing 4x8 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
12. Non-return valve for diaphragm pumps	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13. Tubing reduction PP 51x10x5 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
14. Silicone tubing 4x7 mm.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	vap 40 only
15. Silicone tubing 4x7 mm.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	option
16. Silicone -tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17. Verprene-tubing 8x12 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
18. Verprene tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
19. Silicone tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20. Ventilation glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21. Novoprene-tubing 4.8x8 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
22. Tubing reduction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
23. Silicone tubing 6x10 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
24. PP-distributor with PP-thread	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
25. SKT-valve (built in with brass fitting)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
26. Silicone tubing 8x16x80 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27. Steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
28. PTFE-inlet tubing NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
29. Silicone tubing 8x16 for cooling water inlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
30. Silicone tubing 8x16 for cooling water outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
31. Viton-tubing 6x12*50 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
32. Silicone tubing 4x7 mm.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	option

รายละเอียดการตรวจสอบ

ขั้นตอนการบริการ

ตรวจสอบระบบไฟฟ้า (Electrical Test)

- ความต้านทานทางไฟฟ้าของเครื่องกับกราวด์
- กระแสไฟฟ้าที่ใช้งาน

ตรวจสอบสภาพเครื่อง (Optical Test)

- Main cable
- Electric wiring
- Pumps
- Distribution Head
- Condensor
- Steam generator
- Tubing
- Viton cone

ตรวจสอบ Function การทำงาน (The Function Test)

- ระบบสร้างและควบคุมความดันของ Steam
- ระบบการเติมน้ำเข้า Sample Tube
- ระบบการเติม Na OH
- ระบบการ Suction ตั้ง Sample Tube และ Receiver

รายงานผลการให้บริการ

1. TECHNICAL DATA

	Pass	Fail	N/A	Remark
Main Supply 220 volt + 10% 50 Hz with ground	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Norminal current	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/> 6 a

1.1 COOLING WATER BATH

	Pass	Fail	N/A	Remark
Temperature 15-20 °C	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cooling Water Outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Control Temperature	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

1.2 OPTICAL TEST VAP...30...

	Pass	Fail	N/A	Remark
Screw cap GL14	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Screw cap GL18	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Screw cap GL32	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Distillation Head	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Condensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Viton Cone	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Ventilation Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Micro Switch Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

2. SYSTEM COOLING WATER INLET

	Pass	Fail	N/A	Remark
Cooling Water Inlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cooling Water Outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Magnetic valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

3.SYSTEM CONTROL

	Pass	Fail	N/A	Remark
Key Board	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Program	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Adding H ₂ O	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
Adding NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Adding H ₃ BO ₃	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	vap 40 only
Suction Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only

4.SYSTEM DISTILLATION

	Pass	Fail	N/A	Remark
Boiler	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Level Sensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Novoprene-Tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Solenoid Valve Shut-Off	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Solenoid Valve Steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Excess Pressure Detector	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Ventilation Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Heater	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

5. PUMP

	Pass	Fail	N/A	Remark
Pump H ₂ O Steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
- Non-Return Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Pump H ₂ O Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
- Non-Return Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Pump NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
- Non-Rutum Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Pump H ₃ BO ₃	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
- Non-Rutum Valve	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Pump Suction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

6. The Following Program Run :

	Pass	Fail	N/A	Remark
Addition H ₂ O 0-99 sec.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Addition NaOH 0-99 sec.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Addition H ₃ BO ₃ 0-99 sec.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Reaction Time 0-99 min.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Distillation Time 0-99 min	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Steam Capacity 30%-100%	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Suction Time 0-99 sec.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
The Instrument is in perfect technical shape	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Remark :

.....

.....

Part : ข้อมูลสนับสนุนด้านเทคนิค (General Technical Support)

การบำรุงรักษาทั่วไป (Basic maintenance)

Cleaning

Glass parts and suction pump should be cleaned before long periods of non-usage (i.e. holidays). This way blockages caused by crystalline deposits are avoided.

The following program should be run:

Addition H_3BO_3	0	s
Addition H_2O :	13	s
Addition NaOH:	0	s
Reaction time:	0	s
Distillation time:	7	min.
Steam capacity:	100	%
Suction time:	20	s

Place an empty digestion tube and an Erlenmeyer flask into position, and start the program.

In case of extreme deposits in the glassware you can clean the system by putting about 10 ml of sulphuric acid into the digestion tube.

Error Code

The micro-processor continually surveys all the functions of the distillation system. As soon as an error arises it is shown on the display and accompanied by an acoustic signal.

Error message	Measures	
No tap water	Check cooling water inlet for blockages. Ensure the tap is turned on	→ Enter
No sample tube	Insert tube	→ Enter
Check chemicals	Check set of tanks	→ Enter
Low water Press Enter	Check the water inlet distilled H ₂ O	→ Enter
↓ Filling Steam generator	This message disappears as soon as steam generator is filled	

After the above mentioned errors are corrected, the following message is displayed.

Error message	Measures
Stop Prog.No. x continue=Enter	Enter = continue of interrupted program Reset = Standby-mode

Other error messages

Error message	Measures
Wait for steam	Message disappears as soon as stand-by is reached
Add sol. > 1min Continue=Enter	Check programming Enter=continue of interrupted program Reset=Standby-mode
Program undefined	Check programming → Reset
Excess steam pressure	Switch the system off and call service
Sensor error	Switch the system off and call service