

เอกสารแนบ 6

เอกสารสอบเทียบเครื่องมือที่ใช้ในการวิเคราะห์

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : BURETTE
MANUFACTURER : ISO LAB
MODEL / TYPE : 25 ml
SERIAL NO. : N/A[EM-MBR10002/17]
CLID. NO. : 272201671
JOB CONTROL NO. : 230425044052

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 25 April 2023

DATE OF ISSUED : 02 May 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Sechanart
Calibration Engineer

Approved By :



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q23044052

F3-011-04/01-12

page 1 of 3



REPORT OF CALIBRATION FOR

NOMENCLATURE : BURETTE
MANUFACTURER : ISO LAB
MODEL / TYPE : 25 ml
SERIAL NO. : N/A[EM-MBR10002/17]
DATE OF CALIBRATION : 27 April 2023

ENVIRONMENT CONDITIONS :

Temperature : $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-86** according to **ASTM E542-01:2021** as calibration guidelines.

The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23044052**

F3-011-04/01-12

page 2 of 3



@clccalibration



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

CALIBRATION DATA

CORRECTION OF VOLUME

DUC Test point (ml)	Actual volume (ml)	Correction (ml)	Uncertainty $\pm$ (ml)	Coverage factor k
5	5.0003	+0.0003	0.0038	2,00
15	15.0044	+0.0044	0.0066	2,00
25	25.0092	+0.0092	0.0068	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 94 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23044052

F3-011-04/01-12

page 3 of 3



@clccalibration
u.6/3

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : CYLINDER
MANUFACTURER : FAVORIT
MODEL / TYPE : 50 ml
SERIAL NO. : N/A [EM-VPP02501/21]
CLID. NO. : 272300782
JOB CONTROL NO. : 230328034770

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 04 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Sukgasem Seehanart
Calibration Engineer

Approved By :

Authorized Signatory

04 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23034770

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION FOR

NOMENCLATURE : CYLINDER
MANUFACTURER : FAVORIT
MODEL / TYPE : 50 ml
SERIAL NO. : N/A [EM-VPP02501/21]
DATE OF CALIBRATION : 31 March 2023

ENVIRONMENT CONDITIONS :

Temperature : $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-84** according to **ASTM E542-01:2021** as calibration guidelines.
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23034770**

F3-011-04/01-12

page 2 of 3





CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

CALIBRATION DATA

CORRECTION OF VOLUME

DUC Test point (ml)	Actual volume (ml)	Correction (ml)	Uncertainty $\pm$ (ml)	Coverage factor k
50	50.1999	+0.1999	0.0180	2,00

Type of glassware : ☒ to Contain ☐ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 94 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23034770

F3-011-04/01-12

page 3 of 3



@clccalibration

CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : CYLINDER
MANUFACTURER : BOROSIL
MODEL / TYPE : 500 ml
SERIAL NO. : 0334-58
CLID. NO. : 272201292
JOB CONTROL NO. : 230328034769

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND


DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 04 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Calibration Engineer

Approved By :

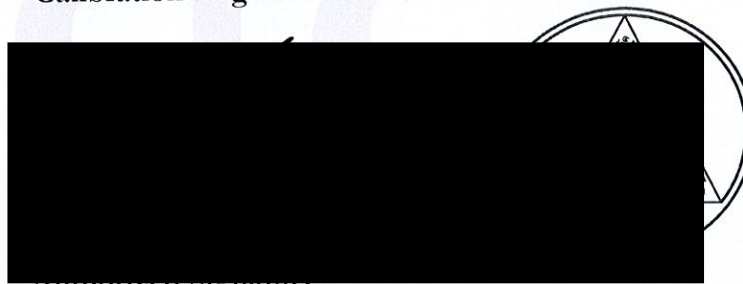

04 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q23034769

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION FOR

NOMENCLATURE : CYLINDER
MANUFACTURER : BOROSIL
MODEL / TYPE : 500 ml
SERIAL NO. : 0334-58
DATE OF CALIBRATION : 31 March 2023

ENVIRONMENT CONDITIONS :

Temperature : $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-84** according to **ASTM E542-01:2021** as calibration guidelines.
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model Secura6102-1s S/N.0042104938.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22121337, Due Date 01 December 2023.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23034769**

F3-011-04/01-12

page 2 of 3



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

CALIBRATION DATA

CORRECTION OF VOLUME

DUC Test point (ml)	Actual volume (ml)	Correction (ml)	Uncertainty $\pm$ (ml)	Coverage factor k
500	498.75	-1.25	0.10	2,00

Type of glassware : ☒ to Contain ☐ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 94 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23034769

F3-011-04/01-12

page 3 of 3



@clccalibration

CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : MEASURING PIPETTE
MANUFACTURER : GLASSCO
MODEL / TYPE : 1 ml
SERIAL NO. : N/A[EM-MER01001/19]
CLID. NO. : 272201297
JOB CONTROL NO. : 230328034780

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 03 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Calibration Engineer

Approved By :

Authorized Signatory

03 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q23034780

F3-011-04/01-12

page 1 of 3



REPORT OF CALIBRATION FOR

NOMENCLATURE : MEASURING PIPETTE
MANUFACTURER : GLASSCO
MODEL / TYPE : 1 ml
SERIAL NO. : N/A[EM-MER01001/19]
DATE OF CALIBRATION : 29 March 2023

ENVIRONMENT CONDITIONS :

Temperature : $(20 \pm 2.5) ^\circ\text{C}$ Relative Humidity : $(50 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-89** according to **ASTM E542-01:2021** as calibration guidelines.
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23034780

F3-011-04/01-12

page 2 of 3



@clcalibration



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

CALIBRATION DATA

CORRECTION OF VOLUME

DUC Test point (ml)	Actual volume (ml)	Correction (ml)	Uncertainty $\pm$ (ml)	Coverage factor k
*0.1	0.1015	+0.0015	0.0024	2,00
*0.5	0.5012	+0.0012	0.0025	2,00
1	1.0003	+0.0003	0.0025	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. * means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 96 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23034780

F3-011-04/01-12

page 3 of 3



@clcalibration

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : MEASURING PIPETTE
MANUFACTURER : GLASSCO
MODEL / TYPE : 5 ml
SERIAL NO. : N/A[EM-MER01001/18]
CLID. NO. : 272201296
JOB CONTROL NO. : 230328034779

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 03 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Calibration Engineer

Approved By :

Authorized Signatory

03 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q23034779

F3-011-04/01-12

page 1 of 3



@clcalibration

REPORT OF CALIBRATION FOR

NOMENCLATURE : MEASURING PIPETTE
MANUFACTURER : GLASSCO
MODEL / TYPE : 5 ml
SERIAL NO. : N/A[EM-MER01001/18]
DATE OF CALIBRATION : 29 March 2023

ENVIRONMENT CONDITIONS :

Temperature : $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-89** according to **ASTM E542-01:2021** as calibration guidelines.
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23034779**

F3-011-04/01-12

page 2 of 3



@clcalibration



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

CALIBRATION DATA

CORRECTION OF VOLUME

DUC Test point (ml)	Actual volume (ml)	Correction (ml)	Uncertainty $\pm$ (ml)	Coverage factor k
*0.5	0.5034	+0.0034	0.0025	2,00
2.5	2.4871	-0.0129	0.0029	2,00
5	4.9818	-0.0182	0.0029	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. * means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 96 of 138

CALIBRATION LABORATORY Co., LTD.

This report is valid for the above stated instrument/s only.

CLC

End of Certificate

Certificate No. Q23034779

F3-011-04/01-12

page 3 of 3



@clcalibration



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : MEASURING PIPETTE
MANUFACTURER : GLASSCO
MODEL / TYPE : 10 ml
SERIAL NO. : N/A[EM-MER01001/17]
CLID. NO. : 272000237
JOB CONTROL NO. : 230328034778

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 03 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Calibration Engineer

Approved By :

Authorized Signatory

03 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q23034778

F3-011-04/01-12

page 1 of 3



@clcalibration

REPORT OF CALIBRATION FOR

NOMENCLATURE : MEASURING PIPETTE
MANUFACTURER : GLASSCO
MODEL / TYPE : 10 ml
SERIAL NO. : N/A[EM-MER01001/17]
DATE OF CALIBRATION : 29 March 2023

ENVIRONMENT CONDITIONS :

Temperature : $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-89** according to **ASTM E542-01:2021** as calibration guidelines.
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23034778

F3-011-04/01-12

page 2 of 3



@clcalibration
16/17

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

CALIBRATION DATA

CORRECTION OF VOLUME

DUC Test point (ml)	Actual volume (ml)	Correction (ml)	Uncertainty $\pm$ (ml)	Coverage factor k
1	1.0058	+0.0058	0.0025	2,00
5	4.9937	-0.0063	0.0029	2,00
10	9.9802	-0.0198	0.0039	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 96 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23034778

F3-011-04/01-12

page 3 of 3



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VOLUMETRIC FLASK
MANUFACTURER : SCI
MODEL / TYPE : 100 ml
SERIAL NO. : N/A[EM-VPP02501/17]
CLID. NO. : 272101212
JOB CONTROL NO. : 230328034773

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 05 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Calibration Engineer

Approved By :

05 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q23034773

F3-011-04/01-12

page 1 of 3



@clcalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : **VOLUMETRIC FLASK**
MANUFACTURER : **SCI**
MODEL / TYPE : **100 ml**
SERIAL NO. : **N/A[EM-VPP02501/17]**
DATE OF CALIBRATION : **03 April 2023**

ENVIRONMENT CONDITIONS :

Temperature : $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-88** according to **ASTM E542-01:2021** as calibration guidelines.
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23034773

F3-011-04/01-12

page 2 of 3



@clcalibration

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

CALIBRATION DATA

CORRECTION OF VOLUME

DUC Test point (ml)	Actual volume (ml)	Correction (ml)	Uncertainty $\pm$ (ml)	Coverage factor k
100	99.9589	-0.0411	0.0190	2,00

Type of glassware : ☒ to Contain ☐ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 95 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23034773

F3-011-04/01-12

page 3 of 3



@clcalibration

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VOLUMETRIC FLASK
MANUFACTURER : BOROSIL
MODEL / TYPE : 500 ml
SERIAL NO. : N/A[EM-VPP02501/18]
CLID. NO. : 272201295
JOB CONTROL NO. : 230328034772

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 06 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Calibration Engineer

Approved By :

Authorized Signatory

06 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q23034772

F3-011-04/01-12

page 1 of 3



@calibration

REPORT OF CALIBRATION FOR

NOMENCLATURE : **VOLUMETRIC FLASK**
MANUFACTURER : **BOROSIL**
MODEL / TYPE : **500 ml**
SERIAL NO. : **N/A[EM-VPP02501/18]**
DATE OF CALIBRATION : **03 April 2023**

ENVIRONMENT CONDITIONS :

Temperature : $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-88** according to **ASTM E542-01:2021** as calibration guidelines.
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model Secura6102-1s S/N.0042104938.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22121337, Due Date 01 December 2023.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23034772

F3-011-04/01-12

page 2 of 3



@clcalibration

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

CALIBRATION DATA

CORRECTION OF VOLUME

DUC Test point (ml)	Actual volume (ml)	Correction (ml)	Uncertainty $\pm$ (ml)	Coverage factor k
500	500.04	+0.04	0.09	2,00

Type of glassware : ☒ to Contain ☐ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 95 of 138

This report is valid for the above stated instrument/s only.

CALIBRATION LABORATORY Co.,LTD.

CLC

End of Certificate

Certificate No. Q23034772

F3-011-04/01-12

page 3 of 3



@clcalibration

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VOLUMETRIC FLASK
MANUFACTURER : BOROSIL
MODEL / TYPE : 1000 ml
SERIAL NO. : N/A [EM-VPP02501/20]
CLID. NO. : 272300783
JOB CONTROL NO. : 230328034771

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 06 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Calibration Engineer

Approved By :

Authorized Signatory

06 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q23034771

F3-011-04/01-12

page 1 of 3



@clcalibration

REPORT OF CALIBRATION FOR

NOMENCLATURE : **VOLUMETRIC FLASK**
MANUFACTURER : **BOROSIL**
MODEL / TYPE : **1000 ml**
SERIAL NO. : **N/A [EM-VPP02501/20]**
DATE OF CALIBRATION : **03 April 2023**

ENVIRONMENT CONDITIONS :

Temperature : $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-88** according to **ASTM E542-01:2021** as calibration guidelines.
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model Secura6102-1s S/N.0042104938.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22121337, Due Date 01 December 2023.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23034771

F3-011-04/01-12

page 2 of 3



@calibration
11/06/2023

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

CALIBRATION DATA

CORRECTION OF VOLUME

DUC Test point (ml)	Actual volume (ml)	Correction (ml)	Uncertainty $\pm$ (ml)	Coverage factor k
1000	1000.05	+0.05	0.14	2,00

Type of glassware : ☒ to Contain ☐ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 95 of 138

This report is valid for the above stated instrument/s only.

CALIBRATION LABORATORY Co., LTD.

CLC

End of Certificate

Certificate No. Q23034771

F3-011-04/01-12

page 3 of 3



@calibration



CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : VOLUMETRIC PIPETTE
MANUFACTURER : GLASSCO
MODEL / TYPE : 10 ml
SERIAL NO. : N/A[EM-Mbro1001/17]
CLID. NO. : 272101209
JOB CONTROL NO. : 230328034776

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 03 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Sukgasem Sechanart

Approved By :

Authorized Signatory

03 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23034776

F3-011-04/01-12

page 1 of 3



@clcalibration

REPORT OF CALIBRATION FOR

NOMENCLATURE : VOLUMETRIC PIPETTE
MANUFACTURER : GLASSCO
MODEL / TYPE : 10 ml
SERIAL NO. : N/A[EM-Mbro1001/17]
DATE OF CALIBRATION : 29 March 2023

ENVIRONMENT CONDITIONS :

Temperature : $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-89** according to **ASTM E542-01:2021** as calibration guidelines.
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23034776

F3-011-04/01-12

page 2 of 3



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

CALIBRATION DATA

CORRECTION OF VOLUME

DUC Test point (ml)	Actual volume (ml)	Correction (ml)	Uncertainty $\pm$ (ml)	Coverage factor k
10	9.9970	-0.0030	0.0043	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 96 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23034776

F3-011-04/01-12

page 3 of 3



@clcalibration



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : VOLUMETRIC PIPETTE
MANUFACTURER : GLASSCO
MODEL / TYPE : 20 ml
SERIAL NO. : N/A[EM-VPP20201/17]
CLID. NO. : 272101208
JOB CONTROL NO. : 230328034775

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 03 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Sukgasem Sechanart

Calibration Engineer

Approved By :

Authorized Signatory

03 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23034775

F3-011-04/01-12

page 1 of 3



@clcalibration

REPORT OF CALIBRATION FOR

NOMENCLATURE : VOLUMETRIC PIPETTE
MANUFACTURER : GLASSCO
MODEL / TYPE : 20 ml
SERIAL NO. : N/A[EM-VPP20201/17]
DATE OF CALIBRATION : 29 March 2023

ENVIRONMENT CONDITIONS :

Temperature : $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-89** according to **ASTM E542-01:2021** as calibration guidelines.
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23034775

F3-011-04/01-12

page 2 of 3



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

CALIBRATION DATA

CORRECTION OF VOLUME

DUC Test point (ml)	Actual volume (ml)	Correction (ml)	Uncertainty $\pm$ (ml)	Coverage factor k
20	20.0020	+0.0020	0.0072	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 96 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23034775

F3-011-04/01-12

page 3 of 3



@calibration



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VOLUMETRIC PIPETTE
MANUFACTURER : HBG
MODEL / TYPE : 25 ml
SERIAL NO. : N/A[EM-VPP02501/17]
CLID. NO. : 272000238
JOB CONTROL NO. : 230328034774

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 03 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Calibration Engineer

Approved By :

Authorized Signatory
03 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to
the International System of Units (SI)

Certificate No. Q23034774

F3-011-04/01-12

page 1 of 3



@clclab

REPORT OF CALIBRATION FOR

NOMENCLATURE : VOLUMETRIC PIPETTE
MANUFACTURER : HBG
MODEL / TYPE : 25 ml
SERIAL NO. : N/A[EM-VPP02501/17]
DATE OF CALIBRATION : 29 March 2023

ENVIRONMENT CONDITIONS :

Temperature : $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-89** according to **ASTM E542-01:2021** as calibration guidelines.
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23034774

F3-011-04/01-12

page 2 of 3



@clclab5tion



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

CALIBRATION DATA

CORRECTION OF VOLUME

DUC Test point (ml)	Actual volume (ml)	Correction (ml)	Uncertainty $\pm$ (ml)	Coverage factor k
25	24.9589	-0.0411	0.0076	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 96 of 138

This report is valid for the above stated instrument/s only.

CALIBRATION LABORATORY Co., LTD.

CLC

End of Certificate

Certificate No. Q23034774

F3-011-04/01-12

page 3 of 3



@clcalibration

CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : DO METER
MANUFACTURER : HANNA INSTRUMENTS
MODEL / TYPE : HI5421/HI76483
SERIAL NO. : 04240005101/KC1A11T8H
CLID. NO. : 272101220
JOB CONTROL NO. : 230425044469

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 25 April 2023

DATE OF ISSUED : 28 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Calibration Engineer

Approved By :

Authorized Signatory

28 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to
the International System of Units (SI)

Certificate No. Q23044469

F3-011-04/01-12

page 1 of 3



@clccalib/37on

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	DO METER
MANUFACTURER	:	HANNA INSTRUMENTS
MODEL / TYPE	:	HI5421/HI76483
SERIAL NO.	:	04240005101/KC1A11T8H
DATE OF CALIBRATION	:	26 April 2023

ENVIRONMENT CONDITIONS :

Temperature : $(25 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPCH-06**. The calibration was performed by direct measurement with Certified Reference Material (CRM).

REFERENCE STANDARD USED :

Dissolved Oxygen, Sigma-Alorich Product ID QC3077-500ML .

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Merck Co., Ltd.

Lot LRAD0713.01 , Due Date September 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 % .
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23044469

F3-011-04/01-12

page 2 of 3



@clccalib360



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of Do Meter.

CALIBRATION DATA

Nominal Value (mg/L)	DUC Reading (mg/L)	Correction (mg/L)	Uncertainty (mg/L)
5.91	5.92	-0.01	± 0.22

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 4 of 54

This report is valid for the above stated instrument/s only.

CALIBRATION LABORATORY Co., LTD.

CLC

End of Certificate

Certificate No. Q23044469

F3-011-04/01-12

page 3 of 3



@clcalab/39on

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : pH METER
MANUFACTURER : HANNA INSTRUMENTS
MODEL / TYPE : HI5521/HI1131
SERIAL NO. : 04160019101/061334CN
CLID. NO. : 272101219
JOB CONTROL NO. : 230425044468

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 25 April 2023

DATE OF ISSUED : 28 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Sechanart
Calibration Engineer

Approved By :

Authorized Signatory

28 April 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to
the International System of Units (SI)

Certificate No. Q23044468

F3-011-04/01-12

page 1 of 3



@clccalibration
u.6/40

REPORT OF CALIBRATION

FOR

NOMENCLATURE : pH METER
MANUFACTURER : HANNA INSTRUMENTS
MODEL / TYPE : HI5521/HI1131
SERIAL NO. : 04160019101/061334CN
DATE OF CALIBRATION : 26 April 2023

ENVIRONMENT CONDITIONS :

Temperature : $(25 \pm 2.5) ^\circ\text{C}$ **Relative Humidity** : $(50 \pm 15) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-128**. The calibration was performed by direct measurement with Certified Reference Material (CRM).

REFERENCE STANDARD USED :

1. pH Standard Solution, NIMT TRM CODE TRM-S-2003, TRM CODE TRM-S-2007.
2. pH Standard Solution, Control Company Catalog Number 06-664-260, 11754256, Lot Number CC728484.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Lot Number. 160221 , 180121. Due Date 05 May 2023.
2. The measurements are traceable to International System of Units (SI) , through Control Company.
Certificate No. 4281-12405788 , Due Date 30 June 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23044468

F3-011-04/01-12

page 2 of 3



@clccalibration
u.6/41



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of pH meter.

CALIBRATION DATA

pH METER RESULT @ 25 °C

Standard pH Buffer Solution (pH)	pH Meter Reading (pH)	pH Meter Reading (mV)	Correction (pH)	Uncertainty of pH Measurement ($\pm$ pH)	k Factor
4.000	3.98	132.0	+0.020	0.014	2,20
6.996	7.00	-41.1	-0.004	0.015	2,06
10.007	10.01	192.5	-0.003	0.100	2,05

Technical Note. Setting function CAL 3 point (4,7,10).

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 91 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23044468

F3-011-04/01-12

page 3 of 3



@clccalibration
11.6/42

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOMETER
MANUFACTURER : HANNA INSTRUMENTS
MODEL / TYPE : HI5521/HI7662-W
SERIAL NO. : 04160019101/0615024N
CLID. NO. : 232202088
JOB CONTROL NO. : 230425044467

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 25 April 2023

DATE OF ISSUED : 02 May 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Monthira Treechum
Calibration Engineer

Approved By :

Authorized Signatory

02 May 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to
the International System of Units (SI)

Certificate No. Q23044467

F3-011-04/01-12

page 1 of 3



REPORT OF CALIBRATION FOR

NOMENCLATURE : DIGITAL THERMOMETER
MANUFACTURER : HANNA INSTRUMENTS
MODEL / TYPE : HI5521/HI7662-W
SERIAL NO. : 04160019101/0615024N
DATE OF CALIBRATION : 27 April 2023

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$ Relative Humidity : $(55 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-187** based on **ASTM E 644-11:2019** as calibration guidelines.
The calibration was performed by using Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
2. Precision Thermometer, ASL Model F200-A-8 S/N. 014433/03.
3. IPRT, ASL Model T100-250-1D S/N. L0193A-1-1.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd. Certificate No. Q22130792, Due Date 05 January 2024.
2. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0010/66, Due Date 06 November 2023.
3. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand). Certificate No. TT-0166-22, Due Date 01 December 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23044467**

F3-011-04/01-12

page 2 of 3



@clccalibration
1.6/44



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC Reading were recorded and the means value were reported of five times measurement in the table below.

CALIBRATION DATA

CORRECTION OF TEMPERATURE [THERMISTOR]

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty $\pm$ (°C)
105	24.00	24.1	-0.10	0.07
	25.01	25.1	-0.09	
	27.00	27.1	-0.10	

Note. Probe $\varnothing$ 3.5 mm

Materials : Metal Sheath.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 35 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23044467

F3-011-04/01-12

page 3 of 3



@clccalibration
1.6/45



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : SS2206-022-0001

Date Issued : 10-Jun-22

Customer : OKLA TESTING & CONSULTING SERVICE CO.,LTD
63/13 Soi.Petchkasem 7, Petchkasem Rd., Thapra, Bangkok Yai, Bangkok
10600

Equipment : Electronic Balance

Manufacturer : Sartorius

Model : BSA224S-CW

Serial No. : 35790699

ID No./Tag No. : -

Date Received : 03-Jun-22

Date Calibrated : 03-Jun-22

Calibrated by : Mr. Nirot Parnkamnoed

Calibration Method or Calibration Procedure Used

In-house method : CP-06 base on UKAS LAB 14 Edition 6 October 2019.


This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by

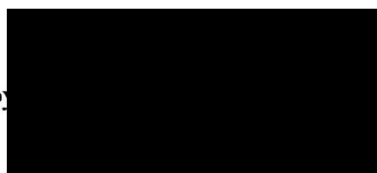

Page 1 of 2

Certificate No. : SS2206-022-0001

Environment : Ambient Temperature : Start record 25.5 °C , Stop record 25.6 °C
Relative Humidity : Start record 54.5 %RH , Stop record 54.6 %RH
Atmospheric Pressure : Start record 1001.2 mbar , Stop record 1001.3 mbar

Max. Capacity : 220 g Resolution : 0.0001 g

Departure from nominal value

Nominal Value (g)	Correction Value (g) Before Adjusted	Correction Value After Adjusted	Uncertainty ± (g)
0 *	0.0000	-	0.000082
20	- 0.0001	-	0.00025
40	- 0.0001	-	0.00026
60	- 0.0001	-	0.00028
80	- 0.0002	-	0.00028
100	- 0.0001	-	0.00028
120	- 0.0002	-	0.00046
140	- 0.0002	-	0.00046
160	- 0.0002	-	0.00046
180	- 0.0003	-	0.00046
220	- 0.0002	-	0.00059


Marked * are not included in the NSC-ONSC accreditation schedule for our laboratory.

Repeatability of reading

Load (g) : 220
Standard deviation (g) : 0.00000
Maximum difference (g) : 0.0000
between successive reading

Off-centre loading

Load (g) : 100
Position A (g) : 100.0000
Position B (g) : 100.0000
Position C (g) : 100.0000
Position D (g) : 100.0000
Position E (g) : 100.0000
Maximum (g) : 0.0000
difference



Front View

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

SPC Certificate No. C02220774 for Weight Set E2 600g Serial No. MIT-STD-280, Due 08-Apr-23

End of Certificate



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : SS2206-022-0006

Date Issued : 10-Jun-22

Customer : OKLA TESTING & CONSULTING SERVICE CO.,LTD
63/13 Soi.Petchkasem 7, Petchkasem Rd., Thapra, Bangkok Yai,
Bangkok 10600

Equipment : Freezer

Manufacturer : S-Cool

Model : SM61M 9.5 Q

Serial No. : OKLA-LAB-011/190118

ID No./Tag No. : -

Date Received : 03-Jun-22

Date Calibrated : 03-Jun-22

Calibrated by : Mr. Nirot Parnkamnoed

Calibration Method or Calibration Procedure Used

Standard method : CP-05 TLAS G-20.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:



(Mr. Natapong Kruadum)



Page 1 of 2

Certificate No. : SS2206-022-0006


Environment : Ambient Temperature : Start record 25.5 °C, Stop record 25.6 °C
Relative Humidity : Start record 54.6 %RH, Stop record 54.7 %RH

Calibration Temperature (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Stability ¹ (°C)	Measured Uniformity ² (°C)	Overall Variation ³ (°C)
2	2.0	2.2	0.12	1.38	2.37
4	4.0	4.0	0.14	0.90	1.82
6	6.0	6.0	0.05	1.08	1.74

Without adjustment

Calibration Temperature (°C)	Standard Reading (°C), Probe No. 9 is Reference Probe										Uncertainty ⁴ ±°C
2	No. 1	No. 2	No. 3	No. 4	No. 5	No. 6	No. 7	No. 8	No. 9		
	2.58	0.88	2.44	1.14	1.67	1.61	2.19	1.20	1.70		
	No. W10	No. W11	No. W12	No. W13							0.38
4	No. 1	No. 2	No. 3	No. 4	No. 5	No. 6	No. 7	No. 8	No. 9		
	4.36	2.72	4.19	2.98	3.42	3.29	3.94	2.97	3.50		
	No. W10	No. W11	No. W12	No. W13							0.31
6	No. 1	No. 2	No. 3	No. 4	No. 5	No. 6	No. 7	No. 8	No. 9		
	6.11	4.69	6.08	4.91	5.23	5.07	5.78	4.88	5.24		
	No. W10	No. W11	No. W12	No. W13							0.30
	5.79	6.28	5.46	4.62							

Setting Air Fresh No. -

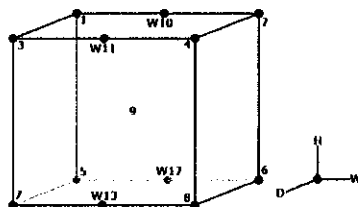

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. AD2202-080-0001 for Digital Thermometer with Probe (Agilent) Module 1 (245) Serial No. US37005130, Due 04-Aug-22

Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.


2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.

3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The uncertainty of measurement is included temperature stability.

5. The temperature uniformity, stability, overall variation and indicating temperature is applicable to all air or gas filled temperature controlled enclosures at atmospheric pressure.

End of Certificate



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160

Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : SS2206-022-0004

Date Issued : 10-Jun-22

Customer : OKLA TESTING & CONSULTING SERVICE CO.,LTD
63/13 Soi.Petchkasem 7, Petchkasem Rd., Thapra, Bangkok Yai,
Bangkok 10600

Equipment : Hot Air Oven

Manufacturer : KWF

Model : S0V70B

Serial No. : KWF2021021902

ID No./Tag No. : -

Date Received : 03-Jun-22

Date Calibrated : 03-Jun-22

Calibrated by : Mr. Nirot Parnkamnoed

Calibration Method or Calibration Procedure Used

Standard method : CP-05 TLAS G-20.


This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

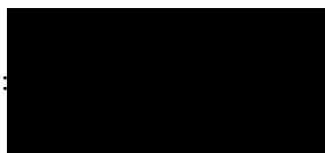

(um)



Page 1 of 2

Certificate No. : SS2206-022-0004

Environment : Ambient Temperature : Start record 25.5 °C, Stop record 25.7 °C
Relative Humidity : Start record 54.6 %RH, Stop record 54.7 %RH


Calibration Temperature (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Stability ¹ (°C)	Measured Uniformity ² (°C)	Overall Variation ³ (°C)
104	104.0	104.0	0.21	0.62	0.82
140	140.0	140.0	0.23	0.82	0.94
160	160.0	160.0	0.21	1.39	1.68
180	180.0	180.0	0.34	1.30	1.81

Without adjustment

Calibration Temperature (°C)	STD No. 1 (°C)	STD No. 2 (°C)	STD No. 3 (°C)	STD No. 4 (°C)	STD No. 5 (°C)	STD No. 6 (°C)	STD No. 7 (°C)	STD No. 8 (°C)	STD No. 9 (°C)	Uncertainty ⁴ ±°C
104	104.56	104.42	104.30	104.43	104.54	104.68	104.34	104.68	104.81	0.95
140	140.25	140.43	140.58	140.51	140.55	140.65	140.32	140.68	140.04	1.0
160	160.16	160.62	160.39	160.55	159.32	160.51	159.73	160.44	159.45	1.1
180	180.50	180.66	180.50	180.45	179.48	180.40	179.69	180.13	179.59	1.1

Note : Probe No. 9 is Reference Probe

Setting Air Fresh No. -



Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. AD2202-084-0002 for Data Acquisition Module 2 TC type T Serial No. US37003770, Due 08-Aug-22

Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.

2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.


3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The uncertainty of measurement is included temperature stability.

5. The temperature uniformity, stability, overall variation and indicating temperature is applicable to all air or gas filled temperature controlled enclosures at atmospheric pressure.

End of Certificate

Page 2 of 2



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : SS2206-022-0008

Date Issued : 10-Jun-22

Customer : OKLA TESTING & CONSULTING SERVICE CO.,LTD
63/13 Soi.Petchkasem 7, Petchkasem Rd., Thapra, Bangkok Yai,
Bangkok 10600

Equipment : Incubator

Manufacturer : S-Cool

Model : SM 61 M

Serial No. : 18021147

ID No./Tag No. : -

Date Received : 03-Jun-22

Date Calibrated : 03-Jun-22

Calibrated by : Mr. Nirot Parnkamnoed

Calibration Method or Calibration Procedure Used

Standard method : CP-05 TLAS G-20.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by



(um)



Page 1 of 2

Certificate No. : SS2206-022-0008

Environment : Ambient Temperature : Start record 25.5 °C, Stop record 25.6 °C
Relative Humidity : Start record 54.5 %RH, Stop record 54.6 %RH


Calibration Temperature (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Stability ¹ (°C)	Measured Uniformity ² (°C)	Overall Variation ³ (°C)
20	20.0	20.0	0.08	0.76	1.11

Without adjustment

Calibration Temperature (°C)	STD No. 1 (°C)	STD No. 2 (°C)	STD No. 3 (°C)	STD No. 4 (°C)	STD No. 5 (°C)	STD No. 6 (°C)	STD No. 7 (°C)	STD No. 8 (°C)	STD No. 9 (°C)	Uncertainty ⁴ ±°C
20	19.47	19.38	19.65	19.80	19.39	20.25	19.26	19.95	20.00	0.25

Note : Probe No. 9 is Reference Probe

Setting Air Fresh No. -



Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. AD2111-076-0001 for Digital Thermometer with Probe (Agilent) Module 1 (08) NTC & Pt1000 Serial No. MY44000197, Due 05-Jun-22

Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.

2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.

3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The uncertainty of measurement is included temperature stability.

5. The temperature uniformity, stability, overall variation and indicating temperature is applicable to all air or gas filled temperature controlled enclosures at atmospheric pressure.

End of Certificate

Page 2 of 2



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : SS2206-022-0007

Date Issued : 10-Jun-22

Customer : OKLA TESTING & CONSULTING SERVICE CO.,LTD
63/13 Soi.Petchkasem 7, Petchkasem Rd., Thapra, Bangkok Yai,
Bangkok 10600

Equipment : Water Bath

Manufacturer : Labtech

Model : LWB-222A

Serial No. : BCCLJ23001C

ID No./Tag No. : -

Date Received : 03-Jun-22

Date Calibrated : 03-Jun-22

Calibrated by : Mr. Nirot Parnkamnoed

Calibration Method or Calibration Procedure Used

In-house method : CP-14 base on ASTM E 715-80 (Reapproved 2011).


This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

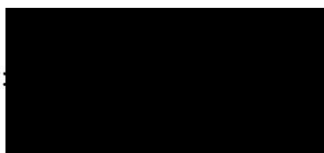

(um)



Page 1 of 2

Certificate No. : SS2206-022-0007


Environment : Ambient Temperature : Start record 25.4 °C, Stop record 25.5 °C
Relative Humidity : Start record 54.5 %RH, Stop record 54.5 %RH

Calibration Temperature (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Stability ¹ (°C)	Measured Uniformity ² (°C)	Overall Variation ³ (°C)
60	60	60	0.24	1.02	1.03

Without adjustment

Calibration Temperature (°C)	STD No. 1 (°C)	STD No. 2 (°C)	STD No. 3 (°C)	STD No. 4 (°C)	STD No. 5 (°C)	Uncertainty ⁴ ±°C
60	61.20	61.18	61.11	61.20	61.59	0.40

Note : Probe No. 5 is Reference Probe

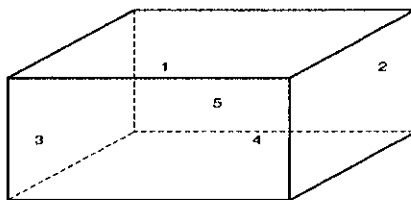

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. AD2111-076-0001 for Digital Thermometer with Probe (Agilent) Module 1 (08) NTC & Pt1000
Serial No. MY44000197, Due 05-Jun-22

- Notes :
1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.
 2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.
 3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.
 4. The uncertainty of measurement is included temperature stability.

End of Certificate

Page 2 of 2