

ภาคผนวกที่ 4

เอกสารสอบเทียบเครื่องมือ



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Rayong Lab	pH at 25 °C	pH meter	RYG_EN0183	27-Feb-23	27-Feb-24	12
Rayong Lab	BOD	DO meter with Sensor	RYG_EN0140	21-Nov-22	21-May-24	18
Rayong Lab	BOD	Incubator	RYG_EN0154	22-Apr-22	21-Oct-23	18
Rayong Lab	Total Suspended Solids	Electronic Balance	RYG_EN0002	1-Mar-23	1-Mar-24	12
Rayong Lab	Total Suspended Solids	Hot Air Oven	RYG_EN0010	20-Oct-22	20-Apr-24	18
Rayong Lab	Oil & Grease	Electronic Balance	RYG_EN0002	1-Mar-23	1-Mar-24	12
Rayong Lab	Oil & Grease	Hot Air Oven	RYG_EN0006	20-Oct-22	20-Apr-24	18
Rayong Lab	Oil & Grease	Water Bath	RYG_EN0061	20-Oct-22	20-Apr-24	18
Rayong Lab	Ammonia Nitrogen	SPECTROPHOTOMETER	RYG_EN0037	27-Sep-22	27-Mar-24	18
Rayong Lab	Nitrate	Spectrophotometer	RYG_EN0037	27-Sep-22	27-Mar-24	18
Rayong Lab	Nitrite	Spectrophotometer	RYG_EN0037	27-Sep-22	27-Mar-24	18
Rayong Lab	Salinity	Conductivity meter	RYG_EN0029	23-Feb-22	24-Aug-23	18
Rayong Lab	Total Kjeldahl Nitrogen	Block Digestion Unit	RYG_EN0188	15-Mar-23	15-Mar-24	12
Rayong Lab	Total Kjeldahl Nitrogen	pH Meter	RYG_EN0152	22-Dec-22	22-Dec-23	12
Rayong Lab	Total Nitrogen	Spectrophotometer	RYG_EN0037	27-Sep-22	27-Mar-24	18
Water Lab	Total Phosphorus	Digestion Unit	BKK_EN0366	30-Jun-22	30-Jun-23	12
Water Lab	Total Phosphorus	Discrete analyzer	BKK_EN0037	5-Jan-23	5-Jan-24	12
Water Lab	Sulfide	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Sulfide	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Copper	ICP-MS	BKK_EL0026	14-Jun-22	14-Dec-23	18
Water Lab	Copper	Hot Block	BKK_EL0054	7-Apr-22	7-Oct-23	18
Water Lab	Copper	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Zinc	ICP-MS	BKK_EL0026	14-Jun-22	14-Dec-23	18
Water Lab	Zinc	Hot Block	BKK_EL0054	7-Apr-22	7-Oct-23	18
Water Lab	Zinc	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Total Coliform	Autoclave	BKK_ML0041	20-May-22	20-Nov-23	18
Water Lab	Total Coliform	Incubator	BKK_ML0010	21-Jan-22	22-Jul-23	18
Water Lab	Total Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Fecal Coliform	Autoclave	BKK_ML0041	20-May-22	20-Nov-23	18
Water Lab	Fecal Coliform	Incubator	BKK_ML0010	21-Jan-22	22-Jul-23	18
Water Lab	Fecal Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Fecal Coliform	Water Bath	BKK_ML0056	20-May-22	20-May-23	12



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Rayong Lab	pH at 25 °C	pH meter	RYG_EN0183	27-Feb-23	27-Feb-24	12
Rayong Lab	BOD	DO meter with Sensor	RYG_EN0140	21-Nov-22	21-May-24	18
Rayong Lab	BOD	Incubator	RYG_EN0154	22-Apr-22	21-Oct-23	18
Rayong Lab	Total Suspended Solids	Electronic Balance	RYG_EN0002	1-Mar-23	1-Mar-24	12
Rayong Lab	Total Suspended Solids	Hot Air Oven	RYG_EN0010	20-Oct-22	20-Apr-24	18
Rayong Lab	Oil & Grease	Electronic Balance	RYG_EN0002	1-Mar-23	1-Mar-24	12
Rayong Lab	Oil & Grease	Hot Air Oven	RYG_EN0006	20-Oct-22	20-Apr-24	18
Rayong Lab	Oil & Grease	Water Bath	RYG_EN0061	20-Oct-22	20-Apr-24	18
Rayong Lab	Ammonia Nitrogen	SPECTROPHOTOMETER	RYG_EN0037	27-Sep-22	27-Mar-24	18
Rayong Lab	Nitrate	Spectrophotometer	RYG_EN0037	27-Sep-22	27-Mar-24	18
Rayong Lab	Nitrite	Spectrophotometer	RYG_EN0037	27-Sep-22	27-Mar-24	18
Rayong Lab	Salinity	Conductivity meter	RYG_EN0029	23-Feb-22	24-Aug-23	18
Rayong Lab	Total Kjeldahl Nitrogen	Block Digestion Unit	RYG_EN0188	15-Mar-23	15-Mar-24	12
Rayong Lab	Total Kjeldahl Nitrogen	pH Meter	RYG_EN0152	22-Dec-22	22-Dec-23	12
Rayong Lab	Total Nitrogen	Spectrophotometer	RYG_EN0037	27-Sep-22	27-Mar-24	18
Water Lab	Total Phosphorus	Digestion Unit	BKK_EN0366	30-Jun-22	30-Jun-23	12
Water Lab	Total Phosphorus	Discrete analyzer	BKK_EN0037	5-Jan-23	5-Jan-24	12
Water Lab	Sulfide	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Sulfide	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Copper	ICP-MS	BKK_EL0026	14-Jun-22	14-Dec-23	18
Water Lab	Copper	Hot Block	BKK_EL0054	7-Apr-22	7-Oct-23	18
Water Lab	Copper	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Zinc	ICP-MS	BKK_EL0026	14-Jun-22	14-Dec-23	18
Water Lab	Zinc	Hot Block	BKK_EL0054	7-Apr-22	7-Oct-23	18
Water Lab	Zinc	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Total Coliform	Autoclave	BKK_ML0041	20-May-22	20-Nov-23	18
Water Lab	Total Coliform	Incubator	BKK_ML0010	21-Jan-22	22-Jul-23	18
Water Lab	Total Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Fecal Coliform	Autoclave	BKK_ML0041	20-May-22	20-Nov-23	18
Water Lab	Fecal Coliform	Incubator	BKK_ML0010	21-Jan-22	22-Jul-23	18
Water Lab	Fecal Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Fecal Coliform	Water Bath	BKK_ML0056	20-May-22	20-May-23	12



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CH275

Page.: 1 of 3

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	SevenCompact S220
Serial No. :	C104059460
ID No. :	RYG_EN0183
Condition As-Received:	Used Item
Received Date :	24 February 2023
Calibration Date :	27 February 2023
Reference :	2302-0886DSC-2
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer

REVIEW BY	N. Banrit
APPROVED BY	D. [Signature]
NEXT CAL. DATE	27/2/24

Calibrated by : Walalak Sirithean

Approved by :

Saithip
Approved Signatory

- () Malee Butkruea
(✓) Saithip Meangmai
() Warakorn Lerngagtrakul

Issue Date : 28 February 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0051538



Cert.No.: 23CH275

Page.: 3 of 3

Calibration Results**Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: 1453404	4.008	4.008	179.1	0.0046	2.00
	6.987	6.988	4.7	0.0084	2.00
	10.010	10.013	-172.4	0.0069	2.00

Function : Temperature Measurement**(*) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : InLabExpert Pro-ISM

- Serial No. : 1453404

Dimension of probe;

- Length : 120 mm.

- Diameter : 12 mm.

- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement ($\pm$ °C)	Coverage factor k
25.0	25.001	24.8	-0.201	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Sauhin

a 1149924



Cert. No.: 23E753

Page.: 2 of 2

Result of calibration :- (*) Without adjustment () After adjustment

Function:	DC voltage measuremer	Range:	2000	mV	
<u>Standard Value</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>		
(mV)	(mV)	(mV)	($\pm$ μ V)		
-200.0000	-200.0	0.0	72		
-150.0000	-150.0	0.0	69		
-100.0000	-100.0	0.0	65		
-50.0000	-50.0	0.0	62		
0.0000	0.0	0.0	58		
50.0000	50.0	0.0	62		
100.0000	99.9	-0.1	65		
150.0000	149.9	-0.1	69		
200.0000	199.9	-0.1	72		

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %

UUC* = Unit Under Calibration.

-o0o-



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2111-0709DSC-2

Cert. No.: 22LM163

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1523	3240076	22I249	02 Mar 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 16C100647

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.003	19.88	-0.123	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Mulu.



Cert.No.: 22TW260

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**

Dissolved Oxygen Probe No.: 16C100647

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.12	8.12	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Malu .

a 1136620



Equipment : Low Temp. Incubator

Condition As-Received : Used Item

Reference : 2204-0146OC-1

Cert. No.: 22TM317

Page.: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44031769	21LM12	02 Sep 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

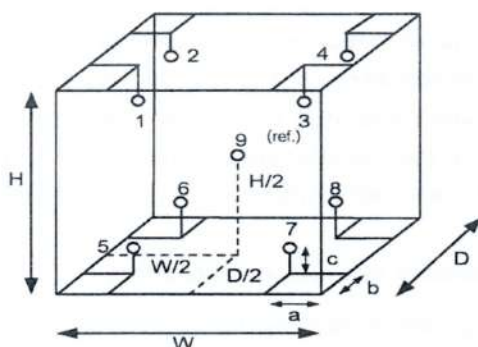

Environment during calibration		
	Beginning	Finished
Temp. (°C)	25	25
REL.Humid. (%)	54	58
AC Supply (Volt)	221	223

Position :	Ref. Std. ID No.:
1	9RTD-2/1
2	9RTD-2/2
3	9RTD-2/3
4	9RTD-2/4
5	9RTD-2/5
6	9RTD-2/6
7	9RTD-2/7
8	9RTD-2/8
9 (ref.)	9RTD-2/9

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.60 m
W = 1.0 m
H = 1.2 m
Capacity = 0.75 m³

Malu

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com



NSC-TISI-TIS 17025

CALIBRATION 0426

SARTORIUS

Certificate

of Calibration

REVIEW BY	Thantall.
APPROVED BY	D. [Signature]
NEXT CAL. DATE	01/03/24

Model Number : MSE224S-100-DU

Description : Analytical Balance

Serial Number : 0026207038

ID No. : RYG_EN0002

Manufacturer : Sartorius

Certificate No. : 23BCI0112

Issued Date : Friday, March 03, 2023

Reference No. : 204833

Page No. : 1 of 2

Customer Name : ALS Laboratory Group (Thailand) Co., Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated Place : ALS Laboratory Group (Thailand) Co., Ltd.(Balance Room)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong.21140, Thailand.

Calibrated By : Mr.Chonchai Inthana

Calibration Date : Wednesday, March 01, 2023

Calibration
 Procedure No. : This calibration was conducted by
Using in-house calibration procedure number (WI-003)
Based on UKAS LAB 14 : 2019

Metrological data :

Capacity : 220 g Readability : 0.0001 g

Ambients Conditions:

Temperature : 23.6 °C ± 5.0 °C

Humidity : 60.0 % RH ± 10.0 % RH

Pressure : ±

Reasons for calibration

☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance

Equipment Condition: ☒ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

Mr.chonchai Inthana(Technical Manager)

S
T
A
M
P



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1517

Page : 1 of 3

Certificate of Calibration

Equipment :	Hot Air Oven	REVIEW BY <i>Thanitall</i> APPROVED BY <i>D. [Signature]</i> NEXT CAL. DATE <i>30/04/24</i>
Manufacturer :	Memmert	
Model :	UFE 500	
Serial No. :	G511.1572	
ID No. :	RYG_EN0010	
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng, Rayong 21140 Thailand	
Location :	Oven Room	
Received Order :	20 October 2022	
Calibration Date :	20 October 2022	
Ambient Temperature :	(26 ± 10) °C	
Relative Humidity :	(50 ± 30) %	
Calibrated by :	Man Pattanapongpaiboon	

Approved by :

Malu

Approved Signatory

- () Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date :

2 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2210-03760C-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 22TM1517

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
104.0	104.0	104.0	0.076	0.52	0.60	0.42	2
180.0	180.0	180.0	0.13	0.88	1.2	1.1	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	103.768	103.734	103.723	103.800	104.215	104.131	104.132	103.740	103.747
180.0	179.723	179.359	179.439	179.489	180.361	180.114	180.131	180.243	179.605

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu .



Equipment : Hot Air Oven
 Condition As-Received : Used Item
 Reference : 2210-0376OC-1

Cert. No.: 22TM1492

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Data Acquisition	34970A	MY44035217	21LM30	23 Dec 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	29
REL.Humid. (%)	43	47
AC Supply (Volt)	220	221

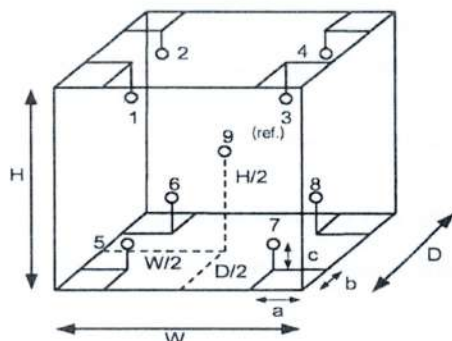

Position :	Ref. Std. ID No.:
1	18-10RTD-01
2	18-10RTD-02
3	18-10RTD-03
4	18-10RTD-04
5	18-10RTD-05
6	18-10RTD-06
7	18-10RTD-07
8	18-10RTD-08
9 (ref.)	18-10RTD-09

Probe Installation Details :

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of Chamber :

D = 0.33 m
 W = 0.40 m
 H = 0.40 m
 Capacity = 0.053 m³

Manu .



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1491

Page : 1 of 3

Certificate of Calibration

Equipment :	Water Bath
Manufacturer :	Memmert
Model :	WNB22
Serial No. :	L513.0648
ID No. :	RYG_EN0061
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5, T. Maenam Khu, A. Pluakdaeng, Rayong 21140, Thailand
Location :	Wet Chemistry Lab
Received Order :	20 October 2022
Calibration Date :	20 October 2022
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Preecha Hlahib

Approved by :

Approved Signatory

- () Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date :

2 November 2022

The Uncertainties are for a confidence probability of approximately 95 %

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2210-0376OC-4
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 22TM1491

Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)				
			Position				
			1	2	3	4	5 (ref.)
85.0	85.0	85.0	84.527	84.563	84.628	84.516	84.580

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
85.0	0.12	0.081	0.18	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu

Calibration Results:
Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.4	0.21	0.14
536.66	536.7	-0.04	0.14
637.98	638.3	-0.32	0.14
748.48	748.8	-0.32	0.14
807.03	807.4	-0.37	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.5605	0.563	-0.0025	0.0045
	0.7334	0.737	-0.0036	0.0045
	1.0534	1.057	-0.0036	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.5503	0.553	-0.0027	0.0045
	0.7179	0.720	-0.0021	0.0045
	1.0312	1.034	-0.0028	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.5024	0.506	-0.0036	0.0045
	0.6693	0.672	-0.0027	0.0045
	0.9604	0.964	-0.0036	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.5168	0.519	-0.0022	0.0045
	0.6903	0.691	-0.0007	0.0045
	0.9904	0.992	-0.0016	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.5525	0.554	-0.0015	0.0045
	0.7175	0.718	-0.0005	0.0045
	1.0301	1.031	-0.0009	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.5367	0.538	-0.0013	0.0045
	0.6847	0.685	-0.0003	0.0046
	0.9823	0.983	-0.0007	0.0045



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CH275

Page.: 1 of 3

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	SevenCompact S220
Serial No. :	C104059460
ID No. :	RYG_EN0183
Condition As-Received:	Used Item
Received Date :	24 February 2023
Calibration Date :	27 February 2023
Reference :	2302-0886DSC-2
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer

REVIEW BY	<i>N. B. Mit</i>
APPROVED BY	<i>D. [Signature]</i>
NEXT CAL. DATE	27/2/24

Calibrated by : Walalak Sirithean

Approved by :

Saithip
Approved Signatory

- () Malee Butkruea
(✓) Saithip Meangmai
() Warakorn Lernagtrakul

Issue Date : 28 February 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0051538



Cert.No.: 23CH275

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	22E2769	24 Aug 2023
2) Ref. Standard Thermometer	4982054	110RC044	22I1306	27 Oct 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	826588	09 July 2024
pH 6.987	CPA chem	826589	09 July 2023
pH 10.010	CPA chem	863835	28 Dec 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ($\pm$ mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: C104059460	4.000	177.48	177.4	4.000	0.058	2.00
	7.000	0.00	-0.1	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Saithip

a 1149925



Cert.No.: 23CH275

Page.: 3 of 3

Calibration Results**Function : pH Measurement****Performing three buffers standard curve by using buffer nominal pH (4,7,10)**

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: 1453404	4.008	4.008	179.1	0.0046	2.00
	6.987	6.988	4.7	0.0084	2.00
	10.010	10.013	-172.4	0.0069	2.00

Function : Temperature Measurement**(*) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : InLabExpert Pro-ISM
- Serial No. : 1453404

Dimension of probe;

- Length : 120 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement ($\pm$ °C)	Coverage factor k
25.0	25.001	24.8	-0.201	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Saitip

a 1149924



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 23E753

Page : 1 of 2

Equipment : pH Meter
Manufacturer: Mettler Toledo
Model : SevenCompact S220
Serial No.: C104059460
ID No.: RYG_EN0183
Condition As-Received: Used Item
Received Date: 24 February 2023
Calibration Date: 28 February 2023

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Reference: 2302-0886DSC
Ambient Temperature: (23 $\pm$ 2) °C
Relative Humidity: (50 $\pm$ 10) %

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Procedure used: Calibration were conducted using In-house calibration Procedure CP-E17 According to direct measurement method with Multi-Product Calibrator.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Multi-Product Calibrator	5500A	6440007	22E1670	18 May 2023

2.This result of calibration was made on requested at the point specified by customer.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Wutchareeporn Wongchutikrane
Issue Date : 02 March 2023

Approved Signatory :


[] Phalinee Prabpaipal
[x] Nuntawat Khamchai
[] Pornthippa Tameyakul

B 0309672



Cert. No.: 23E753

Page.: 2 of 2

Result of calibration :- (*) Without adjustment () After adjustment

Function:	DC voltage measuremer	Range:	2000	mV	
<u>Standard Value</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>		
(mV)	(mV)	(mV)	($\pm \mu V$)		
-200.0000	-200.0	0.0	72		
-150.0000	-150.0	0.0	69		
-100.0000	-100.0	0.0	65		
-50.0000	-50.0	0.0	62		
0.0000	0.0	0.0	58		
50.0000	50.0	0.0	62		
100.0000	99.9	-0.1	65		
150.0000	149.9	-0.1	69		
200.0000	199.9	-0.1	72		

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %

UUC* = Unit Under Calibration.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22LM163

Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5100

Serial No. : 15L102139

ID No. : RYG_EN0140

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Rayong Branch
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng,

Location : TPA Chemistry Calibration Lab.2

Received Order : 18 November 2022

Calibrated Date : 21 November 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lernagtrakul

Approved by : Malee Butkruea
Approved Signatory

() Pornthippa Tameyakul
(/) Malee Butkruea
() Suwit Imjai

Issue Date : 22 November 2022

REVIEW BY	<u>N. Bannet</u>
APPROVED BY	<u>D. [Signature]</u>
NEXT CAL. DATE	<u>21/05/24</u>

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0047730



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2111-0709DSC-2

Cert. No.: 22LM163

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1523	3240076	221249	02 Mar 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 16C100647

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.003	19.88	-0.123	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Mulu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 22TW260

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5100
Serial No. :	15L102139
ID No. :	RYG_EN0140
Received Date :	18 November 2022
Test Date :	21 November 2022
Reference :	2211-0709DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	 _____ Approved Signatory
(☒) Malee Butkruea	
(☐) Saithip Meangmai	
(☐) Warakorn Lernagtrakul	
Issue Date :	22 November 2022



Cert.No.: 22TW260

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 16C100647

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.12	8.12	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Malu .

a 1136620



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM317

Page.: 1 of 3

Certificate of Calibration

Equipment : Low Temp. Incubator

Manufacturer : Memmert

Model : IPP750

Serial No. : V818.0084

ID No. : RYG_EN0154

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
(Rayong Branch)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand

Location : BOD Room

Received Order : 22 April 2022

Calibration Date : 22 April 2022

Ambient Temperature : (26 $\pm$ 10) °C

Relative Humidity : (50 $\pm$ 30) %

Calibrated by : Man Pattanapongpaiboon

REVIEW BY	<i>N. Banwit</i>
APPROVED BY	<i>D. [Signature]</i>
NEXT CAL. DATE	21/10/23

Approved by :

Malee
Approved Signatory

- () Pornthippa Tameyakul
(/) Malee Butkruea
() Suwit Imjai

Issue Date : 3 May 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0040735



Equipment : Low Temp. Incubator
 Condition As-Received : Used Item
 Reference : 2204-0146OC-1

Cert. No.: 22TM317
 Page.: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement
 The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44031769	21LM12	02 Sep 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	25	25
REL.Humid. (%)	54	58
AC Supply (Volt)	221	223

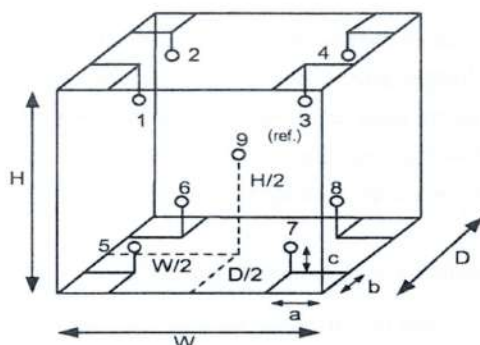

Position :	Ref. Std. ID No.:
1	9RTD-2/1
2	9RTD-2/2
3	9RTD-2/3
4	9RTD-2/4
5	9RTD-2/5
6	9RTD-2/6
7	9RTD-2/7
8	9RTD-2/8
9 (ref.)	9RTD-2/9

Probe Installation Details :

a = 10 cm
 b = 10 cm
 c = 10 cm

Dimension of Chamber :

D = 0.60 m
 W = 1.0 m
 H = 1.2 m
 Capacity = 0.75 m³

Malu



Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2204-0146OC-1
Result of Calibration :- (*) Without Adjustment

Cert. No.: 22TM317

Page.: 3 of 3

Function of UUC* : Temperature Source

Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
20.0	20.0	20.0	0.022	0.20	0.22	0.30	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
20.0	20.209	20.174	20.199	20.110	20.075	20.062	20.027	20.069	20.030

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu .

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com

**SARTORIUS**

Certificate

of Calibration

REVIEW BY	Thavitall.
APPROVED BY	D. [Signature]
NEXT CAL. DATE	01/03/24

Model Number : MSE224S-100-DUCertificate No. : 23BCI0112Description : Analytical BalanceIssued Date : Friday, March 03, 2023Serial Number : 0026207038Reference No. : 204833ID No. : RYG_EN0002Manufacturer : SartoriusPage No. : 1 of 2Customer Name : ALS Laboratory Group (Thailand) Co., Ltd. (Rayong Branch)616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.Calibrated Place : ALS Laboratory Group (Thailand) Co., Ltd.(Balance Room)616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong.21140, Thailand.Calibrated By : Mr.Chonchai InthanaCalibration Date : Wednesday, March 01, 2023

Calibration

Procedure No. : This calibration was conducted byUsing in-house calibration procedure number (WI-003)Based on UKAS LAB 14 : 2019**Metrological data :**Capacity : 220 g Readability : 0.0001 g**Ambients Conditions:**Temperature : 23.6 °C ± 5.0 °CHumidity : 60.0 % RH ± 10.0 % RHPressure : ± **Reasons for calibration**
☐ New Installation
 ☐ Service / Repaired
 ☒ Re-calibration/ Maintenance
Equipment Condition: ☒ Good Operate ☐ Fair**Measurement Method UKAS Publication Ref :Lab 14**

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division
Sartorius (Thailand) Co., Ltd.

Mr.chonchai Inthana(Technical Manager)

S
T
A
M
P

Certificate of Calibration

Model Number : MSE224S-100-DU

Certificate No. : 23BCI0112

Description : Analytical Balance

Issued Date : Friday, March 03, 2023

Serial Number : 0026207038

Reference No. : 204833

ID No. : RYG_EN0002

Manufacturer : Sartorius

Page No. : 2 of 2

Calibration Results : Without Adjustment

Repeatability



The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	199.9999
20 g	20.0000	200.0000
Tolerance	20.0000	199.9999
0.0001 g	20.0000	200.0000
	20.0000	199.9999
Nominal Value : (High Load)	20.0000	199.9999
200 g	19.9999	200.0000
Tolerance	20.0000	200.0000
0.0001 g	20.0000	199.9999
	20.0000	200.0000
Standard Deviation	0.00003	0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 100 g
Tolerance 0.0004 g



	Difference
1	-
2	-0.0001
3	-0.0001
4	0.0001
5	0.0002
6	-

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00014
0.05	0.0500	0.0500	0.0000	0.00014
0.1	0.1000	0.1000	0.0000	0.00014
0.5	0.5000	0.5000	0.0000	0.00014
1	1.0000	1.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0001	0.0001	0.00014
20	20.0000	20.0000	0.0000	0.00024
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	99.9999	-0.0001	0.00019
200	200.0000	200.0000	0.0000	0.00032

End of Report.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1517

Page : 1 of 3

Certificate of Calibration

Equipment :	Hot Air Oven
Manufacturer :	Memmert
Model :	UFE 500
Serial No. :	G511.1572
ID No. :	RYG_EN0010
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng, Rayong 21140 Thailand
Location :	Oven Room
Received Order :	20 October 2022
Calibration Date :	20 October 2022
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Man Pattanapongpaiboon

REVIEW BY	Thanitall.
APPROVED BY	D. [Signature]
NEXT CAL. DATE	20/04/24

Approved by :

Approved Signatory

- () Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date :

2 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Hot Air Oven
 Condition As-Received : Used Item
 Reference : 2210-0376OC-2

Cert. No.: 22TM1517
 Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY49023932	22LM97	29 Jul 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

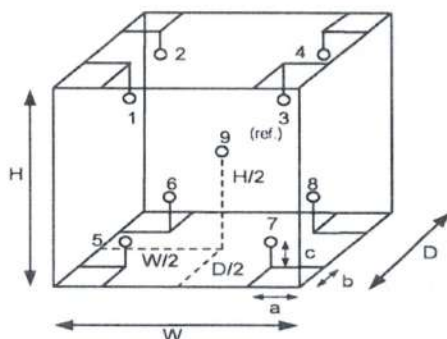

Environment during calibration		
	Beginning	Finished
Temp. (°C)	25	25
REL.Humid. (%)	54	59
AC Supply (Volt)	223	225

Ref. Std. ID No.: @ Calibration Point

Position :	(180) °C	(104) °C
1	21-16TC-01	20-16RTD-01
2	21-16TC-02	20-16RTD-02
3	21-16TC-03	20-16RTD-03
4	21-16TC-04	20-16RTD-04
5	21-16TC-05	22-16RTD-05
6	21-16TC-06	20-16RTD-06
7	21-16TC-07	20-16RTD-07
8	21-16TC-08	22-16RTD-08
9 (ref.)	21-16TC-09	22-16RTD-09

Probe Installation Details :

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of Chamber :

D = 0.40 m
 W = 0.56 m
 H = 0.48 m
 Capacity = 0.11 m³

Malu



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2210-0376OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 22TM1517

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
104.0	104.0	104.0	0.076	0.52	0.60	0.42	2
180.0	180.0	180.0	0.13	0.88	1.2	1.1	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	103.768	103.734	103.723	103.800	104.215	104.131	104.132	103.740	103.747
180.0	179.723	179.359	179.439	179.489	180.361	180.114	180.131	180.243	179.605

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Mulu



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1492

Page : 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Memmert

Model : UM 400

Serial No. : b495.0899

ID No. : RYG_EN0006

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5, T. Maenam Khu,
A. Pluakdaeng,
Rayong 21140, Thailand

Location : Oven Room

Received Order : 20 October 2022

Calibration Date : 20 October 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Preecha Hlahib

Approved by :

Malu
Approved Signatory

() Pornthippa Tameyakul

(✓) Malee Butkruea

() Suwit Imjai

Issue Date : 2 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2210-0376OC-1
Procedure Used :-

Cert. No.: 22TM1492

Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44035217	21LM30	23 Dec 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	29
REL.Humid. (%)	43	47
AC Supply (Volt)	220	221

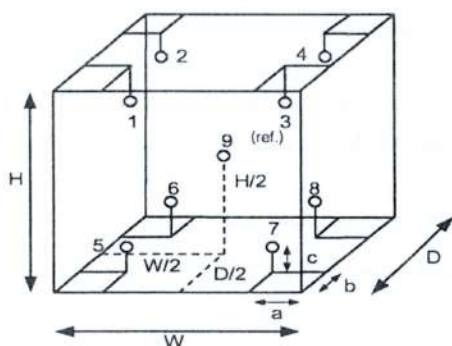

Probe Installation Details :

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :

D = 0.33 m
W = 0.40 m
H = 0.40 m
Capacity = 0.053 m³

Position :	Ref. Std. ID No.:
1	18-10RTD-01
2	18-10RTD-02
3	18-10RTD-03
4	18-10RTD-04
5	18-10RTD-05
6	18-10RTD-06
7	18-10RTD-07
8	18-10RTD-08
9 (ref.)	18-10RTD-09

Mah.



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2210-0376OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 22TM1492

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
70.0	70.0	70.0	0.079	0.47	0.77	0.42	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
70.0	70.262	69.995	70.079	70.177	70.664	70.039	70.688	70.149	70.328

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-27 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 22TM1491

Page : 1 of 3

Certificate of Calibration

Equipment : Water Bath

Manufacturer : Memmert

Model : WNB22

Serial No. : L513.0648

ID No. : RYG_EN0061

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5, T. Maenam Khu,
A. Pluakdaeng,
Rayong 21140, Thailand

Location : Wet Chemistry Lab

Received Order : 20 October 2022

Calibration Date : 20 October 2022

Ambient Temperature : (26 $\pm$ 10) °CRelative Humidity : (50 $\pm$ 30) %

Calibrated by : Preecha Hlahib

Approved by :

Approved Signatory

() Pornthippa Tameyakul

(✓) Malee Butkruea

() Suwit Imjai

Issue Date : 2 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2210-0376OC-4

Cert. No.: 22TM1491
 Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Data Acquisition	34970A	MY44035217	21LM30	23 Dec 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

	<u>Environmental</u>		<u>AC Voltage Supply</u>
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	24	53	222
Finished of Calibration	24	50	221

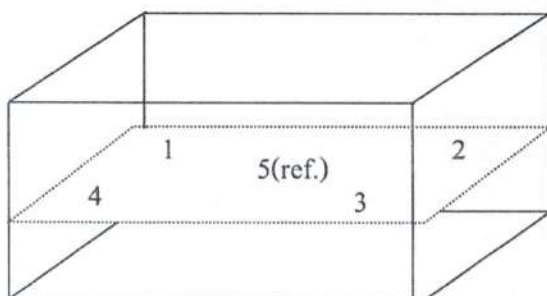

Front

<u>Position :</u>	<u>Ref. Std. S/N.:</u>
1	N37P300726
2	N37P300727
3	N37P300728
4	N37P300729
5(ref.)	N37P300730

Mala



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2210-0376OC-4
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 22TM1491

Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)				
			Position				
			1	2	3	4	5 (ref.)
85.0	85.0	85.0	84.527	84.563	84.628	84.516	84.580

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
85.0	0.12	0.081	0.18	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.

a 1132470



Certificate of Calibration

Equipment:	SPECTROPHOTOMETER	Certificate No.:	C06220464
Model:	DR6000	Issued Date:	27 September 2022
Serial No. (or ID.):	1627845 (RYG_EN0037)	Job No.:	KSPR2212224
Manufacturer:	HACH	Page:	1 of 3
Condition:	In Condition		

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

REVIEW BY	<i>N. Banjit</i>
APPROVED BY	<i>D. Pongngam</i>
NEED CAL. DATE	27/3/24
	3.2 %RH

Environment Condition:

Temperature	23.1	°C	±
Humidity	65.4	%RH	±

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) (Wet Chemistry)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By: Mr. Chattuphon Foithong

Calibration Date: 27 September 2022

The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04

Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 91418 and 91435
The standard for Photometric Certificate No. 91441 and 101088
The standard for Stray light Certificate No. 101041 and 101040
The standard for Spectral resolution Certificate No. 101037

(Signature)
(Mr. Chattuphon Foithong)
Person in charge

(Signature)
(Mr. Thalerngkeat Pongngam)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

DKSH Technology Limited

2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260

2533 Sukhumvit Road, Bangchak, Phraekhanong, Bangkok 10260

Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.4	0.21	0.14
536.66	536.7	-0.04	0.14
637.98	638.3	-0.32	0.14
748.48	748.8	-0.32	0.14
807.03	807.4	-0.37	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.5605	0.563	-0.0025	0.0045
	0.7334	0.737	-0.0036	0.0045
	1.0534	1.057	-0.0036	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.5503	0.553	-0.0027	0.0045
	0.7179	0.720	-0.0021	0.0045
	1.0312	1.034	-0.0028	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.5024	0.506	-0.0036	0.0045
	0.6693	0.672	-0.0027	0.0045
	0.9604	0.964	-0.0036	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.5168	0.519	-0.0022	0.0045
	0.6903	0.691	-0.0007	0.0045
	0.9904	0.992	-0.0016	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.5525	0.554	-0.0015	0.0045
	0.7175	0.718	-0.0005	0.0045
	1.0301	1.031	-0.0009	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.5367	0.538	-0.0013	0.0045
	0.6847	0.685	-0.0003	0.0046
	0.9823	0.983	-0.0007	0.0045

Calibration Results:
Without Adjustment
Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7423	0.744	-0.0017	0.0083
257 nm	0.0000	0.000	0.0000	0.0080
	0.8609	0.861	-0.0001	0.0084
313 nm	0.0000	0.000	0.0000	0.0080
	0.2895	0.292	-0.0025	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6381	0.638	0.0001	0.0080

Stray light *

Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
260.67 +/- 0.11 nm	260.7	2.1	1.678
391.94 +/- 0.11 nm	391.9	1.7	1.770

Spectral Resolution *

Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength (nm)	268.60	266.63	1.39	2.00
UUC: Wavelength (nm)	268.2	266.1		
Std Absorbance (A)	0.4810	0.3176		
Absorbance (A)	0.373	0.268		

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: KSPR2212224

ชนิดเครื่องมือ: SPECTROPHOTOMETER

รุ่น: DR6000

หมายเลขเครื่อง: 1627845

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
27 Sep 2022			27 Sep 2022		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
☒	☐	1. ความสมบูรณ์เครื่อง	☒	☐	
☒	☐	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	☒	☐	
☒	☐	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swich)	☒	☐	
☒	☐	4. ปุ่มกด (Keypad)	☒	☐	
☒	☐	5. หน้าจอ (Display, Screen Contrast)	☒	☐	
		Spectrophotometer			
☐	☐	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	☐	☐	
☐	☐	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	☐	☐	
☒	☐	8. ความยาวคลื่น (Wavelength Check)	☒	☐	656.1 ได้ 656.1 nm
☒	☐	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	☒	☐	
☒	☐	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	☒	☐	
☒	☐	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	☒	☐	
		pH Meter and Conductivity Meter			
☐	☐	12. อิเล็กโทรด (Electrode and Connection Cable)	☐	☐	
☐	☐	13. ระดับสารละลายใน Electrode (Level KCl)	☐	☐	
☐	☐	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	☐	☐	
☐	☐	15. ขาจับอิเล็กโทรด (Stand)	☐	☐	
		Turbidimeter			
☐	☐	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	☐	☐	
☐	☐	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่นเกิน 3.0)	☐	☐	
		Automatic titrator			
☐	☐	18. สภาพ Piston Burettes	☐	☐	
☐	☐	19. Function Rinsing and Dosing	☐	☐	
☐	☐	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	☐	☐	

เพิ่มเติม/ข้อแนะนำ :

Mr. Chattuphon Foithong

Service Engineer



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CH283

Page.: 1 of 2

Certificate of Calibration

Equipment :	Conductivity Meter
Manufacturer :	Mettler Toledo
Model :	S230
Serial No. :	B241407147
ID No. :	RYG_EN0029
Condition As-Received:	Used Item
Received Date :	22 February 2022
Calibration Date :	23 February 2022
Reference :	2202-0732DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 $\pm$ 2.5) °C
Relative Humidity :	(50 $\pm$ 15) %
Calibration Procedure:	In -house method : - CP-CH6 : based on direct measurement by using certified reference material (CRM)
Calibrated by :	Walalak Sirithean



Approved by :

Malee

Approved Signatory

- (☒) Malee Butkruea
(☐) Saithip Meangmai
(☐) Warakorn Lerngagtrakul

Issue Date :

25 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 22CH283

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	9549224	130RC003	211451	15 Apr 2022

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
84.000 $\mu\text{S/cm}$	CPA Chem	754034	28 June 2022
1413.0 $\mu\text{S/cm}$	CPA Chem	766815	04 Sep 2022
12.880 mS/cm	CPA Chem	761022	02 Aug 2022

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results**Function : Conductivity Measurement**(*) After Adjustment at 1413.0 $\mu\text{S/cm}$

Conductivity Electrode Serial No.: 5821441030

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement ($\pm$)	Coverage factor k
84.000 $\mu\text{S/cm}$	82.4 $\mu\text{S/cm}$	84.4 $\mu\text{S/cm}$	0.62 $\mu\text{S/cm}$	2.00
1413.0 $\mu\text{S/cm}$	1375 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	9.2 $\mu\text{S/cm}$	2.00
12.880 mS/cm	12.54 mS/cm	12.81 mS/cm	0.086 mS/cm	2.00

Remark

- UUC* = Unit Under Calibration
- Cell constant = 0.555236 cm^{-1}

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Malu

a 1090534

Certificate of Calibration

Equipment:	Block Digestion Unit	Certificate No.:	C29230010
Model:	KT-20s	Issued Date:	18 March 2023
Serial No. (or ID.):	5720210009/5770200073	Job No.:	KSPR2304362
Manufacturer:	Gerhardt	Page:	1 of 4
Condition:	In Condition	Digestion Block:	20 holes.

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand.

Environment Condition:

Temperature:	25 °C	±	0.5 °C
Humidity:	65 %RH	±	3.7 %RH
Voltage:	231 VAC	±	3.1 VAC

REVIEW BY	<i>N. Banlert</i>
APPROVED BY	<i>D. Srichana</i>
NEXT CAL. DATE	15/03/24

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
(Wet Chemistry Lab)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand.

Calibration By: Mr. Nakarin Ruenros

Calibration Date: 15 March 2023

The Method used: In house method, base on by comparison with standard

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through N.M. Technical Center Laboratory (NTL)
Certificate No.: TC22/0080



(Mr. Nakarin Ruenros)
Person in charge



(Mr. Udon Srichana)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.


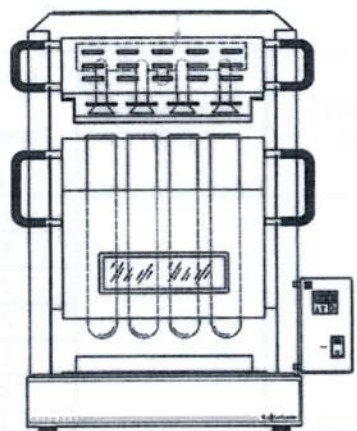


Fig. 1.: Front view

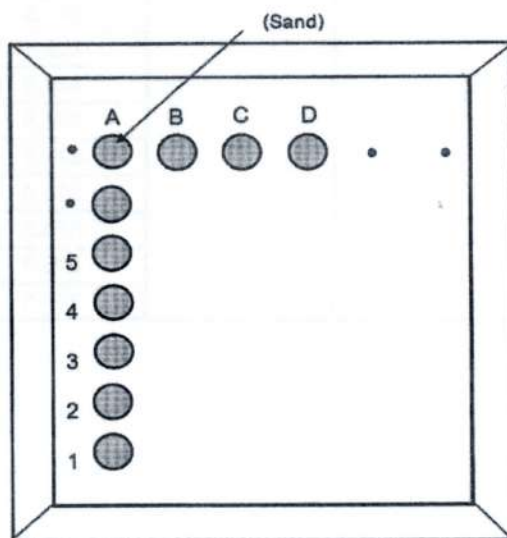

Location of standard

Fig. 2.: Digestion block

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the Digestion block.

Measured Temperature: The average reading of working standard at any positions or location.

Calibration Results:
Before adjustment

Locations	Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
A1	380	380	380	375.1	-4.9	1.5
A2				374.3	-5.7	1.5
A3				374.6	-5.4	1.5
A4				376.3	-3.7	1.5
A5				373.2	-6.8	1.5
B1				374.4	-5.6	1.5
B2				374.3	-5.7	1.5
B3				374.6	-5.4	1.5
B4				375.2	-4.8	1.5
B5				375.1	-4.9	1.5
C1				373.5	-6.5	1.5
C2				372.8	-7.2	1.5
C3				372.1	-7.9	1.5
C4				372.2	-7.8	1.5
C5				374.5	-5.5	1.5
D1				374.7	-5.3	1.5
D2				375.3	-4.7	1.5
D3				375.5	-4.5	1.5
D4				375.8	-4.2	1.5
D5				375.1	-4.9	1.5

Calibration Results:
After adjustment

Locations	Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
A1	380	380	380	379.0	-1.0	1.5
A2				378.7	-1.3	1.5
A3				379.4	-0.6	1.5
A4				379.2	-0.8	1.5
A5				379.2	-0.8	1.5
B1				379.8	-0.2	1.5
B2				379.2	-0.8	1.5
B3				379.5	-0.5	1.5
B4				378.9	-1.1	1.5
B5				379.1	-0.9	1.5
C1				379.1	-0.9	1.5
C2				377.7	-2.3	1.5
C3				378.4	-1.6	1.5
C4				378.2	-1.8	1.5
C5				378.0	-2.0	1.5
D1				379.5	-0.5	1.5
D2				378.7	-1.3	1.5
D3				379.7	-0.3	1.5
D4				379.5	-0.5	1.5
D5				379.4	-0.6	1.5

The End of Certificate

ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: KSPR2304362

ชนิดเครื่องมือ: Block Digestion Unit

รุ่น: KT-20s

หมายเลขเครื่อง: 5720210009/5770200073

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
15 Mar 2023			15 Mar 2023		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
☒	☐	1. สายไฟ	☒	☐	
☒	☐	2. การทำงาน Main Switch	☒	☐	
☒	☐	3. การทำงาน Selector Key	☒	☐	
☒	☐	4. การแสดงผล Display	☒	☐	
☒	☐	5. สภาพ Hole	☒	☐	
☐	☐	6. สภาพฝาปิด	☐	☐	ไม่มี
☒	☐	7. สภาพตัวเครื่อง	☒	☐	
☒	☐	8. สภาพแวดล้อม ณ สถานที่ตั้งเครื่อง	☒	☐	

ข้อแนะนำ :

Mr. Nakarin Ruenros

Service Engineer



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CH1733

Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Mettler Toledo
Model : SevenExcellence
Serial No. : B834291445
ID No. : RYG_EN0152
Condition As-Received: Used Item
Received Date : 21 December 2022
Calibration Date : 22 December 2022
Reference : 2212-0602DSC-1
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Rayong Branch
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lerngagtrakul

Approved by :

Malu.
Approved Signatory

- (/) Malee Butkruea
() Saithip Meangmai
() Warakorn Lerngagtrakul

Issue Date : 26 December 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

REVIEW BY	<i>N. Bannit</i>
APPROVED BY	<i>D. ...</i> 22/12/23
NEXT CAL. DATE	22/06/24 <i>Dr. ...</i>

A 0048758



Cert.No.: 22CH1733

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	22E2769	24 Aug 2023
2) Ref. Standard Thermometer	4982054	110RC044	22I1306	27 Oct 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	826588	09 July 2024
pH 6.987	CPA chem	823322	20 June 2023
pH 10.008	CPA chem	826590	09 July 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: B834291445	4.000	177.48	177.3	4.000	0.058	2.00
	7.000	0.00	-0.1	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Malu



Cert.No.: 22CH1733

Page.: 3 of 3

Calibration Results**Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor <i>k</i>
pH Electrode S/N.: 1475518	4.008	4.011	185.2	0.0052	2.06
	6.987	6.990	10.4	0.0088	2.00
	10.008	10.014	-166.5	0.0072	2.00

Function : Temperature Measurement**(*) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : InLab Expert Pro-ISM

- Serial No. : 1475518

Dimension of probe;

- Length : 120 mm.

- Diameter : 12 mm.

- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor <i>k</i>
25.0	25.001	24.9	-0.101	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Mala



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 22E4098

Page : 1 of 2

Equipment : pH Meter
Manufacturer: Mettler Toledo
Model : SevenExcellence
Serial No.: B834291445
ID No.: RYG_EN0152
Condition As-Received: Used Item
Received Date: 21 December 2022
Calibration Date: 23 December 2022

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Reference: 2212-0602DSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 10) %

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Procedure used: Calibration were conducted using In-house calibration Procedure CP-E17 According to direct measurement method with Multi-Product Calibrator.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Multi-Product Calibrator	5500A	6315011	22E1431	05 May 2023

2.This result of calibration was made on requested at the point specified by customer.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Wutchareeporn Wongchutikrane
Issue Date : 26 December 2022

Approved Signatory :

☒ Phalinee Prabpaipal

☐ Nuntawat Khamchai

☐ Pornthippa Tameyakul

B 0304803



Cert. No.: 22E4098

Page.: 2 of 2

Result of calibration :- (*) Without adjustment () After adjustment

Function: DC voltage measuremer	Range: 2000	mV	
<u>Standard Value</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>
(mV)	(mV)	(mV)	($\pm$ μ V)
-200.0000	-200.0	0.0	72
-150.0000	-150.0	0.0	69
-100.0000	-100.0	0.0	65
-50.0000	-50.0	0.0	62
0.0000	0.0	0.0	58
50.0000	50.0	0.0	62
100.0000	100.0	0.0	65
150.0000	150.0	0.0	69
200.0000	199.9	-0.1	72

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %

*UUC= Unit Under Calibration.

-o0o-

Ag ✓

a 1140616

Certificate No. T221642

Page 1 of 5

Certificate of Calibration

Equipment : Digestion Unit

Manufacturer : SCP Science

Model : DigiPRER HT

Serial No. : HTC1120480658

Customer Code : BKK_EN0366

ID No. : T2635A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab 1

Date of Receipt : 27 June 2022

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 04 JUL 2022

REVIEW BY	<u>Sinluk P.</u>
APPROVED BY	<u>Yeh AL</u>
NEXT CAL. DATE	<u>30/06/23</u>

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T221642

Page 2 of 5

Calibration Report

Equipment : Digestion Unit
Date of Calibration : 30 June 2022
Environment : Temperature : 23.9 - 26.3 °C
Line Voltage : 221.4 - 225.1 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T10.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M7-(CH16-17,CH19-CH20)	T212004	15 October 2022
DATA LOGGER	34970A	T121	T212004	15 October 2022

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant - Hour 26 Minute At 380 °C

Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max

☐ Close

☒ Not Available

5. Adjustment :

(X) without adjustment


() after adjustment

Approved By 

Certificate No. T221642

Page 3 of 5

Calibration Report

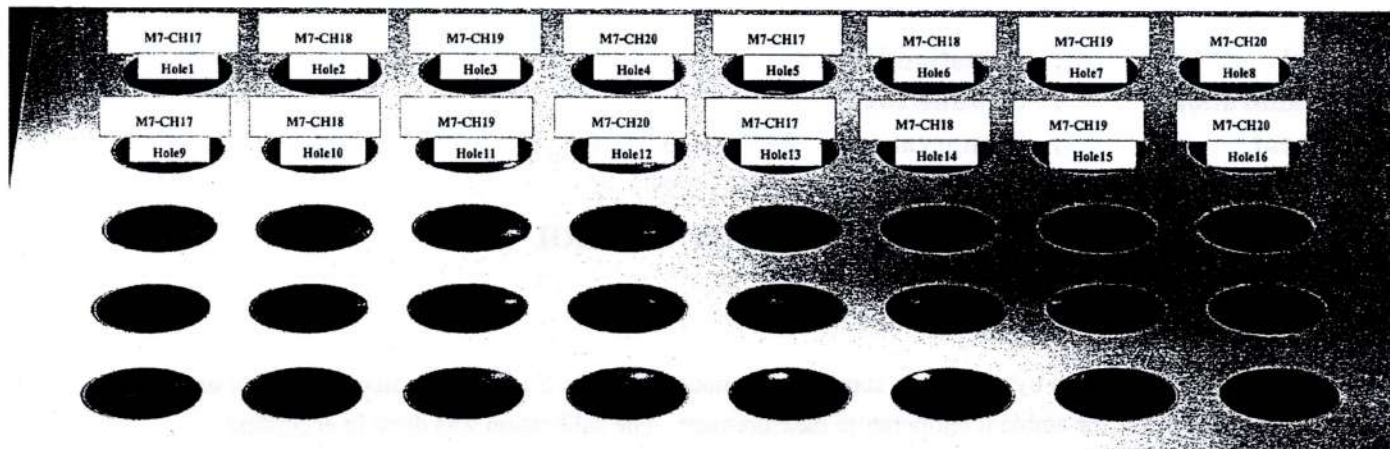

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole1	Hole2	Hole3	Hole4	Hole5	Hole6	Hole7	Hole8
				M7-CH17	M7-CH18	M7-CH19	M7-CH20	M7-CH17	M7-CH18	M7-CH19	M7-CH20
380.0	380.0	379.4 - 380.7	Max °C	379.1	379.8	379.3	377.4	377.6	379.3	379.6	377.9
			Min °C	378.7	379.4	378.9	377.0	377.3	378.8	379.1	377.3
			Average °C	378.9	379.6	379.1	377.2	377.4	379.1	379.3	377.6
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.2	0.2	0.3

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole9	Hole10	Hole11	Hole12	Hole13	Hole14	Hole15	Hole16
				M7-CH17	M7-CH18	M7-CH19	M7-CH20	M7-CH17	M7-CH18	M7-CH19	M7-CH20
380.0	380.0	379.4 - 380.7	Max °C	378.5	378.8	378.1	379.0	380.3	381.6	381.0	379.5
			Min °C	377.8	378.2	377.6	378.6	379.9	381.2	380.5	378.9
			Average °C	378.2	378.5	377.9	378.8	380.1	381.4	380.7	379.2
			Stability ± °C	0.3	0.3	0.2	0.2	0.2	0.2	0.3	0.3


Approved By.



Certificate No. T221642

Page 4 of 5

Calibration Report

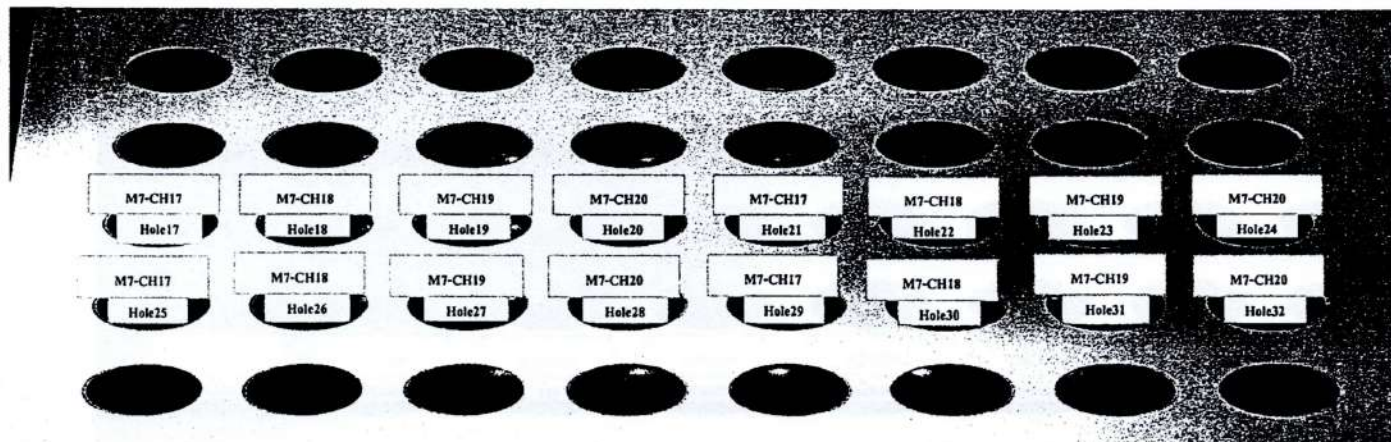

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole17	Hole18	Hole19	Hole20	Hole21	Hole22	Hole23	Hole24
				M7-CH17	M7-CH18	M7-CH19	M7-CH20	M7-CH17	M7-CH18	M7-CH19	M7-CH20
380.0	380.0	379.4 - 380.7	Max °C	378.4	378.8	378.0	379.2	379.0	382.0	381.5	380.3
			Min °C	377.8	378.2	377.7	378.8	378.7	381.5	381.1	379.6
			Average °C	378.1	378.5	377.9	379.0	378.9	381.8	381.3	379.9
			Stability ± °C	0.3	0.3	0.2	0.2	0.2	0.3	0.2	0.4


Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole25	Hole26	Hole27	Hole28	Hole29	Hole30	Hole31	Hole32
				M7-CH17	M7-CH18	M7-CH19	M7-CH20	M7-CH17	M7-CH18	M7-CH19	M7-CH20
380.0	380.0	379.4 - 380.7	Max °C	378.3	378.7	378.4	378.8	379.6	382.6	382.0	380.8
			Min °C	377.6	378.3	377.9	378.4	379.3	382.2	381.4	380.0
			Average °C	378.0	378.5	378.1	378.6	379.5	382.4	381.7	380.4
			Stability ± °C	0.3	0.2	0.2	0.2	0.2	0.2	0.3	0.4

Approved By

Certificate No. T221642

Page 5 of 5

Calibration Report

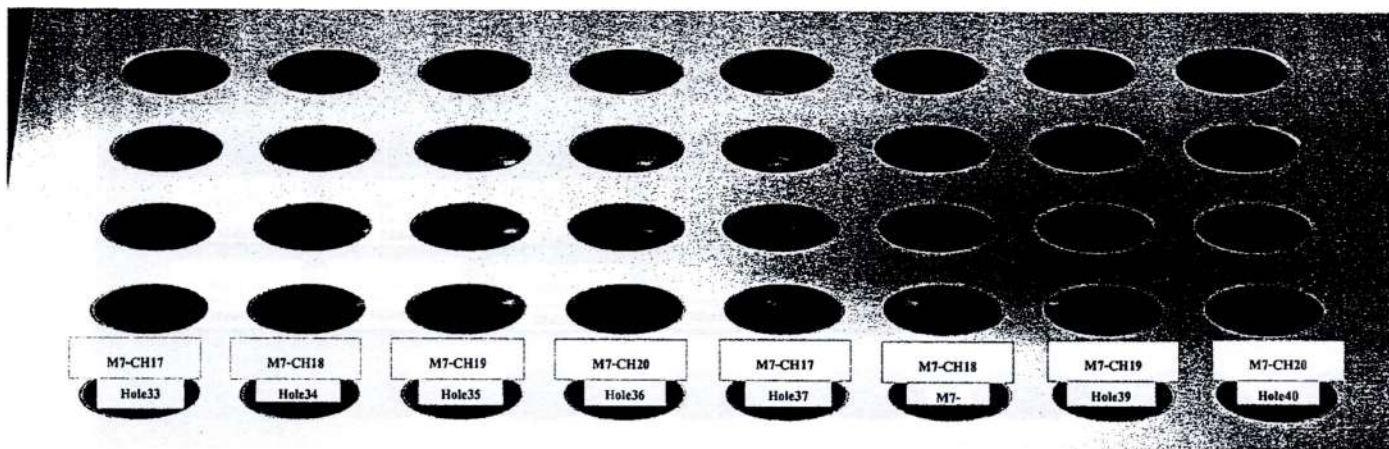

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole33	Hole34	Hole35	Hole36	Hole37	Hole38	Hole39	Hole40
				M7-CH17	M7-CH18	M7-CH19	M7-CH20	M7-CH17	M7-CH18	M7-CH19	M7-CH20
380.0	380.0	379.4 - 380.7	Max °C	378.6	376.7	377.2	378.0	380.0	382.2	381.5	379.7
			Min °C	378.1	376.2	376.7	377.5	379.5	381.7	380.9	379.1
			Average °C	378.3	376.5	377.0	377.7	379.8	381.9	381.2	379.4
			Stability ± °C	0.3	0.3	0.3	0.3	0.3	0.3	0.3	0.3

 The expanded uncertainty of temperature measurement was ± 2.49 °C

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2 , providing a level of confidence of approximately 95 % .

Approved By.





บริษัท ดับเบิล เอส ไดแอกโนสติกส์ จำกัด
DOUBLE S DIAGNOSTICS CO., LTD.

4 ซอยอุดมสุข 14 แขวงบางนา เขตบางนา กรุงเทพฯ 10260 โทรศัพท์: (02) 747-7009 โทรสาร: (02) 747-7008
4 Soi Udomsuk 14, Bangna, Bangkok 10260 Tel. (02) 747-7009 Fax: (02) 747-7008

Maintenance Plan YEAR : 2023

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
รวม	PM & CK											

Periodical maintenance check list for Konelab

	6M	12M	Note!
1.Diluent-wash tubing change	☒	☐	
2.ISE tubing change	☒	☒	none.
3.Syringe check/change		☐	
4.Dispensing check/ change		☐	
5.Waste tubing change when necessary		☐	
6.Lamp check/change	☒	☐	
7.Mixer paddle/paddle change(not Konelab20)		☐	
8.ISE needles check/change		☐	
9.Pump tubing check/ chance	☒	☐	
10.Broken/worn out part check /change		☐	
11.Peristaltic pump check /cleaning/ lubrication	☒	☐	
12.Heating check		☐	
13.Cooling check		☐	
14.Dispenser mechanic check/adjustment	☒	☐	
15.Cuvette transfer mechanic check/adjustment	☒	☐	
16.Dispenser movement check/adjustment	☒	☐	
17.Sample/reagent register check/adjustment	☒	☐	
18.Dispensing tubing tightness check	☒	☐	
19.Photometer and optics cleaning/check/adjustment	☒	☐	
20.Workstation PC cleaning if necessary	☒	☐	
21.Mechanic cleaning/lubrication	☒	☐	
22.Instrument cleaning if necessary	☒	☐	
23.Complete analyzer testing with waterblank/QC or sample	☒	☐	
24.Test parameters/Adjustment/config. Save to USB key	☒	☐	
25.UPS Test	☒	☐	

Place: ALS Laboratory Instrument: Konelab 250
Date/Time: 05-01-66 Serial no: 22781
Service done by: [Signature] Install date:
Signature of customer: [Signature] Date/Time:



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CG3154

Page.: 1 of 2

Certificate of Calibration

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	BKK_EN0171
Manufacturer :	Witeg
Made in :	Germany
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd. Khwaeng Phatthanakan, Khet Suan Luang Bangkok 10250 Thailand
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	759 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Panward Pramklam

REVIEW BY	 <i>Sinluk P.</i>
APPROVED BY	 <i>KLAL</i>
NEXT CAL. DATE	 <i>29/03/2024</i> CWI

Approved by :

Approved Signatory

- () Pornthippa Tameyakul
() Malee Butkruea
(☒) Ponpan Paipim
() Srisuda Khamtha

Issue Date :

31 August 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0044607



Equipment : Burette
Received Date : 26 August 2022
Condition As-Received : Used Item
Calibration Date : 30 August 2022
Reference : 2208-0918DSC-2

Cert.No.: 22CG3154

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID. No.</u>	<u>Certificate No.</u>	<u>Traceability</u>	<u>Due date</u>
1) Balance	AE200S	N03679	140RC001	21MM429	NIMT	22 Sep 2022
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	22H1243	NIST,NIMT	09 June 2023
3) Thermometer	-	1594592	140EC010	22I181	NIMT	10 Feb 2023

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty ($\pm$ mL)	k Factor
50	49.9959	0.010	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-

a 1123908



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th



Certificate No. T221644

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Cold Room)

Manufacturer : KOLDTECH

Model : KM 320

Serial No. : TBN-1012061/05

Customer Code : BKK_EN0167

ID No. : T2463A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.


104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Environmental Laboratory

Date of Receipt : 27 June 2022

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 04 JUL 2022

REVIEW BY	<u>Sinluk P.</u>
APPROVED BY	<u>KL AL</u>
NEXT CAL. DATE	<u>30/12/23</u>

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T221644

Page 2 of 4

Calibration Report

Equipment : Chamber (Cold Room)
Date of Calibration : 30 June - 1 July 2022
Environment : Temperature : 18.9-23.7 °C
Line Voltage : 222.9-226.5 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T210009	30 July 2022
TC	TYPE T	TN171-TN180	T210009	30 July 2022
DATA LOGGER	34970A	T149	T210009	30 July 2022

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 3 Hour - Minute At 3 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

() without adjustment


(X) after adjustment

Approved By. 

Certificate No. T221644

Page 3 of 4

Calibration Report

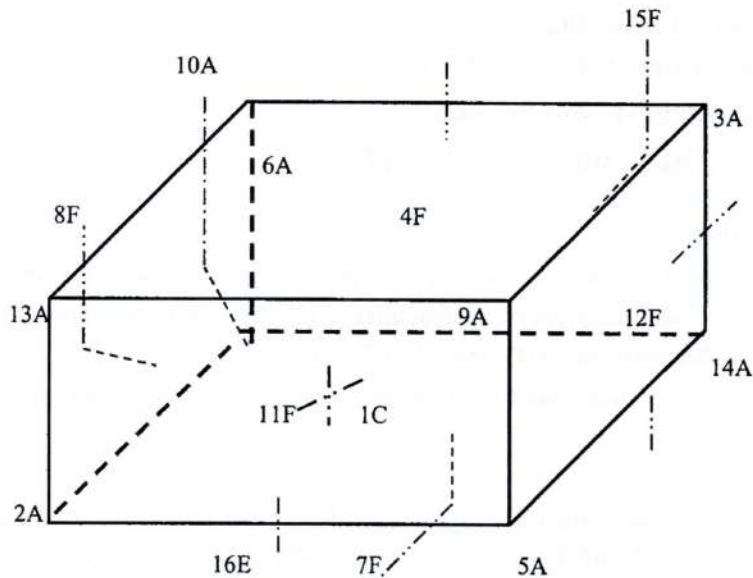

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN161
2A	=	TN162
3A	=	TN163
4F	=	TN164
5A	=	TN165
6A	=	TN166
7F	=	TN167
8F	=	TN168
9A	=	TN169
10A	=	TN170

11F	=	TN171
12F	=	TN172
13A	=	TN173
14A	=	TN174
15F	=	TN175
16E	=	TN176

Approved By. 

Certificate No. T221644

Page 4 of 4

Calibration Report

Measurement Results:

Average Standard Reading at each position (°C)										
Calibration Point	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170
3	2.71	2.82	2.75	2.89	2.95	3.68	3.02	2.96	3.03	2.85
	TN171	TN172	TN173	TN174	TN175	TN176				
	2.97	3.02	2.89	3.04	2.97	3.33				

Chamber (Cold Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage
	Min , Max	Average					Factor <i>k</i>
3.0	2.9 , 4.0	3.2	2.99	1.05	1.30	1.66	2.00


* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



Agilent CrossLab Compliance Services

Agilent
CrossLab

From Insight to Outcome

EQUIPMENT QUALIFICATION REPORT (EQR)

Agilent CrossLab Compliance

Qualification Type:	ICPMS-OQ
System ID:	JP12091612
EQP Name:	AgilentRecommended
EQP Revision:	ICPMS.02.50
EQP Publish Date:	March 2020
Date:	June 14, 2022 10:32:16 AM
Report Type:	Report
Org. Name:	ALS Laboratory Group (Thailand) Co.,Ltd.
Org. Location:	104 Phatthanakarn 40, Suan Luang, Bangkok 10250 Thailand.

REVIEW BY Tattaporn C.APPROVED BY Santana NNEXT CAL. DATE 14/12/23

Table of Contents

Section	Page
Cover	1
Table of Contents	2
Test Summary	3
Service Details	4
Instrument Details	5
Calculation Formulas	6
Protocol Details	7
Tests	8
Autosampler Check : ASX-520	8
Integrated Sample Introduction System (ISIS) Check : ISIS2	9
Autotune : G3281A	10
Background (No Gas Mode) : G3281A	12
Background (Gas Modes) : G3281A	13
20-Minute Stability (No Gas Mode) : G3281A	14
Declaration of Change Control	15
Attachments	16
Electronic Signature	28
Transaction Logs	29

Test Summary

Purpose

This section includes a status for each scheduled test and the overall qualification. For each test that is run, (1) the status is automatically determined based on pre-defined limits, and (2) the total number of times the test was run is displayed. For detailed results and specifications for a test, refer to the test results in this EQR.

Details

Test	Status	Runs
Autosampler Check : ASX-520	Pass	1
Integrated Sample Introduction System (ISIS) Check : ISIS2	Pass	1
Autotune : G3281A	Pass	1
Background (No Gas Mode) : G3281A	Pass	1
Background (Gas Modes) : G3281A	Pass	1
20-Minute Stability (No Gas Mode) : G3281A	Pass	1

Overall Qualification Status

Pass

Service Details

Purpose

This section includes local contact and delivery details for this service.

General Details

Service Order No./Request: 6005218484
EQP Name: AgilentRecommended
EQP Revision: ICPMS.02.50
Report Type: Report

Organization Details

Name: ALS Laboratory Group (Thailand) Co.,Ltd.
Location: 104 Phatthanakarn 40, Suan Luang, Bangkok 10250 Thailand.

Local Contact Details

Name: Khan Chatchanai
Job Title: Lab Manager
Qualification Location: Spectro Room

Operator Details

Name: Panthep Kurasathain
Job Title: Field Service Engineer

Data Acquisition Details

Acquisition Software Name: MassHunter
Acquisition Software Revision: D.01.01

Customer Data System (CDS): IcpMs: MassHunter

Instrument Details

Purpose

This section describes the as found system configuration.

Details

ICP-MS 1

Manufacturer	Agilent Technologies
Name	7700x
Model Number	G3281A
Detector Type	SQ
Nebulizer	Mira Mist (G3161)
Spray Chamber	Quartz
Torch	Quartz
Sampling Cone	Ni
Skimmer Cone	Ni
Serial Number	JP12091612
Firmware Revision	D.01.01

ISIS 1

Manufacturer	Agilent Technologies
Name	ISIS2
Model Number	G4911A
Installed Options	#003: 2 pumps, 1 valve, auto dilution and discrete sampling
Type	Peristaltic pump system

Autosampler 1

Manufacturer	Agilent Technologies
Name	ASX-520
Model Number	G3286A
Serial Number	031403A520

Chiller 1

Manufacturer	Agilent Technologies
Name	Chiller
Model Number	G3292A
Serial Number	4N1220700

Calculation Formulas

Purpose

This section includes calculation formulas for all available tests. Depending upon which tests are scheduled, all or some apply to your qualification.

For a description of calculations for ICP-MS tests performed by the MassHunter software, refer to the MassHunter application and documentation.

Protocol Details

Purpose

This section lists the revisions for all test units used in this report. For complete test-specific and high-level change details, refer to the Revision History document.

Test Revision	Test
ICPMS.02.50	20-Minute Stability (No Gas Mode)
ICPMS.02.50	Autosampler Check
ICPMS.02.50	Autotune
ICPMS.02.50	Background (Gas Modes)
ICPMS.02.50	Background (No Gas Mode)
ICPMS.02.50	Integrated Sample Introduction System (ISIS) Check

Autosampler Check

Purpose

This test demonstrates that the autosampler module is correctly installed and connected. It does not test module performance.

Setpoint

Results

Criteria	Observed Result	Expected Result	Status
After the self test, is probe in the home position?	Yes	Yes	Pass
As commanded, is the probe positioned at vial 2?	Yes	Yes	Pass

Setpoint Status:

Pass

Runs: 1

Overall Autosampler Check Test Status

Pass

Integrated Sample Introduction System (ISIS) Check

Purpose

This test demonstrates that the ISIS module is correctly installed and connected. It does not test module performance.

Setpoint

Results

Criteria	Observed Result	Expected Result	Status
As commanded, does the pump rotate?	Yes	Yes	Pass
As commanded, do the valves load and inject?	Yes	Yes	Pass

Setpoint Status: Pass

Runs: 1

Overall Integrated Sample Introduction System (ISIS) Check Test Status

Pass

Autotune

Purpose

This test uses traceable checkout standards to run a software-executed autotune in all modes. The tune report provides values for peak width, mass axis, sensitivity, oxide species, and doubly-charged species tests.

Setpoint

Results

Peakwidth Mass 7

0.735 AMU

Agilent Recommended:

>= 0.65

<= 0.80

Status:

Pass

Peakwidth Mass 89

0.732 AMU

Agilent Recommended:

>= 0.65

<= 0.80

Status:

Pass

Peakwidth Mass 205

0.746 AMU

Agilent Recommended:

>= 0.65

<= 0.80

Status:

Pass

Mass Axis 7

7.00 AMU

Agilent Recommended:

>= 6.9

<= 7.1

Status:

Pass

Mass Axis 89

89.00 AMU

Agilent Recommended:

>= 88.9

<= 89.1

Status:

Pass

Mass Axis 205

205.00 AMU

Agilent Recommended:

>= 204.9

<= 205.1

Status:

Pass

Mass 7 Sensitivity No Gas

81.18

Mcps/ppm

Agilent Recommended:

>= 25.5

Status:

Pass

Mass 89 Sensitivity No Gas

247.81

Mcps/ppm

Agilent Recommended:

>= 85

Status:

Pass

Mass 205 Sensitivity No Gas

184.87

Mcps/ppm

Agilent Recommended:

>= 51

Status:

Pass

Mass 59 Sensitivity He

84.86

Mcps/ppm

Agilent Recommended:

>= 20.4

Status:

Pass

Oxide Ratio 156/140

1.119

%

Agilent Recommended:

<= 1.38

Status:

Pass

Doubly Charged Species Ratio 70/140

1.140

%

Agilent Recommended:

<= 2.3

Status:

Pass

Setpoint Status: Pass

Runs: 1

Overall Autotune Test Status

Pass

Background (No Gas Mode)

Purpose

This test examines the background of the ICP-MS in no gas mode by monitoring ions during a blank run.

Setpoint

Conditions

Masses:

7	AMU
89	AMU
205	AMU

Measurements and Results

Masses (AMU):

Measured Value:

Agilent Recommended:

Status:

	7		89		205	
	4.900		7.100		18.400	cps
<=	10		<=	10	<=	30
Pass			Pass		Pass	

Setpoint Status:

Pass

Runs: 1

Overall Background (No Gas Mode) Test Status

Pass

Background (Gas Mode)

Purpose

This test examines the background of the ICP-MS in the various gas modes by monitoring ions during a blank run.

Setpoint Gas Mode: Helium

Conditions

Mass: 78 AMU
Integration Time: 1.0 sec
Cycles: 20

Measurements and Results

Mass (AMU): 78
Measured Value: 21.1000 cps
Agilent Recommended: ≤ 460
Status: Pass

Setpoint Status: Pass

Runs: 1

Overall Background (Gas Mode) Test Status

Pass

20-Minute Stability (No Gas Mode)

Purpose

This test monitors the abundance of ions present in the checkout standard over a 20-minute period to verify that the signal is stable. The %RSD of the abundance of given ions is calculated internally by the software and compared to the limit.

Setpoint

Conditions

Mode:	Spectrum
Masses:	7, 9, 59, 89, 140, 205
Integration Time:	9.99 sec
Peak Pattern:	3 points/peak
Repetitions:	20
Sweeps/Replicates:	100

Measurements and Results

Masses (AMU):	7	89	205	
Stability RSD:	0.2	0.6	0.6	%
Agilent Recommended:	<= 3.45	<= 3.45	<= 3.45	
Status:	Pass	Pass	Pass	

Setpoint Status:	Pass	Runs: 1
------------------	------	---------

Overall 20-Minute Stability (No Gas Mode) Test Status

Pass

Declaration of Change Control

This document is under change control. Revision history is maintained and printed on each document. Access to the master documents is limited to process owners. Documents receive periodic review and cannot be assigned an evergreen status. The qualification performed according to this document refers only to the hardware/software configuration in place at the time of the qualification. Agilent Technologies recommends that instrument configuration change management procedures be in place in order to maintain the validation process. Any changes to the analytical or computer hardware or software must be clearly specified. A change management system provides a means for determining the degree of requalification required according to the extent of the changes made. All details of the changes must be thoroughly recorded and documented, together with details of completed tests and their results. Note: Hardware/software configuration management is the customer's responsibility.

Attachments

Training requirements note: The delivery engineer attaches an ACE technique-specific training certificate to the Equipment Qualification Report (EQR). Obtaining ACE technique-specific certification includes pre-requisite trainings for Data Integrity, General Compliance topics (GMP, GLP, ALCOA, etc.), instrument hardware and software components, and the ACE technique itself. The one certificate encompasses all pre-requisite trainings as documented in the Agilent Learning Management System called Success Factors.

Location	Category	Document Name	Page
EQR	General	Certificate of System Qualification	17
EQR	General	Operator's training certificate and qualifications	18
EQR	General	Certificate of Qualification for ACE	19
EQR	General	Certificate of Qualification for ACE	20
EQR	General	Tune reports	21
EQR	General	Test Report	24
EQR	General	Test Report	26

General

Document Name: Certificate of System Qualification

**Agilent Compliance Engine Self Qualification**

Date: September 14, 2021 4:59:15 PM

Drive Serial #: ACA025C9

Platform Revision:

ACE 3.11

Individual self-qualification reports for each specific technique installed are also available upon request. They provide additional details on the general report from the concise summary and are structured by the actual algorithms challenged during the process. There is not a one-to-one relationship between algorithms and OQ program tests because some algorithms are used by several tests and across multiple similar hardware components of the qualified systems.

Technique Type	Tests Completed	Result
Atomic Absorption	7	Conforms
Capillary Electrophoresis	10	Conforms
Dissolution	6	Conforms
Emission Spectroscopy	3	Conforms
Gas Chromatography - GCMS	17	Conforms
Gas Chromatography	29	Conforms
Gel Permeation Chromatography	9	Conforms
ICP-MS	6	Conforms
Infrared Spectroscopy	7	Conforms
Liquid Chromatography	17	Conforms
Liquid Chromatography - LCMS	8	Conforms
Microfluidics	18	Conforms
Sample Preparation - Gas Chromatography	9	Conforms
Sample Preparation - Liquid Chromatography	8	Conforms
Supercritical Fluid Chromatography	15	Conforms
Software	6	Conforms
UV-Vis Spectrophotometer	13	Conforms

Overall Qualification Status

Conforms

General

Document Name: Operator's training certificate and qualifications



Certificate of Completion

Learner Name: Panthep Kurasathain

Title Of Course: AN-CE-ICPMS-2-017-B:7700x/7700s ICP-MS Intro. -Oper.H/W.S/W & OQ/PV

Completion Date: November 22, 2012

Certified By Company: Learning at Agilent

All Service and Support training certificates have the following specific limitations.

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's: Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.

General

Document Name: Certificate of Qualification for ACE



Certificate of Completion

Learner Name:	Panthep Kurasathain
Title Of Course:	AN-CE-SS-II-030-A: ACE 3.X User Update Training
Completion Date:	July 7, 2020
Certified By Company:	Learning at Agilent

All Service and Support training certificates have the following specific limitations.

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's: Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.

General

Document Name: Certificate of Qualification for ACE



Certificate of Completion

Learner Name: Panthep Kurasathain

Title Of Course: AN-CE-ICPMS-2-035-B: CrossLab Compliance Hardware Specific Delivery for Agilent ICP-MS Systems

Completion Date: October 31, 2020

Certified By Company: Learning at Agilent

All Service and Support training certificates have the following specific limitations.

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's: Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.

General


Document Name: Tune reports

Tune Report

Operator Name Supakwan Mak
 Acq/Data Batch C:\Agilent\ICPMH\1\UserTune.b
 Acq. Date-Time 6/14/2022 9:03:15 AM
 Report Comment PMOQ 14 June 2022
 Instrument Name G3281A JP12091612

[No Gas]

Sensitivity

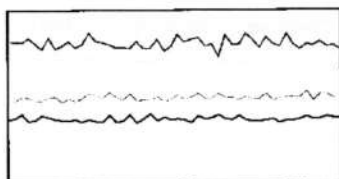


Mass	Range	Count	RSD%	Background
7	10000	8118	3.585	4.900
89	50000	24781	3.128	7.100
205	50000	18487	3.808	18.400

Sampling Period [sec] 0.311
 Integration Time [sec] 0.1

Oxide/Doubly Charged Ratio

Oxide 156 / 140 1.119 %
 Doubly Charged 70 / 140 1.140 %

Resolution/Axis

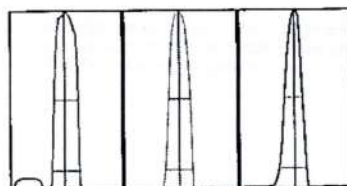

Mass	Peak Height	Axis	W-50%	W-10%
7	8050.47	7.00	0.65	0.735
89	24725.81	89.00	0.57	0.732
205	18559.81	205.00	0.49	0.746

Integration Time [sec] 0.1
 Acquisition Time [sec] 22.74
 Y Axis Linear

Tune Parameters

Plasma Parameters

Plasma Mode	---	Nebulizer Gas	1.05 L/min	Makeup Gas	0.00 L/min
RF Power	1550 W	Option Gas	---	Auxiliary Gas	0.90 L/min
RF Matching	1.80 V	Nebulizer Pump	0.10 rps	Plasma Gas	15.0 L/min
Sample Depth	8.0 mm	S/C Temp	2 °C		

Lens Parameters

Extract 1	0.0 V	Omega Lens	8.6 V	Deflect	12.0 V
Extract 2	-190.0 V	Cell Entrance	-30 V	Plate Bias	-40 V
Omega Bias	-90 V	Cell Exit	-50 V		

Cell Parameters

Use Gas	No	3rd Gas Flow	---	Energy Discrimination	5.0 V
He Flow	0.0 mL/min	OctP Bias	-8.0 V		

1 of 3

6/14/2022 9:03 AM

Date: June 14, 2022 10:32:16 AM
 System ID: JP12091612

Document Name: Tune reports

Tune Report

H2 Flow — OctP RF 200 V

QP Parameters

Mass Gain	152	Axis Gain	1.0032	QP Bias	-3.0 V
Mass Offset	123	Axis Offset	0.12		

Hardware Settings

Torch


Torch H	-0.4 mm	Torch V	0.0 mm
---------	---------	---------	--------

EM

Discriminator	4.5 mV	Analog HV	1708 V	Pulse HV	1356 V
---------------	--------	-----------	--------	----------	--------

[He]

Sensitivity

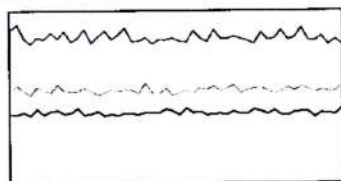

Mass	Range	Count	RSD%	Background
59	10000	8486	3.392	15.700
89	20000	10724	3.135	13.900
205	50000	20200	3.166	22.100

Sampling Period [sec] 0.31
Integration Time [sec] 0.1

Oxide/Doubly Charged Ratio

Oxide 156 / 140 1.122 %
Doubly Charged 70 / 140 1.288 %

Tune Parameters

Plasma Parameters

Plasma Mode	—	Nebulizer Gas	1.05 L/min	Makeup Gas	0.00 L/min
RF Power	1550 W	Option Gas	—	Auxiliary Gas	0.90 L/min
RF Matching	1.80 V	Nebulizer Pump	0.10 rps	Plasma Gas	15.0 L/min
Sample Depth	8.0 mm	S/C Temp	2 °C		

Lens Parameters

Extract 1	0.0 V	Omega Lens	7.4 V	Deflect	3.6 V
Extract 2	-200.0 V	Cell Entrance	-90 V	Plate Bias	-115 V
Omega Bias	-90 V	Cell Exit	-70 V		

Cell Parameters

Use Gas	Yes	3rd Gas Flow	—	Energy Discrimination	3.0 V
He Flow	4.5 mL/min	OctP Bias	-21.0 V		
H2 Flow	—	OctP RF	190 V		

QP Parameters

Mass Gain	152	Axis Gain	1.0032	QP Bias	-18.0 V
Mass Offset	123	Axis Offset	0.12		

Hardware Settings

Torch

Torch H	-0.4 mm	Torch V	0.0 mm
---------	---------	---------	--------

2 of 3

6/14/2022 9:03 AM

Date: June 14, 2022 10:32:16 AM
System ID: JP12091612

Document Name: Tune reports

Tune Report

EM

Discriminator

4.5 mV

Analog HV

1708 V

Pulse HV

1356 V

3 of 3

6/14/2022 9:03 AM

General

Document Name: Test Report

Batch Summary Report

Batch Folder: D:\Agilent Service\PMOQ 13-6-22\BG He.b\

Analysis File: BG He.batch.bin

Tune Step: #1 He

	Row	Acq. Date-Time	Data File	Sample Name	Type	Level	Dilution
	1	6/14/2022 10:03:39 AM	001SMPL.d	BG He	Sample		1.0000

Document Name: Test Report

Batch Summary Report

Analyte Table

		78 He I	
Sample Name		CPS	CPS RSD
1	BG He	21.1000	38.0

Page 2 / 2

6/14/2022 10:09:04 AM

General

Document Name: Test Report

Batch Summary Report

Batch Folder: D:\Agilent Service\PMOQ 13-6-22\ OQ 20 Min.b\

Analysis File: OQ 20 Min.batch.bin

Tune Step: #1 No Gas

	Ret	Acq. Date-Time	Data File	Sample Name	Type	Level	Dilution
1		6/14/2022 9:29:27 AM	0015MPL.d	20 min	Sample		1.0000

Document Name:

Test Report

Batch Summary Report

Analyte Table

		7 [No Gas]		9 [No Gas]		59 [No Gas]		89 [No Gas]	
	Sample Name	CPS	CPS RSD	CPS	CPS RSD	CPS	CPS RSD	CPS	CPS RSD
1	20 min	82477.8975	0.2	285.3875	5.8	162011.0035	0.7	241211.0700	0.6

		140 [No Gas]		205 [No Gas]	
	Sample Name	CPS	CPS RSD	CPS	CPS RSD
1	20 min	252452.6980	0.7	181154.8205	0.6

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Panthep Kurasathain
Logged On User Name:	panthep_kurasathain@agilent.com
Signature Creation Date:	June 14, 2022
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: panthep_kurasathain
 Hostname: ASBKKWX313

System Id: JP12091612
 Print Date: June 14, 2022 10:32:20 AM

ALS OQHW 7700 14Jun2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 14, 2022 10:14:43 AM	Audit	SessionCreated	Session	None
June 14, 2022 10:14:43 AM	Start	Configuration	Session	None
June 14, 2022 10:14:43 AM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
June 14, 2022 10:19:18 AM	Audit	EqpLoaded	Session	EQP details for primary technique [lcpMs] - File path: [ProtocolPacks/lcpMs/Configurations/02.50/lcpMs.02.50.eqp], EQP File Name: [lcpMs.02.50.eqp], EQP Name: [AgilentRecommended]
June 14, 2022 10:19:20 AM	End	Configuration	Session	None
June 14, 2022 10:19:24 AM	Start	Qualification	Session	OQ
June 14, 2022 10:19:24 AM	Start	Execution	Autosampler Check : ASX-520: Autosampler Check	None
June 14, 2022 10:19:42 AM	End	Execution	Autosampler Check : ASX-520: Autosampler Check	Run Count : 1
June 14, 2022 10:19:43 AM	Start	Execution	Integrated Sample Introduction System (ISIS) Check : ISIS2: Integrated Sample Introduction System (ISIS) Check	None
June 14, 2022 10:19:47 AM	End	Execution	Integrated Sample Introduction System (ISIS) Check : ISIS2: Integrated Sample Introduction System (ISIS) Check	Run Count : 1
June 14, 2022 10:19:50 AM	Start	Execution	Autotune : G3281A: Autotune 1	None
June 14, 2022 10:22:22 AM	End	Execution	Autotune : G3281A: Autotune 1	Run Count : 1

User Name: panthep_kurasathain
 Hostname: ASBKKWX313

System Id: JP12091612
 Print Date: June 14, 2022 10:32:20 AM

ALS OQHW 7700 14Jun2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 14, 2022 10:22:24 AM	Start	Execution	Background (No Gas Mode) : G3281A: No Gas Mode Background 1	None
June 14, 2022 10:22:48 AM	End	Execution	Background (No Gas Mode) : G3281A: No Gas Mode Background 1	Run Count : 1
June 14, 2022 10:22:49 AM	Start	Execution	Background (Gas Modes) : G3281A: Gas Mode Background :Helium	None
June 14, 2022 10:23:35 AM	End	Execution	Background (Gas Modes) : G3281A: Gas Mode Background :Helium	Run Count : 1
June 14, 2022 10:23:37 AM	Start	Execution	20-Minute Stability (No Gas Mode) : G3281A: 20-Minute Stability (No Gas Mode) 1	None
June 14, 2022 10:24:06 AM	End	Execution	20-Minute Stability (No Gas Mode) : G3281A: 20-Minute Stability (No Gas Mode) 1	Run Count : 1
June 14, 2022 10:24:08 AM	End	Qualification	Session	OQ
June 14, 2022 10:24:08 AM	Start	Reporting	Session	None
June 14, 2022 10:30:26 AM	Audit	Reporting	Session	Report Generated : Certificate
June 14, 2022 10:30:39 AM	Audit	Reporting	Session	Report Generated : Report

Certificate of System Qualification

ICPMS-OQ

System ID: JP12091612
Organization Name: ALS Laboratory Group (Thailand) Co.,Ltd.
Organization Location: 104 Phatthanakarn 40, Suan Luang, Bangkok 10250 Thailand.

Date: June 14, 2022 10:32:51 AM
EQP Name: AgilentRecommended
EQP Revision: ICPMS.02.50
Overall Qualification Status: Pass

Autosampler Check

Overall Autosampler Check Test Status

Pass

Integrated Sample Introduction System (ISIS) Check

Overall Integrated Sample Introduction System (ISIS) Check Test Status

Pass

Autotune

Peakwidth Mass 7 Pass

Peakwidth Mass 89 Pass

Peakwidth Mass 205 Pass

Mass Axis 7 Pass

Mass Axis 89 Pass

Mass Axis 205 Pass

Mass 7 Sensitivity No Gas Pass

Mass 89 Sensitivity No Gas Pass

Mass 205 Sensitivity No Gas Pass

Mass 59 Sensitivity He Pass

Oxide Ratio 156/140 Pass

Doubly Charged Species Ratio 70/140 Pass

Overall Autotune Test Status

Pass

Date: June 14, 2022 10:32:51 AM
System ID: JP12091612

Background (No Gas Mode)**Setpoint Status:** Pass**Masses (AMU):****Measured Value:****Agilent Recommended:****Status:**

	7		89		205	
	4.900		7.100		18.400	cps
<=	10	<=	10	<=	30	
Pass		Pass		Pass		

Overall Background (No Gas Mode) Test Status

Pass

Background (Gas Mode)**Gas Mode:** Helium**Setpoint Status:** Pass**Mass (AMU):****Measured Value:****Agilent Recommended:****Status:**

	78	
	21.1000	cps
<=	460	
Pass		

Overall Background (Gas Mode) Test Status

Pass

20-Minute Stability (No Gas Mode)**Masses (AMU):****Stability RSD:****Agilent Recommended:****Status:**

	7		89		205	
	0.2		0.6		0.6	%
<=	3.45	<=	3.45	<=	3.45	
Pass		Pass		Pass		

Overall 20-Minute Stability (No Gas Mode) Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

ICP-MS 1

Manufacturer	Agilent Technologies
Name	7700x
Model Number	G3281A
Detector Type	SQ
Nebulizer	Mira Mist (G3161)
Spray Chamber	Quartz
Torch	Quartz
Sampling Cone	Ni
Skimmer Cone	Ni
Serial Number	JP12091612
Firmware Revision	D.01.01

ISIS 1

Manufacturer	Agilent Technologies
Name	ISIS2
Model Number	G4911A
Installed Options	#003: 2 pumps, 1 valve, auto dilution and discrete sampling
Type	Peristaltic pump system

Autosampler 1

Manufacturer	Agilent Technologies
Name	ASX-520
Model Number	G3286A
Serial Number	031403A520

Chiller 1

Manufacturer	Agilent Technologies
Name	Chiller
Model Number	G3292A
Serial Number	4N1220700

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Panthep Kurasathain
Logged On User Name:	panthep_kurasathain@agilent.com
Signature Creation Date:	June 14, 2022
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: panthep_kurasathain
 Hostname: ASBKKWX313

System Id: JP12091612
 Print Date: June 14, 2022 10:32:52 AM

ALS OQHW 7700 14Jun2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 14, 2022 10:14:43 AM	Audit	SessionCreated	Session	None
June 14, 2022 10:14:43 AM	Start	Configuration	Session	None
June 14, 2022 10:14:43 AM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
June 14, 2022 10:19:18 AM	Audit	EqpLoaded	Session	EQP details for primary technique [IcpMs] - File path: [ProtocolPacks/IcpMs/Configurations/02.50/IcpMs.02.50.eqp], EQP File Name: [IcpMs.02.50.eqp], EQP Name: [AgilentRecommended]
June 14, 2022 10:19:20 AM	End	Configuration	Session	None
June 14, 2022 10:19:24 AM	Start	Qualification	Session	OQ
June 14, 2022 10:19:24 AM	Start	Execution	Autosampler Check : ASX-520: Autosampler Check	None
June 14, 2022 10:19:42 AM	End	Execution	Autosampler Check : ASX-520: Autosampler Check	Run Count : 1
June 14, 2022 10:19:43 AM	Start	Execution	Integrated Sample Introduction System (ISIS) Check : ISIS2: Integrated Sample Introduction System (ISIS) Check	None
June 14, 2022 10:19:47 AM	End	Execution	Integrated Sample Introduction System (ISIS) Check : ISIS2: Integrated Sample Introduction System (ISIS) Check	Run Count : 1
June 14, 2022 10:19:50 AM	Start	Execution	Autotune : G3281A: Autotune 1	None
June 14, 2022 10:22:22 AM	End	Execution	Autotune : G3281A: Autotune 1	Run Count : 1

User Name: panthep_kurasathaln
 Hostname: ASBKKWX313

System Id: JP12091612
 Print Date: June 14, 2022 10:32:52 AM

ALS OQHW 7700 14Jun2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 14, 2022 10:22:24 AM	Start	Execution	Background (No Gas Mode) : G3281A: No Gas Mode Background 1	None
June 14, 2022 10:22:48 AM	End	Execution	Background (No Gas Mode) : G3281A: No Gas Mode Background 1	Run Count : 1
June 14, 2022 10:22:49 AM	Start	Execution	Background (Gas Modes) : G3281A: Gas Mode Background :Helium	None
June 14, 2022 10:23:35 AM	End	Execution	Background (Gas Modes) : G3281A: Gas Mode Background :Helium	Run Count : 1
June 14, 2022 10:23:37 AM	Start	Execution	20-Minute Stability (No Gas Mode) : G3281A: 20-Minute Stability (No Gas Mode) 1	None
June 14, 2022 10:24:06 AM	End	Execution	20-Minute Stability (No Gas Mode) : G3281A: 20-Minute Stability (No Gas Mode) 1	Run Count : 1
June 14, 2022 10:24:08 AM	End	Qualification	Session	OQ
June 14, 2022 10:24:08 AM	Start	Reporting	Session	None
June 14, 2022 10:30:26 AM	Audit	Reporting	Session	Report Generated : Certificate
June 14, 2022 10:30:39 AM	Audit	Reporting	Session	Report Generated : Report

User Name: panthep_kurasathain
Hostname: ASBKKWX313

System Id: JP12091612
Print Date: June 14, 2022 10:32:52 AM

ALS OQHW 7700 14Jun2022 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
June 14, 2022 10:32:26 AM	Audit	Reporting	Session	Report Signed : Report PDF Name: ALS OQHW 7700 14Jun2022_20220614_OQ Report_1.pdf User Name: panthep_kurasathain@agilen t.com Full Name of Signer: Panthep Kurasathain Reason for signature: Executed protocol and published this original version of document

Certificate No. T220730

Page 1 of 6

Certificate of Calibration

Equipment : HEATING BLOCK

Manufacturer : Environmental Express

Model : SC 196

Serial No. : 6974CECW3285

Customer Code : BKK_EL0054

ID No. : T5306A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250

Customer Location : Acid Digestion Lab

Date of Receipt : 30 March 2022

Calibrated By : Watcharapon Sangtong (Technician)

Approved By :  / Sujjar Naknakred (Site Calibration Manager)

Date of Issue : 12 APR 2022

REVIEW BY	Tattaporn C.
APPROVED BY	Sangtong
NEXT CAL. DATE	7/10/23


The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T220730

Page 3 of 6

Calibration Report

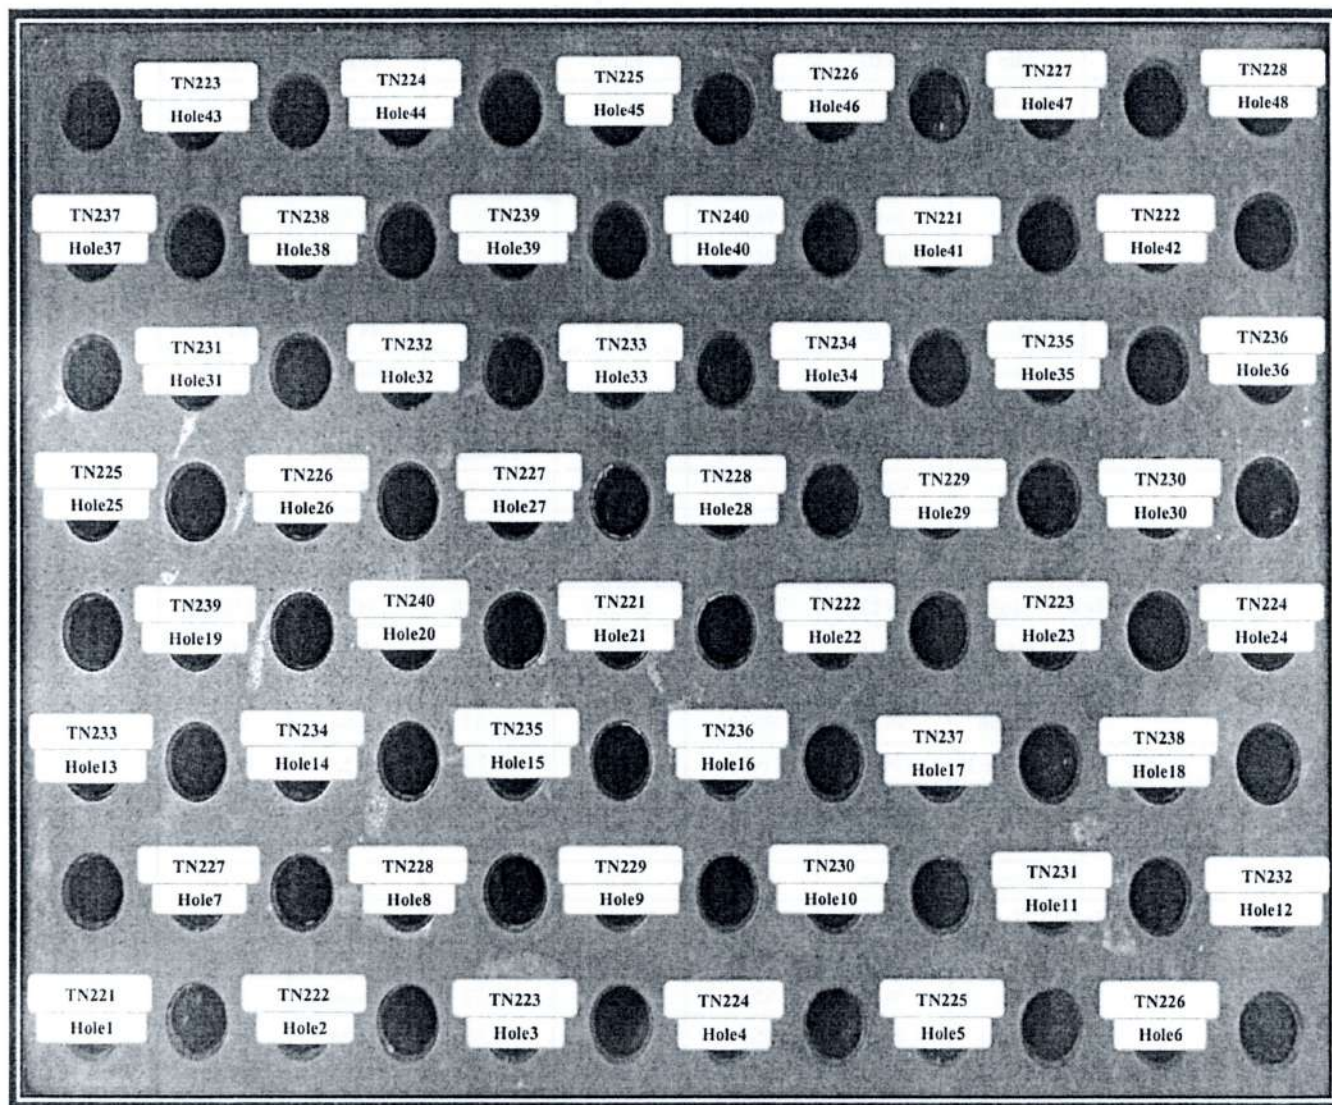

FRONT CONTROL

Approved By. _____



Certificate No. T220730

Page 4 of 6

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (° C)					
R1 Hole1-Hole6		TN221	TN222	TN223	TN224	TN225	TN226
CAL POINT	Max	93.60	93.82	94.05	94.20	94.36	94.26
95	Min	93.07	93.26	93.51	93.66	93.82	93.71
	Average	93.33	93.54	93.78	93.93	94.09	93.98
R2 Hole7-Hole12		TN227	TN228	TN229	TN230	TN231	TN232
	Max	94.59	94.79	94.63	94.55	94.82	95.00
	Min	94.05	94.25	94.08	93.97	94.26	94.44
	Average	94.32	94.52	94.36	94.26	94.54	94.72
R3 Hole13-Hole18		TN233	TN234	TN235	TN236	TN237	TN238
	Max	95.03	94.54	94.78	94.84	95.06	94.73
	Min	94.46	93.98	94.20	94.28	94.49	94.18
	Average	94.74	94.26	94.49	94.56	94.78	94.45
R4 Hole19-Hole24		TN239	TN240	TN221	TN222	TN223	TN224
	Max	94.89	94.82	95.73	95.85	95.73	96.10
	Min	94.33	94.26	95.51	95.62	95.51	95.85
	Average	94.61	94.54	95.62	95.73	95.62	95.97
R5 Hole25-Hole30		TN225	TN226	TN227	TN228	TN229	TN230
	Max	96.28	96.39	96.37	96.54	96.19	96.04
	Min	96.01	96.10	96.02	96.20	95.89	95.71
	Average	96.15	96.24	96.20	96.37	96.04	95.88
R6 Hole31-Hole36		TN231	TN232	TN233	TN234	TN235	TN236
	Max	96.84	96.97	97.03	96.48	96.33	95.76
	Min	96.53	96.65	96.71	96.08	95.98	95.43
	Average	96.68	96.81	96.87	96.28	96.16	95.60
R7 Hole37-Hole42		TN237	TN238	TN239	TN240	TN221	TN222
	Max	96.46	96.15	96.19	96.06	96.95	97.09
	Min	96.13	95.84	95.85	95.72	96.64	96.78
	Average	96.30	95.99	96.02	95.89	96.80	96.93
R8 Hole43-Hole48		TN223	TN224	TN225	TN226	TN227	TN228
	Max	96.91	96.58	96.13	96.19	96.34	96.19
	Min	96.55	96.21	95.80	95.87	96.03	95.88
	Average	96.73	96.40	95.96	96.03	96.18	96.03

Approved By. _____



Certificate No. T220730

Page 5 of 6

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (° C)					
R1 Hole1-Hole6		TN221	TN222	TN223	TN224	TN225	TN226
CAL POINT	Max	104.47	104.65	104.79	105.31	105.47	105.46
105	Min	104.15	104.27	104.45	104.98	105.14	105.20
	Average	104.31	104.46	104.62	105.15	105.31	105.33
R2 Hole7-Hole12		TN227	TN228	TN229	TN230	TN231	TN232
	Max	105.55	105.73	105.65	105.84	105.97	106.07
	Min	105.28	105.43	105.35	105.52	105.68	105.83
	Average	105.42	105.58	105.50	105.68	105.82	105.95
R3 Hole13-Hole18		TN233	TN234	TN235	TN236	TN237	TN238
	Max	106.14	106.06	105.81	106.05	105.81	105.87
	Min	105.85	105.81	105.55	105.80	105.53	105.64
	Average	106.00	105.94	105.68	105.92	105.67	105.75
R4 Hole19-Hole24		TN239	TN240	TN221	TN222	TN223	TN224
	Max	105.86	105.60	104.44	104.51	104.28	104.78
	Min	105.61	105.37	104.27	104.35	104.12	104.61
	Average	105.74	105.48	104.35	104.43	104.20	104.69
R5 Hole25-Hole30		TN225	TN226	TN227	TN228	TN229	TN230
	Max	104.94	104.93	104.97	105.08	104.68	104.69
	Min	104.77	104.75	104.76	104.90	104.51	104.49
	Average	104.85	104.84	104.86	104.99	104.60	104.59
R6 Hole31-Hole36		TN231	TN232	TN233	TN234	TN235	TN236
	Max	105.44	105.45	105.61	104.95	104.84	104.42
	Min	105.27	105.27	105.44	104.76	104.66	104.25
	Average	105.36	105.36	105.53	104.86	104.75	104.33
R7 Hole37-Hole42		TN237	TN238	TN239	TN240	TN221	TN222
	Max	105.17	104.70	104.59	104.51	105.22	105.53
	Min	105.00	104.53	104.41	104.35	105.04	105.37
	Average	105.08	104.62	104.50	104.43	105.13	105.45
R8 Hole43-Hole48		TN223	TN224	TN225	TN226	TN227	TN228
	Max	105.61	105.45	105.10	104.77	104.87	105.02
	Min	105.44	105.28	104.92	104.60	104.70	104.85
	Average	105.53	105.37	105.01	104.69	104.79	104.93

Approved By. _____



Certificate No. T220730

Page 5 of 6

Calibration Report

Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (± °C)	Uncertainty (± °C)
	Min , Max	Average		
100.0	100.0 , 100.4	100.1	0.29	0.83
105.0	105.0 , 105.4	105.1	0.20	0.79

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By.





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM676

Page.: 1 of 3

Certificate of Calibration

Equipment : Autoclave

Manufacturer : TOMY

Model : SX-700

Serial No. : 48134190

ID No. : BKK_ML0041

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 20 May 2022

Calibration Date : 20 May 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Preecha Hlahib

Approved by :

Approved Signatory

() Pornthippa Tameyakul

() Malee Butkruea

(✓) Suwit Imjai

Issue Date : 24 May 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0041435



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2205-0404OC-2

Cert. No.: 22TM676

Page.: 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Data Acquisition	34972A	MY57013823	22LM24	26 Feb 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**


(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)

It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

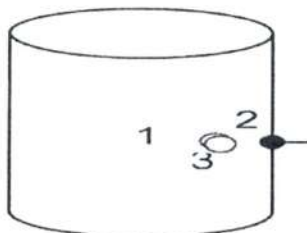

	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	24	55	220
Finished of Calibration	26	57	221

<u>Position</u>	<u>Description</u>	<u>Ref. Std. ID No.:</u>
1 =	Center of chamber	19-17TC-11
2 =	Temperature sensor	19-17TC-12
3 =	Exhaust port	19-17TC-13

Signature



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2205-0404OC-2

Cert. No.: 22TM676
Page.: 3 of 3

Result of Calibration :- (*) Without Adjustment

Operating parameter Set : Temperature = 108 °C
Sterilization period = 10 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
108	108	1	107.536	0.19	0.04	0.91	2
		2	107.542				
		3	107.471				

Operating parameter Set : Temperature = 115 °C
Sterilization period = 20 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
115	115	1	114.502	0.15	0.08	0.89	2
		2	114.582				
		3	114.539				

Operating parameter Set : Temperature = 118 °C
Sterilization period = 10 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
118	118	1	117.517	0.094	0.09	0.88	2
		2	117.616				
		3	117.530				

Result of Calibration :- (*) Without Adjustment

Operating parameter Set : Temperature = 121 °C
Sterilization period = 30 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
121	121	1	120.400	0.18	1.1	0.90	2
		2	120.511				
		3	120.465				

Average* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM102

Page.: 1 of 3

Certificate of Calibration

Equipment : Incubator
Manufacturer : SHEL-LAB
Model : 1915A
Serial No. : 0200599
ID No. : BKK_ML0010

REVIEW BY	Sithichok T.
APPROVED BY	[Signature]
NEXT CAL. DATE	22/07/23

Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Incubation & Micrological Reading

Received Order : 21 January 2022

Calibration Date : 21 January 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

Approved by :

Malee
Approved Signatory

- () Pornthippa Tameyakul
() Malee Butkruea
() Suwit Imjai

Issue Date : 3 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0037377



Equipment : Incubator
 Condition As-Received : Used Item
 Reference : 2201-0616OC-1

Cert. No.: 22TM102

Page.: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Data Acquisition	34972A	MY57013711	21LM7	16 Jun 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

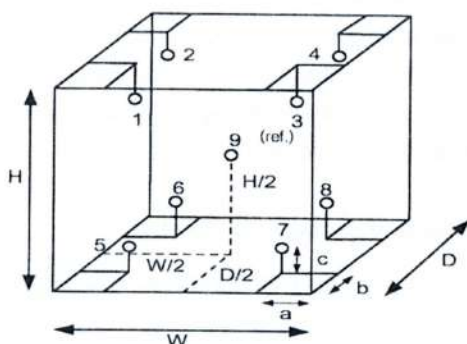

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	25
REL.Humid. (%)	53	54
AC Supply (Volt)	220	221

Position :	Ref. Std. ID No.:
1	18-18RTD-01
2	18-18RTD-02
3	18-18RTD-03
4	18-18RTD-04
5	18-18RTD-05
6	18-18RTD-06
7	18-18RTD-07
8	18-18RTD-08
9 (ref.)	18-18RTD-09

Probe Installation Details :

a = 10 cm
 b = 10 cm
 c = 10 cm

Dimension of Chamber :

D = 0.90 m
 W = 0.75 m
 H = 1.2 m
 Capacity = 0.81 m³

Malu .



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2201-0616OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 22TM102

Page.: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
35.0	35.0	35.0	0.043	0.41	0.42	0.30	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
35.0	34.801	34.868	34.862	35.012	35.040	35.010	35.084	35.040	35.178

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1571

Page : 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Binder

Model : ED 240/E2

Serial No. : 00-15533

ID No. : BKK_ML0013

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 21 November 2022

Calibration Date : 21 November 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

Approved by :

Malee

Approved Signatory

() Pornthippa Tameyakul

(✓) Malee Butkruea

() Suwit Imjai

Issue Date : 29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0048150



Equipment : Hot Air Oven
 Condition As-Received : Used Item
 Reference : 2211-0623OC-1
 Procedure Used :-

Cert. No.: 22TM1571
 Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) After Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	26
REL.Humid. (%)	53	55
AC Supply (Volt)	219	220

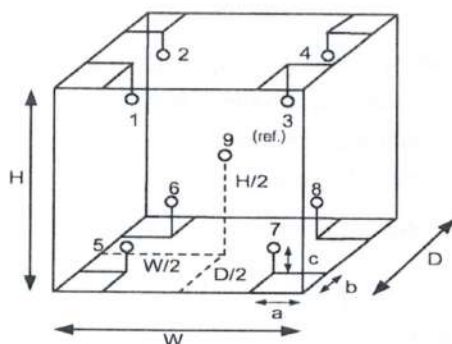

Probe Installation Details :

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of Chamber :

D = 0.50 m
 W = 0.80 m
 H = 0.60 m
 Capacity = 0.24 m³

Position :	Ref. Std. ID No.:
1	21-15TC-01
2	21-15TC-02
3	21-15TC-03
4	21-15TC-04
5	21-15TC-05
6	21-15TC-06
7	21-15TC-07
8	21-15TC-08
9 (ref.)	21-15TC-09

Malu.



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1
Result of Calibration :- (*) After Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 22TM1571
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
180	180	180	0.70	1.5	2.9	1.4	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
180	179.520	180.585	178.855	179.482	178.827	179.938	179.074	180.199	180.068

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM677

Page.: 1 of 3

Certificate of Calibration

Equipment : Water Bath
Manufacturer : Memmert
Model : WNE 45
Serial No. : L712.0429
ID No. : BKK_ML0056
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang ,
Bangkok 10250 Thailand
Location : Incubator & Microbiological Reading
Received Order : 20 May 2022
Calibration Date : 20 May 2022
Ambient Temperature : (26 $\pm$ 10) °C
Relative Humidity : (50 $\pm$ 30) %
Calibrated by : Preecha Hlahib

REVIEW BY	Sithichok
APPROVED BY	[Signature]
NEXT CAL. DATE	20/5/23

Approved by :

[Signature]
Approved Signatory

- () Pornthippa Tameyakul
() Malee Butkruea
(☒) Suwit Imjai

Issue Date :

24 May 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0041433



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2205-0404OC-1

Cert. No.: 22TM677

Page.: 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Data Acquisition	34972A	MY57013823	22LM24	26 Feb 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

	<u>Environmental</u>		<u>AC Voltage Supply</u>
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	24	47	220
Finished of Calibration	24	52	221

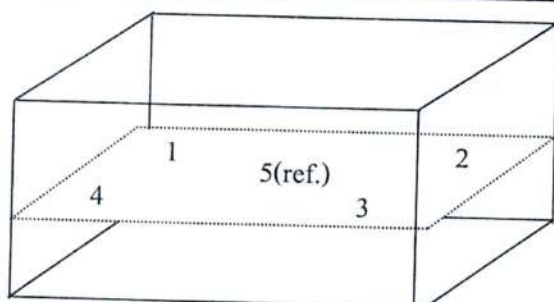

Front

<u>Position :</u>	<u>Ref. Std. S/N.:</u>
1	4804539-006
2	4804539-007
3	4804539-008
4	4804539-009
5(ref.)	4804539-010

Signature



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2205-0404OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 22TM677

Page.: 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)				
			Position				
			1	2	3	4	5 (ref.)
44.5	44.4	44.4	44.539	44.497	44.476	44.506	44.507

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
44.5	0.068	0.030	0.15	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Sanit