

4.3 เอกสารสอบเทียบเครื่องมือ
(บริษัท เอ็ม กรีน กรุ๊ป จำกัด ทะเบียนเลขที่ ว-299)

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No.23-66/0161

MTC.No.23-66/0161

Number of page(s) 2

CALIBRATION CERTIFICATE

Nomenclature : MASS FLOWMETER

Manufacturer : TSI

Serial No.: 41461443012

Model : 4199

Scale range : 0 l/min to 20 l/min

Subdivision : 0.001 l/min

Submitted by : M GREEN GROUP CO.,LTD

188/46, Pracha-Utid Rd.,

Thungkru, Bangkok 10140, Thailand.

Received date : 10 January 2023

Condition of measured item : Normal

Calibration date : 18 January 2023

Standard :

Standard	Certificate No.	Date due	Traceability
RTD Thermometer	PSL-T 643/65	1-Jun-24	TISTR
Molbox/PressureTransducer/UpStream	MP-0013-21	25-Jan-23	NIMT
Primary Flow Calibrator S/N 117982	MW-0011-21	8-Apr-23	NIMT
Primary Flow Calibrator S/N 119521	MW-0012-21	31-Mar-23	NIMT

Calibrated by :

Approved by

Director

Mechanical Engineering Standards Laboratory

Ref. 2013266011000059001

Issued Date 18 January 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
 Changwat Pathumthani 12120, Thailand
 Tel. (66) 0 2577 9000
 Fax. (66) 0 2577 9009
 E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
 Amphoe Muang, Changwat Samutprakan 10280, Thailand
 Tel. (66) 0 2323 1672-80 ext. 115, 116
 Fax. (66) 0 2323 9165
 E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
 Thailand
 Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
 Fax. (66) 0 2579 8592
 E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No.23-66/0161

2/2

MTC.No.23-66/0161

Calibration point : (0.05, 0.1, 0.2, 0.3, 0.4, 0.5, 1, 2, 3) l/min

Ambient condition : Temperature (23 ± 3) °C , Relative humidity (55 ± 15) %

Atmospheric pressure (1010 ± 13) hPa

Calibration method : The flowmeter (UUC) was calibrated by comparison method with standard flowmeter according to CP-370.01.


The reported value is the value that converted to value at reference condition within pressure and temperature of the actual gas entering the UUC

Measurement data :

UUC Value (l/min)	Standard Value (l/min)	Temperature (°C)	Pressure (hPa)	Deviation (%)	Uncertainty (%)
0.054	0.0572	24.920	1008.08	-5.52	1.42
0.105	0.1060	24.903	1008.16	-0.90	1.13
0.204	0.2058	24.897	1008.25	-0.88	1.02
0.304	0.3038	24.922	1008.32	-0.05	1.02
0.402	0.4039	24.937	1008.38	-0.47	1.03
0.504	0.5032	24.919	1008.45	+0.23	1.02
0.999	0.9948	24.906	1008.60	+0.45	0.92
2.003	1.9789	24.922	1009.20	+1.22	0.87
3.007	2.9759	24.923	1009.90	+1.04	0.87

The reported expanded uncertainties are based on standard uncertainties multiplied by a coverage factor $k=2$, which provides a level of confidence of approximately 95%.

The end of calibration certificate.



The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

Certificate of Calibration

Certificate No. : 65-200300-1

Page : 1 of 2

Submitted by : M Green Group Co., Ltd.

188/46 Wisatesuknakhon 25, Pracha-Utid Rd., Thungkru, Bangkok 10140 Thailand

Equipment : Electronic Balance

Manufacturer : SHIMADZU

Model : AP225WD

Serial No. : D316300690

Capacity : 220 g

Resolution : 0.00001g/102g, 0.0001g/220g

Environment : On site calibration was carried out at the Laboratory, M Green Group Co., Ltd.

Ambient Temperature : (26.1 to 26.3) °C

Relative Humidity : (62.1 to 64.5) %

Air Pressure : 1007.0 mbar

Date of Received : 21 September 2022

Date of Calibration : 21 September 2022

Date of Issue : 24 September 2022

Calibrated by : Akaradath Thippichai


Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 5, July 2015

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02213103	18 Nov 2022	National Institute of Metrology (Thailand), (NIMT)

Approved by :



Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-200300-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.001	0.00001	0.000012
0.01	0.00000	0.000014
0.1	0.00001	0.000018
1	0.00000	0.000026
10	0.00000	0.000053
20	-0.00001	0.000071
50	0.00001	0.00011
100	-0.00008	0.00020
150	-0.0001	0.00038
200	-0.0001	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.15$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A B C D E

0.00001 0.00006 0.00004 -0.00006 0.00000 g




Repeatability

Load test : 200 g

Stdev. : 0.000053 g

- o0o -



Certificate of Calibration

Certificate No. : 65-210457-1

Page : 1 of 2

Submitted by : M Green Group Co., Ltd.

188/46 Wisasuknakhon25, Pracha-Utid Rd., Thungkru, Bangkok 10140 Thailand

Equipment : Weight

Manufacturer : N/A

Material : Stainless Steel

Weight size : 1 g

ID No. : 63-210391-1

Assumed density of weight : 7950 kg / m³

Assumed Air density : 1.2 kg / m³

Environment : Ambient Temperature : (20 ± 2) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1001.1 mbar

Date of Received : 21 September 2022

Date of Calibration : 28 September 2022

Date of Issue : 28 September 2022

Calibrated by : Wuttichai Swatphong

Calibration Method : In-house method CAL-M2101 based on OIML R 111-1 : 2004(E)

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.

Cert. No.

Due Date

Traceability

E221-E2210

MM-0042-22

21 Mar 2025

National Institute of Metrology (Thailand), (NIMT)

Approved by

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-210457-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

No.	Nominal Value	Id.Mark	Conventional mass Value		Measuring Uncertainty
1	1 g	none	1 g	-0.016 mg	\pm 0.023 mg

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -

CAL



Certificate of Calibration

Certificate No. : 65-210457-2

Page : 1 of 2

Submitted by : M Green Group Co., Ltd.

188/46 Wisasuknakhon25, Pracha-Utid Rd., Thungkru, Bangkok 10140 Thailand

Equipment : Weight

Manufacturer : N/A

Material : Stainless Steel

Weight size : 100 g

ID No. : 63-210391-2

Assumed density of weight : 7950 kg / m³

Assumed Air density : 1.2 kg / m³

Environment : Ambient Temperature : (20 ± 2) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1001.8 mbar

Date of Received : 21 September 2022

Date of Calibration : 28 September 2022

Date of Issue : 28 September 2022

Calibrated by : Wuttichai Swatphong

Calibration Method : In-house method CAL-M2101 based on OIML R 111-1 : 2004(E)

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.

Cert. No.

Due Date

Traceability

E221-E2210

MM-0042-22

21 Mar 2025

National Institute of Metrology (Thailand), (NIMT)

Approved by :

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-210457-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

No.	Nominal Value	Id.Mark	Conventional mass Value		Measuring Uncertainty
1	100 g	none	100 g	-0.17 mg	\pm 0.11 mg

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -

CAL



www.calibratech.co.th

Certificate of Calibration

Certificate No. : 65-210457-3

Page : 1 of 2

Submitted by : M Green Group Co., Ltd.

188/46 Wisasuknakhon25, Pracha-Utid Rd., Thungkru, Bangkok 10140 Thailand

Equipment : Weight

Manufacturer : N/A

Material : Stainless Steel

Weight size : 200 g

ID No. : 63-210391-3

Assumed density of weight : 7950 kg / m³

Assumed Air density : 1.2 kg / m³

Environment : Ambient Temperature : (20 ± 2) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1001.8 mbar

Date of Received : 21 September 2022

Date of Calibration : 28 September 2022

Date of Issue : 28 September 2022

Calibrated by : Wuttichai Swatphong

Calibration Method : In-house method CAL-M2101 based on OIML R 111-1 : 2004(E)

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E221-E2210	MM-0042-22	21 Mar 2025	National Institute of Metrology (Thailand), (NIMT)

Approved by :

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-210457-3

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

No.	Nominal Value	Id.Mark	Conventional mass Value		Measuring Uncertainty
1	200 g	none	200 g	+0.09 mg	\pm 0.17 mg

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

CAL




www.calibratech.co.th

TEST REPORT

CUSTOMER NAME : M GREEN GROUP COMPANY LIMITED			
EQUIPMENT NAME : SO ₂ Analyzer			
MANUFACTURER : HORIBA	MODEL : APSA-370	SERIAL NO : G8KGHRMX	
STANDARD GAS CONCENTRATION (PPM) : 53.29 PPM		CYLINDER NO : CC734373	
CYLINDER PRESSURE (PSI) : 1,000 PSI		CERTIFIED DATE : 12/05/2020	
CERTIFIED BY : AIRGAS		EXPIRED DATE : 12/05/2028	

TEST RESULTS

POINT NO	TEST RESULTS			
	IDEAL	ACTUAL	ERROR	%ERROR
ZERO	0.00	0.050	0.05	-
1	100.00	99.010	-1.0	-0.99
2	200.00	200.420	0.4	0.21
3	300.00	300.460	0.5	0.15
4	400.00	400.650	0.6	0.16
AVERAGE (%)				0.12

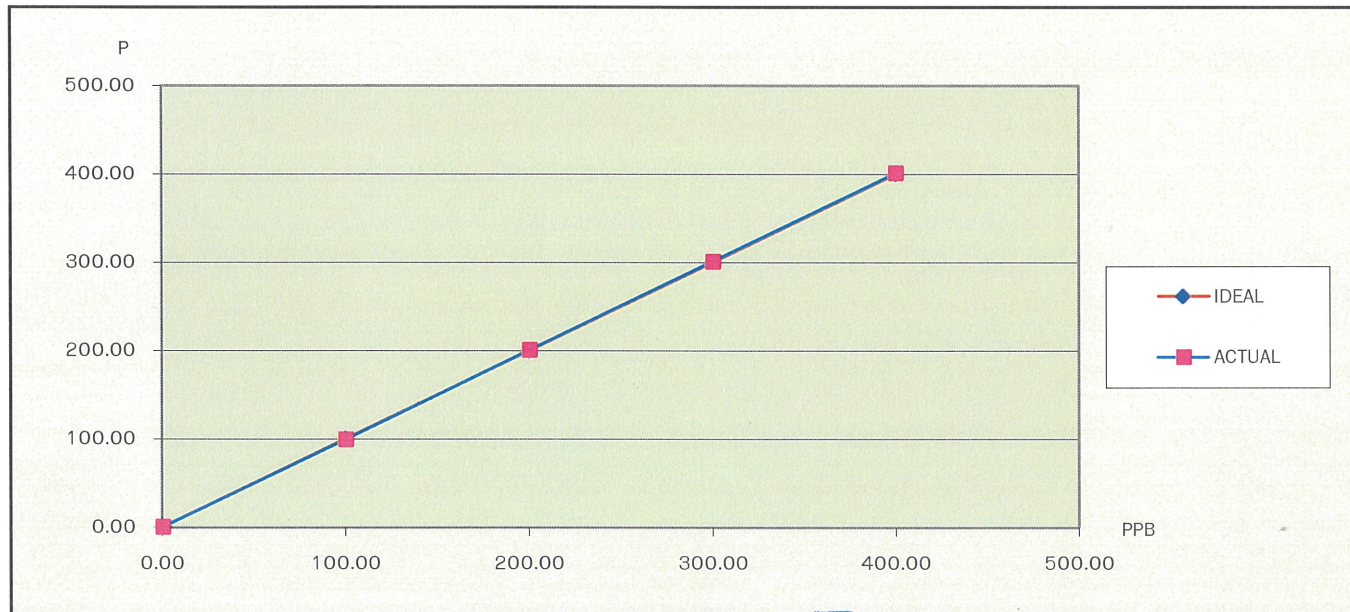

CALIBRATED BY :

DATE :

11/10/65

CHECKED BY :

DATE :

11/10/65

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ถนน ซอยเพชรเกษม 7,7/1 เพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02-868-1889

CHECK LIST

CUSTOMER NAME : M GREEN GROUP COMPANY LIMITED		
EQUIPMENT NAME : SO ₂ Analyzer		
MANUFACTURER : HORIBA	MODEL : APSA-370	SERIAL NO. : G8KGHRMX

TEST VALUES				
NO.	Ambient SO ₂ Monitor	UNIT	BEFORE	AFTER
1	SIGNAL	mV (Voltage of the measured SO ₂ Value)	6.40	9.30
2	LAMP	mV (200mV to 1200 mV)	719.10	1001.70
3	CELL	°C (Ambient tembient temperature +(5°C to 15°C))	38.90	32.20
4	PUMP	kPa (65 kPa or less)	44.40	46.00
5	AMBIENT	kPa	101.50	101.80
6	SAMPLE	L/min (0.6 L/min to 1.0 L/min)	-	-
7	DC 24 V	V (24 V ± 0.5 V)	23.90	23.90
8	DC 5 V	V (5 V ± 0.5 V)	5.00	5.00
9	SAMPLE SO2 Reading	PPB	3.77	0.41
10	Zero	PPB	0.41	0.05
11	Span	PPB	420.10	400.65

Remark : Reference EX-EN-019-56 , Ambient SO2 Monitor APSA-370 Operation Manual Page #78

(Ambeint temperature = 5°C to 40°C)

อาการที่ตรวจพบ

-

รายละเอียดการดำเนินการ

-

ผลการดำเนินการ

- เรียบร้อย เครื่องสามารถดำเนินการตรวจวัดได้ตามปกติ

CALIBRATED BY :

DATE : 11/10/65

CHECKED BY :

DATE : 11/10/65

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com


เลขที่ 63/14-15 , 67/35-36 ซอยเพชรเกษม 7,7/1 ถนนเพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร : 02-868-0812-13 โทรสาร : 02-868-1889

TEST REPORT

CUSTOMER NAME : M GREEN GROUP COMPANY LIMITED			
EQUIPMENT NAME : NO _x Analyzer			
MANUFACTURER : HORIBA	MODEL : APNA-370	SERIAL NO : RSBHK673	
STANDARD GAS CONCENTRATION (PPM) : 53.15 PPM		CYLINDER NO : CC734373	
CYLINDER PRESSURE (PSI) : 1,000 PSI		CERTIFIED DATE : 12/05/2020	
CERTIFIED BY : AIRGAS		EXPIRED DATE : 12/05/2028	

TEST RESULTS

POINT NO	TEST RESULTS						
	IDEAL	ACTUAL NO	ERROR NO	%ERROR NO	ACTUAL NO _x	ERROR NO _x	%ERROR NO _x
ZERO	0.00	-0.43	-0.43	-	-0.13	-0.13	-
1	100.00	99.54	-0.46	-0.46	99.40	-0.60	-0.60
2	200.00	198.72	-1.28	-0.64	198.71	-1.29	-0.64
3	300.00	299.84	-0.16	-0.05	299.91	-0.09	-0.03
4	400.00	400.27	0.27	0.07	400.12	0.12	0.03
AVERAGE (%)				-0.27			-0.31

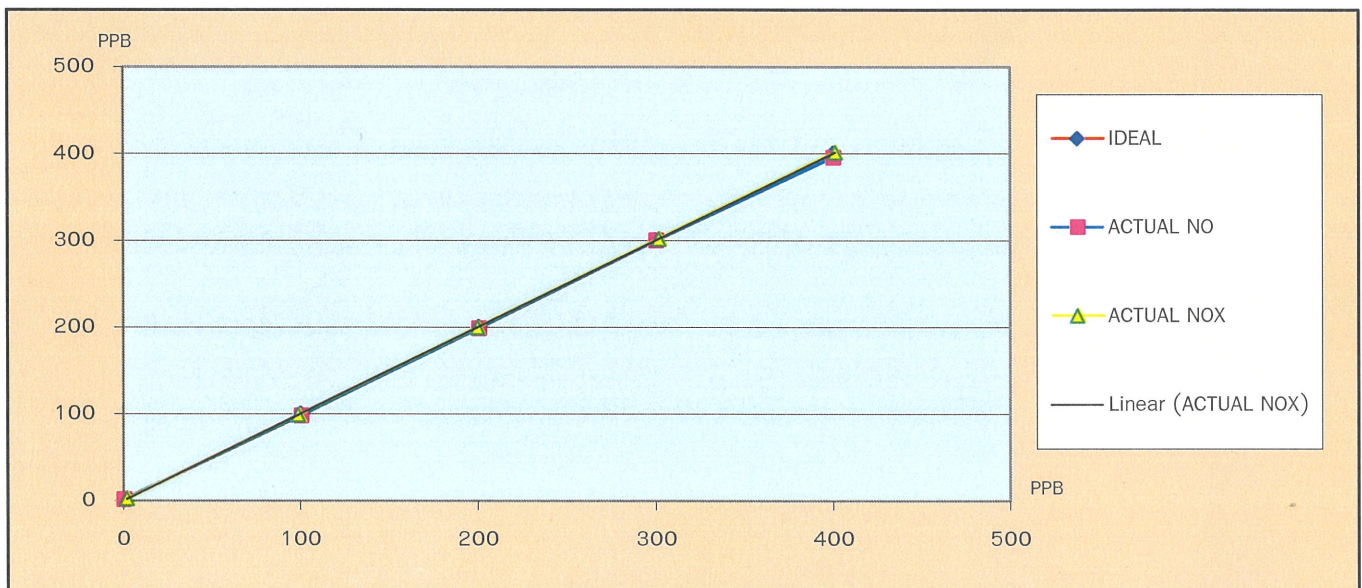

CALIBRATED BY :

DATE :

11/10/65

CHECKED BY :

DATE :

11/10/65

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15,16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ซอยนพพรเกษม 7,7/1 ถนนเพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02-868-1889

CHECK LIST

CUSTOMER NAME : M GREEN GROUP COMPANY LIMITED		
EQUIPMENT NAME : NO _x Analyzer		
MANUFACTURER : HORIBA	MODEL : APNA-370	SERIAL NO. : RSBHK673

TEST VALUES				
NO.	NO _x Analyzer (APNA-370)	UNIT	BEFORE	AFTER
1	Signal (NO)	mV	4.300	2.900
2	Signal (NO _x)	mV	15.300	9.700
3	Detector	Temp °C , Standard Value : Ambient temp+(5°Cto15°C)	42.900	42.900
		Pressure kPa , Standard Value : (Ambient/1013x100-20)±4kPa	77.900	77.600
4	AMBIENT	kPa	101.500	101.200
5	SAMPLE	L/min (1.1 L/min ± 0.3 L/min)	-	-
6	DC 24 V	V (24 V ± 0.5 V)	23.700	23.900
7	DC 5 V	V (5 V ± 0.5 V)	5.000	5.000
8	Sampling NO Reading	PPB	5.610	3.710
9	Sampling NO ₂ Reading	PPB	15.280	12.560
10	Sampling NO _x Reading	PPB	20.900	16.280
11	Zero (NO)	PPB	0.420	-0.430
12	Span(NO)	PPB	390.120	400.270
13	Zero (NO _x)	PPB	4.150	-0.130
14	Span (NO _x)	PPB	396.410	400.120

Remark : Reference EX-EN-022-56 , "Ambient NO_x Monitor APNA-370 Operation Manual " Page #48

(Ambient temperature = 5°C to 40°C)

อาการที่ตรวจพบ

-

รายละเอียดการดำเนินการ

-

ผลการดำเนินการ

- เรียบร้อย เครื่องสามารถดำเนินการตรวจวัดได้ตามปกติ

CALIBRATED BY :

DATE : 11/10/65

CHECKED BY :

DATE : 11/10/65

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com


เลขที่ 63/14-15,67/35-36 ซอยเพชรเกษม 7,7/1 ถนนเพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02-868-1889

TEST REPORT

CUSTOMER NAME : M GREEN GROUP COMPANY LIMITED			
EQUIPMENT NAME : CO Analyzer			
MANUFACTURER : HORIBA	MODEL : APMA-370	SERIAL NO : 84XJ1GRC	
STANDARD GAS CONCENTRATION (PPM) : 4533 PPM		CYLINDER NO : CC734373	
CYLINDER PRESSURE (PSI) : 1,000 PSI		CERTIFIED DATE : 12/05/2020	
CERTIFIED BY : AIRGAS		EXPIRED DATE : 12/05/2028	

TEST RESULTS

POINT NO	CALIBRATION RESULTS			
	IDEAL	ACTUAL	ERROR	%ERROR
ZERO	0.00	0.0000	0.00	-
1	10.00	10.0800	0.1	0.80
2	20.00	20.1200	0.1	0.60
3	30.00	30.1600	0.2	0.53
4	40.00	40.0100	0.0	0.02
AVERAGE (%)				0.49

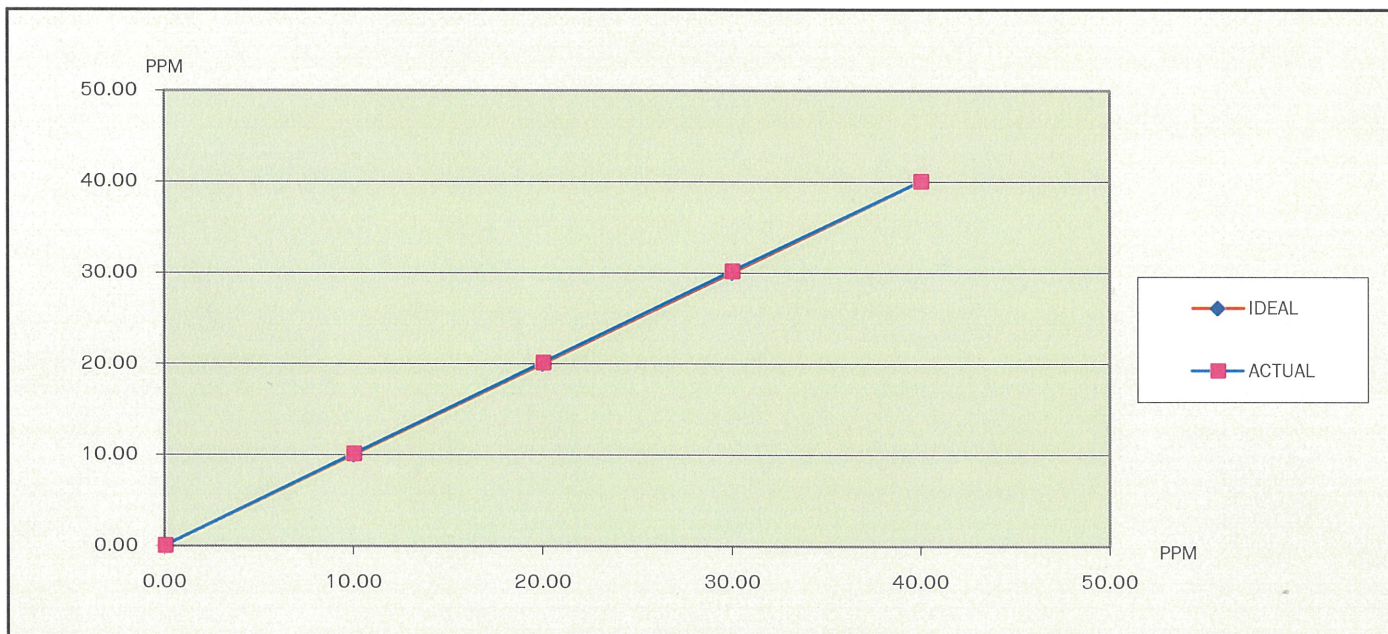

CALIBRATED BY : [REDACTED]

DATE : 11 / 10 / 65

CHECKED BY : [REDACTED]

DATE : 11 / 10 / 65

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-8681246 , E-Mail : Sales@okla-testing.com
63/14-15,67/35-36 ซอยเพชรเกษม 7,7/1 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 เบอร์โทร 02-8681246 แฟกซ์ 02-8680860

CHECK LIST

CUSTOMER NAME : M GREEN GROUP COMPANY LIMITED

EQUIPMENT NAME : CO Analyzer

MANUFACTURER : HORIBA

MODEL : APMA-370

SERIAL NO. : 84XJ1GRC

TEST VALUES

NO.	CO Analyzer (APMA-370)	UNIT	BEFORE	AFTER
1	Signal (MAIN)	mV	-0.200	4.000
2	Signal (COMP)	mV	0.000	0.200
3	CELL	°C , Standard Value : Ambient temperature +(5°Cto15°C)	35.600	35.400
4	PUMP	kPa	39.600	39.700
5	AMBIENT	kPa	101.300	101.500
6	SAMPLE	L/min (1 L/min to L/min)	-	-
7	OVER FLOW	L/min (1.2 L/min or more)	0.000	0.000
8	DC 24 V	V (24 V ± 0.5 V)	23.900	23.900
9	DC 5 V	V (5 V ± 0.5 V)	4.900	4.900
10	Sample Reading	PPM	0.370	0.250
11	Zero	PPM	0.370	0.000
12	Span	PPM	37.000	40.010

Remark : Reference EX-SM-100-58 , "Ambient CO Monitor APMA-370 Operation Manual" Page #48

(Ambient temperature = 5°C to 40°C)

อาการที่ตรวจพบ

-

รายละเอียดการดำเนินการ

- ทำ Check List Analyzer , ทำ Calibration Zero/Span , Multipoint , เช็ค Diagnostics

ผลการดำเนินการ

- เรียบร้อย เครื่องสามารถดำเนินการตรวจวัดได้ตามปกติ

CALIBRATED BY :

DATE :

11 / 10 / 65

CHECKED BY :

DATE :

11 / 10 / 65

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ซอยเพชรเกษม 7,7/1 ถนนเพชรเกษม แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02-868-1889



Certificate of Calibration

Certificate Number : SPR23030320-2

Page : 1 of 3

Customer : M Green Group Co.,Ltd

188/46, Pracha-Utid Rd., Thungkru, Bangkok 10140, Thailand

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 45

Serial Number : PN2448

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 20 Mar 2023

Relative Humidity : 50 % \pm 15 %

Calibration Date : 22 Mar 2023

Location of Calibration : In-Lab

Recommend Due Date : 22 Mar 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 23 Mar 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Approved by :

Calibration Officer

Authorized Signatory



Calibration Report

Certificate Number : SPR23030320-2

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23030320-2

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23030320-1

Page : 1 of 3

Customer : M Green Group Co.,Ltd

188/46, Pracha-Utid Rd., Thungkru, Bangkok 10140, Thailand

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 45

Serial Number : PN2453

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 20 Mar 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 22 Mar 2023

Location of Calibration : In-Lab

Recommend Due Date : 22 Mar 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 23 Mar 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Approved by

Calibration Officer

Authorized Signatory



Calibration Report

Certificate Number : SPR23030320-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23030320-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.8	93.8	-0.2	-0.2	0.15
114	113.7	113.7	-0.3	-0.3	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

– End of Certificate –



**ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT**

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20230034EA

Operation No.: CP2023010028

Certificate of Calibration

Equipment: Sound Calibrator

Manufacturer: Scarlet Tech

Model/Type: ST-120

Serial No.: ST120C0247E

ID No.: -

Customer: M Green Group Co.,Ltd.

Address: 188/46, Pracha-Utid Rd.,
Thungkru, Bangkok 10140 Thailand.

Received Date: 12 January 2023

Calibrated Date: 16 January 2023

Issued Date: 18 January 2023

Calibrated by: Ms. Juntaporn Kunhakom

Approved by

Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20230034EA

Calibration Report

Equipment: Sound Calibrator
Manufacturer: Scarlet Tech
Model/Type: ST-120
Serial No.: ST120C0247E
ID No.: -
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-

IEC 60942:2017

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2661000	AA-1020-22	14 June 2023
2) Waveform Generator	33511B	MY52302264	CK20220058EA	19 June 2023
3) Audio Analyzing DMM	2015-P	4079144	E1U221042	16 March 2023
4) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P220024 CD20220164EA	17 March 2023 24 July 2023

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

1. Function : Sound pressure level

Norminal Frequency (Hz)	Specified Sound Pressure level (dB)	Measured value (dB)	Deviated value ^[1] (dB)	Acceptance limit ^[3] (dB)
1000	94	94.04	0.04	±0.25
1000	114	114.10	0.10	±0.25

2. Function : Frequency

Norminal Sound Pressure level (dB)	Specified Frequency (Hz)	Measured value (Hz)	Deviated value ^[2] (%)	Acceptance limit ^[3] (%)
94	1000	999.5	0.0	±0.7
114	1000	999.6	0.0	±0.7

Certificate No.: CP20230034EA

Calibration Report

3. Function : Total distortion + noise

Normal Sound Pressure level (dB)	Normal Frequency (Hz)	Measured value ^[4] (%)	Acceptance limit ^[5] (%)
94	1000	0.5	2.5
114	1000	0.4	2.5

Uncertainty of measurement

Function	Uncertainty	Maximum-permitted uncertainty of measurement
Sound pressure level	0.10 dB	0.15 dB
Frequency	0.10 %	0.20 %
Total distortion + noise	0.40 %	0.50 %

- Note:
- [1] The deviated value is the absolute value of the difference between the measured value and the corresponding specified sound pressure level.
 - [2] The deviated value is the absolute value of the difference in percent between the measured value and the corresponding specified frequency.
 - [3] The acceptance limit is for the deviated value.
 - [4] The measured value is the total distortion + noise, measured over the frequency range from 20 Hz to 20 kHz.
 - [5] The acceptance limit is for the Measured value.

Remarks: 1. Acceptance limit was IEC 60942:2017 Class 1.
2. The coverage factor $k = 2.00$

-- End of Report --



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



Supplement to Calibration Certificate No. Q22102976

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : N/A
MODEL / TYPE : V9000
SERIAL NO. : 2364
CLID. NO. : 252102170
JOB CONTROL NO. : 221008102976


CUSTOMER : **M GREEN GROUP COMPANY LIMITED**
188/47 PRACHA UTHIT RD.,
BANG MOT, THUNG KHRU, BANGKOK 10140

DATE OF RECEIVED : 08 October 2022

DATE OF ISSUED : 19 October 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong
Calibration Engineer

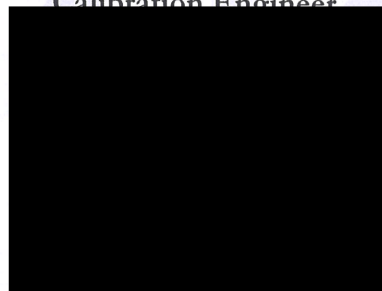

Approved By :

Authorized Signatory
19 October 2022



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22102976A1

F3-012-04/01-12

page 1 of 3



ภาพผนวก ๑-4/41

REPORT OF CALIBRATION FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : N/A
MODEL / TYPE : V9000
SERIAL NO. : 2364
DATE OF CALIBRATION : 10 October 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-127** based on **ISO 16063-21** as calibration guideline.

The calibration was performed by using Digital Multimeter, High Resolution Programmable Timer/Counter, Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Digital Multimeter, Hewlett Packard Model 34401A S/N. 3146A75935.
2. High Resolution Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2525 S/N. 397018, 2434988.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0112-21, Due Date 26 October 2022.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0001/22, Due Date 22 February 2023.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0009-22, Due Date 22 June 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22102976

F3-011-04/01-12

page 2 of 3





CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	\pm (% of rdg.)
10	160 Hz	peak	10.00	10.03	-0.03	1.0
20	160 Hz		20.00	20.02	-0.02	1.0
40	160 Hz		40.00	39.22	+0.78	1.0
60	160 Hz		60.00	57.60	+2.40	1.0
80	160 Hz		80.00	77.21	+2.79	1.0
100	160 Hz		100.00	96.25	+3.75	1.0

Note. The Scope of Accredited TISI Certificate No. 19C087/0655 Issue 1 Page 57 of 111

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22102976

F3-011-04/01-12

page 3 of 3

