



บริษัท ปตท. น้ำมันและ การค้าปลีก จำกัด (มหาชน)

รายงานผลการปฏิบัติตามมาตรการป้องกันและแก้ไขผลกระทบสิ่งแวดล้อม

และมาตรการติดตามตรวจสอบผลกระทบสิ่งแวดล้อม

โครงการปรับปรุงท่าเทียบเรือขนถ่ายน้ำมันและก๊าซปิโตรเลียมเหลว จังหวัดสุราษฎร์ธานี

ระหว่างเดือนกรกฎาคม - ธันวาคม พ.ศ. 2566

ภาคผนวก จ

เอกสารสอบเทียบเครื่องมือ

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Total Hydrocarbon	Total Hydrocarbon Analyzer	BKK_EN0057	9-Aug-22	9-Feb-24	18
Ambient	Total VOC	TVOC Analyzer	BKK_FS0820	8-Sep-23	8-Mar-25	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	SGK_FS0089	13-Jan-23	13-Jul-24	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	SGK_FS0035	13-Jul-22	11-Jan-24	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	SGK_FS0088	13-Jan-23	13-Jul-24	18
Noise	Leq 24 hrs	Sound Calibrator	SGK_FS0114	14-Nov-22	14-Nov-23	12
Noise	Leq 24 hrs	Sound Level Meter	SGK_FS0131	27-Mar-23	27-Mar-24	12
Water Lab	Cadmium	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Cadmium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Cadmium	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Lead	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Lead	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Lead	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	BOD	DO Meter	BKK_EN0205	3-Aug-22	3-Feb-24	18
Water Lab	BOD	Incubator	BKK_EN0272	5-Jul-23	5-Jul-24	12
Water Lab	BOD	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	COD	Hot Block	BKK_EN0222	25-Apr-23	25-Apr-24	12
Water Lab	COD	Spectrophotometer	BKK_EN0018	15-Sep-23	15-Sep-24	12
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0003	9-Aug-23	9-Aug-24	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0148	4-Jul-23	4-Jan-25	18
Water Lab	pH at 25 °C	pH meter	BKK_EN0072	12-Sep-22	12-Mar-24	18
Water Lab	Temperature	pH meter	BKK_LG0044	26-Sep-23	26-Sep-24	12
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0003	9-Aug-23	9-Aug-24	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Water Lab	Total Kjeldahl Nitrogen	Digestion Unit	BKK_EN0366	17-May-23	17-May-24	12
Water Lab	Total Kjeldahl Nitrogen	Discrete analyzer	BKK_EN0037	12-Jul-23	12-Jul-24	12
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Water Lab	Fecal Coliform	Autoclave	BKK_ML0037	17-Jul-23	17-Jan-25	18
Water Lab	Fecal Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	Fecal Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Fecal Coliform	Water Bath	BKK_ML0056	20-Apr-23	20-Apr-24	12
Water Lab	Total Solids	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Solids	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Water Lab	Total Coliform	Autoclave	BKK_ML0037	17-Jul-23	17-Jan-25	18
Water Lab	Total Coliform	Incubator	BKK_ML0011	21-Nov-22	21-May-24	18
Water Lab	Total Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Songkhla Lab	Fecal Coliform	Autoclave	SGK_ML0001	5-Jan-23	5-Jul-24	18
Songkhla Lab	Fecal Coliform	Incubator	SGK_ML0013	6-Aug-22	6-Feb-24	18
Songkhla Lab	Fecal Coliform	pH Meter	SGK_ML0016	5-Jan-23	5-Jul-24	18
Songkhla Lab	Fecal Coliform	Water Bath	SGK_ML0021	30-Jan-23	30-Jul-24	18
Songkhla Lab	Total Coliform	Autoclave	SGK_ML0001	5-Jan-23	5-Jul-24	18
Songkhla Lab	Total Coliform	Incubator	SGK_ML0013	6-Aug-22	6-Feb-24	18
Songkhla Lab	Total Coliform	pH Meter	SGK_ML0016	5-Jan-23	5-Jul-24	18
Songkhla Lab	Total Coliform	Water Bath	SGK_ML0021	30-Jan-23	30-Jul-24	18
Songkhla Lab	BOD	Incubator	SGK_CL0028	13-Jul-23	13-Jan-25	18
Songkhla Lab	BOD	DO/BOD Analyser	SGK_CL0073	21-Nov-22	21-May-24	18
Songkhla Lab	Conductivity	Conductivity Meter	SGK_CL0032	3-May-23	3-May-24	12
Songkhla Lab	Oil & Grease	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Oil & Grease	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Oil & Grease	Water Bath	SGK_CL0035	13-Jul-23	13-Jan-25	18
Songkhla Lab	pH at 25 °C	pH meter	SGK_CL0030	28-Apr-23	28-Oct-24	18
Songkhla Lab	Salinity	Conductivity meter	SGK_CL0032	3-May-23	3-May-24	12
Songkhla Lab	Temperature	Digital Thermometer With Sensor	SRT_FS0018	8-Jun-23	8-Jun-24	12
Songkhla Lab	Total Alkalinity	pH meter	SGK_CL0030	28-Apr-23	28-Oct-24	18
Songkhla Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Total Dissolved Solids 180°C	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Total Dissolved Solids 180°C	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Turbidity	Turbidity Meter	SGK_FS0045	22-May-23	22-May-24	12



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Water Lab	Ammonia Nitrogen	Discrete analyzer	BKK_EN0037	12-Jul-23	12-Jul-24	12
Water Lab	Nitrate	Ion Chromatography	BKK_EN0069	12-Jan-23	12-Jan-24	12
Water Lab	Phosphate	Ion Chromatography	BKK_EN0069	12-Jan-23	12-Jan-24	12
Sludge	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Sludge	Total Petroleum Hydrocarbon	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Sludge	pH aqueous phase 50% (w/v)	pH meter	BKK_EN0072	12-Sep-22	12-Mar-24	18



JIRANATEE ASSOCIATES CO.,LTD.

CALIBRATION REPORT

REVIEW BY Vichuta N.


APPROVED BY Sararat M.

NEXT CAL. DATE 9/2/67

CUSTOMER NAME : ALS Laboratory Group (Thailand) Co., Ltd.	
EQUIPMENT NAME : Total Hydrocarbon Analyzer	
MANUFACTURER : Baseline	MODEL : 9000 NMHC
SERIAL NO : 0314DR0170	
STANDARD GAS CONCENTRATION (PPM) : 100 PPM (Methane)	
CYLINDER NO : ND55981	
CYLINDER PRESSURE (psig) : 900 PSI	
CERTIFIED DATE : 12/02/2022	
CERTIFIED BY : AIRGAS	
EXPIRED DATE : 12/02/2025	

CALIBRATION RESULTS

POINT NO	CALIBRATION RESULTS			
	IDEAL	ACTUAL	ERROR	%ERROR
ZERO	0.00	0.00	0.00	-
1	100.00	101.00	1.0	-1.00
AVERAGE (%)				0.25

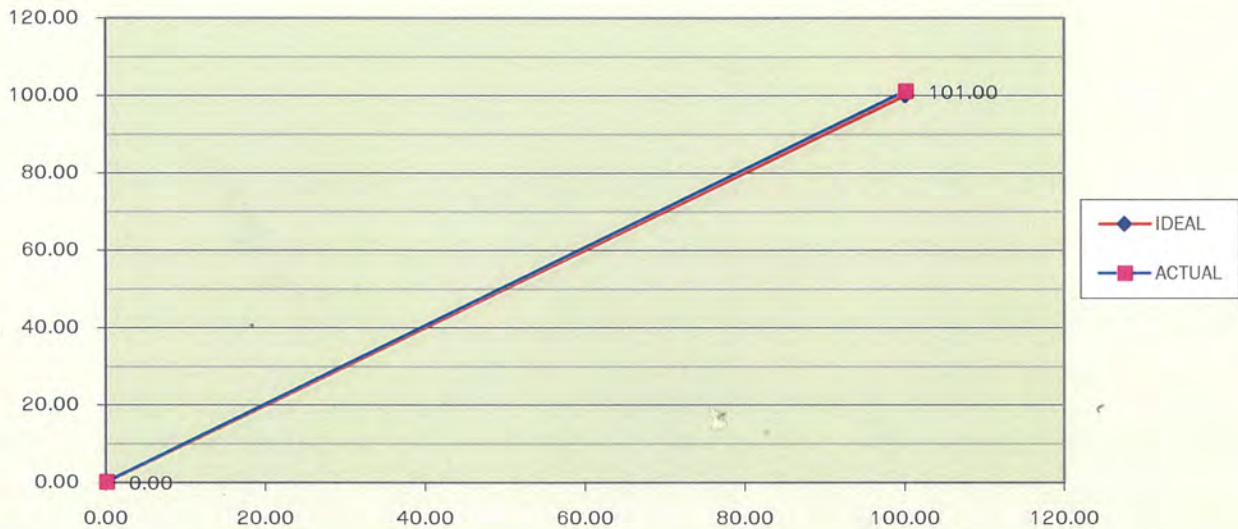

CALIBRATED BY

DATE :

9/8/65

CHECKED BY

DATE :

9/8/65

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 31 , E-Mail : Engineer@Jiranatee.com


เลขที่ 63/14-15,67/35-36 ถนน เพชรเกษม7,7/1 แขวง วัดท่าพระ เขต บางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02868-1889

CALIBRATION REPORT

CUSTOMER NAME :		ALS Laboratory Group (Thailand) Co., Ltd.		
EQUIPMENT NAME :		Total Hydrocarbon Analyzer		
MANUFACTURER :		Baseline	MODEL :	9000 NMHC
			SERIAL NO :	0314DR0170
STANDARD GAS CONCENTRATION (PPM) :		: 100 PPM (Propane)		CYLINDER NO : ND55981
CYLINDER PRESSURE (psig) :		900 PSI		CERTIFIED DATE : 12/02/2022
CERTIFIED BY :		AIRGAS		EXPIRED DATE : 12/02/2025

CALIBRATION RESULTS

POINT NO	CALIBRATION RESULTS			
	IDEAL	ACTUAL	ERROR	%ERROR
ZERO	0.00	0.00	0.00	-
1	300.00	301.00	1.0	0.33
AVERAGE (%)				0.08

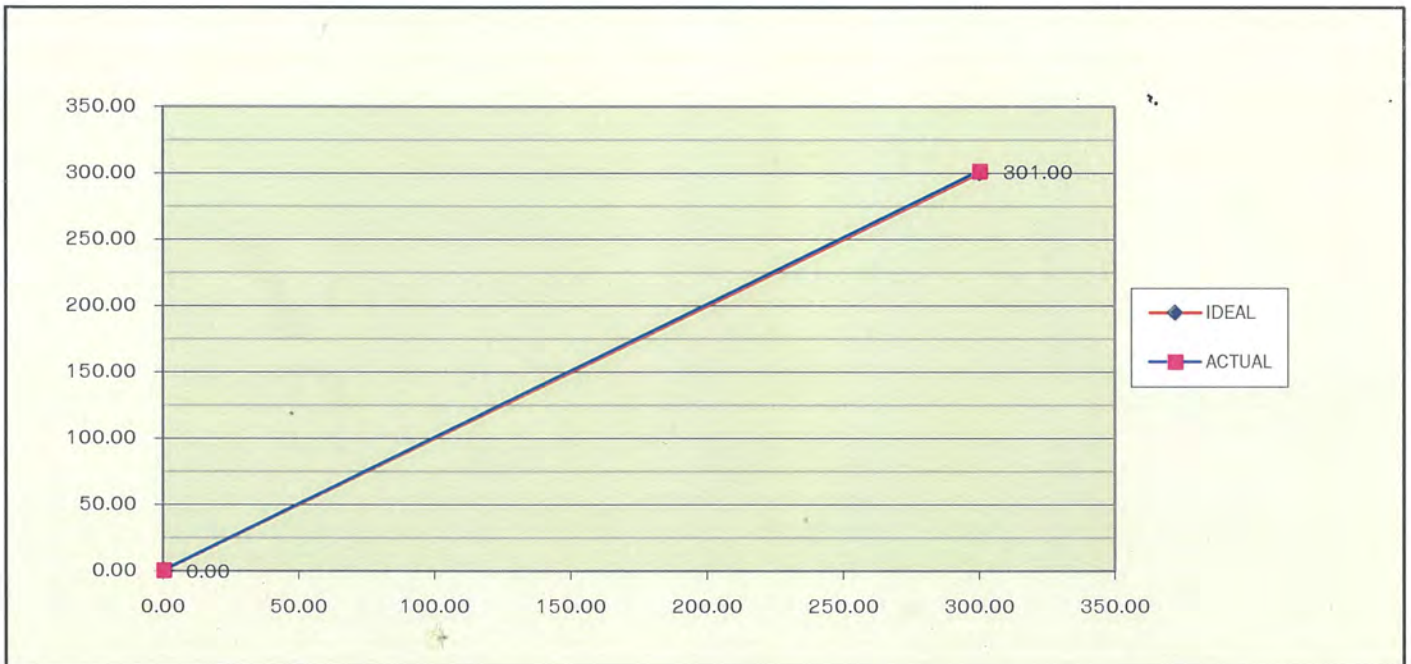

CALIBRATED BY :

DATE : 9/18/65

CHECKED BY :

DATE : 9/18/65



ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 31 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ถนนเพชรเกษม 7,7/1 แขวง วัดท่าพระ เขต บางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02868-1889


FLOW CALIBRATE

CUSTOMER NAME	:	ALS Laboratory Group (Thailand) Co., Ltd.		
EQRIPMENT NAME	:	Flow Calibrator		
MANUFACTURER	:	Bios	MODEL : 510 L	SERIAL NO : 129549

Flow Parameter	Step	Set	Display	Flow Meter
Sample	Before	40	38	15 cc/min
	After	40	40	39.7 cc/min
Air	Before	175	175	190 cc/min
	After	175	175	176 cc/min
Fuel	Before	35	32	36 cc/min
	After	35	35	35 cc/min

CALIBRATED BY :

CHECKED BY :

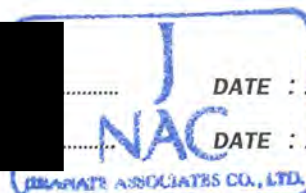

DATE :

DATE :

9/8/65

9/8/65

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ถนน เพชรเกษม7,7/1 แขวง วัดท่าพระ เขต บางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02868-1889



บริษัท เอกเสคคิวทิฟ เทคดิง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230
TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

ที่ RA 202/23

ใบรายงานผลการปรับเทียบ

ชื่อผู้ขอรับบริการ : บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด.
ที่อยู่ : 104 ซ.พัฒนาการ 40 ถ.พัฒนาการ แขวงสวนหลวง เขตสวนหลวง กรุงเทพมหานคร 10250.
ปรับเทียบที่ : บริษัท เอกเสคคิวทิฟ เทคดิง จำกัด
ที่อยู่ : 48/194-5 ซอย ประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวง/เขตลาดพร้าว กรุงเทพฯ 10230

รายละเอียดเครื่องมือที่ทำการปรับเทียบ :

เครื่องมือ : เครื่องตรวจวัดไอระเหยจากสารเคมี
ผลิตภัณฑ์ : RAE Systems
รุ่น : MiniRAE3000
หมายเลขเครื่อง : 592-906502
ID : BKK_FS0820

สภาวะแวดล้อม :

อุณหภูมิ : $(25 \pm 3) ^\circ\text{C}$
ความชื้นสัมพัทธ์ : $(34 \pm 15) \%$
ความดันบรรยากาศ : 760 มิลลิเมตรปรอท



วันที่ปรับเทียบมาตรฐาน : 8 กันยายน 2566

วิธีการปรับเทียบมาตรฐาน : ปรับเทียบโดยใช้ Standard Reference Gas
- Isobutylene Standard Gas 100 ppm; Lot number: 302-402431506.

ผลการปรับเทียบมาตรฐาน

Sensor Type	Reference Concentration	Before Cal.	After Cal.	Error Reading	Result
PID	0.0 ppm (Air Zero)	0.0 ppm	0.0 ppm	0.0 ppm	Pass
PID	100 ppm (Isobutylene)	105.2 ppm	100.0 ppm	0.0 ppm	Pass

Flow Rate of Pump : 475 cc/min.

Accuracy : $\pm 3 \%$ at calibration point

ผู้ปรับเทียบ



Service Engineer

ผู้ตรวจสอบ :



(นายสุทธร วงศ์ทองสงข)

Service Engineer Manager

ผลการสอบเทียบ/ปรับเทียบ นี้ รับรองเฉพาะตัวอย่างและรายการที่ได้ระบุไว้เท่านั้น

การนำรายงานผล/ใบรับรองนี้ไปโฆษณาและการคัดลอกหรือการนำผลบางส่วนไปเผยแพร่ต่อสาธารณะต้องได้รับอนุญาตเป็นลายลักษณ์อักษรจากทางบริษัทฯ



บริษัท เอกเสคคิวทิฟ เทรตติ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230
TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

No. RA 202/23

Certificate of Calibration

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
Address : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang Bangkok 10250 TH.
Calibration location : Executive Trading Limited.
Address : 48/194-5 Soi Praditmanutham 19, Pradit Manutham Road, Latphrao, Bangkok 10230

Tools :
Instrument : Gas Detector
Product : RAE Systems
Model Name : MiniRAE3000
Serial Number : 592-906502
ID : BKK_FS0820

Environmental Condition:
Temperature : $(25 \pm 3) ^\circ\text{C}$
Relative Humidity : $(34 \pm 15) \%$
Pressure : 760 mmHg

Date of Calibration : September 8, 2023
Calibration Method : This instrument has been calibrated using calibration gases. Test and calibration data is On file with Executive trading limited.
Reference Standard : Isobutylene Standard Gas 100 ppm; Lot number: 302-402431506.


Test Result

Sensor Type	Reference Concentration	Before Cal.	After Cal.	Error Reading	Result
PID	0.0 ppm (Air Zero)	0.0 ppm	0.0 ppm	0.0 ppm	Pass
PID	100 ppm (Isobutylene)	105.2 ppm	100.0 ppm	0.0 ppm	Pass

Flow Rate of Pump : 475 cc/min.

Accuracy : $\pm 3 \%$ at calibration point


Calibrated By

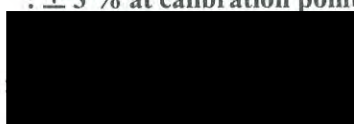

(Mr. Surinthorn Sainate)

Service Engineer

Approved By :

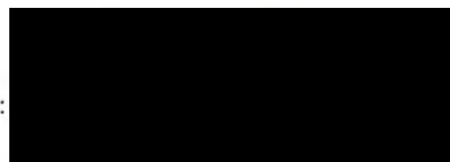

(Mr. Sudwong Kongsongsaeng)

Service Engineer Manager

The results relate only to the items tested or calibrated.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the company.



บริษัท เอกเสคคิวทิฟ เทรตติ้ง จำกัด (สำนักงานใหญ่)

48/194-5 ซอยประดิษฐ์มนูธรรม 19 ถนนประดิษฐ์มนูธรรม แขวงลาดพร้าว เขตลาดพร้าว กรุงเทพฯ 10230
TEL. (662) 515-0145-50 FAX. (662) 515-0144 www.etlthai.com E-mail : info@etlthai.com

ที่ RA 202/23

ใบรายงานการตรวจเช็คเครื่องตรวจวัดก๊าซ รุ่น MiniRAE3000


หมายเลขเครื่อง : 592-906502

วันที่ตรวจเช็ค : 8 กันยายน 2566

ลำดับที่	รายละเอียด การตรวจสอบ	RAW COUNT		สรุป	หมายเหตุ
		REF.	REAL		
1.	PID RAW COUNT				
	Ch.H	10000-62500	55778	■ YES □ NO	
	Ch.L	<62500	55938	■ YES □ NO	
2.	Lamp	>40	41	■ YES □ NO	

ลำดับที่	รายละเอียด การตรวจซ่อม	การแก้ไข	สรุป	หมายเหตุ
1.	Motor Pump	Check flow rate	■ YES □ NO	475 cc/min.
2.	Buzzer	-	■ YES □ NO	-
3.	Li-ion Battery	-	■ YES □ NO	-
4.	Key Pad			
	Y/+	-	■ YES □ NO	-
	N/-	-	■ YES □ NO	-
	MODE	-	■ YES □ NO	-
5.	LCD Display	-	■ YES □ NO	-
6.	THP sensor	-	■ YES □ NO	-
7.	Light Sensor	-	■ YES □ NO	-
8.	Pocket Clip	-	□ YES □ NO	-
9.	PC Port	-	■ YES □ NO	-
10.	Slim Rubber Boot	-	■ YES □ NO	-

ผู้ตรวจเช็ค

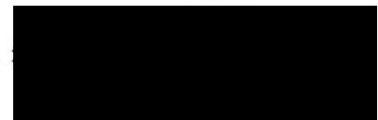

Service Engineer

ผลการสอบเทียบ/ปรับเทียบ นี้ รับรองเฉพาะตัวอย่างและรายการที่ได้ระบุไว้เท่านั้น

การนำรายงานผล/ใบรับรองนี้ไปโฆษณาและการคัดลอกหรือการนำผลบางส่วนไปเผยแพร่ต่อสาธารณะต้องได้รับอนุญาตเป็นลายลักษณ์อักษรจากทางบริษัทฯ



CALGAZ,
A DIVISION OF AIRGAS USA LLC

821 Chesapeake Drive,
Cambridge, MD 21613
USA Tel. 1-800-638-1197
www.calgaz.com

CERTIFICATE OF ANALYSIS

Date: 06/06/2022
Order Number: 1110821892
Lot Number: 302-402431506

Customer: EXECUTIVE TRADING LIMITED
Part Number: 600-0002-000
Use Before: JUN 6, 2027

Component	Concentration (\pm 2%)
ISOBUTYLENE	100PPM
AIR	Balance

Cylinder Size: 1.2 Cu. Ft.
Contents: 34 Liter

Valve: CGA600
Pressure: 494 PSIG

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

Analyst:

Chris Donnelly

CERTIFICATE of Attendance

It is hereby certified that

Mr Surinthorn Sainate
(Executive Trading Limited)


has successfully completed the

RAE Service Training Course


Conducted by

HONEYWELL

on **2nd August 2022**



Conducted by : Desmond Tan
Service Engineer / Technical Trainer
Date of Issue : 2nd August 2022
Certificate valid for 2 years from date of issue

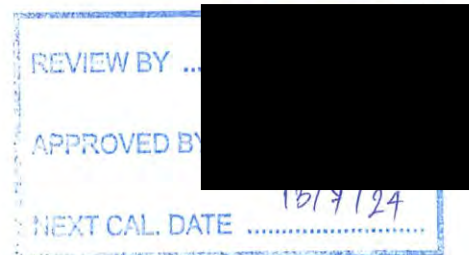

Certificate Number
CL-008-66

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM	: Wind Direction Sensor
MANUFACTURER	: Novalynx
MODEL/TYPE	: Sensor: WS-02F Data logger: 110-WS-25DL-D
SERIAL NUMBER	: Sensor: WSD-013 Data logger: A5792
ID NUMBER	: SGK_FS0089
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (Thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE	: 10 Jan 2023
MEASUREMENT DATE	: 13 Jan 2023
ISSUE DATE	: 13 Jan 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION	: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.
----------------------	---

CALIBRATION CONDITION	: Wind tunnel cross-section area ¹	900	cm ²
	Win direction frontal area ²	129	cm ²
	Diameter of mounting pipe ³	-	mm
	Blockage ratio of test object ⁴	0.143	[-]

Preconditioning	: 24 hours at ambient conditions.
Measurement Condition	: The average values during measurement are (23.8)°C, (51.1) %RH and (1010.8) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory:

.....roen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D^{std} Degree (°)	D^{uuc} Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
4.99	0.000	0	0	0.58
	45.000	42	-3	0.68
	90.000	88	-3	0.76
	135.000	134	-2	0.76
	180.000	181	1	0.68
	225.000	227	2	0.74
	270.000	273	3	0.68
	315.000	318	3	0.68

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration



End of Certificate of Calibration

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD-013
Data logger: A5792
ID NUMBER : SGK_FS0089
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) co., ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 10 Jan 2023
MEASUREMENT DATE : 13 Jan 2023
ISSUE DATE : 13 Jan 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS	: Wind tunnel cross-section area ¹	900	cm ²
	Win direction frontal area ²	100	cm ²
	Diameter of mounting pipe ³	-	mm
	Blockage ratio of test object ⁴	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.5) °C, (43.8) %RH and (1015.3) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

Calibration procedure:

The cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0052-21 and MW-0066-22

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

MEASUREMENT RESULTS ⁵

The cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle, UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

v_{std} ⁶ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{uuc} ⁷ (m/s)	Error (m/s)	U ($k=2$) (m/s)
0.981	23.56	23.50	0.8	-0.2	0.15
2.027	23.44	23.50	1.8	-0.2	0.16
3.049	23.50	23.50	2.9	-0.2	0.21
4.125	23.54	23.50	3.9	-0.2	0.20
5.00	23.50	23.50	4.9	-0.1	0.20
5.98	23.62	23.50	5.9	-0.1	0.17
7.05	23.32	23.50	6.9	-0.1	0.18
8.16	23.60	23.50	8.0	-0.1	0.21
9.09	23.40	23.50	9.1	0.0	0.22
10.10	23.50	23.50	10.0	-0.1	0.24
11.15	23.36	23.50	11.1	-0.1	0.23
12.14	23.46	23.50	12.1	0.0	0.23
13.19	23.40	23.50	13.2	0.0	0.26
14.25	23.40	23.50	14.2	0.0	0.24
15.24	23.34	23.50	15.1	-0.1	0.25
16.29	23.30	23.50	16.2	-0.1	0.33

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No.: WD-02072022

Page 1 of 2 pages

Measurement Item : Wind direction sensor with data logger.

Manufacturer : Data logger: Novalynx.
: Wind direction sensor: Novalynx.

Model/Type : Data logger: 200-WS-25LB
: Wind direction sensor: WS-02F

Serial Number : Data logger: A5192
: Wind direction sensor: -

ID No : Data logger: SGK_FS0035
: Wind direction sensor: -

Customer : ALS laboratory group (Thailand) co., ltd.
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250
Thailand.

Environmental Condition:

The measurement was carried out in an ambient temperature of $(23 \pm 3) ^\circ\text{C}$, and relative humidity of $(40 \pm 10) \%$.

Measurement Method:

The wind direction sensor calibration according to comparison method with reference angle measurement electronic theodolite and line laser is used for axis control. The measurement were taken at 45° intervals in clockwise and counterclockwise directions.

Note: The UUC was warmed up for 1 hour prior to the calibration being performed

Traceability:

The measurement results are traceable to the international system of units (SI) through Certificate No.: Q21086014, Certificate No.: KWS64/0025.

Measurement Date : Jul 13, 2022.

Issued Date : Jul 14, 2022.

Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittrapor Lertsomphol



Approved Signatory:.....

Mr. Pannya Booncharoen.
Calibration Department Manager

Continuation of Certificate of Calibration Number

Certificate No: WD-02072022

Pages 2 of 2 pages

Result of calibration: ☐ Without adjustment ☒ With adjustment.

Calibration in the range of 0 – 360 ° at a calibration interval of 45°.

The results of calibration and associated measurement uncertainties are reported in table below.

NO	Turning Direction	Nominal Angle (°)	Standard Reading (°)	UUC* Reading (°)	Error (°)	Uncertainty ±(°)
1	Clockwise	0/360	360	359	-1	3.0
2		45	45	43	-2	3.0
3		90	90	87	-3	3.0
4		135	135	133	-2	3.0
5		180	180	180	0	3.0
6		225	225	228	3	3.0
7		270	270	274	4	3.0
8		315	315	320	5	3.0
9	Counter Clockwise	0/360	360	359	-1	3.0
10		45	45	43	-2	3.0
11		90	90	87	-3	3.0
12		135	135	133	-2	3.0
13		180	180	180	0	3.0
14		225	225	228	3	3.0
15		270	270	274	4	3.0
16		315	315	320	5	3.0

UUC*: Unit Under Calibration The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No: WS-02072022

Page 1 of 2 pages

Measurement Item : Cup anemometer with data logger.

Manufacturer : Data logger: Novalynx
: Cup anemometer: Novalynx

Model/Type : Data logger: 200-WS-25LB
: Cup anemometer: WS-02F

Serial Number : Data logger: A5193
: Cup anemometer: -

ID No : Data logger: SGK_FS0035
: Cup anemometer: -

Customer : ALS laboratory group (Thailand) co., ltd.
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

Test Conditions : Wind tunnel cross test section area 900 cm²
: Anemometer frontal area 100 cm²
: Diameter of mounting pipe - mm
: Blockage ratio of test object 0.111 [-]

Test Conditions : Air temperature 24.0 ±0.8 °C
: Air pressure 1005.3 ±0.4 hPa
: Relative air humidity 45.1 ±3.5 %RH

Calibration Procedure Calibration was carried out base on;
IEC 61400-12-1 ED.1: 2005-Power Performance Measurements of Electricity Producing Wind Turbines;
MEASNET Anemometer Calibration Procedure – Version 2: 2009;

Traceability This calibration documents the traceable to national standard, Which realize the unit of measurements according to the international system of units (SI) through National Institute of Metrology Thailand (NIMT).

Measurement Date : Jul 13, 2022.

Issued Date : Jul 14, 2022.

Calibrated by

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved Signatory:

Calibration Department Manager

Continuation of Certificate of Calibration Number

Certificate No: WS-02072022

Page 2 of 2 Pages

Result of calibration: ☒ Without adjustment ☐ With adjustment

Calibration in the range of 1 – 16 m/s at a calibration interval of 1 m/s.

The results of calibration and associated measurement uncertainties are reported in the table below.

V _{STD} Reading m/s	V _{UUC} * Reading m/s	Error (m/s)	Uncertainty (%)
2.063	2.0	-0.1	2.4
4.115	4.1	0.0	1.1
5.97	6.1	0.1	0.97
7.99	8.0	0.0	0.79
9.99	10.2	0.2	0.69
12.03	12.3	0.3	0.63
14.02	14.3	0.3	0.58
15.98	16.4	0.4	0.48
14.99	15.3	0.3	0.57
13.01	13.3	0.3	0.52
10.97	11.1	0.1	0.52
8.98	9.0	0.0	0.74
6.99	7.0	0.0	0.81
5.121	5.1	0.0	0.86
3.000	3.0	0.0	1.7
1.040	0.9	-0.1	4.5

UUC*: Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

Appendix 1: Instrumentations

NO	Sensor	Manufacturer	Model/Type	Calibration Date	Certificate Report Number	Range
1	Pitot static	TESTO INC.	06352145	Aug 07, 2021	MW-0034-21	5 – 30 m/s
2	Precision Differential Pressure Meter	Zoglab	DPM2500	Aug 07, 2021	MW-0034-21	5 – 30 m/s
3	Air velocity transducer (hot wire)	TSI INC.	8455-12	Aug 08, 2021	MW-0035-21	0 - 5 m/s
4	Temperature	Zoglab	DSR-THP	March 30, 2022	CL-027-65	-30 - 70°C
5	Relative humidity	Zoglab	DSR-THP	March 30, 2022	RH-03032022	0 - 100 %RH
6	Atmospheric pressure	Zoglab	DSR-THP	March 30, 2022	BP-01032022	500 - 1100 hPa
7	Wind tunnel	ESSOM	MP330D	-	-	0 - 50 Hz

End of certificate of calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

REVIEW BY
APPROVED BY
NEXT CAL D

Certificate Number

CL-007-66

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD-012
Data logger: A5791
ID NUMBER : SGK_FS0088
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) co., ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 10 Jan 2023
MEASUREMENT DATE : 13 Jan 2023
ISSUE DATE : 13 Jan 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS : Wind tunnel cross-section area¹ 900 cm²
Win direction frontal area² 100 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.111 [-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.4) °C, (46.3) %RH and (1011.3) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory:

Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

Calibration procedure:

The cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0052-21 and MW-0066-22

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

MEASUREMENT RESULTS⁵

The cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle, UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

v_{std}^6 (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{uuc}^7 (m/s)	Error (m/s)	$U (k=2)$ (m/s)
0.981	23.64	23.35	0.8	-0.2	0.15
2.041	23.10	23.35	1.8	-0.2	0.16
3.049	23.68	23.35	2.8	-0.2	0.18
4.138	23.12	23.35	3.8	-0.3	0.20
5.00	23.72	23.35	4.8	-0.2	0.19
5.98	23.16	23.35	5.8	-0.2	0.19
7.04	23.66	23.35	6.8	-0.2	0.18
8.16	23.18	23.35	7.8	-0.3	0.18
9.09	23.52	23.35	8.8	-0.3	0.20
10.07	23.42	23.35	9.8	-0.3	0.23
11.15	23.50	23.35	10.8	-0.3	0.22
12.13	23.50	23.35	11.8	-0.3	0.22
13.20	23.58	23.35	12.8	-0.4	0.22
14.26	23.50	23.35	13.9	-0.4	0.22
15.23	23.60	23.35	14.8	-0.4	0.22
16.30	23.52	23.35	15.9	-0.4	0.26

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP

Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

Certificate Number

CL-007-66

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD-012
Data logger: A5791
ID NUMBER : SGK_FS0088
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 10 Jan 2023
MEASUREMENT DATE : 13 Jan 2023
ISSUE DATE : 13 Jan 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION : Wind tunnel cross-section area¹ 900 cm²
Win direction frontal area² 129 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.143 [-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.7)°C, (46.8) %RH and (1011.8) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:



Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS ⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D^6_{std} Degree (°)	D^7_{uuc} Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.02	0.000	0	0	0.58
	45.000	42	-3	0.82
	90.000	90	0	0.74
	135.000	136	1	0.74
	180.000	182	1	0.76
	225.000	228	2	0.76
	270.000	273	3	0.74
	315.000	318	3	0.74

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration



End of Certificate of Calibration



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Pressure measurement laboratory
Calibration services department.



NSC - TISI - TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CL-004-66

Page 1 of 2 Pages

MEASUREMENT ITEM : Digital barometer
MANUFACTURER : Novalynx
MODEL/TYPE : 110-WS-25BP
SERIAL NUMBER : A5791
ID NUMBER : SGK_FS0088
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.
RECEIVED DATE : 10 Jan 2023
MEASUREMENT DATE : 13 Jan 2023
ISSUE DATE : 13 Jan 2023

Calibration procedure:

The pressure calibration was done by In-house calibration method as WI-CL-003 according to comparison method with Digital pressure calibrator based on DKD-R 6-1

Traceability:

The measurement results are traceable to the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) which complies with the requirements of ISO/IEC17025:2017, ANSI/NCSL Z540-1 via Certificate number: MP-0205-22

The reported uncertainty is based on a standard uncertainty multiplied by a coverage $k=2$, providing a level of confidence of approximately 95%.

CONDITION OF THIS RESULT OF CALIBRATION:

1. Reference Standard Instrument:

Instrument	Model	Serial No.	Certificate No.	Due Date
Absolute Pressure Transducer	CPG2500	4100126P	MP-0205-22	02 Dec 2023

1. Calibration effort for calibration sequence A

2. The UUC* was installed in vertical orientation above reference standard instrument and center of UUC* was used as the reference level.

3. Calibration conditions:

4. Condition : ☒ Normal ☐ Abnormal
Pressure transmitting medium : Air
 ρ_{Fl} (20°C, 1 bar) : 1.19 kg/m³
 H_{amb} : (55±15) %
 t_{amb} : (23±3) °C
 p_{amb} : (1010±10) mbar

5. The certificate is valid only to the item calibrated on date and place of calibration

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen

Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Pressure measurement laboratory
Calibration services department.



NSC - TISI - TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CL-004-66

Page 2 of 2 Pages

MEASUREMENT RESULTS : ☒ Without adjustment ☐ With adjustment

CALIBRATION IN THE RANGE OF : 950 – 1050 mbar

The results of calibration and associated measurement uncertainties are reported in the table below.

STD (mbar)	UUC* (mbar)	Error (mbar)	Uncertainty (k=2) (mbar)
950.13	951.0	0.9	1.1
970.10	970.7	0.6	0.79
990.10	990.5	0.4	0.64
1010.11	1010.3	0.2	0.42
1030.08	1030.0	-0.1	0.40
1050.10	1049.7	-0.4	0.60

Note: UUC* Unit Under Calibration

: To convert the result in report unit to Pa should be multiply by 100



SITHIPHORN ASSOCIATES CO.,LTD.

CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd., Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

Cert. No. : ACC22038

Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR
Manufacturer : RION
Model : NC-75
Serial No.: 35024429
ID No.: - SQK_FS 0114



Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 03 NOVEMBER 2022
Calibration Date : 14 NOVEMBER 2022
Date of Issue : 15 NOVEMBER 2022

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACC22038

Job No. : VC66AC0006

Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	33461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23
Audio Analyzer	AVR-3360A	V744B6069	EF-0010-22	07-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACC22038
Job No. : VC66AC0006
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit (dB)
94	93.94	-0.06	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Tolerance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Tolerance limit (%)
0.33	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

————— **End of Calibration Certificate** —————

SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL23105

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 00331094 / 22922 / 22569
ID No.: -

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 17 MARCH 2023
Calibration Date : 27-28 MARCH 2023
Date of Issue : 31 MARCH 2023

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL23105

Job No. : VC66AC0042

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL23105
Job No. : VC66AC0042
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

Continuation of Calibration Certificate

Cert. No. : ACL23105
Job No. : VC66AC0042
Pages : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	8.7
C - weight	14.5
Flat	20.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.3	± 1.0
1000	0.1	0.1	0.1	± 0.7
8000	-0.3	-0.3	-0.2	+ 1.5, - 2.5

Continuation of Calibration Certificate

Cert. No. : ACL23105
Job No. : VC66AC0042
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.1	0.0	±1.0
125	0.1	0.1	0.1	±1.0
250	0.1	0.1	0.0	±1.0
500	0.0	0.1	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

Continuation of Calibration Certificate

Cert. No. : ACL23105
Job No. : VC66AC0042
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	29.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8
28.0	27.9	-0.1	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.9	-0.1	±0.8

Continuation of Calibration Certificate

Cert. No. : ACL23105

Job No. : VC66AC0042

Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
One	136.4	136.2	-0.2	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.1	-0.3	±1.0
Negative half cycle	135.4	135.1	-0.3	±1.0

Continuation of Calibration Certificate

Cert. No. : ACL23105

Job No. : VC66AC0042

Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate



Agilent Technologies

Agilent Technologies (Thailand) Limited
U CHU LIANG BLDG. 22/F UNIT A,D
968 RAMA 4 ROAD, SILOM, BANGRAK
Bangkok 10500 Thailand

Tel. +662 637 6363
Fax: +662 632 4334
Email: ccc-smt@agilent.com
Website: www.agilent.com/chem

Customer Contact:

ALS Laboratory Group (Thailand) Co
Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan
TAX ID : 0105540004859
bounced-imchom.chanattagarn@alsglobal.com
227158760519

Invoice To:

ALS Laboratory Group (Thailand) Co
Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

Delivery Site:

ALS Laboratory Group (Thailand) Co
Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

Location:

Room
Bldg
Lab
Dept

SERVICE REPORT

Customer Purchase Order Number:	Customer Number: 70371013
Service Request:	Service Request Date:
Service Order: 6006068207	Service Confirmation: 6904837529

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	

Direct Inquiries to:

Contact Name: Customer Contact Center
Contact E-mail: ccc-smt@agilent.com
Contact Telephone: +662 637 6363
Contact Fax: +662 632 4334

products | applications | software | services

Learn more about Agilent's Special Offers, Products, Services and our full range of laboratory productivity solutions optimized for your applications and workflows. Visit us at www.agilent.com/chem

Agilent Technologies (Thailand) Limited, Head Office
U Chu Liang Bldg. 22/F Unit A,D
968 Rama 4 Road, Silom, Bangrak,
Bangkok 10500 Thailand
Tax ID : 0105542068218

Citibank N.A. Bangkok Branch
399 Interchange 21 Building, Sukhumvit Road, Klongtoey Nau
Sub-district, Wattana District, Bangkok 10110 Thailand
Acc. No: 012-4452-007 ,
THB:Krung Thai Bank PCL
Siam Square Br.,416/1-2 Rama I Rd.,Pathumwan, BKK 10330
Thailand

ORIGINAL

Service Confirmation Number: 6904837529

Service Confirmation Date: 06.04.2023

Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IM-7900	ICPMS 7900 System			
G8410A	SPS 4 Autosampler	AU15430722	ICP MS 7900	SYS-IM-7900
G8411A	ISIS 3 for Agilent 7850/7900/8900	JP15510227	ICP MS 7900	SYS-IM-7900
G3292A	PSC 6106T Chiller	2U15A1948	ICP MS 7900	SYS-IM-7900
G8403A	Agilent 7900 ICP-MS	JP15471169	ICP MS 7900	SYS-IM-7900

Service Items:

Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EOQ	Enterprise Operational Qualification	1.00	Agreement Entitlement - 100 % covered	06.04.2023	06.04.2023
1010	5185-5850	ICP-MS Checkout Solutions	1.00	Agreement Entitlement - 100 % covered		

Additional Information:

Service Confirmation Number: 6904837529

Service Confirmation Date: 06.04.2023

Service Information:

Problem Description:

WU-S-OQ-ICP MS 7900-5001143313

Service Provided:

Test OQ control of instrument ICPMS = BKK_EL0043. After done all instrument test all Pass.

Service Overview Code:

Reason Code: Scheduled Service

Diagnosis Code: Scheduled Service

Resolution Code: Scheduled Service

Reported Hours:

6.0

Travel Hours:

1.0


Customer Field Service

Representative Name:

Panthep Kurasathain

Customer Field Service

Representative Signature:



Date:

06 Apr 2023

Customer Name:

Anchalee Khamjan

e:

Date:

06 Apr 2023

Additional Comments:



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 1 of 6

Certificate of Calibration

Equipment : HEATING BLOCK

Manufacturer : Environmental Express

Model : SC 196

Serial No. : 6974CECW3285

Customer Code : BKK_EL0054

ID No. : T5306A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250


Customer Location : Acid Digestion Lab

Date of Receipt : 13 September 2023

Calibrated By : Sanee Musikawan (Site Calibration Manager)

Approved By :  / Sujjar Naknakred (Site Calibration Manager)

Date of Issue : 26 SEP 2023

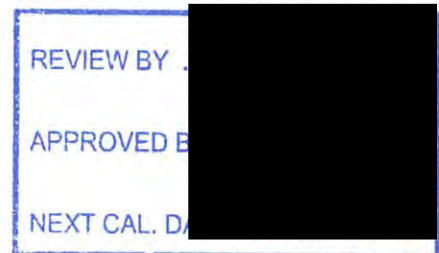

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T231676

Page 2 of 6

Calibration Report

Equipment : HEATING BLOCK
Date of Calibration : 22 September 2023
Environment : Temperature : 21.8-23.1 °C
Line Voltage : 221.6-226.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 20 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN21-TN30	T230014	17 January 2024
TC	TYPE T	TN31-TN40	T230014	17 January 2024
DATA LOGGER	34970A	T151	T230014	17 January 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 2 Hour 20 Minute At 95 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

() without adjustment

(X) after adjustment

Approved By





Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109


Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 3 of 6

Calibration Report

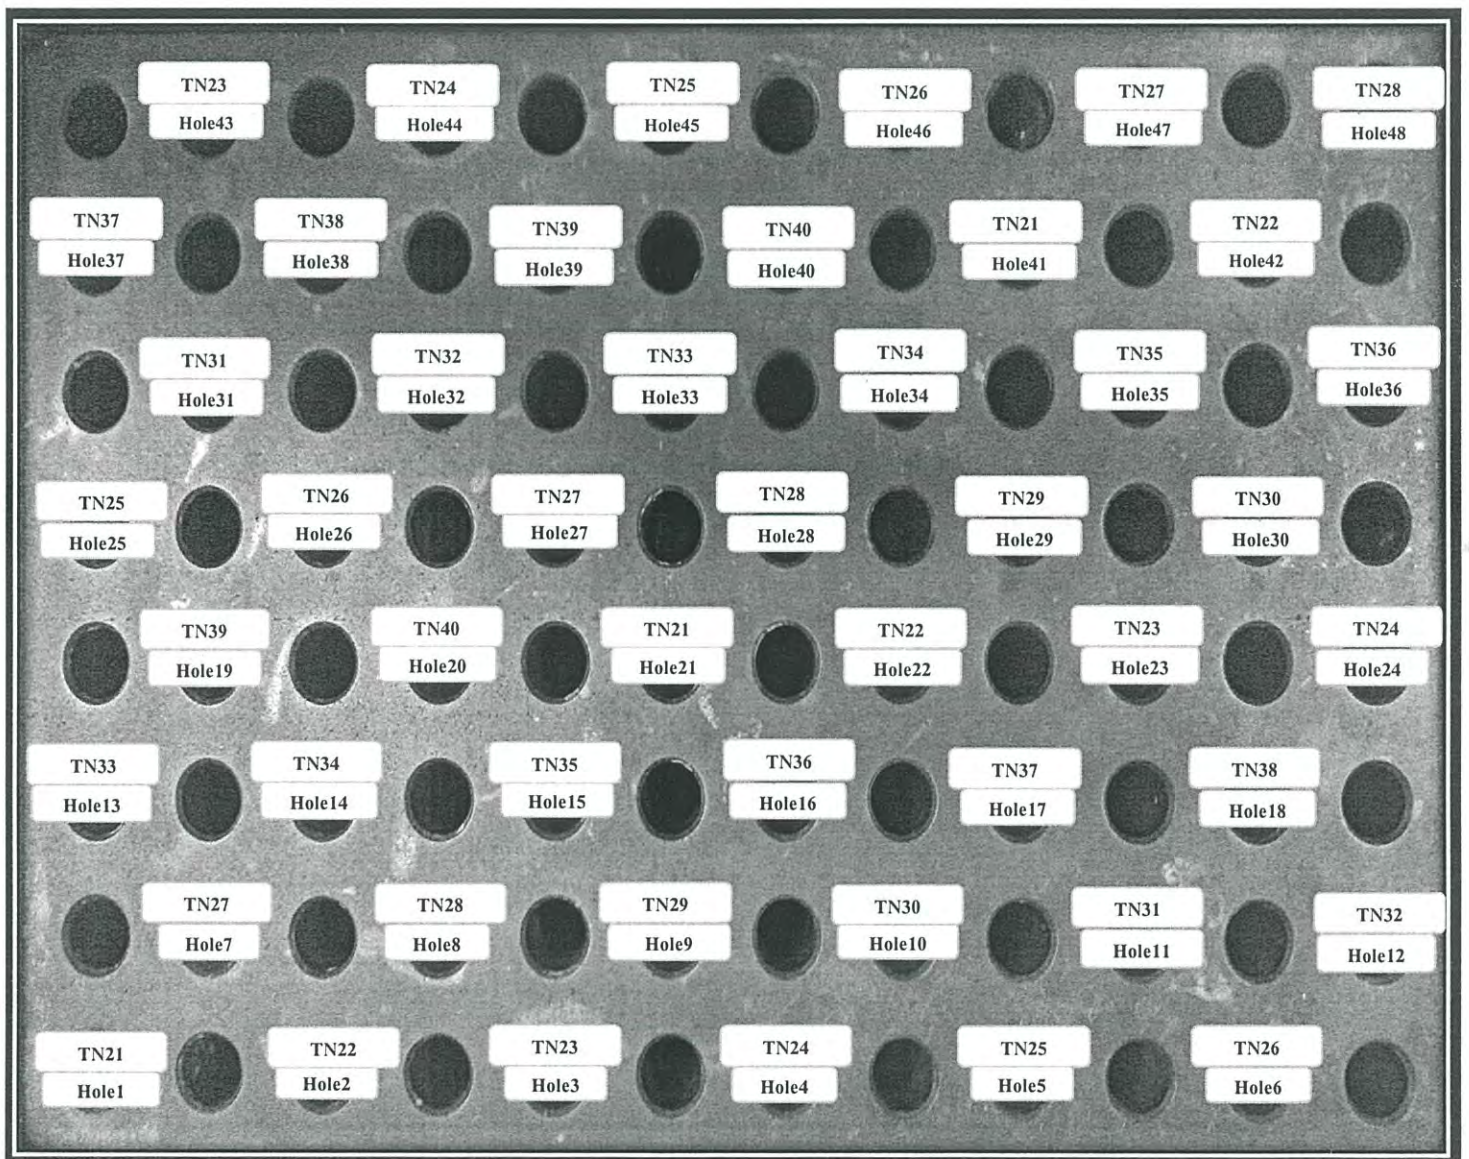

FRONT CONTROL

Approved By. _____



Certificate No T231676

Page 4 of 6

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (° C)					
R1 Hole1-Hole6		TN21	TN22	TN23	TN24	TN25	TN26
CAL POINT	Max	95.01	94.41	95.20	95.41	94.51	95.17
95	Min	94.57	93.95	94.75	94.92	94.00	94.72
	Average	94.79	94.18	94.98	95.17	94.26	94.95
R2 Hole7-Hole12		TN27	TN28	TN29	TN30	TN31	TN32
	Max	95.36	95.43	95.19	95.16	95.35	94.97
	Min	94.94	94.95	94.72	94.71	94.90	94.57
	Average	95.15	95.19	94.96	94.94	95.13	94.77
R3 Hole13-Hole18		TN33	TN34	TN35	TN36	TN37	TN38
	Max	95.37	95.50	95.22	95.21	95.33	95.31
	Min	94.99	95.09	94.78	94.82	94.88	94.96
	Average	95.18	95.30	95.00	95.02	95.11	95.13
R4 Hole19-Hole24		TN39	TN40	TN21	TN22	TN23	TN24
	Max	95.59	94.42	94.52	94.24	94.63	94.67
	Min	95.21	94.06	94.13	93.88	94.28	94.27
	Average	95.40	94.24	94.33	94.06	94.45	94.47
R5 Hole25-Hole30		TN25	TN26	TN27	TN28	TN29	TN30
	Max	95.19	95.38	92.93	95.30	95.14	95.03
	Min	94.83	95.03	92.56	94.95	94.79	94.70
	Average	95.01	95.20	92.75	95.12	94.96	94.87
R6 Hole31-Hole36		TN31	TN32	TN33	TN34	TN35	TN36
	Max	94.63	94.90	94.77	94.31	94.24	93.87
	Min	94.24	94.55	94.44	93.98	93.92	93.56
	Average	94.43	94.72	94.60	94.14	94.08	93.71
R7 Hole37-Hole42		TN37	TN38	TN39	TN40	TN21	TN22
	Max	94.30	94.44	94.04	93.81	94.89	95.35
	Min	93.95	94.05	93.67	93.48	94.39	94.90
	Average	94.13	94.24	93.86	93.65	94.64	95.12
R8 Hole43-Hole48		TN23	TN24	TN25	TN26	TN27	TN28
	Max	95.99	95.63	95.28	95.29	95.45	94.87
	Min	95.57	95.15	94.82	94.84	94.99	94.48
	Average	95.78	95.39	95.05	95.07	95.22	94.68

Approved By. _____

Certificate No T231676

Page 5 of 6

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (° C)					
R1 Hole1-Hole6		TN21	TN22	TN23	TN24	TN25	TN26
CAL POINT	Max	105.23	104.32	105.43	105.25	104.44	105.27
105	Min	104.94	103.95	105.15	105.04	104.11	104.96
	Average	105.09	104.13	105.29	105.15	104.28	105.12
R2 Hole7-Hole12		TN27	TN28	TN29	TN30	TN31	TN32
	Max	105.30	105.12	105.18	105.22	105.12	105.16
	Min	105.11	104.92	104.96	105.00	104.92	104.97
	Average	105.20	105.02	105.07	105.11	105.02	105.06
R3 Hole13-Hole18		TN33	TN34	TN35	TN36	TN37	TN38
	Max	105.37	105.63	105.02	104.80	104.69	105.19
	Min	105.17	105.37	104.75	104.59	104.50	105.00
	Average	105.27	105.50	104.88	104.69	104.60	105.09
R4 Hole19-Hole24		TN39	TN40	TN21	TN22	TN23	TN24
	Max	105.31	104.43	106.41	104.71	105.63	105.82
	Min	105.08	104.22	106.15	104.41	105.37	105.56
	Average	105.19	104.33	106.28	104.56	105.50	105.69
R5 Hole25-Hole30		TN25	TN26	TN27	TN28	TN29	TN30
	Max	104.95	106.26	103.34	105.78	105.59	105.87
	Min	104.67	105.96	103.08	105.56	105.36	105.68
	Average	104.81	106.11	103.21	105.67	105.48	105.77
R6 Hole31-Hole36		TN31	TN32	TN33	TN34	TN35	TN36
	Max	104.75	104.86	104.80	105.20	104.50	104.39
	Min	104.54	104.63	104.59	105.00	104.32	104.18
	Average	104.65	104.75	104.69	105.10	104.41	104.28
R7 Hole37-Hole42		TN37	TN38	TN39	TN40	TN21	TN22
	Max	104.30	104.90	104.85	104.65	104.88	104.85
	Min	104.09	104.72	104.66	104.49	104.63	104.52
	Average	104.19	104.81	104.75	104.57	104.76	104.68
R8 Hole43-Hole48		TN23	TN24	TN25	TN26	TN27	TN28
	Max	105.71	105.85	105.39	105.61	105.42	105.19
	Min	105.45	105.61	105.14	105.27	105.18	104.94
	Average	105.58	105.73	105.27	105.44	105.30	105.07

Approved By. _____



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 6 of 6

Calibration Report

Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (± °C)	Uncertainty (± °C)
	Min , Max	Average		
100.0	100.3 , 100.5	100.4	0.26	0.81
107.0	107.0 , 107.1	107.1	0.19	0.78

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th



Certificate No. T221644

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Cold Room)

Manufacturer : KOLDTECH

Model : KM 320

Serial No. : TBN-1012061/05

Customer Code : BKK_EN0167

ID No. : T2463A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250




Customer Location : Environmental Laboratory

Date of Receipt : 27 June 2022

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 04 JUL 2022

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T221644

Page 2 of 4

Calibration Report

Equipment : Chamber (Cold Room)
Date of Calibration : 30 June - 1 July 2022
Environment : Temperature : 18.9-23.7 °C
Line Voltage : 222.9-226.5 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T210009	30 July 2022
TC	TYPE T	TN171-TN180	T210009	30 July 2022
DATA LOGGER	34970A	T149	T210009	30 July 2022

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 3 Hour - Minute At 3 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

() without adjustment

(X) after adjustment


Approved By-



Certificate No. T221644

Page 3 of 4

Calibration Report

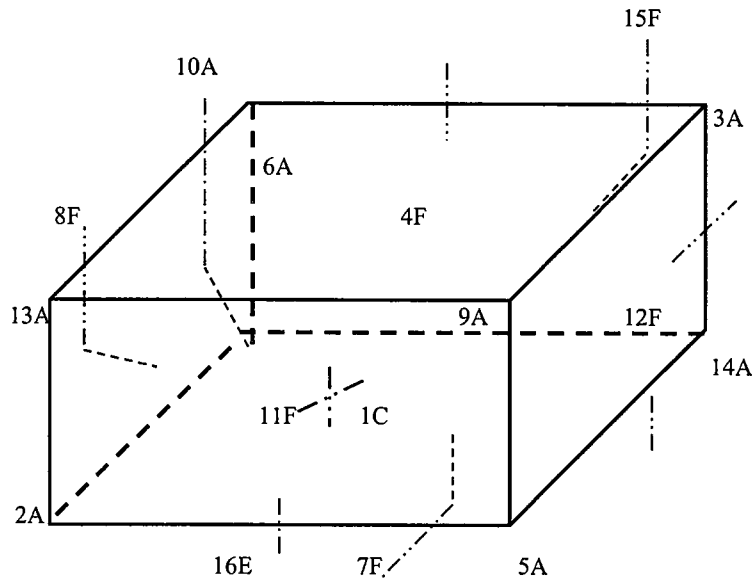

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN161
2A	=	TN162
3A	=	TN163
4F	=	TN164
5A	=	TN165
6A	=	TN166
7F	=	TN167
8F	=	TN168
9A	=	TN169
10A	=	TN170

11F	=	TN171
12F	=	TN172
13A	=	TN173
14A	=	TN174
15F	=	TN175
16E	=	TN176

Approved By _____

Certificate No. T221644

Page 4 of 4

Calibration Report

Measurement Results:

Average Standard Reading at each position (°C)										
Calibration Point	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170
3	2.71	2.82	2.75	2.89	2.95	3.68	3.02	2.96	3.03	2.85
	TN171	TN172	TN173	TN174	TN175	TN176				
	2.97	3.02	2.89	3.04	2.97	3.33				

Chamber (Cold Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage
	Min , Max	Average					Factor <i>k</i>
3.0	2.9 , 4.0	3.2	2.99	1.05	1.30	1.66	2.00

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By _____



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250


TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 22TW178

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5100
Serial No. :	15L103204
ID No. :	BKK_EN0205
Received Date :	02 August 2022
Test Date :	03 August 2022
Reference :	2208-0060DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	<div style="text-align: center;"> _____ Approved Signatory</div>
(✓) Malee Butkruea () Saithip Meangmai () Warakorn Lerngagtrakul	
Issue Date :	4 August 2022

REVIEW BY ...	
APPROVED BY	
NEXT CAL. DATE	



Cert.No.: 22TW178

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	21MM430	21 Sep 2022

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**

Dissolved Oxygen Probe No.: 17A100064

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.06	8.07	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Maler .

a 1119718



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22LM107

Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5100

Serial No. : 15L103204

ID No. : BKK_EN0205

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 2 August 2022

Calibrated Date : 4 August 2022


Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Man Pattanapongpaiboon

Approved by :


Approved Signatory

() Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date : 9 August 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0044131



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2208-0060DSC-2

Cert. No.: 22LM107

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1502A	A52847	21I1144	20 Oct 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 18C100772

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.002	19.93	-0.072	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th

E-Mail : calibrate@scg.com



Certificate No. T231342

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Incubator)

Manufacturer : MEMMERT

Model : ICP 750

Serial No. : F818.0033

Customer Code : BKK_EN0272

ID No. : T8041A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab 2

Date of Receipt : 3 July 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By : [Redacted] / Boonchai Suriyawong (Assistant Calibration Manager)

Date of Issue : 11 JUL 2023



The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T231342

Page 2 of 4

Calibration Report

Equipment : Chamber (Incubator)
Date of Calibration : 5-6 July 2023 (Finished Time 4:30 PM)
Environment : Temperature 26.9-30.3 °C
Line Voltage 221.7-225.5 V

Condition of this results of test. :

1. This instrument was calibrated by insert 12 standard resistance thermometer into its chamber and test according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986.)

All data show below were final values and the initial data may be obtained upon request.

The temperature scale used was based on ITS - 90.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	27-(CH1-10)	T230543	10 April 2024
RTD	100 ohm	28-(CH1-10)	T230543	10 April 2024
DATA LOGGER	34970A	T149	T230543	10 April 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

UUC Description :

Time Constant 6 Hour 35 Minute At 20 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Result of test :

() without adjustment


(X) after adjustment

Approved By _____

Certificate No T231342

Calibration Report

Page 3 of 4

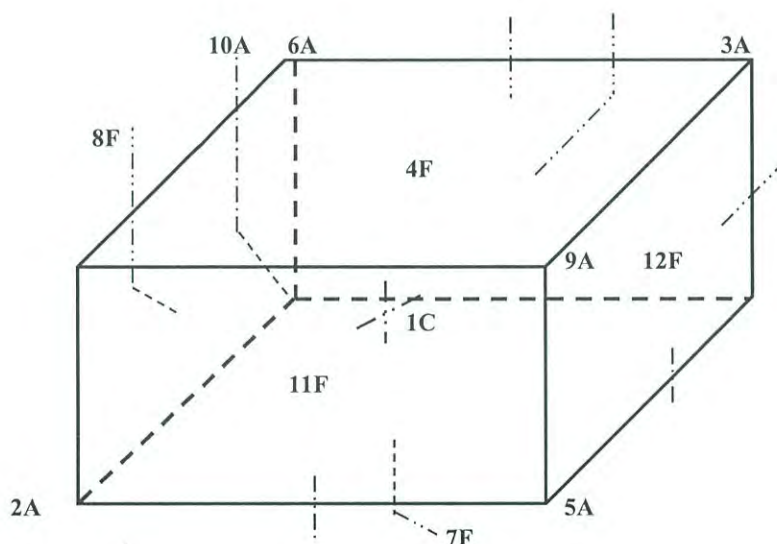

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	27-CH1
2A	=	27-CH2
3A	=	27-CH3
4F	=	27-CH4
5A	=	27-CH5
6A	=	27-CH6
7F	=	27-CH7
8F	=	27-CH8
9A	=	27-CH9
10A	=	27-CH10

11F	=	28-CH1
12F	=	28-CH2

Approved By. [REDACTED]

Certificate No. T231342

Calibration Report

Page 4 of 4

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)									
	27-CH1	27-CH2	27-CH3	27-CH4	27-CH5	27-CH6	27-CH7	27-CH8	27-CH9	27-CH10
20.0	19.82	19.80	20.32	19.78	19.77	19.65	20.11	19.69	19.78	20.18
	28-CH1	28-CH2								
	20.02	19.81								

Chamber (Incubator)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (\pm °C)	Uniformity (°C)	Uncertainty (\pm °C)	Coverage
	Min , Max	Average					Factor k
20.0	19.9 , 20.1	20.0	19.98	0.06	0.61	0.38	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CG3154

Page.: 1 of 2

Certificate of Calibration

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	BKK_EN0171
Manufacturer :	Witeg
Made in :	Germany
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd. Khwaeng Phatthanakan, Khet Suan Luang Bangkok 10250 Thailand
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	759 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Panward Pramklam

REVIEW BY	S
APPROVED BY ...	4
NEXT CAL. DATE	6

Approved by :



Approved Signatory

- () Pornthippa Tameyakul
() Malee Butkruea
(✓) Ponpan Paipim
() Srisuda Khamtha

Issue Date :

31 August 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0044607



Equipment : Burette
Received Date : 26 August 2022
Condition As-Received : Used Item
Calibration Date : 30 August 2022
Reference : 2208-0918DSC-2

Cert.No.: 22CG3154

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID. No.</u>	<u>Certificate No.</u>	<u>Traceability</u>	<u>Due date</u>
1) Balance	AE200S	N03679	140RC001	21MM429	NIMT	22 Sep 2022
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	22H1243	NIST,NIMT	09 June 2023
3) Thermometer	-	1594592	140EC010	22I181	NIMT	10 Feb 2023

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 °C


Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	k Factor
50	49.9959	0.010	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



a 1123908

Certificate No. T230760


Page 1 of 5

Certificate of Calibration

Equipment : HOT BLOCK**Manufacturer** : Environmental Express**Model** : B3000- 240**Serial No.** : 2017CODW116**Customer Code** : BKK_EN0222**ID No.** : T6769A4**Customer** : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

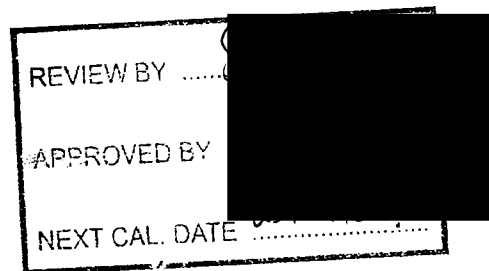Customer Location : Wet Chemistry Lab2**Date of Receipt** : 21 April 2023**Calibrated By** : Watcharasak Puttarat (Technician)**Approved By** :  / Sujjar Naknakred (Site Calibration Manager)**Date of Issue** : 12 MAY 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T230760

Page 2 of 5

Calibration Report

Equipment : HOT BLOCK
Date of Calibration : 25 April 2023
Environment : Temperature : 22.9-24.4 °C
Line Voltage : 222.7-227.8 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 20 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN121-TN130	T222122	5 October 2023
TC	TYPE T	TN131-TN140	T222122	5 October 2023
DATA LOGGER	34970A	T150	T222122	5 October 2023

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 32 Minute At 150 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

(X) without adjustment

() after adjustment

Approved By. 



SCG
CEMENT-BUILDING MATERIALS

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109


Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T230760

Page 3 of 5

Calibration Report

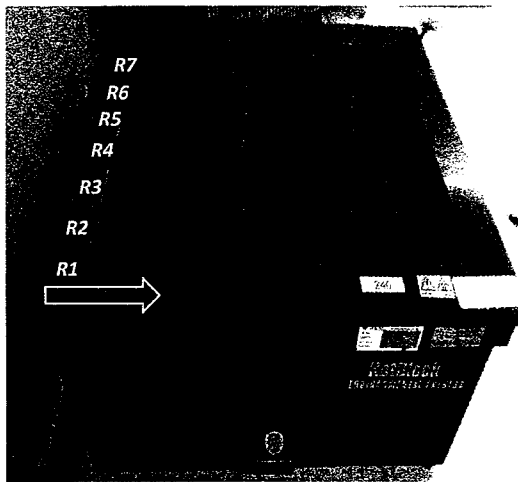

Row	Hole							
R7	H49	H50	H51	H52	H53	H54	H55	H56
R6	H41	H42	H43	H44	H45	H46	H47	H48
R5	H33	H34	H35	H36	H37	H38	H39	H40
R4	H25	H26	H27	H28	H29	H30	H31	H32
R3	H17	H18	H19	H20	H21	H22	H23	H24
R2	H9	H10	H11	H12	H13	H14	H15	H16
R1	H1	H2	H3	H4	H5	H6	H7	H8

H: STANDARD THERMOCOUPLE TYPE T

H1	=	TN121	H9	=	TN129	H17	=	TN137	H25	=	TN125	H33	=	TN133	H41	=	TN121	H49	=	TN129
H2	=	TN122	H10	=	TN130	H18	=	TN138	H26	=	TN126	H34	=	TN134	H42	=	TN122	H50	=	TN130
H3	=	TN123	H11	=	TN131	H19	=	TN139	H27	=	TN127	H35	=	TN135	H43	=	TN123	H51	=	TN131
H4	=	TN124	H12	=	TN132	H20	=	TN140	H28	=	TN128	H36	=	TN136	H44	=	TN124	H52	=	TN132
H5	=	TN125	H13	=	TN133	H21	=	TN121	H29	=	TN129	H37	=	TN137	H45	=	TN125	H53	=	TN133
H6	=	TN126	H14	=	TN134	H22	=	TN122	H30	=	TN130	H38	=	TN138	H46	=	TN126	H54	=	TN134
H7	=	TN127	H15	=	TN135	H23	=	TN123	H31	=	TN131	H39	=	TN139	H47	=	TN127	H55	=	TN135
H8	=	TN128	H16	=	TN136	H24	=	TN124	H32	=	TN132	H40	=	TN140	H48	=	TN128	H56	=	TN136

Approved By. 

Certificate No. T230760

Page 4 of 5

Calibration Report

Measurement Results

			Average Standard Reading at each position (° C)									
Calibration Point			TN121	TN122	TN123	TN124	TN125	TN126	TN127	TN128	TN129	TN130
Point	Setting	Max	149.31	149.49	149.73	148.49	149.26	149.81	149.42	148.86	148.78	149.19
150	150.0	Min	149.14	149.31	149.54	148.36	149.08	149.65	149.22	148.65	149.07	149.07
		Average	149.23	149.40	149.64	148.43	149.16	149.73	149.33	148.76	148.71	149.13
			TN131	TN132	TN133	TN134	TN135	TN136	TN137	TN138	TN139	TN140
		Max	149.90	150.18	150.18	149.16	148.89	149.72	149.28	149.50	150.01	149.32
		Min	149.78	150.06	149.69	149.03	148.76	149.49	149.12	149.37	149.90	149.23
		Average	149.84	150.12	149.76	149.09	148.81	149.62	149.19	149.43	149.95	149.27
			TN121	TN122	TN123	TN124	TN125	TN136	TN127	TN128	TN129	TN130
		Max	149.88	149.14	149.20	150.02	148.75	149.57	149.21	149.18	150.13	148.91
		Min	149.67	148.94	148.98	149.83	148.58	149.43	149.06	149.01	149.91	148.72
		Average	149.78	149.05	149.11	149.94	148.67	149.51	149.13	149.10	150.03	148.83
			TN131	TN132	TN133	TN134	TN135	TN136	TN137	TN138	TN139	TN140
		Max	149.42	149.52	149.13	148.94	148.84	150.16	149.42	149.54	149.66	150.08
		Min	149.27	149.36	148.99	148.81	148.70	149.99	149.27	149.39	149.52	149.97
		Average	149.36	149.45	149.06	148.88	148.76	150.08	149.36	149.48	149.60	150.03
			TN121	TN122	TN123	TN124	TN125	TN126	TN127	TN128	TN129	TN130
		Max	149.21	149.16	149.50	148.68	148.58	149.81	149.06	150.40	148.46	149.24
		Min	149.03	148.93	149.27	148.48	148.42	149.62	148.78	150.26	148.14	149.04
		Average	149.12	149.04	149.39	148.57	148.51	149.72	148.93	150.33	148.29	149.14
			TN131	TN132	TN133	TN134	TN135	TN136				
		Max	148.79	148.23	149.03	149.09	148.46	149.25				
		Min	148.49	147.98	148.88	148.94	148.29	149.12				
		Average	148.61	148.06	148.94	149.02	148.35	149.19				

Approved By.





Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T230760

Page 5 of 5

Calibration Report

Measurement Results

HOT BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (\pm °C)	Uncertainty (\pm °C)
	Min , Max	Average		
150.0	150 , 150.1	150.0	0.20	0.82

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 % .

Approved By. _____



Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No. BSCC-UV-367/23
Equipment UV/Vis Spectrophotometer
Model UV-1800
Manufacturer Shimadzu
Serial No. A11454908533CD
ID No. BKK_EN0018
Date of receipt 15 September 2023
Date of calibration 15 September 2023
Date of issue 22 September 2023



Customer name ALS Laboratory Group (Thailand) Co., Ltd.

Address 104 Soi Phattanakan 40, Phattanakan Road, Phattanakan, Suan Luang, Bangkok 10250

Temperature (23.4 - 24.7) °C (On site)
Humidity (55.5 - 61.2) %RH (On site)

Equipment condition Good Operation

Calibration Location Organic Prep

Calibration Procedure In-house method WI-UV-702-01 based on ASTM E275-01

Traceability Wavelength Accuracy is traceable to certificate No. 95917 and 95918
Photometric Accuracy is traceable to certificate No. 95937 and 95924
Stray Light is traceable to certificate No. 95908
The above certificate are traceable to SI unit through Starna Scientific Ltd.
(UKAS accredited calibration laboratory NO. 0659)

Calibrated by Mr.Wanchana Janloey

Approved by



Mr.Kanchit Choothep
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

Certificate of Calibration

Certificate No.

BSCC-UV-367/23

Number of Page(s)

2 of 3

Calibration Results:

1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (\pm nm)
241.70	241.67	-0.03	0.18
334.02	334.03	0.01	0.18
418.53	418.59	0.06	0.18
572.99	573.14	0.15	0.18
879.41	879.21	-0.20	0.18

2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (\pm A)
235	0.0000	0.0000	0.0000	0.0075
	0.7467	0.7460	-0.0007	0.0075
257	0.0000	0.0000	0.0000	0.0075
	0.8662	0.8646	-0.0016	0.0075
313	0.0000	0.0000	0.0000	0.0075
	0.2904	0.2908	0.0004	0.0075
350	0.0000	0.0001	0.0001	0.0075
	0.6429	0.6415	-0.0014	0.0075

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

Certificate of Calibration

Certificate No. **BSCC-UV-367/23**

Number of Page(s)

3 of 3

Calibration Results:

3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ($\pm A$)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5783	0.5793	0.0010	0.0042
	0.7628	0.7624	-0.0004	0.0042
	1.0206	1.0216	0.0010	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5621	0.5625	0.0004	0.0042
	0.7455	0.7452	-0.0003	0.0042
	0.9985	0.9989	0.0004	0.0042
465.0	0.0000	0.0000	0.0000	0.0042
	0.5227	0.5229	0.0002	0.0042
	0.6880	0.6873	-0.0007	0.0042
	0.9487	0.9486	-0.0001	0.0042
546.1	0.0000	0.0000	0.0000	0.0042
	0.5207	0.5211	0.0004	0.0042
	0.6973	0.6960	-0.0013	0.0042
	0.9959	0.9944	-0.0015	0.0042
590.0	0.0000	0.0000	0.0000	0.0042
	0.5544	0.5538	-0.0006	0.0042
	0.7253	0.7236	-0.0017	0.0042
	1.0942	1.0925	-0.0017	0.0042
635.0	0.0000	0.0000	0.0000	0.0042
	0.5616	0.5612	-0.0004	0.0042
	0.6927	0.6909	-0.0018	0.0042
	1.0881	1.0866	-0.0015	0.0042

*CNR = Customer not request

4. Stray Light*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)		
	Wavelength (nm)	Transmission (%T)	Absorbance (A)
200.96 \pm 0.11nm	200.55	0.9770	2.0104

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

*****End of Certificate*****

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com

**SARTORIUS**

NSC-TISI-TIS 17025

CALIBRATION 0426

Certificate

of Calibration



Model Number : MSE224S-100-DU

Description : Analytical Balance

Serial Number : 27405555

ID No.: BKK_EN0003

Manufacturer : Sartorius

Certificate No. : 23BCI0310

Issued Date : Friday, August 11, 2023

Reference No. : 216011

Page No. : 1 Of 2

Customer Name : ALS Laboratory Group (Thailand)Co., Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250.

Calibrated Place : Lab Room

Calibrated By : Mr.Chonchai Inthana

Calibration Date : Wednesday, August 09, 2023

Calibration

Procedure No. : This calibration was conducted by

Using in-house calibration procedure number (WI-003)

Based on UKAS LAB 14 : 2019

Metrological data :

Capacity : 220 g Readability : 0.0001 g

Ambients Conditions:

Temperature : 22.8 °C ± 5.0 °C

Humidity : 59.0 % RH ± 10.0 % RH

Pressure : ±

Reasons for calibration☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance**Equipment Condition:** ☒ Good Operate ☐ Fair**Measurement Method UKAS Publication Ref :Lab 14**

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2, YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division
Sartorius (Thailand) Co., Ltd.

Mr.chonchai Intrhana(Technical Manager)

S
T
A
M
P

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6 Fax: +66 2643-8367, e-mail: service.thailand@sartorius.com

SARTORIUS

Certificate

of Calibration

Model Number : MSE224S-100-DUDescription : Analytical BalanceSerial Number : 27405555ID No. : BKK_EN0003Manufacturer : SartoriusCertificate No. : 23BCI0310Issued Date : Friday, August 11, 2023Reference No. : 216011Page No. : 2 of 2

Calibration Results : Without Adjustment

Repeatability



The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0000	200.0000
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0001
	20.0000	200.0001
Nominal Value : (High Load)	19.9999	200.0001
200 g	20.0000	200.0000
Tolerance	20.0000	200.0001
0.0001 g	20.0000	200.0001
	20.0000	200.0001
	20.0000	200.0000
Standard Deviation	0.00003	0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 100 g
Tolerance 0.0004 g



Difference

1	—
2	0.0001
3	0.0000
4	0.0000
5	0.0001
6	-

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00014
0.1	0.1000	0.1000	0.0000	0.00014
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0001	0.0001	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	200.0001	0.0001	0.00030

End of Report.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T231303

Page 1 of 3

Certificate of Calibration

Equipment : Liquid Bath (Water)

Manufacturer : MEMMERT

Model : WNB29

Serial No. : L611.0135

Customer Code : BKK_EN0148

ID No. : T6455A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250


Customer Location : ORGANIC PREPARATION LAB

Date of Receipt : 27 June 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 

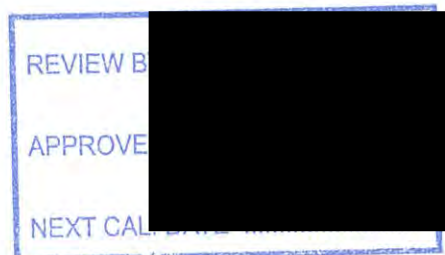

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T231303

Page 2 of 3

Calibration Report

Equipment : Liquid Bath (Water)
Date of Calibration : 4 July 2023
Environment : Temperature : 22.2-22.5 °C
Line Voltage : 221.6-224.8 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 (based on ASTM E715-80 (Reapproved 2001)).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M18 (CH1,CH6-CH7,CH9-CH10)	T230545	10 April 2024
DATA LOGGER	34970A	T149	T230545	10 April 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 3 Hour 45 Minute At 60 °C

5. Adjustment :

(X) without adjustment

() after adjustment


Approved By—



Certificate No. T231303

Page 3 of 3

Calibration Report

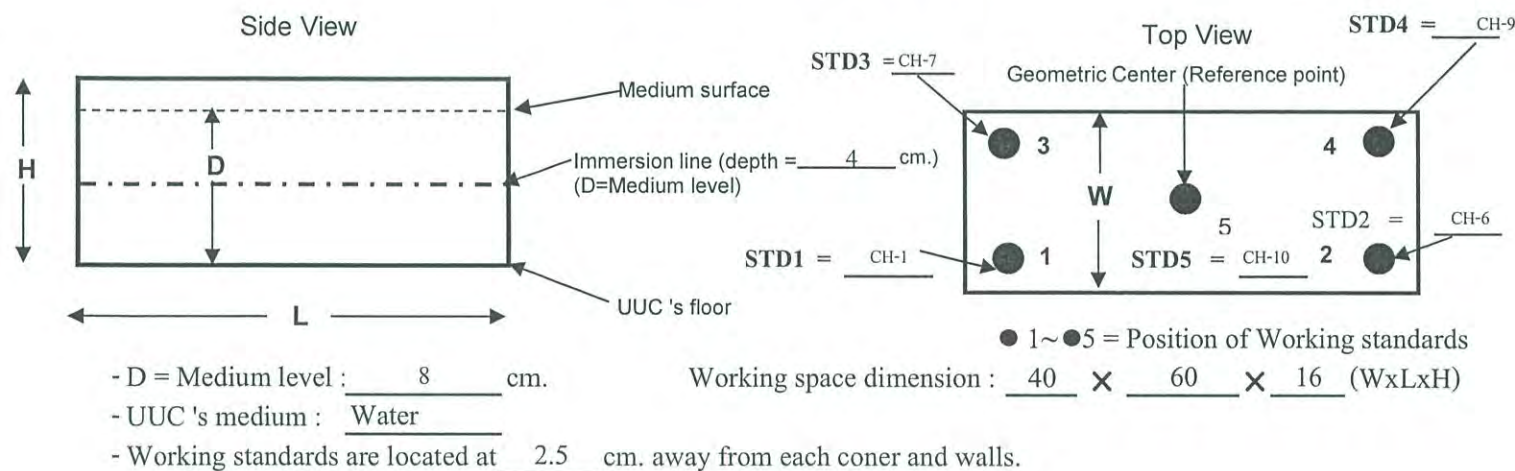

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)				
	CH-1	CH-6	CH-7	CH-9	CH-10
60	60.03	60.06	60.24	60.11	60.18
85	84.79	84.83	85.42	85.05	85.20
95	93.71	93.83	94.62	94.15	94.42

Liquid Bath (Water)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (±°C)	Uncertainty (±°C)	Coverage Factor <i>k</i>
	Min , Max	Average					
61.0	60.9 , 61.1	61.0	60.12	0.13	0.19	0.29	2.04
86.0	85.8 , 86.2	86.0	85.06	0.19	0.47	0.44	2.17
95.0	94.6 , 95	94.9	94.15	0.32	0.65	0.55	2.13

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By _____



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CH1222

Page.: 1 of 2

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	Seven Compact S220
Serial No. :	B520948426
ID No. :	BKK_EN0072
Condition As-Received:	Used Item
Received Date :	09 September 2022
Calibration Date :	12 September 2022
Reference :	2209-0312DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)

REVIEW BY ...

APPROVED BY

NEXT CAL. DA

Calibrated by : Warakorn Lerngagtrakul

Approved by :

Approved Signatory

- (☒) Malee Butkruea
(☐) Saithip Meangmai
(☐) Warakorn Lerngagtrakul

Issue Date : 15 September 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert. No.: 22CH1222

Page.: 2 of 2

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	22E2769	24 Aug 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	823320	20 June 2024
pH 6.985	CPA chem	794122	14 Feb 2023
pH 10.008	CPA chem	823323	20 June 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results**Function : mV Measurement****Performing standard curve by Fluke at pH (4,7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (\pm mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: B520948426	4.000	177.48	177.4	4.000	0.058	2.00
	7.000	0.00	0.0	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Function : pH Measurement**Performing three buffers standard curve by using buffer nominal pH (4,7,10)**

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (\pm)	Coverage factor <i>k</i>
pH Electrode S/N.: PCE-86-EX1001	4.008	3.999	153.9	0.0055	2.09
	6.985	7.017	-13.7	0.0084	2.00
	10.008	9.996	-179.0	0.0078	2.06

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-oOo-

Malu.

a 1126274



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484




Cert.No.: 23CH1209

Page.: 1 of 2

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	Seven2Go pH
Serial No. :	C117620932
ID No. :	BKK_LG0044
Condition As-Received:	Used Item
Received Date :	25 September 2023
Calibration Date :	26 September 2023
Reference :	2309-0827DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	<div style="text-align: center;"> Approved Signatory</div>
	(<input checked="" type="checkbox"/>) Saithip Meangmai (<input type="checkbox"/>) Warakorn Lerngagtrakul (<input type="checkbox"/>) Ponpan Paipim
Issue Date :	29 September 2023

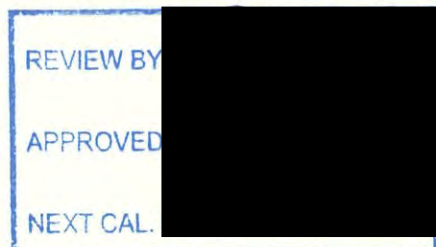

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0058949



Cert. No.: 23CH1209

Page.: 2 of 2

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	913598	14 July 2025
pH 6.986	CPA chem	863833	28 Dec 2023
pH 9.997	CPA chem	913600	14 July 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: C117620932	4.00	177.48	177	4.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-177	10.00	0.58	2.00

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor <i>k</i>
pH Electrode S/N.: 2354505	4.008	4.01	191	0.0079	2.00
	6.986	7.00	18	0.0093	2.00
	9.997	10.00	-159	0.0095	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

a 1182567



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23LM164

Page.: 1 of 2

Certificate of Calibration

Equipment : pH Meter with Sensor

Manufacturer : Metter Toledo

Model : Seven2Go S2

Serial No. : C117620932

ID No. : BKK_LG0044

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : TPA Chemistry Calibration Laboratory

Received Order : 25 September 2023

Calibrated Date : 29 September 2023

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Krisda Malee

Approved by :

Approved Signatory

() Pornthippa Tameyakul

() Ponpan Paipim

(✓) Suwit Imjai

Issue Date : 4 October 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : pH Meter with Sensor
Condition As-Received : Used Item
Reference : 2309-0827DSC-2

Cert. No.: 23LM164

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	A52847	2211325	TPA	31 Oct 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 2354505

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.0	100	20.005	19.9	-0.105	0.16	2.00
25.0	100	24.998	25.0	0.002	0.16	2.00
30.0	100	30.001	29.9	-0.101	0.16	2.00
35.0	100	35.001	34.9	-0.101	0.16	2.00
40.0	100	40.005	39.9	-0.105	0.16	2.00
45.0	100	45.001	44.9	-0.101	0.16	2.00
50.0	100	50.004	49.9	-0.104	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T222502

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Oven)

Manufacturer : Memmert

Model : UF 450

Serial No. : B7170531

Customer Code : BKK_EN0273

ID No. : T8042A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Oven Room

Date of Receipt : 23 November 2022

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By : [Redacted] /Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 09 DEC 2022

REVIEW BY	Sujjar Naknakred
APPROVED BY	[Redacted]
NEXT CAL. DATE	09 DEC 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T222502

Page 2 of 4

Calibration Report

Equipment : Chamber (Oven)
Date of Calibration : 29 November 2022
Environment : Temperature : 29.1-29.6 °C
Line Voltage : 221.3-223.2 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors and nine standard thermocouples type T into its chamber , the other one resistance thermometer detector use for ambient temperature measurement .
The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	27-(CH1-10)	T210004	30 December 2022
TC	TYPE T	TN261-TN270	T210010	30 December 2022
DATA LOGGER	34970A	T149	T210004	30 December 2022

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 49 Minute At 104 °C
Fresh Air Damper ☒ Open ☐ Min ☐ Medium ☒ Max
☐ Close
☐ Not Available

5. Adjustment :

() without adjustment


(X) after adjustment

Approved By. _____

Certificate No. T222502

Page 3 of 4

Calibration Report

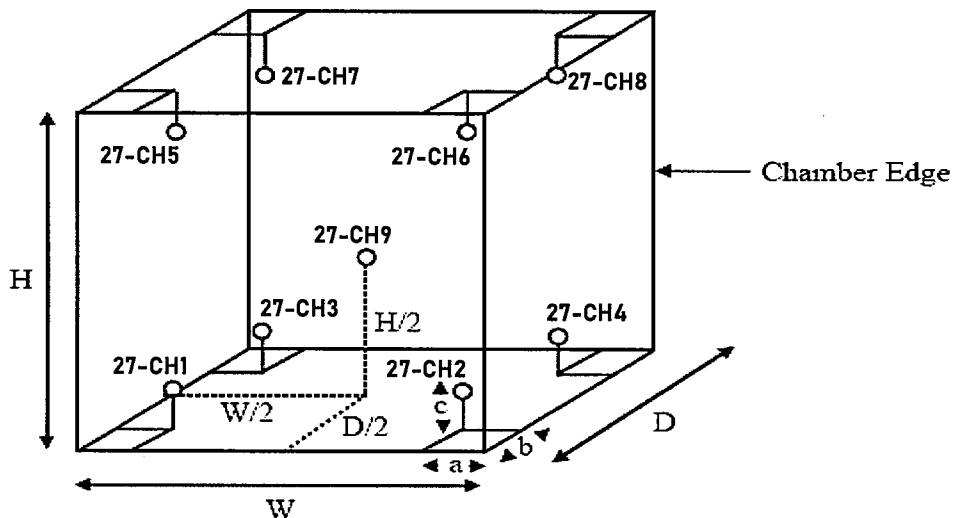

Remark :

Internal Dimensions of Chamber : W (Width) = 104 cm. , H (Height) = 72 cm. and D (Depth) = 60 cm.

Size of Installed Standard sensor number 27-CH1 to number 27-CH8 : a = 5 cm. , b = 5 cm. and c = 5 cm.

Size of Installed Standard sensor number 27-CH9 : W/2 = 104 cm./2 , H/2 = 72 cm./2 and D/2 = 60cm./2

Measurement Results

Average Standard Reading at each position (°C)									
Calibration Point	27-CH1	27-CH2	27-CH3	27-CH4	27-CH5	27-CH6	27-CH7	27-CH8	27-CH9
104	104.07	103.60	103.45	104.02	104.47	103.57	104.59	103.78	104.18

Chamber (Oven)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
	Min , Max	Average					
104.0	-	104.0	103.97	0.07	0.70	0.42	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.


The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____

Certificate No. T222502

Page 4 of 4

Calibration Report

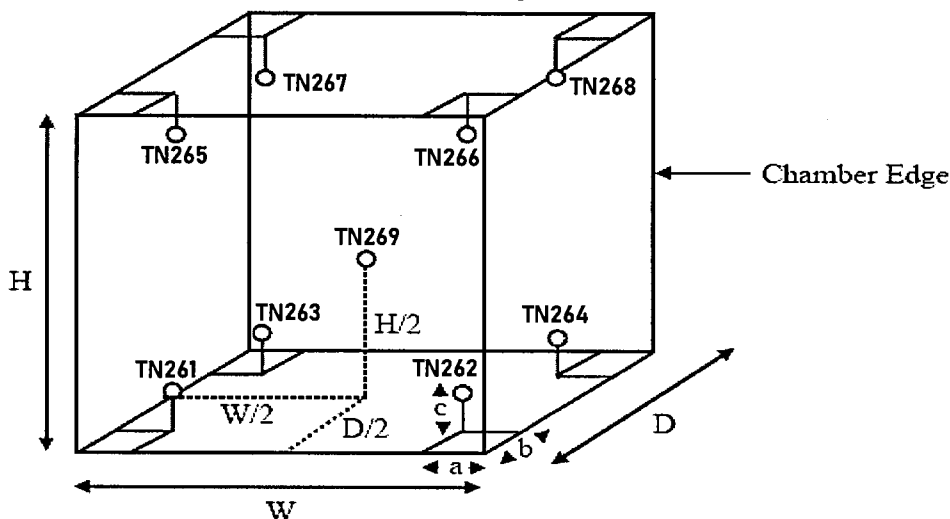

Remark :

Internal Dimensions of Chamber : W (Width) = 104 cm. , H (Height) = 72 cm. and D (Depth) = 60 cm.

Size of Installed Standard sensor number TN261 to number TN268 : a = 5 cm. ,b = 5 cm. and c = 5 cm.

Size of Installed Standard sensor number TN269 : W/2 = 104 cm./2 , H/2 = 72 cm./2 and D/2 = 60cm./2

Measurement Results

Calibration Point	Average Standard Reading at each position (° C)								
	TN261	TN262	TN263	TN264	TN265	TN266	TN267	TN268	TN269
180	179.14	179.17	179.65	179.26	180.41	179.64	181.18	180.99	180.36

Chamber (Oven)			Temperature Distribution				
Setting (° C)	Reading (° C)		Average (° C)	Stability (± ° C)	Uniformity (° C)	Uncertainty (± ° C)	Coverage Factor <i>k</i>
	Min , Max	Average					
180.0	-	180.0	179.98	0.38	1.78	1.10	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing

a level of confidence of approximately 95 % .

Approved By. _____

Certificate No. T230902

Page 1 of 5

Certificate of Calibration

Equipment : Digestion Unit

Manufacturer : SCP Science

Model : DigiPRER HT

Serial No. : HTC1120480658

Customer Code : BKK_EN0366

ID No. : T2635A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250


Customer Location : Wet Chemistry Lab 1

Date of Receipt : 10 May 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 29 MAY 2023

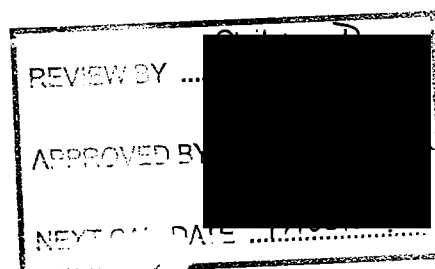

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T230902

Page 2 of 5

Calibration Report

Equipment : Digestion Unit
Date of Calibration : 17 May 2023
Environment : Temperature : 23.9 - 26.3 °C
Line Voltage : 221.8 - 225.9 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T10.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M20A1-(CH17-CH20)	T230547	18 April 2024
DATA LOGGER	34970A	T149	T230547	18 April 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 54 Minute At 380 °C

Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max

☐ Close

☒ Not Available

5. Adjustment :

(X) without adjustment


() after adjustment

Approved By. 

Certificate No. T230902

Page 3 of 5

Calibration Report

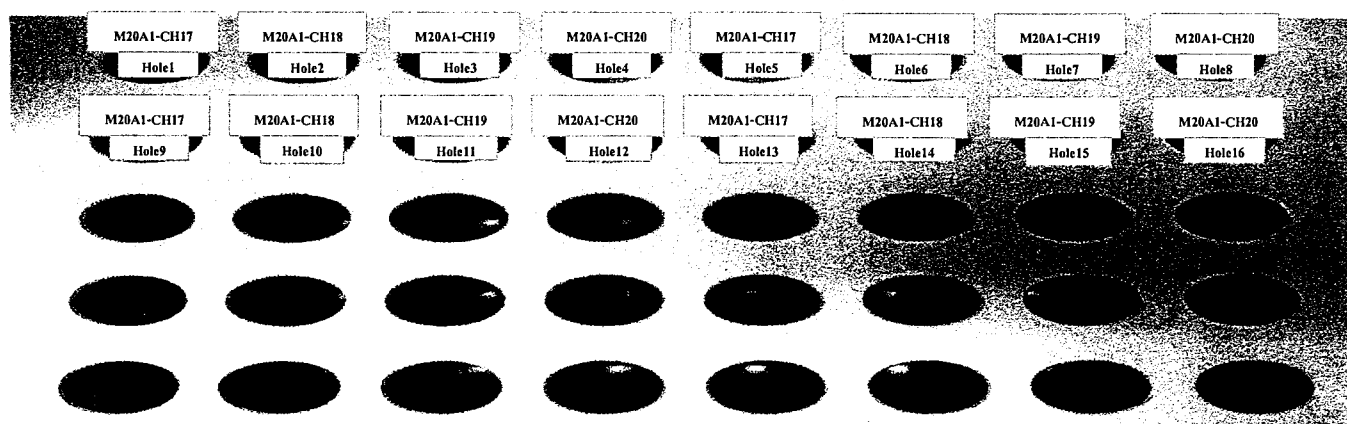

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole1	Hole2	Hole3	Hole4	Hole5	Hole6	Hole7	Hole8
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.3	379.0	379.2	380.2	377.5	379.5	380.7	380.1
			Min °C	376.8	378.6	378.9	379.9	377.0	379.0	380.2	379.6
			Average °C	377.0	378.8	379.1	380.0	377.3	379.2	380.4	379.9
			Stability ± °C	0.2	0.2	0.2	0.2	0.3	0.3	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole9	Hole10	Hole11	Hole12	Hole13	Hole14	Hole15	Hole16
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.1	378.9	379.7	379.9	379.3	379.6	379.5	377.4
			Min °C	376.7	378.5	379.3	379.5	378.9	379.1	379.0	377.0
			Average °C	376.9	378.7	379.5	379.7	379.1	379.4	379.3	377.2
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.3	0.3	0.2


Approved By.



Certificate No. T230902

Page 4 of 5

Calibration Report

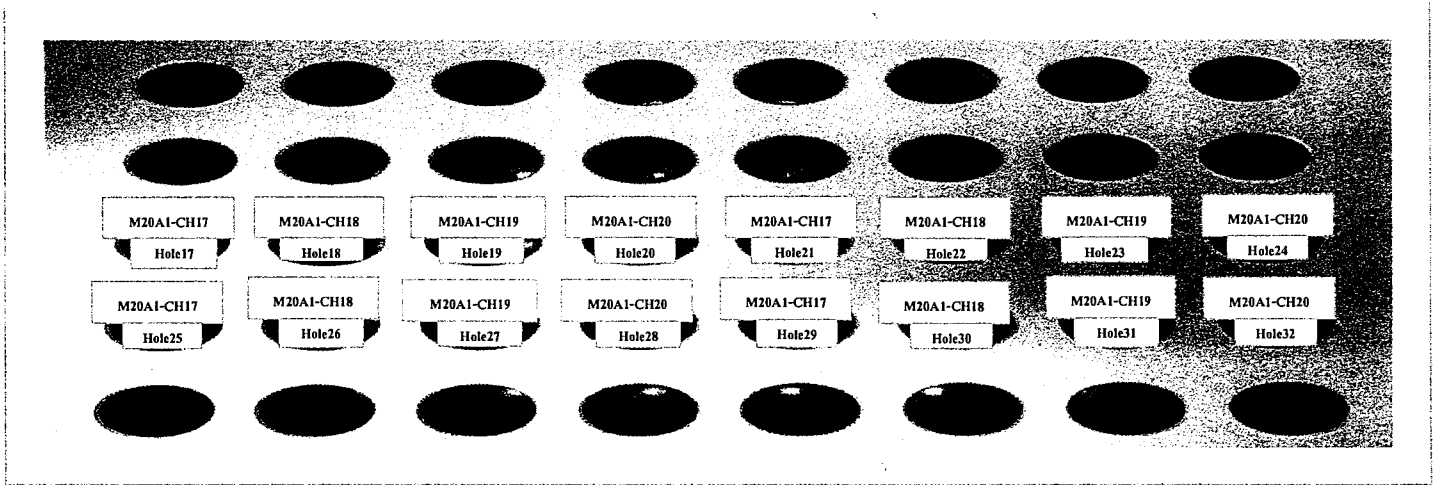

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole17	Hole18	Hole19	Hole20	Hole21	Hole22	Hole23	Hole24
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	378.4	380.1	380.1	380.0	379.1	379.8	379.6	377.8
			Min °C	377.8	379.6	379.7	379.3	378.6	379.2	379.2	377.3
			Average °C	378.1	379.9	379.9	379.7	378.9	379.5	379.4	377.5
			Stability ± °C	0.3	0.3	0.2	0.3	0.3	0.3	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole25	Hole26	Hole27	Hole28	Hole29	Hole30	Hole31	Hole32
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.9	379.4	380.1	380.1	379.3	379.6	378.9	377.3
			Min °C	377.4	378.9	379.7	379.7	378.8	378.9	378.4	376.7
			Average °C	377.7	379.2	379.9	379.9	379.0	379.3	378.6	377.0
			Stability ± °C	0.3	0.3	0.2	0.2	0.3	0.4	0.3	0.3


Approved By.



Certificate No. T230902

Page 5 of 5

Calibration Report

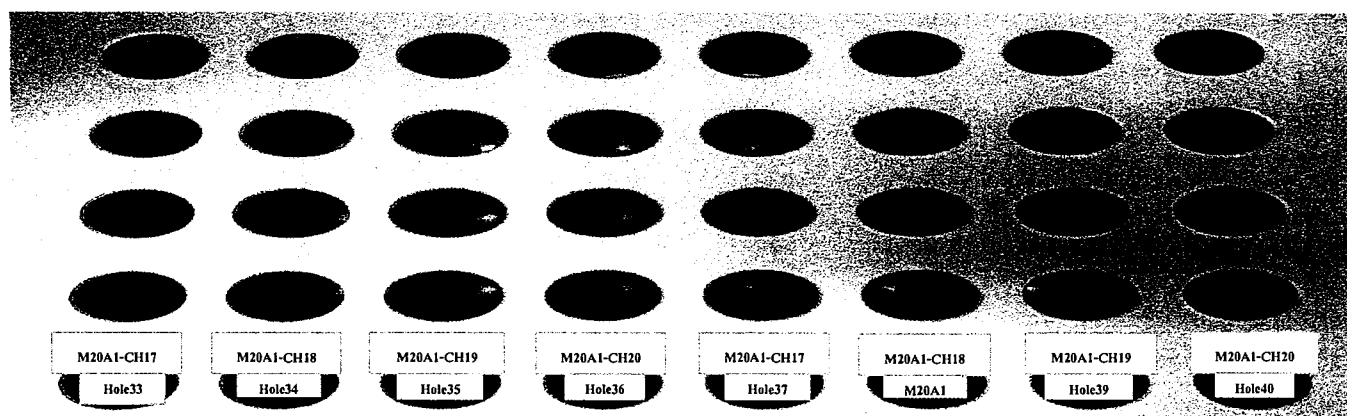

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole33	Hole34	Hole35	Hole36	Hole37	Hole38	Hole39	Hole40
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.7	378.0	378.3	379.0	378.2	378.5	377.3	377.4
			Min °C	377.3	377.6	377.9	378.6	377.7	378.1	376.9	377.0
			Average °C	377.5	377.8	378.1	378.8	378.0	378.3	377.1	377.2
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.2	0.2	0.2

 The expanded uncertainty of temperature measurement was ± 1.85 °C

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

 The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 % .

Approved By.



บริษัท ดับเบิล เอส ไดแอกโนสติกส์ จำกัด
DOUBLE S DIAGNOSTICS CO., LTD.

4 ซอยอุดมสุข 14 แขวงบางนา เขตบางนา กรุงเทพมหานคร 10260 โทรศัพท์: (02) 747-7009 โทรสาร: (02) 747-7008
4 Soi Udomsuk 14, Bangna, Bangkok 10260 Tel. (02) 747-7009 Fax: (02) 747-7008

Maintenance Plan YEAR : 2023

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
รวม							12/7 OK					

Periodical maintenance check list for Konelab

	6M	12M	Note!
1.Diluent-wash tubing change	<input type="checkbox"/>	<input checked="" type="checkbox"/>
2.ISE tubing change	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	none
3.Syringe check/change		<input checked="" type="checkbox"/>
4.Dispensing check/ change		<input checked="" type="checkbox"/>
5.Waste tubing change when necessary		<input checked="" type="checkbox"/>
6.Lamp check/change	<input type="checkbox"/>	<input checked="" type="checkbox"/>
7.Mixer paddle/paddle change(not Konelab20)		<input checked="" type="checkbox"/>
8.ISE needles check/change		<input checked="" type="checkbox"/>	none
9.Pump tubing check/ chance	<input type="checkbox"/>	<input checked="" type="checkbox"/>
10.Broken/worn out part check /change		<input checked="" type="checkbox"/>
11.Peristaltic pump check /cleaning/ lubrication	<input type="checkbox"/>	<input checked="" type="checkbox"/>
12.Heating check		<input checked="" type="checkbox"/>
13.Cooling check		<input checked="" type="checkbox"/>
14.Dispenser mechanic check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>
15.Cuvette transfer mechanic check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>
16.Dispenser movement check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>
17.Sample/reagent register check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>
18.Dispensing tubing tightness check	<input type="checkbox"/>	<input checked="" type="checkbox"/>
19.Photometer and optics cleaning/check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>
20.Workstation PC cleaning if necessary	<input type="checkbox"/>	<input checked="" type="checkbox"/>
21.Mechanic cleaning/lubrication	<input type="checkbox"/>	<input checked="" type="checkbox"/>
22.Instrument cleaning if necessary	<input type="checkbox"/>	<input checked="" type="checkbox"/>
23.Complete analyzer testing with waterblank/QC or sample	<input type="checkbox"/>	<input checked="" type="checkbox"/>
24.Test parameters/Adjustment/config. Save to USB key	<input type="checkbox"/>	<input checked="" type="checkbox"/>
25.UPS Test	<input type="checkbox"/>	<input checked="" type="checkbox"/>

Place: ALS LAB Instrument: k90 Aquakem
Date/Time: 12/7/66 Serial no: 22781
Service done by: ๒๓๖๕ Install date:
Signature of customer: ๒๓๖๕ Date/Time: 12/7/66

Laboratory
Analyzer User

7/12/2023 21:21

Performed 7/12/2023
Lot W166

=====

ACCEPTANCE CRITERIA

=====

	Result	Limit	Warning
Temperature (?C)	37.7	37.0 +/- 1.0	
Dispensing ratio	16.4	14.8 - 17.2	
CV%	1.17	<1.7	
Photometric noise			
Max SD L340_2 (mA)	0.19	<2.0	
Max SD L340_4 (mA)	1.06	<3.0	
Linearity of photometer			
Slope	1.0188	0.94 - 1.06	
Curvature	0.0035	+/- 0.02	
Max bias from linear fit (mA)	3.2	<15.0	
Max delta %	-2.0	+/- 6.0	
Linearity of sample dispensing			
Proport. volume XDISP2 (?l)	2.06	1.96 - 2.16	
Proport. volume XDISP4 (?l)	4.13	3.85 - 4.40	
XDISP2 CV%	0.58	<2.0	
XDISP4 CV%	0.70	<2.0	
XDISP10 CV%	0.59	<2.0	
Needle 0 ?l volume			
Average (A)	0.009	<0.050	
Standard deviation (A)	0.002	<0.005	
Volume (?l)	0.06	<0.32	

=====

OTHER INFORMATION

=====


Dispensing ratio		Photom., noise: SD (mA)	
Posit	Result (A)	Posit	L340_2 L340_4
1	0.1592	1	0.07 0.64
2	0.1624	2	0.09 1.06
3	0.1631	3	0.14 0.50
4	0.1631	4	0.13 0.53
5	0.1625	5	0.19 0.38
6	0.1650	6	0.02 0.64

Linearity of sample dispensing

Test	Absorbance (A)
XDISP2	0.311
XDISP4	0.616
XDISP10	1.478

Linearity of photometer

L340_	Target (A)	Meas (A)	Delta (A)	Delta %
1	0.001	0.005	-0.004	-394.7
2	0.512	0.519	-0.007	-1.5
3	1.523	1.550	-0.027	-1.8
4	2.027	2.066	-0.039	-1.9
5	2.532	2.582	-0.050	-2.0

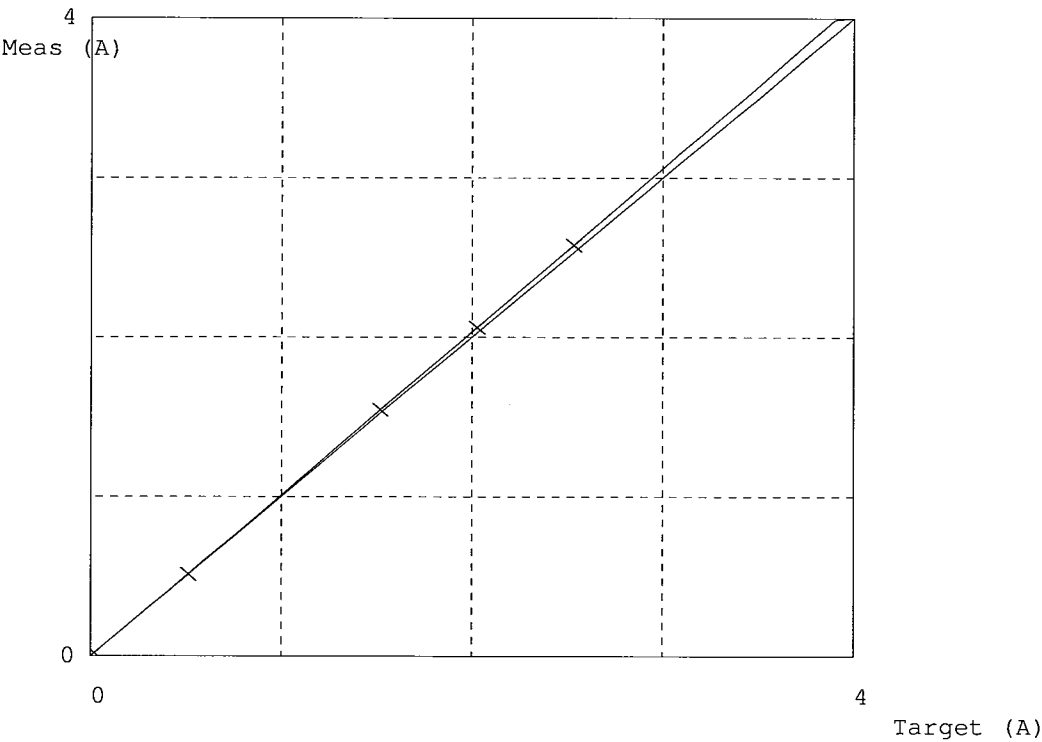

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com



NSC-TISI-TIS 17025

CALIBRATION 0426

SARTORIUS

Certificate

of Calibration

REVIEW BY

APPROVED BY

NEXT CAL. DATE

Model Number : MSE224S-100-DUDescription : Analytical BalanceSerial Number : 26207042ID No. : BKK_EN0002Manufacturer : SartoriusCertificate No. : 23BCI0072Issued Date : Monday, February 13, 2023Reference No. : 203245Page No. : 1 of 2Customer Name : ALS Laboratory Group (Thailand)Co., Ltd.104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.Calibrated Place : Balance RoomCalibrated By : Mr. Chonchai InthanaCalibration Date : Wednesday, February 08, 2023**Calibration**Procedure No. : This calibration was conducted byUsing in-house calibration procedure number (WI-003)Based on UKAS LAB 14 : 2019**Metrological data :**Capacity : 220 g Readability : 0.0001 g**Ambients Conditions:**Temperature : 23.2 °C ± 5.0 °CHumidity : 60.0 % RH ± 10.0 % RHPressure : ± **Reasons for calibration**☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ MaintenanceEquipment Condition: ☒ Good Operate ☐ Fair**Measurement Method****UKAS Publication Ref :Lab 14**

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2, YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division
Sartorius (Thailand) Co., Ltd.

SOP FM 33 03 February 2022

Mr.Chonchai Inthana(Technical Manager)

S
T
A
M
P

Certificate of Calibration

Model Number : MSE224S-100-DU
 Description : Analytical Balance
 Serial Number : 26207042
 ID No. : BKK_EN0002
 Manufacturer : Sartorius

Certificate No. : 23BCI0072
 Issued Date : Monday, February 13, 2023
 Reference No. : 203245
 Page No. : 2 of 2

Calibration Results : Without Adjustment

Repeatability



The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0000	199.9999
Tolerance	20.0000	200.0000
0.0001 g	20.0000	199.9999
	20.0001	200.0000
	20.0000	200.0000
Nominal Value : (High Load)	20.0000	199.9999
200 g	20.0000	199.9999
Tolerance	20.0000	200.0000
0.0001 g	20.0000	199.9999
	20.0001	199.9999
Standard Deviation	0.00004	0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 50 g
 Tolerance 0.0004 g



Difference	
1	—
2	-0.0001
3	0.0000
4	0.0001
5	0.0000
6	—

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00014
0.1	0.1000	0.1000	0.0000	0.00014
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	199.9999	-0.0001	0.00030

End of Report.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1103

Page : 1 of 3

Certificate of Calibration

Equipment : Autoclave

Manufacturer : Sanyo

Model : MLS-3781

Serial No. : 830167

ID No. : BKK_ML0037

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand


Location : Media Preparation Room

Received Order : 17 July 2023

Calibration Date : 17 July 2023

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

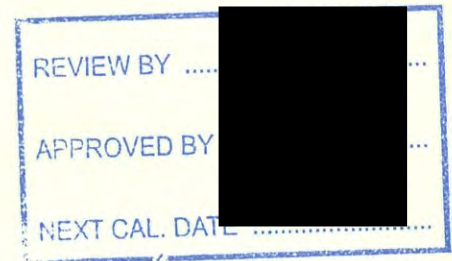

Calibrated by : Preecha Hlahib

Approved by :

Approved Signatory

() Pornthippa Tameyakul
() Malee Butkruea
(✓) Suwit Imjai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2307-0285OC-3

Cert. No.: 23TM1103

Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY57013823	23LM66	TPA	25 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**

(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)


It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

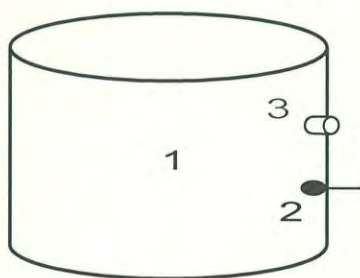

	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	22	53	220
Finished of Calibration	22	54	220

<u>Position</u>	<u>Description</u>	<u>Ref. Std. ID No.:</u>
1 =	Center of chamber	22-17TC-01
2 =	Temperature sensor	23-17TC-02
3 =	Exhaust port	19-17TC-03



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2307-0285OC-3

Cert. No.: 23TM1103

Page : 3 of 3

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Operating parameter Set : Temperature = 121 °C

Sterilization period = 15 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
121	121	1	120.877	0.39	0.12	1.0	2
		2	120.870				
		3	120.866				

Average* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1146

Page : 1 of 3

Certificate of Calibration

Equipment : Incubator

Manufacturer : SHEL-LAB

Model : 1915A

Serial No. : 0200599

ID No. : BKK_ML0010

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthakan Rd.,
Khwawng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Incubation & Micrological Reading

Received Order : 17 July 2023
Calibration Date : 17 July 2023
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon

REVIEW BY	githai l. l.
APPROVED BY	
NEXT CAL. DATE	

Approved by :

Approved Signatory

- () Pornthippa Tameyakul
(/) Malee Butkruea
() Suwit Imjai

Issue Date :

24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0056489



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1
Procedure Used :-

Cert. No.: 23TM1146

Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	24
REL.Humid. (%)	54	56
AC Supply (Volt)	221	223

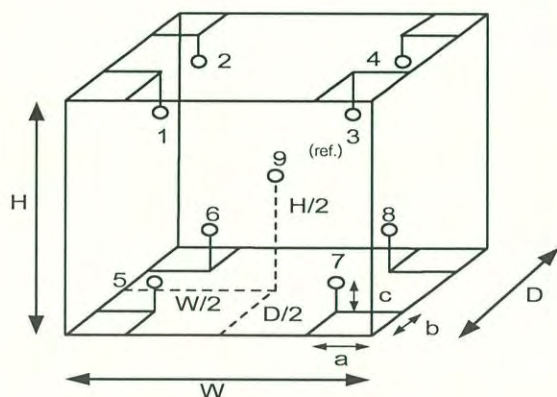

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.50 m
W = 0.75 m
H = 1.2 m
Capacity = 0.45 m³



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 23TM1146

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
35.0	35.0	35.0	0.055	0.30	0.44	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.888	34.933	34.815	34.813	35.064	35.019	35.156	35.141	35.087	0.30

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1571

Page : 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Binder

Model : ED 240/E2

Serial No. : 00-15533

ID No. : BKK_ML0013

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 21 November 2022

Calibration Date : 21 November 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

Approved by :

Approved Signatory

(/) Pornthippa Tameyakul

(/) Malee Butkruea

() Suwit Imjai

Issue Date : 29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0048150



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1

Cert. No.: 22TM1571

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) After Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

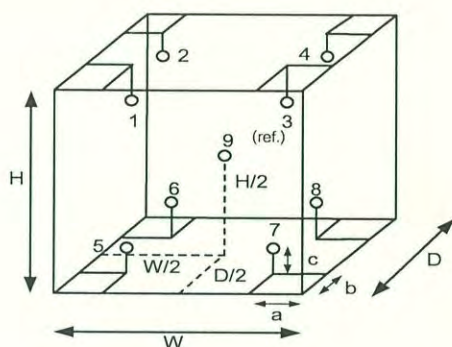

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	26
REL.Humid. (%)	53	55
AC Supply (Volt)	219	220

Position :	Ref. Std. ID No.:
1	21-15TC-01
2	21-15TC-02
3	21-15TC-03
4	21-15TC-04
5	21-15TC-05
6	21-15TC-06
7	21-15TC-07
8	21-15TC-08
9 (ref.)	21-15TC-09

Probe Installation Details :

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :

D = 0.50 m
W = 0.80 m
H = 0.60 m
Capacity = 0.24 m³



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1
Result of Calibration :- (*) After Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 22TM1571

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
180	180	180	0.70	1.5	2.9	1.4	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
180	179.520	180.585	178.855	179.482	178.827	179.938	179.074	180.199	180.068

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM637

Page : 1 of 3

Certificate of Calibration

Equipment : Water Bath

Manufacturer : Memmert

Model : WNE 45

Serial No. : L712.0429

ID No. : BKK_ML0056

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Incubator & Microbiological Reading


Received Order : 20 April 2023

Calibration Date : 20 April 2023

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Kunchit Promprat

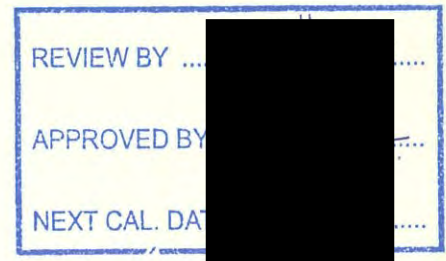

Approved by :

Approved Signatory

- () Pornthippa Tameyakul
(/) Malee Butkruea
() Suwit Imjai

Issue Date :

24 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0053357



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2304-0253OC-1

Cert. No.: 23TM637

Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Data Acquisition	34970A	MY44073381	22LM78/1	12 May 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	<u>Environmental</u>		<u>AC Voltage Supply</u>
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	45	223
Finished of Calibration	25	43	223

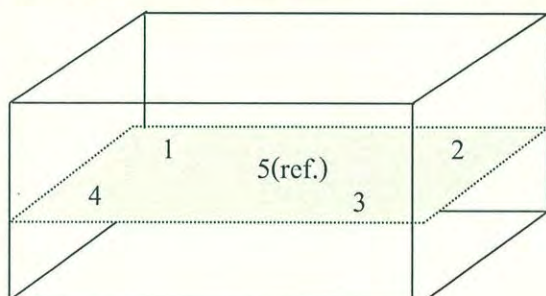

Front

<u>Position :</u>	<u>Ref. Std. S/N.:</u>
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2304-0253OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM637

Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.492	44.463	44.475	44.510	44.491	0.15
45.0	45.0	45.0	45.005	44.962	44.979	45.016	44.986	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor <i>k</i>
44.5	0.051	0.022	2
45.0	0.080	0.026	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1583

Page : 1 of 3

Certificate of Calibration

Equipment : Low Temp. Incubator

Manufacturer : ShellLab

Model : 2020-2E

Serial No. : 0601299

ID No. : BKK_ML0011

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Incubation & Microbiological Reading

Received Order : 21 November 2022

Calibration Date : 21 November 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

Approved by :

App [redacted] tory

(/) Pornthippa Tameyakul
(/) Malee Butkruea
() Suwit Imjai

Issue Date :

29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0048153



Equipment : Low Temp. Incubator
 Condition As-Received : Used Item
 Reference : 2211-0623OC-4

Cert. No.: 22TM1583
 Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) After Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	24
REL.Humid. (%)	50	54
AC Supply (Volt)	219	220

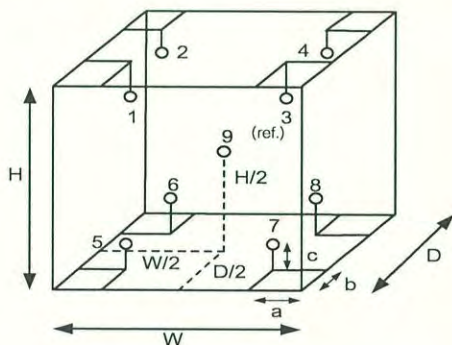

Position :	Ref. Std. ID No.:
1	19-15RTD-01
2	19-15RTD-02
3	19-15RTD-03
4	19-15RTD-04
5	19-15RTD-05
6	21-15RTD-06
7	19-15RTD-07
8	19-15RTD-08
9 (ref.)	19-15RTD-09

Probe Installation Details :

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of Chamber :

D = 0.55 m
 W = 1.2 m
 H = 0.69 m
 Capacity = 0.46 m³



Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2211-0623OC-4
Result of Calibration :- (*) After Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 22TM1583

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
25.0	25.0	25.0	0.019	0.29	0.34	0.30	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
25.0	25.177	25.199	25.166	25.172	25.027	24.893	25.061	25.152	25.173

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 8-Jan-2023

Certificate No. : 23TH0050

CSR No. : A047/02339

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : Autoclave

Manufacturer : TOMY

Model : SX-700

Serial No. : 52134079

ID No. : SGK_ML0001

Resolution : 1 °C

Received Date : 5-Jan-2023

Calibrated Date : 5-Jan-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY
APPROVED BY
NEXT CAL. DATE

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.16.013 based on BS 2646 : 1993 (part 5)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- ScaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Kanyarat Cha

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration


1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data logger With Sensor	GL220	C90432223	22SDAT005	4-May-2023

- The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.
- This certificate is not certified any commercial transaction
- Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

1. Sensor Installation Diagram

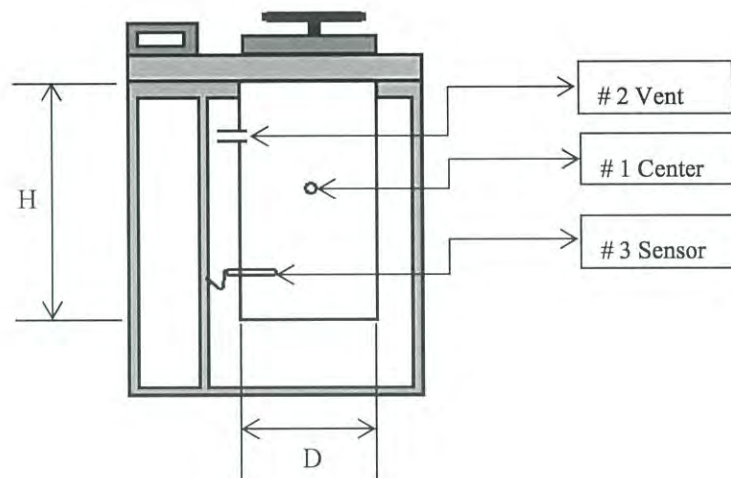

Chamber Diameter (D) : 30 cm

Chamber Height (H) : 70 cm



Certificate No. : 23TH0050

CSR No. : A047/02339

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Autoclave and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)			Pressure Reading	Uncertainty (± °C)
	Center #1	Vent #2	Sensor #3		
115	115.5	115.4	115.5	0.07 MPa	0.76
118	118.7	118.9	119.1	0.09 MPa	0.76
121	122.0	122.1	122.1	0.11 MPa	0.76

3. Performance Result

The performance of the Autoclave are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
115	115	115	0.20	0.30	0.30
118	118	118	0.70	0.70	0.90
121	121	121	0.50	0.40	0.60

- Operating Time = 1800.65 sec

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 9-Aug-2022

Certificate No. : 22OV529

CSR No. : A037/01847

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Kamchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : Incubator

Manufacturer : Memmert

Model : ICP750

Serial No. : F816.0061

ID No. : SGK_ML0013

Resolution : 0.1 °C

Received Date : 6-Aug-2022

Calibrated Date : 6-Aug-2022

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY

APPROVED BY ...

NEXT CAL. DATE

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on G-20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Kanyarat Chaipet / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

(☒) Without Adjustment

(☐) After Adjustment

1. Sensor Installation Diagram

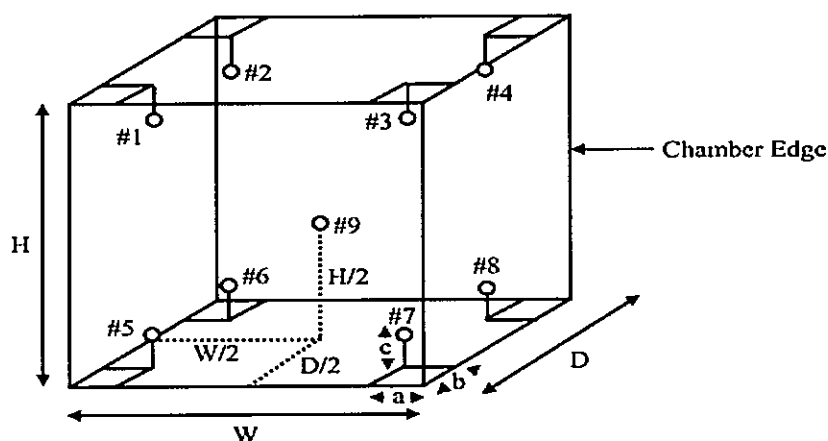

Sensor Installation Details

a = 5.0 cm

b = 5.0 cm

c = 5.0 cm

Dimension of the chamber

W = 104.0 cm

H = 120.0 cm

D = 60.0 cm



Certificate No. : 22OV529

CSR No. : A037/01847

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Incubator and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
35	34.99	34.92	34.95	34.88	34.96	35.00	34.94	34.94	34.94	0.38

3. Performance Result

The performance of the Incubator are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
35	35.0	35.0	0.10	0.12	0.19

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 8-Jan-2023

Certificate No. : 23CH0016

CSR No. : A047/02339

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : pH meter

Manufacturer : Sartorius

Model : Basic pH Meter PB-10

Serial No. : C70160695

ID No. : SGK_ML0016

Electrode No. : N/A

Received Date : 5-Jan-2023

Calibrated Date : 5-Jan-2023

Ambient Temperature : $(25 \pm 3) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \%$

REVIEW BY
APPROVED
NEXT CAL.

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HACH : HACH LANGE GmbH
- WK : WK Electric Co., Ltd.

Calibrated by : Jessadagon Lemhud

Approved by :

Kanyarat Chaipet / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.005	C02950	1733	22-Apr-2024
Standard Solution	7.000	C03001	1783	23-Sep-2024
Standard Solution	10.013	C02953	1735	29-Apr-2024
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	5-Jun-2024

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading (mV)	Correction (mV)	Uncertainty (± mV)
177.48	177.4	0.08	0.17
0.00	0.0	0.00	0.13
-177.48	-177.4	-0.08	0.17

2. Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading (pH)	Correction (pH)	Uncertainty (± pH)
4.004	4.02	-0.016	0.011
7.000	7.01	-0.010	0.013
10.013	10.02	-0.007	0.036

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 2-Feb-2023

Certificate No. : 23TH0521

CSR No. : A075/03704

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : Water Bath

Manufacturer : Memmert

Model : WPE45

Serial No. : L716.0558

ID No. : SGK_ML0021

Resolution : 0.1 °C

Received Date : 30-Jan-2023

Calibrated Date : 30-Jan-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	[Signature]
APPROVED BY	[Signature]
NEXT CAL. DATE ...	

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.014 based on ASTM E 715 : 1980
(reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement
according to the International System of Unit (SI) through :

- SCAI : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration ∴

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

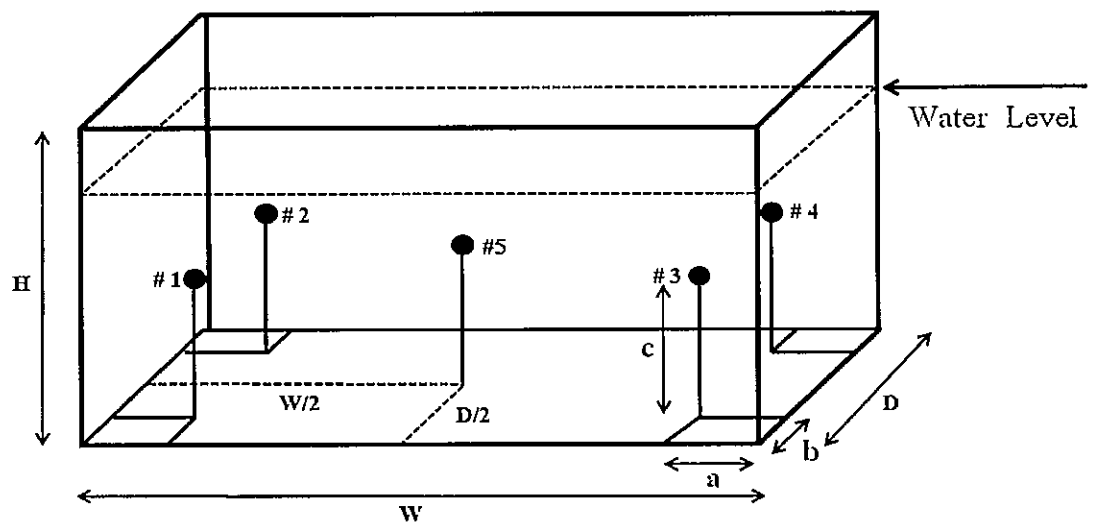

Sensor Installation Details

$a = 5 \text{ cm}$
 $b = 5 \text{ cm}$
 $c = 5 \text{ cm}$

Dimension of the chamber

$W = 45 \text{ cm}$
 $H = 30 \text{ cm}$
 $D = 35 \text{ cm}$



Certificate No. : 23TH0521

CSR No. : A075/03704

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Water Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (± °C)
	#1	#2	#3	#4	Ref.5	
44.5	44.47	44.48	44.45	44.51	44.50	0.14

3. Performance Result

The performance of the Water Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
44.5	44.5	44.5	0.10	0.24	0.25

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 16-Jul-2023

Certificate No. : 23TH3096

CSR No. : A095/04743

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory
Instrument Name : Incubator
Manufacturer : Memmert
Model : ICP750
Serial No. : F816.0063
ID No. : SGK_CL0028
Resolution : 0.1 °C
Received Date : 13-Jul-2023
Calibrated Date : 13-Jul-2023
Ambient Temperature : (30 ± 10) °C
Relative Humidity : (50 ± 30) %

REVIEW BYAnanta B.....
APPROVED BYKamtha H.....
NEXT CAL. DATE13/01/25.....

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- ScaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	23SDAT004	23-May-2024


2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

1. Sensor Installation Diagram

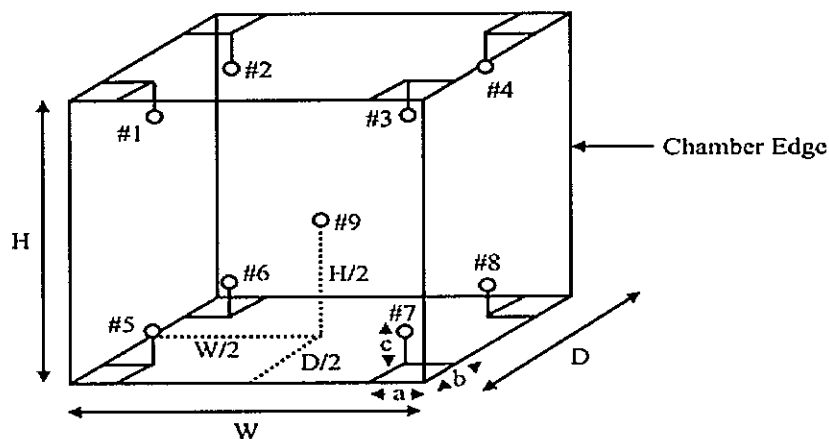

Sensor Installation Details

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of the chamber

W = 40.0 cm
H = 40.0 cm
D = 33.0 cm



Certificate No. : 23TH3096

CSR No. : A095/04743

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Incubator and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
20	20.10	20.04	20.03	19.97	20.08	20.23	20.10	19.94	20.07	0.38

3. Performance Result

The performance of the Incubator are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
20	20.0	20.0	0.14	0.17	0.32

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

... End ...




TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22LM162

Page.: 1 of 2

Certificate of Calibration

Equipment :	DO Meter with Sensor
Manufacturer :	YSI
Model :	5000
Serial No. :	17B101473
ID No. :	SGK_CL0073
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8, Kanjanavanij Rd., Banphru,
Location :	TPA Chemistry Calibration Lab.2
Received Order :	18 November 2022
Calibrated Date :	21 November 2022
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	<div style="text-align: center;"> Approved Signatory</div>
<div style="display: flex; justify-content: space-between;"><div><div><input type="checkbox"/> Pornthippa Tameyakul</div><div><input checked="" type="checkbox"/> Malee Butkruea</div><div><input type="checkbox"/> Suwit Imjai</div></div><div></div></div>	
Issue Date :	22 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0047729



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2111-0663DSC-2

Cert. No.: 22LM162

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1523	3240076	221249	02 Mar 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.


This instrument was connected with temperature sensor, S/N.: 17B100103

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.001	19.88	-0.121	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 22TW259

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000
Serial No. :	17B101473
ID No. :	SGK_CL0073
Received Date :	18 November 2022
Test Date :	21 November 2022
Reference :	2211-0663DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8, Kanjanavanij Rd., Banphru, Hatyai, Songkhla 90250, Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	<div style="text-align: center;"> _____ Approved by</div>
<div>(<input checked="" type="checkbox"/>) Malee Butkruea (<input type="checkbox"/>) Saithip Meangmai (<input type="checkbox"/>) Warakorn Lerngagtrakul</div>	
Issue Date :	22 November 2022



Cert.No.: 22TW259

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 17B100103

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.12	8.12	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-



a 1136621



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI-18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CH553

Page.: 1 of 2

Certificate of Calibration

Equipment :	Conductivity Meter
Manufacturer :	Mettler Toledo
Model :	SevenCompact S230
Serial No. :	B608134488
ID No. :	SGK_CL0032
Condition As-Received:	Used Item
Received Date :	28 April 2023
Calibration Date :	03 May 2023
Reference :	2304-0804DSC-2
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8, Kanjanavanij Rd., Banphru, Hatyai, Songkhla 90250, Thailand
Ambient Temperature :	(25 \pm 2.5) °C
Relative Humidity :	(50 \pm 15) %
Calibration Procedure:	In -house method : - CP-CH6 : based on direct measurement by using certified reference material (CRM)

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	03/05/24

Calibrated by : Warakorn Lerngagtrakul

Approved by :

Approved Signatory

- (✓) Malee Butkruea
() Saithip Meangmai
() Warakorn Lerngagtrakul

Issue Date : 16 May 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0054235



Cert.No.: 23CH553

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	1963878	130RC095	22I1140	12 Sep 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
84.000 $\mu\text{S/cm}$	CPA Chem	823326	20 June 2023
1413.0 $\mu\text{S/cm}$	CPA Chem	826595	09 July 2023

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 1413.0 $\mu\text{S/cm}$

Conductivity Electrode Serial No.: 5816340156

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (\pm)	Coverage factor k
84.000 $\mu\text{S/cm}$	91.0 $\mu\text{S/cm}$	88.4 $\mu\text{S/cm}$	0.62 $\mu\text{S/cm}$	2.00
1413.0 $\mu\text{S/cm}$	1490 $\mu\text{S/cm}$	1414 $\mu\text{S/cm}$	9.2 $\mu\text{S/cm}$	2.00

Remark - UUC* = Unit Under Calibration

- Adjustment Cell constant = 0.101842 cm^{-1}

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



a 1161556

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6 , e-mail: service.thailand@sartorius.com

**SARTORIUS**

Certificate

of Calibration

REVIEW BY

APPROVED BY

NEXT CAL. DATE

Model Number : MSE224S-100-DUDescription : Analytical BalanceSerial Number : 0034705158ID No. : SGK_CL0045Manufacturer : SartoriusCertificate No. : 23BCI0044Issued Date : Friday, January 27, 2023Reference No. : 202361Page No. : 1 of 2Customer Name : ALS Laboratory Group (Thailand) Co., Ltd.Songkhla Branch: 114/1 Moo 8 Karnchanawanich Rd., T. Ban Phru, A. Hat Yai, Songkhla. 90250.Calibrated Place : Balance Room.Calibrated By : Mr. Chonchai InthanaCalibration Date : Wednesday, January 25, 2023

Calibration

Procedure No. : This calibration was conducted byUsing in-house calibration procedure number (WI-003)Based on UKAS LAB 14 : 2019**Metrological data :**Capacity : 220 g Readability : 0.0001 g**Ambients Conditions:**Temperature : 22.4 °C ± 3.0 °CHumidity : 65.0 % RH ± 5.0 % RHPressure : ± **Reasons for calibration**☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ MaintenanceEquipment Condition: ☒ Good Operate ☐ Fair**Measurement Method UKAS Publication Ref :Lab 14**

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 1kg E2 s/n 37929119	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division
Sartorius (Thailand) Co., Ltd.

SOP FM 33 03 February 2022

Mr. Chonchai Inthana (Technical Manager)

S
T
A
M
P

Certificate of Calibration

Model Number : MSE224S-100-DU

Certificate No. : 23BCI0044

Description : Analytical Balance

Issued Date : Friday, January 27, 2023

Serial Number : 0034705158

Reference No. : 202361

ID No. SGK_CL0045

Manufacturer : Sartorius

Page No. : 2 of 2

Calibration Results : Without Adjustment

Repeatability



The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0001	200.0000
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0000
	20.0000	200.0001
Nominal Value : (High Load)	20.0000	200.0000
200 g	20.0000	200.0001
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0001
	20.0000	200.0001
Standard Deviation	0.00003	0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 50 g
Tolerance 0.0004 g



	Difference
1	—
2	0.0001
3	0.0000
4	0.0000
5	0.0000
6	—

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00013
0.1	0.1000	0.1000	0.0000	0.00013
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	200.0001	0.0001	0.00030

End of Report.



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 1-May-2023

Certificate No. : 23TH1728

CSR No. : A088/04367

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : Hot Air Oven

Manufacturer : Memmert

Model : UF110

Serial No. : B416.3387

ID No. : SGK_CL0024

Resolution : 0.1 °C

Received Date : 28-Apr-2023

Calibrated Date : 28-Apr-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY

APPROVED BY

NEXT CAL. DATE

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

(☒) Without Adjustment

(☐) After Adjustment

1. Sensor Installation Diagram

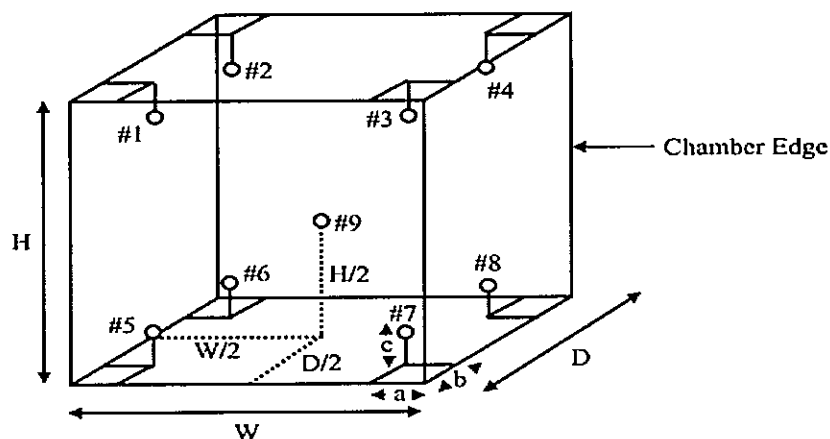

Sensor Installation Details

a = 5.0 cm

b = 5.0 cm

c = 5.0 cm

Dimension of the chamber

W = 40.0 cm

H = 40.0 cm

D = 33.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Hot Air Oven and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
40	40.48	40.28	40.28	39.91	40.17	40.09	39.93	40.27	39.89	0.36
70	70.36	70.23	70.58	69.74	69.99	69.92	69.86	70.13	70.04	0.36
103	103.19	103.12	103.46	103.37	103.10	103.54	103.43	103.06	103.40	0.36
104	104.31	104.23	104.62	103.77	104.12	104.06	103.90	104.20	104.56	0.36
105	105.07	105.03	105.48	105.27	105.12	105.01	105.01	105.00	104.96	0.36
180	180.31	180.00	180.00	180.07	180.18	180.05	180.01	180.10	180.24	0.41

3. Performance Result

The performance of the Hot Air Oven are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
40	40.0	40.0	0.20	0.70	0.72
70	70.0	70.0	0.20	0.60	0.94
103	103.0	103.0	0.20	0.43	0.54
104	104.0	104.0	0.10	0.79	0.88
105	105.0	105.0	0.10	0.59	0.69
180	180.0	180.0	0.10	0.38	0.38

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 16-Jul-2023

Certificate No. : 23TH3097

CSR No. : A095/04743

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : Water Bath

Manufacturer : Memmert

Model : WNE29

Serial No. : L616.0538

ID No. : SGK_CL0035

Resolution : 0.1 °C

Received Date : 13-Jul-2023

Calibrated Date : 13-Jul-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY Ananta B.

APPROVED BY Kanitha B.

NEXT CAL. DATE 13/01/25

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.014 based on ASTM E 715 : 1980
(reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement
according to the International System of Unit (SI) through :

- ScaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	23SDAT004	23-May-2024

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration .:

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

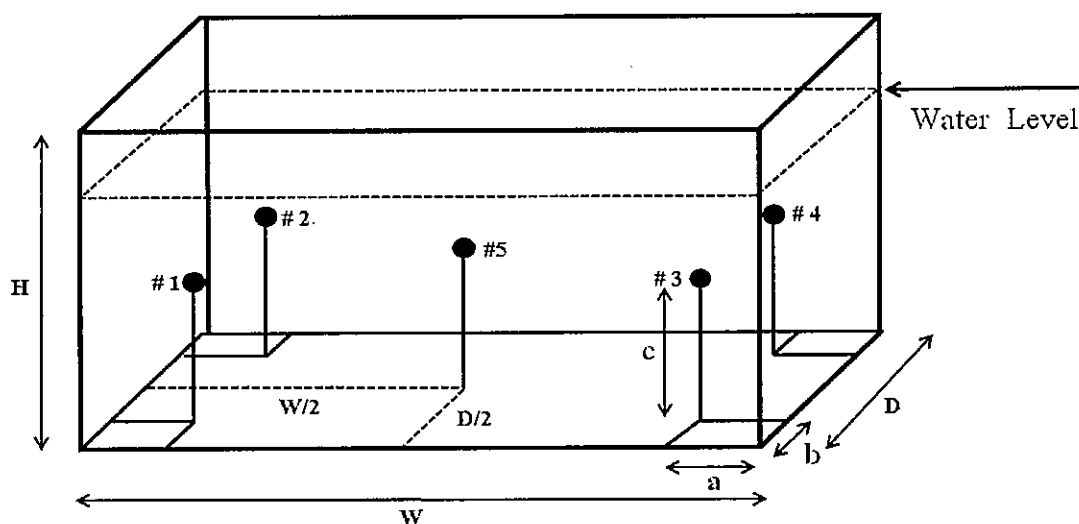

Sensor Installation Details

a = 5 cm
b = 5 cm
c = 5 cm

Dimension of the chamber

W = 45 cm
H = 30 cm
D = 35 cm



Certificate No. : 23TH3097

CSR No. : A095/04743

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Water Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (± °C)
	#1	#2	#3	#4	Ref.5	
80	79.17	79.47	79.43	79.25	79.38	0.14

3. Performance Result

The performance of the Water Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
80	80.0	80.0	0.24	0.38	0.38

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.seal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 1-May-2023

Certificate No. : 23CH0203

CSR No. : A088/04367

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : pH meter

Manufacturer : Mettler Toledo

Model : S220

Serial No. : B625631849

ID No. : SGK_CL0030

Electrode No. : 1204613

Received Date : 28-Apr-2023

Calibrated Date : 28-Apr-2023

Ambient Temperature : (25 ± 3) °C

Relative Humidity : (55 ± 15) %

REVIEW BY

APPROVED BY

NEXT CAL. DATE

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HACH : HACH LANGE GmbH

- SCaL : Sounthern Calibration Service Co., Ltd.,

- WK : WK Electric Co., Ltd.

Calibrated by : Alisara Ma

Approved by :

Imron Rattanayum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.



Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.005	C02994	1777	5-Sep-2024
Standard Solution	7.000	C03007	1787	17-Oct-2024
Standard Solution	10.012	C02953	1735	29-Apr-2024
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	5-Jun-2024
Digital Thermometer With Sensor	DP-77	I.360896	22SDTH005	8-Aug-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading		Correction (mV)	Uncertainty (± mV)
	(mV)	(pH)		
177.48	177.5	3.70	-0.02	0.17
0.00	0.0	6.70	0.00	0.13
-177.48	-177.4	9.80	-0.08	0.17

2. Before Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.005	3.97	159.2	0.035	0.0090
6.999	6.98	-15.4	0.019	0.013
10.012	9.95	-188.0	0.062	0.036

3. After Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.005	3.97	158.9	0.035	0.0090
6.999	7.01	-17.5	-0.011	0.013
10.012	9.98	-187.6	0.032	0.036

4. Temperature Measurement

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25	25.032	25.1	-0.068	0.11

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 23T1030

Page : 1 of 2

Equipment : Digital Thermometer With Sensor

Manufacturer: Testo

Model : 106

Serial No.: 51164837/812

ID No.: SRT_FS0018

Condition As-Received: Used Item

Received Date: 02 June 2023

Calibration Date: 08 June 2023
to 12 June 2023

Reference: 2306-0076DSC

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Procedure used: Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with Platinum Resistance Thermometer (PRT) and Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Digital Thermometer	1529-R	B19520	22I835	11 Jul 2023
2) Platinum Resistance Thermometer	935-14-95	261589/2	22I835	11 Jul 2023
3) Digital Thermometer	1529	A7A609	22I1274	17 Oct 2023
4) Industrial Platinum Resistance Thermometer	5627	824304	22I1274	17 Oct 2023

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)



Calibrated by : Sataporn Mulkamdee
Issue Date : 13 June 2023

Approved Signatory :

[] Phalinee Prabpaipal
[] Chatchawan Khunpiluek
[✓] Wanlop Larperkern

B 0316440



Cert. No.: 23T1030

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Temperature measurement

Dimension of probe : Diameter 3 mm., Length 55 mm. Sheath material : Stainless Steel

Immersion Depth (mm.)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
50	25.0012	25.0	-0.0012	0.12
50	30.0062	29.9	-0.1062	0.12
50	40.0089	40.0	-0.0089	0.12

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

-o0o-



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.seal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 1-May-2023

Certificate No. : 23CH0203

CSR No. : A088/04367

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : pH meter

Manufacturer : Mettler Toledo

Model : S220

Serial No. : B625631849

ID No. : SGK_CL0030

Electrode No. : 1204613

Received Date : 28-Apr-2023

Calibrated Date : 28-Apr-2023

Ambient Temperature : (25 ± 3) °C

Relative Humidity : (55 ± 15) %

REVIEW BY

APPROVED BY

NEXT CAL. DATE

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HACH : HACH LANGE GmbH

- SCaL : Sounthern Calibration Service Co., Ltd.,

- WK : WK Electric Co., Ltd.

Calibrated by : Alisara Ma

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.



Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.005	C02994	1777	5-Sep-2024
Standard Solution	7.000	C03007	1787	17-Oct-2024
Standard Solution	10.012	C02953	1735	29-Apr-2024
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	5-Jun-2024
Digital Thermometer With Sensor	DP-77	I.360896	22SDTH005	8-Aug-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading		Correction (mV)	Uncertainty (± mV)
	(mV)	(pH)		
177.48	177.5	3.70	-0.02	0.17
0.00	0.0	6.70	0.00	0.13
-177.48	-177.4	9.80	-0.08	0.17

2. Before Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.005	3.97	159.2	0.035	0.0090
6.999	6.98	-15.4	0.019	0.013
10.012	9.95	-188.0	0.062	0.036

3. After Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.005	3.97	158.9	0.035	0.0090
6.999	7.01	-17.5	-0.011	0.013
10.012	9.98	-187.6	0.032	0.036

4. Temperature Measurement

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25	25.032	25.1	-0.068	0.11

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Internal Calibration

REVIEW BY .	
APPROVED BY	
NEXT CAL. DATE	

Equipment :	<u>Turbidity Meter</u>	Manufacture :	<u>HACH</u>
ID No. :	<u>SGK_FS0045</u>	Model :	<u>2100Q/QIS</u>
Calibrate Date :	<u>May22 ,2023</u>	Serial No. :	<u>19010C073443</u>

Calibration Point	1st (NTU)	2nd (NTU)	3rd (NTU)	AVG (NTU)	Specifications	Evaluate
Standard 20 NTU	20.1	20.0	20.0	20.0	19 to 21 NTU	Pass
Standard 100 NTU	101.0	101.0	101.0	101.0	95 to 105 NTU	Pass
Standard 800 NTU	799.0	800.0	800.1	799.7	760 to 840 NTU	Pass

Calibrated by Somsak J.
(Scientist 2)

Approved by : Kanitta H.
(Section head)

PC 14/02/13

HACH COMPANY



An ISO 9001 Certified Company

P.O.Box 389
Loveland, CO 80539
(970) 669-3050

Certificate of Analysis

This is a Component of 2659405--TH lot A2307

Page 1

COMMODITY: STABLCAL|sup|TS|sup0 FORMAZIN STANDARD 20 NTU
COMMODITY NUMBER: 2684801 MANUFACTURE DATE: DATE OF ANALYSIS:
LOT NUMBER: A2304 11/14/2022 11/18/2022

<i>TEST</i>	<i>SPECIFICATIONS</i>	<i>RESULTS</i>
Turbidity	19 to 21 NTU	20.3 NTU

The expiration date is Feb 2024

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NIST does not carry turbidity standards. However, the use of Formazin and StablCal® as used in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

Certified by



Scott Als
Analytical Services Chemist

fe 17/02/23

HACH COMPANY



An ISO 9001 Certified Company

P.O.Box 389
Loveland, CO 80539
(970) 669-3050

Certificate of Analysis

This is a Component of 2659405-TH lot A2307

Page 1

COMMODITY: STABLCAL|sup|TS|sup0 FORMAZIN STANDARD 100 NTU
COMMODITY NUMBER: 2684901 MANUFACTURE DATE: DATE OF ANALYSIS:
LOT NUMBER: A2299 11/10/2022 11/17/2022

<i>TEST</i>	<i>SPECIFICATIONS</i>	<i>RESULTS</i>
Turbidity	95 to 105 NTU	102.0 NTU

The expiration date is Feb 2024

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NIST does not carry turbidity standards. However, the use of Formazin and StablCal® as used in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

Certified by



Scott Als
Analytical Services Chemist

PC 17/02/2

HACH COMPANY



An ISO 9001 Certified Company

P.O.Box 389
Loveland, CO 80539
(970) 669-3050

Certificate of Analysis

This is a Component of 2659405-TH lot A2307

Page 1

COMMODITY: STABLCAL|sup|TS|sup0 FORMAZIN STANDARD 800 NTU
COMMODITY NUMBER: 2660501 MANUFACTURE DATE: DATE OF ANALYSIS:
LOT NUMBER: A2318 11/29/2022 12/5/2022

<i>TEST</i>	<i>SPECIFICATIONS</i>	<i>RESULTS</i>
Turbidity	760 to 840 NTU	817.0 NTU

The expiration date is Feb 2024

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NIST does not carry turbidity standards. However, the use of Formazin and StablCal® as used in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

Certified by



Scott Als
Analytical Services Chemist



REVIEW BY ...

APPROVED BY

NEXT CAL. DATE

Certificate of Calibration

ICS-2100: Anion (ID#659)

This certificate is to verify that instrument below are calibrated
by Archemica Lab Co., Ltd.

ICS-2100 S/N: 15010977

AS-HV S/N: 5450A36659

For

ALS Laboratory Group (Thailand) Co., Ltd.



Operator Signature: _____

Date: Jan 12, 2023

(Mr.Nutdanai Laekhwan)

Application Chemist