

ภาคผนวก ค เอกสารสอบเทียบความถูกต้อง
ของเครื่องมือเก็บตัวอย่าง

ANALYTICAL BALANCE

Model : MS204TS/00

Serial No. : B904136539

Mettler-Toledo (Thailand) Ltd.
846/4 - 846/5 Lasalle Rd., Bangna Tai Sub-District
Bangna District, Bangkok 10260
+662 723 0382
MT-TH.ServiceSupport@mt.com

Accuracy Calibration Certificate

Customer

Company: EASTERN THAI CONSULTING 1992 CO., LTD.
Address: 683 Moo 11, Sukhaphiban 8 Rd., Nong Kham
City: Sriracha
Zip / Postal: 20230
State / Province: Chonburi
Contact: Sasiporn Nakin
Order Number: 0352630077

Weighing Device

Manufacturer: Mettler Toledo
Model: MS204TS000
Serial No.: B904136539
Building: Laboratory
Floor: 1
Room: Balance
Instrument Type: Weighing Instrument
Asset Number: LABE 05/4
Terminal Model: N/A
Terminal Serial No.: N/A
Terminal Asset No.: N/A

Range	Max. Capacity	Repeatability (g)
1	220 g	0.0001 g

Procedure

Calibration Guideline: EURAMET cg-18 v. 4.0 (11/2015)
CPW002/20
METTLER TOLEDO Work Instruction:
This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.
The sensitivity/span of the weighing instrument was adjusted before calibration with a built-in weight.
In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

As Found	Start: 25.6 °C	End: 25.2 °C	Start: 50.5 %	End: 44.6 %
Temperature				
Humidity				

As Found Calibration Date: 06-Feb-2023
As Left Calibration Date: N/A
Issue Date: 07-Feb-2023
Calibrator: Thiraphong Salanoi
Approved Signatory: [Signature]

Technical Manager / Head of Calibration Center

COPY


Measurement Results

Repeatability

Test Load: 100 g

	As Found	As Left
1	100.0002 g	N/A
2	100.0002 g	N/A
3	100.0001 g	N/A
4	100.0002 g	N/A
5	100.0002 g	N/A
6	100.0001 g	N/A
7	100.0002 g	N/A
8	100.0002 g	N/A
9	100.0001 g	N/A
10	100.0002 g	N/A

Standard Deviation	0.00005 g	N/A
--------------------	-----------	-----

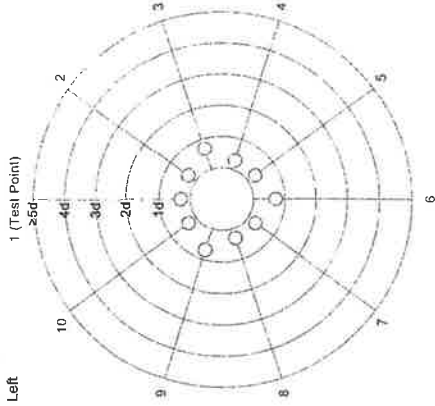


The "d" in the graph represents the repeatability of the range/interval in which the test was performed.
The results of this graph are based upon the absolute values of the differences from the mean value.

Eccentricity

Test Load: 100 g

Position	As Found	As Left
1	100.0002 g	N/A
2	100.0002 g	N/A
3	100.0001 g	N/A
4	100.0001 g	N/A
5	100.0001 g	N/A

Maximum Deviation	0.0001 g	N/A
-------------------	----------	-----




As Found

The "d" in the graph represents the repeatability of the range/interval in which the test was performed.

COPY

Error of Indication

As Found	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.0000 g	0.0000 g	0.0000 g	0.11 mg	2
2	0.0100 g	0.0100 g	0.0000 g	0.13 mg	2
3	0.0500 g	0.0500 g	0.0000 g	0.13 mg	2
4	0.1000 g	0.0999 g	-0.0001 g	0.13 mg	2
5	1.0000 g	0.9999 g	-0.0001 g	0.13 mg	2
6	5.0000 g	4.9999 g	-0.0001 g	0.13 mg	2
7	10.0000 g	9.9999 g	-0.0001 g	0.14 mg	2
8	50.0000 g	50.0001 g	0.0001 g	0.17 mg	2
9	100.0001 g	100.0002 g	0.0001 g	0.24 mg	2
10	150.0001 g	150.0002 g	0.0001 g	0.34 mg	2
11	200.0001 g	200.0002 g	0.0001 g	0.39 mg	2

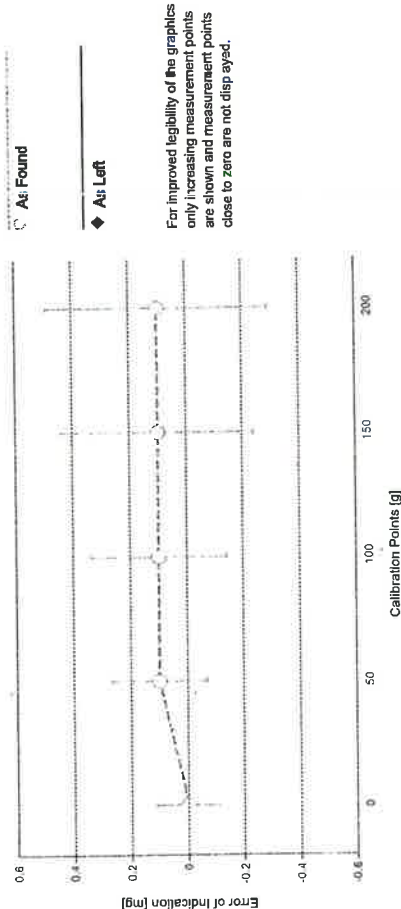

The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor k – which can be larger than 2 according to EURAMET cg-18. The value of the measurand lies within the assigned range of values with a probability of approximately 95 %.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2
Weight Set No.: WS28
Certificate Number: 178498
Date of Issue: 01-Apr-2022
Calibration Due Date: 17-Sep-2023

Thermo Hygrometer
Equipment No.: IN306
Certificate Number: 23H4
Date of Issue: 10-Jan-2023
Calibration Due Date: 03-Jan-2024

COPY

Remarks

FACT adjustment functionality activated
Equipment condition: Good
Next calibration according to customer's procedure
Calibration data not decide by calibration laboratory

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

COPY

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with $k=2$ in use. The formula shall be used for the estimation of the uncertainty under consideration of the error of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use:	$1.5 \cdot 10^{-6} / \text{K}$
Temperature measurement uncertainty in use:	5 K


Linearization of Uncertainty Equation

Linearization of Uncertainty Equation			As Found	As Left
Range				
	d	Max		
1	0.0001 g	220 g	$U_1 = 0.13 \text{ mg} + 0.00625 \text{ mg/g} \cdot R$	N/A

To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement | Uncertainty in Use for Various Net Indications (Examples)

	As Found	As Left
Net indication		
0.0220 g	0.13 mg	N/A
0.2200 g	0.13 mg	N/A
2.2000 g	0.14 mg	N/A
22.0000 g	0.27 mg	N/A
220.0000 g	1.5 mg	N/A

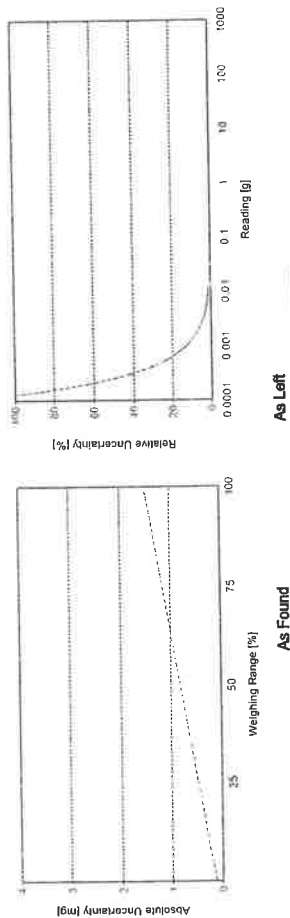

DO NOT

GWP®
Certificate



As Found	As Left
✓	

The weighing device meets the given process requirements.

The weighing device meets the given process requirements.

Tests Performed:	As Found
<p>1. Visual Inspection</p> <p>2. Moisture Content</p> <p>3. Specific Gravity</p> <p>4. Proctor Compaction</p> <p>5. Liquid Limit</p> <p>6. Plastic Limit</p> <p>7. Shrinkage</p> <p>8. Strength</p> <p>9. Durability</p> <p>10. Permeability</p> <p>11. Swell</p> <p>12. Settlement</p> <p>13. Frost Resistance</p> <p>14. Fire Resistance</p> <p>15. Acid Resistance</p> <p>16. Alkali Resistance</p> <p>17. Sulfate Resistance</p> <p>18. Chloride Resistance</p> <p>19. Carbonation</p> <p>20. Rebar Corrosion</p> <p>21. Concrete Cover</p> <p>22. Rebar Spacing</p> <p>23. Rebar Diameter</p> <p>24. Rebar Lap</p> <p>25. Rebar Tie</p> <p>26. Rebar Bend</p> <p>27. Rebar Weld</p> <p>28. Rebar Protection</p> <p>29. Rebar Embedment</p> <p>30. Rebar Anchorage</p> <p>31. Rebar Development</p> <p>32. Rebar Splicing</p> <p>33. Rebar Lapping</p> <p>34. Rebar Tying</p> <p>35. Rebar Bending</p> <p>36. Rebar Welding</p> <p>37. Rebar Protection</p> <p>38. Rebar Embedment</p> <p>39. Rebar Anchorage</p> <p>40. Rebar Development</p> <p>41. Rebar Splicing</p> <p>42. Rebar Lapping</p> <p>43. Rebar Tying</p> <p>44. Rebar Bending</p> <p>45. Rebar Welding</p> <p>46. Rebar Protection</p> <p>47. Rebar Embedment</p> <p>48. Rebar Anchorage</p> <p>49. Rebar Development</p> <p>50. Rebar Splicing</p> <p>51. Rebar Lapping</p> <p>52. Rebar Tying</p> <p>53. Rebar Bending</p> <p>54. Rebar Welding</p> <p>55. Rebar Protection</p> <p>56. Rebar Embedment</p> <p>57. Rebar Anchorage</p> <p>58. Rebar Development</p> <p>59. Rebar Splicing</p> <p>60. Rebar Lapping</p> <p>61. Rebar Tying</p> <p>62. Rebar Bending</p> <p>63. Rebar Welding</p> <p>64. Rebar Protection</p> <p>65. Rebar Embedment</p> <p>66. Rebar Anchorage</p> <p>67. Rebar Development</p> <p>68. Rebar Splicing</p> <p>69. Rebar Lapping</p> <p>70. Rebar Tying</p> <p>71. Rebar Bending</p> <p>72. Rebar Welding</p> <p>73. Rebar Protection</p> <p>74. Rebar Embedment</p> <p>75. Rebar Anchorage</p> <p>76. Rebar Development</p> <p>77. Rebar Splicing</p> <p>78. Rebar Lapping</p> <p>79. Rebar Tying</p> <p>80. Rebar Bending</p> <p>81. Rebar Welding</p> <p>82. Rebar Protection</p> <p>83. Rebar Embedment</p> <p>84. Rebar Anchorage</p> <p>85. Rebar Development</p> <p>86. Rebar Splicing</p> <p>87. Rebar Lapping</p> <p>88. Rebar Tying</p> <p>89. Rebar Bending</p> <p>90. Rebar Welding</p> <p>91. Rebar Protection</p> <p>92. Rebar Embedment</p> <p>93. Rebar Anchorage</p> <p>94. Rebar Development</p> <p>95. Rebar Splicing</p> <p>96. Rebar Lapping</p> <p>97. Rebar Tying</p> <p>98. Rebar Bending</p> <p>99. Rebar Welding</p> <p>100. Rebar Protection</p> <p>101. Rebar Embedment</p> <p>102. Rebar Anchorage</p> <p>103. Rebar Development</p> <p>104. Rebar Splicing</p> <p>105. Rebar Lapping</p> <p>106. Rebar Tying</p> <p>107. Rebar Bending</p> <p>108. Rebar Welding</p> <p>109. Rebar Protection</p> <p>110. Rebar Embedment</p> <p>111. Rebar Anchorage</p> <p>112. Rebar Development</p> <p>113. Rebar Splicing</p> <p>114. Rebar Lapping</p> <p>115. Rebar Tying</p> <p>116. Rebar Bending</p> <p>117. Rebar Welding</p> <p>118. Rebar Protection</p> <p>119. Rebar Embedment</p> <p>120. Rebar Anchorage</p> <p>121. Rebar Development</p> <p>122. Rebar Splicing</p> <p>123. Rebar Lapping</p> <p>124. Rebar Tying</p> <p>125. Rebar Bending</p> <p>126. Rebar Welding</p> <p>127. Rebar Protection</p> <p>128. Rebar Embedment</p> <p>129. Rebar Anchorage</p> <p>130. Rebar Development</p> <p>131. Rebar Splicing</p> <p>132. Rebar Lapping</p> <p>133. Rebar Tying</p> <p>134. Rebar Bending</p> <p>135. Rebar Welding</p> <p>136. Rebar Protection</p> <p>137. Rebar Embedment</p> <p>138. Rebar Anchorage</p> <p>139. Rebar Development</p> <p>140. Rebar Splicing</p> <p>141. Rebar Lapping</p> <p>142. Rebar Tying</p> <p>143. Rebar Bending</p> <p>144. Rebar Welding</p> <p>145. Rebar Protection</p> <p>146. Rebar Embedment</p> <p>147. Rebar Anchorage</p> <p>148. Rebar Development</p> <p>149. Rebar Splicing</p> <p>150. Rebar Lapping</p> <p>151. Rebar Tying</p> <p>152. Rebar Bending</p> <p>153. Rebar Welding</p> <p>154. Rebar Protection</p> <p>155. Rebar Embedment</p> <p>156. Rebar Anchorage</p> <p>157. Rebar Development</p> <p>158. Rebar Splicing</p> <p>159. Rebar Lapping</p> <p>160. Rebar Tying</p> <p>161. Rebar Bending</p> <p>162. Rebar Welding</p> <p>163. Rebar Protection</p> <p>164. Rebar Embedment</p> <p>165. Rebar Anchorage</p> <p>166. Rebar Development</p> <p>167. Rebar Splicing</p> <p>168. Rebar Lapping</p> <p>169. Rebar Tying</p> <p>170. Rebar Bending</p> <p>171. Rebar Welding</p> <p>172. Rebar Protection</p> <p>173. Rebar Embedment</p> <p>174. Rebar Anchorage</p> <p>175. Rebar Development</p> <p>176. Rebar Splicing</p> <p>177. Rebar Lapping</p> <p>178. Rebar Tying</p> <p>179. Rebar Bending</p> <p>180. Rebar Welding</p> <p>181. Rebar Protection</p> <p>182. Rebar Embedment</p> <p>183. Rebar Anchorage</p> <p>184. Rebar Development</p> <p>185. Rebar Splicing</p> <p>186. Rebar Lapping</p> <p>187. Rebar Tying</p> <p>188. Rebar Bending</p> <p>189. Rebar Welding</p> <p>190. Rebar Protection</p> <p>191. Rebar Embedment</p> <p>192. Rebar Anchorage</p> <p>193. Rebar Development</p> <p>194. Rebar Splicing</p> <p>195. Rebar Lapping</p> <p>196. Rebar Tying</p> <p>197. Rebar Bending</p> <p>198. Rebar Welding</p> <p>199. Rebar Protection</p> <p>200. Rebar Embedment</p> <p>201. Rebar Anchorage</p> <p>202. Rebar Development</p> <p>203. Rebar Splicing</p> <p>204. Rebar Lapping</p> <p>205. Rebar Tying</p> <p>206. Rebar Bending</p> <p>207. Rebar Welding</p> <p>208. Rebar Protection</p> <p>209. Rebar Embedment</p> <p>210. Rebar Anchorage</p> <p>211. Rebar Development</p> <p>212. Rebar Splicing</p> <p>213. Rebar Lapping</p> <p>214. Rebar Tying</p> <p>215. Rebar Bending</p> <p>216. Rebar Welding</p> <p>217. Rebar Protection</p> <p>218. Rebar Embedment</p> <p>219. Rebar Anchorage</p> <p>220. Rebar Development</p> <p>221. Rebar Splicing</p> <p>222. Rebar Lapping</p> <p>223. Rebar Tying</p> <p>224. Rebar Bending</p> <p>225. Rebar Welding</p> <p>226. Rebar Protection</p> <p>227. Rebar Embedment</p> <p>228. Rebar Anchorage</p> <p>229. Rebar Development</p> <p>230. Rebar Splicing</p> <p>231. Rebar Lapping</p> <p>232. Rebar Tying</p> <p>233. Rebar Bending</p> <p>234. Rebar Welding</p> <p>235. Rebar Protection</p> <p>236. Rebar Embedment</p> <p>237. Rebar Anchorage</p> <p>238. Rebar Development</p> <p>239. Rebar Splicing</p> <p>240. Rebar Lapping</p> <p>241. Rebar Tying</p> <p>242. Rebar Bending</p> <p>243. Rebar Welding</p> <p>244. Rebar Protection</p> <p>245. Rebar Embedment</p> <p>246. Rebar Anchorage</p> <p>247. Rebar Development</p> <p>248. Rebar Splicing</p> <p>249. Rebar Lapping</p> <p>250. Rebar Tying</p> <p>251. Rebar Bending</p> <p>252. Rebar Welding</p> <p>253. Rebar Protection</p> <p>254. Rebar Embedment</p> <p>255. Rebar Anchorage</p> <p>256. Rebar Development</p> <p>257. Rebar Splicing</p> <p>258. Rebar Lapping</p> <p>259. Rebar Tying</p> <p>260. Rebar Bending</p> <p>261. Rebar Welding</p> <p>262. Rebar Protection</p> <p>263. Rebar Embedment</p> <p>264. Rebar Anchorage</p> <p>265. Rebar Development</p> <p>266. Rebar Splicing</p> <p>267. Rebar Lapping</p> <p>268. Rebar Tying</p> <p>269. Rebar Bending</p> <p>270. Rebar Welding</p> <p>271. Rebar Protection</p> <p>272. Rebar Embedment</p> <p>273. Rebar Anchorage</p> <p>274. Rebar Development</p> <p>275. Rebar Splicing</p> <p>276. Rebar Lapping</p> <p>277. Rebar Tying</p> <p>278. Rebar Bending</p> <p>279. Rebar Welding</p> <p>280. Rebar Protection</p> <p>281. Rebar Embedment</p> <p>282. Rebar Anchorage</p> <p>283. Rebar Development</p> <p>284. Rebar Splicing</p> <p>285. Rebar Lapping</p> <p>286. Rebar Tying</p> <p>287. Rebar Bending</p> <p>288. Rebar Welding</p> <p>289. Rebar Protection</p> <p>290. Rebar Embedment</p> <p>291. Rebar Anchorage</p> <p>292. Rebar Development</p> <p>293. Rebar Splicing</p> <p>294. Rebar Lapping</p> <p>295. Rebar Tying</p> <p>296. Rebar Bending</p> <p>297. Rebar Welding</p> <p>298. Rebar Protection</p> <p>299. Rebar Embedment</p> <p>300. Rebar Anchorage</p> <p>301. Rebar Development</p> <p>302. Rebar Splicing</p> <p>303. Rebar Lapping</p> <p>304. Rebar Tying</p>	

☐ As Left

No adjustments/modifications made. As Left results correspond to As Found.


Process Requirements

Weighing Tolerance: 1%

Smallest Net Weight: 1.0000 g

Safety Factor: 2

Safe Weighing Range

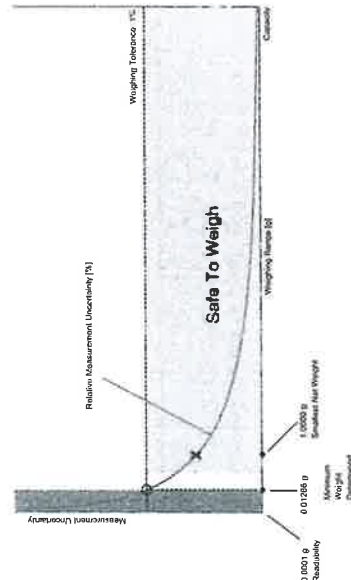

While the values in this graph reflect the actual calibration results, the measurement uncertainty curves are simply a visual representation. This graph reflects As Left testing, unless only As Found were performed.

Dr. [Signature]

Measurement Results
 Results Summary

Repeatability		Eccentricity		Error of Indication	
As Found	As Left	As Found	As Left	As Found	As Left
✓	✓	✓	✓	✓	✓

✓ = Passed
 ✗ = Failed
 A = Safety Factor not met

Repeatability

Test Load: 100 g

Tolerance		Control Limit		As Found		As Left	
				Std. Deviation	Result	Std. Deviation	Result
0.1%		0.00050 g			✓		✓
0.2%		0.00100 g			✓		✓
0.5%		0.00250 g			✓		✓
1%		0.00500 g	0.00005 g		✓	0.00005 g	✓
2%		0.01000 g			✓		✓
5%		0.02500 g			✓		✓

The weighing tolerance is met if the standard deviation is less than or equal to the corresponding control limit.

Eccentricity

Test Load: 100 g

Tolerance		Control Limit		As Found		As Left	
				Deviation	Result	Deviation	Result
0.1%		0.0500 g			✓		✓
0.2%		0.1000 g			✓		✓
0.5%		0.2500 g			✓		✓
1%		0.5000 g	0.0001 g		✓	0.0001 g	✓
2%		1.0000 g			✓		✓
5%		2.5000 g			✓		✓

The weighing tolerance is met if the deviation is less than or equal to the corresponding control limit.

Minimum Weight
 As Found Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Safety Factor					
Tolerance	1	2	3	5	10
0.1%	0.12729 g	0.25618 g	0.38672 g	0.65284 g	1.34917 g
0.2%	0.06344 g	0.12729 g	0.19153 g	0.32124 g	0.65284 g
0.5%	0.02533 g	0.05072 g	0.07618 g	0.12729 g	0.25618 g
1%	0.01266 g	0.02533 g	0.03802 g	0.06344 g	0.12729 g
2%	0.00633 g	0.01266 g	0.01899 g	0.03167 g	0.06344 g
5%	0.00253 g	0.00506 g	0.00759 g	0.01266 g	0.02533 g

Pass: The determined minimum weight meets the requirement for the smallest net weight.

As Left Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Safety Factor					
Tolerance	1	2	3	5	10
0.1%	0.12729 g	0.25618 g	0.38672 g	0.65284 g	1.34917 g
0.2%	0.06344 g	0.12729 g	0.19153 g	0.32124 g	0.65284 g
0.5%	0.02533 g	0.05072 g	0.07618 g	0.12729 g	0.25618 g
1%	0.01266 g	0.02533 g	0.03802 g	0.06344 g	0.12729 g
2%	0.00633 g	0.01266 g	0.01899 g	0.03167 g	0.06344 g
5%	0.00253 g	0.00506 g	0.00759 g	0.01266 g	0.02533 g

Pass: The determined minimum weight meets the requirement for the smallest net weight.

At these net minimum weight values, the measurement uncertainty of the weighing device is equal to or less than 1/1 (no safety factor), 1/2, 1/3, 1/5, or 1/10 of the required tolerance. The values are calculated with k = 2 and based on the linear formula of the measurement uncertainty of the weighing device in use.

The safety factor for As Found is always 1. This implies no safety factor. As Found testing looks at the behavior of the instrument from the past until test occurred. For the past, it is necessary to know that the tolerance was met, but not the safety factor. The safety factor is a proactive measure to apply for future measurements.

Notes on minimum weight values in above table:

- If "N/A" is shown above, no appropriate value could be calculated.
- METTLER TOLEDO is not responsible for the definition of the process requirements.

COPY

Error of Indication

As Found

Reference Value		Control limits for various weighing tolerances						
		Error	0.1%	0.2%	0.5%	1%	2%	5%
0.0000 g	0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A
50.0000 g	0.0001 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g	2.5000 g
100.0001 g	0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g	5.0000 g
150.0001 g	0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g	7.5000 g
200.0001 g	0.0001 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g	10.0000 g
Result		✓	✓	✓	✓	✓	✓	✓

As Left

Reference Value		Control limits for various weighing tolerances						
		Error	0.1%	0.2%	0.5%	1%	2%	5%
0.0000 g	0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A
50.0000 g	0.0001 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g	2.5000 g
100.0001 g	0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g	5.0000 g
150.0001 g	0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g	7.5000 g
200.0001 g	0.0001 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g	10.0000 g
Result		✓	✓	✓	✓	✓	✓	✓

The weighing tolerance is met if the error (of indication) for each test point is less than or equal to the corresponding control limit for that particular weighing tolerance. Results at or close to the zero point cannot be assessed.

COPY

BAROMETER

Equipment : Analog Barometer

ID No. / Tag No. : BM001/41



CALIBRATION CERTIFICATE

Certificate No. : L202305085-002
 Date Issued : 16-May-23

Customer : Eastern Thai Consulting 1992 Co., Ltd.
 683 Moo 11 Sukhapibam 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment : Analog Barometer

Manufacturer : Barigo
Model : -
Serial No. : -
ID No./Tag No. : BM001/41
Date Received : 11-May-23
Date Calibrated : 15-May-23

Calibrated by : Mr. Jame Khaothong

Calibration Method or Calibration Procedure Used

In-house method : CP-21 base on DKD-R 6-1: Edition 3 2014.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: *Sorayuth*
 (Mr. Sarayuth Tochua)



Page 1 of 2

COPY

Certificate No. : L202305085-002
Environment : Ambient Temperature : (25 ± 2)°C
 Relative Humidity : (50 ± 15)%RH

STD Reading mbar	UUC Reading (mbar) Before Adjusted	UUC Reading (mbar) After Adjusted	UUC Error mbar	Uncertainty ± mbar
990.00	990.0	-	0.00	0.61
1000.00	1000.0	-	0.00	0.61
1010.00	1010.0	-	0.00	0.61
1020.00	1020.0	-	0.00	0.61
1030.00	1030.0	-	0.00	0.61

STD = Standard

UUC = Unit Under Calibration

Calibrated condition : Pressure Medium : Air : Density = 1.19 kg/m³ @ 20°C, 1 bar
 Mounting Position : Vertical
 Reference Level : at center of its dial
 Conversion Factor : Multiply by 1.0 E+02 - Pa unit

Description of UUC :

Range : 990 - 1030 mbar Absolute
 Calibration Range : 990 - 1030 mbar Absolute
 Scale Interval : 1 mbar
 Resolution : 0.5 mbar Absolute

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

IRPC Certificate No. CL1-P220104 for Reference Pressure Monitor Serial No. 1598, Due 11-Nov-23

End of Certificate

Page 2 of 2

COPY

Hot Air Oven

Model : UFE 500

Serial No. : G511.0182

NSC-TIS1-TIS17025
CALIBRATION 0152

Page 1 of 3

Certificate No. : 23-006679

Sample Code : 23-02820-002

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)
Manufacturer : Memmert
Model : LUBE 17/4
Serial No. : G511.0182
Date of Receipt : 20 January 2023
Date of Calibration : 20 January 2023

Condition of Calibration

1. Environment	1.1 Ambient temperature	±	Maximum	27.9 °C	Minimum	25.3 °C
	1.2 Relative humidity	±	Maximum	50.9 %	Minimum	38.5 %
	1.3 Line voltage supplied	±	Maximum	221.9 VAC	Minimum	218.5 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-P100)	LB-DA-11 (RTD-138 to RTD-146)	22-040309	21 April 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Sarawoot Thammo

Scientist

Issue date

24 January 2023

(Mr. Somchai Neampunt)
Signed for Director

The uncertainties are for a confidence probability of approximately 95%.
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phiabphla, Wang Thonglang, Bangkok 10310
Rev. 01
TEL 02-516-2422
FAX 02-516-6949
Effective Date 15/10/2

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

Effective Date 15/10/2

NSC-TIS1-TIS17025
CALIBRATION 0152

Page 2 of 3

Certificate No. : 23-006679

Sample Code : 23-02820-002

REPORT OF CALIBRATION

Results of Calibration
Resolution : 0.5 °C

1. Reporting of Temperature

Calibration point (°C)	UUC*		Measured temperature at each positions (°C)								Uncertainty ± (°C)	Coverage factor k	
	setting (°C)	reading (°C)	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8			# 9 ^{Ref}
104	103.5	103.5	104.10	104.08	103.87	103.99	104.08	104.08	103.96	104.01	103.84	0.47	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
104.0	0.08	0.32	0.39

Notes

UUC* = Unit Under Calibration

TEL 02-516-2422

FAX 02-516-6949

Rev. 01

361 Soi Ladprao 122, Ladprao Road,

Phiabphla, Wang Thonglang, Bangkok 10310

Rev. 01

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

Effective Date 15/10/21



REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 23-006679

Sample Code : 23-02820-002

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.

2. Interior dimensions approx of chamber :

W = 56 cm ; D = 40 cm ; H = 48 cm

3. Air valve or fresh air level : Off

4. Fan level : Open

5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".

6. Uniformity - the maximum difference of measured temperatures at the reference location which are observed at the same time.

7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.

8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.

9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.

10. Calibration results without adjustment.

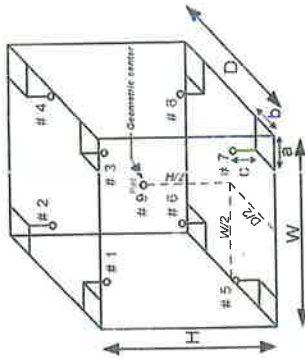


Figure: Example of sensor installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of Report -

[Signature]

COPY

INDUCTIBELY COUPLED PLASMA SPECTROMETER

Model : Prodigy 7

Serial No. : P70177



บริษัท แอปพลิเคชัน ดีไซน์ จำกัด
Application Define Company Limited
133/318 ถนนพหลโยธิน แขวงมีนบุรี เขตมีนบุรี กรุงเทพมหานคร 10510
Tel: (66) 94456-5191 E-mail: support@apdefine.co.th Website: http://www.apdefine.co.th
เลขประจำตัวผู้เสียภาษี 10556032491

CERTIFICATE OF INSTRUMENT PERFORMANCE

INSTRUMENT:

BRAND: Telendyne Leeman Labs

MODEL: Prodigy 7

SERIAL NO. P70177

CUSTOMER: บริษัท อีทีทีเอ็นไทย คอนสตรัคชั่น 1992 จำกัด

CHECKING:

SPECTROMETER Wavelength Accuracy check by use emission line of Hg Lamp

Mercury line 253.652 nm.

Plasma View (Dual View)

CMOS Detector check

Align View by Mn line 257.610 nm.

RF GENERATOR

Incident Power 1,200 ±10 Watt Reading = 1200 Watt

SAMPLE INTRODUCTION

Plasma Torch, Injector, Spray chamber, Nebulizer

Paristaltic pump & Tubing

EXHAUSTING & COOLING SYSTEM

Safety Interlock Switch (Door, Argon pressure, Water pressure)

Cooling System, water flowrate & low pressure switch

Flowrate of Air blower

COMPUTER & SOFTWARE

Plasma Ignition software & Analytical Software

ANALYTICAL TEST

Full Frame Capture & Echellogram check

Calibration Curve & QC Test

DATE: Dec 12, 2022

Mr. Sornchai Chumyung
Engineer Sign

COPY

PREVENTIVE MAINTENANCE / CALIBRATION REPORT FOR PRODIGY7

Customer: บริษัท อีทีทีเอ็นไทย คอนสตรัคชั่น 1992 จำกัด	Date: Dec 12, 2022
Instrument: ICP-OES	Model: Prodigy 7
	S/N: P70177

1. Gas Supply /Water Re-circulator/Exhaust Hood Check:

Gas system: ตรวจระบบแก๊สและการทำงานของ Argon Pressure: 5-5 psi Leak inspected (✓) No leak Nitrogen Pressure: - psi Leak inspected (✓) No leak Oxygen Pressure: - psi Leak inspected (✓) No leak	
() Change camera purge gas Dehydrator (1 times /years) Next time replacement 12/22 เปลี่ยนตัวดูดความชื้นที่เพ็คเตอร์ ทุก 1 ปี	
Water Chiller: RF generator flow rate 4.44 LPM Temperature 24°C ตรวจอุณหภูมิ Leak inspected (✓) No leak ตรวจการรั่วซึม	
Water Chiller: Camera (✓) check water level and refill ตรวจระดับน้ำและเติมน้ำ (✓) change water เปลี่ยนถ่ายน้ำ Temperature 31°C ตรวจอุณหภูมิ	
Exhaust Hood Flow rate 360 CFM (system request > 150)	



TELEDYNE LEEMAN LABS
CALIBRATION SERVICE

COPY

PREVENTIVE MAINTENANCE / CALIBRATION REPORT FOR PRODIGY7

Customer: บริษัท อีทีพี จำกัด
Instrument: ICP-OES
Date: Dec 12, 2022
S/N: P70 77
Model: Prodigy 7

2. Computer & Software Check

Description	Status
Interface Cable USB (✓) No broken	OK
Software Version	OK
(✓) Operation function check :	OK
(✓) Open /Save /Edit method	OK
(✓) Instrument Control	OK
(✓) Sequence	OK
(✓) Full Frame Capture (Echelle Mode)	OK
(✓) Auto alignment /Hg alignment	OK
(✓) Calibration Curve	OK
(✓) Re-Calculation	OK
(✓) Print Report	OK

PREVENTIVE MAINTENANCE / CALIBRATION REPORT FOR PRODIGY7

Customer: บริษัท อีทีพี จำกัด
Instrument: ICP-OES
Date: Dec 12, 2022
S/N: P70177
Model: Prodigy 7

3. Instrument Control

Description	Status
Optical view position: ตรวจสอบตำแหน่งที่คมชัดได้โดยไม่มีฝุ่นบนเลนส์	
Hg Lamp Deltas	
X 2 Y -9	OK
XUV 0	OK
Axial peak positions X 3325 Y 1225	OK
Radial peak positions X 4151 Y 1225	OK
Hg lamp peak positions X 2220 Y 2630	OK
Plasma Control ตรวจสอบการทำงานของหลอดและดับพลาสมา	
(✓) Auto Start	OK
(✓) Extinguish	OK
(✓) RF power setting	OK
(✓) Igniter	OK
(✓) Air Knife	OK
Torch Gas ตรวจสอบการทำงานของระบบแก๊สที่ใช้ในพลาสมา	
(✓) Coolant /Plasma Flow control	OK
(✓) Aux Flow	OK
(✓) Nebulizer Flow	OK
(✓) Optimize sample introduction function	OK
(✓) Peristaltic pump control	OK
(✓) Auto sampler Control	OK
(✓) Camera Support Module	OK
(✓) Diagnostic	OK

Copy

Copy

PREVENTIVE MAINTENANCE / CALIBRATION REPORT FOR PRODIGY7

Customer: บริษัท อีทีพี จำกัด	Date: Dec 12, 2022
Instrument: ICP-OES	Model: Prodigy 7
	S/N: P70177

4. Cleaning & Replacement

Description	Status
(✓) O-Ring Torch replacement	OK
(✓) Pump Tubing replacement	OK
(✓) Glassware cleaning (Torch, Nebulizer, Spray chamber)	OK
(✓) Lube the roll peristaltic pump	OK
(✓) Optical windows cleaning	OK
(✓) Camera Water Re-circulator (water change/ refilled)	OK
(✓) RF Generator Water Re-circulator (water change/ refilled)	OK
(✓) Cleaning Electronics Board with spray cleaner	OK
(✓) Cleaning dust inside Unit	OK
(✓) Cleaning dust filter	OK

5. Safety Interlock

Description	Status
(✓) Door switch	OK
(✓) RF Water Re-circulator	OK
(✓) Camera Water Re-circulator	OK
(✓) Camera purge gas	OK
(✓) Argon pressure	OK
(✓) Nitrogen pressure	OK

COPY

PREVENTIVE MAINTENANCE / CALIBRATION REPORT FOR PRODIGY7

Customer: บริษัท อีทีพี จำกัด	Date: Dec 12, 2022
Instrument: ICP-OES	Model: Prodigy 7
	S/N: P70177

6. Hardware Check with SALSAXE Diagnostics

Power Supply	Value	Status
-12 VDC (11 - 14.5 VDC)	-13.75%	OK
+12 VDC (11 - 14.5 VDC)	+12.01%	OK
+3.3 VDC	3.28%	OK
+5.0 VDC	4.44%	OK
+13.5 VDC	13.45%	OK

Plasma Generator	Value	Status
ICP Current 0.500A = 1kW	0.544	OK
ICP Ref 5.0Vdc = 1kW	5.464	OK
ICP Current 0.00 Vdc = 0kW	0	OK
ICP Ref 0.00Vdc = 0kW	0	OK
RF Water (Hz) OFF	0	OK
RF Water (Hz) ON	23	OK
Air Knife Pres. (0.00V) OFF	0	OK
Air Knife Pres. (3.0 - 7.0 V) ON	4.054	OK
Neb 25 @ setting of 25 PSI	25	OK
Cool 18 @ setting of 18 LPM	18	OK
Aux 0.6 @ setting of 6 LPM	0.6	OK
Pump Current (0.000 A) OFF	0	OK
Pump Voltage (0.000 V) OFF	0	OK
Pump Current (0.8 to 4.0A) ON	1.04	OK
Pump Voltage (8 to 13 V) ON	12.52	OK

Set Points	Value	Status
Air In Set Point 32°C	31	OK
Cam Tec Temperature -32°C	-32	OK
Op Purge Low 0.77 LPM	0.7	OK
Op Purge High 15.50 LPM	15.5	OK
Cam Wtr T 28°C	28	OK



COPY

PREVENTIVE MAINTENANCE / CALIBRATION REPORT FOR PRODIGY7

Customer: บริษัท อีทีพี เทคโนโลยี จำกัด	Date: Dec 12, 2022
Instrument: ICP-OES	S/N: P70177

7. Mn Check for performance Test

	Condition for performance Test	Condition Test	Status
Standard	1 ppm, 5 ppm, 10 ppm	10 ppm	ok
Power plasma	1.20 kw	1.2	ok
Plasma gas	16.0 LPM	16	ok
Auxiliary Gas	0.8 LPM	0.8	ok
Nebulizer	1.2 LPM	25 L/min	ok
Pump Speed	25 RPM	25	ok
Integration time	15 s Axial, 5 s Radial	10 s, 5 s	ok
Nebulizer Type	Seaspray, Conical, Meinhard	Seaspray	ok
Intensity first performance	1 ppm \geq 4,000,000 5 ppm \geq 15,000,000 10 ppm \geq 50,000,000	265,000,000	ok

Engineer Sign	12 Dec 2022
 Somchai Churnyung	 TELEDYNE LEEMAN LABS Everywhere you look


COPY

ORIFICE TRANSFER STANDARD CERTIFICATION

WORKSHEET TE-5025A

ROOTSMETER S/N 0438320

TISCH ENVIRONMENTAL, INC.
145 SOUTH MIAMI AVE
VILLAGE OF CLEVELAND, OH
44102
513.467.9000
877.263.7810 TOLL FREE
513.467.9009 FAX

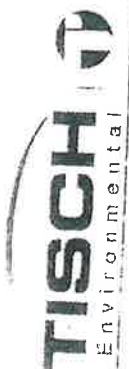

ORIFICE TRANSFER STANDARD CERTIFICATION WORKSHEET TE-5025A

Date - Mar 24, 2016 Rootmeter S/N 0438320 Ta (K) - 295
Operator Tisch Orifice I.D. - 0136 Pa (mm) - 742.95

PLATE OR Run #	VOLUME START (m3)	VOLUME STOP (m3)	DIFF VOLUME (m3)	DIFF TIME (min)	METER DIFF Hg (mm)	ORIFICE DIFF H2O (in.)
1	NA	NA	1.00	1.3400	3.2	2.00
2	NA	NA	1.00	0.9510	6.3	4.00
3	NA	NA	1.00	0.8510	7.8	5.00
4	NA	NA	1.00	0.8130	8.6	5.50
5	NA	NA	1.00	0.6690	12.6	8.00

DATA TABULATION

Vstd	(x axis) Qstd	(y axis)	Va	(x axis) Qa	(y axis)
0.9832	0.7337	1.4054	0.9957	0.7430	0.8911
0.9791	1.0296	1.9875	0.9915	1.0426	1.2603
0.9770	1.1481	2.2221	0.9894	1.1626	1.4090
0.9760	1.2006	2.3305	0.9884	1.2157	1.4778
0.9707	1.4510	2.8107	0.9830	1.4694	1.7823
Qstd slope (m) =	1.96262		Qa slope (m) =	1.22896	
intercept (b) =	-0.03249		intercept (b) =	-0.02060	
coefficient (r) =	0.99993		coefficient (r) =	0.99993	
y axis = SQRT(H2O(Pa/760) (298/Ta))			y axis = SQRT(H2O(Ta/Pa))		

CALCULATIONS

Vstd = Diff. Vol [(Pa-Diff. Hg)/760] (298/Ta)
Qstd = Vstd/Time

Va = Diff Vol [(Pa-Diff Hg)/Pa]
Qa = Va/Time

For subsequent flow rate calculations:

Qstd = $1/m \{ [\text{SQRT}(H2O(Pa/760) (298/Ta))] - b \}$
Qa = $1/m \{ [\text{SQRT}(H2O(Ta/Pa)) - b \}$

Copy

Primary Flow Calibrator
Serial No. : 110619 , 207510

Certificate of Calibration

Certificate No : 23-AFM-022
Request No : Req-2023-0128

Customer
Name : Eastern Thai Consulting 1992 Co., Ltd.
Address : 683 Moo 11, Sukhaphum 8 Rd., Nongkham, Sriracha, Chonburi 20230

Unit Under Calibration Details

Unit Order Number	: 096789
Measurement Item	: Primary Flow Calibrator
Manufacturer	: BIOS
Model	: Defender 510-L
Serial Number	: 110619
Sensor Model :	
Sensor Serial Number : -	

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature	: 23 °C ± 3 °C
Humidity	: 55 %RH ± 20 %RH
Barometric Pressure	: 1013 hPa ± 10 hPa
Received Date	: 20 January 2023
Calibration Date	: 6 February 2023

Calibration Date : 6 February 2023

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	185010110006	Sensidyne	15 June 2023
Air Flow Meter	Gilibrator 3 Standard flow	190310111003	Sensidyne	15 June 2023

Traceability :

Traceability : to recognized national standard, and to the realization of the international System of

Units (SI)

Note :
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Calibration By:

Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :
Mr. Pacit Mathayom

Calibration Engineer Supervisor

Issue Date : 6 February 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval.

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
EN-709-AFM-01 Rev.00 Issue date 01/

Certificate No : 23-AFM-022

Request No : Req-2023-0128

End of Certificate

Note

STD : Standard

Unit Under Calibration

DOX

Certificate No : 23-AFM-024
Request No : Req-2023-0196

Result of Calibration :

Measurement Item	: Primary Flow Calibrator	Sensor Model : -
		Sensor Serial Number : -

Manufacturer	: Mesa Labs
Model	: Defender 510-M
Serial Number	: 207510
Sensor Serial Number	:

FD : - : Location of Calibration : LAB 4 AIR VELOCITY METER

Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Humidity	: 55 %RH \pm 20 %RH
Barometric Pressure	: 1013 hPa \pm 10 hPa
Received Date	: 25 January 2023
Calibration Date	: 6 February 2023

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceable	Due Calibration
As-Flow Meter	Calibrator 3 Standard flow	19031011003	Sensidyne	15 June 2023

Traceability: This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of

Note :
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Approved By: M. P. Mathavom
Mr. Pacit Mathavom
Calibration Engineer Supervisor
Issue Date: 6 February 2023

6 February 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

Calibration Point	STD Flow Reading	UUC Flow Reading	Correction Flow	Uncertainty (\pm)
(cc/min)	(cc/min)	(cc/min)	(cc/min)	(cc/min)
500	501.1	506.43	-5.3	7.2
1000	1019	1032.2	-13	15
2000	2003	2017.8	-15	29
3000	3007	3023.8	-17	43
4000	4013	4027.2	-15	57

Note
STD : Standard
UUC : Unit Under Calibration

End of Certificate

THERMO-HYGROMETER

Model : 608-H1

Serial No. : 45106737

CERTIFICATE OF CALIBRATION

Page 1 of 2
Certificate No. : 23-055203
Sample Code : 23-21440-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration laboratory)

Equipment : Digital thermo-hygrometer
Manufacturer : testo
Serial No. : 45106737
Date of Receipt : 25 May 2023

Model : 608-H1
ID No. : LABE 09/7
Date of Calibration : 29 May 2023

Condition of Calibration

1. **Environment** : 23.0 °C ± 3.0 °C
: 55.0 % ± 15.0 %

1.2 **Relative humidity**

2. **Calibration method**

2.1 In-house method: WI-CL-045 By comparison with thermometer standard / chilled mirror hygrometer in controlled chamber.

2.2 The calibration by comparison unit under calibration (UUC) to the thermometer standard / chilled mirror hygrometer in a chamber at the controlled temperature / relative humidity.

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Chilled Mirror	Optidew Vision	LB-DP-02 & LB-DP-02 (DP)	TH-0157-22	05 December 2023
3.2 Digital Thermometer	Optidew Vision	LB-DP-02 & LB-DP-02 (Temp.)	23-014916	12 February 2024
3.3 Digital Thermometer	34972A	LB-DA-07 with RTD-89	22-095535	06 September 2023

4. This certificate is traceable to the international system of unit (SI Unit).

4.1 Instrument No. 3.1 through National Institute of Metrology (Thailand).

4.2 Instrument No. 3.2 and 3.3 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Miss Pornsuda Lohabai
Scientist

Approved by : (Mr. Somchai Neampunt)
Signed for Director

Issue date : 31 May 2023

The uncertainties are for a confidence probability of approximately 95%
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310

CONTACT@AMARC.CO.TH
TEL 02-516-2422
FAX 02-516-6949
Effective date: 15/10/21

REPORT OF CALIBRATION

Page 2 of 2
Certificate No. : 23-055203
Sample Code : 23-21440-001

Results of Calibration

Temperature measurement

Resolution : 0.1 °C
Range : 0 °C to 50 °C

Calibration point °C	Average of standard reading		Unit under calibration		Expanded uncertainty °C
	Controlled humidity %RH	Temperature °C	Average reading °C	Correction value °C	
20	50	20.00	20.0	0.00	± 0.39
25	50	25.02	25.1	- 0.08	± 0.39
30	50	30.00	30.0	0.00	± 0.39

Humidity measurement

Resolution : 0.1 %RH
Range : 10 %RH to 95 %RH

Calibration point %RH	Average of standard reading		Unit under calibration		Expanded uncertainty %RH
	Air temperature °C	Calculated humidity %RH	Average reading %RH	Correction value %RH	
45	25.00	45.18	53.5	- 8.32	± 1.3
60	25.00	60.03	68.3	- 8.27	± 1.5
75	25.00	75.20	83.2	- 8.00	± 1.7

Notes

- Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of Report -

Copy

CERTIFICATE OF ANALYSIS

EPA PROTOCOL GAS

Cylinder No. : EB0062815

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04NI99E15ACX9C Reference Number: 82-401135335-1
Cylinder Number: EB0062815 Cylinder Volume: 144.4 CF
Laboratory: 124 - Riverton (SAP) - NJ Cylinder Pressure: 2015 PSIG
PGVP Number: B52018 Valve Outlet: 660
Gas Code: CO,NO,NOX,SO2,BALN Certification Date: Mar 13, 2018
Expiration Date: Mar 13, 2026

Certification performed in accordance with EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)* document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	50.00 PPM	50.55 PPM	G1	+/- 1.4% NIST Traceable	03/06/2018, 03/13/2018
NITRIC OXIDE	50.00 PPM	50.50 PPM	G1	+/- 1.4% NIST Traceable	03/06/2018, 03/13/2018
SULFUR DIOXIDE	50.00 PPM	51.01 PPM	G1	+/- 1.0% NIST Traceable	03/06/2018, 03/13/2018
CARBON MONOXIDE	2000 PPM	1977 PPM	G1	+/- 1.0% NIST Traceable	03/06/2018
NITROGEN	Balance				
CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NITRM	16060607	CC442564	50.42 PPM NITRIC OXIDE/NITROGEN	+/- 0.8%	Jun 27, 2020
PRM	12367	APEX1099237	9.82 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Jun 02, 2017
SGMS	0315201604	CC0503358	4.975 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Mar 15, 2019
NITRM	16011025	CC473218	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 07, 2022
NITRM	12060735	CC356192	2488 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Dec 14, 2026
*The SRM, PRM or RGM noted above is only in reference to the GMS used in the assay and not part of the analysis.					
ANALYTICAL EQUIPMENT					
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration			
Nicolet 6700 APW1100391 CO	FTIR	Feb 08, 2018			
Nicolet 6700 APW1100391 NO	FTIR	Feb 15, 2018			
Nicolet 6700 APW1100391 NO2	FTIR	Feb 16, 2018			
Nicolet 6700 APW1100391 SO2	FTIR	Mar 01, 2018			

Triad Data Available Upon Request

NOTES:NET WEIGHT: 10.43lbs
GROSS WEIGHT: 60.93lbs
PO# 5218000763

This calibration std. has been certified in accordance with the May 2012 EPA Traceability Protocol, Document EPA-600/R-12/531. All testing processes and measurements conform to the requirements of ISO/IEC 17025 and to Airgas ISO 9001:2000 and relate only to items identified on this certificate. All concentrations are certified to be NIST Traceable with total uncertainty as detailed under Analytical Uncertainty. This document shall not be reproduced in full without written approval of the issuer.



TESTING CERT No. 3082.05

Don Morris
Approved for Release

SOUND LEVEL CALIBRATOR

MODEL : NC-75

SERIAL No. : 34302326

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



Cert. No. : ACC23013
Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR

Manufacturer : RION

Model : NC-75

Serial No.: 34302326

ID No.:

Condition As Found :

GOOD

Customer :

EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :

Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date :

Calibration Date : 10 MAY 2023
Date of Issue : 19 MAY 2023
24 MAY 2023

Calibrated by :

Natnakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL_BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL_BP 30/0267	13-FEB-24
Digital Multimeter	33461A	MY60024273	EEL_BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24
Audio Analyzer	AVR-3360A	V7744B6069	EF-0012-23	10-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

Continuation of Calibration Certificate

Cert No. : ACC23013
Job No. : VC66AC0058
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.03	0.03	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
0.32	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 01120945

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Banghumnu, Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



NSC-TSI-17025
CALIBRATION 0394

Cert No. : ACL23096
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 01120945 / 21951 / 22334
ID No.:

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 24 JANUARY 2023
Calibration Date : 26-30 JANUARY 2023
Date of Issue : 01 FEBRUARY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23096
Job No. : VC66AC0035
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY
T. Petchurai

Continuation of Calibration Certificate

Cert. No. : ACL23096
Job No. : VC66AC0035
Pages : 3 of 8

Continuation of Calibration Certificate

Cert. No. : ACL23096
Job No. : VC66AC0035
Pages : 4 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	9.9
C - weight	14.9
Flat	20.5

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.2	0.2	0.2
1000	0.1	0.1	0.1
8000	0.0	0.0	0.0
			Acceptance Limits
			±1.0
			±0.7
			+1.5, -2.5

Continuation of Calibration Certificate

Cert. No. : ACL23096
Job No. : VC66AC0035
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
63	-0.1	0.0	±1.0
125	0.0	0.0	±1.0
250	0.0	0.0	±1.0
500	0.0	0.0	±1.0
1000	0.0	0.0	±1.0
2000	0.0	0.1	±1.0
4000	0.0	0.0	±1.0
8000	0.0	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

Continuation of Calibration Certificate

Cert. No. : ACL23096
Job No. : VC66AC0035
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	29.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8
28.0	28.0	0.0	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.8	-0.2	±0.8

Continuation of Calibration Certificate

Cert. No. : ACL23096
Job No. : VC66AC0035
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.5	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.1	-0.3	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	89.5	0.0	±1.5
Negative one-half cycle	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

COPY

S. Reth

Analytical Balances

Model : XS205DU

Serial No : B814654693

Mettler-Toledo (Thailand) Ltd.

846/4 - 846/5 Lasalle Rd., Bangna Tai Sub-District

Bangna District, Bangkok 10260

+66 2723 0382

MT-TH.ServiceSupport@mt.com



NSC-TISI-TIS 17025
CALIBRATION 0062

Accuracy Calibration Certificate

Customer

Company: Eastern Thai Consulting 1992 Co., Ltd.
Address: 129 Moo 1, Nonsi
City: Kabin Buri **Contact:** Tassawan Chansamrong
Zip / Postal: 25110
State / Province: Prachinburi
Order Number: 
0 3 3 2 7 0 0 1 6 6

Weighing Device

Manufacturer: Mettler Toledo **Instrument Type:** Weighing Instrument
Model: XS205DU **Asset Number:** KB-LAB-61/002
Serial No.: B814654693 **Terminal Model:** SAT
Building: Office Laboratory **Terminal Serial No.:** B814654693
Floor: 1 **Terminal Asset No.:** N/A
Room: Laboratory

Range	Max. Capacity	Readability (d)
1	81 g	0.00001 g
2	220 g	0.0001 g

Procedure



Calibration Guideline: EURAMET cg-18 v. 4.0 (11/2015)
METTLER TOLEDO Work Instruction: CP/W002/20

This calibration certificate contains measurements for As Found calibration. No As Left calibration was performed because the device was not modified after As Found calibration. Therefore, results for As Left correspond to As Found.

The sensitivity/span of the weighing instrument was adjusted before calibration with a built-in weight.

In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

	Temperature		Humidity	
As Found	Start: 22.7 °C	End: 22.4 °C	Start: 62.9 %	End: 66.8 %

As Found Calibration Date: 21-Mar-2023 **Calibrator:** 
As Left Calibration Date: N/A
Issue Date: 23-Mar-2023
Approved Signatory: 
Kassakorn Tassanachaisakul
Technical Manager / Head of Calibration Center

Measurement Results


Repeatability

Test Load: 70 g

	As Found	As Left
1	70.00006 g	N/A
2	70.00004 g	N/A
3	70.00004 g	N/A
4	70.00005 g	N/A
5	70.00005 g	N/A
6	70.00006 g	N/A
7	70.00004 g	N/A
8	70.00006 g	N/A
9	70.00007 g	N/A
10	70.00005 g	N/A

Standard Deviation	0.000010 g	N/A
--------------------	------------	-----

○ As Found
◆ As Left

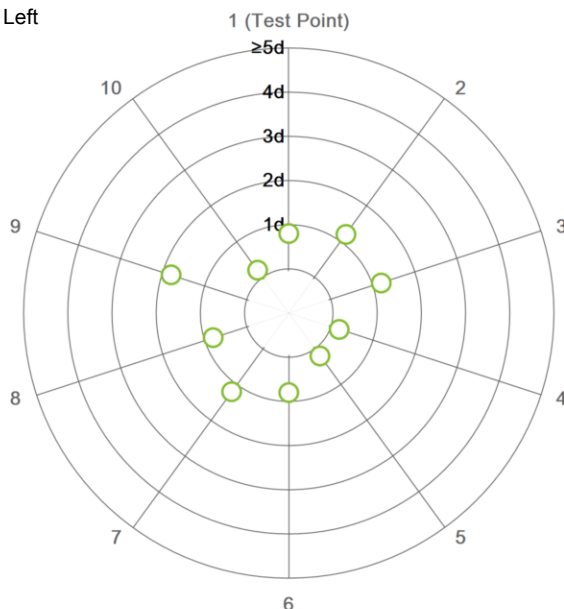

The "d" in the graph represents the readability of the range/interval in which the test was performed.


The results of this graph are based upon the absolute values of the differences from the mean value.

Eccentricity

Test Load: 100 g

Position	As Found	As Left
1	100.0000 g	N/A
2	100.0000 g	N/A
3	100.0001 g	N/A
4	100.0000 g	N/A
5	100.0000 g	N/A

Maximum Deviation	0.0001 g	N/A
-------------------	----------	-----



As Found


The "d" in the graph represents the readability of the range/interval in which the test was performed.

Error of Indication

As Found

	Reference Value	Indication	Error of Indication	Expanded Uncertainty	k
1	0.00000 g	0.00000 g	0.00000 g	0.021 mg	2
2	0.05001 g	0.05003 g	0.00002 g	0.025 mg	2
3	0.10001 g	0.10003 g	0.00002 g	0.026 mg	2
4	0.50001 g	0.50000 g	-0.00001 g	0.031 mg	2
5	1.00002 g	1.00005 g	0.00003 g	0.035 mg	2
6	5.00002 g	5.00005 g	0.00003 g	0.050 mg	2
7	10.00003 g	10.00005 g	0.00002 g	0.062 mg	2
8 ¹	50.00002 g	49.99999 g	-0.00003 g	0.12 mg	2
9	100.0001 g	100.0001 g	0.0000 g	0.21 mg	2
10	150.0001 g	150.0000 g	-0.0001 g	0.32 mg	2
11	200.0001 g	200.0000 g	-0.0001 g	0.37 mg	2

¹The calculated uncertainty was replaced by the CMC (Calibration and Measurement Capabilities) value because the calculated uncertainty was smaller than the CMC value.

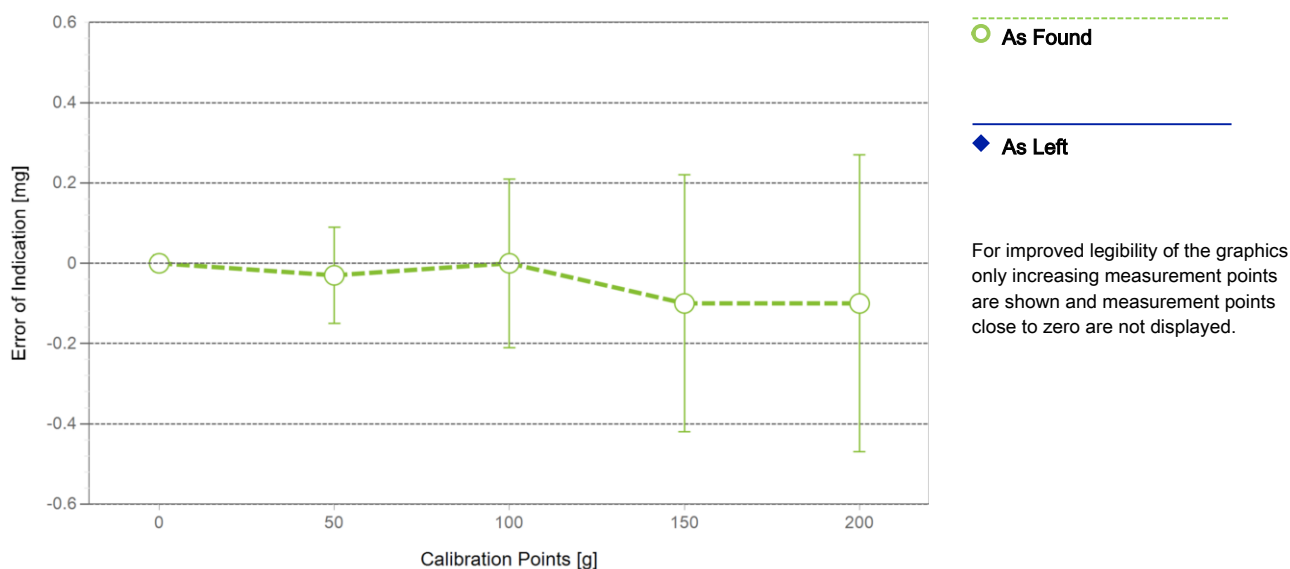

The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor k – which can be larger than 2 according to EURAMET cg-18. The value of the measurand lies within the assigned range of values with a probability of approximately 95%.

The user is responsible for maintaining environmental conditions and the settings of the weighing instrument when it was calibrated.

Test Equipment

All weights used for metrological testing are traceable to national or international standards. The weights were calibrated and certified by an accredited calibration laboratory.

Weight Set 1: OIML E2

Weight Set No.:	WS79	Date of Issue:	23-Feb-2022
Certificate Number:	C208581630	Calibration Due Date:	17-Aug-2023

Thermo Hygrometer

Equipment No.:	IN301	Date of Issue:	14-Sep-2022
Certificate Number:	22H1857	Calibration Due Date:	05-Sep-2023
	N/A		

Remarks

FACT adjustment functionality activated
Equipment condition: Good
Next calibration according to customer's procedure
Calibration data not decide by calibration laboratory

End of Accredited Section

The information below and any attachments to this calibration certificate are not part of the accredited calibration.

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with $k=2$ in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use: $1.5 \cdot 10^{-6} / K$

Temperature range on site for the evaluation of the measurement uncertainty in use: 3 K


Linearization of Uncertainty Equation

Range			As Found	As Left
	d	Max		
1	0.00001 g	81 g	$U_1 = 0.022 \text{ mg} + 0.00487 \text{ mg/g} \cdot R$	N/A
2	0.0001 g	220 g	$U_2 = 0.06 \text{ mg} + 0.00487 \text{ mg/g} \cdot R$	N/A


To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication	As Found		As Left	
0.00220 g	0.022 mg	1.0%	N/A	N/A
0.02200 g	0.022 mg	0.10%	N/A	N/A
0.22000 g	0.023 mg	0.010%	N/A	N/A
2.20000 g	0.033 mg	0.0015%	N/A	N/A
220.0000 g	1.1 mg	0.00051%	N/A	N/A

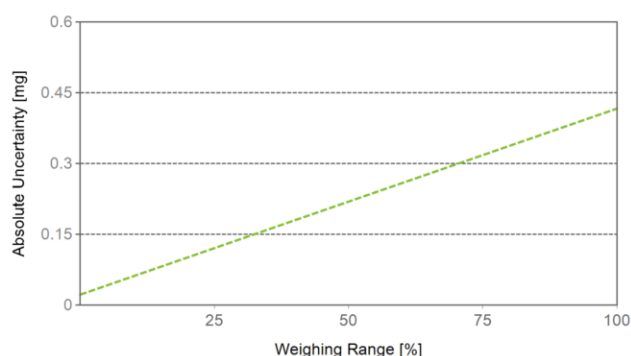

As Found

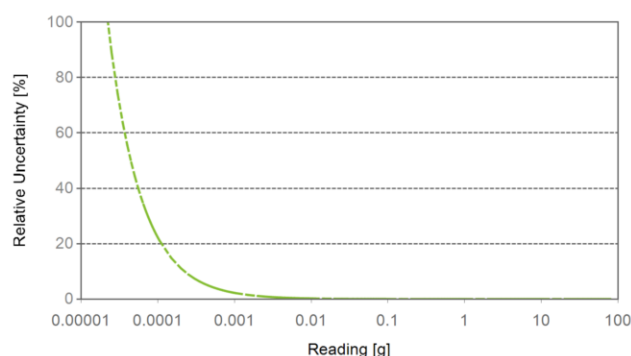

As Left

The weighing range shown in the absolute uncertainty graph refers to the first interval/range of the device.

Thermo Reactor

Model : TR420

Serial No. : 19490657



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T231631

Page 1 of 4

Certificate of Calibration

Equipment : Spectroquant Thermoreactor

Manufacturer : Merck

Model : TR420

Serial No. : 19490657

Customer Code : KB-LAB-63/031

ID No. : T2602A5

Customer : Eastern Thai Consulting 1992 Co.,Ltd.
129 Moo.1 Nonsi,
Kabinburi, Prachinburi 25110

Customer Location : Hot Room

Date of Receipt : 5 September 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 14 SEP 2023

The uncertainties are for a confidence probability of approximately 95%.



This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109


Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T231631

Page 3 of 4

Calibration Report

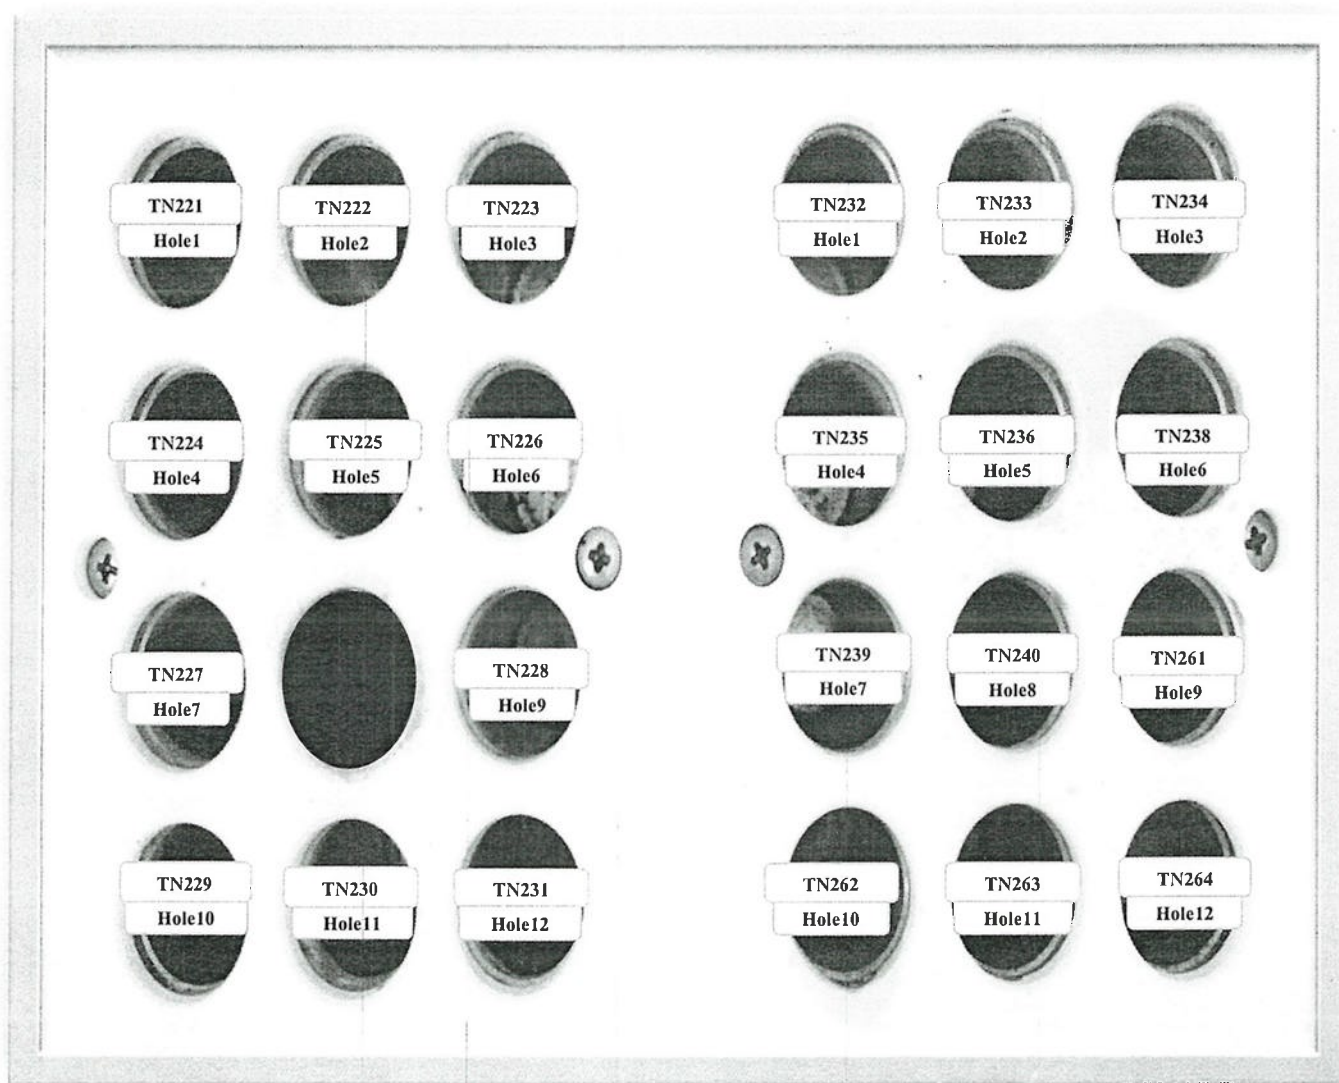

FRONT CONTROL

Approved By. _____

Im Lin

Thassan

Certificate No. T231631

Page 4 of 4

Calibration Report

Measurement Results

Average Standard Reading at each position (° C) BLOCK LEFT

		Hole1	Hole2	Hole3	Hole4	Hole5	Hole6	Hole7	Hole8	Hole9	Hole10	Hole11	Hole12
Calibration Point		TN221	TN222	TN223	TN224	TN225	TN226	TN227		TN228	TN229	TN230	TN231
CAL POINT	Max	149.6	149.4	149.5	150.2	149.9	149.5	148.0		150.0	149.4	150.7	150.9
150	Min	149.3	149.0	149.2	149.8	149.6	149.3	147.7		149.7	149.1	150.4	150.6
	Average	149.4	149.2	149.4	150.0	149.7	149.4	147.9		149.8	149.3	150.6	150.8

Average Standard Reading at each position (° C) BLOCK RIGHT

		Hole1	Hole2	Hole3	Hole4	Hole5	Hole6	Hole7	Hole8	Hole9	Hole10	Hole11	Hole12
Calibration Point		TN232	TN233	TN234	TN235	TN236	TN238	TN239	TN240	TN261	TN262	TN263	TN264
CAL POINT	Max	150.4	149.4	148.9	150.2	150.6	150.6	149.5	149.4	149.6	149.4	148.6	149.8
150	Min	150.3	149.2	148.7	150.0	150.5	150.4	149.4	149.3	149.5	149.2	148.5	149.6
	Average	150.4	149.3	148.8	150.1	150.5	150.5	149.4	149.4	149.4	149.3	148.6	149.7

Spectroquant Thermoreactor				Temperature Distribution	
Setting (° C)	Reading (° C)			Stability (± ° C)	Uncertainty (± ° C)
	Min , Max		Average		
152	-		152	0.2	0.96

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____



Chamber (Incubator)

Model : SRR3-0687 AR

Serial No. : SRR3675A-20070022R



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T231934

Page 1 of 3

Certificate of Calibration

Equipment : Chamber (Incubator)

Manufacturer : SANDEN Intercool

Model : SRR3-0687 AR

Serial No. : SRR3675A-20070022R

Customer Code : KB-LAB-63/019


ID No. : T1548A5

Customer : Eastern Thai Consulting 1992 Co.,Ltd.
129 Moo.1 Nonsi,
Kabinburi, Prachinburi 25110

Customer Location : Laboratory

Date of Receipt : 17 October 2023

Calibrated By : Atiphong Rongrat (Technician)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 06 NOV 2023



The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T231934

Page 2 of 3

Calibration Report

Equipment : Chamber (Incubator)
Date of Calibration : 24 October 2023
Environment : Temperature : 32.6-34.5 °C
Line Voltage : 222.7-227.4 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber, the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
- All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	31-(CH1-10)	T230504	24 March 2024
DATA LOGGER	34970A	T114	T230504	24 March 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour - Minute At 20 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

(X) without adjustment

() after adjustment


Approved By. _____



Certificate No. T231934

Page 3 of 3

Calibration Report

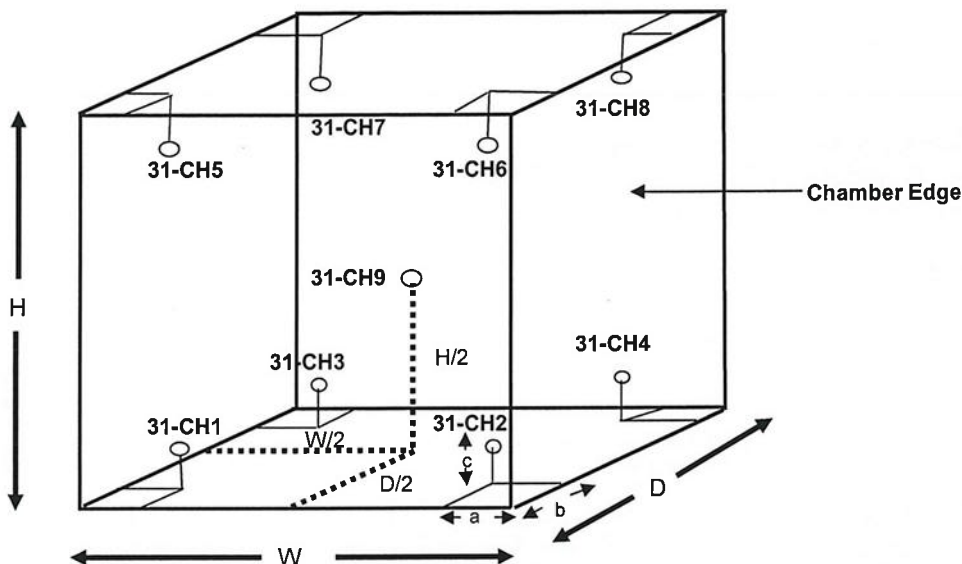

Remark :

Internal Dimensions of Chamber : W (Width) = 58 cm. H(Height)=143 cm. and D(Depth)=61 cm.
 Size of Installed Standard sensor number 31-CH1 to number 31-CH8 a = 5 cm. ,b = 5 cm. and c = 5 cm.
 Size of Installed Standard sensor number 31-CH9 : W/2=58 cm./2 H/2=143 cm./2 and D/2=61 cm./2

Measurement Results	Average Standard Reading at each position (°C)								
Calibration Point	31-CH1	31-CH2	31-CH3	31-CH4	31-CH5	31-CH6	31-CH7	31-CH8	31-CH9
20	19.89	20.02	19.89	20.40	20.26	20.21	20.09	20.10	19.97

Chamber (Incubator)			Temperature Distribution			
Setting (°C)	Reading (°C)		Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor k
	Min , Max	Average				
20.0	-	20.0	0.09	0.37	0.38	2.00

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



Chamber (Refrigerator)

Model : SCR-1320SAD

Serial No. : 0508-00065



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T230515

Page 1 of 3

Certificate of Calibration

Equipment : Chamber (Refrigerator)

Manufacturer : Sanden Intercool

Model : SRC-1320SAD

Serial No. : 0508-00065

Customer Code : KB-LAB-48/034


ID No. : T8421A2

Customer : Eastern Thai Consulting 1992 Co.,Ltd.
129 Moo.1 Nonsi,
Kabinburi, Prachinburi 25110

Customer Location : Laboratory

Date of Receipt : 14 March 2023

Calibrated By : Boonchai Suriyawong (Site Calibration Manager)

Approved By :  / Sujjar Naknakred (Site Calibration Manager)

Date of Issue : 27 MAR 2023

The uncertainties are for a confidence probability of approximately 95%.



This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T230515

Page 2 of 3

Calibration Report

Equipment : Chamber (Refrigerator)
Date of Calibration : 22 March 2023
Environment : Temperature : 27.6-27.7 °C
 Line Voltage : 221.7-225.9 V
 Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	13-(CH1-10)	T222309	08 November 2023
DATA LOGGER	34970A	T121	T222309	08 November 2023

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant - Hour 40 Minute At 3 °C
 Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
 ☐ Close
 ☒ Not Available

5. Adjustment :

(X) without adjustment

() after adjustment

Approved By. _____




Thassan

Certificate No. T230515

Page 3 of 3

Calibration Report

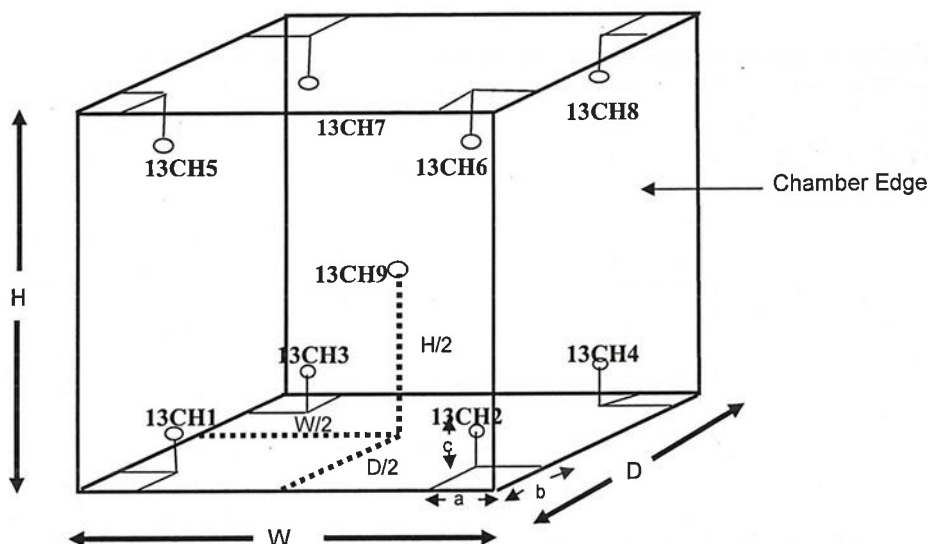

Remark :

Internal Dimensions of Chamber : W (Width) = 100 cm. , H(Height)=135 cm. and D(Depth)=45 cm.
 Size of Installed Standard sensor number13CH1to number13CH8 : a = 5 cm. ,b = 5 cm. and c = 5 cm.
 Size of Installed Standard sensor number13CH9 : W/2=100 cm./2 , H/2=135 cm./2 and D/2=45 cm./2

Measurement Results

Average Standard Reading at each position (°C)									
Calibration Point	13CH1	13CH2	13CH3	13CH4	13CH5	13CH6	13CH7	13CH8	13CH9
3	2.95	3.02	2.80	2.68	3.18	3.98	2.88	2.77	3.27

Chamber (Refrigerator)			Temperature Distribution			
Setting (°C)	Reading (°C)		Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
	Min , Max	Average				
3.0	3 , 4	3.4	0.71	1.46	1.34	2.15

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By _____



Thasorn

pH METER

Model : SevenCompact

Serial No. : B824972289

NSC-TISI-TIS17025
CALIBRATION 0152

Page 1 of 3

CERTIFICATE OF CALIBRATION

Certificate No. : 23-131100

Sample Code : 23-48669-002

Customer : Eastern Thai Consulting 1992 Co., Ltd.
129 Moo 1, Suwannasorn Rd., Nonsri,
Kabinburi, Prachinburi 25110

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : pH Meter

Manufacturer : METTLER TOLEDO **Model** : SevenCompact S220

Serial No. : B824972289 **ID No.** : KB-LAB-61/003

Date of Receipt : 08 November 2023 **Date of Calibration** : 09 November 2023

Condition of Calibration

1. Environment

1.1 Ambient temperature : 25.0 ± 2.5 °C 1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

In house method WI-CL-019: based on direct measurement by using standard voltage calibrator and using certified reference material (CRM).

3. Reference standard / Certified reference material

Instrument	ID No.	Certificate No.	Due Date
3.1 Voltage Calibrator	LB-AMC-01	23E3244	03 October 2024
3.2 Digital Thermometer	LB-TH-33	23-098974	25 August 2024
Certified Reference Material	Lot. No.	Ref No.	Expire Date
3.3 Buffer Solution pH 4.008	919273	PH216.L5	24 September 2025
3.4 Buffer Solution pH 6.985	919274	PH107.L5	24 September 2024
3.5 Buffer Solution pH 10.010	919278	PH220.L5	24 September 2024

4. This certificate is traceable to the international system of unit (SI Unit).

- 4.1 Instrument No. 3.1 through Technology Promotion Association (Thailand-Japan).
- 4.2 Instrument No. 3.2 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.
- 4.3 Buffer Solution No. 3.3 and No. 3.5 traceable to CPA chem (through primary measurement method-Harned cell using calibrated thermometer, barometer, and nanovoltmeter Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).
- 4.4 Buffer Solution No. 3.4 traceable to CPA chem (CPA RefN HARNED CELL LotN 61275737; CPA RefN HARNED CELL LotN 61273986 Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Nuttaput Timula
Scientist

Approved by

(Mr. Somchai Neampunt)
Signed for Director

Issue date

15 November 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



REPORT OF CALIBRATION

Certificate No. : 23-131100

Sample Code : 23-48669-002

Equipment : pH Meter Resolution : 0.01 pH ; 0.1 mV ; 0.1 °C
Manufacturer : METTLER TOLEDO Model : SevenCompact S220
Serial No. : B824972289 ID No. : KB-LAB-61/003
Range : -2.000 pH to 20.000 pH ; ± 2000.0 mV ; -5.0 °C to 130.0 °C

Results of Calibration

Part 1. DC Voltage measurement

pH Meter Serial No. : B824972289

Nominal Value pH	Applied DC Voltage mV	Average indicator reading		Uncertainty mV	Coverage factor k
		mV	pH		
0	414.113	414.0	0.00	± 0.083	2.00
4	177.477	177.5	4.00	± 0.083	2.00
7	0.000	0.1	7.00	± 0.083	2.00
10	-177.477	-177.3	10.00	± 0.083	2.00
14	-414.113	-413.9	14.00	± 0.083	2.00

Part 2. Performance of Electrode system

Electrode Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Electrode Serial No. : 2357000

Three-Point Calibration at pH4, pH7 and pH10 Percent Slope : 99.2

Standard Buffer Solution pH (@ 25 °C)	Average indicator reading		Error Value pH	Uncertainty pH	Coverage factor k
	pH	mV			
4.008	4.01	179.3	0.002	± 0.010	2.00
6.985	6.99	4.2	0.005	± 0.011	2.00
10.010	10.01	-167.2	0.000	± 0.011	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

NSC-TISI-TIS17025
CALIBRATION 0152

Page 3 of 3

REPORT OF CALIBRATION

Certificate No. : 23-131100

Sample Code : 23-48669-002

Equipment : pH Meter (Digital Thermometer with sensor)

Thermometer readout

Manufacturer : METTLER TOLEDO Model : SevenCompact S220
Serial No. : B824972289 ID No. : KB-LAB-61/003
Resolution : 0.1 °C Range : -5.0 °C to 130.0 °C

Thermometer sensor

Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM
Serial No. : 2357000 ID No. : N/A

Condition of Calibration

1. Environment 1.1 Ambient temperature : 23.0 °C ± 3.0 °C
1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

- 2.1 The calibration use in house method WI-CL-021 : by comparison with standard thermometer
2.2 The calibration by comparison unit under calibration (UUC) to the standard thermometer in a calibration bath at the controlled temperature.
2.3 The temperature scale in use of this laboratory is the international temperature scale of 1990 (ITS-90).

3. Reference standard instrument

Instrument	Model	ID. No.	Certificate No.	Due date
3.1 Resistance Thermometer	PT-100	RTD-90	23-098974	25 August 2024
3.2 Thermometer Readout	GT-11	LB-TH-33	23-098974	25 August 2024

4. This certificate is traceable to the international system of unit (SI Unit).

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Accreditation Under TLAS Laboratory Calibration No.0152)

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibration item : Normal

Thasarn

Results of Calibration

Calibration point °C	Average of standard reading °C	Unit under calibration			Expanded uncertainty °C	Coverage factor k
		Immersion depth mm	Average reading °C	Correction value °C		
23	23.001	120	23.0	+ 0.001	± 0.13	2.00
25	25.000	120	25.0	0.000	± 0.13	2.00
27	26.999	120	27.0	- 0.001	± 0.13	2.00

Notes

- Calibration results without adjustment

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

Penw

- End of report -

Conductivity Meter

Model : SevenCompact

Serial No : C038084210



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CH105

Page.: 1 of 2

Certificate of Calibration

Equipment :	Conductivity Meter
Manufacturer :	Mettler Toledo
Model :	SevenCompact
Serial No. :	C038084210
ID No. :	KB-LAB-64/001
Condition As-Received:	Used Item
Received Date :	24 January 2023
Calibration Date :	25 January 2023
Reference :	2301-0755DC-1
Submitted by :	Eastern Thai Consulting 1992 Co.,Ltd. 129 Moo.1 Nonsi, Kabinburi, Prachinburi 25110
Ambient Temperature :	$(25 \pm 2.5) ^\circ\text{C}$
Relative Humidity :	$(50 \pm 15) \%$
Calibration Procedure:	In -house method : - CP-CH6 : based on direct measurement by using certified reference material (CRM)

Calibrated by : Walalak Sirithean

Approved by :

Malee

Approved Signatory

- (☒) Malee Butkruea
(☐) Saithip Meangmai
(☐) Warakorn Lerngagtrakul

Issue Date : 27 January 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Thasarn



Cert.No.: 23CH105

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	9549224	130RC003	221484	17 Apr 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
1413.0 $\mu\text{S/cm}$	CPA Chem	823328	20 June 2023

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 1413.0 $\mu\text{S/cm}$

Conductivity Electrode Serial No.: 5820300339

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (\pm)	Coverage factor k
1413.0 $\mu\text{S/cm}$	1364 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	9.2 $\mu\text{S/cm}$	2.00

Remark

- UUC* = Unit Under Calibration

- Cell constant = 0.550938 cm^{-1}

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Thasorn

Malu

pH Meter

Model : Seven2Go S2

Serial No : B805359649



CERTIFICATE OF CALIBRATION

Certificate No. : 23-055907

Sample Code : 23-21709-001

Customer : Eastern Thai Consulting 1992 Co., Ltd.
129 Moo 1, Suwannasorn Rd., Nonsri,
Kabinburi, Prachinburi 25110

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : pH Meter

Manufacturer : METTLER TOLEDO **Model** : Seven2Go S2

Serial No. : B805359649 **ID No.** : KB-LAB-61-001

Date of Receipt : 25 May 2023 **Date of Calibration** : 25 May 2023

Condition of Calibration

1. Environment

1.1 Ambient temperature : 25.0 \pm 2.5 $^{\circ}\text{C}$ 1.2 Relative humidity : 55.0 % \pm 15.0 %

2. Calibration method

In house method WI-CL-019: based on direct measurement by using standard voltage calibrator and using certified reference material (CRM).

3. Reference standard / Certified reference material

Instrument	ID No.	Certificate No.	Due Date
3.1 Voltage Calibrator	LB-AMC-01	22E3240	03 October 2023
3.2 Digital Thermometer	LB-TH-33	22-107027	02 October 2023
Certified Reference Material	Lot. No.	Ref No.	Expire Date
3.3 Buffer Solution pH 4.008	838357	PH216.L5	15 September 2024
3.4 Buffer Solution pH 6.986	882985	PH107.L5	20 March 2024
3.5 Buffer Solution pH 10.008	838359	PH220.L5	15 September 2023

4. This certificate is traceable to the international system of unit (SI Unit).

- 4.1 Instrument No. 3.1 through Technology Promotion Association (Thailand-Japan).
- 4.2 Instrument No. 3.2 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.
- 4.3 Buffer Solution No. 3.3 and No. 3.5 traceable to CPA chem (through primary measurement method-Harned cell using calibrated thermometer, barometer, and nanovoltmeter Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).
- 4.4 Buffer Solution No. 3.4 traceable to CPA chem (BIM RefN HI-13 LotN 25.05.2022 ; BIM RefN HI-16 LotN 02.06.2022 ; BIM RefN HI-13 LotN 25.05.2022 ; BIM RefN HI-16 LotN 02.06.2022 Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Mr.Anupong Lakawin
Scientist

Approved by (Mr. Somchai Neampunt)
Signed for Director

Issue date 29 May 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



REPORT OF CALIBRATION

Certificate No. : 23-055907

Sample Code : 23-21709-001

Equipment : pH Meter **Resolution** : 0.01 pH ; 1 mV ; 0.1°C
Manufacturer : METTLER TOLEDO **Model** : Seven2Go S2
Serial No. : B805359649 **ID No.** : KB-LAB-61-001
Range : -2.00 pH to 20.00 pH ; ± 1999 mV ; -5.0°C to 105.0°C

Results of Calibration

Part 1. DC Voltage measurement

pH Meter Serial No. : B805359649

Nominal Value pH	Applied DC Voltage mV	Average indicator reading		Uncertainty mV	Coverage factor <i>k</i>
		mV	pH		
0	414.113	414	-0.01	± 0.59	2.00
4	177.477	177	4.00	± 0.59	2.00
7	0.000	0	7.00	± 0.59	2.00
10	-177.477	-177	10.00	± 0.59	2.00
14	-414.113	-414	14.01	± 0.59	2.00

Part 2. Performance of Electrode system

Electrode Manufacturer : METTLER TOLEDO **Model** : InLab Expert Go-ISM
Electrode Serial No. : 2175686 **ID No.** : N/A
Three-Point Calibration at pH4, pH7 and pH10 **Percent Slope** : 98.2

Standard Buffer Solution pH (@ 25 °C)	Average indicator reading		Error Value pH	Uncertainty pH	Coverage factor <i>k</i>
	pH	mV			
4.008	4.02	183	0.012	± 0.010	2.00
6.986	7.00	10	0.014	± 0.010	2.00
10.008	10.02	-165	0.012	± 0.011	2.00

The result expanded uncertainty of measurement *U* is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

REPORT OF CALIBRATION

Certificate No. : 23-055907

Sample Code : 23-21709-001

Equipment : pH Meter (Digital Thermometer with sensor)

Thermometer readout

Manufacturer : METTLER TOLEDO Model : Seven2Go S2
Serial No. : B805359649 ID No. : KB-LAB-61-001
Resolution : 0.1 °C Range : -5.0 °C to 105.0 °C

Thermometer sensor

Manufacturer : METTLER TOLEDO Model : InLab Expert Go-ISM
Serial No. : 2175686 ID No. : N/A

Condition of Calibration

1. Environment
- 1.1 Ambient temperature : 23.0 °C ± 3.0 °C
1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

- 2.1 The calibration use in house method WI-CL-021 : by comparison with standard thermometer
2.2 The calibration by comparison unit under calibration (UUC) to the standard thermometer in a calibration bath at the controlled temperature.
2.3 The temperature scale in use of this laboratory is the international temperature scale of 1990 (ITS-90).

3. Reference standard instrument

Instrument	Model	ID. No.	Certificate No.	Due date
3.1 Platinum Resistance Thermometer	5615-12	LB-TM-22	PSL-T 0199/66	02 January 2024
3.2 Thermometer Readout	1502A	LB-TM-20	PSL-T 0199/66	02 January 2024

4. This certificate is traceable to the international system of unit (SI Unit).

Thailand Institute of Scientific and Technological Research (Accreditation Laboratory Calibration No. 0015)

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibration item : Normal

Results of Calibration

Calibration point °C	Average of standard reading °C	Unit under calibration			Expanded uncertainty °C	Coverage factor k
		Immersion depth mm	Average reading °C	Correction value °C		
0	-0.013	120	-0.3	+ 0.287	± 0.074	2.00
30	29.987	120	30.0	- 0.013	± 0.078	2.00
50	49.984	120	50.0	- 0.016	± 0.078	2.00

Notes

- Calibration results without adjustment

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of report -

Water Bath

Model : WNB22

Serial No : L519.1112

CERTIFICATE OF CALIBRATION

Page 1 of 3

Certificate No. : 23-023261

Sample Code : 23-09257-001

Customer : Eastern Thai Consulting 1992 Co., Ltd.
129 Moo 1, Suwannasorn Rd., Nonsri,
Kabinburi, Prachinburi 25110

Location of Calibration : Eastern Thai Consulting 1992 Co., Ltd.
(Laboratory)

Equipment : Liquid bath (Water bath)

Manufacturer : Memmert

Model : WNB 22

Serial No. : L519.1112

ID No. : KB-LAB-64/002

Date of Receipt : 03 March 2023

Date of Calibration : 03 March 2023

Condition of Calibration

1. Environment	1.1 Ambient temperature	: Maximum	31.7 °C	; Minimum	30.3 °C
	1.2 Relative humidity	: Maximum	49.8 %	; Minimum	39.0 %
	1.3 Line voltage supplied	: Maximum	231.5 VAC	; Minimum	225.8 VAC

2. Calibration method

In-house method WI-CL-023 based on ASTM E 715-80: 2001.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data acquisition with sensor (RTD-Pt100)	LB-DA-11 (RTD-214 to RTD-218)	22-126916	07 December 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Sarawoot Thammo
Scientist

Approved by

(Mr. Somchai Neampunt)
Signed for Director

Issue date

07 March 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

REPORT OF CALIBRATION

Page 2 of 3

Certificate No. : 23-023261

Sample Code : 23-09257-001

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)					Uncertainty ± (°C)	Coverage factor <i>k</i>
			# 1	# 2	# 3	# 4	# 5 ^{Ref.}		
85	85.0	85.0	84.773	84.800	84.802	84.835	84.821	0.18	2.00
95	95.0	95.0	94.821	94.863	94.895	94.916	94.888	0.18	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
85	0.095	0.161	0.281
95	0.100	0.181	0.298

Notes

- UUC* = Unit Under Calibration



REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 23-023261

Sample Code : 23-09257-001

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 Place five calibrated temperature sensors in the unloaded water bath with diffuser plate in place and at lowest position and water level approximately 38 mm from the top.
 - 1.2 Locate one sensor in each of the four corners of the bath approximately 50 mm from each wall and midway between the diffuser plate and the water surface.
 - 1.3 Locate the fifth sensor within 25 mm of the geometric center of the bath.
2. The quoted uncertainty includes "Stability of bath and loading effect in bath at 20% of uniformity".
3. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
4. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
5. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
6. UUC* reading - the average reading of indicating device that forms the integral part of the bath.
7. Controlled circulation or stirrer motor setting : N/A
8. Cooling system : N/A
9. Calibration results without adjustment.

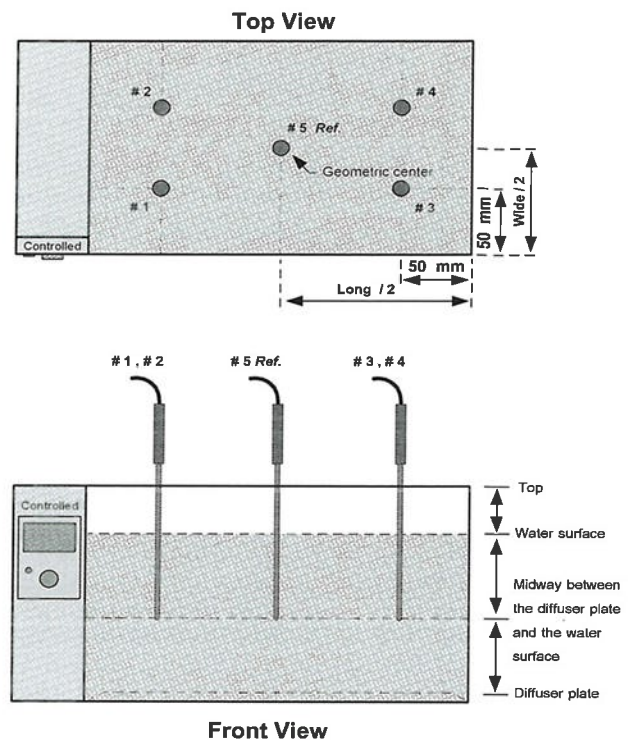


Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

DO METER

Model : YSI5000

Serial No. : 16H102702

CERT.No.: HS-U072J

Harikul Science Co.,Ltd.

694 Soi Ratchadanivet 24, Pracharatbamphen,

Samsaennok, Huaikhwang, Bangkok 10310

Tel: 0-2274-2456 Fax: 0-2274-2443

Email: info@harikul.com www.harikul.com

Certificate of Calibration

Calibration Date : 12 Oct 23

Submitted by : Eastern Thai Consulting 1992 Co., Ltd.

129 Moo 1, Nonsi Subdistrict, Kabinburi

District Prachinburi Province 25110

Avg Room Temp : 20 °C

Avg Water Temp : 20 °C

Air Pressure : 760.00 mmHg

Salinity : 0 ppt

Model : YSI 5000

S/N : 16H102702

Probe : YSI 5010

S/N : 22A00334

ID NO. :

Air Temp ref : S/N. F8065C26

Barometric ref : S/N. F8065C26

Water Temp ref : S/N. 11430

Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.09	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.07	(PASS)	-
Mean Measurement	9.08	mg/l	-
Inaccuracy	0.01	mg/l	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



Technician Signature

(Kittipong Maekwong)




Laboratory Manager

(Natenapha Pisatkunchon)

Digital Thermohygro Meter

Model : 303C

Serial No : 200603234

CERTIFICATE OF CALIBRATION

Page 1 of 2

Certificate No. : 23-132793

Sample Code : 23-49490-001

Customer : Eastern Thai Consulting 1992 Co., Ltd.
129 Moo 1, Suwannasorn Rd., Nonsri,
Kabinburi, Prachinburi 25110

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration laboratory)

Equipment : Digital thermo-hygrometer

Manufacturer : N/A

Model : 303C

Serial No. : 200603234

ID No. : KB-LAB-63/026

Date of Receipt : 13 November 2023

Date of Calibration : 20 November 2023

Condition of Calibration

- 1. Environment**
- | | |
|-------------------------|--------------------|
| 1.1 Ambient temperature | : 23.0 °C ± 3.0 °C |
| 1.2 Relative humidity | : 55.0 % ± 15.0 % |

2. Calibration method

- 2.1 In-house method: WI-CL-045 By comparison with thermometer standard / chilled mirror hygrometer in controlled chamber.
2.2 The calibration by comparison unit under calibration (UUC) to the thermometer standard / chilled mirror hygrometer in a chamber at the controlled temperature / relative humidity.

3. Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Chilled Mirror	Optidew 401	LB-DP-03 & LB-DP-03 (DP)	TH-0064-23	07 August 2024
3.2 Digital Thermometer	Optidew 401	LB-DP-03 & LB-DP-03 (Temp.)	23-103423	03 September 2024
3.3 Digital Thermometer	34972A	LB-DA-07 with RTD-89	23-101374	05 September 2024

4. This certificate is traceable to the international system of unit (SI Unit).

- 4.1 Instrument No. 3.1 through National Institute of Metrology (Thailand).
4.2 Instrument No. 3.2 and 3.3 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Miss Pornsuda Lohabal
Scientist

Approved by

(Mr. Somchai Neampunt)
Signed for Director

Issue date 22 November 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

REPORT OF CALIBRATION

Page 2 of 2

Certificate No. : 23-132793

Sample Code : 23-49490-001

Results of Calibration

Temperature measurement

Resolution : 0.1 °C

Range : -50 °C to 70 °C

Calibration point °C	Average of standard reading		Unit under calibration		Expanded uncertainty °C
	Controlled humidity %RH	Temperature °C	Average reading °C	Correction value °C	
20	50	20.00	19.9	+ 0.10	± 0.39
25	50	25.00	24.8	+ 0.20	± 0.39
30	50	30.00	29.7	+ 0.30	± 0.39

Humidity measurement

Resolution : 1 %RH

Range : 10 %RH to 95 %RH

Calibration point %RH	Average of standard reading		Unit under calibration		Expanded uncertainty %RH
	Air temperature °C	Calculated humidity %RH	Average reading %RH	Correction value %RH	
45	25.01	45.13	39	+ 6.13	± 1.3
60	25.03	59.96	48	+ 11.96	± 1.5
75	25.02	75.06	62	+ 13.06	± 1.7

Notes

- Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -



HOT AIR OVEN

Model : UF110

Serial No. : B420.0827

CERTIFICATE OF CALIBRATION

Certificate No. : 23-117652

Sample Code : 23-433253-003

Customer : Eastern Thai Consulting 1992 Co., Ltd.
129 Moo 1, Suwannasorn Rd., Nonsri,
Kabinburi, Prachinburi 25110

Location of Calibration : Eastern Thai Consulting 1992 Co., Ltd.
(Laboratory)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Memmert **Model** : UF 110

Serial No. : B420.0827 **ID No.** : KB-LAB-63/008

Date of Receipt : 05 October 2023 **Date of Calibration** : 05 October 2023

Condition of Calibration

1. Environment	1.1 Ambient temperature	: Maximum	32.7 °C	; Minimum	30.4 °C
	1.2 Relative humidity	: Maximum	72.0 %	; Minimum	66.7 %
	1.3 Line voltage supplied	: Maximum	224.6 VAC	; Minimum	221.6 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data acquisition with sensor (RTD-Pt100)	LB-DA-12 (RTD-168 to RTD-176)	23-043820	03 May 2024

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Mr. Nophanon Anusak
Scientist

Approved by (Mr. Somchai Neampunt)
Signed for Director

Issue date 09 October 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

REPORT OF CALIBRATION

Certificate No. : 23-117652

Sample Code : 23-433253-003

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor <i>k</i>
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 ^{Ref}		
85	85.0	85.0	85.00	84.50	85.16	84.99	85.12	85.10	85.09	84.76	85.11	0.26	2.00
104	104.0	104.0	103.98	103.48	104.19	103.90	104.10	104.10	104.20	103.52	104.11	0.47	2.00
150	150.0	150.0	149.71	149.02	150.14	149.57	149.87	149.92	150.24	149.01	149.92	0.53	2.00
180	180.0	180.0	179.59	178.78	180.09	179.59	179.74	179.83	180.29	178.71	179.82	0.57	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
85	0.10	0.64	0.77
104	0.26	0.68	1.14
150	0.25	1.04	1.73
180	0.28	1.23	1.95

Notes

- UUC* = Unit Under Calibration




REPORT OF CALIBRATION

Certificate No. : 23-117652

Sample Code : 23-433253-003

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 56 cm ; D = 40 cm ; H = 48 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes" Stability of chamber and loading effect in chamber at 20% of uniformity ".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.


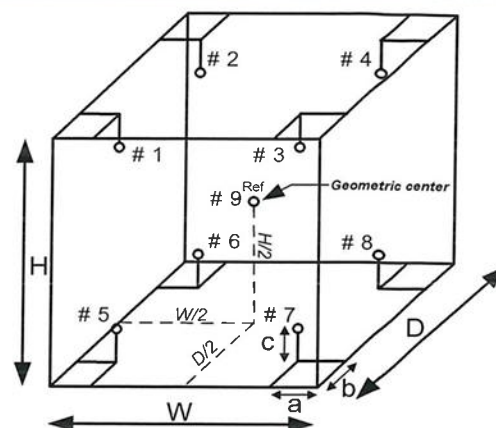


Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -




Dissolved Oxygen and BOD

Model : HI98193

Serial No : 03500057101

Certificate No. : HIT-2321-0645

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment : Dissolved Oxygen and BOD Meter

Meter Model : HI98193 **Serial No. :** 03500057101

Probe Model : HI764073 **Serial No. :** KC1N42MCK

Manufacturer : Hanna Instruments **Made in :** Romania

Condition As-Received : Used Product **Reference :** RE230826

Customer name : Eastern Thai Consulting 1992 Co., Ltd. (Branch 00002)
129 Moo. 1, Nonsi Kabinburi, Kabinburi,
Prachinburi 25110

Received date : 24 May 2023

Calibrate date : 26 May 2023

Issue date : 26 May 2023

Ambient Temperature : $(25 \pm 2)^{\circ}\text{C}$

Relative Humidity : $(50 \pm 15)\% \text{ RH}$

Calibrated Location : Hanna Instruments (Thailand) Ltd.

Calibration Procedure : This calibrator was conducted by using in-house: calibration procedure
CP-11 by using certified reference material (CRM)

Calibrated by : ☒ Mr. Pichit Petthong
☐ Mr. Jakkapob Pentisan
☐ Mr. Channarong Soinak

Approved by : 
Mr. Anan Suwanchaisakul

Authorizer Signatory



This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

**** This certificate may not be reproduced other than in full, except with the prior written ****

approval of the head of Hanna Instrument (Thailand)



Condition of this calibration result

Reference Standard Instruments : This certification is traceable to the International unit of thru Technology Promotion Association (Thailand-Japan).

Instruments	Model	Serial No.	Certificate No.
Thermometer with sensor	HI98509	39643D	22T1521

Standard Dissolved Oxygen Buffer Solution :

Zero Oxygen Solution	Model No.	Mean Value	Ref. No.	Lot Number	Exp. date
HI7040L	HI7040L	0.0 ± 0.1@25°C	20A33	S0008/23	December 2027

Calibration Result

Inspection the accuracy of the Dissolved Oxygen (DO) Meter by using the following certificate reference material value.

Unit Under Calibration	CRM Standard DO	Actual value Reading	Error value Reading	Uncertainty of Measurement (±)
Electrode Model Serial : KC1N42MCK	0 mg/L	0.00 mg/L	0.00 mg/L	N/A
	8.3 mg/L	8.25 mg/L	-0.05 mg/L	0.33 mg/L

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

**** End of certificate ****



SOUND LEVEL CALIBRATOR

MODEL : NC-75

SERIAL No. : 34302326

Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 30/0267	13-FEB-24
Digital Multimeter	33461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24
Audio Analyzer	AVR-3360A	V744B6069	EF-0012-23	10-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

NSC-TS1-TIS 17025
CALIBRATION 0394SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

451-451/1 Srinthorn Rd, Bangbunmu, Bangplud Bangkok 10700 THAILAND.

Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com

Cert. No. : ACC23013

Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR

Manufacturer : RION

Model : NC-75

Serial No.: 34302326

ID No.:

Condition As Found :

GOOD

Customer :

EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :

Ambient Temperature :

(23.0 \pm 3) °C

Pressure :

(101.3 \pm 3) kPa

Relative Humidity :

(50.0 \pm 20) %

Received Date :

10 MAY 2023

Calibration Date :

19 MAY 2023

Date of Issue :

24 MAY 2023

Calibrated by :

Nathakom Pisutpaisan

Approved by :

T. Petchurai

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

COPY

Continuation of Calibration Certificate

Cert. No. : ACC23013
Job No. : VC66AC0058
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.03	0.03	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
0.32	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 01120946

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd. Banglumru, Bangkok 10700 THAILAND.
Tel.0-2433-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



NSC-TS-17025
CALIBRATION 0394

Cert No. : ACL23097
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 01120946 / 21952 / 22335
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 24 JANUARY 2023
Calibration Date : 26-30 JANUARY 2023
Date of Issue : 01 FEBRUARY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23097
Job No. : VC66AC0035
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAJ	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY



Continuation of Calibration Certificate

Cert. No. : ACL23097
Job No. : VC66AC0035
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

COPY

7. Reten

Continuation of Calibration Certificate

Cert. No. : ACL23097
Job No. : VC66AC0035
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	10.8
C - weight	15.6
Flat	21.2

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.1	0.1	0.1
1000	0.1	0.1	0.1
8000	-0.1	0.0	0.0
			Acceptance Limits
			± 1.0
			± 0.7
			+ 1.5, - 2.5

COPY

7. Reten

Continuation of Calibration Certificate

Cert. No. : ACL23097
Job No. : VC66AC0035
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
63	0.0	0.0	±1.0
125	0.0	0.0	±1.0
250	0.0	0.0	±1.0
500	0.0	0.0	±1.0
1000	0.0	0.0	±1.0
2000	0.0	0.0	±1.0
4000	0.0	0.0	±1.0
8000	0.0	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

Continuation of Calibration Certificate

Cert. No. : ACL23097
Job No. : VC66AC0035
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.1	0.1	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.1	0.1	±0.8
29.0	29.0	0.0	±0.8
28.0	28.0	0.0	±0.8
27.0	27.0	0.0	±0.8
26.0	26.1	0.1	±0.8
25.0	25.0	0.0	±0.8

Continuation of Calibration Certificate

Cert. No. : ACL23097
Job No. : VC66AC0035
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.1	-0.3	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

COPY

7. Retin

Continuation of Calibration Certificate

Cert. No. : ACL23097
Job No. : VC66AC0035
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle			
89.8	89.6	-0.2	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

7. Retin

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 01120947

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Srinthorn Rd.,Bangbunru, Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



NSC-TS1-TIS 17025
CALIBRATION 0394

Cert. No. : ACL23098
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 01120947 / 21960 / 22336
ID No.:

Condition As Found : GOOD
Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 24 JANUARY 2023
Calibration Date : 26-30 JANUARY 2023
Date of Issue : 01 FEBRUARY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY



Continuation of Calibration Certificate

Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 3 of 8Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 4 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	9.9
C - weight	15.5
Flat	21.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.2	0.2	0.2
1000	0.1	0.1	0.1
8000	-0.4	-0.4	-0.3
			Acceptance Limits
			± 1.0
			± 0.7
			+ 1.5, - 2.5

COPY

Continuation of Calibration Certificate

Cert No. : ACL23098
Job No. : VC66AC0035
Pages : 5 of 8Cert No. : ACL23098
Job No. : VC66AC0035
Pages : 6 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	0.0	0.0	0.0
125	0.0	0.0	0.0
250	0.0	0.0	0.0
500	0.0	0.0	0.0
1000	0.0	0.0	0.0
2000	0.0	0.0	0.0
4000	0.0	0.0	0.0
8000	0.0	0.1	0.1
16000	0.0	-1.2	-1.2

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.1	0.1	±0.8
84.0	84.1	0.1	±0.8
79.0	79.0	0.0	±0.8
74.0	74.1	0.1	±0.8
69.0	69.1	0.1	±0.8
64.0	64.0	0.0	±0.8
59.0	59.1	0.1	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.0	0.0	±0.8
29.0	29.0	0.0	±0.8
28.0	28.0	0.0	±0.8
27.0	27.0	0.0	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.9	-0.1	±0.8

Continuation of Calibration Certificate

Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.2	-0.2	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

Continuation of Calibration Certificate

Cert. No. : ACL23098
Job No. : VC66AC0035
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	-0.1	±1.5
89.6	89.5		

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

g. Retin

COPY

g. Retin

ANALYTICAL BALANCE (DU)

Model. : XS205DU

Serial No. : 1126323724



Certificate No. :

23-006683

Sample Code :

23-02820-006

Page 1 of 4

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriacha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : 1126323724

ID No. : LABE 05/1

Date of Receipt : 20 January 2023

Date of Calibration : 20 January 2023

Calibrated by Mr. Thanadol Pholthep
Scientist

Issue date 25 January 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)



REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Capacity : Max 81 g / 220 g

Resolution : 0.01 mg / 0.1 mg

Serial No. : 1126323724

ID No. : LABE 05/1

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 80	Before adjustment	After adjustment
<input checked="" type="checkbox"/> No adjustment	Nominal value	40	90
<input type="checkbox"/> Adjustment	Standard weight	40.000042	80.000045
	Average reading of indicator	40.00015	90.00019
	Standard deviation	0.000004	0.000007
Unit : g	Range : 200	Before adjustment	After adjustment
<input checked="" type="checkbox"/> No adjustment	Nominal value	100	200
<input type="checkbox"/> Adjustment	Standard weight	100.000022	200.000199
	Average reading of indicator	100.0001	200.0004
	Standard deviation	0.00004	0.00008



Certificate No. : 23-006683

Sample Code : 23-02820-006

NSC-TIS-1517025
CALIBRATION 0152

Page 3 of 4

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 80		Range : 200	
Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	0.99800	0	0.9980
40	0.99800	100	0.9980
80	0.99800	200	0.9980

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.00000	0.00000	0.0000090	2.01
0.01	0.0100036	0.01000	0.00000	0.0000093	2.01
0.1	0.1000062	0.10000	0.00001	0.000012	2.00
1	1.0000036	1.00001	-0.00001	0.000014	2.00
5	5.0000044	5.00003	-0.00003	0.000020	2.00
10	10.0000000	10.00007	-0.00007	0.000032	2.00
20	20.000016	20.00011	-0.00009	0.000036	2.00
50	50.000029	50.00013	-0.00010	0.000067	2.00
100	100.000022	100.00001	-0.00001	0.00016	2.00
150	150.000051	150.00001	0.00000	0.00023	2.00
200	200.000199	200.00003	-0.00001	0.00028	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-064

TEL 02-516-2422

FAX 02-516-6949
Rev.03

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH
Effective Date: 15/10/21NSC-TIS-151702
CALIBRATION 015

Page 4 of 4

Certificate No. : 23-006683

Sample Code : 23-02820-006

REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off-center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan ☐ Circle ☐ Triangular ☒ Rectangular
Test weight : 50 and 100
Unit : g

Range	Position	Reading of indicator	Reading of indicator
80	1	50.00014	100.00001
200	2	50.00014	99.99998
	3	50.00006	100.00000
	4	50.00010	100.00001
	5	50.00017	100.00001
	6	50.00014	100.00001
Maximum difference		0.00008	0.00003

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : *

* Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument

1) STANDARD WEIGHT 1 mg to 1 kg

Class

E2

ID.No.

LB-WE-57

Certificate No.

22-060639

Due Date

27 June 2023

- End of Report -

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-064

TEL 02-516-2422

FAX 02-516-6949
Rev C3

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH
Effective Date: 15/10/21


ATOMIC ABSORPTION SPECTROPHOTOMETER

Model : PinAAcle 900F

Serial No. : PFBS22080801

PinAAcle 900F Preventive Maintenance (PM)

Company Name:	Eastern Thai Consulting 1992 Co.,Ltd.		
Address (Instrument Location):	683 Moo 11 Sukapibal 8 Rd. Nong Kham,Si Racha, Chonburi 20230		
Serial Number:	PFBS22080801	PM Number:	2 of 2
Customer Name (if applicable):		Telephone Number:	
Customer Support Engineer Name:	Khwanchai	Service Order Number:	WO-01886639
Date PM Performed: (DD-MMM-YY)	24-Oct-2023	Next PM Due Date: (DD-MMM-YY)	24-Apr-2024
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	 PerkinElmer®
09370145 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.
Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.

The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.

Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved.

No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.

Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes
FIAS100		

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	NA
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	NA
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	NA
N9301714	Replacement Acetylene Filter Cartridge	NA
TH001022	Replacement Air Filter Cartridge	NA

Additional Reagents and Standards Required for PM

Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	26-87CUI1	30-Jan-2024

Additional Reagents and Standards Required for PM (Customer Support Solution)

Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 ml.	AR	AR
N/A	0.5% HNO ₃	250 ml.	AR	AR

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Perform general inspection of system for cleanliness.

2. PC Instrument Software:

- ☒ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. Mechanical:

- ☒ Inspect and clean all fans and filters. Replace filters if necessary.
- ☒ Inspect all gas lines for leaks and/or wear. Replace if needed.
- ☒ Clean exterior of the instrument.
- ☒ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ☒ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking slot width. Replace if out of specification.
- ☒ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ☒ Check the drain system for signs of wear. Replace worn or damaged parts.
- ☒ Visually check for proper flame conditions when lighting the Air-C2H2 and N2O-C2H2 flames (if applicable).

4. Electrical:

- ☒ Inspect PC boards. Clean if necessary.
- ☒ Carefully check all internal and external cable connections.
- ☒ Check instrument firmware revisions upgrade to current levels (if necessary).
- ☒ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer EM Log Viewer.

5. Optics:

- ☒ Inspect and clean the sample compartment windows, if needed.
- ☒ Inspect optics. Clean or replace if necessary.

6. Gases:

- ☒ Verify that the Gases supplied to the instrument are within the pressure and purity specifications found in the PinaAde 900 Series Pre-Installation Checklist SDB.
- ☒ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

Additional Tools Required for PM

Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	MG0-056
N1013002	1.0A Neutral density filter	1	MG2-054
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	092216-010130
N3050109	Ba Lumina HCL	1	102416-040160
N3050139	K Lumina HCL	1	110716-010060
N3050152	Ni Lumina HCL	1	100516-030190

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Pass
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Pass
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Pass
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Pass
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Pass
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Pass

8. After PM Performance tests:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	1.0531	1.0230	Pass
0.2 A ND Filter	± 5% from Cert.	0.1806	0.1783	Pass

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0015	Pass

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Pass

8.4 D₂ Background Compensation with Copper

Description: Verifies the instruments ability to compensate for background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0054	Pass

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0001	Pass

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0002	Pass

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	NA	NA
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	0.3878	Pass

10. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.	
This PinAAcle 900F Passes <input checked="" type="checkbox"/> Fails <input type="checkbox"/> the preventive maintenance.	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative:	Date: 24-Oct-2023 (DD-MM-YY)
Authorized Customer Representative:	Date: 24-Oct-2023 (DD-MM-YY)

COPY

BAROMETER

Equipment : Analog Barometer

ID No. / Tag No. : BM001/41



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mtl.in.th>



CALIBRATION CERTIFICATE

Certificate No. : L202305085-002
Date Issued : 16-May-23

Customer : Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11 Sukhapiarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment : Analog Barometer

Manufacturer : Barigo
Model : -
Serial No. : -
ID No./Tag No. : BM001/41
Date Received : 11-May-23
Date Calibrated : 15-May-23

Calibrated by : Mr. Jame Khaothong

Calibration Method or Calibration Procedure Used

In-house method : CP-21 base on DKD-R 6-1: Edition 3 2014.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: *Sorayuth T.*
(Mr. Sarayuth Tochua)



Page 1 of 2

Certificate No. : L202305085-002

Environment : Ambient Temperature : $(25 \pm 2)^{\circ}\text{C}$

Relative Humidity : $(50 \pm 15)\%\text{RH}$

STD Reading mbar	UUC Reading (mbar) Before Adjusted	UUC Reading (mbar) After Adjusted	UUC Error mbar	Uncertainty \pm mbar
990.00	990.0	-	0.00	0.61
1000.00	1000.0	-	0.00	0.61
1010.00	1010.0	-	0.00	0.61
1020.00	1020.0	-	0.00	0.61
1030.00	1030.0	-	0.00	0.61

STD = Standard

UUC = Unit Under Calibration

Calibrated condition :

Pressure Medium : Air : Density = 1.19 kg/m^3 @ 20°C , 1 bar
Mounting Position : Vertical
Reference Level : at center of its dial
Conversion Factor : Multiply by $1.0 \text{ E}+02$ - Pa unit

Description of UUC :

Range : 990 - 1030 mbar Absolute
Calibration Range : 990 - 1030 mbar Absolute
Scale Interval : 1 mbar
Resolution : 0.5 mbar Absolute

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

IRPC Certificate No. CL1-P220104 for Reference Pressure Monitor Serial No. 1598, Due 11-Nov-23

End of Certificate

Page 2 of 2

COPY

COPY

CERTIFICATE OF ANALYSIS

EPA PROTOCOL GAS

Cylinder No. : EB0145030



Airgas Specialty Gases
Airgas USA, LLC
6141 Easton Road
Bldg 2
Plumsteadville, PA 18949
airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E03NI99E15AC004
Cylinder Number: EB0145030
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12021
Gas Code: CH4,PPN,BALN
Reference Number: 160-40224242-1
Cylinder Volume: 144.4 CF
Cylinder Pressure: 2015 PSIG
Valve Outlet: 350
Certification Date: Oct 15, 2021
Expiration Date: Oct 15, 2029

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 800/R-12/001, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder Below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS				
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty
METHANE	180.0 PPM	177.0 PPM	G1	+/- 1.0% NIST Traceable
PROPANE	185.0 PPM	187.0 PPM	G1	+/- 1.0% NIST Traceable
NITROGEN	Balance			
CALIBRATION STANDARDS				
Type	Lot ID	Cylinder No	Concentration	Uncertainty
INTRM	08011503	K002564	246.7 PPM METHANE/AIR	+/- 0.6%
INTRM	200602-06	6162660Y	243.3 PPM PROPANE/AIR	+/- 0.5%
ANALYTICAL EQUIPMENT				
Instrument/Make/Model			Analytical Principle	Last Multipoint Calibration
Nicolet IS50 FTIR AUP2110295 CH4			FTIR	Oct 13, 2021
Nicolet IS50 FTIR AUP2110295 C3H8			FTIR	Oct 14, 2021

Triad Data Available Upon Request

NOTES:

Gross Weight: 28.0 Kg
Net Weight: 4.9 Kg
PO# 5221004861



COPY

Michael A. Harkins

Approved for Release

DRY GAS METER MC-572V

Serial No. : 0504003

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m³)

Meter Console Information

Console Model: MC572V
 Console Serial: 0504003
 DGM Model #: SK25EX
 DGM Serial #: 0009854

Calibration Condition

Calibration Date: 3-Apr-23
 Issue Date: 3-Apr-23
 Cal. Report No.: WDS-SV680039
 Ambient Temp (°C): 25
 Pressure (mm Hg): 758
 Relative Humidity (%): 60

Factors/Conversion

Std. Temp (°K): 298
 Std. Pressure (mm Hg): 760
 K₁ (K/mm Hg): 0.3857

Reference Equipment

WTM Model: W-NKoDa-5B WTM Cal. Due Date: Nov. 2022
 WTM Serial: 600245 Gamma: 1.0000

UUT Meter (DGM)

Reference Meter (WTM)

Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
0	P _{atm}	V _{ini}	V _{fin}	t _{ini}	t _{fin}	V _{ini}	V _{fin}	t _{ini}	t _{fin}
15.00	13.0	2.1249	2.2873	26	26	11.24924	11.40853	25	25
10.00	25.0	1.9384	2.0964	26	26	11.06645	11.22136	25	25
8.00	50.0	1.7294	1.9105	26	26	10.86093	11.03905	25	25
7.00	80.0	1.4887	1.6921	26	26	10.62322	10.82407	25	25
5.00	120.0	1.1950	1.3736	26	26	10.33100	10.50914	25	25

Standardized Data

Calibration Results

Test Meter		Reference Meter		Correction Factor		Flow Rate		
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std. & Corr	0.0212 SCMM	Variation
V _{std} (m ³)	Q _{std} (m ³ /min)	V _{ref} (m ³)	Q _{ref} (m ³ /min)	(Y)	(ΔY)	Q _{std/corr}	ΔH ₂	ΔΔH ₂
0.159	0.011	0.156	0.010	0.983	-0.001	0.010	52.990	5.531
0.155	0.015	0.152	0.015	0.981	-0.002	0.015	47.999	0.540
0.178	0.022	0.175	0.022	0.982	-0.002	0.022	46.896	-0.763
0.200	0.029	0.197	0.028	0.983	-0.001	0.028	45.249	-2.210
0.177	0.035	0.175	0.035	0.989	0.006	0.035	44.361	-3.098
				0.984	= Y Avg		47.459	= ΔH ₂ Avg

Pass/Fail Result: **Pass**

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptably between 0.98 and 1.02.

Note: For ΔH₂, orifice pressure differential that equates to 0.75scfm (0.0212m³/min) at standard temperature and pressure. For acceptable variation of individual values from the average is ±0.2 inches (5.1mm) H₂O.


Approved By: _____

(Patpasu Chaisana)
 Service Manager

Date: 3-Apr-23

COPY

Meter Gamma vs Flowrate

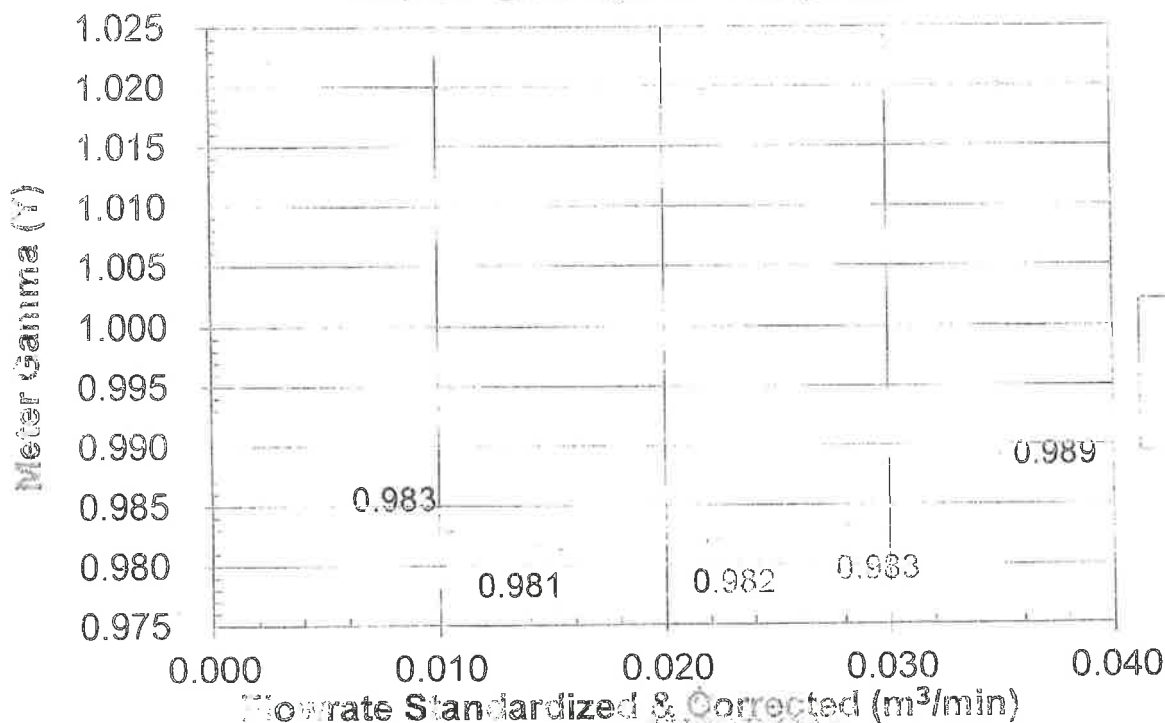

COPY

WDS

WISDOM SCIENCE

Meter Console Information

Console Model : MC572V
 Console serial : 0504003
 Temp Indicator Model : 765-KF
 Temp. Indicator Serial : JC17852

Calibration Conditions

Cal. Date : 3-Apr-23
 Issue Date : 3-Apr-23
 Cal. Report No. : WDS-SV660039
 Ambient Temp. (°C) : 25
 Pressure (mm Hg) : 758
 Humidity (%) : 60

Reference Equipment

Temp. Simulator Model : FLUKE 714B
 Serial No : 60590035

Temperature Sensor Calibration

Reference Point	Ref. Temperature	Temp. Difference
#	°C	°C
1	-18.0	-17.0
2	38.0	37.0
3	93.0	92.0
4	149.0	148.0
5	260.0	259.0
6	371.0	372.0
7	482.0	482.0
8	593.0	594.0
9	816.0	816.0
10	1038.0	1038.0
Maximum		1.0

P-107

Note

For valid test results, the maximum difference between temperature readings should $\leq 1.0^{\circ}\text{C}$ (EPA Method 5, Section 6.1.1.8).
 Perform all TC Channel calibrations. Except meter (DGM) channel

DGM Out Temperature Sensor Calibration

Temperature point	Ref. Temperature	Temp. Difference
#	°C	°C
Ambient	26.5	26.0
Heat	100.5	102.0


Difference Rang

DGM Out Temp. Diff. $\pm 3^{\circ}\text{C}$

PASS

Approved By :

(P. Chaisena :
 Service Manager

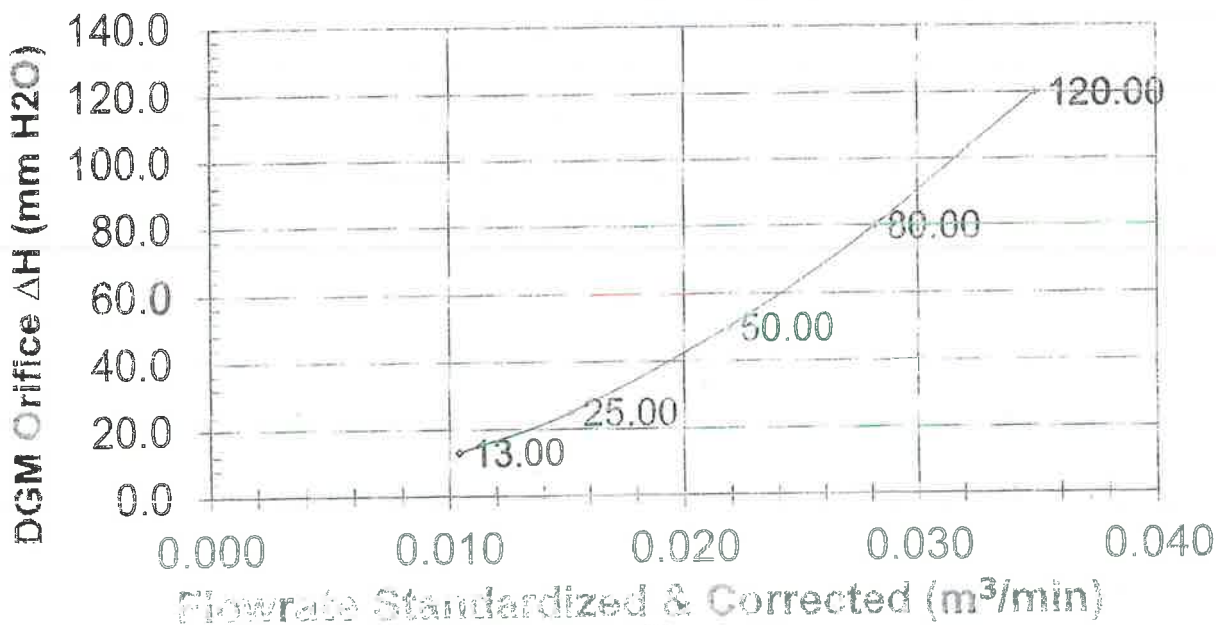Meter Pressure vs Flowrate

Console Serial:

0504003

Console Model:

MC572V

บริษัท วิสโดม ไซนซ์ จำกัด
 WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

COPY

DRY GAS METER XC-572-OV

Serial No. : A2204323



WISDOM SCIENCE
SALE AND SERVICE GROUP COMPANY LIMITED

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m)

Meter Console Information

Console Model : XC-572-OV
Console serial : A2204323
DGM Model # : SK25EX
DGM Serial # : 00008294

Calibration Condition

Calibration Date : 2-May-2023
Due Date : 1-May-2024
Cal. Report No. : WDS-SV660066
Ambient Temp (°C) : 25
Pressure (mm Hg) : 756
Relative Humidity (%) : 55

Factors/Conversion

Std. Temp. (°K) : 298
Std. Pressure (mm Hg) : 760
K₁ (K/mm Hg) : 0.3857

Reference Equipment

WTM Model : W-NKoDa-5B
WTM Serial : 600245
WTM Cal. Date : 22-Nov-2022
Gamma : 1.0000

Run Time (minutes)	DGM Orifice (mm H ₂ O)	UUT Meter (DGM)				Reference Meter (WTM)			
		Volume		Outlet Temp		Volume		Outlet Temp	
		Initial V _{ini}	Final V _{fin}	Initial t _{ini}	Final t _{fin}	Initial V _{ref}	Final V _{ref}	Initial t _{ini}	Final t _{fin}
15.00	13.0	18.0685	18.2252	25	26	17.55844	17.71573	25	25
10.00	25.0	18.2477	18.3984	25	26	17.73837	17.88948	25	25
8.00	50.0	18.4339	18.6056	25	26	17.92517	18.09730	25	25
7.00	80.0	18.6458	18.8344	25	27	18.13775	18.32707	25	25
5.00	120.0	18.8839	19.0510	25	27	18.37705	18.54528	25	25

Standardized Data				Calibration Results				
Test Meter		Reference Meter		Correction Factor		Flow Rate	ΔH@ (mm H ₂ O)	
Std. Volume V _{std} (m ³)	Std. Flow Rate Q _{std} m ³ /min	Std. Volume V _{ref} (m ³)	Std. Flow Rate Q _{ref} m ³ /min	"Gamma" (Y)	Variation (ΔY)	Std & Corr Q _{std} (m ³ /min)	0.0212 SCMM ΔH ₀	Variation ΔΔH ₀
0.154	0.010	0.154	0.010	1.004	0.003	0.010	54.437	3.293
0.148	0.015	0.148	0.015	1.002	0.001	0.015	50.528	-0.616
0.169	0.021	0.169	0.021	0.999	-0.001	0.021	50.086	-1.058
0.186	0.027	0.186	0.027	0.999	-0.001	0.027	50.928	-0.216
0.165	0.033	0.165	0.033	0.999	-0.002	0.033	49.741	-1.403
				1.001	= Y Avg.			
							51.144	= ΔH@ Avg

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance is ±0.02

Note: For ΔH₀, orifice pressure differential that equates to 0.75cm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O.

Pass/Fail Result: **PASS**


Approved By: _____

(Patpasu Chaisana)
Service Manager

WISDOM SCIENCE
บริษัท วิสโดม ซาเล และ เซอร์วิส กรุ๊ป จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Date: 2-May-2023

COPY

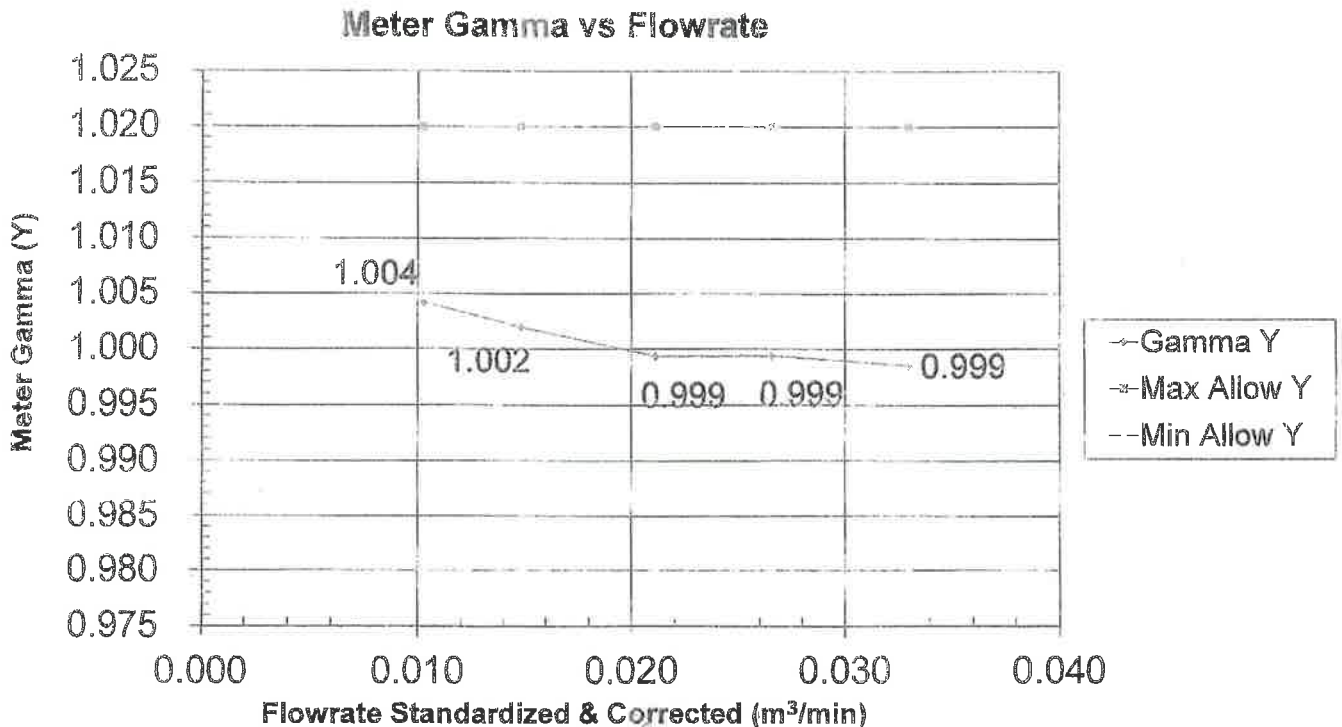

Console Serial:

A2204323

Console Model:

XC-572-OV

WISDOM SCIENCE

บริษัท วิสโดม ซาเล และ เซอร์วิส กรุ๊ป จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY



WISDOM SCIENCE

TEMPERATURE DISPLAY CALIBRATION

Meter Console Information

Console Model : XC-572-OV
Console Serial : A2204323
Temp. Indicator Model : 765-KF
Temp. Indicator Serial : JC19022

Calibration Conditions

Cal. Date : 2-May-2023
Due Date : 1-May-2024
Cal. Report No. : WDS-SV660066
Ambient Temp. (°C) : 25
Pressure (mm Hg) : 758
Humidity (%) : 55

Reference Equipment

Temp. Simulator Model : FLUKE 7-48
Serial No. : 60590035
Calibration Date : 14-Feb-2023

Temperature Sensor Calibration

Reference Point	Ref. Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
1	-18.0	-17.0	1.0
2	25.0	25.0	0.0
3	90.0	90.0	0.0
4	120.0	120.0	0.0
5	250.0	249.0	1.0
6	380.0	380.0	0.0
7	500.0	500.0	0.0
8	620.0	620.0	0.0
9	740.0	739.0	1.0
10	860.0	860.0	0.0
Maximum ¹			1.0

Note

¹ For valid test results, the maximum difference between temperature readings should be $\leq 1.0^{\circ}\text{C}$ (EPA Method 5, Section 6.1.1.8).
Perform AUX, STACK, PROBE, OVEN, FILTER, EXIT. Except meter (DGM) channel

DGM Out Temperature Sensor Calibration

Temperature point	Ref. Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
Ambient	28.8	29.0	-0.2
Heat	100.0	101.3	-1.3

Difference Range


DGM Out Temp. Diff. $\pm 3^{\circ}\text{C}$

Approved By :

Pabsei Chaisana
Service Manager

WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED
Address 9/115 Lumpini Town Ville Ratchapruk-Pinklao Village No. 4, Bang Kruai, Nonthaburi 11130 Thailand

Meter Pressure vs Flowrate

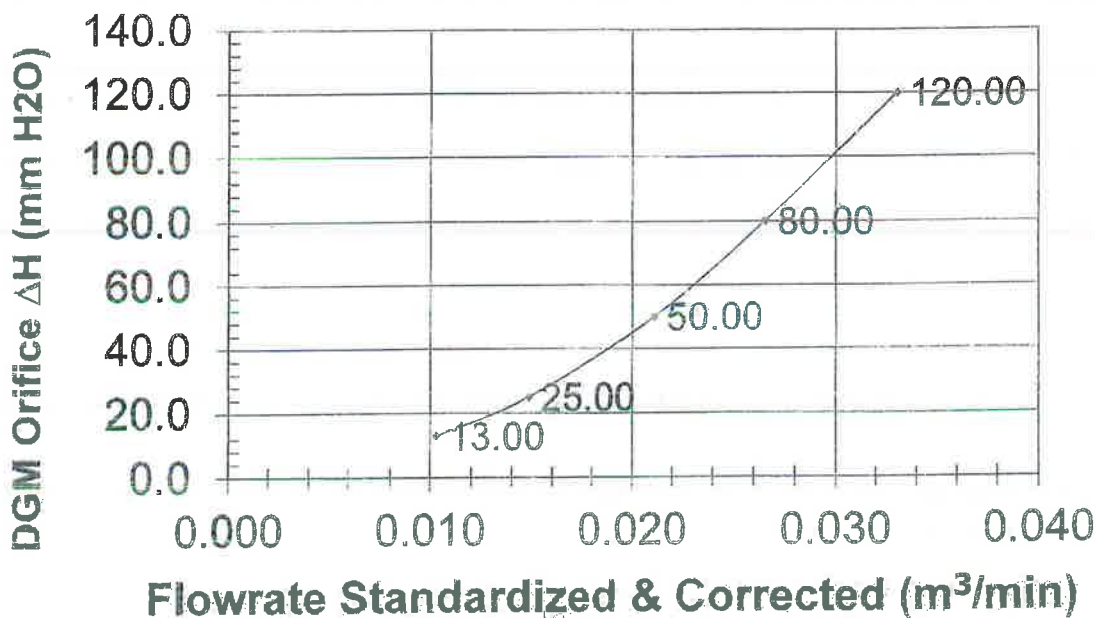

Console Serial:

A2204323

Console Model:

XC-572-OV

บริษัท วิสโดม ไซนซ์ แอนด์ เซอร์วิส กรุ๊ป จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

COPY

DRY GAS METER XC572V

Serial No. : 1110070

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

Meter Console Information

Console Model : XC572V
 Console serial : 1110070
 DGM Model #: SK25EX
 DGM Serial #: 0005413

Calibration Condition

Calibration Date: 3-Jul-23
 Due Date: 2-Jul-24
 Cal. Report No.: WDS-SV660107
 Ambient Temp (°C): 25
 Pressure (mm Hg): 758
 Relative Humidity (%): 80

Factors/Conversion

Std. Temp. (°K): 298
 Std. Pressure (mm Hg): 760
 K₁ (K/mm Hg): 0.3857

Reference Equipment

WTM Model: W-NKoDa-5B WTM Cal. Due Date: Nov. 2022
 WTM Serial: 600245 Gamma: 1.0000

UUT Meter (DGM)

Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
15.00	13.0	599.3828	599.5462	27	27	20.05690	20.22163	28	27
10.00	25.0	599.5889	599.7246	27	26	20.24425	20.39999	27	27
6.00	50.0	599.7405	599.9176	26	26	20.41592	20.59344	27	27
7.00	80.0	599.9333	600.1337	26	26	20.60920	20.81034	27	27
5.00	120.0	600.1559	600.3319	26	26	20.83271	21.00950	27	27

Standardized Data

Calibration Results

Test Meter		Reference Meter		Correction Factor		Flow Rate		ΔH@ (mm H ₂ O)	
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	ΔH _{SCMM}	Variation	
V _{min} (m ³)	Q _{std} m ³ /min	V _{ref} (m ³)	Q _{ref} m ³ /min	(Y)	(ΔY)	Q _{std & Corr}	ΔH _{SC}	ΔΔH _{SC}	
0.159	0.011	0.160	0.011	1.005	0.010	0.011	50.181	2.747	
0.152	0.015	0.152	0.015	0.996	0.000	0.015	48.098	0.662	
0.174	0.022	0.173	0.022	0.995	-0.001	0.022	47.605	0.171	
0.197	0.028	0.196	0.028	0.993	-0.003	0.028	45.688	-1.747	
0.174	0.035	0.172	0.034	0.990	-0.006	0.034	45.602	-1.832	
				0.996	= Y Avg.		47.434	= ΔH@ Avg	

Pass/Fail Result: **Pass**

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02
 Note: For ΔH_{SC} orifice pressure differential that equates to 0.75cfm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O

Approved By: _____

(Patpasu Chaisana)
 Service Manager

บริษัท วิสโดม ไนน์ แอนด์ เซอร์วิส กรุ๊ป จำกัด
 WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Date: 3-Jul-23

COPY

TEMPERATURE DISPLAY CALIBRATION

Reference Equipment

Temp. Simulator Model : FLUKE 714B
 Serial No.: 60590035

Calibration Conditions

Cal. Date: 3-Jul-23
 Due Date: 2-Jul-24
 Cal. Report No.: WDS-SV660107
 Ambient Temp. (°C): 25
 Pressure (mm Hg): 758
 Humidity (%): 60

Temperature Sensor Calibration

Reference Point	Ref. Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
1	-18.0	-17.0	1.0
2	38.0	37.0	1.0
3	93.0	93.0	0.0
4	149.0	149.0	0.0
5	260.0	259.0	1.0
6	371.0	372.0	-1.0
7	482.0	482.0	0.0
8	593.0	593.0	-1.0
9	816.0	816.0	0.0
10	1038.0	1039.0	-1.0
		Maximum ¹	1.0

PASS

P-112

Note

¹ For valid test results, the maximum difference between temperature readings should ≤1.0°C (EPA Method 5, Section 6.1.1.8).
 Perform all TC Channel calibrations. Except meter (DGM) channel

DGM Out Temperature Sensor Calibration

Temperature point	Ref. Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
Ambient	26.5	27.0	-0.5
Heat	100.5	102.5	-2.0

PASS

DGM Out Temp. Diff. ±3 °C

Approved By: _____

(Patpasu Chaisana)
 Service Manager

บริษัท วิสโดม ไนน์ แอนด์ เซอร์วิส กรุ๊ป จำกัด
 WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED
 Address 9/115 Lumpini Town Ville Rajchaphrak-Pinklao Village No. 4, Bang Kharun, Bang Kruai, Nonthaburi 11130 Thailand
 Tel. 090-560-1392 084-598-1944 084-704-1620

ELAPSED TIMER CALIBRATION

Meter Console Information

Model #: XC572V
 Serial #: 1110070
 Elapsed Timer Model #: C342-1464
 Elapsed Timer Serial #: -

Calibration Conditions

Cal. Date : 03-Jul-23
 Due Date : 02-Jul-24
 Cal. Report No. : WDS-SV660107
 Ambient Temp. (°C) : 25
 Pressure (mm Hg) : 758
 Humidity (%) : 60

Reference Equipment

Calibration Standard: JS-307
 Method Reference: Compare

Run Time		Calibration Results				Average Time		Deviation	
Elapsed Time		Elapsed Time		Elapsed Time		Elapsed Time		Elapsed Time	
1	2	3	4	5	6	7	8	9	10
Minute	Minute	Minute	Minute	Minute	Minute	Minute	Minute	Minute	Minute
2.00	2.00	2.00	2.00	2.00	2.00	2.000	0.000	0.000	0.000
3.00	3.00	3.00	3.00	3.00	3.00	3.000	0.000	0.000	0.000
5.00	5.00	5.00	5.00	5.00	5.00	5.000	0.000	0.000	0.000
7.00	7.00	7.00	7.00	7.00	7.00	7.000	0.000	0.000	0.000
9.00	9.00	9.00	9.00	9.00	9.00	9.000	0.000	0.000	0.000

Approved By



(Fatpasi Chaisana)
 Service Engineer

**WISDOM
SCIENCE**

WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED
 Address 9/115 Lumpini Town Ville Rajchaphruek-Pinklao Village No. 4, Bang Khamin, Bang Kruai, Nonthaburi 11130 Thailand
 Tel. 090-660-1392, 084-598-1944, 084-704-1620

Flue gas Analyzer

Testo 350 NEW

Serial No. 60378478



Calibration Certificate

Certificate No: G 660353
Date of issue : 20-Jun-23

ENTECH

Where
Begin

Instrument description : Flue Gas Analyzer
Instrument model : Testo 350 NEW
Instrument serial no. : 60378478
ID no. or control no. :
Manufacturer : Testo SE & Co. KGaA
Probe description :
Probe model :
Probe serial :
Customer name : Eastern Thai Consulting 1992 Company Limited
Customer address : 683 Moo 11, Sukhapibarn 8 Road, Nongkham, Si Racha, Chon Buri 20280

Total pages of certificate : 2 Pages
Receiving no. : L-231787
Receiving date. : 16-Jun-23
Parameter of calibration : Gas Calibration(Oxygen 2.498,10.04,21.02 %vol, Carbon Monoxide 80.14,309.9,1003 ppm Nitrogen Dioxide 80.96 ppm, Nitric Oxide 151.5 ppm, Sulphur Dioxide 100.8 ppm)
Condition of UUC. : Used
Ambient condition : All of the Measurement were carried out the stabilized laboratory
Temperature : 23 ±5 °C
Humidity : 55 ± 15 %RH
Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210
Calibration procedure no. : This instrument was calibrated by comparison with Standard gas mixture according to calibration work instruction no. WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.
This certificate is applied only to item under test Environmental condition.
This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory.
Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.
This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 20-Jun-23

Mr. Kwanchai Khamboung
Calibration Technician

Mrs. Nongluck Wongsettee
Technical Manager



Calibration Certificate

Certificate No.: G 660353

ENTECH

Where
Begin

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O ₂) 2.498 % Vol	4219/21	Linde	30-Sep-25
Oxygen (O ₂) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen (O ₂) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide (CO) 80.14 ppm	CG-0040-22	Nimt	14-Feb-27
Carbon monoxide (CO) 309.9 ppm	2803/21	Linde	22-Jun-23
Carbon monoxide (CO) 1003 ppm	2583/22	Linde	09-Aug-24
Nitrogen Dioxide (NO ₂) 80.96 ppm	3240/21	Linde	26-Jun-24
Nitric Oxide (NO) 151.5 ppm	0161/23	Linde	22-Jan-25
Sulphur Dioxide (SO ₂) 100.8 ppm	3507/22	Linde	09-Nov-24

Measured room conditions

Temperature : 22.9 °C Humidity : 65.2 %RH Pressure : 1008.2 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,200 ml/min Gas pressure : 1019.4 mbar

Calibration Results (before adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.498	2.53	0.032	0.15
O ₂ (%Vol)	10.04	10.08	0.04	0.20
O ₂ (%Vol)	21.02	21.09	0.07	0.30
CO (ppm)	80.14	81	0.86	3.0
CO (ppm)	309.9	311	1.1	6.0
CO (ppm)	1003	1005	2	12
*NO ₂ (ppm)	80.96	72.1	-8.86	8.0
*NO (ppm)	151.5	142	-9.5	8.0
*SO ₂ (ppm)	100.8	102	1.2	6.0

Calibration Results (after adjustment) (Table 3)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.498	2.53	0.032	0.15
O ₂ (%Vol)	10.04	10.08	0.04	0.20
O ₂ (%Vol)	21.02	21.09	0.07	0.30
CO (ppm)	80.14	81	0.86	3.0
CO (ppm)	309.9	311	1.1	6.0
CO (ppm)	1003	1005	2	12
*NO ₂ (ppm)	80.96	81.2	0.24	8.0
*NO (ppm)	151.5	152	0.5	8.0
*SO ₂ (ppm)	100.8	102	1.2	6.0

Remark : 1 cmol/mol = 1 %vol, 1 µmol/mol = 1 ppm.

* Calibrations marked Not TISI Accredited "in this Certificate have been included for completeness."

End of Report

Issued Date 26/02/16

Issued Date 26/02/16

Hot Air Oven

Model : UFE 500

Serial No. : G511.0182

REPORT OF CALIBRATION

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhaphiban 8 Rd., Nongkham,
Sriacha, Chonburi 20230
Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)
Manufacturer : Memmert
Model : UFE 500
Serial No. : G511.0182
ID No. : LABE 17/4
Date of Receipt : 20 January 2023
Date of Calibration : 20 January 2023

Condition of Calibration
1. Environment
1.1 Ambient temperature : Maximum 27.9 °C : Minimum 25.3 °C
1.2 Relative humidity : Maximum 50.9 % : Minimum 38.5 %
1.3 Line voltage supplied : Maximum 221.9 VAC : Minimum 218.5 VAC

2. Calibration method
TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument
Instrument : ID No. : LB-DA-11 (RTD-138 to RTD-146)
Data Acquisition With Sensor : Certificate No. : 22-040309
Due Date : 21 April 2023

4. This certificate is traceable to the international system of unit (SI Unit).
The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Sarawoot Thammo
Scientist
Issue date : 24 January 2023

Approved by : (Mr. Somchai Neampunt)
Signed for Director

The uncertainties are for a confidence probability of approximately 95%.
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310

TEL 02-516-2422
FAX 02-516-6949
Rev. 01

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/11/21

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310

TEL 02-516-2422
FAX 02-516-6949
Rev. 01

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/11/21

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310

TEL 02-516-2422
FAX 02-516-6949
Rev. 01

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/11/21

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310

TEL 02-516-2422
FAX 02-516-6949
Rev. 01




REPORT OF CALIBRATION

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 56 cm ; D = 40 cm ; H = 48 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

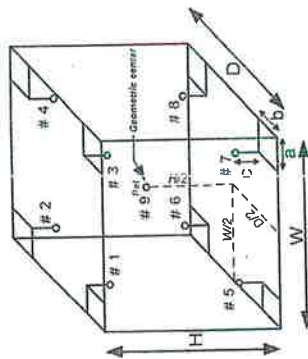Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated at the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of Report -

COPY

UV/VIS SPECTROPHOTOMETER

Model : UV - 1800

Serial No. : A11635101643 CD



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Sliem Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Bara Scientific
Solutions of Success

Certificate of Calibration

2 of 3

Number of Page(s)

Certificate No. BSCC-UV-152/23

Calibration Results:

1. Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
287.71	287.65	-0.06	0.18
445.82	445.80	-0.02	0.18
536.52	536.35	-0.17	0.18
741.02	740.99	-0.03	0.18
879.41	879.27	-0.14	0.18

2. Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000	0.0000	0.0000	0.0075
257	0.7311	0.7313	0.0002	0.0075
257	CNR	CNR	CNR	CNR
313	CNR	CNR	CNR	CNR
350	CNR	CNR	CNR	CNR
350	0.0000	0.0000	0.0000	0.0075
350	0.6306	0.6314	0.0008	0.0075

*CNR = Customer not request

COPY

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate. Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Sliem Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Bara Scientific
Solutions of Success

Certificate of Calibration

1 of 3

Number of Page(s)

Certificate No. BSCC-UV-152/23

Equipment UV/Vis Spectrophotometer

Model UV-1800

Manufacturer Shimadzu

Serial No. A11635101643 CD

ID No. N/A

Date of receipt 25 April 2023

Date of calibration 25 April 2023

Date of issue 27 April 2023

Customer name Eastern Thai Consulting 1992 Co., Ltd

Address 683 Moo 11, Sukkaphibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Temperature (22.4-23.1) °C (On site)

Humidity (44.5-45.2) %RH (On site)

Equipment condition Good Operation

Calibration Location Analysis Department

Calibration Procedure In-house method WJ-UV-702-01 based on ASTM E275-01

Traceability Wavelength Accuracy is traceable to certificate No. 94780 and 94775

Photometric Accuracy is traceable to certificate No. 94808 and 100147

Stray Light is traceable to certificate No. 94791

The above certificate are traceable to SI unit through Starna Scientific Ltd. (UKAS accredited calibration laboratory NO. 0659)

Calibrated by Mr. Pannaphong Phanmekakul

Approved by

Signature

Mr. Kanchit Choothep
Technical Manager

COPY

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate. Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.



Bara Scientific Co., Ltd.
988 U Chu Liang Building Floor 7 Rama4 Road
Sittom Bangrak Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Bara Scientific
SOLUTIONS & SERVICES

Certificate of Calibration

Certificate No.

BSCC-UV-152/23

Number of Page(s)

3 of 3

Calibration Results:

3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5488	0.5508	0.0020	0.0042
	0.7527	0.7535	0.0008	0.0042
	1.0756	1.0758	0.0002	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5391	0.5406	0.0015	0.0042
	0.7355	0.7360	0.0005	0.0042
	1.0509	1.0501	-0.0008	0.0042
465.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
546.1	0.0000	0.0000	0.0000	0.0042
	0.5045	0.5044	-0.0001	0.0042
	0.6884	0.6885	0.0001	0.0042
	0.9816	0.9808	-0.0008	0.0042
590.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
635.0	0.0000	0.0000	0.0000	0.0042
	0.5183	0.5178	-0.0005	0.0042
	0.6864	0.6868	0.0004	0.0042
	0.9747	0.9739	-0.0008	0.0042

*CNR = Customer not request

4. Stray Light*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)	
	Wavelength (nm)	Absorbance (A)
200.75±0.11nm	200.72	2.0164

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A
*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%
End of Certificate

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.

COPY

Area Heat Stress Monitor

Model : QUESTemp 34

Serial No. : TEU080011

CALIBRATION CERTIFICATE



Certificate No. : L202306315-001

Date Issued : 04-Jul-23

Customer : Eastern Thai Consulting 1992 Co., Ltd.
 683 Moo 11 Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment : Area Heat Stress Monitor

Manufacturer : TSI

Model : QUESTemp 34

Serial No. : TEU080011

ID No./Tag No. : NO.10

Date Received : 30-Jun-23

Date Calibrated : 02-Jul-23

Calibrated by : Mr. Apiwat Peanrungrat

Calibration Method or Calibration Procedure Used


In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: 
 (Mr. Sarayuth Tochua)



Page 1 of 2

COPY

Certificate No. : L202306315-001

Environment : Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15)\%\text{RH}$

STD	Reading ($^\circ\text{C}$)	Before Adjusted	After Adjusted	UUC Error ($^\circ\text{C}$)	Measurement Uncertainty ($\pm^\circ\text{C}$)
	37.99	WET 37.9	-	-0.09	0.35
	37.99	DRY 37.7	-	-0.29	0.35
	37.99	GLOBE 37.9	-	-0.09	0.35
	45.01	WET 44.9	-	-0.11	0.35
	45.01	DRY 44.8	-	-0.21	0.35
	45.01	GLOBE 45.0	-	-0.01	0.35

STD = Standard

UUC = Unit Under Calibration

Description of UUC : Range 0 to 100 $^\circ\text{C}$
 Resolution 0.1 $^\circ\text{C}$

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202210258-006 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 10-Nov-23

End of Certificate


Page 2 of 2

COPY

Area Heat Stress Monitor

Model : QUESTemp 34

Serial No. : TEU080014

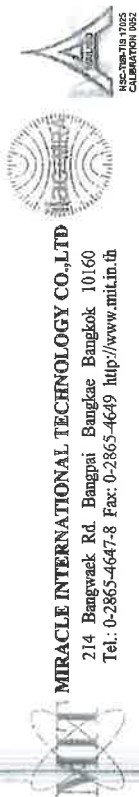

MIRACLE INTERNATIONAL TECHNOLOGY CO., LTD
214 Bangwaek Rd. Bangyai Bangkok 10160
Tel: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : L202307241-0002
Date Issued : 24-Jul-23

Customer : Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11 Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment : Area Heat Stress Monitor

Manufacturer : QUEST TECHNOLOGY

Model : QUESTEMP 34

Serial No. : TEU080014

ID No./Tag No. : No.13

Date Received : 21-Jul-23

Date Calibrated : 22-Jul-23

Calibrated by : Mr. Apiwat Peanrungrat

Calibration Method or Calibration Procedure Used

In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: *Sarayuth T.*

(Mr. Sarayuth Tochua)

Page 1 of 2



COPY

Certificate No. : L202307241-0002

Environment : Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15)\%RH$

STD	Reading ($^\circ\text{C}$)	UUC Reading ($^\circ\text{C}$)	Before Adjusted	After Adjusted	UUC Error ($^\circ\text{C}$)	Measurement Uncertainty ($\pm^\circ\text{C}$)
	38.00		WET 38.1	-	0.10	0.35
	38.00		DRY 38.2	-	0.20	0.35
	38.00		GLOBE 38.0	-	0.00	0.35
	44.99		WET 45.0	-	0.01	0.35
	44.99		DRY 45.1	-	0.11	0.35
	44.99		GLOBE 44.9	-	-0.09	0.35

STD = Standard

UUC = Unit Under Calibration

Description of UUC :
Range 0 to 100 $^\circ\text{C}$
Resolution 0.1 $^\circ\text{C}$

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202210258-006 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 10-Nov-23

End of Certificate

Page 2 of 2

COPY

SOUND LEVEL CALIBRATOR

MODEL : NC-75

SERIAL No. : 34302326



Calibration Certificate

SOUND CALIBRATOR

Equipment :
Manufacturer :
Model :
Serial No. :
ID No. :

RION
NC-75
34302326

Condition As Found :

GOOD

Customer :

EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :

Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date :

10 MAY 2023
Calibration Date : 19 MAY 2023
Date of Issue : 24 MAY 2023

Calibrated by :

Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

Continuation of Calibration Certificate

Cert. No. : ACC23013
Job No. : VC66AC0058
Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.
The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY32302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY3220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY3220076	EEL-BP 30/0267	13-FEB-24
Digital Multimeter	33461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24
Audio Analyzer	AVR-3360A	V744B6069	EF-0012-23	10-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

Continuation of Calibration Certificate

Cert. No. : ACC23013
Job No. : VC66AC0058
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.03	0.03	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
0.32	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00322753

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Srinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



Cert. No. : ACL23142
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322753 / 196476 / 15485
ID No.:

Condition As Found : GOOD
Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %
Received Date : 02 MAY 2023
Calibration Date : 02-04 MAY 2023
Date of Issue : 05 MAY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

SITHIPORN SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23142
Job No. : VC66AC0047
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 300266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 290266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL-BP 310266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

7. Petchurai

Continuation of Calibration Certificate

Cert. No. : ACL23142
Job No. : VC66AC0047
Pages : 3 of 8Cert. No. : ACL23142
Job No. : VC66AC0047
Pages : 4 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	10.8
C - weight	17.2
Flat	22.8

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	Acceptance Limits
125	0.2	0.2	± 1.5
1000	0.0	0.0	± 1.0
8000	0.9	1.0	±5.0

COPY

COPY

7. Reth

7. Reth

Continuation of Calibration Certificate

Cert. No. : ACL23142
Job No. : VC66AC0047
Pages : 5 of 8Cert. No. : ACL23142
Job No. : VC66AC0047
Pages : 6 of 8

4 Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	0.0	-0.1	0.0
125	0.0	0.0	0.0
250	0.0	0.0	0.0
500	0.0	0.1	0.0
1000	0.0	0.0	0.0
2000	0.0	0.1	0.1
4000	0.0	0.1	0.0
8000	0.1	0.1	0.1

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Continuation of Calibration Certificate

Cert No. : ACL23142
Job No. : VC66AC0047
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.5 ; -5.0
	200	800	127.6	127.5	-0.1	±1.0
	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
SEL	2	8	108.0	107.9	-0.1	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.5	-0.9	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	132.9	-0.1	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

Continuation of Calibration Certificate

Cert No. : ACL23142
Job No. : VC66AC0047
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.7	0.2	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

T. Ratcha

COPY

T. Ratcha

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00322748



451-451/1 Srinthorn Rd., Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com

NSC-TIS-TIS 17025
CALIBRATION 0394

Cert. No. : ACL23139
Pages : 1 of 8

Calibration Certificate

Equipment: SOUND LEVEL METER
Manufacturer: RION
Model: NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322748 / 196471 / 15480
ID No.:
Condition As Found: GOOD
Customer: EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location:
Ambient Temperature: (23.0 ± 3) °C
Pressure: (101.3 ± 3) kPa
Relative Humidity: (50.0 ± 20) %
Received Date: 02 MAY 2023
Calibration Date: 02-04 MAY 2023
Date of Issue: 05 MAY 2023

Calibrated by: Nathakorn Pisutpaisan

Approved by: 
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : ACL23139
Job No. : VC66AC0047
Pages : 2 of 8

Calibration Procedure: CF-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

Continuation of Calibration Certificate

Cert No. : ACL23139
Job No. : VC66AC0047
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

COPY

Continuation of Calibration Certificate

Cert No. : ACL23139
Job No. : VC66AC0047
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.2
C - weight	17.2
Flat	23.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.2	0.2	0.2
1000	0.0	0.0	0.0
8000	0.1	0.2	0.2
			Acceptance Limits
			± 1.5
			± 1.0
			±5.0

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23139
Job No. : VC66AC0047
Pages : 6 of 8Cert. No. : ACL23139
Job No. : VC66AC0047
Pages : 5 of 8

Continuation of Calibration Certificate

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	0.0	-0.1	0.0
125	0.0	0.0	0.0
250	0.0	0.0	0.0
500	0.0	0.0	0.0
1000	0.0	0.0	0.0
2000	0.0	0.1	0.0
4000	0.0	0.0	0.0
8000	0.0	0.1	0.1

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	24.9	-0.1	± 1.1

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.1	-0.3	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.7	89.7	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display (dB)		Deviated Value (dB)	Acceptance Limits (dB)
	at initial	at final		
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty u multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

COPY

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00322746

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322746 / 196469 / 15478
ID No.:

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 11 JUNE 2023
Calibration Date : 24-25 JULY 2023
Date of Issue : 02 AUGUST 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KA1	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

T. Petchurai

Continuation of Calibration Certificate

Cert. No. : ACL23245
Job No. : VC66AC0069
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

COPY
T. Petcha

Continuation of Calibration Certificate

Cert. No. : ACL23245
Job No. : VC66AC0069
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.6
C - weight	18.9
Flat	24.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.4	0.4	0.4
1000	0.0	0.0	0.0
8000	0.4	0.5	0.5
			Acceptance Limits
			± 1.5
			± 1.0
			± 5.0

COPY
T. Petcha

Continuation of Calibration Certificate

Cert. No. : ACL23245
Job No. : VC66AC0069
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
63	-0.1	-0.1	±2.0
125	0.0	0.0	±1.5
250	0.0	0.0	±1.5
500	0.0	0.0	±1.5
1000	0.0	0.0	±1.0
2000	0.0	0.0	±2.0
4000	0.0	0.0	±3.0
8000	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)

Continuation of Calibration Certificate

Cert. No. : ACL23245
Job No. : VC66AC0069
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.1	0.1	± 1.1
136.0	136.1	0.1	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.1	0.1	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.1	0.1	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.1	0.1	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL23245
Job No. : VC66AC0069
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighing	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEI	2	8	108.0	108.0	0.0	1.0 ; ±2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.5	-0.9	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

COPY
T. Ratan

Continuation of Calibration Certificate

Cert. No. : ACL23245
Job No. : VC66AC0069
Pages : 8 of 8

11. Overload Indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	0.1	±1.5
89.5	89.6		

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY
T. Ratan

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00222594



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0321

MTC No. EEL. BP. 114/0266

CALIBRATION CERTIFICATE

Submitted by : Eastern Thai Consulting 1992 Co., Ltd.
Address : 683 Moo 11, Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi, 20230
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :
Description : Sound Level Meter
Manufacturer : Rion
Model : NL-42A
Serial No. : 00222594 (No.38)
Microphone : UC-52 No.195906
Preamplifier : NH-24 No.15426

Standards used :
1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistophone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 20 Feb. 2023
Date of Calibration : 15 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : mtr@tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtr@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BL.MTC.002 Rev



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0321

MTC No. EEL. BP. 114/0266

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
11. Digital Multimeter Agilent 34401A S/N MY44005560.
12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 15 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : mtr@tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtr@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BL.MTC.002 Rev.4

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation	Acceptance	Uncertainty	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
113.97	114.4	114.0	0.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 113.8 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
14.7	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	11.2	0.10	N/A
C-Weight	19.9	0.10	N/A
Flat	23.0	0.10	N/A

Date of Calibration : 15 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : mtc@tistr.or.th

Office/Laboratory
Sol 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response curve (dB)		Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight			
125	0.3	0.3	0.2	0.45	0.6
1 000	-0.3	-0.3	-0.2	0.45	0.6
8 000	0.8	0.8	0.7	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response curve (dB)		Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight			
63	0.1	0.0	0.1	0.20	0.6
125	0.0	0.1	0.1	0.20	0.6
250	0.0	0.1	0.1	0.20	0.6
500	0.0	0.1	0.1	0.20	0.6
1 000	0.0	0.0	0.0	0.20	0.6
2 000	-0.2	-0.1	-0.2	0.20	0.6
4 000	-0.2	-0.2	-0.2	0.20	0.6
8 000	0.0	0.0	0.0	0.20	0.7

Date of Calibration : 15 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : mtc@tistr.or.th

Office/Laboratory
Sol 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

5. Long-term stability

Time	Measured value (dB)	Deviated (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 15 Mar. 2023

The results relate only to the items tested/calibrated or value assigned
Advising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR

FM.BLMTC.002 Re

7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
128	128.0	0.0	1.1	0.30	0.3
127	127.0	0.0	1.1	0.30	0.3
126	126.0	0.0	1.1	0.30	0.3
125	125.0	0.0	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	83.9	-0.1	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3
64	63.9	-0.1	1.1	0.30	0.3
59	58.9	-0.1	1.1	0.30	0.3
54	53.9	-0.1	1.1	0.30	0.3
49	48.9	-0.1	1.1	0.30	0.3

Date of Calibration : 15 Mar. 2023

The results relate only to the items tested/calibrated or value assigned
Advising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR

FM.BLMTC.002 Rev.4



7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
44	43.9	-0.1	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	33.9	-0.1	1.1	0.30	0.3
29	28.9	-0.1	1.1	0.30	0.3
28	27.9	-0.1	1.1	0.30	0.3
27	26.9	-0.1	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	24.9	-0.1	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 15 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Re

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Thailand
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : mtc@tistr.or.th

Office/Laboratory
Sol 1C, Bangpoo Industrial Estate, Sukhumvit Road, Thailand
Amphoe Muang Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
40-130	45	45.0	0.0	1.1	0.30	0.3
30-120	35	35.0	0.0	1.1	0.30	0.3
20-110	25	25.0	0.0	1.1	0.30	0.3
20-100	25	25.0	0.0	1.1	0.30	0.3
20-90	25	25.0	0.0	1.1	0.30	0.3
20-80	25	25.0	0.0	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb(ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Fast	200	116.0	0.0	± 1.0	0.20	0.3
	2	99.0	0.0	$+1.0; -2.5$	0.20	0.3
	0.25	90.0	0.0	$+1.5; -5.0$	0.20	0.3
Slow	200	109.6	0.0	± 1.0	0.20	0.3
	2	90.0	0.0	$+1.0; -5.0$	0.20	0.3
	200	110.0	0.0	± 1.0	0.20	0.3
SEL	2	90.0	0.0	$+1.0; -2.5$	0.20	0.3
	0.25	80.9	-0.1	$+1.5; -5.0$	0.20	0.3

Date of Calibration : 15 Mar. 2023

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Thailand
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : mtc@tistr.or.th

Office/Laboratory
Sol 1C, Bangpoo Industrial Estate, Sukhumvit Road, Thailand
Amphoe Muang Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



NSC-TSITIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0321

MTC No. EEL. BP. 114/0266

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.3	-0.1	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle	0.0	1.5	0.20	0.25
136.5	136.5				

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

Wittawat Supanich

(Mr. Wittawat Supanich)

Approved by :



(Mr. Prawit Kiatyapa)

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 15 Mar. 2023

Date of Issue : 16 Mar. 2023

Ref : 2011266022000725002

End of Certificate

COPY

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Re

Head Office
35 Mu. 5 Tambon Khong Ha, Amphoe Khong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rump@tistr.or.th Website: www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyotin Road, Chabuchak Bangkok 1091
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

NOISE DOSI METER

MODEL : CR:110A

SERIAL No. : CB1365

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 10 February 2023 CERTIFICATE NUMBER 187443



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2
Approved signatory R. Thomas
Electronically signed:

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer:	Cirrus Research plc	Notes:	Eastern Thai Consulting 1992 Co., Ltd.
Model:	CR:110A		683 Moo 11, Sukaphibal 8 Rd. NongKham
Serial number:	CB1365		Sriracha, Chonburi 20230
Firmware version:	5.4		

Test summary

Date of calibration: 10 February 2023
The calibration was performed respecting the requirements of ISO/IEC 17025:2017.
The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.
The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	TTi	TG4001	395851
Attenuator	Cirrus Research	ZE:952	52200
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	79620

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
187443

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before	Pressure: 102.28 kPa	Temperature: 22.6 °C	Humidity: 36.4 %
After	Pressure: 102.28 kPa	Temperature: 22.5 °C	Humidity: 36.7 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity	Complies
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies

COPY

NOISE DOSI METER

MODEL : CR:110A

SERIAL No. : CB1498

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 13 February 2023 CERTIFICATE NUMBER 187450

CERTIFICATE OF CALIBRATION

Certificate Number:
187450

Page 2 of 2



Cirrus Research plc

Acoustic House

Bridlington Road

Hunmanby

North Yorkshire

YO14 0PH

United Kingdom

Page 1 of 2

Approved signatory
R.Thomas
Electronically signed:


Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc

Model CR:110A

Serial number: CB1498

Software version: 5.4

Notes:

Eastern Thai Consulting 1992 Co., Ltd.

683 Moo 11, Sukaphibal 8 Rd.

NongKham

Sriracha, Chonburi 20230

Test summary

Date of calibration: 10 February 2023

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.


The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	KEYSIGHT	33511B	MY58001553
Attenuator	Cirrus Research	ZE-952	64370
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	40088

Notes



This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

Environmental conditions

The following conditions were recorded at the time of the test:

Before

Pressure: 102.25 kPa

Temperature: 22.4 °C

Humidity: 36.9 %

After

Pressure: 102.24 kPa

Temperature: 22.7 °C

Humidity: 36.6 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity	Complies
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies

COPY