

ภาคผนวก

3-3

ใบรับรองห้องปฏิบัติการ บริษัท สเปเชียล แล็บ
เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑ ๘ มกราคม ๒๕๖๗

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท สเปเชียล แล็บ เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑ พฤศจิกายน ๒๕๖๖

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท สเปเชียล แล็บ เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด จำนวน ๒ แผ่น

ตามหนังสือที่อ้างถึง บริษัท สเปเชียล แล็บ เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด ห้องปฏิบัติการ
วิเคราะห์เอกชน เลขทะเบียน [REDACTED] สถานที่ตั้งเลขที่ ๔๗/๙๑-๙๓ หมู่ที่ ๓ ตำบลท่าอิฐ อำเภอปากเกร็ด
จังหวัดนนทบุรี ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท สเปเชียล แล็บ เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด
ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

- | | |
|-------------------------|---------------|
| ๑) นางสาวฟาติฮะห์ สุธลง | ทะเบียนเลขที่ |
| ๒) นางสาวอัศวณี ยูโซะ | ทะเบียนเลขที่ |
| ๓) นายมะปารี อาแวกือจิ | ทะเบียนเลขที่ |

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์

- | | |
|------------------------------|---------------|
| ๑) นางสาวบุศรียา ยีชา | ทะเบียนเลขที่ |
| ๒) นางสาวนุรีไลลา มะแซ | ทะเบียนเลขที่ |
| ๓) นางสาวชาอึรา สาแม | ทะเบียนเลขที่ |
| ๔) นางสาวนุรีสา สอเลาะห์ | ทะเบียนเลขที่ |
| ๕) นางสาวณัฐกานต์ บากาโชติ | ทะเบียนเลขที่ |
| ๖) นางสาวซารินา บัวซ์ | ทะเบียนเลขที่ |
| ๗) นางสาวบรั๊กส์ หะยีกาจิ | ทะเบียนเลขที่ |
| ๘) นางสาวโนรีไซเพีย มะนอ | ทะเบียนเลขที่ |
| ๙) นางสาวอามีรา แวหะแน | ทะเบียนเลขที่ |
| ๑๐) นางสาวนุรฮัยมี อาแวกือจิ | ทะเบียนเลขที่ |
| ๑๑) นางสาวอิฟติซาน หะมะ | ทะเบียนเลขที่ |
| ๑๒) นายเสรี จันทวี | ทะเบียนเลขที่ |

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย ตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒๕ มกราคม ๒๕๗๐ หากประสงค์จะต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงาน
อุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ทั้งนี้
สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นายศิระ จันทรเลิศ)

นักวิทยาศาสตร์เชี่ยวชาญ รักษาการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



เอกสารแนบท้ายหนังสือต่ออาัยรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท สเปเชียล แล็บ เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด

ที่ [REDACTED] ลงวันที่ ๑๘ มกราคม ๒๕๖๗

ขอขายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๒๖ รายการ

น้ำเสีย จำนวน 26 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Arsenic	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[2]
2	Barium	Digestion, Direct Nitrous Oxide-Acetylene Flame Method ^[2]
3	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ^[2] 2) 5-Day BOD Test, Membrane Electrode Method ^[2]
4	Cadmium	Digestion, Direct Air-Acetylene Flame Method ^[2]
5	Chemical Oxygen Demand	Closed Reflux, Colorimetric Method ^[2]
6	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[2]
7	Copper	Digestion, Direct Air-Acetylene Flame Method ^[2]
8	Cyanide	Distillation, Colorimetric Method ^[2]
9	Formaldehyde	Distillation, Colorimetric Method ^[1]
10~	Free Chlorine	DPD Colorimetric Method ^[2]
11	Hexavalent Chromium	Colorimetric Method ^[2]
12	Lead	Digestion, Direct Air-Acetylene Flame Method ^[2]
13	Manganese	Digestion, Direct Air-Acetylene Flame Method ^[2]
14	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[2]
15	Nickel	Digestion, Direct Air-Acetylene Flame Method ^[2]
16	Oil & Grease	Liquid-Liquid, Partition-Gravimetric Method ^[2]
17	pH	Electrometric Method ^[2]
18	Phenols	1) Distillation, Chloroform Extraction Method ^[2] 2) Distillation, Direct Photometric Method ^[2]
19	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[2]
20	Sulfide	Iodometric Method ^[2]
21	Temperature	Laboratory and Field Methods ^[2]
22	Total Dissolved Solids	Dried at 180 °C ^[2]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
23	Total Kjeldahl Nitrogen	Macro-Kjeldahl Method ^[2]
24	Total Suspended Solids	Dried from 103-105 °C ^[2]
25	Trivalent Chromium	Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation ^[2]
26	Zinc	Digestion, Direct Air-Acetylene Flame Method ^[2]

เอกสารอ้างอิง

1. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.

2. APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 24th ed. Washington, DC: APHA, 2023.



ใบรับรองเลขที่
(Certificate No.)

ใบรับรองระบบงาน

(Certificate of Accreditation)

อาศัยอำนาจตามความในพระราชบัญญัติการมาตรฐานแห่งชาติ พ.ศ. ๒๕๕๑

(By Virtue of National Standardization Act B.E. 2551 (2008))

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม

(Secretary-General, Thai Industrial Standards Institute)

ออกใบรับรองฉบับนี้ให้

(Issues this certificate to)

บริษัท สเปเชียล แล็บ เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด

(Special Lab Envi and Consultant Co.,Ltd.)

ตั้งอยู่เลขที่

(Address)

๔๗/๙๑-๙๓ หมู่ที่ ๓ ตำบลท่าอิฐ อำเภอปากเกร็ด จังหวัดนนทบุรี

47/91-93 Moo 3, Tha It, Pak Kret, Nonthaburi

ได้รับการรับรองความสามารถ

(Certificate of competence)

ตามมาตรฐานเลขที่

(Standard No. TIS 17025-2561 (2018) (ISO/IEC 17025: 2017))

ข้อกำหนดทั่วไปว่าด้วยความสามารถของ ห้องปฏิบัติการทดสอบและห้องปฏิบัติการสอบเทียบ

General requirements for the competence of testing and calibration laboratories

หมายเลขการรับรองที่

(Accreditation No. Testing 0639)

โดยมีรายละเอียดสาขาและขอบข่ายที่ได้ใบรับรอง แสดงไว้ใน QR CODE และ www.tisi.go.th

(Details of the scheme and scope of the certificate are shown in QR CODE and www.tisi.go.th)

ออกให้ ณ วันที่ ๑๖ กุมภาพันธ์ พ.ศ. ๒๕๖๖

(Issue date : 16 February B.E. 2566 (2023))



Signed by สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม (สมอ.) -
Thai Industrial Standards Institute (TISI)
Date: 2023-02-16T13:24:24.601+07:00

0883aa94

กระทรวงอุตสาหกรรม สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม

(Ministry of Industry Thailand, Thai Industrial Standards Institute)

(นายเอกนิติ รมยานนท์)

รองเลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม

ปฏิบัติราชการแทน

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม



รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

(Certification No, 23-LB0118)



ชื่อห้องปฏิบัติการ
(Laboratory Name)

บริษัท สเปเชียล แล็บ เอ็นไว แอนด์ คอนซัลแตนท์ จำกัด
(Special Lab Envi and Consultant Co.,Ltd.)

หมายเลขการรับรองที่
(Accreditation No.)

(Testing 0639)

ฉบับที่ 04
(Issue No.)

ออกให้ตั้งแต่วันที่ 3 สิงหาคม พ.ศ. 2566
(Valid from) (3 August B.E.2566 (2023))

ถึงวันที่ 2 สิงหาคม พ.ศ. 2571
(Until) (2 August B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ
(Laboratory status)

☒ ถาวร

(Permanent)

☐ นอกสถานที่

(Site)

☐ ชั่วคราว

(Temporary)

☐ เคลื่อนที่

(Mobile)

☐ หลายสถานที่

(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสังแวดล้อม (environmental field) น้ำเสีย (Wastewater)	- Chemical Oxygen Demand (COD) 25 mg/L to 20 000 mg/L - Total Suspended Solids (TSS) 5 mg/L to 5 000 mg/L - pH 4.0 to 10.0	- Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23rd edition, 2017, part 5220 D - Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23rd edition, 2017 , part 2540 D - Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23rd edition, 2017 , part 4500-H⁺ B

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ [REDACTED]

(Certification No. 23-LB0118)



ฉบับที่ 04

(Issue No.)

ออกให้ตั้งแต่วันที่ 3 สิงหาคม พ.ศ. 2566

(Valid from)

(3 August B.E.2566 (2023))

ถึงวันที่ 2 สิงหาคม พ.ศ. 2571

(Until)

(2 August B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ

(Laboratory status)

☒ ถาวร

(Permanent)

☐ นอกสถานที่

(Site)

☐ชั่วคราว

(Temporary)

☐เคลื่อนที่

(Mobile)

☐หลายสถานที่

(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสังแวดล้อม (environmental field) น้ำเสีย (Wastewater)	- Total Dissolved Solids (TDS) 25 mg/L to 6 000 mg/L - Total Dissolved Solids (TDS) at 103 °C to 105 °C 25 mg/L to 6 000 mg/L - Biochemical Oxygen Demand (BOD) 5 mg/L to 5 000 mg/L - Biochemical Oxygen Demand (BOD) 5 mg/L to 5 000 mg/L	- Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23rd edition, 2017 , part 2540 C - WI-LB-25 based on Standard methods For the Examination of Water and Wastewater, APHA, AWWA, WEF, 23rd edition, 2017 , part 2540 C - Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23rd edition, 2017, part 4500-O G., 5210 B - Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23rd edition, 2017, part 4500-O C., 5210 B

1. Block Digestion

ผู้ผลิต : [REDACTED] รุ่น : 3H 220F ... Serial No. [REDACTED] รหัสเครื่อง : [REDACTED]

2. Digital Thermometer with TC Probe

ผู้ผลิต : [REDACTED] รุ่น : Temp...K ... Serial No. [REDACTED] รหัสเครื่อง : [REDACTED]


ความละเอียด : 0.1 °C วันที่สอบเทียบ : 31/01/2023 ... สอบเทียบครั้งต่อไป : 31/01/2024

3. ผลการทวนสอบ (ช่วงเวลา : 9.00 น. - 12.00 น.)

อุณหภูมิห้อง : 25 - 27 °C ความชื้นสัมพัทธ์ : 50 - 55 %

ว/ค/ป ที่ทวน สอบ	Position No.	Set point (°C)	อุณหภูมิที่ อ่านได้จาก เครื่อง (°C)	อุณหภูมิที่อ่านได้เทอร์โมมิเตอร์ (°C)			Error	เกณฑ์ การ ยอมรับ	สรุปผลการทวน สอบ		ผู้ทวน สอบ
				ครั้งที่ 1 (A)	ครั้งที่ 2 (B)	ค่าเฉลี่ยของ อุณหภูมิ			ผ่าน	ไม่ผ่าน	
3/5/66	1	250	251	251.2	251.4	251.3	1.3	±5	✓		[REDACTED]
4/5/66	2	250	250	250.3	250.9	250.6	0.6	±5	✓		
5/5/66	3	250	250	251.2	251.2	251.2	1.2	±5	✓		
8/5/66	4	250	250	250.3	251.3	251.0	1.0	±5	✓		
9/5/66	5	250	251	251.8	252.4	252.1	2.1	±5	✓		
10/5/66	6	250	250	249.8	250.8	250.3	0.3	±5	✓		
11/5/66	7	250	251	250.9	251.3	251.1	1.1	±5	✓		
12/5/66	8	250	251	251.9	252.5	252.2	2.2	±5	✓		
15/5/66	9	250	250	250.9	251.8	251.4	1.4	±5	✓		
18/5/66	10	250	252	252.4	253.2	252.8	2.8	±5	✓		
19/5/66	11	250	251	253.3	254.1	253.7	3.7	±5	✓		
24/5/66	12	250	251	251.3	252.2	251.8	1.8	±5	✓		
27/5/66	13	250	252	253.0	252.8	252.9	2.9	±5	✓		
31/5/66	14	250	252	251.9	252.1	252.0	2.0	±5	✓		
	15										
	16										
	17										
	18										
	19										
	20										

เอกสารสอบเทียบเครื่องมือตรวจวัด



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : [REDACTED]

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co.,Ltd.
47/91 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Buret
Manufacturer : Witeg Class : A
Capacity : 25 ml Graduation : 0.1 ml
ID No. : [REDACTED]

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (60 ± 15) %
Air Pressure : 1009.7 mbar.

Date of Received : 06 April 2023

Date of Calibration : 18 April 2023

Date of Issue : 18 April 2023

Calibrated by : [REDACTED]

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
[REDACTED]	[REDACTED]	02 Jun 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : [REDACTED]

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 40.55 sec.


Nominal Volume (ml)	Measuring Volume (ml)
10	10.0121
20	20.0086
25	25.0116

Uncertainty of measurement with in $\pm$ 0.0066 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. :

Page : 1 of 2

Submitted by :

Special Lab Envi and Consultant Co., Ltd.

47/91 Moo 3, Tambol Tha-it, Pakkret, Nonthaburi 11120

Equipment :

Digital Thermometer with Thermocouple probe Type K
Temperature Indicator

Manufacturer : Thermo Scientific

Model : TEMP 10K

Range : -250 °C to 1372 °C

Resolution : 0.1 °C

Serial No. : 4008958

ID No. : LB-Eq-013

Environment :

Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Line Voltage : (220 ± 22) VAC

Date of Received :

06 April 2023

Date of Calibration :

08 April to 10 April 2023

Date of Issue :

10 April 2023

Calibrated by :

Calibration Method :

This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments :

This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.

Cert. No.

Due Date

Traceability

07 Feb 2024

National Institute of Metrology Thailand (NIMT)

02 Jun 2023

National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.

Cert. No.

Due Date

Traceability

14 Jun 2023

National Institute of Metrology Thailand (NIMT)

14 Jun 2023

National Institute of Metrology Thailand (NIMT)

Approved by

(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : [REDACTED]

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement with Thermocouple probe Type K

Model : Type K Sheath Material : Teflon
Diameter : 2 mm. Length : 1500 mm.
Serial No. : N/A ID No. : SL-39

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
130	3.0036	3.5	-0.5	0.18
130	20.0024	20.4	-0.4	0.18
130	104.0011	104.3	-0.3	0.45
130	150.0027	150.2	-0.2	0.58
130	180.0040	180.0	0.0	0.65

Model : AD-1218-230 Sheath Material : Stainless
Diameter : 3.5 mm. Length : 230 mm.
Serial No. : N/A ID No. : SL-40

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
124	379.9914	379.3	0.7	1.5
124	400.0011	399.2	0.8	1.6

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor providing a level of confidence of approximately 95%

- 000 -





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: [REDACTED]

Page.: 1 of 2

Certificate of Testing

Equipment : DO Meter

Manufacturer : Hanna

Model : [REDACTED]

Serial No. : [REDACTED]

ID No. : [REDACTED]

Received Date : 16 February 2023

Test Date : 17 February 2023

Reference : 2302-0616WN-1

Submitted by : Special Lab Envi And Consultant Co.,Ltd
47/91 Moo 3 Thambon Tha-it,
Pakkret, Nonthaburi 11120

Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %

Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean

Approved by : [REDACTED]
Approved Signatory

(/) Malee Butkruea
() Saithip Meangmai
() Warakorn Lengagtrakul

Issue Date : 20 February 2023



Cert.No.: [REDACTED]
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	[REDACTED]	[REDACTED]	25 Mar 2023
2) Balance	[REDACTED]	[REDACTED]	[REDACTED]	20 Sep 2023

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: [REDACTED]

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.12	8.13	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency. The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

[REDACTED]

[REDACTED]

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkret, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. :



Page : 1 of 2

Submitted by :

Special Lab Envi and Consultant Co., Ltd.

47/91 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment :

Electronic Balance

Manufacturer : AND

Model :

Serial No. :

ID No. :

Capacity : 210 g

Resolution : 0.0001 g

Environment :

On site calibration was carried out at the Laboratory, Special Lab Envi and Consultant Co., Ltd.

Ambient Temperature : (29.4 to 29.7) °C

Relative Humidity : (50.9 to 51.5) %

Air Pressure : 1011.0 mbar

Date of Received : 24 April 2023

Date of Calibration : 24 April 2023

Date of Issue : 26 April 2023

Calibrated by :



Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14

Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units


Standard Weights

ID No.

Cert. No.

Due Date

Traceability



10 Nov 2023

National Institute of Metrology (Thailand), (NIMT)

Approved by :



(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : [REDACTED]

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty $\pm$ (g)
0.001	0.0000	0.00010
0.01	0.0000	0.00011
0.1	0.0000	0.00011
0.5	0.0000	0.00010
2	0.0000	0.00011
5	-0.0001	0.00011
10	0.0000	0.00012
50	-0.0001	0.00014
100	-0.0001	0.00020
200	0.0000	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.06$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A B C D E

-0.0003 0.0001 0.0004 0.0000 0.0000 g



Repeatability

Load test : 200 g

Stdev. : 0.00005 g

- o0o -



1. Heating block (COD)

ผู้ผลิต: [REDACTED] รุ่น: [REDACTED] Serial No. [REDACTED] รหัสเครื่อง: [REDACTED]

วันที่ทวนสอบ: 1 / 3 / 2566 ทวนสอบครั้งต่อไป: 1 / 9 / 2566

2. Digital Thermometer with TC Probe

ผู้ผลิต: [REDACTED] รุ่น: Temp 10 K Serial No. [REDACTED] รหัสเครื่อง: [REDACTED]

ความละเอียด: 0.1 (°C) วันที่ทวนสอบ: 3 พฤศจิกายน 66 ทวนสอบครั้งต่อไป: 2 พฤศจิกายน 66

3. ผลการทวนสอบ (ช่วงเวลา 3.00 น. - 16.30 น.)

อุณหภูมิห้อง: 26.3 (°C) ความชื้นสัมพัทธ์: 47.5 %

วัน/เดือน/ปี	Position No.	Set point (°C)	อุณหภูมิที่อ่านได้จากหน้าจอ (°C)	อุณหภูมิที่อ่านได้จากรีโมต (°C)			สถานะการยอมรับ	สรุปผลการทวนสอบ		ผู้ทวนสอบ
				ครั้งที่ 1 (A)	ครั้งที่ 2 (B)	ค่าเฉลี่ยของอุณหภูมิ		ผ่าน	ไม่ผ่าน	
1/3/2566	1	150.0	150.0	149.8	150.0	149.9	±2	/		บุษเรศ
	2			149.7	149.7	149.7	±2	/		
	3			150.8	150.7	150.8	±2	/		
	4			151.1	151.1	151.1	±2	/		
	5			150.1	150.4	150.3	±2	/		
	6			149.2	148.9	149.1	±2	/		
	7			150.0	149.8	149.9	±2	/		
	8			149.9	149.9	149.9	±2	/		
	9			150.0	149.8	149.9	±2	/		
	10			148.9	149.3	149.1	±2	/		
	11			148.9	149.5	149.2	±2	/		
	12			149.8	150.1	150.0	±2	/		
	13			149.9	150.2	150.1	±2	/		
	14			148.6	150.1	149.4	±2	/		
	15			149.4	149.6	149.5	±2	/		
	16			148.5	149.3	148.9	±2	/		
	17			150.1	150.1	150.1	±2	/		
	18			148.9	150.1	149.5	±2	/		
	19			149.5	149.7	149.6	±2	/		
	20			148.1	148.6	148.4	±2	/		
	21			148.7	148.8	148.8	±2	/		
	22			149.1	149.2	149.2	±2	/		
	23			148.1	148.2	148.2	±2	/		
	24			149.5	148.9	149.2	±2	/		
	25			148.3	148.4	148.4	±2	/		

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkret, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



Certificate of Calibration

Certificate No. : [REDACTED]

Page : 1 of 2

Submitted by :

Special Lab Envi and Consultant Co., Ltd.

47/91 Moo 3 Thambol Tha-it, Pakkret, Nonthaburi 11120

Equipment :

Air Chamber (Incubator)

Manufacturer : Lovibond

Model : FKU 1800

Range : N/A °C

Resolution : 0.1 °C

Serial No. : [REDACTED]

ID No. : [REDACTED]

Environment :

On site calibration was carried out at the Laboratory, Special Lab Envi and Consultant Co., Ltd.

Ambient Temperature : (29.0 to 29.6) °C

Relative Humidity : (40 to 45) %

Line Voltage : (226.0 to 226.5) V

Date of Received : 24 April 2023

Date of Calibration : 24 April 2023

Date of Issue : 26 April 2023

Calibrated by : [REDACTED]

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.

Cert. No.

Due Date

Traceability

02 Aug 2023

National Institute of Metrology Thailand (NIMT)

Approved by :

(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : [REDACTED]


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

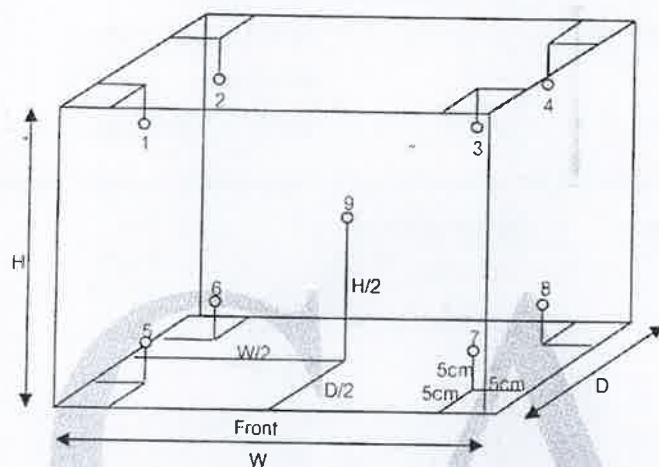

Inside of Chamber

W = 0.55 m

D = 0.73 m

H = 0.50 m

Capacity = 0.20 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	19.9	19.9	20.35	20.35	20.23	20.25	20.12	20.12	20.14	20.28	20.08	0.42

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	19.9	19.9	0.37	0.16	0.6

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. :



Page : 1 of 2

Submitted by

: Special Lab Envi and Consultant Co., Ltd.

47/91-93,96 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment

: Piston Pipette

Manufacturer : sartorius

Model :

Serial No. :

ID No. :

Capacity : 100 µl to 1000 µl Resolution : 5 µl

Environment

: Ambient Temperature : (20 ± 3) °C

Relative Humidity : (55 ± 10) %

Air Pressure : (1007.6 to 1007.7) mbar.

Date of Received : 03 August 2023

Date of Calibration : 07 August 2023

Date of Issue : 07 August 2023

Calibrated by



Calibration Method : In-house method CAL-M3002 base on ISO 8655-6 : 2002-09

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.

Cert. No.


Due Date

Traceability

02 Dec 2023

National Institute of Metrology (Thailand) (NIMT)

Approved by :



(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. :



Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Test Volume (μl)	Measuring Volume at 20°C (μl)	Systematic error ($e_s\%$)	Coeff. of Variation (CV%)	Uncertainty ($\pm \mu\text{l}$)
100	97.92	0.21	0.15	0.69
500	496.58	0.34	0.04	0.69
1000	997.55	0.24	0.01	0.69

e_s : Systematic error (%)


CV : Coefficient of variation (%)

UUC Calibrated by : Blue Tip

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

- oOo -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pukkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. :



Page : 1 of 2

Submitted by :

Special Lab Envi and Consultant Co., Ltd.

47/91 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment :

Piston Pipette

Manufacturer : BIOHIT

Model



Serial No. :



ID No.

Capacity : 100 µl to 1000 µl

Resolution: 5 µl

Environment :

Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : (1010.3 to 1010.4) mbar.

Date of Received : 07 December 2022

Date of Calibration : 09 December 2022

Date of Issue : 09 December 2022

Calibrated by : Wipa Tovadee

Calibration Method : In-house method CAL-M3002 base on ISO 8655-6 : 2002-09-15

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.

Cert. No.

Due Date

Traceability



02 Jun 2023

National Institute of Metrology (Thailand) (NIMT)

Approved by :



(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Test Volume (μ l)	Measuring Volume at 20 °C (μ l)	Systematic error (e_s %)	Coeff. of Variation (CV%)	Uncertainty ($\pm \mu$ l)
100	98.71	0.13	0.13	0.69
500	500.71	0.07	0.01	0.69
1000	1000.17	0.02	0.01	0.69

e_s : Systematic error (%)

CV : Coefficient of variation (%)

UUC Calibrated by : White Tip

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

- o0o -





Thermology Co., Ltd.

96/177-96/178 Moo 6, T. La-harn, A. Bangbuathong, Nonthaburi 11110
Tel : 0 2191 6479 Fax : 0 2191 6480 website : www.thermology.co



CALIBRATION CERTIFICATE

Date of Issue Jun 23, 2023

Cert No.

Site Calibration

Order No.

Customer SPECIAL LAB ENVI AND CONSULTANT CO., LTD.
47/91 Moo 3 Tha-It, Pak Kret, Nonthaburi, 11120.

Place of Calibration 1350, 1352 Sutthisarnwinitchai Rd, Dindaeng, Bangkok 10400. (Calibration Room)

Description Oven

Model UF30

Serial No. B123.0544

ID.No.

Date of Receipt Jun 20, 2023

Date of Calibration Jun 20, 2023

Environment

Temperature (Min) 23.1 °C (Max) 25.3 °C

Relative Humidity (Min) 46.3 %RH (Max) 78.9 %RH

Calibration Method

WI-17 : The reference thermometer was placed into the chamber and measurement was performed based on AS-2853.
The temperature scale in use at this laboratory is the International Temperature Scale of 1990.

Standard

1) Data Acquisition with Sensor Model 34972A S/N. MY49007789, Certificate No. QR23-0024, Calibrated by
Quality Reborn Co., Ltd., ONAC Calibration No. 0292. Due Date Jan 10, 2024.

This certificate is traceable to SI unit.



Thermology Co., Ltd.

96/177-96/178 Moo 6, T. La-harn, A. Bangbuathong, Nonthaburi 11110
Tel : 0 2191 6479 Fax : 0 2191 6480 website : www.thermology.co



CALIBRATION CERTIFICATE


Date of Issue Jun 23, 2023

Site Calibration

Cert No.

Order No.

Results (without adjustment)

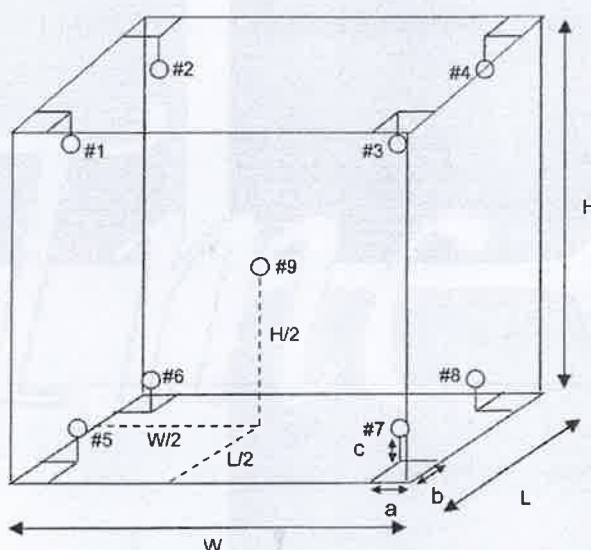

Position of reference thermometers were placed

Note.

- 1). Dimension (W x L x H) is 40 x 25 x 32 cm.
- 2). Stability - greatest one half of difference between max peak and min peak of each reference probe measured temperature obtained during the calibration interval.
- 3). Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.



Thermology Co., Ltd.

96/177-96/178 Moo 6, T. La-harn, A. Bangbuathong, Nonthaburi 11110
Tel : 0 2191 6479 Fax : 0 2191 6480 website : www.thermology.co



CALIBRATION CERTIFICATE

Date of Issue Jun 23, 2023

Cert No.

Site Calibration

Order No.

Results (without adjustment)

UUC Setting (°C)	UUC Reading (°C)	Reference Thermometer (°C)		Stability ± (°C)	Uniformity (°C)	Uncertainty ± (°C)
104.0	104.0	Position 1	104.544	0.058	0.704	0.30
		Position 2	103.789			
		Position 3	103.396			
		Position 4	103.886			
		Position 5	104.031			
		Position 6	103.886			
		Position 7	103.342			
		Position 8	103.939			
		Position 9	103.867			

UUC Setting (°C)	UUC Reading (°C)	Reference Thermometer (°C)		Stability ± (°C)	Uniformity (°C)	Uncertainty ± (°C)
150.0	150.0	Position 1	151.388	0.052	1.248	0.41
		Position 2	150.037			
		Position 3	149.313			
		Position 4	149.849			
		Position 5	150.519			
		Position 6	150.188			
		Position 7	149.370			
		Position 8	150.383			
		Position 9	150.201			



Thermology Co., Ltd.

96/177-96/178 Moo 6, T. La-harn, A. Bangbuathong, Nonthaburi 11110
Tel : 0 2191 6479 Fax : 0 2191 6480 website : www.thermology.co



CALIBRATION CERTIFICATE

Date of Issue Jun 23, 2023

Site Calibration

Cert No.

Order No.

Results (without adjustment)

UUC Setting (°C)	UUC Reading (°C)	Reference Thermometer (°C)		Stability ± (°C)	Uniformity (°C)	Uncertainty ± (°C)
180.0	180.0	Position 1	181.507	0.059	1.693	0.49
		Position 2	179.668			
		Position 3	178.772			
		Position 4	179.371			
		Position 5	180.334			
		Position 6	179.830			
		Position 7	178.855			
		Position 8	180.323			
		Position 9	179.876			

The stability and uniformity was taken into account in the measurement uncertainty stated.

The above results are valid exclusively for calibration samples as mentioned in the report.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%. The uncertainty evaluation has been carried out in accordance with ONAC requirements.

APPROVED SIGNATORY :

- ☐ MR. PRAJUCKPETCH THONGSOOKCHOTE
☒ MR. DAMRONG MULSING
☐ MR. JATURAPAT THONGSOOKCHOTE



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL: 0-2717-3000-29 FAX: 0-2719-9484



Cert.No.:

Page.:

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Eutech
Model : pH 700
Serial No. : [REDACTED]
ID No. : [REDACTED]
Condition As-Received: Used Item
Received Date : 04 August 2023
Calibration Date : 07 August 2023
Reference : [REDACTED]
Submitted by : Special Lab Envi And Consultant Co.,Ltd
47/91-93, 96 Moo 3 Thambon Tha-it, Pakkret
Nonthaburi 11120

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard
voltage calibrator and direct measurement
with certified reference material (CRM)

Calibrated by : [REDACTED]

Approved by : [REDACTED]
Approved Signatory
(✓) Saithip Meangmai
() Warakom Lemgagtrakul
() Ponpan Paipim

Issue Date : 16 August 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert. No.:

Page.:

Condition of this calibration result

1. Reference Standard Instrument : -

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator				24 Aug 2023

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	863832	28 Dec 2024
pH 6.986	CPA chem	863833	28 Dec 2023
pH 10.010	CPA chem	863835	28 Dec 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results**Function : mV Measurement**

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ($\pm$ mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: 2858459	4.00	177.48	177.5	4.01	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	10.00	-177.48	-177.4	10.01	0.058	2.00

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: 3101624	4.008	4.01	170.7	0.0085	2.05
	6.986	6.99	-2.0	0.011	2.00
	10.010	10.01	-178.2	0.0096	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23LM132

Page.: 1 of 2

Certificate of Calibration

Equipment : pH Meter with Sensor
Manufacturer : Eutech
Model : pH 700
Serial No. : [REDACTED]
ID No. : [REDACTED]
Submitted by : Special Lab Envi And Consultant Co.,Ltd.
47/91-93 Moo 3 Thambon Tha-it,
Pakkret,
Nonthaburi 11120
Location : TPA On Site Calibration Laboratory
Received Order : 04 August 2023
Calibrated Date : 09 August 2023
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by :



Approved by :

Approved Signatory

() Pornthippa Tameyakul
() Ponpan Paipim
(✓) Suwit Imjai

Issue Date : 17 August 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0057254



Equipment : pH Meter with Sensor

Condition As-Received : New Item

Cert. No. [REDACTED]

Page.: 2 of 2

Reference : [REDACTED]

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	[REDACTED]	[REDACTED]	TPA	21 Oct 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.


This instrument was connected with temperature sensor, S/N.: PH5TEMB01P

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
25.0	100	25.002	25.0	-0.002	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120


Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. :



Page : 1 of 2

Submitted by :

Special Lab Envi and Consultant Co., Ltd.

47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment :

Air Chamber (Refrigerator)

Manufacturer : Frozen

Model : CC-2288F

Range : N/A °C

Resolution : 1 °C

Serial No. : [Redacted]

ID No. : [Redacted]

Environment :

On site calibration was carried out at the Laboratory, Special Lab Envi and Consultant Co., Ltd.

Ambient Temperature : (31.0 to 32.0) °C

Relative Humidity : (40 to 45) %

Line Voltage : (226.0 to 226.5) V

Date of Received : 02 May 2023

Date of Calibration : 02 May 2023

Date of Issue : 02 May 2023

Calibrated by :



Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.

Cert. No.

Due Date

Traceability

03 Aug 2023

National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. [REDACTED]


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

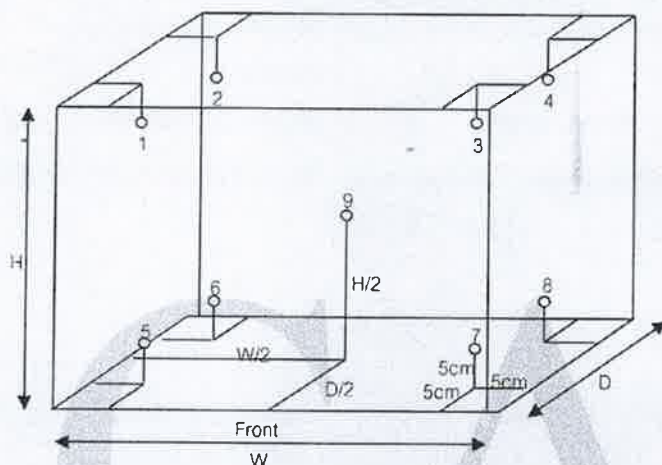

Inside of Chamber

W = 1.02 m

D = 0.47 m

H = 1.48 m

Capacity = 0.71 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
3	3	3	3.21	2.53	2.23	2.38	3.74	4.12	2.20	2.05	3.01	0.83


Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
3	3	3	1.17	0.25	2.5

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -





BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-23-297

Page : 1 of 3

CERTIFICATE OF CALIBRATION

Equipment	:	Spectrophotometer
Manufacturer	:	Thermo Scientific
Model	:	Genesys 20
Serial No.	:	[REDACTED]
ID No.	:	[REDACTED]
Customer	:	Special Lab Envi And Consultant Co., Ltd.
	:	47/91-93 Moo 3, Tambol Tait , Amphur Pakrad,
	:	Nonthaburi, 11120.
Location	:	Becthai Laboratory (Bangkok)
Date of Receipt	:	3 May 2023
Date of Calibration	:	3 May 2023
Date of Issue	:	3 May 2023
Ambient Temperature	:	(25±10) °C
Relative Humidity	:	(60±20) %
Condition As-Received	:	Used Item

Calibrated by

(Mr.Somphop Duangnguan)

Calibration Engineer

Approved by

(Ms. Jintana Sangthaijaroenlap)

Calibration Manager

The reported expended uncertainty of measurement was based on a combined standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Indicated values are valid for the state of the Spectrophotometer at the time of calibration only.



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : [REDACTED]

Page : 2 of 3

CALIBRATION REPORT

Conditions of this result of calibration

1. Reference Standard Material :

<u>Material</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert.No.</u>	<u>Due date</u>
Holmium Glass Filter	RM-HG	[REDACTED]	[REDACTED]	12 Feb 24
Didymium Glass Filter	RM-DG			12 Feb 24
Neutral Density Filter	RM-1N2N3N			13 Feb 24

2. Traceability : This certification is traceable to the International System of Unit maintained at;
The Sarna Scientific Ltd. Accredited Calibration Laboratory No. 0659.

3. Method of calibration :

The calibration procedure was carried out according to ASTM E275-08 (2022) and ASTM E925-09 (2014).

4. Result of calibration :

(☒) without adjustment

(☐) after adjustment

5. Equipment Specifications:

Spectral Bandwidth :	5	nm
Data Interval :	1	nm
Scan Speed :	N/A	nm/min



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : [REDACTED]

Page : 3 of 3

CALIBRATION REPORT

Wavelength Calibration

Certified Values of Reference Material (nm)	Nominal Value (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty of Measurement ($\pm$ nm)
418.40	418	418	-0.40	0.59
537.00	537	537	0.00	0.59
638.00	638	638	0.00	0.59

Photometric Calibration for Visible

Wavelength (nm)	Certified Values of Reference Material (A)	UUC* Reading (A)	Error (A)	Uncertainty of Measurement ($\pm$ A)
420.0	Zero	0.000	0.0000	0.0028
	0.5716	0.572	0.0004	0.0044
	0.7358	0.733	-0.0028	0.0040
	1.0713	1.073	0.0017	0.0039
440.0	Zero	0.000	0.0000	0.0028
	0.561	0.560	-0.0010	0.0042
	0.718	0.714	-0.0040	0.0037
	1.0459	1.044	-0.0019	0.0037
465.0	Zero	0.000	0.0000	0.0028
	0.5111	0.513	0.0019	0.0044
	0.6618	0.661	-0.0008	0.0035
	0.9635	0.966	0.0025	0.0034
546.1 (546.0)	Zero	0.000	0.0000	0.0028
	0.5222	0.523	0.0008	0.0036
	0.6687	0.668	-0.0007	0.0031
	0.9768	0.978	0.0012	0.0043
590.0	Zero	0.000	0.0000	0.0028
	0.5541	0.554	-0.0001	0.0035
	0.6975	0.696	-0.0015	0.0031
	1.0206	1.021	0.0004	0.0045
635.0	Zero	0.000	0.0000	0.0028
	0.5398	0.543	0.0032	0.0035
	0.6658	0.667	0.0012	0.0033
	0.9741	0.977	0.0029	0.0045

Remark : Each individual filter is measured against the empty filter holder (blank) used to zero the Spectrophotometer.

Note:

UUC* : Unit Under Calibration

- End of Report -

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrasan 3 Rd., Bangpoo, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



Certificate of Calibration

Certificate No. :



Page : 1 of 2

Submitted by :

Special Lab Envi and Consultant Co., Ltd.

47/91-93,96 Moo 3.Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment :

Digital Thermo-Hygrometer

Manufacturer : Testo

Model : 608-H1

Range Temperature : 0 °C to 50 °C

Resolution : 0.1 °C

Range Humidity : 10 %R.H. to 95 %R.H.

Resolution : 0.1 %R.H.

Serial No. :



ID No. :



Environment :

Ambient Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Date of Received : 03 August 2023

Date of Calibration : 09 August 2023

Date of Issue : 09 August 2023

Calibrated by :



Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4013

by compared with standard probe sensor humidity/temperature into humidity/temperature chamber.

Reference Standard Instruments : This certification is traceable to the International System of Units

Digital Indicator with Standard Probe Temp&Hum

ID No.

Cert. No.

Due Date

Traceability

400034 & 400035 SG-H-00502/66

06 Jan 2024

Success Gateway Co., Ltd., Accredited by TISI Calibration No.0268

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.




CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 

Page : 2 of 2

UUC Condition As-Received : Good

Result of Calibration : Without Adjustment

Function : Temperature measurement

Reference Humidity @ 50 %R.H.

Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25.01	25.0	0.0	0.46

Result of Calibration : Without Adjustment

Function : Humidity measurement

Reference Temperature @ 25 °C

Standard Humidity (%R.H.)	UUC Reading (%R.H.)	Correction (%R.H.)	Uncertainty (± %R.H.)
49.97	57.0	-7.0	2.2

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -

