

ภาคผนวก ณ

ใบรับรองการสอบเทียบเครื่องมือ



รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Noise	Leq 24 hrs	Sound Calibrator	BKK_FS0607	26-Jan-23	26-Jan-24	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0028	14-Mar-23	14-Mar-24	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0033	2-Nov-22	2-Nov-23	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0097	13-Dec-22	13-Dec-23	12
Noise	Leq 24 hrs	Sound Calibrator	BKK_FS0617	19-Oct-23	19-Oct-24	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0108	19-Jan-23	19-Jan-24	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0115	3-Jan-23	3-Jan-24	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0971	19-Jan-23	19-Jan-24	12
Water Lab	pH at 25 °C	pH meter	BKK_EN0072	12-Sep-22	12-Mar-24	18
Water Lab	Total Alkalinity	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Total Hardness	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Color	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Turbidity	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Dissolved Oxygen	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Dissolved Oxygen	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Nitrate	Ion Chromatography	BKK_EN0069	12-Jan-23	12-Jan-24	12
Water Lab	Phosphate	Ion Chromatography	BKK_EN0069	12-Jan-23	12-Jan-24	12
Water Lab	Chloride	Ion Chromatography	BKK_EN0069	12-Jan-23	12-Jan-24	12
Water Lab	Sulfate	Ion Chromatography	BKK_EN0069	12-Jan-23	12-Jan-24	12
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Water Lab	Total Solids	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Solids	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Water Lab	Total Kjeldahl Nitrogen	Digestion Unit	BKK_EN0366	17-May-23	17-May-24	12
Water Lab	Total Kjeldahl Nitrogen	Discrete analyzer	BKK_EN0037	12-Jul-23	12-Jul-24	12
Water Lab	Conductivity	Conductivity meter	BKK_EN0373	3-Jan-23	3-Jan-24	12
Water Lab	Salinity	Conductivity meter	BKK_EN0373	3-Jan-23	3-Jan-24	12
Water Lab	BOD	DO Meter	BKK_EN0205	3-Aug-22	3-Feb-24	18
Water Lab	BOD	Incubator	BKK_EN0272	5-Jul-23	5-Jul-24	12
Water Lab	COD	Hot Block	BKK_EN0222	25-Apr-23	25-Apr-24	12
Water Lab	COD	Spectrophotometer	BKK_EN0018	15-Sep-23	15-Sep-24	12
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0148	4-Jul-23	4-Jan-25	18
Water Lab	Temperature	Digital Thermometer With Sensor	BKK_LG0055	24-Aug-23	24-Aug-24	12
Water Lab	Temperature	Digital Thermometer With Sensor	BKK_LG0054	24-Aug-23	24-Aug-24	12
Water Lab	Hexavalent Chromium	Spectrophotometer	BKK_EN0018	15-Sep-23	15-Sep-24	12
Water Lab	Iron	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Iron	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Iron	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Lead	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Lead	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Lead	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Manganese	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Manganese	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Manganese	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Calcium	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	18
Water Lab	Calcium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Calcium	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Magnesium	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	18
Water Lab	Magnesium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Magnesium	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Copper	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Copper	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Copper	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Cadmium	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Cadmium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Cadmium	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18



รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Water Lab	Zinc	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Zinc	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Zinc	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Nickel	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Nickel	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Nickel	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Selenium	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Selenium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Selenium	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Barium	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Barium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Barium	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Arsenic	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Arsenic	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Arsenic	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Mercury	DUO-CVAFS / CVAAS	BKK_EL0023	24-May-23	24-May-24	12
Water Lab	Total Coliform	Autoclave	BKK_ML0037	17-Jul-23	17-Jan-25	18
Water Lab	Total Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	Total Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Fecal Coliform	Autoclave	BKK_ML0037	17-Jul-23	17-Jan-25	18
Water Lab	Fecal Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	Fecal Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Fecal Coliform	Water Bath	BKK_ML0056	20-Apr-23	20-Apr-24	12

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.comCert. No. : ACC23008
Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR
Manufacturer : RION
Model : NC-73
Serial No. : 10196929
ID No. : BKK_FS0607

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTANAKAN 40, PHATTANAKAN ROAD,
KHWAENG PHATTANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 24 JANUARY 2023
Calibration Date : 26 JANUARY 2023
Date of Issue : 27 JANUARY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced
other than in full, except with the prior written approval of the head of Calibration Laboratory.

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACC23008
Job No. : VC66AC0031
Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL_BP_04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL_BP_03/0265	09-Feb-23
Digital Multimeter	33461A	MY60024273	EEL_BP_05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23
Audio Analyzer	AVR-3360A	V744B6069	EF-0010-22	07-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACC23008
Job No. : VC66AC0031
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit (dB)
94	93.7	-0.30	3.91	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Tolerance limit (%)
1000	978.7	-2.1	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Tolerance limit (%)
1.70	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 23-SLM-091
Request No : Req-2023-0517

Unit Under Calibration Details

Measurement Item : Sound Level Meter
Microphone Class : 2
Manufacturer : RION
Microphone Model : UC-52
Model : NL-42
Microphone S/N : 157228
Serial Number : 00710644
Preamplifier Model : NH-24
ID : BKCF-50028
Preamplifier S/N : 10645
Resolution : 0.1 dB
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 1 March 2023
Calibrated Date : 14 March 2023
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	S/N	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Multi-frequency Calibrator	Quest	Quest-cal	EFA000234	29 June 2023	TSH
Audio Generator	Svanick	Svan401	131	12 October 2023	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppon Luangrat

Calibration Officer

Approved By : Mr. Pacit Mahaveen

Calibration Engineer Supervisor

Issue Date : 14 March 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

ISM-709-SLM-01 Rev.0 Issue date 01/07/19

Certificate No : 23-SLM-091
Request No : Req-2023-0517

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust	Adjust	UNCERTAINTY	Acceptance
FAST / A / 30-130	Level	UUC	ERR	UUC	ERR
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)
1000 Hz 114.00 dB	113.79	113.9	+0.11	113.8	+0.01
				(± dB)	(± dB)
				0.20	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130	(dB)	(± dB)
UUC Weighting	(dB)	(± dB)
A	14.9	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130	(dB)	(± dB)
UUC Weighting	(dB)	(± dB)
A	11.7	0.10
C	16.1	0.10
Z	20.6	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve	UNCERTAINTY	Acceptance
FAST / 30-130	A C Z	(± dB)	Limit
STD Setting	(dB) (dB) (dB)	(± dB)	(± dB)
125 Hz	0.4 0.5 0.5	0.50	1.5
1000 Hz	0.0 0.0 0.0	0.60	1.0
4000 Hz	-1.1 -1.1 -1.1	0.60	3.0
8000 Hz	-1.8 -1.7 -1.8	0.70	3.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

ISM-709-SLM-01 Rev.0 Issue date 01/07/19

Certificate No : 23-SLM-091
Request No : Req-2023-0517

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve	UNCERTAINTY	Acceptance
FAST / 30-130	A (dB) C (dB) Z (dB)	(± dB)	Limit
STD Setting	(dB) (dB) (dB)	(± dB)	(± dB)
63 Hz	-0.2 -0.1 -0.1	0.2	2.0
125 Hz	-0.1 0.0 -0.1	0.2	1.5
250 Hz	-0.1 0.0 0.0	0.2	1.5
500 Hz	-0.1 0.0 0.0	0.2	1.5
1000 Hz	0.0 0.0 0.0	0.2	1.0
2000 Hz	0.0 0.0 0.0	0.2	2.0
4000 Hz	0.0 0.0 0.0	0.2	3.0
8000 Hz	0.0 0.0 0.0	0.2	5
16000 Hz	-1.4 -1.4 0.0	0.2	+5, -INF.

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured	UNCERTAINTY	Acceptance
FAST / 30-130	REF	UUC	ERR	Limit
UUC Weighting	(dB)	(dB)	(dB)	(± dB)
A	114.00	114.0	0.0	0.2
C	114.00	114.0	0.0	0.2
Z	114.00	114.0	0.0	0.2

UUC Setting	STD	Measured	UNCERTAINTY	Acceptance
30-130 / A	REF	UUC	ERR	Limit
UUC Time Response	(dB)	(dB)	(dB)	(± dB)
Fast	114.00	114.0	0.0	0.1
Slow	114.00	114.0	0.0	0.1
Leq	114.00	114.0	0.0	0.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

ISM-709-SLM-01 Rev.0 Issue date 01/07/19

Certificate No : 23-SLM-091
Request No : Req-2023-0517

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 30-130	UUC		Limit
STD Setting	(dB)	(± dB)	(± dB)
Initial	114.0		
Final	114.0		
Deviated	0.0	0.1	0.3

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation	UNCERTAINTY	Acceptance
FAST / A / 30-130	REF	UUC	ERR	Limit
STD dB	(dB)	(dB)	(dB)	(± dB)
130.00	130	130.0	0.0	1.1
129.00	129	129.0	0.0	1.1
124.00	124	124.0	0.0	1.1
119.00	119	119.0	0.0	1.1
114.00	114	114.0	0.0	1.1
109.00	109	109.0	0.0	1.1
104.00	104	104.0	0.0	1.1
99.00	99	99.0	0.0	1.1
94.00	94	94.0	0.0	1.1
89.00	89	89.0	0.0	1.1
84.00	84	84.0	0.0	1.1
79.00	79	79.0	0.0	1.1
74.00	74	74.0	0.0	1.1
69.00	69	69.0	0.0	1.1
64.00	64	64.0	0.0	1.1
59.00	59	59.0	0.0	1.1
54.00	54	54.0	0.0	1.1
49.00	49	49.0	0.0	1.1
44.00	44	44.0	0.0	1.1
39.00	39	39.1	0.1	1.1
34.00	34	34.2	0.2	1.1
29.00	29	29.5	0.5	1.1
24.00	24	24.6	0.6	1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FSM-700-SLM-01 Rev.0 Issue date 01/07/19

Certificate No : 23-SLM-091
Request No : Req-2023-0517

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 30-130	UUC		Limit
STD Setting	(dB)	(± dB)	(± dB)
Positive one-half cycle	139.5		
Negative one-half cycle	139.3		
Deviated	0.2	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 30-130	UUC		Limit
STD Setting	(dB)	(± dB)	(± dB)
Initial	129.0		
Final	129.0		
Deviated	0.0	0.1	0.3

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FSM-700-SLM-01 Rev.0 Issue date 01/07/19

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthon Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel:0-2435-8800 Fax:0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



Cert. No. : ACL22253
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01122504 / 169436 / 72457
ID No.: BKK_FS0033

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 01 NOVEMBER 2022
Calibration Date : 02-03 NOVEMBER 2022
Date of Issue : 04 NOVEMBER 2022



Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL22253
Job No. : VC66AC0004
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL-BP_04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL-BP_03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL-BP_05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KA1	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

T. Petchur

Continuation of Calibration Certificate

Cert. No. : ACL22253
Job No. : VC66AC0004
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

QF-TS12-04-04-020664

T. Retch.

Continuation of Calibration Certificate

Cert. No. : ACL22253
Job No. : VC66AC0004
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	13.8
C - weight	19.9
Flat	25.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.4	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-1.3	-1.2	-1.1	±5.0

QF-TS12-04-04-020664

T. Retch.

Continuation of Calibration Certificate

Cert. No. : ACL22253
Job No. : VC66AC0004
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

T. Retch.

Continuation of Calibration Certificate

Cert. No. : ACL22253
Job No. : VC66AC0004
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.8	-0.2	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.8	-0.2	± 1.1

QF-TS12-04-04-020664

T. Retch.

Continuation of Calibration Certificate

Cert. No. : ACL22253
Job No. : VC66AC0004
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.7	-0.7	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

QF-TS12-04-04-020664

T. Petchur

Continuation of Calibration Certificate

Cert. No. : ACL22253
Job No. : VC66AC0004
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	(dB)	(dB)
89.6	89.7	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

T. Petchur

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY451-451/1 Sirinthorn Rd., Bangbunmu, Bangplud Bangkok 10700 THAILAND.
Tel:0-2435-8800 Fax:0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.comCert. No. : ACL22287
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00658240 / 157780 / 48095
ID No.: BKK_FS0097

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD,
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 30 NOVEMBER 2022
Calibration Date : 13-16 DECEMBER 2022
Date of Issue : 19 DECEMBER 2022

Calibrated by : Nadiakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL22287
Job No. : VC66AC0015
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM). The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL-BP_04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL-BP_03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL-BP_05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QF-TS12-04-04-020664

T. Petchur

Continuation of Calibration Certificate

Cert. No. : ACL22287
Job No. : VC66AC0015
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

QF-TS12-04-04-020664

T. R. L.

Continuation of Calibration Certificate

Cert. No. : ACL22287
Job No. : VC66AC0015
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.9

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.6
C - weight	18.4
Flat	24.4

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.2	0.2	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-1.0	-1.0	-1.0	±5.0

QF-TS12-04-04-020664

T. R. L.

Continuation of Calibration Certificate

Cert. No. : ACL22287
Job No. : VC66AC0015
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

QF-TS12-04-04-020664

T. R. L.

Continuation of Calibration Certificate

Cert. No. : ACL22287
Job No. : VC66AC0015
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

QF-TS12-04-04-020664

T. R. L.

Continuation of Calibration Certificate

Cert. No. : ACL22287
Job No. : VC66AC0015
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL22287
Job No. : VC66AC0015
Pages : 8 of 8

11. Overload Indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.7	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A-weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.comCert. No. : ACC23038
Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR
Manufacturer : RION
Model : NC-74
Serial No.: 34425566
ID No.: BKK_FS0617

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 22 SEPTEMBER 2023
Calibration Date : 19 OCTOBER 2023
Date of Issue : 19 OCTOBER 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACC23038
Job No. : VC66AC0101
Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.
The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 30/0267	13-FEB-24
Digital Multimeter	33461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KA1	34560495	AA-3002-23	14-FEB-24
Audio Analyzer	AVR-3360A	V744B6069	EF-0012-23	10-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QF-TS12-04-04-020664

Cert. No. : ACC23038
Job No. : VC66AC0101
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94,17	0,17	0,14	0,40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1001,9	0,2	0,1	1,0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
1,21	0,10	3,0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

T. Petchurai

451-451/1 Sirinthorn Rd, Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel:0-2435-8800 Fax:0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com

Cert. No. : ACL23056
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00858518 / 158769 / 58770
ID No.: BKK_FS0108

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD,
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23,0 ± 3) °C
Pressure : (101,3 ± 3) kPa
Relative Humidity : (50,0 ± 20) %

Received Date : 17 JANUARY 2023
Calibration Date : 19-20 JANUARY 2023
Date of Issue : 23 JANUARY 2023



Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

Cert. No. : ACL23056
Job No. : VC66AC0026
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL-BP_04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL-BP_03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL-BP_05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KA1	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL23056
Job No. : VC66AC0026
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0,2	N/A
2. Self-generated noise	✓	-	0,2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0,3	0,6
1000 Hz	✓	-	0,3	0,6
8000 Hz	✓	-	0,3	0,7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0,3	0,6
For > 4 kHz to 10 kHz	✓	-	0,3	0,7
For > 10 kHz to 20 kHz	-	-	-	1,0
5. Frequency and time weightings at 1 kHz	✓	-	0,2	0,2
6. Long - term stability	✓	-	0,1	0,1
7. Level linearity on the reference level range	✓	-	0,2	0,3
8. Level linearity including the level range control	✓	-	0,2	0,3
9. Tone burst response	✓	-	0,2	0,3
10. Peak C sound level	✓	-	0,2	0,35
11. Overload indication	✓	-	0,2	0,25
12. High level stability	✓	-	0,1	0,1

QF-TS12-04-04-020664

T. Petchurai

QF-TS12-04-04-020664

T. Petchurai

Continuation of Calibration Certificate

Cert. No. : ACL23056
Job No. : VC66AC0026
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
17.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	14.8
C - weight	20.8
Flat	26.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.3	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-0.8	-0.7	-0.7	±5.0

QF-TS12-04-04-020664

7. Rth

Continuation of Calibration Certificate

Cert. No. : ACL23056
Job No. : VC66AC0026
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.1	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

QF-TS12-04-04-020664

7. Rth

Continuation of Calibration Certificate

Cert. No. : ACL23056
Job No. : VC66AC0026
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	29.0	0.0	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.8	-0.2	± 1.1

QF-TS12-04-04-020664

7. Rth

Continuation of Calibration Certificate

Cert. No. : ACL23056
Job No. : VC66AC0026
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	132.9	-0.1	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

QF-TS12-04-04-020664

7. Rth

Continuation of Calibration Certificate

Cert. No. : ACL23056
Job No. : VC66AC0026
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.7	89.5	-0.2	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

451-451/1 Sirinthorn Rd, Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel:0-2435-8800 Fax:0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.comCert. No. : ACL23005
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00858525 / 170383 / 72889
ID No.: BKK_FS0115

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %
Received Date : 14 DECEMBER 2022
Calibration Date : 03-05 JANUARY 2023
Date of Issue : 06 JANUARY 2023



Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced
other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL23005
Job No. : VC66AC0021
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference
Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL-BP_04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL-BP_03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL-BP_05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL23005
Job No. : VC66AC0021
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL23005
Job No. : VC66AC0021
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.5

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	14.2
C - weight	20.4
Flat	25.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.3	0.3	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-1.7	-1.6	-1.6	±5.0

QF-TS12-04-04-020664

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23005
Job No. : VC66AC0021
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	-0.1	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23005
Job No. : VC66AC0021
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.1	0.1	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.1	0.1	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.0	0.0	± 1.1

QF-TS12-04-04-020664

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23005
Job No. : VC66AC0021
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

QF-TS12-04-04-020664

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23005
Job No. : VC66AC0021
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664



451-451/1 Sirinthorn Rd., Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com

Cert. No. : ACL23052
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00296514 / 179116 / 87523
ID No.: BKK_FS0971

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 17 JANUARY 2023
Calibration Date : 19-20 JANUARY 2023
Date of Issue : 23 JANUARY 2023



Calibrated by : Nathakorn Pisutpaisan

Approved by : T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL23052
Job No. : VC66AC0026
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL_BP_04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL_BP_03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL_BP_05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL23052
Job No. : VC66AC0026
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

QF-TS12-04-04-020664

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL23052
Job No. : VC66AC0026
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	10.8
C - weight	16.7
Flat	22.5

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.4	0.4	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-0.9	-0.9	-0.9	±5.0

QF-TS12-04-04-020664

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23052
Job No. : VC66AC0026
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A -weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23052
Job No. : VC66AC0026
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	130.9	-0.1	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.1	0.1	± 1.1

QF-TS12-04-04-020664

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23052
Job No. : VC66AC0026
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.7	-0.7	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

QF-TS12-04-04-020664

7. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23052
Job No. : VC66AC0026
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES
1344 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-21 FAX. 0-2719-0484



Cert.No.: 22CH1222
Page.: 1 of 2

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Mettler Toledo
Model : Seven Compact S220
Serial No. : B520948426
ID No. : BKK_EN0072
Condition As-Received : Used Item
Received Date : 09 September 2022
Calibration Date : 12 September 2022
Reference : 2209-0312DSC-1
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwang Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard
voltage calibrator and direct measurement
with certified reference material (CRM)

REVIEW BY	Sinluk P.
APPROVED BY	KLAL
NEXT CAL. DATE	12/03/24

Calibrated by : Warakorn Lemgagrakul

Approved by :
Approved Signatory

(/) Malee Butkruea
() Sathip Meangmai
() Warakorn Lemgagrakul

Issue Date : 15 September 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services, Engineering Calibration and Testing Services.



Cert. No.: 22CH1222
Page.: 2 of 2

Condition of this calibration result

1. Reference Standard Instrument

Instrument Serial No. ID No. Cert. No. Due Date
1) Document Process Calibrator 54030049 130RC116 22E2769 24 Aug 2023

This certification is traceable to the International System of Unit maintained at:-
- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	823320	20 June 2024
pH 6.985	CPA chem	794122	14 Feb 2023
pH 10.008	CPA chem	823323	20 June 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
			mV	pH		
pH Meter S/N : B520948426	4.000	177.48	177.4	4.000	0.058	2.00
	7.000	0.00	0.0	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor k
pH Electrode S/N : PCE-88-EX1001	4.008	3.999	153.9	0.0055	2.09
	6.985	7.017	-13.7	0.0084	2.00
	10.008	9.985	-179.0	0.0078	2.06

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

000-

Wale

a 1126274



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES
1344 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-21 FAX. 0-2719-0484



Cert.No.: 22CG3154
Page.: 1 of 2

Certificate of Calibration

Equipment : Burette
Capacity : 50 mL
Serial No. :
ID No. : BKK_EN0171
Manufacturer : Witeg
Made in : Germany
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.
Khwang Phatthanakan, Khet Suan Luang
Bangkok 10250 Thailand
Ambient Temperature : (20 ± 2.5) °C
Relative Humidity : (50 ± 10) %
Barometric Pressure : 759 mmHg
Calibration Procedure : ASTM E 542 - 01

REVIEW BY	Sinluk P.
APPROVED BY	KLAL
NEXT CAL. DATE	11/03/2024

Calibrated by : Panward Pramklam

Approved by :
Approved Signatory

() Pornthipha Tameyakul
() Malee Butkruea
(/) Ponpan Palpim
() Srisuda Khamthia

Issue Date : 31 August 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services, Engineering Calibration and Testing Services.

A 0044607



Equipment : Burette
 Received Date : 28 August 2022
 Condition As-Received : Used Item
 Calibration Date : 30 August 2022
 Reference : 2208-0818DSC-2

Cert.No.: 22CG3154
 Page: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID No.	Certificate No.	Traceability	Due date
1) Balance	AE2005	N03679	140RC091	21MM429	NIMT	22 Sep 2022
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	22H1243	NIST, NIMT	09 June 2023
3) Thermometer	-	1584592	140EC010	221181	NIMT	10 Feb 2023

This certification is traceable to SI Unit

- The certificate is valid only to the item calibrated on date and place of calibration.
- True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	k Factor
50	48.9859	0.010	2.00

Remark : mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

1123908



Metrological Center
 SCI ECO Services Company Limited
 33/2 Moo 3, T.Banpa, A.Kaengkhroi, Saraburi 18110, Thailand.
 Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100
 Bangkok Tel : +668 9205 6851 , +669 8247 2360
 Website : www.scieco.co.th E-Mail : calibrate@scg.co.th



Certificate No. T221644

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Cold Room)

Manufacturer : KOLDTECH

Model : KM 320

Serial No. : TBN-1012061/05

Customer Code : BKK_EN0167

ID No. : T2463A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Environmental Laboratory

Date of Receipt : 27 June 2022

Calibrated By : Sujjar Nakhakred (Site Calibration Manager)

Approved By : / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 6 JUL 2022

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L13 11/7/01-02-04



Metrological Center
 SCI ECO Services Company Limited
 33/2 Moo 3, T.Banpa, A.Kaengkhroi, Saraburi 18110, Thailand.



Certificate No. T221644

Page 2 of 4

Calibration Report

Equipment : Chamber (Cold Room)
 Date of Calibration : 30 June - 1 July 2022
 Environment : Temperature : 18.9-23.7 °C
 Line Voltage : 222.9-226.5 V
 Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

- This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T210009	30 July 2022
TC	TYPE T	TN171-TN180	T210009	30 July 2022
DATA LOGGER	34970A	T149	T210009	30 July 2022

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244)

4. Condition of calibrated item : good

Equipment Description :

Time Constant : 3 Hour - Minute At 3 °C
 Fresh Air Damper : ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

() without adjustment (X) after adjustment

Approved By:

FM-L13 11/7/01-03-03




Metrological Center
 SCI ECO Services Company Limited
 33/2 Moo 3, T.Banpa, A.Kaengkhroi, Saraburi 18110, Thailand.



Certificate No. T221644

Page 3 of 4

Calibration Report

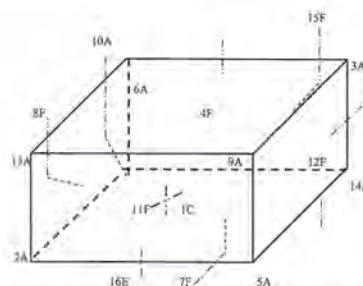

C = Centre, F = Centre of Face, A = Corner, E = Centre of Edge.

1C = TN161
2A = TN162
3A = TN163
4F = TN164
5A = TN165
6A = TN166
7F = TN167
8F = TN168
9A = TN169
10A = TN170

11F = TN171
12F = TN172
13A = TN173
14A = TN174
15F = TN175
16E = TN176

Approved By:

FM-L13 11/7/01-03-03

Certificate No. T221644

Page 4 of 4

Calibration Report

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)									
	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170
3	2.71	2.82	2.75	2.89	2.95	3.08	3.02	2.96	3.03	2.85
	TN171	TN172	TN173	TN174	TN175	TN176				
	2.97	3.02	2.89	3.04	2.97	3.33				

Chamber (Cold Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor k
	Min, Max	Average					
3.0	2.9, 4.0	3.2	2.99	1.05	1.30	1.66	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate at shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k, which for a t-distribution, providing a level of confidence of approximately 95 %.

Approved By: 

TM-L15117/15-05-03

GUL-EN0069

 REVIEW BY: Autcharawan S.
 APPROVED BY: Sirarat M.
 NEXT CAL DATE: 12.3.2024


Certificate of Calibration

ICS-2100: Anion (ID#659)

This certificate is to verify that instrument below are calibrated

by Archimica Lab Co., Ltd.

ICS-2100 S/N: 15010977

AS-HV S/N: 5450A36659

For

ALS Laboratory Group (Thailand) Co., Ltd.

Operator Signature: Nutdanai Date: Jan 12, 2023

(Mr. Nutdanai Laekhwan)

Application Chemist

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2043 8361-6 Fax: +66 2043 8367, e-mail: service.thailand@sartorius.comMSC-TS1-17025
CALIBRATION 0426

SARTORIUS

 REVIEW BY: Sirarat P.
 APPROVED BY: U. A.
 NEXT CAL DATE: 8/1/24

 Model Number: MSE224S-100-DU
 Description: Analytical Balance
 Serial Number: 26207042
 ID No.: BKK_EN0002
 Manufacturer: Sartorius

 Certificate No.: 23BC10072
 Issued Date: Monday, February 13, 2023
 Reference No.: 203245
 Page No.: 1 of 2

Customer Name: ALS Laboratory Group (Thailand) Co., Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.

Calibrated Place: Balance Room

 Calibrated By: Mr. Chonchai Inthana
 Calibration Date: Wednesday, February 08, 2023

 Calibration Procedure No.: This calibration was conducted by
 Using in-house calibration procedure number (WI-003)
 Based on UKAS LAB 14 : 2019

Metrological data:

Capacity: 220 g Readability: 0.0001 g

Ambient Conditions:

 Temperature: 23.2 °C ± 5.0 °C
 Humidity: 60.0 % RH ± 10.0 % RH
 Pressure: ±

Equipment Condition:

☒ Good Operator ☐ Fair

Reasons for calibration

☐ New Installation ☐ Service / Repair ☒ Re-calibration / Maintenance

Measurement Method UKAS Publication Ref: Lab 14

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to the Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YC5011-522-00	Sartorius weight set 1mg - 5000g E2 YC5011-522-00	SPC-RT	C02212566	14-Sep-2023
MHB-382SD	Humidity/Balance/Temp. Lution MHB-382SD	DKSH	C18220444	5-Sep-2023

 This certificate relate and apply this equipment only.
 This certificate may not be reproduced other than in full except with
 the prior written approval of the Verification Operation Division
 Sartorius (Thailand) Co., Ltd.

Mr. Chonchai Inthana (Technical Manager)



SOP FM 33 03 February 2022

Sartorius (Thailand) Co., Ltd.

 129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
 Tel: +66 2043 8361-6 Fax: +66 2043 8367, e-mail: service.thailand@sartorius.com

SARTORIUS

Certificate of Calibration

 Model Number: MSE224S-100-DU
 Description: Analytical Balance
 Serial Number: 26207042
 ID No.: BKK_EN0002
 Manufacturer: Sartorius

 Certificate No.: 23BC10072
 Issued Date: Monday, February 13, 2023
 Reference No.: 203245
 Page No.: 2 of 2

Calibration Results : Without Adjustment

Repeatability			Eccentricity (Off-center loading error)		
The repeatability is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.			The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R110)		
Nominal Value : (Low Load)	20.0000	200.0000	Nominal value :	50	g
20 g	20.0000	199.9999	Tolerance	0.0004	g
Tolerance	0.0001 g	0.0000	Difference		
	20.0000	199.9999			
	20.0001	200.0000			
Nominal Value : (High Load)	200.0000	200.0000			
200 g	200.0000	199.9999			
Tolerance	0.0001 g	0.0000			
	20.0000	199.9999			
	20.0001	200.0000			
	20.0003	199.9999			
Standard Deviation		0.0000%			

Linearity

The linearity, also called linearity error, describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g				
Nominal Value	Conventional Mass Value	Displayed Value	Deviation	Uncertainty
(g)	(g)	(g)	(g)	(g)
0.01	0.01000	0.01000	0.00000	0.00014
0.1	0.10000	0.10000	0.00000	0.00014
1	1.00000	1.00000	0.00000	0.00014
2	2.00000	2.00000	0.00000	0.00014
5	5.00000	5.00000	0.00000	0.00014
10	10.00000	10.00000	0.00000	0.00014
20	20.00000	20.00000	0.00000	0.00014
50	50.00000	50.00000	0.00000	0.00015
100	100.00000	100.00000	0.00000	0.00019
200	200.00000	199.99999	-0.00001	0.00010

End of Report.

SOP FM 33 03 February 2022

Certificate No. T222502

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Oven)

Manufacturer : Memmert

Model : UF 450

Serial No. : B7170531

Customer Code : BKK_EN0273

ID No. : T8042A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250


Customer Location : Oven Room

Date of Receipt : 23 November 2022

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By : /Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 09 DEC 2022



The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L15117/15-05-63

Certificate No. T222502

Page 2 of 4

Calibration Report

Equipment : Chamber (Oven)

Date of Calibration : 29 November 2022

Environment : Temperature : 29.1-29.6 °C
Line Voltage : 221.3-223.2 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors and nine standard thermocouples type T into its chamber , the other one resistance thermometer detector use for ambient temperature measurement .
The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986) .
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	27-CH1-10	T210004	30 December 2022
TC	TYPE T	TN261-TN270	T210010	30 December 2022
DATA LOGGER	34970A	T149	T210004	30 December 2022

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244)

4. Condition of calibrated item : good

Equipment Description :

Time Constant : 1 Hour 49 Minute At 104 °C
Fresh Air Damper : ☒ Open ☐ Min ☐ Medium ☒ Max
☐ Close
☐ Not Available

5. Adjustment :

() without adjustment (X) after adjustment


Approved By:

FM-L15117/15-05-63

Certificate No. T222502

Page 3 of 4

Calibration Report

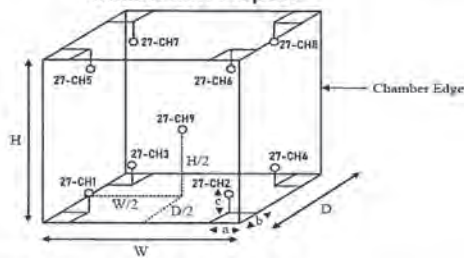

Remark :

Internal Dimensions of Chamber : W (Width) = 104 cm., H (Height) = 72 cm. and D (Depth) = 60 cm.
Size of Installed Standard sensor number 27-CH1 to number 27-CH9 : a = 5 cm, b = 5 cm, and c = 5 cm
Size of Installed Standard sensor number 27-CH9 : W/2 = 104 cm/2, H/2 = 72 cm/2, and D/2 = 60cm/2

Measurement Results

		Average Standard Reading at each position (°C)								
Calibration Point		27-CH1	27-CH2	27-CH3	27-CH4	27-CH5	27-CH6	27-CH7	27-CH8	27-CH9
104		101.07	103.80	103.45	104.62	104.47	103.57	104.39	103.75	104.18

Chamber (Oven)			Temperature Distribution					Coverage Factor k
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)		
	Min	Max						
104.0	-	104.0	103.97	0.07	0.70	0.42	2.00	

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k, which for a t-distribution, providing a level of confidence of approximately 95 %.


Approved By:

FM-L15117/15-05-63

Certificate No. T222502

Page 4 of 4

Calibration Report

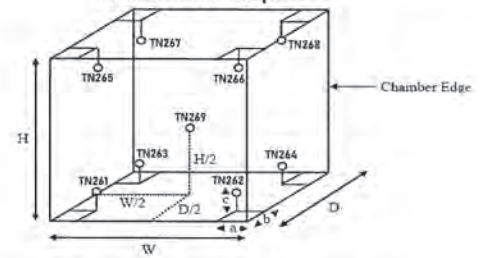

Remark :

Internal Dimensions of Chamber : W (Width) = 104 cm., H (Height) = 72 cm. and D (Depth) = 60 cm.
Size of Installed Standard sensor number TN261 to number TN269 : a = 5 cm, b = 5 cm, and c = 5 cm
Size of Installed Standard sensor number TN269 : W/2 = 104 cm/2, H/2 = 72 cm/2, and D/2 = 60cm/2

Measurement Results

Average Standard Reading at each position (°C)								
Calibration Point	TN261	TN262	TN263	TN264	TN265	TN266	TN267	TN268
180	179.14	179.17	179.65	179.26	180.41	179.64	181.18	180.99

Chamber (Oven)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor k
	Min	Max					
180.0	-	180.0	179.98	0.38	1.78	1.10	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k, which for a t-distribution, providing a level of confidence of approximately 95 %.

Approved By:

FM-L15117/15-05-63



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoh, Saraburi 18110


Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230902

Page 1 of 5

Certificate of Calibration

Equipment : Digestion Unit
Manufacturer : SCP Science
Model : DigiPRER HT
Serial No. : HTC1120480658
Customer Code : BKK_EN0366
ID No. : T2635A5
Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250
Customer Location : Wet Chemistry Lab 1
Date of Receipt : 10 May 2023
Calibrated By : Sujjar Naknakred (Site Calibration Manager)
Approved By :  / Boonchai Suriyawong (Site Calibration Manager)
Date of Issue : 29 MAY 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L12 108/30-05-57



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoh, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230902

Page 2 of 5

Calibration Report


Equipment : Digestion Unit
Date of Calibration : 17 May 2023
Environment : Temperature : 23.9 - 26.3 °C
Line Voltage : 221.8 - 225.9 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

- This equipment was calibrated by insert four standard thermocouples type S into its chamber, the other one thermocouple type T use for ambient temperature measurement. The calibration was done in according to WI-T10.
- Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M20A1-(CH17-CH20)	T230547	18 April 2024
DATA LOGGER	34970A	T149	T230547	18 April 2024
- This certificate is traceable to :
National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244J).
- Condition of calibrated item : good
Equipment Description :

Time Constant	1 Hour	54 Minute	At 380 °C
Fresh Air Damper	<input type="checkbox"/> Open <input type="checkbox"/> Min <input type="checkbox"/> Medium <input type="checkbox"/> Max		
	<input type="checkbox"/> Close		
	<input checked="" type="checkbox"/> Not Available		
- Adjustment :
(X) without adjustment () after adjustment

Approved By : 

FM-L13 108/30-05-57



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoh, Saraburi 18110


Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230902

Page 3 of 5

Calibration Report

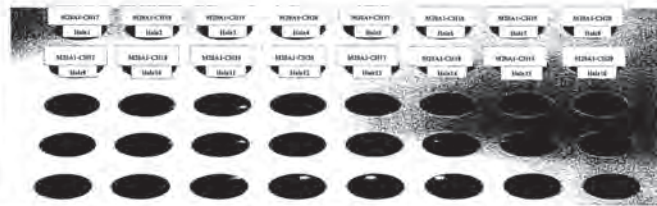

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
°C	°C	°C	Reading	Hole1	Hole2	Hole3	Hole4	Hole5	Hole6	Hole7	Hole8
380.0	380.0	379.4 - 380.7		M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH21	M20A1-CH22	M20A1-CH23	M20A1-CH24
			Max °C	377.3	379.0	379.2	380.2	377.5	379.5	380.7	380.1
			Min °C	376.8	378.6	378.9	379.9	377.0	379.0	380.2	379.6
			Average °C	377.6	378.8	379.1	380.0	377.5	379.2	380.4	379.9
			Stability ± °C	0.2	0.2	0.2	0.2	0.3	0.3	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
°C	°C	°C	Reading	Hole9	Hole10	Hole11	Hole12	Hole13	Hole14	Hole15	Hole16
380.0	380.0	379.4 - 380.7		M20A1-CH25	M20A1-CH26	M20A1-CH27	M20A1-CH28	M20A1-CH29	M20A1-CH30	M20A1-CH31	M20A1-CH32
			Max °C	377.3	378.9	379.7	379.9	379.3	379.6	379.5	377.8
			Min °C	376.7	378.3	379.3	379.5	378.9	379.1	379.9	377.0
			Average °C	376.9	378.7	379.5	379.7	379.1	379.4	379.3	377.2
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.3	0.3	0.2

Approved By : 

FM-L13 108/30-05-57



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoh, Saraburi 18110


Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230902

Page 4 of 5

Calibration Report

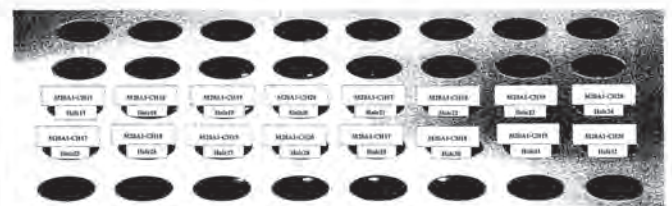

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
°C	°C	°C	Reading	Hole17	Hole18	Hole19	Hole20	Hole21	Hole22	Hole23	Hole24
380.0	380.0	379.4 - 380.7		M20A1-CH25	M20A1-CH26	M20A1-CH27	M20A1-CH28	M20A1-CH29	M20A1-CH30	M20A1-CH31	M20A1-CH32
			Max °C	378.4	380.1	380.1	380.0	379.1	379.8	379.6	377.8
			Min °C	377.8	379.6	379.7	379.3	378.6	379.2	379.2	377.3
			Average °C	378.1	379.9	379.9	379.7	378.9	379.5	379.4	377.5
			Stability ± °C	0.3	0.3	0.2	0.3	0.3	0.3	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
°C	°C	°C	Reading	Hole25	Hole26	Hole27	Hole28	Hole29	Hole30	Hole31	Hole32
380.0	380.0	379.4 - 380.7		M20A1-CH33	M20A1-CH34	M20A1-CH35	M20A1-CH36	M20A1-CH37	M20A1-CH38	M20A1-CH39	M20A1-CH40
			Max °C	377.9	379.4	380.1	380.1	379.3	379.6	378.9	377.3
			Min °C	377.4	378.9	379.7	379.7	378.8	378.9	378.4	376.7
			Average °C	377.7	379.2	379.9	379.9	379.0	379.3	378.6	377.6
			Stability ± °C	0.3	0.3	0.2	0.2	0.3	0.4	0.3	0.3

Approved By : 

FM-L13 108/30-05-57



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoei, Saraburi 18110


Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230902

Page 5 of 5

Calibration Report

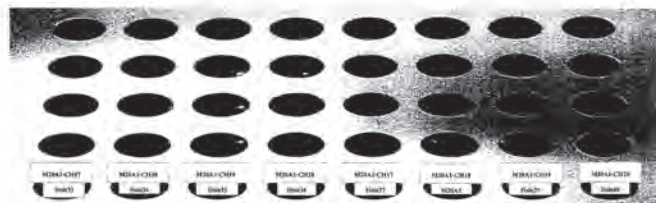

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD	Position of Standards at Block							
$^{\circ}\text{C}$	$^{\circ}\text{C}$	$^{\circ}\text{C}$	Reading	Hole33	Hole34	Hole35	Hole36	Hole37	Hole38	Hole39	Hole40
				NDA1-CUT	NDA1-CUR	NDA1-CHN	NDA1-CHN	NDA1-CHT	NDA1-CHN	NDA1-CHN	NDA1-CHN
			Max $^{\circ}\text{C}$	377.7	378.0	378.3	379.6	378.2	378.5	377.3	377.4
			Min $^{\circ}\text{C}$	377.3	377.6	377.9	378.6	377.7	378.1	376.9	377.0
			Average $^{\circ}\text{C}$	377.5	377.8	378.1	378.8	378.0	378.3	377.1	377.2
			Stability $^{\circ}\text{C}$	0.2	0.2	0.2	0.2	0.2	0.2	0.2	0.2

The expanded uncertainty of temperature measurement was $\pm 1.85^{\circ}\text{C}$

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %.

Approved By

FM-L13 108/30-05-57



บริษัท ดับเบิล เอส ไดแอกโนสติกส์ จำกัด
DOUBLE S DIAGNOSTICS CO., LTD.

10 หมู่ 11 ต.บ้านใหม่ อ.เมือง จ.นนทบุรี 11000 โทร : 02-555-1111 โทรสาร : 02-555-1112
100 หมู่ 11 ต.บ้านใหม่ อ.เมือง จ.นนทบุรี 11000 โทร : 02-555-1111 โทรสาร : 02-555-1112

Maintenance Plan YEAR : 2023

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
130							✓	✓				

Periodical maintenance check list for Konelab

	6M	12M	Note
1.Diluent-wash tubing change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
2.ISE tubing change	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	None
3.Syringe check/change		<input checked="" type="checkbox"/>	
4.Dispensing check/ change		<input checked="" type="checkbox"/>	
5.Waste tubing change when necessary		<input checked="" type="checkbox"/>	
6.Lamp check/change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
7.Mixer paddle/paddle change(not Konelab20)		<input checked="" type="checkbox"/>	
8.ISE needles check/change		<input checked="" type="checkbox"/>	None
9.Pump tubing check/ change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
10.Broken/worn out part check /change		<input checked="" type="checkbox"/>	
11.Peristaltic pump check /cleaning/ lubrication	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
12.Heating check		<input checked="" type="checkbox"/>	
13.Cooling check		<input checked="" type="checkbox"/>	
14.Dispenser mechanic check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
15.Cuvette transfer mechanic check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
16.Dispenser movement check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
17.Sample/reagent register check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
18.Dispensing tubing tightness check	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
19.Photometer and optics cleaning/check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
20.Workstation PC cleaning if necessary	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
21.Mechanic cleaning/lubrication	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
22.Instrument cleaning if necessary	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
23.Complete analyzer testing with waterblank/QC or sample	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
24.Test parameters/Adjustment/config. Save to USB key	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
25.UPS Test	<input type="checkbox"/>	<input checked="" type="checkbox"/>	

Place: AL3 LAB Instrument: K30 Aquakem
Date/Time: 12/7/66 Serial no: 07981
Service done by: 5025 Install date: 12/1/16
Signature of customer: 01991 Date/Time: 12/1/16

Accuracy results Aquakem 7.2.AQ2 Page: 1

Laboratory
Analyzer User

7/12/2023 21:21

Performed 7/12/2023
Sgt. W166

ACCEPTANCE CRITERIA

	Result	Limit	Warning
Temperature (°C)	37.7	37.0 +/- 1.0	
Dispensing ratio	16.4	14.8 - 17.2	
CV%	1.17	<1.7	
Photometric noise			
Max SD L340_2 (nA)	0.19	<2.0	
Max SD L340_4 (nA)	1.06	<3.0	
Linearity of photometer			
Slope	1.0198	0.94 - 1.06	
Curvature	0.0035	+/- 0.02	
Max bias from linear fit (nA)	3.2	<15.0	
Max delta %	-2.0	+/- 6.0	
Linearity of sample dispensing			
Proport. volume XDISP2 (??)	2.06	1.96 - 2.16	
Proport. volume XDISP4 (??)	4.13	3.85 - 4.40	
XDISP2 CV%	0.58	<2.0	
XDISP4 CV%	0.70	<2.0	
XDISP10 CV%	0.59	<2.0	
Needle 0.71 volume			
Average (A)	0.009	<0.050	
Standard deviation (A)	0.002	<0.005	
Volume (??)	0.06	<0.32	

OTHER INFORMATION

Dispensing ratio	Photom. noise: SD (nA)
Posit Result (A)	Posit L340_2 L340_4
1 0.1352	1 0.07 0.64
2 0.1624	2 0.09 1.05
3 0.1631	3 0.14 0.50
4 0.1631	4 0.13 0.53
5 0.1625	5 0.19 0.38
6 0.1650	6 0.02 0.64

Accuracy results Aquakem 7.2.AQ2 Page: 2

Laboratory
Analyzer User


7/12/2023 21:21

Linearity of sample dispensing

Test	Absorbance (A)
XDISP2	0.311
XDISP4	0.616
XDISP10	1.478

Linearity of photometer

L340	Target (A)	Meas (A)	Delta (A)	Delta %
1	0.001	0.005	-0.004	-294.7
2	0.512	0.519	-0.007	-1.3
3	1.523	1.550	-0.027	-1.8
4	2.027	2.066	-0.039	-1.9
5	2.532	2.582	-0.050	-2.0

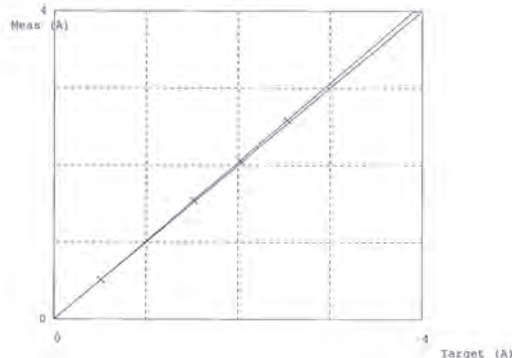



Certificate of Calibration

Equipment: CONDUCTIVITY METER
Model: ORION STAR A215
Serial No. (or ID.): X58031
Manufacturer: Thermo Scientific
Electrode Serial No.: YV1-18416
Condition: In Condition

Certificate No.: C24230001
Issued Date: 5 January 2023
Job No.: KSPR2216356
Page: 1 of 2
Model: ORION 013005MD
Brand: Thermo Scientific

Customer: ALS Laboratory Group (Thailand) Co., Ltd.
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Environment Condition: Temperature 21.6 °C ± 0.2 °C
Humidity 58.0 %RH ± 2.0 %RH

Calibration Place: ALS Laboratory Group (Thailand) Co., Ltd. (Wet Chemistry Lab 2)
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Calibration By: Mr.Nattapat Rungueang
Calibration Date: 3 January 2023
The Method used: In house method, CAL-WI-49, base on ASTM D 1125-14 and D 5391-14

Traceability: This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 836317, 838313, 838315

Signature

(Mr. Nattapat Rungueang)

Person in charge

Signature

(Mr. Nitinun Srihawan)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.
The measurement uncertainty stated in the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

DKSH Technology Limited
2533 Sukhumvit Road, Bangkok, Prachinburi, Bangkok 10250
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/calibration

Delivering Growth - In Asia and Beyond.

CAL-FM-C24-09: 12 Sep 2022



Certificate No.: C24230001

Page: 2 of 2

Calibration Results:

Before Adjustment

Standard Conductivity Solution	Unit Under Calibration Reading	Correction	Coverage Factor (k)	Uncertainty (±)
84.000 µS/cm	102.4 µS/cm	-18.400 µS/cm	2.00	0.68 µS/cm
1413.0 µS/cm	1689 µS/cm	-276.0 µS/cm	2.00	11 µS/cm
12.881 mS/cm	15.42 mS/cm	-2.5390 mS/cm	2.00	0.098 mS/cm

After Adjustment ; at 84.0 µS/cm, 1413 µS/cm, 12.88 mS/cm

Standard Conductivity Solution	Unit Under Calibration Reading	Correction	Coverage Factor (k)	Uncertainty (±)
84.000 µS/cm	84.08 µS/cm	-0.090 µS/cm	2.00	0.68 µS/cm
1413.0 µS/cm	1413 µS/cm	0.0 µS/cm	2.00	11 µS/cm
12.881 mS/cm	12.88 mS/cm	-0.0090 mS/cm	2.00	0.098 mS/cm

The End of Certificate

DKSH Technology Limited
2533 Sukhumvit Road, Bangkok, Prachinburi, Bangkok 10250
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/calibration

Delivering Growth - In Asia and Beyond.

CAL-FM-C24-09: 12 Sep 2022



ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: KSPR2216356

ชนิดเครื่องวัด: CONDUCTIVITY METER

รุ่น: ORION STAR A215

หมายเลขเครื่อง: X58031

ตรวจสอบ (วัน)	รายการตรวจสอบ	ตรวจสอบ (ส่ง)	หมายเหตุ
03 Jan 2023		03 Jan 2023	
ปกติ	ไม่ปกติ	ปกติ	ไม่ปกติ
General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Spectrophotometer			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
pH Meter and Conductivity Meter			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Turbidimeter			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Automatic Titrator			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>

ชื่อหน้า:

Mr.Nattapat Rungueang

Service Engineer

DKSH Technology Limited
2533 Sukhumvit Road, Bangkok, Prachinburi, Bangkok 10250
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/calibration

Delivering Growth - In Asia and Beyond.

CAL-FM-R31-03: 20 Jul 2022



Certificate of Calibration

Equipment: CONDUCTIVITY METER
Model: ORION STAR A215
Serial No. (or ID.): X58031
Manufacturer: Thermo Scientific
Electrode Serial No.: YV1-18416
Condition: In Condition

Certificate No.: C24230001
Issued Date: 5 January 2023
Job No.: KSPR2216356
Page: 1 of 2
Model: ORION 013005MD
Brand: Thermo Scientific

Customer: ALS Laboratory Group (Thailand) Co., Ltd.
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Environment Condition: Temperature 21.6 °C ± 0.2 °C
Humidity 58.0 %RH ± 2.0 %RH

Calibration Place: ALS Laboratory Group (Thailand) Co., Ltd. (Wet Chemistry Lab 2)
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Calibration By: Mr.Nattapat Rungueang
Calibration Date: 3 January 2023
The Method used: In house method, CAL-WI-49, base on ASTM D 1125-14 and D 5391-14

Traceability: This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 836317, 838313, 838315

Signature

(Mr. Nattapat Rungueang)

Person in charge

REVIEW BY
APPROVED BY
NEXT CAL. DATE

(Mr. Nitinun Srihawan)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.
The measurement uncertainty stated in the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

DKSH Technology Limited
2533 Sukhumvit Road, Bangkok, Prachinburi, Bangkok 10250
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/calibration

Delivering Growth - In Asia and Beyond.

CAL-FM-C24-09: 12 Sep 2022

Calibration Results:

Before Adjustment

Standard Conductivity Solution	Unit Under Calibration Reading	Correction	Coverage Factor (k)	Uncertainty (\pm)
84.000 $\mu\text{S/cm}$	102.4 $\mu\text{S/cm}$	-18.400 $\mu\text{S/cm}$	2.00	0.68 $\mu\text{S/cm}$
1413.0 $\mu\text{S/cm}$	1689 $\mu\text{S/cm}$	-276.0 $\mu\text{S/cm}$	2.00	11 $\mu\text{S/cm}$
12.881 mS/cm	15.42 mS/cm	-2.5390 mS/cm	2.00	0.098 mS/cm

After Adjustment : at 84.0 $\mu\text{S/cm}$, 1413 $\mu\text{S/cm}$, 12.88 mS/cm

Standard Conductivity Solution	Unit Under Calibration Reading	Correction	Coverage Factor (k)	Uncertainty (\pm)
84.000 $\mu\text{S/cm}$	84.09 $\mu\text{S/cm}$	-0.090 $\mu\text{S/cm}$	2.00	0.68 $\mu\text{S/cm}$
1413.0 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	0.0 $\mu\text{S/cm}$	2.00	11 $\mu\text{S/cm}$
12.881 mS/cm	12.89 mS/cm	-0.0090 mS/cm	2.00	0.098 mS/cm

The End of Certificate

Unit: Bangkok m/s/call only
DKSH Technology Limited
250 Sukhumvit Road, Bangkok, Phraechin, Bangkok 10260
Phone: +66 269 7100 Email: info@dksh.com Website: www.dksh.com/calibration-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C24-09: 12 Sep 2022

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: KSPR2216356

ชนิดเครื่องมือ: CONDUCTIVITY METER

รุ่น: ORION STAR A215

หมายเลขเครื่อง: X58031

ตรวจสอบ (รับ)	03 Jan 2023	รายการตรวจสอบ	ตรวจสอบ (ส่ง)	03 Jan 2023	หมายเหตุ
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
General					
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตช์ ปิด - เปิด เครื่อง (On-Off Switch)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
Spectrophotometer					
<input type="checkbox"/>	<input type="checkbox"/>	6. แรงดันไฟฟ้า (Battery Backup) ≥ 2.5 VDC	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	7. ตัวคูณเลือกความยาวคลื่น (Wavelength Control)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	9. แสงยูวี (UV $< 3,000$ hour)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	10. แสงที่มองเห็น (Visible $< 5,000$ hour)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	<input type="checkbox"/>	<input type="checkbox"/>	
pH Meter and Conductivity Meter					
<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. อิเล็กโทรด (Electrode and Connection Cable)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	13. ระดับสารละลายใน Electrode (Level KCl)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	<input type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	15. ขาจับอิเล็กโทรด (Stand)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
Turbidimeter					
<input type="checkbox"/>	<input type="checkbox"/>	16. ค่าความทึบที่ต่ำสุด (No Sample)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	17. ระดับการส่องสว่างของแสง (≥ 2.5 ไม่นเกิน 3.0)	<input type="checkbox"/>	<input type="checkbox"/>	
Automatic titrator					
<input type="checkbox"/>	<input type="checkbox"/>	18. สภาพ Piston Burettes	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	19. Function Rinsing and Dosing	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	<input type="checkbox"/>	<input type="checkbox"/>	

ข้อแนะนำ:

Mr.Nattapat Rungruang

Service Engineer

Unit: Bangkok m/s/call only
DKSH Technology Limited
250 Sukhumvit Road, Bangkok, Phraechin, Bangkok 10260
Phone: +66 269 7100 Email: info@dksh.com Website: www.dksh.com/calibration-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-R31-08: 29 Jul 2022



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250


TEL: 0-2719-3080 FAX: 0-2719-9484

Cert.No.: 22TW178

Page: 1 of 2

Certificate of Testing

Equipment : DO Meter
Manufacturer : YSI
Model : 5100
Serial No. : 15L103204
ID No. : BKK_EN0205
Received Date : 02 August 2022
Test Date : 03 August 2022
Reference : 2208-0080DSC-1
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwang Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In-house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : Watalek Sirirhean
Approved by : Malee Butkjesa
Approved Signatory
Issue Date : 4 August 2022



Cert.No.: 22TW178

Page: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	21MM430	21 Sep 2022

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 17A100064

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.06	8.07	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization. It may concern intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory.

-000-

Malee

a 1119718

0293758



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES
3344 PATTANAKARN ROAD SOI 16, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-1000-27 FAX. 0-2719-6188



Cert. No.: 22LM107
Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter with Sensor
Manufacturer : VSI
Model : 5100
Serial No. : 15L103204
ID No. : BKK_EN0205
Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Location : TPA On Site Calibration Laboratory
Received Order : 2 August 2022
Calibrated Date : 4 August 2022
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V
Calibrated by : Man Pattanapongpalboon

Approved by :
Approved Signatory

() Pornthippa Tameyakul
() Malee Butkrua
() Suwit Imjai

Issue Date : 9 August 2022

The Uncertainties are for a confidence probability of approximately 95%.

This certificate may not be reproduced after date of full scope with the prior written approval of the head of Corporate Services. Equipment Calibration and Testing Services.

A 0044131



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2208-0060DSC-2
Procedure Used :-

Cert. No.: 22LM107
Page.: 2 of 2

Calibration was conducted using in-house calibration procedure CP-0101 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Digital Thermometer	1502A	A52847	2111144	20 Oct 2022
2) This certificate is valid only to the item calibrated on date and place of calibration.				
3) This certification is traceable to the International System of Unit.				

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 18C100772

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
20.00	60	20.002	19.93	-0.072	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

a 1120698



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T. Banpa, A. Kaengkhoh, Saraburi 18110, Thailand.
Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100
Bangkok Tel : +668 9205 6851, +668 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.com




Certificate No. T231342

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Incubator)
Manufacturer : MEMMERT
Model : ICP 750
Serial No. : F818.0033
Customer Code : BKK_EN0272
ID No. : T8041A4
Customer : ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250
Customer Location : Wet Chemistry Lab 2
Date of Receipt : 3 July 2023
Calibrated By : Sujjar Naknakred (Site Calibration Manager)
Approved By : / Boonchai Suriyawong (Assistant Calibration Manager)
Date of Issue : 11 JUL 2023



The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L14118/31-08-64



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T. Banpa, A. Kaengkhoh, Saraburi 18110, Thailand.



Certificate No. T231342

Page 2 of 4

Calibration Report

Equipment : Chamber (Incubator)
Date of Calibration : 5-6 July 2023 (Finished Time 4:30 PM)
Environment : Temperature 26.9-30.3 °C
Line Voltage 221.7-225.5 V

Condition of this results of test. :

1. This instrument was calibrated by insert 12 standard resistance thermometer into its chamber and test according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986.)
All data show below were final values and the initial data may be obtained upon request.

The temperature scale used was based on ITS - 90.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	27-(CH1)-10	T230543	10 April 2024
RTD	100 ohm	28-(CH1)-10	T230543	10 April 2024
DATA LOGGER	34970A	T149	T230543	10 April 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 9244.)

4. Condition of calibrated item : good

UUC Description :

Time Constant 6 Hour 35 Minute At 20 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Result of test :

() without adjustment (X) after adjustment


Approved By:

FM-L15117/15-05-63

Certificate No T231342

Calibration Report

Page 3 of 4

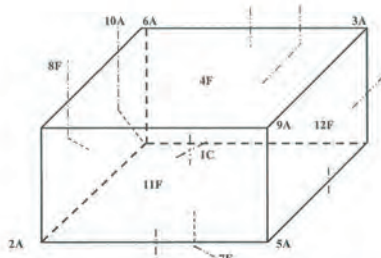

C = Centre, F = Centre of Face, A = Corner, E = Centre of Edge

1C = 27-CH1	11F = 28-CH1
2A = 27-CH2	12F = 28-CH2
3A = 27-CH3	
4F = 27-CH4	
5A = 27-CH5	
6A = 27-CH6	
7F = 27-CH7	
8F = 27-CH8	
9A = 27-CH9	
10A = 27-CH10	

Approved By:

FM-L13 11/7/15-05-63

Certificate No. T231342

Calibration Report

Page 4 of 4

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)									
	27-CH1	27-CH2	27-CH3	27-CH4	27-CH5	27-CH6	27-CH7	27-CH8	27-CH9	27-CH10
20.0	19.82	19.80	20.32	19.78	19.77	19.65	20.11	19.69	19.78	20.18
	28-CH1	28-CH2								
	20.02	19.81								

Chamber (Incubator)		Temperature Distribution					
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor k
	Min, Max	Average					
20.0	19.9, 20.1	20.0	19.98	0.06	0.61	0.38	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 %.

Approved By:


FM-L13 11/7/15-05-63

Certificate No. T230760

Page 1 of 5

Certificate of Calibration

Equipment : HOT BLOCK
Manufacturer : Environmental Express
Model : B3000-240
Serial No. : 2017CODW116
Customer Code : BKK_EN0222
ID No. : T6769A4
Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250
Customer Location : Wet Chemistry Lab2
Date of Receipt : 21 April 2023
Calibrated By : Watchararak Puttarat (Technician)
Approved By : / Sujjar Naknakred (Site Calibration Manager)
Date of Issue : 12 MAY 2023



The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L12 10/30/05-57

Certificate No. T230760

Calibration Report

Page 2 of 5

Equipment : HOT BLOCK
Date of Calibration : 25 April 2023
Environment : Temperature : 22.9-24.4 °C
Line Voltage : 222.7-227.8 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 20 standard thermocouples type T into its chamber, the other one standard thermocouples type T use for ambient temperature measurement. The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986). All data show below were final values and the initial data from customer request. The temperature scale used was based on ITS - 90.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	IN121-IN130	T222122	5 October 2023
TC	TYPE T	IN131-IN140	T222122	5 October 2023
DATA LOGGER	34970A	T150	T222122	5 October 2023

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244).

4. Condition of calibrated item : good

Equipment Description :

Time Constant : 1 Hour 32 Minute At 150 °C
Fresh Air Damper : ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

(X) without adjustment

() after adjustment

Approved By:

FM-L13 10/30/05-57

Calibration Report



Row	Hole							
R7	H49	H50	H51	H52	H53	H54	H55	H56
R6	H41	H42	H43	H44	H45	H46	H47	H48
R5	H33	H34	H35	H36	H37	H38	H39	H40
R4	H25	H26	H27	H28	H29	H30	H31	H32
R3	H17	H18	H19	H20	H21	H22	H23	H24
R2	H9	H10	H11	H12	H13	H14	H15	H16
R1	H1	H2	H3	H4	H5	H6	H7	H8

II: STANDARD THERMOCOUPLE TYPE T

H1 = TN121	H9 = TN129	H17 = TN137	H25 = TN125	H33 = TN133	H41 = TN121	H49 = TN129
H2 = TN122	H10 = TN130	H18 = TN138	H26 = TN126	H34 = TN134	H42 = TN122	H50 = TN130
H3 = TN123	H11 = TN131	H19 = TN139	H27 = TN127	H35 = TN135	H43 = TN123	H51 = TN131
H4 = TN124	H12 = TN132	H20 = TN140	H28 = TN128	H36 = TN136	H44 = TN124	H52 = TN132
H5 = TN125	H13 = TN133	H21 = TN121	H29 = TN129	H37 = TN137	H45 = TN125	H53 = TN133
H6 = TN126	H14 = TN134	H22 = TN122	H30 = TN130	H38 = TN138	H46 = TN126	H54 = TN134
H7 = TN127	H15 = TN135	H23 = TN123	H31 = TN131	H39 = TN139	H47 = TN127	H55 = TN135
H8 = TN128	H16 = TN136	H24 = TN124	H32 = TN132	H40 = TN140	H48 = TN128	H56 = TN136

Approved By.

FM-L11 108/30-05-57

Calibration Report

Measurement Results

		Average Standard Reading at each position (°C)											
Calibration Point		TN121	TN122	TN123	TN124	TN125	TN126	TN127	TN128	TN129	TN130		
Point	Setting	Max	149.31	149.49	149.73	148.49	149.26	149.51	149.42	148.86	148.78	149.19	
	Min	149.14	149.21	149.54	148.36	149.08	149.65	149.22	148.65	149.07	149.07		
	Average	149.23	149.40	149.64	148.43	149.16	149.73	149.33	148.76	148.71	149.13		
Calibration Point		TN131	TN132	TN133	TN134	TN135	TN136	TN137	TN138	TN139	TN140		
	Max	149.90	150.18	150.18	149.16	148.89	149.72	149.28	149.50	150.01	149.32		
	Min	149.78	150.06	149.69	149.03	148.76	149.49	149.12	149.37	149.90	149.23		
	Average	149.84	150.12	149.76	148.99	148.81	149.62	149.19	149.43	149.95	149.27		
Calibration Point		TN121	TN122	TN123	TN124	TN125	TN136	TN127	TN128	TN129	TN130		
	Max	149.88	149.14	149.20	150.02	148.75	149.57	149.21	149.18	150.13	148.91		
	Min	149.67	148.94	148.98	149.53	148.58	149.43	149.06	149.01	149.91	148.72		
	Average	149.78	149.05	149.11	149.94	148.67	149.51	149.13	149.10	150.01	148.83		
Calibration Point		TN131	TN132	TN133	TN134	TN135	TN136	TN137	TN138	TN139	TN140		
	Max	149.42	149.52	149.13	148.94	148.84	150.16	149.42	149.54	149.66	150.08		
	Min	149.27	149.36	148.99	148.81	148.70	149.99	149.27	149.39	149.52	149.97		
	Average	149.36	149.45	149.06	148.88	148.76	150.08	149.36	149.48	149.60	150.03		
Calibration Point		TN121	TN122	TN123	TN124	TN125	TN126	TN127	TN128	TN129	TN130		
	Max	149.21	149.16	149.50	148.68	148.58	149.81	149.06	150.40	148.46	149.24		
	Min	149.03	148.93	149.27	148.48	148.42	149.62	148.78	150.26	148.14	149.04		
	Average	149.12	149.04	149.39	148.57	148.51	149.72	148.93	150.33	148.29	149.14		
Calibration Point		TN131	TN132	TN133	TN134	TN135	TN136						
	Max	148.79	148.23	149.03	149.09	148.46	149.25						
	Min	148.49	147.98	148.88	148.54	148.29	149.12						
	Average	148.61	148.06	148.94	149.02	148.35	149.19						

Approved By.

FM-L11 108/30-05-57

Calibration Report

Measurement Results

HOT BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (±°C)	Uncertainty (±°C)
	Min, Max	Average		
150.0	150, 150.1	150.0	0.20	0.82

The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95 %.

Approved By.

FM-L11 108/30-05-57

Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No. BSCC-UV-367/23
Equipment UV/Vis Spectrophotometer
Model UV-1800
Manufacturer Shimadzu
Serial No. A11454908533CD
ID No. BKK_EN0018
Date of receipt 15 September 2023
Date of calibration 15 September 2023
Date of issue 22 September 2023

REVIEW BY Sirak P.
APPROVED BY KLAL
NEXT CAL DATE 19/9/2024

Customer name ALS Laboratory Group (Thailand) Co., Ltd.
Address 104 Soi Phattananan 40, Phattananan Road, Phattananan, Suan Luang, Bangkok 10250

Temperature (23.4 - 24.7) °C (On site)
Humidity (55.5 - 61.2) %RH (On site)

Equipment condition Good Operation

Calibration Location Organic Prep

Calibration Procedure In-house method WI-UV-702-01 based on ASTM E275-01

Traceability Wavelength Accuracy is traceable to certificate No. 95917 and 95918
Photometric Accuracy is traceable to certificate No. 95937 and 95924
Stray Light is traceable to certificate No. 95908
The above certificate are traceable to SI unit through NIST Scientific Ltd.
(UKAS accredited calibration laboratory NO. 0659)

Calibrated by Mr.Wanchana Janloey

Approved by

Mr.Kanchit Choothep
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

Certificate of Calibration

Certificate No. BSCC-UV-367/23

Number of Page(s) 2 of 3

Calibration Results:

1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
241.70	241.67	-0.03	0.18
334.02	334.03	0.01	0.18
418.53	418.59	0.06	0.18
572.99	573.14	0.15	0.18
879.41	879.21	-0.20	0.18

2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000	0.0000	0.0000	0.0075
	0.7467	0.7460	-0.0007	0.0075
257	0.0000	0.0000	0.0000	0.0075
	0.8662	0.8646	-0.0016	0.0075
313	0.0000	0.0000	0.0000	0.0075
	0.2904	0.2908	0.0004	0.0075
350	0.0000	0.0001	0.0001	0.0075
	0.6429	0.6415	-0.0014	0.0075

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate. Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced, except in full, without written approval of the Bara Scientific Co., Ltd.

FM-UV-708-02 Rev.01 (23/01/63)

Certificate of Calibration

Certificate No. BSCC-UV-367/23

Number of Page(s) 3 of 3

Calibration Results:

3.Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5783	0.5783	0.0010	0.0042
	0.7628	0.7624	-0.0004	0.0042
	1.0206	1.0216	0.0010	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5621	0.5625	0.0004	0.0042
	0.7455	0.7452	-0.0003	0.0042
	0.9985	0.9989	0.0004	0.0042
460.0	0.0000	0.0000	0.0000	0.0042
	0.5227	0.5229	0.0002	0.0042
	0.6880	0.6873	-0.0007	0.0042
	0.9487	0.9486	-0.0001	0.0042
546.1	0.0000	0.0000	0.0000	0.0042
	0.5207	0.5211	0.0004	0.0042
	0.6973	0.6960	-0.0013	0.0042
	0.9959	0.9944	-0.0015	0.0042
590.0	0.0000	0.0000	0.0000	0.0042
	0.5544	0.5538	-0.0006	0.0042
	0.7253	0.7236	-0.0017	0.0042
	1.0942	1.0925	-0.0017	0.0042
635.0	0.0000	0.0000	0.0000	0.0042
	0.5616	0.5612	-0.0004	0.0042
	0.6927	0.6909	-0.0018	0.0042
	1.0881	1.0866	-0.0015	0.0042

*CNR = Customer not request

4.Stray Light*

Standard cut-off wavelength (nm)	Wavelength (nm)	Transmission (%)	Absorbance (A)
200.95±0.11nm	200.55	0.9770	2.0104

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A
*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

End of Certificate

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate. Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced, except in full, without written approval of the Bara Scientific Co., Ltd.

FM-UV-708-02 Rev.01 (23/01/63)

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoh, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com

Certificate No. T231303

Page 1 of 3

Certificate of Calibration

Equipment : Liquid Bath (Water)

Manufacturer : MEMMERT

Model : WNB29

Serial No. : L611.0135

Customer Code : BKK_EN0148

ID No. : T6455A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : ORGANIC PREPARATION LAB

Date of Receipt : 27 June 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By : Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 11 JUL 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L1418/31-08-64

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoh, Saraburi 18110, Thailand.

Certificate No. T231303

Page 2 of 3

Calibration Report

Equipment : Liquid Bath (Water)

Date of Calibration : 4 July 2023

Environment : Temperature : 22.2-22.5 °C

Line Voltage : 221.6-224.8 V

Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 (based on ASTM E715-80 (Reapproved 2001)).

All data show below were final values and the initial data from customer request , The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M18 (CH1,CH6-CH7,CH9-CH10)	T230545	10 April 2024
DATA LOGGER	34970A	T149	T230545	10 April 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TIS-TIS 17025 CALIBRATION 0244)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 3 Hour 45 Minute At 60 °C

5. Adjustment :

(X) without adjustment () after adjustment


Approved By: Boonchai Suriyawong

FM-L15 117/15-05-63

Certificate No. T231303

Page 3 of 3

Calibration Report

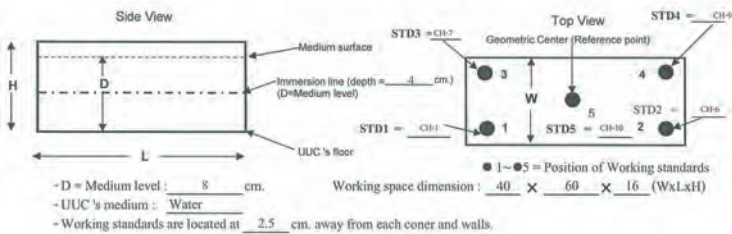

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)				
	CH-1	CH-6	CH-7	CH-9	CH-10
60	60.03	60.06	60.24	60.11	60.18
85	84.79	84.83	85.42	85.05	85.20
95	93.71	93.83	94.62	94.15	94.42

Liquid Bath (Water)		Temperature Distribution					
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (±°C)	Uncertainty (±°C)	Coverage Factor k
	Min, Max	Average					
61.0	60.9, 61.1	61.0	60.12	0.13	0.19	0.29	2.04
86.0	85.8, 86.2	86.0	85.06	0.19	0.47	0.44	2.17
95.0	94.6, 95	94.9	94.15	0.32	0.65	0.55	2.13

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 %.

Approved By: *[Signature]*

FM-L13 117015-05-63

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
53/44 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No.: 23T1512
Page: 1 of 2

Equipment: Digital Thermometer With Sensor

Manufacturer: Testo

Model: 106

Serial No.: 83637871/0122

ID No.: BKK_LG0055

Condition As-Received: Used Item

Received Date: 21 August 2023

Calibration Date: 24 August 2023 to 30 August 2023

Reference: 2308-0616D9C

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khel Suan Luang,
Bangkok 10250 ThailandProcedure used: Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.
The temperature scale used was based on ITS-90.

Condition of this result of calibration


1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Digital Thermometer	1529	A7A809	2211274	17 Oct 2023
2) Industrial Platinum Resistance Thermometer	5627	824304	2211274	17 Oct 2023

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by: Puttichai Manop
Issue Date: 31 August 2023

Approved Signatory:

[] Phalinee Prabpaipal
[] Chatchawan Khunpluek
[x] Wanlop Larpiem

B 0323062

Cert. No.: 23T1512
Page: 2 of 2

Result of Calibration:-

Without Adjustment

Function: Temperature measurement

Dimension of probe: Diameter 3 mm., Length 55 mm. Sheath material: Stainless Steel

Immersion Depth (mm.)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
50	25.0052	25.0	-0.0052	0.12
50	30.0051	30.0	-0.0051	0.12
50	35.0063	35.1	0.0937	0.12
50	40.0034	40.1	0.0966	0.12
50	45.0009	45.0	-0.0009	0.12

UUC*: Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

-000-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
53/44 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No.: 23T1511
Page: 1 of 2

Equipment: Digital Thermometer With Sensor

Manufacturer: Testo

Model: 106

Serial No.: 83637906/0122

ID No.: BKK_LG0054

Condition As-Received: Used Item

Received Date: 21 August 2023

Calibration Date: 24 August 2023 to 30 August 2023

Reference: 2308-0616D9C

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khel Suan Luang,
Bangkok 10250 ThailandProcedure used: Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Digital Thermometer	1529	A7A809	2211274	17 Oct 2023
2) Industrial Platinum Resistance Thermometer	5627	824304	2211274	17 Oct 2023

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by: Puttichai Manop
Issue Date: 31 August 2023

Approved Signatory:

[] Phalinee Prabpaipal
[] Chatchawan Khunpluek
[x] Wanlop Larpiem

B 0323061

a 1178225



Cert. No.: 23T1511
Page.: 2 of 2

Result of Calibration:-

Function: Temperature measurement
Without Adjustment
Dimension of probe : Diameter 3 mm., Length 55 mm. Sheath material : Stainless Steel

Immersion Depth (mm.)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
50	25.0010	25.0	-0.0010	0.12
50	30.0071	30.0	-0.0071	0.12
50	35.0016	35.1	0.0984	0.12
50	39.9960	40.1	0.1040	0.12
50	45.0012	45.1	0.0988	0.12

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

-o0o-

a 1178226

Agilent Technologies

Agilent Technologies (Thailand) Limited
U CHU LIAO BLDG. 22/F UNIT A.D
868 RAMA 4 ROAD, SILOM, BANGRAK
Bangkok 10500 Thailand

Tel: +662 637 6363
Fax: +662 637 6334
Email: ccc-smt@agilent.com
Website: www.agilent.com/chem

Customer Contact:

ALS Laboratory Group (Thailand) Co Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan
TAX ID : 0105540004859
bounced-mchom.chanattagarn@alsglobal.com
227158769519

Invoice To:

ALS Laboratory Group (Thailand) Co Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

SERVICE REPORT

Customer Purchase Order Number:	Customer Number: 79371013
Service Request:	Service Request Date:
Service Order: 6006068207	Service Confirmation: 6904837529

REVIEW BY Archalee K.
APPROVED BY Siamw N
NEXT CAL DATE 06/10/2024

Delivery Site:

ALS Laboratory Group (Thailand) Co Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

Location:

Room
Bldg
Lab
Dept

Direct Inquiries to:

Contact Name: Customer Contact Center
Contact E-mail: ccc-smt@agilent.com
Contact Telephone: +662 637 6363
Contact Fax: +662 632 4334

products | applications | software | services

Learn more about Agilent's Special Offers, Products, Services and our full range of laboratory productivity solutions optimized for your applications and workflows. Visit us at www.agilent.com/chem

Agilent Technologies (Thailand) Limited, Head Office
U Chu Liang Bldg. 22/F Unit A.D
868 Rama 4 Road, Silom, Bangkok,
Bangkok 10500 Thailand
Tax ID : 0105540004859

Original N.A. Bangkok Branch
299 Interchange 21 Building, Sukhumburi Road, Klongtoey New Sub-district, Wattana District, Bangkok 10110 Thailand
Acc. No. 012-4452-007,
THB-Krungsri Thai Bank PCL
Siam Square Bldg. 416/1-2 Rama 1 Rd, Pathumwan, BKK 10330 Thailand

Page 1 of 3

Service Confirmation Number: 6904837529
Service Confirmation Date: 06.04.2023

Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IM-7900	ICPMS 7900 System			
G8410A	SPS 4 Autosampler	AU15430722	ICP MS 7900	SYS-IM-7900
G8411A	ISIS 3 for Agilent 7850/7900/8900	JP15510227	ICP MS 7900	SYS-IM-7900
G3292A	PSC 6100T Chiller	2U15A1948	ICP MS 7900	SYS-IM-7900
G8403A	Agilent 7900 ICP-MS	JP15471169	ICP MS 7900	SYS-IM-7900

Service Items:

Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EQJ	Enterprise Operational Qualification	1.00	Agreement Entitlement - 100 % covered	06.04.2023	06.04.2023
1010	5185-5850	ICP-MS Checkout Solutions	1.00	Agreement Entitlement - 100 % covered		

Additional Information:

Service Information:

Problem Description: WU-S-00-ICP MS 7900-5001143313		
Service Provided: Test OQ control of instrument ICPMS = BKK_EL0043. After done all instrument test all Pass.		
Service Overview Code: Reason Code: Scheduled Service Diagnosis Code: Scheduled Service Resolution Code: Scheduled Service		
Reported Hours: 6.0	Travel Hours: 1.0	
Customer Field Service Representative Name: Panthep Kurasathain	Customer Field Service Representative Signature: 	Date: 06 Apr 2023
Customer Name: Archalee Khamjan	Customer Signature: 	Date: 06 Apr 2023
Additional Comments:		



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 1 of 6

Certificate of Calibration

Equipment : HEATING BLOCK
Manufacturer : Environmental Express
Model : SC 196
Serial No. : 6974CECW3285
Customer Code : BKK_EL0054
ID No. : T5306A3
Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250
Customer Location : Acid Digestion Lab
Date of Receipt : 13 September 2023
Calibrated By : Saneek Musikawan (Site Calibration Manager)
Approved By : / Sujjar Naknakred (Site Calibration Manager)
Date of Issue : 26 SEP 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L12 109/30-05-57



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 2 of 6

Calibration Report

Equipment : HEATING BLOCK
Date of Calibration : 22 September 2023
Environment : Temperature : 21.8-23.1 °C
Line Voltage : 221.6-226.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

- This equipment was calibrated by insert 20 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
- Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN21-TN30	T230014	17 January 2024
TC	TYPE T	TN31-TN40	T230014	17 January 2024
DATA LOGGER	34970A	T151	T230014	17 January 2024
- This certificate is traceable to :
National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244)
- Condition of calibrated item : good
Equipment Description :
Time Constant : 2 Hour 20 Minute At 95 °C
Fresh Air Damper : ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available
- Adjustment :
() without adjustment (X) after adjustment

Approved By.

FM-L13 108/30-05-57



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110


Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 3 of 6

Calibration Report

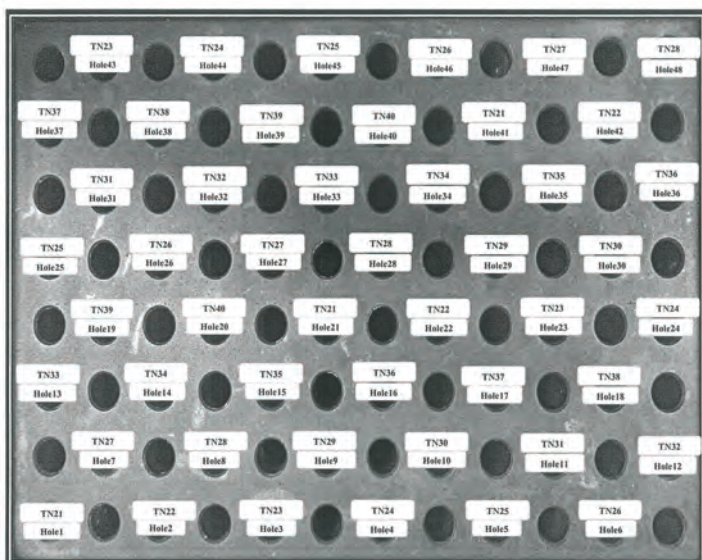

FRONT CONTROL

Approved By.

FM-L13 108/30-05-57



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 4 of 6

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (° C)					
R1 Hole1-Hole6		TN21	TN22	TN23	TN24	TN25	TN26
CAL POINT 95	Max	95.01	94.41	95.20	95.41	94.51	95.17
	Min	94.57	93.95	94.75	94.92	94.00	94.72
	Average	94.79	94.18	94.98	95.17	94.26	94.95
R2 Hole7-Hole12		TN27	TN28	TN29	TN30	TN31	TN32
	Max	95.36	95.43	95.19	95.16	95.35	94.97
	Min	94.94	94.95	94.72	94.71	94.90	94.57
	Average	95.15	95.19	94.96	94.94	95.13	94.77
R3 Hole13-Hole18		TN33	TN34	TN35	TN36	TN37	TN38
	Max	95.37	95.50	95.22	95.21	95.33	95.31
	Min	94.99	95.09	94.78	94.82	94.88	94.96
	Average	95.18	95.30	95.00	95.02	95.11	95.13
R4 Hole19-Hole24		TN39	TN40	TN21	TN22	TN23	TN24
	Max	95.59	94.42	94.52	94.24	94.63	94.67
	Min	95.21	94.06	94.13	93.88	94.28	94.27
	Average	95.40	94.24	94.33	94.06	94.45	94.47
R5 Hole25-Hole30		TN25	TN26	TN27	TN28	TN29	TN30
	Max	95.19	95.38	92.93	95.30	95.14	95.03
	Min	94.83	95.03	92.56	94.95	94.79	94.70
	Average	95.01	95.20	92.75	95.12	94.96	94.87
R6 Hole31-Hole36		TN31	TN32	TN33	TN34	TN35	TN36
	Max	94.63	94.90	94.77	94.31	94.24	93.87
	Min	94.24	94.35	94.44	93.98	93.92	93.56
	Average	94.43	94.72	94.60	94.14	94.08	93.71
R7 Hole37-Hole42		TN37	TN38	TN39	TN40	TN21	TN22
	Max	94.30	94.44	94.04	93.81	94.89	95.35
	Min	93.95	94.05	93.67	93.48	94.39	94.90
	Average	94.13	94.24	93.86	93.65	94.64	95.12
R8 Hole43-Hole48		TN23	TN24	TN25	TN26	TN27	TN28
	Max	95.99	95.63	95.28	95.29	95.45	94.87
	Min	95.57	95.15	94.82	94.84	94.99	94.48
	Average	95.78	95.39	95.05	95.07	95.22	94.68

Approved By.

FM-L13 108/30-05-57



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No T231676

Page 5 of 6

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		TN21	TN22	TN23	TN24	TN25	TN26
CAL POINT	Max	105.23	104.32	105.43	105.25	104.44	105.27
	Min	104.94	103.95	105.15	105.04	104.11	104.96
	Average	105.09	104.13	105.29	105.15	104.28	105.12
R2 Hole7-Hole12		TN27	TN28	TN29	TN30	TN31	TN32
	Max	105.30	105.12	105.18	105.22	105.12	105.16
	Min	105.11	104.92	104.96	105.00	104.92	104.97
	Average	105.20	105.02	105.07	105.11	105.02	105.06
R3 Hole13-Hole18		TN33	TN34	TN35	TN36	TN37	TN38
	Max	105.37	105.63	105.02	104.80	104.69	105.19
	Min	105.17	105.37	104.75	104.59	104.50	105.00
	Average	105.27	105.50	104.88	104.69	104.60	105.09
R4 Hole19-Hole24		TN39	TN40	TN21	TN22	TN23	TN24
	Max	105.31	104.43	106.41	104.71	105.63	105.82
	Min	105.08	104.22	106.15	104.41	105.37	105.56
	Average	105.19	104.33	106.28	104.56	105.50	105.69
R5 Hole25-Hole30		TN25	TN26	TN27	TN28	TN29	TN30
	Max	104.95	106.26	103.34	105.78	105.59	105.87
	Min	104.67	105.96	103.08	105.56	105.36	105.68
	Average	104.81	106.11	103.21	105.67	105.48	105.77
R6 Hole31-Hole36		TN31	TN32	TN33	TN34	TN35	TN36
	Max	104.75	104.86	104.80	105.20	104.50	104.39
	Min	104.54	104.63	104.59	105.00	104.32	104.18
	Average	104.65	104.75	104.69	105.10	104.41	104.28
R7 Hole37-Hole42		TN37	TN38	TN39	TN40	TN21	TN22
	Max	104.30	104.90	104.85	104.65	104.88	104.85
	Min	104.09	104.72	104.66	104.49	104.63	104.52
	Average	104.19	104.81	104.75	104.57	104.76	104.68
R8 Hole43-Hole48		TN23	TN24	TN25	TN26	TN27	TN28
	Max	105.71	105.85	105.39	105.61	105.42	105.19
	Min	105.45	105.61	105.14	105.27	105.18	104.94
	Average	105.58	105.73	105.27	105.44	105.30	105.07

Approved By: _____

FM-L13 108/30-05-57



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 6 of 6

Calibration Report

Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (±°C)	Uncertainty (±°C)
	Min, Max	Average		
100.0	100.3, 100.5	100.4	0.26	0.81
107.0	107.0, 107.1	107.1	0.19	0.78

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 %.

Approved By: _____

FM-L13 108/30-05-57

BKK_EL0037



Agilent Technologies (Thailand) Limited
U CHU LIANG Bldg, 22/F Unit A.D.
968 Rama 4 Road, Silom, Bangkok
Bangkok 10500 Thailand

Tel: +662 637 6383
Fax: +662 632 4334
Email: ccc-sm@agilent.com
Website: www.agilent.com/chem

Service Confirmation Number: 8504800024
Service Confirmation Date: 20.03.2023

Customer Contact:

ALS Laboratory Group (Thailand) Co.
Ltd.
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khuang Phatthanakan Khet Suan
TAX ID : 0105540004859
Chanattagarn.lmchom@alsglobal.com
27603068

Invoice To:

ALS Laboratory Group (Thailand) Co.
Ltd.
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khuang Phatthanakan Khet Suan


Delivery Site:

ALS Laboratory Group (Thailand) Co.
Ltd.
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khuang Phatthanakan Khet Suan

Location:
Room
Bldg
Lab
Dept

SERVICE REPORT

Customer Purchase Order Number:	Customer Number: 70371013
Service Request:	Service Request Date:
Service Order: 6906033911	Service Confirmation: 6904800024



Direct Inquiries to:

Contact Name: Customer Contact Center
Contact E-mail: ccc-sm@agilent.com
Contact Telephone: +662 637 6383
Contact Fax: +662 632 4334

Chitbank N.A. Bangkok Branch
399 Interchange 21 Building, Sukhumvit Road, Klongtoey Nua
Sub-district, Wattana District, Bangkok 10110 Thailand
Acc. No: 012-4452-007
THB-Krung Thai Bank PCL
Siem Square Bldg. A15/1-2 Rama 1 Rd., Pathumwan, BKK 10330
Thailand

Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IO-5100	ICP-DES 5100/5110 System			
G8010A	Agilent 5100 SVDV ICP-DES Spectrometer	MY160100EE	ICP DES 5100	SYS-IO-5100
G8410A	SPS 4 Autosampler	AU15440764	ICP DES 5100	SYS-IO-5100

Service Items:

Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EQD	Enterprise Operational Qualification	1.00	Agreement Entitlement - 100 % covered	20.03.2023	20.03.2023

Additional Information:

gas | fluids | applications | software | services

Learn more about Agilent's Special Offers, Products, Services and our full range of laboratory productivity solutions optimized for your applications and workflows. Visit us at www.agilent.com/chem

Agilent Technologies (Thailand) Limited, Head Office
U Chu Liang Bldg, 22/F Unit A.D.
968 Rama 4 Road, Silom, Bangkok
Bangkok 10500 Thailand
Tax ID : 010554298818

Service Confirmation Number: 6004800024
Service Confirmation Date: 28.03.2023

REVIEW BY	<u>Oranon T.</u>
APPROVED BY	<u>Saatchi N.</u>
NEXT CAL. DATE	<u>24.10.2024</u>

Service Information:

Problem Description: WU-S-OQ-ID-5109-5001143313		
Service Provided: Complete DOHW 5100ICPOES Equipment ID: BKK_EL0027, all tests passed		
Service Overview Code: Reason Code: Scheduled Service Diagnosis Code: Scheduled Service Resolution Code: Scheduled Service		
Reported Hours: 4.0	Travel Hours: 2.0	
Customer Field Service Representative Name: Kanyakorn Sukpharajaree	Customer Field Service Representative Signature: <u>Kanyakorn</u>	Date: 28 Mar 2023
Customer Name: Thitima Boongeng	Customer Signature: <u>Thitima B.</u>	Date: 28 Mar 2023
Additional Comments:		

Page 2 of 3

Maintenance Protocol

Atomic Fluorescence Spectrometer
mercur DUO /
mercur DUO plusSerial-No.: K170A0143 Customer-No.: _____
Date: 24 May 2023 Carried out by: Srichai Fak-onMaintenance with following Operational Qualification (OQ)
(requires a separate OQ protocol) ☐

Company	บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด
User	
Department	ห้องแล็บปฏิบัติการ
Street	104 ซอย 40 ถนนพัฒนาการ แขวงสวนหลวง เขตสวนหลวง
Zip Code, City	กรุงเทพมหานคร 10250
Country	ประเทศไทย
Phone	
Fax	
E-mail	

Maintenance works basic unit

tightness visual check inside the Mercur ☒
 visual check if gold-traps are broken ☒
 visual check if spectrometer is contaminated ☒
 visual check of the fluorescence cell ☒
 visual check of the absorption cell, incl. window ☒
 reactor cleaning ☒
 check pump-hose, if necessary change it ☒
 check swivel drive (SEV) ☒
 check drying-hose, output gas-liquid-separator ☒
 test Bubble-Sensor ☒
 check gas flows ☒
 check volume flows, reagents ☒
 recording stray light values ☒
 measurement with 30 ng/l ☒

Maintenance works Autosampler

Serial No.: 701 739

lubricate the dosing-winding (Teflon-grease-spray) ☒
 clean the dosing cylinder, if necessary exchange it ☒
 lubricate the winding system of the height drive with some drops of oil ☒
 check the toothed belt ☒
 check the position of the mechanical stopper (height: 13mm) ☒
 check the pump rate of mixing pump (<14s AS52, typ.7s/<20s AS52S, typ.10s) ☒
 check the pump rate of washing cup ☒
 check the electrical hose connections for good contact ☒
 check the connectors of the magnetic valves ☒
 check the dosing hose for buckling, if necessary exchange it ☒

Device parameter	nominal value	actual value
visual check general tightness inside the Mercur	o.k.: <input checked="" type="checkbox"/>	changed: <input type="checkbox"/>
visual check Goldtraps	o.k.: <input checked="" type="checkbox"/>	changed: <input type="checkbox"/>
visual check spectrometer		
Fluorescence cell	o.k.: <input checked="" type="checkbox"/>	changed: <input type="checkbox"/>
Absorption cell, incl. window	o.k.: <input checked="" type="checkbox"/>	changed: <input type="checkbox"/>
lens	o.k.: <input checked="" type="checkbox"/>	changed: <input type="checkbox"/>
Swivel drive (SEV)	o.k.: <input checked="" type="checkbox"/>	changed: <input type="checkbox"/>
check pump hoses	o.k.: <input checked="" type="checkbox"/>	changed: <input type="checkbox"/>
check hoses and hose connectors	o.k.: <input checked="" type="checkbox"/>	changed: <input type="checkbox"/>
check and clean reactor	o.k.: <input checked="" type="checkbox"/>	changed: <input type="checkbox"/>
check drying hose output Gas-liquid-separator	o.k.: <input checked="" type="checkbox"/>	changed: <input type="checkbox"/>
check bubble-sensor	o.k.: <input checked="" type="checkbox"/>	not o.k.: <input type="checkbox"/>
Check gasflow		
Argon pressure valve 4	1.2 - 1.5 bar	1.5 bar
Valve 1	10 Nl/h or 0.166 NL/min	0.163 NL/min
Valve 2	50 Nl/h or 0.833 NL/min	0.403 NL/min
Valve 3	5 Nl/h or 0.083 NL/min	0.140 NL/min
Valve 4	10 Nl/h or 0.166 NL/min	0.108 NL/min
Check liquidflow		
Acid	2.5ml/min ± 1 ml	2.5 ml/min
Red.-agent	2.5ml/min ± 1 ml	2.5 ml/min
Sample	10ml/min ± 2 ml	10 ml/min
Adventitious light - values (V)	from file	
100	0	0
200	0	0
300	0	0
350	0	0
400	0	0
450	2	2
500	5	5
550	10	10
575	15	14
600	20	20

Device parameter	nominal value	actual value
Analytical parameters Fluorescence cell		
Conditions.: max.conc.: 10µg/L PMT-voltage: 360 V		
Blank-solution without enrichment / FBR 30 ng/L	Int > 0.0015 RSD < 3 %	Int. 0.00024 Int. 0.00172 RSD 0.45 %
Conditions.: max.conc.: 1.7µg/L PMT-voltage: 352 V		
Blank-solution with enrichment / FBR 30 ng/L	Int > 0.008 RSD < 3 %	Int. 0.00370 Int. 0.01060 RSD 2.38 %
Fok.- factor (Int ₂ / Int ₁)	> 3.5	6.16
Analytical parameters Absorption cell		
Blank-solution without enrichment / FBR 100 ng/L	Ext. > 0.0012 RSD < 5 %	Ext. 0.00093 Ext. 0.00449 RSD 2.58 %
Comments		

Sudchai Paksan
Signature TechnicianOrawan T.
Signature Customer

24 May 2023

Place, Date (DD/MM/YYYY)

24 May 2023

Place, Date (DD/MM/YYYY)

Service Report

Customer's address :	Customer's Ref. No.			
สำนักงานสาธารณสุขจังหวัดขอนแก่น				
PM code to maintenance instrument information				
Information				
E-mail :	Phone :	Fax :		
Job No. 2305282 PM	User :	Service Engineer : นสพ. นพ. นสพ.	Date : 24/5/2023	Page : 1/1
Instrument model Mercur	Serial No. K170A0143	Software Version No. 4.7.10.0		
<input type="checkbox"/> Repair (RE) <input checked="" type="checkbox"/> Maintenance (PM) <input type="checkbox"/> Installation (IN) <input type="checkbox"/> Warranty <input type="checkbox"/> Application (AP) <input type="checkbox"/> Site Prep (SP) <input type="checkbox"/> Visit (VI)				
Fault / Claim : - problem with maintenance PM No. 2305282 / (IN/2305-037)				
- problem PM Control Year 2023 (1 Time / Year 2023)				
Action taken : - Maintenance red Basic Unit				
- Check device parameter.				
- Check gas flow				
- Check liquid flow				
- Check Adventitious light - valves				
# Test run Analytical parameter Fluorescence cell				
Test run Analytical parameter Absorption cell				
Action Pending / Recommendation : - maintenance PM				
<input type="checkbox"/> Spare Part <input type="checkbox"/> Instrument Configuration :				
Item No.	Name	Quantity	Unit Price	
1.				
2.				
3.				
4.				
5.				
6.				
7.				
8.				
Hereby the undersigned confirm the time devoted, the work performed, the perfect function of the device and the receipt/delivery of the specified spare parts. *Traveled hours and kilometers can only be entered after the return of the service engineer.	Date / Signature of Customer	Date / Signature of Service Engineer	Work completed?	
	Orawan T.	นสพ. นพ. นสพ.	<input checked="" type="checkbox"/> Yes <input type="checkbox"/> No	

5/24/2023 12:46 Page 1/4

Mercur

Report file:	C:\WinAAS\TMP\2023\May\Pro_032		
Program version:	4.7.10.0	Printed on:	5/24/2023 12:46
Operator:	PSU_OTA	Recording started on:	5/24/2023 12:35 GMT+7.0
Laboratory:	ALS-BKK		
Code:	IL_Hg095_2023		
Remarks:			
Food, water			

Method parameters

Method	Without enrichment / FBR 30ng/L_PM24052023	Hg	
Created on	5/24/2023	Time	12:27
Program			
Parameters Mercur Technique: Hg fluorescence			
Line	253.7 nm		
Lamp type	Hg-LP		
Integr. mode	Peak height	Integr. time	30 s
PMT	360 V		
AZ time	5 s	Peak smoothing	8/5
Delay	0 s		
Working mode	w/o enrich.		
FBR technique	on	System cleaning	Acid
Pump speed	3	Wash time acid	10 s
Sample load time	10 s	Soaking time	20 s
Reaction time	10 s	Gas load time	5 NL/h
Waiting time AZ	5 s		
Delay	0 s		
Purge time1	28 s		
Purge time2	15 s	Gas wash time2	10 NL/h
Autosampler			
Autosampler	AS51S/F	Tray type	87/139
Working mode	continuous		
Dilution			

QC parameters

QC type	Conc. check	QC check samp. 2	---
QC check samp. 1	---	Conc.	---
Conc.	---	Error limit	---
Error limit	---	Reaction	flag + continue
Rep. measurement	off	QC std.2 no.	1(30.000 ng/L)
QC std.1 no.	1(30.000 ng/L)	QC std.2 limit	± 50.00%
QC std.1 limit	± 50.00%	Reaction	flag + continue
QC std. act.	flag + continue	QC Recal factor	Off
Expect. blank abs.	0.0100± 0.0100		
QC precision	off		

Calibration settings

Calib. meth	Standard calib.	Calibr. unit	ng/L
No. standards	1	Conversion fac.	1000000
Type of standards	---	Standard prep.	Premixed
		Blank correct.	---
		Recalib. std. no.	---
Output unit	µg/L	Conversion fac.	1000
Calib. stat.	Mean	Meas. cycles	3
		Blind cycles	1
Stock sol. 1	---	Stock sol. 2	---
Stock sol. 3	---	Stock sol. 4	---
Type of cal. curve	linear	Intercept	calculated
Weighted cal.	off	Grubbs stat.	off
Check of cal. curve	no outlier test		

Sample statistics

Stat. mode	Mean	Meas. cycles	2
Confid. level	95.4 %	Blind cycles	1
Grubbs stat.	---		

Calibration standards

No	Name	State	Pos	Conc./ ng/L	Ints	SD	RSD/%
1	Cal-Zero	(--)	79	0.000	H: 0.000249 A: 0.004274	0.000132 0.001698	53.13 39.72
2	Cal-Std1	(--)	80	30.000	H: 0.001720 A: 0.02172	0.000007 0.000023	0.459 0.107

Hg

Mercur

Calibration function 1


5/24/2023 12:44 Calibration (Peak height)

Ints=k1+k2*conc

k1=0.000249 k2=0.000049

Recal. factor: ---

Slope	0.00005 Ints/(ng/L)	R2-adjusted	1.0000
sc0	1.000000 ng/L		
Lower limit	0 ng/L	Upper limit	33.0 ng/L
Detection limit	---	Deter. limit	---

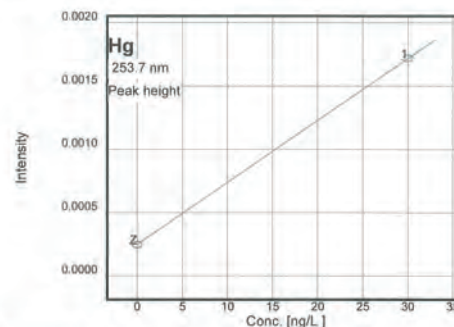


Measurements and events (sorted by time)

Hg	Without enrichment / FBR 30ng/L_PM 24052023					5/24/2023	12:36
ID	Conc.	Ints	BG	SD	RSD/%	Int. type	Time
Cal-Zero		0.000143				PkH	12:37
		0.000397					12:38
		0.000207					12:40
	0ng/L	0.000249		0.0001324	53.13		12:40
Cal-Std1		0.001720				PkH	12:42
		0.001712					12:43
		0.001728					12:44
	30.00ng/L	0.001720		0.000007897	0.459		12:44
Calibration	Calibration function: 01						12:44

Mercur

Peak plots

Hg

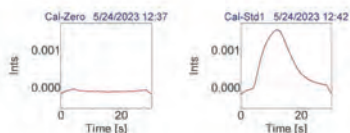

Mercur

Mercur

Report file:	C:\WinAAS\TMP\2023\May\Pro_033			
Program version:	4.7.10.0	Printed on:	5/24/2023	14:01
		Recording started on:	5/24/2023	13:37 GMT+7.0
Operator:	PSU,OTA			
Laboratory:	ALS-BKK			
Code:	II_Hg095_2023			

Remarks:

Food,water

Method parameters

Hg

Method	Enrichment / FER 30ng/L PM_24052023		
Created on	5/24/2023	Time	13:36
Program	---		

Parameters Mercur Technique: Hg fluorescence

Line	253.7 nm		
Lamp type	Hg-LP		
Integr. mode	Peak height	Integr. time	40 s
PMT	352 V		
AZ time	5 s	Peak smoothing	12/11
Delay	0 s		

Working mode	Enr. w/o reload.	System cleaning	Off
FBR technique	off	Wash time acid	10 s
Pump speed	3	Soaking time	20 s
Sample load time	10 s	Gas load time	10 NL/h
Reaction time	10 s		
Waiting time AZ	10 s	Gas AZ wait	10 NL/h
Purge time1	30 s		
Purge time2	15 s	Gas wash time2	5 NL/h
Purge time3	20 s		
Heat time coll.1	20 s	Cool. time coll.1	30 s

Mercur

QC parameters

QC type	Conc. check	QC check samp. 2	---
QC check samp. 1	---	Conc.	---
Conc.	---	Error limit	---
Error limit	---	Reaction	flag + continue
Rep. measurement	off	QC std.2 no.	1(30.000 ng/L)
QC std.1 no.	1(30.000 ng/L)	QC std.2 limit	± 50.00%
QC std.1 limit	± 50.00%	Reaction	flag + continue
QC std. act.	flag + continue	Reaction	flag + continue
Expect. blank abs.	0.0100± 0.0100	Reaction	flag + continue
QC precision	off	Reaction	off
		QC Recal. factor	Off

Calibration settings

Calib. meth	Standard calib.	Calibr. unit	ng/L
No. standards	1	Conversion fac.	1000000
Type of standards	---	Standard prep.	Premixed
		Blank correct.	---
		Recalib. std. no.	---
Output unit	µg/L	Conversion fac.	1000
Calib. stat.	Mean	Meas. cycles	3
		Blind cycles	1
Stock sol. 1	---	Stock sol. 2	---
Stock sol. 3	---	Stock sol. 4	---
Type of cal. curve	linear	Intercept	calculated
Weighted cal.	off	Grubbs stat.	off
Check of cal. curve	no outlier test		

Sample statistics

Stat. mode	off	Meas. cycles	1
Confid. level	95.4 %	Blind cycles	1
Grubbs stat.	---		

Calibration standards

No	Name	State	Pos	Conc./ ng/L	Ints	SD	RSD/%
1	Cal-Zero	(-)	##	0.000	H: 0.003700 A: 0.02531	0.000081 0.000153	2.192 0.607
2	Cal-Std1	(-)	##	30.000	H: 0.01060 A: 0.06689	0.000253 0.002766	2.386 4.136

Hg

Mercur

Calibration function 1


5/24/2023 14:00 Calibration (Peak height)

Ints=k1+k2*conc

k1=0.003700 k2=0.000230

Recal. factor: ---

Slope	0.00023 Ints/(ng/L)	R2-adjusted	1.0000
sc0	1.00000 ng/L		
Lower limit	0 ng/L	Upper limit	33.0 ng/L
Detection limit	---	Deter. limit	---

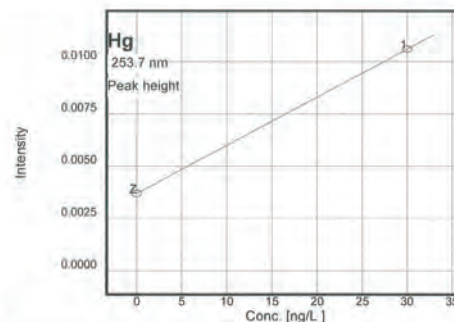


Measurements and events (sorted by time)

Hg	Enrichment / FER	30ng/L	PM_24052023	5/24/2023	13:37
ID	Conc.	Ints	BG	SD	RSD/%
Cal-Zero		0.003792			PkH
		0.003666			13:41
		0.003640			13:43
	0ng/L	0.003700		0.000081090	2.192
					13:44
Cal-Std1		0.008498			PkH
		0.008333			13:49
		0.008961			13:50
	30.00ng/L	0.008931		0.0005830	6.528
					13:52
Cal-Std1		0.01031			PkH
		0.01074			13:57
		0.01076			13:58
	30.00ng/L	0.01060		0.0002530	2.386
					14:00
Calibration	Calibration function: 01				14:00

Mercur

Peak plots

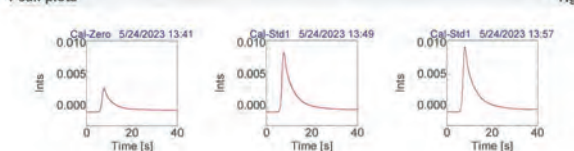

Hg

Mercur

Mercur

Report file:	C:\WinAAS\TMP\2023\May\Pro_034
Program version:	4.7.10.0
Printed on:	5/24/2023 14:33
Recording started on:	5/24/2023 14:19 GMT+7.0
Operator:	PSU,OTA
Laboratory:	ALS-BKK
Code:	IL_Hg095_2023

Remarks:

Food,water

Method parameters

Method	Without enrichment / Abs / FBR 100ng/L_PM 24052023
Created on	5/24/2023 Time 14:18
Program	---

Parameters Mercur Technique: Hg absorption

Line	253.7 nm		
Lamp type	Hg-LP		
Integr. mode	Peak height	Integr. time	55 s
PMT	225 V		
AZ time	5 s	Peak smoothing	2/5
Delay	8 s		

Working mode	w/o enrich.	System cleaning	Acid
FBR technique	on	Wash time acid	15 s
Pump speed	4	Soaking time	20 s
Sample load time	8 s	Gas load time	5 NL/h
Reaction time	12 s		
Waiting time AZ	15 s		
Delay	10 s		
Purge time1	50 s		
Purge time2	10 s	Gas wash time2	10 NL/h

Hg

Mercur

QC parameters

QC type	Conc. check	QC check samp. 2	---
QC check samp. 1	---	Conc.	---
Conc.	---	Error limit	---
Error limit	---	Reaction	flag + continue
Rep. measurement	off	QC std. 2 no.	1(100.00 ng/L)
QC std. 1 no.	1(100.00 ng/L)	QC std. 2 limit	± 0.00%
QC std. 1 limit	± 50.00%	Reaction	flag + continue
QC std. act.	flag + continue	QC Recal. factor	Off
Expect. blank abs.	0.0100± 0.0100		
QC precision	off		

Calibration settings

Calib. meth	Standard calib.	Calibr. unit	ng/L
No. standards	1	Conversion fac.	1000000
Type of standards	---	Standard prep.	Premixed
		Blank correct.	---
		Recalib. std. no.	---
Output unit	µg/L	Conversion fac.	1000
Calib. stat.	Mean	Meas. cycles	3
		Blind cycles	1
Stock sol. 1	---	Stock sol. 2	---
Stock sol. 3	---	Stock sol. 4	---
Type of cal. curve	linear	Intercept	calculated
Weighted cal.	off	Grubbs stat.	off
Check of cal. curve	no outlier test		

Sample statistics

Stat. mode	Mean	Meas. cycles	2
Confd. level	95.4 %	Blind cycles	1
Grubbs stat.	---		

Calibration standards

No	Name	State	Pos	Conc./ ng/L	Abs	SD	RSD/%
1	Cal-Zero	(-)	##	0.00	H: 0.000932 A: 0.035926	0.000138 0.006208	14.88 17.28
2	Cal-Std1	(-)	##	100.00	H: 0.004494 A: 0.061286	0.000116 0.001275	2.566 2.082

Hg

Mercury

Calibration function 1


5/24/2023 14:33 Calibration (Peak height)

Abs=k1+k2*conc

k1=0.000932 k2=0.000036

Recal. factor: ---

Slope	0.00004 Abs/(ng/L)	R2-adjusted	1.0000
sc0	1.00000 ng/L	Charact. conc.	122.411 (ng/L)/1%
Lower limit	0 ng/L	Upper limit	110. ng/L
Detection limit	---	Deter. limit	---

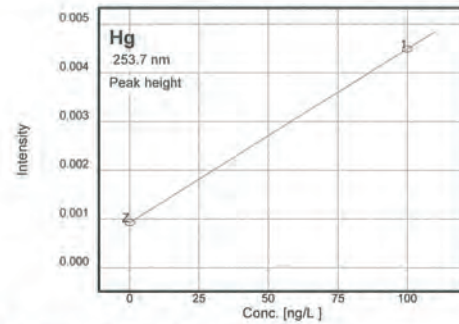


Measurements and events (sorted by time)

Hg	Without enrichment / Abs / FBR 100ng/L_PM 24052023	5/24/2023	14:19
ID	Conc.	Abs	BG
Cal-Zero		0.001039	
		0.000775	
		0.000981	
	0ng/L	0.000932	0.00013872
		0.004528	
Cal-Std1		0.004364	
		0.004589	
	100.ng/L	0.004494	0.00011623
Calibration	Calibration function: 01		

Mercury

Peak plots

Hg

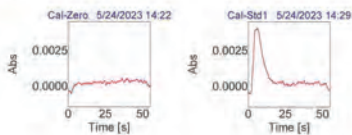

Mercury

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
3344 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

Cert. No.: 23TM1103
Page: 1 of 3

Certificate of Calibration

Equipment :	Autoclave
Manufacturer :	Sanyo
Model :	MLS-3781
Serial No. :	830167
ID No. :	BKK_ML0037
Submitted by :	ALS Laboratory Group (Thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Media Preparation Room
Received Order :	17 July 2023
Calibration Date :	17 July 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Preecha Hlahib
Approved by :	 Approved Signatory
	() Pornthippa Tameyakul () Malee Butkruea (✓) Suwit Imjai
Issue Date :	24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

A 0053615



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2307-0285OC-3
Procedure Used :-

Cert. No.: 23TM1103
Page : 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013823	23LM66	TPA	25 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**

(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)

It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source



	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	22	53	220
Finished of Calibration	22	54	220

Position	Description	Ref. Std. ID No.:
1 =	Center of chamber	22-17TC-01
2 =	Temperature sensor	23-17TC-02
3 =	Exhaust port	19-17TC-03

a 1159503



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2307-0285OC-3

Cert. No.: 23TM1103
Page : 3 of 3

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Operating parameter Set : Temperature = 121 °C
Sterilization period = 15 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor k
121	121	1	120.877	0.39	0.12	1.0	2
		2	120.870				
		3	120.866				

Average* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

a 1159504



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1146
Page : 1 of 3

Certificate of Calibration

Equipment : Incubator

Manufacturer : SHEL-LAB

Model : 1915A

Serial No. : 0200599

ID No. : BKK_ML0010

Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Incubation & Micrological Reading

Received Order : 17 July 2023

Calibration Date : 17 July 2023

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon

Approved by :
Approved Signatory

() Pornthippa Tameyakul
() Malee Butkruea
() Suwit Imjai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services, Equipment Calibration and Testing Services.

A 0056489



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1

Cert. No.: 23TM1146
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	24
REL.Humid. (%)	54	56
AC Supply (Volt)	221	223



Probe installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.50 m
W = 0.75 m
H = 1.2 m
Capacity = 0.45 m³

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

a 1172189



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 23TM1148
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
35.0	35.0	35.0	0.055	0.30	0.44	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.888	34.933	34.815	34.813	35.064	35.019	35.156	35.141	35.087	0.30

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

Malee

a 1172188



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2713-3900-27 FAX. 0-2719-9484



Cert. No.: 22TM1571
Page : 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Binder

Model : ED 240/E2

Serial No. : 00-15533

ID No. : BKK_ML0013

Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 21 November 2022

Calibration Date : 21 November 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

Approved by : 
Approved Signatory

() Pornthippa Tameyakul
(/) Malee Butkruea
() Suwit Imjai

Issue Date : 29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services & Equipment Calibration and Testing Services.

A 0048150



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1

Cert. No.: 22TM1571
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) After Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available



Probe Installation Details :

Dimension of Chamber :

a = 5.0 cm	D = 0.50 m
b = 5.0 cm	W = 0.80 m
c = 5.0 cm	H = 0.60 m
	Capacity = 0.24 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	26
REL.Humid. (%)	53	55
AC Supply (Volt)	219	220

Position :	Ref. Std. ID No.:
1	21-15TC-01
2	21-15TC-02
3	21-15TC-03
4	21-15TC-04
5	21-15TC-05
6	21-15TC-06
7	21-15TC-07
8	21-15TC-08
9 (ref.)	21-15TC-09

Malee

a 1138049



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1
Result of Calibration :- (*) After Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 22TM1571
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (±°C)	Coverage Factor k
180	180	180	0.70	1.5	2.9	1.4	2

Calibration Point (°C)	Measured Temperature (°C)								
	1	2	3	4	5	6	7	8	9 (ref.)
180	179.520	180.585	178.855	179.482	178.827	179.938	179.074	180.199	180.068

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

Malee

a 1138053



Cert. No.: 23TM637
Page : 1 of 3

Certificate of Calibration

Equipment : Water Bath
Manufacturer : Memmert
Model : WNE 45
Serial No. : L712.0429
ID No. : BKK_ML0056
Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Location : Incubator & Microbiological Reading

Received Order : 20 April 2023
Calibration Date : 20 April 2023
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Kunchit Promprai

Approved by :
Approved Signatory

() Ponthippa Tamayakul
() Malee Butkruea
() Suwit Imjai

Issue Date : 24 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services & Equipment Calibration and Testing Services.

A 0053357



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2304-0253OC-1
Procedure Used :-

Cert. No.: 23TM637
Page : 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44073381	22LM78/1	12 May 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- () Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	45	223
Finished of Calibration	25	43	223



Front

Position :	Ref. Std. S/N.:
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016

a 1158265



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2304-0253OC-1
Result of Calibration :- () Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM637
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.492	44.463	44.475	44.510	44.491	0.15
45.0	45.0	45.0	45.005	44.962	44.979	45.016	44.986	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor k
44.5	0.051	0.022	2
45.0	0.080	0.026	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-00-

a 1158264

ภาคผนวก ด

สำเนาหนังสืออนุญาตขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Copper	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
20	Cyanide	Distillation, Colorimetric Method ⁽⁴⁾
21	2,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
22	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
23	2,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
24	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
25	2,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
26	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
27	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
28	Endosulfan Sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
29	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
30	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
31	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
32	Endrin Aldehyde	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
33	Formaldehyde	Distillation, Colorimetric Method ⁽⁴⁾
34	Free Chlorine	1) DPD Ferrous Titrimetric Method ⁽⁴⁾ 2) Iodometric Method ⁽⁴⁾
35	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
36	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
37	Hexavalent Chromium	Filtration, Colorimetric Method ⁽⁴⁾
38	3-Hydroxycarbofuran	High-Performance Liquid Chromatographic Method ⁽⁴⁾
39	Lead	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
40	Manganese	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
41	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/Mass spectrometric Method ⁽⁴⁾
42	Methiocarb	High-Performance Liquid Chromatographic Method ⁽⁴⁾
43	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾

วิมล
(นางรักกัญจน์ อัครสกุลวิไล)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์ของมลพิษ
กรมควบคุมมลพิษ

44 Methomyl...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
44	Methomyl	High-Performance Liquid Chromatographic Method ⁽⁴⁾
45	Nickel	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
46	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method ⁽⁴⁾ 2) Soxhlet Extraction Method ⁽⁴⁾
47	Oxamyl	High-Performance Liquid Chromatographic Method ⁽⁴⁾
48	Propoxur	High-Performance Liquid Chromatographic Method ⁽⁴⁾
49	pH	Electrometric Method ⁽⁴⁾
50	Phenols	1) Distillation, Chloroform Extraction Method ⁽⁴⁾ 2) Distillation, Direct Photometric Method ⁽⁴⁾
51	Selenium	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
52	Sulfide	Iodometric Method ⁽⁴⁾
53	Temperature	Laboratory and Field Methods ⁽⁴⁾
54	Total Dissolved Solids	Dried at 180 °C ⁽⁴⁾
55	Total Kjeldahl Nitrogen	Semi-Micro Kjeldahl Method ⁽⁴⁾
56	Total Suspended Solids	Dried at 103-105 °C ⁽⁴⁾
57	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic Method ⁽⁴⁾
58	Trivalent Chromium	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ⁽⁴⁾ 2) Digestion, inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation ⁽⁴⁾
59	Zinc	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ⁽⁴⁾

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾

วิมล
(นางรักกัญจน์ อัครสกุลวิไล)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์ของมลพิษ
กรมควบคุมมลพิษ

3 Aldrin...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
5	Antimony	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
8	Barium	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
9	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
11	Benzo(a)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
12	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
13	Benzoic Acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
14	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
15	Benzo(g,h,i)perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾

วิมล
(นางรักกัญจน์ อัครสกุลวิไล)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์ของมลพิษ
กรมควบคุมมลพิษ


18 Bis(2-ethylhexyl)phthalate...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
21	Butanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
22	Butyl Benzyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
25	Carbon Disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
27	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
33	Chromium	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾

วิมล
(นางรักกัญจน์ อัครสกุลวิไล)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์ของมลพิษ
กรมควบคุมมลพิษ


34 Chromium (III)...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation ⁽⁸⁾
35	Chromium (VI)	Colorimetric Method ⁽⁴⁾
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
37	Cyanide	Distillation, Colorimetric Method ⁽⁴⁾
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
39	DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
40	DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
41	DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
42	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
43	Di-n-Butyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
47	3,3-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾


 (นางริกาญจน์ นัครสกุลวong)
 ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์สิ่งแวดล้อม
 กรมควบคุมมลพิษ/ป.ป.ช.


51 cis-1,2-Dichloroethylene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
57	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
58	Diethyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
63	Di-n-Octyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
64	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
65	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
67	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾


 (นางริกาญจน์ นัครสกุลวong)
 ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์สิ่งแวดล้อม
 กรมควบคุมมลพิษ/ป.ป.ช.


68 Fluorene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
68	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
69	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
70	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
74	α-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
75	β-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
76	γ-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
81	Lead	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
82	Manganese	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
83	Mercury	1) Cold Vapor Atomic Absorption Spectrometric Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾


 (นางริกาญจน์ นัครสกุลวong)
 ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์สิ่งแวดล้อม
 กรมควบคุมมลพิษ/ป.ป.ช.

84 Methanol...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
84	Methanol	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾ 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
86	Methyl Bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
87	Methylene Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
89	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
90	Methyl tert-Butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
91	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
92	Nickel	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
95	N-Nitrosodi-n-Propylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB 1242 - PCB 1248 - PCB 1254 - PCB 1260	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾


 (นางริกาญจน์ นัครสกุลวong)
 ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์สิ่งแวดล้อม
 กรมควบคุมมลพิษ/ป.ป.ช.

97 Pentachlorophenol...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
98	pH	Electrometric Method ⁽⁴⁾
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
100	Phenol	1) Distillation, Direct Photometric Method ⁽⁴⁾ 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
102	Selenium	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
103	Silver	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
104	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
105	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
106	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
107	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
108	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
109	TPH (C ₈ -C ₆)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(1,3,20)
110	TPH (C ₈ -C ₁₂)	Solvent Extraction, Gas Chromatographic Method ^(9,21)
111	TPH (C ₁₃ -C ₃₃)	Solvent Extraction, Gas Chromatographic Method ^(9,21)
112	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
113	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾

114 1,1,2-Trichloroethane...

(นางริกาญจน์ อัครสกุลวิไล)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์มลพิษ
และประเมินผลกระทบสิ่งแวดล้อม

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
114	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
115	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
118	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
119	Vanadium	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾
120	Vinyl Acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
121	Vinyl Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
122	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
123	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
124	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
125	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ⁽⁴⁾
126	Zinc	1) Digestion, Inductively Coupled Plasma Method ⁽⁴⁾ 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ⁽⁴⁾

ภาคเคมี (ต่อเนื่องจาก) จำนวน 16 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic, Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
2	Arsenic	Isokinetic, Digestion, Inductively Coupled Plasma Method ⁽⁴⁾

3 Carbon Monoxide...

(นางริกาญจน์ อัครสกุลวิไล)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์มลพิษ
และประเมินผลกระทบสิ่งแวดล้อม

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Carbon Monoxide	1) Sampling Bag Non-Dispersive Infrared Method ⁽⁴⁾ 2) Non-Dispersive Infrared Method ⁽⁴⁾ 3) Instrumental Analyzer Method ⁽⁴⁾
4	Chlorine	1) Absorption Sampling, Ion Chromatographic Method ⁽⁴⁾ 2) Isokinetic Sampling, Ion Chromatographic Method ⁽⁴⁾
5	Copper	Isokinetic, Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
6	Dioxins	Isokinetic Sampling, Analysis by ISO/IEC 17025 Accredited Laboratory or Analysis by Department of Industrial Works Registered Laboratory (Dioxins/Furans Analysis Approved) ⁽⁴⁾
7	Hydrogen Chloride	1) Absorption Sampling, Ion Chromatographic Method ⁽⁴⁾ 2) Isokinetic Sampling, Ion Chromatographic Method ⁽⁴⁾
8	Hydrogen Sulfide	Absorption Sampling, Iodometric Method ⁽⁴⁾
9	Lead	Isokinetic, Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
10	Mercury	1) Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽⁴⁾ 2) Isokinetic, Digestion, Inductively Coupled Plasma Method ⁽⁴⁾
11	Opacity	Ringelmann's Method ⁽²⁾
12	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method ⁽⁴⁾ 2) Chemiluminescence Method ⁽⁴⁾ 3) Instrumental Analyzer Method ⁽⁴⁾
13	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method ⁽⁴⁾ 2) UV Fluorescence Method ⁽⁴⁾ 3) Instrumental Analyzer Method ⁽⁴⁾
14	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method ⁽⁴⁾
15	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method ⁽⁴⁾
16	Xylene	Absorption Sampling, Gas Chromatographic Method ⁽⁴⁾

สิ่งบ่งชี้...

(นางริกาญจน์ อัครสกุลวิไล)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์มลพิษ
และประเมินผลกระทบสิ่งแวดล้อม

สิ่งบ่งชี้หรือวัตถุที่ไม่ใช่แล้ว จำนวน 35 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,3,20) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)
2	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,6,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,18) 3) Digestion, Inductively Coupled Plasma Method ^(7,15) 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^(7,16)
3	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,6,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,18) 3) Digestion, Inductively Coupled Plasma Method ^(7,15) 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^(7,16)
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,6,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,18) 3) Digestion, Inductively Coupled Plasma Method ^(7,15) 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^(7,16)
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,6,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,18) 3) Digestion, Inductively Coupled Plasma Method ^(7,15) 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^(7,16)

6 Cadmium...


(นางริกาญจน์ อัครสกุลวิไล)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์มลพิษ
และประเมินผลกระทบสิ่งแวดล้อม

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
6	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,6,15) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,16) 3) Digestion, Inductively Coupled Plasma Method ^(7,15) 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,9,20) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)
8	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,6,15) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,16) 3) Digestion, Inductively Coupled Plasma Method ^(7,15) 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
9	Chromium (III)	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation Method ^(1,6,13,17) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation Method ^(1,6,16,17) 3) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^(7,8,13,17) 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^(7,8,16,17)
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method ^(1,6,17) 2) Alkaline Digestion, Colorimetric Method ^(8,17)


 (นางกัญจน์ ชีรสุกุลชัย)
 ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์สิ่งแวดล้อมพิษ
 กรมควบคุมมลพิษ


11 Cobalt...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,6,15) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,16) 3) Digestion, Inductively Coupled Plasma Method ^(7,15) 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
12	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,6,15) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,16) 3) Digestion, Inductively Coupled Plasma Method ^(7,15) 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
13	2,4-D	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,9,20) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,9,20) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,9,20) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,9,20)


 (นางกัญจน์ ชีรสุกุลชัย)
 ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์สิ่งแวดล้อมพิษ
 กรมควบคุมมลพิษ

2) Soxhlet...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
17	Dieldrin	2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31) 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,9,20) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,9,20) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,9,20) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)
20	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,6,15) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,16) 3) Digestion, Inductively Coupled Plasma Method ^(7,15) 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,9,20) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^(1,6,18)


 (นางกัญจน์ ชีรสุกุลชัย)
 ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์สิ่งแวดล้อมพิษ
 กรมควบคุมมลพิษ

2) Waste Extraction...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
23	Methoxychlor	2) Waste Extraction, Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method ^(1,6,19) 3) Waste Extraction, Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method ^(1,6,20) 4) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^(1,8) 5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method ⁽⁹⁾ 6) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method ⁽²⁰⁾
24	Mirex	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,9,20) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)
25	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,6,15) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,16) 3) Digestion, Inductively Coupled Plasma Method ^(7,15) 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
26	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,6,15) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,16) 3) Digestion, Inductively Coupled Plasma Method ^(7,15) 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)


 (นางกัญจน์ ชีรสุกุลชัย)
 ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์สิ่งแวดล้อมพิษ
 กรมควบคุมมลพิษ

27 Polychlorinated...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5,6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^(1,6,23) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,23) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)

28 PentachlorophenoL...

(นางวิภาดา ชัยกรกุลวิไล)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์มลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
28	Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,9,23) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)
29	pH	Electrometric Method ^(27,36)
30	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,4,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,16) 3) Digestion, Inductively Coupled Plasma Method ^(7,13) 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
31	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,4,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,4,16)
32	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,4,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,4,16) 3) Digestion, Inductively Coupled Plasma Method ^(7,13) 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
33	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^(1,9,23) 2) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^(22,31)
34	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,4,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,6,16) 3) Digestion, Inductively Coupled Plasma Method ^(7,13)

4) Digestion...

(นางวิภาดา ชัยกรกุลวิไล)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์มลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
35	Zinc	4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16) 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^(1,6,13) 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(1,4,16) 3) Digestion, Inductively Coupled Plasma Method ^(7,13) 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)

ดิน จำนวน 125 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
2	Acetone	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(13,20)
3	Aldrin	1) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
4	Anthracene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
5	Antimony	1) Digestion, Inductively Coupled Plasma Method ^(7,13) 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method ^(7,13) 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
7	Atrazine	1) Soxhlet Extraction, Gas Chromatographic Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
8	Barium	1) Digestion, Inductively Coupled Plasma Method ^(7,13) 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)

9 Benz(a)anthracene...

(นางวิภาดา ชัยกรกุลวิไล)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์มลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
9	Benz(a)anthracene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
10	Benzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,20)
11	Benzo(b)fluoranthene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
12	Benzo(k)fluoranthene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
13	Benzolc acid	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
14	Benzo(a)pyrene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
15	Benzo(g,h,i)perylene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method ^(7,13) 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
17	Bis(2-chloroethyl)ether	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
18	Bis(2-ethylhexyl)phthalate	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,20)
20	Bromoform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,20)
21	Butanol	Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(12,20)
22	Butyl Benzyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method ^(7,13) 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
24	Carbazole	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
25	Carbon Disulfide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,20)

26 Carbon tetrachloride...

(นางวิภาดา ชัยกรกุลวิไล)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์มลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
27	Chlordane	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
28	p-Chloroaniline	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
32	2-Chlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
33	Chromium	1) Digestion, Inductively Coupled Plasma Method ^(7,15) 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^(7,16)
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^(7,15,17) 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^(7,16,17)
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method ^(8,17)
36	Chrysene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
37	Cyanide	Extraction, Distillation, Colorimetric Method ^(25,28)
38	2,4-D	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
39	DDO	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)

วิทย์
(นางวิภาดา ชัยยศกุลวิไล)
ผู้อำนวยการศูนย์การวิเคราะห์ทางเคมี

40 DDE...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
40	DDE	1) Soxhlet Extraction, Gas Chromatographic/ Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
41	DDT	1) Soxhlet Extraction, Gas Chromatographic/ Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
42	Dibenz(a,h)anthracene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
43	Di-n-Butyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
47	3,3-Dichlorobenzidine	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
53	2,4-Dichlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)

วิทย์
(นางวิภาดา ชัยยศกุลวิไล)
ผู้อำนวยการศูนย์การวิเคราะห์ทางเคมี

57 Dieldrin...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
57	Dieldrin	1) Soxhlet Extraction, Gas Chromatographic/ Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
58	Diethyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
59	2,4-Dimethylphenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
60	2,4-Dinitrophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
61	2,4-Dinitrotoluene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
62	2,6-Dinitrotoluene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
63	Di-n-Octyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
64	Endosulfan	1) Soxhlet Extraction, Gas Chromatographic/ Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
65	Endrin	1) Soxhlet Extraction, Gas Chromatographic/ Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
67	Fluoranthene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
68	Fluorene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
69	Heptachlor	1) Soxhlet Extraction, Gas Chromatographic/ Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
70	Heptachlor Epoxide	1) Soxhlet Extraction, Gas Chromatographic/ Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)

วิทย์
(นางวิภาดา ชัยยศกุลวิไล)
ผู้อำนวยการศูนย์การวิเคราะห์ทางเคมี

71 Hexachlorobenzene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
71	Hexachlorobenzene	1) Soxhlet Extraction, Gas Chromatographic/ Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^(14,24)
74	α-HCH	1) Soxhlet Extraction, Gas Chromatographic/ Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
75	β-HCH	1) Soxhlet Extraction, Gas Chromatographic/ Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
76	γ-HCH	1) Soxhlet Extraction, Gas Chromatographic/ Method ^(10,22) 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
77	Hexachlorocyclopentadiene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
78	Hexachloroethane	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
79	Indeno(1,2,3-cd)pyrene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
80	Isophorone	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^(25,31)
81	Lead	1) Digestion, Inductively Coupled Plasma Method ^(7,15) 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^(7,16)
82	Manganese	1) Digestion, Inductively Coupled Plasma Method ^(7,15) 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^(7,16)
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ⁽¹⁸⁾

วิทย์
(นางวิภาดา ชัยยศกุลวิไล)
ผู้อำนวยการศูนย์การวิเคราะห์ทางเคมี

2) Thermal...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
84	Methanol	2) Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry ⁽¹⁹⁾
85	Methoxychlor	3) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method ⁽²⁰⁾
86	Methyl Bromide	Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method ^(12,24)
87	Methylene Chloride	1) Soxhlet Extraction, Gas Chromatographic Method ^(25,22)
88	2-methylphenol	2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
89	2-Methylnaphthalene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
90	Methyl tert-Butyl Ether	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
91	Naphthalene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
92	Nickel	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
93	Nitrobenzene	1) Digestion, Inductively Coupled Plasma Method ^(7,13)
94	N-Nitrosodiphenylamine	2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,14)
95	N-Nitrosodipropylamine	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
96	Polychlorinated biphenyls (PCBs)	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
	- Aroclor 1016	1) Soxhlet Extraction, Gas Chromatographic Method ^(10,22)
	- Aroclor 1221	2) Automated Soxhlet Extraction, Gas Chromatographic Method ^(25,31)
	- Aroclor 1232	

สำนักงานสิ่งแวดล้อมแห่งชาติ
(นางวิภาดา ชัยกุลกิจ)

- Aroclor 1242...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
	- Aroclor 1242	
	- Aroclor 1248	
	- Aroclor 1254	
	- Aroclor 1260	
	- 2-Chlorobiphenyl	
	- 2,2',3,3'-Tetrachlorobiphenyl	
	- 2,2',3,4'-Tetrachlorobiphenyl	
	- 2,3',4,4'-Tetrachlorobiphenyl	
	- 2,2',3,4,5-Pentachlorobiphenyl	
	- 2,2',4,5,5'-Pentachlorobiphenyl	
	- 2,3,3',4,6-Pentachlorobiphenyl	
	- 2,2',3,4,4',5'-Hexachlorobiphenyl	
	- 2,2',3,4,5,5'-Hexachlorobiphenyl	
	- 2,2',3,5,5',6-Hexachlorobiphenyl	
	- 2,2',4,4',5,5'-Hexachlorobiphenyl	
	- Hexachlorobiphenyl	
	- 2,2',4,4',5,5'-Hexachlorobiphenyl	
	- 2,2',3,3',4,4',5-Heptachlorobiphenyl	
	- 2,2',3,4,4',5,5'-Heptachlorobiphenyl	
	- 2,2',3,4,4',5,6-Heptachlorobiphenyl	
	- 2,2',3,4,4',5,6-Heptachlorobiphenyl	
	- 2,2',3,3',4,4',5,6-Nonachlorobiphenyl	
97	Pentachlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
98	Phenanthrene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
99	Phenol	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
100	Pyrene	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)

สำนักงานสิ่งแวดล้อมแห่งชาติ
(นางวิภาดา ชัยกุลกิจ)

101 Selenium...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
101	Selenium	1) Digestion, Inductively Coupled Plasma Method ^(7,15)
102	Silver	2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,14)
103	Styrene	1) Digestion, Inductively Coupled Plasma Method ^(7,15)
104	1,1,2,2-Tetrachloroethane	2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
106	Toluene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
107	Toxaphene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
108	TPH (C ₉ -C ₉)	1) Soxhlet Extraction, Gas Chromatographic Method ^(10,22)
109	TPH (C ₉ -C ₁₆)	2) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
110	TPH (C ₁₆ -C ₃₂)	1) Solvent Extraction, Gas Chromatographic Method ^(11,21)
111	1,2,4-Trichlorobenzene	2) Automated Soxhlet Extraction, Gas Chromatographic Method ^(25,31)
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
114	Trichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
115	2,4,5-Trichlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)

สำนักงานสิ่งแวดล้อมแห่งชาติ
(นางวิภาดา ชัยกุลกิจ)

116 2,4,6-Trichlorophenol...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
116	2,4,6-Trichlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^(25,31)
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
118	Vanadium	1) Digestion, Inductively Coupled Plasma Method ^(7,15)
119	Vinyl Acetate	2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,16)
120	Vinyl Chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
121	m-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
122	o-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
123	p-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
124	Xylene (Total)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^(14,24)
125	Zinc	1) Digestion, Inductively Coupled Plasma Method ^(7,12)
		2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^(7,14)


เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2548. เรื่อง การกำจัดสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว.ราชกิจจานุเบกษา. 25 มกราคม 2549. เล่มที่ 123 ตอนที่ 11ง.
- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณแอมโมเนียที่เจือปนในอากาศที่ระบายออกจากปล่องของหน่วยโรงสีข้าวที่ใช้ถ่านหินเชื้อเพลิง.ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนที่ 125ง.
- สมาคมวิศวกรสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรืองวัฒนาภิรมย์, 2547.
- APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 23rd ed. Washington, DC: APHA, 2017.
- United States Environmental Protection Agency. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2019.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SW-846, 1997.

สำนักงานสิ่งแวดล้อมแห่งชาติ
(นางวิภาดา ชัยกุลกิจ)


7. United States...

7. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Acid Digestion of Sludges and Sediments and Soils. SW-846 Method 3050B, 1996.
8. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A, 1996.
9. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Separatory Funnel Liquid-Liquid Extraction. SW-846 Method 3510C, 1996.
10. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Soxhlet Extraction. SW-846 Method 3540C, 1996.
11. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Microscale Solvent Extraction (MSE). SW-846 Method 3570, 2002.
12. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds (VOCs) in Various Sample Matrices Using Equilibrium Headspace Analysis. SW-846 Method 5021A, 2014.
13. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Purge-and-Trap for Aqueous Samples. SW-846 Method 5030B, 1996.
14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples. SW-846 Method 5035, 1996.
15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Inductively Coupled Plasma- Atomic Emission Spectrometry. SW-846 Method 6010B, 1996.
16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Inductively Coupled Plasma-Mass Spectrometry. SW-846 Method 6020A, 2007.
17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A, 1992.
18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B, 2007.
19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry. SW-846 Method 7473, 2007.


(นางริกาญจน์ นัครสกุลไชย)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์ของมลพิษ
(ประเทศไทย) สำนักงาน

20. United States

20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Mercury in Sediment and Tissue Sample by Atomic Fluorescence Spectrometry. SW-846 Method 7474, 2007.
21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Nonhalogenated Organics Using GC/FID. SW-846 Method 8015B, 1996.
22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Organochlorine Pesticides by Gas Chromatography. SW-846 Method 8081B, 2007.
23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Polychlorinated Biphenyls (PCBs) by Gas Chromatography. SW-846 Method 8082, 1996.
24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8260D, 2018.
25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8270E, 2018.
26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Total and Amenable Cyanide: Distillation SW-846 Method 9010B, 1996.
27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Cyanide Extraction Procedure for Solids and Oil. SW-846 Method 9013A, 1996.
28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014, 2014.
29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. pH Electrometric Measurement. SW-846 Method 9040C, 2004.
30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Soil and Waste pH. SW-846 Method 9045D, 2004.
31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Automated Soxhlet Extraction. SW-846 Method 3541, 1994.


(นางริกาญจน์ นัครสกุลไชย)
ผู้อำนวยการศูนย์มาตรฐานวิธีการวิเคราะห์ของมลพิษ
(ประเทศไทย) สำนักงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ การวิจัยและเตือนภัยมลพิษโรงงาน กรมโรงงานอุตสาหกรรม โทร. ๐ ๒๒๐๓ ๔๐๐๒, ๔๐๐๓

ที่ ๒๓ ๐๓๓๐(๑)/ ๕๓๗๕



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๐๔ มีนาคม ๒๕๖๖

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และขอพิจารณาผลของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๔ กุมภาพันธ์ ๒๕๖๖

ตามที่หนังสือที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการ
วิเคราะห์เอกชน เลขทะเบียน ๖-๒๐๔-๕๓๗๕ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ
เขตสามพร้าว กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ออกเลือกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๕ ราย

- | | |
|----------------------------------|--------------------------|
| ๑) นายนคร สุขเจริญ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๑๒ |
| ๒) นายบัญชา นามขัตต์ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๑๓ |
| ๓) นายอรุณพล นิยมวิทย์พันธ์ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๑๔ |
| ๔) นางสาวพัชรียา พงษ์สมบัติ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๑๕ |
| ๕) นางสาวภาณิดา สุวรรณศรีกุล | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๑๖ |
| ๖) นางสาวกรรณิณี อึ้งศิริ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๑๗ |
| ๗) นายสมโภช วัธสา | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๑๘ |
| ๘) นายณัฐนันท์ ปานประเสริฐ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๑๙ |
| ๙) ว่าที่ร้อยตรีภาณุพงศ์ แสนศิริ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๒๐ |
| ๑๐) นายณัฐนันท์ พุดศิริ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๒๑ |
| ๑๑) นายณัฐนันท์ เชื้อละออง | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๒๒ |
| ๑๒) นางสาวกาญจนา คังคุด | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๒๓ |
| ๑๓) นางสาววันฉัตร นิยมกลาง | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๒๔ |
| ๑๔) นางสาวกัญญารัตน์ ศรีนิลลา | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๒๕ |
| ๑๕) นายศิริวัฒน์ พาณิชย์ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๒๖ |
| ๑๖) นางสาวกนกภรณ์ อูระ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๒๗ |
| ๑๗) นางสาวจิตติภา ปะเทืองสุข | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๒๘ |
| ๑๘) นางสาวอริสา วิริยะขันติธรรม | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๒๙ |
| ๑๙) นางสาวภาณิดา ยอดอินทร์ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๓๐ |

๒. ให้เพิ่มเจ้าหน้าที่...

๒. ให้เพิ่มเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ ราย

- | | |
|-------------------------------|---------------------------|
| ๑) นายกาญจน์พิศ กิตติคุณนิษฐ์ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๐๐๑ |
| ๒) นายภัทรพล สว่างใจธรรม | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๐๐๒ |
| ๓) นายราธิบ เพ็ญชัยคำ | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๐๐๓ |
| ๔) นายศิริโชค พงษ์ประสม | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๐๐๔ |
| ๕) นายณัฐนันท์ คังคุด | ทะเบียนเลขที่ ๖-๒๐๔-๖๑๐๐๕ |

อนึ่ง หนังสือฉบับนี้จะส่งต่อมายังหน่วยงานที่เกี่ยวข้องรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ที่ ๒๓ ๐๓๓๐(๑)/๒๐๖๔ ลงวันที่ ๒๘ มกราคม ๒๕๖๔ คือในวันที่ ๒ กันยายน ๒๕๖๖ ทั้งนี้ สามารถยื่นคำขอ
ผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ที่ท้ายหนังสือฉบับนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นางริกาญจน์ นัครสกุลไชย)

นักวิทยาศาสตร์ชำนาญการพิเศษ วิชาการการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติการการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๒๐๓ ๖๓๑๒ ต่อ ๒๒๐๓-๕
โทรสาร ๐ ๒๒๐๓ ๖๓๑๒ ต่อ ๒๒๐๓-๔
ไปรษณีย์อิเล็กทรอนิกส์ sarabangudlw@mail.go.th



"อุตสาหกรรมสีเขียว ประเทศไทยอย่างยั่งยืน ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"





ที่ อภ ๐๓๓๐(๑)/ ๖๑๖๕

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒๓ มีนาคม ๒๕๖๖

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๐ มีนาคม ๒๕๖๖

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด
ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ๖-๒๐๔๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐
ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรของห้องปฏิบัติการ
วิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เปลี่ยนแปลงชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการ
วิเคราะห์ จากเดิม นางสาวสุวิมล มงคลจิ๋วพิทย์ ทะเบียนเลขที่ ๖-๒๐๐๔-๖-๔๗๗๑๙ เป็น นางสาวอัญญพร มงคลจิ๋วพิทย์
ทะเบียนเลขที่ ๖-๒๐๐๔-๖-๔๗๗๑๙

ทั้งนี้ หากท่านมีความประสงค์จะยื่นคำขอใดๆ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์
ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ที่แนบมาด้วย

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

สุวิมล

(นายประสม คำพงษ์)
ผู้อำนวยการกองวิจัยและพัฒนาสิ่งแวดล้อมโรงงาน
ปฏิบัติการกรมโรงงานอุตสาหกรรม

กองวิจัยและพัฒนาสิ่งแวดล้อมโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๕๓๐ ๖๓๓๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๕๓๐ ๖๓๓๒ ต่อ ๒๑๐๓

ไปรษณีย์อิเล็กทรอนิกส์ saraban@dlw.mail.go.th



ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์



"อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา จุลอุตสาหกรรมสีเขียว"



คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน

แบบ ปอ.1

วันที่ 4 เดือน สิงหาคม พ.ศ. 2566

ข้าพเจ้า () ผู้รับใบอนุญาตประกอบกิจการโรงงาน

(✓) บริษัท/ห้างหุ้นส่วนจำกัด เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

ตั้งอยู่ที่เลขที่ 104

หมู่ที่ -

ตรอก/ซอย

พัฒนาการ 40

ถนน

พัฒนาการ

ตำบล/แขวง

พัฒนาการ

อำเภอ/เขต

สวนหลวง

จังหวัด

กรุงเทพมหานคร

รหัสไปรษณีย์ 10250

โทรศัพท์

02 760-3040

โทรสาร

0 2 760-3197

ได้รับทราบระเบียบกรมโรงงานอุตสาหกรรมว่าด้วยการขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน พ.ศ. 2560 โดยตลอดแล้วและยินยอม
ปฏิบัติตามระเบียบทุกประการ และได้แนบเอกสารต่างๆ ตามรายการเอกสารประกอบการพิจารณา (แบบ ปอ.1-1) มาพร้อมนี้

รายการขอดำเนินการ

การดำเนินการ	รายละเอียด (รายการ)				
	น้ำเสีย/น้ำทิ้ง	น้ำใต้ดิน	อากาศเสีย	สิ่งปฏิกูลหรือ วัสดุที่ไม่ใช้แล้ว	ดิน
[] ขอขึ้นทะเบียนห้องปฏิบัติการ วิเคราะห์เอกชน					
[✓] ต่ออายุห้องปฏิบัติการวิเคราะห์ เอกชน	59	126	16	35	125
[✓] เปลี่ยนแปลงสารมลพิษที่วิเคราะห์ (✓) เพิ่มสารมลพิษ () ยกเลิกสารมลพิษ	-	-	12	-	-
[✓] เปลี่ยนแปลงบุคลากร (✓) เพิ่มบุคลากร (✓) ยกเลิกบุคลากร	จำนวน จำนวน	38 ราย (รายละเอียดตาม แบบ ปว.1) 2 ราย (รายละเอียดตาม แบบ ปว.1)			
[] ยกเลิกห้องปฏิบัติการวิเคราะห์เอกชน					
[] อื่นๆ โปรดระบุ					

จึงเรียนมาเพื่อโปรดพิจารณา

นายประสม คำพงษ์

เพื่อโปรดพิจารณา

นายประสม คำพงษ์

ผู้อำนวยการกองวิจัยและพัฒนาสิ่งแวดล้อมโรงงาน

ลงชื่อ

(นางศุภณีย์ เลขากุลพร)

ผู้มีอำนาจลงนามแทนนิติบุคคล

ประทับตรา (ถ้ามี)

ALS Laboratory Group
(Thailand) Co., Ltd.



F-ED-LR-01- 1/1

✉ bangkok@alsglobal.com



ALS Line Official
ID : @alsthailand



ALS Facebook
Search : ALS Thailand



right solutions.
right partner.