ภาคผนวก ง

ใบรับรองการสอบเทียบเครื่องมือ

right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Total Suspended Particulate	High Volume	RYG_FS0174	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0393	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0663	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0176	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0291	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	RYG_EN0001	1-Mar-23	1-Mar-24	12
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0184	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0185	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0190	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0186	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0189	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	Digital Balance	RYG_EN0001	1-Mar-23	1-Mar-24	12
Ambient	Nitrogen Dioxide	NO_2 Analyzer	RYG_FS0453	1-Jul-23	1-Jan-24	6
Ambient	Nitrogen Dioxide	NO_2 Analyzer	RYG_FS0272	1-Jul-23	1-Jan-24	6
Ambient	Nitrogen Dioxide	NO_2 Analyzer	RYG_FS0463	1-Jul-23	1-Jan-24	6
Ambient	Nitrogen Dioxide	NO_2 Analyzer	RYG_FS0459	1-Jul-23	1-Jan-24	6
Ambient	Nitrogen Dioxide	NO_2 Analyzer	RYG_FS0461	1-Jul-23	1-Jan-24	6
Ambient	Sulfur Dioxide	SO_2 Analyzer	RYG_FS0452	2-Jul-23	2-Jan-24	6
Ambient	Sulfur Dioxide	SO_2 Analyzer	RYG_FS0271	2-Jul-23	2-Jan-24	6
Ambient	Sulfur Dioxide	SO_2 Analyzer	RYG_FS0462	2-Jul-23	2-Jan-24	6
Ambient	Sulfur Dioxide	SO_2 Analyzer	RYG_FS0458	2-Jul-23	2-Jan-24	6
Ambient	Sulfur Dioxide	SO_2 Analyzer	RYG_FS0460	2-Jul-23	2-Jan-24	6
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0081	18-Jan-23	18-Jul-24	18
Noise	Leq 24 hrs	Sound Calibrator	RYG_FS0496	17-Jan-23	17-Jan-24	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0016	1-Sep-23	1-Sep-24	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0017	3-Jan-23	3-Jan-24	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0018	3-Jan-23	3-Jan-24	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0019	13-Jan-23	13-Jan-24	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0020	13-Jan-23	13-Jan-24	12
Noise	Leq 5 min	Sound Calibrator	RYG_FS0496	17-Jan-23	17-Jan-24	12
Noise	Leq 5 min	Sound Level Meter	RYG_FS0016	1-Sep-23	1-Sep-24	12
Noise	Leq 5 min	Sound Level Meter	RYG_FS0017	3-Jan-23	3-Jan-24	12
Noise	Leq 5 min	Sound Level Meter	RYG_FS0018	3-Jan-23	3-Jan-24	12
Noise	Leq 5 min	Sound Level Meter	RYG_FS0019	13-Jan-23	13-Jan-24	12
Noise	Leq 5 min	Sound Level Meter	RYG_FS0020	13-Jan-23	13-Jan-24	12
Noise	Noise Annoyance	Sound Calibrator	RYG_FS0496	17-Jan-23	17-Jan-24	12
Noise	Noise Annoyance	Sound Level Meter	RYG_FS0016	1-Sep-23	1-Sep-24	12
Noise	Noise Annoyance	Sound Level Meter	RYG_FS0017	3-Jan-23	3-Jan-24	12
Noise	Noise Annoyance	Sound Level Meter	RYG_FS0018	3-Jan-23	3-Jan-24	12
Noise	Noise Annoyance	Sound Level Meter	RYG_FS0019	13-Jan-23	13-Jan-24	12
Noise	Noise Annoyance	Sound Level Meter	RYG_FS0020	13-Jan-23	13-Jan-24	12
Rayong Lab	Cyanide	SPECTROPHOTOMETER	RYG_EN0037	18-Sep-23	18-Mar-25	18
Rayong Lab	pH at 25 °C	pH meter	RYG_EN0183	27-Feb-23	27-Feb-24	12
Rayong Lab	Nitrate	Spectrophotometer	RYG_EN0037	18-Sep-23	18-Mar-25	18
Rayong Lab	Ammonia Nitrogen	SPECTROPHOTOMETER	RYG_EN0037	18-Sep-23	18-Mar-25	18
Rayong Lab	Dissolved Oxygen	Chamber (Cold Room)	RYG_EN0184	25-Jan-23	25-Jul-24	18
Rayong Lab	BOD	DO meter with Sensor	RYG_EN0032	24-Jul-23	24-Jan-25	18
Rayong Lab	BOD	Incubator	RYG_EN0154	29-May-23	29-Nov-24	18
Rayong Lab	Temperature	Digital Thermometer With Sensor	RYG_FS0468	10-Oct-23	10-Oct-24	12
Rayong Lab	Color	Chamber (Cold Room)	RYG_EN0184	25-Jan-23	25-Jul-24	18
Rayong Lab	Fluoride	pH ISE Meter	RYG_EN0183	27-Feb-23	27-Feb-24	12
Rayong Lab	Sulfate	Spectrophotometer	RYG_EN0037	18-Sep-23	18-Mar-25	18
Rayong Lab	Turbidity	Chamber (Cold Room)	RYG_EN0184	25-Jan-23	25-Jul-24	18
Water Lab	Permanent Hardness	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Total Alkalinity	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Total Hardness	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0273	29-Nov-22	29-May-24	18

right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Water Lab	Hexavalent Chromium	Spectrophotometer	BKK_EN0018	15-Sep-23	15-Sep-24	12
Water Lab	Aluminium	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Aluminium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Aluminium	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Lead	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Lead	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Lead	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Iron	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Iron	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Iron	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Manganese	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Manganese	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Manganese	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Copper	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Copper	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Copper	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Nickel	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Nickel	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Nickel	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Arsenic	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Arsenic	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Arsenic	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Barium	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Barium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Barium	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Chromium	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Chromium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Chromium	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Cadmium	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Cadmium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Cadmium	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Selenium	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Selenium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Selenium	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Silver	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Silver	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Silver	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Zinc	ICP-MS	BKK_EL0026	12-Jun-23	11-Jun-24	12
Water Lab	Zinc	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Zinc	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Water Lab	Mercury	DUO-CVAFS / CVAAS	BKK_EL0023	24-May-23	24-May-24	12
Water Lab	Chloride	Ion Chromatography	BKK_EN0069	12-Jan-23	12-Jan-24	12
Water Lab	*Escherichia coli*	Autoclave	BKK_ML0041	4-Oct-23	4-Apr-25	18
Water Lab	*Escherichia coli*	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	*Escherichia coli*	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	*Escherichia coli*	Water Bath	BKK_ML0056	20-Apr-23	20-Apr-24	12
Water Lab	Fecal Coliform	Autoclave	BKK_ML0041	4-Oct-23	4-Apr-25	18
Water Lab	Fecal Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	Fecal Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Fecal Coliform	Water Bath	BKK_ML0056	20-Apr-23	20-Apr-24	12
Sludge	Silver	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Sludge	Silver	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Sludge	Silver	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Sludge	Lead	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Sludge	Lead	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Sludge	Lead	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Sludge	Mercury	DUO-CVAFS / CVAAS	BKK_EL0023	24-May-23	24-May-24	12

right solutions.
right partner.


รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Sludge	Manganese	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Sludge	Manganese	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Sludge	Manganese	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Sludge	Copper	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Sludge	Copper	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Sludge	Copper	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Sludge	Nickel	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Sludge	Nickel	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Sludge	Nickel	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Sludge	Arsenic	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Sludge	Arsenic	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Sludge	Arsenic	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Sludge	Cadmium	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Sludge	Cadmium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Sludge	Cadmium	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Sludge	Zinc	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Sludge	Zinc	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Sludge	Zinc	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Sludge	Hexavalent Chromium	Spectrophotometer	BKK_EN0018	15-Sep-23	15-Sep-24	12
Soil	Arsenic	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Soil	Arsenic	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Soil	Arsenic	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Soil	Barium	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Soil	Barium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Soil	Barium	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Soil	Cadmium	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Soil	Cadmium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Soil	Cadmium	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Soil	Hexavalent Chromium	Spectrophotometer	BKK_EN0018	15-Sep-23	15-Sep-24	12
Soil	Iron	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Soil	Iron	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Soil	Iron	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Soil	Lead	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Soil	Lead	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Soil	Lead	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Soil	Manganese	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Soil	Manganese	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Soil	Manganese	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Soil	Mercury	Mercury Analyzer	BKK_EL0128	30-Nov-22	30-Nov-23	12
Soil	Moisture	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Soil	Nickel	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Soil	Nickel	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Soil	Nickel	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Soil	pH aqueous phase 50% (w/v)	pH meter	BKK_EN0072	12-Sep-22	12-Mar-24	18
Soil	Selenium	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Soil	Selenium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Soil	Selenium	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Soil	Silver	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Soil	Silver	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Soil	Silver	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18
Soil	Zinc	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	12
Soil	Zinc	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Soil	Zinc	Chamber (Cold Room)	BKK_EN0167	1-Jul-22	30-Dec-23	18

High Volume Air Sampler Calibration Worksheet

Project Site :	Rojana Industriak Park Public Co., Ltd.	**Barometric Pressure (mm Hg) :**	755
Calibrate Location :	สถานีที่ A1 : มัสยิดนูร์ลมุกรอบีน	**Temperature (°C) :**	28
Calibrate Date :	4-Nov-23	**High Volume ID :**	RYG_FS0174
CalibrationSheet No.:	C-041123-RYG_FS0174	**High Volume Model :**	TE-5170D
Calibrator ID:	RYG_FS0206	**High Volume S/N :**	4800
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.47433
Calibrator S/N :	1543	**Calibrator Intercept :**	-0.01503

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	1.8	0.9175	40	Slope : 48.8154
2	2.2	1.0127	44	Intercept : -5.2239
3	2.8	1.1406	50	Correlation Coefficient : 0.9985
4	3.2	1.2183	54	
5	3.8	1.3263	60	

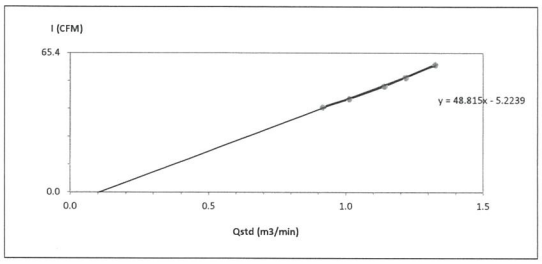

Calibrated by ชัชชัย

(Mr.Chatchai Sukpia)
Field Scientist(1)

Approved by :


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

FORM NO.: F 06-073 REVISION NO.: - ISSUE DATE: 14/03/16

High Volume Air Sampler Calibration Worksheet

Project Site :	Rojana Industriak Park Public Co., Ltd.	**Barometric Pressure (mm Hg) :**	755
Calibrate Location :	สถานีที่ A2 : วัดอัมพวัน	**Temperature (°C) :**	28
Calibrate Date :	4-Nov-23	**High Volume ID :**	RYG_FS0393
CalibrationSheet No.:	C-041123-RYG_FS0393	**High Volume Model :**	TE-5170D
Calibrator ID:	RYG_FS0206	**High Volume S/N :**	5682
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.47433
Calibrator S/N :	1543	**Calibrator Intercept :**	-0.01503

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.0	0.9663	40	Slope : 54.0799
2	2.4	1.0571	44	Intercept : -12.5449
3	2.8	1.1406	50	Correlation Coefficient : 0.9926
4	3.4	1.2553	54	
5	3.8	1.3263	60	

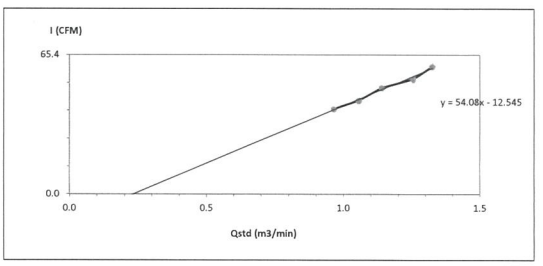

Calibrated by ชัชชัย

(Mr.Chatchai Sukpia)
Field Scientist(1)

Approved by :


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

FORM NO.: F 06-073 REVISION NO.: - ISSUE DATE: 14/03/16

High Volume Air Sampler Calibration Worksheet

Project Site :	Rojana Industriak Park Public Co., Ltd.	**Barometric Pressure (mm Hg) :**	755
Calibrate Location :	สถานีที่ A3 : วัดป่าสามัคคีธรรมาวาส	**Temperature (°C) :**	28
Calibrate Date :	4-Nov-23	**High Volume ID :**	RYG_FS0663
CalibrationSheet No.:	C-041123-RYG_FS0663	**High Volume Model :**	TE-5009X
Calibrator ID:	RYG_FS0206	**High Volume S/N :**	6260
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.47433
Calibrator S/N :	1543	**Calibrator Intercept :**	-0.01503

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.0	0.9663	40	Slope : 61.4314
2	2.4	1.0571	44	Intercept : -20.1079
3	2.8	1.1406	50	Correlation Coefficient : 0.9952
4	3.2	1.2183	54	
5	3.6	1.2913	60	

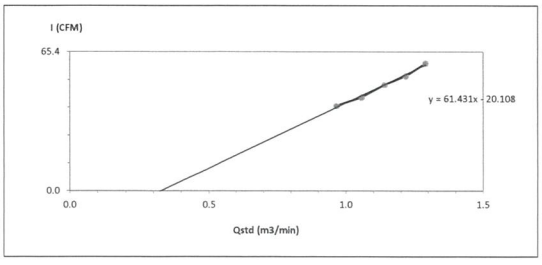

Calibrated by ชัชชัย

(Mr.Chatchai Sukpia)
Field Scientist(1)

Approved by :


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

FORM NO.: F 06-073 REVISION NO.: - ISSUE DATE: 14/03/16

High Volume Air Sampler Calibration Worksheet

Project Site :	Rojana Industriak Park Public Co., Ltd.	**Barometric Pressure (mm Hg) :**	755
Calibrate Location :	สถานีที่ A4 : วัดเวฬุวนาราม	**Temperature (°C) :**	28
Calibrate Date :	4-Nov-23	**High Volume ID :**	RYG_FS0176
CalibrationSheet No.:	C-041123-RYG_FS0176	**High Volume Model :**	TE-5170D
Calibrator ID:	RYG_FS0206	**High Volume S/N :**	4802
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.47433
Calibrator S/N :	1543	**Calibrator Intercept :**	-0.01503

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.0	0.9663	40	Slope : 56.6895
2	2.4	1.0571	44	Intercept : -15.1238
3	2.8	1.1406	50	Correlation Coefficient : 0.9980
4	3.2	1.2183	54	
5	3.8	1.3263	60	

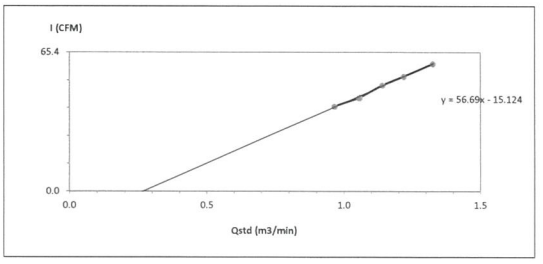

Calibrated by ชัชชัย

(Mr.Chatchai Sukpia)
Field Scientist(1)

Approved by :


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

FORM NO.: F 06-073 REVISION NO.: - ISSUE DATE: 14/03/16

High Volume Air Sampler Calibration Worksheet

Project Site :	Rojana Industriak Park Public Co., Ltd.	**Barometric Pressure (mm Hg) :**	755
Calibrate Location :	สถานีที่ A5 : ฟาร์มไก่พินิจ (ม.2 ต. คะเดียน(เดี่ย)	**Temperature (°C) :**	28
Calibrate Date :	4-Nov-23	**High Volume ID :**	RYG_FS0291
CalibrationSheet No.:	C-041123-RYG_FS0291	**High Volume Model :**	TE-5170D
Calibrator ID:	RYG_FS0206	**High Volume S/N :**	5333
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.47433
Calibrator S/N :	1543	**Calibrator Intercept :**	-0.01503

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.0	0.9663	40	Slope : 59.0486
2	2.4	1.0571	44	Intercept : -17.6121
3	2.8	1.1406	50	Correlation Coefficient : 0.9975
4	3.2	1.2183	54	
5	3.7	1.3089	60	

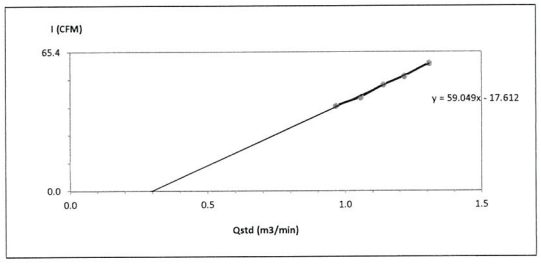

Calibrated by : ชัยธาชัย

(Mr.Chatchai Sukpia)
Field Scientist(1)

Approved by :

(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

FORM NO.: F 06-073 REVISION NO.: - ISSUE DATE: 14/03/16

RYG_EN0001

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel +66 2643 8361-6 , e-mail service.thailand@sartorius.com

NSC-TISI-TIS 17025
CALIBRATION 0426

SARTORIUS

REVIEW BY Thanita U.
APPROVED BY
NEXT CAL DATE 01/03/24

Certificate of Calibration

Model Number :	LA130S-F	Certificate No. :	23BCI0110
Description :	Analytical Balance	Issued Date :	Friday, March 03, 2023
Serial Number :	25409664	Reference No :	204833
ID No. :	RYG_EN0001		
Manufacturer :	Sartorius	Page No. :	1 Of 2

Customer Name : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated Place : ALS Laboratory Group (Thailand) Co., Ltd.(Balance Room)
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand

Calibrated By : Mr.Chonchai Inthana
Calibration Date : Wednesday, March 01, 2023

Calibration Procedure No. : This calibration was conducted by Using in-house calibration procedure number (WI-003) Based on UKAS LAB 14 : 2019

Metrological data :
Capacity : 150 g Readability : 0.0001 g

Ambients Conditions:
Temperature : 24.2 °C ± 5.0 °C
Humidity : 60.0 % RH ± 10.0 % RH
Pressure ± —

Reasons for calibration
☐ New Installation ☐ Service / Repaired ☑ Re-calibration/ Maintenance

Equipment Condition. ☑ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Cetificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.
This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd

Mr.chonchai Intrhana(Technical Manager)

STAMP

SOP FM 33 03 February 2022

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel +66 2643 8361-6 Fax: +66 2643-8367, e-mail service.thailand@sartorius.com

SARTORIUS

Certificate of Calibration

Model Number :	LA130S-F	Certificate No :	23BCI0110
Description :	Analytical Balance	Issued Date :	Friday, March 03, 2023
Serial Number :	25409664	Reference No :	204833
ID No. :	RYG_EN0001		
Manufacturer :	Sartorius	Page No. :	2 of 2

Calibration Results : Without Adjustment

Repeatability


The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	10.0000	100.0001
10 g	10.0000	100.0002
Tolerance	10.0001	100.0001
0.0001 g	10.0000	100.0000
	9.9999	100.0002
Nominal Value : (High Load)	10.0000	100.0001
100 g	10.0001	100.0001
Tolerance	10.0000	100.0001
0.0001 g	9.9999	100.0002
	9.9998	100.0001
Standard Deviation	0.00009	0.00006

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76)

Nominal value : 50 g
Tolerance *0.0004* g



	Difference
1	–
2	0.0000
3	-0.0001
4	0.0001
5	0.0000
6	-

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance *0.0002* g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00022
0.05	0.0500	0.0500	0.0000	0.00023
0.1	0.1000	0.1000	0.0000	0.00023
0.5	0.5000	0.5000	0.0000	0.00023
1	1.0000	1.0000	0.0000	0.00023
2	2.0000	2.0000	0.0000	0.00023
5	5.0000	5.0000	0.0000	0.00022
10	10.0000	10.0001	0.0001	0.00024
20	20.0000	20.0001	0.0001	0.00023
100	100.0000	100.0002	0.0002	0.00026


End of Report.

SOP FM 33 03 February 2022

High Volume Air Sampler Calibration Worksheet

Project Site :	Rojana Industriak Park Public Co., Ltd.	**Barometric Pressure (mm Hg) :**	755
Calibrate Location :	สถานีที่ A1 : มัสยิดนูร์อุมาลอมีน	**Temperature (°C) :**	28
Calibrate Date :	4-Nov-23	**High Volume ID :**	RYG_FS0184
CalibrationSheet No.:	C-041123-RYG_FS0184	**High Volume Model :**	TE-5009X
Calibrator ID:	RYG_FS0206	**High Volume S/N :**	4792
Calibrator Model :	TE-5028A	**Calibrator Slope :**	0.92345
Calibrator S/N :	1543	**Calibrator Intercept :**	-0.0095

Test No.	Delta H_2O (inch)	Qa (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.0	0.976	32	Slope : 39.7563
2	2.4	1.069	36	Intercept : -6.4840
3	2.8	1.154	40	Correlation Coefficient : 0.9982
4	3.4	1.270	44	
5	4.0	1.377	48	

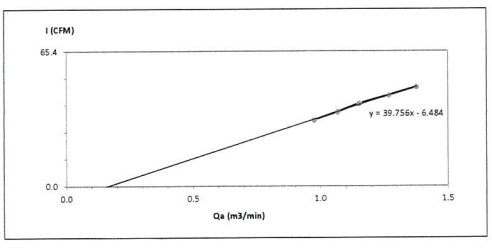

Calibrated by : ชัยธาชัย

(Mr.Chatchai Sukpia)
Field Scientist(1)

Approved by :


(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

FORM NO.: F 06-074 REVISION NO.: - ISSUE DATE: 14/03/16

High Volume Air Sampler Calibration Worksheet

Project Site :	Rojana Industriak Park Public Co., Ltd.	**Barometric Pressure (mm Hg) :**	755
Calibrate Location :	สถานีที่ A2 : วัดบ้านพวัน	**Temperature (°C) :**	28
Calibrate Date :	4-Nov-23	**High Volume ID :**	RYG_FS0185
CalibrationSheet No.:	C-041123-RYG_FS0185	**High Volume Model :**	TE-5009X
Calibrator ID:	RYG_FS0206	**High Volume S/N :**	4793
Calibrator Model :	TE-5028A	**Calibrator Slope :**	0.92345
Calibrator S/N :	1543	**Calibrator Intercept :**	-0.0095

Test No.	Delta H_2O (inch)	Qa (m^3/min)	I : Chart (CFM)	Linear Regression	
1	1.8	0.927	32	Slope :	38.3396
2	2.2	1.024	36	Intercept :	-3.2280
3	2.6	1.112	40	Correlation Coefficient :	0.9984
4	3.2	1.233	44		
5	3.8	1.342	48		

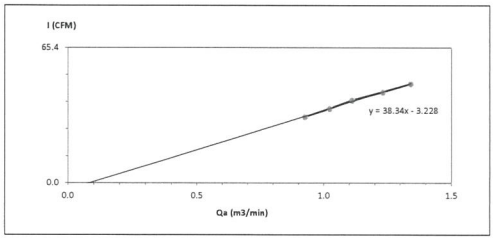

Calibrated by _____
(Mr.Chatchai Sukpia)
Field Scientist(1)


Approved by : _____
(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

FORM NO.: F 06-074 REVISION NO.: - ISSUE DATE: 14/03/16

High Volume Air Sampler Calibration Worksheet

Project Site :	Rojana Industriak Park Public Co., Ltd.	**Barometric Pressure (mm Hg) :**	755
Calibrate Location :	สถานีที่ A3 : วัดป่าสามัคคีธรรมาวาส	**Temperature (°C) :**	28
Calibrate Date :	4-Nov-23	**High Volume ID :**	RYG_FS0190
CalibrationSheet No.:	C-041123-RYG_FS0190	**High Volume Model :**	G1051
Calibrator ID:	RYG_FS0206	**High Volume S/N :**	1625
Calibrator Model :	TE-5028A	**Calibrator Slope :**	0.92345
Calibrator S/N :	1543	**Calibrator Intercept :**	-0.0095

Test No.	Delta H_2O (inch)	Qa (m^3/min)	I : Chart (CFM)	Linear Regression	
1	1.8	0.927	32	Slope :	34.8170
2	2.2	1.024	36	Intercept :	-0.0493
3	2.8	1.154	40	Correlation Coefficient :	0.9991
4	3.4	1.270	44		
5	4.0	1.377	48		

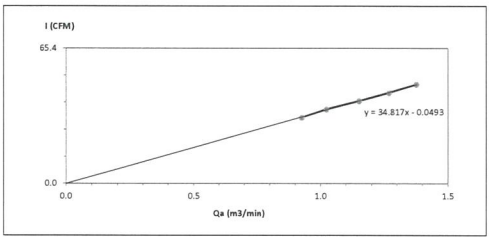

Calibrated by _____
(Mr.Chatchai Sukpia)
Field Scientist(1)


Approved by : _____
(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

FORM NO.: F 06-074 REVISION NO.: - ISSUE DATE: 14/03/16

High Volume Air Sampler Calibration Worksheet

Project Site :	Rojana Industriak Park Public Co., Ltd.	**Barometric Pressure (mm Hg) :**	755
Calibrate Location :	สถานีที่ A4 : วัดเจริญนาราม	**Temperature (°C) :**	28
Calibrate Date :	4-Nov-23	**High Volume ID :**	RYG_FS0186
CalibrationSheet No.:	C-041123-RYG_FS0186	**High Volume Model :**	TE-5009X
Calibrator ID:	RYG_FS0206	**High Volume S/N :**	4794
Calibrator Model :	TE-5028A	**Calibrator Slope :**	0.92345
Calibrator S/N :	1543	**Calibrator Intercept :**	-0.0095

Test No.	Delta H_2O (inch)	Qa (m^3/min)	I : Chart (CFM)	Linear Regression	
1	1.8	0.927	32	Slope :	36.1335
2	2.4	1.069	36	Intercept :	-1.8896
3	2.8	1.154	40	Correlation Coefficient :	0.9977
4	3.4	1.270	44		
5	4.0	1.377	48		

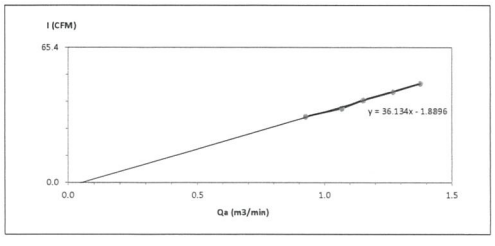

Calibrated by _____
(Mr.Chatchai Sukpia)
Field Scientist(1)


Approved by : _____
(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

FORM NO.: F 06-074 REVISION NO.: - ISSUE DATE: 14/03/16

High Volume Air Sampler Calibration Worksheet

Project Site :	Rojana Industriak Park Public Co., Ltd.	**Barometric Pressure (mm Hg) :**	755
Calibrate Location :	สถานีที่ A5 : ฟาร์มไก่พิจิจ (ม.2 ต. คะเคียนเตี้ย)	**Temperature (°C) :**	28
Calibrate Date :	4-Nov-23	**High Volume ID :**	RYG_FS0189
CalibrationSheet No.:	C-041123-RYG_FS0189	**High Volume Model :**	TE-5009X
Calibrator ID:	RYG_FS0206	**High Volume S/N :**	4797
Calibrator Model :	TE-5028A	**Calibrator Slope :**	0.92345
Calibrator S/N :	1543	**Calibrator Intercept :**	-0.0095

Test No.	Delta H_2O (inch)	Qa (m^3/min)	I : Chart (CFM)	Linear Regression	
1	2.0	0.976	32	Slope :	39.7415
2	2.4	1.069	36	Intercept :	-6.7859
3	3.0	1.194	40	Correlation Coefficient :	0.9980
4	3.4	1.270	44		
5	4.0	1.377	48		

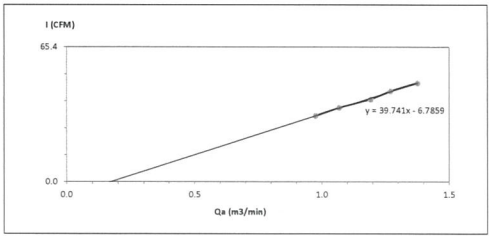

Calibrated by _____
(Mr.Chatchai Sukpia)
Field Scientist(1)


Approved by : _____
(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

FORM NO.: F 06-074 REVISION NO.: - ISSUE DATE: 14/03/16

MULTIPOINT CALIBRATION REPORT

Calibration Date	1-Jul-23	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	AWXG87CR	Equipment ID	RYG_FS0453
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.60	-0.40	-0.40	101.40	1.40	1.40
2	200.00	198.60	-1.40	-0.70	199.80	-0.20	-0.10
3	300.00	299.00	-1.00	-0.33	298.50	-1.50	-0.50
4	400.00	402.10	2.10	0.53	401.20	1.20	0.30
AVERAGE (%)				-0.16			0.24

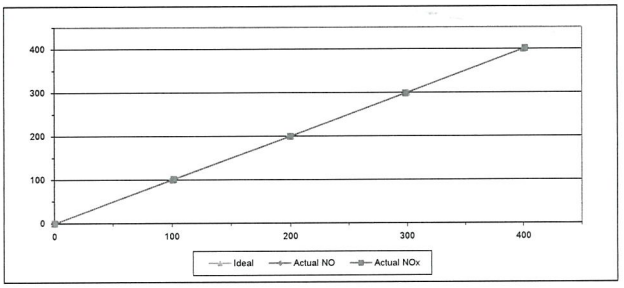

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	1-Jul-23	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	7AV89544	Equipment ID	RYG_FS0272
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.05	0.05	0.05	0.10	0.10	0.10
1	100.00	99.10	-0.90	-0.90	100.10	0.10	0.10
2	200.00	198.60	-1.40	-0.70	199.00	-1.00	-0.50
3	300.00	298.70	-1.30	-0.43	300.50	0.50	0.17
4	400.00	398.00	-2.00	-0.50	398.70	-1.30	-0.33
AVERAGE (%)				-0.50			-0.09

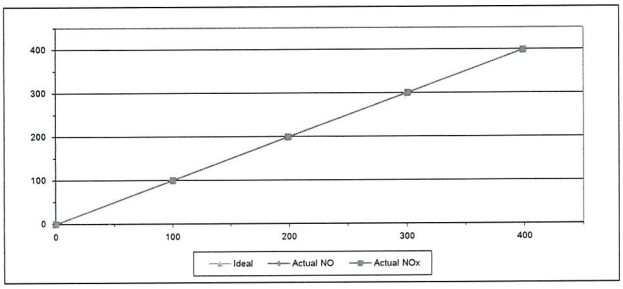

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	1-Jul-23	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	R06K0177	Equipment ID	RYG_FS0463
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	98.80	-1.20	-1.20	101.10	1.10	1.10
2	200.00	201.80	1.80	0.90	201.50	1.50	0.75
3	300.00	299.40	-0.60	-0.20	302.60	2.60	0.87
4	400.00	398.10	-1.90	-0.47	401.90	1.90	0.47
AVERAGE (%)				-0.18			0.66

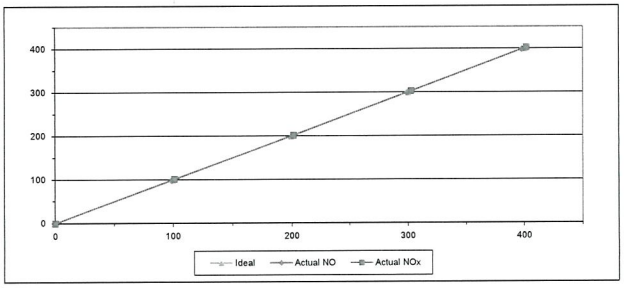

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	1-Jul-23	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	NV0ER3YH	Equipment ID	RYG_FS0459
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.05	0.05	0.05	0.10	0.10	0.10
1	100.00	99.50	-0.50	-0.50	101.80	1.80	1.80
2	200.00	198.70	-1.30	-0.65	199.70	-0.30	-0.15
3	300.00	301.10	1.10	0.37	301.50	1.50	0.50
4	400.00	401.30	1.30	0.33	398.90	-1.10	-0.28
AVERAGE (%)				-0.08			0.39

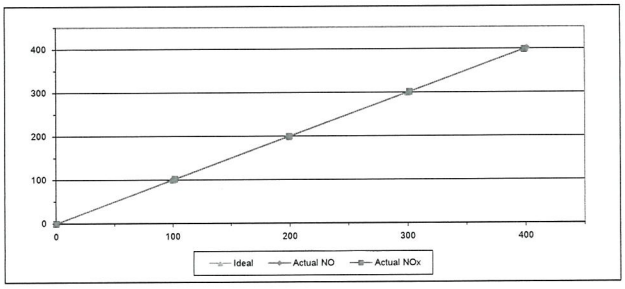

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	1-Jul-23	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	T95HWM41	Equipment ID	RYG_FS0461
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	98.70	-1.30	-1.30	100.10	0.10	0.10
2	200.00	201.00	1.00	0.50	201.40	1.40	0.70
3	300.00	298.30	-1.70	-0.57	302.10	2.10	0.70
4	400.00	398.40	-1.60	-0.40	403.50	3.50	0.88
AVERAGE (%)				-0.33			0.50

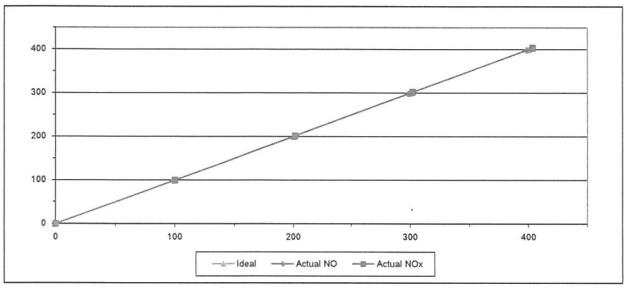

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	2-Jul-23	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	90U0XJ31	Equipment ID	RYG_FS0452
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.60	-1.40	-1.40
2	200.00	198.00	-2.00	-1.00
3	300.00	298.10	-1.90	-0.63
4	400.00	398.20	-1.80	-0.45
AVERAGE (%)				-0.68

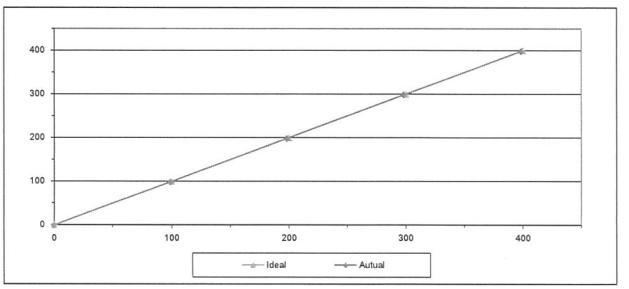

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	2-Jul-23	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	1092NYKM	Equipment ID	RYG_FS0271
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	99.50	-0.50	-0.50
2	200.00	198.20	-1.80	-0.90
3	300.00	297.60	-2.40	-0.80
4	400.00	398.00	-2.00	-0.50
AVERAGE (%)				-0.52

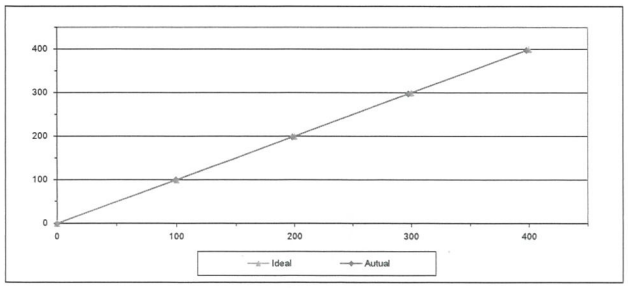

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	2-Jul-23	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	XL29Y85B	Equipment ID	RYG_FS0462
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	99.10	-0.90	-0.90
2	200.00	198.10	-1.90	-0.95
3	300.00	297.90	-2.10	-0.70
4	400.00	403.20	3.20	0.80
AVERAGE (%)				-0.33

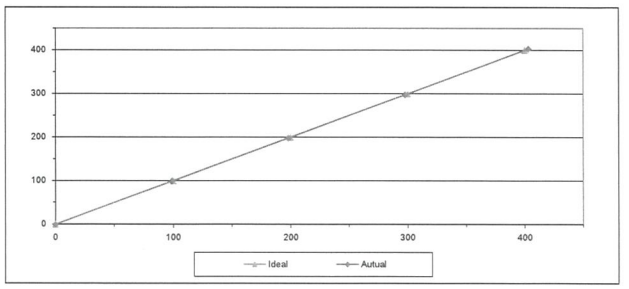

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	2-Jul-23	**Equipment Name**	SO2 Analyzer
Manufacturer	HORIBA	**Model**	APSA-370
Serial No.	PAUY0T7A	**Equipment ID**	RYG_FS0458
Calibrator Manufacturer	Teledyne API	**Model**	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	**Cylinder No.**	GN0027222
Cylinder Pressure (psi)	1800	**Certified By**	Airgas Inc.
Certified Date	9-Feb-22	**Expired Date**	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.90	-1.10	-1.10
2	200.00	201.10	1.10	0.55
3	300.00	302.30	2.30	0.77
4	400.00	398.60	-1.40	-0.35
AVERAGE (%)				-0.01

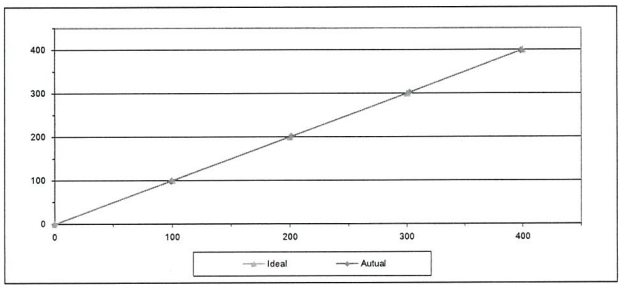

Calibrated By

(Mr.Jirawut Sakam)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager


ALS Laboratory Group

FORM NO.: F 06-056 REVISION NO.: - ISSUE DATE: 02/04/12

MULTIPOINT CALIBRATION REPORT

Calibration Date	2-Jul-23	**Equipment Name**	SO2 Analyzer
Manufacturer	HORIBA	**Model**	APSA-370
Serial No.	VABF9LSH	**Equipment ID**	RYG_FS0460
Calibrator Manufacturer	Teledyne API	**Model**	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	**Cylinder No.**	GN0027222
Cylinder Pressure (psi)	1800	**Certified By**	Airgas Inc.
Certified Date	9-Feb-22	**Expired Date**	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.70	-1.30	-1.30
2	200.00	197.80	-2.20	-1.10
3	300.00	296.50	-3.50	-1.17
4	400.00	398.30	-1.70	-0.42
AVERAGE (%)				-0.78

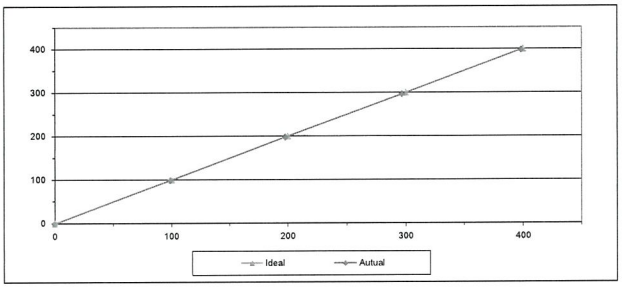

Calibrated By

(Mr.Jirawut Sakam)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

ALS Laboratory Group

FORM NO.: F 06-056 REVISION NO.: - ISSUE DATE: 02/04/12

JNAC
JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 2 2/1, Rd. Watthapra, Bangkoknoi,
Bangkok 10700 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Website: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department

REVIEW BY Nopakan P.
APPROVED BY
ISSUE DATE 19/7/14

Certificate Number
CL-009-66

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM	: Cup anemometer	
MANUFACTURER	: Novalynx	
MODEL/TYPE	: Sensor: WS-02E Data logger: 110-WS-16N	
SERIAL NUMBER	: Sensor: - Data logger: 1159	
ID NUMBER	: RYG_FS0081	
CONDITION AS-RECEIVED	: Used item	
CUSTOMER	: ALS laboratory group (Thailand) co., ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.	
RECEIVED DATE	: 16 Jan 2023	
MEASUREMENT DATE	: 18 Jan 2023	
ISSUE DATE	: 20 Jan 2023	
ENVIRONMENTAL CONDITIONS:		
Ambient condition in the laboratory are as follow:		
Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa
PLACE OF CALIBRATION	: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.	
CALIBRATION CONDITIONS	: Wind tunnel cross-section area[1] 900 cm^2 Win direction frontal area[2] 100 cm^2 Diameter of mounting pipe[3] - mm Blockage ratio of test object[4] 0.111 [-]	
Preconditioning	: 24 hours at ambient conditions.	
Measurement Condition	: The average values during measurement are (23.5) °C, (52.2) %RH and (1014.5) hPa.	

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The cup anemometer was calibrated against Standard air velocity transducer model: 8455-L2 and pitot tube with precision differential pressure meter model: DPM2500 in an close test section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0052-21 and MW-0066-22.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☑ Mr. Sorawit Thachalard
☐ Miss Jittraporn Tantsonphol

Approved signatory: Mr. Parinya Booncharoen
Calibration Department Manager

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CL-009-66


MEASUREMENT RESULTS [5]

The cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle, UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below

v_{std} [4] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{uuc} [5] (m/s)	Error (m/s)	U (k=2) (m/s)
0.981	23.56	23.45	0.8	-0.2	0.15
2.030	23.40	23.45	1.9	-0.2	0.16
3.049	23.50	23.45	2.9	-0.2	0.17
4.129	23.50	23.45	3.9	-0.3	0 20
5.01	23.50	23.45	4.8	-0.2	0.17
5.97	23.54	23.45	5.7	-0.3	0.17
7.05	23.42	23.45	6.8	-0.3	0.18
8.18	23.50	23.45	7.9	-0.3	0.19
9.10	23.34	23.45	8.8	-0.3	0.19
10.10	23.40	23.45	9.7	-0.4	0.19
11.14	23.40	23.45	10.8	-0.4	0.20
12.13	23.32	23.45	11.8	-0.4	0.20
13.20	23.10	23.45	12.9	-0.3	0.20
14.35	23.36	23.45	13.9	-0.4	0.22
15.24	23.22	23.45	14.8	-0.4	0.21
16.30	23.40	23.45	15.8	-0.5	0.22

Remark:
[1] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place
[4] Velocity of standard
[5] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

Jiranatee Associates Co., Ltd.

JNAC
JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthana, Bangkokyai,
Bangkok 10600,(Thailand)
Tel: +66(0)8280812
Mobile: +66(0)3999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

Certificate Number
CL-009-66

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM	: Wind Direction Sensor
MANUFACTURER	: Novalynx
MODEL/TYPE	: Sensor: WS-02E Data logger: 110-WS-16N
SERIAL NUMBER	: Sensor: - Data logger: 1159
ID NUMBER	: RYG_FS0081
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (Thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 16 Jan 2023
MEASUREMENT DATE	: 19 Jan 2023
ISSUE DATE	: 19 Jan 2023

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION

: Wind tunnel cross-section area[1]	900	cm^2
Win direction frontal area[2]	129	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage ratio of test object[4]	0.143	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.8)°C, (47.3) %RH and (1014.8) hPa.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The wind direction sensor was calibrated against Standard Rotary Encoder, model AX4009T5-DM04-P3-S-U0 in an close test section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: DA-0043-22

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☑ Mr. Sorawit Thachalad
☐ Miss Jittrapron Lertsimphol

Approved signatory: 25/Jan/23
Mr. Parinya Booncharoen
Calibration Department Manager

Remarks:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Jiranatee Associates Co., Ltd.

Certificate Number
CL-009-66

MEASUREMENT RESULTS[3]

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed	D'_{std}	D'_{suc}	Error	$U_{(k=2)}$
m/s	Degree (°)	Degree (°)	Degree (°)	Degree (°)
5.01	0.000	0	0	0.58
	45.000	43	-3	0.76
	90.000	89	-2	0.76
	135.000	134	-1	0.74
	180.000	177	-3	0.74
	225.000	229	4	0.58
	270.000	273	3	0.68
	315.000	317	2	0.74

Remark:
[1] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place
[2] Direction of standard
[3] Direction of Unit Under Calibration

End of Certificate of Calibration

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACC23005
Pages : 1 of 3

Calibration Certificate

Equipment :	SOUND CALIBRATOR
Manufacturer :	RION
Model :	NC-75
Serial No.:	35002736
ID No.:	RYG_FS0496
Condition As Found :	GOOD
Customer :	ALS LABORATORY GROUP (THAILAND) CO., LTD. 104 PHATTHANAKAN 40, PHATTHANAKAN ROAD, KHWAENG PHATTHANAKAN, KHET SUAN LUANG, BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Nathakorn P.
APPROVED BY
NEXT CAL. DATE 17/1/24

Received Date :	06 JANUARY 2023
Calibration Date :	17 JANUARY 2023
Date of Issue :	19 JANUARY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard. may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

SITHIPORN associates SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACC23005
Job No. : VC66AC0024
Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :
This equipment was calibrated by based on IEC-60942-2003 Standard.
The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :
1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	33461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23
Audio Analyzer	AVR-3360A	V744B6069	EF-0010-22	07-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 National Institute of Metrology (Thailand).
   3.2 Thailand Institute of Scientific and Technological Research (TISTR).

T. Petch

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit (dB)
94	93.98	-0.02	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Tolerance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Tolerance limit (%)
0.35	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025 CALIBRATION 0304

Cert. No. : ACL23263
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01122567 / 143473 / 22605
ID No.: RYG_FS0016

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

REVIEW BY Nathakorn P.
APPROVED BY
NEXT CAL. DATE 1/9/24

Received Date : 23 AUGUST 2023
Calibration Date : 01 SEPTEMBER 2023
Date of Issue : 04 SEPTEMBER 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Calibration Procedure : CP-AC-01

Calibration Method :
This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :
1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 National Institute of Metrology (Thailand).
   3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.0
C - weight	18.3
Flat	24.2

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.4	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-2.0	-1.9	-1.9	±5.0

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.1	-0.3	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated	Acceptance
Positive one-half cycle	Negative one-half cycle	Value (dB)	Limits (dB)
89.7	89.5	-0.2	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a level of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com

NSC-TISI-TIS 17025 CALIBRATION 0394

Cert. No. : ACL23008
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01122578 / 143486 / 22620
ID No.: RYG_FS0017

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

REVIEW BY Nathakorn P
APPROVED BY
NEXT CAL. DATE 3/1/24

Received Date : 14 DECEMBER 2022
Calibration Date : 03-05 JANUARY 2023
Date of Issue : 06 JANUARY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Calibration Procedure : CP-AC-01

Calibration Method :
This equipment was calibraied by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :
1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	34461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	34461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 National Institute of Metrology (Thailand).
   3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
17.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	16.6
C - weight	22.6
Flat	28.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.6	0.7	0.7	±5.0

SITHIPORN associates SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23008
Job No. : VC66AC0021
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	-0.1	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

SITHIPORN associates SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23008
Job No. : VC66AC0021
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	132.9	-0.1	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.0	0.0	± 1.1

QF-TS12-04-04-020664

SITHIPORN associates SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23008
Job No. : VC66AC0021
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

QF-TS12-04-04-020664

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01122579 / 172172 / 74022
ID No.: RYG_FS0018

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

REVIEW BY
APPROVED BY
NEXT CAL DATE 3/1/2024

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 14 DECEMBER 2022
Calibration Date : 03-05 JANUARY 2023
Date of Issue : 06 JANUARY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : (Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Calibration Procedure : CP-AC-01

Calibration Method :
This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :
1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 National Institute of Metrology (Thailand).
   3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.0
C - weight	20.1
Flat	26.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.1	0.1	0.1	±5.0

SITHIPORN associates SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

Continuation of Calibration Certificate

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.1	±2.0
4000	0.0	0.1	0.1	±3.0
8000	0.1	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

SITHIPORN associates SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

Continuation of Calibration Certificate

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.8	-0.2	± 1.1

SITHIPORN associates SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

Continuation of Calibration Certificate

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025 CALIBRATION 0394

Cert. No. : ACL23046
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01122607 / 145554 / 34373
ID No.: RYG_FS0019

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

REVIEWED BY Monkorn P
APPROVED BY
NEXT CAL DATE 13/1/24

Received Date : 06 JANUARY 2023
Calibration Date : 13-18 JANUARY 2023
Date of Issue : 19 JANUARY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : (Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full. except with the prior written approval of the head of Calibration Laboratory.

Calibration Procedure : CP-AC-01

Calibration Method :
This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :
1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	34461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	34461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAJ	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 National Institute of Metrology (Thailand).
   3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.7

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	9.9
C - weight	16.5
Flat	22.4

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.6	0.6	0.6	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	-2.3	-2.3	-2.3	±5.0

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.8	-0.2	± 1.1

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.1	0.1	-
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.7	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025 CALIBRATION 0394

Cert. No. : ACL23047
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01222716 / 143832 / 22763
ID No.: RYG_FS0020

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

CHECKED BY Nathakorn P
APPROVED BY
NEXT CAL DATE 13/1/24

Received Date : 06 JANUARY 2023
Calibration Date : 13-18 JANUARY 2023
Date of Issue : 19 JANUARY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : (Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Calibration Procedure : CP-AC-01

Calibration Method :
This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :
1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 National Institute of Metrology (Thailand).
   3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.95)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.6
C - weight	17.9
Flat	23.8

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.5	0.5	0.5	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	-1.3	-1.2	-1.2	±5.0

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.1	0.0	±3.0
8000	0.1	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
One	136.4	135.4	-1.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

SITHIPORN associates

SITHIPORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23047
Job No. : VC66AC0024
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighing	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

DKSH

Certificate of Calibration

HSC-TISI-TIS 17025 Calibration 0997

Equipment:	SPECTROPHOTOMETER	Certificate No.:	C06230441
Model:	DR6000	Issued Date:	19 September 2023
Serial No. (or ID.):	1627845 (RYG_EN0037)	Job No.:	WO-00005382
Manufacturer:	HACH	Page:	1 of 3
Condition:	In Condition		

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

REVIEW BY N. Bamrut
APPROVED BY D.
NEXT CAL. DATE 18/3/25

Environment Condition: Temperature 23.9 °C ± 0.2
Humidity 65.3 %RH ± 1.4 %RH

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) (Wet Chemistry)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By: Mr.Nattapat Rungrueang
Calibration Date: 18 September 2023
The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04
Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.
The standard for Wavelength Certificate No. 111583 and 111584
The standard for Photometric Certificate No. 9114984 and 111588
The standard for Stray light Certificate No. 111586 and 111585
The standard for Spectral resolution Certificate No. 111587

(Mr. Nattapat Rungrueang)
Person in charge

(Mr. Nitinun Srihawan)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2633 ถนนสุขุมวิท แขวงพระโขนง เขตพระโขนง กรุงเทพมหานคร 10260
2633 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

DKSH

Calibration Results:

Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.3	0.31	0.13
536.66	536.6	0.06	0.13
637.98	638.3	-0.32	0.13
748.48	748.7	-0.22	0.13
807.03	807.4	-0.37	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.2930	0.289	0.0040	0.0045
	0.5168	0.519	-0.0022	0.0045
	1.0298	1.029	0.0008	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2867	0.283	0.0037	0.0045
	0.5073	0.509	-0.0017	0.0045
	1.0083	1.007	0.0013	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2516	0.250	0.0016	0.0045
	0.4595	0.462	-0.0025	0.0045
	0.9334	0.933	0.0004	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2461	0.245	0.0011	0.0045
	0.4652	0.466	-0.0008	0.0045
	0.9468	0.946	0.0008	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2594	0.259	0.0004	0.0045
	0.5040	0.505	-0.0010	0.0045
	1.0032	1.002	0.0012	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2579	0.257	0.0009	0.0045
	0.4971	0.497	0.0001	0.0045
	0.9720	0.971	0.0010	0.0045

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2633 ถนนสุขุมวิท แขวงพระโขนง เขตพระโขนง กรุงเทพมหานคร 10260
2633 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

DKSH

Calibration Results:

Without Adjustment

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7355	0.737	-0.0015	0.0080
257 nm	0.0000	0.000	0.0000	0.0080
	0.8574	0.857	0.0004	0.0080
313 nm	0.0000	0.000	0.0000	0.0080
	0.2864	0.290	-0.0036	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6374	0.637	0.0004	0.0080

Stray light *

Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
260.62 +/- 0.11 nm	260.6	1.3	1.886
391.44 +/- 0.11 nm	391.4	1.3	1.886

Spectral Resolution *

Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength (nm)	268.66	266.69	1.38	2.00
UUC: Wavelength (nm)	268.2	266.1		
Std Absorbance (A)	0.4566	0.2780		
Absorbance (A)	0.413	0.300		

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2633 ถนนสุขุมวิท แขวงพระโขนง เขตพระโขนง กรุงเทพมหานคร 10260
2633 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

DKSH

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00005382

ชนิดเครื่องมือ: SPECTROPHOTOMETER รุ่น: DR6000 หมายเลขเครื่อง: 1627845

ตรวจสอบ (รับ) 18 Sep 2023 ปกติ	ตรวจสอบ (รับ) 18 Sep 2023 ไม่ปกติ	รายการตรวจเช็ค	ตรวจสอบ (ส่ง) 18 Sep 2023 ปกติ	ตรวจสอบ (ส่ง) 18 Sep 2023 ไม่ปกติ	หมายเหตุ
		General			
☑	☐	1. ความสมบูรณ์เครื่อง	☑	☐	
☑	☐	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	☑	☐	
☑	☐	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swicth)	☑	☐	
☑	☐	4. ปุ่มกด (Keypad)	☑	☐	
☑	☐	5. หน้าจอ (Display, Screen Contrast)	☑	☐	
		Spectrophotometer			
☐	☐	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	☐	☐	
☐	☐	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	☐	☐	
☑	☐	8. ความยาวคลื่น (Wavelength Check)	☑	☐	*
☑	☐	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	☑	☐	9.2 Hours
☑	☐	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	☑	☐	741.5 Hours
☑	☐	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	☑	☐	
		pH Meter and Conductivity Meter			
☐	☐	12. อิเล็คโทรด (Electrode and Connection Cable)	☐	☐	
☐	☐	13. ระดับสารละลายใน Electrode (Level KCl)	☐	☐	
☐	☐	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	☐	☐	
☐	☐	15. ขาจับอิเล็คโทรด (Stand)	☐	☐	
		Turbidimeter			
☐	☐	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	☐	☐	
☐	☐	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่เกิน 3.0)	☐	☐	
		Automatic titrator			
☐	☐	18. สภาพ Piston Burettes	☐	☐	
☐	☐	19. Function Rinsing and Dosing	☐	☐	
☐	☐	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	☐	☐	

เพิ่มเติม/ข้อแนะนำ : *656.1nm=656.1nm

*486.0nm=485.5nm

Mr.Nattapat Rungrueang

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-th/en/

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL 0-2717-3000-29 FAX 0-2719-9484

ISO/IEC 17025 NSC-TISI-TIST1925 CALIBRATION 0008

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	SevenCompact S220
Serial No. :	C104059460
ID No. :	RYG_EN0183
Condition As-Received:	Used Item
Received Date :	24 February 2023
Calibration Date :	27 February 2023
Reference :	2302-0886DSC-2
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer
Calibrated by :	Walalak Sirithean
Approved by :	Approved Signatory

REVIEW BY N.Banit
APPROVED BY
NEXT CAL. DATE 27/2/24

( ) Malee Butkruea
(✓) Saithip Meangmai
( ) Warakorn Lerngagtrakul

Issue Date : 28 February 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services

A 0051538

Condition of this calibration result

1. Reference Standard Instrument : -

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	22E2769	24 Aug 2023
2) Ref. Standard Thermometer	4982054	110RC044	22I1306	27 Oct 2023

This certification is traceable to the International System of Unit maintained at:-
- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	826588	09 July 2024
pH 6.987	CPA chem	826589	09 July 2023
pH 10.010	CPA chem	863835	28 Dec 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	*k*
pH Meter	4.000	177.48	177.4	4.000	0.058	2.00
S/N.: C104059460	7.000	0.00	-0.1	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Saithip

a 1149925

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor *k*
pH Electrode	4.008	4.008	179.1	0.0046	2.00
S/N.: 1453404	6.987	6.988	4.7	0.0084	2.00
	10.010	10.013	-172.4	0.0069	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;
- Model : InLabExpert Pro-ISM
- Serial No. : 1453404

Dimension of probe;
- Length : 120 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor *k*
25.0	25.001	24.8	-0.201	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Saithip

a 1149924

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

NSC-TISI-TIS17025 CALIBRATION 0005

Certificate of Calibration

Certificate No. : 23E753
Page : 1 of 2

Equipment :	pH Meter
Manufacturer:	Mettler Toledo
Model :	SevenCompact S220
Serial No.:	C104059460
ID No.:	RYG_EN0183
Condition As-Received:	Used Item
Received Date:	24 February 2023
Calibration Date:	28 February 2023
Reference:	2302-0886DSC
Ambient Temperature:	(23 ± 2) °C
Relative Humidity:	(50 ± 10) %

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3. Equipment Calibration and Testing Services.

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Procedure used: Calibration were conducted using In-house calibration Prpcedure CP-E17 According to direct measurement method with Multi-Product Calibrator.

Condition of this result of calibration

1.Reference standards instuments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Multi-Product Calibrator	5500A	6440007	22E1670	18 May 2023

2.This result of calibration was made on requested at the point specified by customer.
3.The certificate is valid only to the item calibrated on date and place of calibration.
4.This Certification is traceable to the International System of Unit maintained at:-
-National Institute of Metrology Thailand (NIMT)

Calibrated by : Wutchareeporn Wongchutikrane **Approved Signatory :**
Issue Date : 02 March 2023
[ ] Phalinee Praboalpai
[✓] Nuntawat Khamchai
[ ] Pornthippa Tameyakul

B 0309672

Cert. No.: 23E753
Page.: 2 of 2

Result of calibration :- (*) Without adjustment ( ) After adjustment

Function: DC voltage measuremer Range: 2000 mV

Standard Value (mV)	UUC* Reading (mV)	Error (mV)	Uncertainty (± µV)
-200.0000	-200.0	0.0	72
-150.0000	-150.0	0.0	69
-100.0000	-100.0	0.0	65
-50.0000	-50.0	0.0	62
0.0000	0.0	0.0	58
50.0000	50.0	0.0	62
100.0000	99.9	-0.1	65
150.0000	149.9	-0.1	69
200.0000	199.9	-0.1	72

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*=2, providing a level of confidence of approximately 95 %

UUC* = Unit Under Calibration.

-o0o-

a 1150477

SCG

Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3. T.Banpa, A.Kaengkhoi Saraburi 18110, Thailand.
Saraburi Tel. +66 3627 3096 Fax. +66 3627 3100
Bangkok Tel. +668 9205 6851 , +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.com

NSC-TISI-TIS 17025 CALIBRATION 0244

Certificate No. T230116 Page 1 of 4

Certificate of Calibration

Equipment	:	Chamber (Cooling Room)
Manufacturer	:	MODULAR
Model	:	IREVCOHCOO
Serial No.	:	C00351459
Customer Code	:	RYG_EN0184
ID No.	:	T1939A5
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
		616/10 Moo 5 T.Maenam Khu,
		A.Pluakdaeng, Rayong 21140
Customer Location	:	Laboratory
Date of Receipt	:	23 January 2023
Calibrated By	:	Atiphong Rongrat (Technician)
Approved By	:	Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	07 FEB 2023

REVIEW BY ..
APPROVED BY ..
NEXT CAL DATE 28/07/24

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-T-14118 31-08-64

SCG

Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3. T.Banpa, A.Kaengkhoi. Saraburi 18110, Thailand.

NSC-TISI-TIS 17025 CALIBRATION 0244

Certificate No. T230116 Page 2 of 4

Calibration Report

Equipment	:	**Chamber (Cooling Room)**
Date of Calibration	:	**25 January 2023**
Environment	:	**Temperature : 23.4-24.9 °C**
		Line Voltage : 221.4-230.2 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. Thisequipment was calibrated by insert 16 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN141-TN150	T222123	5 October 2023
TC	TYPE T	TN151-TN160	T222123	5 October 2023
DATA LOGGER	34970A	T150	T222123	5 October 2023


3. This certificate is traceable to :
National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
Equipment Description :
Time Constant 1 Hour - Minute At 3 °C
Fresh Air Damper [ ] Open [ ] Min [ ] Medium [ ] Max
[ ] Close
[X] Not Available
5. Adjustment :
(X) without adjustment ( ) after adjustment

Approved By.

FM-T-15117 15-05-63

Certificate No. T230116 Page 3 of 4

Calibration Report



C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	= TN141	12F	= TN152
2A	= TN142	13A	= TN153
3A	= TN143	14A	= TN154
4F	= TN144	15F	= TN155
5A	= TN145	16E	= TN156
6A	= TN146		
7F	= TN147		
8F	= TN148		
9A	= TN149		
10A	= TN150		
11F	= TN151		

Approved By.

Certificate No. T230116 Page 4 of 4

Calibration Report

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)											
	TN141	TN142	TN143	TN144	TN145	TN146	TN147	TN148	TN149	TN150	TN151	TN152
3.0	3.03	3.16	3.15	3.19	3.45	3.47	3.21	3.35	3.54	3.45	3.24	3.34
	TN153	TN154	TN155	TN156								
	3.28	3.22	3.28	3.21								

Chamber (Cooling Room)			Temperature Distribution			
Setting (°C)	Reading (°C)		Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor *k*
	Min , Max	Average				
3.0	2.8 , 4.1	3.5	1.20	1.20	1.90	2.07

The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By.

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 23TW168
Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000-115V
Serial No. :	15E102796
ID No. :	RYG_EN0032
Received Date :	21 July 2023
Test Date :	24 July 2023
Reference :	2307-0713DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walailak Sirithean
Approved by :	Approved Signatory

REVIEW BY N.Bamin
APPROVED BY
NEXT CAL. DATE 24/07/25

( ) Malee Butkruea
(✓) Saithip Meangmai
( ) Warakorn Lerngagtrakul

Issue Date : 26 July 2023

B 0320211

Cert.No.: 23TW168
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center,Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1) Burette	-	130BU10	23CG1172	22 Mar 2025
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 15E100464

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.17	0.0055

This report was certified only for the instrument we tested.It is allowable to use for study the system efficiency,The environmental impact control and present to organization it may concerned Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full,without written approval of the laboratory

-o0o-

a 1172155

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 29 FAX. 0-2719-9484

Cert. No.: 23LM125
Page.: 1 of 2

Certificate of Calibration

Equipment :	DO Meter with Sensor
Manufacturer :	YSI
Model :	5000-115V
Serial No. :	15E102796
ID No. :	RYG_EN0032
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng, Rayong 21140 Thailand
Location :	TPA On Site Calibration Laboratory
Received Order :	25 July 2023
Calibrated Date :	27 July 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V
Calibrated by :	Preecha Hiahib
Approved by :	Approved Signatory

( ) Pornthippa Tameyakul
( ) Malee Butkruea
(✓) Suwit Imjai

Issue Date : 31 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services

A 0053616

Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2307-0713DSC-2

Cert. No.: 23LM125
Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	22I1285	TPA	21 Oct 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor. S/N.: 1228475367

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor *k*
20.00	100	20.011	19.91	-0.101	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

a 1159515

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 29 FAX. 0-2719-9484

Cert. No.: 23TM962
Page : 1 of 3

Certificate of Calibration

Equipment :	Low Temp. Incubator
Manufacturer :	Memmert
Model :	IPP750
Serial No. :	V818.0084
ID No. :	RYG_EN0154
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng, Rayong 21140 Thailand
Location :	BOD Room
Received Order :	29 May 2023
Calibration Date :	29 May 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Man Pattanapongpaiboon
Approved by :	Approved Signatory

REVIEW BY N.Bamrat
APPROVED BY
NEXT CAL. DATE 29/11/24

( ) Pornthippa Tameyakul
( ) Malee Butkruea
(✓) Suwit Imjai

Issue Date : 7 June 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services

A 0054967

Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2305-0898OC-2

Cert. No.: 23TM962
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration


1. Reference standard instrument.-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY57013711	22LM93	02 Jul 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	23	23
REL.Humid. (%)	54	56
AC Supply (Volt)	223	222



Position :	Ref. Std. ID No.:
1	18-18RTD-01
2	18-18RTD-02
3	18-18RTD-03
4	18-18RTD-04
5	18-18RTD-05
6	18-18RTD-10
7	18-18RTD-07
8	22-18RTD-08
9 (ref.)	18-18RTD-09

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.60	m
W =	1.0	m
H =	1.2	m
Capacity =	0.75	m³

a 1165130

Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2305-0898OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 23TM962
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
20.0	20.0	20.0	0.019	0.72	1.0	2

Calibration Point	Measured Temperature (°C) Position									Uncertainty
(°C)	1	2	3	4	5	6	7	8	9 (ref.)	(±°C)
20.0	19.547	19.780	19.487	19.529	19.408	20.139	20.112	20.406	20.116	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

a 1165129

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

NSC-TIBI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Certificate No. : 23T1769
Page : 1 of 2

Equipment : Digital Thermometer With Sensor
Manufacturer: Testo
Model : 106
Serial No.: 31282167/504
ID No.: RYG_FS0468
Condition As-Received: Used Item
Received Date: 04 October 2023
Calibration Date: 10 October 2023 to 11 October 2023
Reference: 2310-0110DSC
Ambient Temperature: (25 ± 3) °C
Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3 :Equipment Calibration and Testing Services

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand

Procedure used: Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Black Stack Thermometer	1560	8C454	23I600	30 May 2024
2) PRT Scanner Module	2562	A01303	23I600	30 May 2024
3) Industrial Platinum Resistance Thermometer	5627-12	571971	23I600	30 May 2024

2.The certificate is valid only to the item calibrated on date and place of calibration.
3.This Certification is traceable to the International System of Unit maintained through:-
-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

REVIEW BY Pitthaya Th.
APPROVED BY Supt S.
NEXT CAL. DATE 10/10/24

Calibrated by : Wasinee Sawatdee
Issue Date : 12 October 2023
Approved Signatory :
[ ] Phalinee Prabpaipal
[ ] Chatchawan Khunpiluek
[✓] Wanlop Larpkern

B 0326172

Cert. No.: 23T1769
Page.: 2 of 2

Result of Calibration:- Without Adjustment
Function: Temperature measurement
Dimension of probe : Diameter 3 mm., Length 55 mm. Sheath material : Stainless Steel

Immersion Depth (mm.)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
50	25.0022	24.9	-0.1022	0.12
50	30.0037	29.9	-0.1037	0.12
50	40.0021	40.0	-0.0021	0.12

UUC* : Unit Under Calibration
The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

-o0o-

a 1184739

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484

NSC-TIBI-TIS17025 CALIBRATION 0008

Cert.No.: 22CG3154
Page.: 1 of 2

Certificate of Calibration

Equipment : Burette
Capacity : 50 mL
Serial No. : -
ID. No. : BKK_EN0171
Manufacturer : Witeg
Made in : Germany
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.
Khwaeng Phatthanakan, Khet Suan Luang
Bangkok 10250 Thailand

REVIEW BY Sirilak P.
APPROVED BY KL AL
NEXT CAL. DATE 29/03/2024

Ambient Temperature : (20 ± 2.5) °C
Relative Humidity : (50 ± 10) %
Barometric Pressure : 759 mmHg
Calibration Procedure : ASTM E 542 - 01

Calibrated by : Panward Pramklam

Approved by :
Approved Signatory
( ) Pornthippa Tameyakul
( ) Malee Butkruea
(✓) Ponpan Paipim
( ) Srisuda Khamtha

Issue Date : 31 August 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0044607

Equipment : Burette
Received Date : 26 August 2022
Condition As-Received : Used Item
Calibration Date : 30 August 2022
Reference : 2208-0918DSC-2

Cert.No.: 22CG3154
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	AE200S	N03679	140RC001	21MM429	NIMT	22 Sep 2022
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	22H1243	NIST,NIMT	09 June 2023
3) Thermometer	-	1594592	140EC010	22I181	NIMT	10 Feb 2023

   This certification is traceable to SI Unit
2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	*k* Factor
50	49.9959	0.010	2.00

Remark mL = cm^3

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

a 1123908

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2643 8351-6 , e-mail: service.thailand@sartorius.com

NSC-TISI-TIS 17025
CALIBRATION 0426

SARTORIUS

REVIEW BY Sirilut P.
APPROVED BY
NEXT CAL. DATE 8/2/24

Certificate of Calibration

Model Number : MSE224S-100-DU
Description : Analytical Balance
Serial Number : 26207042
ID No. : BKK_EN0002
Manufacturer : Sartorius

Certificate No. : 23BCI0072
Issued Date : Monday, February 13, 2023
Reference No. : 203245
Page No. : 1 0f 2

Customer Name : ALS Laboratory Group (Thailand)Co., Ltd.
104 Phatthanakan 40,Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.
Calibrated Place : Balance Room

Calibrated By : Mr. Chonchai Inthana
Calibration Date : Wednesday, February 08, 2023

Calibration Procedure No. : This calibration was conducted by Using in-house calibration procedure number (WI-003) Based on UKAS LAB 14 : 2019

Metrological data :
Capacity : 220 g Readability : 0.0001 g

Ambients Conditions:
Temperature : 23.2 °C ± 5.0 °C
Humidity : 60.0 % RH ± 10.0 % RH
Pressure _ ± _

Reasons for calibration
☐ New Installation ☐ Service / Repaired ☑ Re-calibration/ Maintenance

Equipment Condition: ☑ Good Operate ☐ Fair

Measurement Method **UKAS Publication Ref :Lab 14**
The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Cetificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	SPC-RT	C02212555	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.
This certificate may not be reproducad other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

Mr.Chonchai Inthana(Technical Manager)

STAMP

SOP FM 33 03 February 2022

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2643 8351-6 Fax: +66 2643-8367, e-mail: service.thailand@sartorius.com

SARTORIUS

Certificate of Calibration

Model Number : MSE224S-100-DU
Description : Analytical Balance
Serial Number : 26207042
ID No. : BKK_EN0002
Manufacturer : Sartorius

Certificate No. : 23BCI0072
Issued Date : Monday, February 13, 2023
Reference No. : 203245
Page No. : 2 of 2

Calibration Results : Without Adjustment

Repeatability


The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0000	199.9999
Tolerance	20.0000	200.0000
0.0001 g	20.0000	199.9999
	20.0001	200.0000
Nominal Value : (High Load)	20.0000	200.0000
200 g	20.0000	199.9999
Tolerance	20.0000	199.9999
0.0001 g	20.0000	200.0000
	20.0001	199.9999
Standard Deviation	0.00004	0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximim capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 50 g
Tolerance *0.0004* g



	Difference
1	–
2	-0.0001
3	0.0000
4	0.0001
5	0.0000
6	–

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance *0.0002* g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00014
0.1	0.1000	0.1000	0.0000	0.00014
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	199.9999	-0.0001	0.00030

End of Report.

SOP FM 33 03 February 2022

SCG

Metrological Center

SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100
Bangkok Tel : +668 9205 6851 , +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.com

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T222502 **Page 1 of 4**

Certificate of Calibration

REVIEW BY Sirilut P.
APPROVED BY
NEXT CAL. DATE 09/05/24

Equipment : Chamber (Oven)
Manufacturer : Memmert
Model : UF 450
Serial No. : B7170531
Customer Code : BKK_EN0273
ID No. : T8042A4
Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250
Customer Location : Oven Room
Date of Receipt : 23 November 2022
Calibrated By : Sujjar Naknakred (Site Calibration Manager)
Approved By : /Boonchai Suriyawong (Site Calibration Manager)
Date of Issue : 09 DEC 2022

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L14I18/31-08-64

SCG
Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
NSC-TISI-TIS 17025 CALIBRATION 0244

Calibration Report

Equipment : Chamber (Oven)
Date of Calibration : 29 November 2022
Environment : Temperature : 29.1-29.6 °C
Line Voltage : 221.3-223.2 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors and nine standard thermocouples type T into its chamber , the other one resistance thermometer detector use for ambient temperature measurement .
The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :


Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	27-(CH1-10)	T210004	30 December 2022
TC	TYPE T	TN261-TN270	T210010	30 December 2022
DATA LOGGER	34970A	T149	T210004	30 December 2022

3. This certificate is traceable to :
National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
Equipment Description :
Time Constant 1 Hour 49 Minute At 104 °C
Fresh Air Damper [X] Open [ ] Min [ ] Medium [X] Max
[ ] Close
[ ] Not Available
5. Adjustment :
( ) without adjustment (X) after adjustment

Approved By.

SCG
Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
NSC-TISI-TIS 17025 CALIBRATION 0244

Calibration Report

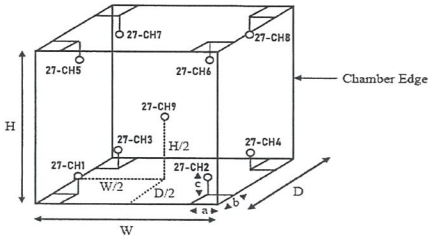

Remark :
Internal Dimensions of Chamber : W (Width) = 104 cm. , H (Height) = 72 cm. and D (Depth) = 60 cm.
Size of Installed Standard sensor number 27-CH1 to number 27-CH8 : a = 5 cm. ,b = 5 cm. and c = 5 cm.
Size of Installed Standard sensor number 27-CH9 : W/2 = 104 cm./2 , H/2 = 72 cm./2 and D/2 = 60cm./2

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)								
	27-CH1	27-CH2	27-CH3	27-CH4	27-CH5	27-CH6	27-CH7	27-CH8	27-CH9
104	104.07	103.60	103.45	104.02	104.47	103.57	104.59	103.78	104.18


Chamber (Oven)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor k
	Min , Max	Average					
104.0	-	104.0	103.97	0.07	0.70	0.42	2.00

* The quoted uncertainty exclude "uniformity"
The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By.

SCG
Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
NSC-TISI-TIS 17025 CALIBRATION 0244

Calibration Report

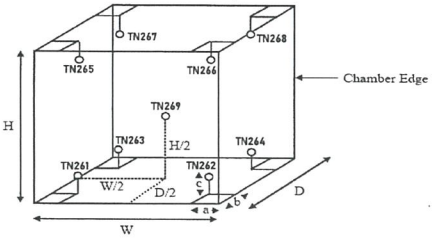

Remark :
Internal Dimensions of Chamber : W (Width) = 104 cm. , H (Height) = 72 cm. and D (Depth) = 60 cm.
Size of Installed Standard sensor number TN261 to number TN268 : a = 5 cm. ,b = 5 cm. and c = 5 cm.
Size of Installed Standard sensor number TN269 : W/2 = 104 cm./2 , H/2 = 72 cm./2 and D/2 = 60cm./2

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)								
	TN261	TN262	TN263	TN264	TN265	TN266	TN267	TN268	TN269
180	179.14	179.17	179.65	179.26	180.41	179.64	181.18	180.99	180.36

Chamber (Oven)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor k
	Min , Max	Average					
180.0	-	180.0	179.98	0.38	1.78	1.10	2.00

* The quoted uncertainty exclude "uniformity"
The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By.

Bara Scientific
Bara Scientific Co., Ltd.
966 U Chu Liang Building Floor7 Rama4 Road
Silom Bangrak Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com

Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No.	BSCC-UV-367/23
Equipment	UV/Vis Spectrophotometer
Model	UV-1800
Manufacturer	Shimadzu
Serial No.	A11454908533CD
ID No.	BKK_EN0018
Date of receipt	15 September 2023
Date of calibration	15 September 2023
Date of issue	22 September 2023

REVIEW BY Siriluk P.
APPROVED BY
NEXT CAL DATE 15/9/2024

Customer name	ALS Laboratory Group (Thailand) Co . Ltd
Address	104 Soi Phattanakan 40. Phattanakan Road. Phattanakan. Suan Luang. Bangkok 10250
Temperature	(23.4 24.7) °C (On site)
Humidity	(55.5 - 61.2) %RH (On site)
Equipment condition	Good Operation
Calibration Location	Organic Prep
Calibration Procedure	In-house method WI-UV-702-01 based on ASTM E275-01
Traceability	Wavelength Accuracy is traceable to certificate No 95917 and 95918 Photometric Accuracy is traceable to certificate No 95937 and 95924 Stray Light is traceable to certificate No 95908 The above certificate are traceble to SI unit through Starna Scientific Ltd (UKAS accredited calibration laboratory NO 0659)
Calibrated by	Mr Wanchana Janloey

Approved by
Mr.Kanchit Choothep
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate. Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.

Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangrak Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com

Certificate of Calibration

Certificate No. BSCC-UV-367/23 Number of Page(s) 2 of 3

Calibration Results:

1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
241.70	241.67	-0.03	0.18
334.02	334.03	0.01	0.18
418.53	418.59	0.06	0.18
572.99	573.14	0.15	0.18
879.41	879.21	-0.20	0.18

2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000	0.0000	0.0000	0.0075
	0.7467	0.7460	-0.0007	0.0075
257	0.0000	0.0000	0.0000	0.0075
	0.8662	0.8646	-0.0016	0.0075
313	0.0000	0.0000	0.0000	0.0075
	0.2904	0.2908	0.0004	0.0075
350	0.0000	0.0001	0.0001	0.0075
	0.6429	0.6415	-0.0014	0.0075

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate. Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.

Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangrak Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com

Certificate of Calibration

Certificate No. BSCC-UV-367/23 Number of Page(s) 3 of 3

Calibration Results:

3.Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5783	0.5793	0.0010	0.0042
	0.7628	0.7624	-0.0004	0.0042
	1.0206	1.0216	0.0010	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5621	0.5625	0.0004	0.0042
	0.7455	0.7452	-0.0003	0.0042
	0.9985	0.9989	0.0004	0.0042
465.0	0.0000	0.0000	0.0000	0.0042
	0.5227	0.5229	0.0002	0.0042
	0.6880	0.6873	-0.0007	0.0042
	0.9487	0.9486	-0.0001	0.0042
546.1	0.0000	0.0000	0.0000	0.0042
	0.5207	0.5211	0.0004	0.0042
	0.6973	0.6960	-0.0013	0.0042
	0.9959	0.9944	-0.0015	0.0042
590.0	0.0000	0.0000	0.0000	0.0042
	0.5544	0.5538	-0.0006	0.0042
	0.7253	0.7236	-0.0017	0.0042
	1.0942	1.0925	-0.0017	0.0042
635.0	0.0000	0.0000	0.0000	0.0042
	0.5616	0.5612	-0.0004	0.0042
	0.6927	0.6909	-0.0018	0.0042
	1.0881	1.0866	-0.0015	0.0042

*CNR = Customer not request

4.Stray Light*

Standard	Unit Under Calibration(UUC)		
cut-off wavelenght (nm)	Wavelength (nm)	Transmission (%T)	Absorbance (A)
200.96±0.11nm	200.55	0.9770	2.0104

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A
*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%

End of Certificate

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate. Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.

Agilent Technologies

7700 Series ICP-MS
Preventive Maintenance Checklist – Standard

Agilent Preventive Maintenance provides factory recommended service for your analytical systems to assure reliable operation and the accuracy of your results. Delivered by highly-trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak.

For more information about Agilent Technologies services please visit our web site using the following URL http://www.chem.agilent.com/en-us/products/services/pages/default.aspx

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of additional or special procedures and/or parts for the instrument service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Service Engineer's Responsibilities

- Only complete/printout pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using a "X" or tick mark "✓" in the checkbox.
- Complete Not Applicable check boxes to indicate services not delivered, as needed.
- Complete the PM service in the order of the tasks listed.
- Complete the Service Review section together with the customer.

REVIEW BY ..... H.
APPROVED BY ..... Sawan Jan. IV
NEXT CAL DATE ..... 11 | 08 | 2024

Agilent Technologies

7700 Series ICP-MS
Preventive Maintenance Checklist – Standard

System Information

Instrument system name and ID	7900X ICP-MS
Instrument system site and location	ALS Laboratory Group (Thailand) Co.,Ltd
List system component product numbers	List the serial numbers of each component
1. G3281A	1. JP12091612
2. G3282A	2. SN 12207000
3. PTX 500	3. US 02129345EO
4.	4.
5.	5.
6.	6.
7.	7.

ICP-MS configuration table	Circle the type or write in the type if other
Nebulizer	MicroMist | Micro Flow | (Mira Mist) | other
Spray Chamber	(Quartz) | PFA | other
Torch	(Quartz) | Demountable | other
Sampling Cone	(Ni) | Pt | other
Skimmer Cone	(Ni) | Pt | Ni plated | other

Preparation

- ☑ Discuss any specific issues with the customer prior to starting.
- ☑ Review the instrument logbook.
- ☑ Save instrument control settings before starting the procedure.
- ☑ Perform general inspection of system for cleanliness
- ☑ Check for proper installation of safety-related parts, assemblies , sensors etc
- ☑ Check for required firmware updates and verify with customers if they would like it installed.
- ☑ Begin system vent.

Inspect and clean system while venting

- ☑ Perform a general inspection of the system.
- ☑ Look for any obvious external damage or problems.
- ☑ Check mechanical pumps for evidence of excessive fluid leaks.
- ☑ Inspect vacuum hoses, pump exhaust tubes and power cord for excessive wear.
- ☑ Inspect Shield plate contacts. Clean if needed.
- ☑ Inspect the tape lining on the peristaltic pump clamp; replace the tape if worn (5043-0030).
- ☐ Check electronics for dust accumulation, clean if necessary.

Mechanical vacuum pumps

- ☑ Drain and replace mechanical pump fluid.
- ☑ Verify proper oil recycling function of mechanical pumps, the gas ballast valve must be open.
- ☑ Replace the oil mist filter.
- ☑ Inspect and clean or replace the inlet filter (P/N 5190-0145 for E2M18, P/N SR03700237 for DS402)
- ☐ Verify proper oil recycling function of mechanical pumps, the gas ballast valve must be open when connected to an Edwards E2M18.

Cooling water system

- ☐ Drain cooling fluid
- ☑ Remove, clean and reinstall metal mesh filter.
- ☑ Re fill Polyclear cooling fluid (G3292-80010)
- ☐ Clean the Air filter and the Condenser by compressed air or vacuum cleaner

Ion lens cleaning

- ☑ Remove extraction/omega lenses and clean all lenses.
- ☐ Remove ORS cell, plate bias and deflect lens, clean all lenses.
- ☐ Replace octopole. Reinstall all lenses and the ORS cell and close analyzer.

Auto Sampler ASX500 Series

- ☑ Clean external surfaces of the Autosampler, this will protect the service technician from potential chemical burns
- ☐ Z-Axis Inspection Inspect the Z-axis PEEK drive cable for kinks or slight bends. Power off the autosampler and manually move the Z-drive up and down using the rotor on the rear of the instrument. Inspect the Z-axis drive cable for kinks or slight bends o If the movement is rough and hard to move then replace Z-axis drive cable (P/N G3286-80331) or Z-axis drive assembly (P/N G3286-80330)

- ☑ Pump Tubing Replacement
  Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles
- ☑ QC Testing
  Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and ensure that the probe is centered in the vial
- ☑ Final Inspection
  Check that all components are tight

Auto Sampler I-AS

- ☐ Clean external surfaces of the Autosampler, this will protect the service technician from potential chemical burns
- ☐ Pump Tubing Replacement
  Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles.
- ☐ QC Testing
  Using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial.

ISIS

- ☑ Replace ISIS valve seal (P/N G3138-65117)
- ☑ Inspect the tape lining on the peristaltic pump clamp; replace the tape if worn (5043-0030).
- ☑ QC test
  Verify the function of valve and Peripump. Make sure that there is no leak from the valve and pump tubing connections.

Restore Instrument

- ☑ Pump system down.
- ☐ Perform the system post check.
  - ☑ Check quadrupole matching.
  - ☑ Perform octopole matching.
  - ☑ Verify good gas control function by changing the flow and observing the meter readings, perform an automatic offset adjustment for the MFC's.
  - ☑ Verify in Tune (using the customer's last tune) that changes in lens voltage result in the expected sensitivity change.
  - ☑ Perform Startup including performance report and an Autotune. Print the Autotune report and attach it to this checklist.
  - ☑ Check the instrument status and record the measurements in the status table. (Use "Record Log" in "Maintenance LogBook" with G7200B software, Use Performance report with G7201A/B software)
  - ☑ Record the EM and discriminator Voltages in the results table.
  - ☑ Run 10 minute stability test with tune solution. Check the result of RSD is below 4%.

Guidance

If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Make an entry in the MassHunter Maintenance Log Book recording the PM activities.
- ☑ Update/reset instrument maintenance counters as appropriate
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section below if there are additional comments
- ☑ Review the service and any test results with the customer.
- ☐ If the Instrument firmware was updated, record the details of the change in the Service Engineer's Comments box below or if necessary, in the customer's IQ records.

7700 Series ICP-MS Status Results Table

- ☐ Check this box if you have run a performance report to record the meter readings. Print out the report and attach it to this checklist, instead of completing the table.

Measurement	Standby Mode	Analysis Mode No Gas Mode	Analysis Mode H_2 Gas @ 4ml/min	Analysis Mode He Gas @ 4ml/min
IF/BK Press	2.65 Pa	242 Pa	– Pa	247 Pa
TMP Revolution	100 %	100 %	– %	100 %
Analyzer Press	5.59×10^{-5} Pa	2.35×10^{-4} Pa	– Pa	3.25×10^{-4} Pa
Water RF/WC/IF	❶	1.50 L/min		
Water Temperature		22.1 °C		
Inlet Temp	25.0 °C	29.9 °C		
Internal Temp	15.0 °C	16.0 °C		
RF Power		1551 Watts		
RF Reflect		5 Watts		
Plasma Freq		26.78 MHz		
Carrier Gas (BP)		441 kPaG		
Ar Gas Tank Press		569 kPaG		
Carrier Gas		1.00 L/min		
MU/Dil. Gas		0.10 L/min		
Plasma Gas		15.00 L/min		
Aux Gas		0.90 L/min		
S/C Temperature		2.0 °C		
OP Gas Tank Press*1	– kPaG	– kPaG		
Optional Gas *1		– %		

❶ Do not fill in the shaded cells in the table. There are no measurements for these combinations.

Notes:

7700 Series ICP-MS Test Results Table

Test Description	Expected Test Result	Actual Test Result
Analog HV Voltage	Not applicable	1761 V
Pulse HV Voltage	Not applicable	1496 V
Discriminator Voltage	Not applicable	4.5 mV

7700 Series ICP-MS Parts List Table

Part Description	Part Number	Product/Model # where used	Quantity Consumed
1L Rough Pump Oil	6040-0834	7700 ICP-MS	2
Oil Mist Filter Kit for E2M18	3162-1056	7700 ICP-MS	1
Oil Mist Filter for DS402	9499342M002	7700 ICP-MS	–
Graphite Gasket for Sample Cone (3pk)	G3280-67009	7700 ICP-MS	1
7700 Octopole	G3286-67045	7700 ICP-MS	1
Polyclear cooling fluid	G3292-80010	G1879B/G3292A	1
Rinse / Drain tubing	G3286-80117	ASX-500	1
Tubing / connection kit for drain	G3286-80118	ASX-500	1
Peristaltic pump tubing set	G3160-65326	I-AS	–
Drain tubing to rinse bottle and drain bottle	G3160-65328	I-AS	–
Rotor seal for Valve (ISIS)	G3138-65117	ISIS	1
Additional parts may be required from engineers stock:			
Inlet Filter E2M18	5190-0145	7700 ICP-MS	–
Inlet Filter DS402	SR03700237	7700 ICP-MS	–
Peristaltic pump tape (30m roll)	5043-0030	7700 ICP-MS	–
Polishing Paper Kit (#400/#1200, 5 sheets each)	G1833-65404	7700 ICP-MS	–
Cotton Swabs, ultra-fine conical bud shape at both ends (100/pk)	9300-2574	7700 ICP-MS	–
Alumina Powder	8660-0791	7700 ICP-MS	–
lint-free-paper	05980-60051	7700 ICP-MS	–
Z-Axis Drive PEEK Cable (Anti-Kink)	G3286-80331	ASX-500	–
Z-Axis Drive Assembly (PEEK, Anti-Kink)	G3286-80330	ASX-500	–

Copyright © 2013

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write in this box.

Other Important Customer Web Links

- ❑ How to get information on your product: Literature Library - http://www.agilent.com/chem/library
- ❑ Need to know more? - www.agilent.com/chem/education
- ❑ Need technical support, FAQs? - www.agilent.com/chem/techsupp
- ❑ Need supplies? - www.agilent.com/chem/supplies

Service Completion

Service request number 600 6142623 Date service completed 12 June 2023

Agilent signature _____ Customer signature Supakwan M.

Document part number: G3280-90078


Copyright © 2013

Tune Report

Operator Name	Supakwan Mak
Acq/Data Batch	C:\Agilent\ICPMH\1\UserTune.b
Acq. Date-Time	6/12/2023 4:05:12 PM
Report Comment	PM 12 June 2023
Instrument Name	G3281A JP12091612

[No Gas]

Sensitivity




Mass	Range	Count	RSD%	Background
7	10000	6340	4.494	2.100
89	50000	27817	3.328	3.600
205	50000	18585	3.537	9.600

Sampling Period [sec] 0.311
Integration Time [sec] 0.1

Oxide/Doubly Charged Ratio

Oxide 156 / 140 1.492 %
Doubly Charged 70 / 140 1.508 %

Resolution/Axis



Mass	Peak Height	Axis	W-50%	W-10%
7	5337.66	7.00	0.64	0.730
89	27561.94	89.00	0.55	0.710
205	19016.73	205.00	0.46	0.726

Integration Time [sec] 0.1
Acquisition Time [sec] 22.74
Y Axis Linear

Tune Parameters

Plasma Parameters

Plasma Mode	—	Nebulizer Gas	1.00 L/min	Makeup Gas	0.10 L/min
RF Power	1550 W	Option Gas	—	Auxiliary Gas	0.90 L/min
RF Matching	1.80 V	Nebulizer Pump	0.10 rps	Plasma Gas	15.0 L/min
Sample Depth	8.0 mm	S/C Temp	2 °C		

Lens Parameters

Extract 1	0.0 V	Omega Lens	6.4 V	Deflect	11.8 V
Extract 2	-145.0 V	Cell Entrance	-30 V	Plate Bias	-40 V
Omega Bias	-90 V	Cell Exit	-50 V		

Cell Parameters

Use Gas	No	3rd Gas Flow	—	Energy Discrimination	5.0 V
He Flow	0.0 mL/min	OctP Bias	-8.0 V		

Tune Report

H2 Flow	—	OctP RF	190 V		

QP Parameters

Mass Gain	145	Axis Gain	1.0021	QP Bias	-3.0 V
Mass Offset	124	Axis Offset	0.12		

Hardware Settings

Torch


Torch H	-0.4 mm	Torch V	0.0 mm		

EM

Discriminator	4.5 mV	Analog HV	1748 V	Pulse HV	1496 V

[He]

Sensitivity



Mass	Range	Count	RSD%	Background
59	20000	11826	2.752	7.200
89	20000	13367	2.527	5.800
205	50000	25671	2.706	13.300

Sampling Period [sec] 0.31
Integration Time [sec] 0.1

Oxide/Doubly Charged Ratio

Oxide 156 / 140 1.166 %
Doubly Charged 70 / 140 1.586 %

Tune Parameters

Plasma Parameters

Plasma Mode	—	Nebulizer Gas	1.00 L/min	Makeup Gas	0.10 L/min
RF Power	1550 W	Option Gas	—	Auxiliary Gas	0.90 L/min
RF Matching	1.80 V	Nebulizer Pump	0.10 rps	Plasma Gas	15.0 L/min
Sample Depth	8.0 mm	S/C Temp	2 °C		

Lens Parameters

Extract 1	0.0 V	Omega Lens	7.4 V	Deflect	3.6 V
Extract 2	-200.0 V	Cell Entrance	-90 V	Plate Bias	-115 V
Omega Bias	-90 V	Cell Exit	-70 V		

Cell Parameters

Use Gas	Yes	3rd Gas Flow	—	Energy Discrimination	3.0 V
He Flow	4.5 mL/min	OctP Bias	-21.0 V		
H2 Flow	—	OctP RF	200 V		

QP Parameters

Mass Gain	145	Axis Gain	1.0021	QP Bias	-18.0 V
Mass Offset	124	Axis Offset	0.12		

Hardware Settings

Torch

Torch H	-0.4 mm	Torch V	0.0 mm		

Tune Report

EM

Discriminator	4.5 mV	Analog HV	1748 V	Pulse HV	1496 V

6/12/2023 4:05 PM

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676 Page 1 of 6

Certificate of Calibration

Equipment	:	HEATING BLOCK
Manufacturer	:	Environmental Express
Model	:	SC 196
Serial No.	:	6974CECW3285
Customer Code	:	BKK_EL0054
ID No.	:	T5306A3
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd.
		104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
		Khet Suan Luang, Bangkok 10250
Customer Location	:	Acid Digestion Lab
Date of Receipt	:	13 September 2023
Calibrated By	:	Sanee Musikawan (Site Calibration Manager)
Approved By	:	_____ / Sujjar Naknakred (Site Calibration Manager)
Date of Issue	:	26 SEP 2023

REVIEW BY Tattsporn C.
APPROVED BY Sujjar N.
NEXT CAL. DATE 22/03/25

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676 Page 2 of 6

Calibration Report

Equipment	:	HEATING BLOCK
Date of Calibration	:	22 September 2023
Environment	:	Temperature : 21.8-23.1 °C
		Line Voltage : 221.6-226.3 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 20 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN21-TN30	T230014	17 January 2024
TC	TYPE T	TN31-TN40	T230014	17 January 2024
DATA LOGGER	34970A	T151	T230014	17 January 2024

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 2 Hour 20 Minute At 95 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By._____

Metrological Center

SCI ECO Services Company Limited


33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676 Page 3 of 6

Calibration Report

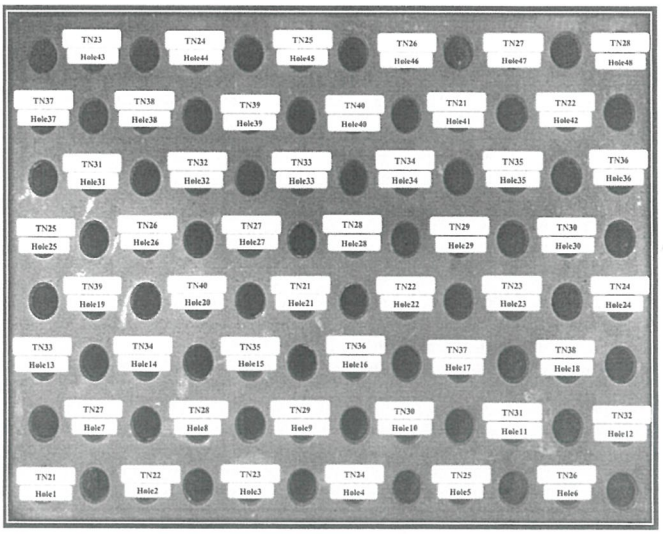

FRONT CONTROL

Approved By._____

Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110
Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		TN21	TN22	TN23	TN24	TN25	TN26
CAL POINT	Max	95.01	94.41	95.20	95.41	94.51	95.17
95	Min	94.57	93.95	94.75	94.92	94.00	94.72
	Average	94.79	94.18	94.98	95.17	94.26	94.95
R2 Hole7-Hole12		TN27	TN28	TN29	TN30	TN31	TN32
	Max	95.36	95.43	95.19	95.16	95.35	94.97
	Min	94.94	94.95	94.72	94.71	94.90	94.57
	Average	95.15	95.19	94.96	94.94	95.13	94.77
R3 Hole13-Hole18		TN33	TN34	TN35	TN36	TN37	TN38
	Max	95.37	95.50	95.22	95.21	95.33	95.31
	Min	94.99	95.09	94.78	94.82	94.88	94.96
	Average	95.18	95.30	95.00	95.02	95.11	95.13
R4 Hole19-Hole24		TN39	TN40	TN21	TN22	TN23	TN24
	Max	95.59	94.42	94.52	94.24	94.63	94.67
	Min	95.21	94.06	94.13	93.88	94.28	94.27
	Average	95.40	94.24	94.33	94.06	94.45	94.47
R5 Hole25-Hole30		TN25	TN26	TN27	TN28	TN29	TN30
	Max	95.19	95.38	92.93	95.30	95.14	95.03
	Min	94.83	95.03	92.56	94.95	94.79	94.70
	Average	95.01	95.20	92.75	95.12	94.96	94.87
R6 Hole31-Hole36		TN31	TN32	TN33	TN34	TN35	TN36
	Max	94.63	94.90	94.77	94.31	94.24	93.87
	Min	94.24	94.55	94.44	93.98	93.92	93.56
	Average	94.43	94.72	94.60	94.14	94.08	93.71
R7 Hole37-Hole42		TN37	TN38	TN39	TN40	TN21	TN22
	Max	94.30	94.44	94.04	93.81	94.89	95.35
	Min	93.95	94.05	93.67	93.48	94.39	94.90
	Average	94.13	94.24	93.86	93.65	94.64	95.12
R8 Hole43-Hole48		TN23	TN24	TN25	TN26	TN27	TN28
	Max	95.99	95.63	95.28	95.29	95.45	94.87
	Min	95.57	95.15	94.82	94.84	94.99	94.48
	Average	95.78	95.39	95.05	95.07	95.22	94.68

Approved By. _____

Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110
Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		TN21	TN22	TN23	TN24	TN25	TN26
CAL POINT	Max	105.23	104.32	105.43	105.25	104.44	105.27
105	Min	104.94	103.95	105.15	105.04	104.11	104.96
	Average	105.09	104.13	105.29	105.15	104.28	105.12
R2 Hole7-Hole12		TN27	TN28	TN29	TN30	TN31	TN32
	Max	105.30	105.12	105.18	105.22	105.12	105.16
	Min	105.11	104.92	104.96	105.00	104.92	104.97
	Average	105.20	105.02	105.07	105.11	105.02	105.06
R3 Hole13-Hole18		TN33	TN34	TN35	TN36	TN37	TN38
	Max	105.37	105.63	105.02	104.80	104.69	105.19
	Min	105.17	105.37	104.75	104.59	104.50	105.00
	Average	105.27	105.50	104.88	104.69	104.60	105.09
R4 Hole19-Hole24		TN39	TN40	TN21	TN22	TN23	TN24
	Max	105.31	104.43	106.41	104.71	105.63	105.82
	Min	105.08	104.22	106.15	104.41	105.37	105.56
	Average	105.19	104.33	106.28	104.56	105.50	105.69
R5 Hole25-Hole30		TN25	TN26	TN27	TN28	TN29	TN30
	Max	104.95	106.26	103.34	105.78	105.59	105.87
	Min	104.67	105.96	103.08	105.56	105.36	105.68
	Average	104.81	106.11	103.21	105.67	105.48	105.77
R6 Hole31-Hole36		TN31	TN32	TN33	TN34	TN35	TN36
	Max	104.75	104.86	104.80	105.20	104.50	104.39
	Min	104.54	104.63	104.59	105.00	104.32	104.18
	Average	104.65	104.75	104.69	105.10	104.41	104.28
R7 Hole37-Hole42		TN37	TN38	TN39	TN40	TN21	TN22
	Max	104.30	104.90	104.85	104.65	104.88	104.85
	Min	104.09	104.72	104.66	104.49	104.63	104.52
	Average	104.19	104.81	104.75	104.57	104.76	104.68
R8 Hole43-Hole48		TN23	TN24	TN25	TN26	TN27	TN28
	Max	105.71	105.85	105.39	105.61	105.42	105.19
	Min	105.45	105.61	105.14	105.27	105.18	104.94
	Average	105.58	105.73	105.27	105.44	105.30	105.07

Approved By. _____

Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110
Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (±°C)	Uncertainty (±°C)
	Min , Max	Average		
100.0	100.3 , 100.5	100.4	0.26	0.81
107.0	107.0 , 107.1	107.1	0.19	0.78

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item

The result of test was found accurate as shown on date and place of test only

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____

Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100
Bangkok Tel : +668 9205 6851 , +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025 CALIBRATION 0244

Certificate of Calibration

Equipment : **Chamber (Cold Room)**

Manufacturer : **KOLDTECH**

Model : **KM 320**

Serial No. : **TBN-1012061/05**

Customer Code : **BKK_EN0167**

ID No. : **T2463A3**

Customer : **ALS Laboratory Group (Thailand) Co.,Ltd.**
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250

Customer Location : **Environmental Laboratory**

Date of Receipt : **27 June 2022**

Calibrated By : **Sujjar Naknakred (Site Calibration Manager)**

Approved By : _____ / **Boonchai Suriyawong (Site Calibration Manager)**

Date of Issue : 04 JUL 2022

REVIEW BY Sinluf P.
APPROVED BY KL AL
NEXT CAL. DATE 30/12/22

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

SCG
Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
NSC-TISI-TIS 17025 CALIBRATION 0244

Calibration Report

Equipment : **Chamber (Cold Room)**
Date of Calibration : **30 June - 1 July 2022**
Environment : **Temperature : 18.9-23.7 °C**
Line Voltage : 222.9-226.5 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :


Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T210009	30 July 2022
TC	TYPE T	TN171-TN180	T210009	30 July 2022
DATA LOGGER	34970A	T149	T210009	30 July 2022

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 3 Hour - Minute At 3 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By.

SCG
Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
NSC-TISI-TIS 17025 CALIBRATION 0244

Calibration Report



C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	= TN161	11F	= TN171
2A	= TN162	12F	= TN172
3A	= TN163	13A	= TN173
4F	= TN164	14A	= TN174
5A	= TN165	15F	= TN175
6A	= TN166	16E	= TN176
7F	= TN167		
8F	= TN168		
9A	= TN169		
10A	= TN170		

Approved By.

SCG
Metrological Center
SCI ECO Services Company Limited
33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.
NSC-TISI-TIS 17025 CALIBRATION 0244

Calibration Report

Measurement Results:

	Average Standard Reading at each position (°C)									
Calibration Point	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170
3	2.71	2.82	2.75	2.89	2.95	3.68	3.02	2.96	3.03	2.85
	TN171	TN172	TN173	TN174	TN175	TN176				
	2.97	3.02	2.89	3.04	2.97	3.33				

Chamber (Cold Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor *k*
	Min , Max	Average					
3.0	2.9 , 4.0	3.2	2.99	1.05	1.30	1.66	2.00

* The quoted uncertainty exclude " uniformity "
The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By.

BKK_EL0023

analytikjena

REVIEW BY Orawan T.
APPROVED BY Sawitree N.
NEXT CAL. DATE 24/05/24

Maintenance Protocol

Atomic Fluorescence Spectrometer

mercur DUO / mercur DUO plus

analytikjena

Serial-No.: K170A0143 Customer-No.:

Date: 24 May 2023 Carried out by: Srichai Fak-on

Maintenance with following Operational Qualification (OQ) ☐
(requires a separate OQ protocol)

Company	บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด
User	
Department	ห้องแลบปฏิบัติการ
Street	104 ซอย 40 ถนนพัฒนาการ แขวงสวนหลวง เขตสวนหลวง
Zip Code, City	กรุงเทพมหานคร 10250
Country	ประเทศไทย
Phone	
Fax	
E-mail	

analytikjena

Maintenance works basic unit

tightness visual check inside the Mercur	☑
visual check if gold-traps are broken	☑
visual check if spectrometer is contaminated	☑
visual check of the fluorescence cell	☑
visual check of the absorption cell, incl. window	☑
reactor cleaning	☑
check pump-hose, if necessary change it	☑
check swivel drive (SEV)	☑
check drying-hose, output gas-liquid-separator	☑
test Bubble-Sensor	☑
check gas flows	☑
check volume flows, reagents	☑
recording stray light values	☑
measurement with 30 ng/l	☑

Maintenance works Autosampler Serial No.: 701 739

lubricate the dosing-winding (Teflon-grease-spray)	☑
clean the dosing cylinder, if necessary exchange it	☑
lubricate the winding system of the height drive with some drops of oil	☑
check the toothed belt	☑
check the position of the mechanical stopper (height: 13mm)	☑
check the pump rate of mixing pump (<14s AS52, typ.7s/<20s AS52S, typ.10s)	☑
check the pump rate of washing cup	☑
check the electrical hose connections for good contact	☑
check the connectors of the magnetic valves	☑
check the dosing hose for buckling, if necessary exchange it	☑

analytikjena

Device parameter		nominal value	actual value
visual check general tightness inside the Mercur		o.k.: ☑	changed: ☐
visual check Goldtraps		o.k.: ☑	changed: ☐
visual check spectrometer			
	Fluorescence cell	o.k.: ☑	changed: ☐
	Absorption cell, incl. window	o.k.: ☑	changed: ☐
	lens	o.k.: ☑	changed: ☐
	Swivel drive (SEV)	o.k.: ☑	changed: ☐
check pump hoses		o.k.: ☑	changed: ☐
check hoses and hose connectors		o.k.: ☑	changed: ☐
check and clean reactor		o.k.: ☑	changed: ☐
check drying hose output Gas-liquid-seperator		o.k.: ☑	changed: ☐
check bubble-sensor		o.k.: ☑	not o.k.: ☐
Check gasflow			
	Argon pressure valve 4	1.2 – 1.5 bar	1.5 bar
	Valve 1	10 Nl/h or 0.166 NL/min	0.163 NL/min
	Valve 2	50 Nl/h or 0.833 NL/min	0.403 NL/min
	Valve 3	5 Nl/h or 0.083 NL/min	0.140 NL/min
	Valve 4	10 Nl/h or 0.166 NL/min	0.108 NL/min
Check liquidflow			
	Acid	2.5ml/min ± 1 ml	2.5 ml/min
	Red.-agent	2.5ml/min ± 1 ml	2.5 ml/min
	Sample	10ml/min ± 2 ml	10 ml/min
Adventitious light - values	**(V)**	**from file**	
	100	0	0
	200	0	0
	300	0	0
	350	0	0
	400	0	0
	450	2	2
	500	5	5
	550	10	10
	575	15	14
	600	20	20

analytikjena

Device parameter	nominal value	actual value
Analytical parameters Fluorescence cell		
Conditions: max.conc.: 10µg/L PMT-voltage: 360 V		
Blank-solution		Int 0.00024
without enrichment / FBR 30 ng/L	Int > 0.0015 RSD < 3 %	Int$_1$ 0.00172 RSD 0.45 %
Conditions: max.conc.: 1.7µg/L PMT-voltage: 352 V		
Blank-solution		Int 0.00370
with enrichment / FBR 30 ng/L	Int > 0.008 RSD < 3 %	Int$_2$ 0.01060 RSD 2.38 %
Fok.- factor (Int$_2$ / Int$_1$)	> 3.5	6.16
Analytical parameters Absorption cell		
Blank-solution		Ext. 0.00093
without enrichment / FBR 100 ng/L	Ext. > 0.0012 RSD < 5 %	Ext. 0.00449 RSD 2.58 %
Comments		

Srichai Fakon
Signature Technician

24 May 2023
Place, Date (DD/MM/YYYY)

Oranan T
Signature Customer

24 May 2023
Place, Date (DD/MM/YYYY)

analytikjena
An Endress+Hauser Company

35 Moo 5, 345 Road, Khlong Khoi, Pak Kret
Nonthaburi, 11120 Thailand
Phone +66(2) 1062979-72
Fax +66(2) 1062973
www.analytik-jena.com

Service Report

Customer's address :	Customer's Ref. No. :
สถาบันเทคโนโลยีพระจอมเกล้าเจ้าคุณทหารลาดกระบัง (สจล) อาคาร 104 ชั้น 4B ภาควิชาวิศวกรรมสิ่งแวดล้อม คณะวิทยาศาสตร์ กรุงเทพมหานคร 10520	
E-mail :	Phone : Fax :

☑ Analytik Jena Instruments (Thailand) Ltd.
☐ Analytik Jena Far East (Thailand) Ltd.

Job No. : B305282 PM	User :	Service Engineer :	Date : 24/5/2023 Page : 1/1
Instrument model : Mercur	Serial No. : K170A0143		Software Version No. : 4.7.10.0

☐ Repair (RE) ☑ Maintenance (PM) ☐ Installation (IN) ☐ Warranty ☐ Application (AP) ☐ Site Prep.(SP) ☐ Visit(VI)

Fault / Claim : – การบำรุงรักษาประจำปี ตามใบสั่งซื้อ Po No. 2300112 / (INV2300-037) ☐☐☐ Error Code
– บริการ PM Contract ปี 2023 (1 Jun / ปี 2023)

Action taken : – Maintenance Main Basic Unit
– Check Device parameter
– Check gas flow
– Check liquid flow
– Check Adventitious light – Valves

Test run Analytical parameter Fluorescence cell
Test run Analytical parameter Absorption cell






Action Pending / Recommendation : ตรวจสอบครั้งต่อไป

☐ Spare Part ☐ Instrument Configuration

Item No.	Name	Quantity	Unit Price
1.			
2.			
3.			
4.			
5.			
6.			
7.			
8.			

Herewith the undersigned confirm the time devoted, the work performed, the perfect function of the device, and the receipt/delivery of the specified spare parts. *Traveled hours and kilometers can only be entered after the return of the service engineer.	Date / Signature of Customer	Date / Signature of Service Engineer	Work completed? ☑ Yes ☐ No
	Oranuch T.		

Services are subject to the General Terms and Conditions of Analytik Jena AG, which will be sent on request.

Mercur

Report file:	C:\WinAAS\TMP\2023\May\Pro_032		
Program version:	4.7.10.0	Printed on:	5/24/2023 12:46
		Recording started on	5/24/2023 12:35 GMT+7.0
Operator:	PSU.OTA		
Laboratory:	ALS-BKK		
Code:	II_Hg095_2023		

Remarks:
Food,water

Method parameters Hg

Method	Without enrichment / FBR 30ng/L_PM24052023		
Created on	5/24/2023 Time 12:27		
Program	---		

Parameters Mercur Technique: Hg fluorescence

Line	253.7 nm		
Lamp type	Hg-LP		
Integr. mode	Peak height	Integr. time	30 s
PMT	360 V		
AZ time	5 s	Peak smoothing	8/5
Delay	0 s		

Working mode	w/o enrich.	System cleaning	Acid
FBR technique	on	Wash time acid	10 s
Pump speed	3	Soaking time	20 s
Sample load time	10 s	Gas load time	5 NL/h
Reaction time	10 s		
Waiting time AZ	5 s		
Delay	0 s		
Purge time1	28 s		
Purge time2	15 s	Gas wash time2	10 NL/h

Autosampler

Autosampler	AS51S/F	Tray type	87/139
Working mode	continuous		
Dilution	---		

QC parameters

QC type	Conc. check		
QC check samp. 1	---	QC check samp. 2	---
Conc.	---	Conc.	---
Error limit	---	Error limit	---
Rep. measurement	off	Reaction	flag + continue
QC std.1 no.	1(30.000 ng/L)	QC std.2 no.	1(30.000 ng/L)
QC std.1 limit	± 50.00%	QC std.2 limit	± 50.00%
QC std. act.	flag + continue		
Expect. blank abs.	0.0100± 0.0100	Reaction	flag + continue
QC precision	off		
		Reaction	off
		QC Recal.factor	Off

Calibration settings

Calib. meth.	Standard calib.	Calibr. unit	ng/L
No. standards	1	Conversion fac.	1000000
Type of standards	---	Standard prep.	Premixed
		Blank correct.	---
		Recalib. std. no.	---
Output unit	µg/L	Conversion fac.	1000
Calib. stat.	Mean	Meas. cycles	3
		Blind cycles	1
Stock sol. 1	---	Stock sol. 2	---
Stock sol. 3	---	Stock sol. 4	---
Type of cal. curve	linear	Intercept	calculated
Weighted cal.	off	Grubbs stat.	off
Check of cal. curve	no outlier test		

Sample statistics

Stat. mode	Mean	Meas. cycles	2
Confid. level	95.4 %	Blind cycles	1
Grubbs stat.	---		


Calibration standards Hg

No.	Name	State	Pos	Conc. / ng/L	Ints	SD	RSD/%
1	Cal-Zero	(--)	79	0.000	H: **0.000249**	**0.000132**	**53.13**
					A: 0.004274	0.001698	39.72
2	Cal-Std1	(--)	80	30.000	H: **0.001720**	**0.000007**	**0.459**
					A: 0.02172	0.000023	0.107

Calibration function 1 **5/24/2023 12:44 Calibration (Peak height)**

Ints=k1+k2*conc
k1=0.000249 k2=0.000049 Recal. factor: ---


Slope	0.00005 Ints/(ng/L)	R2-adjusted	1.0000
sc0	1.00000 ng/L		
Lower limit	0 ng/L	Upper limit	33.0 ng/L
Detection limit	---	Deter. limit	---

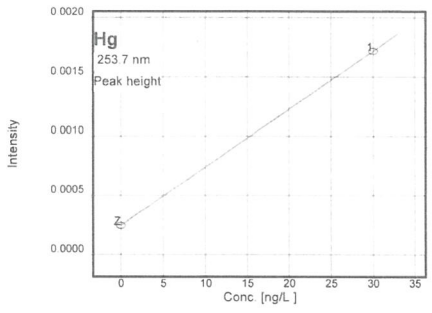

Measurements and events (sorted by time)

Hg	Without enrichment / FBR 30ng/L_PM 24052023					5/24/2023	12:35
ID	**Conc.**	**Ints**	**BG**	**SD**	**RSD/%**	**Int. type**	**Time**
Cal-Zero		0.000143				PkH	12:37
		0.000397					12:38
		0.000207					12:40
	0ng/L	0.000249		0.0001324	53.13		12:40
Cal-Std1		0.001720				PkH	12:42
		0.001712					12:43
		0.001728					12:44
	30.00ng/L	0.001720		0.000007897	0.459		12:44
Calibration	Calibration function: 01						12:44

Peak plots Hg



Mercur

Report file:	C:\WinAAS\TMP\2023\May\Pro_033		
Program version:	4.7.10.0	Printed on:	5/24/2023 14:01
		Recording started on	5/24/2023 13:37 GMT+7.0
Operator:	PSU.OTA		
Laboratory:	ALS-BKK		
Code:	II_Hg095_2023		

Remarks:
Food,water

Method parameters Hg

Method	Enrichment / FER 30ng/L PM_24052023		
Created on	5/24/2023 Time 13:36		
Program	---		

Parameters Mercur Technique: Hg fluorescence

Line	253.7 nm		
Lamp type	Hg-LP		
Integr. mode	Peak height	Integr. time	40 s
PMT	352 V		
AZ time	5 s	Peak smoothing	12/11
Delay	0 s		

Working mode	Enr. w/o reload	System cleaning	Off
FBR technique	off	Wash time acid	10 s
Pump speed	3	Soaking time	20 s
Sample load time	10 s	Gas load time	10 NL/h
Reaction time	10 s		
Waiting time AZ	10 s	Gas AZ wait	10 NL/h
Purge time1	30 s		
Purge time2	15 s	Gas wash time2	5 NL/h
Purge time3	20 s		
Heat.time coll.1	20 s	Cool. time coll.1	30 s

QC parameters

QC type	Conc. check		
QC check samp. 1	---	QC check samp. 2	---
Conc.	---	Conc.	---
Error limit	---	Error limit	---
Rep. measurement	off	Reaction	flag + continue
QC std 1 no.	1(30.000 ng/L)	QC std 2 no.	1(30.000 ng/L)
QC std 1 limit	± 50.00%	QC std 2 limit	± 50.00%
QC std. act.	flag + continue		
Expect. blank abs.	0.0100± 0.0100	Reaction	flag + continue
QC precision	off		
		Reaction	off
		QC Recal.factor	Off

Calibration settings

Calib. meth.	Standard calib.	Calibr. unit	ng/L
No. standards	1	Conversion fac.	1000000
Type of standards	---	Standard prep.	Premixed
		Blank correct.	---
		Recalib. std. no.	---
Output unit	µg/L	Conversion fac.	1000
Calib. stat.	Mean	Meas. cycles	3
		Blind cycles	1
Stock sol. 1	---	Stock sol. 2	---
Stock sol. 3	---	Stock sol. 4	---
Type of cal. curve	linear	Intercept	calculated
Weighted cal.	off	Grubbs stat.	off
Check of cal. curve	no outlier test		

Sample statistics

Stat. mode	off	Meas. cycles	1
Confid. level	95.4 %	Blind cycles	1
Grubbs stat.	---		


Calibration standards Hg

No	Name	State	Pos	Conc / ng/L	Ints	SD	RSD/%
1	Cal-Zero	(--)	##	0.000	H 0.003700	0.000081	2.192
					A 0.02531	0.000153	0.607
2	Cal-Std1	(--)	##	30.000	H 0.01060	0.000253	2.386
					A 0.06689	0.002766	4.136

Calibration function 1 **5/24/2023 14:00 Calibration (Peak height)**

Ints=k1+k2*conc
k1=0.003700 k2=0.000230 Recal. factor: ---


Slope	0.00023 Ints/(ng/L)	R2-adjusted	1.0000
sc0	1.00000 ng/L		
Lower limit	0 ng/L	Upper limit	33.0 ng/L
Detection limit	---	Deter. limit	---

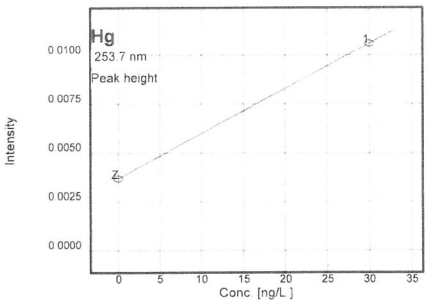

Measurements and events (sorted by time)

Hg	Enrichment / FER 30ng/L PM_24052023				5/24/2023	13:37
ID	**Conc.**	**Ints**	**BG**	**SD**	**RSD/%**	**Int. type**	**Time**
Cal-Zero		0.003792				PkH	13:41
		0.003666					13:43
		0.003640					13:44
	0ng/L	0.003700		0.000081090	2.192		13:44
Cal-Std1		0.009498				PkH	13:49
		0.008333					13:50
		0.008961					13:52
	30.00ng/L	0.008931		0.0005830	6.528		13:52
Cal-Std1		0.01031				PkH	13:57
		0.01074					13:58
		0.01076					14:00
	30.00ng/L	0.01060		0.0002530	2.386		14:00
Calibration	Calibration function 01						14:00

Peak plots Hg



Mercur

Report file:	C:\WinAAS\TMP\2023\May\Pro_034		
Program version:	4.7.10.0	Printed on:	5/24/2023 14:33
		Recording started on	5/24/2023 14:19 GMT+7.0
Operator:	PSU,OTA		
Laboratory:	ALS-BKK		
Code:	II_Hg095_2023		

Remarks:
Food,water

Method parameters Hg

Method	Without enrichment / Abs / FBR 100ng/L_PM 24052023
Created on	5/24/2023 Time 14:18
Program	---

Parameters Mercur Technique: Hg absorption

Line	253.7 nm		
Lamp type	Hg-LP		
Integr. mode	Peak height	Integr. time	55 s
PMT	225 V		
AZ time	5 s	Peak smoothing	2/5
Delay	8 s		

Working mode	w/o enrich.	System cleaning	Acid
FBR technique	on	Wash time acid	15 s
Pump speed	4	Soaking time	20 s
Sample load time	8 s	Gas load time	5 NL/h
Reaction time	12 s		
Waiting time AZ	15 s		
Delay	10 s		
Purge time1	50 s		
Purge time2	10 s	Gas wash time2	10 NL/h

QC parameters

QC type	Conc. check		
QC check samp. 1	---	QC check samp. 2	---
Conc.	---	Conc.	---
Error limit	---	Error limit	---
Rep. measurement	off	Reaction	flag + continue
QC std.1 no.	1(100.00 ng/L)	QC std.2 no.	1(100.00 ng/L)
QC std.1 limit	± 50.00%	QC std.2 limit	± 0.00%
QC std. act.	flag + continue		
Expect. blank abs.	0.0100± 0.0100	Reaction	flag + continue
QC precision	off		
		Reaction	off
		QC Recal.factor	Off

Calibration settings

Calib. meth.	Standard calib.	Calibr. unit	ng/L
No. standards	1	Conversion fac.	1000000
Type of standards	---	Standard prep.	Premixed
		Blank correct.	---
		Recalib. std. no.	---
Output unit	µg/L	Conversion fac.	1000
Calib. stat.	Mean	Meas. cycles	3
		Blind cycles	1
Stock sol. 1	---	Stock sol. 2	---
Stock sol. 3	---	Stock sol. 4	---
Type of cal. curve	linear	Intercept	calculated
Weighted cal.	off	Grubbs stat.	off
Check of cal. curve	no outlier test		

Sample statistics

Stat. mode	Mean	Meas. cycles	2
Confid. level	95.4 %	Blind cycles	1
Grubbs stat.	---		


Calibration standards Hg

No	Name	State	Pos	Conc./ ng/L	Abs	SD	RSD/%
1	Cal-Zero	(--)	##	0.00	H: **0.000932**	**0.000138**	**14.88**
					A: 0.035926	0.006208	17.28
2	Cal-Std1	(--)	##	100.00	H: **0.004494**	**0.000116**	**2.586**
					A: 0.061286	0.001275	2.082

Calibration function 1 **5/24/2023 14:33 Calibration (Peak height)**

Abs=k1+k2*conc
k1=0.000932 k2=0.000036 Recal. factor: ---

Slope	0.00004 Abs/(ng/L)	R2-adjusted	1.0000
sc0	1.00000 ng/L	Charact. conc.	122.411 (ng/L)/1%
Lower limit	0 ng/L	Upper limit	110 ng/L
Detection limit	---	Deter. limit	---

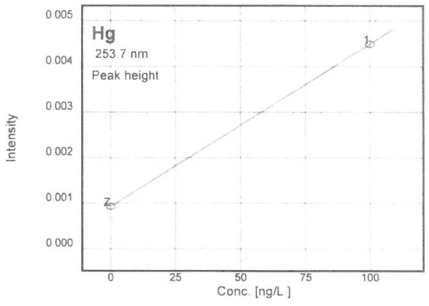


Measurements and events (sorted by time)

Hg	Without enrichment / Abs / FBR 100ng/L_PM 24052023				5/24/2023	14:19
ID	**Conc.**	**Abs**	**BG**	**SD**	**RSD/%**	**Int. type**	**Time**
Cal-Zero		0.001039				PkH	14:22
		0.000775					14:23
		0.000981					14:25
	0ng/L	0.000932		0.00013872	14.88		14:25
Cal-Std1		0.004528				PkH	14:29
		0.004364					14:31
		0.004589					14:33
	100.ng/L	0.004494		0.00011623	2.586		14:33
Calibration	Calibration function 01						14:33

5/24/2023 14:33 Page 4/4

Peak plots Hg



Mercur

BKK - EN0069

REVIEW BY Autcharawan S.
APPROVED BY Smanat M.
NEXT CAL. DATE 12 Jan 24

ARCHEMICA

Certificate of Calibration

ICS-2100: Anion (ID#659)

This certificate is to verify that instrument below are calibrated

by Archemica Lab Co., Ltd.

ICS-2100 S/N: 15010977

AS-HV S/N: 5450A36659

For

ALS Laboratory Group (Thailand) Co., Ltd.

Operator Signature: Nutdanai Date: Jan 12, 2023

(Mr.Nutdanai Laekhwan)

Application Chemist

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3, EQUIPMENT CALIBRATION AND TESTING SERVICES
53/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 ต่อ 29 FAX. 0-2719-9284

ilac-MRA NSC-TTBI-TIS17025 CALIBRATION 0006

Cert. No.: 23TM1408
Page : 1 of 4

Certificate of Calibration

Equipment :	Autoclave
Manufacturer :	TOMY
Model :	SX-700
Serial No. :	48134190
ID No. :	BKK_ML0041
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Media Preparation Room
Received Order :	03 October 2023
Calibration Date :	04 October 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Khit Ruttanaprapachai
Approved by :	Approved Signatory

REVIEW BY Sitthichok
APPROVED BY 04/10/23
NEXT CAL. DATE 04/10/24

( ) Pornthippa Tameyakul
(✓) Ponpan Paipim
( ) Suwit Imjai

Issue Date : 11 October 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 - Equipment Calibration and Testing Services

A 0053272

Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2310-0006OC-6

Cert. No.: 23TM1408
Page : 2 of 4

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013823	23LM66	TPA	25 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.
4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**

(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)


It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directry concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source



	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	26	64	221
Finished of Calibration	27	67	222

Position	Description	Ref. Std. ID No.:
1 =	Center of chamber	19-17TC-08
2 =	Temperature sensor	19-17TC-09
3 =	Exhaust port	19-17TC-10

a 1184533

Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2310-0006OC-6
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Operating parameter Set : Temperature = 108 °C
Sterilization period = 10 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor k
108	108	1	108.352	0.12	0.04	0.90	2
		2	108.263				
		3	108.140				

Operating parameter Set : Temperature = 115 °C
Sterilization period = 20 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor k
115	115	1	115.376	0.13	0.08	0.90	2
		2	115.297				
		3	115.157				

Operating parameter Set : Temperature = 118 °C
Sterilization period = 10 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor k
118	118	1	118.083	0.11	0.09	0.90	2
		2	118.037				
		3	117.954				

Average* : The average of 30 values in each position.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity.

Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2310-0006OC-6
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Operating parameter Set : Temperature = 121 °C
Sterilization period = 30 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor k
121	121	1	121.186	0.17	0.11	0.91	2
		2	121.082				
		3	120.980				

Average* : The average of 30 values in each position.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was excluded stability.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025 CALIBRATION 0006

Certificate of Calibration

Equipment : Incubator
Manufacturer : SHEL-LAB
Model : 1915A
Serial No. : 0200599
ID No. : BKK_ML0010
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthakan Rd.,
Khwawng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Location : Incubation & Micrological Reading

REVIEW BY Sithichok
APPROVED BY
NEXT CAL DATE 17/01/25

Received Order : 17 July 2023
Calibration Date : 17 July 2023
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon

Approved by : Approved Signatory
( ) Pornthippa Tameyakul
(✓) Malee Butkruea
( ) Suwit Imjai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 - Equipment Calibration and Testing Services

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1

Procedure Used :-
Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.


Condition of this result of calibration
1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.
Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	24
REL.Humid. (%)	54	56
AC Supply (Volt)	221	223



Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

Probe Installation Details :
a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :
D = 0.50 m
W = 0.75 m
H = 1.2 m
Capacity = 0.45 m^3

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert No : 23TM1146
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
35.0	35.0	35.0	0.055	0.30	0.44	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.888	34.933	34.815	34.813	35.064	35.019	35.156	35.141	35.087	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

a 1172188

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 EQUIPMENT CALIBRATION AND TESTING SERVICES
53/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0 2717 3000 ต่อ 27 FAX. 0 2719 3454

NSC-TISI-TIS1182S
CALIBRATION 0080

Cert. No.: 22TM1571
Page : 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven
Manufacturer : Binder
Model : ED 240/E2
Serial No. : 00-15533
ID No. : BKK_ML0013

REVIEW BY Sirichk
APPROVED BY
NEXT CAL. DATE 21/05/24

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Location : Media Preparatiom Room

Received Order : 21 November 2022
Calibration Date : 21 November 2022
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

Approved by : Approved Signatory
( ) Pornthippa Tameyakul
(✓) Malee Butkruea
( ) Suwit Imjai

Issue Date : 29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 Equipment Calibration and Testing Services

A 0048150

Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1
Procedure Used :-
Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.
The temperature scale used was based on ITS-90.
Condition of this result of calibration
1. Reference standard instrument:-


Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) After Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 22TM1571
Page : 2 of 3

Environment during calibration	Beginning	Finished
Temp. (°C)	26	26
REL.Humid. (%)	53	55
AC Supply (Volt)	219	220



Probe Installation Details :
a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :
D = 0.50 m
W = 0.80 m
H = 0.60 m
Capacity = 0.24 m³

Position :	Ref. Std. ID No.:
1	21-15TC-01
2	21-15TC-02
3	21-15TC-03
4	21-15TC-04
5	21-15TC-05
6	21-15TC-06
7	21-15TC-07
8	21-15TC-08
9 (ref.)	21-15TC-09

a 1138049

Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1
Result of Calibration :- (*) After Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 22TM1571
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (±°C)	Coverage Factor k
180	180	180	0.70	1.5	2.9	1.4	2

Calibration Point (°C)	Measured Temperature (°C) Position								
	1	2	3	4	5	6	7	8	9 (ref.)
180	179.520	180.585	178.855	179.482	178.827	179.938	179.074	180.199	180.068

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

a 1138053

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18 SUANLUANG SUANLUANG BANGKOK 10250
TEL. 0 2717 3000 29 FAX. 0 2719 6263

NSC-TMI-TIS17825
CALIBRATION 0066

Cert. No.: 23TM637
Page : 1 of 3

Certificate of Calibration

Equipment :	Water Bath
Manufacturer :	Memmert
Model :	WNE 45
Serial No. :	L712.0429
ID No. :	BKK_ML0056
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Incubator & Microbiological Reading
Received Order :	20 April 2023
Calibration Date :	20 April 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Kunchit Promprat

REVIEW BY Sithichok
APPROVED BY
NEXT CAL. DATE 20/4/24

Approved by : Malee .
Approved Signatory

( ) Pornthippa Tameyakul
(✓) Malee Butkruea
( ) Suwit Imjai

Issue Date : 24 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 - Equipment Calibration and Testing Services

A 0053357

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2304-0253OC-1

Cert. No.: 23TM637
Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration


1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44073381	22LM78/1	12 May 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	45	223
Finished of Calibration	25	43	223



Front

Position :	Ref. Std. S/N.:
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016

Malee .

a 1158265

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2304-0253OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM637
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C) Position 1	2	3	4	5 (ref.)	Uncertainty (± °C)
44.5	44.5	44.5	44.492	44.463	44.475	44.510	44.491	0.15
45.0	45.0	45.0	45.005	44.962	44.979	45.016	44.986	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor *k*
44.5	0.051	0.022	2
45.0	0.080	0.026	2

Average* : The average of 30 values in each position.
Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malee .

a 1158264

BKK_EL0037

Agilent Technologies

Agilent Technologies (Thailand) Limited
U CHU LIANG BLDG. 22/F UNIT A,D
968 RAMA 4 ROAD. SILOM. BANGRAK
Bangkok 10500 Thailand

Tel +662 637 6363
Fax +662 632 4334
Email ccc-smt@agilent.com
Website www.agilent.com/chem

Customer Contact:
ALS Laboratory Group (Thailand) Co Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan
TAX ID : 0105540004859
Chanattagarn.Imchom@alsglobal.com
27603068

Invoice To:
ALS Laboratory Group (Thailand) Co Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

SERVICE REPORT

Customer Purchase Order Number:	**Customer Number:** 70371013
Service Request:	**Service Request Date:**
Service Order: 6006033911	**Service Confirmation:** 6904800024

REVIEW BY Thitima S.
APPROVED BY
NEXT CAL. DATE 19 Apr 2024

Delivery Site:
ALS Laboratory Group (Thailand) Co Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

Location:
Room
Bldg
Lab
Dept

Direct Inquiries to:
Contact Name: Customer Contact Center
Contact E-mail: ccc-smt@agilent.com
Contact Telephone: +662 637 6363
Contact Fax: +662 632 4334

products | applications | software | services

Learn more about Agilent's Special Offers, Products, Services and our full range of laboratory productivity solutions optimized for your applications and workflows. Visit us at www.agilent.com/chem

Agilent Technologies (Thailand) Limited. Head Office
U Chu Liang Bldg. 22/F Unit A,D
968 Rama 4 Road. Silom. Bangrak.
Bangkok 10500 Thailand
Tax ID : 0105542068218

Citibank N.A. Bangkok Branch
399 Interchange 21 Building, Sukhumvit Road, Klongtoey Nau Sub-district, Wattana District, Bangkok 10110 Thailand
Acc. No. 012-4452-007
THB Krung Thai Bank PCL
Siam Square Br. 416/1-2 Rama I Rd. Pathumwan, BKK 10330 Thailand

ORIGINAL

Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IO-5100	ICP-OES 5100/5110 System			
G8010A	Agilent 5100 SVDV ICP-OES Spectrometer	MY16010005	ICP OES 5100	SYS-IO-5100
G8410A	SPS 4 Autosampler	AU15440764	ICP OES 5100	SYS-IO-5100

Service Items:

Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EOQ	Enterprise Operational Qualification	1.00	Agreement Entitlement - 100 % covered	20.03.2023	20.03.2023

Additional Information:

Service Information:

Problem Description:
WU-S-OQ-IO-5100-5001143313

Service Provided:
Complete OQHW 5100ICPOES
Equipment ID: BKK_EL0037, all tests passed

Service Overview Code:
Reason Code: Scheduled Service
Diagnosis Code: Scheduled Service
Resolution Code: Scheduled Service

Reported Hours:	Travel Hours:	
4.0	2.0	
Customer Field Service Representative Name: Kanyakorn Sukpathrajarern	**Customer Field Service Representative Signature:**	**Date:** 20 Mar 2023
Customer Name: Thitima Boonpeng	**Customer Signature:** Thitima B.	**Date:** 20 Mar 2023

Additional Comments:

Scientist Instrument

REVIEW BY P. Suriyarng
APPROVED BY Santa N.
NEXT CAL. DATE 30/11/23

Performance Verification Certificate

for Mercury Analyzer

Product ID *Quicktrace M-8000 , Teledyne Leeman Labs*

Equipment ID BKK_EL0128 Mercury Analyzer
S/N: US22133002

BKK_EL0129 Autosampler
S/N: 052222A560

Customer Name ALS Laboratory Group (Thailand) Co., Ltd.
Address 104 Soi Pattana 40, Pattana Rd. Suan Luang, Suan Luang
Bangkok 10250 Thailand

Date of Qualified November 30, 2022
Next Due date November 30, 2023

This certifies for products which was performed in acceptable criteria specifications

Autosampler & Sample Introduction	**PASSED**
Analyzer	**PASSED**
Gas Liquid Separator & Dryer	**PASSED**
CVFS Detector	**PASSED**
Electronics/Mechanical	**PASSED**
Data station/PC	**PASSED**
Analytical test	**PASSED**

Provided by

Scientist Instrument Co.,Ltd.
113 Soi Ekachai 44, Ekachai Road
Khlong Bang Phran, Bangbon
Bangkok 10150 Thailand

Certified by .....

Thunraphol Sakdayos

Service Engineer